

ภาคผนวก ง.

ใบรับรองสอบเทียบเครื่องมือ

ANALYTICAL BALANCE (DU)

Model : XS205DU

Serial No. : B344940005



Certificate No. : 25-205716
Sample Code : 25-90375-006

CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapibarn 8 Rd, Nongkham,
Siracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.
(Analytical Balance Room)

Equipment : ELECTRONIC BALANCE

Manufacturer : METTLER TOLEDO

Model : XS205DU

Serial No. : B344940005

ID No. : LABE 05/3

Date of Receipt : 26 November 2025

Date of Calibration : 26 November 2025

Calibrated by Mr. Thanadol Pholthep
Scientist


Approved by (Mr. Somchai Neampunt)
Signed for Director

Issue date 28 November 2025

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).



Certificate No. : 25-205716
Sample Code : 25-90375-006

REPORT OF CALIBRATION

Equipment : ELECTRONIC BALANCE
Manufacturer : METTLER TOLEDO
Model : XS205DU
Capacity : Max 81 g / 200 g
Resolution : 0.00001 g / 0.0001 g
Serial No. : B344940005
ID No. : LABE 05/3

Result of Calibration

1. Test weight and repeatability of reading

Repeatability is a measure of the ability of a balance to supply the same result in repetitive weighings with one and the same load under the same measurement condition. The measurement of the repeatability must include both the balance specifications and the ambient (vibration, fluctuating air current/temperature/humidity, etc.) Operator handling of the balance is also included in the standard deviation.

Unit : g	Range : 81	☐ Before adjustment	☐ After adjustment
	Nominal value	40	80
☒ No adjustment	Standard weight	40.000087	80.000088
☐ Adjustment	Average reading of indicator	40.00004	80.00004
	Standard deviation	0.000007	0.000007

Unit : g	Range : 200	☐ Before adjustment	☐ After adjustment
	Nominal value	100	200
☒ No adjustment	Standard weight	99.999988	200.000015
☐ Adjustment	Average reading of indicator	99.9999	199.9997
	Standard deviation	0.00005	0.00005



Certificate No. : 25-205716
Sample Code : 25-90375-006

REPORT OF CALIBRATION

Result of Calibration

2. Sensitivity or value of a scale division

Change in the output variable of a measuring instrument divided by the associated change in the input variable

Unit : g

Test Point	Sensitivity, S	Test Point	Sensitivity, S
0	1.00000	0	1.0000
40	1.00000	100	1.0000
80	1.00000	200	1.0000

3. Departure of indication from nominal value, Linearity

Unit : g

Nominal Value	Standard Value	Average Reading of Indicator	Correction Value	Expanded Uncertainty	Coverage Factor (k)
Unload	0.0000000	0.00000	0.00000	0.000011	2.04
0.01	0.0100016	0.01000	0.00000	0.000011	2.04
0.1	0.1000056	0.10000	0.00001	0.000012	2.02
1	1.0000110	1.00000	0.00001	0.000015	2.01
5	4.9999996	4.99998	0.00002	0.000020	2.00
10	9.9999994	9.99999	0.00000	0.000026	2.00
20	20.0000042	20.00000	0.00004	0.000037	2.00
50	50.0000052	50.00003	0.00002	0.000067	2.00
100	99.9999988	100.00000	0.00000	0.00016	2.00
150	150.0000040	150.00001	-0.00001	0.00022	2.00
200	200.0000015	200.00001	-0.00001	0.00027	2.00

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.



Certificate No. : 25-205716
Sample Code : 25-90375-006


REPORT OF CALIBRATION

Result of Calibration :

4. Eccentric or off centre loading

Deviation of the measurement value through off - center (eccentric) loading. The corner load increases with the weight of the load and its removal from the center of the pan support.

Weighing pan	☐ Triangular ☒ Rectangular ☐ Circle	Test weight : 50 and 100 Unit : g
Range	81	200
Position	Reading of indicator	Reading of indicator
1	50.00000	100.0000
2	49.99997	100.0000
3	49.99993	99.9999
4	49.99999	100.0000
5	50.00003	99.9999
6	50.00000	100.0000
Maximum difference	0.00007	0.0001

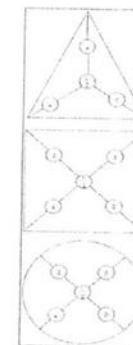

Condition of Calibration

1. Calibration Method : WI-CL-004 base on UKAS LAB 14: 2019
2. This result of calibration was found accurate as shown on date and place of calibration only
3. Condition of Calibration item: Normal
4. This certification is traceable to the International System of Unit maintained at :
Through the reference standard laboratory of Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (Instrument number 1)
5. Reference standard instrument :

Ambient conditions	Min	Max
Temperature (°C)	22.9	24.3
Relative Humidity (%RH)	45.4	47.7
Air pressure (hPa)	1007.2	1011.0

Instrument	Class	ID No	Certificate No.	Due Date
1) STANDARD WEIGHT 1 mg to 1 kg	E2	LB-WE 78	25-1340/4	18 July 2026

End of Report

ANALYTICAL BALANCE

Model : MS204TS/00

Serial No. : B904136539

NSC-TISI-TIS17025
CALIBRATION 0152

Page 1 of 4

Certificate No. : 25-205714
Sample Code : 25-90375-004

CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapibarn 8 Rd, Nongkham,
Sriracha, Chonburi 20230Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.
(Analytical Balance Room)

Equipment : ELECTRONIC BALANCE

Manufacturer : METTLER TOLEDO

Model : MS204TS/00

Serial No. : B904136539

ID No. : LABE 05/4

Date of Receipt : 26 November 2025

Date of Calibration : 26 November 2025


Calibrated by Mr. Pisek Into
ScientistApproved by (Mr. Somchai Neampunt)
Signed for Director

Issue date 28 November 2025

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC)

NSC-TISI-TIS17025
CALIBRATION 0152

Page 2 of 4

Certificate No. : 25-205714
Sample Code : 25-90375-004

REPORT OF CALIBRATION

Equipment : ELECTRONIC BALANCE
Manufacturer : METTLER TOLEDO
Model : MS204TS/00
Capacity : Max 220 g
Resolution : 0.0001 g
Serial No. : B904136539
ID No. : LABE 05/4

Result of Calibration

1. Test weight and repeatability of reading

Repeatability is a measure of the ability of a balance to supply the same result in repetitive weighings with one and the same load under the same measurement condition. The measurement of the repeatability must include both the balance specifications and the ambient (vibration, fluctuating air current/temperature/humidity, etc.) Operator handling of the balance is also included in the standard deviation.

Unit : g	Range : 220	☒ Before adjustment		☒ After adjustment	
	Nominal value	100	200	100	200
☐ No adjustment	Standard weight	100.000045	200.000047	100.000045	200.000047
☒ Adjustment	Average reading of indicator	100.0002	200.0004	100.0000	200.0000
	Standard deviation	0.00005	0.00006	0.00005	0.00005

Unit :	Range :	☐ Before adjustment	☐ After adjustment
	Nominal value		
☐ No adjustment	Standard weight		
☐ Adjustment	Average reading of indicator		
	Standard deviation		

Certificate No. : 25-205714
Sample Code : 25-90375-004

REPORT OF CALIBRATION

Result of Calibration

2. Sensitivity or value of a scale division

Change in the output variable of a measuring instrument divided by the associated change in the input variable.

Unit : g

Range : 220

Range : -

Test Point	Sensitivity, S	Test Point	Sensitivity, S
0	0.8972		
100	0.9969		
200	0.9969		

3. Departure of indication from nominal value, Linearity

Unit : g

Nominal Value	Standard Value	Average Reading of Indicator	Correction Value	Expanded Uncertainty	Coverage Factor (k)
Unload	0.0000000	0.0000	0.0000	0.000094	2.01
0.01	0.0100031	0.0100	0.0000	0.000094	2.01
0.05	0.0500055	0.0500	0.0000	0.000094	2.01
0.1	0.1000023	0.1000	0.0000	0.000094	2.01
1	1.0000136	1.0000	0.0000	0.000095	2.01
5	5.0000210	5.0000	0.0000	0.000096	2.01
10	10.000002	10.0000	0.0000	0.000097	2.01
50	50.000016	50.0000	0.0000	0.00012	2.01
100	100.000045	100.0000	0.0000	0.00016	2.00
150	150.000061	150.0000	0.0001	0.00022	2.00
200	200.000047	200.0000	0.0000	0.00027	2.00

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor, which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

Certificate No. : 25-205714
Sample Code : 25-90375-004

REPORT OF CALIBRATION

Result of Calibration

4. Eccentric or off-centre loading

Deviation of the measurement value through off-center (eccentric) loading. The corner load increases with the weight of the load and its removal from the center of the pan support.

☐ Triangular


☐ Rectangular

☒ Circle

Test weight : 100

Unit : g

Range	Position	Reading of indicator	Reading of indicator
220			
	1	100.0000	
	2	100.0001	
	3	99.9999	
	4	100.0001	
	5	99.9999	
	6	100.0000	
Maximum difference		0.0001	

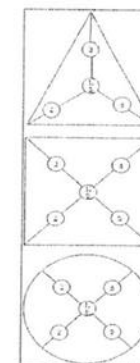

Condition of Calibration

1. Calibration Method : WI CL-004 base on UKAS LAB 14: 2019

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. Condition of Calibration Item: Normal

4. This certification is traceable to the International System of Unit maintained at :

- Through the reference standard laboratory of Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (Instrument number 1).

5. Reference standard instrument :

Instrument	Class	ID No.
1) STANDARD WEIGHT 1 mg to 1 kg	E2	LB-WE-79

Certificate No.	Due Date
25-142885	27 July 2026

End of Report

6. Ambient conditions	Min	Max
Temperature (°C)	23.9	24.6
Relative Humidity (%Rh)	44.9	47.2
Air pressure (hPa)	1008.8	1008.3

COPY

BAROMETER

Serial No. : N/A[S41020124]



CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel: 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com



CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : BAROMETER
MANUFACTURER : BARIO
MODEL / TYPE : N/A
SERIAL NO. : N/A[S41020124]
CLID. NO. : 212500828
JOB CONTROL NO. : 250507051351
CALIBRATION SERVICE : ☒ IN-LABORATORY ☐ ON-SITE

CUSTOMER : EASTERN THAI CONSULTING 1992 CO., LTD.
683 MOO 11, SUKHAPIBARN 8 RD,
NONGKHAM, SRIRACHA, CHONBURI 20230

DATE OF RECEIVED : 07 May 2025

DATE OF ISSUED : 09 May 2025

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sittipong Pimdee
Calibration Engineer

Approved By : Mongkol Yotsoontorn
Authorized Signatory
09 May 2025



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q25051351

F3-011-05/12-23

page 1 of 3

COPY



@clccalibration



CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel: 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com



REPORT OF CALIBRATION

FOR

NOMENCLATURE : BAROMETER
MANUFACTURER : BARIO
MODEL / TYPE : N/A
SERIAL NO. : N/A[S41020124]
DATE OF CALIBRATION : 08 May 2025

ENVIRONMENT CONDITIONS :

Temperature : $(23 \pm 2) ^\circ\text{C}$

Relative Humidity : $(55 \pm 10) \% \text{RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. CLC-CPPP-08 according to DKD-R 6-1 as calibration guidelines.

The calibration was performed by direct measurement with Reference Pressure Monitor which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

Reference Pressure Monitor, Fluke Model RPM3 S/N. 829.

TRACEABILITY :

The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand).
Certificate No. MP-0245-24, Due Date 11 November 2025.

UNCERTAINTY :

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor of $k = 2$. It has been evaluated according to the "Calibration of Pressure Gauges (DKD-R 6-1)" which provides a level of confidence approximately 95%.

Certificate No. Q25051351

F3-011-05/12-23

page 2 of 3

COPY



@clccalibration



CALIBRATION LABORATORY Co., LTD.

210/1114,15 Soi Praset Manuk 29 Yotak 4, Praset Manuk Rd. 1, Lumphini, Bangkok 10230
Tel: 02-576 0334 Fax: 02-576-2072 www.cal-laboratory.com E-mail: ue@cal-laboratory.com



CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The DUC was exercised by applying a known pressure from its zero to full scale 1 times. Then 2 series of known gauge pressure were applied. The STD reading were recorded and the means value were reported in the table below.

CALIBRATION DATA

CORRECTION OF PRESSURE

DUC Test point (hPa)	STD Reading (hPa)		Correction (hPa)	
	Up	Down	Up	Down
990	990.7	990.7	+0.7	+0.7
1000	1000.7	1000.8	+0.7	+0.8
1010	1010.8	1010.8	+0.8	+0.8
1020	1020.8	1020.9	+0.8	+0.9
1030	1030.9	1030.9	+0.9	+0.9

Uncertainty of measurement ± 0.7 hPa

Transmitting fluid : Air.

Note: The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 015 Page 44 of 68

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q25051351

F3-011-05/12-23

COPY



ue@calibration

CERTIFICATE OF ANALYSIS

EPA PROTOCOL GAS

Cylinder No. : EB0145030

CERTIFICATE OF ANALYSIS

Grade of Product: EPA Protocol

Part Number: E03NI99E15AC0U4 Reference Number: 160-402242242-1
Cylinder Number: EB0145030 Cylinder Volume: 144.4 CF
Laboratory: 124 - Plumsteadville - PA Cylinder Pressure: 2015 PSIG
PGVP Number: A12021 Valve Outlet: 350
Gas Code: CH4,PPN,BALN Certification Date: Oct 15, 2021

Expiration Date: Oct 15, 2029

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 000/R-12/031, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted.

Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS					
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
METHANE	180.0 PPM	177.0 PPM	G1	+/- 1.0% NIST Traceable	10/15/2021
PROPANE	185.0 PPM	187.0 PPM	G1	+/- 1.0% NIST Traceable	10/15/2021
NITROGEN	Balance				

CALIBRATION STANDARDS					
Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
NTRM	08011503	K002564	246.7 PPM METHANE/AIR	+/- 0.6%	May 15, 2025
NTRM	200602-06	6162660Y	243.3 PPM PROPANE/AIR	+/- 0.5%	Mar 17, 2027

ANALYTICAL EQUIPMENT		
Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet iS50 FTIR AUP2110295 CH4	FTIR	Oct 13, 2021
Nicolet iS50 FTIR AUP2110295 C3H8	FTIR	Oct 14, 2021

Triad Data Available Upon Request

NOTES:

Gross Weight: 28.0 Kg
Net Weight: 4.9 Kg
PO# 5221004861



Michael A. Markes
Approved for Release



COPY

CERTIFICATE OF ANALYSIS

EPA PROTOCOL GAS

Cylinder No. : EB0178603

CERTIFICATE OF ANALYSIS

Grade of Product: EPA PROTOCOL STANDARD

Customer: BANGKOK INDUSTRIAL
GAS CO LTD
Part Number: E04NI99E15A4385
Cylinder Number: EB0178603
Laboratory: 124 - Plumsteadville - PA
PGVP Number: A12025
Gas Code: CO,NO,NOX,SO2,BALN

Reference Number: 160-403281986-1
Cylinder Volume: 143.7 CF
Cylinder Pressure: 2016 PSIG
Valve Outlet: 660
Certification Date: Mar 17, 2025

Expiration Date: Mar 17, 2033

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results relate only to the items tested. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals

ANALYTICAL RESULTS					
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	50.00 PPM	49.91 PPM	G1	+/- 1.4% NIST Traceable	03/10/2025, 03/17/2025
NITRIC OXIDE	50.00 PPM	49.87 PPM	G1	+/- 1.4% NIST Traceable	03/10/2025, 03/17/2025
SULFUR DIOXIDE	50.00 PPM	50.11 PPM	G1	+/- 0.7% NIST Traceable	03/10/2025, 03/17/2025
CARBON MONOXIDE	3000 PPM	2963 PPM	G1	+/- 0.6% NIST Traceable	03/11/2025
NITROGEN	Balance				

CALIBRATION STANDARDS					
Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
GMIS	402531833-1	CC463968	52.13 PPM NITRIC OXIDE/NITROGEN	+/- 1.0%	Dec 05, 2030
NTRM	210607-21	CC708065	48.41 PPM NITRIC OXIDE/NITROGEN	+/- 1.2%	Sep 21, 2025
GMIS	DCCK1201202242	CC750410	49.10 PPM NITRIC OXIDE/NITROGEN	+/- 0.5%	May 03, 2026
PRM	12404	APEX 1324257	50.04 PPM NITRIC OXIDE/NITROGEN	+/- 0.4%	Dec 22, 2023
GMIS	124206889126	CC323202	4.367 PPM NITROGEN DIOXIDE/NITROGEN	+/- 2.0%	Jan 04, 2027
PRM	C2392001.1	D153445	9.87 PPM NITROGEN DIOXIDE/NITROGEN	+/- 2.0%	Nov 22, 2024
GMIS	15310042024202	CC502382	9.897 PPM NITROGEN DIOXIDE/AIR	+/- 2.1%	Sep 18, 2027
SRM	1693a	FF25467	50.33 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.7%	Jun 27, 2023
GMIS	0712202304	CC265390	49.93 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.7%	Jun 18, 2027
GMIS	0712202327	EB0141202	49.93 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.7%	Jun 12, 2027
CO	220608	CC744768	2501.8 PPM CARBON MONOXIDE/NITROGEN	+/- 0.5%	Sep 30, 2028

The SRM, NTRM, PRM, or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis

ANALYTICAL EQUIPMENT		
Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
MKS FTIR 017675074	FTIR	Mar 04, 2025
Nicolet iS50 FTIR AUP2010245 NO	FTIR	Mar 06, 2025
Nicolet iS50 FTIR AUP2010245 NO2	FTIR	Feb 20, 2025
Nicolet iS50 FTIR AUP2010245 SO2	FTIR	Mar 13, 2025

Triad Data Available Upon Request

NOTES: Gross Weight 27.9 Kg
Net Weight 4.8 Kg
PO# 4225000779



Michael A. Auler
Approved for Release



COPY

Michael A. Auler
Approved for Release



COPY

DRY GAS METER XC-572-V

Serial No. : A2007510

Certificate Of Calibration

Method 5 Pre-Test Console Calibration - Cubic meter (m3)

Meter Console Information

Console Model : XC-572-V
 Console Serial : A2007510
 DGM Model #: SK25EX
 DGM Serial #: 00010219

Calibration Condition

Cal. Date: 24-Sep-25
 Due Date: 24-Sep-26
 Cal. Report No.: WDS-SV6809001
 Ambient Temp (°C): 25
 Pressure (mm Hg): 758
 Relative Humidity (%): 60

Factors/Conversion

Std. Temp. (°K): 298
 Std. Pressure (mm Hg): 760
 K₁ (K/mm Hg): 0.3857

Reference Equipment

WTM Model: W-NKoDa-5B WTM Cal. Due Date: Dec. 2026
 WTM Serial: 600245 Gamma: 1.0000

UUT Meter (DGM)

Reference Meter (WTM)

Run Time (minutes)	DGM Orifice (mm H ₂ O)	Volume		Outlet Temp		Volume		Outlet Temp	
		Initial	Final	Initial	Final	Initial	Final	Initial	Final
θ	P _{m(g)}	V _{int}	V _{ext}	T _{int}	T _{ext}	V _{int}	V _{ext}	T _{int}	T _{ext}
15.00	13.0	0.2808	0.4541	31	31	134.96748	135.13508	25	25
10.00	25.0	0.4844	0.6485	31	31	135.16304	135.32127	25	26
8.00	50.0	0.6702	0.8561	32	32	135.34120	135.52029	26	26
7.00	80.0	0.8899	1.0948	32	32	135.55153	135.74909	26	26
5.00	120.0	1.1160	1.2917	32	32	135.76810	135.93872	26	26

Standardized Data

Calibration Results

Test Meter		Reference Meter		Correction Factor		Flow Rate		ΔH@ (mm H ₂ O)	
Std. Volume	Std. Flow Rate	Std. Volume	Std. Flow Rate	"Gamma"	Variation	Std & Corr	0.0212 SCMM	Variation	
V _{m(std)} (m ³)	Q _{m(std)} m ³ /min	V _{w(std)} (m ³)	Q _{w(std)} m ³ /min	(Y)	(ΔY)	Q _{m(std/corr)}	ΔH _o	ΔΔH _o	
0.167	0.011	0.164	0.011	0.985	0.006	0.011	47.078	0.689	
0.158	0.016	0.155	0.015	0.980	0.000	0.015	45.402	-0.988	
0.179	0.022	0.175	0.022	0.978	-0.002	0.022	45.587	-0.803	
0.198	0.028	0.193	0.028	0.976	-0.004	0.028	46.157	-0.233	
0.170	0.034	0.167	0.033	0.979	0.000	0.033	47.725	1.335	
				0.980	= Y Avg.		46.390	= ΔH@ Avg.	

Pass/Fail Result: **Pass**

Note: For Calibration Factor Y, the ratio of the reading of the calibration meter to the dry gas meter, acceptable tolerance of individual values from the average is ±0.02

Note: For ΔH_o, orifice pressure differential that equates to 0.73cfm (0.0212m³/min) at standard temperature and pressure, acceptable tolerance of individual values from the average is ±0.2inches (5.1mm) H₂O

Approved By:

(Patpasu Chaisana)
 Service Manager

WISDOM
SCIENCE

Date: 24-Sep-25

COPY

Certificate of Calibration - Supplemental

METHOD 6 PRE-TEST CONSOLE CALIBRATION

Nomenclature

Equations

Calibration Train

P_o - Barometric Pressure
 DGM - Dry Gas Meter
 K₁ - Constant based on standard temp and press
 θ - Run time, in minutes
 P_m - ΔH (Meter Pressure, gauge)
 V_m - Volume collected by test meter, corrected for STP
 Q_{m(std)} - Calculated flow rate of test meter
 K' - Critical orifice coefficient
 P_w - Measured pressure of reference meter
 T_w - Temperature measured in reference meter
 T_m - Temperature measured in test meter
 Y - Ratio of volume collected from test meter and orifice
 sc - Scaling Factor
 Counts_{std} - Number of pulse counts, standardized
 Counts_{total} - Number of raw pulse counts of a calibration run

$$V_{w(std)} = Y * K_1 \frac{V_w * (P_{bar} + \frac{P_m(g)}{13.6})}{T_w}$$


$$V_{m(std)} = Counts_{std} * Y_{sc(avg)}$$

$$Counts_{std} = K_1 \frac{C_{total} * (P_{bar} + \frac{P_m}{13.6})}{T_m}$$

$$Q_{w(std)} = \frac{V_{w(std)}}{\theta} \quad Y_{sc} = \frac{V_{w(std)}}{Counts_{std}}$$


$$K_1 = \frac{T_{std}}{P_{std}} \quad Y = \frac{V_{w(std)}}{V_{m(std)}}$$

$$Metric \Delta H_o = \frac{P_{std} * 0.0011696 * (P_{bar} + \frac{P_m}{13.6})}{T_m} * \left(\frac{T_w - \theta}{T_w - P_{std}} \right)^2$$

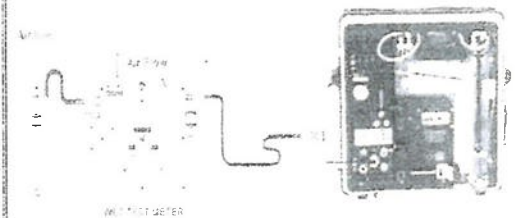


Calibration Graphs

Meter Pressure vs Flowrate

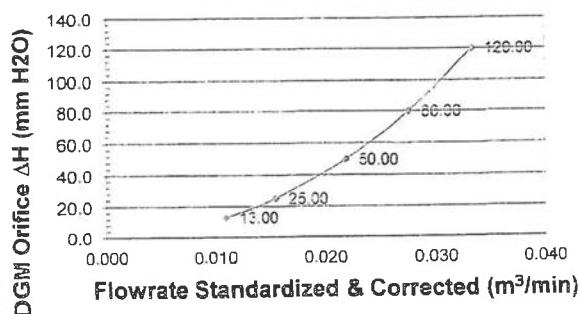

Meter Gamma vs Flowrate

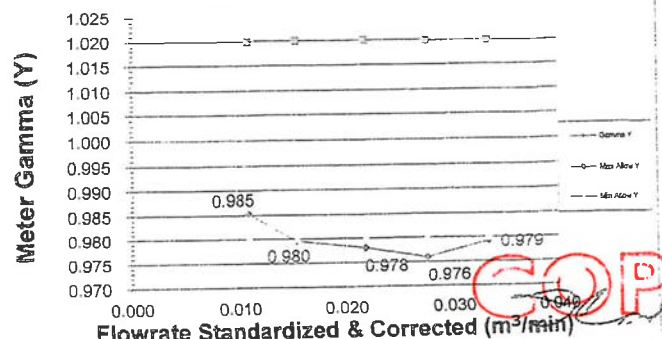

TEMPERATURE DISPLAY CALIBRATION

Meter Console Information

Console Model :	XC-S72-V
Console Serial :	A2007510
Temp. Indicator Model :	755-KF
Temp. Indicator Serial :	JC17852

Calibration Conditions

Cal. Date :	24-Sep-25
Due Date :	24-Sep-26
Cal. Report No. :	WDS-SV809001
Ambient Temp. (°C) :	25
Pressure (mm Hg) :	758
Humidity (%) :	60

Reference Equipment

Temp. Meter Model :	Fluke 714B
Serial No. :	80590035
Cal. Date :	07-Apr-25
Temp. Meter Model :	Fluke 179
Serial No. :	58620112
Cal. Date :	06-Feb-25

Temperature Sensor Calibration

Reference Point	Ref. Thermometer Temperature	Thermocouple Display Temperature	Temperature Difference
#	°C	°C	°C
1	-18.0	-18.0	0.0
2	38.0	38.0	0.0
3	93.0	93.0	0.0
4	149.0	149.0	0.0
5	260.0	260.0	0.0
6	371.0	372.0	-1.0
7	482.0	483.0	-1.0
8	593.0	594.0	-1.0
9	816.0	817.0	-1.0
10	1038.0	1039.0	-1.0
Maximum *			1.0

PASS

Note

* For valid test results, the maximum difference between temperature readings should $\leq 1.0^{\circ}\text{C}$ (EPA Method 5, Section 6.1.1.8).
Perform all TC Channel calibrations. Except meter (DGM) channel

DGM Out Temperature Sensor Calibration

Temperature point	Ref. Thermometer Temperature	Thermocouple Display Temperature	Temperature Difference
#	°C	°C	°C
Ice	0.0	0.0	0.0
Ambient	26.5	27.0	-0.5
Heat	114.3	115.0	-0.7

Difference Range

Temp. Difference $\pm 2^{\circ}\text{F}$ or $\pm 1.1^{\circ}\text{C}$

PASS

Note

The temperatures of the thermocouple and reference thermometers shall agree to within $\pm 2^{\circ}\text{F}$. (EPA Method 5, section 10.5)

Approved By :

[Signature]

(Patpasu Chaisana)

Service Manager

WISDOM
SCIENCE

WISDOM SCIENCE SALE AND SERVICE GROUP COMPANY LIMITED
Address: 9/115 Lumpini Town Villa Ratchaphruek-Pinkao Village, No. 4, Bang Khanun, Bang Kruai, Nonthaburi 11130 Thailand
Tel: 02-120-1122

COPY

DRY GAS METER MC-572

Serial No. : 0011024



WISDOM SCIENCE

Certificate Of Calibration

Method 5 Pre-Test Console Calibration - Cubic meter (m3)

Meter Console Information

Console Model : MC-572
 Console Serial : 0011024
 DGM Model #: SK25EX
 DGM Serial #: 00005437

Calibration Condition

Cal. Date: 25-Jan-26
 Due Date: 25-Jan-27
 Cal. Report No.: WDS-SV6901003
 Ambient Temp (°C): 25
 Pressure (mm Hg): 758
 Relative Humidity (%): 60

Factors/Conversion

Std. Temp. (°K): 298
 Std. Pressure (mm Hg): 760
 K₁ (K/mm Hg): 0.3857

Reference Equipment

WTM Model: W-NKoDa-5B WTM Cal. Due Date: Jan. 2027
 WTM Serial: 600245 Gamma: 1.0000

UUT Meter (DGM)						Reference Meter (WTM)			
Run Time (minutes)	DGM Orifice (mm H ₂ O)	Volume		Outlet Temp		Volume		Outlet Temp	
		Initial	Final	Initial	Final	Initial	Final	Initial	Final
15.00	13.0	1325.8454	1326.0209	24	24	150.37336	150.55701	27	27
10.00	25.0	1326.0448	1326.2062	24	25	150.58598	150.75296	27	27
8.00	50.0	1326.2250	1326.4054	25	25	150.77379	150.95979	27	27
7.00	80.0	1326.4286	1326.6286	26	26	150.98358	151.18895	27	27
5.00	120.0	1326.6411	1326.8148	26	26	151.20211	151.38001	27	27

Standardized Data				Calibration Results				
Test Meter		Reference Meter		Correction Factor		Flow Rate	ΔH@ (mm H ₂ O)	
Std. Volume	Std. Flow Rate	Std. Volume	Std. Flow Rate	"Gamma"	Variation	Std & Corr	0.0212 SCMM	Variation
V _{m(std)} (m ³)	Q _{m(std)} m ³ /min	V _{r(std)} (m ³)	Q _{r(std)} m ³ /min	(Y)	(ΔY)	Q _{m(std/corr)}	ΔH _g	ΔΔH _g
0.173	0.012	0.179	0.012	1.035	0.014	0.012	40.673	-2.374
0.159	0.016	0.163	0.016	1.023	0.003	0.016	42.078	-0.969
0.178	0.022	0.181	0.023	1.019	-0.001	0.023	43.545	0.498
0.197	0.028	0.200	0.029	1.016	-0.005	0.029	43.861	0.814
0.172	0.034	0.173	0.035	1.009	-0.011	0.035	45.079	2.032
				1.020	= Y Avg.		43.047	= ΔH _g Avg.

Pass/Fail Result: Pass

Note: For Calibration Factor Y, the ratio of the reading of the calibration meter to the dry gas meter, acceptable tolerance of individual values from the average is ±0.02.

Note: For ΔH_g, orifice pressure differential that equates to 0.75cfm (0.0212m³/min) at standard temperature and pressure, acceptable tolerance of individual values from the average is ±0.2inches (5.1mm) H₂O.

Approved By:
 (Patpasu Chaisana)
 Service Manager

Date: 25-Jan-26

COPY

Certificate of Calibration - Supplemental

METHOD 5 PRE-TEST CONSOLE CALIBRATION

Nomenclature

P_b - Barometric Pressure
 DGM - Dry Gas Meter
 K₁ - Constant based on standard temp and press
 θ - Run time, in minutes
 P_m - ΔH (Meter Pressure, gauge)
 V_m - Volume collected by test meter, corrected for STP
 Q_{m(std)} - Calculated flow rate of test meter
 K' - Critical orifice coefficient
 P_m - Measured pressure of reference meter
 T_r - Temperature measured in reference meter
 T_m - Temperature measured in test meter
 Y - Ratio of volume collected from test meter and orifice
 SC - Scaling Factor
 Counts_{std} - Number of pulse counts, standardized
 Counts_{total} - Number of raw pulse counts of a calibration run

Equations

$$V_{u(std)} = Y * K_1 \frac{V_w * (P_{bar} + \frac{P_{m(std)}}{13.6})}{T_u}$$

$$V_{m(std)} = Counts_{std} * Y_{sc(avg)}$$

$$Counts_{std} = K_1 \frac{C_{total} * (P_{bar} + \frac{P_{m(std)}}{13.6})}{T_m}$$


$$Q_{u(std)} = \frac{V_{u(std)}}{\theta}$$

$$Y = \frac{V_{u(std)}}{V_{m(std)}}$$


$$K_1 = \frac{T_{std}}{P_{std}}$$

$$Metric: \Delta H_g = \frac{P_{m(std)} * 0.0011596 * (P_{bar} + \frac{P_{m(std)}}{13.6})}{T_m} * \left(\frac{T_w * \theta}{V_u * P_{bar}} \right)^2$$

Calibration Train

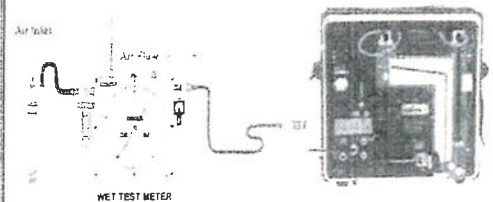


Calibration Graphs

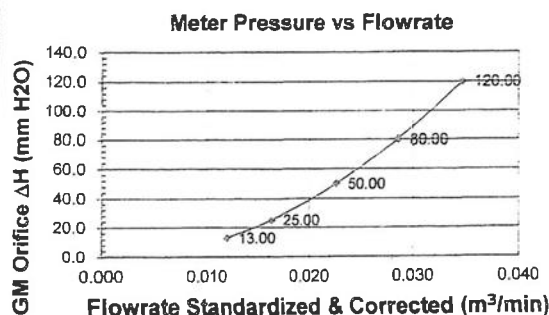

Console Serial: 0011024

Console Model: MC-572

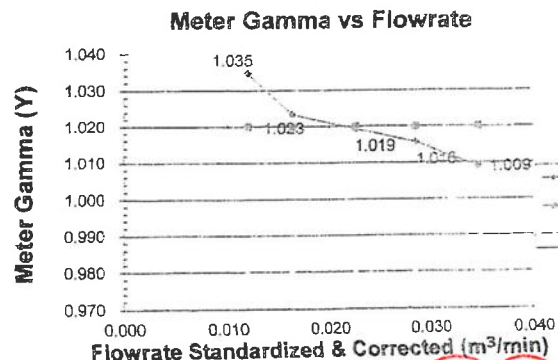

Console Serial: 0011024

Console Model: MC-572

COPY

TEMPERATURE DISPLAY CALIBRATION

Meter Console Information

Console Model : MC-572
 Console Serial : 0011024
 Temp Indicator Model : 785-KF
 Temp Indicator Serial : JC02982

Calibration Conditions

Cal. Date : 25-Jan-26
 Due Date : 25-Jan-27
 Cal. Report No. : WDS-SV8901003
 Ambient Temp. (°C) : 25
 Pressure (mm Hg) : 758
 Humidity (%) : 60

Reference Equipment

Temp. Meter Model : Fluke 714B
 Serial No. : 80590035
 Cal. Date : 07-Apr-25
 Temp Meter Model : Fluke 179
 Serial No. : 58620112
 Cal. Date : 06-Feb-25

Temperature Sensor Calibration

Reference Point	Ref. Thermometer Temperature	Thermocouple Display Temperature	Temperature Difference
#	°C	°C	°C
1	-18.0	-17.0	1.0
2	38.0	38.0	0.0
3	93.0	93.0	0.0
4	149.0	150.0	-1.0
5	261.0	260.0	1.0
6	371.0	372.0	-1.0
7	482.0	483.0	-1.0
8	584.0	584.0	0.0
9	815.0	815.0	0.0
10	1038.0	1038.0	1.0
Maximum ¹			1.0

PASS

Note

¹ For valid test results, the maximum difference between temperature readings should $\leq 1.0^{\circ}\text{C}$ (EPA Method 5, Section 6.1.1.8). Perform all TC Channel calibrations. Except meter (DGM) channel

DGM Out Temperature Sensor Calibration

Temperature point	Ref. Thermometer Temperature	Thermocouple Display Temperature	Temperature Difference
#	°C	°C	°C
Ice	0.0	0.0	0.0
Ambient	29.4	30.0	-0.6
Heat	113.2	114.0	-0.8

Difference Rang

Temp. Difference $\pm 2^{\circ}\text{F}$ or $\pm 1.1^{\circ}\text{C}$

PASS

Note

The temperatures of the thermocouple and reference thermometers shall agree to within $\pm 2^{\circ}\text{F}$. (EPA Method 5, section 10.5)

Approved By :


 (Palpasu Chalsana)
 Service Manager

**WISDOM
SCIENCE**

COPY

DRY GAS METER MC-572

Serial No. : 0504003

Certificate Of Calibration

Method 5 Pre-Test Console Calibration - Cubic meter (m3)

Meter Console Information

Console Model : MC-572
Console Serial : 0504003
DGM Model #: G2.5
DGM Serial #: 202205100796

Calibration Condition

Cal. Date : 09-Mar-26
Due Date : 08-Mar-27
Cal. Report No. : WDS-SV6902009
Ambient Temp (°C): 25
Pressure (mm Hg): 758
Relative Humidity (%): 80

Factors/Conversion

Std. Temp. (°K) : 298
Std. Pressure (mm Hg): 760
K₁ (K/mm Hg): 0.3857

Reference Equipment

WTM Model: W-NKoDa-5B WTM Cal. Due Date: Jan. 2027
WTM Serial: 600245 Gamma: 1.0000

Run Time (minutes)	DGM Orifice (mm H ₂ O)	Volume		Outlet Temp		Volume		Outlet Temp	
		Initial	Final	Initial	Final	Initial	Final	Initial	Final
15.00	13.0	1.8494	2.0072	27	27	161.94235	162.09910	30	30
10.00	25.0	2.0275	2.1830	28	28	162.11834	162.27201	30	30
8.00	50.0	2.3704	2.5530	28	28	162.45057	162.63178	30	30
7.00	80.0	2.5916	2.7969	28	28	162.66630	162.87039	30	30
5.00	120.0	2.8238	3.0039	28	29	162.89345	163.07313	30	30

Standardized Data				Calibration Results			
Test Meter		Reference Meter		Correction Factor		Flow Rate	
Std. Volume	Std. Flow Rate	Std. Volume	Std. Flow Rate	"Gamma"	Variation	Std & Corr	ΔH@ (mm H ₂ O)
V _{test} (m ³)	Q _{test} m ³ /min	V _{ref} (m ³)	Q _{ref} m ³ /min	(Y)	(ΔY)	Q _{test} (corr)	ΔH _g
0.154	0.010	0.151	0.010	0.982	0.001	0.010	56.383
0.151	0.015	0.148	0.015	0.979	-0.002	0.015	50.092
0.178	0.022	0.175	0.022	0.981	0.000	0.022	46.333
0.201	0.029	0.197	0.028	0.980	-0.001	0.028	45.005
0.176	0.035	0.173	0.035	0.983	0.002	0.035	44.631
				0.981	= Y Avg.		48.489 = ΔH _g Avg.

Pass/Fail Result: **Pass**

Note: For Calibration Factor Y, the ratio of the reading of the calibration meter to the dry gas meter, acceptable tolerance of individual values from the average is ±0.02.

Note: For ΔH_g, orifice pressure differential that equates to 0.75cfm (0.0212m³/min) at standard temperature and pressure, acceptable tolerance of individual values from the average is ±0.2inches (5.1mm) H₂O.

Approved By: 
(Patpasu Chaisana)
Service Manager


WISDOM
SCIENCE
Wisdom Science Calibration and Instrumentation
We provide the best calibration and repair services for your equipment.

Date: 09-Mar-26


COPY

Certificate of Calibration - Supplemental

METHOD 5 PRE-TEST CONSOLE CALIBRATION

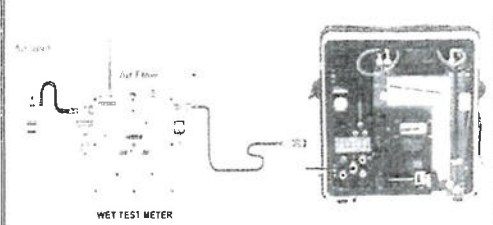Nonomenclature	Equations	Calibration Train
P_b - Barometric Pressure DGM - Dry Gas Meter K₁ - Constant based on standard temp and press θ - Run time, in minutes P_m - ΔH (Meter Pressure, gauge) V_m - Volume collected by test meter, corrected for STP Q_{m(sc)} - Calculated flow rate of test meter K' - Critical orifice coefficient P_w - Measured pressure of reference meter T_w - Temperature measured in reference meter T_m - Temperature measured in test meter Y - Ratio of volume collected from test meter and orifice sc - Scaling Factor Counts_{std} - Number of pulse counts, standardized C_{total} - Number of raw pulse counts of a calibration run	$V_{m(std)} = Y * K_1 \frac{V_w * (P_{bar} + \frac{P_{outlet}}{13.6})}{T_w}$ $V_{m(std)} = Counts_{std} * Y_{sc(avg)}$ $Counts_{std} = K_1 \frac{(Counts_{sc} * V_w - \frac{P}{13.6})}{T_w}$ $Q_{k(std)} = \frac{V_{m(std)}}{\theta}$ $K_1 = \frac{T_{sc}}{P_{sc}}$ $Y = \frac{V_{m(std)}}{V_{w(std)}}$ $Metric \Delta H_g = \frac{P_{sc} - (13.6 * (10 * K_1 * P_{sc} + \frac{P_{sc}}{13.6}))}{T_{sc}} * (\frac{T_w * \theta}{V_w * P_{bar}})^2$	 WET TEST METER

Calibration Graphs

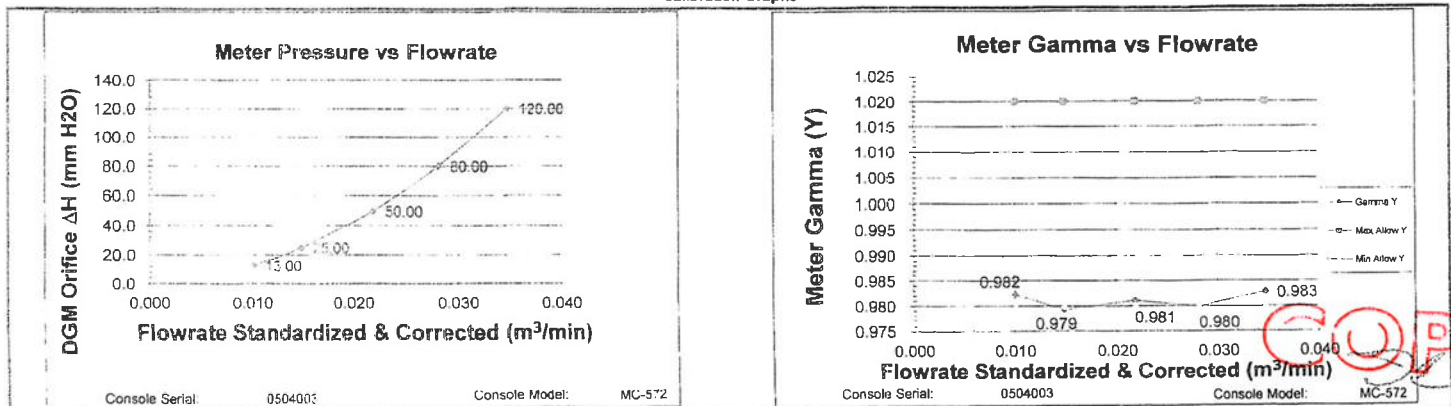

Meter Console Information

Console Model : MC-572
Console Serial : 0504003
Temp. Indicator Model : 765-KF
Temp. Indicator Serial : JC05830

Calibration Conditions

Cal. Date : 09-Mar-26
Due Date : 09-Mar-27
Cal. Report No. : WDS-SV8902009
Ambient Temp. (°C) : 25
Pressure (mm Hg) : 759
Humidity (%) : 60

Reference Equipment

Temp. Meter Model : Fluke 714B
Serial No. : 60590035
Cal. Date : 07-Apr-25
Temp. Meter Model : Fluke 179
Serial No. : 59620112
Cal. Date : 06-Feb-26

Temperature Sensor Calibration

Reference Point	Ref. Thermometer Temperature	Thermocouple Display Temperature	Temperature Difference
#	°C	°C	°C
1	-18.0	-17.0	1.0
2	38.0	38.0	0.0
3	93.0	93.0	0.0
4	149.0	149.0	0.0
5	281.0	280.0	1.0
6	371.0	372.0	-1.0
7	482.0	483.0	-1.0
8	594.0	595.0	-1.0
9	815.0	816.0	-1.0
10	1039.0	1038.0	1.0
Maximum ¹			1.0

PASS

Note

¹ For valid test results, the maximum difference between temperature readings should $\leq 1.0^{\circ}\text{C}$ (EPA Method 5, Section 6.1.1.8). Perform all TC Channel calibrations. Except meter (DGM) channel

DGM Out Temperature Sensor Calibration

Temperature point	Ref Thermometer Temperature	Thermocouple Display Temperature	Temperature Difference
#	°C	°C	°C
Ice	0.0	0.0	0.0
Ambient	29.6	30.0	-0.4
Heat	112.7	113.0	-0.3

Difference Rang

Temp. Difference $\pm 2^{\circ}\text{F}$ or $\pm 1.1^{\circ}\text{C}$

PASS

Note

The temperatures of the thermocouple and reference thermometers shall agree to within $\pm 2^{\circ}\text{F}$. (EPA Method 5, section 10.5)

Approved By :

(Patpasu Chaisana)

Service Manager

WISDOM
SCIENCE

บริษัท วิสโดม ไซน์แอนด์เซอร์วิส กรุ๊ป จำกัด
WISDOM SCIENCE SALE AND SERVICE GROUP COMPANY LIMITED

Flue gas Analyzer

Testo 350

Serial No. 63455658/0722

Certificate No: G 250296
Date of issue : 04-Nov-25

Instrument description : Flue Gas Analyzer
Instrument model : Testo 350
Instrument serial no. : 63455658/0722
Control unit serial no. : 03601409/0722
ID no. or control no. :
Manufacturer : Testo SE & Co. KGaA
Probe description : -
Probe model : -
Probe serial no. : -
Customer name : Eastern Thai Consulting 1992 Company Limited
Customer address : 683 Moo 11, Sukhapibarn 8 Road, Nongkham, Si Racha, Chon Buri 20280

Total pages of certificate : 2 Pages
Receiving no. : L-253802
Receiving date. : 03-Nov-25
Parameter of calibration : Gas Calibration(Oxygen 2.506, 9.984, 21.01 %vol, Carbon Monoxide 80.38, 300.9, 1001 ppm, Nitrogen Dioxide 30.68, 81.8, 202.3 ppm, Nitric Oxide 30.0, 151.8, 322 ppm, Sulphur Dioxide 50.4, 100.7, 605.9 ppm)

Condition of UUC. : Used

Ambient condition : All of the Measurement were carried out in the stabilized laboratory
Temperature : 23 ± 5 °C
Humidity : 55 ± 15 %RH

Calibration place : 17/121 Soi Ngamwongwan 47 Yaek 48, Toongsonghong, Lakki, Bangkok 10210

Calibration procedure no : This instrument was calibrated by comparison with Standard gas mixture according to calibration Work Instruction no. WI-CL-28-C

The calibration certificate expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

This certificate is applied only to item under test Environmental condition.

This Calibration Certificate may not be reproduced other than in full except with the permission of the issuing laboratory.

Calibration certificates without signature and seal not valid and The results relate only to the items tested/calibrated.

This calibration certificate documents are traceability to national standards, which realize measurement according to the International System of Units (SI).

Date of calibration : 04-Nov-25

Mr. Kwanchai Khamdoun
Calibration Technician

Mrs. Nongluck Wongsettee
Technical Manager

COPY

Certificate No.: G 250296

Standard References (Table 1)

Standard	Certificate No.	Vendor	Due date
Oxygen (O2) 2.506 % Vol	1287/25	Linde	08-May-29
Oxygen (O2) 9.984 % Vol	CG-0090-25	Nimt	24-Jun-30
Oxygen (O2) 21.01 % Vol	CG-0112-24	Nimt	01-Aug-29
Carbon monoxide (CO) 80.38 ppm	CG-0105-25	Nimt	04-Aug-30
Carbon monoxide (CO) 300.9 ppm	1422/25	Linde	21-May-29
Carbon monoxide (CO) 1001 ppm	CG-0085-24	Nimt	22-May-29
Nitrogen Dioxide (NO2) 30.68 ppm	2832/24	Linde	08-Sep-26
Nitrogen Dioxide (NO2) 81.8 ppm	2330/24	Linde	01-Aug-26
Nitrogen Dioxide (NO2) 202.3 ppm	2558/25	Linde	02-Sep-27
Nitric Oxide (NO) 30.0 ppm	CG-0065-24	Nimt	06-May-26
Nitric Oxide (NO) 151.8 ppm	0404/25	Linde	09-Feb-27
Nitric Oxide (NO) 322 ppm	1234/25	Linde	04-May-27
Sulphur Dioxide (SO2) 50.4 ppm	1306/25	Linde	12-May-27
Sulphur Dioxide (SO2) 100.7 ppm	2662/24	Linde	25-Aug-26
Sulphur Dioxide (SO2) 605.9 ppm	1229/25	Linde	04-May-27

Measured room conditions

Temperature : 22.6 °C Humidity : 67.7 %RH Pressure : 1011.9 mbar

Calibration conditions

Gas Temperature : 23 °C Flow rate : 1,300 ml/min Gas pressure : 1016.5 mbar

Calibration Results (Without adjustment) (Table 2)

Parameter of Standard	Standard Values	Mean of UUC	Error	Uncertainty (±)
O2 (%Vol)	2.506	2.44	-0.066	0.15
O2 (%Vol)	9.984	10.12	0.136	0.23
O2 (%Vol)	21.01	21.15	0.14	0.30
CO (ppm)	80.38	81	0.62	3.0
CO (ppm)	300.9	303	2.1	6.0
CO (ppm)	1001	1006	5	12
NO2 (ppm)	30.68	29.4	-1.28	8.0
NO2 (ppm)	81.8	79.7	-2.1	8.0
NO2 (ppm)	202.3	199.1	-3.2	12
NO (ppm)	30.0	30	0.0	8.0
NO (ppm)	151.8	151	-0.8	8.0
NO (ppm)	322	323	1	12
SO2 (ppm)	50.4	50	-0.4	6.0
SO2 (ppm)	100.7	102	1.3	6.0
SO2 (ppm)	605.9	610	4.1	13

Remark : 1 cmol/mol = 1 %vol, 1 µmol/mol = 1 ppm., Sensor(CO, NO2)New.

End of Report

COPY

Flue gas Analyzer

Testo 350

Serial No. 63455616/0722

Certificate No.: G 250384

Date of issue : 02-Dec-25

Instrument description : Flue Gas Analyzer
Instrument model : Testo 350
Instrument serial no. : 63455616/0722
Control unit serial no. : 03600177/0722
ID no. or control no. : -
Manufacturer : Testo SE & Co. KGaA
Probe description : -
Probe model : -
Probe serial no. : -
Customer name : Eastern Thai Consulting 1992 Company Limited
Customer address : 683 Moo 11, Sukhapibarn 8 Road, Nongkham, Si Racha, Chon Buri 20280

Total pages of certificate : 2 Pages
Receiving no. : L-254783
Receiving date. : 27-Nov-25
Parameter of calibration : Gas Calibration (Oxygen, Carbon Monoxide, Nitrogen Dioxide, Nitric Oxide, Sulphur Dioxide)

Condition of UUC. : Used
Ambient condition : All of the Measurement were carried out the stabilized laboratory
Temperature : 23 ± 5 °C
Humidity : 55 ± 15 %RH

Calibration place : 17/121 Soi Ngamwongwan 47 Yaek 48, Toongsonghong, Lakso, Bangkok 10210

Calibration procedure no. : This instrument was calibrated by comparison with Standard gas mixture according to calibration Work Instruction no. WI-CL-28-C

The calibration certificate expanded uncertainty of measurement is stated as the standard uncertainty of measurement Multiplied by coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

This certificate is applied only to item under test Environmental condition.

This Calibration Certificate may not be reproduced other than in full except with the permission of the issuing laboratory.

Calibration certificates without signature and seal not valid and The results relate only to the items tested/calibrated.

This calibration certificate documents are traceability to national standards, which realize measurement according to the International System of Units (SI).

Date of calibration : 02-Dec-25

[Signature]

Mr. Kwanchai Khamdoun

Calibration Technician

[Signature]

Mrs. Nongluck Wongsettee

Technical Manager

COPY

Issued Date 26/02/16

Certificate No.: G 250384

Standard References (Table 1)

Standard	Certificate No.	Vendor	Due date
Oxygen (O2) 2.506 % Vol	1287/25	Linde	08-May-29
Oxygen (O2) 9.984 % Vol	CG-0090-25	Nimt	24-Jun-30
Oxygen (O2) 21.01 % Vol	CG-0112-24	Nimt	01-Aug-29
Carbon monoxide (CO) 80.38 ppm	CG-0105-25	Nimt	04-Aug-30
Carbon monoxide (CO) 300.9 ppm	1422/25	Linde	21-May-29
Carbon monoxide (CO) 1000 ppm	3131/25	Linde	27-Oct-29
Nitrogen Dioxide (NO2) 30.68 ppm	2832/24	Linde	08-Sep-26
Nitrogen Dioxide (NO2) 81.8 ppm	2330/24	Linde	01-Aug-26
Nitrogen Dioxide (NO2) 202.3 ppm	2558/25	Linde	02-Sep-27
Nitric Oxide (NO) 30.0 ppm	CG-0065-24	Nimt	06-May-26
Nitric Oxide (NO) 151.8 ppm	0404/25	Linde	09-Feb-27
Nitric Oxide (NO) 322 ppm	1234/25	Linde	04-May-27
Sulphur Dioxide (SO2) 50.4 ppm	1306/25	Linde	12-May-27
Sulphur Dioxide (SO2) 100.7 ppm	2662/24	Linde	25-Aug-26
Sulphur Dioxide (SO2) 605.9 ppm	1229/25	Linde	04-May-27

Measured room conditions

Temperature : 23.3 °C Humidity : 61.9 %RH Pressure : 1010.4 mbar

Calibration conditions

Gas Temperature : 23 °C Flow rate : 1,300 ml/min Gas pressure : 1016.5 mbar

Calibration Results (Without adjustment) (Table 2)

Parameter of Standard	Standard Values	Mean of UUC	Error	Uncertainty (±)
O2 (%Vol)	2.506	2.45	-0.056	0.15
O2 (%Vol)	9.984	10.02	0.036	0.20
O2 (%Vol)	21.01	21.08	0.07	0.30
CO (ppm)	80.38	81	0.62	3.0
CO (ppm)	300.9	300	-0.9	6.0
CO (ppm)	1000	997	-3	12
NO2 (ppm)	30.68	28.7	-1.98	8.0
NO2 (ppm)	81.8	80.2	-1.6	8.0
NO2 (ppm)	202.3	202.8	0.5	12
NO (ppm)	30.0	31	1.0	8.0
NO (ppm)	151.8	154	2.2	8.0
NO (ppm)	322	325	3	12
SO2 (ppm)	50.4	50	-0.4	6.0
SO2 (ppm)	100.7	100	-0.7	6.0
SO2 (ppm)	605.9	605	-0.9	13

Remark : 1 cmol/mol = 1 %vol. 1 μmol/mol = 1 ppm., Sensor(CO, NO2, NO, SO2)New.

End of Certificate of Calibration

COPY

Flue gas Analyzer

Testo 350XL

Serial No. 01859560/006



Certificate No.: G 260016
Date of issue : 12-Jan-26

Instrument description : Flue Gas Analyzer
Instrument model : Testo 350XL
Instrument serial no. : 01859560/006
Control unit serial no. : 01864498/006
ID no. or control no. : -
Manufacturer : Testo SE & Co. KGaA
Probe description : -
Probe model : -
Probe serial no. : -
Customer name : Eastern Thai Consulting 1992 Company Limited
Customer address : 683 Moo 11, Sukhapibarn 8 Road, Nongkham, Si Racha, Chon Buri 20280

Total pages of certificate : 2 Pages
Receiving no. : L-260025
Receiving date. : 30-Dec-25
Parameter of calibration : Gas Calibration(Oxygen, Carbon Monoxide, Nitrogen Dioxide, Nitric Oxide, Sulphur Dioxide)

Condition of UUC. : Used
Ambient condition : All of the Measurment ware caried out the stabilized labotary

Temperature : 23 ±5 °C
Humidity : 55 ± 15 %RH

Calibration place : 17/121 Soi Ngamwongwan 47 Yaek 48, Toongsonghong, Laksi, Bangkok 10210

Calibration procedure no. : This instrument was calibrated by comparison with Standard gas mixture according to calibration Work Instruction no. WI-CL-28-C

The calibration certificate expanded uncertainty of measurement is stated as the standard uncertainty of measurent Multiplied by coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%. This certificate is applied only to item under test Environmental condition. This Calibration Certificate may not be reproduced other than in full except with the permission of the issuing laboratory. Calibration certificates without signature and seal not valid and The results relate only to the items tested/calibrated. This calibration certificate documents are traceability to national standards, which realize measurement according to the International System of Units (SI).

Date of calibration : 09-Jan-26

Kwanchai Khamdoun

Mr. Kwanchai Khamdoun
Calibration Technician

Nongluck Wongsettee

Mrs. Nongluck Wongsettee
Technical Manager

COPY



Certificate No.: G 260016

Standard References (Table 1)

Standard	Certificate No.	Vendor	Due date
Oxygen (O2) 21.01 % Vol	CG-0112-24	Nimt	01 Aug 29
Carbon monoxide (CO) 80.47 ppm	3076/25	Linde	04-Nov-27
Carbon monoxide (CO) 300.9 ppm	1422/25	Linde	21-May-28
Carbon monoxide (CO) 1000 ppm	3131/25	Linde	27 Oct-29
Nitrogen Dioxide (NO2) 30.68 ppm	2832/24	Linde	08-Sep-26
Nitrogen Dioxide (NO2) 61.8 ppm	2230/24	Linde	01 Aug 26
Nitrogen Dioxide (NO2) 202.3 ppm	2558/25	Linde	02-Sep-27
Nitric Oxide (NO) 30.0 ppm	CG-0065-24	Nimt	06-May-26
Nitric Oxide (NO) 151.8 ppm	0404/25	Linde	09-Feb-27
Nitric Oxide (NO) 322 ppm	1234/25	Linde	04-May-27
Sulphur Dioxide (SO2) 50.4 ppm	1306/25	Linde	12-May-27
Sulphur Dioxide (SO2) 100.7 ppm	2662/24	Linde	25 Aug 26
Sulphur Dioxide (SO2) 605.9 ppm	1229/25	Linde	04-May-27

Measured room conditions

Temperature : 21.5 °C Humidity : 57.4 %RH Pressure : 1012.3 mbar

Calibration conditions

Gas Temperature : 23 °C Flow rate : 1,300 ml/min Gas pressure : 1017.5 mbar

Calibration Results (Without adjustment) (Table 2)

Parameter of Standard	Standard Values	Mean of UUC	Error	Uncertainty (±)
O2 (%Vol)	2.506	2.43	-0.076	0.15
O2 (%Vol)	9.984	9.97	-0.014	0.20
O2 (%Vol)	21.01	21.14	0.13	0.30
CO (ppm)	80.47	81	0.53	3.0
CO (ppm)	301	302	1.1	6.0
CO (ppm)	1000	999	-1	12
NO2 (ppm)	30.68	28.7	-1.98	8.0
NO2 (ppm)	81.8	78.3	-3.5	8.0
NO2 (ppm)	202.3	196.2	-6.1	12
NO (ppm)	30.0	31	1.0	8.0
NO (ppm)	151.8	151	-0.8	8.0
NO (ppm)	322	320	-2	12
SO2 (ppm)	50.4	49	-1.4	6.0
SO2 (ppm)	100.7	100	-0.7	6.0
SO2 (ppm)	605.9	602	-3.9	13

Remark : 1 cmol/mol = 1 %vol. 1 μmol/mol = 1 ppm.

End of Certificate of Calibration

COPY

Heat Stress Monitor

Model : Ques Temp 34

Serial No. : TEU080015



Jiranatee Associates Co., Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd Wattthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI TIS 17025
CALIBRATION 0367

Temperature measurement laboratory
Calibration services department.



Continuation of Certificate of Calibration Number CDT-013-69

Page 2 of 2 Pages

Result of Calibration: ☒ Without Adjustment ☐ With Adjustment

Calibration Range: 20 °C to 40 °C

Function:

Table 1: This equipment was connected with wet bulb Temperature probe Model: -, S/N: -.
Dimension: Diameter 4.77 mm. Length 70 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
65	20.052	20.4	0.3	0.099
65	25.042	25.3	0.3	0.099
65	30.033	30.3	0.3	0.099
65	35.020	35.3	0.3	0.14
65	40.011	40.2	0.2	0.099

Table 2: This equipment was connected with Globe Temperature probe Model: -, S/N: -.
Dimension: Diameter 4.77 mm. Length 70 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
65	20.052	20.4	0.3	0.099
65	25.042	25.3	0.3	0.099
65	30.032	30.2	0.2	0.099
65	35.020	35.2	0.2	0.14
65	40.011	40.2	0.2	0.099

Table 3: This equipment was connected with Dry Bulb Temperature probe Model: -, S/N: -.
Dimension: Diameter 4.77 mm. Length 70 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
65	20.052	20.4	0.3	0.099
65	25.042	25.3	0.3	0.099
65	30.032	30.2	0.2	0.099
65	35.020	35.2	0.2	0.14
65	40.011	40.2	0.2	0.14

UUC*: Unit Under Calibration

Remark: The reported uncertainty of measurement is 0.14, based on standard uncertainty multiplied by a coverage factor k=2.14 providing a level of confidence of approximately 95%.

End of Certificate of Calibration

Certificate No. : CDT-013-69

Page 1 of 2 Pages

MEASUREMENT ITEM : Heat Stress Monitor
MANUFACTURER : TSI QUEST
MODEL/TYPE : Ques Temp 34
SERIAL NUMBER : TEU080015
ID NUMBER : NO. 14
CONDITION AS-RECEIVED : Used item
CUSTOMER : Eastern thai consulting 1992 Co.,Ltd.
683 Mao 11, Sukhapibarn 8 Rd,
Nongkham, Sriracha, Chonburi 20230

RECEIVED DATE : 25 Dec 2025
MEASUREMENT DATE : 08 Jan 2026
ISSUE DATE : 08 Jan 2026

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:

The temperature calibration was done by In-House calibration method as WI-CL-001 according to comparison method with standard digital temperature indicator and standard temperature probe. The temperature scale use was based on ITS-90.

Traceability:

The measurement results are traceable to the international system of units (SI) through National Institute of Metrology Thailand (NIMT) Certificate number: TT-1013-25, Certificate number: ER-0061-25.

Reference Used During Calibration:

1. Standard Temperature Probe
Model: STS-100 AS00, Serial No.: 667682-09,
Due date: 9 Apr 2026
2. Digital Temperature Indicator
Model: DTI-1000-A MK II, Serial No.: 671407-
00591 Due date: 22 Apr 2026

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM "Evaluation of measurement data - Guide to the expression of uncertainty in measurement"

Calibrated by:
☐ Mr. Sorawit Thachalad
☒ Miss Jitraporn Lertsomphol
☐ Miss Ruangrumpai Phoommit



Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager

COPY



COPY

Heat Stress Monitor

Model : Ques Temp 34

Serial No. : TEU080011



Jiranatee Associates Co., Ltd.
63/14 15, 67/35 36
Petchkasem 7,7/1, Rd Wathana, Bangkok, Thailand
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC TISI TIS 17025
CALIBRATION 0367

Temperature measurement laboratory
Calibration services department



CERTIFICATE OF CALIBRATION

Certificate No. : CDT-009-69

Page 1 of 2 Pages

MEASUREMENT ITEM

: Heat Stress Monitor

MANUFACTURER

: TSI QUEST

MODEL/TYPE

: Ques Temp 34

SERIAL NUMBER

: TEU080011

ID NUMBER

: NO. 10

CONDITION AS-RECEIVED

: Used item

CUSTOMER

: Eastern Thai Consulting 1992 Co., Ltd.
683 Moo 11, Sukhapibarn 8 Rd,
Nongkham, Sriracha, Chonburi 20230

RECEIVED DATE

: 25 Dec 2025

MEASUREMENT DATE

: 07 Jan 2026

ISSUE DATE

: 08 Jan 2026

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature : 23.0 ± 3.0 °C

Relative Humidity : 55.0 ± 15.0 %RH

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:

The temperature calibration was done by In-House calibration method as WI-CL-001 according to comparison method with standard digital temperature indicator and standard temperature probe. The temperature scale use was based on ITS 90.

Traceability:

The measurement results are traceable to the international system of units (SI) through National Institute of Metrology Thailand (NIMT) Certificate number: TT-1013-25, Certificate number: ER-0061-25.

Reference Used During Calibration:

1. Standard Temperature Probe
Model: STS-100 A500, Serial No.: 667682-09,
Due date: 9 Apr 2026
2. Digital Temperature Indicator
Model: DTI-1000-A MK II, Serial No.: 671407-
00591 Due date: 22 Apr 2026

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Continuation of Certificate of Calibration Number CDT-009-69

Page 2 of 2 Pages

Result of Calibration: ☒ Without Adjustment ☐ With Adjustment

Calibration Range: 20 °C to 40 °C

Function:

Table 1: This equipment was connected with wet bulb Temperature probe Model: -, S/N: -.
Dimension: Diameter 4.77 mm, Length 70 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
65	20.053	20.3	0.2	0.099
65	25.042	25.3	0.3	0.099
65	30.028	30.2	0.2	0.099
65	35.019	35.1	0.1	0.099
65	40.006	40.1	0.1	0.099

Table 2: This equipment was connected with Globe Temperature probe Model: -, S/N: -.
Dimension: Diameter 4.77 mm, Length 70 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
65	20.053	20.4	0.3	0.099
65	25.042	25.3	0.3	0.099
65	30.028	30.2	0.2	0.099
65	35.017	35.2	0.2	0.099
65	40.005	40.0	0.0	0.099


Table 3: This equipment was connected with Dry Bulb Temperature probe Model: -, S/N: -.
Dimension: Diameter 4.77 mm, Length 70 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
65	20.053	20.1	0.0	0.099
65	25.042	25.1	0.1	0.099
65	30.028	30.1	0.1	0.099
65	35.017	35.0	0.0	0.099
65	40.005	40.1	0.1	0.099

UUC: Unit Under Calibration

End of Certificate of Calibration

Calibrated by:
☐ Mr. Sorawit Thachalad
☒ Miss Jitraporn Lertsomphol
☐ Miss Ruangrumpai Phoommit



Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager

COPY



COPY

Heat Stress Monitor

Model : Ques Temp 34

Serial No. : TEU080014



Jiranatee Associates Co., Ltd.
63/14-15, 67/35-16
Petchkusem 7, 7/1, Rd. Wattthapra Bangkokyai,
Bangkok 10600 (Thailand)
Tel : +66(0)6610812
Mobile : +66863999453
E-mail : jnac-calibration@jiranatee.com
Web site : www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC TISI TIS 17025
CALIBRATION 0362

Temperature measurement laboratory
Calibration services department



NSC TISI TIS 17025
CALIBRATION 0367

CERTIFICATE OF CALIBRATION

Certificate No. : CDT-012-69

Page 1 of 2 Pages

MEASUREMENT ITEM : Heat Stress Monitor
MANUFACTURER : TSI QUEST
MODEL/TYPE : Ques Temp 34
SERIAL NUMBER : TEU080014
ID NUMBER : NO. 13
CONDITION AS-RECEIVED : Used item
CUSTOMER : Eastern thai consulting 1992 Co.,Ltd.
683 Moo 11, Sukhapibarn 8 Rd,
Nongkham, Sriracha, Chonburi 20230

RECEIVED DATE : 25 Dec 2025
MEASUREMENT DATE : 08 Jan 2026
ISSUE DATE : 08 Jan 2026

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:
Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:

The temperature calibration was done by In-House calibration method as WI-CL-001 according to comparison method with standard digital temperature indicator and standard temperature probe. The temperature scale use was based on ITS-90.

Traceability:

The measurement results are traceable to the international system of units (SI) through National Institute of Metrology Thailand (NIMT) Certificate number: TT-1013-25, Certificate number: ER-0061-25.

Reference Used During Calibration:

1. Standard Temperature Probe
Model: STS-100 A500, Serial No.: 667682-09,
Due date: 9 Apr 2026
2. Digital Temperature Indicator
Model: DTI 1000-A MK II, Serial No.: 671407-
00591 Due date: 22 Apr 2026

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Continuation of Certificate of Calibration Number CDT-012-69

Page 2 of 2 Pages

Result of Calibration: ☒ Without Adjustment ☐ With Adjustment

Calibration Range: 20 °C to 40 °C

Function:

Table 1: This equipment was connected with wet bulb Temperature probe Model: -, S/N: -, Dimension: Diameter 4.77 mm. Length 70 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
65	20.024	20.5	0.5	0.099
65	25.042	25.4	0.4	0.099
65	30.029	30.4	0.4	0.099
65	35.020	35.3	0.3	0.099
65	40.010	40.3	0.3	0.099

Table 2: This equipment was connected with Globe Temperature probe Model: -, S/N: -, Dimension: Diameter 4.77 mm. Length 70 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
65	20.024	20.3	0.3	0.099
65	25.042	25.3	0.3	0.099
65	30.029	30.3	0.3	0.099
65	35.020	35.2	0.2	0.099
65	40.010	40.2	0.2	0.099

Table 3: This equipment was connected with Dry Bulb Temperature probe Model: -, S/N: -, Dimension: Diameter 4.77 mm. Length 70 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
65	20.024	20.4	0.4	0.099
65	25.042	25.3	0.3	0.099
65	30.029	30.3	0.3	0.099
65	35.020	35.3	0.3	0.14
65	40.010	40.3	0.3	0.099

UUC*: Unit Under Calibration

Remark: The reported uncertainty of measurement is 0.14, based on standard uncertainty multiplied by a coverage factor k=2.14 providing a level of confidence of approximately 95%.

End of Certificate of Calibration

Calibrated by:
☐ Mr. Sorawit Thachalad
☒ Miss Jittraporn Lertsomphol
☐ Miss Ruangrumpai Phoommit



Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager

COPY



COPY

Heat Stress Monitor

Model : Ques Temp 34

Serial No. : TEU080013

CERTIFICATE OF CALIBRATION

Certificate No. : CDT-011-69

Page 1 of 2 Pages

MEASUREMENT ITEM : Heat Stress Monitor
MANUFACTURER : TSI QUEST
MODEL/TYPE : Ques Temp 34
SERIAL NUMBER : TEU080013
ID NUMBER : NO. 12
CONDITION AS-RECEIVED : Used item
CUSTOMER : Eastern thai consulting 1992 Co.,Ltd.
683 Moo 11, Sukhapibarn 8 Rd,
Nongkham, Sriracha, Chonburi 20230

RECEIVED DATE : 25 Dec 2025
MEASUREMENT DATE : 08 Jan 2026
ISSUE DATE : 08 Jan 2026

ENVIRONMENTAL CONDITIONS:
Ambient condition in the laboratory are as follow:
Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:
The table on next page give the measured values.

Calibration procedure:
The temperature calibration was done by
In-House calibration method as WI-CL-001
according to comparison method with standard
digital temperature Indicator and standard
temperature probe. The temperature scale use
was based on ITS-90.

Traceability:
The measurement results are traceable to the
international system of units (SI) through
National Institute of Metrology Thailand (NIMT)
Certificate number: TT-1013-25, Certificate
number: ER-0061-25.

Reference Used During Calibration:
1. Standard Temperature Probe
Model: STS-100 A500, Serial No.: 667682-09,
Due date: 9 Apr 2026
2. Digital Temperature Indicator
Model: DTI-1000-A MK II, Serial No.: 671407-
00591 Due date: 22 Apr 2026

Uncertainty of Measurement:
The reported uncertainty of measurement is
based on the standard uncertainty multiplied by
a coverage factor k=2, Which for a normal
distribution corresponds to a coverage
probability of approximately 95%. The standard
uncertainty has been determined in accordance
with the GUM 'Evaluation of measurement data
- Guide to the expression of uncertainty in
measurement'

Calibrated by:
☐ Mr. Sorawit Thachalad
☒ Miss Jitraporn Lertsomphol
☐ Miss Ruangrumpai Phoommit



Approved signatory:
Mr. Parinya Booncharoen
Calibration Department Manager

COPY

Result of Calibration: ☒ Without Adjustment ☐ With Adjustment

Calibration Range: 20 °C to 40 °C

Function:

Table 1: This equipment was connected with wet bulb Temperature probe Model: -, S/N: -.
Dimension: Diameter 4.77 mm. Length 70 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
65	20.024	20.5	0.5	0.099
65	25.041	25.3	0.3	0.099
65	30.029	30.3	0.3	0.14
65	35.020	35.2	0.2	0.14
65	40.009	40.2	0.2	0.099

Table 2: This equipment was connected with Globe Temperature probe Model: -, S/N: -.
Dimension: Diameter 4.77 mm. Length 70 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
65	20.024	20.4	0.4	0.099
65	25.041	25.4	0.4	0.099
65	30.029	30.4	0.4	0.099
65	35.020	35.4	0.4	0.099
65	40.009	40.3	0.3	0.099

Table 3: This equipment was connected with Dry Bulb Temperature probe Model: -, S/N: -.
Dimension: Diameter 4.77 mm. Length 70 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
65	20.024	20.4	0.4	0.099
65	25.041	25.3	0.3	0.099
65	30.029	30.2	0.2	0.14
65	35.020	35.1	0.1	0.14
65	40.009	39.9	-0.1	0.099

UUC: Unit Under Calibration

Remark: The reported uncertainty of measurement is 0.14, based on standard uncertainty multiplied by a coverage factor k=2.14
providing a level of confidence of approximately 95%.

End of Certificate of Calibration



COPY

Heat Stress Monitor

Model : Ques Temp 32

Serial No. : TPI050069

Result of Calibration: ☒ Without Adjustment ☐ With Adjustment

Calibration Range: 20 °C to 40 °C

Function:

Table 1: This equipment was connected with wet bulb Temperature probe Model: -, S/N: -.
Dimension: Diameter 4.77 mm. Length 70 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
65	20.031	20.3	0.3	0.099
65	25.043	25.3	0.3	0.099
65	30.035	30.3	0.3	0.099
65	35.030	35.3	0.3	0.099
65	40.016	40.3	0.3	0.099

Table 2: This equipment was connected with Globe Temperature probe Model: -, S/N: -.
Dimension: Diameter 4.77 mm. Length 70 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
65	20.031	20.2	0.2	0.099
65	25.043	25.3	0.3	0.099
65	30.036	30.3	0.3	0.099
65	35.030	35.2	0.2	0.099
65	40.016	40.3	0.3	0.099

Table 3: This equipment was connected with Dry Bulb Temperature probe Model: -, S/N: -.
Dimension: Diameter 4.77 mm. Length 70 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
65	20.031	20.2	0.2	0.099
65	25.044	25.3	0.3	0.099
65	30.035	30.2	0.2	0.099
65	35.031	35.3	0.3	0.099
65	40.016	40.2	0.2	0.099

UUC*: Unit Under Calibration

End of Certificate of Calibration

CERTIFICATE OF CALIBRATION

Certificate No. : CDT-015-69

Page 1 of 2 Pages

MEASUREMENT ITEM : Heat Stress Monitor
MANUFACTURER : QUEST TECHNOLOGIES
MODEL/TYPE : Ques Temp 32
SERIAL NUMBER : TPI050069
ID NUMBER : NO. 2
CONDITION AS-RECEIVED : Used item
CUSTOMER : Eastern thai consulting 1992 Co.,Ltd.
683 Moo 11, Sukhapibarn 8 Rd,
Nongkham, Sriracha, Chonburi 20230

RECEIVED DATE : 25 Dec 2025
MEASUREMENT DATE : 09 Jan 2026
ISSUE DATE : 15 Jan 2026

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:
Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:

The temperature calibration was done by
In-House calibration method as WI-CL-001
according to comparison method with standard
digital temperature indicator and standard
temperature probe. The temperature scale use
was based on ITS-90.

Traceability:

The measurement results are traceable to the
international system of units (SI) through
National Institute of Metrology Thailand (NIMT)
Certificate number: TT-1013-25, Certificate
number: ER-0061-25.

Reference Used During Calibration:

1. Standard Temperature Probe
Model: STS-100 A500, Serial No.: 667682-09,
Due date: 9 Apr 2026
2. Digital Temperature Indicator
Model: DTI-1000-A MK II, Serial No.: 671407-
00591 Due date: 22 Apr 2026

Uncertainty of Measurement:

The reported uncertainty of measurement is
based on the standard uncertainty multiplied by
a coverage factor k=2, Which for a normal
distribution corresponds to a coverage
probability of approximately 95%. The standard
uncertainty has been determined in accordance
with the GUM 'Evaluation of measurement data
- Guide to the expression of uncertainty in
measurement'

Calibrated by:
☐ Mr. Sorawit Thachalad
☒ Miss Jittraporn Lertsomphol
☐ Miss Ruangrumpai Phoommit



Approved signatory: 
Mr. Parinya Booncharoen
Calibration Department Manager

COPY



COPY

Heat Stress Monitor

Model : Ques Temp 32

Serial No. : TPL090016



Jranatee Associates Co., Ltd
63/14-15, 67/35-36
Petchkasem 77/1, Rd Wattapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel : +6608680812
Mobile : +66863999453
E-mail : jnac-calibration@jranatee.com
Web site : www.jranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI TIS 17025
CALIBRATION 0367

Temperature measurement laboratory
Calibration services department



Continuation of Certificate of Calibration Number CDT-019-69

Page 2 of 2 Pages

Result of Calibration: ☒ Without Adjustment ☐ With Adjustment

Calibration Range: 20 °C to 40 °C

Function:

Table 1: This equipment was connected with wet bulb Temperature probe Model: -, S/N: -,
Dimension: Diameter 4.77 mm. Length 70 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
65	20.052	20.3	0.2	0.099
65	25.040	25.3	0.3	0.099
65	30.029	30.2	0.2	0.099
65	35.019	35.2	0.2	0.099
65	40.008	40.2	0.2	0.099

Table 2: This equipment was connected with Globe Temperature probe Model: -, S/N: -,
Dimension: Diameter 4.77 mm. Length 70 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
65	20.052	20.3	0.2	0.099
65	25.040	25.3	0.3	0.099
65	30.029	30.3	0.3	0.099
65	35.019	35.3	0.3	0.099
65	40.007	40.3	0.3	0.099

Table 3: This equipment was connected with Dry Bulb Temperature probe Model: -, S/N: -,
Dimension: Diameter 4.77 mm. Length 70 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
65	20.053	20.1	0.0	0.099
65	25.039	25.0	0.0	0.099
65	30.029	30.0	0.0	0.099
65	35.019	35.0	0.0	0.099
65	40.008	39.9	-0.1	0.099

UUC*: Unit Under Calibration

End of Certificate of Calibration

Certificate No. : CDT-019-69

Page 1 of 2 Pages

MEASUREMENT ITEM : Heat Stress Monitor
MANUFACTURER : 3M
MODEL/TYPE : Ques Temp 32
SERIAL NUMBER : TPL090016
ID NUMBER : NO. 6
CONDITION AS-RECEIVED : Used item
CUSTOMER : Eastern thai consulting 1992 Co.,Ltd.
683 Moo 11, Sukhapibarn 8 Rd,
Nongkham, Sriracha, Chonburi 20230

RECEIVED DATE : 25 Dec 2025
MEASUREMENT DATE : 13 Jan 2026
ISSUE DATE : 15 Jan 2026

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:

The temperature calibration was done by
In-House calibration method as WI-CL-001
according to comparison method with standard
digital temperature indicator and standard
temperature probe. The temperature scale use
was based on ITS-90.

Traceability:

The measurement results are traceable to the
international system of units (SI) through
National Institute of Metrology Thailand (NIMT)
Certificate number: TT-1013-25, Certificate
number: ER-0061-25.

Reference Used During Calibration:

1. Standard Temperature Probe
Model: STS-100 A500, Serial No.: 667682-09,
Due date: 9 Apr 2026
2. Digital Temperature Indicator
Model: DTI-1000-A MK II, Serial No.: 671407-
00591 Due date: 22 Apr 2026

Uncertainty of Measurement:

The reported uncertainty of measurement is
based on the standard uncertainty multiplied by
a coverage factor k=2, Which for a normal
distribution corresponds to a coverage
probability of approximately 95%. The standard
uncertainty has been determined in accordance
with the GUM 'Evaluation of measurement data
- Guide to the expression of uncertainty in
measurement'

Calibrated by:
☐ Mr. Sorawit Thachalad
☒ Miss Jitraporn Lertsomphol
☐ Miss Ruangrumpai Phoommit



Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager

COPY



COPY

Heat Stress Monitor

Model : Ques Temp 32

Serial No. : TPQ030024

CERTIFICATE OF CALIBRATION

Certificate No. : CDT-022-69

Page 1 of 2 Pages

MEASUREMENT ITEM : Heat Stress Monitor
MANUFACTURER : 3M
MODEL/TYPE : Ques Temp 32
SERIAL NUMBER : TPQ030024
ID NUMBER : NO. 9
CONDITION AS-RECEIVED : Used item
CUSTOMER : Eastern thai consulting 1992 Co., Ltd.
683 Moo 11, Sukhapibarn 8 Rd,
Nongkham, Sriracha, Chonburi 20230

RECEIVED DATE : 25 Dec 2025
MEASUREMENT DATE : 13 Jan 2026
ISSUE DATE : 15 Jan 2026

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:
Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:

The temperature calibration was done by
In-House calibration method as WI-CL-001
according to comparison method with standard
digital temperature indicator and standard
temperature probe. The temperature scale use
was based on ITS-90.

Traceability:

The measurement results are traceable to the
international system of units (SI) through
National Institute of Metrology Thailand (NIMT)
Certificate number: TT-1013-25, Certificate
number: ER-0061-25.

Reference Used During Calibration:

1. Standard Temperature Probe
Model: STS-100 A500, Serial No.: 667682-09,
Due date: 9 Apr 2026
2. Digital Temperature Indicator
Model: DTI-1000-A MK II, Serial No.: 671407-
00591 Due date: 22 Apr 2026

Uncertainty of Measurement:

The reported uncertainty of measurement is
based on the standard uncertainty multiplied by
a coverage factor k=2, Which for a normal
distribution corresponds to a coverage
probability of approximately 95%. The standard
uncertainty has been determined in accordance
with the GUM 'Evaluation of measurement data
- Guide to the expression of uncertainty in
measurement'

Result of Calibration: ☒ Without Adjustment ☐ With Adjustment

Calibration Range: 20 °C to 40 °C

Function:

Table 1: This equipment was connected with wet bulb Temperature probe Model: -, S/N: -.
Dimension: Diameter 4.77 mm. Length 70 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
65	20.030	20.2	0.2	0.099
65	25.041	25.2	0.2	0.099
65	30.024	30.2	0.2	0.099
65	35.021	35.1	0.1	0.099
65	40.005	40.1	0.1	0.099

Table 2: This equipment was connected with Globe Temperature probe Model: -, S/N: -.
Dimension: Diameter 4.77 mm. Length 70 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
65	20.030	20.3	0.3	0.099
65	25.041	25.2	0.2	0.099
65	30.024	30.2	0.2	0.099
65	35.021	35.2	0.2	0.099
65	40.005	40.1	0.1	0.099

Table 3: This equipment was connected with Dry Bulb Temperature probe Model: -, S/N: -.
Dimension: Diameter 4.77 mm. Length 70 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
65	20.030	20.3	0.3	0.099
65	25.041	25.2	0.2	0.099
65	30.024	30.2	0.2	0.099
65	35.021	35.1	0.1	0.099
65	40.005	40.1	0.1	0.099

UUC*: Unit Under Calibration

End of Certificate of Calibration

Calibrated by:
☐ Mr. Sorawit Thalchalad
☒ Miss Jitraporn Lertsomphol
☐ Miss Ruangrumpai Phoommit



Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager

COPY



COPY

Heat Stress Monitor

Model : Ques Temp 32

Serial No. : TPH060001



Jiranatee Associates Co., Ltd
63/14 15, 67/35-36
Petchkasern 7,7/1, Rd Wathapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +66066060812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI TIS 17025
CALIBRATION 0367

Temperature measurement laboratory
Calibration services department



CERTIFICATE OF CALIBRATION

Certificate No. : CDT-014-69

Page 1 of 2 Pages

MEASUREMENT ITEM : Heat Stress Monitor
MANUFACTURER : TSI QUEST
MODEL/TYPE : Ques Temp 32
SERIAL NUMBER : TPH060001
ID NUMBER : NO. 1
CONDITION AS-RECEIVED : Used item
CUSTOMER : Eastern thai consulting 1992 Co.,Ltd.
683 Moo 11, Sukhapiarn 8 Rd,
Nongkham, Sriracha, Chonburi 20230

RECEIVED DATE : 25 Dec 2025
MEASUREMENT DATE : 09 Jan 2026
ISSUE DATE : 15 Jan 2026

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:
Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:

The temperature calibration was done by
In-House calibration method as WI-CL-001
according to comparison method with standard
digital temperature indicator and standard
temperature probe. The temperature scale use
was based on ITS-90.

Traceability:

The measurement results are traceable to the
international system of units (SI) through
National Institute of Metrology Thailand (NIMT)
Certificate number: TT-1013-25, Certificate
number: ER-0061-25.

Reference Used During Calibration:

- Standard Temperature Probe
Model: STS-100 A500, Serial No.: 667682-09,
Due date: 9 Apr 2026
- Digital Temperature Indicator
Model: DTI-1000-A MK II, Serial No.: 671407-
00591 Due date: 22 Apr 2026

Uncertainty of Measurement:

The reported uncertainty of measurement is
based on the standard uncertainty multiplied by
a coverage factor $k=2$, Which for a normal
distribution corresponds to a coverage
probability of approximately 95%. The standard
uncertainty has been determined in accordance
with the GUM 'Evaluation of measurement data
- Guide to the expression of uncertainty in
measurement'

Continuation of Certificate of Calibration Number CDT-014-69

Page 2 of 2 Pages

Result of Calibration: ☒ Without Adjustment ☐ With Adjustment

Calibration Range: 20 °C to 40 °C

Function:

Table 1: This equipment was connected with wet bulb Temperature probe Model: -, S/N: -,
Dimension: Diameter 4.77 mm. Length 70 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
65	20.052	20.0	-0.1	0.099
65	25.046	25.1	0.1	0.099
65	30.024	29.9	-0.1	0.099
65	35.024	34.9	-0.1	0.099
65	40.002	39.9	-0.1	0.099

Table 2: This equipment was connected with Globe Temperature probe Model: -, S/N: -,
Dimension: Diameter 4.77 mm. Length 70 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
65	20.052	19.9	-0.2	0.099
65	25.046	24.8	-0.3	0.14
65	30.024	29.9	-0.1	0.099
65	35.024	34.7	-0.3	0.14
65	40.002	39.7	-0.3	0.14

Table 3: This equipment was connected with Dry Bulb Temperature probe Model: -, S/N: -,
Dimension: Diameter 4.77 mm. Length 70 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
65	20.051	20.0	-0.1	0.099
65	25.046	25.0	0.0	0.14
65	30.024	29.9	-0.1	0.099
65	35.024	34.9	-0.1	0.099
65	40.002	39.9	-0.1	0.099

UUC*: Unit Under Calibration

Remark: The reported uncertainty of measurement is 0.14, based on standard uncertainty multiplied by a coverage factor $k=2.14$
providing a level of confidence of approximately 95%.

End of Certificate of Calibration

Calibrated by:
☐ Mr. Sorawit Thachalad
☒ Miss Jitraporn Lertsomphol
☐ Miss Ruangrumpai Phoornmit



Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager

COPY



COPY

Heat Stress Monitor

Model : Ques Temp 32

Serial No. : TPL090017



Jiranatee Associates Co., Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel : +6608680812
Mobile: +66863999453
E-mail : jnac-calibration@jiranatee.com
Web site : www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Temperature measurement laboratory
Calibration services department.



CERTIFICATE OF CALIBRATION

Certificate No. : CDT-020-69

Page 1 of 2 Pages

MEASUREMENT ITEM : Heat Stress Monitor
MANUFACTURER : 3M
MODEL/TYPE : Ques Temp 32
SERIAL NUMBER : TPL090017
ID NUMBER : NO. 7
CONDITION AS-RECEIVED : Used item
CUSTOMER : Eastern thai consulting 1992 Co.,Ltd.
683 Moo 11, Sukhapibarn 8 Rd,
Nongkham, Sriracha, Chonburi 20230

RECEIVED DATE : 25 Dec 2025
MEASUREMENT DATE : 13 Jan 2026
ISSUE DATE : 15 Jan 2026

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:
Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:

The temperature calibration was done by
In-House calibration method as WI-CL-001
according to comparison method with standard
digital temperature indicator and standard
temperature probe. The temperature scale use
was based on ITS-90.

Traceability:

The measurement results are traceable to the
international system of units (SI) through
National Institute of Metrology Thailand (NIMT)
Certificate number: TT-1013-25, Certificate
number: ER-0061-25.

Reference Used During Calibration:

1. Standard Temperature Probe
Model: STS-100 A500, Serial No.: 667682-09,
Due date: 9 Apr 2026
2. Digital Temperature Indicator
Model: DTI-1000-A MK II, Serial No.: 671407-
00591 Due date: 22 Apr 2026

Uncertainty of Measurement:

The reported uncertainty of measurement is
based on the standard uncertainty multiplied by
a coverage factor $k=2$, Which for a normal
distribution corresponds to a coverage
probability of approximately 95%. The standard
uncertainty has been determined in accordance
with the GUM 'Evaluation of measurement data
- Guide to the expression of uncertainty in
measurement'

Continuation of Certificate of Calibration Number CDT-020-69

Page 2 of 2 Pages

Result of Calibration: ☒ Without Adjustment ☐ With Adjustment

Calibration Range: 20 °C to 40 °C

Function:

Table 1: This equipment was connected with wet bulb Temperature probe Model: -, S/N: -.
Dimension: Diameter 4.77 mm. Length 70 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
65	20.014	19.8	-0.2	0.099
65	25.040	24.8	-0.2	0.099
65	30.031	29.7	-0.3	0.099
65	35.023	34.8	-0.2	0.099
65	40.002	39.8	-0.2	0.099

Table 2: This equipment was connected with Globe Temperature probe Model: -, S/N: -.
Dimension: Diameter 4.77 mm. Length 70 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
65	20.014	19.9	-0.1	0.099
65	25.040	24.9	-0.1	0.099
65	30.031	29.9	-0.1	0.099
65	35.023	34.9	-0.1	0.099
65	40.002	39.8	-0.2	0.099


Table 3: This equipment was connected with Dry Bulb Temperature probe Model: -, S/N: -.
Dimension: Diameter 4.77 mm. Length 70 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
65	20.014	19.6	-0.4	0.099
65	25.040	24.6	-0.4	0.099
65	30.031	29.6	-0.4	0.099
65	35.023	34.6	-0.4	0.099
65	40.002	39.6	-0.4	0.099

UUC*: Unit Under Calibration

End of Certificate of Calibration

Calibrated by:
☐ Mr. Sorawit Thachalad
☒ Miss Jitraporn Lertsomphol
☐ Miss Ruangrumpai Phoommit



Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager

COPY



COPY

Heat Stress Monitor

Model : Ques Temp 32

Serial No. : TPQ030023



Jiranatee Associates Co., Ltd.
64/14-15, 67/35, 36
Petchkasem 77/1, Rd. Wattana, Bangkokkay,
Bangkok 10600 (Thailand)
Tel. +6608640812
Mobile +66863989453
E-mail jnac.calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC TISI TIS 17025
CALIBRATION 0367

Temperature measurement laboratory
Calibration services department



Continuation of Certificate of Calibration Number CDT-021-69

Page 2 of 2 Pages

Result of Calibration: ☒ Without Adjustment ☐ With Adjustment

Calibration Range: 20 °C to 40 °C

Function:

Table 1: This equipment was connected with wet bulb Temperature probe Model: -, S/N: -,
Dimension: Diameter 4.77 mm. Length 70 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
65	20.013	20.2	0.2	0.099
65	25.041	25.2	0.2	0.099
65	30.033	30.2	0.2	0.14
65	35.023	35.2	0.2	0.099
65	40.006	40.2	0.2	0.099

Table 2: This equipment was connected with Globe Temperature probe Model: -, S/N: -,
Dimension: Diameter 4.77 mm. Length 70 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
65	20.013	20.2	0.2	0.14
65	25.041	25.2	0.1	0.14
65	30.033	30.2	0.1	0.14
65	35.023	35.1	0.1	0.14
65	40.006	40.1	0.1	0.14

Table 3: This equipment was connected with Dry Bulb Temperature probe Model: -, S/N: -,
Dimension: Diameter 4.77 mm. Length 70 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
65	20.013	20.2	0.2	0.099
65	25.041	25.2	0.2	0.099
65	30.033	30.2	0.2	0.099
65	35.023	35.2	0.2	0.099
65	40.006	40.1	0.1	0.099

UUC*: Unit Under Calibration

Remark: The reported uncertainty of measurement is 0.14, based on standard uncertainty multiplied by a coverage factor k=2.14 providing a level of confidence of approximately 95%.

End of Certificate of Calibration

Certificate No. : CDT-021-69

Page 1 of 2 Pages

MEASUREMENT ITEM : Heat Stress Monitor
MANUFACTURER : 3M
MODEL/TYPE : Ques Temp 32
SERIAL NUMBER : TPQ030023
ID NUMBER : NO. 8
CONDITION AS-RECEIVED : Used item
CUSTOMER : Eastern thai consulting 1992 Co.,Ltd.
683 Moo 11, Sukhapibarn 8 Rd,
Nongkham, Sriracha, Chonburi 20230

RECEIVED DATE : 25 Dec 2025
MEASUREMENT DATE : 13 Jan 2026
ISSUE DATE : 15 Jan 2026

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:

The temperature calibration was done by
In-House calibration method as WI-CL-001
according to comparison method with standard
digital temperature indicator and standard
temperature probe. The temperature scale use
was based on ITS-90.

Traceability:

The measurement results are traceable to the
international system of units (SI) through
National Institute of Metrology Thailand (NIMT)
Certificate number: TT-1013-25, Certificate
number: FR-0061-25.

Reference Used During Calibration:

1. Standard Temperature Probe
Model: STS-100 A500, Serial No.: 667682-09,
Due date: 9 Apr 2026
2. Digital Temperature Indicator
Model: DTI-1000-A MK II, Serial No.: 671407-
00591 Due date: 22 Apr 2026

Uncertainty of Measurement:

The reported uncertainty of measurement is
based on the standard uncertainty multiplied by
a coverage factor k=2, Which for a normal
distribution corresponds to a coverage
probability of approximately 95%. The standard
uncertainty has been determined in accordance
with the GUM 'Evaluation of measurement data
- Guide to the expression of uncertainty in
measurement'

Calibrated by:
☐ Mr. Sorawit Thachalad
☒ Miss Jitraporn Lertsomphol
☐ Miss Ruangrumpai Phoommit



Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager

COPY



COPY

Heat Stress Monitor

Model : Ques Temp 32

Serial No. : TPI050070



Jiramatee Associates Co., Ltd.
63/14-15, 67/35-36
Petchkasem 7 7/1, Rd Wattthapari, Bangkokkay,
Bangkok 10600 (Thailand)
Tel : +66(0)260812
Mobile : +66(0)999454
E-mail : jnac-calibration@jiramatee.com
Web site : www.jiramatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC TISI TIS 17025
CALIBRATION 0367

Temperature measurement laboratory
Calibration services department



Continuation of Certificate of Calibration Number CDT-016-69

Page 2 of 2 Pages

Result of Calibration: ☐ Without Adjustment ☒ With Adjustment

Calibration Range: 20.0 to 40.0 °C

Function:

Table 1: This equipment was connected with wet bulb Temperature probe Model: -, S/N: -,
Dimension: Diameter 4.77 mm. Length 70 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
65	20.055	20.4	0.3	0.099
65	25.040	25.4	0.4	0.099
65	30.033	30.3	0.3	0.099
65	35.023	35.3	0.3	0.099
65	40.004	40.3	0.3	0.099

Table 2: This equipment was connected with Globe Temperature probe Model: -, S/N: -,
Dimension: Diameter 4.77 mm. Length 70 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
65	20.055	20.2	0.1	0.099
65	25.040	25.2	0.2	0.099
65	30.033	30.2	0.2	0.099
65	35.023	35.2	0.2	0.099
65	40.004	40.2	0.2	0.099

Table 3: This equipment was connected with Dry Bulb Temperature probe Model: -, S/N: -,
Dimension: Diameter 4.77 mm. Length 70 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
65	20.055	20.4	0.3	0.099
65	25.040	25.3	0.3	0.099
65	30.033	30.3	0.3	0.099
65	35.023	35.3	0.3	0.099
65	40.004	40.3	0.3	0.099

UUC*: Unit Under Calibration

End of Certificate of Calibration

Certificate No. : CDT-016-69

Page 1 of 2 Pages

MEASUREMENT ITEM : Heat Stress Monitor
MANUFACTURER : QUEST TECHNOLOGIES
MODEL/TYPE : Ques Temp 32
SERIAL NUMBER : TP1050070
ID NUMBER : NO. 3
CONDITION AS-RECEIVED : Used item
CUSTOMER : Eastern thai consulting 1992 Co.,Ltd.
683 Moo 11, Sukhapibarn 8 Rd,
Nongkham, Sriracha, Chonburi 20230

RECEIVED DATE : 25 Dec 2025
MEASUREMENT DATE : 12 Jan 2026
ISSUE DATE : 15 Jan 2026

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:

The temperature calibration was done by
In-House calibration method as WI-CL-001
according to comparison method with standard
digital temperature indicator and standard
temperature probe. The temperature scale use
was based on ITS-90.

Traceability:

The measurement results are traceable to the
international system of units (SI) through
National Institute of Metrology Thailand (NIMT)
Certificate number: TT-1013-25, Certificate
number: ER-0061-25.

Reference Used During Calibration:

1. Standard Temperature Probe
Model: STS-100 A500, Serial No.: 667682-09,
Due date: 9 Apr 2026
2. Digital Temperature Indicator
Model: DTI-1000-A MK II, Serial No.: 671407-
00591 Due date: 22 Apr 2026

Uncertainty of Measurement:

The reported uncertainty of measurement is
based on the standard uncertainty multiplied by
a coverage factor k=2, Which for a normal
distribution corresponds to a coverage
probability of approximately 95%. The standard
uncertainty has been determined in accordance
with the GUM 'Evaluation of measurement data -
Guide to the expression of uncertainty in
measurement'

Calibrated by:
☐ Mr. Sorawit Thachalad
☒ Miss Jitraporn Lertsomphol
☐ Miss Ruangrumpai Phoommit



Approved signatory

Mr. Parinya Booncharoen
Calibration Department Manager

COPY



COPY

Hot Air Oven

Model : UFE 500

Serial No. : G511.0182

CERTIFICATE OF CALIBRATION

Certificate No. : 25-215653

Sample Code : 25-94507-006

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
583 Moo 11, Sukhapibarn 8 Rd., Nongkham,
Sriracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.
(Hot Lab)

Equipment : Temperature controlled enclosures (Hot air oven)

Manufacturer : Memmert Model : UFE 500

Serial No. : G511.0182 ID No. : LABE 17/4

Date of Receipt : 16 December 2025 Date of Calibration : 16 December 2025

Condition of Calibration

1. Environment
- | | | | | |
|---------------------------|-----------|-----------|-----------|-----------|
| 1.1 Ambient temperature | : Maximum | 27.6 °C | : Minimum | 26.4 °C |
| 1.2 Relative humidity | : Maximum | 61.4 % | : Minimum | 54.0 % |
| 1.3 Line voltage supplied | : Maximum | 229.7 VAC | : Minimum | 225.6 VAC |

2. Calibration method

TLAS-G-20: Guidelines for calibration and checks of temperature controlled enclosures.

3. Reference standard instrument

Instrument	ID No.	Certificate No.	Due Date
Data acquisition with sensor (RTD-Prt100)	LB-DA-19 (RTD-302 to RTD-303, RTD-311, RTD-305 to RTD-310)	25-010559	04 February 2026

4. This certificate is traceable to the international system of unit (SI Unit).

The measurement is traceable to Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by Mr. Natthanan Phosri
Scientist

Approved by

(Mr. Somchai Nearpunt)
Signed for Director

Issue date 17 December 2025

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

REPORT OF CALIBRATION

Certificate No. : 25-215653

Sample Code : 25-94507-006

Results of Calibration

Resolution : 0.5 °C

1. Reporting of Temperature

Calibration point (°C)	UUC* setting (°C)	UUC* reading (°C)	Measured temperature at each positions (°C)									Uncertainty $\pm$ (°C)	Coverage factor k
			# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9 ^{Ref}		
104	103.5	103.5	103.98	103.97	103.67	103.76	104.10	104.22	103.80	103.52	103.92	0.47	2.00

2. Characterization results

Calibration point (°C)	Stability (°C)	Uniformity (°C)	Open thermocouple (°C)
104	0.07	0.46	0.84

Notes

* UUC* = Unit Under Calibration



COPY

COPY



REPORT OF CALIBRATION

Page 3 of 3


Certificate No. : 25-215653

Sample Code : 25-94507-006

Results of Calibration

Notes

1. Sensor installation locations
 - 1.1 All sensors at any corners or walls should be positioned 5 cm (a x b x c) from the wall.
 - 1.2 The reference sensor is preferably located of the geometric center of the chamber.
2. Interior dimensions approx of chamber :
W = 56 cm ; D = 40 cm ; H = 48 cm
3. Air valve or fresh air level : Off
4. Fan level : Open
5. The quoted uncertainty includes " Stability of chamber and loading effect in chamber at 20% of uniformity ".
6. Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
7. Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.
8. Overall variation - the difference of the maximum and the minimum measured temperatures throughout observation time.
9. UUC* reading - the average reading of indicating device that forms the integral part of the enclosure.
10. Calibration results without adjustment.

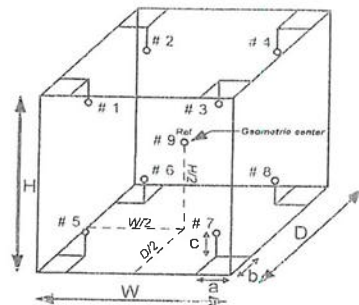Figure: Example of sensor
installation Positions

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003

- End of Report -

COPY

IC-THERMO

Serial No. : 20053176



Certificate of Calibration

Integrion RFIC: Anion and Cation (ID#960)

This certificate is to verify that instrument below are calibrated

by Archemica Lab Co.,Ltd.

Integrion S/N: 20053176

AS-DV S/N: 2008880131

for

Eastern Thai Consulting 1992 Co., Ltd.



Operator Signature : Saharat Popayom

Date : October 6-7, 2025

(Mr. Saharat Popayom)

Applications Chemist

COPY

INDUCTIBELY COUPLED PLASMA SPECTROMETER

Model : Prodigy 7

Serial No. : P70177



Instrument Performance Certificate For ICP-OES

PRODUCT ID *Prodigy 7, Teledyne Leeman Labs*
Serial Number *P70177*

Customer Name *Eastern Thai Consulting 1992 Co.,Ltd*
Address *683 Moo 11 Tambon Nong Kham, Si Racha, Chonburi 20230*

Date of Qualified *Nov 3, 2025*
Next Due date *May 2, 2025*

This certifies for products which was performed in acceptable criteria specifications

Gas supply /Water chiller/Exhaust hood	PASSED
Spectrometer	PASSED
RF Generator	PASSED
Sample Introduction & Autosampler	PASSED
Software & Computer	PASSED
Hardware Diagnostics Test	PASSED
Analytical Test	PASSED

Provided by
Scientist Instrument Co.,Ltd.
113 Soi Ekachai 44, Ekachai Road
Klong Bang Phran, Bangbon
Bangkok 10150 Thailand

Certified by *Thunraphol Sakdayos*
Thunraphol Sakdayos
Service Engineer

COPY



Preventive Maintenance Report

Customer Name:	<i>Eastern Thai Consulting 1992 Co.,Ltd</i>	Date:	<i>Nov 3 ,2025</i>
Instrument/Equipment:	<i>ICP-OES</i>	Model:	<i>Prodigy 7</i>
Brand:	<i>Teledyne Leeman Labs</i>	S/N:	<i>P70177</i>

1. Gas Supply / Water Chiller / Exhaust Hood:	Status
Gas systems:	
Argon Pressure (80-95 psi): <i>90</i> psi	OK ☒
Nitrogen Pressure (80-95 psi): <i>-</i> psi	OK ☐
No leak inspected	OK ☒
Replace camera purge gas Dhydrator	OK ☒ <i>Checked ok</i>
Water Chiller for RF generator	OK ☒
Pressure <i>30</i> psi (2 L/min)	OK ☒
Temperature: <i>22-45</i> °C	OK ☒ <i>Ambient ok</i>
No leak inspected	OK ☒
Water Chiller for Detector	OK ☒
Check water level and refill	OK ☒
Change water	OK ☒
Temperature: <i>28</i> °C	OK ☒
Exhaust Hood:	OK ☒
Air Flow rate (> 105 cfm) <i>>105</i> cfm	OK ☒
2.Spectrometer	Status
Optical view position	
Axial peak positions x <i>332.0</i> y <i>1200</i>	OK ☒
Radial peak positions x <i>422.6</i> y <i>11.96</i>	OK ☒
Hg lamp peak positions x <i>2245</i> y <i>3615</i>	OK ☒
Wavelength Calibrate with HG Lamp	OK ☒
Full Frame Image	OK ☒
Temperature controlled <i>31</i> °C	OK ☒
Purge gas flow control Low/High	OK ☒
Camera Support Module	OK ☒

Engineer Sign

Thunraphol Sakdayos

COPY

3.RF Generator		Status
Plasma Control		
Auto Start	OK ☒	
Extinguish	OK ☒	
RF power setting	OK ☒	
Igniter	OK ☒	
Air Knife	OK ☒	
Coolant/Plasma Flow control	OK ☒	
Aux Flow	OK ☒	
Optimize sample introduction function	OK ☒	
Camera Support Module	OK ☒	
4.Sample Introduction & Autosampler		Status
Plasma torch		
Plasma Torch	OK ☒	
Spray chamber	OK ☒	
Injector	OK ☒	
Nebulizer pressure	OK ☒	
Peristaltic pump and control		
speed control	OK ☒	
Sample tubing	OK ☒	
Drain tubing	OK ☒	
Autosampler Control		
Position movement	OK ☐	No Option
Drain tubing	OK ☐	
Auto Rinse	OK ☐	
5.Computer & Software Check:		Status
Interface Cable USB	OK ☒	
Software Version 5.2	OK ☒	
Operation function check :	OK ☒	
Open /Save /Edit method	OK ☒	
Instrument Control	OK ☒	
Sequence	OK ☒	
Full Frame Capture	OK ☒	
Auto alignment /Hg alignment	OK ☒	
Calibration Curve	OK ☒	
Re-Calculation	OK ☒	
Print Report	OK ☒	

Engineer Sign

Enmar

COPY

6.Hardware Diagnostics Test			
Power Supply	Reference Value	Reading Value	Status
	-12 VDC (+/- 5 %)	-13.7 V	Passed ☒
	+12 VDC (+/- 5 %)	11.91 V	Passed ☒
	3.3VDC (+/- 5 %)	3.206 V	Passed ☒
	+5.0 VDC (+/- 5 %)	4.995 V	Passed ☒
	+13.5 VDC (+/- 7.5 %)	13.4 V	Passed ☒
Plasma Generator			
	ICP Current 0.500A = 1kW	0.502 A	Passed ☐
	ICP Ref 5.0Vdc = 1kW	5.001 V	Passed ☐
	ICP Current 0.00 Vdc = 0kW	0.000 A	Passed ☒
	ICP Ref 0.00Vdc = 0kW	0.000 V	Passed ☒
	RF Water (Hz) OFF (1 Hz)	0 Hz	Passed ☒
	RF Water (Hz) ON (20-35 Hz)	22 Hz	Passed ☒
	Air Knife Pres. (0.00V) OFF	0.0 V	Passed ☒
	Air Knife Pres. (3.0 - 7.0 V) ON	4.2 V	Passed ☒
	Neb pressure setting of 25 psi	25.0 psi	Passed ☒
	Cool flowrate setting of 16 lpm	16.0 lpm	Passed ☒
	Aux flowrate setting of 0.3 lpm	0.34 lpm	Passed ☒
Camera Support Module			
	Pump Current (0.000 A) OFF	0.0 A	Passed ☐
	Pump Voltage (0.000 V) OFF	0.0 V	Passed ☐
	Pump Current (0.8 to 4.0A) ON	1.03 A	Passed ☒
	Pump Voltage (8 to 13 V) ON	12.52 V	Passed ☒
	Water chiller Temp. Setting 25 °C	25.2 °C	Passed ☒
	Cam Tec Temperature Setting 32 °C	32 °C	Passed ☒
Optical purge flowrate			
	Optical Purge Low Setting 5 lpm	5.0 lpm	Passed ☒
	Optical Purge High Setting 10 lpm	10.0 lpm	Passed ☒

7.Cleaning & Replacement		Status
O-Ring Torch replacement	OK ☒	checked ok
Pump Tubing replacement	OK ☒	
Glassware cleaning	OK ☒	
Lubricate the roll peristaltic pump	OK ☒	
Optical windows cleaning	OK ☒	
Change & refilled Detector water chiller	OK ☒	
Change & refilled RF Generator water Chiller	OK ☒	



Engineer Sign

Enmar

COPY

8.Safety Interlock		Status
Argon pressure	OK	☒
Air Knife	OK	☒
RF power regulator	OK	☒
RF power temp	OK	☒
RF power current	OK	☒
RF water	OK	☒
Oscillator cover	OK	☒
Door switch	OK	☒
Camera purge	OK	☒
Camera TE cooler	OK	☒
Water chiller	OK	☒
Heater Fans	OK	☒

9.Analytical Test		Details	Status
Method Name	Mn	Setup	
SRM Standard	Mn	5 ppm	
Calibration curve type		Linear	
Rho	1.0		OK ☒
Element	Mn		
QC standard Check	5 ppm		OK ☒

Customer Sign	Engineer Sign
	 3/11/2568

Diagnostics			
Status		Status	
Minor 1	0.00	Minor 2	0.00
Minor 3	0.00	Minor 4	0.00
Minor 5	0.00	Minor 6	0.00
Minor 7	0.00	Minor 8	0.00
Minor 9	0.00	Minor 10	0.00
Minor 11	0.00	Minor 12	0.00
Minor 13	0.00	Minor 14	0.00
Minor 15	0.00	Minor 16	0.00
Minor 17	0.00	Minor 18	0.00
Minor 19	0.00	Minor 20	0.00
Minor 21	0.00	Minor 22	0.00
Minor 23	0.00	Minor 24	0.00
Minor 25	0.00	Minor 26	0.00
Minor 27	0.00	Minor 28	0.00
Minor 29	0.00	Minor 30	0.00
Minor 31	0.00	Minor 32	0.00
Minor 33	0.00	Minor 34	0.00
Minor 35	0.00	Minor 36	0.00
Minor 37	0.00	Minor 38	0.00
Minor 39	0.00	Minor 40	0.00
Minor 41	0.00	Minor 42	0.00
Minor 43	0.00	Minor 44	0.00
Minor 45	0.00	Minor 46	0.00
Minor 47	0.00	Minor 48	0.00
Minor 49	0.00	Minor 50	0.00
Minor 51	0.00	Minor 52	0.00
Minor 53	0.00	Minor 54	0.00
Minor 55	0.00	Minor 56	0.00
Minor 57	0.00	Minor 58	0.00
Minor 59	0.00	Minor 60	0.00
Minor 61	0.00	Minor 62	0.00
Minor 63	0.00	Minor 64	0.00
Minor 65	0.00	Minor 66	0.00
Minor 67	0.00	Minor 68	0.00
Minor 69	0.00	Minor 70	0.00
Minor 71	0.00	Minor 72	0.00
Minor 73	0.00	Minor 74	0.00
Minor 75	0.00	Minor 76	0.00
Minor 77	0.00	Minor 78	0.00
Minor 79	0.00	Minor 80	0.00
Minor 81	0.00	Minor 82	0.00
Minor 83	0.00	Minor 84	0.00
Minor 85	0.00	Minor 86	0.00
Minor 87	0.00	Minor 88	0.00
Minor 89	0.00	Minor 90	0.00
Minor 91	0.00	Minor 92	0.00
Minor 93	0.00	Minor 94	0.00
Minor 95	0.00	Minor 96	0.00
Minor 97	0.00	Minor 98	0.00
Minor 99	0.00	Minor 100	0.00

~~COPY~~

~~COPY~~

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method - Hg 253.652 m

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

Initial Method


Initial Method

Initial Method

Initial Method

Initial Method

Initial Method

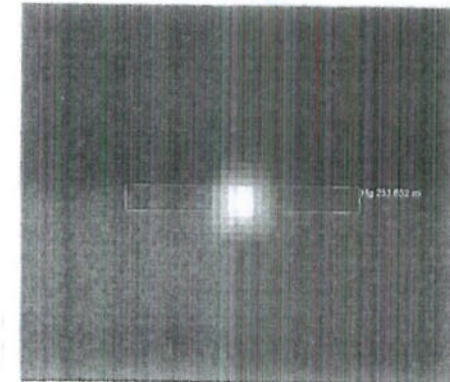


2nd Order

2nd Order

COPY

COPY

Mn Setup - Mn 257.610

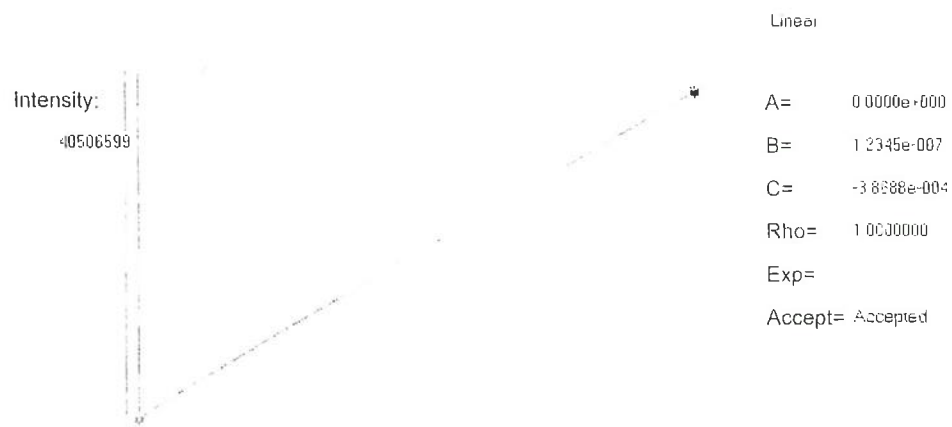

Max Conc: 5.000 ppm

Std ID	Conc	Calc	Dev	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
Mn	5.000	5.000	0.000	40506599	0.2 %	40500970	40404947	40613882		
Blank	0	1.66e-016	0.000	3134	578.179	3952	2727	2724		

~~COPY~~

Mn Setup - Mn 257.610 r



Max Conc: 5.000 ppm

Std ID	Conc	Calc	Dev	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
Mn	5.000	5.000	0.000	367888	0.6 %	368243	364847	370576		
Blank	0	-6.33e-017	0.000	122	3.859	126	117	124		

~~COPY~~

PM Test Report 3 November 2025

Date Printed: 03 Nov 25 11:44:16

Sample ID	Line	Conc.	Intensity
Blank - 1	Mn 257.610	-	3952
Blank - 1	Mn 257.610 r	-	126
Blank - 2	Mn 257.610	-	2727
Blank - 2	Mn 257.610 r	-	117
Blank - 3	Mn 257.610	-	2724
Blank - 3	Mn 257.610 r	-	124
Mn - 1	Mn 257.610	-	40500970
Mn - 1	Mn 257.610 r	-	368243
Mn - 2	Mn 257.610	-	40404947
Mn - 2	Mn 257.610 r	-	364847
Mn - 3	Mn 257.610	-	40613882
Mn - 3	Mn 257.610 r	-	370576
QC Check 5 ppm - 1	Mn 257.610	5.0594	40988160
QC Check 5 ppm - 1	Mn 257.610 r	5.0111	368708
QC Check 5 ppm - 2	Mn 257.610	5.0271	40726441
QC Check 5 ppm - 2	Mn 257.610 r	5.0148	368980
QC Check 5 ppm - 3	Mn 257.610	5.0679	41056315
QC Check 5 ppm - 3	Mn 257.610 r	4.9638	365228
QC Check 5 ppm - 4	Mn 257.610	5.0515	40923751
QC Check 5 ppm - 4	Mn 257.610 r	5.0040	368180
QC Check 5 ppm - 5	Mn 257.610	5.0533	40938450
QC Check 5 ppm - 5	Mn 257.610 r	4.9881	367015
QC Check 5 ppm - 6	Mn 257.610	5.0864	41206181
QC Check 5 ppm - 6	Mn 257.610 r	4.9493	364157
QC Check 5 ppm - 7	Mn 257.610	5.0544	40947211
QC Check 5 ppm - 7	Mn 257.610 r	5.0685	372928
QC Check 5 ppm - 8	Mn 257.610	5.0681	41058127
QC Check 5 ppm - 8	Mn 257.610 r	4.9847	366763
QC Check 5 ppm - 9	Mn 257.610	5.0669	41048908
QC Check 5 ppm - 9	Mn 257.610 r	5.0494	371520
QC Check 5 ppm - 10	Mn 257.610	5.0481	40896149
QC Check 5 ppm - 10	Mn 257.610 r	4.9444	363799

~~COPY~~

ORIFICE TRANSFER STANDARD CERTIFICATION

WORKSHEET TE-5025A

ROOTSMETER S/N 0438320



TISCH ENVIRONMENTAL, INC.
145 SOUTH MIAMI AVE
VILLAGE OF CLEVELAND, OH
44102
513.467.9000
877.263.7810 TOLL FREE
513.467.9009 FAX

ORIFICE TRANSFER STANDARD CERTIFICATION WORKSHEET TE-5025A

Date - Mar 24, 2016 Rootmeter S/N 0438320 Ta (K) - 295
Operator Tisch Orifice I.D. - 0136 Pa (mm) - 742.95

PLATE OR Run #	VOLUME START (m3)	VOLUME STOP (m3)	DIFF VOLUME (m3)	DIFF TIME (min)	METER DIFF Hg (mm)	ORFICE DIFF H2O (in.)
1	NA	NA	1.00	1.3400	3.2	2.00
2	NA	NA	1.00	0.9510	6.3	4.00
3	NA	NA	1.00	0.8510	7.8	5.00
4	NA	NA	1.00	0.8130	8.6	5.50
5	NA	NA	1.00	0.6690	12.6	8.00

DATA TABULATION

Vstd	(x axis) Qstd	(y axis)	Va	(x axis) Qa	(y axis)
0.9832	0.7337	1.4054	0.9957	0.7430	0.8911
0.9791	1.0296	1.9875	0.9915	1.0426	1.2603
0.9770	1.1481	2.2221	0.9894	1.1626	1.4090
0.9760	1.2006	2.3305	0.9884	1.2157	1.4778
0.9707	1.4510	2.8107	0.9830	1.4694	1.7823
Qstd slope (m)	=	1.96262	Qa slope (m)	=	1.22896
intercept (b)	=	-0.03249	intercept (b)	=	-0.02060
coefficient (r)	=	0.99993	coefficient (r)	=	0.99993

y axis = SQRT[H2O(Pa/760) (298/Ta)]

y axis = SQRT[H2O(Ta/Pa)]

CALCULATIONS

Vstd = Diff. Vol [(Pa-Diff. Hg)/760] (298/Ta)
Qstd = Vstd/Time

Va = Diff Vol [(Pa-Diff Hg)/Pa]
Qa = Va/Time

For subsequent flow rate calculations:

Qstd = 1/m{ [SQRT(H2O(Pa/760) (298/Ta))] - b}
Qa = 1/m{ [SQRT H2O(Ta/Pa)] - b}

COPY

Primary Flow Calibrator

Serial No. : 110619 , 207510

Accredited
1903/1913 1/2006

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE	:	PRIMARY FLOW CALIBRATOR
MANUFACTURER	:	BIOS INTERNATIONAL
MODEL / TYPE	:	DEFENDER 510-L
SERIAL NO.	:	110619
CLID. NO.	:	212500238
JOB CONTROL NO.	:	260113004617
CALIBRATION SERVICE	:	☒ IN-LABORATORY ☐ ON-SITE

CUSTOMER : EASTERN THAI CONSULTING 1992 CO., LTD.
683 MOO 11, SUKHAPIBARN 8 RD,
NONGKHAM, SRIRACHA, CHONBURI 20230

DATE OF RECEIVED : 13 January 2026

DATE OF ISSUED : 15 January 2026

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Supphakit Sakuntaharn
Calibration Engineer

ad

Approved By : Mongkol Yotsoontorn
Authorized Signatory
15 January 2026



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q26004617

F3-011-05/12-23

COPY

page 1 of 3



REPORT OF CALIBRATION

444 444
 444 444
 444 444
 444 444

NOMENCLATURE	:	PRIMARY FLOW CALIBRATOR
MANUFACTURER	:	BIOS INTERNATIONAL
MODEL / TYPE	:	DEFENDER 510-I
SERIAL NO.	:	f10619
DATE OF CALIBRATION	:	14 January 2026

ENVIRONMENT CONDITIONS :

Temperature : $(23 \pm 2) ^\circ\text{C}$ Relative Humidity : $(55 \pm 10) \% \text{ RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. CLC-CPPF-03. The calibration was performed by comparison with Gas Flow Meter which refers to the standard condition of 101.325 kPa and 0 °C.

REFERENCE STANDARD USED :

Gas Flow Meter, Alicat Scientific Model M-500SCCM-D-DB15 S/N. 261329.

TRACEABILITY :

The measurements are traceable to International System of Units (SI), through Chell Instrument Ltd.
Certificate No. N039746, Due Date 02 April 2026.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2$ which for a normal distribution corresponds to a coverage probability of approximately 95 %. It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q26004617

P3-011-05/12-23

COPY

page 2 of 3





CALIBRATION LABORATORY CO., LTD.

204/17, 135 Southern Road, 2nd Floor, Prachinburi Road, Prachinburi, Thailand 31000
Tel: 03743 02581, 03743 02582, www.clab.co.th, Email: info@clab.co.th



Accredited
ISO/IEC 17025

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : PRIMARY FLOW CALIBRATOR
MANUFACTURER : MESALABS
MODEL / TYPE : DEFENDER 510-M
SERIAL NO. : 207510
CLID. NO. : 212500237
JOB CONTROL NO. : 260113004618
CALIBRATION SERVICE : ☒ IN-LABORATORY ☐ ON-SITE

CUSTOMER : EASTERN THAI CONSULTING 1992 CO., LTD.
683 MOO 11, SUKHAPIBARN 8 RD,
NONGKHAM, SRIRACHA, CHONBURI 20230

DATE OF RECEIVED : 13 January 2026

DATE OF ISSUED : 15 January 2026

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Supphakit Sakuntaharn

Calibration Engineer

Approved By :

Mongkol Yotsoontorn

Authorized Signatory

15 January 2026



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q26004618

F3-011-05/12-23

page 1 of 3



CALIBRATION LABORATORY CO., LTD.

204/17, 135 Southern Road, 2nd Floor, Prachinburi Road, Prachinburi, Thailand 31000
Tel: 03743 02581, 03743 02582, www.clab.co.th, Email: info@clab.co.th



REPORT OF CALIBRATION

FOR

NOMENCLATURE : PRIMARY FLOW CALIBRATOR
MANUFACTURER : MESALABS
MODEL / TYPE : DEFENDER 510-M
SERIAL NO. : 207510
DATE OF CALIBRATION : 14 January 2026

ENVIRONMENT CONDITIONS :

Temperature : $(23 \pm 2) ^\circ\text{C}$

Relative Humidity : $(55 \pm 10) \% \text{ RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. CLC-CPPE-03. The calibration was performed by comparison with Gas Flow Meter which refers to the standard condition of 101.325 kPa and 0 $^\circ\text{C}$.

REFERENCE STANDARD USED :

Gas Flow Meter, Alicat Scientific Model M-SSLPM-D-DB15 S/N. 261330.

TRACEABILITY :

The measurements are traceable to International System of Units (SI), through Chell Instrument Ltd.

Certificate No. N039747, Due Date 02 April 2026.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2$ which for a normal distribution corresponds to a coverage probability of approximately 95 %. It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q26004618

F3-011-05/12-23

page 2 of 3

COPY



CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The table in the following gives the calibration results and associated measurement uncertainties of the measuring primary flow calibrator.

CALIBRATION DATA

PRIMARY FLOW CALIBRATOR RESULT

Nominal Value (cc/min)	STD Applied (cc/min)	DUC Reading (cc/min)	Correction (cc/min)	Uncertainty ± (cc/min)
0	0.000	0.000	0.000	-
50	50.000	49.508	+0.492	0.300
100	100.000	98.897	+1.103	0.300
200	200.00	197.81	+2.19	0.58
500	500.00	495.09	+4.91	1.43
1000	1000.00	991.68	+8.32	2.87
2000	2000.0	1987.2	+12.8	5.7
3000	3000.0	2985.5	+14.5	8.6
4000	4000.0	3983.1	+16.9	11.5
5000	5000.0	4981.3	+18.7	14.4

Technical Note. Media of Gas : Air

Setting Temperature 0 ° C ; Pressure 101.3 kPa

Note: The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 018 Page 52 of 73

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q26004618

F3-011-05/12-23

COPY



THERMO-HYGROMETER

Model : 608-H1

Serial No. : 45106737

CERTIFICATE OF CALIBRATION

Certificate No. : 25-090091

Sample Code : 25-39161-001

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapibarn 8 Rd., Nongkham,
Sriracha, Chonburi 20230

Location of Calibration : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited
(Calibration laboratory)

Equipment : Digital thermo-hygrometer

Manufacturer : testo Model : 608-H1

Serial No. : 45106737 ID No. : LABE 09/7

Date of Receipt : 21 May 2025 Date of Calibration : 23 May 2025

Condition of Calibration

1. Environment
- 1.1 Ambient temperature : 23.0 °C ± 3.0 °C
- 1.2 Relative humidity : 55.0 % ± 15.0 %

2. Calibration method

- 2.1 In-house method: WI-CL-045 By comparison with thermometer standard / chilled mirror hygrometer in controlled chamber.
- 2.2 The calibration by comparison unit under calibration (UUC) to the thermometer standard / chilled mirror hygrometer in a chamber at the controlled temperature / relative humidity.

3. Reference standard instrument

Instrument	Model	ID No.	Certificate No.	Due Date
3.1 Chilled Mirror	Optidew 401	LB-DP-03 & LB-DP-03 (DP)	TH-0122-24	25 September 2025
3.2 Digital Thermometer	Optidew 401	LB-DP-03 & LB-DP-03 (Temp.)	24-138856	28 October 2025
3.3 Digital Thermometer	34972A	LB-DA-07 with RTD-89	24-106857	21 August 2025

4. This certificate is traceable to the international system of unit (SI Unit).

- 4.1 Instrument No. 3.1 through National Institute of Metrology (Thailand).
- 4.2 Instrument No. 3.2 and 3.3 through Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by Miss Pornsuda Lohabal
Scientist

Approved by (Mr. Somchai Neampunt)
Signed for Director

Issue date 26 May 2025

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This Certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

REPORT OF CALIBRATION

Certificate No. : 25-090091

Sample Code : 25-39161-001

Results of Calibration

Temperature measurement

Resolution : 0.1 °C

Range : 0 °C to 50 °C

Calibration point °C	Average of standard reading		Unit under calibration		uncertainty °C
	Controlled humidity %RH	Temperature °C	Average reading °C	Correction value °C	
20	50	20.01	20.2	- 0.19	± 0.39
25	50	25.01	25.0	+ 0.01	± 0.39
30	50	30.01	30.0	+ 0.01	± 0.39

Humidity measurement

Resolution : 0.1 %RH

Range : 10 %RH to 95 %RH

Calibration point %RH	Average of standard reading		Unit under calibration		uncertainty %RH
	Air temperature °C	Calculated humidity %RH	Average reading %RH	Correction value %RH	
45	25.02	45.10	50.2	- 5.10	± 1.3
60	25.02	60.15	65.2	- 5.05	± 1.5
75	25.02	75.01	82.1	- 7.09	± 1.7

Notes

- Calibration results without adjustment.

The result expanded uncertainty of measurement (U) is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2.00$, which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

- End of Report -

COPY

UV/VIS SPECTROPHOTOMETER

Model : UV-1800

Serial No. : A11635101643 CD



Bara Scientific Co., Ltd.
968 U Chu Liang Building Floor7 Rama4 Road
Silom Bangrak Bangkok Thailand 10500
Tel : 02-6324300 Fax : 02-6375496-7
www.barascientific.com



Certificate of Calibration

Number of Page(s) 1 of 3

Certificate No. BSCC-UV-153/25
Equipment UV/Vis Spectrophotometer
Model UV-1800
Manufacturer Shimadzu
Serial No. A11635101643 CD
ID No. LABE 03/2
Date of receipt 21 April 2025
Date of calibration 21 April 2025
Date of issue 25 April 2025

Customer name Eastern Thai Consulting 1992 Co., Ltd

Address 683 Moo 11, Sukkaphibarn 8 Rd., Nongkham, Sriracha, Chonburi 20230

Temperature (24.7-26.8) °C (On site)
Humidity (36.9-46.2) %RH (On site)

Equipment condition Good Operation

Calibration Location Analysis Department

Calibration Procedure In-house method WI-UV-702-01 based on ASTM E275-01

Traceability Wavelength Accuracy is traceable to certificate No. 114485 and 114511
Photometric Accuracy is traceable to certificate No. 119612 and 114653
Stray Light is traceable to certificate No. 114484
The above certificate are traceable to SI unit through Starna Scientific Ltd.
(UKAS accredited calibration laboratory NO. 0659)

Calibrated by Mr.Phongpak Sontunchu

Approved by

Mr. Pannaphong Phanmekakul
Technical Manager

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate.
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced
except in full, without written approval of the Bara Scientific Co., Ltd



Bara Scientific Co., Ltd.
968 U Chu Liang Building Floor7 Rama4 Road
Silom Bangrak Bangkok Thailand 10500
Tel : 02-6324300 Fax : 02-6375496-7
www.barascientific.com



Certificate of Calibration

Certificate No. BSCC-UV-153/25

Number of Page(s) 2 of 3

Calibration Results:

1.Wavelength Accuracy

Certified Wavelength (nm)	UUC (nm)	Error (nm)	Uncertainty (±nm)
287.71	287.70	-0.01	0.18
445.82	445.87	0.05	0.18
536.52	536.52	0.00	0.18
741.02	741.05	0.03	0.18
879.41	879.33	-0.08	0.18

2.Photometric Accuracy (UV)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty (±A)
235	0.0000 0.7404	-0.0001 0.7416	-0.0001 0.0012	0.0075 0.0075
257	CNR CNR	CNR CNR	CNR CNR	CNR CNR
313	CNR CNR	CNR CNR	CNR CNR	CNR CNR
350	0.0000 0.6397	0.0000 0.6398	0.0000 0.0001	0.0075 0.0075

*CNR = Customer not request

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced
except in full, without written approval of the Bara Scientific Co., Ltd.



Bara Scientific

Bara Scientific Co., Ltd.

968 U Chu Liang Building Floor 7 Rama 4 Road
Siam Bangkok Bangkok Thailand 10500
Tel : 02-6324300 Fax : 02-6375496-7
www.barascientific.com



Certificate of Calibration

Certificate No. BSCC-UV-153/25

Number of Page(s)

3 of 3

Calibration Results:

3. Photometric Accuracy (Visible)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty ($\pm A$)
420.0	0.0000	0.0001	0.0001	0.0042
	0.5733	0.5712	-0.0021	0.0042
	0.7113	0.7097	-0.0016	0.0042
	1.0164	1.0150	-0.0014	0.0042
440.0	0.0000	0.0000	0.0000	0.0042
	0.5581	0.5559	-0.0022	0.0042
	0.6996	0.6975	-0.0021	0.0042
	1.0000	0.9984	-0.0016	0.0042
465.0	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
546.1	0.0000	0.0000	0.0000	0.0042
	0.5217	0.5202	-0.0015	0.0042
	0.6970	0.6947	-0.0023	0.0042
	0.9982	0.9969	-0.0013	0.0042
590.0	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
635.0	0.0000	0.0000	0.0000	0.0042
	0.5630	0.5620	-0.0010	0.0042
	0.7615	0.7594	-0.0021	0.0042
	1.0953	1.0943	-0.0010	0.0042

*CNR = Customer not request

4. Stray Light*

Standard	Unit Under Calibration(UUC)		
cut-off wavelength (nm)	Wavelength (nm)	Transmission (%T)	Absorbance (A)
201.10 $\pm$ 0.11nm	200.85	0.9740	2.0116

The Stray light transmission reference is less than 1.0%T and Stray light absorbance reference is greater than 2.00A

*Stray Light not NSC-ONSC Accredited.

The measurement uncertainty is base on a standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%.

End of Certificate

COPY

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate.
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced
except in full, without written approval of the Bara Scientific Co., Ltd.

SOUND LEVEL CALIBRATOR

MODEL : NC-75

SERIAL No. : 34802645



Cert. No. : ACC25065
Pages : 1 of 3

Calibration Certificate

Equipment : SOUND CALIBRATOR
Manufacturer : RION
Model : NC-75
Serial No.: 34802645
ID No.: -

Condition As Found : GOOD

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
SAHA GROUP INDUSTRIAL PARK, 683 MOO 11,
NONGKHAM, SIRACHA, CHONBURI 20230 THAILAND.

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 08 SEPTEMBER 2025
Calibration Date : 10 OCTOBER 2025
Date of Issue : 10 OCTOBER 2025

Calibrated by : Nathakorn Pisutpaisan

Approved by :
(Nitinun Srihawan)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACC25065
Job No. : VC68AC0181
Pages : 2 of 3

Calibration Procedure : CP-AC-03

Calibration Method :

This equipment was calibrated by follow on IEC-60942-2003 Standard.
The sound pressure level, frequency and total distortion of the sound calibrator was measured using the reference microphone.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EEL-BP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EEL-BP 23/0268	22-APR-26
Digital Multimeter	33461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KA1	34560495	AA-3002-25	19-FEB-26
Audio Analyzer	AVR-3360A	V744B6069	EF-0013-25	13-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :
- 3.1 National Institute of Metrology (Thailand).
 - 3.2 Thailand Institute of Scientific and Technological Research (TISTR).
 - 3.3 Electrical And Electronics Institute (EEL).

COPY

COPY

Cert. No. : ACC25065
Job No. : VC68AC0181
Pages : 3 of 3

Result of calibration :

1. Sound pressure level

Specified sound pressure level (dB)	Measured value (dB)	Deviated value (dB)	Uncertainty (dB)	Acceptance limit (dB)
94	93.98	-0.02	0.15	0.40

2. Frequency

Specified Frequency (Hz)	Measured value (Hz)	Deviated value (%)	Uncertainty (%)	Acceptance limit (%)
1000	1000.0	0.0	0.1	1.0

3. Total distortion

Measured value (%)	Uncertainty (%)	Acceptance limit (%)
0.46	0.10	3.0

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$
or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

COPY

SOUND LEVEL CALIBRATOR

MODEL : NC-75

SERIAL No. : 34745929



Cert. No. : ACC25046

Pages : 1 of 3

Calibration Certificate

Equipment : SOUND CALIBRATOR
Manufacturer : RION
Model : NC-75
Serial No.: 34745929
ID No.: -

Condition As Found : GOOD

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
SAHA GROUP INDUSTRIAL PARK, 683 MOO 11,
NONGKHAM, SIRACHA, CHONBURI 20230 THAILAND.

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 18 AUGUST 2025
Calibration Date : 01 SEPTEMBER 2025
Date of Issue : 02 SEPTEMBER 2025

Calibrated by : Nathakorn Pisutpaisan

Approved by : NITINUN S.
(Nitinun Srihawan)

Cert. No. : ACC25046

Job No. : VC68AC0165

Pages : 2 of 3

Calibration Procedure : CP-AC-03

Calibration Method :

This equipment was calibrated by follow on IEC-60942-2003 Standard.

The sound pressure level, frequency and total distortion of the sound calibrator was measured using the reference microphone.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EEL.BP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EEL.BP 23/0268	22-APR-26
Digital Multimeter	33461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KAI	34560495	AA-3002-25	19-FEB-26
Audio Analyzer	AVR-3360A	V744B6069	EF-0013-25	13-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

3.3 Electrical And Electronics Institute (EEI).

Cert. No. : ACC25046
Job No. : VC68AC0165
Pages : 3 of 3

Result of calibration :

1. Sound pressure level

Specified sound pressure level (dB)	Measured value (dB)	Deviated value (dB)	Uncertainty (dB)	Acceptance limit (dB)
94	93.95	-0.05	0.15	0.40

2. Frequency

Specified Frequency (Hz)	Measured value (Hz)	Deviated value (%)	Uncertainty (%)	Acceptance limit (%)
1000	1000.0	0.0	0.1	1.0

3. Total distortion

Measured value (%)	Uncertainty (%)	Acceptance limit (%)
0.58	0.10	3.0

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$
or any value following calculation, providing a level of confidence of approximately 95 %

----- **End of Calibration Certificate** -----

COPY

SOUND LEVEL METER

MODEL : NL-42A

SERIAL No. : 00322756



Cert. No. : ACL25181

Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42A / Microphone UC-52 / Preamplifier NH-24
Serial No.: 00322756 / 196480 / 15488
ID No.: -

Condition As Found : GOOD

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
SAHA GROUP INDUSTRIAL PARK, 683 MOO 11,
NONGKHAM, SIRACHA, CHONBURI 20230 THAILAND.

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 02 APRIL 2025
Calibration Date : 28 APRIL 2025
Date of Issue : 02 MAY 2025

Calibrated by : Nathakorn Pisutpaisan

Approved by :

T. Petchur
(Thanakul Petchurai)

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference
Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0011-25	11-FEB-26
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	34461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KA1	34560495	AA-3002-25	19-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Electrical And Electronics Institute (EEI).

T. Petchur
COPY

T. Petchur

Cert. No. : ACL25181
Job No. : VC68AC0077
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

Cert. No. : ACL25181
Job No. : VC68AC0077
Page : 4 of 8

Result of calibration :**1. Absolute sensitivity**

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise**2.1 Normal test**

Measured Value (dB)
14.2

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	10.8
C - weight	16.7
Flat	22.5

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			Acceptance Limits
	Flat	C-weight	A-weight	
125	0.5	0.5	0.5	± 1.5
1000	0.1	0.1	0.1	± 1.0
8000	0.0	0.1	0.1	± 5.0

COPY

T. Petch.

COPY

T. Petch.

Cert. No. : ACL25181
Job No. : VC68AC0077
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.1	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Lcq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.1	0.1	± 0.3

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	+ 1.1
136.0	136.0	0.0	+ 1.1
135.0	135.0	0.0	+ 1.1
134.0	134.0	0.0	+ 1.1
133.0	133.0	0.0	+ 1.1
132.0	132.0	0.0	+ 1.1
131.0	131.0	0.0	+ 1.1
129.0	129.0	0.0	+ 1.1
124.0	124.0	0.0	+ 1.1
119.0	119.0	0.0	+ 1.1
114.0	114.0	0.0	+ 1.1
109.0	109.0	0.0	+ 1.1
104.0	104.1	0.1	+ 1.1
99.0	99.0	0.0	+ 1.1
94.0	94.0	0.0	+ 1.1
89.0	89.0	0.0	+ 1.1
84.0	84.0	0.0	+ 1.1
79.0	79.0	0.0	+ 1.1
74.0	74.0	0.0	+ 1.1
69.0	69.0	0.0	+ 1.1
64.0	64.0	0.0	+ 1.1
59.0	59.0	0.0	+ 1.1
54.0	54.0	0.0	+ 1.1
49.0	49.0	0.0	+ 1.1
44.0	44.0	0.0	+ 1.1
39.0	39.0	0.0	+ 1.1
34.0	34.0	0.0	+ 1.1
30.0	29.9	-0.1	+ 1.1
29.0	29.0	0.0	+ 1.1
28.0	27.9	-0.1	+ 1.1
27.0	27.0	0.0	+ 1.1
26.0	25.9	-0.1	+ 1.1
25.0	24.9	-0.1	+ 1.1

Cert. No. : ACL25181
Job No. : VC68AC0077
Pages : 6 of 8

COPY

T. Petch

COPY

T. Petch

Cert. No. : ACL25181
Job No. : VC68AC0077
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	29.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	108.0	0.0	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.0 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

Cert. No. : ACL25181
Job No. : VC68AC0077
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.4	0.0	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	132.9	-0.1	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.5	0.0	±1.5

12. High level stability

Frequency Weighting	S1.M Display at initial (dB)	S1.M Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	136.9	137.0	-0.1	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$
or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

COPY

T. Retan.

COPY

T. Retan.

SOUND LEVEL METER

MODEL : NL-42A

SERIAL No. : 00222593

Cert. No. : ACL26004
Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42A / Microphone UC-52 / Preamplifier NH-24
Serial No.: 00222593 / 195906 / 15426
ID No.: -

Condition As Found : GOOD

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
SAHA GROUP INDUSTRIAL PARK, 683 MOO 11,
NONGKHAM, SIRACHA, CHONBURI 20230 THAILAND.

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 26 DECEMBER 2025
Calibration Date : 05 - 07 JANUARY 2026
Date of Issue : 07 JANUARY 2026

Calibrated by : Nathakorn Pisutpaisan

Approved by :
(Nitinun Srihawan)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL26004
Job No. : VC69AC0048
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC 61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For test results of each items were made by observation of each instrument's display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0011-25	11-FEB-26
Waveform Generator	33511B	MY52402742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EF-JBP 24/0263	22-APR-26
Digital Multimeter	33461A	MY53220076	EF-JBP 23/0268	22-APR-26
Digital Multimeter	34461A	MY60024273	CA20251201A	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	7977900	AA-1902-25	19-FEB-26
Measuring Amplifier	NA-42KA1	34560495	AA-3002-25	19-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only

3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand)
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).
- 3.3 Electrical And Electronics Institute (EEI).

COPY

COPY

Cert. No. : ACL26004
Job No. : VC69AC0048
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
14.2

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	9.9
C - weight	16.6
Flat	22.3

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.3	0.3	0.3	± 1.5
1000	0.1	0.1	0.1	± 1.0
8000	0.8	0.8	0.8	± 5.0

Cert. No. : ACL26004
Job No. : VC69AC0048
Page : 4 of 8

COPY

COPY

Cert. No. : ACL26004
Job No. : VC69AC0048
Pages : 5 of 8

Cert. No. : ACL26004
Job No. : VC69AC0048
Pages : 6 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	-0.1	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
f.cq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.1	0.1	± 1.1
29.0	29.1	0.1	± 1.1
28.0	28.0	0.0	± 1.1
27.0	27.1	0.1	± 1.1
26.0	26.1	0.1	± 1.1
25.0	25.1	0.1	± 1.1

Cert. No. : ACL26004
Job No. : VC69AC0048
Pages : 7 of 8

Cert. No. : ACL26004
Job No. : VC69AC0048
Pages : 8 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	28.8	-0.2	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, T ₀ (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.0 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

10. Peak C sound level

Number of cycle or test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.4	0.0	±3.0

Number of cycle or test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±3.0
Positive half cycle	135.4	135.3	-0.2	±3.0
Negative half cycle	135.4	135.2	-0.2	±3.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one half cycle	Negative one half cycle	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ to give a 95% probability of the true value falling within the stated limits, providing a level of confidence of approximately 95%.

End of Calibration Certificate

COPY

COPY

SOUND LEVEL METER

MODEL : NL-42A

SERIAL No. : 00322748



Cert. No. : ACL26009
Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42A / Microphone MK 216 / Preamplifier NH-24
Serial No.: 00322748 / 412753E / 15480
ID No.: -

Condition As Found : GOOD

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
SAHA GROUP INDUSTRIAL PARK, 683 MOO 11,
NONGKHAM, SIRACHA, CHONBURI 20230 THAILAND.

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 26 DECEMBER 2025
Calibration Date : 05 - 07 JANUARY 2026
Date of Issue : 07 JANUARY 2026

Calibrated by : Nathakorn Pisutpaisan

Approved by :
(Nitinun Srihawan)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL26009
Job No. : VC69AC0048
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :
This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
The test results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0011-25	11-FEB-26
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EEI-BIP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EEI-BIP 23/0268	22-APR-26
Digital Multimeter	34461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KA1	34560495	AA-3007-25	19-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :
- 3.1 National Institute of Metrology (Thailand).
 - 3.2 Thailand Institute of Scientific and Technological Research (TISTR).
 - 3.3 Electrical And Electronics Institute (EEI).

COPY

COPY

Cert. No. : ACL26009
Job No. : VC69AC0048
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

COPY

Cert. No. : ACL26009
Job No. : VC69AC0048
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
15.3

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	7.8
C - weight	15.0
Flat	20.7

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.6	0.6	0.6	± 1.5
1000	0.2	0.1	0.1	± 1.0
8000	-3.1	-3.1	-3.1	±5.0

COPY

Cert. No. : ACL26009
Job No. : VC69AC0048
Pages : 5 of 8

Cert. No. : ACL26009
Job No. : VC69AC0048
Pages : 6 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	53.9	-0.1	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	38.9	-0.1	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	27.0	0.0	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	25.0	0.0	± 1.1

COPY

COPY

Cert. No. : ACL26009
Job No. : VC69AC0048
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	29.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.0 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

Cert. No. : ACL26009
Job No. : VC69AC0048
Pages : 8 of 8

10. Peak 4' sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{epk} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle	0.0	±1.5
89.5	89.5		

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$
or any value following calculation, providing a level of confidence of approximately 95 %

COPY

End of Calibration Certificate

COPY

SOUND LEVEL METER

MODEL : NL-42A

SERIAL No. : 00322751



Cert. No. : ACL26117

Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42A / Microphone UC-52 / Preamplifier NH-24
Serial No.: 00322751 / 196474 / 15483
ID No.: -

Condition As Found : GOOD

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
SAHA GROUP INDUSTRIAL PARK, 683 MOO 11,
NONGKHAM, SIRACHA, CHONBURI 20230 THAILAND.

Location : -
Ambient Temperature : (23.0 $\pm$ 3) °C
Pressure : (101.3 $\pm$ 3) kPa
Relative Humidity : (50.0 $\pm$ 20) %

Received Date : 07 JANUARY 2026
Calibration Date : 30 JANUARY 2026
Date of Issue : 02 FEBRUARY 2026

Calibrated by : Nathakorn Pisutpaisan

Approved by :

(Nitinun Srihawan)

COPY

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL26117

Job No. : VC694C0048

Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0011-25	11-FEB-26
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EEL.BP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EEL.BP 23/0268	22-APR-26
Digital Multimeter	34461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KAJ	34560495	AA-3002-25	19-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).
- 3.3 Electrical And Electronics Institute (EEI).

COPY

Cert. No. : ACL26117
Job No. : VC69AC0048
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
14.2

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	10.8
C - weight	17.3
Flat	23.0

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.2	0.2	0.3	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	-0.4	-0.3	-0.3	±5.0

Cert. No. : ACL26117
Job No. : VC69AC0048
Page : 4 of 8

COPY

COPY

Cert. No. : ACL26117
Job No. : VC69AC0048
Pages : 5 of 8

Cert. No. : ACL26117
Job No. : VC69AC0048
Pages : 6 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	53.9	-0.1	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	38.9	-0.1	± 1.1
34.0	34.0	0.0	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	26.9	-0.1	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.9	-0.1	± 1.1

COPY

Cert. No. : ACL26117
Job No. : VC69AC0048
Pages : 7 of 8

Cert. No. : ACL26117
Job No. : VC69AC0048
Pages : 8 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	28.9	-0.1	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	+1.0
Slow	2	8	108.0	108.0	0.0	1.0 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	+1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lepeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.6	89.6	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A-weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

SOUND LEVEL METER

MODEL : NL-42A

SERIAL No. : 00322752

Cert. No. : ACL25266

Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42A / Microphone UC-52 / Preamplifier NH-24
Serial No.: 00322752 / 196475 / 15484
ID No.: -

Condition As Found : GOOD

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
SAHA GROUP INDUSTRIAL PARK, 683 MOO 11,
NONGKHAM, SIRACHA, CHONBURI 20230 THAILAND.

Location : -
Ambient Temperature : (23.0 $\pm$ 3) °C
Pressure : (101.3 $\pm$ 3) kPa
Relative Humidity : (50.0 $\pm$ 20) %

Received Date : 26 JUNE 2025
Calibration Date : 08 JULY 2025
Date of Issue : 09 JULY 2025

Calibrated by : Nathakorn Pisutpaisan

Approved by :

Wichok E.
(Wichok Ekpongpradit)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL25266

Job No. : VC68AC0096

Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0011-25	11-FEB-26
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EEL.BP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EEL.BP 23/0268	22-APR-26
Digital Multimeter	34461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KAI	34560495	AA-3002-25	19-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

3.3 Electrical And Electronics Institute (EEI).

COPY

Wichok

Cert. No. : ACL25266
Job No. : VC68AC009
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

Cert. No. : ACL25266
Job No. : VC68AC0096
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
17.50000003

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	13.6
C - weight	20.1
Flat	25.8

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	-0.3	-0.3	-0.3	± 1.5
1000	-0.3	-0.3	-0.3	± 1.0
8000	0.8	0.9	0.9	±5.0

COPY

Michael J

COPY

Michael J

Cert. No. : ACL25266
Job No. : VC68AC009
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.1	-0.1	±2.0
125	0.0	0.0	-0.1	±1.5
250	0.0	0.0	-0.1	±1.5
500	0.0	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	132.9	-0.1	± 1.1
132.0	131.9	-0.1	± 1.1
131.0	130.9	-0.1	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.1	0.1	± 1.1
30.0	30.1	0.1	± 1.1
29.0	29.2	0.2	± 1.1
28.0	28.2	0.2	± 1.1
27.0	27.3	0.3	± 1.1
26.0	26.3	0.3	± 1.1
25.0	25.4	0.4	± 1.1

Cert. No. : ACL25266
Job No. : VC68AC009
Pages : 6 of 8

Cert. No. : ACL25266
Job No. : VC68AC009
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	29.1	0.1	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.0 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

Cert. No. : ACL25266
Job No. : VC68AC009
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.4	0.0	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.5	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$
or any value following calculation, providing a level of confidence of approximately 95 %

COPY

micron B

End of Calibration Certificate

COPY

SOUND LEVEL METER

MODEL : NL-42A

SERIAL No. : 00322749



Cert. No. : ACL26010

Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42A / Microphone UC-52 / Preamplifier NH-24
Serial No.: 00322749 / 196472 / 15481
ID No.: -


Condition As Found : GOOD

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
SAHA GROUP INDUSTRIAL PARK, 683 MOO 11,
NONGKHAM, SIRACHA, CHONBURI 20230 THAILAND.

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 26 DECEMBER 2025
Calibration Date : 05 - 07 JANUARY 2026
Date of Issue : 07 JANUARY 2026

Calibrated by : Nathakorn Pisutpaisan

Approved by : 
(Nitinun Srihawan)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL26010

Job No. : VC69AC0048

Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0011-25	11-FEB-26
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EEL-BP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EEL-BP 23/0268	22-APR-26
Digital Multimeter	34461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KA1	34560495	AA-3002-25	19-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).
- 3.3 Electrical And Electronics Institute (EEL).

COPY

COPY

Cert. No. : ACL26010
Job No. : VC69AC0048
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

Cert. No. : ACL26010
Job No. : VC69AC0048
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
13.8

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	10.8
C - weight	16.8
Flat	22.3

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.3	0.3	0.3	± 1.5
1000	0.1	0.1	0.1	± 1.0
8000	0.5	0.6	0.6	±5.0

COPY

COPY

Cert. No. : ACL26010
Job No. : VC69AC0048
Pages : 5 of 8

Cert. No. : ACL26010
Job No. : VC69AC0048
Pages : 6 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.1	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	-0.1	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.1	0.1	± 1.1
30.0	30.1	0.1	± 1.1
29.0	29.0	0.0	± 1.1
28.0	28.1	0.1	± 1.1
27.0	27.1	0.1	± 1.1
26.0	26.1	0.1	± 1.1
25.0	25.1	0.1	± 1.1

Cert. No. : ACL26010
Job No. : VC69AC0048
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	28.9	-0.1	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.0 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

Cert. No. : ACL26010
Job No. : VC69AC0048
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.6	0.0	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	+2.0
Positive half cycle	135.4	135.2	-0.2	+2.0
Negative half cycle	135.4	135.2	-0.2	+2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle	0.0	±1.5
89.5	89.5		

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor k or any value following calculation, providing a level of confidence of approximately 95 %

COPY

End of Calibration Certificate

COPY

SOUND LEVEL METER

MODEL : NL-52A

SERIAL No. : 00230987



Cert. No. : ACL26120

Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-52A / Microphone UC-59 / Preamplifier NH-25
Serial No.: 00230987 / 21950 / 22333
ID No.: -

Condition As Found : GOOD

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
SAHA GROUP INDUSTRIAL PARK, 683 MOO 11,
NONGKHAM, SIRACHA, CHONBURI 20230 THAILAND.

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 07 JANUARY 2026
Calibration Date : 30 JANUARY 2026
Date of Issue : 02 FEBRUARY 2026

Calibrated by : Nathakorn Pisutpaisan

Approved by :

(Nitinun Srihawan)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL26120

Job No. : VC69AC0049

Pages : 2 of 8

Calibration Procedure : CP-AC-02

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0011-25	11-FEB-26
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EELBP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EELBP 23/0268	22-APR-26
Digital Multimeter	34461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KA1	34560495	AA-3002-25	19-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).
- 3.3 Electrical And Electronics Institute (EEI).

COPY

COPY

Cert. No. : ACL26120
Job No. : VC69AC0049
Pages : 3 of 8

Cert. No. : ACL26120
Job No. : VC69AC0049
Page : 4 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.3
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	94.0	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
15.8

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	10.8
C - weight	15.3
Flat	20.5

3. Acoustical signal tests of frequency weightings:

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.3	0.3	0.3	± 1.0
1000	0.2	0.1	0.2	± 0.7
8000	0.1	0.1	0.2	+ 1.5, - 2.5

COPY

COPY

Cert. No. : ACL26120

Job No. : VC69AC0049

Pages : 5 of 8

Cert. No. : ACL26120

Job No. : VC69AC0049

Pages : 6 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response error (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	-0.1	0.0	±1.0
125	0.0	0.0	0.0	±1.0
250	0.0	0.0	0.0	±1.0
500	0.0	0.0	0.0	±1.0
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±1.0
4000	0.0	0.0	0.0	±1.0
8000	0.0	0.1	0.1	+1.5, -1.5
16000	0.0	-1.2	-1.2	+2.5, -16.0

5. Frequency and time weightings at 1 kHz**5.1 Frequency weightings at 1 kHz**

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.1

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	±0.8
136.0	136.0	0.0	±0.8
135.0	135.0	0.0	±0.8
134.0	134.0	0.0	±0.8
133.0	133.0	0.0	±0.8
132.0	132.0	0.0	±0.8
131.0	131.0	0.0	±0.8
129.0	129.0	0.0	±0.8
124.0	124.0	0.0	±0.8
119.0	119.0	0.0	±0.8
114.0	114.0	0.0	±0.8
109.0	109.0	0.0	±0.8
104.0	104.0	0.0	±0.8
99.0	99.0	0.0	±0.8
94.0	94.0	0.0	±0.8
89.0	89.0	0.0	±0.8
84.0	84.0	0.0	±0.8
79.0	78.9	-0.1	±0.8
74.0	74.0	0.0	±0.8
69.0	69.0	0.0	±0.8
64.0	63.9	-0.1	±0.8
59.0	59.0	0.0	±0.8
54.0	53.9	-0.1	±0.8
49.0	48.9	-0.1	±0.8
44.0	43.9	-0.1	±0.8
39.0	38.9	-0.1	±0.8
34.0	34.0	0.0	±0.8
30.0	30.0	0.0	±0.8
29.0	29.0	0.0	±0.8
28.0	28.0	0.0	±0.8
27.0	27.0	0.0	±0.8
26.0	26.0	0.0	±0.8
25.0	24.9	-0.1	±0.8

Cert. No. : ACL26120
Job No. : VC69AC0049
Pages : 7 of 8

Cert. No. : ACL26120
Job No. : VC69AC0049
Pages : 8 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±0.3

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	28.8	-0.2	±0.8

9. Tone burst response

Time Weighting	Tone burst duration, T _b (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.0 ; -3.0
	2	8	117.0	117.0	0.0	1.0 ; -1.5
	200	800	134.0	134.0	0.0	±0.5
Slow	2	8	108.0	108.0	0.0	1.0 ; -3.0
	200	800	127.6	127.6	0.0	±0.5
SEL	0.25	1	99.0	98.9	-0.1	1.0 ; -3.0
	2	8	108.0	108.0	0.0	1.0 ; -1.5
	200	800	128.0	128.0	0.0	±0.5

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±2.0
One	133.4	133.3	-0.1	±2.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±1.0
Positive half cycle	135.4	135.2	-0.2	±1.0
Negative half cycle	135.4	135.2	-0.2	±1.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.6	89.5	-0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.1

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor k or any value following calculation, providing a level of confidence of approximately 95 %

COPY

End of Calibration Certificate

COPY

SOUND LEVEL METER

MODEL : NL-52A

SERIAL No. : 00230993



Cert. No. : ACL26025

Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-52A / Microphone UC-59 / Preamplifier NH-25
Serial No.: 00230993 / 22776 / 22429
ID No.: -

Condition As Found : GOOD

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
SAHA GROUP INDUSTRIAL PARK, 683 MOO 11,
NONGKHAM, SIRACHA, CHONBURI 20230 THAILAND.

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 26 DECEMBER 2025
Calibration Date : 05 - 07 JANUARY 2026
Date of Issue : 07 JANUARY 2026

Calibrated by : Nathakorn Pisutpaisan

Approved by :

(Nitinun Srihawan)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL26025

Job No. : VC69AC0048

Pages : 2 of 8

Calibration Procedure : CP-AC-02

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0011-25	11-FEB-26
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EEL-BP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EEL-BP 23/0268	22-APR-26
Digital Multimeter	34461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KAI	34560495	AA-3002-25	19-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).
- 3.3 Electrical And Electronics Institute (EEI).

COPY

Cert. No. : ACL26025
Job No. : VC69AC0048
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

Result of calibration :**1. Absolute sensitivity**

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	94.0	0.0	±0.3

2. Self-generated noise**2.1 Normal test**

Measured Value (dB)
17.2

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	12.0
C - weight	15.2
Flat	22.2

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.2	0.2	0.3	± 1.0
1000	0.3	0.3	0.3	± 0.7
8000	0.6	0.5	0.6	± 1.5, ± 2.5

COPY

COPY

Cert. No. : ACL26025
Job No. : VC69AC0048
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.1	0.0	0.0	±1.0
125	0.0	0.0	0.0	±1.0
250	0.0	0.0	0.0	±1.0
500	0.0	0.0	0.0	±1.0
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±1.0
4000	0.0	0.0	0.0	±1.0
8000	0.0	0.1	0.1	+ 1.5, - 2.5
16000	0.0	-1.2	-1.2	+ 2.5, -16.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	+ 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.1

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	±0.8
136.0	136.0	0.0	±0.8
135.0	135.0	0.0	±0.8
134.0	134.0	0.0	±0.8
133.0	133.0	0.0	±0.8
132.0	132.0	0.0	±0.8
131.0	131.0	0.0	±0.8
129.0	129.0	0.0	±0.8
124.0	124.0	0.0	±0.8
119.0	119.0	0.0	±0.8
114.0	114.0	0.0	±0.8
109.0	109.0	0.0	±0.8
104.0	104.0	0.0	±0.8
99.0	99.0	0.0	±0.8
94.0	94.0	0.0	±0.8
89.0	89.0	0.0	±0.8
84.0	84.0	0.0	±0.8
79.0	79.0	0.0	±0.8
74.0	74.0	0.0	±0.8
69.0	69.0	0.0	±0.8
64.0	64.0	0.0	±0.8
59.0	59.0	0.0	±0.8
54.0	53.9	-0.1	±0.8
49.0	49.0	0.0	±0.8
44.0	43.9	-0.1	±0.8
39.0	38.9	-0.1	±0.8
34.0	34.0	0.0	±0.8
30.0	30.0	0.0	±0.8
29.0	29.0	0.0	±0.8
28.0	28.0	0.0	±0.8
27.0	26.9	-0.1	±0.8
26.0	26.0	0.0	±0.8
25.0	24.9	-0.1	±0.8

Cert. No. : ACL26025
Job No. : VC69AC0048
Pages : 6 of 8

Cert. No. : ACL26025
Job No. : VC69AC0048
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	± 0.8

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	29.0	0.0	± 0.8

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.0 ; -3.0
	2	8	117.0	117.0	0.0	1.0 ; -1.5
	200	800	134.0	134.0	0.0	± 0.5
Slow	2	8	108.0	108.0	0.0	1.0 ; -3.0
	200	800	127.6	127.6	0.0	± 0.5
SEL	0.25	1	99.0	98.9	-0.1	1.0 ; -3.0
	2	8	108.0	108.0	0.0	1.0 ; -1.5
	200	800	128.0	128.0	0.0	± 0.5

10. Peak C sound level

Number of cycle m test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	± 2.0
One	133.4	133.3	-0.1	± 2.0

Number of cycle m test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	± 1.0
Positive half cycle	135.4	135.2	-0.2	± 1.0
Negative half cycle	135.4	135.2	-0.2	± 1.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle	Value (dB)	Limits (dB)
89.6	89.6		
		0.0	± 1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	± 0.1

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$
or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

COPY

COPY

SOUND LEVEL METER

MODEL : NL-52A

SERIAL No. : 01120947

Cert. No. : ACL26118
Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-52A / Microphone UC-52 / Preamplifier NH-24
Serial No.: 01120947 / 196478 / 15487
ID No.: -

Condition As Found : GOOD

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
SAHA GROUP INDUSTRIAL PARK, 683 MOO 11,
NONGKHAM, SIRACHA, CHONBURI 20230 THAILAND.

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 07 JANUARY 2026
Calibration Date : 30 JANUARY 2026
Date of Issue : 02 FEBRUARY 2026

Calibrated by : Nathakorn Pisutpaisan

Approved by :

(Nitinun Sribawan)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced
other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL26118
Job No. : VC69AC0049
Pages : 2 of 8

Calibration Procedure : CP-AC-02

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference
Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0011-25	11-FEB-26
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EEL-BP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EEL-BP 23/0268	22-APR-26
Digital Multimeter	34461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KAI	34560495	AA-3002-25	19-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).
- 3.3 Electrical And Electronics Institute (EEI).

Cert. No. : ACL26118
Job No. : VC69AC0049
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	94.0	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
17.2

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	14.6
C - weight	20.3
Flat	26.1

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.4	0.4	0.5	± 1.0
1000	0.1	0.1	0.2	± 0.7
8000	0.5	0.5	0.5	+ 1.5, - 2.5

Cert. No. : ACL26118
Job No. : VC69AC0049
Page : 4 of 8

COPY

COPY

Cert. No. : ACL26118
Job No. : VC69AC0049
Pages : 5 of 8

Cert. No. : ACL26118
Job No. : VC69AC0049
Pages : 6 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.1	-0.1	±1.0
125	0.0	0.0	0.0	±1.0
250	0.0	0.0	-0.1	±1.0
500	0.0	0.0	-0.1	±1.0
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±1.0
4000	0.0	0.0	0.0	±1.0
8000	0.0	0.0	0.0	+ 1.5, - 2.5
16000	0.0	-1.2	-1.2	+ 2.5, -16.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.1

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	±0.8
136.0	136.0	0.0	±0.8
135.0	135.1	0.1	±0.8
134.0	134.1	0.1	±0.8
133.0	133.0	0.0	±0.8
132.0	132.0	0.0	±0.8
131.0	131.0	0.0	±0.8
129.0	129.1	0.1	±0.8
124.0	124.0	0.0	±0.8
119.0	119.1	0.1	±0.8
114.0	114.1	0.1	±0.8
109.0	109.1	0.1	±0.8
104.0	104.1	0.1	±0.8
99.0	99.1	0.1	±0.8
94.0	94.0	0.0	±0.8
89.0	89.0	0.0	±0.8
84.0	84.0	0.0	±0.8
79.0	79.0	0.0	±0.8
74.0	74.0	0.0	±0.8
69.0	69.0	0.0	±0.8
64.0	64.0	0.0	±0.8
59.0	59.0	0.0	±0.8
54.0	54.0	0.0	±0.8
49.0	49.0	0.0	±0.8
44.0	44.0	0.0	±0.8
39.0	39.0	0.0	±0.8
34.0	34.0	0.0	±0.8
30.0	30.1	0.1	±0.8
29.0	29.2	0.2	±0.8
28.0	28.2	0.2	±0.8
27.0	27.3	0.3	±0.8
26.0	26.4	0.4	±0.8
25.0	25.5	0.5	±0.8

Cert. No. : ACL26118
Job No. : VC69AC0049
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±0.8

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	29.2	0.2	±0.8

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.0 ; -3.0
	2	8	117.0	116.9	-0.1	1.0 ; -1.5
	200	800	134.0	134.0	0.0	±0.5
Slow	2	8	108.0	108.0	0.0	1.0 ; -3.0
	200	800	127.6	127.6	0.0	±0.5
SEL	0.25	1	99.0	98.9	-0.1	1.0 ; -3.0
	2	8	108.0	108.0	0.0	1.0 ; -1.5
	200	800	128.0	128.0	0.0	±0.5

Cert. No. : ACL26118
Job No. : VC69AC0049
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±2.0
One	133.4	133.4	0.0	±2.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±1.0
Positive half cycle	135.4	135.1	-0.3	±1.0
Negative half cycle	135.4	135.1	-0.3	±1.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.6	0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.1

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$
or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

SOUND LEVEL METER

MODEL : NL-52A

SERIAL No. : 01120950

Cert. No. : ACL26067

Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-52A / Microphone UC-59 / Preamplifier NH-25
Serial No.: 01120950 / 22043 / 22339
ID No.: -

Condition As Found : GOOD

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
SAHA GROUP INDUSTRIAL PARK, 683 MOO 11,
NONGKHAM, SIRACHA, CHONBURI 20230 THAILAND.

Location : -
Ambient Temperature : (23.0 $\pm$ 3) °C
Pressure : (101.3 $\pm$ 3) kPa
Relative Humidity : (50.0 $\pm$ 20) %

Received Date : 26 DECEMBER 2025
Calibration Date : 19 - 21 JANUARY 2026
Date of Issue : 22 JANUARY 2026

Calibrated by : Nathakorn Pisutpaisan

Approved by :

(Nitinun Srihawan)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL26067

Job No. : VCS9ACUM000

Pages : 2 of 8

Calibration Procedure : CP-AC-02

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0011-25	11-FEB-26
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EELBP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EELBP 23/0268	22-APR-26
Digital Multimeter	34461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KAJ	34560495	AA-3002-25	19-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).
- 3.3 Electrical And Electronics Institute (EEI).

COPY

COPY

Cert. No. : ACL26067
Job No. : VC69AC0048
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

Result of calibration :**1. Absolute sensitivity**

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	94.0	0.0	±0.3

2. Self-generated noise**2.1 Normal test**

Measured Value (dB)
20.00000003

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	17.0
C - weight	26.4
Flat	29.6

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	-0.3	-0.2	-0.2	± 1.0
1000	0.0	0.0	0.0	± 0.7
8000	1.0	1.0	1.1	± 1.5, ± 2.5

COPY

COPY

Cert. No. : ACL26067
Job No. : VC69AC0048
Pages : 5 of 8

Cert. No. : ACL26067
Job No. : VC69AC0048
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.2	-0.2	-0.2	±1.0
125	-0.3	-0.3	-0.3	±1.0
250	-0.1	-0.1	-0.1	±1.0
500	0.0	0.0	0.0	±1.0
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±1.0
4000	0.0	0.1	0.1	±1.0
8000	0.1	0.1	0.1	+ 1.5, - 2.5
16000	0.1	-1.1	-1.1	+ 2.5, -16.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.1

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	±0.8
136.0	136.1	0.1	±0.8
135.0	135.1	0.1	±0.8
134.0	134.1	0.1	±0.8
133.0	133.0	0.0	±0.8
132.0	132.0	0.0	±0.8
131.0	131.0	0.0	±0.8
129.0	129.1	0.1	±0.8
124.0	124.0	0.0	±0.8
119.0	119.1	0.1	±0.8
114.0	114.1	0.1	±0.8
109.0	109.1	0.1	±0.8
104.0	104.1	0.1	±0.8
99.0	99.1	0.1	±0.8
94.0	94.0	0.0	±0.8
89.0	89.0	0.0	±0.8
84.0	84.0	0.0	±0.8
79.0	79.0	0.0	±0.8
74.0	74.0	0.0	±0.8
69.0	69.0	0.0	±0.8
64.0	64.0	0.0	±0.8
59.0	59.0	0.0	±0.8
54.0	54.0	0.0	±0.8
49.0	49.0	0.0	±0.8
44.0	44.0	0.0	±0.8
39.0	39.0	0.0	±0.8
34.0	34.1	0.1	±0.8
30.0	30.2	0.2	±0.8
29.0	29.2	0.2	±0.8
28.0	28.3	0.3	±0.8
27.0	27.3	0.3	±0.8
26.0	26.3	0.3	±0.8
25.0	25.3	0.3	±0.8

Cert. No. : ACL26067
Job No. : VC69AC0048
Pages : 7 of 8

Cert. No. : ACL26067
Job No. : VC69AC0048
Pages : 8 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±0.8

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	29.2	0.2	±0.8

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.0 ; -3.0
	2	8	117.0	116.9	-0.1	1.0 ; -1.5
	200	800	134.0	134.0	0.0	±0.5
Slow	2	8	108.0	107.9	-0.1	1.0 ; -3.0
	200	800	127.6	127.6	0.0	±0.5
SEL	0.25	1	99.0	98.8	-0.2	1.0 ; -3.0
	2	8	108.0	107.9	-0.1	1.0 ; -1.5
	200	800	128.0	128.0	0.0	±0.5

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±2.0
One	133.4	133.4	0.0	±2.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±1.0
Positive half cycle	135.4	134.8	-0.6	±1.0
Negative half cycle	135.4	134.8	-0.6	±1.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.6	89.6	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.1

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

SOUND LEVEL METER

MODEL : NL-52A

SERIAL No. : 01120944



Cert. No. : ACL26016

Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-52A / Microphone UC-59 / Preamplifier NH-25
Serial No.: 01120944 / 22221 / 22423
ID No.: -

Condition As Found : GOOD

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
SAHA GROUP INDUSTRIAL PARK, 683 MOO 11,
NONGKHAM, SIRACHA, CHONBURI 20230 THAILAND.

Location : -
Ambient Temperature : (23.0 $\pm$ 3) °C
Pressure : (101.3 $\pm$ 3) kPa
Relative Humidity : (50.0 $\pm$ 20) %

Received Date : 26 DECEMBER 2025
Calibration Date : 05 - 07 JANUARY 2026
Date of Issue : 07 JANUARY 2026

Calibrated by : Nathakorn Pisutpaisan

Approved by :

(Nitinun Srihawan)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL26016

Job No. : VC69AC0048

Pages : 2 of 8

Calibration Procedure : CP-AC-02

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0011-25	11-FEB-26
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EEL.BP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EEL.BP 23/0268	22-APR-26
Digital Multimeter	34461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KAI	34560495	AA-3002-25	19-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

3.3 Electrical And Electronics Institute (EEI).

Cert. No. : ACL26016
Job No. : VC69AC0048
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

Cert. No. : ACL26016
Job No. : VC69AC0048
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	94.0	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
14.6

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	9.9
C - weight	14.7
Flat	20.5

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.0	0.0	0.1	± 1.0
1000	0.1	0.0	0.1	± 0.7
8000	0.8	0.8	0.9	+ 1.5, - 2.5

COPY

COPY

Cert. No. : ACL26016
Job No. : VC69AC0048
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	-0.1	0.0	±1.0
125	0.0	0.0	0.0	±1.0
250	0.0	0.0	-0.1	±1.0
500	0.0	0.0	-0.1	±1.0
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±1.0
4000	0.0	0.0	0.0	±1.0
8000	0.0	0.0	0.1	+ 1.5, - 2.5
16000	0.0	-1.2	-1.2	+ 2.5, -16.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	+ 0.1
Slow	94.0	94.0	0.0	+ 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.1

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	±0.8
136.0	136.0	0.0	±0.8
135.0	135.0	0.0	±0.8
134.0	134.0	0.0	±0.8
133.0	132.9	-0.1	±0.8
132.0	131.9	-0.1	±0.8
131.0	130.9	-0.1	±0.8
129.0	129.0	0.0	±0.8
124.0	124.0	0.0	±0.8
119.0	119.0	0.0	±0.8
114.0	114.0	0.0	±0.8
109.0	109.0	0.0	±0.8
104.0	104.0	0.0	±0.8
99.0	99.0	0.0	±0.8
94.0	94.0	0.0	±0.8
89.0	89.0	0.0	±0.8
84.0	84.0	0.0	±0.8
79.0	79.0	0.0	±0.8
74.0	74.0	0.0	±0.8
69.0	69.0	0.0	±0.8
64.0	64.0	0.0	±0.8
59.0	59.0	0.0	±0.8
54.0	54.0	0.0	±0.8
49.0	49.0	0.0	±0.8
44.0	44.0	0.0	±0.8
39.0	39.0	0.0	±0.8
34.0	34.0	0.0	±0.8
30.0	30.0	0.0	±0.8
29.0	29.0	0.0	±0.8
28.0	28.0	0.0	±0.8
27.0	26.9	-0.1	±0.8
26.0	26.0	0.0	±0.8
25.0	25.0	0.0	±0.8

Cert. No. : ACL26016
Job No. : VC69AC0048
Pages : 6 of 8

COPY

Cert. No. : ACL26016
Job No. : VC69AC0048
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±0.8

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	29.0	0.0	±0.8

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.0 ; -3.0
	2	8	117.0	117.0	0.0	1.0 ; -1.5
	200	800	134.0	134.0	0.0	±0.5
Slow	2	8	108.0	108.0	0.0	1.0 ; -3.0
	200	800	127.6	127.6	0.0	±0.5
SEL	0.25	1	99.0	98.9	-0.1	1.0 ; -3.0
	2	8	108.0	108.0	0.0	1.0 ; -1.5
	200	800	128.0	128.0	0.0	±0.5

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±2.0
One	133.4	133.4	0.0	±2.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±1.0
Positive half cycle	135.4	135.2	-0.2	±1.0
Negative half cycle	135.4	135.2	-0.2	±1.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.5	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.1

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$
or any value following calculation, providing a level of confidence of approximately 95 %.

End of Calibration Certificate

COPY

COPY

SOUND LEVEL METER

MODEL : NL-43

SERIAL No. : 00641700

Cert. No. : ACL25306

Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-43 / Microphone UC-52 / Preamplifier NH-24
Serial No.: 00641700 / 206298 / 34664
ID No.: -


Condition As Found : GOOD

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
SAHA GROUP INDUSTRIAL PARK, 683 MOO 11,
NONGKHAM, SIRACHA, CHONBURI 20230 THAILAND.

Location : -
Ambient Temperature : (23.0 $\pm$ 3) °C
Pressure : (101.3 $\pm$ 3) kPa
Relative Humidity : (50.0 $\pm$ 20) %

Received Date : 23 JUNE 2025
Calibration Date : 13 - 14 AUGUST 2025
Date of Issue : 15 AUGUST 2025

Calibrated by : Nathakorn Pisutpaisan

Approved by : 
(Wichok Ekpongpradit)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL25306

Job No. : VC68AC0160

Pages : 2 of 8

Calibration Procedure : CP-AC-02

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (S.L.M).
The S.L.M had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with S.L.M's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0011-25	11-FEB-26
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EEL-BP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EEL-BP 23/0268	22-APR-26
Digital Multimeter	34461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KA1	34560495	AA-3002-25	19-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).
- 3.3 Electrical And Electronics Institute (EEI).

COPY

Cert. No. : ACL25306
Job No. : VC68AC0160
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

Cert. No. : ACL25306
Job No. : VC68AC0160
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
15.1

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	12.6
C - weight	17.8
Flat	23.7

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.4	0.4	0.4	± 1.5
1000	0.2	0.2	0.2	± 1.0
8000	-0.1	-0.1	-0.1	±5.0

COPY

richana B.

COPY

richana B.

Cert No. : ACL25306
Job No. : VC68AC0160
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	0.1	±2.0
125	0.0	0.1	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.0	0.0	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	38.9	-0.1	± 1.1
34.0	33.9	-0.1	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	26.8	-0.2	± 1.1
26.0	25.8	-0.2	± 1.1
25.0	24.8	-0.2	± 1.1

Cert. No. : ACL25306
Job No. : VC68AC0160
Pages : 6 of 8

Cert. No. : ACL25306
Job No. : VC68AC0160
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	28.9	-0.1	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.0 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

Cert. No. : ACL25306
Job No. : VC68AC0160
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.4	0.0	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.6	89.6	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

COPY

mechai B.

COPY

mechai B.

NOISE DOSI METER

MODEL : CR:110A

SERIAL No. : CB0954

CERTIFICATE OF CALIBRATION

ISSUED BY Cirrus Research plc

DATE OF ISSUE 28 January 2026 CERTIFICATE NUMBER 257818



Cirrus Research plc
Acoustic House
Bridlington Road
Hunmanby
North Yorkshire
YO14 0PH
United Kingdom

Page 1 of 2

Approved signatory
N.Smith
Electronically signed:

Dosemeter : IEC 61252-1993+A1:2000

Instrument information

Manufacturer: Cirrus Research plc
Model: CR:110A
Serial number: CB0954
Firmware version: 5.4

Notes: Eastern Thai Consulting 1992 Co.,Ltd.
683 Moo 11, Sukaphiban 8 Rd.,
Nongkham, Sriracha, Chonburi 20230

Test summary

Date of calibration: 28 January 2026

The calibration was performed respecting the requirements of ISO/IEC 17025:2017.

The dosimeter submitted for testing successfully completed the periodic tests of IEC 61252-1993+A1:2000.

The dosimeter submitted for testing conforms to the specifications in IEC 61252-1993+A1:2000.

Test equipment

Equipment	Manufacturer	Model	Serial number
Signal Generator	SIGLENT	SDG1032X	SDG1XDDD7R6629
Attenuator	Cirrus Research	ZE:952	96919
Environmental Monitor	Comet	T7510	16966334
doseBadge Reader	Cirrus Research plc	RC:110A	79620

Notes

This certificate provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory. The results within this certificate relate only to the items calibrated. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a coverage probability of approximately 95%.

COPY

CERTIFICATE OF CALIBRATION

Certificate Number:

257818

Page 2 of 2

Environmental conditions

The following conditions were recorded at the time of the test:

Before Pressure: 98.68 kPa Temperature: 21.5 °C Humidity: 38.0 %
After Pressure: 98.70 kPa Temperature: 21.6 °C Humidity: 39.0 %

Test results summary

Test	Result
Absolute Acoustic Sensitivity 1995	Complies
Linearity 1995	Complies
Short Duration 1995	Complies
Overload Latching 1995	Complies
Frequency weighting 1995	Complies

COPY

NOISE DOSI METER


MODEL : CR:110A

SERIAL No. : CB1499

CERTIFICATE OF CALIBRATION

ISSUED BY Cirrus Research plc

DATE OF ISSUE 28 January 2026 CERTIFICATE NUMBER 257825



Cirrus Research plc
Acoustic House
Bridlington Road
Hunmanby
North Yorkshire
YO14 0PH
United Kingdom

Page 1 of 2

Approved signatory
N.Smith
Electronically signed:

Dosimeter : IEC 61252-1993+A1:2000

Instrument information

Manufacturer: Cirrus Research plc

Model: CR:110A

Serial number: CB1499

Firmware version: 5.4

Notes: Eastern Thai Consulting 1992 Co.,Ltd.
683 Moo 11, Sukaphiban 8 Rd.,
Nongkham, Sriracha, Chonburi 20230

Test summary

Date of calibration: 28 January 2026

The calibration was performed respecting the requirements of ISO/IEC 17025:2017.

The dosimeter submitted for testing successfully completed the periodic tests of IEC 61252-1993+A1:2000.

The dosimeter submitted for testing conforms to the specifications in IEC 61252-1993+A1:2000.

Test equipment

Equipment	Manufacturer	Model	Serial number
Signal Generator	SIGLENT	SDG1032X	SDG1XDDQ6R6307
Attenuator	Cirrus Research	ZE:952	101220
Environmental Monitor	Comet	T7510	16966334
doseBadge Reader	Cirrus Research plc	UNIDB4A	109292

Notes

This certificate provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory. The results within this certificate relate only to the items calibrated. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a coverage probability of approximately 95%.

CERTIFICATE OF CALIBRATION

Certificate Number:

257825

Page 2 of 2

Environmental conditions

The following conditions were recorded at the time of the test:

Before	Pressure: 98.73 kPa	Temperature: 21.9 °C	Humidity: 39.6 %
After	Pressure: 98.74 kPa	Temperature: 21.9 °C	Humidity: 39.7 %

Test results summary

Test	Result
Absolute Acoustic Sensitivity 1995	Complies
Linearity 1995	Complies
Short Duration 1995	Complies
Overload Latching 1995	Complies
Frequency weighting 1995	Complies

COPY

COPY

NOISE DOSI METER

MODEL : CR:110A

SERIAL No. : CB0958

CERTIFICATE OF CALIBRATION

ISSUED BY Cirrus Research plc

DATE OF ISSUE 28 January 2026 CERTIFICATE NUMBER 257795

Cirrus Research plc
Acoustic House
Bridlington Road
Hunmanby
North Yorkshire
YO14 0PH
United Kingdom

Page 1 of 2

Approved signatory
N.Smith
Electronically signed:

Dosemeter : IEC 61252-1993+A1:2000

Instrument information

Manufacturer: Cirrus Research plc
Model: CR:110A
Serial number: CB0958
Firmware version: 5.4

Notes: Eastern Thai Consulting 1992 Co.,Ltd.
683 Moo 11, Sukaphiban 8 Rd.,
Nongkham, Sriracha, Chonburi 20230

Test summary

Date of calibration: 28 January 2026

The calibration was performed respecting the requirements of ISO/IEC 17025:2017.

The dosimeter submitted for testing successfully completed the periodic tests of IEC 61252-1993+A1:2000.

The dosimeter submitted for testing conforms to the specifications in IEC 61252-1993+A1:2000.

Test equipment

Equipment	Manufacturer	Model	Serial number
Signal Generator	SIGLENT	SDG1032X	SDG1XDCC7R0315
Attenuator	Cirrus Research	ZE:952	101223
Environmental Monitor	Comet	T7510	16966334
doseBadge Reader	Cirrus Research plc	RC:110A	109288

Notes

This certificate provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory. The results within this certificate relate only to the items calibrated. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2, providing a coverage probability of approximately 95%.

CERTIFICATE OF CALIBRATION

Certificate Number:
257795

Page 2 of 2

Environmental conditions

The following conditions were recorded at the time of the test:

Before Pressure: 98.62 kPa Temperature: 20.9 °C Humidity: 37.1 %
After Pressure: 98.66 kPa Temperature: 21.3 °C Humidity: 37.4 %

Test results summary

Test	Result
Absolute Acoustic Sensitivity 1995	Complies
Linearity 1995	Complies
Short Duration 1995	Complies
Overload Latching 1995	Complies
Frequency weighting 1995	Complies

NOISE DOSI METER

MODEL : CR:110A

SERIAL No. : CB1365

CERTIFICATE OF CALIBRATION

ISSUED BY Cirrus Research plc

DATE OF ISSUE 28 January 2026 CERTIFICATE NUMBER 257821



Cirrus Research plc
Acoustic House
Bridlington Road
Hunmanby
North Yorkshire
YO14 0PH
United Kingdom

Page 1 of 2

Approved signatory

N.Smith

Electronically signed:

Dosemeter : IEC 61252-1993+A1:2000

Instrument information

Manufacturer: Cirrus Research plc

Model: CR:110A

Serial number: CB1365

Firmware version: 5.4

Notes: Eastern Thai Consulting 1992 Co.,Ltd.
683 Moo 11, Sukaphiban 8 Rd.,
Nongkham, Sriracha, Chonburi 20230

Test summary

Date of calibration: 27 January 2026

The calibration was performed respecting the requirements of ISO/IEC 17025:2017.

The dosimeter submitted for testing successfully completed the periodic tests of IEC 61252-1993+A1:2000.

The dosimeter submitted for testing conforms to the specifications in IEC 61252-1993+A1:2000.

Test equipment

Equipment	Manufacturer	Model	Serial number
Signal Generator	SIGLENT	SDG1032X	SDG1XDDQ6R6307
Attenuator	Cirrus Research	ZE:952	101220
Environmental Monitor	Comet	T7510	16966334
doseBadge Reader	Cirrus Research plc	UNIDB4A	109292

Notes

COPY

This certificate provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory. The results within this certificate relate only to the items calibrated. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a coverage probability of approximately 95%.

CERTIFICATE OF CALIBRATION

Certificate Number:

257821

Page 2 of 2

Environmental conditions

The following conditions were recorded at the time of the test:

Before Pressure: 97.92 kPa Temperature: 23.3 °C Humidity: 35.2 %
After Pressure: 97.90 kPa Temperature: 23.3 °C Humidity: 36.5 %

Test results summary

Test	Result
Absolute Acoustic Sensitivity 1995	Complies
Linearity 1995	Complies
Short Duration 1995	Complies
Overload Latching 1995	Complies
Frequency weighting 1995	Complies

COPY

NOISE DOSI METER


MODEL : CR:110A

SERIAL No. : CB1500

CERTIFICATE OF CALIBRATION

ISSUED BY Cirrus Research plc

DATE OF ISSUE 28 January 2026 CERTIFICATE NUMBER 257824



Cirrus Research plc
Acoustic House
Bridlington Road
Hunmanby
North Yorkshire
YO14 0PH
United Kingdom

Page 1 of 2

Approved signatory
N.Smith
Electronically signed:

Dosemeter : IEC 61252-1993+A1:2000

Instrument information

Manufacturer: Cirrus Research plc
Model: CR:110A
Serial number: CB1500
Firmware version: 5.4

Notes: Eastern Thai Consulting 1992 Co.,Ltd.
683 Moo 11, Sukaphiban 8 Rd.,
Nongkham, Sriracha, Chonburi 20230

Test summary

Date of calibration: 28 January 2026

The calibration was performed respecting the requirements of ISO/IEC 17025:2017.

The dosimeter submitted for testing successfully completed the periodic tests of IEC 61252-1993+A1:2000.

The dosimeter submitted for testing conforms to the specifications in IEC 61252-1993+A1:2000.

Test equipment

Equipment	Manufacturer	Model	Serial number
Signal Generator	SIGLENT	SDG1032X	SDG1XDDQ6R6307
Attenuator	Cirrus Research	ZE:952	101220
Environmental Monitor	Comet	T7510	16966334
doseBadge Reader	Cirrus Research plc	UNIDB4A	109292

Notes

This certificate provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory. The results within this certificate relate only to the items calibrated. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a coverage probability of approximately 95%.

CERTIFICATE OF CALIBRATION

Certificate Number:

257824

Page 2 of 2

Environmental conditions

The following conditions were recorded at the time of the test:

Before	Pressure: 98.83 kPa	Temperature: 22.4 °C	Humidity: 40.2 %
After	Pressure: 98.84 kPa	Temperature: 22.5 °C	Humidity: 40.6 %

Test results summary

Test	Result
Absolute Acoustic Sensitivity 1995	Complies
Linearity 1995	Complies
Short Duration 1995	Complies
Overload Latching 1995	Complies
Frequency weighting 1995	Complies

COPY

COPY

NOISE DOSI METER


MODEL : CR:110A

SERIAL No. : CB0643

CERTIFICATE OF CALIBRATION

ISSUED BY Cirrus Research plc

DATE OF ISSUE 28 January 2026 CERTIFICATE NUMBER 257791



Cirrus Research plc
Acoustic House
Bridlington Road
Hunmanby
North Yorkshire
YO14 0PH
United Kingdom

Page 1 of 2

Approved signatory
N.Smith
Electronically signed:

Dosemeter : IEC 61252-1993+A1:2000

Instrument information

Manufacturer: Cirrus Research plc
Model: CR:110A
Serial number: CB0643
Firmware version: 5.4

Notes: Eastern Thai Consulting 1992 Co.,Ltd.
683 Moo 11, Sukaphiban 8 Rd.,
Nongkham, Sriracha, Chonburi 20230

Test summary

Date of calibration: 27 January 2026

The calibration was performed respecting the requirements of ISO/IEC 17025:2017.

The dosimeter submitted for testing successfully completed the periodic tests of IEC 61252-1993+A1:2000.

The dosimeter submitted for testing conforms to the specifications in IEC 61252-1993+A1:2000.

Test equipment

Equipment	Manufacturer	Model	Serial number
Signal Generator	SIGLENT	SDG1032X	SDG1XDDC7R0315
Attenuator	Cirrus Research	ZE:952	101223
Environmental Monitor	Comet	T7510	16966334
doseBadge Reader	Cirrus Research plc	RC:110A	109288

Notes

COPY

This certificate provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory. The results within this certificate relate only to the items calibrated. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a coverage probability of approximately 95%.

CERTIFICATE OF CALIBRATION

Certificate Number:
257791

Page 2 of 2

Environmental conditions

The following conditions were recorded at the time of the test:

Before Pressure: 97.90 kPa Temperature: 23.1 °C Humidity: 37.1 %
After Pressure: 97.90 kPa Temperature: 22.7 °C Humidity: 38.6 %

Test results summary

Test	Result
Absolute Acoustic Sensitivity 1995	Complies
Linearity 1995	Complies
Short Duration 1995	Complies
Overload Latching 1995	Complies
Frequency weighting 1995	Complies

COPY

NOISE DOSI METER

MODEL : CR:110A

SERIAL No. : CB0644

CERTIFICATE OF CALIBRATION

ISSUED BY Cirrus Research plc

DATE OF ISSUE 28 January 2026 CERTIFICATE NUMBER 257790



Cirrus Research plc
Acoustic House
Bridlington Road
Hunmanby
North Yorkshire
YO14 0PH
United Kingdom

Page 1 of 2

Approved signatory
N.Smith
Electronically signed:

Dosimeter : IEC 61252-1993+A1:2000

Instrument information

Manufacturer: Cirrus Research plc Notes: Eastern Thai Consulting 1992 Co.,Ltd.
Model: CR:110A 683 Moo 11, Sukaphiban 8 Rd.,
Serial number: CB0644 Nongkham, Sriracha, Chonburi 20230
Firmware version: 5.4

Test summary

Date of calibration: 28 January 2026

The calibration was performed respecting the requirements of ISO/IEC 17025:2017.
The dosimeter submitted for testing successfully completed the periodic tests of IEC 61252-1993+A1:2000.

The dosimeter submitted for testing conforms to the specifications in IEC 61252-1993+A1:2000.

Test equipment

Equipment	Manufacturer	Model	Serial number
Signal Generator	SIGLENT	SDG1032X	SDG1XDDC7R0315
Attenuator	Cirrus Research	ZE:952	101223
Environmental Monitor	Comet	T7510	16966334
doseBadge Reader	Cirrus Research plc	RC:110A	109288

Notes

This certificate provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory. The results within this certificate relate only to the items calibrated. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a coverage probability of approximately 95%.

CERTIFICATE OF CALIBRATION

Certificate Number:
257790

Page 2 of 2

Environmental conditions

The following conditions were recorded at the time of the test:

Before Pressure: 98,57 kPa Temperature: 20,6 °C Humidity: 35,0 %
After Pressure: 98,59 kPa Temperature: 20,9 °C Humidity: 36,5 %

Test results summary

Test	Result
Absolute Acoustic Sensitivity 1995	Complies
Linearity 1995	Complies
Short Duration 1995	Complies
Overload Latching 1995	Complies
Frequency weighting 1995	Complies

COPY

COPY

NOISE DOSI METER


MODEL : CR:110A

SERIAL No. : CB0956

CERTIFICATE OF CALIBRATION

ISSUED BY Cirrus Research plc

DATE OF ISSUE 28 January 2026 CERTIFICATE NUMBER 257794



Cirrus Research plc
Acoustic House
Bridlington Road
Hunmanby
North Yorkshire
YO14 0PH
United Kingdom

Page 1 of 2

Approved signatory
N.Smith
Electronically signed:

Dosemeter : IEC 61252-1993+A1:2000

Instrument information

Manufacturer: Cirrus Research plc

Model: CR:110A

Serial number: CB0956

Firmware version: 5.4

Notes: Eastern Thai Consulting 1992 Co.,Ltd.
683 Moo 11, Sukaphiban 8 Rd.,
Nongkham, Sriracha, Chonburi 20230

Test summary

Date of calibration: 28 January 2026

The calibration was performed respecting the requirements of ISO/IEC 17025:2017.

The dosimeter submitted for testing successfully completed the periodic tests of IEC 61252-1993+A1:2000.

The dosimeter submitted for testing conforms to the specifications in IEC 61252-1993+A1:2000.

Test equipment

Equipment	Manufacturer	Model	Serial number
Signal Generator	SIGLENT	SDG1032X	SDG1XDDQ6R6307
Attenuator	Cirrus Research	ZE:952	101220
Environmental Monitor	Comet	T7510	16966334
doseBadge Reader	Cirrus Research plc	UNIDB4A	109292

Notes

This certificate provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory. The results within this certificate relate only to the items calibrated. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a coverage probability of approximately 95%.

COPY

CERTIFICATE OF CALIBRATION

Certificate Number:

257794

Page 2 of 2

Environmental conditions

The following conditions were recorded at the time of the test:

Before	Pressure: 98.63 kPa	Temperature: 21.2 °C	Humidity: 37.0 %
After	Pressure: 98.67 kPa	Temperature: 21.5 °C	Humidity: 37.7 %

Test results summary

Test	Result
Absolute Acoustic Sensitivity 1995	Complies
Linearity 1995	Complies
Short Duration 1995	Complies
Overload Latching 1995	Complies
Frequency weighting 1995	Complies

COPY

NOISE DOSI METER


MODEL : CR:110A

SERIAL No. : CB0955

CERTIFICATE OF CALIBRATION

ISSUED BY Cirrus Research plc

DATE OF ISSUE 28 January 2026 CERTIFICATE NUMBER 257792



Cirrus Research plc
Acoustic House
Bridlington Road
Hunmanby
North Yorkshire
YO14 0PH
United Kingdom

Page 1 of 2

Approved signatory
N.Smith
Electronically signed:

Dosimeter : IEC 61252-1993+A1:2000

Instrument information

Manufacturer: Cirrus Research plc
Model: CR:110A
Serial number: CB0955
Firmware version: 5.4

Notes: Eastern Thai Consulting 1992 Co.,Ltd.
683 Moo 11, Sukaphiban 8 Rd.,
Nongkham, Sriracha, Chonburi 20230

Test summary

Date of calibration: 28 January 2026

The calibration was performed respecting the requirements of ISO/IEC 17025:2017.

The dosimeter submitted for testing successfully completed the periodic tests of IEC 61252-1993+A1:2000.

The dosimeter submitted for testing conforms to the specifications in IEC 61252-1993+A1:2000.

Test equipment

Equipment	Manufacturer	Model	Serial number
Signal Generator	SIGLENT	SDG1032X	SDG1XDDC7R0315
Attenuator	Cirrus Research	ZE:952	101223
Environmental Monitor	Comet	T7510	16966334
doseBadge Reader	Cirrus Research plc	RC:110A	109288

Notes

This certificate provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory. The results within this certificate relate only to the items calibrated. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a coverage probability of approximately 95%.

CERTIFICATE OF CALIBRATION

Certificate Number:
257792

Page 2 of 2

Environmental conditions

The following conditions were recorded at the time of the test:

Before Pressure: 98.67 kPa Temperature: 21,2 °C Humidity: 38,0 %
After Pressure: 98.69 kPa Temperature: 21,6 °C Humidity: 38,5 %

Test results summary

Test	Result
Absolute Acoustic Sensitivity 1995	Complies
Linearity 1995	Complies
Short Duration 1995	Complies
Overload Latching 1995	Complies
Frequency weighting 1995	Complies

COPY

COPY

NOISE DOSI METER

MODEL : CR:110A

SERIAL No. : CB0957

CERTIFICATE OF CALIBRATION

ISSUED BY Cirrus Research plc

DATE OF ISSUE 28 January 2026 CERTIFICATE NUMBER 257815

Cirrus Research plc
Acoustic House
Bridlington Road
Hunmanby
North Yorkshire
YO14 0PH
United Kingdom

Page 1 of 2

Approved signatory
N.Smith
Electronically signed:

N.Smith

Dosimeter : IEC 61252-1993+A1:2000

Instrument information

Manufacturer: Cirrus Research plc

Model: CR:110A

Serial number: CB0957

Firmware version: 5.4

Notes: Eastern Thai Consulting 1992 Co.,Ltd.
683 Moo 11, Sukaphiban 8 Rd.,
Nongkham, Sriracha, Chonburi 20230

Test summary

Date of calibration: 28 January 2026

The calibration was performed respecting the requirements of ISO/IEC 17025:2017.

The dosimeter submitted for testing successfully completed the periodic tests of IEC 61252-1993+A1:2000.

The dosimeter submitted for testing conforms to the specifications in IEC 61252-1993+A1:2000.

Test equipment

Equipment	Manufacturer	Model	Serial number
Signal Generator	SIGLENT	SDG1032X	SDG1XDDQ6R6307
Attenuator	Cirrus Research	ZE:952	101220
Environmental Monitor	Comet	T7510	16966334
doseBadge Reader	Cirrus Research plc	UNIDB4A	109292

Notes

This certificate provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory. The results within this certificate relate only to the items calibrated. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a coverage probability of approximately 95%.

CERTIFICATE OF CALIBRATION

Certificate Number:

257815

Page 2 of 2

Environmental conditions

The following conditions were recorded at the time of the test:

Before Pressure: 98.70 kPa Temperature: 21.6 °C Humidity: 38.5 %
After Pressure: 98.71 kPa Temperature: 21.6 °C Humidity: 38.8 %

Test results summary

Test	Result
Absolute Acoustic Sensitivity 1995	Complies
Linearity 1995	Complies
Short Duration 1995	Complies
Overload Latching 1995	Complies
Frequency weighting 1995	Complies

COPY

NOISE DOSI METER


MODEL : CR:110A

SERIAL No. : CA8888

CERTIFICATE OF CALIBRATION

ISSUED BY Cirrus Research plc

DATE OF ISSUE 28 January 2026 CERTIFICATE NUMBER 257802



Cirrus Research plc
Acoustic House
Bridlington Road
Hunmanby
North Yorkshire
YO14 0PH
United Kingdom

Page 1 of 2

Approved signatory

N.Smith

Electronically signed:

Dosemeter : IEC 61252-1993+A1:2000

Instrument information

Manufacturer: Cirrus Research plc

Model: CR:110A

Serial number: CA8888

Firmware version: 5.4

Notes: Eastern Thai Consulting 1992 Co.,Ltd.
683 Moo 11, Sukaphiban 8 Rd.,
Nongkham, Sriracha, Chonburi 20230

Test summary

Date of calibration: 28 January 2026

The calibration was performed respecting the requirements of ISO/IEC 17025:2017.

The dosimeter submitted for testing successfully completed the periodic tests of IEC 61252-1993+A1:2000.

The dosimeter submitted for testing conforms to the specifications in IEC 61252-1993+A1:2000.

Test equipment

Equipment	Manufacturer	Model	Serial number
Signal Generator	SIGLENT	SDG1032X	SDG1XDDD7R6629
Attenuator	Cirrus Research	ZE:952	96919
Environmental Monitor	Comet	T7510	16966334
doseBadge Reader	Cirrus Research plc	RC:110A	79620

Notes

This certificate provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory. The results within this certificate relate only to the items calibrated. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a coverage probability of approximately 95%.

CERTIFICATE OF CALIBRATION

Certificate Number:

257802

Page 2 of 2

Environmental conditions

The following conditions were recorded at the time of the test:

Before Pressure: 98.59 kPa Temperature: 20.8 °C Humidity: 37.0 %
After Pressure: 98.63 kPa Temperature: 21.2 °C Humidity: 37.2 %

Test results summary

Test	Result
Absolute Acoustic Sensitivity 1995	Complies
Linearity 1995	Complies
Short Duration 1995	Complies
Overload Latching 1995	Complies
Frequency weighting 1995	Complies

COPY

COPY

NOISE DOSI METER

MODEL : CR:110A

SERIAL No. : CA8889

CERTIFICATE OF CALIBRATION

ISSUED BY Cirrus Research plc

DATE OF ISSUE 28 January 2026 CERTIFICATE NUMBER 257798



Cirrus Research plc
Acoustic House
Bridlington Road
Hunmanby
North Yorkshire
YO14 0PH
United Kingdom

Page 1 of 2

Approved signatory
N.Smith
Electronically signed:

Dosemeter : IEC 61252-1993+A1:2000

Instrument information

Manufacturer: Cirrus Research plc Notes: Eastern Thai Consulting 1992 Co.,Ltd.
Model: CR:110A 683 Moo 11, Sukaphiban 8 Rd.,
Serial number: CA8889 Nongkham, Sriracha, Chonburi 20230
Firmware version: 5.4

Test summary

Date of calibration: 28 January 2026

The calibration was performed respecting the requirements of ISO/IEC 17025:2017.
The dosimeter submitted for testing successfully completed the periodic tests of IEC 61252-1993+A1:2000.

The dosimeter submitted for testing conforms to the specifications in IEC 61252-1993+A1:2000.

Test equipment

Equipment	Manufacturer	Model	Serial number
Signal Generator	SIGLENT	SDG1032X	SDG1XDDQ6R6307
Attenuator	Cirrus Research	ZE:952	101220
Environmental Monitor	Comet	T7510	16966334
doseBadge Reader	Cirrus Research plc	UNIDB4A	109292

Notes

This certificate provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory. The results within this certificate relate only to the items calibrated. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a coverage probability of approximately 95%.

CERTIFICATE OF CALIBRATION

Certificate Number:
257798

Page 2 of 2

Environmental conditions

The following conditions were recorded at the time of the test:

Before Pressure: 98.57 kPa Temperature: 20.7 °C Humidity: 35.7 %
After Pressure: 98.60 kPa Temperature: 20.8 °C Humidity: 37.5 %

Test results summary

Test	Result
Absolute Acoustic Sensitivity 1995	Complies
Linearity 1995	Complies
Short Duration 1995	Complies
Overload Latching 1995	Complies
Frequency weighting 1995	Complies

COPY

COPY

NOISE DOSI METER

MODEL : CR:110A

SERIAL No. : CA8879

CERTIFICATE OF CALIBRATION

ISSUED BY Cirrus Research plc

DATE OF ISSUE 28 January 2026 CERTIFICATE NUMBER 257799

Cirrus Research plc
Acoustic House
Bridlington Road
Hunmanby
North Yorkshire
YO14 0PH
United Kingdom

Page 1 of 2

Approved signatory
N.Smith
Electronically signed:

Dosimeter : IEC 61252-1993+A1:2000

Instrument information

Manufacturer: Cirrus Research plc
Model: CR:110A
Serial number: CA8879
Firmware version: 5.4

Notes: Eastern Thai Consulting 1992 Co.,Ltd.
683 Moo 11, Sukaphiban 8 Rd.,
Nongkham, Sriracha, Chonburi 20230

Test summary

Date of calibration: 27 January 2026

The calibration was performed respecting the requirements of ISO/IEC 17025:2017.
The dosimeter submitted for testing successfully completed the periodic tests of IEC 61252-1993+A1:2000.

The dosimeter submitted for testing conforms to the specifications in IEC 61252-1993+A1:2000.

Test equipment

Equipment	Manufacturer	Model	Serial number
Signal Generator	SIGLENT	SDG1032X	SDG1XDDQ6R6307
Attenuator	Cirrus Research	ZE:952	101220
Environmental Monitor	Comet	T7510	16966334
doseBadge Reader	Cirrus Research plc	UNIDB4A	109292

Notes

This certificate provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory. The results within this certificate relate only to the items calibrated. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a coverage probability of approximately 95%.

CERTIFICATE OF CALIBRATION

Certificate Number:
257799

Page 2 of 2

Environmental conditions

The following conditions were recorded at the time of the test:

Before Pressure: 97.90 kPa Temperature: 22.9 °C Humidity: 37.8 %
After Pressure: 97.90 kPa Temperature: 22.6 °C Humidity: 39.2 %

Test results summary

Test	Result
Absolute Acoustic Sensitivity 1995	Complies
Linearity 1995	Complies
Short Duration 1995	Complies
Overload Latching 1995	Complies
Frequency weighting 1995	Complies

COPY

COPY

ANALYTICAL BALANCE (DU)

Model : XS205DU

Serial No. : B344940005

Certificate No. : 25-205716
Sample Code : 25-90375-006

CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapibarn 8 Rd, Nongkham,
Sriracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.
(Analytical Balance Room)

Equipment : ELECTRONIC BALANCE

Manufacturer : METTLER TOLEDO

Model : XS205DU

Serial No. : B344940005

ID No. : LABE 05/3

Date of Receipt : 26 November 2025

Date of Calibration : 26 November 2025

Calibrated by Mr. Thanadol Pholthep
Scientist

Approved by (Mr. Somchai Neampunt)
Signed for Director

Issue date 28 November 2025

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

Certificate No. : 25-205716
Sample Code : 25-90375-006

REPORT OF CALIBRATION

Equipment : ELECTRONIC BALANCE
Manufacturer : METTLER TOLEDO
Model : XS205DU
Capacity : Max 81 g / 200 g
Resolution : 0.00001 g / 0.0001 g
Serial No. : B344940005
ID No. : LABE 05/3

Result of Calibration

1. Test weight and repeatability of reading

Repeatability is a measure of the ability of a balance to supply the same result in repetitive weighings with one and the same load under the same measurement condition. The measurement of the repeatability must include both the balance specifications and the ambient (vibration, fluctuating air current/temperature/humidity, etc.) Operator handling of the balance is also included in the standard deviation.

Unit : g	Range : 81	☐ Before adjustment	☐ After adjustment
	Nominal value	40	80
☒ No adjustment	Standard weight	40.000087	80.000088
☐ Adjustment	Average reading of indicator	40.00004	80.00004
	Standard deviation	0.000007	0.000007

Unit : g	Range : 200	☐ Before adjustment	☐ After adjustment
	Nominal value	100	200
☒ No adjustment	Standard weight	99.999988	200.000015
☐ Adjustment	Average reading of indicator	99.9999	199.9997
	Standard deviation	0.00005	0.00005

Certificate No. : 25-205716
Sample Code : 25-90375-006

Page 3 of 4

REPORT OF CALIBRATION

Result of Calibration

2. Sensitivity or value of a scale division

Change in the output variable of a measuring instrument divided by the associated change in the input variable.

Unit : g

Range : 81

Range : 200

Test Point	Sensitivity, S	Test Point	Sensitivity, S
0	1.00000	0	1.0000
40	1.00000	100	1.0000
80	1.00000	200	1.0000

3. Departure of indication from nominal value, Linearity

Unit : g

Nominal Value	Standard Value	Average Reading of Indicator	Correction Value	Expanded Uncertainty	Coverage Factor (k)
Unload	0.0000000	0.00000	0.00000	0.000011	2.04
0.01	0.0100016	0.01000	0.00000	0.000011	2.04
0.1	0.1000056	0.10000	0.00001	0.000012	2.02
1	1.0000110	1.00000	0.00001	0.000015	2.01
5	4.9999996	4.99998	0.00002	0.000020	2.00
10	9.9999994	9.99999	0.00000	0.000026	2.00
20	20.000042	20.00000	0.00004	0.000037	2.00
50	50.000052	50.00003	0.00002	0.000067	2.00
100	99.999988	100.00000	0.00000	0.00016	2.00
150	150.000040	150.00001	-0.00001	0.00022	2.00
200	200.000015	200.00001	-0.00001	0.00027	2.00

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

Certificate No. : 25-205716
Sample Code : 25-90375-006

Page 4 of 4


REPORT OF CALIBRATION

Result of Calibration :

4. Eccentric or off-centre loading

Deviation of the measurement value through off - center (eccentric) loading. The corner load increases with the weight of the load and its removal from the center of the pan support.

☐ Triangular ☒ Rectangular ☐ Circle			Test weight : 50 and 100 Unit : g	
Range	81	200		
Position	Reading of indicator	Reading of indicator		
1	50.00000	100.0000		
2	49.99997	100.0000		
3	49.99993	99.9999		
4	49.99999	100.0000		
5	50.00003	99.9999		
6	50.00000	100.0000		
Maximum difference	0.00007	0.0001		

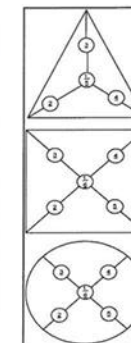

Condition of Calibration

1. Calibration Method : WI-CL-004 base on UKAS LAB 14: 2019

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. Condition of Calibration item: Normal

4. This certification is traceable to the International System of Unit maintained at : -

- Through the reference standard laboratory of Asia Medical and Agricultural Laboratory and Research Center Public

Company Limited (Instrument number 1).

5. Reference standard instrument :

Instrument	Class	ID No.	Certificate No.	Due Date
1) STANDARD WEIGHT 1 mg to 1 kg	E2	LB-WE-78	25-134074	18 July 2026

- End of Report -

6. Ambient conditions	Min	Max
Temperature (°C)	22.9	24.3
Relative Humidity (%Rh)	45.4	47.7
Air pressure (hPa)	1007.2	1011.0

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

ANALYTICAL BALANCE

Model : SECURA224-1S

Serial No. : 0036707137

Certificate No. : 25-205715
Sample Code : 25-90375-005

CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapibarn 8 Rd, Nongkham,
Sriracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.
(Analytical Balance Room)

Equipment : ELECTRONIC BALANCE

Manufacturer : SARTORIUS

Model : SECURA224-1S

Serial No. : 0036707137

ID No. : LABE 05/2

Date of Receipt : 26 November 2025

Date of Calibration : 26 November 2025

Calibrated by Mr. Pisek Into
Scientist

Approved by (Mr. Somchai Neampunt)
Signed for Director

Issue date 28 November 2025

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

Certificate No. : 25-205715
Sample Code : 25-90375-005

REPORT OF CALIBRATION

Equipment : ELECTRONIC BALANCE
Manufacturer : SARTORIUS
Model : SECURA224-1S
Capacity : Max 220 g
Resolution : 0.0001 g
Serial No. : 0036707137
ID No. : LABE 05/2

Result of Calibration

1. Test weight and repeatability of reading

Repeatability is a measure of the ability of a balance to supply the same result in repetitive weighings with one and the same load under the same measurement condition. The measurement of the repeatability must include both the balance specifications and the ambient (vibration, fluctuating air current/temperature/humidity, etc.) Operator handling of the balance is also included in the standard deviation.

Unit : g	Range : 220	☒ Before adjustment	☒ After adjustment
	Nominal value	100	200
☐ No adjustment	Standard weight	100.000045	200.000047
☒ Adjustment	Average reading of indicator	99.9999	199.9998
	Standard deviation	0.00006	0.00008

Unit : -	Range : -	☐ Before adjustment	☐ After adjustment
	Nominal value	-	-
☐ No adjustment	Standard weight	-	-
☐ Adjustment	Average reading of indicator	-	-
	Standard deviation	-	-

COPY

Certificate No. : 25-205715
Sample Code : 25-90375-005

Page 3 of 4

REPORT OF CALIBRATION

Result of Calibration

2. Sensitivity or value of a scale division

Change in the output variable of a measuring instrument divided by the associated change in the input variable.

Unit : g

Range : 220

Range : -

Test Point	Sensitivity, S	Test Point	Sensitivity, S
0	1.0966	-	-
100	0.9969	-	-
200	0.9969	-	-

3. Departure of indication from nominal value, Linearity

Unit : g

Nominal Value	Standard Value	Average Reading of Indicator	Correction Value	Expanded Uncertainty	Coverage Factor (k)
Unload	0.0000000	0.0000	0.0000	0.000094	2.01
0.01	0.0100031	0.0100	0.0000	0.000094	2.01
0.1	0.1000023	0.1000	0.0000	0.000094	2.01
1	1.0000136	1.0000	0.0000	0.000095	2.01
2	2.0000101	2.0000	0.0000	0.000095	2.01
5	5.0000210	5.0000	0.0000	0.000096	2.01
10	10.000002	10.0000	0.0000	0.000097	2.01
20	20.000033	20.0000	0.0000	0.00011	2.01
50	50.000016	50.0000	0.0000	0.00012	2.01
100	100.000045	100.0000	0.0000	0.00016	2.00
200	200.000047	200.0000	0.0000	0.00027	2.00

COPY

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

Certificate No. : 25-205715
Sample Code : 25-90375-005

Page 4 of 4


REPORT OF CALIBRATION

Result of Calibration :

4. Eccentric or off-centre loading

Deviation of the measurement value through off - center (eccentric) loading. The corner load increases with the weight of the load and its removal from the center of the pan support.

Weighing pan	☐ Triangular ☐ Rectangular ☒ Circle	Test weight : 100 Unit : g
Range	220	-
Position	Reading of indicator	Reading of indicator
1	100.0000	-
2	100.0001	-
3	99.9999	-
4	99.9998	-
5	100.0001	-
6	100.0000	-
Maximum difference	0.0002	-

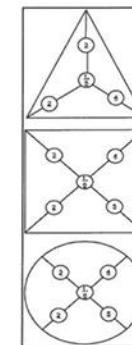

Condition of Calibration

1. Calibration Method : WI-CL-004 base on UKAS LAB 14: 2019

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. Condition of Calibration item: Normal

4. This certification is traceable to the International System of Unit maintained at : -

- Through the reference standard laboratory of Asia Medical and Agricultural Laboratory and Research Center Public

Company Limited (Instrument number 1).

5. Reference standard instrument :

Instrument	Class	ID No.	Certificate No.	Due Date
1) STANDARD WEIGHT 1 mg to 1 kg	E2	LB-WE-79	25-142885	27 July 2026

- End of Report -

COPY

BAROMETER

Serial No. : N/A[S41020124]



CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel: 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com



CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : BAROMETER
MANUFACTURER : BARJO
MODEL / TYPE : N/A
SERIAL NO. : N/A[S41020124]
CLID. NO. : 212500828
JOB CONTROL NO. : 250507051351
CALIBRATION SERVICE : ☒ IN-LABORATORY ☐ ON-SITE

CUSTOMER : EASTERN THAI CONSULTING 1992 CO., LTD.
683 MOO 11, SUKHAPIBARN 8 RD,
NONGKHAM, SRIRACHA, CHONBURI 20230

DATE OF RECEIVED : 07 May 2025

DATE OF ISSUED : 09 May 2025

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sittipong Pimdee
Calibration Engineer

Approved By : Mongkol Yotsoontorn
Authorized Signatory
09 May 2025



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q25051351


F3-011-05/12-23

page 1 of 3



CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel: 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com



REPORT OF CALIBRATION

FOR

NOMENCLATURE : BAROMETER
MANUFACTURER : BARJO
MODEL / TYPE : N/A
SERIAL NO. : N/A[S41020124]
DATE OF CALIBRATION : 08 May 2025

ENVIRONMENT CONDITIONS :

Temperature : $(23 \pm 2) ^\circ\text{C}$

Relative Humidity : $(55 \pm 10) \% \text{RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. CLC-CPPP-08 according to DKD-R 6-1 as calibration guidelines.

The calibration was performed by direct measurement with Reference Pressure Monitor which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

Reference Pressure Monitor, Fluke Model RPM3 S/N. 829.

TRACEABILITY :

The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand).

Certificate No. MP-0245-24, Due Date 11 November 2025.

UNCERTAINTY :

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor of $k = 2$. It has been evaluated according to the "Calibration of Pressure Gauges (DKD-R 6-1)" which provides a level of confidence approximately 95%.

Certificate No. Q25051351

F3-011-05/12-23

page 2 of 3





CALIBRATION LABORATORY CO., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-570-0353-4 Fax 02-578-2672 www.cal laboratory.com E-mail: snie@cal laboratory.com



CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The DUC was exercised by applying a known pressure from its zero to full scale 1 times. Then 2 series of known gauge pressure were applied. The STD reading were recorded and the means value were reported in the table below.

CALIBRATION DATA

CORRECTION OF PRESSURE

DUC Test point (hPa)	STD Reading (hPa)		Correction (hPa)	
	Up	Down	Up	Down
990	990.7	990.7	+0.7	+0.7
1000	1000.7	1000.8	+0.7	+0.8
1010	1010.8	1010.8	+0.8	+0.8
1020	1020.8	1020.9	+0.8	+0.9
1030	1030.9	1030.9	+0.9	+0.9

Uncertainty of measurement ± 0.7 hPa

Transmitting fluid : Air.

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 015 Page 44 of 68

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q25051351

F3-011-05/12-23

COPY



@clccalibration

BAROMETER

Serial No. : N/A[S41020124]



CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Road, Ladphrao, Bangkok 10230
Tel, 02-578-0353-4 Fax, 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com



CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : BAROMETER
MANUFACTURER : BARIO
MODEL / TYPE : N/A
SERIAL NO. : N/A[S41020124]
CLID. NO. : 212500828
JOB CONTROL NO. : 260507056453
CALIBRATION SERVICE : ☒ IN-LABORATORY ☐ ON-SITE

CUSTOMER : EASTERN THAI CONSULTING 1992 CO., LTD.
683 MOO 11, SUKHAPIBARN 8 RD,
NONGKHAM, SRIRACHA, CHONBURI 20230

DATE OF RECEIVED : 07 May 2026

DATE OF ISSUED : 11 May 2026

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sittipong Pimdee
Calibration Engineer

Approved By : Mongkol Yotsoontorn
Authorized Signatory
11 May 2026



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q26056453

F3-011-05/12-23

COPY

page 1 of 3



@clccalibration



CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Road, Ladphrao, Bangkok 10230
Tel, 02-578-0353-4 Fax, 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com



REPORT OF CALIBRATION

FOR

NOMENCLATURE : BAROMETER
MANUFACTURER : BARIO
MODEL / TYPE : N/A
SERIAL NO. : N/A[S41020124]
DATE OF CALIBRATION : 09 May 2026

ENVIRONMENT CONDITIONS :

Temperature : $(23 \pm 2) ^\circ\text{C}$

Relative Humidity : $(55 \pm 10) \% \text{RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. CLC-CPPP-08 according to DKD-R 6-1 as calibration guidelines.

The calibration was performed by direct measurement with Reference Pressure Monitor which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

Reference Pressure Monitor, Fluke Model RPM3 S/N. 829.

TRACEABILITY :

The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand).
Certificate No. MP-0284-25, Due Date 28 November 2026.

UNCERTAINTY :

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor of $k = 2$. It has been evaluated according to the "Calibration of Pressure Gauges (DKD-R 6-1)" which provides a level of confidence approximately 95%.

Certificate No. Q26056453

F3-011-05/12-23

COPY

page 2 of 3



@clccalibration



CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Road, Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com



CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The DUC was exercised by applying a known pressure from its zero to full scale 1 times. Then 2 series of known gauge pressure were applied. The STD reading were recorded and the means value were reported in the table below.

CALIBRATION DATA

CORRECTION OF PRESSURE

DUC Test point (hPa)	STD Reading (hPa)		Correction (hPa)	
	Up	Down	Up	Down
990	990.9	991.0	+0.9	+1.0
1000	1001.0	1001.1	+1.0	+1.1
1010	1011.2	1011.3	+1.2	+1.3
1020	1021.3	1021.4	+1.3	+1.4
1030	1031.4	1031.4	+1.4	+1.4

Uncertainty of measurement ± 0.9 hPa

Transmitting fluid : Air.

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 018 Page 47 of 73

This report is valid for the above stated instrument/s only.

End of Certificate

COPY

Certificate No. Q26056453

F3-011-05/12-23

page 3 of 3



@clcalibration

BOD INCUBATOR

Model : LABE 19/3

CERTIFICATE OF CALIBRATION

Certificate No. : 25-118065

Sample Code : 25-51697-001

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapibarn 8 Rd., Nongkham,
Sriracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.
(Laboratory)

Equipment : Temperature controlled enclosures (Incubator)

Manufacturer : บริษัท เจริญชัย Model : N/A

Serial No. : S43020027 ID No. : LABE 19/3

Date of Receipt : 25 June 2025 Date of Calibration : 25 June 2025

Condition of Calibration

1. Environment
- | | | |
|---------------------------|---------------------|---------------------|
| 1.1 Ambient temperature | : Maximum 34.6 °C | : Minimum 32.2 °C |
| 1.2 Relative humidity | : Maximum 64.0 % | : Minimum 58.7 % |
| 1.3 Line voltage supplied | : Maximum 224.5 VAC | : Minimum 223.8 VAC |

2. Calibration method

TLAS-G-20: Guidelines for calibration and checks of temperature controlled enclosures.

3. Reference standard instrument

Instrument	ID No.	Certificate No.	Due Date
Data Acquisition With Sensor (RTD-Pt100)	LB-DA-08 (RTD-411 to RTD-419)	25-082913	18 May 2026

4. This certificate is traceable to the international system of unit (SI Unit).

The measurement is traceable to Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by

Mr. Pattanapong Pulngern

Approved by

(Mr. Somchai Neampunt)

Scientist

Signed for Director

Issue date

26 June 2025

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

REPORT OF CALIBRATION

Certificate No. : 25-118065

Sample Code : 25-51697-001

Results of Calibration

Resolution : 0.1 °C

1. Reporting of Temperature

Calibration point (°C)	UUC* setting (°C)	UUC* reading (°C)	Measured temperature at each positions (°C)										Uncertainty ± (°C)	Coverage factor k
			#1	#2	#3	#4	#5	#6	#7	#8	#9 ^{Ref}	#10		
20	20.0	20.0	20.61	20.42	19.97	19.90	20.29	20.47	20.25	19.96	20.18		0.24	2.00

2. Characterization results

Calibration point (°C)	Stability ± (°C)	Uniformity (°C)	Overall variation (°C)
20	0.09	0.46	0.89

Notes

- UUC* = Unit Under Calibration



REPORT OF CALIBRATION

Page 3 of 3

Certificate No. : 25-118065

Sample Code : 25-51697-001

Results of Calibration

Notes

1. Sensor installation locations
 - 1.1 All sensors at any corners or walls should be positioned 5 cm (a x b x c) from the wall.
 - 1.2 The reference sensor is preferably located of the geometric center of the chamber.
2. Interior dimensions approx of chamber :
W = 70 cm ; D = 55 cm ; H = 140 cm
3. Air valve or fresh air level : Off
4. Fan level : Open
5. The quoted uncertainty includes " Stability of chamber and loading effect in chamber at 20% of uniformity ".
6. Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
7. Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.
8. Overall variation - the difference of the maximum and the minimum measured temperatures throughout observation time.
9. UUC* reading - the average reading of indicating device that forms the integral part of the enclosure.
10. Calibration results without adjustment.

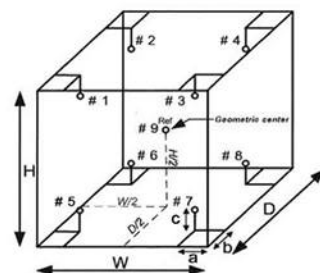


Figure: Example of sensor
installation Positions

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

- End of Report -



COPY

BOD INCUBATOR

Model : LABE 19/5

CERTIFICATE OF CALIBRATION

Page 1 of 3

Certificate No. : 25-042561

Sample Code : 25-18090-002

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapibarn 8 Rd., Nongkham,
Sriracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.
(Laboratory)

Equipment : Temperature controlled enclosures (Incubator)

Manufacturer : Lovibond Model : TC 445 S

Serial No. : 0520/005227 ID No. : LABE 19/5

Date of Receipt : 20 March 2025 Date of Calibration : 20 March 2025

Condition of Calibration

1. Environment
- 1.1 Ambient temperature : Maximum 29.9 °C ; Minimum 27.5 °C
- 1.2 Relative humidity : Maximum 51.9 % ; Minimum 43.4 %
- 1.3 Line voltage supplied : Maximum 239.4 VAC ; Minimum 232.8 VAC

2. Calibration method

TLAS-G-20: Guidelines for calibration and checks of temperature controlled enclosures.

3. Reference standard instrument

Instrument	ID No.	Certificate No.	Due Date
Data Acquisition With Sensor (RTD-P1100)	LB-DA-11 (RTD-148 to RTD-155, RTD-227)	24-040190	03 April 2025

4. This certificate is traceable to the international system of unit (SI Unit).

The measurement is traceable to Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by Mr. Pattanapong Pulngern
Scientist

Approved by

(Mr. Somchai Neampunt)

Signed for Director

Issue date 24 March 2025

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

REPORT OF CALIBRATION

Page 2 of 3

Certificate No. : 25-042561

Sample Code : 25-18090-002

Results of Calibration

Resolution : 0.1 °C

1. Reporting of Temperature

Calibration point (°C)	UUC* setting (°C)	UUC* reading (°C)	Measured temperature at each positions (°C)										Uncertainty ± (°C)	Coverage factor k
			#1	#2	#3	#4	#5	#6	#7	#8	#9 ^{ref}			
20	20.5	20.5	19.91	19.78	19.82	19.86	19.78	19.85	19.93	19.63	19.79		0.38	2.00

2. Characterization results

Calibration point (°C)	Stability ± (°C)	Uniformity (°C)	Overall variation (°C)
20	0.28	0.25	0.83

Notes

- UUC* = Unit Under Calibration



NSC-TISI-TISI17025
CALIBRATION 0152

Page 3 of 3

REPORT OF CALIBRATION

Certificate No. : 25-042561

Sample Code : 25-18090-002

Results of Calibration

Notes

1. Sensor installation locations
 - 1.1 All sensors at any corners or walls should be positioned 5 cm (a x b x c) from the wall.
 - 1.2 The reference sensor is preferably located of the geometric center of the chamber.
2. Interior dimensions approx of chamber :
W = 60 cm ; D = 56 cm ; H = 146 cm
3. Air valve or fresh air level : Off
4. Fan level : Open
5. The quoted uncertainty includes* Stability of chamber and loading effect in chamber at 20% of uniformity*.
6. Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
7. Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.
8. Overall variation - the difference of the maximum and the minimum measured temperatures throughout observation time.
9. UUC* reading - the average reading of indicating device that forms the integral part of the enclosure.
10. Calibration results without adjustment.

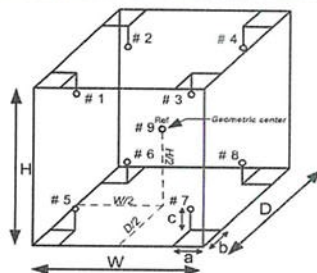


Figure: Example of sensor
installation Positions

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003

- End of Report -

COPY

BOD INCUBATOR

Model : LABE 19/5

CERTIFICATE OF CALIBRATION

Certificate No. : 26-031063

Sample Code : 26-013575-002

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.

683 Moo 11, Sukhapiarn 8 Rd., Nongkham,
Sriracha, Chonburi 20230Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.
(Laboratory)

Equipment : Temperature controlled enclosures (Incubator)

Manufacturer : Lovibond Model : TC 445 S

Serial No. : 0520/005227 ID No. : LABE 19/5

Date of Receipt : 24 February 2026 Date of Calibration : 24 February 2026

Condition of Calibration

1. Environment
- 1.1 Ambient temperature : Maximum 32.3 °C ; Minimum 30.1 °C
- 1.2 Relative humidity : Maximum 56.5 % ; Minimum 49.3 %
- 1.3 Line voltage supplied : Maximum 230.6 VAC ; Minimum 225.3 VAC

2. Calibration method

TLAS-G-20: Guidelines for calibration and checks of temperature controlled enclosures.

3. Reference standard instrument

Instrument	ID No.	Certificate No.	Due Date
Data Acquisition With Sensor (RTD-Pt100)	LB-DA-11 (RTD-441 to RTD-449)	25-040942	01 April 2026

4. This certificate is traceable to the international system of unit (SI Unit).

The measurement is traceable to Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by

Mr. Pattanapong Pulngern

Approved by

(Mr. Nuttaput Timula)

Issue date

27 February 2026

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

REPORT OF CALIBRATION

Certificate No. : 26-031063

Sample Code : 26-013575-002

Results of Calibration

Resolution : 0.1 °C

1. Reporting of Temperature

Calibration point (°C)	UUC* setting (°C)	UUC* reading (°C)	Measured temperature at each positions (°C)									Uncertainty ± (°C)	Coverage factor k
			#1	#2	#3	#4	#5	#6	#7	#8	#9 ^{ref}		
20	20.5	20.5	19.84	19.83	19.85	19.83	19.80	19.70	19.88	19.70	19.72	0.40	2.00

2. Characterization results

Calibration point (°C)	Stability ± (°C)	Uniformity (°C)	Overall variation (°C)
20	0.30	0.32	0.70

Notes

- UUC* = Unit Under Calibration




REPORT OF CALIBRATION

Certificate No. : 26-031063

Sample Code : 26-013575-002

Results of Calibration

Notes

1. Sensor installation locations
 - 1.1 All sensors at any corners or walls should be positioned 5 cm (a x b x c) from the wall.
 - 1.2 The reference sensor is preferably located of the geometric center of the chamber.
2. Interior dimensions approx of chamber :
W = 60 cm ; D = 56 cm ; H = 146 cm
3. Air valve or fresh air level : Off
4. Fan level : Open
5. The quoted uncertainty includes "Stability of chamber and loading effect in chamber at 20% of uniformity".
6. Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
7. Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.
8. Overall variation - the difference of the maximum and the minimum measured temperatures throughout observation time.
9. UUC* reading - the average reading of indicating device that forms the integral part of the enclosure.
10. Calibration results without adjustment.

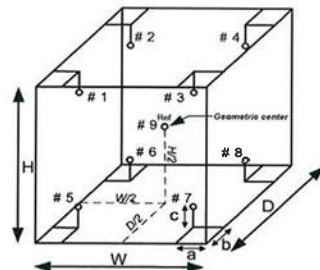


Figure: Example of sensor
installation Positions

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

- End of Report -

COPY

Hot Air Oven

Model : UM 400

Serial No. : 900982

NSC-TISI-TIS17025
CALIBRATION 0152

Page 1 of 3

CERTIFICATE OF CALIBRATION

Certificate No. : 25-215652

Sample Code : 25-94507-005

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapiarn 8 Rd., Nongkham,
Sriracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.
(Hot Lab)

Equipment : Temperature controlled enclosures (Hot air oven)

Manufacturer : Memmert Model : UM 400

Serial No. : 900982 ID No. : LABE 17/1

Date of Receipt : 16 December 2025 Date of Calibration : 16 December 2025

Condition of Calibration

1. Environment
- | | | | | |
|---------------------------|-----------|-----------|-----------|-----------|
| 1.1 Ambient temperature | : Maximum | 27.6 °C | ; Minimum | 26.4 °C |
| 1.2 Relative humidity | : Maximum | 61.4 % | ; Minimum | 54.0 % |
| 1.3 Line voltage supplied | : Maximum | 229.7 VAC | ; Minimum | 225.6 VAC |

2. Calibration method

TLAS-G-20: Guidelines for calibration and checks of temperature controlled enclosures.

3. Reference standard instrument

Instrument	ID No.	Certificate No.	Due Date
Data acquisition with sensor (RTD-Pt100)	LB-DA-20 (RTD-322 to RTD-330)	25-010526	18 February 2026

4. This certificate is traceable to the international system of unit (SI unit).

The measurement is traceable to Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by

Mr. Natthanan Phosri
Scientist

Approved by

(Mr. Somchai Neampunt)
Signed for Director

Issue date

17 December 2025

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

NSC-TISI-TIS17025
CALIBRATION 0152

Page 2 of 3

REPORT OF CALIBRATION

Certificate No. : 25-215652

Sample Code : 25-94507-005

Results of Calibration

Resolution : 0.1 °C

1. Reporting of Temperature

Calibration point (°C)	UUC* setting (°C)	UUC* reading (°C)	Measured temperature at each positions (°C)									Uncertainty ± (°C)	Coverage factor <i>k</i>
			# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9 ^{Ref}		
60	60.0	60.0	61.27	61.38	61.49	60.82	59.60	59.82	59.89	59.80	60.50	0.38	2.00
85	85.0	85.0	85.92	86.20	85.98	85.69	83.63	83.93	84.33	84.04	84.84	0.40	2.00

2. Characterization results

Calibration point (°C)	Stability ± (°C)	Uniformity (°C)	Overall variation (°C)
60	0.19	1.08	2.05
85	0.11	1.44	2.72

Notes

- UUC* = Unit Under Calibration

NSC-TISI-TISI17025
CALIBRATION 0152

REPORT OF CALIBRATION

Page 3 of 3

Certificate No. : 25-215652

Sample Code : 25-94507-005

Results of Calibration

Notes

1. Sensor installation locations
 - 1.1 All sensors at any corners or walls should be positioned 5 cm (a x b x c) from the wall.
 - 1.2 The reference sensor is preferably located of the geometric center of the chamber.
2. Interior dimensions approx of chamber :
W = 40 cm; D = 28 cm; H = 39 cm
3. Air valve or fresh air level : Off
4. Fan level : Open
5. The quoted uncertainty includes "Stability of chamber and loading effect in chamber at 20% of uniformity".
6. Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
7. Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.
8. Overall variation - the difference of the maximum and the minimum measured temperatures throughout observation time.
9. UUC* reading - the average reading of indicating device that forms the integral part of the enclosure.
10. Calibration results without adjustment.

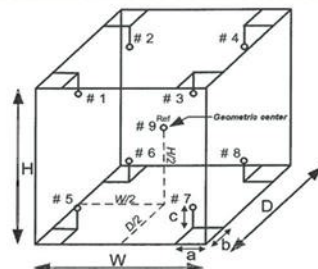


Figure: Example of sensor
installation Positions

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

- End of Report -

~~COPY~~

ICP-OES/Avio550

Serial No. : M81S2210101

ICP-OES/Avio550 Preventive Maintenance (PM)

Company Name:	Eastern Thai Consulting 1992 Cl.,Ltd.		
Address (Instrument Location):	683 Moo 11 Sukapibal 8 Rd. Nong Kham, Si Racha, Chonburi 20230		
Serial Number:	M8152210101	PM Number:	2 of 2
Customer Name (if applicable):		Telephone Number:	
Service Engineer Name:	Khwanchai	Service Order Number:	WO-06379056
Date PM Performed: (DD-MMM-YYYY)	20-Oct-2025	Next PM Due Date: (DD-MMM-YYYY)	20-Apr-2026
Standard Labor Hours to Complete PM :		4 hours	

Part Number	Release	Publication Date	
TH09370188 Rev.2	B	July 2020	

Scope

The purpose of this PM is to ensure the continued functionality of the PerkinElmer / Avio550 by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer. The customer should save their method before the PM begins.

General Instructions:

The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM.

Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files. The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer. Update the PM sticker and instrument logbook as required.

Copyright Information

This document contains proprietary information that is protected by copyright. All rights are reserved. No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of PerkinElmer, Inc. Copyright © 2013 PerkinElmer, Inc.

Trademarks

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners.

Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no Warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.

PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

Component List

Component / Specific Model	Serial #	Configuration Notes
NA	NA	NA

Parts Lists

Parts Included with the PM		
Part Number (if applicable)	Description	Quantity
09995098	Air Filter-Spectrometer	N/A
N077520	Air Filter-RF Generator	N/A
09992731	Axial Window	N/A
B0810377	Radial Window	N/A
N0770438	O-ring kit, injector support adapter	N/A
N0780437	O-ring kit, torch	N/A

Additional Reagents and Standards Required for PM				
Part Number (if applicable)	Description	Quality	Batch/Lot #	Expiry Date (MM/YY)
N0691579	Muti-Element Standard	AR	64-247CRX1	11/2026
N9300221	DL Standard diluted 100 X	AR	65-009CRY1	11/2026
N0582152	Wave Cal Solution	AR	64-241CRX1	07/2026
N9302946	VIS Wavecal Solution	AR	62-183CRT1	08/2026

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. General:

- ☒ Ask customer about unit's performance since last visit.
- ☒ Check incoming AC line voltage under load for proper levels and grounding.
- ☒ Is the instrument operational? if not, please comment.

2. Mechanical:

- ☒ Inspect and clean all fans and filters.
- ☒ Inspect and replace torch components and necessary.

Torch Components Replaced: ☐ Yes ☒ No

- ☐ Inspect all tubing for signs of cracking or leaking and replace as necessary.

Tubing Replaced: ☐ Yes ☒ No

- ☒ Inspect the peristaltic pump for proper operation.
- ☒ Check and adjust if necessary, the external nitrogen, argon shear gas and water supply pressures.
- ☒ Check and adjust if necessary, the internal nitrogen, main argon, torch argon and shear gas pressures.

Regulator	Measured Pressure	Set Pressure
Nitrogen	NA	NA (calibrated in factory)
Main Argon	76	76 psig
Torch Argon	67	67 psig
Shear Gas	65	65 psig
Water	35	35 psig

- ☒ Check shear gas nozzle for blockages and proper, uniform flow.
- ☒ Inspect nitrogen Hi/Low purge and shear gas solenoids for proper function.
- ☒ Inspect the function of all spectrometer motors. Drive the motors from the Spectrometer DCM. (slits, XY motor)
- ☒ Inspect the function of the pneumatic shutter for proper operation.
- ☒ Perform preventative maintenance on the chiller as required. Make the customer aware of the importance of maintaining the chiller fluid level and filter replacement.
- ☒ Drain air compressor surge tank.
- ☒ Clean exterior of instrument.
- ☒ Visually inspect all PC boards for cleanliness and signs of corrosion.

COPY

3. Electronical

- ☒ Check all RF generator and spectrometer power supply voltages.
- ☒ Run instrument diagnostic checks from the appropriate Device Control Module.

RF Generator:

- ☒ Check the RF generator status screens.
- ☒ Check the function of all interlocks.

Spectrometer:

- ☒ Check the spectrometer status screens. Ensure Ready mode with no fatal errors.
- ☒ Check the spectrometer optical tub temperatures (top, bottom, fin, optical base).
- ☒ Check detector temperatures.
- ☒ Check TEC voltages (6.5VDC)

4. Optical:

- ☒ Clean or replace the axial and radial view windows as necessary.

Axial Window Replaced: ☐ Yes ☒ No
Radial Window Replaced: ☐ Yes ☒ No

5. PM Performance Tests:

- ☒ Perform View Align.

Test Spectral Resolution:

- ☒ Measure the spectrometers ability to separate two adjacent wavelengths.

Parameter	Specification	Test Result	Pass/Fail
As 193.696 - Resolution	≤0.007	0.00531	Passed
Ni 231.604 - Resolution	≤0.008	0.00716	Passed
Ni 341.476 - Resolution	≤0.012	0.00891	Passed
La 408.672 - Resolution	≤0.020	0.01629	Passed
Ba 455.403 - Resolution	≤0.025	0.02144	Passed

Test Precision:

- ☒ Test for reproducibility of a set of measurement.

Parameter	Specification	Test Result	Pass/Fail
As 193.696	%RSD ≤ 1 %	0.34	Passed
Zn 213.856	%RSD ≤ 1 %	0.38	Passed
Mn 257.610	%RSD ≤ 1 %	0.28	Passed
La 379.478	%RSD ≤ 1 %	0.24	Passed
Ba 455.403	%RSD ≤ 1 %	0.26	Passed
Ba 493.408	%RSD ≤ 1 %	0.28	Passed

COPY

- ☒ Run an Axial & Radial BEC according to the A&T spec.

Test Axial BEC Cd:

Method "BEC-XL" For Samples "IB (2%HNO3)" and "IS (N930-0221/100)", record intensities.

Calculated BEC: $BEC = (IB * Conc\ of\ Std) / (IS - IB)$. Where Conc of Std = 500 PPB

Element	Conc.	IB	IS	
Cd 226	500	1687.2	359486.8	
IB*Conc	IS-IB	BEC	Spec	Pass/Fail
843600	357799.6	2.36	<150 PPB	Passed

Test Radial BEC Mn:

Method "BEC-RL" For Samples "IB (2%HNO3)" and "IS (N069-1579)", record intensities.

Calculated BEC: $BEC = (IB * Conc\ of\ Std) / (IS - IB)$. Where Conc of Std = 1,000 PPB

Element	Conc.	IB	IS	
Mn 257	1,000	1744.4	255911.4	
IB*Conc	IS-IB	BEC	Spec	Pass/Fail
1744400	254167	6.86	<45 PPB	Passed

6. Review:

- ☒ Review with the customer PM work performed.
☒ Discuss recommended customer supplied materials to have on hand.
☒ Attach PM sticker.

COPY

Additional Comments

Additional Comments Regarding the PM

None

Review

The preventive maintenance checks and if applicable performance tests for ICP-OES/Avio550 have been completed.

This ICP-OES/Avio550 Passes ☒ Fails ☐ the preventive maintenance.

Review of Preventive Maintenance:

Authorized PerkinElmer Representative:	<i>KLS.</i>	Date: 20-Oct-2025 (DD-MMM-YYYY)
Authorized Customer Representative:	<i>601225516</i>	Date: 20-Oct-2025 (DD-MMM-YYYY)

COPY

ICP-OES/Avio550

Serial No. : M81S221010

ICP-OES/Avio500 Preventive Maintenance (PM)

Company Name:	Eastern Thai Consulting 1992 Co.,Ltd		
Address (Instrument Location):	683 Moo 11, Nong Kham Subdistrict, Si Racha District, Chonburi		
Serial Number:	M815221010	PM Number:	1 of 2
Customer Name (if applicable):	Channarong	Telephone Number:	0968761232
Service Engineer Name:	Khwanchai	Service Order Number:	WO-11759162
Date PM Performed: (DD-MMM-YYYY)	08-Apr-2026	Next PM Due Date: (DD-MMM-YYYY)	08-Oct-2026
Standard Labor Hours to Complete PM :		4 hours	

Part Number	Release	Publication Date	
TH09370188 Rev.1	B	July 2020	

Scope

The purpose of this PM is to ensure the continued functionality of the PerkinElmer / Avio500 by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer. The customer should save their method before the PM begins.

General Instructions:

The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM.

Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files. The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer. Update the PM sticker and instrument logbook as required.

Copyright Information

This document contains proprietary information that is protected by copyright. All rights are reserved. No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of PerkinElmer, Inc. Copyright © 2013 PerkinElmer, Inc.

Trademarks

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners.

Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no Warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.

PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

Component List

Component / Specific Model	Serial #	Configuration Notes

Parts Lists

Parts Included with the PM		
Part Number (if applicable)	Description	Quantity
09995098	Air Filter-Spectrometer	1
N077520	Air Filter-RF Generator	1
09992731	Axial Window	1
B0810377	Radial Window	1
N0770438	O-ring kit, injector support adapter	1
N0780437	O-ring kit, torch	1

Additional Reagents and Standards Required for PM				
Part Number (if applicable)	Description	Quality	Batch/Lot #	Expired Date (MM/YY)
N0691579	Muti-Element Standard	AR	64-247CRX1	Nov-2026
N9300221	DL Standard diluted 100 X	AR	65-009CRY1	Nov-2026
N0582152	Wave Cal Solution	AR	64-241CRX1	Jul-2026
N9302946	VIS Wavecal Solution	AR	62-183CRT1	Sep-2026

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. General:

- ☒ Ask customer about unit's performance since last visit.
- ☒ Check incoming AC line voltage under load for proper levels and grounding.
- ☒ Is the instrument operational? If not, please comment.

2. Mechanical:

- ☒ Inspect and clean all fans and filters.
- ☒ Inspect and replace torch components and necessary.

Torch Components Replaced: ☒ Yes ☐ No

- ☒ Inspect all tubing for signs of cracking or leaking and replace as necessary.

Tubing Replaced: ☐ Yes ☒ No

- ☒ Inspect the peristaltic pump for proper operation.
- ☒ Check and adjust if necessary, the external nitrogen, argon shear gas and water supply pressures.
- ☒ Check and adjust if necessary, the internal nitrogen, main argon, torch argon and shear gas pressures.

Regulator	Measured Pressure	Set Pressure
Nitrogen		NA (calibrated in Factory)
Main Argon	76	76 psig
Torch Argon	67	67 psig
Shear Gas	65	65 psig
Water	35	35 psig

- ☒ Check shear gas nozzle for blockages and proper, uniform flow.
- ☒ Inspect nitrogen Hi/Low purge and shear gas solenoids for proper function.
 - ☒ Inspect the function of all spectrometer motors. Drive the motors from the Spectrometer DCM. (slits, XY motor)
- ☒ Inspect the function of the pneumatic shutter for proper operation.
 - ☒ Perform preventative maintenance on the chiller as required. Make the customer aware of the importance of maintaining the chiller fluid level and filter replacement.
- ☒ Drain air compressor surge tank.
- ☒ Clean exterior of instrument.
- ☒ Visually inspect all PC boards for cleanliness and signs of corrosion.

~~COPY~~

3. Electronical

- ☒ Check all RF generator and spectrometer power supply voltages.
- ☒ Run instrument diagnostic checks from the appropriate Device Control Module.

RF Generator:

- ☒ Check the RF generator status screens.
- ☒ Check the function of all interlocks.

Spectrometer:

- ☒ Check the spectrometer status screens. Ensure Ready mode with no fetal errors.
- ☒ Check the spectrometer optical tub temperatures (top, bottom, fin, optical base).
- ☒ Check detector temperatures.
- ☒ Check TEC voltages (6.5VDC)

4. Optical:

- ☒ Clean or replace the axial and radial view windows as necessary.
 - Axial Window Replaced: ☒ Yes ☐ No
 - Radial Window Replaced: ☒ Yes ☐ No

5. PM Performance Tests:

- ☒ Perform View Align.

Test Spectral Resolution:

- ☒ Measure the spectrometers ability to separate two adjacent wavelengths.

Parameter	Specification	Test Result	Pass/Fail
As 193.696 - Resolution	≤0.007	0.00523	Passed
Ni 231.604 - Resolution	≤0.008	0.00741	Passed
Ni 341.476 - Resolution	≤0.012	0.00902	Passed
La 408.672 - Resolution	≤0.020	0.01570	Passed
Ba 455.403 - Resolution	≤0.025	0.02150	Passed

Test Precision:

- ☒ Test for reproducibility of a set of measurement.

Parameter	Specification	Test Result	Pass/Fail
As 193.696	%RSD ≤ 1 %	0.32	Passed
Zn 213.856	%RSD ≤ 1 %	0.25	Passed
Mn 257.610	%RSD ≤ 1 %	0.29	Passed
La 379.478	%RSD ≤ 1 %	0.31	Passed
Ba 455.403	%RSD ≤ 1 %	0.33	Passed
Ba 493.408	%RSD ≤ 1 %	0.37	Passed

~~COPY~~

- ☒ Run an Axial & Radial BEC according to the A&T spec.

Test Axial BEC Cd:

Method "BEC-XL" For Samples "IB (2%HNO3)" and "IS (N930-0221/100)", record intensities.

Calculated BEC: $BEC = (IB * Conc\ of\ Std) / (IS - IB)$. Where Conc of Std = 500 PPB

Element	Conc.	IB	IS	
Cd 226	500	931.0	202313.1	
IB*Conc	IS-IB	BEC	Spec	Pass/Fail
465500	201382.1	2.31	<150 PPB	Passed

Test Radial BEC Mn:

Method "BEC-RL" For Samples "IB (2%HNO3)" and "IS (N069-1579)", record intensities.

Calculated BEC: $BEC = (IB * Conc\ of\ Std) / (IS - IB)$. Where Conc of Std = 1,000 PPB

Element	Conc.	IB	IS	
Mn 257	1,000	717.1	255339.9	
IB*Conc	IS-IB	BEC	Spec	Pass/Fail
717100	254622.8	2.82	<45 PPB	Passed

6. Review:

- ☒ Review with the customer PM work performed.
☒ Discuss recommended customer supplied materials to have on hand.
☒ Attach PM sticker.

~~COPY~~

Additional Comments

Additional Comments Regarding the PM

- Use with Sample introduction AQ for PM test

Review

The preventive maintenance checks and if applicable performance tests for ICP-OES/Avio500 have been completed.

This ICP-OES/Avio500 **Passes** ☒ **Fails** ☐ *the preventive maintenance.*

Review of Preventive Maintenance:

Authorized PerkinElmer Representative: <i>KL.S.</i>	Date: 08-Apr-2026 (DD-MMM-YYYY)
Authorized Customer Representative: <i>กิติ</i>	Date: 08-Apr-2026 (DD-MMM-YYYY)

~~COPY~~

LIQUID IN GLASS THERMOMETER

Model / Type : 0-100 °C

Serial No. : 43560



CALIBRATION LABORATORY CO.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : LIQUID IN GLASS THERMOMETER
MANUFACTURER : AA PRECISION
MODEL / TYPE : 0-100 °C
SERIAL NO. : 43560[LABE 16/1]
CLID. NO. : 232403905
JOB CONTROL NO. : 251115135334
CALIBRATION SERVICE : ☒ IN-LABORATORY ☐ ON-SITE

CUSTOMER : EASTERN THAI CONSULTING 1992 CO., LTD.
683 MOO 11, SUKHAPIBARN 8 RD,
NONGKHAM, SRIRACHA, CHONBURI 20230

DATE OF RECEIVED : 15 November 2025 DATE OF ISSUED : 18 November 2025

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Pimsiri Hemtanon
Calibration Engineer

Approved By : Mongkol Yotsoontorn
Authorized Signatory
18 November 2025



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q25135334

F3-011-05/12-23

COPY



@clccalibration



CALIBRATION LABORATORY CO.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



REPORT OF CALIBRATION

FOR

NOMENCLATURE : LIQUID IN GLASS THERMOMETER
MANUFACTURER : AA PRECISION
MODEL / TYPE : 0-100 °C
SERIAL NO. : 43560[LABE 16/1]
DATE OF CALIBRATION : 17 November 2025

ENVIRONMENT CONDITIONS :

Temperature : $(23 \pm 2) ^\circ\text{C}$ Relative Humidity : $(55 \pm 10) \%$

PROCEDURE USED :

This instrument was calibrated under procedure No. CLC-CPTH-02 based on ASTM E 77-07 as calibration guidelines.
The calibration was performed by comparison with Calibration Bath, Precision Thermometer and IPRT which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. Calibration Bath, Kambic Model OB-22/2 ULT,OB-22/2 S/N. 17115653,17115654.
2. Precision Thermometer, ASL Model F200-A-8 S/N. 014433/03 with IPRT S/N. L0193A-1-1,PO106346-1-13.

TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q24120999,Q25124610. Due Date 26 November 2025,07 November 2026.
2. The measurements are traceable to International System of Units (SI), through Thailand Institute of Scientific and Technological Research (TISTR) and National Institute of Metrology (Thailand). Certificate No. PSL-T 0177/68,TT-0169-24,TT-1008-25. Due Date 10 February 2026,11 December 2025,04 March 2026.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2$ which for a normal distribution corresponds to a coverage probability of approximately 95 %. It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q25135334

F3-011-05/12-23

COPY



@clccalibration



CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The DUC Reading were recorded and the means value were reported of four times measurement in the table below.

CALIBRATION DATA

CORRECTION OF TEMPERATURE

STD Reading (°C)	DUC Reading (°C)	Correction (°C)	Uncertainty $\pm$ (°C)
0.01	0.00	+0.01	0.06
25.02	25.00	+0.02	
50.03	50.00	+0.03	
100.01	100.00	+0.01	

Range : 0 °C to 100 °C

Graduation : 0.1 °C

Immersion Type : Total Immersion.

Correction of Reference Temperature (0 °C) = 0.00 °C

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 016 Page 60 of 73

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q25135334

F3-011-05/12-23

COPY



@clccalibration

pH Meter

Model : SevenCompact S220

Serial No. : B448305208

NSC-TISI-TIS17025
CALIBRATION 0152

Page 1 of 3

CERTIFICATE OF CALIBRATION

Certificate No. : 25-215648

Sample Code : 25-94507-001

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapibarn 8 Rd., Nongkham,
Sriracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.
(Laboratory)

Equipment : pH Meter

Manufacturer : METTLER TOLEDO **Model** : SevenCompact S220

Serial No. : B448305208 **ID No.** : LABE 11/4

Date of Receipt : 18 December 2025 **Date of Calibration** : 16 December 2025

Condition of Calibration

1. **Environment** Ambient temperature : 15.0 to 35.0 °C Relative humidity : 35.0 to 80.0 %RH
1.1 Start time : 23.3 °C ; End time : 24.0 °C 1.2 Start time : 46.7 %RH ; End time : 45.8 %RH

2. Calibration method

In house method WI-CL-019 : Direct measurement with standard voltage calibrator and direct measurement with certified reference material (CRM).

3. Reference standard / Certified reference material

Instrument	ID No.	Certificate No.	Due Date
3.1 Voltage Calibrator	LB-DPC-01	LF25-0350	22 June 2026
3.2 Digital Thermometer	LB-DPC-01	25-141888	29 July 2026
Certified Reference Material		Lot. No.	Expire Date
3.3 Buffer Solution pH 4.008	1174256	PH216.L5	13 December 2027
3.4 Buffer Solution pH 7.000	C03292	S11M004	14 July 2027
3.5 Buffer Solution pH 10.010	1174257	PH220.L5	13 December 2026

4. This certificate is traceable to the international system of unit (SI Unit).

- 4.1 Instrument No. 3.1 through Measuretronix Limited.
- 4.2 Instrument No. 3.2 through Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.
- 4.3 Buffer Solution No. 3.3 and No. 3.5 traceable to CPA chem (through primary measurement method-Harned cell using calibrated thermometer, barometer, and nanovoltmeter Accredited laboratory ISO/IEC 17025 and ISO 17034).
- 4.4 Buffer Solution No. 3.4 traceable to HACH (Certified Reference Material from PTB Certificate Nr. PTB-PHOA-563/30504/23 and Certificate Nr. PTB-PHOB-555/30620/22. According to DIN EN ISO 17034:2017).

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by Mr. Chakrin Chiangsorn
Scientist

Approved by

(Mr. Somchai Neampunt)
Signed for Director

Issue date

18 December 2025

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

NSC-TISI-TIS17025
CALIBRATION 0152

Page 2 of 3

REPORT OF CALIBRATION

Certificate No. : 25-215648

Sample Code : 25-94507-001

Equipment : pH Meter **Resolution** : 0.01 pH ; 0.1 mV ; 0.1 °C

Manufacturer : METTLER TOLEDO **Model** : SevenCompact S220

Serial No. : B448305208 **ID No.** : LABE 11/4

Range : -2.000 pH to 20.000 pH ; -2000.0 mV to 2000.0 mV ; -5.0°C to 130.0°C

Results of Calibration

Part 1. DC Voltage measurement

pH Meter Serial No. : B448305208

Nominal Value	Applied DC Voltage	Average indicator reading		Uncertainty	Coverage factor
		mV	pH		
0	414.113	414.0	0.00	± 0.083	2.00
4	177.477	177.5	4.00	± 0.083	2.00
7	0.000	0.1	7.00	± 0.083	2.00
10	-177.477	-177.3	10.00	± 0.083	2.00
14	-414.113	-413.8	14.00	± 0.083	2.00

Part 2. Performance of Electrode system

Electrode Manufacturer : METTLER TOLEDO Model : InLab Expert Pro-ISM

Electrode Serial No. : 4290677

Three-Point Calibration at pH4 and pH7 Percent Slope : 99.2 , at pH7 and pH10 Percent Slope : 99.7

Standard Buffer Solution	Average indicator reading		Error Value	Uncertainty	Coverage factor
	pH	mV			
pH (@ 25 °C)			pH	pH	k
4.008	4.02	163.7	0.012	± 0.0093	2.00
7.000	7.01	-11.6	0.010	± 0.0093	2.00
10.010	10.00	-187.7	-0.010	± 0.0099	2.00

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

NSC-TISI-TIS17025
CALIBRATION 0152

Page 3 of 3

REPORT OF CALIBRATION

Certificate No. : 25-215648

Sample Code : 25-94507-001

Equipment : pH Meter (Digital Thermometer with sensor)

Thermometer readout

Manufacturer : METTLER TOLEDO Model : SevenCompact S220
Serial No. : B448305208 ID No. : LABE 11/4
Resolution : 0.1 °C Range : -5.0 °C to 130.0 °C

Thermometer sensor

Manufacturer : METTLER TOLEDO Model : InLab Expert Pro-ISM
Serial No. : 4290677 ID No. : N/A

Condition of Calibration

1. Environment 1.1 Ambient temperature : 24.1 °C ± 0.0 °C
1.2 Relative humidity : 45.0 % ± 0.2 %

2. Calibration method

- 2.1 The calibration use in house method WI-CL-021 : by comparison with standard thermometer
2.2 The calibration by comparison unit under calibration (UUC) to the standard thermometer in a calibration bath at the controlled temperature.
2.3 The temperature scale in use of this laboratory is the international temperature scale of 1990 (ITS-90).

3. Reference standard instrument

Instrument	Model	ID. No.	Certificate No.	Due date
3.1 Resistance Thermometer	PT-100	RTD-366	25-141888	29 July 2026
3.2 Thermometer Readout	753	LB-DPC-01	25-141888	29 July 2026

4. This certificate is traceable to the international system of unit (SI Unit).

Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (Accreditation Under TLAS Laboratory Calibration No.0152)

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of Calibration item : Normal

Results of Calibration

Calibration point °C	Average of standard reading °C	Unit under calibration			Expanded uncertainty °C	Coverage factor k
		Immersion depth mm	Average reading °C	Correction value °C		
25	25.00	100	24.9	+ 0.10	± 0.14	2.00

Notes

- Calibration results without adjustment

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

- End of report -

STANDARD WEIGHT 50 g

Certificate No. : 24-062445
Sample Code : 24-25551-001

CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapibarn 8 Rd., Nongkham,
Sriracha, Chonburi 20230

Location of Calibration : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited
(Calibration Laboratory)

Equipment : Standard Weight 50 g

Manufacturer : METTLER TOLEDO

Class : F1

Serial No. : N/A

ID No. : LABE 10/1

Date of Receipt : 23 May 2024

Date of Calibration : 03 June 2024

Calibrated by Mr. Somwang Sangdee
Scientist

Issue date 04 June 2024

Approved by (Mr. Somchai Neampunt)
Signed for Director

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

Certificate No. : 24-062445
Sample Code : 24-25551-001

REPORT OF CALIBRATION

Equipment : Standard Weight 50 g

Manufacturer : METTLER TOLEDO

Class : F1

Serial No. : N/A

ID No. : LABE 10/1

Result of Calibration : ☒ Without adjustment ☐ Adjustment

Conventional value of the result of weighing in air. For a weight taken at a reference temperature (t_{ref}) of 20°C, the conventional mass is the mass of a reference weight of a density (ρ_{ref}) of 8000 kg.m⁻³ which it balances in air of a reference density (ρ_0) of 1.2 kg.m⁻³

Description	Deviation (mg)	Conventional Mass	Expanded Uncertainty (mg)	Maximum Permissible Error $\pm$ (mg)	ID No.
50 g	-0.343	49.999657 g	0.10	0.30	LABE 10/1

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2.0$, which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003

COPY

Certificate No. : 24-062445

Sample Code : 24-25551-001

Page 3 of 3

REPORT OF CALIBRATION

Condition of Calibration

1. Ambient Conditions : Temperature $20^{\circ}\text{C} \pm 1.5^{\circ}\text{C}$, Relative humidity $50\% \pm 10\%$ and air density 1.19 kg/m^3

2. Calibration Method : Direct comparison weighing according to OIML R111-1 : 2004(E)

3. Reference standard instrument

Instrument	Class	ID No.	Certificate No.	Due Date
1) Standard Weight 1 mg to 1 kg	E2	LB-WE-83	24-001894	11 January 2025

4. This certification is traceable to the International System of Unit maintained at : -

Asia Medical and Agricultural Laboratory and Research Center Public Company Limited

(Instrument number 1).

5. Condition of Calibration item: Normal

6. Description of Calibrated item :

Type and Nominal Value :	Standard Weight 50 g
Shape :	Cylindrical weight with knob
Material :	Stainless steel
Case :	Wooden Box
Comments :	Recalibration

- End of Report -



STANDARD WEIGHT 100 g

Certificate No. : 24-079772
Sample Code : 24-31841-002

CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapibarn 8 Rd., NongKham,
Sriracha, Chonburi 20230

Location of Calibration : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited
(Calibration Laboratory)

Equipment : Standard Weight 100 g

Manufacturer : N/A

Class : N/A

Serial No. : N/A

ID No. : LABE 10/2

Date of Receipt : 25 June 2024

Date of Calibration : 30 June 2024

Calibrated by Mr. Nawa Sisuwan
Scientist

Approved by (Mr. Somchai Neampunt)
Signed for Director

Issue date 03 July 2024

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

Certificate No. : 24-079772
Sample Code : 24-31841-002

REPORT OF CALIBRATION

Equipment : Standard Weight 100 g

Manufacturer : N/A

Class : N/A

Serial No. : N/A

ID No. : LABE 10/2

Result of Calibration :

☒ Without adjustment☐ Adjustment

Conventional value of the result of weighing in air. For a weight taken at a reference temperature (t_{ref}) of 20°C, the conventional mass is the mass of a reference weight of a density (ρ_{rel}) of 8000 kg.m⁻³ which it balances in air of a reference density (ρ_0) of 1.2 kg.m⁻³

Description	Deviation	Conventional	Expanded	Maximum	ID No.
	(mg)	Mass	Uncertainty	Permissible Error	
			(mg)	± (mg)	
100 g	-0.173	99.999827 g	0.16	0.50	LABE 10/2

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2.0$, which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003

COPY

Certificate No. : 24-079772
Sample Code : 24-31841-002

Page 3 of 3

REPORT OF CALIBRATION

Condition of Calibration

1. Ambient Conditions : Temperature $20^{\circ}\text{C} \pm 1.5^{\circ}\text{C}$, Relative humidity $50\% \pm 10\%$ and air density 1.19 kg/m^3

2. Calibration Method : WI-CL-007 base on OIML R 111-1 : 2004(E)

3. Reference standard instrument

Instrument	Class	ID.No.	Certificate No.	Due Date
1) Standard Weight 1 mg to 1 kg	E2	LB-WE-83	24-001894	11 January 2025

4. This certification is traceable to the International System of Unit maintained at : -

Asia Medical and Agricultural Laboratory and Research Center Public Company Limited

(Instrument number 1).

5. Condition of Calibration item: Normal

6. Description of Calibrated Item :

Type and Nominal Value :	Standard Weight 100 g
Shape :	Cylindrical weight with knob
Material :	Stainless steel
Case :	Wooden Box
Comments :	Recalibration

- End of Report -

COPY

STANDARD WEIGHT 50 g

Certificate No. : 24-079773
Sample Code : 24-31841-003

CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapibarn 8 Rd., NongKham,
Sriracha, Chonburi 20230

Location of Calibration : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited
(Calibration Laboratory)

Equipment : Standard Weight 50 g

Manufacturer : N/A

Class : N/A

Serial No. : N/A

ID No. : LABE 10/4

Date of Receipt : 25 June 2024

Date of Calibration : 30 June 2024

Calibrated by Mr. Nawa Sisuwan
Scientist

Approved by (Mr. Somchai Neampunt)
Signed for Director

Issue date 03 July 2024

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

Certificate No. : 24-079773
Sample Code : 24-31841-003

REPORT OF CALIBRATION

Equipment : Standard Weight 50 g

Manufacturer : N/A

Class : N/A

Serial No. : N/A

ID No. : LABE 10/4

Result of Calibration : ☒ Without adjustment ☐ Adjustment

Conventional value of the result of weighing in air. For a weight taken at a reference temperature (t_{ref}) of 20°C, the conventional mass is the mass of a reference weight of a density (ρ_{ref}) of 8000 kg.m⁻³ which it balances in air of a reference density (ρ_0) of 1.2 kg.m⁻³

Description	Deviation	Conventional	Expanded	Maximum	ID No.
	(mg)	Mass	Uncertainty	Permissible Error	
			(mg)	± (mg)	
50 g	-0.176	49.999824 g	0.10	0.30	LABE 10/4

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2.0$, which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003

COPY

Certificate No. : 24-079773

Sample Code : 24-31841-003

Page 3 of 3

REPORT OF CALIBRATION

Condition of Calibration

1. Ambient Conditions : Temperature $20^{\circ}\text{C} \pm 1.5^{\circ}\text{C}$, Relative humidity $50\% \pm 10\%$ and air density 1.19 kg/m^3

2. Calibration Method : WI-CL-007 base on OIML R 111-1 : 2004(E)

3. Reference standard instrument

Instrument	Class	ID No.	Certificate No.	Due Date
1) Standard Weight 1 mg to 1 kg	E2	LB-WE-83	24-001894	11 January 2025

4. This certification is traceable to the International System of Unit maintained at : -

Asia Medical and Agricultural Laboratory and Research Center Public Company Limited

(Instrument number 1).

5. Condition of Calibration item: Normal

6. Description of Calibrated Item :

Type and Nominal Value :	Standard Weight 50 g
Shape :	Cylindrical weight with knob
Material :	Stainless steel
Case :	Wooden Box
Comments :	Recalibration

- End of Report -



COPY

THERMO-HYGROMETER

Model : 608-H1

Serial No. : 45106737

CERTIFICATE OF CALIBRATION

Page 1 of 2

Certificate No. : 25-090091

Sample Code : 25-39161-001

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.

683 Moo 11, Sukhaphibarn 8 Rd., Nongkham,

Sriracha, Chonburi 20230

Location of Calibration : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited
(Calibration laboratory)

Equipment : Digital thermo-hygrometer

Manufacturer : testo

Model : 608-H1

Serial No. : 45106737

ID No. : LABE 09/7

Date of Receipt : 21 May 2025

Date of Calibration : 23 May 2025

Condition of Calibration

1. Environment
- 1.1 Ambient temperature : 23.0 °C ± 3.0 °C
- 1.2 Relative humidity : 55.0 % ± 15.0 %

2. Calibration method

- 2.1 In-house method: WI-CL-045 By comparison with thermometer standard / chilled mirror hygrometer in controlled chamber.
- 2.2 The calibration by comparison unit under calibration (UUC) to the thermometer standard / chilled mirror hygrometer in a chamber at the controlled temperature / relative humidity.

3. Reference standard instrument

Instrument	Model	ID No.	Certificate No.	Due Date
3.1 Chilled Mirror	Optidew 401	LB-DP-03 & LB-DP-03 (DP)	TH-0122-24	25 September 2025
3.2 Digital Thermometer	Optidew 401	LB-DP-03 & LB-DP-03 (Temp.)	24-138856	28 October 2025
3.3 Digital Thermometer	34972A	LB-DA-07 with RTD-89	24-106857	21 August 2025

4. This certificate is traceable to the international system of unit (SI Unit).

- 4.1 Instrument No. 3.1 through National Institute of Metrology (Thailand).
- 4.2 Instrument No. 3.2 and 3.3 through Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by

Miss Pornsuda Lohabal

Approved by

(Mr. Somchai Neampunt)

Scientist

Signed for Director

Issue date

26 May 2025

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

361 Soi Ladprao 122, Ladprao Road,
Phlabphla, Wang Thonglang, Bangkok 10310
FM-CL-0114

TEL 02-516-2422
FAX 02-516-6949
Rev 01

CONTACT@AMARC.CO.TH
WWW.AMARC.CO.TH
Effective Date: 15/10/21

REPORT OF CALIBRATION

Page 2 of 2

Certificate No. : 25-090091

Sample Code : 25-39161-001

Results of Calibration

Temperature measurement

Resolution : 0.1 °C

Range : 0 °C to 50 °C

Calibration point °C	Average of standard reading		Unit under calibration		uncertainty °C
	Controlled humidity %RH	Temperature °C	Average reading °C	Correction value °C	
20	50	20.01	20.2	- 0.19	± 0.39
25	50	25.01	25.0	+ 0.01	± 0.39
30	50	30.01	30.0	+ 0.01	± 0.39

Humidity measurement

Resolution : 0.1 %RH

Range : 10 %RH to 95 %RH

Calibration point %RH	Average of standard reading		Unit under calibration		uncertainty %RH
	Air temperature °C	Calculated humidity %RH	Average reading %RH	Correction value %RH	
45	25.02	45.10	50.2	- 5.10	± 1.3
60	25.02	60.15	65.2	- 5.05	± 1.5
75	25.02	75.01	82.1	- 7.09	± 1.7

Notes

- Calibration results without adjustment.

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2.00$, which for a normal distribution corresponds to a coverage probability of approximately 95%. This standard uncertainty of measurement has been determined in accordance with UKAS M3003.

- End of Report -

COPY

361 Soi Ladprao 122, Ladprao Road,
Phlabphla, Wang Thonglang, Bangkok 10310
FM-CL-0114

TEL 02-516-2422
FAX 02-516-6949
Rev 01

CONTACT@AMARC.CO.TH
WWW.AMARC.CO.TH
Effective Date: 15/10/21

THERMO-HYGROMETER

Model : 608-H1

Serial No. : 45106737

CERTIFICATE OF CALIBRATION

Certificate No. : 26-072409

Sample Code : 26-030912-002

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapibarn 8 Rd., Nongkham,
Sriracha, Chonburi 20230

Location of Calibration : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited
(Calibration laboratory)

Equipment : Digital thermo-hygrometer

Manufacturer : testo

Model : 608-H1

Serial No. : 45106737

ID No. : LABE 09/7

Date of Receipt : 30 April 2026

Date of Calibration : 06 May 2026

Condition of Calibration

1. Environment
- 1.1 Ambient temperature : 23.0 °C ± 3.0 °C
- 1.2 Relative humidity : 55.0 % ± 15.0 %

2. Calibration method

- 2.1 In-house method: WI-CL-045 By comparison with thermometer standard / chilled mirror hygrometer in controlled chamber.
- 2.2 The calibration by comparison unit under calibration (UUC) to the thermometer standard / chilled mirror hygrometer in a chamber at the controlled temperature / relative humidity.

3. Reference standard instrument

Instrument	Model	ID No.	Certificate No.	Due Date
3.1 Chilled Mirror	Optidew 401	LB-DP-04 & LB-DP-04 (DP)	TH-0045-25	22 July 2026
3.2 Digital Thermometer	Optidew 401	LB-DP-04 & LB-DP-04 (Temp.)	25-157165	19 August 2026
3.3 Digital Thermometer	34972A	LB-DA-07 with RTD-89	25-115069	18 August 2026

4. This certificate is traceable to the international system of unit (SI Unit).

- 4.1 Instrument No. 3.1 through National Institute of Metrology (Thailand).
- 4.2 Instrument No. 3.2 and 3.3 through Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by

Miss Pornsuda Lohabal

Approved by

(Mr. Nuttaput Timula)

Scientist

Signed for Director

Issue date

08 May 2026

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

REPORT OF CALIBRATION

Certificate No. : 26-072409

Sample Code : 26-030912-002

Results of Calibration

Temperature measurement

Resolution : 0.1 °C

Range : 0 °C to 50 °C

Calibration point °C	Average of standard reading		Unit under calibration		uncertainty °C
	Controlled humidity %RH	Temperature °C	Average reading °C	Correction value °C	
20	50	20.00	19.9	+ 0.10	± 0.39
25	50	25.00	24.9	+ 0.10	± 0.39
30	50	30.02	29.8	+ 0.22	± 0.39

Humidity measurement

Resolution : 0.1 %RH

Range : 10 %RH to 95 %RH

Calibration point %RH	Average of standard reading		Unit under calibration		uncertainty %RH
	Air temperature °C	Calculated humidity %RH	Average reading %RH	Correction value %RH	
45	25.00	45.04	50.2	- 5.16	± 1.3
60	25.00	60.10	65.1	- 5.00	± 1.5
75	25.01	75.06	85.7	- 10.64	± 1.7

Notes

- Calibration results without adjustment.

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2.00$, which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

- End of Report -



ภาคผนวก จ.

สำเนาหนังสืออนุญาตขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
จากกรมโรงงานอุตสาหกรรม และกรมสวัสดิการและคุ้มครองแรงงาน



ที่ อก ๐๓๒๐/๑๑๓๔๒

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๒๗ กรกฎาคม ๒๕๖๖

เรื่อง ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

เรียน กรรมการผู้จัดการ บริษัท อีสเทิร์น ไทย คอนซัลติ้ง ๑๙๙๒ จำกัด

อ้างถึง คำขอต่ออายุของห้องปฏิบัติการวิเคราะห์เอกชน ลงวันที่ ๗ มิถุนายน ๒๕๖๖

สิ่งที่ส่งมาด้วย เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

๑. รายชื่อผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๔๐ ราย
๒. รายชื่อเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๒๕ ราย
๓. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๒๙๒ รายการ
จำนวน ๑๙ แผ่น

ตามหนังสือที่อ้างถึง บริษัท อีสเทิร์น ไทย คอนซัลติ้ง ๑๙๙๒ จำกัด ขอต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๐๐๓ สถานที่ตั้งเลขที่ ๖๘๓ หมู่ที่ ๑๑ ถนนสุขาภิบาล ๘ ตำบลหนองขาม อำเภอศรีราชา จังหวัดชลบุรี ต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้บริษัท อีสเทิร์น ไทย คอนซัลติ้ง ๑๙๙๒ จำกัด ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน โดยมีองค์ประกอบดังนี้

- ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๔๐ ราย ตามสิ่งที่ส่งมาด้วย ๑
- ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๒๕ ราย ตามสิ่งที่ส่งมาด้วย ๒
- ค. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนให้วิเคราะห์ในน้ำเสีย จำนวน ๔๗ รายการ
อากาศเสีย (ปล่องระบาย) จำนวน ๒๑ รายการ น้ำใต้ดิน จำนวน ๑๑ รายการ สิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว
จำนวน ๑๘ รายการ และดิน จำนวน ๙ รายการ รวมทั้งสิ้นจำนวน ๒๙๒ รายการ ตามสิ่งที่ส่งมาด้วย ๓

หนังสือฉบับนี้จะหมดอายุในวันที่ ๕ กรกฎาคม ๒๕๖๙ หากประสงค์จะต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ให้ยื่นคำขอต่ออายุพร้อมเอกสารประกอบคำขอต่อกรมโรงงานอุตสาหกรรม ภายใน ๓๐ วัน ก่อนวันสิ้นอายุของหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ทั้งนี้ สามารถยื่นคำขอผ่านระบบอิเล็กทรอนิกส์ได้ที่หน้าเว็บไซต์กรมโรงงานอุตสาหกรรม

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ


(นายทวี อำพาพันธ์)

ผู้อำนวยการศูนย์วิจัยและเตือนภัยมลพิษโรงงานภาคตะวันออก
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

ศูนย์วิจัยและเตือนภัยมลพิษโรงงานภาคตะวันออก

โทร. ๐ ๓๓๑๓ ๖๐๕๙ ต่อ ๕๐๐๑-๒

ไปรษณีย์อิเล็กทรอนิกส์ eirw@diw.mail.go.th



“อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา อุตสาหกรรมสีเขียว”

~~COPY~~



เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

บริษัท อีสเทิร์น ไทย คอนซัลติ้ง ๑๙๙๒ จำกัด เลขทะเบียน ว-๐๐๓

ที่ อก ๐๓๒๐/๑๑๓๔๒

ลงวันที่ ๒๗ กรกฎาคม ๒๕๖๖

ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๔๐ ราย

๑) นางสาวมาลีเกษ เลขะวัจกุล	ทะเบียนเลขที่	ว-๐๐๓-ค-๐๐๐๑
๒) นายวัฒนา โคตรหล้า	ทะเบียนเลขที่	ว-๐๐๓-ค-๐๐๐๒
๓) นางวรรณเพ็ญ เหลาจินดาว์ฒน์	ทะเบียนเลขที่	ว-๐๐๓-ค-๐๐๐๓
๔) นายกะวีร์ สุธาทรัพย์	ทะเบียนเลขที่	ว-๐๐๓-ค-๐๐๐๔
๕) นางสาวนันท์ณภัส แบนขุนทด	ทะเบียนเลขที่	ว-๐๐๓-ค-๐๐๐๕
๖) นางสาวพรนภา หลงคำหงษ์	ทะเบียนเลขที่	ว-๐๐๓-ค-๐๐๐๖
๗) นางสาวอภิรดี ชื่นอารมย์	ทะเบียนเลขที่	ว-๐๐๓-ค-๐๐๐๗
๘) นางสาวอัจฉรี จิตตะยโสธร	ทะเบียนเลขที่	ว-๐๐๓-ค-๐๐๐๘
๙) นางสาวจิรพร ปานคง	ทะเบียนเลขที่	ว-๐๐๓-ค-๐๐๐๙
๑๐) นายสุทธา สองธนิย์	ทะเบียนเลขที่	ว-๐๐๓-ค-๐๐๑๐
๑๑) นางสาวนันท์ประภา อู๋สูงเนิน	ทะเบียนเลขที่	ว-๐๐๓-ค-๐๐๑๑
๑๒) นายธงไชย บุญศักดิ์	ทะเบียนเลขที่	ว-๐๐๓-ค-๐๐๑๒
๑๓) นางสาวธนาพร กลิ่นโสภณ	ทะเบียนเลขที่	ว-๐๐๓-ค-๐๐๑๓
๑๔) นายธีระพงษ์ นวลอินทร์	ทะเบียนเลขที่	ว-๐๐๓-ค-๐๐๑๔
๑๕) นางสาวแพรว พลเสน	ทะเบียนเลขที่	ว-๐๐๓-ค-๐๐๑๕
๑๖) นายทรงพล ผิวอ้วน	ทะเบียนเลขที่	ว-๐๐๓-ค-๐๐๑๖
๑๗) นายภาคภูมิ บัวสวัสดิ์	ทะเบียนเลขที่	ว-๐๐๓-ค-๐๐๑๗
๑๘) นางสาวจันทน์ สายพันธ์	ทะเบียนเลขที่	ว-๐๐๓-ค-๐๐๑๘
๑๙) นายภาณุพงศ์ บำรุงรส	ทะเบียนเลขที่	ว-๐๐๓-ค-๐๐๑๙
๒๐) นางสาวภาณิน จันดีสอน	ทะเบียนเลขที่	ว-๐๐๓-ค-๐๐๒๐
๒๑) นายวรกร ไวทยะเสวี	ทะเบียนเลขที่	ว-๐๐๓-ค-๐๐๒๑
๒๒) นางสาววรรณภา ไชยศิริ	ทะเบียนเลขที่	ว-๐๐๓-ค-๐๐๒๒
๒๓) นางสาวพรพิมล ภูมิคอนสาร	ทะเบียนเลขที่	ว-๐๐๓-ค-๐๐๒๓
๒๔) นางสาวธมลวรรณ ผลอ้อ	ทะเบียนเลขที่	ว-๐๐๓-ค-๐๐๒๔
๒๕) นางสาวบุญเรือง บุญถม	ทะเบียนเลขที่	ว-๐๐๓-ค-๐๐๒๕
๒๖) นางสาวภัสนันท์ ป้อมน้อย	ทะเบียนเลขที่	ว-๐๐๓-ค-๐๐๒๖
๒๗) นายชานวัฒน์ โชตะวงศ์	ทะเบียนเลขที่	ว-๐๐๓-ค-๐๐๒๗
๒๘) นางสาวพจณีย์ งามวิสัย	ทะเบียนเลขที่	ว-๐๐๓-ค-๐๐๒๘
๒๙) นายวิญญ์วัล สิงห์โต	ทะเบียนเลขที่	ว-๐๐๓-ค-๐๐๒๙
๓๐) นางสาวนุกูล อามรศรี	ทะเบียนเลขที่	ว-๐๐๓-ค-๐๐๓๐
๓๑) นายศุภฤกษ์ พาดกลาง	ทะเบียนเลขที่	ว-๐๐๓-ค-๐๐๓๑
๓๒) นายณิขพล ทองหล่อ	ทะเบียนเลขที่	ว-๐๐๓-ค-๐๐๓๒
๓๓) นายธรรมรัตน์ โพธิ์ตันคำ	ทะเบียนเลขที่	ว-๐๐๓-ค-๐๐๓๓
๓๔) นายโอชา ขวัญศิริมงคล	ทะเบียนเลขที่	ว-๐๐๓-ค-๐๐๓๔
๓๕) นายเมธี สุขประเสริฐ	ทะเบียนเลขที่	ว-๐๐๓-ค-๐๐๓๕

~~COPY~~

๓๖) นางสาวพรพนท...

๓๖) นางสาวพรพินันท์ วิริยกุลกุล	ทะเบียนเลขที่	ว-๐๐๓-ค-๐๐๓๖
๓๗) นางสาวอาภาภรณ์ เสริมสนธิ	ทะเบียนเลขที่	ว-๐๐๓-ค-๐๐๓๗
๓๘) นางสาวนภัทร์ธมณต์ ประดิษฐ์นุช	ทะเบียนเลขที่	ว-๐๐๓-ค-๐๐๓๘
๓๙) นางสาวสุนิษา เอ็งเส้ง	ทะเบียนเลขที่	ว-๐๐๓-ค-๐๐๓๙
๔๐) นางสาวระพีณ อินัน	ทะเบียนเลขที่	ว-๐๐๓-ค-๐๐๔๐

ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๒๕ ราย

๑) นางสาวดวงกมล เนื้อทอง	ทะเบียนเลขที่	ว-๐๐๓-จ-๐๐๐๑
๒) นางสาววัชรภรณ์ อินทสุข	ทะเบียนเลขที่	ว-๐๐๓-จ-๐๐๐๒
๓) นางสาวกัญจน์ธวิกา จันทร์ขอดแก้ว	ทะเบียนเลขที่	ว-๐๐๓-จ-๐๐๐๓
๔) นางสาวฉัตรสุดา มงคลโกชน	ทะเบียนเลขที่	ว-๐๐๓-จ-๐๐๐๔
๕) นางสาวณัฐวดี อำมาตย์ศน์	ทะเบียนเลขที่	ว-๐๐๓-จ-๐๐๐๕
๖) นางสาวนอรอุมา ปาระ	ทะเบียนเลขที่	ว-๐๐๓-จ-๐๐๐๖
๗) นางสาวธัญลักษณ์ ชันโต	ทะเบียนเลขที่	ว-๐๐๓-จ-๐๐๐๗
๘) นางสาวสุทธิดา สร้างแก้ว	ทะเบียนเลขที่	ว-๐๐๓-จ-๐๐๐๘
๙) นายอุดมทรัพย์ เจนจบจริง	ทะเบียนเลขที่	ว-๐๐๓-จ-๐๐๐๙
๑๐) นายนราธิป สงวนศิลป์	ทะเบียนเลขที่	ว-๐๐๓-จ-๐๐๑๐
๑๑) นายวีระชัย พอใจ	ทะเบียนเลขที่	ว-๐๐๓-จ-๐๐๑๑
๑๒) นายอัญชลี ทะพงษ์	ทะเบียนเลขที่	ว-๐๐๓-จ-๐๐๑๒
๑๓) นางสาวสุมลิตรา มีแก่น	ทะเบียนเลขที่	ว-๐๐๓-จ-๐๐๑๓
๑๔) นางสาวสวรรยา เพชรประไพ	ทะเบียนเลขที่	ว-๐๐๓-จ-๐๐๑๔
๑๕) นางสาวจุฑามาศ เจริญพรหม	ทะเบียนเลขที่	ว-๐๐๓-จ-๐๐๑๕
๑๖) นางสาวนิภาพร คำชมภู	ทะเบียนเลขที่	ว-๐๐๓-จ-๐๐๑๖
๑๗) นางสาวอรชา พันธุ์เมือง	ทะเบียนเลขที่	ว-๐๐๓-จ-๐๐๑๗
๑๘) นายกิตติ ไพโรจน์	ทะเบียนเลขที่	ว-๐๐๓-จ-๐๐๑๘
๑๙) นายชาญณรงค์ ตั้งธรรมรักษ์	ทะเบียนเลขที่	ว-๐๐๓-จ-๐๐๑๙
๒๐) นางสาวปวีศา เอสันเทียะ	ทะเบียนเลขที่	ว-๐๐๓-จ-๐๐๒๐
๒๑) นางสาวจุฑาทิพย์ กิจดี	ทะเบียนเลขที่	ว-๐๐๓-จ-๐๐๒๑
๒๒) นางสาวสุภาวดี ศรีละออง	ทะเบียนเลขที่	ว-๐๐๓-จ-๐๐๒๒
๒๓) นางสาวณัฐชยา บรรพบุตร	ทะเบียนเลขที่	ว-๐๐๓-จ-๐๐๒๓
๒๔) นางสาวณัฐนิช นนตานอก	ทะเบียนเลขที่	ว-๐๐๓-จ-๐๐๒๔
๒๕) นางสาวดวงสุดา แสนวันดี	ทะเบียนเลขที่	ว-๐๐๓-จ-๐๐๒๕

~~COPY~~

เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

บริษัท อีสเทิร์น ไทย คอนซัลติ้ง ๑๙๙๒ จำกัด เลขทะเบียน ว-๐๐๓

ที่ อก ๐๓๒๐/๑๑๓๔๒

ลงวันที่ ๒๗ กรกฎาคม ๒๕๖๖

ขอขยายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๒๙๒ รายการ

น้ำเสีย จำนวน 47 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Aldrin	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[4]
2	Arsenic	1) Continuous Hydride Generation/Atomic Absorption Spectrometric Method ^[4] 2) Digestion, Inductively Coupled Plasma Method ^[4]
3	Barium	Digestion, Inductively Coupled Plasma Method ^[4]
4	α -BHC	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[4]
5	β -BHC	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[4]
6	δ -BHC	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[4]
7	γ -BHC	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[4]
8	Biochemical Oxygen Demand	1) 5-Day BOD Test, Membrane Electrode Method ^[4] 2) 5-Day BOD Test, Azide Modification Method ^[4]
9	Cadmium	Digestion, Inductively Coupled Plasma Method ^[4]
10	Chemical Oxygen Demand	Closed Reflux, Titrimetric Method ^[4]
11	cis-Chlordane	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[4]
12	trans-Chlordane	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[4]
13	Chromium	1) Digestion, Direct Air-Acetylene Flame Method ^[4] 2) Digestion, Inductively Coupled Plasma Method ^[4]

~~COPY~~

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
14	Color	ADMI Weighted-Ordinate Spectrophotometric Method ^[4]
15	Copper	1) Digestion, Direct Air-Acetylene Flame Method ^[4] 2) Digestion, Inductively Coupled Plasma Method ^[4]
16	Cyanide	Distillation, Colorimetric Method ^[4]
17	4,4'-DDD	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[4]
18	4,4'-DDE	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[4]
19	DDT	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[4]
20	Dieldrin	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[4]
21	Endosulfan I	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[4]
22	Endosulfan II	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[4]
23	Endosulfan sulfate	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[4]
24	Endrin	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[4]
25	Endrin aldehyde	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[4]
26	Endrin ketone	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[4]
27	Formaldehyde	Distillation, Colorimetric Method ^[3]
28	Free Chlorine	1) Iodometric Method ^[4] 2) Colorimetric Method ^[4]

~~COPY~~

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
29	Heptachlor	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[4]
30	Heptachlor Epoxide	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[4]
31	Hexavalent Chromium	Filtration, Colorimetric Method ^[4]
32	Lead	1) Digestion, Direct Air-Acetylene Flame Method ^[4] 2) Digestion, Inductively Coupled Plasma Method ^[4]
33	Manganese	Digestion, Inductively Coupled Plasma Method ^[4]
34	Mercury	Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^[4]
35	Methoxychlor	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[4]
36	Nickel	1) Digestion, Direct Air-Acetylene Flame Method ^[4] 2) Digestion, Inductively Coupled Plasma Method ^[4]
37	Oil and Grease	Liquid-Liquid, Partition-Gravimetric Method ^[4]
38	pH	Electrometric Method ^[4]
39	Phenols	Distillation, Direct Photometric Method ^[4]
40	Selenium	Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[4]
41	Sulfide	ZnS Precipitation, Iodometric Method ^[4]
42	Temperature	Field Method ^[4]
43	Trivalent Chromium	1) Digestion, Direct Air-Acetylene Flame Method; Filtration, Colorimetric Method; Calculation ^[4] 2) Digestion, Inductively Coupled Plasma Method; Colorimetric Method; Calculation ^[4]
44	Total Dissolved Solids	Dried at 180 °C ^[4]
45	Total Kjeldahl Nitrogen	Macro Kjeldahl Method ^[4]
46	Total Suspended Solids	Dried at 103-105 °C ^[4]
47	Zinc	Digestion, Inductively Coupled Plasma Method ^[4]

~~COPY~~

อากาศเสีย (ปล่อยระบาย) จำนวน 21 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Antimony	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
2	Arsenic	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
3	Cadmium	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
4	Carbon Monoxide	1) Bag, Non-Dispersive Infrared Method ^[5] 2) Instrumental Analyzer Method ^[5]
5	Chromium	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
6	Cobalt	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
7	Copper	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
8	Hydrogen Sulfide	Absorption Sampling, Iodometric Method ^[5]
9	Lead	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
10	Manganese	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
11	Mercury	Isokinetic Sampling, Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^[5]
12	Nickel	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
13	Opacity	Ringelmann's Method ^[1,5]
14	Oxides of Nitrogen	1) Absorption Sampling, Phenoldisulfonic Acid Method ^[8] 2) Instrumental Analyzer Method ^[7]
15	Selenium	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
16	Sulfur Dioxide	1) Absorption Sampling , Barium-Thorin Titrimetric Method ^[5] 2) Instrumental Analyzer Method ^[5]
17	Sulfuric Acid	Isokinetic Sampling, Barium-Thorin Titrimetric Method ^[6]
18	Tin	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]

COPY

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
19	Total Suspended Particulate	Isokinetic Sampling, Gravimetric Method ^[6]
20	Vanadium	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
21	Xylene	Adsorption Sampling, Gas Chromatographic Method ^[6]

น้ำใต้ดิน จำนวน 111 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Acenaphthene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
2	Acetone	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
3	Aldrin	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
4	Anthracene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
5	Antimony	Digestion, Inductively Coupled Plasma Method ^[4]
6	Arsenic	1) Continuous Hydride Generation/Atomic Absorption Spectrometric Method ^[4] 2) Digestion, Inductively Coupled Plasma Method ^[4]
7	Barium	Digestion, Inductively Coupled Plasma Method ^[4]
8	Benz(a)anthracene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
9	Benzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
10	Benzo(b)fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
11	Benzo(k)fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
12	Benzo(a)pyrene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
13	Benzo[g,h,i]perylene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
14	Beryllium	Digestion, Inductively Coupled Plasma Method ^[4]

COPY

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
15	Bis(2-chloroethyl)ether	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
16	Bis(2-ethylhexyl)phthalate	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
17	Bromodichloromethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
18	Bromoform	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
19	Butanol	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
20	Butyl benzyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
21	Cadmium	Digestion, Inductively Coupled Plasma Method ^[4]
22	Carbazole	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
23	Carbon disulfide	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
24	Carbon tetrachloride	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
25	Chlordane	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
26	p-Chloroaniline	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
27	Chlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
28	Chlorodibromomethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
29	Chloroform	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
30	2-Chlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
31	Chromium	1) Digestion, Direct Air-Acetylene Flame Method ^[4] 2) Digestion, Inductively Coupled Plasma Method ^[4]
32	Chromium (III)	1) Digestion, Direct Air-Acetylene Flame Method; Filtration, Colorimetric Method; Calculation ^[4] 2) Digestion, Inductively Coupled Plasma Method; Filtration, Colorimetric Method; Calculation ^[4]

COPY

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
33	Chromium (VI)	Filtration, Colorimetric Method ^[4]
34	Chrysene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
35	Cyanide	Distillation, Colorimetric Method ^[4]
36	DDD	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
37	DDE	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
38	DDT	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
39	Dibenz(a,h)anthracene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
40	Di-n-butyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
41	1,2-Dichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
42	1,3-Dichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
43	1,4-Dichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
44	1,1-Dichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
45	1,2-Dichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
46	1,1-Dichloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
47	cis-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
48	trans-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
49	2,4-Dichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
50	1,2-Dichloropropane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
51	1,3-Dichloropropane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]

COPY

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
52	Dieldrin	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
53	Diethyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
54	2,4-Dimethylphenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
55	2,4-Dinitrotoluene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
56	2,6-Dinitrotoluene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
57	Di-n-octyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
58	Endosulfan	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
59	Endrin	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
60	Ethylbenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
61	Fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
62	Fluorene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
63	Heptachlor	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
64	Heptachlor epoxide	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
65	Hexachlorobenzene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
66	Hexachloro-1,3-butadiene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
67	n-Hexane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
68	α -HCH	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
69	β -HCH	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]

COPY

70 γ -HCH...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
70	γ -HCH	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
71	Hexachlorocyclopentadiene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
72	Hexachloroethane	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
73	Indeno(1,2,3-cd)pyrene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
74	Isophorone	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
75	Lead	1) Digestion, Direct Air-Acetylene Flame Method ^[4] 2) Digestion, Inductively Coupled Plasma Method ^[4]
76	Manganese	Digestion, Inductively Coupled Plasma Method ^[4]
77	Mercury	Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^[4]
78	Methoxychlor	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
79	Methylene chloride	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
80	2-Methylphenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
81	2-Methylnaphthalene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
82	Methyl tert-butyl ether	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
83	Naphthalene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
84	Nickel	Digestion, Inductively Coupled Plasma Method ^[4]
85	Nitrobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
86	N-Nitrosodi-n-propylamine	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
87	pH	Electrometric Method ^[4]
88	Phenanthrene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]

COPY

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
89	Phenol	1) Distillation, Direct Photometric Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
90	Pyrene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
91	Selenium	Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[4]
92	Silver	Digestion, Inductively Coupled Plasma Method ^[4]
93	Styrene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
94	1,1,2,2-Tetrachloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
95	Trichloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
96	1,2,4-Trichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
97	1,1,1-Trichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
98	1,1,2-Trichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
99	Tetrachloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
100	Toluene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
101	2,4,5-Trichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
102	2,4,6-Trichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
103	1,3,5-Trimethylbenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
104	Vanadium	Digestion, Inductively Coupled Plasma Method ^[4]
105	Vinyl acetate	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
106	Vinyl chloride	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]

COPY

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
107	m-Xylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
108	o-Xylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
109	p-Xylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
110	Xylene (Total)	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
111	Zinc	Digestion, Inductively Coupled Plasma Method ^[4]

สิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว จำนวน 18 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Antimony	Digestion, Inductively Coupled Plasma Method ^[9,10]
2	Arsenic	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,9,10] 2) Digestion, Inductively Coupled Plasma Method ^[9,10]
3	Barium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,9,10] 2) Digestion, Inductively Coupled Plasma Method ^[9,10]
4	Beryllium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,9,10] 2) Digestion, Inductively Coupled Plasma Method ^[9,10]
5	Cadmium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,9,10] 2) Digestion, Inductively Coupled Plasma Method ^[9,10]
6	Chromium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,9,10] 2) Digestion, Inductively Coupled Plasma Method ^[9,10]
7	Chromium (VI)	1) Waste Extraction, Digestion, Colorimetric Method ^[2,13] 2) Alkaline Digestion, Colorimetric Method ^[9,13]
8	Cobalt	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,9,10] 2) Digestion, Inductively Coupled Plasma Method ^[9,10]
9	Copper	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,9,10] 2) Digestion, Inductively Coupled Plasma Method ^[9,10]

COPY

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
10	Lead	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,9,10]
11	Mercury	2) Digestion, Inductively Coupled Plasma Method ^[9,10] 1) Waste Extraction, Digestion, Cold Vapor Atomic Absorption Spectrometric Method ^[2,11] 2) Digestion, Cold vapor Atomic Absorption Spectrometric Method ^[9,11]
12	Nickel	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,9,10] 2) Digestion, Inductively Coupled Plasma Method ^[9,10]
13	Molybdenum	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,9,10] 2) Digestion, Inductively Coupled Plasma Method ^[9,10]
14	Selenium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,9,10] 2) Digestion, Inductively Coupled Plasma Method ^[9,10]
15	Silver	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,9,10] 2) Digestion, Inductively Coupled Plasma Method ^[9,10]
16	Thallium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,9,10] 2) Digestion, Inductively Coupled Plasma Method ^[9,10]
17	Vanadium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,9,10] 2) Digestion, Inductively Coupled Plasma Method ^[9,10]
18	Zinc	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[2,9,10] 2) Digestion, Inductively Coupled Plasma Method ^[9,10]

~~COPY~~

ดิน จำนวน 95 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Acenaphthene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[15,17]
2	Acetone	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[14,16]
3	Anthracene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[15,17]
4	Antimony	Digestion, Inductively Coupled Plasma Method ^[9,10]
5	Arsenic	Digestion, Inductively Coupled Plasma Method ^[9,10]
6	Barium	Digestion, Inductively Coupled Plasma Method ^[9,10]
7	Benz(a)anthracene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[15,17]
8	Benzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[14,16]
9	Benzo(b)fluoranthene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[15,17]
10	Benzo(k)fluoranthene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[15,17]
11	Benzo(a)pyrene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[15,17]
12	Benzo[g,h,i]perylene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[15,17]
13	Beryllium	Digestion, Inductively Coupled Plasma Method ^[9,10]
14	Bis(2-chloroethyl)ether	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[15,17]
15	Bis(2-ethylhexyl)phthalate	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[15,17]
16	Bromodichloromethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[14,16]
17	Bromoform	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[14,16]
18	Butanol	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[14,16]

COPY



ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
19	Butyl benzyl phthalate	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[15,17]
20	Cadmium	Digestion, Inductively Coupled Plasma Method ^[9,10]
21	Carbazole	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[15,17]
22	Carbon disulfide	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[14,16]
23	Carbon tetrachloride	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[14,16]
24	p-Chloroaniline	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[15,17]
25	Chlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[14,16]
26	Chlorodibromomethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[14,16]
27	Chloroform	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[14,16]
28	2-Chlorophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[15,17]
29	Chromium	Digestion, Inductively Coupled Plasma Method ^[9,10]
30	Chromium (III)	Digestion, Inductively Coupled Plasma Method; Filtration, Colorimetric Method; Calculation ^[9,10]
31	Chromium (VI)	Alkaline Digestion, Colorimetric Method ^[12,13]
32	Chrysene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[15,17]
33	Dibenz(a,h)anthracene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[15,17]
34	Di-n-butyl phthalate	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[15,17]
35	1,2-Dichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[14,16]
36	1,3-Dichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[14,16]
37	1,4-Dichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[14,16]

COPY

38 1,1-Dichloroethane...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
38	1,1-Dichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[14,16]
39	1,2-Dichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[14,16]
40	1,1-Dichloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[14,16]
41	cis-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[14,16]
42	trans-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[14,16]
43	2,4-Dichlorophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[15,17]
44	1,2-Dichloropropane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[14,16]
45	1,3-Dichloropropane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[14,16]
46	Diethyl phthalate	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[15,17]
47	2,4-Dimethylphenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[15,17]
48	2,4-Dinitrotoluene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[15,17]
49	2,6-Dinitrotoluene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[15,17]
50	Di-n-octyl phthalate	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[15,17]
51	Ethylbenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[14,16]
52	Fluoranthene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[15,17]
53	Fluorene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[15,17]
54	Hexachlorobenzene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[15,17]
55	Hexachloro-1,3-butadiene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[15,17]

COPY

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
56	n-Hexane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[14,16]
57	Hexachlorocyclopentadiene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[15,17]
58	Hexachloroethane	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[15,17]
59	Indeno(1,2,3-cd)pyrene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[15,17]
60	Isophorone	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[15,17]
61	Lead	Digestion, Inductively Coupled Plasma Method ^[9,10]
62	Manganese	Digestion, Inductively Coupled Plasma Method ^[9,10]
63	Mercury	Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^[9,11]
64	Methylene chloride	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[14,16]
65	2-Methylphenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[15,17]
66	2-Methylnaphthalene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[15,17]
67	Methyl tert-butyl ether	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[14,16]
68	Naphthalene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[14,16]
69	Nickel	Digestion, Inductively Coupled Plasma Method ^[9,10]
70	Nitrobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[14,16]
71	N-Nitrosodi-n-propylamine	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[15,17]
72	Phenanthrene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[15,17]
73	Phenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[15,17]
74	Pyrene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[15,17]

COPY

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
75	Selenium	Digestion, Inductively Coupled Plasma Method ^[9,10]
76	Silver	Digestion, Inductively Coupled Plasma Method ^[9,10]
77	Styrene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[14,16]
78	1,1,2,2-Tetrachloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[14,16]
79	Tetrachloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[14,16]
80	Toluene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[14,16]
81	1,2,4-Trichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[14,16]
82	1,1,1-Trichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[14,16]
83	1,1,2-Trichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[14,16]
84	Trichloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[14,16]
85	2,4,5-Trichlorophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[15,17]
86	2,4,6-Trichlorophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[15,17]
87	1,3,5-Trimethylbenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[14,16]
88	Vanadium	Digestion, Inductively Coupled Plasma Method ^[9,10]
89	Vinyl acetate	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[14,16]
90	Vinyl chloride	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[14,16]
91	m-Xylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[14,16]
92	o-Xylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[14,16]
93	p-Xylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[14,16]

~~COPY~~

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
94	Xylene (Total)	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[14,16]
95	Zinc	Digestion, Inductively Coupled Plasma Method ^[9,10]

เอกสารอ้างอิง

1. กระทรวงอุตสาหกรรม. **ประกาศกระทรวงอุตสาหกรรม พ.ศ.2549** เรื่องกำหนดค่าปริมาณเขม่าควันที่เจือปนในอากาศที่ระบายออกจากปล่องของหม้อน้ำโรงสีข้าวที่ใช้กลบเป็นเชื้อเพลิง. ราชกิจจานุเบกษา. 4 ธันวาคม 2549. เล่มที่ 123 ตอนพิเศษ 125 ง.
2. กระทรวงอุตสาหกรรม. **ประกาศกระทรวงอุตสาหกรรม พ.ศ.2548** เรื่อง การกำจัดสิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว. ราชกิจจานุเบกษา. 25 มกราคม 2549. เล่มที่ 123 ตอนพิเศษ 11ง.
3. สมาคมวิศวกรรมสิ่งแวดล้อมแห่งประเทศไทย. คู่มือวิเคราะห์น้ำเสีย. พิมพ์ครั้งที่ 4. กรุงเทพฯ: เรือนแก้วการพิมพ์, 2547.
4. APHA, AWWA, WEF. **Standard Methods for the Examination of Water and Wastewater**. 23rd ed. Washington, DC : APHA, 2017
5. United States Environmental Protection Agency. **Standard of Performance for New Stationary Sources**. 40 CFR Part 60. Appendix A, 2017.
6. United States Environmental Protection Agency. **Standard of Performance for New Stationary Sources**. 40 CFR Part 60. Appendix A, 2019.
7. United States Environmental Protection Agency. **Standard of Performance for New Stationary Sources**. 40 CFR Part 60. Appendix A, 2020.
8. United States Environmental Protection Agency. **Standard of Performance for New Stationary Sources**. 40 CFR Part 60. Appendix A, 2023.
9. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Acid Digestion of Sediments Sludge and Soils. SW-846 Method 3050B**, 1996.
10. United States Environment Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Inductively Coupled Plasma-Atomic Emission spectrometry. SW-846 Method 6010C**, 2007.
11. United States Environment Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Mercury in Solid or Semisolid Waste (Manual Cold-Vapor Technique). SW-846 Method 7471B**, 2007.
12. United States Environment Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Alkaline digestion for Hexavalent Chromium. SW-846 Method 3060A**, 1996.

COPY

13. United States Environment Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Chromium. Hexavalent (Colorimetric). SW-846 Method 7196A**, 1992

14. United States Environment Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Closed-System Purge-and-Trap and Extraction for Volatile Organics in Soil and Waste Samples. SW-846 Method 5035A**, 2002

15. United States Environment Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Ultrasonic Extraction. SW-846 Method 3550C**, 2007

16. United States Environment Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Volatile Organic Compounds by Gas Chromatography/Mass Spectrometry (GC/MS). SW-846 Method 8260D**, 2018

17. United States Environment Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Semivolatile Organic Compounds by Gas Chromatography/Mass Spectrometry. SW-846 Method 8270E**, 2018



~~COPY~~



ที่ อก ๐๓๒๐/ ๔๖๐๔

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๑๔ พฤษภาคม ๒๕๖๗

เรื่อง เปลี่ยนแปลงเอกสารอ้างอิงวิธีวิเคราะห์สารมลพิษ เปลี่ยนแปลงสารมลพิษในดิน และเปลี่ยนแปลงบุคลากร
ของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท อีสเทิร์น ไทย คอนซัลติ้ง ๑๙๙๒ จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๔ มีนาคม ๒๕๖๗

สิ่งที่ส่งมาด้วย เอกสารแนบท้ายหนังสือเปลี่ยนแปลงเอกสารอ้างอิงวิธีวิเคราะห์สารมลพิษ และเปลี่ยนแปลง
สารมลพิษบริษัท อีสเทิร์น ไทย คอนซัลติ้ง ๑๙๙๒ จำกัด จำนวน ๑๒ แผ่น

ตามคำขอฯ ที่อ้างถึง บริษัท อีสเทิร์น ไทย คอนซัลติ้ง ๑๙๙๒ จำกัด ห้องปฏิบัติการวิเคราะห์
เอกชน เลขทะเบียน ว-๐๐๓ สถานที่ตั้งเลขที่ ๖๘๓ หมู่ที่ ๑๑ ถนนสุขาภิบาล ๘ ตำบลหนองขาม
อำเภอศรีราชา จังหวัดชลบุรี แจ้งขอเปลี่ยนแปลงเอกสารอ้างอิงวิธีวิเคราะห์สารมลพิษในน้ำเสีย น้ำใต้ดิน
เปลี่ยนแปลงสารมลพิษในดิน และเปลี่ยนแปลงบุคลากร นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว มีความเห็นดังนี้

๑. ให้ยกเลิกผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๑ ราย

นายวัฒนา โคตรหล้า ทะเบียนเลขที่ ว-๐๐๓-ค-๐๐๐๒

๒. ให้ยกเลิกเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๓ ราย

๑) นางสาวอัญชลี ทะพงษ์ ทะเบียนเลขที่ ว-๐๐๓-จ-๐๐๑๒

๒) นางสาวจุฑามาศ เจริญพรหม ทะเบียนเลขที่ ว-๐๐๓-จ-๐๐๑๕

๓) นางสาวณัฐฐนิช นนตานอก ทะเบียนเลขที่ ว-๐๐๓-จ-๐๐๒๔

๓. ให้ยกเลิกขอบข่ายรายการสารมลพิษในน้ำเสีย และน้ำใต้ดินตามรายการเอกสารแนบท้าย
หนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชนที่ อก ๐๓๒๐/๑๑๓๔๒ ลงวันที่ ๒๗ กรกฎาคม ๒๕๖๖

๔. ให้วิเคราะห์สารมลพิษตามขอบข่ายที่ได้รับขึ้นทะเบียนให้วิเคราะห์ในน้ำเสีย จำนวน ๔๗ รายการ
และน้ำใต้ดิน จำนวน ๑๑๑ รายการ รวมทั้งสิ้นจำนวน ๑๕๘ รายการ ตามเอกสารแนบท้ายหนังสือเปลี่ยนแปลง
เอกสารอ้างอิงวิธีวิเคราะห์สารมลพิษ เปลี่ยนแปลงสารมลพิษในดิน และเปลี่ยนแปลงบุคลากร ดังสิ่งที่ส่งมาด้วย

๕. ให้วิเคราะห์สารมลพิษตามขอบข่ายที่ได้รับขึ้นทะเบียนให้วิเคราะห์เพิ่มเติมในดิน จำนวน
๑๒ รายการ ตามเอกสารแนบท้ายหนังสือเปลี่ยนแปลงเอกสารอ้างอิงวิธีวิเคราะห์สารมลพิษเปลี่ยนแปลงสารมลพิษ
ในดิน และเปลี่ยนแปลงบุคลากร ดังสิ่งที่ส่งมาด้วย

อนึ่ง หนังสือ

~~COPY~~



อนึ่ง หนังสือฉบับนี้จะหมดอายุพร้อมหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์
เอกชนในวันที่ ๕ กรกฎาคม ๒๕๖๙

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ



(นายพรยศ กลั่นกรอง)

รองอธิบดี ปฏิบัติราชการแทน

อธิบดีกรมโรงงานอุตสาหกรรม

ศูนย์วิจัยและเตือนภัยมลพิษโรงงานภาคตะวันออก

โทร. ๐ ๓๓๑๓ ๖๐๕๙ ต่อ ๕๐๐๑-๒

ไปรษณีย์อิเล็กทรอนิกส์ eirw@diw.mail.go.th

~~COPY~~



เอกสารแนบท้ายหนังสือเปลี่ยนแปลงเอกสารอ้างอิงวิธีวิเคราะห์สารมลพิษ

บริษัท อีสเทิร์น ไทย คอนซัลติ้ง ๑๙๙๒ จำกัด

เลขทะเบียน ว-๐๐๓

ที่ อก ๐๓๒๐/

ลงวันที่

ขอขยายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๑๗๐ รายการ
 น้ำเสีย จำนวน 47 รายการ

ลำดับ ที่	สารมลพิษ	วิธีวิเคราะห์
1	Aldrin	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[1] 2) Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[1]
2	Arsenic	1) Continuous Hydride Generation/Atomic Absorption Spectrometric Method ^[1] 2) Digestion, Inductively Coupled Plasma Method ^[1]
3	Barium	Digestion, Inductively Coupled Plasma Method ^[1]
4	α -BHC	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[1] 2) Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[1]
5	β -BHC	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[1] 2) Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[1]
6	δ -BHC	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[1] 2) Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[1]
7	γ -BHC	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[1] 2) Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[1]
8	Biochemical Oxygen Demand	1) 5-Day BOD Test, Membrane Electrode Method ^[1] 2) 5-Day BOD Test, Azide Modification Method ^[1]
9	Cadmium	Digestion, Inductively Coupled Plasma Method ^[1]
10	Chemical Oxygen Demand	Closed Reflux, Titrimetric Method ^[1]
11	cis-Chlordane	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[1] 2) Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[1]

~~COPY~~

12 trans-Chlordane ...

ลำดับ ที่	สารมลพิษ	วิธีวิเคราะห์
12	trans-Chlordane	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[1] 2) Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[1]
13	Chromium	1) Digestion, Direct Air-Acetylene Flame Method ^[1] 2) Digestion, Inductively Coupled Plasma Method ^[1]
14	Color	ADMI Weighted-Ordinate Spectrophotometric Method ^[1]
15	Copper	1) Digestion, Direct Air-Acetylene Flame Method ^[1] 2) Digestion, Inductively Coupled Plasma Method ^[1]
16	Cyanide	Distillation, Colorimetric Method ^[1]
17	4,4'-DDD	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[1] 2) Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[1]
18	4,4'-DDE	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[1] 2) Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[1]
19	DDT	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[1]
20	Dieldrin	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[1] 2) Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[1]
21	Endosulfan I	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[1] 2) Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[1]
22	Endosulfan II	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[1] 2) Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[1]
23	Endosulfan sulfate	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[1] 2) Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[1]
24	Endrin	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[1]

~~COPY~~

ลำดับ ที่	สารมลพิษ	วิธีวิเคราะห์
25	Endrin aldehyde	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[1] 2) Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[1]
26	Endrin ketone	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[1] 2) Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[1]
27	Formaldehyde	Distillation, Colorimetric Method ^[4]
28	Free Chlorine	1) Iodometric Method ^[1] 2) Colorimetric Method ^[1]
29	Heptachlor	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[1] 2) Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[1]
30	Heptachlor Epoxide	1) Liquid-Liquid Extraction, Gas Chromatographic Method ^[1] 2) Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[1]
31	Hexavalent Chromium	Filtration, Colorimetric Method ^[1]
32	Lead	1) Digestion, Direct Air-Acetylene Flame Method ^[1] 2) Digestion, Inductively Coupled Plasma Method ^[1]
33	Manganese	Digestion, Inductively Coupled Plasma Method ^[1]
34	Mercury	Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^[1]
35	Methoxychlor	Liquid-Liquid Extraction, Gas Chromatographic / Mass Spectrometric Method ^[1]
36	Nickel	1) Digestion, Direct Air-Acetylene Flame Method ^[1] 2) Digestion, Inductively Coupled Plasma Method ^[1]
37	Oil and Grease	Liquid-Liquid, Partition-Gravimetric Method ^[1]
38	pH	Electrometric Method ^[1]
39	Phenols	Distillation, Direct Photometric Method ^[1]
40	Selenium	Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[1]

~~COPY~~

ลำดับ ที่	สารมลพิษ	วิธีวิเคราะห์
41	Sulfide	ZnS Precipitation, Iodometric Method ^[1]
42	Temperature	Field Method ^[1]
43	Trivalent Chromium	1) Digestion, Direct Air-Acetylene Flame Method; Filtration, Colorimetric Method; Calculation ^[1] 2) Digestion, Inductively Coupled Plasma Method; Colorimetric Method; Calculation ^[1]
44	Total Dissolved Solids	Dried at 180 °C ^[1]
45	Total Kjeldahl Nitrogen	Macro Kjeldahl Method ^[1]
46	Total Suspended Solids	Dried at 103-105 °C ^[1]
47	Zinc	Digestion, Inductively Coupled Plasma Method ^[1]

น้ำใต้ดิน จำนวน 111 รายการ

ลำดับ ที่	สารมลพิษ	วิธีวิเคราะห์
1	Acenaphthene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1]
2	Acetone	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[1]
3	Aldrin	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1]
4	Anthracene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1]
5	Antimony	Digestion, Inductively Coupled Plasma Method ^[1]
6	Arsenic	1) Continuous Hydride Generation/Atomic Absorption Spectrometric Method ^[1] 2) Digestion, Inductively Coupled Plasma Method ^[1]
7	Barium	Digestion, Inductively Coupled Plasma Method ^[1]
8	Benz(a)anthracene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1]

COPY

ลำดับ ที่	สารมลพิษ	วิธีวิเคราะห์
9	Benzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[1]
10	Benzo(b)fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1]
11	Benzo(k)fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1]
12	Benzo(a)pyrene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1]
13	Benzo[g,h,i]perylene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1]
14	Beryllium	Digestion, Inductively Coupled Plasma Method ^[1]
15	Bis(2-chloroethyl)ether	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1]
16	Bis(2-ethylhexyl)phthalate	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1]
17	Bromodichloromethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[1]
18	Bromoform	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[1]
19	Butanol	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[1]
20	Butyl benzyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1]
21	Cadmium	Digestion, Inductively Coupled Plasma Method ^[1]
22	Carbazole	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1]
23	Carbon disulfide	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[1]
24	Carbon tetrachloride	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[1]

ลำดับ ที่	สารมลพิษ	วิธีวิเคราะห์
25	Chlordane	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1]
26	p-Chloroaniline	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1]
27	Chlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[1]
28	Chlorodibromomethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[1]
29	Chloroform	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[1]
30	2-Chlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1]
31	Chromium	1) Digestion, Direct Air-Acetylene Flame Method ^[1] 2) Digestion, Inductively Coupled Plasma Method ^[1]
32	Chromium (III)	1) Digestion, Direct Air-Acetylene Flame Method; Filtration, Colorimetric Method; Calculation ^[1] 2) Digestion, Inductively Coupled Plasma Method; Filtration, Colorimetric Method; Calculation ^[1]
33	Chromium (VI)	Filtration, Colorimetric Method ^[1]
34	Chrysene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1]
35	Cyanide	Distillation, Colorimetric Method ^[1]
36	DDD	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1]
37	DDE	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1]
38	DDT	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1]
39	Dibenz(a,h)anthracene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1]

ลำดับ ที่	สารมลพิษ	วิธีวิเคราะห์
40	Di-n-butyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1]
41	1,2-Dichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[1]
42	1,3-Dichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[1]
43	1,4-Dichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[1]
44	1,1-Dichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[1]
45	1,2-Dichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[1]
46	1,1-Dichloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[1]
47	cis-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[1]
48	trans-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[1]
49	2,4-Dichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1]
50	1,2-Dichloropropane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[1]
51	1,3-Dichloropropane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[1]
52	Dieldrin	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1]
53	Diethyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1]
54	2,4-Dimethylphenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1]

ลำดับ ที่	สารมลพิษ	วิธีวิเคราะห์
55	2,4-Dinitrotoluene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1]
56	2,6-Dinitrotoluene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1]
57	Di-n-octyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1]
58	Endosulfan	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1]
59	Endrin	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1]
60	Ethylbenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[1]
61	Fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1]
62	Fluorene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1]
63	Heptachlor	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1]
64	Heptachlor epoxide	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1]
65	Hexachlorobenzene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1]
66	Hexachloro-1,3-butadiene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1]
67	n-Hexane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[1]
68	α -HCH	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1]
69	β -HCH	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1]

COPY

ลำดับ ที่	สารมลพิษ	วิธีวิเคราะห์
70	γ -HCH	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1]
71	Hexachlorocyclopentadiene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1]
72	Hexachloroethane	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1]
73	Indeno(1,2,3-cd)pyrene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1]
74	Isophorone	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1]
75	Lead	1) Digestion, Direct Air-Acetylene Flame Method ^[1] 2) Digestion, Inductively Coupled Plasma Method ^[1]
76	Manganese	Digestion, Inductively Coupled Plasma Method ^[1]
77	Mercury	Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^[1]
78	Methoxychlor	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1]
79	Methylene chloride	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[1]
80	2-Methylphenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1]
81	2-Methylnaphthalene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1]
82	Methyl tert-butyl ether	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[1]
83	Naphthalene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[1]
84	Nickel	Digestion, Inductively Coupled Plasma Method ^[1]
85	Nitrobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[1]

ลำดับ ที่	สารมลพิษ	วิธีวิเคราะห์
86	N-Nitrosodi-n-propylamine	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1]
87	pH	Electrometric Method ^[4]
88	Phenanthrene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
89	Phenol	1) Distillation, Direct Photometric Method ^[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
90	Pyrene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
91	Selenium	Digestion, Hydride Generation/Atomic Absorption Spectrometric Method ^[4]
92	Silver	Digestion, Inductively Coupled Plasma Method ^[4]
93	Styrene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
94	1,1,2,2-Tetrachloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
95	Trichloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
96	1,2,4-Trichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
97	1,1,1-Trichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
98	1,1,2-Trichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
99	Tetrachloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
100	Toluene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
101	2,4,5-Trichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]

COPY

2,2,4,6-Trichlorophenol ...

ลำดับ ที่	สารมลพิษ	วิธีวิเคราะห์
102	2,4,6-Trichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
103	1,3,5-Trimethylbenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
104	Vanadium	Digestion, Inductively Coupled Plasma Method ^[4]
105	Vinyl acetate	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
106	Vinyl chloride	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
107	m-Xylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
108	o-Xylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
109	p-Xylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
110	Xylene (Total)	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
111	Zinc	Digestion, Inductively Coupled Plasma Method ^[4]

ดิน จำนวน 12 รายการ

ลำดับ ที่	สารมลพิษ	วิธีวิเคราะห์
1	α -HCH	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
2	β -HCH	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
3	γ -HCH	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
4	Heptachlor	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]

COPY

ลำดับ ที่	สารมลพิษ	วิธีวิเคราะห์
5	Aldrin	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
6	Heptachlor epoxide	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
7	Chlordane	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
8	Dieldrin	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
9	Endrin	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
10	DDD	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
11	DDT	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]
12	Methoxychlor	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method ^[2,3]

เอกสารอ้างอิง

1. APHA, AWWA, WEF. **Standard Methods for the Examination of Water and Wastewater**. 24th ed. Washington, DC: APHA, 2023.
2. United States Environment Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Ultrasonic Extraction**. SW-846 Method 3550C, 2007
3. United States Environment Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Semivolatile Organic Compounds by Gas Chromatography/Mass Spectrometry**. SW-846 Method 8270E, 2018
4. สมาคมวิศวกรรมสิ่งแวดล้อมแห่งประเทศไทย. คู่มือวิเคราะห์น้ำเสีย. พิมพ์ครั้งที่ 4. กรุงเทพฯ: เรือนแก้วการพิมพ์, 2547.

COPY

ที่ อก ๐๓๑๐(๓)/ ๘๓ ๕ ๕



กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๐๙ ตุลาคม ๒๕๖๘

เรื่อง เปลี่ยนแปลงบุคลากรและสารมลพิษที่วิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท อีสเทิร์น ไทย คอนซัลติ้ง ๑๙๙๒ จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๒๙ สิงหาคม ๒๕๖๘

สิ่งที่ส่งมาด้วย เอกสารแนบท้ายหนังสือเปลี่ยนแปลงบุคลากรและสารมลพิษที่วิเคราะห์
บริษัท อีสเทิร์น ไทย คอนซัลติ้ง ๑๙๙๒ จำกัด จำนวน ๑ แผ่น

ตามคำขอที่อ้างถึง บริษัท อีสเทิร์น ไทย คอนซัลติ้ง ๑๙๙๒ จำกัด ห้องปฏิบัติการวิเคราะห์
เอกชน เลขทะเบียน ว-๐๐๓ สถานที่ตั้งเลขที่ ๖๘๓ หมู่ที่ ๑๑ ถนนสุขาภิบาล ๘ ตำบลหนองขาม อำเภอสรีราชา
จังหวัดชลบุรี ขอเปลี่ยนแปลงบุคลากรและสารมลพิษที่วิเคราะห์ ต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว มีความเห็นดังนี้

๑. ให้ยกเลิกผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๑ ราย

นายภาคภูมิ บัวสวัสดิ์

ทะเบียนเลขที่ ว-๐๐๓-ค-๐๐๑๓๗

๒. ให้ยกเลิกเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๓ ราย

๑) นางสาวนิอรอุมา ปาระ

ทะเบียนเลขที่ ว-๐๐๓-จ-๐๐๐๖

๒) นางสาวสุทธิดา สร้างแก้ว

ทะเบียนเลขที่ ว-๐๐๓-จ-๐๐๐๘

๓) นางสาวดวงสุดา แสนวันดี

ทะเบียนเลขที่ ว-๐๐๓-จ-๐๐๒๕

๓. ให้เพิ่มเจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน จำนวน ๑ ราย

นายวรารุธ อารีเอื้อ

ทะเบียนเลขที่ ว-๐๐๓-จ-๐๐๒๖

๔. ให้เพิ่มขอบข่ายชนิดสารมลพิษที่วิเคราะห์ในน้ำใต้ดิน และดิน ตามสิ่งที่ส่งมาด้วย

อนึ่ง หนังสือฉบับนี้จะสิ้นสุดอายุพร้อมหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
ในวันที่ ๕ กรกฎาคม ๒๕๖๙

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นางสาวปัทมวรรณ คุณประเสริฐ)

ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน

ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

ศูนย์วิจัยและเตือนภัยมลพิษโรงงานภาคตะวันออก

โทร. ๐ ๓๓๑๓ ๖๐๕๕ ต่อ ๕๐๐๑-๒

ไปรษณีย์อิเล็กทรอนิกส์ eirw@diw.mail.go.th

~~COPY~~



เอกสารแนบท้ายหนังสือเปลี่ยนแปลงบุคลากรและสารมลพิษที่วิเคราะห์

บริษัท อีสเทิร์น ไทย คอนซัลติ้ง ๑๙๙๒ จำกัด
ที่ อก ๐๓๑๐(๓)/ ๘๓ ๔ ๕

เลขทะเบียน ว-๐๐๓
ลงวันที่ ๐๙ ตุลาคม ๒๕๖๔

ขอขยายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๙ รายการ
น้ำใต้ดิน จำนวน 4 รายการ

ลำดับที่	ชนิดสารมลพิษ	วิธีวิเคราะห์
1	Aluminum	Digestion, Inductively Coupled Plasma Method ^[1]
2	Copper	Digestion, Inductively Coupled Plasma Method ^[1]
3	Iron	Digestion, Inductively Coupled Plasma Method ^[1]
4	Molybdenum	Digestion, Inductively Coupled Plasma Method ^[1]

ดิน จำนวน 5 รายการ

ลำดับที่	ชนิดสารมลพิษ	วิธีวิเคราะห์
1	Aluminum	Digestion, Inductively Coupled Plasma Method ^[2,3]
2	Copper	Digestion, Inductively Coupled Plasma Method ^[2,3]
3	Iron	Digestion, Inductively Coupled Plasma Method ^[2,3]
4	Molybdenum	Digestion, Inductively Coupled Plasma Method ^[2,3]
5	pH	Electrometric Method ^[4]

เอกสารอ้างอิง

1. APHA, AWWA, WEF. **Standard Methods for the Examination of Water and Wastewater**. 24th ed. Washington, DC : APHA, 2023
2. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Acid Digestion of Sediments, Sludges, and Soils. **SW-846 Method 3050B**, 1996.
3. United States Environmental Protection Agency. Inductively Coupled Plasma - Atomic Emission Spectrometry. **SW-846 Method 6010C**, 2007
4. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Soil and Waste pH. **SW-846 Method 9045D**, 2004.



~~COPY~~