

ภาคผนวก ค

ใบรับรองผลการวิเคราะห์

คุณภาพอากาศในบรรยากาศ



Analysis / Test Report

TESTING
No.0042

Client : THAI MMA Co., Ltd.
88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150

P/O : PMM-2025-336

Project Name : Environmental Monitoring

Project Location : CCS Site 7

Lot ID: 2610896

Date Received : Mar 10, 2026

Date Reported : Mar 14, 2026

Report Number: 3500989-1

Page 1 of 1

Sample Description	Air Quality
Location	ม.บ้านนา (GPS 47P 0735660, 1409166)
Date Analysis Commenced	Mar 10, 2026
Condition of Sample	Drawn into one glass filter paper (8x10 inch) placed in plastic bag and one quartz filter paper (8x10 inch) placed in plastic bag

Sample Number	Sampled Date	Sampling Condition		Total Suspended Particulate (ug/m3)	Particulate Matter (PM-10) (ug/m3)
		Pressure (mm Hg)	Temperature (°C)		
2610896-1	Mar 02 - Mar 03, 2026	755	32.1	56.6	29.2
2610896-2	Mar 03 - Mar 04, 2026	755	31.2	58.8	28.8
2610896-3	Mar 04 - Mar 05, 2026	755	32.2	61.6	30.6
2610896-4	Mar 05 - Mar 06, 2026	755	32.2	75.6	52.0
2610896-5	Mar 06 - Mar 07, 2026	755	31.1	51.4	23.2
2610896-6	Mar 07 - Mar 08, 2026	755	31.8	46.6	21.0
2610896-7	Mar 08 - Mar 09, 2026	755	31.6	39.9	20.9
Guideline	-	-	-	200	100

Reference Method

Total Suspended Particulate : United States Environmental Protection Agency 40 CFR, method 50, Appendix B, revised as of July 1, 2008

Particulate Matter (PM-10) : United States Environmental Protection Agency 40 CFR, method 50, Appendix J, revised as of July 1, 2008

Guideline : Notification of the National Environmental Board., 2026 (B.E.2569) dated January 21, 2026.

Sampled By : Santi Chaichana

Approved by

Thanita K.

Thanita Kulsuriwong
Scientist (4)

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

Client : THAI MMA Co., Ltd.
88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150
P/O : PMM-2025-336
Project Name : Environmental Monitoring
Project Location : CCS Site 7

TESTING
No.0042
Lot ID: 2610896
Date Received : Mar 10, 2026
Date Reported : Mar 14, 2026
Report Number: 3500989-2

Page 1 of 1

Sample Description	Air Quality				
Location	รณรงค (GPS 47P 0734594, 1408565)				
Date Analysis Commenced	Mar 10, 2026				
Condition of Sample	Drawn into one glass filter paper (8x10 inch) placed in plastic bag and one quartz filter paper (8x10 inch) placed in plastic bag				
Sample Number	Sampled Date	Sampling Condition		Total Suspended Particulate (ug/m3)	Particulate Matter (PM-10) (ug/m3)
		Pressure (mm Hg)	Temperature (°C)		
2610896-8	Mar 02 - Mar 03, 2026	755	32.1	61.0	35.1
2610896-9	Mar 03 - Mar 04, 2026	755	31.2	64.9	46.8
2610896-10	Mar 04 - Mar 05, 2026	755	32.2	69.2	30.6
2610896-11	Mar 05 - Mar 06, 2026	755	32.2	70.7	36.3
2610896-12	Mar 06 - Mar 07, 2026	755	31.1	47.1	23.5
2610896-13	Mar 07 - Mar 08, 2026	755	31.8	49.7	20.3
2610896-14	Mar 08 - Mar 09, 2026	755	31.6	47.0	36.3
Guideline	-	-	-	200	100

Reference Method

Total Suspended Particulate : United States Environmental Protection Agency 40 CFR, method 50, Appendix B, revised as of July 1, 2008
Particulate Matter (PM-10) : United States Environmental Protection Agency 40 CFR, method 50, Appendix J, revised as of July 1, 2008

Guideline : Notification of the National Environmental Board., 2026 (B.E.2569) dated January 21, 2026.

Sampled By : Santi Chaichana

Approved by

Thanita K.

Thanita Kulsuriwong
Scientist (4)

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.



Analysis / Test Report

TESTING
No.0042

Client : THAI MMA Co., Ltd.
88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150

P/O : PMM-2025-336

Project Name : Environmental Monitoring

Project Location : CCS Site 7

Lot ID: 2610896

Date Received : Mar 10, 2026

Date Reported : Mar 14, 2026

Report Number: 3500989-3

Page 1 of 1

Sample Description	Air Quality
Location	บ้านเนินพยอม (GPS 47P 0736415, 1410971)
Date Analysis Commenced	Mar 10, 2026
Condition of Sample	Drawn into one glass filter paper (8x10 inch) placed in plastic bag and one quartz filter paper (8x10 inch) placed in plastic bag

Sample Number	Sampled Date	Sampling Condition		Total Suspended Particulate (ug/m3)	Particulate Matter (PM-10) (ug/m3)
		Pressure (mm Hg)	Temperature (°C)		
2610896-15	Mar 02 - Mar 03, 2026	755	32.1	55.8	19.2
2610896-16	Mar 03 - Mar 04, 2026	755	31.2	80.8	31.8
2610896-17	Mar 04 - Mar 05, 2026	755	32.2	94.4	34.0
2610896-18	Mar 05 - Mar 06, 2026	755	32.2	95.2	38.4
2610896-19	Mar 06 - Mar 07, 2026	755	31.1	74.8	32.6
2610896-20	Mar 07 - Mar 08, 2026	755	31.8	68.6	24.2
2610896-21	Mar 08 - Mar 09, 2026	755	31.6	55.5	22.9
Guideline	-	-	-	200	100

Reference Method

Total Suspended Particulate : United States Environmental Protection Agency 40 CFR, method 50, Appendix B, revised as of July 1, 2008

Particulate Matter (PM-10) : United States Environmental Protection Agency 40 CFR, method 50, Appendix J, revised as of July 1, 2008

Guideline : Notification of the National Environmental Board., 2026 (B.E.2569) dated January 21, 2026.

Sampled By : Santi Chaichana

Approved by

Thanita K.

Thanita Kulsuriwong
Scientist (4)

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.



Analysis / Test Report

Client : THAI MMA Co., Ltd.

88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150

P/O : PMM-2025-336

Project Name : Environmental Monitoring

Project Location : CCS Site 7

Lot ID: 2610898

Date Received : Mar 10, 2026

Date Reported : Mar 16, 2026

Report Number : 3500987-1

Page 1 of 2

Sample Number : 2610898-1 to 7
Parameter : Wind Speed / Wind Direction
Location : มังกรวน (GPS 47P 0735660, 1409166)
Sampling Date : Mar 02 - Mar 09, 2026
Sampling by : Santi Chaichana

Time	Mar 02 - Mar 03, 2026			Mar 03 - Mar 04, 2026			Mar 04 - Mar 05, 2026			Mar 05 - Mar 06, 2026			Mar 06 - Mar 07, 2026			Mar 07 - Mar 08, 2026			Mar 08 - Mar 09, 2026		
	WS (m/s)	WD (deg)		WS (m/s)	WD (deg)		WS (m/s)	WD (deg)		WS (m/s)	WD (deg)		WS (m/s)	WD (deg)		WS (m/s)	WD (deg)		WS (m/s)	WD (deg)	
12:00 PM - 01:00 PM	3.2	95.0	E	1.4	203.0	SSW	2.4	193.0	SSW	2.8	112.0	ESE	4.9	145.0	SE	2.6	108.0	ESE	4.3	117.0	ESE
01:00 PM - 02:00 PM	3.4	166.0	SSE	3.6	142.0	SE	3.6	167.0	SSE	1.9	185.0	S	3.1	103.0	ESE	4.8	162.0	SSE	3.4	99.0	E
02:00 PM - 03:00 PM	2.8	181.0	S	2.6	119.0	ESE	2.5	203.0	SSW	1.9	95.0	E	4.5	128.0	SE	6.3	157.0	SSE	7.6	76.0	ENE
03:00 PM - 04:00 PM	2.1	174.0	S	1.6	140.0	SE	1.8	189.0	S	3.4	184.0	S	5.4	125.0	SE	5.1	117.0	ESE	3.8	126.0	SE
04:00 PM - 05:00 PM	2.6	167.0	SSE	1.6	128.0	SE	1.8	118.0	ESE	2.8	181.0	S	6.4	129.0	SE	4.4	98.0	E	5.4	76.0	ENE
05:00 PM - 06:00 PM	1.9	165.0	SSE	0.4	136.0	SE	2.4	169.0	S	0.7	150.0	SSE	4.2	164.0	SSE	3.8	103.0	ESE	2.3	71.0	ENE
06:00 PM - 07:00 PM	2.0	125.0	SE	0.9	104.0	ESE	1.3	113.0	ESE	1.4	114.0	ESE	4.2	183.0	S	5.1	88.0	E	1.1	100.0	E
07:00 PM - 08:00 PM	0.4	155.0	SSE	0.4	97.0	E	0.3	180.0	S	0.2	-	-	4.5	68.0	ENE	2.9	77.0	ENE	0.5	72.0	ENE
08:00 PM - 09:00 PM	1.0	140.0	SE	0.0	-	-	0.6	170.0	S	0.0	-	-	0.4	203.0	SSW	0.8	314.0	NW	0.6	55.0	NE
09:00 PM - 10:00 PM	0.6	168.0	SSE	1.5	140.0	SE	0.4	189.0	S	0.1	-	-	4.6	53.0	NE	1.8	308.0	NW	0.5	68.0	ENE
10:00 PM - 11:00 PM	1.2	118.0	ESE	0.6	159.0	SSE	0.0	-	-	0.2	-	-	1.3	207.0	SSW	1.4	109.0	ESE	0.4	74.0	ENE
11:00 PM - 12:00 AM	0.0	-	-	0.0	-	-	1.1	154.0	SSE	0.1	-	-	2.2	3.0	N	3.7	169.0	S	0.0	-	-
12:00 AM - 01:00 AM	1.4	212.0	SSW	0.4	133.0	SE	0.4	186.0	S	0.6	41.0	NE	0.9	321.0	NW	0.2	-	-	1.1	205.0	SSW
01:00 AM - 02:00 AM	2.1	164.0	SSE	0.6	191.0	S	0.3	177.0	S	0.2	-	-	0.0	-	-	0.0	-	-	0.3	21.0	NNE
02:00 AM - 03:00 AM	0.6	262.0	W	1.9	181.0	S	0.0	-	-	0.3	100.0	E	0.6	301.0	WNW	2.0	327.0	NNW	0.0	-	-
03:00 AM - 04:00 AM	0.0	-	-	0.8	233.0	SW	0.3	114.0	ESE	0.5	41.0	NE	1.8	289.0	WNW	0.7	304.0	NW	1.3	46.0	NE
04:00 AM - 05:00 AM	0.3	5.0	N	0.0	-	-	1.0	214.0	SW	0.2	-	-	1.4	338.0	NNW	0.0	-	-	3.8	16.0	NNE
05:00 AM - 06:00 AM	0.2	-	-	0.2	-	-	0.5	248.0	WSW	0.0	-	-	1.0	0.0	N	1.6	22.0	NNE	1.2	3.0	N
06:00 AM - 07:00 AM	0.9	358.0	N	0.0	-	-	0.9	263.0	W	1.6	5.0	N	1.0	332.0	NNW	1.9	348.0	NNW	0.8	341.0	NNW
07:00 AM - 08:00 AM	0.5	0.0	N	0.2	-	-	0.7	310.0	NW	0.9	28.0	NNE	3.9	300.0	WNW	3.0	325.0	NW	2.0	52.0	NE
08:00 AM - 09:00 AM	1.4	279.0	W	0.5	175.0	S	1.0	345.0	NNW	0.6	92.0	E	3.9	200.0	SSW	3.3	334.0	NNW	1.8	355.0	N
09:00 AM - 10:00 AM	1.2	97.0	E	1.2	223.0	SW	2.3	184.0	S	0.5	2.0	N	0.5	221.0	SW	3.7	209.0	SSW	2.0	346.0	NNW
10:00 AM - 11:00 AM	1.7	108.0	ESE	1.3	213.0	SSW	2.9	143.0	SE	2.1	107.0	ESE	2.7	225.0	SW	5.6	3.0	N	1.0	46.0	NE
11:00 AM - 12:00 PM	1.8	188.0	S	2.1	163.0	SSE	1.4	138.0	SE	7.4	139.0	SE	5.5	165.0	SSE	1.6	359.0	N	0.8	58.0	ENE

Reference Method : Cup Anemometer & Anodized Aluminium Vane Method

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any form without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

Approved by

Sarayuth Jittranont
Assistant General Manager



Analysis / Test Report

Client : THAI MMA Co., Ltd.

88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150

P/O : PMM-2025-336

Project Name : Environmental Monitoring

Project Location : CCS Site 7

Lot ID: 2610898


Date Received : Mar 10, 2026

Date Reported : Mar 16, 2026


Report Number : 3500987-1

Page 2 of 2


Wind Rose




Date : Mar 02-03, 2026




Date : Mar 03-04, 2026




Date : Mar 04-05, 2026




Date : Mar 05-06, 2026




Date : Mar 06-07, 2026



Date : Mar 07-08, 2026



Date : Mar 08-09, 2026



Date : Mar 02-09, 2026

WS (m/s)	%
≥ 10.0	0.00
8.0-10.0	0.00
5.5-8.0	3.57
3.3-5.5	15.48
1.7-3.3	22.62
0.3-1.7	43.45
Calms	14.88

Location : บ้านนา (GPS 47P 0735660, 1409166)

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any form without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

Approved by

Sarayuth Jitranont
Assistant General Manager



Analysis / Test Report

Client : THAI MMA Co., Ltd.

88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150

P/O : PMM-2025-336

Project Name : Environmental Monitoring

Project Location : CCS Site 7

Lot ID: 2610898

Date Received :Mar 10, 2026

Date Reported :Mar 16, 2026

Report Number :3500987-1

Page 1 of 2

Sample Number 2610898-8 to 14
Parameter Wind Speed / Wind Direction
Location บ้านนาทราย (GPS 47P 0734594, 1408565)
Sampling Date Mar 02 - Mar 09, 2026
Sampling by Santi Chaichana

Time	Mar 02 - Mar 03, 2026			Mar 03 - Mar 04, 2026			Mar 04 - Mar 05, 2026			Mar 05 - Mar 06, 2026			Mar 06 - Mar 07, 2026			Mar 07 - Mar 08, 2026			Mar 08 - Mar 09, 2026		
	WS (m/s)	WD (deg)		WS (m/s)	WD (deg)		WS (m/s)	WD (deg)		WS (m/s)	WD (deg)		WS (m/s)	WD (deg)		WS (m/s)	WD (deg)		WS (m/s)	WD (deg)	
01:00 PM - 02:00 PM	2.7	238.0	WSW	2.0	218.0	SW	2.2	143.0	SE	2.0	188.0	S	1.6	180.0	S	1.9	210.0	SSW	0.6	228.0	SW
02:00 PM - 03:00 PM	1.6	156.0	SSE	2.6	163.0	SSE	4.0	195.0	SSW	1.9	142.0	SE	2.2	253.0	WSW	1.8	235.0	SW	1.5	246.0	WSW
03:00 PM - 04:00 PM	2.6	200.0	SSW	1.4	179.0	S	1.7	193.0	SSW	3.5	186.0	S	1.7	270.0	W	2.9	285.0	WNW	0.2	-	-
04:00 PM - 05:00 PM	0.7	149.0	SSE	0.3	177.0	S	1.4	145.0	SE	1.7	178.0	S	3.0	196.0	SSW	0.6	296.0	WNW	2.3	332.0	NNW
05:00 PM - 06:00 PM	1.6	122.0	ESE	1.6	187.0	S	0.6	124.0	SE	1.0	166.0	SSE	1.7	178.0	S	0.5	278.0	W	0.9	298.0	WNW
06:00 PM - 07:00 PM	1.0	159.0	SSE	0.8	123.0	ESE	0.4	161.0	SSE	0.4	136.0	SE	1.2	328.0	NNW	0.5	261.0	W	0.1	-	-
07:00 PM - 08:00 PM	0.1	-	-	0.3	141.0	SE	0.3	153.0	SSE	0.6	137.0	SE	1.7	87.0	E	0.5	322.0	NW	0.2	-	-
08:00 PM - 09:00 PM	0.9	171.0	S	1.2	180.0	S	0.0	-	-	0.9	87.0	E	0.8	351.0	N	0.4	83.0	E	0.6	11.0	N
09:00 PM - 10:00 PM	0.3	180.0	S	0.6	190.0	S	0.0	-	-	0.2	-	-	1.6	92.0	E	0.0	-	-	0.4	40.0	NE
10:00 PM - 11:00 PM	0.7	180.0	S	0.0	-	-	0.0	-	-	0.3	38.0	NE	0.0	-	-	0.5	192.0	SSW	0.2	-	-
11:00 PM - 12:00 AM	0.0	-	-	0.8	179.0	S	0.3	139.0	SE	0.5	40.0	NE	0.4	332.0	NNW	0.6	199.0	SSW	0.3	80.0	E
12:00 AM - 01:00 AM	0.0	-	-	0.8	198.0	SSW	0.5	193.0	SSW	0.4	81.0	E	0.5	81.0	E	0.1	-	-	0.0	-	-
01:00 AM - 02:00 AM	0.0	-	-	0.2	-	-	0.2	-	-	0.2	-	-	0.0	-	-	0.3	198.0	SSW	0.2	-	-
02:00 AM - 03:00 AM	0.3	359.0	N	0.0	-	-	0.4	210.0	SSW	0.7	44.0	NE	0.2	-	-	0.2	-	-	0.1	-	-
03:00 AM - 04:00 AM	0.0	-	-	0.2	-	-	0.3	193.0	SSW	0.1	-	-	0.4	48.0	NE	0.6	73.0	ENE	0.3	26.0	NNE
04:00 AM - 05:00 AM	0.8	65.0	ENE	0.3	52.0	NE	0.2	-	-	0.7	130.0	SE	0.6	309.0	NW	0.0	-	-	1.0	21.0	NNE
05:00 AM - 06:00 AM	0.0	-	-	0.0	-	-	0.8	225.0	SW	0.8	359.0	N	0.4	17.0	NNE	0.4	43.0	NE	1.2	80.0	E
06:00 AM - 07:00 AM	0.2	-	-	0.6	86.0	E	0.6	316.0	NW	0.7	347.0	NNW	0.5	340.0	NNW	0.3	95.0	E	0.5	85.0	E
07:00 AM - 08:00 AM	0.0	-	-	1.0	212.0	SSW	1.2	292.0	WNW	1.0	99.0	E	0.4	76.0	ENE	2.3	325.0	NW	1.5	89.0	E
08:00 AM - 09:00 AM	0.9	156.0	SSE	0.6	161.0	SSE	1.2	124.0	SE	0.4	158.0	SSE	1.3	103.0	ESE	0.6	145.0	SE	2.0	85.0	E
09:00 AM - 10:00 AM	1.4	167.0	SSE	0.5	208.0	SSW	1.2	116.0	ESE	2.5	127.0	SE	1.0	98.0	E	0.7	17.0	NNE	1.0	344.0	NNW
10:00 AM - 11:00 AM	0.8	209.0	SSW	2.3	107.0	ESE	1.0	165.0	SSE	1.9	158.0	SSE	1.5	95.0	E	4.2	152.0	SSE	1.2	54.0	NE
11:00 AM - 12:00 PM	1.4	201.0	SSW	1.8	216.0	SW	1.3	183.0	S	1.0	182.0	S	1.8	197.0	SSW	1.2	300.0	WNW	1.0	84.0	E
12:00 PM - 01:00 PM	2.6	180.0	S	1.8	88.0	E	1.5	83.0	E	2.5	178.0	S	3.7	228.0	SW	2.8	268.0	W	2.0	100.0	E

Reference Method : Cup Anemometer & Anodized Aluminium Vane Method

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any form without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

Approved by

Sarayuth Jittrantont
Assistant General Manager



Analysis / Test Report

Client : THAI MMA Co., Ltd.

88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150

P/O : PMM-2025-336

Project Name : Environmental Monitoring

Project Location : CCS Site 7

Lot ID: 2610898


Date Received : Mar 10, 2026

Date Reported : Mar 16, 2026


Report Number : 3500987-1

Page 2 of 2


Wind Rose




Date : Mar 02-03, 2026




Date : Mar 03-04, 2026




Date : Mar 04-05, 2026




Date : Mar 05-06, 2026




Date : Mar 06-07, 2026



Date : Mar 07-08, 2026



Date : Mar 08-09, 2026



Date : Mar 02-09, 2026

WS (m/s)	%
≥ 10.0	0.00
8.0-10.0	0.00
5.5-8.0	0.00
3.3-5.5	2.38
1.7-3.3	17.86
0.3-1.7	58.93
Calms	20.83

Location : ราชฉนวน (GPS 47P 0734594, 1408565)

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any form without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

Approved by

Sarayuth Jitranont
Assistant General Manager



Analysis / Test Report

Client : THAI MMA Co., Ltd.

88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150

Lot ID: 2610898

Date Received :Mar 10, 2026

Date Reported :Mar 16, 2026

Report Number :3500987-1

P/O : PMM-2025-336

Project Name : Environmental Monitoring

Project Location : CCS Site 7

Page 1 of 2

Sample Number 2610898-15 to 21
Parameter Wind Speed / Wind Direction
Location บ้านเนินพยอม (GPS 47P 0736415, 1410971)
Sampling Date Mar 02 - Mar 09, 2026
Sampling by Santi Chaichana

Time	Mar 02 - Mar 03, 2026			Mar 03 - Mar 04, 2026			Mar 04 - Mar 05, 2026			Mar 05 - Mar 06, 2026			Mar 06 - Mar 07, 2026			Mar 07 - Mar 08, 2026			Mar 08 - Mar 09, 2026		
	WS (m/s)	WD (deg)		WS (m/s)	WD (deg)		WS (m/s)	WD (deg)		WS (m/s)	WD (deg)		WS (m/s)	WD (deg)		WS (m/s)	WD (deg)		WS (m/s)	WD (deg)	
02:00 PM - 03:00 PM	2.8	99.0	E	1.0	207.0	SSW	1.8	205.0	SSW	2.9	124.0	SE	1.9	267.0	W	2.0	0.0	N	2.5	304.0	NW
03:00 PM - 04:00 PM	3.0	170.0	S	3.2	146.0	SE	3.0	179.0	S	2.0	197.0	SSW	1.6	291.0	WNW	2.3	252.0	WSW	3.2	255.0	WSW
04:00 PM - 05:00 PM	2.4	185.0	S	2.2	123.0	ESE	1.9	215.0	SW	2.0	107.0	ESE	1.9	300.0	WNW	1.7	252.0	WSW	1.6	260.0	W
05:00 PM - 06:00 PM	1.7	178.0	S	1.2	144.0	SE	1.2	201.0	SSW	3.5	196.0	SSW	0.4	320.0	NW	0.0	-	-	0.9	345.0	NNW
06:00 PM - 07:00 PM	2.2	171.0	S	1.2	132.0	SE	1.2	130.0	SE	2.9	193.0	SSW	1.4	355.0	N	0.0	-	-	0.0	-	-
07:00 PM - 08:00 PM	1.5	169.0	S	0.6	140.0	SE	1.8	181.0	S	0.8	162.0	SSE	0.8	346.0	NNW	0.0	-	-	0.0	-	-
08:00 PM - 09:00 PM	1.6	129.0	SE	1.1	108.0	ESE	0.7	125.0	SE	1.5	126.0	SE	1.0	16.0	NNE	0.4	86.0	E	0.0	-	-
09:00 PM - 10:00 PM	0.0	-	-	0.6	101.0	E	0.3	192.0	SSW	0.3	142.0	SE	0.6	20.0	NNE	0.2	-	-	0.0	-	-
10:00 PM - 11:00 PM	0.6	144.0	SE	0.2	-	-	0.0	-	-	0.1	-	-	0.0	-	-	0.0	-	-	0.0	-	-
11:00 PM - 12:00 AM	0.2	-	-	1.7	144.0	SE	0.1	-	-	0.2	-	-	0.0	-	-	0.5	91.0	E	0.0	-	-
12:00 AM - 01:00 AM	0.8	122.0	ESE	0.8	163.0	SSE	0.2	-	-	0.3	3.0	N	0.5	289.0	WNW	0.0	-	-	0.0	-	-
01:00 AM - 02:00 AM	0.6	150.0	SSE	0.2	-	-	0.3	166.0	SSE	0.2	-	-	0.2	-	-	0.7	91.0	E	0.0	-	-
02:00 AM - 03:00 AM	1.0	216.0	SW	0.6	137.0	SE	0.5	198.0	SSW	0.7	71.0	ENE	0.1	-	-	0.2	-	-	0.3	92.0	E
03:00 AM - 04:00 AM	1.7	168.0	SSE	0.8	195.0	SSW	0.3	189.0	S	0.3	79.0	E	0.4	81.0	E	0.7	107.0	ESE	0.8	81.0	E
04:00 AM - 05:00 AM	0.2	-	-	2.1	185.0	S	0.1	-	-	0.4	130.0	SE	0.7	40.0	NE	0.0	-	-	1.6	89.0	E
05:00 AM - 06:00 AM	0.5	80.0	E	1.0	237.0	WSW	0.2	-	-	0.6	71.0	ENE	1.3	255.0	WSW	0.0	-	-	0.5	88.0	E
06:00 AM - 07:00 AM	0.6	9.0	N	0.2	-	-	0.4	226.0	SW	0.3	43.0	NE	0.3	64.0	ENE	1.1	69.0	ENE	0.6	104.0	ESE
07:00 AM - 08:00 AM	0.5	9.0	N	0.4	256.0	WSW	0.6	260.0	W	0.1	-	-	0.0	-	-	1.2	95.0	E	1.4	87.0	E
08:00 AM - 09:00 AM	0.5	5.0	N	0.2	-	-	1.0	275.0	W	1.7	35.0	NE	1.0	171.0	S	0.2	-	-	0.9	11.0	N
09:00 AM - 10:00 AM	0.1	-	-	0.4	4.0	N	0.8	322.0	NW	1.0	58.0	ENE	0.5	54.0	NE	1.5	167.0	SSE	1.0	166.0	SSE
10:00 AM - 11:00 AM	1.0	283.0	WNW	0.7	179.0	S	1.1	357.0	N	0.7	122.0	ESE	0.8	73.0	ENE	1.9	96.0	E	0.6	300.0	WNW
11:00 AM - 12:00 PM	0.8	101.0	E	1.4	227.0	SW	2.4	196.0	SSW	0.6	32.0	NNE	1.2	0.0	N	0.7	18.0	NNE	1.2	350.0	N
12:00 PM - 01:00 PM	1.3	112.0	ESE	1.5	225.0	SW	3.0	155.0	SSE	2.8	254.0	WSW	2.0	0.0	N	1.2	257.0	WSW	1.3	355.0	N
01:00 PM - 02:00 PM	1.4	192.0	SSW	1.5	175.0	S	1.5	150.0	SSE	2.9	268.0	W	1.1	252.0	WSW	2.1	266.0	W	2.0	321.0	NW

Reference Method : Cup Anemometer & Anodized Aluminium Vane Method

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any form without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

Approved by

Sarayuth Jittranont
Assistant General Manager



Analysis / Test Report

Client : THAI MMA Co., Ltd.

88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150

P/O : PMM-2025-336

Project Name : Environmental Monitoring

Project Location : CCS Site 7

Lot ID: 2610898

Date Received :Mar 10, 2026

Date Reported :Mar 16, 2026


Report Number :3500987-1

Page 2 of 2


Wind Rose




Date : Mar 02-03, 2026




Date : Mar 03-04, 2026




Date : Mar 04-05, 2026



Date : Mar 05-06, 2026




Date : Mar 06-07, 2026



Date : Mar 07-08, 2026



Date : Mar 08-09, 2026



Date : Mar 02-09, 2026

WS (m/s)	%
> 10.0	0.00
8.0-10.0	0.00
5.5-8.0	0.00
3.3-5.5	0.60
1.7-3.3	20.24
0.3-1.7	55.36
Calms	23.81

Location : บ้านเนินพยอม (GPS 47P 0736415, 1410971)

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any form without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

Approved by

Sarayuth Jitranont
Assistant General Manager

คุณภาพอากาศจากปล่องระบายอากาศ



Analysis / Test Report

TESTING
No.0042

Client : THAI MMA Co., Ltd.
88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150
P/O : PMM-2025-336
Project Name : Environmental Monitoring
Project Location : CCS Site 7

Lot ID: 2610904

Date Received : Mar 04, 2026
Date Reported : Mar 10, 2026
Report Number: 3501002-1

Page 1 of 2

Sample Number 2610904-1
Sampled Date Mar 04, 2026
Sample Description Emission from Stationary Source
Location Turbulence dust collector
Date Analysis Commenced Mar 05, 2026
Condition of Sample Extracted into one filter paper placed in plastic petri dish and one plastic bottle

Stack Description

Ambient Pressure	755	mmHg	Diameter	0.80	m	Oxygen	20.9	%
Ambient Temperature	33.4	°C	Shape	Circle		Carbon Dioxide	0.0	%
Type of Process	Process		Stack Temperature	36.0	°C	Gas Velocity	10.2	m/s
Type of Fuel	-		Moisture	2.42	%	Flow Rate (Actual O2)	17184	Nm3/hr

Analyte	Sampled Time	Unit	LOD	LOQ (LOR)	Result	Guideline (1)	Guideline (2)	Method	Testing Location
Air Testing									
Total Suspended Particulate	10:52 AM - 11:52 AM	mg/m3	-	0.5	<0.5	400	60	U.S. Environmental Protection Agency 40 CFR method 5, Appendix A, December 7, 2020 (Include sampling)	Rayong

Guideline : Guideline(1) : Notification of the Ministry of Industry 2006 (B.E. 2549) Published in the Royal Government Gazette, Vol.123 Special Part 125 D, dated December 4, 2006 (B.E. 2549)
Guideline(2) : Environmental Impact Assessment Report of THAI MMA Co., Ltd.

Technical Management

Thanita K.

Thanita Kulsuriwong
Scientist (4)
ทะเบียนเลขที่ ว-323-จ-0029

Approved by

D. Changchon.

Dej Changchon
Senior Manager
ทะเบียนเลขที่ ว-323-ค-0001

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. No part of this report may be reproduced in any form without written consent from the laboratory.
ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

TESTING
No.0042

Client : THAI MMA Co., Ltd.
88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150
P/O : PMM-2025-336
Project Name : Environmental Monitoring
Project Location : CCS Site 7

Lot ID: 2610904

Date Received : Mar 04, 2026
Date Reported : Mar 10, 2026
Report Number: 3501002-1

Page 2 of 2

Sample Number 2610904-1
Sampled Date Mar 04, 2026
Sample Description Emission from Stationary Source
Location Turbulence dust collector
Date Analysis Commenced Mar 05, 2026
Condition of Sample Extracted into one filter paper placed in plastic petri dish and one plastic bottle

Stack Description

Ambient Pressure	755	mmHg	Diameter	0.80	m	Oxygen	20.9	%
Ambient Temperature	33.4	°C	Shape	Circle		Carbon Dioxide	0.0	%
Type of Process	Process		Stack Temperature	36.0	°C	Gas Velocity	10.2	m/s
Type of Fuel	-		Moisture	2.42	%	Flow Rate (Actual O2)	17184	Nm3/hr

Analyte	Sampled Time	Unit	LOD	LOQ (LOR)	Result Emission Rate	Guideline (1)	Guideline (2)	Method	Testing Location
Air Testing									
Total Suspended Particulate *	10:52 AM - 11:52 AM	g/s	-	-	<0.002	-	0.22	Calculated	Rayong

Guideline : Guideline(1) : Notification of the Ministry of Industry 2006 (B.E. 2549) Published in the Royal Government Gazette, Vol.123 Special Part 125 D, dated December 4, 2006 (B.E. 2549)
Guideline(2) : Environmental Impact Assessment Report of THAI MMA Co., Ltd.

Sampling By : Sathapron Thakarw ทะเบียนเลขที่ ว-323-จ-0036

Remark :

- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)
- Analyte(s) marked * is/are not included in scope of Accreditation ISO/IEC 17025.

Technical Management

Thanita K.

Thanita Kulsuriwong
Scientist (4)
ทะเบียนเลขที่ ว-323-จ-0029

Approved by

D. Changchon

Dej Changchon
Senior Manager
ทะเบียนเลขที่ ว-323-ค-0001

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. No part of this report may be reproduced in any form without written consent from the laboratory.
ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER

16417-21/ EMAIL

S:\Reports_Air Stack_2GL.rpt (10:37AM)



Analysis / Test Report

Client : THAI MMA Co., Ltd.
88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150
P/O : PMM-2025-336
Project Name : Environmental Monitoring
Project Location : CCS Site 7

Lot ID: 2610905

Date Received : Mar 04, 2026
Date Reported : Mar 20, 2026
Report Number: 3501023-1

Page 1 of 2

Sample Number 2610905-1
Sampled Date Mar 04, 2026
Sample Description Emission from Stationary Source
Location Main Stack
Date Analysis Commenced Mar 05, 2026
Condition of Sample Extracted into two sorbent tube, refrigerated

Stack Description

Ambient Pressure	755	mmHg	Diameter	1.60 x 1.60	m	Oxygen	20.9	%
Ambient Temperature	33.4	°C	Shape	Square		Carbon Dioxide	0.0	%
Type of Process	Process		Stack Temperature	23.0	°C	Gas Velocity	3.6	m/s
Type of Fuel	-		Moisture	2.73	%	Flow Rate (Actual O2)	32401	Nm3/hr

Analyte	Sampled Time	Unit	LOD	LOQ (LOR)	Result	Guideline Limit	Method	Testing Location
Air Testing								
Butyl acrylate	11:00 AM - 11:15 AM	ppm	-	0.3	<0.3	No Standard	U.S. Environmental Protection Agency, EPA Method 18	Bangkok
Butyl acrylate	11:00 AM - 11:15 AM	mg/m3	-	1.0	<1.0	39	U.S. Environmental Protection Agency, EPA Method 18	Bangkok
Methyl Methacrylate	11:00 AM - 11:15 AM	ppm	-	0.3	18.0	No Standard	U.S. Environmental Protection Agency, EPA Method 18	Bangkok
Methyl Methacrylate	11:00 AM - 11:15 AM	mg/m3	-	1.0	73.7	520	U.S. Environmental Protection Agency, EPA Method 18	Bangkok

Approved by

Orawan R.

Orawan Rakyong
Scientist (3)

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.



Analysis / Test Report

Client : THAI MMA Co., Ltd.
88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150
P/O : PMM-2025-336
Project Name : Environmental Monitoring
Project Location : CCS Site 7

Lot ID: 2610905

Date Received : Mar 04, 2026
Date Reported : Mar 20, 2026
Report Number: 3501023-1

Page 2 of 2

Sample Number 2610905-1
Sampled Date Mar 04, 2026
Sample Description Emission from Stationary Source
Location Main Stack
Date Analysis Commenced Mar 05, 2026
Condition of Sample Extracted into two sorbent tube, refrigerated

Stack Description

Ambient Pressure	755	mmHg	Diameter	1.60 x 1.60	m	Oxygen	20.9	%
Ambient Temperature	33.4	°C	Shape	Square		Carbon Dioxide	0.0	%
Type of Process	Process		Stack Temperature	23.0	°C	Gas Velocity	3.6	m/s
Type of Fuel	-		Moisture	2.73	%	Flow Rate (Actual O2)	32401	Nm3/hr

Analyte	Sampled Time	Unit	LOD	LOQ (LOR)	Result Emission Rate	Guideline Limit	Method	Testing Location
Air Testing								
Butyl acrylate	11:00 AM - 11:15 AM	g/s	-	-	<0.01	0.13	Calculated	Bangkok
Methyl Methacrylate	11:00 AM - 11:15 AM	g/s	-	-	0.66	1.73	Calculated	Bangkok

Guideline : Environmental Impact Assessment Report of THAI MMA Co., Ltd.

Sampling By : Jakkarin Manwicha

Remark :

- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

Approved by

Orawan R.

Orawan Rakyong
Scientist (3)

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.



Analysis / Test Report

Client : THAI MMA Co., Ltd.
88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150
P/O : PMM-2025-336
Project Name : Environmental Monitoring
Project Location : CCS Site 7

Lot ID: 2610906

Date Received : Mar 04, 2026
Date Reported : Mar 10, 2026
Report Number: 3519401-1

Page 1 of 1

Sample Number 2610906-1
Sampled Date Mar 04, 2026
Sample Description Emission from Stationary Source
Location ปล่อง Carbon Absorber
Date Analysis Commenced Mar 06, 2026
Condition of Sample Extracted into one 10-L air sampling bag

Stack Description

Ambient Pressure	755	mmHg	Diameter	0.15	m	Oxygen	20.9	%
Ambient Temperature	33.4	°C	Shape	Circle		Carbon Dioxide	0.0	%
Type of Process	Process		Stack Temperature	33.0	°C	Gas Velocity	9.2	m/s
Type of Fuel	-		Moisture	3.17	%	Flow Rate (Actual O2)	551	Nm3/hr

Analyte	Sampled Time	Unit	LOD	LOQ (LOR)	Result	Method	Testing Location
Air Testing							
Total VOCs as Propane	11:25 AM - 11:35 AM	ppm	-	1.0	28.2	U.S. Environmental Protection Agency, EPA Method 25A	Rayong

Sampling By : Jakkarin Manwicha

Remark :

- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

Approved by

Thanita K.

Thanita Kulsuriwong
Scientist (4)

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. No part of this report may be reproduced in any form without written consent from the laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

คุณภาพน้ำ



Analysis / Test Report

Client : THAI MMA Co., Ltd.
88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150

P/O :

Project Name : Environmental Monitoring

Project Location: CCS Site 7

TESTING

No.0042

Lot ID: 25114666

Date Received : Jan 12, 2026

Date Reported : Jan 19, 2026

Report Number : 3478151-1

Page 1 of 2

Sample Number	25114666-1						
Sampled Date	Jan 12, 2026 1:55 PM						
Sample Description	Wastewater						
Location	บ่อสุดท้าย Cesspool						
Date Analysis Commenced	Jan 12, 2026						
Condition of Sample	Contained in one amber glass bottle and three plastic bottles, sample containers comply to pretreatment - preservation standards (APHA, USEPA)						

Analyte	Unit	LOD	LOQ (LOR)	Result	Guideline / Specification	Method	Testing Location
Water Testing							
BOD (5 days at 20 Degree C)	mg/L	-	2.0	25.0	≤500	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5210 B, part 4500 - O G	Rayong
COD	mg/L	1.5	25	60	≤750	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5220 D	Rayong
Oil & Grease	mg/L	-	3	<3	≤10	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5520 B	Rayong
pH at 25 degree C		-	-	7.3	5.5-9.0	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 4500 - H (B)	Rayong
Sulfate *	mg/L	0.6	2	56.9	No Standard	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 4500-SO4 (E)	Rayong
Temperature *	Degree C	-	-	32.2	≤45	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 2550 B	Rayong
Total Dissolved Solids Dried at 180 degree C	mg/L	-	5	240	≤3000	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 2540 C	Rayong
Total Suspended Solids Dried at 103-105 degree C	mg/L	-	5	<5	≤200	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 2540 D	Rayong

Guideline : Notification of the Industrial Estate Authority of Thailand No.029/2567 : General Standards for Wastewater drainage into central wastewater treatment systems in Industrial Estates.

Sampling By : Wanlop Hunchainaow ทะเบียนเลขที่ ว-323-จ-0038

Remark :

Technical Management

Photchana S

Photchana Seeda

Scientist (4)

ทะเบียนเลขที่ ว-323-จ-0028

Approved by

D. Chumson.

Dej Changchon

Senior Manager

ทะเบียนเลขที่ ว-323-ค-0001

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

Client : THAI MMA Co., Ltd.
88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150

P/O :

Project Name : Environmental Monitoring

Project Location: CCS Site 7

TESTING

No.0042

Lot ID: 25114666

Date Received : Jan 12, 2026

Date Reported : Jan 19, 2026

Report Number : 3478151-1

Page 2 of 2

- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)
- Analyte(s) marked * is/are not included in scope of Accreditation ISO/IEC 17025.
- Sampling is not included in scope of accreditation ISO/IEC 17025

Technical Management

PhotchanaS

Photchana Seeda
Scientist (4)

ทะเบียนเลขที่ ว-323-จ-0028

Approved by

D. Changchon

Dej Changchon
Senior Manager

ทะเบียนเลขที่ ว-323-ค-0001

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

TESTING
No.0042

Client : THAI MMA Co., Ltd.
88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150
P/O : PMM-2025-336
Project Name : Environmental Monitoring
Project Location : CCS Site 7

Lot ID: 266124

Date Received : Feb 06, 2026

Date Reported : Feb 13, 2026

Report Number : 3491819-1

Page 1 of 2

Sample Number	266124-1
Sampled Date	Feb 06, 2026 1:50 PM
Sample Description	Wastewater
Location	บ่อสุดท้าย Cesspool
Date Analysis Commenced	Feb 06, 2026
Condition of Sample	Contained in one amber glass bottle and three plastic bottles, sample containers comply to pretreatment - preservation standards (APHA, USEPA)

Analyte	Unit	LOD	LOQ (LOR)	Result	Guideline / Specification	Method	Testing Location
Water Testing							
BOD (5 days at 20 Degree C)	mg/L	-	2.0	46.3	≤500	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5210 B, part 4500 - O G	Rayong
COD	mg/L	1.5	25	65	≤750	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5220 D	Rayong
Oil & Grease	mg/L	-	3	<3	≤10	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5520 B	Rayong
pH at 25 degree C		-	-	8.2	5.5-9.0	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 4500 - H (B)	Rayong
Temperature *	Degree C	-	-	37.4	≤45	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 2550 B	Rayong
Total Dissolved Solids Dried at 180 degree C	mg/L	-	5	302	≤3000	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 2540 C	Rayong
Total Suspended Solids Dried at 103-105 degree C	mg/L	-	5	<5	≤200	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 2540 D	Rayong

Guideline : Notification of the Industrial Estate Authority of Thailand No.029/2567 : General Standards for Wastewater drainage into central wastewater treatment systems in Industrial Estates.

Sampling By : Wanlop Hunchainaow ทะเบียนเลขที่ ว-323-จ-0038

Remark :

- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)
- Analyte(s) marked * is/are not included in scope of Accreditation ISO/IEC 17025.
- Sampling is not included in scope of accreditation ISO/IEC 17025

Technical Management

Photchana S

Photchana Seeda

Scientist (4)

ทะเบียนเลขที่ ว-323-จ-0028

Approved by

D. Chumson

Dej Changchon

Senior Manager

ทะเบียนเลขที่ ว-323-ค-0001

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

Client : THAI MMA Co., Ltd.
88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150
P/O : PMM-2025-336
Project Name : Environmental Monitoring
Project Location : CCS Site 7

TESTING
No.0042
Lot ID: 266124
Date Received : Feb 06, 2026
Date Reported : Feb 13, 2026
Report Number : 3491819-1

Page 2 of 2

Technical Management

PhotchanaS

Photchana Seeda
Scientist (4)
ทะเบียนเลขที่ ว-323-จ-0028

Approved by

D. Johnson

Dej Changchon
Senior Manager
ทะเบียนเลขที่ ว-323-ค-0001

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

Client : THAI MMA Co., Ltd.
88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150
P/O : PMM-2025-336
Project Name : Environmental Monitoring
Project Location : CCS Site 7

Lot ID: 266124

Date Received : Feb 06, 2026

Date Reported : Feb 13, 2026

Report Number : 3491819-2

Page 1 of 1

Sample Number	266124-1
Sampled Date	Feb 06, 2026 1:50 PM
Sample Description	Wastewater
Location	บ่อสุดท้าย Cesspool
Date Analysis Commenced	Feb 11, 2026
Condition of Sample	Contained in one amber glass bottle and three plastic bottles, sample containers comply to pretreatment - preservation standards (APHA, USEPA)

Analyte	Unit	LOD	LOQ (LOR)	Result	Guideline / Specification	Method	Testing Location
Water Testing							
Sulfate	mg/L	0.6	2	60.0	No Standard	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 4500-SO4 (E)	Rayong

Guideline : Notification of the Industrial Estate Authority of Thailand No.029/2567 : General Standards for Wastewater drainage into central wastewater treatment systems in Industrial Estates.

Sampling By : Wanlop Hunchainaow

Remark :

- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

Approved by

PhotchanaS

Photchana Seeda
Scientist (4)

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

Client : THAI MMA Co., Ltd.
88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150
P/O : PMM-2025-336
Project Name : Environmental Monitoring
Project Location : CCS Site 7

TESTING
No.0042

Lot ID: 2610909

Date Received : Mar 11, 2026

Date Reported : Mar 18, 2026

Report Number : 3501050-1

Page 1 of 2

Sample Number	2610909-1
Sampled Date	Mar 11, 2026 2:00 PM
Sample Description	Wastewater
Location	บ่อสุดท้าย Cesspool
Date Analysis Commenced	Mar 11, 2026
Condition of Sample	Contained in one amber glass bottle and three plastic bottles, sample containers comply to pretreatment - preservation standards (APHA, USEPA)

Analyte	Unit	LOD	LOQ (LOR)	Result	Guideline / Specification	Method	Testing Location
Water Testing							
BOD (5 days at 20 Degree C)	mg/L	-	2.0	17.5	≤500	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5210 B, part 4500 - O G	Rayong
COD	mg/L	1.5	25	57	≤750	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5220 D	Rayong
Oil & Grease	mg/L	-	3	<3	≤10	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5520 B	Rayong
pH at 25 degree C		-	-	7.2	5.5-9.0	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 4500 - H (B)	Rayong
Temperature *	Degree C	-	-	33.8	≤45	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 2550 B	Rayong
Total Dissolved Solids Dried at 180 degree C	mg/L	-	5	324	≤3000	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 2540 C	Rayong
Total Suspended Solids Dried from 103-105 degree C	mg/L	-	5	8	≤200	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 2540 D	Rayong

Guideline : Notification of the Industrial Estate Authority of Thailand No.029/2567 : General Standards for Wastewater drainage into central wastewater treatment systems in Industrial Estates.

Sampling By : Wanlop Hunchainaow ทะเบียนเลขที่ ว-323-จ-0038

Remark :

- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)
- Analyte(s) marked * is/are not included in scope of Accreditation ISO/IEC 17025.
- Sampling is not included in scope of accreditation ISO/IEC 17025

Technical Management

Photchana S

Photchana Seeda

Scientist (4)

ทะเบียนเลขที่ ว-323-จ-0028

Approved by

D. Changchon

Dej Changchon

Senior Manager

ทะเบียนเลขที่ ว-323-ค-0001

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

Client : THAI MMA Co., Ltd.
88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150
P/O : PMM-2025-336
Project Name : Environmental Monitoring
Project Location : CCS Site 7

TESTING
No.0042
Lot ID: 2610909
Date Received : Mar 11, 2026
Date Reported : Mar 18, 2026
Report Number : 3501050-1

Page 2 of 2

Technical Management

PhotchanaS

Photchana Seeda
Scientist (4)
ทะเบียนเลขที่ ว-323-จ-0028

Approved by

D. Chumson.

Dej Changchon
Senior Manager
ทะเบียนเลขที่ ว-323-ค-0001

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

Client : THAI MMA Co., Ltd.
88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150

P/O : PMM-2025-336

Project Name : Environmental Monitoring

Project Location : CCS Site 7

Lot ID: 2610909

Date Received : Mar 11, 2026

Date Reported : Mar 18, 2026

Report Number : 3501050-2

Page 1 of 1

Sample Number	2610909-1						
Sampled Date	Mar 11, 2026 2:00 PM						
Sample Description	Wastewater						
Location	บ่อเสถียร Cesspool						
Date Analysis Commenced	Mar 11, 2026						
Condition of Sample	Contained in one amber glass bottle and three plastic bottles, sample containers comply to pretreatment - preservation standards (APHA, USEPA)						

Analyte	Unit	LOD	LOQ (LOR)	Result	Guideline / Specification	Method	Testing Location
Water Testing							
Sulfate	mg/L	0.6	2	61.3	No Standard	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 4500-SO4 (E)	Rayong

Guideline : Notification of the Industrial Estate Authority of Thailand No.029/2567 : General Standards for Wastewater drainage into central wastewater treatment systems in Industrial Estates.

Sampling By : Wanlop Hunchainaow

Remark :

- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

Approved by

PhotchanaS

Photchana Seeda
Scientist (4)

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

Client : THAI MMA Co., Ltd.
88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150
P/O : PMM-2025-336
Project Name : Environmental Monitoring
Project Location : CCS Site 7

TESTING
No.0042

Lot ID: 2623675

Date Received : Apr 10, 2026

Date Reported : Apr 21, 2026

Report Number : 3529269-1

Page 1 of 2

Sample Number	2623675-1						
Sampled Date	Apr 10, 2026 1:58 PM						
Sample Description	Wastewater						
Location	บ่อสุดท้าย Cesspool						
Date Analysis Commenced	Apr 10, 2026						
Condition of Sample	Contained in one amber glass bottle and three plastic bottles, sample containers comply to pretreatment - preservation standards (APHA, USEPA)						

Analyte	Unit	LOD	LOQ (LOR)	Result	Guideline / Specification	Method	Testing Location
Water Testing							
BOD (5 days at 20 Degree C)	mg/L	-	2.0	13.6	≤500	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5210 B, part 4500 - O G	Rayong
COD	mg/L	1.5	25	56	≤750	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5220 D	Rayong
Oil & Grease	mg/L	-	3	<3	≤10	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5520 B	Rayong
pH at 25 degree C		-	-	7.1	5.5-9.0	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 4500 - H (B)	Rayong
Temperature *	Degree C	-	-	34.6	≤45	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 2550 B	Rayong
Total Dissolved Solids Dried at 180 degree C	mg/L	-	5	294	≤3000	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 2540 C	Rayong
Total Suspended Solids Dried from 103-105 degree C	mg/L	-	5	<5	≤200	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 2540 D	Rayong

Guideline : Notification of the Industrial Estate Authority of Thailand No.029/2567 : General Standards for Wastewater drainage into central wastewater treatment systems in Industrial Estates.

Sampling By : Wanlop Hunchainaow ทะเบียนเลขที่ ว-323-จ-0038

Remark :

- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)
- Analyte(s) marked * is/are not included in scope of Accreditation ISO/IEC 17025.
- Sampling is not included in scope of accreditation ISO/IEC 17025

Technical Management

Photchana S

Photchana Seeda

Scientist (4)

ทะเบียนเลขที่ ว-323-จ-0028

Approved by

D. Chumson

Dej Changchon

Senior Manager

ทะเบียนเลขที่ ว-323-ค-0001

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

Client : THAI MMA Co., Ltd.
88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150
P/O : PMM-2025-336
Project Name : Environmental Monitoring
Project Location : CCS Site 7

TESTING
No.0042
Lot ID: 2623675
Date Received : Apr 10, 2026
Date Reported : Apr 21, 2026
Report Number : 3529269-1

Page 2 of 2

Technical Management

PhotchanaS

Photchana Seeda
Scientist (4)
ทะเบียนเลขที่ ว-323-จ-0028

Approved by

D. Chumson

Dej Changchon
Senior Manager
ทะเบียนเลขที่ ว-323-ค-0001

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

Client : THAI MMA Co., Ltd.
88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150

P/O : PMM-2025-336

Project Name : Environmental Monitoring

Project Location : CCS Site 7

Lot ID: 2623675

Date Received : Apr 10, 2026

Date Reported : Apr 21, 2026

Report Number : 3529269-2

Page 1 of 1

Sample Number	2623675-1						
Sampled Date	Apr 10, 2026 1:58 PM						
Sample Description	Wastewater						
Location	บ่อเสาะน้ำ Cesspool						
Date Analysis Commenced	Apr 10, 2026						
Condition of Sample	Contained in one amber glass bottle and three plastic bottles, sample containers comply to pretreatment - preservation standards (APHA, USEPA)						

Analyte	Unit	LOD	LOQ (LOR)	Result	Guideline / Specification	Method	Testing Location
Water Testing							
Sulfate	mg/L	0.6	2	70.1	No Standard	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 4500-SO4 (E)	Rayong

Guideline : Notification of the Industrial Estate Authority of Thailand No.029/2567 : General Standards for Wastewater drainage into central wastewater treatment systems in Industrial Estates.

Sampling By : Wanlop Hunchainaow

Remark :

- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

Approved by

PhotchanaS

Photchana Seeda
Scientist (4)

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

TESTING
No.0042

Client : THAI MMA Co., Ltd.
88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150
P/O : PMM-2025-336
Project Name : Environmental Monitoring
Project Location : CCS Site 7

Lot ID: 2633650
Date Received : May 08, 2026
Date Reported : May 15, 2026
Report Number : 3554968-1

Page 1 of 2

Sample Number	2633650-1
Sampled Date	May 08, 2026 1:56 PM
Sample Description	Wastewater
Location	บ่อสุดท้าย Cesspool
Date Analysis Commenced	May 08, 2026
Condition of Sample	Contained in one amber glass bottle and three plastic bottles, sample containers comply to pretreatment - preservation standards (APHA, USEPA)

Analyte	Unit	LOD	LOQ (LOR)	Result	Guideline / Specification	Method	Testing Location
Water Testing							
BOD (5 days at 20 Degree C)	mg/L	-	2.0	39.2	≤500	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5210 B, part 4500 - O G	Rayong
COD	mg/L	1.5	25	76	≤750	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5220 D	Rayong
Oil & Grease	mg/L	-	3	<3	≤10	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5520 B	Rayong
pH at 25 degree C		-	-	6.9	5.5-9.0	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 4500 - H (B)	Rayong
Temperature *	Degree C	-	-	34.6	≤45	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 2550 B	Rayong
Total Dissolved Solids Dried at 180 degree C	mg/L	-	5	252	≤3000	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 2540 C	Rayong
Total Suspended Solids Dried from 103-105 degree C	mg/L	-	5	8	≤200	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 2540 D	Rayong

Guideline : Notification of the Industrial Estate Authority of Thailand No.029/2567 : General Standards for Wastewater drainage into central wastewater treatment systems in Industrial Estates.

Sampling By : Wanlop Hunchainaow ทะเบียนเลขที่ ว-323-จ-0038

Remark :

- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)
- Analyte(s) marked * is/are not included in scope of Accreditation ISO/IEC 17025.
- Sampling is not included in scope of accreditation ISO/IEC 17025

Technical Management

Photchana S

Photchana Seeda
Scientist (4)

ทะเบียนเลขที่ ว-323-จ-0028

Approved by

D. Chumson

Dej Changchon
Senior Manager

ทะเบียนเลขที่ ว-323-ค-0001

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

Client : THAI MMA Co., Ltd.
88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150
P/O : PMM-2025-336
Project Name : Environmental Monitoring
Project Location: CCS Site 7

TESTING
No.0042
Lot ID: 2633650
Date Received : May 08, 2026
Date Reported : May 15, 2026
Report Number : 3554968-1

Page 2 of 2

Technical Management

PhotchanaS

Photchana Seeda
Scientist (4)
ทะเบียนเลขที่ ว-323-จ-0028

Approved by

D. Chumson.

Dej Changchon
Senior Manager
ทะเบียนเลขที่ ว-323-ค-0001

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

Client : THAI MMA Co., Ltd.
88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150

P/O : PMM-2025-336

Project Name : Environmental Monitoring

Project Location : CCS Site 7

Lot ID: 2633650

Date Received : May 08, 2026

Date Reported : May 15, 2026

Report Number : 3554968-2

Page 1 of 1

Sample Number	2633650-1						
Sampled Date	May 08, 2026 1:56 PM						
Sample Description	Wastewater						
Location	บ่อเสาะน้ำ Cesspool						
Date Analysis Commenced	May 11, 2026						
Condition of Sample	Contained in one amber glass bottle and three plastic bottles, sample containers comply to pretreatment - preservation standards (APHA, USEPA)						

Analyte	Unit	LOD	LOQ (LOR)	Result	Guideline / Specification	Method	Testing Location
Water Testing							
Sulfate	mg/L	0.6	2	54.1	No Standard	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 4500-SO4 (E)	Rayong

Guideline : Notification of the Industrial Estate Authority of Thailand No.029/2567 : General Standards for Wastewater drainage into central wastewater treatment systems in Industrial Estates.

Sampling By : Wanlop Hunchainaow

Remark :

- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

Approved by

PhotchanaS

Photchana Seeda
Scientist (4)

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

Client : THAI MMA Co., Ltd.
88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150
P/O : PMM-2025-336
Project Name : Environmental Monitoring
Project Location : CCS Site 7

TESTING
No.0042

Lot ID: 2643436

Date Received : Jun 12, 2026

Date Reported : Jun 19, 2026

Report Number : 3574605-1

Page 1 of 2

Sample Number	2643436-1
Sampled Date	Jun 12, 2026 1:45 PM
Sample Description	Wastewater
Location	บ่อสุดท้าย Cesspool
Date Analysis Commenced	Jun 12, 2026
Condition of Sample	Contained in one amber glass bottle and three plastic bottles, sample containers comply to pretreatment - preservation standards (APHA, USEPA)

Analyte	Unit	LOD	LOQ (LOR)	Result	Guideline / Specification	Method	Testing Location
Water Testing							
BOD (5 days at 20 Degree C)	mg/L	-	2.0	30.0	≤500	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5210 B, part 4500 - O G	Rayong
COD	mg/L	1.5	25	71	≤750	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5220 D	Rayong
Oil & Grease	mg/L	-	3	<3	≤10	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5520 B	Rayong
pH at 25 degree C		-	-	7.3	5.5-9.0	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 4500 - H (B)	Rayong
Sulfate *	mg/L	0.6	2	45.8	No Standard	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 4500-SO4 (E)	Rayong
Temperature *	Degree C	-	-	33.8	≤45	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 2550 B	Rayong
Total Dissolved Solids Dried at 180 degree C	mg/L	-	5	314	≤3000	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 2540 C	Rayong
Total Suspended Solids Dried from 103-105 degree C	mg/L	-	5	10	≤200	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 2540 D	Rayong

Guideline : Notification of the Industrial Estate Authority of Thailand No.029/2567 : General Standards for Wastewater drainage into central wastewater treatment systems in Industrial Estates.

Sampling By : Wanlop Hunchainaow ทะเบียนเลขที่ ว-323-จ-0038

Remark :

Technical Management

Photchana S

Photchana Seeda

Scientist (4)

ทะเบียนเลขที่ ว-323-จ-0028

Approved by

D. Chongchon

Dej Changchon

Senior Manager

ทะเบียนเลขที่ ว-323-ค-0001

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

Client : THAI MMA Co., Ltd.
88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150
P/O : PMM-2025-336
Project Name : Environmental Monitoring
Project Location: CCS Site 7

TESTING
No.0042
Lot ID: 2643436
Date Received : Jun 12, 2026
Date Reported : Jun 19, 2026
Report Number : 3574605-1

Page 2 of 2

- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)
- Analyte(s) marked * is/are not included in scope of Accreditation ISO/IEC 17025.
- Sampling is not included in scope of accreditation ISO/IEC 17025

Technical Management

PhotchanaS

Photchana Seeda
Scientist (4)

ทะเบียนเลขที่ ว-323-จ-0028

Approved by

D. Chumson.

Dej Changchon
Senior Manager

ทะเบียนเลขที่ ว-323-ค-0001

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER

ระดับเสียง



Analysis / Test Report

TESTING
No.0042

Client : THAI MMA Co., Ltd.
88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150
P/O : PMM-2025-336
Project Name : Environmental Monitoring
Project Location : CCS Site 7

Lot ID: 2610902

Date Received : Mar 10, 2026
Date Reported : Mar 14, 2026
Report Number: 3528034-1

Page 1 of 1

Sample Number 2610902-1
Parameter Noise (Leq 24 hrs.)
Location บ้านบน (GPS 47P 0735641, 1409191)
Measurement Date Mar 02 - Mar 03, 2026
Measurement by Santi Chaichana
Sound Level meter Serial No. 734221

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
12:00 PM - 01:00 PM	59.8	76.3	56.2
01:00 PM - 02:00 PM	59.0	79.5	55.6
02:00 PM - 03:00 PM	59.2	84.3	56.1
03:00 PM - 04:00 PM	58.5	77.9	56.0
04:00 PM - 05:00 PM	58.8	76.4	56.3
05:00 PM - 06:00 PM	59.0	77.3	56.8
06:00 PM - 07:00 PM	59.7	79.7	56.5
07:00 PM - 08:00 PM	59.0	78.9	54.6
08:00 PM - 09:00 PM	55.8	82.6	46.4
09:00 PM - 10:00 PM	54.9	77.7	45.2
10:00 PM - 11:00 PM	54.8	78.2	43.9
11:00 PM - 12:00 AM	54.6	76.4	43.8
12:00 AM - 01:00 AM	55.2	75.9	44.2
01:00 AM - 02:00 AM	50.5	68.8	42.7
02:00 AM - 03:00 AM	52.8	75.6	43.1
03:00 AM - 04:00 AM	52.2	74.8	43.4
04:00 AM - 05:00 AM	53.1	72.6	45.6
05:00 AM - 06:00 AM	60.6	82.5	52.3
06:00 AM - 07:00 AM	59.2	83.3	53.3
07:00 AM - 08:00 AM	58.0	73.5	54.7
08:00 AM - 09:00 AM	58.1	69.5	54.8
09:00 AM - 10:00 AM	58.9	79.5	56.1
10:00 AM - 11:00 AM	58.2	70.9	55.5
11:00 AM - 12:00 PM	57.9	74.7	55.3

Leq Average 24 hrs. (dB(A)) 57.7
Lmax (dB(A)) 84.3
L90 (dB(A)) 54.6
Ldn (dB(A)) 62.9
Standard (dB(A)) 70 115

Reference Method : ISO 1996-1 : 2016

Standard : 1. ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ ฉบับที่ 15 (พ.ศ. 2540) เรื่องกำหนดมาตรฐานระดับเสียงโดยทั่วไป
2. ประกาศกระทรวงอุตสาหกรรม เรื่องกำหนดค่าระดับเสียงการรบกวน และระดับเสียงที่เกิดจากการประกอบกิจการโรงงาน พ.ศ. 2548

Remark : The laboratory has been accepted as an accredited laboratory complying with the ISO/IEC 17025.

Technical Management

Thanita K.

Thanita Kulsuriwong
Scientist (4)

Approved by

Supot S.

Supot Salamteh
Section Head

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

TESTING
No.0042

Client : THAI MMA Co., Ltd.
88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150
P/O : PMM-2025-336
Project Name : Environmental Monitoring
Project Location : CCS Site 7

Lot ID: 2610902
Date Received : Mar 10, 2026
Date Reported : Mar 14, 2026
Report Number: 3528035-1

Page 1 of 1

Sample Number 2610902-2
Parameter Noise (Leq 24 hrs.)
Location บ้านบน (GPS 47P 0735641, 1409191)
Measurement Date Mar 03 - Mar 04, 2026
Measurement by Santi Chaichana
Sound Level meter Serial No. 734221

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
12:00 PM - 01:00 PM	58.6	78.7	55.6
01:00 PM - 02:00 PM	58.3	74.3	55.6
02:00 PM - 03:00 PM	58.7	77.7	55.8
03:00 PM - 04:00 PM	59.2	73.3	56.3
04:00 PM - 05:00 PM	59.9	77.4	56.5
05:00 PM - 06:00 PM	59.1	77.9	56.3
06:00 PM - 07:00 PM	59.7	86.7	56.4
07:00 PM - 08:00 PM	58.5	79.5	54.2
08:00 PM - 09:00 PM	56.1	74.2	47.1
09:00 PM - 10:00 PM	52.6	75.3	42.9
10:00 PM - 11:00 PM	52.0	81.7	41.8
11:00 PM - 12:00 AM	51.1	75.5	41.4
12:00 AM - 01:00 AM	50.2	70.5	40.8
01:00 AM - 02:00 AM	51.0	76.6	40.6
02:00 AM - 03:00 AM	49.4	70.9	39.8
03:00 AM - 04:00 AM	50.7	68.8	41.0
04:00 AM - 05:00 AM	54.1	76.1	44.9
05:00 AM - 06:00 AM	59.7	78.2	52.5
06:00 AM - 07:00 AM	61.2	76.4	56.6
07:00 AM - 08:00 AM	58.6	75.1	55.1
08:00 AM - 09:00 AM	58.7	78.9	55.0
09:00 AM - 10:00 AM	59.1	74.5	56.0
10:00 AM - 11:00 AM	58.5	75.1	55.3
11:00 AM - 12:00 PM	57.7	73.9	54.9

Leq Average 24 hrs. (dB(A)) 57.6
Lmax (dB(A)) 86.7
L90 (dB(A)) 54.9
Ldn (dB(A)) 62.5
Standard (dB(A)) 70 115

Reference Method : ISO 1996-1 : 2016

Standard : 1. ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ ฉบับที่ 15 (พ.ศ. 2540) เรื่องกำหนดมาตรฐานระดับเสียงโดยทั่วไป
2. ประกาศกระทรวงอุตสาหกรรม เรื่องกำหนดค่าระดับเสียงการรบกวน และระดับเสียงที่เกิดจากการประกอบกิจการโรงงาน พ.ศ. 2548

Remark : The laboratory has been accepted as an accredited laboratory complying with the ISO/IEC 17025.

Technical Management

Thanita K.

Thanita Kulsuriwong
Scientist (4)

Approved by

Supot S.

Supot Salamteh
Section Head

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

TESTING
No.0042

Client : THAI MMA Co., Ltd.
88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150
P/O : PMM-2025-336
Project Name : Environmental Monitoring
Project Location : CCS Site 7

Lot ID: 2610902
Date Received : Mar 10, 2026
Date Reported : Mar 14, 2026
Report Number: 3528036-1

Page 1 of 1

Sample Number 2610902-3
Parameter Noise (Leq 24 hrs.)
Location บ้านบน (GPS 47P 0735641, 1409191)
Measurement Date Mar 04 - Mar 05, 2026
Measurement by Santi Chaichana
Sound Level meter Serial No. 734221

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
12:00 PM - 01:00 PM	57.7	79.0	54.7
01:00 PM - 02:00 PM	56.9	73.1	54.4
02:00 PM - 03:00 PM	57.9	79.6	54.5
03:00 PM - 04:00 PM	56.9	72.0	54.9
04:00 PM - 05:00 PM	57.9	70.8	55.7
05:00 PM - 06:00 PM	58.3	70.6	56.3
06:00 PM - 07:00 PM	58.6	73.0	56.3
07:00 PM - 08:00 PM	58.7	77.5	54.2
08:00 PM - 09:00 PM	55.9	74.8	46.4
09:00 PM - 10:00 PM	55.7	74.5	44.5
10:00 PM - 11:00 PM	53.0	72.7	42.0
11:00 PM - 12:00 AM	53.3	77.2	41.3
12:00 AM - 01:00 AM	51.5	77.0	40.3
01:00 AM - 02:00 AM	49.2	72.5	40.1
02:00 AM - 03:00 AM	48.6	69.1	39.7
03:00 AM - 04:00 AM	51.8	77.5	40.8
04:00 AM - 05:00 AM	55.6	78.4	43.5
05:00 AM - 06:00 AM	60.3	81.4	53.3
06:00 AM - 07:00 AM	59.4	77.6	54.2
07:00 AM - 08:00 AM	57.9	75.4	54.3
08:00 AM - 09:00 AM	57.9	71.1	54.3
09:00 AM - 10:00 AM	58.1	70.3	55.1
10:00 AM - 11:00 AM	59.1	84.2	55.2
11:00 AM - 12:00 PM	59.9	85.0	56.0

Leq Average 24 hrs. (dB(A)) 57.2
Lmax (dB(A)) 85.0
L90 (dB(A)) 54.2
Ldn (dB(A)) 62.3
Standard (dB(A)) 70 115

Reference Method : ISO 1996-1 : 2016

Standard : 1. ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ ฉบับที่ 15 (พ.ศ. 2540) เรื่องกำหนดมาตรฐานระดับเสียงโดยทั่วไป
2. ประกาศกระทรวงอุตสาหกรรม เรื่องกำหนดค่าระดับเสียงการรบกวน และระดับเสียงที่เกิดจากการประกอบกิจการโรงงาน พ.ศ. 2548

Remark : The laboratory has been accepted as an accredited laboratory complying with the ISO/IEC 17025.

Technical Management

Thanita K.

Thanita Kulsuriwong
Scientist (4)

Approved by

Supot S.

Supot Salamteh
Section Head

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report



TESTING
No.0042

Client : THAI MMA Co., Ltd.
88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150
P/O : PMM-2025-336
Project Name : Environmental Monitoring
Project Location : CCS Site 7

Lot ID: 2610902

Date Received : Mar 10, 2026
Date Reported : Mar 14, 2026
Report Number: 3528037-1

Page 1 of 1

Sample Number 2610902-4
Parameter Noise (Leq 24 hrs.)
Location บ้านนาบยา (GPS 47P 0734556, 1408551)
Measurement Date Mar 02 - Mar 03, 2026
Measurement by Santi Chaichana
Sound Level meter Serial No. 233183

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
01:00 PM - 02:00 PM	60.4	76.9	56.8
02:00 PM - 03:00 PM	59.6	80.1	56.2
03:00 PM - 04:00 PM	59.8	84.9	56.7
04:00 PM - 05:00 PM	59.1	78.5	56.6
05:00 PM - 06:00 PM	59.4	77.0	56.9
06:00 PM - 07:00 PM	59.6	77.9	57.4
07:00 PM - 08:00 PM	60.3	80.3	57.1
08:00 PM - 09:00 PM	59.6	79.5	55.2
09:00 PM - 10:00 PM	56.4	83.2	47.0
10:00 PM - 11:00 PM	55.5	78.3	45.8
11:00 PM - 12:00 AM	55.4	78.8	44.5
12:00 AM - 01:00 AM	55.2	77.0	44.4
01:00 AM - 02:00 AM	55.8	76.5	44.8
02:00 AM - 03:00 AM	51.1	69.4	43.3
03:00 AM - 04:00 AM	53.4	76.2	43.7
04:00 AM - 05:00 AM	52.8	75.4	44.0
05:00 AM - 06:00 AM	53.7	73.2	46.2
06:00 AM - 07:00 AM	61.2	83.1	52.9
07:00 AM - 08:00 AM	59.8	83.9	53.9
08:00 AM - 09:00 AM	58.6	74.1	55.3
09:00 AM - 10:00 AM	58.7	70.1	55.4
10:00 AM - 11:00 AM	59.5	80.1	56.7
11:00 AM - 12:00 PM	58.8	71.5	56.1
12:00 PM - 01:00 PM	58.5	75.3	55.9

Leq Average 24 hrs. (dB(A)) 58.3
Lmax (dB(A)) 84.9
L90 (dB(A)) 55.2
Ldn (dB(A)) 63.0
Standard (dB(A)) 70 115

Reference Method : ISO 1996-1 : 2016

Standard : 1. ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ ฉบับที่ 15 (พ.ศ. 2540) เรื่องกำหนดมาตรฐานระดับเสียงโดยทั่วไป
2. ประกาศกระทรวงอุตสาหกรรม เรื่องกำหนดค่าระดับเสียงการรบกวน และระดับเสียงที่เกิดจากการประกอบกิจการโรงงาน พ.ศ. 2548

Remark : The laboratory has been accepted as an accredited laboratory complying with the ISO/IEC 17025.

Technical Management

Thanita K.

Thanita Kulsuriwong
Scientist (4)

Approved by

Supot S.

Supot Salamteh
Section Head



Analysis / Test Report



TESTING
No.0042

Client : THAI MMA Co., Ltd.
88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150
P/O : PMM-2025-336
Project Name : Environmental Monitoring
Project Location : CCS Site 7

Lot ID: 2610902

Date Received : Mar 10, 2026
Date Reported : Mar 14, 2026
Report Number: 3528038-1

Page 1 of 1

Sample Number 2610902-5
Parameter Noise (Leq 24 hrs.)
Location บ้านนาบยา (GPS 47P 0734556, 1408551)
Measurement Date Mar 03 - Mar 04, 2026
Measurement by Santi Chaichana
Sound Level meter Serial No. 233183

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
01:00 PM - 02:00 PM	59.2	79.3	56.2
02:00 PM - 03:00 PM	58.9	74.9	56.2
03:00 PM - 04:00 PM	59.3	78.3	56.4
04:00 PM - 05:00 PM	59.8	73.9	56.9
05:00 PM - 06:00 PM	60.5	78.0	57.1
06:00 PM - 07:00 PM	59.7	78.5	56.9
07:00 PM - 08:00 PM	60.3	87.3	57.0
08:00 PM - 09:00 PM	59.1	80.1	54.8
09:00 PM - 10:00 PM	56.7	74.8	47.7
10:00 PM - 11:00 PM	53.2	75.9	43.5
11:00 PM - 12:00 AM	52.6	82.3	42.4
12:00 AM - 01:00 AM	51.7	76.1	42.0
01:00 AM - 02:00 AM	50.8	71.1	41.4
02:00 AM - 03:00 AM	51.6	77.2	41.2
03:00 AM - 04:00 AM	50.0	71.5	40.4
04:00 AM - 05:00 AM	51.3	69.4	41.6
05:00 AM - 06:00 AM	54.7	76.7	45.5
06:00 AM - 07:00 AM	60.3	78.8	53.1
07:00 AM - 08:00 AM	61.8	77.0	57.2
08:00 AM - 09:00 AM	59.2	75.7	55.7
09:00 AM - 10:00 AM	59.3	79.5	55.6
10:00 AM - 11:00 AM	59.7	75.1	56.6
11:00 AM - 12:00 PM	59.1	75.7	55.9
12:00 PM - 01:00 PM	58.3	74.5	55.5

Leq Average 24 hrs. (dB(A)) 58.2
Lmax (dB(A)) 87.3
L90 (dB(A)) 55.5
Ldn (dB(A)) 61.9
Standard (dB(A)) 70 115

Reference Method : ISO 1996-1 : 2016

Standard : 1. ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ ฉบับที่ 15 (พ.ศ. 2540) เรื่องกำหนดมาตรฐานระดับเสียงโดยทั่วไป
2. ประกาศกระทรวงอุตสาหกรรม เรื่องกำหนดค่าระดับเสียงการรบกวน และระดับเสียงที่เกิดจากการประกอบกิจการโรงงาน พ.ศ. 2548

Remark : The laboratory has been accepted as an accredited laboratory complying with the ISO/IEC 17025.

Technical Management

Thanita K.

Thanita Kulsuriwong
Scientist (4)

Approved by

Supot S.

Supot Salamteh
Section Head



Analysis / Test Report

TESTING
No.0042

Client : THAI MMA Co., Ltd.
88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150
P/O : PMM-2025-336
Project Name : Environmental Monitoring
Project Location : CCS Site 7

Lot ID: 2610902
Date Received : Mar 10, 2026
Date Reported : Mar 14, 2026
Report Number: 3528039-1

Page 1 of 1

Sample Number 2610902-6
Parameter Noise (Leq 24 hrs.)
Location บ้านนาบยา (GPS 47P 0734556, 1408551)
Measurement Date Mar 04 - Mar 05, 2026
Measurement by Santi Chaichana
Sound Level meter Serial No. 233183

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
01:00 PM - 02:00 PM	58.3	79.6	55.3
02:00 PM - 03:00 PM	57.5	73.7	55.0
03:00 PM - 04:00 PM	58.5	80.2	55.1
04:00 PM - 05:00 PM	57.5	72.6	55.5
05:00 PM - 06:00 PM	58.3	71.2	56.1
06:00 PM - 07:00 PM	58.7	71.0	56.7
07:00 PM - 08:00 PM	59.0	73.4	56.7
08:00 PM - 09:00 PM	59.1	77.9	54.6
09:00 PM - 10:00 PM	56.3	75.2	46.8
10:00 PM - 11:00 PM	56.1	74.9	44.9
11:00 PM - 12:00 AM	53.4	73.1	42.4
12:00 AM - 01:00 AM	53.7	77.6	41.7
01:00 AM - 02:00 AM	51.9	77.4	40.7
02:00 AM - 03:00 AM	49.6	72.9	40.5
03:00 AM - 04:00 AM	49.0	69.5	40.1
04:00 AM - 05:00 AM	52.2	77.9	41.2
05:00 AM - 06:00 AM	56.0	78.8	43.9
06:00 AM - 07:00 AM	60.7	81.8	53.7
07:00 AM - 08:00 AM	59.8	78.0	54.6
08:00 AM - 09:00 AM	58.3	75.8	54.7
09:00 AM - 10:00 AM	58.3	71.5	54.7
10:00 AM - 11:00 AM	58.5	70.7	55.5
11:00 AM - 12:00 PM	59.5	84.6	55.6
12:00 PM - 01:00 PM	60.6	77.1	57.0

Leq Average 24 hrs. (dB(A)) 57.6
Lmax (dB(A)) 84.6
L90 (dB(A)) 54.6
Ldn (dB(A)) 62.2
Standard (dB(A)) 70 115

Reference Method : ISO 1996-1 : 2016

Standard : 1. ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ ฉบับที่ 15 (พ.ศ. 2540) เรื่องกำหนดมาตรฐานระดับเสียงโดยทั่วไป
2. ประกาศกระทรวงอุตสาหกรรม เรื่องกำหนดค่าระดับเสียงการรบกวน และระดับเสียงที่เกิดจากการประกอบกิจการโรงงาน พ.ศ. 2548

Remark : The laboratory has been accepted as an accredited laboratory complying with the ISO/IEC 17025.

Technical Management

Thanita K.

Thanita Kulsuriwong
Scientist (4)

Approved by

Supot S.

Supot Salamteh
Section Head

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER

คุณภาพอากาศภายในสถานประกอบการ



Analysis / Test Report

TESTING
No.0042

Client : THAI MMA Co., Ltd.
88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150
P/O : PMM-2025-336
Project Name : Environmental Monitoring
Project Location : CCS Site 7

Lot ID: 266126

Date Received : Feb 11, 2026
Date Reported : Feb 17, 2026
Report Number : 3491831-1

Page 1 of 5

Sample Number 266126-1
Sampled Date Feb 11, 2026
Sample Description Air Quality
Location ไส้ระเหยออกจากถังซีลน้ำ (Water Seal)
Date Analysis Commenced Feb 12, 2026
Condition of Sample Drawn into one 10-L air sampling bag

Analyte	Sampled Date/time	Unit	LOD	LOQ (LOR)	Result	Guideline Limit	Method	Guideline	Testing Location
Air Testing									
Total VOC *	09:56 AM - 11:56 AM	ppm	-	0.10	6.3	No Standard	Total VOC Analyzer	-	Bangkok

Guideline :

Sampled By : Tarin Octjinda

Remark :

- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)
- Analyte(s) marked * is/are not included in scope of Accreditation ISO/IEC 17025.

Approved by

Thanita K.

Thanita Kulsuriwong
Scientist (4)

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

TESTING
No.0042

Client : THAI MMA Co., Ltd.
88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150
P/O : PMM-2025-336
Project Name : Environmental Monitoring
Project Location : CCS Site 7

Lot ID: 266126

Date Received : Feb 11, 2026
Date Reported : Feb 17, 2026
Report Number : 3491831-1

Page 2 of 5

Sample Number 266126-2
Sampled Date Feb 11, 2026
Sample Description Air Quality
Location ไหระเหยที่ออกจากขั้นตอนการนำสารที่ได้จากการทำให้บริสุทธิ์ถ่ายลงถังขนาด 200 ลิตร
Date Analysis Commenced Feb 12, 2026
Condition of Sample Drawn into one 10-L air sampling bag

Analyte	Sampled Date/time	Unit	LOD	LOQ (LOR)	Result	Guideline Limit	Method	Guideline	Testing Location
Air Testing									
Total VOC *	09:50 AM - 11:50 AM	ppm	-	0.10	19.4	No Standard	Total VOC Analyzer	-	Bangkok

Guideline :

Sampled By : Tarin Octjinda

Remark :

- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)
- Analyte(s) marked * is/are not included in scope of Accreditation ISO/IEC 17025.

Approved by

Thanita K.

Thanita Kulsuriwong
Scientist (4)

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

TESTING
No.0042

Client : THAI MMA Co., Ltd.
88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150
P/O : PMM-2025-336
Project Name : Environmental Monitoring
Project Location : CCS Site 7

Lot ID: 266126

Date Received : Feb 11, 2026
Date Reported : Feb 17, 2026
Report Number : 3491831-1

Page 3 of 5

Sample Number 266126-3
Sampled Date Feb 11, 2026
Sample Description Air Quality
Location ไหระเหยจากการถ่ายของเสียที่ไม่สามารถนำกลับมาใช้ได้เกิดจากกระบวนการลงสู่ถังขนาด 200 ลิตร
Date Analysis Commenced Feb 12, 2026
Condition of Sample Drawn into one 10-L air sampling bag

Analyte	Sampled Date/time	Unit	LOD	LOQ (LOR)	Result	Guideline Limit	Method	Guideline	Testing Location
Air Testing									
Total VOC *	09:56 AM - 11:56 AM	ppm	-	0.10	12.2	No Standard	Total VOC Analyzer	-	Bangkok

Guideline :

Sampled By : Tarin Octjinda

Remark :

- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)
- Analyte(s) marked * is/are not included in scope of Accreditation ISO/IEC 17025.

Approved by

Thanita K.

Thanita Kulsuriwong
Scientist (4)

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

TESTING
No.0042

Client : THAI MMA Co., Ltd.
88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150
P/O : PMM-2025-336
Project Name : Environmental Monitoring
Project Location : CCS Site 7

Lot ID: 266126

Date Received : Feb 11, 2026
Date Reported : Feb 17, 2026
Report Number : 3491831-1

Page 4 of 5

Sample Number 266126-4
Sampled Date Feb 11, 2026
Sample Description Air Quality
Location โรงระเหยขาดอากาศ Carbon Absorber
Date Analysis Commenced Feb 12, 2026
Condition of Sample Drawn into one 10-L air sampling bag

Analyte	Sampled Date/time	Unit	LOD	LOQ (LOR)	Result	Guideline Limit	Method	Guideline	Testing Location
Air Testing									
Total VOC *	09:54 AM - 11:54 AM	ppm	-	0.10	7.8	No Standard	Total VOC Analyzer	-	Bangkok

Guideline :

Sampled By : Tarin Octjinda

Remark :

- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)
- Analyte(s) marked * is/are not included in scope of Accreditation ISO/IEC 17025.

Approved by

Thanita K.

Thanita Kulsuriwong
Scientist (4)

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

TESTING
No.0042

Client : THAI MMA Co., Ltd.
88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150
P/O : PMM-2025-336
Project Name : Environmental Monitoring
Project Location : CCS Site 7

Lot ID: 266126

Date Received : Feb 11, 2026
Date Reported : Feb 17, 2026
Report Number : 3491831-1

Page 5 of 5

Sample Number 266126-5
Sampled Date Feb 11, 2026
Sample Description Air Quality
Location Cutter Zone
Date Analysis Commenced Feb 12, 2026
Condition of Sample Drawn into one filter paper placed in plastic cassette
Barometric Pressure 755 mmHg
Atmospheric Temperature 26.7 °C

Analyte	Sampled Date/time	Unit	LOD	LOQ (LOR)	Result	Guideline Limit	Method	Guideline	Testing Location
Air Testing									
Total Dust	09:40 AM - 11:40 AM	mg/m3	-	0.15	<0.15	15	In-house method : STM 02-022 based on NIOSH Manual of Analytical Method, 4th ed., NMAM, method 0500 Issue 2, 1994 (Include sampling)	OSHA	Rayong

Guideline :

OSHA : Occupational Safety and Health Administration

Sampled By : Tarin Octjinda

Remark :

- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)
- Analyte(s) marked * is/are not included in scope of Accreditation ISO/IEC 17025.

Approved by

Thanita K.

Thanita Kulsuriwong
Scientist (4)

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

TESTING
No.0042

Client : THAI MMA Co., Ltd.
88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150
P/O : PMM-2025-336
Project Name : Environmental Monitoring
Project Location : CCS Site 7

Lot ID: 2633644

Date Received : May 18, 2026
Date Reported : May 27, 2026
Report Number : 3573588-1

Page 1 of 5

Sample Number 2633644-1
Sampled Date May 18, 2026
Sample Description Air Quality
Location ไล้ระเหยออกจากถังซีลน้ำ (Water Seal)
Date Analysis Commenced May 19, 2026
Condition of Sample Drawn into one 10-L air sampling bag

Analyte	Sampled Date/time	Unit	LOD	LOQ (LOR)	Result	Guideline Limit	Method	Guideline	Testing Location
Air Testing									
Total VOC *	09:00 AM - 11:00 AM	ppm	-	0.1	4.1	No Standard	Total VOC Analyzer	-	Rayong

Guideline :

Sampled By : Natchapon Thamklang

Remark :

- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)
- Analyte(s) marked * is/are not included in scope of Accreditation ISO/IEC 17025.

Approved by

Thanita K.

Thanita Kulsuriwong
Scientist (4)

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

TESTING
No.0042

Client : THAI MMA Co., Ltd.
88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150
P/O : PMM-2025-336
Project Name : Environmental Monitoring
Project Location : CCS Site 7

Lot ID: 2633644

Date Received : May 18, 2026
Date Reported : May 27, 2026
Report Number : 3573588-1

Page 2 of 5

Sample Number 2633644-2
Sampled Date May 18, 2026
Sample Description Air Quality
Location ไหระเหยที่ออกจากขั้นตอนการนำสารที่ได้จากการทำให้บริสุทธิ์ถ่ายลงถังขนาด 200 ลิตร
Date Analysis Commenced May 19, 2026
Condition of Sample Drawn into one 10-L air sampling bag

Analyte	Sampled Date/time	Unit	LOD	LOQ (LOR)	Result	Guideline Limit	Method	Guideline	Testing Location
Air Testing									
Total VOC *	09:00 AM - 11:00 AM	ppm	-	0.1	15.5	No Standard	Total VOC Analyzer	-	Rayong

Guideline :

Sampled By : Natchapon Thamklang

Remark :

- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)
- Analyte(s) marked * is/are not included in scope of Accreditation ISO/IEC 17025.

Approved by

Thanita K.

Thanita Kulsuriwong
Scientist (4)

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

TESTING
No.0042

Client : THAI MMA Co., Ltd.
88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150
P/O : PMM-2025-336
Project Name : Environmental Monitoring
Project Location : CCS Site 7

Lot ID: 2633644

Date Received : May 18, 2026
Date Reported : May 27, 2026
Report Number : 3573588-1

Page 3 of 5

Sample Number 2633644-3
Sampled Date May 18, 2026
Sample Description Air Quality
Location ไหระเหยจากการถ่ายของเสียที่ไม่สามารถนำกลับมาใช้ได้เกิดจากกระบวนการลงสู่ถังขนาด 200 ลิตร
Date Analysis Commenced May 19, 2026
Condition of Sample Drawn into one 10-L air sampling bag

Analyte	Sampled Date/time	Unit	LOD	LOQ (LOR)	Result	Guideline Limit	Method	Guideline	Testing Location
Air Testing									
Total VOC *	09:00 AM - 11:00 AM	ppm	-	0.1	10.2	No Standard	Total VOC Analyzer	-	Rayong

Guideline :

Sampled By : Natchapon Thamklang

Remark :

- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)
- Analyte(s) marked * is/are not included in scope of Accreditation ISO/IEC 17025.

Approved by

Thanita K.

Thanita Kulsuriwong
Scientist (4)

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

TESTING
No.0042

Client : THAI MMA Co., Ltd.
88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150
P/O : PMM-2025-336
Project Name : Environmental Monitoring
Project Location : CCS Site 7

Lot ID: 2633644

Date Received : May 18, 2026
Date Reported : May 27, 2026
Report Number : 3573588-1

Page 4 of 5

Sample Number 2633644-4
Sampled Date May 18, 2026
Sample Description Air Quality
Location โรงระเหยขาดกลาก Carbon Absorber
Date Analysis Commenced May 19, 2026
Condition of Sample Drawn into one 10-L air sampling bag

Analyte	Sampled Date/time	Unit	LOD	LOQ (LOR)	Result	Guideline Limit	Method	Guideline	Testing Location
Air Testing									
Total VOC *	09:00 AM - 11:00 AM	ppm	-	0.1	8.8	No Standard	Total VOC Analyzer	-	Rayong

Guideline :

Sampled By : Natchapon Thamklang

Remark :

- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)
- Analyte(s) marked * is/are not included in scope of Accreditation ISO/IEC 17025.

Approved by

Thanita K.

Thanita Kulsuriwong
Scientist (4)

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

TESTING
No.0042

Client : THAI MMA Co., Ltd.
88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150
P/O : PMM-2025-336
Project Name : Environmental Monitoring
Project Location : CCS Site 7

Lot ID: 2633644

Date Received : May 18, 2026
Date Reported : May 27, 2026
Report Number : 3573588-1

Page 5 of 5

Sample Number : 2633644-5
Sampled Date : May 18, 2026
Sample Description : Air Quality
Location : Cutter Zone
Date Analysis Commenced : May 23, 2026
Condition of Sample : Drawn into one filter paper placed in plastic cassette
Barometric Pressure : 751 mmHg
Atmospheric Temperature : 30.8 °C

Analyte	Sampled Date/time	Unit	LOD	LOQ (LOR)	Result	Guideline Limit	Method	Guideline	Testing Location
Air Testing									
Total Dust	09:30 AM - 11:30 AM	mg/m3	-	0.15	<0.15	15	In-house method : STM 02-022 based on NIOSH Manual of Analytical Method, 4th ed., NMAM, method 0500 Issue 2, 1994 (Include sampling)	OSHA	Rayong

Guideline :

OSHA : Occupational Safety and Health Administration

Sampled By : Natchapon Thamklang

Remark :

- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)
- Analyte(s) marked * is/are not included in scope of Accreditation ISO/IEC 17025.

Approved by

Thanita K.

Thanita Kulsuriwong
Scientist (4)

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER

ระดับเสียงภายในสถานประกอบการ



Analysis / Test Report

Client : THAI MMA Co., Ltd.
88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150
P/O : PMM-2025-336
Project Name : Environmental Monitoring
Project Location : CCS Site 7

Lot ID: 2633646

Date Received : May 18, 2026
Date Reported : May 22, 2026
Report Number: 3578056-1

Page 1 of 1

Sample Number 2633646-1
Parameter Noise (Leq 8 hrs.)
Location บริเวณ Process 300
Measurement Date May 18, 2026
Measurement by Natchapon Thamklang

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
09:11 AM - 10:11 AM	80.4	82.8	80.0
10:11 AM - 11:11 AM	80.4	84.3	80.0
11:11 AM - 12:11 PM	80.2	87.6	79.8
12:11 PM - 01:11 PM	80.1	86.9	79.7
01:11 PM - 02:11 PM	79.6	88.1	79.2
02:11 PM - 03:11 PM	79.8	87.6	79.2
03:11 PM - 04:11 PM	79.6	85.0	79.1
04:11 PM - 05:11 PM	79.7	86.5	79.3

Leq Average 8 hrs. (dB(A))

80.0

Lmax (dB(A))

88.1

Standard (dB(A))

90

140

Reference Method : ISO 1996-1 : 2016

Standard : ประกาศกระทรวงอุตสาหกรรม เรื่อง มาตรการคุ้มครองความปลอดภัย
ในการประกอบกิจการโรงงานเกี่ยวกับสภาวะแวดล้อมในการทำงาน พ.ศ. ๒๕๔๖

Technical Management

Chontichak

Chonticha Subongkoch
Scientist (3)

Approved by

Supot S

Supot Salamteh
Section Head

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER



Analysis / Test Report

Client : THAI MMA Co., Ltd.
88/6, 3191 Road, T. Map Ta Phut, A. Muang, Rayong Thailand 21150
P/O : PMM-2025-336
Project Name : Environmental Monitoring
Project Location : CCS Site 7

Lot ID: 2633646

Date Received : May 18, 2026
Date Reported : May 22, 2026
Report Number: 3578057-1

Page 1 of 1

Sample Number 2633646-2
Parameter Noise (Leq 8 hrs.)
Location บริเวณ Packing
Measurement Date May 18, 2026
Measurement by Natchapon Thamklang

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
09:17 AM - 10:17 AM	72.8	86.2	69.6
10:17 AM - 11:17 AM	72.2	93.8	68.8
11:17 AM - 12:17 PM	72.9	90.1	69.4
12:17 PM - 01:17 PM	72.7	89.8	69.2
01:17 PM - 02:17 PM	72.4	88.5	69.5
02:17 PM - 03:17 PM	73.0	85.7	69.5
03:17 PM - 04:17 PM	72.1	86.7	68.8
04:17 PM - 05:17 PM	72.3	85.0	68.8

Leq Average 8 hrs. (dB(A)) 72.6
Lmax (dB(A)) 93.8
Standard (dB(A)) 90
Reference Method : ISO 1996-1 : 2016
Standard : ประกาศกระทรวงอุตสาหกรรม เรื่อง มาตรการคุ้มครองความปลอดภัย
ในการประกอบกิจการโรงงานเกี่ยวกับสภาวะแวดล้อมในการทำงาน พ.ศ. ๒๕๔๖

Technical Management

Chontichak

Chonticha Subongkoch
Scientist (3)

Approved by

Supot S

Supot Salamteh
Section Head

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences

www.alsglobal.com

RIGHT SOLUTIONS RIGHT PARTNER

ภาคผนวก ง

ใบรับรองการสอบเทียบเครื่องมือ



right solutions.
right partner.

รายการเครื่องมือที่ใช้ในการวิเคราะห์ / ทดสอบ


Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Ambient	Particulate Matter (PM-10)	High Volume	RYG_FS0188	-	-	On site Calibration
Ambient	Particulate Matter (PM-10)	High Volume	NKH_FS0045	-	-	On site Calibration
Ambient	Particulate Matter (PM-10)	High Volume	NKH_FS0047	-	-	On site Calibration
Ambient	Particulate Matter (PM-10)	Digital Balance	RYG_EN0001	3-Feb-26	3-Feb-27	12
Ambient	Total Suspended Particulate	High Volume	RYG_FS0178	-	-	On site Calibration
Ambient	Total Suspended Particulate	High Volume	NKH_FS0052	-	-	On site Calibration
Ambient	Total Suspended Particulate	High Volume	NKH_FS0051	-	-	On site Calibration
Ambient	Total Suspended Particulate	Digital Balance	RYG_EN0001	3-Feb-26	3-Feb-27	12
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	RYG_FS0728	18-Feb-26	17-Aug-27	18
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	RYG_FS0611	6-Jan-26	5-Jul-27	18
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	RYG_FS0608	21-Jan-26	20-Jul-27	18
Stack	Total Suspended Particulate	Console Control Unit	BKK_FS0556	6-Jan-26	6-Jul-26	6
Stack	Total Suspended Particulate	Pitot Tube	BKK_FS0560	6-Jan-26	6-Jul-26	6
Stack	Total Suspended Particulate	Fuel Gas Analyzer	RYG_FS0464	24-Mar-25	23-Mar-26	12
Stack	Total Suspended Particulate	Digital Balance	RYG_EN0003	3-Feb-26	3-Feb-27	12
Stack	Butyl Acrylate	Pitot Tube	BKK_FS0561	6-Jan-26	6-Jul-26	6
Stack	Butyl Acrylate	Fuel Gas Analyzer	RYG_FS0464	24-Mar-25	23-Mar-26	12
Stack	Butyl Acrylate	DRYCAL FLOWMETER	BKK_FS0614	10-Sep-25	9-Sep-26	12
Stack	Butyl Acrylate	DRYCAL FLOWMETER	BKK_FS0619	10-Sep-25	9-Sep-26	12
Stack	Butyl Acrylate	Air Sampling Pump	RYG_FS0131	4-Jan-26	4-Apr-26	3
Stack	Butyl Acrylate	Air Sampling Pump	RYG_FS0107	6-Jan-26	6-Apr-26	3
Stack	Butyl Acrylate	GC-MSD	BKK_EN0410	9-May-25	9-May-26	12
Stack	Methyl Methacrylate	Pitot Tube	BKK_FS0561	6-Jan-26	6-Jul-26	6
Stack	Methyl Methacrylate	Fuel Gas Analyzer	RYG_FS0464	24-Mar-25	23-Mar-26	12
Stack	Methyl Methacrylate	DRYCAL FLOWMETER	BKK_FS0614	10-Sep-25	9-Sep-26	12
Stack	Methyl Methacrylate	DRYCAL FLOWMETER	BKK_FS0619	10-Sep-25	9-Sep-26	12
Stack	Methyl Methacrylate	Air Sampling Pump	RYG_FS0131	4-Jan-26	4-Apr-26	3
Stack	Methyl Methacrylate	Air Sampling Pump	RYG_FS0122	7-Jan-26	7-Apr-26	3
Stack	Methyl Methacrylate	GC-MSD	BKK_EN0410	9-May-25	9-May-26	12
Stack	Total VOCs as Propane	Pitot Tube	BKK_FS0561	6-Jan-26	6-Jul-26	6
Stack	Total VOCs as Propane	Fuel Gas Analyzer	RYG_FS0464	24-Mar-25	23-Mar-26	12
Stack	Total VOCs as Propane	DRYCAL FLOWMETER	BKK_FS0614	10-Sep-25	9-Sep-26	12
Stack	Total VOCs as Propane	DRYCAL FLOWMETER	BKK_FS0619	10-Sep-25	9-Sep-26	12
Stack	Total VOCs as Propane	Air Sampling Pump	RYG_FS0131	4-Jan-26	4-Apr-26	3
Stack	Total VOCs as Propane	Air Sampling Pump	RYG_FS0122	7-Jan-26	7-Apr-26	3
Stack	Total VOCs as Propane	FID Analyzer	BKK_FS0758	5-Jan-26	5-Jul-26	6
Noise	Leq 24 hrs	Sound Calibrator	RYG_FS0496	19-Mar-25	19-Mar-26	12
Noise	Leq 24 hrs	Sound Level Meter	RYG_FS0024	28-Jan-26	27-Jan-27	12
Noise	Leq 24 hrs	Sound Level Meter	RYG_FS0027	21-Jan-26	20-Jan-27	12
Noise	Leq 8 hrs	Sound Calibrator	RYG_FS0213	9-Jan-26	8-Jan-27	12
Noise	Leq 8 hrs	Sound Level Meter	RYG_FS0023	6-Apr-26	5-Apr-27	12
Noise	Leq 8 hrs	Sound Level Meter	RYG_FS0628	21-Jan-26	20-Jan-27	12
Workplace	Total VOC	DRYCAL FLOWMETER	BKK_FS0614	10-Sep-25	9-Sep-26	12
Workplace	Total VOC	DRYCAL FLOWMETER	BKK_FS0619	10-Sep-25	9-Sep-26	12
Workplace	Total VOC	FID Analyzer	BKK_FS0758	12-Mar-26	11-Mar-27	12
Workplace	Total Dust	DRYCAL FLOWMETER	BKK_FS0614	10-Sep-25	9-Sep-26	12
Workplace	Total Dust	DRYCAL FLOWMETER	BKK_FS0619	10-Sep-25	9-Sep-26	12
Workplace	Total Dust	Digital Balance	RYG_EN0004	3-Feb-26	3-Feb-27	12
Rayong Lab	BOD	DO meter with Sensor	RYG_EN0032	20-Jan-25	20-Jul-26	18
Rayong Lab	BOD	Incubator	RYG_EN0154	18-Mar-26	18-Sep-27	18
Rayong Lab	BOD	Burette	RYG_EN0216	18-Sep-25	18-Sep-26	12
Rayong Lab	COD	Spectrophotometer	RYG_EN0037	18-Mar-25	18-Sep-26	18
Rayong Lab	Oil & Grease	Electronic Balance	RYG_EN0003	3-Feb-26	3-Feb-27	12
Rayong Lab	Oil & Grease	Liquid Bath (Water)	RYG_EN0220	27-Nov-25	27-Nov-26	12
Rayong Lab	pH at 25 °C	pH meter	RYG_EN0183	18-Jul-25	18-Jan-27	18
Rayong Lab	Total Suspended Solids	Electronic Balance	RYG_EN0163	3-Feb-26	3-Feb-27	12
Rayong Lab	Total Suspended Solids	Chamber (Oven)	RYG_EN0012	10-Sep-25	10-Mar-27	18
Rayong Lab	Total Dissolved Solids 180°C	Electronic Balance	RYG_EN0163	3-Feb-26	3-Feb-27	12
Rayong Lab	Total Dissolved Solids 180°C	Chamber (Oven)	RYG_EN0012	10-Sep-25	10-Mar-27	18
Rayong Lab	Temperature	Digital Thermometer With Sensor	RYG_FS0466	9-Oct-25	9-Oct-26	12



High Volume Air Sampler Calibration Worksheet

Project Site :	Thai MMA Co.,Ltd	Barometric Pressure (mm Hg) :	755.3
Calibrate Location :	บ้านบน	Temperature (°C) :	32.1
Calibrate Date :	2-Mar-26	High Volume ID :	RYG_FS0188
CalibrationSheet No.:	C-020326-RYG_FS0188	High Volume Model :	TE-5009X
Calibrator ID:	RYG_FS0205	High Volume S/N :	4796
Calibrator Model :	TE-5028A	Calibrator Slope :	0.95091
Calibrator S/N :	1166	Calibrator Intercept :	-0.01856

Test No.	Delta H ₂ O (inch)	Qa (m ³ /min)	I : Chart (CFM)	Linear Regression
1	1.6	0.864	30	Slope : 37.2614 Intercept : -2.1069 Correlation Coefficient : 0.9985
2	2.2	1.010	36	
3	2.8	1.137	40	
4	3.4	1.251	44	
5	4.2	1.388	50	

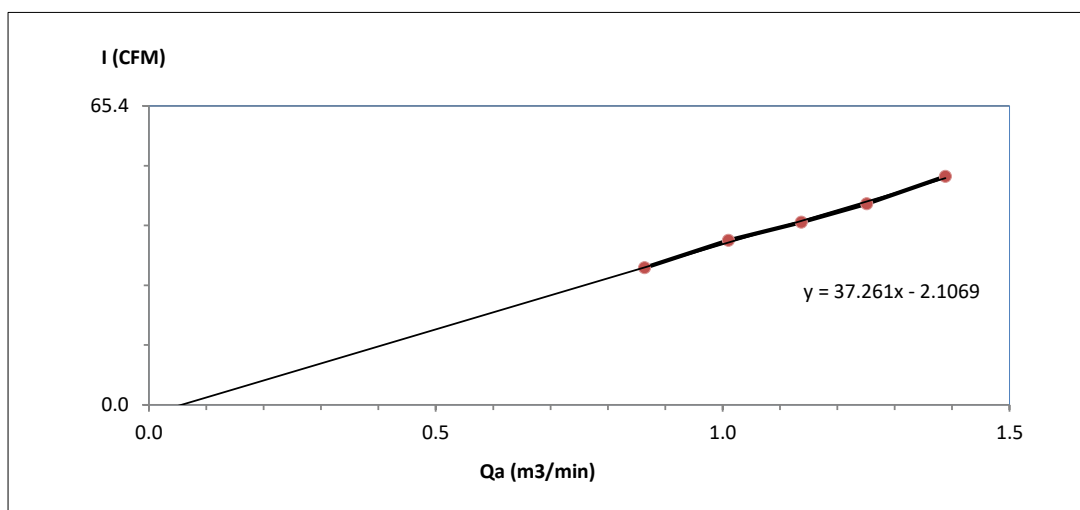

Calibrated by

(Mr. Santi Chaichana)
RYG Field Services Scientist (2)

Approved by :


(Mr. Supot Salamteh)
Field Services Section Head



High Volume Air Sampler Calibration Worksheet

Project Site :	Thai MMA Co.,Ltd	Barometric Pressure (mm Hg) :	755.3
Calibrate Location :	บ้านนาบข	Temperature (°C) :	32.1
Calibrate Date :	2-Mar-26	High Volume ID :	NKH_FS0045
CalibrationSheet No.:	C-020326-NKH_FS0045	High Volume Model :	TE-5009X
Calibrator ID:	RYG_FS0205	High Volume S/N :	5846
Calibrator Model :	TE-5028A	Calibrator Slope :	0.95091
Calibrator S/N :	1166	Calibrator Intercept :	-0.01856

Test No.	Delta H ₂ O (inch)	Qa (m ³ /min)	I : Chart (CFM)	Linear Regression
1	1.7	0.890	30	Slope : 41.2283 Intercept : -7.0324 Correlation Coefficient : 0.9982
2	2.4	1.054	36	
3	2.8	1.137	40	
4	3.4	1.251	44	
5	4.1	1.372	50	

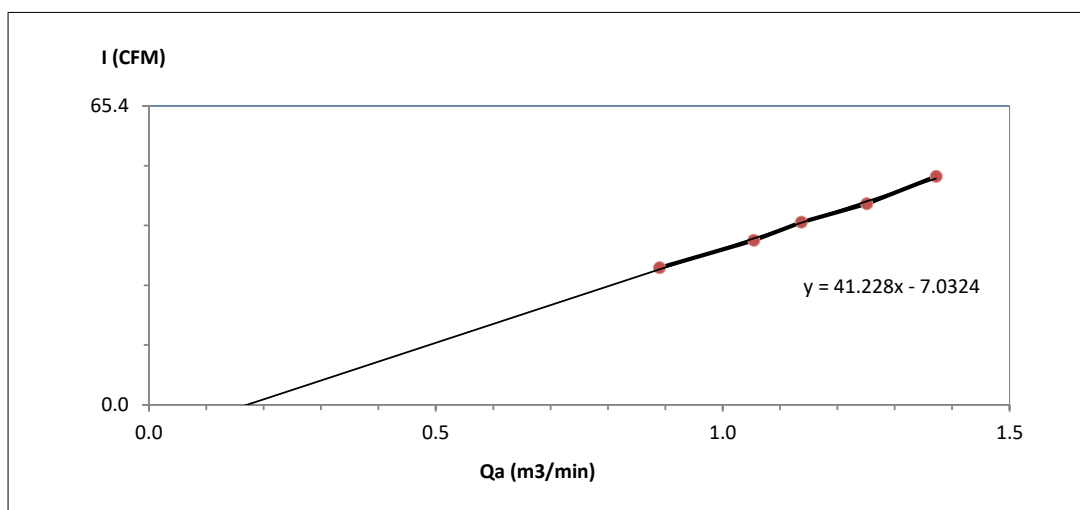

Calibrated by

(Mr. Santi Chaichana)
RYG Field Services Scientist (2)

Approved by :


(Mr. Supot Salamteh)
Field Services Section Head



High Volume Air Sampler Calibration Worksheet

Project Site :	Thai MMA Co.,Ltd	Barometric Pressure (mm Hg) :	755.3
Calibrate Location :	บ้านเนินพยอม	Temperature (°C) :	32.1
Calibrate Date :	2-Mar-26	High Volume ID :	NKH_FS0047
CalibrationSheet No.:	C-020326-NKH_FS0047	High Volume Model :	TE-5009X
Calibrator ID:	RYG_FS0205	High Volume S/N :	5848
Calibrator Model :	TE-5028A	Calibrator Slope :	0.95091
Calibrator S/N :	1166	Calibrator Intercept :	-0.01856

Test No.	Delta H ₂ O (inch)	Qa (m ³ /min)	I : Chart (CFM)	Linear Regression
1	1.7	0.890	30	Slope : 33.0720 Intercept : 0.8122 Correlation Coefficient : 0.9988
2	2.4	1.054	36	
3	3.0	1.176	40	
4	3.8	1.321	44	
5	4.8	1.483	50	

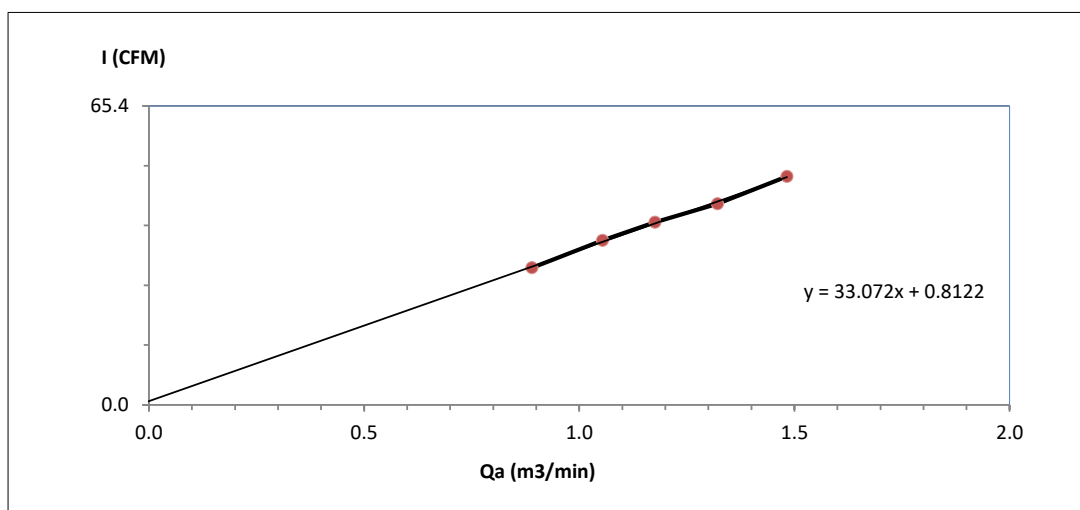

Calibrated by

(Mr. Santi Chaichana)
RYG Field Services Scientist (2)

Approved by :

(Mr. Supot Salamteh)
Field Services Section Head

Accredited by

NSC-TISI-TIS 17025

Calibration 0426



Calibration certificate

Calibration Certificate No. 26BCI0067

Object	Electronic non-automatic weighing instrument	This calibration certificate documents the traceability to national standards.
Manufacturer	Sartorius	Uncertainties of measurements are taken into account when only statements of compliance are made.
Type	LA130S-F	This certificate was prepared by Sartorius Corporation in accordance to the current ISO/IEC 17025:2017 standard and Sartorius Work Instruction (Method) SOP WI 08.
Serial QM Ident. no.	25409664 RYG_EN0001	This certificate relate and apply this equipment only.
Customer	ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)	
	616/10 Moo 5 T.Maenamkoo, A.Pluak Daeng, Rayong 21140, Thailand.	
Order no.	278579	REVIEW BY <i>Thanita K.</i>
Number of pages	4	APPROVED BY <i>D. Khunon</i>
Date of calibration	03 Feb 2026	NEXT CAL DATE 03/02/27

This calibration certificate may not be reproduced other than in full except with the permission of NSC-TISI-TIS-17025 and the issuing laboratory. Calibration certificates without signature are not valid.

The user is obliged to have the object recalibrated at appropriate intervals.

Date of issue	03 Feb 2026	Approval of the Calibration Certificate	Person in charge
			
		Mr. Chonchai Inthana	Chonchai Inthana

Calibration object

Single range instrument

Model	LA130S-F
Serial Number	25409664
QM Ident. no Inventory no.	RYG_EN0001 ---

Maximum capacity (Max. load)	150.0000 g
Measured up to	150.0000 g
Scale interval	0.0001 g

Place of calibration

Address	According to page 1
Department Cost center	Laboratory Department. ---
Building Floor	--- 1st Floor.
Room	Balance Room.
Maximum temperature variation at place of calibration	5 K

Calibration procedure

EURAMET Calibration Guide No. 18, Version 4.0 (11/2015) - Guidelines on the Calibration of Non-Automatic Weighing Instruments

Test equipment

Test equipment type	Test equipment ID	Valid until
Thermometer	Testo 174H H/T250743 (Traceable to Si unit through ENTECH)	18 Nov 2026
Test weight set OIML R111 E2	Certificate No.M2508149S ,E2(Traceable to SI unit through TCS)	19 Aug 2027

Adjustment Status

The measuring device was internally adjusted before the calibration.

Environmental and measuring conditions

Date of calibration	03 Feb 2026
Temperature at place of calibration Temp. diff. $T_{\text{weights}} - T_{\text{place}}$	24.5 °C 0.5 K
Measuring conditions	The installation site is suitable. The device is level. Balance was loaded up to Max before test.
Comments	Humidity 52.0 %RH.

Measurement results | Measurement uncertainties

Repeatability

Test load (nominal): 10 g 100 g		
	10 g	100 g
1	10.0000 g	100.0000 g
2	10.0000 g	99.9998 g
3	9.9999 g	100.0000 g
4	10.0001 g	100.0000 g
5	10.0000 g	99.9999 g
6	9.9999 g	100.0000 g
7	9.9999 g	99.9999 g
8	9.9999 g	100.0000 g
9	9.9999 g	100.0000 g
10	9.9999 g	99.9999 g
	$s = 0.00007 \text{ g}$	$s = 0.00007 \text{ g}$

Eccentricity

Test load (nominal): 50 g	
Center	50.0000 g
Front left	50.0001 g
Back left	50.0001 g
Back right	50.0000 g
Front right	50.0001 g
Maximum deviation from centric loading indication $ \Delta_{\text{ecc}} _{\text{max}} = 0.0001 \text{ g}$	

Error of indication

Testload	Indication	Error	Expansion factor	Uncertainty	Uncertainty relative
L	I	E	k	$U(E)$	$U_{\text{rel}}(E)$
0.0100 g	0.0100 g	0.0000 g	2.00	0.00016 g	1.6 %
0.0500 g	0.0500 g	0.0000 g	2.00	0.00016 g	0.33 %
0.1000 g	0.1000 g	0.0000 g	2.00	0.00016 g	0.16 %
0.5000 g	0.5000 g	0.0000 g	2.00	0.00016 g	0.033 %
1.0000 g	1.0000 g	0.0000 g	2.00	0.00016 g	0.016 %
2.0000 g	2.0000 g	0.0000 g	2.00	0.00017 g	0.0083 %
5.0000 g	5.0001 g	0.0001 g	2.00	0.00017 g	0.0033 %
10.0000 g	10.0001 g	0.0001 g	2.00	0.00017 g	0.0017 %
20.0000 g	20.0000 g	0.0000 g	2.00	0.00017 g	0.00086 %
100.0000 g	100.0001 g	0.0001 g	2.00	0.00023 g	0.00023 %
150.0000 g	150.0001 g	0.0001 g	2.00	0.00030 g	0.00020 %
Maximum error of indication		$ E _{\text{max}} = 0.0001 \text{ g}$			

$U_{\text{rel}}(E)$ is the quotient of $U(E)$ and test load L . The uncertainty of measurement $U(E)$ is valid only if error E is considered. You will find reference notes on the uncertainty of measurement in use under: Appendix to the calibration certificate | Interpretation of measurement results.
Reference note: The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the documented Expansion factor, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

End of calibration certificate

Uncertainty of measurement in use

Device adjusted before measurement	Yes
Temperature deviation considered	1.5 K (isoCAL active)
Temperature coefficient considered	$1 \cdot 10^{-6}/\text{K}$


Uncertainty of the weighing result $U_{gl}(W)$

$U_{gl}(W) = 0.00016 \text{ g} + 1.95 \cdot 10^{-5} \cdot R$

Reference note: The current uncertainty of measurement is calculated by entering of the reading R into this formula. In relation to this, there is no need for a correction of the indication error. The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied with an Expansion factor of 2, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

Indication in % from max load	Net indication R	Uncertainty $U_{gl}(W)$	Uncertainty relative $U_{gl}(W)_{rel}$
1 %	1.5000 g	0.00019 g	0.013 %
25 %	37.5000 g	0.00089 g	0.0024 %
50 %	75.0000 g	0.0016 g	0.0022 %
75 %	112.5000 g	0.0024 g	0.0021 %
100 %	150.0000 g	0.0031 g	0.0021 %

Graphic realization of the relative uncertainty of measurement | process accuracy

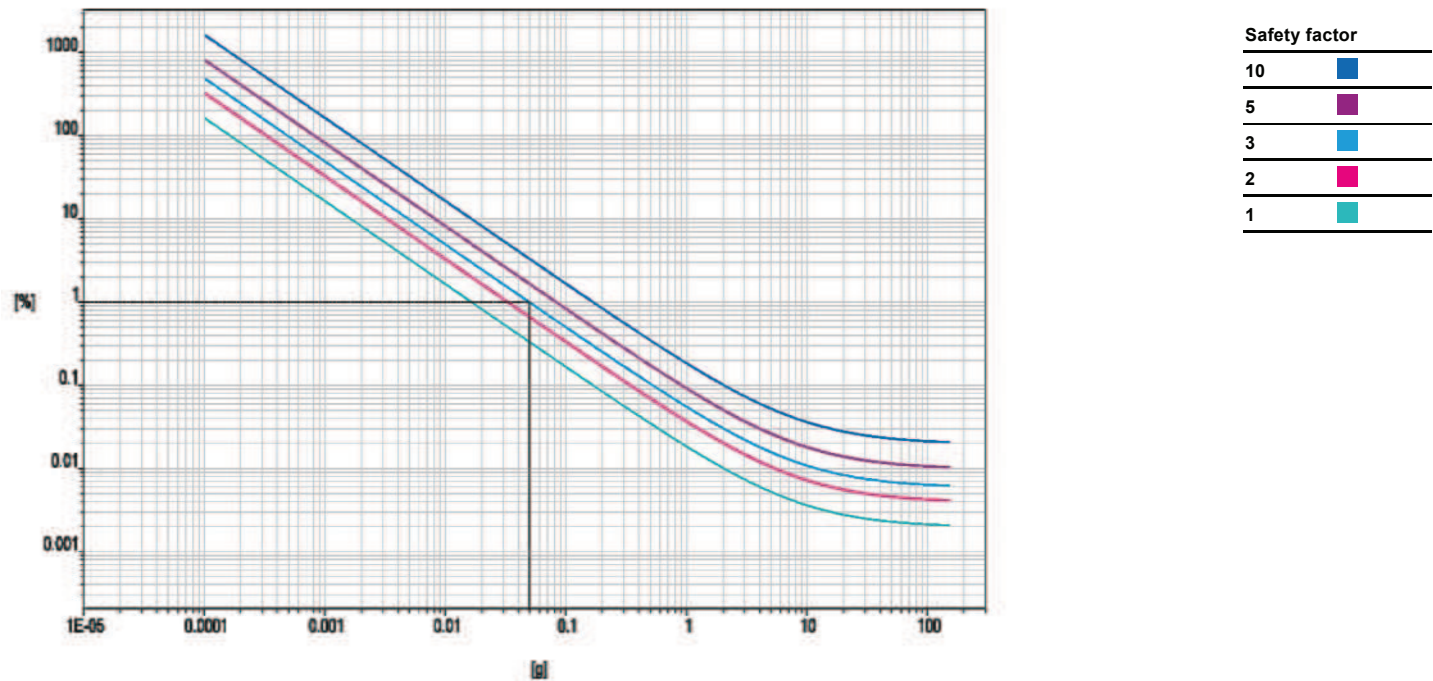

Displayed example


Process accuracy	1.00 %
Safety factor	3
Minimum sample weight	0.0493 g



High Volume Air Sampler Calibration Worksheet

Project Site :	Thai MMA Co.,Ltd	Barometric Pressure (mm Hg) :	755.3
Calibrate Location :	บ้านบน	Temperature (°C) :	32.1
Calibrate Date :	2-Mar-26	High Volume ID :	RYG_FS0178
CalibrationSheet No.:	C-020326-RYG_FS0178	High Volume Model :	TE-5170D
Calibrator ID:	RYG_FS0205	High Volume S/N :	4804
Calibrator Model :	TE-5028A	Calibrator Slope :	1.51825
Calibrator S/N :	1166	Calibrator Intercept :	-0.02964

Test No.	Delta H ₂ O (inch)	Q _{std} (m ³ /min)	I : Chart (CFM)	Linear Regression
1	2.6	1.0760	40	Slope : 31.6472 Intercept : 5.9340 Correlation Coefficient : 0.9989
2	3.6	1.2609	46	
3	4.4	1.3908	50	
4	5.4	1.5376	54	
5	6.6	1.6968	60	

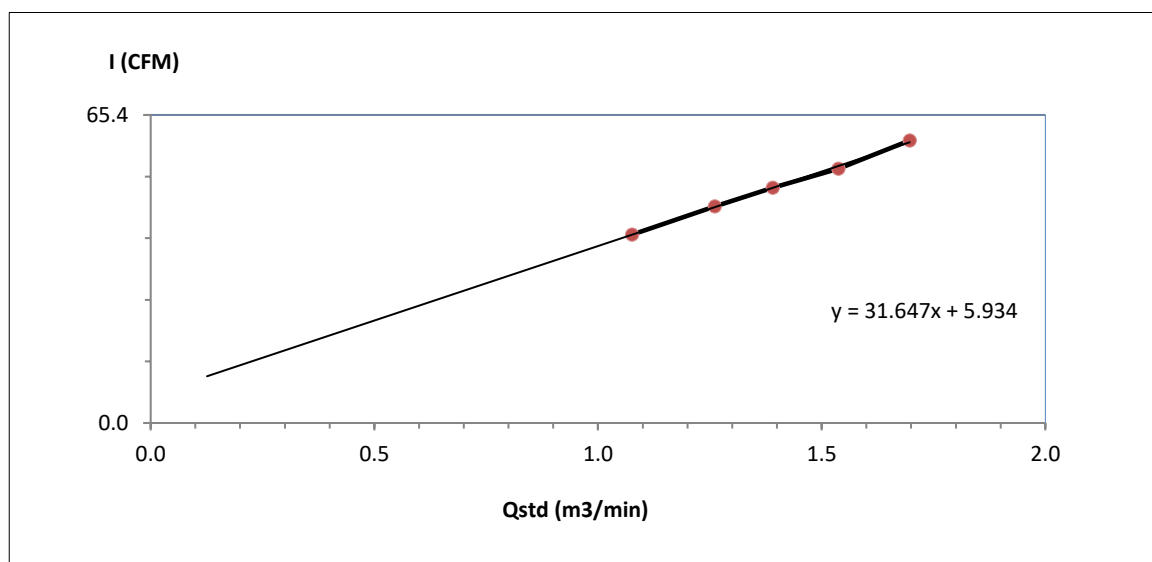

Calibrated by

(Mr. Santi Chaichana)
RYG Field Services Scientist (2)

Approved by :


(Mr. Supot Salamteh)
Field Services Section Head



High Volume Air Sampler Calibration Worksheet

Project Site :	Thai MMA Co.,Ltd	Barometric Pressure (mm Hg) :	755.3
Calibrate Location :	บ้านนาบชา	Temperature (°C) :	32.1
Calibrate Date :	2-Mar-26	High Volume ID :	NKH_FS0052
CalibrationSheet No.:	C-020326-NKH_FS0052	High Volume Model :	TE-5170D
Calibrator ID:	RYG_FS0205	High Volume S/N :	5855
Calibrator Model :	TE-5028A	Calibrator Slope :	1.51825
Calibrator S/N :	1166	Calibrator Intercept :	-0.02964

Test No.	Delta H ₂ O (inch)	Q _{std} (m ³ /min)	I : Chart (CFM)	Linear Regression
1	2.6	1.0760	40	Slope : 31.9238 Intercept : 5.7377 Correlation Coefficient : 0.9994
2	3.6	1.2609	46	
3	4.3	1.3753	50	
4	5.3	1.5236	54	
5	6.6	1.6968	60	

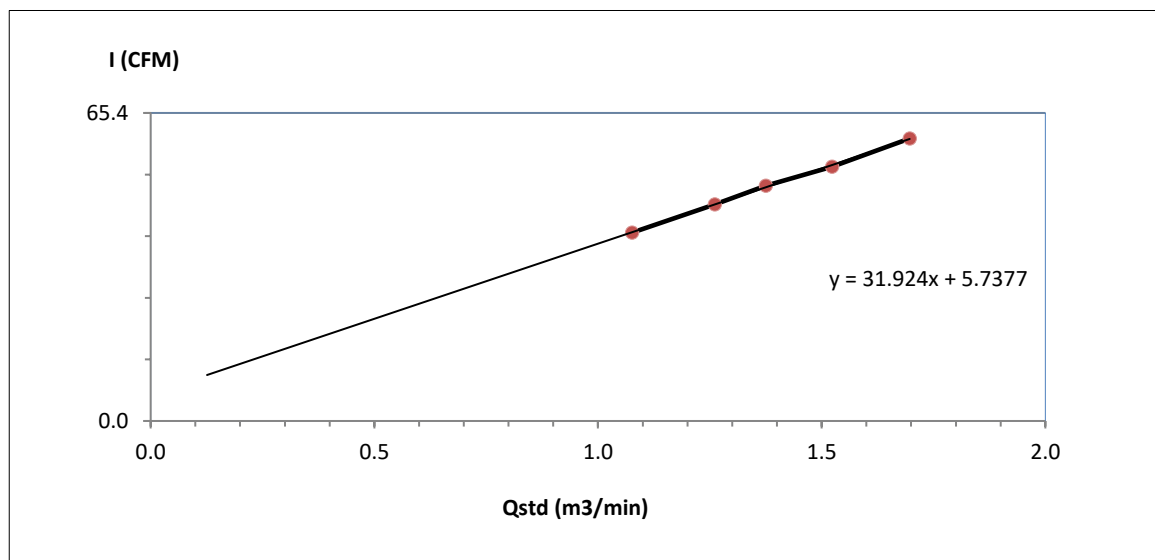

Calibrated by

(Mr. Santi Chaichana)
RYG Field Services Scientist (2)

Approved by :


(Mr. Supot Salamteh)
Field Services Section Head



High Volume Air Sampler Calibration Worksheet

Project Site :	Thai MMA Co.,Ltd	Barometric Pressure (mm Hg) :	755.3
Calibrate Location :	บ้านเนินพยอม	Temperature (°C) :	32.1
Calibrate Date :	2-Mar-26	High Volume ID :	NKH_FS0051
CalibrationSheet No.:	C-020326-NKH_FS0051	High Volume Model :	TE-5170D
Calibrator ID:	RYG_FS0205	High Volume S/N :	5854
Calibrator Model :	TE-5028A	Calibrator Slope :	1.51825
Calibrator S/N :	1166	Calibrator Intercept :	-0.02964

Test No.	Delta H ₂ O (inch)	Q _{std} (m ³ /min)	I : Chart (CFM)	Linear Regression
1	2.7	1.0959	40	Slope : 32.5119 Intercept : 4.5003 Correlation Coefficient : 0.9985
2	3.6	1.2609	46	
3	4.5	1.4062	50	
4	5.4	1.5376	54	
5	6.6	1.6968	60	

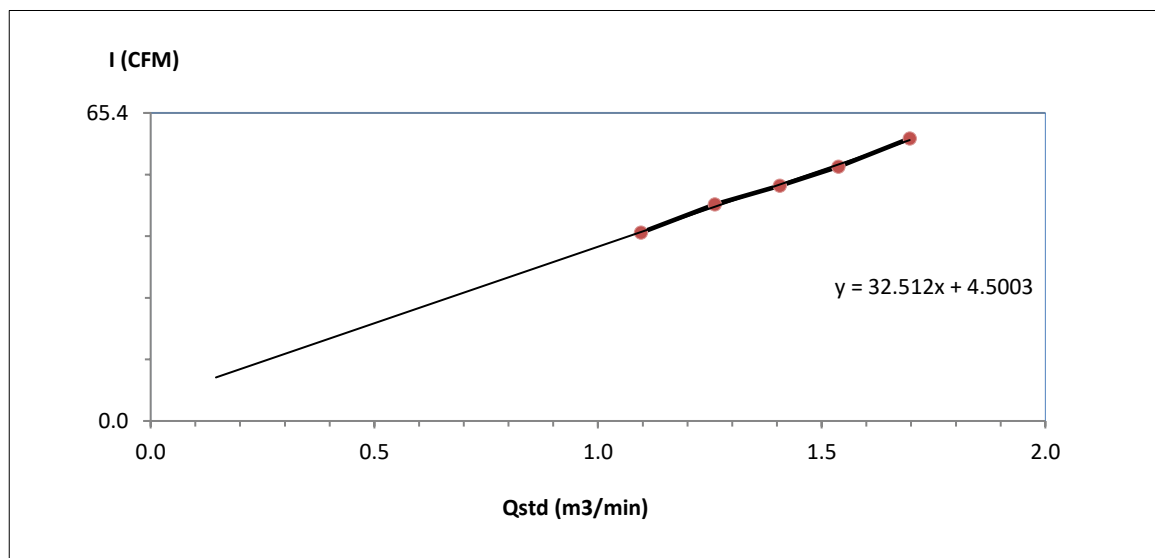

Calibrated by

(Mr. Santi Chaichana)
RYG Field Services Scientist (2)

Approved by :

(Mr. Supot Salamteh)
Field Services Section Head



JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Air speed measurement laboratory
Calibration services department.



Certificate Number

CWS-017-69

CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

MEASUREMENT ITEM : Cup anemometer
MANUFACTURER : Novalyx
MODEL/TYPE : Sensor: WS-02FA
Data logger: 110-WS-25DL-D
SERIAL NUMBER : Sensor: WSD-A5990
Data logger: A5990
ID NUMBER : RYG_FS0728
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd,
Khwaeng Suan Luang, Khet Suan Luang,
Bangkok 10250 Thailand.

RECEIVED DATE : 06 Feb 2026
MEASUREMENT DATE : 18 Feb 2026
ISSUE DATE : 18 Feb 2026

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa

PLACE OF CALIBRATION : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITIONS	: Wind tunnel cross-section area ¹	900	cm ²
	Cup anemometer frontal area ²	100	cm ²
	Diameter of mounting pipe ³	-	mm
	Blockage ratio of test object ⁴	0.111	[-]

Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are (23.3) °C, (57.1) %RH and (1014.5) hPa.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibrated by:

- ☒ Mr. Sorawit Thachalad
☐ Miss Jittraporn Lertsomphol



Approved signatory: _____

Mr. Parinya Booncharoen
Calibration Department Manager

Calibration procedure:

The Cup anemometer was calibrated against Standard air velocity transducer model: 8455-12 and pitot tube with precision differential pressure meter model: DPM2500 in an close test-section of Eiffel-type wind tunnel with 900 cm² cross test section area. The WI-CL-007 based on IEC 61400-12-1, Wind energy generation systems – Part 12-1: Power performance measurements of electricity producing wind turbines, March 2017 was used as a calibration guideline.

Traceability:

This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MW-0019-25 and MW-0059-25

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

REVIEW BY _____

APPROVED BY _____

NEXT CAL DATE: 17/ 08/ 2027

Remark:

- ¹ Nozzle cross-section area of the wind tunnel
² Projected cross-section area of the tested object include mounting pipe
³ Diameter of mounting pipe
⁴ Ratio ² to ¹

MEASUREMENT RESULTS⁵

The Cup anemometer, Unit Under Calibration (UUC) was exercise at 10 m/s for 5 minutes prior to calibration being performed. The standard air velocity 0.5 m/s to 5 m/s was calculated by a standard air velocity transducer which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section and the standard air velocity 5 m/s to 30 m/s was calculated by a pitot tube with precision differential pressure meter which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section, UUC was mounted on a round vertical tube of the lower plate at center of test section. The calibration was carried out under both rising and falling air velocity in the range of 1 m/s to 16 m/s at calibration interval of 1 m/s. The results of calibration and associated measurement uncertainties are reported in the table below.


V_{std} ⁶ (m/s)	Temp. wind tunnel (°C)	Temp. room (°C)	V_{UUC} ⁷ (m/s)	Error (m/s)	$U (k=2)$ (m/s)
1.004	23.22	23.30	0.9	-0.1	0.31
2.104	23.16	23.30	1.9	-0.2	0.31
3.018	23.12	23.30	2.8	-0.2	0.31
4.198	23.14	23.30	3.9	-0.3	0.31
5.01	23.00	23.30	4.9	-0.1	0.31
6.03	23.10	23.30	5.9	-0.1	0.31
7.02	23.08	23.30	6.9	-0.1	0.31
8.02	23.08	23.30	7.9	-0.1	0.31
9.01	22.84	23.30	9.0	0.0	0.31
10.00	23.04	23.30	10.0	0.0	0.31
11.01	22.98	23.30	11.1	0.1	0.31
11.98	23.32	23.30	12.0	0.0	0.31
12.99	23.12	23.30	13.0	0.0	0.31
13.98	23.22	23.30	14.2	0.2	0.31
14.98	23.12	23.30	15.1	0.1	0.31
16.04	23.10	23.30	16.1	0.1	0.33

Remark:


⁵ Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

⁶ Velocity of standard

⁷ Velocity of Unit Under Calibration

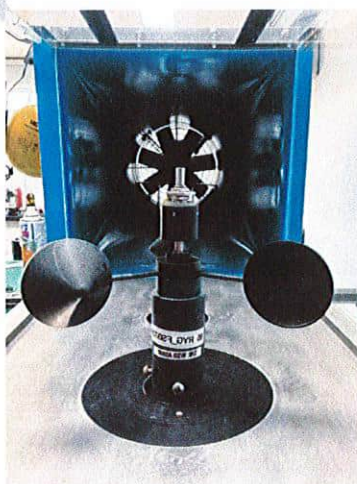PHOTO OF CALIBRATION SET-UP

Calibration set-up of the Cup anemometer calibration in the wind tunnel of Jiranatee Associates Co., Ltd. The Cup anemometer shown may differ from the calibrated one. Remark: The proportion of the set- up is not true to scale due to imaging geometry.



Certificate Number

CWD-017-69

CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

MEASUREMENT ITEM : Wind Direction Sensor
MANUFACTURER : Novalynx
MODEL/TYPE : Sensor: WS-02FA
Data logger: 110-WS-25DL-D
SERIAL NUMBER : Sensor: WSD-A5990
Data logger: A5990
ID NUMBER : RYG_FS0728
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd,
Khwaeng Suan Luang, Khet Suan Luang,
Bangkok 10250 Thailand.

RECEIVED DATE : 06 Feb 2026
MEASUREMENT DATE : 18 Feb 2026
ISSUE DATE : 18 Feb 2026

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa

PLACE OF CALIBRATION : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITION	: Wind tunnel cross-section area ¹	900	cm ²
	Wind direction frontal area ²	129	cm ²
	Diameter of mounting pipe ³	-	mm
	Blockage ratio of test object ⁴	0.143	[-]

Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are (23.1)°C, (58.5) %RH and (1011.6) hPa.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibrated by:

- ☒ Mr. Sorawit Thachalad
☐ Miss Jitraporn Lertsomphol



Approved signatory:

(Signature)

Mr. Parinya Booncharoen
Calibration Department Manager

Remark:

- ¹ Nozzle cross-section area of the wind tunnel
² Projected cross-section area of the tested object include mounting pipe
³ Diameter of mounting pipe
⁴ Ratio ² to ¹

MEASUREMENT RESULTS⁵

The wind direction sensor was calibrated against standard rotary encoder by comparison method. During calibration, the measurement was carried out at 45° intervals in clockwise and counterclockwise directions after offset adjustment has been made. The flow speed of wind tunnel (usually 5 m/s) is kept constant while the sensor is rotated around its vertical axis. The results of calibration and associated measurement uncertainties are reported in the table below.

Air speed m/s	D°_{std} Degree (°)	D°_{uuc} Degree (°)	Error Degree (°)	$U (k=2)$ Degree (°)
5.01	45.000	41	-4	0.60
	90.000	86	-4	0.60
	135.000	132	-3	0.60
	180.000	179	-1	0.82
	225.000	227	2	0.82
	270.000	274	4	0.60
	315.000	320	5	0.60
	360.000	359	-1	0.60

Remark:

⁵ Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

⁶ Direction of standard

⁷ Direction of Unit Under Calibration

End of Certificate of Calibration





JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Temperature measurement laboratory
Calibration services department.



CERTIFICATE OF CALIBRATION

Certificate No. : CDT-063-69

Page 1 of 2 Pages

MEASUREMENT ITEM : Data Logger with Temperature sensor
MANUFACTURER : Novalynx
MODEL/TYPE : 110-WS-25DL-D
SERIAL NUMBER : A5990
ID NUMBER : RYG_FS0728
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Suan Luang, Khet Suan Luang,
Bangkok 10250 Thailand.

RECEIVED DATE : 06 Feb 2026
MEASUREMENT DATE : 18 Feb 2026
ISSUE DATE : 18 Feb 2026

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:

The temperature calibration was done by In-House calibration method as WI-CL-001 according to comparison method with standard digital temperature indicator and standard temperature probe. The temperature scale use was based on ITS-90.

Traceability:

The measurement results are traceable to the international system of units (SI) through National Institute of Metrology Thailand (NIMT) Certificate number: TT-1013-25, Certificate number: ER-0061-25.

Reference Used During Calibration:

1. Standard Temperature Probe
Model: STS-100 A500, Serial No.: 667682-09,
Due date: 9 Apr 2027
2. Digital Temperature Indicator
Model: DTI-1000-A MK II, Serial No.: 671407-00591 Due date: 22 Apr 2027

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor $k=2$, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Calibrated by:

- ☐ Mr. Sorawit Thachalad
☒ Miss Jitraporn Lertsomphol
☐ Miss Ruangrumpai Phoommit



Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager



JIRANATEE ASSOCIATES CO.,LTD.

Continuation of Certificate of Calibration Number CDT-063-69

Page 2 of 2 Pages

Result of Calibration: ☒ Without Adjustment ☐ With Adjustment

Calibration Range: 20 °C to 40 °C

Function:

Table 1: This equipment was connected with temperature sensor Model: HMP60 S/N: W2920792.
Dimension: Diameter 12 mm. Length 80 mm.

<u>Immersion Depth</u> (mm)	<u>Standard Reading</u> (°C)	<u>UUC Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
80	20.026	19.9	-0.1	0.099
80	25.008	24.9	-0.1	0.099
80	30.003	29.8	-0.2	0.099
80	34.998	34.7	-0.3	0.099
80	39.995	39.7	-0.3	0.099

UUC*: Unit Under Calibration

End of Certificate of Calibration



CERTIFICATE OF CALIBRATION

Certificate No. : CRT-008-69

Page 1 of 2 Pages

MEASUREMENT ITEM : Relative humidity with data logger
MANUFACTURER : Novalynx
MODEL/TYPE : Data Logger: 110-WS-25DL-D
Sensor: HMP60
SERIAL NUMBER : Data Logger: A5990
Sensor: W2920792
ID NUMBER : RYG_FS0728
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,
Khet Suan Luang, Bangkok 10250 Thailand.
RECEIVED DATE : 06 Feb 2026
MEASUREMENT DATE : 18 Feb 2026
ISSUE DATE : 18 Feb 2026

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:

The Relative humidity and Air Temperature calibration was done by In-House calibration method as WI-CL-009 and WI-CL-010 according to comparison method with Standard Chilled Mirror hygrometer with Temperature sensor and standard Humidity generator chamber.

Traceability:

The measurements are traceable to the international system of units (SI) through National Institute of Metrology Thailand (NIMT). Certificate number: TH-0146-24 and Jiranatee Associates Co., Ltd. Certificate number: CDT-027-69.

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor $k=2$, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Calibrated by:

- ☐ Mr. Sorawit Thachalad
☒ Miss Jittraporn Lertsomphol
☐ Miss Ruangrumpai Phoommit



Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager

Measurement Results:

The results of calibration and associated measurement uncertainties are reported in the table below.

Result of Calibration: ☒ Without Adjustment ☐ With Adjustment

Table 1: The results of calibration of relative humidity at 30 °C are reported in table below.

Calibration Range: 20%RH to 80%RH

<u>Air Temperature</u> (°C)	<u>Standard Reading</u> (%RH)	<u>UUC Reading</u> (%RH)	<u>Error</u> (%RH)	<u>Uncertainty</u> ± (%RH)
30.06	19.99	18.7	-1.3	0.78
30.06	50.18	48.4	-1.8	1.3
30.04	80.10	79.2	-0.9	2.1

UUC*: Unit Under Calibration

End of Certificate of Calibration





JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Pressure measurement laboratory
Calibration services department.



CERTIFICATE OF CALIBRATION

Certificate No. : CPR-012-69

Page 1 of 2 Pages

MEASUREMENT ITEM : Digital barometer
MANUFACTURER : Novalynx
MODEL/TYPE : Sensor: 110-WS-25BP
Data logger: 110-WS-25DL-D
SERIAL NUMBER : Sensor: BP-A5990
Data logger: A5990
ID NUMBER : RYG_FS0728
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd,
Khwaeng Suan Luang, Khet Suan Luang,
Bangkok 10250 Thailand.

RECEIVED DATE : 06 Feb 2026
MEASUREMENT DATE : 18 Feb 2026
ISSUE DATE : 18 Feb 2026

Calibration procedure:

The Digital barometer was calibrated against Digital pressure calibrator. The WI-CL-003 was used as a calibration guideline.

Traceability:

The measurement results are traceable to the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MP-0017-25

Reference Used During Calibration:

1. Absolute Pressure Transducer
Model: CPG2500, Serial No.: 4100126P

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor $k=2$, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

CONDITION OF THIS RESULT OF CALIBRATION:

- Calibration effort for calibration sequence C
- The UUC* was installed in vertical orientation above reference standard instrument and center of UUC* was used as the reference level.
- Calibration conditions:
- Condition : ☒ Normal ☐ Abnormal
Pressure transmitting medium : Air
 ρ_{Fl} (20°C, 1 bar) : 1.19 kg/m³
 H_{amb} : (62.4±7.2) %
 t_{amb} : (22.9±0.3) °C
 p_{amb} : (1014.5±0.9) mbar
- The certificate is valid only to the item calibrated on date and place of calibration

Calibrated by:

- ☒ Mr. Sorawit Thachalad
☐ Miss Jitraporn Lertsomphol



Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager



JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd.
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367



Pressure measurement laboratory
Calibration services department.

CERTIFICATE OF CALIBRATION

Certificate No. : CPR-012-69

Page 2 of 2 Pages

MEASUREMENT RESULTS : ☒ Without adjustment ☐ With adjustment

CALIBRATION IN THE RANGE OF : 950 mbar to 1050 mbar

The results of calibration and associated measurement uncertainties are reported in the table below.

STD (mbar)	UUC* (mbar)	Error (mbar)	Uncertainty (k=2) (mbar)
949.94	951.9	1.9	0.37
970.00	971.3	1.3	0.37
990.01	990.7	0.7	0.37
1009.99	1010.2	0.2	0.37
1030.00	1029.6	-0.4	0.37
1050.01	1049.0	-1.0	0.37

Note: UUC* Unit Under Calibration

: To convert the result in report unit to Pa should be multiply by 100

End of certificate



Certificate Number

CWS-003-69

CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

MEASUREMENT ITEM : Cup anemometer
MANUFACTURER : Novalynx
MODEL/TYPE : Sensor: WS-02F
Data logger: 110-WS-25DL-D
SERIAL NUMBER : Sensor: WSD-A5912
Data logger: A5912
ID NUMBER : RYG_FS0611
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd,
Khwaeng Suan Luang, Khet Suan Luang,
Bangkok 10250 Thailand.

RECEIVED DATE : 19 Dec 2025
MEASUREMENT DATE : 06 Jan 2026
ISSUE DATE : 06 Jan 2026

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa

PLACE OF CALIBRATION : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITIONS

: Wind tunnel cross-section area ¹	900	cm ²
Cup anemometer frontal area ²	100	cm ²
Diameter of mounting pipe ³	-	mm
Blockage ratio of test object ⁴	0.111	[-]

Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are (24.4) °C, (58.1) %RH and (1008.5) hPa.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibrated by:

- ☒ Mr. Sorawit Thachalad
☐ Miss Jittraporn Lertsomphol



Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager

Calibration procedure:

The Cup anemometer was calibrated against Standard air velocity transducer model: 8455-12 and pitot tube with precision differential pressure meter model: DPM2500 in an close test-section of Eiffel-type wind tunnel with 900 cm² cross test section area. The WI-CL-007 based on IEC 61400-12-1, Wind energy generation systems – Part 12-1: Power performance measurements of electricity producing wind turbines, March 2017 was used as a calibration guideline.

Traceability:

This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MW-0019-25 and MW-0059-25

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

REVIEW BY *Supt S*

APPROVED BY *[Signature]*

NEXT CAL DATE..... 05/ 07/ 2027

Remark:

- ¹ Nozzle cross-section area of the wind tunnel
² Projected cross-section area of the tested object include mounting pipe
³ Diameter of mounting pipe
⁴ Ratio ² to ¹

MEASUREMENT RESULTS⁵

The Cup anemometer, Unit Under Calibration (UUC) was exercised at 10 m/s for 5 minutes prior to calibration being performed. The standard air velocity 0.5 m/s to 5 m/s was calculated by a standard air velocity transducer which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section and the standard air velocity 5 m/s to 30 m/s was calculated by a pitot tube with precision differential pressure meter which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section, UUC was mounted on a round vertical tube of the lower plate at center of test section. The calibration was carried out under both rising and falling air velocity in the range of 1 m/s to 16 m/s at calibration interval of 1 m/s. The results of calibration and associated measurement uncertainties are reported in the table below.

V_{std} ⁶ (m/s)	Temp. wind tunnel (°C)	Temp. room (°C)	V_{UUC} ⁷ (m/s)	Error (m/s)	$U (k=2)$ (m/s)
1.015	24.32	24.35	0.8	-0.2	0.31
2.249	24.30	24.35	2.0	-0.2	0.31
3.011	24.50	24.35	2.8	-0.2	0.31
4.232	24.46	24.35	3.9	-0.3	0.31
4.96	24.30	24.35	4.9	-0.1	0.31
6.03	24.88	24.35	5.9	-0.1	0.31
6.97	24.30	24.35	6.9	-0.1	0.31
7.97	24.70	24.35	8.0	0.0	0.31
8.97	24.40	24.35	9.0	0.0	0.31
9.97	24.50	24.35	10.0	0.0	0.31
11.02	24.30	24.35	11.1	0.1	0.31
12.03	24.34	24.35	12.1	0.1	0.31
13.01	24.18	24.35	13.2	0.2	0.31
14.01	24.12	24.35	14.2	0.2	0.31
15.00	24.04	24.35	15.3	0.3	0.35
16.01	24.00	24.35	16.3	0.3	0.31

Remark:

⁵ Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

⁶ Velocity of standard

⁷ Velocity of Unit Under Calibration

PHOTO OF CALIBRATION SET-UP

Calibration set-up of the Cup anemometer calibration in the wind tunnel of Jiranatee Associates Co., Ltd. The Cup anemometer shown may differ from the calibrated one. Remark: The proportion of the set-up is not true to scale due to imaging geometry.

End of Certificate of Calibration

**J
NAC**

JIRANATEE ASSOCIATES CO., LTD.

Certificate Number

CWD-003-69

CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

MEASUREMENT ITEM : Wind Direction Sensor
MANUFACTURER : Novalynx
MODEL/TYPE : Sensor: WS-02F
Data logger: 110-WS-25DL-D
SERIAL NUMBER : Sensor: WSD- A5912
Data logger: A5912
ID NUMBER : RYG_FS0611
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd,
Khwaeng Suan Luang, Khet Suan Luang,
Bangkok 10250 Thailand.

RECEIVED DATE : 19 Dec 2025
MEASUREMENT DATE : 06 Jan 2026
ISSUE DATE : 06 Jan 2026

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa

PLACE OF CALIBRATION : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITION	: Wind tunnel cross-section area ¹	900	cm ²
	Wind direction frontal area ²	129	cm ²
	Diameter of mounting pipe ³	-	mm
	Blockage ratio of test object ⁴	0.143	[-]

Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are (24.7)°C, (63.6) %RH and (1007.9) hPa.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibrated by:

- ☒ Mr. Sorawit Thachalad
☐ Miss Jitraporn Lertsomphol



Approved signatory:

Mr. Parinya Booncharoen
Mr. Parinya Booncharoen
Calibration Department Manager

Remark:

- ¹ Nozzle cross-section area of the wind tunnel
² Projected cross-section area of the tested object include mounting pipe
³ Diameter of mounting pipe
⁴ Ratio ² to ¹

MEASUREMENT RESULTS⁵

The wind direction sensor was calibrated against standard rotary encoder by comparison method. During calibration, the measurement was carried out at 45° intervals in clockwise and counterclockwise directions after offset adjustment has been made. The flow speed of wind tunnel (usually 5 m/s) is kept constant while the sensor is rotated around its vertical axis. The results of calibration and associated measurement uncertainties are reported in the table below.

Air speed m/s	D°_{std} Degree (°)	D°_{uuc} Degree (°)	Error Degree (°)	$U (k=2)$ Degree (°)
4.99	0.000	0	0	0.60
	45.000	42	-3	0.82
	90.000	87	-3	0.89
	135.000	132	-3	0.95
	180.000	177	-3	0.82
	225.000	224	-1	0.82
	270.000	271	1	0.82
	315.000	318	3	0.82

Remark:

⁵ Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

⁶ Direction of standard

⁷ Direction of Unit Under Calibration

End of Certificate of Calibration



CERTIFICATE OF CALIBRATION

Certificate No. : CDT-002-69

Page 1 of 2 Pages

MEASUREMENT ITEM : Data Logger with Temperature sensor
MANUFACTURER : Novalynx
MODEL/TYPE : 110-WS-25DL-D
SERIAL NUMBER : A5912
ID NUMBER : RYG_FS0611
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Suan Luang, Khet Suan Luang,
Bangkok 10250 Thailand.

RECEIVED DATE : 19 Dec 2025
MEASUREMENT DATE : 06 Jan 2026
ISSUE DATE : 06 Jan 2026

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:

The temperature calibration was done by In-House calibration method as WI-CL-001 according to comparison method with standard digital temperature indicator and standard temperature probe. The temperature scale use was based on ITS-90.

Traceability:

The measurement results are traceable to the international system of units (SI) through National Institute of Metrology Thailand (NIMT) Certificate number: TT-1013-25, Certificate number: ER-0061-25.

Reference Used During Calibration:

1. Standard Temperature Probe
Model: STS-100 A500, Serial No.: 667682-09,
Due date: 9 Apr 2026
2. Digital Temperature Indicator
Model: DTI-1000-A MK II, Serial No.: 671407-00591 Due date: 22 Apr 2026

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor $k=2$, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Calibrated by:

- ☐ Mr. Sorawit Thachalad
☒ Miss Jitraporn Lertsomphol
☐ Miss Ruangrumpai Phoommit



Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager

Result of Calibration: ☒ Without Adjustment ☐ With Adjustment

Calibration Range: 20 °C to 40 °C

Function:

Table 1: This equipment was connected with temperature sensor Model: HMP60 S/N: U3911247.
Dimension: Diameter 12 mm. Length 80 mm.

<u>Immersion Depth</u> (mm)	<u>Standard Reading</u> (°C)	<u>UUC Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
80	20.059	19.7	-0.4	0.099
80	25.043	24.6	-0.4	0.099
80	30.035	29.7	-0.3	0.099
80	35.022	34.6	-0.4	0.099
80	39.998	39.5	-0.5	0.099

UUC*: Unit Under Calibration

End of Certificate of Calibration





JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367



Relative humidity and Air Temperature measurement laboratory
Calibration services department.

CERTIFICATE OF CALIBRATION

Certificate No. : CRT-002-69

Page 1 of 2 Pages

MEASUREMENT ITEM : Relative humidity with data logger
MANUFACTURER : Novalynx
MODEL/TYPE : Data Logger: 110-WS-25DL-D
Sensor: HMP60
SERIAL NUMBER : Data Logger: A5912
Sensor: U3911247
ID NUMBER : RYG_FS0611
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,
Khet Suan Luang, Bangkok 10250 Thailand.
RECEIVED DATE : 19 Dec 2025
MEASUREMENT DATE : 06 Jan 2026
ISSUE DATE : 06 Jan 2026

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:

The Relative humidity and Air Temperature calibration was done by In-House calibration method as WI-CL-009 and WI-CL-010 according to comparison method with Standard Chilled Mirror hygrometer with Temperature sensor and standard Humidity generator chamber.

Traceability:

The measurements are traceable to the international system of units (SI) through National Institute of Metrology Thailand (NIMT). Certificate number: TH-0146-24 and Jiranatee Associates Co., Ltd. Certificate number: CDT-026-68.

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor $k=2$, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Calibrated by:

- ☐ Mr. Sorawit Thachalad
☒ Miss Jitraporn Lertsomphol
☐ Miss Ruangrumpai Phoommit



Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager



JIRANATEE ASSOCIATES CO.,LTD.

Continuation of Certificate of Calibration Number: CRT-002-69

Page 2 of 2 Pages

Measurement Results:

The results of calibration and associated measurement uncertainties are reported in the table below.

Result of Calibration: ☒ Without Adjustment ☐ With Adjustment

Table 1: The results of calibration of relative humidity at 30 °C are reported in table below.

Calibration Range: 20%RH to 80%RH

<u>Air Temperature</u> (°C)	<u>Standard Reading</u> (%RH)	<u>UUC Reading</u> (%RH)	<u>Error</u> (%RH)	<u>Uncertainty</u> ± (%RH)
30.03	20.01	19.0	-1.0	0.78
30.06	50.03	48.5	-1.5	1.3
30.03	80.04	77.3	-2.7	2.1

UUC*: Unit Under Calibration

End of Certificate of Calibration





JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd.Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Pressure measurement laboratory
Calibration services department.



CERTIFICATE OF CALIBRATION

Certificate No. : CPR-002-69

Page 1 of 2 Pages

MEASUREMENT ITEM : Digital barometer
MANUFACTURER : Novalynx
MODEL/TYPE : Sensor: 110-WS-25BP
Data logger: 110-WS-25DL-D
SERIAL NUMBER : Sensor: BP-A5912
Data logger: A5912
ID NUMBER : RYG_FS0611
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd,
Khwaeng Suan Luang, Khet Suan Luang,
Bangkok 10250 Thailand.

RECEIVED DATE : 19 Dec 2025
MEASUREMENT DATE : 06 Jan 2026
ISSUE DATE : 06 Jan 2026

Calibration procedure:

The Digital barometer was calibrated against Digital pressure calibrator. The WI-CL-003 was used as a calibration guideline.

Traceability:

The measurement results are traceable to the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MP-0017-25

Reference Used During Calibration:

1. Absolute Pressure Transducer
Model: CPG2500, Serial No.: 4100126P

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor $k=2$, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

CONDITION OF THIS RESULT OF CALIBRATION:

- Calibration effort for calibration sequence C
- The UUC* was installed in vertical orientation above reference standard instrument and center of UUC* was used as the reference level.
- Calibration conditions:
- Condition : ☒ Normal ☐ Abnormal
Pressure transmitting medium : Air
 ρ_{Fi} (20°C, 1 bar) : 1.19 kg/m³
 H_{amb} : (53.1±5.2) %
 t_{amb} : (23.2±0.2) °C
 p_{amb} : (1012.5±0.6) mbar
- The certificate is valid only to the item calibrated on date and place of calibration

Calibrated by:

- ☒ Mr. Sorawit Thachalad
☐ Miss Jitraporn Lertsomphol



Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager



JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd.
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Pressure measurement laboratory
Calibration services department.



CERTIFICATE OF CALIBRATION

Certificate No. : CPR-002-69

Page 2 of 2 Pages

MEASUREMENT RESULTS : ☐ Without adjustment ☒ With adjustment

CALIBRATION IN THE RANGE OF : 950 mbar to 1050 mbar

The results of calibration and associated measurement uncertainties are reported in the table below.

STD (mbar)	UUC* (mbar)	Error (mbar)	Uncertainty (k=2) (mbar)
950.03	951.3	1.3	0.37
970.01	970.9	0.9	0.40
990.02	990.5	0.5	0.37
1010.00	1010.2	0.2	0.37
1029.99	1029.7	-0.3	0.41
1049.99	1049.3	-0.7	0.37

Note: UUC* Unit Under Calibration

: To convert the result in report unit to Pa should be multiply by 100





JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Air speed measurement laboratory
Calibration services department.



NSC – TISI – TIS 17025
CALIBRATION 0367

Certificate Number

CWS-009-69

CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

MEASUREMENT ITEM : Cup anemometer
MANUFACTURER : Novalynx
MODEL/TYPE : Sensor: WS-02F
Data logger: 110-WS-25DL-D
SERIAL NUMBER : Sensor: WSD-A5909
Data logger: A5909
ID NUMBER : RYG_FS0608
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd,
Khwaeng Suan Luang, Khet Suan Luang,
Bangkok 10250 Thailand.

RECEIVED DATE : 09 Jan 2026
MEASUREMENT DATE : 21 Jan 2026
ISSUE DATE : 21 Jan 2026

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa

PLACE OF CALIBRATION : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITIONS

Wind tunnel cross-section area ¹	900	cm ²
Cup anemometer frontal area ²	100	cm ²
Diameter of mounting pipe ³	-	mm
Blockage ratio of test object ⁴	0.111	[-]

Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are (23.4) °C, (56.6) %RH and (1008.9) hPa.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibrated by:

- ☒ Mr. Sorawit Thachalad
☐ Miss Jitraporn Lertsomphol



Approved signatory: _____

Mr. Parinya Booncharoen
Calibration Department Manager

Calibration procedure:

The Cup anemometer was calibrated against Standard air velocity transducer model: 8455-12 and pitot tube with precision differential pressure meter model: DPM2500 in an close test-section of Eiffel-type wind tunnel with 900 cm² cross test section area. The WI-CL-007 based on IEC 61400-12-1, Wind energy generation systems – Part 12-1: Power performance measurements of electricity producing wind turbines, March 2017 was used as a calibration guideline.

Traceability:

This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MW-0019-25 and MW-0059-25

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

REVIEW BY

APPROVED BY

NEXT CAL DATE 20/ 07/ 2027

Remark:

- ¹ Nozzle cross-section area of the wind tunnel
² Projected cross-section area of the tested object include mounting pipe
³ Diameter of mounting pipe
⁴ Ratio ² to ¹

MEASUREMENT RESULTS ⁵

The Cup anemometer, Unit Under Calibration (UUC) was exercised at 10 m/s for 5 minutes prior to calibration being performed. The standard air velocity 0.5 m/s to 5 m/s was calculated by a standard air velocity transducer which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section and the standard air velocity 5 m/s to 30 m/s was calculated by a pitot tube with precision differential pressure meter which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section, UUC was mounted on a round vertical tube of the lower plate at center of test section. The calibration was carried out under both rising and falling air velocity in the range of 1 m/s to 16 m/s at calibration interval of 1 m/s. The results of calibration and associated measurement uncertainties are reported in the table below.


V_{std} ⁶ (m/s)	Temp. wind tunnel (°C)	Temp. room (°C)	V_{UUC} ⁷ (m/s)	Error (m/s)	$U (k=2)$ (m/s)
1.039	23.30	23.35	0.9	-0.1	0.31
2.182	23.40	23.35	2.0	-0.2	0.31
2.997	23.32	23.35	2.9	-0.1	0.31
4.241	23.32	23.35	4.0	-0.2	0.31
4.96	23.18	23.35	5.0	0.0	0.31
6.02	23.50	23.35	6.0	0.0	0.31
6.96	23.08	23.35	6.9	0.0	0.31
7.96	23.50	23.35	8.0	0.0	0.31
8.94	22.90	23.35	9.1	0.2	0.31
9.96	23.48	23.35	10.1	0.1	0.31
10.95	23.00	23.35	11.2	0.2	0.31
12.01	23.22	23.35	12.2	0.2	0.31
13.00	23.06	23.35	13.4	0.4	0.31
14.02	23.06	23.35	14.3	0.3	0.31
14.98	22.86	23.35	15.5	0.5	0.31
15.99	22.84	23.35	16.5	0.5	0.31

Remark:

⁵ Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

⁶ Velocity of standard

⁷ Velocity of Unit Under Calibration

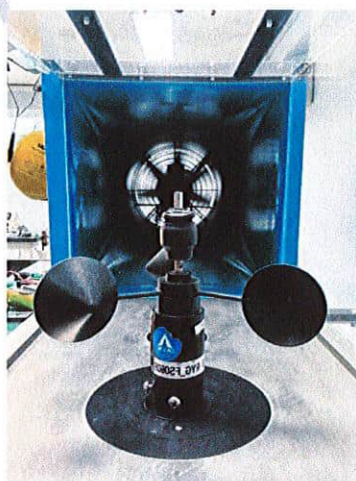PHOTO OF CALIBRATION SET-UP

Calibration set-up of the Cup anemometer calibration in the wind tunnel of Jiranatee Associates Co., Ltd. The Cup anemometer shown may differ from the calibrated one. Remark: The proportion of the set-up is not true to scale due to imaging geometry.



JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Wind direction measurement laboratory
Calibration services department.



NSC – TISI – TIS 17025
CALIBRATION 0367

Certificate Number

CWD-009-69

CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

MEASUREMENT ITEM : Wind Direction Sensor
MANUFACTURER : Novalynx
MODEL/TYPE : Sensor: WS-02F
Data logger: 110-WS-25DL-D
SERIAL NUMBER : Sensor: WSD- A5909
Data logger: A5909
ID NUMBER : RYG_FS0608
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd,
Khwaeng Suan Luang, Khet Suan Luang,
Bangkok 10250 Thailand.

RECEIVED DATE : 09 Jan 2026
MEASUREMENT DATE : 21 Jan 2026
ISSUE DATE : 21 Jan 2026

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa

PLACE OF CALIBRATION : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITION	: Wind tunnel cross-section area ¹	900	cm ²
	Wind direction frontal area ²	129	cm ²
	Diameter of mounting pipe ³	-	mm
	Blockage ratio of test object ⁴	0.143	[-]

Preconditioning : 24 hours at ambient conditions.

Measurement Condition : The average values during measurement are (23.5)°C, (62.6) %RH and (1008.6) hPa.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibrated by:

- ☒ Mr. Sorawit Thachalad
☐ Miss Jittrapon Lertsomphol



Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager

Remark:

- ¹ Nozzle cross-section area of the wind tunnel
² Projected cross-section area of the tested object include mounting pipe
³ Diameter of mounting pipe
⁴ Ratio ² to ¹

MEASUREMENT RESULTS⁵

The wind direction sensor was calibrated against standard rotary encoder by comparison method. During calibration, the measurement was carried out at 45° intervals in clockwise and counterclockwise directions after offset adjustment has been made. The flow speed of wind tunnel (usually 5 m/s) is kept constant while the sensor is rotated around its vertical axis. The results of calibration and associated measurement uncertainties are reported in the table below.

Air speed m/s	D°_{std} Degree (°)	D°_{uuc} Degree (°)	Error Degree (°)	$U (k=2)$ Degree (°)
5.02	0.000	0	0	0.60
	45.000	42	-3	0.93
	90.000	87	-3	0.60
	135.000	132	-3	0.60
	180.000	178	-2	0.60
	225.000	226	1	0.60
	270.000	273	3	0.60
	315.000	320	5	0.60

Remark:

⁵ Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

⁶ Direction of standard

⁷ Direction of Unit Under Calibration

End of Certificate of Calibration





JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd.
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Temperature measurement laboratory
Calibration services department.



CERTIFICATE OF CALIBRATION

Certificate No. : CDT-029-69

Page 1 of 2 Pages

MEASUREMENT ITEM : Data Logger with Temperature sensor
MANUFACTURER : Novalynx
MODEL/TYPE : 110-WS-25DL-D
SERIAL NUMBER : A5909
ID NUMBER : RYG_FS0608
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Suan Luang, Khet Suan Luang,
Bangkok 10250 Thailand.

RECEIVED DATE : 09 Jan 2026
MEASUREMENT DATE : 21 Jan 2026
ISSUE DATE : 21 Jan 2026

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:

The temperature calibration was done by In-House calibration method as WI-CL-001 according to comparison method with standard digital temperature indicator and standard temperature probe. The temperature scale use was based on ITS-90.

Traceability:

The measurement results are traceable to the international system of units (SI) through National Institute of Metrology Thailand (NIMT) Certificate number: TT-1013-25, Certificate number: ER-0061-25.

Reference Used During Calibration:

1. Standard Temperature Probe
Model: STS-100 A500, Serial No.: 667682-09,
Due date: 9 Apr 2026
2. Digital Temperature Indicator
Model: DTI-1000-A MK II, Serial No.: 671407-00591 Due date: 22 Apr 2026

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor $k=2$, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Calibrated by:

- ☐ Mr. Sorawit Thachalad
☒ Miss Jitraporn Lertsomphol
☐ Miss Ruangrumpai Phoommit



Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager



JIRANATEE ASSOCIATES CO.,LTD.

Continuation of Certificate of Calibration Number CDT-029-69

Page 2 of 2 Pages

Result of Calibration: ☒ Without Adjustment ☐ With Adjustment

Calibration Range: 20 °C to 40 °C

Function:

Table 1: This equipment was connected with temperature sensor Model: HMP60 S/N: U3641220.
Dimension: Diameter 12 mm. Length 80 mm.

<u>Immersion Depth</u> (mm)	<u>Standard Reading</u> (°C)	<u>UUC Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
80	20.047	19.8	-0.2	0.099
80	25.031	24.8	-0.2	0.099
80	30.030	29.8	-0.2	0.099
80	35.015	34.7	-0.3	0.099
80	40.001	39.8	-0.2	0.099

UUC*: Unit Under Calibration

End of Certificate of Calibration





JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Relative humidity and Air Temperature measurement laboratory
Calibration services department.



CERTIFICATE OF CALIBRATION

Certificate No. : CRT-005-69

Page 1 of 2 Pages

MEASUREMENT ITEM : Relative humidity with data logger
MANUFACTURER : Novalynx
MODEL/TYPE : Data Logger: 110-WS-25DL-D
Sensor: HMP60
SERIAL NUMBER : Data Logger: A5909
Sensor: U3641220
ID NUMBER : RYG_FS0608
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,
Khet Suan Luang, Bangkok 10250 Thailand.
RECEIVED DATE : 09 Jan 2026
MEASUREMENT DATE : 21 Jan 2026
ISSUE DATE : 21 Jan 2026

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:

The Relative humidity and Air Temperature calibration was done by In-House calibration method as WI-CL-009 and WI-CL-010 according to comparison method with Standard Chilled Mirror hygrometer with Temperature sensor and standard Humidity generator chamber.

Traceability:

The measurements are traceable to the international system of units (SI) through National Institute of Metrology Thailand (NIMT). Certificate number: TH-0146-24 and Jiranatee Associates Co., Ltd. Certificate number: CDT-026-68.

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor $k=2$, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Calibrated by:

- ☐ Mr. Sorawit Thachalad
☒ Miss Jitraporn Lertsomphol
☐ Miss Ruangrumpai Phoommit



Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager



JIRANATEE ASSOCIATES CO.,LTD.

Continuation of Certificate of Calibration Number: CRT-005-69

Page 2 of 2 Pages

Measurement Results:

The results of calibration and associated measurement uncertainties are reported in the table below.

Result of Calibration: ☐ Without Adjustment ☒ With Adjustment

Table 1: The results of calibration of relative humidity at 30 °C are reported in table below.

Calibration Range: 20%RH to 80%RH

<u>Air Temperature</u> (°C)	<u>Standard Reading</u> (%RH)	<u>UUC Reading</u> (%RH)	<u>Error</u> (%RH)	<u>Uncertainty</u> ± (%RH)
30.10	19.96	21.3	1.3	0.78
30.11	49.95	50.4	0.4	1.3
30.11	80.06	79.2	-0.9	2.1

UUC*: Unit Under Calibration

End of Certificate of Calibration





CONSOLE CONTROL UNIT CALIBRATION TEST REPORT

Calibration of Date **6-Jan-26**
 Next Calibration Date 06-Jul-26
 Certificate No. C-060126-BKK_FS0556

Barometric Pressure (mm.Hg) : **756.1**
 Relative Humidity (%) : **46.5**
 Temperature (°C) : **27.0**

Console Control Meter Data

Dry Gas Meter ID **BKK_FS0556**
 Brand APEX INSTRUMENT
 Serial No. 1606041
 Model No. XC-572-V

Reference Dry Gas Meter Data

Reference Dry Gas Meter ID : **BKK_FS1122**
 Serial No. : A2003240
 Correction Factor (Y) : 1.000
 Next Calibration Date : 26-Feb-26

ΔH (mm.H ₂ O)	Θ Minutes	Reference Dry Gas Meter Calibration				Console Control ; Drygas Meter						Dry Gas Meter	Orifice
		Vr (Liters)			Tr (°C)	Vm (Liters)			Ti (°C)	To (°C)	Avg.Tm (°C)	Correction	Calibration
		Final	Initial	Total		Final	Initial	Total				Factor (Y)	Factor $\Delta H@$
15	11.90	150.03	0.00	150.03	30.0	707296.8	707153.0	143.80	28.0	28.0	28.0	1.0349	43.8195
25	9.25	150.12	0.00	150.12	29.0	707448.8	707304.0	144.80	28.0	28.0	28.0	1.0308	43.7838
50	6.60	150.10	0.00	150.10	28.0	707599.4	707454.0	145.40	28.0	28.0	28.0	1.0273	44.2943
100	4.67	150.40	0.00	150.40	27.0	707752.0	707606.2	145.80	28.0	28.0	28.0	1.0250	43.8844
150	3.80	150.11	0.00	150.11	25.0	707904.8	707759.2	145.60	28.0	28.0	28.0	1.0264	43.1725
Avg.												1.0289	43.7909

Y : Ratio of reading of reference to dry gas meter : tolerance for individual values ± 0.02 from average .

$\Delta H@$: Orifice pressure differential that equates to 21.24 lm of air @ 25 C and 760 mm of mercury , mmH₂O ; tolerance for individual values ± 5.08 from average .

Procedure; 40 CFR 60,APP A,METH ,SEC 5.3 & 7

Calibrated by:

Apisit Singha

(Mr. Apisit Singha)

Field Services Scientist (4)

Approved by:

Natthapon Jiengwareewong

(Mr. Natthapon Jiengwareewong)

Field Services Specialist (1)

Issue date : 07-Jan-26




DIGITAL TEMPERATURE CALIBRATION DATA SHEET

Calibration Date :	6 Jan 26	Ambient Temperature (°C)	27
Calibration sheet No. :	C-060126-BKK_FS0557	Relative Humidity (%) :	46.5
Digital Temperature ID :	BKK_FS0557	Reference Temperature ID	RYF_FS0681
Serial No. :	1302005	Serial No. :	201090014918
Model :	XC-572-V	Model :	DIGICON CC-VT-MS
		Next Calibrate :	16 Jan 27


Location	Reference Temperature °C	Digital Temperature °C	Error °C	MPE	Pass / Fail
Stack	0	0	0	±3	Pass
	25	26	1	±3	Pass
	50	50	0	±3	Pass
	100	101	1	±3	Pass
	150	151	1	±3	Pass
	200	200	0	±3	Pass
	250	250	0	±3	Pass
	300	301	1	±3	Pass
	500	501	1	±3	Pass
Probe	100	101	1	±3	Pass
	120	121	1	±3	Pass
	140	141	1	±3	Pass
Oven	100	101	-2	±3	Pass
	120	121	-3	±3	Pass
	140	141	3	±3	Pass
Filter	100	100	0	±3	Pass
	120	120	0	±3	Pass
	140	141	1	±3	Pass
Exit	0	0	0	±3	Pass
	10	11	1	±3	Pass
	20	21	1	±3	Pass
Meter	0	0	0	±3	Pass
	25	25	0	±3	Pass
	50	51	1	±3	Pass
AUX	0	0	0	±3	Pass
	25	26	1	±3	Pass
	50	51	1	±3	Pass

MPE : (Maximum permissible error of measurement) ค่าความผิดพลาดสูงสุดของการวัดที่ยอมรับได้

Calibrated by : 

(Mr.Apisit Sing-ha)

Field Scientist (4)

Approved by : 

Mr.Natthapol Jiengwareewong

Field Specialist (1)



PROBE NOZZLE DIAMETER CALIBRATION DATA SHEET

Calibration Date : 6 Jan 26	Nozzle Set ID. : BKK_FS0562
Calibration Sheet No. : C-060126-BKK_FS0562	Vernier Caliper ID.: BKK_FS0626


Nozzle ID #	Nozzle Diameter (cm.)			Hi - Lo	$(D_1 + D_2 + D_3) / 3$
	D_1	D_2	D_3	ΔD	D_{avg}
1	0.300	0.300	0.302	0.002	0.301
2	0.475	0.475	0.469	0.006	0.473
3	0.530	0.525	0.530	0.005	0.528
4	0.625	0.628	0.630	0.005	0.628
5	0.759	0.760	0.765	0.006	0.761
6	0.975	0.977	0.980	0.005	0.977
7	1.082	1.085	1.081	0.004	1.083
8	1.272	1.270	1.275	0.005	1.272
9	1.605	1.601	1.609	0.008	1.605

Where :

D_1, D_2, D_3 = There different nozzle diameters at 60 degrees to each other, each measured the nearest 0.025 mm.

ΔD = Maximum distance between any two diameters, must be ≤ 0.100 mm.

D_{avg} = $(D_1 + D_2 + D_3) / 3$

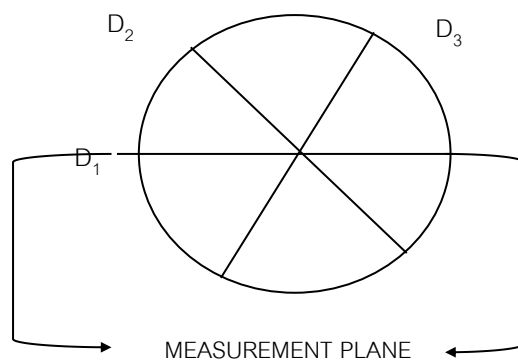

Calibrated by : 

(Mr. Warawut Pubpa)

Field Scientist (3)

Approved by : 


(Mr. Natthapol Jiengwareewong)

Field Specialist (1)



Type S Pitot Tube Calibration

Date Calibration	6-Jan-26	Due Date	6-Jul-26
Pitot ID	BKK_FS0560	Inclinometer ID	BKK_FS1131
Pitot SN	1803811	Vernier ID	RYG_FS0539

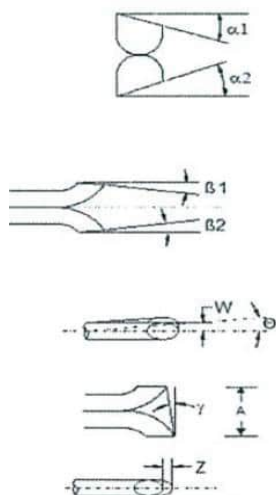

Parameter	Value	Allowable Range	Check
$\alpha 1$	0.4	$-10^{\circ} < \alpha 1 < +10^{\circ}$	OK
$\alpha 2$	1.6	$-10^{\circ} < \alpha 2 < +10^{\circ}$	OK
$\beta 1$	1.7	$-5^{\circ} < \beta 1 < +5^{\circ}$	OK
$\beta 2$	0.2	$-5^{\circ} < \beta 2 < +5^{\circ}$	OK
γ	2.2	-	-
θ	1.6	-	-
$Z = A \tan \gamma$	0.032	$Z \leq 0.125"$	OK
$W = A \tan \theta$	0.023	$W \leq 0.031"$	OK
Dt	0.300	0.188" to 0.375"	OK
$A/2Dt$	1.373	$1.05 \leq PA/Dt \leq 1.5$	OK
A	0.824	$2.1Dt \leq A \leq 3Dt$	OK

Certify that pitot tube/porbe meets or exceeds all specifications, criteria and/or applicable design features and is hereby assigned a pitot tube certification fact of 0.84 . See 40 CFR Pt. 60, App. A,EPA Method 2.

Calibrated by : Saksit Phaisanphisut
 (Mr. Saksit Phaisanphisut)
 RYG Field Services Scientist (4)

Approved By : Nattapol Jiengwareewong
 (Mr.Nattapol Jiengwareewong)
 RYG Field Services Specialist (1)

Certificate No: G 680210

Date of issue : 25-Mar-25

Instrument description :	Flue Gas Analyzer
Instrument model :	Testo 350 New
Instrument serial no. :	62087344/1119
Control unit serial no. :	03401649/1119
ID no. or control no. :	RYG_FS0464
Manufacturer :	Testo SE & Co. KGaA
Probe description :	-
Probe model :	-
Probe serial no. :	-
Customer name :	ALS LABORATORY GROUP (THAILAND) CO.,LTD.
Customer address :	104 Phatthanakan 40, Phatthanakan Road, Khwaeng Phatthanakan, Khet Suan Luang, Bangkok, 10250 Thailand
Total pages of certificate :	3 Pages
Receiving no. :	L-250946
Receiving date. :	18-Mar-25
Parameter of calibration :	Gas Calibration(Oxygen 2.50,9.984,21.02 %vol, Carbon Monoxide 80.45,302,1007 ppm, Nitrogen Dioxide 30.68,81.8,202.6 ppm, Nitric Oxide 30.0,151.8,322.5 ppm, Sulphur Dioxide 50.36,100.7,600.8 ppm)
Condition of UUC. :	Used
Ambient condition :	All of the Measurment ware caried out the stabilized labotary Temperature : 23 ±5 °C Humidity : 55 ± 15 %RH
Calibration place :	17/121 Soi Ngamwongwan 47 Yaek 48, Toongsonghong, Laksi, Bangkok 10210 THAILAND
Calibration procedure no :	This instrument was calibrated by comparison with Standard gas mixture according to calibration Work Instruction no. WI-CL-28-C

REVIEW BY 

APPROVED BY..... 

NEXT CAL DATE.....23/ 03/ 2026

*The calibration certificate expanded uncertainty of measurement is stated as the standard uncertainty of measurent
Multiplied by coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.*

This certificate is applied only to item under test Environmental condition.

*This Calibration Certificate may not be reporduced other than in full except with the permission of the issuing laboratory.
Calibration certificates without signature and seal not valid and The results relate only to the items tested/calibrated.*

*This calibration certificate documents are tracebility to national standards, which realize measurement according to the
International System of Units (SI).*

Date of calibration : 24-Mar-25



Mr. Kwanchai Khamdoun
Calibration Technician



Mrs. Nongluck Wongsettee
Technical Manager

Certificate No.: G 680210

Standard References (Table 1)

Standard	Certificate No.	Vendor	Due date
Oxygen (O ₂) 2.50 % Vol	2412/23	Linde	27-Aug-27
Oxygen (O ₂) 9.984 % Vol	CG-0113-24	Nimt	01-Aug-29
Oxygen (O ₂) 21.02 % Vol	CG-0041-22	Nimt	10-Feb-27
Carbon monoxide (CO) 80.45 ppm	CG-0132-24	Nimt	10-Sep-29
Carbon monoxide (CO) 302 ppm	1915/23	Linde	16-Jun-25
Carbon monoxide (CO) 1007 ppm	1870/24	Linde	17-Jun-26
Nitrogen Dioxide (NO ₂) 30.68 ppm	2832/24	Linde	08-Sep-26
Nitrogen Dioxide (NO ₂) 81.8 ppm	2330/24	Linde	01-Aug-26
Nitrogen Dioxide (NO ₂) 202.6 ppm	3794/24	Linde	23-Dec-26
Nitric Oxide (NO) 30.0 ppm	CG-0065-24	Nimt	06-May-26
Nitric Oxide (NO) 151.8 ppm	0404/25	Linde	09-Feb-27
Nitric Oxide (NO) 322.5 ppm	1974/23	Linde	17-Jul-25
Sulphur Dioxide (SO ₂) 50.36 ppm	2004/23	Linde	17-Jul-25
Sulphur Dioxide (SO ₂) 100.7 ppm	2662/24	Linde	25-Aug-26
Sulphur Dioxide (SO ₂) 600.8 ppm	2003/23	Linde	17-Jul-25

Measured room conditions

Temperature : 22.7 °C Humidity : 62.6 %RH Pressure : 1010.5 mbar

Calibration conditions

Gas Temperature : 23 °C Flow rate : 1,300 ml/min Gas pressure : 1016.2 mbar

Calibration Results (Before adjustment) (Table 2)

Parameter of Standard	Standard Values	Mean of UUC	Error	Uncertainty (±)
O ₂ (%Vol)	2.50	2.46	-0.04	0.15
O ₂ (%Vol)	9.984	9.95	-0.034	0.20
O ₂ (%Vol)	21.02	21.08	0.06	0.30
CO (ppm)	80.45	81	0.55	3.0
CO (ppm)	302	302	0	6.0
CO (ppm)	1007	1010	3	12
NO ₂ (ppm)	30.68	26.9	-3.78	8.0
NO ₂ (ppm)	81.8	67.1	-14.7	8.0
NO ₂ (ppm)	202.6	181.3	-21.3	12
NO (ppm)	30.0	24	-6.0	8.0
NO (ppm)	151.8	145	-6.8	8.0
NO (ppm)	322.5	302	-20.5	12
SO ₂ (ppm)	50.36	48	-2.36	6.0
SO ₂ (ppm)	100.7	97	-3.7	6.0
SO ₂ (ppm)	600.8	589	-11.8	13

Calibration Results (After adjustment) (Table 3)

Parameter of Standard	Standard Values	Mean of UUC	Error	Uncertainty (±)
O2 (%Vol)	2.50	2.46	-0.04	0.15
O2 (%Vol)	9.984	9.95	-0.034	0.20
O2 (%Vol)	21.02	21.08	0.06	0.30
CO (ppm)	80.45	81	0.55	3.0
CO (ppm)	302	302	0	6.0
CO (ppm)	1007	1010	3	12
NO2 (ppm)	30.68	29.4	-1.28	8.0
NO2 (ppm)	81.8	79.7	-2.1	8.0
NO2 (ppm)	202.6	199.2	-3.4	12
NO (ppm)	30.0	30	0.0	8.0
NO (ppm)	151.8	153	1.2	8.0
NO (ppm)	322.5	324	1.5	12
SO2 (ppm)	50.36	50	-0.36	6.0
SO2 (ppm)	100.7	101	0.3	6.0
SO2 (ppm)	600.8	599	-1.8	13

Remark : 1 cmol/mol = 1 %vol. 1 μmol/mol = 1 ppm., Sensor CO New.

End of Report

Accredited by

NSC-TISI-TIS 17025

Calibration 0426



Calibration certificate

Calibration Certificate No. 26BCI0066

Object	Electronic non-automatic weighing instrument	This calibration certificate documents the traceability to national standards.
Manufacturer	Sartorius	Uncertainties of measurements are taken into account when only statements of compliance are made.
Type	MSU224S-100-DU	This certificate was prepared by Sartorius Corporation in accordance to the current ISO/IEC 17025:2017 standard and Sartorius Work Instruction (Method) SOP WI 08.
Serial QM Ident. no.	31709552 RYG_EN0003	This certificate relate and apply this equipment only.
Customer	ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)	
	616/10 Moo 5 T.Maenamkoo, A.Pluak Daeng, Rayong 21140, Thailand.	
Order no.	278579	REVIEW BY <i>Thanita K.</i>
Number of pages	4	APPROVED BY <i>D. J. J. J.</i>
Date of calibration	03 Feb 2026	NEXT CAL DATE..... 03/02/27

This calibration certificate may not be reproduced other than in full except with the permission of NSC-TISI-TIS-17025 and the issuing laboratory. Calibration certificates without signature are not valid.

The user is obliged to have the object recalibrated at appropriate intervals.

Date of issue	03 Feb 2026	Approval of the Calibration Certificate	Person in charge
		Mr. Chonchai Inthana	Chonchai Inthana

Calibration object

Single range instrument

Model	MSU224S-100-DU
Serial Number	31709552
QM Ident. no Inventory no.	RYG_EN0003 ---

Maximum capacity (Max. load)	220.0000 g
Measured up to	220.0000 g
Scale interval	0.0001 g

Place of calibration

Address	According to page 1
Department Cost center	Laboratory Department. ---
Building Floor	--- 1st Floor.
Room	Balance Room.
Maximum temperature variation at place of calibration	5 K

Calibration procedure

EURAMET Calibration Guide No. 18, Version 4.0 (11/2015) - Guidelines on the Calibration of Non-Automatic Weighing Instruments

Test equipment

Test equipment type	Test equipment ID	Valid until
Thermometer	Testo 174H H/T250743 (Traceable to Si unit through ENTECH)	18 Nov 2026
Test weight set OIML R111 E2	Certificate No.M2508149S ,E2(Traceable to SI unit through TCS)	19 Aug 2027

Adjustment Status

The measuring device was internally adjusted before the calibration.

Environmental and measuring conditions

Date of calibration	03 Feb 2026
Temperature at place of calibration Temp. diff. <i>T</i> _{weights} - <i>T</i> _{place}	24.5 °C 0.5 K
Measuring conditions	The installation site is suitable. The device is level. Balance was loaded up to Max before test.
Comments	Humidity 52.0 %RH.

Measurement results | Measurement uncertainties

Repeatability

Test load (nominal): 10 g 200 g		
	10 g	200 g
1	10.0000 g	200.0000 g
2	10.0000 g	200.0001 g
3	10.0000 g	200.0001 g
4	10.0001 g	200.0001 g
5	10.0000 g	200.0001 g
6	10.0000 g	200.0000 g
7	10.0000 g	200.0000 g
8	10.0000 g	200.0000 g
9	10.0000 g	200.0000 g
10	10.0000 g	200.0000 g
	<i>s</i> = 0.00003 g	<i>s</i> = 0.00005 g

Eccentricity

Test load (nominal): 100 g	
Center	100.0000 g
Front left	100.0000 g
Back left	99.9999 g
Back right	100.0000 g
Front right	100.0000 g
Maximum deviation from centric loading indication $ \Delta_{ecc} _{max} = 0.0001\text{ g}$	

Error of indication

Testload	Indication	Error	Expansion factor	Uncertainty	Uncertainty relative
<i>L</i>	<i>I</i>	<i>E</i>	<i>k</i>	<i>U</i> (<i>E</i>)	<i>U</i> _{rel} (<i>E</i>)
0.0100 g	0.0100 g	0.0000 g	2.00	0.00010 g	1.0 %
0.1000 g	0.1000 g	0.0000 g	2.00	0.00013 g	0.13 %
0.5000 g	0.5000 g	0.0000 g	2.00	0.00013 g	0.027 %
1.0000 g	1.0000 g	0.0000 g	2.00	0.00013 g	0.013 %
5.0000 g	5.0000 g	0.0000 g	2.00	0.00014 g	0.0027 %
10.0000 g	10.0000 g	0.0000 g	2.00	0.00014 g	0.0014 %
20.0000 g	20.0000 g	0.0000 g	2.00	0.00014 g	0.00071 %
50.0000 g	50.0001 g	0.0001 g	2.00	0.00015 g	0.00030 %
100.0000 g	100.0000 g	0.0000 g	2.00	0.00018 g	0.00018 %
200.0000 g	200.0000 g	0.0000 g	2.00	0.00028 g	0.00014 %
220.0000 g	220.0000 g	0.0000 g	2.00	0.00032 g	0.00015 %
Maximum error of indication		$ E _{max} = 0.0001\text{ g}$			

*U*_{rel}(*E*) is the quotient of *U*(*E*) and test load *L*. The uncertainty of measurement *U*(*E*) is valid only if error *E* is considered. You will find reference notes on the uncertainty of measurement in use under: Appendix to the calibration certificate | Interpretation of measurement results.
Reference note: The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the documented Expansion factor, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

End of calibration certificate

Uncertainty of measurement in use

Device adjusted before measurement	Yes
Temperature deviation considered	1.5 K (isoCAL active)
Temperature coefficient considered	$1 \cdot 10^{-6}/\text{K}$


Uncertainty of the weighing result $U_{gl}(W)$

$U_{gl}(W) = 0.00013 \text{ g} + 3.65 \cdot 10^{-6} \cdot R$

Reference note: The current uncertainty of measurement is calculated by entering of the reading R into this formula. In relation to this, there is no need for a correction of the indication error. The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied with an Expansion factor of 2, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

Indication in % from max load	Net indication R	Uncertainty $U_{gl}(W)$	Uncertainty relative $U_{gl}(W)_{rel}$
1 %	2.2000 g	0.00014 g	0.0063 %
25 %	55.0000 g	0.00033 g	0.00060 %
50 %	110.0000 g	0.00053 g	0.00048 %
75 %	165.0000 g	0.00073 g	0.00044 %
100 %	220.0000 g	0.00093 g	0.00042 %

Graphic realization of the relative uncertainty of measurement | process accuracy

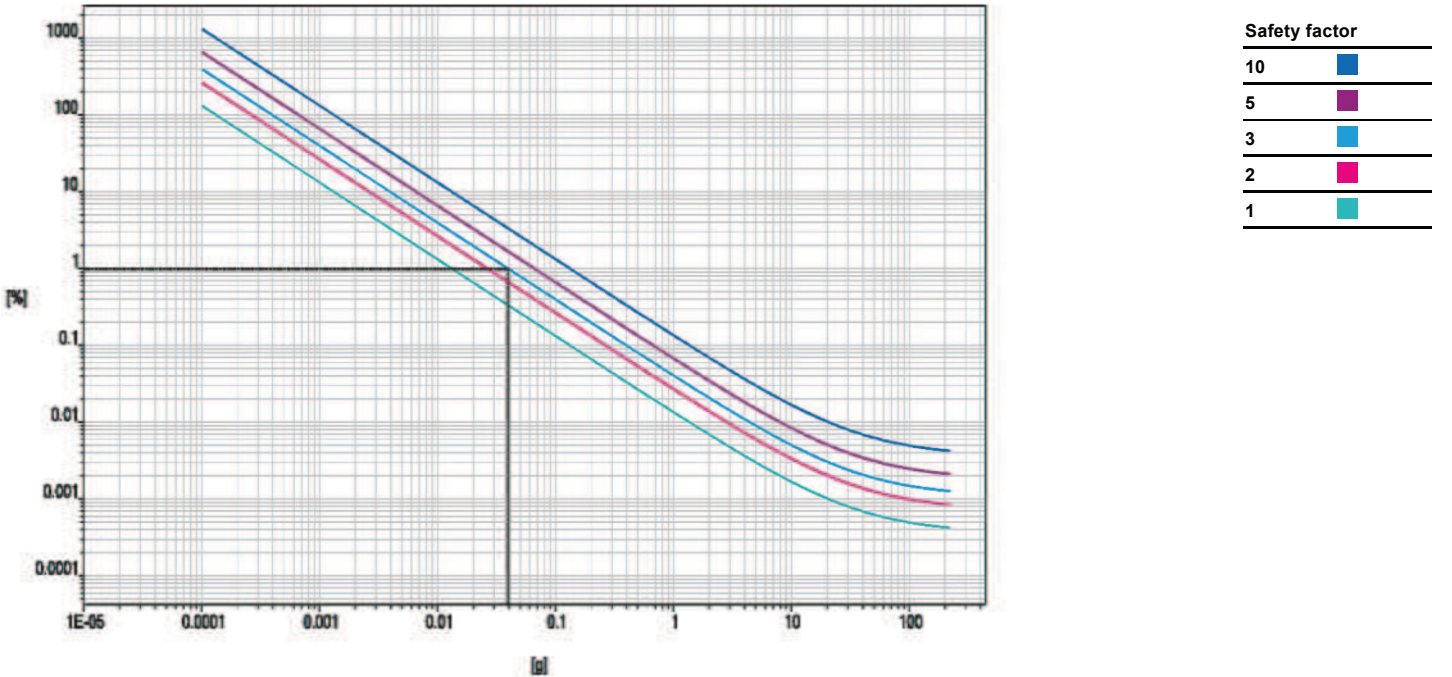


Displayed example

Process accuracy	1.00 %
Safety factor	3
Minimum sample weight	0.0395 g



Type S Pitot Tube Calibration

Date Calibration	6-Jan-26	Due Date	6-Jul-26
Pitot ID	BKK_FS0561	Inclinometer ID	BKK_FS1131
Pitot SN	-	Vernier ID	RYG_FS0539

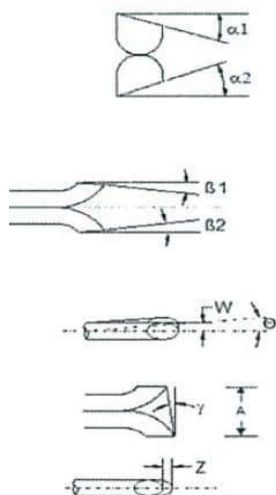

Parameter	Value	Allowable Range	Check
$\alpha 1$	0.4	$-10^{\circ} < \alpha 1 < +10^{\circ}$	OK
$\alpha 2$	0.2	$-10^{\circ} < \alpha 2 < +10^{\circ}$	OK
$\beta 1$	2	$-5^{\circ} < \beta 1 < +5^{\circ}$	OK
$\beta 2$	2.4	$-5^{\circ} < \beta 2 < +5^{\circ}$	OK
γ	1.4	-	-
θ	1.6	-	-
$Z = A \tan \gamma$	0.020	$Z \leq 0.125"$	OK
$W = A \tan \theta$	0.023	$W \leq 0.031"$	OK
Dt	0.320	0.188" to 0.375"	OK
$A/2Dt$	1.286	$1.05 \leq PA/Dt \leq 1.5$	OK
A	0.823	$2.1Dt \leq A \leq 3Dt$	OK

Certify that pitot tube/porbe meets or exceeds all specifications, criteria and/or applicable design features and is hereby assigned a pitot tube certification fact of 0.84 . See 40 CFR Pt. 60, App. A,EPA Method 2.

Calibrated by : Saksit Phaisanphisut
 (Mr. Saksit Phaisanphisut)
 RYG Field Services Scientist (4)

Approved By : Nattapol Jiengwareewong
 (Mr.Nattapol Jiengwareewong)
 RYG Field Services Specialist (1)



Certificate of Calibration

Customer

Name : ALS Laboratory Group Thailand Co., Ltd.
Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang, Bangkok
10250

Certificate No : 25-AFM-208

Request No : Req-2025-1986

Unit Under Calibration Details

Measurement Item : Air Flow Meter
Manufacturer : Mesa Labs
Model : 200-510M
Serial Number : 151114
ID : BKK_FS0614
Location of Calibration : LAB 4 AIR VELOCITY METER

Sensor Model : -
Sensor Serial Number : -
Instrument Status : Used

Calibration Environment and Details

Temperature : 23 °C ± 3 °C
Humidity : 55 %RH ± 20 %RH
Barometric Pressure : 1013 hPa ± 10 hPa
Received Date : 3 September 2025
Calibration Date : 10 September 2025
Calibration Procedure : In-house method CP-AFM-01 by Comparison technique with Standard Primary Flow Calibrator

REVIEW BY	<i>Narakon P.</i>
APPROVED BY	<i>[Signature]</i>
NEXT CAL DATE	09/09/26

Reference Standard	Model	Serial Number	Traceble	Due Calibration
Air Flow Meter	Gilibrator 3 Low flow	18501010006	Sensidyne	5 May 2026
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	6 May 2026
Temperature meter	GT 11	08000057	Qreborn	15 October 2025
Pressure meter	CPG2400	41000KDU/651882	TPA	21 October 2025

Traceability :

This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01 and MIT NSC-TISI-TIS Accreditation No. 0052

Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k = 2$, providing a level of confidence approximately 95 %.

Calibration By : *[Signature]*
Mr. Noppadon Luangart
Service Calibration Engineer

Approved By : *[Signature]*
Mr. Pacit Mathavorn
Calibration Engineer Supervisor

Issue Date : 10 September 2025



Certificate No : 25-AFM-208

Request No : Req-2025-1986

Result of Calibration : Without Adjustment

STD Reading			UUC Readingg			Error (cc/min)	Uncertainty		
Temperature (°C)	Pressure (kPa)	Flow (cc/min)	Temperature (°C)	Pressure (kPa)	Flow (cc/min)		(cc/min)	(°C)	(kPa)
25.5	100.98	100	-	-	100.02	0.0	3.6	1.0	0.50
25.7	100.97	503	-	-	500.81	-2.2	9.5	1.0	0.50
25.8	100.89	1003	-	-	1000.4	-3	19	1.0	0.50
26.1	100.88	2000	-	-	2001.9	2	38	1.0	0.50
26.5	100.85	3014	-	-	3002.2	-12	57	1.0	0.50
26.7	100.81	4027	-	-	4000.9	-26	76	1.0	0.50
27.0	100.74	5048	-	-	5001.8	-46	95	1.0	0.50

Note

STD : Standard UUC : Unit Under Calibration

- UUC Reference Condition : At atmospheric pressure and room temperature condition, Air ☐

- Flow Rate was corrected for non-standard operating condition by using equation :

$$Q_{meas} = Q_{ref} \times \frac{P_{ref}}{P_{meas}} \times \frac{T_{meas}}{T_{ref}}$$

where Q = Flow Rate P = Absolute Pressure T = Absolute Temperature

meas = Measurement Condition ref = Standard Condition

* Indicates non accredited

End of Certificate



Certificate of Calibration

Customer

Name : ALS Laboratory Group Thailand Co., Ltd.
Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang, Bangkok
10250

Certificate No : 25-AFM-207

Request No : Req-2025-1987

Unit Under Calibration Details

Measurement Item : Air Flow Meter
Manufacturer : Mesa Labs
Model : 200-510L
Serial Number : 130026
ID : BKK_FS0619
Location of Calibration : LAB 4 AIR VELOCITY METER

Sensor Model : -

Sensor Serial Number : -

Instrument Status : Used

Calibration Environment and Details

Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$
Humidity : $55\% \text{RH} \pm 20\% \text{RH}$
Barometric Pressure : $1013 \text{ hPa} \pm 10 \text{ hPa}$
Received Date : 3 September 2025
Calibration Date : 10 September 2025
Calibration Procedure : In-house method CP-AFM-01 by Comparison technique with Standard Primary Flow Calibrator

REVIEW BY *Manakorn P.*

APPROVED BY *[Signature]*

NEXT CAL DATE 09/09/26

Reference Standard	Model	Serial Number	Traceable	Due Calibration
Air Flow Meter	Gilibrator 3 Low flow	18501010006	Sensidyne	5 May 2026
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	6 May 2026
Temperature meter	GT 11	08000057	Qreborn	15 October 2025
Pressure meter	CPG2400	41000KDU/651882	TPA	21 October 2025

Traceability :

This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01 and MIT NSC-TISI-TIS Accreditation No. 0052

Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k = 2$, providing a level of confidence approximately 95 %.

Calibration By :

[Signature]
Mr. Noppadon Luangart
Service Calibration Engineer

Approved By :

[Signature]
Mr. Pacit Mathavorn
Calibration Engineer Supervisor

Issue Date : 10 September 2025

Certificate No : 25-AFM-207

Request No : Req-2025-1987

Result of Calibration : Without Adjustment

STD Reading			UUC Readingg			Error (cc/min)	Uncertainty		
Temperature (°C)	Pressure (kPa)	Flow (cc/min)	Temperature (°C)	Pressure (kPa)	Flow (cc/min)		(cc/min)	(°C)	(kPa)
25.5	100.98	20	-	-	20.042	0.0	1.6	1.0	0.50
25.5	100.90	50	-	-	49.921	-0.1	4.0	1.0	0.50
25.5	100.91	100	-	-	100.09	0.1	3.6	1.0	0.50
25.4	100.86	150	-	-	150.34	0.3	5.4	1.0	0.50
25.6	100.93	199	-	-	200.17	1.2	7.2	1.0	0.50
25.6	100.95	301	-	-	300.05	-1	11	1.0	0.50
25.7	100.96	402	-	-	401.03	-1	14	1.0	0.50
25.7	100.95	503	-	-	500.26	-3	10	1.0	0.50

Note

STD : Standard UUC : Unit Under Calibration

- UUC Reference Condition : At atmospheric pressure and room temperature condition, Air ☐
- Flow Rate was corrected for non-standard operating condition by using equation :

$$Q_{meas} = Q_{ref} \times \frac{P_{ref}}{P_{meas}} \times \frac{T_{meas}}{T_{ref}}$$

where Q = Flow Rate P = Absolute Pressure T = Absolute Temperature
 meas = Measurement Condition ref = Standard Condition

* Indicates non accredited

End of Certificate



Certificate of Calibration

Certificate No. C-040126-RYG_FS0131

Air Sampling Pump Detail

Equipment name : Personal Air Sampling Pump
Brand : Gilian
Model/Type : GilAir Plus

Equipment ID : RYG_FS0131
Serial No. : 20150410007
Calibration Date : 04-Jan-26
Next calibration date : 04-Apr-26

Reference Standard Low Flow Meter

Equipment name : Air Flow Meter
Brand : MesaLabs
Model/Type : Defender 510-L

Equipment ID : BKK_FS0619
Serial No. : 130026
Calibration Date : 10-Sep-25
Due Date : 9-Sep-26

Reference Standard High Flow Meter

Equipment name : Air Flow Meter
Brand : MesaLabs
Model/Type : Defender 510-M

Equipment ID : BKK_FS0614
Serial No. : 151114
Calibration Date : 10-Sep-25
Due Date : 09-Sep-26

Calibration Data

Air Sampling Pump setting (cc/min)	Reference Std. Flow Reading (cc/min)			Avg. (cc/min)	%Error acceptance	Acceptable range (cc/min)	Evaluation (Pass/ Fail)
	1	2	3				
Low Flow							
20	19.9	20.1	20.1	20.0	5%	19 - 21	Passed
50	51.0	51.0	50.9	51.0	5%	48 - 53	Passed
100	99.4	99.2	98.5	99.0	5%	95 - 105	Passed
200	199.0	198.7	198.9	198.9	5%	190 - 210	Passed
High Flow							
500	503.3	501.3	502.1	502.2	3%	485 - 515	Passed
1000	1003.9	1003.3	1000.7	1002.6	3%	970 - 1030	Passed
2000	1999.3	1997.1	1998.3	1998.2	3%	1940 - 2060	Passed
2500	2499.8	2499.6	2499.7	2499.7	3%	2425 - 2575	Passed

----- END OF REPORT -----

Calibrated By: 

(Mr. Watcharin Pongsamsuan)
RYG Field Services Scientist (1)

Issue date : 05-Jan-26

Approved By: 

(Mr. Supot Salamteh)
Field Services Section Head



Certificate of Calibration

Certificate No. C-060126-RYG_FS0107

Air Sampling Pump Detail

Equipment name : Personal Air Sampling Pump
Brand : Gilian
Model/Type : GilAir PlusEquipment ID : RYG_FS0107
Serial No. : 20150210174
Calibration Date : 06-Jan-26
Next calibration date : 06-Apr-26

Reference Standard Low Flow Meter

Equipment name : Air Flow Meter
Brand : MesaLabs
Model/Type : Defender 510-LEquipment ID : BKK_FS0619
Serial No. : 130026
Calibration Date : 10-Sep-25
Due Date : 09-Sep-26

Reference Standard High Flow Meter

Equipment name : Air Flow Meter
Brand : MesaLabs
Model/Type : Defender 510-MEquipment ID : BKK_FS0614
Serial No. : 151114
Calibration Date : 10-Sep-25
Due Date : 09-Sep-26

Calibration Data

Air Sampling Pump setting (cc/min)	Reference Std. Flow Reading (cc/min)			Avg. (cc/min)	%Error acceptance	Acceptable range (cc/min)	Evaluation (Pass/ Fail)
	1	2	3				
Low Flow							
20	19.4	19.4	19.2	19.3	5%	19 - 21	Passed
50	52.1	51.9	51.3	51.8	5%	48 - 53	Passed
100	102.3	101.6	102.3	102.1	5%	95 - 105	Passed
200	202.6	202.1	202.6	202.4	5%	190 - 210	Passed
High Flow							
500	507.3	507.9	508.9	508.0	3%	485 - 515	Passed
1000	1005.4	997.2	999.9	1000.8	3%	970 - 1030	Passed
2000	2000.4	2014.1	2008.1	2007.5	3%	1940 - 2060	Passed
2500	2496.2	2506.7	2506.5	2503.1	3%	2425 - 2575	Passed

----- END OF REPORT -----

Calibrated By: นันทapon

(Mr. Natchapon Thamklang)

RYG Field Services Scientist (1)

Issue date : 07-Jan-26

Approved By: Supot S

(Mr. Supot Salamteh)

Field Services Section Head

Certificate of System Qualification

GC-OQ + GCMS-OQ

System ID: GM-12
Organization Name: ALS Laboratory Groups (Thailand) Co Ltd.
Organization Location: 104 Phattanakan 40 Phattanakan Rd Bangkok 10250

Date: May 9, 2025 3:29:14 PM
EQP Name: AgilentRecommended , AgilentRecommended

EQP Revision: GC.02.53, GCMS.02.54
Overall Qualification Status: Pass

REVIEW BY Suchada T.
APPROVED BY Tanyatorn M.
NEXT CAL. DATE 9 May 26.

CDS Logon Verification - GC

Logon: asbkk.env03

Overall CDS Logon Verification - GC Test Status

Pass

System Inspection and Basic Safety and Operation

Name: 8890
Setpoint Status: Pass

Overall System Inspection and Basic Safety and Operation Test Status

Pass

Inlet Pressure Accuracy

Name: 8890
Front SSL

Setpoint Status: Pass

Setpoint Actual
Inlet Pressure: 25.0 psi 24.8 psi
Accuracy: 0.2 psi
Agilent Recommended: <= 1.2

Date: May 9, 2025 3:29:14 PM
System ID: GM-12

Overall Inlet Pressure Accuracy Test Status

Pass

GC Oven Temperature Accuracy

Name: 8890

Setpoint Status: Pass

Zone: Oven

Setpoint/Actual

Temperature: 230.0 230.1 °C

Accuracy: 0.1 °C

Agilent Recommended: ≥ -1.0 % setpoint in K (-5.0 °C)
 ≤ 1.0 % setpoint in K (5.0 °C)

Setpoint Status: Pass

Zone: Oven

Setpoint/Actual

Temperature: 100.0 100.1 °C

Accuracy: 0.1 °C

Agilent Recommended: ≥ -1.0 % setpoint in K (-3.7 °C)
 ≤ 1.0 % setpoint in K (3.7 °C)

Overall GC Oven Temperature Accuracy Test Status

Pass

GC Oven Temperature Stability

Name: 8890

Setpoint Status: Pass

Setpoint/Average

Temperature: 100.0 100.1167 °C

Stability: 0.1 °C

Agilent Recommended: ≤ 0.5

Overall GC Oven Temperature Stability Test Status

Pass

Log Amp

Tested Combination1 Front SSL / External SQ

Name: 5977C

Setpoint Status: Pass

Overall Log Amp Test StatusPass

RFPA

Tested Combination1 Front SSL / External SQ

Name: 5977C

Setpoint Status: Pass

Amu: 1050 m/z

Drift After Five Minutes:

RFPA Voltage:

Agilent Recommended:

1 mV
≥ -100

and

≤ 100

497 mV
≤ 1100**Overall RFPA Test Status**Pass

Tune EI

Tested Combination1 Front SSL / External SQ

Name: 5977C

Setpoint Status: Pass

Filament: 1

Setpoint Status: Pass

Filament: 2

Overall Tune EI Test StatusPass

Scouting Run

Date: May 9, 2025 3:29:14 PM
System ID: GM-12

Tested Combination1 Front SSL / External SQ

Injection Tower

Name: 7693A

Source: EI - Extractor

Setpoint Status: Completed

Injection Volume on Column: 1.0 uL

Overall Scouting Run Status

Completed

Instrument Detection Limit

Tested Combination1 Front SSL / External SQ

Injection Tower

Name: 7693A

Source: EI - Extractor

Setpoint Status: Pass

Injection Volume on Column: 1.0 uL

Area

Minimum RSD: 1.27 %

Agilent Recommended: <= 5.00

Status: Pass

Retention Time

0.01 %

<= 1.00

Pass

Instrument Detection Limit: 4.28135 fg

Agilent Recommended: <= 16.82500

Status: Pass

Overall Instrument Detection Limit Test Status

Pass

Mass Ratio Precision

Tested Combination1	Front	SSL	/ External	SQ
	Injection Tower			
Name:	7693A			
Source:	EI - Extractor			
Setpoint Status:	Pass			
Injection Volume on Column:	1.0	uL		
	Area Mass 1		Mass Ratio	
	Abundance*s			
RSD:	2.17	%	0.50	%
Agilent Recommended:	<= 5.00		<= 5.00	
	Pass		Pass	

Overall Mass Ratio Precision Test Status

Pass

NOTE: This test's 1 comment(s) and 0 deviation(s) are available in the Attachments section.

Instrument Details

Purpose

This section describes the as found system configuration.

Details

Tested Combination1	
Injection Technique	Injection Tower
Inlet	Front
Detector	External
LTM Included?	No
Sampler 1	
Manufacturer	Agilent Technologies
Type	Injection Tower
Name	7693A
Model Number	G4513A
Serial Number	CN23125102
Firmware Revision	A.11.07
Usage	Sample Injection
Location	Front
Syringe Volume (µL)	10
Sampler 2	
Manufacturer	Agilent Technologies
Type	Tray
Name	7693A
Model Number	G4514A
Serial Number	CN23147049
Firmware Revision	A.12.03
Vial Heater	Not installed

Mainframe 1

Manufacturer	Agilent Technologies
Name	8890
Model Number	G3540A
Serial Number	CN2303A031
Firmware Revision	2.8.1.6
Oven Type	Standard

Inlet 1

Manufacturer	Agilent Technologies
Name	8890
Type	SSL
Location	Front
Carrier Gas	Helium
Control Type	Electronic Pressure Control (EPC)
Purged Inlet	Yes

Mass Spectrometer 1

Manufacturer	Agilent Technologies
Type	SQ
Name	5977C
Model Number	G7077C
Serial Number	US2307MA35
Firmware Revision	6.00.35
Rough Pump	Wet Mechanical Vacuum Pump
High Vacuum System	Turbo Pump
Scouting Run Standard	OFN Std

Electronic Signature

Purpose

This signature page was created and published because the ACE sign-off action was executed, which is valid for the entire document, including attachments. The ACE sign-off is an electronic signature that requires two distinct identification components: unique username and personal password. The Agilent representative who has delivered this service understands the meaning and legal status of an electronic signature. As a trained official operator, the Agilent representative has a unique password and logon to access ACE and electronically sign this document. (Other e-signatures can be applied to this document using a Document Content Management or other suitable method defined in your data access and control procedures.)

Details

Full Name of Signer:	Phuwanai Yoktragul
Logged On User Name:	phuwanai.yoktragul@agilent.com
Signature Creation Date:	May 9, 2025
Reason for Signature:	Executed protocol and published this original version of document

ACE Self Qualification Status

The installed version of ACE used to deliver this service passed qualification; the results conform with expected values. The self qualification summary report is available in the session folder location SDS\ClearStore\AceSelfQualification.

Regulatory Disclaimer

This document provides a protocol to verify and record instrument configuration and evidence of proper operation. It has been prepared from our interpretation of applicable regulations as well as industry best practices. The document is designed to provide an important component of a complete compliance package. Validation depends upon many factors and use of this protocol alone does not assure compliance. Agilent Technologies makes no promises or representations as to its sufficiency for any specific regulatory program.

Warranty

Agilent Technologies makes no warranty of any kind to this material, including but not limited to, the implied warranties or merchantability and fitness for a particular purpose. Agilent Technologies shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance, or use of this material.

User Name: phuwanai.yoktragul
Report Generated by Hostname: 5CG9217CJG

System Id: GM-12
Print Date: May 9, 2025 3:29:17 PM

OQ2025_GM-12 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
May 8, 2025 2:38:52 PM	Audit	SessionCreated	Session	Host Name: 5CG9217CJG, Drive Serial Number: BC4F1A47
May 8, 2025 2:38:52 PM	start	Configuration	Session	None
May 8, 2025 2:38:52 PM	Audit	Entitlement	Licensing	User is FieldEngineer and does not require an unlock code
May 8, 2025 2:41:01 PM	Audit	EqpLoaded	Session	EQP details for primary technique [Gc] - File path: [ProtocolPacks/Gc/Configurat ions/02.53/Gc.02.53.eqp], EQP File Name: [Gc.02.53.eqp], EQP Name: [AgilentRecommended],Proto col Revision :[Gc.02.53] EQP details for hyphenated technique [GcMs] - File path: [ProtocolPacks/GcMs/Config urations/02.54/GcMs.02.54.e qp], EQP File Name: [GcMs.02.54.eqp], EQP Name: [AgilentRecommended]
May 8, 2025 2:41:05 PM	End	Configuration	Session	None
May 8, 2025 2:41:09 PM	start	Qualification	Session	OQ
May 8, 2025 2:41:10 PM	start	Execution	CDS Logon Verification - GC - 8890: - Qualitative test	None
May 8, 2025 2:42:42 PM	End	Execution	CDS Logon Verification - GC - 8890: - Qualitative test	Run Count : 1

User Name: phuwanai.yoktragul
Report Generated by Hostname: 5CG9217CJG

System Id: GM-12
Print Date: May 9, 2025 3:29:17 PM

OQ2025_GM-12 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
May 8, 2025 2:43:00 PM	start	Execution	System Inspection and Basic Safety and Operation - 8890: - Qualitative Test - No setpoints associated	None
May 8, 2025 2:43:16 PM	End	Execution	System Inspection and Basic Safety and Operation - 8890: - Qualitative Test - No setpoints associated	Run Count : 1
May 8, 2025 2:43:21 PM	start	Execution	Inlet Pressure Accuracy - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	None
May 8, 2025 2:44:22 PM	End	Execution	Inlet Pressure Accuracy - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	Run Count : 1
May 8, 2025 2:44:28 PM	start	Execution	GC Oven Temperature Accuracy - 8890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
May 8, 2025 2:52:02 PM	Audit	Data	GC Oven Temperature Accuracy - 8890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry
May 8, 2025 2:52:05 PM	End	Execution	GC Oven Temperature Accuracy - 8890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1
May 8, 2025 2:52:13 PM	start	Execution	GC Oven Temperature Accuracy - 8890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
May 8, 2025 3:01:36 PM	Audit	Data	GC Oven Temperature Accuracy - 8890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry

User Name: phuwanai.yoktragul
Report Generated by Hostname: 5CG9217CJG

System Id: GM-12
Print Date: May 9, 2025 3:29:17 PM

OQ2025_GM-12 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
May 8, 2025 3:01:39 PM	End	Execution	GC Oven Temperature Accuracy - 8890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1
May 8, 2025 3:01:42 PM	start	Execution	GC Oven Temperature Stability - 8890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	None
May 8, 2025 3:20:17 PM	Audit	Data	GC Oven Temperature Stability - 8890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Manual Data Entry
May 8, 2025 3:20:19 PM	End	Execution	GC Oven Temperature Stability - 8890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Run Count : 1
May 8, 2025 3:20:42 PM	start	Execution	Log Amp - 5977C SQ: - Source: EI - Extractor	None
May 8, 2025 3:25:45 PM	End	Execution	Log Amp - 5977C SQ: - Source: EI - Extractor	Run Count : 1
May 8, 2025 3:25:48 PM	start	Execution	RFP - 5977C SQ: - Source: EI - Extractor	None
May 8, 2025 3:36:10 PM	End	Execution	RFP - 5977C SQ: - Source: EI - Extractor	Run Count : 1
May 8, 2025 3:36:50 PM	start	Execution	Tune EI - 5977C SQ: - Source: EI - Extractor Filament 1 (Qualitative - No setpoints associated)	None
May 8, 2025 3:43:21 PM	End	Execution	Tune EI - 5977C SQ: - Source: EI - Extractor Filament 1 (Qualitative - No setpoints associated)	Run Count : 1
May 8, 2025 3:43:27 PM	start	Execution	Tune EI - 5977C SQ: - Source: EI - Extractor Filament 2 (Qualitative - No setpoints associated)	None

Page 3 / 10

User Name: phuwanai.yoktragul
Report Generated by Hostname: 5CG9217CJG

System Id: GM-12
Print Date: May 9, 2025 3:29:17 PM

OQ2025_GM-12 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
May 8, 2025 3:45:57 PM	End	Execution	Tune EI - 5977C SQ: - Source: - Run Count : 1 EI - Extractor Filament 2 (Qualitative - No setpoints associated)	
May 8, 2025 3:46:04 PM	Audit	AceClosed	Session	None
May 9, 2025 9:33:04 AM	Audit	AceRestarted	Session	Host Name: 5CG9217CJG, Drive Serial Number: BC4F1A47
May 9, 2025 9:33:06 AM	Audit	SessionReloaded	Session	None
May 9, 2025 9:33:59 AM	start	Qualification	Session	OQ
May 9, 2025 9:34:19 AM	start	Execution	Scouting Run - Injection Tower, Front SSL, SQ: - Source: - EI - Extractor- Part of GCMS System Preparation	None
May 9, 2025 9:35:36 AM	start	Execution	Instrument Detection Limit - Injection Tower, Front SSL, SQ: - Source: - EI - Extractor - RSD L (Area): <= 5.00% - RSD L (Ret. Time): <= 1.00%	None
May 9, 2025 9:39:00 AM	start	Execution	Scouting Run - Injection Tower, Front SSL, SQ: - Source: - EI - Extractor- Part of GCMS System Preparation	None
May 9, 2025 9:39:03 AM	start	Execution	Mass Ratio Precision - Injection Tower, Front SSL, SQ: - Source: EI - Extractor - L (RSD): <= 5.00%	None
May 9, 2025 9:43:57 AM	start	Execution	Scouting Run - Injection Tower, Front SSL, SQ: - Source: - EI - Extractor- Part of GCMS System Preparation	None

User Name: phuwanai.yoktragul

System Id: GM-12

Report Generated by Hostname: 5CG9217CJG

Print Date: May 9, 2025 3:29:17 PM

OQ2025_GM-12 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
May 9, 2025 10:04:26 AM	start	Execution	Instrument Detection Limit - Injection Tower, Front SSL, SQ: - Source: - EI - Extractor - RSD L (Area): <= 5.00% - RSD L (Ret. Time): <= 1.00%	None
May 9, 2025 10:04:28 AM	start	Execution	Scouting Run - Injection Tower, Front SSL, SQ: - Source: - EI - Extractor- Part of GCMS System Preparation	None
May 9, 2025 1:12:30 PM	start	Execution	Mass Ratio Precision - Injection Tower, Front SSL, SQ: - Source: EI - Extractor - L (RSD): <= 5.00%	None
May 9, 2025 3:02:09 PM	start	Execution	Scouting Run - Injection Tower, Front SSL, SQ: - Source: - EI - Extractor- Part of GCMS System Preparation	None
May 9, 2025 3:03:52 PM	Audit	Data	Scouting Run - Injection Tower, Front SSL, SQ: - Source: - EI - Extractor- Part of GCMS System Preparation	Data files Path : C:\Users\yoktragul\Downloads\ALS_OQ2025\OQ2025\SC_OFN.D
May 9, 2025 3:04:25 PM	Audit	Reporting	Reintegration	Reintegration Count: 1 -- [Integration Type: Injection; Baseline Correction Mode: Advanced; Initial Slope Sensitivity: 10; Initial Peak Width: 0.01; Initial Area Reject: 0; Initial Height Reject: 150; Integration: Off at 0; Integration: On at 4]

User Name: phuwanai.yoktragul
Report Generated by Hostname: 5CG9217CJG

System Id: GM-12
Print Date: May 9, 2025 3:29:17 PM

OQ2025_GM-12 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
May 9, 2025 3:04:39 PM	Audit	Reporting	Reintegration	Reintegration Count: 2 -- [Integration Type: Injection; Baseline Correction Mode: Advanced; Initial Slope Sensitivity: 10; Initial Peak Width: 0.01; Initial Area Reject: 0; Initial Height Reject: 100; Integration: Off at 0; Integration: On at 4]
May 9, 2025 3:04:46 PM	Audit	Reporting	Reintegration	Reintegration Count: 3 -- [Integration Type: Injection; Baseline Correction Mode: Advanced; Initial Slope Sensitivity: 10; Initial Peak Width: 0.02; Initial Area Reject: 0; Initial Height Reject: 100; Integration: Off at 0; Integration: On at 4]
May 9, 2025 3:05:17 PM	End	Execution	Scouting Run - Injection Tower, Front SSL, SQ: - Source: - EI - Extractor- Part of GCMS System Preparation	Run Count : 1
May 9, 2025 3:05:21 PM	start	Execution	Instrument Detection Limit - Injection Tower, Front SSL, SQ: - Source: - EI - Extractor - RSD L (Area): <= 5.00% - RSD L (Ret. Time): <= 1.00%	None
May 9, 2025 3:07:51 PM	Audit	Data	Instrument Detection Limit - Injection Tower, Front SSL, SQ: - Source: - EI - Extractor - RSD L (Area): <= 5.00% - RSD L (Ret. Time): <= 1.00%	Data files Path : C:\Users\yoktragu\Downloads\ALS_OQ2025\OQ2025\OQ2025\IDL2.D

User Name: phuwanai.yoktragul
Report Generated by Hostname: 5CG9217CJG

System Id: GM-12
Print Date: May 9, 2025 3:29:17 PM

OQ2025_GM-12 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
May 9, 2025 3:07:51 PM	Audit	Data	Instrument Detection Limit - Injection Tower, Front SSL, SQ: - Source: - EI - Extractor - RSD L (Area): <= 5.00% - RSD L (Ret. Time): <= 1.00%	Data files Path : C:\Users\yoktragul\Downloads VALS_OQ2025\OQ2025\OQ2025\IDL3.D
May 9, 2025 3:07:51 PM	Audit	Data	Instrument Detection Limit - Injection Tower, Front SSL, SQ: - Source: - EI - Extractor - RSD L (Area): <= 5.00% - RSD L (Ret. Time): <= 1.00%	Data files Path : C:\Users\yoktragul\Downloads VALS_OQ2025\OQ2025\OQ2025\IDL4.D
May 9, 2025 3:07:51 PM	Audit	Data	Instrument Detection Limit - Injection Tower, Front SSL, SQ: - Source: - EI - Extractor - RSD L (Area): <= 5.00% - RSD L (Ret. Time): <= 1.00%	Data files Path : C:\Users\yoktragul\Downloads VALS_OQ2025\OQ2025\OQ2025\IDL5.D
May 9, 2025 3:07:51 PM	Audit	Data	Instrument Detection Limit - Injection Tower, Front SSL, SQ: - Source: - EI - Extractor - RSD L (Area): <= 5.00% - RSD L (Ret. Time): <= 1.00%	Data files Path : C:\Users\yoktragul\Downloads VALS_OQ2025\OQ2025\OQ2025\IDL6.D
May 9, 2025 3:07:51 PM	Audit	Data	Instrument Detection Limit - Injection Tower, Front SSL, SQ: - Source: - EI - Extractor - RSD L (Area): <= 5.00% - RSD L (Ret. Time): <= 1.00%	Data files Path : C:\Users\yoktragul\Downloads VALS_OQ2025\OQ2025\OQ2025\IDL7.D
May 9, 2025 3:07:51 PM	Audit	Data	Instrument Detection Limit - Injection Tower, Front SSL, SQ: - Source: - EI - Extractor - RSD L (Area): <= 5.00% - RSD L (Ret. Time): <= 1.00%	Data files Path : C:\Users\yoktragul\Downloads VALS_OQ2025\OQ2025\OQ2025\IDL8.D
May 9, 2025 3:07:51 PM	Audit	Data	Instrument Detection Limit - Injection Tower, Front SSL, SQ: - Source: - EI - Extractor - RSD L (Area): <= 5.00% - RSD L (Ret. Time): <= 1.00%	Data files Path : C:\Users\yoktragul\Downloads VALS_OQ2025\OQ2025\OQ2025\IDL9.D

Page 7 / 10

User Name: phuwanai.yoktragul
Report Generated by Hostname: 5CG9217CJG

System Id: GM-12
Print Date: May 9, 2025 3:29:17 PM

OQ2025_GM-12 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
May 9, 2025 3:07:51 PM	Audit	Data	Instrument Detection Limit - Injection Tower, Front SSL, SQ: - Source: - EI - Extractor - RSD L (Area): <= 5.00% - RSD L (Ret. Time): <= 1.00%	Data files Path : C:\Users\yoktragul\Downloads VALS_OQ2025\OQ2025\OQ2 025\IDL10.D
May 9, 2025 3:07:51 PM	Audit	Data	Instrument Detection Limit - Injection Tower, Front SSL, SQ: - Source: - EI - Extractor - RSD L (Area): <= 5.00% - RSD L (Ret. Time): <= 1.00%	Data files Path : C:\Users\yoktragul\Downloads VALS_OQ2025\OQ2025\OQ2 025\IDL11.D
May 9, 2025 3:08:43 PM	Audit	Reporting	Reintegration	Reintegration Count: 1 -- [Integration Type: Injection;Baseline Correction Mode: Advanced;Initial Slope Sensitivity: 10;Initial Peak Width: 0.01;Initial Area Reject: 0;Initial Height Reject: 50;Integration: Off at 0;Integration: On at 4.6]
May 9, 2025 3:09:07 PM	Audit	Reporting	Reintegration	Reintegration Count: 2 -- [Integration Type: Injection;Baseline Correction Mode: Advanced;Initial Slope Sensitivity: 10;Initial Peak Width: 0.01;Initial Area Reject: 0;Initial Height Reject: 200;Integration: Off at 0;Integration: On at 4.6]
May 9, 2025 3:10:29 PM	End	Execution	Instrument Detection Limit - Injection Tower, Front SSL, SQ: - Source: - EI - Extractor - RSD L (Area): <= 5.00% - RSD L (Ret. Time): <= 1.00%	Run Count : 1

User Name: phuwanai.yoktragul

System Id: GM-12

Report Generated by Hostname: 5CG9217CJG

Print Date: May 9, 2025 3:29:17 PM

OQ2025_GM-12 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
May 9, 2025 3:11:01 PM	start	Execution	Mass Ratio Precision - Injection Tower, Front SSL, SQ: - Source: EI - Extractor - L (RSD): ≤ 5.00%	None
May 9, 2025 3:12:51 PM	Audit	Data	Mass Ratio Precision - Injection Tower, Front SSL, SQ: - Source: EI - Extractor - L (RSD): ≤ 5.00%	Data files Path : C:\Users\yoktragu\Downloads VALS_OQ2025\OQ2025\OQ2 025\MRP5.D
May 9, 2025 3:12:51 PM	Audit	Data	Mass Ratio Precision - Injection Tower, Front SSL, SQ: - Source: EI - Extractor - L (RSD): ≤ 5.00%	Data files Path : C:\Users\yoktragu\Downloads VALS_OQ2025\OQ2025\OQ2 025\MRP6.D
May 9, 2025 3:12:51 PM	Audit	Data	Mass Ratio Precision - Injection Tower, Front SSL, SQ: - Source: EI - Extractor - L (RSD): ≤ 5.00%	Data files Path : C:\Users\yoktragu\Downloads VALS_OQ2025\OQ2025\OQ2 025\MRP7.D
May 9, 2025 3:12:51 PM	Audit	Data	Mass Ratio Precision - Injection Tower, Front SSL, SQ: - Source: EI - Extractor - L (RSD): ≤ 5.00%	Data files Path : C:\Users\yoktragu\Downloads VALS_OQ2025\OQ2025\OQ2 025\MRP8.D
May 9, 2025 3:12:51 PM	Audit	Data	Mass Ratio Precision - Injection Tower, Front SSL, SQ: - Source: EI - Extractor - L (RSD): ≤ 5.00%	Data files Path : C:\Users\yoktragu\Downloads VALS_OQ2025\OQ2025\OQ2 025\MRP9.D
May 9, 2025 3:12:51 PM	Audit	Data	Mass Ratio Precision - Injection Tower, Front SSL, SQ: - Source: EI - Extractor - L (RSD): ≤ 5.00%	Data files Path : C:\Users\yoktragu\Downloads VALS_OQ2025\OQ2025\OQ2 025\MRP10.D

Page 9 / 10

User Name: phuwanal.yoktragul
Report Generated by Hostname: 5CG9217CJG

System Id: GM-12
Print Date: May 9, 2025 3:29:17 PM

OQ2025_GM-12 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
May 9, 2025 3:13:49 PM	Audit	Reporting	Reintegration	Reintegration Count: 1 -- [Integration Type: Injection; Baseline Correction Mode: Advanced; Initial Slope Sensitivity: 10; Initial Peak Width: 0.01; Initial Area Reject: 0; Initial Height Reject: 50000; Integration: Off at 0; Integration: On at 2]
May 9, 2025 3:15:04 PM	End	Execution	Mass Ratio Precision - Injection Tower, Front SSL, SQ: - Source: EI - Extractor - L (RSD): <= 5.00%	Run Count : 1
May 9, 2025 3:16:15 PM	End	Qualification	Session	OQ
May 9, 2025 3:16:15 PM	start	Reporting	Session	None
May 9, 2025 3:26:19 PM	Audit	Reporting	Session	Report Generated : Certificate
May 9, 2025 3:27:20 PM	Audit	Reporting	Session	Report Generated : Report
May 9, 2025 3:28:25 PM	Audit	Reporting	Session	Report Generated : Report with Certificate



Certificate of Calibration

Certificate No. C-070126-RYG_FS0122

Air Sampling Pump Detail

Equipment name : Personal Air Sampling Pump
Brand : Gilian
Model/Type : GilAir Plus

Equipment ID : RYG_FS0122
Serial No. : 20220731510
Calibration Date : 07-Jan-26
Next calibration date : 07-Apr-26

Reference Standard Low Flow Meter

Equipment name : Air Flow Meter
Brand : MesaLabs
Model/Type : Defender 510-L

Equipment ID : BKK_FS0619
Serial No. : 130026
Calibration Date : 10-Sep-25
Due Date : 9-Sep-26

Reference Standard High Flow Meter

Equipment name : Air Flow Meter
Brand : MesaLabs
Model/Type : Defender 510-M

Equipment ID : BKK_FS0614
Serial No. : 151114
Calibration Date : 10-Sep-25
Due Date : 09-Sep-26

Calibration Data

Air Sampling Pump setting (cc/min)	Reference Std. Flow Reading (cc/min)			Avg. (cc/min)	%Error acceptance	Acceptable range (cc/min)		Evaluation (Pass/ Fail)	
	1	2	3						
Low Flow									
20	20.3	20.4	20.8	20.5	5%	19	-	21	Passed
50	50.2	50.3	50.4	50.3	5%	48	-	53	Passed
100	100.8	100.9	101.5	101.1	5%	95	-	105	Passed
200	200.8	200.6	201.5	201.0	5%	190	-	210	Passed
High Flow									
500	503.4	502.0	502.7	502.7	3%	485	-	515	Passed
1000	996.8	1004.5	1013.5	1004.9	3%	970	-	1030	Passed
2000	2002.7	2004.3	2008.4	2005.1	3%	1940	-	2060	Passed
2500	2495.7	2507.3	2493.3	2498.8	3%	2425	-	2575	Passed

----- END OF REPORT -----

Calibrated By: 

(Mr. Watcharin Pongsamsuan)

RYG Field Services Scientist (1)

Issue date : 08-Jan-26

Approved By: 

(Mr. Supot Salamteh)

Field Services Section Head




CALIBRATION REPORT

Calibration Date	5-Jan-26	Equipment ID	BKK_FS0758
Equipment Name	FID Analyzer	Manufacturer	Baseline Mocon
Model	9000H	Serial No.	0315EF0047
Std.Gas Conc.(ppm)	152	Cylinder No.	D878173
Certified Date	27-Jun-18	Expired Date	27-Jun-26

CALIBRATION RESULTS

Point	CALIBRATION RESULTS			
	Ideal	Actual	Error	%Error
ZERO	0.00	0.10	0.10	0.10
SPAN	152.00	151.10	-0.90	-0.59
AVERAGE (%)				-0.25

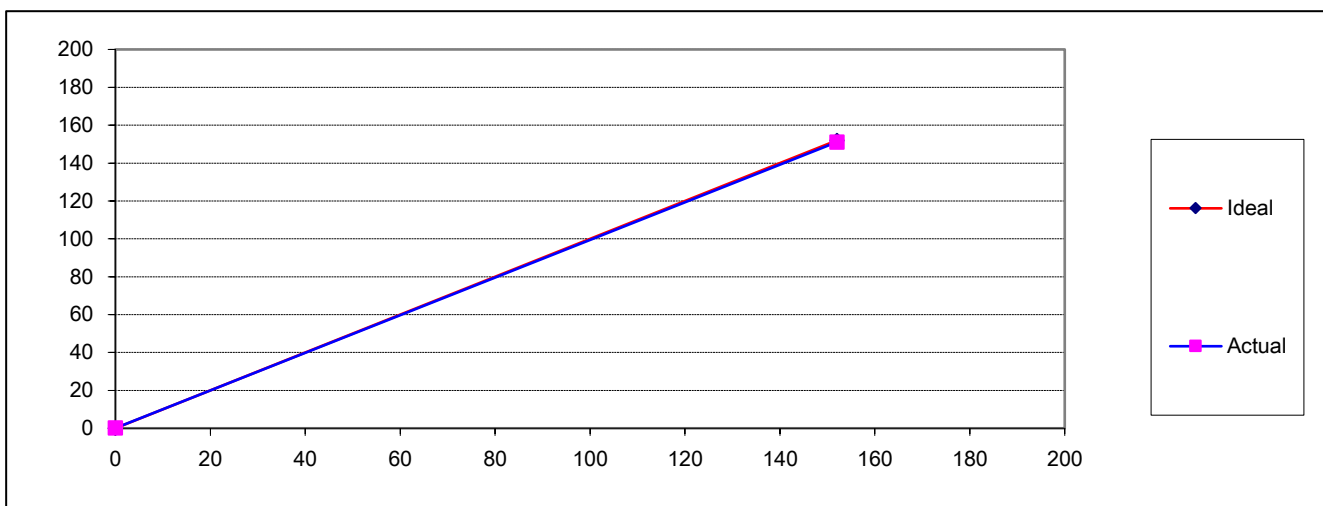

Calibrated By

(Mr.Apisit Sing-ha)
Field Environmental Scientist (4)

Approved By

(Mr.Sarayuth Jittrantont)
Assistant General Manager

Certificate of Calibration

Customer

Name : ALS Laboratory Group Thailand Co., Ltd. **Certificate No** : 25-ACT-042
Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang, **Request No** : Req-2025-0604
Bangkok 10250

Unit Under Calibration Details

Measurement item : Acoustic Calibrator Class : 1
Manufacturer : RION Range : 94 dB / 1000 Hz
Model : NC-75 Instrument Status : Used
Serial Number : 35002736
ID : RYG_FS0496

Calibration Environment and Details

Temperature : (23 $\pm$ 2 $^{\circ}$ C)
Humidity : (50 $\pm$ 20 %RH)
Barometric Pressure : (1013 $\pm$ 10.0 hPa)
Received Date : 6 March 2025
Calibration Date : 19 March 2025
Location of Calibration : LAB 1 Acoustic
Calibration Procedure : In-house method CP-ACT-02 based on IEC 60942:2017 Electroacoustics - Sound calibrators


REVIEW BY 
APPROVED BY 
NEXT CAL DATE 19/03/26

Reference Standard	Model	Serial Number	Traceable	Due Calibration
Sound Calibrator	SV 35A	58079	EEI	12 June 2025
THD Multimeter	2015	1047765	NIMT	4 February 2026

Traceability : This certificate provides traceability of measurement to recognized national standard, and to the realization of the international System of Units (SI).

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k=2$, providing a level of confidence approximately 95 %.

Calibrated By : 
Mr. Noppadon Luangart
Service Calibration Engineer

Approved By : 
Mr. Pacit Mathavorn
Calibration Engineer Supervisor

Issue Date : 19 March 2025

Certificate No : 25-ACT-042

Request No : Req-2025-0604

Sound pressure level

Calibration Results : Without Adjustment

Calibration Range (dB)	Without Adjustment (dB)		Adjustment (dB)		Uncertainty (± dB)	Acceptance limit Class 1 (± dB)	Result
	Measured	Deviated value	Measured	Deviated value			
94 dB / 1000 Hz	94.06	0.06	-	-	0.13	0.25	Pass

Frequency of Sound pressure level

Calibration Range (Hz)	Without Adjustment		Adjustment		Uncertainty (± %)	Acceptance limit Class 1 (± %)	Result
	Measured (Hz)	Deviated	Measured (Hz)	Deviated			
94 dB / 1000 Hz	1000.00	0.00	-	-	0.01	0.70	Pass

Total Harmonic Distortion plus Noise of Sound pressure level (THD+N %)

Calibration Range (Hz)	Without Adjustment	Adjustment	Uncertainty (± %)	Acceptance limit Class 1 (± %)	Result
	Measured (%)	Measured (%)			
94 dB / 1000 Hz	0.98	-	0.40	2.5	Pass

Note :

Function	Maximum-permitted Uncertainty of measurement
Sound pressure level	0.15 dB
Frequency	0.20%
Total distortion+noise	0.50%

- Acceptance limit was IEC60942:2017 Class 1
- The calibration results exclude the calibrator pressure correction
- The calibration results exclude the microphone volume correction

Certificate No : 25-ACT-042

Request No : Req-2025-0604

Decision Rule for Statements of Conformity


The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09/2019; Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass¹ = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail¹ = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

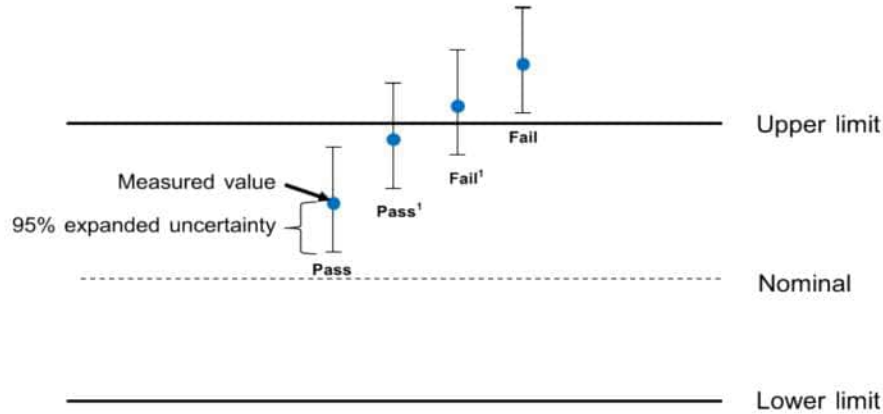

End of Calibration

Cert. No. : ACL26103

Pages : 1 of 8

Calibration Certificate


Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.: 00233183 / 157777 / 22653
ID No.: RYG_FS0024

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWANG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 $\pm$ 3) °C
Pressure : (101.3 $\pm$ 3) kPa
Relative Humidity : (50.0 $\pm$ 20) %

Received Date : 12 JANUARY 2026
Calibration Date : 28-30 JANUARY 2026
Date of Issue : 02 FEBRUARY 2026

REVIEW BY	
APPROVED BY	
NEXT CAL DATE	27/ 01/ 2027

Calibrated by : Nathakorn Pisutpaisan

Approved by : 
(Nitinun Srihawan)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL26103
Job No. : VC69AC0058
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0011-25	11-FEB-26
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EEL.BP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EEL.BP 23/0268	22-APR-26
Digital Multimeter	34461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KAI	34560495	AA-3002-25	19-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).
- 3.3 Electrical And Electronics Institute (EEI).

Cert. No. : ACL26103

Job No. : VC69AC0058

Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

Cert. No. : ACL26103

Job No. : VC69AC0058

Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
17.6

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	12.4
C - weight	18.5
Flat	24.3

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.6	0.6	0.6	± 1.5
1000	0.0	0.1	0.1	± 1.0
8000	-1.4	-1.3	-1.3	±5.0

Cert. No. : ACL26103

Job No. : VC69AC0058

Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.1	-0.1	±2.0
125	-0.1	0.0	-0.1	±1.5
250	-0.1	-0.1	-0.1	±1.5
500	0.0	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.0	0.0	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

Nettver. 5

Cert. No. : ACL26103
Job No. : VC69AC0058
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	135.9	-0.1	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	132.9	-0.1	± 1.1
132.0	131.9	-0.1	± 1.1
131.0	130.9	-0.1	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	93.9	-0.1	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	29.0	0.0	± 1.1
28.0	28.0	0.0	± 1.1
27.0	27.0	0.0	± 1.1
26.0	26.0	0.0	± 1.1
25.0	24.9	-0.1	± 1.1

Cert. No. : ACL26103
Job No. : VC69AC0058
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	28.9	-0.1	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.0 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

Cert. No. : ACL26103
Job No. : VC69AC0058
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.6	89.5	-0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$
or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

NGTC-001-5

Cert. No. : ACL26078

Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.: 00734221 / 187363 / 23230
ID No.: RYG_FS0027

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAEANG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 $\pm$ 3) °C
Pressure : (101.3 $\pm$ 3) kPa
Relative Humidity : (50.0 $\pm$ 20) %

Received Date : 05 JANUARY 2026
Calibration Date : 21 - 23 JANUARY 2026
Date of Issue : 26 JANUARY 2026

REVIEW BY	
APPROVED BY	
NEXT CAL DATE	20/ 01/ 2027

Calibrated by :

Nathakorn Pisutpaisan

Approved by :


(Nitinun Srihawan)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL26078
Job No. : VC69AC0053
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0011-25	11-FEB-26
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EEL.BP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EEL.BP 23/0268	22-APR-26
Digital Multimeter	34461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KAI	34560495	AA-3002-25	19-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

3.3 Electrical And Electronics Institute (EEI).

Cert. No. : ACL26078
Job No. : VC69AC0053
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

Cert. No. : ACL26078

Job No. : VC69AC0053

Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
15.1

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	11.3
C - weight	17.6
Flat	23.4

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.4	0.4	0.5	± 1.5
1000	0.2	0.2	0.2	± 1.0
8000	1.4	1.5	1.5	±5.0

Cert. No. : ACL26078

Job No. : VC69AC0053

Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	0.0	±2.0
125	0.0	0.1	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.1	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.1	0.1	± 0.3

Cert. No. : ACL26078

Job No. : VC69AC0053

Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	26.9	-0.1	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.9	-0.1	± 1.1

Cert. No. : ACL26078
Job No. : VC69AC0053
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	28.9	-0.1	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.0 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

Cert. No. : ACL26078
Job No. : VC69AC0053
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.4	0.0	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	132.9	-0.1	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.5	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$
or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

Signature

Certificate of Calibration

Customer

Name : ALS Laboratory Group Thailand Co., Ltd. **Certificate No** : 26-ACT-007
Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang, **Request No** : Rcq-2026-0043
Bangkok 10250

Unit Under Calibration Details

Measurement item : Acoustic Calibrator Class : 1
Manufacturer : RION Range : 94 dB / 1000 Hz
Model : NC-74 Instrument Status : Used
Serial Number : 34178121
ID : RYG_FS0213

Calibration Environment and Details

Temperature : (23 ±2 °C)
Humidity : (50 ± 20 %RH)
Barometric Pressure : (1013 ±10.0 hPa)
Received Date : 7 January 2026
Calibration Date : 9 January 2026
Location of Calibration : LAB 1 Acoustic

Calibration Procedure : In-house method CP-ACT-02 based on IEC 60942:2017 Electroacoustics - Sound calibrators

REVIEW BY 
APPROVED BY 
NEXT CAL DATE... 08/ 01/ 2027

Reference Standard	Model	Serial Number	Traceable	Due Calibration
Sound Calibrator	SV 35A	58079	EEI	20 June 2026
THD Multimeter	2015	1047765	NIMT	4 February 2026

Traceability : This certificate provides traceability of measurement to recognized national standard, and to the realization of the international System of Units (SI).

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k=2$, providing a level of confidence approximately 95 %.

Calibrated By :



Mr. Noppadon Luangart
Service Calibration Engineer

Approved By :



Mr. Pacit Mathavorn
Calibration Engineer Supervisor

Issue Date : 9 January 2026



Certificate No : 26-ACT-007

Request No : Req-2026-0043

Sound pressure level

Calibration Results : Without Adjustment

Calibration Range (dB)	Without Adjustment (dB)		Adjustment (dB)		Uncertainty (± dB)
	Measured	Deviated value	Measured	Deviated value	
94 dB / 1000 Hz	94.08	0.08	-	-	0.12

Frequency of Sound pressure level

Calibration Range (Hz)	Without Adjustment		Adjustment		Uncertainty (± %)
	Measured (Hz)	Deviated value (%)	Measured (Hz)	Deviated value (%)	
94 dB / 1000 Hz	1000.00	0.000	-	-	0.010

Total Harmonic Distortion plus Noise of Sound pressure level (THD+N %)

Calibration Range (Hz)	Without Adjustment	Adjustment	Uncertainty (± %)
	Measured (%)	Measured (%)	
94 dB / 1000 Hz	1.84	-	0.17

Note :

- The calibration results exclude the calibrator pressure correction
- The calibration results exclude the microphone volume correction

End of Calibration



Certificate of Calibration

Customer

Name : ALS Laboratory Group Thailand Co., Ltd.

Certificate No : 26-SLM-144

Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang, Bangkok 10250

Request No : Req-2026-0704

Unit Under Calibration Details

Measurement item : Sound Level Meter

Microphone Class : 2

Manufacturer : RION

Microphone Model : UC-52

Model : NL-42

Microphone S/N : 143486

Serial Number : 01222724

Preamplifier Model : NH-24

ID : RYG_FS0023

Preamplifier S/N : 22620

Resolution : 0.1 dB

Instrument Status : Used

Calibration Environment and Details

Temperature : 23 °C ± 2 °C

Humidity : 50 %RH ± 20 %RH

Barometric Pressure : 1013 hPa ± 10 hPa

Received Date : 11 March 2026

Calibrated Date : 6 April 2026

Calibration Procedure : In-house method CP-SLM-01 based on IEC 61672-3 : 2013 Electroacoustics - Sound level meters - Part 3: Periodic tests

Location of Calibration : Lab Acoustic

Reference Standard

Instrument	Brand	Model	SN.	Due calibration	Traceability
Standard Microphone	Bruel&Kjaer	4226	3412381	7 May 2026	NIMT
Audio Generator	Svantek	Svan401	131	27 September 2026	WK Electric

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k = 2$, providing a level of confidence approximately 95 %.

Calibrated By :

Mr. Noppadon Luangart

Service Calibration Engineer

Approved By :

Mr. Pacit Mathavorn

Calibration Engineer Supervisor

Issue Date :

6 April 2026

REVIEW BY

APPROVED BY

NEXT CAL DATE: 05/ 04/ 2027



Certificate No : 26-SLM-144

Request No : Req-2026-0704

1. Indication at the calibration check frequency

UUC Setting	Nominal	Before Adjust		After Adjust		UNCERTAINTY (± dB)
FAST / A / 30-130	Level (dB)	UUC	ERR	UUC	ERR	
Calibrator Setting		(dB)	(dB)	(dB)	(dB)	
1000 Hz 94 dB	93.99	94.2	0.21	94.0	0.01	0.20

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand RION, Model NC-75, SN. 35002736

2. Self-generated noise, Microphone installed

UUC Setting	Measured (dB)	UNCERTAINTY (± dB)
FAST / 30-130		
UUC Weighting	(dB)	(± dB)
A		
	19.8	0.10

3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting	Measured (dB)	UNCERTAINTY (± dB)
FAST / 30-130		
UUC Weighting	(dB)	(± dB)
A		
	14.9	0.10
C	(dB)	(± dB)
	18.9	0.10
Z	(dB)	(± dB)
	22.7	0.10

4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting	Deviation from various Frequency Weighting Response curve			UNCERTAINTY (± dB)
FAST / 30-130	A	C	Z	
STD Setting	(dB)	(dB)	(dB)	(± dB)
125 Hz	-0.1	0.0	0.0	
1000 Hz	0.0	0.0	0.0	0.60
4000 Hz	1.1	1.2	1.2	0.60
8000 Hz	0.1	0.2	0.1	0.70



Certificate No : 26-SLM-144

Request No : Req-2026-0704

5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz

UUC Setting	Deviation from various Frequency			UNCERTAINTY
FAST / 30-130	Weighting Responce curve			
STD Setting	A (dB)	C (dB)	Z (dB)	(± dB)
63 Hz	-0.2	0.0	0.0	0.20
125 Hz	-0.1	0.0	0.0	
250 Hz	-0.1	0.0	0.0	
500 Hz	0.0	0.0	0.0	
1000 Hz	0.0	0.0	0.0	
2000 Hz	0.0	0.0	0.0	
4000 Hz	0.0	0.0	0.0	
8000 Hz	0.1	0.1	0.0	
16000 Hz	-1.4	-1.4	0.0	

6. Frequency and time weightings at 1kHz

UUC Setting	STD	Measured		UNCERTAINTY
FAST / 30-130	REF	UUC	ERR	
UUC Weighting	(dB)	(dB)	(dB)	(± dB)
A	114.00	114.0	0.0	0.20
C	114.00	114.0	0.0	
Z	114.00	114.0	0.0	

UUC Setting	STD	Measured		UNCERTAINTY
30-130 / A	REF	UUC	ERR	
UUC Time Responce	(dB)	(dB)	(dB)	(± dB)
Fast	114.00	114.0	0.0	0.20
Slow	114.00	114.0	0.0	
Leq	114.00	114.0	0.0	



Certificate No : 26-SLM-144
Request No : Req-2026-0704

7. Long Term Stability

UUC Setting	Measured	UNCERTAINTY (± dB)
FAST / A / 30-130	UUC	
STD Setting	(dB)	
Initial	114.0	
Final	114.0	
Deviated	0.0	0.10

8. Level linearity on the reference level range

UUC Setting	Anticipated	Deviation		UNCERTAINTY (± dB)
FAST / A / 30-130	REF	UUC	ERR	
STD dB	(dB)	(dB)	(dB)	
138.00	138	137.9	-0.1	0.30
134.00	134	134.0	0.0	
129.00	129	129.0	0.0	
124.00	124	124.0	0.0	
119.00	119	119.0	0.0	
114.00	114	114.0	0.0	
109.00	109	109.0	0.0	
104.00	104	104.0	0.0	
99.00	99	99.0	0.0	
94.00	94	94.0	0.0	
89.00	89	89.0	0.0	
84.00	84	84.0	0.0	
79.00	79	79.0	0.0	
74.00	74	74.0	0.0	
69.00	69	69.0	0.0	
64.00	64	64.0	0.0	
59.00	59	59.0	0.0	
54.00	54	54.0	0.0	
49.00	49	49.0	0.0	
44.00	44	44.0	0.0	
39.00	39	38.9	-0.1	
34.00	34	33.9	-0.1	
29.00	29	28.9	-0.1	
24.00	24	23.9	-0.1	



Certificate No : 26-SLM-144

Request No : Req-2026-0704

9. Level linearity including the level range control

UUC Setting	STD	Measured		UNCERTAINTY
FAST / A	REF	UUC	ERR	(± dB)
UUC Range	(dB)	(dB)	(dB)	
30-130	29.70	29.8	0.1	0.30
	114	114.0	0.0	

10. Tone burst response

UUC Setting	STD	Anticipated	Measured		UNCERTAINTY
A / 30-130	Toneburst	Ref	UUC	ERR	(± dB)
UUC Time Response	(ms)	(dB)	(dB)	(dB)	
Fast	200	126.0	126.0	0.0	0.20
	2	109.0	109.0	0.0	
	0.25	100.0	99.9	-0.1	
Slow	200	119.6	119.6	0.0	
	2	100.0	100.0	0.0	
SEL	200	120.0	120.0	0.0	
	2	100.0	100.0	0.0	
	0.25	91.0	90.9	-0.1	

11. Peak C Sound level

UUC Setting	Anticipated	Measured		UNCERTAINTY
FAST / C / 55-141	REF	UUC	ERR	(± dB)
STD Setting	(dB)	(dB)	(dB)	
Complete cycle	136.4	136.4	0.00	0.20
Positive half cycle	135.4	135.2	-0.20	
Negative half cycle	135.4	135.2	-0.20	



Certificate No : 26-SLM-144

Request No : Req-2026-0704

12. Overload indication

UUC Setting	Measured	UNCERTAINTY
FAST / A / 30-130	UUC	
STD Setting	(dB)	(± dB)
Positive one-half cycle	139.3	
Negative one-half cycle	139.5	
Deviated	-0.2	0.20

13. High Level Stability

UUC Setting	Measured	UNCERTAINTY
FAST / A / 30-130	UUC	
STD Setting	(dB)	(± dB)
Initial	129.0	
Final	129.0	
Deviated	0.0	0.10

End of Certificate

Cert. No. : ACL26086

Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-52A / Microphone UC-59 / Preamplifier NH-25
Serial No.: 01220937 / 21845 / 22326
ID No.: RYG_FS0628

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWANG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 $\pm$ 3) °C
Pressure : (101.3 $\pm$ 3) kPa
Relative Humidity : (50.0 $\pm$ 20) %

Received Date : 05 JANUARY 2026
Calibration Date : 21 - 23 JANUARY 2026
Date of Issue : 26 JANUARY 2026

REVIEW BY	
APPROVED BY	
NEXT CAL DATE	20/ 01/ 2027

Calibrated by : Nathakorn Pisutpaisan

Approved by : 
(Nitinun Srihawan)

Cert. No. : ACL26086
Job No. : VC69AC0053
Pages : 2 of 8

Calibration Procedure : CP-AC-02

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0011-25	11-FEB-26
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EEL.BP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EEL.BP 23/0268	22-APR-26
Digital Multimeter	34461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KAI	34560495	AA-3002-25	19-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

3.3 Electrical And Electronics Institute (EEI).

Cert. No. : ACL26086
Job No. : VC69AC0053
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

Cert. No. : ACL26086

Job No. : VC69AC0053

Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	94.0	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
14.2

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	9.9
C - weight	14.3
Flat	19.9

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.2	0.2	0.2	± 1.0
1000	0.2	0.2	0.2	± 0.7
8000	0.5	0.6	0.6	+ 1.5, - 2.5

Cert. No. : ACL26086

Job No. : VC69AC0053

Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	0.0	±1.0
125	0.0	0.1	0.1	±1.0
250	0.0	0.0	0.0	±1.0
500	0.0	0.1	0.0	±1.0
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±1.0
4000	0.0	0.0	0.0	±1.0
8000	0.0	0.1	0.1	+ 1.5, - 2.5
16000	0.0	-1.2	-1.1	+ 2.5, -16.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.1

MTCU-5.

Cert. No. : ACL26086

Job No. : VC69AC0053

Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	±0.8
136.0	136.0	0.0	±0.8
135.0	135.0	0.0	±0.8
134.0	134.0	0.0	±0.8
133.0	133.0	0.0	±0.8
132.0	132.0	0.0	±0.8
131.0	131.0	0.0	±0.8
129.0	129.0	0.0	±0.8
124.0	124.0	0.0	±0.8
119.0	119.0	0.0	±0.8
114.0	114.0	0.0	±0.8
109.0	109.0	0.0	±0.8
104.0	104.0	0.0	±0.8
99.0	99.0	0.0	±0.8
94.0	94.0	0.0	±0.8
89.0	89.0	0.0	±0.8
84.0	84.0	0.0	±0.8
79.0	79.0	0.0	±0.8
74.0	74.0	0.0	±0.8
69.0	69.0	0.0	±0.8
64.0	64.0	0.0	±0.8
59.0	59.0	0.0	±0.8
54.0	54.0	0.0	±0.8
49.0	49.0	0.0	±0.8
44.0	44.0	0.0	±0.8
39.0	39.0	0.0	±0.8
34.0	34.0	0.0	±0.8
30.0	30.0	0.0	±0.8
29.0	29.0	0.0	±0.8
28.0	28.0	0.0	±0.8
27.0	27.0	0.0	±0.8
26.0	26.0	0.0	±0.8
25.0	25.0	0.0	±0.8

Niramon S.

Cert. No. : ACL26086

Job No. : VC69AC0053

Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±0.8

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	29.0	0.0	±0.8

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.0 ; -3.0
	2	8	117.0	117.0	0.0	1.0 ; -1.5
	200	800	134.0	134.1	0.1	±0.5
Slow	2	8	108.0	108.0	0.0	1.0 ; -3.0
	200	800	127.6	127.6	0.0	±0.5
SEL	0.25	1	99.0	98.9	-0.1	1.0 ; -3.0
	2	8	108.0	108.0	0.0	1.0 ; -1.5
	200	800	128.0	128.0	0.0	±0.5

Cert. No. : ACL26086
Job No. : VC69AC0053
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{cpeak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±2.0
One	133.4	133.4	0.0	±2.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	132.9	-0.1	±1.0
Positive half cycle	135.4	135.1	-0.3	±1.0
Negative half cycle	135.4	135.1	-0.3	±1.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.6	89.5	-0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.1

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$
or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

Mittra S.



JIRANATEE ASSOCIATES CO., LTD.

CALIBRATION REPORT

CUSTOMER NAME : ALS Laboratory Group (Thailand) Co., Ltd.			
EQUIPMENT NAME : Total Hydrocarbon Analyzer			
MANUFACTURER : Baseline	MODEL : 9000 HTHA	SERIAL NO :	0315EF0047
STANDARD GAS CONCENTRATION (PPM) : 506.1 PPM (Methane)		CYLINDER NO :	CC734373
CYLINDER PRESSURE (psig) : 1,000 PSI		CERTIFIED DATE :	12/05/2020
CERTIFIED BY : AIRGAS		EXPIRED DATE :	12/05/2028

CALIBRATION RESULTS

POINT NO	CALIBRATION RESULTS			
	IDEAL	ACTUAL	ERROR	%ERROR
ZERO	0.00	0.10	0.10	-
1	506.10	506.10	0.0	0.00
AVERAGE (%)				0.00


REVIEW BY

Supt S

APPROVED BY

Supt S

NEXT CAL DATE 11/03/2027

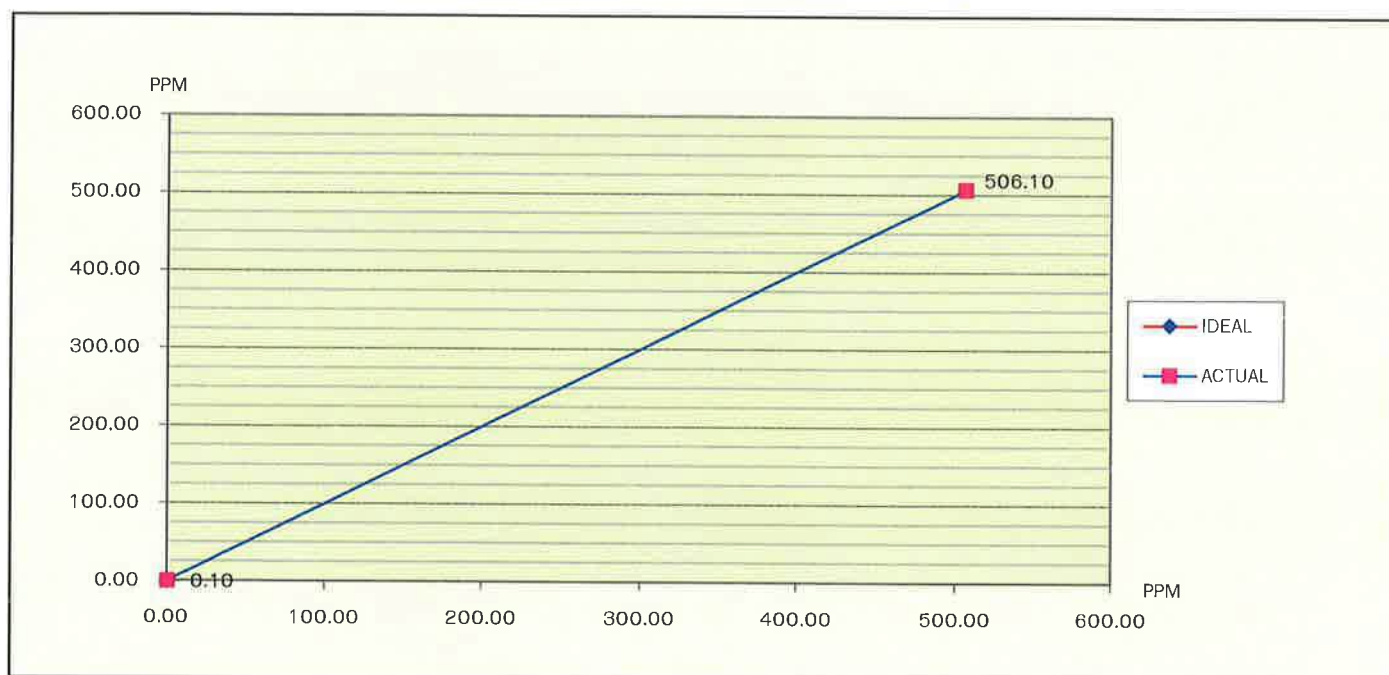

CALIBRATED BY

Supt S

DATE

12/3/69

CHECKED BY

Supt S

DATE

12/3/69

ต้องการข้อมูลทางด้านเทคนิคเพิ่มเติม : เจ้าหน้าที่ฝ่ายบริการหลังการขาย , โทร 02-868-0812 # 31 , E-Mail : Engineer@jiranatee.com

เลขที่ 63/14-15,67/35-36 ถนน เพชรเกษม 7,7/1 แขวง วัดท่าพระ เขต บางกอกใหญ่ กรุงเทพฯ 10600 โทร 02-868-0812-13 โทรสาร 02868-1889




JIRANATEE ASSOCIATES CO., LTD.

FLOW CALIBRATE

CUSTOMER NAME	:	ALS Laboratory Group (Thailand) Co., Ltd.		
EQUIPMENT NAME	:	Flow Calibrator		
MANUFACTURER	:	Bios	MODEL : 510 L	SERIAL NO : 129549

Flow Parameter	Step	Set	Display	Flow Meter
Sample	Before	40	39	28.75 cc/min
	After	40	40	40.90 cc/min
Air	Before	175	174	163.58 cc/min
	After	175	175	175.13 cc/min
Fuel	Before	35	34	29.67 cc/min
	After	35	35	34.12 cc/min

CALIBRATED BY : 

DATE : 12 / 3 / 69

CHECKED BY : 

DATE : 12 / 3 / 69

ต้องการข้อมูลทางด้านเทคนิคเพิ่มเติม : เจ้าหน้าที่ฝ่ายบริการหลังการขาย , โทร 02-868-0812 # 15-16 , E-Mail : Engineer@jiranatee.com
เลขที่ 63/14-15,67/35-36 ถนน เพชรเกษม 7, 7/1 แขวง วัดท่าพระ เขต บางกอกใหญ่ กรุงเทพฯ 10600 โทร 02-868-0812-13 โทรสาร 02868-1889

Accredited by

NSC-TISI-TIS 17025

Calibration 0426



Calibration certificate

Calibration Certificate No. 26BCI0069

Object	Electronic non-automatic weighing instrument	This calibration certificate documents the traceability to national standards.
Manufacturer	Sartorius	Uncertainties of measurements are taken into account when only statements of compliance are made.
Type	MSE125P-100-DU.	This certificate was prepared by Sartorius Corporation in accordance to the current ISO/IEC 17025:2017 standard and Sartorius Work Instruction (Method) SOP WI 08.
Serial QM Ident. no.	33108993 RYG_EN0004	This certificate relate and apply this equipment only.
Customer	ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)	
	616/10 Moo 5 T.Maenamkoo, A.Pluak Daeng, Rayong 21140, Thailand.	
Order no.	278579	REVIEW BY <i>Thanitak.</i>
Number of pages	6	APPROVED BY <i>D. Inthana.</i>
Date of calibration	03 Feb 2026	NEXT CAL DATE <i>03/02/27</i>

This calibration certificate may not be reproduced other than in full except with the permission of NSC-TISI-TIS-17025 and the issuing laboratory. Calibration certificates without signature are not valid.

The user is obliged to have the object recalibrated at appropriate intervals.

Date of issue	03 Feb 2026	Approval of the Calibration Certificate ☐ Mr. Chonchai Inthana	Person in charge Chonchai Inthana
---------------	-------------	--	--------------------------------------

Calibration object

Multi range instrument

Model	MSE125P-100-DU.	
Serial Number	33108993	
QM Ident. no Inventory no.	RYG_EN0004 ---	
Range	1	2
Maximum capacity (Max. load)	60.00000 g	120.0000 g
Measured up to	60.00000 g	120.0000 g
Scale interval	0.00001 g	0.0001 g

Place of calibration

Address	According to page 1
Department Cost center	Laboratory Department. ---
Building Floor	--- ---
Room	Laboratory Room.
Maximum temperature variation at place of calibration	5 K

Calibration procedure

EURAMET Calibration Guide No. 18, Version 4.0 (11/2015) - Guidelines on the Calibration of Non-Automatic Weighing Instruments

Test equipment

Test equipment type	Test equipment ID	Valid until
Thermometer	Testo 174H H/T250743 (Traceable to Si unit through ENTECH)	18 Nov 2026
Test weight set OIML R111 E2	Certificate No.M2508149S ,E2(Traceable to SI unit through TCS)	19 Aug 2027

Range 1

Adjustment Status

The measuring device was internally adjusted before the calibration.

Environmental and measuring conditions

Date of calibration	03 Feb 2026
Temperature at place of calibration Temp. diff. <i>T</i> _{weights} - <i>T</i> _{place}	24 °C 0.5 K
Measuring conditions	The installation site is suitable. The device is level. Balance was loaded up to Max before test.
Comments	Humidity 54.0 %RH.

Measurement results | Measurement uncertainties

Repeatability	
Test load (nominal): 50 g	
50 g	
1	50.00001 g
2	50.00001 g
3	50.00000 g
4	50.00001 g
5	50.00002 g
6	50.00001 g
7	50.00001 g
8	50.00002 g
9	50.00001 g
10	50.00000 g
<i>s</i> = 0.000007 g	

Eccentricity	
Test load (nominal): 50 g	
Center	50.00001 g
Front left	50.00001 g
Back left	50.00001 g
Back right	50.00001 g
Front right	50.00000 g
Maximum deviation from centric loading indication $ \Delta_{ecc} _{max}$ = 0.00001 g	

Testload	Indication	Error	Expansion factor	Uncertainty	Uncertainty relative
<i>L</i>	<i>I</i>	<i>E</i>	<i>k</i>	<i>U</i> (<i>E</i>)	<i>U</i> _{rel} (<i>E</i>)
0.01000 g	0.01000 g	0.00000 g	2.00	0.000024 g	0.24 %
0.05000 g	0.05000 g	0.00000 g	2.00	0.000024 g	0.048 %
0.10000 g	0.10000 g	0.00000 g	2.00	0.000037 g	0.037 %
0.50000 g	0.50000 g	0.00000 g	2.00	0.000037 g	0.0074 %
1.00000 g	1.00000 g	0.00000 g	2.00	0.000037 g	0.0037 %
2.00003 g	2.00003 g	0.00000 g	2.00	0.000050 g	0.0025 %
5.00002 g	5.00002 g	0.00000 g	2.00	0.000050 g	0.0010 %
10.00001 g	10.00001 g	0.00000 g	2.00	0.000069 g	0.00069 %
19.99999 g	20.00000 g	0.00001 g	2.00	0.000069 g	0.00035 %
50.00001 g	50.00001 g	0.00000 g	2.00	0.000091 g	0.00018 %
57.00005 g	57.00006 g	0.00001 g	2.00	0.00017 g	0.00030 %
Maximum error of indication		$ E _{max}$ = 0.00001 g			

*U*_{rel}(*E*) is the quotient of *U*(*E*) and test load *L*. The uncertainty of measurement *U*(*E*) is valid only if error *E* is considered. You will find reference notes on the uncertainty of measurement in use under: Appendix to the calibration certificate | Interpretation of measurement results.
Reference note: The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the documented Expansion factor, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

Range 2

Adjustment Status

The measuring device was internally adjusted before the calibration.

Environmental and measuring conditions

Date of calibration	03 Feb 2026
Temperature at place of calibration Temp. diff. $T_{\text{weights}} - T_{\text{place}}$	24 °C 0.5 K
Measuring conditions	The installation site is suitable. The device is level. Balance was loaded up to Max before test.
Comments	Humidity 54.0 %RH.

Measurement results | Measurement uncertainties

Repeatability

Test load (nominal): 100 g	
100 g	
1	100.0000 g
2	100.0000 g
3	100.0000 g
4	99.9999 g
5	100.0000 g
6	100.0000 g
7	100.0000 g
8	100.0000 g
9	100.0000 g
10	100.0000 g
$s = 0.00003 \text{ g}$	

Eccentricity

Test load (nominal):	50 g
Center	50.00001 g
Front left	50.00001 g
Back left	50.00001 g
Back right	50.00001 g
Front right	50.00000 g
Maximum deviation from centric loading indication $ \Delta_{\text{ecc}} _{\text{max}} = 0.00001 \text{ g}$	

Error of indication

Testload L	Indication I	Error E	Expansion factor k	Uncertainty $U(E)$	Uncertainty relative $U_{\text{rel}}(E)$
10.00001 g	10.00001 g	0.00000 g	2.00	0.000069 g	0.00069 %
65.0000 g	65.0000 g	0.0000 g	2.00	0.00017 g	0.00026 %
70.0000 g	70.0000 g	0.0000 g	2.00	0.00017 g	0.00024 %
75.0000 g	75.0000 g	0.0000 g	2.00	0.00018 g	0.00023 %
80.0000 g	80.0000 g	0.0000 g	2.00	0.00018 g	0.00023 %
85.0000 g	85.0000 g	0.0000 g	2.00	0.00021 g	0.00025 %
90.0000 g	90.0000 g	0.0000 g	2.00	0.00019 g	0.00021 %
95.0000 g	95.0000 g	0.0000 g	2.00	0.00022 g	0.00023 %
100.0000 g	100.0000 g	0.0000 g	2.00	0.00017 g	0.00017 %
110.0000 g	110.0000 g	0.0000 g	2.00	0.00028 g	0.00025 %
120.0000 g	120.0000 g	0.0000 g	2.00	0.00028 g	0.00023 %
Maximum error of indication		$ E _{\text{max}} = 0.0000 \text{ g}$			

$U_{\text{rel}}(E)$ is the quotient of $U(E)$ and test load L . The uncertainty of measurement $U(E)$ is valid only if error E is considered. You will find reference notes on the uncertainty of measurement in use under: Appendix to the calibration certificate | Interpretation of measurement results.
Reference note: The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the documented Expansion factor, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

End of calibration certificate

Uncertainty of measurement in use

Range 1

Device adjusted before measurement	Yes
Temperature deviation considered	1.5 K (isoCAL active)
Temperature coefficient considered	$2 \cdot 10^{-6}/\text{K}$


Uncertainty of the weighing result $U_{gI}(W)$

$U_{gI}(W) = 0.000016 \text{ g} + 3.70 \cdot 10^{-6} \cdot R$

Reference note: The current uncertainty of measurement is calculated by entering of the reading R into this formula. In relation to this, there is no need for a correction of the indication error. The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied with an Expansion factor of 2, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

Indication in % from max load	Net indication R	Uncertainty $U_{gI}(W)$	Uncertainty relative $U_{gI}(W)_{rel}$
1 %	0.60000 g	0.000018 g	0.0030 %
25 %	15.00000 g	0.000072 g	0.00048 %
50 %	30.00000 g	0.00013 g	0.00042 %
75 %	45.00000 g	0.00018 g	0.00041 %
100 %	60.00000 g	0.00024 g	0.00040 %

Graphic realization of the relative uncertainty of measurement | process accuracy

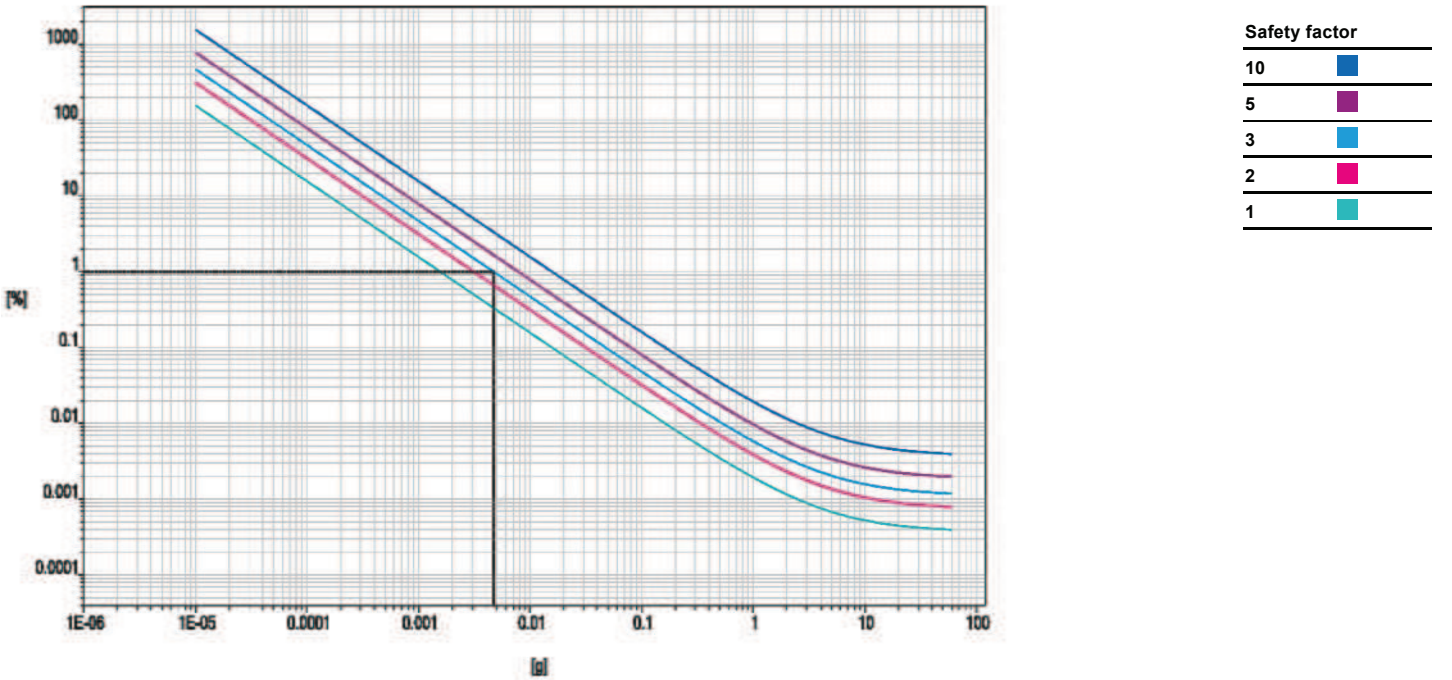

Displayed example

Process accuracy	1.00 %
Safety factor	3
Minimum sample weight	0.00470 g

Uncertainty of measurement in use

Range 2

Device adjusted before measurement	Yes
Temperature deviation considered	1.5 K (isoCAL active)
Temperature coefficient considered	$2 \cdot 10^{-6}/\text{K}$


Uncertainty of the weighing result $U_{gl}(W)$

$U_{gl}(W) = 0.000086 \text{ g} + 3.00 \cdot 10^{-6} \cdot R$

Reference note: The current uncertainty of measurement is calculated by entering of the reading R into this formula. In relation to this, there is no need for a correction of the indication error. The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied with an Expansion factor of 2, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

Indication in % from max load	Net indication R	Uncertainty $U_{gl}(W)$	Uncertainty relative $U_{gl}(W)_{rel}$
1 %	1.20000 g	0.000090 g	0.0075 %
25 %	30.00000 g	0.00018 g	0.00059 %
50 %	60.00000 g	0.00027 g	0.00044 %
75 %	90.0000 g	0.00036 g	0.00040 %
100 %	120.0000 g	0.00045 g	0.00038 %

Graphic realization of the relative uncertainty of measurement | process accuracy

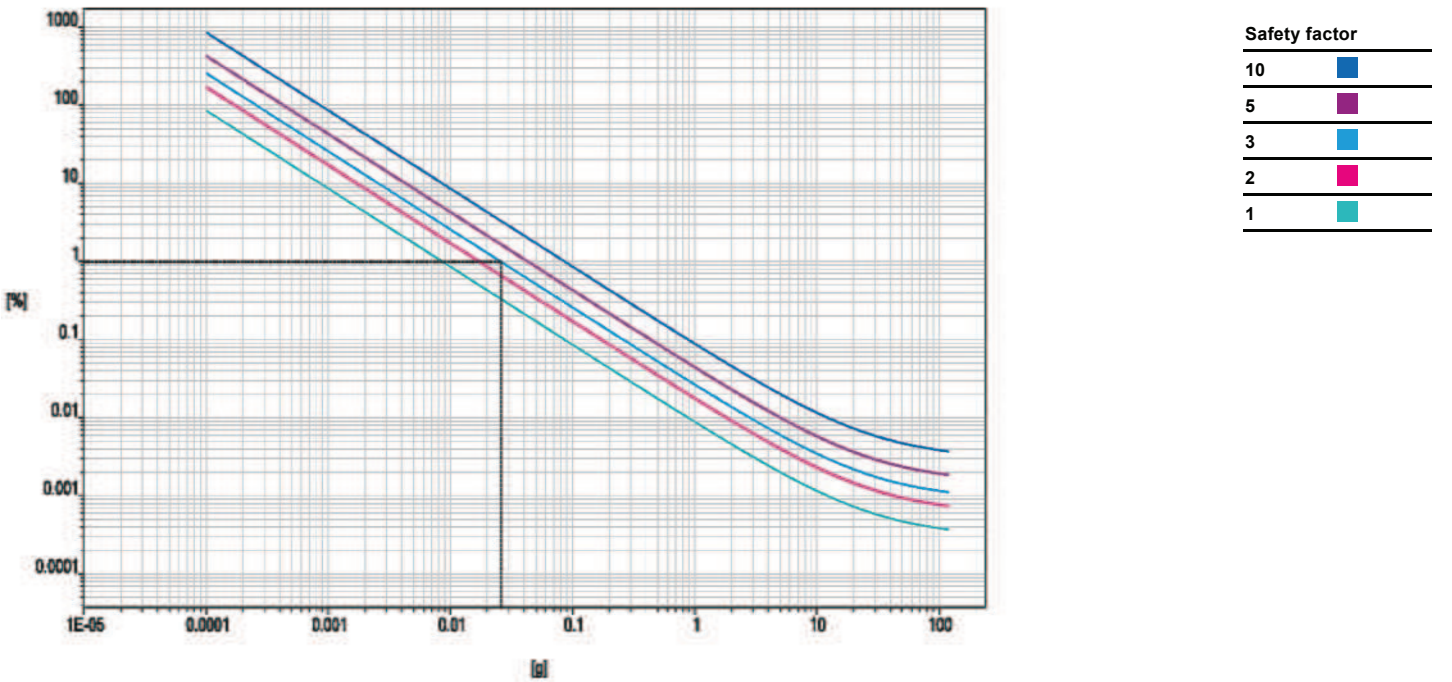

Displayed example

Process accuracy	1.00 %
Safety factor	3
Minimum sample weight	0.02577 g



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert. No.: 25LM10

Page.: 1 of 2

Equipment : DO Meter with Sensor

Manufacturer : YSI

Model : 5000-115V

Serial No. : 15E102796

ID No. : RYG_EN0032

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
(Rayong Branch)
616/10 Moo 5 T. Maenam Khu, A. Pluakdaeng,
Rayong 21140 Thailand

Location : TPA On Site Calibration Laboratory

Received Order : 17 January 2025

Calibrated Date : 20 January 2025

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

AC Line Voltage : (220 ± 22) V

Calibrated by : Warakorn Lerngagtrakul

Approved by :

Approved Signatory

() Chakrit Waewwanjua

(✓) Suwit Imjai

() Kunchit Promprat

Issue Date : 23 January 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

REVIEW BY Photchana S.

APPROVED BY

NEXT CAL DATE 20/07/26



Equipment : DO Meter with Sensor
Condition As-Received : Used Item
Reference : 2501-0600DSC-2

Cert. No.: 25LM10

Page.: 2 of 2

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1) Digital Thermometer	2188080	2411022	TPA	17 Sep 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N.: 15E100464

<u>Calibration Point</u> (°C)	<u>Immersion Depth</u> (mm)	<u>Standard Temperature</u> (°C)	<u>UUC* Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (± °C)	<u>Coverage Factor</u> <i>k</i>
20.00	60	20.002	19.81	-0.192	0.15	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES

534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000 FAX. 0-2719-9484

Certificate of Testing

Cert.No.: 25TW15

Page.: 1 of 2

Equipment : DO Meter

Manufacturer : YSI

Model : 5000-115V

Serial No. : 15E102796

ID No. : RYG_EN0032

Received Date : 17 January 2025

Test Date : 20 January 2025

Reference : 2501-0600DSC-1

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
(Rayong Branch)
616/10 Moo 5, T.Maenam Khu, A.Pluakdaeng,
Rayong 21140, Thailand

Laboratory Condition : Temperature (25 ± 5) °C
Humidity (50 ± 20) %

Test Procedure : In - house method : CP-CH9
by Comparison Technique with Azide Modification Method

Tested by : Walalak Sirithean

Approved by : 
Approved Signatory

() Pornthippa Tameyakul
() Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 21 January 2025



Cert.No.: 25TW15

Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

<u>Instruments</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1. Burette	-	130BU10	23CG1172	22 Mar 2025
2. Balance	14233821	110RC001	24MM131	04 July 2025

2. Standard Material :-

<u>Material</u>	<u>Manufacturer</u>	<u>Lot.No.</u>	<u>Assay</u>
Sodium Thiosulfate 5-Hydrate AR	KEMAUS	2203162447	99.6%

Result : Dissolved Oxygen Meter Adjustment With Air 100 %

Dissolved Oxygen Probe No.: 15E100464

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.20	8.20	0.0084

This report was certified only for the instrument we tested. It is allowable to use for study. Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced other in full, without written approval of the laboratory.

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert. No.: 24TM1663

Page : 1 of 3

Equipment : Low Temp. Incubator

Manufacturer : Memmert

Model : IPP750

Serial No. : V818.0084

ID No. : RYG_EN0154

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd. Rayong Branch
616/10 Moo 5, T.Maenam Khu,
A.Pluakdaeng,
Rayong 21140, Thailand

Location : BOD Room

Received Order : 01 November 2024

Calibration Date : 01 November 2024

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

AC Line Voltage : (220 ± 22) V

Calibrated by : Krisda Malee

Approved by :

Kunchit

Approved Signatory

() Ponpan Paipim

() Suwit Imjai

(✓) Kunchit Promprat

Issue Date :

07 November 2024

REVIEW BY *Thanitak*

APPROVED BY *D. Khunon*

NEXT CAL DATE..... 01/05/26

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : Low Temp. Incubator
Condition As-Received : Used Item
Reference : 2411-0002OC-1

Cert. No.: 24TM1663

Page : 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1) Data Acquisition	MY44073381	24LM73	TPA	18 May 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.


3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close

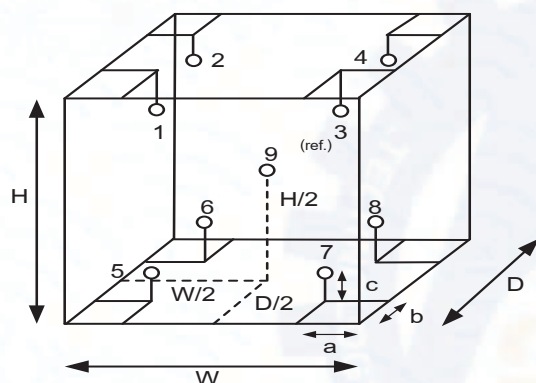

Environment during calibration		
	Beginning	Finished
Temp. (°C)	24	25
REL.Humid. (%)	55	53
AC Supply (Volt)	220	221

Position :	Ref. Std. ID No.:
1	1RTD-2/1
2	1RTD-2/2
3	22-01RTD-03
4	1RTD-2/4
5	1RTD-2/5
6	1RTD-2/6
7	23-01RTD-07
8	1RTD-2/8
9 (ref.)	23-01RTD-09

Probe Installation Details :

a = 10 cm
b = 10 cm
c = 10 cm

Dimension of Chamber :

D = 0.60 m
W = 1.0 m
H = 1.2 m
Capacity = 0.72 m³



Equipment : Low Temp. Incubator
Condition As-Received : Used Item
Reference : 2411-0002OC-1
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Cert. No.: 24TM1663

Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor <i>k</i>
20.0	20.0	20.0	0.026	0.26	0.53	2

Calibration Point (°C)	Measured Temperature (°C)									Uncertainty (±°C)
	Position									
	1	2	3	4	5	6	7	8	9 (ref.)	
20.0	20.071	19.915	20.273	20.179	19.977	19.782	20.056	20.026	20.033	0.30

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert. No.: 26TM461

Page : 1 of 3

Equipment : Low Temp. Incubator

Manufacturer : Memmert

Model : IPP750

Serial No. : V818.0084

ID No. : RYG_EN0154

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd. Rayong Branch
616/10 Moo 5, T.Maenamkoo, A.Pluakdaeng,
Rayong 21140, Thailand

Location : BOD Room

Received Order : 18 March 2026

Calibration Date : 18 March 2026

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

AC Line Voltage : (220 ± 22) V

Calibrated by : Preecha Hlahib

Approved by :

Kunchit

Approved Signatory

() Chakrit Waewwanjua

() Suwit Imjai

(✓) Kunchit Promprat

Issue Date : 31 March 2026

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : Low Temp. Incubator
Condition As-Received : New Item
Reference : 2603-0502OC-2

Cert. No.: 26TM461
Page : 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1) Data Acquisition	MY49023932	25LM121	TPA,	27 Jul 2026

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This measurement result is traceable to the International System of Unit maintained through :


Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Not Available

Environment during calibration		
	Beginning	Finished
Temp. (°C)	23	21
REL.Humid. (%)	37	33
AC Supply (Volt)	220	221

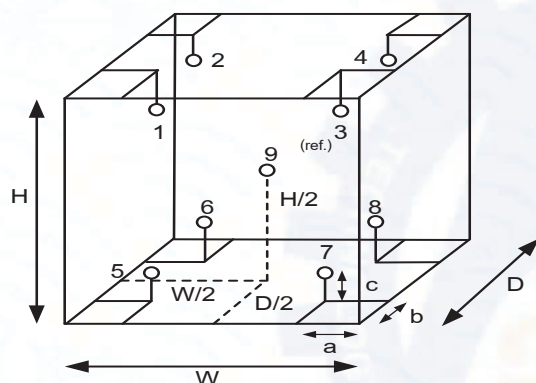

Position :	Ref. Std. ID No.:
1	19-16RTD-01
2	19-16RTD-02
3	19-16RTD-03
4	23-16RTD-04
5	19-16RTD-05
6	19-14RTD-06
7	21-16RTD-07
8	19-16RTD-08
9 (ref.)	19-16RTD-09

Probe Installation Details :

a = 10 cm
 b = 10 cm
 c = 10 cm

Dimension of Chamber :

D = 0.60 m
 W = 1.0 m
 H = 1.2 m
 Capacity = 0.72 m³



Equipment : Low Temp. Incubator
Condition As-Received : New Item
Reference : 2603-0502OC-2
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Not Available

Cert. No.: 26TM461

Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor <i>k</i>
20.0	20.0	20.0	0.019	0.19	0.34	2

Calibration Point (°C)	Measured Temperature (°C)									Uncertainty (±°C)
	Position									
	1	2	3	4	5	6	7	8	9 (ref.)	
20.0	20.185	20.132	20.303	20.160	20.001	20.054	19.983	20.060	20.163	0.30

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert.No.: 25CG3668

Page.: 1 of 2

Equipment :	Burette
Capacity :	50 mL
Serial No. :	-
ID. No. :	RYG_EN0216
Manufacturer :	Witeg
Made in :	Germany
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. Rayong Branch 616/10 Moo 5 T.MaenamKoo, A.Pluakdaeng Rayong 21140, Thailand
Ambient Temperature :	(20 ± 2.5) °C
Relative Humidity :	(50 ± 10) %
Barometric Pressure :	753 mmHg
Calibration Procedure :	ASTM E 542 - 01
Calibrated by :	Srisuda Khamtha
Approved by :	 Approved Signatory
() Ponpan Paipim	
(✓) Chakrit Waewwanjua	

REVIEW BY *Thanitak*

APPROVED BY *D. Khamtha*

NEXT CAL DATE **18/09/26**

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : Burette
Received Date : 16 September 2025
Condition As-Received : Used Item
Calibration Date : 18 September 2025
Reference : 2509-0564DSC-3

Cert.No.: 25CG3668

Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

<u>Instruments</u>	<u>Model</u>	<u>Serial No.</u>	<u>ID. No.</u>	<u>Certificate No.</u>	<u>Traceability</u>	<u>Due date</u>
1) Balance	XP205	B134206712	140RC007	25MM296	TPA	16 July 2026
2) Humidity/Baro/Temp	MHB-382SD	AM.42259	140EC016	25H1616	TPA	14 Aug 2026
3) Digital Thermometer	HH376	230806555	140EC013	25I1740	TPA	17 Jan 2026

This measurement result is traceable to SI Unit

2. The certificate is valid only to the item calibrated on date and place of calibration.

3. True value is converted to true volume at the standard temperature of 20 °C


Calibration result :

Nominal capacity (mL)	Reading (mL)	Uncertainty (± mL)	k Factor
10	10.0264	0.0082	2.00
25	25.0141	0.0087	2.00
50	49.9952	0.010	2.00

Remark mL = cm³

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-




Certificate of Calibration

Equipment: SPECTROPHOTOMETER
Model: DR6000
Serial No. (or ID.): 1627845 (RYG_EN0037)
Manufacturer: HACH
Condition: In Condition

Certificate No.: C06250108
Issued Date: 18 March 2025
Job No.: WO-00064379
Page: 1 of 3

Customer: ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
616/10 Moo 5 T.Maenam Khu,
A.Pluakdaeng, Rayong 21140, Thailand.

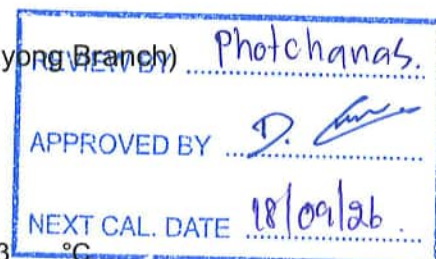

Environment Condition:

Temperature	24.4	°C	±	0.3	°C
Humidity	60.8	%RH	±	3.5	%RH

Calibration Place: ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
(Wet Chemistry Lab)
616/10 Moo 5 T.Maenam Khu, A.Pluakdaeng, Rayong 21140, Thailand.

Calibration By: Mr.Preecha Phooarsai

Calibration Date: 18 March 2025

The Method used: In house method, CAL-WI-24, base on ASTM E 275-08 and ASTM E 387-04

Traceability: This certificate is traceable to the CRM maintained by National Institute of Standards and Technology (NIST) through Starna Scientific Limited.

The standard for Wavelength Certificate No. 111583 and 111584

The standard for Photometric Certificate No. 9114984 and 111588

The standard for Stray light Certificate No. 111586 and 111585

The standard for Spectral resolution Certificate No. 111587



(Mr. Preecha Phooarsai)

Person in charge



(Miss Kaewkan Suradech)

Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ($k=2$) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด

DKSH Technology Limited

2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260

2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Calibration Results:
Without Adjustment

Wavelength Accuracy (nm), The spectral bandwidth of Std at 2 nm and UUC at 2 nm

Standard Wavelength	Unit Under Calibration	Correction	Uncertainty
418.61	418.5	0.11	0.13
536.66	536.7	-0.04	0.13
637.98	638.3	-0.32	0.13
748.48	748.8	-0.32	0.13
807.03	807.5	-0.47	0.13

Photometric Accuracy (Absorbance)

Wavelength	Standard absorbance	Unit Under Calibration	Correction	Uncertainty
420 nm	0.0000	0.000	0.0000	0.0045
	0.2930	0.291	0.0020	0.0045
	0.5168	0.518	-0.0012	0.0045
	1.0298	1.031	-0.0012	0.0045
440 nm	0.0000	0.000	0.0000	0.0045
	0.2867	0.285	0.0017	0.0045
	0.5073	0.508	-0.0007	0.0045
	1.0083	1.009	-0.0007	0.0045
465 nm	0.0000	0.000	0.0000	0.0045
	0.2516	0.250	0.0016	0.0045
	0.4595	0.461	-0.0015	0.0045
	0.9334	0.935	-0.0016	0.0045
546.1 nm	0.0000	0.000	0.0000	0.0045
	0.2461	0.246	0.0001	0.0045
	0.4652	0.466	-0.0008	0.0045
	0.9468	0.948	-0.0012	0.0045
590 nm	0.0000	0.000	0.0000	0.0045
	0.2594	0.259	0.0004	0.0045
	0.5040	0.505	-0.0010	0.0045
	1.0032	1.004	-0.0008	0.0045
635 nm	0.0000	0.000	0.0000	0.0045
	0.2579	0.258	-0.0001	0.0045
	0.4971	0.497	0.0001	0.0045
	0.9720	0.973	-0.0010	0.0045

Calibration Results:
Without Adjustment
Photometric Accuracy (Absorbance)

Wavelength	Standard absorbance	Unit Under Calibration	Correction	Uncertainty
235 nm	0.0000	0.000	0.0000	0.0080
	0.7355	0.738	-0.0025	0.0080
257 nm	0.0000	0.000	0.0000	0.0080
	0.8574	0.857	0.0004	0.0080
313 nm	0.0000	0.000	0.0000	0.0080
	0.2864	0.290	-0.0036	0.0080
350 nm	0.0000	0.000	0.0000	0.0080
	0.6374	0.637	0.0004	0.0080

Stray light *

Standard: cut-off	UUC: Wavelength (nm)	UUC: Transmission (%T)	Absorbance (A)
260.62 +/- 0.11 nm	260.6	1.7	1.770
391.44 +/- 0.11 nm	391.4	1.4	1.854

Spectral Resolution *

Nominal Concentration 0.02 % v/v	Peak	Trough	Ratio	SBW
Standard Wavelength (nm)	268.66	266.69	1.38	2.00
UUC: Wavelength (nm)	268.2	266.2		
Std Absorbance (A)	0.4566	0.2780		
UUC: Absorbance (A)	0.413	0.299		

* Calibration Marked " Not TISI Accredited " in this Certificate have been included for completeness.

The End of Certificate

ใบตรวจสอบสภาพเครื่องวัดสิ่งแวดล้อม

เลขที่ใบงาน: WO-00064379

ชนิดเครื่องมือ: SPECTROPHOTOMETER

รุ่น: DR6000

หมายเลขเครื่อง: 1627845

ตรวจสอบ (รับ)		รายการตรวจเช็ค	ตรวจสอบ (ส่ง)		หมายเหตุ
18 Mar 2025			18 Mar 2025		
ปกติ	ไม่ปกติ		ปกติ	ไม่ปกติ	
		General			
☒	☐	1. ความสมบูรณ์เครื่อง	☒	☐	
☒	☐	2. ความสะอาด (ช่องใส่ตัวอย่าง, ภายใน-นอกเครื่อง)	☒	☐	
☒	☐	3. สวิทช์ ปิด – เปิด เครื่อง (On-Off Swicth)	☒	☐	
☒	☐	4. ปุ่มกด (Keypad)	☒	☐	
☒	☐	5. หน้าจอ (Display, Screen Contrast)	☒	☐	
		Spectrophotometer			
☐	☐	6. แรงดันไฟฟ้า (Battery Backup) >= 2.5 VDC	☐	☐	
☐	☐	7. ตัวหมุนเลือกความยาวคลื่น (Wavelength Control)	☐	☐	
☒	☐	8. ความยาวคลื่น (Wavelength Check)	☒	☐	*
☒	☐	9. แหล่งกำเนิดแสง (UV < 3,000 hour)	☒	☐	13.5 Hours
☒	☐	10. แหล่งกำเนิดแสง (Visible < 5,000 hour)	☒	☐	893.0 Hours
☒	☐	11. ช่องวัดหลายตัวอย่าง (Carousel Module)	☒	☐	
		pH Meter and Conductivity Meter			
☐	☐	12. อิเล็กโทรด (Electrode and Connection Cable)	☐	☐	
☐	☐	13. ระดับสารละลายใน Electrode (Level KCl)	☐	☐	
☐	☐	14. ฝาปิดกันปลาย Electrode (Dust Protection Hood)	☐	☐	
☐	☐	15. ขาจับอิเล็กโทรด (Stand)	☐	☐	
		Turbidimeter			
☐	☐	16. ค่าความขุ่นที่ต่ำสุด (No Sample)	☐	☐	
☐	☐	17. ระดับการส่องสว่างของแสง (>= 2.5 ไม่เกิน 3.0)	☐	☐	
		Automatic titrator			
☐	☐	18. สภาพ Piston Burettes	☐	☐	
☐	☐	19. Function Rinsing and Dosing	☐	☐	
☐	☐	20. ระบบท่อสายยางและอุปกรณ์ประกอบ	☐	☐	

เพิ่มเติม/ข้อแนะนำ : * 656.1nm = 656.1nm

* 486.0nm = 485.7nm

Mr.Preecha Phooarsai

Service Engineer

Accredited by

NSC-TISI-TIS 17025

Calibration 0426



Calibration certificate

Calibration Certificate No. 25BKL0003

Object	Electronic non-automatic weighing instrument	This calibration certificate documents the traceability to national standards.
Manufacturer	Sartorius	Uncertainties of measurements are taken into account when only statements of compliance are made.
Type	MSU224S-100-DU	This certificate was prepared by Sartorius Corporation in accordance to the current ISO/IEC 17025:2017 standard and Sartorius Work Instruction (Method) SOP WI 08.
Serial QM Ident. no.	31709552 RYG_EN0003	This certificate relate and apply this equipment only.
Customer	ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)	
	616/10 Moo 5 T.Maenam Khu, A.Pluak Daeng, Rayong 21140, Thailand.	
Order no.	2230	
Number of pages	4	
Date of calibration	20 Feb 2025	

REVIEW BY

Thanitak.

APPROVED BY

D. Khunon.

NEXT CAL DATE

20/02/26

This calibration certificate may not be reproduced other than in full except with the permission of NSC-TISI-TIS-17025 and the issuing laboratory. Calibration certificates without signature are not valid.

The user is obliged to have the object recalibrated at appropriate intervals.

Date 06 Mar 2025

Approval of the Calibration Certificate



Mr. Chonchai Inthana

Person in charge

Kachen Lalee

Calibration object

Single range instrument

Model	MSU224S-100-DU
Serial Number	31709552
QM Ident. no Inventory no.	RYG_EN0003 ---

Maximum capacity (Max. load)	220.0000 g
Measured range	220.0000 g
Scale interval	0.0001 g

Place of calibration

Address	According to page 1
Department Cost center	Laboratory Department. ---
Building Floor	--- 1st Floor.
Room	Balance Room.
Maximum temperature variation at place of calibration	5 K

Calibration procedure

EURAMET cg-18, V4.0 - Guidelines on the Calibration of Non-Automatic Weighing Instruments

Test equipment

Test equipment type	Test equipment ID	Valid until
Thermometer	MHB-382SD s/nB011342 Traceable to SI unit through DKSH	21 Aug 2025
Test weight set OIML R111 E2	Certificate No.M2308197S ,E2(Traceable to SI unit through TCS)	23 Aug 2025

Adjustment Status

The measuring device was internally adjusted before the calibration.

Environmental and measuring conditions

Date of calibration	20 Feb 2025
Temperature at place of calibration Temp. diff. <i>T</i> _{weights} - <i>T</i> _{place}	24.7 °C 0.3 K
Measuring conditions	The installation site is suitable. The device was levelled. Balance was loaded up to Max before test.
Comments	Humidity 62.3 %RH.

Measurement results | Measurement uncertainties

Repeatability			Eccentricity	
Test load (nominal): 10 g 200 g			Test load (nominal): 100 g	
	10 g	200 g		
1	10.0000 g	200.0000 g	Center	
2	10.0000 g	200.0001 g	Front left	
3	9.9999 g	200.0000 g	Back left	
4	10.0000 g	200.0000 g	Back right	
5	10.0000 g	200.0001 g	Front right	
6	9.9999 g	200.0000 g	Maximum deviation from centric loading indication	
7	10.0000 g	200.0000 g	Δ _{ecc} max = 0.0001 g	
8	10.0000 g	200.0000 g		
9	10.0000 g	200.0000 g		
10	10.0000 g	200.0001 g		
	<i>s</i> = 0.00004 g	<i>s</i> = 0.00005 g		

Testload	Indication	Error	Expansion factor	Uncertainty	Uncertainty relative
<i>L</i>	<i>I</i>	<i>E</i>	<i>k</i>	<i>U</i> (<i>E</i>)	<i>U</i> _{rel} (<i>E</i>)
0.0100 g	0.0100 g	0.0000 g	2.00	0.00012 g	1.2 %
0.1000 g	0.1000 g	0.0000 g	2.00	0.00013 g	0.13 %
0.5000 g	0.5000 g	0.0000 g	2.00	0.00013 g	0.026 %
1.0000 g	1.0000 g	0.0000 g	2.00	0.00013 g	0.013 %
5.0000 g	5.0000 g	0.0000 g	2.00	0.00013 g	0.0026 %
10.0000 g	10.0000 g	0.0000 g	2.00	0.00013 g	0.0013 %
20.0000 g	20.0000 g	0.0000 g	2.00	0.00014 g	0.00068 %
50.0000 g	50.0000 g	0.0000 g	2.00	0.00015 g	0.00029 %
100.0000 g	100.0001 g	0.0001 g	2.00	0.00018 g	0.00018 %
200.0000 g	200.0000 g	0.0000 g	2.00	0.00028 g	0.00014 %
220.0000 g	220.0000 g	0.0000 g	2.00	0.00032 g	0.00015 %
Maximum error of indication		<i>E</i> _{max} = 0.0001 g			

*U*_{rel}(*E*) is the quotient of *U*(*E*) and test load *L*. The uncertainty of measurement *U*(*E*) is valid only if error *E* is considered. You will find reference notes on the uncertainty of measurement in use under: Appendix to the calibration certificate | Interpretation of measurement results.
Reference note: The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the documented Expansion factor, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

End of calibration certificate

Uncertainty of measurement in use

Device adjusted before measurement	Yes
Temperature deviation considered	1.5 K (isoCAL active)
Temperature coefficient considered	$1 \cdot 10^{-6}/\text{K}$


Uncertainty of the weighing result $U_{gl}(W)$

$U_{gl}(W) = 0.00013 \text{ g} + 3.42 \cdot 10^{-6} \cdot R$

Reference note: The current uncertainty of measurement is calculated by entering of the reading R into this formula. In relation to this, there is no need for a correction of the indication error. The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied with an Expansion factor of 2, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

Indication in % from max load	Net indication R	Uncertainty $U_{gl}(W)$	Uncertainty relative $U_{gl}(W)_{rel}$
1 %	2.2000 g	0.00014 g	0.0063 %
25 %	55.0000 g	0.00032 g	0.00058 %
50 %	110.0000 g	0.00051 g	0.00046 %
75 %	165.0000 g	0.00069 g	0.00042 %
100 %	220.0000 g	0.00088 g	0.00040 %

Graphic realization of the relative uncertainty of measurement | process accuracy

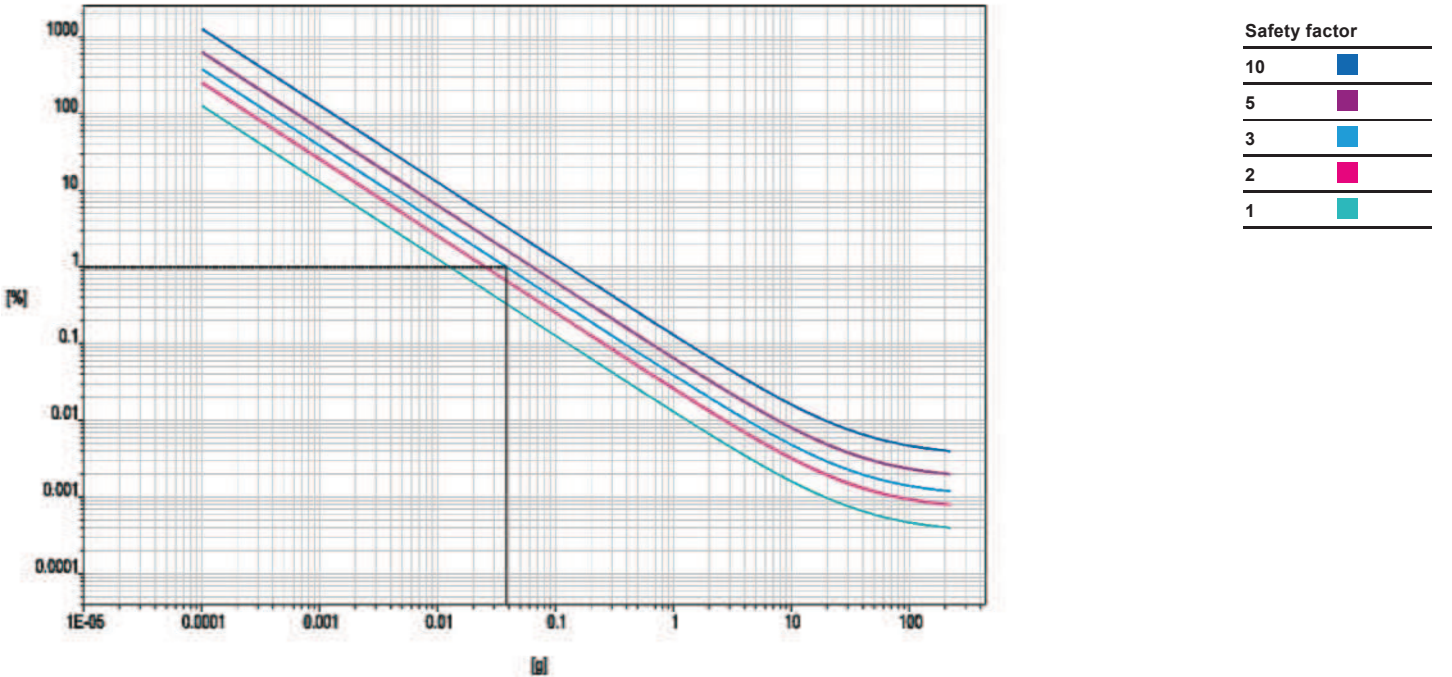

Displayed example

Process accuracy	1.00 %
Safety factor	3
Minimum sample weight	0.0380 g

Accredited by

NSC-TISI-TIS 17025

Calibration 0426



Calibration certificate

Calibration Certificate No. 26BCI0066

Object	Electronic non-automatic weighing instrument	This calibration certificate documents the traceability to national standards.
Manufacturer	Sartorius	Uncertainties of measurements are taken into account when only statements of compliance are made.
Type	MSU224S-100-DU	This certificate was prepared by Sartorius Corporation in accordance to the current ISO/IEC 17025:2017 standard and Sartorius Work Instruction (Method) SOP WI 08.
Serial QM Ident. no.	31709552 RYG_EN0003	This certificate relate and apply this equipment only.
Customer	ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)	
	616/10 Moo 5 T.Maenamkoo, A.Pluak Daeng, Rayong 21140, Thailand.	
Order no.	278579	REVIEW BY <i>Thanita K.</i>
Number of pages	4	APPROVED BY <i>D. J. J. J.</i>
Date of calibration	03 Feb 2026	NEXT CAL DATE..... 03/02/27

This calibration certificate may not be reproduced other than in full except with the permission of NSC-TISI-TIS-17025 and the issuing laboratory. Calibration certificates without signature are not valid.

The user is obliged to have the object recalibrated at appropriate intervals.

Date of issue	03 Feb 2026	Approval of the Calibration Certificate	Person in charge
		Mr. Chonchai Inthana	Chonchai Inthana

Calibration object

Single range instrument

Model	MSU224S-100-DU
Serial Number	31709552
QM Ident. no Inventory no.	RYG_EN0003 ---

Maximum capacity (Max. load)	220.0000 g
Measured up to	220.0000 g
Scale interval	0.0001 g

Place of calibration

Address	According to page 1
Department Cost center	Laboratory Department. ---
Building Floor	--- 1st Floor.
Room	Balance Room.
Maximum temperature variation at place of calibration	5 K

Calibration procedure

EURAMET Calibration Guide No. 18, Version 4.0 (11/2015) - Guidelines on the Calibration of Non-Automatic Weighing Instruments

Test equipment

Test equipment type	Test equipment ID	Valid until
Thermometer	Testo 174H H/T250743 (Traceable to Si unit through ENTECH)	18 Nov 2026
Test weight set OIML R111 E2	Certificate No.M2508149S ,E2(Traceable to SI unit through TCS)	19 Aug 2027

Adjustment Status

The measuring device was internally adjusted before the calibration.

Environmental and measuring conditions

Date of calibration	03 Feb 2026
Temperature at place of calibration Temp. diff. <i>T</i> _{weights} - <i>T</i> _{place}	24.5 °C 0.5 K
Measuring conditions	The installation site is suitable. The device is level. Balance was loaded up to Max before test.
Comments	Humidity 52.0 %RH.

Measurement results | Measurement uncertainties

Repeatability

Test load (nominal): 10 g 200 g		
	10 g	200 g
1	10.0000 g	200.0000 g
2	10.0000 g	200.0001 g
3	10.0000 g	200.0001 g
4	10.0001 g	200.0001 g
5	10.0000 g	200.0001 g
6	10.0000 g	200.0000 g
7	10.0000 g	200.0000 g
8	10.0000 g	200.0000 g
9	10.0000 g	200.0000 g
10	10.0000 g	200.0000 g
	<i>s</i> = 0.00003 g	<i>s</i> = 0.00005 g

Eccentricity

Test load (nominal): 100 g	
Center	100.0000 g
Front left	100.0000 g
Back left	99.9999 g
Back right	100.0000 g
Front right	100.0000 g
Maximum deviation from centric loading indication $ \Delta_{ecc} _{max} = 0.0001\text{ g}$	

Error of indication

Testload	Indication	Error	Expansion factor	Uncertainty	Uncertainty relative
<i>L</i>	<i>I</i>	<i>E</i>	<i>k</i>	<i>U</i> (<i>E</i>)	<i>U</i> _{rel} (<i>E</i>)
0.0100 g	0.0100 g	0.0000 g	2.00	0.00010 g	1.0 %
0.1000 g	0.1000 g	0.0000 g	2.00	0.00013 g	0.13 %
0.5000 g	0.5000 g	0.0000 g	2.00	0.00013 g	0.027 %
1.0000 g	1.0000 g	0.0000 g	2.00	0.00013 g	0.013 %
5.0000 g	5.0000 g	0.0000 g	2.00	0.00014 g	0.0027 %
10.0000 g	10.0000 g	0.0000 g	2.00	0.00014 g	0.0014 %
20.0000 g	20.0000 g	0.0000 g	2.00	0.00014 g	0.00071 %
50.0000 g	50.0001 g	0.0001 g	2.00	0.00015 g	0.00030 %
100.0000 g	100.0000 g	0.0000 g	2.00	0.00018 g	0.00018 %
200.0000 g	200.0000 g	0.0000 g	2.00	0.00028 g	0.00014 %
220.0000 g	220.0000 g	0.0000 g	2.00	0.00032 g	0.00015 %
Maximum error of indication		$ E _{max} = 0.0001\text{ g}$			

*U*_{rel}(*E*) is the quotient of *U*(*E*) and test load *L*. The uncertainty of measurement *U*(*E*) is valid only if error *E* is considered. You will find reference notes on the uncertainty of measurement in use under: Appendix to the calibration certificate | Interpretation of measurement results.
Reference note: The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the documented Expansion factor, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

End of calibration certificate

Uncertainty of measurement in use

Device adjusted before measurement	Yes
Temperature deviation considered	1.5 K (isoCAL active)
Temperature coefficient considered	$1 \cdot 10^{-6}/\text{K}$


Uncertainty of the weighing result $U_{gl}(W)$

$U_{gl}(W) = 0.00013 \text{ g} + 3.65 \cdot 10^{-6} \cdot R$

Reference note: The current uncertainty of measurement is calculated by entering of the reading R into this formula. In relation to this, there is no need for a correction of the indication error. The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied with an Expansion factor of 2, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

Indication in % from max load	Net indication R	Uncertainty $U_{gl}(W)$	Uncertainty relative $U_{gl}(W)_{rel}$
1 %	2.2000 g	0.00014 g	0.0063 %
25 %	55.0000 g	0.00033 g	0.00060 %
50 %	110.0000 g	0.00053 g	0.00048 %
75 %	165.0000 g	0.00073 g	0.00044 %
100 %	220.0000 g	0.00093 g	0.00042 %

Graphic realization of the relative uncertainty of measurement | process accuracy

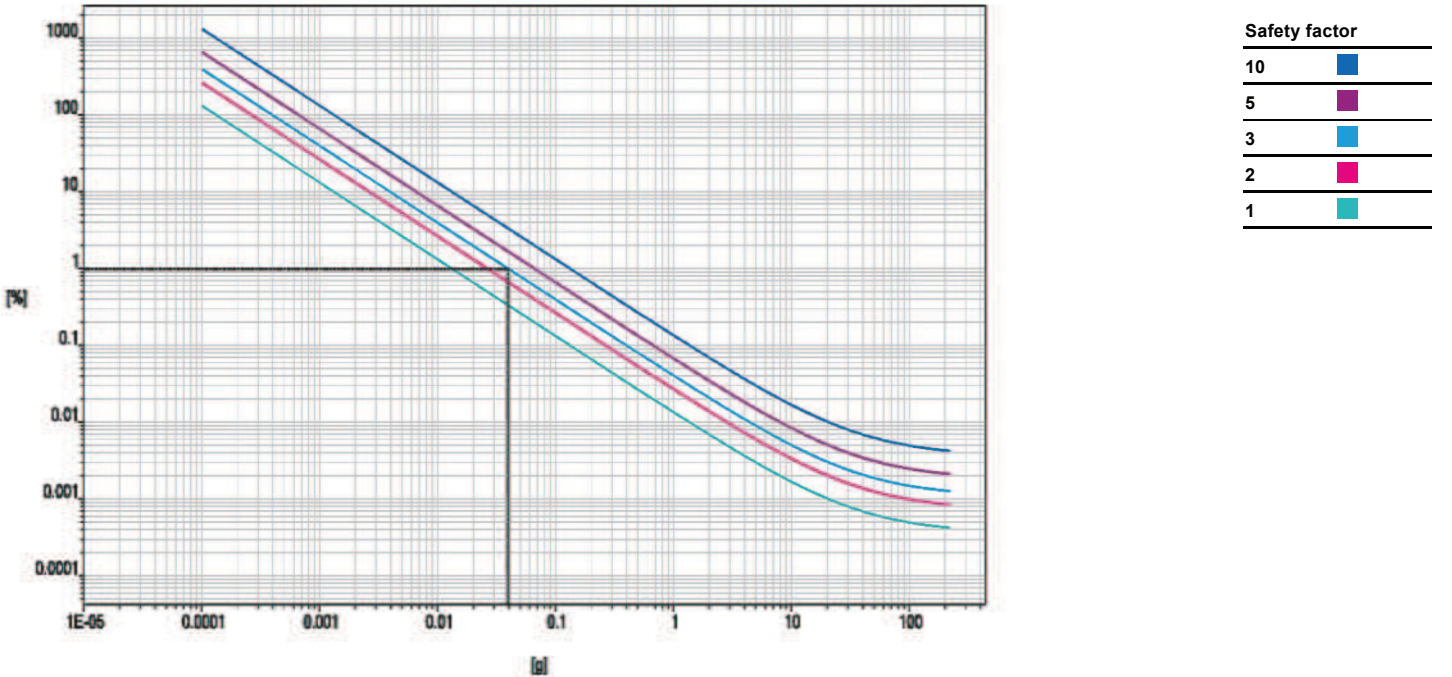

Displayed example

Process accuracy	1.00 %
Safety factor	3
Minimum sample weight	0.0395 g



Metrology Center
SCI ECO Services Company Limited

51 Moo 8, Tubkwang, Kaeng Khoi, Saraburi, Thailand 18260

Bangkok Tel : +668 9205 6851 , +669 81924 0059

Saraburi Tel : +669 8247 2360

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th



Certificate No. T252169

Page 1 of 3

Certificate of Calibration

Equipment : Liquid Bath (Water)

Manufacturer : Memmert

Model : WNE29

Serial No. : L623.0105

Customer Code : RYG_EN0220

ID No. : T5650A5

Customer : ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
616/10 Moo 5 T.Maenamkoo,
A.Pluakdaeng, Rayong 21140

Customer Location : Wet Chemistry Lab

Date of Receipt : 19 November 2025

Calibrated By : Sujjar Naknakred (Site Calibration Manager)

Approved By :  / Boonchai Suriyawong (Site Calibration Manager)

Date of Issue : 01 DEC 2025

REVIEW BY	Thavitall.
APPROVED BY	
NEXT CAL. DATE	27/11/26

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Certificate No. T252169

Page 2 of 3

Calibration Report

Equipment : Liquid Bath (Water)
Date of Calibration : 27 November 2025
Environment : Temperature : 25.5-25.7 °C
Line Voltage : 221.8-225.5 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert five resistance thermometer detectors into its water bath , the other one thermocouple type T use for ambient temperature measurement . The calibration was done in according to WI-T36 (based on ASTM E715-80 (Reapproved 2022)).

All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
RTD	100 OHM	M18 (CH1-CH5)	T251758	17 October 2026
DATA LOGGER	34970A	T261	T251758	17 October 2026

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

Equipment Description :

Time Constant 1 Hour 3 Minute At 63 °C

5. Adjustment :

(X) without adjustment

() after adjustment


Approved By. _____

Certificate No. T252169


Page 3 of 3

Calibration Report

Side View

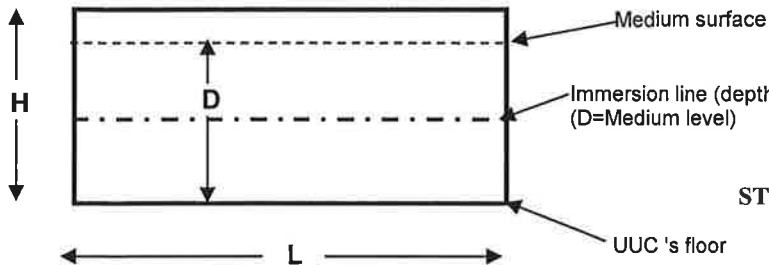

Top View

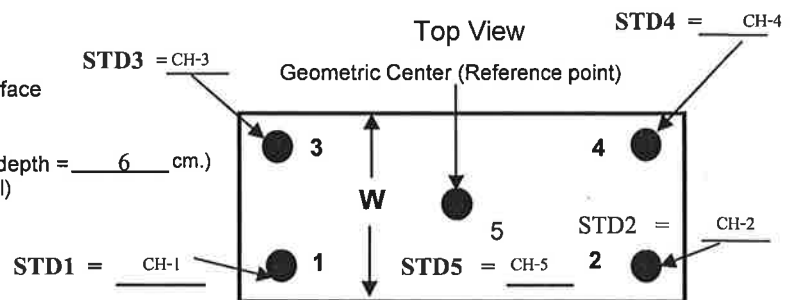

● 1 ~ ● 5 = Position of Working standards

- D = Medium level : 12 cm.

Working space dimension : 59 × 35 × 14 (WxLxH)

- UUC 's medium : Water

- Working standards are located at 2.5 cm. away from each corner and walls.

Measurement Results:

Calibration Point	Average Standard Reading at each position (° C)				
	CH-1	CH-2	CH-3	CH-4	CH-5
63	62.93	63.13	62.94	63.10	63.09
85	85.15	85.33	85.21	85.43	85.20

Liquid Bath (Water)			Temperature Distribution				
Setting (° C)	Reading (° C)		Average (° C)	Stability (± ° C)	Uniformity (± ° C)	Uncertainty (± ° C)	Coverage Factor <i>k</i>
	Min , Max	Average					
63.0	62.9 , 63.1	63.0	63.04	0.08	0.17	0.27	2.06
85.0	84.8 , 85.2	85.0	85.26	0.13	0.24	0.43	2.23


* The quoted uncertainty exclude "uniformity"

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

End of Certificate.

Approved By. 



Certificate of Calibration

Cert.No.: 25CH847

Page.: 1 of 3

Equipment : pH Meter
Manufacturer : Mettler Toledo
Model : SevenCompact S220
Serial No. : C104059460
ID No. : RYG_EN0183
Condition As-Received: Used Item
Received Date : 17 July 2025
Calibration Date : 18 July 2025
Reference : 2507-0561DSC-3
Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
Rayong Branch
616/10 Moo 5, T.Maenam Khu,
A.Pluakdaeng, Rayong 21140, Thailand

Ambient Temperature : $(25 \pm 2.5) ^\circ\text{C}$
Relative Humidity : $(50 \pm 15) \%$
Calibration Procedure : In - house method :
- CP-CH5 by direct measurement with DC voltage
standard and direct measurement with
certified reference material (CRM)
- CP-CH8 by comparison with temperature standard

Calibrated by : Walalak Sirithean

Approved by :

Saithip

Approved Signatory

() Chakrit Waewwanjua

() Ponpan Paipim

(✓) Saithip Meangmai

Issue Date : 21 July 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Cert.No.: 25CH847

Page.: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Document Process Calibrator	54030049	130RC116	24E2759	25 Aug 2025
2) Ref. Standard Thermometer	3240076	60RC033	25I394	01 Apr 2026

- This measurement result is traceable to SI through Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.007	CPA chem	1066665	18 Jan 2027
pH 6.965	CPA chem	1066667	18 Jan 2026
pH 10.010	CPA chem	1114385	08 June 2026

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4,7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (±mV)	Coverage factor <i>k</i>
	pH	mV	mV	pH		
pH Meter S/N.: C104059460	4.000	177.48	177.3	4.000	0.058	2.00
	7.000	0.00	-0.2	7.000	0.058	2.00
	10.000	-177.48	-177.6	10.000	0.058	2.00



Cert.No.: 25CH847

Page.: 3 of 3

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement ($\pm$)	Coverage factor k
pH Electrode S/N.: 5240606	4.007	4.008	184.6	0.0044	2.00
	6.965	6.966	10.2	0.0084	2.00
	10.010	10.009	-164.9	0.0065	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : InLabExpert Pro-ISM

- Serial No. : 5240606

Dimension of probe

- Length : 120 mm.

- Diameter : 12 mm.

- Immersion Depth : 100 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement ($\pm$ °C)	Coverage factor k
25.0	25.001	25.0	-0.001	0.13	2.00

Remark - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484



Certificate of Calibration

Certificate No. : 25E2372

Page : 1 of 2

Equipment : pH Meter
Manufacturer: Mettler Toledo
Model : SevenCompact S220
Serial No.: C104059460
ID No.: RYG_EN0183

Condition As-Received: Used Item

Received Date: 17 July 2025

Calibration Date: 22 July 2025

Reference: 2507-0561DSC

Ambient Temperature: (23 ± 2) °C

Relative Humidity: (50 ± 10) %

This certificate may not be reproduced other than in full,
except with the prior written approval of the head of
Corporate Services 3: Equipment Calibration and Testing Services.

Submitted by: ALS Laboratory Group (Thailand) Co.,Ltd. Rayong Branch

616/10 Moo 5, T.Maenam Khu, A.Pluakdaeng,
Rayong 21140, Thailand

Procedure used: Calibration were conducted using calibration procedure No. CP-E17 according to EURAMET cg-15.

Condition of this result of calibration

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Multi-Product Calibrator	5500A	6315011	25E1627	19 May 2026

2.This result of calibration was made on requested at the point specified by customer.

3.The certificate is valid only to the item calibrated on date and place of calibration.

4.This measurement result is traceable to the International System of Unit maintained through:-

-Technology Promotion Association (Thailand-Japan), NSC-ONSC Accredited No. Calibration 0008

Calibrated by : Napachanok Prasomsoosiri
Issue Date : 23 July 2025

Approved Signatory : _____

[] Phalinee Prabpaipal

[] Nuntawat Khamchai

[✓] Pongsagorn Boonyaporn



Cert. No.: 25E2372

Page.: 2 of 2

Result of calibration :- (*) Without adjustment () After adjustment

Function: DC voltage measurement

Range:

2000

mV

<u>Standard Value</u>	<u>UUC* Reading</u>	<u>Error</u>	<u>Uncertainty</u>
(mV)	(mV)	(mV)	($\pm$ μ V)
-200.0000	-200.0	0.0	68
-150.0000	-150.0	0.0	65
-100.0000	-100.0	0.0	63
-50.0000	-50.0	0.0	61
0.0000	0.0	0.0	58
50.0000	49.9	-0.1	61
100.0000	99.9	-0.1	63
150.0000	149.9	-0.1	65
200.0000	199.9	-0.1	68

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95 %

UUC* = Unit Under Calibration.

-o0o-

Accredited by

NSC-TISI-TIS 17025

Calibration 0426



Calibration certificate

Calibration Certificate No. 25BKL0002

Object	Electronic non-automatic weighing instrument	This calibration certificate documents the traceability to national standards.
Manufacturer	Sartorius	Uncertainties of measurements are taken into account when only statements of compliance are made.
Type	MCE224S-2S00-U	This certificate was prepared by Sartorius Corporation in accordance to the current ISO/IEC 17025:2017 standard and Sartorius Work Instruction (Method) SOP WI 08.
Serial QM Ident. no.	38101399 RYG_EN0163	This certificate relate and apply this equipment only.
Customer	ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)	
	616/10 Moo 5 T.Maenam Khu, A.Pluak Daeng, Rayong 21140, Thailand.	
Order no.	2230	
Number of pages	4	
Date of calibration	20 Feb 2025	

REVIEW BY *Thanitak.*APPROVED BY *D. Khunon.*NEXT CAL DATE *20/02/26*

This calibration certificate may not be reproduced other than in full except with the permission of NSC-TISI-TIS-17025 and the issuing laboratory. Calibration certificates without signature are not valid.

The user is obliged to have the object recalibrated at appropriate intervals.

Date	06 Mar 2025	Approval of the Calibration Certificate	Person in charge
		Mr. Chonchai Inthana	Kachen Lalee

Calibration object

Single range instrument

Model	MCE224S-2S00-U
Serial Number	38101399
QM Ident. no Inventory no.	RYG_EN0163 ---

Maximum capacity (Max. load)	220.0000 g
Measured range	220.0000 g
Scale interval	0.0001 g

Place of calibration

Address	According to page 1
Department Cost center	Laboratory Department. ---
Building Floor	--- 1st Floor.
Room	Balance Room.
Maximum temperature variation at place of calibration	5 K

Calibration procedure

EURAMET cg-18, V4.0 - Guidelines on the Calibration of Non-Automatic Weighing Instruments

Test equipment

Test equipment type	Test equipment ID	Valid until
Thermometer	MHB-382SD s/nB011342 Traceable to SI unit through DKSH	21 Aug 2025
Test weight set OIML R111 E2	Certificate No.M2308197S ,E2(Traceable to SI unit through TCS)	23 Aug 2025

Adjustment Status

The measuring device was internally adjusted before the calibration.

Environmental and measuring conditions

Date of calibration	20 Feb 2025
Temperature at place of calibration Temp. diff. <i>T</i> _{weights} - <i>T</i> _{place}	24.4 °C 0.6 K
Measuring conditions	The installation site is suitable. The device was levelled. Balance was loaded up to Max before test.
Comments	Humidity 58.0 %RH.

Measurement results | Measurement uncertainties

Repeatability

Test load (nominal): 10 g 200 g		
	10 g	200 g
1	10.0000 g	200.0000 g
2	10.0000 g	200.0000 g
3	10.0000 g	200.0001 g
4	9.9999 g	200.0000 g
5	9.9999 g	200.0000 g
6	10.0000 g	200.0001 g
7	10.0000 g	200.0000 g
8	10.0000 g	200.0000 g
9	9.9999 g	200.0001 g
10	10.0000 g	200.0000 g
	<i>s</i> = 0.00005 g	<i>s</i> = 0.00005 g

Eccentricity

Test load (nominal): 100 g	
Center	100.0000 g
Front left	100.0000 g
Back left	100.0000 g
Back right	100.0000 g
Front right	99.9999 g
Maximum deviation from centric loading indication $ \Delta_{ecc} _{max} = 0.0001\text{ g}$	

Error of indication

Testload	Indication	Error	Expansion factor	Uncertainty	Uncertainty relative
<i>L</i>	<i>I</i>	<i>E</i>	<i>k</i>	<i>U</i> (<i>E</i>)	<i>U</i> _{rel} (<i>E</i>)
0.0100 g	0.0100 g	0.0000 g	2.00	0.00013 g	1.3 %
0.1000 g	0.1000 g	0.0000 g	2.00	0.00013 g	0.13 %
0.5000 g	0.5000 g	0.0000 g	2.00	0.00013 g	0.026 %
1.0000 g	1.0000 g	0.0000 g	2.00	0.00013 g	0.013 %
5.0000 g	5.0000 g	0.0000 g	2.00	0.00013 g	0.0026 %
10.0000 g	9.9999 g	-0.0001 g	2.00	0.00013 g	0.0013 %
20.0000 g	20.0000 g	0.0000 g	2.00	0.00014 g	0.00068 %
50.0000 g	50.0001 g	0.0001 g	2.00	0.00015 g	0.00029 %
100.0000 g	100.0000 g	0.0000 g	2.00	0.00018 g	0.00018 %
200.0000 g	200.0000 g	0.0000 g	2.00	0.00028 g	0.00014 %
220.0000 g	220.0000 g	0.0000 g	2.00	0.00032 g	0.00015 %
Maximum error of indication		$ E _{max} = 0.0001\text{ g}$			

*U*_{rel}(*E*) is the quotient of *U*(*E*) and test load *L*. The uncertainty of measurement *U*(*E*) is valid only if error *E* is considered. You will find reference notes on the uncertainty of measurement in use under: Appendix to the calibration certificate | Interpretation of measurement results.
Reference note: The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the documented Expansion factor, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

End of calibration certificate

Uncertainty of measurement in use

Device adjusted before measurement	Yes
Temperature deviation considered	1.5 K (isoCAL active)
Temperature coefficient considered	$1 \cdot 10^{-6}/\text{K}$


Uncertainty of the weighing result $U_{gl}(W)$

$U_{gl}(W) = 0.00013 \text{ g} + 1.16 \cdot 10^{-5} \cdot R$

Reference note: The current uncertainty of measurement is calculated by entering of the reading R into this formula. In relation to this, there is no need for a correction of the indication error. The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied with an Expansion factor of 2, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

Indication in % from max load	Net indication R	Uncertainty $U_{gl}(W)$	Uncertainty relative $U_{gl}(W)_{rel}$
1 %	2.2000 g	0.00016 g	0.0071 %
25 %	55.0000 g	0.00077 g	0.0014 %
50 %	110.0000 g	0.0014 g	0.0013 %
75 %	165.0000 g	0.0020 g	0.0012 %
100 %	220.0000 g	0.0027 g	0.0012 %

Graphic realization of the relative uncertainty of measurement | process accuracy

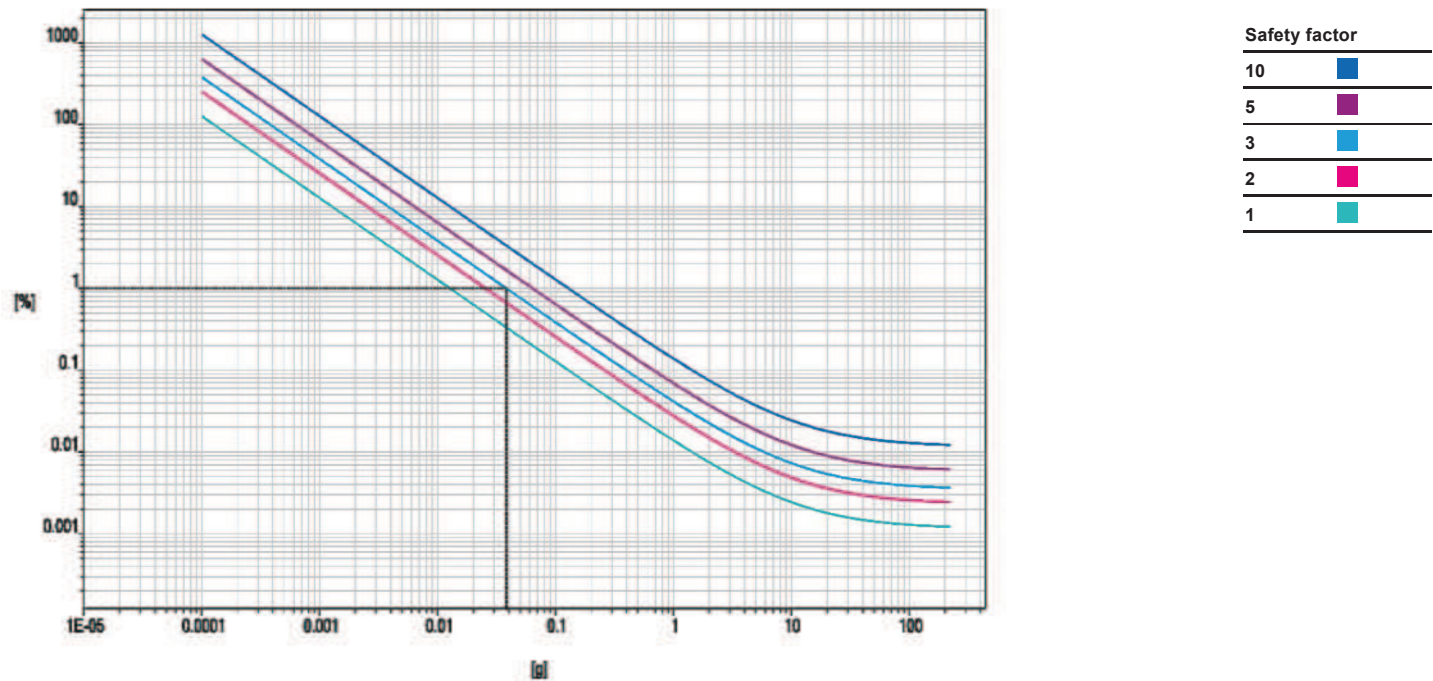

Displayed example

Process accuracy	1.00 %
Safety factor	3
Minimum sample weight	0.0381 g

Accredited by

NSC-TISI-TIS 17025

Calibration 0426



Calibration certificate

Calibration Certificate No. 26BCI0064

Object	Electronic non-automatic weighing instrument	This calibration certificate documents the traceability to national standards.
Manufacturer	Sartorius	Uncertainties of measurements are taken into account when only statements of compliance are made.
Type	MCE224S-2S00-U	This certificate was prepared by Sartorius Corporation in accordance to the current ISO/IEC 17025:2017 standard and Sartorius Work Instruction (Method) SOP WI 08.
Serial QM Ident. no.	38101399 RYG_EN0163	This certificate relate and apply this equipment only.
Customer	ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)	
	616/10 Moo 5 T.Maenamkoo, A.Pluak Daeng, Rayong 21140, Thailand.	
Order no.	278579	REVIEW BY <i>Thanita K.</i>
Number of pages	4	APPROVED BY <i>D. Johnson</i>
Date of calibration	03 Feb 2026	NEXT CAL DATE..... 03/02/27

This calibration certificate may not be reproduced other than in full except with the permission of NSC-TISI-TIS-17025 and the issuing laboratory. Calibration certificates without signature are not valid.

The user is obliged to have the object recalibrated at appropriate intervals.

Date of issue	03 Feb 2026	Approval of the Calibration Certificate	Person in charge
			
		Mr. Chonchai Inthana	Chonchai Inthana

Calibration object

Single range instrument

Model	MCE224S-2S00-U
Serial Number	38101399
QM Ident. no Inventory no.	RYG_EN0163 ---

Maximum capacity (Max. load)	220.0000 g
Measured up to	220.0000 g
Scale interval	0.0001 g

Place of calibration

Address	According to page 1
Department Cost center	Laboratory Department. ---
Building Floor	--- 1st Floor.
Room	Balance Room.
Maximum temperature variation at place of calibration	5 K

Calibration procedure

EURAMET Calibration Guide No. 18, Version 4.0 (11/2015) - Guidelines on the Calibration of Non-Automatic Weighing Instruments

Test equipment

Test equipment type	Test equipment ID	Valid until
Thermometer	Testo 174H H/T250743 (Traceable to Si unit through ENTECH)	18 Nov 2026
Test weight set OIML R111 E2	Certificate No.M2508149S ,E2(Traceable to SI unit through TCS)	19 Aug 2027

Adjustment Status

The measuring device was internally adjusted before the calibration.

Environmental and measuring conditions

Date of calibration	03 Feb 2026
Temperature at place of calibration Temp. diff. <i>T</i> _{weights} - <i>T</i> _{place}	25 °C 0.5 K
Measuring conditions	The installation site is suitable. The device is level. Balance was loaded up to Max before test.
Comments	Humidity 49.0 %RH.

Measurement results | Measurement uncertainties

Repeatability

Test load (nominal): 10 g 200 g		
	10 g	200 g
1	10.0000 g	200.0000 g
2	10.0000 g	199.9999 g
3	10.0000 g	200.0000 g
4	10.0000 g	200.0001 g
5	9.9999 g	199.9999 g
6	10.0000 g	200.0000 g
7	10.0000 g	199.9999 g
8	10.0000 g	200.0000 g
9	9.9999 g	200.0001 g
10	10.0000 g	200.0000 g
	<i>s</i> = 0.00004 g	<i>s</i> = 0.00007 g

Eccentricity

Test load (nominal): 100 g	
Center	100.0001 g
Front left	100.0002 g
Back left	100.0002 g
Back right	100.0000 g
Front right	100.0000 g
Maximum deviation from centric loading indication $ \Delta_{ecc} _{max} = 0.0001\text{ g}$	

Error of indication

Testload	Indication	Error	Expansion factor	Uncertainty	Uncertainty relative
<i>L</i>	<i>I</i>	<i>E</i>	<i>k</i>	<i>U</i> (<i>E</i>)	<i>U</i> _{rel} (<i>E</i>)
0.0100 g	0.0100 g	0.0000 g	2.00	0.00012 g	1.2 %
0.1000 g	0.1000 g	0.0000 g	2.00	0.00017 g	0.17 %
0.5000 g	0.5000 g	0.0000 g	2.00	0.00017 g	0.034 %
1.0000 g	1.0000 g	0.0000 g	2.00	0.00017 g	0.017 %
5.0000 g	5.0000 g	0.0000 g	2.00	0.00017 g	0.0034 %
10.0000 g	10.0000 g	0.0000 g	2.00	0.00017 g	0.0017 %
20.0000 g	20.0000 g	0.0000 g	2.00	0.00018 g	0.00088 %
50.0000 g	50.0000 g	0.0000 g	2.00	0.00018 g	0.00037 %
100.0000 g	100.0001 g	0.0001 g	2.00	0.00021 g	0.00021 %
200.0000 g	200.0000 g	0.0000 g	2.00	0.00030 g	0.00015 %
220.0000 g	220.0001 g	0.0001 g	2.00	0.00034 g	0.00015 %
Maximum error of indication		$ E _{max} = 0.0001\text{ g}$			

*U*_{rel}(*E*) is the quotient of *U*(*E*) and test load *L*. The uncertainty of measurement *U*(*E*) is valid only if error *E* is considered. You will find reference notes on the uncertainty of measurement in use under: Appendix to the calibration certificate | Interpretation of measurement results.
Reference note: The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the documented Expansion factor, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

End of calibration certificate

Uncertainty of measurement in use

Device adjusted before measurement	Yes
Temperature deviation considered	1.5 K (isoCAL active)
Temperature coefficient considered	$1 \cdot 10^{-6}/\text{K}$


Uncertainty of the weighing result $U_{gl}(W)$

$U_{gl}(W) = 0.00017 \text{ g} + 4.25 \cdot 10^{-6} \cdot R$

Reference note: The current uncertainty of measurement is calculated by entering of the reading R into this formula. In relation to this, there is no need for a correction of the indication error. The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied with an Expansion factor of 2, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

Indication in % from max load	Net indication R	Uncertainty $U_{gl}(W)$	Uncertainty relative $U_{gl}(W)_{rel}$
1 %	2.2000 g	0.00018 g	0.0082 %
25 %	55.0000 g	0.00040 g	0.00073 %
50 %	110.0000 g	0.00064 g	0.00058 %
75 %	165.0000 g	0.00087 g	0.00053 %
100 %	220.0000 g	0.0011 g	0.00050 %

Graphic realization of the relative uncertainty of measurement | process accuracy

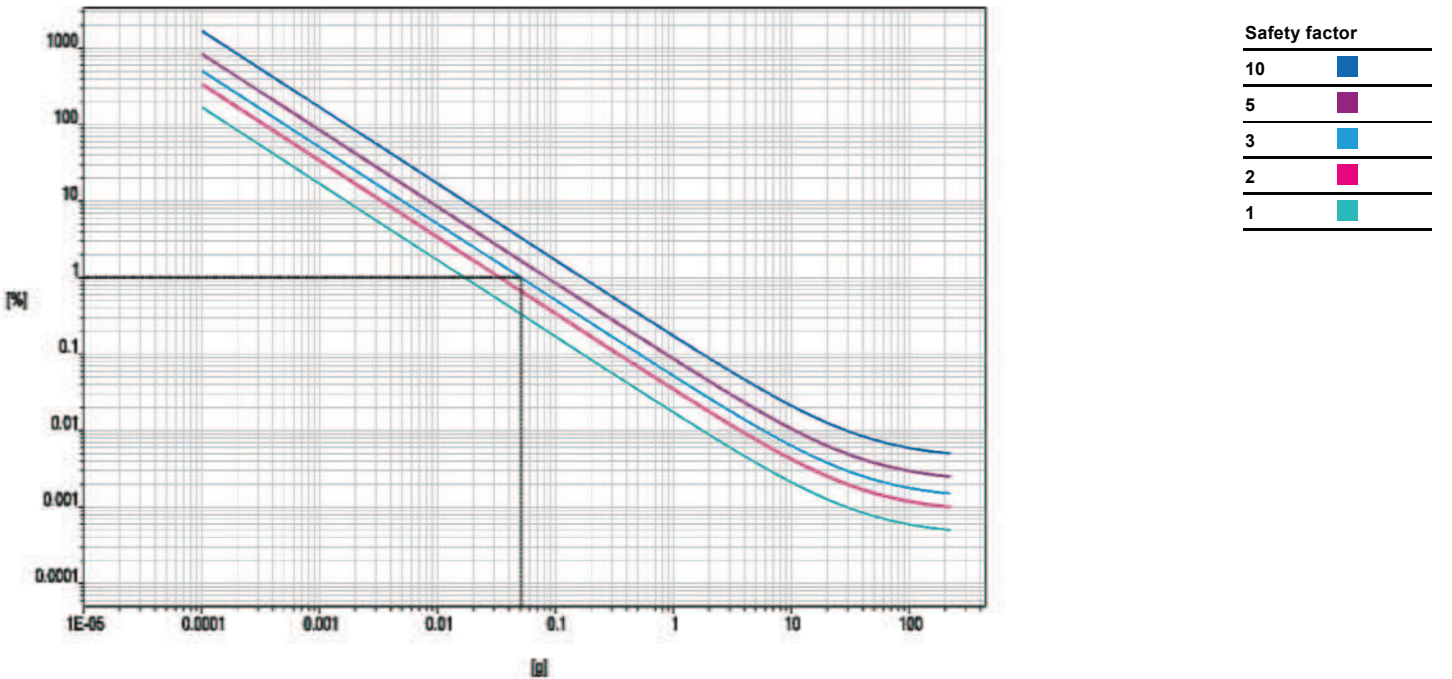

Displayed example

Process accuracy	1.00 %
Safety factor	3
Minimum sample weight	0.0507 g


Certificate No. T251530

Page 1 of 3

Certificate of Calibration**Equipment** : Chamber (Oven)**Manufacturer** : MEMMERT**Model** : UF 110**Serial No.** : B416.2420**Customer Code** : RYG_EN0012**ID No.** : T6444A5**Customer** : ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)

616/10 Moo 5 T.Maenamkoo,

A.Pluakdaeng, Rayong 21140

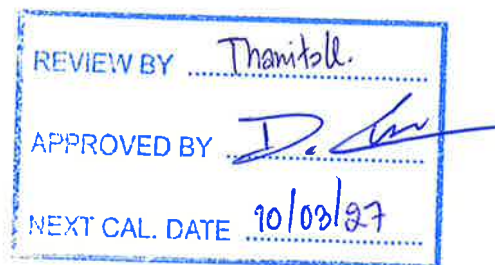Customer Location : ENVIRONMENT LABORATORY**Date of Receipt** : 3 September 2025**Calibrated By** : Sujjar Naknakred (Site Calibration Manager)**Approved By** :  Boonchai Suriyawong (Site Calibration Manager)**Date of Issue** : 17 SEP 2025**The uncertainties are for a confidence probability of approximately 95%.**

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Certificate No. T251530

Page 2 of 3

Calibration Report

Equipment : Chamber (Oven)
Date of Calibration : 10 September 2025
Environment : Temperature : 35.7-36.6 °C
Line Voltage : 226.8-233.7 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert nine resistance thermometer detectors into its chamber , the other one resistance thermometer detector use for ambient temperature measurement . The calibration was done in according to WI-T20 (based on ASTM E145-94 (Reapproved 2019) and AS2853-1986).

All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
RTD	100 ohm	30-(CH1-10)	T242203	9 November 2025
DATA LOGGER	34970A	T47	T242203	9 November 2025

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.

4. Condition of calibrated item : good

Equipment Description :

Time Constant 3 Hour 29 Minute At 104 °C

Fresh Air Damper ☒ Open ☒ Min ☐ Medium ☐ Max

☐ Close

☐ Not Available

5. Adjustment :


() without adjustment

(X) after adjustment

Approved By. _____



Calibration Report

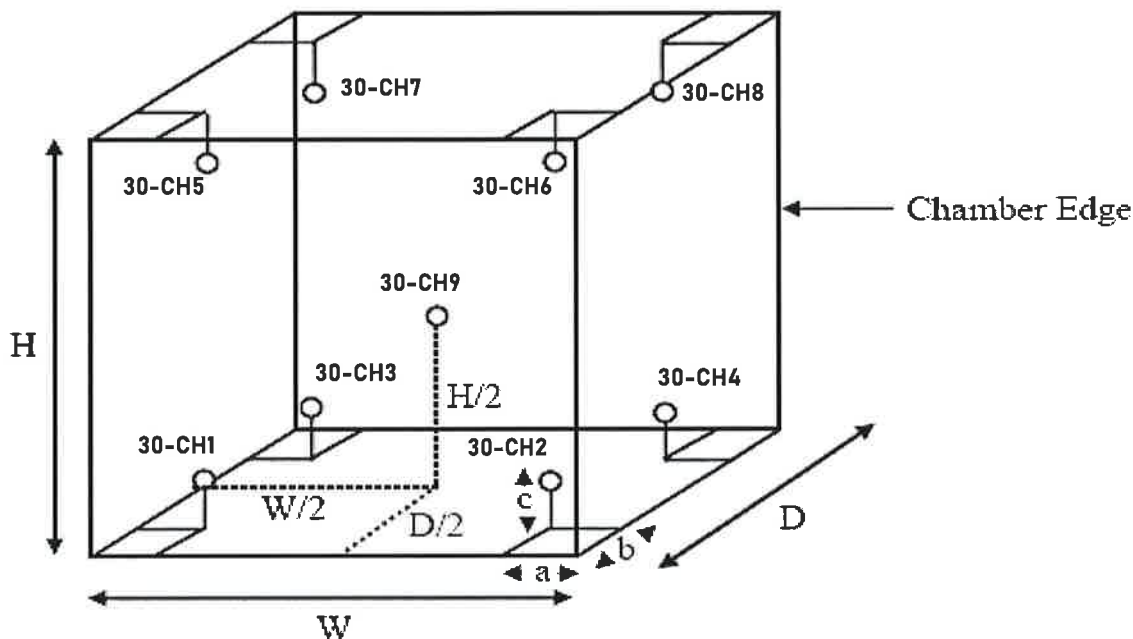

Remark : Internal Dimensions of Chamber : W (Width) = 56 cm. , H (Height) = 48 cm. and D (Depth) = 40 cm.
 Size of Installed Standard sensor number 30-CH1 to number 30-CH8 : a = 5 cm. ,b = 5 cm. and c = 5 cm.
 Size of Installed Standard sensor number 30-CH9 : W/2 = 56 cm./2 , H/2 = 48 cm./2 and D/2 = 40cm./2

Measurement Results

Average Standard Reading at each position (°C)									
Calibration Point	30-CH1	30-CH2	30-CH3	30-CH4	30-CH5	30-CH6	30-CH7	30-CH8	30-CH9
104	104.02	103.70	104.01	104.16	104.11	104.08	104.01	104.33	103.61
180	180.67	178.78	180.38	179.85	179.16	180.27	180.98	181.04	179.49

Chamber (Oven)			Temperature Distribution				
Setting °C	Reading (°C)		Average (°C)	Stability (± °C)	Uniformity (°C)	Uncertainty (± °C)	Coverage Factor k
	Min , Max	Average					
104.0	103.9 , 104.1	104.0	104.00	0.08	0.61	0.42	2.00
180.0	179.9 , 180.1	180.0	180.07	0.21	1.51	0.52	2.00

* The quoted uncertainty exclude "uniformity"

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k which for a t-distribution, providing a level of confidence of approximately 95 % .

End of Certificate.

Approved By. _____





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484



Certificate of Calibration

Certificate No. : 25T1631

Page : 1 of 2

Equipment : Digital Thermometer With Sensor

Manufacturer: Testo

Model : 106

Serial No.: 31129895/202

ID No.: RYG_FS0466

Condition As-Received: Used Item

Received Date: 30 September 2025

Calibration Date: 09 October 2025
to 17 October 2025

Reference: 2509-1019DSC

Ambient Temperature: (25 ± 3) °C

Relative Humidity: (50 ± 20) %

This certificate may not be reproduced other than in full,
except with the prior written approval of the head of
Corporate Services 3: Equipment Calibration and Testing Services.

Submitted by: ALS Laboratory Group (Thailand) Co.,Ltd. Rayong Branch

616/10 Moo 5 T.Maenamkoo, A.Pluakdaeng, Rayong 21140,
Thailand

Procedure used: Calibration were conducted using in-house calibration procedure CP-T01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into liquid bath temperature controller.
The temperature scale used was based on ITS-90.

Condition of this result of calibration

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Black Stack Thermometer	1560	8C454	25I625	06 Jun 2026
2) PRT Scanner Module	2562	A01303	25I625	06 Jun 2026
3) Industrial Platinum Resistance Thermometer	5627-12	571971	25I625	06 Jun 2026

2.The certificate is valid only to the item calibrated on date and place of calibration.

3.This measurement result is traceable to the International System of Unit maintained through:-

-Technology Promotion Association (Thailand-Japan), NSC-ONSC Accredited No. Calibration 0008

REVIEW BY	Pitthaya T.
APPROVED BY	Supt S.
NEXT CAL DATE	09/10/26

Calibrated by : Theerapong Ameen

Issue Date : 20 October 2025

Approved Signatory :

[] Phalinee Prabpaipal

[] Chatchawan Khunpiluek

[✓] Wanlop Larpkern



Cert. No.: 25T1631

Page.: 2 of 2

Result of Calibration:-

Without Adjustment

Function:

Temperature measurement

Dimension of probe : Diameter 3 mm Length 55 mm Sheath material : Stainless Steel

Immersion	Standard	UUC*		Uncertainty
<u>Depth</u>	<u>Temperature</u>	<u>Reading</u>	<u>Error</u>	<u>of Measurement</u>
(mm)	(°C)	(°C)	(°C)	(±°C)
50	25.0039	24.9	-0.1039	0.12
50	44.9961	45.0	0.0039	0.12

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

-o0o-

ภาคผนวก จ

สำเนาหนังสืออนุญาตขึ้นทะเบียน
ห้องปฏิบัติการวิเคราะห์เอกชน

ที่อก ๐๓๑๐(๑)/ ๑๖๑๖๘



กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๒๐ พฤศจิกายน ๒๕๖๖

เรื่อง ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๔ สิงหาคม ๒๕๖๖

- สิ่งที่ส่งมาด้วย ๑. รายชื่อผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๑ แผ่น
๒. รายชื่อเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๕ แผ่น
๓. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๓๑ แผ่น

ตามหนังสือที่อ้างถึง บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ขอต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๒๐๔ สถานที่ตั้งเลขที่ ๑๐๔ ซอยพัฒนาการ ๔๐ ถนนพัฒนาการ แขวงพัฒนาการ เขตสวนหลวง กรุงเทพมหานคร ต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน โดยมีองค์ประกอบดังนี้

- ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๖ ราย ตามสิ่งที่ส่งมาด้วย ๑
ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ ๑๘๑ ราย ตามสิ่งที่ส่งมาด้วย ๒
ค. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนให้วิเคราะห์ในน้ำเสีย น้ำใต้ดิน อากาศเสีย สิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว และดิน ตามสิ่งที่ส่งมาด้วย ๓

หนังสือฉบับนี้จะหมดอายุในวันที่ ๒ กันยายน ๒๕๖๙ หากประสงค์จะต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ให้ยื่นคำขอต่ออายุพร้อมเอกสารประกอบคำขอต่อกรมโรงงานอุตสาหกรรม ภายใน ๓๐ วัน ก่อนวันสิ้นสุดอายุของหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ทั้งนี้ สามารถยื่นคำขอผ่านระบบอิเล็กทรอนิกส์ได้ที่หน้าเว็บไซต์กรมโรงงานอุตสาหกรรม

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายสิระ จันทร์เจ็ด)

นักวิทยาศาสตร์เชี่ยวชาญ วิชาการราชการแทน
ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน

กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ

โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕

โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๔๙

ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th



“อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา อุตสาหกรรมสีเขียว”



เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด เลขทะเบียน ว-๒๐๔
ที่ ออก ๐๓๑๐(๑)/ ๑ ๖ ๑ ๖ ๘ ลงวันที่ ๒๐ พฤศจิกายน ๒๕๖๖

ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๖ ราย

- | | |
|--------------------------------|----------------------------|
| ๑) นางสาวยุพาพร จันทรเปล่ง | ทะเบียนเลขที่ ว-๒๐๔-ค-๐๐๐๑ |
| ๒) นางสาวชัชชัย โกมารกุล ณ นคร | ทะเบียนเลขที่ ว-๒๐๔-ค-๐๐๐๒ |
| ๓) นายศรายุทธ จิตรานนท์ | ทะเบียนเลขที่ ว-๒๐๔-ค-๐๐๐๓ |
| ๔) นางสาวนกกร เอนก | ทะเบียนเลขที่ ว-๒๐๔-ค-๐๐๐๔ |
| ๕) นายสุริยา สอนแก้ว | ทะเบียนเลขที่ ว-๒๐๔-ค-๐๐๐๕ |
| ๖) นายวิชาญ ชุณหะวัณ | ทะเบียนเลขที่ ว-๒๐๔-ค-๐๐๐๖ |

วิมล

เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

เลขทะเบียน ว-๒๐๔

ที่ ออก ๐๓๑๐(๑)/ ๑๖๑๖๘

ลงวันที่ ๒๐ พฤศจิกายน ๒๕๖๖

ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๑๘๑ ราย

๑) นายกาจบัณฑิต กิตติคุณวิชัย	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๐๑
๒) นายภัทรพล สว่างใจธรรม	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๐๒
๓) นายนราธิป เทือกชัยคำ	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๐๓
๔) นายศิริโชค พงษ์ประสม	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๐๔
๕) นายณัฐวุฒิ ดั่งแพง	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๐๕
๖) นางสาวจินดา ไชจุลธรรม	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๐๖
๗) นางสาวสาวิตรี น้อยเสงี่ยม	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๐๗
๘) นางสาวชนัญญาญจน์ อัมมขม	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๐๘
๙) นางสาวนรินทร์ สายเส็ง	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๐๙
๑๐) นางสาวนันทวดี สมบูรณ์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๑๐
๑๑) นางสาวศรณิยา เฉลิมธารงค์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๑๑
๑๒) นางสาวธัญญธร มงคลจิรวุฒิ	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๑๒
๑๓) นางสาวศิริลักษณ์ บุญนา	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๑๓
๑๔) นายพนพงค์ จันทุพันธุ์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๑๔
๑๕) นายนรเศรษฐ์ โกมลาลัย	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๑๕
๑๖) นายธันวา จริยา	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๑๖
๑๗) นางสาวเกศรินทร์ แก้วมัน	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๑๗
๑๘) นางสาวสุวิมล ชัยเรืองวุฒิ	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๑๘
๑๙) นางสาวสุชาดา ธรรมถาวร	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๑๙
๒๐) นางสาวเปมิกา ชัยเดชธนกุล	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๒๐
๒๑) นางสาวศศิธร หมูสวัสดิ์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๒๑
๒๒) นางสาวเสาวลักษณ์ ภูณภาพพร	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๒๒
๒๓) นายอภิสิทธิ์ สิงหา	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๒๓
๒๔) นายศักดิ์สิทธิ์ ไพศาลพิสุทธิ	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๒๔
๒๕) ว่าที่ร้อยตรีหญิง พรรณิภา ขำเจริญ	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๒๕
๒๖) นางจิตตา คำภูแก้ว	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๒๖
๒๗) นางสาวอรรวรรณ รักยง	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๒๗
๒๘) นางสาวนพรัตน์ แยมกรานต์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๒๘
๒๙) นายจุลเดช วารินทร์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๒๙
๓๐) นางสาวดาญรัตน์ ร้องคำ	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๓๐
๓๑) นายพรมมี ศรีปัดเนตร	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๓๑
๓๒) นายอุทิศ อุ่นสีม	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๓๒
๓๓) ว่าที่ร้อยตรี เฉลิมเกียรติ อมรศรีเสริม	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๓๓
๓๔) นางสาววริยา สร้างนา	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๓๔
๓๕) นายอนุพงศ์ รัตนศรีประเสริฐ	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๓๕



๓๖) นางสาวจุฑารัตน์...

๓๖) นางสาวจุฑารัตน์ โอนสันเทียะ
๓๗) นางสาวจารุวรรณ พิมพ์อภิฤติยา
๓๘) นางสาวปรางค์ทิพย์ กิจไพศาลศักดิ์
๓๙) นางสาวเดือนใจ ทางกลาง
๔๐) นางสาวจิราพร ศิริเวช
๔๑) นายวรากร ผูกרך
๔๒) นายทง วิริยะสทกิจ
๔๓) นายธนิศ เจนจบ
๔๔) นายคณิศร ขำเพชร
๔๕) นายภูวิช พรหมสะอาด
๔๖) นายธนเดช โกศาพิพัฒน์
๔๗) นายชวฤทธิ์ วงษ์จันทร์
๔๘) นายอาทิตย์ ศรีเสน
๔๙) นายเจษดินทร์ คงศักดิ์ไทย
๕๐) นายจรัส บุญยั้ง
๕๑) นายธนาณัติ เอนก
๕๒) นายอภิวัฒน์ ทุมหนู
๕๓) นางสาวสุภาขวัญ มาก
๕๔) นางสาวหัตถพร ขวาลสมบุรณ์
๕๕) นางสาวธิตีมา บุญเพ็ง
๕๖) นางสาวภานุมาศ นามวัฒน์
๕๗) นางสาวอุไรรัตน์ ทังสร้างแป้น
๕๘) นายธีรวัฒน์ ปวงสุข
๕๙) นายอิทธิพล ยะโส
๖๐) นายประพจน์ วรรณชูชัย
๖๑) นายชยธร พวงทิพย์
๖๒) นางสาวกนกวรรณ จันทบาล
๖๓) นายสิทธิโชค ธงเงิน
๖๔) นางศิวาวรรณ ใจบุญ
๖๕) นางสาวพรรณธิดา พุ่มคง
๖๖) นายนวกัทร ศรีวิริยะ
๖๗) นายสุวิชา ทองอ่อน
๖๘) นายวิญญู บุญตะนัย
๖๙) นายสมบุรณ์ บุตรจันทร์
๗๐) นายวิรัตน์ ไชยนระรา
๗๑) นายณฤเบศน์ เพิ่มพูน
๗๒) นายจิรณัฐ ขาวละออ
๗๓) นายอัสนี นามบุรี
๗๔) นายอัศวเรศ จ่อสา

ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๓๖
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๓๗
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๓๘
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๓๙
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๔๐
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๔๑
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๔๒
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๔๓
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๔๔
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๔๕
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๔๖
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๔๗
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๔๘
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๔๙
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๕๐
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๕๑
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๕๒
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๕๓
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๕๔
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๕๕
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๕๖
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๕๗
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๕๘
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๕๙
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๐
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๑
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๒
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๓
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๔
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๕
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๖
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๗
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๘
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๙
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๗๐
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๗๑
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๗๒
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๗๓
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๗๔

37/1

๗๕) นายประเสริฐ สุระขันธุ์
๗๖) นายอนุกุล จันทน์เนียม
๗๗) นายพิรพงษ์ ทองคุณปรีดา
๗๘) นายณฤพล ทองนุช
๗๙) นายอนุวัฒน์ ม่วงแพ
๘๐) นายเจตศราวุฒิ ปัตตะมะ
๘๑) นายกฤษณะ สายวรรณ
๘๒) นายพิชัย บุญยงค์
๘๓) นายภาณุพงศ์ โสมวงศ์
๘๔) นายสามารถ คุ่มปลี
๘๕) นายสัญญาชัย โกศรีนาม
๘๖) นายณัฐวุฒิ ศรีประเสริฐ
๘๗) นายชวัลธัช นาคพนม
๘๘) นายพงศธร ชัยทิพย์
๘๙) นายสิทธิโชค ทาสีดา
๙๐) นายธนากร อินสุตา
๙๑) นางสาววรรณิษา ชาตวันชัย
๙๒) นางสาวพิมพ์ตะวัน มินากุล
๙๓) นางสาวเพชรรัตน์ สิงห์สมบุญ
๙๔) นางสาวชญานิษฐ์ พรหมจันทร์
๙๕) นายกীরติ ทวีราช
๙๖) นายจักริน หมั่นวิชา
๙๗) นายฉัตรชัย สุขเปี้ย
๙๘) นายณรรณท์ ต๊ะทองคำ
๙๙) นายศุภผล สนนอก
๑๐๐) นายทักษ์ดนัย อุบลศรี
๑๐๑) นายธนศวรร นามะกฤษณา
๑๐๒) นายธิตพิงค์ บัวแดง
๑๐๓) นายนนทชัย อุปถัมภ์
๑๐๔) นายณัฐพล คุณสุทธิ
๑๐๕) นายณัฏฐวัฒน์ สาริน
๑๐๖) นายปิยะนัฐ พลมะศรี
๑๐๗) นายพงศ์สิริ โสมเขียว
๑๐๘) นายพีรพัฒน์ กำคำ
๑๐๙) นายภาณุพงศ์ มานิตย์
๑๑๐) นายมงคล ผลาทิพย์
๑๑๑) นายสิรินันท์ ทองอ้น
๑๑๒) นายอเนชา ทันสมัย
๑๑๓) นายอดิศักดิ์ ผมไผ

ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๗๕
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๗๖
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๗๗
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๗๘
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๗๙
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๘๐
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๘๑
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๘๒
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๘๓
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๘๔
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๘๕
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๘๖
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๘๗
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๘๘
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๘๙
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๙๐
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๙๑
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๙๒
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๙๓
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๙๔
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๙๕
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๙๖
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๙๗
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๙๘
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๙๙
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๐
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๑
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๒
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๓
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๔
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๕
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๖
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๗
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๘
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๙
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๑๐
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๑๑
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๑๒
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๑๓

รวม

๑๑๔) นายอนันตชัย...

๑๑๔) นายอนันตชัย วิสม
๑๑๕) นายวรวิธ ตีนัก
๑๑๖) นายแสงตะวัน นະตะสັต
๑๑๗) นายยุทธพงศ์ รัตนะ
๑๑๘) นายชัยวัฒน์ ไชยชนะนิจ
๑๑๙) นายวิศรุต ศรีธรรมมา
๑๒๐) นายณนทกร เผือกผ่อง
๑๒๑) นายกำชัย สุทธะ
๑๒๒) นางสาวณัฐภรณ์ บุญตะนัย
๑๒๓) นางสาวพัชรินทร์ แสนสร้อย
๑๒๔) นายไพรวลัย เปี่ยมพิมาย
๑๒๕) นางสาวศุภมาศ ทองมาก
๑๒๖) นางสาวลลิตา จิตรสว่าง
๑๒๗) นางสาวไมพร เสิกภูเขียว
๑๒๘) นางสาวกฤติมาพร คำมีแก่น
๑๒๙) นางสาวสกุลรัตน์ ภาคภูมิ
๑๓๐) นางสาวไพรินทร์ ศรีรูปี
๑๓๑) นางสาวทิพนเตร ผุยปัญญา
๑๓๒) นางสาวสาธิตา ปานทอง
๑๓๓) นางสาวอริสา ทองนวล
๑๓๔) นางสาวอรยา คำคล้อง
๑๓๕) นางสาวชุตาภรณ์ สุนทรสนาน
๑๓๖) นางสาวอัญชลี คำจันทร์
๑๓๗) นายบุญฤทธิ์ เอี่ยมเทศ
๑๓๘) นางสาวศุภรดา บันมยุรา
๑๓๙) นางสาวพาฤดี คุณนาน
๑๔๐) นางสาวจิราเจต ฟองดา
๑๔๑) นางสาวอารยา มีชัย
๑๔๒) นางสาววิษุตา นาคผจญ
๑๔๓) นางสาวนันทิยา จันทะสุน
๑๔๔) นายกิตติพงศ์ แซ่ลี
๑๔๕) นายอนวัติ ภูถวิล
๑๔๖) นายธีรพล แสงทอง
๑๔๗) นายศักดิ์พิพัฒน์ บุญมัน
๑๔๘) นายฐิติวัลด์ เอมอุไร
๑๔๙) นายชัยณรงค์ ศรีบุรินทร์
๑๕๐) นางสาวอัจฉราวรรณ สอนสนอง
๑๕๑) นางสาวณัฐพร สิงหา
๑๕๒) นายกัมเรศ แหยมโต

ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๑๔
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๑๕
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๑๖
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๑๗
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๑๘
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๑๙
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๒๐
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๒๑
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๒๒
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๒๓
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๒๔
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๒๕
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๒๖
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๒๗
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๒๘
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๒๙
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๐
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๑
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๒
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๓
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๔
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๕
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๖
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๗
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๘
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๙
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๔๐
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๔๑
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๔๒
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๔๓
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๔๔
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๔๕
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๔๖
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๔๗
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๔๘
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๔๙
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๕๐
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๕๑
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๕๒

31/๑๖

๑๕๓) นางสาวอุบล...

๑๕๓) นางสาวอุบล เคิกศิริ
๑๕๔) นางสาวมโนรัตน์ ทองบุตร
๑๕๕) นายภาคภูมิ แทนไทย
๑๕๖) นางสาวสุภาณัฐ เมล์พวง
๑๕๗) นางสาวพรทิศา สาดาชนม์
๑๕๘) นายเอกวิทย์ วันทะนา
๑๕๙) นายไตรมณฑล ทิพย์วรรณ
๑๖๐) นายจิรเมธ ประเสริฐสิริพงศ์
๑๖๑) นายจิรายุส เกษมสุข
๑๖๒) นายจิรศักดิ์ ศรีวิชัย
๑๖๓) นายณัฐกฤษณ์ สะพานแก้ว
๑๖๔) นายบุญศักดิ์ ปะที
๑๖๕) นายปณณวิทย์ เสมอทรัพย์
๑๖๖) นายพิษณุพงษ์ ไชยา
๑๖๗) นายภัทรพงษ์ มณฑาทอง
๑๖๘) นายวสันต์ ตรีนกุล
๑๖๙) นายภาณุเดช เพชรอุด
๑๗๐) นายอนุกุล วิละแสง
๑๗๑) นายภัทรพงษ์ มีสุข
๑๗๒) นางสาวนุชรี ลีละทีป
๑๗๓) นางสาวสุภาวดี โกศรีนาม
๑๗๔) นางสาวอรณิข เทียนคำ
๑๗๕) นางสาวพรเพ็ญ ชอบสอน
๑๗๖) นางสาววันวิสา ขอนพิกุล
๑๗๗) นางสาวอรรณณ เถาว์ทอง
๑๗๘) นางสาวอัยยลีน เมอร์วิณณ์
๑๗๙) นางสาววิสรา ค่อยครอง
๑๘๐) นายวุฒิกร ศิริวรรณ
๑๘๑) นางสาวจรรวรรณ กระจำงพันธุ์

ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๕๓
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๕๔
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๕๕
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๕๖
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๕๗
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๕๘
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๕๙
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๐
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๑
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๒
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๓
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๔
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๕
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๖
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๗
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๘
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๙
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๗๐
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๗๑
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๗๒
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๗๓
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๗๔
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๗๕
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๗๖
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๗๗
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๗๘
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๗๙
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๘๐
ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๘๑

วิมล

เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด เลขทะเบียน ว-๒๐๔

ที่ อก ๐๓๑๐(๑)/ ๑๖๑๖๘ ลงวันที่ ๒๐ พฤศจิกายน ๒๕๖๖

ค. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๓๗๔ รายการ

น้ำเสีย จำนวน 60 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Aldicarb	High-Performance Liquid Chromatographic Method ^[4]
2	Aldicarb Sulfone	High-Performance Liquid Chromatographic Method ^[4]
3	Aldicarb Sulfoxide	High-Performance Liquid Chromatographic Method ^[4]
4	Aldrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
5	Arsenic	1) Digestion, Inductively Coupled Plasma Method ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4]
6	Barium	1) Digestion, Inductively Coupled Plasma Method ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4]
7	α -BHC	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
8	β -BHC	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
9	δ -BHC	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
10	γ -BHC	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
11	Biochemical Oxygen Demand	1) 5-Day BOD Test, Azide Modification Method ^[4] 2) 5-Day BOD Test, Membrane Electrode Method ^[4]
12	Carbaryl	High-Performance Liquid Chromatographic Method ^[4]
13	Carbofuran	High-Performance Liquid Chromatographic Method ^[4]
14	Cadmium	1) Digestion, Inductively Coupled Plasma Method ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4]
15	Chemical Oxygen Demand	1) Closed Reflux, Colorimetric Method ^[4] 2) Closed Reflux, Titrimetric Method ^[4]
16	Chlordane	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
17	Chromium	1) Digestion, Inductively Coupled Plasma Method ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4]
18	Color	ADMI Weighted-Ordinate Spectrophotometric Method ^[4]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
19	Copper	1) Digestion, Inductively Coupled Plasma Method ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4]
20	Cyanide	Distillation, Colorimetric Method ^[4]
21	2,4'-DDD	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
22	4,4'-DDD	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
23	2,4'-DDE	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
24	4,4'-DDE	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
25	2,4'-DDT	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
26	4,4'-DDT	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
27	Dieldrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
28	Endosulfan Sulfate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
29	Endosulfan I	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
30	Endosulfan II	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
31	Endrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
32	Endrin Aldehyde	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
33	Formaldehyde	Distillation, Colorimetric Method ^[3]
34	Free Chlorine	1) DPD Ferrous Titrimetric Method ^[4] 2) DPD Colorimetric Method ^[4]
35	Heptachlor	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
36	Heptachlor Epoxide	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
37	Hexavalent Chromium	Colorimetric Method ^[4]
38	3-Hydroxycarbofuran	High-Performance Liquid Chromatographic Method ^[4]
39	Lead	1) Digestion, Inductively Coupled Plasma Method ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4]

Small

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
40	Manganese	1) Digestion, Inductively Coupled Plasma Method ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4]
41	Mercury	1) Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass spectrometric Method ^[4]
42	Methiocarb	High-Performance Liquid Chromatographic Method ^[4]
43	Methoxychlor	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
44	Methomyl	High-Performance Liquid Chromatographic Method ^[4]
45	Nickel	1) Digestion, Inductively Coupled Plasma Method ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4]
46	Oil & Grease	1) Liquid-Liquid, Partition-Gravimetric Method ^[4] 2) Soxhlet Extraction Method ^[4]
47	Oxamyl	High-Performance Liquid Chromatographic Method ^[4]
48	Propoxur	High-Performance Liquid Chromatographic Method ^[4]
49	pH	Electrometric Method ^[4]
50	Phenols	1) Distillation, Chloroform Extraction Method ^[4] 2) Distillation, Direct Photometric Method ^[4]
51	Selenium	1) Digestion, Inductively Coupled Plasma Method ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4]
52	Sulfide	Iodometric Method ^[4]
53	Temperature	Laboratory and Field Methods ^[4]
54	Total Dissolved Solids	Dried at 180 °C ^[4]
55	Total Kjeldahl Nitrogen	Semi-Micro Kjeldahl Method ^[4]
56	Total Phosphorous	Digestion, Colorimetric Method ^[4]
57	Total Suspended Solids	Dried from 103-105 °C ^[4]
58	Toxaphene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
59	Trivalent Chromium	1) Digestion, Inductively Coupled Plasma Method; Colorimetric Method; Calculation ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method; Colorimetric Method; Calculation ^[4]
60	Zinc	1) Digestion, Inductively Coupled Plasma Method ^[4] 2) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[4]

วิมล

น้ำใต้ดิน จำนวน 126 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Acenaphthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
2	Acetone	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
3	Aldrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
4	Anthracene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
5	Antimony	1) Digestion, Inductively Coupled Plasma Method ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4]
6	Arsenic	1) Digestion, Inductively Coupled Plasma Method ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4]
7	Atrazine	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
8	Barium	1) Digestion, Inductively Coupled Plasma Method ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4]
9	Benz(a)anthracene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
10	Benzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
11	Benzo(b)fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
12	Benzo(k)fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
13	Benzoic Acid	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
14	Benzo(a)pyrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
15	Benzo[g,h,i]perylene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
16	Beryllium	1) Digestion, Inductively Coupled Plasma Method ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4]
17	Bis(2-chloroethyl)ether	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
18	Bis(2-ethylhexyl)phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
19	Bromodichloromethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
20	Bromoform	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
21	Butanol	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
22	Butyl benzyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
23	Cadmium	1) Digestion, Inductively Coupled Plasma Method ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4]
24	Carbazole	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
25	Carbon disulfide	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
26	Carbon tetrachloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
27	Chlordane	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
28	p-Chloroaniline	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
29	Chlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
30	Chlorodibromomethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
31	Chloroform	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
32	2-Chlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
33	Chromium	1) Digestion, Inductively Coupled Plasma Method ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4]
34	Chromium (III)	1) Digestion, Inductively Coupled Plasma Method; Colorimetric Method; Calculation ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method; Colorimetric Method; Calculation ^[4]
35	Chromium (VI)	Colorimetric Method ^[4]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
36	Chrysene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
37	Cyanide	Distillation, Colorimetric Method ^[4]
38	2,4-D	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
39	DDD	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
40	DDE	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
41	DDT	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
42	Dibenz(a,h)anthracene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
43	Di-n-Butyl Phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
44	1,2-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
45	1,3-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
46	1,4-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
47	3,3-Dichlorobenzidine	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
48	1,1-Dichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
49	1,2-Dichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
50	1,1-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
51	cis-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
52	trans-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
53	2,4-Dichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
54	1,2-Dichloropropane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
55	1,3-Dichloropropane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]

3m

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
56	1,3-Dichloropropene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
57	Dieldrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
58	Diethyl Phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
59	2,4-Dimethylphenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
60	2,4-Dinitrophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
61	2,4-Dinitrotoluene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
62	2,6-Dinitrotoluene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
63	Di-n-octyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
64	Endosulfan	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
65	Endrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
66	Ethylbenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
67	Fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
68	Fluorene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
69	Heptachlor	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
70	Heptachlor epoxide	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
71	Hexachlorobenzene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
72	Hexachloro-1,3-butadiene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
73	n-Hexane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
74	α-HCH	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
75	β-HCH	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]

3m2

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
76	γ-HCH	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
77	Hexachlorocyclopentadiene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
78	Hexachloroethane	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
79	Indeno(1,2,3-cd)pyrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
80	Isophorone	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
81	Lead	1) Digestion, Inductively Coupled Plasma Method ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4]
82	Manganese	1) Digestion, Inductively Coupled Plasma Method ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4]
83	Mercury	1) Digestion, Cold Vapor Atomic Absorption Spectrometric Method ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4]
84	Methanol	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
85	Methoxychlor	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
86	Methyl bromide	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
87	Methylene chloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
88	2-Methylphenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
89	2-Methylnaphthalene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
90	Methyl tert-butyl Ether	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
91	Naphthalene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
92	Nickel	1) Digestion, Inductively Coupled Plasma Method ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4]
93	Nitrobenzene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
94	N-Nitrosodiphenylamine	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
95	N-Nitrosodi-n-Propylamine	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
96	Polychlorinated Biphenyls - PCB 1016 - PCB 1221 - PCB 1232 - PCB 1242 - PCB 1248 - PCB 1254 - PCB 1260	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
97	Pentachlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
98	pH	Electrometric Method ^[4]
99	Phenanthrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
100	Phenol	1) Distillation, Chloroform Extraction Method ^[4] 2) Distillation, Direct Photometric Method ^[4] 3) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
101	Pyrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
102	Selenium	1) Digestion, Inductively Coupled Plasma Method ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4]
103	Silver	1) Digestion, Inductively Coupled Plasma Method ^[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4]
104	Styrene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
105	1,1,2,2-Tetrachloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
106	Tetrachloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
107	Toluene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[4]
108	Toxaphene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[4]
109	TPH (C ₅ -C ₈)	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[14,25]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
110	TPH (C ₈ -C ₁₆)	Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^[9,22]
111	TPH (C ₁₆ -C ₃₅)	Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method ^[9,22]
112	1,2,4-Trichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
113	1,1,1-Trichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
114	1,1,2-Trichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
115	Trichloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
116	2,4,5-Trichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
117	2,4,6-Trichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[4]
118	1,3,5-Trimethylbenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
119	Vanadium	1) Digestion, Inductively Coupled Plasma Method ^[4] 2) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[4]
120	Vinyl acetate	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
121	Vinyl chloride	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
122	m-Xylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
123	o-Xylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
124	p-Xylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
125	Xylene (Total)	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method ^[4]
126	Zinc	1) Digestion, Inductively Coupled Plasma Method ^[4] 2) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[4]

3/11/25

อากาศเสีย (ปล่อยระบาย) จำนวน 28 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Antimony	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[5]
2	Arsenic	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[5]
3	Beryllium	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[5]
4	Cadmium	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[5]
5	Carbon Monoxide	1) Instrumental Analyzer Method ^[5] 2) Sampling Bag Non-Dispersive Infrared Method ^[5]
6	Chlorine	1) Absorption Sampling, Ion Chromatographic Method ^[5] 2) Isokinetic Sampling, Ion Chromatographic Method ^[5]
7	Chromium	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[5]
8	Cobalt	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[5]
9	Copper	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[5]
10	Cresol	Adsorption Sampling, Gas Chromatographic Method ^[5]
11	Dioxins	Isokinetic Sampling ^[5]
12	Hydrogen Chloride	1) Absorption Sampling, Ion Chromatographic Method ^[5] 2) Isokinetic Sampling, Ion Chromatographic Method ^[5]
13	Hydrogen Fluoride	1) Absorption Sampling, Ion Chromatographic Method ^[5] 2) Isokinetic Sampling, Ion Chromatographic Method ^[5]
14	Hydrogen Sulfide	Absorption Sampling, Iodometric Method ^[5]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
15	Lead	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
16	Manganese	2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[5]
17	Mercury	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
18	Nickel	2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[5]
19	Opacity	1) Isokinetic Sampling, Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^[5]
20	Oxides of Nitrogen	2) Isokinetic Sampling, Digestion, Cold-Vapor Atomic Fluorescence Spectrometric Method ^[5]
21	Selenium	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
22	Sulfur Dioxide	2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[5]
23	Sulfuric Acid	1) Absorption Sampling, Phenoldisulfonic Acid Method ^[5]
24	Tellurium	2) Absorption Sampling, Alkaline Permanganate/Colorimetric Method ^[5]
25	Tin	3) Instrumental Analyzer Method ^[5]
26	Total Suspended Particulate	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
		2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[5]
		1) Absorption Sampling, Barium-Thorin Titrimetric Method ^[5]
		2) Instrumental Analyzer Method ^[5]
		Isokinetic Sampling, Barium-Thorin Titrimetric Method ^[5]
		1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
		2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[5]
		1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
		2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[5]
		1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5]
		2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[5]
		1) Isokinetic Sampling, Gravimetric Method ^[5]
		2) Paired Train, Isokinetic Sampling, Gravimetric Method ^[5]

3mml

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
27	Vanadium	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method ^[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[5]
28	Xylene	Adsorption Sampling, Gas Chromatographic Method ^[5]

สิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว จำนวน 35 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Aldrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1,9,26] 2) Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[11,26]
2	Antimony	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,6,17] 3) Digestion, Inductively Coupled Plasma Method ^[7,16] 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[7,17]
3	Arsenic	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,6,17] 3) Digestion, Inductively Coupled Plasma Method ^[7,16] 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[7,17]
4	Barium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,6,17] 3) Digestion, Inductively Coupled Plasma Method ^[7,16] 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[7,17]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
5	Beryllium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,6,17] 3) Digestion, Inductively Coupled Plasma Method ^[7,16] 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[7,17]
6	Cadmium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,6,17] 3) Digestion, Inductively Coupled Plasma Method ^[7,16] 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[7,17]
7	Chlordane	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1,9,26] 2) Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[11,26]
8	Chromium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,6,17] 3) Digestion, Inductively Coupled Plasma Method ^[7,16] 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[7,17]
9	Chromium (III)	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method; Waste Extraction, Colorimetric Method; Calculation Method ^[1,6,16,19] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method; Waste Extraction, Colorimetric Method; Calculation Method ^[1,6,17,19] 3) Digestion, Inductively Coupled Plasma Method; Alkaline Digestion, Colorimetric Method; Calculation Method ^[7,8,16,19] 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method; Alkaline Digestion, Colorimetric Method; Calculation Method ^[7,8,17,19]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
10	Chromium (VI)	1) Waste Extraction, Colorimetric Method ^[1,6,19] 2) Alkaline Digestion, Colorimetric Method ^[8,19]
11	Cobalt	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,6,17] 3) Digestion, Inductively Coupled Plasma Method ^[7,16] 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[7,17]
12	Copper	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,6,17] 3) Digestion, Inductively Coupled Plasma Method ^[7,16] 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[7,17]
13	2,4-D	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1,9,26] 2) Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[11,26]
14	DDD	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1,9,26] 2) Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[11,26]
15	DDE	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1,9,26] 2) Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[11,26]
16	DDT	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1,9,26]

amal

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
17	Dieldrin	2) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26] 1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1,9,26]
18	Endrin	2) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26] 1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1,9,26]
19	Heptachlor	2) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26] 1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1,9,26]
20	Lead	2) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26] 1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,6,17] 3) Digestion, Inductively Coupled Plasma Method ^[7,16]
21	Lindane	4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[7,17] 1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1,9,26] 2) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
22	Mercury	1) Waste Extraction, Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^[1,6,20] 2) Waste Extraction, Digestion, Cold-Vapor Atomic Fluorescence Spectrometric Method ^[1,6,30] 3) Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^[20] 4) Digestion, Cold-Vapor Atomic Fluorescence Spectrometric Method ^[30] 5) Thermal Decomposition Amalgamation and Atomic Absorption Spectrometric Method ^[21]
23	Methoxychlor	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1,9,26] 2) Soxhlet Extraction, Gas Chromatographic / Mass Spectrometric Method ^[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic / Mass Spectrometric Method ^[11,26]
24	Mirex	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1,9,26] 2) Soxhlet Extraction, Gas Chromatographic / Mass Spectrometric Method ^[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic / Mass Spectrometric Method ^[11,26]
25	Molybdenum	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,6,17] 3) Digestion, Inductively Coupled Plasma Method ^[7,16] 4) Digestion, Inductively Coupled Plasma / Mass Spectrometric Method ^[7,17]
26	Nickel	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,6,17] 3) Digestion, Inductively Coupled Plasma Method ^[7,16] 4) Digestion, Inductively Coupled Plasma / Mass Spectrometric Method ^[7,17]
27	Polychlorinated biphenyls (PCBs) - Aroclor 1016 - Aroclor 1221 - Aroclor 1232 - Aroclor 1242 - Aroclor 1248 - Aroclor 1254 - Aroclor 1260	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1,9,26] 2) Soxhlet Extraction, Gas Chromatographic Method ^[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic Method ^[11,26]

3m


ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
	- 2-Chlorobiphenyl - 2,3-Dichlorobiphenyl - 2,2',5-Trichlorobiphenyl - 2,4',5-Trichlorobiphenyl - 2,2',3,5'-Tetrachlorobiphenyl - 2,2',5,5'-Tetrachlorobiphenyl - 2,3',4,4'-Tetrachlorobiphenyl - 2,2',3,4,5'-Pentachlorobiphenyl - 2,2',4,5,5'-Pentachlorobiphenyl - 2,3,3',4',6-Pentachlorobiphenyl - 2,2',3,4,4',5'-Hexachlorobiphenyl - 2,2',3,4,5,5'-Hexachlorobiphenyl - 2,2',3,5,5',6-Hexachlorobiphenyl - 2,2',4,4',5,5'-Hexachlorobiphenyl - 2,2',3,3',4,4',5-Heptachlorobiphenyl - 2,2',3,4,4',5,5'-Heptachlorobiphenyl - 2,2',3,4,4',5',6-Heptachlorobiphenyl - 2,2',3,4',5,5',6-Heptachlorobiphenyl - 2,2',3,3',4,4',5,5',6-Nonachlorobiphenyl	
28	Pentachlorophenol	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1,9,26] 2) Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[11,26]
29	pH	Electrometric Method ^[23,24]
30	Selenium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,6,17] 3) Digestion, Inductively Coupled Plasma Method ^[7,16] 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[7,17]

31

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
31	Silver	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,6,17] 3) Digestion, Inductively Coupled Plasma Method ^[7,16] 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[7,17]
32	Thallium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,6,17] 3) Digestion, Inductively Coupled Plasma Method ^[7,16] 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[7,17]
33	Toxaphene	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method ^[1,9,26] 2) Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method ^[11,26]
34	Vanadium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,6,17] 3) Digestion, Inductively Coupled Plasma Method ^[7,16] 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[7,17]
35	Zinc	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,6,17] 3) Digestion, Inductively Coupled Plasma Method ^[7,16] 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[7,17]

31/10/2554

ดิน จำนวน 125 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Acenaphthene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
2	Acetone	1) Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25] 2) Equilibrium Headspace, Gas Chromatographic/ Mass Spectrometric Method ^[13]
3	Aldrin	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
4	Anthracene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
5	Antimony	1) Digestion, Inductively Coupled Plasma Method ^[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[7,17]
6	Arsenic	1) Digestion, Inductively Coupled Plasma Method ^[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[7,17]
7	Atrazine	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
8	Barium	1) Digestion, Inductively Coupled Plasma Method ^[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[7,17]
9	Benz(a)anthracene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
10	Benzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25] 

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
11	Benzo(b)fluoranthene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
12	Benzo(k)fluoranthene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
13	Benzoic acid	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
14	Benzo(a)pyrene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
15	Benzo(g,h,i)perylene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
16	Beryllium	1) Digestion, Inductively Coupled Plasma Method ^[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[7,17]
17	Bis(2-chloroethyl)ether	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
18	Bis(2-ethylhexyl)phthalate	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
19	Bromodichloromethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
20	Bromoform	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
21	Butanol	Equilibrium Headspace, Gas Chromatographic/ Mass Spectrometric Method ^[13,25]
22	Butyl Benzyl Phthalate	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]

สม

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
23	Cadmium	1) Digestion, Inductively Coupled Plasma Method ^[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[7,17]
24	Carbazole	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
25	Carbon Disulfide	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
26	Carbon tetrachloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
27	Chlordane	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
28	p-Chloroaniline	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
29	Chlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
30	Chlorodibromomethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
31	Chloroform	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
32	2-Chlorophenol	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
33	Chromium	1) Digestion, Inductively Coupled Plasma Method ^[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[7,17]
34	Chromium (III)	1) Digestion, Inductively Coupled Plasma Method; Alkaline Digestion, Colorimetric Method; Calculation Method ^[7,8,16,19] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method; Alkaline Digestion, Colorimetric Method; Calculation Method ^[7,8,17,19]
35	Chromium (VI)	Alkaline Digestion, Colorimetric Method ^[8,19]

3mrd

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
36	Chrysene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
37	Cyanide	Extraction, Distillation, Colorimetric Method ^[27,28,29]
38	2,4-D	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
39	DDD	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
40	DDE	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
41	DDT	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
42	Dibenz(a,h)anthracene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
43	Di-n-Butyl Phthalate	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
44	1,2-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
45	1,3-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
46	1,4-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
47	3,3-Dichlorobenzidine	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
48	1,1-Dichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]

Smel

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
49	1,2-Dichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
50	1,1-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
51	cis-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
52	trans-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
53	2,4-Dichlorophenol	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
54	1,2-Dichloropropane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
55	1,3-Dichloropropane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
56	1,3-Dichloropropene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
57	Dieldrin	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
58	Diethyl Phthalate	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
59	2,4-Dimethylphenol	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
60	2,4-Dinitrophenol	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
61	2,4-Dinitrotoluene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
62	2,6-Dinitrotoluene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]

Signature

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
63	Di-n-Octyl Phthalate	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
64	Endosulfan	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
65	Endrin	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
66	Ethylbenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
67	Fluoranthene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
68	Fluorene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
69	Heptachlor	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
70	Heptachlor epoxide	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
71	Hexachlorobenzene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
72	Hexachloro-1,3-butadiene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
73	n-Hexane	1) Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25] 2) Equilibrium Headspace, Gas Chromatographic/ Mass Spectrometric Method ^[13]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
74	α -HCH	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
75	β -HCH	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
76	γ -HCH	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
77	Hexachlorocyclopentadiene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
78	Hexachloroethane	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
79	Indeno(1,2,3-cd)pyrene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
80	Isophorone	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
81	Lead	1) Digestion, Inductively Coupled Plasma Method ^[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[7,17]
82	Manganese	1) Digestion, Inductively Coupled Plasma Method ^[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[7,17]
83	Mercury	1) Digestion, Cold-Vapor Atomic Absorption Spectrometric Method ^[20] 2) Thermal Decomposition, Amalgamation, and Atomic Absorption Spectrophotometry ^[21] 3) Digestion, Cold-Vapor Atomic Fluorescence Spectrometric Method ^[30]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
84	Methanol	1) Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25] 2) Equilibrium Headspace, Gas Chromatographic/ Mass Spectrometric Method ^[13,25]
85	Methoxychlor	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
86	Methyl Bromide	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
87	Methylene Chloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
88	2-methylphenol	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
89	2-Methylnaphthalene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
90	Methyl tert-Butyl Ether	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
91	Naphthalene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
92	Nickel	1) Digestion, Inductively Coupled Plasma Method ^[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[7,17]
93	Nitrobenzene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
94	N-Nitrosodiphenylamine	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
95	N-Nitrosodi-n-propylamine	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]

สมช

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
96	Polychlorinated biphenyls (PCBs) - Aroclor 1016 - Aroclor 1221 - Aroclor 1232 - Aroclor 1242 - Aroclor 1248 - Aroclor 1254 - Aroclor 1260 - 2-Chlorobiphenyl - 2,2',3,5'-Tetrachlorobiphenyl - 2,2',5,5'-Tetrachlorobiphenyl - 2,3',4,4'-Tetrachlorobiphenyl - 2,2',3,4,5'-Pentachlorobiphenyl - 2,2',4,5,5'-Pentachlorobiphenyl - 2,3,3',4',6-Pentachlorobiphenyl - 2,2',3,4,4',5'-Hexachlorobiphenyl - 2,2',3,4,5,5'-Hexachlorobiphenyl - 2,2',3,5,5',6-Hexachlorobiphenyl - 2,2',4,4',5,5'-Hexachlorobiphenyl - 2,2',3,3',4,4',5-Heptachlorobiphenyl - 2,2',3,4,4',5,5'-Heptachlorobiphenyl - 2,2',3,4,4',5',6-Heptachlorobiphenyl - 2,2',3,4',5,5',6-Heptachlorobiphenyl - 2,2',3,3',4,4',5,5',6-Nonachlorobiphenyl	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
97	Pentachlorophenol	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
98	Phenanthrene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]

Small

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
99	Phenol	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
100	Pyrene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
101	Selenium	1) Digestion, Inductively Coupled Plasma Method ^[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[7,17]
102	Silver	1) Digestion, Inductively Coupled Plasma Method ^[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[7,17]
103	Styrene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
104	1,1,2,2-Tetrachloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
105	Tetrachloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
106	Toluene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
107	Toxaphene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
108	TPH (C ₅ -C ₈)	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
109	TPH (C ₈ - C ₁₆)	1) Automate Extraction, Gas Chromatographic Method ^[11,22] 2) Solvent Extraction, Gas Chromatographic Method ^[12,22] 3) Ultrasonic Extraction, Gas Chromatographic Method ^[22,31]
110	TPH (C ₁₆ - C ₃₅)	1) Automate Extraction, Gas Chromatographic Method ^[11,22] 2) Solvent Extraction, Gas Chromatographic Method ^[12,22] 3) Ultrasonic Extraction, Gas Chromatographic Method ^[22,31]
111	1,2,4-Trichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
112	1,1,1-Trichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
113	1,1,2-Trichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
114	Trichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]

สมย

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
115	2,4,5-Trichlorophenol	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
116	2,4,6-Trichlorophenol	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method ^[11,26]
117	1,3,5-Trimethylbenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
118	Vanadium	1) Digestion, Inductively Coupled Plasma Method ^[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[7,17]
119	Vinyl Acetate	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
120	Vinyl Chloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
121	m-Xylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
122	o-Xylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
123	p-Xylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
124	Xylene (Total)	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method ^[15,25]
125	Zinc	1) Digestion, Inductively Coupled Plasma Method ^[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[7,17]

วิมล

เอกสารอ้างอิง

- กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2566. เรื่อง การจัดการสิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว. ราชกิจจานุเบกษา. 31 พฤษภาคม 2566. เล่มที่ 140 ตอนพิเศษ 126 ง.
- กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2549. เรื่อง กำหนดค่าปริมาณเขม่าควันที่เจือปนในอากาศที่ระบายออกจากปล่องของหม้อน้ำโรงสีข้าวที่ใช้กลบเป็นเชื้อเพลิง. ราชกิจจานุเบกษา. 4 ธันวาคม 2549. เล่มที่ 123 ตอนพิเศษ 125 ง.
- สมาคมวิศวกรรมสิ่งแวดล้อมแห่งประเทศไทย. คู่มือวิเคราะห์น้ำเสีย. พิมพ์ครั้งที่ 4. กรุงเทพฯ: เรือนแก้วการพิมพ์, 2547.
- APHA, AWWA, WEF. Standard Methods for the Examination of Water and Wastewater. 24th ed. Washington, DC: APHA, 2023.

5. United States Environmental Protection Agency. **Standards of Performance for New Stationary Sources**. 40 CFR 60. Appendix A, 2023.

6. United States Environmental Protection Agency. **Test Methods for Evaluating Solid Waste Physical/Chemical Methods**. SW-846, 2014.

7. United States Environmental Protection Agency. **Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Acid Digestion of Sludges and Sediments and Soils**. SW-846 Method 3050B, 1996.

8. United States Environmental Protection Agency. **Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Alkaline Digestion for Hexavalent Chromium**. SW-846 Method 3060A, 1996.

9. United States Environmental Protection Agency. **Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Separatory Funnel Liquid-Liquid Extraction**. SW-846 Method 3510C, 1996.

10. United States Environmental Protection Agency. **Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Soxhlet Extraction**. SW-846 Method 3540C, 1996.

11. United States Environmental Protection Agency. **Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Automated Soxhlet Extraction**. SW-846 Method 3541, 1994.

12. United States Environmental Protection Agency. **Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Microscale Solvent Extraction (MSE)**. SW-846 Method 3570, 2002.

13. United States Environmental Protection Agency. **Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Volatile Organic Compounds (VOCs) in Various Sample Matrices Using Equilibrium Headspace Analysis**. SW-846 Method 5021A, 2014.


14. United States Environmental Protection Agency. **Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Purge-and-Trap for Aqueous Samples**. SW-846 Method 5030B, 1996.

15. United States Environmental Protection Agency. **Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Closed-System Purge-and-Trap and Extraction for Volatile Organics in Soil and Waste Samples**. SW-846 Method 5035, 1996.

16. United States Environmental Protection Agency. **Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Inductively Coupled Plasma-Atomic Emission Spectrometry**. SW-846 Method 6010B, 1996.

17. United States Environmental Protection Agency. **Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Inductively Coupled Plasma-Mass Spectrometry**. SW-846 Method 6020A, 2007.

18. United States Environmental Protection Agency. **Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Antimony and Arsenic (Atomic Absorption, Borohydride Reduction)**. SW-846 Method 7062, 1994. เพิ่มใหม่

19. United States Environmental Protection Agency. **Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Chromium, Hexavalent (Colorimetric)**. SW-846 Method 7196A, 1992. 

20. United States...

20. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Mercury in Solid or Semisolid Waste (Manual Cold-Vapor Technique). SW-846 Method 7471B, 2007.

21. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Mercury in Solids and Solutions by Thermal Decomposition, Amalgamation, and Atomic Absorption Spectrophotometry. SW-846 Method 7473, 2007.

22. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Nonhalogenated Organics by Gas Chromatography. SW-846 Method 8015C, 2007.

23. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. pH Electrometric Measurement. SW-846 Method 9040C, 2004.

24. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Soil and Waste pH. SW-846 Method 9045D, 2004.

25. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Volatile Organic Compounds by Gas Chromatography/Mass Spectrometry (GC/MS). SW-846 Method 8260D, 2018.

26. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Semivolatile Organic Compounds by Gas Chromatography/Mass Spectrometry (GC/MS). SW-846 Method 8270E, 2018.

27. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Total and Amenable Cyanide: Distillation SW-846 Method 9010B, 1996.

28. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Cyanide Extraction Procedure for Solids and Oil. SW-846 Method 9013A, 1996.

29. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Cyanide in Waters and Extracts Using Titrimetric and Manual Spectrophotometric Procedures. SW-846 Method 9014, 2014.

30. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Mercury in Sediment and Tissue Samples by Atomic Fluorescence Spectrometry. SW-846 Method 7474, 2007.

31. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. Ultrasonic Extraction. SW-846 Method 3550C, 2007.

Smal



ที่ อก ๐๓๑๐(๑)/ ๔๑ ๒๑

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๒๕ เมษายน ๒๕๖๗

เรื่อง เปลี่ยนแปลงบุคลากรของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๒๙ มีนาคม ๒๕๖๗

ตามคำขอที่อ้างถึง บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๒๐๔ สถานที่ตั้งเลขที่ ๑๐๔ ซอยพัฒนาการ ๔๐ ถนนพัฒนาการ แขวงพัฒนาการ เขตสวนหลวง กรุงเทพมหานคร ขอเปลี่ยนแปลงบุคลากร ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว มีความเห็นดังนี้

๑. ให้ยกเลิกเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๓ ราย

- | | |
|--------------------------|----------------------------|
| ๑) นางสาวพรรณธิดา พุ่มคง | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๕ |
| ๒) นายกำชัย สุทธะ | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๒๑ |
| ๓) นางสาวศุภรดา บัณมยุรา | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๘ |

๒. ให้เพิ่มเจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน จำนวน ๑๒ ราย

- | | |
|-----------------------------|----------------------------|
| ๑) นางสาวฐานิดา กลิ่นเขียว | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๘๒ |
| ๒) นางสาวกัญญภััสสร สายคำ | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๘๓ |
| ๓) นางสาวณัฐนันท์ กันทะวงศ์ | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๘๔ |
| ๔) นายอำนาจ วงษาเคน | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๘๕ |
| ๕) นายกฤษณพล ปัญญาวงศ์ | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๘๖ |
| ๖) นายณชากร หารรักษา | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๘๗ |
| ๗) นายวัชรินทร์ ผ่องสามสวน | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๘๘ |
| ๘) นายณัฐพงศ์ โสภา | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๘๙ |
| ๙) นายศักรินทร์ ปานเพ็ง | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๙๐ |
| ๑๐) นายณัฐพล ชุ่มชื่น | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๙๑ |
| ๑๑) นายธนา สุพาพันธุ์ | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๙๒ |
| ๑๒) นายนราธร แก้วพงษ์ชา | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๙๓ |

อนึ่ง หนังสือฉบับนี้จะหมดอายุพร้อมหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
ในวันที่ ๒ กันยายน ๒๕๖๙

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายพริต กัตน์กรอง)

รองอธิบดี ปฏิบัติราชการแทน

อธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน

กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ

โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕

โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๙๙

ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th



ที่อก ๐๓๑๐(๑)/ ๑๒ ๓๖ ๘ /



กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๑๘ ธันวาคม ๒๕๖๗

เรื่อง ยกเลิกบุคลากรของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน ลงวันที่ ๒ ธันวาคม ๒๕๖๗

ตามคำขอที่อ้างถึง บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๒๐๔ สถานที่ตั้งเลขที่ ๑๐๔ ซอยพัฒนาการ ๔๐ ถนนพัฒนาการ แขวงพัฒนาการ เขตสวนหลวง กรุงเทพมหานคร ขอยกเลิกบุคลากร ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้ยกเลิกเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๘ ราย ได้แก่

- | | |
|-------------------------------|----------------------------|
| ๑) นายประพจน์ วรรณชูชัย | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๐ |
| ๒) นายจิรณัฐ ขาวละออ | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๗๒ |
| ๓) นายพีรพัฒน์ กำคำ | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๘ |
| ๔) นางสาวอรยา คำคล่อง | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๔ |
| ๕) นายกิตติพงศ์ แซ่ลี | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๔๔ |
| ๖) นายจิรเมธ ประเสริฐศิริพงศ์ | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๐ |
| ๗) นายภัทรพงษ์ มณฑาทอง | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๗ |
| ๘) นางสาวจารุวรรณ กระจำงพันธ์ | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๘๑ |

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายธีรทัศน์ อิศรางกูร ณ อยุธยา)
รองอธิบดี ปฏิบัติราชการแทน
อธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน

กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ

โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕

โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๙๙

ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th



“อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา อุตสาหกรรมสีเขียว”



ที่ อก ๐๓๑๐(๑)/ ๓๑๕๐



กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๕๐๐

๑๐ เมษายน ๒๕๖๘

เรื่อง ยกเลิกบุคลากรของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๒ เมษายน ๒๕๖๘

ตามคำขอที่อ้างถึง บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๒๐๔ สถานที่ตั้งเลขที่ ๑๐๔ ซอยพัฒนาการ ๔๐ ถนนพัฒนาการ แขวงพัฒนาการ เขตสวนหลวง กรุงเทพมหานคร ขอยกเลิกบุคลากร ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้ยกเลิกเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์
จำนวน ๒ ราย ได้แก่

๑) นายธิตพิงค์ บัวแดง

ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๒

๒) นายมงคล ผลาทิพย์

ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๑๐

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายธีรทัศน์ อิศรางกูร ณ อยุธยา)

รองอธิบดี ปฏิบัติราชการแทน

อธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน

กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ

โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕

โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๙๙

ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th





ที่ อก ๐๓๑๐(๑)/ ๕๖ ๗ ๓

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๐๕ มิถุนายน ๒๕๖๔

เรื่อง เปลี่ยนแปลงบุคลากรของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๗ พฤษภาคม ๒๕๖๔

ตามคำขอที่อ้างถึง บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ห้องปฏิบัติการ
วิเคราะห์เอกชน เลขทะเบียน ว-๒๐๔ สถานที่ตั้งเลขที่ ๑๐๔ ซอยพัฒนาการ ๔๐ ถนนพัฒนาการ แขวงพัฒนาการ
เขตสวนหลวง กรุงเทพมหานคร ขอเปลี่ยนแปลงบุคลากร ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้เพิ่มเจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน
จำนวน ๑๑ ราย ได้แก่

- | | |
|-----------------------------------|----------------------------|
| ๑) นายคุณากร มั่นชื่น | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๙๔ |
| ๒) นายชัยมงคล แสนมาตร | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๙๕ |
| ๓) นายเอกรินทร์ บุตส์ักดิ์ | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๙๖ |
| ๔) นายพิชานนท์ อินปริง | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๙๗ |
| ๕) นายศตวรรษ แก้วกันหา | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๙๘ |
| ๖) นายวิกรม มีศิริ | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๙๙ |
| ๗) นายภคนันท์ คำจันทราช | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๒๐๐ |
| ๘) นายศิริวิทย์ มีไพฑูรย์ | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๒๐๑ |
| ๙) นายธีรพงษ์ ศรีคำแหง | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๒๐๒ |
| ๑๐) นายอภิสิทธิ์ ศรีคงแก้ว | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๒๐๓ |
| ๑๑) ว่าที่ร้อยตรี ภาณุพงศ์ แสนศรี | ทะเบียนเลขที่ ว-๒๐๔-จ-๐๒๐๔ |

อนึ่ง หนังสือฉบับนี้จะสิ้นอายุพร้อมหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
ในวันที่ ๒ กันยายน ๒๕๖๔

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายศิระ จันท์เกิด)

นักวิทยาศาสตร์เชี่ยวชาญ รัชการยการแทน
ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน

กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ

โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕

โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๙๙

ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th



“อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา อุตสาหกรรมสีเขียว”



ที่ อก ๐๓๑๐(๑)/ ๒๕๐๘



กรมโรงงานอุตสาหกรรม

ถนนพระรามที่ ๖ แขวงทุ่งพญาไท

เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๒๑ สิงหาคม ๒๕๖๔

เรื่อง เปลี่ยนแปลงสารมลพิษที่วิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๒๗ มิถุนายน ๒๕๖๔

สิ่งที่ส่งมาด้วย เอกสารแนบท้ายหนังสือเปลี่ยนแปลงสารมลพิษที่วิเคราะห์

บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด จำนวน ๖ แผ่น

ตามคำขอที่อ้างถึง บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๒๐๔ สถานที่ตั้งเลขที่ ๑๐๔ ซอยพัฒนาการ ๔๐ ถนนพัฒนาการ แขวงพัฒนาการ เขตสวนหลวง กรุงเทพมหานคร ขอเปลี่ยนแปลงสารมลพิษที่วิเคราะห์ ต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด เพิ่มขอบข่ายชนิดสารมลพิษที่วิเคราะห์ในน้ำใต้ดิน สิ่งปฏิกูลและวัสดุที่ไม่ใช้แล้ว และดิน ตามสิ่งที่ส่งมาด้วย

อนึ่ง หนังสือฉบับนี้จะสิ้นสุดอายุพร้อมหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
ในวันที่ ๒ กันยายน ๒๕๖๕

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นางสาวปัทมวรรณ คุณประเสริฐ)

ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน

ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน

กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ

โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕

โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๙๙

ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th



เอกสารแนบท้ายหนังสือเปลี่ยนแปลงสารมลพิษที่วิเคราะห์

บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

เลขทะเบียน ว-๒๐๔

ที่ อก ๐๓๑๐(๑)/ ๖๕ ๐ ๘

ลงวันที่

๒๑

สิงหาคม ๒๕๖๔

ขอขยายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๔๐ รายการ

น้ำใต้ดิน จำนวน ๔ รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Aluminum	Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[2]
2	Copper	Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[2]
3	Iron	Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[2]
4	Molybdenum	Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[2]

สิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว จำนวน 17 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Antimony	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,3,7] 3) Digestion, Inductively Coupled Plasma Method ^[4,6] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4,7]
2	Arsenic	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,3,7] 3) Digestion, Inductively Coupled Plasma Method ^[4,6] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4,7]
3	Barium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,3,7] 3) Digestion, Inductively Coupled Plasma Method ^[4,6] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4,7]

๗๖

Beryllium

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
4	Beryllium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,3,7] 3) Digestion, Inductively Coupled Plasma Method ^[4,6] 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[4,7]
5	Cadmium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,3,7] 3) Digestion, Inductively Coupled Plasma Method ^[4,6] 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[4,7]
6	Chromium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,3,7] 3) Digestion, Inductively Coupled Plasma Method ^[4,6] 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[4,7]
7	Chromium (III)	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method; Waste Extraction, Colorimetric Method; Calculation Method ^[1,3,6,8] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method; Waste Extraction, Colorimetric Method; Calculation Method ^[1,3,7,8] 3) Digestion, Inductively Coupled Plasma Method; Alkaline Digestion, Colorimetric Method; Calculation Method ^[4,5,6,8] 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method; Alkaline Digestion, Colorimetric Method; Calculation Method ^[4,5,7,8]
8	Cobalt	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,3,7]

๑๗

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
9	Copper	3) Digestion, Inductively Coupled Plasma Method ^[4,6] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4,7] 1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,3,7] 3) Digestion, Inductively Coupled Plasma Method ^[4,6] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4,7]
10	Lead	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,3,7] 3) Digestion, Inductively Coupled Plasma Method ^[4,6] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4,7]
11	Molybdenum	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,3,7] 3) Digestion, Inductively Coupled Plasma Method ^[4,6] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4,7]
12	Nickel	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,3,7] 3) Digestion, Inductively Coupled Plasma Method ^[4,6] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4,7]
13	Selenium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,3,7] 3) Digestion, Inductively Coupled Plasma Method ^[4,6] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4,7]

อนันต์

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
14	Silver	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,3,7] 3) Digestion, Inductively Coupled Plasma Method ^[4,6] 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[4,7]
15	Thallium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,3,7] 3) Digestion, Inductively Coupled Plasma Method ^[4,6] 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[4,7]
16	Vanadium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,3,7] 3) Digestion, Inductively Coupled Plasma Method ^[4,6] 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[4,7]
17	Zinc	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method ^[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[1,3,7] 3) Digestion, Inductively Coupled Plasma Method ^[4,6] 4) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[4,7]

ดิน จำนวน 19 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Aluminum	1) Digestion, Inductively Coupled Plasma Method ^[4,6] 2) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[4,7]
2	Antimony	1) Digestion, Inductively Coupled Plasma Method ^[4,6] 2) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method ^[4,7]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
3	Arsenic	1) Digestion, Inductively Coupled Plasma Method ^[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4,7]
4	Barium	1) Digestion, Inductively Coupled Plasma Method ^[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4,7]
5	Beryllium	1) Digestion, Inductively Coupled Plasma Method ^[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4,7]
6	Cadmium	1) Digestion, Inductively Coupled Plasma Method ^[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4,7]
7	Chromium	1) Digestion, Inductively Coupled Plasma Method ^[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4,7]
8	Chromium (III)	1) Digestion, Inductively Coupled Plasma Method; Alkaline Digestion, Colorimetric Method; Calculation Method ^[4,5,6,8] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method; Alkaline Digestion, Colorimetric Method; Calculation Method ^[4,5,7,8]
9	Copper	1) Digestion, Inductively Coupled Plasma Method ^[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4,7]
10	Iron	1) Digestion, Inductively Coupled Plasma Method ^[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4,7]
11	Lead	1) Digestion, Inductively Coupled Plasma Method ^[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4,7]
12	Manganese	1) Digestion, Inductively Coupled Plasma Method ^[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4,7]
13	Molybdenum	1) Digestion, Inductively Coupled Plasma Method ^[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4,7]
14	Nickel	1) Digestion, Inductively Coupled Plasma Method ^[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4,7]

๑๒

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
15	pH	Electrometric Method ^[9]
16	Selenium	1) Digestion, Inductively Coupled Plasma Method ^[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4,7]
17	Silver	1) Digestion, Inductively Coupled Plasma Method ^[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4,7]
18	Vanadium	1) Digestion, Inductively Coupled Plasma Method ^[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4,7]
19	Zinc	1) Digestion, Inductively Coupled Plasma Method ^[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method ^[4,7]

เอกสารอ้างอิง

- กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2566. เรื่อง การจัดการสิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว. **ราชกิจจานุเบกษา**. 31 พฤษภาคม 2566. เล่มที่ 140 ตอนพิเศษ 126 ง.
- APHA, AWWA, WEF. **Standard Methods for the Examination of Water and Wastewater**. 24th ed. Washington, DC: APHA, 2023.
- United States Environmental Protection Agency. **Test Methods for Evaluating Solid Waste Physical/Chemical Methods. SW-846**.
- United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Acid Digestion of Sediments, Sludges, and Soils. SW-846 Method 3050B**, 1996.
- United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Alkaline Digestion for Hexavalent Chromium. SW-846 Method 3060A**, 1996.
- United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Inductively Coupled Plasma-Optical Emission Spectrometry. SW-846 Method 6010D**, 2018.
- United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Inductively Coupled Plasma-Mass Spectrometry. SW-846 Method 6020B**, 2014.
- United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Chromium, Hexavalent (Colorimetric). SW-846 Method 7196A**, 1992.
- United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Soil and Waste pH. SW-846 Method 9045D**, 2004.

กมลวิ

ที่ อก ๐๓๑๐(๑)๘๐ ๑ ๑



กรมโรงงานอุตสาหกรรม

ถนนพระรามที่ ๖ แขวงทุ่งพญาไท

เขตราชเทวี กรุงเทพฯ ๑๐๕๐๐

๒๖ กันยายน ๒๕๖๔

เรื่อง เปลี่ยนแปลงบุคลากร ชื่อตัวและชื่อสกุลของบุคลากร

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกซเรย์
ลงวันที่ ๒๑ สิงหาคม ๒๕๖๔

ตามคำขอที่อ้างถึง บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัดห้องปฏิบัติการวิเคราะห์เอกซเรย์ เลขทะเบียน ว-๒๐๔ สถานที่ตั้งเลขที่ ๑๐๔ ซอยพัฒนาการ ๔๐ ถนนพัฒนาการ แขวงพัฒนาการ เขตสวนหลวง กรุงเทพมหานคร ขอเปลี่ยนแปลงบุคลากร ชื่อตัวและชื่อสกุลของบุคลากร ต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว มีความเห็นดังนี้

๑. ให้ยกเลิกเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๒ ราย

๑) นางสาวพาฤดี คุณนาน

ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๙

๒) นางสาวอรณิษ เทียนดำ

ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๗๔

๒. ให้เปลี่ยนชื่อตัวและชื่อสกุลของเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จากเดิม นายอาทิตย์ ศรีเสน เป็น นายรัฐธีร์ ทวีกิจวรพจน์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๔๘

อนึ่ง หนังสือฉบับนี้จะสิ้นอายุพร้อมหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกซเรย์ ในวันที่ ๒ กันยายน ๒๕๖๔

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นางสาวปัทมวรรณ คุณประเสริฐ)

ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน

ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน

กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ

โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕

โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๙๙

ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th



“อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา อุตสาหกรรมสีเขียว”





๐๔ สิงหาคม ๒๕๖๗

เรื่อง ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์
เอกชน ลงวันที่ ๒๗ พฤษภาคม ๒๕๖๗

สิ่งที่ส่งมาด้วย เอกสารแนบท้ายหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด จำนวน ๓ แผ่น

ตามคำขอที่อ้างถึง บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ขอต่ออายุ
หนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๓๒๓ สถานที่ตั้งเลขที่ ๖๑๖/๑๐ หมู่ที่ ๕
ตำบลแม่น้ำคู้ อำเภอลวกแดง จังหวัดระยอง ต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย)
จำกัด ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน โดยมีองค์ประกอบดังนี้

ก. ผู้ควบคุมห้องปฏิบัติการวิเคราะห์เอกชน

- | | |
|--------------------------|----------------------------|
| ๑) นายเดช ช้างชน | ทะเบียนเลขที่ ว-๓๒๓-ค-๐๐๐๑ |
| ๒) นางวิลาวัลย์ บริรักษ์ | ทะเบียนเลขที่ ว-๓๒๓-ค-๐๐๐๒ |
| ๓) นายสุพจน์ สลามเต๊ะ | ทะเบียนเลขที่ ว-๓๒๓-ค-๐๐๐๓ |

ข. เจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน

- | | |
|--------------------------------|----------------------------|
| ๑) นายณัฐพงษ์ เพ็งขาวนา | ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๐๑ |
| ๒) นางสาวกัลยพรรณ รักษ์ดี | ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๐๒ |
| ๓) นางสาวจุฑารัตน์ สีสทองกลาง | ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๐๓ |
| ๔) นางสาวจิตสุภา ประเทืองสุข | ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๐๔ |
| ๕) นายสรสรเสรีญ์ ค่อยยกสุย | ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๐๕ |
| ๖) นายณัฐวุฒิ ออมพรมราช | ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๐๖ |
| ๗) นายจิตรกร สีวะสา | ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๐๗ |
| ๘) นายสิทธิปวิญญ์ สุวรรณรัตน์ | ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๐๘ |
| ๙) นายสิทธิพันธ์ เสนาชีว | ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๐๙ |
| ๑๐) นายอนุเวศน์ เตมา | ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๑๐ |
| ๑๑) นายสุรวิทย์ นราพงษ์ | ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๑๑ |
| ๑๒) นายณัฐพล เจียงวรวงศ์ | ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๑๓ |
| ๑๓) นายชานนท์ บุญชื่น | ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๑๔ |
| ๑๔) นายณัฐกานต์ วงศ์อินทร์อยู่ | ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๑๕ |
| ๑๕) นายอานนท์ โพธิ์พระทอง | ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๑๖ |

๑๖) นายณัฐพล...

๑๖) นายณัฏฐพล ถ้ำกลาง	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๑๗
๑๗) นายศุภณัฐ พิสัยพันธ์	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๑๘
๑๘) นายวสันต์ คินันติ	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๑๙
๑๙) นายวรัญญู นิมพาสิทธิ์	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๒๐
๒๐) นายศุภณัฐ สกฤกิตติมงคลดี	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๒๑
๒๑) นายเอกชัย ถันทอง	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๒๒
๒๒) นายพงษ์เทพ สิทธิเลาะ	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๒๓
๒๓) นายทินกร กุมภาชี	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๒๔
๒๔) นางสาวนันทยา เบญจพันธ์	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๒๕
๒๕) นายสิทธิชัย ยันพิมาย	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๒๖
๒๖) นางสาวปภาณิน หลอดทอง	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๒๗
๒๗) นางสาวพจนา สีดา	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๒๘
๒๘) นางสาวธนิดา กุลศิริวงศ์	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๒๙
๒๙) นายพิทยา ทองแดง	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๓๐
๓๐) นางสาวชลธิชา สุปงกช	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๓๑
๓๑) ว่าที่ร้อยตรี ธรณชัย ม่วงมา	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๓๒
๓๒) นายวรารุณ พับพา	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๓๓
๓๓) นายศักดิ์นรินทร์ จรัสกาย	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๓๔
๓๔) นายสุรศักดิ์ สาชิน	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๓๕
๓๕) นายสถาพร ถาแก้ว	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๓๖
๓๖) นายสุทธิดำรง โชคปิณฑินท์	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๓๗
๓๗) นายวัลลภ หันไชยเนาว์	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๓๘
๓๘) นางสาววนาลี เจริญตระกูล	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๓๙
๓๙) นายธนะสิทธิ์ วงศ์ไชย	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๔๐
๔๐) นายชัยนุสรณ์ เลิศนันทกุลชัย	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๔๑
๔๑) นายสัจจา เพ็ชรแสง	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๔๒
๔๒) นายกัณตภณ มณีสัมพันธ์	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๔๓
๔๓) นายธารินทร์ อ็อกจินดา	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๔๔
๔๔) นายศุภชัย วงศ์สุริยฉาย	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๔๕
๔๕) นายไสว ตันโพธิ์	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๔๖
๔๖) นางสาวกิตติยา สันญาอริยาภรณ์	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๔๗
๔๖) นางสาวธิดารัตน์ ศิริมังคะโร	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๔๘
๔๗) นายพิพัฒน์ นิภัทร์เศรษฐ์	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๔๙
๔๘) นายศิริวิทย์ เรืองสม	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๕๐
๔๙) นายปารามาศ สัตยาคุณ	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๕๑
๕๐) นายนฤนาท ธรรมสระโร	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๕๒
๕๑) นางสาวศุภรัตน์ โสจันทร์	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๕๓

๕๒) นายพชรกร เจ็ญเจริญ	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๕๔
๕๓) นายทิวากร เชื้อมาก	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๕๕
๕๔) นายอนุรักษ ทองขจรศักดิ์ดา	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๕๖
๕๕) นายอภิชาติ วิชาส	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๕๗
๕๖) นายจรัสระวี ศรีรักษา	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๕๘
๕๘) นายประสานมิตร เชื้อนเพชร	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๕๙
๕๙) นายภาณุวัฒน์ วังบง	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๖๐
๖๐) นายสันติ ชัยชนะ	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๖๑
๖๑) นายทินกร กุลชาติ	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๖๒

ค. ขอบข่ายชนิดสารมลพิษที่ได้รับขึ้นทะเบียนให้วิเคราะห์ในน้ำเสีย น้ำใต้ดิน อากาศเสีย ตามสิ่งที่ส่งมาด้วย

หนังสือฉบับนี้จะหมดอายุในวันที่ ๒๘ มิถุนายน ๒๕๗๑ หากประสงค์จะต่ออายุหนังสือ รับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ให้ยื่นคำขอต่ออายุพร้อมเอกสารประกอบคำขอต่อกรมโรงงาน อุตสาหกรรมภายใน ๖๐ วัน ก่อนวันสิ้นอายุของหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายพริต กลนกรอง)

รองอธิบดี ปฏิบัติราชการแทน

อธิบดีกรมโรงงานอุตสาหกรรม

ศูนย์วิจัยและเตือนภัยมลพิษโรงงานภาคตะวันออก

โทร. ๐ ๓๓๑๓ ๖๐๕๔ ต่อ ๕๐๐๑-๒

ไปรษณีย์อิเล็กทรอนิกส์ eirw@diw.mail.go.th



“อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา อุตสาหกรรมสีเขียว”



เอกสารแนบท้ายหนังสือเปลี่ยนแปลงสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด เลขทะเบียน ว-๓๒๓
ที่ ออก ๐๓๒๐/ ๗ ๙๓ ๘ ลงวันที่ ๐๘ สิงหาคม ๒๕๖๗

ขอขยายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๒๔ รายการ
น้ำเสีย จำนวน 14 รายการ

ลำดับ ที่	สารมลพิษ	วิธีวิเคราะห์
1	Biochemical Oxygen Demand	1) 5-Day BOD Test, Membrane Electrode Method ^[2] 2) 5-Day BOD Test, Azide Modification Method ^[2]
2	Chemical Oxygen Demand	1) Open Reflux, Titrimetric Method ^[2] 2) Closed Reflux, Colorimetric Method ^[2] 3) Closed Reflux, Titrimetric Method ^[2]
3	Color	ADMI Weighted-Ordinate Spectrophotometric Method ^[2]
4	Cyanide	Distillation, Colorimetric Method ^[2]
5	Formaldehyde	Distillation, Colorimetric Method ^[1]
6	Free Chlorine	DPD Ferrous Titrimetric Method ^[2]
7	Oil and Grease	Liquid-Liquid, Partition-Gravimetric Method ^[2]
8	pH	Electrometric Method ^[2]
9	Phenols	1) Distillation, Chloroform Extraction Method ^[2] 2) Distillation, Direct Photometric Method ^[2]
10	Sulfide	ZnS Precipitation, Iodometric Method ^[2]
11	Temperature	Field Method ^[2]
12	Total Dissolved Solids	Dried at 180 °C ^[2]
13	Total Kjeldahl Nitrogen	Semi-Macro Kjeldahl Method ^[2]
14	Total Suspended Solids	Dried at 103-105 °C ^[2]

น้ำใต้ดิน จำนวน 3 รายการ

ลำดับ ที่	สารมลพิษ	วิธีวิเคราะห์
1	Cyanide	Distillation, Colorimetric Method ^[2]
2	pH	Electrometric Method ^[2]
3	Phenols	Distillation, Direct Photometric Method ^[2]

อากาศเสีย...

อากาศเสีย (ปล่อยระบาย) จำนวน 7 รายการ

ลำดับ ที่	สารมลพิษ	วิธีวิเคราะห์
1	Carbon Monoxide	1) Sampling Bag, Non-Dispersive Infrared Method ^[5] 2) Instrumental Analyzer Method ^[9]
2	Hydrogen Sulfide	Absorption Sampling, Iodometric Method ^[5]
3	Opacity	Ringelmann's Method ^[3,4]
4	Oxide of Nitrogen	1) Absorption Sampling, Phenoldisulfonic Acid Method ^[8] 2) Instrumental Analyzer Method ^[10]
5	Sulfur Dioxide	1) Absorption Sampling, Barium-Thorin Titrimetric Acid Method ^[5] 2) Instrumental Analyzer Method ^[11]
6	Sulfuric Acid	Isokinetic Sampling, Barium – Titrimetric Method ^[6]
7	Total Suspended Particulate	Isokinetic Sampling, Gravimetric Method ^[7]

เอกสารอ้างอิง

1. ธงชัย พรรณสวัสดิ์ และวิบูลย์ลักษณ์ วิสุมิศักดิ์, บรรณาธิการ. (2547) คู่มือวิเคราะห์น้ำเสีย. พิมพ์ครั้งที่ 4. กรุงเทพฯ: สมาคมวิศวกรรมสิ่งแวดล้อมแห่งประเทศไทย.

2. APHA, AWWA, WEF. Standard Methods for the Examination of Water and Wastewater. 24th ed. Washington, DC : APHA, 2023

3. กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2549. เรื่อง กำหนดค่าปริมาณเขม่าควันที่เจือปนในอากาศที่ระบายออกจากปล่องของหม้อน้ำโรงสีข้าวที่ใช้กลบเป็นเชื้อเพลิง. ราชกิจจานุเบกษา. 4 ธันวาคม 2549. เล่มที่ 123 ตอนพิเศษ 125ง

4. กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2549. เรื่อง กำหนดค่าปริมาณเขม่าควันที่เจือปนในอากาศที่ระบายออกจากปล่องของหม้อน้ำของโรงงาน. ราชกิจจานุเบกษา. 4 ธันวาคม 2549. เล่มที่ 123 ตอนพิเศษ 125ง

5. United States Environmental Protection Agency. Standards of Performance for New Stationary Sources. 40 CFR 60. Appendix A, 2017.

6. United States Environmental Protection Agency. Standards of Performance for New Stationary Sources. 40 CFR 60. Appendix A, 2019.

7. United States...

7. United States Environmental Protection Agency. **Standards of Performance for New Stationary Sources**. 40 CFR 60. Appendix A, 2020.

8. United States Environmental Protection Agency. **Standards of Performance for New Stationary Sources**. 40 CFR 60. Appendix A, 2023.

9. United States Environmental Protection Agency. **Determination of Carbon Monoxide Emission from Stationary Sources; Instrumental Analyzer Procedure**. 40 CFR 60. Appendix A Method 10, 2017.

10. United States Environmental Protection Agency. **Determination of Oxide of Nitrogen Emission from Stationary Sources; Instrumental Analyzer Procedure**. 40 CFR 60. Appendix A Method 7E, 2023.

11. United States Environmental Protection Agency. **Determination of Sulfur dioxide Emission from Stationary Sources; Instrumental Analyzer Procedure**. 40 CFR 60. Appendix A Method 6C, 2017.

A handwritten signature in black ink, consisting of a large, stylized 'O' followed by a horizontal line and a short vertical stroke.

ที่ อก ๐๓๒๐/ ๑๐๐๙ ๙



กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๐๔ ตุลาคม ๒๕๖๗

เรื่อง แกไขรายชื่อเจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลборาทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง หนังสือ บริษัท เอแอลเอส แลборาทอรี กรุ๊ป (ประเทศไทย) จำกัด เลขที่ Env 2024/005

ลงวันที่ ๓๐ สิงหาคม ๒๕๖๗

ตามหนังสือที่อ้างถึง บริษัท เอแอลเอส แลборาทอรี กรุ๊ป (ประเทศไทย) จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๓๒๓ สถานที่ตั้งเลขที่ ๖๑๖/๑๐ หมู่ที่ ๕ ตำบลแม่น้ำคู้ อำเภอบลวกแดง จังหวัดระยอง ขอแก้ไขชื่อเจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน เนื่องจากมีความคลาดเคลื่อน ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรม ได้รับทราบและดำเนินการแก้ไขรายชื่อเจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน จำนวน ๕ ราย ตามที่แจ้งเรียบร้อยแล้ว เป็นดังนี้

ลำดับที่ ๒๗ นางพจนา สีดา

ลำดับที่ ๒๘ นางสาวธนิศา กุลสุริวงศ์

ลำดับที่ ๓๐ นางชลธิชา สุปงกช

ลำดับที่ ๓๖ นายสุทธิดำรงค์ โชคปิตินันท์

ลำดับที่ ๔๒ นายกันตภณ มณีสัมพันธ์

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

น

(นายพรยศ กลั่นกรอง)

รองอธิบดี ปฏิบัติราชการแทน

อธิบดีกรมโรงงานอุตสาหกรรม

ศูนย์วิจัยและเตือนภัยมลพิษโรงงานภาคตะวันออก

โทร. ๐ ๓๓๑๓ ๖๐๕๙ ต่อ ๕๐๐๑-๒

ไปรษณีย์อิเล็กทรอนิกส์ eirw@diw.mail.go.th



“อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา อุตสาหกรรมสีเขียว”



ที่ อก ๐๓๑๐(๓)/ ๕๒๔๖



กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๒๐ พฤษภาคม ๒๕๖๔

เรื่อง ยกเลิกบุคลากรของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๑๐ เมษายน ๒๕๖๔

ตามคำขอที่อ้างถึง บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๓๒๓ สถานที่ตั้งเลขที่ ๖๑๖/๑๐ หมู่ที่ ๕ ตำบลแม่น้ำคู้ อำเภอปลวกแดง จังหวัดระยอง ขอยกเลิกบุคลากร ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้ยกเลิกเจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน
จำนวน ๑ ราย ได้แก่ นายปารามาศ สัตยาคุณ ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๕๑

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายประสม ดำรงพงษ์)

ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

ศูนย์วิจัยและเตือนภัยมลพิษโรงงานภาคตะวันออก

โทร. ๐ ๓๓๑๓ ๖๐๕๔ ต่อ ๕๐๐๑-๒

ไปรษณีย์อิเล็กทรอนิกส์ eirw@diw.mail.go.th



“อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา อุตสาหกรรมสีเขียว”



ที่ อก ๐๓๑๐(๓)/ ๕๕๐๙



กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๕๐๐

๒๗ พฤษภาคม ๒๕๖๘

เรื่อง เปลี่ยนแปลงชื่อ-สกุลบุคลากรของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๑๕ พฤษภาคม ๒๕๖๘

ตามคำขอที่อ้างถึง บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๓๒๓ สถานที่ตั้งเลขที่ ๖๑๖/๑๐ หมู่ที่ ๕ ตำบลแม่ไม้ อำเภอปลวกแดง จังหวัดระยอง ขอเปลี่ยนแปลงชื่อ-สกุลบุคลากร ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้เปลี่ยนแปลงชื่อ-สกุลบุคลากร จำนวน ๑ ราย
จากนายธนະสิทธิ์ วงศ์ไชย เป็น นายอมลวิษฐ์ วงศ์ไชย

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายประสม ดำรงพงษ์)

ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

ศูนย์วิจัยและเตือนภัยมลพิษโรงงานภาคตะวันออก

โทร. ๐ ๓๓๑๓ ๖๐๕๙ ต่อ ๕๐๐๑-๒

ไปรษณีย์อิเล็กทรอนิกส์ eirw@diw.mail.go.th



“อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา อุตสาหกรรมสีเขียว”





ที่ อก ๐๓๑๐(๓)/ ๕๗๖๔

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๐ ๒ ธันวาคม ๒๕๖๘

เรื่อง เปลี่ยนแปลงสารมลพิษที่วิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๓๑ ตุลาคม ๒๕๖๘

สิ่งที่ส่งมาด้วย เอกสารแนบท้ายหนังสือเปลี่ยนแปลงสารมลพิษที่วิเคราะห์

บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด จำนวน ๒ แผ่น

ตามคำขอที่อ้างถึง บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๓๒๓ สถานที่ตั้งเลขที่ ๖๑๖/๑๐ หมู่ที่ ๕ ตำบลแม่แก้ว อำเภอลำปาง จังหวัดลำปาง ขอเปลี่ยนแปลงสารมลพิษที่วิเคราะห์ ต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด เพิ่มขอบข่ายชนิดสารมลพิษที่วิเคราะห์ในน้ำเสีย และน้ำใต้ดิน ตามสิ่งที่ส่งมาด้วย

อนึ่ง หนังสือฉบับนี้จะสิ้นอายุพร้อมหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
ในวันที่ ๒๘ มิถุนายน ๒๕๗๑

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นางสาวปัทมวรรณ คุณประเสริฐ)

ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน

ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน

ศูนย์วิจัยและเตือนภัยมลพิษโรงงานภาคตะวันออก

โทร. ๐ ๓๓๑๓ ๖๐๕๙ ต่อ ๕๐๐๑-๒

ไปรษณีย์อิเล็กทรอนิกส์ eirw@diw.mail.go.th



“อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา อุตสาหกรรมสีเขียว”



เอกสารแนบท้ายหนังสือเปลี่ยนแปลงสารมลพิษที่วิเคราะห์

บริษัท เอแอลเอส แลборาทอรี กรุ๊ป (ประเทศไทย) จำกัด เลขทะเบียน ว-๓๒๓

ที่ ออก ๐๓๑๐(๓)/ ๙๗๖๔

ลงวันที่ ๐๒ ธันวาคม ๒๕๖๔

ขอขยายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๒๓ รายการ

น้ำเสีย จำนวน 13 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Arsenic	Digestion, Inductively Coupled Plasma Method
2	Barium	Digestion, Inductively Coupled Plasma Method
3	Cadmium	Digestion, Inductively Coupled Plasma Method
4	Chromium	Digestion, Inductively Coupled Plasma Method
5	Copper	Digestion, Inductively Coupled Plasma Method
6	Hexavalent Chromium	Colorimetric Method
7	Lead	Digestion, Inductively Coupled Plasma Method
8	Manganese	Digestion, Inductively Coupled Plasma Method
9	Mercury	Digestion, Cold-Vapor Atomic Absorption Spectrometric Method
10	Nickel	Digestion, Inductively Coupled Plasma Method
11	Selenium	Digestion, Inductively Coupled Plasma Method
12	Trivalent Chromium	Calculation
13	Zinc	Digestion, Inductively Coupled Plasma Method

น้ำใต้ดิน จำนวน 20 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Aluminum	Digestion, Inductively Coupled Plasma Method
2	Antimony	Digestion, Inductively Coupled Plasma Method
3	Arsenic	Digestion, Inductively Coupled Plasma Method
4	Barium	Digestion, Inductively Coupled Plasma Method
5	Beryllium	Digestion, Inductively Coupled Plasma Method
6	Cadmium	Digestion, Inductively Coupled Plasma Method
7	Chromium	Digestion, Inductively Coupled Plasma Method
8	Chromium (III)	Calculation
9	Chromium (VI)	Colorimetric Method
10	Copper	Digestion, Inductively Coupled Plasma Method

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
11	Iron	Digestion, Inductively Coupled Plasma Method
12	Lead	Digestion, Inductively Coupled Plasma Method
13	Manganese	Digestion, Inductively Coupled Plasma Method
14	Mercury	Digestion Cold-Vapor Atomic Absorption Spectrometric Method
15	Molybdenum	Digestion, Inductively Coupled Plasma Method
16	Nickel	Digestion, Inductively Coupled Plasma Method
17	Selenium	Digestion, Inductively Coupled Plasma Method
18	Silver	Digestion, Inductively Coupled Plasma Method
19	Vanadium	Digestion, Inductively Coupled Plasma Method
20	Zinc	Digestion, Inductively Coupled Plasma Method

เอกสารอ้างอิง

APHA, AWWA, WEF. **Standard Methods for the Examination of Water and Wastewater**. 24th ed. Washington, DC: APHA, 2023.

ที่ อก ๐๓๑๐(๓)/ ๑๗๗๘



กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๐๖ มีนาคม ๒๕๖๙

เรื่อง เปลี่ยนแปลงบุคลากรของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๖ กุมภาพันธ์ ๒๕๖๙

ตามคำขอที่อ้างถึง บริษัท เอแอลเอส แลบบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๓๒๓ สถานที่ตั้งเลขที่ ๖๑๖/๑๐ หมู่ที่ ๕ ตำบลแม่น้ำคู้ อำเภอบลวกแดง จังหวัดระยอง ขอเปลี่ยนแปลงบุคลากร ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้เพิ่มเจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน จำนวน ๗ ราย ได้แก่

๑) นายอนวัช คงปลีก	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๖๓
๒) นายธนาริพ อิติวุตตา	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๖๔
๓) นายเฉลิมชัย บุญซุบ	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๖๕
๔) นางสาวจิตรรา งามเสียม	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๖๖
๕) นางสาวลลิตา คำสมัย	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๖๗
๖) นางสาวปติตตา ชูตินันท์	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๖๘
๗) นายปฎิญา ปานทองทา	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๖๙

อนึ่ง หนังสือฉบับนี้จะสิ้นอายุพร้อมหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
ในวันที่ ๒๘ มิถุนายน ๒๕๗๑

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายศิระ จันทรเจ็ด)

นักวิทยาศาสตร์เชี่ยวชาญ รักษาราชการแทน
ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน

ศูนย์วิจัยและเตือนภัยมลพิษโรงงานภาคตะวันออก

โทร. ๐ ๓๓๑๓ ๖๐๕๙ ต่อ ๕๐๐๑-๒

ไปรษณีย์อิเล็กทรอนิกส์ eirw@diw.mail.go.th



“อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา อุตสาหกรรมสีเขียว”





บริษัท ไทย เอ็มเอ็มเอ จำกัด
เลขที่ 88/6 นิคมอุตสาหกรรม อาร์ ไอ แอล
ตำบลมาบตาพุด อำเภอเมืองระยอง จังหวัดระยอง 21150 โทรศัพท์ +66(0)38-911835



บริษัท เอแอลเอส แล็บอราทอรี กรุ๊ป (ประเทศไทย) จำกัด
104 ซอยพัฒนาการ 40 ถนนพัฒนาการ แขวงพัฒนาการ เขตสวนหลวง กรุงเทพฯ 10250
โทรศัพท์ 0-2760-3000 โทรสาร 0-2760-3197
www.alsglobal.com