ภาคผนวก จ

เอกสารการสอบเทียบเครื่องมือตรวจวิเคราะห์

right solutions.
right partner.

รายการเครื่องมือที่ใช้ในการวิเคราะห์ / ทดสอบ

Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Stack	Total Suspended Particulate	Console Control Unit	BKK_FS0427	19-Nov-25	18-May-26	6
Stack	Total Suspended Particulate	Pitot Tube	BKK_FS0551	22-Oct-25	23-Apr-26	6
Stack	Total Suspended Particulate	Digital Balance	BKK_EN0309	29-Oct-25	29-Oct-26	12
Stack	Ammonia	Console Control Unit	BKK_FS0427	19-Nov-25	18-May-26	6
Stack	Ammonia	Pitot Tube	BKK_FS0551	22-Oct-25	23-Apr-26	6
Stack	Ammonia	DRYCAL FLOWMETER	BKK_FS0614	10-Sep-25	9-Sep-26	12
Stack	Ammonia	DRYCAL FLOWMETER	BKK_FS0619	10-Sep-25	9-Sep-26	12
Stack	Ammonia	Air Sampling Pump	NKH_FS0125	9-Feb-26	9-May-26	3
Stack	Ammonia	Spectrophotometer	BKK_EN0356	8-Oct-25	8-Oct-26	12
Stack (CEMs)	Oxides of Nitrogen	Analyzer , System calibration, Sta	-	-	-	-
Stack (CEMs)	Sulfur Dioxide	Analyzer , System calibration, Sta	-	-	-	-
Ambient	Nitrogen Dioxide	NO_2 Analyzer	BKK_FS0800	5-Jan-26	5-Jul-26	6
Ambient	Nitrogen Dioxide	NO_2 Analyzer	BKK_FS0785	5-Jan-26	5-Jul-26	6
Ambient	Nitrogen Dioxide	NO_2 Analyzer	BKK_FS1092	5-Jan-26	5-Jul-26	6
Ambient	Nitrogen Dioxide	NO_2 Analyzer	BKK_FS1457	5-Jan-26	5-Jul-26	6
Ambient	Sulfur Dioxide	SO_2 Analyzer	BKK_FS0799	5-Jan-26	5-Jul-26	6
Ambient	Sulfur Dioxide	SO_2 Analyzer	BKK_FS0784	5-Jan-26	5-Jul-26	6
Ambient	Sulfur Dioxide	SO_2 Analyzer	BKK_FS1091	5-Jan-26	5-Jul-26	6
Ambient	Sulfur Dioxide	SO_2 Analyzer	BKK_FS1456	5-Jan-26	5-Jul-26	6
Ambient	Particulate Matter (PM-10)	High Volume	BKK_FS1486	-	-	On site Calibration
Ambient	Particulate Matter (PM-10)	High Volume	BKK_FS1487	-	-	On site Calibration
Ambient	Particulate Matter (PM-10)	High Volume	BKK_FS1061	-	-	On site Calibration
Ambient	Particulate Matter (PM-10)	High Volume	BKK_FS1377	-	-	On site Calibration
Ambient	Particulate Matter (PM-10)	Digital Balance	BKK_EN0403	30-May-25	30-May-26	12
Ambient	Total Suspended Particulate	High Volume	BKK_FS1484	-	-	On site Calibration
Ambient	Total Suspended Particulate	High Volume	BKK_FS1485	-	-	On site Calibration
Ambient	Total Suspended Particulate	High Volume	BKK_FS0364	-	-	On site Calibration
Ambient	Total Suspended Particulate	High Volume	BKK_FS0370	-	-	On site Calibration
Ambient	Total Suspended Particulate	Digital Balance	BKK_EN0403	30-May-25	30-May-26	12
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	BKK_FS0917	25-Nov-24	25-May-26	18
Noise	Leq 24 hrs	Sound Calibrator	BKK_FS0632	9-Jan-26	8-Jan-27	12
Noise	Leq 24 hrs	Sound Level Meter	BKK_FS0109	27-Jan-26	26-Jan-27	12
Noise	Leq 24 hrs	Sound Level Meter	BKK_FS0107	2-Oct-25	1-Oct-26	12
Noise	Leq 24 hrs	Sound Level Meter	BKK_FS0108	27-Jan-26	26-Jan-27	12
Noise	Leq 24 hrs	Sound Level Meter	BKK_FS0106	2-Oct-25	1-Oct-26	12
Noise	Leq 8 hrs	Sound Calibrator	BKK_FS0618	24-Nov-25	23-Nov-26	12
Noise	Leq 8 hrs	Sound Level Meter	BKK_FS0099	4-Sep-25	3-Sep-26	12
Noise	Leq 8 hrs	Sound Level Meter	BKK_FS0113	27-Jan-26	26-Jan-27	12
Noise	Leq 8 hrs	Sound Level Meter	BKK_FS0111	15-Jan-26	14-Jan-27	12
Noise	Leq 8 hrs	Sound Level Meter	BKK_FS0930	28-Apr-25	28-Apr-26	12
Noise	Leq 8 hrs	Sound Level Meter	BKK_FS0116	27-Jan-26	26-Jan-27	12
Noise	Leq 8 hrs	Sound Level Meter	BKK_FS0880	18-Dec-25	17-Dec-26	12
Noise	Leq 8 hrs	Sound Calibrator	BKK_FS0630	16-Jul-25	15-Jul-26	12
Noise	Leq 8 hrs	Sound Level Meter	BKK_FS0876	15-Jan-26	14-Jan-27	12
Noise	Leq 8 hrs	Sound Level Meter	BKK_FS0875	15-Jan-26	14-Jan-27	12
Noise	Leq 8 hrs	Sound Level Meter	BKK_FS0930	16-Apr-26	15-Apr-27	12
Noise	Leq 8 hrs	Sound Level Meter	BKK_FS0929	27-Jan-26	26-Jan-27	12
Noise	Leq 8 hrs	Sound Level Meter	BKK_FS0993	29-Sep-25	28-Sep-26	12
Noise	Leq 8 hrs	Sound Level Meter	BKK_FS0995	24-Nov-25	23-Nov-26	12
Illuminance	Illuminance	Lux Meter	BKK_FS1345	20-Jan-26	19-Jan-27	12
Illuminance	Illuminance	Lux Meter	BKK_FS1395	21-Nov-25	20-Nov-26	12

right solutions.
right partner.

รายการเครื่องมือที่ใช้ในการวิเคราะห์ / ทดสอบ

Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Heat	Heat Stress	Heat Stress Monitor	BKK_FS0663	6-Jun-25	6-Jun-26	12
Heat	Heat Stress	Heat Stress Monitor	BKK_FS0681	19-Nov-25	18-Nov-26	12
Heat	Heat Stress	Heat Stress Monitor	BKK_FS0671	19-Nov-25	18-Nov-26	12
Heat	Heat Stress	Heat Stress Monitor	CHM_FS0099	2-Jul-25	2-Jul-26	12
Heat	Heat Stress	Heat Stress Monitor	CHM_FS0098	2-Jul-25	2-Jul-26	12
Heat	Heat Stress	Heat Stress Monitor	CHM_FS0104	3-Jul-25	2-Jul-26	12
Water Lab	Temperature	Digital Thermometer With Sensor	BKK_LG0059	5-Sep-25	5-Sep-26	12
Water Lab	COD	Spectrophotometer	BKK_EN0356	8-Oct-25	8-Oct-26	12
Water Lab	Iron	ICP-MS	BKK_EL0043	3-Oct-25	2-Oct-26	12
Water Lab	Iron	Hot Block	BKK_EL0054	4-Mar-25	4-Sep-26	18
Water Lab	Iron	Chamber (Cooling Room)	BKK_EN0167	4-Jun-25	4-Dec-26	18
Water Lab	Copper	ICP-MS	BKK_EL0043	3-Oct-25	2-Oct-26	12
Water Lab	Copper	Hot Block	BKK_EL0054	4-Mar-25	4-Sep-26	18
Water Lab	Copper	Chamber (Cooling Room)	BKK_EN0167	4-Jun-25	4-Dec-26	18
Water Lab	Zinc	ICP-MS	BKK_EL0043	3-Oct-25	2-Oct-26	12
Water Lab	Zinc	Hot Block	BKK_EL0054	4-Mar-25	4-Sep-26	18
Water Lab	Zinc	Chamber (Cooling Room)	BKK_EN0167	4-Jun-25	4-Dec-26	18
Water Lab	pH at 25 °C	pH meter	BKK_EN0342	9-Oct-25	9-Oct-26	12
Water Lab	Oil & Grease	Electronic Top-Loading Balance	BKK_EN0003	17-Jul-25	17-Jul-26	12
Water Lab	Oil & Grease	Water Bath	BKK_EN0439	9-Oct-25	9-Oct-26	12
Water Lab	Total Suspended Solids	Electronic Top-Loading Balance	BKK_EN0003	17-Jul-25	17-Jul-26	12
Water Lab	Total Suspended Solids	Oven	BKK_EN0425	6-Oct-25	6-Oct-26	12
Water Lab	Total Dissolved Solids 180°C	Electronic Top-Loading Balance	BKK_EN0003	17-Jul-25	17-Jul-26	12
Water Lab	Total Dissolved Solids 180°C	Oven	BKK_EN0425	6-Oct-25	6-Oct-26	12
Water Lab	Conductivity	Conductivity meter	BKK_EN0373	30-Jun-25	30-Jun-26	12
Water Lab	BOD	DO Meter	BKK_EN0017	20-May-25	20-Nov-26	18
Water Lab	BOD	Incubator	BKK_EN0305	23-Dec-25	23-Dec-26	12
Water Lab	BOD	Burette	BKK_EN0422	3-Sep-25	3-Sep-26	12

CONSOLE CONTROL UNIT CALIBRATION TEST REPORT

Calibration of Date **19-Nov-25**
Next Calibration Date 18-May-26
Certificate No. C-191125-BKK_FS0427

Barometric Pressure (mm.Hg) : **760.0**
Relative Humidity (%) : **69**
Temperature (˚C) : **30.0**

Console Control Meter Data

Dry Gas Meter ID **BKK_FS0427**
Brand APEX INSTRUMENT
Serial No. 1612
Model No. XC-572-V

Reference Dry Gas Meter Data

Reference Dry Gas Meter ID : **BKK_FS0629**
Serial No. : 1607009
Correction Factor (Y) : 1.000
Next Calibration Date : 10-Jan-26

ΔH ($mm.H_2O$)	Θ Minutes	Reference Dry Gas Meter Calibration				Console Control ; Drygas Meter						Dry Gas Meter Correction Factor (Y)	Orifice Calibration Factor ΔH@
		Vr (Liters)			Tr (°C)	Vm (Liters)			Ti (°C)	To (°C)	Avg.Tm (°C)		
		Final	Initial	Total		Final	Initial	Total					
15	11.64	150.10	0.00	150.10	30.0	36560.0	36410.0	150.00	31.0	31.0	31.0	1.0025	41.2581
25	9.20	150.10	0.00	150.10	30.0	36720.0	36570.0	150.00	31.0	31.0	31.0	1.0015	42.9564
50	6.65	150.03	0.00	150.03	31.0	36880.0	36730.0	150.00	32.0	32.0	32.0	0.9987	45.0782
80	5.28	150.23	0.00	150.23	31.0	37040.0	36890.0	150.00	32.0	32.0	32.0	0.9971	45.3475
120	4.30	150.06	0.00	150.06	32.0	37210.0	37060.0	150.00	32.0	32.0	32.0	0.9889	45.5145
											Avg.	0.9977	44.0309

Y : Ratio of reading of reference to dry gas meter : tolerance for individual values ± 0.02 from average .

ΔH@ : Orifice pressure differential that equates to 21.24 lm of air @ 25 C and 760 mm of mercury , mmH2O ; tolerance for individual values ± 5.08 from average .

Procedure; 40 CFR 60,APP A,METH ,SEC 5.3 & 7

Calibrated by: KRITSANA
(Mr.Kritsana Saiwan)
Field Services Scientist (2)

Approved by:
(Mr.Samart Roo-Ngan)
Field Services Specialist (1)

Issue date : 20-Nov-25

DIGITAL TEMPERATURE CALIBRATION DATA SHEET

Calibration Date :	19 Nov 25	Ambient Temperature (°C)	28.0
Calibration sheet No. :	C-191125-BKK_FS0427	Relative Humidity (%) :	69

Digital Temperature ID :	BKK_FS0427	Reference Temperature ID	BKK_FS1144
Serial No. :	1612	Serial No. :	201090006013
Model :	XC-572-V	Model :	Digicon-CC-VT-MS
		Next Calibrate :	16 Jan 26

Location	Reference Temperature °C	Digital Temperature °C	Error °C	MPE	Pass / Fail
Stack	0	2	2	±3	Pass
	25	23	-2	±3	Pass
	50	48	-2	±3	Pass
	100	98	-2	±3	Pass
	150	147	-3	±3	Pass
	200	197	-3	±3	Pass
	250	247	-3	±3	Pass
	300	297	-3	±3	Pass
	500	497	-3	±3	Pass
Probe	100	99	-1	±3	Pass
	120	119	-1	±3	Pass
	140	139	-1	±3	Pass
Oven	100	100	0	±3	Pass
	120	119	-1	±3	Pass
	140	139	-1	±3	Pass
Filter	100	98	-2	±3	Pass
	120	118	-2	±3	Pass
	140	139	-1	±3	Pass
Exit	0	2	2	±3	Pass
	10	12	2	±3	Pass
	20	21	1	±3	Pass
Meter	0	0	0	±3	Pass
	25	25	0	±3	Pass
	50	50	0	±3	Pass
AUX	0	2	2	±3	Pass
	25	23	-2	±3	Pass
	50	48	-2	±3	Pass

MPE : (Maximum permissible error of measurement) ค่าความผิดพลาดสูงสุดของการวัดที่ยอมได้

Calibrated by : Chawalit

(Mr.Chawalit wongchan)

Field Scientist (3)

Approved by :

Mr.Samart Roo-ngan

Specialist (1)

PROBE NOZZLE DIAMETER

CALIBRATION DATA SHEET

Calibration Date :	19 Nov 25	Nozzle Set ID. :	BKK_FS0427
Calibration Sheet No. : C-191125-BKK_FS0427		Vernier Caliper ID.:	RYG_FS0539


Nozzle ID #	Nozzle Diameter (cm.)			Hi - Lo	$(D_1 + D_2 + D_3) / 3$
	D_1	D_2	D_3	ΔD	D_{avg}
1	0.315	0.315	0.315	0.000	0.315
2	0.475	0.475	0.475	0.000	0.475
3	0.530	0.530	0.530	0.000	0.530
4	0.635	0.635	0.635	0.000	0.635
5	0.790	0.790	0.790	0.000	0.790
6	0.950	0.950	0.950	0.000	0.950
7	1.110	1.110	1.110	0.000	1.110
8	1.270	1.270	1.270	0.000	1.270
9	1.600	1.600	1.600	0.000	1.600

Where :

D_1, D_2, D_3 = There different nozzle diameters at 60 degrees to each other, each measured the nearest 0.025 mm.

ΔD = Maximum distance between any two diameters, must be $\leq$ 0.100 mm.

D_{avg} = $(D_1 + D_2 + D_3) / 3$

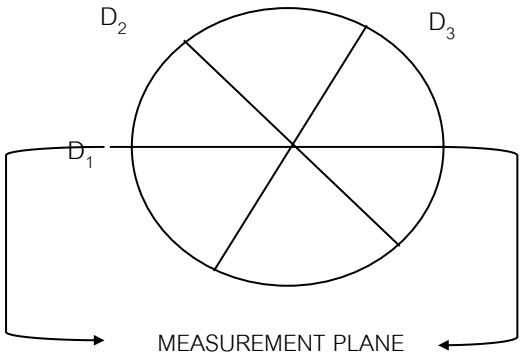

Calibrated by : Chawalit

(Mr. Chawalit Wongchan)

Field Scientist (3)


Approved by :

(Mr.Samart Roo-ngan)

Field Specialist (1)

Type S Pitot Tube Calibration

Date Calibration	22-Oct-25	**Due Date**	23-Apr-26
Pitot ID	BKK_FS0551	**Inclinometer ID**	BKK_FS1131
Pitot SN	-	**Vernier ID**	BKK_FS1405

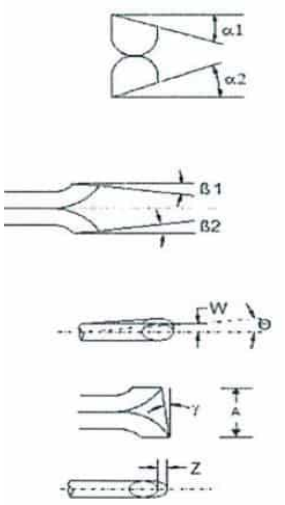

Parameter	Value	Allowable Range	Check
α1	2.4	-10° < α1 < +10°	OK
α2	-3.1	-10° < α2 < +10°	OK
β1	-0.4	-5° < β1 < +5°	OK
β2	9.3	-5° < β2 < +5°	OK
γ	1.3	-	-
θ	1.4	-	-
Z = A tan γ	0.020	Z ≤ 0.125"	OK
W = A tan θ	0.021	W ≤ 0.031"	OK
Dt	0.375	0.188" to 0.375"	OK
A/2Dt	1.160	1.05 ≤ PA/Dt ≤ 1.5	OK
A	0.87	2.1Dt ≤ A ≤ 3Dt	OK

Certify that pitot tube/porbe meets or exceeds all specifications, crieria and/or applicable design features and is hereby assigned a pitot tube certification fact of 0.84 . See 40 CFR Pt. 60, App. A,EPA Method 2.

Calibrated by : _____

(Mr.Prasert.Surakhan)

Enviro Field Services Scientist (3)

Approved By : _____

(Mr.Samart Roo-ngan)

Enviro Field Services Specialist (1)

Accredited by

NSC-TISI-TIS 17025
Calibration 0426

Calibration certificate

Calibration Certificate No. 25BCI0423

Object	Electronic non-automatic weighing instrument
Manufacturer	Sartorius
Type	SECURA224-1S
Serial | QM Ident. no.	38304165 | BKK_EN0309
Customer	ALS Laboratory Group (Thailand)Co., Ltd. 104 Phatthanakarn 40,Phattanakarn Rd.,Khwaeng Phatthanakarn ,Khet Suan Luang,Bangkok 10250
Order no.	272173
Number of pages	4
Date of calibration	29 Oct 2025

This calibration certificate documents the traceability to national standards.

Uncertainties of measurements are taken into account when only statements of compliance are made.

This certificate was prepared by Sartorius Corporation in accordance to the current ISO/IEC 17025:2017 standard and Sartorius Work Instruction (Method) SOP WI 08.

This certificate relate and apply this equipment only.

REVIEW BY ...Sinda K.....

APPROVED BY...Siriluk P.....

NEXT CAL DATE.....29/10/26.....

This calibration certificate may not be reproduced other than in full except with the permission of NSC-TISI-TIS-17025 and the issuing laboratory. Calibration certificates without signature are not valid.

The user is obliged to have the object recalibrated at appropriate intervals.

Date of issue	Approval of the Calibration Certificate	Person in charge
29 Oct 2025	Mr. Chonchai Inthana	Chonchai Inthana

Calibration object

Single range instrument

Model	SECURA224-1S
Serial Number	38304165
QM Ident. no | Inventory no.	BKK_EN0309 | ---

Maximum capacity (Max. load)	220.0000 g
Measured up to	220.0000 g
Scale interval	0.0001 g

Place of calibration

Address	According to page 1
Department | Cost center	Laboratory Department. | ---
Building | Floor	--- | 1st Floor.
Room	Laboratory Room.
Maximum temperature variation at place of calibration	5 K

Calibration procedure

EURAMET Calibration Guide No. 18, Version 4.0 (11/2015) - Guidelines on the Calibration of Non-Automatic Weighing Instruments

Test equipment

Test equipment type	Test equipment ID	Valid until
Thermometer	Testo 174(Traceable to Si unit through ENTECH)	11 Nov 2025
Test weight set OIML R111 E2	Certificate No.M2508149S ,E2(Traceable to SI unit through TCS)	19 Aug 2027

Adjustment Status

The measuring device was internally adjusted before the calibration.

Environmental and measuring conditions

Date of calibration	29 Oct 2025
Temperature at place of calibration | Temp. diff. $T_{weights}$ - T_{place}	20 °C | 0.5 K
Measuring conditions	The installation site is suitable. The device is level. Balance was loaded up to Max before test.
Comments	Humidity 62.0 %RH.

Measurement results | Measurement uncertainties

Repeatability

Test load (nominal): 10 g | 100 g		
	10 g	**100 g**
1	10.0000 g	100.0000 g
2	10.0001 g	100.0000 g
3	10.0000 g	100.0001 g
4	10.0000 g	100.0000 g
5	10.0000 g	100.0000 g
6	10.0000 g	100.0001 g
7	10.0001 g	100.0000 g
8	10.0000 g	100.0000 g
9	10.0000 g	99.9999 g
10	10.0000 g	100.0000 g
	s = 0.00004 g	s = 0.00006 g

Eccentricity

Test load (nominal):	**100 g**
Center	99.9999 g
Front left	99.9999 g
Back left	99.9999 g
Back right	99.9998 g
Front right	99.9999 g
Maximum deviation from centric loading indication $\lvert\Delta I_{ecc}\rvert_{max}$ = 0.0001 g	

Error of indication

Testload ***L***	**Indication** ***I***	**Error** ***E***	**Expansion factor** ***k***	**Uncertainty** ***U(E)***	**Uncertainty relative** $U_{rel}(E)$
0.0100 g	0.0100 g	0.0000 g	2.00	0.00012 g	1.2 %
0.0500 g	0.0500 g	0.0000 g	2.00	0.00014 g	0.28 %
0.1000 g	0.1000 g	0.0000 g	2.00	0.00014 g	0.14 %
0.5000 g	0.5000 g	0.0000 g	2.00	0.00014 g	0.028 %
1.0000 g	1.0000 g	0.0000 g	2.00	0.00014 g	0.014 %
2.0000 g	2.0000 g	0.0000 g	2.00	0.00014 g	0.0071 %
5.0000 g	5.0000 g	0.0000 g	2.00	0.00014 g	0.0029 %
10.0000 g	10.0000 g	0.0000 g	2.00	0.00015 g	0.0015 %
20.0000 g	20.0000 g	0.0000 g	2.00	0.00015 g	0.00075 %
200.0000 g	199.9999 g	-0.0001 g	2.00	0.00028 g	0.00014 %
210.0000 g	209.9999 g	-0.0001 g	2.00	0.00032 g	0.00015 %
Maximum error of indication		$\lvert E\rvert_{max}$ = 0.0001 g			

$U_{rel}(E)$ is the quotient of $U(E)$ and test load L. The uncertainty of measurement $U(E)$ is valid only if error E is considered. You will find reference notes on the uncertainty of measurement in use under: Appendix to the calibration certificate | Interpretation of measurement results.
Reference note: The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the documented Expansion factor, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

End of calibration certificate


Uncertainty of measurement in use

Device adjusted before measurement	Yes
Temperature deviation considered	1 K (isoCAL active)
Temperature coefficient considered	$2 \cdot 10^{-6}$/K
Uncertainty of the weighing result $U_{gl}(W)$	**$U_{gl}(W) = 0.00014\ g + 3.58 \cdot 10^{-6} \cdot R$**

Reference note: The current uncertainty of measurement is calculated by entering of the reading *R* into this formula. In relation to this, there is no need for a correction of the indication error. The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied with an Expansion factor of 2, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

Indication in % from max load	Net indication *R*	Uncertainty $U_{gl}(W)$	Uncertainty relative $U_{gl}(W)_{rel}$
1 %	2.2000 g	0.00015 g	0.0067 %
25 %	55.0000 g	0.00034 g	0.00061 %
50 %	110.0000 g	0.00053 g	0.00049 %
75 %	165.0000 g	0.00073 g	0.00044 %
100 %	220.0000 g	0.00093 g	0.00042 %

Graphic realization of the relative uncertainty of measurement | process accuracy

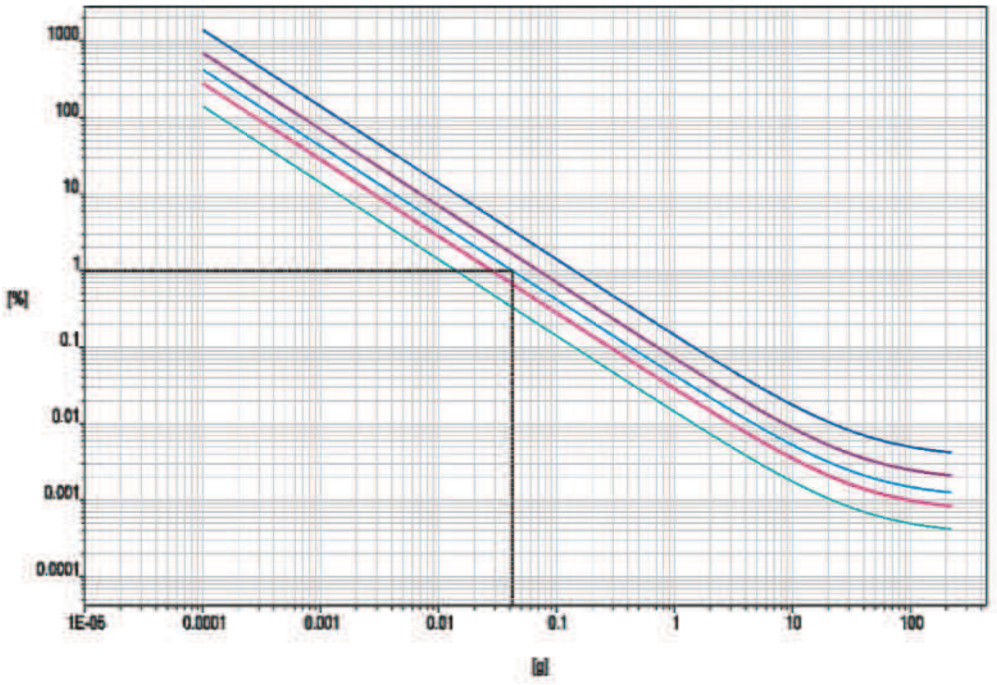

Safety factor
10
5
3
2
1

Displayed example

Process accuracy	1.00 %
Safety factor	3
Minimum sample weight	0.0420 g

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate of Calibration

Customer

Certificate No : 25-AFM-208

Name : ALS Laboratory Group Thailand Co., Ltd.

Request No : Req-2025-1986

Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang, Bangkok 10250

Unit Under Calibration Details

Measurement Item : Air Flow Meter

Manufacturer : Mesa Labs

Sensor Model : -

Model : 200-510M

Sensor Serial Number : -

Serial Number : 151114

Instrument Status : Used

ID : BKK_FS0614

Location of Calibration : LAB 4 AIR VELOCITY METER

REVIEW BY ..... Narakorn P.

APPROVED BY.....

NEXT CAL DATE..... 09/09/26

Calibration Environment and Details

Temperature : 23 ˚C ± 3 ˚C

Humidity : 55 %RH ± 20 %RH

Barometric Pressure : 1013 hPa ± 10 hPa

Received Date : 3 September 2025

Calibration Date : 10 September 2025

Calibration Procedure : In-house method CP-AFM-01 by Comparison technique with Standard Primary Flow Calibrator

Reference Standard	Model	Serial Number	Traceble	Due Calibration
Air Flow Meter	Gilibrator 3 Low flow	18501010006	Sensidyne	5 May 2026
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	6 May 2026
Temperature meter	GT 11	08000057	Qreborn	15 October 2025
Pressure meter	CPG2400	41000KDU/651882	TPA	21 October 2025

Traceability :

This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01 and MIT NSC-TISI-TIS Accreditation No. 0052

Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k = 2, providing a level of confidence approximately 95 %.

Calibration By :

Mr. Noppadon Luangart

Service Calibration Engineer

Approved By :

Mr. Pacit Mathavorn

Calibration Engineer Supervisor

Issue Date : 10 September 2025

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate No : 25-AFM-208

Request No : Req-2025-1986

Result of Calibration : Without Adjustment

STD Reading			UUC Readinng			Error	Uncertainty		
Temperature (°C)	Pressure (kPa)	Flow (cc/min)	Temperature (°C)	Pressure (kPa)	Flow (cc/min)	(cc/min)	(cc/min)	(°C)	(kPa)
25.5	100.98	100	-	-	100.02	0.0	3.6	1.0	0.50
25.7	100.97	503	-	-	500.81	-2.2	9.5	1.0	0.50
25.8	100.89	1003	-	-	1000.4	-3	19	1.0	0.50
26.1	100.88	2000	-	-	2001.9	2	38	1.0	0.50
26.5	100.85	3014	-	-	3002.2	-12	57	1.0	0.50
26.7	100.81	4027	-	-	4000.9	-26	76	1.0	0.50
27.0	100.74	5048	-	-	5001.8	-46	95	1.0	0.50

Note STD : Standard UUC : Unit Under Calibration

- UUC Reference Condition : At atmospheric pressure and room temperature condition, Air
- Flow Rate was corrected for non-standard operating condition by using equation :

$$Qmeas = \mathrm{Qref}\, x \frac{\mathrm{Pref}}{\mathrm{Pmeas}} x \frac{\mathrm{Tmeas}}{\mathrm{Tref}}$$

where Q = Flow Rate P = Absolute Pressure T = Absolute Temperature
meas = Measurement Condition ref = Standard Condition

* Indicates non accredited

End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate of Calibration

Customer

Certificate No : 25-AFM-207

Name : ALS Laboratory Group Thailand Co., Ltd.

Request No : Req-2025-1987

Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang, Bangkok 10250

Unit Under Calibration Details

Measurement Item : Air Flow Meter

Manufacturer : Mesa Labs

Sensor Model : -

Model : 200-510L

Sensor Serial Number : -

Serial Number : 130026

Instrument Status : Used

ID : BKK_FS0619

Location of Calibration : LAB 4 AIR VELOCITY METER

REVIEW BY ..... Narakorn P. .....

APPROVED BY .....

NEXT CAL DATE..... 09/09/26 .....

Calibration Environment and Details

Temperature : 23 °C ± 3 °C

Humidity : 55 %RH ± 20 %RH

Barometric Pressure : 1013 hPa ± 10 hPa

Received Date : 3 September 2025

Calibration Date : 10 September 2025

Calibration Procedure : In-house method CP-AFM-01 by Comparison technique with Standard Primary Flow Calibrator

Reference Standard	Model	Serial Number	Traceble	Due Calibration
Air Flow Meter	Gilibrator 3 Low flow	18501010006	Sensidyne	5 May 2026
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	6 May 2026
Temperature meter	GT 11	08000057	Qreborn	15 October 2025
Pressure meter	CPG2400	41000KDU/651882	TPA	21 October 2025

Traceability :

This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01 and MIT NSC-TISI-TIS Accreditation No. 0052

Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k = 2, providing a level of confidence approximately 95 %.

Calibration By :

Mr. Noppadon Luangart

Service Calibration Engineer

Approved By :

Mr. Pacit Mathavorn

Calibration Engineer Supervisor

Issue Date : 10 September 2025

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate No : 25-AFM-207

Request No : Req-2025-1987

Result of Calibration : Without Adjustment

STD Reading			UUC Readinng			Error	Uncertainty		
Temperature (°C)	Pressure (kPa)	Flow (cc/min)	Temperature (°C)	Pressure (kPa)	Flow (cc/min)	(cc/min)	(cc/min)	(°C)	(kPa)
25.5	100.98	20	-	-	20.042	0.0	1.6	1.0	0.50
25.5	100.90	50	-	-	49.921	-0.1	4.0	1.0	0.50
25.5	100.91	100	-	-	100.09	0.1	3.6	1.0	0.50
25.4	100.86	150	-	-	150.34	0.3	5.4	1.0	0.50
25.6	100.93	199	-	-	200.17	1.2	7.2	1.0	0.50
25.6	100.95	301	-	-	300.05	-1	11	1.0	0.50
25.7	100.96	402	-	-	401.03	-1	14	1.0	0.50
25.7	100.95	503	-	-	500.26	-3	10	1.0	0.50

Note STD : Standard UUC : Unit Under Calibration

- UUC Reference Condition : At atmospheric pressure and room temperature condition, Air

- Flow Rate was corrected for non-standard operating condition by using equation :

$$Qmeas = \mathrm{Qref}\, x\, \frac{\mathrm{Pref}}{\mathrm{Pmeas}}\, x\, \frac{\mathrm{Tmeas}}{\mathrm{Tref}}$$

where Q = Flow Rate P = Absolute Pressure T = Absolute Temperature

meas = Measurement Condition ref = Standard Condition

* Indicates non accredited

End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

ALS Laboratory Group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Phatthanakan, Suan Luang, Bangkok 10250
T +66 2 760 3000 F +66 2 760 3197

Certificate of Calibration

Certificate No. C-090226-NKH_FS0125

Air Sampling Pump Detail

Equipment name	: Personal Air Sampling Pump		Equiment ID	: NKH_FS0125
Brand	: Gilian		Serial No.	: 20221110028
Model/Type	: GilAir Plus		Calibration Date	: 09-Feb-26
			Next calibration date	: 09-May-26

Reference Standard Low Flow Meter

Equipment name	: Air Flow Meter		Equiment ID	: BKK_FS0619
Brand	: MesaLabs		Serial No.	: 130026
Model/Type	: Defender 510-L		Calibration Date	: 10-Sep-25
			Due Date	: 09-Sep-26

Reference Standard High Flow Meter

Equipment name	: Air Flow Meter		Equiment ID	: BKK_FS0614
Brand	: MesaLabs		Serial No.	: 151114
Model/Type	: Defender 510-M		Calibration Date	: 10-Sep-25
			Due Date	: 09-Sep-26

Calibration Data

Air Sampling Pump setting (cc/min)	Reference Std. Flow Reading (cc/min)			Avg. (cc/min)	%Error acceptance	Acceptable range (cc/min)			Evaluation (Pass/ Fail)
	1	2	3						
Low Flow									
20	19.6	19.7	20.0	19.7	5%	19	-	21	Passed
50	49.6	49.6	49.4	49.5	5%	48	-	53	Passed
100	99.2	99.4	99.5	99.3	5%	95	-	105	Passed
200	204.2	204.1	204.2	204.2	5%	190	-	210	Passed
High Flow									
500	503.2	505.3	506.6	505.1	3%	485	-	515	Passed
1000	996.8	995.3	1000.9	997.7	3%	970	-	1030	Passed
2000	2001.8	1996.6	2000.1	1999.5	3%	1940	-	2060	Passed
2500	2524.2	2527.5	2511.2	2521.0	3%	2425	-	2575	Passed

---------- END OF REPORT ----------

Calibrated By: .....

(Mr. Narupol Thongnuch)

BKK Field Services Scientist (2)

Approved By: .....

(Mr. Warakorn Pookrak)

Field Services Supervisor

Issue date : 10-Feb-26

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Certificate of Calibration

Cert.No.: 25CHO537
Page.: 1 of 3

Equipment :	Spectrophotometer
Manufacturer :	HACH
Model :	DR3900
Serial No. :	2021559
ID No. :	BKK_EN0356
Condition As-Received:	Used Item
Received Date :	08 October 2025
Calibration Date :	08 October 2025
Reference :	2510-0042OC-11
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand
Calibration Place :	Wet Chemistry Lab 2
Ambient Temperature :	(21.9 to 21.9) °C (On-Site)
Relative Humidity :	(62 to 65) % (On-Site)
Calibration Procedure :	In - house method : CP-OCH4 based on ASTM E 275-08

REVIEW BY ..... Sirida K.....

APPROVED BY ..... Siriluk P.....

NEXT CAL DATE..... 08/10/26.....

Calibrated by : Uthen Kankawi

Approved by : Saithip

Approved Signatory

( ) Chakrit Waewwanjua
( ) Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 9 October 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Condition of calibration result

1. Reference Standard Material :

Material	Serial No.	Certificate No.	Due date
1. Absorbance Standard set	44487	122584	31 May 2026
2. Wavelength Standard set	36730	118120	15 Jan 2026
3. Wavelength Standard set	36730	118121	15 Jan 2026

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certificate is traceable to the International System of Unit maintained through :
   - Starna Scientific Ltd.
4. Spectral BandWidth : 5 nm
   Scan Speed : - nm/min

Calibration Results : without adjustment

Wavelength Accuracy

Certified Values of Reference Material (nm)	UUC Reading (nm)	Uncertainty of Measurement (± nm)	Coverage Factor *k*
418.40	418	0.59	2.00
479.88	480	0.59	2.00
513.75	513	0.59	2.00
537.00	536	0.59	2.00
638.00	638	0.59	2.00
747.61	748	0.59	2.00
807.04	807	0.59	2.00

Calibration Results : without adjustment

Photometric Accuracy

Wavelength (nm)	Certified Values of Reference Material (Abs)	UUC Reading (Abs)	Uncertainty of Measurement (±Abs)	Coverage Factor *k*
420.0	Zero	0.000	0.0028	2.00
	0.5750	0.573	0.0028	2.00
	0.7156	0.713	0.0028	2.00
	1.0176	1.014	0.0028	2.00
440.0	Zero	0.000	0.0028	2.00
	0.5598	0.557	0.0028	2.00
	0.7037	0.700	0.0028	2.00
	1.0013	0.997	0.0028	2.00
465.0	Zero	0.000	0.0028	2.00
	0.5222	0.522	0.0028	2.00
	0.6646	0.664	0.0028	2.00
	0.9444	0.945	0.0028	2.00
546.1	Zero	0.000	0.0028	2.00
	0.5234	0.523	0.0028	2.00
	0.7007	0.700	0.0028	2.00
	0.9992	0.999	0.0028	2.00
590.0	Zero	0.000	0.0028	2.00
	0.5573	0.556	0.0028	2.00
	0.7760	0.773	0.0028	2.00
	1.1104	1.108	0.0028	2.00
635.0	Zero	0.000	0.0028	2.00
	0.5648	0.565	0.0028	2.00
	0.7654	0.765	0.0028	2.00
	1.0961	1.096	0.0028	2.00

Remark

- Each individual filter is measured against the empty filter holder (blank) used to zero the spectrophotometer
- UUC = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k* , providing a level of confidence of approximately 95 %.

-o0o-

Lot No. 2622735-1

ANALYZER CALIBRATION DATA

Client : **Hin Kong Power Company Limited** **Location** : **ปล่องระบายมลสารของโรงไฟฟ้า หน่วยการผลิตที่ 1 (HRSG Stack Unit 1)**

Date : **17 Mar 26** **Test Operator** : **Ussaree N.**

O_2 ANALYZER

Model : **TELEDYNE API 200EH** **Serial No.** : **549**

Span (%) : **25**

	Cylinder Value (%)	Initial Analyzers Calibration Response (%)	Final Analyzers Calibration Response (%)	Difference (Percent of Span)
Zero Gas	0.00	0.00	0.00	0.00
Low-Level Gas	8.05	8.02	7.99	0.12
Span Gas	16.11	16.12	16.14	0.08

NO_X ANALYZER

Model : **TELEDYNE API 200EH** **Serial No.** : **549**

Span (ppm) : **100**

	Cylinder Value (ppm)	Initial Analyzers Calibration Response (ppm)	Final Analyzers Calibration Response (ppm)	Difference (Percent of Span)
Zero Gas	0.00	0.00	0.03	0.03
Low-Level Gas	55.38	54.91	54.55	0.36
Span Gas	81.83	81.81	81.38	0.43

SO2 ANALYZER

Model : **TELEDYNE API 100EH** **Serial No.** : **282**

Span (ppm) : **100**

	Cylinder Value (ppm)	Initial Analyzers Calibration Response (ppm)	Final Analyzers Calibration Response (ppm)	Difference (Percent of Span)
Zero Gas	0.00	0.00	0.01	0.01
Low-Level Gas	55.31	55.15	54.89	0.26
Span Gas	80.36	80.27	79.64	0.63

Calibrated by

Ussaree N.

Ussaree Namburee

BKK Field Services Scientist (4)

Lot No. 2622735-1

SYSTEM CALIBRATION BIAS AND DRIFT DATA

Client	:	**Hin Kong Power Company Limited**	**Location**	:	**ปล่องระบายมลสารของโรงไฟฟ้า หน่วยการผลิตที่ 1 (HRSG Stack Unit 1)**
Date	:	**17 Mar 26**	**Test Operator**	:	**Ussaree N.**

O_2 ANALYZER

Cylinder Conc. (%) : **16.11** **Span (%)** : **25**

	O_2 Analyzer Calibration Response	Initial Values		Final Values		Drift (% of Span)
		System Calibration Response	System Cal Bias (% of Span)	System Calibration Response	System Cal Bias (% of Span)	
Zero Gas	0.00	0.01	0.04	0.01	0.04	0.00
Upscale Gas	16.12	16.16	0.16	16.20	0.32	0.16

NO_X ANALYZER

Cylinder Conc. (ppm) : **81.83** **Span (ppm)** : **100**

	NO_X Analyzer Calibration Response	Initial Values		Final Values		Drift (% of Span)
		System Calibration Response	System Cal Bias (% of Span)	System Calibration Response	System Cal Bias (% of Span)	
Zero Gas	0.00	0.04	0.04	0.07	0.07	0.03
Upscale Gas	81.81	79.48	2.33	79.61	2.20	0.13

SO_2 ANALYZER

Cylinder Conc. (ppm) : **80.36** **Span (ppm)** : **100**

	SO_2 Analyzer Calibration Response	Initial Values		Final Values		Drift (% of Span)
		System Calibration Response	System Cal Bias (% of Span)	System Calibration Response	System Cal Bias (% of Span)	
Zero Gas	0.00	0.01	0.01	0.01	0.01	0.00
Upscale Gas	80.27	79.39	0.88	79.08	1.19	0.31

Calibrated by

Ussaree N.

Ussaree Namburee

BKK Field Services Scientist (4)

EMISSION TEST RESULT

		Run #	1
Client	Hin Kong Power Company Limited	Location	ปล่องระบายมลสารของโรงไฟฟ้า หน่วยการผลิตที่ 1 (HRSG Stack Unit 1)
Date	17 Mar 26	Test Operator	Ussaree N.
Start Time	12:30	Finish Time	12:50
SO_2 Analyzer Model	TELEDYNE API 100EH	Serial No.	282
NO_x/O_2 Analyzer Model	TELEDYNE API 200EH	Serial No.	549
CO/CO_2 Analyzer Model	TELEDYNE API T300M	Serial No.	845

Time (min)	O_2 (%)	CO_2 (%)	NOx (ppm)	SO_2 (ppm)	CO (ppm)	Remark
12:30	12.47	5.00	19.51	0.34	-	
12:31	12.45	5.00	18.95	0.34	-	
12:32	12.36	5.06	19.76	0.37	-	
12:33	12.30	5.12	21.42	0.34	-	
12:34	12.45	5.05	21.22	0.37	-	
12:35	12.47	5.02	19.60	0.34	-	
12:36	12.43	5.04	19.11	0.36	-	
12:37	12.32	5.10	20.29	0.38	-	
12:38	12.27	5.14	22.07	0.86	-	
12:39	12.21	5.15	24.00	0.50	-	
12:40	12.19	5.22	25.74	0.56	-	
12:41	12.25	5.18	25.57	0.46	-	
12:42	12.23	5.17	25.07	0.55	-	
12:43	12.27	5.16	24.51	0.49	-	
12:44	12.45	5.03	17.67	0.50	-	
12:45	12.48	4.99	17.67	0.45	-	
12:46	12.44	5.04	18.27	0.49	-	
12:47	12.51	4.97	17.97	0.40	-	
12:48	12.47	5.00	17.54	0.51	-	
12:49	12.51	4.97	17.61	0.45	-	
12:50	12.50	4.99	17.80	0.53	-	
Average	**12.39**	**5.07**	**20.54**	**0.45**	**-**	

Ussaree N.

Ussaree Namburee

BKK Field Services Scientist (4)

EMISSION TEST RESULT

		Run #	2
Client	Hin Kong Power Company Limited	Location	ปล่องระบายมลสารของโรงไฟฟ้า หน่วยการผลิตที่ 1 (HRSG Stack Unit 1)
Date	17 Mar 26	Test Operator	Ussaree N.
Start Time	12:51	Finish Time	13:11
SO_2 Analyzer Model	TELEDYNE API 100EH	Serial No.	282
NO_x/O_2 Analyzer Model	TELEDYNE API 200EH	Serial No.	549
CO/CO_2 Analyzer Model	TELEDYNE API T300M	Serial No.	845

Time (min)	O_2 (%)	CO_2 (%)	NOx (ppm)	SO_2 (ppm)	CO (ppm)	Remark
12:51	12.43	5.02	18.20	0.41	-	
12:52	12.30	5.12	19.82	0.44	-	
12:53	12.24	5.13	22.09	0.46	-	
12:54	12.19	5.15	24.42	0.45	-	
12:55	12.26	5.14	24.75	0.44	-	
12:56	12.27	5.13	24.36	0.47	-	
12:57	12.29	5.13	23.72	0.92	-	
12:58	12.31	5.11	23.19	0.47	-	
12:59	12.32	5.08	22.16	0.46	-	
13:00	12.29	5.12	21.81	0.45	-	
13:01	12.34	5.07	21.72	0.41	-	
13:02	12.33	5.09	21.43	0.45	-	
13:03	12.27	5.12	21.60	0.48	-	
13:04	12.30	5.12	22.57	0.51	-	
13:05	12.41	5.04	21.42	0.54	-	
13:06	12.30	5.10	20.31	0.08	-	
13:07	12.25	5.14	21.87	0.09	-	
13:08	12.23	5.16	23.75	0.59	-	
13:09	12.31	5.12	23.87	0.53	-	
13:10	12.29	5.11	23.46	0.61	-	
13:11	12.31	5.11	23.12	0.54	-	
Average	**12.30**	**5.11**	**22.36**	**0.46**	**-**	

Ussaree N.

Ussaree Namburee

BKK Field Services Scientist (4)

EMISSION TEST RESULT

		Run #	3
Client	Hin Kong Power Company Limited	Location	ปล่องระบายมลสารของโรงไฟฟ้า หน่วยการผลิตที่ 1 (HRSG Stack Unit 1)
Date	17 Mar 26	Test Operator	Ussaree N.
Start Time	13:12	Finish Time	13:32
SO_2 Analyzer Model	TELEDYNE API 100EH	Serial No.	282
NO_x/O_2 Analyzer Model	TELEDYNE API 200EH	Serial No.	549
CO/CO_2 Analyzer Model	TELEDYNE API T300M	Serial No.	845

Time (min)	O_2 (%)	CO_2 (%)	NOx (ppm)	SO_2 (ppm)	CO (ppm)	Remark
13:12	12.29	5.12	23.05	0.13	-	
13:13	12.26	5.15	22.94	0.57	-	
13:14	12.33	5.11	22.78	0.60	-	
13:15	12.34	5.07	22.05	0.54	-	
13:16	12.31	5.09	22.05	0.63	-	
13:17	12.34	5.09	22.27	0.53	-	
13:18	12.31	5.09	22.34	0.56	-	
13:19	12.25	5.12	22.52	0.50	-	
13:20	12.36	5.07	22.56	0.48	-	
13:21	12.53	4.98	20.41	0.47	-	
13:22	12.50	4.96	17.74	0.45	-	
13:23	12.35	5.09	17.86	0.62	-	
13:24	12.28	5.14	20.39	0.63	-	
13:25	12.26	5.15	22.16	0.71	-	
13:26	12.31	5.11	22.45	0.64	-	
13:27	12.27	5.11	23.20	0.75	-	
13:28	12.25	5.14	24.09	0.65	-	
13:29	12.29	5.10	24.37	0.71	-	
13:30	12.29	5.11	23.23	0.67	-	
13:31	12.25	5.13	23.46	0.74	-	
13:32	12.28	5.14	24.20	0.67	-	
Average	**12.32**	**5.10**	**22.20**	**0.58**	**-**	

Ussaree N.

Ussaree Namburee

BKK Field Services Scientist (4)

Lot No. 2622736-1

ANALYZER CALIBRATION DATA

Client	:	**Hin Kong Power Company Limited**	**Location**	:	**ปล่องระบายมลสารของโรงไฟฟ้า หน่วยการผลิตที่ 2 (HRSG Stack Unit 2)**
Date	:	**18 Mar 26**	**Test Operator**	:	**Ussaree N.**

O_2 ANALYZER

Model	:	**TELEDYNE API 200EH**	**Serial No.**	:	**549**
Span (%)	:	**25**			

	Cylinder Value (%)	Initial Analyzers Calibration Response (%)	Final Analyzers Calibration Response (%)	Difference (Percent of Span)
Zero Gas	0.00	0.00	0.00	0.00
Low-Level Gas	8.05	8.06	8.03	0.12
Span Gas	16.11	16.10	16.13	0.12

NO_X ANALYZER

Model	:	**TELEDYNE API 200EH**	**Serial No.**	:	**549**
Span (ppm)	:	**100**			

	Cylinder Value (ppm)	Initial Analyzers Calibration Response (ppm)	Final Analyzers Calibration Response (ppm)	Difference (Percent of Span)
Zero Gas	0.00	0.00	0.04	0.04
Low-Level Gas	55.38	55.04	54.87	0.17
Span Gas	81.83	81.79	81.24	0.55

SO2 ANALYZER

Model	:	**TELEDYNE API 100EH**	**Serial No.**	:	**282**
Span (ppm)	:	**100**			

	Cylinder Value (ppm)	Initial Analyzers Calibration Response (ppm)	Final Analyzers Calibration Response (ppm)	Difference (Percent of Span)
Zero Gas	0.00	0.00	0.00	0.00
Low-Level Gas	55.31	55.20	54.91	0.29
Span Gas	80.36	80.32	79.88	0.44

Calibrated by

Ussaree N.

Ussaree Namburee

BKK Field Services Scientist (4)

Lot No. 2622736-1

SYSTEM CALIBRATION BIAS AND DRIFT DATA

Client	:	**Hin Kong Power Company Limited**	**Location**	:	**ปล่องระบายมลสารของโรงไฟฟ้า หน่วยการผลิตที่ 2 (HRSG Stack Unit 2)**
Date	:	**18 Mar 26**	**Test Operator**	:	**Ussaree N.**

O_2 ANALYZER

Cylinder Conc. (%) : **16.11** **Span (%)** : **25**

	O_2 Analyzer Calibration Response	Initial Values		Final Values		Drift (% of Span)
		System Calibration Response	System Cal Bias (% of Span)	System Calibration Response	System Cal Bias (% of Span)	
Zero Gas	0.00	0.00	0.00	0.02	0.08	0.08
Upscale Gas	16.10	16.15	0.20	16.18	0.32	0.12

NO_X ANALYZER

Cylinder Conc. (ppm) : **81.83** **Span (ppm)** : **100**

	NO_X Analyzer Calibration Response	Initial Values		Final Values		Drift (% of Span)
		System Calibration Response	System Cal Bias (% of Span)	System Calibration Response	System Cal Bias (% of Span)	
Zero Gas	0.00	0.03	0.03	0.05	0.05	0.02
Upscale Gas	81.79	80.55	1.24	79.94	1.85	0.61

SO_2 ANALYZER

Cylinder Conc. (ppm) : **80.36** **Span (ppm)** : **100**

	SO_2 Analyzer Calibration Response	Initial Values		Final Values		Drift (% of Span)
		System Calibration Response	System Cal Bias (% of Span)	System Calibration Response	System Cal Bias (% of Span)	
Zero Gas	0.00	0.00	0.00	0.01	0.01	0.01
Upscale Gas	80.32	79.31	1.01	79.56	0.76	0.25

Calibrated by

Ussaree N.

Ussaree Namburee

BKK Field Services Scientist (4)

EMISSION TEST RESULT

		Run #	1
Client	Hin Kong Power Company Limited	Location	ปล่องระบายมลสารของโรงไฟฟ้า หน่วยการผลิตที่ 2 (HRSG Stack Unit 2)
Date	18 Mar 26	Test Operator	Ussaree N.
Start Time	11:40	Finish Time	12:00
SO_2 Analyzer Model	TELEDYNE API 100EH	Serial No.	282
NO_x/O_2 Analyzer Model	TELEDYNE API 200EH	Serial No.	549
CO/CO_2 Analyzer Model	TELEDYNE API T300M	Serial No.	845

Time (min)	O_2 (%)	CO_2 (%)	NOx (ppm)	SO_2 (ppm)	CO (ppm)	Remark
11:40	12.58	5.01	14.73	0.27	-	
11:41	12.46	5.15	15.50	0.68	-	
11:42	12.41	5.16	16.56	0.73	-	
11:43	12.39	5.17	17.43	0.69	-	
11:44	12.34	5.18	17.95	0.76	-	
11:45	12.36	5.20	18.46	0.68	-	
11:46	12.40	5.15	18.17	0.62	-	
11:47	12.38	5.16	17.54	0.71	-	
11:48	12.36	5.16	17.73	0.75	-	
11:49	12.59	5.02	16.63	0.64	-	
11:50	12.58	5.04	14.46	0.74	-	
11:51	12.46	5.10	14.76	0.66	-	
11:52	12.56	5.04	15.25	0.74	-	
11:53	12.42	5.14	15.54	0.70	-	
11:54	12.36	5.18	16.60	0.78	-	
11:55	12.37	5.17	17.83	0.70	-	
11:56	12.38	5.17	17.84	0.74	-	
11:57	12.52	5.03	16.70	0.41	-	
11:58	12.51	5.07	15.50	0.37	-	
11:59	12.39	5.15	15.35	0.42	-	
12:00	12.34	5.19	16.94	0.43	-	
Average	**12.43**	**5.13**	**16.55**	**0.63**	**-**	

Ussaree N.

Ussaree Namburee

BKK Field Services Scientist (4)

EMISSION TEST RESULT

		Run #	2
Client	Hin Kong Power Company Limited	Location	ปล่องระบายมลสารของโรงไฟฟ้า หน่วยการผลิตที่ 2 (HRSG Stack Unit 2)
Date	18 Mar 26	Test Operator	Ussaree N.
Start Time	12:01	Finish Time	12:21
SO_2 Analyzer Model	TELEDYNE API 100EH	Serial No.	282
NO_x/O_2 Analyzer Model	TELEDYNE API 200EH	Serial No.	549
CO/CO_2 Analyzer Model	TELEDYNE API T300M	Serial No.	845

Time (min)	O_2 (%)	CO_2 (%)	NOx (ppm)	SO_2 (ppm)	CO (ppm)	Remark
12:01	12.30	5.21	18.84	0.45	-	
12:02	12.34	5.19	19.28	0.43	-	
12:03	12.34	5.18	18.94	0.45	-	
12:04	12.30	5.21	18.87	0.44	-	
12:05	12.37	5.19	19.01	0.68	-	
12:06	12.49	5.08	18.06	0.73	-	
12:07	12.52	5.05	17.15	0.67	-	
12:08	12.56	5.03	16.36	0.70	-	
12:09	12.47	5.08	16.10	0.67	-	
12:10	12.39	5.15	16.75	0.31	-	
12:11	12.35	5.18	17.82	0.30	-	
12:12	12.35	5.18	18.31	0.31	-	
12:13	12.30	5.18	18.78	0.69	-	
12:14	12.32	5.18	19.18	0.77	-	
12:15	12.34	5.17	19.49	0.65	-	
12:16	12.51	5.05	17.80	0.64	-	
12:17	12.53	5.08	16.60	0.43	-	
12:18	12.49	5.09	15.85	0.84	-	
12:19	12.55	5.03	15.99	0.44	-	
12:20	12.49	5.09	15.85	0.46	-	
12:21	12.61	5.00	15.19	0.43	-	
Average	**12.42**	**5.12**	**17.63**	**0.55**	**-**	

Ussaree N.

Ussaree Namburee

BKK Field Services Scientist (4)

EMISSION TEST RESULT

		Run #	3
Client	Hin Kong Power Company Limited	Location	ปล่องระบายมลสารของโรงไฟฟ้า หน่วยการผลิตที่ 2 (HRSG Stack Unit 2)
Date	18 Mar 26	Test Operator	Ussaree N.
Start Time	12:22	Finish Time	12:42
SO_2 Analyzer Model	TELEDYNE API 100EH	Serial No.	282
NO_x/O_2 Analyzer Model	TELEDYNE API 200EH	Serial No.	549
CO/CO_2 Analyzer Model	TELEDYNE API T300M	Serial No.	845

Time (min)	O_2 (%)	CO_2 (%)	NOx (ppm)	SO_2 (ppm)	CO (ppm)	Remark
12:22	12.48	5.10	15.06	0.47	-	
12:23	12.37	5.16	16.06	0.48	-	
12:24	12.42	5.09	17.25	0.44	-	
12:25	12.53	5.04	16.59	0.47	-	
12:26	12.41	5.15	16.23	0.48	-	
12:27	12.36	5.15	17.45	0.48	-	
12:28	12.53	5.04	17.23	0.46	-	
12:29	12.62	5.00	15.28	0.46	-	
12:30	12.55	5.02	13.68	0.46	-	
12:31	12.53	5.05	13.92	0.47	-	
12:32	12.39	5.16	15.48	0.45	-	
12:33	12.34	5.18	17.11	0.61	-	
12:34	12.30	5.20	18.54	0.68	-	
12:35	12.52	5.05	17.98	0.60	-	
12:36	12.45	5.07	16.98	0.67	-	
12:37	12.50	5.04	16.34	0.60	-	
12:38	12.58	5.01	16.07	0.57	-	
12:39	12.44	5.13	15.91	0.69	-	
12:40	12.38	5.16	16.72	0.64	-	
12:41	12.51	5.02	17.01	0.66	-	
12:42	12.52	5.04	16.03	0.63	-	
Average	**12.46**	**5.09**	**16.33**	**0.55**	**-**	

Ussaree N.

Ussaree Namburee

BKK Field Services Scientist (4)

Airgas
an Air Liquide company

Airgas Specialty Gases
Airgas USA LLC
6141 Easton Road
Plumsteadville, PA 18949
Airgas.com

CERTIFICATE OF ANALYSIS

Grade of Product: EPA PROTOCOL STANDARD

Customer:	AIR LIQUIDE (THAILAND) LTD		
Part Number:	E04NI99E15A0664	Reference Number:	160-402885484-1
Cylinder Number:	EB0171192	Cylinder Volume:	144.0 CF
Laboratory:	124 - Plumsteadville - PA	Cylinder Pressure:	2015 PSIG
PGVP Number:	A12023	Valve Outlet:	660
Gas Code:	CO,NO,NOX,SO2,BALN	Certification Date:	Nov 17, 2023

Expiration Date: Nov 17, 2031

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results relate only to the items tested. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS

Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	55.00 PPM	55.38 PPM	G1	+/- 1.4% NIST Traceable	11/10/2023, 11/17/2023
CARBON MONOXIDE	55.00 PPM	56.29 PPM	G1	+/- 0.7% NIST Traceable	11/10/2023
NITRIC OXIDE	55.00 PPM	55.36 PPM	G1	+/- 1.3% NIST Traceable	11/10/2023, 11/17/2023
SULFUR DIOXIDE	55.00 PPM	55.31 PPM	G1	+/- 0.9% NIST Traceable	11/10/2023, 11/17/2023
NITROGEN	Balance				

CALIBRATION STANDARDS

Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
NTRM	120112-32	KAL004540	49.24 PPM CARBON MONOXIDE/NITROGEN	+/- 0.6%	Aug 31, 2024
PRM	12409	D913660	15.01 PPM NITROGEN DIOXIDE/AIR	+/- 1.5%	Feb 17, 2023
GMIS	402531833-1-1	CC202889	49.73 PPM NITRIC OXIDE/NITROGEN	+/- 1.0%	Oct 13, 2025
SRM	1693a	FF25467	50.33 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.7%	Jun 27, 2023
GMIS	401648675101	CC500133	4.981 PPM NITROGEN DIOXIDE/NITROGEN	+/- 1.6%	Sep 29, 2025
GMIS	071220222B17	EB0141234	50.05 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.7%	Dec 21, 2026

The SRM, NTRM, PRM, or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet iS50 FTIR AUP2010245 CO	FTIR	Nov 09, 2023
Nicolet iS50 FTIR AUP2010245 NO	FTIR	Nov 16, 2023
Nicolet iS50 FTIR AUP2010245 NO2	FTIR	Nov 02, 2023
Nicolet iS50 FTIR AUP2010245 SO2	FTIR	Oct 26, 2023

Triad Data Available Upon Request

NOTES: Gross Weight: 27.79Kg
Net Weight: 4.82 Kg

Approved for Release

Airgas
an Air Liquide company

Airgas Specialty Gases
Airgas USA LLC
6141 Easton Road
Plumsteadville, PA 18949
Airgas.com

CERTIFICATE OF ANALYSIS

Grade of Product: EPA PROTOCOL STANDARD

Customer:	AIR LIQUIDE (THAILAND) LTD		
Part Number:	E04NI99E15A0440	Reference Number:	160-402885483-1
Cylinder Number:	EB0171195	Cylinder Volume:	144.0 CF
Laboratory:	124 - Plumsteadville - PA	Cylinder Pressure:	2015 PSIG
PGVP Number:	A12023	Valve Outlet:	660
Gas Code:	CO,NO,NOX,SO2,BALN	Certification Date:	Nov 21, 2023

Expiration Date: Nov 21, 2031

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results relate only to the items tested. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS

Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	80.00 PPM	81.83 PPM	G1	+/- 0.7% NIST Traceable	11/13/2023, 11/21/2023
CARBON MONOXIDE	80.00 PPM	80.27 PPM	G1	+/- 0.5% NIST Traceable	11/13/2023
NITRIC OXIDE	80.00 PPM	81.83 PPM	G1	+/- 0.7% NIST Traceable	11/13/2023, 11/21/2023
SULFUR DIOXIDE	80.00 PPM	80.36 PPM	G1	+/- 0.8% NIST Traceable	11/13/2023, 11/21/2023
NITROGEN	Balance				

CALIBRATION STANDARDS

Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
NTRM	110101-08	KAL003090	97.31 PPM CARBON MONOXIDE/NITROGEN	+/- 0.4%	May 25, 2028
PRM	C2219101	APE1514048	100.19 PPM NITRIC OXIDE/NITROGEN	+/- 0.3%	Feb 28, 2025
GMIS	2023042502	CC754074	98.48 PPM NITRIC OXIDE/NITROGEN	+/- 0.4%	May 25, 2031
PRM	12409	D913660	15.01 PPM NITROGEN DIOXIDE/AIR	+/- 1.5%	Feb 17, 2023
GMIS	401648675101	CC500133	4.981 PPM NITROGEN DIOXIDE/NITROGEN	+/- 1.6%	Sep 29, 2025
NTRM	160102-22	KAL003820	97.69 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.8%	Nov 01, 2027

The SRM, NTRM, PRM, or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet iS50 FTIR AUP2010245 CO	FTIR	Nov 09, 2023
Nicolet iS50 FTIR AUP2010245 NO	FTIR	Nov 16, 2023
Nicolet iS50 FTIR AUP2010245 NO2	FTIR	Nov 02, 2023
Nicolet iS50 FTIR AUP2010245 SO2	FTIR	Oct 26, 2023

Triad Data Available Upon Request

NOTES: Gross Weight: 27.8 Kg
Net Weight: 4.8 Kg

Approved for Release

6

Airgas
an Air Liquide company

Airgas Specialty Gases
Airgas USA LLC
6141 Easton Road
Plumsteadville, PA 18949
Airgas.com

CERTIFICATE OF ANALYSIS

Grade of Product: EPA PROTOCOL STANDARD

Customer:	AIR LIQUIDE (THAILAND) LTD		
Part Number:	E02NI92E15A3100	Reference Number:	160-403186618-1
Cylinder Number:	EB0172556	Cylinder Volume:	145.0 CF
Laboratory:	124 - Plumsteadville - PA	Cylinder Pressure:	2015 PSIG
PGVP Number:	A12024	Valve Outlet:	590
Gas Code:	O2,BALN	Certification Date:	Nov 11, 2024

Expiration Date: Nov 11, 2032

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results relate only to the items tested. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS

Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
OXYGEN	8.000 %	8.049 %	G1	+/- 0.4% NIST Traceable	11/11/2024
NITROGEN	Balance				

CALIBRATION STANDARDS

Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
NTRM	060602	CC263047	9.96 % OXYGEN/NITROGEN	+/-0.3%	Jun 27, 2030

ANALYTICAL EQUIPMENT

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
SIEMENS OXYMAT 6 - N1-W5-951 - O2	PARAMAGNETIC	Oct 30, 2024

Triad Data Available Upon Request

NOTES: Gross Weight: 27.7 Kg
Net Weight: 4.8 Kg

Approved for Release

Airgas
an Air Liquide company

Airgas Specialty Gases
Airgas USA LLC
6141 Easton Road
Plumsteadville, PA 18949
Airgas.com

CERTIFICATE OF ANALYSIS

Grade of Product: EPA PROTOCOL STANDARD

Customer:	AIR LIQUIDE (THAILAND) LTD		
Part Number:	E02NI84E15A07B7	Reference Number:	160-403186616-1
Cylinder Number:	EB0172564	Cylinder Volume:	146.0 CF
Laboratory:	124 - Plumsteadville - PA	Cylinder Pressure:	2015 PSIG
PGVP Number:	A12024	Valve Outlet:	590
Gas Code:	O2,BALN	Certification Date:	Nov 12, 2024

Expiration Date: Nov 12, 2032

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results relate only to the items tested. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS

Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
OXYGEN	16.00 %	16.11 %	G1	+/- 0.3% NIST Traceable	11/12/2024
NITROGEN	Balance				

CALIBRATION STANDARDS

Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
NTRM	220605	CC745621	23.124 % OXYGEN/NITROGEN	+/-0.2%	Mar, 31, 2028

ANALYTICAL EQUIPMENT

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
SIEMENS OXYMAT 6 - N1-W5-951 - O2	PARAMAGNETIC	Oct 30, 2024

Triad Data Available Upon Request


NOTES: Gross Weight: 27.6 Kg
Net Weight: 4.9 Kg

Approved for Release

MULTIPOINT CALIBRATION REPORT

Calibration Date	5-Jan-26	Equipment Name	NOx Analyzer
Manufacturer	HORIBA	Model	APNA-370
Serial No.	HCWSR681	Equipment ID	BKK_FS0800
Calibrator Manufacturer	Teledyne API	Model	700
Serial No.	947		
Std. Gas Concentration (PPM)	55.88	Cylinder No.	GN0027222
Cylinder Pressure (psi)	1800	Certified By	Airgas Inc.
Certified Date	9-Feb-22	Expired Date	9-Feb-30

Point	CALIBRATION RESULTS						
	Ideal	Actual NO	Error NO	%Error NO	Actual NOx	Error NOx	%Error NOx
ZERO	0.00	0.10	0.10	0.10	0.10	0.10	0.10
1	100.00	99.10	-0.90	-0.90	100.50	0.50	0.50
2	200.00	198.80	-1.20	-0.60	201.30	1.30	0.65
3	300.00	298.00	-2.00	-0.67	301.30	1.30	0.43
4	400.00	398.70	-1.30	-0.33	401.30	1.30	0.33
AVERAGE (%)				-0.48			0.40

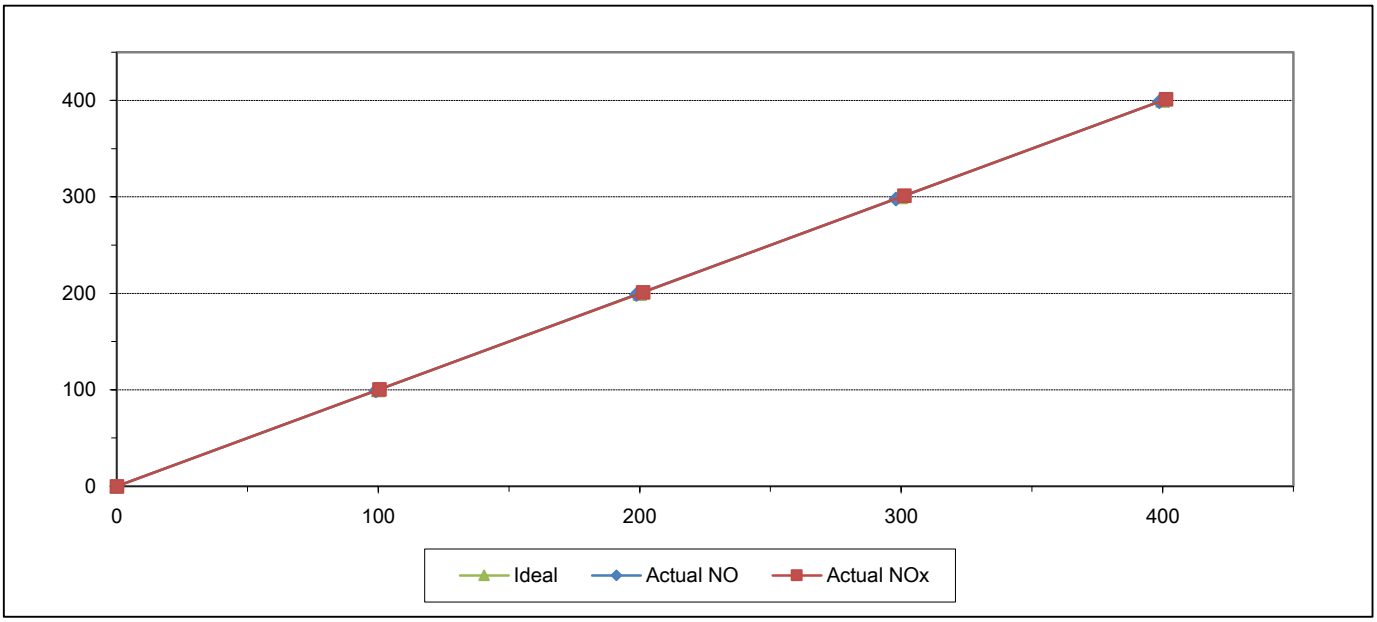

Calibrated By

(Mr.Jirawut Sakarn)
Field Environmental Scientist (3)


Approved By

(Mr.Sarayuth Jittranont)
Assistant General Manager

MULTIPOINT CALIBRATION REPORT

Calibration Date	5-Jan-26	Equipment Name	NOx Analyzer
Manufacturer	HORIBA	Model	APNA-370
Serial No.	TLTATGDW	Equipment ID	BKK_FS0785
Calibrator Manufacturer	Teledyne API	Model	700
Serial No.	947		
Std. Gas Concentration (PPM)	55.88	Cylinder No.	GN0027222
Cylinder Pressure (psi)	1800	Certified By	Airgas Inc.
Certified Date	9-Feb-22	Expired Date	9-Feb-30

Point	CALIBRATION RESULTS						
	Ideal	Actual NO	Error NO	%Error NO	Actual NOx	Error NOx	%Error NOx
ZERO	0.00	0.10	0.10	0.10	0.10	0.10	0.10
1	100.00	99.00	-1.00	-1.00	100.30	0.30	0.30
2	200.00	199.30	-0.70	-0.35	200.50	0.50	0.25
3	300.00	299.00	-1.00	-0.33	301.10	1.10	0.37
4	400.00	398.70	-1.30	-0.33	399.30	-0.70	-0.17
AVERAGE (%)				-0.38			0.17

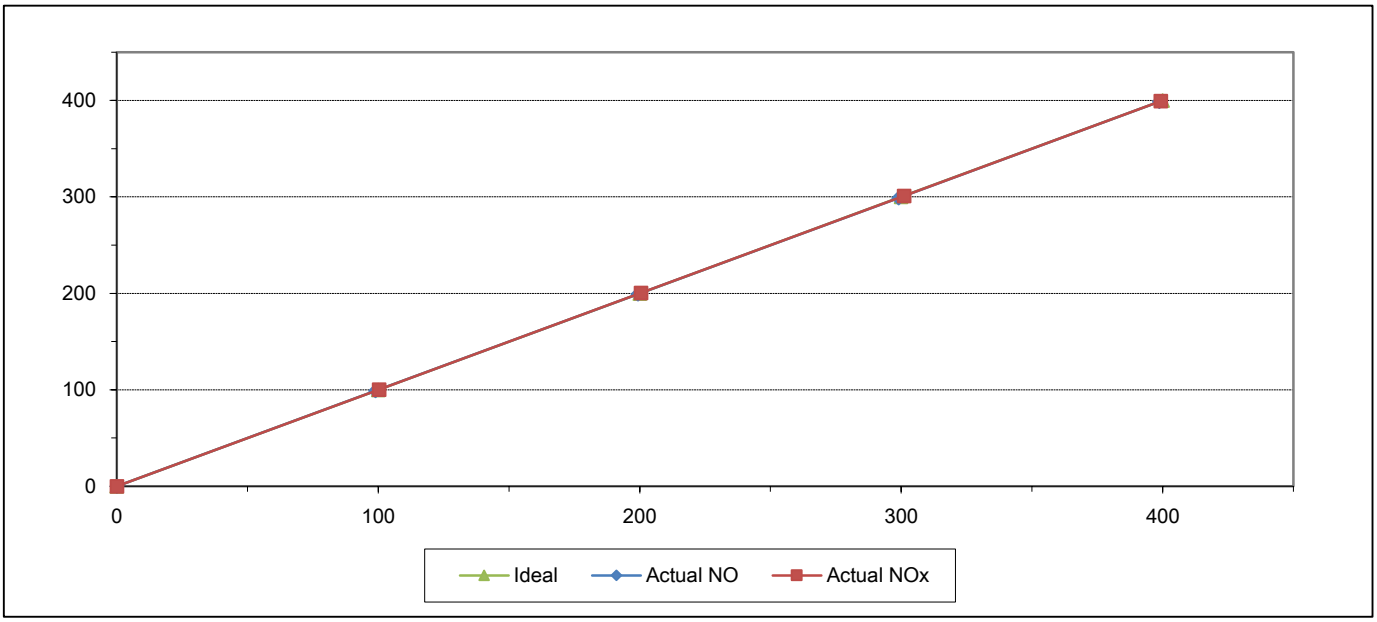

Calibrated By

(Mr.Jirawut Sakarn)
Field Environmental Scientist (3)


Approved By

(Mr.Sarayuth Jittranont)
Assistant General Manager

MULTIPOINT CALIBRATION REPORT

Calibration Date	5-Jan-26	Equipment Name	NOx Analyzer
Manufacturer	HORIBA	Model	APNA-370
Serial No.	XLTWRBSJ	Equipment ID	BKK_FS1092
Calibrator Manufacturer	Teledyne API	Model	700
Serial No.	947		
Std. Gas Concentration (PPM)	55.88	Cylinder No.	GN0027222
Cylinder Pressure (psi)	1800	Certified By	Airgas Inc.
Certified Date	9-Feb-22	Expired Date	9-Feb-30

Point	CALIBRATION RESULTS						
	Ideal	Actual NO	Error NO	%Error NO	Actual NOx	Error NOx	%Error NOx
ZERO	0.00	0.10	0.10	0.10	0.10	0.10	0.10
1	100.00	99.70	-0.30	-0.30	101.00	1.00	1.00
2	200.00	198.00	-2.00	-1.00	201.20	1.20	0.60
3	300.00	299.20	-0.80	-0.27	301.10	1.10	0.37
4	400.00	398.20	-1.80	-0.45	401.30	1.30	0.33
AVERAGE (%)				-0.38			0.48

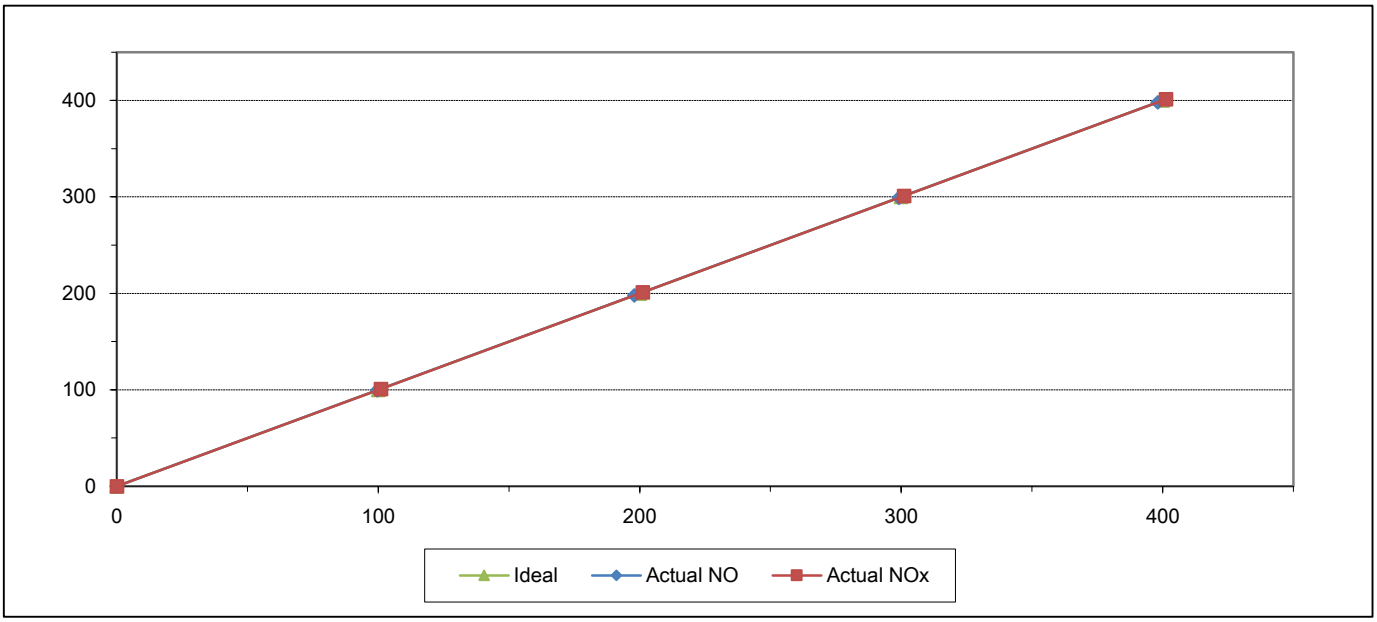

Calibrated By

(Mr.Jirawut Sakarn)
Field Environmental Scientist (3)


Approved By

(Mr.Sarayuth Jittranont)
Assistant General Manager

MULTIPOINT CALIBRATION REPORT

Calibration Date	5-Jan-26	Equipment Name	NOx Analyzer
Manufacturer	HORIBA	Model	APNA-370
Serial No.	V9L01NF0	Equipment ID	BKK_FS1457
Calibrator Manufacturer	Teledyne API	Model	700
Serial No.	947		
Std. Gas Concentration (PPM)	55.88	Cylinder No.	GN0027222
Cylinder Pressure (psi)	1800	Certified By	Airgas Inc.
Certified Date	9-Feb-22	Expired Date	9-Feb-30

Point	CALIBRATION RESULTS						
	Ideal	Actual NO	Error NO	%Error NO	Actual NOx	Error NOx	%Error NOx
ZERO	0.00	0.10	0.10	0.10	0.10	0.10	0.10
1	100.00	99.60	-0.40	-0.40	101.10	1.10	1.10
2	200.00	198.70	-1.30	-0.65	201.20	1.20	0.60
3	300.00	299.00	-1.00	-0.33	301.30	1.30	0.43
4	400.00	398.80	-1.20	-0.30	401.50	1.50	0.38
AVERAGE (%)				-0.32			0.52

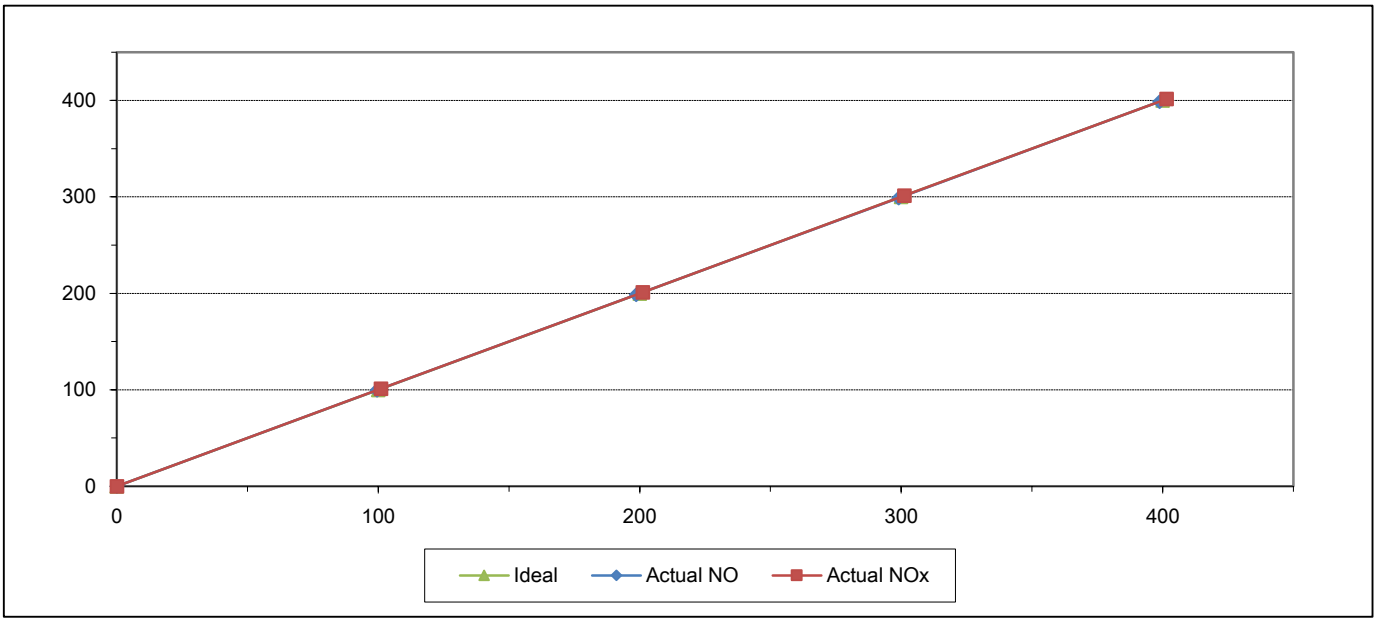

Calibrated By

(Mr.Jirawut Sakarn)
Field Environmental Scientist (3)


Approved By

(Mr.Sarayuth Jittranont)
Assistant General Manager

MULTIPOINT CALIBRATION REPORT

Calibration Date	5-Jan-26	Equipment Name	SO2 Analyzer
Manufacturer	HORIBA	Model	APSA-370
Serial No.	YU9BY9F9	Equipment ID	BKK_FS0799
Calibrator Manufacturer	Teledyne API	Model	700
Serial No.	947		
Std. Gas Concentration (PPM)	56.3	Cylinder No.	GN0027222
Cylinder Pressure (psi)	1800	Certified By	Airgas Inc.
Certified Date	9-Feb-22	Expired Date	9-Feb-30

Point	CALIBRATION RESULTS			
	Ideal	Autual	Error	%Error
ZERO	0.00	0.10	0.10	0.10
1	100.00	101.10	1.10	1.10
2	200.00	199.10	-0.90	-0.45
3	300.00	298.50	-1.50	-0.50
4	400.00	398.80	-1.20	-0.30
AVERAGE (%)				-0.01

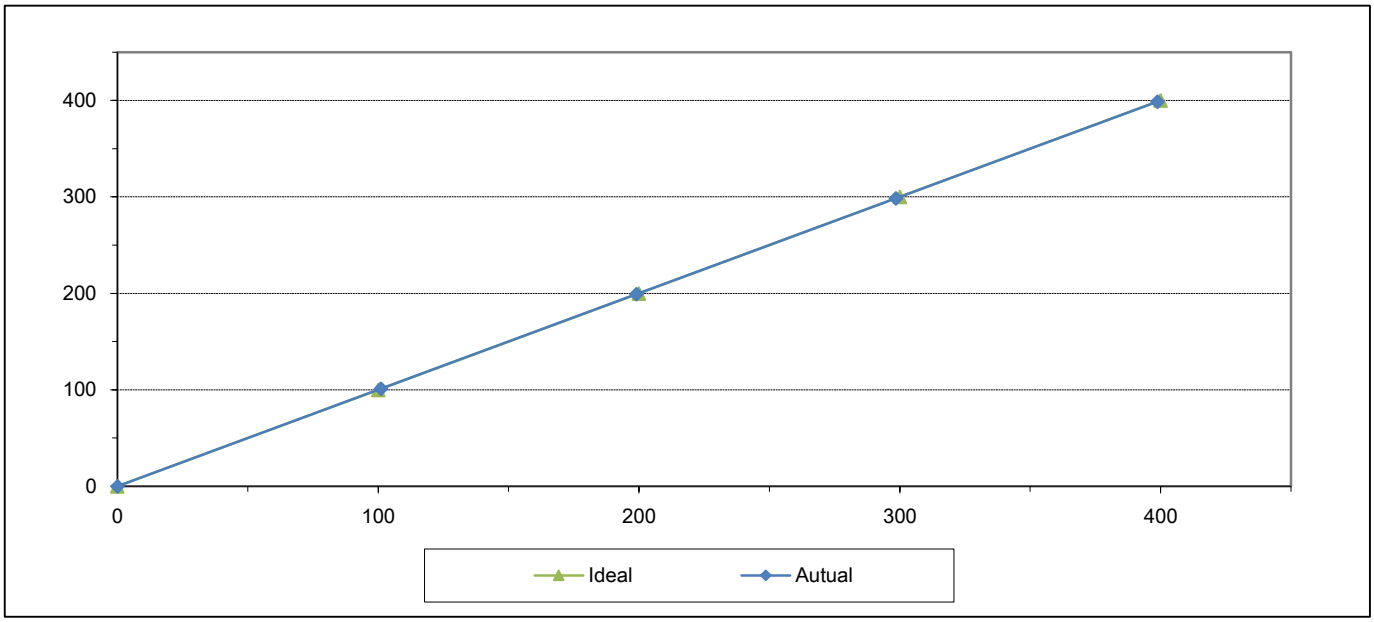

Calibrated By

(Mr.Jirawut Sakarn)
Field Environmental Scientist (3)


Approved By

(Mr.Sarayuth Jittranont)
Assistant General Manager

MULTIPOINT CALIBRATION REPORT

Calibration Date	5-Jan-26	Equipment Name	SO2 Analyzer
Manufacturer	HORIBA	Model	APSA-370
Serial No.	3C72K8HB	Equipment ID	BKK_FS0784
Calibrator Manufacturer	Teledyne API	Model	700
Serial No.	947		
Std. Gas Concentration (PPM)	56.3	Cylinder No.	GN0027222
Cylinder Pressure (psi)	1800	Certified By	Airgas Inc.
Certified Date	9-Feb-22	Expired Date	9-Feb-30

Point	CALIBRATION RESULTS			
	Ideal	Autual	Error	%Error
ZERO	0.00	0.10	0.10	0.10
1	100.00	99.60	-0.40	-0.40
2	200.00	198.60	-1.40	-0.70
3	300.00	298.70	-1.30	-0.43
4	400.00	401.10	1.10	0.28
AVERAGE (%)				-0.23

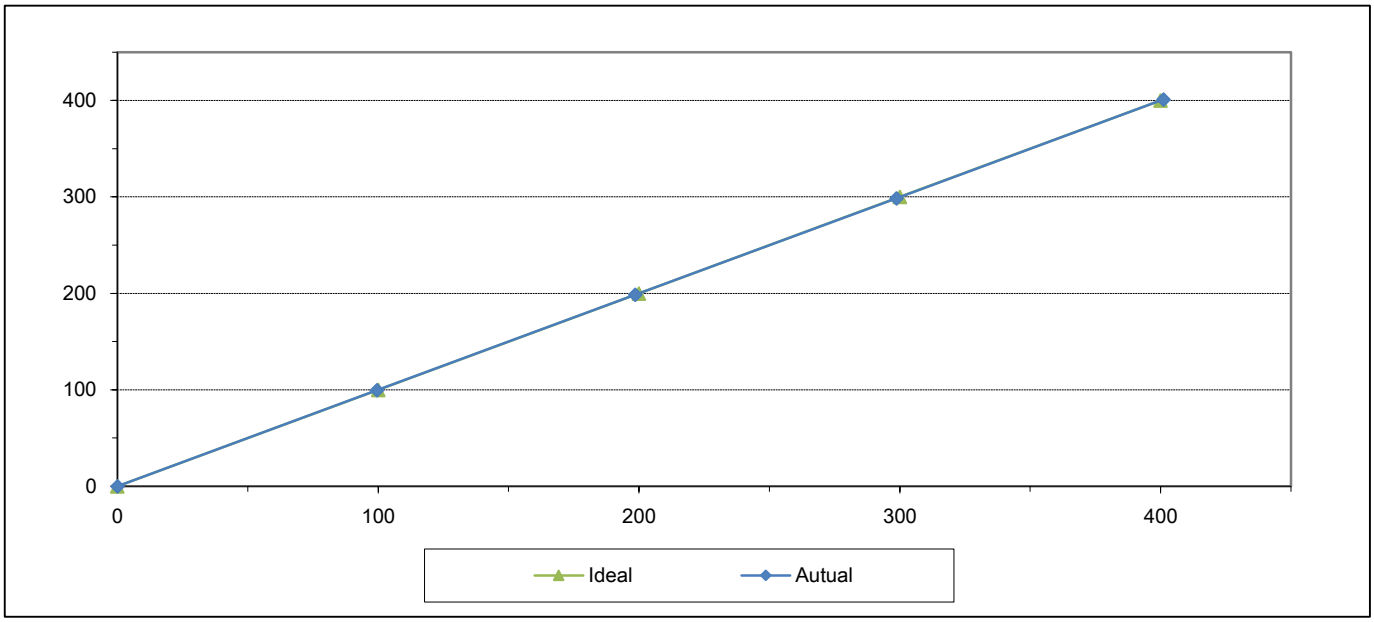

Calibrated By

(Mr.Jirawut Sakarn)
Field Environmental Scientist (3)


Approved By

(Mr.Sarayuth Jittranont)
Assistant General Manager

MULTIPOINT CALIBRATION REPORT

Calibration Date	5-Jan-26	Equipment Name	SO2 Analyzer
Manufacturer	HORIBA	Model	APSA-370
Serial No.	6BVW9P1K	Equipment ID	BKK_FS1091
Calibrator Manufacturer	Teledyne API	Model	700
Serial No.	947		
Std. Gas Concentration (PPM)	56.3	Cylinder No.	GN0027222
Cylinder Pressure (psi)	1800	Certified By	Airgas Inc.
Certified Date	9-Feb-22	Expired Date	9-Feb-30

Point	CALIBRATION RESULTS			
	Ideal	Autual	Error	%Error
ZERO	0.00	0.00	0.00	0.00
1	100.00	98.50	-1.50	-1.50
2	200.00	198.80	-1.20	-0.60
3	300.00	298.70	-1.30	-0.43
4	400.00	398.90	-1.10	-0.28
AVERAGE (%)				-0.56

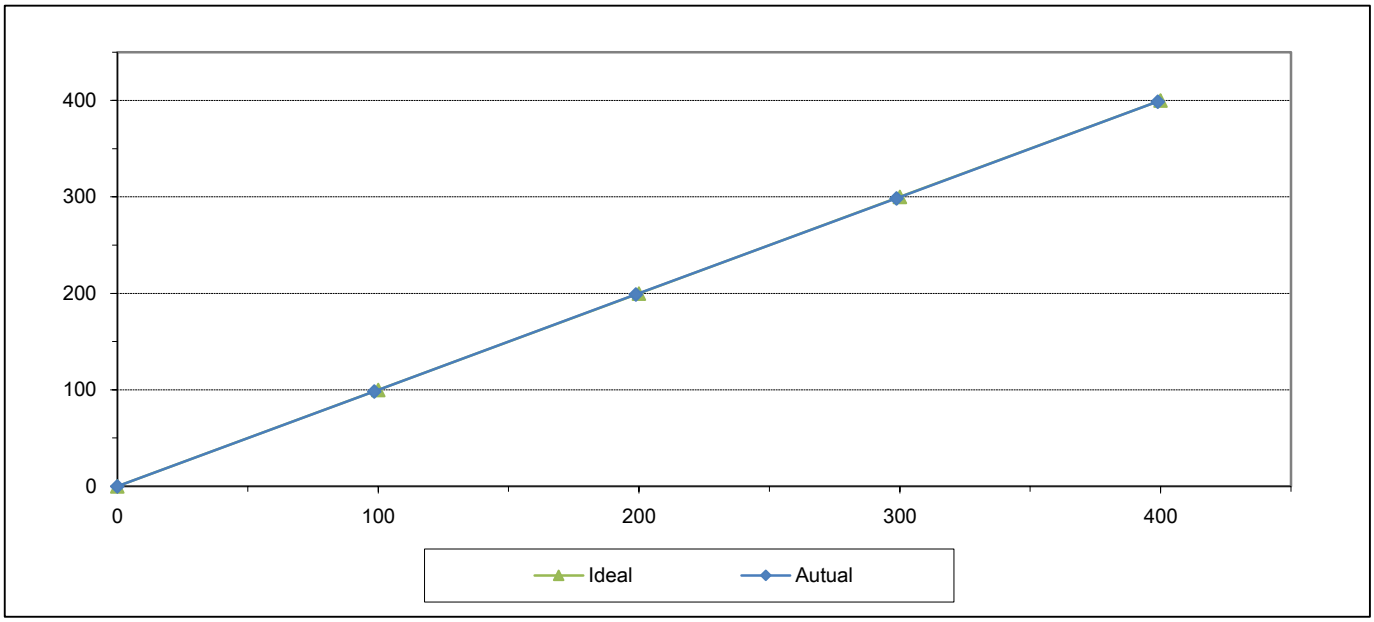

Calibrated By

(Mr.Jirawut Sakarn)
Field Environmental Scientist (3)


Approved By

(Mr.Sarayuth Jittranont)
Assistant General Manager

MULTIPOINT CALIBRATION REPORT

Calibration Date	5-Jan-26	Equipment Name	SO2 Analyzer
Manufacturer	HORIBA	Model	APSA-370
Serial No.	LRB7V6X	Equipment ID	BKK_FS1456
Calibrator Manufacturer	Teledyne API	Model	700
Serial No.	947		
Std. Gas Concentration (PPM)	56.3	Cylinder No.	GN0027222
Cylinder Pressure (psi)	1800	Certified By	Airgas Inc.
Certified Date	9-Feb-22	Expired Date	9-Feb-30

Point	CALIBRATION RESULTS			
	Ideal	Autual	Error	%Error
ZERO	0.00	0.10	0.10	0.10
1	100.00	98.60	-1.40	-1.40
2	200.00	198.80	-1.20	-0.60
3	300.00	298.90	-1.10	-0.37
4	400.00	399.50	-0.50	-0.13
AVERAGE (%)				-0.48

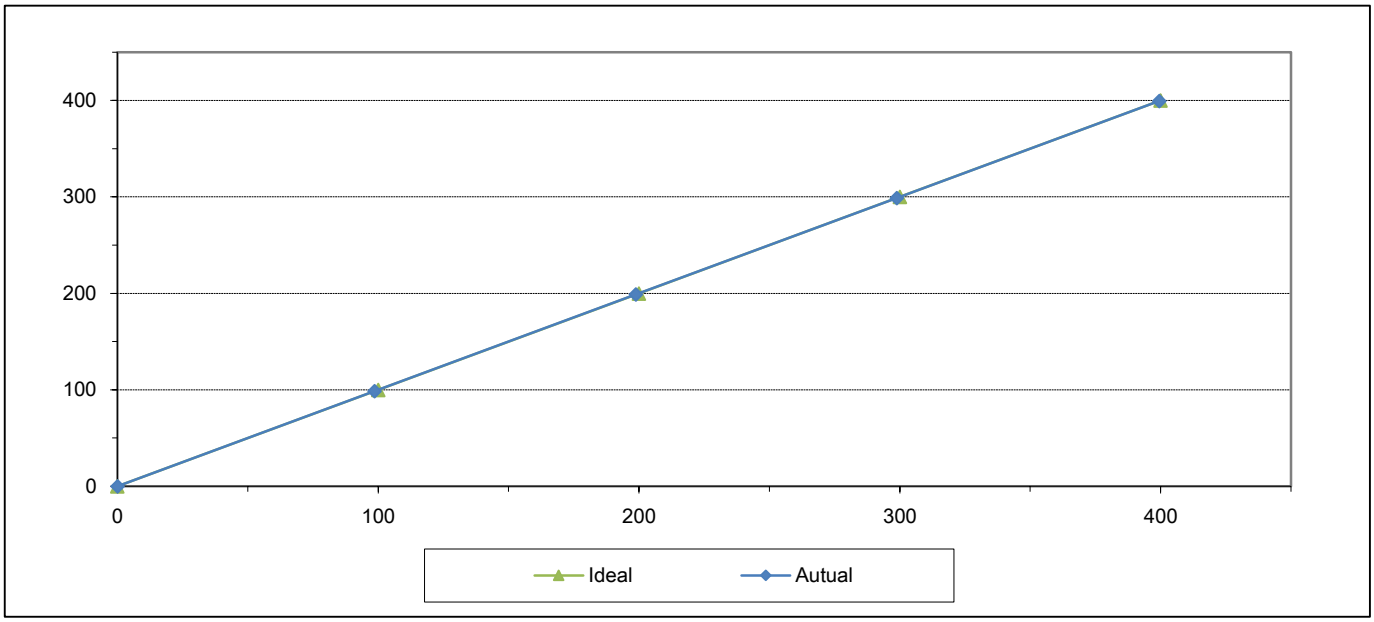

Calibrated By

(Mr.Jirawut Sakarn)
Field Environmental Scientist (3)


Approved By

(Mr.Sarayuth Jittranont)
Assistant General Manager

High Volume Air Sampler Calibration Worksheet

Project Site :	Hin Kong Power Company Limited	**Barometric Pressure (mm Hg) :**	758.4
Calibrate Location :	บริเวณวัดหินกอง	**Temperature (°C) :**	33.0
Calibrate Date :	16-Mar-26	**High Volume ID :**	BKK_FS1486
CalibrationSheet No.:	**C-160326-BKK_FS1486**	**High Volume Model :**	TE-5009X
Calibrator ID:	BKK_FS0624	**High Volume S/N :**	6431
Calibrator Model :	TE-5028A	**Calibrator Slope :**	1.03094
Calibrator S/N :	2584	**Calibrator Intercept :**	-0.01512

Test No.	Delta H_2O (inch)	Qa (m^3/min)	I : Chart (CFM)	Linear Regression
1	2.2	0.929	30	Slope : 53.4285
2	2.8	1.046	36	Intercept : -19.6702
3	3.2	1.117	40	Correlation Coefficient : 0.9995
4	3.6	1.184	44	
5	4.4	1.308	50	

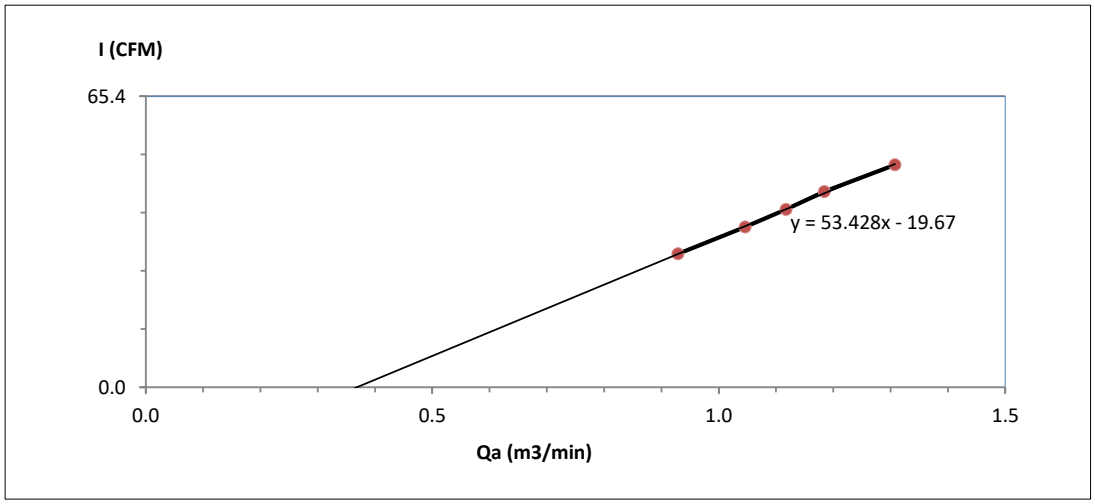

Calibrated by Autit Aoonsim

(Mr. Autit Aoonsim)
BKK Field Services Scientist (2)


Approved by : Warakorn P.

(Mr. Warakorn Pookrak)
Field Services Supervisor

High Volume Air Sampler Calibration Worksheet

Project Site :	Hin Kong Power Company Limited	**Barometric Pressure (mm Hg) :**	758.4
Calibrate Location :	บริเวณวัดห้วยไผ่	**Temperature (°C) :**	33.0
Calibrate Date :	16-Mar-26	**High Volume ID :**	BKK_FS1487
CalibrationSheet No.:	**C-160326-BKK_FS1487**	**High Volume Model :**	TE-5009X
Calibrator ID:	BKK_FS0624	**High Volume S/N :**	6432
Calibrator Model :	TE-5028A	**Calibrator Slope :**	1.03094
Calibrator S/N :	2584	**Calibrator Intercept :**	-0.01512

Test No.	Delta H_2O (inch)	Qa (m^3/min)	I : Chart (CFM)	Linear Regression
1	2.1	0.908	30	Slope : 50.8515
2	2.8	1.046	36	Intercept : -16.5785
3	3.2	1.117	40	Correlation Coefficient : 0.9984
4	3.6	1.184	44	
5	4.4	1.308	50	

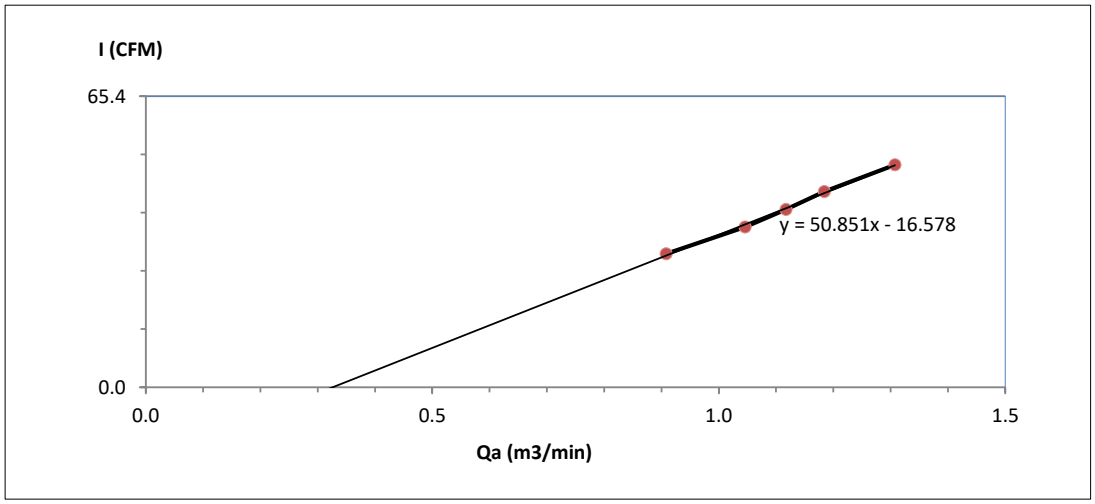

Calibrated by Autit Aoonsim

(Mr. Autit Aoonsim)
BKK Field Services Scientist (2)


Approved by : Warakorn P.

(Mr. Warakorn Pookrak)
Field Services Supervisor

High Volume Air Sampler Calibration Worksheet

Project Site :	Hin Kong Power Company Limited	**Barometric Pressure (mm Hg) :**	758.4
Calibrate Location :	บริเวณโรงเรียนวัดห้วยปลาดุก(โรงเรียน อบจ. ราชบุรี) (วัดห้วยปลาดุก อนันตกูล	**Temperature (°C) :**	33.0
Calibrate Date :	16-Mar-26	**High Volume ID :**	BKK_FS1061
CalibrationSheet No.:	**C-160326-BKK_FS1061**	**High Volume Model :**	TE-5009X
Calibrator ID:	BKK_FS0624	**High Volume S/N :**	5504
Calibrator Model :	TE-5028A	**Calibrator Slope :**	1.03094
Calibrator S/N :	2584	**Calibrator Intercept :**	-0.01512

Test No.	Delta H_2O (inch)	Qa (m^3/min)	I : Chart (CFM)	Linear Regression
1	2.0	0.886	30	Slope : 41.2237
2	2.6	1.009	36	Intercept : -6.1177
3	3.2	1.117	40	Correlation Coefficient : 0.9989
4	3.8	1.216	44	
5	4.8	1.365	50	

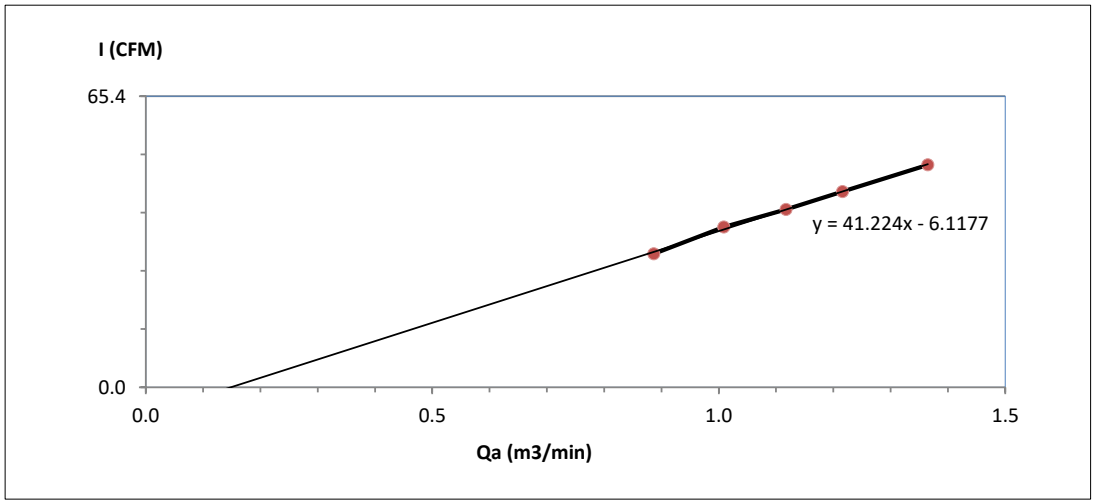

Calibrated by Autit Aoonsim

(Mr. Autit Aoonsim)
BKK Field Services Scientist (2)


Approved by : Warakorn P.

(Mr. Warakorn Pookrak)
Field Services Supervisor

High Volume Air Sampler Calibration Worksheet

Project Site :	Hin Kong Power Company Limited	**Barometric Pressure (mm Hg) :**	758.4
Calibrate Location :	บริเวณ รพ.สต.เจดีย์หัก(บ้านห้วยหมู)	**Temperature (°C) :**	33.0
Calibrate Date :	16-Mar-26	**High Volume ID :**	BKK_FS1377
CalibrationSheet No.:	**C-160326-BKK_FS1377**	**High Volume Model :**	TE-5009X
Calibrator ID:	BKK_FS0624	**High Volume S/N :**	6262
Calibrator Model :	TE-5028A	**Calibrator Slope :**	1.03094
Calibrator S/N :	2584	**Calibrator Intercept :**	-0.01512

Test No.	Delta H_2O (inch)	Qa (m^3/min)	I : Chart (CFM)	Linear Regression
1	2.0	0.886	30	Slope : 43.3908
2	2.6	1.009	36	Intercept : -8.2955
3	3.2	1.117	40	Correlation Coefficient : 0.9986
4	3.8	1.216	44	
5	4.6	1.337	50	

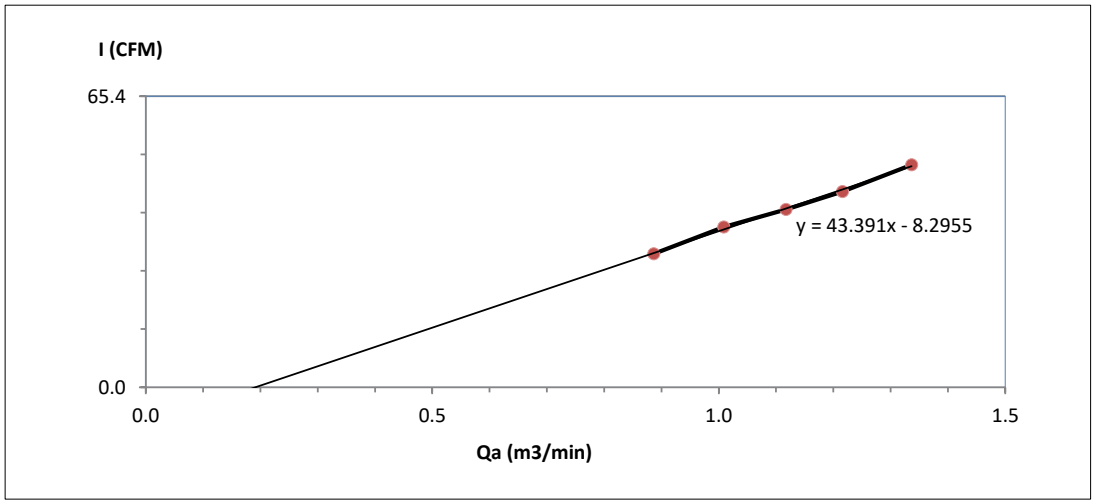

Calibrated by Autit Aoonsim

(Mr. Autit Aoonsim)
BKK Field Services Scientist (2)

Approved by : Warakorn P.

(Mr. Warakorn Pookrak)
Field Services Supervisor

Accredited by

NSC-TISI-TIS 17025
Calibration 0426

Calibration certificate

Calibration Certificate No. 25BCI0197

Object	Electronic non-automatic weighing instrument
Manufacturer	Ohaus
Type	EX225D/AD
Serial | QM Ident. no.	C309774648 | BKK_EN0403
Customer	ALS Laboratory Group (Thailand)Co., Ltd.
	104 Phatthanakarn 40,Phattanakarn Rd.,Khwaeng Phatthanakarn ,Khet Suan Luang,Bangkok 10250
Order no.	261969
Number of pages	6
Date of calibration	30 May 2025

This calibration certificate documents the traceability to national standards.

Uncertainties of measurements are taken into account when only statements of compliance are made.

This certificate was prepared by Sartorius Corporation in accordance to the current ISO/IEC 17025:2017 standard and Sartorius Work Instruction (Method) SOP WI 08.

This certificate relate and apply this equipment only.

REVIEW BY ..... Linda K .....

APPROVED BY ..... Siriluk P .....

NEXT CAL DATE ..... 30/05/26 .....

This calibration certificate may not be reproduced other than in full except with the permission of NSC-TISI-TIS-17025 and the issuing laboratory. Calibration certificates without signature are not valid.

The user is obliged to have the object recalibrated at appropriate intervals.

Date	Approval of the Calibration Certificate	Person in charge
30 May 2025	Mr. Chonchai Inthana	Chonchai Inthana

Calibration object

Multi range instrument

Model	EX225D/AD	
Serial Number	C309774648	
QM Ident. no | Inventory no.	BKK_EN0403 | ---	
Range	1	2
Maximum capacity (Max. load)	120.00000 g	220.0000 g
Measured range	120.00000 g	220.0000 g
Scale interval	0.00001 g	0.0001 g

Place of calibration

Address	According to page 1
Department | Cost center	Environment Department. | ---
Building | Floor	--- | 1st Floor.
Room	Laboratory Room.
Maximum temperature variation at place of calibration	5 K

Calibration procedure

EURAMET cg-18, V4.0 - Guidelines on the Calibration of Non-Automatic Weighing Instruments

Test equipment

Test equipment type	Test equipment ID	Valid until
Thermometer	Testo 174(Traceable to Si unit through ENTECH)	11 Nov 2025
Test weight set OIML R111 E2	Certificate No.M2308197S ,E2(Traceable to SI unit through TCS)	23 Aug 2025

Range 1

Adjustment Status

The measuring device was internally adjusted before the calibration.

Environmental and measuring conditions

Date of calibration	30 May 2025
Temperature at place of calibration | Temp. diff. $T_{weights}$ - T_{place}	21.7 °C | 0.5 K
Measuring conditions	The installation site is suitable. The device was levelled. Balance was loaded up to Max before test.
Comments	Humidity 60.0 %RH.

Measurement results | Measurement uncertainties

Repeatability

Test load (nominal): 1 g | 100 g		
	1 g	**100 g**
1	0.99993 g	99.99971 g
2	0.99991 g	99.99971 g
3	0.99992 g	99.99974 g
4	0.99993 g	99.99973 g
5	0.99992 g	99.99974 g
6	0.99991 g	99.99970 g
7	0.99993 g	99.99973 g
8	0.99994 g	99.99972 g
9	0.99995 g	99.99971 g
10	0.99995 g	99.99969 g
	s = 0.000014 g	s = 0.000017 g

Eccentricity

Test load (nominal):	**50 g**
Center	49.99996 g
Front left	49.99993 g
Back left	49.99993 g
Back right	49.99994 g
Front right	49.99990 g
Maximum deviation from centric loading indication $\lvert\Delta I_{ecc}\rvert_{max}$ = 0.00006 g	

Error of indication

Testload ***L***	**Indication** ***I***	**Error** ***E***	**Expansion factor** ***k***	**Uncertainty** ***U(E)***	**Uncertainty relative** $U_{rel}(E)$
0.00000 g	0.00000 g	0.00000 g	2.00	0.000030 g	---
0.01000 g	0.00995 g	-0.00005 g	2.00	0.000037 g	0.37 %
0.10000 g	0.09991 g	-0.00009 g	2.00	0.000038 g	0.038 %
0.50000 g	0.49985 g	-0.00015 g	2.00	0.000040 g	0.0080 %
1.00000 g	0.99991 g	-0.00009 g	2.00	0.000041 g	0.0041 %
5.00002 g	4.99997 g	-0.00005 g	2.00	0.000050 g	0.0010 %
10.00002 g	10.00003 g	0.00001 g	2.00	0.000069 g	0.00069 %
50.00002 g	49.99972 g	-0.00030 g	2.00	0.000091 g	0.00018 %
70.00004 g	69.99975 g	-0.00029 g	2.00	0.00017 g	0.00024 %
100.00001 g	99.99958 g	-0.00043 g	2.00	0.00017 g	0.00017 %
115.00006 g	114.99966 g	-0.00040 g	2.00	0.00028 g	0.00024 %
Maximum error of indication		$\lvert E\rvert_{max}$ = 0.00043 g			

$U_{rel}(E)$ is the quotient of $U(E)$ and test load L. The uncertainty of measurement $U(E)$ is valid only if error E is considered. You will find reference notes on the uncertainty of measurement in use under: Appendix to the calibration certificate | Interpretation of measurement results.
Reference note: The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the documented Expansion factor, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

Range 2

Adjustment Status

The measuring device was internally adjusted before the calibration.

Environmental and measuring conditions

Date of calibration	30 May 2025
Temperature at place of calibration | Temp. diff. $T_{weights}$ - T_{place}	21.7 °C | 0.5 K
Measuring conditions	The installation site is suitable. The device was levelled. Balance was loaded up to Max before test.
Comments	Humidity 60.0 %RH.

Measurement results | Measurement uncertainties

Repeatability

Test load (nominal): 200 g	
	200 g
1	199.9998 g
2	199.9998 g
3	199.9998 g
4	200.0000 g
5	199.9998 g
6	199.9999 g
7	199.9999 g
8	200.0000 g
9	199.9998 g
10	199.9999 g
	s = 0.00008 g

Eccentricity

Test load (nominal):	**100 g**
Center	99.99984 g
Front left	99.99990 g
Back left	99.99983 g
Back right	99.99979 g
Front right	99.99979 g
Maximum deviation from centric loading indication $\lvert\Delta I_{ecc}\rvert_{max}$ = 0.00006 g	

Error of indication

Testload ***L***	**Indication** ***I***	**Error** ***E***	**Expansion factor** ***k***	**Uncertainty** ***U(E)***	**Uncertainty relative** $U_{rel}(E)$
0.00000 g	0.00000 g	0.00000 g	2.00	0.000030 g	---
20.00002 g	19.99986 g	-0.00016 g	2.00	0.000069 g	0.00034 %
50.00002 g	49.99978 g	-0.00024 g	2.00	0.000091 g	0.00018 %
70.00004 g	69.99981 g	-0.00023 g	2.00	0.00017 g	0.00024 %
90.00007 g	89.99976 g	-0.00031 g	2.00	0.00018 g	0.00020 %
110.00003 g	109.99986 g	-0.00017 g	2.00	0.00028 g	0.00025 %
130.0001 g	129.9999 g	-0.0002 g	2.00	0.00028 g	0.00022 %
150.0000 g	149.9999 g	-0.0001 g	2.00	0.00028 g	0.00019 %
170.0000 g	170.0000 g	0.0000 g	2.00	0.00028 g	0.00016 %
200.0000 g	199.9998 g	-0.0002 g	2.00	0.00028 g	0.00014 %
220.0000 g	219.9999 g	-0.0001 g	2.00	0.00029 g	0.00013 %
Maximum error of indication		$\lvert E\rvert_{max}$ = 0.0003 g			

$U_{rel}(E)$ is the quotient of $U(E)$ and test load L. The uncertainty of measurement $U(E)$ is valid only if error E is considered. You will find reference notes on the uncertainty of measurement in use under: Appendix to the calibration certificate | Interpretation of measurement results.
Reference note: The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the documented Expansion factor, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

End of calibration certificate

Uncertainty of measurement in use


Range 1

Device adjusted before measurement	Yes
Temperature deviation considered	5 K
Temperature coefficient considered	$2 \cdot 10^{-6}$/K
Uncertainty of the weighing result $U_{gl}(W)$	**$U_{gl}(W) = 0.000035\ g + 1.38 \cdot 10^{-5} \cdot R$**

Reference note: The current uncertainty of measurement is calculated by entering of the reading *R* into this formula. In relation to this, there is no need for a correction of the indication error. The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied with an Expansion factor of 2, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

Indication in % from max load	Net indication *R*	Uncertainty $U_{gl}(W)$	Uncertainty relative $U_{gl}(W)_{rel}$
1 %	1.20000 g	0.000052 g	0.0043 %
25 %	30.00000 g	0.00045 g	0.0015 %
50 %	60.00000 g	0.00086 g	0.0014 %
75 %	90.00000 g	0.0013 g	0.0014 %
100 %	120.00000 g	0.0017 g	0.0014 %

Graphic realization of the relative uncertainty of measurement | process accuracy

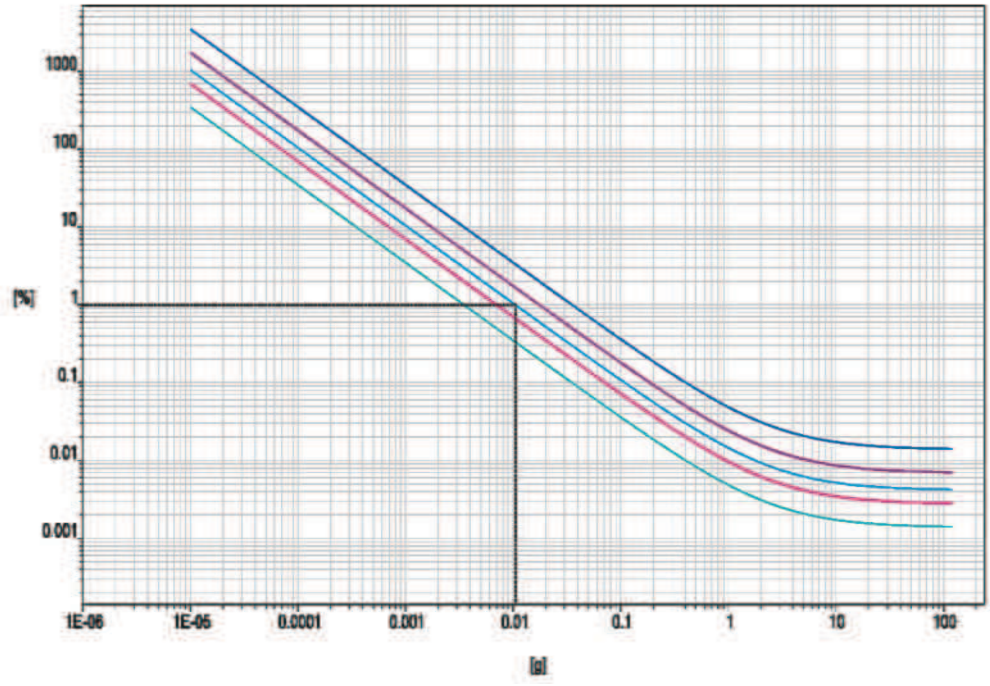

Safety factor	
10	
5	
3	
2	
1	

Displayed example

Process accuracy	1.00 %
Safety factor	3
Minimum sample weight	0.01045 g

Uncertainty of measurement in use


Range 2

Device adjusted before measurement	Yes
Temperature deviation considered	5 K
Temperature coefficient considered	$2 \cdot 10^{-6}$/K
Uncertainty of the weighing result $U_{gl}(W)$	**$U_{gl}(W) = 0.000067\ g + 9.52 \cdot 10^{-6} \cdot R$**

Reference note: The current uncertainty of measurement is calculated by entering of the reading *R* into this formula. In relation to this, there is no need for a correction of the indication error. The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied with an Expansion factor of 2, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

Indication in % from max load	Net indication *R*	Uncertainty $U_{gl}(W)$	Uncertainty relative $U_{gl}(W)_{rel}$
1 %	2.20000 g	0.000088 g	0.0040 %
25 %	55.00000 g	0.00059 g	0.0011 %
50 %	110.00000 g	0.0011 g	0.0010 %
75 %	165.0000 g	0.0016 g	0.00099 %
100 %	220.0000 g	0.0022 g	0.00098 %

Graphic realization of the relative uncertainty of measurement | process accuracy

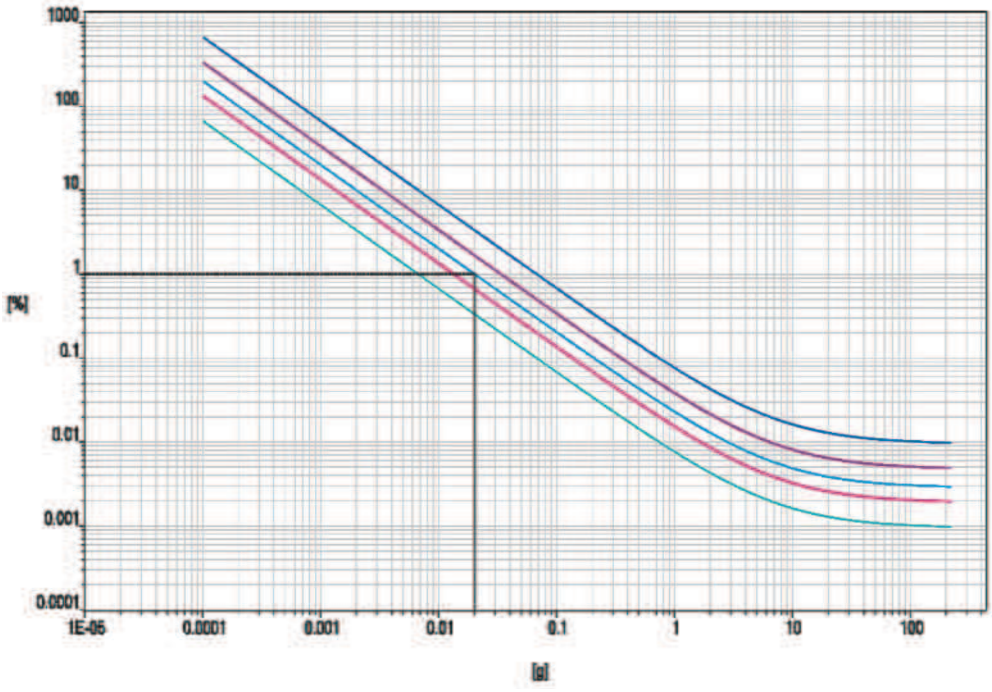

Safety factor
10
5
3
2
1


Displayed example

Process accuracy	1.00 %
Safety factor	3
Minimum sample weight	0.02019 g

High Volume Air Sampler Calibration Worksheet

Project Site :	Hin Kong Power Company Limited	**Barometric Pressure (mm Hg) :**	758.4
Calibrate Location :	บริเวณวัดหินกอง	**Temperature (°C) :**	33.0
Calibrate Date :	16-Mar-26	**High Volume ID :**	BKK_FS1484
CalibrationSheet No.:	**C-160326-BKK_FS1484**	**High Volume Model :**	TE-5009X
Calibrator ID:	BKK_FS0624	**High Volume S/N :**	6429
Calibrator Model :	TE-5028A	**Calibrator Slope :**	1.64598
Calibrator S/N :	2584	**Calibrator Intercept :**	-0.02439

Test No.	Delta H_2O (inch)	Q_{std} (m^3/min)	I : Chart (CFM)	Linear Regression
1	3.4	1.1287	40	Slope : 38.7005
2	4.2	1.2518	44	Intercept : -4.1313
3	5.3	1.4032	50	Correlation Coefficient : 0.9982
4	6.2	1.5157	54	
5	7.3	1.6426	60	

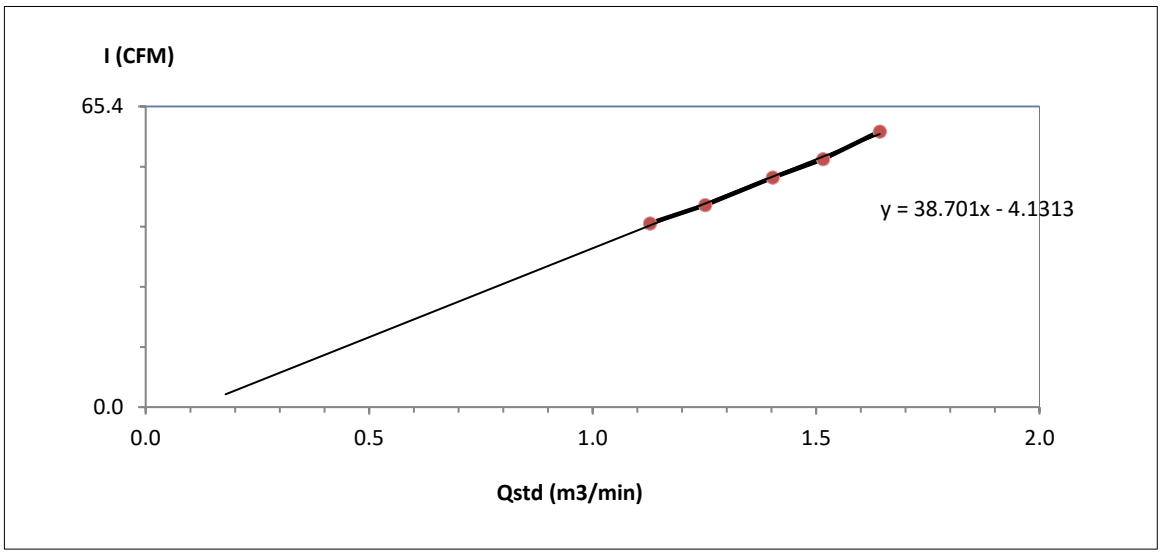

Calibrated by Autit Aoonsim

(Mr. Autit Aoonsim)
BKK Field Services Scientist (2)


Approved by : Warakorn P.

(Mr. Warakorn Pookrak)
Field Services Supervisor

High Volume Air Sampler Calibration Worksheet

Project Site :	Hin Kong Power Company Limited	**Barometric Pressure (mm Hg) :**	758.4
Calibrate Location :	บริเวณวัดห้วยไผ่	**Temperature (°C) :**	33.0
Calibrate Date :	16-Mar-26	**High Volume ID :**	BKK_FS1485
CalibrationSheet No.:	**C-160326-BKK_FS1485**	**High Volume Model :**	TE-5009X
Calibrator ID:	BKK_FS0624	**High Volume S/N :**	6430
Calibrator Model :	TE-5028A	**Calibrator Slope :**	1.64598
Calibrator S/N :	2584	**Calibrator Intercept :**	-0.02439

Test No.	Delta H_2O (inch)	Q_{std} (m^3/min)	I : Chart (CFM)	Linear Regression
1	3.4	1.1287	40	Slope : 36.8664
2	4.2	1.2518	44	Intercept : -1.8275
3	5.3	1.4032	50	Correlation Coefficient : 0.9997
4	6.2	1.5157	54	
5	7.6	1.6755	60	

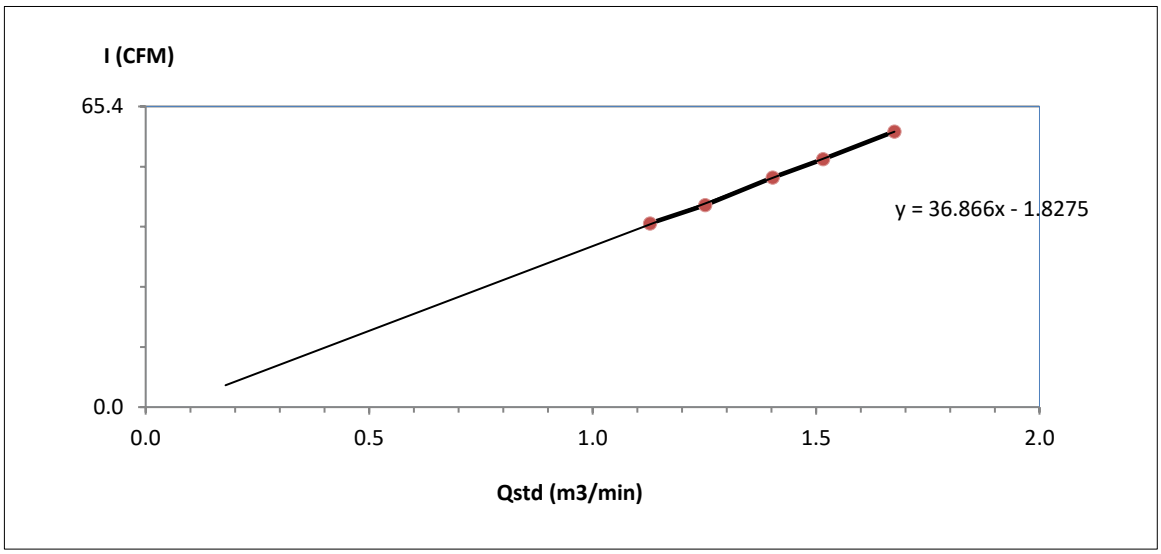

Calibrated by Autit Aoonsim

(Mr. Autit Aoonsim)
BKK Field Services Scientist (2)


Approved by : Warakorn P.

(Mr. Warakorn Pookrak)
Field Services Supervisor

High Volume Air Sampler Calibration Worksheet

Project Site :	Hin Kong Power Company Limited	**Barometric Pressure (mm Hg) :**	758.4
Calibrate Location :	บริเวณโรงเรียนวัดห้วยปลาดุก (โรงเรียน อบจ. ราชบุรี) (วัดห้วยปลาดุก อนันตกูลอุปถัมภ์)	**Temperature (°C) :**	33.0
Calibrate Date :	16-Mar-26	**High Volume ID :**	BKK_FS0364
CalibrationSheet No.:	**C-160326-BKK_FS0364**	**High Volume Model :**	TE-5009X
Calibrator ID:	BKK_FS0624	**High Volume S/N :**	4154
Calibrator Model :	TE-5028A	**Calibrator Slope :**	1.64598
Calibrator S/N :	2584	**Calibrator Intercept :**	-0.02439

Test No.	Delta H_2O (inch)	Q_{std} (m^3/min)	I : Chart (CFM)	Linear Regression
1	3.2	1.0958	40	Slope : 35.0803
2	4.2	1.2518	44	Intercept : 0.8954
3	5.3	1.4032	50	Correlation Coefficient : 0.9976
4	6.2	1.5157	54	
5	7.6	1.6755	60	

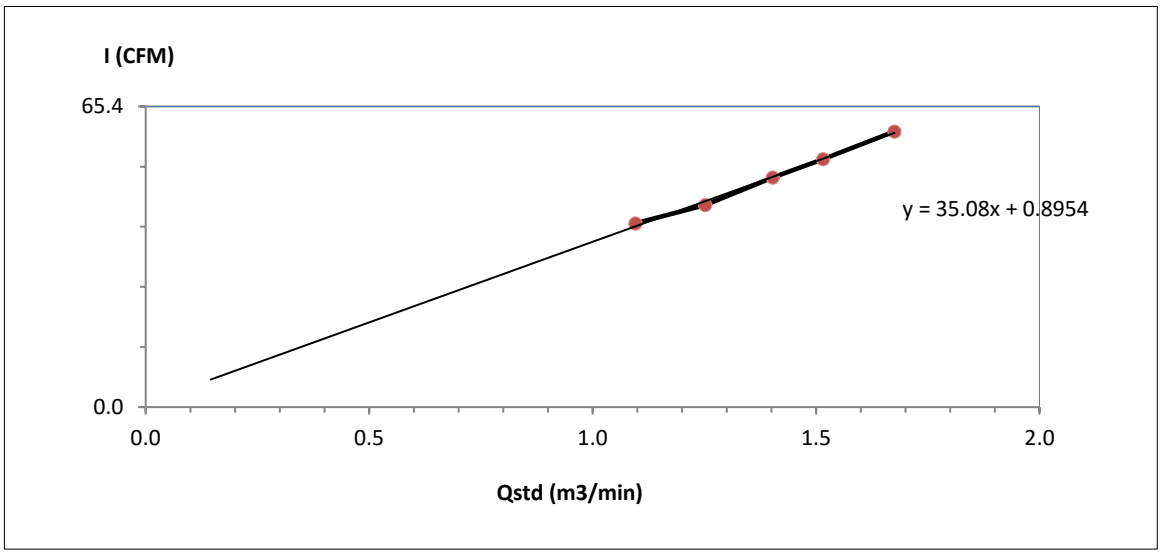

Calibrated by Autit Aoonsim

(Mr. Autit Aoonsim)
BKK Field Services Scientist (2)


Approved by : Warakorn P.

(Mr. Warakorn Pookrak)
Field Services Supervisor

High Volume Air Sampler Calibration Worksheet

Project Site :	Hin Kong Power Company Limited	**Barometric Pressure (mm Hg) :**	758.4
Calibrate Location :	บริเวณ รพ.สต.เจดีย์หัก (บ้านห้วยหมู)	**Temperature (°C) :**	33.0
Calibrate Date :	16-Mar-26	**High Volume ID :**	BKK_FS0370
CalibrationSheet No.:	**C-160326-BKK_FS0370**	**High Volume Model :**	TE-5009X
Calibrator ID:	BKK_FS0624	**High Volume S/N :**	4798
Calibrator Model :	TE-5028A	**Calibrator Slope :**	1.64598
Calibrator S/N :	2584	**Calibrator Intercept :**	-0.02439

Test No.	Delta H_2O (inch)	Q_{std} (m^3/min)	I : Chart (CFM)	Linear Regression
1	3.3	1.1124	40	Slope : 35.9814
2	4.2	1.2518	44	Intercept : -0.3812
3	5.2	1.3901	50	Correlation Coefficient : 0.9986
4	6.2	1.5157	54	
5	7.6	1.6755	60	

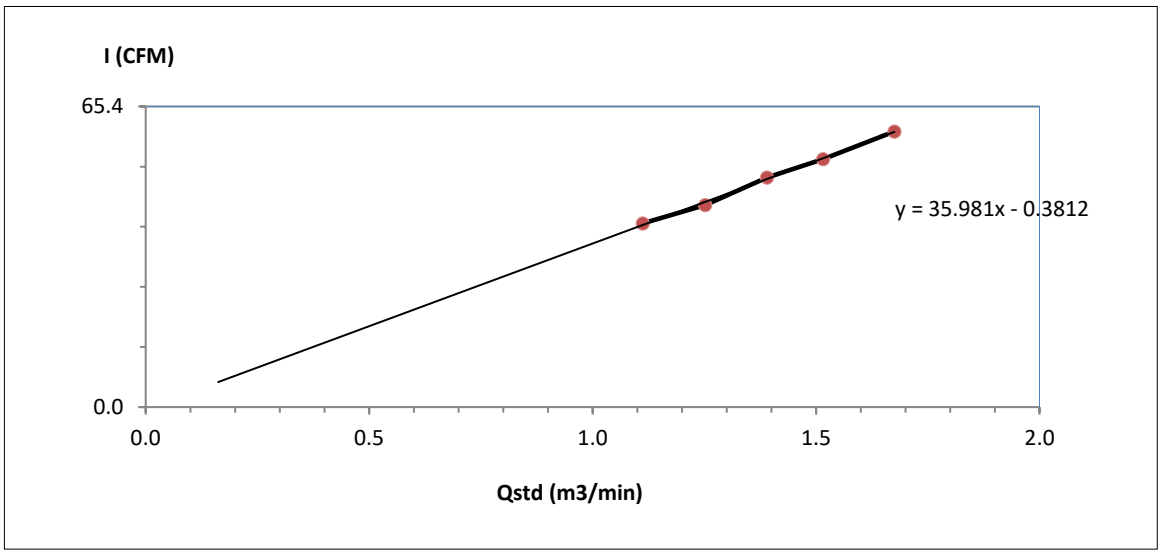

Calibrated by Autit Aoonsim

(Mr. Autit Aoonsim)
BKK Field Services Scientist (2)

Approved by : Warakorn P.

(Mr. Warakorn Pookrak)
Field Services Supervisor

JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Wind direction measurement laboratory
Calibration services department.

NSC – TISI – TIS 17025
CALIBRATION 0367

Certificate Number
CWD-061-67

CERTIFICATE OF CALIBRATION

MEASUREMENT ITEM	: Wind Direction Sensor
MANUFACTURER	: Novalynx
MODEL/TYPE	: Sensor: WS-02F Data logger: 200-WS-25LB
SERIAL NUMBER	: Sensor: WSD-A5377 Data logger: A5377
ID NUMBER	: BKK_FS0917
CONDITION AS-RECEIVED	: Used item
CUSTOMER	: ALS laboratory group (Thailand) Co., Ltd. 104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250 Thailand.
RECEIVED DATE	: 22 Nov 2024
MEASUREMENT DATE	: 25 Nov 2024
ISSUE DATE	: 25 Nov 2024

ENVIRONMENTAL CONDITIONS:
Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010± 10	hPa

PLACE OF CALIBRATION : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITION

: Wind tunnel cross-section area[1]	900	cm^2
Wind direction frontal area[2]	129	cm^2
Diameter of mounting pipe[3]	-	mm
Blockage ratio of test object[4]	0.143	[-]

Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are (23.7)°C, (50.3) %RH and (1007.9) hPa.

TABULATION OF RESULTS:
The table on next page give the measured values.

Calibrated by:
☑ Mr. Sorawit Thachalad
☐ Miss Jittraporn Lertsomphol

Approved signatory: .....
Mr. Parinya Booncharoen
Calibration Department Manager

Calibration procedure:
The wind direction sensor was calibrated against Standard Rotary Encoder model: AX4009TS-DM04-P3-S-U0 in an close test-section of Eiffel-type wind tunnel with 900 cm^2 cross test section area. The WI-CL-008 based on IEC 61400-12-1, Wind energy generation systems – Part 12-1: Power performance measurements of electricity producing wind turbines, March 2017 was used as a calibration guideline.

Traceability:
This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: DA-0027-24.

Uncertainty of Measurement:
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

REVIEW BY ..... Narakorn P.
APPROVED BY .....
NEXT CAL DATE..... 25/05/26

Remark:
[1] Nozzle cross-section area of the wind tunnel
[2] Projected cross-section area of the tested object include mounting pipe
[3] Diameter of mounting pipe
[4] Ratio [2] to [1]

Jiranatee Associates Co., Ltd.

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

Certificate Number
CWD-061-67

MEASUREMENT RESULTS [5]

The wind direction sensor was calibrated against standard rotary encoder by comparison method. During calibration, the measurement was carried out at 45° intervals in clockwise and counterclockwise directions after offset adjustment has been made. The flow speed of wind tunnel (usually 5 m/s) is kept constant while the sensor is rotated around its vertical axis. The results of calibration and associated measurement uncertainties are reported in the table below.

Air speed	D°_{std}	D°_{uuc}	Error	*U (k=2)*
m/s	Degree (°)	Degree (°)	Degree (°)	Degree (°)
5.02	45.000	41	-4	0.80
	90.000	86	-4	0.80
	135.000	132	-3	0.80
	180.000	181	1	0.80
	225.000	229	4	0.80
	270.000	275	5	0.80
	315.000	320	5	0.80
	360.000	359	-1	0.80

Remark:

[5] Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

[6] Direction of standard

[7] Direction of Unit Under Calibration

End of Certificate of Calibration

JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co., Ltd.

JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Air speed measurement laboratory
Calibration services department.

NSC – TISI – TIS 17025
CALIBRATION 0367

Certificate Number
CWS-061-67

CERTIFICATE OF CALIBRATION

MEASUREMENT ITEM : Cup anemometer
MANUFACTURER : Novalynx
MODEL/TYPE : Sensor: WS-02F
Data logger: 200-WS-25LB
SERIAL NUMBER : Sensor: WSD-A5377
Data logger: A5377
ID NUMBER : BKK_FS0917
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,
Khet Suan Luang, Bangkok 10250 Thailand.

RECEIVED DATE : 22 Nov 2024
MEASUREMENT DATE : 25 Nov 2024
ISSUE DATE : 25 Nov 2024

ENVIRONMENTAL CONDITIONS:
Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010± 10	hPa

PLACE OF CALIBRATION : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITIONS

: Wind tunnel cross-section area[1]	900	cm^2
Wind direction frontal area[2]	100	cm^2
Diameter of mounting pipe[3]	-	mm
Blockage ratio of test object[4]	0.111	[-]

Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are (24.9) °C, (43.3) %RH and (1008.2) hPa.

Calibration procedure:
The Cup anemometer was calibrated against Standard air velocity transducer model: 8455-12 and pitot tube with precision differential pressure meter model: DPM2500 in an close test-section of Eiffel-type wind tunnel with 900 cm^2 cross test section area. The WI-CL-007 based on IEC 61400-12-1, Wind energy generation systems – Part 12-1: Power performance measurements of electricity producing wind turbines, March 2017 was used as a calibration guideline.

Traceability:
This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MW-0007-24 and MW-0065-24

Uncertainty of Measurement:
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

TABULATION OF RESULTS:
The table on next page give the measured values.

Calibrated by:
☑ Mr. Sorawit Thachalad
☐ Miss Jittraporn Lertsomphol

JNAC JIRANATEE ASSOCIATES CO.,LTD.

Approved signatory: .....
Mr. Parinya Booncharoen
Calibration Department Manager

Remark:
[1] Nozzle cross-section area of the wind tunnel
[2] Projected cross-section area of the tested object include mounting pipe
[3] Diameter of mounting pipe
[4] Ratio [2] to [1]

Jiranatee Associates Co.,Ltd.

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

Certificate Number
CWS-061-67

MEASUREMENT RESULTS [5]

The Cup anemometer, Unit Under Calibration (UUC) was exercise at 10 m/s for 5 minutes prior to calibration being performed. The standard air velocity 0.5 m/s to 5 m/s was calculated by a standard air velocity transducer which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section and the standard air velocity 5 m/s to 30 m/s was calculated by a pitot tube with precision differential pressure meter which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section, UUC was mounted on a round vertical tube of the lower plate at center of test section. The calibration was carried out under both rising and falling air velocity in the range of 1 m/s to 16 m/s at calibration interval of 1 m/s. The results of calibration and associated measurement uncertainties are reported in the table below.

v_{std} [6] (m/s)	Temp. wind tunnel (°C)	Temp. room (°C)	v_{uuc} [7] (m/s)	Error (m/s)	*U (k=2)* (m/s)
1.012	24.10	24.90	0.9	-0.2	0.31
2.218	25.58	24.90	2.0	-0.2	0.31
3.050	24.10	24.90	2.9	-0.1	0.31
4.223	24.10	24.90	4.0	-0.2	0.31
4.94	24.10	24.90	5.0	0.0	0.31
5.96	24.60	24.90	6.0	0.0	0.31
7.03	24.10	24.90	7.2	0.1	0.31
7.96	24.34	24.90	8.1	0.1	0.31
8.97	24.10	24.90	9.0	0.1	0.31
9.97	24.18	24.90	9.9	-0.1	0.31
11.09	24.12	24.90	11.2	0.1	0.31
12.03	24.10	24.90	12.1	0.1	0.31
12.92	24.18	24.90	13.0	0.1	0.33
13.92	24.10	24.90	14.0	0.1	0.31
14.98	24.30	24.90	15.1	0.1	0.31
15.98	24.10	24.90	16.1	0.1	0.35


Remark:

[5] Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

[6] Velocity of standard

[7] Velocity of Unit Under Calibration

PHOTO OF CALIBRATION SET-UP

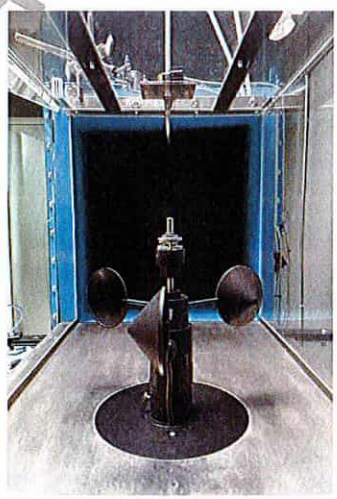

Calibration set-up of the Cup anemometer calibration in the wind tunnel of Jiranatee Associates Co., Ltd. The Cup anemometer shown may differ from the calibrated one. Remark: The proportion of the set- up is not true to scale due to imaging geometry.

End of Certificate of Calibration

JIRANATEE ASSOCIATES CO.,LTD

Jiranatee Associates Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate of Calibration

Customer

Name : ALS Laboratory Group Thailand Co., Ltd.
Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang, Bangkok 10250

Certificate No : 26-ACT-006
Request No : Req-2026-0042

Unit Under Calibration Details

Measurement item : Acoustic Calibrator
Manufacturer : RION
Model : NC-74
Serial Number : 34178119
ID : BKK_FS0632

Class : 1
Range : 94 dB / 1000 Hz
Instrument Status : Used

REVIEW BY ..... Narakorn P.
APPROVED BY.....
NEXT CAL DATE..... 08/01/27

Calibration Environment and Details

Temperature : (23 ±2 °C)
Humidity : (50 ± 20 %RH)
Barometric Pressure : (1013 ±10.0 hPa)
Received Date : 7 January 2026
Calibration Date : 9 January 2026
Location of Calibration : LAB 1 Acoustic
Calibration Procedure : In-house method CP-ACT-02 based on IEC 60942:2017 Electroacoustics - Sound calibrators

Reference Standard	Model	Serial Number	Traceable	Due Calibration
Sound Calibrator	SV 35A	58079	EEI	20 June 2026
THD Multimeter	2015	1047765	NIMT	4 February 2026

Traceability : This certificate providoes traceability of measurement to recognized national standard, and to the realization of the international System of Units (SI).

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k =2, providing a level of confidence approximately 95 %.

Calibrated By : Mr. Noppadon Luangart
Service Calibration Engineer

Approved By : Mr. Pacit Mathavorn
Calibration Engineer Supervisor

Issue Date : 9 January 2026

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate No : 26-ACT-006

Request No : Req-2026-0042

Sound pressure level **Calibration Results :** Without Adjustment

Calibration Range (dB)	Without Adjustment (dB)		Adjustment (dB)		Uncertainty (± dB)
	Measured	Deviated value	Measured	Deviated value	
94 dB / 1000 Hz	93.78	-0.22	-	-	0.12

Frequency of Sound pressure level

Calibration Range (Hz)	Without Adjustment		Adjustment		Uncertainty (± %)
	Measured (Hz)	Deviated value (%)	Measured (Hz)	Deviated value (%)	
94 dB / 1000 Hz	1000.00	0.000	-	-	0.010

Total Harmonic Distortion plus Noise of Sound pressure level (THD+N %)

Calibration Range (Hz)	Without Adjustment	Adjustment	Uncertainty (± %)
	Measured (%)	Measured (%)	
94 dB / 1000 Hz	1.52	-	0.17

Note :

- The calibration results exclude the calibrator pressure correction
- The calibration results exclude the microphone volume correction

End of Calibration

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

NSC-TISI-TIS 17025
CALIBRATION 0394

Calibration Certificate

Equipment :	SOUND LEVEL METER
Manufacturer :	RION
Model :	NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.:	00858519 / 157785/ 48094
ID No.:	BKK_FS0109

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location :	-	
Ambient Temperature :	(23.0 ± 3)	°C
Pressure :	(101.3 ± 3)	kPa
Relative Humidity :	(50.0 ± 20)	%

Received Date :	12 JANUARY 2026
Calibration Date :	27 JANUARY 2026
Date of Issue :	28 JANUARY 2026

REVIEW BY ..... Narakorn P.

APPROVED BY.....

NEXT CAL DATE..... 26/01/27

Calibrated by : Nathakorn Pisutpaisan

Approved by : Nitinun S.

(Nitinun Srihawan)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL26095
Job No. : VC69AC0057
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0011-25	11-FEB-26
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EEL.BP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EEL.BP 23/0268	22-APR-26
Digital Multimeter	34461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KAI	34560495	AA-3002-25	19-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :
   - 3.1 National Institute of Metrology (Thailand).
   - 3.2 Thailand Institute of Scientific and Technological Research (TISTR).
   - 3.3 Electrical And Electronics Institute (EEI).

Cert. No. : ACL26095
Job No. : VC69AC0057
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

Cert. No. : ACL26095
Job No. : VC69AC0057
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
14.6

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	12.0
C - weight	18.1
Flat	23.9

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.2	0.2	0.2	± 1.5
1000	-0.1	-0.1	0.0	± 1.0
8000	-0.8	-0.7	-0.6	±5.0

Cert. No. : ACL26095
Job No. : VC69AC0057
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	-0.1	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	-0.1	±1.5
500	0.0	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

NETINGALS.

Cert. No. : ACL26095
Job No. : VC69AC0057
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	29.0	0.0	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	26.9	-0.1	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	25.0	0.0	± 1.1

Cert. No. : ACL26095
Job No. : VC69AC0057
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	29.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.0 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

Cert. No. : ACL26095
Job No. : VC69AC0057
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.4	0.0	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.6	89.6	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a lavel of confidence of approximately 95 %

End of Calibration Certificate

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : ACL25383
Pages : 1 of 8

Calibration Certificate

Equipment :	SOUND LEVEL METER
Manufacturer :	RION
Model :	NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.:	00858517 / 157784 / 48099
ID No.:	BKK_FS0107

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location :	-	
Ambient Temperature :	(23.0 ± 3)	°C
Pressure :	(101.3 ± 3)	kPa
Relative Humidity :	(50.0 ± 20)	%

Received Date :	26 SEPTEMBER 2025
Calibration Date :	02 OCTOBER 2025
Date of Issue :	06 OCTOBER 2025

REVIEW BY ..... Nathakorn P.

APPROVED BY .....

NEXT CAL DATE..... 01/10/26 .....

Calibrated by : Nathakorn Pisutpaisan

Approved by : Nitinun S.

(Nitinun Srihawan)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL25383
Job No. : VC68AC0191
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0011-25	11-FEB-26
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EEL.BP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EEL.BP 23/0268	22-APR-26
Digital Multimeter	34461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KAI	34560495	AA-3002-25	19-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

3.3 Electrical And Electronics Institute (EEI).

Cert. No. : ACL25383
Job No. : VC68AC0191
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

Cert. No. : ACL25383
Job No. : VC68AC0191
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
17.06333333

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	13.1
C - weight	19.2
Flat	25.0

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.4	0.5	0.5	± 1.5
1000	0.1	0.1	0.1	± 1.0
8000	-0.4	-0.3	-0.3	±5.0

Cert. No. : ACL25383
Job No. : VC68AC0191
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	0.0	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

Cert. No. : ACL25383
Job No. : VC68AC0191
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	53.9	-0.1	± 1.1
49.0	48.9	-0.1	± 1.1
44.0	44.0	0.0	± 1.1
39.0	38.9	-0.1	± 1.1
34.0	33.9	-0.1	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	26.9	-0.1	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.8	-0.2	± 1.1

Cert. No. : ACL25383
Job No. : VC68AC0191
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	28.9	-0.1	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.0 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

Cert. No. : ACL25383
Job No. : VC68AC0191
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.6	0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a lavel of confidence of approximately 95 %

End of Calibration Certificate

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

SITHIPORN associates

ILAC-MRA

NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : ACL26094
Pages : 1 of 8

Calibration Certificate

Equipment :	SOUND LEVEL METER
Manufacturer :	RION
Model :	NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.:	00858518 / 136951/ 22311
ID No.:	BKK_FS0108

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location :	-	
Ambient Temperature :	(23.0 ± 3)	°C
Pressure :	(101.3 ± 3)	kPa
Relative Humidity :	(50.0 ± 20)	%

Received Date :	12 JANUARY 2026
Calibration Date :	27 JANUARY 2026
Date of Issue :	28 JANUARY 2026

REVIEW BY ..... Nathakorn P.

APPROVED BY .....

NEXT CAL DATE..... 26/01/27

Calibrated by : Nathakorn Pisutpaisan

Approved by : Nitinun S.

(Nitinun Srihawan)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL26094
Job No. : VC69AC0057
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0011-25	11-FEB-26
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EEL.BP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EEL.BP 23/0268	22-APR-26
Digital Multimeter	34461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KAI	34560495	AA-3002-25	19-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :
   - 3.1 National Institute of Metrology (Thailand).
   - 3.2 Thailand Institute of Scientific and Technological Research (TISTR).
   - 3.3 Electrical And Electronics Institute (EEI).

CYITRONICS

Cert. No. : ACL26094
Job No. : VC69AC0057
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

Cert. No. : ACL26094
Job No. : VC69AC0057
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
16.2

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	10.8
C - weight	17.5
Flat	23.1

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.4	0.4	0.4	± 1.5
1000	0.0	0.1	0.0	± 1.0
8000	-2.0	-1.9	-1.9	±5.0

Cert. No. : ACL26094
Job No. : VC69AC0057
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	0.0	-0.1	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

Nattawat.S.

Cert. No. : ACL26094
Job No. : VC69AC0057
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	78.9	-0.1	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	53.9	-0.1	± 1.1
49.0	48.9	-0.1	± 1.1
44.0	43.9	-0.1	± 1.1
39.0	38.9	-0.1	± 1.1
34.0	33.9	-0.1	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	26.9	-0.1	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.9	-0.1	± 1.1

Cert. No. : ACL26094
Job No. : VC69AC0057
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	28.8	-0.2	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.0 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

METHODS.

Cert. No. : ACL26094
Job No. : VC69AC0057
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.6	0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a lavel of confidence of approximately 95 %

End of Calibration Certificate

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

NSC-TISI-TIS 17025
CALIBRATION 0394

Calibration Certificate

Equipment :	SOUND LEVEL METER
Manufacturer :	RION
Model :	NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.:	00858516 / 158775 / 10641
ID No.:	BKK_FS0106

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location :	-	
Ambient Temperature :	(23.0 ± 3)	°C
Pressure :	(101.3 ± 3)	kPa
Relative Humidity :	(50.0 ± 20)	%

REVIEW BY ..... Nathakorn P.

APPROVED BY.....

NEXT CAL DATE..... 01/10/26

Received Date :	26 SEPTEMBER 2025
Calibration Date :	02 OCTOBER 2025
Date of Issue :	06 OCTOBER 2025

Calibrated by : Nathakorn Pisutpaisan

Approved by : N.S.

(Nitinun Srihawan)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL25382
Job No. : VC68AC0191
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0011-25	11-FEB-26
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EEL.BP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EEL.BP 23/0268	22-APR-26
Digital Multimeter	34461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KAI	34560495	AA-3002-25	19-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :
   - 3.1 National Institute of Metrology (Thailand).
   - 3.2 Thailand Institute of Scientific and Technological Research (TISTR).
   - 3.3 Electrical And Electronics Institute (EEI).

Cert. No. : ACL25382
Job No. : VC68AC0191
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

Cert. No. : ACL25382
Job No. : VC68AC0191

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
16.08333333

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	9.9
C - weight	16.7
Flat	22.4

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	1.0	1.1	1.1	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	-3.5	-3.4	-3.4	±5.0

Cert. No. : ACL25382
Job No. : VC68AC0191
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

Cert. No. : ACL25382
Job No. : VC68AC0191
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	29.0	0.0	± 1.1
28.0	28.0	0.0	± 1.1
27.0	26.9	-0.1	± 1.1
26.0	26.0	0.0	± 1.1
25.0	25.0	0.0	± 1.1

Cert. No. : ACL25382
Job No. : VC68AC0191
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	28.9	-0.1	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.0 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

Cert. No. : ACL25382
Job No. : VC68AC0191
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.6	89.5	-0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a lavel of confidence of approximately 95 %

End of Calibration Certificate

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

NSC-TISI-TIS 17025
CALIBRATION 0394

Calibration Certificate

Equipment :	SOUND CALIBRATOR
Manufacturer :	RION
Model :	NC-74
Serial No.:	34425567
ID No.:	BKK_FS0618

REVIEW BY ..... Nathakorn P.

APPROVED BY.....

NEXT CAL DATE..... 23/11/26

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location :	-	
Ambient Temperature :	(23.0 ± 3)	°C
Pressure :	(101.3 ± 3)	kPa
Relative Humidity :	(50.0 ± 20)	%

Received Date :	12 NOVEMBER 2025
Calibration Date :	24 NOVEMBER 2025
Date of Issue :	25 NOVEMBER 2025

Calibrated by : Nathakorn Pisutpaisan

Approved by : Nitinun S.

(Nitinun Srihawan)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACC25077
Job No. : VC69AC0032
Pages : 2 of 3

Calibration Procedure : CP-AC-03

Calibration Method :

This equipment was calibrated by follow on IEC-60942-2003 Standard.

The sound pressure level, frequency and total distortion of the sound calibrator was measured using the reference microphone.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EEL.BP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EEL.BP 23/0268	22-APR-26
Digital Multimeter	33461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KAI	34560495	AA-3002-25	19-FEB-26
Audio Analyzer	AVR-3360A	V744B6069	EF-0013-25	13-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

3.3 Electrical And Electronics Institute (EEI).

Cert. No. : ACC25077
Job No. : VC69AC0032
Pages : 3 of 3

Result of calibration :

1. Sound pressure level

Specified sound pressure level (dB)	Measured value (dB)	Deviated value (dB)	Uncertainty (dB)	Acceptance limit (dB)
94	94.03	0.03	0.14	0.40

2. Frequency

Specified Frequency (Hz)	Measured value (Hz)	Deviated value (%)	Uncertainty (%)	Acceptance limit (%)
1000	1004.4	0.4	0.1	1.0

3. Total distortion

Measured value (%)	Uncertainty (%)	Acceptance limit (%)
2.09	0.10	3.0

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a lavel of confidence of approximately 95 %

End of Calibration Certificate

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

NSC-TISI-TIS 17025
CALIBRATION 0394

Calibration Certificate

Equipment :	SOUND LEVEL METER
Manufacturer :	RION
Model :	NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.:	00658242 / 157782 / 48097
ID No.:	BKK_FS0099

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location :	-	
Ambient Temperature :	(23.0 ± 3)	°C
Pressure :	(101.3 ± 3)	kPa
Relative Humidity :	(50.0 ± 20)	%

REVIEW BY Narakorn P.

APPROVED BY

NEXT CAL DATE 03/09/26

Received Date :	22 AUGUST 2025
Calibration Date :	04 SEPTEMBER 2025
Date of Issue :	05 SEPTEMBER 2025

Calibrated by : Nathakorn Pisutpaisan

Approved by : Nitinun S.

(Nitinun Srihawan)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL25348
Job No. : VC68AC0172
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0011-25	11-FEB-26
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EEL.BP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EEL.BP 23/0268	22-APR-26
Digital Multimeter	34461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KAI	34560495	AA-3002-25	19-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :
   - 3.1 National Institute of Metrology (Thailand).
   - 3.2 Thailand Institute of Scientific and Technological Research (TISTR).
   - 3.3 Electrical And Electronics Institute (EEI).

Cert. No. : ACL25348
Job No. : VC68AC0172
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

Cert. No. : ACL25348
Job No. : VC68AC0172
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
17.4

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	15.7
C - weight	21.5
Flat	27.3

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.5	0.5	0.5	± 1.5
1000	0.1	0.1	0.1	± 1.0
8000	-1.8	-1.7	-1.7	±5.0

Cert. No. : ACL25348
Job No. : VC68AC0172
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.1	-0.1	±2.0
125	0.0	0.0	-0.1	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

Cert. No. : ACL25348
Job No. : VC68AC0172
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	29.0	0.0	± 1.1
28.0	28.0	0.0	± 1.1
27.0	27.0	0.0	± 1.1
26.0	26.0	0.0	± 1.1
25.0	25.0	0.0	± 1.1

Cert. No. : ACL25348
Job No. : VC68AC0172
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	28.9	-0.1	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.0 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

Cert. No. : ACL25348
Job No. : VC68AC0172
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.2	-0.2	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.6	89.6	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a lavel of confidence of approximately 95 %

End of Calibration Certificate

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : ACL26096
Pages : 1 of 8

Calibration Certificate

Equipment :	SOUND LEVEL METER
Manufacturer :	RION
Model :	NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.:	00858523 / 170666 / 73129
ID No.:	BKK_FS0113

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location :	-	
Ambient Temperature :	(23.0 ± 3)	°C
Pressure :	(101.3 ± 3)	kPa
Relative Humidity :	(50.0 ± 20)	%

Received Date :	12 JANUARY 2026
Calibration Date :	27 JANUARY 2026
Date of Issue :	28 JANUARY 2026

REVIEW BY Nathakorn P.

APPROVED BY

NEXT CAL DATE 26/01/27

Calibrated by : Nathakorn Pisutpaisan

Approved by : Nitinun S.

(Nitinun Srihawan)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL26096
Job No. : VC69AC0057
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0011-25	11-FEB-26
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EEL.BP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EEL.BP 23/0268	22-APR-26
Digital Multimeter	34461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KAI	34560495	AA-3002-25	19-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :
   - 3.1 National Institute of Metrology (Thailand).
   - 3.2 Thailand Institute of Scientific and Technological Research (TISTR).
   - 3.3 Electrical And Electronics Institute (EEI).

Cert. No. : ACL26096
Job No. : VC69AC0057
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

Cert. No. : ACL26096
Job No. : VC69AC0057
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
15.4

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	12.0
C - weight	18.1
Flat	23.9

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.0	0.1	0.2	± 1.5
1000	-0.1	-0.1	-0.1	± 1.0
8000	0.0	0.0	0.0	±5.0

Cert. No. : ACL26096
Job No. : VC69AC0057
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	-0.1	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

Cert. No. : ACL26096
Job No. : VC69AC0057
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	78.9	-0.1	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	63.9	-0.1	± 1.1
59.0	59.0	0.0	± 1.1
54.0	53.9	-0.1	± 1.1
49.0	48.9	-0.1	± 1.1
44.0	43.9	-0.1	± 1.1
39.0	38.9	-0.1	± 1.1
34.0	33.9	-0.1	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	26.9	-0.1	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.8	-0.2	± 1.1

METHODS

Cert. No. : ACL26096
Job No. : VC69AC0057
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	28.9	-0.1	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.0 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

Cert. No. : ACL26096
Job No. : VC69AC0057
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.6	89.6	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a lavel of confidence of approximately 95 %

End of Calibration Certificate

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : ACL26052
Pages : 1 of 8

Calibration Certificate

Equipment :	SOUND LEVEL METER
Manufacturer :	RION
Model :	NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.:	00858521 / 158765 / 58767
ID No.:	BKK_FS0111

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location :	-	
Ambient Temperature :	(23.0 ± 3)	°C
Pressure :	(101.3 ± 3)	kPa
Relative Humidity :	(50.0 ± 20)	%

Received Date : 05 JANUARY 2026
Calibration Date : 15 - 16 JANUARY 2026
Date of Issue : 19 JANUARY 2026

REVIEW BY ..... Nathakorn P.

APPROVED BY .....

NEXT CAL DATE..... 14/01/27

Calibrated by : Nathakorn Pisutpaisan

Approved by : Nitinun. S.

(Nitinun Srihawan)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL26052
Job No. : VC69AC0052
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0011-25	11-FEB-26
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EEL.BP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EEL.BP 23/0268	22-APR-26
Digital Multimeter	34461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KAI	34560495	AA-3002-25	19-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :
   - 3.1 National Institute of Metrology (Thailand).
   - 3.2 Thailand Institute of Scientific and Technological Research (TISTR).
   - 3.3 Electrical And Electronics Institute (EEI).

Cert. No. : ACL26052
Job No. : VC69AC0052
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

Cert. No. : ACL26052
Job No. : VC69AC0052
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
14.2

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	10.8
C - weight	17.0
Flat	22.7

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.7	0.7	0.7	± 1.5
1000	0.1	0.1	0.1	± 1.0
8000	-2.0	-1.9	-1.8	±5.0

Cert. No. : ACL26052
Job No. : VC69AC0052
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	0.0	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

Cert. No. : ACL26052
Job No. : VC69AC0052
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.1	0.1	± 1.1
30.0	30.0	0.0	± 1.1
29.0	29.1	0.1	± 1.1
28.0	28.3	0.3	± 1.1
27.0	27.1	0.1	± 1.1
26.0	26.1	0.1	± 1.1
25.0	25.2	0.2	± 1.1

Cert. No. : ACL26052
Job No. : VC69AC0052
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	29.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.0 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

Cert. No. : ACL26052
Job No. : VC69AC0052
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.4	0.0	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.5	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a lavel of confidence of approximately 95 %

End of Calibration Certificate

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate of Calibration

Customer

Name ALS Laboratory Group Thailand Co., Ltd. **Certificate No :** 25-SLM-147

Address 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang, Bangkok 10250 **Request No :** Req-2025-0772

Unit Under Calibration Details

Measurement item : : Sound Level Meter
Manufacturer : RION
Model : NL-42
Serial Number : 00873053
ID : BKK_FS0930
Resolution : 0.1 dB

Microphone Class : 2
Microphone Model : UC-52
Microphone S/N : 171587
Preamplifier Model : NH-24
Preamplifier S/N : 73329
Instrument Status : Used

Calibration Environment and Details

Temperature : 23 °C ± 2 °C
Humidity : 50 %RH ± 20 %RH
Barometric Pressure : 1013 hPa ± 10 hPa
Received Date : 28 March 2025
Calibrated Date : 28 April 2025
Calibration Procedure : In-house method CP-SLM-01 based on IEC 61672-3 : 2013 Electroacoustics - Sound level meters - Part 3: Periodic tests
Location of Calibration : Lab Acoustic

REVIEW BY ..... Narakorn P.
APPROVED BY .....
NEXT CAL DATE..... 28/04/26

Reference Standard

Instrument	**Brand**	Model	SN.	Due calibration	Tracebility
Standard Microphone	Bruel&Kjaer	4192	2294985	25 June 2025	NIMT
Audio Generator	Svantek	Svan401	131	15 October 2025	WK Electric

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k = 2, providing a level of confidence approximately 95 %.

Calibrated By : Mr. Noppadon Luangart
Service Calibration Engineer

Approved By : Mr. Pacit Mathavorn
Calibration Engineer Supervisor

Issue Date : 28 April 2025

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate No : 25-SLM-147

Request No : Req-2025-0772

1. Indication at the calibration check frequency

UUC Setting	Nominal	Before Adjust		After Adjust		UNCERTAINTY
FAST / A / 30-130	Level	UUC	ERR	UUC	ERR	
Calibrator Setting	(dB)	(dB)	(dB)	(dB)	(dB)	(± dB)
1000 Hz 94 dB	93.77	94.1	0.33	93.8	0.03	0.20

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand Svantek, Model SV35A, SN. 58079

2. Self-generated noise, Microphone installed

UUC Setting	Measured	UNCERTAINTY
FAST / 30-130		
UUC Weighting	(dB)	(± dB)
A	15.7	0.10

3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting	Measured	UNCERTAINTY
FAST / 30-130		
UUC Weighting	(dB)	(± dB)
A	12.4	0.10
C	16.3	0.10
Z	20.4	0.10

4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting	Deviation from various Frequency Weighting Respone curve			UNCERTAINTY
FAST / 30-130	A	C	Z	(± dB)
STD Setting	(dB)	(dB)	(dB)	
125 Hz	0.2	0.4	0.4	0.60
1000 Hz	0.0	0.0	0.0	0.60
4000 Hz	0.0	0.1	0.0	0.60
8000 Hz	-1.3	-1.4	-1.4	0.70

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate No : 25-SLM-147

Request No : Req-2025-0772

5. Electrical signal test of frequency weightings, Weighting network respone with relative to 1 kHz

UUC Setting	Deviation from various Frequency Weighting Respone curve			UNCERTAINTY
FAST / 30-130				
STD Setting	**A (dB)**	**C (dB)**	**Z (dB)**	**(± dB)**
63 Hz	-0.2	0.0	0.0	0.20
125 Hz	-0.1	0.1	0.0	
250 Hz	0.0	0.0	0.0	
500 Hz	0.0	0.1	0.1	
1000 Hz	0.0	0.0	0.1	
2000 Hz	0.1	0.1	0.1	
4000 Hz	0.0	0.1	0.1	
8000 Hz	0.1	0.1	0.1	
16000 Hz	-1.3	-1.3	0.1	

6. Frequency and time weightings at 1kHz

UUC Setting	STD	Measured		UNCERTAINTY
FAST / 30-130	REF	UUC	ERR	
UUC Weighting	**(dB)**	**(dB)**	**(dB)**	**(± dB)**
A	114.00	114.0	0.0	0.20
C	114.00	114.0	0.0	
Z	114.00	114.0	0.0	

UUC Setting	STD	Measured		UNCERTAINTY
30-130 / A	REF	UUC	ERR	
UUC Time Respone	**(dB)**	**(dB)**	**(dB)**	**(± dB)**
Fast	114.00	114.0	0.0	0.20
Slow	114.00	114.0	0.0	
Leq	114.00	114.0	0.0	

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate No : 25-SLM-147

Request No : Req-2025-0772

7. Long Term Stability

UUC Setting	Measured	UNCERTAINTY
FAST / A / 30-130	UUC	
STD Setting	(dB)	(± dB)
Initial	114.0	
Final	114.0	
Deviated	0.0	0.10

8. Level linearity on the reference level range

UUC Setting	Anticipated	Deviation		UNCERTAINTY
FAST / A / 30-130	REF	UUC	ERR	
STD dB	(dB)	(dB)	(dB)	(± dB)
138.00	138	138.0	0.0	0.30
134.00	134	134.0	0.0	
129.00	129	129.0	0.0	
124.00	124	124.0	0.0	
119.00	119	119.0	0.0	
114.00	114	114.0	0.0	
109.00	109	109.0	0.0	
104.00	104	104.0	0.0	
99.00	99	99.0	0.0	
94.00	94	94.0	0.0	
89.00	89	89.0	0.0	
84.00	84	84.0	0.0	
79.00	79	79.0	0.0	
74.00	74	74.0	0.0	
69.00	69	69.0	0.0	
64.00	64	64.0	0.0	
59.00	59	59.0	0.0	
54.00	54	54.0	0.0	
49.00	49	49.0	0.0	
44.00	44	44.0	0.0	
39.00	39	39.1	0.1	
34.00	34	34.1	0.1	
29.00	29	29.1	0.1	
24.00	24	24.0	0.0	

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate No : 25-SLM-147

Request No : Req-2025-0772

9. Level linearity including the level range control

UUC Setting	STD	Measured		UNCERTAINTY
FAST / A	REF	UUC	ERR	
UUC Range	(dB)	(dB)	(dB)	(± dB)
30-130	29.50	29.6	0.1	0.30
	114	114.0	0.0	

10. Tone burst response

UUC Setting	STD	Anticipated	Measured		UNCERTAINTY
A / 30-130	Toneburst	Ref	UUC	ERR	
UUC Time Respone	(ms)	(dB)	(dB)	(dB)	(± dB)
Fast	200	126.0	126.1	+0.1	0.20
	2	109.0	109.0	0.0	
	0.25	100.0	99.9	-0.1	
Slow	200	119.6	119.6	0.0	
	2	100.0	100.0	0.0	
SEL	200	120.0	120.0	0.0	
	2	100.0	100.0	0.0	
	0.25	91.0	90.9	-0.1	

11. Peak C Sound level

UUC Setting	Anticipated	Measured		UNCERTAINTY
FAST / C / 55-141	REF	UUC	ERR	
STD Setting	(dB)	(dB)	(dB)	(± dB)
Complete cycle	136.4	135.8	-0.60	0.20
Positive half cycle	135.4	135.2	-0.20	
Negative half cycle	135.4	135.2	-0.20	

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate No : 25-SLM-147

Request No : Req-2025-0772

12. Overload indication

UUC Setting	Measured	UNCERTAINTY
FAST / A / 30-130	UUC	
STD Setting	(dB)	(± dB)
Positive one-half cycle	139.3	
Negative one-half cycle	139.5	
Deviated	-0.2	0.20

13. High Level Stability

UUC Setting	Measured	UNCERTAINTY
FAST / A / 30-130	UUC	
STD Setting	(dB)	(± dB)
Initial	129.0	
Final	129.0	
Deviated	0.0	0.10

End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

NSC-TISI-TIS 17025
CALIBRATION 0394

Calibration Certificate

Equipment :	SOUND LEVEL METER
Manufacturer :	RION
Model :	NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.:	00858526 / 158764 / 58770
ID No.:	BKK_FS0116

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location :	-	
Ambient Temperature :	(23.0 ±3)	°C
Pressure :	(101.3 ±3)	kPa
Relative Humidity :	(50.0 ±20)	%

Received Date :	12 JANUARY 2026
Calibration Date :	27 JANUARY 2026
Date of Issue :	28 JANUARY 2026

REVIEW BY ..... Nathakorn P.

APPROVED BY.....

NEXT CAL DATE..... 26/01/27

Calibrated by : Nathakorn Pisutpaisan

Approved by : NITINUN.S.

(Nitinun Srihawan)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL26098
Job No. : VC69AC0057
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0011-25	11-FEB-26
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EEL.BP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EEL.BP 23/0268	22-APR-26
Digital Multimeter	34461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KAI	34560495	AA-3002-25	19-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :
   - 3.1 National Institute of Metrology (Thailand).
   - 3.2 Thailand Institute of Scientific and Technological Research (TISTR).
   - 3.3 Electrical And Electronics Institute (EEI).

Cert. No. : ACL26098
Job No. : VC69AC0057
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

Cert. No. : ACL26098
Job No. : VC69AC0057
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
13.4

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	9.9
C - weight	16.3
Flat	22.0

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.5	0.6	0.6	± 1.5
1000	-0.1	-0.1	-0.1	± 1.0
8000	-2.3	-2.2	-2.2	±5.0

Cert. No. : ACL26098
Job No. : VC69AC0057
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.1	0.0	±2.0
125	-0.1	0.0	0.0	±1.5
250	-0.1	0.0	-0.1	±1.5
500	-0.1	0.1	-0.1	±1.5
1000	0.0	0.0	-0.1	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.1	0.0	±3.0
8000	0.0	0.1	0.0	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.1	0.1	± 0.3

NEITHONS.

Cert. No. : ACL26098
Job No. : VC69AC0057
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.1	0.1	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.1	0.1	± 1.1
114.0	114.1	0.1	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.1	0.1	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	26.9	-0.1	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.9	-0.1	± 1.1

Cert. No. : ACL26098
Job No. : VC69AC0057
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	29.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	108.0	0.0	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.1	0.1	1.0 ; -5.0
	200	800	127.6	127.7	0.1	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

Cert. No. : ACL26098
Job No. : VC69AC0057
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.4	0.0	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.6	0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a lavel of confidence of approximately 95 %

End of Calibration Certificate

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : ACL25493
Pages : 1 of 8

Calibration Certificate

Equipment :	SOUND LEVEL METER
Manufacturer :	RION
Model :	NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.:	00572564 / 170401 / 72902
ID No.:	BKK_FS0880

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location :	-	
Ambient Temperature :	(23.0 ± 3)	°C
Pressure :	(101.3 ± 3)	kPa
Relative Humidity :	(50.0 ± 20)	%

Received Date :	08 DECEMBER 2025
Calibration Date :	18-19 DECEMBER 2025
Date of Issue :	22 DECEMBER 2025

REVIEW BY ..... Nanakorn P.

APPROVED BY .....

NEXT CAL DATE.....17/12/26.....

Calibrated by : Nathakorn Pisutpaisan

Approved by : Nitinun S.

(Nitinun Srihawan)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL25493
Job No. : VC69AC0042
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0011-25	11-FEB-26
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EEL.BP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EEL.BP 23/0268	22-APR-26
Digital Multimeter	34461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KAI	34560495	AA-3002-25	19-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :
   - 3.1 National Institute of Metrology (Thailand).
   - 3.2 Thailand Institute of Scientific and Technological Research (TISTR).
   - 3.3 Electrical And Electronics Institute (EEI).

Cert. No. : ACL25493
Job No. : VC69AC0042
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

Cert. No. : ACL25493
Job No. : VC69AC0042
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
16.4

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	11.2
C - weight	17.3
Flat	23.3

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.3	0.3	0.3	± 1.5
1000	-0.1	-0.1	-0.1	± 1.0
8000	-0.8	-0.8	-0.8	±5.0

Cert. No. : ACL25493
Job No. : VC69AC0042
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.1	-0.1	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	-0.1	-0.1	±1.5
500	0.0	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.0	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

Cert. No. : ACL25493
Job No. : VC69AC0042
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.1	0.1	± 1.1
136.0	136.1	0.1	± 1.1
135.0	135.1	0.1	± 1.1
134.0	134.1	0.1	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.1	0.1	± 1.1
124.0	124.1	0.1	± 1.1
119.0	119.1	0.1	± 1.1
114.0	114.1	0.1	± 1.1
109.0	109.1	0.1	± 1.1
104.0	104.1	0.1	± 1.1
99.0	99.1	0.1	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	28.0	0.0	± 1.1
27.0	27.0	0.0	± 1.1
26.0	26.0	0.0	± 1.1
25.0	25.0	0.0	± 1.1

Cert. No. : ACL25493
Job No. : VC69AC0042
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	28.9	-0.1	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.0 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.8	-0.2	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

Cert. No. : ACL25493
Job No. : VC69AC0042
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.4	0.0	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.5	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a lavel of confidence of approximately 95 %

End of Calibration Certificate

NTBoonyo-5.

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

NSC-TISI-TIS 17025
CALIBRATION 0394

Calibration Certificate

Equipment :	SOUND CALIBRATOR
Manufacturer :	RION
Model :	NC-74
Serial No.:	34178117
ID No.:	BKK_FS0630

REVIEW BY Nathakorn P.

APPROVED BY

NEXT CAL DATE 15/07/26

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location :	-	
Ambient Temperature :	(23.0 ± 3)	°C
Pressure :	(101.3 ± 3)	kPa
Relative Humidity :	(50.0 ± 20)	%

Received Date :	07 JULY 2025
Calibration Date :	16 JULY 2025
Date of Issue :	17 JULY 2025

Calibrated by : Nathakorn Pisutpaisan

Approved by : Wichok E.

(Wichok Ekpongpradit)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACC25033
Job No. : VC68AC0144
Pages : 2 of 3

Calibration Procedure : CP-AC-03

Calibration Method :

This equipment was calibrated by follow on IEC-60942-2003 Standard.

The sound pressure level, frequency and total distortion of the sound calibrator was measured using the reference microphone.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EEL.BP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EEL.BP 23/0268	22-APR-26
Digital Multimeter	33461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KAI	34560495	AA-3002-25	19-FEB-26
Audio Analyzer	AVR-3360A	V744B6069	EF-0013-25	13-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :
   - 3.1 National Institute of Metrology (Thailand).
   - 3.2 Thailand Institute of Scientific and Technological Research (TISTR).
   - 3.3 Electrical And Electronics Institute (EEI).

Cert. No. : ACC25033
Job No. : VC68AC0144
Pages : 3 of 3

Result of calibration :

1. Sound pressure level

Specified sound pressure level (dB)	Measured value (dB)	Deviated value (dB)	Uncertainty (dB)	Acceptance limit (dB)
94	94.20	0.20	0.14	0.40

2. Frequency

Specified Frequency (Hz)	Measured value (Hz)	Deviated value (%)	Uncertainty (%)	Acceptance limit (%)
1000	1001.7	0.2	0.1	1.0

3. Total distortion

Measured value (%)	Uncertainty (%)	Acceptance limit (%)
1.53	0.10	3.0

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a lavel of confidence of approximately 95 %

End of Calibration Certificate

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : ACL26055
Pages : 1 of 8

Calibration Certificate

Equipment :	SOUND LEVEL METER
Manufacturer :	RION
Model :	NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.:	00572551 / 158776 / 58777
ID No.:	BKK_FS0876

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location :	-	
Ambient Temperature :	(23.0 ±3)	°C
Pressure :	(101.3 ±3)	kPa
Relative Humidity :	(50.0 ±20)	%

Received Date :	05 JANUARY 2026
Calibration Date :	15 - 16 JANUARY 2026
Date of Issue :	19 JANUARY 2026

REVIEW BY ..... Nathakorn P.

APPROVED BY .....

NEXT CAL DATE..... 14/01/27

Calibrated by : Nathakorn Pisutpaisan

Approved by :

(Nitinun Srihawan)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL26055
Job No. : VC69AC0052
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0011-25	11-FEB-26
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EEL.BP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EEL.BP 23/0268	22-APR-26
Digital Multimeter	34461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KAI	34560495	AA-3002-25	19-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :
   - 3.1 National Institute of Metrology (Thailand).
   - 3.2 Thailand Institute of Scientific and Technological Research (TISTR).
   - 3.3 Electrical And Electronics Institute (EEI).

Cert. No. : ACL26055
Job No. : VC69AC0052
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

Cert. No. : ACL26055
Job No. : VC69AC0052
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
17.4

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	11.3
C - weight	17.3
Flat	23.1

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.2	0.2	0.2	± 1.5
1000	0.2	0.2	0.1	± 1.0
8000	3.0	3.1	3.1	±5.0

Cert. No. : ACL26055
Job No. : VC69AC0052
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.1	-0.1	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

Cert. No. : ACL26055
Job No. : VC69AC0052
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	53.9	-0.1	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	38.9	-0.1	± 1.1
34.0	33.9	-0.1	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	26.9	-0.1	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.9	-0.1	± 1.1

Cert. No. : ACL26055
Job No. : VC69AC0052
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	28.9	-0.1	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.0 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

Cert. No. : ACL26055
Job No. : VC69AC0052
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.6	89.6	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a lavel of confidence of approximately 95 %

End of Calibration Certificate

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : ACL26054
Pages : 1 of 8

Calibration Certificate

Equipment :	SOUND LEVEL METER
Manufacturer :	RION
Model :	NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.:	00572566 / 142140 / 22309
ID No.:	BKK_FS0875

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location :	-	
Ambient Temperature :	(23.0 ±3)	°C
Pressure :	(101.3 ±3)	kPa
Relative Humidity :	(50.0 ±20)	%

REVIEW BY Nrakorn P.

APPROVED BY .....

NEXT CAL DATE 14/01/27

Received Date :	05 JANUARY 2026
Calibration Date :	15 - 16 JANUARY 2026
Date of Issue :	19 JANUARY 2026

Calibrated by : Nathakorn Pisutpaisan

Approved by : Nitinun S.

(Nitinun Srihawan)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL26054
Job No. : VC69AC0052
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0011-25	11-FEB-26
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EEL.BP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EEL.BP 23/0268	22-APR-26
Digital Multimeter	34461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KAI	34560495	AA-3002-25	19-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :
   - 3.1 National Institute of Metrology (Thailand).
   - 3.2 Thailand Institute of Scientific and Technological Research (TISTR).
   - 3.3 Electrical And Electronics Institute (EEI).

Cert. No. : ACL26054
Job No. : VC69AC0052
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

Cert. No. : ACL26054
Job No. : VC69AC0052

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
16.1

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	14.3
C - weight	21.0
Flat	26.0

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.3	0.4	0.4	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	-0.5	-0.4	-0.4	±5.0

Cert. No. : ACL26054
Job No. : VC69AC0052
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.1	0.0	0.0	±2.0
125	0.1	0.1	0.1	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.1	0.1	± 0.3

Cert. No. : ACL26054
Job No. : VC69AC0052
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	29.0	0.0	± 1.1
28.0	28.0	0.0	± 1.1
27.0	27.1	0.1	± 1.1
26.0	26.2	0.2	± 1.1
25.0	25.2	0.2	± 1.1

Cert. No. : ACL26054
Job No. : VC69AC0052
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	29.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.0 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

Cert. No. : ACL26054
Job No. : VC69AC0052
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.4	0.0	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	132.9	-0.1	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.5	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a lavel of confidence of approximately 95 %

End of Calibration Certificate

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : ACL26137
Pages : 1 of 8

Calibration Certificate

Equipment :	SOUND LEVEL METER			
Manufacturer :	RION	Model :	NL-42	Serial No.: 00873053
Microphone :	RION	Model :	UC-52	Serial No.: 171587
Preamplifier No.:	RION	Model :	NH-24	Serial No.: 73329
Class No.:	CLASS 2			
ID No.:	BKK_FS0930			

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location :	-	
Ambient Temperature :	(23.0 ±3)	°C
Pressure :	(101.3 ±3)	kPa
Relative Humidity :	(50.0 ±20)	%

Received Date : 08 APRIL 2026
Calibration Date : 16-22 APRIL 2026
Date of Issue : 22 APRIL 2026

REVIEW BY ..... Nnakorn P.
APPROVED BY .....
NEXT CAL DATE..... 15/04/27

Calibrated by : Mr. Nathakorn Pisutpaisan

Approved by : Nitinun S.

(Nitinun Srihawan)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL26137
Job No. : VC69AC0087
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0014-26	12-FEB-27
Waveform Generator	33511B	MY52302742	EF-0015-26	11-FEB-27
Digital Multimeter	33461A	MY53220104	CA20260104EA	17-MAR-27
Digital Multimeter	33461A	MY53220076	CA20260102EA	18-MAR-27
Digital Multimeter	34461A	MY60024273	CA20260103EA	18-MAR-27
Programmable Attenuator	MAT-1070	62100114	EF-0016-26	11-FEB-27
Condenser Microphone	4180	2977900	AA-1006-26	12-FEB-27
Measuring Amplifier	NA-42KAI	34560495	AA-3004-26	17-FEB-27

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

   3.1 National Institute of Metrology (Thailand).

   3.2 Electrical And Electronics Institute (EEI).

Cert. No. : ACL26137
Job No. : VC69AC0087
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.1	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.1	0.25
12. High level stability	0.1	0.1

Cert. No. : ACL26137
Job No. : VC69AC0087
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.99)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
15.4

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	12.0
C - weight	17.9
Flat	23.8

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.2	0.3	0.3	± 1.5
1000	0.0	0.1	0.0	± 1.0
8000	0.3	0.4	0.3	±5.0

Cert. No. : ACL26137
Job No. : VC69AC0087
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	-0.1	-0.1	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	-0.1	±1.5
500	0.0	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

Cert. No. : ACL26137
Job No. : VC69AC0087
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	29.0	0.0	± 1.1
28.0	28.0	0.0	± 1.1
27.0	27.0	0.0	± 1.1
26.0	26.0	0.0	± 1.1
25.0	25.0	0.0	± 1.1

Cert. No. : ACL26137
Job No. : VC69AC0087
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	28.9	-0.1	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.0 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

Cert. No. : ACL26137
Job No. : VC69AC0087
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.4	0.0	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.6	89.5	-0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a lavel of confidence of approximately 95 %

End of Calibration Certificate

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

NSC-TISI-TIS 17025
CALIBRATION 0394

Calibration Certificate

Equipment :	SOUND LEVEL METER
Manufacturer :	RION
Model :	NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.:	00672789 / 158774 / 58775
ID No.:	BKK_FS0929

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location :	-	
Ambient Temperature :	(23.0 ±3)	°C
Pressure :	(101.3 ±3)	kPa
Relative Humidity :	(50.0 ±20)	%

Received Date :	12 JANUARY 2026
Calibration Date :	27 JANUARY 2026
Date of Issue :	28 JANUARY 2026

REVIEW BY ..... Nathakorn P.

APPROVED BY .....

NEXT CAL DATE..... 26/01/27

Calibrated by : Nathakorn Pisutpaisan

Approved by : NITINUN.S.

(Nitinun Srihawan)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL26100
Job No. : VC69AC0057
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0011-25	11-FEB-26
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EEL.BP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EEL.BP 23/0268	22-APR-26
Digital Multimeter	34461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KAI	34560495	AA-3002-25	19-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :
   - 3.1 National Institute of Metrology (Thailand).
   - 3.2 Thailand Institute of Scientific and Technological Research (TISTR).
   - 3.3 Electrical And Electronics Institute (EEI).

Cert. No. : ACL26100
Job No. : VC69AC0057
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

Cert. No. : ACL26100
Job No. : VC69AC0057
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
13.8

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	8.7
C - weight	15.9
Flat	21.8

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.7	0.3	0.7	± 1.5
1000	0.1	0.1	0.2	± 1.0
8000	-1.8	-1.7	-1.7	±5.0

Cert. No. : ACL26100
Job No. : VC69AC0057
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	-0.1	-0.1	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	-0.1	±1.5
500	0.0	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

ATTENTION-S.

Cert. No. : ACL26100
Job No. : VC69AC0057
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.1	0.1	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	29.0	0.0	± 1.1
28.0	28.0	0.0	± 1.1
27.0	27.0	0.0	± 1.1
26.0	26.0	0.0	± 1.1
25.0	24.9	-0.1	± 1.1

Cert. No. : ACL26100
Job No. : VC69AC0057
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	28.9	-0.1	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.0 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

Cert. No. : ACL26100
Job No. : VC69AC0057
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.4	0.0	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.5	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a lavel of confidence of approximately 95 %

End of Calibration Certificate

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

SITHIPORN associates

NSC-TISI-TIS 17025
CALIBRATION 0394

Calibration Certificate

Equipment :	SOUND LEVEL METER
Manufacturer :	RION
Model :	NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.:	00597155 / 180398 / 88168
ID No.:	BKK_FS0993

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location :	-	
Ambient Temperature :	(23.0 ± 3)	°C
Pressure :	(101.3 ± 3)	kPa
Relative Humidity :	(50.0 ± 20)	%

Received Date :	11 SEPTEMBER 2025
Calibration Date :	29 SEPTEMBER 2025
Date of Issue :	30 SEPTEMBER 2025

REVIEW BY ..... Nathakorn P.

APPROVED BY .....

NEXT CAL DATE..... 28/09/26

Calibrated by : Nathakorn Pisutpaisan

Approved by : Nitinun. S.

(Nitinun Srihawan)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL25375
Job No. : VC68AC0183
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0011-25	11-FEB-26
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EEL.BP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EEL.BP 23/0268	22-APR-26
Digital Multimeter	34461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KAI	34560495	AA-3002-25	19-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :
   - 3.1 National Institute of Metrology (Thailand).
   - 3.2 Thailand Institute of Scientific and Technological Research (TISTR).
   - 3.3 Electrical And Electronics Institute (EEI).

Cert. No. : ACL25375
Job No. : VC68AC0183
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

Cert. No. : ACL25375
Job No. : VC68AC0183
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
18.07333333

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	11.6
C - weight	17.8
Flat	23.4

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.1	0.1	0.2	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	1.0	1.0	1.1	±5.0

Cert. No. : ACL25375
Job No. : VC68AC0183
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	0.0	±2.0
125	0.0	0.1	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

Cert. No. : ACL25375
Job No. : VC68AC0183
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	28.0	0.0	± 1.1
27.0	26.9	-0.1	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	25.0	0.0	± 1.1

Cert. No. : ACL25375
Job No. : VC68AC0183
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	29.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.0 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

Cert. No. : ACL25375
Job No. : VC68AC0183
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.5	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a lavel of confidence of approximately 95 %

End of Calibration Certificate

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

NSC-TISI-TIS 17025
CALIBRATION 0394

Calibration Certificate

Equipment :	SOUND LEVEL METER
Manufacturer :	RION
Model :	NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.:	00597159 / 180402 / 88172
ID No.:	BKK_FS0995

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location :	-	
Ambient Temperature :	(23.0 ± 3)	°C
Pressure :	(101.3 ± 3)	kPa
Relative Humidity :	(50.0 ± 20)	%

REVIEW BY ..... Nathakorn P.

APPROVED BY .....

NEXT CAL DATE..... 23/11/26

Received Date :	12 NOVEMBER 2025
Calibration Date :	24 NOVEMBER 2025
Date of Issue :	25 NOVEMBER 2025

Calibrated by : Nathakorn Pisutpaisan

Approved by : NITINUN S.

(Nitinun Srihawan)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL25442
Job No. : VC69AC0032
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0011-25	11-FEB-26
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EEL.BP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EEL.BP 23/0268	22-APR-26
Digital Multimeter	34461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KAI	34560495	AA-3002-25	19-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

3.3 Electrical And Electronics Institute (EEI).

Nittakun.S.

Cert. No. : ACL25442
Job No. : VC69AC0032
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.5	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

Cert. No. : ACL25442
Job No. : VC69AC0032
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
15.8

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	13.4
C - weight	19.2
Flat	24.7

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.1	0.2	0.1	± 1.5
1000	0.0	0.1	0.0	± 1.0
8000	1.5	2.1	2.1	±5.0

Cert. No. : ACL25442
Job No. : VC69AC0032
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	0.0	±2.0
125	0.0	0.1	0.0	±1.5
250	0.1	0.0	0.0	±1.5
500	0.0	0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.1	±2.0
4000	0.0	0.1	0.1	±3.0
8000	0.1	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.1	0.1	± 0.3

Cert. No. : ACL25442
Job No. : VC69AC0032
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.1	0.1	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.1	0.1	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	29.0	0.0	± 1.1
28.0	28.0	0.0	± 1.1
27.0	27.0	0.0	± 1.1
26.0	26.0	0.0	± 1.1
25.0	25.1	0.1	± 1.1

Cert. No. : ACL25442
Job No. : VC69AC0032
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	28.9	-0.1	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	116.9	-0.1	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	107.9	-0.1	1.0 ; -5.0
	200	800	127.6	127.5	-0.1	±1.0
SEL	0.25	1	99.0	98.8	-0.2	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

Cert. No. : ACL25442
Job No. : VC69AC0032
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.4	0.0	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.5	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a lavel of confidence of approximately 95 %

End of Calibration Certificate

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Certificate of Calibration

Certificate No. : 26PH20
Page : 1 of 2

Equipment :	Lux Meter
Manufacturer:	Extech
Model :	407026
Serial No.:	A.060287
ID No.:	BKK_FS1345
Condition As-Received:	Used Item
Received Date:	12 January 2026
Calibration Date:	20 January 2026
Reference:	2601-0279WSC
Ambient Temperature:	(23 ± 2) °C
Relative Humidity:	(50 ± 15) %

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

Submitted by: ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand

Procedure used: Calibration were conducted using calibration procedure No. CP-PH01 based on inverse square law technique.

Condition of this result of calibration

1.Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Photometry & Encorder	LMguide 9,6 m	120RC003	DL-0030-25	18 Jul 2028
2) STANDARD LAMP	OL FEL-U	F-1784	TP-1014-25	24 Feb 2026

2.This result of calibration was made on requested at the point specified by customer.

3.Test Equipment : Programmable Voltage/Current Source (Model : OL83A, S/N : 16221394).

4.Test Equipment : Illuminance Meter (Model : 51002, S/N : 080129).

5.The certificate is valid only to the item calibrated on date and place of calibration.

6.This measurement result is traceable to the International System of Unit maintained through:-

-National Institute of Metrology Thailand (NIMT)

-National Institute of Metrology (Thailand), NSC-ONSC Accredited No. Calibration 0144

REVIEW BY ..... Narakorn P.

APPROVED BY .....

NEXT CAL DATE..... 19/01/27

Calibrated by : Nivat Nitas
Issue Date : 21 January 2026

Approved Signatory : .....

[ ] Phalinee Prabpaipal
[ ] Chatchawan Khunpiluek
[✓] Nuntawat Khamchai

Result of calibration:- (*) Without adjustment ( ) After adjustment

Function : Illuminance Measurement **Range :** 2000 lx

Standard Value	UUC* Reading	Error	Uncertainty
(lx)	(lx)	(lx)	(± lx)
0	0	0	-
15	13	-2	0.61
100	101	1	1.3
500	510	10	6.5
1000	1016	16	13
1500	1518	18	20
1900	1916	16	25

Function : Illuminance Measurement **Range :** 20000 lx

Standard Value	UUC* Reading	Error	Uncertainty
(lx)	(lx)	(lx)	(± lx)
2000	2010	10	26
3000	2970	-30	39
4000	3930	-70	52
5000	4890	-110	65

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95 %

Light source factor setting mode : L
UUC* = Unit Under Calibration.

-o0o-

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Certificate of Calibration

Certificate No. : 25PH553

Equipment : Lux Meter
Manufacturer: TENMARS
Model : TM-201L
Serial No.: 230701779
ID No.: BKK_FS1395
Condition As-Received: Used Item
Received Date: 17 November 2025
Calibration Date: 21 November 2025

This certificate may not be reproduced other than in full,
except with the prior written approval of the head of
Corporate Services 3: Equipment Calibration and Testing Services.

Reference: 2511-0465WSC
Ambient Temperature: (23 ± 2) °C
Relative Humidity: (50 ± 15) %

Submitted by: ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand

Procedure used: Calibration were conducted using calibration procedure No. CP-PH01 based on inverse square law technique.

Condition of this result of calibration

1.Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Photometry & Encorder	LMguide 9,6 m	120RC003	DL-0030-25	18 Jul 2028
2) STANDARD LAMP	OL FEL-U	F-1783	TP-1013-25	30 Dec 2025

2.This result of calibration was made on requested at the point specified by customer.

3.Test Equipment : Programmable Voltage/Current Source (Model : OL83A, S/N : 16221394).

4.Test Equipment : Illuminance Meter (Model : 51002, S/N : 080129).

5.The certificate is valid only to the item calibrated on date and place of calibration.

6.This measurement result is traceable to the International System of Unit maintained through:-

-National Institute of Metrology Thailand (NIMT)

-National Institute of Metrology (Thailand), NSC-ONSC Accredited No. Calibration 0144

REVIEW BY ..... Narakorn P.
APPROVED BY.....
NEXT CAL DATE.....20/11/26.....

Calibrated by : Nivat Nitas
Issue Date : 21 November 2025

Approved Signatory : _____

[ ] Phalinee Prabpaipal
[ ] Chatchawan Khunpiluek
[✓] Nuntawat Khamchai

Result of calibration:- (*) Without adjustment ( ) After adjustment

Function : Illuminance Measurement **Range :** 200 lx

Standard Value	UUC* Reading	Error	Uncertainty
(lx)	(lx)	(lx)	(± lx)
0	0.0	0.0	-
15	15.1	0.1	0.20
20	20.1	0.1	0.65
50	50.1	0.1	1.3
100	100.1	0.1	1.3
150	150.0	0.0	2.0
190	190.0	0.0	2.5

Function : Illuminance Measurement **Range :** 2000 lx

Standard Value	UUC* Reading	Error	Uncertainty
(lx)	(lx)	(lx)	(± lx)
200	202	2	2.6
500	502	2	6.5
1000	1001	1	13
1500	1500	0	20
1900	1900	0	25

Function : Illuminance Measurement **Range :** 20000 lx

Standard Value	UUC* Reading	Error	Uncertainty
(lx)	(lx)	(lx)	(± lx)
2000	2020	20	26
3000	3010	10	39
4000	4010	10	52
5000	5010	10	65

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k = 2* , providing a level of confidence of approximately 95 %

UUC* = Unit Under Calibration.

-o0o-

JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd.Watthapra, Bangkokyai,
Bangkok 10600(Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Temperature measurement laboratory
Calibration services department.

NSC – TISI – TIS 17025
CALIBRATION 0367

REVIEW BY ..... Narakorn P.

APPROVED BY.....

NEXT CAL DATE..... 06/06/26

CERTIFICATE OF CALIBRATION

Certificate No. : CDT-089-68

MEASUREMENT ITEM	: Heat Stress Monitor
MANUFACTURER	: Delta OHM
MODEL/TYPE	: HD32.2
SERIAL NUMBER	: 15006302
ID NUMBER	: BKK_FS0663
CONDITION AS-RECEIVED	: Used item
CUSTOMER	: ALS laboratory group (thailand) Co., Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250 Thailand.
RECEIVED DATE	: 15 May 2025
MEASUREMENT DATE	: 06 Jun 2025
ISSUE DATE	: 10 Jun 2025

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH

NOTED: *The certificate is valid only to the item calibrated on date and place of calibration.*

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:
The temperature calibration was done by In-House calibration method as WI-CL-001 according to comparison method with standard digital temperature indicator and standard temperature probe. The temperature scale use was based on ITS-90.

Traceability:
The measurement results are traceable to the international system of units (SI) through National Institute of Metrology Thailand (NIMT) Certificate number: TT-1013-25, Certificate number: ER-0061-25.

Reference Used During Calibration:
1. Standard Temperature Probe
Model: STS-100 A500, Serial No.: 667682-09, Due date: 9 Apr 2026
2. Digital Temperature Indicator
Model: DTI-1000-A MK II, Serial No.: 671407-00591 Due date: 22 Apr 2026

Uncertainty of Measurement:
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Calibrated by:
☐ Mr. Sorawit Thachalad
☑ Miss Jittraporn Lertsomphol
☐ Miss Ruangrumpai Phoommit

JIRANATEE ASSOCIATES CO.,LTD.

Approved signatory: .....
Mr. Parinya Booncharoen
Calibration Department Manager

Jiranatee Associates Co., Ltd.

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

JIRANATEE ASSOCIATES CO.,LTD.

Result of Calibration: ☑ Without Adjustment ☐ With Adjustment

Calibration Range: 20 °C to 40 °C

Function:

Table 1: This equipment was connected with wet bulb probe Model: HP3201.2, S/N: 22035259.
Dimension: Diameter 3.3 mm. Length 170 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
80	20.057	20.0	-0.1	0.14
80	25.046	25.0	0.0	0.099
80	30.036	30.0	0.0	0.099
80	35.024	35.0	0.0	0.099
80	39.997	40.0	0.0	0.099

Table 2: This equipment was connected with Globe thermometer probe Model: TP3276.2, S/N: 20032620.
Dimension: Diameter 3.3 mm. Length 205 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
110	20.057	20.2	0.1	0.099
110	25.046	25.2	0.2	0.099
110	30.036	30.2	0.2	0.099
110	35.024	35.2	0.2	0.099
110	39.997	40.1	0.1	0.099

Table 3: This equipment was connected with temperature probe Model: TP3207.2, S/N: 15008018.
Dimension: Diameter 14 mm. Length 150 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
75	20.057	20.3	0.2	0.099
75	25.046	25.1	0.1	0.099
75	30.036	30.0	0.0	0.099
75	35.023	34.9	-0.1	0.099
75	39.997	39.8	-0.2	0.099

UUC*: Unit Under Calibration
Remark: The reported uncertainty of measurement is 0.14, based on standard uncertainty multiplied by a coverage factor k=2.14 providing a level of confidence of approximately 95%.

End of Certificate of Calibration

JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co., Ltd.

JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Temperature measurement laboratory
Calibration services department.

NSC – TISI – TIS 17025
CALIBRATION 0367

CERTIFICATE OF CALIBRATION

Certificate No. : **CDT-196-68**

MEASUREMENT ITEM	: Heat Stress Monitor
MANUFACTURER	: Delta OHM
MODEL/TYPE	: HD32.2
SERIAL NUMBER	: 16002004
ID NUMBER	: BKK_FS0681
CONDITION AS-RECEIVED	: Used item
CUSTOMER	: ALS laboratory group (thailand) Co., Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250 Thailand.
RECEIVED DATE	: 12 Nov 2025
MEASUREMENT DATE	: 19 Nov 2025
ISSUE DATE	: 19 Nov 2025

ENVIRONMENTAL CONDITIONS:
Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH

NOTED: *The certificate is valid only to the item calibrated on date and place of calibration.*

TABULATION OF RESULTS:
The table on next page give the measured values.

Calibration procedure:
The temperature calibration was done by In-House calibration method as WI-CL-001 according to comparison method with standard digital temperature indicator and standard temperature probe. The temperature scale use was based on ITS-90.

Traceability:
The measurement results are traceable to the international system of units (SI) through National Institute of Metrology Thailand (NIMT) Certificate number: TT-1013-25, Certificate number: ER-0061-25.

Reference Used During Calibration:
1. Standard Temperature Probe
Model: STS-100 A500, Serial No.: 667682-09, Due date: 9 Apr 2026
2. Digital Temperature Indicator
Model: DTI-1000-A MK II, Serial No.: 671407-00591 Due date: 22 Apr 2026

Uncertainty of Measurement:
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

REVIEW BY ..... Narakorn P.

APPROVED BY.....

NEXT CAL DATE.....18/11/26

JIRANATEE ASSOCIATES CO.,LTD.

Calibrated by:
☐ Mr. Sorawit Thachalad
☑ Miss Jittraporn Lertsomphol
☐ Miss Ruangrumpai Phoommit

Approved signatory: .....
Mr. Parinya Booncharoen
Calibration Department Manager

Jiranatee Associates Co., Ltd.

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

JIRANATEE ASSOCIATES CO.,LTD.

Result of Calibration: ☑ Without Adjustment ☐ With Adjustment

Calibration Range: 10 °C to 45 °C

Function:

Table 1: This equipment was connected with wet bulb probe Model: HP3201.2, S/N: 16008207.
Dimension: Diameter 3.3 mm. Length 170 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
80	10.061	10.1	0.0	0.099
80	20.058	20.0	-0.1	0.099
80	25.054	25.0	-0.1	0.099
80	30.042	30.0	0.0	0.099
80	35.021	35.0	0.0	0.099
80	45.009	44.9	-0.1	0.099

Table 2: This equipment was connected with Globe thermometer probe Model: TP3276.2, S/N: 22035458.
Dimension: Diameter 3.3 mm. Length 205 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
110	10.061	10.1	0.0	0.099
110	20.058	20.1	0.0	0.099
110	25.054	25.0	-0.1	0.099
110	30.042	30.0	0.0	0.099
110	35.021	35.0	0.0	0.099
110	45.009	45.0	0.0	0.099

Table 3: This equipment was connected with temperature probe Model: TP3207.2, S/N: 15008020.
Dimension: Diameter 14 mm. Length 150 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
75	10.061	10.4	0.3	0.099
75	20.058	20.1	0.0	0.099
75	25.054	25.0	-0.1	0.099
75	30.042	30.0	0.0	0.099
75	35.021	34.9	-0.1	0.099
75	45.009	44.8	-0.2	0.099

UUC*: Unit Under Calibration

End of Certificate of Calibration

JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd.

JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Temperature measurement laboratory
Calibration services department.

NSC – TISI – TIS 17025
CALIBRATION 0367

CERTIFICATE OF CALIBRATION

Certificate No. : **CDT-194-68**

MEASUREMENT ITEM	: Heat Stress Monitor
MANUFACTURER	: Delta OHM
MODEL/TYPE	: HD32.2
SERIAL NUMBER	: 15006708
ID NUMBER	: BKK_FS0671
CONDITION AS-RECEIVED	: Used item
CUSTOMER	: ALS laboratory group (thailand) Co., Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250 Thailand.
RECEIVED DATE	: 12 Nov 2025
MEASUREMENT DATE	: 19 Nov 2025
ISSUE DATE	: 19 Nov 2025

ENVIRONMENTAL CONDITIONS:
Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH

NOTED: *The certificate is valid only to the item calibrated on date and place of calibration.*

TABULATION OF RESULTS:
The table on next page give the measured values.

REVIEW BY ..... Warakorn P.

APPROVED BY.....

NEXT CAL DATE.....18/11/26.....

Calibration procedure:
The temperature calibration was done by In-House calibration method as WI-CL-001 according to comparison method with standard digital temperature indicator and standard temperature probe. The temperature scale use was based on ITS-90.

Traceability:
The measurement results are traceable to the international system of units (SI) through National Institute of Metrology Thailand (NIMT) Certificate number: TT-1013-25, Certificate number: ER-0061-25.

Reference Used During Calibration:
1. Standard Temperature Probe
Model: STS-100 A500, Serial No.: 667682-09, Due date: 9 Apr 2026
2. Digital Temperature Indicator
Model: DTI-1000-A MK II, Serial No.: 671407-00591 Due date: 22 Apr 2026

Uncertainty of Measurement:
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Calibrated by:
☐ Mr. Sorawit Thachalad
☑ Miss Jittraporn Lertsomphol
☐ Miss Ruangrumpai Phoommit

JIRANATEE ASSOCIATES CO.,LTD.

Approved signatory: .....
Mr. Parinya Booncharoen
Calibration Department Manager

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

JNAC
JIRANATEE ASSOCIATES CO.,LTD.

Continuation of Certificate of Calibration Number CDT-194-68

Result of Calibration: ☑ Without Adjustment ☐ With Adjustment

Calibration Range: 10 °C to 45 °C

Function:

Table 1: This equipment was connected with wet bulb probe Model: HP3201.2, S/N: 15015843.
Dimension: Diameter 3.3 mm. Length 170 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
80	10.066	10.1	0.0	0.099
80	20.059	20.1	0.0	0.099
80	25.054	25.1	0.0	0.099
80	30.044	30.1	0.1	0.099
80	35.029	35.1	0.1	0.099
80	45.010	45.1	0.1	0.099

Table 2: This equipment was connected with Globe thermometer probe Model: TP3276.2, S/N: 22035454.
Dimension: Diameter 3.3 mm. Length 205 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
110	10.066	10.1	0.0	0.099
110	20.059	20.0	-0.1	0.099
110	25.054	25.0	-0.1	0.099
110	30.044	30.1	0.1	0.099
110	35.029	35.1	0.1	0.099
110	45.010	45.1	0.1	0.099

Table 3: This equipment was connected with temperature probe Model: TP3207.2, S/N: 16009383.
Dimension: Diameter 14 mm. Length 150 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
75	10.066	10.4	0.3	0.099
75	20.059	20.0	-0.1	0.099
75	25.054	25.0	-0.1	0.099
75	30.044	29.9	-0.1	0.099
75	35.029	34.8	-0.2	0.099
75	45.010	44.8	-0.2	0.099

UUC*: Unit Under Calibration

End of Certificate of Calibration

JNAC
JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd.

JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Temperature measurement laboratory
Calibration services department.

NSC – TISI – TIS 17025
CALIBRATION 0367

CERTIFICATE OF CALIBRATION

Certificate No. : **CDT-101-68**

MEASUREMENT ITEM	: Heat Stress Monitor
MANUFACTURER	: Delta OHM
MODEL/TYPE	: HD32.2
SERIAL NUMBER	: 22016393
ID NUMBER	: CHM_FS0099
CONDITION AS-RECEIVED	: Used item
CUSTOMER	: ALS laboratory group (thailand) Co., Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250 Thailand.
RECEIVED DATE	: 19 Jun 2025
MEASUREMENT DATE	: 02 Jul 2025
ISSUE DATE	: 04 Jul 2025

ENVIRONMENTAL CONDITIONS:
Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	˚C
Relative Humidity	: 55.0 ± 15.0	%RH

NOTED: *The certificate is valid only to the item calibrated on date and place of calibration.*

TABULATION OF RESULTS:
The table on next page give the measured values.

REVIEW BY ..... Narakorn P.

APPROVED BY.....

NEXT CAL DATE..... 02/07/26

Calibration procedure:
The temperature calibration was done by In-House calibration method as WI-CL-001 according to comparison method with standard digital temperature indicator and standard temperature probe. The temperature scale use was based on ITS-90.

Traceability:
The measurement results are traceable to the international system of units (SI) through National Institute of Metrology Thailand (NIMT) Certificate number: TT-1013-25, Certificate number: ER-0061-25.

Reference Used During Calibration:
1. Standard Temperature Probe
Model: STS-100 A500, Serial No.: 667682-09,
Due date: 9 Apr 2026
2. Digital Temperature Indicator
Model: DTI-1000-A MK II, Serial No.: 671407-00591 Due date: 22 Apr 2026

Uncertainty of Measurement:
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Calibrated by:
☐ Mr. Sorawit Thachalad
☑ Miss Jittraporn Lertsomphol
☐ Miss Ruangrumpai Phoommit

JNAC JIRANATEE ASSOCIATES CO.,LTD.

Approved signatory: .....
Mr. Parinya Booncharoen
Calibration Department Manager

Jiranatee Associates Co., Ltd.

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

JIRANATEE ASSOCIATES CO.,LTD.

Continuation of Certificate of Calibration Number CDT-101-68

Result of Calibration: ☑ Without Adjustment ☐ With Adjustment

Calibration Range: 20 °C to 40 °C

Function:

Table 1: This equipment was connected with wet bulb probe Model: HP3201.2, S/N: 22025584. Dimension: Diameter 3.3 mm. Length 170 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
80	20.061	20.1	0.0	0.099
80	25.044	25.0	0.0	0.099
80	30.032	30.0	0.0	0.099
80	35.019	35.0	0.0	0.099
80	40.005	40.0	0.0	0.099

Table 2: This equipment was connected with Globe thermometer probe Model: TP3276.2, S/N: 22023933. Dimension: Diameter 3.3 mm. Length 205 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
110	20.061	20.1	0.0	0.099
110	25.044	25.1	0.1	0.099
110	30.031	30.1	0.1	0.099
110	35.019	35.1	0.1	0.099
110	40.005	40.0	0.0	0.099

Table 3: This equipment was connected with temperature probe Model: TP3207.2, S/N: 22025050. Dimension: Diameter 14 mm. Length 150 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
75	20.061	20.1	0.0	0.099
75	25.043	25.0	0.0	0.099
75	30.031	29.9	-0.1	0.099
75	35.019	34.8	-0.2	0.099
75	40.005	39.7	-0.3	0.099

UUC*: Unit Under Calibration

Jiranatee Associates Co.,Ltd.

End of Certificate of Calibration

JIRANATEE ASSOCIATES CO.,LTD.

JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Temperature measurement laboratory
Calibration services department.

NSC – TISI – TIS 17025
CALIBRATION 0367

CERTIFICATE OF CALIBRATION

Certificate No. : **CDT-100-68**

MEASUREMENT ITEM	: Heat Stress Monitor
MANUFACTURER	: Delta OHM
MODEL/TYPE	: HD32.2
SERIAL NUMBER	: 22016392
ID NUMBER	: CHM_FS0098
CONDITION AS-RECEIVED	: Used item
CUSTOMER	: ALS laboratory group (thailand) Co., Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250 Thailand.
RECEIVED DATE	: 19 Jun 2025
MEASUREMENT DATE	: 02 Jul 2025
ISSUE DATE	: 04 Jul 2025

ENVIRONMENTAL CONDITIONS:
Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	˚C
Relative Humidity	: 55.0 ± 15.0	%RH

NOTED: *The certificate is valid only to the item calibrated on date and place of calibration.*

TABULATION OF RESULTS:
The table on next page give the measured values.

Calibration procedure:
The temperature calibration was done by In-House calibration method as WI-CL-001 according to comparison method with standard digital temperature indicator and standard temperature probe. The temperature scale use was based on ITS-90.

Traceability:
The measurement results are traceable to the international system of units (SI) through National Institute of Metrology Thailand (NIMT) Certificate number: TT-1013-25, Certificate number: ER-0061-25.

Reference Used During Calibration:
1. Standard Temperature Probe
Model: STS-100 A500, Serial No.: 667682-09, Due date: 9 Apr 2026
2. Digital Temperature Indicator
Model: DTI-1000-A MK II, Serial No.: 671407-00591 Due date: 22 Apr 2026

Uncertainty of Measurement:
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

REVIEW BY ..... Narakorn P.

APPROVED BY.....

NEXT CAL DATE..... 02/07/26

Calibrated by:
☐ Mr. Sorawit Thachalad
☑ Miss Jittraporn Lertsomphol
☐ Miss Ruangrumpai Phoommit

JIRANATEE ASSOCIATES CO.,LTD.

Approved signatory: .....
Mr. Parinya Booncharoen
Calibration Department Manager

Jiranatee Associates Co., Ltd.

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

JIRANATEE ASSOCIATES CO.,LTD.

Continuation of Certificate of Calibration Number CDT-100-68

Result of Calibration: ☑ Without Adjustment ☐ With Adjustment

Calibration Range: 20 °C to 40 °C

Function:

Table 1: This equipment was connected with wet bulb probe Model: HP3201.2, S/N: 22025582. Dimension: Diameter 3.3 mm. Length 170 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
80	20.069	19.9	-0.2	0.099
80	25.042	24.9	-0.1	0.099
80	30.035	29.9	-0.1	0.099
80	35.003	34.8	-0.2	0.099
80	39.994	39.8	-0.2	0.099

Table 2: This equipment was connected with Globe thermometer probe Model: TP3276.2, S/N: 22023952. Dimension: Diameter 3.3 mm. Length 205 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
110	20.069	20.1	0.0	0.099
110	25.042	25.1	0.1	0.099
110	30.035	30.1	0.1	0.099
110	35.003	35.1	0.1	0.099
110	39.994	40.1	0.1	0.099

Table 3: This equipment was connected with temperature probe Model: TP3207.2, S/N: 22025057. Dimension: Diameter 14 mm. Length 150 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
75	20.069	20.2	0.1	0.099
75	25.042	25.1	0.1	0.099
75	30.035	30.1	0.1	0.099
75	35.003	35.0	0.0	0.099
75	39.994	39.9	-0.1	0.099

UUC*: Unit Under Calibration

Jiranatee Associates Co., Ltd.

End of Certificate of Calibration

JIRANATEE ASSOCIATES CO.,LTD.

JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Temperature measurement laboratory
Calibration services department.

NSC – TISI – TIS 17025
CALIBRATION 0367

CERTIFICATE OF CALIBRATION

Certificate No. : **CDT-106-68**

MEASUREMENT ITEM	: Heat Stress Monitor
MANUFACTURER	: Delta OHM
MODEL/TYPE	: HD32.2
SERIAL NUMBER	: 22016398
ID NUMBER	: CHM_FS0104
CONDITION AS-RECEIVED	: Used item
CUSTOMER	: ALS laboratory group (thailand) Co., Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250 Thailand.
RECEIVED DATE	: 19 Jun 2025
MEASUREMENT DATE	: 03 Jul 2025
ISSUE DATE	: 04 Jul 2025

ENVIRONMENTAL CONDITIONS:
Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH

NOTED: *The certificate is valid only to the item calibrated on date and place of calibration.*

TABULATION OF RESULTS:
The table on next page give the measured values.

Calibration procedure:
The temperature calibration was done by In-House calibration method as WI-CL-001 according to comparison method with standard digital temperature indicator and standard temperature probe. The temperature scale use was based on ITS-90.

Traceability:
The measurement results are traceable to the international system of units (SI) through National Institute of Metrology Thailand (NIMT) Certificate number: TT-1013-25, Certificate number: ER-0061-25.

Reference Used During Calibration:
1. Standard Temperature Probe
Model: STS-100 A500, Serial No.: 667682-09, Due date: 9 Apr 2026
2. Digital Temperature Indicator
Model: DTI-1000-A MK II, Serial No.: 671407-00591 Due date: 22 Apr 2026

Uncertainty of Measurement:
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

REVIEW BY ..... Narakorn P.

APPROVED BY.....

NEXT CAL DATE..... 02/07/26

Calibrated by:
☐ Mr. Sorawit Thachalad
☑ Miss Jittraporn Lertsomphol
☐ Miss Ruangrumpai Phoommit

Approved signatory: .....
Mr. Parinya Booncharoen
Calibration Department Manager

Jiranatee Associates Co., Ltd.

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

JIRANATEE ASSOCIATES CO.,LTD.

Continuation of Certificate of Calibration Number CDT-106-68

Result of Calibration: ☑ Without Adjustment ☐ With Adjustment

Calibration Range: 20 °C to 40 °C

Function:

Table 1: This equipment was connected with wet bulb probe Model: HP3201.2, S/N: 22025581. Dimension: Diameter 3.3 mm. Length 170 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
80	20.048	20.0	0.0	0.099
80	25.053	25.0	-0.1	0.099
80	30.035	29.9	-0.1	0.099
80	35.022	34.9	-0.1	0.099
80	40.002	39.9	-0.1	0.099

Table 2: This equipment was connected with Globe thermometer probe Model: TP3276.2, S/N: 22023957. Dimension: Diameter 3.3 mm. Length 205 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
110	20.048	20.1	0.0	0.14
110	25.053	25.1	0.0	0.14
110	30.035	30.0	0.0	0.099
110	35.022	35.0	0.0	0.099
110	40.002	40.0	0.0	0.099

Table 3: This equipment was connected with temperature probe Model: TP3207.2, S/N: 22025038. Dimension: Diameter 14 mm. Length 150 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
75	20.048	20.1	0.1	0.099
75	25.053	25.0	-0.1	0.099
75	30.035	29.9	-0.1	0.099
75	35.022	34.8	-0.2	0.099
75	40.000	39.7	-0.3	0.099

UUC*: Unit Under Calibration

Remark: The reported uncertainty of measurement is 0.14, based on standard uncertainty multiplied by a coverage factor k=2.14 providing a level of confidence of approximately 95%.

End of Certificate of Calibration

JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co., Ltd.

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Certificate of Calibration

Certificate No. : 25T1455
Page : 1 of 2

Equipment : Digital Thermometer With Sensor
Manufacturer: Testo
Model : 106
Serial No.: 83638005/0122
ID No.: BKK_LG0059
Condition As-Received: Used Item
Received Date: 22 August 2025
Calibration Date: 05 September 2025 to 09 September 2025
Reference: 2508-0752DSC
Ambient Temperature: (25 ± 3) °C
Relative Humidity: (50 ± 20) %

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

Submitted by: ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand

Procedure used: Calibration were conducted using in-house calibration procedure CP-T01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into liquid bath temperature controller.
The temperature scale used was based on ITS-90.

Condition of this result of calibration

1.Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Black Stack Thermometer	1560	8C454	25I625	06 Jun 2026
2) PRT Scanner Module	2562	A01303	25I625	06 Jun 2026
3) Industrial Platinum Resistance Thermometer	5627-12	571971	25I625	06 Jun 2026

2.The certificate is valid only to the item calibrated on date and place of calibration.

3.This measurement result is traceable to the International System of Unit maintained through:-

-Technology Promotion Association (Thailand-Japan), NSC-ONSC Accredited No. Calibration 0008

REVIEW BY Chayathron P.
APPROVED BY Wanakorn P.
NEXT CAL DATE 05/09/26

Calibrated by : Sitthinon Poomai
Issue Date : 11 September 2025

Approved Signatory :
[ ] Phalinee Prabpaipal
[ ] Chatchawan Khunpiluek
[✓] Wanlop Larpkern

Result of Calibration:- Without Adjustment

Function: Temperature measurement

Dimension of probe : Diameter 3 mm, Length 55 mm Sheath material : Stainless Steel

Immersion Depth (mm)	Standard Temperature (℃)	UUC* Reading (℃)	Error (℃)	Uncertainty of Measurement (±℃)
50	25.0062	25.0	-0.0062	0.12
50	45.0015	45.0	-0.0015	0.12

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95%.

-o0o-

Agilent Technologies

Agilent Technologies (Thailand) Limited
U CHU LIANG BLDG. 22/F UNIT A,D
968 RAMA 4 ROAD, SILOM, BANGRAK
Bangkok 10500 Thailand

Tel. +662 637 6363
Fax: +662 632 4334
Email: ccc-smt@agilent.com
Website: www.agilent.com/chem

Customer Contact:
ALS Laboratory Group (Thailand) Co Ltd Head Office

104 Phatthanakan 40 Phatthanakan Rd Khwaeng Phatthanakan Khet Suan

TAX ID : 0105540004859

Chanattagarn.lmchom@alsglobal.com
27603068

Invoice To:
ALS Laboratory Group (Thailand) Co Ltd Head Office

104 Phatthanakan 40 Phatthanakan Rd Khwaeng Phatthanakan Khet Suan

SERVICE REPORT

Customer Purchase Order Number:	**Customer Number:** 70371013
Service Request:	**Service Request Date:**
Service Order: 6007607368	**Service Confirmation:** 6906615981

Delivery Site:
ALS Laboratory Group (Thailand) Co Ltd Head Office

104 Phatthanakan 40 Phatthanakan Rd Khwaeng Phatthanakan Khet Suan

Location:
Room
Bldg
Lab
Dept

Direct Inquiries to:
Contact Name: Customer Contact Center
Contact E-mail: ccc-smt@agilent.com
Contact Telephone: +662 637 6363
Contact Fax: +662 632 4334

REVIEW BY Andhalee K.
APPROVED BY Samitree N.
NEXT CAL. DATE 02/10/2026

products | applications | software | services

Learn more about Agilent's Special Offers, Products, Services and our full range of laboratory productivity solutions optimized for your applications and workflows. Visit us at **www.agilent.com/chem**

Service Instrument:

Model Number	Model Description	Serial Number	System Handle	Parent Asset
SYS-IM-7900	ICPMS 7900 System			
G8410A	SPS 4 Autosampler	AU15430722	ICP MS 7900	SYS-IM-7900
G8411A	ISIS 3 for Agilent 7850/7900/8900	JP15510227	ICP MS 7900	SYS-IM-7900
G3292A	PSC 6106T Chiller	2U15A1948	ICP MS 7900	SYS-IM-7900
G8403A	Agilent 7900 ICP-MS	JP15471169	ICP MS 7900	SYS-IM-7900

Service Items:

Item	Service/Part #	Description	Qty	Entitlement	Service Start	Service End
1000	EOQ	Enterprise Operational Qualification	1.00	Agreement Entitlement - 100 % covered	03.10.2025	03.10.2025
1010	5185-5850	ICP-MS Checkout Solutions	1.00	Agreement Entitlement - 100 % covered		

Additional Information:

Service Information:

Problem Description: *WU-EOQ-IM-7900-5001413366		
Service Provided: Perform OQ hardware control. Test logon , tune , BG and stability. Test OQ control of instrument ICPMS=BKK_EL0043 After done the instrument test all pass.		
Service Overview Code: Reason Code: Scheduled Service Diagnosis Code: Scheduled Service Resolution Code: Scheduled Service		
Reported Hours: 5.0	**Travel Hours:** 1.5	
Customer Field Service Representative Name: **Panthep Kurasathain**	**Customer Field Service Representative Signature:**	**Date:** **03 Oct 2025**
Customer Name: **Anchalee Khamjan**	**Customer Signature:** Anchalee K.	**Date:** **03 Oct 2025**
Additional Comments:		

Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No. T250355

Certificate of Calibration

Equipment	:	HEATING BLOCK
Manufacturer	:	Environmental Express
Model	:	SC 196
Serial No.	:	6974CECW3285
Customer Code	:	BKK_EL0054
ID No.	:	T5306A3
Customer	:	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250
Customer Location	:	Acid Digestion Lab
Date of Receipt	:	26 February 2025
Calibrated By	:	Atiphong Rongrat (Technician)
Approved By	:	_____ / Boonchai Suriyawong (Site Calibration Manager)
Date of Issue	:	17 MAR 2025

REVIEW BY Tattaporn C.
APPROVED BY Sawitr N.
NEXT CAL. DATE ~~04/09/26~~ แก้ไขปี พ.ศ. Sawitr N.
04/09/26

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Calibration Report

Equipment : **HEATING BLOCK**
Date of Calibration : **4 March 2025**
Environment : **Temperature : 24.4-24.9 °C**
Line Voltage : 221.6-226.3 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert nine standard thermocouples type T into its chamber , the other one standard thermocouples type T use for ambient temperature measurement . The calibration was done in according to WI-T20.
   All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .
2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN221-TN230	T240712	19 April 2025
TC	TYPE T	TN231-TN240	T240712	19 April 2025
TC	TYPE T	TN241-TN250	T240401	16 March 2025
TC	TYPE T	TN251-TN260	T240401	16 March 2025
DATA LOGGER	34970A	T193	T240401	16 March 2025

3. This certificate is traceable to :
   National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)
4. Condition of calibrated item : good
   Equipment Description :
   Time Constant 2 Hour 40 Minute At 95 °C
   Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
   ☐ Close
   ☒ Not Available
5. Adjustment :
   ( ) without adjustment (X) after adjustment

Approved By. _____

Metrological Center


SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Calibration Report

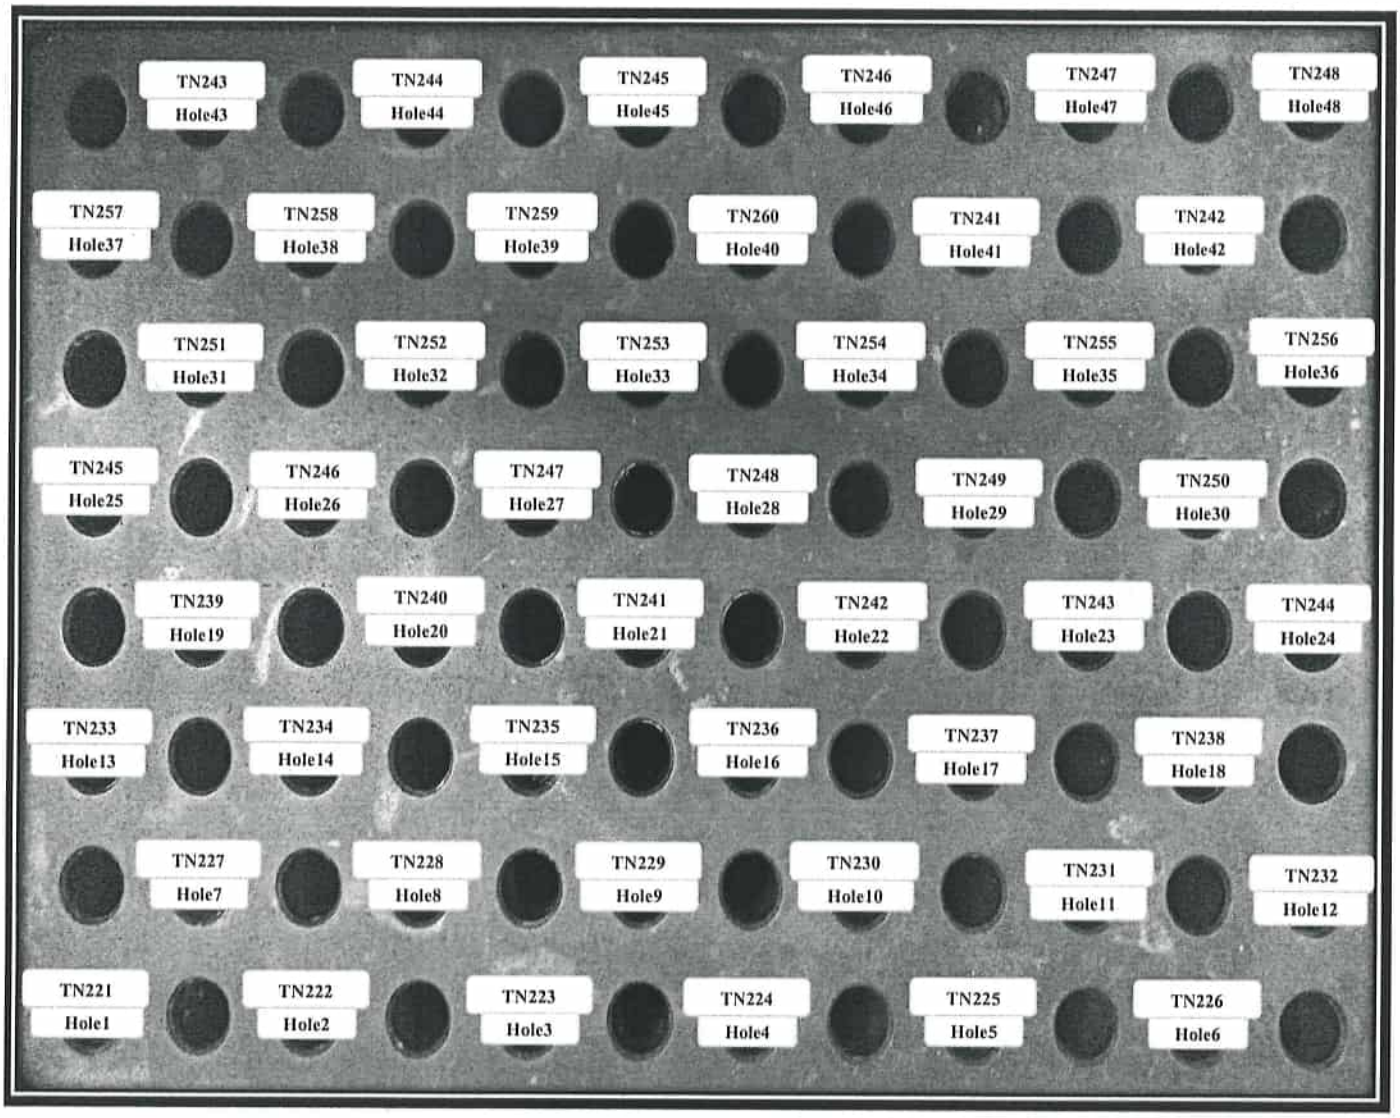

FRONT CONTROL

Approved By. _____

Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Calibration Report

Measurement Results

Calibration Point		Average Standard Reading at each position (°C)					
R1 Hole1-Hole6		**TN221**	**TN222**	**TN223**	**TN224**	**TN225**	**TN226**
CAL POINT	Max	94.85	95.37	95.03	95.25	95.52	94.75
95	Min	94.17	94.66	94.38	94.63	94.87	94.12
	Average	94.51	95.02	94.70	94.94	95.20	94.43
R2 Hole7-Hole12		**TN227**	**TN228**	**TN229**	**TN230**	**TN231**	**TN232**
	Max	94.71	94.56	94.79	95.32	95.44	95.06
	Min	94.05	93.88	94.10	94.65	94.90	94.65
	Average	94.38	94.22	94.44	94.99	95.17	94.85
R3 Hole13-Hole18		**TN233**	**TN234**	**TN235**	**TN236**	**TN237**	**TN238**
	Max	95.26	95.43	95.40	95.71	95.41	95.06
	Min	94.54	94.64	94.71	95.10	94.86	94.42
	Average	94.90	95.03	95.06	95.41	95.13	94.74
R4 Hole19-Hole24		**TN239**	**TN240**	**TN241**	**TN242**	**TN243**	**TN244**
	Max	95.13	95.06	95.68	96.16	95.35	95.80
	Min	94.39	94.43	94.86	95.51	94.88	95.12
	Average	94.76	94.75	95.27	95.83	95.12	95.46
R5 Hole25-Hole30		**TN245**	**TN246**	**TN247**	**TN248**	**TN249**	**TN250**
	Max	94.95	95.81	95.39	95.82	95.66	95.66
	Min	94.47	95.03	94.67	94.99	94.84	94.87
	Average	94.71	95.42	95.03	95.41	95.25	95.27
R6 Hole31-Hole36		**TN251**	**TN252**	**TN253**	**TN254**	**TN255**	**TN256**
	Max	96.07	95.34	96.28	95.39	94.95	95.12
	Min	95.28	94.55	95.51	94.62	94.13	94.35
	Average	95.67	94.95	95.90	95.00	94.54	94.73
R7 Hole37-Hole42		**TN257**	**TN258**	**TN259**	**TN260**	**TN241**	**TN242**
	Max	95.15	95.63	96.11	95.09	95.34	95.51
	Min	94.38	94.88	95.32	94.28	94.54	94.72
	Average	94.76	95.25	95.71	94.69	94.94	95.11
R8 Hole43-Hole48		**TN243**	**TN244**	**TN245**	**TN246**	**TN247**	**TN248**
	Max	95.84	95.87	95.44	95.72	95.65	95.75
	Min	95.06	95.10	94.60	94.95	94.87	94.98
	Average	95.45	95.48	95.02	95.34	95.26	95.36

Approved By.

Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Calibration Report

Measurement Results

Calibration Point		Average Standard Reading at each position (°C)					
R1 Hole1-Hole6		**TN221**	**TN222**	**TN223**	**TN224**	**TN225**	**TN226**
CAL POINT	Max	104.48	104.40	104.60	105.27	105.24	105.19
105	Min	104.15	104.02	104.25	104.94	104.91	104.93
	Average	104.32	104.21	104.42	105.10	105.08	105.06
R2 Hole7-Hole12		**TN227**	**TN228**	**TN229**	**TN230**	**TN231**	**TN232**
	Max	105.20	105.45	105.58	105.96	105.81	106.03
	Min	104.92	105.14	105.29	105.64	105.53	105.79
	Average	105.06	105.29	105.43	105.80	105.67	105.91
R3 Hole13-Hole18		**TN233**	**TN234**	**TN235**	**TN236**	**TN237**	**TN238**
	Max	106.09	106.14	105.83	106.25	105.97	105.88
	Min	105.80	105.89	105.57	106.00	105.69	105.65
	Average	105.94	106.01	105.70	106.13	105.83	105.77
R4 Hole19-Hole24		**TN239**	**TN240**	**TN241**	**TN242**	**TN243**	**TN244**
	Max	105.87	105.75	105.30	105.07	105.22	105.66
	Min	105.62	105.52	105.13	104.90	105.05	105.49
	Average	105.74	105.63	105.21	104.98	105.14	105.57
R5 Hole25-Hole30		**TN245**	**TN246**	**TN247**	**TN248**	**TN249**	**TN250**
	Max	105.62	105.54	105.52	105.75	105.97	105.69
	Min	105.45	105.35	105.31	105.57	105.81	105.49
	Average	105.53	105.44	105.41	105.66	105.89	105.59
R6 Hole31-Hole36		**TN251**	**TN252**	**TN253**	**TN254**	**TN255**	**TN256**
	Max	106.19	106.34	106.47	105.96	105.76	105.35
	Min	106.02	106.16	106.31	105.77	105.58	105.18
	Average	106.10	106.25	106.39	105.87	105.67	105.27
R7 Hole37-Hole42		**TN257**	**TN258**	**TN259**	**TN260**	**TN241**	**TN242**
	Max	106.21	105.59	105.45	105.36	106.08	106.09
	Min	106.04	105.42	105.28	105.20	105.90	105.92
	Average	106.12	105.51	105.37	105.28	105.99	106.00
R8 Hole43-Hole48		**TN243**	**TN244**	**TN245**	**TN246**	**TN247**	**TN248**
	Max	106.54	106.33	105.78	105.38	105.42	105.69
	Min	106.38	106.16	105.60	105.20	105.25	105.52
	Average	106.46	106.25	105.69	105.29	105.33	105.61

Approved By.

Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Calibration Report

Measurement Results:

HEATING BLOCK			Temperature Distribution	
Setting (°C)	Reading (°C)		Stability (±°C)	Uncertainty (±°C)
	Min , Max	Average		
102.0	-	102.0	0.43	0.83
107.0	-	107.0	0.20	0.70

*** The quoted uncertainty exclude " uniformity "**

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By. _____

Metrology Center
SCI ECO Services Company Limited

51 Moo 8, Tubkwang, Kaeng Khoi, Saraburi, Thailand 18260
Bangkok Tel : +668 9205 6851 , +669 81924 0059
Saraburi Tel : +669 8247 2360
Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

NSC-TISI-TIS 17025
CALIBRATION 0244

Certificate No. T250873

Certificate of Calibration

Equipment	:	Chamber (Cooling Room)
Manufacturer	:	KOLDTECH
Model	:	KM 320
Serial No.	:	TBN-1012061/05
Customer Code	:	BKK_EN0167
ID No.	:	T2463A3
Customer	:	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250
Customer Location	:	Laboratory Room
Date of Receipt	:	28 May 2025
Calibrated By	:	Atiphong Rongrat (Technician)
Approved By	:	_____ / Boonchai Suriyawong (Site Calibration Manager)
Date of Issue	:	19 JUN 2025

REVIEW BY ..... Sirilak P.....

APPROVED BY ..... Sirilak P.....

NEXT CAL DATE..... 04/12/26 .....

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Certificate No. T250873

Calibration Report

Equipment : **Chamber (Cooling Room)**
Date of Calibration : **4 June 2025**
Environment : **Temperature : 23.4-24.9 °C**
Line Voltage : 221.4-230.2 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. Thisequipment was calibrated by insert 16 standard thermocouples type T into its chamber , the other one standard thermocouples type T use for ambient temperature measurement . The calibration was done in according to WI-T20 (based on ASTM E145-94 (Reapproved 2001) and AS2853-1986).
   All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .
2. Reference Standard Instrument :


Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN91-TN100	T242036	3 December 2025
TC	TYPE T	TN101-TN110	T242036	3 December 2025
DATA LOGGER	34970A	T121	T242036	3 December 2025

3. This certificate is traceable to :
   National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)
4. Condition of calibrated item : good
   Equipment Description :
   Time Constant 2 Hour 20 Minute At 3 °C
   Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
   ☐ Close
   ☒ Not Available
5. Adjustment :
   (X) without adjustment ( ) after adjustment

Approved By. _____

Certificate No. T250873

Calibration Report

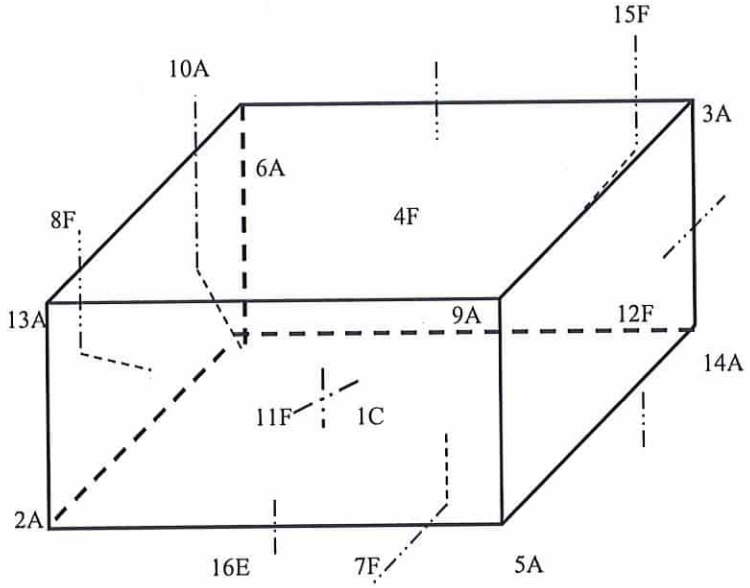

C = Centre , F = Centre of Face , A = Corner , E = Centre of Edge

1C	= TN91	
2A	= TN92	
3A	= TN93	
4F	= TN94	
5A	= TN95	
6A	= TN96	
7F	= TN97	
8F	= TN98	
9A	= TN99	
10A	= TN100	
11F	= TN101	

12F	= TN102
13A	= TN103
14A	= TN104
15F	= TN105
16E	= TN106

Approved By. _____

Metrology Center
SCI ECO Services Company Limited
51 Moo 8, Tubkwang, Kaeng Khoi, Saraburi, Thailand 18260

NSC-TISI-TIS 17025
CALIBRATION 0244

Certificate No. T250873

Calibration Report

Measurement Results

	Average Standard Reading at each position (°C)											
Calibration Point	TN91	TN92	TN93	TN94	TN95	TN96	TN97	TN98	TN99	TN100	TN101	TN102
3.0	2.95	2.92	3.09	2.92	3.16	3.50	3.40	3.03	3.14	2.98	3.44	3.13
	TN103	TN104	TN105	TN106								
	3.19	3.06	3.46	2.92								

Chamber (Cooling Room)			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (±°C)	Uniformity (°C)	Uncertainty (±°C)	Coverage Factor *k*
	Min , Max	Average					
3.0	2.8 , 3.9	3.4	3.14	1.20	1.30	1.90	2.04

The calibration result apply only the above calibrated item.
The result of test was found accurate as shown on date and place of test only.
The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By._____

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Certificate of Calibration

Cert.No.: 25CH1162
Page.: 1 of 3

Equipment :	pH Meter
Manufacturer :	Hach
Model :	HQ411d
Serial No. :	200100031163
ID No. :	BKK_EN0342
Condition As-Received:	Used Item
Received Date :	08 October 2025
Calibration Date :	09 October 2025
Reference :	2510-0271DSC-1
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure :	In - house method : - CP-CH5 by direct measurement with certified reference material (CRM) - CP-CH8 by comparison with temperature standard
Calibrated by :	Walalak Sirithean
Approved by :	Saithip Approved Signatory

REVIEW BY ..... Sinda K .....

APPROVED BY ..... Siriluk P .....

NEXT CAL DATE ..... 09/10/26 .....

( ) Chakrit Waewwanjua
( ) Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 10 October 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Condition of this calibration result

1. Reference Standard Instrument

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1) Ref. Standard Thermometer	4982054	110RC044	25I708	03 July 2026

- This measurement result is traceable to SI throught Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.007	CPA chem	1114384	12 June 2027
pH 6.965	CPA chem	1066667	18 Jan 2026
pH 10.010	CPA chem	1135355	16 Aug 2026

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (±)	Coverage factor *k*
pH Electrode	4.007	3.996	176.6	0.0046	2.00
S/N.: 252063043080	6.965	6.974	1.1	0.0084	2.00
	10.010	9.996	-176.9	0.0070	2.00

Remark - Can not connect the BNC because the plug does not match with the socket.

Calibration Results

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : PHC281
- Serial No. : 252063043080

Dimension of probe

- Length : 103 mm.
- Diameter : 12 mm.
- Immersion Depth : 90 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (± °C)	Coverage factor *k*
25.0	25.001	25.0	-0.001	0.13	2.00

Remark - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Accredited by

NSC-TISI-TIS 17025
Calibration 0426

Calibration certificate

Calibration Certificate No. 25BCI0265

Object	Electronic non-automatic weighing instrument
Manufacturer	Sartorius
Type	MSE224S-100-DU
Serial | QM Ident. no.	27405555 | BKK_EN0003
Customer	ALS Laboratory Group (Thailand)Co., Ltd. 104 Phatthanakarn 40,Phattanakarn Rd.,Khwaeng Phatthanakarn ,Khet Suan Luang,Bangkok 10250
Order no.	265054
Number of pages	4
Date of calibration	17 Jul 2025

This calibration certificate documents the traceability to national standards.

Uncertainties of measurements are taken into account when only statements of compliance are made.

This certificate was prepared by Sartorius Corporation in accordance to the current ISO/IEC 17025:2017 standard and Sartorius Work Instruction (Method) SOP WI 08.

This certificate relate and apply this equipment only.

REVIEW BY ..... Sirida K.....

APPROVED BY ..... Siriluk P.....

NEXT CAL DATE..... 17/07/26 .....

This calibration certificate may not be reproduced other than in full except with the permission of NSC-TISI-TIS-17025 and the issuing laboratory. Calibration certificates without signature are not valid.

The user is obliged to have the object recalibrated at appropriate intervals.

Date of issue	Approval of the Calibration Certificate	Person in charge
17 Jul 2025	Mr. Chonchai Inthana	Chonchai Inthana

Calibration object

Single range instrument

Model	MSE224S-100-DU
Serial Number	27405555
QM Ident. no | Inventory no.	BKK_EN0003 | ---

Maximum capacity (Max. load)	220.0000 g
Measured up to	220.0000 g
Scale interval	0.0001 g

Place of calibration

Address	According to page 1
Department | Cost center	ENVI Department | ---
Building | Floor	--- | 1st Floor.
Room	Laboratory Room.
Maximum temperature variation at place of calibration	5 K

Calibration procedure

EURAMET Calibration Guide No. 18, Version 4.0 (11/2015) - Guidelines on the Calibration of Non-Automatic Weighing Instruments

Test equipment

Test equipment type	Test equipment ID	Valid until
Thermometer	Testo 174(Traceable to Si unit through ENTECH)	11 Nov 2025
Test weight set OIML R111 E2	Certificate No.M2308197S ,E2(Traceable to SI unit through TCS)	23 Aug 2025

Adjustment Status

The measuring device was internally adjusted before the calibration.

Environmental and measuring conditions

Date of calibration	17 Jul 2025
Temperature at place of calibration | Temp. diff. $T_{weights}$ - T_{place}	22.5 °C | 0.7 K
Measuring conditions	The installation site is suitable. The device is level. Balance was loaded up to Max before test.
Comments	Humidity 58.0 %RH.

Measurement results | Measurement uncertainties

Repeatability

Test load (nominal): 10 g | 200 g		
	10 g	**200 g**
1	10.0000 g	200.0000 g
2	10.0000 g	199.9999 g
3	10.0000 g	200.0000 g
4	10.0000 g	200.0000 g
5	10.0001 g	199.9999 g
6	10.0000 g	200.0000 g
7	10.0000 g	200.0000 g
8	10.0001 g	200.0000 g
9	10.0000 g	200.0000 g
10	10.0000 g	199.9999 g
	s = 0.00004 g	s = 0.00005 g

Eccentricity

Test load (nominal):	**100 g**
Center	100.0000 g
Front left	100.0001 g
Back left	100.0000 g
Back right	100.0001 g
Front right	100.0001 g
Maximum deviation from centric loading indication $\lvert\Delta I_{ecc}\rvert_{max}$ = 0.0001 g	

Error of indication

Testload ***L***	**Indication** ***I***	**Error** ***E***	**Expansion factor** ***k***	**Uncertainty** ***U(E)***	**Uncertainty relative** $U_{rel}(E)$
0.0100 g	0.0100 g	0.0000 g	2.00	0.00012 g	1.2 %
0.1000 g	0.1000 g	0.0000 g	2.00	0.00013 g	0.13 %
1.0000 g	1.0000 g	0.0000 g	2.00	0.00013 g	0.013 %
2.0000 g	2.0000 g	0.0000 g	2.00	0.00013 g	0.0065 %
5.0000 g	5.0000 g	0.0000 g	2.00	0.00013 g	0.0026 %
10.0000 g	10.0000 g	0.0000 g	2.00	0.00013 g	0.0013 %
20.0000 g	20.0000 g	0.0000 g	2.00	0.00014 g	0.00068 %
50.0000 g	50.0000 g	0.0000 g	2.00	0.00015 g	0.00029 %
100.0000 g	100.0000 g	0.0000 g	2.00	0.00018 g	0.00018 %
200.0000 g	200.0000 g	0.0000 g	2.00	0.00028 g	0.00014 %
220.0000 g	220.0001 g	0.0001 g	2.00	0.00032 g	0.00015 %
Maximum error of indication		$\lvert E\rvert_{max}$ = 0.0001 g			

$U_{rel}(E)$ is the quotient of $U(E)$ and test load L. The uncertainty of measurement $U(E)$ is valid only if error E is considered. You will find reference notes on the uncertainty of measurement in use under: Appendix to the calibration certificate | Interpretation of measurement results.
Reference note: The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the documented Expansion factor, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

End of calibration certificate


Uncertainty of measurement in use

Device adjusted before measurement	Yes
Temperature deviation considered	1.5 K (isoCAL active)
Temperature coefficient considered	$1 \cdot 10^{-6}$/K
Uncertainty of the weighing result $U_{gl}(W)$	**$U_{gl}(W) = 0.00013\ g + 4.19 \cdot 10^{-6} \cdot R$**

Reference note: The current uncertainty of measurement is calculated by entering of the reading *R* into this formula. In relation to this, there is no need for a correction of the indication error. The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied with an Expansion factor of 2, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

Indication in % from max load	Net indication *R*	Uncertainty $U_{gl}(W)$	Uncertainty relative $U_{gl}(W)_{rel}$
1 %	2.2000 g	0.00014 g	0.0063 %
25 %	55.0000 g	0.00036 g	0.00066 %
50 %	110.0000 g	0.00059 g	0.00054 %
75 %	165.0000 g	0.00082 g	0.00050 %
100 %	220.0000 g	0.0011 g	0.00048 %

Graphic realization of the relative uncertainty of measurement | process accuracy

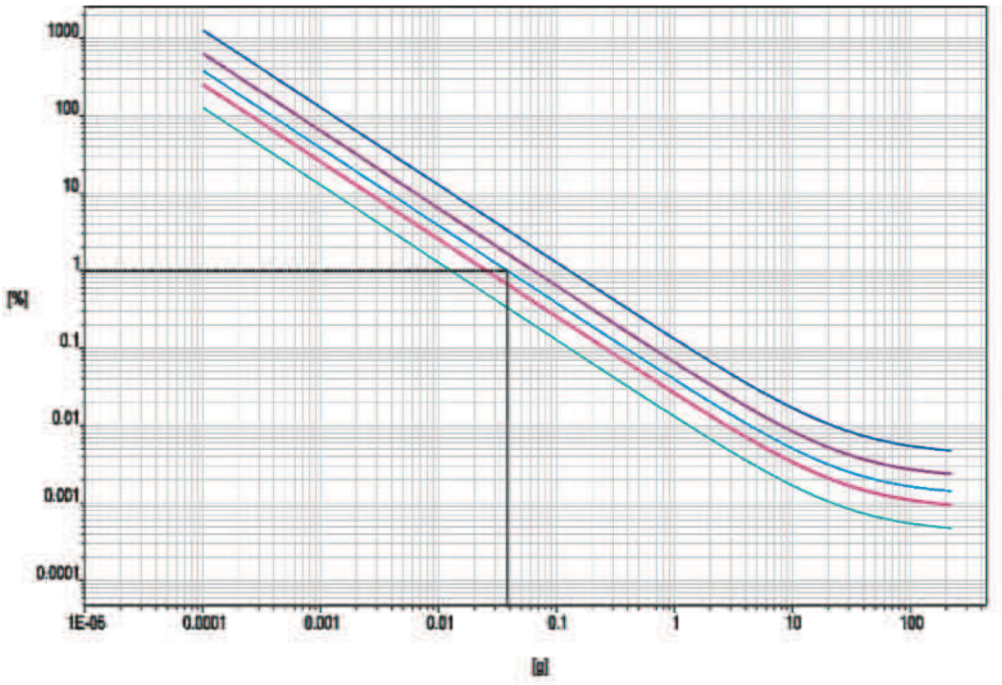

Safety factor
10
5
3
2
1

Displayed example

Process accuracy	1.00 %
Safety factor	3
Minimum sample weight	0.0380 g

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Certificate of Calibration

Cert. No.: 25TM528
Page : 1 of 3

Equipment :	Water Bath
Manufacturer :	Memmert
Model :	WNE 29
Serial No. :	L622.0282
ID No. :	BKK_EN0439

REVIEW BY Sinda K.....
APPROVED BY Siriluk P.....
NEXT CAL DATE.....09/10/26.....

Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand
Location :	Organic Preparation Lab
Received Order :	08 October 2025
Calibration Date :	09 October 2025
Ambient Temperature :	(26 ± 10) °C
Relative Humidity :	(50 ± 30) %
AC Line Voltage :	(220 ± 22) V

Calibrated by : Kunchit Promprat

Approved by :

Approved Signatory

( ) Chakrit Waewwanjua
( ) Ponpan Paipim
(✓) Suwit Imjai

Issue Date : 28 October 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Equipment : Water Bath **Cert. No.:** 25TM528

Condition As-Received : Used Item

Reference : 2510-0042OC-13

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT04 Based on ASTM E715 according to direct measurement method with Data Acquisition which connected with Industrial Platinum Resistance Thermometer (IPRT).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY58041391	25LM20	TPA	08 Feb 2026

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This measurement result is traceable to the International System of Unit maintained through :


Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Heat transfer medium used : Water

	Environmental		AC Voltage Supply
	(°C)	(%R.H.)	(Volt)
Beginning of Calibration	24	63	224
Finished of Calibration	24	58	224

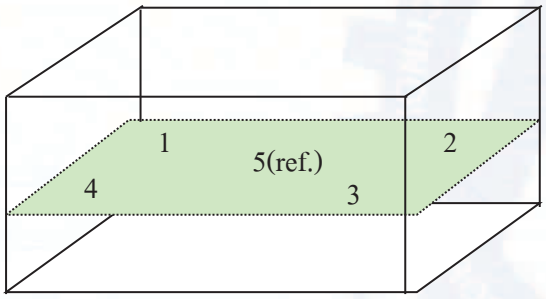

Front

Position :	Ref. Std. ID No.:
1	70RC143
2	70RC144
3	70RC145
4	70RC146
5(ref.)	70RC147

Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2510-0042OC-13
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source

Cert. No.: 25TM528

Calibration point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Average* Standard Reading (°C) Position					Uncertainty (± °C)
			1	2	3	4	5 (ref.)	
85.0	85.0	85.0	84.863	84.748	84.869	84.990	84.966	0.21

Calibration point (°C)	Uniformity (°C)	Stability (± °C)	Coverage Factor *k*
85.0	0.33	0.12	2

Average* : The average of 30 values in each position.
Uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.
Stability : One-half of the greatest maximum difference of measured temperature at any one probe.
UUC* : Unit Under Calibration
Note : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor ***k***, providing a level of confidence of approximately 95 %.

-o0o-

SCG

Metrology Center

SCI ECO Services Company Limited

51 Moo 8, Tubkwang, Kaeng Khoi, Saraburi, Thailand 18260

Bangkok Tel : +668 9205 6851 , +669 81924 0059

Saraburi Tel : +669 8247 2360

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

NSC-TISI-TIS 17025
CALIBRATION 0244

Certificate No. T251785

Certificate of Calibration

Equipment	:	**Chamber (Oven)**
Manufacturer	:	**Memmert**
Model	:	**UF110**
Serial No.	:	**B423.1549**
Customer Code	:	**BKK_EN0425**
ID No.	:	**T4671A5**
Customer	:	**ALS Laboratory Group (Thailand) Co.,Ltd.** **104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,** **Khet Suan Luang, Bangkok 10250**
Customer Location	:	**Oven Room**
Date of Receipt	:	**1 October 2025**
Calibrated By	:	**Sujjar Naknakred (Site Calibration Manager)**
Approved By	:	**Boonchai Suriyawong (Site Calibration Manager)**
Date of Issue	:	10 OCT 2025

REVIEW BY Jinda K.
APPROVED BY Siriluk P.
NEXT CAL. DATE 06/10/26

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

SCG

Metrology Center
SCI ECO Services Company Limited
51 Moo 8, Tubkwang, Kaeng Khoi, Saraburi, Thailand 18260

NSC-TISI-TIS 17025
CALIBRATION 0244

Calibration Report

Equipment : **Chamber (Oven)**
Date of Calibration : **6 October 2025**
Environment : **Temperature : 24.4-25.8 °C**
Line Voltage : 220.5-225.2 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert nine resistance thermometer detectors into its chamber , the other one resistance thermometer detector use for ambient temperature measurement . The calibration was done in according to WI-T20 (based on ASTM E145-94 (Reapproved 2019) and AS2853-1986).
   All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .
2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
RTD	100 ohm	23-(CH1-10)	T250314	6 April 2026
DATA LOGGER	34970A	T195	T250314	6 April 2026

3. This certificate is traceable to :
   National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.
4. Condition of calibrated item : good
   Equipment Description :
   Time Constant 2 Hour 14 Minute At 104 °C
   Fresh Air Damper [X] Open [X] Min [ ] Medium [ ] Max
   [ ] Close
   [ ] Not Available
5. Adjustment :
   ( ) without adjustment (X) after adjustment

Approved By.

SCG

Metrology Center


SCI ECO Services Company Limited

51 Moo 8, Tubkwang, Kaeng Khoi, Saraburi, Thailand 18260

NSC-TISI-TIS 17025
CALIBRATION 0244

Certificate No. T251785

Calibration Report

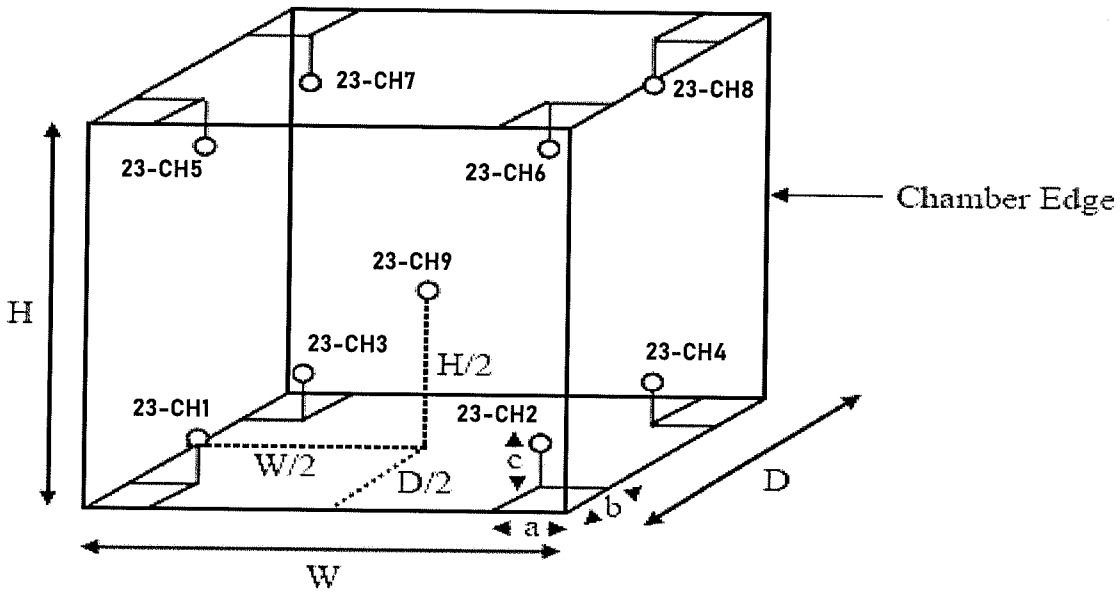

Remark : Internal Dimensions of Chamber : W (Width) = 56 cm. , H (Height) = 48 cm. and D (Depth) = 40 cm.
Size of Installed Standard sensor number 23-CH1 to number 23-CH8 : a = 5 cm. ,b = 5 cm. and c = 5 cm.
Size of Installed Standard sensor number 23-CH9 : W/2 = 56 cm./2 , H/2 = 48 cm./2 and D/2 = 40cm./2

Measurement Results

	Average Standard Reading at each position (°C)								
Calibration Point	23-CH1	23-CH2	23-CH3	23-CH4	23-CH5	23-CH6	23-CH7	23-CH8	23-CH9
104	104.13	103.54	103.92	104.37	104.40	104.51	104.18	103.86	103.80
180	180.05	179.82	179.64	179.52	181.20	180.29	180.19	179.35	179.89

Chamber (Oven)			Temperature Distribution				
Setting °C	Reading (°C)		Average (°C)	Stability (± °C)	Uniformity (°C)	Uncertainty (± °C)	Coverage Factor *k*
	Min , Max	Average					
104.0	-	104.0	104.08	0.28	0.87	0.45	2.00
180.0	180.0 , 180.1	180.0	179.99	0.37	1.49	0.61	2.00

* The quoted uncertainty exclude "uniformity"
The calibration result apply only the above calibrated item.
The result of test was found accurate as shown on date and place of test only.
The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k which for a t-distribution, providing a level of confidence of approximately 95 % .

End of Certificate.

Approved By. _____

DKSH

NSC-TISI-TIS 17025
Calibration 0087

Certificate of Calibration

Equipment:	pH METER	Certificate No.:	C07250317
Manufacturer:	SI Analytics	Job No.:	WO-00076560
Model:	TitroLine 7000	Issued Date:	30 June 2025
Serial No.:	10013826	Due Date:	30 June 2026
ID No.:	BKK_EN0373	Page:	1 of 3
Condition of the item:	Normal		

Customer: ALS Laboratory Group (Thailand) Co., Ltd
104 Soi Pattanakarn 40, Pattanakarn Rd.,
Suan Luang, Bangkok 10250 Thailand

REVIEW BY linda K
APPROVED BY Siriluk P
NEXT CAL. DATE 30/06/26

Environment Condition:	Temperature	22.3	°C	±	0.1	°C
	Relative Humidity	56.3	%	±	0.4	%

Calibration Place: ALS Laboratory Group (Thailand) Co., Ltd.(Wet Chemistry Lab 2)
104 Soi Pattanakarn 40, Pattanakarn Rd.,
Suan Luang, Bangkok 10250 Thailand

Calibration By: Mr.Pongpisut Suebchantha

Calibration Date: 30 June 2025

The Method Used: In house method, CAL-WI-58, base on ASTM E 70-07

Traceability: This certificate is traceable to SI Units, Sample Test is assured through primary meaurement method Harned cell, through CPAchem Ltd. (ISO/IEC 17034) Certificate No. 1100242, 1100244, 1034231 And pH Scale traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through Industrial Foundation Electrical and Electronics Institute Certificate No. CA20240602EA

(Mr. Pongpisut Suebchantha)
Person in charge

(Miss Kaewkan Suradech)
Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with Evaluation of measurement data - Guide to the expression of uncertainty in measurement (JCGM 100).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Calibration Results:

pH Scale

Input	pH Meter Reading			Uncertainty of Measurement (mV)	Coverage Factor (k)
(mV)	(mV)	Error (mV)	(pH)		
414.12	413.9	-0.22	0.000	0.065	2.00
354.96	354.8	-0.16	1.000	0.065	2.00
295.8	295.7	-0.10	2.001	0.065	2.00
236.64	236.6	-0.04	3.001	0.065	2.00
177.48	177.4	-0.08	4.000	0.065	2.00
118.32	118.3	-0.02	5.000	0.065	2.00
59.16	59.1	-0.06	6.000	0.065	2.00
0	0.0	0.00	7.000	0.065	2.00
-59.16	-59.1	0.06	8.000	0.065	2.00
-118.32	-118.3	0.02	9.000	0.065	2.00
-177.48	-177.4	0.08	10.000	0.065	2.00
-236.64	-236.5	0.14	11.000	0.065	2.00
-295.8	-295.6	0.20	12.000	0.065	2.00
-354.96	-354.8	0.16	13.000	0.065	2.00
-414.12	-413.9	0.22	14.000	0.065	2.00

Sample Test Results

Manufacturer: Thermo Scientific **Model:** 8157BNUMD **Electrode Serial No.:** BW1-13563

The three-point calibration using three standard buffer solutions; pH 4.007 , pH 6.988 and pH 10.010

- During calibration, display of pH meter can be adjust to reading; pH 4.007 , pH 6.988 and pH 10.010

Standard Buffer Solution (pH)	Unit Under Calibration (pH)	Difference (pH)	Uncertainty of Measurement (pH)	Coverage Factor (k)
4.007	3.999	-0.008	0.0086	2.28
6.988	6.993	0.005	0.0085	2.00
10.010	10.013	0.003	0.013	2.00

Practical slope and zero point*

The three-point calibration using three standard buffer solutions; pH 4.007 , pH 6.988 and pH 10.010

- During calibration, display of pH meter can be adjust to reading; pH 4.007 , pH 6.988 and pH 10.010

The practical slope of the pH electrode; 57.73 (mV/pH), 97.58%

The zero point of the pH electrode; 6.41 (pH)

* Calibration Marked " Not TISI Accredited " in this Certificate have been included for completeness.

The End of Certificate

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Checklist for pH Meter

Worksheet number: WO-00076560

Instrument type: pH METER Model: TitroLine 7000 S/N: 10013826

Check (receive) 30 Jun 2025		Checklist	Check (send) 30 Jun 2025		Note
Normal	Defective		Normal	Defective	
☑	☐	1. Integrity of the tools	☑	☐	
☑	☐	2. Cleanliness of tools	☑	☐	
☑	☐	3. On-Off Swicth	☑	☐	
☑	☐	4. Keypad	☑	☐	
☑	☐	5. Display, Screen Contrast	☑	☐	
☑	☐	6. Electrode and Connection Cable	☑	☐	
☑	☐	7. Electrode (Level KCl)	☑	☐	
☑	☐	8. Electrode (Dust Protection Hood)	☑	☐	
☑	☐	9. Stand	☑	☐	

Recommend : _____

_____

_____

Mr.Pongpisut Suebchantha

Service Engineer

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

DKSH

NSC-TISI-TIS 17025
Calibration 0087

Certificate of Calibration

Equipment :	Digital Thermometer with Probe	Certificate No. :	C15250720
Manufacturer:	SI Analytics	Job No. :	WO-00076560
Model:	TitroLine 7000	Issued Date :	1 July 2025
Serial No.:	10013826	Due Date:	30 June 2026
ID No.:	BKK_EN0373	Page:	1 of 2
Condition of the item:	Normal		

Customer : ALS Laboratory Group (Thailand) Co., Ltd.
104 Soi Pattanakarn 40, Pattanakarn Rd.,
Suan Luang, Bangkok 10250 Thailand

Environment Condition :

Temperature:	30 °C	±	10 °C
Humidity:	55 %RH	±	25 %RH
Voltage:	220 VAC	±	10 %

Calibration Place : ALS Laboratory Group (Thailand) Co., Ltd.(Wet Chemistry Lab 2)
104 Soi Pattanakarn 40, Pattanakarn Rd.,
Suan Luang, Bangkok 10250 Thailand

Calibration By : Ms. Kaewkan Suradech

Calibration Date : 30 June 2025

The Method used : In house method, CAL-WI-69, by comparison with standard thermometer

Traceability : This certificate is traceable to the International System of Unit maintained by: Quality Reborn Co.,Ltd. (QR)

(Miss Kaewkan Suradech)
Person in charge

(Mr. Tweewong Thaithiang)
Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with Evaluation of measurement data - Guide to the expression of uncertainty in measurement (JCGM 100).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Reference standard equipment:

Equipment	Certificate no	Cal. date	Next Cal. date
Digital Thermometer with Probe	QR24-2043	21 August 2024	21 August 2025

Calibration Results:

Without Adjustment

Sensor Type: RTD Electrode Serial No.: BW1-13563 Channel: -

Diameter (mm): 12 Length (mm): 120 Immersion (mm): 120


Calibrate Point.(°C)	STD. Reading (°C)	UUC. Reading (°C)	Correction of UUC (°C)	Uncertainty (± °C)
25.0	24.994	24.9	0.094	0.20

The End of Certificate

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

C15250720

Without Adjustment

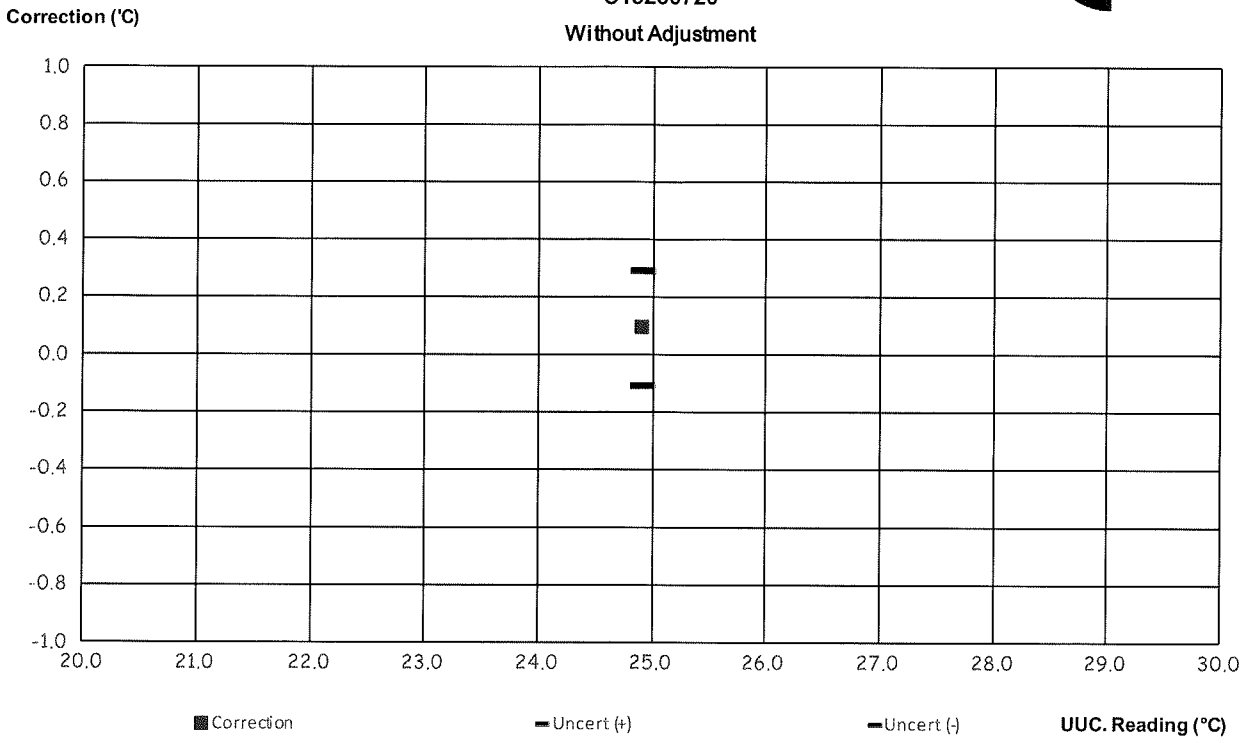

ใบตรวจสอบสภาพเครื่องมือวัดอุณหภูมิ
(Digital Thermometer Checklist)

Equipment : Digital Thermometer with Probe

Certificate No. : C15250720

Serial No. : 10013826

Model : TitroLine 7000

Check Date		รายการตรวจเช็ค (Description)	Check before delivery		หมายเหตุ (Remark)
30-Jun-2025			30-Jun-2025		
Normal	Defective		Normal	Defective	
		General			
☑	☐	1. สายไฟ (Electric wire)	☑	☐	
☑	☐	2. Adaptor / Power supply 220 / 110 VAC	☑	☐	
☑	☐	3. การทำงาน (On/Off Switch)	☑	☐	
☑	☐	4. การทำงาน (Selector Key)	☑	☐	
☑	☐	5. หน้าจอแสดงผล (Display)	☑	☐	
☐	☐	6. แบตเตอรี่ (Battery)	☐	☐	ไม่มี
☑	☐	7. สภาพตัวเครื่อง (Equipment Body)	☑	☐	
☑	☐	8. หัววัดเซ็นเซอร์ (Sensor (In / Ex)	☑	☐	

Note : _____

_____

_____

Ms. Kaewkan Suradech

Service Engineer

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth – in Asia and Beyond.

DKSH

NSC-TISI-TIS 17025
Calibration 0087

Certificate of Calibration

Equipment:	CONDUCTIVITY METER	Certificate No.:	C24250156
Manufacturer:	Thermo Scientific	Job No.:	WO-00076560
Model:	ORION STAR A215	Issued Date:	30 June 2025
Serial No.:	X58031	Due Date:	30 June 2026
ID No.:	BKK_EN0373	Page:	1 of 2
Condition of the item:	Normal		

Customer: ALS Laboratory Group (Thailand) Co., Ltd.
104 Soi Pattanakarn 40, Pattanakarn Rd.,
Suan Luang, Bangkok 10250 Thailand

Environment Condition:

Temperature	22.5	°C	±	0.1	°C
Relative Humidity	56.2	%	±	0.4	%

Calibration Place: ALS Laboratory Group (Thailand) Co., Ltd.(Wet Chemistry Lab 2)
104 Soi Pattanakarn 40, Pattanakarn Rd.,
Suan Luang, Bangkok 10250 Thailand

Calibration By: Mr. Pongpisut Suebchantha

Calibration Date: 30 June 2025

The Method Used: In house method, CAL-WI-49, base on ASTM D 1125-14 and D 5391-14

Traceability: This certificate is traceable to the SI Units maintained by CRM of NIST(SRM) through CPA chem Co., Ltd. (ISO/IEC 17034) Certificate No. 1066607, 1066608, 1066609

(Mr. Pongpisut Suebchantha)
Person in charge

(Miss Kaewkan Suradech)
Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with Evaluation of measurement data - Guide to the expression of uncertainty in measurement (JCGM 100).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Calibration Results:

Manufacturer: Thermo Scientific **Model :** ORION 013005MD **Electrode Serial No.:** YV1-18416

Before Adjustment

Standard Conductivity Solution		Unit Under Calibration Reading		Correction		Coverage Factor (k)	Uncertainty (±)	
84.003	µS/cm	91.88	µS/cm	-7.877	µS/cm	2.00	0.68	µS/cm
1413.1	µS/cm	1445	µS/cm	-31.9	µS/cm	2.00	11	µS/cm
12.881	mS/cm	13.06	mS/cm	-0.179	mS/cm	2.00	0.098	mS/cm

After Adjustment ; at 84.003 µS/cm, 1413.1 µS/cm, 12.880 mS/cm

Standard Conductivity Solution		Unit Under Calibration Reading		Correction		Coverage Factor (k)	Uncertainty (±)	
84.003	µS/cm	84.14	µS/cm	-0.137	µS/cm	2.00	0.68	µS/cm
1413.1	µS/cm	1413	µS/cm	0.1	µS/cm	2.00	11	µS/cm
12.881	mS/cm	12.89	mS/cm	-0.009	mS/cm	2.00	0.098	mS/cm

The End of Certificate

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Checklist for Conductivity Meter

Worksheet number: WO-00076560

Instrument type: Conductivity Meter Model: ORION STAR A215 S/N: X58031

Check (receive) 30 Jun 2025		Checklist	Check (send) 30 Jun 2025		Note
Normal	Defective		Normal	Defective	
☑	☐	1. Integrity of the tools	☑	☐	
☑	☐	2. Cleanliness of tools	☑	☐	
☑	☐	3. On-Off Swicth	☑	☐	
☑	☐	4. Keypad	☑	☐	*
☑	☐	5. Display, Screen Contrast	☑	☐	
☑	☐	6. Electrode and Connection Cable	☑	☐	
☐	☐	7. Electrode (Dust Protection Hood)	☐	☐	
☑	☐	8. Stand	☑	☐	

Recommend : * ปุ่มกดเลื่อน ขึ้น-ลง,ซ้าย-ขวา กดยาก

Mr. Pongpisut Suebchantha

Service Engineer

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

DKSH

NSC-TISI-TIS 17025
Calibration 0087

Certificate of Calibration

Equipment :	Digital Thermometer with Probe	Certificate No. :	C15250721
Manufacturer:	Thermo Scientific	Job No. :	WO-00076560
Model:	ORION STAR A215	Issued Date :	1 July 2025
Serial No.:	X58031	Due Date:	30 June 2026
ID No.:	BKK_EN0373	Page:	1 of 2
Condition of the item:	Normal		

Customer : ALS Laboratory Group (Thailand) Co., Ltd.
104 Soi Pattanakarn 40, Pattanakarn Rd.,
Suan Luang, Bangkok 10250 Thailand

Environment Condition :

Temperature:	30 °C	±	10 °C
Humidity:	55 %RH	±	25 %RH
Voltage:	220 VAC	±	10 %

Calibration Place : ALS Laboratory Group (Thailand) Co., Ltd.(Wet Chemistry Lab 2)
104 Soi Pattanakarn 40, Pattanakarn Rd.,
Suan Luang, Bangkok 10250 Thailand

Calibration By : Ms. Kaewkan Suradech

Calibration Date : 30 June 2025

The Method used : In house method, CAL-WI-69, by comparison with standard thermometer

Traceability : This certificate is traceable to the International System of Unit maintained by: Quality Reborn Co.,Ltd. (QR)

(Miss Kaewkan Suradech)
Person in charge

(Mr. Tweewong Thaithiang)
Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with Evaluation of measurement data - Guide to the expression of uncertainty in measurement (JCGM 100).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Reference standard equipment:

Equipment	Certificate no	Cal. date	Next Cal. date
Digital Thermometer with Probe	QR24-2043	21 August 2024	21 August 2025

Calibration Results:

Without Adjustment


Sensor Type: RTD Electrode Serial No.: YV1-18416 Channel: -

Diameter (mm): 15 Length (mm): 120 Immersion (mm): 120

Calibrate Point.(°C)	STD. Reading (°C)	UUC. Reading (°C)	Correction of UUC (°C)	Uncertainty (± °C)
25.0	24.994	25.0	-0.006	0.20

The End of Certificate

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

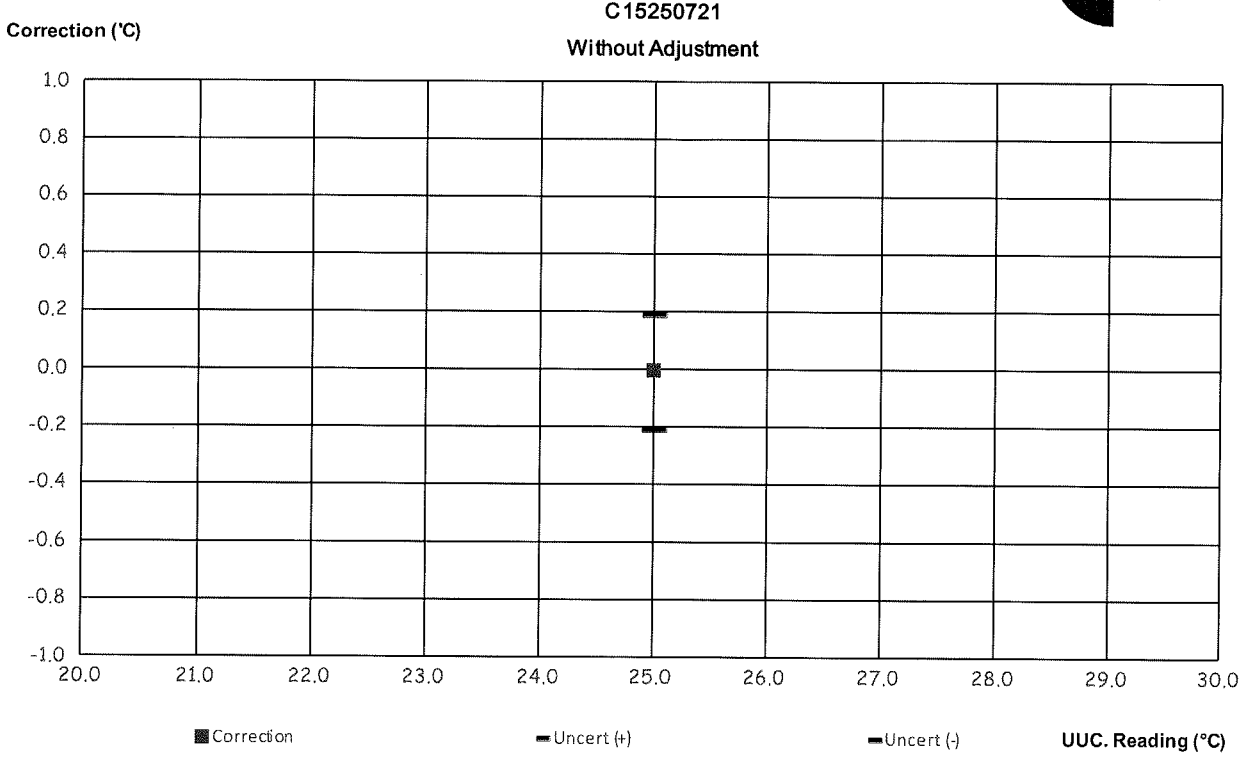
C15250721
Without Adjustment
Correction (°C)
1.0
0.8
0.6
0.4
0.2
0.0
-0.2
-0.4
-0.6
-0.8
-1.0
20.0
21.0
22.0
23.0
24.0
25.0
26.0
27.0
28.0
29.0
30.0
Correction
Uncert (+)
Uncert (-)
UUC. Reading (°C)

ใบตรวจสอบสภาพเครื่องมือวัดอุณหภูมิ
(Digital Thermometer Checklist)

Equipment : Digital Thermometer with Probe

Certificate No. : C15250721

Serial No. : X58031

Model : ORION STAR A215

Check Date		รายการตรวจเช็ค (Description)	Check before delivery		หมายเหตุ (Remark)
30-Jun-2025			30-Jun-2025		
Normal	Defective		Normal	Defective	
		General			
☑	☐	1. สายไฟ (Electric wire)	☑	☐	
☑	☐	2. Adaptor / Power supply 220 / 110 VAC	☑	☐	
☑	☐	3. การทำงาน (On/Off Switch)	☑	☐	
☑	☐	4. การทำงาน (Selector Key)	☑	☐	
☑	☐	5. หน้าจอแสดงผล (Display)	☑	☐	
☐	☐	6. แบตเตอรี่ (Battery)	☐	☐	ไม่มี
☑	☐	7. สภาพตัวเครื่อง (Equipment Body)	☑	☐	
☑	☐	8. หัววัดเซ็นเซอร์ (Sensor (In / Ex)	☑	☐	

Note : _____

_____

_____

Ms. Kaewkan Suradech

Service Engineer

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth – in Asia and Beyond.

Certificate of Calibration

Equipment:	Automatic Titrator	Certificate No.:	C32250030
Manufacturer:	SI Analytics	Job No.:	WO-00076560
Model:	TitroLine 7000	Issued Date:	30 June 2025
Serial No.:	10013826	Due Date:	30 June 2026
ID No.:	BKK_EN0373	Page:	1 of 3
Type of Titration :	Motor - driven		
Condition of the item:	Normal		

Customer: ALS Laboratory Group (Thailand) Co., Ltd.
104 Soi Pattanakarn 40, Pattanakarn Rd.,
Suan Luang, Bangkok 10250 Thailand

Environment Condition:

Temperature	22	°C	±	0.4 °C
Relative Humidity	56	%	±	1.4 %
Atmospheric Pressure	1009	mbar	±	0.4 mbar

Calibration Place: ALS Laboratory Group (Thailand) Co., Ltd. (Wet Chemistry Lab 2)
104 Soi Pattanakarn 40, Pattanakarn Rd.,
Suan Luang, Bangkok 10250 Thailand

Calibration By: Mr. Atachai Ngamchanat

Calibration Date: 30 June 2025

The Method Used: In house method, CAL-WI-57, base on ISO 8655:2002

Traceability: This certificate is traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through DKSH Technology Limited. Certificate No. C01243206

(Mr. Atachai Ngamchanat)
Person in charge

(Miss Kaewkan Suradech)
Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with Evaluation of measurement data - Guide to the expression of uncertainty in measurement (JCGM 100).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Calibration Results:

Nominal Volume 20 ml

Manufacturer: SI Analytics Burettes Model : TZ 3920 Serial No., Nr : 007734

Exchange Unit Model : WA-20 Exchange Unit Serial No. : 10045524 Nominal Vol.: 20 ml

Piston burettes of volumetric apparatus for automatic titrator

Volume (%)	Volume (ml)	Measurement Volume (V_{20}) (ml)	Systematic error (trueness)		Random error (precision)		Measurement Uncertainty (µl)	k
			es (%)	es (µl)	CV (%)	S_r (µl)		
10%	2.0000	1.9997	-0.002	-0.3	0.004	0.7	0.73	2.04
50%	10.0000	10.0076	0.038	7.6	0.003	0.7	1.0	2.00
100%	20.0000	20.0026	0.013	2.6	0.003	0.6	1.5	2.00

ISO 8655-3:2002(E) Table 1 - Maximum permissible errors for motor-driven piston burettes

Nominal volume	Maximum permissible systematic error		Maximum permissible random error	
ml	± %	± µl [a]	± % [b]	± µl [c]
≤1	0.6	6	0.1	1
2	0.5	10	0.1	2
5	0.3	15	0.1	5
10	0.2	20	0.07	7
20	0.2	40	0.07	14
25	0.2	50	0.07	17.5
50	0.2	100	0.05	25
100	0.2	200	0.03	30

a Expressed as the deviation of the mean of tenfold measurement from the nominal volume or from the selected volume (see ISO 8655-6:2002, 8.4)

b Expressed as the coefficient of variation of a tenfold measurement (see ISO 8655-6:2002, 8.5)

c Expressed as the repeatability standard deviation of a tenfold measurement (see ISO 8655-6:2002, 8.5)

The End of Certificate

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Checklist for Automatic Titrator

Worksheet number: WO-00076560

Instrument type: Automatic Titrator Model: TitroLine 7000 S/N: 10013826

Check (receive) 30 Jun 2025		Checklist	Check (send) 30 Jun 2025		Note
Normal	Defective		Normal	Defective	
☑	☐	1. Integrity of the tools	☑	☐	
☑	☐	2. Cleanliness of tools	☑	☐	
☑	☐	3. On-Off Swicth	☑	☐	
☑	☐	4. Keypad	☑	☐	
☑	☐	5. Display, Screen Contrast	☑	☐	
☑	☐	6. Piston Burettes	☑	☐	
☑	☐	7. Function Rinsing and Dosing	☑	☐	
☑	☐	8. Dosing silicone tube and Accessories	☑	☐	

Recommend : _____

_____

_____

Mr. Atachai Ngamchanat

Service Engineer

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Certificate of Calibration

Equipment:	Automatic Titrator	Certificate No.:	C32250031
Manufacturer:	SI Analytics	Job No.:	WO-00076560
Model:	TitroLine 7000	Issued Date:	30 June 2025
Serial No.:	10013826	Due Date:	30 June 2026
ID No.:	BKK_EN0373	Page:	1 of 3
Type of Titration :	Motor - driven		
Condition of the item:	Normal		

Customer: ALS Laboratory Group (Thailand) Co., Ltd.
104 Soi Pattanakarn 40, Pattanakarn Rd.,
Suan Luang, Bangkok 10250 Thailand

Environment Condition:

Temperature	22	°C	±	0.2 °C
Relative Humidity	56	%	±	1.9 %
Atmospheric Pressure	1009	mbar	±	0.2 mbar

Calibration Place: ALS Laboratory Group (Thailand) Co., Ltd. (Wet Chemistry Lab 2)
104 Soi Pattanakarn 40, Pattanakarn Rd.,
Suan Luang, Bangkok 10250 Thailand

Calibration By: Mr. Atachai Ngamchanat

Calibration Date: 30 June 2025

The Method Used: In house method, CAL-WI-57, base on ISO 8655:2002

Traceability: This certificate is traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through DKSH Technology Limited. Certificate No. C01243206

(Mr. Atachai Ngamchanat)
Person in charge

(Miss Kaewkan Suradech)
Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with Evaluation of measurement data - Guide to the expression of uncertainty in measurement (JCGM 100).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Calibration Results:

Nominal Volume 20 ml

Manufacturer: SI Analytics Burettes Model : TZ 3920 Serial No., Nr : 007773

Exchange Unit Model : WA-20 Exchange Unit Serial No. : 10045489 Nominal Vol.: 20 ml

Piston burettes of volumetric apparatus for automatic titrator

Volume (%)	Volume (ml)	Measurement Volume (V_{20}) (ml)	Systematic error (trueness)		Random error (precision)		Measurement Uncertainty (µl)	k
			es (%)	es (µl)	CV (%)	S_r (µl)		
10%	2.0000	2.0009	0.004	0.9	0.004	0.7	0.73	2.04
50%	10.0000	10.0050	0.025	5.0	0.002	0.4	0.90	2.00
100%	20.0000	20.0054	0.027	5.4	0.003	0.5	1.5	2.00

ISO 8655-3:2002(E) Table 1 - Maximum permissible errors for motor-driven piston burettes

Nominal volume ml	Maximum permissible systematic error		Maximum permissible random error	
	± %	± µl [a]	± % [b]	± µl [c]
≤1	0.6	6	0.1	1
2	0.5	10	0.1	2
5	0.3	15	0.1	5
10	0.2	20	0.07	7
20	0.2	40	0.07	14
25	0.2	50	0.07	17.5
50	0.2	100	0.05	25
100	0.2	200	0.03	30

a Expressed as the deviation of the mean of tenfold measurement from the nominal volume or from the selected volume (see ISO 8655-6:2002, 8.4)

b Expressed as the coefficient of variation of a tenfold measurement (see ISO 8655-6:2002, 8.5)

c Expressed as the repeatability standard deviation of a tenfold measurement (see ISO 8655-6:2002, 8.5)

The End of Certificate

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Checklist for Automatic Titrator

Worksheet number: WO-00076560

Instrument type: Automatic Titrator Model: TitroLine 7000 S/N: 10013826

Check (receive)		Checklist	Check (send)		Note
30 Jun 2025			30 Jun 2025		
Normal	Defective		Normal	Defective	
☑	☐	1. Integrity of the tools	☑	☐	
☑	☐	2. Cleanliness of tools	☑	☐	
☑	☐	3. On-Off Swicth	☑	☐	
☑	☐	4. Keypad	☑	☐	
☑	☐	5. Display, Screen Contrast	☑	☐	
☑	☐	6. Piston Burettes	☑	☐	
☑	☐	7. Function Rinsing and Dosing	☑	☐	
☑	☐	8. Dosing silicone tube and Accessories	☑	☐	

Recommend : _____

_____

_____

Mr. Atachai Ngamchanat

Service Engineer

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)

CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES

534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000 FAX. 0-2719-9484

Certificate of Testing

Cert.No.: 25TW101
Page.: 1 of 2

Equipment :	DO Meter
Manufacturer :	YSI
Model :	5000-230V
Serial No. :	09J101147
ID No. :	BKK_EN0017
Received Date :	19 May 2025
Test Date :	20 May 2025
Reference :	2505-0593DSC-1
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand
Laboratory Condition :	Temperature (25 ± 5) °C Humidity (50 ± 20) %
Test Procedure :	In - house method : CP-CH9 by Comparison Technique with Azide Modification Method
Tested by :	Walalak Sirithean
Approved by :	Approved Signatory

REVIEW BY Sinda K.

APPROVED BY Siriluk P.

NEXT CAL DATE 20/11/26

( ) Chakrit Waewwanjua
( ) Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 20 May 2025

Condition of this result of calibration

1. Reference Standard Instruments :
   This measurement result is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

Instruments	Serial No.	ID No.	Certificate No.	Due Date
1. Burette	-	130BU10	25CG1126	18 Mar 2027
2. Balance	14233821	110RC001	24MM131	04 July 2025

2. Standard Material :-

Material	Manufacturer	Lot.No.	Assay
Sodium Thiosulfate 5-Hydrate AR	KEMAUS	2203162447	99.6%

Result : **Dissolved Oxygen Meter Adjustment With Air 100 %**
Dissolved Oxygen Probe No.: 16K100498

Titration Method (Azide Modification Method) (mg/L)	**DO Meter Reading** (mg/L)	**Standard Deviation** (mg/L)
8.20	8.21	0.0090

This report was certified only for the instrument we tested.It is allowable to use for study Intend to use for advertising and referral purpose is prohibited.This report may not be reproduced other in full, without written approval of the laboratory

-o0o-

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

ilac-MRA

NSC-TISI-TIS17025
CALIBRATION 0008

Certificate of Calibration

Cert. No.: 25LM83

Equipment :	DO Meter with Sensor
Manufacturer :	YSI
Model :	5000-230V
Serial No. :	09J101147
ID No. :	BKK_EN0017
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand
Location :	TPA On Site Calibration Laboratory
Received Order :	19 May 2025
Calibrated Date :	20 May 2025
Ambient Temperature :	(26 ± 10) °C
Relative Humidity :	(50 ± 30) %
AC Line Voltage :	(220 ± 22) V

Calibrated by : Warakorn Lerngagtrakul

Approved by : Kunchit

Approved Signatory

( ) Chakrit Waewwanjua
( ) Suwit Imjai
(✓) Kunchit Promprat

Issue Date : 26 May 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Equipment : DO Meter with Sensor **Cert. No.:** 25LM83

Condition As-Received : Used Item

Reference : 2505-0593DSC-2

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Digital Thermometer	2188080	24I1022	TPA	17 Sep 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N.: 16K100498

Calibration Point (°C)	Immersion Depth (mm)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty (± °C)	Coverage Factor *k*
20.00	60	20.003	19.92	-0.083	0.15	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor ***k***, providing a level of confidence of approximately 95 %.

-o0o-

SCG

Metrology Center

SCI ECO Services Company Limited

51 Moo 8, Tubkwang, Kaeng Khoi, Saraburi, Thailand 18260

Bangkok Tel : +668 9205 6851 , +669 81924 0059

Saraburi Tel : +669 8247 2360

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

NSC-TISI-TIS 17025
CALIBRATION 0244

Certificate No. T252280

Certificate of Calibration

Equipment	:	Chamber (Incubator)
Manufacturer	:	Memmert
Model	:	ICP 750
Serial No.	:	F818.0075
Customer Code	:	BKK_EN0305
ID No.	:	T9571A4
Customer	:	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250
Customer Location	:	Wet Chemistry Lab 2
Date of Receipt	:	17 December 2025
Calibrated By	:	Atiphong Rongrat (Technician)
Approved By	:	_____ / Boonchai Suriyawong (Site Calibration Manager)
Date of Issue	:	12 JAN 2026

REVIEW BY Linda K.
APPROVED BY Siriluk P.
NEXT CAL. DATE 23/12/26.

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Certificate No. T252280

Calibration Report

Equipment : Chamber (Incubator)
Date of Calibration : 23 December 2025
Environment : Temperature : 23.4-24.9 °C
Line Voltage : 221.4-224.7 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :


1. This equipment was calibrated by insert 12 resistance thermometer detectors into its chamber , the other one resistance thermometer detector use for ambient temperature measurement . The calibration was done in according to WI-T20 (based on ASTM E145-94 (Reapproved 2001) and AS2853-1986).
   All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .
2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
RTD	100 ohm	31-(CH1-10)	T250835	24 May 2026
RTD	100 ohm	32-(CH1-10)	T250835	24 May 2026
DATA LOGGER	34970A	T193	T250835	24 May 2026

3. This certificate is traceable to :
   National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)
4. Condition of calibrated item : good
   Equipment Description :
   Time Constant 2 Hour - Minute At 20 °C
   Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
   ☐ Close
   ☒ Not Available
5. Adjustment :
   (X) without adjustment ( ) after adjustment

Approved By. _____

Calibration Report

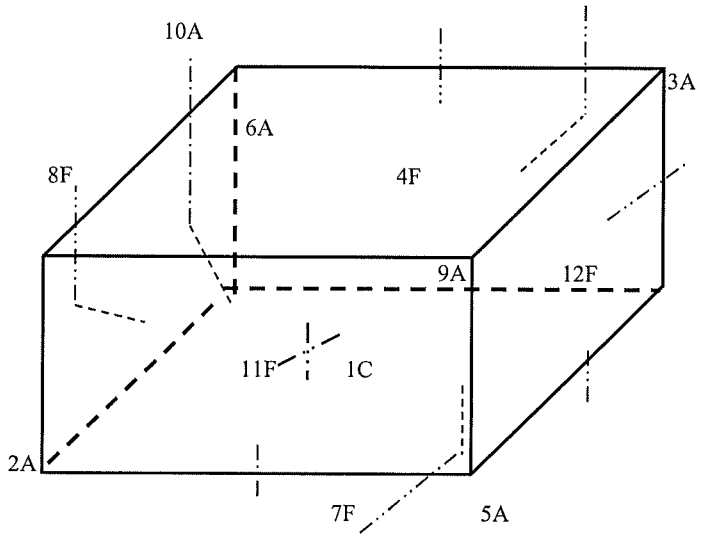

C = Centre , F = Centre of Face , A = Corner , E = Centre of Edge

1C	=	31-CH1
2A	=	31-CH2
3A	=	31-CH3
4F	=	31-CH4
5A	=	31-CH5
6A	=	31-CH6
7F	=	31-CH7
8F	=	31-CH8
9A	=	31-CH9
10A	=	31-CH10
11F	=	32-CH1
12F	=	32-CH2

Approved By.

SCG

Metrology Center

SCI ECO Services Company Limited

51 Moo 8, Tubkwang, Kaeng Khoi, Saraburi, Thailand 18260

NSC-TISI-TIS 17025
CALIBRATION 0244

Certificate No. T252280

Calibration Report

Measurement Results :

	Average Standard Reading at each position (°C)											
Calibration Point	31-CH1	31-CH2	31-CH3	31-CH4	31-CH5	31-CH6	31-CH7	31-CH8	31-CH9	31-CH10	32-CH1	32-CH2
20	20.14	20.33	20.04	20.35	20.03	19.87	19.92	20.24	20.29	20.20	19.93	19.81

	Average Standard Reading at each position (°C)											
Calibration Point	31-CH1	31-CH2	31-CH3	31-CH4	31-CH5	31-CH6	31-CH7	31-CH8	31-CH9	31-CH10	32-CH1	32-CH2
25	24.96	25.23	25.12	25.17	25.24	24.99	25.09	24.97	25.27	25.08	25.31	25.17

Chamber (Incubator)			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (±°C)	Uniformity (°C)	Uncertainty (±°C)	Coverage Factor **k**
	Min , Max	Average					
20.0	-	20.0	20.09	0.10	0.41	0.38	2.02
25.0	-	25.0	25.13	0.10	0.37	0.38	2.02

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor **k** which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By._____

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Certificate of Calibration

Cert.No.: 25CG3385
Page.: 1 of 2

Equipment :	Burette
Capacity :	50 mL
Serial No. :	-
ID. No. :	BKK_EN0422
Manufacturer :	Witeg
Made in :	Germany
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand
Ambient Temperature :	(20 ± 2.5) °C
Relative Humidity :	(50 ± 10) %
Barometric Pressure :	753 mmHg
Calibration Procedure :	ASTM E 542 - 01
Calibrated by :	Srisuda Khamtha
Approved by :	Approved Signatory

REVIEW BY Srisuda K.

APPROVED BY Siriluk P.

NEXT CAL DATE 03/09/26

( ) Ponpan Paipim
(✓) Chakrit Waewwanjua

Issue Date : 3 September 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Equipment : Burette
Received Date : 1 September 2025
Condition As-Received : Used Item
Calibration Date : 3 September 2025
Reference : 2509-0049DSC-1

Cert.No.: 25CG3385

Condition of this result of calibration

1. Reference Standard Instruments :

Instruments	Model	Serial No.	ID. No.	Certificate No.	Traceability	Due date
1) Balance	MS204TS	C226356983	140RC010	24MM603	TPA	10 Oct 2025
2) Data Logger	HL-20D	20683159	140EC012	24H2129	TPA	15 Oct 2025
3) Digital Thermometer	HH376	230806555	140EC013	25I1740	TPA	17 Jan 2026

This measurement result is traceable to SI Unit

2. The certificate is valid only to the item calibrated on date and place of calibration.
3. True value is converted to true volume at the standard temperature of 20 $^{\circ}$C

Calibration result :

Nominal capacity (mL)	Reading (mL)	Uncertainty (± mL)	*k* Factor
10	9.9941	0.0082	2.00
25	24.9804	0.0087	2.00
50	49.9819	0.010	2.00

Remark mL = cm^3

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k* , providing a level of confidence of approximately 95 %.

-o0o-

ภาคผนวก ฉ

สำเนาหนังสืออนุญาตขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน



ที่ อก ๐๓๑๐(๑)/ ๑๖๑๖๘

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๒๐ พฤศจิกายน ๒๕๖๖

เรื่อง ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน ลงวันที่ ๔ สิงหาคม ๒๕๖๖

สิ่งที่ส่งมาด้วย ๑. รายชื่อผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๑ แผ่น
๒. รายชื่อเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๕ แผ่น
๓. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๓๑ แผ่น

ตามหนังสือที่อ้างถึง บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ขอต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๒๐๔ สถานที่ตั้งเลขที่ ๑๐๔ ซอยพัฒนาการ ๔๐ ถนนพัฒนาการ แขวงพัฒนาการ เขตสวนหลวง กรุงเทพมหานคร ต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน โดยมีองค์ประกอบดังนี้

ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๖ ราย ตามสิ่งที่ส่งมาด้วย ๑

ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ ๑๘๑ ราย ตามสิ่งที่ส่งมาด้วย ๒

ค. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนให้วิเคราะห์ในน้ำเสีย น้ำใต้ดิน อากาศเสีย สิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว และดิน ตามสิ่งที่ส่งมาด้วย ๓

หนังสือฉบับนี้จะหมดอายุในวันที่ ๒ กันยายน ๒๕๖๙ หากประสงค์จะต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ให้ยื่นคำขอต่ออายุพร้อมเอกสารประกอบคำขอต่อกรมโรงงานอุตสาหกรรม ภายใน ๓๐ วัน ก่อนวันสิ้นอายุของหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ทั้งนี้ สามารถยื่นคำขอผ่านระบบอิเล็กทรอนิกส์ได้ที่หน้าเว็บไซต์กรมโรงงานอุตสาหกรรม

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายศิระ จันทร์เฉิด)
นักวิทยาศาสตร์เชี่ยวชาญ รักษาราชการแทน
ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน
กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ
โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕
โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๙๙
ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th

สิ่งที่ส่งมาด้วย ๑

เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด เลขทะเบียน ว-๒๐๔
ที่ อก ๐๓๑๐(๑)/ ๑๖๑๖๘ ลงวันที่ ๒๐ พฤศจิกายน ๒๕๖๖

ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๖ ราย

๑) นางสาวยุพาพร จันทร์เปล่ง	ทะเบียนเลขที่ ว-๒๐๔-ค-๐๐๐๑
๒) นางสาวชัชนัย โกมารกุล ณ นคร	ทะเบียนเลขที่ ว-๒๐๔-ค-๐๐๐๒
๓) นายศรายุทธ จิตรานนท์	ทะเบียนเลขที่ ว-๒๐๔-ค-๐๐๐๓
๔) นางสาวกนกกร เอนก	ทะเบียนเลขที่ ว-๒๐๔-ค-๐๐๐๔
๕) นายสุริยา สอนแก้ว	ทะเบียนเลขที่ ว-๒๐๔-ค-๐๐๐๕
๖) นายวิชาญ ชุณหรัต	ทะเบียนเลขที่ ว-๒๐๔-ค-๐๐๐๖

เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด เลขทะเบียน ว-๒๐๔
ที่ อก ๐๓๑๐(๑)/ ๑๖๑๖๘ ลงวันที่ ๒๐ พฤศจิกายน ๒๕๖๖

ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๑๘๑ ราย

๑) นายกาจบัณฑิต กิตติศุภวณิชย์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๐๑
๒) นายภัทรพล สว่างใจธรรม์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๐๒
๓) นายนราธิป เทือกชัยคำ	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๐๓
๔) นายศิริโชค พงษ์ประสม	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๐๔
๕) นายณัฐวุฒิ ด้วงแพง	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๐๕
๖) นางสาวจินดา โขจุลธรรม	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๐๖
๗) นางสาวสาวิตรี น้อยเสงี่ยม	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๐๗
๘) นางสาวชณัฐกาญจน์ อิ่มชม	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๐๘
๙) นางสาวนรินทร์ สายเส็ง	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๐๙
๑๐) นางสาวนันทวดี สมบูรณ์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๑๐
๑๑) นางสาวศรัณยา เฉลิมธำรงค์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๑๑
๑๒) นางสาวธัญญธร มงคลจิรวุฒิ	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๑๒
๑๓) นางสาวศิริลักษณ์ บุนนาค	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๑๓
๑๔) นายนพพงศ์ จันทรุพันธุ์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๑๔
๑๕) นายนรเศรษฐ์ โกมาลย์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๑๕
๑๖) นายธันวา จริยา	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๑๖
๑๗) นางสาวเกศรินทร์ แก้วมั่น	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๑๗
๑๘) นางสาวสุวิมล ชัยเรืองวุฒิ	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๑๘
๑๙) นางสาวสุชาดา ธรรมถาวร	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๑๙
๒๐) นางสาวเปมิกา ชัยเดชธนกุล	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๒๐
๒๑) นางสาวศศิธร หมูสวัสดิ์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๒๑
๒๒) นางสาวเสาวลักษณ์ ภู่นภาอำพร	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๒๒
๒๓) นายอภิสิทธิ์ สิงหา	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๒๓
๒๔) นายศักดิ์สิทธิ์ ไพศาลพิสุทธิ์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๒๔
๒๕) ว่าที่ร้อยตรีหญิง พรรณิภา ขำเจริญ	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๒๕
๒๖) นางจิลดา คำภูแก้ว	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๒๖
๒๗) นางสาวอรวรรณ รักยง	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๒๗
๒๘) นางสาวนพรัตน์ แย้มกรานต์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๒๘
๒๙) นายจุลเดช วารินทร์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๒๙
๓๐) นางสาวดายุรัตน์ ร้องคำ	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๓๐
๓๑) นายพรมมี ศรีปัตเนตร	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๓๑
๓๒) นายอุทิศ อุ่นสิม	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๓๒
๓๓) ว่าที่ร้อยตรี เฉลิมเกียรติ อมรศรีเสริม	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๓๓
๓๔) นางสาววริยา สร้างนา	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๓๔
๓๕) นายอนุพงศ์ รัตนศรีประเสริฐ	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๓๕

๓๖) นางสาวจุฑารัตน์...

๓๖) นางสาวจุฑารัตน์ โอนสันเทียะ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๓๖
๓๗) นางสาวจารุวรรณ พิมพ์อภิกฤติยา ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๓๗
๓๘) นางสาวปรางค์ทิพย์ กิจไพศาลศักดิ์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๓๘
๓๙) นางสาวเตือนใจ ทางกลาง ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๓๙
๔๐) นางสาวจิราพร ศิริเวช ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๔๐
๔๑) นายวรากร ผูกรักษ์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๔๑
๔๒) นายทนง วิริยะสหกิจ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๔๒
๔๓) นายธนิต เจนจบ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๔๓
๔๔) นายคณิศร ขำเพชร ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๔๔
๔๕) นายภูวิช พรหมสะอาด ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๔๕
๔๖) นายธนเดช โภคาพิพัฒน์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๔๖
๔๗) นายชวฤทธิ์ วงษ์จันทร์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๔๗
๔๘) นายอาทิตย์ ศรีเสน ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๔๘
๔๙) นายเจษดินทร์ คงศักดิไทย ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๔๙
๕๐) นายจรัส บุญยิ่ง ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๕๐
๕๑) นายธนาณัติ เอนก ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๕๑
๕๒) นายอภิวัฒน์ ทุมทนู ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๕๒
๕๓) นางสาวสุภาขวัญ มาก ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๕๓
๕๔) นางสาวทัตพร ชวาลสมบูรณ์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๕๔
๕๕) นางสาวธิติมา บุญเพ็ง ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๕๕
๕๖) นางสาวภานุมาศ นามวัฒน์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๕๖
๕๗) นางสาวอุไรรัตน์ ทึงสร้างแป้น ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๕๗
๕๘) นายธีรวัฒน์ ปวงสุข ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๕๘
๕๙) นายอิทธิพล ยะโส ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๕๙
๖๐) นายประพจน์ วรรณชูชัย ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๐
๖๑) นายชยธร พวงทิพย์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๑
๖๒) นางสาวกนกวรรณ จันทบาล ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๒
๖๓) นายสิทธิโชค ธงเงิน ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๓
๖๔) นางศิลาวรรณ ใจบุญ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๔
๖๕) นางสาวพรรณธิดา พุ่มคง ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๕
๖๖) นายนวภัทร ศรีวิริยะ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๖
๖๗) นายสุวิชา ทองอ่อน ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๗
๖๘) นายวิญญู บุญตะนัย ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๘
๖๙) นายสมบูรณ์ บุตรจันทร์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๙
๗๐) นายวิรัตน์ ไชยนะรา ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๗๐
๗๑) นายนฤเบศน์ เพิ่มพูน ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๗๑
๗๒) นายจิรณัฐ ขาวละออ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๗๒
๗๓) นายอัสรี นามบุรี ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๗๓
๗๔) นายอัศวเรศ จ่อสาว ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๗๔

๗๕) นายประเสริฐ...

๗๕) นายประเสริฐ สุระขันธ์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๗๕
๗๖) นายนุกูล จันทร์เนียม ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๗๖
๗๗) นายพีรพงษ์ ทองคูณปรีดา ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๗๗
๗๘) นายนฤพล ทองนุช ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๗๘
๗๙) นายอนุวัฒน์ ม่วงแพร ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๗๙
๘๐) นายเจตศราวุฒิ ปัตตะมะ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๘๐
๘๑) นายกฤษณะ สายวรรณ์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๘๑
๘๒) นายพิชัย บุญยงค์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๘๒
๘๓) นายภานุพงศ์ โฮมวงศ์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๘๓
๘๔) นายสามารถ คุ้มปลี ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๘๔
๘๕) นายสัญชัย โกศรีนาม ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๘๕
๘๖) นายณัฐวุฒิ ศรีประเสริฐ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๘๖
๘๗) นายชวัลธัช นาคพนม ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๘๗
๘๘) นายพงศธร ชัยทิพย์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๘๘
๘๙) นายสิทธิโชค ทาสีดา ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๘๙
๙๐) นายธนากร อินสุตา ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๙๐
๙๑) นางสาววรณิชชา ชาติวันชัย ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๙๑
๙๒) นางสาวพิมพ์ตะวัน มินากูล ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๙๒
๙๓) นางสาวเพชรัตน์ สิงห์สมบุญ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๙๓
๙๔) นางสาวชญานิน พรหมจันทร์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๙๔
๙๕) นายกีรติ ทวีราช ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๙๕
๙๖) นายจักริน หมั่นวิชา ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๙๖
๙๗) นายฉัตรชัย สุขเปีย ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๙๗
๙๘) นายณรนนท์ ต๊ะทองคำ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๙๘
๙๙) นายดุลยพล สนนอก ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๙๙
๑๐๐) นายทักษ์ดนัย อุบลศรี ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๐
๑๐๑) นายธนศวร นามะกุณณา ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๑
๑๐๒) นายธิติพงศ์ บัวแดง ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๒
๑๐๓) นายนนทชัย อุปถัมภ์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๓
๑๐๔) นายนัฐพล คุณสุทธิ์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๔
๑๐๕) นายนันทวัฒน์ สาริน ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๕
๑๐๖) นายปิยะนัฐ พลมะศรี ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๖
๑๐๗) นายพงศ์สิริ โสมเขียว ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๗
๑๐๘) นายพีรพัฒน์ กำคำ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๘
๑๐๙) นายภาณุพงศ์ มานิตย์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๙
๑๑๐) นายมงคล ผลาทิพย์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๑๐
๑๑๑) นายสิรินนท์ ทองอั่น ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๑๑
๑๑๒) นายอเนชา ทันสมัย ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๑๒
๑๑๓) นายอดิศักดิ์ ผมไผ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๑๓

๑๑๔) นายอนันตชัย...

๑๑๔) นายอนันตชัย วีสม ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๑๔
๑๑๕) นายวรวุธ ดีนัก ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๑๕
๑๑๖) นายแสงตะวัน นะตะสัต ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๑๖
๑๑๗) นายยุทธพงศ์ รัตนะ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๑๗
๑๑๘) นายชยัณวุฒิ ไชยฮะนิจ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๑๘
๑๑๙) นายวิศรุต ศรีธรรมมา ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๑๙
๑๒๐) นายนนทกร เผือกผ่อง ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๒๐
๑๒๑) นายกำชัย สุทธะ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๒๑
๑๒๒) นางสาวณัฐภรณ์ บุญตะนัย ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๒๒
๑๒๓) นางสาวพัชรินทร์ แสนสร้อย ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๒๓
๑๒๔) นายไพรวัลย์ เปรี่ยมพิมาย ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๒๔
๑๒๕) นางสาวศุภมาศ ทองมาก ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๒๕
๑๒๖) นางสาวลลิตา จิตรสว่าง ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๒๖
๑๒๗) นางสาวชไมพร เสิกภู่เขียว ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๒๗
๑๒๘) นางสาวกฤติมาพร คำมีแก่น ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๒๘
๑๒๙) นางสาวสกุลรัตน์ ภาคภูมิ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๒๙
๑๓๐) นางสาวไพรินทร์ ศรีรูปี ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๐
๑๓๑) นางสาวทิพเนตร ผุยปัญญา ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๑
๑๓๒) นางสาวสาธิตา ปานทอง ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๒
๑๓๓) นางสาวอริสา ทองนวล ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๓
๑๓๔) นางสาวอรยา ค้าคล่อง ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๔
๑๓๕) นางสาวชุดาภรณ์ สุนทรสนาน ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๕
๑๓๖) นางสาวอัญชลี คำจันทร์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๖
๑๓๗) นายบุญฤทธิ์ เอี่ยมเทศ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๗
๑๓๘) นางสาวศุภรดา ปั้นมยุรา ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๘
๑๓๙) นางสาวพาฤดี คุณนาน ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๙
๑๔๐) นางสาวจิราเจต ฟองดา ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๔๐
๑๔๑) นางสาวอารยา มีชัย ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๔๑
๑๔๒) นางสาววิชชุตา นาคผจญ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๔๒
๑๔๓) นางสาวนันทิยา จันทะลุน ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๔๓
๑๔๔) นายกิตติพงศ์ แซ่ลี้ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๔๔
๑๔๕) นายอนุวัติ ภูถวิล ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๔๕
๑๔๖) นายธีรพล แสงทอง ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๔๖
๑๔๗) นายศักดิ์พิพัฒน์ บุญมั่น ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๔๗
๑๔๘) นายฐิติวัลค์ เอมอุไร ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๔๘
๑๔๙) นายชัยณรงค์ ศรีบุรินทร์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๔๙
๑๕๐) นางสาวอัจฉราวรรณ สวนสนอง ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๕๐
๑๕๑) นางสาวณัฐฐาพร สิงหา ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๕๑
๑๕๒) นายภีมเรศ แหยมโต ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๕๒

๑๕๓) นางสาวอุบล...

๑๕๓) นางสาวอุบล เศิกศิริ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๕๓
๑๕๔) นางสาวมโนรัตน์ ทองบุตร ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๕๔
๑๕๕) นายภาคภูมิ แทนไทย ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๕๕
๑๕๖) นางสาวสุภาณัฐ เมล์พ่วง ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๕๖
๑๕๗) นางสาวพรทิวา สาตาชนม์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๕๗
๑๕๘) นายเอกวิทย์ วันทะนา ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๕๘
๑๕๙) นายไตรมณฑล ทิพย์วรรณ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๕๙
๑๖๐) นายจิรเมธ ประเสริฐสิริพงศ์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๐
๑๖๑) นายจิรายุส เกษมสุข ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๑
๑๖๒) นายจีรศักดิ์ ศรีวิชัย ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๒
๑๖๓) นายณัฐกฤษณ์ สะพานแก้ว ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๓
๑๖๔) นายบูรณศักดิ์ ปะทิ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๔
๑๖๕) นายปัณณวิชญ์ เสมอทรัพย์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๕
๑๖๖) นายพิษณุพงษ์ ไชยา ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๖
๑๖๗) นายภัทรพงษ์ มณฑาทอง ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๗
๑๖๘) นายวสันต์ ตรีนกุล ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๘
๑๖๙) นายภาณุเดช เพชรอุด ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๙
๑๗๐) นายอนุกูล วิละแสง ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๗๐
๑๗๑) นายภัทรพงษ์ มีสุข ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๗๑
๑๗๒) นางสาวนุชรวี ลีละทีป ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๗๒
๑๗๓) นางสาวสุภาวดี โกศรีนาม ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๗๓
๑๗๔) นางสาวอรณิช เทียนดำ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๗๔
๑๗๕) นางสาวพรเพ็ญ ชอบสอน ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๗๕
๑๗๖) นางสาววันวิสา ขอนพิกุล ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๗๖
๑๗๗) นางสาวอรวรรณ เถาว์ทอง ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๗๗
๑๗๘) นางสาวอัยย์ลิณ เมอร์วิณณ์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๗๘
๑๗๙) นางสาวรวิสรา คุ่ยครอง ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๗๙
๑๘๐) นายวุฒิกร ศิริวรรณ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๘๐
๑๘๑) นางสาวจารุวรรณ กระจ่างพันธุ์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๘๑

เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด เลขทะเบียน ว-๒๐๔
ที่ อก ๐๓๑๐(๑)/ ๑๖๑๖๘ ลงวันที่ ๒๐ พฤศจิกายน ๒๕๖๖

ค. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๓๗๔ รายการ

น้ำเสีย จำนวน 60 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Aldicarb	High-Performance Liquid Chromatographic Method[4]
2	Aldicarb Sulfone	High-Performance Liquid Chromatographic Method[4]
3	Aldicarb Sulfoxide	High-Performance Liquid Chromatographic Method[4]
4	Aldrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
5	Arsenic	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
6	Barium	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
7	α-BHC	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
8	β-BHC	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
9	δ-BHC	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
10	γ-BHC	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
11	Biochemical Oxygen Demand	1) 5-Day BOD Test, Azide Modification Method[4] 2) 5-Day BOD Test, Membrane Electrode Method[4]
12	Carbaryl	High-Performance Liquid Chromatographic Method[4]
13	Carbofuran	High-Performance Liquid Chromatographic Method[4]
14	Cadmium	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
15	Chemical Oxygen Demand	1) Closed Reflux, Colorimetric Method[4] 2) Closed Reflux, Tritimetric Method[4]
16	Chlordane	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
17	Chromium	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
18	Color	ADMI Weighted-Ordinate Spectrophotometric Method[4]

19 Copper...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
19	Copper	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
20	Cyanide	Distillation, Colorimetric Method[4]
21	2,4´-DDD	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
22	4,4´-DDD	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
23	2,4´-DDE	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
24	4,4´-DDE	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
25	2,4´-DDT	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
26	4,4´-DDT	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
27	Dieldrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
28	Endosulfan Sulfate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
29	Endosulfan I	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
30	Endosulfan II	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
31	Endrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
32	Endrin Aldehyde	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
33	Formaldehyde	Distillation, Colorimetric Method[3]
34	Free Chlorine	1) DPD Ferrous Titrimetric Method[4] 2) DPD Colorimetric Method[4]
35	Heptachlor	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
36	Heptachlor Epoxide	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
37	Hexavalent Chromium	Colorimetric Method[4]
38	3-Hydroxycarbofuran	High-Performance Liquid Chromatographic Method[4]
39	Lead	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]

40 Manganese...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
40	Manganese	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
41	Mercury	1) Digestion, Cold-Vapor Atomic Absorption Spectrometric Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass spectrometric Method[4]
42	Methiocarb	High-Performance Liquid Chromatographic Method[4]
43	Methoxychlor	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
44	Methomyl	High-Performance Liquid Chromatographic Method[4]
45	Nickel	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
46	Oil & Grease	1) Liquid-Liquid, Partition-Gravimetric Method[4] 2) Soxhlet Extraction Method[4]
47	Oxamyl	High-Performance Liquid Chromatographic Method[4]
48	Propoxur	High-Performance Liquid Chromatographic Method[4]
49	pH	Electrometric Method[4]
50	Phenols	1) Distillation, Chloroform Extraction Method[4] 2) Distillation, Direct Photometric Method[4]
51	Selenium	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
52	Sulfide	Iodometric Method[4]
53	Temperature	Laboratory and Field Methods[4]
54	Total Dissolved Solids	Dried at 180 ^{0}C[4]
55	Total Kjeldahl Nitrogen	Semi-Micro Kjeldahl Method[4]
56	Total Phosphorous	Digestion, Colorimetric Method[4]
57	Total Suspended Solids	Dried from 103-105 ^{0}C[4]
58	Toxaphene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
59	Trivalent Chromium	1) Digestion, Inductively Coupled Plasma Method; Colorimetric Method; Calculation[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method; Colorimetric Method; Calculation[4]
60	Zinc	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[4]

น้ำใต้ดิน...

น้ำใต้ดิน จำนวน 126 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Acenaphthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
2	Acetone	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
3	Aldrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
4	Anthracene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
5	Antimony	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
6	Arsenic	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
7	Atrazine	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
8	Barium	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
9	Benz(a)anthracene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
10	Benzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
11	Benzo(b)fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
12	Benzo(k)fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
13	Benzoic Acid	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
14	Benzo(a)pyrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
15	Benzo[g,h,i]perylene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
16	Beryllium	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
17	Bis(2-chloroethyl)ether	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]

18 Bis(2-ethylhexyl)phthalate...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
18	Bis(2-ethylhexyl)phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
19	Bromodichloromethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
20	Bromoform	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
21	Butanol	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
22	Butyl benzyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
23	Cadmium	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
24	Carbazole	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
25	Carbon disulfide	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
26	Carbon tetrachloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
27	Chlordane	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
28	p-Chloroaniline	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
29	Chlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
30	Chlorodibromomethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
31	Chloroform	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
32	2-Chlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
33	Chromium	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
34	Chromium (III)	1) Digestion, Inductively Coupled Plasma Method; Colorimetric Method; Calculation[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method; Colorimetric Method; Calculation[4]
35	Chromium (VI)	Colorimetric Method[4]

36 Chrysene...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
36	Chrysene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
37	Cyanide	Distillation, Colorimetric Method[4]
38	2,4-D	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
39	DDD	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
40	DDE	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
41	DDT	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
42	Dibenz(a,h)anthracene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
43	Di-n-Butyl Phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
44	1,2-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
45	1,3-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
46	1,4-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
47	3,3-Dichlorobenzidine	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
48	1,1-Dichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
49	1,2-Dichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
50	1,1-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
51	cis-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
52	trans-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
53	2,4-Dichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
54	1,2-Dichloropropane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
55	1,3-Dichloropropane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
56	1,3-Dichloropropene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
57	Dieldrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
58	Diethyl Phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
59	2,4-Dimethylphenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
60	2,4-Dinitrophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
61	2,4-Dinitrotoluene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
62	2,6-Dinitrotoluene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
63	Di-n-octyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
64	Endosulfan	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
65	Endrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
66	Ethylbenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
67	Fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
68	Fluorene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
69	Heptachlor	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
70	Heptachlor epoxide	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
71	Hexachlorobenzene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
72	Hexachloro-1,3-butadiene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
73	n-Hexane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
74	α-HCH	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
75	β-HCH	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
76	γ-HCH	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
77	Hexachlorocyclopentadiene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
78	Hexachloroethane	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
79	Indeno(1,2,3-cd)pyrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
80	Isophorone	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
81	Lead	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
82	Manganese	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
83	Mercury	1) Digestion, Cold Vapor Atomic Absorption Spectrometric Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
84	Methanol	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
85	Methoxychlor	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
86	Methyl bromide	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
87	Methylene chloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
88	2-Methylphenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
89	2-Methylnapthalene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
90	Methyl tert-butyl Ether	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
91	Naphthalene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
92	Nickel	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
93	Nitrobenzene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]

94 N-Nitrosodiphenylamine...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
94	N-Nitrosodiphenylamine	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
95	N-Nitrosodi-n-Propylamine	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
96	Polychlorinated Biphenyls - PCB 1016 - PCB 1221 - PCB 1232 - PCB 1242 - PCB 1248 - PCB 1254 - PCB 1260	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
97	Pentachlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
98	pH	Electrometric Method[4]
99	Phenanthrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
100	Phenol	1) Distillation, Chloroform Extraction Method[4] 2) Distillation, Direct Photometric Method[4] 3) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
101	Pyrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
102	Selenium	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
103	Silver	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
104	Styrene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
105	1,1,2,2-Tetrachloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
106	Tetrachloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
107	Toluene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
108	Toxaphene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
109	TPH (C_5-C_8)	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,25]

110 TPH ($C_{>8}$-C_{16})...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
110	TPH ($C_{>8}$-C_{16})	Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[9,22]
111	TPH ($C_{>16}$-C_{35})	Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[9,22]
112	1,2,4-Trichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
113	1,1,1-Trichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
114	1,1,2-Trichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
115	Trichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
116	2,4,5-Trichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
117	2,4,6-Trichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
118	1,3,5-Trimethylbenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
119	Vanadium	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
120	Vinyl acetate	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
121	Vinyl chloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
122	m-Xylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
123	o-Xylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
124	p-Xylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
125	Xylene (Total)	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
126	Zinc	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]

อากาศเสีย...

อากาศเสีย (ปล่องระบาย) จำนวน 28 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Antimony	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5]
		2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[5]
2	Arsenic	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5]
		2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[5]
3	Beryllium	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5]
		2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[5]
4	Cadmium	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5]
		2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[5]
5	Carbon Monoxide	1) Instrumental Analyzer Method[5]
		2) Sampling Bag Non-Dispersive Infrared Method[5]
6	Chlorine	1) Absorption Sampling, Ion Chromatographic Method[5]
		2) Isokinetic Sampling, Ion Chromatographic Method [5]
7	Chromium	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5]
		2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[5]
8	Cobalt	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5]
		2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[5]
9	Copper	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5]
		2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[5]
10	Cresol	Adsorption Sampling, Gas Chromatographic Method[5]
11	Dioxins	Isokinetic Sampling[5]
12	Hydrogen Chloride	1) Absorption Sampling, Ion Chromatographic Method[5]
		2) Isokinetic Sampling, Ion Chromatographic Method[5]
13	Hydrogen Fluoride	1) Absorption Sampling, Ion Chromatographic Method[5]
		2) Isokinetic Sampling, Ion Chromatographic Method[5]
14	Hydrogen Sulfide	Absorption Sampling, Iodometric Method[5]

15 Lead...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
15	Lead	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[5]
16	Manganese	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[5]
17	Mercury	1) Isokinetic Sampling, Digestion, Cold-Vapor Atomic Absorption Spectrometric Method[5] 2) Isokinetic Sampling, Digestion, Cold-Vapor Atomic Fluorescence Spectrometric Method[5]
18	Nickel	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[5]
19	Opacity	Ringelmann's Method[2]
20	Oxides of Nitrogen	1) Absorption Sampling, Phenoldisulfonic Acid Method[5] 2) Absorption Sampling, Alkaline Permanganate/ Colorimetric Method[5] 3) Instrumental Analyzer Method[5]
21	Selenium	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[5]
22	Sulfur Dioxide	1) Absorption Sampling, Barium-Thorin Titrimetric Method[5] 2) Instrumental Analyzer Method[5]
23	Sulfuric Acid	Isokinetic Sampling, Barium-Thorin Titrimetric Method[5]
24	Tellurium	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[5]
25	Tin	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[5]
26	Total Suspended Particulate	1) Isokinetic Sampling, Gravimetric Method[5] 2) Paired Train, Isokinetic Sampling, Gravimetric Method[5]

27 Vanadium...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
27	Vanadium	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[5]
28	Xylene	Adsorption Sampling, Gas Chromatographic Method[5]

<u>สิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว จำนวน 35 รายการ</u>

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Aldrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,26] 2) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
2	Antimony	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,17] 3) Digestion, Inductively Coupled Plasma Method[7,16] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
3	Arsenic	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,17] 3) Digestion, Inductively Coupled Plasma Method[7,16] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
4	Barium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,17] 3) Digestion, Inductively Coupled Plasma Method[7,16] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]

5 Beryllium...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
5	Beryllium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,17] 3) Digestion, Inductively Coupled Plasma Method[7,16] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
6	Cadmium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,17] 3) Digestion, Inductively Coupled Plasma Method[7,16] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
7	Chlordane	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,26] 2) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
8	Chromium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,17] 3) Digestion, Inductively Coupled Plasma Method[7,16] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
9	Chromium (III)	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method; Waste Extraction, Colorimetric Method; Calculation Method[1,6,16,19] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method; Waste Extraction, Colorimetric Method; Calculation Method[1,6,17,19] 3) Digestion, Inductively Coupled Plasma Method; Alkaline Digestion, Colorimetric Method; Calculation Method[7,8,16,19] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method; Alkaline Digestion, Colorimetric Method; Calculation Method[7,8, 17,19]

10 Chromium (VI)...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
10	Chromium (VI)	1) Waste Extraction, Colorimetric Method[1,6,19] 2) Alkaline Digestion, Colorimetric Method[8,19]
11	Cobalt	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,17] 3) Digestion, Inductively Coupled Plasma Method[7,16] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
12	Copper	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,17] 3) Digestion, Inductively Coupled Plasma Method[7,16] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
13	2,4-D	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,26] 2) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
14	DDD	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,26] 2) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
15	DDE	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,26] 2) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
16	DDT	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,26]

2) Soxhlet...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
		2) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26]
		3) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
17	Dieldrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,26]
		2) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26]
		3) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
18	Endrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,26]
		2) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26]
		3) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
19	Heptachlor	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,26]
		2) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26]
		3) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
20	Lead	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,16]
		2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,17]
		3) Digestion, Inductively Coupled Plasma Method[7,16]
		4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
21	Lindane	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,26]
		2) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26]
		3) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]

22 Mercury...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
22	Mercury	1) Waste Extraction, Digestion, Cold-Vapor Atomic Absorption Spectrometric Method[1,6,20] 2) Waste Extraction, Digestion, Cold-Vapor Atomic Fluorescence Spectrometric Method[1,6,30] 3) Digestion, Cold-Vapor Atomic Absorption Spectrometric Method[20] 4) Digestion, Cold-Vapor Atomic Fluorescence Spectrometric Method[30] 5) Thermal Decomposition Amalgamation and Atomic Absorption Spectrometric Method[21]
23	Methoxychlor	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,26] 2) Soxhlet Extraction, Gas Chromatographic / Mass Spectrometric Method[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic /Mass Spectrometric Method[11,26]
24	Mirex	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,26] 2) Soxhlet Extraction, Gas Chromatographic / Mass Spectrometric Method[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic /Mass Spectrometric Method[11,26]
25	Molybdenum	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,17] 3) Digestion, Inductively Coupled Plasma Method[7,16] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
26	Nickel	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,17] 3) Digestion, Inductively Coupled Plasma Method[7,16] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
27	Polychlorinated biphenyls (PCBs) - Aroclor 1016 - Aroclor 1221 - Aroclor 1232 - Aroclor 1242 - Aroclor 1248 - Aroclor 1254 - Aroclor 1260	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,26] 2) Soxhlet Extraction, Gas Chromatographic Method[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic Method[11,26]

- 2-Chlorobiphenyl...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
	- 2-Chlorobiphenyl - 2,3-Dichlorobiphenyl - 2,2',5-Trichlorobiphenyl - 2,4',5-Trichlorobiphenyl - 2,2',3,5'-Tetrachlorobiphenyl - 2,2',5,5'-Tetrachlorobiphenyl - 2,3',4,4'-Tetrachlorobiphenyl - 2,2',3,4,5'-Pentachlorobiphenyl - 2,2',4,5,5'-Pentachlorobiphenyl - 2,3,3',4',6-Pentachlorobiphenyl - 2,2',3,4,4',5'-Hexachlorobiphenyl - 2,2',3,4,5,5'-Hexachlorobiphenyl - 2,2',3,5,5',6-Hexachlorobiphenyl - 2,2',4,4',5,5'-Hexachlorobiphenyl - 2,2',3,3',4,4',5-Heptachlorobiphenyl - 2,2',3,4,4',5,5'-Heptachlorobiphenyl - 2,2',3,4,4',5',6-Heptachlorobiphenyl - 2,2',3,4',5,5',6-Heptachlorobiphenyl - 2,2',3,3',4,4',5,5',6-Nonachlorobiphenyl	
28	Pentachlorophenol	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,26] 2) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
29	pH	Electrometric Method[23,24]
30	Selenium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,17] 3) Digestion, Inductively Coupled Plasma Method[7,16] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]

31 Silver...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
31	Silver	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,17] 3) Digestion, Inductively Coupled Plasma Method[7,16] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
32	Thallium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,17] 3) Digestion, Inductively Coupled Plasma Method[7,16] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
33	Toxaphene	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,26] 2) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
34	Vanadium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,17] 3) Digestion, Inductively Coupled Plasma Method[7,16] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
35	Zinc	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,17] 3) Digestion, Inductively Coupled Plasma Method[7,16] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]

ดิน จำนวน 125 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Acenaphthene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
2	Acetone	1)Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25] 2) Equilibrium Headspace, Gas Chromatographic/ Mass Spectrometric Method[13]
3	Aldrin	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
4	Anthracene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
5	Antimony	1) Digestion, Inductively Coupled Plasma Method[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
6	Arsenic	1) Digestion, Inductively Coupled Plasma Method[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
7	Atrazine	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
8	Barium	1) Digestion, Inductively Coupled Plasma Method[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
9	Benz(a)anthracene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
10	Benzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]

11 Benzo(b)fluoranthene

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
11	Benzo(b)fluoranthene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
12	Benzo(k)fluoranthene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
13	Benzoic acid	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
14	Benzo(a)pyrene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
15	Benzo(g,h,i)perylene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
16	Beryllium	1) Digestion, Inductively Coupled Plasma Method[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
17	Bis(2-chloroethyl)ether	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
18	Bis(2-ethylhexyl)phthalate	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
19	Bromodichloromethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
20	Bromoform	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
21	Butanol	Equilibrium Headspace, Gas Chromatographic/ Mass Spectrometric Method[13,25]
22	Butyl Benzyl Phthalate	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]

23 Cadmium...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
23	Cadmium	1) Digestion, Inductively Coupled Plasma Method[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
24	Carbazole	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
25	Carbon Disulfide	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
26	Carbon tetrachloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
27	Chlordane	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
28	p-Chloroaniline	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
29	Chlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
30	Chlorodibromomethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
31	Chloroform	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
32	2-Chlorophenol	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
33	Chromium	1) Digestion, Inductively Coupled Plasma Method[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
34	Chromium (III)	1) Digestion, Inductively Coupled Plasma Method; Alkaline Digestion, Colorimetric Method; Calculation Method[7,8,16,19] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method; Alkaline Digestion, Colorimetric Method; Calculation Method[7,8,17,19]
35	Chromium (VI)	Alkaline Digestion, Colorimetric Method[8,19]

36 Chrysene...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
36	Chrysene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
37	Cyanide	Extraction, Distillation, Colorimetric Method[27,28,29]
38	2,4-D	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
39	DDD	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
40	DDE	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
41	DDT	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
42	Dibenz(a,h)anthracene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
43	Di-n-Butyl Phthalate	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
44	1,2-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
45	1,3-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
46	1,4-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
47	3,3-Dichlorobenzidine	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
48	1,1-Dichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]

49 1,2-Dichloroethane...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
49	1,2-Dichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
50	1,1-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
51	cis-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
52	trans-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
53	2,4-Dichlorophenol	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
54	1,2-Dichloropropane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
55	1,3-Dichloropropane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
56	1,3-Dichloropropene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
57	Dieldrin	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
58	Diethyl Phthalate	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
59	2,4-Dimethylphenol	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
60	2,4-Dinitrophenol	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
61	2,4-Dinitrotoluene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
62	2,6-Dinitrotoluene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]

63 Di-n-Octyl Phthalate...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
63	Di-n-Octyl Phthalate	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
64	Endosulfan	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
65	Endrin	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
66	Ethylbenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
67	Fluoranthene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
68	Fluorene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
69	Heptachlor	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
70	Heptachlor epoxide	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
71	Hexachlorobenzene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
72	Hexachloro-1,3-butadiene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
73	n-Hexane	1) Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25] 2) Equilibrium Headspace, Gas Chromatographic/ Mass Spectrometric Method[13]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
74	α-HCH	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
75	β-HCH	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
76	γ-HCH	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
77	Hexachlorocyclopentadiene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
78	Hexachloroethane	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
79	Indeno(1,2,3-cd)pyrene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
80	Isophorone	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
81	Lead	1) Digestion, Inductively Coupled Plasma Method[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
82	Manganese	1) Digestion, Inductively Coupled Plasma Method[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
83	Mercury	1) Digestion, Cold-Vapor Atomic Absorption Spectrometric Method[20] 2) Thermal Decomposition, Amalgamation, and Atomic Absorption Spectrophotometry[21] 3) Digestion, Cold-Vapor Atomic Fluorescence Spectrometric Method[30]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
84	Methanol	1) Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25] 2) Equilibrium Headspace, Gas Chromatographic/ Mass Spectrometric Method[13,25]
85	Methoxychlor	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
86	Methyl Bromide	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
87	Methylene Chloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
88	2-methylphenol	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
89	2-Methylnaphthalene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
90	Methyl tert-Butyl Ether	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
91	Naphthalene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
92	Nickel	1) Digestion, Inductively Coupled Plasma Method[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
93	Nitrobenzene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26
94	N-Nitrosodiphenylamine	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
95	N-Nitrosodi-n-propylamine	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]

96 Polychlorinated biphenyls (PCBs)

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
96	Polychlorinated biphenyls (PCBs) - Aroclor 1016 - Aroclor 1221 - Aroclor 1232 - Aroclor 1242 - Aroclor 1248 - Aroclor 1254 - Aroclor 1260 - 2-Chlorobiphenyl - 2,2',3,5'-Tetrachlorobiphenyl - 2,2',5,5'-Tetrachlorobiphenyl - 2,3',4,4'-Tetrachlorobiphenyl - 2,2',3,4,5'-Pentachlorobiphenyl - 2,2',4,5,5'-Pentachlorobiphenyl - 2,3,3',4',6-Pentachlorobiphenyl - 2,2',3,4,4',5'-Hexachlorobiphenyl - 2,2',3,4,5,5'-Hexachlorobiphenyl - 2,2',3,5,5',6-Hexachlorobiphenyl - 2,2',4,4',5,5'-Hexachlorobiphenyl - 2,2',3,3',4,4',5-Heptachlorobiphenyl - 2,2',3,4,4',5,5'-Heptachlorobiphenyl - 2,2',3,4,4',5',6-Heptachlorobiphenyl - 2,2',3,4',5,5',6-Heptachlorobiphenyl - 2,2',3,3',4,4',5,5',6-Nonachlorobiphenyl	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
97	Pentachlorophenol	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
98	Phenanthrene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]

99 Phenol...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
99	Phenol	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
100	Pyrene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
101	Selenium	1) Digestion, Inductively Coupled Plasma Method[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
102	Silver	1) Digestion, Inductively Coupled Plasma Method[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
103	Styrene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
104	1,1,2,2-Tetrachloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
105	Tetrachloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
106	Toluene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
107	Toxaphene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
108	TPH (C_5–C_8)	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
109	TPH ($C_{>8}$– C_{16})	1) Automate Extraction, Gas Chromatographic Method[11,22] 2) Solvent Extraction, Gas Chromatographic Method[12,22] 3) Ultrasonic Extraction, Gas Chromatographic Method[22,31
110	TPH ($C_{>16}$ – C_{35})	1) Automate Extraction, Gas Chromatographic Method[11,22] 2) Solvent Extraction, Gas Chromatographic Method[12,22] 3) Ultrasonic Extraction, Gas Chromatographic Method[22,31]
111	1,2,4-Trichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
112	1,1,1-Trichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
113	1,1,2-Trichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
114	Trichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]

115 2,4,5-Trichlorophenol...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
115	2,4,5-Trichlorophenol	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
116	2,4,6-Trichlorophenol	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
117	1,3,5-Trimethylbenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
118	Vanadium	1) Digestion, Inductively Coupled Plasma Method[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
119	Vinyl Acetate	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
120	Vinyl Chloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
121	m-Xylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
122	o-Xylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
123	p-Xylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
124	Xylene (Total)	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
125	Zinc	1) Digestion, Inductively Coupled Plasma Method[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]

<u>เอกสารอ้างอิง</u>

1. กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2566. เรื่อง การจัดการสิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว. **ราชกิจจานุเบกษา.** 31 พฤษภาคม 2566. เล่มที่ 140 ตอนพิเศษ 126 ง.

2. กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2549. เรื่อง กำหนดค่าปริมาณเขม่าควันที่เจือปนในอากาศที่ระบายออกจากปล่องของหม้อน้ำโรงสีข้าวที่ใช้แกลบเป็นเชื้อเพลิง. **ราชกิจจานุเบกษา.** 4 ธันวาคม 2549. เล่มที่ 123 ตอนพิเศษ 125ง.

3. สมาคมวิศวกรรมสิ่งแวดล้อมแห่งประเทศไทย. **คู่มือวิเคราะห์น้ำเสีย.** พิมพ์ครั้งที่ 4. กรุงเทพฯ: เรือนแก้วการพิมพ์, 2547.

4. APHA, AWWA, WEF. **Standard Methods for the Examination of Water and Wastewater.** 24th ed. Washington, DC: APHA, 2023.

5. United States...

5. United States Environmental Protection Agency. **Standards of Performance for New Stationary Sources.** 40 CFR 60. Appendix A, 2023.

6. United States Environmental Protection Agency. **Test Methods for Evaluating Solid Waste Physical/Chemical Methods. SW-846,** 2014.

7. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Acid Digestion of Sludges and Sediments and Soils. SW-846 Method 3050B,** 1996.

8. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Alkaline Digestion for Hexavalent Chromium. SW-846 Method 3060A,** 1996.

9. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Separatory Funnel Liquid-Liquid Extraction. SW-846 Method 3510C,** 1996.

10. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Soxhlet Extraction. SW-846 Method 3540C,** 1996.

11. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Automated Soxhlet Extraction. SW-846 Method 3541,** 1994.

12. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Microscale Solvent Extraction (MSE). SW-846 Method 3570,** 2002.

13. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Volatile Organic Compounds (VOCs) in Various Sample Matrices Using Equilibrium Headspace Analysis. SW-846 Method 5021A,** 2014.

14. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Purge-and-Trap for Aqueous Samples. SW-846 Method 5030B,** 1996.

15. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Closed-System Purge-and-Trap and Extraction for Volatile Organics in Soil and Waste Samples. SW-846 Method 5035,** 1996.

16. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Inductively Coupled Plasma-Atomic Emission Spectrometry. SW-846 Method 6010B,** 1996.

17. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Inductively Coupled Plasma-Mass Spectrometry. SW-846 Method 6020A,** 2007.

18. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Antimony and Arsenic (Atomic Absorption, Borohydride Reduction). SW-846 Method 7062,** 1994. เพิ่มใหม่

19. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Chromium, Hexavalent (Colorimetric). SW-846 Method 7196A,** 1992.

20. United States...

20. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Mercury in Solid or Semisolid Waste (Manual Cold-Vapor Technique). SW-846 Method 7471B,** 2007.

21. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Mercury in Solids and Solutions by Thermal Decomposition, Amalgamation, and Atomic Absorption Spectrophotometry. SW-846 Method 7473,** 2007.

22. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Nonhalogenated Organics by Gas Chromatography. SW-846 Method 8015C,** 2007.

23. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **pH Electrometric Measurement. SW-846 Method 9040C,** 2004.

24. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Soil and Waste pH. SW-846 Method 9045D,** 2004.

25. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Volatile Organic Compounds by Gas Chromatography/ Mass Spectrometry (GC/MS). SW-846 Method 8260D,** 2018.

26. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Semivolatile Organic Compounds by Gas Chromatography/ Mass Spectrometry (GC/MS). SW-846 Method 8270E,** 2018.

27. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Total and Amenable Cyanide: Distillation SW-846 Method 9010B,** 1996.

28. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Cyanide Extraction Procedure for Solids and Oil. SW-846 Method 9013A,** 1996.

29. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Cyanide in Waters and Extracts Using Titrimetric and Manual Spectrophotometric Procedures. SW-846 Method 9014,** 2014.

30. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Mercury in Sediment and Tissue Samples by Atomic Fluorescence Spectrometry. SW-846 Method 7474,** 2007.

31. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Ultrasonic Extraction. SW-846 Method 3550C,** 2007.



ที่ อก ๐๓๑๐(๑)/ ๔๑๒๑

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๒๕ เมษายน ๒๕๖๗

เรื่อง เปลี่ยนแปลงบุคลากรของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน ลงวันที่ ๒๙ มีนาคม ๒๕๖๗

ตามคำขอที่อ้างถึง บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๒๐๔ สถานที่ตั้งเลขที่ ๑๐๔ ซอยพัฒนาการ ๔๐ ถนนพัฒนาการ แขวงพัฒนาการ เขตสวนหลวง กรุงเทพมหานคร ขอเปลี่ยนแปลงบุคลากร ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว มีความเห็นดังนี้

๑. ให้ยกเลิกเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๓ ราย

๑) นางสาวพรรณธิดา พุ่มคง	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๕
๒) นายกำชัย สุทธะ	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๒๑
๓) นางสาวศุภรดา ปั้นมยุรา	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๘

๒. ให้เพิ่มเจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน จำนวน ๑๒ ราย

๑) นางสาวฐานิดา กลิ่นเขียว	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๘๒
๒) นางสาวกัญญ์ภัสสร สายคำ	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๘๓
๓) นางสาวณัฐนันท์ กันทะวงค์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๘๔
๔) นายอำนาจ วงษาเคน	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๘๕
๕) นายกฤษณพล ปัญญาวงค์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๘๖
๖) นายณชากร หรรษา	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๘๗
๗) นายวัชรินทร์ ผ่องสามสวน	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๘๘
๘) นายณัฐพงศ์ โสภา	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๘๙
๙) นายศักรินทร์ ปานเพ็ง	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๙๐
๑๐) นายณัฐพล ชุ่มชื่น	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๙๑
๑๑) นายธนา สุพาพันธุ์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๙๒
๑๒) นายนราธร แก้วพงษ์ษา	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๙๓

อนึ่ง หนังสือฉบับนี้...

อนึ่ง หนังสือฉบับนี้จะหมดอายุพร้อมหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ในวันที่ ๒ กันยายน ๒๕๖๙

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายพรยศ กลั่นกรอง)
รองอธิบดี ปฏิบัติราชการแทน
อธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน
กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ
โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕
โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๙๙
ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th

ที่ อก ๐๓๑๐(๑)/๑๒๓๖๘ ๑

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๑๘ ธันวาคม ๒๕๖๗

เรื่อง ยกเลิกบุคลากรของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน ลงวันที่ ๒ ธันวาคม ๒๕๖๗

ตามคำขอที่อ้างถึง บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๒๐๔ สถานที่ตั้งเลขที่ ๑๐๔ ซอยพัฒนาการ ๔๐ ถนนพัฒนาการ แขวงพัฒนาการ เขตสวนหลวง กรุงเทพมหานคร ขอยกเลิกบุคลากร ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้ยกเลิกเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๘ ราย ได้แก่

๑) นายประพจน์ วรรณชูชัย	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๐
๒) นายจิรณัฐ ขาวละออ	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๗๒
๓) นายพีรพัฒน์ ก่ำคำ	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๘
๔) นางสาวอรยา ค้าคล่อง	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๔
๕) นายกิตติพงศ์ แซ่ลี้	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๔๔
๖) นายจิรเมธ ประเสริฐสิริพงศ์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๐
๗) นายภัทรพงษ์ มณฑาทอง	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๗
๘) นางสาวจารุวรรณ กระจ่างพันธุ์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๘๑

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายธีรทัศน์ อิศรางกูร ณ อยุธยา)
รองอธิบดี ปฏิบัติราชการแทน
อธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน
กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ
โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕
โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๙๙
ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th



ที่ อก ๐๓๑๐(๑)/ ๓๑๔๐

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๑๐ เมษายน ๒๕๖๘

เรื่อง ยกเลิกบุคลากรของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน ลงวันที่ ๒ เมษายน ๒๕๖๘

ตามคำขอที่อ้างถึง บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๒๐๔ สถานที่ตั้งเลขที่ ๑๐๔ ซอยพัฒนาการ ๔๐ ถนนพัฒนาการ แขวงพัฒนาการ เขตสวนหลวง กรุงเทพมหานคร ขอยกเลิกบุคลากร ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้ยกเลิกเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๒ ราย ได้แก่

๑) นายธิติพงศ์ บัวแดง	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๒
๒) นายมงคล ผลาทิพย์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๑๐

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายธีรทัศน์ อิศรางกูร ณ อยุธยา)
รองอธิบดี ปฏิบัติราชการแทน
อธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน
กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ
โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕
โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๙๙
ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th





ที่ อก ๐๓๑๐(๑)/ ๔๖๗๓

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๐๕ มิถุนายน ๒๕๖๘

เรื่อง เปลี่ยนแปลงบุคลากรของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน ลงวันที่ ๗ พฤษภาคม ๒๕๖๘

ตามคำขอที่อ้างถึง บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๒๐๔ สถานที่ตั้งเลขที่ ๑๐๔ ซอยพัฒนาการ ๔๐ ถนนพัฒนาการ แขวงพัฒนาการ เขตสวนหลวง กรุงเทพมหานคร ขอเปลี่ยนแปลงบุคลากร ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้เพิ่มเจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน จำนวน ๑๑ ราย ได้แก่

๑) นายคุณากร มั่นชื่น	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๙๔
๒) นายชัยมงคล แสนมาตร	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๙๕
๓) นายเอกรินทร์ บุดสักที	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๙๖
๔) นายพัชชานนท์ อินปริก	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๙๗
๕) นายศตวรรษ แก้วกันหา	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๙๘
๖) นายวิกรม มีศิริ	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๙๙
๗) นายภคนันท์ คำจันทราช	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๒๐๐
๘) นายศิรวิทย์ มิไพทูรย์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๒๐๑
๙) นายธีรพงษ์ ศรีคำแหง	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๒๐๒
๑๐) นายอภิสิทธิ์ ศรีคงแก้ว	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๒๐๓
๑๑) ว่าที่ร้อยตรี ภาณุพงศ์ แสนศรี	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๒๐๔

อนึ่ง หนังสือฉบับนี้จะสิ้นอายุพร้อมหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ในวันที่ ๒ กันยายน ๒๕๖๙

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายศิระ จันทร์เฉิด)
นักวิทยาศาสตร์เชี่ยวชาญ รักษาราชการแทน
ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน
กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ
โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕
โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๙๙
ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th



ที่ อก ๐๓๑๐(๑)/ ๖๙๐๘

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๒๑ สิงหาคม ๒๕๖๘

เรื่อง เปลี่ยนแปลงสารมลพิษที่วิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน ลงวันที่ ๒๗ มิถุนายน ๒๕๖๘

สิ่งที่ส่งมาด้วย เอกสารแนบท้ายหนังสือเปลี่ยนแปลงสารมลพิษที่วิเคราะห์ บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด จำนวน ๖ แผ่น

ตามคำขอที่อ้างถึง บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๒๐๔ สถานที่ตั้งเลขที่ ๑๐๔ ซอยพัฒนาการ ๔๐ ถนนพัฒนาการ แขวงพัฒนาการ เขตสวนหลวง กรุงเทพมหานคร ขอเปลี่ยนแปลงสารมลพิษที่วิเคราะห์ ต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด เพิ่มขอบข่ายชนิดสารมลพิษที่วิเคราะห์ในน้ำใต้ดิน สิ่งปฏิกูลและวัสดุที่ไม่ใช้แล้ว และดิน ตามสิ่งที่ส่งมาด้วย

อนึ่ง หนังสือฉบับนี้จะสิ้นอายุพร้อมหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ในวันที่ ๒ กันยายน ๒๕๖๙

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นางสาวปัทมวรรณ คุณประเสริฐ)
ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน
กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ
โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕
โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๙๙
ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th

เอกสารแนบท้ายหนังสือเปลี่ยนแปลงสารมลพิษที่วิเคราะห์
บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด เลขทะเบียน ว-๒๐๔
ที่ อก ๐๓๑๐(๑)/ ๖๙๐๘ ลงวันที่ ๒๑ สิงหาคม ๒๕๖๘

ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๔๐ รายการ

น้ำใต้ดิน จำนวน ๔ รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Aluminum	Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[2]
2	Copper	Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[2]
3	Iron	Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[2]
4	Molybdenum	Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[2]

สิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว จำนวน 17 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Antimony	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,3,7] 3) Digestion, Inductively Coupled Plasma Method[4,6] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
2	Arsenic	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,3,7] 3) Digestion, Inductively Coupled Plasma Method[4,6] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
3	Barium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,3,7] 3) Digestion, Inductively Coupled Plasma Method[4,6] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]

ฯลฯ

Beryllium

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
4	Beryllium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,3,7] 3) Digestion, Inductively Coupled Plasma Method[4,6] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
5	Cadmium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,3,7] 3) Digestion, Inductively Coupled Plasma Method[4,6] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
6	Chromium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,3,7] 3) Digestion, Inductively Coupled Plasma Method[4,6] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
7	Chromium (III)	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method; Waste Extraction, Colorimetric Method; Calculation Method[1,3,6,8] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method; Waste Extraction, Colorimetric Method; Calculation Method[1,3,7,8] 3) Digestion, Inductively Coupled Plasma Method; Alkaline Digestion, Colorimetric Method; Calculation Method[4,5,6,8] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method; Alkaline Digestion, Colorimetric Method; Calculation Method[4,5,7,8]
8	Cobalt	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,3,7]

3) Digestion...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
		3) Digestion, Inductively Coupled Plasma Method[4,6] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
9	Copper	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,3,7] 3) Digestion, Inductively Coupled Plasma Method[4,6] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
10	Lead	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,3,7] 3) Digestion, Inductively Coupled Plasma Method[4,6] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
11	Molybdenum	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,3,7] 3) Digestion, Inductively Coupled Plasma Method[4,6] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
12	Nickel	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,3,7] 3) Digestion, Inductively Coupled Plasma Method[4,6] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
13	Selenium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,3,7] 3) Digestion, Inductively Coupled Plasma Method[4,6] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]

14 Silver...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
14	Silver	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,3,7] 3) Digestion, Inductively Coupled Plasma Method[4,6] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
15	Thallium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,3,7] 3) Digestion, Inductively Coupled Plasma Method[4,6] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
16	Vanadium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,3,7] 3) Digestion, Inductively Coupled Plasma Method[4,6] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
17	Zinc	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,3,7] 3) Digestion, Inductively Coupled Plasma Method[4,6] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]

ดิน จำนวน 19 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Aluminum	1) Digestion, Inductively Coupled Plasma Method[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
2	Antimony	1) Digestion, Inductively Coupled Plasma Method[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]

3 Arsenic...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
3	Arsenic	1) Digestion, Inductively Coupled Plasma Method[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
4	Barium	1) Digestion, Inductively Coupled Plasma Method[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
5	Beryllium	1) Digestion, Inductively Coupled Plasma Method[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
6	Cadmium	1) Digestion, Inductively Coupled Plasma Method[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
7	Chromium	1) Digestion, Inductively Coupled Plasma Method[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
8	Chromium (III)	1) Digestion, Inductively Coupled Plasma Method; Alkaline Digestion, Colorimetric Method; Calculation Method[4,5,6,8] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method; Alkaline Digestion, Colorimetric Method; Calculation Method[4,5,7,8]
9	Copper	1) Digestion, Inductively Coupled Plasma Method[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
10	Iron	1) Digestion, Inductively Coupled Plasma Method[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
11	Lead	1) Digestion, Inductively Coupled Plasma Method[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
12	Manganese	1) Digestion, Inductively Coupled Plasma Method[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
13	Molybdenum	1) Digestion, Inductively Coupled Plasma Method[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
14	Nickel	1) Digestion, Inductively Coupled Plasma Method[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]

15 pH...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
15	pH	Electrometric Method[9]
16	Selenium	1) Digestion, Inductively Coupled Plasma Method[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
17	Silver	1) Digestion, Inductively Coupled Plasma Method[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
18	Vanadium	1) Digestion, Inductively Coupled Plasma Method[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
19	Zinc	1) Digestion, Inductively Coupled Plasma Method[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]

เอกสารอ้างอิง

1. กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2566. เรื่อง การจัดการสิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว. **ราชกิจจานุเบกษา.** 31 พฤษภาคม 2566. เล่มที่ 140 ตอนพิเศษ 126 ง.

2. APHA, AWWA, WEF. **Standard Methods for the Examination of Water and Wastewater.** 24th ed. Washington, DC: APHA, 2023.

3. United States Environmental Protection Agency. **Test Methods for Evaluating Solid Waste Physical/Chemical Methods. SW-846.**

4. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Acid Digestion of Sediments, Sludges, and Soils. SW-846 Method 3050B,** 1996.

5. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Alkaline Digestion for Hexavalent Chromium. SW-846 Method 3060A,** 1996.

6. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Inductively Coupled Plasma-Optical Emission Spectrometry. SW-846 Method 6010D,** 2018.

7. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Inductively Coupled Plasma-Mass Spectrometry. SW-846 Method 6020B,** 2014.

8. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Chromium, Hexavalent (Colorimetric). SW-846 Method 7196A,** 1992.

9. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Soil and Waste pH. SW-846 Method 9045D,** 2004.



ที่ อก ๐๓๑๐(๑)/๘๐ ๑๓

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๒๖ กันยายน ๒๕๖๘

เรื่อง เปลี่ยนแปลงบุคลากร ชื่อตัวและชื่อสกุลของบุคลากร

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน ลงวันที่ ๒๑ สิงหาคม ๒๕๖๘

ตามคำขอที่อ้างถึง บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัดห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๒๐๔ สถานที่ตั้งเลขที่ ๑๐๔ ซอยพัฒนาการ ๔๐ ถนนพัฒนาการ แขวงพัฒนาการ เขตสวนหลวง กรุงเทพมหานคร ขอเปลี่ยนแปลงบุคลากร ชื่อตัวและชื่อสกุลของบุคลากร ต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว มีความเห็นดังนี้

๑. ให้ยกเลิกเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๒ ราย

๑) นางสาวพาฤดี คุณนาน ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๙

๒) นางสาวอรณิช เทียนดำ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๗๔

๒. ให้เปลี่ยนชื่อตัวและชื่อสกุลของเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จากเดิม นายอาทิตย์ ศรีเสน เป็น นายรัฐธีร์ ทวีกิจวรพจน์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๔๘

อนึ่ง หนังสือฉบับนี้จะสิ้นอายุพร้อมหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ในวันที่ ๒ กันยายน ๒๕๖๙

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นางสาวปัทมวรรณ คุณประเสริฐ)
ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน
กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ
โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕
โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๙๙
ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th

บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด (สำนักงานใหญ่)
104 ซอยพัฒนาการ 40 ถนนพัฒนาการ
แขวงพัฒนาการ เขตสวนหลวง กรุงเทพฯ 10250



ติดต่อเรา