ภาคผนวก ค

รายงานผลการตรวจวัดคุณภาพสิ่งแวดล้อม

Thai Environmental Technic Limited
บริษัท เทคนิคสิ่งแวดล้อมไทย จำกัด

1/6 Soi Ramkhamhaeng 145, Khwaeng / Khet Saphansung, Bangkok 10240
1/6 ซอยรามคำแหง 145 แขวงสะพานสูง เขตสะพานสูง กรุงเทพมหานคร 10240
E-mail : th08_contact@eurofinsasia.com
Tel : 0-2373-7799 (Auto) Fax : 0-2373-7979

TEST REPORT

Analysis No. : R26-2474
Received Date : 22-29/06/26
Customer : Technical Division of Thai Environmental Technic Limited
For บริษัท ชิน เคอ หยวน จำกัด
โครงการโรงงานผลิตเหล็กแผ่น เหล็กรูปพรรณ และเหล็กลวด
Address : 666 หมู่ 2 ตำบลตาสิทธิ์ อำเภอปลวกแดง จังหวัดระยอง 21140
Contact : Tel. (033) 684 290-7 Fax. (033) 684 298-9

Report Date : 03/07/26
Analysis Date : 22/06-02/07/26
Job No. : S690658/June
Sampling By : TET
Type of Sample : Ambient Air

Sampling Point	Sample No.	Sampling Date	Result		Analysis Date
			TSP ($\mu g/m^3$)	PM-10 ($\mu g/m^3$)	
บ้านเฉลิมลาภ (A1) (47P 0742734 UTM 1447405)	2606-AA1164	19-20/06/26	32	14	22-25/06/26
	2606-AA1230	20-21/06/26	21	11	22-25/06/26
	2606-AA1342	21-22/06/26	33	15	23-26/06/26
	2606-AA1389	22-23/06/26	45	14	24-29/06/26
	2606-AA1476	23-24/06/26	47	13	25-30/06/26
	2606-AA1659	24-25/06/26	38	8	26/06-01/07/26
	2606-AA1896	25-26/06/26	24	6	29/06-02/07/26
บ้านเขาระฆัง (A2) (47P 0744494 UTM 1446004)	2606-AA1165	19-20/06/26	20	12	22-25/06/26
	2606-AA1231	20-21/06/26	22	11	22-25/06/26
	2606-AA1343	21-22/06/26	25	13	23-26/06/26
	2606-AA1390	22-23/06/26	29	12	24-29/06/26
	2606-AA1477	23-24/06/26	12	6	25-30/06/26
	2606-AA1660	24-25/06/26	17	8	26/06-01/07/26
	2606-AA1897	25-26/06/26	18	7	29/06-02/07/26
Standard			200	100	

Method : TSP = Gravimetric Method (US.EPA 40 CFR Part 50 Appendix B)
PM-10 = Gravimetric Method (US.EPA 40 CFR Part 50 Appendix J)
Standard : Notification of the National Environment Board (2026) (B.E. 2569), 24-hr. average value

Reviewed by
Ms. Wareerat Prachumdaeng
Chief of Laboratory
03/07/26

Approved by
Mrs. Porntip Pethshee
Laboratory Manager
03/07/26



• REPORTED RESULTS REFER TO SUBMITTED SAMPLE(S) ONLY
• DO NOT COPY PARTIAL OF THIS ANALYSIS REPORT WITHOUT OFFICIAL APPROVAL

Thai Environmental Technic Limited
บริษัท เทคนิคสิ่งแวดล้อมไทย จำกัด

1/6 Soi Ramkhamhaeng 145, Khwaeng / Khet Saphansung, Bangkok 10240
1/6 ซอยรามคำแหง 145 แขวงสะพานสูง เขตสะพานสูง กรุงเทพมหานคร 10240
E-mail : th08_contact@eurofinsasia.com
Tel : 0-2373-7799 (Auto) Fax : 0-2373-7979

TEST REPORT

Analysis No. : R26-2474
Received Date : 22-29/06/26
Customer : Technical Division of Thai Environmental Technic Limited
For บริษัท ซิน เคอ หยวน จำกัด
โครงการโรงงานผลิตเหล็กแผ่น เหล็กรูปพรรณ และเหล็กลวด
Address : 666 หมู่ 2 ตำบลตาสิทธิ์ อำเภอปลวกแดง จังหวัดระยอง 21140
Contact : Tel. (033) 684 290-7 Fax. (033) 684 298-9

Report Date : 03/07/26
Analysis Date : 22/06-02/07/26
Job No. : S690658/June
Sampling By : TET
Type of Sample : Ambient Air

Sampling Point	Sample No.	Sampling Date	Result		Analysis Date
			TSP ($\mu g/m^3$)	PM-10 ($\mu g/m^3$)	
บ้านใต้สุน (A3) (47P 0740109 UTM 1444442)	2606-AA1166	19-20/06/26	59	36	22-25/06/26
	2606-AA1232	20-21/06/26	16	4	22-25/06/26
	2606-AA1344	21-22/06/26	59	40	23-26/06/26
	2606-AA1391	22-23/06/26	91	77	24-29/06/26
	2606-AA1478	23-24/06/26	31	28	25-30/06/26
	2606-AA1661	24-25/06/26	32	6	26/06-01/07/26
	2606-AA1898	25-26/06/26	41	14	29/06-02/07/26
โรงเรียนบ้านระเวิง (A4) (47P 0739498 UTM 1447954)	2606-AA1167	19-20/06/26	27	16	22-25/06/26
	2606-AA1233	20-21/06/26	16	3	22-25/06/26
	2606-AA1345	21-22/06/26	30	21	23-26/06/26
	2606-AA1392	22-23/06/26	44	28	24-29/06/26
	2606-AA1479	23-24/06/26	16	8	25-30/06/26
	2606-AA1662	24-25/06/26	23	7	26/06-01/07/26
	2606-AA1899	25-26/06/26	20	6	29/06-02/07/26
Standard			200	100	

Method : TSP = Gravimetric Method (US.EPA 40 CFR Part 50 Appendix B)
PM-10 = Gravimetric Method (US.EPA 40 CFR Part 50 Appendix J)
Standard : Notification of the National Environment Board (2026) (B.E. 2569), 24-hr. average value

Reviewed by
Ms. Wareerat Prachumdaeng
Chief of Laboratory
03/07/26

Approved by
Mrs. Porntip Pethshee
Laboratory Manager
03/07/26



• REPORTED RESULTS REFER TO SUBMITTED SAMPLE(S) ONLY
• DO NOT COPY PARTIAL OF THIS ANALYSIS REPORT WITHOUT OFFICIAL APPROVAL

Thai Environmental Technic Limited
บริษัท เทคนิคสิ่งแวดล้อมไทย จำกัด

1/6 Soi Ramkhamhaeng 145, Khwaeng / Khet Saphansung, Bangkok 10240
1/6 ซอยรามคำแหง 145 แขวงสะพานสูง เขตสะพานสูง กรุงเทพมหานคร 10240

E-mail : TH08_Contact@eurofinsasia.com
Tel : 0-2373-7799 (Auto) Fax : 0-2373-7979

TEST REPORT

Customer Name : บริษัท ชิน เคอ หยวน จำกัด
Project : โครงการโรงงานผลิตเหล็กแผ่น เหล็กรูปพรรณ และเหล็กลวด
Address : 666 หมู่ 2 ตำบลตาสิทธิ์ อำเภอปลวกแดง
จังหวัดระยอง 21140
T. (033) 684 290-7 F. (033) 684 298-9
Job No. : S690658/June

Report No. : 2474/2026/1-7
Report Date : July 3, 2026
Sampling Date : June 19-26, 2026
Type of Sample : WS & WD

Item	Time	บ้านเฉลิมลาภ (A1)													
		19-20/06/26		20-21/06/26		21-22/06/26		22-23/06/26		23-24/06/26		24-25/06/26		25-26/06/26	
		WS	WD	WS	WD	WS	WD	WS	WD	WS	WD	WS	WD	WS	WD
1.	14:00-15:00	0.9	NW	0.9	NW	0.0	NW	0.9	NW	0.9	WNW	0.9	SW	0.4	WNW
2.	15:00-16:00	1.3	N	0.4	NW	0.0	NW	0.4	W	0.9	WSW	0.4	WSW	0.0	WSW
3.	16:00-17:00	0.4	N	0.0	NW	0.4	NW	0.0	WNW	0.4	WSW	0.4	SW	0.0	SSW
4.	17:00-18:00	0.4	N	0.0	NW	0.9	N	0.0	WNW	0.0	WSW	0.4	WSW	0.0	SSW
5.	18:00-19:00	0.0	N	0.0	NW	0.9	W	0.0	WNW	0.0	WSW	0.0	WSW	0.0	SSW
6.	19:00-20:00	0.4	N	0.0	N	0.9	N	0.0	WNW	0.0	WSW	0.0	WSW	0.0	SSW
7.	20:00-21:00	0.0	N	0.0	N	0.0	WSW	0.0	WNW	0.0	WSW	0.0	WSW	0.0	SSW
8.	21:00-22:00	0.0	N	0.0	N	0.0	WSW	0.0	WNW	0.0	WSW	0.0	WSW	0.0	WSW
9.	22:00-23:00	0.0	N	0.4	WSW	0.0	WNW	0.0	WNW	0.0	WSW	0.0	WSW	0.0	N
10.	23:00-00:00	0.9	N	0.4	WSW	0.0	WNW	0.0	WNW	0.0	WSW	0.0	WSW	0.0	N
11.	00:00-01:00	1.3	N	0.4	WSW	0.0	WNW	0.0	WNW	0.0	WSW	0.0	WSW	0.0	N
12.	01:00-02:00	0.4	N	0.0	N	0.0	WNW	0.0	WNW	0.0	WSW	0.0	WSW	0.0	N
13.	02:00-03:00	0.4	N	0.0	N	0.0	WNW	0.0	WNW	0.0	WSW	0.0	WSW	0.0	N
14.	03:00-04:00	0.9	NW	0.0	N	0.0	WNW	0.0	WNW	0.0	WSW	0.0	WSW	0.0	N
15.	04:00-05:00	1.3	N	0.0	N	0.0	WNW	0.0	WNW	0.0	WSW	0.0	WSW	0.0	N
16.	05:00-06:00	0.4	N	0.0	N	0.0	WNW	0.0	WNW	0.0	NE	0.0	WSW	0.0	N
17.	06:00-07:00	0.4	N	0.0	N	0.0	WNW	0.0	WNW	0.0	N	0.0	WSW	0.0	N
18.	07:00-08:00	0.0	WNW	0.0	N	0.0	WNW	0.4	NNE	0.4	N	0.0	WSW	0.0	N
19.	08:00-09:00	0.0	WNW	0.4	N	0.0	W	0.4	NNW	0.9	WNW	0.0	NW	0.4	SW
20.	09:00-10:00	0.0	WNW	0.4	N	0.4	SW	0.4	NE	0.4	WNW	0.9	N	0.4	N
21.	10:00-11:00	0.0	W	0.4	WNW	0.4	WNW	0.4	NNW	0.4	WSW	0.4	NW	0.9	WNW
22.	11:00-12:00	0.9	WSW	0.9	N	0.9	WNW	0.9	WNW	0.4	WSW	0.4	W	0.9	SW
23.	12:00-13:00	0.9	NW	0.9	W	0.4	WNW	0.9	WNW	1.3	W	0.4	N	0.9	WNW
24.	13:00-14:00	1.3	NW	0.9	N	0.9	W	0.9	NW	0.9	SSW	0.4	N	0.9	SW
-	Average	0.5	-	0.3	-	0.3	-	0.2	-	0.3	-	0.2	-	0.2	-


Remark : WS = WIND SPEED (m/s)
WD = WIND DIRECTION

Pramual M.
Pramual Moonsarn



Wannasiri S.
Wannasiri Suriyawong

- REPORTED RESULTS REFER TO SUBMITTED SAMPLE(S) ONLY
- DO NOT COPY PARTIAL OF THIS ANALYSIS REPORT WITHOUT OFFICIAL APPROVAL

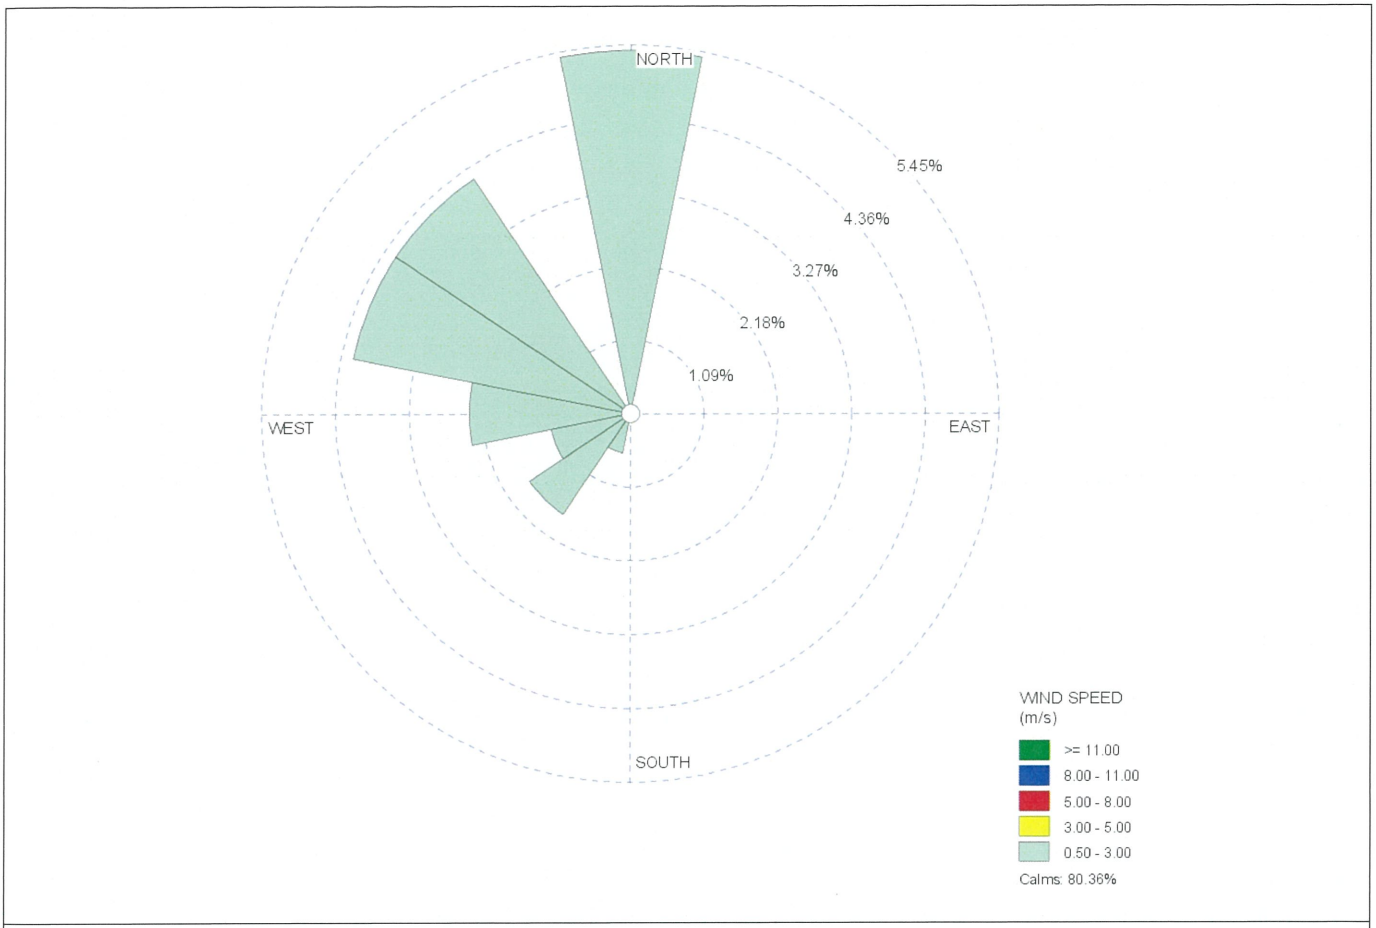

ผังแสดงความเร็วลมและทิศทางลม บริเวณบ้านเฉลิมลาภ (A1)

ระหว่างวันที่ 19-26 มิถุนายน 2569

Thai Environmental Technic Limited
บริษัท เทคนิคสิ่งแวดล้อมไทย จำกัด

1/6 Soi Ramkhamhaeng 145, Khwaeng / Khet Saphansung, Bangkok 10240
1/6 ซอยรามคำแหง 145 แขวงสะพานสูง เขตสะพานสูง กรุงเทพมหานคร 10240

E-mail : TH08_Contact@eurofinsasia.com
Tel : 0-2373-7799 (Auto) Fax : 0-2373-7979

TEST REPORT

Customer Name : บริษัท ชิน เคอ หยวน จำกัด
Project : โครงการโรงงานผลิตเหล็กแผ่น เหล็กรูปพรรณ และเหล็กลวด
Address : 666 หมู่ 2 ตำบลตาสิทธิ์ อำเภอปลวกแดง
T. (033) 684 290-7 F. (033) 684 298-9
Job No. : S690658/June

Report No. : 2474/2026/2-7
Report Date : July 3, 2026
Sampling Date : June 19-26, 2026
Type of Sample : Sound Level

Item	Time	Result dB(A) บ้านเฉลิมลาภ (N1)											
		19-20/06/26			20-21/06/26			21-22/06/26			22-23/06/26		
		Leq	Lmax	L_{90}	Leq	Lmax	L_{90}	Leq	Lmax	L_{90}	Leq	Lmax	L_{90}
1.	13.00-14.00	52.9	69.3	44.7	54.6	69.9	53.2	54.6	69.3	52.7	54.1	67.5	52.5
2.	14.00-15.00	54.5	67.4	52.8	55.5	71.5	53.8	54.5	69.0	53.2	54.1	69.8	52.7
3.	15.00-16.00	55.7	67.8	53.8	55.0	74.1	53.6	53.4	70.1	51.8	53.0	66.2	51.3
4.	16.00-17.00	55.9	68.4	54.1	52.9	64.1	51.7	52.8	71.4	49.9	53.0	69.6	51.3
5.	17.00-18.00	53.9	64.1	51.8	54.4	68.9	53.2	54.0	72.4	52.1	52.9	64.4	50.5
6.	18.00-19.00	54.9	63.3	53.3	53.5	75.9	50.1	50.9	60.2	48.2	52.3	63.3	48.9
7.	19.00-20.00	55.0	63.8	53.4	53.1	72.5	49.0	53.7	65.9	51.6	54.1	62.2	52.3
8.	20.00-21.00	54.5	58.0	53.5	55.3	65.7	53.4	54.7	64.9	52.7	54.2	64.6	52.4
9.	21.00-22.00	54.9	64.9	53.4	54.9	61.6	53.6	55.2	61.6	53.2	53.8	62.2	52.3
10.	22.00-23.00	54.7	61.5	52.7	55.0	64.3	53.1	54.0	63.1	52.5	52.9	60.9	50.6
11.	23.00-00.00	54.7	66.9	53.0	54.3	64.3	51.9	52.7	62.1	50.0	53.8	62.7	52.2
12.	00.00-01.00	53.5	61.5	50.8	54.0	69.9	52.7	54.4	63.8	52.6	55.0	64.7	53.1
13.	01.00-02.00	54.9	63.7	53.1	54.5	62.9	52.8	54.9	66.6	53.8	53.8	62.6	52.4
14.	02.00-03.00	54.5	62.0	52.8	55.1	63.2	53.5	54.0	63.8	52.1	52.0	60.7	50.2
15.	03.00-04.00	54.3	61.3	52.7	53.3	62.4	51.3	51.3	64.3	47.9	46.7	62.5	45.9
16.	04.00-05.00	52.2	59.9	48.5	49.8	58.0	47.3	52.4	64.2	49.7	51.9	63.2	50.2
17.	05.00-06.00	52.4	61.2	49.5	53.1	64.6	51.1	52.3	60.6	50.6	50.8	63.0	48.9
18.	06.00-07.00	52.9	66.0	50.3	51.6	63.9	48.2	51.0	64.6	48.3	49.2	66.1	46.4
19.	07.00-08.00	50.2	65.8	48.0	51.7	73.9	48.2	54.6	71.6	51.8	54.6	72.0	52.7
20.	08.00-09.00	55.0	73.4	52.7	56.1	72.6	53.9	55.0	69.5	52.9	54.5	73.5	52.6
21.	09.00-10.00	56.1	73.2	53.6	55.9	73.6	53.4	54.8	71.9	52.8	53.5	65.6	50.9
22.	10.00-11.00	54.0	72.6	52.5	54.7	78.6	52.4	54.1	65.4	52.2	59.9	85.6	51.0
23.	11.00-12.00	55.9	74.8	54.1	61.3	89.0	51.9	53.1	67.0	51.7	51.4	57.6	49.8
24.	12.00-13.00	53.9	70.9	50.7	52.1	67.4	50.0	53.0	66.2	50.5	52.6	58.6	51.4
Leq 24 hr		54.4	-	-	54.9	-	-	53.7	-	-	53.7	-	-
Lmax		-	74.8	-	-	89.0	-	-	72.4	-	-	85.6	-
Standard[(1)(2)]		70	115	-	70	115	-	70	115	-	70	115	-
Ldn		60.4	-	-	60.4	-	-	59.7	-	-	59.1	-	-

Standard : (1) Notification of the National Environment No. 15 (1997)(B.E. 2540)
(2) Notification of the Ministry of Industry (2005)(B.E. 2548)

Pramual Moonsarn

Wannasiri Suriyawong

- REPORTED RESULTS REFER TO SUBMITTED SAMPLE(S) ONLY
- DO NOT COPY PARTIAL OF THIS ANALYSIS REPORT WITHOUT OFFICIAL APPROVAL

Thai Environmental Technic Limited
บริษัท เทคนิคสิ่งแวดล้อมไทย จำกัด

1/6 Soi Ramkhamhaeng 145, Khwaeng / Khet Saphansung, Bangkok 10240 E-mail : TH08_Contact@eurofinsasia.com
1/6 ซอยรามคำแหง 145 แขวงสะพานสูง เขตสะพานสูง กรุงเทพมหานคร 10240 Tel : 0-2373-7799 (Auto) Fax : 0-2373-7979

TEST REPORT

Customer Name : บริษัท ชิน เคอ หยวน จำกัด
Project : โครงการโรงงานผลิตเหล็กแผ่น เหล็กรูปพรรณ และเหล็กลวด
Address : 666 หมู่ 2 ตำบลตาสิทธิ์ อำเภอปลวกแดง
T. (033) 684 290-7 F. (033) 684 298-9
Job No. : S690658/June

Report No. : 2474/2026/3-7
Report Date : July 3, 2026
Sampling Date : June 19-26, 2026
Type of Sample : Sound Level

Item	Time	Result dB(A) บ้านเฉลิมลาภ (N1)								
		23-24/06/26			24-25/06/26			25-26/06/26		
		Leq	Lmax	L_{90}	Leq	Lmax	L_{90}	Leq	Lmax	L_{90}
1.	13.00-14.00	52.4	63.1	51.2	51.8	66.7	49.6	55.4	66.7	51.4
2.	14.00-15.00	52.0	65.6	50.8	51.5	60.1	50.2	51.0	59.8	48.5
3.	15.00-16.00	51.3	58.5	49.5	51.3	64.3	49.3	50.7	62.4	48.3
4.	16.00-17.00	51.2	62.3	49.8	51.3	60.3	50.0	50.5	71.9	48.3
5.	17.00-18.00	49.5	55.6	47.3	49.4	57.8	47.0	50.3	63.2	47.6
6.	18.00-19.00	50.0	58.6	48.0	50.8	62.5	49.0	53.5	62.0	51.8
7.	19.00-20.00	51.4	65.6	49.7	51.6	60.3	50.0	54.3	63.4	52.6
8.	20.00-21.00	51.2	64.5	50.1	51.9	59.1	50.6	54.1	62.9	52.7
9.	21.00-22.00	51.4	57.2	50.0	51.9	57.1	50.7	51.9	63.8	49.8
10.	22.00-23.00	51.3	57.8	49.3	51.0	57.6	48.8	51.6	63.9	49.9
11.	23.00-00.00	51.2	62.9	49.8	52.0	62.9	50.4	53.7	65.3	52.0
12.	00.00-01.00	50.9	66.1	49.3	51.2	58.1	49.5	53.8	66.2	51.7
13.	01.00-02.00	52.0	59.9	50.5	50.4	58.3	48.5	52.9	63.2	51.9
14.	02.00-03.00	50.3	60.0	48.0	47.0	52.9	45.9	46.4	59.2	45.7
15.	03.00-04.00	50.5	65.0	47.6	46.9	52.9	45.8	46.6	63.5	42.8
16.	04.00-05.00	51.6	59.3	50.0	49.8	56.8	48.7	48.4	67.1	43.9
17.	05.00-06.00	51.0	57.6	49.0	49.1	55.4	48.0	49.8	65.8	44.7
18.	06.00-07.00	50.3	58.5	48.5	50.3	60.8	48.3	47.4	71.3	43.8
19.	07.00-08.00	51.4	65.4	50.0	52.5	61.3	50.4	52.6	72.7	43.9
20.	08.00-09.00	52.1	66.9	50.0	55.3	73.2	50.4	53.1	66.0	51.2
21.	09.00-10.00	51.7	58.8	49.8	57.6	69.9	50.6	53.3	66.9	51.7
22.	10.00-11.00	52.3	62.6	50.8	55.3	62.9	52.0	51.2	70.8	47.5
23.	11.00-12.00	50.1	62.4	47.3	47.2	54.8	45.2	55.5	74.2	47.6
24.	12.00-13.00	52.5	65.8	50.9	54.8	71.4	50.6	53.2	69.3	46.3
Leq 24 hr		51.3	-	-	52.1	-	-	52.4	-	-
Lmax		-	66.9	-	-	73.2	-	-	74.2	-
Standard[1][2]		70	115	-	70	115	-	70	115	-
Ldn		57.5	-	-	57.0	-	-	57.7	-	-

Standard : [1] Notification of the National Environment No. 15 (1997)(B.E. 2540)
[2] Notification of the Ministry of Industry (2005)(B.E. 2548)

Pramual M.
Pramual Moonsarn

Wannasiri S.
Wannasiri Suriyawong

- REPORTED RESULTS REFER TO SUBMITTED SAMPLE(S) ONLY
- DO NOT COPY PARTIAL OF THIS ANALYSIS REPORT WITHOUT OFFICIAL APPROVAL

Thai Environmental Technic Limited
บริษัท เทคนิคสิ่งแวดล้อมไทย จำกัด

1/6 Soi Ramkhamhaeng 145, Khwaeng / Khet Saphansung, Bangkok 10240
1/6 ซอยรามคำแหง 145 แขวงสะพานสูง เขตสะพานสูง กรุงเทพมหานคร 10240

E-mail : TH08_Contact@eurofinsasia.com
Tel : 0-2373-7799 (Auto) Fax : 0-2373-7979

TEST REPORT

Customer Name : บริษัท ชิน เคอ หยวน จำกัด
Project : โครงการโรงงานผลิตเหล็กแผ่น เหล็กรูปพรรณ และเหล็กลวด
Address : 666 หมู่ 2 ตำบลตาสิทธิ์ อำเภอปลวกแดง
T. (033) 684 290-7 F. (033) 684 298-9
Job No. : S690658/June

Report No. : 2474/2026/4-7
Report Date : July 3, 2026
Sampling Date : June 19-26, 2026
Type of Sample : Sound Level

Item	Time	Result dB(A) บ้านเขาระฆัง (N2)											
		19-20/06/26			20-21/06/26			21-22/06/26			22-23/06/26		
		Leq	Lmax	L_{90}	Leq	Lmax	L_{90}	Leq	Lmax	L_{90}	Leq	Lmax	L_{90}
1.	11.00-12.00	55.8	77.4	43.7	58.1	85.7	46.4	54.0	70.6	45.9	59.6	85.5	53.5
2.	12.00-13.00	55.9	76.1	44.3	55.5	78.0	46.9	52.2	67.0	44.0	59.4	76.9	50.9
3.	13.00-14.00	54.4	73.5	46.8	54.7	75.9	44.4	52.0	69.0	45.6	60.2	84.7	49.2
4.	14.00-15.00	55.3	69.1	50.3	55.1	76.8	44.0	47.9	70.5	43.2	52.1	75.1	46.2
5.	15.00-16.00	57.0	66.9	55.9	54.2	77.3	43.9	52.1	63.7	45.1	52.2	73.5	46.7
6.	16.00-17.00	51.8	66.2	43.3	55.4	77.4	44.7	53.7	67.7	46.4	50.5	77.7	45.1
7.	17.00-18.00	54.6	67.7	51.1	55.3	74.2	47.6	55.8	78.7	46.2	48.7	66.6	45.1
8.	18.00-19.00	51.1	59.5	43.0	53.8	69.2	45.6	50.4	64.0	45.6	48.9	67.4	45.7
9.	19.00-20.00	46.3	59.7	42.1	52.8	62.1	43.8	53.3	70.4	47.0	48.5	63.7	46.4
10.	20.00-21.00	48.5	71.4	40.9	53.4	69.5	47.9	52.8	70.1	45.0	47.0	60.3	45.1
11.	21.00-22.00	46.7	67.4	42.2	47.2	60.1	42.7	50.0	69.8	44.1	46.7	64.1	44.0
12.	22.00-23.00	46.6	70.6	42.2	46.4	70.2	40.8	50.9	70.8	45.7	47.6	64.4	45.0
13.	23.00-00.00	46.9	72.6	40.1	52.2	61.3	45.0	49.4	62.2	45.2	45.6	56.8	43.8
14.	00.00-01.00	45.9	66.9	40.4	47.0	59.8	44.2	53.3	71.0	44.2	47.6	65.2	43.9
15.	01.00-02.00	45.5	62.2	42.1	52.0	69.2	48.4	53.1	73.5	41.9	46.3	64.9	42.1
16.	02.00-03.00	46.0	68.9	40.8	47.3	61.2	43.1	53.7	73.4	40.7	50.0	69.7	44.3
17.	03.00-04.00	45.7	65.8	40.4	46.8	62.3	41.7	47.6	70.3	41.0	53.5	89.9	46.0
18.	04.00-05.00	50.9	73.0	39.8	51.1	72.0	40.6	46.2	68.7	39.3	57.2	89.5	47.6
19.	05.00-06.00	55.4	75.3	39.7	52.3	73.2	38.5	50.8	74.5	44.6	56.2	85.5	51.8
20.	06.00-07.00	55.7	76.5	42.2	50.8	74.6	43.7	50.4	73.7	45.5	58.6	80.9	49.3
21.	07.00-08.00	57.2	77.4	43.7	46.8	61.4	42.6	53.3	73.1	47.5	57.3	79.5	53.3
22.	08.00-09.00	60.5	85.3	46.0	51.0	72.6	43.2	56.1	75.8	43.8	56.9	74.0	53.3
23.	09.00-10.00	62.0	81.5	45.5	51.8	75.7	42.5	54.9	75.9	44.0	56.4	79.9	51.5
24.	10.00-11.00	61.7	81.1	45.9	54.7	73.5	48.3	59.0	86.6	51.4	54.1	72.8	49.4
Leq 24 hr		55.4	-	-	53.0	-	-	53.1	-	-	54.9	-	-
Lmax		-	85.3	-	-	85.7	-	-	86.6	-	-	89.9	-
Standard[1][2]		70	115	-	70	115	-	70	115	-	70	115	-
Ldn		58.8	-	-	57.4	-	-	58.1	-	-	60.5	-	-

Standard : [1] Notification of the National Environment No. 15 (1997)(B.E. 2540)
[2] Notification of the Ministry of Industry (2005)(B.E. 2548)

Pramual Moonsarn

Wannasiri Suriyawong

- REPORTED RESULTS REFER TO SUBMITTED SAMPLE(S) ONLY
- DO NOT COPY PARTIAL OF THIS ANALYSIS REPORT WITHOUT OFFICIAL APPROVAL

Thai Environmental Technic Limited
บริษัท เทคนิคสิ่งแวดล้อมไทย จำกัด

1/6 Soi Ramkhamhaeng 145, Khwaeng / Khet Saphansung, Bangkok 10240
1/6 ซอยรามคำแหง 145 แขวงสะพานสูง เขตสะพานสูง กรุงเทพมหานคร 10240

E-mail : TH08_Contact@eurofinsasia.com
Tel : 0-2373-7799 (Auto) Fax : 0-2373-7979

TEST REPORT

Customer Name : บริษัท ชิน เคอ หยวน จำกัด
Project : โครงการโรงงานผลิตเหล็กแผ่น เหล็กรูปพรรณ และเหล็กลวด
Address : 666 หมู่ 2 ตำบลตาสิทธิ์ อำเภอปลวกแดง
T. (033) 684 290-7 F. (033) 684 298-9
Job No. : S690658/June

Report No. : 2474/2026/5-7
Report Date : July 3, 2026
Sampling Date : June 19-26, 2026
Type of Sample : Sound Level

Item	Time	Result dB(A) บ้านเขาระฆัง (N2)								
		23-24/06/26			24-25/06/26			25-26/06/26		
		Leq	Lmax	L_{90}	Leq	Lmax	L_{90}	Leq	Lmax	L_{90}
1.	11.00-12.00	55.7	70.6	52.7	56.5	74.8	46.1	53.0	70.3	46.5
2.	12.00-13.00	56.1	83.3	49.6	54.1	72.4	46.1	51.4	68.7	45.7
3.	13.00-14.00	58.2	77.0	50.5	53.5	72.5	46.9	49.6	63.2	44.9
4.	14.00-15.00	51.4	73.6	44.9	54.2	76.3	46.4	53.8	73.5	47.6
5.	15.00-16.00	52.6	76.7	45.5	49.1	66.0	43.8	52.6	66.6	46.0
6.	16.00-17.00	49.5	65.6	46.1	47.2	67.7	43.0	51.8	70.8	44.8
7.	17.00-18.00	49.6	65.0	46.8	51.4	65.6	44.0	50.8	71.1	44.4
8.	18.00-19.00	48.9	64.6	45.7	54.6	71.2	44.9	48.4	62.7	42.8
9.	19.00-20.00	49.5	65.3	46.5	51.4	66.5	47.6	51.5	69.3	44.0
10.	20.00-21.00	47.3	64.0	44.3	53.5	70.7	45.6	52.7	72.7	45.5
11.	21.00-22.00	46.0	62.3	43.8	51.1	72.1	46.6	52.2	73.8	44.2
12.	22.00-23.00	47.9	64.2	45.7	51.0	66.8	44.1	51.9	72.4	45.3
13.	23.00-00.00	46.7	63.6	44.3	53.7	73.0	45.0	52.7	63.6	49.1
14.	00.00-01.00	46.8	64.7	44.1	51.3	66.2	47.1	52.9	71.4	45.0
15.	01.00-02.00	48.8	65.5	45.7	49.7	69.0	43.0	54.6	71.7	44.2
16.	02.00-03.00	56.6	89.7	47.1	53.6	72.8	43.1	52.8	70.7	46.0
17.	03.00-04.00	52.3	70.1	45.9	51.7	70.5	44.0	53.3	74.1	46.4
18.	04.00-05.00	52.8	75.9	46.0	52.3	67.7	45.1	55.6	77.4	47.4
19.	05.00-06.00	53.1	81.3	47.6	52.5	74.1	42.5	53.6	74.3	46.4
20.	06.00-07.00	57.9	79.8	51.3	50.7	69.0	44.8	54.7	74.8	46.9
21.	07.00-08.00	54.6	72.6	49.0	52.8	71.5	44.0	50.6	71.6	44.6
22.	08.00-09.00	53.7	79.2	45.2	49.2	63.1	44.9	49.2	69.3	44.0
23.	09.00-10.00	52.8	81.1	42.7	55.3	74.1	43.4	55.8	77.2	43.0
24.	10.00-11.00	55.5	81.5	44.6	48.4	65.8	43.8	56.0	76.9	43.4
Leq 24 hr		53.3	-	-	52.6	-	-	53.0	-	-
Lmax		-	89.7	-	-	76.3	-	-	77.4	-
Standard[1][2]		70	115	-	70	115	-	70	115	-
Ldn		59.6	-	-	58.6	-	-	60.0	-	-

Standard : [1] Notification of the National Environment No. 15 (1997)(B.E. 2540)
[2] Notification of the Ministry of Industry (2005)(B.E. 2548)

Pramual Moonsarn

Wannasiri Suriyawong

- REPORTED RESULTS REFER TO SUBMITTED SAMPLE(S) ONLY
- DO NOT COPY PARTIAL OF THIS ANALYSIS REPORT WITHOUT OFFICIAL APPROVAL

Thai Environmental Technic Limited
บริษัท เทคนิคสิ่งแวดล้อมไทย จำกัด

1/6 Soi Ramkhamhaeng 145, Khwaeng / Khet Saphansung, Bangkok 10240
1/6 ซอยรามคำแหง 145 แขวงสะพานสูง เขตสะพานสูง กรุงเทพมหานคร 10240

E-mail : TH08_Contact@eurofinsasia.com
Tel : 0-2373-7799 (Auto) Fax : 0-2373-7979

TEST REPORT

Customer Name : บริษัท ซิน เคอ หยวน จำกัด
Project : โครงการโรงงานผลิตเหล็กแผ่น เหล็กรูปพรรณ และเหล็กลวด
Address : 666 หมู่ 2 ตำบลตาสิทธิ์ อำเภอปลวกแดง
T. (033) 684 290-7 F. (033) 684 298-9
Job No. : S690658/June

Report No. : 2474/2026/6-7
Report Date : July 3, 2026
Sampling Date : June 19-26, 2026
Type of Sample : เสียงรบกวน

Item	Sampling Date	Time	Result (dB(A))				
			บ้านเฉลิมลาภ (N1)				
			ระดับเสียงขณะเกิดเสียงของแหล่งกำเนิด (Leq)	ระดับเสียงขณะไม่มีการรบกวน (Leq)	ระดับเสียงขณะมีการรบกวน	ระดับเสียงพื้นฐาน (L_{90})	ค่าระดับการรบกวน
1.	19-20/06/26	06.00-22.00	50.2-56.1	49.0-58.0	40.4-54.0	46.4-52.9	-11.6-7.3
		22.00-06.00	49.1-57.2	48.4-55.3	37.8-58.6	45.9-53.7	-11.9-12.2
2.	20-21/06/26	06.00-22.00	51.6-61.3	50.3-60.7	37.1-60.4	47.5-53.5	-14.9-8.8
		22.00-06.00	48.8-58.1	47.1-55.8	40.4-59.7	45.1-54.3	-12.1-12.4
3.	21-22/06/26	06.00-22.00	50.9-55.2	49.2-54.7	42.2-53.1	47.3-52.4	-9.1-5.8
		22.00-06.00	47.9-56.2	47.7-55.3	42.4-58.2	45.4-53.9	-7.1-12.1
4.	22-23/06/26	06.00-22.00	49.2-59.9	49.3-57.4	41.7-59.0	46.2-51.9	-8.0-9.1
		22.00-06.00	45.0-56.5	43.8-54.9	41.7-58.3	43.2-53.5	-7.1-12.1
5.	23-24/06/26	06.00-22.00	49.5-52.5	48.5-52.1	41.6-52.0	46.0-50.7	-8.9-1.5
		22.00-06.00	47.5-53.7	47.2-53.0	34.1-54.3	44.7-51.1	-11.5-8.7
6.	24-25/06/26	06.00-22.00	47.2-57.6	47.8-59.9	33.0-57.6	45.4-53.6	-14.1-7.6
		22.00-06.00	44.4-53.1	43.8-52.5	34.4-53.5	43.5-50.6	-12.1-6.6
7.	25-26/06/26	06.00-22.00	47.4-55.5	46.0-54.5	41.6-53.9	42.5-41.9	-6.0-9.0
		22.00-06.00	44.6-56.3	43.8-54.8	36.9-57.7	40.3-53.3	-7.9-11.7
Standard[1][2]							10

Standard : [1] Notification of the National Environment Board No. 29 (2007) (B.E. 2550)
[2] Notification of the Ministry of Industry (2005) (B.E. 2548)

Pramual M.
Pramual Moonsarn

Wannasiri S.
Wannasiri Suriyawong

- REPORTED RESULTS REFER TO SUBMITTED SAMPLE(S) ONLY
- DO NOT COPY PARTIAL OF THIS ANALYSIS REPORT WITHOUT OFFICIAL APPROVAL

Thai Environmental Technic Limited
บริษัท เทคนิคสิ่งแวดล้อมไทย จำกัด

1/6 Soi Ramkhamhaeng 145, Khwaeng / Khet Saphansung, Bangkok 10240 E-mail : TH08_Contact@eurofinsasia.com
1/6 ซอยรามคำแหง 145 แขวงสะพานสูง เขตสะพานสูง กรุงเทพมหานคร 10240 Tel : 0-2373-7799 (Auto) Fax : 0-2373-7979

TEST REPORT

Customer Name : บริษัท ชิน เคอ หยวน จำกัด
Project : โครงการโรงงานผลิตเหล็กแผ่น เหล็กรูปพรรณ และเหล็กลวด
Address : 666 หมู่ 2 ตำบลตาสิทธิ์ อำเภอปลวกแดง
T. (033) 684 290-7 F. (033) 684 298-9
Job No. : S690658/June

Report No. : 2474/2026/7-7
Report Date : July 3, 2026
Sampling Date : June 19-26, 2026
Type of Sample : เสียงรบกวน

Item	Sampling Date	Time	Result (dB(A)) บ้านเขาระมัง (N2) ระดับเสียงขณะเกิดเสียงของแหล่งกำเนิด (Leq)	ระดับเสียงขณะไม่มีการรบกวน (Leq)	ระดับเสียงขณะมีการรบกวน	ระดับเสียงพื้นฐาน (L_{90})	ค่าระดับการรบกวน
1.	19-20/06/26	06.00-22.00	46.3-62.0	44.0-59.3	41.6-58.7	40.1-53.1	0.0-15.3
		22.00-06.00	40.6-57.5	38.2-56.2	30.5-58.6	35.5-44.9	-10.5-19.3
2.	20-21/06/26	06.00-22.00	46.8-58.1	44.3-54.9	43.1-55.3	40.0-46.0	3.1-11.3
		22.00-06.00	40.4-57.6	38.6-56.0	32.4-59.4	34.9-55.6	-6.9-19.0
3.	21-22/06/26	06.00-22.00	47.9-59.0	44.9-56.4	43.8-55.5	41.0-48.1	2.2-12.2
		22.00-06.00	41.5-58.2	38.8-55.1	37.3-60.3	35.2-53.7	-6.6-19.4
4.	22-23/06/26	06.00-22.00	46.7-60.2	44.6-58.1	42.5-57.8	41.6-51.7	0.6-11.7
		22.00-06.00	41.4-61.9	39.9-61.4	32.663.3	38.1-52.2	-10.8-17.3
5.	23-24/06/26	06.00-22.00	46.0-58.2	44.2-55.4	41.3-55.5	40.5-49.0	-0.5-9.1
		22.00-06.00	43.4-61.5	40.5-62.5	35.8-61.5	39.5-53.0	-5.8-16.8
6.	24-25/06/26	06.00-22.00	47.2-56.5	45.9-52.9	41.3-54.1	40.7-45.4	0.6-10.6
		22.00-06.00	44.6-58.9	40.7-58.3	40.7-61.3	37.8-48.3	-3.4-19.3
7.	25-26/06/26	06.00-22.00	48.4-56.0	46.1-53.6	44-5.52.7	39.9-44.8	2.7-11.7
		22.00-06.00	47.0-58.4	45.1-56.9	37.3-60.9	39.0-49.3	-7.7-18.2
Standard[1][2]							10

Standard : [1] Notification of the National Environment Board No. 29 (2007) (B.E. 2550)
[2] Notification of the Ministry of Industry (2005) (B.E. 2548)

Pramual M.
Pramual Moonsarn

Thai Environmental Technic Limited

Wannasiri S.
Wannasiri Suriyawong

- REPORTED RESULTS REFER TO SUBMITTED SAMPLE(S) ONLY
- DO NOT COPY PARTIAL OF THIS ANALYSIS REPORT WITHOUT OFFICIAL APPROVAL

Thai Environmental Technic Limited
บริษัท เทคนิคสิ่งแวดล้อมไทย จำกัด

NSC-TISI-TIS 17025
TESTING 0412

1/6 Soi Ramkhamhaeng 145, Khwaeng / Khet Saphansung, Bangkok 10240
1/6 ซอยรามคำแหง 145 แขวงสะพานสูง เขตสะพานสูง กรุงเทพมหานคร 10240
E-mail : TH08_Contact@eurofins
Tel : 0-2373-7799 (Auto) Fax : 0-2373-7979

TEST REPORT

Analysis No. : R26-2474
Received Date : 26/06/26
Customer : Technical Division of Thai Environmental Technic Limited
For บริษัท ซิน เคอ หยวน จำกัด
โครงการโรงงานผลิตเหล็กแผ่น เหล็กรูปพรรณ และเหล็กลวด
Address : เลขที่ 666 หมู่ 2 ตำบลตาสิทธิ์ อำเภอปลวกแดง จังหวัดระยอง 21140
Contact : Tel. (033) 684 290-7 Fax. (033) 684 298-9

Report Date : 03/07/26
Analysis Date : 25/06-02/07/26
Job No. : S690658/June
Sampling Date * : 25/06/26
Sampling By * : TET
Type of Sample : Surface Water

Sample Conditions : 2606-WF1087 = yellow turbid/slight black sediment

Item	Parameter	Unit	Method	Result 2606-WF1087 คลองมาบไข่เน่า (SW2)	Standard	Analysis Date
1	pH *	-	Electrometric Method (SM 4500 B)	8.11	5.0-9.0	25/06/26
2	DO *	mg/L	Membrane Electrode (SM 4500 G)	2.34	≥ 4.0	25/06/26
3	BOD *	mg/L	5-Days BOD Test, Azide Modification Method (SM 5210B)	2.5	2.0	26/06-01/07/26
4	Total Hardness *	mg/L as $CaCO_3$	EDTA Titrimetric (SM 2340 C)	168.0	-	30/06/26
5	NO_3 *	mg/L	Cadmium Reduction (SM 4500-NO_3 E)	2.14	5.0	30/06/26
6	NH_3 *	mg/L	Distillation/Titrimetric Method (SM 4500-NH_3 C)	2.73	0.5	26/06/26
7	Cyanide *	mg/L	Distillation, Colorimetric Method (SM 4500-CN^- B/E)	< 0.001	0.005	29/06/26
8	Cr^{+6} *	mg/L	Filtration, Colorimetric Method (SM 3500-Cr B)	< 0.02	0.05	26/06/26
9	Pb *	mg/L	Digestion, Electrothermal AAS Method (SM 3030E and 3113B)	0.009	0.05	02/07/26
10	Cd *	mg/L	Digestion, Electrothermal AAS Method (SM 3030E and 3113B)	< 0.001	0.05(1)	29/06/26
11	Ni *	mg/L	Digestion, Electrothermal AAS Method (SM 3030E and 3113B)	< 0.010	0.1	30/06/26
12	Total Hg *	mg/L	Cold-Vapor AAS Method (SM 3112 B)	< 0.0005	0.002	01/07/26
13	As *	mg/L	Digestion, Continuous Hydride generation/AAS Method (SM 3114 C)	0.0083	0.01	26/06/26
14	Cu	mg/L	Digestion, ICP-OES Method (SM 3030F and 3120B)	< 0.05	0.1	30/06/26
15	Mn	mg/L	Digestion, ICP-OES Method (SM 3030F and 3120B)	0.54	1.0	30/06/26
16	Zn	mg/L	Digestion, ICP-OES Method (SM 3030F and 3120B)	< 0.04	1.0	30/06/26
17	Fecal Coliform Bacteria *	MPN/100 mL	Multiple-Tube Fermentation Technique (SM 9221 C&E)	1.4×10^3	4,000	26/06-01/07/26
18	Total Coliform Bacteria *	MPN/100 mL	Multiple-Tube Fermentation Technique (SM 9221 B&C)	2.4×10^4	20,000	26/06-01/07/26

Remarks * "Test marked "Not TISI Accredited" in this Report are not included in the TISI Accreditation Schedule for our Laboratory"
: คลองมาบไข่เน่า (SW2) = 47P 0744485 UTM 1445566
: BOD มีค่าปริมาณต่ำสุดที่สามารถรายงานเป็นตัวเลขได้ = 2 mg/L
Method : SM = Standard Method for the Examination of Water and Wastewater, APHA, AWWA, WEF, 24th Edition, 2023
Standard : Notification of the National Environment Board No. 8 (1994) (B.E. 2537), Class 3
(1) แคดเมียม (Cd) ในน้ำที่มีความกระด้างในรูปของ $CaCO_3$ ไม่เกินกว่า 100 มิลลิกรัมต่อลิตร มีค่าไม่เกินกว่า 0.005 มิลลิกรัมต่อลิตร และ ในน้ำที่มีความกระด้างในรูปของ $CaCO_3$ เกินกว่า 100 มิลลิกรัมต่อลิตร มีค่าไม่เกินกว่า 0.05 มิลลิกรัมต่อลิตร

Reviewed by
Ms. Wareerat Prachumdaeng
Chief of Laboratory
03/07/26

Approved by
Mrs. Porntip Pethshee
Laboratory Manager
03/07/26

- REPORTED RESULTS REFER TO SUBMITTED SAMPLE(S) ONLY
- DO NOT COPY PARTIAL OF THIS ANALYSIS REPORT WITHOUT OFFICIAL APPROVAL

Thai Environmental Technic Limited
บริษัท เทคนิคสิ่งแวดล้อมไทย จำกัด

NSC-TISI-TIS 17025
TESTING 0412

1/6 Soi Ramkhamhaeng 145, Khwaeng / Khet Saphansung, Bangkok 10240
1/6 ซอยรามคำแหง 145 แขวงสะพานสูง เขตสะพานสูง กรุงเทพมหานคร 10240

E-mail : TH08_Contact@eurofins
Tel : 0-2373-7799 (Auto) Fax : 0-2373-7979

TEST REPORT

Analysis No. : R26-2474
Received Date : 26/06/26
Customer : Technical Division of Thai Environmental Technic Limited
For บริษัท ซิน เคอ หยวน จำกัด
โครงการโรงงานผลิตเหล็กแผ่น เหล็กรูปพรรณ และเหล็กลวด
Address : เลขที่ 666 หมู่ 2 ตำบลตาสิทธิ์ อำเภอปลวกแดง จังหวัดระยอง 21140
Contact : Tel. (033) 684 290-7 Fax. (033) 684 298-9

Report Date : 03/07/26
Analysis Date : 25/06-02/07/26
Job No. : S690658/June
Sampling Date * : 25/06/26
Sampling By * : TET
Type of Sample : Surface Water

Sample Conditions : 2606-WF1088 = yellow turbid/slight black sediment

Item	Parameter	Unit	Method	Result 2606-WF1088 คลองงอแง (SW3)	Standard	Analysis Date
1	pH *	-	Electrometric Method (SM 4500 B)	8.16	5.0-9.0	25/06/26
2	DO *	mg/L	Membrane Electrode (SM 4500 G)	2.34	≥ 4.0	25/06/26
3	BOD *	mg/L	5-Days BOD Test, Azide Modification Method (SM 5210B)	2.8	2.0	26/06-01/07/26
4	Total Hardness *	mg/L as $CaCO_3$	EDTA Titrimetric (SM 2340 C)	62.0	-	30/06/26
5	NO_3 *	mg/L	Cadmium Reduction (SM 4500-NO_3 E)	2.19	5.0	30/06/26
6	NH_3 *	mg/L	Distillation/Titrimetric Method (SM 4500-NH_3 C)	0.27	0.5	26/06/26
7	Cyanide *	mg/L	Distillation, Colorimetric Method (SM 4500-CN^- B/E)	< 0.001	0.005	29/06/26
8	Cr^{+6} *	mg/L	Filtration, Colorimetric Method (SM 3500-Cr B)	< 0.02	0.05	26/06/26
9	Pb *	mg/L	Digestion, Electrothermal AAS Method (SM 3030E and 3113B)	0.008	0.05	02/07/26
10	Cd *	mg/L	Digestion, Electrothermal AAS Method (SM 3030E and 3113B)	< 0.001	0.005(1)	29/06/26
11	Ni *	mg/L	Digestion, Electrothermal AAS Method (SM 3030E and 3113B)	< 0.010	0.1	30/06/26
12	Total Hg *	mg/L	Cold-Vapor AAS Method (SM 3112 B)	< 0.0005	0.002	01/07/26
13	As *	mg/L	Digestion, Continuous Hydride generation/AAS Method (SM 3114 C)	0.0049	0.01	26/06/26
14	Cu	mg/L	Digestion, ICP-OES Method (SM 3030F and 3120B)	< 0.05	0.1	30/06/26
15	Mn	mg/L	Digestion, ICP-OES Method (SM 3030F and 3120B)	0.33	1.0	30/06/26
16	Zn	mg/L	Digestion, ICP-OES Method (SM 3030F and 3120B)	< 0.04	1.0	30/06/26
17	Fecal Coliform Bacteria *	MPN/100 mL	Multiple-Tube Fermentation Technique (SM 9221 C&E)	2.3×10^3	4,000	26/06-01/07/26
18	Total Coliform Bacteria *	MPN/100 mL	Multiple-Tube Fermentation Technique (SM 9221 B&C)	7.0×10^3	20,000	26/06-01/07/26

Remarks * "Test marked "Not TISI Accredited" in this Report are not included in the TISI Accreditation Schedule for our Laboratory"
: คลองงอแง (SW3) = 47P 0745268 UTM 1446468
: BOD มีค่าปริมาณต่ำสุดที่สามารถรายงานเป็นตัวเลขได้ = 2 mg/L
Method : SM = Standard Method for the Examination of Water and Wastewater, APHA, AWWA, WEF, 24th Edition, 2023
Standard : Notification of the National Environment Board No. 8 (1994) (B.E. 2537), Class 3
(1) แคดเมียม (Cd) ในน้ำที่มีความกระด้างในรูปของ $CaCO_3$ ไม่เกินกว่า 100 มิลลิกรัมต่อลิตร มีค่าไม่เกินกว่า 0.005 มิลลิกรัมต่อลิตร และ ในน้ำที่มีความกระด้างในรูปของ $CaCO_3$ เกินกว่า 100 มิลลิกรัมต่อลิตร มีค่าไม่เกินกว่า 0.05 มิลลิกรัมต่อลิตร

Reviewed by
Ms. Wareerat Prachumdaeng
Chief of Laboratory
03/07/26

Approved by
Mrs. Porntip Pethshee
Laboratory Manager
03/07/26

END OF REPORT

- REPORTED RESULTS REFER TO SUBMITTED SAMPLE(S) ONLY
- DO NOT COPY PARTIAL OF THIS ANALYSIS REPORT WITHOUT OFFICIAL APPROVAL

ภาคผนวก ง

กฎหมายที่เกี่ยวข้อง

ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ

เรื่อง กำหนดมาตรฐานคุณภาพอากาศในบรรยากาศโดยทั่วไป

พ.ศ. ๒๕๖๙

โดยที่เป็นการสมควรปรับปรุงการกำหนดมาตรฐานคุณภาพอากาศในบรรยากาศโดยทั่วไป ให้เหมาะสมตามความก้าวหน้าในทางวิทยาศาสตร์ เทคโนโลยี และความเปลี่ยนแปลงทางเศรษฐกิจและสังคมของประเทศ เพื่อเป็นเกณฑ์ทั่วไปสำหรับการส่งเสริมและรักษาคุณภาพสิ่งแวดล้อมตามพระราชบัญญัติส่งเสริมและรักษาคุณภาพสิ่งแวดล้อมแห่งชาติ พ.ศ. ๒๕๓๕

อาศัยอำนาจตามความในมาตรา ๓๒ (๔) และมาตรา ๓๔ แห่งพระราชบัญญัติส่งเสริมและรักษาคุณภาพสิ่งแวดล้อมแห่งชาติ พ.ศ. ๒๕๓๕ และตามคำสั่งสำนักนายกรัฐมนตรี ที่ ๓๐๒/๒๕๖๘ ลงวันที่ ๒๔ กันยายน พ.ศ. ๒๕๖๘ เรื่อง มอบหมายและมอบอำนาจให้รองนายกรัฐมนตรีและรัฐมนตรีประจำสำนักนายกรัฐมนตรี ปฏิบัติหน้าที่ประธานกรรมการ และมอบหมายให้รองนายกรัฐมนตรีและรัฐมนตรีประจำสำนักนายกรัฐมนตรีปฏิบัติหน้าที่ประธานกรรมการ รองประธานกรรมการและกรรมการในคณะกรรมการต่าง ๆ ตามกฎหมาย และระเบียบสำนักนายกรัฐมนตรี ประกอบกับมติคณะกรรมการสิ่งแวดล้อมแห่งชาติ ในการประชุมครั้งที่ ๕/๒๕๖๘ เมื่อวันที่ ๑๕ ตุลาคม พ.ศ. ๒๕๖๘ จึงออกประกาศไว้ ดังต่อไปนี้

ข้อ ๑ ให้ยกเลิก

๑.๑ ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ ฉบับที่ ๑๐ (พ.ศ. ๒๕๓๘) ออกตามความในพระราชบัญญัติส่งเสริมและรักษาคุณภาพสิ่งแวดล้อมแห่งชาติ พ.ศ. ๒๕๓๕ เรื่อง กำหนดมาตรฐานคุณภาพอากาศในบรรยากาศโดยทั่วไป ลงวันที่ ๑๗ เมษายน พ.ศ. ๒๕๓๘

๑.๒ ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ ฉบับที่ ๑๒ (พ.ศ. ๒๕๓๘) ออกตามความในพระราชบัญญัติส่งเสริมและรักษาคุณภาพสิ่งแวดล้อมแห่งชาติ พ.ศ. ๒๕๓๕ เรื่อง กำหนดมาตรฐานค่าก๊าซซัลเฟอร์ไดออกไซด์ในบรรยากาศโดยทั่วไป ในเวลา ๑ ชั่วโมง ลงวันที่ ๒๖ มิถุนายน พ.ศ. ๒๕๓๘

๑.๓ ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ ฉบับที่ ๒๑ (พ.ศ. ๒๕๔๔) ออกตามความในพระราชบัญญัติส่งเสริมและรักษาคุณภาพสิ่งแวดล้อมแห่งชาติ พ.ศ. ๒๕๓๕ เรื่อง กำหนดมาตรฐานค่าก๊าซซัลเฟอร์ไดออกไซด์ในบรรยากาศโดยทั่วไป ในเวลา ๑ ชั่วโมง ลงวันที่ ๙ เมษายน พ.ศ. ๒๕๔๔

๑.๔ ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ ฉบับที่ ๒๔ (พ.ศ. ๒๕๔๗) เรื่อง กำหนดมาตรฐานคุณภาพอากาศในบรรยากาศโดยทั่วไป ลงวันที่ ๙ สิงหาคม พ.ศ. ๒๕๔๗

๑.๕ ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ ฉบับที่ ๒๘ (พ.ศ. ๒๕๕๐) เรื่อง กำหนดมาตรฐานคุณภาพอากาศในบรรยากาศโดยทั่วไป ลงวันที่ ๑๐ เมษายน พ.ศ. ๒๕๕๐

๑.๖ ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ ฉบับที่ ๓๓ (พ.ศ. ๒๕๕๒) เรื่อง กำหนดมาตรฐานค่าก๊าซไนโตรเจนไดออกไซด์ในบรรยากาศโดยทั่วไป ลงวันที่ ๑๗ มิถุนายน พ.ศ. ๒๕๕๒

๑.๗ ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ เรื่อง กำหนดมาตรฐานฝุ่นละอองขนาดไม่เกิน ๒.๕ ไมครอน ในบรรยากาศโดยทั่วไป ลงวันที่ ๒๓ มิถุนายน พ.ศ. ๒๕๖๕

ข้อ ๒ กำหนดค่ามาตรฐานคุณภาพอากาศในบรรยากาศโดยทั่วไปไว้ ดังนี้

๒.๑ ก๊าซซัลเฟอร์ไดออกไซด์

(๑) ค่าเฉลี่ยของก๊าซซัลเฟอร์ไดออกไซด์ ในเวลา ๑ ชั่วโมง จะต้องไม่เกิน ๑๐๐ ส่วนในพันล้านส่วน

(๒) ค่าเฉลี่ยของก๊าซซัลเฟอร์ไดออกไซด์ ในเวลา ๒๔ ชั่วโมง จะต้องไม่เกิน ๕๐ ส่วนในพันล้านส่วน

๒.๒ ก๊าซไนโตรเจนไดออกไซด์

(๑) ค่าเฉลี่ยของก๊าซไนโตรเจนไดออกไซด์ ในเวลา ๑ ชั่วโมง จะต้องไม่เกิน ๑๒๐ ส่วนในพันล้านส่วน

(๒) ค่าเฉลี่ยของก๊าซไนโตรเจนไดออกไซด์ในเวลา ๑ ปี จะต้องไม่เกิน ๓๐ ส่วนในพันล้านส่วน

๒.๓ ก๊าซคาร์บอนมอนอกไซด์

(๑) ค่าเฉลี่ยของก๊าซคาร์บอนมอนอกไซด์ ในเวลา ๑ ชั่วโมง จะต้องไม่เกิน ๓๐ ส่วนในล้านส่วน

(๒) ค่าเฉลี่ยของก๊าซคาร์บอนมอนอกไซด์ ในเวลา ๘ ชั่วโมง จะต้องไม่เกิน ๙ ส่วนในล้านส่วน

๒.๔ ก๊าซโอโซน

(๑) ค่าเฉลี่ยของก๊าซโอโซน ในเวลา ๑ ชั่วโมง จะต้องไม่เกิน ๑๐๐ ส่วนในพันล้านส่วน

(๒) ค่าเฉลี่ยของก๊าซโอโซน ในเวลา ๘ ชั่วโมง จะต้องไม่เกิน ๗๐ ส่วนในพันล้านส่วน

๒.๕ ฝุ่นรวมหรือฝุ่นละอองขนาดไม่เกิน ๑๐๐ ไมครอน

(๑) ค่าเฉลี่ยของฝุ่นรวมหรือฝุ่นละอองขนาดไม่เกิน ๑๐๐ ไมครอน ในเวลา ๒๔ ชั่วโมง จะต้องไม่เกิน ๒๐๐ ไมโครกรัมต่อลูกบาศก์เมตร

(๒) ค่าเฉลี่ยของฝุ่นรวมหรือฝุ่นละอองขนาดไม่เกิน ๑๐๐ ไมครอน ในเวลา ๑ ปี จะต้องไม่เกิน ๘๐ ไมโครกรัมต่อลูกบาศก์เมตร

๒.๖ ฝุ่นละอองขนาดไม่เกิน ๑๐ ไมครอน

(๑) ค่าเฉลี่ยของฝุ่นละอองขนาดไม่เกิน ๑๐ ไมครอน ในเวลา ๒๔ ชั่วโมง จะต้องไม่เกิน ๑๐๐ ไมโครกรัมต่อลูกบาศก์เมตร

(๒) ค่าเฉลี่ยของฝุ่นละอองขนาดไม่เกิน ๑๐ ไมครอน ในเวลา ๑ ปี จะต้องไม่เกิน ๕๐ ไมโครกรัมต่อลูกบาศก์เมตร

๒.๗ ฝุ่นละอองขนาดไม่เกิน ๒.๕ ไมครอน

(๑) ค่าเฉลี่ยของฝุ่นละอองขนาดไม่เกิน ๒.๕ ไมครอน ในเวลา ๒๔ ชั่วโมง จะต้องไม่เกิน ๓๗.๕ ไมโครกรัมต่อลูกบาศก์เมตร

(๒) ค่าเฉลี่ยของฝุ่นละอองขนาดไม่เกิน ๒.๕ ไมครอน ในเวลา ๑ ปี จะต้องไม่เกิน ๑๕ ไมโครกรัมต่อลูกบาศก์เมตร

๒.๘ สารตะกั่ว ค่าเฉลี่ยของสารตะกั่ว ในเวลา ๑ เดือน จะต้องไม่เกิน ๑ ไมโครกรัมต่อลูกบาศก์เมตร

ข้อ ๓ วิธีการตรวจวัดค่าเฉลี่ยของสารมลพิษทางอากาศ ดังนี้

๓.๑ ค่าเฉลี่ยของก๊าซซัลเฟอร์ไดออกไซด์ในเวลา ๑ ชั่วโมง หรือค่าเฉลี่ยในเวลา ๒๔ ชั่วโมง ให้ใช้วิธีพาราโรซานิลีน (Pararosaniline) หรือวิธีอุลตร้าไวโอเลต ฟลูออเรสเซน (Ultraviolet Fluorescence)

๓.๒ ค่าเฉลี่ยของก๊าซไนโตรเจนไดออกไซด์ในเวลา ๑ ชั่วโมง หรือค่าเฉลี่ยในเวลา ๑ ปี ให้ใช้วิธีเคมีลูมิเนสเซน (Chemiluminescence) หรือวิธีคาวิตี แอทเทนนูเอเต็ด เฟสชิพ สเปกโทรสโกปี (Cavity Attenuated Phase Shift Spectroscopy : CAPS)

๓.๓ ค่าเฉลี่ยของก๊าซคาร์บอนมอนอกไซด์ในเวลา ๑ ชั่วโมง หรือค่าเฉลี่ยในเวลา ๘ ชั่วโมง ให้ใช้วิธีนันดีสเปอร์ซีฟ อินฟราเรด ดีเทคชัน (Non-dispersive Infrared Detection) หรือวิธีนันดีสเปอร์ซีฟ อินฟราเรด ดีเทคชัน ก๊าซฟิลเตอร์คอริเรชัน (Non-dispersive Infrared Detection Gas Filter Correlation)

๓.๔ ค่าเฉลี่ยของก๊าซโอโซนในเวลา ๑ ชั่วโมง หรือค่าเฉลี่ยของก๊าซโอโซนในเวลา ๘ ชั่วโมง ให้ใช้วิธีเคมีลูมิเนสเซน (Chemiluminescence) หรือวิธีอุลตร้าไวโอเลต แอ็บซอปชัน โฟโตเมตตริก (Ultraviolet Absorption Photometry)

๓.๕ ค่าเฉลี่ยของฝุ่นรวมหรือฝุ่นละอองขนาดไม่เกิน ๑๐๐ ไมครอน ในเวลา ๒๔ ชั่วโมง หรือค่าเฉลี่ย ในเวลา ๑ ปี ให้ใช้วิธีตรวจวัดอ้างอิง คือวิธีกราวิเมตริก (Gravimetric)

๓.๖ ค่าเฉลี่ยของฝุ่นละอองขนาดไม่เกิน ๑๐ ไมครอน ในเวลา ๒๔ ชั่วโมง หรือค่าเฉลี่ยในเวลา ๑ ปี ให้ใช้วิธีตรวจวัดอ้างอิง คือวิธีกราวิเมตริก (Gravimetric) หรือวิธีตรวจวัดเทียบเท่า ได้แก่ วิธีเบต้าเรดิเอชัน แอทเทนนูเอชัน (Beta Radiation Attenuation) วิธีเทปเปอร์ อิลิเมนต์ ออสซิเลติง ไมโครบาลานซ์ (Tapered Element Oscillating Microbalance : TEOM)

วิธีการกระเจิงของแสง (Light Scattering) และวิธีเก็บตัวอย่างด้วยเครื่องเก็บตัวอย่างอากาศแบบไดโคโตมัส (Dichotomous Air Sampler)

๓.๗ ค่าเฉลี่ยของฝุ่นละอองขนาดไม่เกิน ๒.๕ ไมครอน ในเวลา ๒๔ ชั่วโมง หรือค่าเฉลี่ยในเวลา ๑ ปี ให้ใช้วิธีตรวจวัดอ้างอิง คือวิธีกราวิเมตริก (Gravimetric) หรือวิธีตรวจวัดเทียบเท่า ได้แก่ วิธีเบต้า เรดิเอชัน แอทเทนนูเอชัน (Beta Radiation Attenuation) วิธีเทปเปอร์ อิลิเมนต์ ออสซิเลติง ไมโครบาลานซ์ (Tapered Element Oscillating Microbalance : TEOM) วิธีการกระเจิงของแสง (Light Scattering) และวิธีเก็บตัวอย่างด้วยเครื่องเก็บตัวอย่างอากาศแบบไดโคโตมัส (Dichotomous Air Sampler)

๓.๘ ค่าเฉลี่ยของสารตะกั่ว ในเวลา ๑ เดือน ให้ใช้วิธีอะตอมมิก แอบซอพชัน สเปคโตรมิเตอร์ (Atomic Absorption Spectrometer)

ข้อ ๔ วิธีการตรวจวัดค่าเฉลี่ยของสารมลพิษทางอากาศตามข้อ ๓ ให้ใช้วิธีตรวจวัดอ้างอิงหรือวิธีตรวจวัดเทียบเท่า ตามที่องค์การพิทักษ์สิ่งแวดล้อมแห่งสหรัฐอเมริกา (United States Environmental Protection Agency : US EPA) หรือมาตรฐานของสหภาพยุโรป (European Union : EU) กำหนด หรือวิธีอื่นตามที่อธิบดีกรมควบคุมมลพิษประกาศในราชกิจจานุเบกษา

ข้อ ๕ การตรวจวัดค่าเฉลี่ยของสารมลพิษทางอากาศให้ดำเนินการ ดังนี้

๕.๑ การตรวจวัดค่าเฉลี่ยของสารมลพิษทางอากาศในข้อ ๓.๑ ถึงข้อ ๓.๔ ให้ทำในบรรยากาศโดยทั่วไป และต้องสูงจากพื้นดินอย่างน้อย ๓ เมตร แต่ไม่เกิน ๖ เมตร ตามวัตถุประสงค์ของการตรวจวัด การคำนวณค่าความเข้มข้นของสารมลพิษทางอากาศให้เทียบที่อุณหภูมิ ๒๕ องศาเซลเซียส และความดัน ๑ บรรยากาศ

๕.๒ การตรวจวัดค่าเฉลี่ยของสารมลพิษทางอากาศในข้อ ๓.๕ ข้อ ๓.๖ และข้อ ๓.๘ ให้ทำในบรรยากาศโดยทั่วไป และต้องสูงจากพื้นดินอย่างน้อย ๑.๕๐ เมตร แต่ไม่เกิน ๖ เมตร ตามวัตถุประสงค์ของการตรวจวัด การคำนวณค่าความเข้มข้นของสารมลพิษทางอากาศให้เทียบที่อุณหภูมิ ๒๕ องศาเซลเซียส และความดัน ๑ บรรยากาศ

๕.๓ การตรวจวัดค่าเฉลี่ยของสารมลพิษทางอากาศในข้อ ๓.๗ ให้ทำในบรรยากาศโดยทั่วไป และต้องสูงจากพื้นดินอย่างน้อย ๑.๕๐ เมตร แต่ไม่เกิน ๑๕ เมตร ตามวัตถุประสงค์ของการตรวจวัด การคำนวณค่าความเข้มข้นของสารมลพิษทางอากาศให้เทียบที่อุณหภูมิและความดันบรรยากาศสภาวะจริง

ข้อ ๖ การคำนวณค่าความเข้มข้นของสารมลพิษทางอากาศตามข้อ ๕ ต้องมีความครบถ้วนสมบูรณ์ของข้อมูล ไม่น้อยกว่าร้อยละ ๗๕

ข้อ ๗ การกำหนดดัชนีคุณภาพอากาศของประเทศไทยสำหรับสารมลพิษทางอากาศตามประกาศนี้ ให้เป็นไปตามหลักเกณฑ์ วิธีการ และเงื่อนไข ที่อธิบดีกรมควบคุมมลพิษประกาศในราชกิจจานุเบกษา

ข้อ ๘ ประกาศนี้ให้ใช้บังคับนับแต่วันถัดจากวันประกาศในราชกิจจานุเบกษา

ประกาศ ณ วันที่ ๖ มกราคม พ.ศ. ๒๕๖๙
สุชาติ ชมกลิ่น
รองนายกรัฐมนตรี
ประธานกรรมการสิ่งแวดล้อมแห่งชาติ



ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ
ฉบับที่ ๑๕ (พ.ศ. ๒๕๔๐)
เรื่อง กำหนดมาตรฐานระดับเสียงโดยทั่วไป

อาศัยอำนาจตามความในมาตรา ๓๒ (๕) แห่งพระราชบัญญัติส่งเสริมและรักษาคุณภาพสิ่งแวดล้อมแห่งชาติ พ.ศ. ๒๕๓๕ คณะกรรมการสิ่งแวดล้อมแห่งชาติกำหนดมาตรฐานระดับเสียงโดยทั่วไปไว้ดังต่อไปนี้

ข้อ ๑ ในประกาศนี้

"ระดับเสียงโดยทั่วไป" หมายความว่า ระดับเสียงที่เกิดขึ้นในสิ่งแวดล้อม

"ค่าระดับเสียงสูงสุด" หมายความว่า ค่าระดับเสียงสูงสุดที่เกิดขึ้นในขณะใดขณะหนึ่งระหว่างการตรวจวัดระดับเสียง โดยมีหน่วยเป็นเดซิเบลเอ หรือ dB (A)

"ค่าระดับเสียงเฉลี่ย ๒๔ ชั่วโมง" หมายความว่า ค่าระดับเสียงคงที่ที่มีพลังงานเทียบเท่าระดับเสียงที่เกิดขึ้นจริง ซึ่งมีระดับเสียงเปลี่ยนแปลงตามเวลาในช่วง ๒๔ ชั่วโมง (๒๔ hours A-weighted Equivalent Continuous Sound Level) ซึ่งเรียกโดยย่อว่า Leq ๒๔ hr โดยมีหน่วยเป็นเดซิเบลเอ หรือ dB (A)

"มาตรระดับเสียง" หมายความว่า เครื่องวัดระดับเสียงตามมาตรฐาน IEC ๖๕๑ หรือ IEC ๘๐๔ ของคณะกรรมาธิการระหว่างประเทศว่าด้วยเทคนิคไฟฟ้า (International Electrotechnical Commission, IEC)

ข้อ ๒ ให้กำหนดมาตรฐานระดับเสียงโดยทั่วไป ไว้ดังต่อไปนี้

(๑) ค่าระดับเสียงสูงสุด ไม่เกิน ๑๑๕ เดซิเบลเอ

(๒) ค่าระดับเสียงเฉลี่ย ๒๔ ชั่วโมง ไม่เกิน ๗๐ เดซิเบลเอ

ข้อ ๓ การตรวจวัดระดับเสียงโดยทั่วไป ให้ดำเนินการดังต่อไปนี้

(๑) การตรวจวัดค่าระดับเสียงสูงสุด ให้ใช้มาตรระดับเสียงตรวจวัดระดับเสียงในบริเวณที่มีคนอยู่หรืออาศัยอยู่

(๒) การตรวจวัดค่าระดับเสียงเฉลี่ย ๒๔ ชั่วโมง ให้ใช้มาตรระดับเสียงตรวจวัดระดับเสียงอย่างต่อเนื่องตลอดเวลา ๒๔ ชั่วโมงใดๆ

(๓) การตั้งไมโครโฟนของมาตรระดับเสียงที่บริเวณภายนอกอาคารให้ตั้งสูงจากพื้นไม่น้อยกว่า ๑.๒๐ เมตร โดยในรัศมี ๓.๕๐ เมตร ตามแนวราบรอบไมโครโฟนต้องไม่มีกำแพงหรือสิ่งอื่นใดที่มีคุณสมบัติในการสะท้อนเสียงกีดขวางอยู่

(๔) การตั้งไมโครโฟนของมาตรระดับเสียงที่บริเวณภายในอาคารให้ตั้งสูงจากพื้นไม่น้อยกว่า ๑.๒๐ เมตร โดยในรัศมี ๑.๐๐ เมตร ตามแนวราบรอบไมโครโฟนต้องไม่มีกำแพงสิ่งอื่นใดที่มีคุณสมบัติในการสะท้อนเสียงกีดขวางอยู่และต้องห่างจากช่องหน้าต่างหรือช่องทางที่เปิดออกนอกอาคารอย่างน้อย ๑.๕๐ เมตร

ข้อ ๔ การคำนวณค่าระดับเสียงจะต้องเป็นไปตามวิธีการที่องค์การระหว่างประเทศว่าด้วยมาตรฐาน (International Organization for Standardization, ISO) กำหนด ซึ่งกรมควบคุมมลพิษจะประกาศในราชกิจจานุเบกษา

ประกาศ ณ วันที่ ๑๒ มีนาคม พ.ศ. ๒๕๔๐
พลเอก ชวลิต ยงใจยุทธ
นายกรัฐมนตรี
ประธานคณะกรรมการสิ่งแวดล้อมแห่งชาติ

(ประกาศในราชกิจจานุเบกษา เล่ม ๑๑๔ ตอนที่ ๒๗ ง วันที่ ๓ เมษายน ๒๕๔๐)

ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ

ฉบับที่ ๒๙ (พ.ศ. ๒๕๕๐)

เรื่อง ค่าระดับเสียงรบกวน

โดยที่เป็นการสมควร ปรับปรุงค่ามาตรฐานระดับเสียงรบกวน ให้เหมาะสมกับกฎเกณฑ์และหลักฐานทางวิทยาศาสตร์ โดยคำนึงถึงความเป็นไปได้ในเชิงเศรษฐกิจสังคมและเทคโนโลยีที่เกี่ยวข้อง อาศัยอำนาจตามความในมาตรา ๓๔ แห่งพระราชบัญญัติส่งเสริมและรักษาคุณภาพสิ่งแวดล้อมแห่งชาติ พ.ศ. ๒๕๓๕ และคำสั่งสำนักนายกรัฐมนตรี ที่ ๗๑/๒๕๕๐ คณะกรรมการสิ่งแวดล้อมแห่งชาติจึงออกประกาศกำหนดค่าระดับเสียงรบกวน ไว้ดังต่อไปนี้

ข้อ ๑ ให้ยกเลิกประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ ฉบับที่ ๑๗ (พ.ศ. ๒๕๔๓) ลงวันที่ ๖ มิถุนายน ๒๕๔๓ เรื่อง ค่าระดับเสียงรบกวน

ข้อ ๒ ให้กำหนดระดับเสียงรบกวนเท่ากับ ๑๐ เดซิเบลเอ

หากระดับการรบกวนที่คำนวณได้มีค่ามากกว่าระดับเสียงรบกวนตามวรรคแรก ให้ถือว่าเป็นเสียงรบกวน

ข้อ ๓ วิธีการตรวจวัดระดับเสียงพื้นฐาน ระดับเสียงขณะไม่มีการรบกวน การตรวจวัดและคำนวณระดับเสียงขณะมีการรบกวน การคำนวณค่าระดับการรบกวน และแบบบันทึกการตรวจวัดเสียงรบกวนให้เป็นไปตามที่ คณะกรรมการควบคุมมลพิษประกาศในราชกิจจานุเบกษา

ประกาศ ณ วันที่ ๒๙ มิถุนายน พ.ศ. ๒๕๕๐
โฆสิต ปั้นเปี่ยมรัษฎ์
รองนายกรัฐมนตรี
ประธานกรรมการสิ่งแวดล้อมแห่งชาติ

ประกาศกระทรวงอุตสาหกรรม

เรื่อง กำหนดค่าระดับเสียงการรบกวนและระดับเสียงที่เกิดจากการประกอบกิจการโรงงาน

พ.ศ. ๒๕๔๘

อาศัยอำนาจตามความในข้อ ๑๗ แห่งกฎกระทรวง ฉบับที่ ๒ (พ.ศ. ๒๕๓๕) ออกตามความในพระราชบัญญัติโรงงาน พ.ศ. ๒๕๓๕ อันเป็นพระราชบัญญัติที่มีบทบัญญัติบางประการเกี่ยวกับการจำกัดสิทธิและเสรีภาพของบุคคล ซึ่งมาตรา ๒๙ ประกอบกับมาตรา ๓๕ มาตรา ๔๘ และมาตรา ๕๐ ของรัฐธรรมนูญแห่งราชอาณาจักรไทย บัญญัติให้กระทำได้โดยอาศัยอำนาจตามบทบัญญัติแห่งกฎหมาย รัฐมนตรีว่าการกระทรวงอุตสาหกรรมจึงได้ออกประกาศไว้ ดังต่อไปนี้

ข้อ ๑ ในประกาศนี้

“เสียงรบกวน” หมายความว่า ระดับเสียงตรวจวัดนอกบริเวณโรงงาน ที่เกิดจากการประกอบกิจการโรงงาน ขณะมีการรบกวน ซึ่งมีระดับเสียงสูงกว่าระดับเสียงพื้นฐาน และมีระดับการรบกวนเกินกว่าค่าที่กำหนดไว้ในประกาศนี้

“ระดับเสียงพื้นฐาน” หมายความว่า ระดับเสียงที่ตรวจวัดในสิ่งแวดล้อมเดิม ขณะยังไม่มีเสียงรบกวนจากการประกอบกิจการโรงงานเป็นระดับเสียงเปอร์เซ็นไทล์ที่ ๙๐ (Percentile Level 90 , L_{90})

“ระดับเสียงเปอร์เซ็นไทล์ที่ ๙๐ (L_{90})” หมายความว่า ระดับเสียงที่ร้อยละ ๙๐ ของเวลาที่ตรวจวัดจะมีระดับเสียงเกินระดับนี้

“ระดับเสียงขณะมีการรบกวน” หมายความว่า ระดับเสียงที่ตรวจวัดหรือคำนวณจากการประกอบกิจการโรงงานขณะเกิดเสียงรบกวน

“ระดับการรบกวน” หมายความว่า ระดับความแตกต่างของระดับเสียงขณะมีการรบกวนกับระดับเสียงพื้นฐาน

“ระดับเสียงเฉลี่ย ๒๔ ชั่วโมง” หมายความว่า ระดับเสียงคงที่นอกบริเวณโรงงานที่มีพลังงานเทียบเท่าระดับเสียงที่เกิดขึ้นจริง ซึ่งมีระดับเสียงเปลี่ยนแปลงตามเวลาในช่วง ๒๔ ชั่วโมง (24 hours A-weighted Equivalent Continuous Sound Level) ซึ่งเรียกโดยย่อว่า Leq 24 hr โดยมีหน่วยเป็นเดซิเบลเอ หรือ dB(A)

"ระดับเสียงสูงสุด" หมายความว่า ระดับเสียงสูงสุดนอกบริเวณโรงงาน ที่เกิดขึ้นในขณะใดขณะหนึ่งระหว่างการตรวจวัดระดับเสียง โดยมีหน่วยเป็นเดซิเบลเอ หรือ dB(A)

"มาตรระดับเสียง" หมายความว่า เครื่องวัดระดับเสียงตามมาตรฐาน IEC 60804 หรือ IEC 61672 ของคณะกรรมาธิการระหว่างประเทศว่าด้วยเทคนิคไฟฟ้า (International Electrotechnical Commission , IEC)

ข้อ ๒ ค่าระดับการรบกวน ที่เกิดจากการประกอบกิจการโรงงาน ไม่เกิน ๑๐ เดซิเบลเอ

ข้อ ๓ ค่าระดับเสียงเฉลี่ย ๒๔ ชั่วโมง ที่เกิดจากการประกอบกิจการโรงงาน ไม่เกิน ๗๐ เดซิเบลเอ

ข้อ ๔ ค่าระดับเสียงสูงสุด ที่เกิดจากการประกอบกิจการโรงงาน ไม่เกิน ๑๑๕ เดซิเบลเอ

ข้อ ๕ วิธีการตรวจวัดระดับเสียงการรบกวน ระดับเสียงเฉลี่ย ๒๔ ชั่วโมง และระดับเสียงสูงสุดที่เกิดจากการประกอบกิจการโรงงาน ให้เป็นไปตามที่กรมโรงงานอุตสาหกรรมกำหนด

ทั้งนี้ ให้ใช้บังคับตั้งแต่วันถัดจากวันประกาศในราชกิจจานุเบกษาเป็นต้นไป

ประกาศ ณ วันที่ ๒๗ ธันวาคม พ.ศ. ๒๕๔๘

สุริยะ จึงรุ่งเรืองกิจ

รัฐมนตรีว่าการกระทรวงอุตสาหกรรม



ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ
ฉบับที่ ๘ (พ.ศ. ๒๕๓๗)
ออกตามความในพระราชบัญญัติส่งเสริมและรักษาคุณภาพสิ่งแวดล้อมแห่งชาติ
พ.ศ. ๒๕๓๕
เรื่อง กำหนดมาตรฐานคุณภาพน้ำในแหล่งน้ำผิวดิน

อาศัยอำนาจตามความในมาตรา ๓๒ (๑) แห่งพระราชบัญญัติส่งเสริมและรักษาคุณภาพสิ่งแวดล้อมแห่งชาติ พ.ศ. ๒๕๓๕ คณะกรรมการสิ่งแวดล้อมแห่งชาติประกาศกำหนดมาตรฐานคุณภาพน้ำในแหล่งน้ำผิวดิน ไว้ดังต่อไปนี้

หมวด ๑
บททั่วไป

ข้อ ๑ ในประกาศนี้

"แหล่งน้ำผิวดิน" หมายถึง แม่น้ำ ลำคลอง หนอง บึง ทะเลสาบ อ่างเก็บน้ำ และแหล่งน้ำสาธารณะอื่นๆ ที่อยู่ภายในผืนแผ่นดิน ซึ่งหมายความรวมถึงแหล่งน้ำสาธารณะที่อยู่ภายในผืนแผ่นดินบนเกาะด้วย แต่ไม่รวมถึงน้ำบาดาล และในกรณีที่แหล่งน้ำนั้นอยู่ติดกับทะเลให้หมายความถึงแหล่งน้ำที่อยู่ภายในปากแม่น้ำหรือปากทะเลสาบ

ปากแม่น้ำและปากทะเลสาบให้ถือแนวเขตตามที่กรมเจ้าท่ากำหนด

หมวด ๒

ประเภทและมาตรฐานคุณภาพน้ำในแหล่งน้ำผิวดิน

ข้อ ๒ ให้แบ่งแหล่งน้ำผิวดินออกเป็น ๕ ประเภทคือ แหล่งน้ำประเภทที่ ๑ แหล่งน้ำประเภทที่ ๒ แหล่งน้ำประเภทที่ ๓ แหล่งน้ำประเภทที่ ๔ และแหล่งน้ำประเภทที่ ๕

(๑) แหล่งน้ำประเภทที่ ๑ ได้แก่ แหล่งน้ำที่คุณภาพน้ำมีสภาพตามธรรมชาติโดยปราศจากน้ำทิ้งจากกิจกรรมทุกประเภทและสามารถเป็นประโยชน์เพื่อ

(ก) การอุปโภคและบริโภคโดยต้องผ่านการฆ่าเชื้อโรคตามปกติก่อน

(ข) การขยายพันธุ์ตามธรรมชาติของสิ่งมีชีวิตระดับพื้นฐาน

(ค) การอนุรักษ์ระบบนิเวศน์ของแหล่งน้ำ

(๒) แหล่งน้ำประเภทที่ ๒ ได้แก่ แหล่งน้ำที่ได้รับน้ำทิ้งจากกิจกรรมบางประเภทและสามารถเป็นประโยชน์เพื่อ

(ก) การอุปโภคและบริโภคโดยต้องผ่านการฆ่าเชื้อโรคตามปกติและผ่านกระบวนการปรับปรุงคุณภาพน้ำทั่วไปก่อน

(ข) การอนุรักษ์สัตว์น้ำ

(ค) การประมง

(ง) การว่ายน้ำและกีฬาทางน้ำ

(๓) แหล่งน้ำประเภทที่ ๓ ได้แก่ แหล่งน้ำที่ได้รับน้ำทิ้งจากกิจกรรมบางประเภทและสามารถเป็นประโยชน์เพื่อ

(ก) การอุปโภคและบริโภคโดยต้องผ่านการฆ่าเชื้อโรคตามปกติและผ่านกระบวนการปรับปรุงคุณภาพน้ำทั่วไปก่อน

(ข) การเกษตร

(๔) แหล่งน้ำประเภทที่ ๔ ได้แก่ แหล่งน้ำที่ได้รับน้ำทิ้งจากกิจกรรมบางประเภทและสามารถเป็นประโยชน์เพื่อ

(ก) การอุปโภคและบริโภคโดยต้องผ่านการฆ่าเชื้อโรคตามปกติและผ่านกระบวนการปรับปรุงคุณภาพน้ำเป็นพิเศษก่อน

(ข) การอุตสาหกรรม

(๕) แหล่งน้ำประเภทที่ ๕ ได้แก่ แหล่งน้ำที่ได้รับน้ำทิ้งจากกิจกรรมบางประเภท และสามารถเป็นประโยชน์เพื่อการคมนาคม

ข้อ ๓ คุณภาพน้ำในแหล่งน้ำประเภทที่ ๑ ต้องมีสภาพตามธรรมชาติ และสามารถใช้ประโยชน์ได้ตามข้อ ๒ (๑)

ข้อ ๔ คุณภาพน้ำในแหล่งน้ำประเภทที่ ๒ ต้องมีมาตรฐานดังต่อไปนี้

(๑) ไม่มีวัตถุหรือสิ่งของที่เกิดจากการกระทำของมนุษย์ซึ่งจะทำให้ สี กลิ่น และรสของน้ำเปลี่ยนไปตามธรรมชาติ

(๒) อุณหภูมิ (Temperature) ไม่สูงกว่าอุณหภูมิตามธรรมชาติเกิน ๓ องศาเซลเซียส

(๓) ความเป็นกรดและด่าง (pH) มีค่าระหว่าง ๕.๐-๙.๐

(๔) ออกซิเจนละลาย (DO) มีค่าไม่น้อยกว่า ๖.๐ มิลลิกรัมต่อลิตร

(๕) บีโอดี (BOD) มีค่าไม่เกินกว่า ๑.๕ มิลลิกรัมต่อลิตร

(๖) แบคทีเรียกลุ่มโคลิฟอร์มทั้งหมด (Total Coliform Bacteria) มีค่าไม่เกินกว่า ๕,๐๐๐ เอ็ม.พี.เอ็น. ต่อ ๑๐๐ มิลลิลิตร

(๗) แบคทีเรียกลุ่มฟีคอลโคลิฟอร์ม (Fecal Coliform Bacteria) มีค่าไม่เกินกว่า ๑,๐๐๐ เอ็ม.พี.เอ็น. ต่อ ๑๐๐ มิลลิลิตร

(๘) ไนเตรต (NO_3) ในหน่วยไนโตรเจน มีค่าไม่เกินกว่า ๕.๐ มิลลิกรัมต่อลิตร

(๙) แอมโมเนีย (NH_3) ในหน่วยไนโตรเจน มีค่าไม่เกินกว่า ๐.๕ มิลลิกรัมต่อลิตร

(๑๐) ฟีนอล (Phenols) มีค่าไม่เกินกว่า ๐.๐๐๕ มิลลิกรัมต่อลิตร

(๑๑) ทองแดง (Cu) มีค่าไม่เกินกว่า ๐.๑ มิลลิกรัมต่อลิตร

(๑๒) นิคเกิล (Ni) มีค่าไม่เกินกว่า ๐.๑ มิลลิกรัมต่อลิตร

(๑๓) แมงกานีส (Mn) มีค่าไม่เกินกว่า ๑.๐ มิลลิกรัมต่อลิตร

(๑๔) สังกะสี (Zn) มีค่าไม่เกินกว่า ๑.๐ มิลลิกรัมต่อลิตร

(๑๕) แคดเมียม (Cd) ในน้ำที่มีความกระด้างในรูปของ $CaCO_3$ ไม่เกินกว่า ๑๐๐ มิลลิกรัมต่อลิตร มีค่าไม่เกินกว่า ๐.๐๐๕ มิลลิกรัมต่อลิตร และในน้ำที่มีความกระด้างในรูปของ $CaCO_3$ เกินกว่า ๑๐๐ มิลลิกรัมต่อลิตร มีค่าไม่เกินกว่า ๐.๐๕ มิลลิกรัมต่อลิตร

(๑๖) โครเมียมชนิดเฮ็กซาวาเล้นท์ (Cr Hexavalent) มีค่าไม่เกินกว่า ๐.๐๕ มิลลิกรัมต่อลิตร

(๑๗) ตะกั่ว (Pb) มีค่าไม่เกิน ๐.๐๕ มิลลิกรัมต่อลิตร

(๑๘) ปรอททั้งหมด (Total Hg) มีค่าไม่เกินกว่า ๐.๐๐๒ มิลลิกรัมต่อลิตร

(๑๙) สารหนู (As) มีค่าไม่เกินกว่า ๐.๐๑ มิลลิกรัมต่อลิตร

(๒๐) ไซยาไนด์ (Cyanide) มีค่าไม่เกินกว่า ๐.๐๐๕ มิลลิกรัมต่อลิตร

(๒๑) กัมมันตภาพรังสี (Radioactivity) มีค่ารังสีแอลฟา (Alpha) ไม่เกินกว่า ๐.๑ เบคเคอเรลต่อลิตร และรังสีเบตา (Beta) ไม่เกินกว่า ๑.๐ เบคเคอเรลต่อลิตร

(๒๒) สารฆ่าศัตรูพืชและสัตว์ชนิดที่มีคลอรีนทั้งหมด (Total Organochlorine Pesticides) มีค่าไม่เกินกว่า ๐.๐๕ มิลลิกรัมต่อลิตร

(๒๓) ดีดีที (DDT) มีค่าไม่เกินกว่า ๑.๐ ไมโครกรัมต่อลิตร

(๒๔) บีเอชซีชนิดแอลฟา (Alpha-BHC) มีค่าไม่เกินกว่า ๐.๐๒ ไมโครกรัมต่อลิตร

(๒๕) ดิลดริน (Dieldrin) มีค่าไม่เกินกว่า ๐.๑ ไมโครกรัมต่อลิตร

(๒๖) อัลดริน (Aldrin) มีค่าไม่เกินกว่า ๐.๑ ไมโครกรัมต่อลิตร

(๒๗) เฮปตาคลอร์ (Heptachlor) และเฮปตาคลอร์อีปอกไซด์ (Heptachlorepoxide) มีค่าไม่เกินกว่า ๐.๒ ไมโครกรัมต่อลิตร

(๒๘) เอนดริน (Endrin) ไม่สามารถตรวจพบได้ตามวิธีการตรวจสอบที่กำหนด

ข้อ ๕ คุณภาพน้ำในแหล่งน้ำประเภทที่ ๓ ต้องมีมาตรฐานตาม ข้อ ๔ เว้นแต่

(๑) ออกซิเจนละลาย มีค่าไม่น้อยกว่า ๔.๐ มิลลิกรัมต่อลิตร

(๒) บีโอดี มีค่าไม่เกินกว่า ๒.๐ มิลลิกรัมต่อลิตร

(๓) แบคทีเรียกลุ่มโคลิฟอร์มทั้งหมด มีค่าไม่เกินกว่า ๒๐,๐๐๐ เอ็ม.พี.เอ็น. ต่อ ๑๐๐ มิลลิลิตร

(๔) แบคทีเรียกลุ่มฟีคอลโคลิฟอร์ม มีค่าไม่เกินกว่า ๔,๐๐๐ เอ็ม.พี.เอ็น. ต่อ ๑๐๐ มิลลิลิตร

ข้อ ๖ คุณภาพน้ำในแหล่งน้ำประเภทที่ ๔ ต้องมีมาตรฐานตามข้อ ๔ (๑) ถึง (๕) และ (๘) ถึง (๒๘) เว้นแต่

(๑) ออกซิเจนละลาย มีค่าไม่น้อยกว่า ๒.๐ มิลลิกรัมต่อลิตร

(๒) บีโอดี มีค่าไม่เกินกว่า ๔.๐ มิลลิกรัมต่อลิตร

ข้อ ๗ คุณภาพน้ำในแหล่งน้ำประเภทที่ ๕ ต้องมีมาตรฐานต่ำกว่าคุณภาพน้ำ ในแหล่งน้ำประเภทที่ ๔

ข้อ ๘ การกำหนดให้แหล่งน้ำผิวดินแหล่งใดแหล่งหนึ่งเป็นประเภทใดตามข้อ ๒ ให้เป็นไปตามที่กรมควบคุมมลพิษประกาศในราชกิจจานุเบกษา

หมวด ๓
วิธีการเก็บตัวอย่างและตรวจสอบคุณภาพน้ำในแหล่งน้ำผิวดิน

ข้อ ๙ การเก็บตัวอย่างน้ำเพื่อตรวจสอบคุณภาพตามข้อ ๓ ถึง ข้อ ๗ ให้ใช้วิธีการดังต่อไปนี้

(๑) แหล่งน้ำไหล ซึ่งได้แก่ แม่น้ำ ลำคลอง เป็นต้น ให้เก็บที่จุดกึ่งกลางความกว้างของแหล่งน้ำที่ระดับกึ่งกลางความลึก ณ จุดตรวจสอบ เว้นแต่แบคทีเรียกลุ่มโคลิฟอร์มทั้งหมดและแบคทีเรียกลุ่มฟีคอลโคลิฟอร์ม ให้เก็บที่ระดับความลึก ๓๐ เซนติเมตร ณ จุดตรวจสอบ

(๒) แหล่งน้ำนิ่ง ซึ่งได้แก่ ทะเลสาบ หนอง บึง อ่างเก็บน้ำ เป็นต้น ให้เก็บที่ระดับความลึก ๑ เมตร ณ จุดตรวจสอบสำหรับแหล่งน้ำที่มีความลึกเกินกว่า ๒ เมตร และให้เก็บที่จุดกึ่งกลางความลึก ณ จุดตรวจสอบสำหรับแหล่งน้ำที่มีความลึกไม่เกิน ๒ เมตร เว้นแต่แบคทีเรียกลุ่มโคลิฟอร์มทั้งหมดและแบคทีเรียกลุ่มฟีคอลโคลิฟอร์ม ให้เก็บที่ระดับความลึก ๓๐ เซนติเมตร ณ จุดตรวจสอบ

จุดตรวจสอบตาม (๑) และ (๒) ของแหล่งน้ำที่กำหนดตามข้อ ๘ ให้เป็นไปตามที่กรมควบคุมมลพิษกำหนด

ข้อ ๑๐ การตรวจสอบคุณภาพน้ำตามข้อ ๓ ถึงข้อ ๗ ให้ใช้วิธีการดังต่อไปนี้

(๑) การตรวจสอบอุณหภูมิ ให้ใช้เครื่องวัดอุณหภูมิ (Thermometer) วัดขณะทำการเก็บตัวอย่างน้ำ

(๒) การตรวจสอบค่าความเป็นกรดและด่าง ให้ใช้เครื่องวัดความเป็นกรดและด่างของน้ำ (pH meter) ตามวิธีการหาค่าแบบอีเล็คโตรเมตริก (Electrometric)

(๓) การตรวจสอบค่าออกซิเจนละลาย ให้ใช้วิธีอะไซด์โมดิฟิเคชั่น (Azide Modification)

(๔) การตรวจสอบค่าบีโอดี ให้ใช้วิธีอะไซด์โมดิฟิเคชั่น (Azide Modification) ที่อุณหภูมิ ๒๐ องศาเซลเซียส เป็นเวลา ๕ วันติดต่อกัน

(๕) การตรวจสอบค่าแบคทีเรียกลุ่มโคลิฟอร์มทั้งหมดและค่าแบคทีเรียกลุ่มฟีคอลโคลิฟอร์ม ให้ใช้วิธีมัลติเพิ้ล ทิ้วบ์ เฟอร์เมนเตชั่น เทคนิค (Multiple Tube Fermentation Technique)

(๖) การตรวจสอบค่าไนเตรตในหน่วยไนโตรเจน ให้ใช้วิธีแคดเมียมรีดัคชั่น (Cadmium Reduction)

(๗) การตรวจสอบค่าแอมโมเนียในหน่วยไนโตรเจน ให้ใช้วิธีดิสทิลเลชั่นเนสสเลอร์ไรเซชั่น (Distillation Nesslerization)

(๘) การตรวจสอบค่าฟีนอล ให้ใช้วิธีดิสทิลเลชั่น ๔ - อะมิโนแอนติไพรีน (Distillation, 4-Amino antipyrene)

(๙) การตรวจสอบค่าทองแดง นิคเกิล แมงกานีส สังกะสี แคดเมียม โครเมียมชนิดเฮ็กซาวาเล้นท์ และตะกั่ว ให้ใช้วิธีอะตอมมิค แอบซอพชั่น ไดเร็ค แอสไพเรชั่น (Atomic Absorption - Direct Aspiration)

(๑๐) การตรวจสอบค่าปรอททั้งหมด ให้ใช้วิธีอะตอมมิค แอบซอพชั่น โคลด์เวเปอร์ เทคนิค (Atomic Absorption-Cold Vapour Technique)

(๑๑) การตรวจสอบค่าสารหนู ให้ใช้วิธีอะตอมมิค แอบซอพชั่น แก๊สซัส ไฮไดรด์ (Atomic Absorption - Gaseous Hydride)

(๑๒) การตรวจสอบค่าไซยาไนด์ ให้ใช้วิธีไพริดีน บาร์บิทูริค แอซิด (Pyridine - Barbituric Acid)

(๑๓) การตรวจสอบค่ากัมมันตภาพรังสี ให้ใช้วิธีโลว์ แบ็คกราวด์ พร็อพพอร์ชั่นนอล เคาน์เตอร์ (Low Background Proportional Counter)

(๑๔) การตรวจค่าสารฆ่าศัตรูพืชและสัตว์ชนิดที่มีคลอรีนทั้งหมด ดีดีที บีเอชซีชนิดแอลฟา ดิลดริน อัลดริน เฮปตาคลอร์อีปอกไซด์ และเอนดริน ให้ใช้วิธีก๊าซ - โครมาโตกราฟี่ (Gas - Chromatography)

ข้อ ๑๑ การตรวจสอบค่าออกซิเจนละลายให้ใช้ค่าเปอร์เซ็นไทล์ที่ ๒๐ (20^{th} Percentile Value) ส่วนการตรวจสอบค่าบีโอดี แบคทีเรียกลุ่มโคลิฟอร์มทั้งหมด และแบคทีเรียกลุ่มฟีคอลโคลิฟอร์ม ให้ใช้ค่าเปอร์เซ็นไทล์ที่ ๘๐ โดยจำนวนและระยะเวลาสำหรับการเก็บตัวอย่างน้ำดังกล่าว ให้เป็นไปตามที่กรมควบคุมมลพิษกำหนด

ข้อ ๑๒ การเก็บตัวอย่างน้ำตามข้อ ๙ และการตรวจสอบคุณภาพน้ำตามข้อ ๑๐ จะต้องเป็นไปตามวิธีการมาตรฐานสำหรับการวิเคราะห์น้ำและน้ำเสีย (Standard Methods for Examination of Water and Wastewater) ซึ่ง American Public Health Association และ American Water Works Association กับ Water Pollution Control Federation ของสหรัฐอเมริกา ร่วมกันกำหนดไว้ด้วย

ประกาศ ณ วันที่ ๒๐ มกราคม พ.ศ. ๒๕๓๗
ชวน หลีกภัย
นายกรัฐมนตรี
ประธานคณะกรรมการสิ่งแวดล้อมแห่งชาติ

(ประกาศในราชกิจจานุเบกษา เล่ม ๑๑๑ ตอนที่ ๑๖ ง วันที่ ๒๔ กุมภาพันธ์ ๒๕๓๗)

ภาคผนวก จ

เอกสารสอบเทียบเครื่องมือที่ใช้ในการตรวจวิเคราะห์ (Calibration)

ตารางการสอบเทียบเครื่องมือที่ใช้ในการตรวจวัดและวิเคราะห์

Item	Description	Parameter	List of Equipment	Equipment No.	Calibration	Next Calibration
1.	Ambient Air	TSP	ORIFICE TRANSFER STANDARD/Tisch	S/N 0068	17/03/2026	March 2027
			High Volume Air Sampler/TET	S/N TSP-16	25/05/2026	May 2027
			High Volume Air Sampler/TET	S/N TSP-33	25/05/2026	May 2027
			High Volume Air Sampler/TET	S/N TSP-35	26/05/2026	May 2027
			High Volume Air Sampler/TET	S/N TSP-37	26/05/2026	May 2027
			Electronic Balance/XP 205 DR	S/N 1129273885	03/09/2025	September 2026
		PM-10	High Volume Air Sampler/TET	S/N PM10-2	25/05/2026	May 2027
			High Volume Air Sampler/TET	S/N PM10-16	25/05/2026	May 2027
			High Volume Air Sampler/TET	S/N PM10-28	25/05/2026	May 2027
			High Volume Air Sampler/TET	S/N PM10-30	25/05/2026	May 2027
			Electronic Balance/XP 205 DR	S/N 1129273885	03/09/2025	September 2026
		WS & WD	Wind Speed and Wind Direction/Weather Wizard III	S/N WC50206A21	09/01/2026	January 2027
2.	Sound Level	Leq 24 hr &	Sound Calibrator/ST-120	S/N ST120C0263E	20/10/2025	October 2026
		เสียงรบกวน	Sound Level Meter/ACO 6226	S/N 100102	15/06/2026	July 2026
			Sound Level Meter/ACO 6226	S/N 130127	15/06/2026	July 2026
			Sound Level Meter/ACO 6226	S/N 160211	15/06/2026	July 2026
			Sound Level Meter/ACO 6226	S/N 160213	15/06/2026	July 2026
3.	Water	pH	pH Meter/Horiba F-71G	S/N V3B1F8H3	28/10/2025	October 2026
		DO	DO Meter/HORIBA	S/N D75J0012	13/01/2026	January 2027
		BOD	BOD Incubator/Model i250	S/N 0408-0115-0008	09/03/2026	March 2027
		Cr^{+6}	Spectrophotometer/Perkin Elmer	S/N 365K9042909	07/11/2025	November 2026
		Pb, Cd, Ni	Atomic Absorption Spectrophotometer	S/N PZBS23100902	20/06/2025	27/06/2026
			Model/PinAAcle 900Z			

ตารางการสอบเทียบเครื่องมือที่ใช้ในการตรวจวัดและวิเคราะห์ (ต่อ)

Item	Description	Parameter	List of Equipment	Equipment No.	Calibration	Next Calibration
3.	Water (Cont.)	Total Hg, As	Atomic Absorption Spectrophotometer Model/AAnalyst 100	S/N 040S0110503	17/03/2026	September 2026
		Cu, Mn, Zn	ICP394/PerkinElmer/OPTIMA8000	S/N 078S1310024C	17/03/2026	September 2026
		Total Coliform Bacteria	Incubator Model INE 500	S/N E.505.0595	09/03/2026	March 2027
		Fecal Coliform Bacteria	Incubator Model INE 500	S/N E.505.1143	09/03/2026	March 2027
		NO_3	Spectrophotometer/Perkin Elmer	S/N 365K9042909	07/11/2025	November 2026
		Cyanide	Spectrophotometer/Perkin Elmer	S/N 365K9042909	07/11/2025	November 2026

JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Flow measurement laboratory
Calibration services department.

NSC – TISI – TIS 17025
CALIBRATION 0367

CERTIFICATE OF CALIBRATION

Certificate No. : COF-010-69

MEASUREMENT ITEM	: Top Load Orifice
MANUFACTURER	: TISCH
MODEL/TYPE	: TE-5025A
SERIAL NUMBER	: 0068
ID NUMBER	: -
CONDITION AS-RECEIVED	: Used item
CUSTOMER	: Thai Environmental Technic Limited. 1/6 Soi Ramkhamhaeng 145, Khwaeng/Khet Saphan Sung, Bangkok 10240
RECEIVED DATE	: 12 Mar 2026
MEASUREMENT DATE	: 17 Mar 2026
ISSUE DATE	: 17 Mar 2026

Calibration procedure:
The Orifice gas flow device was calibrated against Standard Rotary Displacement Meter (Roots Meter) Model G65/IMC/W2-dp. The WI-CL-004 was used as a calibration guideline.

Traceability:
This certificate provides a traceability of the measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MW-0005-26.

Uncertainty of Measurement:
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

ENVIRONMENTAL CONDITIONS:
Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa

CALIBRATION CONDITION:

Preconditioning	: 24 hours at ambient conditions.
Measurement Condition	: The average values during measurement are 23.8 °C and 48.0 %RH.

***NOTED:** The certificate is valid only to the item calibrated on date and place of calibration.*

TABULATION OF RESULTS:
The table on next page give the measured values.

Calibrated by:

☐ Mr. Sorawit Thachalad
☑ Miss Jittraporn Lertsomphol

JIRANATEE ASSOCIATES CO.,LTD.

Approved signatory: .....

Mr. Parinya Booncharoen
Calibration Department Manager

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

JNAC
JIRANATEE ASSOCIATES CO.,LTD.

MEASUREMENT RESULTS:

The Orifice gas flow device was calibrated by direct comparison method with the Standard Rotary Displacement Meter (Roots Meter). The Humid air was used as a medium in the system. The standard conditions are 25°C (298.15 K) and 760 mmHg for standard temperature and standard pressure respectively.

Table 1: The results of Q Standard calibration data

Plate	Flow rate m^3/min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Δp_meter mmHg	Δp_Orifice inH_2O	Y	Standard Flow [Q_s] m^3/min
1	0.705	757.085	23.72	22.84	51.234	1.704	1.306	0.659
2	0.998	757.085	23.72	23.18	54.876	3.388	1.841	0.928
3	1.120	757.007	23.72	23.18	37.899	4.468	2.114	1.066
4	1.170	757.082	23.71	23.16	27.798	5.041	2.246	1.130
5	1.418	757.025	23.67	23.12	27.451	7.428	2.726	1.370

Slope (m): **1.99819**

Intercept (b): **-0.01290**

Correlation coefficient (r): **0.99988**

Uncertainty (k=2): **0.015** **m^3/min**

Table 2: The results of Q actual calibration data

Plate	Flow rate m^3/min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Δp_meter mmHg	Δp_Orifice inH_2O	Y	Standard Flow [Q_a] m^3/min
1	0.705	757.085	23.72	22.84	51.234	1.704	0.817	0.659
2	0.998	757.085	23.72	23.18	54.876	3.388	1.153	0.928
3	1.120	757.007	23.72	23.18	37.899	4.468	1.324	1.066
4	1.170	757.082	23.71	23.16	27.798	5.041	1.406	1.129
5	1.418	757.025	23.67	23.12	27.451	7.428	1.707	1.369

Slope (m): **1.25154**

Intercept (b): **-0.00807**

Correlation coefficient (r): **0.99988**

Uncertainty (k = 2): **0.015** **m^3/min**

*****End of Certificate of Calibration*****

JNAC
JIRANATEE ASSOCIATES CO.,LTD.

Thai Environmental Technic Limited
บริษัท เทคนิคสิ่งแวดล้อมไทย จำกัด

High Volume TSP&PM-10 Calibration Report

Location : Thai Environmemtal Tech Site ID : Bangkok Date : 25-May-26

ITEM : TSP Serial No : (No.16) Calibrate By : Pipat

Site Conditions

Barometric Pressure (mm Hg) :	760.00	Corrected Pressure (mm Hg) :	760.0
Temperature (°C) :	25.0	Temperature (deg K) :	298.0
Average Press. (mm Hg) :	754.8	Corrected Average (mm Hg) :	-
Average Temp (°C) :	33.2	Average Temp: (Deg K) :	-

Calibration Orifice

Make : Tisch	Qstd Slope : 2.00326
Model : TE-5025A	Qstd Intercept : -0.02008
Serial# : 0068	Calibration Due Date : 26-Mar-26

Calibration Information

Plate or Test #	ORIFICE (in H_2O)	Qstd (m3/min)	Indicate (CFM)	IC (corrected)
1	12.30	1.761	58.0	58.00
2	9.30	1.532	54.0	54.00
3	7.20	1.349	50.0	50.00
4	5.00	1.126	40.0	40.00
5	3.00	0.875	30.0	30.00

Linear Regression
Slope : 32.3226
Intercept : 3.4534
Corr. Coeff : 0.9822
# of Observations: 5

Calculations

Qstd = 1/m[Sqrt(H2O(Pa/Pstd)(Tstd/Ta))-b]
IC =I[Sqrt(Pa/Pstd)(Tstd/Ta)]

Qstd = standard flow rate
IC = corrected chart response
I = actual chart response
m = calibrator Qstd slope
b = calibrator Qstd intercept
Ta = actual temperature during calibration (deg K)
Pa = actual pressure during calibration (mm Hg)
Tstd = 298 deg K
Pstd = 760 mm Hg
For subsequent calculation of sampler flow:
1/m((I)[Sqrt(298/Tav)(Pav/760)]-b)

m = sampler slope
b = sampler intercept
I = chart response
Tav = daily average temperature
Pav = daily average pressure

Calibrate By : _____

Approve By : _____

NOTE: Ensure calibration orifice has been certified within 12 months of use

Thai Environmental Technic Limited
บริษัท เทคนิคสิ่งแวดล้อมไทย จำกัด

High Volume TSP&PM-10 Calibration Report

Location : Thai Environmemtal Tech Site ID : Bangkok Date : 25-May-26
ITEM : TSP Serial No : (No.33) Calibrate By : Pipat

Site Conditions

Barometric Pressure (mm Hg) :	760.00	Corrected Pressure (mm Hg) :	760.0
Temperature (°C) :	25.0	Temperature (deg K) :	298.0
Average Press. (mm Hg) :	754.6	Corrected Average (mm Hg) :	-
Average Temp (°C) :	32.5	Average Temp: (Deg K) :	-

Calibration Orifice

Make : Tisch	Qstd Slope : 2.00326
Model : TE-5025A	Qstd Intercept : -0.02008
Serial# : 0068	Calibration Due Date : 26-Mar-26

Calibration Information

Plate or Test #	ORIFICE (in H_2O)	Qstd (m3/min)	Indicate (CFM)	IC (corrected)
1	12.30	1.761	60.0	57.00
2	9.60	1.557	54.0	52.00
3	7.20	1.349	50.0	48.00
4	5.00	1.126	40.0	40.00
5	3.00	0.875	30.0	30.00

Linear Regression
Slope : 30.1498
Intercept : 5.1934
Corr. Coeff : 0.9896
# of Observations: 5

Calculations

Qstd = 1/m[Sqrt(H2O(Pa/Pstd)(Tstd/Ta))-b]
IC =I[Sqrt(Pa/Pstd)(Tstd/Ta)]

Qstd = standard flow rate
IC = corrected chart response
I = actual chart response
m = calibrator Qstd slope
b = calibrator Qstd intercept
Ta = actual temperature during calibration (deg K)
Pa = actual pressure during calibration (mm Hg)
Tstd = 298 deg K
Pstd = 760 mm Hg
For subsequent calculation of sampler flow:
1/m((I)[Sqrt(298/Tav)(Pav/760)]-b)

m = sampler slope
b = sampler intercept
I = chart response
Tav = daily average temperature
Pav = daily average pressure

Calibrate By : _____

Approve By : Bamua M

NOTE: Ensure calibration orifice has been certified within 12 months of use

Thai Environmental Technic Limited
บริษัท เทคนิคสิ่งแวดล้อมไทย จำกัด

High Volume TSP&PM-10 Calibration Report

Location : Thai Environmemtal Tech | Site ID : Bangkok | Date : 26-May-26
ITEM : TSP | Serial No : (No.35) | Calibrate By : Pipat

Site Conditions

Barometric Pressure (mm Hg) :	760.00	Corrected Pressure (mm Hg) :	760.0
Temperature (°C) :	25.0	Temperature (deg K) :	298.0
Average Press. (mm Hg) :	754.8	Corrected Average (mm Hg) :	-
Average Temp (°C) :	29.8	Average Temp: (Deg K) :	-

Calibration Orifice

Make : Tisch	Qstd Slope : 2.00326
Model : TE-5025A	Qstd Intercept : -0.02008
Serial# : 0068	Calibration Due Date : 26-Mar-26

Calibration Information

Plate or Test #	ORIFICE (in H_2O)	Qstd (m3/min)	Indicate (CFM)	IC (corrected)
1	12.30	1.761	60.0	57.00
2	9.20	1.524	54.0	52.00
3	7.00	1.331	50.0	48.00
4	5.00	1.126	40.0	40.00
5	3.00	0.875	30.0	30.00

Linear Regression
Slope : 30.5013
Intercept : 5.0377
Corr. Coeff : 0.9864
# of Observations: 5

Calculations

Qstd = 1/m[Sqrt(H2O(Pa/Pstd)(Tstd/Ta))-b]
IC =I[Sqrt(Pa/Pstd)(Tstd/Ta)]

Qstd = standard flow rate
IC = corrected chart response
I = actual chart response
m = calibrator Qstd slope
b = calibrator Qstd intercept
Ta = actual temperature during calibration (deg K)
Pa = actual pressure during calibration (mm Hg)
Tstd = 298 deg K
Pstd = 760 mm Hg

For subsequent calculation of sampler flow:
1/m{(I)[Sqrt(298/Tav)(Pav/760)]-b}

m = sampler slope
b = sampler intercept
I = chart response
Tav = daily average temperature
Pav = daily average pressure

Calibrate By : _____

Approve By : _____

NOTE: Ensure calibration orifice has been certified within 12 months of use

Thai Environmental Technic Limited
บริษัท เทคนิคสิ่งแวดล้อมไทย จำกัด

High Volume TSP&PM-10 Calibration Report

Location : Thai Environmemtal Tech
Site ID : Bangkok
Date : 26-May-26
ITEM : TSP
Serial No : (No.37)
Calibrate By : Pipat

Site Conditions

Barometric Pressure (mm Hg) :	760.00	Corrected Pressure (mm Hg) :	760.0
Temperature (°C) :	25.0	Temperature (deg K) :	298.0
Average Press. (mm Hg) :	754.6	Corrected Average (mm Hg) :	-
Average Temp (°C) :	30.9	Average Temp: (Deg K) :	-

Calibration Orifice

Make : Tisch	Qstd Slope : 2.00326
Model : TE-5025A	Qstd Intercept : -0.02008
Serial# : 0068	Calibration Due Date : 26-Mar-26

Calibration Information

Plate or Test #	ORIFICE (in H_2O)	Qstd (m3/min)	Indicate (CFM)	IC (corrected)
1	12.30	1.761	60.0	57.00
2	9.40	1.540	54.0	52.00
3	7.20	1.349	50.0	48.00
4	5.00	1.126	40.0	40.00
5	3.00	0.875	30.0	30.00

Linear Regression
Slope : 30.3684
Intercept : 5.0004
Corr. Coeff : 0.9896
# of Observations: 5

Calculations

Qstd = 1/m[Sqrt(H2O(Pa/Pstd)(Tstd/Ta))-b]
IC =I[Sqrt(Pa/Pstd)(Tstd/Ta)]

Qstd = standard flow rate
IC = corrected chart response
I = actual chart response
m = calibrator Qstd slope
b = calibrator Qstd intercept
Ta = actual temperature during calibration (deg K)
Pa = actual pressure during calibration (mm Hg)
Tstd = 298 deg K
Pstd = 760 mm Hg
For subsequent calculation of sampler flow:
1/m((I)[Sqrt(298/Tav)(Pav/760)]-b)

m = sampler slope
b = sampler intercept
I = chart response
Tav = daily average temperature
Pav = daily average pressure

Calibrate By :

Approve By : Ramual M

NOTE: Ensure calibration orifice has been certified within 12 months of use

Thai Environmental Technic Limited
บริษัท เทคนิคสิ่งแวดล้อมไทย จำกัด

High Volume TSP&PM-10 Calibration Report

Location : Thai Environmemtal Tech | Site ID : Bangkok | Date : 25-May-26
ITEM : PM10 | Serial No : (No. 2) | Calibrate By : Pipat

Site Conditions

Barometric Pressure (mm Hg) :	760.00	Corrected Pressure (mm Hg) :	760.0
Temperature (°C) :	25.0	Temperature (deg K) :	298.0
Average Press. (mm Hg) :	754.6	Corrected Average (mm Hg) :	-
Average Temp (°C) :	32.5	Average Temp: (Deg K) :	-

Calibration Orifice

Make : Tisch	Qstd Slope : 2.00326
Model : TE-5025A	Qstd Intercept : -0.02008
Serial# : 0068	Calibration Due Date : 26-Mar-26

Calibration Information

Plate or Test #	ORIFICE (in H_2O)	Qstd (m3/min)	Indicate (CFM)	IC (corrected)
1	12.00	1.739	60.0	60.00
2	9.00	1.508	54.0	54.00
3	7.20	1.349	48.0	48.00
4	5.00	1.126	40.0	40.00
5	3.00	0.875	30.0	30.00

Linear Regression
Slope : 35.1083
Intercept : 0.0768
Corr. Coeff : 0.9970
# of Observations: 5

Calculations

Qstd = 1/m[Sqrt(H2O(Pa/Pstd)(Tstd/Ta))-b]
IC =I[Sqrt(Pa/Pstd)(Tstd/Ta)]

Qstd = standard flow rate
IC = corrected chart response
I = actual chart response
m = calibrator Qstd slope
b = calibrator Qstd intercept
Ta = actual temperature during calibration (deg K)
Pa = actual pressure during calibration (mm Hg)
Tstd = 298 deg K
Pstd = 760 mm Hg
For subsequent calculation of sampler flow:
1/m((I)[Sqrt(298/Tav)(Pav/760)]-b)

m = sampler slope
b = sampler intercept
I = chart response
Tav = daily average temperature
Pav = daily average pressure

Calibrate By : _____

Approve By : Ramnal M

NOTE: Ensure calibration orifice has been certified within 12 months of use

Thai Environmental Technic Limited
บริษัท เทคนิคสิ่งแวดล้อมไทย จำกัด

High Volume TSP&PM-10 Calibration Report

Location : Thai Environmemtal Tech Site ID : Bangkok Date : 25-May-26

ITEM : PM10 Serial No : (No. 16) Calibrate By : Pipat

Site Conditions

Barometric Pressure (mm Hg) : 760.00
Temperature (°C) : 25.0
Average Press. (mm Hg) : 754.6
Average Temp (°C) : 32.6

Corrected Pressure (mm Hg) : 760.0
Temperature (deg K) : 298.0
Corrected Average (mm Hg) : -
Average Temp: (Deg K) : -

Calibration Orifice

Make : Tisch
Model : TE-5025A
Serial# : 0068

Qstd Slope : 2.00326
Qstd Intercept : -0.02008
Calibration Due Date : 26-Mar-26

Calibration Information

Plate or Test #	ORIFICE (in H_2O)	Qstd (m3/min)	Indicate (CFM)	IC (corrected)
1	12.20	1.754	60.0	60.00
2	9.20	1.524	54.0	54.00
3	7.00	1.331	50.0	50.00
4	5.20	1.148	40.0	40.00
5	3.00	0.875	30.0	30.00

Linear Regression
Slope : 34.7105
Intercept : 0.7637
Corr. Coeff : 0.9878
# of Observations: 5

Calculations

Qstd = 1/m{Sqrt(H2O(Pa/Pstd)(Tstd/Ta))-b]
IC =I{Sqrt(Pa/Pstd)(Tstd/Ta)]

Qstd = standard flow rate
IC = corrected chart response
I = actual chart response
m = calibrator Qstd slope
b = calibrator Qstd intercept
Ta = actual temperature during calibration (deg K)
Pa = actual pressure during calibration (mm Hg)
Tstd = 298 deg K
Pstd = 760 mm Hg
For subsequent calculation of sampler flow:
1/m{(I){Sqrt(298/Tav)(Pav/760)}-b}

m = sampler slope
b = sampler intercept
I = chart response
Tav = daily average temperature
Pav = daily average pressure

Calibrate By : _____

Approve By : Pramual M

NOTE: Ensure calibration orifice has been certified within 12 months of use

Thai Environmental Technic Limited
บริษัท เทคนิคสิ่งแวดล้อมไทย จำกัด

High Volume TSP&PM-10 Calibration Report

Location : Thai Environmemtal Tech Site ID : Bangkok Date : 25-May-26
ITEM : PM10 Serial No : (No. 28) Calibrate By : Pipat

Site Conditions

Barometric Pressure (mm Hg) :	760.00	Corrected Pressure (mm Hg) :	760.0
Temperature (°C) :	25.0	Temperature (deg K) :	298.0
Average Press. (mm Hg) :	754.6	Corrected Average (mm Hg) :	-
Average Temp (°C) :	32.8	Average Temp: (Deg K) :	-

Calibration Orifice

Make : Tisch	Qstd Slope : 2.00326
Model : TE-5025A	Qstd Intercept : -0.02008
Serial# : 0068	Calibration Due Date : 26-Mar-26

Calibration Information

Plate or Test #	ORIFICE (in H_2O)	Qstd (m3/min)	Indicate (CFM)	IC (corrected)
1	12.20	1.754	60.0	60.00
2	9.20	1.524	54.0	54.00
3	7.20	1.349	50.0	50.00
4	5.00	1.126	40.0	40.00
5	3.00	0.875	30.0	30.00

Linear Regression
Slope : 34.5011
Intercept : 1.0647
Corr. Coeff : 0.9913
# of Observations: 5

Calculations

Qstd = 1/m[Sqrt(H2O(Pa/Pstd)(Tstd/Ta))-b]
IC =I[Sqrt(Pa/Pstd)(Tstd/Ta)]

Qstd = standard flow rate
IC = corrected chart response
I = actual chart response
m = calibrator Qstd slope
b = calibrator Qstd intercept
Ta = actual temperature during calibration (deg K)
Pa = actual pressure during calibration (mm Hg)
Tstd = 298 deg K
Pstd = 760 mm Hg
For subsequent calculation of sampler flow:
1/m((I)[Sqrt(298/Tav)(Pav/760)]-b)

m = sampler slope
b = sampler intercept
I = chart response
Tav = daily average temperature
Pav = daily average pressure

Calibrate By : _____

Approve By : Ramual M

NOTE: Ensure calibration orifice has been certified within 12 months of use

Thai Environmental Technic Limited
บริษัท เทคนิคสิ่งแวดล้อมไทย จำกัด

High Volume TSP&PM-10 Calibration Report

Location : Thai Environmemtal Tech Site ID : Bangkok Date : 25-May-26
ITEM : PM10 Serial No : (No. 30) Calibrate By : Pipat

Site Conditions

Barometric Pressure (mm Hg) :	760.00	Corrected Pressure (mm Hg) :	760.0
Temperature (°C) :	25.0	Temperature (deg K) :	298.0
Average Press. (mm Hg) :	754.8	Corrected Average (mm Hg) :	-
Average Temp (°C) :	31.2	Average Temp: (Deg K) :	-

Calibration Orifice

Make : Tisch	Qstd Slope : 2.00326
Model : TE-5025A	Qstd Intercept : -0.02008
Serial# : 0068	Calibration Due Date : 26-Mar-26

Calibration Information

Plate or Test #	ORIFICE (in H_2O)	Qstd (m3/min)	Indicate (CFM)	IC (corrected)
1	12.30	1.761	62.0	62.00
2	9.80	1.573	56.0	56.00
3	7.40	1.368	52.0	52.00
4	5.20	1.148	42.0	42.00
5	3.20	0.903	32.0	32.00

Linear Regression
Slope : 34.7710
Intercept : 1.8399
Corr. Coeff : 0.9914
# of Observations: 5

Calculations

Qstd = 1/m[Sqrt(H2O(Pa/Pstd)(Tstd/Ta))-b]
IC =I[Sqrt(Pa/Pstd)(Tstd/Ta)]

Qstd = standard flow rate
IC = corrected chart response
I = actual chart response
m = calibrator Qstd slope
b = calibrator Qstd intercept
Ta = actual temperature during calibration (deg K)
Pa = actual pressure during calibration (mm Hg)
Tstd = 298 deg K
Pstd = 760 mm Hg

m = sampler slope
b = sampler intercept
I = chart response
Tav = daily average temperature
Pav = daily average pressure

Calibrate By : _____

Approve By : _____

For subsequent calculation of sampler flow:
1/m((I)[Sqrt(298/Tav)(Pav/760)]-b)

NOTE: Ensure calibration orifice has been certified within 12 months of use

THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 9 January, 2026 Certification No. 028/26

Object : Wind speed and wind direction

Manufacturer : Davis Instruments Inc.

Type : Weather Wizard III

Serial No. : WC50206A21 ID No. : No.22

Customer : Thai Environmental Technic Limited.
1/6 Soi Ramkhamhaeng 145,
Khwaeng/Khet Saphan Sung, Bangkok 10240.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1006.9 hPa

NATIONAL STANDARD WIND TUNNEL :

: Micromanometer Theodor Friedrichs FC014 Serial No. 9310119

: HOOK GAGE NO 1425 Pitot Tube Theodor Friedrichs Type 0800.0000 serial 9023

N.I.S.T. Test Reference Number 731/241460 : Standard Velocity at 20 - 30 m/sec

: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)

Serial Number 110730029 (sensor 120629586)

JAPAN QUALITY ASSURANCE ORGANIZATION : Standard Velocity at 2 - 20 m/sec

Calibrated by : Signed :

Mr. Watcharapol Subwat Mr. Pisood Promsut

Mechanical Engineer

(Authorised Signatory)
for the Chief
Sub-Standard Instrument

METEOROLOGICAL DEPARTMENT

THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration

Certification No. 028/26

9 January, 2026

Standard	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
Ultrasonic Anemometer	Pressure	Vacumm	Velocity	Velocity	Correction
m/sec	inches H2O	inches H2O	m/sec	m/sec	m/sec
1.00	-	-	-	0.9	0.10
3.02	-	-	-	2.7	0.32
5.00	-	-	-	4.9	0.10
7.00	-	-	-	6.7	0.30
9.02	-	-	-	8.9	0.12
11.01	-	-	-	10.9	0.11
13.01	-	-	-	13.0	0.01
15.01	-	-	-	14.9	0.11
17.02	-	-	-	17.0	0.02
20.02	-	-	-	20.0	0.02

Vane Angel Bench Stand Model 18112 Young Meteorological Instruments	
WIND DIRECTION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	270

Calibrated by : Watcharapol

Mr. Watcharapol Subwat

Mechanical Engineer

Calibration & Test Section

Meteorological Instruments Bureau

METEOROLOGICAL DEPARTMENT

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-69/0029 **MTC No.** EEL. BP. 55/1068

CALIBRATION CERTIFICATE

Submitted by : Thai Environmental Technic Limited.

Address : 1/6 Soi Ramkhamhaeng 145, Saphan Sung, Saphan Sung, Bangkok, 10240.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Sound Calibrator

Manufacturer : Scarlet Tech

Model : ST-120

Serial No. : ST120C0263E

Ambient Environment

Temperature : (23 ± 3) °C

Relative Humidity : (50 ± 15) %

Ambient Pressure : (101.325 ± 1.500) kPa

Standards used :
1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.
2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.
3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.
4. Digital Multimeter Agilent 34401A S/N MY44005560.
5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.
6. Audio Analyzer Panasonic VP-7722A S/N 041477D122.
7. Condenser Microphone B&K 4180 S/N 2633526.

Calibration Procedure: CP-102-04 based on IEC 60942-2003. The sound pressure level of instrument was measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 15 Oct. 2025

Date of Calibration : 20 Oct. 2025

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-69/0029 **MTC No.** EEL. BP. 55/1068

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20μPa at 1000 Hz

Acoustic Output in dB re 20μPa , Corrected to Reference Conditions : 101.325 kPa , 23.0°C and 50 %RH

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	94.08	0.08	± 0.10	±0.40 dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	997.1	-2.9	± 1.5	±1.0%

3. Total distortion

Standard Microphone Type	Measured Total distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	0.76	± 0.50	±3.0%

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Date of Calibration : 20 Oct. 2025

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-69/0029 **MTC No.** EEL. BP. 55/1068

Nominal Output of Unit Under Test = 114 dB re 20μPa at 1000 Hz

Acoustic Output in dB re 20μPa , Corrected to Reference Conditions : 101.325 kPa , 23.0 °C and 50 %RH

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	114.15	0.15	± 0.10	±0.40 dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	997.2	-2.8	± 1.5	±1.0%

3. Total Distortion

Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	0.19	± 0.50	±3.0%

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Calibrated by :

.....

(Mr.Weerachai Deechaiyac)

Approved by :

.....

(Mr.[illegible]pa)

Director

วว.TISTR

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 20 Oct. 2025

Date of Issue : 22 Oct. 2025

Ref : 20112681015041050O1

End of Certificate

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

Thai Environmental Technic Limited
บริษัท เทคนิคสิ่งแวดล้อมไทย จำกัด

Sound Level Meter Calibration Report

Equipment Type	: Sound Level Meter	**Calibration Date**	: 15-June-2026
Calibrator	: SCARLET ST-120	**Barometric pressure (mmHg)**	: 759.0 mmHg
Standard	: IEC 60942:2017 CLASS1	**Temperature (23±3)°C**	: 25 °C
Accuracy	: 94.0 ±0.3 dB and 114.0±0.5 dB	**Relative Humidity(50±15 %)**	: 50 % RH
Frequency	: at 1,000 Hz ±1%	**Dued Date of Calibrate**	: 14-July-2026
Calibrator Serial NO.	: ST120C0263E		

Item	Instrument Calibrated			Reference	Before Adjust				After Adjust	Deviation	Result
	Brand	Model	Serial NO.	Acoustic dB	ครั้งที่1	ครั้งที่ 2	ครั้งที่ 3	เฉลี่ย	± dB	± dB	Calibrate
23	RION	NL-21	00487676	94.0	94.1	94.1	94.1	94.1	94.0	0.1	PASS
				114.0	114.0	114.0	114.0	114.0			
28	ACO	6226	100101	94.0	94.1	94.1	94.1	94.1	94.0	0.1	PASS
				114.0	114.1	114.1	114.1	114.1			
29	ACO	6226	100102	94.0	94.1	94.1	94.1	94.1	94.0	0.1	PASS
				114.0	114.0	114.0	114.0	114.0			
30	ACO	6226	100106	94.0	93.8	93.8	93.8	93.8	94.0	0.2	PASS
				114.0	113.8	113.8	113.8	113.8			
31	ACO	6226	110098	94.0	94.1	94.1	94.1	94.1	94.0	0.1	PASS
				114.0	114.1	114.1	114.1	114.1			
32	ACO	6226	110105	94.0	94.1	94.1	94.1	94.1	94.0	0.1	PASS
				114.0	114.1	114.1	114.1	114.1			
34	ACO	6226	110099	94.0	94.1	94.1	94.1	94.1	94.0	0.1	PASS
				114.0	114.0	114.0	114.0	114.0			

Calibration By :

Approve by : Ramnad M

Thai Environmental Technic Limited
บริษัท เทคนิคสิ่งแวดล้อมไทย จำกัด

Sound Level Meter Calibration Report

Equipment Type	: Sound Level Meter	**Calibration Date**	: 15-June-2026
Calibrator	: SCARLET ST-120	**Barometric pressure (mmHg)**	: 759.0 mmHg
Standard	: IEC 60942:2017 CLASS1	**Temperature (23±3)°C**	: 25 °C
Accuracy	: 94.0 ±0.3 dB and 114.0±0.5 dB	**Relative Humidity(50±15 %)**	: 50 % RH
Frequency	: at 1,000 Hz ±1%	**Dued Date of Calibrate**	: 14-July-2026
Calibrator Serial NO.	: ST120C0263E		

Item	Instrument Calibrated			Reference	Before Adjust				After Adjust	Deviation	Result
	Brand	Model	Serial NO.	Acoustic dB	ครั้งที่1	ครั้งที่ 2	ครั้งที่ 3	เฉลี่ย	± dB	± dB	Calibrate
35	ACO	6226	110097	94.0	94.1	94.1	94.1	94.1	94.0	0.1	PASS
				114.0	114.1	114.1	114.1	114.1			
36	ACO	6226	110102	94.0	93.9	93.9	93.9	93.9	94.0	0.1	PASS
				114.0	114.0	114.0	114.0	114.0			
37	ACO	6226	110101	94.0	93.7	93.7	93.7	93.7	94.0	0.3	PASS
				114.0	113.7	113.7	113.7	113.7			
38	ACO	6226	110106	94.0	94.2	94.2	94.2	94.2	94.0	0.2	PASS
				114.0	114.1	114.1	114.1	114.1			
39	ACO	6226	110104	94.0	94.1	94.1	94.1	94.1	94.0	0.1	PASS
				114.0	114.0	114.0	114.0	114.0			
40	ACO	6226	110100	94.0	94.1	94.1	94.1	94.1	94.0	0.1	PASS
				114.0	114.1	114.1	114.1	114.1			
41	ACO	6226	130127	94.0	93.9	93.9	93.9	93.9	94.0	0.1	PASS
				114.0	114.0	114.0	114.0	114.0			
42	ACO	6226	130128	94.0	93.7	93.7	93.7	93.7	94.0	0.3	PASS
				114.0	113.7	113.7	113.7	113.7			
44	ACO	6226	130130	94.0	94.1	94.1	94.1	94.1	94.0	0.1	PASS
				114.0	114.1	114.1	114.1	114.1			
45	ACO	6226	130131	94.0	94.1	94.1	94.1	94.1	94.0	0.1	PASS
				114.0	114.0	114.0	114.0	114.0			

Calibration By : .....

Approve by : .....

Thai Environmental Technic Limited
บริษัท เทคนิคสิ่งแวดล้อมไทย จำกัด

Sound Level Meter Calibration Report

Equipment Type	: Sound Level Meter	**Calibration Date**	: 15-June-2026
Calibrator	: SCARLET ST-120	**Barometric pressure (mmHg)**	: 759.0 mmHg
Standard	: IEC 60942:2017 CLASS1	**Temperature (23±3)°C**	: 25 °C
Accuracy	: 94.0 ±0.3 dB and 114.0±0.5 dB	**Relative Humidity(50±15 %)**	: 50 % RH
Frequency	: at 1,000 Hz ±1%	**Dued Date of Calibrate**	: 14-July-2026
Calibrator Serial NO.	: ST120C0263E		

Item	Instrument Calibrated			Reference	Before Adjust				After Adjust	Deviation	Result
	Brand	Model	Serial NO.	Acoustic dB	ครั้งที่1	ครั้งที่ 2	ครั้งที่ 3	เฉลี่ย	± dB	± dB	Calibrate
57	ACO	6226	160099	94.0	94.1	94.1	94.1	94.1	94.0	0.1	PASS
				114.0	114.1	114.1	114.1	114.1			
58	ACO	6226	160143	94.0	94.2	94.2	94.2	94.2	94.0	0.2	PASS
				114.0	114.1	114.1	114.1	114.1			
59	ACO	6226	160203	94.0	94.2	94.2	94.2	94.2	94.0	0.2	PASS
				114.0	114.0	114.0	114.0	114.0			
60	ACO	6226	160204	94.0	94.2	94.2	94.2	94.2	94.0	0.2	PASS
				114.0	114.0	114.0	114.0	114.0			
61	ACO	6226	160205	94.0	93.8	93.8	93.8	93.8	94.0	0.2	PASS
				114.0	113.8	113.8	113.8	113.8			
62	ACO	6226	160211	94.0	94.1	94.1	94.1	94.1	94.0	0.1	PASS
				114.0	114.1	114.1	114.1	114.1			
63	ACO	6226	160212	94.0	93.9	93.9	93.9	93.9	94.0	0.1	PASS
				114.0	114.0	114.0	114.0	114.0			
64	ACO	6226	160213	94.0	93.7	93.7	93.7	93.7	94.0	0.3	PASS
				114.0	113.7	113.7	113.7	113.7			
66	ACO	6226	160215	94.0	94.2	94.2	94.2	94.2	94.0	0.2	PASS
				114.0	114.1	114.1	114.1	114.1			
67	ACO	6226	160216	94.0	93.9	93.9	93.9	93.9	94.0	0.1	PASS
				114.0	113.9	113.9	113.9	113.9			

Calibration By :

Approve by :

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

ilac-MRA

NSC-TISI-TIS17025
CALIBRATION 0008

Certificate of Calibration

Cert.No.: 25CHO572
Page.: 1 of 2

Equipment :	pH Meter
Manufacturer :	Horiba
Model :	F-71G
Serial No. :	V3B1F8H3
ID No. :	Ins-LAB-025
Condition As-Received:	Used Item
Received Date :	28 October 2025
Calibration Date :	28 October 2025
Reference :	2510-0662OC-1
Submitted by :	Thai Environmental Technic Limited 1/6 Soi Ramkhamhaeng 145, Khwaeng/Khet Saphan Sung, Bangkok 10240
Calibration Place :	Laboratory (Thai Environmental Technic Limited)
Ambient Temperature :	(27.1 to 26.2) °C (On-Site)
Relative Humidity :	(56 to 59) % (On-Site)
Calibration Procedure :	In - house method : - CP-OCH2 by direct measurement with DC voltage standard and direct measurement with certified reference material (CRM)
Calibrated by :	Uthen Kankawi
Approved by :	Saithip Approved Signatory

( ) Chakrit Waewwanjua
( ) Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 30 October 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Condition of this calibration result

1. Reference Standard Instrument

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1) Document Process Calibrator	58440003	130RC120	24E3731	14 Nov 2025
2) Digital Thermometer	-	130RC017	25T625	23 Apr 2026

- This measurement result is traceable to SI through Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.007	CPA chem	1114384	12 Jun 2027
pH 6.876	CPA chem	1005301	15 Jun 2026
pH 9.180	CPA chem	1135356	16 Aug 2026

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4,7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement	Coverage factor
	pH	mV	mV	pH	(±mV)	*k*
pH Meter	4.000	177.48	177.5	4.000	0.058	2.00
S/N.: V3B1F8H3	6.860	8.28	8.3	6.860	0.058	2.00
	7.000	0.00	0.0	7.000	0.058	2.00
	9.180	-128.97	-128.9	9.180	0.058	2.00
	10.000	-177.48	-177.4	10.000	0.058	2.00

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7,9)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (±)	Coverage factor *k*
pH Electrode	4.007	4.007	168.7	0.0048	2.00
S/N.: 9X2E0223	6.876	6.875	1.2	0.0086	2.00
	9.180	9.176	-134.4	0.014	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

METROLOGY SYSTEM (THAILAND) CO.,LTD.

A Trescal company

69/29 Moo 1 Klongsi Klongluang Pathumthani 12120 Tel: (662) 193-2217-20 www.spmetrology.co.th www.สอบเทียบเครื่องมือวัด.com

Certificate of Calibration

Certificate Number : SPR26010053-2 Page : 1 of 3

Customer : Thai Environmental Technic Limited.
1/6 Soi Ramkhamhaeng 145, Khwaeng Saphan Sung, Khet Saphan Sung, Bangkok 10240, Thailand.

Equipment Name	:	DO Meter			
Manufacturer	:	Horiba			
Model	:	OM-71G			
Serial Number	:	D75J0012			
ID. Number	:	No.07			
Environmental Conditions					
Ambient Temperature	:	23 °C ± 2 °C	Received Date	:	09 Jan 2026
Relative Humidity	:	50 % ± 15 %	Calibration Date	:	13 Jan 2026
Location of Calibration	:	In-Lab	Recommend Due Date	:	13 Jan 2027
Calibration Procedure	:	In-House Method	Date of Issue	:	14 Jan 2026

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received.Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full,without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Kijja Visitsilp
Calibration Officer

Approved by

SPM A Trescal SP Metrology System (Thailand) Co., Ltd.

(Mr.Poothipong A.)
Authorized Signatory

SP METROLOGY SYSTEM (THAILAND) CO.,LTD.
A Trescal company

Calibration Report

Certificate Number : SPR26010053-2

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Zero Oxygen Solution	HI7040L	Lot S0027-23 _	21C31	21 Mar 2028

Traceability

This certification is traceable to the International System of Unit maintained at :

HANNA - Hanna Instruments (Thailand) Ltd.

69/29 Moo 1 Klongsi Klongluang Pathumthani 12120 Tel: (662) 193-2217-20 www.spmetrology.co.th www.สปเมตรอโลยี.com

METROLOGY SYSTEM (THAILAND) CO.,LTD.
A Trescal company

Result of Calibration

Certificate Number : SPR26010053-2

Dissolved Oxygen Permanance Test

Jnit : mg/L

Actual Standard	UUC Reading	Error	Uncertainty (±)
0.00	0.44	0.44	0.13
8.26	6.28	-1.98	0.13

Note :

The result of calibration was found accurate as show on date and place of calibration only. This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor k = 2.00, providing a level of confidence approximately 95%.

- End of Certificate -

69/29 Moo 1 Klongsi Klongluang Pathumthani 12120 Tel: (662) 193-2217-20 www.spmetrology.co.th www.ศูนย์เทียบเครื่องมือวัด.com

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

ilac-MRA

NSC-TISI-TIS17025
CALIBRATION 0008

Certificate of Calibration

Cert. No.: 26TM425
Page : 1 of 3

Equipment :	BOD Incubator
Manufacturer :	Accuplus
Model :	I250
Serial No. :	0408-0115-0008
ID No. :	Ins-LAB-046
Submitted by :	Thai Environmental Technic Limited 1/6 Soi Ramkhamhaeng 145, Khwaeng/Khet Saphan Sung, Bangkok 10240
Location :	Laboratory (Thai Environmental Technic Limited)
Received Order :	09 March 2026
Calibration Date :	09 March 2026
Ambient Temperature :	(26 ± 10) °C
Relative Humidity :	(50 ± 30) %
AC Line Voltage :	(220 ± 22) V

Calibrated by : Preecha Hlahib

Approved by : Kunchit

Approved Signatory

( ) Chakrit Waewwanjua
( ) Suwit Imjai
(✓) Kunchit Promprat

Issue Date : 21 March 2026

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Equipment : BOD Incubator
Condition As-Received : Used Item
Reference : 2603-0127OC-10

Cert. No.: 26TM425

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-


Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY49023932	25LM121	TPA,	27 Jul 2026

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This measurement result is traceable to the International System of Unit maintained through :

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Not Available

Environment during calibration		
	Beginning	Finished
Temp. (°C)	27	26
REL.Humid. (%)	56	59
AC Supply (Volt)	220	220

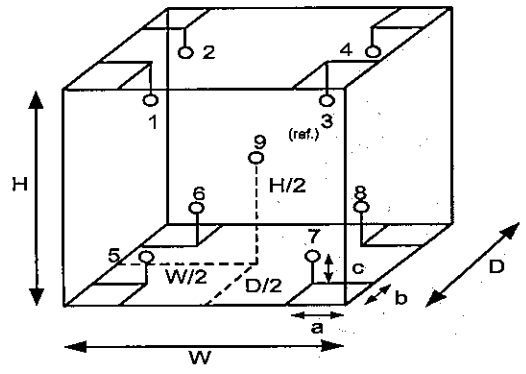

Position :	Ref. Std. ID No.:
1	19-16RTD-01
2	19-16RTD-02
3	19-16RTD-03
4	23-16RTD-04
5	19-16RTD-05
6	19-14RTD-06
7	21-16RTD-07
8	19-16RTD-08
9 (ref.)	19-16RTD-09

Probe Installation Details :

a =	10	cm
b =	10	cm
c =	10	cm

Dimension of Chamber :

D =	0.48	m
W =	0.50	m
H =	1.1	m
Capacity =	0.26	m^3

Equipment : BOD Incubator
Condition As-Received : Used Item
Reference : 2603-0127OC-10
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Not Available

Cert. No.: 26TM425

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor *k*
20.0	20.0	20.0	0.48	0.48	1.1	2

Calibration Point (°C)	Measured Temperature (°C) Position									Uncertainty (±°C)
	1	2	3	4	5	6	7	8	9 (ref.)	
20.0	20.313	20.256	20.108	20.244	20.183	20.157	19.969	19.986	20.121	0.64

Average* : The average of 30 values in each position.
Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.
Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.
Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.
UUC* : Unit Under Calibration
Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor ***k***, providing a level of confidence of approximately 95 %.

-o0o-

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Certificate of Calibration

Cert.No.: 25CHO582

Equipment :	Spectrophotometer
Manufacturer :	Perkin Elmer
Model :	Lambda 365
Serial No. :	365K9042909
ID No. :	-
Condition As-Received:	Used Item
Received Date :	07 November 2025
Calibration Date :	07 November 2025
Reference :	2511-0009OC-1
Submitted by :	Thai Environmental Technic Limited 1/6 Soi Ramkhamhaeng 145, Khwaeng/Khet Saphan Sung, Bangkok 10240
Calibration Place :	Laboratory (Thai Environmental Technic Limited)
Ambient Temperature :	(26.4 to 26.5) °C (On-Site)
Relative Humidity :	(64.1 to 62.9) % (On-Site)
Calibration Procedure :	In - house method : CP-OCH4 based on ASTM E 275-08
Calibrated by :	Uthen Kankawi
Approved by :	Saithip Approved Signatory

( ) Chakrit Waewwanjua
( ) Ponpan Palpim
(✓) Saithip Meangmai

Issue Date : 07 November 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Condition of calibration result

1. Reference Standard Material :

Material	Serial No.	Certificate No.	Due date
1. Absorbance Standard set	44487	122584	31 May 2026
2. Wavelength Standard set	29829	135831	06 Oct 2027
3. Wavelength Standard set	29829	135832	06 Oct 2027
4. Stray Light Standard set	45507	126055	04 Oct 2026

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certificate is traceable to the International System of Unit maintained through :
   - Starna Scientific Ltd.
4. Spectral BandWidth : 1 nm
   Scan Speed : 30 nm/min

Calibration Results : without adjustment

Wavelength Accuracy

Certified Values of Reference Material (nm)	UUC Reading (nm)	Uncertainty of Measurement (± nm)	Coverage Factor *k*
418.53	418.35	0.12	2.00
536.52	536.15	0.13	2.00
638.00	637.90	0.13	2.00
684.50	684.49	0.12	2.00
879.41	879.18	0.12	2.00

Calibration Results : without adjustment

Photometric Accuracy

Wavelength (nm)	Certified Values of Reference Material (Abs)	UUC Reading (Abs)	Uncertainty of Measurement (±Abs)	Coverage Factor *k*
420.0	Zero	0.0000	0.0028	2.00
	0.5750	0.5726	0.0028	2.00
	0.7156	0.7138	0.0028	2.00
	1.0176	1.0140	0.0028	2.00
546.1	Zero	0.0000	0.0028	2.00
	0.5234	0.5217	0.0028	2.00
	0.7007	0.6985	0.0028	2.00
	0.9992	0.9957	0.0028	2.00
635.0	Zero	0.0000	0.0028	2.00
	0.5648	0.5638	0.0028	2.00
	0.7654	0.7651	0.0028	2.00
	1.0961	1.0939	0.0028	2.00

Stray Light

* Straylight at 260.57 ± 0.11 nm	Reading at 260.57 ± 0.11 nm
Abs	1.7208
%T	0.7459

Remark

- Each individual filter is measured against the empty filter holder (blank) used to zero the spectrophotometer
- The Potassium Dichromate filled cells are measured against a Perchloric acid blank.
- Cut-off wavelength of stray light reference material (Potassium Iodide) at Wavelength 260.57 ± 0.11 nm
- Result = Pass, If Absorbance > 2.00 Abs and Transmission < 1.0 %T at Wavelength 260.57 ± 0.11 nm
- * : Not NSC-ONSC Accredited
- UUC = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k* , providing a level of confidence of approximately 95 %.

-o0o-

PerkinElmer
For the Better

WO-07108030/2025

MAINTENANCE REPORT AND CALIBRATION CERTIFICATE

ATOMIC ABSORPTION SPECTROPHOTOMETER MODEL

PinAACle 900Z

Customer :	THAI ENVIRONMENTAL	Date Tested:	June 20, 2025
	TECHNIC LIMITED	Recommendation Recertification	
Address :	1/6 Soi Ramkhamheang 145	Period	12 Months
	Khwaeng/Khet Saphan Sung	Recertification Due:	June 19, 2026
	Bangkok 10240	Date Last Certified:	December 30, 2024
User Name:	Khun Kanokwan Rermprachathipatai	Visit Number:	1 of 2
Phone:	02-7353101-3	PerkinElmer Phone:	02-719-6420 ext 8
Fax:	phorntip.p@tet1995.com	PerkinElmer Fax:	02-318-5597
	admin@tet1995.com		

CONFIGURATION TESTED

MODEL	SERIAL NUMBER	SOFTWARE
PinAACle 900Z	PZBS23100902	Syngristix V 5.1
AS 900	AS9C23047632	

TEST STANDARD USED	PART NUMBER	EXPIRATION DATE
GFAAS Mixed standard	N9300244	DEC 30 ,2025

PerkinElmer Scientific (Thailand) Co., Ltd.
290 Soi Soonvijai 4, Bangkapi, Huay Kwang, Bangkok 10310 Head Office

PerkinElmer
For the Better

MAINTENANCE REPORT AND CALIBRATION CERTIFICATE

ATOMIC ABSORPTION SPECTROPHOTOMETER MODEL

PinAACle 900Z

SERIAL NUMBER- PZBS23100902 DATE TESTED June 20, 2025

1. INSTRUMENT CHECKS	
A. The Mirror and Lenses Condition	OK
B. Grating Condition	OK
C. Replace or Clean Dust Filter	OK
D. Cleaning the Contact Cylinders	OK
E. Cleaning the Furnace Windows	OK
2. AUTOSAMPLE CHECK	
A. Sampling and Arm	OK
B. Sampling & Rinse Pump	OK
C. Sample Position & Clean	OK
3. COOLING SYSTEM CHECKS	
A. Clean and Change Distill water	OK
B. Themosensor	OK
4. FIAS CHECKS	
A. Pump and 5 Port Valve	OK
B. Chemifold and Tubing	OK
C. Power Supply	OK
D. Flow meter and Gas system	OK

PerkinElmer Scientific (Thailand) Co., Ltd.
290 Soi Soonvijai 4, Bangkapi, Huay Kwang, Bangkok 10310 Head Office

PerkinElmer
For the Better

WO-07108030/2025

MAINTENANCE REPORT AND CALIBRATION CERTIFICATE

ATOMIC ABSORPTION SPECTROPHOTOMETER MODEL

PinAACle 900Z

SERIAL NUMBER PZBS23100902 DATE TESTED June 20, 2025

PARAMETER	SPECIFICATION	ACTUAL VAULE	
THGA Tests			
1. Furnace Gas Flows			
Internal Flow	250 ± 25 mL/min	250	mL/min
External Flow	100 ± 10 mL/min	100	mL/min
2. Chromium Baseline Noise (357.87 nm)			
(mesure 5 furnace dry firings without any sample)			
	Baseline ≤ 0.005 Int.Abs	0.001	Int.Abs
	SD ≤ 0.005 Int.Abs	0.0005	int.Abs
3. Chromium Characteristic Mass(m_0) and Precition (357.87 nm)			
(measure 5 furnace firing using 20 ul			
sample injections of 10 ug/L Cr standard)			
	m_0 Results ≤ 7.0 pg/0.0044A-s	6.6	pg/0.0044A-s
	Precision ≤ 2.0%	0.78	%
4. Copper Characteristic Mass(m_0) and Zeeman Ratio (324.75 nm)			
(measure 5 furnace firing using 20 ul			
sample injections of 25 ug/L Cu standard)			
	m_0 Results ≤ 17.0 pg/0.0044A-s	16.3	pg/0.0044A-s
	Zeeman Ratio 0.52 ± 0.04	0.494	

PerkinElmer Scientific (Thailand) Co., Ltd.
290 Soi Soonvijai 4, Bangkapi, Huay Kwang, Bangkok 10310 Head Office

PerkinElmer
For the Better

MAINTENANCE REPORT AND CALIBRATION CERTIFICATE

ATOMIC ABSORPTION SPECTROPHOTOMETER MODEL

PinAACle 900Z

SERIAL NUMBER PZBS23100902 **DATE TESTED** June 20, 2025

Remarks :

Zeeman Ratio = $\frac{\text{Atomic Signal(peak area)}}{\text{Atomic Signal(peak area)+Backgroung Signal(peak area)}}$

= 0.1360/ (0.1360+0.1395)

= 0.494

This is to certify that the above tests have been perfomed and the configuration tested

[✔] meets

[ ] does not meet

the PerkinElmer Specifications listed on this certificate.

This certificate does not modify PerkinElmer's standard terms and condition of sale, including warranty terms.

Service Department PerkinElmer Ltd.

Customer Service Engineer: วิพัฒน์ พรหมลุมดา

(Wiphan Promlumda)

Service Engineer

PerkinElmer Scientific (Thailand) Co., Ltd.
290 Soi Soonvijai 4, Bangkapi, Huay Kwang, Bangkok 10310 Head Office

PerkinElmer TruQ

Atomic Spectroscopy Standard

ISO 9001 CERTIFIED

Certificate of Analysis

PerkinElmer Number: N9300244
Description: GFAAS Mixed Standard
Matrix: 5% HNO_3 / Tr. HF / Tr. Tart. Acid
Lot Number: 63-011CRY1

Certification Date: JUN - - 2024
Expiration Date: DEC 3 0 2025

*** Instrumental Analysis using ICP Spectrometer:**

Analyte	Labeled	Measured	SRM	Analyte	Labeled	Measured	SRM
Al	100 µg/mL	100 µg/mL	3101a*	Cu	50.0 µg/mL	50.6 µg/mL	3114*
As	100 µg/mL	101 µg/mL	3103a*	Ni	50.0 µg/mL	50.7 µg/mL	3136*
Pb	100 µg/mL	100 µg/mL	3128*	Cr	20.0 µg/mL	19.8 µg/mL	3112a*
Sb	100 µg/mL	101 µg/mL	3102a*	Fe	20.0 µg/mL	20.2 µg/mL	3126a*
Se	100 µg/mL	100 µg/mL	3149*	Mn	20.0 µg/mL	19.8 µg/mL	3132*
Tl	100 µg/mL	99.8 µg/mL	3158*	Ag	10.0 µg/mL	10.0 µg/mL	3151*
Ba	50.0 µg/mL	49.9 µg/mL	3104a*	Be	5.00 µg/mL	5.02 µg/mL	3105a*
Co	50.0 µg/mL	50.0 µg/mL	3113*	Cd	5.00 µg/mL	5.00 µg/mL	3108*

* - Indicates NIST SRM † - Indicates CRM (when NIST SRM is not available)

Reference Multi: Lot# 60-004CR, 58-142CR

Refer to side 2 for details of certification.

Balances are calibrated with weight sets traceable to NIST.

We guarantee that our PerkinElmer TruQ Atomic Spectroscopy Standards are stable and accurate to ±0.5% of certified concentration until the expiration date, provided the standards are kept tightly capped and stored under normal laboratory conditions. This value is the sum of cumulative errors associated with the analytical determinations, pipetting, and diluting to final volume. For these solutions we use high purity acids, ASTM Type I water (18 megohm double deionized), and leached, triple-rinsed bottles. All glassware used is class A.

Certifying Officer: Y. Parikh

PerkinElmer®

PerkinElmer, Inc.

U.S.A. Tel: 1-203-925-4600
U.S.A. Toll Free: 1-800-762-4000

Visit www.perkinelmer.com/lasoffices for a complete listing of our global offices.

MAINTENANCE REPORT

ATOMIC ABSORPTION SPECTROPHOTOMETER MODEL

AAnalyst 100

Customer :	บริษัท เทคนิคสิ่งแวดล้อมไทย จำกัด	Date Tested:	17-มี.ค.-69
Address :	1/6 ซอยรามคำแหง 145, แขวงสะพานสูง, เขตสะพานสูง, กรุงเทพฯ 10240 TH	Recommendation Recertification Period	6 Months
		Recertification Due:	17-ก.ย.-69
		Date Last Certified:	19-ก.ย.-68
User Name:	คุณ กิตติศักดิ์ เมืองงาม	Visit Number:	ONE
Phone:	02-3737799	TH ONE SOURCE Phone:	081-7316733
E-mail:	Ketsarin.Chuayphin@eurofinsasia.com	E-mail:	thonesource@gmail.com

CONFIGURATION TESTED

MODEL	SERIAL NUMBER	SOFTWARE
AAnalyst 100	040S0110503	AA WinLab 3.2

TEST STANDARD USED	PART NUMBER
Copper	N9300183
Filter 0.2 %	MG0-057

MAINTENANCE REPORT

ATOMIC ABSORPTION SPECTROPHOTOMETER MODEL

AAnalyst 100

SERIAL NUMBER 040S0110503 **DATE TESTED** 17-มี.ค.-69

1. OPTIC CHECKS

A. Optical alignment condition (if necessary)	OK
B. Condition of Mirrors,Lenses etc.(if necessary)	OK

2. GAS SYSTEM CHECKS

A. Leak test all internal and extenal gas box joints	OK
B. All gas box safety features	OK
C. Burner system including nebulizer and all o-ring and gasket	OK
D. Drain system (safety)	F

3. ELECTRONICS CHECKS

A. Power Supplies

+ 5.00 Vdc ± 0.2 Vdc	+ 5.02 Vdc
+ 11.50 Vdc ± 0.2 Vdc	+ 11.41 Vdc
+ 15.00 Vdc ± 1.0 Vdc	+14.98 Vdc
- 15.00 Vdc ± 1.0 Vdc	-15.03 Vdc
+ 35.00 Vdc ± 3.0 Vdc	+35.2 Vdc

4. WAVELENGTH ACCURACY TEST

A. Zn Lamp wavelength 213.9 nm ± 0.3 nm.	213.9 nm.
B. Fe Lamp wavelength 248.3 nm ± 0.3 nm.	248.24 nm.
C. Cu Lamp wavelength 324.8 nm ± 0.3 nm.	324.84 nm.

TH ONE SOURCE Co.,Ltd. 33/119, T.Ladsawai, A.Lam Luk Ka, Pathum Thani 12150, Thailand

MAINTENANCE REPORT

ATOMIC ABSORPTION SPECTROPHOTOMETER MODEL

AAnalyst 100

SERIAL NUMBER	040S0110503	**DATE TESTED**	17-มี.ค.-69

5. PERFORMANCE TESTS	**SPEC.**	**RESULTS**
*A. Neutral density filter checks with Copper (324.8 nm)		
Neutral Density Filter 0.2 Abs,	**0.180 ± 10%**	0.171 Abs.
B. AA Baseline noise test with Copper (324.8 nm)		
Integration time = 0.5 seconds		
Replicates = 99 times		
Standard Deviation	**≤ 0.001**	0.000
C. Flame sensitivity with Copper (324.8nm)		
(5 mg/L Cu Standard a read time of 10 seconds		
10 replicates, standard burner)		
Stainless steel nebulizer	**≥ 0.25**	0.305 Abs.
%RSD		0.56 %
Measured Characteristic Concentration :		0.072 mg/L

TH ONE SOURCE Co.,Ltd. 33/119, T.Ladsawai, A.Lam Luk Ka, Pathum Thani 12150, Thailand

MAINTENANCE REPORT

ATOMIC ABSORPTION SPECTROPHOTOMETER MODEL

AAnalyst 100

SERIAL NUMBER 040S0110503 **DATE TESTED** 17-มี.ค.-69

Remarks :

This is to certify that the above tests have been perfomed and the configuration tested

- [x] meets
- [ ] does not meet

This certificate does not modify PerkinElmer's standard terms and condition of sale, including warranty terms.

Service Department TH ONE SOURCE CO., LTD.

Krungchai T.

(**Krungchai Treevichien**)

Customer Support Engineer

TH ONE SOURCE Co.,Ltd. 33/119, T.Ladsawai, A.Lam Luk Ka, Pathum Thani 12150, Thailand

MAINTENANCE REPORT

OPTIMA 8000

Customer :	บริษัท เทคนิกสิ่งแวดล้อมไทย จำกัด	Date Tested:	March 17, 2026
		Recommendation Recertification Period	6 Months
Address :	1/6 ซอยรามคำแหง 145, แขวงสะพานสูง, เขตสะพานสูง, กรุงเทพฯ 10240 TH	Recertification Due:	September 17, 2026
		Date Last Certified:	September 19, 2025
User Name:	คุณ ณัฐพงศ์ โคตะมา	Visit Number:	ONE
Phone:	02-3737799, 081-1303495	TH ONE SOURCE Phone:	081-7316733
E-mail:	Ketsarin.Chuayphan@eurofinsasia.com Phorntip.phethshee@eurofinsasia.com	E-mail :	thonesource@gmail.com

CONFIGURATION TESTED		ACCESSORIES/COMPONENT NOT INCLUDED
MODEL	SERIAL NUMBER	
OPTIMA 8000	078S1310024C	WinLab32 Version 5.5.0
N0772045	1F1380368	PN:6150T21E4Q1E
TESTED EQUIPMENT		
IPV Methods		
TEST STANDARD USED	PE NUMBER	
Mixed standard 1/10	N0691579	
Mixed standard 1/100	N9300221	
CUSTOMER SUPPLIED	COMMENTS	
2 % HNO3		
10 % HNO3		

MAINTENANCE REPORT

OPTIMA 8000

SERIAL NUMBER 078S1310024C **DATE TESTED** March 17, 2026

1. MECHANICAL CHECKS

A. Inspect and clean all fans and filters.	OK
B. Inspect and replace as necessary, all torch components including the RF Flat coil	OK
C. Inspect all tubing for sign of clacking or leaking.	OK
D. Adjust water and gas pressure regulator settings.	OK
E. Inspect and leak check pneumatics drawers.	OK
F. Clean the exterior of the instrument.	OK

2. OPTICAL CHECKS

A. Inspect and clean all optical components.	OK
B. As reqiured, check and replace all purge filters.	OK
C. Recheck optical alignment.	OK

3. COOLING SYSTEM CHECKS

A. Perform preventive maintenance on chiller.	OK
B. Flush out water the chiller and replace with coolant mix30plus every twelve months	OK

4. PERFORMANCE CHECKS

A. Torch View Alignment.	OK
B. Wavelength Calibration.	OK

TH One Source Co.,Ltd. 33/119 Moo 10, Ladsawai, Lam Luk Ka, Pathum Thani 12150, Thailand

MAINTENANCE REPORT

OPTIMA 8000

SERIAL NUMBER 078S1310024C	DATE TESTED	March 17, 2026
PARAMETER	**SPECIFICATION**	**FINAL VAULE**
Precision		
Zn 213.856	% RSD ≤ 1.0	0.79
Mg 280.260	% RSD ≤ 1.0	0.68
Mg 285.207	% RSD ≤ 1.0	0.38
Ba 455.403	% RSD ≤ 1.0	0.43
Detection Limits: Axial		
	As 193 nm, 3(sd) ≤ 10.0 ppb	0.81
	Se 196 nm, 3(sd) ≤ 5.0 ppb	5.0
	Tl 190 nm, 3(sd) ≤ 10.0 ppb	0.48
	Pb 220 nm, 3(sd) ≤ 3.0 ppb	0.40
BEC: Axial	Mn 257 nm, ≤ 30 ppb	2.61
Detection Limits: Radial		
	As 193 nm, 3(sd) ≤ 60.0 ppb	4.95
	Zn 213 nm, 3(sd) ≤ 2.0 ppb	0.12
	Mn 257 nm, 3(sd) ≤ 1.0 ppb	0.03
	La 379 nm, 3(sd) ≤ 3.0 ppb	0.27
	Ba 455 nm, 3(sd) ≤ 0.3 ppb	0.02
	Ba 493 nm, 3(sd) ≤ 0.6 ppb	0.02
BEC: Radial	Mn 257 nm, ≤ 30 ppb	7.13
Spectral Resolution: UV		
	As 193 nm, ≤ 0.009	0.00759
	Ni 231 nm, ≤ 0.011	0.00841
	Ni 341 nm, ≤ 0.015	0.01266
Spectral Resolution: VIS		
	Ba 455 nm, ≤ 0.020	0.01585

TH One Source Co.,Ltd. 33/119 Moo 10, Ladsawai, Lam Luk Ka, Pathum Thani 12150, Thailand

MAINTENANCE REPORT

OPTIMA 8000

SERIAL NUMBER 078S1310024C **DATE TESTED** March 17, 2026

Remarks :

Commissioning follow as commissioning performance sheets.

Calculate MnBEC = IB * STD Conc / IS-IB , where standard conc = 1000 ug/L

IB = Intensity of blank

IS = Intensity of Standard

Used Mira Mist Nebulizer

This is to certify that the above tests have been perfomed and the configuration tested

[✔] meets

[ ] does not meet

This certificate does not modify PerkinElmer's standard terms and condition of sale, including warranty terms.

Service Department TH One Source Co., Ltd.

Krungchai T.

(**Krungchai Treevichien**)

Customer Support Engineer

TH One Source Co.,Ltd. 33/119 Moo 10, Ladsawai, Lam Luk Ka, Pathum Thani 12150, Thailand

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Certificate of Calibration

Cert. No.: 26TM418

Equipment :	Incubator
Manufacturer :	Memmert
Model :	INE 500
Serial No. :	E505.0595
ID No. :	Ins-LAB-041
Submitted by :	Thai Environmental Technic Limited 1/6 Soi Ramkhamhaeng 145, Khwaeng/Khet Saphan Sung, Bangkok 10240
Location :	Bacteria Room
Received Order :	09 March 2026
Calibration Date :	10 - 11 March 2026
Ambient Temperature :	(26 ± 10) °C
Relative Humidity :	(50 ± 30) %
AC Line Voltage :	(220 ± 22) V

Calibrated by : Preecha Hlahib

Approved by : Kunchit

Approved Signatory

( ) Chakrit Waewwanjua
( ) Suwit Imjai
(✓) Kunchit Promprat

Issue Date : 24 March 2026

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Equipment : Incubator
Condition As-Received : Used Item
Reference : 2603-0127OC-2

Cert. No.: 26TM418

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-


Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY49023932	25LM121	TPA	27 Jul 2026

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This measurement result is traceable to the International System of Unit maintained through :

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Environment during calibration		
	Beginning	**Finished**
Temp. (°C)	24	20
REL.Humid. (%)	34	40
AC Supply (Volt)	221	221

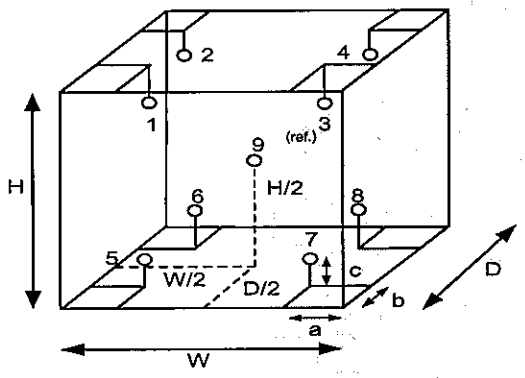

Position :	Ref. Std. ID No.:
1	20-16RTD-01
2	20-16RTD-02
3	20-16RTD-03
4	20-16RTD-04
5	22-16RTD-05
6	20-16RTD-06
7	20-16RTD-07
8	22-16RTD-08
9 (ref.)	22-16RTD-09

Probe Installation Details :

a = 5.0 cm
b = 5.0 cm
c = 5.0 cm

Dimension of Chamber :

D = 0.40 m
W = 0.56 m
H = 0.48 m
Capacity = 0.11 m^3

Equipment : Incubator
Condition As-Received : Used Item
Reference : 2603-0127OC-2
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor *k*
35.0	35.0	35.0	0.031	0.27	0.43	2
41.5	41.5	41.5	0.033	0.68	0.96	2
44.5	44.5	44.5	0.031	0.48	0.73	2

Calibration Point (°C)	Measured Temperature (°C) Position									Uncertainty (±°C)
	1	2	3	4	5	6	7	8	9 (ref.)	
35.0	35.149	35.101	35.194	35.177	34.802	35.192	34.935	34.958	35.066	0.30
41.5	41.831	41.732	41.918	41.951	41.009	41.340	41.027	41.389	41.651	0.30
44.5	44.674	44.571	44.704	44.661	44.022	44.250	44.052	44.243	44.462	0.30

Average* : The average of 30 values in each position.
Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.
Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.
Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.
UUC* : Unit Under Calibration
Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor ***k***, providing a level of confidence of approximately 95 %.

-o0o-

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Certificate of Calibration

Cert. No.: 26TM419
Page : 1 of 3

Equipment :	Incubator
Manufacturer :	Memmert
Model :	INE 500
Serial No. :	E505.1143
ID No. :	Ins-LAB-042
Submitted by :	Thai Environmental Technic Limited 1/6 Soi Ramkhamhaeng 145, Khwaeng/Khet Saphan Sung, Bangkok 10240
Location :	Bacteria Room
Received Order :	09 March 2026
Calibration Date :	09 - 10 March 2026
Ambient Temperature :	(26 ± 10) °C
Relative Humidity :	(50 ± 30) %
AC Line Voltage :	(220 ± 22) V

Calibrated by : Preecha Hlahib

Approved by : Kunchit

Approved Signatory

( ) Chakrit Waewwanjua
( ) Suwit Imjai
(✓) Kunchit Promprat

Issue Date : 24 March 2026

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Equipment : Incubator
Condition As-Received : Used Item
Reference : 2603-0127OC-3

Cert. No.: 26TM419

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-


Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY49023932	25LM121	TPA	27 Jul 2026

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This measurement result is traceable to the International System of Unit maintained through :

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Environment during calibration		
	Beginning	Finished
Temp. (°C)	35	23
REL.Humid. (%)	35	37
AC Supply (Volt)	220	221

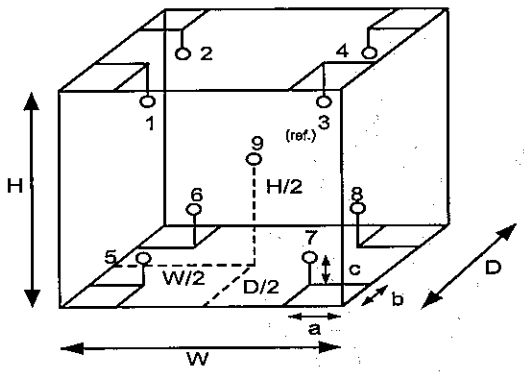

Position :	Ref. Std. ID No.:
1	20-16RTD-01
2	20-16RTD-02
3	20-16RTD-03
4	20-16RTD-04
5	22-16RTD-05
6	20-16RTD-06
7	20-16RTD-07
8	22-16RTD-08
9 (ref.)	22-16RTD-09

Probe Installation Details :

a =	5.0	cm
b =	5.0	cm
c =	5.0	cm

Dimension of Chamber :

D =	0.40	m
W =	0.56	m
H =	0.48	m
Capacity =	0.11	m^3

Equipment : Incubator
Condition As-Received : Used Item
Reference : 2603-0127OC-3
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor *k*
35.0	35.0	35.0	0.039	0.42	0.69	2
41.5	41.0	41.0	0.034	0.56	0.76	2
44.5	44.0	44.0	0.095	0.37	0.72	2

Calibration Point (°C)	Measured Temperature (°C) Position									Uncertainty (±°C)
	1	2	3	4	5	6	7	8	9 (ref.)	
35.0	35.145	35.137	35.363	35.378	34.954	35.575	34.991	35.522	35.178	0.30
41.5	41.354	41.244	41.367	41.355	41.459	41.941	41.375	41.759	41.401	0.30
44.5	44.543	44.333	44.669	44.726	44.281	44.813	44.164	44.771	44.507	0.30

Average* : The average of 30 values in each position.
Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.
Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.
Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.
UUC* : Unit Under Calibration
Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor ***k***, providing a level of confidence of approximately 95 %.

-o0o-

ภาคผนวก ฉ

หนังสือขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
เลขทะเบียน ว-236



ที่ อก ๐๓๑๐(๑)/ ๓๐๗๔

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๐๑ พฤษภาคม ๒๕๖๙

เรื่อง ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

เรียน กรรมการผู้จัดการ บริษัท เทคนิคสิ่งแวดล้อมไทย จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน ลงวันที่ ๑๗ กุมภาพันธ์ ๒๕๖๙

สิ่งที่ส่งมาด้วย ๑. รายชื่อผู้ควบคุมห้องปฏิบัติการวิเคราะห์เอกชน จำนวน ๘ ราย
๒. เจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน จำนวน ๓๗ ราย
๓. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม

ตามคำขอที่อ้างถึง บริษัท เทคนิคสิ่งแวดล้อมไทย จำกัด ขอต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๒๓๖ สถานที่ตั้งเลขที่ ๑/๖ ซอยรามคำแหง ๑๔๕ แขวงสะพานสูง เขตสะพานสูง กรุงเทพมหานคร ต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้บริษัท เทคนิคสิ่งแวดล้อมไทย จำกัด ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน โดยมีองค์ประกอบดังนี้

ก. ผู้ควบคุมห้องปฏิบัติการวิเคราะห์เอกชน จำนวน ๘ ราย ตามสิ่งที่ส่งมาด้วย ๑
ข. เจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน จำนวน ๓๗ ราย ตามสิ่งที่ส่งมาด้วย ๒
ค. ขอบข่ายชนิดสารมลพิษที่ได้รับขึ้นทะเบียนให้วิเคราะห์ในน้ำ/น้ำเสีย น้ำใต้ดิน อากาศเสีย สิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว และดิน ตามสิ่งที่ส่งมาด้วย ๓

หนังสือฉบับนี้จะสิ้นอายุในวันที่ ๑๓ มีนาคม ๒๕๗๓ หากประสงค์จะต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ให้ยื่นคำขอต่ออายุพร้อมเอกสารประกอบคำขอต่อกรมโรงงานอุตสาหกรรม ภายใน ๖๐ วัน ก่อนวันสิ้นอายุของหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายศิระ จันทร์เฉิด)
นักวิทยาศาสตร์เชี่ยวชาญ รักษาราชการแทน
ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน
กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ
โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕
โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๙๙
ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th

สิ่งที่ส่งมาด้วย ๑

เอกสารแนบท้ายหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท เทคนิคสิ่งแวดล้อมไทย จำกัด **เลขทะเบียน ว-๒๓๖**
ที่ อก ๐๓๑๐(๑)/ ๓๐๗๔ **ลงวันที่** ๐๑ พฤษภาคม ๒๕๖๙

ก. ผู้ควบคุมห้องปฏิบัติการวิเคราะห์เอกชน จำนวน ๘ ราย

๑) นายณัฐพงศ์ โคตะมา	ทะเบียนเลขที่ ว-๒๓๖-ค-๐๐๐๑
๒) นางสาววารีรัตน์ ประชุมแดง	ทะเบียนเลขที่ ว-๒๓๖-ค-๐๐๐๒
๓) นางพรทิพย์ เพชรชี	ทะเบียนเลขที่ ว-๒๓๖-ค-๐๐๐๓
๔) นายสมชาย ปิยะวรสกุล	ทะเบียนเลขที่ ว-๒๓๖-ค-๐๐๐๔
๕) นายประมวล มูลสาร	ทะเบียนเลขที่ ว-๒๓๖-ค-๐๐๐๕
๖) นายรัฐพล สุขดี	ทะเบียนเลขที่ ว-๒๓๖-ค-๐๐๐๖
๗) นางสาวมาลินี มณีรัตน์	ทะเบียนเลขที่ ว-๒๓๖-ค-๐๐๐๗
๘) นางสาวดอกรัก สีแหล้	ทะเบียนเลขที่ ว-๒๓๖-ค-๐๐๐๘

เอกสารแนบท้ายหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท เทคนิคสิ่งแวดล้อมไทย จำกัด **เลขทะเบียน ว-๒๓๖**
ที่ อก ๐๓๑๐(๑)/ ๓๐๗๔ **ลงวันที่** ๐๑ พฤษภาคม ๒๕๖๙

ข. เจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน จำนวน ๓๗ ราย

๑) นางสาวกมลลักษณ์ ดีมงคล	ทะเบียนเลขที่ ว-๒๓๖-จ-๐๐๐๒
๒) นางสาวกนกวรรณ เริ่มประชาธิปไตย	ทะเบียนเลขที่ ว-๒๓๖-จ-๐๐๐๓
๓) นางสาวฐิติพรรณ ศรีสุวรรณ์	ทะเบียนเลขที่ ว-๒๓๖-จ-๐๐๐๔
๔) นางสาวธนิดา กมุทชาติ	ทะเบียนเลขที่ ว-๒๓๖-จ-๐๐๐๕
๕) นางสาวพัชราพรรณ สว่างภพ	ทะเบียนเลขที่ ว-๒๓๖-จ-๐๐๐๗
๖) นายสุริยะพงศ์ ยงยุทธ	ทะเบียนเลขที่ ว-๒๓๖-จ-๐๐๐๘
๗) นางสาวศิริพร กาจุ๊ด	ทะเบียนเลขที่ ว-๒๓๖-จ-๐๐๑๐
๘) นายสุชาติ ศรีบุญ	ทะเบียนเลขที่ ว-๒๓๖-จ-๐๐๑๑
๙) นายเกียรติศักดิ์ วันดี	ทะเบียนเลขที่ ว-๒๓๖-จ-๐๐๑๒
๑๐) นายจิรวัฒน์ อินทะเสย์	ทะเบียนเลขที่ ว-๒๓๖-จ-๐๐๑๓
๑๑) นางสาวนิตยา เย็นวัฒนา	ทะเบียนเลขที่ ว-๒๓๖-จ-๐๐๑๔
๑๒) นางสาวณัฐธญาน์ ปรังการ	ทะเบียนเลขที่ ว-๒๓๖-จ-๐๐๑๕
๑๓) นายกิตติศักดิ์ เมืองงาม	ทะเบียนเลขที่ ว-๒๓๖-จ-๐๐๑๖
๑๔) นายเฉลิมวุฒิ พูลสงวน	ทะเบียนเลขที่ ว-๒๓๖-จ-๐๐๑๘
๑๕) นางสาววรรณศิริ สุริยวงศ์	ทะเบียนเลขที่ ว-๒๓๖-จ-๐๐๒๐
๑๖) นายวิทูน วลัยรัตน์	ทะเบียนเลขที่ ว-๒๓๖-จ-๐๐๒๑
๑๗) นางสาวกังสดาล จอกสูงเนิน	ทะเบียนเลขที่ ว-๒๓๖-จ-๐๐๒๒
๑๘) นางสาวสุภัคชญา อยู่นิ่ม	ทะเบียนเลขที่ ว-๒๓๖-จ-๐๐๒๓
๑๙) นายเจอ แซ่หว้า	ทะเบียนเลขที่ ว-๒๓๖-จ-๐๐๒๕
๒๐) นายอรรถพล วงศ์สวัสดิ์	ทะเบียนเลขที่ ว-๒๓๖-จ-๐๐๒๖
๒๑) นายประหยัด จิวเดช	ทะเบียนเลขที่ ว-๒๓๖-จ-๐๐๒๗
๒๒) นายเบญจพล กรีคงคา	ทะเบียนเลขที่ ว-๒๓๖-จ-๐๐๒๘
๒๓) นายวีรพล บุดสา	ทะเบียนเลขที่ ว-๒๓๖-จ-๐๐๒๙
๒๔) นายพิเชฐ อยู่ดีรัมย์	ทะเบียนเลขที่ ว-๒๓๖-จ-๐๐๓๐
๒๕) นายณัฐดนัย ศรีรัตน์ชัชวาลย์	ทะเบียนเลขที่ ว-๒๓๖-จ-๐๐๓๑
๒๖) นายฐิติศักดิ์ คงแก้ว	ทะเบียนเลขที่ ว-๒๓๖-จ-๐๐๓๒
๒๗) นายอดิศร จินดามณี	ทะเบียนเลขที่ ว-๒๓๖-จ-๐๐๓๓
๒๘) นายรัฐศาสตร์ เศรษฐกร	ทะเบียนเลขที่ ว-๒๓๖-จ-๐๐๓๔
๒๙) นายธนบัติ มะลัย	ทะเบียนเลขที่ ว-๒๓๖-จ-๐๐๓๕
๓๐) นายสิทธิพงศ์ ใจแก้ว	ทะเบียนเลขที่ ว-๒๓๖-จ-๐๐๓๖
๓๑) นายจตุรพร กังวานไพเราะ	ทะเบียนเลขที่ ว-๒๓๖-จ-๐๐๓๗
๓๒) นางสาวขวัญจิรา ทับอุไร	ทะเบียนเลขที่ ว-๒๓๖-จ-๐๐๓๘

๓๓) นางสาวจีรทัศนีย์...

๓๓) นางสาวจีรทัศนีย์ บุญเกตุ	ทะเบียนเลขที่ ว-๒๓๖-จ-๐๐๓๙
๓๔) นางสาวสุรัชชา สุภิรักษ์	ทะเบียนเลขที่ ว-๒๓๖-จ-๐๐๔๐
๓๕) นายสุรภัฏ มะลิงาม	ทะเบียนเลขที่ ว-๒๓๖-จ-๐๐๔๑
๓๖) นายอนันทชัย เสียมไหม	ทะเบียนเลขที่ ว-๒๓๖-จ-๐๐๔๒
๓๙) นายปัฐวีย์ อินทร์ลี	ทะเบียนเลขที่ ว-๒๓๖-จ-๐๐๔๓

เอกสารแนบท้ายหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท เทคนิคสิ่งแวดล้อมไทย จำกัด เลขทะเบียน ว-๒๓๖
ที่ อก ๐๓๑๐(๑)/ ลงวันที่ ๐๑ พฤษภาคม ๒๕๖๙

ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๓๔๖ รายการ

น้ำ/น้ำเสีย จำนวน 40 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Aldrin	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
2	Arsenic	Digestion, Hydride Generation/Atomic Absorption Spectrometric Method[4]
3	Barium	1) Digestion, Electrothermal Atomic Absorption Spectrometric Method[4] 2) Digestion, Flame Atomic Absorption Spectrometric Method[4] 3) Digestion, Inductively Coupled Plasma Method[4]
4	α-BHC	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
5	γ-BHC	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
6	Biochemical Oxygen Demand	5-Day BOD Test, Azide Modification Method[4]
7	Cadmium	1) Digestion, Electrothermal Atomic Absorption Spectrometric Method[4] 2) Digestion, Flame Atomic Absorption Spectrometric Method[4] 3) Digestion, Inductively Coupled Plasma Method[4]
8	Chemical Oxygen Demand	Closed Reflux, Titrimetric Method[4]
9	Chlordane	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
10	Chromium	1) Digestion, Electrothermal Atomic Absorption Spectrometric Method[4] 2) Digestion, Flame Atomic Absorption Spectrometric Method[4] 3) Digestion, Inductively Coupled Plasma Method[4]
11	Color	ADMI Weighted-Ordinate Spectrophotometric Method[4]
12	Copper	1) Digestion, Electrothermal Atomic Absorption Spectrometric Method[4] 2) Digestion, Flame Atomic Absorption Spectrometric Method[4] 3) Digestion, Inductively Coupled Plasma Method[4]

13 Cyanide...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
13	Cyanide	Total Cyanide after Distillation, Colorimetric Method[4]
14	4,4'-DDE	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
15	4,4'-DDT	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
16	Dieldrin	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
17	Endosulfan I	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
18	Endosulfan II	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
19	Endosulfan Sulfate	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
20	Endrin	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
21	Formaldehyde	Distillation, Colorimetric Method[3]
22	Free Chlorine	DPD Ferrous Titrimetric Method[4]
23	Heptachlor	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
24	Heptachlor Epoxide	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
25	Hexavalent Chromium	Colorimetric Method[4]
26	Lead	1) Digestion, Electrothermal Atomic Absorption Spectrometric Method[4] 2) Digestion, Flame Atomic Absorption Spectrometric Method[4] 3) Digestion, Inductively Coupled Plasma Method[4]
27	Manganese	1) Digestion, Electrothermal Atomic Absorption Spectrometric Method[4] 2) Digestion, Flame Atomic Absorption Spectrometric Method[4] 3) Digestion, Inductively Coupled Plasma Method[4]
28	Mercury	Digestion, Cold-Vapor Atomic Absorption Spectrometric Method[4]
29	Nickel	1) Digestion, Electrothermal Atomic Absorption Spectrometric Method[4] 2) Digestion, Flame Atomic Absorption Spectrometric Method[4] 3) Digestion, Inductively Coupled Plasma Method[4]
30	Oil & Grease	1) Liquid-Liquid, Partition-Gravimetric Method[4] 2) Soxhlet Extraction Method[4]
31	pH	Electrometric Method[4]
32	Phenols	Distillation, Direct Photometric Method[4]
33	Selenium	Digestion, Hydride Generation/Atomic Absorption Spectrometric Method[4]

34 Sulfide...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
34	Sulfide	1) Iodometric Method[4] 2) Methylene Blue Method[4]
35	Temperature	Laboratory and Field Methods[4]
36	Total Dissolved Solids	Dried at 180 °C[4]
37	Total Kjeldahl Nitrogen	Macro-Kjeldahl Method[4]
38	Total Suspended Solids	Dried from 103 to 105 °C[4]
39	Trivalent Chromium	Calculation[4]
40	Zinc	1) Digestion, Electrothermal Atomic Absorption Spectrometric Method[4] 2) Digestion, Inductively Coupled Plasma Method[4]

น้ำใต้ดิน จำนวน 126 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Acenaphthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
2	Acetone	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method[4]
3	Aldrin	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
4	Aluminum	Digestion, Inductively Coupled Plasma Method[4]
5	Anthracene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
6	Antimony	1) Digestion, Electrothermal Atomic Absorption Spectrometric Method[4] 2) Digestion, Inductively Coupled Plasma Method[4]
7	Arsenic	Digestion, Hydride Generation/Atomic Absorption Spectrometric Method[4]
8	Atrazine	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
9	Barium	1) Digestion, Electrothermal Atomic Absorption Spectrometric Method[4] 2) Digestion, Flame Atomic Absorption Spectrometric Method[4] 3) Digestion, Inductively Coupled Plasma Method[4]
10	Benz(a)anthracene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
11	Benzene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method[4]

12 Benzo(b)fluoranthene...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
12	Benzo(b)fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
13	Benzo(k)fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
14	Benzoic acid	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
15	Benzo(a)pyrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
16	Benzo(g,h,i)perylene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
17	Beryllium	1) Digestion, Electrothermal Atomic Absorption Spectrometric Method[4] 2) Digestion, Inductively Coupled Plasma Method[4]
18	Bis(2-chloroethyl)ether	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
19	Bis(2-ethylhexyl)phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
20	Bromodichloromethane	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method[4]
21	Bromoform	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method[4]
22	Butanol	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method[4]
23	Butyl benzyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
24	Cadmium	1) Digestion, Electrothermal Atomic Absorption Spectrometric Method[4] 2) Digestion, Inductively Coupled Plasma Method[4]
25	Carbazole	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
26	Carbon disulfide	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method[4]
27	Carbon tetrachloride	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method[4]
28	Chlordane	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
29	p-Chloroaniline	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
30	Chlorobenzene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method[4]

31 Chlorodibromomethane...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
31	Chlorodibromomethane	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method[4]
32	Chloroform	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method[4]
33	Chromium	1) Digestion, Electrothermal Atomic Absorption Spectrometric Method[4] 2) Digestion, Flame Atomic Absorption Spectrometric Method[4] 3) Digestion, Inductively Coupled Plasma Method[4]
34	Chromium (III)	Calculation[4]
35	Chromium (VI)	Colorimetric Method[4]
36	Chrysene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
37	Copper	1) Digestion, Electrothermal Atomic Absorption Spectrometric Method[4] 2) Digestion, Flame Atomic Absorption Spectrometric Method[4] 3) Digestion, Inductively Coupled Plasma Method[4]
38	Cyanide	Total Cyanide after Distillation, Colorimetric Method[4]
39	2,4-D	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
40	DDD	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
41	DDE	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
42	DDT	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
43	Dibenz(a,h)anthracene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
44	Di-n-butyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
45	1,2-Dichlorobenzene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method[4]
46	1,3-Dichlorobenzene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method[4]
47	1,4-Dichlorobenzene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method[4]
48	1,1-Dichloroethane	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method[4]
49	1,2-Dichloroethane	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method[4]

50 1,1-Dichloroethylene...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
50	1,1-Dichloroethylene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method[4]
51	cis-1,2-Dichloroethylene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method[4]
52	trans-1,2-Dichloroethylene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method[4]
53	1,2-Dichloropropane	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method[4]
54	1,3-Dichloropropane	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method[4]
55	1,3-Dichloropropene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method[4]
56	Dieldrin	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
57	Diethyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
58	2,4-Dimethylphenol	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
59	2,4-Dinitrophenol	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
60	2,4-Dinitrotoluene	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
61	2,6-Dinitrotoluene	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
62	Di-n-Octyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
63	Endosulfan	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
64	Endrin	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
65	Ethylbenzene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method[4]
66	Fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
67	Fluorene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
68	Heptachlor	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
69	Heptachlor epoxide	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
70	Hexachloro-1,3-butadiene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method[4]
71	n-Hexane	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method[4]
72	α-HCH	Liquid-Liquid Extraction, Gas Chromatographic Method[4]

73 β-HCH...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
73	β-HCH	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
74	γ-HCH	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
75	Hexachlorocyclopentadiene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
76	Hexachloroethane	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
77	Indeno(1,2,3-cd)pyrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
78	Iron	1) Digestion, Flame Atomic Absorption Spectrometric Method[4] 2) Digestion, Inductively Coupled Plasma Method[4]
79	Isophorone	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
80	Lead	1) Digestion, Electrothermal Atomic Absorption Spectrometric Method[4] 2) Digestion, Inductively Coupled Plasma Method[4]
81	Manganese	1) Digestion, Electrothermal Atomic Absorption Spectrometric Method[4] 2) Digestion, Flame Atomic Absorption Spectrometric Method[4] 3) Digestion, Inductively Coupled Plasma Method[4]
82	Mercury	Digestion, Cold-Vapor Atomic Absorption Spectrometric Method[4]
83	Methanol	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method[4]
84	Methoxychlor	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
85	Methyl bromide	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method[4]
86	Methylene chloride	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method[4]
87	2-Methylphenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
88	2-Methylnaphthalene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
89	Methyl tert-butyl ether	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method[4]
90	Molybdenum	Digestion, Inductively Coupled Plasma Method[4]

91 Naphthalene ...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
91	Naphthalene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method[4]
92	Nickel	1) Digestion, Electrothermal Atomic Absorption Spectrometric Method[4] 2) Digestion, Inductively Coupled Plasma Method[4]
93	Nitrobenzene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
94	N-Nitrosodiphenylamine	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
95	N-Nitrosodi-n-propylamine	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
96	Polychlorinated Biphenyls PCB-1016 PCB-1221 PCB-1232 PCB-1242 PCB-1248 PCB-1254 PCB-1260	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
97	Pentachlorophenol	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
98	pH	Electrometric Method[4]
99	Phenanthrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
100	Phenol	1) Distillation, Direct Photometric Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic Method[4]
101	Pyrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
102	Selenium	Digestion, Hydride Generation/Atomic Absorption Spectrometric Method[4]
103	Silver	1) Digestion, Electrothermal Atomic Absorption Spectrometric Method[4] 2) Digestion, Inductively Coupled Plasma Method[4]
104	Styrene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method[4]
105	1,1,2,2-Tetrachloroethane	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method[4]
106	Tetrachloroethylene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method[4]

107 Toluene ...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
107	Toluene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method[4]
108	Toxaphene	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
109	TPH (C_5-C_8)	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,22]
110	TPH ($C_{>8}$-C_{16})	Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[9,22]
111	TPH ($C_{>16}$-C_{35})	Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[9,22]
112	1,2,4-Trichlorobenzene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method[4]
113	1,1,1-Trichloroethane	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method[4]
114	1,1,2-Trichloroethane	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method[4]
115	Trichloroethylene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method[4]
116	2,4,5-Trichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
117	2,4,6-Trichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
118	1,3,5-Trimethylbenzene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method[4]
119	Vanadium	1) Digestion, Electrothermal Atomic Absorption Spectrometric Method[4] 2) Digestion, Inductively Coupled Plasma Method[4]
120	Vinyl acetate	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method[4]
121	Vinyl chloride	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method[4]
122	m-Xylene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method[4]
123	o-Xylene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method[4]
124	p-Xylene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method[4]
125	Xylene (Total)	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method[4]
126	Zinc	1) Digestion, Flame Atomic Absorption Spectrometric Method[4] 2) Digestion, Inductively Coupled Plasma Method[4]

อากาศเสีย...

อากาศเสีย (ปล่องระบาย) จำนวน 18 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Antimony	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5] 2) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method[5] 3) Isokinetic Sampling, Digestion, Graphite Furnace Atomic Absorption Spectrometric Method[5]
2	Arsenic	Isokinetic Sampling, Digestion, Hydride Generation/ Atomic Absorption Spectrometric Method[5]
3	Carbon monoxide	Instrumental Analyzer Method[5]
4	Chlorine	Absorption Sampling, Ion Chromatographic Method[5]
5	Copper	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5] 2) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method[5]
6	Cresol	Adsorption Sampling, Gas Chromatographic Method[5]
7	Dioxins/Furans	Isokinetic Sampling, Analysis by ISO/IEC 17025 Accredited Laboratory or Analysis by Department of Industrial Works Registered Laboratory (Dioxins/Furans Analysis Approved)[5]
8	Hydrogen Chloride	Absorption Sampling, Ion Chromatographic Method[5]
9	Hydrogen Fluoride	Absorption Sampling, Ion Chromatographic Method[5]
10	Hydrogen Sulfide	Absorption Sampling, Iodometric Method[5]
11	Lead	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5] 2) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method[5] 3) Isokinetic Sampling, Digestion, Graphite Furnace Atomic Absorption Spectrometric Method[5]
12	Mercury	Isokinetic Sampling, Digestion, Cold-Vapor Atomic Absorption Spectrometric Method[5]
13	Opacity	Ringelmann's Method[2]
14	Oxides of Nitrogen	1) Absorption Sampling, Phenoldisulfonic acid Method[5] 2) Instrumental Analyzer Method[5]
15	Sulfur dioxide	1) Absorption Sampling, Barium-Thorin Titrimetric Method[5] 2) Instrumental Analyzer Method[5]

16 Sulfuric acid...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
16	Sulfuric acid	Isokinetic Sampling, Barium-Thorin Titrimetric Method[5]
17	Total Suspended Particulate	Isokinetic Sampling, Gravimetric Method[5]
18	Xylene	Adsorption Sampling, Gas Chromatographic Method[5]

<u>สิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว จำนวน 37 รายการ</u>

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Aldrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[1,9,23] 2) Soxhlet Extraction, Gas Chromatographic Method[10,23]
2	Antimony	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method[1,6,14] 2) Waste Extraction, Digestion, Graphite Furnace Atomic Absorption Spectrometric Method[1,6,15] 3) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,13] 4) Digestion, Flame Atomic Absorption Spectrometric Method[7,14] 5) Digestion, Graphite Furnace Atomic Absorption Spectrometric Method[7,15] 6) Digestion, Inductively Coupled Plasma Method[7,13]
3	Arsenic	1) Waste Extraction, Digestion, Hydride Generation/ Atomic Absorption Spectrometric Method[1,6,16] 2) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method[7,16]
4	Barium	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method[1,6,14] 2) Waste Extraction, Digestion, Graphite Furnace Atomic Absorption Spectrometric Method[1,6,15] 3) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,13] 4) Digestion, Flame Atomic Absorption Spectrometric Method[7,14] 5) Digestion, Graphite Furnace Atomic Absorption Spectrometric Method[7,15] 6) Digestion, Inductively Coupled Plasma Method[7,13]

5 Beryllium...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
5	Beryllium	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method[1,6,14] 2) Waste Extraction, Digestion, Graphite Furnace Atomic Absorption Spectrometric Method[1,6,15] 3) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,13] 4) Digestion, Flame Atomic Absorption Spectrometric Method[7,14] 5) Digestion, Graphite Furnace Atomic Absorption Spectrometric Method[7,15] 6) Digestion, Inductively Coupled Plasma Method[7,13]
6	Cadmium	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method[1,6,14] 2) Waste Extraction, Digestion, Graphite Furnace Atomic Absorption Spectrometric Method[1,6,15] 3) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,13] 4) Digestion, Flame Atomic Absorption Spectrometric Method[7,14] 5) Digestion, Graphite Furnace Atomic Absorption Spectrometric Method[7,15] 6) Digestion, Inductively Coupled Plasma Method[7,13]
7	Chlordane	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[1,9,23] 2) Soxhlet Extraction, Gas Chromatographic Method[10,23]
8	Chromium	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method[1,6,14] 2) Waste Extraction, Digestion, Graphite Furnace Atomic Absorption Spectrometric Method[1,6,15] 3) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,13] 4) Digestion, Flame Atomic Absorption Spectrometric Method[7,14] 5) Digestion, Graphite Furnace Atomic Absorption Spectrometric Method[7,15] 6) Digestion, Inductively Coupled Plasma Method[7,13]

9 Chromium (III)...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
9	Chromium (III)	Calculation[1,6,7,8,13,14,15,17]
10	Chromium (VI)	1) Waste Extraction, Colorimetric Method[1,17] 2) Alkaline Digestion, Colorimetric Method[8,17]
11	Cobalt	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method[1,6,14] 2) Waste Extraction, Digestion, Graphite Furnace Atomic Absorption Spectrometric Method[1,6,15] 3) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,13] 4) Digestion, Flame Atomic Absorption Spectrometric Method[7,14] 5) Digestion, Graphite Furnace Atomic Absorption Spectrometric Method[7,15] 6) Digestion, Inductively Coupled Plasma Method[7,13]
12	Copper	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method[1,6,14] 2) Waste Extraction, Digestion, Graphite Furnace Atomic Absorption Spectrometric Method[1,6,15] 3) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,13] 4) Digestion, Flame Atomic Absorption Spectrometric Method[7,14] 5) Digestion, Graphite Furnace Atomic Absorption Spectrometric Method[7,15] 6) Digestion, Inductively Coupled Plasma Method[7,13]
13	2,4-D	Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[1,9,26]
14	DDD	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[1,9,23] 2) Soxhlet Extraction, Gas Chromatographic Method[10,23]
15	DDE	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[1,9,23] 2) Soxhlet Extraction, Gas Chromatographic Method[10,23]

คุมปี

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
16	DDT	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[1,9,23] 2) Soxhlet Extraction, Gas Chromatographic Method[10,23]
17	Dieldrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[1,9,23] 2) Soxhlet Extraction, Gas Chromatographic Method[10,23]
18	Endrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[1,9,23] 2) Soxhlet Extraction, Gas Chromatographic Method[10,23]
19	Fluoride	Waste Extraction, Ion-Selective Electrode Method[33]
20	Heptachlor	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[1,9,23] 2) Soxhlet Extraction, Gas Chromatographic Method[10,23]
21	Lead	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method[1,6,14] 2) Waste Extraction, Digestion, Graphite Furnace Atomic Absorption Spectrometric Method[1,6,15] 3) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,13] 4) Digestion, Flame Atomic Absorption Spectrometric Method[7,14] 5) Digestion, Graphite Furnace Atomic Absorption Spectrometric Method[7,15] 6) Digestion, Inductively Coupled Plasma Method[7,13]
22	Lindane	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[1,9,23] 2) Soxhlet Extraction, Gas Chromatographic Method[10,23]
23	Mercury	1) Waste Extraction, Digestion, Cold-Vapor Atomic Absorption Spectrometric Method[1,6,18] 2) Digestion, Cold-Vapor Atomic Absorption Spectrometric Method[19]

24 Methoxychlor...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
24	Methoxychlor	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[1,9,23] 2) Soxhlet Extraction, Gas Chromatographic Method[10,23]
25	Mirex	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[1,9,23] 2) Soxhlet Extraction, Gas Chromatographic Method[10,23]
26	Molybdenum	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method[1,6,14] 2) Waste Extraction, Digestion, Graphite Furnace Atomic Absorption Spectrometric Method[1,6,15] 3) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,13] 4) Digestion, Flame Atomic Absorption Spectrometric Method[7,14] 5) Digestion, Graphite Furnace Atomic Absorption Spectrometric Method[7,15] 6) Digestion, Inductively Coupled Plasma Method[7,13]
27	Nickel	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method[1,6,14] 2) Waste Extraction, Digestion, Graphite Furnace Atomic Absorption Spectrometric Method[1,6,15] 3) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,13] 4) Digestion, Flame Atomic Absorption Spectrometric Method[7,14] 5) Digestion, Graphite Furnace Atomic Absorption Spectrometric Method[7,15] 6) Digestion, Inductively Coupled Plasma Method[7,13]
28	Polychlorinated Biphenyls Aroclor 1016 Aroclor 1221 Aroclor 1232 Aroclor 1242 Aroclor 1248 Aroclor 1254 Aroclor 1260	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[1,9,24] 2) Soxhlet Extraction, Gas Chromatographic Method[10,24]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
	2,4,4'-Trichlorobiphenyl 2,2',5,5'-Tetrachlorobiphenyl 2,2',4,5,5'-Pentachlorobiphenyl 2,2',3,4,4',5'-Hexachlorobiphenyl 2,2',4,4',5,5'-Hexachlorobiphenyl 2,2',3,4,4',5,5'-Heptachlorobiphenyl	
29	Pentachlorophenol	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[1,9,22] 2) Soxhlet Extraction, Gas Chromatographic Method[10,22]
30	Selenium	1) Waste Extraction, Digestion, Hydride Generation/ Atomic Absorption Spectrometric Method[1,6,20] 2) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method[7,20]
31	Silver	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method[1,6,14] 2) Waste Extraction, Digestion, Graphite Furnace Atomic Absorption Spectrometric Method[1,6,15] 3) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,13] 4) Digestion, Flame Atomic Absorption Spectrometric Method[7,14] 5) Digestion, Graphite Furnace Atomic Absorption Spectrometric Method[7,15] 6) Digestion, Inductively Coupled Plasma Method[7,13]
32	Thallium	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method[1,6,14] 2) Waste Extraction, Digestion, Graphite Furnace Atomic Absorption Spectrometric Method[1,6,15] 3) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,13] 4) Digestion, Flame Atomic Absorption Spectrometric Method[7,14] 5) Digestion, Graphite Furnace Atomic Absorption Spectrometric Method[7,15] 6) Digestion, Inductively Coupled Plasma Method[7,13]
	33 Toxaphene	

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
33	Toxaphene	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[1,9,23] 2) Soxhlet Extraction, Gas Chromatographic Method[10,23]
34	Trichloroethylene	1) Waste Extraction, Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[1,11,27] 2) Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,27]
35	Vanadium	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method[1,6,14] 2) Waste Extraction, Digestion, Graphite Furnace Atomic Absorption Spectrometric Method[1,6,15] 3) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,13] 4) Digestion, Flame Atomic Absorption Spectrometric Method[7,14] 5) Digestion, Graphite Furnace Atomic Absorption Spectrometric Method[7,15] 6) Digestion, Inductively Coupled Plasma Method[7,13]
36	Vinyl chloride	1) Waste Extraction, Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[1,11,27] 2) Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,27]
37	Zinc	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method[1,6,14] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,13] 3) Digestion, Flame Atomic Absorption Spectrometric Method[7,14] 4) Digestion, Inductively Coupled Plasma Method[7,13]

<u>ดิน จำนวน 125 รายการ</u>

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Acenaphthene	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,28]
2	Acetone	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,27]

3 Aldrin...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
3	Aldrin	Soxhlet Extraction, Gas Chromatographic Method[10,23]
4	Aluminum	Digestion, Inductively Coupled Plasma Method[7,13]
5	Anthracene	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,28]
6	Antimony	1) Digestion, Flame Atomic Absorption Spectrometric Method[7,14] 2) Digestion, Graphite Furnace Atomic Absorption Spectrometric Method[7,15] 3) Digestion, Inductively Coupled Plasma Method[7,13]
7	Arsenic	Digestion, Hydride Generation/Atomic Absorption Spectrometric Method[7,16]
8	Atrazine	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,28]
9	Barium	1) Digestion, Flame Atomic Absorption Spectrometric Method[7,14] 2) Digestion, Graphite Furnace Atomic Absorption Spectrometric Method[7,15] 3) Digestion, Inductively Coupled Plasma Method[7,13]
10	Benz(a)anthracene	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,28]
11	Benzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,27]
12	Benzo(b)fluoranthene	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,28]
13	Benzo(k)fluoranthene	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,28]
14	Benzoic acid	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,28]
15	Benzo(a)pyrene	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,28]
16	Benzo(g,h,i)perylene	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,28]
17	Beryllium	1) Digestion, Flame Atomic Absorption Spectrometric Method[7,14] 2) Digestion, Graphite Furnace Atomic Absorption Spectrometric Method[7,15] 3) Digestion, Inductively Coupled Plasma Method[7,13]
18	Bis(2-chloroethyl)ether	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,28]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
19	Bis(2-ethylhexyl)phthalate	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,28]
20	Bromodichloromethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,27]
21	Bromoform	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,27]
22	Butanol	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,27]
23	Butyl benzyl phthalate	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,28]
24	Cadmium	1) Digestion, Flame Atomic Absorption Spectrometric Method[7,14] 2) Digestion, Graphite Furnace Atomic Absorption Spectrometric Method[7,15] 3) Digestion, Inductively Coupled Plasma Method[7,13]
25	Carbazole	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,28]
26	Carbon disulfide	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,27]
27	Carbon tetrachloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,27]
28	Chlordane	Soxhlet Extraction, Gas Chromatographic Method[10,23]
29	p-Chloroaniline	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,28]
30	Chlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,27]
31	Chlorodibromomethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,27]
32	Chloroform	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,27]
33	Chromium	1) Digestion, Flame Atomic Absorption Spectrometric Method[7,14] 2) Digestion, Graphite Furnace Atomic Absorption Spectrometric Method[7,15] 3) Digestion, Inductively Coupled Plasma Method[7,13]
34	Chromium (III)	Calculation[7,8,13,14,15,17]
35	Chromium (VI)	Alkaline Digestion, Colorimetric Method[8,17]

36 Copper...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
36	Copper	1) Digestion, Flame Atomic Absorption Spectrometric Method[7,14] 2) Digestion, Graphite Furnace Atomic Absorption Spectrometric Method[7,15] 3) Digestion, Inductively Coupled Plasma Method[7,13]
37	Chrysene	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,28]
38	Cyanide	Extraction, Distillation, Colorimetric Method[29,30,31]
39	DDD	Soxhlet Extraction, Gas Chromatographic Method[10,23]
40	DDE	Soxhlet Extraction, Gas Chromatographic Method[10,23]
41	DDT	Soxhlet Extraction, Gas Chromatographic Method[10,23]
42	Dibenz(a,h)anthracene	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,28]
43	Di-n-butyl phthalate	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,28]
44	1,2-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,27]
45	1,3-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,27]
46	1,4-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,27]
47	1,1-Dichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,27]
48	1,2-Dichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,27]
49	1,1-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,27]
50	cis-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,27]
51	trans-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,27]
52	1,2-Dichloropropane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,27]
53	1,3-Dichloropropane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,27]
54	1,3-Dichloropropene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,27]
55	Dieldrin	Soxhlet Extraction, Gas Chromatographic Method[10,23]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
56	Diethyl phthalate	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,28]
57	2,4-Dimethylphenol	Soxhlet Extraction, Gas Chromatographic Method[10,23]
58	2,4-Dinitrophenol	Soxhlet Extraction, Gas Chromatographic Method[10,23]
59	2,4-Dinitrotoluene	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,28]
60	2,6-Dinitrotoluene	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,28]
61	Di-n-Octyl phthalate	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,28]
62	Endosulfan	Soxhlet Extraction, Gas Chromatographic Method[10,23]
63	Endrin	Soxhlet Extraction, Gas Chromatographic Method[10,23]
64	Ethylbenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,27]
65	Fluoranthene	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,28]
66	Fluorene	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,28]
67	Heptachlor	Soxhlet Extraction, Gas Chromatographic Method[10,23]
68	Heptachlor epoxide	Soxhlet Extraction, Gas Chromatographic Method[10,23]
69	Hexachloro-1,3-butadiene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,27]
70	n-Hexane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,27]
71	α-HCH	Soxhlet Extraction, Gas Chromatographic Method[10,23]
72	β-HCH	Soxhlet Extraction, Gas Chromatographic Method[10,23]
73	γ-HCH	Soxhlet Extraction, Gas Chromatographic Method[10,23]
74	Hexachlorocyclopentadiene	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,28]
75	Hexachloroethane	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,28]
76	Indeno(1,2,3-cd)pyrene	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,28]
77	Iron	1) Digestion, Flame Atomic Absorption Spectrometric Method[7,14] 2) Digestion, Inductively Coupled Plasma Method[7,13]
78	Isophorone	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,28]

79 Lead...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
79	Lead	1) Digestion, Flame Atomic Absorption Spectrometric Method[7,14] 2) Digestion, Graphite Furnace Atomic Absorption Spectrometric Method[7,15] 3) Digestion, Inductively Coupled Plasma Method[7,13]
80	Manganese	1) Digestion, Flame Atomic Absorption Spectrometric Method[7,14] 2) Digestion, Graphite Furnace Atomic Absorption Spectrometric Method[7,15] 3) Digestion, Inductively Coupled Plasma Method[7,13]
81	Mercury	Digestion, Cold-Vapor Atomic Absorption Spectrometric Method[19]
82	Methanol	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,27]
83	Methoxychlor	Soxhlet Extraction, Gas Chromatographic Method[10,23]
84	Methyl bromide	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,27]
85	Methylene chloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,27]
86	2-Methylphenol	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,28]
87	2-Methylnaphthalene	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,28]
88	Methyl tert-butyl ether	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,27]
89	Molybdenum	Digestion, Inductively Coupled Plasma Method[7,13]
90	Naphthalene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,27]
91	Nickel	1) Digestion, Flame Atomic Absorption Spectrometric Method[7,14] 2) Digestion, Graphite Furnace Atomic Absorption Spectrometric Method[7,15] 3) Digestion, Inductively Coupled Plasma Method[7,13]
92	Nitrobenzene	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,28]
93	N-Nitrosodiphenylamine	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,28]
94	N-Nitrosodi-n-propylamine	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,28]

95 Polychlorinated...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
95	Polychlorinated Biphenyls Aroclor 1016 Aroclor 1221 Aroclor 1232 Aroclor 1242 Aroclor 1248 Aroclor 1254 Aroclor 1260 2,2',5,5'-Tetrachlorobiphenyl 2,2',4,5,5'-Pentachlorobiphenyl 2,2',3,4,4',5'-Hexachlorobiphenyl 2,2',4,4',5,5'-Hexachlorobiphenyl 2,2',3,4,4',5,5'-Heptachlorobiphenyl	Soxhlet Extraction, Gas Chromatographic Method[10,24]
96	Pentachlorophenol	Soxhlet Extraction, Gas Chromatographic Method[10,23]
97	pH	Electrometric Method[32]
98	Phenanthrene	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,28]
99	Phenol	Soxhlet Extraction, Gas Chromatographic Method[10,22]
100	Pyrene	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,28]
101	Selenium	Digestion, Hydride Generation/Atomic Absorption Spectrometric Method[7,20]
102	Silver	1) Digestion, Flame Atomic Absorption Spectrometric Method[7,14] 2) Digestion, Graphite Furnace Atomic Absorption Spectrometric Method[7,15] 3) Digestion, Inductively Coupled Plasma Method[7,13]
103	Styrene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,27]
104	1,1,2,2-Tetrachloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,27]
105	Tetrachloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,27]
106	Toluene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,27]

107 Toxaphene...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
107	Toxaphene	Soxhlet Extraction, Gas Chromatographic Method[10,23]
108	TPH (C_5-C_8)	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,27]
109	TPH ($C_{>8}$-C_{16})	Soxhlet Extraction, Gas Chromatographic Method[10,21]
110	TPH ($C_{>16}$-C_{35})	Soxhlet Extraction, Gas Chromatographic Method[10,21]
111	1,2,4-Trichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,27]
112	1,1,1-Trichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,27]
113	1,1,2-Trichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,27]
114	Trichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,27]
115	2,4,5-Trichlorophenol	Soxhlet Extraction, Gas Chromatographic Method[10,22]
116	2,4,6-Trichlorophenol	Soxhlet Extraction, Gas Chromatographic Method[10,22]
117	1,3,5-Trimethylbenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,27]
118	Vanadium	1) Digestion, Flame Atomic Absorption Spectrometric Method[7,14] 2) Digestion, Graphite Furnace Atomic Absorption Spectrometric Method[7,15] 3) Digestion, Inductively Coupled Plasma Method[7,13]
119	Vinyl acetate	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,27]
120	Vinyl chloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,27]
121	m-Xylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,27]
122	o-Xylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,27]
123	p-Xylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,27]
124	Xylene (Total)	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,27]
125	Zinc	1) Digestion, Flame Atomic Absorption Spectrometric Method[7,14] 2) Digestion, Inductively Coupled Plasma Method[7,13]

เอกสารอ้างอิง...

เอกสารอ้างอิง

1. กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2566. เรื่อง การจัดการสิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว. **ราชกิจจานุเบกษา.** 31 พฤษภาคม 2566. เล่มที่ 140 ตอนพิเศษ 126 ง.

2. กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2549. เรื่อง กำหนดค่าปริมาณเขม่าควันที่เจือปนในอากาศที่ระบายออกจากปล่องของหม้อน้ำโรงสีข้าวที่ใช้แกลบเป็นเชื้อเพลิง. **ราชกิจจานุเบกษา.** 4 ธันวาคม 2549. เล่มที่ 123 ตอนพิเศษ 125ง.

3. สมาคมวิศวกรรมสิ่งแวดล้อมแห่งประเทศไทย. **คู่มือวิเคราะห์น้ำเสีย.** พิมพ์ครั้งที่ 4. กรุงเทพฯ: เรือนแก้วการพิมพ์, 2547.

4. APHA, AWWA, WEF. **Standard Methods for the Examination of Water and Wastewater.** 24th ed. Washington, DC: APHA, 2023.

5. United States Environmental Protection Agency. **Standards of Performance for New Stationary Sources.** 40 CFR 60. Appendix A, 2022.

6. United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods. SW-846,** 1997.

7. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Acid Digestion of Sludges and Sediments and Soils. SW-846 Method 3050B,** 1996.

8. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Alkaline Digestion for Hexavalent Chromium. SW-846 Method 3060A,** 1996.

9. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Separatory Funnel Liquid-Liquid Extraction. SW-846 Method 3510C,** 1996.

10. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Soxhlet Extraction. SW-846 Method 3540C,** 1996.

11. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Purge-and-Trap for Aqueous Samples. SW-846 Method 5030C,** 2003.

12. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Closed-System Purge-and-Trap and Extraction for Volatile Organics in Soil and Waste Samples. SW-846 Method 5035A,** 2002.

13. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Inductively Coupled Plasma-Optical Emission Spectrometry. SW-846 Method 6010D,** 2018.

14. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Flame Atomic Absorption Spectrophotometry. SW-846 Method 7000B,** 2007.

15. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Graphite Furnace Atomic Absorption Spectrophotometry. SW-846 Method 7010,** 2007.

16. United...

16. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Antimony and Arsenic (Atomic Absorption, Borohydride Reduction). SW-846 Method 7062, 1994.**

17. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Chromium, Hexavalent (Colorimetric). SW-846 Method 7196A,** 1992.

18. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Mercury in Liquid Waste (Manual Cold-Vapor Technique). SW-846 Method 7470A,** 1994.

19. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Mercury in Solid or Semisolid Waste (Manual Cold-Vapor Technique). SW-846 Method 7471B,** 2007.

20. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Selenium (Atomic Absorption, Borohydride Reduction). SW-846 Method 7742,** 1994.

21. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Nonhalogenated Organics Using GC/FID. SW-846 Method 8015D,** 2003.

22. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Phenols by Gas Chromatography. SW-846 Method 8041,** 1996.

23. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Organochlorine Pesticides by Gas Chromatography. SW-846 Method 8081B,** 2007.

24. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Polychlorinate Biphenyls (PCBs) by Gas Chromatography. SW-846 Method 8082A,** 2007.

25. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Organophoshorus Compounds by Gas Chromatography. SW-846 Method 8141B,** 2007.

26. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Chlorinated Herbicides by GC Using Methylation or Pentafluorobenzylation Derivatization. SW-846 Method 8151A,** 1996.

27. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Volatile Organic Compounds by Gas Chromatography/Mass Spectrometry (GC/MS). SW-846 Method 8260D,** 2018.

28. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Semivolatile Organic Compounds by Gas Chromatography/Mass Spectrometry. SW-846 Method 8270E,** 2018.

29. United...

29. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Total and Amenable Cyanide: Distillation. SW-846 Method 9010C,** 2004.

30. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Cyanide Extraction Procedure for Solids and Oil. SW-846 Method 9013A,** 1996.

31. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Cyanide in Waters and Extracts Using Titrimetric and Manual Spectrophotometric Procedures. SW-846 Method 9014,** 2014.

32. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Soil and Waste pH. SW-846 Method 9045D,** 2004.

33. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/ Chemical Methods. **Potentiometric Determination of Fluoride in Aqueous Samples with Ion-Selective Electrode. SW-846 Method 9214,** 1996.