

ภาคผนวก ง

ใบรับรองเอกสารการสอบเทียบเครื่องมือตรวจวิเคราะห์



right solutions.
right partner.

รายการเครื่องมือที่ใช้ในการวิเคราะห์ / ทดสอบ


Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Noise	Noise Dose, TWA	Dose Badge Reader	PHK_FS0008	12-Jan-26	11-Jan-27	12
Noise	Noise Dose, TWA	Dosemeter	SGK_FS0003	5-Sep-25	4-Sep-26	12
Noise	Noise Dose, TWA	Dosemeter	SGK_FS0057	5-Sep-25	4-Sep-26	12
Noise	Noise Dose, TWA	Dosemeter	SGK_FS0098	18-Feb-26	16-Feb-27	12
Noise	Noise Dose, TWA	Dosemeter	SGK_FS0100	18-Feb-26	17-Feb-27	12
Noise	Leq 8 hrs	Sound Calibrator	SGK_FS0011	8-Oct-25	7-Oct-26	12
Noise	Leq 8 hrs	Sound Level Meter	SGK_FS0024	7-Jan-26	6-Jan-27	12
Noise	Leq 8 hrs	Sound Level Meter	SGK_FS0131	5-Jun-25	4-Jun-26	12
Noise	Leq 8 hrs	Sound Level Meter	SGK_FS0025	7-Jan-26	6-Jan-27	12
Noise	Leq 8 hrs	Sound Level Meter	SGK_FS0134	5-Jun-25	4-Jun-26	12
Noise	Leq 8 hrs	Sound Calibrator	SGK_FS0011	8-Oct-25	7-Oct-26	12
Noise	Leq 8 hrs	Sound Level Meter	SGK_FS0023	7-Jan-26	6-Jan-27	12
Noise	Leq 24 hrs	Sound Calibrator	SGK_FS0011	8-Oct-25	7-Oct-26	12
Noise	Leq 24 hrs	Sound Level Meter	SGK_FS0133	5-Jun-25	4-Jun-26	12
Illuminance	Illuminance	Lux Meter	SGK_FS0020	16-Aug-25	15-Aug-26	12
Songkhla Lab	Arsenic	ICP-MS	SGK_CL0048	4-Feb-25	3-Aug-26	18
Songkhla Lab	Arsenic	Cold Room	SGK_CL0065	15-Dec-25	15-Jun-27	18
Songkhla Lab	BOD	Incubator	SGK_CL0028	10-Jan-25	10-Jul-26	18
Songkhla Lab	BOD	DO Meter With Sensor	SGK_CL0101	24-Feb-26	24-Feb-27	12
Songkhla Lab	Cadmium	ICP-MS	SGK_CL0048	4-Feb-25	3-Aug-26	18
Songkhla Lab	Cadmium	Cold Room	SGK_CL0065	15-Dec-25	15-Jun-27	18
Songkhla Lab	COD	COD Reactor	SGK_CL0085	12-Jan-26	12-Jan-27	12
Songkhla Lab	COD	Spectrophotometer	SGK_CL0100	12-Jan-26	12-Jan-27	12
Songkhla Lab	Color (at Original pH)	Spectrophotometer	SGK_CL0040	13-Jan-26	13-Jan-27	12
Songkhla Lab	Color (at pH 7.0)	Spectrophotometer	SGK_CL0040	13-Jan-26	13-Jan-27	12
Songkhla Lab	Hexavalent Chromium	Spectrophotometer	SGK_CL0040	13-Jan-26	13-Jan-27	12
Songkhla Lab	Hexavalent Chromium	Cold Room	SGK_CL0065	15-Dec-25	15-Jun-27	18
Songkhla Lab	Trivalent Chromium	Spectrophotometer	SGK_CL0040	13-Jan-26	13-Jan-27	12
Songkhla Lab	Trivalent Chromium	Cold Room	SGK_CL0065	15-Dec-25	15-Jun-27	18
Songkhla Lab	Lead	ICP-MS	SGK_CL0048	4-Feb-25	3-Aug-26	18
Songkhla Lab	Lead	Cold Room	SGK_CL0065	15-Dec-25	15-Jun-27	18
Songkhla Lab	Mercury	ICP-MS	SGK_CL0048	4-Feb-25	3-Aug-26	18
Songkhla Lab	Mercury	Cold Room	SGK_CL0065	15-Dec-25	15-Jun-27	18
Songkhla Lab	Oil & Grease	Electronic Top-Loading Balance	SGK_CL0045	15-Dec-25	15-Dec-26	12
Songkhla Lab	Oil & Grease	Oven	SGK_CL0024	31-Mar-26	1-Oct-27	18
Songkhla Lab	Total Dissolved Solids 180°C	Electronic Top-Loading Balance	SGK_CL0045	15-Dec-25	15-Dec-26	12
Songkhla Lab	Total Dissolved Solids 180°C	Oven	SGK_CL0024	31-Mar-26	1-Oct-27	18
Songkhla Lab	Total Suspended Solids	Electronic Top-Loading Balance	SGK_CL0045	15-Dec-25	15-Dec-26	12
Songkhla Lab	Total Suspended Solids	Oven	SGK_CL0024	31-Mar-26	1-Oct-27	18

CERTIFICATE OF CALIBRATION

ISSUED BY Cirrus Research plc

DATE OF ISSUE 12 January 2026

CERTIFICATE NUMBER 256619



Cirrus Research plc
Acoustic House
Bridlington Road
Hunnamby
North Yorkshire
YO14 0PH
United Kingdom

Page 1 of 2

Approved signatory
N.Smith
Electronically signed:

doseBadge Reader : IEC 60942:2003

Instrument information

Manufacturer: Cirrus Research plc
Model: RC:110A
Serial number: 96891
Class: 2

Notes:

Test summary

Date of calibration: 12 January 2026

The doseBadge reader detailed above has been calibrated to the published data as described in the operating manual and in the half-inch configuration. The procedures and techniques used are as described in IEC60942:2003 Annex B – Periodic Tests and three determinations of the sound pressure level, frequency and total distortion were made.

The sound pressure level was measured using a WS2F condenser microphone type MK224 manufactured by Cirrus Research plc.

The results have been corrected to the reference pressure of 101.33 kPa using the manufacturer's data.

The doseBadge Reader has been shown to conform to the Class 2 requirements for periodic testing, described in Annex B of IEC 60942:2003 for the sound pressure level(s) and frequency(ies) stated, for the environmental conditions under which the tests were performed.

However, as public evidence was not available, from a testing organisation responsible for pattern approval, to demonstrate that the model of doseBadge Reader conformed to the requirements for pattern evaluation described in Annex A of IEC 60942:2003, no general statement or conclusion can be made about conformance of the doseBadge Reader to the requirements of IEC 60942:2003.

Notes:

REVIEW BY

APPROVED BY

NEXT CAL DATE: 11/01/2027

This certificate provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory. The results within this certificate relate only to the items calibrated. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2, providing a coverage probability of approximately 95%.

CERTIFICATE OF CALIBRATION

Certificate Number:
256619

Page 2 of 2

Environmental conditions

The following conditions were recorded at the time of the test:

Before Pressure: 98.87 kPa Temperature: 23.4 °C Humidity: 43.5 %
After Pressure: 98.87 kPa Temperature: 23.4 °C Humidity: 37.1 %

Test equipment

Equipment	Manufacturer	Model	Serial number
Distortion Meter	Keithley	2015	1053426
Environmental Monitor	Comet	T7510	21962628

Initial Acoustic Results

	Expected	Sample 1	Sample 2	Sample 3	Average	Deviation	Tolerance	Uncertainty
Level (dB)	114.00	114.34	114.32	114.32	114.33	0.33	±0.75	0.11 dB
Distortion (%)	< 4.00	0.09	0.08	0.10	0.09	0.09	+4.00	0.13 %
Frequency (Hz)	1000.0	997.6	997.6	997.7	997.6	-2.4	±20.0	0.1 Hz

The measured quantities or deviations (as applicable), extended by the expanded combined uncertainty of measurement, must not exceed the corresponding tolerance.

Adjusted Acoustic Results

	Expected	Sample 1	Sample 2	Sample 3	Average	Deviation	Tolerance	Uncertainty
Level (dB)	114.00	114.00	114.00	114.00	114.00	0.00	±0.75	0.11 dB
Distortion (%)	< 4.00	0.10	0.11	0.13	0.11	0.11	+4.00	0.13 %
Frequency (Hz)	1000.0	997.6	997.5	997.6	997.5	-2.5	±20.0	0.1 Hz

Functionality Results

Function	Result
Keypad	Pass
Battery Power	Pass
Display	Pass
Communication	Pass
2 way IR link	Pass
Clock	Pass

End of results



JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 6/35-36
Petchkasem 7/71, Rd. Watthapra, Bangkokyay,
Bangkok 10600 (Thailand)
Tel: +6686889812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
MSC-TS-175 17025
CALIBRATION 0367

Acoustic calibration laboratory
Calibration services department.

REVIEW BY

APPROVED BY

NEXT CAL DATE: 04/09/2026

Calibration report Number

CDM-070-68

CALIBRATION REPORT

Page 1 of 1 Pages

MEASUREMENT ITEM

MANUFACTURER

MODEL/TYPE

SERIAL NUMBER

ID NUMBER

CONDITION AS-RECEIVED

CUSTOMER

: Dose meter

: Cirrus Research plc

: CR:110A1S

: YG190

: SSK_F50003

: Used Item

: ALS laboratory group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,
Khet Suan Luang, Bangkok 10250 Thailand.

RECEIVED DATE

MEASUREMENT DATE

ISSUE DATE

: 02 Sep 2025

: 05 Sep 2025

: 05 Sep 2025

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature : 23.0 ± 3.0 °C

Relative Humidity : 55.0 ± 15.0 %RH

Atmospheric Pressure : 1010 ± 10 hPa

PRECONDITIONING

: The dose meter (Unit Under Calibration) was preconditioning 24 hours at ambient conditions prior to calibration being performed.

STANDARD USED DURING CALIBRATION:

Instrument name: doseBadge Reader Manufacturer: Cirrus Research plc Model: RC:110A Serial number: 81051

Remark: doseBadge Reader Unit with Internal Acoustic Calibrator to IEC 60942: 2003 Class 2.

CALIBRATION RESULTS:

Table 1: The results of dose meter calibration are reported in the table below.

DoseBadge Reader Level ¹ (dB)	Noise Dosimeter reading ² (dB)	Error (dB)	Status
114.0	114.0	0.0	✓

Calibrated by:

☒ Mr. Sorawit Thachalad
☐ Miss Jitraporn Lertsomphol



Approved signatory:

Mr. Parniya Booncharoen
Calibration Department Manager

Remark:

¹ The decibel level of standard doseBadge reader that supplied to Unit Under Calibration.² The measurement reading of Unit Under Calibration.

THIS CALIBRATION REPORT MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED
IN WRITING FROM THE LABORATORY



JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 6/35-36
Petchkasem 7/71, Rd. Watthapra, Bangkokyay,
Bangkok 10600 (Thailand)
Tel: +6686889812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
MSC-TS-175 17025
CALIBRATION 0367

Acoustic calibration laboratory
Calibration services department.

REVIEW BY

APPROVED BY

NEXT CAL DATE: 04/09/2026

Calibration report Number

CDM-076-68

CALIBRATION REPORT

Page 1 of 1 Pages

MEASUREMENT ITEM

MANUFACTURER

MODEL/TYPE

SERIAL NUMBER

ID NUMBER

CONDITION AS-RECEIVED

CUSTOMER

: Dose meter

: Cirrus Research plc

: CR:110A1S

: YG266

: SSK_F50057

: Used Item

: ALS laboratory group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,
Khet Suan Luang, Bangkok 10250 Thailand.

RECEIVED DATE

MEASUREMENT DATE

ISSUE DATE

: 02 Sep 2025

: 05 Sep 2025

: 05 Sep 2025

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature : 23.0 ± 3.0 °C

Relative Humidity : 55.0 ± 15.0 %RH

Atmospheric Pressure : 1010 ± 10 hPa

PRECONDITIONING

: The dose meter (Unit Under Calibration) was preconditioning 24 hours at ambient conditions prior to calibration being performed.

STANDARD USED DURING CALIBRATION:

Instrument name: doseBadge Reader Manufacturer: Cirrus Research plc Model: RC:110A Serial number: 81051

Remark: doseBadge Reader Unit with Internal Acoustic Calibrator to IEC 60942: 2003 Class 2.

CALIBRATION RESULTS:

Table 1: The results of dose meter calibration are reported in the table below.

DoseBadge Reader Level ¹ (dB)	Noise Dosimeter reading ² (dB)	Error (dB)	Status
114.0	114.0	0.0	✓

Calibrated by:

☒ Mr. Sorawit Thachalad
☐ Miss Jitraporn Lertsomphol



Approved signatory:

Mr. Parniya Booncharoen
Calibration Department Manager

Remark:

¹ The decibel level of standard doseBadge reader that supplied to Unit Under Calibration.² The measurement reading of Unit Under Calibration.

THIS CALIBRATION REPORT MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED
IN WRITING FROM THE LABORATORY

CERTIFICATE OF CALIBRATION

ISSUED BY
Cirrus Research plc

DATE OF ISSUE
18 February 2026


CERTIFICATE NUMBER
259676

SGK_FS0098

Page 1 of 6

Approved signatory
N.Smith

Electronically signed:

Cirrus Research plc

Acoustic House

Bridlington Road

Hunmanby

North Yorkshire

YO14 0PH

United Kingdom

Dosimeter : IEC 61252-1993+A1:2000

Instrument information

Manufacturer: Cirrus Research plc

Model: CR:110A

Serial number: CB1545

Firmware version: 5.4

Notes:

Test summary

Date of calibration: 18 February 2026

The calibration was performed respecting the requirements of ISO/IEC 17025:2017.


The dosimeter submitted for testing successfully completed the periodic tests of IEC 61252-1993+A1:2000.

The dosimeter submitted for testing conforms to the specifications in IEC 61252-1993+A1:2000.

Equipment	Manufacturer	Model	Serial number
Signal Generator	SIGLENT	SDG1032X	SDG1XDDC7R0315
Attenuator	Cirrus Research	ZE-952	101223
Environmental Monitor	Comet	T7510	16966334
doseBadge Reader	Cirrus Research plc	RC:110A	109288

Notes

REVIEW BY: 

APPROVED BY: 

NEXT CAL DATE: 16/ 02/ 2027

This certificate provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory. The results within this certificate relate only to the items calibrated. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2, providing a coverage probability of approximately 95%.

CERTIFICATE OF CALIBRATION

Certificate Number:
259676

Page 3 of 6

Laboratory uncertainties

Requirement	Value
Absolute acoustic sensitivity	0.2 dB
Level linearity	0.15 dB
Short duration signals	0.2 dB
Overload latching indication	0.2 dB
Electrical freq. weighting 125 Hz	0.15 dB
Electrical freq. weighting 8 kHz	0.15 dB

CERTIFICATE OF CALIBRATION

Certificate Number:
259676

Page 2 of 6

Environmental conditions

The following conditions were recorded at the time of the test:

Before Pressure: 100.41 kPa Temperature: 21.2 °C Humidity: 33.1 %

After Pressure: 100.39 kPa Temperature: 21.4 °C Humidity: 34.2 %

Test	Result
Absolute Acoustic Sensitivity 1995	Complies
Linearity 1995	Complies
Short Duration 1995	Complies
Overload Latching 1995	Complies
Frequency weighting 1995	Complies

CERTIFICATE OF CALIBRATION

Certificate Number:
259676

Page 4 of 6

B1: Absolute Acoustical Sensitivity

Frequency: 1000 Hz

Uncertainty: 0.2 dB

Result: Passed

Name	Input Level (dB)	Reading (dB)	Deviation (dB)	Limits (dB)
Initial	114	114.90	-0.9	113 / 115
Adjusted	114	114.00	0	113 / 115

B2: Linearity Of Response To Steady Signals

Frequency: 1000 Hz

Uncertainty: 0.2 dB

Range: 80 – 130 dB

Result: Passed

Input Level (dB)	Expected Exposure (Pa²h)	Exposure (Pa²h)	Duration (s)	Deviation (Pa²h)	Limits (Pa²h)	Deviation (%)	Limits (%)
80	0.000222	0.000280	20	-0.000058	0.000175 / 0.000280	26	-21 / +26
90	0.002222	0.002327	20	-0.000105	0.001755 / 0.002800	5	-21 / +26
100	0.022222	0.022740	20	-0.000518	0.017555 / 0.028000	2	-21 / +26
110	0.222222	0.227398	20	-0.005176	0.175555 / 0.280000	2	-21 / +26
120	2.222222	2.326952	20	-0.104730	1.755555 / 2.800000	5	-21 / +26
130	22.222223	23.811541	20	-1.589318	17.555556 / 28.000001	7	-21 / +26

CERTIFICATE OF CALIBRATION

Certificate Number:
259676
Page 5 of 6

B3: Frequency Weightings

Reference Frequency: 1000 Hz
Reference Exposure: 5.6984599601109
Reference Input Level: 127 dB
Duration: 10 Seconds

Result: Passed

Frequency (Hz)	Exposure (Pa ² h)	Exposure Ratio	Ratio Limit	Uncertainty
125	0.127573	0.0224	0.0174 / 0.0347	0.15
8000	2.375513	0.4169	0.246 / 2.455	0.15

B4: Short-Duration Signals

Uncertainty: 0.2 dB
Frequency: 4000 Hz

Result: Passed

Input Level (dB)	Burst Level (dB)	Ratio	Duration (s)	Burst Duration (ms)	Duration Between Bursts (ms)	Expected Exposure (Pa ² h)	Exposure (Pa ² h)	Deviation (%)	Limits (%)
114	95	1:100	10	10	990	0.003595	0.003279	-9	-21 / +26
129	100	1:1000	10	1	999	0.011370	0.009903	-13	-29 / +41

CERTIFICATE OF CALIBRATION

ISSUED BY
Cirrus Research plc

DATE OF ISSUE
18 February 2026

CERTIFICATE NUMBER
259674

Cirrus Research plc
Acoustic House
Bridlington Road
Hunmanby
North Yorkshire
YO14 0PH
United Kingdom

Page 1 of 6
Approved signatory
N.Smith
Electronically signed:

Dosimeter : IEC 61252-1993+A1:2000

Instrument information

Manufacturer: Cirrus Research plc
Model: CR:110A
Serial number: CB1547
Firmware version: 5.4

Notes

Test summary

Date of calibration: 18 February 2026

The calibration was performed respecting the requirements of ISO/IEC 17025:2017.

The dosimeter submitted for testing successfully completed the periodic tests of IEC 61252-1993+A1:2000.

The dosimeter submitted for testing conforms to the specifications in IEC 61252-1993+A1:2000.

Test equipment

Equipment	Manufacturer	Model	Serial number
Signal Generator	SIGLENT	SDG1032X	SDG1XDDQ6R6307
Attenuator	Cirrus Research	ZE:952	101220
Environmental Monitor	Comet	T7510	16966334
doseBadge Reader	Cirrus Research plc	RC:110A	100498

Notes

REVIEW BY:
APPROVED BY:
NEXT CAL DATE: 17/02/2027

This certificate provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory. The results within this certificate relate only to the items calibrated. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2, providing a coverage probability of approximately 95%.

CERTIFICATE OF CALIBRATION

Certificate Number:
259676
Page 6 of 6

B6: Latching Overload Indicator

Frequency: 1000 Hz
Uncertainty: 0.2 dB

Result: Passed

Level (dB)	Expected To Overload	Overloaded
130	No	No
133	Yes	Yes

CERTIFICATE OF CALIBRATION

Certificate Number:
259674
Page 2 of 6

Environmental conditions

The following conditions were recorded at the time of the test:

Before Pressure: 100.36 kPa
Temperature: 21.4 °C
Humidity: 34.6 %

After Pressure: 100.34 kPa
Temperature: 21.3 °C
Humidity: 35.2 %

Test results summary

Test	Result
Absolute Acoustic Sensitivity 1995	Complies
Linearity 1995	Complies
Short Duration 1995	Complies
Overload Latching 1995	Complies
Frequency weighting 1995	Complies

End of results

CERTIFICATE OF CALIBRATION

Certificate Number:
259674
Page 3 of 6

Laboratory uncertainties

Requirement	Value
Absolute acoustic sensitivity	0.2 dB
Level linearity	0.15 dB
Short duration signals	0.2 dB
Overload latching indication	0.2 dB
Electrical freq. weighting 125 Hz	0.15 dB
Electrical freq. weighting 8 kHz	0.15 dB

CERTIFICATE OF CALIBRATION

Certificate Number:
259674
Page 5 of 6

B3: Frequency Weightings

Reference Frequency: 1000 Hz Reference Exposure: 9.215338495193
Reference Input Level: 127 dB Duration: 10 Seconds

Frequency (Hz)	Exposure (Pa ² h)	Exposure Ratio	Ratio Limit	Uncertainty
125	0.201610	0.0219	0.0174 / 0.0347	0.15
8000	2.068986	0.4266	0.246 / 2.455	0.15

Result: Passed

B4: Short-Duration Signals

Uncertainty: 0.2 dB Frequency: 4000 Hz

Input Level (dB)	Burst Level (dB)	Ratio	Duration (s)	Burst Duration (ms)	Duration Between Bursts (ms)	Expected Exposure (Pa ² h)	Exposure (Pa ² h)	Deviation (%)	Limits (%)
114	95	1:100	10	10	990	0.003595	0.003356	-7	-21 / +26
129	100	1:1000	10	1	999	0.011370	0.010369	-9	-29 / +41

Result: Passed

CERTIFICATE OF CALIBRATION

Certificate Number:
259674
Page 4 of 6

B1: Absolute Acoustical Sensitivity

Frequency: 1000 Hz Uncertainty: 0.2 dB

Name	Input Level (dB)	Reading (dB)	Deviation (dB)	Limits (dB)
Initial	114	115.30	-1.3	113 / 115
Adjusted	114	114.00	0	113 / 115

Result: Passed

B2: Linearity Of Response To Steady Signals

Result: Passed

Frequency: 1000 Hz Uncertainty: 0.2 dB Range: 80 – 130 dB

Input Level (dB)	Expected Exposure (Pa ² h)	Exposure (Pa ² h)	Duration (s)	Deviation (Pa ² h)	Limits (Pa ² h)	Deviation (%)	Limits (%)
80	0.000222	0.000267	20	-0.000045	0.000175 / 0.000280	20	-21 / +26
90	0.003111	0.003040	20	0.000071	0.002458 / 0.003920	-2	-21 / +26
100	0.022222	0.022222	20	-0.000000	0.017555 / 0.028000	-0	-21 / +26
110	0.311111	0.318358	20	-0.007247	0.245778 / 0.392000	2	-21 / +26
120	3.111111	3.183578	20	-0.072467	2.457778 / 3.920000	2	-21 / +26
130	31.111112	33.336157	20	-2.225045	24.577778 / 39.200001	7	-21 / +26

CERTIFICATE OF CALIBRATION

Certificate Number:
259674
Page 6 of 6

B6: Latching Overload Indicator

Result: Passed

Frequency: 1000 Hz Uncertainty: 0.2 dB

Level (dB)	Expected To Overload	Overloaded
130	No	No
133	Yes	Yes

End of results

Cert. No. : ACC25059
Pages : 1 of 3

Calibration Certificate

Equipment : SOUND CALIBRATOR
Manufacturer : RION
Model : NC-74
Serial No.: 34478386
ID No.: SGK_FS0011

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 26 SEPTEMBER 2025
Calibration Date : 08 OCTOBER 2025
Date of Issue : 10 OCTOBER 2025

Calibrated by : Nathakorn Pisutpaisan

Approved by :
(Nitinun Srihawan)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACC25059
Job No. : VC68AC0190
Pages : 3 of 3

Result of calibration :

1. Sound pressure level

Specified sound pressure level (dB)	Measured value (dB)	Deviated value (dB)	Uncertainty (dB)	Acceptance limit (dB)
94	94.15	0.15	0.14	0.40

2. Frequency

Specified Frequency (Hz)	Measured value (Hz)	Deviated value (%)	Uncertainty (%)	Acceptance limit (%)
1000	1002.5	0.3	0.1	1.0

3. Total distortion

Measured value (%)	Uncertainty (%)	Acceptance limit (%)
1.45	0.10	3.0

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

Cert. No. : ACC25059
Job No. : VC68AC0190
Pages : 2 of 3

Calibration Procedure : CP-AC-03

Calibration Method :

This equipment was calibrated by follow on IEC-60942-2003 Standard.
The sound pressure level, frequency and total distortion of the sound calibrator was measured using the reference microphone.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EELBP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EELBP 23/0268	22-APR-26
Digital Multimeter	33461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KAI	34560495	AA-3002-25	19-FEB-26
Audio Analyzer	AVR-3360A	V744B6069	EF-0013-25	13-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).
- 3.3 Electrical And Electronics Institute (EEI).

Cert. No. : ACL26034
Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.: 00672671 / 179122 / 87529
ID No.: SGK_FS0024

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 05 JANUARY 2026
Calibration Date : 07 JANUARY 2026
Date of Issue : 09 JANUARY 2026

Calibrated by : Nathakorn Pisutpaisan

Approved by :
(Nitinun Srihawan)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL26034
Job No. : VC69AC0051
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0011-25	11-FEB-26
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EEL-BP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EEL-BP 23/0268	22-APR-26
Digital Multimeter	34461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KAI	34560495	AA-3002-25	19-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).
- 3.3 Electrical And Electronics Institute (EEI).

Signature

Cert. No. : ACL26034
Job No. : VC69AC0051
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
16.4

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	12.6
C - weight	18.8
Flat	24.6

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.1	0.2	0.2	± 1.5
1000	-0.1	-0.1	0.1	± 1.0
8000	2.5	2.6	2.6	±5.0

Signature

Cert. No. : ACL26034
Job No. : VC69AC0051
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

Signature

Cert. No. : ACL26034
Job No. : VC69AC0051
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	-0.1	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

Signature

Cert. No. : ACL26034
Job No. : VC69AC0051
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	53.9	-0.1	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	38.9	-0.1	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	26.9	-0.1	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.9	-0.1	± 1.1

02/06/2026

Cert. No. : ACL26034
Job No. : VC69AC0051
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.4	0.0	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.5	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

02/06/2026

Cert. No. : ACL26034
Job No. : VC69AC0051
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1


Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	28.9	-0.1	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, T _b (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.0 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

02/06/2026

451-451/1 Sirinthon Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiporn.com



Cert. No. : ACL25217
Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-52A / Microphone UC-59 / Preamplifier NH-25
Serial No.: 00331094 / 22922 / 22569
ID No.: SGK_FS0131

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 26 MAY 2025
Calibration Date : 05 JUNE 2025
Date of Issue : 06 JUNE 2025

Calibrated by : Nathakorn Pisutpaisan

Approved by : Wichok Ekpongpradit

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL25217
Job No. : VC68AC0112
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0011-25	11-FEB-26
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EEL-BP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EEL-BP 23/0268	22-APR-26
Digital Multimeter	34461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KAI	34560495	AA-3002-25	19-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).
- 3.3 Electrical And Electronics Institute (EEI).

Michael E.

Cert. No. : ACL25217
Job No. : VC68AC0112
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	94.0	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
13.8

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	10.8
C - weight	16.0
Flat	21.3

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.5	0.6	0.6	± 1.0
1000	0.3	0.3	0.3	± 0.7
8000	0.5	0.6	0.6	+ 1.5, - 2.5

Michael E.

Cert. No. : ACL25217
Job No. : VC68AC0112
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

Michael E.

Cert. No. : ACL25217
Job No. : VC68AC0112
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	0.1	±1.0
125	0.1	0.1	0.1	±1.0
250	0.0	0.1	0.0	±1.0
500	0.0	0.1	0.0	±1.0
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±1.0
4000	0.0	0.0	0.0	±1.0
8000	0.0	0.1	0.1	+ 1.5, - 2.5
16000	0.0	-1.2	-1.2	+ 2.5, -16.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Lcq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.1

Michael E.

Cert. No. : ACL25217
Job No. : VC68AC0112
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	±0.8
136.0	136.0	0.0	±0.8
135.0	135.0	0.0	±0.8
134.0	134.0	0.0	±0.8
133.0	133.0	0.0	±0.8
132.0	132.0	0.0	±0.8
131.0	131.0	0.0	±0.8
129.0	129.0	0.0	±0.8
124.0	124.0	0.0	±0.8
119.0	119.0	0.0	±0.8
114.0	114.0	0.0	±0.8
109.0	109.0	0.0	±0.8
104.0	104.0	0.0	±0.8
99.0	99.0	0.0	±0.8
94.0	94.0	0.0	±0.8
89.0	89.0	0.0	±0.8
84.0	84.0	0.0	±0.8
79.0	79.0	0.0	±0.8
74.0	74.0	0.0	±0.8
69.0	69.0	0.0	±0.8
64.0	64.0	0.0	±0.8
59.0	59.0	0.0	±0.8
54.0	54.0	0.0	±0.8
49.0	49.0	0.0	±0.8
44.0	44.0	0.0	±0.8
39.0	39.0	0.0	±0.8
34.0	34.0	0.0	±0.8
30.0	30.0	0.0	±0.8
29.0	28.9	-0.1	±0.8
28.0	27.9	-0.1	±0.8
27.0	27.0	0.0	±0.8
26.0	26.0	0.0	±0.8
25.0	24.9	-0.1	±0.8

Wichon E.

Cert. No. : ACL25217
Job No. : VC68AC0112
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±2.0
One	133.4	133.3	-0.1	±2.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±1.0
Positive half cycle	135.4	135.1	-0.3	±1.0
Negative half cycle	135.4	135.1	-0.3	±1.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.6	0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.1

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

Wichon E.

Cert. No. : ACL25217
Job No. : VC68AC0112
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±0.8

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	29.0	0.0	±0.8

9. Tone burst response

Time Weighting	Tone burst duration, T _b (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.0 ; -3.0
	2	8	117.0	117.0	0.0	1.0 ; -1.5
	200	800	134.0	134.1	0.1	±0.5
Slow	2	8	108.0	108.0	0.0	1.0 ; -3.0
	200	800	127.6	127.6	0.0	±0.5
SEL	0.25	1	99.0	98.9	-0.1	1.0 ; -3.0
	2	8	108.0	108.0	0.0	1.0 ; -1.5
	200	800	128.0	128.1	0.1	±0.5

Wichon E.

Cert. No. : ACL26035
Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.: 00873117 / 169442 / 72463
ID No.: SGK_FS0025

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 05 JANUARY 2026
Calibration Date : 07 JANUARY 2026
Date of Issue : 09 JANUARY 2026

Calibrated by : Nathakorn Pisutpaisan

Approved by : Nitinun Srihawan

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL26035
Job No. : VC69AC0051
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0011-25	11-FEB-26
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EEL_BP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EEL_BP 23/0268	22-APR-26
Digital Multimeter	34461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KAI	34560495	AA-3002-25	19-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).
- 3.3 Electrical And Electronics Institute (EEI).

CP/Rev. 0.5

Cert. No. : ACL26035
Job No. : VC69AC0051
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
16.1

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	13.1
C - weight	19.1
Flat	24.7

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.2	0.3	0.3	± 1.5
1000	0.1	0.1	0.1	± 1.0
8000	1.2	1.3	1.3	±5.0

CP/Rev. 0.5

Cert. No. : ACL26035
Job No. : VC69AC0051
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

CP/Rev. 0.5

Cert. No. : ACL26035
Job No. : VC69AC0051
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

CP/Rev. 0.5

Cert. No. : ACL26035
Job No. : VC69AC0051
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	38.9	-0.1	± 1.1
34.0	34.0	0.0	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	28.0	0.0	± 1.1
27.0	26.9	-0.1	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.9	-0.1	± 1.1

Reference

Cert. No. : ACL26035
Job No. : VC69AC0051
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.4	0.0	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.5	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

Reference

Cert. No. : ACL26035
Job No. : VC69AC0051
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	28.9	-0.1	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, T _b (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.0 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

Reference

451-451/1 Sirinthorn Road, Bangbunmu, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiporn.com



Cert. No. : ACL25220
Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-52A / Microphone UC-59 / Preamplifier NH-25
Serial No.: 00331097 / 22940 / 22572
ID No.: SGK_FS0134

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWANG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 26 MAY 2025
Calibration Date : 05 JUNE 2025
Date of Issue : 06 JUNE 2025

Calibrated by : Nathakorn Pisutpaisan

Approved by :
(Wichok Ekpongpradit)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL25220
Job No. : VC68AC0112
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0011-25	11-FEB-26
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EEL-BP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EEL-BP 23/0268	22-APR-26
Digital Multimeter	34461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KAI	34560495	AA-3002-25	19-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).
- 3.3 Electrical And Electronics Institute (EEI).

นิชกร เอ.

Cert. No. : ACL25220
Job No. : VC68AC0112
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	94.0	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
14.6

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	12.0
C - weight	16.8
Flat	22.6

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.4	0.4	0.4	± 1.0
1000	0.2	0.2	0.2	± 0.7
8000	0.5	0.6	0.6	+ 1.5, - 2.5

นิชกร เอ.

Cert. No. : ACL25220
Job No. : VC68AC0112
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

นิชกร เอ.

Cert. No. : ACL25220
Job No. : VC68AC0112
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	-0.1	0.0	±1.0
125	0.0	0.0	0.0	±1.0
250	0.0	0.0	0.0	±1.0
500	0.0	0.0	-0.1	±1.0
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±1.0
4000	0.0	0.0	0.0	±1.0
8000	0.0	0.0	0.0	+ 1.5, - 2.5
16000	0.0	-1.3	-1.2	+ 2.5, -16.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.1

นิชกร เอ.

Cert. No. : ACL25220
Job No. : VC68AC0112
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	±0.8
136.0	136.0	0.0	±0.8
135.0	135.1	0.1	±0.8
134.0	134.1	0.1	±0.8
133.0	133.0	0.0	±0.8
132.0	132.0	0.0	±0.8
131.0	131.0	0.0	±0.8
129.0	129.0	0.0	±0.8
124.0	124.0	0.0	±0.8
119.0	119.1	0.1	±0.8
114.0	114.1	0.1	±0.8
109.0	109.0	0.0	±0.8
104.0	104.1	0.1	±0.8
99.0	99.0	0.0	±0.8
94.0	94.0	0.0	±0.8
89.0	89.0	0.0	±0.8
84.0	84.0	0.0	±0.8
79.0	79.0	0.0	±0.8
74.0	74.0	0.0	±0.8
69.0	69.0	0.0	±0.8
64.0	64.0	0.0	±0.8
59.0	59.0	0.0	±0.8
54.0	54.0	0.0	±0.8
49.0	49.0	0.0	±0.8
44.0	44.0	0.0	±0.8
39.0	39.0	0.0	±0.8
34.0	34.0	0.0	±0.8
30.0	30.0	0.0	±0.8
29.0	29.0	0.0	±0.8
28.0	27.9	-0.1	±0.8
27.0	27.0	0.0	±0.8
26.0	26.0	0.0	±0.8
25.0	24.9	-0.1	±0.8

Nithin S.

Cert. No. : ACL25220
Job No. : VC68AC0112
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±2.0
One	133.4	133.3	-0.1	±2.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±1.0
Positive half cycle	135.4	135.2	-0.2	±1.0
Negative half cycle	135.4	135.2	-0.2	±1.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.5	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.1

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

Nithin S.

Cert. No. : ACL25220
Job No. : VC68AC0112
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±0.8

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	28.9	-0.1	±0.8

9. Tone burst response

Time Weighting	Tone burst duration, T _b (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.0 ; -3.0
	2	8	117.0	116.9	-0.1	1.0 ; -1.5
	200	800	134.0	134.0	0.0	±0.5
Slow	2	8	108.0	108.0	0.0	1.0 ; -3.0
	200	800	127.6	127.6	0.0	±0.5
	0.25	1	99.0	98.8	-0.2	1.0 ; -3.0
SEL	2	8	108.0	107.9	-0.1	1.0 ; -1.5
	200	800	128.0	128.0	0.0	±0.5

Nithin S.

Cert. No. : ACL26033
Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.: 00672670 / 169441 / 72462
ID No.: SGK_FS0023

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 05 JANUARY 2026
Calibration Date : 07 JANUARY 2026
Date of Issue : 09 JANUARY 2026

Calibrated by : Nathakorn Pisutpaisan

Approved by : Nitinun Srihawan

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL26033
Job No. : VC69AC0051
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0011-25	11-FEB-26
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EEL-BP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EEL-BP 23/0268	22-APR-26
Digital Multimeter	34461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KAI	34560495	AA-3002-25	19-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).
- 3.3 Electrical And Electronics Institute (EEI).

CSSTechon.S.

Cert. No. : ACL26033
Job No. : VC69AC0051
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
15.4

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	12.6
C - weight	18.5
Flat	24.3

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.1	0.2	0.2	± 1.5
1000	-0.1	0.0	0.0	± 1.0
8000	1.2	1.3	1.2	±5.0

CSSTechon.S.

Cert. No. : ACL26033
Job No. : VC69AC0051
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

CSSTechon.S.

Cert. No. : ACL26033
Job No. : VC69AC0051
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

CSSTechon.S.

Cert. No. : ACL26033
Job No. : VC69AC0051
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.1	0.1	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.1	0.1	± 1.1
69.0	69.1	0.1	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.1	0.1	± 1.1
30.0	30.1	0.1	± 1.1
29.0	29.1	0.1	± 1.1
28.0	28.1	0.1	± 1.1
27.0	27.1	0.1	± 1.1
26.0	26.2	0.2	± 1.1
25.0	25.1	0.1	± 1.1

MPTK00005

Cert. No. : ACL26033
Job No. : VC69AC0051
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.2	-0.2	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.6	0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$

or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

MPTK00005

Cert. No. : ACL26033
Job No. : VC69AC0051
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	29.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, T _b (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.0 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

MPTK00005

Cert. No. : ACL25219
Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-S2A / Microphone UC-59 / Preamplifier NH-25
Serial No.: 00331096 / 22929 / 22571
ID No.: SGK_FS0133

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 26 MAY 2025
Calibration Date : 05 JUNE 2025
Date of Issue : 06 JUNE 2025

Calibrated by : Nathakorn Pisutpaisan

Approved by : 
(Wichok Ekpongpradit)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL25219
Job No. : VC68AC0112
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0011-25	11-FEB-26
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EEL-BP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EEL-BP 23/0268	22-APR-26
Digital Multimeter	34461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KAI	34560495	AA-3002-25	19-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).
- 3.3 Electrical And Electronics Institute (EEI).

Signature

Cert. No. : ACL25219
Job No. : VC68AC0112
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	94.0	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
13.4

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	8.7
C - weight	14.3
Flat	19.8

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.4	0.4	0.4	± 1.0
1000	0.2	0.2	0.2	± 0.7
8000	0.5	0.6	0.6	+ 1.5, - 2.5

Signature

Cert. No. : ACL25219
Job No. : VC68AC0112
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

Signature

Cert. No. : ACL25219
Job No. : VC68AC0112
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.1	0.0	0.1	±1.0
125	0.1	0.1	0.0	±1.0
250	0.0	0.0	0.0	±1.0
500	0.0	0.0	0.0	±1.0
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±1.0
4000	0.0	0.0	0.0	±1.0
8000	0.0	0.1	0.1	+ 1.5, - 2.5
16000	0.0	-1.2	-1.2	+ 2.5, -16.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Lcq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.1

Signature

Cert. No. : ACL25219
Job No. : VC68AC0112
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	±0.8
136.0	136.0	0.0	±0.8
135.0	135.0	0.0	±0.8
134.0	134.0	0.0	±0.8
133.0	133.0	0.0	±0.8
132.0	132.0	0.0	±0.8
131.0	131.0	0.0	±0.8
129.0	129.0	0.0	±0.8
124.0	124.0	0.0	±0.8
119.0	119.0	0.0	±0.8
114.0	114.0	0.0	±0.8
109.0	109.0	0.0	±0.8
104.0	104.0	0.0	±0.8
99.0	99.0	0.0	±0.8
94.0	94.0	0.0	±0.8
89.0	89.0	0.0	±0.8
84.0	83.9	-0.1	±0.8
79.0	78.9	-0.1	±0.8
74.0	74.0	0.0	±0.8
69.0	68.9	-0.1	±0.8
64.0	63.9	-0.1	±0.8
59.0	58.9	-0.1	±0.8
54.0	53.9	-0.1	±0.8
49.0	48.9	-0.1	±0.8
44.0	43.9	-0.1	±0.8
39.0	38.9	-0.1	±0.8
34.0	33.9	-0.1	±0.8
30.0	29.9	-0.1	±0.8
29.0	28.9	-0.1	±0.8
28.0	27.9	-0.1	±0.8
27.0	26.9	-0.1	±0.8
26.0	25.9	-0.1	±0.8
25.0	24.9	-0.1	±0.8

nicola E.

Cert. No. : ACL25219
Job No. : VC68AC0112
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±2.0
One	133.4	133.3	-0.1	±2.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±1.0
Positive half cycle	135.4	135.2	-0.2	±1.0
Negative half cycle	135.4	135.2	-0.2	±1.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.6	0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.1

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

nicola E.

Cert. No. : ACL25219
Job No. : VC68AC0112
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±0.8

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	28.9	-0.1	±0.8

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.0 ; -3.0
	2	8	117.0	117.0	0.0	1.0 ; -1.5
	200	800	134.0	134.0	0.0	±0.5
Slow	2	8	108.0	108.0	0.0	1.0 ; -3.0
	200	800	127.6	127.6	0.0	±0.5
	0.25	1	99.0	98.9	-0.1	1.0 ; -3.0
SEL	2	8	108.0	108.0	0.0	1.0 ; -1.5
	200	800	128.0	128.0	0.0	±0.5

nicola E.



CALIBRATION LABORATORY Co., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2872 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : DIGITAL LUX METER
MANUFACTURER : DELTA OHM
MODEL / TYPE : HD2102.2
SERIAL NO. : 17020596 [SGK_FS0020]
CLID. NO. : 252502055
JOB CONTROL NO. : 250815094790
CALIBRATION SERVICE : ☒ IN-LABORATORY ☐ ON-SITE

CUSTOMER : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN RD.,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG, BANGKOK 10250, THAILAND

DATE OF RECEIVED : 15 August 2025

DATE OF ISSUED : 18 August 2025

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Suwit Phuanbusabong
Calibration Engineer

Approved By : Mongkol Yotsoontorn
Authorized Signatory
18 August 2025



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q25094790
F3-011-05/12-23

page 1 of 3





CALIBRATION LABORATORY CO., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



REPORT OF CALIBRATION

FOR

NOMENCLATURE : DIGITAL LUX METER
MANUFACTURER : DELTA OHM
MODEL / TYPE : HD2102.2
SERIAL NO. : 17020596 [SGK_FS0020]
DATE OF CALIBRATION : 16 August 2025

ENVIRONMENT CONDITIONS :

Temperature : $(23 \pm 2) ^\circ\text{C}$ Relative Humidity : $(55 \pm 15) \% \text{RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. CLC-CPEE-18 by comparison with Photometer/Radiometer & Illuminance

Sensor which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

Photometer/Radiometer & Illuminance Sensor, Bentham Model ORM400/DI400VL S/N. 27710/1/27585/3.

TRACEABILITY :

The measurements are traceable to International System of Units (SI) , through Optical Test and Calibration Ltd.

Certificate No. 158628/ABU, Due Date 01 May 2027.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2.00$ which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4:02 M:2022)"

Certificate No. Q25094790

F3-011-05/12-23

page 2 of 3



@clccalibration


Agilent Technologies

Agilent Technologies (Thailand) Limited
U CHU LIANG BLDG. 22/F UNIT A.D
968 RAMA 4 ROAD, SILOM, BANGRAK
Bangkok 10500 Thailand

Tel. +662 637 6363
Fax. +662 632 4334
Email: ccc-smt@agilent.com
Website: www.agilent.com/chem

SERVICE REPORT

Customer Purchase Order Number:	Customer Number: 70371013
Service Request:	Service Request Date:
Service Order: 6007493912	Service Confirmation: 6906126918



Invoice To:

ALS Laboratory Group (Thailand) Co Ltd Head Office

104 Phatthanakan 40 Phatthanakan Rd
Khaeng Phatthanakan Khet Suan

Payer:

ALS Laboratory Group (Thailand) Co Ltd Branch Number 0002
114/1 Moo8 Banplu Subdistrict Hat Yai District

SONGKHLA 90250

Delivery Site:

ALS Laboratory Group (Thailand) Co Ltd Branch Number 0002
114/1 Moo8 Banplu Subdistrict Hat Yai District

Location:

Room
Bldg
Lab
Dept

Direct Inquiries to:

Contact Name: Customer Contact Center
Contact E-mail: ccc-smt@agilent.com
Contact Telephone: +662 637 6363
Contact Fax: +662 632 4334

products | applications | software | services

Learn more about Agilent's Special Offers, Products, Services and our full range of laboratory productivity solutions optimized for your applications and workflows. Visit us at www.agilent.com/chem

Agilent Technologies (Thailand) Limited, Head Office
U Chu Liang Bldg 22/F Unit A.D
968 Rama 4 Road, Silom, Bangrak,
Bangkok 10500 Thailand
Tax ID : 010554208218

Citibank N.A. Bangkok Branch
389 Interchange 21 Building, Sukhumvit Road, Klongtoey Nau Sub-district, Wattana District, Bangkok 10110 Thailand
Acc. No: 012 4452-007
THB:Krung Thai Bank PCL
Siam Square Br. 415/1-2 Rama 1 Rd, Pathumwan, BKK 10330 Thailand

ORIGINAL

Page 1 of 3



CALIBRATION LABORATORY CO., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment () adjustment

CALIBRATION DATA

DIGITAL LUX METER RESULT

STD Applied (lux)	DUC Reading (lux)	Correction (lux)	Uncertainty $\pm$ (% of rdg.)
0.00	0.00	0.00	-
15.00	14.99	+0.01	3.2
50.00	50.80	-0.80	2.6
100.00	101.97	-1.97	2.6
500.0	511.3	-11.3	2.6
1000.0	1022.9	-22.9	2.6
2000	2046	-46	3.8
3000	3069	-69	3.8
4000	4093	-93	3.8
5000	5116	-116	3.8

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 015 Page 56 of 68

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q25094790

F3-011-05/12-23

page 3 of 3



@clccalibration

Service Confirmation Number: 6906126918

Service Confirmation Date: 04.02.2025

Service Instrument:

Model Number	Model Description	Serial Number	System Handle	Parent Asset
SYS-IM-7900	ICPMS 7900 System			
G7201C	ICP-MS MassHunter SW only (excludes PC)	USH3799575	ICP MS 7900	SYS-IM-7900
G8403A	Agilent 7900 ICP-MS	JP16511669	ICP MS 7900	SYS-IM-7900
G8411A	ISIS 3 for Agilent 7850/7900/8900	JP16510379	ICP MS 7900	SYS-IM-7900

Service Items:

Item	Service/Part #	Description	Qty	Entitlement	Service Start	Service End
1000	EQQ	Enterprise Operational Qualification	1.00	Agreement Entitlement 100 % covered	03.02.2025	04.02.2025
1010	5185-5850	ICP-MS Checkout Solutions	1.00	Agreement Entitlement 100 % covered		

Additional Information:

Page 2 of 3

Service Information:

Problem Description:
*PR-OQ-ICP MS 7900-5001391286

Service Provided:
OQ_SGK_CL0048
Perform oq test . Sensitivity, resolution background both He and H2 mode. Stability test all pass. Sent oq report to customer. Let s customer test run sample.

Service Overview Code:
Reason Code: Scheduled Service
Diagnosis Code: Scheduled Service
Resolution Code: Scheduled Service

Reported Hours:
7.0

Travel Hours:
2.0

Customer Field Service
Representative Name:
Worawit Timakul

Customer Field Service
Representative Signature:

Date:
04 Feb 2025

Customer Name:
TANYATORN MONGKONJIRAWUT

Customer Signature:

Date:
04 Feb 2025

Additional Comments:

Details of Calibration


1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data Acquisition Switch Unit with Sensor	DAQ970A	MY58036254	QR25-2036	1-Jul-2026

- The results reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.
- This certificate is not certified any commercial transaction
- Condition of item : normal condition , no indication for any damage or malfunction

Result of Calibration : [✓] Without Adjustment [] After Adjustment

1. Sensor Installation Diagram

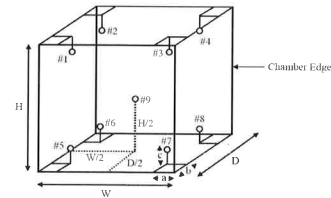

Sensor Installation Details

a = 5.0 cm
b = 5.0 cm
c = 5.0 cm

Dimension of the chamber

W = 40.0 cm
H = 40.0 cm
D = 33.0 cm

Southern Calibration Service Co., Ltd.

669/35 Kanjanavanit Rd., Banpru, Hatyai, Songkhla 90250 Thailand
Tel : 08 1599 0417 Fax : 0 7480 5133 Email : s.calibration@gmail.com www.scal.co.th



CALIBRATION CERTIFICATE

Issued Date : 18-Dec-2025

Certificate No. : 25TH5497

CSR No. : A230/11460

Page : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Chemical Laboratory

Instrument Name : Cold Room

Manufacturer : N/A

Model : N/A

Serial No. : N/A

ID No. : SGK_CL0065


Resolution : 0.1 °C

Received Date : 15-Dec-2025

Calibrated Date : 15-Dec-2025

Ambient Temperature : (30 ± 10) °C

Relative Humidity : (50 ± 30) %



Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.012 based on GLA - 20

The Southern Calibration Service Co.,Ltd calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- Q Reborn : Quality Reborn Co.,Ltd.

Calibrated by : Ibrorhim Saleemin

Approved by :

Imron Rattanaylum / Technical Manager



The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Result of Calibration :

2. Temperature Measurement Accuracy Test

The measurement results of the Cold Room and associates are reported in the manner as shown below

Cal point (°C)	Measured Standard Temperature At Spread Locations (°C)								Uncertainty (±°C)	
	#1	#2	#3	#4	#5	#6	#7	#8		Ref. 9
4	3.95	4.10	4.10	4.02	4.10	3.95	3.90	3.99	3.95	0.38

3. Temperature Performance Result

The performance of the Cold Room are reported as shown below

UUC Setting (°C)	UUC Reading (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
4.0	4.0	0.05	0.86	0.86

UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95%

... End ...

CARIBRATION CERTIFICATE

Issued Date : 13-Jan-2025

Certificate No. : 25TH0226

CSR No. : A101/05028

Page. : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Kamchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Customer Laboratory
Instrument Name : Incubator
Manufacturer : Memmert
Model : ICP750
Serial No. : F816.0063
ID No. : SGK_CL0028
Resolution : 0.1 °C
Received Date : 10-Jan-2025
Calibrated Date : 10-Jan-2025
Ambient Temperature : (30 ± 10) °C
Relative Humidity : (50 ± 30) %

REVIEW BY Ananta B.
APPROVED BY Kampha H.
NEXT CAL. DATE 10/1/26

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.012 based on GLA - 20

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and/or national standards which realize the units of measurement
according to the International System of Unit (SI) through :

- TISTR : Thailand Institute of Scientific and Technological Research

Calibrated by : Ibrorhim Saleemin

Approved by :

Imron Rattanaylum / Technical Manager



The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Certificate No. : 25TH0226

CSR No. : A101/05028

Page. : 2 of 3

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data Acquisition/Switch Unit	34970A	MY58009813	PSL-T0707-1/67	22-May-2025

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration
and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction


4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration :

(✓) Without Adjustment

() After Adjustment

1. Sensor Installation Diagram

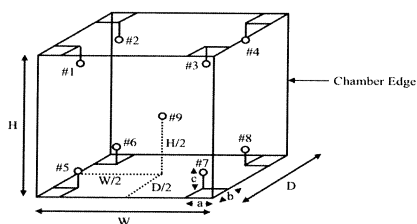

Sensor Installation Details

a = 5.0 cm
b = 5.0 cm
c = 5.0 cm

Dimension of the chamber

W = 104.0 cm
H = 120.0 cm
D = 60.0 cm

CARIBRATION CERTIFICATE

Issued Date : 27-Feb-2026

Certificate No. : 26CH0116

CSR No. : A240/11995

Page. : 1 of 2

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Kamchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : SCaL Laboratory
Instrument Name : DO meter
Manufacturer : YSI
Model : 4010-1W
Serial No. : 24200618
ID No. : SGK_CL0101
Receipt Date : 20-Feb-2026
Calibration Date : 24-Feb-2026
Ambient Temperature : (25 ± 3) °C
Relative Humidity : (55 ± 15) %

REVIEW BY Kampha H.
APPROVED BY Kampha H.
NEXT CAL. DATE 24/2/27

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.062 based on direct measurement by
using certified reference Material (CRM)

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and/or national standards which realize the units of measurement
according to the International System of Unit (SI) through :

- HANNA : Hanna Instruments.

Calibrated by : Alisara Ma

Approved by :

Sakeereen Heemhad / Laboratory Manager



The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Zero Oxygen Solution	HI7040L	C02374	S0032/21	12-Apr-2026

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.
3. This certificate is not certified any commercial transaction
4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration : (✓) Without Adjustment () After Adjustment

Sample Test Measurement

Serial Probe No. : 24F102419

Standard Buffer Solutions	UUC Reading	Correction	Uncertainty (±)
8.26 mg/L	8.26 mg/L	0.00 mg/L	0.16 mg/L

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95%

... End ...

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Digital Thermometer With Sensor (PRT)	1529	B4C223	QR25-2862	25-Sep-2026

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.
3. This certificate is not certified any commercial transaction
4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration : (✓) Without Adjustment () After Adjustment

Sensor Type : RTD Channel : OUT Serial Probe No. : 24F102419

Length : 6.8 cm. Diameter : 0.2 cm. Immersion : 6.8 cm.

Cal Point (°C)	Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
20	20.007	20.2	-0.193	0.077

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95%

...End...

Southern Calibration Service Co., Ltd.

669/35 Kanjanavanit Rd., Banpru, Hatyai, Songkhla 90250 Thailand
Tel : 08 1599 0417 Fax : 0 7480 5133 Email : s.calibration@gmail.com www.sca.co.th



CALIBRATION CERTIFICATE

Issued Date : 27-Feb-2026


Certificate No. : 26TH0817

CSR No. : A240/11995

Page. : 1 of 2

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Kamchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : SCaL Laboratory
Instrument Name : DO Meter with probe
Manufacturer : YSI
Model : 4010-1W
Serial No. : 24200618
ID No. : SGK_CL0101
Resolution : 0.1 °C
Received Date : 20-Feb-2026
Calibrated Date : 24-Feb-2026
Ambient Temperature : (25 ± 3) °C
Relative Humidity : (55 ± 15) %



Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.011 by comparison technique with standard thermometer

The Southern Calibration Service Co.,Ltd calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- Q Reborn : Quality Reborn Co.,Ltd.

Calibrated by : Iborhim Saleemin

Approved by : 
Sakeereen Heemhad / Laboratory Manager



The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

Certificate of Calibration

Cert. No.: 26TM151
Page.: 1 of 3

Equipment : COD Reactor

Manufacturer : Hach

Model : DRB200

Serial No. : 21120C1313

ID No. : SGK_CL0085

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
(Songkhla Branch)
114/1 Moo 8 Kamchanawanich Rd., T. Ban Phru,
A. Hat Yai, Songkhla 90250 Thailand
Chemistry Lab

Location :

Received Order : 12 January 2026
Calibration Date : 12 January 2026
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %
AC Line Voltage : (220 ± 22) V

Calibrated by : Kunchit Promprat


Approved by :

- () Chakrit Waewwanjua
() Ponpan Paipim
(✓) Suwit Imjai

Issue Date : 23 January 2026

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Calibration and Testing Equipment Services.




Approved Signatory



Equipment : COD Reactor
Condition As-Received : Used Item
Reference : 2601-0210OC-1
Procedure Used :-

Cert. No.: 26TM151
Page.: 2 of 3

As agreed with customer the calibration was performed using in-house calibration method according to directed measurement method with Data Acquisition which connected with Thermocouple Type T.
The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY49023932	25LM121	TPA	27 Jul 2026

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This measurement result is traceable to the International System of Unit maintained through :

Remark : TPA : Technology Promotion Association (Thailand-Japan), NSC-ONSC Accredited No. Calibration 0008

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Heat transfer medium used : Alumina Calcined

Environment during calibration			Left		Right	
	Beginning	Finished	Position	ID No. of Sensor	Position	ID No. of Sensor
Temp.(°C)	25	24	L1	25-16TC-03	R1	-
REL.Humi.(%)	50	54	L2	25-16TC-02	R2	-
AC Supply (Volt)	223	224	L3	25-16TC-03	R3	-

L13L14L15

L10L11L12

L7L8L9

L4L5L6

L1L2L3

R13R14R15

R10R11R12

R7R8R9

R4R5R6

R1R2R3

LeftRight

Display

Top View



Equipment : COD Reactor
Condition As-Received : Used Item
Reference : 2601-0210OC-1
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Calibration Point : 150 °C

Cert. No.: 26TM151
Page.: 3 of 3

UUC* Setting (°C)	UUC* Reading (°C)	Measured Temperature (°C)						Temperature stability (± °C)	Uncertainty (± °C)	Coverage Factor k	
		Position									
		Left			Right						
Left	151	L13	L14	L15	R13	R14	R15	Left	0.076	1.1	2
		147.709	147.893	147.802	-	-	-				
		L10	L11	L12	R10	R11	R12				
		148.176	148.485	148.084	-	-	-				
		L7	L8	L9	R7	R8	R9				
Right	-	149.766	149.205	149.819	-	-	-	Right	-	-	-
		L4	L5	L6	R4	R5	R6				
		149.648	150.341	149.867	-	-	-				
		L1	L2	L3	R1	R2	R3				
		149.759	149.691	149.642	-	-	-				

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-000-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert.No.: 26CHO12
Page.: 1 of 3

Equipment : Spectrophotometer
Manufacturer : Hach
Model : DR 3900
Serial No. : 2403637
ID No. : SGK_CL0100
Condition As-Received : Used Item
Received Date : 12 January 2026
Calibration Date : 12 January 2026
Reference : 2601-0210OC-3
Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.,
Songkhla Branch,
114/1 Moo 8, Kamchanawanich Rd., T.Ban Phru,
A.Hat Yai, Songkhla 90250, Thailand

Calibration Place : Chemistry Room
Ambient Temperature : (25.2 to 24.4) °C (On-Site)
Relative Humidity : (50.7 to 55.2) % (On-Site)
Calibration Procedure : In - house method :
CP-0CH4 based on ASTM E 275-08

Calibrated by : Kunchit Promprat
Approved by :
Approved Signatory

(✓) Chakrit Waewwanjua
() Ponpan Paipim
() Saithip Meangmai

Issue Date : 21 January 2026

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Cert. No.: 26CHO12
Page : 2 of 3

Condition of calibration result

1. Reference Standard Material :

Material	Serial No.	Certificate No.	Due date
1. Absorbance Standard set	44487	122584	31 May 2026
2. Wavelength Standard set	36730	118120	15 Jan 2026
3. Wavelength Standard set	36730	118121	15 Jan 2026

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certificate is traceable to the International System of Unit maintained through :
- Starna Scientific Ltd.

4. Spectral BandWidth : 5 nm
Scan Speed : - nm/min

Calibration Results : without adjustment

Wavelength Accuracy

Certified Values of Reference Material (nm)	UUC Reading (nm)	Uncertainty of Measurement (± nm)	Coverage Factor k
418.40	418	0.59	2.00
479.88	480	0.59	2.00
513.75	514	0.59	2.00
537.00	537	0.59	2.00
638.00	638	0.59	2.00
684.70	685	0.59	2.00
747.61	748	0.59	2.00
807.04	807	0.59	2.00



Cert. No. : 26CHO12
Page : 3 of 3

Calibration Results : without adjustment

Photometric Accuracy

Wavelength (nm)	Certified Values of Reference Material (Abs)	UUC Reading (Abs)	Uncertainty of Measurement (±Abs)	Coverage Factor k
420.0	Zero	0.000	0.0028	2.00
	0.5750	0.573	0.0028	2.00
	0.7156	0.714	0.0028	2.00
	1.0176	1.016	0.0028	2.00
440.0	Zero	0.000	0.0028	2.00
	0.5598	0.557	0.0028	2.00
	0.7037	0.700	0.0028	2.00
	1.0013	0.997	0.0028	2.00
465.0	Zero	0.000	0.0028	2.00
	0.5222	0.521	0.0028	2.00
	0.6646	0.664	0.0028	2.00
	0.9444	0.944	0.0028	2.00
546.1	Zero	0.000	0.0028	2.00
	0.5234	0.522	0.0028	2.00
	0.7007	0.700	0.0028	2.00
	0.9992	0.999	0.0028	2.00
590.0	Zero	0.000	0.0028	2.00
	0.5573	0.554	0.0028	2.00
	0.7760	0.772	0.0028	2.00
	1.1104	1.105	0.0028	2.00
635.0	Zero	0.000	0.0028	2.00
	0.5648	0.563	0.0028	2.00
	0.7654	0.763	0.0028	2.00
	1.0961	1.094	0.0028	2.00

Remark

- Each individual filter is measured against the empty filter holder (blank) used to zero the spectrophotometer
- UUC = Unit Under Calibration
- The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-000-



Cert. No. : 26CHO11
Page : 2 of 4

Condition of calibration result

1. Reference Standard Material :

Material	Serial No.	Certificate No.	Due date
1. Absorbance Standard set	42525	137241	19 Nov 2027
2. Absorbance Standard set	44487	122584	31 May 2026
3. Wavelength Standard set	36730	118120	15 Jan 2026
4. Wavelength Standard set	36730	118121	15 Jan 2026

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certificate is traceable to the International System of Unit maintained through :
- Sarna Scientific Ltd.

4. Spectral Bandwidth : 1.5 nm
Scan Speed : 40 nm/min

Calibration Results : without adjustment

Wavelength Accuracy

Certified Values of Reference Material (nm)	UUC Reading (nm)	Uncertainty of Measurement (± nm)	Coverage Factor k
241.72	240.9	0.13	2.00
334.06	333.4	0.13	2.00
418.59	418.2	0.13	2.00
573.17	573.3	0.13	2.00
879.28	879.2	0.16	2.05



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert.No.: 26CHO11
Page.: 1 of 4

Equipment : UV-VIS Spectrophotometer
Manufacturer : Agilent
Model : Cary 60 UV-VIS
Serial No. : MY16510028
ID No. : SGK_CL0040
Condition As-Received: Used Item
Received Date : 12 January 2026
Calibration Date : 13 January 2026
Reference : 2601-02100C-2
Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
Songkhla Branch.
114/1 Moo 8, Kamchanawanich Rd., T.Ban Phru,
A.Hat Yai, Songkhla 90250, Thailand
Chemistry Lab
Calibration Place :
Ambient Temperature : (25.5 to 26.1) °C (On-Site)
Relative Humidity : (56.9 to 55.8) % (On-Site)
Calibration Procedure : In - house method :
CP-OCH4 based on ASTM E 275-08
Calibrated by : Kunchit Promprat
Approved by :
(✓) Chakrit Waewwanjua
() Ponpan Paipim
() Saithip Meangmai
Issue Date : 21 January 2026

REVIEW BY: Chandanan M.
APPROVED BY: Kanitta H.
NEXT CAL DATE: 13/01/27

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.



Cert. No. : 26CHO11
Page : 3 of 4

Calibration Results : without adjustment

Photometric Accuracy

Wavelength (nm)	Certified Values of Reference Material (Abs)	UUC Reading (Abs)	Uncertainty of Measurement (±Abs)	Coverage Factor k
235.0	Zero	-0.0001	0.0046	2.00
	0.4940	0.4929	0.0095	2.00
	0.7388	0.7375	0.0050	2.00
257.0	Zero	0.0001	0.0046	2.00
	0.5729	0.5709	0.0076	2.00
	0.8598	0.8576	0.0050	2.00
313.0	Zero	0.0001	0.0046	2.00
	0.1924	0.1928	0.0062	2.00
	0.2875	0.2880	0.0050	2.00
350.0	Zero	0.0000	0.0046	2.00
	0.4263	0.4250	0.0061	2.00
	0.6386	0.6362	0.0050	2.00
420.0	Zero	0.0000	0.0028	2.00
	0.5750	0.5729	0.0028	2.00
	0.7156	0.7145	0.0028	2.00
	1.0176	1.0153	0.0028	2.00
440.0	Zero	0.0000	0.0028	2.00
	0.5598	0.5578	0.0028	2.00
	0.7037	0.7028	0.0028	2.00
	1.0013	0.9997	0.0028	2.00

Remark

- Each individual filter is measured against the empty filter holder (blank) used to zero the spectrophotometer
- The Potassium Dichromate filled cells are measured against a Perchloric acid blank.
- UUC = Unit Under Calibration



Cert. No. : 26CHO11
Page : 4 of 4

Calibration Results : without adjustment

Photometric Accuracy

Wavelength (nm)	Certified Values of Reference Material (Abs)	UUC Reading (Abs)	Uncertainty of Measurement (±Abs)	Coverage Factor k
465.0	Zero	0.0000	0.0028	2.00
	0.5222	0.5206	0.0028	2.00
	0.6646	0.6641	0.0028	2.00
	0.9444	0.9434	0.0028	2.00
546.1	Zero	0.0000	0.0028	2.00
	0.5234	0.5215	0.0028	2.00
	0.7007	0.6993	0.0028	2.00
	0.9992	0.9970	0.0028	2.00
590.0	Zero	0.0000	0.0028	2.00
	0.5573	0.5553	0.0028	2.00
	0.7760	0.7742	0.0028	2.00
	1.1104	1.1074	0.0028	2.00
635.0	Zero	0.0000	0.0028	2.00
	0.5648	0.5634	0.0028	2.00
	0.7654	0.7643	0.0028	2.00
	1.0961	1.0939	0.0028	2.00

Remark

- Each individual filter is measured against the empty filter holder (blank) used to zero the spectrophotometer
- UUC = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-00-



Certificate No. : 25MA2641
CSR No. : A230/11462
Page : 2 of 3

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Standard Weight Set	2mg to 1kg	11119514/01	25SWS001	2-Jul-2026

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction

4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration : [✓] Without Adjustment [] After Adjustment

1. Repeatability


Nominal Value (g)	Standard Deviation (g)
20	0.00000
200	0.00000

2. Off-center loading

A mass approximately 100g was placed on a pan and moved to various position .

The balance reading obtained are given in the table.

Position					Maximum Error from Center (g)
1	2	3	4	5	
100.0000	100.0001	100.0000	100.0001	100.0000	0.0001



3. Effect of tare

Nominal Value (g)	Standard Value (g)	Balance Reading (g)	UUC Error (g)
20	19.9999	20.0000	0.0001
40	39.9999	40.0000	0.0001
60	60.0001	60.0000	-0.0001
80	80.0000	80.0001	0.0001
100	100.0000	100.0000	0.0000

SCAL.F0.018/6010723



Southern Calibration Service Co., Ltd.

669/35 Kanjanavanit Rd., Banpru, Hatyai, Songkhla 90250 Thailand
Tel: 08 1599 0417 Fax: 0 7480 5133 Email: s.calibration@gmail.com www.scal.co.th



CALIBRATION CERTIFICATE

Issued Date : 18-Dec-2025

Certificate No. : 25MA2641

CSR No. : A230/11462

Page : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Kamchanawanikh Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Chemical Laboratory

Instrument Name : Electronic Balance

Manufacturer : Sartorius

Model : MSE224S-100-DU

Serial No. : 34705158

ID No. : SGK_CL0045


Resolution : 0.0001 g

Received Date : 15-Dec-2025

Calibrated Date : 15-Dec-2025

Ambient Temperature : (30 ± 10) °C

Relative Humidity : (50 ± 20) %



Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.001 based on UKAS LAB 14 : 2022

The Southern Calibration Service Co., Ltd. calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement

according to the International System of Unit (SI) through :

- SCaL : Southern Calibration Service Co., Ltd.,

Calibrated by : Hadbordee Dettawee

Approved by :

Innon Rattanayum / Technical Manager

SCAL.F0.018/6010723



The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.



Certificate No. : 25MA2641
CSR No. : A230/11462
Page : 3 of 3

Result of Calibration : cont.

4. Departure from nominal value

Nominal Value (g)	Standard Value (g)	UUC Reading (g)	Correction (g)	Uncertainty (±g)	Coverage Factor (k)
0	0.0000	0.0000	0.0000	0.00008	2.0
0.01	0.0100	0.0100	0.0000	0.00008	2.0
0.1	0.1000	0.1000	0.0000	0.00008	2.0
0.5	0.5000	0.5000	0.0000	0.00008	2.0
1	1.0000	1.0000	0.0000	0.00008	2.0
2	2.0000	2.0000	0.0000	0.00008	2.0
5	5.0000	5.0000	0.0000	0.00009	2.0
10	10.0000	10.0000	0.0000	0.00009	2.0
20	19.9999	20.0000	-0.0001	0.00009	2.0
40	39.9999	40.0000	-0.0001	0.00012	2.0
60	60.0001	60.0000	0.0001	0.00013	2.0
80	80.0000	80.0000	0.0000	0.00017	2.0
100	100.0000	100.0000	0.0000	0.00016	2.0
120	119.9999	120.0000	-0.0001	0.00024	2.0
140	139.9999	140.0001	-0.0002	0.00024	2.0
160	160.0001	160.0001	0.0000	0.00026	2.0
180	180.0000	180.0001	-0.0001	0.00030	2.0
200	199.9998	200.0000	-0.0002	0.00029	2.0

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95%

...End...

SCAL.F0.018/6010723

CALIBRATION CERTIFICATE

Issued Date : 3-Apr-2026


Certificate No. : 26TH1563

CSR No. : A247/12304

Page : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Kamchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Customer Laboratory
Instrument Name : Hot Air Oven
Manufacturer : Memmert
Model : UF110
Serial No. : B416.3387
ID No. : SGK_CL0024
Resolution : 0.1 °C
Received Date : 31-Mar-2026
Calibrated Date : 31-Mar-2026
Ambient Temperature : (30 ± 10) °C
Relative Humidity : (50 ± 30) %



Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.012 based on GLA - 20

The Southern Calibration Service Co., Ltd. calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- Q Reborn : Quality Reborn Co., Ltd.

Calibrated by : Ibrorhim Saleemin

Approved by :

Aisara Ma / Supervisor Manager

SCAL.FO.018/010723



The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Result of Calibration :

2. Temperature Measurement Accuracy Test

The measurement results of the Hot Air Oven and associates are reported in the manner as shown below

Cal point (°C)	Measured Standard Temperature At Spread Locations (°C)									Uncertainty (±°C)
	#1	#2	#3	#4	#5	#6	#7	#8	Ref. 9	
40	40.52	40.44	40.53	40.53	40.53	40.46	40.59	40.54	40.44	0.38
70	70.81	70.87	71.28	70.87	70.18	70.96	70.24	70.47	70.09	0.44
103	103.36	103.37	103.49	103.42	102.74	103.02	103.47	102.92	102.96	0.39
104	104.06	104.09	104.50	104.14	103.50	104.15	104.47	103.84	103.84	0.42
105	105.20	105.22	105.54	105.41	105.36	105.22	105.31	105.01	105.09	0.38
180	180.78	180.86	180.98	180.98	179.46	179.33	179.32	179.41	179.42	0.55

3. Temperature Performance Result

The performance of the Hot Air Oven are reported as shown below

UUC Setting (°C)	UUC Reading (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
40.0	40.0	0.10	0.33	0.33
70.0	70.0	0.05	1.17	1.17
103.0	103.0	0.10	0.72	0.94
104.0	104.0	0.15	0.95	1.27
105.0	105.0	0.10	0.63	0.77
180.0	180.0	0.25	1.73	1.85

UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95%

... End ...

SCAL.FO.018/010723

Certificate No. : 26TH1563

CSR No. : A247/12304

Page : 2 of 3

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data Acquisition Switch Unit with Sensor	DAQ970A	MY58036254	QR25-2036	1-Jul-2026


2. The results reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction

4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration : ☒ Without Adjustment ☐ After Adjustment

1. Sensor Installation Diagram

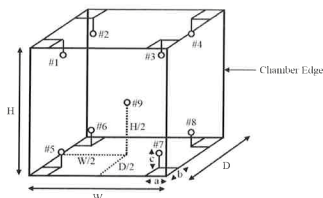

Sensor Installation Details

Dimension of the chamber

a = 5.0 cm	W = 40.0 cm
b = 5.0 cm	H = 40.0 cm
c = 5.0 cm	D = 33.0 cm