

ภาคผนวกที่ 4

เอกสารสอบเทียบความถูกต้องของเครื่องมือตรวจวัดคุณภาพสิ่งแวดล้อม

- | | |
|------------|---------------------------|
| ลำดับที่ 1 | คุณภาพอากาศในบรรยากาศ |
| ลำดับที่ 2 | คุณภาพอากาศจากแหล่งกำเนิด |
| ลำดับที่ 3 | ระดับเสียง |
| ลำดับที่ 4 | คุณภาพน้ำ |
| ลำดับที่ 5 | คุณภาพอากาศในการทำงาน |
| ลำดับที่ 6 | ระดับความร้อนในการทำงาน |

**ตารางสรุปรายการเอกสารการสอบเทียบความถูกต้องของเครื่องมือเก็บตัวอย่าง
และเครื่องมือตรวจวิเคราะห์คุณภาพสิ่งแวดล้อม (ระยะดำเนินการ)**

รายการตรวจวัด	เครื่องมือเก็บตัวอย่าง	เครื่องมือตรวจวิเคราะห์
	ชื่อเครื่องมือ	ชื่อเครื่องมือ
1. คุณภาพอากาศในบรรยากาศ		
Total Suspended Particulate (TSP)	High Volume Air Sampler Rec No.Blow No. R10, R11	Digital Balance
Particulate Matter less than 10 microns (PM-10)	High Volume PM-10 Air Sampler Rec No.Blow No. R03, R06	Digital Balance
Nitrogen Dioxide (NO _x)	NO/NO ₂ /NO _x Analyzer No. R06, R11	NO/NO ₂ /NO _x Analyzer No. R06, R11
2. คุณภาพอากาศจากแหล่งกำเนิด		
Total Suspended Particulate (TSP)	Console No. B05 Pitot Tube No. B45	Digital Balance
Oxides of Nitrogen (NO _x)	Vacuum Gauge	Spectrophotometer
3. ระดับเสียง		
L _{eq} 24 hr, L ₉₀ , L _{max} และ L _{dn}	Acoustic Calibrator Sound Level Meter No. ACO-B03, B05, B19, B41, B43, R40, R55	-
L _{eq} 1 hr, L _{eq} 8 hr และ Noise Dose	Acoustic Calibrator Sound Level Meter NMD No. R02, R03, R35	-
4. คุณภาพน้ำ		
pH	-	pH Meter
Total Dissolved Solids (TDS)	-	Digital Balance
Total Suspended Solids (TSS)	-	Digital Balance
Biochemical Oxygen Demand (BOD ₅)	-	BOD Analyzer
Chemical Oxygen Demand (COD)	-	COD Reactor
Grease & Oil	-	Digital Balance
Temperature	-	Thermometer
Lead (Pb)	-	Atomic Absorption Spectrophotometer
Aluminium (Al)	-	ICP
5. คุณภาพอากาศในสถานที่ทำงาน		
Total Dust	Personal Pump SKC No. B34, R02 Rotameter No. H-R1	Digital Balance
Respirable Dust	Personal Pump SKC No. R07 Rotameter No. H-R1	Digital Balance
Aluminum	Personal Pump SKC No. R20, R25 Rotameter No. H-R1	ICP

ตารางสรุปรายการเอกสารการสอบเทียบความถูกต้องของเครื่องมือเก็บตัวอย่าง
และเครื่องมือตรวจวิเคราะห์คุณภาพสิ่งแวดล้อม (ระยะดำเนินการ) (ต่อ)

รายการตรวจวัด	เครื่องมือเก็บตัวอย่าง	เครื่องมือตรวจวิเคราะห์
	ชื่อเครื่องมือ	ชื่อเครื่องมือ
5. คุณภาพอากาศในสถานที่ทำงาน (ต่อ) Hydrogen Fluoride	Personal Pump SKC No. R20 Rotameter No. L-R1	Ion Chromatography
Oil Mist	Personal Pump SKC No. R27 Rotameter No. H-R1	Ion Chromatography
6. ระดับความร้อนในการทำงาน WBGT	Heat Stress WBGT Meter No. R08, R09, R12	-

คุณภาพอากาศในบรรยากาศ



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร กรุงเทพมหานคร 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompet, Chulachak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sales@spscn.com, www.spscn.com

High Volume Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard Model : TE 5025A S/N : 3611

Calibration Data

High Volume Air Sampler Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (ft ³ /min)	R ²
B35	B35	06/05/2026	y = 1.130x-2.698	0.999
B36	B36	05/05/2026	y = 1.112x-2.644	0.998
B37	B37	05/05/2026	y = 1.124x-2.608	0.996
B38	B38	06/05/2026	y = 1.139x-1.817	0.999
B39	B39	05/05/2026	y = 1.099x+0.749	0.997
B40	B40	05/05/2026	y = 1.135x-2.517	0.997
B41	B41	06/05/2026	y = 1.103x-0.803	0.998
B42	B42	05/05/2026	y = 1.138x-3.754	0.999
B43	B43	06/05/2026	y = 1.132x-2.425	0.997
B44	B44	06/05/2026	y = 1.128x-2.443	0.998
R01	R01	07/05/2026	y = 1.103x-2.879	0.997
R02	R02	02/05/2026	y = 1.130x-2.934	0.997
R03	R03	05/05/2026	y = 1.124x-2.685	0.996
R04	R04	05/05/2026	y = 1.114x-0.914	0.998
R05	R05	06/05/2026	y = 1.059x+0.368	0.998
R06	R06	06/05/2026	y = 1.088x+0.020	0.996
R07	R07	06/05/2026	y = 1.122x-2.809	0.996
R08	R08	05/05/2026	y = 1.101x-1.418	0.999
R09	R09	05/05/2026	y = 1.084x+0.212	0.997
R10	R10	05/05/2026	y = 1.104x-2.080	0.998
R11	R11	06/05/2026	y = 1.112x-2.545	0.999
R12	R12	05/05/2026	y = 1.119x-0.906	0.997
R13	R13	05/05/2026	y = 1.116x-3.391	0.997
R14	R14	02/05/2026	y = 1.080x-1.101	0.996
R15	R15	06/05/2026	y = 1.095x-0.708	0.998
R16	R16	02/05/2026	y = 1.104x-1.452	0.997
R17	R17	06/05/2026	y = 1.102x-1.932	0.998
R18	R18	02/05/2026	y = 1.128x-4.180	0.997
R19	R19	02/05/2026	y = 1.090x-3.037	0.996
R20	R20	06/05/2026	y = 1.130x-2.859	0.999

Calibrated by :

Approved by :



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร กรุงเทพมหานคร 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompet, Chulachak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sales@spscn.com, www.spscn.com

High Volume PM-10 Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard Model : TE 5025A S/N : 3611

Calibration Data

High Volume PM-10 Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (ft ³ /min)	R ²
R01	R01	06/05/2026	y = 1.023x+2.784	0.996
R02	R02	06/05/2026	y = 1.060x+0.840	0.997
R03	R03	06/05/2026	y = 1.086x-1.550	0.998
R04	R04	05/05/2026	y = 1.117x-3.501	0.999
R05	R05	06/05/2026	y = 1.075x-1.953	0.997
R06	R06	06/05/2026	y = 1.113x-2.377	0.996
R07	R07	06/05/2026	y = 1.104x-1.898	0.997
R08	R08	05/05/2026	y = 1.119x-2.379	0.998
R09	R09	05/05/2026	y = 1.044x+0.730	0.998
R10	R10	06/05/2026	y = 1.103x-2.555	0.997
R11	R11	05/05/2026	y = 1.021x+2.220	0.998
R12	R12	06/05/2026	y = 1.033x+1.005	0.999
R13	R13	06/05/2026	y = 1.112x-3.260	0.997
R14	R14	06/05/2026	y = 1.074x-2.039	0.999
R15	R15	06/05/2026	y = 1.093x-1.992	0.996
R16	R16	06/05/2026	y = 1.113x-2.436	0.997
R17	R17	06/05/2026	y = 1.086x-1.693	0.998
R18	R18	05/05/2026	y = 1.100x-4.540	0.999
R19	R19	05/05/2026	y = 1.067x+1.116	0.997
R20	R20	05/05/2026	y = 1.077x-1.807	0.999

Calibrated by :

Approved by :



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT					
NO / NO ₂ / NO _x ANALYZER					
DATE :	09 June 2026	BRAND :	API	MODEL :	200E
NO.	NOX-R06	SERIAL NO.	4466		
Calibrator (Dilution System)					
Brand	: API		Model	: 700	
Last Cal. Date	: 01 September 2025		Serial No.	: 911	
Reference Standard Gas					
Standard Gas	: Nitric Oxide (NO)		Cylinder No.	: A00674SV	
Certified Date	: 12 March 2025	Expired Date	: 12 March 2028	Cylinder Conc.	: 48.7 ppm
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.6	°C
			% RH	50	
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	
Zero	0	-0.10	-	0	
NO Span	400	399.5	-0.125	400.0	
NO _x Span	400	400.0	0.000	400.0	

Calibrated by :



Approved by :



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT					
NO / NO ₂ / NO _x ANALYZER					
DATE :	09 June 2026	BRAND :	API	MODEL :	200E
NO.	NOX-R11	SERIAL NO.	2621		
Calibrator (Dilution System)					
Brand	: API		Model	: 700	
Last Cal. Date	: 01 September 2025		Serial No.	: 911	
Reference Standard Gas					
Standard Gas	: Nitric Oxide (NO)		Cylinder No.	: A00674SV	
Certified Date	: 12 March 2025	Expired Date	: 12 March 2028	Cylinder Conc.	: 48.7 ppm
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.6	°C
			% RH	50	
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	
Zero	0	-0.10	-	0	
NO Span	400	399.9	-0.025	400.0	
NO _x Span	400	400.2	0.050	400.0	

Calibrated by :



Approved by :





CERTIFICATE No : 26M2266
REFERENCE No : 80204-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE
MANUFACTURER : METTLER TOLEDO
MODEL : XS105DU
SERIAL No : 1126422905
ID No : BA 05/50
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : SUCHAT S.
CALIBRATION DATE : 05-Mar-26

APPROVED BY : 
ISSUED DATE : 06-Mar-26
RECEIVED DATE : 05-Mar-26



CERTIFICATE No : 26M2266

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE
MANUFACTURER : METTLER TOLEDO
ID No : BA 05/50
AIR PRESSURE : 1004mbar $\pm$ 1mbar
AMBIENT TEMPERATURE : 25° C $\pm$ 1° C
MODEL : XS105DU
S/N : 1126422905
RECEIVED DATE : 05-Mar-26
CALIBRATION DATE : 05-Mar-26
RELATIVE HUMIDITY : 50 %RH $\pm$ 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	C02250116	28-Jan-27
2) STANDARD WEIGHT	E2	15843	C02250117	29-Jan-27

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.


5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
- NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL
2. TARE FUNCTION : NORMAL
3. REPEATABILITY OF READING AT 120 g WAS 0.000055 g
4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ($\pm$ g)
0.00	0.00000	0.00000	0.000065
0.02	0.02000	0.00000	0.000065
0.10	0.10000	0.00000	0.000066
0.20	0.20000	0.00000	0.000066
0.50	0.50001	-0.00001	0.000065
1.00	1.00001	-0.00001	0.000066
2.00	2.00000	0.00000	0.000067
5.00	5.00001	-0.00001	0.000068
10.00	10.00004	-0.00004	0.000070
20.00	20.00006	-0.00006	0.000078
50.00	50.00000	0.00000	0.00012
100.00	100.00002	-0.00002	0.00019
120.00	120.00002	-0.00002	0.00022

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.0000
2	50.0000
3	50.0000
4	50.0000
5	50.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A
COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



คุณภาพอากาศจากแหล่งกำเนิด



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com, www.spscon.com

Console Calibration Report

Calibration Method

Critical Orifices

Calibration Data

Console Data

Calibration Data

No.	Serial No.	Date	y	ΔH_{g} (mmH ₂ O)
B01	1563	03/06/2026	0.999	49.74
B02	8002514	02/06/2026	1.004	49.63
B03	1503016	03/06/2026	0.998	49.52
B04	00006659	01/06/2026	0.997	49.68
B05	00007428	01/06/2026	1.002	49.50
R01	1561	02/06/2026	1.004	49.81
R02	8002513	02/06/2026	1.003	49.45
R03	1570	04/06/2026	0.998	49.67
R04	8002519	04/06/2026	0.997	49.76
R05	1503015	01/06/2026	1.002	49.88

Remark : Accept Value of y (test) is $0.97 < y < 1.03$

Accept Value of ΔH_{g} (test) is 46.7 ± 6.4 (mmH₂O)

Calibrated by :

Approved by :



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com, www.spscon.com

High Volume Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard

Model : TE 5025A

S/N : 3611

Calibration Data

High Volume Air Sampler Data

Calibration Data

Recorder No.	Blower No.	Date	Actual Flowrate (ft ³ /min)	R ²
B35	B35	06/05/2026	y = 1.130x-2.698	0.999
B36	B36	05/05/2026	y = 1.112x-2.644	0.998
B37	B37	05/05/2026	y = 1.124x-2.608	0.996
B38	B38	06/05/2026	y = 1.139x-1.817	0.999
B39	B39	05/05/2026	y = 1.099x+0.749	0.997
B40	B40	05/05/2026	y = 1.135x-2.517	0.997
B41	B41	06/05/2026	y = 1.103x-0.803	0.998
B42	B42	05/05/2026	y = 1.138x-3.754	0.999
B43	B43	06/05/2026	y = 1.132x-2.425	0.997
B44	B44	06/05/2026	y = 1.128x-2.443	0.998
R01	R01	07/05/2026	y = 1.103x-2.879	0.997
R02	R02	02/05/2026	y = 1.130x-2.934	0.997
R03	R03	05/05/2026	y = 1.124x-2.685	0.996
R04	R04	05/05/2026	y = 1.114x-0.914	0.998
R05	R05	06/05/2026	y = 1.059x+0.368	0.998
R06	R06	06/05/2026	y = 1.088x+0.020	0.996
R07	R07	06/05/2026	y = 1.122x-2.809	0.996
R08	R08	05/05/2026	y = 1.101x-1.418	0.999
R09	R09	05/05/2026	y = 1.084x+0.212	0.997
R10	R10	05/05/2026	y = 1.104x-2.080	0.998
R11	R11	06/05/2026	y = 1.112x-2.545	0.999
R12	R12	05/05/2026	y = 1.119x-0.906	0.997
R13	R13	05/05/2026	y = 1.116x-3.391	0.997
R14	R14	02/05/2026	y = 1.080x-1.101	0.996
R15	R15	06/05/2026	y = 1.095x-0.708	0.998
R16	R16	02/05/2026	y = 1.104x-1.452	0.997
R17	R17	06/05/2026	y = 1.102x-1.932	0.998
R18	R18	02/05/2026	y = 1.128x-4.180	0.997
R19	R19	02/05/2026	y = 1.090x-3.037	0.996
R20	R20	06/05/2026	y = 1.130x-2.859	0.999


Calibrated by :

Approved by :



CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE	VACUUM GAUGE
MANUFACTURER	HI-LIGHT
MODEL/TYPE	N/A
SERIAL NO.	N/A [64-220088-1]
CLID.NO.	212301422
JOB CONTROL NO.	240720076546

CUSTOMER S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24 ROAD., JOMPOL,
CHATUCHAK, BANGKOK 10900

DATE OF RECEIVED : 19 July 2025

DATE OF ISSUED: 24 July 2025

The report or calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sittipong Pimdee
Calibration Engineer

Approved By : Mongkol Yotsoontorn
Authorized Signatory
24 July 2025



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q24076546


F3-011-05/12-23

page 1 of 3



CALIBRATION LABORATORY Co., LTD.

211Q-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



REPORT OF CALIBRATION

FOR

NOMENCLATURE	VACUUM GAUGE
MANUFACTURER	HI-LIGHT
MODEL/TYPE	N/A
SERIAL NO.	N/A [64-220088-1]
DATE OF CALIBRATION	23 July 2025
DUE DATE OF CALIBRATION	23 July 2026

ENVIRONMENT CONDITIONS

Temperature : $(23 \pm 2)^{\circ}\text{C}$

Relative Humidity $(55 \pm 10) \% \text{RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. CLC-CPPP-05 according to DKD-R 6-1 as calibration guidelines.

The calibration was performed by direct measurement with Document Process Calibrator and Pressure Module which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

Document Process Calibrator, Fluke Model 74 1B S/N. 8295020 with Pressure Module Model 700PD5 S/N. 89404505.

TRACEABILITY :

The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand).
Certificate No: MP-0040-24.

UNCERTAINTY :

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor of $k=2$. It has been evaluated according to the "Calibration of Pressure Gauges (DKD-R 6-1)" which provides a level of confidence approximately 95%.

Certificate No. Q24076546

F3-011-05/12-23

page 2 of 3



CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax:02-578-2672 www.caLaboratory.com Email:sale@cal-laboratory.com



CONDITION OF CALIBRATION ITEM :RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS: (X) without adjustment () adjustment

The DUC was exercised by applying a known pressure from its zero to full scale 1 times, Then 2 series of known gauge pressure were applied. The STD reading were recorded and the means value were reported in the table below:

CALIBRATION DATA

CORRECTION OF PRESSURE

DUC Test point (inHg)	STD Reading (kPa)		Conversion to inHg		Correction (inHg)	
	Up	Down	Up	Down	Up	Down
0	0.00	0.00	0.0	0.0	0.0	0.0
-5	-15.07	-15.10	-4.5	-4.5	+0.5	+0.5
-10	-32.50	-32.84	-9.6	-9.7	+0.4	+0.3
-15	-49.44	-49.77	-14.6	-14.7	+0.4	+0.3
-20	-66.70	-66.70	-19.7	-19.7	+0.3	+0.3
-25	-83.63	-83.97	-24.7	-24.8	+0.3	+0.2
-30	-100.39	-100.39	-29.6	-29.6	+0.4	+0.4

Uncertainty of measurement± 0.2 inHg

Transmitting fluid : Air.

Technical Note. Conversion factor 1 kPa ; 0.2953003 inHg

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 012 Page 43 of 67

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q24076546

F3-011-05/ 12-23

page 3 of 3



QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkac, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com



CERTIFICATE No : 26M2266

REFERENCE No : 80204-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE
MANUFACTURER : METTLER TOLEDO
MODEL : XS105DU
SERIAL No : 1126422905
ID No : BA 05/50
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : SUCHAT S.

CALIBRATION DATE : 05-Mar-26

APPROVED BY :

ISSUED DATE : 06-Mar-26

RECEIVED DATE : 05-Mar-26

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.



F-G010 REV 03



QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkoe, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com

CERTIFICATE No : 26M2266

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE
MANUFACTURER : METTLER TOLEDO
ID No : BA 05/50
AIR PRESSURE : 1004mbar $\pm$ 1mbar
AMBIENT TEMPERATURE : 25° C $\pm$ 1° C
MODEL : XS105DU
S/N : 1126422905
RECEIVED DATE : 05-Mar-26
CALIBRATION DATE : 05-Mar-26
RELATIVE HUMIDITY : 50 %RH $\pm$ 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	OK-I-151	C02250116	28-Jan-27
2) STANDARD WEIGHT	E2	15843	C02250117	29-Jan-27

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 120 g WAS 0.000055 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ($\pm$ g)
0.00	0.00000	0.00000	0.000065
0.02	0.02000	0.00000	0.000065
0.10	0.10000	0.00000	0.000066
0.20	0.20000	0.00000	0.000066
0.50	0.50001	-0.00001	0.000065
1.00	1.00001	-0.00001	0.000066
2.00	2.00000	0.00000	0.000067
5.00	5.00001	-0.00001	0.000068
10.00	10.00004	-0.00004	0.000070
20.00	20.00006	-0.00006	0.000078
50.00	50.00000	0.00000	0.00012
100.00	100.00002	-0.00002	0.00019
120.00	120.00002	-0.00002	0.00022

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.0000
2	50.0000
3	50.0000
4	50.0000
5	50.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/1 Sirinthon Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand

Tel. +66 2433 8331

Email : calibration@sithiporn.com

SITHIPORN
associates



NSC-TIS-17025
CALIBRATION 0394

Cert. No. : SP25026

Pages : 1 of 4

Calibration Certificate

Equipment : UV-VIS SPECTROPHOTOMETER
Manufacturer : PERKINELMER
Model : LAMBDA 25
Serial No.: 501S14123010
ID No.: SP03/58
Calibration Mode : WAVELENGTH ACCURACY
PHOTOMETRIC ACCURACY
STRAY LIGHT

Condition As Found : GOOD

Customer : S.P.S CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN ROAD,
CHOMPHON SUB-DISTRICT, CHATUCHAK DISTRICT,
BANGKOK PROVINCE 10900 THAILAND.

Location : ORGANIC LABORATORY IV

Ambient Temperature : (22.9 $\pm$ 5) °C

Relative Humidity : (53.7 $\pm$ 25) %

Received Date : 22 AUGUST 2025

Calibration Date : 22 AUGUST 2025

Date of Issue : 25 AUGUST 2025

Calibrated by : Nitinun Srihawan

Approved by :

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : SP25026
Job No. : VC68SP0019
Pages : 2 of 4

Calibration Method :

This instrument was calibrated by using on-site calibration procedure In-house method : CP-SP-01
The calibration procedure to direct measurement wavelength accuracy by using wavelength standard solution, Photometric accuracy by using absorbance standard filter and absorbance standard solution
The calibration procedure used was based on ASTM E275-01, ASTM E925-02

Condition of this result of calibration :

1. Certified reference materials

Material	Ref. type	Cell serial No.	Cert. No.	Due Date
Holmium liquid	RM-HL	29706	126461	24/10/2026
Didymium liquid	RM-DL	28912	126462	24/10/2026
Neutral density filter	RM-1N2N3N	13877	126457	24/10/2026
Potassium dichromate solutions	RM-0204060810	14204	126497	25/10/2026
Potassium Iodide solution	-	KI-0701-001	CI-0185-24	14/05/2026

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 The UK National Physical Laboratory (NPL)

Result of calibration : Wavelength Accuracy

(Without adjustment)

Material	Certified Values of Reference Material (nm)	UUC* Reading (nm)	Error (nm)	Uncertainty ± (nm)	k Factor
RM-HL	278.13	278.21	0.08	0.16	2.00
	361.25	361.39	0.14	0.16	2.00
	467.82	467.71	-0.11	0.16	2.00
	536.56	536.50	-0.06	0.16	2.00
	640.50	640.36	-0.14	0.16	2.00
RM-DL	740.09	739.85	-0.24	0.16	2.00
	864.94	865.12	0.18	0.16	2.00

UUC* = Unit Under Calibration

Michael B.

Cert. No. : SP25026
Job No. : VC68SP0019
Pages : 3 of 4

Result of calibration : Photometric Accuracy

Material	Wavelength (nm)	Filter S/N	Nominal Absorbance (A)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor
Neutral Density glass filter	440.0	29381	0.5	0.5443	0.5413	-0.0030	0.0043	2.00
		29914	0.7	0.7484	0.7455	-0.0029	0.0054	2.00
		29360	1.0	1.0527	1.0535	0.0008	0.0032	2.00
	465.0	29381	0.5	0.4948	0.4922	-0.0026	0.0041	2.00
		29914	0.7	0.6906	0.6877	-0.0029	0.0050	2.00
		29360	1.0	0.9695	0.9709	0.0014	0.0031	2.00
	546.1	29381	0.5	0.5090	0.5068	-0.0022	0.0036	2.00
		29914	0.7	0.6985	0.6960	-0.0025	0.0041	2.00
		29360	1.0	0.9814	0.9825	0.0011	0.0031	2.00
	590.0	29381	0.5	0.5375	0.5353	-0.0022	0.0034	2.00
		29914	0.7	0.7256	0.7231	-0.0025	0.0037	2.00
		29360	1.0	1.0213	1.0219	0.0006	0.0032	2.00
	635.0	29381	0.5	0.5223	0.5202	-0.0021	0.0033	2.00
		29914	0.7	0.6927	0.6901	-0.0026	0.0036	2.00
		29360	1.0	0.9744	0.9750	0.0006	0.0032	2.00

UUC* = Unit Under Calibration

Michael B.

Cert. No. : SP25026
Job No. : VC68SP0019
Pages : 4 of 4

Result of calibration : Photometric Accuracy

(Without adjustment)

Material	Wavelength (nm)	Solution (mg/l)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor
Potassium dichromate solutions	235.0	20	0.2415	0.2443	0.0028	0.0101	2.00
		40	0.4866	0.4871	0.0005	0.0115	2.00
		60	0.7415	0.7295	-0.0120	0.0067	2.00
		80	0.9854	0.9844	-0.0010	0.0071	2.00
		100	1.2444	1.2425	-0.0019	0.0073	2.00

UUC* = Unit Under Calibration

Condition of this result of calibration : Spectrophotometer PERKINELMER Model LAMBDA 25 S/N 501S14123010

Resolution of Wavelength Mode 0.1 nm

Resolution of Photometric Mode 0.001 A

Parameter Setting

Measurement Mode Wavelength, Absorbance

Wavelength Scan 190 nm - 1100 nm

Scanning Speed 7.5 nm/min

Band width(Wavelength) 1.0

Band width(Vis) 1.0

Band width(Uv) 1.0

Stray Light** UUC* Reading at 220.0 nm	
Transmission T(%)	Absorbance(A)
0.020	3.7032

**Specific Acceptance :

Transmission ≤ 1.0 T(%), Absorbance ≥ 2.0 A

**Stray light not TISI Accredited

The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95%

End of Calibration Certificate

ระดับเสียง



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-69/0204

MTC No. EEL. BP. 152/0169

CALIBRATION CERTIFICATE

Submitted by : S.P.S.CONSULTING SERVICE CO.,LTD.

Address : 7 Soi Phaholyothin 24, Phaholyothin Road, Jompol, Chatuchak, Bangkok 10900.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Sound Calibrator

Manufacturer : ACO

Model : 2127

Serial No. : 130006

Ambient Environment

Temperature : (23 + 3) °C

Relative Humidity : (50 ± 15) %

Ambient Pressure : (101.325 ± 1.500) kPa

- Standards used :
1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.
 2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.
 3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.
 4. Digital Multimeter Agilent 34401A S/N MY44005560.
 5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.
 6. Audio Analyzer Keithley 2015-P S/N 4106495.
 7. Condenser Microphone Bruel&Kjaer 4180 S/N 2889871.

Calibration Procedure: CP-102-04 based on IEC 60942:2003; The sound pressure level generated by sound calibrator under test shall be measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 29 Jan. 2026

Date of Calibration : 11 Feb. 2026

1/2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoo Mai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-69/0204

MTC No. EEL. BP. 152/0169

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20μPa at 1000 Hz

Acoustic Output in dB re 20μPa, Corrected to Reference Conditions: 101.325 kPa, 23.0 °C and 50 %RH.

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	93.89	-0.11	± 0.10	±0.40 dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	999.9	-0.1	± 1.5	±1.0%

3. Total Distortion

Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	1.90	± 0.50	±3.0%

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Calibrated by

Approved by :

Date of Calibration : 11 Feb. 2026

Date of Issue : 12 Feb. 2026

Electrical and Electronic Standards Laboratory
Industrial Metrology and Testing Service Centre

Ref : 2011269012900497001

End of Certificate

2/2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoo Mai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

Noise R_355/26

Sound Level Meter Calibration Report

Acoustic Calibrator Data						
Brand	ACO		Number	AC 03/56		
Model	2127		Serial No.	130006		
Calibration Range	94 dB, 1000 Hz		Last Calibration	11 February 2026		
			Due Date	11 February 2027		

Calibration Data						
Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-B03	ACO	6236	192028	09 June 2026	93.9	93.9
ACO-B05	ACO	6236	222311	09 June 2026	93.8	93.9
ACO-B19	ACO	6236	172057	09 June 2026	93.9	93.9
ACO-R55	ACO	6236	00222309	09 June 2026	93.8	93.9
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.81 ± 0.10 dB	

Calibrated by :



Approved by :



Noise R_164/26

Sound Level Meter Calibration Report

Acoustic Calibrator Data						
Brand	ACO		Number	AC 03/56		
Model	2127		Serial No.	130006		
Calibration Range	94 dB, 1000 Hz		Last Calibration	11 February 2026		
			Due Date	11 February 2027		

Calibration Data						
Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-B41	ACO	6236	00192032	08 April 2026	93.9	93.9
ACO-B43	ACO	6236	00192034	08 April 2026	93.9	93.9
ACO-R40	ACO	6236	00192052	08 April 2026	94.0	93.9
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.89 ± 0.10 dB	

Calibrated by :



Approved by :



Request No. 21-68/0514

MTC No. EEL. BP. 34/0868

CALIBRATION CERTIFICATE

Submitted by : S.P.S.Consulting Service Co.,Ltd.

Address : 7 Soi Phaholyothin 24, Phaholyothin Road, Jompol, Chatuchak, Bangkok 10900.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
: Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Sound Calibrator

Manufacturer : SVANTEK

Model : SV34

Serial No. : 83820

Ambient Environment

Temperature : (23 ± 3) °C

Relative Humidity : (50 ± 15) %

Ambient Pressure : (101.325 ± 1.500) kPa

- Standards used :**
1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.
 2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.
 3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.
 4. Digital Multimeter Agilent 34401A S/N MY44005560.
 5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.
 6. Audio Analyzer Panasonic VP-7722A S/N 041477D122.
 7. Condenser Microphone B&K 4180 S/N 2633526.

Calibration Procedure: CP-102-04 based on IEC 60942-2003; The sound pressure level generated by sound calibrator under test shall be measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 14 Aug. 2025

Date of Calibration : 22 Aug. 2025

1/2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

Request No. 21-68/0514

MTC No. EEL. BP. 34/0868

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 114 dB re 20µPa at 1000 Hz

Acoustic Output in dB re 20µPa, Corrected to Reference Conditions: 101.325 kPa, 23.0 °C and 50 %RH.

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	114.02	0.02	± 0.10	±0.75 dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	1000.0	0.0	± 1.5	±2.0%

3. Total Distortion

Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	0.21	± 0.50	±4.0%

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Calibrated by :

Approved by :

Date of Calibration : 22 Aug. 2025

Date of Issue : 25 Aug. 2025

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Ref : 2011268081403169011

End of Certificate

2 / 2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

Noise Dose R_165/26

Noise Dose Meter Calibration Report

Acoustic Calibrator Data

Brand	SVANTEK	Number	SV 03/60
Model	SV34	Serial No.	83820
Calibration Range	114 dB, 1000 Hz	Last Calibration	25 August 2025
		Due Date	25 August 2026

Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
NMD-R02	SVANTEK	SV-104IS	60152	08 April 2026	114.0	114.0
NMD-R03	SVANTEK	SV-104IS	60153	08 April 2026	114.0	114.0
NMD-R35	SVANTEK	SV-104IS	80873	08 April 2026	113.9	114.0
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					114.02± 0.10 dB	

Calibrated by :



Approved by :



คุณภาพน้ำ



CERTIFICATE No : 26E3363
REFERENCE No : 80514-1

PAGE : 1 OF 3

Certificate of Calibration

EQUIPMENT : pH METER
MANUFACTURER : HANNA
MODEL : HI3512
SERIAL No : TH118035
ID No : PH 04/56
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.
CALIBRATION DATE : 02-Apr-26

APPROVED BY : 

ISSUED DATE : 02-Apr-26

RECEIVED DATE : 01-Apr-26

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.



CERTIFICATE No : 26E3363

PAGE : 2 OF 3

Calibration Report

EQUIPMENT : pH METER
MANUFACTURER : HANNA
ID No : PH 04/56
RECEIVED DATE : 01-Apr-26
AMBIENT TEMPERATURE : 23 °C ± 3 °C
MODEL : HI3512
SERIAL NUMBER : TH118035
CALIBRATION DATE : 02-Apr-26
RELATIVE HUMIDITY : 50 % RH ± 10% RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT METHOD BASED ON WI-TQ-062 AND WI-TQ-063. THE DISPLAY UNIT WAS TESTED BY GENERATING STANDARD VOLTAGE TO THE UNIT AND READING THE VALUE COMPARED WITH THE CALCULATED VALUE. THE DISPLAY AND ELECTROD WAS CALIBRATED BY USING STANDARD pH BUFFER
2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No/ LOT No	CERTIFICATE No	DUE DATE
1) pH STANDARD SOLUTION	00651-36	CC829914	4956-16178366	11-Sep-27
2) pH STANDARD SOLUTION	00651-38	CC831093	4957-16224157	01-Oct-27
3) pH STANDARD SOLUTION	00651-40	CC826321	4958-16046326	10-Jul-27
4) PROCESS CALIBRATOR	CA150	91S6079	26E936	17-Mar-27
5) BATH	260014	1247 48074	25T9431	12-Sep-26
6) THERMOMETER WITH PROBE	421504	55000379	25T9466	12-Sep-26

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO SI UNIT MAINTAINED AT :-
 - NATIONAL INSTITUTE OF STANDARD AND TECHNOLOGY, USA.
 - NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION : ADJUSTMENT

1. DISPLAY UNIT ONLY

SLOPE FACTOR k = 2.303 RT/F = 59 mV/pH

mV APPLIED	UUC READING (mV)	CORRECTION (mV)	UUC READING (pH)	UNCERTAINTY OF MEASUREMENT (± mV)	COVERAGE FACTOR k
414.11	414.3	-0.19	-0.256	0.15	2.00
354.95	355.1	-0.15	0.759	0.15	2.00
295.80	296.0	-0.20	1.773	0.15	2.00
236.64	236.8	-0.16	2.787	0.15	2.00
177.48	177.7	-0.22	3.801	0.15	2.00
118.32	118.5	-0.18	4.816	0.15	2.00
59.16	59.4	-0.24	5.831	0.15	2.00
0.00	0.2	-0.20	6.845	0.15	2.00
-59.16	-58.9	-0.26	7.878	0.15	2.00
-118.32	-118.1	-0.22	8.915	0.15	2.00
-177.48	-177.2	-0.28	9.952	0.15	2.00
-236.64	-236.4	-0.24	10.990	0.15	2.00
-295.80	-295.5	-0.30	12.027	0.15	2.00
-354.95	-354.7	-0.25	13.064	0.15	2.00
-414.11	-413.8	-0.31	14.101	0.15	2.00

END OF CALIBRATION REPORT PAGE 2 OF 3





CERTIFICATE No : 26E3363

PAGE : 3 OF 3

Calibration Report

RESULT OF CALIBRATION (CONTINUE) :

2. DISPLAY UNIT WITH pH ELECTRODE S/N: 11340D0M

STANDARD pH BUFFER SOLUTION (pH)	UUC READING (pH)	CORRECTION (pH)	VALUE BEFORE ADJUSTMENT	UNCERTAINTY OF MEASUREMENT ($\pm$ pH)	COVERAGE FACTOR k
4.008	4.008	0.000	4.142	0.012	2.00
6.998	7.000	-0.002	7.068	0.012	2.00
10.007	10.009	-0.002	10.226	0.014	2.00

3. DISPLAY UNIT WITH TEMPERATURE

STANDARD READING ($^{\circ}$ C)	UUC READING ($^{\circ}$ C)	CORRECTION ($^{\circ}$ C)	VALUE BEFORE ADJUSTMENT	UNCERTAINTY OF MEASUREMENT ($\pm$ $^{\circ}$ C)	COVERAGE FACTOR k
25.004	25.0	0.004	---	0.0085	2.00

4. PERCENT SLOPE 91%

UUC : UNIT UNDER CALIBRATION

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



CERTIFICATE No : 26M2268
REFERENCE No : 80204-3

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE
MANUFACTURER : SARTORIUS
MODEL : BSA224S-CW
SERIAL No : 36591843
ID No : BA 09/61
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : SUCHAT S.
CALIBRATION DATE : 05-Mar-26

APPROVED BY : 
ISSUED DATE : 06-Mar-26
RECEIVED DATE : 05-Mar-26

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF QUALITY CALIBRATION CO., LTD.



**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkac, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com

CERTIFICATE No : 26M2268

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : BSA224S-CW
MANUFACTURER : SARTORIUS S/N : 36591843
ID No : BA 09/61 RECEIVED DATE : 05-Mar-26
AIR PRESSURE : 1004mbar $\pm$ 1mbar CALIBRATION DATE : 05-Mar-26
AMBIENT TEMPERATURE : 25° C $\pm$ 1° C RELATIVE HUMIDITY : 50 %RH $\pm$ 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-i-151	C02250116	28-Jan-27
2) STANDARD WEIGHT	E2	15843	C02250117	29-Jan-27

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT


1. ZERO SETTING FUNCTION : NORMAL

2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0.000055 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ($\pm$ g)
0.0	0.0000	0.0000	0.00010
0.1	0.1000	0.0000	0.00011
0.2	0.2000	0.0000	0.00010
0.5	0.5000	0.0000	0.00011
1.0	1.0000	0.0000	0.00011
2.0	2.0000	0.0000	0.00011
5.0	5.0000	0.0000	0.00011
10.0	10.0000	0.0000	0.00011
20.0	20.0001	-0.0001	0.00011
50.0	50.0000	0.0000	0.00013
100.0	100.0001	-0.0001	0.00019
200.0	200.0001	-0.0001	0.00032

5. OFF CENTER LOADING ERROR

POINT	READING (g)
1	100.0000
2	100.0000
3	100.0000
4	100.0000
5	100.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

**QUALITY CALIBRATION CO., LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkac, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com

CERTIFICATE No : 26T0464

REFERENCE No : 79659-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : COD REACTOR
MANUFACTURER : HACH
MODEL : DRB 200
SERIAL No : 15110C0497
ID No : DRB 04/59
SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : SOMCHAI S.

CALIBRATION DATE : 30-Jan-26

APPROVED BY :

ISSUED DATE : 30-Jan-26

RECEIVED DATE : 30-Jan-26

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.





QUALITY CALIBRATION CO., LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkac, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 26T0464

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : COD REACTOR
MANUFACTURER : HACH
ID NUMBER : DRB 04/59
RECEIVED DATE : 30-Jan-26
AMBIENT TEMPERATURE : 23° C ± 1° C
MODEL : DRB 200
SERIAL NUMBER : 15110C0497
CALIBRATION DATE : 30-Jan-26
RELATIVE HUMIDITY : 54 %RH ± 10 % RH


CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT METHOD WITH CALIBRATED THERMOCOUPLE TYPE K UNDER NO LOAD CONDITION. THE THERMOCOUPLES WERE PLACED ON POINTS AND LOCATED AS THE PICTURE.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT MODEL SERIAL No CERTIFICATE No DUE DATE
1) DATA LOGGER WITH TC TYPE K HYDRA 2635A 6849323 25T5342 18-Jun-26
3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO., LTD.

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

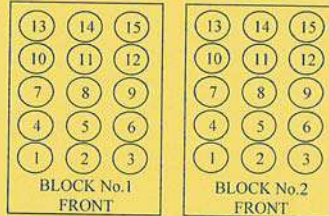

TEMPERATURE MEASUREMENT ACCURACY TEST

Block No.	1	2
Controller temperature (°C)	144	145
Indicating Temperature	144	145
Measured Temperature (°C) at Spread Locations	1	149.3
	2	149.1
	3	149.9
	4	149.6
	5	149.3
	6	149.5
	7	149.9
	8	149.7
	9	149.5
	10	149.4
	11	148.5
	12	149.1
	13	149.0
	14	149.1
	15	148.5
Uncertainty of Measurement(± °C)	0.89	0.89

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2 : LOCATION 10 WAS REFERENCE LOCATION.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY COVERAGE FACTOR k=2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



MAINTENANCE AND TEST CERTIFICATE MODEL OPTIMA 5300DV

Customer : S.P.S.Consulting Service Co.,Ltd Date Tested: December 18, 2025
Recommendation Recertification
Address : 7 Soi Phaholyothin 24 Period 6 Months
Phaholyothin Road Recertification Due: June 28, 2026
Jompol Chatuchak, Bangkok 1090 Date Last Certified: July 1, 2025
User Name: K.Phenpha Vipasthawatt Visit Number: 2of 2
Phone: 083-9269252 PerkinElmer Phone: 02-719-6420 ext 206
Fax: 02-513-4221 PerkinElmer Fax: 02-318-5597

CONFIGURATION TESTED

MODEL SERIAL NUMBER
OPTIMA 5300DV 077C7042401

TESTED EQUIPMENT CALIBRATION NUMBER EXPIRATION

IPV Methods

TEST STANDARD USED PART NUMBER EXPIRATION DATE

Multielement Standard N069-1579 November 30, 2026

Wavecal Solution N058-2152 July 30, 2026

VIS Wavecal solution N930-2946 August 30, 2026

Instrument Cal. STD4 N930-0221 November 30, 2026

CUSTOMER SUPPLIED COMMENTS CUSTOMER INITIALS

2 % HNO3

10 % HNO3

Page 1 of 4

PerkinElmer Scientific (Thailand) Co., Ltd.
290 Soi Soonvijai 4, Bangkapi, Huay Kwang, Bangkok 10310 Head Office



MAINTENANCE AND TEST CERTIFICATE MODEL OPTIMA 5300DV

SERIAL NUMBER 077C7042401
DATE TESTED December 18, 2025
1. MECHANICAL CHECKS

A. Inspect and clean all fans and filters.

☐ OK

B. Inspect and replace as necessary, all torch components including the RF coil.

☐ OK

C. Inspect all tubing for sign of clacking or leaking.

☐ OK

D. Adjust water and gas pressure regulator settings.

☐ OK

E. Inspect and leak check pneumatics drawers.

☐ OK

F. Clean the exterior of the instrument.

☐ OK

2. OPTICAL CHECKS

A. Inspect and clean all optical components.

☐ OK

B. As required, check and replace all purgefilters.

☐ OK

C. Recheck optical alignment.

☐ OK

3. COOLING SYSTEM CHECKS

A. Perform preventive maintenance on chiller.

☐ OK

B. Flush out the chiller every year.

☐ N/A

4. PERFORMANCE CHECKS

A. Torch View Alignment.

☐ OK

B. Wavelength Calibration.

☐ OK


MAINTENANCE AND TEST CERTIFICATE MODEL OPTIMA 5300DV

SERIAL NUMBER : 077C7042401
DATE TESTED : December 18, 2025

PARAMETER	SPECIFICATION			FINAL VALUE	
Spectral Resolution : UV	As	193.696 nm	≤ 0.007	0.00530	
	Ni	231.604 nm	≤ 0.008	0.00708	
	Ni	341.476 nm	≤ 0.012	0.00776	
Spectral Resolution : VIS	La	408.672 nm	≤ 0.020	0.01614	
	Ba	455.403 nm	≤ 0.025	0.02377	
Precision	As	193.656 nm	% RSD < 1.0	0.67	%
	Zn	213.856 nm	% RSD < 1.0	0.62	%
	Mn	257.610 nm	% RSD < 1.0	0.88	%
	La	379.478 nm	% RSD < 1.0	0.63	%
	Ba	455.403 nm	% RSD < 1.0	0.65	%
	Ba	493.408 nm	% RSD < 1.0	0.45	%
Detection Limits : Axial	Tl	190.080 nm	3(sd)	3.21	ppb
	As	193.696 nm	3(sd)	6.06	ppb
	Pb	220.353 nm	3(sd)	0.92	ppb
Detection Limits : Radial	As	193.696 nm	3(sd)	17.35	ppb
	Zn	213.856 nm	3(sd)	1.79	ppb
	Mn	257.610 nm	3(sd)	0.18	ppb
	La	379.478 nm	3(sd)	0.76	ppb
	Ba	455.403 nm	3(sd)	0.11	ppb
	Ba	493.408 nm	3(sd)	0.56	ppb
BEC : Axial (IB X 500)/(IS-IB)	Cd	226.502 nm	≤ 150 ppb	40.52	
BEC : Radial (IB X 1000)/(IS-IB)	Mn	257.610 nm	≤ 45 ppb	42.33	



MAINTENANCE AND TEST CERTIFICATE MODEL
OPTIMA 5300DV

SERIAL NUMBER 077C7042401 **DATE TESTED** December 18, 2025

Remarks :

Commissioning follow as commissioning performance sheets.

This is to certify that the above tests have been performed and the configuration tested



meets




does not meet

the PerkinElmer Specifications listed on this certificate.

This certificate does not modify PerkinElmer's standard terms and condition of sale,
including warranty terms.

Service Department PerkinElmer Ltd

Authorized Representative:

()
Wiphan Promlunda
Service Engineer



right solutions.
right partner.

รายการเครื่องมือที่ใช้ในการวิเคราะห์ / ทดสอบ

Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Rayong Lab	BOD	DO meter with Sensor	RYG_EN0032	20-Jan-25	20-Jul-26	18
Rayong Lab	BOD	Incubator	RYG_EN0154	1-Nov-24	1-May-26	18
Rayong Lab	BOD	Burette	RYG_EN0216	18-Sep-25	18-Sep-26	12
Rayong Lab	Oil & Grease	Electronic Balance	RYG_EN0003	3-Feb-26	3-Feb-27	12
Rayong Lab	Oil & Grease	Liquid Bath (Water)	RYG_EN0220	27-Nov-25	27-Nov-26	12
Rayong Lab	pH at 25 °C	pH meter	RYG_EN0183	18-Jul-25	18-Jan-27	18



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert. No.: 25LM10

Page.: 1 of 2

Equipment : DO Meter with Sensor

Manufacturer : YSI

Model : 5000-115V

Serial No. : 15E102796

ID No. : RYG_EN0032

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
(Rayong Branch)
616/10 Moo 5 T. Maenam Khu, A. Pluakdaeng,
Rayong 21140 Thailand

Location : TPA On Site Calibration Laboratory

Received Order : 17 January 2025

Calibrated Date : 20 January 2025

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

AC Line Voltage : (220 ± 22) V

Calibrated by : Warakorn Lernagatrakul

Approved by :

() Chakrit Waewwanjua

(✓) Suwit Imjai

() Kunchit Promprat

Issue Date : 23 January 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

REVIEW BY

APPROVED BY

NEXT CAL DATE.....20/07/26



Equipment : DO Meter with Sensor

Condition As-Received : Used Item

Reference : 2501-0600DSC-2

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1) Digital Thermometer	2188080	2411022	TPA	17 Sep 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N.: 15E100464

<u>Calibration Point</u>	<u>Immersion Depth</u>	<u>Standard Temperature</u>	<u>UUC* Reading</u>	<u>Error</u>	<u>Uncertainty</u>	<u>Coverage Factor</u>
(°C)	(mm)	(°C)	(°C)	(°C)	(± °C)	<i>k</i>
20.00	60	20.002	19.81	-0.192	0.15	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)

CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES

534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000 FAX. 0-2719-9484

Certificate of Testing

Cert.No.: 25TW15

Page.: 1 of 2

Equipment : DO Meter

Manufacturer : YSI

Model : 5000-115V

Serial No. : 15E102796

ID No. : RYG_EN0032

Received Date : 17 January 2025

Test Date : 20 January 2025

Reference : 2501-0600DSC-1

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
(Rayong Branch)
616/10 Moo 5, T.Maenam Khu, A.Pluakdaeng,
Rayong 21140, Thailand

Laboratory Condition : Temperature (25 ± 5) °C
Humidity (50 ± 20) %
In - house method : CP-CH9
by Comparison Technique with Azide Modification Method

Test Procedure :

Tested by : 

Approved by :

() Pornthippa Tameyakul
() Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 21 January 2025



Cert.No.: 25TW15
Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

<u>Instruments</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1. Burette	-	130BU10	23CG1172	22 Mar 2025
2. Balance	14233821	110RC001	24MM131	04 July 2025

2. Standard Material :-

<u>Material</u>	<u>Manufacturer</u>	<u>Lot.No.</u>	<u>Assay</u>
Sodium Thiosulfate 5-Hydrate AR	KEMAUS	2203162447	99.6%

Result : Dissolved Oxygen Meter Adjustment With Air 100 %
Dissolved Oxygen Probe No.: 15E100464

<u>Titration Method</u> (Azide Modification Method)	<u>DO Meter</u> <u>Reading</u>	<u>Standard Deviation</u>
(mg/L)	(mg/L)	(mg/L)
8.20	8.20	0.0084

This report was certified only for the instrument we tested. It is allowable to use for study
Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced
other in full, without written approval of the laboratory

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert. No.: 24TM1663
Page : 1 of 3

Equipment : Low Temp. Incubator

Manufacturer : Memmert

Model : IPP750

Serial No. : V818.0084

ID No. : RYG_EN0154

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd. Rayong Branch
616/10 Moo 5, T.Maenam Khu,
A.Pluakdaeng,
Rayong 21140, Thailand

Location : BOD Room

Received Order : 01 November 2024

Calibration Date : 01 November 2024

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

AC Line Voltage : (220 ± 22) V

Calibrated by :

Approved by :

() Ponpan Paipim
() Suwit Imjai
(✓) Kunchit Promprat

Issue Date : 07 November 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : Low Temp. Incubator
Condition As-Received : Used Item
Reference : 2411-0002OC-1

Cert. No.: 24TM1663
Page : 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY44073381	24LM73	TPA	18 May 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.


3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close

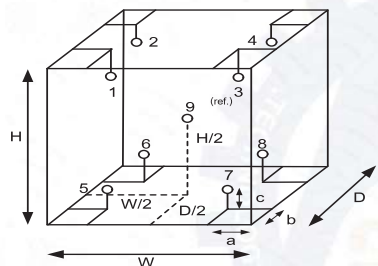

Probe Installation Details :

a = 10 cm
b = 10 cm
c = 10 cm

Dimension of Chamber :

D = 0.60 m
W = 1.0 m
H = 1.2 m
Capacity = 0.72 m³

Environment during calibration		
	Beginning	Finished
Temp. (°C)	24	25
REL.Humid. (%)	55	53
AC Supply (Volt)	220	221

Position :	Ref. Std. ID No.:
1	1RTD-2/1
2	1RTD-2/2
3	22-01RTD-03
4	1RTD-2/4
5	1RTD-2/5
6	1RTD-2/6
7	23-01RTD-07
8	1RTD-2/8
9 (ref.)	23-01RTD-09



Equipment : Low Temp. Incubator
Condition As-Received : Used Item
Reference : 2411-0002OC-1

Cert. No.: 24TM1663
Page : 3 of 3

Result of Calibration :-

(*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor k
20.0	20.0	20.0	0.026	0.26	0.53	2

Calibration Point (°C)	Measured Temperature (°C)									Uncertainty (± °C)
	Position									
	1	2	3	4	5	6	7	8	9 (ref.)	
20.0	20.071	19.915	20.273	20.179	19.977	19.782	20.056	20.026	20.033	0.30

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor **k**, providing a level of confidence of approximately 95 %.

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0 2717 3000 30 FAX.0 2710 0484



Certificate of Calibration

Cert.No.: 25CG3668
Page.: 1 of 2

Equipment : Burette
Capacity : 50 mL
Serial No. : -
ID. No. : RYG_EN0216
Manufacturer : Witeg
Made in : Germany
Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
Rayong Branch
616/10 Moo 5 T.MaenamKoo, A,Pluakdaeng
Rayong 21140, Thailand
Ambient Temperature : (20 ± 2.5) °C
Relative Humidity : (50 ± 10) %
Barometric Pressure : 753 mmHg
Calibration Procedure : ASTM E 542 - 01
Calibrated by : Srisuda Khamtha
Approved by :
() Ponpan Paipim
(✓) Chakrit Waewwanjua

Issue Date : 19 September 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.



Equipment : Burette
Received Date : 16 September 2025
Condition As-Received : Used Item
Calibration Date : 18 September 2025
Reference : 2509-0564DSC-3

Cert.No.: 25CG3668
Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

Instruments	Model	Serial No.	ID. No.	Certificate No.	Traceability	Due date
1) Balance	XP205	B134206712	140RC007	25MM296	TPA	16 July 2026
2) Humidity/Baro/Temp	MHB-382SD	AM.42259	140EC016	25H1616	TPA	14 Aug 2026
3) Digital Thermometer	HH376	230806555	140EC013	25I1740	TPA	17 Jan 2026

This measurement result is traceable to SI Unit

2. The certificate is valid only to the item calibrated on date and place of calibration.
3. True value is converted to true volume at the standard temperature of 20 °C

Calibration result :

Nominal capacity (mL)	Reading (mL)	Uncertainty (± mL)	k Factor
10	10.0264	0.0082	2.00
25	25.0141	0.0087	2.00
50	49.9952	0.010	2.00

Remark mL = cm³

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-



Accredited by
NSC-TISI-TIS 17025
Calibration 0426

Calibration certificate

Calibration Certificate No. 26BCI0066

Object	Electronic non-automatic weighing instrument	This calibration certificate documents the traceability to national standards.
Manufacturer	Sartorius	Uncertainties of measurements are taken into account when only statements of compliance are made.
Type	MSU224S-100-DU	This certificate was prepared by Sartorius Corporation in accordance to the current ISO/IEC 17025:2017 standard and Sartorius Work Instruction (Method) SOP WI 08.
Serial QM Ident. no.	31709552 RYG_EN0003	This certificate relate and apply this equipment only.
Customer	ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)	
	616/10 Moo 5 T.Maenamkoo, A.Pluak Daeng, Rayong 21140, Thailand.	
Order no.	278579	REVIEW BY [Redacted] ...
Number of pages	4	APPROVED [Redacted] ...
Date of calibration	03 Feb 2026	NEXT CAL D [Redacted] ...

This calibration certificate may not be reproduced other than in full except with the permission of NSC-TISI-TIS-17025 and the issuing laboratory. Calibration certificates without signature are not valid.

The user is obliged to have the object recalibrated at appropriate intervals.

Date of issue	03 Feb 2026	Approval of the Calibration Certificate	Person in charge
		Mr. Chonchai Inthana	Chonchai Inthana

Calibration object

Single range instrument

Model	MSU224S-100-DU
Serial Number	31709552
QM Ident. no Inventory no.	RYG_EN0003 ---

Maximum capacity (Max. load)	220.0000 g
Measured up to	220.0000 g
Scale interval	0.0001 g

Place of calibration

Address	According to page 1
Department Cost center	Laboratory Department. ---
Building Floor	--- 1st Floor.
Room	Balance Room.
Maximum temperature variation at place of calibration	5 K

Calibration procedure

EURAMET Calibration Guide No. 18, Version 4.0 (11/2015) - Guidelines on the Calibration of Non-Automatic Weighing Instruments

Test equipment

Test equipment type	Test equipment ID	Valid until
Thermometer	Testo 174H H/T250743 (Traceable to SI unit through ENTECH)	18 Nov 2026
Test weight set OIML R111 E2	Certificate No.M2508149S ,E2(Traceable to SI unit through TCS)	19 Aug 2027

Adjustment Status

The measuring device was internally adjusted before the calibration.

Environmental and measuring conditions

Date of calibration	03 Feb 2026
Temperature at place of calibration Temp. diff. <i>T</i> _{weights} - <i>T</i> _{place}	24,5 °C 0.5 K
Measuring conditions	The installation site is suitable. The device is level. Balance was loaded up to Max before test.
Comments	Humidity 52.0 %RH.

Measurement results | Measurement uncertainties

Repeatability			Eccentricity		
Test load (nominal): 10 g 200 g			Test load (nominal): 100 g		
	10 g	200 g			
1	10.0000 g	200.0000 g	Center		100.0000 g
2	10.0000 g	200.0001 g	Front left		100.0000 g
3	10.0000 g	200.0001 g	Back left		99.9999 g
4	10.0001 g	200.0001 g	Back right		100.0000 g
5	10.0000 g	200.0001 g	Front right		100.0000 g
6	10.0000 g	200.0000 g	Maximum deviation from centric loading indication		
7	10.0000 g	200.0000 g	Δ <i>f</i> _{ecc} max = 0.0001 g		
8	10.0000 g	200.0000 g			
9	10.0000 g	200.0000 g			
10	10.0000 g	200.0000 g			
	<i>s</i> = 0.00003 g	<i>s</i> = 0.00005 g			

Error of indication						
Testload	Indication	Error	Expansion factor	Uncertainty	Uncertainty relative	
<i>L</i>	<i>I</i>	<i>E</i>	<i>k</i>	<i>U</i> (<i>E</i>)	<i>U</i> _{rel} (<i>E</i>)	
0.0100 g	0.0100 g	0.0000 g	2.00	0.00010 g	1.0 %	
0.1000 g	0.1000 g	0.0000 g	2.00	0.00013 g	0.13 %	
0.5000 g	0.5000 g	0.0000 g	2.00	0.00013 g	0.027 %	
1.0000 g	1.0000 g	0.0000 g	2.00	0.00013 g	0.013 %	
5.0000 g	5.0000 g	0.0000 g	2.00	0.00014 g	0.0027 %	
10.0000 g	10.0000 g	0.0000 g	2.00	0.00014 g	0.0014 %	
20.0000 g	20.0000 g	0.0000 g	2.00	0.00014 g	0.00071 %	
50.0000 g	50.0001 g	0.0001 g	2.00	0.00015 g	0.00030 %	
100.0000 g	100.0000 g	0.0000 g	2.00	0.00018 g	0.00018 %	
200.0000 g	200.0000 g	0.0000 g	2.00	0.00028 g	0.00014 %	
220.0000 g	220.0000 g	0.0000 g	2.00	0.00032 g	0.00015 %	
Maximum error of indication		<i>E</i> _{max} = 0.0001 g				

*U*_{rel}(*E*) is the quotient of *U*(*E*) and test load *L*. The uncertainty of measurement *U*(*E*) is valid only if error *E* is considered. You will find reference notes on the uncertainty of measurement in use under: Appendix to the calibration certificate | Interpretation of measurement results.
Reference note: The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the documented Expansion factor, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

End of calibration certificate

Uncertainty of measurement in use

Device adjusted before measurement	Yes
Temperature deviation considered	1.5 K (isoCAL active)
Temperature coefficient considered	1 · 10 ⁻⁶ /K


Uncertainty of the weighing result *U*_g(*W*)

*U*_g(*W*) = 0.00013 g + 3.65 · 10⁻⁶ · *R*

Reference note: The current uncertainty of measurement is calculated by entering of the reading *R* into this formula. In relation to this, there is no need for a correction of the indication error. The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied with an Expansion factor of 2, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

Indication in % from max load	Net indication <i>R</i>	Uncertainty <i>U</i> _g (<i>W</i>)	Uncertainty relative <i>U</i> _g (<i>W</i>) _{rel}
1 %	2.2000 g	0.00014 g	0.0063 %
25 %	55.0000 g	0.00033 g	0.00060 %
50 %	110.0000 g	0.00053 g	0.00048 %
75 %	165.0000 g	0.00073 g	0.00044 %
100 %	220.0000 g	0.00093 g	0.00042 %

Graphic realization of the relative uncertainty of measurement | process accuracy

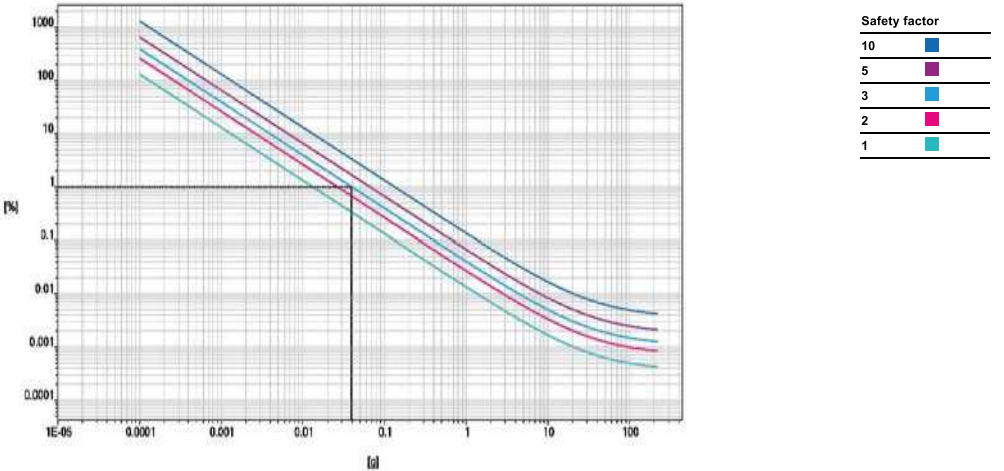

Displayed example	
Process accuracy	1.00 %
Safety factor	3
Minimum sample weight	0.0395 g




Metrology Center
SCI ECO Services Company Limited
51 Moo 8, Tubkwang, Kaeng Khoi, Saraburi, Thailand 18260
Bangkok Tel : +668 9205 6851 , +669 81924 0059
Saraburi Tel : +669 8247 2360
Website : www.scieco.co.th E-Mail : calibrate@scg.co.th




Certificate No. T252169

Certificate of Calibration

Page 1 of 3

Equipment : Liquid Bath (Water)
Manufacturer : Memmert
Model : WNE29
Serial No. : L623.0105
Customer Code : RYG_EN0220
ID No. : T5650A5
Customer : AIS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
616/10 Moo 5 T.Maenamkoo,
A.Plukdaeng, Rayong 21140
Customer Location : Wet Chemistry Lab
Date of Receipt : 19 November 2025
Calibrated By : Sujjar Naknakred (Site Calibration Manager)
Approved By :  / Boonchai Suriyawong (Site Calibration Manager)
Date of Issue : 01 DEC 2025

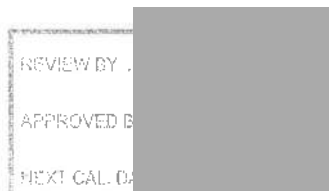

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.



Metrology Center
SCI ECO Services Company Limited
51 Moo 8, Tubkwang, Kaeng Khoi, Saraburi, Thailand 18260



Certificate No. T252169

Calibration Report

Page 2 of 3

Equipment : Liquid Bath (Water)
Date of Calibration : 27 November 2025
Environment : Temperature : 25.5-25.7 °C
Line Voltage : 221.8-225.5 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

- This equipment was calibrated by insert five resistance thermometer detectors into its water bath , the other one thermocouple type T use for ambient temperature measurement . The calibration was done in according to WI-T36 (based on ASTM E715-80 (Reapproved 2022)).
All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .
- Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
RTD	100 OHM	M18 (CH1-CH5)	T251758	17 October 2026
DATA LOGGER	34970A	T261	T251758	17 October 2026
- This certificate is traceable to :
National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)
- Condition of calibrated item : good
Equipment Description :
Time Constant 1 Hour 3 Minute At 63 °C
- Adjustment :
(X) without adjustment () after adjustment


Approve



Certificate No. T252169

Page 3 of 3

Calibration Report

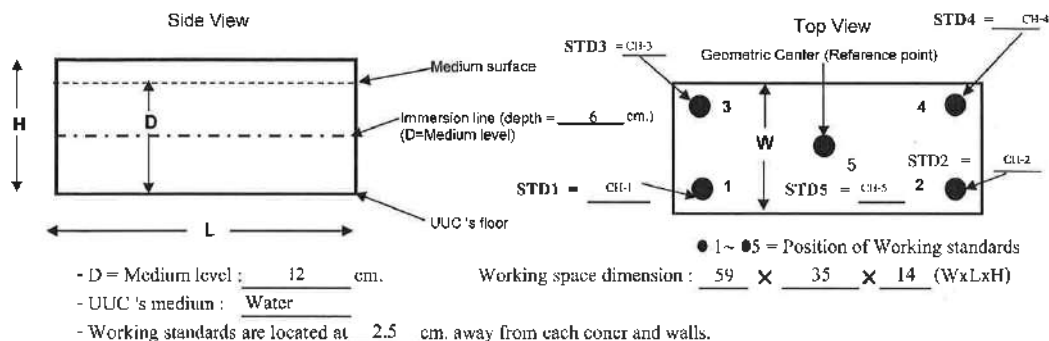

Measurement Results:

Calibration Point	Average Standard Reading at each position (°C)				
	CH-1	CH-2	CH-3	CH-4	CH-5
63	62.93	63.13	62.94	63.10	63.09
85	85.15	85.33	85.21	85.43	85.20

Liquid Bath (Water)			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (± °C)	Uniformity (± °C)	Uncertainty (± °C)	Coverage Factor k
	Min , Max	Average					
63.0	62.9 , 63.1	63.0	63.04	0.08	0.17	0.27	2.06
85.0	84.8 , 85.2	85.0	85.26	0.13	0.24	0.43	2.23

* The quoted uncertainty exclude "uniformity"

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k which for a t-distribution, providing a level of confidence of approximately 95 % .

End of Certificate.

Approved By _____

Certificate of Calibration

Cert.No.: 25CH847

Page: 1 of 3

Equipment :

pH Meter

Manufacturer :

Mettler Toledo

Model :

SevenCompact S220

Serial No. :

C104059460

ID No. :

RYG_EN0183

Condition As-Received:

Used Item

Received Date :

17 July 2025

Calibration Date :

18 July 2025

Reference :

2507-0561DSC-3

Submitted by :

ALS Laboratory Group (Thailand) Co.,Ltd.
 Rayong Branch
 616/10 Moo 5, T.Maenam Khu,
 A.Pluakdaeng, Rayong 21140, Thailand

Ambient Temperature :

(25 ± 2.5) °C

Relative Humidity :

(50 ± 15) %

Calibration Procedure :

In - house method :
 - CP-CH5 by direct measurement with DC voltage standard and direct measurement with certified reference material (CRM)
 - CP-CH8 by comparison with temperature standard

Calibrated by :

Walalak Sirithean

Approved by :

() Chakrit Waewwanjua

() Ponpan Paipim

(✓) Saithip Meangmai

Issue Date :

21 July 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Cert.No.: 25CH847
Page.: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1) Document Process Calibrator	54030049	130RC116	24E2759	25 Aug 2025
2) Ref. Standard Thermometer	3240076	60RC033	25I394	01 Apr 2026

- This measurement result is traceable to SI through Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.007	CPA chem	1066665	18 Jan 2027
pH 6.965	CPA chem	1066667	18 Jan 2026
pH 10.010	CPA chem	1114385	08 June 2026

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4,7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (±mV)	Coverage factor <i>k</i>
	pH	mV	mV	pH		
pH Meter S/N.: C104059460	4.000	177.48	177.3	4.000	0.058	2.00
	7.000	0.00	-0.2	7.000	0.058	2.00
	10.000	-177.48	-177.6	10.000	0.058	2.00



Cert.No.: 25CH847
Page.: 3 of 3

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (±)	Coverage factor <i>k</i>
pH Electrode S/N.: 5240606	4.007	4.008	184.6	0.0044	2.00
	6.965	6.966	10.2	0.0084	2.00
	10.010	10.009	-164.9	0.0065	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : InLabExpert Pro-ISM

- Serial No. : 5240606

Dimension of probe

- Length : 120 mm.

- Diameter : 12 mm.

- Immersion Depth : 100 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (± °C)	Coverage factor <i>k</i>
25.0	25.001	25.0	-0.001	0.13	2.00

Remark - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484



Certificate of Calibration

Certificate No. : 25E2372

Page : 1 of 2

Equipment : pH Meter
Manufacturer: Mettler Toledo
Model : SevenCompact S220
Serial No.: C104059460
ID No.: RYG_EN0183

Condition As-Received: Used Item

Received Date: 17 July 2025

Calibration Date: 22 July 2025

Reference: 2507-0561DSC

Ambient Temperature: (23 ± 2) °C

Relative Humidity: (50 ± 10) %

Submitted by: ALS Laboratory Group (Thailand) Co.,Ltd. Rayong Branch

This certificate may not be reproduced other than in full,
except with the prior written approval of the head of
Corporate Services 3: Equipment Calibration and Testing Services.

616/10 Moo 5, T.Maenam Khu, A.Pluakdaeng,
Rayong 21140, Thailand

Procedure used: Calibration were conducted using calibration procedure No. CP-E17 according to EURAMET cg-15.

Condition of this result of calibration

1.Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Multi-Product Calibrator	5500A	6315011	25E1627	19 May 2026

2.This result of calibration was made on requested at the point specified by customer.

3.The certificate is valid only to the item calibrated on date and place of calibration.

4.This measurement result is traceable to the International System of Unit maintained through:-

-Technology Promotion Association (Thailand-Japan), NSC-ONSC Accredited No. Calibration 0008

Calibrated by : Napachanok Prasomsosoori
Issue Date : 23 July 2025

Approved Signatory : 
[] Pha
[] Nuntawat Khamchai
[✓] Pongsagorn Boonyaporn



Cert. No.: 25E2372

Page.: 2 of 2

Result of calibration :- (*) Without adjustment () After adjustment

Function:	DC voltage measurement	Range:	2000 mV	
	<u>Standard Value</u>	<u>UUC* Reading</u>	<u>Error</u>	<u>Uncertainty</u>
	(mV)	(mV)	(mV)	(± μV)
	-200.0000	-200.0	0.0	68
	-150.0000	-150.0	0.0	65
	-100.0000	-100.0	0.0	63
	-50.0000	-50.0	0.0	61
	0.0000	0.0	0.0	58
	50.0000	49.9	-0.1	61
	100.0000	99.9	-0.1	63
	150.0000	149.9	-0.1	65
	200.0000	199.9	-0.1	68

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95 %

UUC* = Unit Under Calibration.

-o0o-

คุณภาพอากาศในการทำงาน



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Environmental Conditions

Temperature : 25 ± 3 °C
Pressure : 1010 ± 15 mmbar

Personal Pump Data				Calibration Data									
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve		
					Setting			Actual (Q std.)			y		
					1	2	3	1	2	3	y	R ²	
B01	SKC	224-PCXR4	262101	01/04/2026	1,000	1,500	2,000	1,002	1,503	2,004	1.002x - 1.364	1.000	
B02	SKC	224-PCXR4	626166	01/04/2026	1,000	1,500	2,000	1,004	1,501	2,003	1.001x - 0.594	1.000	
B03	SKC	224-PCXR4	612968	01/04/2026	1,000	1,500	2,000	1,003	1,502	1,994	1.003x - 0.098	0.999	
B04	SKC	224-PCXR4	602804	01/04/2026	1,000	1,500	2,000	1,000	1,502	1,998	0.998x + 0.642	1.000	
B05	SKC	224-PCXR4	612693	01/04/2026	1,000	1,500	2,000	1,001	1,504	1,999	1.000x - 1.767	1.000	
B06	SKC	224-PCXR4	262188	01/04/2026	1,000	1,500	2,000	999	1,500	2,002	1.001x - 3.590	1.000	
B07	SKC	224-PCXR4	626262	01/04/2026	1,000	1,500	2,000	997	1,506	2,003	1.004x - 9.859	0.999	
B08	SKC	224-PCXR4	626100	01/04/2026	1,000	1,500	2,000	1,003	1,503	2,005	1.003x - 4.140	1.000	
B09	SKC	224-PCXR4	626479	01/04/2026	1,000	1,500	2,000	998	1,497	1,997	1.000x - 3.362	1.000	
B10	SKC	224-PCXR4	091950	01/04/2026	1,000	1,500	2,000	1,004	1,506	1,996	1.003x - 7.323	0.999	
B11	SKC	224-PCXR8	564315	01/04/2026	1,000	1,500	2,000	1,000	1,493	2,003	1.005x - 10.601	1.000	
B12	SKC	224-PCXR4	034656	01/04/2026	1,000	1,500	2,000	997	1,495	1,997	0.998x - 1.755	1.000	
B13	SKC	224-PCXR4	602073	01/04/2026	1,000	1,500	2,000	1,001	1,501	1,986	0.996x + 2.864	0.999	
B14	SKC	224-PCXR4	626313	01/04/2026	1,000	1,500	2,000	999	1,494	1,997	0.999x - 1.898	0.999	
B15	SKC	224-PCXR4	626474	01/04/2026	1,000	1,500	2,000	996	1,498	1,993	1.007x - 17.126	0.999	
B16	SKC	224-PCXR4	626477	01/04/2026	1,000	1,500	2,000	1,002	1,499	1,997	0.997x + 1.352	1.000	
B17	SKC	224-PCXR4	626660	01/04/2026	1,000	1,500	2,000	996	1,510	1,999	1.005x - 12.252	0.999	
B18	SKC	224-PCXR4	691484	01/04/2026	1,000	1,500	2,000	995	1,499	1,997	1.006x - 12.384	1.000	
B19	SKC	224-PCXR4	691599	01/04/2026	1,000	1,500	2,000	998	1,501	1,991	1.004x - 10.506	0.999	
B20	SKC	224-PCXR4	691587	01/04/2026	1,000	1,500	2,000	997	1,495	1,998	1.003x - 7.247	1.000	
B21	SKC	224-PCXR4	691531	03/04/2026	1,000	1,500	2,000	998	1,496	1,996	1.000x - 3.454	1.000	
B22	SKC	224-PCXR4	691654	03/04/2026	1,000	1,500	2,000	996	1,494	1,997	0.998x - 2.784	1.000	
B23	SKC	224-PCXR4	798393	02/04/2026	1,000	1,500	2,000	1,000	1,503	1,999	0.999x - 1.308	1.000	
B24	SKC	224-PCXR4	626363	03/04/2026	1,000	1,500	2,000	1,001	1,509	1,995	1.002x - 6.940	0.999	
B25	SKC	224-PCXR4	798489	03/04/2026	1,000	1,500	2,000	1,002	1,502	2,004	1.004x - 7.267	1.000	
B26	SKC	224-PCXR4	798479	03/04/2026	1,000	1,500	2,000	996	1,503	2,003	1.006x - 12.675	1.000	
B27	SKC	224-PCXR4	691673	02/04/2026	1,000	1,500	2,000	1,000	1,504	2,000	0.999x + 0.483	1.000	
B28	SKC	224-PCXR4	691570	03/04/2026	1,000	1,500	2,000	997	1,510	2,001	0.998x - 0.435	0.999	
B29	SKC	224-PCXR4	626472	03/04/2026	1,000	1,500	2,000	998	1,494	1,992	1.000x - 5.221	1.000	
B30	SKC	224-PCXR4	691489	03/04/2026	1,000	1,500	2,000	1,008	1,504	2,006	1.003x - 2.114	1.000	
B31	SKC	224-PCXR4	691509	03/04/2026	1,000	1,500	2,000	1,003	1,503	2,002	0.997x + 0.610	0.999	
B32	SKC	224-PCXR4	091567	03/04/2026	1,000	1,500	2,000	1,002	1,502	1,996	0.996x + 7.008	1.000	
B33	SKC	224-PCXR4	091756	03/04/2026	1,000	1,500	2,000	998	1,501	1,992	1.006x - 12.101	0.999	
B34	SKC	224-PCXR4	612962	03/04/2026	1,000	1,500	2,000	1,001	1,494	2,004	1.004x - 8.196	1.000	
B35	SKC	224-PCXR4	602682	03/04/2026	1,000	1,500	2,000	997	1,504	1,998	1.000x - 2.804	1.000	
B36	SKC	224-PCXR4	626164	03/04/2026	1,000	1,500	2,000	996	1,512	1,996	1.001x - 5.867	0.999	
B37	SKC	224-PCXR4	626256	03/04/2026	1,000	1,500	2,000	999	1,496	2,005	1.007x - 11.487	1.000	
B38	SKC	224-PCXR4	626167	03/04/2026	1,000	1,500	2,000	1,002	1,500	2,003	1.008x - 16.377	0.999	
B39	SKC	224-PCXR4	034637	03/04/2026	1,000	1,500	2,000	998	1,490	1,994	0.996x - 0.044	1.000	
B40	SKC	224-PCXR4	798349	03/04/2026	1,000	1,500	2,000	1,001	1,501	2,000	0.995x + 0.921	0.999	

Calibrated by :

Approved by :



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136833

Environmental Conditions

Temperature : 25 ± 3 °C
Pressure : 1010 ± 15 mmbar

Personal Pump Data				Calibration Data									
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve		
					Setting			Actual (Q std.)			y		
					1	2	3	1	2	3	y	R ²	
R01	SKC	224-PCXR4	602467	01/04/2026	1,000	1,500	2,000	1,001	1,500	2,007	1.005x - 6.003	1.000	
R02	SKC	224-PCXR4	626450	03/04/2026	1,000	2,000	3,000	1,000	1,503	2,001	1.001x - 0.383	1.000	
R03	SKC	224-PCXR4	691592	03/04/2026	1,000	1,500	2,000	1,005	1,501	2,000	1.007x - 15.384	0.999	
R04	SKC	224-PCXR4	691672	03/04/2026	1,000	1,500	2,000	1,007	1,513	1,999	0.996x + 5.855	0.999	
R05	SKC	224-PCXR4	798470	05/04/2026	1,000	1,500	2,000	1,000	1,499	1,997	0.997x + 3.107	1.000	
R06	SKC	224-PCXR4	798456	03/04/2026	1,000	1,500	2,000	998	1,497	1,996	0.998x + 0.120	1.000	
R07	SKC	224-PCXR4	798480	05/04/2026	1,000	1,500	2,000	1,002	1,506	2,001	0.999x + 3.219	1.000	
R08	SKC	224-PCXR4	883215	03/04/2026	1,000	1,500	2,000	1,004	1,501	1,992	1.003x - 9.877	0.999	
R09	SKC	224-PCXR4	034650	03/04/2026	1,000	1,500	2,000	998	1,506	2,003	1.004x - 5.723	1.000	
R10	SKC	224-PCXR4	091745	03/04/2026	1,000	1,500	2,000	999	1,507	1,996	1.005x - 13.080	0.999	
R11	SKC	224-PCXR4	091763	05/04/2026	1,000	1,500	2,000	1,001	1,504	2,001	1.000x + 0.104	1.000	
R12	SKC	224-PCXR4	091548	03/04/2026	1,000	1,500	2,000	998	1,505	1,996	0.998x + 1.482	1.000	
R13	SKC	224-PCXR4	091638	03/04/2026	1,000	1,500	2,000	1,001	1,504	2,000	0.999x + 2.097	1.000	
R14	SKC	224-PCXR4	091764	05/04/2026	1,000	1,500	2,000	1,007	1,506	2,001	1.004x - 8.866	0.999	
R15	SKC	224-PCXR8	529457	05/04/2026	1,000	1,500	2,000	998	1,492	1,999	1.001x - 6.322	1.000	
R16	SKC	224-PCXR8	529643	03/04/2026	1,000	1,500	2,000	1,004	1,506	2,004	1.007x - 11.726	0.999	
R17	SKC	224-PCXR8	529645	05/04/2026	1,000	1,500	2,000	998	1,503	1,998	1.000x - 0.703	1.000	
R18	SKC	224-PCXR8	566756	03/04/2026	1,000	1,500	2,000	999	1,508	1,995	1.002x - 8.012	0.999	
R19	SKC	224-PCXR8	566802	05/04/2026	1,000	1,500	2,000	998	1,502	1,998	1.000x - 0.823	1.000	
R20	SKC	224-PCXR8	529089	03/04/2026	1,000	1,500	2,000	999	1,503	1,996	0.997x + 2.001	1.000	
R21	SKC	224-PCXR8	665728	03/04/2026	1,000	1,500	2,000	998	1,505	1,999	1.000x - 0.483	1.000	
R22	SKC	224-PCXR8	707444	05/04/2026	1,000	1,500	2,000	1,007	1,496	2,000	1.001x - 6.418	0.999	
R23	SKC	224-PCXR8	761067	05/04/2026	1,000	1,500	2,000	1,001	1,502	2,004	1.002x - 1.446	1.000	
R24	SKC	224-PCXR8	707693	03/04/2026	1,000	1,500	2,000	1,002	1,503	2,001	0.999x + 2.560	1.000	
R25	SKC	224-PCXR8	761052	03/04/2026	1,000	1,500	2,000	1,009	1,504	2,005	0.997x + 4.106	0.999	
R26	SKC	224-PCXR8	707656	05/04/2026	1,000	1,500	2,000	1,002	1,503	2,000	0.998x + 4.497	1.000	
R27	SKC	224-PCXR8	707398	03/04/2026	1,000	1,500	2,000	1,001	1,505	2,004	1.003x - 1.921	1.000	
R28	SKC	224-PCXR8	707481	05/04/2026	1,000	1,500	2,000	1,010	1,513	2,006	0.997x + 5.531	0.999	
R29	SKC	224-PCXR8	707402	03/04/2026	1,000	1,500	2,000	1,003	1,502	1,992	1.003x - 10.216	0.999	



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Rotameter Calibration Report (For Personal Pump High Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136833

Calibration Data

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (mL/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R ²
H-R01	Dwyer	VFB-65	01/04/2026	500	1,000	2,000	499.7	1000.6	1996.7	$1.000x - 0.544$	1.000
H-R02	Dwyer	VFB-65	01/04/2026	500	1,000	2,000	501.2	992.4	1990.0	$1.001x - 5.362$	0.999
H-R03	Dwyer	VFB-65	03/04/2026	500	1,000	2,000	501.4	997.5	1997.3	$0.998x + 2.606$	1.000
H-R04	Dwyer	VFB-65	05/04/2026	500	1,000	2,000	502.5	993.6	1985.2	$0.999x - 2.085$	0.999
H-R05	Dwyer	VFB-65	05/04/2026	500	1,000	2,000	500.4	1001.3	1999.8	$1.000x + 1.247$	1.000
H-R06	Dwyer	VFB-65	03/04/2026	500	1,000	2,000	500.8	997.2	1994.6	$0.999x - 0.348$	1.000

Calibrated by :

Approved by :



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Rotameter Calibration Report (For Personal Pump Low Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136833

Calibration Data

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (mL/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R ²
L-R01	Dwyer	VFA-21	01/04/2026	50	100	200	50.3	101.1	201.9	$0.998x + 0.955$	1.000
L-R02	Dwyer	VFA-21	01/04/2026	50	100	200	50.2	101.7	201.0	$0.999x + 0.367$	0.999
L-R03	Dwyer	VFA-21	03/04/2026	50	100	200	50.3	101.2	201.0	$1.001x + 0.605$	1.000
L-R04	Dwyer	VFA-21	05/04/2026	50	100	200	50.7	100.8	200.2	$1.000x + 0.719$	1.000
L-R05	Dwyer	VFA-21	05/04/2026	50	100	200	50.1	101.2	200.5	$1.001x - 0.213$	0.999
L-R06	Dwyer	VFA-21	03/04/2026	50	100	200	50.3	100.8	200.1	$0.999x + 0.639$	1.000

Calibrated by :

Approved by :



CERTIFICATE No : 26M2266
REFERENCE No : 80204-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE
MANUFACTURER : METTLER TOLEDO
MODEL : XS105DU
SERIAL No : 1126422905
ID No : BA 05/50
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : SUCHAT S.
CALIBRATION DATE : 05-Mar-26

APPROVED BY :
ISSUED DATE : 06-Mar-26
RECEIVED DATE : 05-Mar-26



CERTIFICATE No : 26M2266

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE
MANUFACTURER : METTLER TOLEDO
ID No : BA 05/50
AIR PRESSURE : 1004mbar $\pm$ 1mbar
AMBIENT TEMPERATURE : 25° C $\pm$ 1° C
MODEL : XS105DU
S/N : 1126422905
RECEIVED DATE : 05-Mar-26
CALIBRATION DATE : 05-Mar-26
RELATIVE HUMIDITY : 50 %RH $\pm$ 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	C02250116	28-Jan-27
2) STANDARD WEIGHT	E2	15843	C02250117	29-Jan-27

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
- NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL
2. TARE FUNCTION : NORMAL
3. REPEATABILITY OF READING AT 120 g WAS 0.000055 g
4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ($\pm$ g)
0.00	0.00000	0.00000	0.000065
0.02	0.02000	0.00000	0.000065
0.10	0.10000	0.00000	0.000066
0.20	0.20000	0.00000	0.000066
0.50	0.50001	-0.00001	0.000065
1.00	1.00001	-0.00001	0.000066
2.00	2.00000	0.00000	0.000067
5.00	5.00001	-0.00001	0.000068
10.00	10.00004	-0.00004	0.000070
20.00	20.00006	-0.00006	0.000078
50.00	50.00000	0.00000	0.00012
100.00	100.00002	-0.00002	0.00019
120.00	120.0002	-0.0002	0.00022

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.0000
2	50.0000
3	50.0000
4	50.0000
5	50.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A
COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





WO-11540201/2025

MAINTENANCE AND TEST CERTIFICATE MODEL
OPTIMA 5300DV

Customer : S.P.S.Consulting Service Co.,Ltd **Date Tested:** December 18, 2025
Address : 7 Soi Phaholyothin 24 **Period** 6 **Months**
Paholyothin Road **Recertification Due:** June 28, 2026
Jompoi Chatuchak, Bangkok 1090 **Date Last Certified:** July 1, 2025
User Name: K.Phenpha Vipasthawatt **Visit Number:** 2 of 2
Phone: 083-9269252 **PerkinElmer Phone:** 02-719-6420 ext 206
Fax: 02-513-4221 **PerkinElmer Fax:** 02-318-5597

CONFIGURATION TESTED

MODEL
OPTIMA 5300DV

SERIAL NUMBER
077C7042401

**ACCESSORIES/COMPONENT
NOT INCLUDED**

TESTED EQUIPMENT

IPV Methods

CALIBRATION NUMBER

EXPIRATION

TEST STANDARD USED

Multielement Standard

N069-1579

November 30, 2026

Wavecal Solution

N058-2152

July 30, 2026

VIS Wavecal solution

N930-2946

August 30, 2026

Instrument Cal. STD4

N930-0221

November 30, 2026

CUSTOMER SUPPLIED

COMMENTS

CUSTOMER INITIALS

2 % HNO3

10 % HNO3

Page 1 of 4



WO-11540201/2025

MAINTENANCE AND TEST CERTIFICATE MODEL
OPTIMA 5300DV

SERIAL NUMBER 077C7042401 **DATE TESTED** December 18, 2025

1. MECHANICAL CHECKS

A. Inspect and clean all fans and filters.

☐ OK

B. Inspect and replace as necessary, all torch components including the RF coil.

☐ OK

C. Inspect all tubing for sign of clacking or leaking.

☐ OK

D. Adjust water and gas pressure regulator settings.

☐ OK

E. Inspect and leak check pneumatics drawers.

☐ OK

F. Clean the exterior of the instrument.

☐ OK

2. OPTICAL CHECKS

A. Inspect and clean all optical components.

☐ OK

B. As required, check and replace all purgefilters.

☐ OK

C. Recheck optical alignment.

☐ OK

3. COOLING SYSTEM CHECKS

A. Perform preventive maintenance on chiller.

☐ OK

B. Flush out the chiller every year.

☐ N/A

4. PERFORMANCE CHECKS

A. Torch View Alignment.

☐ OK

B. Wavelength Calibration.

☐ OK

Page 2 of 4



MAINTENANCE AND TEST CERTIFICATE MODEL

OPTIMA 5300DV

SERIAL NUMBER : <u>077C7042401</u>		DATE TESTED : <u>December 18, 2025</u>	
PARAMETER	SPECIFICATION		FINAL VALUE
Spectral Resolution : UV	As 193.696 nm	≤ 0.007	0.00530
	Ni 231.604 nm	≤ 0.008	0.00708
	Ni 341.476 nm	≤ 0.012	0.00776
Spectral Resolution : VIS	La 408.672 nm	≤ 0.020	0.01614
	Ba 455.403 nm	≤ 0.025	0.02377
Precision	As 193.656 nm	% RSD < 1.0	0.67 %
	Zn 213.856 nm	% RSD < 1.0	0.62 %
	Mn 257.610 nm	% RSD < 1.0	0.88 %
	La 379.478 nm	% RSD < 1.0	0.63 %
	Ba 455.403 nm	% RSD < 1.0	0.65 %
	Ba 493.408 nm	% RSD < 1.0	0.45 %
Detection Limits : Axial	Tl 190.080 nm	3(sd)	3.21 ppb
	As 193.696 nm	3(sd)	6.06 ppb
	Pb 220.353 nm	3(sd)	0.92 ppb
Detection Limits : Radial	As 193.696 nm	3(sd)	17.35 ppb
	Zn 213.856 nm	3(sd)	1.79 ppb
	Mn 257.610 nm	3(sd)	0.18 ppb
	La 379.478 nm	3(sd)	0.76 ppb
	Ba 455.403 nm	3(sd)	0.11 ppb
	Ba 493.408 nm	3(sd)	0.56 ppb
BEC : Axial (IB X 500)/(IS-IB)	Cd 226.502 nm	≤ 150 ppb	40.52
BEC : Radial (IB X 1000)/(IS-IB)	Mn 257.610 nm	≤ 45 ppb	42.33



MAINTENANCE AND TEST CERTIFICATE MODEL

OPTIMA 5300DV

SERIAL NUMBER	<u>077C7042401</u>	DATE TESTED	<u>December 18, 2025</u>
---------------	--------------------	-------------	--------------------------

Remarks :

Commissioning follow as commissioning performance sheets.

This is to certify that the above tests have been performed and the configuration tested

☒ meets

☐ does not meet

the PerkinElmer Specifications listed on this certificate.

This certificate does not modify PerkinElmer's standard terms and condition of sale, including warranty terms.

Service Department PerkinElmer Ltd

Authorized Representative: _____

(Wiphan Promlumda)

Service Engineer



Certificate of Calibration

Aquion : Anion (ID#894)

This certificate is to verify that instrument below are calibrated

by Archemica Lab Co.,Ltd.

AQUION S/N : 190840059

AS-DV S/N : 190915235

for

S.P.S. Consulting Service Co., Ltd.



Operator Signature :

Date : April 27, 2026

Test Engineer

ระดับเสียงในการทำงาน



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-69/0204

MTC No. EEL. BP. 152/0169

CALIBRATION CERTIFICATE

Submitted by : S.P.S.CONSULTING SERVICE CO.,LTD.

Address : 7 Soi Phaholyothin 24, Phaholyothin Road, Jompol, Chatuchak, Bangkok 10900.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Sound Calibrator

Manufacturer : ACO

Model : 2127

Serial No. : 130006

Ambient Environment

Temperature : (23 + 3) °C

Relative Humidity : (50 ± 15) %

Ambient Pressure : (101.325 ± 1.500) kPa

- Standards used :
1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.
 2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.
 3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.
 4. Digital Multimeter Agilent 34401A S/N MY44005560.
 5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.
 6. Audio Analyzer Keithley 2015-P S/N 4106495.
 7. Condenser Microphone Bruel&Kjaer 4180 S/N 2889871.

Calibration Procedure: CP-102-04 based on IEC 60942:2003; The sound pressure level generated by sound calibrator under test shall be measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 29 Jan. 2026

Date of Calibration : 11 Feb. 2026

1/2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.5

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory

668 Mu 2 Tambon Bangpoo Mai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440

E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office

196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-69/0204

MTC No. EEL. BP. 152/0169

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20μPa at 1000 Hz

Acoustic Output in dB re 20μPa, Corrected to Reference Conditions: 101.325 kPa, 23.0 °C and 50 %RH.

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	93.89	-0.11	± 0.10	±0.40 dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	999.9	-0.1	± 1.5	±1.0%

3. Total Distortion

Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	1.90	± 0.50	±3.0%

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Calibrated by :

Approved by :

Date of Calibration : 11 Feb. 2026

Date of Issue : 12 Feb. 2026

Electrical and Electronic Standards Laboratory
Industrial Metrology and Testing Service Centre

Ref : 2011269012900497001

End of Certificate

2 / 2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.5

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory

668 Mu 2 Tambon Bangpoo Mai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440

E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office

196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Noise R_355/26

Sound Level Meter Calibration Report

Acoustic Calibrator Data

Brand	ACO	Number	AC 03/56
Model	2127	Serial No.	130006
Calibration Range	94 dB, 1000 Hz	Last Calibration	11 February 2026
		Due Date	11 February 2027

Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-B03	ACO	6236	192028	09 June 2026	93.9	93.9
ACO-B05	ACO	6236	222311	09 June 2026	93.8	93.9
ACO-B19	ACO	6236	172057	09 June 2026	93.9	93.9
ACO-R55	ACO	6236	00222309	09 June 2026	93.8	93.9
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.81 ± 0.10 dB	

Calibrated by :

Approved by :



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Noise R_164/26

Sound Level Meter Calibration Report

Acoustic Calibrator Data

Brand	ACO	Number	AC 03/56
Model	2127	Serial No.	130006
Calibration Range	94 dB, 1000 Hz	Last Calibration	11 February 2026
		Due Date	11 February 2027

Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-B41	ACO	6236	00192032	08 April 2026	93.9	93.9
ACO-B43	ACO	6236	00192034	08 April 2026	93.9	93.9
ACO-R40	ACO	6236	00192052	08 April 2026	94.0	93.9
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.89 ± 0.10 dB	

Calibrated by :

Approved by :

Request No. 21-68/0514

MTC No. EEL. BP. 34/0868

CALIBRATION CERTIFICATE

Submitted by : S.P.S.Consulting Service Co.,Ltd.

Address : 7 Soi Phaholyothin 24, Phaholyothin Road, Jompol, Chatuchak, Bangkok 10900.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
: Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Sound Calibrator

Manufacturer : SVANTEK

Model : SV34

Serial No. : 83820

Ambient Environment

Temperature : (23 ± 3) °C

Relative Humidity : (50 ± 15) %

Ambient Pressure : (101.325 ± 1.500) kPa

- Standards used :**
1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.
 2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.
 3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.
 4. Digital Multimeter Agilent 34401A S/N MY44005560.
 5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.
 6. Audio Analyzer Panasonic VP-7722A S/N 041477D122.
 7. Condenser Microphone B&K 4180 S/N 2633526.

Calibration Procedure: CP-102-04 based on IEC 60942-2003; The sound pressure level generated by sound calibrator under test shall be measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 14 Aug. 2025

Date of Calibration : 22 Aug. 2025

1/2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

Request No. 21-68/0514

MTC No. EEL. BP. 34/0868

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 114 dB re 20μPa at 1000 Hz

Acoustic Output in dB re 20μPa, Corrected to Reference Conditions: 101.325 kPa, 23.0 °C and 50 %RH.

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	114.02	0.02	± 0.10	±0.75 dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	1000.0	0.0	± 1.5	±2.0%

3. Total Distortion

Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	0.21	± 0.50	±4.0%

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Calibrated by

Approved by :

Date of Calibration : 22 Aug. 2025

Date of Issue : 25 Aug. 2025

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Ref : 2011268081403169011

End of Certificate

2 / 2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Noise Dose R_165/26

Noise Dose Meter Calibration Report

Acoustic Calibrator Data

Brand	SVANTEK	Number	SV 03/60
Model	SV34	Serial No.	83820
Calibration Range	114 dB, 1000 Hz	Last Calibration	25 August 2025
		Due Date	25 August 2026

Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
NMD-R02	SVANTEK	SV-104IS	60152	08 April 2026	114.0	114.0
NMD-R03	SVANTEK	SV-104IS	60153	08 April 2026	114.0	114.0
NMD-R35	SVANTEK	SV-104IS	80873	08 April 2026	113.9	114.0
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					114.02± 0.10 dB	

Calibrated by

Approved by :

ระดับความร้อนในการทำงาน

Certificate of Calibration

Certificate Number : SPR26010387-1 Page : 1 of 3

Customer : S.P.S. CONSULTING SERVICE CO., LTD.
7 Soi Phaholyothin 24 Phaholyothin Road., Jompol, Chatuchak,
Bangkok 10900

Equipment Name : Area Heat Stress Monitor
Manufacturer : Quest Technologies
Model : QUESTemp 34
Serial Number : TEH090208
ID. Number : R08

Environmental Conditions

Ambient Temperature : 23 °C ± 2 °C Received Date : 30 Jan 2026
Relative Humidity : 50 % ± 15 % Calibration Date : 03 Feb 2026
Location of Calibration : In-Lab Recommend Due Date : 03 Feb 2027
Calibration Procedure : SP-CPT-04-13 Date of Issue : 04 Feb 2026

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Jirasak Pumbut

Calibration Officer

Approved by



(Mr.Worapong Sinthusopa)

Authorized Signatory

SP-FM-04-15 rev.0

Calibration Report

Certificate Number : SPR26010387-1

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
THERMO-HYGROMETER	5020A	A47046	TMU2500342	29 Jan 2027
Temp & Humidity Test Chamber	TEMI1500-01/SD/N/N/	S7110ZL742 1014	SPR25040010-13	20 Apr 2026

Traceability

This certification is traceable to the International System of Unit maintained at :
NA - NA Caltechnologies Co., Ltd.
SP Metrology - SP Metrology system (Thailand) Co.Ltd.



Result of Calibration

Certificate Number : SPR26010387-1

Page : 3 of 3

Temperature Accuracy in the Measurement. (WET)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.009	29.7	-0.309	0.20
35.0	35.012	34.7	-0.312	0.20
40.0	40.017	39.7	-0.317	0.21

Temperature Accuracy in the Measurement. (DRY)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.009	29.6	-0.409	0.20
35.0	35.012	34.6	-0.412	0.20
40.0	40.017	39.6	-0.417	0.21

Temperature Accuracy in the Measurement. (GLOBE)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.009	29.7	-0.309	0.20
35.0	35.012	34.7	-0.312	0.20
40.0	40.017	39.7	-0.317	0.21

Note :

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2$, providing a level of confidence approximately 95%.

- End of Certificate -

SP-FM-04-15 REV.0



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com, www.spscon.com

Heat R025

Heat Stress WBGT Meter Verification Report			
Verification Data			
Heat Stress WBGT Meter No. :	R08	Verification Date :	08 April 2026
Brand :	Quest Technologies	Ambient Temp. :	24.6 °C
Model :	QUESTemp 34	Barometric Pressure :	1010 mmbar
Serial No. :	TEH090208	Relative Humidity :	48 %
Verification Module (Electronic Sensor Check) :			
Verification Module No. : 21 WB = 12.5 °C, DB = 47.1 °C, G = 69.3 °C			
Result of Verification : Without Adjustment			
Wet Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
12.5	12.6	-0.1	± 0.5
Dry Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
47.1	47.2	-0.1	± 0.5
Globe Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
69.3	69.2	0.1	± 0.5
UUC* = UNIT UNDER CALIBRATION			

Verified by :



Approved by :





Certificate of Calibration

Certificate Number : SPR25110089-3

Page : 1 of 3

Customer : S.P.S. CONSULTING SERVICE CO., LTD.

7 Soi Phaholyothin 24 Phaholyothin Road., Jompol, Chatuchak,
Bangkok 10900

Equipment Name : Area Heat Stress Monitor

Manufacturer : Quest Technologies

Model : QUESTemp 36

Serial Number : TKE060012

ID. Number : R09

Environmental Conditions

Ambient Temperature : 23 °C ± 2 °C

Relative Humidity : 50 % ± 15 %

Location of Calibration : In-Lab

Calibration Procedure : SP-CPT-04-13

Received Date : 07 Nov 2025

Calibration Date : 26 Nov 2025

Recommend Due Date : 26 Nov 2026

Date of Issue : 27 Nov 2025

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Kijja Visitsilp

Calibration Officer

Approved by



Authorized Signatory

SP-FM-04-15 rev.0



Calibration Report

Certificate Number : SPR25110089-3

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
THERMO-HYGROMETER	5020A	A47046	TMU2500342	29 Jan 2026
Temp & Humidity Test Chamber	TEMI1500-01/SD/N/N/	S7110ZL742 1014	SPR25040010-13	20 Apr 2026

Traceability

This certification is traceable to the International System of Unit maintained at :
NA - NA Caltechnologies Co., Ltd.

SP Metrology - SP Metrology system (Thailand) Co.Ltd.

SP-FM-04-15 rev.0



Result of Calibration

Certificate Number : SPR25110089-3

Page : 3 of 3

Temperature Accuracy in the Measurement. (WET)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.006	29.6	-0.406	0.20
35.0	35.009	34.6	-0.409	0.20
40.0	40.008	39.6	-0.408	0.21

Temperature Accuracy in the Measurement. (DRY)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.006	29.8	-0.206	0.20
35.0	35.009	34.8	-0.209	0.20
40.0	40.008	39.8	-0.208	0.21

Temperature Accuracy in the Measurement. (GLOVE)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.006	29.6	-0.406	0.20
35.0	35.009	34.6	-0.409	0.20
40.0	40.008	39.6	-0.408	0.21

Note :

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2$, providing a level of confidence approximately 95%.

- End of Certificate -



Heat R025

Heat Stress WBGT Meter Verification Report			
Verification Data			
Heat Stress WBGT Meter No. :	R09	Verification Date :	08 April 2026
Brand :	Quest Technologies	Ambient Temp. :	24.6 °C
Model :	QUESTemp ³⁶	Barometric Pressure :	1010 mmbar
Serial No. :	TKE060012	Relative Humidity :	48 %
Verification Module (Electronic Sensor Check) :			
Verification Module No. : 21 WB = 12.5 °C, DB = 47.1 °C, G = 69.3 °C			
Result of Verification : Without Adjustment			
Wet Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
12.5	12.6	-0.1	± 0.5
Dry Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
47.1	47.2	-0.1	± 0.5
Globe Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
69.3	69.2	0.1	± 0.5
UUC* = UNIT UNDER CALIBRATION			

Verified by

Approved by :



Certificate of Calibration

Certificate Number : SPR26030173-5

Page : 1 of 3

Customer : S.P.S. CONSULTING SERVICE CO., LTD.

7 Soi Phaholyothin 24 Phaholyothin Road., Jompol, Chatuchak,
Bangkok 10900

Equipment Name : Area Heat Stress Monitor

Manufacturer : Quest Technologies

Model : QUESTemp 32

Serial Number : TPE070001

ID. Number : R12

Environmental Conditions

Ambient Temperature : 23 °C ± 2 °C

Relative Humidity : 50 % ± 15 %

Location of Calibration : In-Lab

Calibration Procedure : SP-CPT-04-13

Received Date : 11 Mar 2026

Calibration Date : 14 Mar 2026

Recommend Due Date : 14 Mar 2027

Date of Issue : 15 Mar 2026

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform

this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr. Witthawat Jansuwan

Calibration Officer

Approved by



Authorized Signatory

SP-FM-04-15 rev.0



Calibration Report

Certificate Number : SPR26030173-5

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
THERMO-HYGROMETER	5020A	A47046	TMU2600443	01 Feb 2027
Temp & Humidity Test Chamber	TEMI1500-01/SD/N/N/	S7110ZL742 1014	SPR25040010-13	20 Apr 2026

Traceability

This certification is traceable to the International System of Unit maintained at :

NA - NA Caltechnologies Co., Ltd.

SP Metrology - SP Metrology system (Thailand) Co.Ltd.

SP-FM-04-15 rev.0



Result of Calibration

Certificate Number : SPR26030173-5

Page : 3 of 3

Temperature Accuracy in the Measurement. (WET)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.012	30.2	0.188	0.20
35.0	35.009	35.2	0.191	0.20
40.0	40.011	40.1	0.089	0.21

Temperature Accuracy in the Measurement. (DRY)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.012	30.0	-0.012	0.20
35.0	35.009	35.1	0.091	0.20
40.0	40.011	40.1	0.089	0.21

Temperature Accuracy in the Measurement. (GLOBE)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.012	30.0	-0.012	0.20
35.0	35.009	34.9	-0.109	0.20
40.0	40.011	39.9	-0.111	0.21

Note :

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2$, providing a level of confidence approximately 95%.

- End of Certificate -

SP-FM-04-15 REV.0



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompoi, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com, www.spscon.com

Heat R025

Heat Stress WBGT Meter Verification Report			
Verification Data			
Heat Stress WBGT Meter No. :	R12	Verification Date :	08 April 2026
Brand :	Quest Technologies	Ambient Temp. :	24.6 °C
Model :	QUESTemp 32	Barometric Pressure :	1010 mmbar
Serial No. :	TPE070001	Relative Humidity :	48 %
Verification Module (Electronic Sensor Check) :			
Verification Module No. : 21 WB = 12.5 °C, DB = 47.1 °C, G = 69.3 °C			
Result of Verification : Without Adjustment			
Wet Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
12.5	12.6	-0.1	± 0.5
Dry Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
47.1	47.2	-0.1	± 0.5
Globe Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
69.3	69.2	0.1	± 0.5
UUC* = UNIT UNDER CALIBRATION			

Verified by :



Approved by

