ภาคผนวกที่ 4

เอกสารสอบเทียบความถูกต้องของเครื่องมือตรวจวัดคุณภาพสิ่งแวดล้อม

ลำดับที่ 1 คุณภาพอากาศในบรรยากาศ

ลำดับที่ 2 คุณภาพอากาศจากแหล่งกำเนิด

ลำดับที่ 3 คุณภาพน้ำ

ลำดับที่ 4 ระดับเสียงโดยทั่วไป

ลำดับที่ 5 คุณภาพอากาศในสถานประกอบการ

ลำดับที่ 6 ระดับเสียงในสถานประกอบการ

ลำดับที่ 7 ปริมาณเสียงสะสมติดตัวบุคคล

ตารางสรุปรายการเอกสารการสอบเทียบความถูกต้องของเครื่องมือเก็บตัวอย่าง
และเครื่องมือตรวจวิเคราะห์คุณภาพสิ่งแวดล้อม

รายการตรวจวัด	เครื่องมือเก็บตัวอย่าง	เครื่องมือตรวจวิเคราะห์
	ชื่อเครื่องมือ	ชื่อเครื่องมือ
1. คุณภาพอากาศในบรรยากาศ		
Total Suspended Particulate	High Volume Air Sampler No. B05, B18, R04, R16	Digital Balance
Sulfur Dioxide	SO_2 Analyzer No. B02, B03, B06 Serial No. CM06280010	SO_2 Analyzer No. B02, B03, B06 Serial No. CM06280010
Nitrogen Dioxide	$NO/NO_2/NO_X$ Analyzer No. B02, R05, R08 Serial No. 1170530044	$NO/NO_2/NO_X$ Analyzer No. B02, R05, R08 Serial No. 1170530044
VOCs	Mass Flow Meter	GC/MS
2. คุณภาพอากาศจากแหล่งกำเนิด		
Total Suspended Particulate	Console No. R03 Pitot Tube No. B38	Digital Balance
Oxides of Nitrogen	Vacuum Gauge	Spectrophotometer
Sulfur Dioxide	Personal Pump SKC No. R43, B78 Rotameter No. H-R02	Spectrophotometer
Carbon Monoxide	Personal Pump SKC No. B37, B67 Rotameter No. H-R02	CO Analyzer No. B02
3. คุณภาพน้ำ		
pH	-	pH Meter
BOD_5	-	BOD Analyzer
COD	-	COD Rector
Total Suspended Solids (TSS)	-	Digital Balance
Total Dissolved Solids (TDS)	-	Digital Balance
Grease & Oil	-	Digital Balance
4. ระดับเสียงโดยทั่วไป		
L_{eq} 24 hr และ L_{90}	Acoustic Calibrator Sound Level Meter No. ST-C1-B06, B07	-

ตารางสรุปรายการเอกสารการสอบเทียบความถูกต้องของเครื่องมือเก็บตัวอย่าง
และเครื่องมือตรวจวิเคราะห์คุณภาพสิ่งแวดล้อม

รายการตรวจวัด	เครื่องมือเก็บตัวอย่าง	เครื่องมือตรวจวิเคราะห์
	ชื่อเครื่องมือ	ชื่อเครื่องมือ
5. คุณภาพอากาศในสถานประกอบการ		
1,3-Butadiene	Drycal Flowmeter	Drycal Flowmeter
	GC-FID	GC-FID
6. ระดับเสียงในสถานประกอบการ		
L_{eq} 8 hr, L_{max} และ TWA	Acoustic Calibrator Sound Level Meter ACO No. R40	-
7. ระดับเสียงสะสมแบบติดตัวบุคคล		
Noise Dose	Acoustic Calibrator Sound Level Meter ACO No. R51	-

คุณภาพอากาศในบรรยากาศ

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com.. www.spscon.com

High Volume Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard	Model : TE 5025A	S/N : 3611

Calibration Data				
High Volume Air Sampler Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (ft^3/min)	R^2
B01	B01	02/02/2026	y = 1.147x-3.983	0.998
B02	B02	02/02/2026	y = 1.158x-3.531	0.997
B03	B03	02/02/2026	y = 1.109x-2.595	0.999
B04	B04	02/02/2026	y = 1.123x-1.928	0.998
B05	B05	02/02/2026	y = 1.145x-3.659	0.999
B06	B06	02/02/2026	y = 1.100x-2.379	0.999
B07	B07	02/02/2026	y = 1.122x-2.377	0.999
B08	B08	02/02/2026	y = 1.102x-2.500	0.998
B09	B09	02/02/2026	y = 1.121x-3.479	0.999
B10	B10	02/02/2026	y = 1.143x-3.199	0.996
B11	B11	03/02/2026	y = 1.105x-1.251	0.999
B12	B12	03/02/2026	y = 1.136x-3.106	0.996
B13	B13	03/02/2026	y = 1.142x-2.536	0.998
B14	B14	03/02/2026	y = 1.135x-3.133	0.998
B15	B15	03/02/2026	y = 1.111x-2.932	0.998
B16	B16	04/02/2026	y = 1.104x-3.794	0.998
B17	B17	04/02/2026	y = 1.151x-2.773	0.998
B18	B18	04/02/2026	y = 1.140x-2.730	0.998
B19	B19	04/02/2026	y = 1.137x-2.624	0.998
B20	B20	04/02/2026	y = 1.139x-1.402	0.998
B21	B21	04/02/2026	y = 1.131x-1.657	0.999
B22	B22	04/02/2026	y = 1.166x-3.887	0.997
B23	B23	04/02/2026	y = 1.162x-4.278	0.998
B24	B24	04/02/2026	y = 1.128x-2.436	0.998
B25	B25	04/02/2026	Y = 1.159x-4.833	0.998
B26	B26	03/02/2026	y = 1.103x-1.969	0.997
B27	B27	04/02/2026	y = 1.149x-3.761	0.997
B28	B28	04/02/2026	y = 1.134x-3.377	0.999
B29	B29	04/02/2026	y = 1.118x-2.903	0.997
B30	B30	04/02/2026	y = 1.157x-2.504	0.999
B31	B31	04/02/2026	y = 1.165x-3.108	0.999
B32	B32	04/02/2026	y = 1.113x-2.480	0.999
B33	B33	04/02/2026	y = 1.155x-2.774	0.997
B34	B34	04/02/2026	y = 1.125x-1.905	0.997

Calibrated by :	Approved by :
Adul Dangklom	
(Mr.Adul Dangklom)	(Mr. Peera Detudom)

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com.. www.spscon.com

High Volume Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard	Model : TE 5025A	S/N : 3611

Calibration Data				
High Volume Air Sampler Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (ft^3/min)	R^2
B35	B35	04/02/2026	y = 1.154x-3.696	0.996
B36	B36	04/02/2026	y = 1.119x-2.463	0.997
B37	B37	04/02/2026	y = 1.129x-3.721	0.998
B38	B38	02/02/2026	y = 1.182x-2.931	0.997
B39	B39	02/02/2026	y = 1.062x-1.512	0.999
B40	B40	02/02/2026	y = 1.163x-3.556	0.997
B41	B41	02/02/2026	y = 1.116x-1.975	0.996
B42	B42	02/02/2026	y = 1.152x-4.140	0.997
B43	B43	02/02/2026	y = 1.167x-3.646	0.996
B44	B44	02/02/2026	y = 1.178x-4.362	0.999
R01	R01	02/02/2026	y = 1.097x-2.630	0.997
R02	R02	02/02/2026	y = 1.138x-3.218	0.996
R03	R03	02/02/2026	y = 1.133x-3.084	0.998
R04	R04	02/02/2026	y = 1.121x-2.102	0.998
R05	R05	02/02/2026	y = 1.041x-0.894	0.997
R06	R06	02/02/2026	y = 1.075x-0.254	0.997
R07	R07	03/02/2026	y = 1.126x-2.841	0.996
R08	R08	03/02/2026	y = 1.091x-2.104	0.996
R09	R09	03/02/2026	y = 1.065x+0.557	0.996
R10	R10	03/02/2026	y = 1.093x-1.217	0.999
R11	R11	03/02/2026	y = 1.130x-3.938	0.999
R12	R12	05/02/2026	y = 1.164x-2.698	0.997
R13	R13	05/02/2026	y = 1.120x-3.336	0.998
R14	R14	05/02/2026	y = 1.034x+0.445	0.997
R15	R15	05/02/2026	y = 1.076x+0.429	0.998
R16	R16	05/02/2026	y = 1.107x-1.468	0.996
R17	R17	05/02/2026	y = 1.078x-1.668	0.998
R18	R18	05/02/2026	y = 1.160x-5.001	0.997
R19	R19	05/02/2026	y = 1.077x-2.680	0.997
R20	R20	05/02/2026	y = 1.185x-4.839	0.998

Calibrated by :	Approved by :
Adul Dangklom	
(Mr.Adul Dangklom)	(Mr. Peera Detudom)

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72 Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT

SO_2 FLUORESCENT ANALYZER

DATE :	19 April 2026	BRAND :	API	MODEL :	100A
NO.	SO_2-B02			SERIAL NO.	1847

Calibrator (Dilution System)

Brand	: Teledyne	Model	: 700
Last Cal. Date	: 24 October 2025	Serial No.	: 421

Reference Standard Gas

Standard Gas	: Sulphur Dicxide (SO_2)			Cylinder No.	: A00814SK
Certified Date	: 21 June 2021	Expired Date	: 21 June 2029	Cylinder Conc.	: 49.8 ppm

CALIBRATING CONDITION

Pressure	1011 mmbar	Temp.	24.6 °C	% RH	48

CALIBRATION SETTING

Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.10	-	0	-
SO_2 Span	400.0	400.3	0.075	400.0	1.005

API Model 100A SO_2 Analyzer Check list

Test Values	Observed Value	Units	Nominal Range
RANGE	500	PPB	0-500
SAMPLE PRESS	28.5	in-Hg	25-35
SAMPLE FLOW	654	cc/min	650 ± 10%
PMT	103.2	mV	-20-150 with Zero Air
UV LAMP	2889.6	mV	1000-4900
STR. LGT	61.3	PPB	<100
DRK PMT	62.9	mV	-50 - 200
DRK LMP	57.8	mV	-50 - 200
HVPS	671	V	550-900 constant
DCPS	2518	mV	2500 ± 200
RCELL TEMP	50.2	°C	50 ± 1
BOX TEMP	29.2	°C	5-40
PMT TEMP	7.0	°C	7 ± 2.0
SO_2 Span Conc	400	PPB	20-20,000
SO_2 Slope	1.005	-	1.0 ± 0.3
SO_2 Offset	21.9	mV	<250
Stability at Zero	0.1	PPB	<0.2
Stability at Span	0.2	PPB	0.5% of reading (above 50 ppb)

Calibrated by : Heeson L.
(Mr.Heeson Lormae)

Approved by : Yutthana T.
(Mr.Yutthana Tanatharanit)

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72 Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT

SO_2 FLUORESCENT ANALYZER

DATE :	19 April 2026	BRAND :	API	MODEL :	100A
NO.	SO_2-B03			SERIAL NO.	1846

Calibrator (Dilution System)

Brand	: Teledyne	Model	: 700
Last Cal. Date	: 24 October 2025	Serial No.	: 421

Reference Standard Gas

Standard Gas	: Sulphur Dicxide (SO_2)			Cylinder No.	: A00814SK
Certified Date	: 21 June 2021	Expired Date	: 21 June 2029	Cylinder Conc.	: 49.8 ppm

CALIBRATING CONDITION

Pressure	1010 mmbar	Temp.	24.6 °C	% RH	49

CALIBRATION SETTING

Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.10	-	0	-
SO_2 Span	400.0	400.3	0.075	400.0	1.004

API Model 100A SO_2 Analyzer Check list

Test Values	Observed Value	Units	Nominal Range
RANGE	500	PPB	0-500
SAMPLE PRESS	28.4	in-Hg	25-35
SAMPLE FLOW	656	cc/min	650 ± 10%
PMT	102.8	mV	-20-150 with Zero Air
UV LAMP	2892.5	mV	1000-4900
STR. LGT	61.4	PPB	<100
DRK PMT	62.8	mV	-50 - 200
DRK LMP	57.7	mV	-50 - 200
HVPS	671	V	550-900 constant
DCPS	2517	mV	2500 ± 200
RCELL TEMP	50.2	°C	50 ± 1
BOX TEMP	29.2	°C	5-40
PMT TEMP	7.0	°C	7 ± 2.0
SO_2 Span Conc	400	PPB	20-20,000
SO_2 Slope	1.004	-	1.0 ± 0.3
SO_2 Offset	21.7	mV	<250
Stability at Zero	0.1	PPB	<0.2
Stability at Span	0.2	PPB	0.5% of reading (above 50 ppb)

Calibrated by : Heeson L.
(Mr.Heeson Lormae)

Approved by : Yutthana T.
(Mr.Yutthana Tanatharanit)

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com. www.spscon.com

CALIBRATION REPORT

SO_2 FLUORESCENT ANALYZER

DATE :	19 April 2026	BRAND :	API	MODEL :	100E
NO.	SO_2-B06			SERIAL NO.	3430

Calibrator (Dilution System)

Brand	: Teledyne	Model	: 700
Last Cal. Date	: 24 October 2025	Serial No.	: 421

Reference Standard Gas

Standard Gas	: Sulphur Dicxide (SO_2)			Cylinder No.	: A00814SK
Certified Date	: 21 June 2021	Expired Date	: 21 June 2029	Cylinder Conc.	: 49.8 ppm

CALIBRATING CONDITION

Pressure	1010 mmbar	Temp.	24.6 °C	% RH	49

CALIBRATION SETTING

Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.10	-	0	-
SO_2 Span	400.0	400.2	0.050	400.0	1.008

API Model 100E SO_2 Analyzer Check list

Test Values	Observed Value	Units	Nominal Range
RANGE	500	PPB	0-500
SAMPLE PRESS	28.4	in-Hg	25-35
SAMPLE FLOW	654	cc/min	650 ± 10%
PMT	103.2	mV	-20-150 with Zero Air
UV LAMP	2892.1	mV	1000-4900
STR. LGT	61.5	PPB	<100
DRK PMT	62.8	mV	-50 - 200
DRK LMP	57.6	mV	-50 - 200
HVPS	674	V	550-900 constant
DCPS	2517	mV	2500 ± 200
RCELL TEMP	50.1	°C	50 ± 1
BOX TEMP	29.3	°C	5-40
PMT TEMP	7.0	°C	7 ± 2.0
SO_2 Span Conc	400	PPB	20-20,000
SO_2 Slope	1.008	-	1.0 ± 0.3
SO_2 Offset	21.9	mV	<250
Stability at Zero	0.1	PPB	<0.2
Stability at Span	0.2	PPB	0.5% of reading (above 50 ppb)

Calibrated by : Heeson L.
(Mr.Heeson Lormae)

Approved by : Yutthana T.
(Mr.Yutthana Tanatharanit)

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com. www.spscon.com

CALIBRATION REPORT

CHEMILUMINESCENT NO / NO_2 / NO_X ANALYZER

DATE :	19 April 2026	BRAND :	API	MODEL :	200A
NO.	NOX-B02			SERIAL NO.	2409

Calibrator (Dilution System)

Brand	: Teledyne	Model	: 700
Last Cal. Date	: 24 October 2025	Serial No.	: 421

Reference Standard Gas

Standard Gas	: Nitric Oxide (NO)			Cylinder No.	: A00674SV
Certified Date	: 12 March 2025	Expired Date	: 12 March 2028	Cylinder Conc.	: 48.7 ppm

CALIBRATING CONDITION

Pressure	1011 mmbar	Temp.	24.5 °C	% RH	48

CALIBRATION SETTING

Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.10	-	0	-
NO Span	400	399.8	-0.050	400.0	1.004
NO_X Span	400	400.2	0.050	400.0	1.007

API Model 200A NO_X Analyzer Check List

Test Values	Observed Value	Units	Nominal Range
RANGE	500	PPB	500 standard
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air
SAMPLE FLOW	507	cc/min	500 ± 50
OZONE FLOW	78	cc/min	80 ± 15
PMT	102.9	mV	-20 - 150
AZERO	93.9	mV	-20 - 150
HVPS	670	V	420 - 900 constant
RCELL TEMP	50.3	°C	50 ± 1
BOX TEMP	28.9	°C	8 - 48
PMT TEMP	7.2	°C	7 ± 2
MOLY TEMP	314.9	°C	315 ± 5
RCELL PRESS	8.4	IN-Hg-A	2 - 10 constant
SAMPLE PRESS	28.5	IN-Hg-A	25 - 30 constant
NO Span Conc	400	PPB	20 - 20,000
NO_X Span Conc	400	PPB	20 - 20,000
NO Slope	1.004	-	1.0 ± 0.3
NO_X Slope	1.007	-	1.0 ± 0.3
NO Offset	0.9	mV	-20 to +150
NO_X Offset	0.5	mV	-20 to 150
Stability at Zero	0.1	PPB	< 0.2
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas

Calibrated by : Heeson L.
(Mr.Heeson Lormae)

Approved by : Yutthana T.
(Mr.Yutthana Tanatharanit)

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com. www.spscon.com

CALIBRATION REPORT

CHEMILUMINESCENT NO / NO_2 / NO_X ANALYZER

DATE :	19 April 2026	BRAND :	API	MODEL :	200E
NO.	NOX-R05			SERIAL NO.	4413

Calibrator (Dilution System)

Brand	: Teledyne	Model	: 700
Last Cal. Date	: 24 October 2025	Serial No.	: 421

Reference Standard Gas

Standard Gas	: Nitric Oxide (NO)			Cylinder No.	: A00674SV
Certified Date	: 12 March 2025	Expired Date	: 12 March 2028	Cylinder Conc.	: 48.7 ppm

CALIBRATING CONDITION

Pressure	1010 mmbar	Temp.	24.6 °C	% RH	49

CALIBRATION SETTING

Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.11	-	0	-
NO Span	400	399.7	-0.075	400.0	0.999
NO_X Span	400	400.2	0.050	400.0	1.003

API Model 200E NO_X Analyzer Check List

Test Values	Observed Value	Units	Nominal Range
RANGE	500	PPB	500 standard
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air
SAMPLE FLOW	505	cc/min	500 ± 50
OZONE FLOW	79	cc/min	80 ± 15
PMT	103.7	mV	-20 - 150
AZERO	94.4	mV	-20 - 150
HVPS	670	V	420 - 900 constant
RCELL TEMP	50.3	°C	50 ± 1
BOX TEMP	29.3	°C	8 - 48
PMT TEMP	7.1	°C	7 ± 2
MOLY TEMP	314.9	°C	315 ± 5
RCELL PRESS	8.3	IN-Hg-A	2 - 10 constant
SAMPLE PRESS	28.6	IN-Hg-A	25 - 30 constant
NO Span Conc	400	PPB	20 - 20,000
NO_X Span Conc	400	PPB	20 - 20,000
NO Slope	0.999	-	1.0 ± 0.3
NO_X Slope	1.003	-	1.0 ± 0.3
NO Offset	1.1	mV	-20 to +150
NO_X Offset	0.7	mV	-20 to 150
Stability at Zero	0.1	PPB	< 0.2
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas

Calibrated by : Heeson L.
(Mr.Heeson Lormae)

Approved by : Yutthana T.
(Mr.Yutthana Tanatharanit)

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com. www.spscon.com

CALIBRATION REPORT

CHEMILUMINESCENT NO / NO_2 / NO_X ANALYZER

DATE :	19 April 2026	BRAND :	API	MODEL :	200E
NO.	NOX-R08			SERIAL NO.	243

Calibrator (Dilution System)

Brand	: Teledyne	Model	: 700
Last Cal. Date	: 24 October 2025	Serial No.	: 421

Reference Standard Gas

Standard Gas	: Nitric Oxide (NO)			Cylinder No.	: A00674SV
Certified Date	: 12 March 2025	Expired Date	: 12 March 2028	Cylinder Conc.	: 48.7 ppm

CALIBRATING CONDITION

Pressure	1010 mmbar	Temp.	24.5 °C	% RH	49

CALIBRATION SETTING

Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	-0.10	-	0	-
NO Span	400	399.8	-0.050	400.0	1.005
NO_X Span	400	400.2	0.050	400.0	1.009

API Model 200E NO_X Analyzer Check List

Test Values	Observed Value	Units	Nominal Range
RANGE	500	PPB	500 standard
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air
SAMPLE FLOW	507	cc/min	500 ± 50
OZONE FLOW	78	cc/min	80 ± 15
PMT	103.4	mV	-20 - 150
AZERO	94.2	mV	-20 - 150
HVPS	672	V	420 - 900 constant
RCELL TEMP	50.3	°C	50 ± 1
BOX TEMP	28.6	°C	8 - 48
PMT TEMP	7.4	°C	7 ± 2
MOLY TEMP	315.3	°C	315 ± 5
RCELL PRESS	8.5	IN-Hg-A	2 - 10 constant
SAMPLE PRESS	28.3	IN-Hg-A	25 - 30 constant
NO Span Conc	400	PPB	20 - 20,000
NO_X Span Conc	400	PPB	20 - 20,000
NO Slope	1.005	-	1.0 ± 0.3
NO_X Slope	1.009	-	1.0 ± 0.3
NO Offset	1.0	mV	-20 to +150
NO_X Offset	0.6	mV	-20 to 150
Stability at Zero	0.1	PPB	< 0.2
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas

Calibrated by : Heeson L.
(Mr.Heeson Lormae)

Approved by : Yutthana T.
(Mr.Yutthana Tanatharanit)

Job Number :	J092600062	Customer Name :	IRPC
Equipment :	AQMs Station.	Contact Name :	KhunWirasakKhumsuk
Model :	AQMs Station.	Telephone Number :	081-803-0475
Serial Number :	Pluak Kate Station	E-mail address/Fax. :	wirasak.k@irpc.co.th
Working Date :	20 April 2026	Working Hour :	4 Hours

Service Report

Working Scope:

Service Station

Physical Checking:

- ตรวจเช็ค Data logger พบว่าทำงานได้ปกติ
- ตรวจเช็ค Diagnostic of all analyzers อยู่ในเกณฑ์ปกติ
- ตรวจเช็ค Reading of all analyzers และ Met sensor พบว่าปกติ
- ตรวจเช็ค ผล Calibration พบว่าอยู่ในเกณฑ์ปกติ
- ตรวจเช็ค Dilutor และ Zero Air พบว่าทำงานได้ปกติ
- ตรวจเช็ค เครื่องวัดฝุ่น PM-10 พบว่าทำงานได้ปกติ
- ตรวจเช็ค เครื่อง THC analyzer พบว่าทำงานได้ปกติ
- ตรวจเช็ค การทำงานของระบบไฟฟ้า และ UPS พบว่าทำงานได้ปกติ
- ทำความสะอาดภายในสถานี และ บริเวณรอบสถานี

Correction working:

Calibrate single-point of all analyzers.	Drain water for pump of Zero Air.
Replace sample filter 47 mm.	

Part Replacements:

- Sample Filter 47 mm. 5 ea. (Part support by IRPC)

Addition Recommended:

– End –

Serviced by :	ชิโนรส มุขโรจน์	Serviced Date	20 April 2026
Approved by:		Approved Date :	20 April 2026

บริษัท คิว-ซี โซลูชั่นส์ จำกัด
7/409 ซอยวิภาวดีรังสิต 36 ถนนวิภาวดีรังสิต แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900
โทรศัพท์ : (662) 939-5711 (12 Lines) โทรสาร : (662) 939-4207-8
Website http://www.qshe.co.th E-mail-address: info@qshe.co.th

Q-SHE SOLUTIONS CO., LTD.

General Checking

Equipment :	AQMs Pluak Kate	Model :	-
Serial Number :	Pluak Kate Station	Manufacturer :	-

Item	Description	Set-Point Value	Status & Value	Remark
	On Mobile			
1	Air conditioner operation	OK	OK	
2	Mobile temperature	25-27 °C	26°C	
3	Lighting system	OK	OK	
4	Lamp in sampling box	OK	OK	
5	Sampling probe	Clean	Clean	
6	Blower	OK	OK	
7	Drain liquid in tank	Drain	-	
8	Compressor tank set pressure	80 psi	-	
9	Zero air compressor operation	OK	-	
10	Silica gel for dry air of NO_X analyzer	OK	OK	
11	UPS 3 KVA	OK	OK	
12	Data logger	OK	OK	
13	Ventilation fan	OK	OK	
14	Power cable	OK	OK	
15	Hydrogen Gas	-	400/40 psi	
16	Standard gas#1 (NO,SO_2,HC,CO)	-	1900/32 psi	

Note :

บริษัท คิว-ซี โซลูชั่นส์ จำกัด
7/409 ซอยวิภาวดีรังสิต 36 ถนนวิภาวดีรังสิต แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900
โทรศัพท์ : (662) 939-5711 (12 Lines) โทรสาร : (662) 939-4207-8
Website http://www.qshe.co.th E-mail-address: info@qshe.co.th

$NO-NO_2-NOx$ Analyzer

Equipment :	$NO-NO_2-NOx$ analyzer.	Model :	42i
Serial Number :	1170530044	Manufacturer :	Thermo Scientific

Diagnostic test value				
Parameter	Observed value		Unit	Nominal range
	Before	After		
Sample reading				
NO reading	0.7	14.1	ppb	
NO_X reading	5.0	28.0	ppb	
Range	500	500	ppb	50 to 1000 ppb
Averaging Time	30	30	Sec	10 to 300 Sec
Calibration Factors				
NO BKG. ppb	13.1	13.0	ppb	0 tc 60
NO_X BKG. ppb	13.8	13.8	ppb	0 tc 60
NO COEF.	0.950	0.950	-	1.0 ± 0.3
NOX COEF.	1.000	1.000	-	1.0 ± 0.3
NO2 COEF.	1.000	1.000	-	1.0 ± 0.3
Instrument Controls				
Ozonator	On	On		On/Off
PMT Supply	On	On		On/Off
Auto/Manual Mode	NO/NO_X	NO/NO_X		NO/NOx, NO, NOx
Baud Rate	9600	9600	bps	1200 to 9600
Temp Compensation	On	On	-	On/Off
Pressure Compensation	On	On	-	On/Off
Screen Contrast	45	45	%	0 tc 100
Service Mode	Off	Off	-	On/Off, Up to used
Diagnostics				
Voltages				
PMT Supply	-903.1	-903.2	Vdc	-400 to -1200 Vdc
5 Supply	4.9	4.9	Vdc	5.0 ± 1 Vdc
15 Supply	15.1	15.1	Vdc	15.0 ± 1 Vdc
-15 Supply	-15.0	-15.0	Vdc	-15.0 ± 1 Vdc
Temperatures				
Internal	38.3	38.1	°C	15 °C to 45 °C
Chamber	49.8	49.9	°C	50°C ± 2 °C
Cooler	-2.8	-3.0	°C	(-)3 °C ± 2 °C
Converter	326.8	323.4	°C	325 °C ± 5 °C
Converter Set	325.0	325.0	°C	325 °C
Pressure	233.7	232.4	mmHg	250 ± 100 mmHg
Flow	0.726	0.725	L/min	0.5 to 1.00 L/min

Note :

บริษัท คิว-ซี โซลูชั่นส์ จำกัด
7/409 ซอยวิภาวดีรังสิต 36 ถนนวิภาวดีรังสิต แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900
โทรศัพท์ : (662) 939-5711 (12 Lines) โทรสาร : (662) 939-4207-8
Website http://www.qshe.co.th E-mail-address: info@qshe.co.th

Q-SHE SOLUTIONS CO., LTD.

SO_2 Analyzer

Equipment :	Sulfur Dioxide analyzer.	Model :	43I-BZSAB
Serial Number :	CM06280010	Manufacturer :	Thermo Scientific

Diagnostic test value				
Parameter	Observed value		Unit	Nominal range
	Before	After		
Sample reading	1.9	1.8	ppb	
Range	500	500	ppb	50 to 1000 ppb
Averaging Time	30	30	Sec	10 to 300 Sec
Calibration Factors				
SO_2 BKG. ppb	25.5	25.5	ppb	0 tc 60
SO_2 COEF	1.000	1.000	-	1.0 ± 0.3
Instrument Controls				
Temp Correction	On	On	On/Off	On
Pressure Correction	On	On	On/Off	On
Flash Lamp	On	On	On/Off	On
Communication setting				
Baud Rate	9600	9600	bps	9600 to 115000
Instrument ID	43	43	-	0 tc 99
Screen Brightness	50	50	%	0 tc 100
Service Mode	Off	Off	On/Off	Up to used
Diagnostics				
Voltages				
Motherboard voltages:				
3.3 Supply	3.3	3.3	Vdc	3.3 +/- 1 Vdc
5.0 Supply	5.0	5.0	Vdc	5.0 +/- 1 Vdc
15.0 Supply	15.1	15.1	Vdc	15.0 +/- 1 Vdc
24.0 Supply	23.9	23.9	Vdc	24.0 +/- 1 Vdc
-3.3 Supply	-3.2	-3.2	Vdc	- 3.3 +/- 1 Vdc
Interface board voltages:				
PMT Supply	-601.0	-601.0		
Flash Supply	828	828		
3.3 Supply	3.3	3.3	Vdc	3.3 +/- 1 Vdc
5.0 Supply	5.0	5.0	Vdc	5.0 +/- 1 Vdc
15.0 Supply	14.7	14.7	Vdc	15.0 +/- 1 Vdc
-15.0 Supply	-15.0	-15.0	Vdc	-15.0 +/- 1 Vdc
24.0 Supply	23.9	23.9	Vdc	24.0 +/- 1 Vdc
Temperatures				
Internal	37.0	36.6	°C	15°C to 45°C
Chamber	45.2	45.1	°C	45°C ± 2°C
Pressure	722.4	721.5	mmHg	750 ± 100 mmHg
Flow	0.624	0.624	L/min	0.5 to 1.00 L/min
Lamp intensity	91	92	%	40 – 100 %

Note :

บริษัท คิว-ซี โซลูชั่นส์ จำกัด
7/409 ซอยวิภาวดีรังสิต 36 ถนนวิภาวดีรังสิต แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900
โทรศัพท์ : (662) 939-5711 (12 Lines) โทรสาร : (662) 939-4207-8
Website http://www.qshe.co.th E-mail-address: info@qshe.co.th

SINGLE-POINT GAS CALIBRATION

All analyzer.

Equipment :	All analyzer.	Model :	42C, 43i , 48i, 49i
Serial Number :	0504710413,CM06280010, 1201351403,CM09040067	Manufacturer :	Thermo

Standard gas concentration			Dilutor detail	
Sulfur Dioxide (SO_2)	44.7	ppm	Manufacturer :	Thermo
Nitric Oxide (NO)	45.0	ppm	Model :	146C
Methane (CH_4)	498	ppm	Serial number :	0504710414
Carbon oxide (CO)	4550	ppm		
Cylinder NO. :	A00931SK			
Expiration Date :	8 Sep 2026			

BEFORE CALIBRATION RESULT

PARAMETER	ZERO			SPAN			JUDGEMENT
	IDEAL	ACTUAL	ERROR	IDEAL	ACTUAL	%ERROR	
NO (ppb)	0.00			400			
NO_X (ppb)	0.00			400			
SO_2 (ppb)	0.00			400			
CO (ppm)	0.00			40.3			
O3 (ppb)	0.00			400			
CH4 (ppm)	0.00			5.00			
THC (ppm)	0.00			5.00			

AFTER CALIBRATION RESULT

PARAMETER	ZERO			SPAN			JUDGEMENT
	IDEAL	ACTUAL	ERROR	IDEAL	ACTUAL	%ERROR	
NO (ppb)	0.00	1.0	1.00	400	399.0	-0.25	Valid
NO_X (ppb)	0.00	1.9	1.90	400	405.0	1.25	Valid
SO_2 (ppb)	0.00	1.2	1.20	400	401.0	0.25	Valid
CO (ppm)	0.00	0.20	0.20	40.3	40.2	-0.25	Valid
O3 (ppb)	0.00	1.0	1.00	400	400.0	0.00	Valid
CH4 (ppm)	0.00	0.00	0.00	5.00	4.98	-0.40	Valid
THC (ppm)	0.00	0.00	0.00	5.00	5.00	0.00	Valid

Remark :

บริษัท คิว-ซี โซลูชั่นส์ จำกัด
7/409 ซอยวิภาวดีรังสิต 36 ถนนวิภาวดีรังสิต แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900
โทรศัพท์ : (662) 939-5711 (12 Lines) โทรสาร : (662) 939-4207-8
Website http://www.qshe.co.th E-mail-address: info@qshe.co.th

Q-SHE SOLUTIONS CO., LTD.

ภาพถ่ายการเข้าปฏิบัติงานตามแผนการบำรุงรักษา

Stations Pluakgate IRPC



Inside Station



Lamp Sampling Box



Replace Filter



Gas H_2



Gas STD.



บริษัท คิว-ซี โซลูชั่นส์ จำกัด
7/409 ซอยวิภาวดีรังสิต 36 ถนนวิภาวดีรังสิต แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900
โทรศัพท์ : (662) 939-5711 (12 Lines) โทรสาร : (662) 939-4207-8
Website http://www.qshe.co.th E-mail-address: info@qshe.co.th

MIRACLE INTERNATIONAL TECHNOLOGY CO.,LTD
214 Bangwaek Rd. Bangpai Bangkae Bangkok 10160
Tel.: 0-2865-4647-8 Fax: 0-2865-4649 http://www.mit.in.th

NSC-TISI-TIS 17025
CALIBRATION 0052

CALIBRATION CERTIFICATE

Certificate No. : L202511307-0001

Date Issued : 01-Dec-25

Customer	:	S.P.S. CONSULTING SERVICE CO., LTD. 7 Soi Phaholyothin 24 Phaholyothin Road., Jompol, Chatuchak, Bangkok 10900
Equipment	:	Mass Flow meter
Manufacturer	:	Dwyer
Model	:	GMF-2101
Serial No.	:	-
ID No./Tag No.	:	MF01/51
Date Received	:	27-Nov-25
Date Calibrated	:	30-Nov-25
Calibrated by	:	Nattawat Laochai

Calibration Method or Calibration Procedure Used

In-house method : CP-34 by comparison against mass flow calibrator.

This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

Result of Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor k = 2, providing a level confidence approximately 95 percent.

This certificate may not be reproduced other than in full except with the prior written approval of the Miracle International Technology Company Limited.

Approved by: K. Nathapong (Nathapong Krudaum)

CERTIFIED MIT

Certificate No. : L202511307-0001

Ambient Temperature : (25 ± 2)°C

Relative Humidity : (50 ± 15)%RH

Capacity Range : 17 ml/min

Calibration Media : Nitrogen


Type : Mass Flowmeter

Unit Under Calibration Reference Condition : Pressure 101.325 kPa(abs) , 21 °C , Nitrogen

Temperature (°C)	Pressure (kPa)	UUC Reading (ml/min)	STD Reading (ml/min)	Error (ml/min)	Uncertainty (± ml/min)
24.69	101.22	0.00	0.000 *	0.000	0.063
24.44	119.03	3.30	3.358	-0.058	0.14
24.38	118.17	7.30	7.4	-0.10	0.15
24.30	156.08	13.50	13.6	-0.10	0.15
24.25	169.92	17.00	17.1	-0.10	0.18

Error = Unit Under Calibration - Standard

Marked * are not included in the NSC-ONSC accreditation schedule for our laboratory.

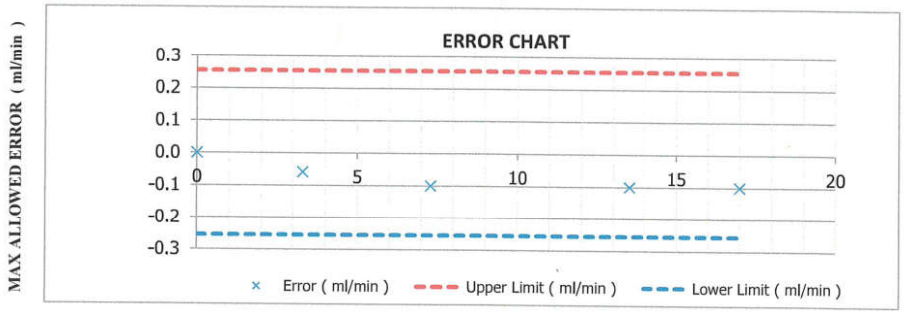

Certificate No. : L202511307-0001

Note : The actual flow rate is determined by the equation :

$$Q_{Meas} = Q_{Ref} \times \frac{P_{Ref}}{P_{Meas}} \times \frac{T_{Meas}}{T_{Ref}}$$

; Q = Flow rate

; P = Absolute pressure

; T = Absolute temperature

; Subscript "Meas" = Measurement condition

; Subscript "Ref" = Reference condition

Condition As-Received : Used Item

The measurment results and statements of conformity with specification only relate to the item calibrated.

Traceability of Certificate :

The International System of Units (SI) through

NIMT Calibration Certificate No. MW-0047-24 for Gas Flow meter Serial No. M5209179B/M5209179A, Due 28-Jun-26

NIMT Calibration Certificate No. MW-0048-24 for Gas Flow meter Serial No. M5209179C/M5209179A, Due 02-Jul-26

End of Certificate

QUALITY CALIBRATION CO.,LTD.
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584
www.qcalibration.com

ilac-MRA

NSC-TISI-TIS17025
CALIBRATION 0049

CERTIFICATE No : 26M2266
REFERENCE No : 80204-1

Certificate of Calibration

EQUIPMENT	:	DIGITAL BALANCE
MANUFACTURER	:	METTLER TOLEDO
MODEL	:	XS105DU
SERIAL No	:	1126422905
ID No	:	BA 05/50
CONDITION AS RECEIVED	:	USED ITEM
SUBMITTED BY	:	S.P.S. CONSULTING SERVICE CO., LTD. 7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD., JOMPOL, CHATUCHAK, BANGKOK 10900
CALIBRATED BY	:	SUCHAT S.
CALIBRATION DATE	:	05-Mar-26
APPROVED BY	:	PONGSAK J.
ISSUED DATE	:	06-Mar-26
RECEIVED DATE	:	05-Mar-26

Certificate

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF QUALITY CALIBRATION CO., LTD.

QUALITY CALIBRATION CO.,LTD.
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584
www.qcalibration.com

CERTIFICATE No : 26M2266

Calibration Report

EQUIPMENT	:	DIGITAL BALANCE	**MODEL**	:	XS105DU
MANUFACTURER	:	METTLER TOLEDO	**S/N**	:	1126422905
ID No	:	BA 05/50	**RECEIVED DATE**	:	05-Mar-26
AIR PRESSURE	:	1004mbar ± 1mbar	**CALIBRATION DATE**	:	05-Mar-26
AMBIENT TEMPERATURE	:	25° C ± 1° C	**RELATIVE HUMIDITY**	:	50 %RH ± 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARLITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.
2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	C02250116	28-Jan-27
2) STANDARD WEIGHT	E2	15843	C02250117	29-Jan-27


3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
   - NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL
2. TARE FUNCTION : NORMAL
3. REPEATABILITY OF READING AT 120 g WAS 0.000055 g
4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (± g)
0.00	0.00000	0.00000	0.000065
0.02	0.02000	0.00000	0.000065
0.10	0.10000	0.00000	0.000066
0.20	0.20000	0.00000	0.000066
0.50	0.50001	-0.00001	0.000065
1.00	1.00001	-0.00001	0.000066
2.00	2.00000	0.00000	0.000067
5.00	5.00001	-0.00001	0.000068
10.00	10.00004	-0.00004	0.000070
20.00	20.00006	-0.00006	0.000078
50.00	50.0000	0.0000	0.00012
100.00	100.0002	-0.0002	0.00019
120.00	120.0002	-0.0002	0.00022

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.0000
2	50.0000
3	50.0000
4	50.0000
5	50.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k =2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

Copy

PerkinElmer

GC Clarus 600/680 Preventive Maintenance (PM)

Company Name:	**S.P.S. Consulting Service Co.,Ltd**		
Address (Instrument Location):	7 Soi Phaholyothin24 Phaholyothin Road, Jompol, Chatuchak, Bangkok, 10900.		
Serial Number:	680S14042502	**Service Tag:**	N68APSSFXMP
Customer Name (if applicable):	Ms.Naruecha	**PM number:**	2 of 2
Service Engineer Name:	Monchai Kitcharoenkeat	**Service Order Number:**	WO-06815714
Date PM Performed: (DD-MMM-YYYY)	13-Aug-2025	**Next PM Due Date:** (DD-MMM-YYYY)	13-Feb-2026

Part Number	Release	Publication Date	
TH09370070	C	August 2016	PerkinElmer

Scope
The purpose of this PM is to ensure the continued functionality of the Clarus 600 and Clarus 680 GC by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer. The customer should save their method before the PM begins.

General Instructions:
The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM. Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files. The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer. Update the PM sticker and instrument logbook as required.

Copyright Information
This document contains proprietary information that is protected by copyright. All rights are reserved. No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of Perkin Elmer, Inc. **Copyright © 2013 PerkinElmer, Inc.**

Trademarks
Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners. **Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no Warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.** PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

PerkinElmer

Component List

Component / Specific Model	Serial #	Software Version	Configuration Notes
Clarus680	680S14042502	Totalchrom6.3.2	PSS, PSS, FID,
Clarus SQ8T	648N4050804	Turbomass 6.4	
AtomX	US14113002	Tekma AtomX	

Parts Lists

Additional Tools Required for PM				
Part Number (if applicable)	**Description**	**Quantity**	**Serial #**	**Calibration Due Date (MM/YY)**
N/A				
Additional Reagents and Standards Required for PM				
Part Number (if applicable)	**Description**	**Quantity**	**Batch/Lot #**	**Expiration Date (MM/YY)**
N/A				

PerkinElmer

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. **General:**

☑ Review the instrument performance with the customer and document any recent problems.

☑ Check incoming AC line voltage for proper levels and grounding.
L-N 220 Volt
L-G 220 Volt
N-G 0.32 Volt

**Neutral to ground not more than 0.5 volts peak to peak*

☑ Inspect all gas line filters and traps; Replace if necessary with customer supplied spares.
Carrier gas ☑ Helium ☐ Nitrogen ☐ Hydrogen
Moisture level ☑ Good ☐ Need to replace ☐ Other _____

Detector gas ☑ Air Zero ☑ Hydrogen ☐ Nitrogen ☐ Helium
Moisture level ☑ Good ☐ Need to replace ☐ Other _____

☑ Inspect the customer log book and make any appropriate PM entries.

☑ Leak check all fittings from the gas source to instrument.
Gas leakage ☑ Pass ☐ Fail Comment _____

☑ Perform general inspection of system for cleanliness.

☑ Inspect for functional and clean electronic cooling and oven vent fans
Electronic cooling fan ☑ Yes ☐ No
Oven cooling fan ☑ Yes ☐ No

2. **Electronic :**

☑ Check oven temperature. Calibrate if necessary.
Oven temperature set point 150 ^{0}C ☑ Pass ☐ Fail

☐ Check sub-ambient option. (If installed).
Oven temperature set point 5 ^{0}C ☐ Pass ☐ Fail

☑ Perform routine maintenance on detector/injector. Replace parts as necessary with customer supplied spares.

☑ Check flows, including split flows if applicable. Calibrate if necessary.
Carrier flow Pass
Split flow Pass

☑ Check detector gas flows and adjust if necessary.
Detector flow Pass

☑ Autosampler installed ☑ Yes ☐ No
Check autosampler sensor for wear and replace if necessary.
Vial sensor Pass
Door sensor Pass
Tower sensor Pass
Plunger sensor Pass
Elevator sensor Pass

☑ Remove syringe, manually flush. Replace with customer supplied spare if necessary.

☑ Check firmware version. Upgrade to current levels if necessary.
Firmware version 6.5

☑ Measure all accessible power supply voltages.
5 Volt Pass
+15 Volt Pass
-15 Volt Pass
24 Volt Pass

☑ Record all detector voltage signal.
Detector Channel A 0.98 mV.
Detector Channel B NA mV.

3. Diagnostics Tests:

☑ Run instrument diagnostics.
☑ BRAM Pass
☑ EPROM Pass

☑ Run Autosampler diagnostics.
☑ BRAM Pass
☑ EPROM Pass

4. Review:

☑ Review with the customer PM work performed.
☑ Review with the customer routine maintenance procedures.
☑ Discuss recommended customer-supplied materials to have on hand
☑ Attach PM sticker.
☑ Update Logbook.

Additional Comments

Additional Comments Regarding the PM

Review

The preventive maintenance checks and if applicable performance tests for Clarus600/680 GC have been completed. ***This Clarus600/680 GC*** **Pass** ***the preventive maintenance.***	
Review of Preventive Maintenance:	
Authorized PerkinElmer Representative: Monchai Kitcharoenkeat *Monchai*	Date: 13-Aug-2025 (DD-MMM-YYYY)
Authorized Customer Representative: Ms.Naruecha *Naruecha*	Date: 13-Aug-2025 (DD-MMM-YYYY)

PerkinElmer®

GC Clarus 600/680 Preventive Maintenance (PM)

Company Name:	**S.P.S. Consulting Service Co.,Ltd**		
Address (Instrument Location):	7 Soi Phaholyothin24 Phaholyothin Road, Jompol, Chatuchak, Bangkok, 10900.		
Serial Number:	680S14042502	**Service Tag:**	N68APSSFXMP
Customer Name (if applicable):	Ms.Naruecha	**PM number:**	1 of 2
Service Engineer Name:	Monchai Kitcharoenkeat	**Service Order Number:**	WO-11858723
Date PM Performed: (DD-MMM-YYYY)	13-Feb-2026	**Next PM Due Date:** (DD-MMM-YYYY)	13-Aug-2026

Part Number	Release	Publication Date	
TH09370070	C	August 2016	PerkinElmer®

Scope

The purpose of this PM is to ensure the continued functionality of the Clarus 600 and Clarus 680 GC by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer. The customer should save their method before the PM begins.

General Instructions:

The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM. Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files. The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer. Update the PM sticker and instrument logbook as required.

Copyright Information

This document contains proprietary information that is protected by copyright. All rights are reserved. No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of Perkin Elmer, Inc. **Copyright © 2013 PerkinElmer, Inc.**

Trademarks

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners. **Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no Warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.** PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

PerkinElmer®

Component List

Component / Specific Model	Serial #	Software Version	Configuration Notes
Clarus680	680S14042502	Totalchrom6.3.2	PSS, PSS, FID,
Clarus SQ8T	648N4050804	Turbomass 6.4	
AtomX	US14113002	Tekma AtomX	

Parts Lists

Additional Tools Required for PM				
Part Number (if applicable)	**Description**	**Quantity**	**Serial #**	**Calibration Due Date** (MM/YY)
N/A				
Additional Reagents and Standards Required for PM				
Part Number (if applicable)	**Description**	**Quantity**	**Batch/Lot #**	**Expiration Date** (MM/YY)
N/A				

PerkinElmer®

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. General:

☑ Review the instrument performance with the customer and document any recent problems.

☑ Check incoming AC line voltage for proper levels and grounding.
L-N 220 Volt
L-G 220 Volt
N-G 0.46 Volt

**Neutral to ground not more than 0.5 volts peak to peak*

☑ Inspect all gas line filters and traps; Replace if necessary with customer supplied spares.
Carrier gas ☑ Helium ☐ Nitrogen ☐ Hydrogen
Moisture level ☑ Good ☐ Need to replace ☐ Other _____

Detector gas ☑ Air Zero ☑ Hydrogen ☐ Nitrogen ☐ Helium
Moisture level ☑ Good ☐ Need to replace ☐ Other _____

☑ Inspect the customer log book and make any appropriate PM entries.

☑ Leak check all fittings from the gas source to instrument.
Gas leakage ☑ Pass ☐ Fail Comment _____

☑ Perform general inspection of system for cleanliness.

☑ Inspect for functional and clean electronic cooling and oven vent fans
Electronic cooling fan ☑ Yes ☐ No
Oven cooling fan ☑ Yes ☐ No

2. Electronic :

☑ Check oven temperature. Calibrate if necessary.
Oven temperature set point 150 ^{0}C ☑ Pass ☐ Fail

☐ Check sub-ambient option. (If installed).
Oven temperature set point 5 ^{0}C ☐ Pass ☐ Fail

☑ Perform routine maintenance on detector/injector. Replace parts as necessary with customer supplied spares.

PerkinElmer®

☑ Check flows, including split flows if applicable. Calibrate if necessary.
Carrier flow Pass
Split flow Pass

☑ Check detector gas flows and adjust if necessary.
Detector flow Pass

☑ Autosampler installed ☑ Yes ☐ No
Check autosampler sensor for wear and replace if necessary.
Vial sensor Pass
Door sensor Pass
Tower sensor Pass
Plunger sensor Pass
Elevator sensor Pass

☑ Remove syringe, manually flush. Replace with customer supplied spare if necessary.

☑ Check firmware version. Upgrade to current levels if necessary.
Firmware version 6.5

☑ Measure all accessible power supply voltages.
5 Volt Pass
+15 Volt Pass
-15 Volt Pass
24 Volt Pass

☑ Record all detector voltage signal.
Detector Channel A 0.87 mV.
Detector Channel B NA mV.

3. Diagnostics Tests:

☑ Run instrument diagnostics.
☑ BRAM Pass
☑ EPROM Pass

☑ Run Autosampler diagnostics.
☑ BRAM Pass
☑ EPROM Pass

4. Review:

☑ Review with the customer PM work performed.
☑ Review with the customer routine maintenance procedures.
☑ Discuss recommended customer-supplied materials to have on hand
☑ Attach PM sticker.
☑ Update Logbook.

PerkinElmer®

Additional Comments

Additional Comments Regarding the PM

Review

The preventive maintenance checks and if applicable performance tests for Clarus600/680 GC have been completed. ***This Clarus600/680 GC*** **Pass** ***the preventive maintenance.***	
Review of Preventive Maintenance:	
Authorized PerkinElmer Representative: Monchai Kitcharoenkeat	Date: 13-Feb-2026 (DD-MMM-YYYY)
Authorized Customer Representative: Ms.Naruecha	Date: 13-Feb-2026 (DD-MMM-YYYY)

คุณภาพอากาศจากแหล่งกำเนิด

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com.. www.spscon.com

Console Calibration Report

Calibration Method	Critical Orifices

Calibration Data				
Console Data		Calibration Data		
No.	Serial No.	Date	y	$\Delta H_@$ (mmH_2O)
B01	1563	02/03/2026	0.998	49.85
B02	8002514	02/03/2026	1.003	49.77
B03	1503016	03/03/2026	0.997	49.68
B04	00006659	03/03/2026	0.996	49.82
B05	00007428	02/03/2026	0.999	49.65
R01	1561	03/03/2026	1.002	49.98
R02	8002513	03/03/2026	1.004	49.56
R03	1570	03/03/2026	0.997	49.73
R04	8002519	03/03/2026	0.999	49.80
R05	1503015	02/03/2026	1.003	49.95

Remark : Accept Value of y (test) is $0.97 < y < 1.03$

Accept Value of $\Delta H_@$ (test) is 46.7 ± 6.4 (mmH_2O)

Calibrated by :	Approved by :
Adul Dangklom	
(Mr. Adul Dangklom)	(Mr. Peera Detudom)

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com.. www.spscon.com

Pitot Tube Calibration Report

Calibration Method	Standard Pitot Tube

Calibration Data					
Pitot Tube Data			Calibration Data		
No.	Type of Pitot	Coefficience of Standard Pitot	Date	Avg. of Cp (test)	
				Side A	Side B
B36	S	0.99	04/02/2026	0.85	0.84
B37	S	0.99	02/02/2026	0.84	0.83
B38	S	0.99	03/02/2026	0.83	0.84
B39	S	0.99	03/02/2026	0.85	0.84
B40	S	0.99	02/02/2026	0.84	0.84
B41	S	0.99	02/02/2026	0.83	0.84
B44	S	0.99	04/02/2026	0.84	0.84
B45	S	0.99	04/02/2026	0.85	0.84
B46	S	0.99	04/02/2026	0.83	0.84
B47	S	0.99	04/02/2026	0.84	0.85
B48	S	0.99	03/02/2026	0.84	0.84
B49	S	0.99	03/02/2026	0.85	0.84
B54	S	0.99	02/02/2026	0.84	0.84
B56	S	0.99	02/02/2026	0.84	0.83
B57	S	0.99	03/02/2026	0.84	0.85
B58	S	0.99	03/02/2026	0.84	0.84

Remark : Accept value of Cp (test) is 0.84 ± 0.01

Calibrated by :	Approved by :
Adul Dangklom	
(Mr. Adul Dangklom)	(Mr. Peera Detudom)

CALIBRATION LABORATORY Co.,LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-G353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com

CLC Accredited ISO/IEC17025

ilac-MRA

ANAB ACCREDITED CALIBRATION AND DIMENSIONAL MEASUREMENT ACDM-28 14

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE	VACUUM GAUGE
MANUFACTURER	HI-LIGHT
MODEL/TYPE	N/A
SERIAL NO.	N/A[64-220088-1]
CLID.NO.	212301422
JOB CONTROL NO.	240720076546

CUSTOMER S.P.S. CONSULTING SERVICE CO., LTD.
7SOI PHAHOLYOTHrN 24 ROAD., JOMPOL,
CHATUCHAK, BANGKOK 10900

DATE OF RECEIVED : 19 July 2025 **DATE OF ISSUED: 24 July 2025**

The report or calibration shall not be reproduced except in full without approval of the Calib.-ation Laborator·y Co., Ltd.

Calibrated By : Sittipong Pimdee
Calibration Engineer

Approved By : Mongkol Yotsoontorn
Authorized Signatory
24 July 2025

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

CALIBRATION LABORATORY Co., LTD.
211Q-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-Q353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com

CLC AccredUed ISO/IEC 17025

ilac-MRA

ANAB CALIBRATION AND DIMENSIONAL MEASUREMENT ACDM-2814

REPORT OF CALIBRATION

FOR

NOMENCLATURE	VACUUM GAUGE
MANUFACTURER	HI-LIGHT
MODEL/TYPE	N/A
SERIAL NO.	N/A [64-220088-1]
DATE OF CALIBRATION	23 July 2025
DUE DATE OF CALIBRATION	23 July 2026

ENVIRONMENT CONDITIONS

Temperature : (23 ± 2) °C Relative Humidity (55± 10) %RH

PROCEDURE USED :

This instrument was calibrated under procedure No. CLC-CPPP-05 according to DKD-R 6-1 as calibration guidelines. The calibration was performed by direct measurement with Document Process Calibrator and Pressure Module which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

Document Process Calibrator, Fluke Model 74 1B *SIN.* 8295020 with Pressure Module Model 700PD5 *SIN.* 89404505.

TRACEABILITY :

The measurement s are traceable to International System of Units (SI), through National Institute of Metrology (Thailand). Certificate No. MP-0040-24.

UNCERTAINTY :

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor of $k = 2$. Ithas been evaluated according to the "Calibration of Pressure Gauges (DKD-R 6-1)" which provides a level of confidence approximately 95%.

CALIBRATION LABORATORY Co., LTD.
2/1Q-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-D353-4 Fax:02-578-2672 ww.w.caHaboratory.com E-mail:sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
ilac-MRA ANAB ACCREDITED CALIBRATION AND DIMENSIONAL MEASUREMENT ACDM-2814

CONDITION OF CALIBRATION ITEM :RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS: (X) without adjustment ( ) adjustment

The DUC was exercised by applying a known pressure from its zero to full scale 1 times. Then 2 series of known gauge pressure were applied. The STD reading were recorded and the means value were reported in the table below.

CALIBRATION DATA

CORRECTION OF PRESSURE

DUC Test point	STD Reading (kPa)		Conversion to inHg		Correction (inHg)	
(inHg)	Up	Down	Up	Down	Up	Down
0	0.00	0.00	0.0	0.0	0.0	0.0
-5	-15.07	-15.10	-4.5	-4.5	+0.5	+0.5
-10	-32.50	-32.84	-9.6	-9.7	+0.4	+0.3
-15	-49.44	-49.77	-14.6	-14.7	+0.4	+0.3
-20	-66.70	-66.70	-19.7	-19.7	+0.3	+0.3
-25	-83.63	-83.97	-24.7	-24.8	+0.3	+0.2
-30	-100.39	-100.39	-29.6	-29.6	+0.4	+0.4

Uncertainty of measurement± 0.2 inHg

Transmitting fluid : Air.

Technical Note. Conversion factor 1 kPa ; 0.2953003 inHg

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 012 Page 43 of 67

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q24076546

F3-011-05/ 12-23

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72 Fax : (662) 513-4221, E-mail : sale@spscon.com , www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter	Model : Defender 510-H	S/N : 136833

Environmental Conditions

Temperature	25	± 3	°C
Pressure	1010	± 15	mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R^2
R01	SKC	224-PCXR4	602467	01/04/2026	1,000	1,500	2,000	1,001	1,500	2,007	1.005x - 6.003	1.000
R02	SKC	224-PCXR4	626450	05/04/2026	1,000	2,000	3,000	1,000	1,503	2,001	1.001x - 0.383	1.000
R03	SKC	224-PCXR4	691592	03/04/2026	1,000	1,500	2,000	1,005	1,501	2,000	1.007x - 15.384	0.999
R04	SKC	224-PCXR4	691672	03/04/2026	1,000	1,500	2,000	1,007	1,513	1,999	0.996x + 5.855	0.999
R05	SKC	224-PCXR4	798470	05/04/2026	1,000	1,500	2,000	1,000	1,499	1,997	0.997x + 3.107	1.000
R06	SKC	224-PCXR4	798456	03/04/2026	1,000	1,500	2,000	998	1,497	1,996	0.998x + 0.120	1.000
R07	SKC	224-PCXR4	798480	05/04/2026	1,000	1,500	2,000	1,002	1,506	2,001	0.999x + 3.219	1.000
R08	SKC	224-PCXR4	883215	03/04/2026	1,000	1,500	2,000	1,004	1,501	1,992	1.003x - 9.877	0.999
R09	SKC	224-PCXR4	034650	03/04/2026	1,000	1,500	2,000	998	1,506	2,003	1.004x - 5.723	1.000
R10	SKC	224-PCXR4	091765	03/04/2026	1,000	1,500	2,000	999	1,507	1,996	1.005x - 13.080	0.999
R11	SKC	224-PCXR4	091763	05/04/2026	1,000	1,500	2,000	1,001	1,504	2,001	1.000x + 0.104	1.000
R12	SKC	224-PCXR4	091568	03/04/2026	1,000	1,500	2,000	998	1,505	1,996	0.998x + 1.482	1.000
R13	SKC	224-PCXR4	091638	03/04/2026	1,000	1,500	2,000	1,001	1,504	2,000	0.999x + 2.097	1.000
R14	SKC	224-PCXR4	091764	05/04/2026	1,000	1,500	2,000	1,007	1,505	2,001	1.004x - 8.866	0.999
R15	SKC	224-PCXR8	529457	05/04/2026	1,000	1,500	2,000	998	1,492	1,999	1.001x - 6.322	1.000
R16	SKC	224-PCXR8	529643	03/04/2026	1,000	1,500	2,000	1,004	1,506	2,004	1.007x - 11.726	0.999
R17	SKC	224-PCXR8	529645	05/04/2026	1,000	1,500	2,000	998	1,503	1,998	1.000x - 0.703	1.000
R18	SKC	224-PCXR8	566756	03/04/2026	1,000	1,500	2,000	999	1,508	1,995	1.002x - 8.012	0.999
R19	SKC	224-PCXR8	566802	05/04/2026	1,000	1,500	2,000	998	1,502	1,998	1.000x - 0.823	1.000
R20	SKC	224-PCXR8	529089	03/04/2026	1,000	1,500	2,000	999	1,503	1,996	0.997x + 2.001	1.000
R21	SKC	224-PCXR8	665728	03/04/2026	1,000	1,500	2,000	998	1,505	1,999	1.000x - 0.483	1.000
R22	SKC	224-PCXR8	707444	05/04/2026	1,000	1,500	2,000	1,007	1,496	2,000	1.001x - 6.418	0.999
R23	SKC	224-PCXR8	761067	05/04/2026	1,000	1,500	2,000	1,001	1,502	2,004	1.002x - 1.446	1.000
R24	SKC	224-PCXR8	707893	03/04/2026	1,000	1,500	2,000	1,002	1,503	2,001	0.999x + 2.560	1.000
R25	SKC	224-PCXR8	761052	03/04/2026	1,000	1,500	2,000	1,009	1,504	2,005	0.997x + 4.106	0.999
R26	SKC	224-PCXR8	707956	05/04/2026	1,000	1,500	2,000	1,002	1,503	2,000	0.998x + 4.497	1.000
R27	SKC	224-PCXR8	707398	03/04/2026	1,000	1,500	2,000	1,001	1,505	2,004	1.003x - 1.921	1.000
R28	SKC	224-PCXR8	707481	05/04/2026	1,000	1,500	2,000	1,010	1,513	2,006	0.997x + 5.531	0.999
R29	SKC	224-PCXR8	707402	03/04/2026	1,000	1,500	2,000	1,003	1,502	1,992	1.003x - 10.216	0.999
R30	SKC	224-PCXR8	093811	05/04/2026	1,000	1,500	2,000	999	1,512	2,005	1.007x - 9.705	1.000
R31	SKC	224-PCXR8	093183	05/04/2026	1,000	1,500	2,000	1,011	1,510	2,011	1.001x + 2.983	0.999
R32	SKC	224-PCXR8	671950	03/04/2026	1,000	1,500	2,000	1,001	1,500	2,001	0.999x + 2.272	1.000
R33	SKC	224-PCXR4	626254	05/04/2026	1,000	1,500	2,000	998	1,507	2,002	1.005x - 10.975	1.000
R34	SKC	224-PCXR4	626131	05/04/2026	1,000	1,500	2,000	997	1,496	2,000	1.007x - 14.230	1.000
R35	SKC	224-PCXR8	707460	05/04/2026	1,000	1,500	2,000	998	1,509	1,996	1.000x - 2.915	1.000
R36	SKC	224-PCXR8	707446	05/04/2026	1,000	1,500	2,000	1,003	1,492	2,003	1.007x - 16.135	0.999
R37	SKC	224-PCXR8	707432	03/04/2026	1,000	1,500	2,000	999	1,507	2,005	1.003x - 6.095	1.000
R38	SKC	224-PCXR8	707349	03/04/2026	1,000	1,500	2,000	1,003	1,499	1,999	0.997x + 2.141	1.000
R39	SKC	224-PCXR8	761095	05/04/2026	1,000	1,500	2,000	1,005	1,508	2,004	1.000x - 0.152	0.999

Calibrated by :	Approved by :
Adul Dangklom (Mr. Adul Dangklom)	(Mr. Peera Detudom)

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com.. www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter | Model : Defender 510-H | S/N : 136833

Environmental Conditions
Temperature . 25 ± 3 °C
Pressure . 1010 ± 15 mmbar

Personal Pump Data				Calibration Data							
					Flow Rate (ml/min)						
					Setting			Actual (Q std.)			Value From Calibration Curve
No.	Brand	Model	Serial No.	Date	1	2	3	1	2	3	y	R^2
R40	SKC	224-PCXR4	612753	05/04/2026	1,000	1,500	2,000	1,004	1,457	2,000	0.998x + 1.430	1.000
R41	SKC	224-PCXR4	626140	03/04/2026	1,000	1,500	2,000	998	1,498	1,997	0.999x + 0.943	1.000
R42	SKC	224-PCXR4	626463	05/04/2026	1,000	1,500	2,000	1,005	1,513	1,998	0.997x + 4.138	0.999
R43	SKC	224-PCXR4	626129	03/04/2026	1,000	1,500	2,000	1,003	1,498	2,000	0998x + 2.029	1.000
R44	SKC	224-PCXR4	602753	03/04/2026	1,000	1,500	2,000	996	1,509	1,997	1.003x - 8.036	1.000
R45	SKC	224-PCXR4	626137	05/04/2026	1,000	1,500	2,000	1,011	1,514	2,005	0.995x + 8.367	0.999

Calibrated by : Adul Dangklom (Mr. Adul Dangklom)

Approved by : (Mr. Peera Detudom)

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com.. www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter | Model : Defender 510-H | S/N : 136164

Environmental Conditions
Temperature . 25 ± 3 °C
Pressure . 1010 ± 15 mmbar

Personal Pump Data				Calibration Data							
					Flow Rate (ml/min)						
					Setting			Actual (Q std.)			Value From Calibration Curve
No.	Brand	Model	Serial No.	Date	1	2	3	1	2	3	y	R^2
B41	SKC	224-PCXR4	612669	03/04/2026	1,000	1,500	2,000	996	1,498	1,991	1.006x - 15.132	0.999
B42	SKC	224-PCXR4	626041	03/04/2026	1,000	1,500	2,000	998	1,495	1,998	1.001x - 5.029	1.000
B43	SKC	224-PCXR4	034636	03/04/2026	1,000	1,500	2,000	996	1,512	1,995	1.000x - 4.272	0.999
B44	SKC	224-PCXR8	529341	03/04/2026	1,000	1,500	2,000	1,000	1,501	2,000	0.999x + 0.802	1.000
B45	SKC	224-PCXR8	529594	03/04/2026	1,000	1,500	2,000	996	1,495	1,999	1.003x - 8.918	1.000
B46	SKC	224-PCXR8	566743	03/04/2026	1,000	1,500	2,000	998	1,501	1,992	1.006x - 12.300	0.999
B47	SKC	224-PCXR8	566747	03/04/2026	1,000	1,500	2,000	996	1,505	2,000	1.004x - 8.392	1.000
B48	SKC	224-PCXR8	566753	03/04/2026	1,000	1,500	2,000	1,011	1,508	2,008	0.998x + 4.726	0.999
B49	SKC	224-PCXR8	566780	03/04/2026	1,000	1,500	2,000	997	1,495	1,999	1.003x - 8.045	1.000
B50	SKC	224-PCXR8	500400	03/04/2026	1,000	1,500	2,000	1,000	1,499	1,994	0.996x + 3.906	1.000
B51	SKC	224-PCXR8	500363	03/04/2026	1,000	1,500	2,000	997	1,505	1,997	1.005x - 14.055	0.999
B52	SKC	224-PCXR8	093186	03/04/2026	1,000	1,500	2,000	996	1,506	2,000	1.002x - 5.484	1.000
B53	SKC	224-PCXR8	707670	03/04/2026	1,000	1,500	2,000	993	1,505	2,001	1.009x - 20.477	0.999
B54	SKC	224-PCXR3	509821	06/04/2026	1,000	1,500	2,000	1,005	1,500	2,008	1.007x - 10.015	1.000
B55	SKC	224-PCXR3	510710	06/04/2026	1,000	1,500	2,000	1,013	1,502	2,007	1.002x - 2.573	0.999
B56	SKC	224-PCXR3	511450	06/04/2026	1,000	1,500	2,000	992	1,492	1,999	1.004x - 10.669	1.000
B57	SKC	224-PCXR3	510798	06/04/2026	1,000	1,500	2,000	999	1,496	1,996	0.998x - 0.463	1.000
B58	SKC	224-PCXR3	509852	06/04/2026	1,000	1,500	2,000	1,003	1,499	1,999	0.996x + 4.204	1.000
B59	SKC	224-PCXR3	509862	06/04/2026	1,000	1,500	2,000	1,000	1,500	1,998	0.998x + 0.850	1.000
B60	SKC	224-PCXR3	512655	06/04/2026	1,000	1,500	2,000	997	1,506	2,002	1.003x - 8.264	0.999
B61	SKC	224-PCXR3	503915	06/04/2026	1,000	1,500	2,000	999	1,505	2,006	1.004x - 6.792	1.000
B62	SKC	224-PCXR3	505975	06/04/2026	1,000	1,500	2,000	998	1,504	2,004	1.005x - 10.095	1.000
B63	SKC	224-PCXR3	511432	09/04/2026	1,000	1,500	2,000	999	1,500	1,997	0.999x - 2.345	1.000
B64	SKC	224-PCXR3	508302	09/04/2026	1,000	1,500	2,000	1,001	1,491	1,996	0.997x + 0.511	1.000
B65	SKC	224-PCXR3	508310	09/04/2026	1,000	1,500	2,000	1,002	1,509	1,994	1.000x - 4.906	0.999
B66	SKC	224-PCXR3	509861	09/04/2026	1,000	1,500	2,000	995	1,501	2,004	1.008x - 15.001	1.000
B67	SKC	224-PCXR3	506295	09/04/2026	1,000	1,500	2,000	1,002	1,500	1,999	0.998x + 1.468	1.000
B68	SKC	224-PCXR3	505872	09/04/2026	1,000	1,500	2,000	1,005	1,494	1,994	0.996x - 1.783	0.999
B69	SKC	224-PCXR3	508375	09/04/2026	1,000	1,500	2,000	997	1,505	2,005	1.009x - 17.840	0.999
B70	SKC	224-PCXR3	510623	09/04/2026	1,000	1,500	2,000	998	1,499	1,999	1.000x - 2.573	1.000
B71	SKC	224-PCXR3	508367	09/04/2026	1,000	1,500	2,000	1,002	1,503	1,989	0.997x - 0.594	0.999
B72	SKC	224-PCXR3	505977	09/04/2026	1,000	1,500	2,000	999	1,504	2,001	1.002x - 4.551	1.000
B73	SKC	224-PCXR3	512606	09/04/2026	1,000	1,500	2,000	1,001	1,502	2,002	1.000x - 1.555	1.000
B74	SKC	224-PCXR3	505993	09/04/2026	1,000	1,500	2,000	1,003	1,504	2,008	1.006x - 6.832	1.000
B75	SKC	224-PCXR3	509820	09/04/2026	1,000	1,500	2,000	1,002	1,503	1,990	1.002x - 9.465	0.999
B76	SKC	224-PCXR3	509811	09/04/2026	1,000	1,500	2,000	1,001	1,500	2,002	1.001x - 2.688	1.000
B77	SKC	224-PCXR3	508301	09/04/2026	1,000	1,500	2,000	999	1,501	1,996	0.998x + 0.550	1.000
B78	SKC	224-PCXR3	510677	09/04/2026	1,000	1,500	2,000	1,000	1,496	1,997	1.000x - 3.151	1.000
B79	SKC	224-PCXR3	510920	09/04/2026	1,000	1,500	2,000	1,002	1,502	1,986	0.997x - 2.026	0.999

Calibrated by : Adul Dangklom (Mr. Adul Dangklom)

Approved by : (Mr. Peera Detudom)

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com.. www.spscon.com

Rotameter Calibration Report (For Personal Pump High Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter	Model : Defender 510-H	S/N : 136833

Calibration Data

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (ml/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R^2
H-R01	Dwyer	VFB-65	01/04/2026	500	1,000	2,000	499.7	1000.6	1996.7	1.000x - 0.544	1.000
H-R02	Dwyer	VFB-65	01/04/2026	500	1,000	2,000	501.2	992.4	1990.0	1.001x - 5.362	0.999
H-R03	Dwyer	VFB-65	03/04/2026	500	1,000	2,000	501.4	997.5	1997.3	0.998x + 2.606	1.000
H-R04	Dwyer	VFB-65	05/04/2026	500	1,000	2,000	502.5	993.6	1985.2	0.999x - 2.085	0.999
H-R05	Dwyer	VFB-65	05/04/2026	500	1,000	2,000	500.4	1001.3	1999.8	1.000x + 1.247	1.000
H-R06	Dwyer	VFB-65	03/04/2026	500	1,000	2,000	500.8	997.2	1994.6	0.999x - 0.348	1.000

Calibrated by :	Approved by :
Adul Bangklom (Mr.Adul Bangklom)	(Mr. Peera Detudom)

QUALITY CALIBRATION CO.,LTD.
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584
www.qcalibration.com

ilac-MRA NSC-TISI-TIS17025 CALIBRATION 0049

CERTIFICATE No : 26M2266
REFERENCE No : 80204-1

Certificate of Calibration

EQUIPMENT	:	DIGITAL BALANCE
MANUFACTURER	:	METTLER TOLEDO
MODEL	:	XS105DU
SERIAL No	:	1126422905
ID No	:	BA 05/50
CONDITION AS RECEIVED	:	USED ITEM
SUBMITTED BY	:	S.P.S. CONSULTING SERVICE CO., LTD. 7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD., JOMPOL, CHATUCHAK, BANGKOK 10900
CALIBRATED BY	:	SUCHAT S.
CALIBRATION DATE	:	05-Mar-26
APPROVED BY	:	PONGSAK J.
ISSUED DATE	:	06-Mar-26
RECEIVED DATE	:	05-Mar-26

Certificate

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF QUALITY CALIBRATION CO., LTD.

QUALITY CALIBRATION CO.,LTD.
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584
www.qcalibration.com

CERTIFICATE No : 26M2266

Calibration Report

EQUIPMENT	:	DIGITAL BALANCE	**MODEL**	:	XS105DU
MANUFACTURER	:	METTLER TOLEDO	**S/N**	:	1126422905
ID No	:	BA 05/50	**RECEIVED DATE**	:	05-Mar-26
AIR PRESSURE	:	1004mbar ± 1mbar	**CALIBRATION DATE**	:	05-Mar-26
AMBIENT TEMPERATURE	:	25° C ± 1° C	**RELATIVE HUMIDITY**	:	50 %RH ± 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARLITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.
2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	C02250116	28-Jan-27
2) STANDARD WEIGHT	E2	15843	C02250117	29-Jan-27


3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
   - NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL
2. TARE FUNCTION : NORMAL
3. REPEATABILITY OF READING AT 120 g WAS 0.000055 g
4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (± g)
0.00	0.00000	0.00000	0.000065
0.02	0.02000	0.00000	0.000065
0.10	0.10000	0.00000	0.000066
0.20	0.20000	0.00000	0.000066
0.50	0.50001	-0.00001	0.000065
1.00	1.00001	-0.00001	0.000066
2.00	2.00000	0.00000	0.000067
5.00	5.00001	-0.00001	0.000068
10.00	10.00004	-0.00004	0.000070
20.00	20.00006	-0.00006	0.000078
50.00	50.0000	0.0000	0.00012
100.00	100.0002	-0.0002	0.00019
120.00	120.0002	-0.0002	0.00022

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.0000
2	50.0000
3	50.0000
4	50.0000
5	50.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k =2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

Copyright

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY
451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

SITHIPORN associates

ilac-MRA

NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : SP25026
Pages : 1 of 4

Calibration Certificate

Equipment :	UV-VIS SPECTROPHOTOMETER
Manufacturer :	PERKINELMER
Model :	LAMBDA 25
Serial No.:	501S14123010
ID No.:	SP03/58
Calibration Mode :	WAVELENGTH ACCURACY PHOTOMETRIC ACCURACY STRAY LIGHT
Condition As Found :	GOOD
Customer :	S.P.S CONSULTING SERVICE CO., LTD. 7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN ROAD, CHOMPHON SUB-DISTRICT, CHATUCHAK DISTRICT, BANGKOK PROVINCE 10900 THAILAND.
Location :	ORGANIC LABORATORY IV
Ambient Temperature :	(22.9 ± 5) °C
Relative Humidity :	(53.7 ± 25) %
Received Date :	22 AUGUST 2025
Calibration Date :	22 AUGUST 2025
Date of Issue :	25 AUGUST 2025

Calibrated by : Nitinun Srihawan

Approved by : Wichok B.
(Wichok Ekpongpradit)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : SP25026
Job No. : VC68SP0019
Pages : 2 of 4

Calibration Method :

This instrument was calibrated by using on-site calibration procedure In-house method : CP-SP-01

The calibration procedure to direct measurement wavelength accuracy by using wavelength standard solution, Photometric accuracy by using absorbance standard filter and absorbance standard solution

The calibration procedure used was based on ASTM E275-01,ASTM E925-02

Condition of this result of calibration :

1. Certified reference materials

Material	Ref. type	Cell serial No.	Cert. No.	Due Date
Holmium liquid	RM-HL	29706	126461	24/10/2026
Didymium liquid	RM-DL	28912	126462	24/10/2026
Neutral density filter	RM-1N2N3N	13877	126457	24/10/2026
Potassium dichromate solutions	RM-0204060810	14204	126497	25/10/2026
Potassium Iodide solution	-	KI-0701-001	CI-0185-24	14/05/2026

2. This result of calibration was found accurate as shown on date and place of calibration only.
3. This certificate is traceable to the international system of unit maintained at :
   3.1 The UK National Physical Laboratory (NPL)

Result of calibration : Wavelength Accuracy

(Without adjustment)

Material	Certified Values of Reference Material (nm)	UUC* Reading (nm)	Error (nm)	Uncertainty ± (nm)	*k* Factor
RM-HL	278.13	278.21	0.08	0.16	2.00
	361.25	361.39	0.14	0.16	2.00
	467.82	467.71	-0.11	0.16	2.00
	536.56	536.50	-0.06	0.16	2.00
	640.50	640.36	-0.14	0.16	2.00
RM-DL	740.09	739.85	-0.24	0.16	2.00
	864.94	865.12	0.18	0.16	2.00

UUC* = Unit Under Calibration

Michou B.

SITHIPORN associates
SITHIPORN ASSOCIATES
CALIBRATION LABORATORY

Cert. No. : SP25026
Job No. : VC68SP0019
Pages : 3 of 4

Result of calibration : Photometric Accuracy

Material	Wavelength (nm)	Filter S/N	Nominal Absorbance (A)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	*k* Factor
Neutral Density glass filter	440.0	29381	0.5	0.5443	0.5413	-0.0030	0.0043	2.00
		29914	0.7	0.7484	0.7455	-0.0029	0.0054	2.00
		29360	1.0	1.0527	1.0535	0.0008	0.0032	2.00
	465.0	29381	0.5	0.4948	0.4922	-0.0026	0.0041	2.00
		29914	0.7	0.6906	0.6877	-0.0029	0.0050	2.00
		29360	1.0	0.9695	0.9709	0.0014	0.0031	2.00
	546.1	29381	0.5	0.5090	0.5068	-0.0022	0.0036	2.00
		29914	0.7	0.6985	0.6960	-0.0025	0.0041	2.00
		29360	1.0	0.9814	0.9825	0.0011	0.0031	2.00
	590.0	29381	0.5	0.5375	0.5353	-0.0022	0.0034	2.00
		29914	0.7	0.7256	0.7231	-0.0025	0.0037	2.00
		29360	1.0	1.0213	1.0219	0.0006	0.0032	2.00
	635.0	29381	0.5	0.5223	0.5202	-0.0021	0.0033	2.00
		29914	0.7	0.6927	0.6901	-0.0026	0.0036	2.00
		29360	1.0	0.9744	0.9750	0.0006	0.0032	2.00

UUC* = Unit Under Calibration

Michou B.

SITHIPORN associates

SITHIPORN ASSOCIATES
CALIBRATION LABORATORY

Cert. No. : SP25026
Job No. : VC68SP0019
Pages : 4 of 4

Result of calibration : Photometric Accuracy

(Without adjustment)

Material	Wavelength (nm)	Solution (mg/l)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	*k* Factor
Potassium dichromate solutions	235.0	20	0.2415	0.2443	0.0028	0.0101	2.00
		40	0.4866	0.4871	0.0005	0.0115	2.00
		60	0.7415	0.7295	-0.0120	0.0067	2.00
		80	0.9854	0.9844	-0.0010	0.0071	2.00
		100	1.2444	1.2425	-0.0019	0.0073	2.00

UUC* = Unit Under Calibration

Condition of this result of calibration : Spectrophotometer PERKINELMER Model LAMBDA 25 S/N 501S14123010

Resolution of Wavelength Mode 0.1 nm
Resolution of Photometric Mode 0.001 A
Parameter Setting
Measurement Mode Wavelength, Absorbance
Wavelength Scan 190 nm - 1100 nm
Scanning Speed 7.5 nm/min
Band width(Wavelength) 1.0
Band width(Vis) 1.0
Band width(Uv) 1.0

Stray Light** UUC* Reading at 220.0 nm	
Transimission T(%)	**Absorbance(A)**
0.020	3.7032

**Specific Acceptance :
Transmission ≤ 1.0 T(%), Absorbance ≥ 2.0 A
**Stray light not TISI Accredited

The reported uncertainty is based on a standard uncertainty mutiplied by a coverage factor *k*, providing a level of confidence of approximately 95%

End of Calibration Certificate

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phahonyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com.. www.spscon.com

Calibration Report
Non-Dispersive Infrared CO Analyzer

Date :	01 April 2026	Brand :	API	Model :	300E
No.	CO-B02			Serial No.	965

Calibrator (Dilution System)

Brand	: API	Model	: 700
Last Cal. Date	: 01 September 2025	Serial No.	: 911

Reference Standard Gas

Standard Gas	: Carbon Monoxide (CO)			Cylinder No.	: D711839
Certified Date	: 14 March 2024	Expired Date	: 14 March 2032	Cylinder Conc.	: 4,580 ppm

Calibrating Condition

Pressure	1011	mmbar	Temp. 24.5	°C	% RH 48

Calibration Setting

Span	Initial Reading (Before Adj.), PPM			Final Reading (After Adj.), PPM
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response
Zero	0	-0.10	-	0
CO Span	40.00	39.97	-0.075	40.00

API Model 300E CO Analyzer Check List

Parameter	Observed Value	Units	Nominal Range
Range	50	PPM	0-1000 ppm
Stability	0.10	PPM	< 1 ppm With Zero Air
CO Measure	4015.9	mV	2500-4800 mV
CO Reference	3949.6	mV	2500-4800 mV
Measure/Reference Ratio	1.179	-	1.1-1.3 W/Zero Air
Sample Pressure	28.5	In-Hg-A	~2"< Ambient Absolute Pressure
Sample Flow	811	CC/Min	800 ± 10%
Sample Temperature	48.5	°C	48 ± 4
Bench Temperature	48.2	°C	48 ± 2
Wheel Temperature	68.4	°C	68 ± 2
Box Temperature	30.7	°C	Ambient Temp + 7 ± 10
Photo-Drive	3034.5	mV	250 mV to 4750 mV
Slope	1.017	-	1.0 ± 0.3
Offset	0.2	-	0 ± 0.3

Calibrated by : Adul Dangklom
(Mr.Adul Dangklom)

Approved by :
(Mr. Peera Detudom)

คุณภาพน้ำ

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com

CLC Accredited ISO/IEC 17025

ilac-MRA

ANAB ACCREDITED ISO/IEC 17025 CALIBRATION AND DIMENSIONAL MEASUREMENT ACDM-2814

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE	:	pH METER
MANUFACTURER	:	HANNA
MODEL / TYPE	:	HI3512/HI1332/HI7662-T
SERIAL NO.	:	08685754/11250B7M/092806BN[PH04/56]
CLID. NO.	:	272501562
JOB CONTROL NO.	:	250617070523
CALIBRATION SERVICE	:	☑ IN-LABORATORY ☐ ON-SITE

CUSTOMER : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24 ROAD, JOMPOL,
CHATUCHAK, BANGKOK 10900

DATE OF RECEIVED : 17 June 2025 DATE OF ISSUED : 20 June 2025

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sukgasem Seehanart
Wenick Inchaisri
Calibration Engineer

Approved By : Mongkol Yotsoontorn
Authorized Signatory
20 June 2025

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

@clccalibration

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com

CLC Accredited ISO/IEC 17025

ilac-MRA

ANAB ACCREDITED ISO/IEC 17025 CALIBRATION AND DIMENSIONAL MEASUREMENT ACDM-2814

REPORT OF CALIBRATION

FOR

NOMENCLATURE	:	pH METER
MANUFACTURER	:	HANNA
MODEL / TYPE	:	HI3512/HI1332/HI7662-T
SERIAL NO.	:	08685754/11250B7M/092806BN[PH04/56]
DATE OF CALIBRATION	:	18 June 2025

ENVIRONMENT CONDITIONS :

Temperature : (25 ± 2.5) °C Relative Humidity : (50 ± 15) % RH

PROCEDURE USED :

This instrument was calibrated under procedure No. **CLC-CPCH-01** [pH Meter]. The calibration was performed by direct measurement with Certified Reference Material (CRM).

This instrument was calibrated under procedure No. **CLC-CPTH-04** [Temperature] based on **ASTM E 644-04** as calibration guidelines. The calibration was performed by using Calibration Bath, Precision Thermometer and IPRT which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. pH Standard Solution, NIMT TRM CODE TRM-S-2003, TRM CODE TRM-S-2007.
2. pH Standard Solution, Control Company Catalog Number 06664260,11754256, Lot Number CC787362.
3. Calibration Bath, Kambic Model OB-22/2 ULT S/N. 17115653.
4. Precision Thermometer, ASL Model F250 S/N. 1334023800.
5. IPRT, Wika Model CTP5000-250-D S/N. PO00043543-1-10-1.

@clccalibration

TRACEABILITY :

1. The measurements are traceable to International System of Units (SI) , through National Institute of Metrology (Thailand).
Lot Number. 080124 , 120124. Due Date 23 January 2026.

2. The measurements are traceable to International System of Units (SI) , through Control Company.
Certificate No. 4281-14495731 , Due Date 27 September 2025.

3. The measurements are traceable to International System of Units (SI) , through Calibration Laboratory Co., Ltd.
Certificate No. Q24120999, Due Date 26 November 2025.

4. The measurements are traceable to International System of Units (SI) , through Thailand Institute of Scientific and Technological Research (TISTR). Certificate No. PSL-T 1042/67, Due Date 16 October 2025.

5. The measurements are traceable to International System of Units (SI) , through National Institute of Metrology (Thailand).
Certificate No. TT-0146-24, Due Date 28 October 2025.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
ACCREDITED ISO/IEC 17025 CALIBRATION AND DIMENSIONAL MEASUREMENT ACDM-2814

CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment ( ) adjustment

The table in the following gives the calibration results and associated measurement uncertainties of pH meter.

CALIBRATION DATA

1. pH METER RESULT @ 25 °C

Standard pH Buffer Solution (pH)	pH Meter Reading (pH)	pH Meter Reading (mV)	Correction (pH)	Uncertainty of pH Measurement (± pH)	*k* Factor
4.003	4.005	168.2	-0.002	0.010	2,00
7.005	7.010	-8.1	-0.005	0.013	2,00
10.015	10.010	-177.7	+0.005	0.014	2,00

Technical Note. Setting function CAL 3 point (4,7,10).

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 015 Page 4 of 68

2. TEMPERATURE RESULT

Immersion depth (mm)	Actual Temperature (°C)	DUC Reading (°C)	Correction (°C)	Uncertainty ± (°C)
100	25.00	25.0	0.00	0.07

Technical Note. Type of sensor : Thermistor

Probe ∅ 3 mm

Materials : Metal Sheath.

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor of $k = 2,00$.

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 015 Page 56 of 68

This report is valid for the above stated instrument/s only.

End of Certificate

QUALITY CALIBRATION CO., LTD.
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

NSC-TISI-TIS17025 CALIBRATION 0049

CERTIFICATE No : 26E3363
REFERENCE No : 80514-1

Certificate of Calibration

EQUIPMENT	:	pH METER
MANUFACTURER	:	HANNA
MODEL	:	HI3512
SERIAL No	:	TH118035
ID No	:	PH 04/56
CONDITION AS RECEIVED	:	USED ITEM
SUBMITTED BY	:	S.P.S. CONSULTING SERVICE CO., LTD. 7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD., JOMPOL, CHATUCHAK, BANGKOK 10900
CALIBRATED BY	:	ATSAWIN Y.
CALIBRATION DATE	:	02-Apr-26
APPROVED BY	:	PONGSAK J.
ISSUED DATE	:	02-Apr-26
RECEIVED DATE	:	01-Apr-26

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF QUALITY CALIBRATION CO., LTD.

QUALITY CALIBRATION CO., LTD.
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 26E3363

Calibration Report

EQUIPMENT	:	pH METER			
MANUFACTURER	:	HANNA	**MODEL**	:	HI3512
ID No	:	PH 04/56	**SERIAL NUMBER**	:	TH118035
RECEIVED DATE	:	01-Apr-26	**CALIBRATION DATE**	:	02-Apr-26
AMBIENT TEMPERATURE	:	23 ° C ± 3 ° C	**RELATIVE HUMIDITY**	:	50 % RH ± 10% RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT METHOD BASED ON WI-TQ-062 AND WI-TQ-063. THE DISPLAY UNIT WAS TESTED BY GENERATING STANDARD VOLTAGE TO THE UNIT AND READING THE VALUE COMPARED WITH THE CALCULATED VALUE. THE DISPLAY AND ELECTROD WAS CALIBRATED BY USING STANDARD pH BUFFER
2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No/ LOT No	CERTIFICATE No	DUE DATE
1) pH STANDARD SOLUTION	00651-36	CC829914	4956-16178366	11-Sep-27
2) pH STANDARD SOLUTION	00651-38	CC831093	4957-16224157	01-Oct-27
3) pH STANDARD SOLUTION	00651-40	CC826321	4958-16046326	10-Jul-27
4) PROCESS CALIBRATOR	CA150	91S6079	26E936	17-Mar-27
5) BATH	260014	1247 48074	25T9431	12-Sep-26
6) THERMOMETER WITH PROBE	421504	55000379	25T9466	12-Sep-26

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO SI UNIT MAINTAINED AT :-
   - NATIONAL INSTITUTE OF STANDARD AND TECHNOLOGY, USA.
   - NATIONAL INSTUTITE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION : ADJUSTMENT

1. DISPLAY UNIT ONLY

SLOPE FACTOR k = 2.303 RT/F = 59 mV/pH

mV APPLIED	UUC READING (mV)	CORRECTION (mV)	UUC READING (pH)	UNCERTAINTY OF MEASUREMENT (± mV)	COVERAGE FACTOR k
414.11	414.3	-0.19	-0.256	0.15	2.00
354.95	355.1	-0.15	0.759	0.15	2.00
295.80	296.0	-0.20	1.773	0.15	2.00
236.64	236.8	-0.16	2.787	0.15	2.00
177.48	177.7	-0.22	3.801	0.15	2.00
118.32	118.5	-0.18	4.816	0.15	2.00
59.16	59.4	-0.24	5.831	0.15	2.00
0.00	0.2	-0.20	6.845	0.15	2.00
-59.16	-58.9	-0.26	7.878	0.15	2.00
-118.32	-118.1	-0.22	8.915	0.15	2.00
-177.48	-177.2	-0.28	9.952	0.15	2.00
-236.64	-236.4	-0.24	10.990	0.15	2.00
-295.80	-295.5	-0.30	12.027	0.15	2.00
-354.95	-354.7	-0.25	13.064	0.15	2.00
-414.11	-413.8	-0.31	14.101	0.15	2.00

END OF CALIBRATION REPORT PAGE 2 OF 3

F-G010 REV 03

QUALITY CALIBRATION CO., LTD.
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 26E3363

Calibration Report

RESULT OF CALIBRATION (CONTINUE) :

2. DISPLAY UNIT WITH pH ELECTRODE S/N: 11340D0M

STANDARD pH BUFFER SOLUTION (pH)	UUC READING (pH)	CORRECTION (pH)	VALUE BEFORE ADJUSTMENT	UNCERTAINTY OF MEASUREMENT (± pH)	COVERAGE FACTOR k
4.008	4.008	0.000	4.142	0.012	2.00
6.998	7.000	-0.002	7.068	0.012	2.00
10.007	10.009	-0.002	10.226	0.014	2.00

3. DISPLAY UNIT WITH TEMPERATURE

STANDARD READING (°C)	UUC READING (°C)	CORRECTION (°C)	VALUE BEFORE ADJUSTMENT	UNCERTAINTY OF MEASUREMENT (± °C)	COVERAGE FACTOR k
25.004	25.0	0.004	---	0.0085	2.00

4. PERCENT SLOPE 91%

UUC : UNIT UNDER CALIBRATION

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

Certificate

Harikul Science Co.,Ltd.
694 Soi Ratchadanivet 24, Pracharatbamphen,
Samsaennok, Huaikhwang, Bangkok 10310
Tel: 0-2274-2456 Fax: 0-2274-2443
Email: info@harikul.com www.harikul.com

Certificate of Calibration

CERT.No.: HS-W015C

Calibration Date :	18 Mar 25	Model	: YSI 5000
Submitted by :	S.P.S CONSULTING SERVICE CO.,LTD	S/N	: 15B100751
	7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol,	Probe	: YSI 5010
	Chatuchak, Bangkok, Thailand 10900	S/N	: 22D100097
		ID NO.	: -
Avg Room Temp :	20 °C	Air Temp ref	: S/N. F8065C26
Avg Water Temp :	20 °C	Barometric ref	: S/N. F8065C26
Air Pressure :	760.00 mmHg	Water Temp ref	: -
Salinity :	0 ppt	ID NO.	HS001
		Technician	: Kittipong M.

Calibration Details

Calibration Point	100% air sat. (@20 °C, DO = 9.09 mg/l)	(status)		(status)
Measurement 1 (mg/l)	9.08	(PASS)	-	-
Measurement 2 (mg/l)	9.08	(PASS)	-	-
Measurement 3 (mg/l)	9.08	(PASS)	-	-
Measurement 4 (mg/l)	9.07	(PASS)	-	-
Measurement 5 (mg/l)	9.07	(PASS)	-	-
Measurement 6 (mg/l)	9.07	(PASS)	-	-
Measurement 7 (mg/l)	9.07	(PASS)	-	-
Measurement 8 (mg/l)	9.07	(PASS)	-	-
Measurement 9 (mg/l)	9.07	(PASS)		-
Measurement 10 (mg/l)	9.07	(PASS)	-	-
Mean Measurement	9.07	mg/l	-	-
Inaccuracy	0.02	mg/l	-	-

Overall Status (PASS)

Manufacturer Specification

Accuracy = +/- 0.02 mg/l

1) This certificate is issued based on the result that are found as shown on date and place of test only.
2) The calibration procedure followed in accordance with Harikul Science Co., Ltd.
3) This result shall not be used for advertising purpose.

Technician Signature
(Kittipong Maekwong)

Laboratory Manager
(Natenapha Pisatkunchon)

HARIKUL SCIENCE

Harikul Science Co.,Ltd.
694 Soi Ratchadanivet 24, Pracharatbamphen,
Samsaennok, Huaikhwang, Bangkok 10310
Tel: 0-2274-2456 Fax: 0-2274-2443
Email: info@harikul.com www.harikul.com

CERT.No.: HS-X014C

Certificate of Calibration

Calibration Date : 16 March 2026

Submitted by : S.P.S CONSULTING SERVICE CO.,LTD
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol,
Chatuchak, Bangkok, Thailand 10900

Avg Room Temp : 20 °C
Avg Water Temp : 20 °C
Air Pressure : 760.00 mmHg
Salinity : 0 ppt

Model : YSI 5000
S/N : 15B100751
Probe : YSI 5010
S/N : 22D100097
ID NO. :
Air Temp ref : S/N. F8065C26
Barometric ref : S/N. F8065C26
Water Temp ref : -
ID NO. HS001
Technician : Kittipong M.

Calibration Details

Calibration Point	100% air sat. (@20 °C, DO = 9.09 mg/l)	(status)		(status)
Measurement 1 (mg/l)	9.09	(PASS)	-	-
Measurement 2 (mg/l)	9.09	(PASS)	-	-
Measurement 3 (mg/l)	9.09	(PASS)	-	-
Measurement 4 (mg/l)	9.09	(PASS)	-	-
Measurement 5 (mg/l)	9.09	(PASS)	-	-
Measurement 6 (mg/l)	9.08	(PASS)	-	-
Measurement 7 (mg/l)	9.08	(PASS)	-	-
Measurement 8 (mg/l)	9.08	(PASS)	-	-
Measurement 9 (mg/l)	9.08	(PASS)		-
Measurement 10 (mg/l)	9.08	(PASS)	-	-
Mean Measurement	9.09	mg/l	-	-
Inaccuracy	0.00	mg/l	-	-
Overall Status	(PASS)			

Manufacturer Specification

Accuracy = +/- 0.02 mg/l

1) This certificate is issued based on the result that are found as shown on date and place of test only.
2) The calibration procedure followed in accordance with Harikul Science Co., Ltd.
3) This result shall not be used for advertising purpose.

Technician Signature
(Kittipong Maekwong)

Laboratory Manager
(Natenapha Pisatkunchon)

QUALITY CALIBRATION CO., LTD.
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584
www.qcalibration.com

CERTIFICATE No : 25T0521
REFERENCE No : 75853-2

Certificate of Calibration

EQUIPMENT	:	COD REACTOR
MANUFACTURER	:	HACH
MODEL	:	DRB 200
SERIAL No	:	15110C0498
ID No	:	CRB 06/59
CONDITION AS RECEIVED	:	USED ITEM
SUBMITTED BY	:	S.P.S. CONSULTING SERVICE CO., LTD. 7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD., JOMPOL, CHATUCHAK, BANGKOK 10900
CALIBRATED BY	:	CHAICHARN CH.
CALIBRATION DATE	:	03-Feb-25
APPROVED BY	:	PONGSAK J.
ISSUED DATE	:	03-Feb-25
RECEIVED DATE	:	15-Jan-25

Certificate

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF QUALITY CALIBRATION CO., LTD.

QUALITY CALIBRATION CO., LTD.
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 25T0521

Calibration Report

EQUIPMENT	:	COD REACTOR			
MANUFACTURER	:	HACH	**MODEL**	:	DRB 200
ID NUMBER	:	CRB 06/59	**SERIAL NUMBER**	:	15110C0498
RECEIVED DATE	:	15-Jan-25	**CALIBRATION DATE**	:	03-Feb-25
AMBIENT TEMPERATURE	:	23° C ± 1° C	**RELATIVE HUMIDITY**	:	53 %RH ± 10 % RH


CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASURMENT METHOD WITH CALIBRATED THERMOCOUPLE TYPE K UNDER NO LOAD CONDITION. THE THERMOCOUPLES WERE PLACED ON POINTS AND LOCATED AS THE PICTURE .
2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH TC TYPE K	HYDRA 2635A	7301307	24T6467	26-Jun-25

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
   - NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO., LTD.

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

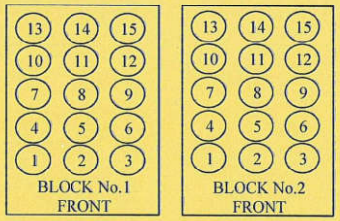

Block No.		1	2
Calibration Point (°C)		150	150
Controller temperature (°C)		145	145
Indicating Temperature		145	145
Measured Temperature (° C) at Spread Locations	1	150.23	150.64
	2	149.73	149.78
	3	150.29	150.29
	4	150.04	150.49
	5	150.09	150.51
	6	150.74	150.67
	7	149.97	150.66
	8	150.76	150.57
	9	150.54	150.51
	10	149.44	149.94
	11	150.12	150.64
	12	149.93	150.33
	13	149.19	149.82
	14	148.96	149.70
	15	149.09	149.79
Uncertainty of Measurement(± °C)		0.88	0.88

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.
NOTE 2 : LOCATION 10 WAS REFERENCE LOCATION.
NOTE 3 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k =2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

QUALITY CALIBRATION CO., LTD.
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584
www.qcalibration.com

CERTIFICATE No : 26T0464
REFERENCE No : 79659-1

Certificate of Calibration

EQUIPMENT	:	COD REACTOR
MANUFACTURER	:	HACH
MODEL	:	DRB 200
SERIAL No	:	15110C0497
ID No	:	DRB 04/59
SUBMITTED BY	:	S.P.S. CONSULTING SERVICE CO., LTD. 7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD., JOMPOL, CHATUCHAK, BANGKOK 10900
CALIBRATED BY	:	SOMCHAI S.
CALIBRATION DATE	:	30-Jan-26
APPROVED BY	:	PONGSAK J.
ISSUED DATE	:	30-Jan-26
RECEIVED DATE	:	30-Jan-26

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF QUALITY CALIBRATION CO., LTD.

QUALITY CALIBRATION CO., LTD.
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 26T0464

Calibration Report

EQUIPMENT	:	COD REACTOR			
MANUFACTURER	:	HACH	**MODEL**	:	DRB 200
ID NUMBER	:	DRB 04/59	**SERIAL NUMBER**	:	15110C0497
RECEIVED DATE	:	30-Jan-26	**CALIBRATION DATE**	:	30-Jan-26
AMBIENT TEMPERATURE	:	23° C ± 1° C	**RELATIVE HUMIDITY**	:	54 %RH ± 10 % RH


CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASURMENT METHOD WITH CALIBRATED THERMOCOUPLE TYPE K UNDER NO LOAD CONDITION. THE THERMOCOUPLES WERE PLACED ON POINTS AND LOCATED AS THE PICTURE .
2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH TC TYPE K	HYDRA 2635A	6849323	25T5342	18-Jun-26

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
   - NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO., LTD.

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

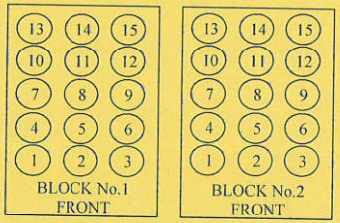

TEMPERATURE MEASUREMENT ACCURACY TEST

Block No.		1	2
Controller temperature (°C)		144	145
Indicating Temperature		144	145
Measured Temperature (° C) at Spread Locations	1	149.3	149.8
	2	149.1	149.9
	3	149.9	149.6
	4	150.0	149.3
	5	149.8	149.5
	6	149.9	149.1
	7	149.7	149.7
	8	149.5	149.9
	9	149.8	149.4
	10	148.5	149.4
	11	149.1	150.2
	12	149.2	150.0
	13	149.0	149.6
	14	149.1	150.3
	15	148.5	149.0
Uncertainty of Measurement(± °C)		0.89	0.89

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.
NOTE 2 : LOCATION 10 WAS REFERENCE LOCATION.
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k =2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

QUALITY CALIBRATION CO.,LTD.
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584
www.qcalibration.com

ilac-MRA
NSC-TISI-TIS17025
CALIBRATION 0049

CERTIFICATE No : 25M2256
REFERENCE No : 76365-3

Certificate of Calibration

EQUIPMENT	:	DIGITAL BALANCE
MANUFACTURER	:	SARTORIUS
MODEL	:	BSA224S-CW
SERIAL No	:	36591843
ID No	:	BA09/61
CONDITION AS RECEIVED	:	USED ITEM
SUBMITTED BY	:	S.P.S. CONSULTING SERVICE CO., LTD. 7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD., JOMPOL, CHATUCHAK, BANGKOK 10900
CALIBRATED BY	:	ATSAWIN Y.
CALIBRATION DATE	:	07-Mar-25
APPROVED BY	:	PONGSAK J.
ISSUED DATE	:	13-Mar-25
RECEIVED DATE	:	07-Mar-25

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF QUALITY CALIBRATION CO., LTD.

QUALITY CALIBRATION CO.,LTD.
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584
www.qcalibration.com

Calibration Report

EQUIPMENT	:	DIGITAL BALANCE	**MODEL**	:	BSA224S-CW
MANUFACTURER	:	SARTORIUS	**S/N**	:	36591843
ID No	:	BA09/61	**RECEIVED DATE**	:	07-Mar-25
AIR PRESSURE	:	1009mbar ± 1mbar	**CALIBRATION DATE**	:	07-Mar-25
AMBIENT TEMPERATURE	:	24° C ± 1° C	**RELATIVE HUMIDITY**	:	52 %RH ± 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARLITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.
2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	C02250116	28-Jan-27
2) STANDARD WEIGHT	E2	15843	C02250117	29-Jan-27


3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
   - NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL
2. TARE FUNCTION : NORMAL
3. REPEATABILITY OF READING AT 200 g WAS 0.000071 g
4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (± g)
0.00	0.0000	0.0000	0.00012
0.10	0.1000	0.0000	0.00012
0.20	0.2000	0.0000	0.00012
0.50	0.5000	0.0000	0.00012
1.00	1.0000	0.0000	0.00012
2.00	2.0000	0.0000	0.00012
5.00	5.0000	0.0000	0.00012
10.00	10.0000	0.0000	0.00012
20.00	20.0001	-0.0001	0.00012
50.00	50.0000	0.0000	0.00014
100.00	100.0001	-0.0001	0.00019
200.00	200.0001	-0.0001	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	100.0000
2	100.0000
3	100.0000
4	100.0000
5	100.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k =2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

QUALITY CALIBRATION CO.,LTD.
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584
www.qcalibration.com

NSC-TISI-TISI7025
CALIBRATION 0049

Certificate of Calibration

EQUIPMENT	:	DIGITAL BALANCE
MANUFACTURER	:	SARTORIUS
MODEL	:	BSA224S-CW
SERIAL No	:	36591843
ID No	:	BA 09/61
CONDITION AS RECEIVED	:	USED ITEM
SUBMITTED BY	:	S.P.S. CONSULTING SERVICE CO., LTD. 7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD., JOMPOL, CHATUCHAK, BANGKOK 10900
CALIBRATED BY	:	SUCHAT S.
CALIBRATION DATE	:	05-Mar-26
APPROVED BY	:	PONGSAK J.
ISSUED DATE	:	06-Mar-26
RECEIVED DATE	:	05-Mar-26

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF QUALITY CALIBRATION CO., LTD.

QUALITY CALIBRATION CO.,LTD.
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584
www.qcalibration.com

Calibration Report

EQUIPMENT	:	DIGITAL BALANCE	**MODEL**	:	BSA224S-CW
MANUFACTURER	:	SARTORIUS	**S/N**	:	36591843
ID No	:	BA 09/61	**RECEIVED DATE**	:	05-Mar-26
AIR PRESSURE	:	1004mbar ± 1mbar	**CALIBRATION DATE**	:	05-Mar-26
AMBIENT TEMPERATURE	:	25° C ± 1° C	**RELATIVE HUMIDITY**	:	50 %RH ± 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARLITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.
2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	C02250116	28-Jan-27
2) STANDARD WEIGHT	E2	15843	C02250117	29-Jan-27


3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
   - NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL
2. TARE FUNCTION : NORMAL
3. REPEATABILITY OF READING AT 200 g WAS 0.000055 g
4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (± g)
0.0	0.0000	0.0000	0.00010
0.1	0.1000	0.0000	0.00011
0.2	0.2000	0.0000	0.00010
0.5	0.5000	0.0000	0.00011
1.0	1.0000	0.0000	0.00011
2.0	2.0000	0.0000	0.00011
5.0	5.0000	0.0000	0.00011
10.0	10.0000	0.0000	0.00011
20.0	20.0001	-0.0001	0.00011
50.0	50.0000	0.0000	0.00013
100.0	100.0001	-0.0001	0.00019
200.0	200.0001	-0.0001	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	100.0000
2	100.0000
3	100.0000
4	100.0000
5	100.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k =2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

ระดับเสียงโดยทั่วไป

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-69/0204 **MTC No.** EEL. BP. 152/0169

CALIBRATION CERTIFICATE

Submitted by : S.P.S.CONSULTING SERVICE CO.,LTD.

Address : 7 Soi Phaholyothin 24, Phaholyothin Road, Jompol, Chatuchak, Bangkok 10900.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre. Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Sound Calibrator

Manufacturer : ACO

Model : 2127

Serial No. : 130006

Ambient Environment

Temperature : (23 + 3) °C

Relative Humidity : (50 ± 15) %

Ambient Pressure : (101.325 ± 1.500) kPa

Standards used :

1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.
2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.
3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.
4. Digital Multimeter Agilent 34401A S/N MY44005560.
5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.
6. Audio Analyzer Keithley 2015-P S/N 4106495.
7. Condenser Microphone Bruel&Kjaer 4180 S/N 2889871.

Calibration Procedure: CP-102-04 based on IEC 60942-2003; The sound pressure level generated by sound calibrator under test shall be measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 29 Jan. 2026

Date of Calibration : 11 Feb. 2026

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

NSC-TISI-TIS 17025
CALIBRATION 0037

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-69/0204 **MTC No.** EEL. BP. 152/0169

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20μPa at 1000 Hz

Acoustic Output in dB re 20μPa, Corrected to Reference Conditions: 101.325 kPa, 23.0 °C and 50 %RH.

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	93.89	-0.11	± 0.10	±0.40 dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	999.9	-0.1	± 1.5	±1.0%

3. Total Distortion

Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	1.90	± 0.50	±3.0%

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Calibrated by :

(Mr.Weerachai Deechaiyae)

Approved by :

(Mr.Prawate Kluaypa)

Director

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 11 Feb. 2026

Date of Issue : 12 Feb. 2026

Ref : 20112690129004970O1

End of Certificate

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Noise R_265/26

Sound Level Meter Calibration Report

Acoustic Calibrator Data

Brand	ACO	Number	AC 03/56
Model	2127	Serial No.	130006
Calibration Range	94 dB, 1000 Hz	Last Calibration	11 February 2026
		Due Date	11 February 2027

Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-B02	ACO	6236	00090370	15 April 2026	93.9	93.9
ACO-B12	ACO	6236	00150081	15 April 2026	93.8	93.9
ACO-B17	ACO	6236	00172042	15 April 2026	93.9	93.9
ACO-R03	ACO	6236	00142023	15 April 2026	93.8	93.9
ACO-R12	ACO	6236	00172040	15 April 2026	93.9	93.9
ACO-R13	ACO	6236	00172041	15 April 2026	93.8	93.9
ACO-R14	ACO	6236	00090517	15 April 2026	93.9	93.9
ACO-R19	ACO	6236	00182001	15 April 2026	93.8	93.9
ST-C1-B06	SCARLET	ST-12D	10351461	15 April 2026	93.9	93.9
ST-C1-B07	SCARLET	ST-12D	10351464	15 April 2026	93.8	93.9
ST-C1-B08	SCARLET	ST-12D	10351469	15 April 2026	93.9	93.9
ST-C1-B09	SCARLET	ST-12D	10351478	15 April 2026	93.8	93.9
ST-C1-B10	SCARLET	ST-12D	10351483	15 April 2026	93.9	93.9
ST-C1-B11	SCARLET	ST-12D	10351484	15 April 2026	93.8	93.9
ST-C1-B12	SCARLET	ST-12D	10351485	15 April 2026	93.9	93.9
ST-C1-B13	SCARLET	ST-12D	10351486	15 April 2026	93.8	93.9
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.81 ± 0.10 dB	

Calibrated by : Heeson L.
(Mr. Heeson Lormae)

Approved by : Yutthana T.
(Mr. Yutthana Tanatharanit)

คุณภาพอากาศในสถานประกอบการ

right solutions.
right partner.

รายการเครื่องมือที่ใช้ในการวิเคราะห์ / ทดสอบ

Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Workplace	Butadiene	DRYCAL FLOWMETER	BKK_FS0614	10-Sep-25	9-Sep-26	12
Workplace		DRYCAL FLOWMETER	BKK_FS0619	10-Sep-25	9-Sep-26	12
Workplace		Air Sampling Pump	RYG_FS0499	7-Jan-26	7-Apr-26	3
Workplace		Air Sampling Pump	RYG_FS0135	7-Jan-26	7-Apr-26	3
Workplace	Butadiene	GC-FID	BKK_EN0126	22-Oct-25	21-Oct-26	12

right solutions.
right partner.

รายการเครื่องมือที่ใช้ในการวิเคราะห์ / ทดสอบ

Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Workplace	Butadiene,	DRYCAL FLOWMETER	BKK_FS0614	10-Sep-25	9-Sep-26	12
Workplace		DRYCAL FLOWMETER	BKK_FS0619	10-Sep-25	9-Sep-26	12
Workplace		Air Sampling Pump	RYG_FS0361	6-Jan-26	6-Apr-26	3
Workplace		Air Sampling Pump	RYG_FS0503	3-Apr-26	3-Jul-26	3
Workplace	Butadiene	GC-FID	BKK_EN0126	22-Oct-25	21-Oct-26	12

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate of Calibration

Customer

Certificate No : 25-AFM-208

Name : ALS Laboratory Group Thailand Co., Ltd.

Request No : Req-2025-1986

Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang, Bangkok 10250

Unit Under Calibration Details

Measurement Item : Air Flow Meter

Manufacturer : Mesa Labs

Sensor Model : -

Model : 200-510M

Sensor Serial Number : -

Serial Number : 151114

Instrument Status : Used

ID : BKK_FS0614

Location of Calibration : LAB 4 AIR VELOCITY METER

Calibration Environment and Details

Temperature : 23 °C ± 3 °C

Humidity : 55 %RH ± 20 %RH

Barometric Pressure : 1013 hPa ± 10 hPa

Received Date : 3 September 2025

Calibration Date : 10 September 2025

Calibration Procedure : In-house method CP-AFM-01 by Comparison technique with Standard Primary Flow Calibrator

REVIEW BY Nmakorn P.

APPROVED BY

NEXT CAL DATE 09/09/26

Reference Standard	Model	Serial Number	Traceble	Due Calibration
Air Flow Meter	Gilibrator 3 Low flow	18501010006	Sensidyne	5 May 2026
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	6 May 2026
Temperature meter	GT 11	08000057	Qreborn	15 October 2025
Pressure meter	CPG2400	41000KDU/651882	TPA	21 October 2025

Traceability :

This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01 and MIT NSC-TISI-TIS Accreditation No. 0052

Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k = 2, providing a level of confidence approximately 95 %.

Calibration By :

Mr. Noppadon Luangart

Service Calibration Engineer

Approved By :

Mr. Pacit Mathavorn

Calibration Engineer Supervisor

Issue Date : 10 September 2025

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate No : 25-AFM-208

Request No : Req-2025-1986

Result of Calibration : Without Adjustment

STD Reading			UUC Readinng			Error	Uncertainty		
Temperature (°C)	Pressure (kPa)	Flow (cc/min)	Temperature (°C)	Pressure (kPa)	Flow (cc/min)	(cc/min)	(cc/min)	(°C)	(kPa)
25.5	100.98	100	-	-	100.02	0.0	3.6	1.0	0.50
25.7	100.97	503	-	-	500.81	-2.2	9.5	1.0	0.50
25.8	100.89	1003	-	-	1000.4	-3	19	1.0	0.50
26.1	100.88	2000	-	-	2001.9	2	38	1.0	0.50
26.5	100.85	3014	-	-	3002.2	-12	57	1.0	0.50
26.7	100.81	4027	-	-	4000.9	-26	76	1.0	0.50
27.0	100.74	5048	-	-	5001.8	-46	95	1.0	0.50

Note STD : Standard UUC : Unit Under Calibration

- UUC Reference Condition : At atmospheric pressure and room temperature condition, Air
- Flow Rate was corrected for non-standard operating condition by using equation :

$$Qmeas = \mathrm{Qref}\, x \frac{\mathrm{Pref}}{\mathrm{Pmeas}} x \frac{\mathrm{Tmeas}}{\mathrm{Tref}}$$

where Q = Flow Rate P = Absolute Pressure T = Absolute Temperature
meas = Measurement Condition ref = Standard Condition

* Indicates non accredited

End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

FM-708-AFM-01 Rev.06 Issue date 21/2/25

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate of Calibration

Customer

Certificate No : 25-AFM-207

Name : ALS Laboratory Group Thailand Co., Ltd.

Request No : Req-2025-1987

Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang, Bangkok 10250

Unit Under Calibration Details

Measurement Item : Air Flow Meter

Manufacturer : Mesa Labs

Sensor Model : -

Model : 200-510L

Sensor Serial Number : -

Serial Number : 130026

Instrument Status : Used

ID : BKK_FS0619

Location of Calibration : LAB 4 AIR VELOCITY METER

REVIEW BY .....

APPROVED BY .....

NEXT CAL DATE..... 09/09/26

Calibration Environment and Details

Temperature : 23 °C ± 3 °C

Humidity : 55 %RH ± 20 %RH

Barometric Pressure : 1013 hPa ± 10 hPa

Received Date : 3 September 2025

Calibration Date : 10 September 2025

Calibration Procedure : In-house method CP-AFM-01 by Comparison technique with Standard Primary Flow Calibrator

Reference Standard	Model	Serial Number	Traceble	Due Calibration
Air Flow Meter	Gilibrator 3 Low flow	18501010006	Sensidyne	5 May 2026
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	6 May 2026
Temperature meter	GT 11	08000057	Qreborn	15 October 2025
Pressure meter	CPG2400	41000KDU/651882	TPA	21 October 2025

Traceability :

This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01 and MIT NSC-TISI-TIS Accreditation No. 0052

Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k = 2, providing a level of confidence approximately 95 %.

Calibration By :

Mr. Noppadon Luangart

Service Calibration Engineer

Approved By :

Mr. Pacit Mathavorn

Calibration Engineer Supervisor

Issue Date : 10 September 2025

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate No : 25-AFM-207

Request No : Req-2025-1987

Result of Calibration : Without Adjustment

STD Reading			UUC Readinng			Error	Uncertainty		
Temperature (°C)	Pressure (kPa)	Flow (cc/min)	Temperature (°C)	Pressure (kPa)	Flow (cc/min)	(cc/min)	(cc/min)	(°C)	(kPa)
25.5	100.98	20	-	-	20.042	0.0	1.6	1.0	0.50
25.5	100.90	50	-	-	49.921	-0.1	4.0	1.0	0.50
25.5	100.91	100	-	-	100.09	0.1	3.6	1.0	0.50
25.4	100.86	150	-	-	150.34	0.3	5.4	1.0	0.50
25.6	100.93	199	-	-	200.17	1.2	7.2	1.0	0.50
25.6	100.95	301	-	-	300.05	-1	11	1.0	0.50
25.7	100.96	402	-	-	401.03	-1	14	1.0	0.50
25.7	100.95	503	-	-	500.26	-3	10	1.0	0.50

Note STD : Standard UUC : Unit Under Calibration

- UUC Reference Condition : At atmospheric pressure and room temperature condition, Air☐
- Flow Rate was corrected for non-standard operating condition by using equation :

$$Qmeas = \mathrm{Qref}\, x \frac{\mathrm{Pref}}{\mathrm{Pmeas}} x \frac{\mathrm{Tmeas}}{\mathrm{Tref}}$$

where Q = Flow Rate P = Absolute Pressure T = Absolute Temperature

meas = Measurement Condition ref = Standard Condition

* Indicates non accredited

End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

FM-708-AFM-01 Rev.06 Issue date 21/2/25

ALS Laboratory Group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Phatthanakan, Suan Luang, Bangkok 10250
T +66 2 760 3000 F +66 2 760 3197

Certificate of Calibration

Certificate No. C-070126-RYG_FS0499

Air Sampling Pump Detail

Equipment name	: Personal Air Sampling Pump	Equiment ID	: RYG_FS0499
Brand	: Gilian	Serial No.	: 20201110088
Model/Type	: GilAir Plus	Calibration Date	: 07-Jan-26
		Next calibration date	: 07-Apr-26

Reference Standard Low Flow Meter

Equipment name	: Air Flow Meter	Equiment ID	: BKK_FS0619
Brand	: MesaLabs	Serial No.	: 130026
Model/Type	: Defender 510-L	Calibration Date	: 10-Sep-25
		Due Date	: 9-Sep-26

Reference Standard High Flow Meter

Equipment name	: Air Flow Meter	Equiment ID	: BKK_FS0614
Brand	: MesaLabs	Serial No.	: 151114
Model/Type	: Defender 510-M	Calibration Date	: 10-Sep-25
		Due Date	: 09-Sep-26

Calibration Data

Air Sampling Pump setting (cc/min)	Reference Std. Flow Reading (cc/min)			Avg. (cc/min)	%Error acceptance	Acceptable range (cc/min)	Evaluation (Pass/ Fail)
	1	2	3				
Low Flow							
20	19.3	19.5	19.9	19.6	5%	19 - 21	Passed
50	50.2	49.2	52.2	50.5	5%	48 - 53	Passed
100	99.0	99.2	99.1	99.1	5%	95 - 105	Passed
200	199.3	198.2	197.7	198.4	5%	190 - 210	Passed
High Flow							
500	506.1	503.3	505.8	505.1	3%	485 - 515	Passed
1000	1009.1	1007.6	1009.3	1008.7	3%	970 - 1030	Passed
2000	2000.3	2000.0	2001.3	2000.5	3%	1940 - 2060	Passed
2500	2503.3	2501.0	2502.2	2502.2	3%	2425 - 2575	Passed

---------- END OF REPORT ----------

Calibrated By: .....
(Mr. Watcharin Pongsamsuan)
RYG Field Services Scientist (1)

Approved By: .....
(Mr. Supot Salamteh)
Field Services Section Head

Issue date : 08-Jan-26

ALS Laboratory Group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Phatthanakan, Suan Luang, Bangkok 10250
T +66 2 760 3000 F +66 2 760 3197

Certificate of Calibration

Certificate No. C-070126-RYG_FS0135

Air Sampling Pump Detail

Equipment name	: Personal Air Sampling Pump	Equiment ID	: RYG_FS0135
Brand	: Gilian	Serial No.	: 20150410011
Model/Type	: GilAir Plus	Calibration Date	: 07-Jan-26
		Next calibration date	: 07-Apr-26

Reference Standard Low Flow Meter

Equipment name	: Air Flow Meter	Equiment ID	: BKK_FS0619
Brand	: MesaLabs	Serial No.	: 130026
Model/Type	: Defender 510-L	Calibration Date	: 10-Sep-25
		Due Date	: 9-Sep-26

Reference Standard High Flow Meter

Equipment name	: Air Flow Meter	Equiment ID	: BKK_FS0614
Brand	: MesaLabs	Serial No.	: 151114
Model/Type	: Defender 510-M	Calibration Date	: 10-Sep-25
		Due Date	: 09-Sep-26

Calibration Data

Air Sampling Pump setting (cc/min)	Reference Std. Flow Reading (cc/min)			Avg. (cc/min)	%Error acceptance	Acceptable range (cc/min)	Evaluation (Pass/ Fail)
	1	2	3				
Low Flow							
20	20.3	20.8	20.4	20.5	5%	19 - 21	Passed
50	49.4	48.9	49.6	49.3	5%	48 - 53	Passed
100	98.9	102.6	101.9	101.1	5%	95 - 105	Passed
200	198.5	198.1	199.2	198.6	5%	190 - 210	Passed
High Flow							
500	501.5	497.8	499.0	499.4	3%	485 - 515	Passed
1000	999.5	996.0	992.5	996.0	3%	970 - 1030	Passed
2000	1999.9	2006.1	2003.2	2003.1	3%	1940 - 2060	Passed
2500	2496.2	2494.6	2493.6	2494.8	3%	2425 - 2575	Passed

---------- END OF REPORT ----------

Calibrated By: .....
(Mr. Watcharin Pongsamsuan)
RYG Field Services Scientist (1)

Approved By: .....
(Mr. Supot Salamteh)
Field Services Section Head

Issue date : 08-Jan-26

© 2025 by Agilent Technologies

Certificate of System Qualification

GC-OQ

REVIEW BY Jida K.

APPROVED BY

NEXT CAL DATE 21/10/26

System ID:	BKK_EN0126_GC6
Organization Name:	ALS Laboratory Group (Thailand) Co., Ltd.
Organization Location:	104 Soi 40 Phattanakan Rd., Khwang Suan Luang, Khet Suan Luang, BANGKOK 10250
Date:	October 22, 2025 2:51:58 PM
EQP Name:	AgilentRecommended
EQP Revision:	GC.02.53
Overall Qualification Status:	Pass

CDS Logon Verification - GC

Logon: Suriya Thongkaew

Overall CDS Logon Verification - GC Test Status

Pass

System Inspection and Basic Safety and Operation

Name: 7890

Setpoint Status: **Pass**

Overall System Inspection and Basic Safety and Operation Test Status

Pass

Inlet Pressure Decay

Name: 7890

Front SSL

Setpoint Status: **Pass**

Pressure: 25.0 psi

Pressure Change: 0.3 psi /5 minutes

Agilent Recommended: >= -2.0 and <= 0.5

© 2025 by Agilent Technologies

Agilent CrossLab Compliance Services

Overall Inlet Pressure Decay Test Status

Pass

Inlet Pressure Accuracy

Name: 7890

Front SSL

Setpoint Status: **Pass**

	Setpoint		Actual	
Inlet Pressure:	25.0	psi	25.2	psi

Accuracy: 0.2 psi

Agilent Recommended: <= 1.2

Overall Inlet Pressure Accuracy Test Status

Pass

Inlet Pressure Decay

Name: 7890

Back SSL

Setpoint Status: **Pass**

Pressure: 25.0 psi

Pressure Change: 0.4 psi /5 minutes

Agilent Recommended: >= -2.0 and <= 0.5

Overall Inlet Pressure Decay Test Status

Pass

Inlet Pressure Accuracy

Name: 7890

Back SSL

Setpoint Status: Pass

	Setpoint		Actual	
Inlet Pressure:	25.0	psi	25.2	psi

Accuracy: 0.2 psi

Agilent Recommended: <= 1.2

Overall Inlet Pressure Accuracy Test Status

Pass

22111dijeuifhuie1

Detector Flow Accuracy

Name: 7890

Front FID

Setpoint Status: Pass

Flow Type: Fuel

Setpoint: 30.0 mL/min Measured Flow: 30.8 mL/min

Accuracy: 0.8 mL/min

Agilent Recommended: <= 10.0 % setpoint (3.0 ml/min)

Limit is percentage of setpoint or 0.5 ml/minute, whichever is largest.

Setpoint Status: Pass

Flow Type: Oxidizer

Setpoint: 400.0 mL/min Measured Flow: 396.0 mL/min

Accuracy: 4.0 mL/min

Agilent Recommended: <= 10.0 % setpoint (40.0 ml/min)

Limit is percentage of setpoint or 0.5 ml/minute, whichever is largest.

Setpoint Status: Pass

Flow Type: Makeup

Setpoint: 25.0 mL/min Measured Flow: 24.7 mL/min

Accuracy: 0.3 mL/min

Agilent Recommended: <= 10.0 % setpoint (2.5 ml/min)

Limit is percentage of setpoint or 0.5 ml/minute, whichever is largest.

Overall Detector Flow Accuracy Test Status

Pass

Detector Flow Accuracy

Name: 7890

Back FID

Setpoint Status: Pass

Flow Type: Fuel

Setpoint: 30.0 mL/min Measured Flow: 29.5 mL/min

Accuracy: 0.5 mL/min

Agilent Recommended: <= 10.0 % setpoint (3.0 ml/min)

Limit is percentage of setpoint or 0.5 ml/minute, whichever is largest.

Setpoint Status: Pass

Flow Type: Oxidizer

Setpoint: 400.0 mL/min Measured Flow: 397.0 mL/min

Accuracy: 3.0 mL/min

Agilent Recommended: <= 10.0 % setpoint (40.0 ml/min)

Limit is percentage of setpoint or 0.5 ml/minute, whichever is largest.

Setpoint Status: Pass

Flow Type: Makeup

Setpoint: 25.0 mL/min Measured Flow: 24.8 mL/min

Accuracy: 0.2 mL/min

Agilent Recommended: <= 10.0 % setpoint (2.5 ml/min)

Limit is percentage of setpoint or 0.5 ml/minute, whichever is largest.

Overall Detector Flow Accuracy Test Status

Pass

GC Oven Temperature Accuracy

Name: 7890

Setpoint Status:	**Pass**					
Zone:	Oven					
	Setpoint/Actual					
Temperature:	230.0	229.1	°C			
Accuracy:		-0.9	°C			
Agilent Recommended:	>=	-1.0	% setpoint in K	(	-5.0	°C)
	<=	1.0	% setpoint in K	(	5.0	°C)

Setpoint Status:	**Pass**					
Zone:	Oven					
	Setpoint/Actual					
Temperature:	100.0	99.9	°C			
Accuracy:		-0.1	°C			
Agilent Recommended:	>=	-1.0	% setpoint in K	(	-3.7	°C)
	<=	1.0	% setpoint in K	(	3.7	°C)

Overall GC Oven Temperature Accuracy Test Status

Pass

GC Oven Temperature Stability

Name:	7890		
Setpoint Status:	**Pass**		
	Setpoint/Average		
Temperature:	100.0	99.95	°C
Stability:		0.1	°C
Agilent Recommended:	<=	0.5	

Overall GC Oven Temperature Stability Test Status

Pass

Scouting Run

Tested Combination1	Front	SSL	/ Front	FID	
	Injection Tower				
Name:	7693A				

22111dijeuifhuie1

© 2025 by Agilent Technologies Agilent CrossLab Compliance Services

Setpoint Status:	**Completed**		
Injection Volume on Column:	1.0	uL	

Overall Scouting Run Status

Completed

Noise and Drift

Tested Combination1	Front	SSL	/ Front	FID		
Name:	7890					
Setpoint Status:	**Pass**					
Base Signal:	14.3	pA				
		ASTM Noise			Drift	
		pA			pA/h	
		0.05			0.03	
Agilent Recommended:	<=	0.10		<=	2.50	
Status:	Pass			Pass		

Overall Noise and Drift Test Status

Pass

Injection Precision

Tested Combination1	Front	SSL	/ Front	FID			
Name:	7693A						
Setpoint Status:	**Pass**						
Injection Volume on Column:	1.0	uL					
Area RSD:		0.33	%	Retention Time RSD:		0.10	%
Agilent Recommended:	<=	3.00			<=	1.00	

Overall Injection Precision Test Status

Pass

Signal to Noise

Tested Combination1	Front	SSL	/ Front	FID
	Injection Tower			
Name:	7890			

Setpoint Status: **Pass**

Signal to Noise:		1393680
Agilent Recommended:	>=	300000

Overall Signal to Noise Test Status

Pass

Scouting Run

Tested Combination2	Back	SSL	/ Back	FID
	Injection Tower			
Name:	7693A			

Setpoint Status: **Completed**

Injection Volume on Column: 1.0 uL

Overall Scouting Run Status

Completed

Noise and Drift

Tested Combination2	Back	SSL	/ Back	FID
Name:	7890			

Setpoint Status: **Pass**

Base Signal: 13.3 pA

		ASTM Noise		Drift
		pA		pA/h
		0.05		0.01
Agilent Recommended:	<=	0.10	<=	2.50
Status:		Pass		Pass

Overall Noise and Drift Test Status

Pass

Injection Precision

Tested Combination2	Back	SSL	/ Back	FID
Name:	7693A			

Setpoint Status: **Pass**

Injection Volume on Column: 1.0 uL

Area RSD:		0.43	%	Retention Time RSD:	0.09 %
Agilent Recommended:	<=	3.00		<=	1.00

Overall Injection Precision Test Status

Pass

Signal to Noise

Tested Combination2	Back	SSL	/ Back	FID
	Injection Tower			
Name:	7890			

Setpoint Status: **Pass**

Signal to Noise:		1251862
Agilent Recommended:	>=	300000

Overall Signal to Noise Test Status

Pass

Instrument Details

Purpose

This section describes the as found system configuration.

Details

System

System ID	BKK_EN0126_GC6
Manufacturer	Agilent Technologies
Name	7890
Flow Data Input	Manual Data
Temperature Data Input	Manual Data or Other Data Logging

Tested Combination1

Injection Technique	Injection Tower
Sampler Identifier	Sampler 1
Inlet	Front
Detector	Front
LTM Included?	No

Tested Combination2

Injection Technique	Injection Tower
Sampler Identifier	Sampler 2
Inlet	Back
Detector	Back
LTM Included?	No

Sampler 1

Manufacturer	Agilent Technologies
Type	Injection Tower
Name	7693A
Model Number	G4513A
Serial Number	CN10340103
Firmware Revision	A.11.06
Usage	Sample Injection
Location	Front
Syringe Volume (µL)	10

Sampler 2

Manufacturer	Agilent Technologies
Type	Injection Tower
Name	7693A
Model Number	G4513A
Serial Number	CN16280128
Firmware Revision	A.11.06
Usage	Sample Injection
Location	Back
Syringe Volume (µL)	10

Sampler 3

Manufacturer	Agilent Technologies
Type	Tray
Name	7693A
Model Number	G4514A
Serial Number	CN18250032
Firmware Revision	A.12.04
Vial Heater	Not installed

Mainframe 1

Manufacturer	Agilent Technologies
Name	7890
Model Number	G3440A
Serial Number	CN11461066
Firmware Revision	A.01.16
Component ID/Asset No.	BKK_EN0126_GC-6
Oven Type	Standard

Inlet 1

Manufacturer	Agilent Technologies
Name	7890
Type	SSL
Location	Front
Carrier Gas	Helium
Control Type	Electronic Pressure Control (EPC)
Purged Inlet	Yes

Inlet 2

Manufacturer	Agilent Technologies
Name	7890
Type	SSL
Location	Back
Carrier Gas	Helium
Control Type	Electronic Pressure Control (EPC)
Purged Inlet	Yes

Detector 1

Manufacturer	Agilent Technologies
Name	7890
Type	FID
Adapter	Capillary
Control Type	Electronic Pressure Control (EPC)
Location	Front
Makeup Gas	Nitrogen

Detector 2

Manufacturer	Agilent Technologies
Name	7890
Type	FID
Adapter	Capillary
Control Type	Electronic Pressure Control (EPC)
Location	Back
Makeup Gas	Nitrogen

© 2025 by Agilent Technologies Agilent CrossLab Compliance Services

Electronic Signature

Purpose

This signature page was created and published because the ACE sign-off action was executed, which is valid for the entire document, including attachments. The ACE sign-off is an electronic signature that requires two distinct identification components: unique username and personal password. The Agilent representative who has delivered this service understands the meaning and legal status of an electronic signature. As a trained official operator, the Agilent representative has a unique password and logon to access ACE and electronically sign this document. (Other e-signatures can be applied to this document using a Document Content Management or other suitable method defined in your data access and control procedures.)

Details

Full Name of Signer:	Suriya Thongkaew
Logged On User Name:	suriya.thongkaew@non.agilent.com
Signature Creation Date:	October 22, 2025
Reason for Signature:	Executed protocol and published this original version of document

ACE Self Qualification Status

The installed version of ACE used to deliver this service passed qualification; the results conform with expected values. The self qualification summary report is available in the session folder location SDS\ClearStore\AceSelfQualification.

Regulatory Disclaimer

This document provides a protocol to verify and record instrument configuration and evidence of proper operation. It has been prepared from our interpretation of applicable regulations as well as industry best practices. The document is designed to provide an important component of a complete compliance package. Validation depends upon many factors and use of this protocol alone does not assure compliance. Agilent Technologies makes no promises or representations as to its sufficiency for any specific regulatory program.

Warranty

Agilent Technologies makes no warranty of any kind to this material, including but not limited to, the implied warranties or merchantability and fitness for a particular purpose. Agilent Technologies shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance, or use of this material.

User Name: suriya.thongkaew
Report Generated by Hostname: DESKTOP-2H6MTKJ

System Id: BKK_EN0126_GC6
Print Date: October 22, 2025 2:52:00 PM

OQ2025 GC ALS GC-6 CN11461066 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 21, 2025 1:44:51 PM	Audit	SessionCreated	Session	Host Name: DESKTOP-2H6MTKJ, Drive Serial Number: 76C1E981
October 21, 2025 1:44:51 PM	start	Configuration	Session	None
October 21, 2025 1:44:51 PM	Audit	Entitlement	Licensing	Session identifier generated: XYP0-PNEJ-0W00-0RZ5-HR80
October 21, 2025 1:48:11 PM	Audit	Entitlement	Licensing	Succesfully unlocked session identified by XYP0-PNEJ-0W00-0RZ5-HR80 with unlock code 76BX-519E-XKYX-1JR1-JR60
October 21, 2025 1:57:15 PM	Audit	EqpLoaded	Session	EQP details for primary technique [Gc] - File path: [ProtocolPacks/Gc/Configurations/02.53/Gc.02.53.eqp], EQP File Name: [Gc.02.53.eqp], EQP Name: [AgilentRecommended],Protocol Revision :[Gc.02.53]
October 21, 2025 1:57:39 PM	End	Configuration	Session	None
October 21, 2025 1:57:46 PM	start	Qualification	Session	OQ
October 21, 2025 1:57:46 PM	start	Execution	CDS Logon Verification - GC - 7890: - Qualitative test	None
October 21, 2025 2:18:54 PM	End	Execution	CDS Logon Verification - GC - 7890: - Qualitative test	Run Count : 1

User Name: suriya.thongkaew
Report Generated by Hostname: DESKTOP-2H6MTKJ

System Id: BKK_EN0126_GC6
Print Date: October 22, 2025 2:52:00 PM

OQ2025 GC ALS GC-6 CN11461066 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 21, 2025 2:19:27 PM	start	Execution	System Inspection and Basic Safety and Operation - 7890: - Qualitative Test - No setpoints associated	None
October 21, 2025 2:19:47 PM	End	Execution	System Inspection and Basic Safety and Operation - 7890: - Qualitative Test - No setpoints associated	Run Count : 1
October 21, 2025 2:19:50 PM	start	Execution	Inlet Pressure Decay - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: >= -2.0 psi and <= 0.5 psi	None
October 21, 2025 2:25:44 PM	End	Execution	Inlet Pressure Decay - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: >= -2.0 psi and <= 0.5 psi	Run Count : 1
October 21, 2025 2:25:52 PM	start	Execution	Inlet Pressure Accuracy - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	None
October 21, 2025 2:28:43 PM	End	Execution	Inlet Pressure Accuracy - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	Run Count : 1
October 21, 2025 2:28:45 PM	start	Execution	Inlet Pressure Decay - Back SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: >= -2.0 psi and <= 0.5 psi	None
October 21, 2025 2:33:42 PM	End	Execution	Inlet Pressure Decay - Back SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: >= -2.0 psi and <= 0.5 psi	Run Count : 1
October 21, 2025 2:33:50 PM	start	Execution	Inlet Pressure Accuracy - Back SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	None

User Name: suriya.thongkaew
Report Generated by Hostname: DESKTOP-2H6MTKJ
System Id: BKK_EN0126_GC6
Print Date: October 22, 2025 2:52:00 PM

OQ2025 GC ALS GC-6 CN11461066 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 21, 2025 2:34:27 PM	End	Execution	Inlet Pressure Accuracy - Back SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	Run Count : 1
October 21, 2025 2:34:32 PM	start	Execution	Detector Flow Accuracy - Front FID: - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	None
October 21, 2025 2:50:39 PM	Audit	Data	Detector Flow Accuracy - Front FID: - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry
October 21, 2025 2:50:41 PM	start	Execution	Detector Flow Accuracy - Front FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	None
October 21, 2025 2:50:45 PM	start	Execution	Detector Flow Accuracy - Front FID: - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	None
October 21, 2025 2:50:53 PM	End	Execution	Detector Flow Accuracy - Front FID: - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	Run Count : 1
October 21, 2025 2:50:56 PM	start	Execution	Detector Flow Accuracy - Front FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	None
October 21, 2025 2:54:08 PM	Audit	Data	Detector Flow Accuracy - Front FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry
October 21, 2025 2:54:15 PM	Audit	Data	DataManager	DataManager was in a data verification state but the user chose to start over
October 21, 2025 2:54:31 PM	Audit	Data	Detector Flow Accuracy - Front FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry
October 21, 2025 2:54:34 PM	End	Execution	Detector Flow Accuracy - Front FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	Run Count : 1

© 2025 by Agilent Technologies Agilent CrossLab Compliance Services

User Name: suriya.thongkaew
Report Generated by Hostname: DESKTOP-2H6MTKJ
System Id: BKK_EN0126_GC6
Print Date: October 22, 2025 2:52:00 PM

OQ2025 GC ALS GC-6 CN11461066 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 21, 2025 2:54:48 PM	start	Execution	Detector Flow Accuracy - Front FID: - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	None
October 21, 2025 2:57:00 PM	Audit	Data	Detector Flow Accuracy - Front FID: - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry
October 21, 2025 2:57:03 PM	End	Execution	Detector Flow Accuracy - Front FID: - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	Run Count : 1
October 21, 2025 2:57:38 PM	start	Execution	Detector Flow Accuracy - Back FID: - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	None
October 21, 2025 3:00:15 PM	Audit	Data	Detector Flow Accuracy - Back FID: - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry
October 21, 2025 3:00:17 PM	End	Execution	Detector Flow Accuracy - Back FID: - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	Run Count : 1
October 21, 2025 3:00:20 PM	start	Execution	Detector Flow Accuracy - Back FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	None
October 21, 2025 3:03:03 PM	Audit	Data	Detector Flow Accuracy - Back FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry
October 21, 2025 3:03:06 PM	End	Execution	Detector Flow Accuracy - Back FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	Run Count : 1
October 21, 2025 3:03:08 PM	start	Execution	Detector Flow Accuracy - Back FID: - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	None
October 21, 2025 3:07:25 PM	Audit	Data	Detector Flow Accuracy - Back FID: - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry

User Name: suriya.thongkaew
Report Generated by Hostname: DESKTOP-2H6MTKJ
System Id: BKK_EN0126_GC6
Print Date: October 22, 2025 2:52:00 PM

OQ2025 GC ALS GC-6 CN11461066 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 21, 2025 3:07:28 PM	End	Execution	Detector Flow Accuracy - Back FID: - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	Run Count : 1
October 21, 2025 3:07:53 PM	start	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
October 21, 2025 3:21:20 PM	Audit	Data	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry
October 21, 2025 3:21:22 PM	End	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1
October 21, 2025 3:21:36 PM	start	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
October 21, 2025 3:30:43 PM	Audit	Data	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry
October 21, 2025 3:30:45 PM	End	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1
October 21, 2025 3:30:48 PM	start	Execution	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	None
October 21, 2025 3:50:20 PM	Audit	Data	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Manual Data Entry

Page 5 / 12

User Name: suriya.thongkaew
Report Generated by Hostname: DESKTOP-2H6MTKJ
System Id: BKK_EN0126_GC6
Print Date: October 22, 2025 2:52:00 PM

OQ2025 GC ALS GC-6 CN11461066 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 21, 2025 3:50:24 PM	End	Execution	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Run Count : 1
October 21, 2025 3:50:31 PM	start	Execution	GC Scouting Run - Injection Tower, Front SSL, Front FID: - Part of System Preparation - No limits associated	None
October 21, 2025 3:55:30 PM	Audit	AceClosed	Session	None
October 22, 2025 10:10:41 AM	Audit	AceRestarted	Session	Host Name: DESKTOP-2H6MTKJ, Drive Serial Number: 76C1E981
October 22, 2025 10:10:42 AM	Audit	SessionReloaded	Session	None
October 22, 2025 10:10:44 AM	start	Qualification	Session	OQ
October 22, 2025 10:10:45 AM	start	Execution	GC Scouting Run - Injection Tower, Front SSL, Front FID: - Part of System Preparation - No limits associated	None
October 22, 2025 2:15:45 PM	Audit	Data	DataManager	DataManager was in a data verification state but the user chose to start over
October 22, 2025 2:16:36 PM	Audit	Data	GC Scouting Run - Injection Tower, Front SSL, Front FID: - Part of System Preparation - No limits associated	Data files Path : D:\ALS GC-6\OQ2025\SCOUTING_01.D\FID1A.ch

Page 6 / 12

User Name: suriya.thongkaew System Id: BKK_EN0126_GC6
Report Generated by Hostname: DESKTOP-2H6MTKJ Print Date: October 22, 2025 2:52:00 PM

OQ2025 GC ALS GC-6 CN11461066 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 22, 2025 2:17:00 PM	Audit	Reporting	Reintegration	Reintegration Count: 1 -- [Integration Type: Injection;Baseline Correction Mode: Advanced;Initial Slope Sensitivity: 10;Initial Peak Width: 0.01;Initial Area Reject: 0;Initial Height Reject: 100;Integration: Off at 0;Integration: On at 0.1;Integration: Off at 0.5]
October 22, 2025 2:17:42 PM	End	Execution	GC Scouting Run - Injection Tower, Front SSL, Front FID: - Part of System Preparation - No limits associated	Run Count : 1
October 22, 2025 2:17:53 PM	start	Execution	Noise and Drift - Front FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	None
October 22, 2025 2:19:13 PM	Audit	Data	Noise and Drift - Front FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	Data files Path : D:\ALS GC-6\OQ2025\OQ2025 2025-10-22 11-05-22\SIGNSDRF_F_01. D\FID1A.ch
October 22, 2025 2:19:28 PM	End	Execution	Noise and Drift - Front FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	Run Count : 1
October 22, 2025 2:19:30 PM	start	Execution	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	None

Page 7 / 12

User Name: suriya.thongkaew System Id: BKK_EN0126_GC6
Report Generated by Hostname: DESKTOP-2H6MTKJ Print Date: October 22, 2025 2:52:00 PM

OQ2025 GC ALS GC-6 CN11461066 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 22, 2025 2:19:56 PM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : D:\ALS GC-6\OQ2025\OQ2025 2025-10-22 11-05-22\INJPREC_F_02.D\ FID1A.ch
October 22, 2025 2:19:56 PM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : D:\ALS GC-6\OQ2025\OQ2025 2025-10-22 11-05-22\INJPREC_F_03.D\ FID1A.ch
October 22, 2025 2:19:56 PM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : D:\ALS GC-6\OQ2025\OQ2025 2025-10-22 11-05-22\INJPREC_F_04.D\ FID1A.ch
October 22, 2025 2:19:56 PM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : D:\ALS GC-6\OQ2025\OQ2025 2025-10-22 11-05-22\INJPREC_F_05.D\ FID1A.ch
October 22, 2025 2:19:56 PM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : D:\ALS GC-6\OQ2025\OQ2025 2025-10-22 11-05-22\INJPREC_F_06.D\ FID1A.ch
October 22, 2025 2:19:56 PM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : D:\ALS GC-6\OQ2025\OQ2025 2025-10-22 11-05-22\INJPREC_F_07.D\ FID1A.ch

Page 8 / 12

User Name: suriya.thongkaew System Id: BKK_EN0126_GC6
Report Generated by Hostname: DESKTOP-2H6MTKJ Print Date: October 22, 2025 2:52:00 PM

OQ2025 GC ALS GC-6 CN11461066 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 22, 2025 2:20:04 PM	Audit	Reporting	Reintegration	Reintegration Count: 1 -- [Integration Type: Injection;Baseline Correction Mode: Advanced;Initial Slope Sensitivity: 10;Initial Peak Width: 0.01;Initial Area Reject: 0;Initial Height Reject: 100;Integration: Off at 0;Integration: On at 0.1;Integration: Off at 0.5]
October 22, 2025 2:20:24 PM	End	Execution	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Run Count : 1
October 22, 2025 2:20:34 PM	start	Execution	Signal to Noise - Injection Tower, Front SSL, Front FID: - Detector FID - L: >= 300000	None
October 22, 2025 2:20:58 PM	Audit	Data	Signal to Noise - Injection Tower, Front SSL, Front FID: - Detector FID - L: >= 300000	Data files Path : D:\ALS GC-6\OQ2025\OQ2025 2025-10-22 11-05-22\SIGTONS_F_01.D\ FID1A.ch
October 22, 2025 2:21:06 PM	Audit	Reporting	Reintegration	Reintegration Count: 1 -- [Integration Type: Injection;Baseline Correction Mode: Advanced;Initial Slope Sensitivity: 10;Initial Peak Width: 0.01;Initial Area Reject: 0;Initial Height Reject: 100;Integration: Off at 0;Integration: On at 0.1;Integration: Off at 0.5]
October 22, 2025 2:21:19 PM	End	Execution	Signal to Noise - Injection Tower, Front SSL, Front FID: - Detector FID - L: >= 300000	Run Count : 1

Page 9 / 12

© 2025 by Agilent Technologies Agilent CrossLab Compliance Services

User Name: suriya.thongkaew System Id: BKK_EN0126_GC6
Report Generated by Hostname: DESKTOP-2H6MTKJ Print Date: October 22, 2025 2:52:00 PM

OQ2025 GC ALS GC-6 CN11461066 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 22, 2025 2:21:25 PM	start	Execution	GC Scouting Run - Injection Tower, Back SSL, Back FID: - Part of System Preparation - No limits associated	None
October 22, 2025 2:25:23 PM	Audit	Data	GC Scouting Run - Injection Tower, Back SSL, Back FID: - Part of System Preparation - No limits associated	Data files Path : D:\ALS GC-6\OQ2025_B\SCOUTING _B_01.D\FID2B.ch
October 22, 2025 2:26:18 PM	End	Execution	GC Scouting Run - Injection Tower, Back SSL, Back FID: - Part of System Preparation - No limits associated	Run Count : 1
October 22, 2025 2:26:21 PM	start	Execution	Noise and Drift - Back FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	None
October 22, 2025 2:27:00 PM	Audit	Data	Noise and Drift - Back FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	Data files Path : D:\ALS GC-6\OQ2025_B\OQ2025 2025-10-22 11-05-22\SIGNSDRF_B_01. D\FID2B.ch
October 22, 2025 2:27:42 PM	End	Execution	Noise and Drift - Back FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	Run Count : 1
October 22, 2025 2:27:46 PM	start	Execution	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	None
October 22, 2025 2:28:07 PM	Audit	Data	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : D:\ALS GC-6\OQ2025_B\OQ2025 2025-10-22 11-05-22\INJPREC_B_02.D\ FID2B.ch

Page 10 / 12

User Name: suriya.thongkaew System Id: BKK_EN0126_GC6
Report Generated by Hostname: DESKTOP-2H6MTKJ Print Date: October 22, 2025 2:52:00 PM

OQ2025 GC ALS GC-6 CN11461066 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 22, 2025 2:28:07 PM	Audit	Data	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : D:\ALS GC-6\OQ2025_B\OQ2025 2025-10-22 11-05-22\INJPREC_B_03.D\ FID2B.ch
October 22, 2025 2:28:07 PM	Audit	Data	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : D:\ALS GC-6\OQ2025_B\OQ2025 2025-10-22 11-05-22\INJPREC_B_04.D\ FID2B.ch
October 22, 2025 2:28:07 PM	Audit	Data	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : D:\ALS GC-6\OQ2025_B\OQ2025 2025-10-22 11-05-22\INJPREC_B_05.D\ FID2B.ch
October 22, 2025 2:28:07 PM	Audit	Data	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : D:\ALS GC-6\OQ2025_B\OQ2025 2025-10-22 11-05-22\INJPREC_B_06.D\ FID2B.ch
October 22, 2025 2:28:07 PM	Audit	Data	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : D:\ALS GC-6\OQ2025_B\OQ2025 2025-10-22 11-05-22\INJPREC_B_07.D\ FID2B.ch
October 22, 2025 2:28:21 PM	End	Execution	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Run Count : 1
October 22, 2025 2:28:28 PM	start	Execution	Signal to Noise - Injection Tower, Back SSL, Back FID: - Detector FID - L: >= 300000	None

Page 11 / 12

© 2025 by Agilent Technologies Agilent CrossLab Compliance Services

User Name: suriya.thongkaew System Id: BKK_EN0126_GC6
Report Generated by Hostname: DESKTOP-2H6MTKJ Print Date: October 22, 2025 2:52:00 PM

OQ2025 GC ALS GC-6 CN11461066 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 22, 2025 2:28:47 PM	Audit	Data	Signal to Noise - Injection Tower, Back SSL, Back FID: - Detector FID - L: >= 300000	Data files Path : D:\ALS GC-6\OQ2025_B\OQ2025 2025-10-22 11-05-22\SIGTONS_B_01.D\ FID2B.ch
October 22, 2025 2:29:53 PM	End	Execution	Signal to Noise - Injection Tower, Back SSL, Back FID: - Detector FID - L: >= 300000	Run Count : 1
October 22, 2025 2:30:01 PM	End	Qualification	Session	OQ
October 22, 2025 2:30:01 PM	start	Reporting	Session	None
October 22, 2025 2:50:41 PM	Audit	Reporting	Session	Report Generated : Certificate
October 22, 2025 2:51:22 PM	Audit	Reporting	Session	Report Generated : Report

Page 12 / 12

ระดับเสียงในสถานประกอบการ

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-69/0204 **MTC No.** EEL. BP. 152/0169

CALIBRATION CERTIFICATE

Submitted by : S.P.S.CONSULTING SERVICE CO.,LTD.

Address : 7 Soi Phaholyothin 24, Phaholyothin Road, Jompol, Chatuchak, Bangkok 10900.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre. Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Sound Calibrator

Manufacturer : ACO

Model : 2127

Serial No. : 130006

Ambient Environment

Temperature : (23 + 3) °C

Relative Humidity : (50 ± 15) %

Ambient Pressure : (101.325 ± 1.500) kPa

Standards used :

1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.
2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.
3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.
4. Digital Multimeter Agilent 34401A S/N MY44005560.
5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.
6. Audio Analyzer Keithley 2015-P S/N 4106495.
7. Condenser Microphone Bruel&Kjaer 4180 S/N 2889871.

Calibration Procedure: CP-102-04 based on IEC 60942-2003; The sound pressure level generated by sound calibrator under test shall be measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 29 Jan. 2026

Date of Calibration : 11 Feb. 2026

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

NSC-TISI-TIS 17025
CALIBRATION 0037

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-69/0204 **MTC No.** EEL. BP. 152/0169

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20μPa at 1000 Hz

Acoustic Output in dB re 20μPa, Corrected to Reference Conditions: 101.325 kPa, 23.0 °C and 50 %RH.

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	93.89	-0.11	± 0.10	±0.40 dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	999.9	-0.1	± 1.5	±1.0%

3. Total Distortion

Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	1.90	± 0.50	±3.0%

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Calibrated by :

(Mr.Weerachai Deechaiyae)

Approved by :

(Mr.Prawate Kluaypa)

Director

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 11 Feb. 2026

Date of Issue : 12 Feb. 2026

Ref : 20112690129004970O1

End of Certificate

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Noise R_207/26

Sound Level Meter Calibration Report

Acoustic Calibrator Data

Brand	ACO	Number	AC 03/56
Model	2127	Serial No.	130006
Calibration Range	94 dB, 1000 Hz	Last Calibration	11 February 2026
		Due Date	11 February 2027

Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-R40	ACO	6236	00192052	21 April 2026	93.9	93.9
ACO-R51	ACO	6236	00192063	21 April 2026	93.8	93.9
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.89 ± 0.10 dB	

Calibrated by : Heeson L.
(Mr. Heeson Lormae)

Approved by : Yutthana T.
(Mr. Yutthana Tanatharanit)

ปริมาณเสียงสะสมติดตัวบุคคล

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-69/0204 **MTC No.** EEL. BP. 152/0169

CALIBRATION CERTIFICATE

Submitted by : S.P.S.CONSULTING SERVICE CO.,LTD.

Address : 7 Soi Phaholyothin 24, Phaholyothin Road, Jompol, Chatuchak, Bangkok 10900.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre. Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Sound Calibrator

Manufacturer : ACO

Model : 2127

Serial No. : 130006

Ambient Environment

Temperature : (23 + 3) °C

Relative Humidity : (50 ± 15) %

Ambient Pressure : (101.325 ± 1.500) kPa

Standards used :

1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.
2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.
3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.
4. Digital Multimeter Agilent 34401A S/N MY44005560.
5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.
6. Audio Analyzer Keithley 2015-P S/N 4106495.
7. Condenser Microphone Bruel&Kjaer 4180 S/N 2889871.

Calibration Procedure: CP-102-04 based on IEC 60942-2003; The sound pressure level generated by sound calibrator under test shall be measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 29 Jan. 2026

Date of Calibration : 11 Feb. 2026

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

NSC-TISI-TIS 17025
CALIBRATION 0037

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-69/0204 **MTC No.** EEL. BP. 152/0169

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20μPa at 1000 Hz

Acoustic Output in dB re 20μPa, Corrected to Reference Conditions: 101.325 kPa, 23.0 °C and 50 %RH.

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	93.89	-0.11	± 0.10	±0.40 dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	999.9	-0.1	± 1.5	±1.0%

3. Total Distortion

Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	1.90	± 0.50	±3.0%

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Calibrated by :

(Mr.Weerachai Deechaiyae)

Approved by :

(Mr.Prawate Kluaypa)

Director

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 11 Feb. 2026

Date of Issue : 12 Feb. 2026

Ref : 20112690129004970O1

End of Certificate

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Noise R_207/26

Sound Level Meter Calibration Report

Acoustic Calibrator Data

Brand	ACO	Number	AC 03/56
Model	2127	Serial No.	130006
Calibration Range	94 dB, 1000 Hz	Last Calibration	11 February 2026
		Due Date	11 February 2027

Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-R40	ACO	6236	00192052	21 April 2026	93.9	93.9
ACO-R51	ACO	6236	00192063	21 April 2026	93.8	93.9
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.89 ± 0.10 dB	

Calibrated by : Heeson L.
(Mr. Heeson Lormae)

Approved by : Yutthana T.
(Mr. Yutthana Tanatharanit)