

ภาคผนวกที่ 4

เอกสารสอบเทียบความถูกต้องของเครื่องมือ

เอกสารสอบเทียบเครื่องมือการตรวจวัดคุณภาพอากาศจากปล่อง

เอกสารสอบเทียบเครื่องมือการตรวจวัดคุณภาพอากาศในบรรยากาศ

เอกสารสอบเทียบเครื่องมือการตรวจวิเคราะห์คุณภาพน้ำเสีย

เอกสารสอบเทียบเครื่องมือการตรวจวิเคราะห์คุณภาพน้ำผิวดิน

เอกสารสอบเทียบการตรวจวัดระดับเสียงที่ขอบเขตรั้วพื้นที่โรงงาน

เอกสารสอบเทียบการตรวจวัดระดับเสียงในพื้นที่ทำงาน

เอกสารสอบเทียบการตรวจวัดคุณภาพอากาศในสถานที่ทำงาน

**ตารางสรุปรายการเอกสารการสอบเทียบความถูกต้องของเครื่องมือเก็บตัวอย่าง
และเครื่องมือวิเคราะห์คุณภาพสิ่งแวดล้อม**

รายการตรวจวิเคราะห์	เครื่องมือเก็บตัวอย่าง	เครื่องมือตรวจวิเคราะห์
	ชื่อเครื่องมือ	ชื่อเครื่องมือ
1. คุณภาพอากาศจากปล่อง		
Total Suspended Particulate	Console No. R02	Digital Balance
	Pitot Tube No. R40	
NO _x	Vacuum Gauge	Spectrophotometer
SO ₂	Personal Pump SKC No. R43	-
	Rotameter No. L-R02	
CO	CO Analyzer	CO Analyzer
Acrylonitrile	Mass Flow Meter	GC/FID
Styrene	Mass Flow Meter	GC/FID
1, 3 Butadiene	Mass Flow Meter	GC/FID
Alpha Methyl Styrene	Mass Flow Meter	GC/FID
2. คุณภาพอากาศในบรรยากาศ		
NO _x	NO ₂ Analyzer -R03, R04, R05, R07	NO ₂ Analyzer
SO ₂	SO ₂ Analyzer -R01, R02, R04, R07	SO ₂ Analyzer
3. คุณภาพน้ำทิ้ง		
pH	-	pH Meter
Temperature	-	Thermometer
TDS	-	Digital Balance
SS	-	Digital Balance
BOD ₅	-	BOD Analyzer
COD	-	COD Reactor
Grease & Oil	-	Digital Balance
4. ระดับเสียงที่ขอบรั้วพื้นที่โครงการ		
L _{eq} 24 hr	Acoustic Calibrator Sound Level Meter No. ACO- R21, R22, R23, R45, R48, R49, R54, R55	-

ตารางสรุปรายการเอกสารการสอบเทียบความถูกต้องของเครื่องมือเก็บตัวอย่าง
และเครื่องมือวิเคราะห์คุณภาพสิ่งแวดล้อม

รายการตรวจวิเคราะห์	เครื่องมือเก็บตัวอย่าง	เครื่องมือตรวจวิเคราะห์
	ชื่อเครื่องมือ	ชื่อเครื่องมือ
5. ระดับเสียงในสถานประกอบการ		
L _{eq} 8 hr และ Octave Band	Acoustic Calibrator	-
	Sound Level Meter No. ACO- R40, R41, R50, R51, R52	
Noise Dose	Acoustic Calibrator	-
	Sound Level Meter No. NMD- R03, R06, R13, R22, R26, R35	
6. คุณภาพอากาศในสถานประกอบการ		
Acrylonitrile	Personal Pump SKC No. R22, R30, R32, R36, R42, R45 Rotameter No. L-R02	GC/FID
Styrene	Personal Pump SKC No. R22, R30, R32, R36, R42, R45 Rotameter No. L-R02	GC/FID
1, 3 Butadiene	Personal Pump SKC No. R22, R30, R32, R36, R42, R45 Rotameter No. L-R02	GC/MS
Alpha Methyl Styrene	Personal Pump SKC No. R22, R30, R32, R36, R42, R45 Rotameter No. L-R02	GC/FID

เอกสารสอบเทียบเครื่องมือการตรวจวัดคุณภาพอากาศจากปล่อง



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
 7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
 7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
 Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Rotameter Calibration Report (For Personal Pump Low Flow Adjust)											
Calibration Method : Dry Cal Primary Flowmeter				Model : Defender 510-H				S/N : 136833			
Calibration Data											
Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (ml/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R ²
L-R01	Dwyer	VFA-21	01/04/2026	50	100	200	50.3	101.1	201.9	0.998x + 0.955	1.000
L-R02	Dwyer	VFA-21	01/04/2026	50	100	200	50.2	101.7	201.0	0.999x + 0.367	0.999
L-R03	Dwyer	VFA-21	03/04/2026	50	100	200	50.3	101.2	201.0	1.001x + 0.605	1.000
L-R04	Dwyer	VFA-21	05/04/2026	50	100	200	50.7	100.8	200.2	1.000x + 0.719	1.000
L-R05	Dwyer	VFA-21	05/04/2026	50	100	200	50.1	101.2	200.5	1.001x - 0.213	0.999
L-R06	Dwyer	VFA-21	03/04/2026	50	100	200	50.3	100.8	200.1	0.999x + 0.639	1.000

Calibrated by : (Mr. Abdul Dangklom)	Approved by : (Mr. Peera Detudom)
--	---



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136833

Environmental Conditions

Temperature : 25 ± 3 °C
Pressure : 1010 ± 15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R ²
R01	SKC	224-PCXR4	602467	01/04/2026	1,000	1,500	2,000	1,001	1,500	2,007	1.005x - 6.003	1.000
R02	SKC	224-PCXR4	626450	05/04/2026	1,000	2,000	3,000	1,000	1,503	2,001	1.001x - 0.383	1.000
R03	SKC	224-PCXR4	691592	03/04/2026	1,000	1,500	2,000	1,005	1,501	2,000	1.007x - 15.384	0.999
R04	SKC	224-PCXR4	691672	03/04/2026	1,000	1,500	2,000	1,007	1,513	1,999	0.996x + 5.855	0.999
R05	SKC	224-PCXR4	798470	05/04/2026	1,000	1,500	2,000	1,000	1,499	1,997	0.997x + 3.107	1.000
R06	SKC	224-PCXR4	798456	03/04/2026	1,000	1,500	2,000	998	1,497	1,996	0.998x + 0.120	1.000
R07	SKC	224-PCXR4	798480	05/04/2026	1,000	1,500	2,000	1,002	1,506	2,001	0.999x + 3.219	1.000
R08	SKC	224-PCXR4	883215	03/04/2026	1,000	1,500	2,000	1,004	1,501	1,992	1.003x - 9.877	0.999
R09	SKC	224-PCXR4	034650	03/04/2026	1,000	1,500	2,000	998	1,506	2,003	1.004x - 5.723	1.000
R10	SKC	224-PCXR4	091765	03/04/2026	1,000	1,500	2,000	999	1,507	1,996	1.005x - 13.080	0.999
R11	SKC	224-PCXR4	091763	05/04/2026	1,000	1,500	2,000	1,001	1,504	2,001	1.000x + 0.104	1.000
R12	SKC	224-PCXR4	091568	03/04/2026	1,000	1,500	2,000	998	1,505	1,996	0.998x + 1.482	1.000
R13	SKC	224-PCXR4	091638	03/04/2026	1,000	1,500	2,000	1,001	1,504	2,000	0.999x + 2.097	1.000
R14	SKC	224-PCXR4	091764	05/04/2026	1,000	1,500	2,000	1,007	1,506	2,001	1.004x - 8.866	0.999
R15	SKC	224-PCXR8	529457	05/04/2026	1,000	1,500	2,000	998	1,492	1,999	1.001x - 6.322	1.000
R16	SKC	224-PCXR8	529643	03/04/2026	1,000	1,500	2,000	1,004	1,506	2,004	1.007x - 11.726	0.999
R17	SKC	224-PCXR8	529645	05/04/2026	1,000	1,500	2,000	998	1,503	1,998	1.000x - 0.703	1.000
R18	SKC	224-PCXR8	566756	03/04/2026	1,000	1,500	2,000	999	1,508	1,995	1.002x - 8.012	0.999
R19	SKC	224-PCXR8	566802	05/04/2026	1,000	1,500	2,000	998	1,502	1,998	1.000x - 0.823	1.000
R20	SKC	224-PCXR8	529089	03/04/2026	1,000	1,500	2,000	999	1,503	1,996	0.997x + 2.001	1.000
R21	SKC	224-PCXR8	665728	03/04/2026	1,000	1,500	2,000	998	1,505	1,999	1.000x - 0.483	1.000
R22	SKC	224-PCXR8	707444	05/04/2026	1,000	1,500	2,000	1,007	1,496	2,000	1.001x - 6.418	0.999
R23	SKC	224-PCXR8	761067	05/04/2026	1,000	1,500	2,000	1,001	1,502	2,004	1.002x - 1.446	1.000
R24	SKC	224-PCXR8	707893	03/04/2026	1,000	1,500	2,000	1,002	1,503	2,001	0.999x + 2.560	1.000
R25	SKC	224-PCXR8	761052	03/04/2026	1,000	1,500	2,000	1,009	1,504	2,005	0.997x + 4.106	0.999
R26	SKC	224-PCXR8	707956	05/04/2026	1,000	1,500	2,000	1,002	1,503	2,000	0.998x + 4.497	1.000
R27	SKC	224-PCXR8	707398	03/04/2026	1,000	1,500	2,000	1,001	1,505	2,004	1.003x - 1.921	1.000
R28	SKC	224-PCXR8	707481	05/04/2026	1,000	1,500	2,000	1,010	1,513	2,006	0.997x + 5.531	0.999
R29	SKC	224-PCXR8	707402	03/04/2026	1,000	1,500	2,000	1,003	1,502	1,992	1.003x - 10.216	0.999
R30	SKC	224-PCXR8	093811	05/04/2026	1,000	1,500	2,000	999	1,512	2,005	1.007x - 9.705	1.000
R31	SKC	224-PCXR8	093183	05/04/2026	1,000	1,500	2,000	1,011	1,510	2,011	1.001x + 2.983	0.999
R32	SKC	224-PCXR8	671950	03/04/2026	1,000	1,500	2,000	1,001	1,500	2,001	0.999x + 2.272	1.000
R33	SKC	224-PCXR4	626254	05/04/2026	1,000	1,500	2,000	998	1,507	2,002	1.005x - 10.975	1.000
R34	SKC	224-PCXR4	626131	05/04/2026	1,000	1,500	2,000	997	1,496	2,000	1.007x - 14.230	1.000
R35	SKC	224-PCXR8	707460	05/04/2026	1,000	1,500	2,000	998	1,509	1,996	1.000x - 2.915	1.000
R36	SKC	224-PCXR8	707446	05/04/2026	1,000	1,500	2,000	1,003	1,492	2,003	1.007x - 16.135	0.999
R37	SKC	224-PCXR8	707432	03/04/2026	1,000	1,500	2,000	999	1,507	2,005	1.003x - 6.095	1.000
R38	SKC	224-PCXR8	707349	03/04/2026	1,000	1,500	2,000	1,003	1,499	1,999	0.997x + 2.141	1.000
R39	SKC	224-PCXR8	761095	05/04/2026	1,000	1,500	2,000	1,005	1,508	2,004	1.000x - 0.152	0.999

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

Peera Detudom
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136833

Environmental Conditions

Temperature : 25 $\pm$ 3 $^{\circ}$ C
Pressure : 1010 $\pm$ 15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R ²
R40	SKC	224-PCXR4	612753	05/04/2026	1,000	1,500	2,000	1,004	1,497	2,000	0.998x + 1.430	1.000
R41	SKC	224-PCXR4	626140	03/04/2026	1,000	1,500	2,000	998	1,498	1,997	0.999x + 0.943	1.000
R42	SKC	224-PCXR4	626463	05/04/2026	1,000	1,500	2,000	1,005	1,513	1,998	0.997x + 4.138	0.999
R43	SKC	224-PCXR4	626129	03/04/2026	1,000	1,500	2,000	1,003	1,498	2,000	0.998x + 2.029	1.000
R44	SKC	224-PCXR4	602753	03/04/2026	1,000	1,500	2,000	996	1,509	1,997	1.003x - 8.036	1.000
R45	SKC	224-PCXR4	626137	05/04/2026	1,000	1,500	2,000	1,011	1,514	2,005	0.995x + 8.367	0.999

Calibrated by :

Adul Dangklom

(Mr. Adul Dangklom)

Approved by :

Peera Detudom

(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Calibration Report
Non-Dispersive Infrared CO Analyzer

Date : 06 May 2026 Brand : API Model : 300E
No. CO-R02 Serial No. 171-5

Calibrator (Dilution System)

Brand : API Model : 700
Last Cal. Date : 01 September 2025 Serial No. : 911

Reference Standard Gas

Standard Gas : Carbon Monoxide (CO) Cylinder No. : D711839
Certified Date : 14 March 2024 Expired Date : 14 March 2032 Cylinder Conc. : 4,580 ppm

Calibrating Condition

Pressure 1011 mmbar Temp. 24.6 °C % RH 50

Calibration Setting

Span	Initial Reading (Before Adj.), PPM			Final Reading (After Adj.), PPM
	Expected Concentration	Analyzer Response	%Dif	Analyzer Response
Zero	0	-0.10	-	0
CO Span	40.00	40.04	0.100	40.00

API Model 300E CO Analyzer Check List

Parameter	Observed Value	Units	Nominal Range
Range	50	PPM	0-1000 ppm
Stability	0.10	PPM	< 1 ppm With Zero Air
CO Measure	4016.4	mV	2500-4800 mV
CO Reference	3947.5	mV	2500-4800 mV
Measure/Reference Ratio	1.180	-	1.1-1.3 W/Zero Air
Sample Pressure	28.4	In-Hg-A	~2" < Ambient Absolute Pressure
Sample Flow	807	CC/Min	800 ± 10%
Sample Temperature	48.3	°C	48 ± 4
Bench Temperature	48.1	°C	48 ± 2
Wheel Temperature	68.5	°C	68 ± 2
Box Temperature	30.8	°C	Ambient Temp + 7 ± 10
Photo-Drive	3029.2	mV	250 mV to 4750 mV
Slope	1.017	-	1.0 ± 0.3
Offset	0.2	-	0 ± 0.3

Calibrated by :

Adul Dangklom
(Mr.Adul Dangklom)

Approved by :

Peera Detudom
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Calibration Report
Non-Dispersive Infrared CO Analyzer

Date : 06 May 2026

Brand : API

Model : 300E

No. CO-R03

Serial No. 1352

Calibrator (Dilution System)

Brand : API

Model : 700

Last Cal. Date : 01 September 2025

Serial No. : 911

Reference Standard Gas

Standard Gas : Carbon Monoxide (CO)

Cylinder No. : D711839

Certified Date : 14 March 2024

Expired Date : 14 March 2032

Cylinder Conc. : 4,580 ppm

Calibrating Condition

Pressure 1011

mmbar

Temp. 24.6 °C

% RH 50

Calibration Setting

Span Set Point	Initial Reading (Before Adj.), PPM			Final Reading (After Adj.), PPM
	Expected Concentration	Analyzer Response	%Dif	Analyzer Response
Zero	0	0.11	-	0
CO Span	40.00	40.07	0.175	40.00

API Model 300E CO Analyzer Check List

Parameter	Observed Value	Units	Nominal Range
Range	50	PPM	0-1000 ppm
Stability	0.10	PPM	< 1 ppm With Zero Air
CO Measure	4014.3	mV	2500-4800 mV
CO Reference	3946.8	mV	2500-4800 mV
Measure/Reference Ratio	1.180	-	1.1-1.3 W/Zero Air
Sample Pressure	28.6	In-Hg-A	~2" < Ambient Absolute Pressure
Sample Flow	808	CC/Min	800 ± 10%
Sample Temperature	48.2	°C	48 ± 4
Bench Temperature	48.0	°C	48 ± 2
Wheel Temperature	68.3	°C	68 ± 2
Box Temperature	30.9	°C	Ambient Temp + 7 ± 10
Photo-Drive	3027.3	mV	250 mV to 4750 mV
Slope	1.017	-	1.0 ± 0.3
Offset	0.2	-	0 ± 0.3

Calibrated by :


Adul Dangklom

(Mr. Adul Dangklom)

Approved by :

Peera Detudom

(Mr. Peera Detudom)



MIRACLE INTERNATIONAL TECHNOLOGY CO.,LTD

214 Bangwaek Rd. Bangpai Bangkoe Bangkok 10160
Tel.: 0-2865-4647-8 Fax: 0-2865-4649 <http://www.mit.in.th>



CALIBRATION CERTIFICATE

Page 1 of 3

Certificate No. : L202511307-0001

Date Issued : 01-Dec-25

Customer : S.P.S. CONSULTING SERVICE CO., LTD.
7 Soi Phaholyothin 24 Phaholyothin Road., Jompol, Chatuchak, Bangkok
10900

Equipment : Mass Flow meter

Manufacturer : Dwyer

Model : GMF-2101

Serial No. : -

ID No./Tag No. : MF01/51

Date Received : 27-Nov-25

Date Calibrated : 30-Nov-25

Calibrated by : Nattawat Laochai

Calibration Method or Calibration Procedure Used

In-house method : CP-34 by comparison against mass flow calibrator.

This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

Result of Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level confidence approximately 95 percent.

This certificate may not be reproduced other than in full except with the prior written approval of the Miracle International Technology Company Limited.

Approved by:

K. Nathong
(Nathapong Krudaum)



Certificate No. : L202511307-0001

Ambient Temperature : $(25 \pm 2)^{\circ}\text{C}$

Relative Humidity : $(50 \pm 15)\% \text{RH}$

Capacity Range : 17 ml/min

Calibration Media : Nitrogen


Type : Mass Flowmeter

Unit Under Calibration Reference Condition : Pressure 101.325 kPa(abs) , 21 $^{\circ}\text{C}$, Nitrogen

Temperature ($^{\circ}\text{C}$)	Pressure (kPa)	UUC Reading (ml/min)	STD Reading (ml/min)	Error (ml/min)	Uncertainty ($\pm$ ml/min)
24.69	101.22	0.00	0.000 *	0.000	0.063
24.44	119.03	3.30	3.358	-0.058	0.14
24.38	118.17	7.30	7.4	-0.10	0.15
24.30	156.08	13.50	13.6	-0.10	0.15
24.25	169.92	17.00	17.1	-0.10	0.18

Error = Unit Under Calibration - Standard

Marked * are not included in the NSC-ONSC accreditation schedule for our laboratory.

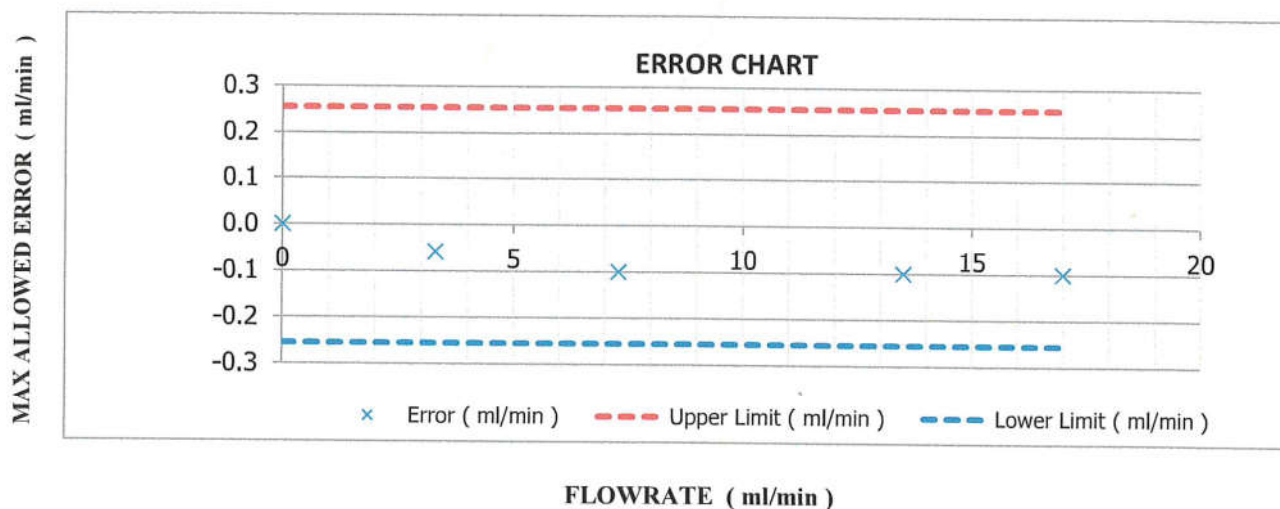

Certificate No. : L202511307-0001

Note : The actual flow rate is determined by the equation :

$$Q_{Meas} = Q_{Ref} \times \frac{P_{Ref}}{P_{Meas}} \times \frac{T_{Meas}}{T_{Ref}}$$

; Q = Flow rate

; P = Absolute pressure

; T = Absolute temperature

; Subscript "Meas" = Measurement condition

; Subscript "Ref" = Reference condition

Condition As-Received : Used Item

The measurement results and statements of conformity with specification only relate to the item calibrated.

Traceability of Certificate :

The International System of Units (SI) through

NIMT Calibration Certificate No. MW-0047-24 for Gas Flow meter Serial No. M5209179B/M5209179A, Due 28-Jun-26

NIMT Calibration Certificate No. MW-0048-24 for Gas Flow meter Serial No. M5209179C/M5209179A, Due 02-Jul-26

End of Certificate



CERTIFICATE No : 26M2266
REFERENCE No : 80204-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE
MANUFACTURER : METTLER TOLEDO
MODEL : XS105DU
SERIAL No : 1126422905
ID No : BA 05/50
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : SUCHAT S.

CALIBRATION DATE : 05-Mar-26

APPROVED BY :  PONGSAK J.

ISSUED DATE : 06-Mar-26

RECEIVED DATE : 05-Mar-26





CERTIFICATE No : 26M2266

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : XS105DU
MANUFACTURER : METTLER TOLEDO S/N : 1126422905
ID No : BA 05/50 RECEIVED DATE : 05-Mar-26
AIR PRESSURE : 1004mbar $\pm$ 1mbar CALIBRATION DATE : 05-Mar-26
AMBIENT TEMPERATURE : 25° C $\pm$ 1° C RELATIVE HUMIDITY : 50 %RH $\pm$ 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	C02250116	28-Jan-27
2) STANDARD WEIGHT	E2	15843	C02250117	29-Jan-27

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 120 g WAS 0.000055 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ($\pm$ g)
0.00	0.00000	0.00000	0.000065
0.02	0.02000	0.00000	0.000065
0.10	0.10000	0.00000	0.000066
0.20	0.20000	0.00000	0.000066
0.50	0.50001	-0.00001	0.000065
1.00	1.00001	-0.00001	0.000066
2.00	2.00000	0.00000	0.000067
5.00	5.00001	-0.00001	0.000068
10.00	10.00004	-0.00004	0.000070
20.00	20.00006	-0.00006	0.000078
50.00	50.00000	0.00000	0.00012
100.00	100.0002	-0.0002	0.00019
120.00	120.0002	-0.0002	0.00022

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.0000
2	50.0000
3	50.0000
4	50.0000
5	50.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN
associates



Cert. No. : SP25026

Pages : 1 of 4

Calibration Certificate

Equipment : UV-VIS SPECTROPHOTOMETER
Manufacturer : PERKINELMER
Model : LAMBDA 25
Serial No.: 501S14123010
ID No.: SP03/58
Calibration Mode : WAVELENGTH ACCURACY
PHOTOMETRIC ACCURACY
STRAY LIGHT

Condition As Found : GOOD

Customer : S.P.S CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN ROAD,
CHOMPHON SUB-DISTRICT, CHATUCHAK DISTRICT,
BANGKOK PROVINCE 10900 THAILAND.

Location : ORGANIC LABORATORY IV

Ambient Temperature : (22.9 $\pm$ 5) °C
Relative Humidity : (53.7 $\pm$ 25) %

Received Date : 22 AUGUST 2025
Calibration Date : 22 AUGUST 2025
Date of Issue : 25 AUGUST 2025

Calibrated by :

Nitinun Srihawan

Approved by :

Wichok B.
(Wichok Ekpongpradit)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : SP25026

Job No. : VC68SP0019

Pages : 2 of 4

Calibration Method :

This instrument was calibrated by using on-site calibration procedure In-house method : CP-SP-01

The calibration procedure to direct measurement wavelength accuracy by using wavelength standard solution, Photometric accuracy by using absorbance standard filter and absorbance standard solution

The calibration procedure used was based on ASTM E275-01, ASTM E925-02

Condition of this result of calibration :

1. Certified reference materials

<u>Material</u>	<u>Ref. type</u>	<u>Cell serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Holmium liquid	RM-HL	29706	126461	24/10/2026
Didymium liquid	RM-DL	28912	126462	24/10/2026
Neutral density filter	RM-1N2N3N	13877	126457	24/10/2026
Potassium dichromate solutions	RM-0204060810	14204	126497	25/10/2026
Potassium Iodide solution	-	KI-0701-001	CI-0185-24	14/05/2026

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 The UK National Physical Laboratory (NPL)

Result of calibration : Wavelength Accuracy

(Without adjustment)

Material	Certified Values of Reference Material (nm)	UUC* Reading (nm)	Error (nm)	Uncertainty ± (nm)	k Factor
RM-HL	278.13	278.21	0.08	0.16	2.00
	361.25	361.39	0.14	0.16	2.00
	467.82	467.71	-0.11	0.16	2.00
	536.56	536.50	-0.06	0.16	2.00
	640.50	640.36	-0.14	0.16	2.00
RM-DL	740.09	739.85	-0.24	0.16	2.00
	864.94	865.12	0.18	0.16	2.00

UUC* = Unit Under Calibration

Cert. No. : SP25026
Job No. : VC68SP0019
Pages : 3 of 4

Result of calibration : Photometric Accuracy

Material	Wavelength (nm)	Filter S/N	Nominal Absorbance (A)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor
Neutral Density glass filter	440.0	29381	0.5	0.5443	0.5413	-0.0030	0.0043	2.00
		29914	0.7	0.7484	0.7455	-0.0029	0.0054	2.00
		29360	1.0	1.0527	1.0535	0.0008	0.0032	2.00
	465.0	29381	0.5	0.4948	0.4922	-0.0026	0.0041	2.00
		29914	0.7	0.6906	0.6877	-0.0029	0.0050	2.00
		29360	1.0	0.9695	0.9709	0.0014	0.0031	2.00
	546.1	29381	0.5	0.5090	0.5068	-0.0022	0.0036	2.00
		29914	0.7	0.6985	0.6960	-0.0025	0.0041	2.00
		29360	1.0	0.9814	0.9825	0.0011	0.0031	2.00
	590.0	29381	0.5	0.5375	0.5353	-0.0022	0.0034	2.00
		29914	0.7	0.7256	0.7231	-0.0025	0.0037	2.00
		29360	1.0	1.0213	1.0219	0.0006	0.0032	2.00
	635.0	29381	0.5	0.5223	0.5202	-0.0021	0.0033	2.00
		29914	0.7	0.6927	0.6901	-0.0026	0.0036	2.00
		29360	1.0	0.9744	0.9750	0.0006	0.0032	2.00

UUC* = Unit Under Calibration

Cert. No. : SP25026

Job No. : VC68SP0019

Pages : 4 of 4

Result of calibration : Photometric Accuracy

(Without adjustment)

Material	Wavelength (nm)	Solution (mg/l)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor
Potassium dichromate solutions	235.0	20	0.2415	0.2443	0.0028	0.0101	2.00
		40	0.4866	0.4871	0.0005	0.0115	2.00
		60	0.7415	0.7295	-0.0120	0.0067	2.00
		80	0.9854	0.9844	-0.0010	0.0071	2.00
		100	1.2444	1.2425	-0.0019	0.0073	2.00

UUC* = Unit Under Calibration

Condition of this result of calibration : Spectrophotometer PERKINELMER Model LAMBDA 25 S/N 501S14123010

Resolution of Wavelength Mode 0.1 nm

Resolution of Photometric Mode 0.001 A

Parameter Setting

Measurement Mode Wavelength, Absorbance

Wavelength Scan 190 nm - 1100 nm

Scanning Speed 7.5 nm/min

Band width(Wavelength) 1.0

Band width(Vis) 1.0

Band width(Uv) 1.0

Stray Light** UUC* Reading at 220.0 nm	
Transimission T(%)	Absorbance(A)
0.020	3.7032

**Specific Acceptance :

Transmission ≤ 1.0 T(%), Absorbance ≥ 2.0 A

**Stray light not TISI Accredited

The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95%

End of Calibration Certificate



บริษัท ไทยยูนิค จำกัด

THAI UNIQUE CO., LTD.

80-82 ถนนประชาธิปไตย แขวงบางขุนพรหม เขตพระนคร กรุงเทพฯ 10200

80-82 Prachathipatai Rd., Bangkhunphrom, Pranakorn, Bangkok 10200

Tel. 0-2629-0191-6, 0-2280-1787, Fax. 0-2280-1788, E-mail : thawatt@thaiunique.com, Website : www.thaiunique.com

GAS CHROMATOGRAPH TEST CERTIFICATION

Certificate No. : SV0825/23032

Instrument Type : Gas Chromatography

Model : 3800

Serial Number : 00734

Organization : S.P.S. Consulting Service Co., Ltd.

Address : 7 Phahonyothin Soi 24 Phahonyothin Rd. Ladyao Chatuchak Bangkok 10900

Date : 02/08/2025

ELECTRONIC TEST

CPU	☒ PASS	☐ FAIL
DISPLAY & LED TEST	☒ PASS	☐ FAIL
VENT TEST	☒ PASS	☐ FAIL
KEY ECHO TEST	☒ PASS	☐ FAIL
DESTRUCTION RAM TEST	☒ PASS	☐ FAIL

RUN CHROMATOGRAM TEST

DETECTOR : Flame Ionization Detectors (FID Channel-Front)

INJECTOR : 1079 Injector

GC CONDITION:

Column	80 °C hold 1 min., rate 20 °C/min. to 200 °C hold 1min.
Injector	220 °C
Detector	300 °C
Column flow	5 mL/min
Makeup flow	25 mL/min
Air flow	300 mL/min
Hydrogen flow	30 mL/min

Column:Capillary Column CP sil 5 CB 0.25 ID x 15 M

Sample: 1 µL Injection FID Test Sample 0.218g/L C14,C15,C16 in hexane (diluted to 30ppm)

SENSITIVITY TEST: C15. (Area count) = 515,940 Counts.



VARIAN



บริษัท ไทยยูนิค จำกัด

THAI UNIQUE CO., LTD.

80-82 ถนนประชาธิปไตย แขวงบางขุนพรหม เขตพระนคร กรุงเทพฯ 10200

80-82 Prachathipatai Rd., Bangkhunphrom, Pranakorn, Bangkok 10200

Tel: 0-2629-0191-6, 0-2280-1787, Fax: 0-2280-1788, E-mail : thawatt@thaiunique.com, Website : www.thaiunique.com

Detector Sensitivity (FID)

Detector Response	Result	Specification
Baseline Noise (μ V)	2.40	≤ 50
Baseline Drift (%)	0.18	≤ 1
Sensitivity (S/N for C15)	19,716	$\geq 1,024$

Temperature Specification

Temperature	Set	Result	Specification
Column Oven ($^{\circ}$ C)	80	79	± 5
Injector ($^{\circ}$ C)	220	218	± 5
Detector ($^{\circ}$ C)	300	298	± 5
Incubator ($^{\circ}$ C)	60	N/A	± 5

Relative Standard Deviation % (%RSD)

Checkout Procedure	Result	Specification
Area C15 (%)	1.48	≤ 5
Retention Time C15 (%)	0.08	≤ 0.5

APPROVAL :

Signature:

Engineer : Somchai Pohtongkam

Date : 02/08/2025



VARIAN



บริษัท ไทยยูนิค จำกัด

THAI UNIQUE CO., LTD.

80-82 ถนนประชาธิปไตย แขวงบางขุนพรหม เขตพระนคร กรุงเทพฯ 10200

80-82 Prachathipatai Rd., Bangkhunphrom, Pranakorn, Bangkok 10200

Tel. 0-2629-0191-6, 0-2280-1787, Fax. 0-2280-1788, E-mail : thawatt@thaiunique.com, Website : www.thaiunique.com

Results Integrated System Testing

Checkout Procedure	FID
Detector Position	Front
Inlet Type	1079 Injector
C15 Area 1	506,043
C15 Area 2	520,497
C15 Area 3	522,154
C15 Area 4	521,664
C15 Area 5	509,340
C15 Area Average	515,940
* % RSD (< 5 %)	1.48

* The precision specification should be less than 2.0 % RSD ** (Relative Standard Deviation) for an Auto sampler injection and less than 5 % for Manual injections. To calculate the %RSD, select the C15 peak area for each of the five (5) samples.

** (Relative Standard Deviation is determined by dividing the standard deviation by the average and multiplying by 100.)

$$\% \text{ RSD} = (\text{std.dev} / \text{avg}) * 100$$

Compliance	☒ Pass	☐ Fail
Performance by	<i>Sachin P.</i>	
Date	02/08/2025	



Comments			
Reviewed by	<i>Wattana</i>	Date	02/08/2025



VARIAN



บริษัท ไทยยูนิค จำกัด

THAI UNIQUE CO., LTD.

80-82 ถนนประชาธิปไตย แขวงบางขุนพรหม เขตพระนคร กรุงเทพฯ 10200

80-82 Prachathipatai Rd., Bangkhunphrom, Pranakorn, Bangkok 10200

Tel. 0-2629-0191-6, 0-2280-1787, Fax. 0-2280-1788, E-mail : thawatt@thaiunique.com, Website : www.thaiunique.com

Results Integrated System Testing

Checkout Procedure	FID
Detector Position	Front
Inlet Type	1079 Injector
C15 RT 1	3.874
C15 RT 2	3.880
C15 RT 3	3.875
C15 RT 4	3.872
C15 RT 5	3.878
C15 RT Average	3.876
* % RSD (< 0.5 %)	0.08

* The precision specification should be less than 0.5 % RSD ** (Relative Standard Deviation) for an Auto sampler injection and less than 0.5 % for Manual injections. To calculate the %RSD, select the RT C15 peak for each of the five (5) samples.

** (Relative Standard Deviation is determined by dividing the standard deviation by the average and multiplying by 100.)

$$\% \text{ RSD} = (\text{std.dev} / \text{avg}) * 100$$

Compliance	☒ Pass	☐ Fail
Performance by	<i>Somchai P.</i>	
Date	02/08/2025	



Comments			
Reviewed by	<i>Wattana</i>	Date	02/08/2025



VARIAN


Title :
Run File : e:\sps2025\blk001.run
Method File : c:\star\data\tu\2025\cal fid.mth
Sample ID : blk

Injection Date: 2/8/2568 12:01 Calculation Date: 2/8/2568 12:33

Operator : watsamon Detector Type: 3800 (10 Volts)
Workstation: GC-LAB Bus Address : 44
Instrument : Sample Rate : 10.00 Hz
Channel : Front = FID Run Time : 20.005 min

** LC Workstation Version 6.20 ** 02511-7390-ae7-0265 **

Chart Speed = 1.13 cm/min Attenuation = 1 Zero Offset = 50%
Start Time = 0.000 min End Time = 20.005 min Min / Tick = 1.00

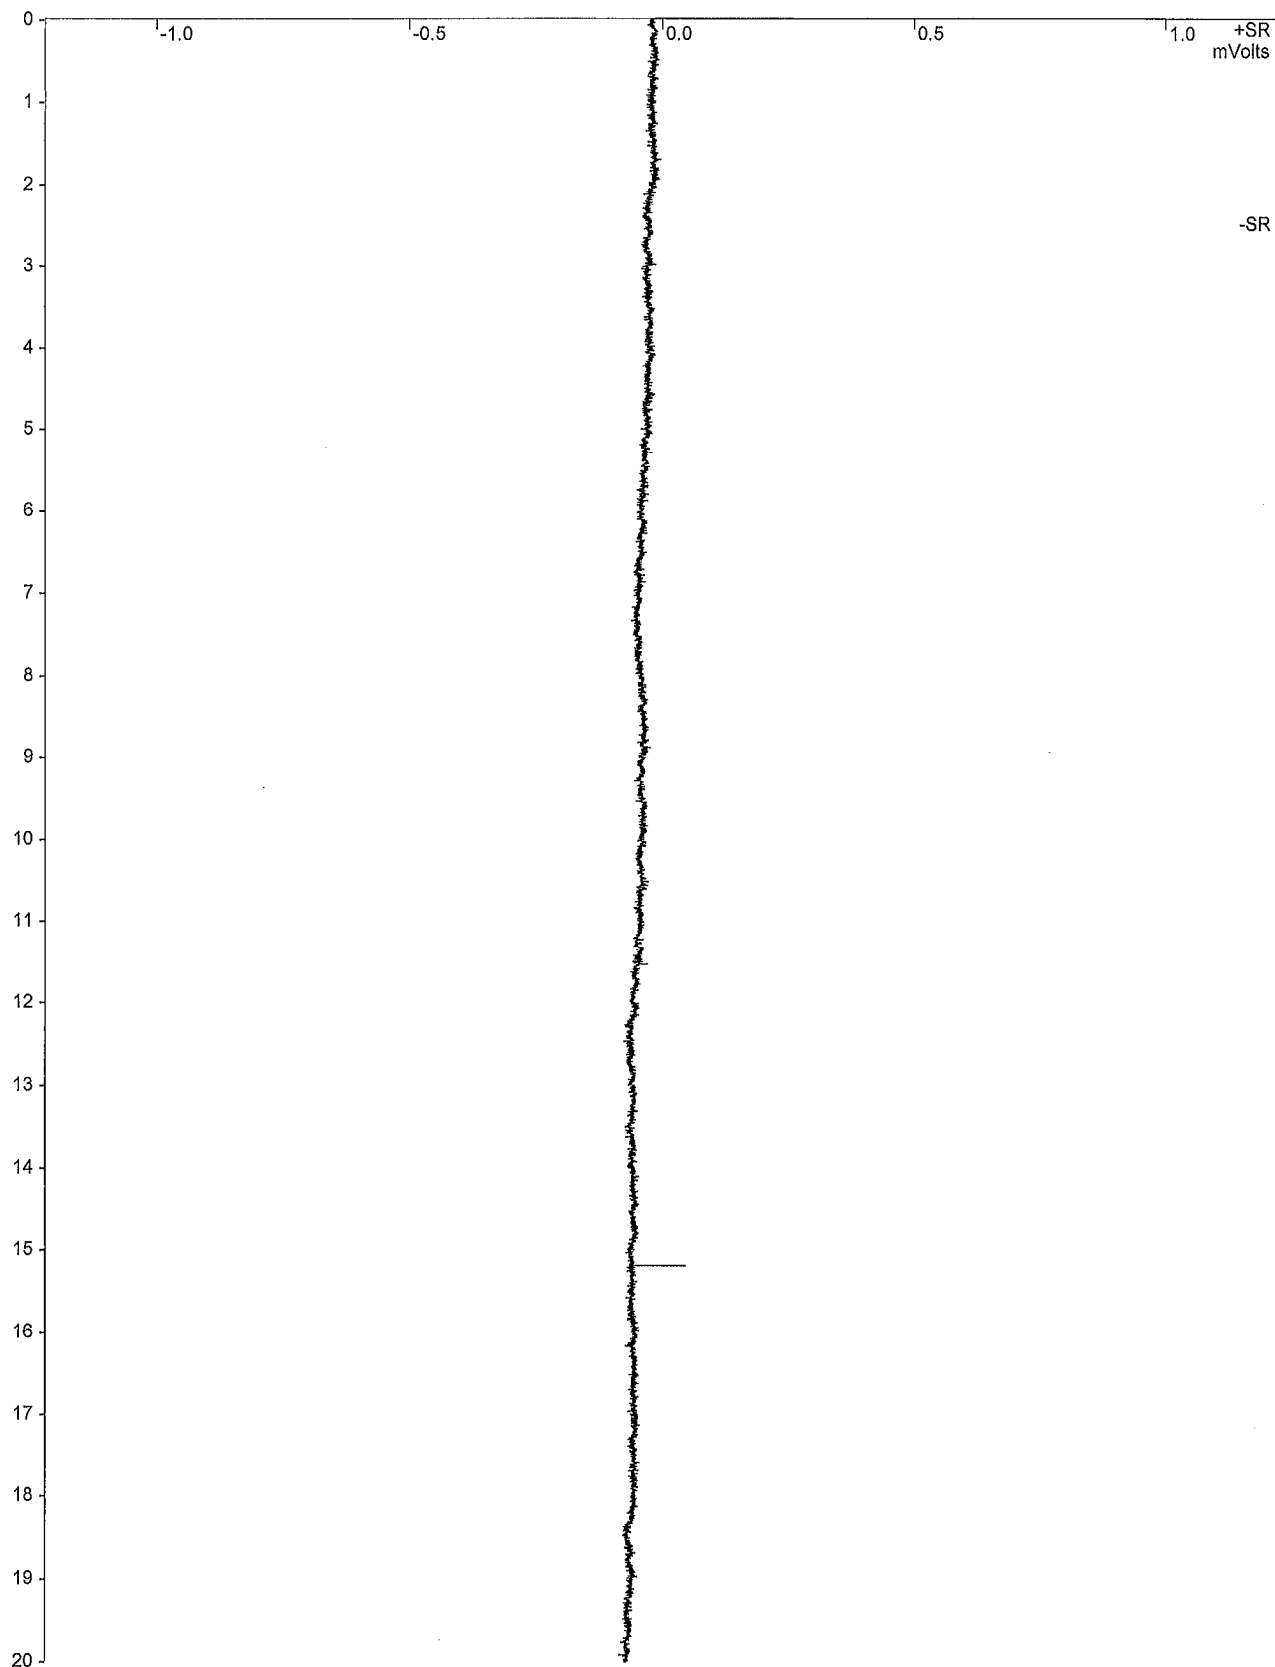

Title :
Run File : e:\sps2025\blk001.run
Method File : c:\star\data\tu\2025\cal fid.mth
Sample ID : blk

Injection Date: 2/8/2568 12:01 Calculation Date: 2/8/2568 12:33

Operator : watsamon Detector Type: 3800 (10 Volts)
Workstation: GC-LAB Bus Address : 44
Instrument : Sample Rate : 10.00 Hz
Channel : Front = FID Run Time : 20.005 min

** LC Workstation Version 6.20 ** 02511-7390-ae7-0265 **

Run Mode : Analysis
Peak Measurement: Peak Area
Calculation Type: External Standard

Peak No.	Peak Name	Result ()	Ret. Time (min)	Time Offset (min)	Area (counts)	Sep. Code	Width 1/2 (sec)	Status Codes
----	-----	-----	-----	-----	-----	----	-----	-----
----	-----	=====	-----	=====	=====	----	-----	-----
	Totals:	0.0000		0.000	0			

Total Unidentified Counts : 0 counts

Detected Peaks: 0 Rejected Peaks: 0 Identified Peaks: 0

Multiplier: 1 Divisor: 1 Unidentified Peak Factor: 0

Baseline Offset: -14 microVolts LSB: 1 microVolts

Noise (used): 24 microVolts - monitored before this run

Manual injection

Data Handling: No peaks


Title :
Run File : e:\sps2025\fidstd001.run
Method File : c:\star\data\tu\2025\cal fid.mth
Sample ID : fidstd

Injection Date: 2/8/2568 12:34 Calculation Date: 2/8/2568 13:26

Operator : watsamon Detector Type: 3800 (10 Volts)
Workstation: GC-LAB Bus Address : 44
Instrument : Sample Rate : 10.00 Hz
Channel : Front = FID Run Time : 7.993 min

** LC Workstation Version 6.20 ** 02511-7390-ae7-0265 **

Chart Speed = 2.83 cm/min Attenuation = 79 Zero Offset = 2%
Start Time = 0.000 min End Time = 7.993 min Min / Tick = 1.00

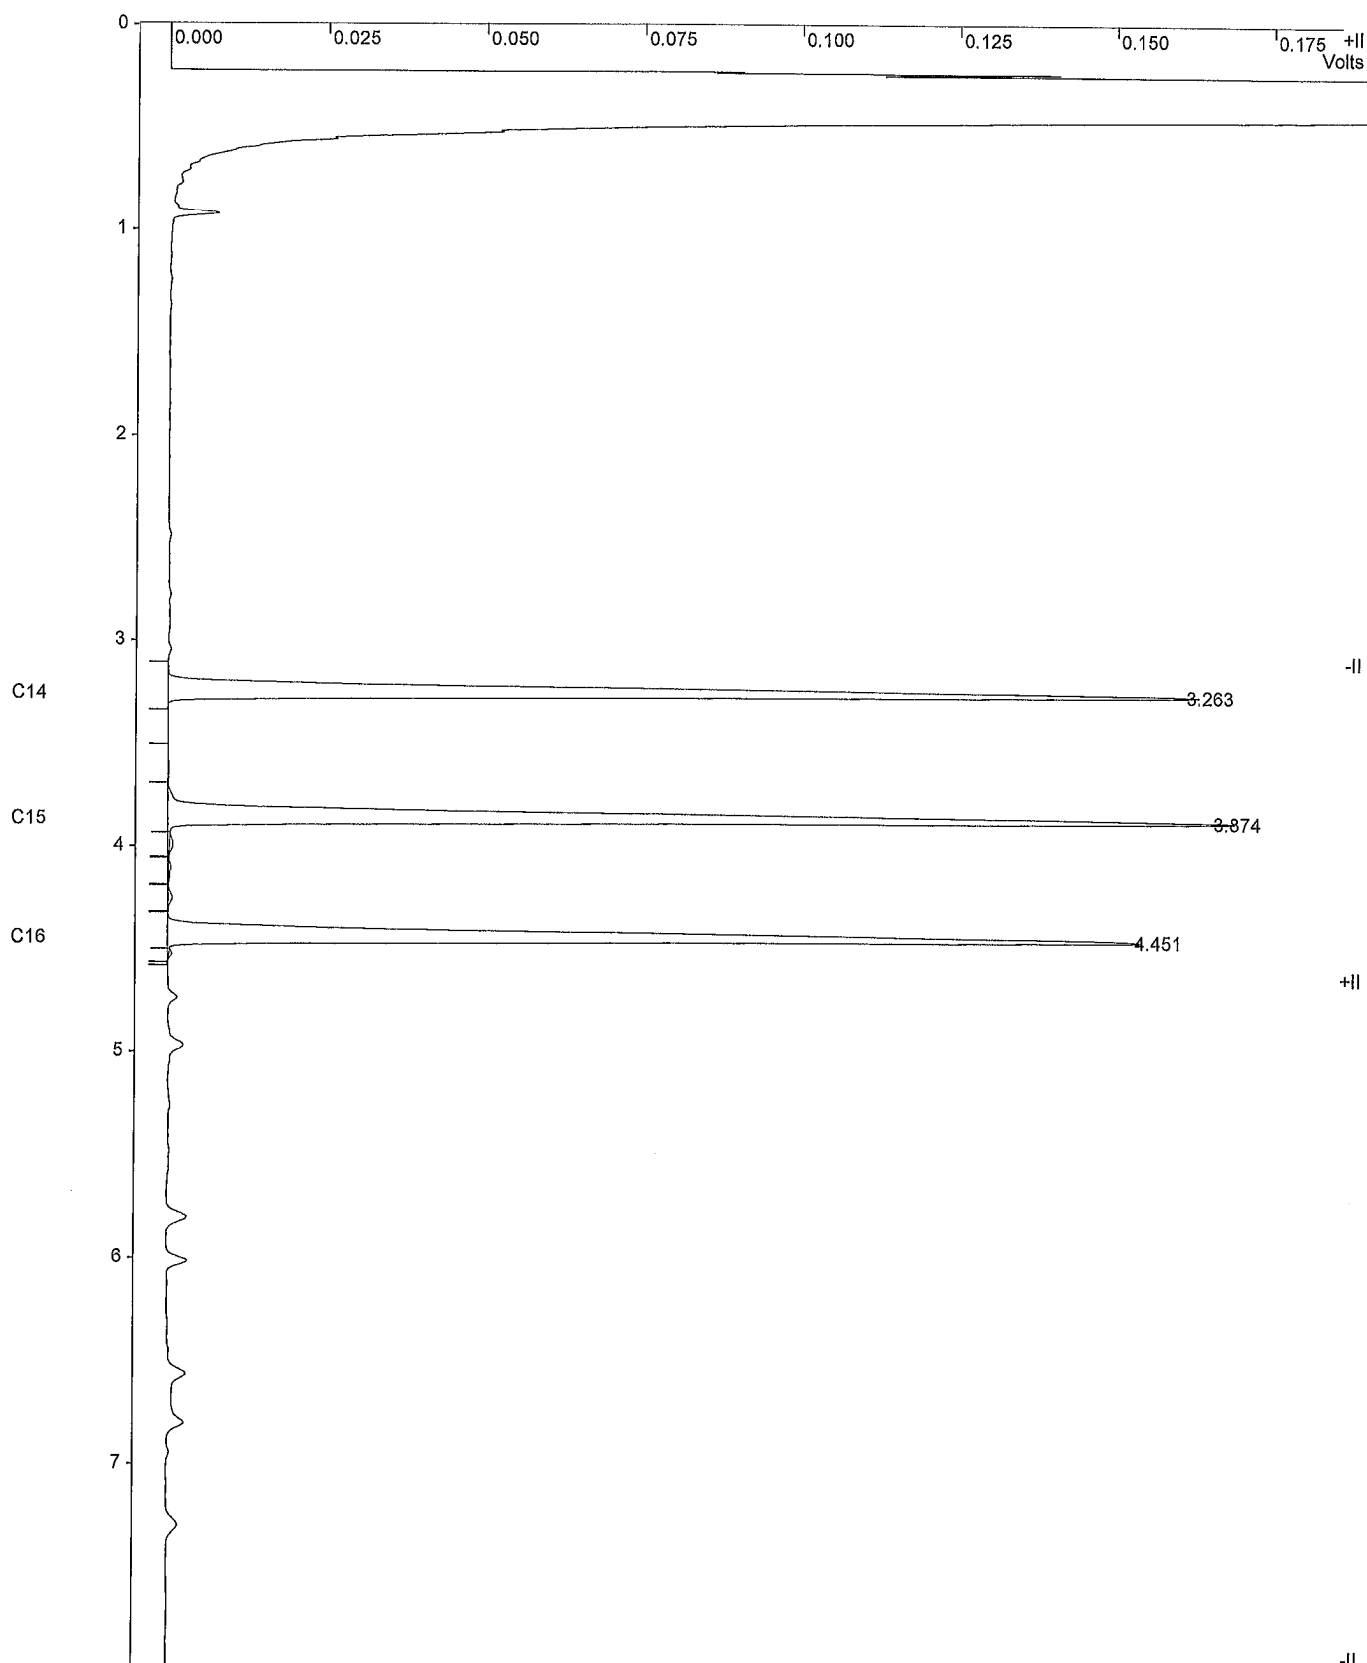

Title :
Run File : e:\sps2025\fidstd001.run
Method File : c:\star\data\tu\2025\cal fid.mth
Sample ID : fidstd

Injection Date: 2/8/2568 12:34 Calculation Date: 2/8/2568 13:26

Operator : watsamon Detector Type: 3800 (10 Volts)
Workstation: GC-LAB Bus Address : 44
Instrument : Sample Rate : 10.00 Hz
Channel : Front = FID Run Time : 7.993 min

** LC Workstation Version 6.20 ** 02511-7390-ae7-0265 **

Run Mode : Calibration
Peak Measurement: Peak Area
Calculation Type: External Standard
Level : 1

Peak No.	Peak Name	Ret. Time (min)	Time Offset (min)	Area (counts)	Sep. Code	Width 1/2 (sec)	Status Codes
1	C14	3.263	0.002	458627	BB	2.7	
2	C15	3.874	0.002	506043	VV	2.8	
3	C16	4.451	0.001	460610	VB	2.8	
Totals:			0.005	1425280			

Total Unidentified Counts : 0 counts

Detected Peaks: 8 Rejected Peaks: 5 Identified Peaks: 3

Multiplier: N/A Divisor: N/A Unidentified Peak Factor: 0

Baseline Offset: 6 microVolts LSB: 1 microVolts

Noise (used): 2 microVolts - monitored before this run

Manual injection

Sample ID: **fid std**



Operator (Inj): **watsamon**

Injection Date: **02/08/2025**

Calc Date: **02/08/2025**

Run Time (min): **7.993**

Workstation: **GC-LAB**

Instrument (Inj):

VARIAN


Run Mode: **Calibration**

Peak Measurement: **Peak Area**

Calculation Type: **External Std.**

e:\sps2025\fidstd001.run

A = FID 10 V RESULTS

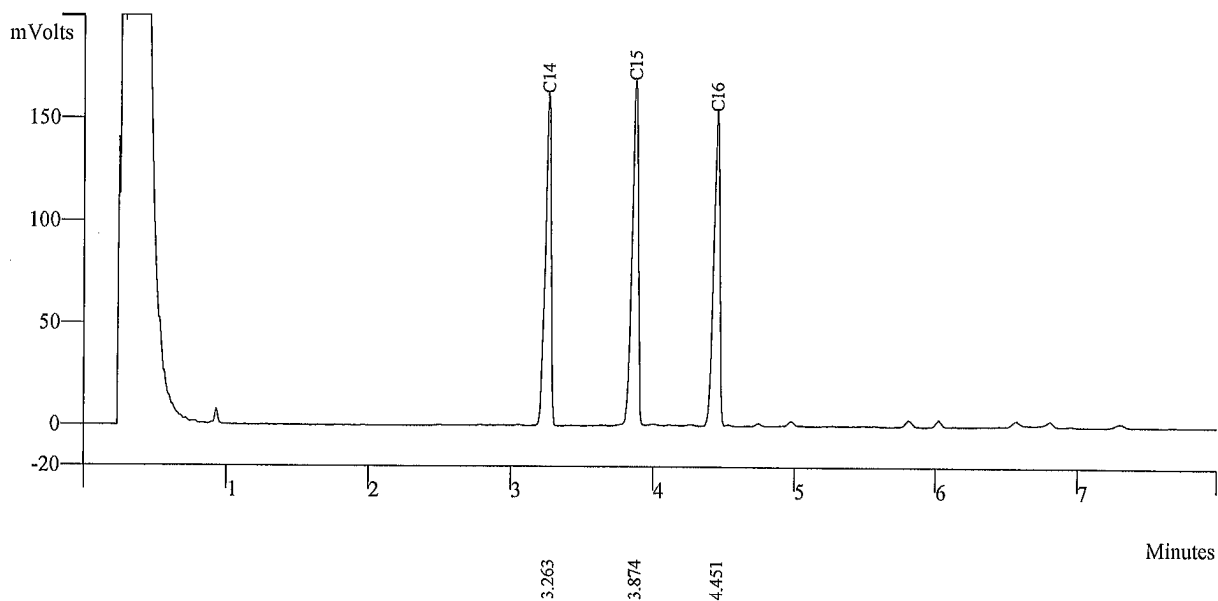

Peak No	Peak Name	Result ()	Ret Time (min)	Peak Area (counts)	Sep. Code	Width 1/2 (sec)
1	C14	0.0000	3.263	458627	BB	2.7
2	C15	0.0000	3.874	506043	VV	2.8
3	C16	0.0000	4.451	460610	VB	2.8
	Totals	0.0000		1425280		



Sample ID: fid std




VARIAN

Operator (Inj): watsamon
Injection Date: 02/08/2025
Calc Date: 02/08/2025
Run Time (min): 7.993
Workstation: GC-LAB
Instrument (Inj):

Run Mode: Calibration
Peak Measurement: Peak Area
Calculation Type: External Std.

e:\sps2025\fidstd002.run

A = FID 10 V RESULTS

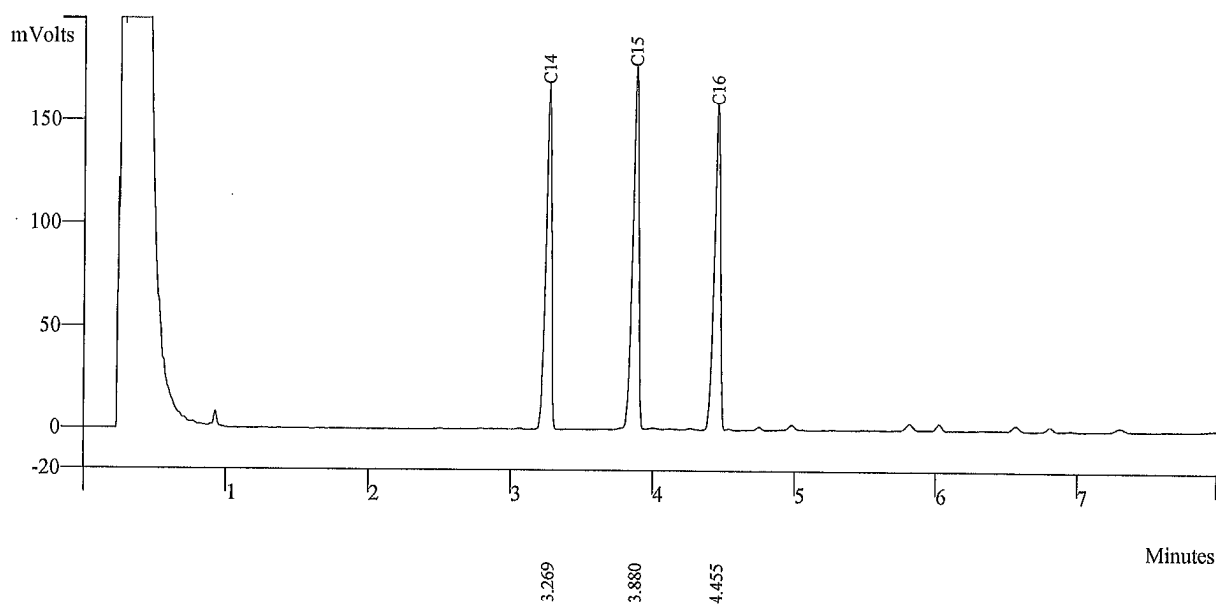

Peak No	Peak Name	Result ()	Ret Time (min)	Peak Area (counts)	Sep. Code	Width 1/2 (sec)
1	C14	0.0000	3.269	472338	BB	2.6
2	C15	0.0000	3.880	520497	VV	2.7
3	C16	0.0000	4.455	471916	VB	2.8
	Totals	0.0000		1464751		



Sample ID: **fid std**



Operator (Inj): **watsamon**

Injection Date: **02/08/2025**

Calc Date: **02/08/2025**

Run Time (min): **7.993**

Workstation: **GC-LAB**

Instrument (Inj):

VARIAN


Run Mode: **Calibration**

Peak Measurement: **Peak Area**

Calculation Type: **External Std.**

e:\sps2025\fidstd003.run

A = FID 10 V RESULTS

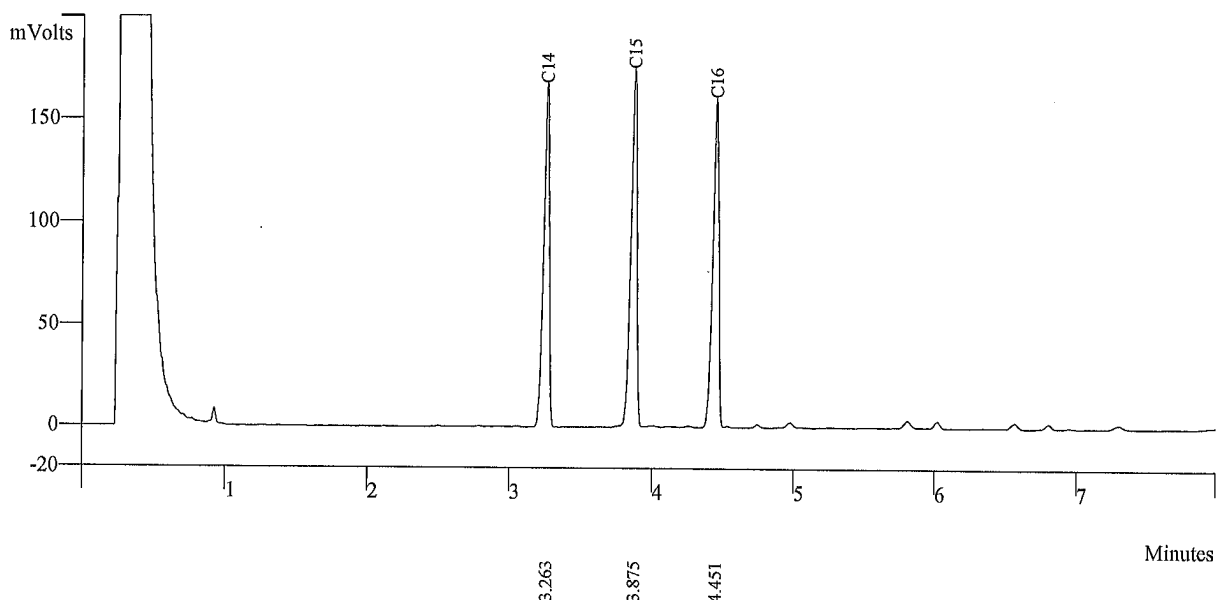

Peak No	Peak Name	Result ()	Ret Time (min)	Peak Area (counts)	Sep. Code	Width 1/2 (sec)
1	C14	0.0000	3.263	469265	BB	2.6
2	C15	0.0000	3.875	522154	VV	2.8
3	C16	0.0000	4.451	478526	VB	2.8
	Totals	0.0000		1469945		



Sample ID: fid std



VARIAN

Operator (Inj): watsamon

Injection Date: 02/08/2025

Calc Date: 02/08/2025

Run Time (min): 7.993

Workstation: GC-LAB

Instrument (Inj):


Run Mode: Calibration

Peak Measurement: Peak Area

Calculation Type: External Std.

e:\sps2025\fidstd004.run

A = FID 10 V RESULTS

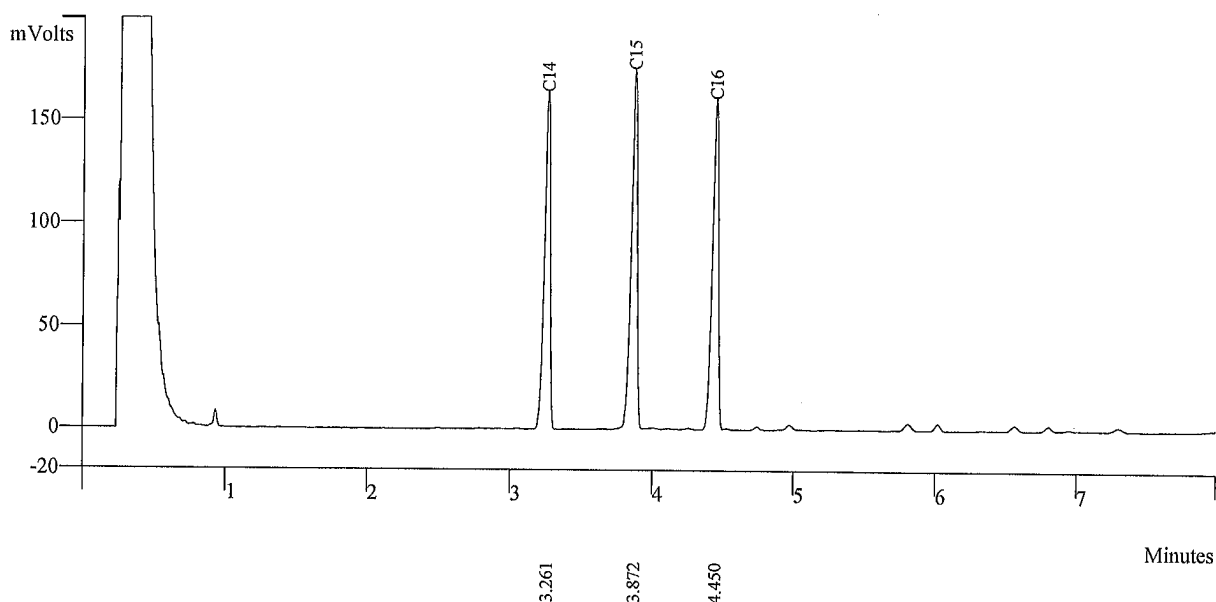

Peak No	Peak Name	Result ()	Ret Time (min)	Peak Area (counts)	Sep. Code	Width 1/2 (sec)
1	C14	0.0000	3.261	468907	BB	2.7
2	C15	0.0000	3.872	521664	VV	2.8
3	C16	0.0000	4.450	478772	VB	2.8
	Totals	0.0000		1469343		



Sample ID: **fid std**



VARIAN

Operator (Inj): watsamon

Injection Date: 02/08/2025

Calc Date: 02/08/2025

Run Time (min): 7.993

Workstation: GC-LAB

Instrument (Inj):


Run Mode: Calibration

Peak Measurement: Peak Area

Calculation Type: External Std.

e:\sps2025\fidstd005.run

A = FID 10 V RESULTS

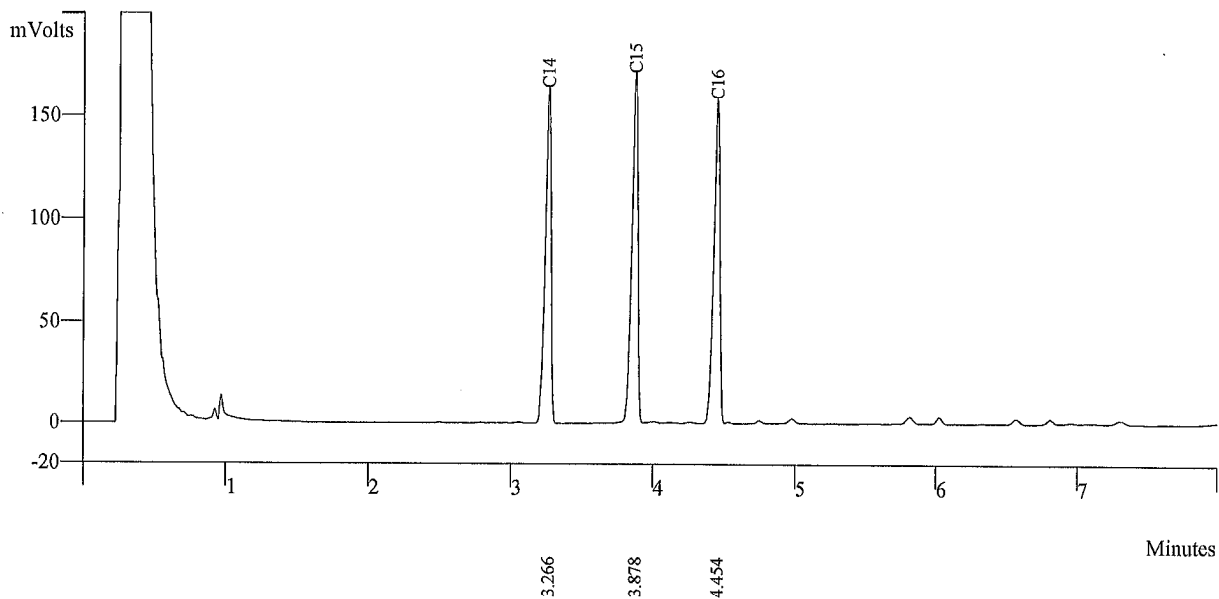


Peak No	Peak Name	Result ()	Ret Time (min)	Peak Area (counts)	Sep. Code	Width 1/2 (sec)
1	C14	0.0000	3.266	459351	BB	2.6
2	C15	0.0000	3.878	509340	VV	2.8
3	C16	0.0000	4.454	468353	VB	2.8
	Totals	0.0000		1437044		



C14

External Standard Analysis
Curve Type: Linear
Origin: Force
 $y = +1.552325e+004x$


Resp. Fact. RSD: 1.347%
Coeff. Det.(r²): 0.999130

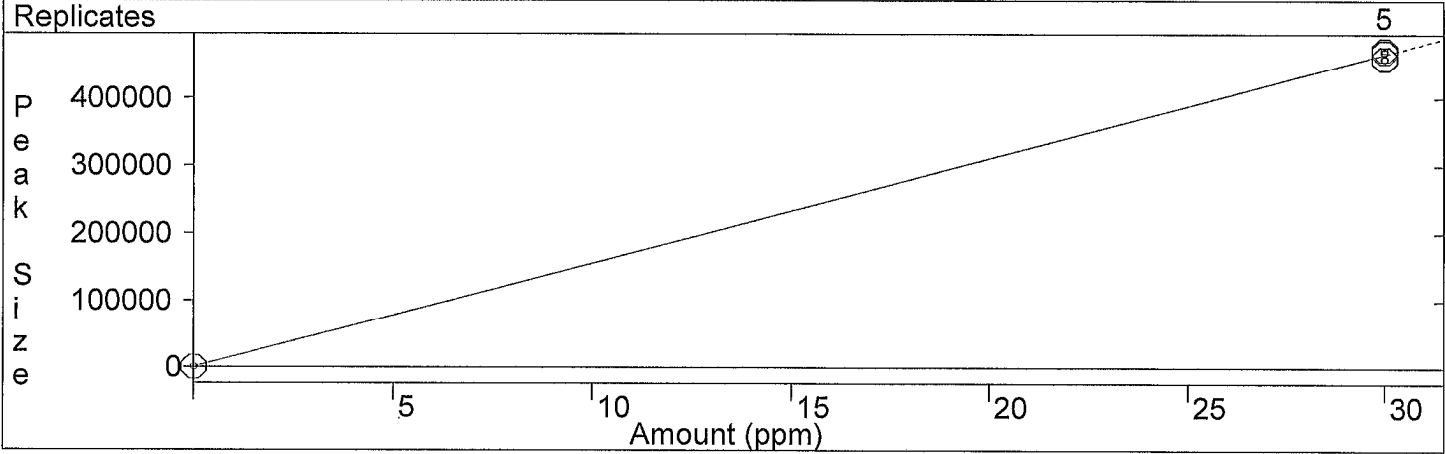

C15

External Standard Analysis
Curve Type: Linear
Origin: Force
 $y = +1.719798e+004x$


Resp. Fact. RSD: 1.481%
Coeff. Det.(r²): 0.998948

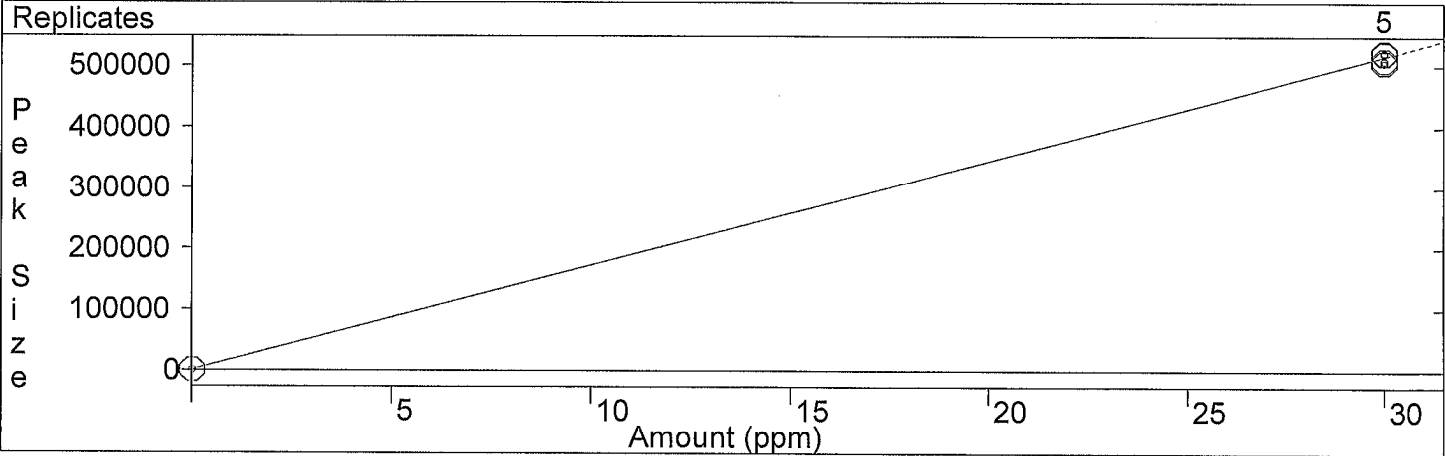

C16

External Standard Analysis
Curve Type: Linear
Origin: Force
 $y = +1.572118e+004x$

Resp. Fact. RSD: 1.611%
Coeff. Det.(r²): 0.998756

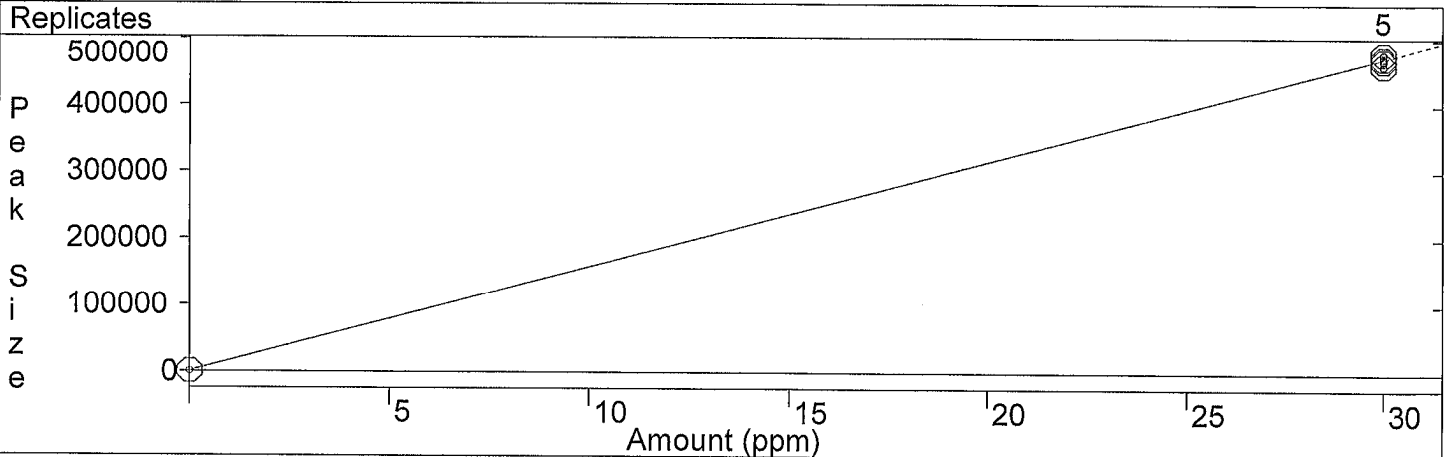

CERTIFICATE

This is to certify, that

Somchai Pohthongkham

has participated the course


Basic GC and Sampler training

Date: ***24 – 27 May 2004***

Location: ***Middelburg***

Instructor: ***W.J. Buys***

Signature instructor:

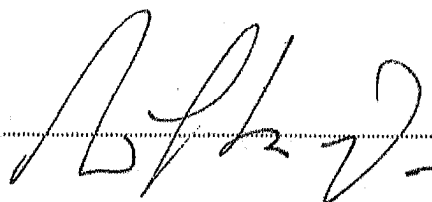

VARIAN

Varian Analytical Instruments
Varian Chrompack International BV
Herculesweg 8
P.O. Box 8033
4330 EA Middelburg
The Netherlands

Tel.: +31 118 671000
Fax: +31 118 633118

www.varianinc.com



WK Electric Co., Ltd.



68/242 Moo 5, Sawaipracharaj Rd., Tumbol Ladsawai, Amphur Lamlukka, Pathumthani 12150

Tel. +66 2993 4773, +66 2153 7132-3 Fax. +66 2994 5509 E-mail : wk.calibrations@gmail.com www.wk-etc.com

Certificate of Calibration

Certificate No.: WK2412-053-1

Page 1 of 2

Customer : THAI UNIQUE CO., LTD.
80-82 Prachathipatai Rd., Bangkhunphrom,
Pranakorn, Bangkok 10200

Instrument	: AMD Flow Meter	Ambient Temperature	: (23 ± 2) °C
Manufacturer	: Agilent Technologies	Humidity	: (50 ± 15) %RH
Model	: G6691A	Received Date	: 4-Dec-24
Serial No.	: MY16470347	Calibrated Date	: 11-Dec-24
Identity No.	: SV-DF-001	Issued Date	: 13-Dec-24
Range	: 0 ml/min to 750 ml/min	Calibrated Location	: In Lab
Resolution	: See to Data		
Calibration Method	: CP-WK-M10		

Reference standard instruments :

Instrument	Serial No.	Certificate No.	Due Date	Traceability to
Flow Calibrator	140215-134	L202304114-001	18-Apr-25	MIT
Primary Flow Calibrator	1107-S	WK2405-049-5	22-May-25	WK Electric Co., Ltd.

MIT : Miracle International Technology Co., Ltd.

This result calibrate was found accurate as shown on date place of calibrate only

This certificate is traceability to the International System of Unit (SI)

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence approximately 95%

Calibrated by : Mr.Thippatai Mungpungklang

Approved by :

Ms. Budsagorn Patcha

Authorized Signatory

This certificate may not be reproduced except in full unless permission for the reproduction has been obtained in writing from the laboratory.



Measuretronix Limited
2425/2 Lat Phrao Road, Saphan Song
Wangthonglang, Bangkok 10310, Thailand
Phone : 0-2514-1000, 0-2514-1234
Fax : 0-2514-0001, 0-2514-0003
Website : www.measuretronix.com



Certificate of Calibration

Certificate Number : LF25-0305
Equipment : Thermometer
Manufacturer : Fluke
Model : 51
Serial Number : 5910857
Asset Number : 5910857
Customer : Thai Unique Co., Ltd.
80-82 Prachathipatai Road,
Bangkhunphrom, Pranakorn,
Bangkok 10200
Date of Calibrate : 6-Jun-2025
Date of Issue : 6-Jun-2025

This calibration certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI).

This calibration certificate applies only to the item identified and shall not be reproduced other than in full, without specific written approved by Measuretronix Cal-Lab. Calibration certificates without signature are not valid.

The measurements marked with an asterisk () in this certificate are outside our range of accreditation. They have been included for completeness.*

The Calibration interval (Cal.Due) is the responsibility of the end user.

Calibrated by

Mr. Samak Uaonkaonoi
Metrology Technician

Approved by

Miss Juthamas Sukhathainirun
Cal-Lab Manager



Agilent Technologies

Certificate of Analysis

FID-TCD Performance Evaluation Sample Kit

Agilent Part
Number: 5080-8842, 18710-60170

Sample Lot
Number: 0006750304

This analytical reference material was manufactured and verified in accordance with an ISO 9001 registered quality system, and the analyte concentrations were verified by an ISO 17025 accredited laboratory. The certified value for each analyte was determined gravimetrically.

Concentrations:

n-tetradecane	0.218 g/L ($\pm 0.5\%$)	0.033 w/w %
n-pentadecane	0.218 g/L ($\pm 0.5\%$)	0.033 w/w %
n-hexadecane	0.218 g/L ($\pm 0.5\%$)	0.033 w/w %

Solvent: hexane


Calibrated Class A glassware and clean bottles were used in the manufacture of this standard. Balances used in the manufacture of this standard are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z-540-1 and ISO 9001.

Purities:

n-tetradecane	99.6%
n-pentadecane	99%
n-hexadecane	99.5%
hexane	99%

Typical Analytical Spectrum or Chromatography

GC Chromatography – n-tetradecane, n-pentadecane, and n-hexadecane in hexane

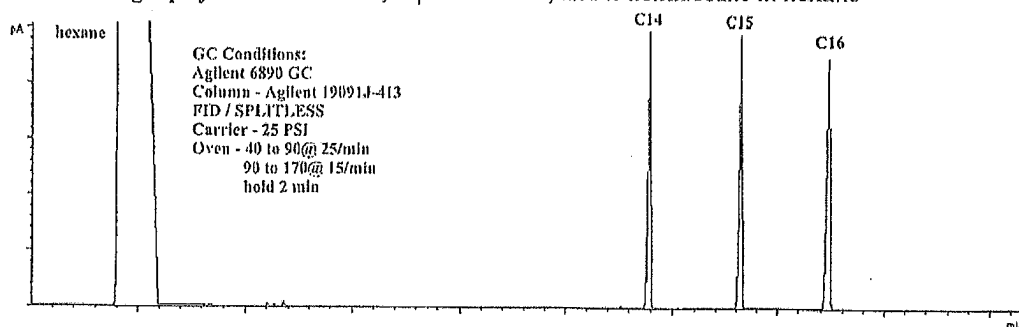

Date of release: 30 June 2023

Date of expiration: 31 July 2025

Monica Bourgeois
QMS Representative

เอกสารสอบเทียบเครื่องมือการตรวจวัดคุณภาพอากาศในบรรยากาศ



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT					
CHEMILUMINESCENT NO / NO ₂ / NO _x ANALYZER					
DATE :	06 May 2026	BRAND :	API	MODEL :	200E
NO.	NOX-R03			SERIAL NO.	4410
Calibrator (Dilution System)					
Brand : Teledyne			Model : 700		
Last Cal. Date : 24 October 2025			Serial No. : 421		
Reference Standard Gas					
Standard Gas : Nitric Oxide (NO)			Cylinder No. : A006745V		
Certified Date : 12 March 2025		Expired Date : 12 March 2028		Cylinder Conc. : 48.7 ppm	
CALIBRATING CONDITION					
Pressure	1010	mmbar	Temp.	24.5	°C
			% RH	48	
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.10	-	0	-
NO Span	400	400.1	0.025	400.0	1.003
NO _x Span	400	400.2	0.050	400.0	1.005
API Model 200E NO _x Analyzer Check List					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	500 standard		
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air		
SAMPLE FLOW	510	cc/min	500 ± 50		
OZONE FLOW	79	cc/min	80 ± 15		
PMT	102.8	mV	-20 - 150		
AZERO	94.0	mV	-20 - 150		
HVPS	674	V	420 - 900 constant		
RCELL TEMP	50.4	°C	50 ± 1		
BOX TEMP	29.0	°C	8 - 48		
PMT TEMP	7.5	°C	7 ± 2		
MOLY TEMP	315.3	°C	315 ± 5		
RCELL PRESS	8.3	IN-Hg-A	2 - 10 constant		
SAMPLE PRESS	28.5	IN-Hg-A	25 - 30 constant		
NO Span Conc	400	PPB	20 - 20,000		
NO _x Span Conc	400	PPB	20 - 20,000		
NO Slope	1.003	-	1.0 ± 0.3		
NO _x Slope	1.005	-	1.0 ± 0.3		
NO Offset	0.8	mV	-20 to +150		
NO _x Offset	0.3	mV	-20 to 150		
Stability at Zero	0.1	PPB	< 0.2		
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas		

Calibrated by :

Heeson L.

(Mr.Heeson Lormae)

Approved by :

Yuthana J.

(Mr.Yuthana Tanatharanit)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT					
CHEMILUMINESCENT NO / NO ₂ / NO _x ANALYZER					
DATE :	06 May 2026	BRAND :	API	MODEL :	200E
NO.	NOX-R04	SERIAL NO.	4411		
Calibrator (Dilution System)					
Brand	: Teledyne			Model	: 700
Last Cal. Date	: 24 October 2025			Serial No.	: 421
Reference Standard Gas					
Standard Gas	: Nitric Oxide (NO)			Cylinder No.	: A006745V
Certified Date	: 12 March 2025		Expired Date	: 12 March 2028	
				Cylinder Conc.	: 48.7 ppm
CALIBRATING CONDITION					
Pressure	1010	mmbar	Temp.	24.5	°C
			% RH	48	
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.10	-	0	-
NO Span	400	399.9	-0.025	400.0	1.002
NO _x Span	400	400.1	0.025	400.0	1.005
API Model 200E NO _x Analyzer Check List					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	500 standard		
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air		
SAMPLE FLOW	504	cc/min	500 ± 50		
OZONE FLOW	79	cc/min	80 ± 15		
PMT	102.9	mV	-20 - 150		
AZERO	93.9	mV	-20 - 150		
HVPS	675	V	420 - 900 constant		
RCELL TEMP	50.2	°C	50 ± 1		
BOX TEMP	29.2	°C	8 - 48		
PMT TEMP	7.1	°C	7 ± 2		
MOLY TEMP	315.1	°C	315 ± 5		
RCELL PRESS	8.3	IN-Hg-A	2 - 10 constant		
SAMPLE PRESS	28.5	IN-Hg-A	25 - 30 constant		
NO Span Conc	400	PPB	20 - 20,000		
NO _x Span Conc	400	PPB	20 - 20,000		
NO Slope	1.002	-	1.0 ± 0.3		
NO _x Slope	1.005	-	1.0 ± 0.3		
NO Offset	1.0	mV	-20 to +150		
NO _x Offset	0.5	mV	-20 to 150		
Stability at Zero	0.1	PPB	< 0.2		
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas		

Calibrated by : Heeson L.
(Mr.Heeson Lormae)

Approved by : Yutthana J.
(Mr.Yutthana Tanatharanit)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT					
CHEMILUMINESCENT NO / NO ₂ / NO _x ANALYZER					
DATE :	06 May 2026	BRAND :	API	MODEL :	200E
NO.	NOX-R05	SERIAL NO.	4413		
Calibrator (Dilution System)					
Brand : Teledyne			Model : 700		
Last Cal. Date : 24 October 2025			Serial No. : 421		
Reference Standard Gas					
Standard Gas : Nitric Oxide (NO)			Cylinder No. : A006745V		
Certified Date : 12 March 2025		Expired Date : 12 March 2028		Cylinder Conc. : 48.7 ppm	
CALIBRATING CONDITION					
Pressure	1010	mmbar	Temp.	24.5	°C
% RH 48					
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.11	-	0	-
NO Span	400	399.8	-0.050	400.0	1.002
NO _x Span	400	400.1	0.025	400.0	1.006
API Model 200E NO _x Analyzer Check List					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	500 standard		
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air		
SAMPLE FLOW	505	cc/min	500 ± 50		
OZONE FLOW	79	cc/min	80 ± 15		
PMT	103.7	mV	-20 - 150		
AZERO	94.4	mV	-20 - 150		
HVPS	670	V	420 - 900 constant		
RCELL TEMP	50.3	°C	50 ± 1		
BOX TEMP	29.3	°C	8 - 48		
PMT TEMP	7.1	°C	7 ± 2		
MOLY TEMP	314.9	°C	315 ± 5		
RCELL PRESS	8.3	IN-Hg-A	2 - 10 constant		
SAMPLE PRESS	28.6	IN-Hg-A	25 - 30 constant		
NO Span Conc	400	PPB	20 - 20,000		
NO _x Span Conc	400	PPB	20 - 20,000		
NO Slope	1.002	-	1.0 ± 0.3		
NO _x Slope	1.006	-	1.0 ± 0.3		
NO Offset	1.1	mV	-20 to +150		
NO _x Offset	0.7	mV	-20 to 150		
Stability at Zero	0.1	PPB	< 0.2		
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas		

Calibrated by :

Heeson L.

(Mr.Heeson Lormae)

Approved by :

Yutthana J.

(Mr.Yutthana Tanatharanit)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT					
CHEMILUMINESCENT NO / NO ₂ / NO _x ANALYZER					
DATE :	06 May 2026	BRAND :	API	MODEL :	200E
NO.	NOX-R07	SERIAL NO.	4468		
Calibrator (Dilution System)					
Brand	: Teledyne			Model	: 700
Last Cal. Date	: 24 October 2025			Serial No.	: 421
Reference Standard Gas					
Standard Gas	: Nitric Oxide (NO)			Cylinder No.	: A006745V
Certified Date	: 12 March 2025		Expired Date	: 12 March 2028	
				Cylinder Conc.	: 48.7 ppm
CALIBRATING CONDITION					
Pressure	1010	mmbar	Temp.	24.5	°C
			% RH	48	
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	-0.10	-	0	-
NO Span	400	399.9	-0.025	400.0	1.003
NO _x Span	400	400.2	0.050	400.0	1.006
API Model 200E NO _x Analyzer Check List					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	500 standard		
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air		
SAMPLE FLOW	506	cc/min	500 ± 50		
OZONE FLOW	78	cc/min	80 ± 15		
PMT	103.2	mV	-20 - 150		
AZERO	94.3	mV	-20 - 150		
HVPS	672	V	420 - 900 constant		
RCELL TEMP	50.0	°C	50 ± 1		
BOX TEMP	29.4	°C	8 - 48		
PMT TEMP	7.2	°C	7 ± 2		
MOLY TEMP	315.2	°C	315 ± 5		
RCELL PRESS	8.3	IN-Hg-A	2 - 10 constant		
SAMPLE PRESS	28.6	IN-Hg-A	25 - 30 constant		
NO Span Conc	400	PPB	20 - 20,000		
NO _x Span Conc	400	PPB	20 - 20,000		
NO Slope	1.003	-	1.0 ± 0.3		
NO _x Slope	1.006	-	1.0 ± 0.3		
NO Offset	1.0	mV	-20 to +150		
NO _x Offset	0.5	mV	-20 to 150		
Stability at Zero	0.1	PPB	< 0.2		
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas		

Calibrated by :

Heeson L.

(Mr.Heeson Lormae)

Approved by :

Yutthana J.

(Mr.Yutthana Tanatharanit)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT					
SO ₂ FLUORESCENT ANALYZER					
DATE :	06 May 2026	BRAND :	API	MODEL :	100E
NO.	SO ₂ -R01			SERIAL NO.	3415
Calibrator (Dilution System)					
Brand	: Teledyne			Model	: 700
Last Cal. Date	: 24 October 2025			Serial No.	: 421
Reference Standard Gas					
Standard Gas	: Sulphur Dioxide (SO ₂)			Cylinder No.	: A00814SK
Certified Date	: 21 June 2021	Expired Date	: 21 June 2029	Cylinder Conc.	: 49.8 ppm
CALIBRATING CONDITION					
Pressure	1010	mmbar	Temp.	24.5	°C
				% RH	48
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	-0.10	-	0	-
SO ₂ Span	400.0	400.4	0.100	400.0	1.005
API Model 100E SO ₂ Analyzer Check list					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	0-500		
SAMPLE PRESS	28.5	in-Hg	25-35		
SAMPLE FLOW	652	cc/min	650 ± 10%		
PMT	103.2	mV	-20-150 with Zero Air		
UV LAMP	3078.3	mV	1000-4900		
STR. LGT	61.3	PPB	<100		
DRK PMT	62.9	mV	-50 - 200		
DRK LMP	57.8	mV	-50 - 200		
HVPS	671	V	550-900 constant		
DCPS	2518	mV	2500 ± 200		
RCELL TEMP	50.1	°C	50 ± 1		
BOX TEMP	29.3	°C	5-40		
PMT TEMP	7.0	°C	7 ± 2.0		
SO ₂ Span Conc	400	PPB	20-20,000		
SO ₂ Slope	1.005	-	1.0 ± 0.3		
SO ₂ Offset	21.9	mV	<250		
Stability at Zero	0.1	PPB	<0.2		
Stability at Span	0.2	PPB	0.5% of reading (above 50 ppb)		

Calibrated by :

Heeson L.

(Mr.Heeson Lormae)

Approved by :

Yutthana J.

(Mr.Yutthana Tanatharanit)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT					
SO ₂ FLUORESCENT ANALYZER					
DATE :	06 May 2026	BRAND :	API	MODEL :	100E
NO.	SO ₂ -R02			SERIAL NO.	3431
Calibrator (Dilution System)					
Brand	: Teledyne			Model	: 700
Last Cal. Date	: 24 October 2025			Serial No.	: 421
Reference Standard Gas					
Standard Gas	: Sulphur Dioxide (SO ₂)			Cylinder No.	: A00814SK
Certified Date	: 21 June 2021	Expired Date	: 21 June 2029	Cylinder Conc.	: 49.8 ppm
CALIBRATING CONDITION					
Pressure	1010	mmbar	Temp.	24.5	°C
				% RH	48
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	-0.10	-	0	-
SO ₂ Span	400.0	400.2	0.050	400.0	1.004
API Model 100E SO ₂ Analyzer Check list					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	0-500		
SAMPLE PRESS	28.6	in-Hg	25-35		
SAMPLE FLOW	653	cc/min	650 ± 10%		
PMT	103.3	mV	-20-150 with Zero Air		
UV LAMP	2892.3	mV	1000-4900		
STR. LGT	60.9	PPB	<100		
DRK PMT	62.7	mV	-50 - 200		
DRK LMP	57.6	mV	-50 - 200		
HVPS	672	V	550-900 constant		
DCPS	2517	mV	2500 ± 200		
RCELL TEMP	50.0	°C	50 ± 1		
BOX TEMP	29.2	°C	5-40		
PMT TEMP	7.2	°C	7 ± 2.0		
SO ₂ Span Conc	400	PPB	20-20,000		
SO ₂ Slope	1.004	-	1.0 ± 0.3		
SO ₂ Offset	21.8	mV	<250		
Stability at Zero	0.1	PPB	<0.2		
Stability at Span	0.2	PPB	0.5% of reading (above 50 ppb)		

Calibrated by :

Heeson L.

(Mr.Heeson Lormae)

Approved by :

Yuthana J.

(Mr.Yuthana Tanatharanit)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT					
SO ₂ FLUORESCENT ANALYZER					
DATE :	06 May 2026	BRAND :	API	MODEL :	100E
NO.	SO ₂ -R04			SERIAL NO.	3489
Calibrator (Dilution System)					
Brand	: Teledyne			Model	: 700
Last Cal. Date	: 24 October 2025			Serial No.	: 421
Reference Standard Gas					
Standard Gas	: Sulphur Dioxide (SO ₂)			Cylinder No.	: A00814SK
Certified Date	: 21 June 2021	Expired Date	: 21 June 2029	Cylinder Conc.	: 49.8 ppm
CALIBRATING CONDITION					
Pressure	1010	mmbar	Temp.	24.5	°C
				% RH	48
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.10	-	0	-
SO ₂ Span	400.0	400.3	0.075	400.0	1.004
API Model 100E SO ₂ Analyzer Check list					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	0-500		
SAMPLE PRESS	28.3	in-Hg	25-35		
SAMPLE FLOW	652	cc/min	650 ± 10%		
PMT	102.8	mV	-20-150 with Zero Air		
UV LAMP	3015.3	mV	1000-4900		
STR. LGT	61.2	PPB	<100		
DRK PMT	63.5	mV	-50 - 200		
DRK LMP	57.8	mV	-50 - 200		
HVPS	673	V	550-900 constant		
DCPS	2515	mV	2500 ± 200		
RCELL TEMP	50.1	°C	50 ± 1		
BOX TEMP	29.3	°C	5-40		
PMT TEMP	7.1	°C	7 ± 2.0		
SO ₂ Span Conc	400	PPB	20-20,000		
SO ₂ Slope	1.004	-	1.0 ± 0.3		
SO ₂ Offset	22.0	mV	<250		
Stability at Zero	0.1	PPB	<0.2		
Stability at Span	0.2	PPB	0.5% of reading (above 50 ppb)		

Calibrated by :

Heeson L.

(Mr.Heeson Lormae)

Approved by :

Yuthana J.

(Mr.Yuthana Tanatharanit)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT					
SO ₂ FLUORESCENT ANALYZER					
DATE :	06 May 2026	BRAND :	TELEDYNE	MODEL :	TML-60
NO.	SO ₂ -R07			SERIAL NO.	TR51068
Calibrator (Dilution System)					
Brand	: Teledyne			Model	: 700
Last Cal. Date	: 24 October 2025			Serial No.	: 421
Reference Standard Gas					
Standard Gas	: Sulphur Dioxide (SO ₂)			Cylinder No.	: A00814SK
Certified Date	: 21 June 2021	Expired Date	: 21 June 2029	Cylinder Conc.	: 49.8 ppm
CALIBRATING CONDITION					
Pressure	1010	mmbar	Temp.	24.5	°C
				% RH	48
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.10	-	0	-
SO ₂ Span	400.0	400.2	0.050	400.0	1.003
API Model TML-60 SO ₂ Analyzer Check list					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	0-500		
SAMPLE PRESS	28.7	in-Hg	25-35		
SAMPLE FLOW	657	cc/min	650 ± 10%		
PMT	102.8	mV	-20-150 with Zero Air		
UV LAMP	2090.5	mV	1000-4900		
STR. LGT	60.9	PPB	<100		
DRK PMT	62.7	mV	-50 - 200		
DRK LMP	57.9	mV	-50 - 200		
HVPS	673	V	550-900 constant		
DCPS	2517	mV	2500 ± 200		
RCELL TEMP	50.3	°C	50 ± 1		
BOX TEMP	29.1	°C	5-40		
PMT TEMP	7.2	°C	7 ± 2.0		
SO ₂ Span Conc	400	PPB	20-20,000		
SO ₂ Slope	1.003	-	1.0 ± 0.3		
SO ₂ Offset	22.1	mV	<250		
Stability at Zero	0.1	PPB	<0.2		
Stability at Span	0.2	PPB	0.5% of reading (above 50 ppb)		

Calibrated by :

Heeson L.

(Mr.Heeson Lormae)

Approved by :

Yuthana J.

(Mr.Yuthana Tanatharanit)

เอกสารสอบเทียบเครื่องมือการตรวจวิเคราะห์คุณภาพน้ำเสีย

**QUALITY CALIBRATION CO., LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584



CERTIFICATE No : 26E3363
REFERENCE No : 80514-1

PAGE : 1 OF 3

Certificate of Calibration

EQUIPMENT : pH METER
MANUFACTURER : HANNA
MODEL : HI3512
SERIAL No : TH118035
ID No : PH 04/56
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.

CALIBRATION DATE : 02-Apr-26

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 02-Apr-26

RECEIVED DATE : 01-Apr-26

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.



**QUALITY CALIBRATION CO., LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 26E3363

PAGE : 2 OF 3

Calibration Report

EQUIPMENT : pH METER
MANUFACTURER : HANNA
ID No : PH 04/56
RECEIVED DATE : 01-Apr-26
AMBIENT TEMPERATURE : 23 °C ± 3 °C

MODEL : HI3512
SERIAL NUMBER : TH118035
CALIBRATION DATE : 02-Apr-26
RELATIVE HUMIDITY : 50 % RH ± 10% RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT METHOD BASED ON WI-TQ-062 AND WI-TQ-063. THE DISPLAY UNIT WAS TESTED BY GENERATING STANDARD VOLTAGE TO THE UNIT AND READING THE VALUE COMPARED WITH THE CALCULATED VALUE. THE DISPLAY AND ELECTRODE WAS CALIBRATED BY USING STANDARD pH BUFFER
2. REFERENCE STANDARD INSTRUMENTS :-

<u>INSTRUMENT</u>	<u>MODEL</u>	<u>SERIAL No/</u> <u>LOT No</u>	<u>CERTIFICATE No</u>	<u>DUE DATE</u>
1) pH STANDARD SOLUTION	00651-36	CC829914	4956-16178366	11-Sep-27
2) pH STANDARD SOLUTION	00651-38	CC831093	4957-16224157	01-Oct-27
3) pH STANDARD SOLUTION	00651-40	CC826321	4958-16046326	10-Jul-27
4) PROCESS CALIBRATOR	CA150	91S6079	26E936	17-Mar-27
5) BATH	260014	1247 48074	25T9431	12-Sep-26
6) THERMOMETER WITH PROBE	421504	55000379	25T9466	12-Sep-26

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO SI UNIT MAINTAINED AT :-
- NATIONAL INSTITUTE OF STANDARD AND TECHNOLOGY, USA.
 - NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION : ADJUSTMENT**1. DISPLAY UNIT ONLY**SLOPE FACTOR $k = 2.303 RT/F = 59 \text{ mV/pH}$

mV APPLIED	UUC READING (mV)	CORRECTION (mV)	UUC READING (pH)	UNCERTAINTY OF MEASUREMENT (± mV)	COVERAGE FACTOR k
414.11	414.3	-0.19	-0.256	0.15	2.00
354.95	355.1	-0.15	0.759	0.15	2.00
295.80	296.0	-0.20	1.773	0.15	2.00
236.64	236.8	-0.16	2.787	0.15	2.00
177.48	177.7	-0.22	3.801	0.15	2.00
118.32	118.5	-0.18	4.816	0.15	2.00
59.16	59.4	-0.24	5.831	0.15	2.00
0.00	0.2	-0.20	6.845	0.15	2.00
-59.16	-58.9	-0.26	7.878	0.15	2.00
-118.32	-118.1	-0.22	8.915	0.15	2.00
-177.48	-177.2	-0.28	9.952	0.15	2.00
-236.64	-236.4	-0.24	10.990	0.15	2.00
-295.80	-295.5	-0.30	12.027	0.15	2.00
-354.95	-354.7	-0.25	13.064	0.15	2.00
-414.11	-413.8	-0.31	14.101	0.15	2.00

END OF CALIBRATION REPORT PAGE 2 OF 3



**QUALITY CALIBRATION CO., LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 26E3363

PAGE : 3 OF 3

Calibration Report**RESULT OF CALIBRATION (CONTINUE):****2. DISPLAY UNIT WITH pH ELECTRODE S/N: 11340D0M**

STANDARD pH BUFFER SOLUTION (pH)	UUC READING (pH)	CORRECTION (pH)	VALUE BEFORE ADJUSTMENT	UNCERTAINTY OF MEASUREMENT ($\pm$ pH)	COVERAGE FACTOR k
4.008	4.008	0.000	4.142	0.012	2.00
6.998	7.000	-0.002	7.068	0.012	2.00
10.007	10.009	-0.002	10.226	0.014	2.00

3. DISPLAY UNIT WITH TEMPERATURE

STANDARD READING ($^{\circ}$ C)	UUC READING ($^{\circ}$ C)	CORRECTION ($^{\circ}$ C)	VALUE BEFORE ADJUSTMENT	UNCERTAINTY OF MEASUREMENT ($\pm$ $^{\circ}$ C)	COVERAGE FACTOR k
25.004	25.0	0.004	---	0.0085	2.00

4. PERCENT SLOPE 91%

UUC : UNIT UNDER CALIBRATION

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



Certificate of Calibration

Certificate No. : 69-400023-2

Page : 1 of 2

Submitted by : S. P. S Consulting Service Co., Ltd.

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Equipment : Liquid in Glass Thermometer

Manufacturer : SK

Model : N/A

Range : 0 °C to 100 °C

Resolution : 1 °C

Serial No. : N/A

Immersion : Total

ID No. : TM21/59

Environment : Ambient Temperature : (23 ± 2) °C

Relative Humidity : (50 ± 15) %

Line Voltage : (220 ± 22) VAC

Date of Received : 13 January 2026

Date of Calibration : 16 January 2026

Date of Issue : 16 January 2026

Calibrated by : Chortip Samchusri

Calibration Method : This instrument was calibrated by In-house method comparison technique CAL-M4001 based on ASTM E77-07 by compared with PRT in the liquid bath at the constant controlled temperature.

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Platinum Resistance Thermometer (PRT)

ID No.	Cert. No.	Due Date	Traceability
400001	TT-0023-24	16 Feb 2026	National Institute of Metrology Thailand (NIMT)

2. Standard Digital Thermometer

ID No.	Cert. No.	Due Date	Traceability
400003	25E1656	22 May 2027	National Institute of Metrology Thailand (NIMT)
400004	25E1656	22 May 2027	National Institute of Metrology Thailand (NIMT)

Approved by :



(Permpon Chanpu)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 69-400023-2

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

Ice point check : UUC* reading 0 °C Standard reading 0.4773 °C

Standard Reading (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
20.3922	20	0.4	0.31

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o()o -





CERTIFICATE No : 26M2268
REFERENCE No : 80204-3

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE

MANUFACTURER : SARTORIUS

MODEL : BSA224S-CW

SERIAL No : 36591843

ID No : BA 09/61

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : SUCHAT S.

CALIBRATION DATE : 05-Mar-26

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 06-Mar-26

RECEIVED DATE : 05-Mar-26





CERTIFICATE No : 26M2268

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : BSA224S-CW
MANUFACTURER : SARTORIUS S/N : 36591843
ID No : BA 09/61 RECEIVED DATE : 05-Mar-26
AIR PRESSURE : 1004mbar $\pm$ 1mbar CALIBRATION DATE : 05-Mar-26
AMBIENT TEMPERATURE : 25° C $\pm$ 1° C RELATIVE HUMIDITY : 50 %RH $\pm$ 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	C02250116	28-Jan-27
2) STANDARD WEIGHT	E2	15843	C02250117	29-Jan-27

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0.000055 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ($\pm$ g)
0.0	0.0000	0.0000	0.00010
0.1	0.1000	0.0000	0.00011
0.2	0.2000	0.0000	0.00010
0.5	0.5000	0.0000	0.00011
1.0	1.0000	0.0000	0.00011
2.0	2.0000	0.0000	0.00011
5.0	5.0000	0.0000	0.00011
10.0	10.0000	0.0000	0.00011
20.0	20.0001	-0.0001	0.00011
50.0	50.0000	0.0000	0.00013
100.0	100.0001	-0.0001	0.00019
200.0	200.0001	-0.0001	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	100.0000
2	100.0000
3	100.0000
4	100.0000
5	100.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





QUALITY CALIBRATION CO., LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkoe, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com

CERTIFICATE No : 26T0464

REFERENCE No : 79659-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : COD REACTOR

MANUFACTURER : HACH

MODEL : DRB 200

SERIAL No : 15110C0497

ID No : DRB 04/59

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : SOMCHAI S.

CALIBRATION DATE : 30-Jan-26

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 30-Jan-26

RECEIVED DATE : 30-Jan-26

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.



F-G010 REV : 03



CERTIFICATE No : 26T0464

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : COD REACTOR
MANUFACTURER : HACH
ID NUMBER : DRB 04/59
RECEIVED DATE : 30-Jan-26
AMBIENT TEMPERATURE : 23° C ± 1° C

MODEL : DRB 200
SERIAL NUMBER : 15110C0497
CALIBRATION DATE : 30-Jan-26
RELATIVE HUMIDITY : 54 %RH ± 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT METHOD WITH CALIBRATED THERMOCOUPLE TYPE K UNDER NO LOAD CONDITION. THE THERMOCOUPLES WERE PLACED ON POINTS AND LOCATED AS THE PICTURE.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT

MODEL

SERIAL No

CERTIFICATE No

DUE DATE

1) DATA LOGGER WITH TC TYPE K

HYDRA 2635A

6849323

25T5342

18-Jun-26

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO., LTD.

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

13	14	15
10	11	12
7	8	9
4	5	6
1	2	3
BLOCK No.1 FRONT		

13	14	15
10	11	12
7	8	9
4	5	6
1	2	3
BLOCK No.2 FRONT		

TEMPERATURE MEASUREMENT ACCURACY TEST

Block No.		1	2
Controller temperature (°C)		144	145
Indicating Temperature		144	145
Measured Temperature (°C) at Spread Locations	1	149.3	149.8
	2	149.1	149.9
	3	149.9	149.6
	4	150.0	149.3
	5	149.8	149.5
	6	149.9	149.1
	7	149.7	149.7
	8	149.5	149.9
	9	149.8	149.4
	10	148.5	149.4
	11	149.1	150.2
	12	149.2	150.0
	13	149.0	149.6
	14	149.1	150.3
	15	148.5	149.0
Uncertainty of Measurement(± °C)		0.89	0.89

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2 : LOCATION 10 WAS REFERENCE LOCATION.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k =2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



เอกสารสอบเทียบเครื่องมือการตรวจวิเคราะห์คุณภาพน้ำผิวดิน

**QUALITY CALIBRATION CO., LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584



CERTIFICATE No : 26E3363
REFERENCE No : 80514-1

PAGE : 1 OF 3

Certificate of Calibration

EQUIPMENT : pH METER
MANUFACTURER : HANNA
MODEL : HI3512
SERIAL No : TH118035
ID No : PH 04/56
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.

CALIBRATION DATE : 02-Apr-26

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 02-Apr-26

RECEIVED DATE : 01-Apr-26

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.



**QUALITY CALIBRATION CO., LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 26E3363

PAGE : 2 OF 3

Calibration Report

EQUIPMENT : pH METER
MANUFACTURER : HANNA MODEL : HI3512
ID No : PH 04/56 SERIAL NUMBER : TH118035
RECEIVED DATE : 01-Apr-26 CALIBRATION DATE : 02-Apr-26
AMBIENT TEMPERATURE : 23 °C ± 3 °C RELATIVE HUMIDITY : 50 % RH ± 10% RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT METHOD BASED ON WI-TQ-062 AND WI-TQ-063. THE DISPLAY UNIT WAS TESTED BY GENERATING STANDARD VOLTAGE TO THE UNIT AND READING THE VALUE COMPARED WITH THE CALCULATED VALUE. THE DISPLAY AND ELECTRODE WAS CALIBRATED BY USING STANDARD pH BUFFER
2. REFERENCE STANDARD INSTRUMENTS :-

<u>INSTRUMENT</u>	<u>MODEL</u>	<u>SERIAL No/</u> <u>LOT No</u>	<u>CERTIFICATE No</u>	<u>DUE DATE</u>
1) pH STANDARD SOLUTION	00651-36	CC829914	4956-16178366	11-Sep-27
2) pH STANDARD SOLUTION	00651-38	CC831093	4957-16224157	01-Oct-27
3) pH STANDARD SOLUTION	00651-40	CC826321	4958-16046326	10-Jul-27
4) PROCESS CALIBRATOR	CA150	91S6079	26E936	17-Mar-27
5) BATH	260014	1247 48074	25T9431	12-Sep-26
6) THERMOMETER WITH PROBE	421504	55000379	25T9466	12-Sep-26

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO SI UNIT MAINTAINED AT :-
- NATIONAL INSTITUTE OF STANDARD AND TECHNOLOGY, USA.
 - NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION : ADJUSTMENT**1. DISPLAY UNIT ONLY**SLOPE FACTOR $k = 2.303 RT/F = 59 \text{ mV/pH}$

mV APPLIED	UUC READING (mV)	CORRECTION (mV)	UUC READING (pH)	UNCERTAINTY OF MEASUREMENT (± mV)	COVERAGE FACTOR k
414.11	414.3	-0.19	-0.256	0.15	2.00
354.95	355.1	-0.15	0.759	0.15	2.00
295.80	296.0	-0.20	1.773	0.15	2.00
236.64	236.8	-0.16	2.787	0.15	2.00
177.48	177.7	-0.22	3.801	0.15	2.00
118.32	118.5	-0.18	4.816	0.15	2.00
59.16	59.4	-0.24	5.831	0.15	2.00
0.00	0.2	-0.20	6.845	0.15	2.00
-59.16	-58.9	-0.26	7.878	0.15	2.00
-118.32	-118.1	-0.22	8.915	0.15	2.00
-177.48	-177.2	-0.28	9.952	0.15	2.00
-236.64	-236.4	-0.24	10.990	0.15	2.00
-295.80	-295.5	-0.30	12.027	0.15	2.00
-354.95	-354.7	-0.25	13.064	0.15	2.00
-414.11	-413.8	-0.31	14.101	0.15	2.00

END OF CALIBRATION REPORT PAGE 2 OF 3



**QUALITY CALIBRATION CO., LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 26E3363

PAGE : 3 OF 3

Calibration Report**RESULT OF CALIBRATION (CONTINUE):****2. DISPLAY UNIT WITH pH ELECTRODE S/N: 11340D0M**

STANDARD pH BUFFER SOLUTION (pH)	UUC READING (pH)	CORRECTION (pH)	VALUE BEFORE ADJUSTMENT	UNCERTAINTY OF MEASUREMENT ($\pm$ pH)	COVERAGE FACTOR k
4.008	4.008	0.000	4.142	0.012	2.00
6.998	7.000	-0.002	7.068	0.012	2.00
10.007	10.009	-0.002	10.226	0.014	2.00

3. DISPLAY UNIT WITH TEMPERATURE

STANDARD READING ($^{\circ}$ C)	UUC READING ($^{\circ}$ C)	CORRECTION ($^{\circ}$ C)	VALUE BEFORE ADJUSTMENT	UNCERTAINTY OF MEASUREMENT ($\pm$ $^{\circ}$ C)	COVERAGE FACTOR k
25.004	25.0	0.004	---	0.0085	2.00

4. PERCENT SLOPE 91%

UUC : UNIT UNDER CALIBRATION

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



Certificate of Calibration

Certificate No. : 69-400023-2

Page : 1 of 2

Submitted by : S. P. S Consulting Service Co., Ltd.

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Equipment : Liquid in Glass Thermometer

Manufacturer : SK

Model : N/A

Range : 0 °C to 100 °C

Resolution : 1 °C

Serial No. : N/A

Immersion : Total

ID No. : TM21/59

Environment : Ambient Temperature : (23 ± 2) °C

Relative Humidity : (50 ± 15) %

Line Voltage : (220 ± 22) VAC

Date of Received : 13 January 2026

Date of Calibration : 16 January 2026

Date of Issue : 16 January 2026

Calibrated by : Chortip Samchusri

Calibration Method : This instrument was calibrated by In-house method comparison technique CAL-M4001 based on ASTM E77-07 by compared with PRT in the liquid bath at the constant controlled temperature.

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Platinum Resistance Thermometer (PRT)

ID No.	Cert. No.	Due Date	Traceability
400001	TT-0023-24	16 Feb 2026	National Institute of Metrology Thailand (NIMT)

2. Standard Digital Thermometer

ID No.	Cert. No.	Due Date	Traceability
400003	25E1656	22 May 2027	National Institute of Metrology Thailand (NIMT)
400004	25E1656	22 May 2027	National Institute of Metrology Thailand (NIMT)

Approved by :



(Permpon Chanpu)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 69-400023-2

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

Ice point check : UUC* reading 0 °C Standard reading 0.4773 °C

Standard Reading (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
20.3922	20	0.4	0.31

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o()o -





CERTIFICATE No : 26M2268
REFERENCE No : 80204-3

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE

MANUFACTURER : SARTORIUS

MODEL : BSA224S-CW

SERIAL No : 36591843

ID No : BA 09/61

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : SUCHAT S.

CALIBRATION DATE : 05-Mar-26

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 06-Mar-26

RECEIVED DATE : 05-Mar-26





CERTIFICATE No : 26M2268

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : BSA224S-CW
MANUFACTURER : SARTORIUS S/N : 36591843
ID No : BA 09/61 RECEIVED DATE : 05-Mar-26
AIR PRESSURE : 1004mbar $\pm$ 1mbar CALIBRATION DATE : 05-Mar-26
AMBIENT TEMPERATURE : 25°C $\pm$ 1°C RELATIVE HUMIDITY : 50 %RH $\pm$ 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	C02250116	28-Jan-27
2) STANDARD WEIGHT	E2	15843	C02250117	29-Jan-27

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0.000055 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ($\pm$ g)
0.0	0.0000	0.0000	0.00010
0.1	0.1000	0.0000	0.00011
0.2	0.2000	0.0000	0.00010
0.5	0.5000	0.0000	0.00011
1.0	1.0000	0.0000	0.00011
2.0	2.0000	0.0000	0.00011
5.0	5.0000	0.0000	0.00011
10.0	10.0000	0.0000	0.00011
20.0	20.0001	-0.0001	0.00011
50.0	50.0000	0.0000	0.00013
100.0	100.0001	-0.0001	0.00019
200.0	200.0001	-0.0001	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	100.0000
2	100.0000
3	100.0000
4	100.0000
5	100.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





QUALITY CALIBRATION CO., LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkoe, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com

CERTIFICATE No : 26T0464

REFERENCE No : 79659-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : COD REACTOR

MANUFACTURER : HACH

MODEL : DRB 200

SERIAL No : 15110C0497

ID No : DRB 04/59

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : SOMCHAI S.

CALIBRATION DATE : 30-Jan-26

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 30-Jan-26

RECEIVED DATE : 30-Jan-26

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.





QUALITY CALIBRATION CO., LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 26T0464

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : COD REACTOR
MANUFACTURER : HACH
ID NUMBER : DRB 04/59
RECEIVED DATE : 30-Jan-26
AMBIENT TEMPERATURE : 23° C ± 1° C
MODEL : DRB 200
SERIAL NUMBER : 15110C0497
CALIBRATION DATE : 30-Jan-26
RELATIVE HUMIDITY : 54 %RH ± 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT METHOD WITH CALIBRATED THERMOCOUPLE TYPE K UNDER NO LOAD CONDITION. THE THERMOCOUPLES WERE PLACED ON POINTS AND LOCATED AS THE PICTURE.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT

MODEL

SERIAL No

CERTIFICATE No

DUE DATE

1) DATA LOGGER WITH TC TYPE K

HYDRA 2635A

6849323

25T5342

18-Jun-26


3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO., LTD.

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

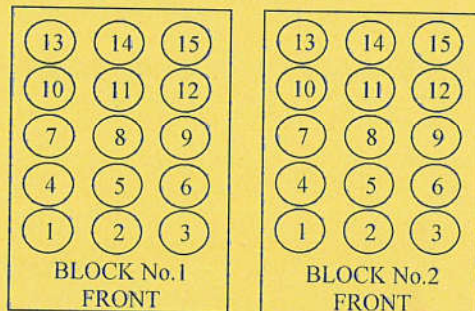

TEMPERATURE MEASUREMENT ACCURACY TEST

Block No.		1	2
Controller temperature (°C)		144	145
Indicating Temperature		144	145
Measured Temperature (°C) at Spread Locations	1	149.3	149.8
	2	149.1	149.9
	3	149.9	149.6
	4	150.0	149.3
	5	149.8	149.5
	6	149.9	149.1
	7	149.7	149.7
	8	149.5	149.9
	9	149.8	149.4
	10	148.5	149.4
	11	149.1	150.2
	12	149.2	150.0
	13	149.0	149.6
	14	149.1	150.3
	15	148.5	149.0
Uncertainty of Measurement(± °C)		0.89	0.89

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2 : LOCATION 10 WAS REFERENCE LOCATION.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k =2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



เอกสารสอบเทียบการตรวจวัดระดับเสียงที่ขอบเขตรั้วพื้นที่โรงงาน



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com., www.spscon.com

Noise R_055/26

Sound Level Meter Calibration Report

Acoustic Calibrator Data						
Brand	ACO		Number	AC 03/56		
Model	2127		Serial No.	130006		
Calibration Range	94 dB, 1000 Hz		Last Calibration	21 February 2025		
			Due Date	21 February 2026		

Calibration Data						
Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-R45	ACO	6236	00192057	20 January 2026	93.9	93.9
ACO-R48	ACO	6236	00192060	20 January 2026	94.0	93.9
ACO-R49	ACO	6236	00192061	20 January 2026	93.9	93.9
ACO-R54	ACO	6236	00222307	20 January 2026	93.9	93.9

Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)	93.81 ± 0.10 dB
--	-----------------

Calibrated by : _____
(Mr. Heeson Lormae)

Approved by : Yutthana J.
(Mr. Yutthana Tanatharanit)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Noise R_247/26

Sound Level Meter Calibration Report

Acoustic Calibrator Data

Brand	ACO	Number	AC 03/56
Model	2127	Serial No.	130006
Calibration Range	94 dB, 1000 Hz	Last Calibration	11 February 2026
		Due Date	11 February 2027

Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-R21	ACO	6236	00182004	15 April 2026	93.9	93.9
ACO-R22	ACO	6236	00182010	15 April 2026	93.9	93.9
ACO-R23	ACO	6236	00192035	15 April 2026	94.0	93.9
ACO-R55	ACO	6236	00222309	15 April 2026	93.9	93.9
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.89 ± 0.10 dB	

Calibrated by :

Heeson L.
(Mr. Heeson Lormae)

Approved by :

Yutthana J.
(Mr. Yutthana Tanatharanit)

เอกสารสอบเทียบการตรวจวัดระดับเสียงในพื้นที่ทำงาน



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com, www.spscon.com

Noise R_056/26

Sound Level Meter Calibration Report

Acoustic Calibrator Data

Brand	ACO	Number	AC 03/56
Model	2127	Serial No.	130006
Calibration Range	94 dB, 1000 Hz	Last Calibration	21 February 2025
		Due Date	21 February 2026

Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-R40	ACO	6236	00192052	21 January 2026	93.9	93.9
ACO-R41	ACO	6236	00192053	21 January 2026	93.9	93.9
ACO-R50	ACO	6236	00192062	21 January 2026	93.9	93.9
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.81 ± 0.10 dB	

Calibrated by :

Heeson L.

(Mr. Heeson Lormae)

Approved by :

Yutthana J.

(Mr. Yutthana Tanatharanit)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Noise R_074/26

Sound Level Meter Calibration Report

Acoustic Calibrator Data						
Brand	ACO		Number	AC 03/56		
Model	2127		Serial No.	130006		
Calibration Range	94 dB, 1000 Hz		Last Calibration	21 February 2025		
			Due Date	21 February 2026		
Calibration Data						
Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-R40	ACO	6236	00192052	01 February 2026	93.9	93.9
ACO-R41	ACO	6236	00192053	01 February 2026	93.9	93.9
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.81 ± 0.10 dB	

Calibrated by :

Heeson L.

(Mr. Heeson Lormae)

Approved by :

Yutthana J.

(Mr. Yutthana Tanatharanit)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Noise R_159/26

Sound Level Meter Calibration Report

Acoustic Calibrator Data

Brand	ACO	Number	AC 03/56
Model	2127	Serial No.	130006
Calibration Range	94 dB, 1000 Hz	Last Calibration	11 February 2026
		Due Date	11 February 2027

Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-R51	ACO	6236	00192063	02 April 2026	93.9	93.9
ACO-R52	ACO	6236	00192064	02 April 2026	93.9	93.9
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.89 ± 0.10 dB	

Calibrated by : _____
(Mr. Heeson Lormae)

Approved by : _____
(Mr. Yutthana Tanatharanit)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com. www.spscon.com

Noise Dose R_057/26

Noise Dose Meter Calibration Report

Acoustic Calibrator Data

Brand	SVANTEK	Number	SV 03/60
Model	SV34	Serial No.	83820
Calibration Range	114 dB, 1000 Hz	Last Calibration	25 August 2025
		Due Date	25 August 2026

Calibration Data

Sound Level Meter Data

Calibration Data

SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
NMD-R03	SVANTEK	SV-104IS	60153	21 January 2026	114.0	114.0
NMD-R06	SVANTEK	SV-104IS	60146	21 January 2026	114.0	114.0
NMD-R13	SVANTEK	SV-104IS	63438	21 January 2026	114.0	114.0
NMD-R22	SVANTEK	SV-104IS	80801	21 January 2026	114.0	114.0
NMD-R26	SVANTEK	SV-104IS	80836	21 January 2026	114.1	114.0
NMD-R35	SVANTEK	SV-104IS	80873	21 January 2026	114.0	114.0
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					114.02± 0.10 dB	

Calibrated by :

Heeson L.

(Mr. Heeson Lormae)

Approved by :

Yutthana J.

(Mr. Yutthana Tanatharanit)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Noise Dose R_073/26

Noise Dose Meter Calibration Report

Acoustic Calibrator Data

Brand	SVANTEK	Number	SV 03/60
Model	SV34	Serial No.	83820
Calibration Range	114 dB, 1000 Hz	Last Calibration	25 August 2025
		Due Date	25 August 2026

Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
NMD-R03	SVANTEK	SV-104IS	60153	01 February 2026	114.0	114.0
NMD-R06	SVANTEK	SV-104IS	60146	01 February 2026	114.0	114.0
NMD-R26	SVANTEK	SV-104IS	80836	01 February 2026	114.0	114.0
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					114.02± 0.10 dB	

Calibrated by :

Heeson L.

(Mr. Heeson Lormae)

Approved by :

Yutthana J.

(Mr. Yutthana Tanatharanit)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Noise Dose R_160/26

Noise Dose Meter Calibration Report

Acoustic Calibrator Data

Brand	SVANTEK	Number	SV 03/60
Model	SV34	Serial No.	83820
Calibration Range	114 dB, 1000 Hz	Last Calibration	25 August 2025
		Due Date	25 August 2026

Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
NMD-R03	SVANTEK	SV-104IS	60153	02 April 2026	114.0	114.0
NMD-R13	SVANTEK	SV-104IS	63438	02 April 2026	114.0	114.0
NMD-R22	SVANTEK	SV-104IS	80801	02 April 2026	114.0	114.0
NMD-R26	SVANTEK	SV-104IS	80836	02 April 2026	114.1	114.0
NMD-R35	SVANTEK	SV-104IS	80873	02 April 2026	114.0	114.0
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					114.02± 0.10 dB	

Calibrated by : _____
(Mr. Heeson Lormae)

Approved by : _____
(Mr. Yutthana Tanatharanit)

เอกสารสอบเทียบการตรวจวัดคุณภาพอากาศในสถานที่ทำงาน



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136833

Environmental Conditions

Temperature : 25 ± 3 °C
Pressure : 1010 ± 15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R ²
R01	SKC	224-PCXR4	602467	05/01/2026	1,000	1,500	2,000	999	1,505	2,009	1.011x - 15.308	1.000
R02	SKC	224-PCXR4	626450	05/01/2026	1,000	2,000	3,000	1,001	1,505	2,005	1.005x - 5.625	1.000
R03	SKC	224-PCXR4	691592	05/01/2026	1,000	1,500	2,000	998	1,499	2,010	1.009x - 11.382	1.000
R04	SKC	224-PCXR4	691672	05/01/2026	1,000	1,500	2,000	999	1,496	2,000	0.992x + 5.045	0.999
R05	SKC	224-PCXR4	798470	06/01/2026	1,000	1,500	2,000	997	1,480	1,991	0.995x - 8.487	0.999
R06	SKC	224-PCXR4	798456	06/01/2026	1,000	1,500	2,000	1,000	1,502	1,992	0.993x + 2.874	0.999
R07	SKC	224-PCXR4	798480	06/01/2026	1,000	1,500	2,000	1,000	1,508	2,000	1.000x + 1.559	1.000
R08	SKC	224-PCXR4	883215	07/01/2026	1,000	1,500	2,000	1,001	1,500	2,000	1.004x - 8.216	1.000
R09	SKC	224-PCXR4	034650	05/01/2026	1,000	1,500	2,000	999	1,509	2,005	1.005x - 6.025	1.000
R10	SKC	224-PCXR4	091765	05/01/2026	1,000	1,500	2,000	1,001	1,509	2,008	1.007x - 8.311	1.000
R11	SKC	224-PCXR4	091763	05/01/2026	1,000	1,500	2,000	999	1,502	1,995	1.002x - 10.594	0.999
R12	SKC	224-PCXR4	091568	06/01/2026	1,000	1,500	2,000	999	1,495	1,994	0.994x - 1.683	0.999
R13	SKC	224-PCXR4	091638	06/01/2026	1,000	1,500	2,000	999	1,499	1,994	0.998x - 7.136	0.999
R14	SKC	224-PCXR4	091764	06/01/2026	1,000	1,500	2,000	1,004	1,507	2,006	1.007x - 8.975	1.000
R15	SKC	224-PCXR8	529457	06/01/2026	1,000	1,500	2,000	1,004	1,502	2,002	0.999x + 1.731	1.000
R16	SKC	224-PCXR8	529643	05/01/2026	1,000	1,500	2,000	1,001	1,511	2,010	1.010x - 13.433	1.000
R17	SKC	224-PCXR8	529645	06/01/2026	1,000	1,500	2,000	1,004	1,502	2,003	0.998x + 4.238	1.000
R18	SKC	224-PCXR8	566756	05/01/2026	1,000	1,500	2,000	1,003	1,504	2,006	1.004x - 3.774	1.000
R19	SKC	224-PCXR8	566802	05/01/2026	1,000	1,500	2,000	1,003	1,498	1,995	1.001x - 8.224	0.999
R20	SKC	224-PCXR8	529089	06/01/2026	1,000	1,500	2,000	997	1,509	1,985	0.994x + 5.269	0.999
R21	SKC	224-PCXR8	665728	06/01/2026	1,000	1,500	2,000	1,000	1,510	1,995	0.998x - 1.139	0.999
R22	SKC	224-PCXR8	707444	05/01/2026	1,000	1,500	2,000	1,004	1,507	2,008	1.004x - 5.709	1.000
R23	SKC	224-PCXR8	761067	05/01/2026	1,000	1,500	2,000	1,009	1,504	2,006	1.000x + 1.179	1.000
R24	SKC	224-PCXR8	707893	05/01/2026	1,000	1,500	2,000	999	1,497	1,992	0.998x - 8.383	0.999
R25	SKC	224-PCXR8	761052	06/01/2026	1,000	1,500	2,000	998	1,503	1,975	0.984x + 17.071	0.999
R26	SKC	224-PCXR8	707956	05/01/2026	1,000	1,500	2,000	997	1,492	1,992	0.991x + 0.388	1.000
R27	SKC	224-PCXR8	707398	05/01/2026	1,000	1,500	2,000	1,000	1,495	2,002	1.002x - 3.898	1.000
R28	SKC	224-PCXR8	707481	06/01/2026	1,000	1,500	2,000	1,009	1,503	2,008	0.996x + 8.659	1.000
R29	SKC	224-PCXR8	707402	07/01/2026	1,000	1,500	2,000	1,006	1,513	2,009	1.002x - 1.219	0.999
R30	SKC	224-PCXR8	093811	07/01/2026	1,000	1,500	2,000	1,001	1,513	2,008	1.008x - 9.239	1.000
R31	SKC	224-PCXR8	093183	06/01/2026	1,000	1,500	2,000	1,010	1,507	2,013	1.003x - 0.780	1.000
R32	SKC	224-PCXR8	671950	06/01/2026	1,000	1,500	2,000	999	1,498	1,999	1.000x + 0.668	1.000
R33	SKC	224-PCXR4	626254	06/01/2026	1,000	1,500	2,000	1,000	1,508	2,007	1.004x - 5.149	1.000
R34	SKC	224-PCXR4	626131	05/01/2026	1,000	1,500	2,000	996	1,498	2,003	1.010x - 18.178	1.000
R35	SKC	224-PCXR8	707460	05/01/2026	1,000	1,500	2,000	1,006	1,496	2,004	0.999x + 0.388	1.000
R36	SKC	224-PCXR8	707446	05/01/2026	1,000	1,500	2,000	1,006	1,504	2,008	1.005x - 6.281	1.000
R37	SKC	224-PCXR8	707432	06/01/2026	1,000	1,500	2,000	1,003	1,505	2,004	1.004x - 5.005	1.000
R38	SKC	224-PCXR8	707349	06/01/2026	1,000	1,500	2,000	998	1,498	1,997	0.999x - 1.655	1.000
R39	SKC	224-PCXR8	761095	06/01/2026	1,000	1,500	2,000	1,000	1,497	2,003	1.005x - 8.068	1.000

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

Peera Detudom
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chaluchak, Bangkok 10900

Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com., www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136833

Environmental Conditions

Temperature : 25 $\pm$ 3 $^{\circ}$ C
Pressure : 1010 $\pm$ 15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R ²
R40	SKC	224-PCXR4	612753	05/01/2026	1,000	1,500	2,000	997	1,506	1,998	1.000x - 0.556	1.000
R41	SKC	224-PCXR4	626140	05/01/2026	1,000	1,500	2,000	995	1,504	1,992	0.996x - 3.574	0.999
R42	SKC	224-PCXR4	626463	05/01/2026	1,000	1,500	2,000	1,006	1,505	1,984	0.988x + 15.108	0.999
R43	SKC	224-PCXR4	626129	05/01/2026	1,000	1,500	2,000	993	1,504	1,972	0.982x + 17.902	0.999
R44	SKC	224-PCXR4	602753	06/01/2026	1,000	1,500	2,000	1,001	1,495	2,000	1.001x - 3.434	1.000
R45	SKC	224-PCXR4	626137	06/01/2026	1,000	1,500	2,000	998	1,494	1,997	0.996x + 1.827	1.000

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

Peera Detudom
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136833

Environmental Conditions

Temperature : 25 ± 3 °C
Pressure : 1010 ± 15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R ²
R01	SKC	224-PCXR4	602467	01/04/2026	1,000	1,500	2,000	1,001	1,500	2,007	1.005x - 6.003	1.000
R02	SKC	224-PCXR4	626450	05/04/2026	1,000	2,000	3,000	1,000	1,503	2,001	1.001x - 0.383	1.000
R03	SKC	224-PCXR4	691592	03/04/2026	1,000	1,500	2,000	1,005	1,501	2,000	1.007x - 15.384	0.999
R04	SKC	224-PCXR4	691672	03/04/2026	1,000	1,500	2,000	1,007	1,513	1,999	0.996x + 5.855	0.999
R05	SKC	224-PCXR4	798470	05/04/2026	1,000	1,500	2,000	1,000	1,499	1,997	0.997x + 3.107	1.000
R06	SKC	224-PCXR4	798456	03/04/2026	1,000	1,500	2,000	998	1,497	1,996	0.998x + 0.120	1.000
R07	SKC	224-PCXR4	798480	05/04/2026	1,000	1,500	2,000	1,002	1,506	2,001	0.999x + 3.219	1.000
R08	SKC	224-PCXR4	883215	03/04/2026	1,000	1,500	2,000	1,004	1,501	1,992	1.003x - 9.877	0.999
R09	SKC	224-PCXR4	034650	03/04/2026	1,000	1,500	2,000	998	1,506	2,003	1.004x - 5.723	1.000
R10	SKC	224-PCXR4	091765	03/04/2026	1,000	1,500	2,000	999	1,507	1,996	1.005x - 13.080	0.999
R11	SKC	224-PCXR4	091763	05/04/2026	1,000	1,500	2,000	1,001	1,504	2,001	1.000x + 0.104	1.000
R12	SKC	224-PCXR4	091568	03/04/2026	1,000	1,500	2,000	998	1,505	1,996	0.998x + 1.482	1.000
R13	SKC	224-PCXR4	091638	03/04/2026	1,000	1,500	2,000	1,001	1,504	2,000	0.999x + 2.097	1.000
R14	SKC	224-PCXR4	091764	05/04/2026	1,000	1,500	2,000	1,007	1,506	2,001	1.004x - 8.866	0.999
R15	SKC	224-PCXR8	529457	05/04/2026	1,000	1,500	2,000	998	1,492	1,999	1.001x - 6.322	1.000
R16	SKC	224-PCXR8	529643	03/04/2026	1,000	1,500	2,000	1,004	1,506	2,004	1.007x - 11.726	0.999
R17	SKC	224-PCXR8	529645	05/04/2026	1,000	1,500	2,000	998	1,503	1,998	1.000x - 0.703	1.000
R18	SKC	224-PCXR8	566756	03/04/2026	1,000	1,500	2,000	999	1,508	1,995	1.002x - 8.012	0.999
R19	SKC	224-PCXR8	566802	05/04/2026	1,000	1,500	2,000	998	1,502	1,998	1.000x - 0.823	1.000
R20	SKC	224-PCXR8	529089	03/04/2026	1,000	1,500	2,000	999	1,503	1,996	0.997x + 2.001	1.000
R21	SKC	224-PCXR8	665728	03/04/2026	1,000	1,500	2,000	998	1,505	1,999	1.000x - 0.483	1.000
R22	SKC	224-PCXR8	707444	05/04/2026	1,000	1,500	2,000	1,007	1,496	2,000	1.001x - 6.418	0.999
R23	SKC	224-PCXR8	761067	05/04/2026	1,000	1,500	2,000	1,001	1,502	2,004	1.002x - 1.446	1.000
R24	SKC	224-PCXR8	707893	03/04/2026	1,000	1,500	2,000	1,002	1,503	2,001	0.999x + 2.560	1.000
R25	SKC	224-PCXR8	761052	03/04/2026	1,000	1,500	2,000	1,009	1,504	2,005	0.997x + 4.106	0.999
R26	SKC	224-PCXR8	707956	05/04/2026	1,000	1,500	2,000	1,002	1,503	2,000	0.998x + 4.497	1.000
R27	SKC	224-PCXR8	707398	03/04/2026	1,000	1,500	2,000	1,001	1,505	2,004	1.003x - 1.921	1.000
R28	SKC	224-PCXR8	707481	05/04/2026	1,000	1,500	2,000	1,010	1,513	2,006	0.997x + 5.531	0.999
R29	SKC	224-PCXR8	707402	03/04/2026	1,000	1,500	2,000	1,003	1,502	1,992	1.003x - 10.216	0.999
R30	SKC	224-PCXR8	093811	05/04/2026	1,000	1,500	2,000	999	1,512	2,005	1.007x - 9.705	1.000
R31	SKC	224-PCXR8	093183	05/04/2026	1,000	1,500	2,000	1,011	1,510	2,011	1.001x + 2.983	0.999
R32	SKC	224-PCXR8	671950	03/04/2026	1,000	1,500	2,000	1,001	1,500	2,001	0.999x + 2.272	1.000
R33	SKC	224-PCXR4	626254	05/04/2026	1,000	1,500	2,000	998	1,507	2,002	1.005x - 10.975	1.000
R34	SKC	224-PCXR4	626131	05/04/2026	1,000	1,500	2,000	997	1,496	2,000	1.007x - 14.230	1.000
R35	SKC	224-PCXR8	707460	05/04/2026	1,000	1,500	2,000	998	1,509	1,996	1.000x - 2.915	1.000
R36	SKC	224-PCXR8	707446	05/04/2026	1,000	1,500	2,000	1,003	1,492	2,003	1.007x - 16.135	0.999
R37	SKC	224-PCXR8	707432	03/04/2026	1,000	1,500	2,000	999	1,507	2,005	1.003x - 6.095	1.000
R38	SKC	224-PCXR8	707349	03/04/2026	1,000	1,500	2,000	1,003	1,499	1,999	0.997x + 2.141	1.000
R39	SKC	224-PCXR8	761095	05/04/2026	1,000	1,500	2,000	1,005	1,508	2,004	1.000x - 0.152	0.999

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

Peera Detudom
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136833

Environmental Conditions

Temperature : 25 $\pm$ 3 $^{\circ}$ C
Pressure : 1010 $\pm$ 15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R ²
R40	SKC	224-PCXR4	612753	05/04/2026	1,000	1,500	2,000	1,004	1,497	2,000	0.998x + 1.430	1.000
R41	SKC	224-PCXR4	626140	03/04/2026	1,000	1,500	2,000	998	1,498	1,997	0.999x + 0.943	1.000
R42	SKC	224-PCXR4	626463	05/04/2026	1,000	1,500	2,000	1,005	1,513	1,998	0.997x + 4.138	0.999
R43	SKC	224-PCXR4	626129	03/04/2026	1,000	1,500	2,000	1,003	1,498	2,000	0.998x + 2.029	1.000
R44	SKC	224-PCXR4	602753	03/04/2026	1,000	1,500	2,000	996	1,509	1,997	1.003x - 8.036	1.000
R45	SKC	224-PCXR4	626137	05/04/2026	1,000	1,500	2,000	1,011	1,514	2,005	0.995x + 8.367	0.999

Calibrated by :

Adul Dangklom

(Mr. Adul Dangklom)

Approved by :

Peera Detudom

(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Rotameter Calibration Report (For Personal Pump Low Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136833

Calibration Data

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (mL/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R ²
L-R01	Dwyer	VFA-21	01/04/2026	50	100	200	50.3	101.1	201.9	0.998x + 0.955	1.000
L-R02	Dwyer	VFA-21	01/04/2026	50	100	200	50.2	101.7	201.0	0.999x + 0.367	0.999
L-R03	Dwyer	VFA-21	03/04/2026	50	100	200	50.3	101.2	201.0	1.001x + 0.605	1.000
L-R04	Dwyer	VFA-21	05/04/2026	50	100	200	50.7	100.8	200.2	1.000x + 0.719	1.000
L-R05	Dwyer	VFA-21	05/04/2026	50	100	200	50.1	101.2	200.5	1.001x - 0.213	0.999
L-R06	Dwyer	VFA-21	03/04/2026	50	100	200	50.3	100.8	200.1	0.999x + 0.639	1.000

Calibrated by :

Adul Dangklom
(Mr.Adul Dangklom)

Approved by :

Peera Detudom
(Mr. Peera Detudom)



บริษัท ไทยยูนิค จำกัด

THAI UNIQUE CO., LTD.

80-82 ถนนประชาธิปไตย แขวงบางขุนพรหม เขตพระนคร กรุงเทพฯ 10200

80-82 Prachathipatai Rd., Bangkhunphrom, Pranakorn, Bangkok 10200

Tel. 0-2629-0191-6, 0-2280-1787, Fax. 0-2280-1788, E-mail : thawatt@thaiunique.com, Website : www.thaiunique.com

GAS CHROMATOGRAPH TEST CERTIFICATION

Certificate No. : SV0825/23032

Instrument Type : Gas Chromatography

Model : 3800

Serial Number : 00734

Organization : S.P.S. Consulting Service Co., Ltd.

Address : 7 Phahonyothin Soi 24 Phahonyothin Rd. Ladyao Chatuchak Bangkok 10900

Date : 02/08/2025

ELECTRONIC TEST

CPU	☒ PASS	☐ FAIL
DISPLAY & LED TEST	☒ PASS	☐ FAIL
VENT TEST	☒ PASS	☐ FAIL
KEY ECHO TEST	☒ PASS	☐ FAIL
DESTRUCTION RAM TEST	☒ PASS	☐ FAIL

RUN CHROMATOGRAM TEST

DETECTOR : Flame Ionization Detectors (FID Channel-Front)

INJECTOR : 1079 Injector

GC CONDITION:

Column	80 °C hold 1 min., rate 20 °C/min. to 200 °C hold 1min.
Injector	220 °C
Detector	300 °C
Column flow	5 mL/min
Makeup flow	25 mL/min
Air flow	300 mL/min
Hydrogen flow	30 mL/min

Column:Capillary Column CP sil 5 CB 0.25 ID x 15 M

Sample: 1 µL Injection FID Test Sample 0.218g/L C14,C15,C16 in hexane (diluted to 30ppm)

SENSITIVITY TEST: C15. (Area count) = 515,940 Counts.



VARIAN



บริษัท ไทยยูนิค จำกัด

THAI UNIQUE CO., LTD.

80-82 ถนนประชาธิปไตย แขวงบางขุนพรหม เขตพระนคร กรุงเทพฯ 10200

80-82 Prachathipatai Rd., Bangkhunphrom, Pranakorn, Bangkok 10200

Tel: 0-2629-0191-6, 0-2280-1787, Fax: 0-2280-1788, E-mail : thawatt@thaiunique.com, Website : www.thaiunique.com

Detector Sensitivity (FID)

Detector Response	Result	Specification
Baseline Noise (μ V)	2.40	≤ 50
Baseline Drift (%)	0.18	≤ 1
Sensitivity (S/N for C15)	19,716	$\geq 1,024$

Temperature Specification

Temperature	Set	Result	Specification
Column Oven ($^{\circ}$ C)	80	79	± 5
Injector ($^{\circ}$ C)	220	218	± 5
Detector ($^{\circ}$ C)	300	298	± 5
Incubator ($^{\circ}$ C)	60	N/A	± 5

Relative Standard Deviation % (%RSD)

Checkout Procedure	Result	Specification
Area C15 (%)	1.48	≤ 5
Retention Time C15 (%)	0.08	≤ 0.5

APPROVAL :

Signature:

Engineer : Somchai Pohtongkam

Date : 02/08/2025



VARIAN



บริษัท ไทยยูนิค จำกัด

THAI UNIQUE CO., LTD.

80-82 ถนนประชาธิปไตย แขวงบางขุนพรหม เขตพระนคร กรุงเทพฯ 10200

80-82 Prachathipatai Rd., Bangkhunphrom, Pranakorn, Bangkok 10200

Tel. 0-2629-0191-6, 0-2280-1787, Fax. 0-2280-1788, E-mail : thawatt@thaiunique.com, Website : www.thaiunique.com

Results Integrated System Testing

Checkout Procedure	FID
Detector Position	Front
Inlet Type	1079 Injector
C15 Area 1	506,043
C15 Area 2	520,497
C15 Area 3	522,154
C15 Area 4	521,664
C15 Area 5	509,340
C15 Area Average	515,940
* % RSD (< 5 %)	1.48

* The precision specification should be less than 2.0 % RSD ** (Relative Standard Deviation) for an Auto sampler injection and less than 5 % for Manual injections. To calculate the %RSD, select the C15 peak area for each of the five (5) samples.

** (Relative Standard Deviation is determined by dividing the standard deviation by the average and multiplying by 100.)

$$\% \text{ RSD} = (\text{std.dev} / \text{avg}) * 100$$

Compliance	☒ Pass	☐ Fail
Performance by	<i>Sachin P.</i>	
Date	02/08/2025	



Comments			
Reviewed by	<i>Wattana</i>	Date	02/08/2025



VARIAN



บริษัท ไทยยูนิค จำกัด

THAI UNIQUE CO., LTD.

80-82 ถนนประชาธิปไตย แขวงบางขุนพรหม เขตพระนคร กรุงเทพฯ 10200

80-82 Prachathipatai Rd., Bangkhunphrom, Pranakorn, Bangkok 10200

Tel. 0-2629-0191-6, 0-2280-1787, Fax. 0-2280-1788, E-mail : thawatt@thaiunique.com, Website : www.thaiunique.com

Results Integrated System Testing

Checkout Procedure	FID
Detector Position	Front
Inlet Type	1079 Injector
C15 RT 1	3.874
C15 RT 2	3.880
C15 RT 3	3.875
C15 RT 4	3.872
C15 RT 5	3.878
C15 RT Average	3.876
* % RSD (< 0.5 %)	0.08

* The precision specification should be less than 0.5 % RSD ** (Relative Standard Deviation) for an Auto sampler injection and less than 0.5 % for Manual injections. To calculate the %RSD, select the RT C15 peak for each of the five (5) samples.

** (Relative Standard Deviation is determined by dividing the standard deviation by the average and multiplying by 100.)

$$\% \text{ RSD} = (\text{std.dev} / \text{avg}) * 100$$

Compliance	☒ Pass	☐ Fail
Performance by	<i>Somchai P.</i>	
Date	02/08/2025	



Comments			
Reviewed by	<i>Wattana</i>	Date	02/08/2025



VARIAN


Title :
Run File : e:\sps2025\blk001.run
Method File : c:\star\data\tu\2025\cal fid.mth
Sample ID : blk

Injection Date: 2/8/2568 12:01 Calculation Date: 2/8/2568 12:33

Operator : watsamon Detector Type: 3800 (10 Volts)
Workstation: GC-LAB Bus Address : 44
Instrument : Sample Rate : 10.00 Hz
Channel : Front = FID Run Time : 20.005 min

** LC Workstation Version 6.20 ** 02511-7390-ae7-0265 **

Chart Speed = 1.13 cm/min Attenuation = 1 Zero Offset = 50%
Start Time = 0.000 min End Time = 20.005 min Min / Tick = 1.00

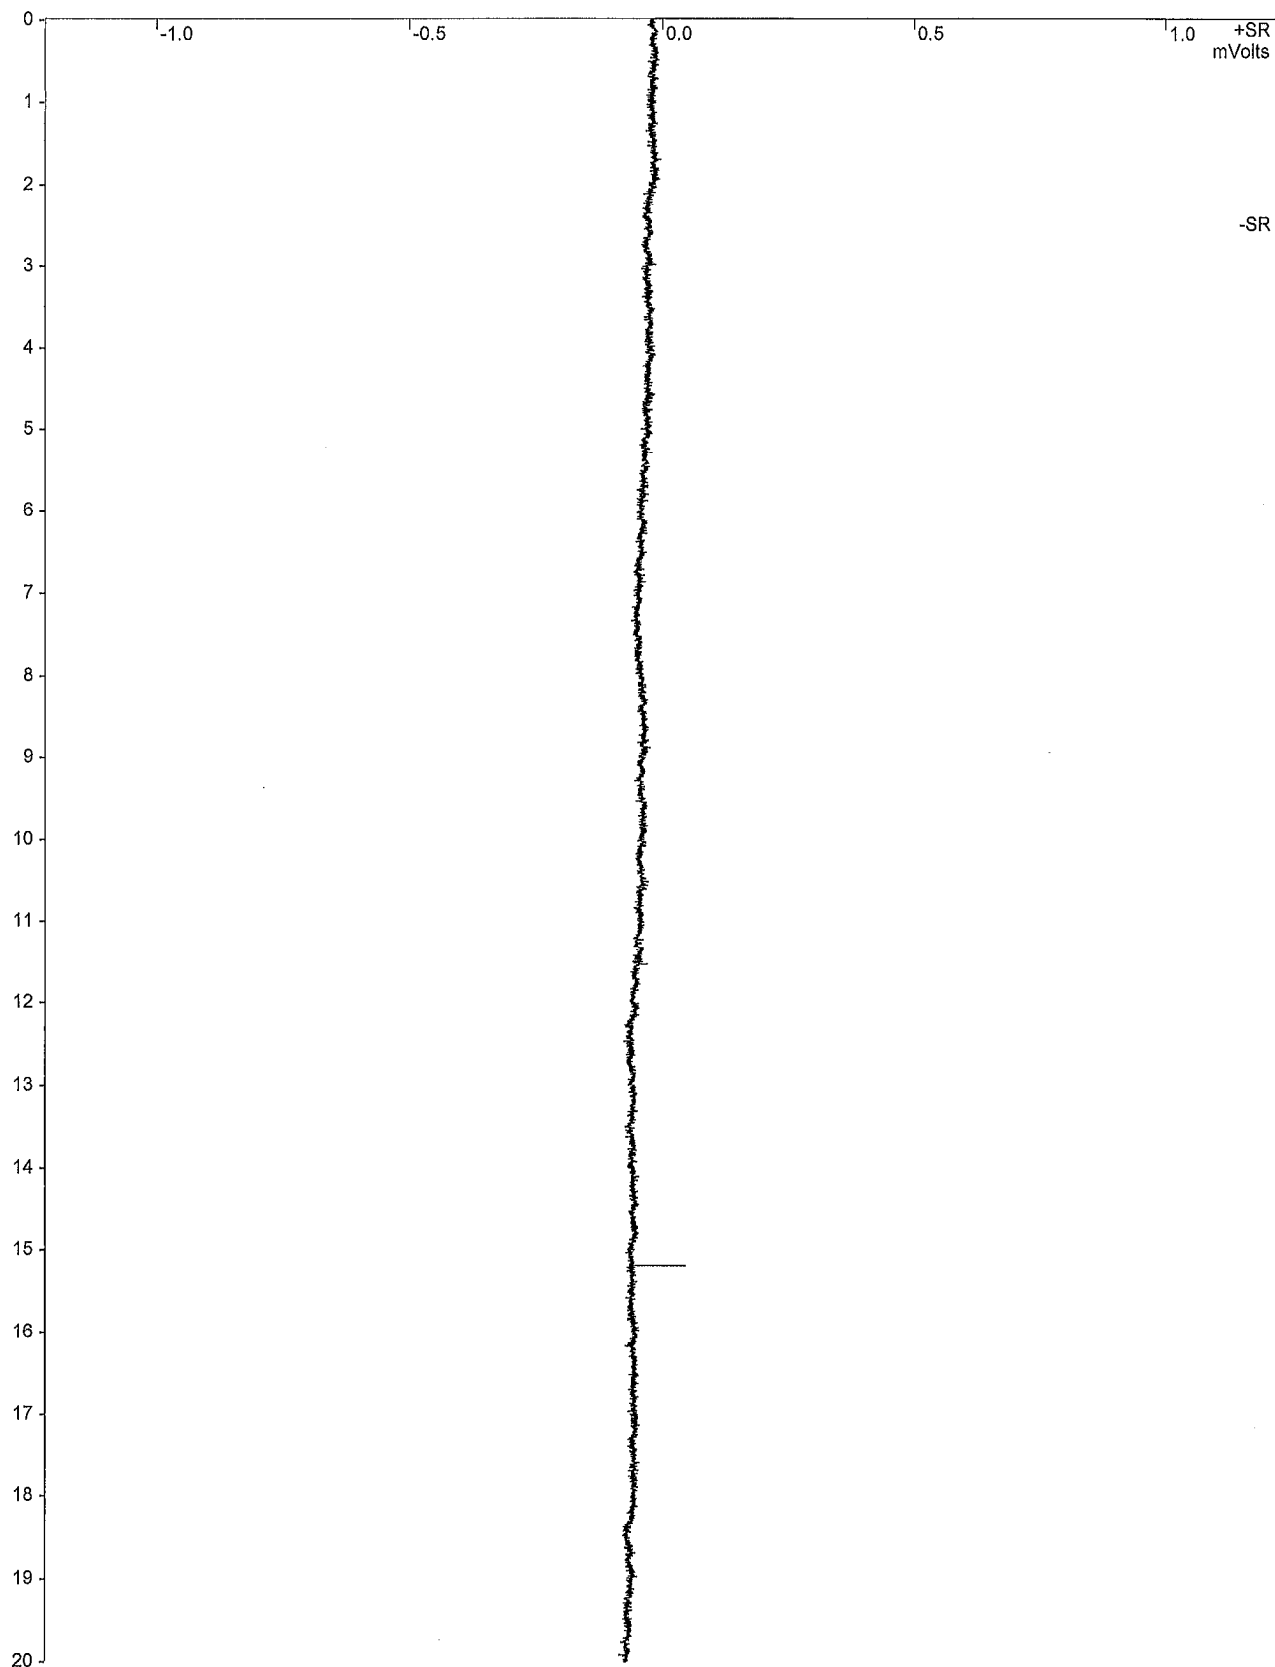

Title :
Run File : e:\sps2025\blk001.run
Method File : c:\star\data\tu\2025\cal fid.mth
Sample ID : blk

Injection Date: 2/8/2568 12:01 Calculation Date: 2/8/2568 12:33

Operator : watsamon Detector Type: 3800 (10 Volts)
Workstation: GC-LAB Bus Address : 44
Instrument : Sample Rate : 10.00 Hz
Channel : Front = FID Run Time : 20.005 min

** LC Workstation Version 6.20 ** 02511-7390-ae7-0265 **

Run Mode : Analysis
Peak Measurement: Peak Area
Calculation Type: External Standard

Peak No.	Peak Name	Result ()	Ret. Time (min)	Time Offset (min)	Area (counts)	Sep. Code	Width 1/2 (sec)	Status Codes
-----	-----	-----	-----	-----	-----	-----	-----	-----
----	-----	=====	-----	=====	=====	-----	-----	-----
	Totals:	0.0000		0.000	0			

Total Unidentified Counts : 0 counts

Detected Peaks: 0 Rejected Peaks: 0 Identified Peaks: 0

Multiplier: 1 Divisor: 1 Unidentified Peak Factor: 0

Baseline Offset: -14 microVolts LSB: 1 microVolts

Noise (used): 24 microVolts - monitored before this run

Manual injection

Data Handling: No peaks


Title :
Run File : e:\sps2025\fidstd001.run
Method File : c:\star\data\tu\2025\cal fid.mth
Sample ID : fidstd

Injection Date: 2/8/2568 12:34 Calculation Date: 2/8/2568 13:26

Operator : watsamon Detector Type: 3800 (10 Volts)
Workstation: GC-LAB Bus Address : 44
Instrument : Sample Rate : 10.00 Hz
Channel : Front = FID Run Time : 7.993 min

** LC Workstation Version 6.20 ** 02511-7390-ae7-0265 **

Chart Speed = 2.83 cm/min Attenuation = 79 Zero Offset = 2%
Start Time = 0.000 min End Time = 7.993 min Min / Tick = 1.00

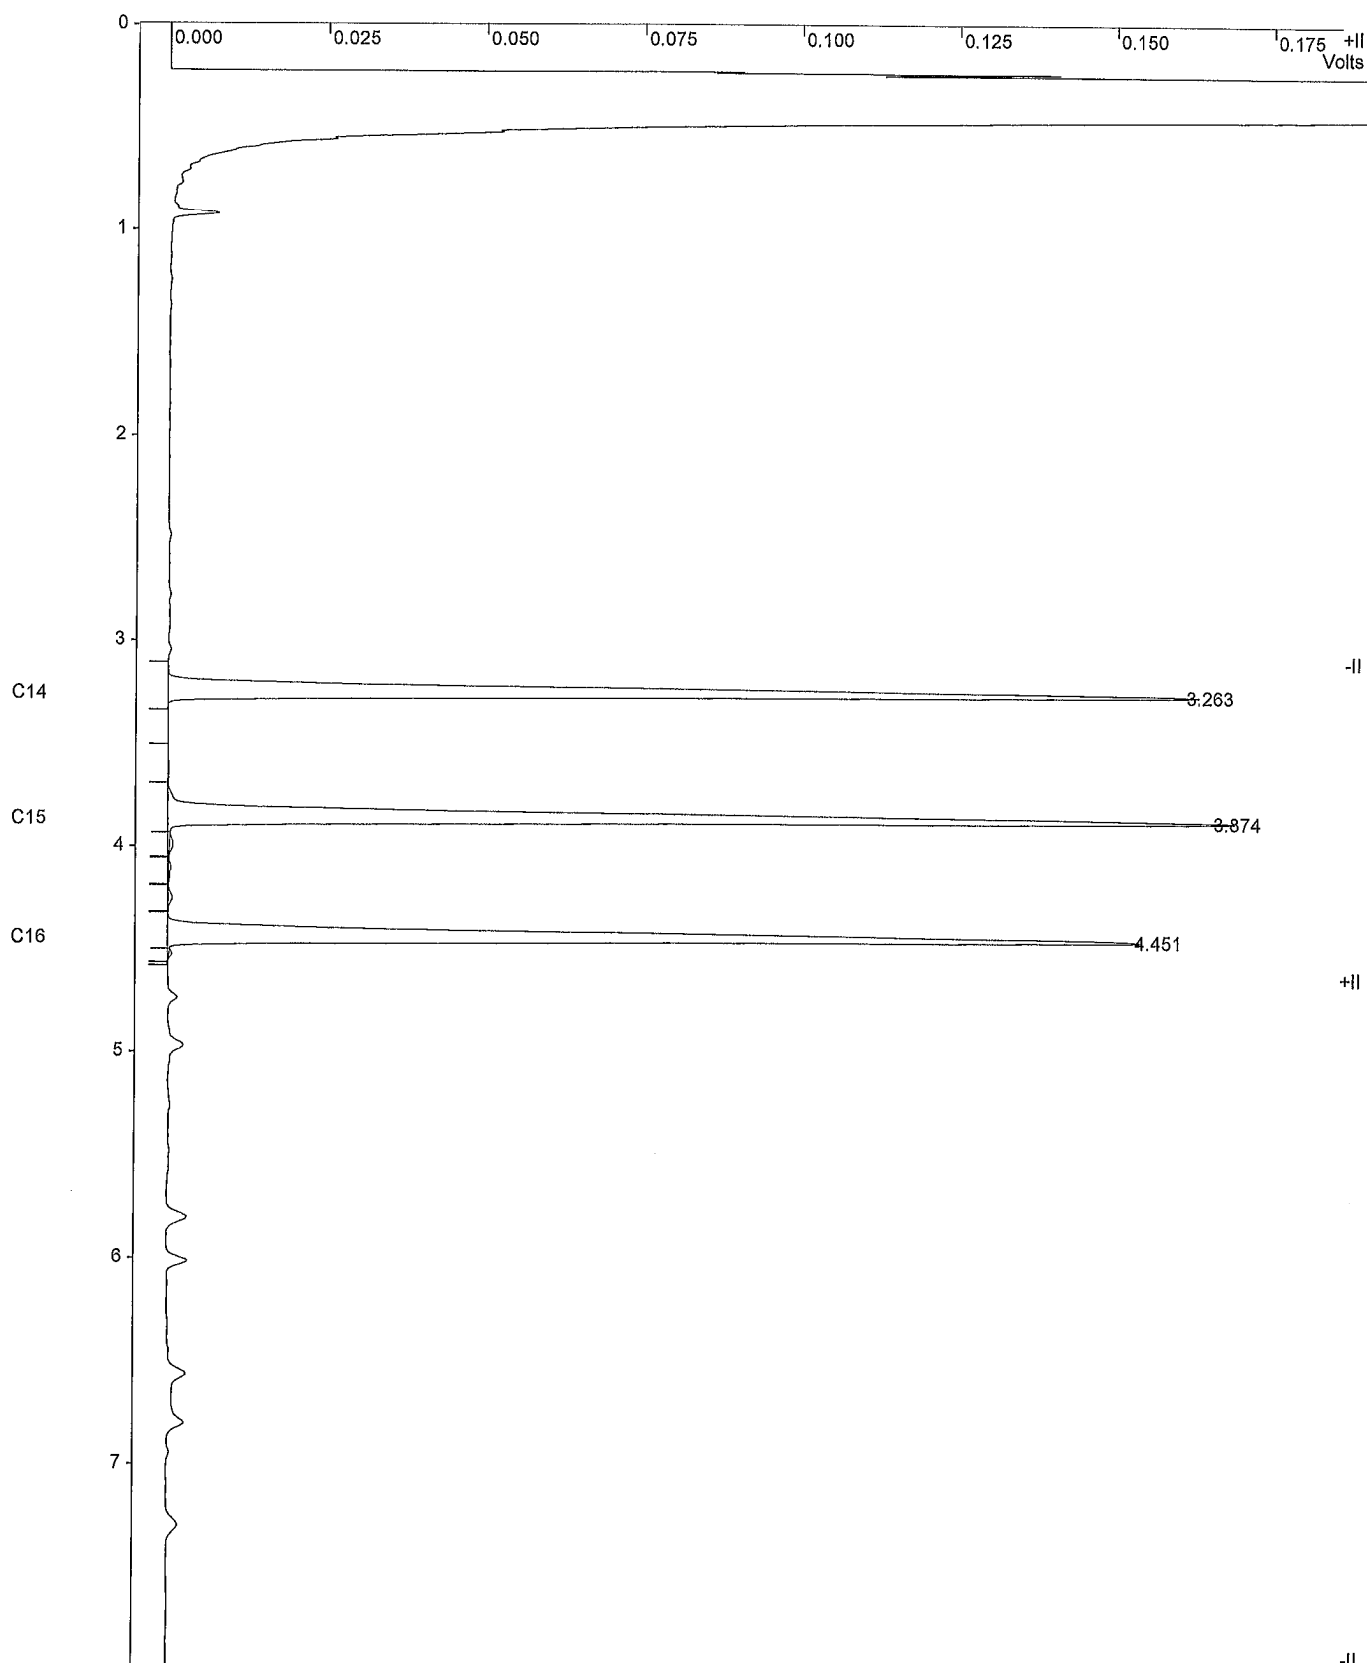

Title :
Run File : e:\sps2025\fidstd001.run
Method File : c:\star\data\tu\2025\cal fid.mth
Sample ID : fidstd

Injection Date: 2/8/2568 12:34 Calculation Date: 2/8/2568 13:26

Operator : watsamon Detector Type: 3800 (10 Volts)
Workstation: GC-LAB Bus Address : 44
Instrument : Sample Rate : 10.00 Hz
Channel : Front = FID Run Time : 7.993 min

** LC Workstation Version 6.20 ** 02511-7390-ae7-0265 **

Run Mode : Calibration
Peak Measurement: Peak Area
Calculation Type: External Standard
Level : 1

Peak No.	Peak Name	Ret. Time (min)	Time Offset (min)	Area (counts)	Sep. Code	Width 1/2 (sec)	Status Codes
1	C14	3.263	0.002	458627	BB	2.7	
2	C15	3.874	0.002	506043	VV	2.8	
3	C16	4.451	0.001	460610	VB	2.8	
Totals:			0.005	1425280			

Total Unidentified Counts : 0 counts

Detected Peaks: 8 Rejected Peaks: 5 Identified Peaks: 3

Multiplier: N/A Divisor: N/A Unidentified Peak Factor: 0

Baseline Offset: 6 microVolts LSB: 1 microVolts

Noise (used): 2 microVolts - monitored before this run

Manual injection

Sample ID: **fid std**



Operator (Inj): **watsamon**

Injection Date: **02/08/2025**

Calc Date: **02/08/2025**

Run Time (min): **7.993**

Workstation: **GC-LAB**

Instrument (Inj):

VARIAN


Run Mode: **Calibration**

Peak Measurement: **Peak Area**

Calculation Type: **External Std.**

e:\sps2025\fidstd001.run

A = FID 10 V RESULTS

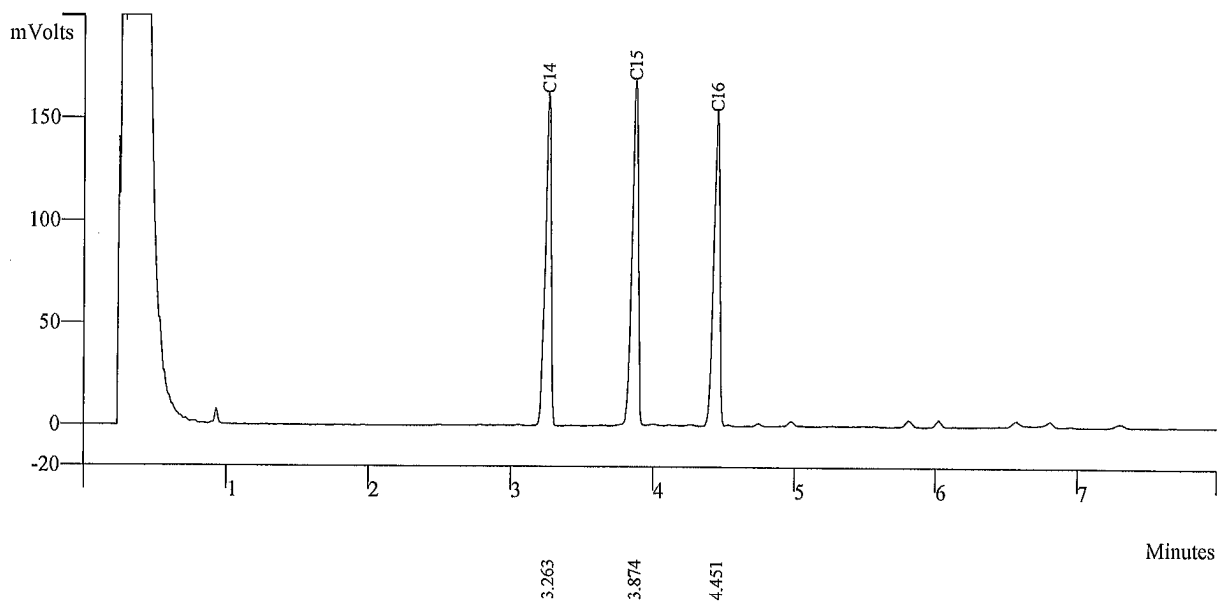

Peak No	Peak Name	Result ()	Ret Time (min)	Peak Area (counts)	Sep. Code	Width 1/2 (sec)
1	C14	0.0000	3.263	458627	BB	2.7
2	C15	0.0000	3.874	506043	VV	2.8
3	C16	0.0000	4.451	460610	VB	2.8
	Totals	0.0000		1425280		



Sample ID: fid std




VARIAN

Operator (Inj): watsamon
Injection Date: 02/08/2025
Calc Date: 02/08/2025
Run Time (min): 7.993
Workstation: GC-LAB
Instrument (Inj):

Run Mode: Calibration
Peak Measurement: Peak Area
Calculation Type: External Std.

e:\sps2025\fidstd002.run

A = FID 10 V RESULTS

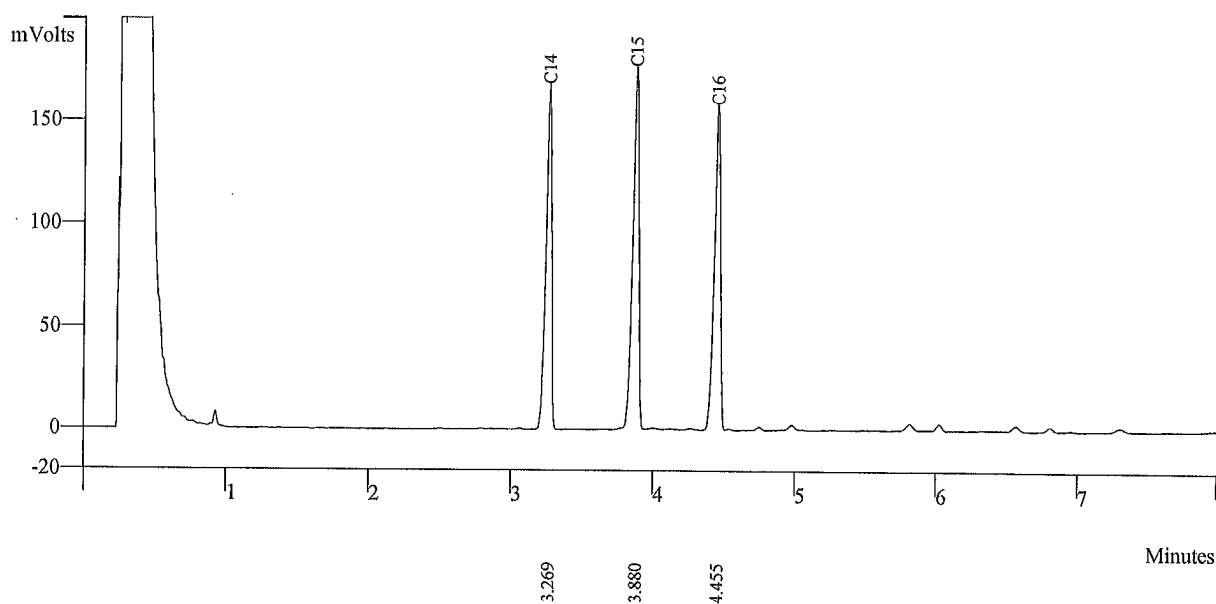

Peak No	Peak Name	Result ()	Ret Time (min)	Peak Area (counts)	Sep. Code	Width 1/2 (sec)
1	C14	0.0000	3.269	472338	BB	2.6
2	C15	0.0000	3.880	520497	VV	2.7
3	C16	0.0000	4.455	471916	VB	2.8
	Totals	0.0000		1464751		



Sample ID: fid std



Operator (Inj): watsamon

Injection Date: 02/08/2025

Calc Date: 02/08/2025

Run Time (min): 7.993

Workstation: GC-LAB

Instrument (Inj):

VARIAN


Run Mode: Calibration

Peak Measurement: Peak Area

Calculation Type: External Std.

e:\sps2025\fidstd003.run

A = FID 10 V RESULTS

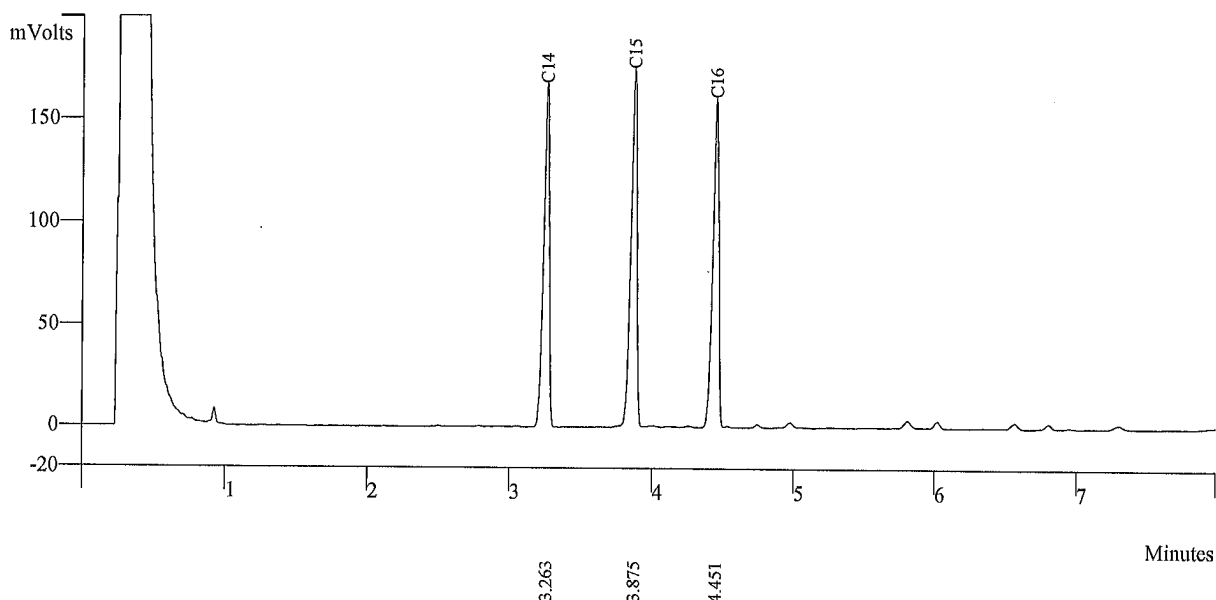

Peak No	Peak Name	Result ()	Ret Time (min)	Peak Area (counts)	Sep. Code	Width 1/2 (sec)
1	C14	0.0000	3.263	469265	BB	2.6
2	C15	0.0000	3.875	522154	VV	2.8
3	C16	0.0000	4.451	478526	VB	2.8
	Totals	0.0000		1469945		



Sample ID: fid std



VARIAN

Operator (Inj): watsamon

Injection Date: 02/08/2025

Calc Date: 02/08/2025

Run Time (min): 7.993

Workstation: GC-LAB

Instrument (Inj):


Run Mode: Calibration

Peak Measurement: Peak Area

Calculation Type: External Std.

e:\sps2025\fidstd004.run

A = FID 10 V RESULTS

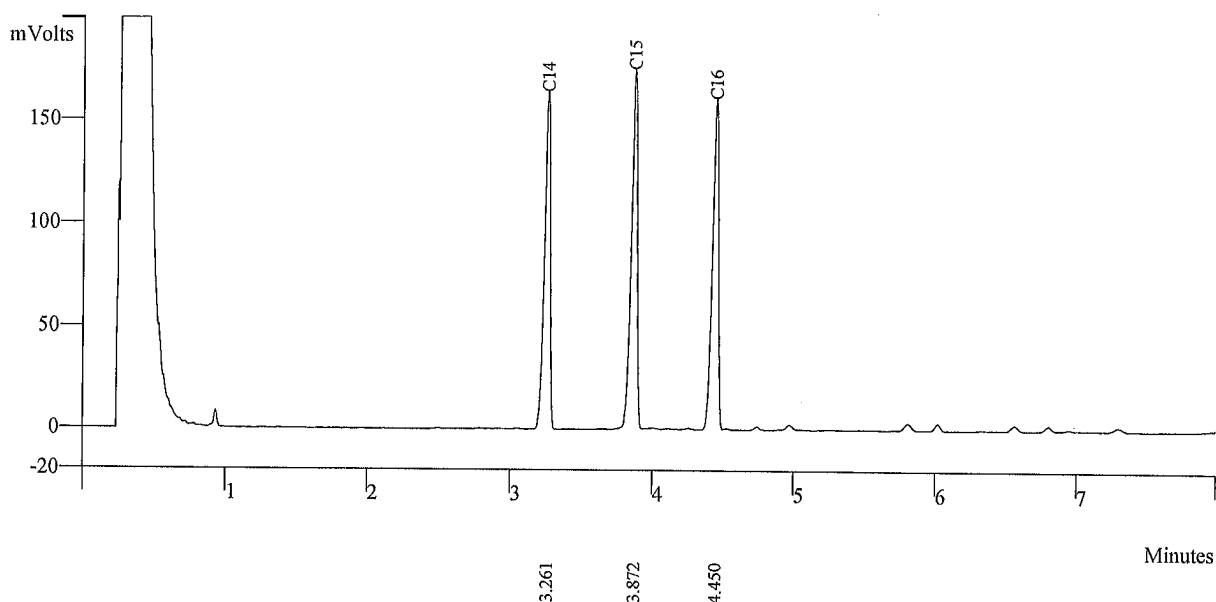

Peak No	Peak Name	Result ()	Ret Time (min)	Peak Area (counts)	Sep. Code	Width 1/2 (sec)
1	C14	0.0000	3.261	468907	BB	2.7
2	C15	0.0000	3.872	521664	VV	2.8
3	C16	0.0000	4.450	478772	VB	2.8
Totals		0.0000		1469343		



Sample ID: **fid std**



Operator (Inj): **watsamon**

Injection Date: **02/08/2025**

Calc Date: **02/08/2025**

Run Time (min): **7.993**

Workstation: **GC-LAB**

Instrument (Inj):

VARIAN


Run Mode: **Calibration**

Peak Measurement: **Peak Area**

Calculation Type: **External Std.**

e:\sps2025\fidstd005.run

A = FID 10 V RESULTS

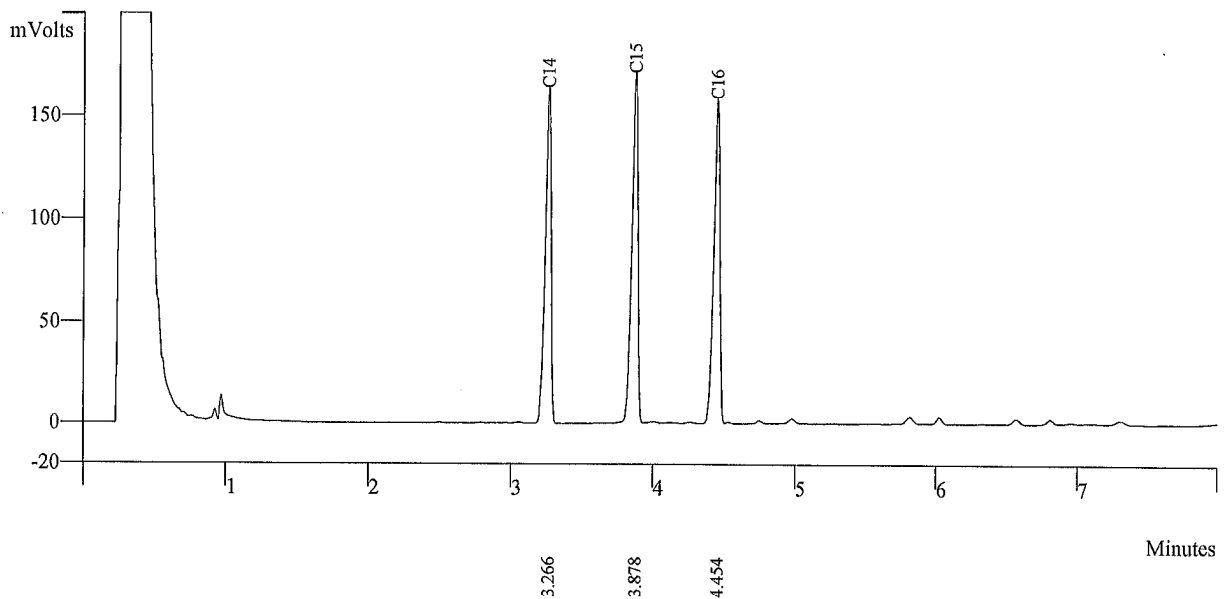


Peak No	Peak Name	Result ()	Ret Time (min)	Peak Area (counts)	Sep. Code	Width 1/2 (sec)
1	C14	0.0000	3.266	459351	BB	2.6
2	C15	0.0000	3.878	509340	VV	2.8
3	C16	0.0000	4.454	468353	VB	2.8
	Totals	0.0000		1437044		



C14

External Standard Analysis
Curve Type: Linear
Origin: Force
 $y = +1.552325e+004x$


Resp. Fact. RSD: 1.347%
Coeff. Det.(r²): 0.999130

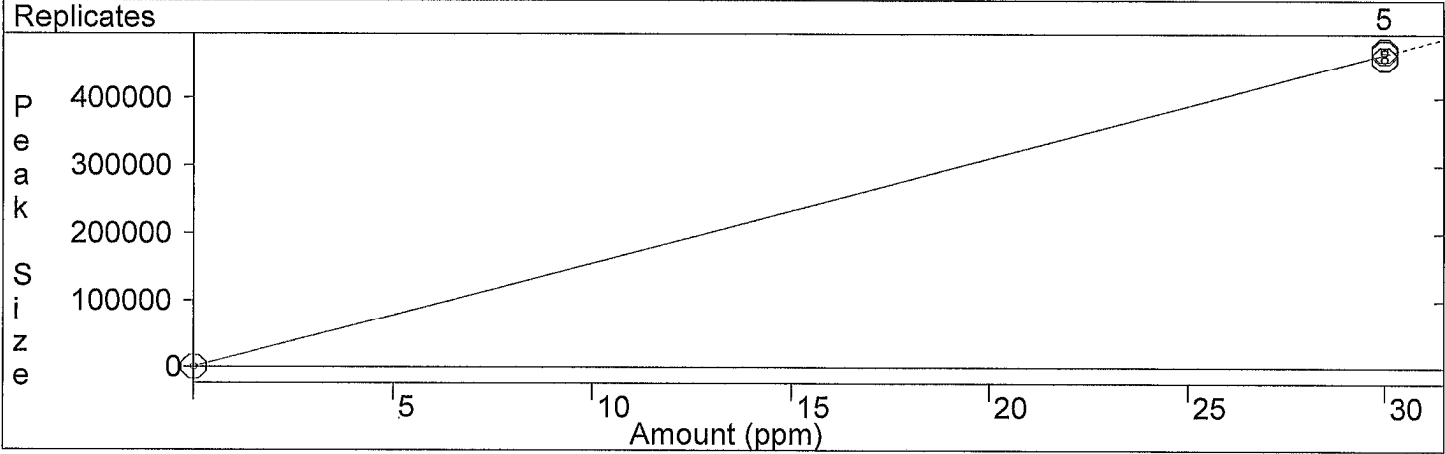

C15

External Standard Analysis
Curve Type: Linear
Origin: Force
 $y = +1.719798e+004x$


Resp. Fact. RSD: 1.481%
Coeff. Det.(r²): 0.998948

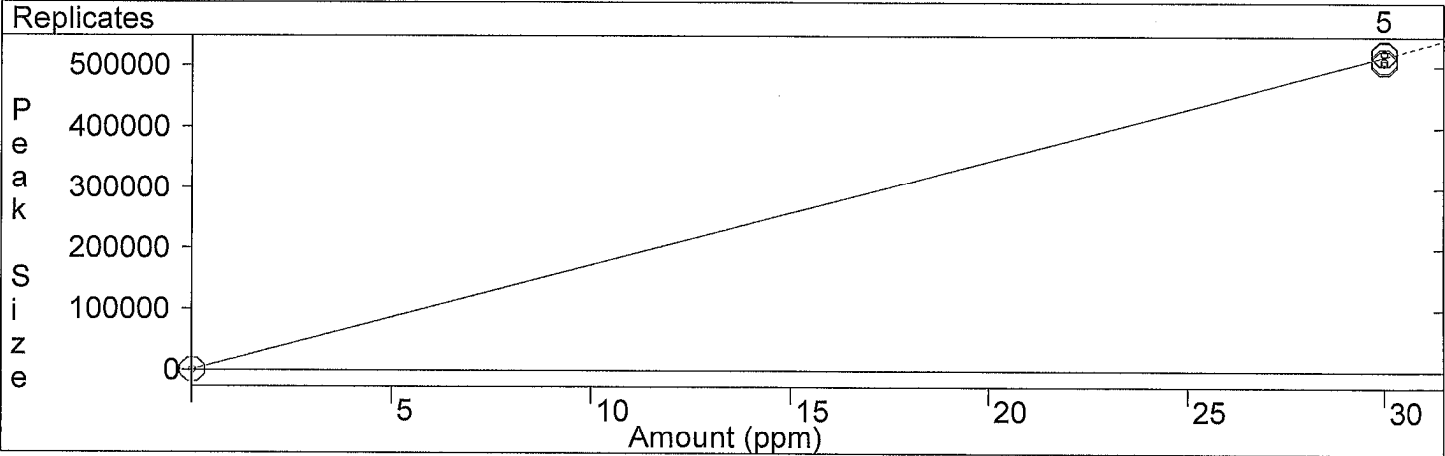

C16

External Standard Analysis
Curve Type: Linear
Origin: Force
 $y = +1.572118e+004x$

Resp. Fact. RSD: 1.611%
Coeff. Det.(r²): 0.998756

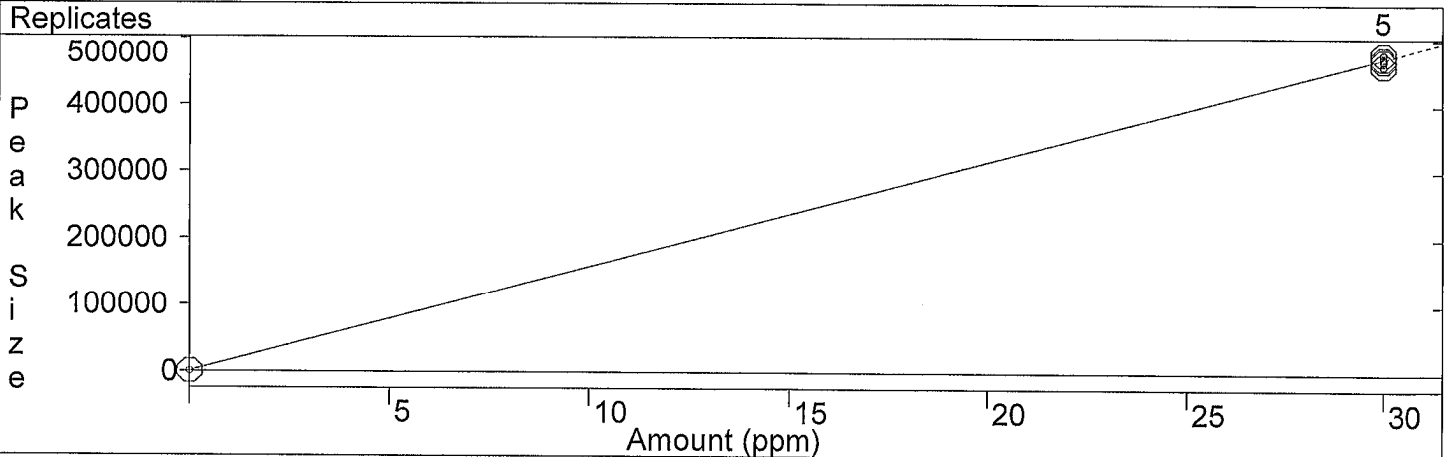

CERTIFICATE

This is to certify, that

Somchai Pohthongkham

has participated the course


Basic GC and Sampler training

Date: ***24 – 27 May 2004***

Location: ***Middelburg***

Instructor: ***W.J. Buys***

Signature instructor:

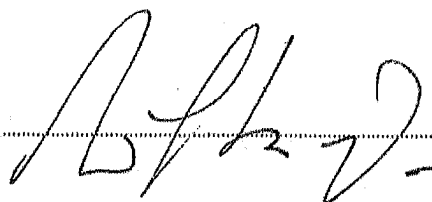

VARIAN

Varian Analytical Instruments
Varian Chrompack International BV
Herculesweg 8
P.O. Box 8033
4330 EA Middelburg
The Netherlands

Tel.: +31 118 671000
Fax: +31 118 633118

www.varianinc.com



WK Electric Co., Ltd.



68/242 Moo 5, Sawaipracharaj Rd., Tumbol Ladsawai, Amphur Lamlukka, Pathumthani 12150

Tel. +66 2993 4773, +66 2153 7132-3 Fax. +66 2994 5509 E-mail : wk.calibrations@gmail.com www.wk-etc.com

Certificate of Calibration

Certificate No.: WK2412-053-1

Page 1 of 2

Customer : THAI UNIQUE CO., LTD.
80-82 Prachathipatai Rd., Bangkhunphrom,
Pranakorn, Bangkok 10200

Instrument	: AMD Flow Meter	Ambient Temperature	: (23 ± 2) °C
Manufacturer	: Agilent Technologies	Humidity	: (50 ± 15) %RH
Model	: G6691A	Received Date	: 4-Dec-24
Serial No.	: MY16470347	Calibrated Date	: 11-Dec-24
Identity No.	: SV-DF-001	Issued Date	: 13-Dec-24
Range	: 0 ml/min to 750 ml/min	Calibrated Location	: In Lab
Resolution	: See to Data		
Calibration Method	: CP-WK-M10		

Reference standard instruments :

Instrument	Serial No.	Certificate No.	Due Date	Traceability to
Flow Calibrator	140215-134	L202304114-001	18-Apr-25	MIT
Primary Flow Calibrator	1107-S	WK2405-049-5	22-May-25	WK Electric Co., Ltd.

MIT : Miracle International Technology Co., Ltd.

This result calibrate was found accurate as shown on date place of calibrate only

This certificate is traceability to the International System of Unit (SI)

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence approximately 95%

Calibrated by : Mr.Thippatai Mungpungklang

Approved by :

Ms. Budsagorn Patcha

Authorized Signatory

This certificate may not be reproduced except in full unless permission for the reproduction has been obtained in writing from the laboratory.



Measuretronix Limited
2425/2 Lat Phrao Road, Saphan Song
Wangthonglang, Bangkok 10310, Thailand
Phone : 0-2514-1000, 0-2514-1234
Fax : 0-2514-0001, 0-2514-0003
Website : www.measuretronix.com



Certificate of Calibration

Certificate Number : LF25-0305
Equipment : Thermometer
Manufacturer : Fluke
Model : 51
Serial Number : 5910857
Asset Number : 5910857
Customer : Thai Unique Co., Ltd.
80-82 Prachathipatai Road,
Bangkhunphrom, Pranakorn,
Bangkok 10200
Date of Calibrate : 6-Jun-2025
Date of Issue : 6-Jun-2025

This calibration certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI).

This calibration certificate applies only to the item identified and shall not be reproduced other than in full, without specific written approved by Measuretronix Cal-Lab. Calibration certificates without signature are not valid.

The measurements marked with an asterisk () in this certificate are outside our range of accreditation. They have been included for completeness.*

The Calibration interval (Cal.Due) is the responsibility of the end user.

Calibrated by

Samak

Mr. Samak Uaonkaonoi
Metrology Technician

Approved by

Juthamas Sukhathainirun

Miss Juthamas Sukhathainirun
Cal-Lab Manager



Agilent Technologies

Certificate of Analysis

FID-TCD Performance Evaluation Sample Kit

Agilent Part
Number: 5080-8842, 18710-60170

Sample Lot
Number: 0006750304

This analytical reference material was manufactured and verified in accordance with an ISO 9001 registered quality system, and the analyte concentrations were verified by an ISO 17025 accredited laboratory. The certified value for each analyte was determined gravimetrically.

Concentrations:

n-tetradecane	0.218 g/L ($\pm 0.5\%$)	0.033 w/w %
n-pentadecane	0.218 g/L ($\pm 0.5\%$)	0.033 w/w %
n-hexadecane	0.218 g/L ($\pm 0.5\%$)	0.033 w/w %

Solvent: hexane


Calibrated Class A glassware and clean bottles were used in the manufacture of this standard. Balances used in the manufacture of this standard are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z-540-1 and ISO 9001.

Purities:

n-tetradecane	99.6%
n-pentadecane	99%
n-hexadecane	99.5%
hexane	99%

Typical Analytical Spectrum or Chromatography

GC Chromatography – n-tetradecane, n-pentadecane, and n-hexadecane in hexane

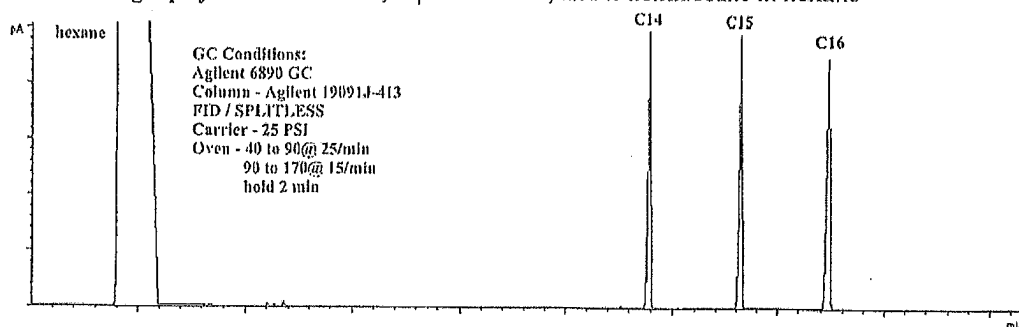

Date of release: 30 June 2023

Date of expiration: 31 July 2025

Monica Bourgeois
Monica Bourgeois
QMS Representative

GC Clarus 600/680 Preventive Maintenance (PM)

Company Name:	S.P.S. Consulting Service Co.,Ltd		
Address (Instrument Location):	7 Soi Phaholyothin 24 Phaholyothin Road, Jompol, Chatuchak, Bangkok, 10900.		
Serial Number:	680S14042502	Service Tag:	N68APSSFEMP
Customer Name (if applicable):	Ms.Naruecha	PM number:	1 of 2
Service Engineer Name:	Monchai Kitcharoenkeat	Service Order Number:	WO-11858723
Date PM Performed: (DD-MMM-YYYY)	13-Feb-2026	Next PM Due Date: (DD-MMM-YYYY)	13-Aug-2026

Part Number	Release	Publication Date	 PerkinElmer®
TH09370070	C	August 2016	

Scope

The purpose of this PM is to ensure the continued functionality of the Clarus 600 and Clarus 680 GC by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer. The customer should save their method before the PM begins.

General Instructions:

The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM. Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files. The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer. Update the PM sticker and instrument logbook as required.

Copyright Information

This document contains proprietary information that is protected by copyright. All rights are reserved. No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of Perkin Elmer, Inc. **Copyright © 2013 PerkinElmer, Inc.**

Trademarks

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners. **Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no Warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.** PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

Component List

Component / Specific Model	Serial #	Software Version	Configuration Notes
Clarus680	680S14042502	Totalchrom6.3.2	PSS, PSS, FID,
Clarus SQ8T	648N4050804	Turbomass 6.4	
AtomX	US14113002	Tekma AtomX	

Parts Lists

Additional Tools Required for PM				
Part Number (if applicable)	Description	Quantity	Serial #	Calibration Due Date (MM/YY)
N/A				
Additional Reagents and Standards Required for PM				
Part Number (if applicable)	Description	Quantity	Batch/Lot #	Expiration Date (MM/YY)
N/A				

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. General:

- ☒ Review the instrument performance with the customer and document any recent problems.

- ☒ Check incoming AC line voltage for proper levels and grounding.

L-N 220 Volt

L-G 220 Volt

N-G 0.46 Volt

**Neutral to ground not more than 0.5 volts peak to peak*

- ☒ Inspect all gas line filters and traps; Replace if necessary with customer supplied spares.

Carrier gas ☒ Helium ☐ Nitrogen ☐ Hydrogen

Moisture level ☒ Good ☐ Need to replace ☐ Other _____

Detector gas ☒ Air Zero ☒ Hydrogen ☐ Nitrogen ☐ Helium

Moisture level ☒ Good ☐ Need to replace ☐ Other _____

- ☒ Inspect the customer log book and make any appropriate PM entries.

- ☒ Leak check all fittings from the gas source to instrument.

Gas leakage ☒ Pass ☐ Fail Comment _____

- ☒ Perform general inspection of system for cleanliness.

- ☒ Inspect for functional and clean electronic cooling and oven vent fans

Electronic cooling fan ☒ Yes ☐ No

Oven cooling fan ☒ Yes ☐ No

2. Electronic :

- ☒ Check oven temperature. Calibrate if necessary.

Oven temperature set point 150 °C ☒ Pass ☐ Fail

- ☐ Check sub-ambient option. (If installed).

Oven temperature set point 5 °C ☐ Pass ☐ Fail

- ☒ Perform routine maintenance on detector/injector. Replace parts as necessary with customer supplied spares.

- ☒ Check flows, including split flows if applicable. Calibrate if necessary.

Carrier flow	Pass
Split flow	Pass
- ☒ Check detector gas flows and adjust if necessary.

Detector flow	Pass
---------------	------
- ☒ Autosampler installed ☒ Yes ☐ No

Check autosampler sensor for wear and replace if necessary.	
Vial sensor	Pass
Door sensor	Pass
Tower sensor	Pass
Plunger sensor	Pass
Elevator sensor	Pass
- ☒ Remove syringe, manually flush. Replace with customer supplied spare if necessary.
- ☒ Check firmware version. Upgrade to current levels if necessary.

Firmware version	<u>6.5</u>
------------------	------------
- ☒ Measure all accessible power supply voltages.

5 Volt	Pass
+15 Volt	Pass
-15 Volt	Pass
24 Volt	Pass
- ☒ Record all detector voltage signal.

Detector Channel A	<u>0.87</u>	mV.
Detector Channel B	<u>NA</u>	mV.

3. Diagnostics Tests:

- ☒ Run instrument diagnostics.

☒ BRAM	Pass
☒ EPROM	Pass
- ☒ Run Autosampler diagnostics.

☒ BRAM	Pass
☒ EPROM	Pass

4. Review:

- ☒ Review with the customer PM work performed.
- ☒ Review with the customer routine maintenance procedures.
- ☒ Discuss recommended customer-supplied materials to have on hand
- ☒ Attach PM sticker.
- ☒ Update Logbook.

Additional Comments

Additional Comments Regarding the PM

Review

<i>The preventive maintenance checks and if applicable performance tests for Clarus600/680 GC have been completed.</i>	
<i>This Clarus600/680 GC</i>	<i>Pass</i>
<i>the preventive maintenance.</i>	
Review of Preventive Maintenance:	
Authorized PerkinElmer Representative: Monchai Kitcharoenkeat	Date: 13-Feb-2026 (DD-MMM-YYYY)
Authorized Customer Representative: Ms.Naruecha	Date: 13-Feb-2026 (DD-MMM-YYYY)