ภาคผนวกที่ 4

เอกสารสอบเทียบความถูกต้องของเครื่องมือตรวจวัดคุณภาพสิ่งแวดล้อม

ลำดับที่ 1 คุณภาพอากาศในบรรยากาศ

ลำดับที่ 2 คุณภาพอากาศจากแหล่งกำเนิด

ลำดับที่ 3 ระดับเสียงในบรรยากาศโดยทั่วไป

ลำดับที่ 4 คุณภาพน้ำทิ้ง

ลำดับที่ 5 ระดับเสียงในสถานประกอบการ

ลำดับที่ 6 ปริมาณเสียงสะสมที่ตัวพนักงานเฉลี่ยตลอดระยะเวลาการทำงาน

ลำดับที่ 7 ระดับความร้อนในสถานประกอบการ

ลำดับที่ 8 คุณภาพอากาศในสถานประกอบการ

ตารางสรุปรายการเอกสารการสอบเทียบความถูกต้องของเครื่องมือตรวจวัด

รายการตรวจวัด	เครื่องมือเก็บตัวอย่าง	เครื่องมือตรวจวิเคราะห์
	ชื่อเครื่องมือ	ชื่อเครื่องมือ
1. คุณภาพอากาศในบรรยากาศ - Total Suspended Particulate (TSP)	- High Volume Air Sampler - Rec No. Blower No. R14, R15, R16	- Digital Balance
- Particulate Matter less than 10 µm (PM_{10})	- High Volume Air Sampler - Rec No. Blower No. R12, R14, R13, R16	- Digital Balance
- Nitrogen Dioxide	- $NO/NO_x/NO_2$ Analyzer No. R03, R05, R10, R11	- $NO/NO_x/NO_2$ Analyzer No. R03, R05, R10, R11
- Ethylene	- Mass Flow Meter	- GC/MS
- Propylene	- Mass Flow Meter	- GC/MS
2. คุณภาพอากาศจากปล่องระบาย - Total Suspended Particulate	- Console No. R04, B05 - Pitot Tube No. B24	- Digital Balance
- Oxides of Nitrogen	- Vacuum Gauge	- Spectrophotometer
- Carbon Monoxide	- Personal Pump SKC No. R21 - Rotameter No. H-R03	- CO Analyzer No. R02
- Hexene-1	- Personal Pump SKC No. R21 - Rotameter No. H-R03	- GC/MS
3. ระดับเสียงทั่วไป – L_{eq} 1 hr, L_{eq} 24 hr, L_{max} , L_{dn} และ L_{90}	- Acoustic Calibrator - Sound Level Meter Aco – R07, R09, R15, R22 CN-B06, B07	–
4. คุณภาพน้ำ - pH	–	- pH Meter
- Temperature	–	- Thermometer
- Total Suspended Solids	–	- Digital Balance
- Total Dissolved Solids	–	- Digital Balance
- BOD_5	–	- BOD Analyzer
- COD	–	- COD Reactor
- Grease & Oil	–	- Digital Balance
- Total Solids	–	- Digital Balance

ตารางสรุปรายการเอกสารการสอบเทียบความถูกต้องของเครื่องมือตรวจวัด

รายการตรวจวัด	เครื่องมือเก็บตัวอย่าง	เครื่องมือตรวจวิเคราะห์
	ชื่อเครื่องมือ	ชื่อเครื่องมือ
5. เสียงในสถานประกอบการ L_{eq} 8 hr, TWA 8 hr, L_{max}	- Acoustic Calibrator - Sound Level Meter ACO- R40, R41, R42, R50, R51, R52	-
6.ปริมาณเสียงสะสมที่ตัวพนักงาน (Noise Dose)	- Sound Calibrator SVANTEK - Acoustic Dose SVANTEK - Noise Dosimeter NO. B01, B02, B03, B04, B05, B06, B07, B08, B09, B10, B11, B12, B13, B14, B15 B16, B17, B18, B19, B20, R02, R03, R06, R13, R15, R20, R22, R26, R27, R35	-
7. ความร้อนในสถานประกอบการ - WBGT	- Heat Stress WBGT Meter No. R30, R31, R32, R33	-
8. คุณภาพอากาศในสถานประกอบการ - Total Dust	- Personal Pump SKC No. B50, B59, B83, R10, R13, R34, R43, R44, R45 - Rotameter No. H-R02, R06, R10	- Digital Balance
- Respirable Dust	- Personal Pump SKC No. B50, B56, B57, B59, B61, B78, B83, R02, R06, R11, R15, R23, R33, R45 - Rotameter No. H-R02, R06, R10	- Digital Balance
- Propylene	- Personal Pump SKC No. B51, B54, B60, B61, R02, R08, R11, R12, R13, R15, R39, R49 - Rotameter No. L-R02, R04, R06, R10	- GC/MS
- Ethylene	- Personal Pump SKC No. B51, R02, R11, R12, R15 - Rotameter No. L-R02, R04, R06, R10	- GC/MS
- Butene-1	- Personal Pump SKC No. B51, B54, R10, R11, R24, R38, R39 - Rotameter No. H-R02, R05, R06	- GC/MS
- Hexene-1	- Personal Pump SKC No. B51, B54, B60, B61, R17, R42 - Rotameter No. H-R02, R06, R10	- GC/MS

ลำดับที่ 1

คุณภาพอากาศในบรรยากาศ

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com.. www.spscon.com

High Volume Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard	Model : TE 5025A	S/N : 3611

Calibration Data				
High Volume Air Sampler Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (ft^3/min)	R^2
B35	B35	04/02/2026	y = 1.154x-3.696	0.996
B36	B36	04/02/2026	y = 1.119x-2.463	0.997
B37	B37	04/02/2026	y = 1.129x-3.721	0.998
B38	B38	02/02/2026	y = 1.182x-2.931	0.997
B39	B39	02/02/2026	y = 1.062x-1.512	0.999
B40	B40	02/02/2026	y = 1.163x-3.556	0.997
B41	B41	02/02/2026	y = 1.116x-1.975	0.996
B42	B42	02/02/2026	y = 1.152x-4.140	0.997
B43	B43	02/02/2026	y = 1.167x-3.646	0.996
B44	B44	02/02/2026	y = 1.178x-4.362	0.999
R01	R01	02/02/2026	y = 1.097x-2.630	0.997
R02	R02	02/02/2026	y = 1.138x-3.218	0.996
R03	R03	02/02/2026	y = 1.133x-3.084	0.998
R04	R04	02/02/2026	y = 1.121x-2.102	0.998
R05	R05	02/02/2026	y = 1.041x+0.894	0.997
R06	R06	02/02/2026	y = 1.075x+0.254	0.997
R07	R07	03/02/2026	y = 1.126x-2.841	0.996
R08	R08	03/02/2026	y = 1.091x-2.104	0.996
R09	R09	03/02/2026	y = 1.065x+0.557	0.996
R10	R10	03/02/2026	y = 1.093x-1.217	0.999
R11	R11	03/02/2026	y = 1.130x-3.938	0.999
R12	R12	05/02/2026	y = 1.164x-2.698	0.997
R13	R13	05/02/2026	y = 1.120x-3.336	0.998
R14	R14	05/02/2026	y = 1.034x+0.445	0.997
R15	R15	05/02/2026	y = 1.076x+0.429	0.998
R16	R16	05/02/2026	y = 1.107x-1.468	0.996
R17	R17	05/02/2026	y = 1.078x-1.668	0.998
R18	R18	05/02/2026	y = 1.160x-5.001	0.997
R19	R19	05/02/2026	y = 1.077x-2.680	0.997
R20	R20	05/02/2026	y = 1.185x-4.839	0.998

Calibrated by : [redacted]	Approved by : [redacted]

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

High Volume PM-10 Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard	Model : TE 5025A	S/N : 3611

Calibration Data				
High Volume PM-10 Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (ft^3/min)	R^2
R01	R01	04/02/2026	y = 1.057x+0.776	0.998
R02	R02	04/02/2026	y = 1.126x-3.479	0.999
R03	R03	04/02/2026	y = 1.099x-1.897	0.996
R04	R04	04/02/2026	y = 1.130x-3.885	0.998
R05	R05	04/02/2026	y = 1.082x-2.165	0.999
R06	R06	04/02/2026	y = 1.132x-2.551	0.997
R07	R07	04/02/2026	y = 1.116x-2.326	0.998
R08	R08	02/02/2026	y = 1.133x-2.404	0.998
R09	R09	02/02/2026	y = 1.063x+0.125	0.998
R10	R10	02/02/2026	y = 1.119x-2.628	0.997
R11	R11	02/02/2026	y = 1.030x+1.723	0.999
R12	R12	02/02/2026	y = 1.035x+0.921	0.999
R13	R13	02/02/2026	y = 1.117x-3.172	0.999
R14	R14	02/02/2026	y = 1.083x-2.455	0.999
R15	R15	02/02/2026	y = 1.103x-3.395	0.997
R16	R16	02/02/2026	y = 1.146x-4.022	0.998
R17	R17	02/02/2026	y = 1.091x-1.835	0.998
R18	R18	02/02/2026	y = 1.104x-4.944	0.998
R19	R19	03/02/2026	y = 1.097x+0.011	0.996
R20	R20	03/02/2026	y = 1.107x-2.872	0.998

Calibrated by : [redacted]	Approved by : [redacted]

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

CALIBRATION REPORT

CHEMILUMINESCENT NO / NO_2 / NO_X ANALYZER

DATE :	01 March 2026	BRAND :	API	MODEL :	200E
NO.	NOX-R03			SERIAL NO.	4410

Calibrator (Dilution System)

Brand	: Teledyne	Model	: 700
Last Cal. Date	: 24 October 2025	Serial No.	: 421

Reference Standard Gas

Standard Gas	: Nitric Oxide (NO)			Cylinder No.	: A00674SV
Certified Date	: 12 March 2025	Expired Date	: 12 March 2028	Cylinder Conc.	: 48.7 ppm

CALIBRATING CONDITION

Pressure	1011	mmbar	Temp.	24.5 °C	% RH 49

CALIBRATION SETTING

Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.10	-	0	-
NO Span	400	400.1	0.025	400.0	1.002
NO_x Span	400	400.3	0.075	400.0	1.006

API Model 200E NO_X Analyzer Check List

Test Values	Observed Value	Units	Nominal Range
RANGE	500	PPB	500 standard
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air
SAMPLE FLOW	510	cc/min	500 ± 50
OZONE FLOW	79	cc/min	80 ± 15
PMT	102.8	mV	-20 - 150
AZERO	94.0	mV	-20 - 150
HVPS	673	V	420 - 900 constant
RCELL TEMP	50.4	°C	50 ± 1
BOX TEMP	29.0	°C	8 - 48
PMT TEMP	7.5	°C	7 ± 2
MOLY TEMP	315.3	°C	315 ± 5
RCELL PRESS	8.3	IN-Hg-A	2 - 10 constant
SAMPLE PRESS	28.5	IN-Hg-A	25 - 30 constant
NO Span Conc	400	PPB	20 - 20,000
NO_x Span Conc	400	PPB	20 - 20,000
NO Slope	1.002	-	1.0 ± 0.3
NO_x Slope	1.006	-	1.0 ± 0.3
NO Offset	0.8	mV	-20 to +150
NO_x Offset	0.3	mV	-20 to 150
Stability at Zero	0.1	PPB	< 0.2
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas

Calibrated by : [redacted]

Approved by : [redacted]

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT

CHEMILUMINESCENT NO / NO_2 / NO_x ANALYZER

DATE :	01 March 2026	BRAND :	API	MODEL :	200E
NO.	NOX-R05			SERIAL NO.	4413

Calibrator (Dilution System)

Brand	: Teledyne	Model	: 700
Last Cal. Date	: 24 October 2025	Serial No.	: 421

Reference Standard Gas

Standard Gas	: Nitric Oxide (NO)			Cylinder No.	: A00674SV
Certified Date	: 12 March 2025	Expired Date	: 12 March 2028	Cylinder Conc.	: 48.7 ppm

CALIBRATING CONDITION

Pressure	1010	mmbar	Temp.	24.6	°C	% RH	49

CALIBRATION SETTING

Span Set Point	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.11	-	0	-
NO Span	400	399.7	-0.075	400.0	0.999
NO_x Span	400	400.2	0.050	400.0	1.003

API Model 200E NO_x Analyzer Check List

Test Values	Observed Value	Units	Nominal Range
RANGE	500	PPB	500 standard
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air
SAMPLE FLOW	505	cc/min	500 ± 50
OZONE FLOW	79	cc/min	80 ± 15
PMT	103.7	mV	-20 - 150
AZERO	94.4	mV	-20 - 150
HVPS	670	V	420 - 900 constant
RCELL TEMP	50.3	°C	50 ± 1
BOX TEMP	29.3	°C	8 - 48
PMT TEMP	7.1	°C	7 ± 2
MOLY TEMP	314.9	°C	315 ± 5
RCELL PRESS	8.3	IN-Hg-A	2 - 10 constant
SAMPLE PRESS	28.6	IN-Hg-A	25 - 30 constant
NO Span Conc	400	PPB	20 - 20,000
NO_x Span Conc	400	PPB	20 - 20,000
NO Slope	0.999	-	1.0 ± 0.3
NO_x Slope	1.003	-	1.0 ± 0.3
NO Offset	1.1	mV	-20 to +150
NO_x Offset	0.7	mV	-20 to 150
Stability at Zero	0.1	PPB	< 0.2
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas

Calibrated by : [redacted]

Approved by : [redacted]

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT

CHEMILUMINESCENT NO / NO_2 / NO_X ANALYZER

DATE :	01 March 2026	BRAND :	API	MODEL :	200E
NO.	NOX-R10			SERIAL NO.	1991

Calibrator (Dilution System)

Brand	: Teledyne	Model	: 700
Last Cal. Date	: 24 October 2025	Serial No.	: 421

Reference Standard Gas

Standard Gas	: Nitric Oxide (NO)			Cylinder No.	: A00674SV
Certified Date	: 12 March 2025	Expired Date	: 12 March 2028	Cylinder Conc.	: 48.7 ppm

CALIBRATING CONDITION

Pressure	1011 mmbar	Temp.	24.5 °C	% RH	48

CALIBRATION SETTING

Span Set Point	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.10	-	0	-
NO Span	400	399.9	-0.025	400.0	1.001
NO_x Span	400	400.1	0.025	400.0	1.004

API Model 200E NO_X Analyzer Check List

Test Values	Observed Value	Units	Nominal Range
RANGE	500	PPB	500 standard
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air
SAMPLE FLOW	504	cc/min	500 ± 50
OZONE FLOW	78	cc/min	80 ± 15
PMT	103.5	mV	-20 - 150
AZERO	93.8	mV	-20 - 150
HVPS	671	V	420 - 900 constant
RCELL TEMP	50.3	°C	50 ± 1
BOX TEMP	29.1	°C	8 - 48
PMT TEMP	7.0	°C	7 ± 2
MOLY TEMP	315.1	°C	315 ± 5
RCELL PRESS	8.4	IN-Hg-A	2 - 10 constant
SAMPLE PRESS	28.4	IN-Hg-A	25 - 30 constant
NO Span Conc	400	PPB	20 - 20,000
NO_x Span Conc	400	PPB	20 - 20,000
NO Slope	1.001	-	1.0 ± 0.3
NO_x Slope	1.004	-	1.0 ± 0.3
NO Offset	0.9	mV	-20 to +150
NO_x Offset	0.5	mV	-20 to 150
Stability at Zero	0.1	PPB	< 0.2
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas

Calibrated by : [redacted]

Approved by : [redacted]

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72 Fax : (662) 513-4221, E-mail : sale@spscon.com.. www.spscon.com

CALIBRATION REPORT

CHEMILUMINESCENT NO / NO_2 / NO_x ANALYZER

DATE :	01 March 2026	BRAND :	API	MODEL :	200E
NO.	NOX-R11			SERIAL NO.	2621

Calibrator (Dilution System)

Brand	: Teledyne	Model	: 700
Last Cal. Date	: 24 October 2025	Serial No.	: 421

Reference Standard Gas

Standard Gas	: Nitric Oxide (NO)			Cylinder No.	: A006745V
Certified Date	: 12 March 2025	Expired Date	: 12 March 2028	Cylinder Conc.	: 48.7 ppm

CALIBRATING CONDITION

Pressure	1010	mmbar	Temp.	24.6	°C	% RH	49

CALIBRATION SETTING

Span Set Point	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	-0.10	-	0	-
NO Span	400	399.9	-0.025	400.0	1.001
NO_x Span	400	400.2	0.050	400.0	1.004

API Model 200E NO_x Analyzer Check List

Test Values	Observed Value	Units	Nominal Range
RANGE	500	PPB	500 standard
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air
SAMPLE FLOW	506	cc/min	500 ± 50
OZONE FLOW	79	cc/min	80 ± 15
PMT	103.2	mV	-20 - 150
AZERO	94.1	mV	-20 - 150
HVPS	671	V	420 - 900 constant
RCELL TEMP	50.2	°C	50 ± 1
BOX TEMP	28.9	°C	8 - 48
PMT TEMP	7.1	°C	7 ± 2
MOLY TEMP	314.9	°C	315 ± 5
RCELL PRESS	8.4	IN-Hg-A	2 - 10 constant
SAMPLE PRESS	28.4	IN-Hg-A	25 - 30 constant
NO Span Conc	400	PPB	20 - 20,000
NO_x Span Conc	400	PPB	20 - 20,000
NO Slope	1.001	-	1.0 ± 0.3
NO_x Slope	1.004	-	1.0 ± 0.3
NO Offset	0.9	mV	-20 to +150
NO_x Offset	0.5	mV	-20 to 150
Stability at Zero	0.1	PPB	< 0.2
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas

Calibrated by : [redacted]

Approved by : [redacted]

MIRACLE INTERNATIONAL TECHNOLOGY CO.,LTD
214 Bangwaek Rd. Bangpai Bangkae Bangkok 10160
Tel.: 0-2865-4647-8 Fax: 0-2865-4649 http://www.mit.in.th

NSC-TISI-TIS 17025
CALIBRATION 0052

CALIBRATION CERTIFICATE

Certificate No. : L202511307-0001

Date Issued : 01-Dec-25

Customer	: S.P.S. CONSULTING SERVICE CO., LTD. 7 Soi Phaholyothin 24 Phaholyothin Road., Jompol, Chatuchak, Bangkok 10900
Equipment	: Mass Flow meter
Manufacturer	: Dwyer
Model	: GMF-2101
Serial No.	: -
ID No./Tag No.	: MF01/51
Date Received	: 27-Nov-25
Date Calibrated	: 30-Nov-25
Calibrated by	: Nattawat Laochai

Calibration Method or Calibration Procedure Used

In-house method : CP-34 by comparison against mass flow calibrator.

This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

Result of Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor k = 2, providing a level confidence approximately 95 percent.

This certificate may not be reproduced other than in full except with the prior written approval of the Miracle International Technology Company Limited.

Approved by: [redacted]

CERTIFIED MIT

Certificate No. : L202511307-0001

Ambient Temperature : (25 ± 2)°C

Relative Humidity : (50 ± 15)%RH

Capacity Range : 17 ml/min

Calibration Media : Nitrogen


Type : Mass Flowmeter

Unit Under Calibration Reference Condition : Pressure 101.325 kPa(abs) , 21 °C , Nitrogen

Temperature (° C)	Pressure (kPa)	UUC Reading (ml/min)	STD Reading (ml/min)	Error (ml/min)	Uncertainty (± ml/min)
24.69	101.22	0.00	0.000 *	0.000	0.063
24.44	119.03	3.30	3.358	-0.058	0.14
24.38	118.17	7.30	7.4	-0.10	0.15
24.30	156.08	13.50	13.6	-0.10	0.15
24.25	169.92	17.00	17.1	-0.10	0.18

Error = Unit Under Calibration - Standard

Marked * are not included in the NSC-ONSC accreditation schedule for our laboratory.

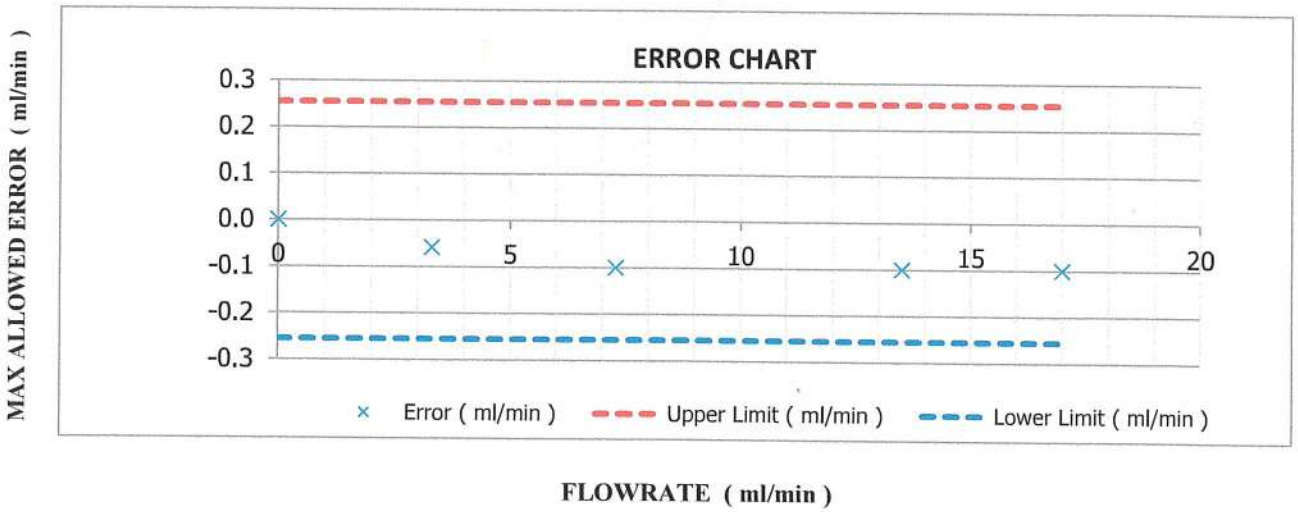

Certificate No. : L202511307-0001

Note : The actual flow rate is determined by the equation :

$$Q_{Meas} = Q_{Ref} \times \frac{P_{Ref}}{P_{Meas}} \times \frac{T_{Meas}}{T_{Ref}}$$

; Q = Flow rate

; P = Absolute pressure

; T = Absolute temperature

; Subscript "Meas" = Measurement condition

; Subscript "Ref" = Reference condition

Condition As-Received : Used Item

The measurment results and statements of conformity with specification only relate to the item calibrated.

Traceability of Certificate :

The International System of Units (SI) through

NIMT Calibration Certificate No. MW-0047-24 for Gas Flow meter Serial No. M5209179B/M5209179A, Due 28-Jun-26

NIMT Calibration Certificate No. MW-0048-24 for Gas Flow meter Serial No. M5209179C/M5209179A, Due 02-Jul-26

End of Certificate

QUALITY CALIBRATION CO.,LTD.
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584
www.qcalibration.com

NSC-TISI-TIS17025
CALIBRATION 0049

CERTIFICATE No : 26M2266
REFERENCE No : 80204-1

Certificate of Calibration

EQUIPMENT	:	DIGITAL BALANCE
MANUFACTURER	:	METTLER TOLEDO
MODEL	:	XS105DU
SERIAL No	:	1126422905
ID No	:	BA 05/50
CONDITION AS RECEIVED	:	USED ITEM
SUBMITTED BY	:	S.P.S. CONSULTING SERVICE CO., LTD. 7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD., JOMPOL, CHATUCHAK, BANGKOK 10900
CALIBRATED BY	:	SUCHAT S.
CALIBRATION DATE	:	05-Mar-26
APPROVED BY	:	[redacted]
ISSUED DATE	:	06-Mar-26
RECEIVED DATE	:	05-Mar-26

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF QUALITY CALIBRATION CO., LTD.

QUALITY CALIBRATION CO.,LTD.
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584
www.qcalibration.com

CERTIFICATE No : 26M2266

Calibration Report

EQUIPMENT	:	DIGITAL BALANCE	**MODEL**	:	XS105DU
MANUFACTURER	:	METTLER TOLEDO	**S/N**	:	1126422905
ID No	:	BA 05/50	**RECEIVED DATE**	:	05-Mar-26
AIR PRESSURE	:	1004mbar ± 1mbar	**CALIBRATION DATE**	:	05-Mar-26
AMBIENT TEMPERATURE	:	25° C ± 1° C	**RELATIVE HUMIDITY**	:	50 %RH ± 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARLITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.
2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	C02250116	28-Jan-27
2) STANDARD WEIGHT	E2	15843	C02250117	29-Jan-27


3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
   - NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL
2. TARE FUNCTION : NORMAL
3. REPEATABILITY OF READING AT 120 g WAS 0.000055 g
4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (± g)
0.00	0.00000	0.00000	0.000065
0.02	0.02000	0.00000	0.000065
0.10	0.10000	0.00000	0.000066
0.20	0.20000	0.00000	0.000066
0.50	0.50001	-0.00001	0.000065
1.00	1.00001	-0.00001	0.000066
2.00	2.00000	0.00000	0.000067
5.00	5.00001	-0.00001	0.000068
10.00	10.00004	-0.00004	0.000070
20.00	20.00006	-0.00006	0.000078
50.00	50.0000	0.0000	0.00012
100.00	100.0002	-0.0002	0.00019
120.00	120.0002	-0.0002	0.00022

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.0000
2	50.0000
3	50.0000
4	50.0000
5	50.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k =2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

[redacted]

GC Clarus 600/680 Preventive Maintenance (PM)

Company Name:	**S.P.S. Consulting Service Co.,Ltd**		
Address (Instrument Location):	7 Soi Phaholyothin24 Phaholyothin Road, Jompol, Chatuchak, Bangkok, 10900.		
Serial Number:	680S14042502	**Service Tag:**	N68APSSFXMP
Customer Name (if applicable):	Ms.Naruecha	**PM number:**	2 of 2
Service Engineer Name:	Monchai Kitcharoenkeat	**Service Order Number:**	WO-06815714
Date PM Performed: (DD-MMM-YYYY)	13-Aug-2025	**Next PM Due Date:** (DD-MMM-YYYY)	13-Feb-2026

Part Number	Release	Publication Date
TH09370070	C	August 2016

Scope

The purpose of this PM is to ensure the continued functionality of the Clarus 600 and Clarus 680 GC by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer. The customer should save their method before the PM begins.

General Instructions:

The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM. Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files. The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer. Update the PM sticker and instrument logbook as required.

Copyright Information

This document contains proprietary information that is protected by copyright. All rights are reserved. No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of Perkin Elmer, Inc. **Copyright © 2013 PerkinElmer, Inc.**

Trademarks

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners. **Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no Warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.** PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

Component List

Component / Specific Model	Serial #	Software Version	Configuration Notes
Clarus680	680S14042502	Totalchrom6.3.2	PSS, PSS, FID,
Clarus SQ8T	648N4050804	Turbomass 6.4	
AtomX	US14113002	Tekma AtomX	

Parts Lists

Additional Tools Required for PM				
Part Number (if applicable)	**Description**	**Quantity**	**Serial #**	**Calibration Due Date (MM/YY)**
N/A				
Additional Reagents and Standards Required for PM				
Part Number (if applicable)	**Description**	**Quantity**	**Batch/Lot #**	**Expiration Date (MM/YY)**
N/A				

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. General:

☑ Review the instrument performance with the customer and document any recent problems.

☑ Check incoming AC line voltage for proper levels and grounding.
L-N 220 Volt
L-G 220 Volt
N-G 0.32 Volt

**Neutral to ground not more than 0.5 volts peak to peak*

☑ Inspect all gas line filters and traps; Replace if necessary with customer supplied spares.
Carrier gas ☑ Helium ☐ Nitrogen ☐ Hydrogen
Moisture level ☑ Good ☐ Need to replace ☐ Other _____

Detector gas ☑ Air Zero ☑ Hydrogen ☐ Nitrogen ☐ Helium
Moisture level ☑ Good ☐ Need to replace ☐ Other _____

☑ Inspect the customer log book and make any appropriate PM entries.

☑ Leak check all fittings from the gas source to instrument.
Gas leakage ☑ Pass ☐ Fail Comment _____

☑ Perform general inspection of system for cleanliness.

☑ Inspect for functional and clean electronic cooling and oven vent fans
Electronic cooling fan ☑ Yes ☐ No
Oven cooling fan ☑ Yes ☐ No

2. Electronic :

☑ Check oven temperature. Calibrate if necessary.
Oven temperature set point 150 ^{0}C ☑ Pass ☐ Fail

☐ Check sub-ambient option. (If installed).
Oven temperature set point 5 ^{0}C ☐ Pass ☐ Fail

☑ Perform routine maintenance on detector/injector. Replace parts as necessary with customer supplied spares.

☑ Check flows, including split flows if applicable. Calibrate if necessary.
Carrier flow Pass
Split flow Pass

☑ Check detector gas flows and adjust if necessary.
Detector flow Pass

☑ Autosampler installed ☑ Yes ☐ No
Check autosampler sensor for wear and replace if necessary.
Vial sensor Pass
Door sensor Pass
Tower sensor Pass
Plunger sensor Pass
Elevator sensor Pass

☑ Remove syringe, manually flush. Replace with customer supplied spare if necessary.

☑ Check firmware version. Upgrade to current levels if necessary.
Firmware version 6.5

☑ Measure all accessible power supply voltages.
5 Volt Pass
+15 Volt Pass
-15 Volt Pass
24 Volt Pass

☑ Record all detector voltage signal.
Detector Channel A 0.98 mV.
Detector Channel B NA mV.

3. Diagnostics Tests:

☑ Run instrument diagnostics.
☑ BRAM Pass
☑ EPROM Pass

☑ Run Autosampler diagnostics.
☑ BRAM Pass
☑ EPROM Pass

4. Review:

☑ Review with the customer PM work performed.
☑ Review with the customer routine maintenance procedures.
☑ Discuss recommended customer-supplied materials to have on hand
☑ Attach PM sticker.
☑ Update Logbook.

Additional Comments

Additional Comments Regarding the PM

Review

The preventive maintenance checks and if applicable performance tests for Clarus600/680 GC have been completed. ***This Clarus600/680 GC*** **Pass** ***the preventive maintenance.***	
Review of Preventive Maintenance:	
Authorized PerkinElmer Representative: Monchai Kitcharoenkeat Monchai	Date: 13-Aug-2025 (DD-MMM-YYYY)
Authorized Customer Representative: Ms.Naruecha Naruecha	Date: 13-Aug-2025 (DD-MMM-YYYY)

GC Clarus 600/680 Preventive Maintenance (PM)

Company Name:	**S.P.S. Consulting Service Co.,Ltd**		
Address (Instrument Location):	7 Soi Phaholyothin24 Phaholyothin Road, Jompol, Chatuchak, Bangkok, 10900.		
Serial Number:	680S14042502	**Service Tag:**	N68APSSFXMP
Customer Name (if applicable):	Ms.Naruecha	**PM number:**	1 of 2
Service Engineer Name:	Monchai Kitcharoenkeat	**Service Order Number:**	WO-11858723
Date PM Performed: (DD-MMM-YYYY)	13-Feb-2026	**Next PM Due Date:** (DD-MMM-YYYY)	13-Aug-2026

Part Number	Release	Publication Date
TH09370070	C	August 2016

Scope

The purpose of this PM is to ensure the continued functionality of the Clarus 600 and Clarus 680 GC by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer. The customer should save their method before the PM begins.

General Instructions:

The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM. Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files. The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer. Update the PM sticker and instrument logbook as required.

Copyright Information

This document contains proprietary information that is protected by copyright. All rights are reserved. No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of Perkin Elmer, Inc. **Copyright © 2013 PerkinElmer, Inc.**

Trademarks

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners. **Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no Warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.** PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

Component List

Component / Specific Model	Serial #	Software Version	Configuration Notes
Clarus680	680S14042502	Totalchrom6.3.2	PSS, PSS, FID,
Clarus SQ8T	648N4050804	Turbomass 6.4	
AtomX	US14113002	Tekma AtomX	

Parts Lists

Additional Tools Required for PM				
Part Number (if applicable)	**Description**	**Quantity**	**Serial #**	**Calibration Due Date (MM/YY)**
N/A				
Additional Reagents and Standards Required for PM				
Part Number (if applicable)	**Description**	**Quantity**	**Batch/Lot #**	**Expiration Date (MM/YY)**
N/A				

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. General:

☑ Review the instrument performance with the customer and document any recent problems.

☑ Check incoming AC line voltage for proper levels and grounding.
L-N 220 Volt
L-G 220 Volt
N-G 0.46 Volt

**Neutral to ground not more than 0.5 volts peak to peak*

☑ Inspect all gas line filters and traps; Replace if necessary with customer supplied spares.
Carrier gas ☑ Helium ☐ Nitrogen ☐ Hydrogen
Moisture level ☑ Good ☐ Need to replace ☐ Other _____

Detector gas ☑ Air Zero ☑ Hydrogen ☐ Nitrogen ☐ Helium
Moisture level ☑ Good ☐ Need to replace ☐ Other _____

☑ Inspect the customer log book and make any appropriate PM entries.

☑ Leak check all fittings from the gas source to instrument.
Gas leakage ☑ Pass ☐ Fail Comment _____

☑ Perform general inspection of system for cleanliness.

☑ Inspect for functional and clean electronic cooling and oven vent fans
Electronic cooling fan ☑ Yes ☐ No
Oven cooling fan ☑ Yes ☐ No

2. Electronic :

☑ Check oven temperature. Calibrate if necessary.
Oven temperature set point 150 ^{0}C ☑ Pass ☐ Fail

☐ Check sub-ambient option. (If installed).
Oven temperature set point 5 ^{0}C ☐ Pass ☐ Fail

☑ Perform routine maintenance on detector/injector. Replace parts as necessary with customer supplied spares.

☑ Check flows, including split flows if applicable. Calibrate if necessary.
Carrier flow Pass
Split flow Pass

☑ Check detector gas flows and adjust if necessary.
Detector flow Pass

☑ Autosampler installed ☑ Yes ☐ No
Check autosampler sensor for wear and replace if necessary.
Vial sensor Pass
Door sensor Pass
Tower sensor Pass
Plunger sensor Pass
Elevator sensor Pass

☑ Remove syringe, manually flush. Replace with customer supplied spare if necessary.

☑ Check firmware version. Upgrade to current levels if necessary.
Firmware version 6.5

☑ Measure all accessible power supply voltages.
5 Volt Pass
+15 Volt Pass
-15 Volt Pass
24 Volt Pass

☑ Record all detector voltage signal.
Detector Channel A 0.87 mV.
Detector Channel B NA mV.

3. Diagnostics Tests:

☑ Run instrument diagnostics.
☑ BRAM Pass
☑ EPROM Pass

☑ Run Autosampler diagnostics.
☑ BRAM Pass
☑ EPROM Pass

4. Review:

☑ Review with the customer PM work performed.
☑ Review with the customer routine maintenance procedures.
☑ Discuss recommended customer-supplied materials to have on hand
☑ Attach PM sticker.
☑ Update Logbook.

Additional Comments

Additional Comments Regarding the PM

Review

The preventive maintenance checks and if applicable performance tests for Clarus600/680 GC have been completed. ***This Clarus600/680 GC*** **Pass** ***the preventive maintenance.***	
Review of Preventive Maintenance:	
Authorized PerkinElmer Representative: Monchai Kitcharoenkeat	Date: 13-Feb-2026 (DD-MMM-YYYY)
Authorized Customer Representative: Ms.Naruecha	Date: 13-Feb-2026 (DD-MMM-YYYY)

ลำดับที่ 2

คุณภาพอากาศจากแหล่งกำเนิด

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com.. www.spscon.com

Console Calibration Report

Calibration Method	Critical Orifices

Calibration Data				
Console Data		Calibration Data		
No.	Serial No.	Date	y	$\Delta H_@$ (mmH_2O)
B01	1563	02/03/2026	0.998	49.85
B02	8002514	02/03/2026	1.003	49.77
B03	1503016	03/03/2026	0.997	49.68
B04	00006659	03/03/2026	0.996	49.82
B05	00007428	02/03/2026	0.999	49.65
R01	1561	03/03/2026	1.002	49.98
R02	8002513	03/03/2026	1.004	49.56
R03	1570	03/03/2026	0.997	49.73
R04	8002519	03/03/2026	0.999	49.80
R05	1503015	02/03/2026	1.003	49.95

Remark : Accept Value of y (test) is $0.97 < y < 1.03$

Accept Value of $\Delta H_@$ (test) is 46.7 ± 6.4 (mmH_2O)

Calibrated by :	Approved by :
[redacted]	[redacted]

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Pitot Tube Calibration Report

Calibration Method	Standard Pitot Tube

Calibration Data					
Pitot Tube Data			Calibration Data		
No.	Type of Pitot	Coefficience of Standard Pitot	Date	Avg. of Cp (test)	
				Side A	Side B
B03	S	0.99	02/02/2026	0.84	0.84
B04	S	0.99	02/02/2026	0.84	0.83
B05	S	0.99	03/02/2026	0.84	0.84
B07	S	0.99	04/02/2026	0.84	0.83
B08	S	0.99	04/02/2026	0.85	0.84
B09	S	0.99	04/02/2026	0.84	0.84
B11	S	0.99	03/02/2026	0.84	0.85
B16	S	0.99	03/02/2026	0.83	0.84
B18	S	0.99	03/02/2026	0.84	0.84
B19	S	0.99	02/02/2026	0.84	0.84
B21	S	0.99	02/02/2026	0.84	0.83
B24	S	0.99	02/02/2026	0.84	0.83
B27	S	0.99	02/02/2026	0.84	0.84
B30	S	0.99	03/02/2026	0.84	0.85
B31	S	0.99	03/02/2026	0.84	0.84
B33	S	0.99	03/02/2026	0.83	0.84
B35	S	0.99	04/02/2026	0.84	0.84

Remark : Accept value of Cp (test) is 0.84 ± 0.01

Calibrated by : [redacted]	Approved by : [redacted]

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com

CLC Accredited ISO/IEC 17025

ilac-MRA

ANAB ANSI National Accreditation Board ACCREDITED ISO/IEC 17025 CALIBRATION AND DIMENSIONAL MEASUREMENT ACDM-2814

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE	:	VACUUM GAUGE
MANUFACTURER	:	HI-LIGHT
MODEL / TYPE	:	N/A
SERIAL NO.	:	N/A[64-220088-1]
CLID. NO.	:	212301419
JOB CONTROL NO.	:	240720076545
CALIBRATION SERVICE	:	☑ IN-LABORATORY ☐ ON-SITE

CUSTOMER : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24 ROAD., JOMPOL,
CHATUCHAK, BANGKOK 10900

DATE OF RECEIVED : 20 July 2024 DATE OF ISSUED : 23 July 2024

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sittipong Pimdee
Calibration Engineer

Approved By : [redacted]
Authorized Signatory
23 July 2024

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q24076545

@clccalibration

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com

CLC Accredited ISO/IEC 17025

ilac-MRA

ANAB ANSI National Accreditation Board ACCREDITED ISO/IEC 17025 CALIBRATION AND DIMENSIONAL MEASUREMENT ACDM-2814

REPORT OF CALIBRATION

FOR

NOMENCLATURE	:	**VACUUM GAUGE**
MANUFACTURER	:	**HI-LIGHT**
MODEL / TYPE	:	**N/A**
SERIAL NO.	:	**N/A[64-220088-1]**
DATE OF CALIBRATION	:	**22 July 2024**
DUE DATE OF CALIBRATION	:	**22 July 2025**

ENVIRONMENT CONDITIONS :

Temperature : (23 ± 2) °C **Relative Humidity : (55 ± 10) %RH**

PROCEDURE USED :

This instrument was calibrated under procedure No. **CLC-CPPP-05** according to **DKD-R 6-1** as calibration guidelines.

The calibration was performed by direct measurement with Document Process Calibrator and Pressure Module which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

Document Process Calibrator, Fluke Model 741B S/N. 8295020 with Pressure Module Model 700PD5 S/N. 89404505.

TRACEABILITY :

The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand). Certificate No. MP-0040-24, Due Date 08 February 2025.

UNCERTAINTY :

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor of $k = 2$. It has been evaluated according to the "Calibration of Pressure Gauges (DKD-R 6-1)" which provides a level of confidence approximately 95%.

@clccalibration

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
ilac-MRA
ANAB ANSI National Accreditation Board ACCREDITED ISO/IEC 17025 CALIBRATION AND DIMENSIONAL MEASUREMENT ACDM-2814

CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment ( ) adjustment

The DUC was exercised by applying a known pressure from its zero to full scale 1 times. Then 2 series of known gauge pressure were applied. The STD reading were recorded and the means value were reported in the table below.

CALIBRATION DATA

CORRECTION OF PRESSURE

DUC Test point	STD Reading (kPa)		Conversion to inHg		Correction (inHg)	
(inHg)	Up	Down	Up	Down	Up	Down
0	0.00	0.00	0.0	0.0	0.0	0.0
-5	-15.58	-15.58	-4.6	-4.6	+0.4	+0.4
-10	-32.51	-32.84	-9.6	-9.7	+0.4	+0.3
-15	-49.44	-49.77	-14.6	-14.7	+0.4	+0.3
-20	-66.70	-66.70	-19.7	-19.7	+0.3	+0.3
-25	-83.63	-83.97	-24.7	-24.8	+0.3	+0.2
-30	-100.90	-100.90	-29.8	-29.8	+0.2	+0.2

Uncertainty of measurement ± 0.2 inHg

Transmitting fluid : Air.

Technical Note. Conversion factor 1 kPa ; 0.2953003 inHg

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 012 Page 43 of 67

This report is valid for the above stated instrument/s only.

End of Certificate

@clccalibration

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter	Model : Defender 510-H	S/N : 136833

Environmental Conditions

Temperature	.	25	± 3	°C
Pressure	.	1010	± 15	mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R^2
R01	SKC	224-PCXR4	602467	01/07/2026	1,000	1,500	2,000	1,002	1,497	2,004	1.002x - 5.096	1.000
R02	SKC	224-PCXR4	626450	01/07/2026	1,000	2,000	3,000	1,001	1,500	2,002	1.000x - 0.064	1.000
R03	SKC	224-PCXR4	691592	03/07/2026	1,000	1,500	2,000	1,004	1,503	2,001	1.005x - 8.854	1.000
R04	SKC	224-PCXR4	691672	03/07/2026	1,000	1,500	2,000	1,005	1,507	1,998	1.000x - 1.981	0.999
R05	SKC	224-PCXR4	798470	03/07/2026	1,000	1,500	2,000	996	1,495	1,994	0.999x - 2.792	1.000
R06	SKC	224-PCXR4	798456	03/07/2026	1,000	1,500	2,000	1,004	1,510	1,997	1.001x - 2.424	0.999
R07	SKC	224-PCXR4	798480	04/07/2026	1,000	1,500	2,000	1,005	1,502	1,996	0.998x + 0.096	1.000
R08	SKC	224-PCXR4	883215	04/07/2026	1,000	1,500	2,000	1,000	1,493	2,004	1.000x - 1.234	1.000
R09	SKC	224-PCXR4	034650	04/07/2026	1,000	1,500	2,000	999	1,512	2,000	1.003x - 5.751	1.000
R10	SKC	224-PCXR4	091765	05/07/2026	1,000	1,500	2,000	997	1,497	2,001	1.002x - 4.225	1.000
R11	SKC	224-PCXR4	091763	05/07/2026	1,000	1,500	2,000	1,003	1,509	1,996	1.002x - 3.706	0.999
R12	SKC	224-PCXR4	091568	05/07/2026	1,000	1,500	2,000	999	1,494	1,998	1.000x - 1.098	1.000
R13	SKC	224-PCXR4	091638	05/07/2026	1,000	1,500	2,000	1,004	1,508	1,997	0.998x + 2.061	1.000
R14	SKC	224-PCXR4	091764	03/07/2026	1,000	1,500	2,000	1,005	1,499	2,005	1.001x - 2.105	1.000
R15	SKC	224-PCXR8	529457	03/07/2026	1,000	1,500	2,000	999	1,496	2,000	1.003x - 7.289	1.000
R16	SKC	224-PCXR8	529643	04/07/2026	1,000	1,500	2,000	1,005	1,504	2,003	1.006x - 9.553	0.999
R17	SKC	224-PCXR8	529645	04/07/2026	1,000	1,500	2,000	999	1,498	2,002	0.999x + 0.124	1.000
R18	SKC	224-PCXR8	566756	04/07/2026	1,000	1,500	2,000	996	1,504	1,997	1.003x - 8.994	1.000
R19	SKC	224-PCXR8	566802	04/07/2026	1,000	1,500	2,000	999	1,492	2,002	0.999x - 2.217	1.000
R20	SKC	224-PCXR8	529089	01/07/2026	1,000	1,500	2,000	997	1,509	1,995	1.002x - 7.432	0.999
R21	SKC	224-PCXR8	665728	04/07/2026	1,000	1,500	2,000	996	1,508	1,996	1.001x - 5.831	1.000
R22	SKC	224-PCXR8	707444	01/07/2026	1,000	1,500	2,000	1,003	1,503	2,005	1.003x - 4.501	1.000
R23	SKC	224-PCXR8	761067	05/07/2026	1,000	1,500	2,000	1,004	1,510	1,999	1.004x - 5.951	0.999
R24	SKC	224-PCXR8	707893	05/07/2026	1,000	1,500	2,000	997	1,508	1,995	1.000x - 4.785	1.000
R25	SKC	224-PCXR8	761052	03/07/2026	1,000	1,500	2,000	1,008	1,495	2,002	0.996x + 4.565	1.000
R26	SKC	224-PCXR8	707956	01/07/2026	1,000	1,500	2,000	1,001	1,496	1,999	0.997x + 1.857	1.000
R27	SKC	224-PCXR8	707398	05/04/2026	1,000	1,500	2,000	1,002	1,502	2,000	1.004x - 7.864	1.000
R28	SKC	224-PCXR8	707481	05/07/2026	1,000	1,500	2,000	1,007	1,507	2,002	1.000x - 1.246	0.999
R29	SKC	224-PCXR8	707402	05/07/2026	1,000	1,500	2,000	1,004	1,504	2,005	1.002x - 2.456	1.000
R30	SKC	224-PCXR8	093811	04/07/2026	1,000	1,500	2,000	998	1,503	2,004	1.005x - 8.826	1.000
R31	SKC	224-PCXR8	093183	04/07/2026	1,000	1,500	2,000	999	1,499	1,999	1.002x - 3.934	1.000
R32	SKC	224-PCXR8	671950	04/07/2026	1,000	1,500	2,000	1,004	1,502	1,996	1.000x - 2.460	1.000
R33	SKC	224-PCXR4	626254	04/07/2026	1,000	1,500	2,000	999	1,509	2,000	1.006x - 11.522	0.999
R34	SKC	224-PCXR4	626131	04/07/2026	1,000	1,500	2,000	998	1,504	2,002	1.005x - 9.801	1.000
R35	SKC	224-PCXR8	707460	04/07/2026	1,000	1,500	2,000	1,003	1,513	1,997	0.999x + 3.435	1.000
R36	SKC	224-PCXR8	707446	04/07/2026	1,000	1,500	2,000	1,005	1,498	2,004	1.003x - 4.114	1.000
R37	SKC	224-PCXR8	707432	04/07/2026	1,000	1,500	2,000	997	1,508	1,999	1.005x - 11.510	0.999
R38	SKC	224-PCXR8	707349	04/07/2026	1,000	1,500	2,000	1,001	1,501	1,992	0.996x + 4.713	1.000
R39	SKC	224-PCXR8	761095	04/07/2026	1,000	1,500	2,000	1,006	1,502	2,005	1.003x - 6.542	0.999

Calibrated by : [redacted]

Approved by : [redacted]

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Rotameter Calibration Report (For Personal Pump High Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter	Model : Defender 510-H	S/N : 136164

Calibration Data

Rotameter Data			Calibration Data							
No.	Brand	Model	Date	Flow Rate (ml/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R^2
H-B01	Dwyer	VFB-65	02/07/2026	500	1,000	2,000	501.0	1000.6	1997.5	0.998x + 2.483	1.000
H-B02	Dwyer	VFB-65	02/07/2026	500	1,000	2,000	500.2	999.1	1997.0	0.999x + 0.803	1.000
H-B03	Dwyer	VFB-65	02/07/2026	500	1,000	2,000	499.8	1000.5	1998.1	0.998x + 1.218	1.000
H-B04	Dwyer	VFB-65	02/07/2026	500	1,000	2,000	500.5	999.3	1997.4	0.999x + 3.065	0.999
H-B05	Dwyer	VFB-65	02/07/2026	500	1,000	2,000	498.7	999.1	1998.3	1.000x - 0.843	1.000
H-B06	Dwyer	VFB-65	02/07/2026	500	1,000	2,000	500.4	999.5	2000.0	0.999x + 0.942	1.000
H-B07	Dwyer	VFB-65	03/07/2026	500	1,000	2,000	499.3	999.8	2001.7	1.000x + 2.397	0.999
H-B08	Dwyer	VFB-65	03/07/2026	500	1,000	2,000	499.2	998.7	1999.4	1.001x - 1.249	1.000
H-B09	Dwyer	VFB-65	03/07/2026	500	1,000	2,000	500.4	999.4	1997.3	0.999x + 1.010	1.000
H-B10	Dwyer	VFB-65	03/07/2026	500	1,000	2,000	499.3	999.0	1997.0	0.998x + 0.297	1.000

Calibrated by : [redacted]

Approved by : [redacted]

QUALITY CALIBRATION CO.,LTD.
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584
www.qcalibration.com

NSC-TISI-TIS17025
CALIBRATION 0049

CERTIFICATE No : 26M2266
REFERENCE No : 80204-1

Certificate of Calibration

EQUIPMENT	:	DIGITAL BALANCE
MANUFACTURER	:	METTLER TOLEDO
MODEL	:	XS105DU
SERIAL No	:	1126422905
ID No	:	BA 05/50
CONDITION AS RECEIVED	:	USED ITEM
SUBMITTED BY	:	S.P.S. CONSULTING SERVICE CO., LTD. 7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD., JOMPOL, CHATUCHAK, BANGKOK 10900
CALIBRATED BY	:	SUCHAT S.
CALIBRATION DATE	:	05-Mar-26
APPROVED BY	:	[redacted]
ISSUED DATE	:	06-Mar-26
RECEIVED DATE	:	05-Mar-26

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF QUALITY CALIBRATION CO., LTD.

QUALITY CALIBRATION CO.,LTD.
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584
www.qcalibration.com

CERTIFICATE No : 26M2266

Calibration Report

EQUIPMENT	:	DIGITAL BALANCE	**MODEL**	:	XS105DU
MANUFACTURER	:	METTLER TOLEDO	**S/N**	:	1126422905
ID No	:	BA 05/50	**RECEIVED DATE**	:	05-Mar-26
AIR PRESSURE	:	1004mbar ± 1mbar	**CALIBRATION DATE**	:	05-Mar-26
AMBIENT TEMPERATURE	:	25° C ± 1° C	**RELATIVE HUMIDITY**	:	50 %RH ± 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARLITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.
2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	C02250116	28-Jan-27
2) STANDARD WEIGHT	E2	15843	C02250117	29-Jan-27


3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
   - NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL
2. TARE FUNCTION : NORMAL
3. REPEATABILITY OF READING AT 120 g WAS 0.000055 g
4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (± g)
0.00	0.00000	0.00000	0.000065
0.02	0.02000	0.00000	0.000065
0.10	0.10000	0.00000	0.000066
0.20	0.20000	0.00000	0.000066
0.50	0.50001	-0.00001	0.000065
1.00	1.00001	-0.00001	0.000066
2.00	2.00000	0.00000	0.000067
5.00	5.00001	-0.00001	0.000068
10.00	10.00004	-0.00004	0.000070
20.00	20.00006	-0.00006	0.000078
50.00	50.0000	0.0000	0.00012
100.00	100.0002	-0.0002	0.00019
120.00	120.0002	-0.0002	0.00022

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.0000
2	50.0000
3	50.0000
4	50.0000
5	50.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k =2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

[redacted]

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

NSC-TISI-TIS 17025
CALIBRATION 0394

Calibration Certificate

Equipment :	UV-VIS SPECTROPHOTOMETER
Manufacturer :	PERKINELMER
Model :	LAMBDA 25
Serial No.:	501S14123010
ID No.:	SP03/58
Calibration Mode :	WAVELENGTH ACCURACY PHOTOMETRIC ACCURACY STRAY LIGHT
Condition As Found :	GOOD
Customer :	S.P.S CONSULTING SERVICE CO., LTD. 7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN ROAD, CHOMPHON SUB-DISTRICT, CHATUCHAK DISTRICT, BANGKOK PROVINCE 10900 THAILAND.
Location :	ORGANIC LABORATORY IV
Ambient Temperature :	(22.9 ± 5) °C
Relative Humidity :	(53.7 ± 25) %
Received Date :	22 AUGUST 2025
Calibration Date :	22 AUGUST 2025
Date of Issue :	25 AUGUST 2025

Calibrated by : Nitinun Srihawan

Approved by : ([redacted])

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : SP25026
Job No. : VC68SP0019

Calibration Method :

This instrument was calibrated by using on-site calibration procedure In-house method : CP-SP-01

The calibration procedure to direct measurement wavelength accuracy by using wavelength standard solution, Photometric accuracy by using absorbance standard filter and absorbance standard solution

The calibration procedure used was based on ASTM E275-01,ASTM E925-02

Condition of this result of calibration :

1. Certified reference materials

Material	Ref. type	Cell serial No.	Cert. No.	Due Date
Holmium liquid	RM-HL	29706	126461	24/10/2026
Didymium liquid	RM-DL	28912	126462	24/10/2026
Neutral density filter	RM-1N2N3N	13877	126457	24/10/2026
Potassium dichromate solutions	RM-0204060810	14204	126497	25/10/2026
Potassium Iodide solution	-	KI-0701-001	CI-0185-24	14/05/2026

2. This result of calibration was found accurate as shown on date and place of calibration only.
3. This certificate is traceable to the international system of unit maintained at :
   3.1 The UK National Physical Laboratory (NPL)

Result of calibration : Wavelength Accuracy

(Without adjustment)

Material	Certified Values of Reference Material (nm)	UUC* Reading (nm)	Error (nm)	Uncertainty ± (nm)	*k* Factor
RM-HL	278.13	278.21	0.08	0.16	2.00
	361.25	361.39	0.14	0.16	2.00
	467.82	467.71	-0.11	0.16	2.00
	536.56	536.50	-0.06	0.16	2.00
	640.50	640.36	-0.14	0.16	2.00
RM-DL	740.09	739.85	-0.24	0.16	2.00
	864.94	865.12	0.18	0.16	2.00

UUC* = Unit Under Calibration

Cert. No. : SP25026
Job No. : VC68SP0019

Result of calibration : Photometric Accuracy

Material	Wavelength (nm)	Filter S/N	Nominal Absorbance (A)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	*k* Factor
Neutral Density glass filter	440.0	29381	0.5	0.5443	0.5413	-0.0030	0.0043	2.00
		29914	0.7	0.7484	0.7455	-0.0029	0.0054	2.00
		29360	1.0	1.0527	1.0535	0.0008	0.0032	2.00
	465.0	29381	0.5	0.4948	0.4922	-0.0026	0.0041	2.00
		29914	0.7	0.6906	0.6877	-0.0029	0.0050	2.00
		29360	1.0	0.9695	0.9709	0.0014	0.0031	2.00
	546.1	29381	0.5	0.5090	0.5068	-0.0022	0.0036	2.00
		29914	0.7	0.6985	0.6960	-0.0025	0.0041	2.00
		29360	1.0	0.9814	0.9825	0.0011	0.0031	2.00
	590.0	29381	0.5	0.5375	0.5353	-0.0022	0.0034	2.00
		29914	0.7	0.7256	0.7231	-0.0025	0.0037	2.00
		29360	1.0	1.0213	1.0219	0.0006	0.0032	2.00
	635.0	29381	0.5	0.5223	0.5202	-0.0021	0.0033	2.00
		29914	0.7	0.6927	0.6901	-0.0026	0.0036	2.00
		29360	1.0	0.9744	0.9750	0.0006	0.0032	2.00

UUC* = Unit Under Calibration

[redacted]

Cert. No. : SP25026
Job No. : VC68SP0019
Pages : 4 of 4

Result of calibration : Photometric Accuracy

(Without adjustment)

Material	Wavelength (nm)	Solution (mg/l)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	*k* Factor
Potassium dichromate solutions	235.0	20	0.2415	0.2443	0.0028	0.0101	2.00
		40	0.4866	0.4871	0.0005	0.0115	2.00
		60	0.7415	0.7295	-0.0120	0.0067	2.00
		80	0.9854	0.9844	-0.0010	0.0071	2.00
		100	1.2444	1.2425	-0.0019	0.0073	2.00

UUC* = Unit Under Calibration

Condition of this result of calibration : Spectrophotometer PERKINELMER Model LAMBDA 25 S/N 501S14123010

Resolution of Wavelength Mode 0.1 nm
Resolution of Photometric Mode 0.001 A
Parameter Setting

Measurement Mode	Wavelength, Absorbance
Wavelength Scan	190 nm - 1100 nm
Scanning Speed	7.5 nm/min
Band width(Wavelength)	1.0
Band width(Vis)	1.0
Band width(Uv)	1.0

Stray Light** UUC* Reading at 220.0 nm	
Transimission T(%)	**Absorbance(A)**
0.020	3.7032

**Specific Acceptance :
Transmission ≤ 1.0 T(%), Absorbance ≥ 2.0 A
**Stray light not TISI Accredited

The reported uncertainty is based on a standard uncertainty mutiplied by a coverage factor *k*, providing a level of confidence of approximately 95%

End of Calibration Certificate

GC Clarus 600/680 Preventive Maintenance (PM)

Company Name:	**S.P.S. Consulting Service Co.,Ltd**		
Address (Instrument Location):	7 Soi Phaholyothin24 Phaholyothin Road, Jompol, Chatuchak, Bangkok, 10900.		
Serial Number:	680S14042502	**Service Tag:**	N68APSSFXMP
Customer Name (if applicable):	Ms.Naruecha	**PM number:**	1 of 2
Service Engineer Name:	Monchai Kitcharoenkeat	**Service Order Number:**	WO-11858723
Date PM Performed: (DD-MMM-YYYY)	13-Feb-2026	**Next PM Due Date:** (DD-MMM-YYYY)	13-Aug-2026

Part Number	Release	Publication Date
TH09370070	C	August 2016

Scope

The purpose of this PM is to ensure the continued functionality of the Clarus 600 and Clarus 680 GC by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer. The customer should save their method before the PM begins.

General Instructions:

The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM. Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files. The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer. Update the PM sticker and instrument logbook as required.

Copyright Information

This document contains proprietary information that is protected by copyright. All rights are reserved. No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of Perkin Elmer, Inc. **Copyright © 2013 PerkinElmer, Inc.**

Trademarks

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners. **Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no Warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.** PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

Component List

Component / Specific Model	Serial #	Software Version	Configuration Notes
Clarus680	680S14042502	Totalchrom6.3.2	PSS, PSS, FID,
Clarus SQ8T	648N4050804	Turbomass 6.4	
AtomX	US14113002	Tekma AtomX	

Parts Lists

Additional Tools Required for PM				
Part Number (if applicable)	**Description**	**Quantity**	**Serial #**	**Calibration Due Date (MM/YY)**
N/A				
Additional Reagents and Standards Required for PM				
Part Number (if applicable)	**Description**	**Quantity**	**Batch/Lot #**	**Expiration Date (MM/YY)**
N/A				

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. General:

☑ Review the instrument performance with the customer and document any recent problems.

☑ Check incoming AC line voltage for proper levels and grounding.
L-N 220 Volt
L-G 220 Volt
N-G 0.46 Volt

**Neutral to ground not more than 0.5 volts peak to peak*

☑ Inspect all gas line filters and traps; Replace if necessary with customer supplied spares.
Carrier gas ☑ Helium ☐ Nitrogen ☐ Hydrogen
Moisture level ☑ Good ☐ Need to replace ☐ Other _____

Detector gas ☑ Air Zero ☑ Hydrogen ☐ Nitrogen ☐ Helium
Moisture level ☑ Good ☐ Need to replace ☐ Other _____

☑ Inspect the customer log book and make any appropriate PM entries.

☑ Leak check all fittings from the gas source to instrument.
Gas leakage ☑ Pass ☐ Fail Comment _____

☑ Perform general inspection of system for cleanliness.

☑ Inspect for functional and clean electronic cooling and oven vent fans
Electronic cooling fan ☑ Yes ☐ No
Oven cooling fan ☑ Yes ☐ No

2. Electronic :

☑ Check oven temperature. Calibrate if necessary.
Oven temperature set point 150 ^{0}C ☑ Pass ☐ Fail

☐ Check sub-ambient option. (If installed).
Oven temperature set point 5 ^{0}C ☐ Pass ☐ Fail

☑ Perform routine maintenance on detector/injector. Replace parts as necessary with customer supplied spares.

☑ Check flows, including split flows if applicable. Calibrate if necessary.
Carrier flow Pass
Split flow Pass

☑ Check detector gas flows and adjust if necessary.
Detector flow Pass

☑ Autosampler installed ☑ Yes ☐ No
Check autosampler sensor for wear and replace if necessary.
Vial sensor Pass
Door sensor Pass
Tower sensor Pass
Plunger sensor Pass
Elevator sensor Pass

☑ Remove syringe, manually flush. Replace with customer supplied spare if necessary.

☑ Check firmware version. Upgrade to current levels if necessary.
Firmware version 6.5

☑ Measure all accessible power supply voltages.
5 Volt Pass
+15 Volt Pass
-15 Volt Pass
24 Volt Pass

☑ Record all detector voltage signal.
Detector Channel A 0.87 mV.
Detector Channel B NA mV.

3. Diagnostics Tests:

☑ Run instrument diagnostics.
☑ BRAM Pass
☑ EPROM Pass

☑ Run Autosampler diagnostics.
☑ BRAM Pass
☑ EPROM Pass

4. Review:

☑ Review with the customer PM work performed.
☑ Review with the customer routine maintenance procedures.
☑ Discuss recommended customer-supplied materials to have on hand
☑ Attach PM sticker.
☑ Update Logbook.

Additional Comments

Additional Comments Regarding the PM

Review

The preventive maintenance checks and if applicable performance tests for Clarus600/680 GC have been completed. ***This Clarus600/680 GC*** **Pass** ***the preventive maintenance.***	
Review of Preventive Maintenance:	
Authorized PerkinElmer Representative: Monchai Kitcharoenkeat	Date: 13-Feb-2026 (DD-MMM-YYYY)
Authorized Customer Representative: Ms.Naruecha	Date: 13-Feb-2026 (DD-MMM-YYYY)

ลำดับที่ 3

ระดับเสียงในบรรยากาศโดยทั่วไป

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-69/0204 **MTC No.** EEL. BP. 152/0169

CALIBRATION CERTIFICATE

Submitted by : S.P.S.CONSULTING SERVICE CO.,LTD.

Address : 7 Soi Phaholyothin 24, Phaholyothin Road, Jompol, Chatuchak, Bangkok 10900.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre. Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Sound Calibrator

Manufacturer : ACO

Model : 2127

Serial No. : 130006

Ambient Environment

Temperature : (23 + 3) °C

Relative Humidity : (50 ± 15) %

Ambient Pressure : (101.325 ± 1.500) kPa

Standards used :

1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.
2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.
3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.
4. Digital Multimeter Agilent 34401A S/N MY44005560.
5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.
6. Audio Analyzer Keithley 2015-P S/N 4106495.
7. Condenser Microphone Bruel&Kjaer 4180 S/N 2889871.

Calibration Procedure: CP-102-04 based on IEC 60942-2003; The sound pressure level generated by sound calibrator under test shall be measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 29 Jan. 2026

Date of Calibration : 11 Feb. 2026

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-69/0204 **MTC No.** EEL. BP. 152/0169

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20μPa at 1000 Hz

Acoustic Output in dB re 20μPa, Corrected to Reference Conditions: 101.325 kPa, 23.0 °C and 50 %RH.

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	93.89	-0.11	± 0.10	±0.40 dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	999.9	-0.1	± 1.5	±1.0%

3. Total Distortion

Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	1.90	± 0.50	±3.0%

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Calibrated by : [redacted]

Approved by : [redacted]

Director

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 11 Feb. 2026

Date of Issue : 12 Feb. 2026

Ref : 2011269012900497001

End of Certificate

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Noise R_112/26

Sound Level Meter Calibration Report

Acoustic Calibrator Data

Brand	ACO	Number	AC 03/56
Model	2127	Serial No.	130006
Calibration Range	94 dB, 1000 Hz	Last Calibration	11 February 2026
		Due Date	11 February 2027

Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-R07	ACO	6236	00152080	01 March 2026	93.9	93.9
ACO-R09	ACO	6236	00172035	01 March 2026	93.9	93.9
ACO-R15	ACO	6236	00172062	01 March 2026	93.9	93.9
ACO-R22	ACO	6236	00182010	01 March 2026	93.9	93.9
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.81 ± 0.10 dB	

Calibrated by : [redacted]

Approved by : [redacted]

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Noise R_112-1/26

Sound Level Meter Calibration Report

Acoustic Calibrator Data

Brand	CIRRUS	Number	AC-CR01/63
Model	CR515	Serial No.	92002
Calibration Range	94 dB, 1000 Hz	Last Calibration	11 February 2026
		Due Date	11 February 2027

Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
CR-B06	Cirrus	CR161B	G301151	01 March 2026	94.0	94.0
CR-B07	Cirrus	CR161B	G301167	01 March 2026	94.0	94.0
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.98 ± 0.10 dB	

Calibrated by : [redacted]

Approved by : [redacted]

ลำดับที่ 4

คุณภาพน้ำทิ้ง

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com

CLC Accredited ISO/IEC 17025

ilac-MRA

ANAB ANSI National Accreditation Board ACCREDITED ISO/IEC 17025 CALIBRATION AND DIMENSIONAL MEASUREMENT ACDM-2814

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE	:	pH METER
MANUFACTURER	:	HANNA
MODEL / TYPE	:	HI3512/HI1332/HI7662-T
SERIAL NO.	:	08685754/11250B7M/092806BN[PH04/56]
CLID. NO.	:	272501562
JOB CONTROL NO.	:	250617070523
CALIBRATION SERVICE	:	☑ IN-LABORATORY ☐ ON-SITE

CUSTOMER : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24 ROAD, JOMPOL,
CHATUCHAK, BANGKOK 10900

DATE OF RECEIVED : 17 June 2025 DATE OF ISSUED : 20 June 2025

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sukgasem Seehanart
Wenick Inchaisri
Calibration Engineer

[redacted]

Approved By : [redacted]

Authorized Signatory
20 June 2025

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q25070523

@clccalibration

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com

CLC Accredited ISO/IEC 17025

ilac-MRA

ANAB ANSI National Accreditation Board ACCREDITED ISO/IEC 17025 CALIBRATION AND DIMENSIONAL MEASUREMENT ACDM-2814

REPORT OF CALIBRATION

FOR

NOMENCLATURE	:	**pH METER**
MANUFACTURER	:	**HANNA**
MODEL / TYPE	:	**HI3512/HI1332/HI7662-T**
SERIAL NO.	:	**08685754/11250B7M/092806BN[PH04/56]**
DATE OF CALIBRATION	:	**18 June 2025**

ENVIRONMENT CONDITIONS :

Temperature : **(25 ± 2.5) °C** **Relative Humidity :** **(50 ± 15) % RH**

PROCEDURE USED :

This instrument was calibrated under procedure No. **CLC-CPCH-01** [pH Meter]. The calibration was performed by direct measurement with Certified Reference Material (CRM).

This instrument was calibrated under procedure No. **CLC-CPTH-04** [Temperature] based on **ASTM E 644-04** as calibration guidelines. The calibration was performed by using Calibration Bath, Precision Thermometer and IPRT which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. pH Standard Solution, NIMT TRM CODE TRM-S-2003, TRM CODE TRM-S-2007.
2. pH Standard Solution, Control Company Catalog Number 06664260,11754256, Lot Number CC787362.
3. Calibration Bath, Kambic Model OB-22/2 ULT S/N. 17115653.
4. Precision Thermometer, ASL Model F250 S/N. 1334023800.
5. IPRT, Wika Model CTP5000-250-D S/N. PO00043543-1-10-1.

@clccalibration

TRACEABILITY :

1. The measurements are traceable to International System of Units (SI) , through National Institute of Metrology (Thailand). Lot Number. 080124 , 120124. Due Date 23 January 2026.

2. The measurements are traceable to International System of Units (SI) , through Control Company. Certificate No. 4281-14495731 , Due Date 27 September 2025.

3. The measurements are traceable to International System of Units (SI) , through Calibration Laboratory Co., Ltd. Certificate No. Q24120999, Due Date 26 November 2025.

4. The measurements are traceable to International System of Units (SI) , through Thailand Institute of Scientific and Technological Research (TISTR). Certificate No. PSL-T 1042/67, Due Date 16 October 2025.

5. The measurements are traceable to International System of Units (SI) , through National Institute of Metrology (Thailand). Certificate No. TT-0146-24, Due Date 28 October 2025.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %. It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment ( ) adjustment

The table in the following gives the calibration results and associated measurement uncertainties of pH meter.

CALIBRATION DATA

1. pH METER RESULT @ 25 °C

Standard pH Buffer Solution (pH)	pH Meter Reading (pH)	pH Meter Reading (mV)	Correction (pH)	Uncertainty of pH Measurement (± pH)	*k* Factor
4.003	4.005	168.2	-0.002	0.010	2,00
7.005	7.010	-8.1	-0.005	0.013	2,00
10.015	10.010	-177.7	+0.005	0.014	2,00

Technical Note. Setting function CAL 3 point (4,7,10).

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 015 Page 4 of 68

2. TEMPERATURE RESULT

Immersion depth (mm)	Actual Temperature (°C)	DUC Reading (°C)	Correction (°C)	Uncertainty ± (°C)
100	25.00	25.0	0.00	0.07

Technical Note. Type of sensor : Thermistor

Probe ∅ 3 mm

Materials : Metal Sheath.

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor of $k = 2,00$.

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 015 Page 56 of 68

This report is valid for the above stated instrument/s only.

End of Certificate

CAL
Calibratech Co.,Ltd.
7/106-7 Moo 2, Sukhaprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120
Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech_cal@yahoo.com, calibratech_cal@hotmail.com

NSC-TISI-TIS17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : **68-400046-2** **Page : 1 of 2**

Submitted by : S. P. S Consulting Service Co., Ltd.
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Equipment : Liquid in Glass Thermometer

Manufacturer :	SK	Model :	N/A
Range :	0 °C to 100 °C	Resolution :	1 °C
Serial No. :	N/A	Immersion :	Total
ID No. :	TM21/59		

Environment :

Ambient Temperature :	(23 ± 2)	°C
Relative Humidity :	(50 ± 15)	%
Line Voltage :	(220 ± 22)	VAC

Date of Received : 21 January 2025
Date of Calibration : 24 January 2025
Date of Issue : 24 January 2025
Calibrated by : Chortip Samchusri

Calibration Method : This instrument was calibrated by In-house method comparison technique CAL-M4001 based on ASTM E77-07 by compared with PRT in the liquid bath at the constant controlled temperature.

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Platinum Resistance Thermometer (PRT)

ID No.	Cert. No.	Due Date	Traceability
400001	TT-0023-24	16 Feb 2026	National Institute of Metrology Thailand (NIMT)

2. Standard Digital Thermometer

ID No.	Cert. No.	Due Date	Traceability
400003	23E1866	01 Jun 2025	National Institute of Metrology Thailand (NIMT)
400004	23E1866	01 Jun 2025	National Institute of Metrology Thailand (NIMT)

Approved by : [redacted]
Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This cerificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.

CAL
Calibratech Co.,Ltd.
7/106-7 Moo 2, Sukhaprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120
Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech_cal@yahoo.com, calibratech_cal@hotmail.com

Certificate of Calibration

Certificate No. : 68-400046-2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

Ice point check : UUC* reading 0 ° C Standard reading 0.4429 ° C

Standard Reading (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (±°C)
20.4801	20	0.5	0.31

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2 , providing a level of confidence of approximately 95%

- o0o -

[redacted]

CAL
Calibratech Co.,Ltd.
7/106-7 Moo 2, Sukhaprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120
Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech_cal@yahoo.com, calibratech_cal@hotmail.com

NSC-TISI-TIS17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : **69-400023-2**

Submitted by : S. P. S Consulting Service Co., Ltd.
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Equipment : Liquid in Glass Thermometer

Manufacturer :	SK	Model :	N/A
Range :	0 °C to 100 °C	Resolution :	1 °C
Serial No. :	N/A	Immersion :	Total
ID No. :	TM21/59		

Environment :

Ambient Temperature :	(23 ± 2)	°C
Relative Humidity :	(50 ± 15)	%
Line Voltage :	(220 ± 22)	VAC

Date of Received : 13 January 2026
Date of Calibration : 16 January 2026
Date of Issue : 16 January 2026
Calibrated by : Chortip Samchusri

Calibration Method : This instrument was calibrated by In-house method comparison technique CAL-M4001 based on ASTM E77-07 by compared with PRT in the liquid bath at the constant controlled temperature.

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Platinum Resistance Thermometer (PRT)

ID No.	Cert. No.	Due Date	Traceability
400001	TT-0023-24	16 Feb 2026	National Institute of Metrology Thailand (NIMT)

2. Standard Digital Thermometer

ID No.	Cert. No.	Due Date	Traceability
400003	25E1656	22 May 2027	National Institute of Metrology Thailand (NIMT)
400004	25E1656	22 May 2027	National Institute of Metrology Thailand (NIMT)

Approved by : [redacted]
Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This cerificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.

CAL
Calibratech Co.,Ltd.
7/106-7 Moo 2, Sukhaprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120
Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech_cal@yahoo.com, calibratech_cal@hotmail.com

Certificate of Calibration

Certificate No. : 69-400023-2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

Ice point check : UUC* reading 0 ° C Standard reading 0.4773 ° C

Standard Reading (° C)	UUC Reading (° C)	Correction (° C)	Uncertainty (± ° C)
20.3922	20	0.4	0.31

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2 , providing a level of confidence of approximately 95%

- oOo -

[redacted]

QUALITY CALIBRATION CO.,LTD.
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584
www.qcalibration.com

NSC-TISI-TIS17025
CALIBRATION 0049

CERTIFICATE No : 25M2256
REFERENCE No : 76365-3

Certificate of Calibration

EQUIPMENT	:	DIGITAL BALANCE
MANUFACTURER	:	SARTORIUS
MODEL	:	BSA224S-CW
SERIAL No	:	36591843
ID No	:	BA09/61
CONDITION AS RECEIVED	:	USED ITEM
SUBMITTED BY	:	S.P.S. CONSULTING SERVICE CO., LTD. 7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD., JOMPOL, CHATUCHAK, BANGKOK 10900
CALIBRATED BY	:	ATSAWIN Y.
CALIBRATION DATE	:	07-Mar-25
APPROVED BY	:	[redacted]
ISSUED DATE	:	13-Mar-25
RECEIVED DATE	:	07-Mar-25

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF QUALITY CALIBRATION CO., LTD.

QUALITY CALIBRATION CO.,LTD.
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584
www.qcalibration.com

CERTIFICATE No : 25M2256

Calibration Report

EQUIPMENT	:	DIGITAL BALANCE	**MODEL**	:	BSA224S-CW
MANUFACTURER	:	SARTORIUS	**S/N**	:	36591843
ID No	:	BA09/61	**RECEIVED DATE**	:	07-Mar-25
AIR PRESSURE	:	1009mbar ± 1mbar	**CALIBRATION DATE**	:	07-Mar-25
AMBIENT TEMPERATURE	:	24° C ± 1° C	**RELATIVE HUMIDITY**	:	52 %RH ± 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARLITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.
2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	C02250116	28-Jan-27
2) STANDARD WEIGHT	E2	15843	C02250117	29-Jan-27


3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
   - NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL
2. TARE FUNCTION : NORMAL
3. REPEATABILITY OF READING AT 200 g WAS 0.000071 g
4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (± g)
0.00	0.0000	0.0000	0.00012
0.10	0.1000	0.0000	0.00012
0.20	0.2000	0.0000	0.00012
0.50	0.5000	0.0000	0.00012
1.00	1.0000	0.0000	0.00012
2.00	2.0000	0.0000	0.00012
5.00	5.0000	0.0000	0.00012
10.00	10.0000	0.0000	0.00012
20.00	20.0001	-0.0001	0.00012
50.00	50.0000	0.0000	0.00014
100.00	100.0001	-0.0001	0.00019
200.00	200.0001	-0.0001	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	100.0000
2	100.0000
3	100.0000
4	100.0000
5	100.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k =2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

[redacted]

QUALITY CALIBRATION CO.,LTD.
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584
www.qcalibration.com

NSC-TISI-TIS17025
CALIBRATION 0049

CERTIFICATE No : 26M2268
REFERENCE No : 80204-3

Certificate of Calibration

EQUIPMENT	:	DIGITAL BALANCE
MANUFACTURER	:	SARTORIUS
MODEL	:	BSA224S-CW
SERIAL No	:	36591843
ID No	:	BA 09/61
CONDITION AS RECEIVED	:	USED ITEM
SUBMITTED BY	:	S.P.S. CONSULTING SERVICE CO., LTD. 7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD., JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY	:	SUCHAT S.
CALIBRATION DATE	:	05-Mar-26
APPROVED BY	:	[redacted]
ISSUED DATE	:	06-Mar-26
RECEIVED DATE	:	05-Mar-26

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF QUALITY CALIBRATION CO., LTD.

QUALITY CALIBRATION CO.,LTD.
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584
www.qcalibration.com

Calibration Report

EQUIPMENT	:	DIGITAL BALANCE	**MODEL**	:	BSA224S-CW
MANUFACTURER	:	SARTORIUS	**S/N**	:	36591843
ID No	:	BA 09/61	**RECEIVED DATE**	:	05-Mar-26
AIR PRESSURE	:	1004mbar ± 1mbar	**CALIBRATION DATE**	:	05-Mar-26
AMBIENT TEMPERATURE	:	25° C ± 1° C	**RELATIVE HUMIDITY**	:	50 %RH ± 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARLITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.
2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	C02250116	28-Jan-27
2) STANDARD WEIGHT	E2	15843	C02250117	29-Jan-27


3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
   - NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL
2. TARE FUNCTION : NORMAL
3. REPEATABILITY OF READING AT 200 g WAS 0.000055 g
4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (± g)
0.0	0.0000	0.0000	0.00010
0.1	0.1000	0.0000	0.00011
0.2	0.2000	0.0000	0.00010
0.5	0.5000	0.0000	0.00011
1.0	1.0000	0.0000	0.00011
2.0	2.0000	0.0000	0.00011
5.0	5.0000	0.0000	0.00011
10.0	10.0000	0.0000	0.00011
20.0	20.0001	-0.0001	0.00011
50.0	50.0000	0.0000	0.00013
100.0	100.0001	-0.0001	0.00019
200.0	200.0001	-0.0001	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	100.0000
2	100.0000
3	100.0000
4	100.0000
5	100.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k =2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

[redacted]

Harikul Science Co.,Ltd.
694 Soi Ratchadanivet 24, Pracharatbamphen,
Samsaennok, Huaikhwang, Bangkok 10310
Tel: 0-2274-2456 Fax: 0-2274-2443
Email: info@harikul.com www.harikul.com

CERT.No.: HS-W015C

Certificate of Calibration

Calibration Date :	18 Mar 25	Model	: YSI 5000
Submitted by :	S.P.S CONSULTING SERVICE CO.,LTD	S/N	: 15B100751
	7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol,	Probe	: YSI 5010
	Chatuchak, Bangkok, Thailand 10900	S/N	: 22D100097
		ID NO.	: -
Avg Room Temp :	20 °C	Air Temp ref	: S/N. F8065C26
Avg Water Temp :	20 °C	Barometric ref	: S/N. F8065C26
Air Pressure :	760.00 mmHg	Water Temp ref	: -
Salinity :	0 ppt	ID NO.	HS001
		Technician	: Kittipong M.

Calibration Details

Calibration Point	100% air sat. (@20 °C, DO = 9.09 mg/l)	(status)		(status)
Measurement 1 (mg/l)	9.08	(PASS)	-	-
Measurement 2 (mg/l)	9.08	(PASS)	-	-
Measurement 3 (mg/l)	9.08	(PASS)	-	-
Measurement 4 (mg/l)	9.07	(PASS)	-	-
Measurement 5 (mg/l)	9.07	(PASS)	-	-
Measurement 6 (mg/l)	9.07	(PASS)	-	-
Measurement 7 (mg/l)	9.07	(PASS)	-	-
Measurement 8 (mg/l)	9.07	(PASS)	-	-
Measurement 9 (mg/l)	9.07	(PASS)		-
Measurement 10 (mg/l)	9.07	(PASS)	-	-
Mean Measurement	9.07	mg/l	-	-
Inaccuracy	0.02	mg/l	-	-

Overall Status (PASS)

Manufacturer Specification

Accuracy = +/- 0.02 mg/l

1) This certificate is issued based on the result that are found as shown on date and place of test only.
2) The calibration procedure followed in accordance with Harikul Science Co., Ltd.
3) This result shall not be used for advertising purpose.

[redacted]

(Kittipong Maekwong)

[redacted]

(Natenapha Pisatkunchon)

Harikul Science Co.,Ltd.
694 Soi Ratchadanivet 24, Pracharatbamphen,
Samsaennok, Huaikhwang, Bangkok 10310
Tel: 0-2274-2456 Fax: 0-2274-2443
Email: info@harikul.com www.harikul.com

CERT.No.: HS-X014C

Certificate of Calibration

Calibration Date : 16 March 2026

Submitted by : S.P.S CONSULTING SERVICE CO.,LTD
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol,
Chatuchak, Bangkok, Thailand 10900

Avg Room Temp : 20 °C
Avg Water Temp : 20 °C
Air Pressure : 760.00 mmHg
Salinity : 0 ppt

Model : YSI 5000
S/N : 15B100751
Probe : YSI 5010
S/N : 22D100097
ID NO. :
Air Temp ref : S/N. F8065C26
Barometric ref : S/N. F8065C26
Water Temp ref : -
ID NO. HS001
Technician : Kittipong M.

Calibration Details

Calibration Point	100% air sat. (@20 °C, DO = 9.09 mg/l)	(status)		(status)
Measurement 1 (mg/l)	9.09	(PASS)	-	-
Measurement 2 (mg/l)	9.09	(PASS)	-	-
Measurement 3 (mg/l)	9.09	(PASS)	-	-
Measurement 4 (mg/l)	9.09	(PASS)	-	-
Measurement 5 (mg/l)	9.09	(PASS)	-	-
Measurement 6 (mg/l)	9.08	(PASS)	-	-
Measurement 7 (mg/l)	9.08	(PASS)	-	-
Measurement 8 (mg/l)	9.08	(PASS)	-	-
Measurement 9 (mg/l)	9.08	(PASS)		-
Measurement 10 (mg/l)	9.08	(PASS)	-	-
Mean Measurement	9.09	mg/l	-	-
Inaccuracy	0.00	mg/l	-	-
Overall Status	(PASS)			

Manufacturer Specification

Accuracy = +/- 0.02 mg/l

1) This certificate is issued based on the result that are found as shown on date and place of test only.
2) The calibration procedure followed in accordance with Harikul Science Co., Ltd.
3) This result shall not be used for advertising purpose.

[redacted]
(Kittipong Maekwong)

[redacted]
(Natenapha Pisatkunchon)

QUALITY CALIBRATION CO., LTD.
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584
www.qcalibration.com

CERTIFICATE No : 25T0521
REFERENCE No : 75853-2

Certificate of Calibration

EQUIPMENT	:	COD REACTOR
MANUFACTURER	:	HACH
MODEL	:	DRB 200
SERIAL No	:	15110C0498
ID No	:	CRB 06/59
CONDITION AS RECEIVED	:	USED ITEM
SUBMITTED BY	:	S.P.S. CONSULTING SERVICE CO., LTD. 7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD., JOMPOL, CHATUCHAK, BANGKOK 10900
CALIBRATED BY	:	CHAICHARN CH.
CALIBRATION DATE	:	03-Feb-25
APPROVED BY	:	[redacted]
ISSUED DATE	:	03-Feb-25
RECEIVED DATE	:	15-Jan-25

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF QUALITY CALIBRATION CO., LTD.

QUALITY CALIBRATION CO., LTD.
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 25T0521

Calibration Report

EQUIPMENT	:	COD REACTOR			
MANUFACTURER	:	HACH	**MODEL**	:	DRB 200
ID NUMBER	:	CRB 06/59	**SERIAL NUMBER**	:	15110C0498
RECEIVED DATE	:	15-Jan-25	**CALIBRATION DATE**	:	03-Feb-25
AMBIENT TEMPERATURE	:	23° C ± 1° C	**RELATIVE HUMIDITY**	:	53 %RH ± 10 % RH


CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASURMENT METHOD WITH CALIBRATED THERMOCOUPLE TYPE K UNDER NO LOAD CONDITION. THE THERMOCOUPLES WERE PLACED ON POINTS AND LOCATED AS THE PICTURE .
2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH TC TYPE K	HYDRA 2635A	7301307	24T6467	26-Jun-25

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
   - NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO., LTD.

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

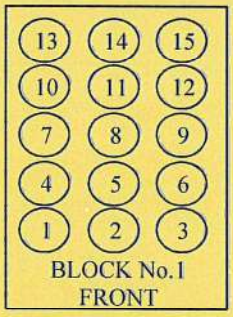



Block No.		1	2
Calibration Point (°C)		150	150
Controller temperature (°C)		145	145
Indicating Temperature		145	145
Measured Temperature (° C) at Spread Locations	1	150.23	150.64
	2	149.73	149.78
	3	150.29	150.29
	4	150.04	150.49
	5	150.09	150.51
	6	150.74	150.67
	7	149.97	150.66
	8	150.76	150.57
	9	150.54	150.51
	10	149.44	149.94
	11	150.12	150.64
	12	149.93	150.33
	13	149.19	149.82
	14	148.96	149.70
	15	149.09	149.79
Uncertainty of Measurement(± °C)		0.88	0.88

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAM
NOTE 2 : LOCATION 10 WAS REFERENCE LOCATION.
NOTE 3 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY M
COVERAGE FACTOR k =2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

[redacted]

QUALITY CALIBRATION CO., LTD.
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584
www.qcalibration.com

CERTIFICATE No : 26T0464
REFERENCE No : 79659-1

Certificate of Calibration

EQUIPMENT	:	COD REACTOR
MANUFACTURER	:	HACH
MODEL	:	DRB 200
SERIAL No	:	15110C0497
ID No	:	DRB 04/59
SUBMITTED BY	:	S.P.S. CONSULTING SERVICE CO., LTD. 7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD., JOMPOL, CHATUCHAK, BANGKOK 10900
CALIBRATED BY	:	SOMCHAI S.
CALIBRATION DATE	:	30-Jan-26
APPROVED BY	:	[redacted]
ISSUED DATE	:	30-Jan-26
RECEIVED DATE	:	30-Jan-26

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF QUALITY CALIBRATION CO., LTD.

QUALITY CALIBRATION CO., LTD.
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 26T0464

Calibration Report

EQUIPMENT	:	COD REACTOR			
MANUFACTURER	:	HACH	**MODEL**	:	DRB 200
ID NUMBER	:	DRB 04/59	**SERIAL NUMBER**	:	15110C0497
RECEIVED DATE	:	30-Jan-26	**CALIBRATION DATE**	:	30-Jan-26
AMBIENT TEMPERATURE	:	23° C ± 1° C	**RELATIVE HUMIDITY**	:	54 %RH ± 10 % RH


CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASURMENT METHOD WITH CALIBRATED THERMOCOUPLE TYPE K UNDER NO LOAD CONDITION. THE THERMOCOUPLES WERE PLACED ON POINTS AND LOCATED AS THE PICTURE .
2. REFERENCE STANDARD INSTRUMENTS :-

	INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1)	DATA LOGGER WITH TC TYPE K	HYDRA 2635A	6849323	25T5342	18-Jun-26

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
   - NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO., LTD.

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

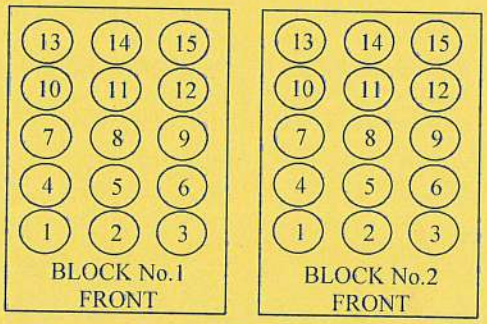

TEMPERATURE MEASUREMENT ACCURACY TEST

Block No.		1	2
Controller temperature (°C)		144	145
Indicating Temperature		144	145
Measured Temperature (° C) at Spread Locations	1	149.3	149.8
	2	149.1	149.9
	3	149.9	149.6
	4	150.0	149.3
	5	149.8	149.5
	6	149.9	149.1
	7	149.7	149.7
	8	149.5	149.9
	9	149.8	149.4
	10	148.5	149.4
	11	149.1	150.2
	12	149.2	150.0
	13	149.0	149.6
	14	149.1	150.3
	15	148.5	149.0
Uncertainty of Measurement(± °C)		0.89	0.89

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.
NOTE 2 : LOCATION 10 WAS REFERENCE LOCATION.
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MU
COVERAGE FACTOR k =2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

[redacted]

ลำดับที่ 5

ระดับเสียงในสถานประกอบการ

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-69/0204 **MTC No.** EEL. BP. 152/0169

CALIBRATION CERTIFICATE

Submitted by : S.P.S.CONSULTING SERVICE CO.,LTD.

Address : 7 Soi Phaholyothin 24, Phaholyothin Road, Jompol, Chatuchak, Bangkok 10900.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre. Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Sound Calibrator

Manufacturer : ACO

Model : 2127

Serial No. : 130006

Ambient Environment

Temperature : (23 + 3) °C

Relative Humidity : (50 ± 15) %

Ambient Pressure : (101.325 ± 1.500) kPa

Standards used :

1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.
2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.
3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.
4. Digital Multimeter Agilent 34401A S/N MY44005560.
5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.
6. Audio Analyzer Keithley 2015-P S/N 4106495.
7. Condenser Microphone Bruel&Kjaer 4180 S/N 2889871.

Calibration Procedure: CP-102-04 based on IEC 60942-2003; The sound pressure level generated by sound calibrator under test shall be measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 29 Jan. 2026

Date of Calibration : 11 Feb. 2026

[redacted]

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

NSC-TISI-TIS 17025
CALIBRATION 0037

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-69/0204 **MTC No.** EEL. BP. 152/0169

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20μPa at 1000 Hz

Acoustic Output in dB re 20μPa, Corrected to Reference Conditions: 101.325 kPa, 23.0 °C and 50 %RH.

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	93.89	-0.11	± 0.10	±0.40 dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	999.9	-0.1	± 1.5	±1.0%

3. Total Distortion

Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	1.90	± 0.50	±3.0%

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Calibrated by : [redacted]

Approved by : [redacted]

Director

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 11 Feb. 2026

Date of Issue : 12 Feb. 2026

Ref : 2011269012900497001

End of Certificate

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Noise R_077/26

Sound Level Meter Calibration Report

Acoustic Calibrator Data			
Brand	ACO	Number	AC 03/56
Model	2127	Serial No.	130006
Calibration Range	94 dB, 1000 Hz	Last Calibration	21 February 2025
		Due Date	21 February 2026

Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-R40	ACO	6236	00192052	03 February 2026	93.9	93.9
ACO-R41	ACO	6236	00192053	03 February 2026	93.9	93.9
ACO-R50	ACO	6236	00192062	03 February 2026	93.9	93.9
ACO-R51	ACO	6236	00192063	03 February 2026	93.9	93.9
ACO-R52	ACO	6236	00192064	03 February 2026	93.9	93.9
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.81 ± 0.10 dB	

Calibrated by : [redacted]

Approved by : [redacted]

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Noise R_125/26

Sound Level Meter Calibration Report

Acoustic Calibrator Data			
Brand	ACO	Number	AC 03/56
Model	2127	Serial No.	130006
Calibration Range	94 dB, 1000 Hz	Last Calibration	11 February 2026
		Due Date	11 February 2027

Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-R40	ACO	6236	00192052	15 March 2026	93.9	93.9
ACO-R41	ACO	6236	00192053	15 March 2026	93.9	93.9
ACO-R50	ACO	6236	00192062	15 March 2026	93.9	93.9
ACO-R51	ACO	6236	00192063	15 March 2026	93.9	93.9
ACO-R52	ACO	6236	00192064	15 March 2026	93.9	93.9
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.81 ± 0.10 dB	

Calibrated by : [redacted]

Approved by : [redacted]

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Noise R_296/26

Sound Level Meter Calibration Report

Acoustic Calibrator Data			
Brand	ACO	Number	AC 03/56
Model	2127	Serial No.	130006
Calibration Range	94 dB, 1000 Hz	Last Calibration	11 February 2026
		Due Date	11 February 2027

Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-R40	ACO	6236	00192052	21 May 2026	93.8	93.9
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.81 ± 0.10 dB	

Calibrated by : [redacted]

Approved by : [redacted]

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Noise R_324/26

Sound Level Meter Calibration Report

Acoustic Calibrator Data			
Brand	ACO	Number	AC 03/56
Model	2127	Serial No.	130006
Calibration Range	94 dB, 1000 Hz	Last Calibration	11 February 2026
		Due Date	11 February 2027

Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-R40	ACO	6236	00192052	03 June 2026	93.9	93.9
ACO-R41	ACO	6236	00192053	03 June 2026	93.8	93.9
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.81 ± 0.10 dB	

Calibrated by : [redacted]

Approved by : [redacted]

ลำดับที่ 6

ปริมาณเสียงสะสมที่ตัวพนักงานเฉลี่ยตลอดระยะเวลาการทำงาน

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0514 **MTC No.** EEL. BP. 34/0868

CALIBRATION CERTIFICATE

Submitted by : S.P.S.Consulting Service Co.,Ltd.

Address : 7 Soi Phaholyothin 24, Phaholyothin Road, Jompol, Chatuchak, Bangkok 10900.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.

: Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Sound Calibrator

Manufacturer : SVANTEK

Model : SV34

Serial No. : 83820

Ambient Environment

Temperature : (23 ± 3) °C

Relative Humidity : (50 ± 15) %

Ambient Pressure : (101.325 ± 1.500) kPa

Standards used :

1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.
2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.
3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.
4. Digital Multimeter Agilent 34401A S/N MY44005560.
5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.
6. Audio Analyzer Panasonic VP-7722A S/N 041477D122.
7. Condenser Microphone B&K 4180 S/N 2633526.

Calibration Procedure: CP-102-04 based on IEC 60942-2003; The sound pressure level generated by sound calibrator under test shall be measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 14 Aug. 2025

Date of Calibration : 22 Aug. 2025

[redacted]

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0514 **MTC No.** EEL. BP. 34/0868

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 114 dB re 20µPa at 1000 Hz

Acoustic Output in dB re 20µPa, Corrected to Reference Conditions: 101.325 kPa, 23.0 °C and 50 %RH.

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	114.02	0.02	± 0.10	±0.75 dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	1000.0	0.0	± 1.5	±2.0%

3. Total Distortion

Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	0.21	± 0.50	±4.0%

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Calibrated by : [redacted]

Approved by : [redacted]

Director

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 22 Aug. 2025

Date of Issue : 25 Aug. 2025

Ref : 20112680814031690l1

End of Certificate

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com.. www.spscon.com

Noise Dose R_078/26

Noise Dose Meter Calibration Report

Acoustic Calibrator Data			
Brand	SVANTEK	Number	SV 03/60
Model	SV34	Serial No.	83820
Calibration Range	114 dB, 1000 Hz	Last Calibration	25 August 2025
		Due Date	25 August 2026

Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
NMD-B07	SVANTEK	SV-104IS	80817	03 February 2026	114.0	114.0
NMD-B08	SVANTEK	SV-104IS	80818	03 February 2026	114.0	114.0
NMD-R02	SVANTEK	SV-104IS	60152	03 February 2026	114.0	114.0
NMD-R03	SVANTEK	SV-104IS	60153	03 February 2026	114.0	114.0
NMD-R06	SVANTEK	SV-104IS	60146	03 February 2026	114.0	114.0
NMD-R13	SVANTEK	SV-104IS	63438	03 February 2026	114.0	114.0
NMD-R22	SVANTEK	SV-104IS	80801	03 February 2026	114.1	114.0
NMD-R26	SVANTEK	SV-104IS	80836	03 February 2026	114.0	114.0
NMD-R35	SVANTEK	SV-104IS	80873	03 February 2026	114.0	114.0
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					114.02± 0.10 dB	

Calibrated by : [redacted]

Approved by : [redacted]

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Noise Dose R_078-1/26

Noise Dose Meter Calibration Report

Acoustic Calibrator Data			
Brand	SVANTEK	Number	SV 03/60
Model	SV34	Serial No.	83820
Calibration Range	114 dB, 1000 Hz	Last Calibration	25 August 2025
		Due Date	25 August 2026

Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
NMD-B03	SVANTEK	SV-104IS	80852	08 February 2026	114.0	114.0
NMD-B04	SVANTEK	SV-104IS	80854	08 February 2026	114.1	114.0
NMD-B05	SVANTEK	SV-104IS	80856	08 February 2026	114.0	114.0
NMD-B06	SVANTEK	SV-104IS	80816	08 February 2026	114.0	114.0
NMD-B07	SVANTEK	SV-104IS	80817	08 February 2026	114.0	114.0
NMD-B08	SVANTEK	SV-104IS	80818	08 February 2026	114.0	114.0
NMD-R02	SVANTEK	SV-104IS	60152	08 February 2026	114.0	114.0
NMD-R03	SVANTEK	SV-104IS	60153	08 February 2026	114.0	114.0
NMD-R06	SVANTEK	SV-104IS	60146	08 February 2026	114.0	114.0
NMD-R13	SVANTEK	SV-104IS	63438	08 February 2026	114.0	114.0
NMD-R22	SVANTEK	SV-104IS	80801	08 February 2026	114.1	114.0
NMD-R26	SVANTEK	SV-104IS	80836	08 February 2026	114.0	114.0
NMD-R35	SVANTEK	SV-104IS	80873	08 February 2026	114.0	114.0
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					114.02± 0.10 dB	

Calibrated by : [redacted]

Approved by : [redacted]

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Noise Dose R_078-2/26

Noise Dose Meter Calibration Report

Acoustic Calibrator Data			
Brand	SVANTEK	Number	SV 03/60
Model	SV34	Serial No.	83820
Calibration Range	114 dB, 1000 Hz	Last Calibration	25 August 2025
		Due Date	25 August 2026

Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
NMD-B07	SVANTEK	SV-104IS	80817	17 February 2026	114.0	114.0
NMD-B08	SVANTEK	SV-104IS	80818	17 February 2026	114.0	114.0
NMD-R02	SVANTEK	SV-104IS	60152	17 February 2026	114.0	114.0
NMD-R03	SVANTEK	SV-104IS	60153	17 February 2026	114.0	114.0
NMD-R06	SVANTEK	SV-104IS	60146	17 February 2026	114.0	114.0
NMD-R13	SVANTEK	SV-104IS	63438	17 February 2026	114.0	114.0
NMD-R22	SVANTEK	SV-104IS	80801	17 February 2026	114.0	114.0
NMD-R26	SVANTEK	SV-104IS	80836	17 February 2026	114.0	114.0
NMD-R35	SVANTEK	SV-104IS	80873	17 February 2026	114.0	114.0
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					114.02± 0.10 dB	

Calibrated by : [redacted]

Approved by : [redacted]

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Noise Dose R_078-3/26

Noise Dose Meter Calibration Report

Acoustic Calibrator Data			
Brand	SVANTEK	Number	SV 03/60
Model	SV34	Serial No.	83820
Calibration Range	114 dB, 1000 Hz	Last Calibration	25 August 2025
		Due Date	25 August 2026

Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
NMD-R02	SVANTEK	SV-104IS	60152	26 February 2026	114.0	114.0
NMD-R03	SVANTEK	SV-104IS	60153	26 February 2026	114.0	114.0
NMD-R06	SVANTEK	SV-104IS	60146	26 February 2026	114.0	114.0
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					114.02± 0.10 dB	

Calibrated by : [redacted]

Approved by : [redacted]

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72 Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Noise Dose R_126/26

Noise Dose Meter Calibration Report

Acoustic Calibrator Data

Brand	SVANTEK	Number	SV 03/60
Model	SV34	Serial No.	83820
Calibration Range	114 dB, 1000 Hz	Last Calibration	25 August 2025
		Due Date	25 August 2026

Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
NMD-B01	SVANTEK	SV-104IS	80840	15 March 2026	113.9	114.0
NMD-B02	SVANTEK	SV-104IS	80842	15 March 2026	114.0	114.0
NMD-B03	SVANTEK	SV-104IS	80852	15 March 2026	114.0	114.0
NMD-B04	SVANTEK	SV-104IS	80854	15 March 2026	114.0	114.0
NMD-B05	SVANTEK	SV-104IS	80856	15 March 2026	113.9	114.0
NMD-B06	SVANTEK	SV-104IS	80816	15 March 2026	114.0	114.0
NMD-B07	SVANTEK	SV-104IS	80817	15 March 2026	114.0	114.0
NMD-B08	SVANTEK	SV-104IS	80818	15 March 2026	114.0	114.0
NMD-B09	SVANTEK	SV-104IS	80829	15 March 2026	114.0	114.0
NMD-B10	SVANTEK	SV-104IS	80830	15 March 2026	114.0	114.0
NMD-B11	SVANTEK	SV-104IS	80831	15 March 2026	114.0	114.0
NMD-B12	SVANTEK	SV-104IS	80832	15 March 2026	114.0	114.0
NMD-B13	SVANTEK	SV-104IS	80834	15 March 2026	113.9	114.0
NMD-B14	SVANTEK	SV-104IS	80875	15 March 2026	114.0	114.0
NMD-B15	SVANTEK	SV-104IS	80880	15 March 2026	114.0	114.0
NMD-B16	SVANTEK	SV-104IS	106120	15 March 2026	114.0	114.0
NMD-B18	SVANTEK	SV-104IS	106123	15 March 2026	114.0	114.0
NMD-B19	SVANTEK	SV-104IS	106124	15 March 2026	113.9	114.0
NMD-B20	SVANTEK	SV-104IS	106131	15 March 2026	114.0	114.0
NMD-R02	SVANTEK	SV-104IS	60152	15 March 2026	114.0	114.0
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					114.02± 0.10 dB	

Calibrated by : [redacted]

Approved by : [redacted]

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Noise Dose R_126-1/26

Noise Dose Meter Calibration Report

Acoustic Calibrator Data			
Brand	SVANTEK	Number	SV 03/60
Model	SV34	Serial No.	83820
Calibration Range	114 dB, 1000 Hz	Last Calibration	25 August 2025
		Due Date	25 August 2026

Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
NMD-R03	SVANTEK	SV-104IS	60153	15 March 2026	114.0	114.0
NMD-R05	SVANTEK	SV-104IS	60155	15 March 2026	113.9	114.0
NMD-R06	SVANTEK	SV-104IS	60146	15 March 2026	114.0	114.0
NMD-R13	SVANTEK	SV-104IS	63438	15 March 2026	114.0	114.0
NMD-R20	SVANTEK	SV-104IS	70035	15 March 2026	113.9	114.0
NMD-R22	SVANTEK	SV-104IS	80801	15 March 2026	114.0	114.0
NMD-R26	SVANTEK	SV-104IS	80836	15 March 2026	114.0	114.0
NMD-R27	SVANTEK	SV-104IS	80837	15 March 2026	113.9	114.0
NMD-R35	SVANTEK	SV-104IS	80873	15 March 2026	114.0	114.0
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					114.02± 0.10 dB	

Calibrated by : [redacted]

Approved by : [redacted]

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Noise Dose R_126-2/26

Noise Dose Meter Calibration Report

Acoustic Calibrator Data			
Brand	SVANTEK	Number	SV 03/60
Model	SV34	Serial No.	83820
Calibration Range	114 dB, 1000 Hz	Last Calibration	25 August 2025
		Due Date	25 August 2026

Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
NMD-B17	SVANTEK	SV-104IS	106122	22 March 2026	114.0	114.0
NMD-B20	SVANTEK	SV-104IS	106131	22 March 2026	113.9	114.0
NMD-R35	SVANTEK	SV-104IS	80873	22 March 2026	114.0	114.0
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					114.02± 0.10 dB	

Calibrated by : [redacted]

Approved by : [redacted]

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Noise Dose R_148/26

Noise Dose Meter Calibration Report

Acoustic Calibrator Data			
Brand	SVANTEK	Number	SV 03/60
Model	SV34	Serial No.	83820
Calibration Range	114 dB, 1000 Hz	Last Calibration	25 August 2025
		Due Date	25 August 2026

Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
NMD-R03	SVANTEK	SV-104IS	60153	29 March 2026	114.0	114.0
NMD-R06	SVANTEK	SV-104IS	60146	29 March 2026	114.0	114.0
NMD-R13	SVANTEK	SV-104IS	63438	29 March 2026	113.9	114.0
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					114.02± 0.10 dB	

Calibrated by : [redacted]

Approved by : [redacted]

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Noise Dose R_365/26

Noise Dose Meter Calibration Report

Acoustic Calibrator Data			
Brand	SVANTEK	Number	SV 03/60
Model	SV34	Serial No.	83820
Calibration Range	114 dB, 1000 Hz	Last Calibration	25 August 2025
		Due Date	25 August 2026

Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
NMD-R02	SVANTEK	SV-104IS	60152	15 June 2026	114.0	114.0
NMD-R03	SVANTEK	SV-104IS	60153	15 June 2026	114.0	114.0
NMD-R06	SVANTEK	SV-104IS	60146	15 June 2026	114.0	114.0
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					114.02± 0.10 dB	

Calibrated by : [redacted]

Approved by : [redacted]

ลำดับที่ 7

ระดับความร้อนในสถานประกอบการ

METROLOGY SYSTEM (THAILAND) CO.,LTD.
A Trescal company

Certificate of Calibration

Certificate Number : SPR25100063-1 Page : 1 of 3

Customer : S.P.S. CONSULTING SERVICE CO., LTD.
7 Soi Phaholyothin 24 Phaholyothin Road., Jompol, Chatuchak, Bangkok 10900

Equipment Name : Area Heat Stress Monitor
Manufacturer : Quest Technologies
Model : QUESTemp 32
Serial Number : TPH050057
ID. Number : B30

Environmental Conditions

Ambient Temperature	: 23 °C ± 2 °C	Received Date	: 06 Oct 2025
Relative Humidity	: 50 % ± 15 %	Calibration Date	: 08 Oct 2025
Location of Calibration	: In-Lab	Recommend Due Date	: 08 Oct 2026
Calibration Procedure	: SP-CPT-04-13	Date of Issue	: 09 Oct 2025

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received.Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full,without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Navaporn Uengseng
Calibration Officer

Approved by [redacted]
Authorized Signatory

SPM A Trescal SP Metrology System (Thailand) Co., Ltd.

69/29 Moo 1 Klongsi Klongluang Pathumthani 12120 Tel: (662) 193-2217-20 www.spmetrology.co.th www.สอบเทียบเครื่องมือวัด.com

Calibration Report

Certificate Number : SPR25100063-1

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
THERMO-HYGROMETER	5020A	A47046	TMU2500342	29 Jan 2026
Temp & Humidity Test Chamber	TEMI1500-01/SD/N/N/	S7110ZL742 1014	SPR25040010-13	20 Apr 2026

Traceability

This certification is traceable to the International System of Unit maintained at :

NA - NA Caltechnologies Co., Ltd.

SP Metrology - SP Metrology system (Thailand) Co.Ltd.

69/29 Moo 1 Klongsi Klongluang Pathumthani 12120 Tel: (662) 193-2217-20 www.spmetrology.co.th www.สอบเทียบเครื่องมือวัด.com

METROLOGY SYSTEM (THAILAND) CO.,LTD.
A Trescal company

Result of Calibration

Certificate Number : SPR25100063-1

Temperature Accuracy in the Measurement. (WET)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.014	30.0	-0.014	0.20
35.0	35.012	35.0	-0.012	0.20
40.0	40.018	40.0	-0.018	0.20

Temperature Accuracy in the Measurement. (DRY)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.014	29.9	-0.114	0.20
35.0	35.012	34.9	-0.112	0.20
40.0	40.018	39.9	-0.118	0.20

Temperature Accuracy in the Measurement. (GLOVE)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.014	29.9	-0.114	0.20
35.0	35.012	34.9	-0.112	0.20
40.0	40.018	39.9	-0.118	0.20

Note :

The result of calibration was found accurate as show on date and place of calibration only. This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor k = 2, providing a level of confidence approximately 95%.

- End of Certificate -

69/29 Moo 1 Klongsi Klongluang Pathumthani 12120 Tel: (662) 193-2217-20 www.spmetrology.co.th www.สอบเทียบเครื่องมือวัด.com

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Heat R015

Heat Stress WBGT Meter Verification Report

Verification Data

Heat Stress WBGT Meter No.	:	B30	Verification Date	:	01 April 2026	
Brand	:	Quest Technologies	Ambient Temp.	:	24.5	^{o}C
Model	:	QUESTemp^{o}32	Barometric Pressure	:	1011	mmbar
Serial No.	:	TPH050057	Relative Humidity	:	49	%

Verification Module (Electronic Sensor Check) :

Verification Module No. : 21 WB = 12.5 ^{o}C, DB = 47.1 ^{o}C, G = 69.3 ^{o}C

Result of Verification : Without Adjustment

Wet Probe Temperature Measurement

Verification Module Reading (^{o}C)	UUC* Reading (^{o}C)	Correction (^{o}C)	Tolerance Limit (^{o}C)
12.5	12.6	-0.1	± 0.5

Dry Probe Temperature Measurement

Verification Module Reading (^{o}C)	UUC* Reading (^{o}C)	Correction (^{o}C)	Tolerance Limit (^{o}C)
47.1	47.2	-0.1	± 0.5

Globe Probe Temperature Measurement

Verification Module Reading (^{o}C)	UUC* Reading (^{o}C)	Correction (^{o}C)	Tolerance Limit (^{o}C)
69.3	69.2	0.1	± 0.5

UUC* = UNIT UNDER CALIBRATION

Verified by : [redacted]

Approved by : [redacted]

METROLOGY SYSTEM (THAILAND) CO.,LTD.
A Trescal company

Certificate of Calibration

Certificate Number : SPR25110089-4 Page : 1 of 3

Customer : S.P.S. CONSULTING SERVICE CO., LTD.
7 Soi Phaholyothin 24 Phaholyothin Road., Jompol, Chatuchak, Bangkok 10900

Equipment Name	:	Area Heat Stress Monitor			
Manufacturer	:	Quest Technologies			
Model	:	QUESTemp 32			
Serial Number	:	TPH050047			
ID. Number	:	B31			
Environmental Conditions					
Ambient Temperature	:	23 °C ± 2 °C	Received Date	:	07 Nov 2025
Relative Humidity	:	50 % ± 15 %	Calibration Date	:	01 Dec 2025
Location of Calibration	:	In-Lab	Recommend Due Date	:	01 Dec 2026
Calibration Procedure	:	SP-CPT-04-13	Date of Issue	:	02 Dec 2025

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received.Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full,without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Chatchai Kittisopha
Calibration Officer

Approved by

[redacted]

Authorized Signatory

SP-FM-04-15 rev.0

69/29 Moo 1 Klongsi Klongluang Pathumthani 12120 Tel: (662) 193-2217-20 www.spmetrology.co.th www.สอบเทียบเครื่องมือวัด.com

Calibration Report

Certificate Number : SPR25110089-4

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
THERMO-HYGROMETER	5020A	A47046	TMU2500342	29 Jan 2026
Temp & Humidity Test Chamber	TEMI1500-01/SD/N/N/	S7110ZL742 1014	SPR25040010-13	20 Apr 2026

Traceability

This certification is traceable to the International System of Unit maintained at :

NA - NA Caltechnologies Co., Ltd.

SP Metrology - SP Metrology system (Thailand) Co.Ltd.

69/29 Moo 1 Klongsi Klongluang Pathumthani 12120 Tel: (662) 193-2217-20 www.spmetrology.co.th www.สอบเทียบเครื่องมือวัด.com

METROLOGY SYSTEM (THAILAND) CO.,LTD.
A Trescal company

Result of Calibration

Certificate Number : SPR25110089-4

Temperature Accuracy in the Measurement. (WET)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.006	29.5	-0.506	0.20
35.0	35.009	34.6	-0.409	0.20
40.0	40.008	39.5	-0.508	0.21

Temperature Accuracy in the Measurement. (DRY)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.006	29.5	-0.506	0.20
35.0	35.009	34.6	-0.409	0.20
40.0	40.008	39.6	-0.408	0.21

Temperature Accuracy in the Measurement. (GLOVE)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.006	29.6	-0.406	0.20
35.0	35.009	34.7	-0.309	0.20
40.0	40.008	39.7	-0.308	0.21

Note :

The result of calibration was found accurate as show on date and place of calibration only. This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor k = 2, providing a level of confidence approximately 95%.

- End of Certificate -

69/29 Moo 1 Klongsi Klongluang Pathumthani 12120 Tel: (662) 193-2217-20 www.spmetrology.co.th www.สอบเทียบเครื่องมือวัด.com

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Heat R015

Heat Stress WBGT Meter Verification Report

Verification Data

Heat Stress WBGT Meter No.	:	B31	Verification Date	:	01 April 2026	
Brand	:	Quest Technologies	Ambient Temp.	:	24.5	°C
Model	:	QUESTemp°32	Barometric Pressure	:	1011	mmbar
Serial No.	:	TPH050047	Relative Humidity	:	49	%

Verification Module (Electronic Sensor Check) :

Verification Module No. : 21 WB = 12.5 °C, DB = 47.1 °C, G = 69.3 °C

Result of Verification : Without Adjustment

Wet Probe Temperature Measurement

Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
12.5	12.6	-0.1	± 0.5

Dry Probe Temperature Measurement

Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
47.1	47.2	-0.1	± 0.5

Globe Probe Temperature Measurement

Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
69.3	69.2	0.1	± 0.5

UUC* = UNIT UNDER CALIBRATION

Verified by : [redacted]

Approved by : [redacted]

METROLOGY SYSTEM (THAILAND) CO.,LTD.

A Trescal company

Certificate of Calibration

Certificate Number : SPR26010387-4 Page : 1 of 3

Customer : S.P.S. CONSULTING SERVICE CO., LTD.
7 Soi Phaholyothin 24 Phaholyothin Road., Jompol, Chatuchak, Bangkok 10900

Equipment Name	:	Area Heat Stress Monitor			
Manufacturer	:	Quest Technologies			
Model	:	QUESTemp 32			
Serial Number	:	TPH050015			
ID. Number	:	B32			
Environmental Conditions					
Ambient Temperature	:	23 °C ± 2 °C	Received Date	:	30 Jan 2026
Relative Humidity	:	50 % ± 15 %	Calibration Date	:	03 Feb 2026
Location of Calibration	:	In-Lab	Recommend Due Date	:	03 Feb 2027
Calibration Procedure	:	SP-CPT-04-13	Date of Issue	:	04 Feb 2026

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received.Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full,without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Jirasak Pumbut
Calibration Officer

Approved by

[redacted]

Authorized Signatory

SPM A Trescal SP Metrology System (Thailand) Co., Ltd.

69/29 Moo 1 Klongsi Klongluang Pathumthani 12120 Tel: (662) 193-2217-20 www.spmetrology.co.th www.สอบเทียบเครื่องมือวัด.com

METROLOGY SYSTEM (THAILAND) CO.,LTD.
A Trescal company

Calibration Report

Certificate Number : SPR26010387-4

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
THERMO-HYGROMETER	5020A	A47046	TMU2500342	29 Jan 2027
Temp & Humidity Test Chamber	TEMI1500-01/SD/N/N/	S7110ZL742 1014	SPR25040010-13	20 Apr 2026

Traceability

This certification is traceable to the International System of Unit maintained at :

NA - NA Caltechnologies Co., Ltd.

SP Metrology - SP Metrology system (Thailand) Co.Ltd.

69/29 Moo 1 Klongsi Klongluang Pathumthani 12120 Tel: (662) 193-2217-20 www.spmetrology.co.th www.สอบเทียบเครื่องมือวัด.com

METROLOGY SYSTEM (THAILAND) CO.,LTD.
A Trescal company

Result of Calibration

Certificate Number : SPR26010387-4

Temperature Accuracy in the Measurement. (WET)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.009	29.8	-0.209	0.20
35.0	35.012	34.8	-0.212	0.20
40.0	40.017	39.8	-0.217	0.21

Temperature Accuracy in the Measurement. (DRY)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.009	29.9	-0.109	0.20
35.0	35.012	34.9	-0.112	0.20
40.0	40.017	39.9	-0.117	0.21

Temperature Accuracy in the Measurement. (GLOBE)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.009	30.1	0.091	0.20
35.0	35.012	35.1	0.088	0.20
40.0	40.017	40.1	0.083	0.21

Note :

The result of calibration was found accurate as show on date and place of calibration only. This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor k = 2, providing a level of confidence approximately 95%.

- End of Certificate -

69/29 Moo 1 Klongsi Klongluang Pathumthani 12120 Tel: (662) 193-2217-20 www.spmetrology.co.th www.สอบเทียบเครื่องมือวัด.com

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com,. www.spscon.com

Heat R015

Heat Stress WBGT Meter Verification Report

Verification Data

Heat Stress WBGT Meter No.	: B32	Verification Date	:	01 April 2026	
Brand	: Quest Technologies	Ambient Temp.	:	24.5	°C
Model	: QUESTemp°32	Barometric Pressure	:	1011	mmbar
Serial No.	: TPH050015	Relative Humidity	:	49	%

Verification Module (Electronic Sensor Check) :

Verification Module No. : 21 WB = 12.5 °C, DB = 47.1 °C, G = 69.3 °C

Result of Verification : Without Adjustment

Wet Probe Temperature Measurement

Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
12.5	12.6	-0.1	± 0.5

Dry Probe Temperature Measurement

Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
47.1	47.2	-0.1	± 0.5

Globe Probe Temperature Measurement

Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
69.3	69.2	0.1	± 0.5

UUC* = UNIT UNDER CALIBRATION

Verified by : [redacted]

Approved by : [redacted]

METROLOGY SYSTEM (THAILAND) CO.,LTD.
A Trescal company

Certificate of Calibration

Certificate Number : SPR25100063-6 Page : 1 of 3

Customer : S.P.S. CONSULTING SERVICE CO., LTD.
7 Soi Phaholyothin 24 Phaholyothin Road., Jompol, Chatuchak, Bangkok 10900

Equipment Name	:	Area Heat Stress Monitor			
Manufacturer	:	Quest Technologies			
Model	:	QUESTemp 32			
Serial Number	:	TPK120034			
ID. Number	:	B33			
Environmental Conditions					
Ambient Temperature	:	23 °C ± 2 °C	Received Date	:	06 Oct 2025
Relative Humidity	:	50 % ± 15 %	Calibration Date	:	21 Oct 2025
Location of Calibration	:	In-Lab	Recommend Due Date	:	21 Oct 2026
Calibration Procedure	:	SP-CPT-04-13	Date of Issue	:	22 Oct 2025

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received.Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full,without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Jirasak Pumbut
Calibration Officer

Approved by

[redacted]

Authorized Signatory

SP-FM-04-15 rev.0

69/29 Moo 1 Klongsi Klongluang Pathumthani 12120 Tel: (662) 193-2217-20 www.spmetrology.co.th www.สอบเทียบเครื่องมือวัด.com

Calibration Report

Certificate Number : SPR25100063-6

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
THERMO-HYGROMETER	5020A	A47046	TMU2500342	29 Jan 2026
Temp & Humidity Test Chamber	TEMI1500-01/SD/N/N/	S7110ZL742 1014	SPR25040010-13	20 Apr 2026

Traceability

This certification is traceable to the International System of Unit maintained at :

NA - NA Caltechnologies Co., Ltd.

SP Metrology - SP Metrology system (Thailand) Co.Ltd.

69/29 Moo 1 Klongsi Klongluang Pathumthani 12120 Tel: (662) 193-2217-20 www.spmetrology.co.th www.สอบเทียบเครื่องมือวัด.com

METROLOGY SYSTEM (THAILAND) CO.,LTD.
A Trescal company

Result of Calibration

Certificate Number : SPR25100063-6

Temperature Accuracy in the Measurement. (WET)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.007	30.0	-0.007	0.20
35.0	35.009	35.1	0.091	0.20
40.0	40.005	40.1	0.095	0.21

Temperature Accuracy in the Measurement. (DRY)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.007	30.1	0.093	0.20
35.0	35.009	35.1	0.091	0.20
40.0	40.005	40.1	0.095	0.21

Temperature Accuracy in the Measurement. (GLOVE)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.007	29.9	-0.107	0.20
35.0	35.009	34.9	-0.109	0.20
40.0	40.005	39.9	-0.105	0.21

Note :

The result of calibration was found accurate as show on date and place of calibration only. This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor k = 2, providing a level of confidence approximately 95%.

- End of Certificate -

69/29 Moo 1 Klongsi Klongluang Pathumthani 12120 Tel: (662) 193-2217-20 www.spmetrology.co.th www.สอบเทียบเครื่องมือวัด.com

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Heat R015

Heat Stress WBGT Meter Verification Report

Verification Data

Heat Stress WBGT Meter No.	:	B33	Verification Date	:	01 April 2026	
Brand	:	Quest Technologies	Ambient Temp.	:	24.5	°C
Model	:	QUESTemp°32	Barometric Pressure	:	1011	mmbar
Serial No.	:	TPK120034	Relative Humidity	:	49	%

Verification Module (Electronic Sensor Check) :

Verification Module No. : 21 WB = 12.5 °C, DB = 47.1 °C, G = 69.3 °C

Result of Verification : Without Adjustment

Wet Probe Temperature Measurement

Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
12.5	12.6	-0.1	± 0.5

Dry Probe Temperature Measurement

Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
47.1	47.2	-0.1	± 0.5

Globe Probe Temperature Measurement

Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
69.3	69.2	0.1	± 0.5

UUC* = UNIT UNDER CALIBRATION

Verified by : [redacted]

Approved by : [redacted]

ลำดับที่ 8

คุณภาพอากาศในสถานประกอบการ

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H | S/N : 136164

Environmental Conditions

Temperature	25	± 3	°C
Pressure	1010	± 15	mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R^2
B01	SKC	224-PCXR4	262101	05/01/2026	1,000	1,500	2,000	1,004	1,501	2,003	1.010x – 18.941	0.999
B02	SKC	224-PCXR4	626166	05/01/2026	1,000	1,500	2,000	1,000	1,500	2,002	1.012x - 23.432	0.999
B03	SKC	224-PCXR4	612968	05/01/2026	1,000	1,500	2,000	993	1,503	2,001	1.008x - 15.587	1.000
B04	SKC	224-PCXR4	602804	06/01/2026	1,000	1,500	2,000	1,001	1,498	1,996	0.997x + 2.672	1.000
B05	SKC	224-PCXR4	612693	07/01/2026	1,000	1,500	2,000	999	1,494	1,993	0.995x + 1.555	1.000
B06	SKC	224-PCXR4	262188	06/01/2026	1,000	1,500	2,000	1,002	1,501	2,004	1.007x - 12.528	1.000
B07	SKC	224-PCXR4	626262	06/01/2026	1,000	1,500	2,000	1,003	1,501	2,002	1.010x - 19.021	0.999
B08	SKC	224-PCXR4	626100	06/01/2026	1,000	1,500	2,000	1,005	1,500	2,006	1.006x - 8.619	1.000
B09	SKC	224-PCXR4	626479	05/01/2026	1,000	1,500	2,000	1,001	1,500	2,000	1.007x - 14.458	1.000
B10	SKC	224-PCXR4	091950	05/01/2026	1,000	1,500	2,000	998	1,503	2,000	1.001x – 5.945	1.000
B11	SKC	224-PCXR8	564315	05/01/2026	1,000	1,500	2,000	993	1,494	1,993	1.010x - 25.765	0.999
B12	SKC	224-PCXR4	034656	05/01/2026	1,000	1,500	2,000	995	1,497	1,998	0.996x - 4.790	0.999
B13	SKC	224-PCXR4	602073	05/01/2026	1,000	1,500	2,000	994	1,499	1,975	0.990x + 6.525	0.999
B14	SKC	224-PCXR4	626313	05/01/2026	1,000	1,500	2,000	993	1,499	1,994	1.001x - 7.291	1.000
B15	SKC	224-PCXR4	626474	05/01/2026	1,000	1,500	2,000	992	1,505	2,002	1.012x - 23.464	1.000
B16	SKC	224-PCXR4	626477	06/01/2026	1,000	1,500	2,000	993	1,496	1,991	0.996x + 0.945	1.000
B17	SKC	224-PCXR4	626860	06/01/2026	1,000	1,500	2,000	1,000	1,500	2,001	1.007x - 14.414	1.000
B18	SKC	224-PCXR4	691484	05/01/2026	1,000	1,500	2,000	994	1,502	2,002	1.015x - 30.763	0.999
B19	SKC	224-PCXR4	691599	05/01/2026	1,000	1,500	2,000	993	1,490	1,999	1.006x - 14.713	1.000
B20	SKC	224-PCXR4	691587	05/01/2026	1,000	1,500	2,000	991	1,500	1,997	1.005x - 13.565	1.000
B21	SKC	224-PCXR4	691531	05/01/2026	1,000	1,500	2,000	1,002	1,500	2,000	1.002x - 6.050	1.000
B22	SKC	224-PCXR4	691654	05/01/2026	1,000	1,500	2,000	1,008	1,498	1,995	1.000x - 6.158	0.999
B23	SKC	224-PCXR4	798393	06/01/2026	1,000	1,500	2,000	992	1,498	1,972	0.990x + 3.813	0.999
B24	SKC	224-PCXR4	626363	06/01/2026	1,000	1,500	2,000	1,003	1,493	2,002	1.001x - 5.201	1.000
B25	SKC	224-PCXR4	798489	06/01/2026	1,000	1,500	2,000	993	1,496	1,995	1.003x - 10.857	1.000
B26	SKC	224-PCXR4	798479	06/01/2026	1,000	1,500	2,000	994	1,505	2,002	1.012x - 23.253	1.000
B27	SKC	224-PCXR4	691673	06/01/2026	1,000	1,500	2,000	996	1,506	1,989	0.994x + 5.799	1.000
B28	SKC	224-PCXR4	691570	06/01/2026	1,000	1,500	2,000	995	1,502	1,998	0.999x - 5.193	1.000
B29	SKC	224-PCXR4	626472	05/01/2026	1,000	1,500	2,000	995	1,491	1,993	0.999x - 4.662	1.000
B30	SKC	224-PCXR4	691489	05/01/2026	1,000	1,500	2,000	1,003	1,500	1,998	1.002x – 6.804	1.000
B31	SKC	224-PCXR4	691509	05/01/2026	1,000	1,500	2,000	993	1,500	1,997	0.992x + 4.256	1.000
B32	SKC	224-PCXR4	091567	05/01/2026	1,000	1,500	2,000	994	1,487	1,972	0.990x - 2.389	0.999
B33	SKC	224-PCXR4	091756	05/01/2026	1,000	1,500	2,000	993	1,496	1,998	1.013x – 28.816	0.999
B34	SKC	224-PCXR4	612962	05/01/2026	1,000	1,500	2,000	994	1,502	2,003	1.011x - 21.717	1.000
B35	SKC	224-PCXR4	602682	06/01/2026	1,000	1,500	2,000	998	1,493	2,000	1.001x - 2.561	1.000
B36	SKC	224-PCXR4	626164	06/01/2026	1,000	1,500	2,000	993	1,497	1,994	1.003x - 8.755	1.000
B37	SKC	224-PCXR4	626256	06/01/2026	1,000	1,500	2,000	993	1,508	2,007	1.009x - 10.996	1.000
B38	SKC	224-PCXR4	626167	06/01/2026	1,000	1,500	2,000	993	1,502	2,000	1.013x - 28.162	0.999
B39	SKC	224-PCXR4	034637	06/01/2026	1,000	1,500	2,000	1,000	1,497	1,993	0.991x + 9.544	1.000
B40	SKC	224-PCXR4	798349	06/01/2026	1,000	1,500	2,000	1,000	1,499	1,994	0.998x - 0.160	1.000

Calibrated by : [redacted]

Approved by : [redacted]

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H | S/N : 136164

Environmental Conditions

Temperature	.	25	± 3	°C
Pressure	.	1010	± 15	mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R^2
B41	SKC	224-PCXR4	612669	05/01/2026	1,000	1,500	2,000	995	1,490	1,997	1.004x - 11.846	1.000
B42	SKC	224-PCXR4	626041	05/01/2026	1,000	1,500	2,000	996	1,510	1,999	0.999x - 0.630	1.000
B43	SKC	224-PCXR4	034636	05/01/2026	1,000	1,500	2,000	1,000	1,493	2,004	1.004x - 6.760	1.000
B44	SKC	224-PCXR8	529341	05/01/2026	1,000	1,500	2,000	995	1,512	1,995	1.000x - 4.571	0.999
B45	SKC	224-PCXR8	529594	05/01/2026	1,000	1,500	2,000	997	1,503	2,001	1.004x - 10.178	1.000
B46	SKC	224-PCXR8	566743	05/01/2026	1,000	1,500	2,000	997	1,491	2,007	1.013x - 21.797	1.000
B47	SKC	224-PCXR8	566747	06/01/2026	1,000	1,500	2,000	995	1,508	1,999	1.007x - 15.240	0.999
B48	SKC	224-PCXR8	566753	06/01/2026	1,000	1,500	2,000	998	1,493	1,992	0.997x - 0.746	1.000
B49	SKC	224-PCXR8	566780	06/01/2026	1,000	1,500	2,000	994	1,475	1,991	1.002x - 18.905	0.999
B50	SKC	224-PCXR8	500400	06/01/2026	1,000	1,500	2,000	990	1,498	1,992	0.991x + 4.770	0.999
B51	SKC	224-PCXR8	500363	06/01/2026	1,000	1,500	2,000	995	1,498	1,994	1.008x - 21.051	0.999
B52	SKC	224-PCXR8	093186	06/01/2026	1,000	1,500	2,000	1,001	1,494	1,995	0.993x + 6.362	1.000
B53	SKC	224-PCXR8	707670	06/01/2026	1,000	1,500	2,000	992	1,502	2,007	1.016x - 28.087	1.000
B54	SKC	224-PCXR3	509821	06/01/2026	1,000	1,500	2,000	1,000	1,497	2,002	1.009x - 18.056	1.000
B55	SKC	224-PCXR3	510710	05/01/2026	1,000	1,500	2,000	999	1,497	2,001	1.008x - 15.994	1.000
B56	SKC	224-PCXR3	511450	05/01/2026	1,000	1,500	2,000	996	1,510	2,001	1.005x - 11.080	0.999
B57	SKC	224-PCXR3	510798	05/01/2026	1,000	1,500	2,000	1,000	1,493	2,001	1.000x - 1.575	1.000
B58	SKC	224-PCXR3	509852	05/01/2026	1,000	1,500	2,000	997	1,473	1,995	1.000x - 11.132	0.999
B59	SKC	224-PCXR3	509862	05/01/2026	1,000	1,500	2,000	961	1,461	1,969	1.021x - 71.317	0.999
B60	SKC	224-PCXR3	512655	06/01/2026	1,000	1,500	2,000	971	1,469	2,001	1.027x - 56.285	0.999
B61	SKC	224-PCXR3	503915	06/01/2026	1,000	1,500	2,000	1,000	1,476	2,001	1.006x - 16.496	0.999
B62	SKC	224-PCXR3	505975	06/01/2026	1,000	1,500	2,000	997	1,503	2,001	1.004x - 10.186	1.000
B63	SKC	224-PCXR3	511432	06/01/2026	1,000	1,500	2,000	1,000	1,496	1,994	0.996x - 0.574	1.000
B64	SKC	224-PCXR3	508302	06/01/2026	1,000	1,500	2,000	1,000	1,500	1,997	1.000x - 4.850	1.000
B65	SKC	224-PCXR3	508310	05/01/2026	1,000	1,500	2,000	998	1,505	1,999	1.001x - 5.999	1.000
B66	SKC	224-PCXR3	509861	05/01/2026	1,000	1,500	2,000	1,003	1,501	2,006	1.009x - 15.631	0.999
B67	SKC	224-PCXR3	506295	05/01/2026	1,000	1,500	2,000	996	1,496	1,993	0.999x - 4.016	1.000
B68	SKC	224-PCXR3	505872	05/01/2026	1,000	1,500	2,000	1,003	1,491	2,001	0.995x + 5.309	1.000
B69	SKC	224-PCXR3	508375	06/01/2026	1,000	1,500	2,000	994	1,507	2,002	1.008x - 16.847	0.999
B70	SKC	224-PCXR3	510623	06/01/2026	1,000	1,500	2,000	993	1,506	2,003	1.010x - 18.889	1.000
B71	SKC	224-PCXR3	508367	07/01/2026	1,000	1,500	2,000	997	1,501	1,994	0.999x - 0.148	1.000
B72	SKC	224-PCXR3	505977	06/01/2026	1,000	1,500	2,000	1,000	1,503	2,003	1.004x - 8.252	1.000
B73	SKC	224-PCXR3	512606	06/01/2026	1,000	1,500	2,000	996	1,495	1,995	0.998x - 1.627	1.000
B74	SKC	224-PCXR3	505993	06/01/2026	1,000	1,500	2,000	995	1,506	1,999	1.008x - 17.629	0.999
B75	SKC	224-PCXR3	509820	05/01/2026	1,000	1,500	2,000	997	1,491	1,999	1.001x - 6.461	1.000
B76	SKC	224-PCXR3	509811	05/01/2026	1,000	1,500	2,000	1,000	1,472	2,004	1.008x - 18.391	1.000
B77	SKC	224-PCXR3	508301	05/01/2026	1,000	1,500	2,000	993	1,471	1,995	1.000x - 10.813	0.999
B78	SKC	224-PCXR3	510677	05/01/2026	1,000	1,500	2,000	999	1,477	2,000	1.003x - 12.304	0.999
B79	SKC	224-PCXR3	510920	06/01/2026	1,000	1,500	2,000	1,001	1,500	1,997	0.998x + 0.215	1.000

Calibrated by : [redacted]

Approved by : [redacted]

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H | S/N : 136164

Environmental Conditions

Temperature	.	25	± 3	°C
Pressure	.	1010	± 15	mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R^2
B80	SKC	224-PCXR3	504569	06/01/2026	1,000	1,500	2,000	995	1,499	1,996	0.991x + 5.480	0.999
B81	SKC	224-PCXR3	503480	06/01/2026	1,000	1,500	2,000	1,000	1,474	1,999	1.001x - 10.358	0.999
B82	SKC	224-PCXR3	505673	06/01/2026	1,000	1,500	2,000	1,000	1,474	1,995	0.998x - 6.617	0.999
B83	SKC	224-PCXR3	510785	06/01/2026	1,000	1,500	2,000	1,002	1,503	1,992	0.991x + 10.253	1.000
B84	SKC	224-PCXR3	508333	05/01/2026	1,000	1,500	2,000	994	1,501	1,989	0.997x - 2.939	1.000
B85	SKC	224-PCXR3	505757	05/01/2026	1,000	1,500	2,000	995	1,494	2,006	1.012x - 22.072	0.999
B86	SKC	224-PCXR3	512625	05/01/2026	1,000	1,500	2,000	997	1,507	1,992	0.998x + 11.080	0.999
B87	SKC	224-PCXR3	504324	05/01/2026	1,000	1,500	2,000	994	1,473	1,996	1.000x - 10.529	0.999
B88	SKC	224-PCXR3	508307	05/01/2026	1,000	1,500	2,000	993	1,470	1,989	0.991x - 3.749	0.999
B89	SKC	224-PCXR3	509860	05/01/2026	1,000	1,500	2,000	1,001	1,499	2,005	1.007x - 12.041	1.000
B90	SKC	224-PCXR3	508366	06/01/2026	1,000	1,500	2,000	997	1,494	2,001	1.003x - 8.172	1.000
B91	SKC	224-PCXR3	510919	06/01/2026	1,000	1,500	2,000	995	1,491	1,997	1.004x - 14.630	1.000
B92	SKC	224-PCXR3	510987	06/01/2026	1,000	1,500	2,000	974	1,499	1,995	1.017x - 40.878	0.999
B93	SKC	224-PCXR3	509845	06/01/2026	1,000	1,500	2,000	995	1,493	1,997	0.992x + 3.414	0.999

Calibrated by : [redacted]

Approved by : [redacted]

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136833

Environmental Conditions

Temperature	.	25	± 3	°C
Pressure	.	1010	± 15	mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R^2
R01	SKC	224-PCXR4	602467	05/01/2026	1,000	1,500	2,000	999	1,505	2,009	1.011x - 15.308	1.000
R02	SKC	224-PCXR4	626450	05/01/2026	1,000	2,000	3,000	1,001	1,505	2,005	1.005x - 5.625	1.000
R03	SKC	224-PCXR4	691592	05/01/2026	1,000	1,500	2,000	998	1,499	2,010	1.009x – 11.382	1.000
R04	SKC	224-PCXR4	691672	05/01/2026	1,000	1,500	2,000	999	1,496	2,000	0.992x + 5.045	0.999
R05	SKC	224-PCXR4	798470	06/01/2026	1,000	1,500	2,000	997	1,480	1,991	0.995x - 8.487	0.999
R06	SKC	224-PCXR4	798456	06/01/2026	1,000	1,500	2,000	1,000	1,502	1,992	0.993x + 2.874	0.999
R07	SKC	224-PCXR4	798480	06/01/2026	1,000	1,500	2,000	1,000	1,508	2,000	1.000x + 1.559	1.000
R08	SKC	224-PCXR4	883215	07/01/2026	1,000	1,500	2,000	1,001	1,500	2,000	1.004x - 8.216	1.000
R09	SKC	224-PCXR4	034650	05/01/2026	1,000	1,500	2,000	999	1,509	2,005	1.005x - 6.025	1.000
R10	SKC	224-PCXR4	091765	05/01/2026	1,000	1,500	2,000	1,001	1,509	2,008	1.007x - 8.311	1.000
R11	SKC	224-PCXR4	091763	05/01/2026	1,000	1,500	2,000	999	1,502	1,995	1.002x - 10.594	0.999
R12	SKC	224-PCXR4	091568	06/01/2026	1,000	1,500	2,000	999	1,495	1,994	0.994x - 1.683	0.999
R13	SKC	224-PCXR4	091638	06/01/2026	1,000	1,500	2,000	999	1,499	1,994	0.998x - 7.136	0.999
R14	SKC	224-PCXR4	091764	06/01/2026	1,000	1,500	2,000	1,004	1,507	2,006	1.007x - 8.975	1.000
R15	SKC	224-PCXR8	529457	06/01/2026	1,000	1,500	2,000	1,004	1,502	2,002	0.999x + 1.731	1.000
R16	SKC	224-PCXR8	529643	05/01/2026	1,000	1,500	2,000	1,001	1,511	2,010	1.010x - 13.433	1.000
R17	SKC	224-PCXR8	529645	06/01/2026	1,000	1,500	2,000	1,004	1,502	2,003	0.998x + 4.238	1.000
R18	SKC	224-PCXR8	566756	05/01/2026	1,000	1,500	2,000	1,003	1,504	2,006	1.004x - 3.774	1.000
R19	SKC	224-PCXR8	566802	05/01/2026	1,000	1,500	2,000	1,003	1,498	1,995	1.001x - 8.224	0.999
R20	SKC	224-PCXR8	529089	06/01/2026	1,000	1,500	2,000	997	1,509	1,985	0.994x + 5.269	0.999
R21	SKC	224-PCXR8	665728	06/01/2026	1,000	1,500	2,000	1,000	1,510	1,995	0.998x - 1.139	0.999
R22	SKC	224-PCXR8	707444	05/01/2026	1,000	1,500	2,000	1,004	1,507	2,008	1.004x - 5.709	1.000
R23	SKC	224-PCXR8	761067	05/01/2026	1,000	1,500	2,000	1,009	1,504	2,006	1.000x + 1.179	1.000
R24	SKC	224-PCXR8	707893	05/01/2026	1,000	1,500	2,000	999	1,497	1,992	0.998x - 8.383	0.999
R25	SKC	224-PCXR8	761052	06/01/2026	1,000	1,500	2,000	998	1,503	1,975	0.984x + 17.071	0.999
R26	SKC	224-PCXR8	707956	05/01/2026	1,000	1,500	2,000	997	1,492	1,992	0.991x + 0.388	1.000
R27	SKC	224-PCXR8	707398	05/01/2026	1,000	1,500	2,000	1,000	1,495	2,002	1.002x - 3.898	1.000
R28	SKC	224-PCXR8	707481	06/01/2026	1,000	1,500	2,000	1,009	1,503	2,008	0.996x + 8.659	1.000
R29	SKC	224-PCXR8	707402	07/01/2026	1,000	1,500	2,000	1,006	1,513	2,009	1.002x - 1.219	0.999
R30	SKC	224-PCXR8	093811	07/01/2026	1,000	1,500	2,000	1,001	1,513	2,008	1.008x - 9.239	1.000
R31	SKC	224-PCXR8	093183	06/01/2026	1,000	1,500	2,000	1,010	1,507	2,013	1.003x - 0.780	1.000
R32	SKC	224-PCXR8	671950	06/01/2026	1,000	1,500	2,000	999	1,498	1,999	1.000x + 0.668	1.000
R33	SKC	224-PCXR4	626254	06/01/2026	1,000	1,500	2,000	1,000	1,508	2,007	1.004x - 5.149	1.000
R34	SKC	224-PCXR4	626131	05/01/2026	1,000	1,500	2,000	996	1,498	2,003	1.010x - 18.178	1.000
R35	SKC	224-PCXR8	707460	05/01/2026	1,000	1,500	2,000	1,006	1,496	2,004	0.999x + 0.388	1.000
R36	SKC	224-PCXR8	707446	05/01/2026	1,000	1,500	2,000	1,006	1,504	2,008	1.005x - 6.281	1.000
R37	SKC	224-PCXR8	707432	06/01/2026	1,000	1,500	2,000	1,003	1,505	2,004	1.004x - 5.005	1.000
R38	SKC	224-PCXR8	707349	06/01/2026	1,000	1,500	2,000	998	1,498	1,997	0.999x – 1.655	1.000
R39	SKC	224-PCXR8	761095	06/01/2026	1,000	1,500	2,000	1,000	1,497	2,003	1.005x - 8.068	1.000

Calibrated by : [redacted]

Approved by : [redacted]

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H | S/N : 136833

Environmental Conditions

Temperature	25	± 3	°C
Pressure	1010	± 15	mmbar

Personal Pump Data				Calibration Data							
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R^2
R40	SKC	224-PCXR4	612753	05/01/2026	1,000	1,500	2,000	997	1,506	1,998	1.000x - 0.556	1.000
R41	SKC	224-PCXR4	626140	05/01/2026	1,000	1,500	2,000	995	1,504	1,992	0.996x - 3.574	0.999
R42	SKC	224-PCXR4	626463	05/01/2026	1,000	1,500	2,000	1,006	1,505	1,984	0.988x + 15.108	0.999
R43	SKC	224-PCXR4	626129	05/01/2026	1,000	1,500	2,000	993	1,504	1,972	0982.x + 17.902	0.999
R44	SKC	224-PCXR4	602753	06/01/2026	1,000	1,500	2,000	1,001	1,495	2,000	1.001x - 3.434	1.000
R45	SKC	224-PCXR4	626137	06/01/2026	1,000	1,500	2,000	998	1,494	1,997	0.996x + 1.827	1.000

Calibrated by : [redacted]

Approved by : [redacted]

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72. Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter	Model : Defender 510-H	S/N : 136164

Environmental Conditions

Temperature	.	25	± 3	°C
Pressure	.	1010	± 15	mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R^2
B01	SKC	224-PCXR4	262101	01/04/2026	1,000	1,500	2,000	1,002	1,503	2,004	1.002x – 1.364	1.000
B02	SKC	224-PCXR4	626166	01/04/2026	1,000	1,500	2,000	1,004	1,501	2,003	1.001x - 0.594	1.000
B03	SKC	224-PCXR4	612968	01/04/2026	1,000	1,500	2,000	1,003	1,502	1,994	1.003x - 9.098	0.999
B04	SKC	224-PCXR4	602804	01/04/2026	1,000	1,500	2,000	1,000	1,502	1,998	0.998x + 0.642	1.000
B05	SKC	224-PCXR4	612693	01/04/2026	1,000	1,500	2,000	1,001	1,504	1,999	1.000x - 1.767	1.000
B06	SKC	224-PCXR4	262188	01/04/2026	1,000	1,500	2,000	999	1,500	2,002	1.001x - 3.590	1.000
B07	SKC	224-PCXR4	626262	01/04/2026	1,000	1,500	2,000	997	1,506	2,003	1.004x - 9.859	0.999
B08	SKC	224-PCXR4	626100	01/04/2026	1,000	1,500	2,000	1,003	1,503	2,005	1.003x - 4.160	1.000
B09	SKC	224-PCXR4	626479	01/04/2026	1,000	1,500	2,000	998	1,497	1,997	1.000x - 3.382	1.000
B10	SKC	224-PCXR4	091950	01/04/2026	1,000	1,500	2,000	1,004	1,506	1,996	1.003x – 7.323	0.999
B11	SKC	224-PCXR8	564315	01/04/2026	1,000	1,500	2,000	1,000	1,493	2,003	1.005x - 10.601	1.000
B12	SKC	224-PCXR4	034656	01/04/2026	1,000	1,500	2,000	997	1,495	1,997	0.998x - 1.755	1.000
B13	SKC	224-PCXR4	602073	01/04/2026	1,000	1,500	2,000	1,001	1,501	1,986	0.996x + 2.864	0.999
B14	SKC	224-PCXR4	626313	01/04/2026	1,000	1,500	2,000	999	1,494	1,997	0.999x - 1.898	0.999
B15	SKC	224-PCXR4	626474	01/04/2026	1,000	1,500	2,000	996	1,498	1,993	1.007x - 17.126	0.999
B16	SKC	224-PCXR4	626477	01/04/2026	1,000	1,500	2,000	1,002	1,499	1,997	0.997x + 1.352	1.000
B17	SKC	224-PCXR4	626860	01/04/2026	1,000	1,500	2,000	996	1,510	1,999	1.005x - 12.252	0.999
B18	SKC	224-PCXR4	691484	01/04/2026	1,000	1,500	2,000	995	1,499	1,997	1.006x - 12.384	1.000
B19	SKC	224-PCXR4	691599	01/04/2026	1,000	1,500	2,000	998	1,501	1,991	1.004x - 10.506	0.999
B20	SKC	224-PCXR4	691587	01/04/2026	1,000	1,500	2,000	997	1,495	1,998	1.003x - 7.247	1.000
B21	SKC	224-PCXR4	691531	03/04/2026	1,000	1,500	2,000	998	1,496	1,996	1.000x - 3.454	1.000
B22	SKC	224-PCXR4	691654	03/04/2026	1,000	1,500	2,000	996	1,494	1,997	0.998x - 2.784	1.000
B23	SKC	224-PCXR4	798393	02/04/2026	1,000	1,500	2,000	1,000	1,503	1,999	0.999x - 1.308	1.000
B24	SKC	224-PCXR4	626363	03/04/2026	1,000	1,500	2,000	1,001	1,509	1,995	1.002x - 6.940	0.999
B25	SKC	224-PCXR4	798489	03/04/2026	1,000	1,500	2,000	1,002	1,502	2,004	1.004x - 7.267	1.000
B26	SKC	224-PCXR4	798479	03/04/2026	1,000	1,500	2,000	996	1,503	2,003	1.006x - 12.675	1.000
B27	SKC	224-PCXR4	691673	02/04/2026	1,000	1,500	2,000	1,000	1,504	2,000	0.999x + 0.483	1.000
B28	SKC	224-PCXR4	691570	03/04/2026	1,000	1,500	2,000	997	1,510	2,001	0.998x - 0.455	0.999
B29	SKC	224-PCXR4	626472	03/04/2026	1,000	1,500	2,000	998	1,494	1,992	1.000x - 5.221	1.000
B30	SKC	224-PCXR4	691489	03/04/2026	1,000	1,500	2,000	1,008	1,504	2,006	1.003x - 2.114	1.000
B31	SKC	224-PCXR4	691509	03/04/2026	1,000	1,500	2,000	1,003	1,503	2,002	0.997x + 0.610	0.999
B32	SKC	224-PCXR4	091567	03/04/2026	1,000	1,500	2,000	1,002	1,502	1,996	0.996x + 7.008	1.000
B33	SKC	224-PCXR4	091756	03/04/2026	1,000	1,500	2,000	998	1,501	1,992	1.006x - 12.101	0.999
B34	SKC	224-PCXR4	612962	03/04/2026	1,000	1,500	2,000	1,001	1,494	2,004	1.004x - 8.196	1.000
B35	SKC	224-PCXR4	602682	03/04/2026	1,000	1,500	2,000	997	1,504	1,998	1.000x - 2.804	1.000
B36	SKC	224-PCXR4	626164	03/04/2026	1,000	1,500	2,000	996	1,512	1,996	1.001x - 5.867	0.999
B37	SKC	224-PCXR4	626256	03/04/2026	1,000	1,500	2,000	999	1,496	2,005	1.007x - 11.487	1.000
B38	SKC	224-PCXR4	626167	03/04/2026	1,000	1,500	2,000	1,002	1,500	2,003	1.008x - 16.377	0.999
B39	SKC	224-PCXR4	034637	03/04/2026	1,000	1,500	2,000	998	1,490	1,994	0.996x - 0.044	1.000
B40	SKC	224-PCXR4	798349	03/04/2026	1,000	1,500	2,000	1,001	1,501	2,000	0.995x + 0.921	0.999

Calibrated by :	Approved by :
[redacted]	[redacted]

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com., www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter	Model : Defender 510-H	S/N : 136164

Environmental Conditions

Temperature	.	25	± 3	°C
Pressure	.	1010	± 15	mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R^2
B41	SKC	224-PCXR4	612669	03/04/2026	1,000	1,500	2,000	996	1,498	1,991	1.006x - 15.132	0.999
B42	SKC	224-PCXR4	626041	03/04/2026	1,000	1,500	2,000	998	1,495	1,998	1.001x - 5.029	1.000
B43	SKC	224-PCXR4	034636	03/04/2026	1,000	1,500	2,000	996	1,512	1,995	1.000x - 4.272	0.999
B44	SKC	224-PCXR8	529341	03/04/2026	1,000	1,500	2,000	1,000	1,501	2,000	0.999x + 0.802	1.000
B45	SKC	224-PCXR8	529594	03/04/2026	1,000	1,500	2,000	996	1,495	1,999	1.003x - 8.918	1.000
B46	SKC	224-PCXR8	566743	03/04/2026	1,000	1,500	2,000	998	1,501	1,992	1.006x - 12.300	0.999
B47	SKC	224-PCXR8	566747	03/04/2026	1,000	1,500	2,000	996	1,505	2,000	1.004x - 8.392	1.000
B48	SKC	224-PCXR8	566753	03/04/2026	1,000	1,500	2,000	1,011	1,508	2,008	0.998x + 4.726	0.999
B49	SKC	224-PCXR8	566780	03/04/2026	1,000	1,500	2,000	997	1,495	1,999	1.003x - 8.045	1.000
B50	SKC	224-PCXR8	500400	03/04/2026	1,000	1,500	2,000	1,000	1,499	1,994	0.996x + 3.406	1.000
B51	SKC	224-PCXR8	500363	03/04/2026	1,000	1,500	2,000	997	1,505	1,997	1.005x - 14.055	0.999
B52	SKC	224-PCXR8	093186	03/04/2026	1,000	1,500	2,000	996	1,506	2,000	1.002x - 5.484	1.000
B53	SKC	224-PCXR8	707670	03/04/2026	1,000	1,500	2,000	993	1,505	2,001	1.009x - 20.477	0.999
B54	SKC	224-PCXR3	509821	06/04/2026	1,000	1,500	2,000	1,005	1,500	2,008	1.007x - 10.015	1.000
B55	SKC	224-PCXR3	510710	06/04/2026	1,000	1,500	2,000	1,013	1,502	2,007	1.002x - 2.573	0.999
B56	SKC	224-PCXR3	511450	06/04/2026	1,000	1,500	2,000	992	1,492	1,999	1.004x - 10.669	1.000
B57	SKC	224-PCXR3	510798	06/04/2026	1,000	1,500	2,000	999	1,496	1,996	0.998x - 0.463	1.000
B58	SKC	224-PCXR3	509852	06/04/2026	1,000	1,500	2,000	1,003	1,499	1,999	0.996x + 4.204	1.000
B59	SKC	224-PCXR3	509862	06/04/2026	1,000	1,500	2,000	1,000	1,500	1,998	0.998x + 0.850	1.000
B60	SKC	224-PCXR3	512655	06/04/2026	1,000	1,500	2,000	997	1,506	2,002	1.003x - 8.264	0.999
B61	SKC	224-PCXR3	503915	06/04/2026	1,000	1,500	2,000	999	1,505	2,006	1.004x - 6.792	1.000
B62	SKC	224-PCXR3	505975	06/04/2026	1,000	1,500	2,000	998	1,504	2,004	1.005x - 10.095	1.000
B63	SKC	224-PCXR3	511432	09/04/2026	1,000	1,500	2,000	999	1,500	1,997	0.999x - 2.345	1.000
B64	SKC	224-PCXR3	508302	09/04/2026	1,000	1,500	2,000	1,001	1,491	1,996	0.997x + 0.511	1.000
B65	SKC	224-PCXR3	508310	09/04/2026	1,000	1,500	2,000	1,002	1,509	1,994	1.000x - 4.906	0.999
B66	SKC	224-PCXR3	509861	09/04/2026	1,000	1,500	2,000	995	1,501	2,004	1.008x - 15.001	1.000
B67	SKC	224-PCXR3	506295	09/04/2026	1,000	1,500	2,000	1,002	1,500	1,999	0.998x + 1.468	1.000
B68	SKC	224-PCXR3	505872	09/04/2026	1,000	1,500	2,000	1,005	1,494	1,994	0.996x - 1.783	0.999
B69	SKC	224-PCXR3	508375	09/04/2026	1,000	1,500	2,000	997	1,505	2,005	1.009x - 17.840	0.999
B70	SKC	224-PCXR3	510623	09/04/2026	1,000	1,500	2,000	998	1,499	1,999	1.000x - 2.573	1.000
B71	SKC	224-PCXR3	508367	09/04/2026	1,000	1,500	2,000	1,002	1,503	1,989	0.997x - 0.594	0.999
B72	SKC	224-PCXR3	505977	09/04/2026	1,000	1,500	2,000	999	1,504	2,001	1.002x - 4.551	1.000
B73	SKC	224-PCXR3	512606	09/04/2026	1,000	1,500	2,000	1,001	1,502	2,002	1.000x - 1.555	1.000
B74	SKC	224-PCXR3	505993	09/04/2026	1,000	1,500	2,000	1,003	1,504	2,008	1.006x - 6.832	1.000
B75	SKC	224-PCXR3	509820	09/04/2026	1,000	1,500	2,000	1,002	1,503	1,990	1.002x - 9.465	0.999
B76	SKC	224-PCXR3	509811	09/04/2026	1,000	1,500	2,000	1,001	1,500	2,002	1.001x - 2.688	1.000
B77	SKC	224-PCXR3	508301	09/04/2026	1,000	1,500	2,000	999	1,501	1,996	0.998x + 0.550	1.000
B78	SKC	224-PCXR3	510677	09/04/2026	1,000	1,500	2,000	1,000	1,496	1,997	1.000x - 3.151	1.000
B79	SKC	224-PCXR3	510920	09/04/2026	1,000	1,500	2,000	1,002	1,502	1,986	0.997x - 2.026	0.999

Calibrated by : [redacted]	Approved by : [redacted]

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com., www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter	Model : Defender 510-H	S/N : 136164

Environmental Conditions

Temperature	.	25	± 3	°C
Pressure	.	1010	± 15	mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R^2
B80	SKC	224-PCXR3	504569	01/04/2026	1,000	1,500	2,000	1,002	1,500	2,002	0.999x - 1.161	1.000
B81	SKC	224-PCXR3	503480	01/04/2026	1,000	1,500	2,000	993	1,497	1,991	0.997x - 0.040	1.000
B82	SKC	224-PCXR3	505673	01/04/2026	1,000	1,500	2,000	1,001	1,501	1,986	0.996x + 2.864	0.999
B83	SKC	224-PCXR3	510785	01/04/2026	1,000	1,500	2,000	1,009	1,500	1,993	0.994x + 6.437	0.999
B84	SKC	224-PCXR3	508333	03/04/2026	1,000	1,500	2,000	1,003	1,502	1,990	0.999x - 3.542	0.999
B85	SKC	224-PCXR3	505757	01/04/2026	1,000	1,500	2,000	1,004	1,499	2,001	0.996x + 5.197	1.000
B86	SKC	224-PCXR3	512625	01/04/2026	1,000	1,500	2,000	1,001	1,502	1,997	0.997x + 1.603	1.000
B87	SKC	224-PCXR3	504324	01/04/2026	1,000	1,500	2,000	1,002	1,492	2,001	0.999x - 1.855	1.000
B88	SKC	224-PCXR3	508307	03/04/2026	1,000	1,500	2,000	1,011	1,501	2,003	0.997x + 4.084	0.999
B89	SKC	224-PCXR3	509860	03/04/2026	1,000	1,500	2,000	999	1,502	1,991	1.005x - 10.506	0.999
B90	SKC	224-PCXR3	508366	01/04/2026	1,000	1,500	2,000	998	1,500	2,002	1.003x - 5.376	1.000
B91	SKC	224-PCXR3	510919	01/04/2026	1,000	1,500	2,000	1,003	1,499	2,004	1.002x - 4.399	1.000
B92	SKC	224-PCXR3	510987	01/04/2026	1,000	1,500	2,000	997	1,495	2,000	1.004x - 9.780	1.000
B93	SKC	224-PCXR3	509845	03/04/2026	1,000	1,500	2,000	1,003	1,503	1,998	0.997x + 3.219	1.000

Calibrated by : [redacted]

Approved by : [redacted]

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter	Model : Defender 510-H	S/N : 136833

Environmental Conditions

Temperature	.	25	± 3	°C
Pressure	.	1010	± 15	mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R^2
R01	SKC	224-PCXR4	602467	01/04/2026	1,000	1,500	2,000	1,001	1,500	2,007	1.005x - 6.003	1.000
R02	SKC	224-PCXR4	626450	05/04/2026	1,000	2,000	3,000	1,000	1,503	2,001	1.001x - 0.383	1.000
R03	SKC	224-PCXR4	691592	03/04/2026	1,000	1,500	2,000	1,005	1,501	2,000	1.007x - 15.384	0.999
R04	SKC	224-PCXR4	691672	03/04/2026	1,000	1,500	2,000	1,007	1,513	1,999	0.996x + 5.855	0.999
R05	SKC	224-PCXR4	798470	05/04/2026	1,000	1,500	2,000	1,000	1,499	1,997	0.997x + 3.107	1.000
R06	SKC	224-PCXR4	798456	03/04/2026	1,000	1,500	2,000	998	1,497	1,996	0.998x + 0.120	1.000
R07	SKC	224-PCXR4	798480	05/04/2026	1,000	1,500	2,000	1,002	1,506	2,001	0.999x + 3.219	1.000
R08	SKC	224-PCXR4	883215	03/04/2026	1,000	1,500	2,000	1,004	1,501	1,992	1.003x - 9.877	0.999
R09	SKC	224-PCXR4	034650	03/04/2026	1,000	1,500	2,000	998	1,506	2,003	1.004x - 5.723	1.000
R10	SKC	224-PCXR4	091765	03/04/2026	1,000	1,500	2,000	999	1,507	1,996	1.005x - 13.080	0.999
R11	SKC	224-PCXR4	091763	05/04/2026	1,000	1,500	2,000	1,001	1,504	2,001	1.000x + 0.104	1.000
R12	SKC	224-PCXR4	091568	03/04/2026	1,000	1,500	2,000	998	1,505	1,996	0.998x + 1.482	1.000
R13	SKC	224-PCXR4	091638	03/04/2026	1,000	1,500	2,000	1,001	1,504	2,000	0.999x + 2.097	1.000
R14	SKC	224-PCXR4	091764	05/04/2026	1,000	1,500	2,000	1,007	1,506	2,001	1.004x - 8.866	0.999
R15	SKC	224-PCXR8	529457	05/04/2026	1,000	1,500	2,000	998	1,492	1,999	1.001x - 6.322	1.000
R16	SKC	224-PCXR8	529643	03/04/2026	1,000	1,500	2,000	1,004	1,506	2,004	1.007x - 11.726	0.999
R17	SKC	224-PCXR8	529645	05/04/2026	1,000	1,500	2,000	998	1,503	1,998	1.000x - 0.703	1.000
R18	SKC	224-PCXR8	566756	03/04/2026	1,000	1,500	2,000	999	1,508	1,995	1.002x - 8.012	0.999
R19	SKC	224-PCXR8	566802	05/04/2026	1,000	1,500	2,000	998	1,502	1,998	1.000x - 0.823	1.000
R20	SKC	224-PCXR8	529089	03/04/2026	1,000	1,500	2,000	999	1,503	1,996	0.997x + 2.001	1.000
R21	SKC	224-PCXR8	665728	03/04/2026	1,000	1,500	2,000	998	1,505	1,999	1.000x - 0.483	1.000
R22	SKC	224-PCXR8	707444	05/04/2026	1,000	1,500	2,000	1,007	1,496	2,000	1.001x - 6.418	0.999
R23	SKC	224-PCXR8	761067	05/04/2026	1,000	1,500	2,000	1,001	1,502	2,004	1.002x - 1.446	1.000
R24	SKC	224-PCXR8	707893	03/04/2026	1,000	1,500	2,000	1,002	1,503	2,001	0.999x + 2.560	1.000
R25	SKC	224-PCXR8	761052	03/04/2026	1,000	1,500	2,000	1,009	1,504	2,005	0.997x + 4.106	0.999
R26	SKC	224-PCXR8	707956	05/04/2026	1,000	1,500	2,000	1,002	1,503	2,000	0.998x + 4.497	1.000
R27	SKC	224-PCXR8	707398	03/04/2026	1,000	1,500	2,000	1,001	1,505	2,004	1.003x - 1.921	1.000
R28	SKC	224-PCXR8	707481	05/04/2026	1,000	1,500	2,000	1,010	1,513	2,006	0.997x + 5.531	0.999
R29	SKC	224-PCXR8	707402	03/04/2026	1,000	1,500	2,000	1,003	1,502	1,992	1.003x - 10.216	0.999
R30	SKC	224-PCXR8	093811	05/04/2026	1,000	1,500	2,000	999	1,512	2,005	1.007x - 9.705	1.000
R31	SKC	224-PCXR8	093183	05/04/2026	1,000	1,500	2,000	1,011	1,510	2,011	1.001x + 2.983	0.999
R32	SKC	224-PCXR8	671950	03/04/2026	1,000	1,500	2,000	1,001	1,500	2,001	0.999x + 2.272	1.000
R33	SKC	224-PCXR4	626254	05/04/2026	1,000	1,500	2,000	998	1,507	2,002	1.005x - 10.975	1.000
R34	SKC	224-PCXR4	626131	05/04/2026	1,000	1,500	2,000	997	1,496	2,000	1.007x - 14.230	1.000
R35	SKC	224-PCXR8	707460	05/04/2026	1,000	1,500	2,000	998	1,509	1,996	1.000x - 2.915	1.000
R36	SKC	224-PCXR8	707446	05/04/2026	1,000	1,500	2,000	1,003	1,492	2,003	1.007x - 16.135	0.999
R37	SKC	224-PCXR8	707432	03/04/2026	1,000	1,500	2,000	999	1,507	2,005	1.003x - 6.095	1.000
R38	SKC	224-PCXR8	707349	03/04/2026	1,000	1,500	2,000	1,003	1,499	1,999	0.997x + 2.141	1.000
R39	SKC	224-PCXR8	761095	05/04/2026	1,000	1,500	2,000	1,005	1,508	2,004	1.000x - 0.152	0.999

Calibrated by : [redacted]	Approved by : [redacted]

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H | S/N : 136833

Environmental Conditions

Temperature	.	25	± 3	°C
Pressure	.	1010	± 15	mmbar

Personal Pump Data				Calibration Data							
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R^2
R40	SKC	224-PCXR4	612753	05/04/2026	1,000	1,500	2,000	1,004	1,497	2,000	0.998x + 1.430	1.000
R41	SKC	224-PCXR4	626140	03/04/2026	1,000	1,500	2,000	998	1,498	1,997	0.999x + 0.943	1.000
R42	SKC	224-PCXR4	626463	05/04/2026	1,000	1,500	2,000	1,005	1,513	1,998	0.997x + 4.138	0.999
R43	SKC	224-PCXR4	626129	03/04/2026	1,000	1,500	2,000	1,003	1,498	2,000	0998x + 2.029	1.000
R44	SKC	224-PCXR4	602753	03/04/2026	1,000	1,500	2,000	996	1,509	1,997	1.003x - 8.036	1.000
R45	SKC	224-PCXR4	626137	05/04/2026	1,000	1,500	2,000	1,011	1,514	2,005	0.995x + 8.367	0.999

Calibrated by : [redacted]
(Mr. Adul Dangklom)

Approved by : [redacted]

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Rotameter Calibration Report (For Personal Pump High Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter	Model : Defender 510-H	S/N : 136833

Calibration Data											
Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (ml/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R^2
H-R01	Dwyer	VFB-65	05/01/2026	500	1,000	2,000	503.6	992.4	1980.9	0.999x - 3.140	0.999
H-R02	Dwyer	VFB-65	06/01/2026	500	1,000	2,000	500.8	995.8	1986.2	1.002x - 5.343	1.000
H-R03	Dwyer	VFB-65	05/01/2026	500	1,000	2,000	495.3	992.1	1982.9	1.004x - 17.510	0.999
H-R04	Dwyer	VFB-65	05/01/2026	500	1,000	2,000	496.4	994.6	2019.5	1.007x - 11.385	1.000
H-R05	Dwyer	VFB-65	06/01/2026	500	1,000	2,000	497.2	991.5	1987.3	1.003x - 7.563	1.000
H-R06	Dwyer	VFB-65	06/01/2026	500	1,000	2,000	501.1	992.4	1982.9	1.001x - 6.139	0.999

Calibrated by : [redacted]	Approved by : [redacted]

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Rotameter Calibration Report (For Personal Pump High Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter	Model : Defender 510-H	S/N : 136833

Calibration Data

Rotameter Data			Calibration Data							
No.	Brand	Model	Date	Flow Rate (ml/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R^2
H-R01	Dwyer	VFB-65	01/04/2026	500	1,000	2,000	499.7	1000.6	1996.7	1.000x - 0.544	1.000
H-R02	Dwyer	VFB-65	01/04/2026	500	1,000	2,000	501.2	992.4	1990.0	1.001x - 5.362	0.999
H-R03	Dwyer	VFB-65	03/04/2026	500	1,000	2,000	501.4	997.5	1997.3	0.998x + 2.606	1.000
H-R04	Dwyer	VFB-65	05/04/2026	500	1,000	2,000	502.5	993.6	1985.2	0.999x - 2.085	0.999
H-R05	Dwyer	VFB-65	05/04/2026	500	1,000	2,000	500.4	1001.3	1999.8	1.000x + 1.247	1.000
H-R06	Dwyer	VFB-65	03/04/2026	500	1,000	2,000	500.8	997.2	1994.6	0.999x - 0.348	1.000

Calibrated by : [redacted]

Approved by : [redacted]

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Rotameter Calibration Report (For Personal Pump Low Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter	Model : Defender 510-H	S/N : 136833

Calibration Data

Rotameter Data			Calibration Data							
No.	Brand	Model	Date	Flow Rate (ml/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R^2
L-R01	Dwyer	VFA-21	05/01/2026	50	100	200	50.2	102.0	203.9	0.991x + 2.329	1.000
L-R02	Dwyer	VFA-21	05/01/2026	50	100	200	50.4	101.3	200.5	1.006x - 0.627	0.999
L-R03	Dwyer	VFA-21	06/01/2026	50	100	200	50.1	99.4	202.7	1.017x - 1.144	1.000
L-R04	Dwyer	VFA-21	06/01/2026	50	100	200	49.8	100.5	201.0	1.010x - 1.541	0.999
L-R05	Dwyer	VFA-21	05/01/2026	50	100	200	50.2	101.4	203.8	0.990x + 2.384	1.000
L-R06	Dwyer	VFA-21	06/01/2026	50	100	200	50.4	99.1	201.5	1.003x - 0.197	1.000

Calibrated by : [redacted]

Approved by : [redacted]

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Rotameter Calibration Report (For Personal Pump Low Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter	Model : Defender 510-H	S/N : 136833

Calibration Data

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (ml/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R^2
L-R01	Dwyer	VFA-21	01/04/2026	50	100	200	50.3	101.1	201.9	0.998x + 0.955	1.000
L-R02	Dwyer	VFA-21	01/04/2026	50	100	200	50.2	101.7	201.0	0.999x + 0.367	0.999
L-R03	Dwyer	VFA-21	03/04/2026	50	100	200	50.3	101.2	201.0	1.001x + 0.605	1.000
L-R04	Dwyer	VFA-21	05/04/2026	50	100	200	50.7	100.8	200.2	1.000x + 0.719	1.000
L-R05	Dwyer	VFA-21	05/04/2026	50	100	200	50.1	101.2	200.5	1.001x - 0.213	0.999
L-R06	Dwyer	VFA-21	03/04/2026	50	100	200	50.3	100.8	200.1	0.999x + 0.639	1.000

Calibrated by : [redacted]

Approved by : [redacted]

QUALITY CALIBRATION CO.,LTD.
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584
www.qcalibration.com

NSC-TISI-TIS17025
CALIBRATION 0049

CERTIFICATE No : 25M2254
REFERENCE No : 76365-1

Certificate of Calibration

EQUIPMENT	:	DIGITAL BALANCE
MANUFACTURER	:	METTLER TOLEDO
MODEL	:	XS105DU
SERIAL No	:	1126422905
ID No	:	BA05/50
CONDITION AS RECEIVED	:	USED ITEM
SUBMITTED BY	:	S.P.S. CONSULTING SERVICE CO., LTD. 7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD., JOMPOL, CHATUCHAK, BANGKOK 10900
CALIBRATED BY	:	ATSAWIN Y.
CALIBRATION DATE	:	07-Mar-25
APPROVED BY	:	[redacted]
ISSUED DATE	:	13-Mar-25
RECEIVED DATE	:	07-Mar-25

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF QUALITY CALIBRATION CO., LTD.

QUALITY CALIBRATION CO.,LTD.
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584
www.qcalibration.com

CERTIFICATE No : 25M2254

Calibration Report

EQUIPMENT	:	DIGITAL BALANCE	**MODEL**	:	XS105DU
MANUFACTURER	:	METTLER TOLEDO	**S/N**	:	1126422905
ID No	:	BA05/50	**RECEIVED DATE**	:	07-Mar-25
AIR PRESSURE	:	1009mbar ± 1mbar	**CALIBRATION DATE**	:	07-Mar-25
AMBIENT TEMPERATURE	:	24° C ± 1° C	**RELATIVE HUMIDITY**	:	54 %RH ± 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARLITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.
2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	C02250116	28-Jan-27
2) STANDARD WEIGHT	E2	15843	C02250117	29-Jan-27


3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
   - NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL
2. TARE FUNCTION : NORMAL
3. REPEATABILITY OF READING AT 120 g WAS 0.000055 g
4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (± g)
0.00	0.00000	0.00000	0.000065
0.02	0.01999	0.00001	0.000065
0.10	0.10001	-0.00001	0.000066
0.20	0.20001	-0.00001	0.000066
0.50	0.50002	-0.00002	0.000065
1.00	1.00003	-0.00003	0.000066
2.00	2.00001	-0.00001	0.000067
5.00	5.00002	-0.00002	0.000068
10.00	10.00000	0.00000	0.000070
20.00	20.00004	-0.00004	0.000078
50.00	50.0000	0.0000	0.00013
100.00	100.0001	-0.0001	0.00019
120.00	120.0002	-0.0002	0.00022

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.0000
2	50.0000
3	50.0000
4	50.0000
5	50.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k =2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

QUALITY CALIBRATION CO.,LTD.
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584
www.qcalibration.com

NSC-TISI-TIS17025
CALIBRATION 0049

CERTIFICATE No : 26M2266
REFERENCE No : 80204-1

Certificate of Calibration

EQUIPMENT	:	DIGITAL BALANCE
MANUFACTURER	:	METTLER TOLEDO
MODEL	:	XS105DU
SERIAL No	:	1126422905
ID No	:	BA 05/50
CONDITION AS RECEIVED	:	USED ITEM
SUBMITTED BY	:	S.P.S. CONSULTING SERVICE CO., LTD. 7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD., JOMPOL, CHATUCHAK, BANGKOK 10900
CALIBRATED BY	:	SUCHAT S.
CALIBRATION DATE	:	05-Mar-26
APPROVED BY	:	[redacted]
ISSUED DATE	:	06-Mar-26
RECEIVED DATE	:	05-Mar-26

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF QUALITY CALIBRATION CO., LTD.

QUALITY CALIBRATION CO.,LTD.
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584
www.qcalibration.com

CERTIFICATE No : 26M2266

Calibration Report

EQUIPMENT	:	DIGITAL BALANCE	**MODEL**	:	XS105DU
MANUFACTURER	:	METTLER TOLEDO	**S/N**	:	1126422905
ID No	:	BA 05/50	**RECEIVED DATE**	:	05-Mar-26
AIR PRESSURE	:	1004mbar ± 1mbar	**CALIBRATION DATE**	:	05-Mar-26
AMBIENT TEMPERATURE	:	25° C ± 1° C	**RELATIVE HUMIDITY**	:	50 %RH ± 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARLITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.
2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	C02250116	28-Jan-27
2) STANDARD WEIGHT	E2	15843	C02250117	29-Jan-27


3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
   - NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL
2. TARE FUNCTION : NORMAL
3. REPEATABILITY OF READING AT 120 g WAS 0.000055 g
4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (± g)
0.00	0.00000	0.00000	0.000065
0.02	0.02000	0.00000	0.000065
0.10	0.10000	0.00000	0.000066
0.20	0.20000	0.00000	0.000066
0.50	0.50001	-0.00001	0.000065
1.00	1.00001	-0.00001	0.000066
2.00	2.00000	0.00000	0.000067
5.00	5.00001	-0.00001	0.000068
10.00	10.00004	-0.00004	0.000070
20.00	20.00006	-0.00006	0.000078
50.00	50.0000	0.0000	0.00012
100.00	100.0002	-0.0002	0.00019
120.00	120.0002	-0.0002	0.00022

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.0000
2	50.0000
3	50.0000
4	50.0000
5	50.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k =2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

[redacted]

GC Clarus 600/680 Preventive Maintenance (PM)

Company Name:	**S.P.S. Consulting Service Co.,Ltd**		
Address (Instrument Location):	7 Soi Phaholyothin24 Phaholyothin Road, Jompol, Chatuchak, Bangkok, 10900.		
Serial Number:	680S14042502	**Service Tag:**	N68APSSFXMP
Customer Name (if applicable):	Ms.Naruecha	**PM number:**	2 of 2
Service Engineer Name:	Monchai Kitcharoenkeat	**Service Order Number:**	WO-06815714
Date PM Performed: (DD-MMM-YYYY)	13-Aug-2025	**Next PM Due Date:** (DD-MMM-YYYY)	13-Feb-2026

Part Number	Release	Publication Date
TH09370070	C	August 2016

Scope

The purpose of this PM is to ensure the continued functionality of the Clarus 600 and Clarus 680 GC by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer. The customer should save their method before the PM begins.

General Instructions:

The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM. Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files. The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer. Update the PM sticker and instrument logbook as required.

Copyright Information

This document contains proprietary information that is protected by copyright. All rights are reserved. No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of Perkin Elmer, Inc. **Copyright © 2013 PerkinElmer, Inc.**

Trademarks

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners. **Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no Warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.** PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

Component List

Component / Specific Model	Serial #	Software Version	Configuration Notes
Clarus680	680S14042502	Totalchrom6.3.2	PSS, PSS, FID,
Clarus SQ8T	648N4050804	Turbomass 6.4	
AtomX	US14113002	Tekma AtomX	

Parts Lists

Additional Tools Required for PM				
Part Number (if applicable)	**Description**	**Quantity**	**Serial #**	**Calibration Due Date (MM/YY)**
N/A				
Additional Reagents and Standards Required for PM				
Part Number (if applicable)	**Description**	**Quantity**	**Batch/Lot #**	**Expiration Date (MM/YY)**
N/A				

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. General:

☑ Review the instrument performance with the customer and document any recent problems.

☑ Check incoming AC line voltage for proper levels and grounding.
L-N 220 Volt
L-G 220 Volt
N-G 0.32 Volt

**Neutral to ground not more than 0.5 volts peak to peak*

☑ Inspect all gas line filters and traps; Replace if necessary with customer supplied spares.
Carrier gas ☑ Helium ☐ Nitrogen ☐ Hydrogen
Moisture level ☑ Good ☐ Need to replace ☐ Other _____

Detector gas ☑ Air Zero ☑ Hydrogen ☐ Nitrogen ☐ Helium
Moisture level ☑ Good ☐ Need to replace ☐ Other _____

☑ Inspect the customer log book and make any appropriate PM entries.

☑ Leak check all fittings from the gas source to instrument.
Gas leakage ☑ Pass ☐ Fail Comment _____

☑ Perform general inspection of system for cleanliness.

☑ Inspect for functional and clean electronic cooling and oven vent fans
Electronic cooling fan ☑ Yes ☐ No
Oven cooling fan ☑ Yes ☐ No

2. Electronic :

☑ Check oven temperature. Calibrate if necessary.
Oven temperature set point 150 ^{0}C ☑ Pass ☐ Fail

☐ Check sub-ambient option. (If installed).
Oven temperature set point 5 ^{0}C ☐ Pass ☐ Fail

☑ Perform routine maintenance on detector/injector. Replace parts as necessary with customer supplied spares.

☑ Check flows, including split flows if applicable. Calibrate if necessary.
Carrier flow Pass
Split flow Pass

☑ Check detector gas flows and adjust if necessary.
Detector flow Pass

☑ Autosampler installed ☑ Yes ☐ No
Check autosampler sensor for wear and replace if necessary.
Vial sensor Pass
Door sensor Pass
Tower sensor Pass
Plunger sensor Pass
Elevator sensor Pass

☑ Remove syringe, manually flush. Replace with customer supplied spare if necessary.

☑ Check firmware version. Upgrade to current levels if necessary.
Firmware version 6.5

☑ Measure all accessible power supply voltages.
5 Volt Pass
+15 Volt Pass
-15 Volt Pass
24 Volt Pass

☑ Record all detector voltage signal.
Detector Channel A 0.98 mV.
Detector Channel B NA mV.

3. Diagnostics Tests:

☑ Run instrument diagnostics.
☑ BRAM Pass
☑ EPROM Pass

☑ Run Autosampler diagnostics.
☑ BRAM Pass
☑ EPROM Pass

4. Review:

☑ Review with the customer PM work performed.
☑ Review with the customer routine maintenance procedures.
☑ Discuss recommended customer-supplied materials to have on hand
☑ Attach PM sticker.
☑ Update Logbook.

Additional Comments

Additional Comments Regarding the PM

Review

The preventive maintenance checks and if applicable performance tests for Clarus600/680 GC have been completed. ***This Clarus600/680 GC*** **Pass** ***the preventive maintenance.***	
Review of Preventive Maintenance:	
Authorized PerkinElmer Representative: Monchai Kitcharoenkeat Monchai	Date: 13-Aug-2025 (DD-MMM-YYYY)
Authorized Customer Representative: Ms.Naruecha Naruecha	Date: 13-Aug-2025 (DD-MMM-YYYY)

GC Clarus 600/680 Preventive Maintenance (PM)

Company Name:	**S.P.S. Consulting Service Co.,Ltd**		
Address (Instrument Location):	7 Soi Phaholyothin24 Phaholyothin Road, Jompol, Chatuchak, Bangkok, 10900.		
Serial Number:	680S14042502	**Service Tag:**	N68APSSFXMP
Customer Name (if applicable):	Ms.Naruecha	**PM number:**	1 of 2
Service Engineer Name:	Monchai Kitcharoenkeat	**Service Order Number:**	WO-11858723
Date PM Performed: (DD-MMM-YYYY)	13-Feb-2026	**Next PM Due Date:** (DD-MMM-YYYY)	13-Aug-2026

Part Number	Release	Publication Date
TH09370070	C	August 2016

Scope

The purpose of this PM is to ensure the continued functionality of the Clarus 600 and Clarus 680 GC by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer. The customer should save their method before the PM begins.

General Instructions:

The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM. Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files. The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer. Update the PM sticker and instrument logbook as required.

Copyright Information

This document contains proprietary information that is protected by copyright. All rights are reserved. No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of Perkin Elmer, Inc. **Copyright © 2013 PerkinElmer, Inc.**

Trademarks

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners. **Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no Warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.** PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

Component List

Component / Specific Model	Serial #	Software Version	Configuration Notes
Clarus680	680S14042502	Totalchrom6.3.2	PSS, PSS, FID,
Clarus SQ8T	648N4050804	Turbomass 6.4	
AtomX	US14113002	Tekma AtomX	

Parts Lists

Additional Tools Required for PM				
Part Number (if applicable)	**Description**	**Quantity**	**Serial #**	**Calibration Due Date (MM/YY)**
N/A				
Additional Reagents and Standards Required for PM				
Part Number (if applicable)	**Description**	**Quantity**	**Batch/Lot #**	**Expiration Date (MM/YY)**
N/A				

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. General:

☑ Review the instrument performance with the customer and document any recent problems.

☑ Check incoming AC line voltage for proper levels and grounding.
L-N 220 Volt
L-G 220 Volt
N-G 0.46 Volt

**Neutral to ground not more than 0.5 volts peak to peak*

☑ Inspect all gas line filters and traps; Replace if necessary with customer supplied spares.
Carrier gas ☑ Helium ☐ Nitrogen ☐ Hydrogen
Moisture level ☑ Good ☐ Need to replace ☐ Other _____

Detector gas ☑ Air Zero ☑ Hydrogen ☐ Nitrogen ☐ Helium
Moisture level ☑ Good ☐ Need to replace ☐ Other _____

☑ Inspect the customer log book and make any appropriate PM entries.

☑ Leak check all fittings from the gas source to instrument.
Gas leakage ☑ Pass ☐ Fail Comment _____

☑ Perform general inspection of system for cleanliness.

☑ Inspect for functional and clean electronic cooling and oven vent fans
Electronic cooling fan ☑ Yes ☐ No
Oven cooling fan ☑ Yes ☐ No

2. Electronic :

☑ Check oven temperature. Calibrate if necessary.
Oven temperature set point 150 ^{0}C ☑ Pass ☐ Fail

☐ Check sub-ambient option. (If installed).
Oven temperature set point 5 ^{0}C ☐ Pass ☐ Fail

☑ Perform routine maintenance on detector/injector. Replace parts as necessary with customer supplied spares.

☑ Check flows, including split flows if applicable. Calibrate if necessary.
Carrier flow Pass
Split flow Pass

☑ Check detector gas flows and adjust if necessary.
Detector flow Pass

☑ Autosampler installed ☑ Yes ☐ No
Check autosampler sensor for wear and replace if necessary.
Vial sensor Pass
Door sensor Pass
Tower sensor Pass
Plunger sensor Pass
Elevator sensor Pass

☑ Remove syringe, manually flush. Replace with customer supplied spare if necessary.

☑ Check firmware version. Upgrade to current levels if necessary.
Firmware version 6.5

☑ Measure all accessible power supply voltages.
5 Volt Pass
+15 Volt Pass
-15 Volt Pass
24 Volt Pass

☑ Record all detector voltage signal.
Detector Channel A 0.87 mV.
Detector Channel B NA mV.

3. Diagnostics Tests:

☑ Run instrument diagnostics.
☑ BRAM Pass
☑ EPROM Pass

☑ Run Autosampler diagnostics.
☑ BRAM Pass
☑ EPROM Pass

4. Review:

☑ Review with the customer PM work performed.
☑ Review with the customer routine maintenance procedures.
☑ Discuss recommended customer-supplied materials to have on hand
☑ Attach PM sticker.
☑ Update Logbook.

Additional Comments

Additional Comments Regarding the PM

Review

The preventive maintenance checks and if applicable performance tests for Clarus600/680 GC have been completed. ***This Clarus600/680 GC*** **Pass** ***the preventive maintenance.***	
Review of Preventive Maintenance:	
Authorized PerkinElmer Representative: Monchai Kitcharoenkeat	Date: 13-Feb-2026 (DD-MMM-YYYY)
Authorized Customer Representative: Ms.Naruecha	Date: 13-Feb-2026 (DD-MMM-YYYY)