

ภาคผนวกที่ 4

เอกสารสอบเทียบความถูกต้องของเครื่องมือตรวจวัดคุณภาพสิ่งแวดล้อม

ลำดับที่ 1	คุณภาพอากาศในบรรยากาศทั่วไป
ลำดับที่ 2	คุณภาพอากาศจากปล่องระบายอากาศ
ลำดับที่ 3	ระดับเสียงในบรรยากาศ
ลำดับที่ 4	คุณภาพน้ำเสียอุตสาหกรรม
ลำดับที่ 5	คุณภาพน้ำผิวดิน
ลำดับที่ 6	คุณภาพน้ำใต้ดิน
ลำดับที่ 7	ระดับเสียงในสถานที่ทำงาน

**ตารางสรุปรายการเอกสารการสอบเทียบความถูกต้องของเครื่องมือเก็บตัวอย่าง
และเครื่องมือตรวจวิเคราะห์คุณภาพสิ่งแวดล้อม**

รายการตรวจวัด	เครื่องมือเก็บตัวอย่าง	เครื่องมือตรวจวิเคราะห์
	ชื่อเครื่องมือ	ชื่อเครื่องมือ
1. คุณภาพอากาศในบรรยากาศ		
Total Suspended Particulate	High Volume Air Sampler Blower & Recorder No. R01, R10, R11	Digital Balance
SO ₂	Serial No. 3488, TRS1068, 76	Serial No. 3488, TRS1068, 76
NO ₂	Serial No. 4410, 4413, 1991	Serial No. 4410, 4413, 1991
2. คุณภาพอากาศจากปล่อง		
Total Suspended Particulate	Console No. R03, R04, R05 Pitot Tube No. B21, B24, B33, B36	Digital Balance
NO ₂	Vacuum Gauge	Spectrophotometer
SO ₂	Personal Pump SKC No. R45 Rotameter No. H-R02	-
CO	Personal Pump SKC No. R30 Rotameter No. H-R02	CO Analyzer No. R02
Styrene	Personal Pump SKC No. B61, B78, R05, R11, R13, R14, R15, R19, R21, R22, R26, R28, R30, R32, R34, R35, R36, R38, Rotameter No. L-R02, L-R03	GC/FID
Ethylbenzene	Personal Pump SKC No. B61, B78, R05, R11, R13, R14, R15, R19, R20, R21, R22, R26, R28, R30, R32, R34, R35, R36, R38, Rotameter No. L-R02, L-R03	GC/FID
3. ระดับเสียงในบรรยากาศ		
L _{eq} 5 min, L _{eq} 1 hr., L _{eq} 24 hrs., L _{max} , L ₉₀	Acoustic Calibrator Sound Level Meter ACO-R45	-
4. คุณภาพน้ำเสียอุตสาหกรรม		
pH	-	pH Meter
BOD ₅	-	BOD Analyzer
COD	-	COD Reactor
TSS	-	Digital Balance
TDS	-	Digital Balance

รายการตรวจวัด	เครื่องมือเก็บตัวอย่าง	เครื่องมือตรวจวิเคราะห์
	ชื่อเครื่องมือ	ชื่อเครื่องมือ
4. คุณภาพน้ำเสียอุตสาหกรรม (ต่อ)		
Free Chlorine	-	Spectrophotometer
Phosphate	-	Spectrophotometer
Zinc	-	AAS
Grease & Oil	-	Digital Balance
Conductivity	-	Conductivity Meter
5. คุณภาพน้ำผิวดิน		
pH	-	pH Meter
TDS	-	Digital Balance
TSS	-	Digital Balance
BOD ₅	-	BOD Analyzer
COD	-	COD Reactor
Grease & Oil	-	Digital Balance
Total Coliform Bacteria	-	Incubator
Phenol	-	Spectrophotometer
Nitrate	-	Spectrophotometer
Hexavalent Chromium	-	Spectrophotometer
Cadmium	-	AAS
Copper	-	AAS
Lead	-	AAS
Mercury	-	AAS
Manganese	-	AAS
Nickel	-	AAS
Zinc	-	AAS
6. คุณภาพน้ำใต้ดิน		
pH	-	pH Meter
Styrene	-	GCMS
Ethylbenzene	-	GCMS
7. ระดับเสียงในสถานที่ทำงาน		
Leq 8 hr, TWA	Acoustic Calibrator Sound Level Meter ACO- B43, R30, R40, R41	-

ลำดับที่ 1

คุณภาพอากาศในบรรยากาศทั่วไป



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com., www.spscon.com

High Volume Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard

Model : TE 5025A

S/N : 3611

Calibration Data

High Volume Air Sampler Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (ft ³ /min)	R ²
B35	B35	06/05/2026	$y = 1.130x - 2.698$	0.999
B36	B36	05/05/2026	$y = 1.112x - 2.644$	0.998
B37	B37	05/05/2026	$y = 1.124x - 2.608$	0.996
B38	B38	06/05/2026	$y = 1.139x - 1.817$	0.999
B39	B39	05/05/2026	$y = 1.099x + 0.749$	0.997
B40	B40	05/05/2026	$y = 1.135x - 2.517$	0.997
B41	B41	06/05/2026	$y = 1.103x - 0.803$	0.998
B42	B42	05/05/2026	$y = 1.138x - 3.754$	0.999
B43	B43	06/05/2026	$y = 1.132x - 2.425$	0.997
B44	B44	06/05/2026	$y = 1.128x - 2.443$	0.998
R01	R01	07/05/2026	$y = 1.103x - 2.879$	0.997
R02	R02	02/05/2026	$y = 1.130x - 2.934$	0.997
R03	R03	05/05/2026	$y = 1.124x - 2.685$	0.996
R04	R04	05/05/2026	$y = 1.114x - 0.914$	0.998
R05	R05	06/05/2026	$y = 1.059x + 0.368$	0.998
R06	R06	06/05/2026	$y = 1.088x + 0.020$	0.996
R07	R07	06/05/2026	$y = 1.122x - 2.809$	0.996
R08	R08	05/05/2026	$y = 1.101x - 1.418$	0.999
R09	R09	05/05/2026	$y = 1.084x + 0.212$	0.997
R10	R10	05/05/2026	$y = 1.104x - 2.080$	0.998
R11	R11	06/05/2026	$y = 1.112x - 2.545$	0.999
R12	R12	05/05/2026	$y = 1.119x - 0.906$	0.997
R13	R13	05/05/2026	$y = 1.116x - 3.391$	0.997
R14	R14	02/05/2026	$y = 1.080x - 1.101$	0.996
R15	R15	06/05/2026	$y = 1.095x - 0.708$	0.998
R16	R16	02/05/2026	$y = 1.104x - 1.452$	0.997
R17	R17	06/05/2026	$y = 1.102x - 1.932$	0.998
R18	R18	02/05/2026	$y = 1.128x - 4.180$	0.997
R19	R19	02/05/2026	$y = 1.090x - 3.037$	0.996
R20	R20	06/05/2026	$y = 1.130x - 2.859$	0.999

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :


(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT					
CHEMILUMINESCENT NO / NO ₂ / NO _x ANALYZER					
DATE :	10 May 2026	BRAND :	API	MODEL :	200E
NO.	NOX-R03	SERIAL NO.	4410		
Calibrator (Dilution System)					
Brand	: Teledyne			Model	: 700
Last Cal. Date	: 24 October 2025			Serial No.	: 421
Reference Standard Gas					
Standard Gas	: Nitric Oxide (NO)			Cylinder No.	: A00674SV
Certified Date	: 12 March 2025	Expired Date	: 12 March 2028	Cylinder Conc.	: 48.7 ppm
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.6	°C
% RH 50					
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.10	-	0	-
NO Span	400	399.7	-0.075	400.0	1.004
NO _x Span	400	399.9	-0.025	400.0	1.008
API Model 200E NO _x Analyzer Check List					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	500 standard		
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air		
SAMPLE FLOW	510	cc/min	500 ± 50		
OZONE FLOW	79	cc/min	80 ± 15		
PMT	103.4	mV	-20 - 150		
AZERO	94.0	mV	-20 - 150		
HVPS	675	V	420 - 900 constant		
RCELL TEMP	50.1	°C	50 ± 1		
BOX TEMP	29.0	°C	8 - 48		
PMT TEMP	7.5	°C	7 ± 2		
MOLY TEMP	314.8	°C	315 ± 5		
RCELL PRESS	8.4	IN-Hg-A	2 - 10 constant		
SAMPLE PRESS	28.7	IN-Hg-A	25 - 30 constant		
NO Span Conc	400	PPB	20 - 20,000		
NO _x Span Conc	400	PPB	20 - 20,000		
NO Slope	1.004	-	1.0 ± 0.3		
NO _x Slope	1.008	-	1.0 ± 0.3		
NO Offset	1.1	mV	-20 to +150		
NO _x Offset	0.6	mV	-20 to 150		
Stability at Zero	0.1	PPB	< 0.2		
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas		

Calibrated by :

Heeson L.
(Mr. Heeson Lormae)

Approved by :

Yuthana J.
(Mr. Yuthana Tanatharanit)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT						
CHEMILUMINESCENT NO / NO ₂ / NO _x ANALYZER						
DATE :	10 May 2026	BRAND :	API	MODEL :	200E	
NO.	NOX-R05	SERIAL NO.	4413			
Calibrator (Dilution System)						
Brand	: Teledyne			Model	: 700	
Last Cal. Date	: 24 October 2025			Serial No.	: 421	
Reference Standard Gas						
Standard Gas	: Nitric Oxide (NO)			Cylinder No.	: A00674SV	
Certified Date	: 12 March 2025	Expired Date	: 12 March 2028	Cylinder Conc.	: 48.7 ppm	
CALIBRATING CONDITION						
Pressure	1011	mmbar	Temp.	24.6	°C	
% RH						50
CALIBRATION SETTING						
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB		
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope	
Zero	0	0.11	-	0	-	
NO Span	400	399.7	-0.075	400.0	1.006	
NO _x Span	400	400.2	0.050	400.0	1.009	
API Model 200E NO _x Analyzer Check List						
Test Values	Observed Value	Units	Nominal Range			
RANGE	500	PPB	500 standard			
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air			
SAMPLE FLOW	505	cc/min	500 ± 50			
OZONE FLOW	78	cc/min	80 ± 15			
PMT	103.0	mV	-20 - 150			
AZERO	93.7	mV	-20 - 150			
HVPS	670	V	420 - 900 constant			
RCELL TEMP	50.3	°C	50 ± 1			
BOX TEMP	29.5	°C	8 - 48			
PMT TEMP	7.1	°C	7 ± 2			
MOLY TEMP	314.8	°C	315 ± 5			
RCELL PRESS	8.3	IN-Hg-A	2 - 10 constant			
SAMPLE PRESS	28.6	IN-Hg-A	25 - 30 constant			
NO Span Conc	400	PPB	20 - 20,000			
NO _x Span Conc	400	PPB	20 - 20,000			
NO Slope	1.006	-	1.0 ± 0.3			
NO _x Slope	1.009	-	1.0 ± 0.3			
NO Offset	1.2	mV	-20 to +150			
NO _x Offset	0.7	mV	-20 to 150			
Stability at Zero	0.1	PPB	< 0.2			
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas			

Calibrated by :

Heeson L.
(Mr. Heeson Lormae)

Approved by :

Yuthana J.
(Mr. Yuthana Tanatharanit)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT						
CHEMILUMINESCENT NO / NO ₂ / NO _x ANALYZER						
DATE :	10/5/2026	BRAND :	API	MODEL :	200E	
NO.	NOX-R10	SERIAL NO.	1991			
Calibrator (Dilution System)						
Brand	: Teledyne			Model	: 700	
Last Cal. Date	: 24 October 2025			Serial No.	: 421	
Reference Standard Gas						
Standard Gas	: Nitric Oxide (NO)			Cylinder No.	: A00674SV	
Certified Date	: 12 March 2025	Expired Date	: 12 March 2028	Cylinder Conc.	: 48.7 ppm	
CALIBRATING CONDITION						
Pressure	1011	mmbar	Temp.	24.6	°C	
% RH						50
CALIBRATION SETTING						
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB		
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope	
Zero	0	-0.10	-	0	-	
NO Span	400	400.1	0.025	400.0	1.007	
NO _x Span	400	400.2	0.050	400.0	1.010	
API Model 200E NO _x Analyzer Check List						
Test Values	Observed Value	Units	Nominal Range			
RANGE	500	PPB	500 standard			
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air			
SAMPLE FLOW	511	cc/min	500 ± 50			
OZONE FLOW	79	cc/min	80 ± 15			
PMT	103.2	mV	-20 - 150			
AZERO	94.0	mV	-20 - 150			
HVPS	671	V	420 - 900 constant			
RCELL TEMP	50.2	°C	50 ± 1			
BOX TEMP	29.3	°C	8 - 48			
PMT TEMP	7.5	°C	7 ± 2			
MOLY TEMP	315.4	°C	315 ± 5			
RCELL PRESS	8.2	IN-Hg-A	2 - 10 constant			
SAMPLE PRESS	28.5	IN-Hg-A	25 - 30 constant			
NO Span Conc	400	PPB	20 - 20,000			
NO _x Span Conc	400	PPB	20 - 20,000			
NO Slope	1.007	-	1.0 ± 0.3			
NO _x Slope	1.010	-	1.0 ± 0.3			
NO Offset	1.5	mV	-20 to +150			
NO _x Offset	0.9	mV	-20 to 150			
Stability at Zero	0.1	PPB	< 0.2			
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas			

Calibrated by :

Heeson L.
(Mr. Heeson Lormae)

Approved by :

Yuthana J.
(Mr. Yuthana Tanathananit)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT					
SO ₂ FLUORESCENT ANALYZER					
DATE :	10 May 2026	BRAND :	API	MODEL :	100E
NO.	SO ₂ -R03			SERIAL NO.	3488
Calibrator (Dilution System)					
Brand : Teledyne			Model : 700		
Last Cal. Date : 24 October 2025			Serial No. : 421		
Reference Standard Gas					
Standard Gas : Sulphur Dioxide (SO ₂)			Cylinder No. : A00814SK		
Certified Date : 21 June 2021		Expired Date : 21 June 2029		Cylinder Conc. : 49.8 ppm	
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.6	°C
			% RH	50	
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.10	-	0	-
SO ₂ Span	400.0	400.1	0.025	400.0	1.011
API Model TML-50 SO ₂ Analyzer Check list					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	0-500		
SAMPLE PRESS	28.4	in-Hg	25-35		
SAMPLE FLOW	656	cc/min	650 ± 10%		
PMT	103.5	mV	-20-150 with Zero Air		
UV LAMP	3050.3	mV	1000-4900		
STR. LGT	61.7	PPB	<100		
DRK PMT	63.1	mV	-50 - 200		
DRK LMP	57.9	mV	-50 - 200		
HVPS	669	V	550-900 constant		
DCPS	2514	mV	2500 ± 200		
RCELL TEMP	50.3	°C	50 ± 1		
BOX TEMP	29.0	°C	5-40		
PMT TEMP	7.2	°C	7 ± 2.0		
SO ₂ Span Conc	400	PPB	20-20,000		
SO ₂ Slope	1.010	-	1.0 ± 0.3		
SO ₂ Offset	22.2	mV	<250		
Stability at Zero	0.1	PPB	<0.2		
Stability at Span	0.2	PPB	0.5% of reading (above 50 ppb)		

Calibrated by : Heeson L.
(Mr. Heeson Lormae)

Approved by : Yutthana J.
(Mr. Yutthana Tanatharanit)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT					
SO ₂ FLUORESCENT ANALYZER					
DATE :	10 May 2026	BRAND :	TELEDYNE	MODEL :	TML-60
NO.	SO ₂ -R07			SERIAL NO.	TRS1068
Calibrator (Dilution System)					
Brand : Teledyne			Model : 700		
Last Cal. Date : 24 October 2025			Serial No. : 421		
Reference Standard Gas					
Standard Gas : Sulphur Dioxide (SO ₂)			Cylinder No. : A00814SK		
Certified Date : 21 June 2021		Expired Date : 21 June 2029		Cylinder Conc. : 49.8 ppm	
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.6	°C
			% RH	50	
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.10	-	0	-
SO ₂ Span	400.0	399.6	-0.100	400.0	1.006
API Model TML-60 SO ₂ Analyzer Check list					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	0-500		
SAMPLE PRESS	28.3	in-Hg	25-35		
SAMPLE FLOW	657	cc/min	650 ± 10%		
PMT	103.2	mV	-20-150 with Zero Air		
UV LAMP	3036.3	mV	1000-4900		
STR. LGT	61.8	PPB	<100		
DRK PMT	63.4	mV	-50 - 200		
DRK LMP	58.0	mV	-50 - 200		
HVPS	673	V	550-900 constant		
DCPS	2529	mV	2500 ± 200		
RCELL TEMP	50.3	°C	50 ± 1		
BOX TEMP	29.1	°C	5-40		
PMT TEMP	7.5	°C	7 ± 2.0		
SO ₂ Span Conc	400	PPB	20-20,000		
SO ₂ Slope	1.006	-	1.0 ± 0.3		
SO ₂ Offset	22.1	mV	<250		
Stability at Zero	0.1	PPB	<0.2		
Stability at Span	0.2	PPB	0.5% of reading (above 50 ppb)		

Calibrated by : Heeson L.
(Mr. Heeson Lormae)

Approved by : Yuthana J.
(Mr. Yuthana Tanatharanit)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT					
SO ₂ FLUORESCENT ANALYZER					
DATE :	10 May 2026	BRAND :	API	MODEL :	100E
NO.	SO ₂ -R09			SERIAL NO.	76
Calibrator (Dilution System)					
Brand : Teledyne			Model : 700		
Last Cal. Date : 24 October 2025			Serial No. : 421		
Reference Standard Gas					
Standard Gas : Sulphur Dioxide (SO ₂)			Cylinder No. : A00814SK		
Certified Date : 21 June 2021		Expired Date : 21 June 2029		Cylinder Conc. : 49.8 ppm	
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.6	°C
			% RH	50	
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	-0.10	-	0	-
SO ₂ Span	400.0	399.8	-0.050	400.0	1.009
API Model 100E SO ₂ Analyzer Check list					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	0-500		
SAMPLE PRESS	28.5	in-Hg	25-35		
SAMPLE FLOW	658	cc/min	650 ± 10%		
PMT	103.4	mV	-20-150 with Zero Air		
UV LAMP	3048.7	mV	1000-4900		
STR. LGT	61.7	PPB	<100		
DRK PMT	63.2	mV	-50 - 200		
DRK LMP	57.9	mV	-50 - 200		
HVPS	672	V	550-900 constant		
DCPS	2515	mV	2500 ± 200		
RCELL TEMP	50.1	°C	50 ± 1		
BOX TEMP	29.2	°C	5-40		
PMT TEMP	7.0	°C	7 ± 2.0		
SO ₂ Span Conc	400	PPB	20-20,000		
SO ₂ Slope	1.009	-	1.0 ± 0.3		
SO ₂ Offset	22.2	mV	<250		
Stability at Zero	0.1	PPB	<0.2		
Stability at Span	0.2	PPB	0.5% of reading (above 50 ppb)		

Calibrated by : Heeson L.
(Mr. Heeson Lormae)

Approved by : Yuthana J.
(Mr. Yuthana Tanatharanit)



CERTIFICATE No : 26M2266

REFERENCE No : 80204-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE

MANUFACTURER : METTLER TOLEDO

MODEL : XS105DU

SERIAL No : 1126422905

ID No : BA 05/50

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : SUCHAT S.

CALIBRATION DATE : 05-Mar-26

APPROVED BY : PONGSAK J.

ISSUED DATE : 06-Mar-26

RECEIVED DATE : 05-Mar-26





CERTIFICATE No : 26M2266

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : XS105DU
MANUFACTURER : METTLER TOLEDO S/N : 1126422905
ID No : BA 05/50 RECEIVED DATE : 05-Mar-26
AIR PRESSURE : 1004mbar $\pm$ 1mbar CALIBRATION DATE : 05-Mar-26
AMBIENT TEMPERATURE : 25° C $\pm$ 1° C RELATIVE HUMIDITY : 50 %RH $\pm$ 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	C02250116	28-Jan-27
2) STANDARD WEIGHT	E2	15843	C02250117	29-Jan-27

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 120 g WAS 0.000055 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ($\pm$ g)
0.00	0.00000	0.00000	0.000065
0.02	0.02000	0.00000	0.000065
0.10	0.10000	0.00000	0.000066
0.20	0.20000	0.00000	0.000066
0.50	0.50001	-0.00001	0.000065
1.00	1.00001	-0.00001	0.000066
2.00	2.00000	0.00000	0.000067
5.00	5.00001	-0.00001	0.000068
10.00	10.00004	-0.00004	0.000070
20.00	20.00006	-0.00006	0.000078
50.00	50.00000	0.00000	0.00012
100.00	100.00002	-0.00002	0.00019
120.00	120.00002	-0.00002	0.00022

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.0000
2	50.0000
3	50.0000
4	50.0000
5	50.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



ลำดับที่ 2

คุณภาพอากาศจากปล่องระบายอากาศ



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Console Calibration Report

Calibration Method

Critical Orifices

Calibration Data

Console Data		Calibration Data		
No.	Serial No.	Date	y	ΔH_{g} (mmH ₂ O)
B01	1563	02/03/2026	0.998	49.85
B02	8002514	02/03/2026	1.003	49.77
B03	1503016	03/03/2026	0.997	49.68
B04	00006659	03/03/2026	0.996	49.82
B05	00007428	02/03/2026	0.999	49.65
R01	1561	03/03/2026	1.002	49.98
R02	8002513	03/03/2026	1.004	49.56
R03	1570	03/03/2026	0.997	49.73
R04	8002519	03/03/2026	0.999	49.80
R05	1503015	02/03/2026	1.003	49.95

Remark : Accept Value of y (test) is $0.97 < y < 1.03$
Accept Value of ΔH_{g} (test) is 46.7 ± 6.4 (mmH₂O)

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

Peera Detudom
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com., www.spscon.com

Pitot Tube Calibration Report

Calibration Method

Standard Pitot Tube

Calibration Data

Pitot Tube Data			Calibration Data		
No.	Type of Pitot	Coefficient of Standard Pitot	Date	Avg. of Cp (test)	
				Side A	Side B
B03	S	0.99	05/05/2026	0.84	0.83
B04	S	0.99	05/05/2026	0.84	0.85
B05	S	0.99	05/05/2026	0.84	0.83
B07	S	0.99	05/05/2026	0.84	0.84
B08	S	0.99	05/05/2025	0.84	0.84
B09	S	0.99	05/05/2026	0.85	0.84
B11	S	0.99	05/05/2026	0.84	0.84
B16	S	0.99	06/05/2026	0.84	0.84
B18	S	0.99	06/05/2026	0.85	0.84
B19	S	0.99	06/05/2025	0.84	0.85
B21	S	0.99	05/05/2026	0.84	0.84
B24	S	0.99	05/05/2026	0.84	0.85
B27	S	0.99	05/05/2026	0.85	0.84
B30	S	0.99	05/05/2026	0.84	0.85
B31	S	0.99	05/05/2026	0.83	0.84
B33	S	0.99	05/05/2026	0.84	0.84
B35	S	0.99	03/05/2026	0.84	0.85

Remark : Accept value of Cp (test) is 0.84 ± 0.01

Calibrated by :

Adul Dangklom

(Mr. Adul Dangklom)

Approved by :

Peera Detudom

(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Pitot Tube Calibration Report

Calibration Method

Standard Pitot Tube

Calibration Data					
Pitot Tube Data			Calibration Data		
No.	Type of Pitot	Coefficient of Standard Pitot	Date	Avg. of Cp (test)	
				Side A	Side B
B36	S	0.99	05/05/2026	0.84	0.84
B37	S	0.99	03/05/2026	0.84	0.85
B38	S	0.99	03/05/2026	0.84	0.84
B39	S	0.99	06/05/2026	0.84	0.85
B40	S	0.99	06/05/2026	0.85	0.84
B41	S	0.99	05/05/2026	0.84	0.85
B44	S	0.99	06/05/2026	0.84	0.83
B45	S	0.99	05/05/2026	0.84	0.84
B46	S	0.99	05/05/2026	0.84	0.85
B47	S	0.99	03/05/2026	0.84	0.84
B48	S	0.99	03/05/2026	0.85	0.84
B49	S	0.99	03/05/2026	0.84	0.84
B54	S	0.99	05/05/2026	0.85	0.84
B56	S	0.99	03/05/2026	0.84	0.84
B57	S	0.99	05/05/2026	0.84	0.84
B58	S	0.99	03/05/2026	0.84	0.84


Remark : Accept value of Cp (test) is 0.84 ± 0.01

Calibrated by : <u>Adul Dangklom</u> (Mr. Adul Dangklom)	Approved by : <u>(Signature)</u> (Mr. Peera Detudom)
---	---



CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-G353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CERTIFICATE OF CALIBRATION FOR

NOMENCLATURE	VACUUM GAUGE
MANUFACTURER	HI-LIGHT
MODEL/TYPE	N/A
SERIAL NO.	N/A[64-220088-1]
CLID.NO.	212301422
JOB CONTROL NO.	240720076546

CUSTOMER S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24 ROAD., JOMPOL,
CHATUCHAK, BANGKOK 10900

DATE OF RECEIVED : 19 July 2025

DATE OF ISSUED: 24 July 2025

The report or calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sittipong Pimdee
Calibration Engineer

Approved By : Mongkol Yotsoontorn
Authorized Signatory
24 July 2025



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q24076546

F3-011-05/12-23

page 1 of 3



CALIBRATION LABORATORY Co., LTD.

211Q-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-Q353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CALIBRATION AND
DIMENSIONAL MEASUREMENT
ACDM-2814

REPORT OF CALIBRATION

FOR

NOMENCLATURE	VACUUM GAUGE
MANUFACTURER	HI-LIGHT
MODEL/TYPE	N/A
SERIAL NO.	N/A [64-220088-1]
DATE OF CALIBRATION	23 July 2025
DUE DATE OF CALIBRATION	23 July 2026

ENVIRONMENT CONDITIONS

Temperature : $(23 \pm 2) ^\circ\text{C}$

Relative Humidity $(55 \pm 10) \% \text{RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. CLC-CPPP-05 according to DKD-R 6-1 as calibration guidelines.

The calibration was performed by direct measurement with Document Process Calibrator and Pressure Module which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

Document Process Calibrator, Fluke Model 74 1B *S/N.* 8295020 with Pressure Module Model 700PD5 *S/N.* 89404505.

TRACEABILITY :

The measurement s are traceable to International System of Units (SI), through National Institute of Metrology (Thailand).
Certificate No. MP-0040-24.

UNCERTAINTY :

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor of $k = 2$. It has been evaluated according to the "Calibration of Pressure Gauges (DKD-R 6-1)" which provides a level of confidence approximately 95%.

Certificate No. Q24076546


F3-011-05/12-23

page 2 of 3



CALIBRATION LABORATORY Co., LTD.

2/1Q-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-D353-4 Fax: 02-578-2672 www.caHaboratory.com E-mail: sale@cal-laboratory.com



CONDITION OF CALIBRATION ITEM :RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS: (X) without adjustment () adjustment

The DUC was exercised by applying a known pressure from its zero to full scale 1 times. Then 2 series of known gauge pressure were applied. The STD reading were recorded and the means value were reported in the table below.

CALIBRATION DATA

CORRECTION OF PRESSURE

DUC Test point (inHg)	STD Reading (kPa)		Conversion to inHg		Correction (inHg)	
	Up	Down	Up	Down	Up	Down
0	0.00	0.00	0.0	0.0	0.0	0.0
-5	-15.07	-15.10	-4.5	-4.5	+0.5	+0.5
-10	-32.50	-32.84	-9.6	-9.7	+0.4	+0.3
-15	-49.44	-49.77	-14.6	-14.7	+0.4	+0.3
-20	-66.70	-66.70	-19.7	-19.7	+0.3	+0.3
-25	-83.63	-83.97	-24.7	-24.8	+0.3	+0.2
-30	-100.39	-100.39	-29.6	-29.6	+0.4	+0.4

Uncertainty of measurement ± 0.2 inHg

Transmitting fluid : Air.

Technical Note. Conversion factor 1 kPa ; 0.2953003 inHg

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 012 Page 43 of 67

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q24076546

F3-011-05/ 12-23



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Environmental Conditions

Temperature : 25 ± 3 °C
Pressure : 1010 ± 15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (mL/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R ²
B41	SKC	224-PCXR4	612669	05/01/2026	1,000	1,500	2,000	995	1,490	1,997	1.004x - 11.846	1.000
B42	SKC	224-PCXR4	626041	05/01/2026	1,000	1,500	2,000	996	1,510	1,999	0.999x - 0.630	1.000
B43	SKC	224-PCXR4	034636	05/01/2026	1,000	1,500	2,000	1,000	1,493	2,004	1.004x - 6.760	1.000
B44	SKC	224-PCXR8	529341	05/01/2026	1,000	1,500	2,000	995	1,512	1,995	1.000x - 4.571	0.999
B45	SKC	224-PCXR8	529594	05/01/2026	1,000	1,500	2,000	997	1,503	2,001	1.004x - 10.178	1.000
B46	SKC	224-PCXR8	566743	05/01/2026	1,000	1,500	2,000	997	1,491	2,007	1.013x - 21.797	1.000
B47	SKC	224-PCXR8	566747	06/01/2026	1,000	1,500	2,000	995	1,508	1,999	1.007x - 15.240	0.999
B48	SKC	224-PCXR8	566753	06/01/2026	1,000	1,500	2,000	998	1,493	1,992	0.997x - 0.746	1.000
B49	SKC	224-PCXR8	566780	06/01/2026	1,000	1,500	2,000	994	1,475	1,991	1.002x - 18.905	0.999
B50	SKC	224-PCXR8	500400	06/01/2026	1,000	1,500	2,000	990	1,498	1,992	0.991x + 4.770	0.999
B51	SKC	224-PCXR8	500363	06/01/2026	1,000	1,500	2,000	995	1,498	1,994	1.008x - 21.051	0.999
B52	SKC	224-PCXR8	093186	06/01/2026	1,000	1,500	2,000	1,001	1,494	1,995	0.993x + 6.362	1.000
B53	SKC	224-PCXR8	707670	06/01/2026	1,000	1,500	2,000	992	1,502	2,007	1.016x - 28.087	1.000
B54	SKC	224-PCXR3	509821	06/01/2026	1,000	1,500	2,000	1,000	1,497	2,002	1.009x - 18.056	1.000
B55	SKC	224-PCXR3	510710	05/01/2026	1,000	1,500	2,000	999	1,497	2,001	1.008x - 15.994	1.000
B56	SKC	224-PCXR3	511450	05/01/2026	1,000	1,500	2,000	996	1,510	2,001	1.005x - 11.080	0.999
B57	SKC	224-PCXR3	510798	05/01/2026	1,000	1,500	2,000	1,000	1,493	2,001	1.000x - 1.575	1.000
B58	SKC	224-PCXR3	509852	05/01/2026	1,000	1,500	2,000	997	1,473	1,995	1.000x - 11.132	0.999
B59	SKC	224-PCXR3	509862	05/01/2026	1,000	1,500	2,000	961	1,461	1,969	1.021x - 71.317	0.999
B60	SKC	224-PCXR3	512655	06/01/2026	1,000	1,500	2,000	971	1,469	2,001	1.027x - 56.285	0.999
B61	SKC	224-PCXR3	503915	06/01/2026	1,000	1,500	2,000	1,000	1,476	2,001	1.006x - 16.496	0.999
B62	SKC	224-PCXR3	505975	06/01/2026	1,000	1,500	2,000	997	1,503	2,001	1.004x - 10.186	1.000
B63	SKC	224-PCXR3	511432	06/01/2026	1,000	1,500	2,000	1,000	1,496	1,994	0.996x - 0.574	1.000
B64	SKC	224-PCXR3	508302	06/01/2026	1,000	1,500	2,000	1,000	1,500	1,997	1.000x - 4.850	1.000
B65	SKC	224-PCXR3	508310	05/01/2026	1,000	1,500	2,000	998	1,505	1,999	1.001x - 5.999	1.000
B66	SKC	224-PCXR3	509861	05/01/2026	1,000	1,500	2,000	1,003	1,501	2,006	1.009x - 15.631	0.999
B67	SKC	224-PCXR3	506295	05/01/2026	1,000	1,500	2,000	996	1,496	1,993	0.999x - 4.016	1.000
B68	SKC	224-PCXR3	505872	05/01/2026	1,000	1,500	2,000	1,003	1,491	2,001	0.995x + 5.309	1.000
B69	SKC	224-PCXR3	508375	06/01/2026	1,000	1,500	2,000	994	1,507	2,002	1.008x - 16.847	0.999
B70	SKC	224-PCXR3	510623	06/01/2026	1,000	1,500	2,000	993	1,506	2,003	1.010x - 18.889	1.000
B71	SKC	224-PCXR3	508367	07/01/2026	1,000	1,500	2,000	997	1,501	1,994	0.999x - 0.148	1.000
B72	SKC	224-PCXR3	505977	06/01/2026	1,000	1,500	2,000	1,000	1,503	2,003	1.004x - 8.252	1.000
B73	SKC	224-PCXR3	512606	06/01/2026	1,000	1,500	2,000	996	1,495	1,995	0.998x - 1.627	1.000
B74	SKC	224-PCXR3	505993	06/01/2026	1,000	1,500	2,000	995	1,506	1,999	1.008x - 17.629	0.999
B75	SKC	224-PCXR3	509820	05/01/2026	1,000	1,500	2,000	997	1,491	1,999	1.001x - 6.461	1.000
B76	SKC	224-PCXR3	509811	05/01/2026	1,000	1,500	2,000	1,000	1,472	2,004	1.008x - 18.391	1.000
B77	SKC	224-PCXR3	508301	05/01/2026	1,000	1,500	2,000	993	1,471	1,995	1.000x - 10.813	0.999
B78	SKC	224-PCXR3	510677	05/01/2026	1,000	1,500	2,000	999	1,477	2,000	1.003x - 12.304	0.999
B79	SKC	224-PCXR3	510920	06/01/2026	1,000	1,500	2,000	1,001	1,500	1,997	0.998x + 0.215	1.000

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

Peera Detudom
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chafuchak, Bangkok 10900

Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com.. www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136833

Environmental Conditions

Temperature 25 ± 3 °C
Pressure 1010 ± 15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R ²
R01	SKC	224-PCXR4	602467	05/01/2026	1,000	1,500	2,000	999	1,505	2,009	1.011x - 15.308	1.000
R02	SKC	224-PCXR4	626450	05/01/2026	1,000	2,000	3,000	1,001	1,505	2,005	1.005x - 5.625	1.000
R03	SKC	224-PCXR4	691592	05/01/2026	1,000	1,500	2,000	998	1,499	2,010	1.009x - 11.382	1.000
R04	SKC	224-PCXR4	691672	05/01/2026	1,000	1,500	2,000	999	1,496	2,000	0.992x + 5.045	0.999
R05	SKC	224-PCXR4	798470	06/01/2026	1,000	1,500	2,000	997	1,480	1,991	0.995x - 8.487	0.999
R06	SKC	224-PCXR4	798456	06/01/2026	1,000	1,500	2,000	1,000	1,502	1,992	0.993x + 2.874	0.999
R07	SKC	224-PCXR4	798480	06/01/2026	1,000	1,500	2,000	1,000	1,508	2,000	1.000x + 1.559	1.000
R08	SKC	224-PCXR4	883215	07/01/2026	1,000	1,500	2,000	1,001	1,500	2,000	1.004x - 8.216	1.000
R09	SKC	224-PCXR4	034650	05/01/2026	1,000	1,500	2,000	999	1,509	2,005	1.005x - 6.025	1.000
R10	SKC	224-PCXR4	091765	05/01/2026	1,000	1,500	2,000	1,001	1,509	2,008	1.007x - 8.311	1.000
R11	SKC	224-PCXR4	091763	05/01/2026	1,000	1,500	2,000	999	1,502	1,995	1.002x - 10.594	0.999
R12	SKC	224-PCXR4	091568	06/01/2026	1,000	1,500	2,000	999	1,495	1,994	0.994x - 1.683	0.999
R13	SKC	224-PCXR4	091638	06/01/2026	1,000	1,500	2,000	999	1,499	1,994	0.998x - 7.136	0.999
R14	SKC	224-PCXR4	091764	06/01/2026	1,000	1,500	2,000	1,004	1,507	2,006	1.007x - 8.975	1.000
R15	SKC	224-PCXR8	529457	06/01/2026	1,000	1,500	2,000	1,004	1,502	2,002	0.999x + 1.731	1.000
R16	SKC	224-PCXR8	529643	05/01/2026	1,000	1,500	2,000	1,001	1,511	2,010	1.010x - 13.433	1.000
R17	SKC	224-PCXR8	529645	06/01/2026	1,000	1,500	2,000	1,004	1,502	2,003	0.998x + 4.238	1.000
R18	SKC	224-PCXR8	566756	05/01/2026	1,000	1,500	2,000	1,003	1,504	2,006	1.004x - 3.774	1.000
R19	SKC	224-PCXR8	566802	05/01/2026	1,000	1,500	2,000	1,003	1,498	1,995	1.001x - 8.224	0.999
R20	SKC	224-PCXR8	529089	06/01/2026	1,000	1,500	2,000	997	1,509	1,985	0.994x + 5.269	0.999
R21	SKC	224-PCXR8	665728	06/01/2026	1,000	1,500	2,000	1,000	1,510	1,995	0.998x - 1.139	0.999
R22	SKC	224-PCXR8	707444	05/01/2026	1,000	1,500	2,000	1,004	1,507	2,008	1.004x - 5.709	1.000
R23	SKC	224-PCXR8	761067	05/01/2026	1,000	1,500	2,000	1,009	1,504	2,006	1.000x + 1.179	1.000
R24	SKC	224-PCXR8	707893	05/01/2026	1,000	1,500	2,000	999	1,497	1,992	0.998x - 8.383	0.999
R25	SKC	224-PCXR8	761052	06/01/2026	1,000	1,500	2,000	998	1,503	1,975	0.984x + 17.071	0.999
R26	SKC	224-PCXR8	707956	05/01/2026	1,000	1,500	2,000	997	1,492	1,992	0.991x + 0.388	1.000
R27	SKC	224-PCXR8	707398	05/01/2026	1,000	1,500	2,000	1,000	1,495	2,002	1.002x - 3.898	1.000
R28	SKC	224-PCXR8	707481	06/01/2026	1,000	1,500	2,000	1,009	1,503	2,008	0.996x + 8.659	1.000
R29	SKC	224-PCXR8	707402	07/01/2026	1,000	1,500	2,000	1,006	1,513	2,009	1.002x - 1.219	0.999
R30	SKC	224-PCXR8	093811	07/01/2026	1,000	1,500	2,000	1,001	1,513	2,008	1.008x - 9.239	1.000
R31	SKC	224-PCXR8	093183	06/01/2026	1,000	1,500	2,000	1,010	1,507	2,013	1.003x - 0.780	1.000
R32	SKC	224-PCXR8	671950	06/01/2026	1,000	1,500	2,000	999	1,498	1,999	1.000x + 0.668	1.000
R33	SKC	224-PCXR4	626254	06/01/2026	1,000	1,500	2,000	1,000	1,508	2,007	1.004x - 5.149	1.000
R34	SKC	224-PCXR4	626131	05/01/2026	1,000	1,500	2,000	996	1,498	2,003	1.010x - 18.178	1.000
R35	SKC	224-PCXR8	707460	05/01/2026	1,000	1,500	2,000	1,006	1,496	2,004	0.999x + 0.388	1.000
R36	SKC	224-PCXR8	707446	05/01/2026	1,000	1,500	2,000	1,006	1,504	2,008	1.005x - 6.281	1.000
R37	SKC	224-PCXR8	707432	06/01/2026	1,000	1,500	2,000	1,003	1,505	2,004	1.004x - 5.005	1.000
R38	SKC	224-PCXR8	707349	06/01/2026	1,000	1,500	2,000	998	1,498	1,997	0.999x - 1.655	1.000
R39	SKC	224-PCXR8	761095	06/01/2026	1,000	1,500	2,000	1,000	1,497	2,003	1.005x - 8.068	1.000

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

Peera Detodom
(Mr. Peera Detodom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136833

Environmental Conditions

Temperature : 25 $\pm$ 3 $^{\circ}$ C
Pressure : 1010 $\pm$ 15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (mL/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R ²
R40	SKC	224-PCXR4	612753	05/01/2026	1,000	1,500	2,000	997	1,506	1,998	1.000x - 0.556	1.000
R41	SKC	224-PCXR4	626140	05/01/2026	1,000	1,500	2,000	995	1,504	1,992	0.996x - 3.574	0.999
R42	SKC	224-PCXR4	626463	05/01/2026	1,000	1,500	2,000	1,006	1,505	1,984	0.988x + 15.108	0.999
R43	SKC	224-PCXR4	626129	05/01/2026	1,000	1,500	2,000	993	1,504	1,972	0.982x + 17.902	0.999
R44	SKC	224-PCXR4	602753	06/01/2026	1,000	1,500	2,000	1,001	1,495	2,000	1.001x - 3.434	1.000
R45	SKC	224-PCXR4	626137	06/01/2026	1,000	1,500	2,000	998	1,494	1,997	0.996x + 1.827	1.000

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

Peera Detudom
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136833

Environmental Conditions

Temperature : 25 $\pm$ 3 $^{\circ}$ C
Pressure : 1010 $\pm$ 15 mmbar

Personal Pump Data					Calibration Data							
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)			y	R ²
					1	2	3	1	2	3		
R01	SKC	224-PCXR4	602467	01/04/2026	1,000	1,500	2,000	1,001	1,500	2,007	1.005x - 6.003	1.000
R02	SKC	224-PCXR4	626450	05/04/2026	1,000	2,000	3,000	1,000	1,503	2,001	1.001x - 0.383	1.000
R03	SKC	224-PCXR4	691592	03/04/2026	1,000	1,500	2,000	1,005	1,501	2,000	1.007x - 15.384	0.999
R04	SKC	224-PCXR4	691672	03/04/2026	1,000	1,500	2,000	1,007	1,513	1,999	0.996x + 5.855	0.999
R05	SKC	224-PCXR4	798470	05/04/2026	1,000	1,500	2,000	1,000	1,499	1,997	0.997x + 3.107	1.000
R06	SKC	224-PCXR4	798456	03/04/2026	1,000	1,500	2,000	998	1,497	1,996	0.998x + 0.120	1.000
R07	SKC	224-PCXR4	798480	05/04/2026	1,000	1,500	2,000	1,002	1,506	2,001	0.999x + 3.219	1.000
R08	SKC	224-PCXR4	883215	03/04/2026	1,000	1,500	2,000	1,004	1,501	1,992	1.003x - 9.877	0.999
R09	SKC	224-PCXR4	034650	03/04/2026	1,000	1,500	2,000	998	1,506	2,003	1.004x - 5.723	1.000
R10	SKC	224-PCXR4	091765	03/04/2026	1,000	1,500	2,000	999	1,507	1,996	1.005x - 13.080	0.999
R11	SKC	224-PCXR4	091763	05/04/2026	1,000	1,500	2,000	1,001	1,504	2,001	1.000x + 0.104	1.000
R12	SKC	224-PCXR4	091568	03/04/2026	1,000	1,500	2,000	998	1,505	1,996	0.998x + 1.482	1.000
R13	SKC	224-PCXR4	091638	03/04/2026	1,000	1,500	2,000	1,001	1,504	2,000	0.999x + 2.097	1.000
R14	SKC	224-PCXR4	091764	05/04/2026	1,000	1,500	2,000	1,007	1,506	2,001	1.004x - 8.866	0.999
R15	SKC	224-PCXR8	529457	05/04/2026	1,000	1,500	2,000	998	1,492	1,999	1.001x - 6.322	1.000
R16	SKC	224-PCXR8	529643	03/04/2026	1,000	1,500	2,000	1,004	1,506	2,004	1.007x - 11.726	0.999
R17	SKC	224-PCXR8	529645	05/04/2026	1,000	1,500	2,000	998	1,503	1,998	1.000x - 0.703	1.000
R18	SKC	224-PCXR8	566756	03/04/2026	1,000	1,500	2,000	999	1,508	1,995	1.002x - 8.012	0.999
R19	SKC	224-PCXR8	566802	05/04/2026	1,000	1,500	2,000	998	1,502	1,998	1.000x - 0.823	1.000
R20	SKC	224-PCXR8	529089	03/04/2026	1,000	1,500	2,000	999	1,503	1,996	0.997x + 2.001	1.000
R21	SKC	224-PCXR8	665728	03/04/2026	1,000	1,500	2,000	998	1,505	1,999	1.000x - 0.483	1.000
R22	SKC	224-PCXR8	707444	05/04/2026	1,000	1,500	2,000	1,007	1,496	2,000	1.001x - 6.418	0.999
R23	SKC	224-PCXR8	761067	05/04/2026	1,000	1,500	2,000	1,001	1,502	2,004	1.002x - 1.446	1.000
R24	SKC	224-PCXR8	707893	03/04/2026	1,000	1,500	2,000	1,002	1,503	2,001	0.999x + 2.560	1.000
R25	SKC	224-PCXR8	761052	03/04/2026	1,000	1,500	2,000	1,009	1,504	2,005	0.997x + 4.106	0.999
R26	SKC	224-PCXR8	707956	05/04/2026	1,000	1,500	2,000	1,002	1,503	2,000	0.998x + 4.497	1.000
R27	SKC	224-PCXR8	707398	03/04/2026	1,000	1,500	2,000	1,001	1,505	2,004	1.003x - 1.921	1.000
R28	SKC	224-PCXR8	707481	05/04/2026	1,000	1,500	2,000	1,010	1,513	2,006	0.997x + 5.531	0.999
R29	SKC	224-PCXR8	707402	03/04/2026	1,000	1,500	2,000	1,003	1,502	1,992	1.003x - 10.216	0.999
R30	SKC	224-PCXR8	093811	05/04/2026	1,000	1,500	2,000	999	1,512	2,005	1.007x - 9.705	1.000
R31	SKC	224-PCXR8	093183	05/04/2026	1,000	1,500	2,000	1,011	1,510	2,011	1.001x + 2.983	0.999
R32	SKC	224-PCXR8	671950	03/04/2026	1,000	1,500	2,000	1,001	1,500	2,001	0.999x + 2.272	1.000
R33	SKC	224-PCXR4	626254	05/04/2026	1,000	1,500	2,000	998	1,507	2,002	1.005x - 10.975	1.000
R34	SKC	224-PCXR4	626131	05/04/2026	1,000	1,500	2,000	997	1,496	2,000	1.007x - 14.230	1.000
R35	SKC	224-PCXR8	707460	05/04/2026	1,000	1,500	2,000	998	1,509	1,996	1.000x - 2.915	1.000
R36	SKC	224-PCXR8	707446	05/04/2026	1,000	1,500	2,000	1,003	1,492	2,003	1.007x - 16.135	0.999
R37	SKC	224-PCXR8	707432	03/04/2026	1,000	1,500	2,000	999	1,507	2,005	1.003x - 6.095	1.000
R38	SKC	224-PCXR8	707349	03/04/2026	1,000	1,500	2,000	1,003	1,499	1,999	0.997x + 2.141	1.000
R39	SKC	224-PCXR8	761095	05/04/2026	1,000	1,500	2,000	1,005	1,508	2,004	1.000x - 0.152	0.999

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

Peera Detudom
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136833

Environmental Conditions

Temperature . 25 $\pm$ 3 $^{\circ}$ C
Pressure . 1010 $\pm$ 15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R ²
R40	SKC	224-PCXR4	612753	05/04/2026	1,000	1,500	2,000	1,004	1,497	2,000	0.998x + 1.430	1.000
R41	SKC	224-PCXR4	626140	03/04/2026	1,000	1,500	2,000	998	1,498	1,997	0.999x + 0.943	1.000
R42	SKC	224-PCXR4	626463	05/04/2026	1,000	1,500	2,000	1,005	1,513	1,998	0.997x + 4.138	0.999
R43	SKC	224-PCXR4	626129	03/04/2026	1,000	1,500	2,000	1,003	1,498	2,000	0.998x + 2.029	1.000
R44	SKC	224-PCXR4	602753	03/04/2026	1,000	1,500	2,000	996	1,509	1,997	1.003x - 8.036	1.000
R45	SKC	224-PCXR4	626137	05/04/2026	1,000	1,500	2,000	1,011	1,514	2,005	0.995x + 8.367	0.999

Calibrated by :

Adul Dangklom

(Mr. Adul Dangklom)

Approved by :

Peer Detudom

(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Rotameter Calibration Report (For Personal Pump High Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136833


Calibration Data

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (mL/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R ²
H-R01	Dwyer	VFB-65	05/01/2026	500	1,000	2,000	503.6	992.4	1980.9	0.999x - 3.140	0.999
H-R02	Dwyer	VFB-65	06/01/2026	500	1,000	2,000	500.8	995.8	1986.2	1.002x - 5.343	1.000
H-R03	Dwyer	VFB-65	05/01/2026	500	1,000	2,000	495.3	992.1	1982.9	1.004x - 17.510	0.999
H-R04	Dwyer	VFB-65	05/01/2026	500	1,000	2,000	496.4	994.6	2019.5	1.007x - 11.385	1.000
H-R05	Dwyer	VFB-65	06/01/2026	500	1,000	2,000	497.2	991.5	1987.3	1.003x - 7.563	1.000
H-R06	Dwyer	VFB-65	06/01/2026	500	1,000	2,000	501.1	992.4	1982.9	1.001x - 6.139	0.999

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

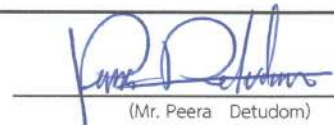
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Rotameter Calibration Report (For Personal Pump Low Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136833

Calibration Data

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (mL/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R ²
L-R01	Dwyer	VFA-21	05/01/2026	50	100	200	50.2	102.0	203.9	0.991x + 2.329	1.000
L-R02	Dwyer	VFA-21	05/01/2026	50	100	200	50.4	101.3	200.5	1.006x - 0.627	0.999
L-R03	Dwyer	VFA-21	06/01/2026	50	100	200	50.1	99.4	202.7	1.017x - 1.144	1.000
L-R04	Dwyer	VFA-21	06/01/2026	50	100	200	49.8	100.5	201.0	1.010x - 1.541	0.999
L-R05	Dwyer	VFA-21	05/01/2026	50	100	200	50.2	101.4	203.8	0.990x + 2.384	1.000
L-R06	Dwyer	VFA-21	06/01/2026	50	100	200	50.4	99.1	201.5	1.003x - 0.197	1.000

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :


(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Rotameter Calibration Report (For Personal Pump High Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136833

Calibration Data

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (mL/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R ²
H-R01	Dwyer	VFB-65	01/04/2026	500	1,000	2,000	499.7	1000.6	1996.7	1.000x - 0.544	1.000
H-R02	Dwyer	VFB-65	01/04/2026	500	1,000	2,000	501.2	992.4	1990.0	1.001x - 5.362	0.999
H-R03	Dwyer	VFB-65	03/04/2026	500	1,000	2,000	501.4	997.5	1997.3	0.998x + 2.606	1.000
H-R04	Dwyer	VFB-65	05/04/2026	500	1,000	2,000	502.5	993.6	1985.2	0.999x - 2.085	0.999
H-R05	Dwyer	VFB-65	05/04/2026	500	1,000	2,000	500.4	1001.3	1999.8	1.000x + 1.247	1.000
H-R06	Dwyer	VFB-65	03/04/2026	500	1,000	2,000	500.8	997.2	1994.6	0.999x - 0.348	1.000

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :


(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com., www.spscon.com

Rotameter Calibration Report (For Personal Pump Low Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136833

Calibration Data

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (mL/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R ²
L-R01	Dwyer	VFA-21	01/04/2026	50	100	200	50.3	101.1	201.9	0.998x + 0.955	1.000
L-R02	Dwyer	VFA-21	01/04/2026	50	100	200	50.2	101.7	201.0	0.999x + 0.367	0.999
L-R03	Dwyer	VFA-21	03/04/2026	50	100	200	50.3	101.2	201.0	1.001x + 0.605	1.000
L-R04	Dwyer	VFA-21	05/04/2026	50	100	200	50.7	100.8	200.2	1.000x + 0.719	1.000
L-R05	Dwyer	VFA-21	05/04/2026	50	100	200	50.1	101.2	200.5	1.001x - 0.213	0.999
L-R06	Dwyer	VFA-21	03/04/2026	50	100	200	50.3	100.8	200.1	0.999x + 0.639	1.000

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

Peera Detudom
(Mr. Peera Detudom)



CERTIFICATE No : 26M2266
REFERENCE No : 80204-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE
MANUFACTURER : METTLER TOLEDO
MODEL : XS105DU
SERIAL No : 1126422905
ID No : BA 05/50
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : SUCHAT S.

CALIBRATION DATE : 05-Mar-26

APPROVED BY :  PONGSAK J.

ISSUED DATE : 06-Mar-26

RECEIVED DATE : 05-Mar-26





CERTIFICATE No : 26M2266

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : XS105DU
MANUFACTURER : METTLER TOLEDO S/N : 1126422905
ID No : BA 05/50 RECEIVED DATE : 05-Mar-26
AIR PRESSURE : 1004mbar $\pm$ 1mbar CALIBRATION DATE : 05-Mar-26
AMBIENT TEMPERATURE : 25° C $\pm$ 1° C RELATIVE HUMIDITY : 50 %RH $\pm$ 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	C02250116	28-Jan-27
2) STANDARD WEIGHT	E2	15843	C02250117	29-Jan-27

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 120 g WAS 0.000055 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ($\pm$ g)
0.00	0.00000	0.00000	0.000065
0.02	0.02000	0.00000	0.000065
0.10	0.10000	0.00000	0.000066
0.20	0.20000	0.00000	0.000066
0.50	0.50001	-0.00001	0.000065
1.00	1.00001	-0.00001	0.000066
2.00	2.00000	0.00000	0.000067
5.00	5.00001	-0.00001	0.000068
10.00	10.00004	-0.00004	0.000070
20.00	20.00006	-0.00006	0.000078
50.00	50.00000	0.00000	0.00012
100.00	100.00002	-0.00002	0.00019
120.00	120.00002	-0.00002	0.00022

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.0000
2	50.0000
3	50.0000
4	50.0000
5	50.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN
associates



Cert. No. : SP25026

Pages : 1 of 4

Calibration Certificate

Equipment : UV-VIS SPECTROPHOTOMETER
Manufacturer : PERKINELMER
Model : LAMBDA 25
Serial No.: 501S14123010
ID No.: SP03/58
Calibration Mode : WAVELENGTH ACCURACY
PHOTOMETRIC ACCURACY
STRAY LIGHT

Condition As Found : GOOD

Customer : S.P.S CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN ROAD,
CHOMPHON SUB-DISTRICT, CHATUCHAK DISTRICT,
BANGKOK PROVINCE 10900 THAILAND.

Location : ORGANIC LABORATORY IV

Ambient Temperature : (22.9 $\pm$ 5) °C
Relative Humidity : (53.7 $\pm$ 25) %

Received Date : 22 AUGUST 2025
Calibration Date : 22 AUGUST 2025
Date of Issue : 25 AUGUST 2025

Calibrated by :

Nitinun Srihawan

Approved by :

Wichok B.
(Wichok Ekpongpradit)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : SP25026

Job No. : VC68SP0019

Pages : 2 of 4

Calibration Method :

This instrument was calibrated by using on-site calibration procedure In-house method : CP-SP-01

The calibration procedure to direct measurement wavelength accuracy by using wavelength standard solution, Photometric accuracy by using absorbance standard filter and absorbance standard solution

The calibration procedure used was based on ASTM E275-01, ASTM E925-02

Condition of this result of calibration :

1. Certified reference materials

<u>Material</u>	<u>Ref. type</u>	<u>Cell serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Holmium liquid	RM-HL	29706	126461	24/10/2026
Didymium liquid	RM-DL	28912	126462	24/10/2026
Neutral density filter	RM-1N2N3N	13877	126457	24/10/2026
Potassium dichromate solutions	RM-0204060810	14204	126497	25/10/2026
Potassium Iodide solution	-	KI-0701-001	CI-0185-24	14/05/2026

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 The UK National Physical Laboratory (NPL)

Result of calibration : Wavelength Accuracy

(Without adjustment)

Material	Certified Values of Reference Material (nm)	UUC* Reading (nm)	Error (nm)	Uncertainty ± (nm)	k Factor
RM-HL	278.13	278.21	0.08	0.16	2.00
	361.25	361.39	0.14	0.16	2.00
	467.82	467.71	-0.11	0.16	2.00
	536.56	536.50	-0.06	0.16	2.00
	640.50	640.36	-0.14	0.16	2.00
RM-DL	740.09	739.85	-0.24	0.16	2.00
	864.94	865.12	0.18	0.16	2.00

UUC* = Unit Under Calibration

Cert. No. : SP25026

Job No. : VC68SP0019

Pages : 3 of 4

Result of calibration : Photometric Accuracy

Material	Wavelength (nm)	Filter S/N	Nominal Absorbance (A)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor
Neutral Density glass filter	440.0	29381	0.5	0.5443	0.5413	-0.0030	0.0043	2.00
		29914	0.7	0.7484	0.7455	-0.0029	0.0054	2.00
		29360	1.0	1.0527	1.0535	0.0008	0.0032	2.00
	465.0	29381	0.5	0.4948	0.4922	-0.0026	0.0041	2.00
		29914	0.7	0.6906	0.6877	-0.0029	0.0050	2.00
		29360	1.0	0.9695	0.9709	0.0014	0.0031	2.00
	546.1	29381	0.5	0.5090	0.5068	-0.0022	0.0036	2.00
		29914	0.7	0.6985	0.6960	-0.0025	0.0041	2.00
		29360	1.0	0.9814	0.9825	0.0011	0.0031	2.00
	590.0	29381	0.5	0.5375	0.5353	-0.0022	0.0034	2.00
		29914	0.7	0.7256	0.7231	-0.0025	0.0037	2.00
		29360	1.0	1.0213	1.0219	0.0006	0.0032	2.00
	635.0	29381	0.5	0.5223	0.5202	-0.0021	0.0033	2.00
		29914	0.7	0.6927	0.6901	-0.0026	0.0036	2.00
		29360	1.0	0.9744	0.9750	0.0006	0.0032	2.00

UUC* = Unit Under Calibration

Cert. No. : SP25026

Job No. : VC68SP0019

Pages : 4 of 4

Result of calibration : Photometric Accuracy

(Without adjustment)

Material	Wavelength (nm)	Solution (mg/l)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor
Potassium dichromate solutions	235.0	20	0.2415	0.2443	0.0028	0.0101	2.00
		40	0.4866	0.4871	0.0005	0.0115	2.00
		60	0.7415	0.7295	-0.0120	0.0067	2.00
		80	0.9854	0.9844	-0.0010	0.0071	2.00
		100	1.2444	1.2425	-0.0019	0.0073	2.00

UUC* = Unit Under Calibration

Condition of this result of calibration : Spectrophotometer PERKINELMER Model LAMBDA 25 S/N 501S14123010

Resolution of Wavelength Mode 0.1 nm

Resolution of Photometric Mode 0.001 A

Parameter Setting

Measurement Mode Wavelength, Absorbance

Wavelength Scan 190 nm - 1100 nm

Scanning Speed 7.5 nm/min

Band width(Wavelength) 1.0

Band width(Vis) 1.0

Band width(Uv) 1.0

Stray Light** UUC* Reading at 220.0 nm	
Transimission T(%)	Absorbance(A)
0.020	3.7032

**Specific Acceptance :

Transmission ≤ 1.0 T(%), Absorbance ≥ 2.0 A

**Stray light not TISI Accredited

The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95%

End of Calibration Certificate



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Calibration Report					
Non-Dispersive Infrared CO Analyzer					
Date :	06 May 2026	Brand :	API	Model :	300E
No.	CO-R02			Serial No.	171-S
Calibrator (Dilution System)					
Brand : API			Model : 700		
Last Cal. Date : 01 September 2025			Serial No. : 911		
Reference Standard Gas					
Standard Gas : Carbon Monoxide (CO)			Cylinder No. : D711839		
Certified Date : 14 March 2024		Expired Date : 14 March 2032		Cylinder Conc. : 4,580 ppm	
Calibrating Condition					
Pressure : 1011 mmbar		Temp. : 24.6 °C		% RH : 50	
Calibration Setting					
Span	Initial Reading (Before Adj.), PPM			Final Reading (After Adj.), PPM	
Set Point	Expected Concentration	Analyzer Response		%Dif	
Zero	0	-0.10		-	
CO Span	40.00	40.04		0.100	
API Model 300E CO Analyzer Check List					
Parameter	Observed Value	Units	Nominal Range		
Range	50	PPM	0-1000 ppm		
Stability	0.10	PPM	< 1 ppm With Zero Air		
CO Measure	4016.4	mV	2500-4800 mV		
CO Reference	3947.5	mV	2500-4800 mV		
Measure/Reference Ratio	1.180	-	1.1-1.3 W/Zero Air		
Sample Pressure	28.4	In-Hg-A	~2" < Ambient Absolute Pressure		
Sample Flow	807	CC/Min	800 ± 10%		
Sample Temperature	48.3	°C	48 ± 4		
Bench Temperature	48.1	°C	48 ± 2		
Wheel Temperature	68.5	°C	68 ± 2		
Box Temperature	30.8	°C	Ambient Temp + 7 ± 10		
Photo-Drive	3029.2	mV	250 mV to 4750 mV		
Slope	1.017	-	1.0 ± 0.3		
Offset	0.2	-	0 ± 0.3		

Calibrated by :

Adul Dangkhom
(Mr. Adul Dangkhom)

Approved by :

Peera Detudom
(Mr. Peera Detudom)



GAS CHROMATOGRAPH TEST CERTIFICATION

Certificate No. : SV0825/23032

Instrument Type : Gas Chromatography

Model : 3800

Serial Number : 00734

Organization : S.P.S. Consulting Service Co., Ltd.

Address : 7 Phahonyothin Soi 24 Phahonyothin Rd. Ladyao Chatuchak Bangkok 10900

Date : 02/08/2025

ELECTRONIC TEST

CPU	☒ PASS	☐ FAIL
DISPLAY & LED TEST	☒ PASS	☐ FAIL
VENT TEST	☒ PASS	☐ FAIL
KEY ECHO TEST	☒ PASS	☐ FAIL
DESTRUCTION RAM TEST	☒ PASS	☐ FAIL

RUN CHROMATOGRAM TEST

DETECTOR : Flame Ionization Detectors (FID Channel-Front)

INJECTOR : 1079 Injector

GC CONDITION:

Column	80 °C hold 1 min., rate 20 °C/min. to 200 °C hold 1min.
Injector	220 °C
Detector	300 °C
Column flow	5 mL/min
Makeup flow	25 mL/min
Air flow	300 mL/min
Hydrogen flow	30 mL/min

Column: Capillary Column CP sil 5 CB 0.25 ID x 15 M

Sample: 1 µL Injection FID Test Sample 0.218g/L C14,C15,C16 in hexane (diluted to 30ppm)

SENSITIVITY TEST: C15. (Area count) = 515,940 Counts.





บริษัท ไทยยูนิค จำกัด

THAI UNIQUE CO., LTD.

80-82 ถนนประชาทิพย์ไทย แขวงบางขุนพรหม เขตพระนคร กรุงเทพฯ 10200

80-82 Prachathipatai Rd., Bangkhunphrom, Pranakorn, Bangkok 10200

Tel. 0-2629-0191-6, 0-2280-1787, Fax. 0-2280-1788, E-mail : thuwatt@thaiunique.com, Website : www.thaiunique.com

Detector Sensitivity (FID)

Detector Response	Result	Specification
Baseline Noise (μV)	2.40	≤ 50
Baseline Drift (%)	0.18	≤ 1
Sensitivity (S/N for C15)	19,716	$\geq 1,024$

Temperature Specification

Temperature	Set	Result	Specification
Column Oven ($^{\circ}C$)	80	79	± 5
Injector ($^{\circ}C$)	220	218	± 5
Detector ($^{\circ}C$)	300	298	± 5
Incubator ($^{\circ}C$)	60	N/A	± 5

Relative Standard Deviation % (%RSD)

Checkout Procedure	Result	Specification
Area C15 (%)	1.48	≤ 5
Retention Time C15 (%)	0.08	≤ 0.5

APPROVAL :

Signature:

Engineer : Somchai Pohtongkam

Date : 02/08/2025



VARIAN



บริษัท ไทยยูนิค จำกัด

THAI UNIQUE CO., LTD.

80-82 ถนนประชาธิปไตย แขวงบางขุนพรหม เขตพระนคร กรุงเทพฯ 10200

80-82 Prachathipatai Rd., Bangkhunphrom, Pranakorn, Bangkok 10200

Tel. 0-2629-0191-6, 0-2280-1787, Fax. 0-2280-1788, E-mail : thawatt@thaiunique.com, Website : www.thaiunique.com

Results Integrated System Testing

Checkout Procedure	FID
Detector Position	Front
Inlet Type	1079 Injector
C15 Area 1	506,043
C15 Area 2	520,497
C15 Area 3	522,154
C15 Area 4	521,664
C15 Area 5	509,340
C15 Area Average	515,940
* % RSD (< 5 %)	1.48

* The precision specification should be less than 2.0 % RSD ** (Relative Standard Deviation) for an Auto sampler injection and less than 5 % for Manual injections. To calculate the %RSD, select the C15 peak area for each of the five (5) samples.

** (Relative Standard Deviation is determined by dividing the standard deviation by the average and multiplying by 100.)

$$\% \text{ RSD} = (\text{std.dev} / \text{avg}) * 100$$

Compliance	☒ Pass	☐ Fail
Performance by	<i>Sachin P.</i>	
Date	02/08/2025	



Comments			
Reviewed by	<i>Wattana</i>	Date	02/08/2025



VARIAN



บริษัท ไทยยูนิค จำกัด

THAI UNIQUE CO., LTD.

80-82 ถนนประชาธิปไตย แขวงบางขุนพรหม เขตพระนคร กรุงเทพฯ 10200

80-82 Prachathipatai Rd., Bangkhunphrom, Pranakorn, Bangkok 10200

Tel. 0-2629-0191-6, 0-2280-1787, Fax. 0-2280-1788, E-mail : thawatt@thaiunique.com, Website : www.thaiunique.com

Results Integrated System Testing

Checkout Procedure	FID
Detector Position	Front
Inlet Type	1079 Injector
C15 RT 1	3.874
C15 RT 2	3.880
C15 RT 3	3.875
C15 RT 4	3.872
C15 RT 5	3.878
C15 RT Average	3.876
* % RSD (< 0.5 %)	0.08

* The precision specification should be less than 0.5 % RSD ** (Relative Standard Deviation) for an Auto sampler injection and less than 0.5 % for Manual injections. To calculate the %RSD, select the RT C15 peak for each of the five (5) samples.

** (Relative Standard Deviation is determined by dividing the standard deviation by the average and multiplying by 100.)

$$\% \text{ RSD} = (\text{std.dev} / \text{avg}) * 100$$

Compliance	☒ Pass	☐ Fail
Performance by	<i>Somchai P.</i>	
Date	02/08/2025	



Comments			
Reviewed by	<i>Wattana</i>	Date	02/08/2025



VARIAN


Title :
Run File : e:\sps2025\blk001.run
Method File : c:\star\data\tu\2025\cal fid.mth
Sample ID : blk

Injection Date: 2/8/2568 12:01 Calculation Date: 2/8/2568 12:33

Operator : watsamon Detector Type: 3800 (10 Volts)
Workstation: GC-LAB Bus Address : 44
Instrument : Sample Rate : 10.00 Hz
Channel : Front = FID Run Time : 20.005 min

** LC Workstation Version 6.20 ** 02511-7390-ae7-0265 **

Chart Speed = 1.13 cm/min Attenuation = 1 Zero Offset = 50%
Start Time = 0.000 min End Time = 20.005 min Min / Tick = 1.00

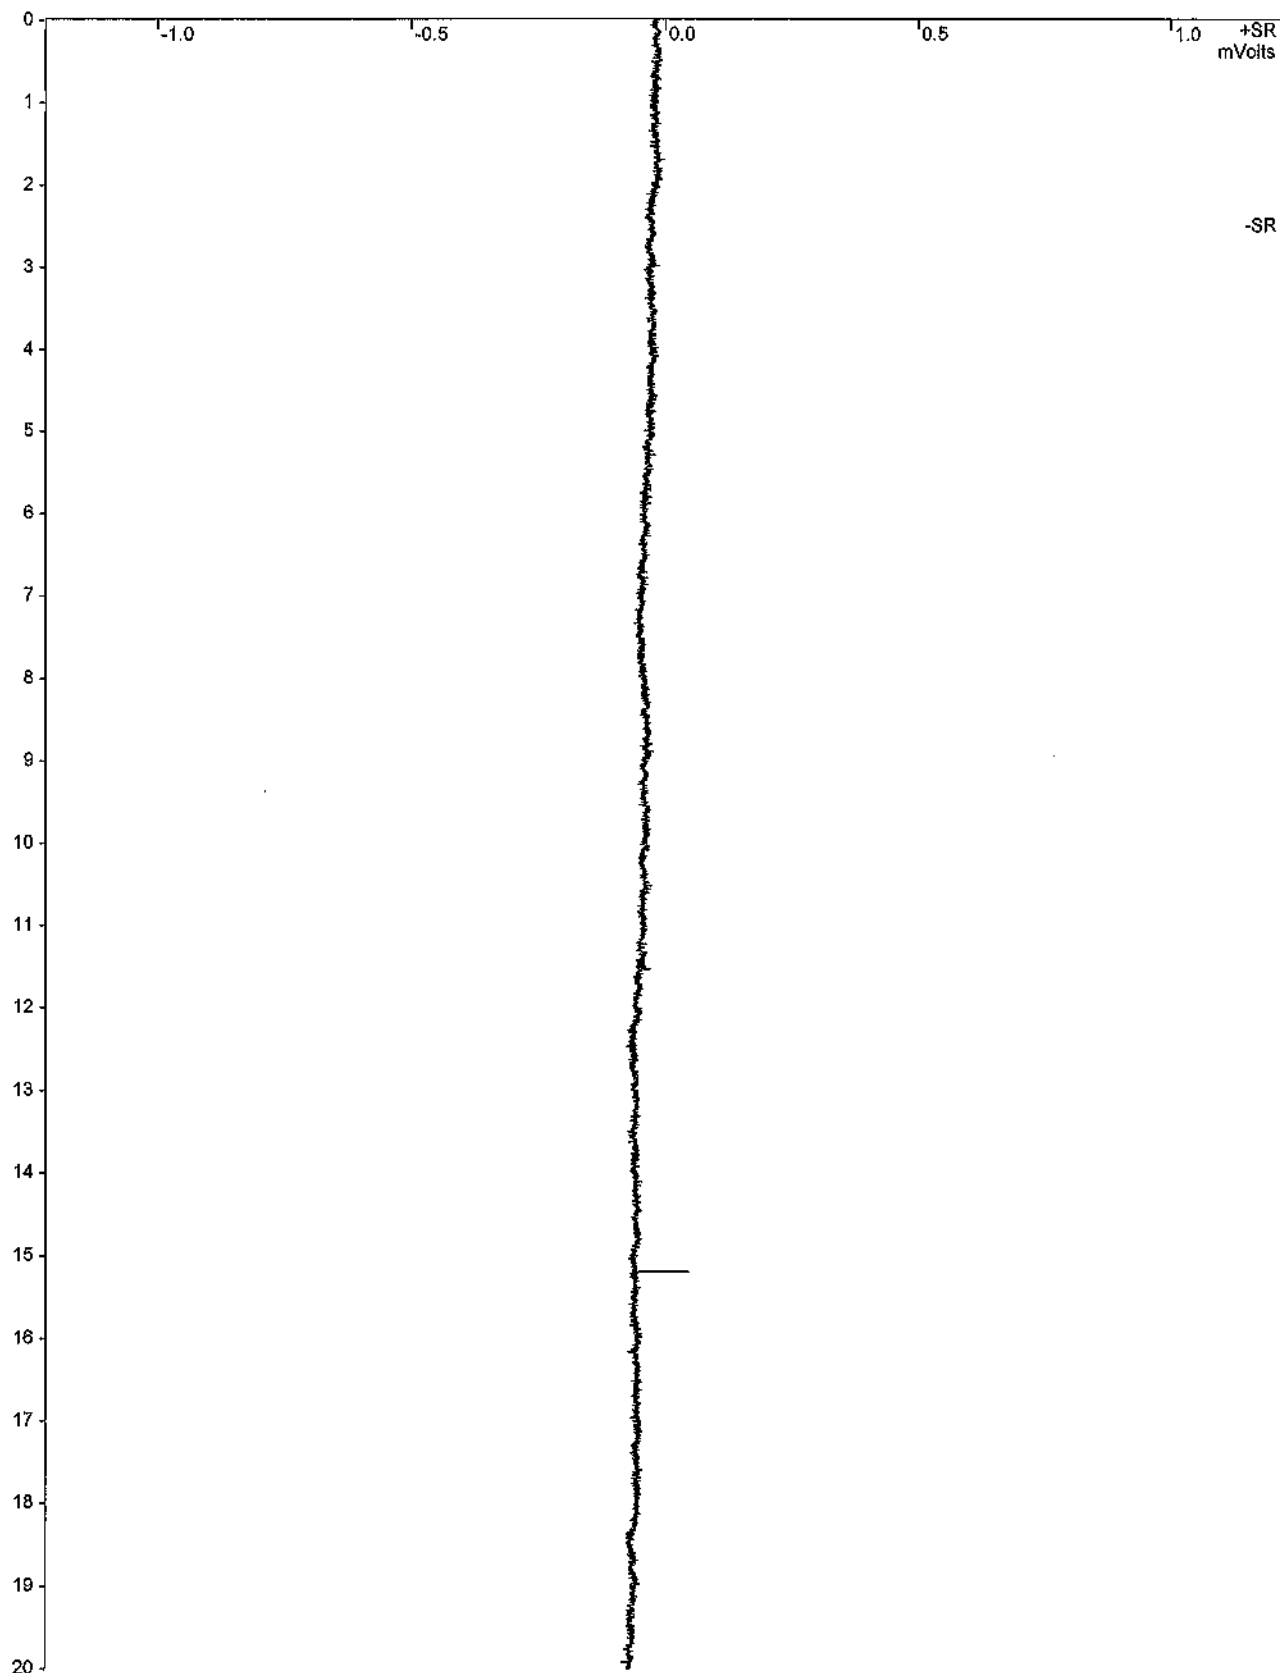

Title :
Run File : e:\sps2025\blk001.run
Method File : c:\star\data\tu\2025\cal fid.mth
Sample ID : blk

Injection Date: 2/8/2568 12:01 Calculation Date: 2/8/2568 12:33

Operator : watsamon Detector Type: 3800 (10 Volts)
Workstation: GC-LAB Bus Address : 44
Instrument : Sample Rate : 10.00 Hz
Channel : Front = FID Run Time : 20.005 min

** LC Workstation Version 6.20 ** 02511-7390-ae7-0265 **

Run Mode : Analysis
Peak Measurement: Peak Area
Calculation Type: External Standard

Peak No.	Peak Name	Result ()	Ret. Time (min)	Time Offset (min)	Area (counts)	Sep. Code	Width 1/2 (sec)	Status Codes
-----	-----	-----	-----	-----	-----	-----	-----	-----
Totals:		0.0000		0.000	0			

Total Unidentified Counts : 0 counts

Detected Peaks: 0 Rejected Peaks: 0 Identified Peaks: 0

Multiplier: 1 Divisor: 1 Unidentified Peak Factor: 0

Baseline Offset: -14 microVolts LSB: 1 microVolts

Noise (used): 24 microVolts - monitored before this run

Manual injection

Data Handling: No peaks


Title :
Run File : e:\sps2025\fidstd001.run
Method File : c:\star\data\tu\2025\cal fid.mth
Sample ID : fidstd

Injection Date: 2/8/2568 12:34 Calculation Date: 2/8/2568 13:26

Operator : watsamon Detector Type: 3800 (10 Volts)
Workstation: GC-LAB Bus Address : 44
Instrument : Sample Rate : 10.00 Hz
Channel : Front = FID Run Time : 7.993 min

** LC Workstation Version 6.20 ** 02511-7390-ae7-0265 **

Chart Speed = 2.83 cm/min Attenuation = 79 Zero Offset = 2%
Start Time = 0.000 min End Time = 7.993 min Min / Tick = 1.00

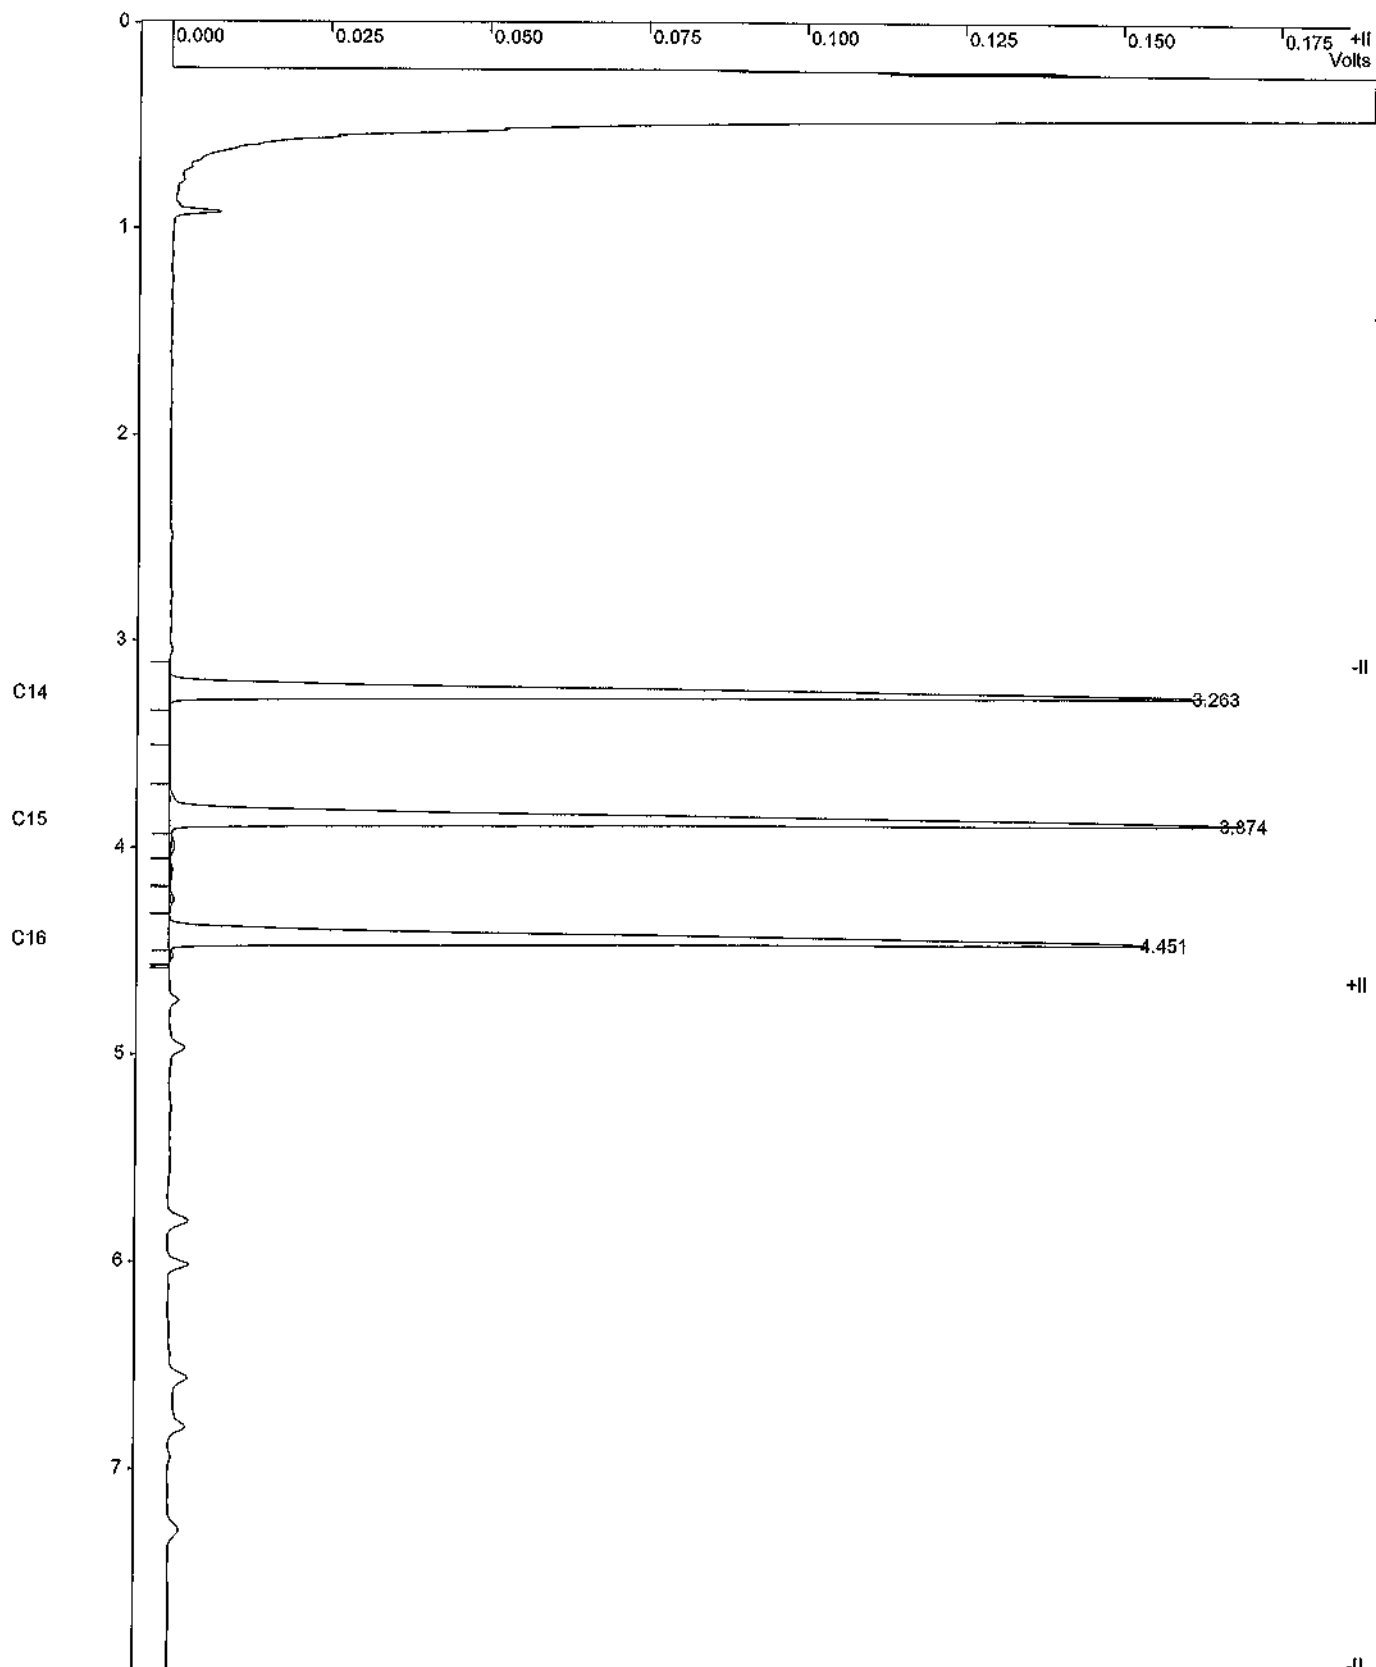

Title :
Run File : e:\sps2025\fidstd001.run
Method File : c:\star\data\tu\2025\cal fid.mth
Sample ID : fidstd

Injection Date: 2/8/2568 12:34 Calculation Date: 2/8/2568 13:26

Operator : watsamon Detector Type: 3800 (10 Volts)
Workstation: GC-LAB Bus Address : 44
Instrument : Sample Rate : 10.00 Hz
Channel : Front = FID Run Time : 7.993 min

** LC Workstation Version 6.20 ** 02511-7390-ae7-0265 **

Run Mode : Calibration
Peak Measurement: Peak Area
Calculation Type: External Standard
Level : 1

Peak No.	Peak Name	Ret. Time (min)	Time Offset (min)	Area (counts)	Sep. Code	Width 1/2 (sec)	Status Codes
1	C14	3.263	0.002	458627	BB	2.7	
2	C15	3.874	0.002	506043	VV	2.8	
3	C16	4.451	0.001	460610	VB	2.8	
Totals:			0.005	1425280			

Total Unidentified Counts : 0 counts

Detected Peaks: 8 Rejected Peaks: 5 Identified Peaks: 3

Multiplier: N/A Divisor: N/A Unidentified Peak Factor: 0

Baseline Offset: 6 microVolts LSB: 1 microVolts

Noise (used): 2 microVolts - monitored before this run

Manual injection

Sample ID: fid std

Operator (Inj): watsamon

Injection Date: 02/08/2025

Calc Date: 02/08/2025

Run Time (min): 7.993

Workstation: GC-LAB

Instrument (Inj):



VARIAN


Run Mode: Calibration

Peak Measurement: Peak Area

Calculation Type: External Std.

e:\sps2025\fidstd001.run

A = FID 10 V RESULTS

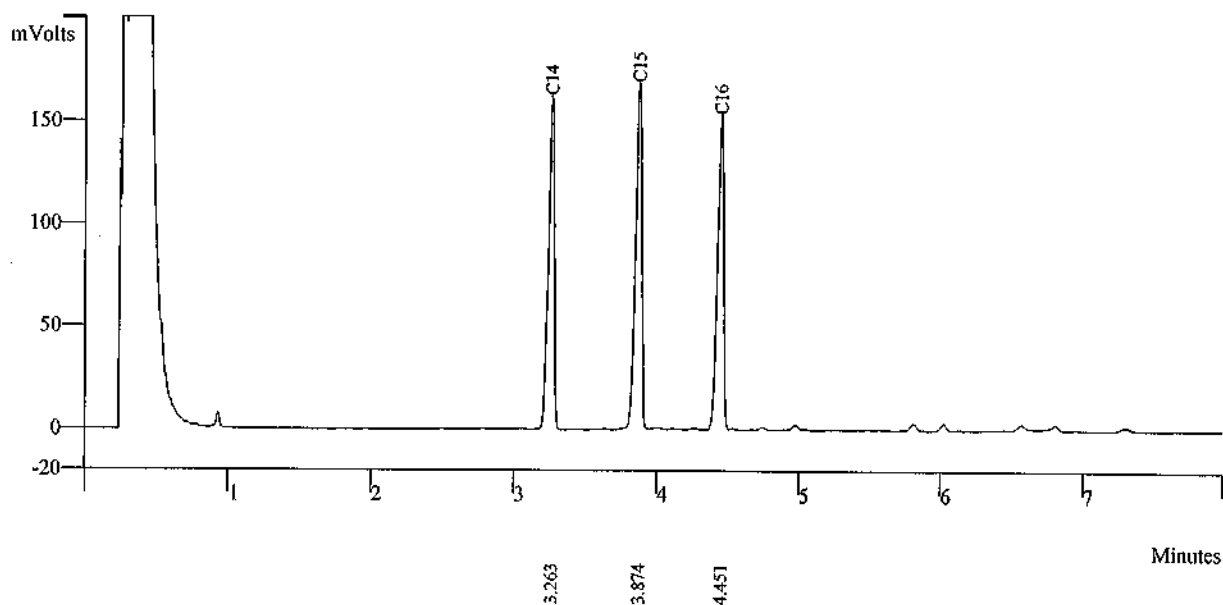

Peak No	Peak Name	Result ()	Ret Time (min)	Peak Area (counts)	Sep. Code	Width 1/2 (sec)
1	C14	0.0000	3.263	458627	BB	2.7
2	C15	0.0000	3.874	506043	VV	2.8
3	C16	0.0000	4.451	460610	VB	2.8
	Totals	0.0000		1425280		

Sample ID: **fid std**



Operator (Inj): **watsamon**

Injection Date: **02/08/2025**

Calc Date: **02/08/2025**

Run Time (min): **7.993**

Workstation: **GC-LAB**

Instrument (Inj):

VARIAN


Run Mode: **Calibration**

Peak Measurement: **Peak Area**

Calculation Type: **External Std.**

e:\sps2025\fidstd002.run

A = FID 10 V RESULTS

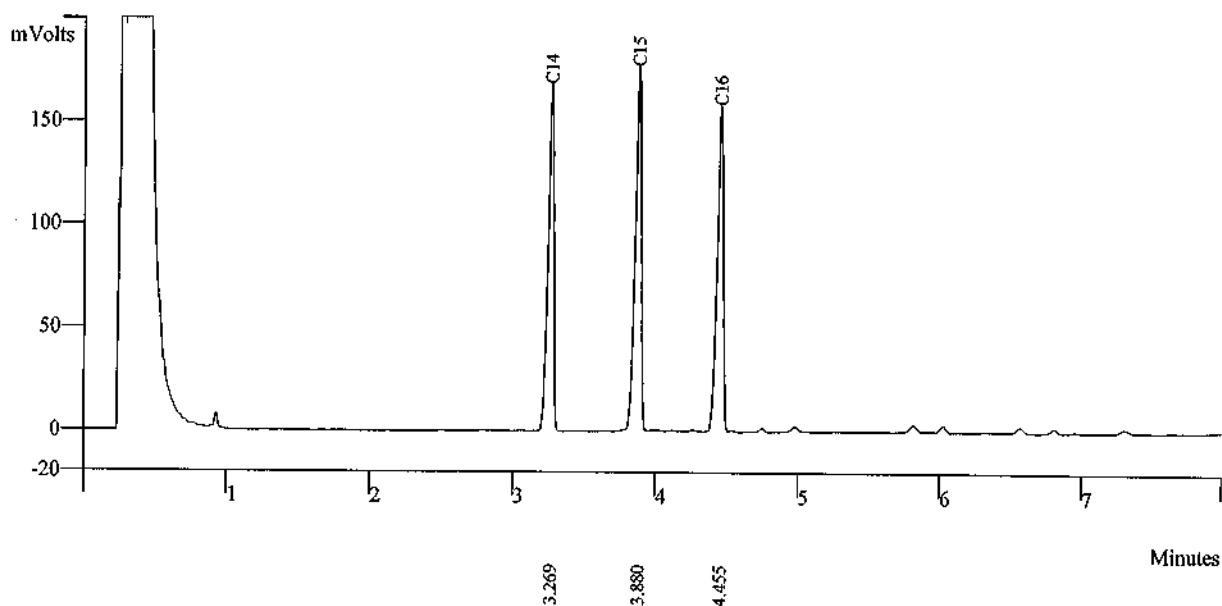

Peak No	Peak Name	Result ()	Ret Time (min)	Peak Area (counts)	Sep. Code	Width 1/2 (sec)
1	C14	0.0000	3.269	472338	BB	2.6
2	C15	0.0000	3.880	520497	VV	2.7
3	C16	0.0000	4.455	471916	VB	2.8
	Totals	0.0000		1464751		

Sample ID: fid std

Operator (Inj): watsamon

Injection Date: 02/08/2025

Calc Date: 02/08/2025

Run Time (min): 7.993

Workstation: GC-LAB

Instrument (Inj):



VARIAN


Run Mode: Calibration

Peak Measurement: Peak Area

Calculation Type: External Std.

e:\sps2025\fidstd003.run

A = FID 10 V RESULTS

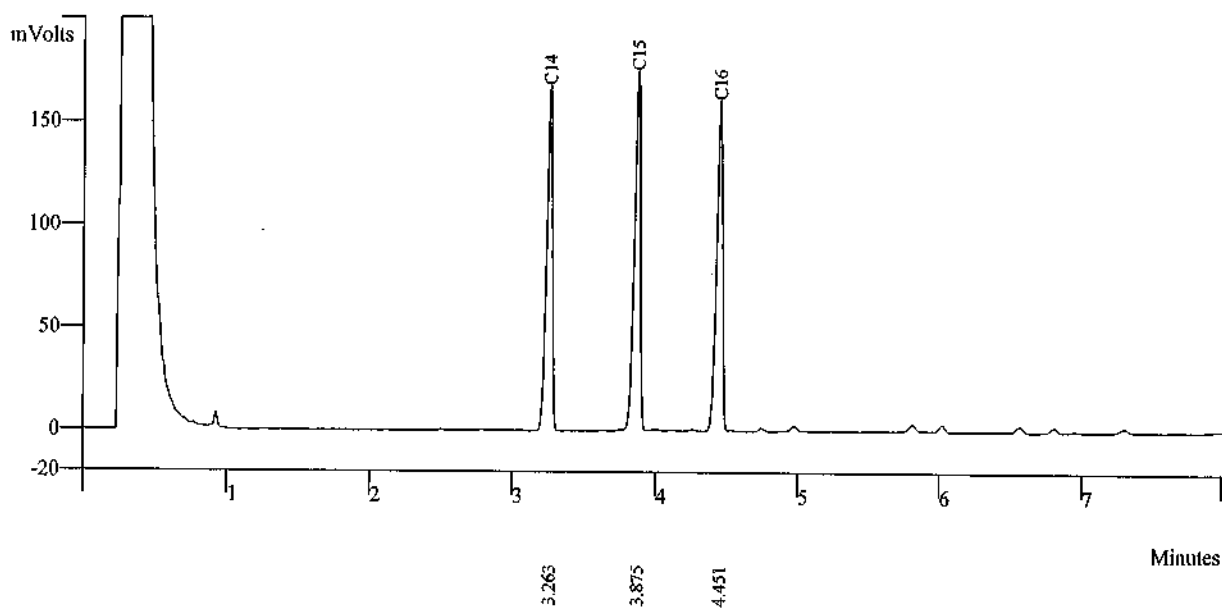

Peak No	Peak Name	Result ()	Ret Time (min)	Peak Area (counts)	Sep. Code	Width 1/2 (sec)
1	C14	0.0000	3.263	469265	BB	2.6
2	C15	0.0000	3.875	522154	VV	2.8
3	C16	0.0000	4.451	478526	VB	2.8
	Totals	0.0000		1469945		

Sample ID: fid std



Operator (Inj): watsamon

Injection Date: 02/08/2025

Calc Date: 02/08/2025

Run Time (min): 7.993

Workstation: GC-LAB

Instrument (Inj):

VARIAN


Run Mode: Calibration

Peak Measurement: Peak Area

Calculation Type: External Std.

e:\sps2025\fidstd004.run

A = FID 10 V RESULTS

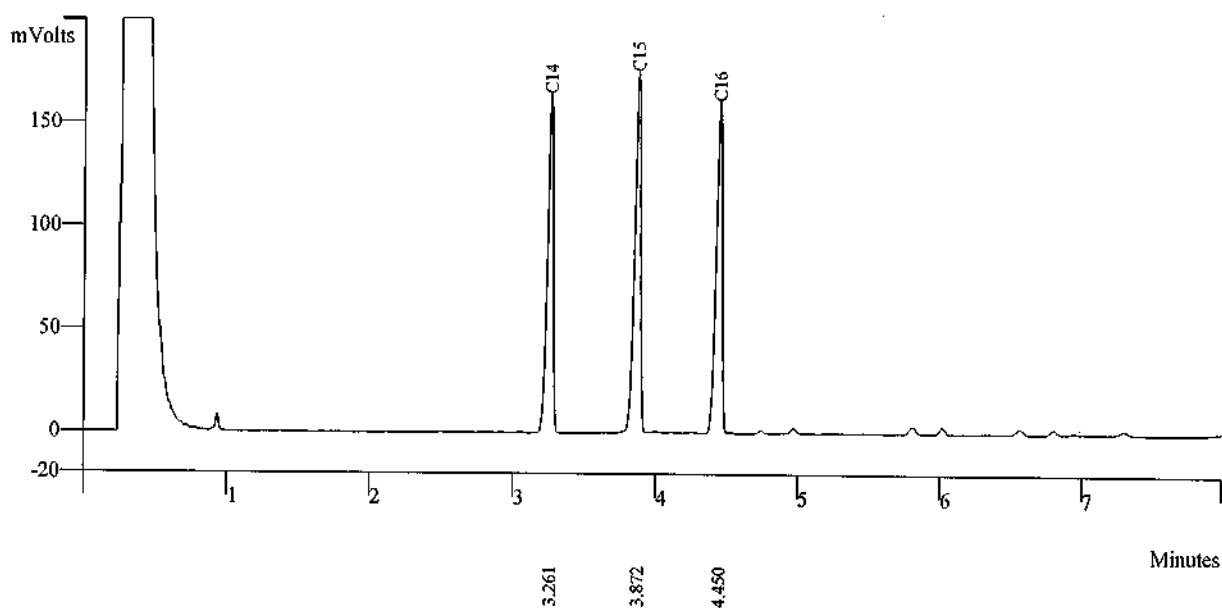

Peak No	Peak Name	Result ()	Ret Time (min)	Peak Area (counts)	Sep. Code	Width 1/2 (sec)
1	C14	0.0000	3.261	468907	BB	2.7
2	C15	0.0000	3.872	521664	VV	2.8
3	C16	0.0000	4.450	478772	VB	2.8
	Totals	0.0000		1469343		

Sample ID: **fid std**



Operator (Inj): **watsamon**

Injection Date: **02/08/2025**

Calc Date: **02/08/2025**

Run Time (min): **7.993**

Workstation: **GC-LAB**

Instrument (Inj):

VARIAN


Run Mode: **Calibration**

Peak Measurement: **Peak Area**

Calculation Type: **External Std.**

e:\sps2025\fidstd005.run

A = FID 10 V RESULTS

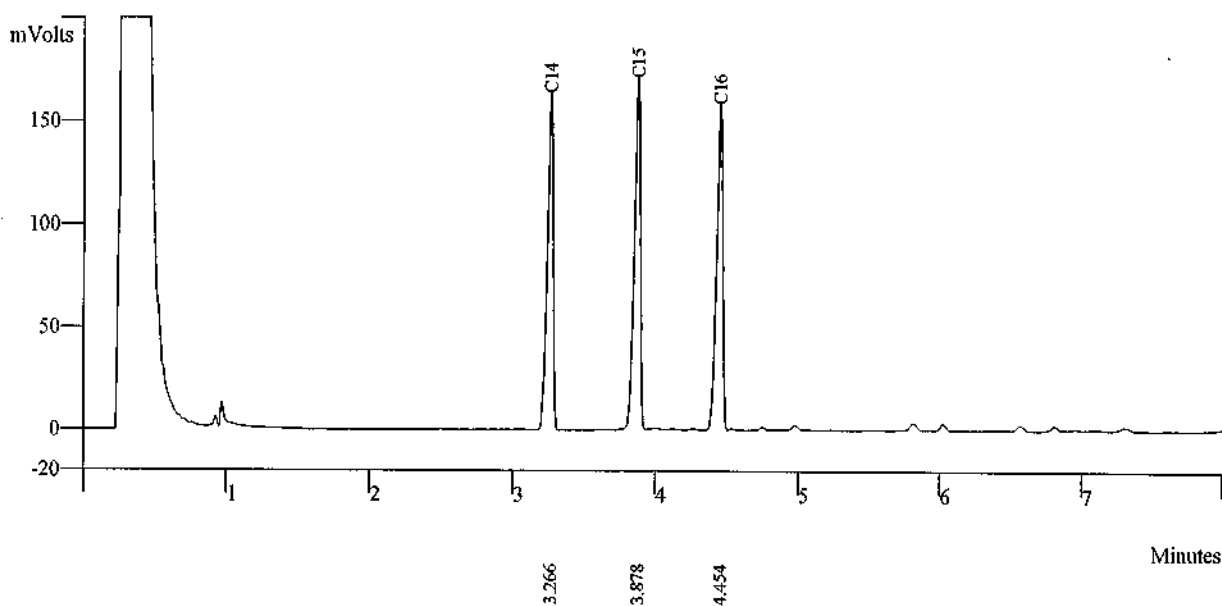

Peak No	Peak Name	Result ()	Ret Time (min)	Peak Area (counts)	Sep. Code	Width 1/2 (sec)
1	C14	0.0000	3.266	459351	BB	2.6
2	C15	0.0000	3.878	509340	VV	2.8
3	C16	0.0000	4.454	468353	VB	2.8
	Totals	0.0000		1437044		



C14

External Standard Analysis


Curve Type: Linear

Origin: Force

$y = +1.552325e+004x$

Resp. Fact. RSD: 1.347%

Coeff. Det. (r^2): 0.999130

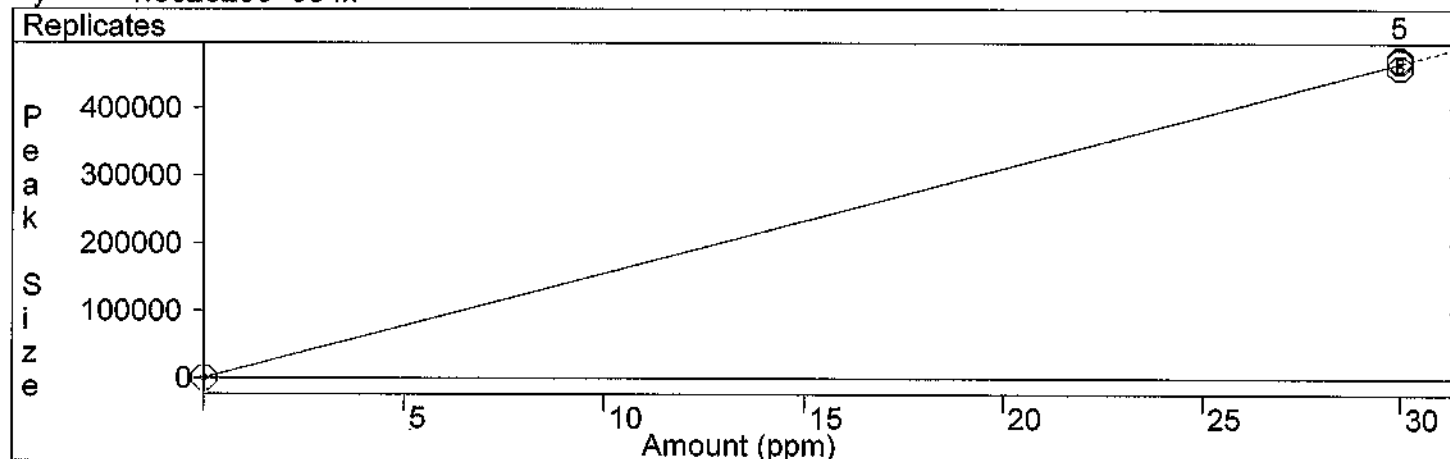

C15

External Standard Analysis


Curve Type: Linear

Origin: Force

$y = +1.719798e+004x$

Resp. Fact. RSD: 1.481%

Coeff. Det. (r^2): 0.998948

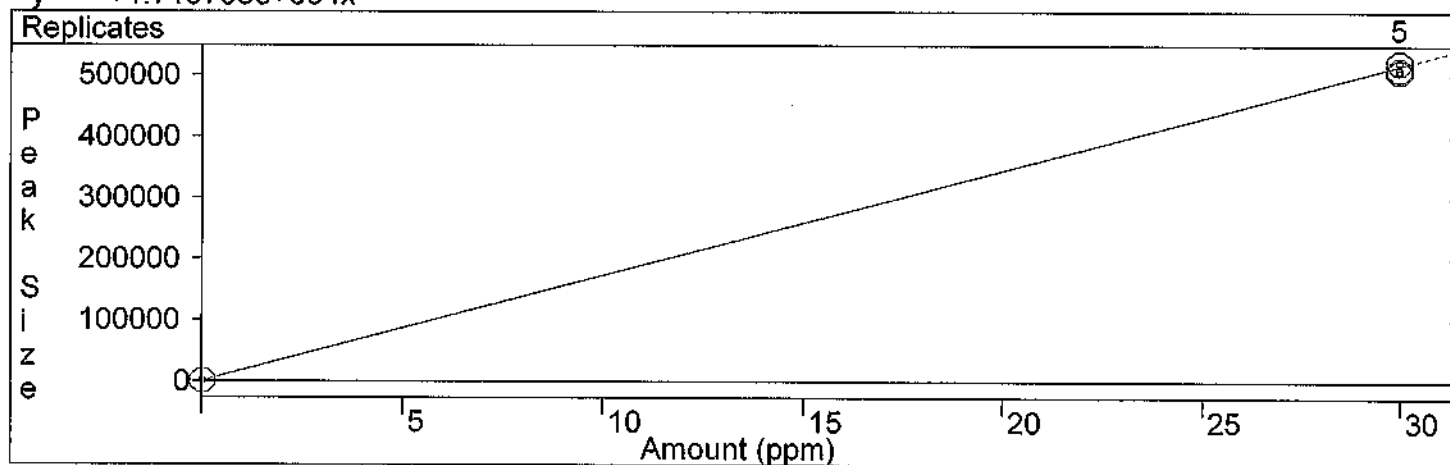

C16

External Standard Analysis


Curve Type: Linear

Origin: Force

$y = +1.572118e+004x$

Resp. Fact. RSD: 1.611%

Coeff. Det. (r^2): 0.998756

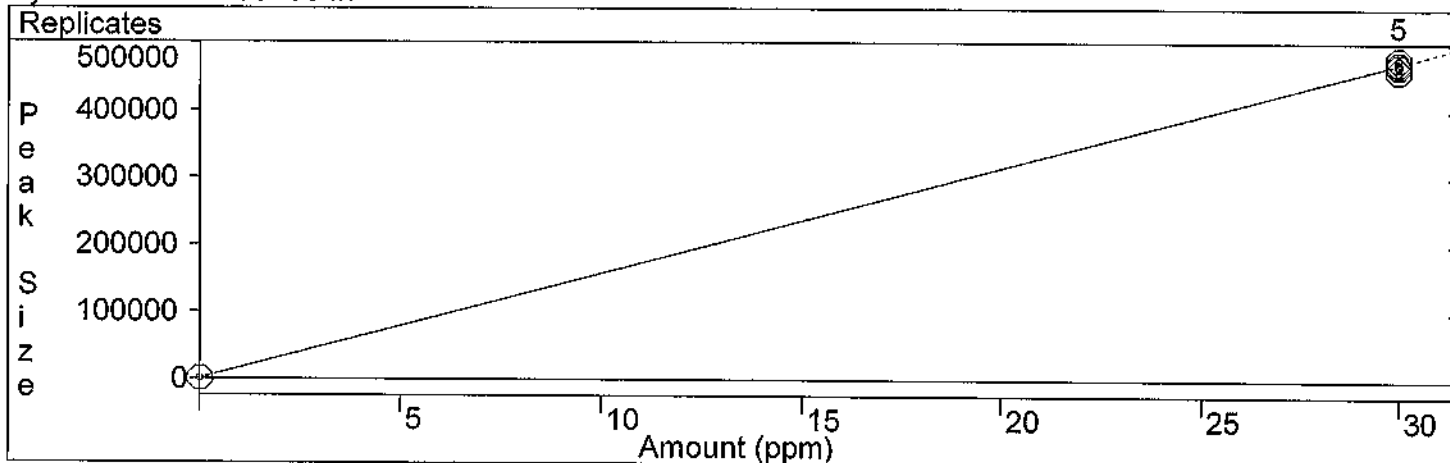

CERTIFICATE

This is to certify, that

Somchai Pohthongkham

has participated the course


Basic GC and Sampler training

Date: ***24 – 27 May 2004***

Location: ***Middelburg***

Instructor: ***W.J. Buys***

Signature instructor:

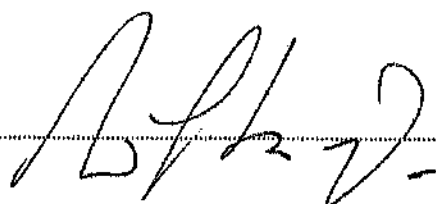

VARIAN

Varian Analytical Instruments
Varian Chrompack International BV
Herculesweg 8
P.O. Box 8033
4330 EA Middelburg
The Netherlands
Tel.: +31 118 671000
Fax: +31 118 633110
www.varianinc.com



WK Electric Co., Ltd.



68/242 Moo 5, Sawaipracharaj Rd., Tambol Ladsawai, Amphur Lamlukka, Pathumthani 12150

Tel. +66 2993 4773, +66 2153 7132-3 Fax. +66 2994 5509 E-mail : wk.calibrations@gmail.com www.wk-etc.com

Certificate of Calibration

Certificate No.: WK2412-053-1

Page 1 of 2

Customer : THAI UNIQUE CO., LTD.
80-82 Prachathipatai Rd., Bangkhunphrom,
Pranakorn, Bangkok 10200

Instrument : AMD Flow Meter
Manufacturer : Agilent Technologies
Model : G6691A
Serial No. : MY16470347
Identity No. : SV-DF-001
Range : 0 ml/min to 750 ml/min
Resolution : See to Data
Calibration Method : CP-WK-M10

Ambient Temperature : $(23 \pm 2) ^\circ\text{C}$
Humidity : $(50 \pm 15) \% \text{RH}$
Received Date : 4-Dec-24
Calibrated Date : 11-Dec-24
Issued Date : 13-Dec-24
Calibrated Location : In Lab

Reference standard instruments :

<u>Instrument</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>	<u>Traceability to</u>
Flow Calibrator	140215-134	L202304114-001	18-Apr-25	MIT
Primary Flow Calibrator	1107-S	WK2405-049-5	22-May-25	WK Electric Co., Ltd.

MIT : Miracle International Technology Co., Ltd.

This result calibrate was found accurate as shown on date place of calibrate only

This certificate is traceability to the International System of Unit (SI)

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence approximately 95%

Calibrated by : Mr.Thippatai Mungpungklang

Approved by :

Ms. Budsagorn Patcha

Authorized Signatory

This certificate may not be reproduced except in full unless permission for the reproduction has been obtained in writing from the laboratory.



Measuretronix Limited
2425/2 Lat Phrao Road, Saphan Song
Wangthonglang, Bangkok 10310, Thailand
Phone : 0-2514-1000, 0-2514-1234
Fax : 0-2514-0001, 0-2514-0003
Website : www.measuretronix.com



Certificate of Calibration

Certificate Number : LF25-0305
Equipment : Thermometer
Manufacturer : Fluke
Model : 51
Serial Number : 5910857
Asset Number : 5910857
Customer : Thal Unique Co., Ltd.
80-82 Prachathipatal Road,
Bangkhunphrom, Pranakorn,
Bangkok 10200
Date of Calibrate : 6-Jun-2025
Date of Issue : 6-Jun-2025

This calibration certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI).

This calibration certificate applies only to the item identified and shall not be reproduced other than in full, without specific written approved by Measuretronix Cal-Lab. Calibration certificates without signature are not valid.


The measurements marked with an asterisk () in this certificate are outside our range of accreditation. They have been included for completeness.*

The Calibration interval (Cal.Due) is the responsibility of the end user.

Calibrated by


Mr. Samak Uaonkaonoi
Metrology Technician

Approved by


Miss Juthamas Sukhathainirun
Cal-Lab Manager



Agilent Technologies

Certificate of Analysis

FID-TCD Performance Evaluation Sample Kit

Agilent Part
Number: 5080-8842, 18710-60170

Sample Lot
Number: 0006750304

This analytical reference material was manufactured and verified in accordance with an ISO 9001 registered quality system, and the analyte concentrations were verified by an ISO 17025 accredited laboratory. The certified value for each analyte was determined gravimetrically.

Concentrations:

n-tetradecane	0.218 g/L ($\pm 0.5\%$)	0.033 w/w %
n-pentadecane	0.218 g/L ($\pm 0.5\%$)	0.033 w/w %
n-hexadecane	0.218 g/L ($\pm 0.5\%$)	0.033 w/w %

Solvent: hexane


Calibrated Class A glassware and clean bottles were used in the manufacture of this standard. Balances used in the manufacture of this standard are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z-540-1 and ISO 9001.

Purities:

n-tetradecane	99.6%
n-pentadecane	99%
n-hexadecane	99.5%
hexane	99%

Typical Analytical Spectrum or Chromatography

GC Chromatography – n-tetradecane, n-pentadecane, and n-hexadecane in hexane

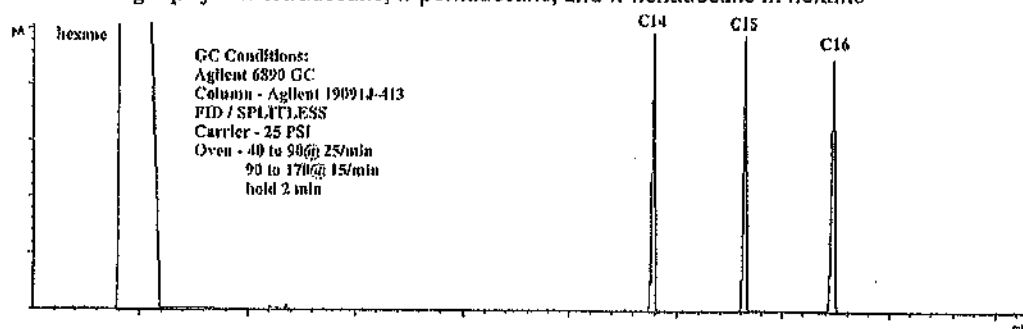

Date of release: 30 June 2023

Date of expiration: 31 July 2025

Monica Bourgeois
Monica Bourgeois
QMS Representative

ลำดับที่ 3

ระดับเสียงในบรรยากาศ



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-69/0204

MTC No. EEL. BP. 152/0169

CALIBRATION CERTIFICATE

Submitted by : S.P.S.CONSULTING SERVICE CO.,LTD.

Address : 7 Soi Phaholyothin 24, Phaholyothin Road, Jompol, Chatuchak, Bangkok 10900.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Sound Calibrator

Manufacturer : ACO

Model : 2127

Serial No. : 130006

Ambient Environment

Temperature : $(23 \pm 3) ^\circ\text{C}$

Relative Humidity : $(50 \pm 15) \%$

Ambient Pressure : $(101.325 \pm 1.500) \text{ kPa}$

- Standards used :**
1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.
 2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.
 3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.
 4. Digital Multimeter Agilent 34401A S/N MY44005560.
 5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.
 6. Audio Analyzer Keithley 2015-P S/N 4106495.
 7. Condenser Microphone Bruel&Kjaer 4180 S/N 2889871.

Calibration Procedure: CP-102-04 based on IEC 60942-2003; The sound pressure level generated by sound calibrator under test shall be measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 29 Jan. 2026

Date of Calibration : 11 Feb. 2026

1 / 2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory

668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office

196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-69/0204

MTC No. EEL. BP. 152/0169

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20 μ Pa at 1000 Hz

Acoustic Output in dB re 20 μ Pa, Corrected to Reference Conditions: 101.325 kPa, 23.0 °C and 50 %RH.

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	93.89	-0.11	± 0.10	± 0.40 dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	999.9	-0.1	± 1.5	$\pm 1.0\%$

3. Total Distortion

Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	1.90	± 0.50	$\pm 3.0\%$

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Calibrated by :


(Mr. Weerachai Deechaiyae)

Approved by :


(Mr. Prawate Kluaypa)
Director

Date of Calibration : 11 Feb. 2026

Date of Issue : 12 Feb. 2026

Electrical and Electronic Standards Laboratory
Industrial Metrology and Testing Service Centre

Ref : 2011269012900497001

End of Certificate

2 / 2

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory

668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office

196 Phahonyothin Road, Ladyao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Noise R_306/26

Sound Level Meter Calibration Report

Acoustic Calibrator Data						
Brand	ACO			Number	AC 03/56	
Model	2127			Serial No.	130006	
Calibration Range	94 dB, 1000 Hz			Last Calibration	11 February 2026	
				Due Date	11 February 2027	
Calibration Data						
Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-R45	ACO	6236	00192057	10 May 2026	93.9	93.9
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.81 ± 0.10 dB	

Calibrated by :

Heeson L.
(Mr. Heeson Lormae)

Approved by :

Yutthana J.
(Mr. Yutthana Tanatharanit)

ลำดับที่ 4

คุณภาพน้ำเสียอุตสาหกรรม



ISOCAL TECHNOLOGY CO.,LTD.

Industrial Instrument Calibration Center

170/405 Moo 3 Serithai Rd., Kannayao Kannayao Bangkok 10230

Tel. 0-2906-3040-1 Fax. 0-2919-9948

Certificate of Calibration

Certificate Number : C25/0106B

Page : 1 of 3

Customer : S.P.S. Consulting Service Co.,Ltd.

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol,
Chatuchak, Bangkok 10900

Equipment Name : pH Meter
Model : HQ1110
Serial No. : 232651110029
ID No. : -
Manufacture : Hach
Environment : Ambient Temperature (23 ± 2) °C
: Relative Humidity (50 ± 15) %
Location of Calibration : In-Lab
Date of Received : 23-Jun-2025
Date of Calibration : 24-Jun-2025
Date of Issued : 27-Jun-2025
Condition as Received : Normal
Calibration Method : Calibration Procedure Number WI-10A-2

This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

This certificate shall not be reproduced other than in full except without the prior written approval of the Head of Calibration Laboratory of Isocal Technology Co.,Ltd.

Calibrated by : Miss Watchara Inchaidee

Technical

Approved by :

(Mr. Narong Phetjaron)



ISOCAL TECHNOLOGY CO.,LTD.

Calibration Report

Certificate Number : C25/0106B

Page : 2 of 3

Equipment Standards Used

Description	Serial No.	Certificate No.	Cal. Due Date
Multi Function Calibrator	2197	E2U2400315	15-Oct-25
pH Solution	1.09435.1000	HC32117435	31-Mar-26
pH Solution	1.09439.1000	HC33442639	30-Nov-26
pH Solution	1.09438.1000	HC20293938	31-Aug-25

Traceability :-

The calibration within the certificate are traceable through

: NIST - National Institute of Standard and Technology , U.S.A.

: PTB - Physikalisch-Technische Bundesanstalt , Germany

: NIMT - National Institute of Metrology, Thailand

to the International System of Units (SI).



ISOCAL TECHNOLOGY CO.,LTD.

Calibration Report

Certificate Number : C25/0106B

Page : 3 of 3

Result of Calibration : Adjustment (Yes)

Function : pH Measurement with Solution @ 25 °C

Scale Range : 4.01 pH to 10.01 pH

Resolution : 0.01 pH

Standard Value (pH)	UUC Reading (pH)	Error (pH)	Uncertainty (pH)
4.01	3.96	-0.05	0.012
7.01	7.03	0.02	0.012
10.01	9.97	-0.04	0.012

Function : pH Measurement

Scale Range : 0 pH to 14 pH

Resolution : 0.01 pH

Standard Normal (pH)	UUC Reading (pH)	Error (pH)	Uncertainty (pH)
0	0.00	0.00	0.006
1	1.00	0.00	0.006
2	2.00	0.00	0.006
3	3.00	0.00	0.006
4	4.00	0.00	0.006
5	5.00	0.00	0.006
6	6.00	0.00	0.006
7	7.00	0.00	0.006
8	8.00	0.00	0.006
9	9.00	0.00	0.006
10	10.00	0.00	0.006
11	11.00	0.00	0.006
12	12.00	0.00	0.006
13	13.00	0.00	0.006
14	14.00	0.00	0.006

... END ...

CERT.No.: HS-W015C

Calibration Date : 18 Mar 25
 Submitted by : S.P.S CONSULTING SERVICE CO.,LTD
 7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol,
 Chatuchak, Bangkok, Thailand 10900

Avg Room Temp : 20 °C
 Avg Water Temp : 20 °C
 Air Pressure : 760.00 mmHg
 Salinity : 0 ppt

Model : YSI 5000
 S/N : 15B100751
 Probe : YSI 5010
 S/N : 22D100097
 ID NO. : -
 Air Temp ref : S/N. F8065C26
 Barometric ref : S/N. F8065C26
 Water Temp ref : -
 ID NO. HS001
 Technician : Kittipong M.

Calibration Details

Calibration Point	100% air sat. (@20 °C, DO = 9.09 mg/l)	(status)	(status)
Measurement 1 (mg/l)	9.08	(PASS)	-
Measurement 2 (mg/l)	9.08	(PASS)	-
Measurement 3 (mg/l)	9.08	(PASS)	-
Measurement 4 (mg/l)	9.07	(PASS)	-
Measurement 5 (mg/l)	9.07	(PASS)	-
Measurement 6 (mg/l)	9.07	(PASS)	-
Measurement 7 (mg/l)	9.07	(PASS)	-
Measurement 8 (mg/l)	9.07	(PASS)	-
Measurement 9 (mg/l)	9.07	(PASS)	-
Measurement 10 (mg/l)	9.07	(PASS)	-

Mean Measurement	9.07	mg/l	-	-
Inaccuracy	0.02	mg/l	-	-

Overall Status (PASS)

Manufacturer Specification

Accuracy = +/- 0.02 mg/l

- 1) This certificate is issued based on the result that are found as shown on date and place of test only.
- 2) The calibration procedure followed in accordance with Harikul Science Co., Ltd.
- 3) This result shall not be used for advertising purpose.



Technician Signature
 (Kittipong Maekwong)



Laboratory Manager
 (Natenapha Pisatkunchon)

CERT.No.: HS-X014C

Certificate of Calibration

Calibration Date : 16 March 2026

Submitted by : S.P.S CONSULTING SERVICE CO.,LTD

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol,

Chatuchak, Bangkok, Thailand 10900

Avg Room Temp : 20 °C

Avg Water Temp : 20 °C

Air Pressure : 760.00 mmHg

Salinity : 0 ppt

Model : YSI 5000

S/N : 15B100751

Probe : YSI 5010

S/N : 22D100097

ID NO. :

Air Temp ref : S/N. F8065C26

Barometric ref : S/N. F8065C26

Water Temp ref : -

ID NO. HS001

Technician : Kittipong M.

Calibration Details

Calibration Point	100% air sat. (@20 °C, DO = 9.09 mg/l)	(status)	(status)
Measurement 1 (mg/l)	9.09	(PASS)	-
Measurement 2 (mg/l)	9.09	(PASS)	-
Measurement 3 (mg/l)	9.09	(PASS)	-
Measurement 4 (mg/l)	9.09	(PASS)	-
Measurement 5 (mg/l)	9.09	(PASS)	-
Measurement 6 (mg/l)	9.08	(PASS)	-
Measurement 7 (mg/l)	9.08	(PASS)	-
Measurement 8 (mg/l)	9.08	(PASS)	-
Measurement 9 (mg/l)	9.08	(PASS)	-
Measurement 10 (mg/l)	9.08	(PASS)	-

Mean Measurement	9.09	mg/l	-	-
Inaccuracy	0.00	mg/l	-	-

Overall Status (PASS)

Manufacturer Specification

Accuracy = +/- 0.02 mg/l

- 1) This certificate is issued based on the result that are found as shown on date and place of test only.
- 2) The calibration procedure followed in accordance with Harikul Science Co., Ltd.
- 3) This result shall not be used for advertising purpose.



Technician Signature

(Kittipong Maekwong)



Laboratory Manager

(Natenapha Pisatkunchon)



QUALITY CALIBRATION CO., LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com

CERTIFICATE No : 25T0521

REFERENCE No : 75853-2

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : COD REACTOR

MANUFACTURER : HACH

MODEL : DRB 200

SERIAL No : 15110C0498

ID No : CRB 06/59

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : CHAICHARN CH.

CALIBRATION DATE : 03-Feb-25

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 03-Feb-25

RECEIVED DATE : 15-Jan-25

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.





QUALITY CALIBRATION CO., LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 25T0521

PAGE : 2 OF 2

Calibration Report


EQUIPMENT : COD REACTOR
MANUFACTURER : HACH
ID NUMBER : CRB 06/59
RECEIVED DATE : 15-Jan-25
AMBIENT TEMPERATURE : 23° C ± 1° C
MODEL : DRB 200
SERIAL NUMBER : 15110C0498
CALIBRATION DATE : 03-Feb-25
RELATIVE HUMIDITY : 53 %RH ± 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT METHOD WITH CALIBRATED THERMOCOUPLE TYPE K UNDER NO LOAD CONDITION. THE THERMOCOUPLES WERE PLACED ON POINTS AND LOCATED AS THE PICTURE.
2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH TC TYPE K	HYDRA 2635A	7301307	24T6467	26-Jun-25
3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO., LTD.

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

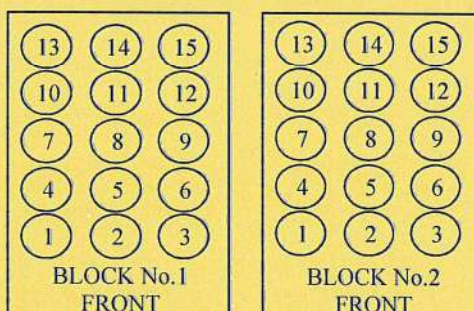

Block No.	1	2
Calibration Point (°C)	150	150
Controller temperature (°C)	145	145
Indicating Temperature	145	145
Measured Temperature (°C) at Spread Locations	1	150.23
	2	149.73
	3	150.29
	4	150.04
	5	150.09
	6	150.74
	7	149.97
	8	150.76
	9	150.54
	10	149.44
	11	150.12
	12	149.93
	13	149.19
	14	148.96
	15	149.09
Uncertainty of Measurement(± °C)	0.88	0.88

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2 : LOCATION 10 WAS REFERENCE LOCATION.

NOTE 3 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





CERTIFICATE No : 26T0464

REFERENCE No : 79659-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : COD REACTOR

MANUFACTURER : HACH

MODEL : DRB 200

SERIAL No : 15110C0497

ID No : DRB 04/59

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : SOMCHAI S.

CALIBRATION DATE : 30-Jan-26

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 30-Jan-26

RECEIVED DATE : 30-Jan-26





CERTIFICATE No : 26T0464

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : COD REACTOR
MANUFACTURER : HACH
ID NUMBER : DRB 04/59
RECEIVED DATE : 30-Jan-26
AMBIENT TEMPERATURE : 23° C ± 1° C

MODEL : DRB 200
SERIAL NUMBER : 15110C0497
CALIBRATION DATE : 30-Jan-26
RELATIVE HUMIDITY : 54 %RH ± 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT METHOD WITH CALIBRATED THERMOCOUPLE TYPE K UNDER NO LOAD CONDITION. THE THERMOCOUPLES WERE PLACED ON POINTS AND LOCATED AS THE PICTURE.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT

MODEL

SERIAL No

CERTIFICATE No

DUE DATE

1) DATA LOGGER WITH TC TYPE K

HYDRA 2635A

6849323

25T5342

18-Jun-26


3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO., LTD.

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

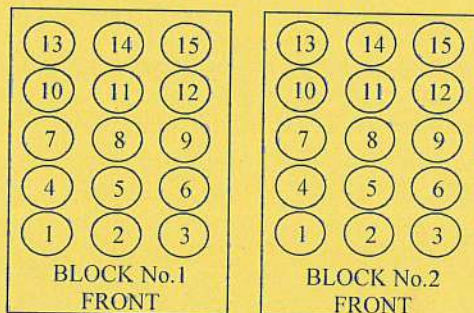

TEMPERATURE MEASUREMENT ACCURACY TEST

Block No.	1	2
Controller temperature (°C)	144	145
Indicating Temperature	144	145
Measured Temperature (°C) at Spread Locations	1	149.3
	2	149.1
	3	149.9
	4	149.6
	5	149.3
	6	149.5
	7	149.1
	8	149.7
	9	149.7
	10	149.5
	11	149.9
	12	149.4
	13	150.2
	14	149.4
	15	149.6
Uncertainty of Measurement(± °C)	0.89	0.89

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2 : LOCATION 10 WAS REFERENCE LOCATION.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k =2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





CERTIFICATE No : 25M2256

REFERENCE No : 76365-3

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE

MANUFACTURER : SARTORIUS

MODEL : BSA224S-CW

SERIAL No : 36591843

ID No : BA09/61

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.

CALIBRATION DATE : 07-Mar-25

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 13-Mar-25

RECEIVED DATE : 07-Mar-25

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.





CERTIFICATE No : 25M2256

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : BSA224S-CW
MANUFACTURER : SARTORIUS S/N : 36591843
ID No : BA09/61 RECEIVED DATE : 07-Mar-25
AIR PRESSURE : 1009mbar $\pm$ 1mbar CALIBRATION DATE : 07-Mar-25
AMBIENT TEMPERATURE : 24° C $\pm$ 1° C RELATIVE HUMIDITY : 52 %RH $\pm$ 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

<u>INSTRUMENT</u>	<u>MODEL</u>	<u>SERIAL No</u>	<u>CERTIFICATE No</u>	<u>DUE DATE</u>
1) STANDARD WEIGHT SET	E2	QK-I-151	C02250116	28-Jan-27
2) STANDARD WEIGHT	E2	15843	C02250117	29-Jan-27

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT


1. ZERO SETTING FUNCTION : NORMAL

2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0.000071 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ($\pm$ g)
0.00	0.0000	0.0000	0.00012
0.10	0.1000	0.0000	0.00012
0.20	0.2000	0.0000	0.00012
0.50	0.5000	0.0000	0.00012
1.00	1.0000	0.0000	0.00012
2.00	2.0000	0.0000	0.00012
5.00	5.0000	0.0000	0.00012
10.00	10.0000	0.0000	0.00012
20.00	20.0001	-0.0001	0.00012
50.00	50.0000	0.0000	0.00014
100.00	100.0001	-0.0001	0.00019
200.00	200.0001	-0.0001	0.00032

5. OFF CENTER LOADING ERROR

POINT	READING (g)
1	100.0000
2	100.0000
3	100.0000
4	100.0000
5	100.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





CERTIFICATE No : 26M2268

REFERENCE No : 80204-3

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE

MANUFACTURER : SARTORIUS

MODEL : BSA224S-CW

SERIAL No : 36591843

ID No : BA 09/61

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : SUCHAT S.

CALIBRATION DATE : 05-Mar-26

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 06-Mar-26

RECEIVED DATE : 05-Mar-26





CERTIFICATE No : 26M2268

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE **MODEL** : BSA224S-CW
MANUFACTURER : SARTORIUS **S/N** : 36591843
ID No : BA 09/61 **RECEIVED DATE** : 05-Mar-26
AIR PRESSURE : 1004mbar $\pm$ 1mbar **CALIBRATION DATE** : 05-Mar-26
AMBIENT TEMPERATURE : 25° C $\pm$ 1° C **RELATIVE HUMIDITY** : 50 %RH $\pm$ 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

<u>INSTRUMENT</u>	<u>MODEL</u>	<u>SERIAL No</u>	<u>CERTIFICATE No</u>	<u>DUE DATE</u>
1) STANDARD WEIGHT SET	E2	QK-I-151	C02250116	28-Jan-27
2) STANDARD WEIGHT	E2	15843	C02250117	29-Jan-27

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0.000055 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ($\pm$ g)
0.0	0.0000	0.0000	0.00010
0.1	0.1000	0.0000	0.00011
0.2	0.2000	0.0000	0.00010
0.5	0.5000	0.0000	0.00011
1.0	1.0000	0.0000	0.00011
2.0	2.0000	0.0000	0.00011
5.0	5.0000	0.0000	0.00011
10.0	10.0000	0.0000	0.00011
20.0	20.0001	-0.0001	0.00011
50.0	50.0000	0.0000	0.00013
100.0	100.0001	-0.0001	0.00019
200.0	200.0001	-0.0001	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	100.0000
2	100.0000
3	100.0000
4	100.0000
5	100.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN
associates



Cert. No. : SP25026

Pages : 1 of 4

Calibration Certificate

Equipment : UV-VIS SPECTROPHOTOMETER
Manufacturer : PERKINELMER
Model : LAMBDA 25
Serial No.: 501S14123010
ID No.: SP03/58
Calibration Mode : WAVELENGTH ACCURACY
PHOTOMETRIC ACCURACY
STRAY LIGHT

Condition As Found : GOOD

Customer : S.P.S CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN ROAD,
CHOMPHON SUB-DISTRICT, CHATUCHAK DISTRICT,
BANGKOK PROVINCE 10900 THAILAND.

Location : ORGANIC LABORATORY IV

Ambient Temperature : (22.9 $\pm$ 5) °C
Relative Humidity : (53.7 $\pm$ 25) %

Received Date : 22 AUGUST 2025
Calibration Date : 22 AUGUST 2025
Date of Issue : 25 AUGUST 2025

Calibrated by :

Nitinun Srihawan

Approved by :

Wichok B.
(Wichok Ekpongpradit)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : SP25026

Job No. : VC68SP0019

Pages : 2 of 4

Calibration Method :

This instrument was calibrated by using on-site calibration procedure In-house method : CP-SP-01

The calibration procedure to direct measurement wavelength accuracy by using wavelength standard solution, Photometric accuracy by using absorbance standard filter and absorbance standard solution

The calibration procedure used was based on ASTM E275-01, ASTM E925-02

Condition of this result of calibration :

1. Certified reference materials

<u>Material</u>	<u>Ref. type</u>	<u>Cell serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Holmium liquid	RM-HL	29706	126461	24/10/2026
Didymium liquid	RM-DL	28912	126462	24/10/2026
Neutral density filter	RM-1N2N3N	13877	126457	24/10/2026
Potassium dichromate solutions	RM-0204060810	14204	126497	25/10/2026
Potassium Iodide solution	-	KI-0701-001	CI-0185-24	14/05/2026

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 The UK National Physical Laboratory (NPL)

Result of calibration : Wavelength Accuracy

(Without adjustment)

Material	Certified Values of Reference Material (nm)	UUC* Reading (nm)	Error (nm)	Uncertainty ± (nm)	k Factor
RM-HL	278.13	278.21	0.08	0.16	2.00
	361.25	361.39	0.14	0.16	2.00
	467.82	467.71	-0.11	0.16	2.00
	536.56	536.50	-0.06	0.16	2.00
	640.50	640.36	-0.14	0.16	2.00
RM-DL	740.09	739.85	-0.24	0.16	2.00
	864.94	865.12	0.18	0.16	2.00

UUC* = Unit Under Calibration

Cert. No. : SP25026
Job No. : VC68SP0019
Pages : 3 of 4

Result of calibration : Photometric Accuracy

Material	Wavelength (nm)	Filter S/N	Nominal Absorbance (A)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor
Neutral Density glass filter	440.0	29381	0.5	0.5443	0.5413	-0.0030	0.0043	2.00
		29914	0.7	0.7484	0.7455	-0.0029	0.0054	2.00
		29360	1.0	1.0527	1.0535	0.0008	0.0032	2.00
	465.0	29381	0.5	0.4948	0.4922	-0.0026	0.0041	2.00
		29914	0.7	0.6906	0.6877	-0.0029	0.0050	2.00
		29360	1.0	0.9695	0.9709	0.0014	0.0031	2.00
	546.1	29381	0.5	0.5090	0.5068	-0.0022	0.0036	2.00
		29914	0.7	0.6985	0.6960	-0.0025	0.0041	2.00
		29360	1.0	0.9814	0.9825	0.0011	0.0031	2.00
	590.0	29381	0.5	0.5375	0.5353	-0.0022	0.0034	2.00
		29914	0.7	0.7256	0.7231	-0.0025	0.0037	2.00
		29360	1.0	1.0213	1.0219	0.0006	0.0032	2.00
	635.0	29381	0.5	0.5223	0.5202	-0.0021	0.0033	2.00
		29914	0.7	0.6927	0.6901	-0.0026	0.0036	2.00
		29360	1.0	0.9744	0.9750	0.0006	0.0032	2.00

UUC* = Unit Under Calibration

Cert. No. : SP25026
Job No. : VC68SP0019
Pages : 4 of 4

Result of calibration : Photometric Accuracy

(Without adjustment)

Material	Wavelength (nm)	Solution (mg/l)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor
Potassium dichromate solutions	235.0	20	0.2415	0.2443	0.0028	0.0101	2.00
		40	0.4866	0.4871	0.0005	0.0115	2.00
		60	0.7415	0.7295	-0.0120	0.0067	2.00
		80	0.9854	0.9844	-0.0010	0.0071	2.00
		100	1.2444	1.2425	-0.0019	0.0073	2.00

UUC* = Unit Under Calibration

Condition of this result of calibration : Spectrophotometer PERKINELMER Model LAMBDA 25 S/N 501S14123010

Resolution of Wavelength Mode 0.1 nm

Resolution of Photometric Mode 0.001 A

Parameter Setting

Measurement Mode Wavelength, Absorbance

Wavelength Scan 190 nm - 1100 nm

Scanning Speed 7.5 nm/min

Band width(Wavelength) 1.0

Band width(Vis) 1.0

Band width(Uv) 1.0

Stray Light** UUC* Reading at 220.0 nm	
Transimission T(%)	Absorbance(A)
0.020	3.7032

**Specific Acceptance :

Transmission ≤ 1.0 T(%), Absorbance ≥ 2.0 A

**Stray light not TISI Accredited

The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95%

End of Calibration Certificate

PinAAcle 900T Preventive Maintenance Report

Company Name: S.P.S. Consulting Service Co.,Ltd.

Instrument Location: 7, 24 Soi Phaholyothin,

Ladyao, Khet, Bangkok 10900

Instrument Serial No.: PTCS14111103

Date: 18 Jun 2026

PinAAcle 900T Preventive Maintenance (PM)

Company Name:	S.P.S. Consulting Service Co.,Ltd.		
Address (Instrument Location):	7, 24 Soi Phaholyothin, Ladyao, Khet, Bangkok 10900		
Serial Number:	PTCS14111103	PM Number:	1 of 2
Customer Name (if applicable):	K. Phenpha	Telephone Number:	083-926-9252
Customer Support Engineer Name:	K. Chayanon	Service Order Number:	WO-11540403
Date PM Performed: (DD-MMM-YYYY)	18 Jun 2026	Next PM Due Date: (DD-MMM-YYYY)	18 Jun 2027
Standard Labor Hours to Complete PM :		5 hours	

Part Number	Release	Publication Date	
09370143 Rev.9	A	January 2018	

Scope

The purpose of this PM is to ensure the continued functionality of the PinAAcle 900T by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer.

The customer should save their method before the PM begins.

General Instructions:

The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM. Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files. The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer. Update the PM sticker and instrument logbook as required.

Copyright Information

This document contains proprietary information that is protected by copyright. All rights are reserved. No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of PerkinElmer, Inc. **Copyright © 2013 PerkinElmer, Inc.**

Trademarks

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners.

Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no Warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.

PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

Component List

Component / Specific Model	Serial #	Configuration Notes
PinAAcle900T	PTCS14111103	Winlab32
Fias100	100S14090404	Winlab32

Parts Lists

Parts Included with the PM		
Part Number (if applicable)	Description	Quantity
B0501696	Fan Filters	1
B3002013	THGA Contact Cylinders	1
B3141064	Glycerol for THGA Cooling	1
N3160156	O-Ring Kits for Sampling Introduction (Stainless Steels Nebulizer)	N/A
N3160157	O-Ring Kits for Sampling Introduction (Plastic Nebulizer)	2
N9301714	Replacement Acetylene Filter Cartridge	1
TH001022	Replacement Air Filter Cartridge	1

Additional Reagents and Standards Required for PM				
Part Number (if applicable)	Description	Quality	Batch/Lot #	Expired Date (MM/YY)
N9300183	1000 mg/L Copper Standard	AR	28-83CUY1	Nov 26
N9300244	GFAAS Mixed Standard	AR	60-004CRY1	Jun 26

Additional Reagents and Standards Required for PM (Customer Support Solution)				
Part Number (if applicable)	Description	Quantity	Batch/Lot #	Expiration Date (MM/YY)
N/A	DI Water	250 ml.	AR	AR
N/A	0.5% HNO ₃	250 ml.	AR	AR

Additional Tools Required for PM			
Part Number (if applicable)	Description	Quantity	Serial #
N1013000	0.2A Neutral density filter	1	101N0089015
N1013002	1.0A Neutral density filter	1	101N0089015
B3100652 Or N9307029	Electronic Flow Meter	1	NA
B0505495	Test Jig	1	NA
03030997	System 2 EDL Driver	1	030309-97E
N3050605	As System 2 EDL	1	000003-26798A
N3050121	Cu Lumina HCL	1	060419-030180
N3050109	Ba Lumina HCL	1	061219-020041
N3050139	K Lumina HCL	1	030819-010130
N3050152	Ni Lumina HCL	1	052719-020020
N3050119	Cr Lumina HCL	1	060419-030180

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. General:

- ✓ Review the instrument performance with the customer and document any recent problems.
- ✓ Inspect the customer log book and make any appropriate PM entries.
- ✓ Perform general inspection of system for cleanliness.

2. PC Instrument Software:

- ✓ Instrument Software user files/databases archived, packed, and/or deleted as needed.

3. Mechanical:

- ✓ Inspect and clean all fans and filters. Replace filters if necessary
- ✓ Inspect all gas and water lines for leaks and/or wear. Replace if needed. Thoroughly inspect all quick connects. Replace the Y connector, P/N 09921079, if needed.
- ✓ Clean exterior of the instrument.

3.1 Flame Technique

- ✓ Inspect the burner head, burner chamber, and nebulizer. Clean if needed as stated in the Hardware Guide.
- ✓ Check burner head dimensions with the feeler gauge as stated in the Hardware Guide in the Maintenance chapter section on cleaning the burner head and checking sloth width. Replace if out of specification
- ✓ Check the condition of the end cap, burner head, and nebulizer O-rings. Replace if necessary.
- ✓ Check the drain system for signs of wear. Replace worn or damaged parts.
- ✓ Visually check for proper flame conditions when igniting the Air-C₂H₂ and N₂O-C₂H₂ flames (if applicable).

3.2 THGA Technique

- ✓ Inspect the pole pieces and clean where the pole pieces contact the furnace. Replace the pole piece p-rings as needed, P/N's B0501018 & B0501250. Grease the O-rings as needed with Apiezon L grease, P/N 09905148
- ✓ Inspect the four insulation pads on the front contact housing of the THGA in furnace. If the pads are missing replace the THGA furnace or replace the insulator pads on the furnace.
- ✓ Inspect the graphite tube and clean the contact cylinders. Replace if necessary.
- ✓ Check internal and external gas flows with the Electronic Gas Flow Meter and the Gas Flow Test Probe as described in the Service Manual. Correct if necessary.
- ✓ Check furnace open/close function.
- ✓ Verify the operation of the GFTV Camera for proper operation and viewing alignment in the furnace camera Tube View window. Align if needed.
- ✓ Check the operation of the Halogen Light ASSY for the GFTV Camera. Replace if needed.
- ✓ Check the water level/quality in the recirculation (if applicable). Add distilled water if necessary.
- ✓ Check the cooling system fluid flow rate with the FCS In-Line Flow Meter for proper levels if needed. Refer to SDB# COSY008.STN

- ✓ Perform Cooling System maintenance if needed per SDB# COSY005.STN.
- ✓ Check auto sampler operation.
- ✓ Perform an auto sampler check valve test as described in the Service Manual.
- ✓ Lubricate the spindles of the auto sampler pumps and all moving parts of the tray mechanics as described in the Service Manual.
- ✓ Inspect the auto sampler sampling capillary as described in the Service Manual. Replace if necessary.

4. Electrical:

- ✓ Inspect PC boards. Clean if necessary.
- ✓ Carefully check all internal and external cable connections.
- ✓ Check instrument firmware revisions upgrade to current levels (if necessary)
- ✓ Run Diagnostics Test within the Advanced function of the Spectrometer page. Check the results in the service log folder in the Spectrometer BM Log Viewer.

5. Optics:

- ✓ Inspect and clean the sample compartment windows, if needed.
- ✓ Inspect and clean the furnace windows, if needed.
- ✓ Inspect and clean the GFTV camera lens, if needed.
- ✓ Inspect optics. Clean or replace if necessary,

6. Gasses:

- ✓ Verify that the Gasses supplied to the instrument are within the pressure and purity specifications found in the PinAAcle 900 Series Pre-installation Checklist SDB.
- ✓ Verify that the air filter element is dry. Replace if necessary.

7. Flame Interlock Check:

Description: Check to ensure that all safety interlocks are closed.

Parameter	Specification	Test Results	Pass/Fail
Flame Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
Drain Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
Nebulizer Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
C ₂ H ₂ Pressure Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
Air Pressure Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
Burner Head Sensor	Choosing Nitrous Oxide as the oxidant should trigger an interlock shuts down	Active	Passed

8. After PM Performance tests [Flame]:

8.1 Detector Linearity with Barium

Description: Ensures that the detector is linear in the Visible Range.

Parameter	Specification	Certificate Value at 553.6 nm (Abs.)	Test Results	Pass/Fail
1.0 A ND Filter	± 5% from Cert.	2.0405	1.9997	Passed
0.2 A ND Filter	± 5% from Cert.	0.1953	0.1855	Passed

8.2 Baseline Noise at 1.0 Absorbance with Barium

Description: Ensures that a high absorbance will not produce excessive noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.010	0.001	Passed

8.3 AA Baseline Noise with Copper

Description: Check baseline noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.001	0.0001	Passed

8.4 D₂ Background Compensation with Copper

Description: Verifies the instruments ability to compensate for Background absorption.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.010	0.0001	Passed

8.5 AA-BG Baseline Noise with Copper

Description: Ensures that background correction does not produce excessive noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.005	0.0003	Passed

8.6 AA-BG Baseline Noise with Arsenic

Description: Ensures that background correction does not produce excessive noise at a low wavelength.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.005	0.0001	Passed

8.7 Flame Sensitivity

Description: Instrument Sensitivity checked against Copper standard.

Standard Copper Sensitivity	Specification	Results (Abs.)	Pass/Fail
5 mg/L Sensitivity SS Neb (if applicable)	> 0.250 Abs.	NA	Not Applicable
2 mg/L Sensitivity HS Neb (if applicable)	> 0.250 Abs.	0.356	Passed

9. After PM Performance tests [THGA]:

9.1 Furnace Gas Flows

Description: Ensures the flow rates are within specification.

Parameter	Specification	Test Results	Pass/Fail
Internal Flow Rate	250 mL/min $\pm$ 25 mL/min	260	Passed
External Flow Rate	100 mL/min $\pm$ 10 mL/min	105	Passed

9.2 Chromium Baseline Noise

Description: Signal to noise check.

Parameter	Specification	Results	Pass/Fail
Baseline Noise	≤ 0.005 Abs.	0.0002	Passed
Standard Deviation	≤ 0.005	0.0001	Passed

9.3 Chromium Characteristic Mass and Precision

Description: Calculate the characteristic mass using the characteristic mass tool and precision from the integrated absorbance values.

Parameter	Specification	Results	Pass/Fail
Cr m_0 Results	≤ 7.0 pg/0.0044 A-s	5.4	Passed
Precision	≤ 2.0 %	0.14	Passed

9.4 Copper Characteristic Mass and Zeeman Ratio

Description: Calculate the characteristic mass using the characteristic mass tool and check the Zeeman Ratio.

Parameter	Specification	Results	Pass/Fail
Cu m ₀ Result	≤ 16.5 pg/0.0044 A-s	14.5	Passed
Zeeman Ratio	0.52 ± 0.04	0.54	Passed

10. Review:

- ☒ Review with the customer PM work performed.
- ☒ Review with the customer routine maintenance procedures.
- ☒ Discuss recommended customer supplied materials to have on hand.
- ☒ Attach PM sticker.

Additional Comments

Additional Comments Regarding the PM	
Zeeman Ratio	$= \frac{\text{Atomic Signal (Peak area)}}{\text{Atomic Signal (Peak area)} + \text{Background Signal (Peak area)}}$ $= \frac{0.1551}{0.1551 + 0.1315}$ $= 0.54$

Review

<i>The preventive maintenance checks and if applicable performance tests for PinAAcle 900T have been completed.</i>	
<i>This PinAAcle 900T Passes ☒ Fails ☐ the preventive maintenance.</i>	
Review of Preventive Maintenance:	
Authorized PerkinElmer Representative: Chayanan ✱	Date: 18 Jun 2026 (DD-MMM-YYYY)
Authorized Customer Representative: [Signature]	Date: 18 Jun 2026 (DD-MMM-YYYY)



CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : CONDUCTIVITY METER
MANUFACTURER : METTLER TOLEDO
MODEL / TYPE : SEVEN COMPACT S230
SERIAL NO. : C141708983/5821320179[CD 05/65]
CLID. NO. : 272300452
JOB CONTROL NO. : 250204013412
CALIBRATION SERVICE : ☒ IN-LABORATORY ☐ ON-SITE

CUSTOMER : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24 ROAD, JOMPOL,
CHATUCHAK, BANGKOK 10900

DATE OF RECEIVED : 04 February 2025

DATE OF ISSUED : 06 February 2025

The report of calibration shall not be reproduced except in full without approval of the calibration Laboratory Co., Ltd.

Calibrated By : Sukgasem Sechanart

Wenick Inchaisri

Calibration Engineer

Approved By :

Mongkol Yotsoontorn

Authorized Signatory

06 February 2025



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q25013412

F3-011-05/12-23

page 1 of 4



@clccalibration

REPORT OF CALIBRATION

FOR

NOMENCLATURE	:	CONDUCTIVITY METER
MANUFACTURER	:	METTLER TOLEDO
MODEL / TYPE	:	SEVEN COMPACT S230
SERIAL NO.	:	C141708983/5821320179[CD 05/65]
DATE OF CALIBRATION	:	05 February 2025

ENVIRONMENT CONDITIONS :

Temperature : $(25 \pm 2.5) ^\circ\text{C}$

Relative Humidity : $(50 \pm 15) \% \text{ RH}$

PROCEDURE USED :

This instrument [Conductivity Meter] was calibrated under procedure No. **WI-305-130**.

The calibration was performed by direct measurement with Certified Reference Material (CRM) and Reference Material (RM) .

This instrument [Temperature] was calibrated by comparison with Calibration Bath, Precision Thermometer and IPRT which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. Conductivity Solution , Hanna Product Code HI 7033L Lot Number 7830.
2. Potassium Chloride Solution (nominal 1.41 mS/cm)
3. Potassium Chloride Solution (nominal 12.8 mS/cm)
4. Calibration Bath, Kambic Model OB-22/2 ULT S/N. 17115653.
5. Precision Thermometer, ASL Model F201 S/N. 016168/09.
6. IPRT, ASL Model T100-250-1D S/N. PO106346-1-13.





CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



TRACEABILITY :

1. The measurements are traceable to International System of Units (SI) , through Hanna instruments.

Certificate No. 20F21 , Due Date June 2025 .

2. The measurements are traceable to International System of Units (SI) , through Sigma-Aldrich Canada Co.

Certificate No. HC30595403 , Due Date 31 January 2026 .

3. The measurements are traceable to International System of Units (SI) , through Sigma-Aldrich Canada Co.

Certificate No. HC20111554 , Due Date 30 September 2025.

4. The measurements are traceable to International System of Units (SI) , through Calibration Laboratory Co , Ltd.

Certificate No. Q24120999, Due Date 26 November 2025.

5. The measurements are traceable to International System of Units (SI) , through Thailand Institute of Scientific and Technological Research (TISTR). Certificate No. PSL-T 0424/67, Due Date 21 February 2025.

6. The measurements are traceable to International System of Units (SI) , through National Institute of Metrology (Thailand).

Certificate No. TT-0035-24, Due Date 01 March 2025.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q25013412

F3-011-05/12-23

page 3 of 4



@clccalibration

CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The table in the following gives the calibration results and associated measurement uncertainties of Conductivity Meter.

CALIBRATION DATA

1. Conductivity Solution Test @ 25°C

Standard Conductivity Solution	DUC Reading	Uncertainty of Measurement	k Factor
*84.00 µS/cm	84.02 µS/cm [Cell Constant 0.548589]	± 1.00 µS/cm	2,00
1414.0 µS/cm	1414 µS/cm [Cell Constant 0.548589]	± 21.0 µS/cm	2,00
12.83 mS/cm	12.84 mS/cm [Cell Constant 0.548589]	± 0.19 mS/cm	2,00

Note. The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 02 Page 91 of 138

* means Calibrations marked "Not TISI Accredited" in this Certificate have been included for completeness.

*2. TEMPERATURE RESULT

Immersion depth (mm)	Actual Temperature (°C)	DUC Reading (°C)	Correction (°C)	Uncertainty ± (°C)
100	25.01	24.9	+0.11	0.07

Technical Note. Type of sensor : Conductivity Probe

Probe Ø 12 mm

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor of $k = 2,00$.

Note. * means Calibrations marked "Not TISI Accredited" in this Certificate have been included for completeness.

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q25013412

F3-011-05/12-23

page 4 of 4





CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Road, Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com



CERTIFICATE OF CALIBRATION FOR

NOMENCLATURE : CONDUCTIVITY METER
MANUFACTURER : METTLER TOLEDO
MODEL / TYPE : SEVEN COMPACT S230
SERIAL NO. : C141708983/5821320179[CD 05/65]
CLID. NO. : 272300452
JOB CONTROL NO. : 260202014122
CALIBRATION SERVICE : ☒ IN-LABORATORY ☐ ON-SITE

CUSTOMER : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24 ROAD., JOMPOL,
CHATUCHAK, BANGKOK 10900

DATE OF RECEIVED : 02 February 2026

DATE OF ISSUED : 04 February 2026

The report of calibration shall not be reproduced except in full without approval of the calibration Laboratory Co., Ltd.

Calibrated By : Sukgasem Seehanart
Wenick Inchaisri
Calibration Engineer

Approved By : Mongkol Yotsoontorn
Authorized Signatory
04 February 2026



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to
the International System of Units (SI)

Certificate No. Q26014122

F3-011-05/12-23

page 1 of 4



@clccalibration

REPORT OF CALIBRATION

FOR

NOMENCLATURE : **CONDUCTIVITY METER**
MANUFACTURER : **METTLER TOLEDO**
MODEL / TYPE : **SEVEN COMPACT S230**
SERIAL NO. : **C141708983/5821320179[CD 05/65]**
DATE OF CALIBRATION : **03 February 2026**

ENVIRONMENT CONDITIONS :

Temperature : $(25 \pm 2.5) ^\circ\text{C}$

Relative Humidity : $(50 \pm 15) \% \text{ RH}$

PROCEDURE USED :

This instrument [Conductivity Meter] was calibrated under procedure No. **WI-305-130**.

The calibration was performed by direct measurement with Certified Reference Material (CRM) and Reference Material (RM) .

This instrument [Temperature] was calibrated by comparison with Temperature Bath, Precision Thermometer and IPRT which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. Conductivity Standard , Hanna Product Code HI7033L Lot Number 0101.
2. Potassium Chloride Solution, Sigma-Aldrich Canada Co Product No. 1.01203.0500.
3. Potassium Chloride Solution, Sigma-Aldrich Canada Co Product No. 1.01254.0500.
4. Temperature Bath, Jingmi Model RTS-35S S/N. 16339.
5. Precision Thermometer, ASL Model F200-A-8 S/N. 014433/03.
6. IPRT, ASL Model T100-250-1D S/N. PO106346-1-13.

Certificate No. Q26014122

F3-011-05/12-23

page 2 of 4





CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Road, Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com



TRACEABILITY :

1. The measurements are traceable to International System of Units (SI) , through Hanna instruments.

Certificate No. 07D45, Due Date April 2027.

2. The measurements are traceable to International System of Units (SI) , through Sigma-Aldrich Canada Co.

Lot Number. HC56384703, Due Date 31 January 2028.

3. The measurements are traceable to International System of Units (SI) , through Sigma-Aldrich Canada Co.

Lot Number. HC33528554, Due Date 30 November 2026.

4. The measurements are traceable to International System of Units (SI) , through Calibration Laboratory Co., Ltd.

Certificate No. Q25097314, Due Date 29 August 2026.

5. The measurements are traceable to International System of Units (SI) , through Thailand Institute of Scientific and Technological Research (TISTR). Certificate No. PSL-T 0177/68, Due Date 10 February 2026.

6. The measurements are traceable to International System of Units (SI) , through National Institute of Metrology (Thailand).

Certificate No. TT-1008-25, Due Date 04 March 2026.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q26014122

F3-011-05/12-23

page 3 of 4



@clccalibration

CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The table in the following gives the calibration results and associated measurement uncertainties of Conductivity Meter.

CALIBRATION DATA

1. Conductivity Solution Test @ 25°C

Standard Conductivity Solution	DUC Reading	Uncertainty of Measurement	k Factor
*84 µS/cm	83.95 µS/cm [Cell Constant 0.470]	± 1.15 µS/cm	2,00
1414 µS/cm	1414 µS/cm [Cell Constant 0.510]	± 21 µS/cm	2,00
12.83 mS/cm	12.83 mS/cm [Cell Constant 0.570]	± 0.19 mS/cm	2,00

Note. The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 02 Page 91 of 138

* means Calibrations marked "Not TISI Accredited" in this Certificate have been included for completeness.

*2. TEMPERATURE RESULT

Immersion depth (mm)	Actual Temperature (°C)	DUC Reading (°C)	Correction (°C)	Uncertainty ± (°C)
100	25.00	25.1	-0.10	0.08

Technical Note. Type of sensor : Conductivity Probe

Probe Ø 12 mm

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor of $k = 2$.

Note. * means Calibrations marked "Not TISI Accredited" in this Certificate have been included for completeness.

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q26014122

F3-011-05/12-23

page 4 of 4



ลำดับที่ 5

คุณภาพน้ำผิวดิน



ISOCAL TECHNOLOGY CO.,LTD.

Industrial Instrument Calibration Center

170/405 Moo 3 Serithai Rd., Kannayao Kannayao Bangkok 10230

Tel. 0-2906-3040-1 Fax. 0-2919-9948

Certificate of Calibration

Certificate Number : C25/0106B

Page : 1 of 3

Customer : S.P.S. Consulting Service Co.,Ltd.

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol,
Chatuchak, Bangkok 10900

Equipment Name : pH Meter
Model : HQ1110
Serial No. : 232651110029
ID No. : -
Manufacture : Hach
Environment : Ambient Temperature (23 ± 2) °C
: Relative Humidity (50 ± 15) %
Location of Calibration : In-Lab
Date of Received : 23-Jun-2025
Date of Calibration : 24-Jun-2025
Date of Issued : 27-Jun-2025
Condition as Received : Normal
Calibration Method : Calibration Procedure Number WI-10A-2

This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

This certificate shall not be reproduced other than in full except without the prior written approval of the Head of Calibration Laboratory of Isocal Technology Co.,Ltd.

Calibrated by : Miss Watchara Inchaidee

Technical

Approved by :

(Mr. Narong Phetjaroorn)



ISOCAL TECHNOLOGY CO.,LTD.

Calibration Report

Certificate Number : C25/0106B

Page : 2 of 3

Equipment Standards Used

Description	Serial No.	Certificate No.	Cal. Due Date
Multi Function Calibrator	2197	E2U2400315	15-Oct-25
pH Solution	1.09435.1000	HC32117435	31-Mar-26
pH Solution	1.09439.1000	HC33442639	30-Nov-26
pH Solution	1.09438.1000	HC20293938	31-Aug-25

Traceability :-

The calibration within the certificate are traceable through

: NIST - National Institute of Standard and Technology , U.S.A.

: PTB - Physikalisch-Technische Bundesanstalt , Germany

: NIMT - National Institute of Metrology, Thailand

to the International System of Units (SI).



ISOCAL TECHNOLOGY CO.,LTD.

Calibration Report

Certificate Number : C25/0106B

Page : 3 of 3

Result of Calibration : Adjustment (Yes)

Function : pH Measurement with Solution @ 25 °C

Scale Range : 4.01 pH to 10.01 pH

Resolution : 0.01 pH

Standard Value (pH)	UUC Reading (pH)	Error (pH)	Uncertainty (pH)
4.01	3.96	-0.05	0.012
7.01	7.03	0.02	0.012
10.01	9.97	-0.04	0.012

Function : pH Measurement

Scale Range : 0 pH to 14 pH

Resolution : 0.01 pH

Standard Normal (pH)	UUC Reading (pH)	Error (pH)	Uncertainty (pH)
0	0.00	0.00	0.006
1	1.00	0.00	0.006
2	2.00	0.00	0.006
3	3.00	0.00	0.006
4	4.00	0.00	0.006
5	5.00	0.00	0.006
6	6.00	0.00	0.006
7	7.00	0.00	0.006
8	8.00	0.00	0.006
9	9.00	0.00	0.006
10	10.00	0.00	0.006
11	11.00	0.00	0.006
12	12.00	0.00	0.006
13	13.00	0.00	0.006
14	14.00	0.00	0.006

... END ...



CERTIFICATE No : 25M2256
REFERENCE No : 76365-3

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE

MANUFACTURER : SARTORIUS

MODEL : BSA224S-CW

SERIAL No : 36591843

ID No : BA09/61

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.

CALIBRATION DATE : 07-Mar-25

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 13-Mar-25

RECEIVED DATE : 07-Mar-25

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.





CERTIFICATE No : 25M2256

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : BSA224S-CW
MANUFACTURER : SARTORIUS S/N : 36591843
ID No : BA09/61 RECEIVED DATE : 07-Mar-25
AIR PRESSURE : 1009mbar $\pm$ 1mbar CALIBRATION DATE : 07-Mar-25
AMBIENT TEMPERATURE : 24° C $\pm$ 1° C RELATIVE HUMIDITY : 52 %RH $\pm$ 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	C02250116	28-Jan-27
2) STANDARD WEIGHT	E2	15843	C02250117	29-Jan-27

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0.000071 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ($\pm$ g)
0.00	0.0000	0.0000	0.00012
0.10	0.1000	0.0000	0.00012
0.20	0.2000	0.0000	0.00012
0.50	0.5000	0.0000	0.00012
1.00	1.0000	0.0000	0.00012
2.00	2.0000	0.0000	0.00012
5.00	5.0000	0.0000	0.00012
10.00	10.0000	0.0000	0.00012
20.00	20.0001	-0.0001	0.00012
50.00	50.0000	0.0000	0.00014
100.00	100.0001	-0.0001	0.00019
200.00	200.0001	-0.0001	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	100.0000
2	100.0000
3	100.0000
4	100.0000
5	100.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





CERTIFICATE No : 26M2268

REFERENCE No : 80204-3

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE

MANUFACTURER : SARTORIUS

MODEL : BSA224S-CW

SERIAL No : 36591843

ID No : BA 09/61

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : SUCHAT S.

CALIBRATION DATE : 05-Mar-26

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 06-Mar-26

RECEIVED DATE : 05-Mar-26



CERT.No.: HS-W015C

Calibration Date : 18 Mar 25
 Submitted by : S.P.S CONSULTING SERVICE CO.,LTD
 7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol,
 Chatuchak, Bangkok, Thailand 10900

Avg Room Temp : 20 °C
 Avg Water Temp : 20 °C
 Air Pressure : 760.00 mmHg
 Salinity : 0 ppt

Model : YSI 5000
 S/N : 15B100751
 Probe : YSI 5010
 S/N : 22D100097
 ID NO. : -
 Air Temp ref : S/N. F8065C26
 Barometric ref : S/N. F8065C26
 Water Temp ref : -
 ID NO. HS001
 Technician : Kittipong M.

Calibration Details

Calibration Point	100% air sat. (@20 °C, DO = 9.09 mg/l)	(status)	(status)
Measurement 1 (mg/l)	9.08	(PASS)	-
Measurement 2 (mg/l)	9.08	(PASS)	-
Measurement 3 (mg/l)	9.08	(PASS)	-
Measurement 4 (mg/l)	9.07	(PASS)	-
Measurement 5 (mg/l)	9.07	(PASS)	-
Measurement 6 (mg/l)	9.07	(PASS)	-
Measurement 7 (mg/l)	9.07	(PASS)	-
Measurement 8 (mg/l)	9.07	(PASS)	-
Measurement 9 (mg/l)	9.07	(PASS)	-
Measurement 10 (mg/l)	9.07	(PASS)	-

Mean Measurement	9.07	mg/l	-	-
Inaccuracy	0.02	mg/l	-	-

Overall Status (PASS)

Manufacturer Specification

Accuracy = +/- 0.02 mg/l

- 1) This certificate is issued based on the result that are found as shown on date and place of test only.
- 2) The calibration procedure followed in accordance with Harikul Science Co., Ltd.
- 3) This result shall not be used for advertising purpose.



Technician Signature
 (Kittipong Maekwong)



Laboratory Manager
 (Natenapha Pisatkunchon)

CERT.No.: HS-X014C

Certificate of Calibration

Calibration Date : 16 March 2026

Submitted by : S.P.S CONSULTING SERVICE CO.,LTD

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol,

Chatuchak, Bangkok, Thailand 10900

Avg Room Temp : 20 °C

Avg Water Temp : 20 °C

Air Pressure : 760.00 mmHg

Salinity : 0 ppt

Model : YSI 5000

S/N : 15B100751

Probe : YSI 5010

S/N : 22D100097

ID NO. :

Air Temp ref : S/N. F8065C26

Barometric ref : S/N. F8065C26

Water Temp ref : -

ID NO. HS001

Technician : Kittipong M.

Calibration Details

Calibration Point	100% air sat. (@20 °C, DO = 9.09 mg/l)	(status)	(status)
Measurement 1 (mg/l)	9.09	(PASS)	-
Measurement 2 (mg/l)	9.09	(PASS)	-
Measurement 3 (mg/l)	9.09	(PASS)	-
Measurement 4 (mg/l)	9.09	(PASS)	-
Measurement 5 (mg/l)	9.09	(PASS)	-
Measurement 6 (mg/l)	9.08	(PASS)	-
Measurement 7 (mg/l)	9.08	(PASS)	-
Measurement 8 (mg/l)	9.08	(PASS)	-
Measurement 9 (mg/l)	9.08	(PASS)	-
Measurement 10 (mg/l)	9.08	(PASS)	-

Mean Measurement	9.09	mg/l	-	-
Inaccuracy	0.00	mg/l	-	-

Overall Status (PASS)

Manufacturer Specification

Accuracy = +/- 0.02 mg/l

- 1) This certificate is issued based on the result that are found as shown on date and place of test only.
- 2) The calibration procedure followed in accordance with Harikul Science Co., Ltd.
- 3) This result shall not be used for advertising purpose.



Technician Signature

(Kittipong Maekwong)



Laboratory Manager

(Natenapha Pisatkunchon)



QUALITY CALIBRATION CO., LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com

CERTIFICATE No : 25T0521

REFERENCE No : 75853-2

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : COD REACTOR

MANUFACTURER : HACH

MODEL : DRB 200

SERIAL No : 15110C0498

ID No : CRB 06/59

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : CHAICHARN CH.

CALIBRATION DATE : 03-Feb-25

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 03-Feb-25

RECEIVED DATE : 15-Jan-25





QUALITY CALIBRATION CO., LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 25T0521

PAGE : 2 OF 2

Calibration Report


EQUIPMENT : COD REACTOR
MANUFACTURER : HACH
ID NUMBER : CRB 06/59
RECEIVED DATE : 15-Jan-25
AMBIENT TEMPERATURE : 23° C ± 1° C
MODEL : DRB 200
SERIAL NUMBER : 15110C0498
CALIBRATION DATE : 03-Feb-25
RELATIVE HUMIDITY : 53 %RH ± 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT METHOD WITH CALIBRATED THERMOCOUPLE TYPE K UNDER NO LOAD CONDITION. THE THERMOCOUPLES WERE PLACED ON POINTS AND LOCATED AS THE PICTURE.
2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH TC TYPE K	HYDRA 2635A	7301307	24T6467	26-Jun-25
3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO., LTD.

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

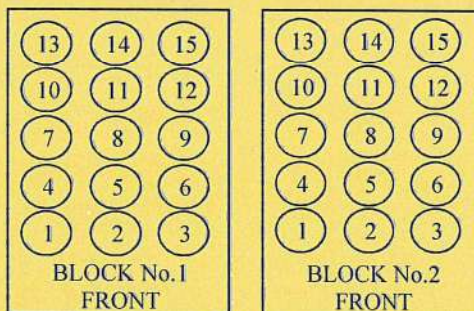

Block No.		1	2
Calibration Point (°C)		150	150
Controller temperature (°C)		145	145
Indicating Temperature		145	145
Measured Temperature (° C) at Spread Locations	1	150.23	150.64
	2	149.73	149.78
	3	150.29	150.29
	4	150.04	150.49
	5	150.09	150.51
	6	150.74	150.67
	7	149.97	150.66
	8	150.76	150.57
	9	150.54	150.51
	10	149.44	149.94
	11	150.12	150.64
	12	149.93	150.33
	13	149.19	149.82
	14	148.96	149.70
	15	149.09	149.79
Uncertainty of Measurement(± °C)		0.88	0.88

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2 : LOCATION 10 WAS REFERENCE LOCATION.

NOTE 3 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





CERTIFICATE No : 26T0464

REFERENCE No : 79659-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : COD REACTOR

MANUFACTURER : HACH

MODEL : DRB 200

SERIAL No : 15110C0497

ID No : DRB 04/59

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : SOMCHAI S.

CALIBRATION DATE : 30-Jan-26

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 30-Jan-26

RECEIVED DATE : 30-Jan-26





CERTIFICATE No : 26T0464

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : COD REACTOR
MANUFACTURER : HACH
ID NUMBER : DRB 04/59
RECEIVED DATE : 30-Jan-26
AMBIENT TEMPERATURE : 23° C ± 1° C

MODEL : DRB 200
SERIAL NUMBER : 15110C0497
CALIBRATION DATE : 30-Jan-26
RELATIVE HUMIDITY : 54 %RH ± 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT METHOD WITH CALIBRATED THERMOCOUPLE TYPE K UNDER NO LOAD CONDITION. THE THERMOCOUPLES WERE PLACED ON POINTS AND LOCATED AS THE PICTURE.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT

MODEL

SERIAL No

CERTIFICATE No

DUE DATE

1) DATA LOGGER WITH TC TYPE K

HYDRA 2635A

6849323

25T5342

18-Jun-26


3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO., LTD.

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

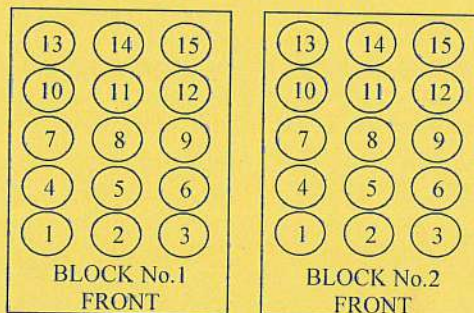

TEMPERATURE MEASUREMENT ACCURACY TEST

Block No.	1	2
Controller temperature (°C)	144	145
Indicating Temperature	144	145
Measured Temperature (°C) at Spread Locations	1	149.3
	2	149.1
	3	149.9
	4	149.6
	5	149.3
	6	149.5
	7	149.1
	8	149.7
	9	149.7
	10	149.5
	11	149.9
	12	149.4
	13	150.2
	14	149.4
	15	149.6
Uncertainty of Measurement(± °C)	0.89	0.89

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2 : LOCATION 10 WAS REFERENCE LOCATION.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k =2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





CERTIFICATE No : 26M2268

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE **MODEL** : BSA224S-CW
MANUFACTURER : SARTORIUS **S/N** : 36591843
ID No : BA 09/61 **RECEIVED DATE** : 05-Mar-26
AIR PRESSURE : 1004mbar $\pm$ 1mbar **CALIBRATION DATE** : 05-Mar-26
AMBIENT TEMPERATURE : 25° C $\pm$ 1° C **RELATIVE HUMIDITY** : 50 %RH $\pm$ 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

<u>INSTRUMENT</u>	<u>MODEL</u>	<u>SERIAL No</u>	<u>CERTIFICATE No</u>	<u>DUE DATE</u>
1) STANDARD WEIGHT SET	E2	QK-I-151	C02250116	28-Jan-27
2) STANDARD WEIGHT	E2	15843	C02250117	29-Jan-27

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0.000055 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ($\pm$ g)
0.0	0.0000	0.0000	0.00010
0.1	0.1000	0.0000	0.00011
0.2	0.2000	0.0000	0.00010
0.5	0.5000	0.0000	0.00011
1.0	1.0000	0.0000	0.00011
2.0	2.0000	0.0000	0.00011
5.0	5.0000	0.0000	0.00011
10.0	10.0000	0.0000	0.00011
20.0	20.0001	-0.0001	0.00011
50.0	50.0000	0.0000	0.00013
100.0	100.0001	-0.0001	0.00019
200.0	200.0001	-0.0001	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	100.0000
2	100.0000
3	100.0000
4	100.0000
5	100.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





MIRACLE INTERNATIONAL TECHNOLOGY CO.,LTD

214 Bangwaek Rd. Bangpai Bangkae Bangkok 10160
Tel.: 0-2865-4647-8 Fax: 0-2865-4649 <http://www.mit.in.th>



CALIBRATION CERTIFICATE

Page 1 of 2

Certificate No. : S2025070410-0003

Date Issued : 24-Jul-25

Customer : S.P.S. CONSULTING SERVICE CO., LTD.
7 Soi Phaholyothin 24 Phaholyothin Road., Jompol, Chatuchak,
Bangkok 10900

Equipment : Incubator

Manufacturer : BINDER

Model : BD 115

Serial No. : 12-16967

ID No./Tag No. : IN 05/56

Date Received : 22-Jul-25

Date Calibrated : 22-Jul-25

Calibrated by : Auttapol Kunaumpal

Calibration Method or Calibration Procedure Used

Standard method : CP-05 TLAS G-20.

This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

Result of Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level confidence approximately 95 percent.

This certificate may not be reproduced other than in full except with the prior written approval of the Miracle International Technology Company Limited.

Approved by:

K. Nathang
(Nathapong Krudaum)



Certificate No. : S2025070410-0003

Environment : Ambient Temperature : Start record 25.1 °C, Stop record 25.1 °C
Relative Humidity : Start record 48.9 %RH, Stop record 49.3 %RH

Calibration Temperature (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Stability ¹ (°C)	Measured Uniformity ² (°C)	Overall Variation ³ (°C)
35	35.0	35.0	0.13	0.37	0.57
41.5	41.5	41.5	0.10	0.35	0.49


Without adjustment

Calibration Temperature (°C)	STD No. 1 (°C)	STD No. 2 (°C)	STD No. 3 (°C)	STD No. 4 (°C)	STD No. 5 (°C)	STD No. 6 (°C)	STD No. 7 (°C)	STD No. 8 (°C)	STD No. 9 (°C)	Uncertainty ⁴ (±°C)
35	34.97	34.91	34.96	34.82	34.81	34.86	34.83	35.11	34.95	0.23
41.5	41.51	41.37	41.40	41.26	41.27	41.42	41.43	41.53	41.50	0.23

STD = Standard

Note : Probe No. 9 is Reference Probe

Setting Air Fresh No. OFF



Condition As-Received : Used Item

The measurement results and statements of conformity with specification only relate to the item calibrated.

Measurement Standards Used & Traceability :

The International System of Units (SI) through

MIT Certificate No. L202412300-0027 for Temperature Indicator with Sensor Serial No. US37020317, Due 09-Sep-25

Notes : 1. The temperature stability is the one-half of greatest maximum difference of measured temperatures at any one probe.

2. The temperature uniformity is the maximum difference of measured temperatures between of any probes and the measured temperature at the reference location which are observed at same time.

3. Overall variation is the difference of maximum and minimum measured temperatures throughout observation time.

4. The uncertainty of measurement is included temperature stability.

5. The temperature uniformity, stability, overall variation and indicating temperature is applicable to all air or gas filled temperature controlled enclosures at atmospheric pressure.

End of Certificate

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN
associates



Cert. No. : SP25026

Pages : 1 of 4

Calibration Certificate

Equipment : UV-VIS SPECTROPHOTOMETER
Manufacturer : PERKINELMER
Model : LAMBDA 25
Serial No.: 501S14123010
ID No.: SP03/58
Calibration Mode : WAVELENGTH ACCURACY
PHOTOMETRIC ACCURACY
STRAY LIGHT

Condition As Found : GOOD

Customer : S.P.S CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN ROAD,
CHOMPHON SUB-DISTRICT, CHATUCHAK DISTRICT,
BANGKOK PROVINCE 10900 THAILAND.

Location : ORGANIC LABORATORY IV

Ambient Temperature : (22.9 $\pm$ 5) °C
Relative Humidity : (53.7 $\pm$ 25) %

Received Date : 22 AUGUST 2025
Calibration Date : 22 AUGUST 2025
Date of Issue : 25 AUGUST 2025

Calibrated by :

Nitinun Srihawan

Approved by :

Wichok B.
(Wichok Ekpongpradit)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : SP25026

Job No. : VC68SP0019

Pages : 2 of 4

Calibration Method :

This instrument was calibrated by using on-site calibration procedure In-house method : CP-SP-01

The calibration procedure to direct measurement wavelength accuracy by using wavelength standard solution, Photometric accuracy by using absorbance standard filter and absorbance standard solution

The calibration procedure used was based on ASTM E275-01, ASTM E925-02

Condition of this result of calibration :

1. Certified reference materials

<u>Material</u>	<u>Ref. type</u>	<u>Cell serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Holmium liquid	RM-HL	29706	126461	24/10/2026
Didymium liquid	RM-DL	28912	126462	24/10/2026
Neutral density filter	RM-1N2N3N	13877	126457	24/10/2026
Potassium dichromate solutions	RM-0204060810	14204	126497	25/10/2026
Potassium Iodide solution	-	KI-0701-001	CI-0185-24	14/05/2026

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 The UK National Physical Laboratory (NPL)

Result of calibration : Wavelength Accuracy

(Without adjustment)

Material	Certified Values of Reference Material (nm)	UUC* Reading (nm)	Error (nm)	Uncertainty ± (nm)	k Factor
RM-HL	278.13	278.21	0.08	0.16	2.00
	361.25	361.39	0.14	0.16	2.00
	467.82	467.71	-0.11	0.16	2.00
	536.56	536.50	-0.06	0.16	2.00
	640.50	640.36	-0.14	0.16	2.00
RM-DL	740.09	739.85	-0.24	0.16	2.00
	864.94	865.12	0.18	0.16	2.00

UUC* = Unit Under Calibration

Cert. No. : SP25026
Job No. : VC68SP0019
Pages : 3 of 4

Result of calibration : Photometric Accuracy

Material	Wavelength (nm)	Filter S/N	Nominal Absorbance (A)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor
Neutral Density glass filter	440.0	29381	0.5	0.5443	0.5413	-0.0030	0.0043	2.00
		29914	0.7	0.7484	0.7455	-0.0029	0.0054	2.00
		29360	1.0	1.0527	1.0535	0.0008	0.0032	2.00
	465.0	29381	0.5	0.4948	0.4922	-0.0026	0.0041	2.00
		29914	0.7	0.6906	0.6877	-0.0029	0.0050	2.00
		29360	1.0	0.9695	0.9709	0.0014	0.0031	2.00
	546.1	29381	0.5	0.5090	0.5068	-0.0022	0.0036	2.00
		29914	0.7	0.6985	0.6960	-0.0025	0.0041	2.00
		29360	1.0	0.9814	0.9825	0.0011	0.0031	2.00
	590.0	29381	0.5	0.5375	0.5353	-0.0022	0.0034	2.00
		29914	0.7	0.7256	0.7231	-0.0025	0.0037	2.00
		29360	1.0	1.0213	1.0219	0.0006	0.0032	2.00
	635.0	29381	0.5	0.5223	0.5202	-0.0021	0.0033	2.00
		29914	0.7	0.6927	0.6901	-0.0026	0.0036	2.00
		29360	1.0	0.9744	0.9750	0.0006	0.0032	2.00

UUC* = Unit Under Calibration

Cert. No. : SP25026

Job No. : VC68SP0019

Pages : 4 of 4

Result of calibration : Photometric Accuracy

(Without adjustment)

Material	Wavelength (nm)	Solution (mg/l)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor
Potassium dichromate solutions	235.0	20	0.2415	0.2443	0.0028	0.0101	2.00
		40	0.4866	0.4871	0.0005	0.0115	2.00
		60	0.7415	0.7295	-0.0120	0.0067	2.00
		80	0.9854	0.9844	-0.0010	0.0071	2.00
		100	1.2444	1.2425	-0.0019	0.0073	2.00

UUC* = Unit Under Calibration

Condition of this result of calibration : Spectrophotometer PERKINELMER Model LAMBDA 25 S/N 501S14123010

Resolution of Wavelength Mode 0.1 nm

Resolution of Photometric Mode 0.001 A

Parameter Setting

Measurement Mode Wavelength, Absorbance

Wavelength Scan 190 nm - 1100 nm

Scanning Speed 7.5 nm/min

Band width(Wavelength) 1.0

Band width(Vis) 1.0

Band width(Uv) 1.0

Stray Light** UUC* Reading at 220.0 nm	
Transimission T(%)	Absorbance(A)
0.020	3.7032

**Specific Acceptance :

Transmission ≤ 1.0 T(%), Absorbance ≥ 2.0 A

**Stray light not TISI Accredited

The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95%

End of Calibration Certificate

PinAAcle 900T Preventive Maintenance Report

Company Name: S.P.S. Consulting Service Co.,Ltd.

Instrument Location: 7, 24 Soi Phaholyothin,

Ladyao, Khet, Bangkok 10900

Instrument Serial No.: PTCS14111103

Date: 18 Jun 2026

PinAAcle 900T Preventive Maintenance (PM)

Company Name:	S.P.S. Consulting Service Co.,Ltd.		
Address (Instrument Location):	7, 24 Soi Phaholyothin, Ladyao, Khet, Bangkok 10900		
Serial Number:	PTCS14111103	PM Number:	1 of 2
Customer Name (if applicable):	K. Phenpha	Telephone Number:	083-926-9252
Customer Support Engineer Name:	K. Chayanon	Service Order Number:	WO-11540403
Date PM Performed: (DD-MMM-YYYY)	18 Jun 2026	Next PM Due Date: (DD-MMM-YYYY)	18 Jun 2027
Standard Labor Hours to Complete PM :		5 hours	

Part Number	Release	Publication Date	
09370143 Rev.9	A	January 2018	

Scope

The purpose of this PM is to ensure the continued functionality of the PinAAcle 900T by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer.

The customer should save their method before the PM begins.

General Instructions:

The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM. Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files. The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer. Update the PM sticker and instrument logbook as required.

Copyright Information

This document contains proprietary information that is protected by copyright. All rights are reserved. No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of PerkinElmer, Inc. **Copyright © 2013 PerkinElmer, Inc.**

Trademarks

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners.

Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no Warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.

PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

Component List

Component / Specific Model	Serial #	Configuration Notes
PinAAcle900T	PTCS14111103	Winlab32
Fias100	100S14090404	Winlab32

Parts Lists

Parts Included with the PM		
Part Number (if applicable)	Description	Quantity
B0501696	Fan Filters	1
B3002013	THGA Contact Cylinders	1
B3141064	Glycerol for THGA Cooling	1
N3160156	O-Ring Kits for Sampling Introduction (Stainless Steels Nebulizer)	N/A
N3160157	O-Ring Kits for Sampling Introduction (Plastic Nebulizer)	2
N9301714	Replacement Acetylene Filter Cartridge	1
TH001022	Replacement Air Filter Cartridge	1

Additional Reagents and Standards Required for PM				
Part Number (if applicable)	Description	Quality	Batch/Lot #	Expired Date (MM/YY)
N9300183	1000 mg/L Copper Standard	AR	28-83CUY1	Nov 26
N9300244	GFAAS Mixed Standard	AR	60-004CRY1	Jun 26

Additional Reagents and Standards Required for PM (Customer Support Solution)				
Part Number (if applicable)	Description	Quantity	Batch/Lot #	Expiration Date (MM/YY)
N/A	DI Water	250 ml.	AR	AR
N/A	0.5% HNO ₃	250 ml.	AR	AR

Additional Tools Required for PM			
Part Number (if applicable)	Description	Quantity	Serial #
N1013000	0.2A Neutral density filter	1	101N0089015
N1013002	1.0A Neutral density filter	1	101N0089015
B3100652 Or N9307029	Electronic Flow Meter	1	NA
B0505495	Test Jig	1	NA
03030997	System 2 EDL Driver	1	030309-97E
N3050605	As System 2 EDL	1	000003-26798A
N3050121	Cu Lumina HCL	1	060419-030180
N3050109	Ba Lumina HCL	1	061219-020041
N3050139	K Lumina HCL	1	030819-010130
N3050152	Ni Lumina HCL	1	052719-020020
N3050119	Cr Lumina HCL	1	060419-030180

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. General:

- ✓ Review the instrument performance with the customer and document any recent problems.
- ✓ Inspect the customer log book and make any appropriate PM entries.
- ✓ Perform general inspection of system for cleanliness.

2. PC Instrument Software:

- ✓ Instrument Software user files/databases archived, packed, and/or deleted as needed.

3. Mechanical:

- ✓ Inspect and clean all fans and filters. Replace filters if necessary
- ✓ Inspect all gas and water lines for leaks and/or wear. Replace if needed. Thoroughly inspect all quick connects. Replace the Y connector, P/N 09921079, if needed.
- ✓ Clean exterior of the instrument.

3.1 Flame Technique

- ✓ Inspect the burner head, burner chamber, and nebulizer. Clean if needed as stated in the Hardware Guide.
- ✓ Check burner head dimensions with the feeler gauge as stated in the Hardware Guide in the Maintenance chapter section on cleaning the burner head and checking sloth width. Replace if out of specification
- ✓ Check the condition of the end cap, burner head, and nebulizer O-rings. Replace if necessary.
- ✓ Check the drain system for signs of wear. Replace worn or damaged parts.
- ✓ Visually check for proper flame conditions when igniting the Air-C₂H₂ and N₂O-C₂H₂ flames (if applicable).

3.2 THGA Technique

- ✓ Inspect the pole pieces and clean where the pole pieces contact the furnace. Replace the pole piece p-rings as needed, P/N's B0501018 & B0501250. Grease the O-rings as needed with Apiezon L grease, P/N 09905148
- ✓ Inspect the four insulation pads on the front contact housing of the THGA in furnace. If the pads are missing replace the THGA furnace or replace the insulator pads on the furnace.
- ✓ Inspect the graphite tube and clean the contact cylinders. Replace if necessary.
- ✓ Check internal and external gas flows with the Electronic Gas Flow Meter and the Gas Flow Test Probe as described in the Service Manual. Correct if necessary.
- ✓ Check furnace open/close function.
- ✓ Verify the operation of the GFTV Camera for proper operation and viewing alignment in the furnace camera Tube View window. Align if needed.
- ✓ Check the operation of the Halogen Light ASSY for the GFTV Camera. Replace if needed.
- ✓ Check the water level/quality in the recirculation (if applicable). Add distilled water if necessary.
- ✓ Check the cooling system fluid flow rate with the FCS In-Line Flow Meter for proper levels if needed. Refer to SDB# COSY008.STN

- ✓ Perform Cooling System maintenance if needed per SDB# COSY005.STN.
- ✓ Check auto sampler operation.
- ✓ Perform an auto sampler check valve test as described in the Service Manual.
- ✓ Lubricate the spindles of the auto sampler pumps and all moving parts of the tray mechanics as described in the Service Manual.
- ✓ Inspect the auto sampler sampling capillary as described in the Service Manual. Replace if necessary.

4. Electrical:

- ✓ Inspect PC boards. Clean if necessary.
- ✓ Carefully check all internal and external cable connections.
- ✓ Check instrument firmware revisions upgrade to current levels (if necessary)
- ✓ Run Diagnostics Test within the Advanced function of the Spectrometer page. Check the results in the service log folder in the Spectrometer BM Log Viewer.

5. Optics:

- ✓ Inspect and clean the sample compartment windows, if needed.
- ✓ Inspect and clean the furnace windows, if needed.
- ✓ Inspect and clean the GFTV camera lens, if needed.
- ✓ Inspect optics. Clean or replace if necessary,

6. Gasses:

- ✓ Verify that the Gasses supplied to the instrument are within the pressure and purity specifications found in the PinAAcle 900 Series Pre-installation Checklist SDB.
- ✓ Verify that the air filter element is dry. Replace if necessary.

7. Flame Interlock Check:

Description: Check to ensure that all safety interlocks are closed.

Parameter	Specification	Test Results	Pass/Fail
Flame Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
Drain Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
Nebulizer Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
C ₂ H ₂ Pressure Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
Air Pressure Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
Burner Head Sensor	Choosing Nitrous Oxide as the oxidant should trigger an interlock shuts down	Active	Passed

8. After PM Performance tests [Flame]:

8.1 Detector Linearity with Barium

Description: Ensures that the detector is linear in the Visible Range.

Parameter	Specification	Certificate Value at 553.6 nm (Abs.)	Test Results	Pass/Fail
1.0 A ND Filter	± 5% from Cert.	2.0405	1.9997	Passed
0.2 A ND Filter	± 5% from Cert.	0.1953	0.1855	Passed

8.2 Baseline Noise at 1.0 Absorbance with Barium

Description: Ensures that a high absorbance will not produce excessive noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.010	0.001	Passed

8.3 AA Baseline Noise with Copper

Description: Check baseline noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.001	0.0001	Passed

8.4 D₂ Background Compensation with Copper

Description: Verifies the instruments ability to compensate for Background absorption.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.010	0.0001	Passed

8.5 AA-BG Baseline Noise with Copper

Description: Ensures that background correction does not produce excessive noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.005	0.0003	Passed

8.6 AA-BG Baseline Noise with Arsenic

Description: Ensures that background correction does not produce excessive noise at a low wavelength.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.005	0.0001	Passed

8.7 Flame Sensitivity

Description: Instrument Sensitivity checked against Copper standard.

Standard Copper Sensitivity	Specification	Results (Abs.)	Pass/Fail
5 mg/L Sensitivity SS Neb (if applicable)	> 0.250 Abs.	NA	Not Applicable
2 mg/L Sensitivity HS Neb (if applicable)	> 0.250 Abs.	0.356	Passed

9. After PM Performance tests [THGA]:

9.1 Furnace Gas Flows

Description: Ensures the flow rates are within specification.

Parameter	Specification	Test Results	Pass/Fail
Internal Flow Rate	250 mL/min $\pm$ 25 mL/min	260	Passed
External Flow Rate	100 mL/min $\pm$ 10 mL/min	105	Passed

9.2 Chromium Baseline Noise

Description: Signal to noise check.

Parameter	Specification	Results	Pass/Fail
Baseline Noise	≤ 0.005 Abs.	0.0002	Passed
Standard Deviation	≤ 0.005	0.0001	Passed

9.3 Chromium Characteristic Mass and Precision

Description: Calculate the characteristic mass using the characteristic mass tool and precision from the integrated absorbance values.

Parameter	Specification	Results	Pass/Fail
Cr m_0 Results	≤ 7.0 pg/0.0044 A-s	5.4	Passed
Precision	≤ 2.0 %	0.14	Passed

9.4 Copper Characteristic Mass and Zeeman Ratio

Description: Calculate the characteristic mass using the characteristic mass tool and check the Zeeman Ratio.

Parameter	Specification	Results	Pass/Fail
Cu m ₀ Result	≤ 16.5 pg/0.0044 A-s	14.5	Passed
Zeeman Ratio	0.52 ± 0.04	0.54	Passed

10. Review:

- ☒ Review with the customer PM work performed.
- ☒ Review with the customer routine maintenance procedures.
- ☒ Discuss recommended customer supplied materials to have on hand.
- ☒ Attach PM sticker.

Additional Comments

Additional Comments Regarding the PM	
Zeeman Ratio	$= \frac{\text{Atomic Signal (Peak area)}}{\text{Atomic Signal (Peak area)} + \text{Background Signal (Peak area)}}$ $= \frac{0.1551}{0.1551 + 0.1315}$ $= 0.54$

Review

<i>The preventive maintenance checks and if applicable performance tests for PinAAcle 900T have been completed.</i>	
<i>This PinAAcle 900T Passes ☒ Fails ☐ the preventive maintenance.</i>	
Review of Preventive Maintenance:	
Authorized PerkinElmer Representative: Chayanan ✱	Date: 18 Jun 2026 (DD-MMM-YYYY)
Authorized Customer Representative: Chayanan ✱	Date: 18 Jun 2026 (DD-MMM-YYYY)

ลำดับที่ 6

คุณภาพน้ำใต้ดิน



ISOCAL TECHNOLOGY CO.,LTD.

Industrial Instrument Calibration Center

170/405 Moo 3 Serithai Rd., Kannayao Kannayao Bangkok 10230

Tel. 0-2906-3040-1 Fax. 0-2919-9948

Certificate of Calibration

Certificate Number : C25/0106B

Page : 1 of 3

Customer : S.P.S. Consulting Service Co.,Ltd.

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol,
Chatuchak, Bangkok 10900

Equipment Name : pH Meter
Model : HQ1110
Serial No. : 232651110029
ID No. : -
Manufacture : Hach
Environment : Ambient Temperature (23 ± 2) °C
: Relative Humidity (50 ± 15) %
Location of Calibration : In-Lab
Date of Received : 23-Jun-2025
Date of Calibration : 24-Jun-2025
Date of Issued : 27-Jun-2025
Condition as Received : Normal
Calibration Method : Calibration Procedure Number WI-10A-2

This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

This certificate shall not be reproduced other than in full except without the prior written approval of the Head of Calibration Laboratory of Isocal Technology Co.,Ltd.

Calibrated by : Miss Watchara Inchaidee

Technical

Approved by :

(Mr. Narong Phetjaroorn)



ISOCAL TECHNOLOGY CO.,LTD.

Calibration Report

Certificate Number : C25/0106B

Page : 2 of 3

Equipment Standards Used

Description	Serial No.	Certificate No.	Cal. Due Date
Multi Function Calibrator	2197	E2U2400315	15-Oct-25
pH Solution	1.09435.1000	HC32117435	31-Mar-26
pH Solution	1.09439.1000	HC33442639	30-Nov-26
pH Solution	1.09438.1000	HC20293938	31-Aug-25

Traceability :-

The calibration within the certificate are traceable through

: NIST - National Institute of Standard and Technology , U.S.A.

: PTB - Physikalisch-Technische Bundesanstalt , Germany

: NIMT - National Institute of Metrology, Thailand

to the International System of Units (SI).



ISOCAL TECHNOLOGY CO.,LTD.

Calibration Report

Certificate Number : C25/0106B

Page : 3 of 3

Result of Calibration : Adjustment (Yes)

Function : pH Measurement with Solution @ 25 °C

Scale Range : 4.01 pH to 10.01 pH

Resolution : 0.01 pH

Standard Value (pH)	UUC Reading (pH)	Error (pH)	Uncertainty (pH)
4.01	3.96	-0.05	0.012
7.01	7.03	0.02	0.012
10.01	9.97	-0.04	0.012

Function : pH Measurement

Scale Range : 0 pH to 14 pH

Resolution : 0.01 pH

Standard Normalinal (pH)	UUC Reading (pH)	Error (pH)	Uncertainty (pH)
0	0.00	0.00	0.006
1	1.00	0.00	0.006
2	2.00	0.00	0.006
3	3.00	0.00	0.006
4	4.00	0.00	0.006
5	5.00	0.00	0.006
6	6.00	0.00	0.006
7	7.00	0.00	0.006
8	8.00	0.00	0.006
9	9.00	0.00	0.006
10	10.00	0.00	0.006
11	11.00	0.00	0.006
12	12.00	0.00	0.006
13	13.00	0.00	0.006
14	14.00	0.00	0.006

... END ...

GC Clarus 600/680 Preventive Maintenance (PM)

Company Name:	S.P.S. Consulting Service Co.,Ltd		
Address (Instrument Location):	7 Soi Phaholyothin24 Phaholyothin Road, Jompol, Chatuchak, Bangkok, 10900.		
Serial Number:	680S14042502	Service Tag:	N68APSSFEMP
Customer Name (if applicable):	Ms.Naruecha	PM number:	1 of 2
Service Engineer Name:	Monchai Kitcharoenkeat	Service Order Number:	WO-11858723
Date PM Performed: (DD-MMM-YYYY)	13-Feb-2026	Next PM Due Date: (DD-MMM-YYYY)	13-Aug-2026

Part Number	Release	Publication Date	
TH09370070	C	August 2016	

Scope

The purpose of this PM is to ensure the continued functionality of the Clarus 600 and Clarus 680 GC by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer. The customer should save their method before the PM begins.

General Instructions:

The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM. Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files. The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer. Update the PM sticker and instrument logbook as required.

Copyright Information

This document contains proprietary information that is protected by copyright. All rights are reserved. No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of Perkin Elmer, Inc. **Copyright © 2013 PerkinElmer, Inc.**

Trademarks

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners. **Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no Warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.** PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

Component List

Component / Specific Model	Serial #	Software Version	Configuration Notes
Clarus680	680S14042502	Totalchrom6.3.2	PSS, PSS, FID,
Clarus SQ8T	648N4050804	Turbomass 6.4	
AtomX	US14113002	Tekma AtomX	

Parts Lists

Additional Tools Required for PM				
Part Number (if applicable)	Description	Quantity	Serial #	Calibration Due Date (MM/YY)
N/A				
Additional Reagents and Standards Required for PM				
Part Number (if applicable)	Description	Quantity	Batch/Lot #	Expiration Date (MM/YY)
N/A				

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. General:

- ☒ Review the instrument performance with the customer and document any recent problems.

- ☒ Check incoming AC line voltage for proper levels and grounding.

L-N 220 Volt

L-G 220 Volt

N-G 0.46 Volt

**Neutral to ground not more than 0.5 volts peak to peak*

- ☒ Inspect all gas line filters and traps; Replace if necessary with customer supplied spares.

Carrier gas ☒ Helium ☐ Nitrogen ☐ Hydrogen

Moisture level ☒ Good ☐ Need to replace ☐ Other _____

Detector gas ☒ Air Zero ☒ Hydrogen ☐ Nitrogen ☐ Helium

Moisture level ☒ Good ☐ Need to replace ☐ Other _____

- ☒ Inspect the customer log book and make any appropriate PM entries.

- ☒ Leak check all fittings from the gas source to instrument.

Gas leakage ☒ Pass ☐ Fail Comment _____

- ☒ Perform general inspection of system for cleanliness.

- ☒ Inspect for functional and clean electronic cooling and oven vent fans

Electronic cooling fan ☒ Yes ☐ No

Oven cooling fan ☒ Yes ☐ No

2. Electronic :

- ☒ Check oven temperature. Calibrate if necessary.

Oven temperature set point 150 °C ☒ Pass ☐ Fail

- ☐ Check sub-ambient option. (If installed).

Oven temperature set point 5 °C ☐ Pass ☐ Fail

- ☒ Perform routine maintenance on detector/injector. Replace parts as necessary with customer supplied spares.

- ☒ Check flows, including split flows if applicable. Calibrate if necessary.

Carrier flow	Pass
Split flow	Pass
- ☒ Check detector gas flows and adjust if necessary.

Detector flow	Pass
---------------	------
- ☒ Autosampler installed ☒ Yes ☐ No

Check autosampler sensor for wear and replace if necessary.	
Vial sensor	Pass
Door sensor	Pass
Tower sensor	Pass
Plunger sensor	Pass
Elevator sensor	Pass
- ☒ Remove syringe, manually flush. Replace with customer supplied spare if necessary.
- ☒ Check firmware version. Upgrade to current levels if necessary.

Firmware version	<u>6.5</u>
------------------	------------
- ☒ Measure all accessible power supply voltages.

5 Volt	Pass
+15 Volt	Pass
-15 Volt	Pass
24 Volt	Pass
- ☒ Record all detector voltage signal.

Detector Channel A	<u>0.87</u>	mV.
Detector Channel B	<u>NA</u>	mV.

3. Diagnostics Tests:

- ☒ Run instrument diagnostics.

☒ BRAM	Pass
☒ EPROM	Pass
- ☒ Run Autosampler diagnostics.

☒ BRAM	Pass
☒ EPROM	Pass

4. Review:

- ☒ Review with the customer PM work performed.
- ☒ Review with the customer routine maintenance procedures.
- ☒ Discuss recommended customer-supplied materials to have on hand
- ☒ Attach PM sticker.
- ☒ Update Logbook.

Additional Comments

Additional Comments Regarding the PM

Review

<i>The preventive maintenance checks and if applicable performance tests for Clarus600/680 GC have been completed.</i>	
<i>This Clarus600/680 GC Pass the preventive maintenance.</i>	
Review of Preventive Maintenance:	
Authorized PerkinElmer Representative: Monchai Kitcharoenkeat	Date: 13-Feb-2026 (DD-MMM-YYYY)
Authorized Customer Representative: Ms.Naruecha	Date: 13-Feb-2026 (DD-MMM-YYYY)

ลำดับที่ 7

ระดับเสียงในสถานที่ทำงาน



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-69/0204

MTC No. EEL. BP. 152/0169

CALIBRATION CERTIFICATE

Submitted by : S.P.S.CONSULTING SERVICE CO.,LTD.

Address : 7 Soi Phaholyothin 24, Phaholyothin Road, Jompol, Chatuchak, Bangkok 10900.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Sound Calibrator

Manufacturer : ACO

Model : 2127

Serial No. : 130006

Ambient Environment

Temperature : $(23 \pm 3) ^\circ\text{C}$

Relative Humidity : $(50 \pm 15) \%$

Ambient Pressure : $(101.325 \pm 1.500) \text{ kPa}$

- Standards used :**
1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.
 2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.
 3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.
 4. Digital Multimeter Agilent 34401A S/N MY44005560.
 5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.
 6. Audio Analyzer Keithley 2015-P S/N 4106495.
 7. Condenser Microphone Bruel&Kjaer 4180 S/N 2889871.

Calibration Procedure: CP-102-04 based on IEC 60942-2003; The sound pressure level generated by sound calibrator under test shall be measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 29 Jan. 2026

Date of Calibration : 11 Feb. 2026

1 / 2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory

668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office

196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-69/0204

MTC No. EEL. BP. 152/0169

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20 μ Pa at 1000 Hz

Acoustic Output in dB re 20 μ Pa, Corrected to Reference Conditions: 101.325 kPa, 23.0 °C and 50 %RH.

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	93.89	-0.11	± 0.10	± 0.40 dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	999.9	-0.1	± 1.5	$\pm 1.0\%$

3. Total Distortion

Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	1.90	± 0.50	$\pm 3.0\%$

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Calibrated by :


(Mr. Weerachai Deechaiyae)

Approved by :


(Mr. Prawate Kluaypa)
Director

Date of Calibration : 11 Feb. 2026

Date of Issue : 12 Feb. 2026

Electrical and Electronic Standards Laboratory
Industrial Metrology and Testing Service Centre

Ref : 2011269012900497001

End of Certificate

2 / 2

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, .
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory

668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office

196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Noise R_236/26

Sound Level Meter Calibration Report

Acoustic Calibrator Data

Brand	ACO	Number	AC 03/56
Model	2127	Serial No.	130006
Calibration Range	94 dB, 1000 Hz	Last Calibration	11 February 2026
		Due Date	11 February 2027

Calibration Data

Sound Level Meter Data

Calibration Data

SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-R40	ACO	6236	00192052	29 April 2026	93.8	93.9
ACO-R41	ACO	6236	00192053	29 April 2026	93.9	93.9
ACO-R50	ACO	6236	00192062	29 April 2026	93.9	93.9
ACO-R51	ACO	6236	00192063	29 April 2026	93.8	93.9

Acoustic Certified Value : Thailand Institute of Scientific and Technological Research
(TISTR)

93.89 ± 0.10 dB

Calibrated by :

Heeson L.
(Mr. Heeson Lormae)

Approved by :

Yutthana J.
(Mr. Yutthana Tanatharanit)