

เอกสารสอบเทียบความถูกต้องของเครื่องมือตรวจวัดคุณภาพสิ่งแวดล้อม

- | | |
|------------|--|
| ลำดับที่ 1 | คุณภาพอากาศในบรรยากาศ |
| ลำดับที่ 2 | คุณภาพอากาศจากปล่องระบาย |
| ลำดับที่ 3 | ระดับเสียงในบรรยากาศโดยทั่วไป |
| ลำดับที่ 4 | คุณภาพน้ำทิ้ง |
| ลำดับที่ 5 | คุณภาพอากาศในสถานประกอบการ |
| ลำดับที่ 6 | ระดับเสียงในสถานประกอบการ |
| ลำดับที่ 7 | ระดับเสียงที่ลูกจ้างได้รับเฉลี่ยตลอดระยะเวลาในแต่ละวัน |
| ลำดับที่ 8 | ระดับความร้อนในสถานประกอบการ |

**ตารางสรุปรายการเอกสารการสอบเทียบความถูกต้องของเครื่องมือเก็บตัวอย่าง
และเครื่องมือตรวจวิเคราะห์คุณภาพสิ่งแวดล้อม**

รายการตรวจวัด	เครื่องมือเก็บตัวอย่าง	เครื่องมือตรวจวิเคราะห์
	ชื่อเครื่องมือ	ชื่อเครื่องมือ
1. คุณภาพอากาศในบรรยากาศ		
TSP	High Volume Air Sampler Rec No. Blower No. R04, R05, R12	Digital Balance
PM ₁₀	High Volume Air Sampler Rec No. Blower No. R06, R12, R13	Digital Balance
PM _{2.5}	High Volume Air Sampler Rec No. Blower No. B08, B09, B10	Digital Balance
NO _x	NO _x Analyzer No. B02, R07, R10	NO _x Analyzer No. B02, B17, R04
2. คุณภาพอากาศจากปล่อง		
Total Suspended Particulate	Console No. R04 Pitot Tube No. B44	Digital Balance
PM ₁₀	Console No. R04 Pitot Tube No. B44	Digital Balance
Oxides of Nitrogen	Vacuum Gauge	Spectrophotometer
Fume Al	Console No. R04 Pitot Tube No. B44	ICP
Hydrogen Fluoride	Console No. R04 Pitot Tube No. B44	IC
Hydrogen Chloride	Console No. R04 Pitot Tube No. B44	IC
Dioxins	Console No. R04 Pitot Tube No. B44	GC/MS
3. คุณภาพน้ำ		
pH	-	pH Meter
Total Suspended Solids	-	Digital Balance
Total Dissolved Solids	-	Digital Balance
BOD ₅	-	BOD Analyzer
COD	-	COD Reactor
Grease & Oil	-	Digital Balance
Aluminium	-	Spectrophotometer

รายการตรวจวัด	เครื่องมือเก็บตัวอย่าง	เครื่องมือตรวจวิเคราะห์
	ชื่อเครื่องมือ	ชื่อเครื่องมือ
4. ระดับเสียงในบรรยากาศ L_{eq} 24 hrs., L_{max} , L_{90} , L_{dn} , เสียงรบกวน	Acoustic Calibrator Sound Level Meter ST-C1-B06, B07, CR-B09, B10	-
5. คุณภาพอากาศในสถานประกอบการ Total Dust	- Personal Pump SKC No. R43, B26, R44, R34 - Rotameter No. H-R02	- Digital Balance
Respirable Dust	- Personal Pump SKC No. R22, R15, R34, R44 R22 - Rotameter No. H-R02	- Digital Balance
6. ระดับเสียงในสถานประกอบการ L_{eq} 24 hr และ TWA	Acoustic Calibrator Sound Level Meter ACO-R41, R50, R51, R52	-
7. ระดับเสียงที่ลูกจ้างได้รับเฉลี่ยตลอดระยะเวลาในแต่ละวัน Noise Dose	Acoustic Calibrator Sound Level Meter SV-B14, B15, B16	-
8. ระดับความร้อนในสถานประกอบการ WBGT	Digital Thermometer Heat Stress WBGT Mater No. R04, R05	-

ลำดับที่ 1

คุณภาพอากาศในบรรยากาศ



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

High Volume Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard

Model : TE 5025A

S/N : 3611

Calibration Data

High Volume Air Sampler Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (ft ³ /min)	R ²
B01	B01	02/02/2026	$y = 1.147x - 3.983$	0.998
B02	B02	02/02/2026	$y = 1.158x - 3.531$	0.997
B03	B03	02/02/2026	$y = 1.109x - 2.595$	0.999
B04	B04	02/02/2026	$y = 1.123x - 1.928$	0.998
B05	B05	02/02/2026	$y = 1.145x - 3.659$	0.999
B06	B06	02/02/2026	$y = 1.100x - 2.379$	0.999
B07	B07	02/02/2026	$y = 1.122x - 2.377$	0.999
B08	B08	02/02/2026	$y = 1.102x - 2.500$	0.998
B09	B09	02/02/2026	$y = 1.121x - 3.479$	0.999
B10	B10	02/02/2026	$y = 1.143x - 3.199$	0.996
B11	B11	03/02/2026	$y = 1.105x - 1.251$	0.999
B12	B12	03/02/2026	$y = 1.136x - 3.106$	0.996
B13	B13	03/02/2026	$y = 1.142x - 2.536$	0.998
B14	B14	03/02/2026	$y = 1.135x - 3.133$	0.998
B15	B15	03/02/2026	$y = 1.111x - 2.932$	0.998
B16	B16	04/02/2026	$y = 1.104x - 3.794$	0.998
B17	B17	04/02/2026	$y = 1.151x - 2.773$	0.998
B18	B18	04/02/2026	$y = 1.140x - 2.730$	0.998
B19	B19	04/02/2026	$y = 1.137x - 2.624$	0.998
B20	B20	04/02/2026	$y = 1.139x - 1.402$	0.998
B21	B21	04/02/2026	$y = 1.131x - 1.657$	0.999
B22	B22	04/02/2026	$y = 1.166x - 3.887$	0.997
B23	B23	04/02/2026	$y = 1.162x - 4.278$	0.998
B24	B24	04/02/2026	$y = 1.128x - 2.436$	0.998
B25	B25	04/02/2026	$Y = 1.159x - 4.833$	0.998
B26	B26	03/02/2026	$y = 1.103x - 1.969$	0.997
B27	B27	04/02/2026	$y = 1.149x - 3.761$	0.997
B28	B28	04/02/2026	$y = 1.134x - 3.377$	0.999
B29	B29	04/02/2026	$y = 1.118x - 2.903$	0.997
B30	B30	04/02/2026	$y = 1.157x - 2.504$	0.999
B31	B31	04/02/2026	$y = 1.165x - 3.108$	0.999
B32	B32	04/02/2026	$y = 1.113x - 2.480$	0.999
B33	B33	04/02/2026	$y = 1.155x - 2.774$	0.997
B34	B34	04/02/2026	$y = 1.125x - 1.905$	0.997

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :


(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

High Volume Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard

Model : TE 5025A

S/N : 3611

Calibration Data

High Volume Air Sampler Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (ft ³ /min)	R ²
B35	B35	04/02/2026	$y = 1.154x - 3.696$	0.996
B36	B36	04/02/2026	$y = 1.119x - 2.463$	0.997
B37	B37	04/02/2026	$y = 1.129x - 3.721$	0.998
B38	B38	02/02/2026	$y = 1.182x - 2.931$	0.997
B39	B39	02/02/2026	$y = 1.062x - 1.512$	0.999
B40	B40	02/02/2026	$y = 1.163x - 3.556$	0.997
B41	B41	02/02/2026	$y = 1.116x - 1.975$	0.996
B42	B42	02/02/2026	$y = 1.152x - 4.140$	0.997
B43	B43	02/02/2026	$y = 1.167x - 3.646$	0.996
B44	B44	02/02/2026	$y = 1.178x - 4.362$	0.999
R01	R01	02/02/2026	$y = 1.097x - 2.630$	0.997
R02	R02	02/02/2026	$y = 1.138x - 3.218$	0.996
R03	R03	02/02/2026	$y = 1.133x - 3.084$	0.998
R04	R04	02/02/2026	$y = 1.121x - 2.102$	0.998
R05	R05	02/02/2026	$y = 1.041x + 0.894$	0.997
R06	R06	02/02/2026	$y = 1.075x + 0.254$	0.997
R07	R07	03/02/2026	$y = 1.126x - 2.841$	0.996
R08	R08	03/02/2026	$y = 1.091x - 2.104$	0.996
R09	R09	03/02/2026	$y = 1.065x + 0.557$	0.996
R10	R10	03/02/2026	$y = 1.093x - 1.217$	0.999
R11	R11	03/02/2026	$y = 1.130x - 3.938$	0.999
R12	R12	05/02/2026	$y = 1.164x - 2.698$	0.997
R13	R13	05/02/2026	$y = 1.120x - 3.336$	0.998
R14	R14	05/02/2026	$y = 1.034x + 0.445$	0.997
R15	R15	05/02/2026	$y = 1.076x + 0.429$	0.998
R16	R16	05/02/2026	$y = 1.107x - 1.468$	0.996
R17	R17	05/02/2026	$y = 1.078x - 1.668$	0.998
R18	R18	05/02/2026	$y = 1.160x - 5.001$	0.997
R19	R19	05/02/2026	$y = 1.077x - 2.680$	0.997
R20	R20	05/02/2026	$y = 1.185x - 4.839$	0.998

Calibrated by :


(Mr. Abdul Dangklom)

Approved by :


(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

High Volume PM-10 Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard

Model : TE 5025A

S/N : 3611

Calibration Data

High Volume PM-10 Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (ft ³ /min)	R ²
R01	R01	04/02/2026	$y = 1.057x + 0.776$	0.998
R02	R02	04/02/2026	$y = 1.126x - 3.479$	0.999
R03	R03	04/02/2026	$y = 1.099x - 1.897$	0.996
R04	R04	04/02/2026	$y = 1.130x - 3.885$	0.998
R05	R05	04/02/2026	$y = 1.082x - 2.165$	0.999
R06	R06	04/02/2026	$y = 1.132x - 2.551$	0.997
R07	R07	04/02/2026	$y = 1.116x - 2.326$	0.998
R08	R08	02/02/2026	$y = 1.133x - 2.404$	0.998
R09	R09	02/02/2026	$y = 1.063x + 0.125$	0.998
R10	R10	02/02/2026	$y = 1.119x - 2.628$	0.997
R11	R11	02/02/2026	$y = 1.030x + 1.723$	0.999
R12	R12	02/02/2026	$y = 1.035x + 0.921$	0.999
R13	R13	02/02/2026	$y = 1.117x - 3.172$	0.999
R14	R14	02/02/2026	$y = 1.083x - 2.455$	0.999
R15	R15	02/02/2026	$y = 1.103x - 3.395$	0.997
R16	R16	02/02/2026	$y = 1.146x - 4.022$	0.998
R17	R17	02/02/2026	$y = 1.091x - 1.835$	0.998
R18	R18	02/02/2026	$y = 1.104x - 4.944$	0.998
R19	R19	03/02/2026	$y = 1.097x + 0.011$	0.996
R20	R20	03/02/2026	$y = 1.107x - 2.872$	0.998

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

Peera Detudom
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 21 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 21, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel: (662) 939-4370 (Automatic 5 Lines) Fax: (662) 513-4221 E-mail: sale@spscon.com

CALIBRATION REPORT			
PM2.5 AIR SAMPLER (VERY SHARP CUT CYCLONE-VSCC)			
DATE :	19 February 2026	BRAND :	BGI
NO.	PM2.5-08	MODEL :	PQ200
		SERIAL NO.	159904 (VSCC)
CALIBRATING CONDITION			
Pressure	1010	mmbar	Temp. 24.6 °C
		% RH	49
Calibration Method : Dry Cal Primary		Model : Defender 510 H	S/N : 136164
CALIBRATION SETTING			
detaCal	PM2.5 AIR SAMPLER		
Flowrate Reading,L/min	Initial Flowrate Reading (Before Adj.),L/min	%Dif.	Final Flowrate Reading (After Adj.),L/min
16.70	16.67	0.180	16.70

Calibrated by : Heeson L.
(Mr.Heeson Lormae)

Approved by : Yutthana S.
(Mr.Yutthana Tanatharanit)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
 7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
 7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
 Tel: (662) 939-4370 (Automatic 5 Lines) Fax: (662) 513-4221 E-mail: sale@spscon.com

CALIBRATION REPORT			
PM2.5 AIR SAMPLER (VERY SHARP CUT CYCLONE-VSCC)			
DATE :	19 February 2026	BRAND :	BGI
NO.	PM2.5-09	MODEL :	PQ200
		SERIAL NO.	152125 (VSCC)
CALIBRATING CONDITION			
Pressure	1010	mmbar	
Temp.	24.6	°C	% RH
			49
Calibration Method : Dry Cal Primary		Model : Defender 510 H	S/N : 136164
CALIBRATION SETTING			
detaCal	PM2.5 AIR SAMPLER		
Flowrate Reading, L/min	Initial Flowrate Reading (Before Adj.), L/min	% Dif.	Final Flowrate Reading (After Adj.), L/min
16.70	16.66	0.240	16.70

Calibrated by :

Heeson L.

(Mr. Heeson Lormae)

Approved by :

Yutthana S.

(Mr. Yutthana Tanatharañit)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel: (662) 939-4370 (Automatic 5 Lines) Fax: (662) 513-4221 E-mail: sale@spscon.com

CALIBRATION REPORT			
PM2.5 AIR SAMPLER (VERY SHARP CUT CYCLONE-VSCC)			
DATE :	19 February 2026	BRAND :	BGI
		MODEL :	PQ200
NO.	PM2.5-10	SERIAL NO.	164598 (VSCC)
CALIBRATING CONDITION			
Pressure	1010	mmbar	Temp. 24.6 °C
		% RH	49
Calibration Method : Dry Cal Primary		Model : Defender 510 H	S/N : 136164
CALIBRATION SETTING			
detaCal	PM2.5 AIR SAMPLER		
Flowrate Reading,L/min	Initial Flowrate Reading (Before Adj.),L/min	%Dif.	Final Flowrate Reading (After Adj.),L/min
16.70	16.67	0.180	16.70

Calibrated by : Heeson L.
(Mr.Heeson Lormae)

Approved by : Yutthana S.
(Mr.Yutthana Tanatharanit)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscn.com, www.spscn.com

CALIBRATION REPORT					
CHEMILUMINESCENT NO / NO ₂ / NO _x ANALYZER					
DATE :	19 February 2026	BRAND :	API	MODEL :	200E
NO.	NOX-R02	SERIAL NO.	2285		
Calibrator (Dilution System)					
Brand	: Teledyne		Model	: 700	
Last Cal. Date	: 24 October 2025		Serial No.	: 421	
Reference Standard Gas					
Standard Gas	: Nitric Oxide (NO)		Cylinder No.	: A00674SV	
Certified Date	: 12 March 2025		Expired Date	: 12 March 2028	
			Cylinder Conc.	: 48.7 ppm	
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.6	°C
			% RH	48	
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.), PPB			Final Reading (After Adj.), PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	-0.10	-	0	-
NO Span	400	399.8	-0.050	400.0	1.004
NO _x Span	400	400.2	0.050	400.0	1.005
API Model 200E NO _x Analyzer Check List					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	500 standard		
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air		
SAMPLE FLOW	508	cc/min	500 ± 50		
OZONE FLOW	79	cc/min	80 ± 15		
PMT	103.6	mV	-20 - 150		
AZERO	94.3	mV	-20 - 150		
HVPS	671	V	420 - 900 constant		
RCELL TEMP	50.0	°C	50 ± 1		
BOX TEMP	28.8	°C	8 - 48		
PMT TEMP	7.1	°C	7 ± 2		
MOLY TEMP	315.6	°C	315 ± 5		
RCELL PRESS	8.4	IN-Hg-A	2 - 10 constant		
SAMPLE PRESS	28.5	IN-Hg-A	25 - 30 constant		
NO Span Conc	400	PPB	20 - 20,000		
NO _x Span Conc	400	PPB	20 - 20,000		
NO Slope	1.004	-	1.0 ± 0.3		
NO _x Slope	1.005	-	1.0 ± 0.3		
NO Offset	0.8	mV	-20 to +150		
NO _x Offset	0.4	mV	-20 to 150		
Stability at Zero	0.1	PPB	< 0.2		
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas		

Calibrated by :

Heeson L.
(Mr. Heeson Lormae)

Approved by :

Yutthana S.
(Mr. Yutthana Tanathananit)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT

CHEMILUMINESCENT NO / NO₂ / NO_x ANALYZER

DATE : 19 February 2026

BRAND : API

MODEL : 200E

NO. NOX-R07

SERIAL NO. 4468

Calibrator (Dilution System)

Brand : Teledyne

Model : 700

Last Cal. Date : 24 October 2025

Serial No. : 421

Reference Standard Gas

Standard Gas : Nitric Oxide (NO)

Cylinder No. : A00674SV

Certified Date : 12 March 2025

Expired Date : 12 March 2028

Cylinder Conc. : 48.7 ppm

CALIBRATING CONDITION

Pressure 1011 mmbar

Temp. 24.6 °C

% RH 48

CALIBRATION SETTING

Span	Initial Reading (Before Adj.), PPB			Final Reading (After Adj.), PPB	
	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	-0.10	-	0	-
NO Span	400	400.1	0.025	400.0	1.003
NO _x Span	400	400.3	0.075	400.0	1.004

API Model 200E NO_x Analyzer Check List

Test Values	Observed Value	Units	Nominal Range
RANGE	500	PPB	500 standard
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air
SAMPLE FLOW	507	cc/min	500 ± 50
OZONE FLOW	77	cc/min	80 ± 15
PMT	103.4	mV	-20 - 150
AZERO	94.5	mV	-20 - 150
HVPS	674	V	420 - 900 constant
RCELL TEMP	50.0	°C	50 ± 1
BOX TEMP	29.5	°C	8 - 48
PMT TEMP	7.2	°C	7 ± 2
MOLY TEMP	315.4	°C	315 ± 5
RCELL PRESS	8.2	IN-Hg-A	2 - 10 constant
SAMPLE PRESS	28.4	IN-Hg-A	25 - 30 constant
NO Span Conc	400	PPB	20 - 20,000
NO _x Span Conc	400	PPB	20 - 20,000
NO Slope	1.003	-	1.0 ± 0.3
NO _x Slope	1.004	-	1.0 ± 0.3
NO Offset	0.9	mV	-20 to +150
NO _x Offset	0.5	mV	-20 to 150
Stability at Zero	0.1	PPB	< 0.2
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas

Calibrated by :

Heeson L.

(Mr.Heeson Lormae)

Approved by :

Yutthana S.

(Mr.Yutthana Tanatharanit)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jomjot, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT

CHEMILUMINESCENT NO / NO₂ / NO_x ANALYZER

DATE : 19 February 2026

BRAND : API

MODEL : 200E

NO. NOX-R10

SERIAL NO. 1991

Calibrator (Dilution System)

Brand : Teledyne

Model : 700

Last Cal. Date : 24 October 2025

Serial No. : 421

Reference Standard Gas

Standard Gas : Nitric Oxide (NO)

Cylinder No. : A006745V

Certified Date : 12 March 2025

Expired Date : 12 March 2028

Cylinder Conc. : 48.7 ppm

CALIBRATING CONDITION

Pressure 1011 mmbar

Temp. 24.5 °C

% RH 48

CALIBRATION SETTING

Span	Initial Reading (Before Adj.), PPB			Final Reading (After Adj.), PPB	
	Expected Concentration	Analyzer Response	% Dif	Analyzer Response	Slope
Zero	0	0.10	-	0	-
NO Span	400	399.7	-0.075	400.0	1.002
NO _x Span	400	400.2	0.050	400.0	1.003

API Model 200E NO_x Analyzer Check List

Test Values	Observed Value	Units	Nominal Range
RANGE	500	PPB	500 standard
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air
SAMPLE FLOW	502	cc/min	500 ± 50
OZONE FLOW	79	cc/min	80 ± 15
PMT	103.4	mV	-20 - 150
AZERO	93.8	mV	-20 - 150
HVPS	672	V	420 - 900 constant
RCELL TEMP	50.5	°C	50 ± 1
BOX TEMP	29.4	°C	8 - 48
PMT TEMP	7.0	°C	7 ± 2
MOLY TEMP	315.5	°C	315 ± 5
RCELL PRESS	8.5	IN-Hg-A	2 - 10 constant
SAMPLE PRESS	28.5	IN-Hg-A	25 - 30 constant
NO Span Conc	400	PPB	20 - 20,000
NO _x Span Conc	400	PPB	20 - 20,000
NO Slope	1.002	-	1.0 ± 0.3
NO _x Slope	1.003	-	1.0 ± 0.3
NO Offset	0.9	mV	-20 to +150
NO _x Offset	0.5	mV	-20 to 150
Stability at Zero	0.1	PPB	< 0.2
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas

Calibrated by :

Heeson L.

(Mr. Heeson Lormae)

Approved by :

Yutthana J.

(Mr. Yutthana Tanathanit)



CERTIFICATE No : 25M2254

REFERENCE No : 76365-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE

MANUFACTURER : METTLER TOLEDO

MODEL : XS105DU

SERIAL No : 1126422905

ID No : BA05/50

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.

CALIBRATION DATE : 07-Mar-25

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 13-Mar-25

RECEIVED DATE : 07-Mar-25

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.





CERTIFICATE No : 25M2254

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : XS105DU
MANUFACTURER : METTLER TOLEDO S/N : 1126422905
ID No : BA05/50 RECEIVED DATE : 07-Mar-25
AIR PRESSURE : 1009mbar $\pm$ 1mbar CALIBRATION DATE : 07-Mar-25
AMBIENT TEMPERATURE : 24°C $\pm$ 1°C RELATIVE HUMIDITY : 54 %RH $\pm$ 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	C02250116	28-Jan-27
2) STANDARD WEIGHT	E2	15843	C02250117	29-Jan-27

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 120 g WAS 0.000055 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ($\pm$ g)
0.00	0.00000	0.00000	0.000065
0.02	0.01999	0.00001	0.000065
0.10	0.10001	-0.00001	0.000066
0.20	0.20001	-0.00001	0.000066
0.50	0.50002	-0.00002	0.000065
1.00	1.00003	-0.00003	0.000066
2.00	2.00001	-0.00001	0.000067
5.00	5.00002	-0.00002	0.000068
10.00	10.00000	0.00000	0.000070
20.00	20.00004	-0.00004	0.000078
50.00	50.00000	0.00000	0.00013
100.00	100.0001	-0.0001	0.00019
120.00	120.0002	-0.0002	0.00022

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.0000
2	50.0000
3	50.0000
4	50.0000
5	50.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



ลำดับที่ 2

คุณภาพอากาศจากปล่องระบาย



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Console Calibration Report

Calibration Method

Critical Orifices

Calibration Data

Console Data		Calibration Data		
No.	Serial No.	Date	y	ΔH_{g} (mmH ₂ O)
B01	1563	02/03/2026	0.998	49.85
B02	8002514	02/03/2026	1.003	49.77
B03	1503016	03/03/2026	0.997	49.68
B04	00006659	03/03/2026	0.996	49.82
B05	00007428	02/03/2026	0.999	49.65
R01	1561	03/03/2026	1.002	49.98
R02	8002513	03/03/2026	1.004	49.56
R03	1570	03/03/2026	0.997	49.73
R04	8002519	03/03/2026	0.999	49.80
R05	1503015	02/03/2026	1.003	49.95

Remark : Accept Value of y (test) is $0.97 < y < 1.03$
Accept Value of ΔH_{g} (test) is 46.7 ± 6.4 (mmH₂O)

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

Peera Detudom
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Pitot Tube Calibration Report

Calibration Method

Standard Pitot Tube

Calibration Data					
Pitot Tube Data			Calibration Data		
No.	Type of Pitot	Coefficient of Standard Pitot	Date	Avg. of Cp (test)	
				Side A	Side B
B36	S	0.99	05/05/2026	0.84	0.84
B37	S	0.99	03/05/2026	0.84	0.85
B38	S	0.99	03/05/2026	0.84	0.84
B39	S	0.99	06/05/2026	0.84	0.85
B40	S	0.99	06/05/2026	0.85	0.84
B41	S	0.99	05/05/2026	0.84	0.85
B44	S	0.99	06/05/2026	0.84	0.83
B45	S	0.99	05/05/2026	0.84	0.84
B46	S	0.99	05/05/2026	0.84	0.85
B47	S	0.99	03/05/2026	0.84	0.84
B48	S	0.99	03/05/2026	0.85	0.84
B49	S	0.99	03/05/2026	0.84	0.84
B54	S	0.99	05/05/2026	0.85	0.84
B56	S	0.99	03/05/2026	0.84	0.84
B57	S	0.99	05/05/2026	0.84	0.84
B58	S	0.99	03/05/2026	0.84	0.84

Remark : Accept value of Cp (test) is 0.84 ± 0.01

Calibrated by : <u>Adul Dangklom</u> (Mr. Adul Dangklom)	Approved by : <u>(Signature)</u> (Mr. Peera Detudom)
---	---



CERTIFICATE No : 25M2254

REFERENCE No : 76365-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE

MANUFACTURER : METTLER TOLEDO

MODEL : XS105DU

SERIAL No : 1126422905

ID No : BA05/50

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.

CALIBRATION DATE : 07-Mar-25

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 13-Mar-25

RECEIVED DATE : 07-Mar-25

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.





CERTIFICATE No : 25M2254

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : XS105DU
MANUFACTURER : METTLER TOLEDO S/N : 1126422905
ID No : BA05/50 RECEIVED DATE : 07-Mar-25
AIR PRESSURE : 1009mbar $\pm$ 1mbar CALIBRATION DATE : 07-Mar-25
AMBIENT TEMPERATURE : 24°C $\pm$ 1°C RELATIVE HUMIDITY : 54 %RH $\pm$ 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	C02250116	28-Jan-27
2) STANDARD WEIGHT	E2	15843	C02250117	29-Jan-27

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 120 g WAS 0.000055 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ($\pm$ g)
0.00	0.00000	0.00000	0.000065
0.02	0.01999	0.00001	0.000065
0.10	0.10001	-0.00001	0.000066
0.20	0.20001	-0.00001	0.000066
0.50	0.50002	-0.00002	0.000065
1.00	1.00003	-0.00003	0.000066
2.00	2.00001	-0.00001	0.000067
5.00	5.00002	-0.00002	0.000068
10.00	10.00000	0.00000	0.000070
20.00	20.00004	-0.00004	0.000078
50.00	50.00000	0.00000	0.00013
100.00	100.0001	-0.0001	0.00019
120.00	120.0002	-0.0002	0.00022

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.0000
2	50.0000
3	50.0000
4	50.0000
5	50.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





CERTIFICATE No : 26M2266

REFERENCE No : 80204-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE

MANUFACTURER : METTLER TOLEDO

MODEL : XS105DU

SERIAL No : 1126422905

ID No : BA 05/50

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : SUCHAT S.

CALIBRATION DATE : 05-Mar-26

APPROVED BY :  PONGSAK J.

ISSUED DATE : 06-Mar-26

RECEIVED DATE : 05-Mar-26





CERTIFICATE No : 26M2266

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : XS105DU
MANUFACTURER : METTLER TOLEDO S/N : 1126422905
ID No : BA 05/50 RECEIVED DATE : 05-Mar-26
AIR PRESSURE : 1004mbar $\pm$ 1mbar CALIBRATION DATE : 05-Mar-26
AMBIENT TEMPERATURE : 25° C $\pm$ 1° C RELATIVE HUMIDITY : 50 %RH $\pm$ 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	C02250116	28-Jan-27
2) STANDARD WEIGHT	E2	15843	C02250117	29-Jan-27

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 120 g WAS 0.000055 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ($\pm$ g)
0.00	0.00000	0.00000	0.000065
0.02	0.02000	0.00000	0.000065
0.10	0.10000	0.00000	0.000066
0.20	0.20000	0.00000	0.000066
0.50	0.50001	-0.00001	0.000065
1.00	1.00001	-0.00001	0.000066
2.00	2.00000	0.00000	0.000067
5.00	5.00001	-0.00001	0.000068
10.00	10.00004	-0.00004	0.000070
20.00	20.00006	-0.00006	0.000078
50.00	50.00000	0.00000	0.00012
100.00	100.00002	-0.00002	0.00019
120.00	120.00002	-0.00002	0.00022

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.0000
2	50.0000
3	50.0000
4	50.0000
5	50.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN
associates



Cert. No. : SP25026

Pages : 1 of 4

Calibration Certificate

Equipment : UV-VIS SPECTROPHOTOMETER
Manufacturer : PERKINELMER
Model : LAMBDA 25
Serial No.: 501S14123010
ID No.: SP03/58
Calibration Mode : WAVELENGTH ACCURACY
PHOTOMETRIC ACCURACY
STRAY LIGHT

Condition As Found : GOOD

Customer : S.P.S CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN ROAD,
CHOMPHON SUB-DISTRICT, CHATUCHAK DISTRICT,
BANGKOK PROVINCE 10900 THAILAND.

Location : ORGANIC LABORATORY IV

Ambient Temperature : (22.9 $\pm$ 5) °C
Relative Humidity : (53.7 $\pm$ 25) %

Received Date : 22 AUGUST 2025
Calibration Date : 22 AUGUST 2025
Date of Issue : 25 AUGUST 2025

Calibrated by :

Nitinun Srihawan

Approved by :

Wichok B.
(Wichok Ekpongpradit)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : SP25026

Job No. : VC68SP0019

Pages : 2 of 4

Calibration Method :

This instrument was calibrated by using on-site calibration procedure In-house method : CP-SP-01

The calibration procedure to direct measurement wavelength accuracy by using wavelength standard solution, Photometric accuracy by using absorbance standard filter and absorbance standard solution

The calibration procedure used was based on ASTM E275-01, ASTM E925-02

Condition of this result of calibration :

1. Certified reference materials

<u>Material</u>	<u>Ref. type</u>	<u>Cell serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Holmium liquid	RM-HL	29706	126461	24/10/2026
Didymium liquid	RM-DL	28912	126462	24/10/2026
Neutral density filter	RM-1N2N3N	13877	126457	24/10/2026
Potassium dichromate solutions	RM-0204060810	14204	126497	25/10/2026
Potassium Iodide solution	-	KI-0701-001	CI-0185-24	14/05/2026

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 The UK National Physical Laboratory (NPL)

Result of calibration : Wavelength Accuracy

(Without adjustment)

Material	Certified Values of Reference Material (nm)	UUC* Reading (nm)	Error (nm)	Uncertainty ± (nm)	k Factor
RM-HL	278.13	278.21	0.08	0.16	2.00
	361.25	361.39	0.14	0.16	2.00
	467.82	467.71	-0.11	0.16	2.00
	536.56	536.50	-0.06	0.16	2.00
	640.50	640.36	-0.14	0.16	2.00
RM-DL	740.09	739.85	-0.24	0.16	2.00
	864.94	865.12	0.18	0.16	2.00

UUC* = Unit Under Calibration

Cert. No. : SP25026

Job No. : VC68SP0019

Pages : 3 of 4

Result of calibration : Photometric Accuracy

Material	Wavelength (nm)	Filter S/N	Nominal Absorbance (A)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor
Neutral Density glass filter	440.0	29381	0.5	0.5443	0.5413	-0.0030	0.0043	2.00
		29914	0.7	0.7484	0.7455	-0.0029	0.0054	2.00
		29360	1.0	1.0527	1.0535	0.0008	0.0032	2.00
	465.0	29381	0.5	0.4948	0.4922	-0.0026	0.0041	2.00
		29914	0.7	0.6906	0.6877	-0.0029	0.0050	2.00
		29360	1.0	0.9695	0.9709	0.0014	0.0031	2.00
	546.1	29381	0.5	0.5090	0.5068	-0.0022	0.0036	2.00
		29914	0.7	0.6985	0.6960	-0.0025	0.0041	2.00
		29360	1.0	0.9814	0.9825	0.0011	0.0031	2.00
	590.0	29381	0.5	0.5375	0.5353	-0.0022	0.0034	2.00
		29914	0.7	0.7256	0.7231	-0.0025	0.0037	2.00
		29360	1.0	1.0213	1.0219	0.0006	0.0032	2.00
	635.0	29381	0.5	0.5223	0.5202	-0.0021	0.0033	2.00
		29914	0.7	0.6927	0.6901	-0.0026	0.0036	2.00
		29360	1.0	0.9744	0.9750	0.0006	0.0032	2.00

UUC* = Unit Under Calibration

Cert. No. : SP25026

Job No. : VC68SP0019

Pages : 4 of 4

Result of calibration : Photometric Accuracy

(Without adjustment)

Material	Wavelength (nm)	Solution (mg/l)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor
Potassium dichromate solutions	235.0	20	0.2415	0.2443	0.0028	0.0101	2.00
		40	0.4866	0.4871	0.0005	0.0115	2.00
		60	0.7415	0.7295	-0.0120	0.0067	2.00
		80	0.9854	0.9844	-0.0010	0.0071	2.00
		100	1.2444	1.2425	-0.0019	0.0073	2.00

UUC* = Unit Under Calibration

Condition of this result of calibration : Spectrophotometer PERKINELMER Model LAMBDA 25 S/N 501S14123010

Resolution of Wavelength Mode 0.1 nm

Resolution of Photometric Mode 0.001 A

Parameter Setting

Measurement Mode Wavelength, Absorbance

Wavelength Scan 190 nm - 1100 nm

Scanning Speed 7.5 nm/min

Band width(Wavelength) 1.0

Band width(Vis) 1.0

Band width(Uv) 1.0

Stray Light** UUC* Reading at 220.0 nm	
Transimission T(%)	Absorbance(A)
0.020	3.7032

**Specific Acceptance :

Transmission ≤ 1.0 T(%), Absorbance ≥ 2.0 A

**Stray light not TISI Accredited

The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95%

End of Calibration Certificate



MAINTENANCE AND TEST CERTIFICATE MODEL

OPTIMA 5300DV

Customer : <u>S.P.S.Consulting Service Co.,Ltd</u>	Date Tested: <u>July 1, 2025</u>	
	Recommendation Recertification	
Address : <u>7 Soi Phaholyothin 24</u>	Period <u>6</u>	Months <u>Months</u>
<u>Paholyothin Road</u>	Recertification Due: <u>January 1, 2026</u>	
<u>Jompol Chatuchak, Bangkok 1090</u>	Date Last Certified: <u>January 6, 2025</u>	
User Name: <u>K.Phenpha Vipasthawatt</u>	Visit Number: <u>1of 2</u>	
Phone: <u>083-9269252</u>	PerkinElmer Phone: <u>02-719-6420 ext 206</u>	
Fax: <u>02-513-4221</u>	PerkinElmer Fax: <u>02-318-5597</u>	

CONFIGURATION TESTED		ACCESSORIES/COMPONENT NOT INCLUDED
MODEL	SERIAL NUMBER	
<u>OPTIMA 5300DV</u>	<u>077C7042401</u>	
TESTED EQUIPMENT	CALIBRATION NUMBER	EXPIRATION
<u>IPV Methods</u>		
TEST STANDARD USED	PART NUMBER	EXPIRATION DATE
<u>Multielement Standard</u>	<u>N069-1579</u>	<u>December 30, 2024</u>
<u>Wavecal Solution</u>	<u>N058-2152</u>	<u>March 30, 2024</u>
<u>VIS Wavecal solution</u>	<u>N930-2946</u>	<u>February 28, 2024</u>
<u>Instrument Cal. STD4</u>	<u>N930-0221</u>	<u>November 30, 2024</u>
CUSTOMER SUPPLIED	COMMENTS	CUSTOMER INITIALS
<u>2 % HNO3</u>		
<u>10 % HNO3</u>		



MAINTENANCE AND TEST CERTIFICATE MODEL

OPTIMA 5300DV

SERIAL NUMBER 077C7042401

DATE TESTED July 1, 2025

1. MECHANICAL CHECKS

- | | |
|--|-----------------------------|
| A. Inspect and clean all fans and filters. | ☐ OK |
| B. Inspect and replace as necessary, all torch components including the RF coil. | ☐ OK |
| C. Inspect all tubing for sign of clacking or leaking. | ☐ OK |
| D. Adjust water and gas pressure regulator settings. | ☐ OK |
| E. Inspect and leak check pneumatics drawers. | ☐ OK |
| F. Clean the exterior of the instrument. | ☐ OK |

2. OPTICAL CHECKS

- | | |
|---|-----------------------------|
| A. Inspect and clean all optical components. | ☐ OK |
| B. As required, check and replace all purgefilters. | ☐ OK |
| C. Recheck optical alignment. | ☐ OK |

3. COOLING SYSTEM CHECKS

- | | |
|---|------------------------------|
| A. Perform preventive maintenance on chiller. | ☐ OK |
| B. Flush out the chiller every year. | ☐ N/A |

4. PERFORMANCE CHECKS

- | | |
|----------------------------|-----------------------------|
| A. Torch View Alignment. | ☐ OK |
| B. Wavelength Calibration. | ☐ OK |



MAINTENANCE AND TEST CERTIFICATE MODEL

OPTIMA 5300DV

SERIAL NUMBER : 077C7042401
DATE TESTED : July 1, 2025

PARAMETER		SPECIFICATION		FINAL VALUE	
Spectral Resolution : UV	As	193.696 nm	≤ 0.007	<u>0.00570</u>	
	Ni	231.604 nm	≤ 0.008	<u>0.00734</u>	
	Ni	341.476 nm	≤ 0.012	<u>0.00763</u>	
Spectral Resolution : VIS	La	408.672 nm	≤ 0.020	<u>0.01627</u>	
	Ba	455.403 nm	≤ 0.025	<u>0.02428</u>	
Precision					
	As	193.656 nm	% RSD < 1.0	<u>0.82</u>	%
	Zn	213.856 nm	% RSD < 1.0	<u>0.83</u>	%
	Mn	257.610 nm	% RSD < 1.0	<u>0.20</u>	%
	La	379.478 nm	% RSD < 1.0	<u>0.89</u>	%
	Ba	455.403 nm	% RSD < 1.0	<u>0.92</u>	%
	Ba	493.408 nm	% RSD < 1.0	<u>0.75</u>	%
Detection Limits : Axial	Tl	190.080 nm	3(sd)	<u>10.65</u>	ppb
	As	193.696 nm	3(sd)	<u>2.48</u>	ppb
	Pb	220.353 nm	3(sd)	<u>3.09</u>	ppb
Detection Limits : Radial	As	193.696 nm	3(sd)	<u>331.50</u>	ppb
	Zn	213.856 nm	3(sd)	<u>0.98</u>	ppb
	Mn	257.610 nm	3(sd)	<u>0.34</u>	ppb
	La	379.478 nm	3(sd)	<u>2.54</u>	ppb
	Ba	455.403 nm	3(sd)	<u>2.19</u>	ppb
	Ba	493.408 nm	3(sd)	<u>4.32</u>	ppb
BEC : Axial (IB X 500)/(IS-IB)	Cd	226.502 nm	≤ 150 ppb	<u>140.03</u>	
BEC : Radial (IB X 1000)/(IS-IB)	Mn	257.610 nm	≤ 45 ppb	<u>24.17</u>	



MAINTENANCE AND TEST CERTIFICATE MODEL

OPTIMA 5300DV

SERIAL NUMBER 077C7042401DATE TESTED July 1, 2025**Remarks :**

Commissioning follow as commissioning performance sheets.

This is to certify that the above tests have been performed and the configuration tested



meets



does not meet

the PerkinElmer Specifications listed on this certificate.

This certificate does not modify PerkinElmer's standard terms and condition of sale,
including warranty terms.

Service Department PerkinElmer Ltd.**Authorized Representative:**

(Wiphan Promlumda)

Service Engineer



Certificate of Calibration

Aquion : Anion (ID#894)

This certificate is to verify that instrument below are calibrated

by Archemica Lab Co.,Ltd.

AQUION S/N : 190840059

AS-DV S/N : 190915235

for

S.P.S. Consulting Service Co., Ltd.



บริษัท อาร์เคมีกา แล็บ จำกัด
ARCHEMICA LAB CO.,LTD.

Operator Signature : Teerapat B

Date : Jun 6, 2025

(Mr. Teerapat Boonla)

Application Chemist



Certificate of Calibration

Aquion : Anion (ID#894)

This certificate is to verify that instrument below are calibrated

by Archemica Lab Co.,Ltd.

AQUION S/N : 190840059

AS-DV S/N : 190915235

for

S.P.S. Consulting Service Co., Ltd.



Operator Signature : Wasin Date : April 27, 2026

(Mr. Wasin Nintalad)

Test Engineer

GC Clarus 600/680 Preventive Maintenance (PM)

Company Name:	S.P.S. Consulting Service Co.,Ltd		
Address (Instrument Location):	7 Soi Phaholyothin24 Phaholyothin Road, Jompol, Chatuchak, Bangkok, 10900.		
Serial Number:	680S14042502	Service Tag:	N68APSSFXMP
Customer Name (if applicable):	Ms.Naruecha	PM number:	1 of 2
Service Engineer Name:	Monchai Kitcharoenkeat	Service Order Number:	WO-11858723
Date PM Performed: (DD-MMM-YYYY)	13-Feb-2026	Next PM Due Date: (DD-MMM-YYYY)	13-Aug-2026

Part Number	Release	Publication Date	
TH09370070	C	August 2016	

Scope

The purpose of this PM is to ensure the continued functionality of the Clarus 600 and Clarus 680 GC by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer. The customer should save their method before the PM begins.

General Instructions:

The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM. Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files. The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer. Update the PM sticker and instrument logbook as required.

Copyright Information

This document contains proprietary information that is protected by copyright. All rights are reserved. No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of Perkin Elmer, Inc. **Copyright © 2013 PerkinElmer, Inc.**

Trademarks

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners. **Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no Warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.** PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

Component List

Component / Specific Model	Serial #	Software Version	Configuration Notes
Clarus680	680S14042502	Totalchrom6.3.2	PSS, PSS, FID,
Clarus SQ8T	648N4050804	Turbomass 6.4	
AtomX	US14113002	Tekma AtomX	

Parts Lists

Additional Tools Required for PM				
Part Number (if applicable)	Description	Quantity	Serial #	Calibration Due Date (MM/YY)
N/A				
Additional Reagents and Standards Required for PM				
Part Number (if applicable)	Description	Quantity	Batch/Lot #	Expiration Date (MM/YY)
N/A				

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. General:

- ☒ Review the instrument performance with the customer and document any recent problems.

- ☒ Check incoming AC line voltage for proper levels and grounding.

L-N 220 Volt

L-G 220 Volt

N-G 0.46 Volt

**Neutral to ground not more than 0.5 volts peak to peak*

- ☒ Inspect all gas line filters and traps; Replace if necessary with customer supplied spares.

Carrier gas ☒ Helium ☐ Nitrogen ☐ Hydrogen

Moisture level ☒ Good ☐ Need to replace ☐ Other _____

Detector gas ☒ Air Zero ☒ Hydrogen ☐ Nitrogen ☐ Helium

Moisture level ☒ Good ☐ Need to replace ☐ Other _____

- ☒ Inspect the customer log book and make any appropriate PM entries.

- ☒ Leak check all fittings from the gas source to instrument.

Gas leakage ☒ Pass ☐ Fail Comment _____

- ☒ Perform general inspection of system for cleanliness.

- ☒ Inspect for functional and clean electronic cooling and oven vent fans

Electronic cooling fan ☒ Yes ☐ No

Oven cooling fan ☒ Yes ☐ No

2. Electronic :

- ☒ Check oven temperature. Calibrate if necessary.

Oven temperature set point 150 °C ☒ Pass ☐ Fail

- ☐ Check sub-ambient option. (If installed).

Oven temperature set point 5 °C ☐ Pass ☐ Fail

- ☒ Perform routine maintenance on detector/injector. Replace parts as necessary with customer supplied spares.

- ☒ Check flows, including split flows if applicable. Calibrate if necessary.

Carrier flow	Pass
Split flow	Pass
- ☒ Check detector gas flows and adjust if necessary.

Detector flow	Pass
---------------	------
- ☒ Autosampler installed ☒ Yes ☐ No

Check autosampler sensor for wear and replace if necessary.	
Vial sensor	Pass
Door sensor	Pass
Tower sensor	Pass
Plunger sensor	Pass
Elevator sensor	Pass
- ☒ Remove syringe, manually flush. Replace with customer supplied spare if necessary.
- ☒ Check firmware version. Upgrade to current levels if necessary.

Firmware version	<u>6.5</u>
------------------	------------
- ☒ Measure all accessible power supply voltages.

5 Volt	Pass
+15 Volt	Pass
-15 Volt	Pass
24 Volt	Pass
- ☒ Record all detector voltage signal.

Detector Channel A	<u>0.87</u>	mV.
Detector Channel B	<u>NA</u>	mV.

3. Diagnostics Tests:

- ☒ Run instrument diagnostics.

☒ BRAM	Pass
☒ EPROM	Pass
- ☒ Run Autosampler diagnostics.

☒ BRAM	Pass
☒ EPROM	Pass

4. Review:

- ☒ Review with the customer PM work performed.
- ☒ Review with the customer routine maintenance procedures.
- ☒ Discuss recommended customer-supplied materials to have on hand
- ☒ Attach PM sticker.
- ☒ Update Logbook.

Additional Comments

Additional Comments Regarding the PM

Review

<i>The preventive maintenance checks and if applicable performance tests for Clarus600/680 GC have been completed.</i>	
<i>This Clarus600/680 GC Pass the preventive maintenance.</i>	
Review of Preventive Maintenance:	
Authorized PerkinElmer Representative: Monchai Kitcharoenkeat	Date: 13-Feb-2026 (DD-MMM-YYYY)
Authorized Customer Representative: Ms.Naruecha	Date: 13-Feb-2026 (DD-MMM-YYYY)

ลำดับที่ 3

ระดับเสียงในบรรยากาศโดยทั่วไป



CERTIFICATE OF CALIBRATION

NO. 20250704103

Name of Product:	Sound Level Meter
Model:	ST-12D
Serial Number:	10351461
Specification:	Class 1
Conclusion:	Pass
Date of calibration:	2025-09-05
Due Date:	2026-09-04



Calibrated by:

- This report certifies that all calibration equipment used in the test is traceable with the internal ISO9001 procedures and meets all specification given in the Manual(s) or respectively surpass then, and applies only to the unit identified above.
- This certificate is produced with advanced equipment & procedures which permit comprehensive quality assurance verification of all data supplied herein.
- This certificate of calibration shall not be reproduced except in full, without written permission of the Scarlet Tech Co Ltd Taiwan.

1. Preliminary inspection: OK

2. Type & serial No. of Microphone: AWA14425-80380

4. Measuring up limit: 140 dBA

3. Adjustments to indicated sound levels:

5. Frequency weightings (Acoustic signal tests for Z weighting, other electric signal tests.)

Type of Calibrator B&K 4231

Sound Pressure Level 94.0 dB

Equivalent Free-field Sound Level (reference environment conditions) 93.8 dB

Nominal frequency /Hz	Frequency weighting / dB			Nominal frequency /Hz	Frequency weighting / dB		
	A	C	Z		A	C	Z
10	-69.7	-14.3	0.0	1000	0.0	0.0	0.0
20	-50.4	-6.2	+0.1	2000	+1.1	-0.2	0.0
31.5	-39.5	-3.0	0.0	4000	+1.0	-0.8	0.0
63	-26.2	-0.8	0.0	8000	-1.1	-3.0	0.0
125	-16.2	-0.2	0.0	12500	-6.0	-7.9	-0.9
250	-8.7	0.0	+0.1	16000	-6.5	-8.5	0.0
500	-3.3	0.0	+0.1	20000	-9.3	-11.2	0.0

6. Self-generated noise

Microphone replaced by electrical input signal device

10.9 dB(A)	11.5 dB(C)	17.3 dB(Z)
------------	------------	------------

7. F&S Weighting

Rate of the F weighting decrease (dB/s)	34.4
Rate of the S weighting decrease (dB/s)	3.4
Deviation of F&S	0.0

8. Level Linearity (A-weighting at frequency 1 kHz)

Reference sound level 90.0 dB

Max error at 10dB steps upper reference sound level 0.1 dB

Max error at 1dB steps within 5dB of the upper limit linear operating range 0.0 dB

Max error at 10dB steps below reference sound level 0.2 dB

Max error at 1dB steps within 5dB upper the lower limit linear operating range 0.2 dB

9. Tone burst response (A Weighting) :

Single Toneburst duration /ms	Toneburst response /dB			
	LAFmax-LA	LASmax-LA	LAE-LA	LAeqT-LA
500	-0.1	-4.1	-3.0	-7.0
200	-1.0	-7.5	-7.0	-7.0
2	-18.1	-27.1	-27.2	-7.1
0.25	-27.1	/	-36.1	-7.0

10. Peak C sound level (500Hz) :

Cycle	One cycle	nominal value	Positive half	nominal value	Negative half	nominal value
LCpeak-LC(dB)	3.4	3.5	2.3	2.4	2.3	2.4

11. Overload indication: Pass

12. Statistical analysis function

Sweep signal maximum indicated sound level: 112.8 dB

Sweep amplitude: 40 dB

Scan cycle time: 60 S; Measurement period: 180 S.

Items	Measured value/dB	Theoretical calculated value/dB	Error/dB
LAeq,T	103.2	103.1	0.1
L5	110.8	110.8	0.0
L10	108.8	108.8	0.0
L50	92.9	92.8	0.1
L90	76.9	76.9	0.0
L95	75.0	74.9	0.1

Uncertainty of measurement results: 0.4 dB (k=2)

13.Part of sound exposure: Pass

14.Data logging function: Pass

15. TF card & wave recording function: Pass

Environment conditions:

Air temperature: 25 °C

Relative humidity: 60 %

Static pressure: 102.0 kPa

References:

IEC 61672-3 Sound Level Meters Part 3: Periodic tests



CERTIFICATE OF CALIBRATION

NO. 20250704106

Name of Product:	Sound Level Meter
Model:	ST-12D
Serial Number:	10351464
Specification:	Class 1
Conclusion:	Pass
Date of calibration:	2025-09-05
Due Date:	2026-09-04



Calibrated by:

- This report certifies that all calibration equipment used in the test is traceable with the internal ISO9001 procedures and meets all specification given in the Manual(s) or respectively surpass them, and applies only to the unit identified above.
- This certificate is produced with advanced equipment & procedures which permit comprehensive quality assurance verification of all data supplied herein.
- This certificate of calibration shall not be reproduced except in full, without written permission of the Scarlet Tech Co Ltd Taiwan.

1. Preliminary inspection: OK

2. Type & serial No. of Microphone: AWA14425-80364

4. Measuring up limit: 140 dBA

3. Adjustments to indicated sound levels:

5. Frequency weightings (Acoustic signal tests for Z weighting, other electric signal tests.)

Type of Calibrator B&K 4231

Sound Pressure Level 94.0 dB

Equivalent Free-field Sound Level (reference environment conditions) 93.8 dB

Nominal frequency /Hz	Frequency weighting / dB			Nominal frequency /Hz	Frequency weighting / dB		
	A	C	Z		A	C	Z
10	-69.7	-14.3	+0.1	1000	0.0	0.0	0.0
20	-50.4	-6.1	+0.1	2000	+1.1	-0.1	0.0
31.5	-39.4	-2.9	0.0	4000	+1.0	-0.8	0.0
63	-26.1	-0.8	0.0	8000	-1.1	-3.0	0.0
125	-16.2	-0.1	0.0	12500	-6.0	-7.9	-0.8
250	-8.7	0.0	+0.1	16000	-6.4	-8.4	0.0
500	-3.3	0.0	+0.1	20000	-9.3	-11.1	0.0

6. Self-generated noise

Microphone replaced by electrical input signal device

10.9 dB(A)	11.6 dB(C)	16.7 dB(Z)
------------	------------	------------

7. F&S Weighting

Rate of the F weighting decrease (dB/s)	34.6
Rate of the S weighting decrease (dB/s)	3.4
Deviation of F&S	0.0

8. Level Linearity (A-weighting at frequency 1 kHz)Reference sound level 90.0 dBMax error at 10dB steps upper reference sound level 0.1 dBMax error at 1dB steps within 5dB of the upper limit linear operating range 0.0 dBMax error at 10dB steps below reference sound level 0.2 dBMax error at 1dB steps within 5dB upper the lower limit linear operating range 0.2 dB**9. Tone burst response (A Weighting) :**

Single Toneburst duration /ms	Toneburst response /dB			
	$L_{AFmax}-L_A$	$L_{ASmax}-L_A$	$L_{AE}-L_A$	$L_{AeqT}-L_A$
500	-0.1	-4.1	-3.0	-7.0
200	-1.0	-7.5	-7.0	-7.0
2	-18.1	-27.1	-27.2	-7.1
0.25	-27.2	/	-36.1	-7.0

10. Peak C sound level (500Hz) :

Cycle	One cycle	nominal value	Positive half	nominal value	Negative half	nominal value
$LC_{peak}-LC(dB)$	3.4	3.5	2.4	2.4	2.4	2.4

11. Overload indication: Pass**12. Statistical analysis function**Sweep signal maximum indicated sound level: 112.8 dBSweep amplitude: 40 dBScan cycle time: 60 S; Measurement period: 180 S.

Items	Measured value/dB	Theoretical calculated value/dB	Error/dB
L_{Aeq,T}	103.2	103.1	0.1
L₅	110.8	110.8	0.0
L₁₀	108.8	108.8	0.0
L₅₀	92.9	92.8	0.1
L₉₀	76.9	76.9	0.0
L₉₅	75.0	74.9	0.1

Uncertainty of measurement results: 0.4 dB (k=2)

13.Part of sound exposure: Pass

14.Data logging function: Pass

15. TF card & wave recording function: Pass

Environment conditions:

Air temperature: 25 °C

Relative humidity: 60 %

Static pressure: 102.0 kPa

References:

IEC 61672-3 Sound Level Meters Part 3: Periodic tests



Certificate of Calibration

Certificate Number : SPR25100435-1

Page : 1 of 3

Customer : S.P.S. CONSULTING SERVICE CO., LTD.

7 Soi Phaholyothin 24 Phaholyothin Road., Jompol, Chatuchak,
Bangkok 10900

Equipment Name : Sound Level Meter

Manufacturer : Cirrus

Model : N/A

Serial Number : G301401

ID. Number : CR-B09

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Relative Humidity : $50\% \pm 15\%$

Location of Calibration : In-Lab

Calibration Procedure : SP-CPE-04-01

Received Date : 29 Oct 2025

Calibration Date : 30 Oct 2025

Recommend Due Date : 30 Oct 2026

Date of Issue : 31 Oct 2025

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Chumpon Dokpikul

Calibration Officer

Approved by



(Mr.Worapong Sinthusopa)

Authorized Signatory



Calibration Report

Certificate Number : SPR25100435-1

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP.22/0268	20 Feb 2026

Traceability

This certification is traceable to the International System of Unit maintained at :
TISTR - Thailand Institute of Scientific and Technological Research



Result of Calibration

Certificate Number : SPR25100435-1

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.9	113.9	-0.1	-0.1	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.9	113.9	-0.1	-0.1	0.15

Note :

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -

Certificate No. EN-250601-15

Calibration & Test Certificate

FOR

Equipment Name : Sound Level Meter

Received Date : May 28, 2025

Manufacturer : CIRRUS

Calibration Date : June 1, 2025

Model : CR161 B

Recommended Due Date : N/A

Serial Number : G301407

Location of Calibration : In Lab

Customer Name : S.P.S. CONSULTING SERVICE CO., LTD.

7 SOI PHAHOLYOTHIN 24 ROAD, JOMPHOL, CHATUCHAK,
BANGKOK 10900

CONDITION AS RECIVED : Normal

Environmental Conditions

Ambient Temperature : (25 ± 2) °C

Relative Humidity : (50 ± 15) %RH

Result : No Adjustment (See data attached in page 2 to the end of certificate)

1. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $K = 2$ providing a level of confidence of approximately 95%
2. The Unit Under Calibration (UUC) has been calibrated by using the working standard which is traceable to SI-Unit. The calibration procedure documented is intended to implement the requirements of ISO/IEC 17025 : 2005 (TAF)
3. The working standard is indicated in page 2 of this certificate.
4. The report applies to the item and shall not be reproduced except in full, without written approval by Calibration Laboratory, Envir Service Co., Ltd.

Date of Calibration : June 1, 2025

Valid to : May 31, 2026



Calibrated By : 

Kittisak Jansangwattana
(Technician)

Approved By : 

Pasagorn Samol
(Technician Manager)

Certificate No. EN-250601-15

We hereby certify that the instrument under mentioned has been certainly calibrated according to our calibration standard and the testing result in the calibration procedure has been good enough within the tolerance regulated in our specification.

Reference Standard

Equipment Name	Model	Serial Number	Due Date
Standard SOUND LEVEL METER	B&K 2239	2449143	OCT/22/2025

The Standard generators used for calibration procedure are proofed once a year and cab be traceable to the standard authorized by public organization.

Result of Calibration

Calibration Range : 94 dB, 114 dB

Function : @ 1KHz

Select A Fast response

STD Setting	UUC Reading (dB)	Correction (dB)	Uncertainty (±)
94.01	93.8	0.21	0.88
114.04	114.0	0.04	0.88

Select A Slow response

STD Setting	UUC Reading (dB)	Correction (dB)	Uncertainty (±)
94.01	93.8	0.21	0.88
114.04	113.9	0.14	0.88

Select C Fast response

STD Setting	UUC Reading (dB)	Correction (dB)	Uncertainty (±)
94.01	93.8	0.21	0.88
114.04	113.9	0.14	0.88

Select C Slow response

STD Setting	UUC Reading (dB)	Correction (dB)	Uncertainty (±)
94.01	93.9	0.11	0.88
114.04	113.8	0.24	0.88

STD = Standard

UUC = Unit Under Calibration



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sales@spscon.com, www.spscon.com

Noise R_094/26

Sound Level Meter Calibration Report

Acoustic Calibrator Data

Brand	CIRRUS	Number	AC-CR01/63
Model	CR515	Serial No.	92002
Calibration Range	94 dB, 1000 Hz	Last Calibration	11 February 2026
		Due Date	11 February 2027

Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ST-C1-B06	SCARLET	ST-12D	10351461	19 February 2026	94.0	94.0
ST-C1-B07	SCARLET	ST-12D	10351464	19 February 2026	94.1	94.0
CR-B09	Cirrus	CR161B	G301401	19 February 2026	94.0	94.0
CR-B10	Cirrus	CR161B	G301407	19 February 2026	94.0	94.0
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.98 ± 0.10 dB	

Calibrated by :

Heeson L.

(Mr. Heeson Lormae)

Approved by :

Yutthana J.

(Mr. Yutthana Tanatharanit)

ลำดับที่ 4

คุณภาพน้ำทิ้ง

**QUALITY CALIBRATION CO., LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584



CERTIFICATE No : 26E3363
REFERENCE No : 80514-1


PAGE : 1 OF 3

Certificate of Calibration

EQUIPMENT : pH METER
MANUFACTURER : HANNA
MODEL : HI3512
SERIAL No : TH118035
ID No : PH 04/56
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.

CALIBRATION DATE : 02-Apr-26

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 02-Apr-26

RECEIVED DATE : 01-Apr-26

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.





QUALITY CALIBRATION CO., LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 26E3363

PAGE : 2 OF 3

Calibration Report

EQUIPMENT : pH METER
MANUFACTURER : HANNA
ID No : PH 04/56
RECEIVED DATE : 01-Apr-26
AMBIENT TEMPERATURE : 23 ° C ± 3 ° C
MODEL : HI3512
SERIAL NUMBER : TH118035
CALIBRATION DATE : 02-Apr-26
RELATIVE HUMIDITY : 50 % RH ± 10% RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT METHOD BASED ON WI-TQ-062 AND WI-TQ-063. THE DISPLAY UNIT WAS TESTED BY GENERATING STANDARD VOLTAGE TO THE UNIT AND READING THE VALUE COMPARED WITH THE CALCULATED VALUE. THE DISPLAY AND ELECTROD WAS CALIBRATED BY USING STANDARD pH BUFFER
2. REFERENCE STANDARD INSTRUMENTS :-

<u>INSTRUMENT</u>	<u>MODEL</u>	<u>SERIAL No/</u> <u>LOT No</u>	<u>CERTIFICATE No</u>	<u>DUE DATE</u>
1) pH STANDARD SOLUTION	00651-36	CC829914	4956-16178366	11-Sep-27
2) pH STANDARD SOLUTION	00651-38	CC831093	4957-16224157	01-Oct-27
3) pH STANDARD SOLUTION	00651-40	CC826321	4958-16046326	10-Jul-27
4) PROCESS CALIBRATOR	CA150	91S6079	26E936	17-Mar-27
5) BATH	260014	1247 48074	25T9431	12-Sep-26
6) THERMOMETER WITH PROBE	421504	55000379	25T9466	12-Sep-26

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO SI UNIT MAINTAINED AT :-
 - NATIONAL INSTITUTE OF STANDARD AND TECHNOLOGY, USA.
 - NATIONAL INSTUTITE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION : ADJUSTMENT

1. DISPLAY UNIT ONLY

SLOPE FACTOR $k = 2.303 RT/F = 59 \text{ mV/pH}$

mV APPLIED	UUC READING (mV)	CORRECTION (mV)	UUC READING (pH)	UNCERTAINTY OF MEASUREMENT (± mV)	COVERAGE FACTOR k
414.11	414.3	-0.19	-0.256	0.15	2.00
354.95	355.1	-0.15	0.759	0.15	2.00
295.80	296.0	-0.20	1.773	0.15	2.00
236.64	236.8	-0.16	2.787	0.15	2.00
177.48	177.7	-0.22	3.801	0.15	2.00
118.32	118.5	-0.18	4.816	0.15	2.00
59.16	59.4	-0.24	5.831	0.15	2.00
0.00	0.2	-0.20	6.845	0.15	2.00
-59.16	-58.9	-0.26	7.878	0.15	2.00
-118.32	-118.1	-0.22	8.915	0.15	2.00
-177.48	-177.2	-0.28	9.952	0.15	2.00
-236.64	-236.4	-0.24	10.990	0.15	2.00
-295.80	-295.5	-0.30	12.027	0.15	2.00
-354.95	-354.7	-0.25	13.064	0.15	2.00
-414.11	-413.8	-0.31	14.101	0.15	2.00

END OF CALIBRATION REPORT PAGE 2 OF 3





QUALITY CALIBRATION CO., LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkai, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 26E3363

PAGE : 3 OF 3

Calibration Report

RESULT OF CALIBRATION (CONTINUE) :

2. DISPLAY UNIT WITH pH ELECTRODE S/N: 11340D0M

STANDARD pH BUFFER SOLUTION (pH)	UUC READING (pH)	CORRECTION (pH)	VALUE BEFORE ADJUSTMENT	UNCERTAINTY OF MEASUREMENT ($\pm$ pH)	COVERAGE FACTOR k
4.008	4.008	0.000	4.142	0.012	2.00
6.998	7.000	-0.002	7.068	0.012	2.00
10.007	10.009	-0.002	10.226	0.014	2.00

3. DISPLAY UNIT WITH TEMPERATURE

STANDARD READING ($^{\circ}$ C)	UUC READING ($^{\circ}$ C)	CORRECTION ($^{\circ}$ C)	VALUE BEFORE ADJUSTMENT	UNCERTAINTY OF MEASUREMENT ($\pm$ $^{\circ}$ C)	COVERAGE FACTOR k
25.004	25.0	0.004	---	0.0085	2.00

4. PERCENT SLOPE 91%

UUC : UNIT UNDER CALIBRATION

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





CALIBRATION LABORATORY Co., LTD.

2/10-11,14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CERTIFICATE OF CALIBRATION FOR

NOMENCLATURE : pH METER
MANUFACTURER : HANNA
MODEL / TYPE : HI3512/HI1332/HI7662-T
SERIAL NO. : 08685754/11250B7M/092806BN[PH04/56]
CLID. NO. : 272501562
JOB CONTROL NO. : 250617070523
CALIBRATION SERVICE : ☒ IN-LABORATORY ☐ ON-SITE

CUSTOMER : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24 ROAD, JOMPOL,
CHATUCHAK, BANGKOK 10900

DATE OF RECEIVED : 17 June 2025

DATE OF ISSUED : 20 June 2025

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sukgasem Seehanart
Wenick Inchaisri
Calibration Engineer

Approved By : Mongkol Yotsoontorn
Authorized Signatory
20 June 2025



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to
the International System of Units (SI)

Certificate No. Q25070523

F3-011-05/12-23

page 1 of 4



@clccalibration



CLC
Accredited
ISO/IEC 17025

CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230

Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



REPORT OF CALIBRATION

FOR

NOMENCLATURE : **pH METER**
MANUFACTURER : **HANNA**
MODEL / TYPE : **HI3512/HI1332/HI7662-T**
SERIAL NO. : **08685754/11250B7M/092806BN[PH04/56]**
DATE OF CALIBRATION : **18 June 2025**

ENVIRONMENT CONDITIONS :

Temperature : **$(25 \pm 2.5) ^\circ\text{C}$**

Relative Humidity : **$(50 \pm 15) \% \text{ RH}$**

PROCEDURE USED :

This instrument was calibrated under procedure No. **CLC-CPCH-01** [pH Meter]. The calibration was performed by direct measurement with Certified Reference Material (CRM).

This instrument was calibrated under procedure No. **CLC-CPTH-04** [Temperature] based on **ASTM E 644-04** as calibration guidelines. The calibration was performed by using Calibration Bath, Precision Thermometer and IPRT which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. pH Standard Solution, NIMT TRM CODE TRM-S-2003, TRM CODE TRM-S-2007.
2. pH Standard Solution, Control Company Catalog Number 06664260,11754256, Lot Number CC787362.
3. Calibration Bath, Kambic Model OB-22/2 ULT S/N. 17115653.
4. Precision Thermometer, ASL Model F250 S/N. 1334023800.
5. IPRT, Wika Model CTP5000-250-D S/N. PO00043543-1-10-1.

Certificate No. **Q25070523**

F3-011-05/12-23

page 2 of 4



@clccalibration



CALIBRATION LABORATORY CO., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



TRACEABILITY :

1. The measurements are traceable to International System of Units (SI) , through National Institute of Metrology (Thailand).
Lot Number. 080124 , 120124. Due Date 23 January 2026.
2. The measurements are traceable to International System of Units (SI) , through Control Company.
Certificate No. 4281-14495731 , Due Date 27 September 2025.
3. The measurements are traceable to International System of Units (SI) , through Calibration Laboratory Co., Ltd.
Certificate No. Q24120999, Due Date 26 November 2025.
4. The measurements are traceable to International System of Units (SI) , through Thailand Institute of Scientific and Technological Research (TISTR). Certificate No. PSL-T 1042/67, Due Date 16 October 2025.
5. The measurements are traceable to International System of Units (SI) , through National Institute of Metrology (Thailand).
Certificate No. TT-0146-24, Due Date 28 October 2025.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q25070523

F3-011-05/12-23

page 3 of 4



@clccalibration



CLC
Accredited
ISO/IEC 17025

CALIBRATION LABORATORY Co., LTD.

2/10-11, 14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230

Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The table in the following gives the calibration results and associated measurement uncertainties of pH meter.

CALIBRATION DATA

1. pH METER RESULT @ 25 °C

Standard pH Buffer Solution (pH)	pH Meter Reading (pH)	pH Meter Reading (mV)	Correction (pH)	Uncertainty of pH Measurement ($\pm$ pH)	k Factor
4.003	4.005	168.2	-0.002	0.010	2,00
7.005	7.010	-8.1	-0.005	0.013	2,00
10.015	10.010	-177.7	+0.005	0.014	2,00

Technical Note. Setting function CAL 3 point (4,7,10).

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 015 Page 4 of 68

2. TEMPERATURE RESULT

Immersion depth (mm)	Actual Temperature (°C)	DUC Reading (°C)	Correction (°C)	Uncertainty $\pm$ (°C)
100	25.00	25.0	0.00	0.07

Technical Note. Type of sensor : Thermistor

Probe $\varnothing$ 3 mm

Materials : Metal Sheath.

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor of $k = 2,00$.

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 015 Page 56 of 68

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q25070523

F3-011-05/12-23

page 4 of 4



@clccalibration



CERTIFICATE No : 25M2256
REFERENCE No : 76365-3

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE

MANUFACTURER : SARTORIUS

MODEL : BSA224S-CW

SERIAL No : 36591843

ID No : BA09/61

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.

CALIBRATION DATE : 07-Mar-25

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 13-Mar-25

RECEIVED DATE : 07-Mar-25

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.





CERTIFICATE No : 25M2256

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : BSA224S-CW
MANUFACTURER : SARTORIUS S/N : 36591843
ID No : BA09/61 RECEIVED DATE : 07-Mar-25
AIR PRESSURE : 1009mbar $\pm$ 1mbar CALIBRATION DATE : 07-Mar-25
AMBIENT TEMPERATURE : 24° C $\pm$ 1° C RELATIVE HUMIDITY : 52 %RH $\pm$ 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	C02250116	28-Jan-27
2) STANDARD WEIGHT	E2	15843	C02250117	29-Jan-27

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0.000071 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ($\pm$ g)
0.00	0.0000	0.0000	0.00012
0.10	0.1000	0.0000	0.00012
0.20	0.2000	0.0000	0.00012
0.50	0.5000	0.0000	0.00012
1.00	1.0000	0.0000	0.00012
2.00	2.0000	0.0000	0.00012
5.00	5.0000	0.0000	0.00012
10.00	10.0000	0.0000	0.00012
20.00	20.0001	-0.0001	0.00012
50.00	50.0000	0.0000	0.00014
100.00	100.0001	-0.0001	0.00019
200.00	200.0001	-0.0001	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	100.0000
2	100.0000
3	100.0000
4	100.0000
5	100.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





CERTIFICATE No : 26M2268

REFERENCE No : 80204-3

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE

MANUFACTURER : SARTORIUS

MODEL : BSA224S-CW

SERIAL No : 36591843

ID No : BA 09/61

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : SUCHAT S.

CALIBRATION DATE : 05-Mar-26

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 06-Mar-26

RECEIVED DATE : 05-Mar-26





CERTIFICATE No : 26M2268

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE **MODEL** : BSA224S-CW
MANUFACTURER : SARTORIUS **S/N** : 36591843
ID No : BA 09/61 **RECEIVED DATE** : 05-Mar-26
AIR PRESSURE : 1004mbar $\pm$ 1mbar **CALIBRATION DATE** : 05-Mar-26
AMBIENT TEMPERATURE : 25° C $\pm$ 1° C **RELATIVE HUMIDITY** : 50 %RH $\pm$ 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

<u>INSTRUMENT</u>	<u>MODEL</u>	<u>SERIAL No</u>	<u>CERTIFICATE No</u>	<u>DUE DATE</u>
1) STANDARD WEIGHT SET	E2	QK-I-151	C02250116	28-Jan-27
2) STANDARD WEIGHT	E2	15843	C02250117	29-Jan-27

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0.000055 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ($\pm$ g)
0.0	0.0000	0.0000	0.00010
0.1	0.1000	0.0000	0.00011
0.2	0.2000	0.0000	0.00010
0.5	0.5000	0.0000	0.00011
1.0	1.0000	0.0000	0.00011
2.0	2.0000	0.0000	0.00011
5.0	5.0000	0.0000	0.00011
10.0	10.0000	0.0000	0.00011
20.0	20.0001	-0.0001	0.00011
50.0	50.0000	0.0000	0.00013
100.0	100.0001	-0.0001	0.00019
200.0	200.0001	-0.0001	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	100.0000
2	100.0000
3	100.0000
4	100.0000
5	100.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





QUALITY CALIBRATION CO., LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com

CERTIFICATE No : 25T0521

REFERENCE No : 75853-2

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : COD REACTOR

MANUFACTURER : HACH

MODEL : DRB 200

SERIAL No : 15110C0498

ID No : CRB 06/59

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : CHAICHARN CH.

CALIBRATION DATE : 03-Feb-25

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 03-Feb-25

RECEIVED DATE : 15-Jan-25





QUALITY CALIBRATION CO., LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 25T0521

PAGE : 2 OF 2

Calibration Report


EQUIPMENT : COD REACTOR
MANUFACTURER : HACH
ID NUMBER : CRB 06/59
RECEIVED DATE : 15-Jan-25
AMBIENT TEMPERATURE : 23° C ± 1° C
MODEL : DRB 200
SERIAL NUMBER : 15110C0498
CALIBRATION DATE : 03-Feb-25
RELATIVE HUMIDITY : 53 %RH ± 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT METHOD WITH CALIBRATED THERMOCOUPLE TYPE K UNDER NO LOAD CONDITION. THE THERMOCOUPLES WERE PLACED ON POINTS AND LOCATED AS THE PICTURE.
2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH TC TYPE K	HYDRA 2635A	7301307	24T6467	26-Jun-25
3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO., LTD.

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

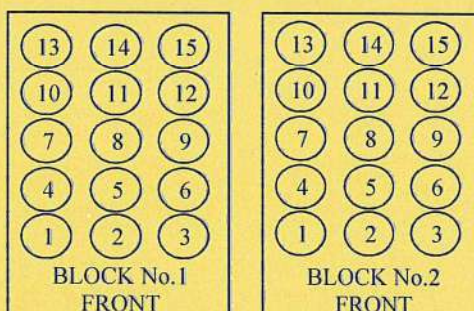

Block No.	1	2
Calibration Point (°C)	150	150
Controller temperature (°C)	145	145
Indicating Temperature	145	145
Measured Temperature (°C) at Spread Locations	1	150.23
	2	149.73
	3	150.29
	4	150.04
	5	150.09
	6	150.74
	7	149.97
	8	150.76
	9	150.54
	10	149.44
	11	150.12
	12	149.93
	13	149.19
	14	148.96
	15	149.09
Uncertainty of Measurement(± °C)	0.88	0.88

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2 : LOCATION 10 WAS REFERENCE LOCATION.

NOTE 3 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





QUALITY CALIBRATION CO., LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com

CERTIFICATE No : 26T0464

REFERENCE No : 79659-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : COD REACTOR

MANUFACTURER : HACH

MODEL : DRB 200

SERIAL No : 15110C0497

ID No : DRB 04/59

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : SOMCHAI S.

CALIBRATION DATE : 30-Jan-26

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 30-Jan-26

RECEIVED DATE : 30-Jan-26

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.



F-G010 REV : 03



CERTIFICATE No : 26T0464

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : COD REACTOR
MANUFACTURER : HACH
ID NUMBER : DRB 04/59
RECEIVED DATE : 30-Jan-26
AMBIENT TEMPERATURE : 23° C ± 1° C

MODEL : DRB 200
SERIAL NUMBER : 15110C0497
CALIBRATION DATE : 30-Jan-26
RELATIVE HUMIDITY : 54 %RH ± 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT METHOD WITH CALIBRATED THERMOCOUPLE TYPE K UNDER NO LOAD CONDITION. THE THERMOCOUPLES WERE PLACED ON POINTS AND LOCATED AS THE PICTURE.

2. REFERENCE STANDARD INSTRUMENTS :-


INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH TC TYPE K	HYDRA 2635A	6849323	25T5342	18-Jun-26

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO., LTD.

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

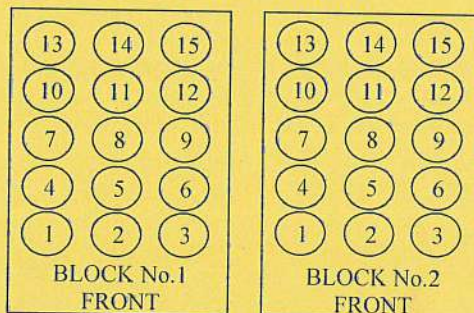

TEMPERATURE MEASUREMENT ACCURACY TEST

Block No.	1	2
Controller temperature (°C)	144	145
Indicating Temperature	144	145
Measured Temperature (°C) at Spread Locations	1	149.3
	2	149.1
	3	149.9
	4	149.6
	5	149.3
	6	149.5
	7	149.1
	8	149.7
	9	149.7
	10	149.5
	11	149.9
	12	149.4
	13	150.2
	14	149.4
	15	149.6
Uncertainty of Measurement(± °C)	0.89	0.89

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2 : LOCATION 10 WAS REFERENCE LOCATION.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k =2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



CERT.No.: HS-W015C

Calibration Date : 18 Mar 25
 Submitted by : S.P.S CONSULTING SERVICE CO.,LTD
 7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol,
 Chatuchak, Bangkok, Thailand 10900

Avg Room Temp : 20 °C
 Avg Water Temp : 20 °C
 Air Pressure : 760.00 mmHg
 Salinity : 0 ppt

Model : YSI 5000
 S/N : 15B100751
 Probe : YSI 5010
 S/N : 22D100097
 ID NO. : -
 Air Temp ref : S/N. F8065C26
 Barometric ref : S/N. F8065C26
 Water Temp ref : -
 ID NO. HS001
 Technician : Kittipong M.

Calibration Details

Calibration Point	100% air sat. (@20 °C, DO = 9.09 mg/l)	(status)	(status)
Measurement 1 (mg/l)	9.08	(PASS)	-
Measurement 2 (mg/l)	9.08	(PASS)	-
Measurement 3 (mg/l)	9.08	(PASS)	-
Measurement 4 (mg/l)	9.07	(PASS)	-
Measurement 5 (mg/l)	9.07	(PASS)	-
Measurement 6 (mg/l)	9.07	(PASS)	-
Measurement 7 (mg/l)	9.07	(PASS)	-
Measurement 8 (mg/l)	9.07	(PASS)	-
Measurement 9 (mg/l)	9.07	(PASS)	-
Measurement 10 (mg/l)	9.07	(PASS)	-

Mean Measurement	9.07	mg/l	-	-
Inaccuracy	0.02	mg/l	-	-

Overall Status (PASS)

Manufacturer Specification

Accuracy = +/- 0.02 mg/l

- 1) This certificate is issued based on the result that are found as shown on date and place of test only.
- 2) The calibration procedure followed in accordance with Harikul Science Co., Ltd.
- 3) This result shall not be used for advertising purpose.



Technician Signature
 (Kittipong Maekwong)



Laboratory Manager
 (Natenapha Pisatkunchon)

CERT.No.: HS-X014C

Certificate of Calibration

Calibration Date : 16 March 2026

Submitted by : S.P.S CONSULTING SERVICE CO.,LTD

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol,

Chatuchak, Bangkok, Thailand 10900

Avg Room Temp : 20 °C

Avg Water Temp : 20 °C

Air Pressure : 760.00 mmHg

Salinity : 0 ppt

Model : YSI 5000

S/N : 15B100751

Probe : YSI 5010

S/N : 22D100097

ID NO. :

Air Temp ref : S/N. F8065C26

Barometric ref : S/N. F8065C26

Water Temp ref : -

ID NO. HS001

Technician : Kittipong M.

Calibration Details

Calibration Point	100% air sat. (@20 °C, DO = 9.09 mg/l)	(status)	(status)
Measurement 1 (mg/l)	9.09	(PASS)	-
Measurement 2 (mg/l)	9.09	(PASS)	-
Measurement 3 (mg/l)	9.09	(PASS)	-
Measurement 4 (mg/l)	9.09	(PASS)	-
Measurement 5 (mg/l)	9.09	(PASS)	-
Measurement 6 (mg/l)	9.08	(PASS)	-
Measurement 7 (mg/l)	9.08	(PASS)	-
Measurement 8 (mg/l)	9.08	(PASS)	-
Measurement 9 (mg/l)	9.08	(PASS)	-
Measurement 10 (mg/l)	9.08	(PASS)	-

Mean Measurement	9.09	mg/l	-	-
Inaccuracy	0.00	mg/l	-	-

Overall Status (PASS)

Manufacturer Specification

Accuracy = +/- 0.02 mg/l

- 1) This certificate is issued based on the result that are found as shown on date and place of test only.
- 2) The calibration procedure followed in accordance with Harikul Science Co., Ltd.
- 3) This result shall not be used for advertising purpose.



Technician Signature

(Kittipong Maekwong)



Laboratory Manager

(Natenapha Pisatkunchon)

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN
associates



Cert. No. : SP25026

Pages : 1 of 4

Calibration Certificate

Equipment : UV-VIS SPECTROPHOTOMETER
Manufacturer : PERKINELMER
Model : LAMBDA 25
Serial No.: 501S14123010
ID No.: SP03/58
Calibration Mode : WAVELENGTH ACCURACY
PHOTOMETRIC ACCURACY
STRAY LIGHT

Condition As Found : GOOD

Customer : S.P.S CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN ROAD,
CHOMPHON SUB-DISTRICT, CHATUCHAK DISTRICT,
BANGKOK PROVINCE 10900 THAILAND.

Location : ORGANIC LABORATORY IV

Ambient Temperature : (22.9 $\pm$ 5) °C
Relative Humidity : (53.7 $\pm$ 25) %

Received Date : 22 AUGUST 2025
Calibration Date : 22 AUGUST 2025
Date of Issue : 25 AUGUST 2025

Calibrated by :

Nitinun Srihawan

Approved by :

Wichok B.
(Wichok Ekpongpradit)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : SP25026

Job No. : VC68SP0019

Pages : 2 of 4

Calibration Method :

This instrument was calibrated by using on-site calibration procedure In-house method : CP-SP-01

The calibration procedure to direct measurement wavelength accuracy by using wavelength standard solution, Photometric accuracy by using absorbance standard filter and absorbance standard solution

The calibration procedure used was based on ASTM E275-01, ASTM E925-02

Condition of this result of calibration :

1. Certified reference materials

<u>Material</u>	<u>Ref. type</u>	<u>Cell serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Holmium liquid	RM-HL	29706	126461	24/10/2026
Didymium liquid	RM-DL	28912	126462	24/10/2026
Neutral density filter	RM-1N2N3N	13877	126457	24/10/2026
Potassium dichromate solutions	RM-0204060810	14204	126497	25/10/2026
Potassium Iodide solution	-	KI-0701-001	CI-0185-24	14/05/2026

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 The UK National Physical Laboratory (NPL)

Result of calibration : Wavelength Accuracy

(Without adjustment)

Material	Certified Values of Reference Material (nm)	UUC* Reading (nm)	Error (nm)	Uncertainty ± (nm)	k Factor
RM-HL	278.13	278.21	0.08	0.16	2.00
	361.25	361.39	0.14	0.16	2.00
	467.82	467.71	-0.11	0.16	2.00
	536.56	536.50	-0.06	0.16	2.00
	640.50	640.36	-0.14	0.16	2.00
RM-DL	740.09	739.85	-0.24	0.16	2.00
	864.94	865.12	0.18	0.16	2.00

UUC* = Unit Under Calibration

Cert. No. : SP25026

Job No. : VC68SP0019

Pages : 3 of 4

Result of calibration : Photometric Accuracy

Material	Wavelength (nm)	Filter S/N	Nominal Absorbance (A)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor
Neutral Density glass filter	440.0	29381	0.5	0.5443	0.5413	-0.0030	0.0043	2.00
		29914	0.7	0.7484	0.7455	-0.0029	0.0054	2.00
		29360	1.0	1.0527	1.0535	0.0008	0.0032	2.00
	465.0	29381	0.5	0.4948	0.4922	-0.0026	0.0041	2.00
		29914	0.7	0.6906	0.6877	-0.0029	0.0050	2.00
		29360	1.0	0.9695	0.9709	0.0014	0.0031	2.00
	546.1	29381	0.5	0.5090	0.5068	-0.0022	0.0036	2.00
		29914	0.7	0.6985	0.6960	-0.0025	0.0041	2.00
		29360	1.0	0.9814	0.9825	0.0011	0.0031	2.00
	590.0	29381	0.5	0.5375	0.5353	-0.0022	0.0034	2.00
		29914	0.7	0.7256	0.7231	-0.0025	0.0037	2.00
		29360	1.0	1.0213	1.0219	0.0006	0.0032	2.00
	635.0	29381	0.5	0.5223	0.5202	-0.0021	0.0033	2.00
		29914	0.7	0.6927	0.6901	-0.0026	0.0036	2.00
		29360	1.0	0.9744	0.9750	0.0006	0.0032	2.00

UUC* = Unit Under Calibration

Cert. No. : SP25026

Job No. : VC68SP0019

Pages : 4 of 4

Result of calibration : Photometric Accuracy

(Without adjustment)

Material	Wavelength (nm)	Solution (mg/l)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor
Potassium dichromate solutions	235.0	20	0.2415	0.2443	0.0028	0.0101	2.00
		40	0.4866	0.4871	0.0005	0.0115	2.00
		60	0.7415	0.7295	-0.0120	0.0067	2.00
		80	0.9854	0.9844	-0.0010	0.0071	2.00
		100	1.2444	1.2425	-0.0019	0.0073	2.00

UUC* = Unit Under Calibration

Condition of this result of calibration : Spectrophotometer PERKINELMER Model LAMBDA 25 S/N 501S14123010

Resolution of Wavelength Mode 0.1 nm

Resolution of Photometric Mode 0.001 A

Parameter Setting

Measurement Mode Wavelength, Absorbance

Wavelength Scan 190 nm - 1100 nm

Scanning Speed 7.5 nm/min

Band width(Wavelength) 1.0

Band width(Vis) 1.0

Band width(Uv) 1.0

Stray Light** UUC* Reading at 220.0 nm	
Transimission T(%)	Absorbance(A)
0.020	3.7032

**Specific Acceptance :

Transmission ≤ 1.0 T(%), Absorbance ≥ 2.0 A

**Stray light not TISI Accredited

The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95%

End of Calibration Certificate

ลำดับที่ 5

คุณภาพอากาศในสถานประกอบการ



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Environmental Conditions

Temperature : 25 ± 3 °C
Pressure : 1010 ± 15 mmbar

Personal Pump Data					Calibration Data							
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)			y	R ²
					1	2	3	1	2	3		
B01	SKC	224-PCXR4	262101	05/01/2026	1,000	1,500	2,000	1,004	1,501	2,003	1.010x - 18.941	0.999
B02	SKC	224-PCXR4	626166	05/01/2026	1,000	1,500	2,000	1,000	1,500	2,002	1.012x - 23.432	0.999
B03	SKC	224-PCXR4	612968	05/01/2026	1,000	1,500	2,000	993	1,503	2,001	1.008x - 15.587	1.000
B04	SKC	224-PCXR4	602804	06/01/2026	1,000	1,500	2,000	1,001	1,498	1,996	0.997x + 2.672	1.000
B05	SKC	224-PCXR4	612693	07/01/2026	1,000	1,500	2,000	999	1,494	1,993	0.995x + 1.555	1.000
B06	SKC	224-PCXR4	262188	06/01/2026	1,000	1,500	2,000	1,002	1,501	2,004	1.007x - 12.528	1.000
B07	SKC	224-PCXR4	626262	06/01/2026	1,000	1,500	2,000	1,003	1,501	2,002	1.010x - 19.021	0.999
B08	SKC	224-PCXR4	626100	06/01/2026	1,000	1,500	2,000	1,005	1,500	2,006	1.006x - 8.619	1.000
B09	SKC	224-PCXR4	626479	05/01/2026	1,000	1,500	2,000	1,001	1,500	2,000	1.007x - 14.458	1.000
B10	SKC	224-PCXR4	091950	05/01/2026	1,000	1,500	2,000	998	1,503	2,000	1.001x - 5.945	1.000
B11	SKC	224-PCXR8	564315	05/01/2026	1,000	1,500	2,000	993	1,494	1,993	1.010x - 25.765	0.999
B12	SKC	224-PCXR4	034656	05/01/2026	1,000	1,500	2,000	995	1,497	1,998	0.996x - 4.790	0.999
B13	SKC	224-PCXR4	602073	05/01/2026	1,000	1,500	2,000	994	1,499	1,975	0.990x + 6.525	0.999
B14	SKC	224-PCXR4	626313	05/01/2026	1,000	1,500	2,000	993	1,499	1,994	1.001x - 7.291	1.000
B15	SKC	224-PCXR4	626474	05/01/2026	1,000	1,500	2,000	992	1,505	2,002	1.012x - 23.464	1.000
B16	SKC	224-PCXR4	626477	06/01/2026	1,000	1,500	2,000	993	1,496	1,991	0.996x + 0.945	1.000
B17	SKC	224-PCXR4	626860	06/01/2026	1,000	1,500	2,000	1,000	1,500	2,001	1.007x - 14.414	1.000
B18	SKC	224-PCXR4	691484	05/01/2026	1,000	1,500	2,000	994	1,502	2,002	1.015x - 30.763	0.999
B19	SKC	224-PCXR4	691599	05/01/2026	1,000	1,500	2,000	993	1,490	1,999	1.006x - 14.713	1.000
B20	SKC	224-PCXR4	691587	05/01/2026	1,000	1,500	2,000	991	1,500	1,997	1.005x - 13.565	1.000
B21	SKC	224-PCXR4	691531	05/01/2026	1,000	1,500	2,000	1,002	1,500	2,000	1.002x - 6.050	1.000
B22	SKC	224-PCXR4	691654	05/01/2026	1,000	1,500	2,000	1,008	1,498	1,995	1.000x - 6.158	0.999
B23	SKC	224-PCXR4	798393	06/01/2026	1,000	1,500	2,000	992	1,498	1,972	0.990x + 3.813	0.999
B24	SKC	224-PCXR4	626363	06/01/2026	1,000	1,500	2,000	1,003	1,493	2,002	1.001x - 5.201	1.000
B25	SKC	224-PCXR4	798489	06/01/2026	1,000	1,500	2,000	993	1,496	1,995	1.003x - 10.857	1.000
B26	SKC	224-PCXR4	798479	06/01/2026	1,000	1,500	2,000	994	1,505	2,002	1.012x - 23.253	1.000
B27	SKC	224-PCXR4	691673	06/01/2026	1,000	1,500	2,000	996	1,506	1,989	0.994x + 5.799	1.000
B28	SKC	224-PCXR4	691570	06/01/2026	1,000	1,500	2,000	995	1,502	1,998	0.999x - 5.193	1.000
B29	SKC	224-PCXR4	626472	05/01/2026	1,000	1,500	2,000	995	1,491	1,993	0.999x - 4.662	1.000
B30	SKC	224-PCXR4	691489	05/01/2026	1,000	1,500	2,000	1,003	1,500	1,998	1.002x - 6.804	1.000
B31	SKC	224-PCXR4	691509	05/01/2026	1,000	1,500	2,000	993	1,500	1,997	0.992x + 4.256	1.000
B32	SKC	224-PCXR4	091567	05/01/2026	1,000	1,500	2,000	994	1,487	1,972	0.990x - 2.389	0.999
B33	SKC	224-PCXR4	091756	05/01/2026	1,000	1,500	2,000	993	1,496	1,998	1.013x - 28.816	0.999
B34	SKC	224-PCXR4	612962	05/01/2026	1,000	1,500	2,000	994	1,502	2,003	1.011x - 21.717	1.000
B35	SKC	224-PCXR4	602682	06/01/2026	1,000	1,500	2,000	998	1,493	2,000	1.001x - 2.561	1.000
B36	SKC	224-PCXR4	626164	06/01/2026	1,000	1,500	2,000	993	1,497	1,994	1.003x - 8.755	1.000
B37	SKC	224-PCXR4	626256	06/01/2026	1,000	1,500	2,000	993	1,508	2,007	1.009x - 10.996	1.000
B38	SKC	224-PCXR4	626167	06/01/2026	1,000	1,500	2,000	993	1,502	2,000	1.013x - 28.162	0.999
B39	SKC	224-PCXR4	034637	06/01/2026	1,000	1,500	2,000	1,000	1,497	1,993	0.991x + 9.544	1.000
B40	SKC	224-PCXR4	798349	06/01/2026	1,000	1,500	2,000	1,000	1,499	1,994	0.998x - 0.160	1.000

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

Peera Detudom
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chafuchak, Bangkok 10900

Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com., www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136833

Environmental Conditions

Temperature 25 ± 3 °C
Pressure 1010 ± 15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R ²
R01	SKC	224-PCXR4	602467	05/01/2026	1,000	1,500	2,000	999	1,505	2,009	1.011x - 15.308	1.000
R02	SKC	224-PCXR4	626450	05/01/2026	1,000	2,000	3,000	1,001	1,505	2,005	1.005x - 5.625	1.000
R03	SKC	224-PCXR4	691592	05/01/2026	1,000	1,500	2,000	998	1,499	2,010	1.009x - 11.382	1.000
R04	SKC	224-PCXR4	691672	05/01/2026	1,000	1,500	2,000	999	1,496	2,000	0.992x + 5.045	0.999
R05	SKC	224-PCXR4	798470	06/01/2026	1,000	1,500	2,000	997	1,480	1,991	0.995x - 8.487	0.999
R06	SKC	224-PCXR4	798456	06/01/2026	1,000	1,500	2,000	1,000	1,502	1,992	0.993x + 2.874	0.999
R07	SKC	224-PCXR4	798480	06/01/2026	1,000	1,500	2,000	1,000	1,508	2,000	1.000x + 1.559	1.000
R08	SKC	224-PCXR4	883215	07/01/2026	1,000	1,500	2,000	1,001	1,500	2,000	1.004x - 8.216	1.000
R09	SKC	224-PCXR4	034650	05/01/2026	1,000	1,500	2,000	999	1,509	2,005	1.005x - 6.025	1.000
R10	SKC	224-PCXR4	091765	05/01/2026	1,000	1,500	2,000	1,001	1,509	2,008	1.007x - 8.311	1.000
R11	SKC	224-PCXR4	091763	05/01/2026	1,000	1,500	2,000	999	1,502	1,995	1.002x - 10.594	0.999
R12	SKC	224-PCXR4	091568	06/01/2026	1,000	1,500	2,000	999	1,495	1,994	0.994x - 1.683	0.999
R13	SKC	224-PCXR4	091638	06/01/2026	1,000	1,500	2,000	999	1,499	1,994	0.998x - 7.136	0.999
R14	SKC	224-PCXR4	091764	06/01/2026	1,000	1,500	2,000	1,004	1,507	2,006	1.007x - 8.975	1.000
R15	SKC	224-PCXR8	529457	06/01/2026	1,000	1,500	2,000	1,004	1,502	2,002	0.999x + 1.731	1.000
R16	SKC	224-PCXR8	529643	05/01/2026	1,000	1,500	2,000	1,001	1,511	2,010	1.010x - 13.433	1.000
R17	SKC	224-PCXR8	529645	06/01/2026	1,000	1,500	2,000	1,004	1,502	2,003	0.998x + 4.238	1.000
R18	SKC	224-PCXR8	566756	05/01/2026	1,000	1,500	2,000	1,003	1,504	2,006	1.004x - 3.774	1.000
R19	SKC	224-PCXR8	566802	05/01/2026	1,000	1,500	2,000	1,003	1,498	1,995	1.001x - 8.224	0.999
R20	SKC	224-PCXR8	529089	06/01/2026	1,000	1,500	2,000	997	1,509	1,985	0.994x + 5.269	0.999
R21	SKC	224-PCXR8	665728	06/01/2026	1,000	1,500	2,000	1,000	1,510	1,995	0.998x - 1.139	0.999
R22	SKC	224-PCXR8	707444	05/01/2026	1,000	1,500	2,000	1,004	1,507	2,008	1.004x - 5.709	1.000
R23	SKC	224-PCXR8	761067	05/01/2026	1,000	1,500	2,000	1,009	1,504	2,006	1.000x + 1.179	1.000
R24	SKC	224-PCXR8	707893	05/01/2026	1,000	1,500	2,000	999	1,497	1,992	0.998x - 8.383	0.999
R25	SKC	224-PCXR8	761052	06/01/2026	1,000	1,500	2,000	998	1,503	1,975	0.984x + 17.071	0.999
R26	SKC	224-PCXR8	707956	05/01/2026	1,000	1,500	2,000	997	1,492	1,992	0.991x + 0.388	1.000
R27	SKC	224-PCXR8	707398	05/01/2026	1,000	1,500	2,000	1,000	1,495	2,002	1.002x - 3.898	1.000
R28	SKC	224-PCXR8	707481	06/01/2026	1,000	1,500	2,000	1,009	1,503	2,008	0.996x + 8.659	1.000
R29	SKC	224-PCXR8	707402	07/01/2026	1,000	1,500	2,000	1,006	1,513	2,009	1.002x - 1.219	0.999
R30	SKC	224-PCXR8	093811	07/01/2026	1,000	1,500	2,000	1,001	1,513	2,008	1.008x - 9.239	1.000
R31	SKC	224-PCXR8	093183	06/01/2026	1,000	1,500	2,000	1,010	1,507	2,013	1.003x - 0.780	1.000
R32	SKC	224-PCXR8	671950	06/01/2026	1,000	1,500	2,000	999	1,498	1,999	1.000x + 0.668	1.000
R33	SKC	224-PCXR4	626254	06/01/2026	1,000	1,500	2,000	1,000	1,508	2,007	1.004x - 5.149	1.000
R34	SKC	224-PCXR4	626131	05/01/2026	1,000	1,500	2,000	996	1,498	2,003	1.010x - 18.178	1.000
R35	SKC	224-PCXR8	707460	05/01/2026	1,000	1,500	2,000	1,006	1,496	2,004	0.999x + 0.388	1.000
R36	SKC	224-PCXR8	707446	05/01/2026	1,000	1,500	2,000	1,006	1,504	2,008	1.005x - 6.281	1.000
R37	SKC	224-PCXR8	707432	06/01/2026	1,000	1,500	2,000	1,003	1,505	2,004	1.004x - 5.005	1.000
R38	SKC	224-PCXR8	707349	06/01/2026	1,000	1,500	2,000	998	1,498	1,997	0.999x - 1.655	1.000
R39	SKC	224-PCXR8	761095	06/01/2026	1,000	1,500	2,000	1,000	1,497	2,003	1.005x - 8.068	1.000

Calibrated by :

Adul Dangklorn
(Mr. Adul Dangklorn)

Approved by :

Peera Detodom
(Mr. Peera Detodom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136833

Environmental Conditions

Temperature : 25 $\pm$ 3 $^{\circ}$ C
Pressure : 1010 $\pm$ 15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (mL/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R ²
R40	SKC	224-PCXR4	612753	05/01/2026	1,000	1,500	2,000	997	1,506	1,998	1.000x - 0.556	1.000
R41	SKC	224-PCXR4	626140	05/01/2026	1,000	1,500	2,000	995	1,504	1,992	0.996x - 3.574	0.999
R42	SKC	224-PCXR4	626463	05/01/2026	1,000	1,500	2,000	1,006	1,505	1,984	0.988x + 15.108	0.999
R43	SKC	224-PCXR4	626129	05/01/2026	1,000	1,500	2,000	993	1,504	1,972	0.982x + 17.902	0.999
R44	SKC	224-PCXR4	602753	06/01/2026	1,000	1,500	2,000	1,001	1,495	2,000	1.001x - 3.434	1.000
R45	SKC	224-PCXR4	626137	06/01/2026	1,000	1,500	2,000	998	1,494	1,997	0.996x + 1.827	1.000

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

Peera Detudom
(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Rotameter Calibration Report (For Personal Pump High Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136833


Calibration Data

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (mL/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R ²
H-R01	Dwyer	VFB-65	05/01/2026	500	1,000	2,000	503.6	992.4	1980.9	0.999x - 3.140	0.999
H-R02	Dwyer	VFB-65	06/01/2026	500	1,000	2,000	500.8	995.8	1986.2	1.002x - 5.343	1.000
H-R03	Dwyer	VFB-65	05/01/2026	500	1,000	2,000	495.3	992.1	1982.9	1.004x - 17.510	0.999
H-R04	Dwyer	VFB-65	05/01/2026	500	1,000	2,000	496.4	994.6	2019.5	1.007x - 11.385	1.000
H-R05	Dwyer	VFB-65	06/01/2026	500	1,000	2,000	497.2	991.5	1987.3	1.003x - 7.563	1.000
H-R06	Dwyer	VFB-65	06/01/2026	500	1,000	2,000	501.1	992.4	1982.9	1.001x - 6.139	0.999

Calibrated by :

Adul Dangklom
(Mr. Adul Dangklom)

Approved by :

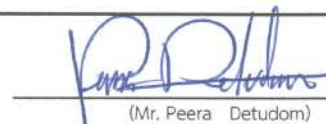
(Mr. Peera Detudom)



CERTIFICATE No : 25M2254

REFERENCE No : 76365-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE

MANUFACTURER : METTLER TOLEDO

MODEL : XS105DU

SERIAL No : 1126422905

ID No : BA05/50

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.

CALIBRATION DATE : 07-Mar-25

APPROVED BY : 
PONGSAK J.

ISSUED DATE : 13-Mar-25

RECEIVED DATE : 07-Mar-25

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.





CERTIFICATE No : 25M2254

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : XS105DU
MANUFACTURER : METTLER TOLEDO S/N : 1126422905
ID No : BA05/50 RECEIVED DATE : 07-Mar-25
AIR PRESSURE : 1009mbar $\pm$ 1mbar CALIBRATION DATE : 07-Mar-25
AMBIENT TEMPERATURE : 24°C $\pm$ 1°C RELATIVE HUMIDITY : 54 %RH $\pm$ 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	C02250116	28-Jan-27
2) STANDARD WEIGHT	E2	15843	C02250117	29-Jan-27

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 120 g WAS 0.000055 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ($\pm$ g)
0.00	0.00000	0.00000	0.000065
0.02	0.01999	0.00001	0.000065
0.10	0.10001	-0.00001	0.000066
0.20	0.20001	-0.00001	0.000066
0.50	0.50002	-0.00002	0.000065
1.00	1.00003	-0.00003	0.000066
2.00	2.00001	-0.00001	0.000067
5.00	5.00002	-0.00002	0.000068
10.00	10.00000	0.00000	0.000070
20.00	20.00004	-0.00004	0.000078
50.00	50.00000	0.00000	0.00013
100.00	100.0001	-0.0001	0.00019
120.00	120.0002	-0.0002	0.00022

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.0000
2	50.0000
3	50.0000
4	50.0000
5	50.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



ลำดับที่ 6

ระดับเสียงในสถานประกอบการ



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-69/0204

MTC No. EEL. BP. 152/0169

CALIBRATION CERTIFICATE

Submitted by : S.P.S.CONSULTING SERVICE CO.,LTD.

Address : 7 Soi Phaholyothin 24, Phaholyothin Road, Jompol, Chatuchak, Bangkok 10900.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Sound Calibrator

Manufacturer : ACO

Model : 2127

Serial No. : 130006

Ambient Environment

Temperature : $(23 \pm 3) ^\circ\text{C}$

Relative Humidity : $(50 \pm 15) \%$

Ambient Pressure : $(101.325 \pm 1.500) \text{ kPa}$

- Standards used :**
1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.
 2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.
 3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.
 4. Digital Multimeter Agilent 34401A S/N MY44005560.
 5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.
 6. Audio Analyzer Keithley 2015-P S/N 4106495.
 7. Condenser Microphone Bruel&Kjaer 4180 S/N 2889871.

Calibration Procedure: CP-102-04 based on IEC 60942-2003; The sound pressure level generated by sound calibrator under test shall be measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 29 Jan. 2026

Date of Calibration : 11 Feb. 2026

1 / 2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory

668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office

196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-69/0204

MTC No. EEL. BP. 152/0169

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20 μ Pa at 1000 Hz

Acoustic Output in dB re 20 μ Pa, Corrected to Reference Conditions: 101.325 kPa, 23.0 °C and 50 %RH.

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	93.89	-0.11	± 0.10	± 0.40 dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	999.9	-0.1	± 1.5	$\pm 1.0\%$

3. Total Distortion

Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	1.90	± 0.50	$\pm 3.0\%$

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Calibrated by :


(Mr. Weerachai Deechaiyae)

Approved by :


(Mr. Prawate Kluaypa)
Director

Electrical and Electronic Standards Laboratory
Industrial Metrology and Testing Service Centre

Date of Calibration : 11 Feb. 2026

Date of Issue : 12 Feb. 2026

Ref : 2011269012900497001

End of Certificate

2 / 2

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory

668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office

196 Phahonyothin Road, Ladyao, Chatuchak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Noise R_105/26

Sound Level Meter Calibration Report

Acoustic Calibrator Data

Brand	ACO	Number	AC 03/56
Model	2127	Serial No.	130006
Calibration Range	94 dB, 1000 Hz	Last Calibration	11 February 2026
		Due Date	11 February 2027

Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-R41	ACO	6236	00192053	25 February 2026	93.9	93.9
ACO-R50	ACO	6236	00192062	25 February 2026	93.9	93.9
ACO-R51	ACO	6236	00192063	25 February 2026	93.9	93.9
ACO-R52	ACO	6236	00192064	25 February 2026	93.9	93.9
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.81 ± 0.10 dB	

Calibrated by :

Heeson L.

(Mr. Heeson Lormae)

Approved by :

Yutthana I.

(Mr. Yutthana Tanatharanit)

ลำดับที่ 7

ระดับเสียงที่ลูกจ้างได้รับเฉลี่ยตลอดระยะเวลาในแต่ละวัน



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0514

MTC No. EEL. BP. 34/0868

CALIBRATION CERTIFICATE

Submitted by : S.P.S.Consulting Service Co.,Ltd.

Address : 7 Soi Phaholyothin 24, Phaholyothin Road, Jompol, Chatuchak, Bangkok 10900.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
: Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Sound Calibrator

Manufacturer : SVANTEK

Model : SV34

Serial No. : 83820

Ambient Environment

Temperature : $(23 \pm 3) ^\circ\text{C}$

Relative Humidity : $(50 \pm 15) \%$

Ambient Pressure : $(101.325 \pm 1.500) \text{ kPa}$

Standards used : 1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.
2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.
3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.
4. Digital Multimeter Agilent 34401A S/N MY44005560.
5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.
6. Audio Analyzer Panasonic VP-7722A S/N 041477D122.
7. Condenser Microphone B&K 4180 S/N 2633526.

Calibration Procedure: CP-102-04 based on IEC 60942-2003; The sound pressure level generated by sound calibrator under test shall be measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 14 Aug. 2025

Date of Calibration : 22 Aug. 2025

1 / 2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory

668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office

196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-68/0514

MTC No. EEL. BP. 34/0868

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 114 dB re 20 μ Pa at 1000 Hz

Acoustic Output in dB re 20 μ Pa, Corrected to Reference Conditions: 101.325 kPa, 23.0 °C and 50 %RH.

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	114.02	0.02	± 0.10	± 0.75 dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	1000.0	0.0	± 1.5	$\pm 2.0\%$

3. Total Distortion

Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	0.21	± 0.50	$\pm 4.0\%$

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Calibrated by :


(Mr. Weerachai Deechaiyae)

Approved by :


(Mr. Prawate Kluaypa)



Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 22 Aug. 2025

Date of Issue : 25 Aug. 2025

Ref : 2011268081403169011

End of Certificate

2 / 2

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory

668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office

196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Noise Dose R_106/26

Noise Dose Meter Calibration Report

Acoustic Calibrator Data

Brand	SVANTEK	Number	SV 03/60
Model	SV34	Serial No.	83820
Calibration Range	114 dB, 1000 Hz	Last Calibration	25 August 2025
		Due Date	25 August 2026

Calibration Data

Sound Level Meter Data

Calibration Data

SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
NMD-B14	SVANTEK	SV-104IS	80875	25 February 2026	114.0	114.0
NMD-B15	SVANTEK	SV-104IS	80880	25 February 2026	114.0	114.0
NMD-B16	SVANTEK	SV-104IS	106120	25 February 2026	114.0	114.0
NMD-B17	SVANTEK	SV-104IS	106122	25 February 2026	114.0	114.0
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					114.02± 0.10 dB	

Calibrated by :

Heeson L.

(Mr. Heeson Lormae)

Approved by :

Yutthana J.

(Mr. Yutthana Tanatharanit)

ลำดับที่ 8

ระดับความร้อนในสถานประกอบการ



Certificate of Calibration

Certificate Number : SPR25100063-4

Page : 1 of 3

Customer : S.P.S. CONSULTING SERVICE CO., LTD.

7 Soi Phaholyothin 24 Phaholyothin Road., Jompol, Chatuchak,
Bangkok 10900

Equipment Name : Area Heat Stress Monitor

Manufacturer : Quest Technologies

Model : QUESTemp 34

Serial Number : TEN040005

ID. Number : R04

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 2^{\circ}\text{C}$

Relative Humidity : $50\% \pm 15\%$

Location of Calibration : In-Lab

Calibration Procedure : SP-CPT-04-13

Received Date : 06 Oct 2025

Calibration Date : 08 Oct 2025

Recommend Due Date : 08 Oct 2026

Date of Issue : 09 Oct 2025

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr. Navaporn Uengseng

Approved by

Calibration Officer



(Mr. Pootthipong A.)

Authorized Signatory

SP-FM-04-15 rev.0



Calibration Report

Certificate Number : SPR25100063-4

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
THERMO-HYGROMETER	5020A	A47046	TMU2500342	29 Jan 2026
Temp & Humidity Test Chamber	TEMI1500-01/SD/N/N/	S7110ZL742 1014	SPR25040010-13	20 Apr 2026

Traceability

This certification is traceable to the International System of Unit maintained at :

NA - NA Caltechnologies Co., Ltd.

SP Metrology - SP Metrology system (Thailand) Co.Ltd.



Result of Calibration

Certificate Number : SPR25100063-4

Page : 3 of 3

Temperature Accuracy in the Measurement. (WET)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.014	29.8	-0.214	0.20
35.0	35.012	34.8	-0.212	0.20
40.0	40.018	39.8	-0.218	0.20

Temperature Accuracy in the Measurement. (DRY)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.014	29.7	-0.314	0.20
35.0	35.012	34.7	-0.312	0.20
40.0	40.018	39.7	-0.318	0.20

Temperature Accuracy in the Measurement. (GLOVE)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.014	29.8	-0.214	0.20
35.0	35.012	34.8	-0.212	0.20
40.0	40.018	39.8	-0.218	0.20

Note :

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2$, providing a level of confidence approximately 95%.

- End of Certificate -



Certificate of Calibration

Certificate Number : SPR25100063-9

Page : 1 of 3

Customer : S.P.S. CONSULTING SERVICE CO., LTD.

7 Soi Phaholyothin 24 Phaholyothin Road., Jompol, Chatuchak,
Bangkok 10900

Equipment Name : Area Heat Stress Monitor

Manufacturer : Quest Technologies

Model : QUESTemp 34

Serial Number : TEH060047

ID. Number : B05

Environmental Conditions

Ambient Temperature : $23\text{ }^{\circ}\text{C} \pm 2\text{ }^{\circ}\text{C}$

Relative Humidity : $50\% \pm 15\%$

Location of Calibration : In-Lab

Calibration Procedure : SP-CPT-04-13

Received Date : 06 Oct 2025

Calibration Date : 29 Oct 2025

Recommend Due Date : 29 Oct 2026

Date of Issue : 30 Oct 2025

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr. Surasak Ritthikaew

Calibration Officer

Approved by



(Mr. Worapong Sinthusopa)

Authorized Signatory



Calibration Report

Certificate Number : SPR25100063-9

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
THERMO-HYGROMETER	5020A	A47046	TMU2500342	29 Jan 2026
Temp & Humidity Test Chamber	TEMI1500-01/SD/N/N/	S7110ZL742 1014	SPR25040010-13	20 Apr 2026

Traceability

This certification is traceable to the International System of Unit maintained at :

NA - NA Caltechnologies Co., Ltd.

SP Metrology - SP Metrology system (Thailand) Co.Ltd.



Result of Calibration

Certificate Number : SPR25100063-9

Page : 3 of 3

Temperature Accuracy in the Measurement. (WET)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.018	30.1	0.082	0.20
35.0	35.014	35.1	0.086	0.20
40.0	40.011	40.1	0.089	0.21

Temperature Accuracy in the Measurement. (DRY)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.021	30.1	0.079	0.20
35.0	35.015	35.0	-0.015	0.20
40.0	40.010	40.0	-0.010	0.21

Temperature Accuracy in the Measurement. (GLOVE)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.022	30.1	0.078	0.20
35.0	35.018	35.1	0.082	0.20
40.0	40.013	40.1	0.087	0.21

Note :

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2$, providing a level of confidence approximately 95%.

- End of Certificate -



Certificate of Calibration

Certificate Number : SPR26010387-2

Page : 1 of 3

Customer : S.P.S. CONSULTING SERVICE CO., LTD.

7 Soi Phaholyothin 24 Phaholyothin Road., Jompol, Chatuchak,
Bangkok 10900

Equipment Name : Area Heat Stress Monitor

Manufacturer : Metrosonics

Model : hs-32

Serial Number : MCD070035

ID. Number : R05

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 2^{\circ}\text{C}$

Relative Humidity : $50\% \pm 15\%$

Location of Calibration : In-Lab

Calibration Procedure : SP-CPT-04-13

Received Date : 30 Jan 2026

Calibration Date : 03 Feb 2026

Recommend Due Date : 03 Feb 2027

Date of Issue : 04 Feb 2026

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr. Jirasak Pumbut

Calibration Officer

Approved by



(Mr. Worapong Sinthusopa)

Authorized Signatory



Calibration Report

Certificate Number : SPR26010387-2

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
THERMO-HYGROMETER	5020A	A47046	TMU2500342	29 Jan 2027
Temp & Humidity Test Chamber	TEMI1500-01/SD/N/N/	S7110ZL742 1014	SPR25040010-13	20 Apr 2026

Traceability

This certification is traceable to the International System of Unit maintained at :

NA - NA Caltechnologies Co., Ltd.

SP Metrology - SP Metrology system (Thailand) Co.Ltd.



Result of Calibration

Certificate Number : SPR26010387-2

Page : 3 of 3

Temperature Accuracy in the Measurement. (WET)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.009	29.7	-0.309	0.20
35.0	35.012	34.7	-0.312	0.20
40.0	40.017	39.7	-0.317	0.21

Temperature Accuracy in the Measurement. (DRY)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.009	29.7	-0.309	0.20
35.0	35.012	34.7	-0.312	0.20
40.0	40.017	39.7	-0.317	0.21

Temperature Accuracy in the Measurement. (GLOBE)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.009	29.7	-0.309	0.20
35.0	35.012	34.7	-0.312	0.20
40.0	40.017	39.7	-0.317	0.21

Note :

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2$, providing a level of confidence approximately 95%.

- End of Certificate -



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Heat R005

Heat Stress WBGT Meter Verification Report			
Verification Data			
Heat Stress WBGT Meter No.	: R04	Verification Date	: 25 February 2026
Brand	: Quest Technologies	Ambient Temp.	: 24.5 °C
Model	: QUESTemp 34	Barometric Pressure	: 1011 mmbar
Serial No.	: TEN040005	Relative Humidity	: 48 %
Verification Module (Electronic Sensor Check) :			
Verification Module No. : 21 WB = 12.5 °C, DB = 47.1 °C, G = 69.3 °C			
Result of Verification : Without Adjustment			
Wet Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
12.5	12.6	-0.1	± 0.5
Dry Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
47.1	47.2	-0.1	± 0.5
Globe Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
69.3	69.1	0.2	± 0.5
UUC* = UNIT UNDER CALIBRATION			

Verified by : Heeson L.
(Mr. Heeson Lormae)

Approved by : Yutthana J.
(Mr. Yutthana Tanatharanit)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com., www.spscon.com

Heat R005

Heat Stress WBGT Meter Verification Report			
Verification Data			
Heat Stress WBGT Meter No.	: R05	Verification Date	: 25 February 2026
Brand	: METROSONICS	Ambient Temp.	: 24.5 °C
Model	: hs-32	Barometric Pressure	: 1011 mmbar
Serial No.	: MCD070035	Relative Humidity	: 48 %
Verification Module (Electronic Sensor Check) :			
Verification Module No. : 21 WB = 12.5 °C, DB = 47.1 °C, G = 69.3 °C			
Result of Verification : Without Adjustment			
Wet Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
12.5	12.6	-0.1	± 0.5
Dry Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
47.1	47.3	-0.2	± 0.5
Globe Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
69.3	69.2	0.1	± 0.5
UUC* = UNIT UNDER CALIBRATION			

Verified by : Heeson L.
(Mr. Heeson Lormae)

Approved by : Yutthana S.
(Mr. Yutthana Tanatharanit)

