

เอกสารแนบ



เอกสารแนบ 4

เอกสารผลการตรวจวัดคุณภาพสิ่งแวดล้อม



ANALYSIS REPORT

CUSTOMER NAME : เดอะ วัลลีย์ เขาใหญ่
ADDRESS : เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เขาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.
SAMPLING LOCATION : ตั้งแยกจากของระบบบำบัดน้ำเสีย อาคาร A
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : เหลือง ชุ่น มีตะกอน มีกลิ่นเหม็นเล็กน้อย
SAMPLING DATE : JANUARY 28, 2026
SAMPLING TIME : 10:30
SAMPLING BY : นายพีรพล ถวิลพ่วง


REPORT NO. : RN260110119
SAMPLING SOURCE : WASTEWATER
RECEIVED DATE : JANUARY 28, 2026
ANALYTICAL DATE : JANUARY 28 - FEBRUARY 05, 2026
REPORT DATE : FEBRUARY 06, 2026

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
pH [#]	-	Electrometric (SM: 4500-H ⁺ B.)	7.1 at 25°C	-	-
Biochemical Oxygen Demand	mg/l	Azide Modification (SM: 4500-O C, 5210 B.)	48.0	2.0	-
Total Dissolved Solids [#]	mg/l	Total Dissolved Solids Dried at 180°C (SM: 2540 C.)	556.0	-	-
Total Suspended Solids [#]	mg/l	Total Suspended Solids Dried at 103-105°C (SM: 2540 D.)	41.0	-	-
Settleable Solids	ml/l	Settleable Solids (SM: 2540 F.)	<0.1	-	-
Sulfide as H ₂ S	mg/l	Iodometric (SM: 4500-S ²⁻ F.)	Not Detected	-	-
Total Kjeldahl Nitrogen	mg/l	Macro Kjeldahl (SM: 4500-N _{org} B)	27.0	-	-
Oil & Grease	mg/l	Liquid-Liquid Partition-Gravimetric (SM: 5520 B.)	3.8	1.4	-
Total Coliform Bacteria	MPN/100 ml	MPN Test	>2.4 x 10 ⁶	-	-
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	>2.4 x 10 ⁶	-	-

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED.,2023 (AWWA,APHA, WEF)

Remark : 1. * Notification of the Ministry of Natural Resources and Environment, dated June 28, B.E. 2567 (2024), which was published in the Royal Government Gazette, Vol. 141, Part 233D dated August 27, B.E. 2567 (2024) . (Category B)

2. [#] ISO/IEC 17025 ACCREDITED BY DEPARTMENT OF SCIENCE SERVICE (DSS)



(MR TAWATCHAI CHONGVUTICHA)

LABORATORY SUPERVISOR



ANALYSIS REPORT

CUSTOMER NAME : เดอะ วิลลีย์ เขาใหญ่
ADDRESS : เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เขาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.
SAMPLING LOCATION : บ่อพักน้ำแรกหลังจากการระบบบำบัดน้ำเสีย อาคาร A
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : เหลือง ชุ่น ไม่มีตะกอน มีกลิ่นเหม็นเล็กน้อย
SAMPLING DATE : JANUARY 28, 2026
SAMPLING TIME : 10:30
SAMPLING BY : นายพิรพล ถวิลหวัง
REPORT NO. : RN260110120
SAMPLING SOURCE : WASTEWATER
RECEIVED DATE : JANUARY 28, 2026
ANALYTICAL DATE : JANUARY 28 - FEBRUARY 05, 2026
REPORT DATE : FEBRUARY 06, 2026

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
pH [#]	-	Electrometric (SM: 4500-H ⁺ B.)	7.1 at 25°C	-	5.5-9.0
Biochemical Oxygen Demand	mg/l	Azide Modification (SM: 4500-O C, 5210 B.)	28.0	2.0	≤30
Total Dissolved Solids [#]	mg/l	Total Dissolved Solids Dried at 180°C (SM: 2540 C.)	624.0	-	≤1,000
Total Suspended Solids	mg/l	Total Suspended Solids Dried at 103-105°C (SM: 2540 D.)	Not Detected	-	≤40
Settleable Solids	ml/l	Settleable Solids (SM: 2540 F.)	<0.1	-	-
Sulfide as H ₂ S	mg/l	Iodometric (SM: 4500-S ²⁻ F.)	Not Detected	-	≤1.0
Total Kjeldahl Nitrogen	mg/l	Macro Kjeldahl (SM: 4500-N _{org} B)	24.0	-	<35
Oil & Grease	mg/l	Liquid-Liquid Partition-Gravimetric (SM: 5520 B.)	2.0	1.4	<20
Total Coliform Bacteria	MPN/100 ml	MPN Test	>2.4 x 10 ⁶	-	-
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	>2.4 x 10 ⁶	-	-

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED.,2023 (AWWA,APHA, WEF)

Remark : 1. * Notification of the Ministry of Natural Resources and Environment, dated June 28, B.E. 2567 (2024), which was published in the Royal Government Gazette, Vol. 141, Part 233D dated August 27, B.E. 2567 (2024) . (Category B)
2. [#] ISO/IEC 17025 ACCREDITED BY DEPARTMENT OF SCIENCE SERVICE (DSS)

(MR TAWATCHAI CHONGVUTICHA)

LABORATORY SUPERVISOR



ANALYSIS REPORT


CUSTOMER NAME : เดอะ วิลลีย์ เขาใหญ่
ADDRESS : เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เขาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.
SAMPLING LOCATION : ถังแยกกากของระบบบำบัดน้ำเสีย อาคาร B
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : เหลือง ขุ่น มีตะกอน มีกลิ่นเหม็นเล็กน้อย
SAMPLING DATE : JANUARY 28, 2026
SAMPLING TIME : 10:30
SAMPLING BY : นายพีรพล ถวิลหวัง

REPORT NO. : RN260110121
SAMPLING SOURCE : WASTEWATER
RECEIVED DATE : JANUARY 28, 2026
ANALYTICAL DATE : JANUARY 28 - FEBRUARY 05, 2026
REPORT DATE : FEBRUARY 06, 2026

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
pH [#]	-	Electrometric (SM: 4500-H ⁺ B.)	6.8 at 25°C	-	-
Biochemical Oxygen Demand	mg/l	Azide Modification (SM: 4500-O C, 5210 B.)	25.0	2.0	-
Total Dissolved Solids [#]	mg/l	Total Dissolved Solids Dried at 180°C (SM: 2540 C.)	576.0	-	-
Total Suspended Solids [#]	mg/l	Total Suspended Solids Dried at 103-105°C (SM: 2540 D.)	16.0	-	-
Settleable Solids	ml/l	Settleable Solids (SM: 2540 F.)	<0.1	-	-
Sulfide as H ₂ S	mg/l	Iodometric (SM: 4500-S ²⁻ F.)	Not Detected	-	-
Total Kjeldahl Nitrogen	mg/l	Macro Kjeldahl (SM: 4500-N _{org} B)	15.0	-	-
Oil & Grease	mg/l	Liquid-Liquid Partition-Gravimetric (SM: 5520 B.)	2.4	1.4	-
Total Coliform Bacteria	MPN/100 ml	MPN Test	2.1 x 10 ⁵	-	-
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	4.8 x 10 ⁴	-	-

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED.,2023 (AWWA,APHA, WEF)

Remark : 1. Notification of the Ministry of Natural Resources and Environment, dated June 28, B.E. 2567 (2024), which was published in the Royal Government Gazette, Vol. 141, Part 233D dated August 27, B.E. 2567 (2024) . (Category B)
2. [#] ISO/IEC 17025 ACCREDITED BY DEPARTMENT OF SCIENCE SERVICE (DSS)

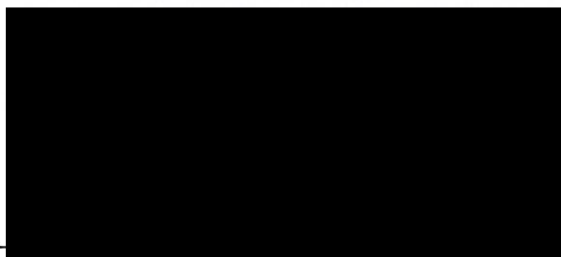

(MR TAWATCHAI CHONGVUTICHA)

LABORATORY SUPERVISOR




ANALYSIS REPORT

CUSTOMER NAME : เดอะ วิลลีย์ เขาใหญ่
ADDRESS : เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เขาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.
SAMPLING LOCATION : บ่อกักน้ำแรกหลังออกจากระบบบำบัดน้ำเสีย อาคาร B
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : เหลือง ขุ่น ไม่มีตะกอน ไม่มีกลิ่น
SAMPLING DATE : JANUARY 28, 2026
SAMPLING TIME : 10:30
SAMPLING BY : นายพีรพล ถวิลหวัง
REPORT NO. : RN260110122
SAMPLING SOURCE : WASTEWATER
RECEIVED DATE : JANUARY 28, 2026
ANALYTICAL DATE : JANUARY 28 - FEBRUARY 05, 2026
REPORT DATE : FEBRUARY 06, 2026

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
pH [#]	-	Electrometric (SM: 4500-H ⁺ B.)	7.2 at 25°C	-	5.5-9.0
Biochemical Oxygen Demand	mg/l	Azide Modification (SM: 4500-O C, 5210 B.)	28.5	2.0	≤30
Total Dissolved Solids [#]	mg/l	Total Dissolved Solids Dried at 180°C (SM: 2540 C.)	562.0	-	≤1,000
Total Suspended Solids [#]	mg/l	Total Suspended Solids Dried at 103-105°C (SM: 2540 D.)	8.0	-	≤40
Settleable Solids	ml/l	Settleable Solids (SM: 2540 F.)	<0.1	-	-
Sulfide as H ₂ S	mg/l	Iodometric (SM: 4500-S ²⁻ F.)	Not Detected	-	≤1.0
Total Kjeldahl Nitrogen	mg/l	Macro Kjeldahl (SM: 4500-N _{org} B)	17.0	-	<35
Oil & Grease	mg/l	Liquid-Liquid Partition-Gravimetric (SM: 5520 B.)	1.4	1.4	<20
Total Coliform Bacteria	MPN/100 ml	MPN Test	1.1 x 10 ⁶	-	-
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	2.9 x 10 ⁵	-	-

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED., 2023 (AWWA, APHA, WEF)

Remark : 1. * Notification of the Ministry of Natural Resources and Environment, dated June 28, B.E. 2567 (2024), which was published in the Royal Government Gazette, Vol. 141, Part 233D dated August 27, B.E. 2567 (2024) . (Category B)
2. [#] ISO/IEC 17025 ACCREDITED BY DEPARTMENT OF SCIENCE SERVICE (DSS)



LABORATORY SUPERVISOR



ANALYSIS REPORT

CUSTOMER NAME : เดอะ วัลลีย์ เขาใหญ่
ADDRESS : เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เขาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.
SAMPLING LOCATION : ตั้งแยกจากของระบบบำบัดน้ำเสีย อาคาร C
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : เหลือง ขุ่น มีตะกอน มีกลิ่นเหม็นเล็กน้อย
SAMPLING DATE : JANUARY 28, 2026
SAMPLING TIME : 10:30
SAMPLING BY : นายพีรพล ถวิลหวัง


REPORT NO. : RN260110123
SAMPLING SOURCE : WASTEWATER
RECEIVED DATE : JANUARY 28, 2026
ANALYTICAL DATE : JANUARY 28 - FEBRUARY 05, 2026
REPORT DATE : FEBRUARY 06, 2026

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
pH [#]	-	Electrometric (SM: 4500-H ⁺ B.)	7.7 at 25°C	-	-
Biochemical Oxygen Demand	mg/l	Azide Modification (SM: 4500-O C, 5210 B.)	57.0	2.0	-
Total Dissolved Solids [#]	mg/l	Total Dissolved Solids Dried at 180°C (SM: 2540 C.)	494.0	-	-
Total Suspended Solids [#]	mg/l	Total Suspended Solids Dried at 103-105°C (SM: 2540 D.)	38.0	-	-
Settleable Solids	ml/l	Settleable Solids (SM: 2540 F.)	<0.1	-	-
Sulfide as H ₂ S	mg/l	Iodometric (SM: 4500-S ²⁻ F.)	Not Detected	-	-
Total Kjeldahl Nitrogen	mg/l	Macro Kjeldahl (SM: 4500-N _{org} B)	39.0	-	-
Oil & Grease	mg/l	Liquid-Liquid Partition-Gravimetric (SM: 5520 B.)	2.6	1.4	-
Total Coliform Bacteria	MPN/100 ml	MPN Test	>2.4 x 10 ⁶	-	-
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	1.1 x 10 ⁶	-	-

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED., 2023 (AWWA, APHA, WEF)

Remark : 1. * Notification of the Ministry of Natural Resources and Environment, dated June 28, B.E. 2567 (2024), which was published in the Royal Government Gazette, Vol. 141, Part 233D dated August 27, B.E. 2567 (2024) . (Category B)

2. [#] ISO/IEC 17025 ACCREDITED BY DEPARTMENT OF SCIENCE SERVICE (DSS)

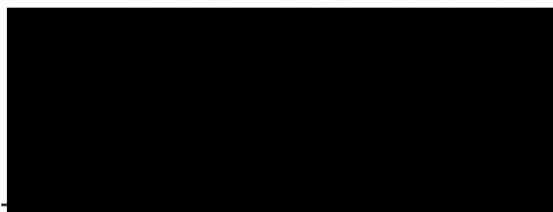

(MR TAWATCHAI CHONGVUTICHAJ)

LABORATORY SUPERVISOR



ANALYSIS REPORT


CUSTOMER NAME : เดอะ วัลลีย์ เขาใหญ่
ADDRESS : เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เขาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.
SAMPLING LOCATION : บ่อพักน้ำแรกหลังจากการบำบัดน้ำเสีย อาคาร C
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : เหลือง ขุ่น ไม่มีตะกอน ไม่มีกลิ่น
SAMPLING DATE : JANUARY 28, 2026
SAMPLING TIME : 10:30
SAMPLING BY : นายพีรพล ถวิลหวัง

REPORT NO. : RN260110124
SAMPLING SOURCE : WASTEWATER
RECEIVED DATE : JANUARY 28, 2026
ANALYTICAL DATE : JANUARY 28 - FEBRUARY 05, 2026
REPORT DATE : FEBRUARY 06, 2026

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
pH [#]	-	Electrometric (SM: 4500-H ⁺ B.)	7.5 at 25°C	-	5.5-9.0
Biochemical Oxygen Demand	mg/l	Azide Modification (SM: 4500-O C, 5210 B.)	4.6	2.0	≤30
Total Dissolved Solids [#]	mg/l	Total Dissolved Solids Dried at 180°C (SM: 2540 C.)	524.0	-	≤1,000
Total Suspended Solids [#]	mg/l	Total Suspended Solids Dried at 103-105°C (SM: 2540 D.)	16.0	-	≤40
Settleable Solids	ml/l	Settleable Solids (SM: 2540 F.)	<0.1	-	-
Sulfide as H ₂ S	mg/l	Iodometric (SM: 4500-S ²⁻ F.)	Not Detected	-	≤1.0
Total Kjeldahl Nitrogen	mg/l	Macro Kjeldahl (SM: 4500-N _{org} B)	2.5	-	<35
Oil & Grease	mg/l	Liquid-Liquid Partition-Gravimetric (SM: 5520 B.)	1.8	1.4	<20
Total Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	-
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	-

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED.,2023 (AWWA,APHA, WEF)

- Remark : 1. ^{*} Notification of the Ministry of Natural Resources and Environment, dated June 28, B.E. 2567 (2024), which was published in the Royal Government Gazette, Vol. 141, Part 233D dated August 27, B.E. 2567 (2024) . (Category B)
2. [#] ISO/IEC 17025 ACCREDITED BY DEPARTMENT OF SCIENCE SERVICE (DSS)



(MR TAWATCHAI CHONGVUTICHAJ)

LABORATORY SUPERVISOR



ANALYSIS REPORT


CUSTOMER NAME : เดอะ วัลลีย์ เขาใหญ่
ADDRESS : เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เขาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.
SAMPLING LOCATION : สระว่ายน้ำ (ส่วนต้น)
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER :ใส ไม่มีตะกอน ไม่มีกลิ่น
SAMPLING DATE : JANUARY 28, 2026
SAMPLING TIME : 10:30
SAMPLING BY : นายพีรพล ถวิลหวั่ง

REPORT NO. : RN260110125
SAMPLING SOURCE : SWIMMING POOL
RECEIVED DATE : JANUARY 28, 2026
ANALYTICAL DATE : JANUARY 28 - FEBRUARY 05, 2026
REPORT DATE : FEBRUARY 06, 2026

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
Total Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	<10
<i>Escherichia Coli</i>	per 100 ml	E.coli Procedure Using Fluorogenic Substrate (SM: 9221 F.)	Not Detected	-	Not Detected

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED.,2023 (AWWA,APHA, WEF)

- Remark :
- * Recommendations of the Public Health Committee No. 1/2007 regarding the control of swimming pool operations or other businesses Likewise.
 - ** mean analysis were performed by HVE Co.,Ltd .



LABORATORY SUPERVISOR



บริษัท เอชวีอี จำกัด 603 ซอยจรัญสนิทวงศ์ 46 ถนนจรัญสนิทวงศ์ แขวงบางมด เขตบางพลัด กรุงเทพฯ 10700
HVE CO. LTD. 603 Sol Jarunsnitwong 46 Jarunsnitwong Road Bangyeekan Bangplad Bangkok 10700
Tel : (02) 8834956-7 , (02) 8834274 Fax : (02) 8834958 E-mail address hv_eng@hotmail.com

รายงานผลการทดสอบ
(ANALYSIS REPORT)

รายงานหมายเลข (Report No.) 8640126 วันที่ (Date) 6 กุมภาพันธ์ 2569
ชื่อตัวอย่าง (Sample Name)^c น้ำระเหยน้ำ (ส่วนดื่ม)
รหัสตัวอย่าง (Sample No.) No. 0901886
ลักษณะตัวอย่างทางกายภาพ^c ไม่มีสี, ไม่มีตะกอน
ชื่อลูกค้า (Customer name)^c บริษัท โอกลา เทสติ้ง แอนด์ คอนซัลติ้ง เซอร์วิส จำกัด (สำนักงานใหญ่)
สถานที่เก็บตัวอย่าง (Sampling site)^c Project TWL75
ที่อยู่ (Address)^c 63/13 ซอยเพชรเกษม 7 แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพฯ 10600
วันที่รับตัวอย่าง (Received Date) 28 มกราคม 2569 วันที่ตรวจวิเคราะห์ (Analysis Date) 28 มกราคม 2569 - 8 กุมภาพันธ์ 2569
วันที่เก็บตัวอย่าง (Collected Date)^c 28 มกราคม 2569 วิธีการเก็บตัวอย่าง (Sampling Method)^c เก็บแบบ จ้วง (Grab)

พารามิเตอร์ (Parameter)	หน่วย (Unit)	ผลการวิเคราะห์ (Result)	MDL	ค่ามาตรฐาน ⁱⁱ (Standard)	วิธีทดสอบ ⁱⁱⁱ (Test Method)
		น้ำระเหยน้ำ (ส่วนดื่ม)			
<i>Staphylococcus aureus</i>	per 100 mL	Not Detected	-	Not Detected	In-house method based on APHA, AWWA, WEF 24 th ed. 2023, 9213 B
<i>Pseudomonas aeruginosa</i>	per 100 mL	Not Detected	-	Not Detected	APHA, AWWA, WEF 24 th ed. 2023, 9213 E


หมายเหตุ : ⁱ ค่าเฉลี่ยของคณะกรรมการสาธารณสุข ฉบับที่ 1/2550 เรื่อง การควบคุมการประกอบกิจการระเหยน้ำ หรือกิจการอื่นฯ ในท้องถิ่น

ⁱⁱ Standard Methods for the Examination of Water and Wastewater, APHA, AWWA, WEF, 24th ed. 2023

^c เป็นข้อมูลที่มาจากรายงาน

- สภาวะแวดล้อมของห้องปฏิบัติการ 25 ± 5 °C

- ห้องปฏิบัติการมีนโยบายไม่รับตัวอย่างเอง



ผู้จัดการฝ่ายวิชาการ

ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์
ทะเบียนเลขที่ ว-358-ค-0002

- รายงานผลการทดสอบนี้ให้รับรองเฉพาะตัวอย่างตามที่ได้รับมาทดสอบเท่านั้น
- ห้ามนำรายงานผลการทดสอบนี้ไปประกาศโฆษณา
- รายงานผลการทดสอบนี้ห้ามคัดลอกถ่ายทำสำเนาเฉพาะเพียงบางส่วน โดยไม่ได้รับอนุญาตจากห้องปฏิบัติการเป็นลายลักษณ์อักษร ยกเว้นทำทั้งฉบับ



ANALYSIS REPORT

CUSTOMER NAME : เดอะ วิลลีย์ เขาใหญ่
ADDRESS : เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เขาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.
SAMPLING LOCATION : สระว่ายน้ำ (ส่วนลึก)
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER :ใส ไม่มีตะกอน ไม่มีกลิ่น
SAMPLING DATE : JANUARY 28, 2026
SAMPLING TIME : 10:30
SAMPLING BY : นายพีรพล ถวิลหวั่ง

REPORT NO. : RN260110126
SAMPLING SOURCE : SWIMMING POOL
RECEIVED DATE : JANUARY 28, 2026
ANALYTICAL DATE : JANUARY 28 - FEBRUARY 05, 2026
REPORT DATE : FEBRUARY 06, 2026

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD
Total Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	<10
<i>Escherichia Coli</i>	per 100 ml	E.coli Procedure Using Fluorogenic Substrate (SM: 9221 F.)	Not Detected	-	Not Detected

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED.,2023 (AWWA,APHA, WEF)

- Remark :
- Recommendations of the Public Health Committee No. 1/2007 regarding the control of swimming pool operations or other businesses Likewise.
 - ** mean analysis were performed by HVE Co.,Ltd .



(Mr. THAWAT CHONGVONHAK)

LABORATORY SUPERVISOR



บริษัท เอชวีอี จำกัด 603 ซอยจรัญสนิทวงศ์ 46 ถนนจรัญสนิทวงศ์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพฯ 10700
HVE CO. LTD. 603 Soi Jarunsnitwong 46 Jarunsnitwong Road Bangyeekan Bangplad Bangkok 10700
Tel : (02) 8834958-7 , (02) 8834274 Fax : (02) 8834958 E-mail address hv_eng@hotmail.com

รายงานผลการทดสอบ
(ANALYSIS REPORT)

รายงานหมายเลข (Report No.) 8650126 วันที่ (Date) 6 กุมภาพันธ์ 2569
ชื่อตัวอย่าง (Sample Name)^c น้ำระวายน้ำ (ส่วนลึก)
รหัสตัวอย่าง (Sample No.) No. 6901887
ลักษณะตัวอย่างทางกายภาพ^c ไม่มีสี, ไม่มีตะกอน
ชื่อลูกค้า (Customer name)^c บริษัท โอกลา เทสดีง แอนด์ คอนซัลติ้ง เซอร์วิส จำกัด (สำนักงานใหญ่)
สถานที่เก็บตัวอย่าง (Sampling site)^c Project TWL75
ที่อยู่ (Address)^c 63/13 ซอยเพชรเกษม 7 แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพฯ 10600
วันที่รับตัวอย่าง (Received Date) 28 มกราคม 2569 วันที่ตรวจวิเคราะห์ (Analysis Date) 28 มกราคม 2569 - 6 กุมภาพันธ์ 2569
วันที่เก็บตัวอย่าง (Collected Date)^c 28 มกราคม 2569 วิธีการเก็บตัวอย่าง (Sampling Method)^c เก็บแบบ จ้วง (Grab)

พารามิเตอร์ (Parameter)	หน่วย (Unit)	ผลการวิเคราะห์ (Result)	MDL	ค่ามาตรฐาน ^{1/} (Standard)	วิธีทดสอบ ^{4/} (Test Method)
		น้ำระวายน้ำ (ส่วนลึก)			
<i>Staphylococcus aureus</i>	per 100 mL	Not Detected	-	Not Detected	In-house method based on APHA, AWWA, WEF 24 th ed. 2023, 9213 B
<i>Pseudomonas aeruginosa</i>	per 100 mL	Not Detected	-	Not Detected	APHA, AWWA, WEF 24 th ed. 2023, 9213 E

หมายเหตุ : ^{1/} ส่วนหนึ่งของคณะกรรมการสาธารณสุข ฉบับที่ 1/2550 เรื่อง การควบคุมการประกอบกิจการระวายน้ำ หรือกิจการอื่นๆ ในทางองค์เดียวกัน

^{4/} Standard Methods for the Examination of Water and Wastewater, APHA, AWWA, WEF, 24th ed. 2023

^c เป็นข้อมูลที่ได้จากลูกค้า

- สภาวะแวดล้อมของห้องปฏิบัติการ 25 ± 5 °C
- ห้องปฏิบัติการมีนโยบายไม่ชักตัวอย่างเอง

(นายฐานนท์ นิการัตน)
ผู้จัดการฝ่ายวิชาการ

(นางสาวทิพวรรณ วงศ์บุญตัน)
ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์
ทะเบียนเลขที่ ว-358-ค-0002

- รายงานผลการทดสอบนี้ใช้รับรองเฉพาะตัวอย่างตามที่ได้นำมาทดสอบเท่านั้น
- ห้ามนำรายงานผลการทดสอบนี้ไปประกาศโฆษณา
- รายงานผลการทดสอบนี้ห้ามคัดลอกถ่ายทำสำเนาเฉพาะเพียงบางส่วน โดยไม่ได้รับอนุญาตจากห้องปฏิบัติการเป็นลายลักษณ์อักษร ยกเว้นทำหังฉบับ



ANALYSIS REPORT


CUSTOMER NAME : เดอะ วิลลีย์ เขาใหญ่
ADDRESS : เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เขาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.
SAMPLING LOCATION : ถังแยกกากของระบบบำบัดน้ำเสีย อาคาร A
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : เหลืองเข้ม ขุ่นเล็กน้อย มีตะกอน มีกลิ่นเหม็นเล็กน้อย
SAMPLING DATE : FEBRUARY 12, 2026
SAMPLING TIME : 11:30
SAMPLING BY : นายโกวิท นุฬา
REPORT NO. : RN260210294
SAMPLING SOURCE : WASTEWATER
RECEIVED DATE : FEBRUARY 12, 2026
ANALYTICAL DATE : FEBRUARY 12-20, 2026
REPORT DATE : FEBRUARY 23, 2026

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
pH [#]	-	Electrometric (SM: 4500-H ⁺ B.)	8.8 at 25°C	-	-
Biochemical Oxygen Demand	mg/l	Azide Modification (SM: 4500-O C, 5210 B.)	70.0	2.0	-
Total Dissolved Solids [#]	mg/l	Total Dissolved Solids Dried at 180°C (SM: 2540 C.)	616.0	-	-
Total Suspended Solids [#]	mg/l	Total Suspended Solids Dried at 103-105°C (SM: 2540 D.)	40.0	-	-
Settleable Solids	ml/l	Settleable Solids (SM: 2540 F.)	3.0	-	-
Sulfide as H ₂ S	mg/l	Iodometric (SM: 4500-S ²⁻ F.)	Not Detected	-	-
Total Kjeldahl Nitrogen	mg/l	Macro Kjeldahl (SM: 4500-N _{org} B)	36.0	-	-
Oil & Grease	mg/l	Liquid-Liquid Partition-Gravimetric (SM: 5520 B.)	3.6	1.4	-
Total Coliform Bacteria	MPN/100 ml	MPN Test	>2.4 x 10 ⁶	-	-
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	>2.4 x 10 ⁶	-	-

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED.,2023 (AWWA,APHA, WEF)

Remark : 1. Notification of the Ministry of Natural Resources and Environment, dated June 28, B.E. 2567 (2024), which was published in the Royal Government Gazette, Vol. 141, Part 233D dated August 27, B.E. 2567 (2024) . (Category B)

2. [#]ISO/IEC 17025 ACCREDITED BY DEPARTMENT OF SCIENCE SERVICE (DSS)



(MR TAWAN CHAI CHONGVOTICHAI)

LABORATORY SUPERVISOR




ANALYSIS REPORT

CUSTOMER NAME : เดอะ วิลลีย์ เขาใหญ่
ADDRESS : เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เขาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.
SAMPLING LOCATION : บ่อพักน้ำแรกหลังจากการระบบบำบัดน้ำเสีย อาคาร A
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : น้ำตาล ไส มีตะกอน ไม่มีกลิ่น
SAMPLING DATE : FEBRUARY 12, 2026
SAMPLING TIME : 11:30
SAMPLING BY : นายโกวิท บุฬา
REPORT NO. : RN260210295
SAMPLING SOURCE : WASTEWATER
RECEIVED DATE : FEBRUARY 12, 2026
ANALYTICAL DATE : FEBRUARY 12-20, 2026
REPORT DATE : FEBRUARY 23, 2026

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
pH [#]	-	Electrometric (SM: 4500-H ⁺ B.)	8.1 at 25°C	-	5.5-9.0
Biochemical Oxygen Demand	mg/l	Azide Modification (SM: 4500-O C, 5210 B.)	27.5	2.0	≤30
Total Dissolved Solids [#]	mg/l	Total Dissolved Solids Dried at 180°C (SM: 2540 C.)	612.0	-	≤1,000
Total Suspended Solids [#]	mg/l	Total Suspended Solids Dried at 103-105°C (SM: 2540 D.)	10.0	-	≤40
Settleable Solids	ml/l	Settleable Solids (SM: 2540 F.)	3.0	-	-
Sulfide as H ₂ S	mg/l	Iodometric (SM: 4500-S ²⁻ F.)	Not Detected	-	≤1.0
Total Kjeldahl Nitrogen	mg/l	Macro Kjeldahl (SM: 4500-N _{org} B)	33.0	-	<35
Oil & Grease	mg/l	Liquid-Liquid Partition-Gravimetric (SM: 5520 B.)	2.0	1.4	<20
Total Coliform Bacteria	MPN/100 ml	MPN Test	>2.4 x 10 ⁶	-	-
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	>2.4 x 10 ⁶	-	-

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED.,2023 (AWWA,APHA, WEF)

- Remark : 1. * Notification of the Ministry of Natural Resources and Environment, dated June 28, B.E. 2567 (2024), which was published in the Royal Government Gazette, Vol. 141, Part 233D dated August 27, B.E. 2567 (2024) . (Category B)
2. [#] ISO/IEC 17025 ACCREDITED BY DEPARTMENT OF SCIENCE SERVICE (DSS)



LABORATORY SUPERVISOR




ANALYSIS REPORT

CUSTOMER NAME : เดอะ วิลลีย์ เขาใหญ่
ADDRESS : เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เขาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.
SAMPLING LOCATION : ถังแยกกากของระบบบำบัดน้ำเสีย อาคาร B
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : น้ำตาล ชุ่น มีตะกอน ไม่มีกลิ่น
SAMPLING DATE : FEBRUARY 12, 2026
SAMPLING TIME : 11:30
SAMPLING BY : นายโกวิท บุหา
REPORT NO. : RN260210296
SAMPLING SOURCE : WASTEWATER
RECEIVED DATE : FEBRUARY 12, 2026
ANALYTICAL DATE : FEBRUARY 12-20, 2026
REPORT DATE : FEBRUARY 23, 2026

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
pH [#]	-	Electrometric (SM: 4500-H ⁺ B.)	8.0 at 25°C	-	-
Biochemical Oxygen Demand	mg/l	Azide Modification (SM: 4500-O C, 5210 B.)	36.5	2.0	-
Total Dissolved Solids [#]	mg/l	Total Dissolved Solids Dried at 180°C (SM: 2540 C.)	602.0	-	-
Total Suspended Solids [#]	mg/l	Total Suspended Solids Dried at 103-105°C (SM: 2540 D.)	35.0	-	-
Settleable Solids	ml/l	Settleable Solids (SM: 2540 F.)	<0.1	-	-
Sulfide as H ₂ S	mg/l	Iodometric (SM: 4500-S ²⁻ F.)	Not Detected	-	-
Total Kjeldahl Nitrogen	mg/l	Macro Kjeldahl (SM: 4500-N _{org} B)	27.0	-	-
Oil & Grease	mg/l	Liquid-Liquid Partition-Gravimetric (SM: 5520 B.)	1.8	1.4	-
Total Coliform Bacteria	MPN/100 ml	MPN Test	4.8 x 10 ⁵	-	-
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	2.9 x 10 ⁵	-	-

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED.,2023 (AWWA,APHA, WEF)

- Remark : 1. Notification of the Ministry of Natural Resources and Environment, dated June 28, B.E. 2567 (2024), which was published in the Royal Government Gazette, Vol. 141, Part 233D dated August 27, B.E. 2567 (2024) . (Category B)
2. [#] ISO/IEC 17025 ACCREDITED BY DEPARTMENT OF SCIENCE SERVICE (DSS)

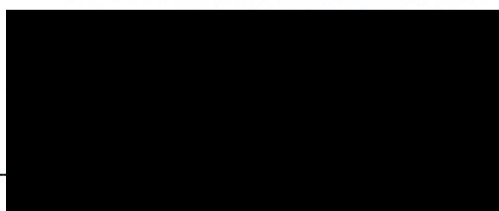

LABORATORY SUPERVISOR



ANALYSIS REPORT


CUSTOMER NAME : เดอะ วัลลีย์ เขาใหญ่
ADDRESS : เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เขาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.
SAMPLING LOCATION : บ่อพักน้ำแรกหลังจากจากระบบบำบัดน้ำเสีย อาคาร B
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : เหลืออุณหภูมิ ไม่มีตะกอน ไม่มีกลิ่น
SAMPLING DATE : FEBRUARY 12, 2026
SAMPLING TIME : 11:30
SAMPLING BY : นายโกวิท นุฬา
REPORT NO. : RN260210297
SAMPLING SOURCE : WASTEWATER
RECEIVED DATE : FEBRUARY 12, 2026
ANALYTICAL DATE : FEBRUARY 12-20, 2026
REPORT DATE : FEBRUARY 23, 2026

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
pH [#]	-	Electrometric (SM: 4500-H ⁺ B.)	8.7 at 25°C	-	5.5-9.0
Biochemical Oxygen Demand	mg/l	Azide Modification (SM: 4500-O C, 5210 B.)	21.5	2.0	≤30
Total Dissolved Solids [#]	mg/l	Total Dissolved Solids Dried at 180°C (SM: 2540 C.)	566.0	-	≤1,000
Total Suspended Solids [#]	mg/l	Total Suspended Solids Dried at 103-105°C (SM: 2540 D.)	10.0	-	≤40
Settleable Solids	ml/l	Settleable Solids (SM: 2540 F.)	<0.1	-	-
Sulfide as H ₂ S	mg/l	Iodometric (SM: 4500-S ²⁻ F.)	Not Detected	-	≤1.0
Total Kjeldahl Nitrogen	mg/l	Macro Kjeldahl (SM: 4500-N _{org} B)	15.0	-	<35
Oil & Grease	mg/l	Liquid-Liquid Partition-Gravimetric (SM: 5520 B.)	Not Detected	1.4	<20
Total Coliform Bacteria	MPN/100 ml	MPN Test	1.2 × 10 ⁵	-	-
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	9.0 × 10 ⁴	-	-

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED.,2023 (AWWA,APHA, WEF)

Remark : 1. * Notification of the Ministry of Natural Resources and Environment, dated June 28, B.E. 2567 (2024), which was published in the Royal Government Gazette, Vol. 141, Part 233D dated August 27, B.E. 2567 (2024) . (Category B)

2. [#] ISO/IEC 17025 ACCREDITED BY DEPARTMENT OF SCIENCE SERVICE (DSS)



LABORATORY SUPERVISOR



ANALYSIS REPORT

CUSTOMER NAME : เดอะ วอลล์ เซาท์ไฮ
ADDRESS : เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เขาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.
SAMPLING LOCATION : ถังแยกกากของระบบบำบัดน้ำเสีย อาคาร C
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : น้ำตาลอ่อนใส ไม่มีตะกอน มีกลิ่นเหม็นเล็กน้อย
SAMPLING DATE : FEBRUARY 12, 2026
SAMPLING TIME : 11:30
SAMPLING BY : นายโกวิท บุฬา
REPORT NO. : RN260210298
SAMPLING SOURCE : WASTEWATER
RECEIVED DATE : FEBRUARY 12, 2026
ANALYTICAL DATE : FEBRUARY 12-20, 2026
REPORT DATE : FEBRUARY 23, 2026

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD
pH [#]	-	Electrometric (SM: 4500-H ⁺ B.)	8.8 at 25°C	-	-
Biochemical Oxygen Demand	mg/l	Azide Modification (SM: 4500-O C, 5210 B.)	14.8	2.0	-
Total Dissolved Solids [#]	mg/l	Total Dissolved Solids Dried at 180°C (SM: 2540 C.)	692.0	-	-
Total Suspended Solids	mg/l	Total Suspended Solids Dried at 103-105°C (SM: 2540 D.)	4.0	-	-
Settleable Solids	ml/l	Settleable Solids (SM: 2540 F.)	<0.1	-	-
Sulfide as H ₂ S	mg/l	Iodometric (SM: 4500-S ²⁻ F.)	Not Detected	-	-
Total Kjeldahl Nitrogen	mg/l	Macro Kjeldahl (SM: 4500-N _{org} B)	6.7	-	-
Oil & Grease	mg/l	Liquid-Liquid Partition-Gravimetric (SM: 5520 B.)	2.0	1.4	-
Total Coliform Bacteria	MPN/100 ml	MPN Test	960.0	-	-
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	150.0	-	-

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED., 2023 (AWWA, APHA, WEF)

Remark : 1. Notification of the Ministry of Natural Resources and Environment, dated June 28, B.E. 2567 (2024), which was published in the Royal Government Gazette, Vol. 141, Part 233D dated August 27, B.E. 2567 (2024) . (Category B)
2. [#] ISO/IEC 17025 ACCREDITED BY DEPARTMENT OF SCIENCE SERVICE (DSS)



LABORATORY SUPERVISOR




ANALYSIS REPORT

CUSTOMER NAME : เดอะ วิลลีย์ เขาใหญ่
ADDRESS : เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เขาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.
SAMPLING LOCATION : บ่อพักน้ำแรกหลังจากกระบบบำบัดน้ำเสีย อาคาร C
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : ใส ไม่มีสี ไม่มีตะกอน ไม่มีกลิ่น
SAMPLING DATE : FEBRUARY 12, 2026
SAMPLING TIME : 11:30
SAMPLING BY : นายโกวิท บุฬา
REPORT NO. : RN260210299
SAMPLING SOURCE : WASTEWATER
RECEIVED DATE : FEBRUARY 12, 2026
ANALYTICAL DATE : FEBRUARY 12-20, 2026
REPORT DATE : FEBRUARY 23, 2026

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
pH [#]	-	Electrometric (SM: 4500-H ⁺ B.)	8.2 at 25°C	-	5.5-9.0
Biochemical Oxygen Demand	mg/l	Azide Modification (SM: 4500-O C, 5210 B.)	8.4	2.0	≤30
Total Dissolved Solids [#]	mg/l	Total Dissolved Solids Dried at 180°C (SM: 2540 C.)	518.0	-	≤1,000
Total Suspended Solids	mg/l	Total Suspended Solids Dried at 103-105°C (SM: 2540 D.)	Not Detected	-	≤40
Settleable Solids	ml/l	Settleable Solids (SM: 2540 F.)	<0.1	-	-
Sulfide as H ₂ S	mg/l	Iodometric (SM: 4500-S ²⁻ F.)	Not Detected	-	≤1.0
Total Kjeldahl Nitrogen	mg/l	Macro Kjeldahl (SM: 4500-N _{org} B)	5.0	-	<35
Oil & Grease	mg/l	Liquid-Liquid Partition-Gravimetric (SM: 5520 B.)	Not Detected	1.4	<20
Total Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	-
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	-

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED.,2023 (AWWA,APHA, WEF)

- Remark : 1. Notification of the Ministry of Natural Resources and Environment, dated June 28, B.E. 2567 (2024), which was published in the Royal Government Gazette, Vol. 141, Part 233D dated August 27, B.E. 2567 (2024) . (Category B)
2. [#] ISO/IEC 17025 ACCREDITED BY DEPARTMENT OF SCIENCE SERVICE (DSS)

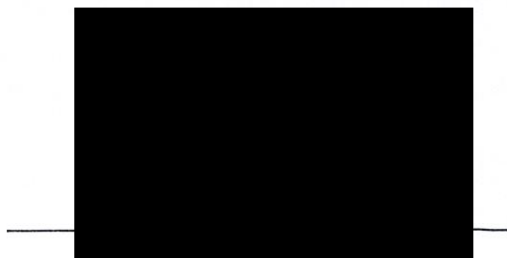

LABORATORY SUPERVISOR



ANALYSIS REPORT

CUSTOMER NAME : เดอะ วัลลีย์ เขาใหญ่
ADDRESS : เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เขาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.
SAMPLING LOCATION : สระว่ายน้ำ (ส่วนต้น)
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : ใส ไม่มีตะกอน ไม่มีกลิ่น
SAMPLING DATE : FEBRUARY 12, 2026
SAMPLING TIME : 11:30
SAMPLING BY : นายโกวิท บุฬา

REPORT NO. : RN260210300
SAMPLING SOURCE : SWIMMING POOL
RECEIVED DATE : FEBRUARY 12, 2026
ANALYTICAL DATE : FEBRUARY 12-20, 2026
REPORT DATE : FEBRUARY 23, 2026

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD
Total Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	<10
Escherichia Coli	per 100 ml	E.coli Procedure Using Fluorogenic Substrate (SM: 9221 F.)	Not Detected	-	Not Detected

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED.,2023 (AWWA,APHA, WEF)

- Remark :
- Recommendations of the Public Health Committee No. 1/2007 regarding the control of swimming pool operations or other businesses Likewise.
 - mean analysis were performed by HVE Co.,Ltd .



(MR TAWATCHAI CHONGVUTICHAJ)

LABORATORY SUPERVISOR



บริษัท เอชวี จำกัด 603 ซอยจรัญสนิทวงศ์ 46 ถนนจรัญสนิทวงศ์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพฯ 10700
HVE CO. LTD. 603 Sol Jarunsanitwong 46 Jarunsanitwong Road Bangyeekan Bangplad Bangkok 10700
Tel : (02) 8834958-7 , (02) 8834274 Fax : (02) 8834958 E-mail address hv_eng@hotmail.com

รายงานผลการทดสอบ
(ANALYSIS REPORT)

รายงานหมายเลข (Report No.) 3350226 วันที่ (Date) 21 กุมภาพันธ์ 2569
ชื่อตัวอย่าง (Sample Name)^c น้ำระวายน้ำ (ส่วนต้น)
รหัสตัวอย่าง (Sample No.) No. 6902310
ลักษณะตัวอย่างทางกายภาพ^c ใส่ ไม่มีตะกอน
ชื่อลูกค้า (Customer name)^c บริษัท โอกลา เทสดิง แอนด์ คอนซัลติง เซอร์วิส จำกัด (สำนักงานใหญ่)
สถานที่เก็บตัวอย่าง (Sampling site)^c Project TWL75
ที่อยู่ (Address)^c 63/13 ซอยเพชรเกษม 7 แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพฯ 10600
วันที่รับตัวอย่าง (Received Date) 12 กุมภาพันธ์ 2569 วันที่ตรวจวิเคราะห์ (Analyse Date) 12 กุมภาพันธ์ 2569 - 21 กุมภาพันธ์ 2569
วันที่เก็บตัวอย่าง (Collected Date)^c 12 กุมภาพันธ์ 2569 วิธีการเก็บตัวอย่าง (Sampling Method)^c เก็บแบบ จ้วง (Grab)

พารามิเตอร์ (Parameter)	หน่วย (Unit)	ผลการวิเคราะห์ (Result)	MDL	ค่ามาตรฐาน ^{1/} (Standard)	วิธีทดสอบ ^{4/} (Test Method)
		น้ำระวายน้ำ (ส่วนต้น)			
<i>Staphylococcus aureus</i>	per 100 mL	Not Detected	-	Not Detected	In-house method based on APHA, AWWA, WEF 24 th ed. 2023, 9213 B
<i>Pseudomonas aeruginosa</i>	per 100 mL	Not Detected	-	Not Detected	APHA, AWWA, WEF 24 th ed. 2023, 9213 E

หมายเหตุ : ^{1/} ค่าแนะนำของคณะกรรมการสาธารณสุข ฉบับที่ 1/2550 เรื่อง การควบคุมการประกอบกิจการระวายน้ำ หรือกิจการอื่นๆ ในพื้นที่ของเดิม

^{4/} Standard Methods for the Examination of Water and Wastewater, APHA, AWWA, WEF, 24th ed. 2023

^c เป็นข้อมูลที่ได้จากลูกค้า

- สภาพแวดล้อมของห้องปฏิบัติการ 25 ± 5 °C

- ห้องปฏิบัติการมีใบอนุญาตไม่ชักตัวอย่างเอง

(นายฐานันท์ นภารัตน์)
ผู้จัดการฝ่ายวิชาการ

(นางสาวทพพรรัตน์ วงศ์บุญตัน)
ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์
ทะเบียนเลขที่ ว-358-ค-0002

- รายงานผลการทดสอบนี้ได้รับรองเฉพาะตัวอย่างตามที่ได้รับมาทดสอบเท่านั้น
- ห้ามนำรายงานผลการทดสอบนี้ไปประกาศโฆษณา
- รายงานผลการทดสอบนี้ห้ามคัดลอกถ่ายทำสำเนาเฉพาะเพียงบางส่วน โดยไม่ได้รับอนุญาตจากห้องปฏิบัติการเป็นลายลักษณ์อักษร ยกเว้นทำหนังสือ




ANALYSIS REPORT

CUSTOMER NAME : เดอะ วัลลีย์ เขาใหญ่
ADDRESS : เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เขาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.
SAMPLING LOCATION : สระว่ายน้ำ (ส่วนลึก)
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : ใส ไม่มีตะกอน ไม่มีกลิ่น
SAMPLING DATE : FEBRUARY 12, 2026
SAMPLING TIME : 11:30
SAMPLING BY : นายโกวิท บุฬา
REPORT NO. : RN260210301
SAMPLING SOURCE : SWIMMING POOL
RECEIVED DATE : FEBRUARY 12, 2026
ANALYTICAL DATE : FEBRUARY 12-20, 2026
REPORT DATE : FEBRUARY 23, 2026

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD
Total Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	<10
<i>Escherichia Coli</i>	per 100 ml	E.coli Procedure Using Fluorogenic Substrate (SM: 9221 F.)	Not Detected	-	Not Detected

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED.,2023 (AWWA,APHA, WEF)

- Remark :
1. Recommendations of the Public Health Committee No. 1/2007 regarding the control of swimming pool operations or other businesses Likewise.
 2. ** mean analysis were performed by HVE Co.,Ltd .



(MR TAWATCHAI CHONGVUTICHA)

LABORATORY SUPERVISOR



บริษัท เอชวีอี จำกัด 603 ซอยจรัญสนิทวงศ์ 46 ถนนจรัญสนิทวงศ์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพฯ 10700
HVE CO. LTD. 603 Soi Jarunsnitwong 46 Jarunsnitwong Road Bangyeekan Bangplad Bangkok 10700
Tel : (02) 8834956-7 , (02) 8834274 Fax : (02) 8834956 E-mail address hv_eng@hotmail.com

รายงานผลการทดสอบ
(ANALYSIS REPORT)

รายงานหมายเลข (Report No.) 3360226 วันที่ (Date) 21 กุมภาพันธ์ 2569
ชื่อตัวอย่าง (Sample Name)^c น้ำระวายน้ำ (ส่วนลึก)
รหัสตัวอย่าง (Sample No.) No. 6902311
ลักษณะตัวอย่างทางกายภาพ^c ใส ไม่มีตะกอน
ชื่อลูกค้า (Customer name)^c บริษัท โอกลา เทสติ้ง แอนด์ คอนซัลติ้ง เซอร์วิส จำกัด (สำนักงานใหญ่)
สถานที่เก็บตัวอย่าง (Sampling site)^c Project TWL75
ที่อยู่ (Address)^c 63/13 ซอยเพชรเกษม 7 แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพฯ 10600
วันที่รับตัวอย่าง (Received Date) 12 กุมภาพันธ์ 2569 วันที่ตรวจวิเคราะห์ (Analysis Date) 12 กุมภาพันธ์ 2569 - 21 กุมภาพันธ์ 2569
วันที่เก็บตัวอย่าง (Collected Date)^c 12 กุมภาพันธ์ 2569 วิธีการเก็บตัวอย่าง (Sampling Method)^c เก็บแบบ จ้วง (Grab)

พารามิเตอร์ (Parameter)	หน่วย (Unit)	ผลการวิเคราะห์ (Result)	MDL	ค่ามาตรฐาน ^{1/} (Standard)	วิธีทดสอบ ^{4/} (Test Method)
		น้ำระวายน้ำ (ส่วนลึก)			
<i>Staphylococcus aureus</i>	per 100 mL	Not Detected	-	Not Detected	In-house method based on APHA, AWWA, WEF 24 th ed. 2023, 9213 B
<i>Pseudomonas aeruginosa</i>	per 100 mL	Not Detected	-	Not Detected	APHA, AWWA, WEF 24 th ed. 2023, 9213 E

หมายเหตุ : ^{1/} ค่าแนะนำของคณะกรรมการสาธารณสุข ฉบับที่ 1/2550 เรื่อง การควบคุมการประกอบกิจการระวายน้ำ หรือกิจการอื่นๆ ใน شأنของเสีย

^{4/} Standard Methods for the Examination of Water and Wastewater, APHA, AWWA, WEF, 24th ed. 2023

^c เป็นข้อมูลที่มาจากการสุ่ม

- สภาวะแวดล้อมของห้องปฏิบัติการ 25 ± 5 °C

- ห้องปฏิบัติการมีนโยบายไม่ชักตัวอย่างเอง

(นายฐานันท์ นิภารัตน์)
ผู้จัดการฝ่ายวิชาการ

(นางสาวทิพวรรณ วงศ์บุญตัน)
ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์
ทะเบียนเลขที่ ว-358-ค-0002

- รายงานผลการทดสอบนี้ใช้รับรองเฉพาะตัวอย่างตามที่ได้รับมาทดสอบเท่านั้น
- ห้ามนำรายงานผลการทดสอบนี้ไปประกาศโฆษณา
- รายงานผลการทดสอบนี้ห้ามคัดลอกถ่ายทำสำเนาเฉพาะเพียงบางส่วน โดยมิได้รับอนุญาตจากห้องปฏิบัติการเป็นลายลักษณ์อักษร ยกเว้นทำทั้งฉบับ



ANALYSIS REPORT

CUSTOMER NAME : เดอะ วัลลีย์ เขาใหญ่
ADDRESS : เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เขาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.
SAMPLING LOCATION : ถังแยกกากของระบบบำบัดน้ำเสีย อาคาร A
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : เหลืองเข้ม ขุ่นเล็กน้อย มีตะกอน มีกลิ่นเหม็นรุนแรง
SAMPLING DATE : MARCH 17, 2026
SAMPLING TIME : 11:00
SAMPLING BY : นายโกวิท บุฬา
REPORT NO. : RN260310558
SAMPLING SOURCE : WASTEWATER
RECEIVED DATE : MARCH 17, 2026
ANALYTICAL DATE : MARCH 17-30, 2026
REPORT DATE : MARCH 31, 2026

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
pH [#]	-	Electrometric (SM: 4500-H ⁺ B.)	8.0 at 25°C	-	-
Biochemical Oxygen Demand	mg/l	Membrane Electrode (SM: 4500-O ₂ G, 5210 B.)	46.6	2.0	-
Total Dissolved Solids [#]	mg/l	Total Dissolved Solids Dried at 180°C (SM: 2540 C.)	568.0	-	-
Total Suspended Solids [#]	mg/l	Total Suspended Solids Dried at 103-105°C (SM: 2540 D.)	40.0	-	-
Settleable Solids	ml/l	Settleable Solids (SM: 2540 F.)	<0.1	-	-
Sulfide as H ₂ S	mg/l	Iodometric (SM: 4500-S ²⁻ F.)	Not Detected	-	-
Total Kjeldahl Nitrogen	mg/l	Macro Kjeldahl (SM: 4500-N _{org} B)	23.0	-	-
Oil & Grease	mg/l	Liquid-Liquid Partition-Gravimetric (SM: 5520 B.)	3.4	1.4	-
Total Coliform Bacteria	MPN/100 ml	MPN Test	4.8 x 10 ⁵	-	-
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	1.6 x 10 ⁵	-	-

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED.,2023 (AWWA,APHA, WEF)

- Remark : 1. Notification of the Ministry of Natural Resources and Environment, dated June 28, B.E. 2567 (2024), which was published in the Royal Government Gazette, Vol. 141, Part 233D dated August 27, B.E. 2567 (2024) . (Category B)
2. [#] ISO/IEC 17025 ACCREDITED BY DEPARTMENT OF SCIENCE SERVICE (DSS)

(MR TAWATCHAI CHONGVUTICHAI)

LABORATORY SUPERVISOR




ANALYSIS REPORT

CUSTOMER NAME : เดอะ วัลลีย์ เขาใหญ่
ADDRESS : เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เขาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.
SAMPLING LOCATION : บ่อพักน้ำแรกหลังจากการระบบบำบัดน้ำเสีย อาคาร A
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : เหลืองเข้ม ขุ่นเล็กน้อย มีตะกอน มีกลิ่นเหม็นเล็กน้อย
SAMPLING DATE : MARCH 17, 2026
SAMPLING TIME : 11:00
SAMPLING BY : นายโกวิท บุฬา
REPORT NO. : RN260310559
SAMPLING SOURCE : WASTEWATER
RECEIVED DATE : MARCH 17, 2026
ANALYTICAL DATE : MARCH 17-30, 2026
REPORT DATE : MARCH 31, 2026

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
pH ^u	-	Electrometric (SM: 4500-H ⁺ B.)	8.1 at 25°C	-	5.5-9.0
Biochemical Oxygen Demand	mg/l	Membrane Electrode (SM: 4500-O G, 5210 B.)	21.8	2.0	≤30
Total Dissolved Solids ^u	mg/l	Total Dissolved Solids Dried at 180°C (SM: 2540 C.)	528.0	-	≤1,000
Total Suspended Solids ^u	mg/l	Total Suspended Solids Dried at 103-105°C (SM: 2540 D.)	35.0	-	≤40
Settleable Solids	ml/l	Settleable Solids (SM: 2540 F.)	<0.1	-	-
Sulfide as H ₂ S	mg/l	Iodometric (SM: 4500-S ²⁻ F.)	Not Detected	-	≤1.0
Total Kjeldahl Nitrogen	mg/l	Macro Kjeldahl (SM: 4500-N _{org} B)	13.0	-	<35
Oil & Grease	mg/l	Liquid-Liquid Partition-Gravimetric (SM: 5520 B.)	1.8	1.4	<20
Total Coliform Bacteria	MPN/100 ml	MPN Test	1.5 x 10 ⁵	-	-
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	9.0 x 10 ⁴	-	-

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED.,2023 (AWWA,APHA, WEF)

- Remark : 1. Notification of the Ministry of Natural Resources and Environment, dated June 28, B.E. 2567 (2024), which was published in the Royal Government Gazette, Vol. 141, Part 233D dated August 27, B.E. 2567 (2024) . (Category B)
2. [#] ISO/IEC 17025 ACCREDITED BY DEPARTMENT OF SCIENCE SERVICE (DSS)

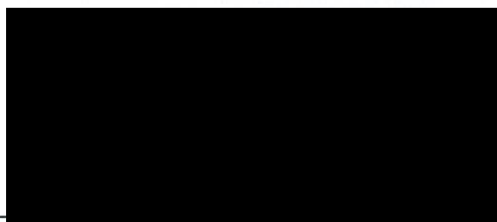

(MR TAWATCHAI CHONGVUTICHA)

LABORATORY SUPERVISOR




ANALYSIS REPORT

CUSTOMER NAME : เดอะ วัลลีย์ เขาใหญ่
ADDRESS : เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เขาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.
SAMPLING LOCATION : ถังแยกกากของระบบบำบัดน้ำเสีย อาคาร B
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : เหลืองอ่อน ชุ่นเล็กน้อย ไม่มีตะกอน ไม่มีกลิ่น
SAMPLING DATE : MARCH 17, 2026
SAMPLING TIME : 11:00
SAMPLING BY : นายไกรวิทย์ บุษหา
REPORT NO. : RN260310560
SAMPLING SOURCE : WASTEWATER
RECEIVED DATE : MARCH 17, 2026
ANALYTICAL DATE : MARCH 17-30, 2026
REPORT DATE : MARCH 31, 2026

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
pH [#]	-	Electrometric (SM: 4500-H ⁺ B.)	8.2 at 25°C	-	-
Biochemical Oxygen Demand	mg/l	Membrane Electrode (SM: 4500-O ₂ G, 5210 B.)	1.3	2.0	-
Total Dissolved Solids [#]	mg/l	Total Dissolved Solids Dried at 180°C (SM: 2540 C.)	576.0	-	-
Total Suspended Solids [#]	mg/l	Total Suspended Solids Dried at 103-105°C (SM: 2540 D.)	20.0	-	-
Settleable Solids	ml/l	Settleable Solids (SM: 2540 F.)	<0.1	-	-
Sulfide as H ₂ S	mg/l	Iodometric (SM: 4500-S ²⁻ F.)	Not Detected	-	-
Total Kjeldahl Nitrogen	mg/l	Macro Kjeldahl (SM: 4500-N _{org} B)	Not Detected	-	-
Oil & Grease	mg/l	Liquid-Liquid Partition-Gravimetric (SM: 5520 B.)	Not Detected	1.4	-
Total Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	-
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	-

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED.,2023 (AWWA,APHA, WEF)

- Remark : 1. Notification of the Ministry of Natural Resources and Environment, dated June 28, B.E. 2567 (2024), which was published in the Royal Government Gazette, Vol. 141, Part 233D dated August 27, B.E. 2567 (2024) . (Category B)
2. [#] ISO/IEC 17025 ACCREDITED BY DEPARTMENT OF SCIENCE SERVICE (DSS)



(MR TAWATCHAI CHONGVUTICHAJ)

LABORATORY SUPERVISOR



ANALYSIS REPORT


CUSTOMER NAME : เดอะ วัลลีย์ เขาใหญ่
ADDRESS : เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เขาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.
SAMPLING LOCATION : ป่อกักน้ำแรกหลังออกจากระบบบำบัดน้ำเสีย อาคาร B
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : เหลืองอ่อน ขุ่นเล็กน้อย ไม่มีตะกอน ไม่มีกลิ่น
SAMPLING DATE : MARCH 17, 2026
SAMPLING TIME : 11:00
SAMPLING BY : นายโกวิท บุฬา
REPORT NO. : RN260310561
SAMPLING SOURCE : WASTEWATER
RECEIVED DATE : MARCH 17, 2026
ANALYTICAL DATE : MARCH 17-30, 2026
REPORT DATE : MARCH 31, 2026

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
pH [#]	-	Electrometric (SM: 4500-H ⁺ B.)	8.3 at 25°C	-	5.5-9.0
Biochemical Oxygen Demand	mg/l	Membrane Electrode (SM: 4500-O ₂ G, 5210 B.)	1.6	2.0	≤30
Total Dissolved Solids [#]	mg/l	Total Dissolved Solids Dried at 180°C (SM: 2540 C.)	604.0	-	≤1,000
Total Suspended Solids	mg/l	Total Suspended Solids Dried at 103-105°C (SM: 2540 D.)	6.0	-	≤40
Settleable Solids	ml/l	Settleable Solids (SM: 2540 F.)	<0.1	-	-
Sulfide as H ₂ S	mg/l	Iodometric (SM: 4500-S ²⁻ F.)	Not Detected	-	≤1.0
Total Kjeldahl Nitrogen	mg/l	Macro Kjeldahl (SM: 4500-N _{org} B)	Not Detected	-	<35
Oil & Grease	mg/l	Liquid-Liquid Partition-Gravimetric (SM: 5520 B.)	Not Detected	1.4	<20
Total Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	-
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	-

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED.,2023 (AWWA,APHA, WEF)

Remark : 1. Notification of the Ministry of Natural Resources and Environment, dated June 28, B.E. 2567 (2024), which was published in the Royal Government Gazette, Vol. 141, Part 233D dated August 27, B.E. 2567 (2024) . (Category B)

2. [#] ISO/IEC 17025 ACCREDITED BY DEPARTMENT OF SCIENCE SERVICE (DSS)

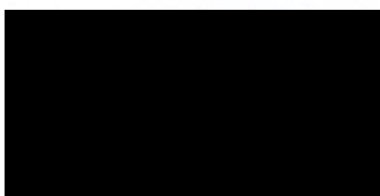

(MR TAWATCHAI CHONGVUTICHA)

LABORATORY SUPERVISOR



ห้องปฏิบัติการวิเคราะห์บริษัท โอกลา เทสติ้ง แอนด์ คอนซัลติง เซอร์วิส จำกัด

63/13 เพชรเกษม ซอย 7 แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพฯ 10600

Tel: 0 2868 1246 Fax: 0 2868 0860 www.okla-testing.com J-NAC Group



TESTING
No.0334

ANALYSIS REPORT


CUSTOMER NAME : เดอะ วัลลีย์ เขาใหญ่
ADDRESS : เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เขาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.
SAMPLING LOCATION : ถังแยกกากของระบบบำบัดน้ำเสีย อาคาร C
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : ไม่มีสี ใส ไม่มีตะกอน ไม่มีกลิ่น
SAMPLING DATE : MARCH 17, 2026
SAMPLING TIME : 11:00
SAMPLING BY : นายไกรวิทย์ บุษหา

REPORT NO. : RN260310562
SAMPLING SOURCE : WASTEWATER
RECEIVED DATE : MARCH 17, 2026
ANALYTICAL DATE : MARCH 17-30, 2026
REPORT DATE : MARCH 31, 2026

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD
pH [#]	-	Electrometric (SM: 4500-H ⁺ B.)	7.3 at 25°C	-	-
Biochemical Oxygen Demand	mg/l	Membrane Electrode (SM: 4500-O G, 5210 B.)	14.0	2.0	-
Total Dissolved Solids [#]	mg/l	Total Dissolved Solids Dried at 180°C (SM: 2540 C.)	692.0	-	-
Total Suspended Solids	mg/l	Total Suspended Solids Dried at 103-105°C (SM: 2540 D.)	Not Detected	-	-
Settleable Solids	ml/l	Settleable Solids (SM: 2540 F.)	<0.1	-	-
Sulfide as H ₂ S	mg/l	Iodometric (SM: 4500-S ²⁻ F.)	Not Detected	-	-
Total Kjeldahl Nitrogen	mg/l	Macro Kjeldahl (SM: 4500-N _{org} B)	5.9	-	-
Oil & Grease	mg/l	Liquid-Liquid Partition-Gravimetric (SM: 5520 B.)	Not Detected	1.4	-
Total Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	-
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	-

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED., 2023 (AWWA, APHA, WEF)

- Remark : 1. Notification of the Ministry of Natural Resources and Environment, dated June 28, B.E. 2567 (2024), which was published in the Royal Government Gazette, Vol. 141, Part 233D dated August 27, B.E. 2567 (2024) . (Category B)
2. [#] ISO/IEC 17025 ACCREDITED BY DEPARTMENT OF SCIENCE SERVICE (DSS)

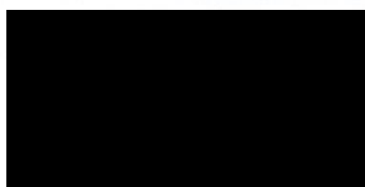

(MR TAWATCHAI CHONGVUTICHAJ)

LABORATORY SUPERVISOR

*** Reported analysis refers to submitted sample only. Report analysis shall not be reproduced except in full, without written approval of Laboratory. ***



ANALYSIS REPORT


CUSTOMER NAME : เดอะ วัลลีย์ เขาใหญ่
ADDRESS : เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เขาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.
SAMPLING LOCATION : บ่อพักน้ำแรกหลังจากการระบบบำบัดน้ำเสีย อาคาร C
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : ไม่มีสี ใส ไม่มีตะกอน ไม่มีกลิ่น
SAMPLING DATE : MARCH 17, 2026
SAMPLING TIME : 11:00
SAMPLING BY : นายไกรวิทย์ บุพผา

REPORT NO. : RN260310563
SAMPLING SOURCE : WASTEWATER
RECEIVED DATE : MARCH 17, 2026
ANALYTICAL DATE : MARCH 17-30, 2026
REPORT DATE : MARCH 31, 2026

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD *
pH [#]	-	Electrometric (SM: 4500-H ⁺ B.)	7.8 at 25°C	-	5.5-9.0
Biochemical Oxygen Demand	mg/l	Membrane Electrode (SM: 4500-O ₂ G, 5210 B.)	Not Detected	2.0	≤30
Total Dissolved Solids [#]	mg/l	Total Dissolved Solids Dried at 180°C (SM: 2540 C.)	310.0	-	≤1,000
Total Suspended Solids	mg/l	Total Suspended Solids Dried at 103-105°C (SM: 2540 D.)	4.0	-	≤40
Settleable Solids	ml/l	Settleable Solids (SM: 2540 F.)	<0.1	-	-
Sulfide as H ₂ S	mg/l	Iodometric (SM: 4500-S ²⁻ F.)	Not Detected	-	≤1.0
Total Kjeldahl Nitrogen	mg/l	Macro Kjeldahl (SM: 4500-N _{org} B.)	Not Detected	-	<35
Oil & Grease	mg/l	Liquid-Liquid Partition-Gravimetric (SM: 5520 B.)	Not Detected	1.4	<20
Total Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	-
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	-

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED., 2023 (AWWA, APHA, WEF)

- Remark : 1. * Notification of the Ministry of Natural Resources and Environment, dated June 28, B.E. 2567 (2024), which was published in the Royal Government Gazette, Vol. 141, Part 233D dated August 27, B.E. 2567 (2024) . (Category B)
2. [#] ISO/IEC 17025 ACCREDITED BY DEPARTMENT OF SCIENCE SERVICE (DSS)



LABORATORY SUPERVISOR



ANALYSIS REPORT

CUSTOMER NAME : เดอะ วัลลีย์ เขาใหญ่
ADDRESS : เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เขาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.
SAMPLING LOCATION : สระว่ายน้ำ (ส่วนต้น)
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER :ใส ไม่มีตะกอน ไม่มีกลิ่น
SAMPLING DATE : MARCH 17, 2026
SAMPLING TIME : 11:00
SAMPLING BY : นายโกวิท นุฬา
REPORT NO. : RN260310564
SAMPLING SOURCE : SWIMMING POOL
RECEIVED DATE : MARCH 17, 2026
ANALYTICAL DATE : MARCH 17-30, 2026
REPORT DATE : MARCH 31, 2026

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD
Total Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	<10
<i>Escherichia Coli</i>	per 100 ml	E.coli Procedure Using Fluorogenic Substrate (SM: 9221 F.)	Not Detected	-	Not Detected

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED.,2023 (AWWA,APHA, WEF)

- Remark :
- Recommendations of the Public Health Committee No. 1/2007 regarding the control of swimming pool operations or other businesses Likewise.
 - mean analysis were performed by HVE Co.,Ltd .

(MR TAWATCHAI CHONGVUTICHA)

LABORATORY SUPERVISOR



บริษัท เอชวีซี จำกัด 603 ซอยจรัญสนิทวงศ์ 46 ถนนจรัญสนิทวงศ์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพฯ 10700
HVE CO. LTD. 603 Sol Jarunsanitwong 46 Jarunsanitwong Road Bangyeeakan Bangplad Bangkok 10700
Tel : (02) 8834956-7 , (02) 8834274 Fax : (02) 8834956 E-mail address hv_eng@hotmail.com

รายงานผลการทดสอบ
(ANALYSIS REPORT)

รายงานหมายเลข (Report No.) 6080326 วันที่ (Date) 26 มีนาคม 2569
ชื่อตัวอย่าง (Sample Name)^c น้ำระเหยน้ำ (ส่วนต้น)
รหัสตัวอย่าง (Sample No.) No. 6903627
ลักษณะตัวอย่างทางกายภาพ^c ไม่มีสี ไม่มีตะกอน
ชื่อลูกค้า (Customer name)^c บริษัท โอกลา เทสต์ติ้ง แอนด์ คอนซัลติ้ง เซอร์วิส จำกัด (สำนักงานใหญ่)
สถานที่เก็บตัวอย่าง (Sampling site)^c Project TWL75
ที่อยู่ (Address)^c 63/13 ซอยเพชรเกษม 7 แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพฯ 10600
วันที่รับตัวอย่าง (Received Date) 17 มีนาคม 2569 วันที่ตรวจวิเคราะห์ (Analysis Date) 17 มีนาคม 2569 - 26 มีนาคม 2569
วันที่เก็บตัวอย่าง (Collected Date)^c 17 มีนาคม 2569 วิธีการเก็บตัวอย่าง (Sampling Method)^c เก็บแบบ จ้วง (Grab)

พารามิเตอร์ (Parameter)	หน่วย (Unit)	ผลการวิเคราะห์ (Result)	MDL	ค่ามาตรฐาน ^{1/} (Standard)	วิธีทดสอบ ^{4/} (Test Method)
		น้ำระเหยน้ำ (ส่วนต้น)			
<i>Staphylococcus aureus</i>	per 100 mL	Not Detected	-	Not Detected	In-house method based on APHA, AWWA, WEF 24 th ed. 2023, 9213 B
<i>Pseudomonas aeruginosa</i>	per 100 mL	Not Detected	-	Not Detected	APHA, AWWA, WEF 24 th ed. 2023, 9213 E

หมายเหตุ : ^{1/} ส่วนหนึ่งของคณะกรรมการสาธารณสุข ฉบับที่ 1/2550 เรื่อง การควบคุมการประกอบกิจการระเหยน้ำ หรือกิจการอื่นๆ ในทางของเสีย

^{4/} Standard Methods for the Examination of Water and Wastewater, APHA, AWWA, WEF, 24th ed. 2023

^c เป็นข้อมูลที่มาจากลูกค้า

- สภาวะแวดล้อมของห้องปฏิบัติการ 25 ± 5 °C
- ห้องปฏิบัติการมีนโยบายไม่รับตัวอย่างเอง

(นายธำนิษฐ์ นิภารัตน์)
ผู้จัดการฝ่ายวิชาการ

(นางสาวทิพวรรณ วงศ์บุญตัน)
ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์
ทะเบียนเลขที่ ว-358-ค-0002

- รายงานผลการทดสอบนี้ได้รับรองเฉพาะตัวอย่างตามที่ได้รับมาทดสอบเท่านั้น
- ห้ามนำรายงานผลการทดสอบนี้ไปประกาศโฆษณา
- รายงานผลการทดสอบนี้ห้ามคัดลอกถ่ายทำสำเนาเผยแพร่บางส่วน โดยไม่ได้รับอนุญาตจากห้องปฏิบัติการเป็นลายลักษณ์อักษร ยกเว้นทำทั้งหมด

ANALYSIS REPORT

CUSTOMER NAME : เดอะ วิลลีย์ เขาใหญ่
 ADDRESS : เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เขาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.
 SAMPLING LOCATION : สระว่ายน้ำ (ส่วนลึก)
 SAMPLING METHOD : GRAB
 SAMPLING CONDITION : NORMAL
 CHARACTERISTICS OF WATER : ใส ไม่มีตะกอน ไม่มีกลิ่น
 SAMPLING DATE : MARCH 17, 2026
 SAMPLING TIME : 11:00
 SAMPLING BY : นายโกวิท บุพา

REPORT NO. : RN260310565
 SAMPLING SOURCE : SWIMMING POOL
 RECEIVED DATE : MARCH 17, 2026
 ANALYTICAL DATE : MARCH 17-30, 2026
 REPORT DATE : MARCH 31, 2026

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD
Total Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	<10
<i>Escherichia Coli</i>	per 100 ml	E.coli Procedure Using Fluorogenic Substrate (SM: 9221 F.)	Not Detected	-	Not Detected

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED.,2023 (AWWA,APHA, WEF)

- Remark :
- Recommendations of the Public Health Committee No. 1/2007 regarding the control of swimming pool operations or other businesses Likewise.
 - ** mean analysis were performed by HVE Co.,Ltd .

(MR TAWATCHAI CHONGVUTICHA)

LABORATORY SUPERVISOR



บริษัท เอชวีอี จำกัด 603 ซอยเจริญสุขนิทวงศ์ 46 ถนนเจริญสุขนิทวงศ์ แขวงบางพลัด กรุงเทพฯ 10700
HVE CO. LTD. 603 Soi Jarunsanitwong 46 Jarunsanitwong Road Bangyeeek Bangkok 10700
Tel : (02) 8834956-7 , (02) 8834274 Fax : (02) 8834956 E-mail address hv_eng@hotmail.com

รายงานผลการทดสอบ
(ANALYSIS REPORT)

รายงานหมายเลข (Report No.) 6090326 วันที่ (Date) 26 มีนาคม 2569
ชื่อตัวอย่าง (Sample Name)^c น้ำระเหยน้ำ (ส่วนลึก)
รหัสตัวอย่าง (Sample No.) No. 6903628
ลักษณะตัวอย่างทางกายภาพ^c ไม่มีสี ไม่มีตะกอน
ชื่อลูกค้า (Customer name)^c บริษัท โอกลา เทสติ้ง แอนด์ คอนซัลติ้ง เซอร์วิส จำกัด (สำนักงานใหญ่)
สถานที่เก็บตัวอย่าง (Sampling site)^c Project TWL75
ที่อยู่ (Address)^c 63/13 ซอยเพชรเกษม 7 แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพฯ 10600
วันที่รับตัวอย่าง (Received Date) 17 มีนาคม 2569 วันที่ตรวจวิเคราะห์ (Analysis Date) 17 มีนาคม 2569 - 26 มีนาคม 2569
วันที่เก็บตัวอย่าง (Collected Date)^c 17 มีนาคม 2569 วิธีการเก็บตัวอย่าง (Sampling Method)^c เก็บแบบ จ้วง (Grab)

พารามิเตอร์ (Parameter)	หน่วย (Unit)	ผลการวิเคราะห์ (Result)	MDL	ค่ามาตรฐาน ^{1/} (Standard)	วิธีทดสอบ ^{4/} (Test Method)
		น้ำระเหยน้ำ (ส่วนลึก)			
<i>Staphylococcus aureus</i>	per 100 mL	Not Detected	-	Not Detected	In-house method based on APHA, AWWA, WEF 24 th ed. 2023, 9213 B
<i>Pseudomonas aeruginosa</i>	per 100 mL	Not Detected	-	Not Detected	APHA, AWWA, WEF 24 th ed. 2023, 9213 E

หมายเหตุ : ^{1/} ค่าแนะนำของคณะกรรมการสาธารณสุข ฉบับที่ 1/2550 เรื่อง การควบคุมการประกอบกิจการระเหยน้ำ เพื่อการดื่ม ในทางอนามัย

^{4/} Standard Methods for the Examination of Water and Wastewater, APHA, AWWA, WEF, 24th ed. 2023

^c เป็นข้อมูลที่ได้จากลูกค้า

- สภาวะแวดล้อมของห้องปฏิบัติการ 25 ± 5 °C

- ห้องปฏิบัติการมีนโยบายไม่ชักตัวอย่างเอง

(ลายเซ็น) [Redacted]
ผู้จัดการฝ่ายวิชาการ

ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์
ทะเบียนเลขที่ ว-358-ค-0002

- รายงานผลการทดสอบนี้ใช้รับรองเฉพาะตัวอย่างตามที่ได้รับมาทดสอบเท่านั้น
- ห้ามนำรายงานผลการทดสอบนี้ไปประกาศโฆษณา
- รายงานผลการทดสอบนี้ห้ามคัดลอกถ่ายทำสำเนาเฉพาะเพียงบางส่วน โดยไม่ได้รับอนุญาตจากห้องปฏิบัติการเป็นลายลักษณ์อักษร ยกเว้นทำทั้งฉบับ



ANALYSIS REPORT

CUSTOMER NAME : เดอะ วิลลีย์ เขาใหญ่
ADDRESS : เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เขาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.
SAMPLING LOCATION : ถังแยกกากของระบบบำบัดน้ำเสีย อาคาร A
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : เหลือง ขุ่นเล็กน้อย มีตะกอน มีกลิ่นเหม็นเล็กน้อย
SAMPLING DATE : APRIL 22, 2026
SAMPLING TIME : 11:00
SAMPLING BY : นายโกวิท บุนหา
REPORT NO. : RN260410764
SAMPLING SOURCE : WASTEWATER
RECEIVED DATE : APRIL 22, 2026
ANALYTICAL DATE : APRIL 22 - 30, 2026
REPORT DATE : May 4, 2026

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
pH [#]	-	Electrometric (SM: 4500-H ⁺ B.)	7.6 at 25°C	-	-
Biochemical Oxygen Demand	mg/l	Membrane Electrode (SM: 4500-O ₂ G, 5210 B.)	42.0	-	-
Total Dissolved Solids [#]	mg/l	Total Dissolved Solids Dried at 180°C (SM: 2540 C.)	372.0	-	-
Total Suspended Solids [#]	mg/l	Total Suspended Solids Dried at 103-105°C (SM: 2540 D.)	34.0	-	-
Settleable Solids	ml/l	Settleable Solids (SM: 2540 F.)	<0.1	-	-
Sulfide as H ₂ S	mg/l	Iodometric (SM: 4500-S ²⁻ F.)	Not Detected	-	-
Total Kjeldahl Nitrogen	mg/l	Macro Kjeldahl (SM: 4500-N _{org} B)	25.0	-	-
Oil & Grease	mg/l	Liquid-Liquid Partition-Gravimetric (SM: 5520 B.)	2.4	-	-
Total Coliform Bacteria	MPN/100 ml	MPN Test	2.9 × 10 ⁵	-	-
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	1.2 × 10 ⁵	-	-

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED.,2023 (AWWA,APHA, WEF)

- Remark : 1. * Notification of the Ministry of Natural Resources and Environment, dated June 28, B.E. 2567 (2024), which was published in the Royal Government Gazette, Vol. 141, Part 233D dated August 27, B.E. 2567 (2024) . (Category B)
2. [#] ISO/IEC 17025 ACCREDITED BY DEPARTMENT OF SCIENCE SERVICE (DSS)

(MR TAWATCHAI CHONGVUTICHA)

LABORATORY SUPERVISOR



ห้องปฏิบัติการวิเคราะห์บริษัท โอกลา เทสติ้ง แอนด์ คอนซัลติง เซอร์วิส จำกัด

63/13 เพชรเกษม ซอย 7 แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพฯ 10600

Tel: 0 2868 1246 Fax: 0 2868 0860 www.okla-testing.com J-NAC Group



TESTING
No.0334

ANALYSIS REPORT


CUSTOMER NAME : เดอะ วัลลีย์ เขาใหญ่
ADDRESS : เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เขาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.
SAMPLING LOCATION : บ่อพักน้ำแรกหลังจากจากระบบบำบัดน้ำเสีย อาคาร A
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : เหลือง ขุ่นเล็กน้อย ไม่มีตะกอน มีกลิ่นเหม็นเล็กน้อย
SAMPLING DATE : APRIL 22, 2026
SAMPLING TIME : 11:00
SAMPLING BY : นายโกวิท บุฬา

REPORT NO. : RN260410765
SAMPLING SOURCE : WASTEWATER
RECEIVED DATE : APRIL 22, 2026
ANALYTICAL DATE : APRIL 22 - 30, 2026
REPORT DATE : May 4, 2026

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
pH [#]	-	Electrometric (SM: 4500-H ⁺ B.)	8.1 at 25°C	-	5.5-9.0
Biochemical Oxygen Demand	mg/l	Membrane Electrode (SM: 4500-O G, 5210 B.)	18.0	-	≤30
Total Dissolved Solids [#]	mg/l	Total Dissolved Solids Dried at 180°C (SM: 2540 C.)	366.0	-	≤1,000
Total Suspended Solids [#]	mg/l	Total Suspended Solids Dried at 103-105°C (SM: 2540 D.)	20.0	-	≤40
Settleable Solids	ml/l	Settleable Solids (SM: 2540 F.)	<0.1	-	-
Sulfide as H ₂ S	mg/l	Iodometric (SM: 4500-S ²⁻ F.)	Not Detected	-	≤1.0
Total Kjeldahl Nitrogen	mg/l	Macro Kjeldahl (SM: 4500-N _{org} B)	13.0	-	<35
Oil & Grease	mg/l	Liquid-Liquid Partition-Gravimetric (SM: 5520 B.)	1.0	-	<20
Total Coliform Bacteria	MPN/100 ml	MPN Test	9.1 × 10 ³	-	-
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	430.0	-	-

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED.,2023 (AWWA,APHA, WEF)

- Remark : 1. * Notification of the Ministry of Natural Resources and Environment, dated June 28, B.E. 2567 (2024), which was published in the Royal Government Gazette, Vol. 141, Part 233D dated August 27, B.E. 2567 (2024) . (Category B)
2. [#] ISO/IEC 17025 ACCREDITED BY DEPARTMENT OF SCIENCE SERVICE (DSS)



(MR TAWATCHAI CHONGVUTICHA)

LABORATORY SUPERVISOR

*** Reported analysis refers to submitted sample only. Report analysis shall not be reproduced except in full, without written approval of Laboratory. ***



ANALYSIS REPORT

CUSTOMER NAME : เดอะ วิลลีย์ เขาใหญ่
ADDRESS : เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เขาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.
SAMPLING LOCATION : ถังแยกกากของระบบบำบัดน้ำเสีย อาคาร B
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : เหลืองใส มีตะกอน ไม่มีกลิ่น
SAMPLING DATE : APRIL 22, 2026
SAMPLING TIME : 11:00
SAMPLING BY : นายโกวิท บุฬา
REPORT NO. : RN260410766
SAMPLING SOURCE : WASTEWATER
RECEIVED DATE : APRIL 22, 2026
ANALYTICAL DATE : APRIL 22 - 30, 2026
REPORT DATE : May 4, 2026

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
pH [#]	-	Electrometric (SM: 4500-H ⁺ B.)	8.3 at 25°C	-	-
Biochemical Oxygen Demand	mg/l	Membrane Electrode (SM: 4500-O ₂ G, 5210 B.)	5.4	-	-
Total Dissolved Solids [#]	mg/l	Total Dissolved Solids Dried at 180°C (SM: 2540 C.)	428.0	-	-
Total Suspended Solids	mg/l	Total Suspended Solids Dried at 103-105°C (SM: 2540 D.)	Not Detected	-	-
Settleable Solids	ml/l	Settleable Solids (SM: 2540 F.)	<0.1	-	-
Sulfide as H ₂ S	mg/l	Iodometric (SM: 4500-S ²⁻ F.)	Not Detected	-	-
Total Kjeldahl Nitrogen	mg/l	Macro Kjeldahl (SM: 4500-N _{org} B)	2.2	-	-
Oil & Grease	mg/l	Liquid-Liquid Partition-Gravimetric (SM: 5520 B.)	Not Detected	-	-
Total Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	-
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	-

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED.,2023 (AWWA,APHA, WEF)

- Remark : 1. Notification of the Ministry of Natural Resources and Environment, dated June 28, B.E. 2567 (2024), which was published in the Royal Government Gazette, Vol. 141, Part 233D dated August 27, B.E. 2567 (2024) . (Category B)
2. [#] ISO/IEC 17025 ACCREDITED BY DEPARTMENT OF SCIENCE SERVICE (DSS)

(MR TAWATCHAI CHONGVUTICHA)

LABORATORY SUPERVISOR



ANALYSIS REPORT

CUSTOMER NAME : เดอะ วอลล์ เซาใหญ่
ADDRESS : เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เซาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.
SAMPLING LOCATION : บ่อพักน้ำแรกหลังจากการระบบบำบัดน้ำเสีย อาคาร B
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
REPORT NO. : RN260410767
CHARACTERISTICS OF WATER : เหลืองใส มีตะกอน ไม่มีกลิ่น
SAMPLING DATE : APRIL 22, 2026
SAMPLING TIME : 11:00
ANALYTICAL DATE : APRIL 22 - 30, 2026
SAMPLING BY : นายโกวิท นุฬา
REPORT DATE : May 4, 2026

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
pH [#]	-	Electrometric (SM: 4500-H ⁺ B.)	8.2 at 25°C	-	5.5-9.0
Biochemical Oxygen Demand	mg/l	Membrane Electrode (SM: 4500-O G, 5210 B.)	1.1	-	≤30
Total Dissolved Solids [#]	mg/l	Total Dissolved Solids Dried at 180°C (SM: 2540 C.)	397.0	-	≤1,000
Total Suspended Solids	mg/l	Total Suspended Solids Dried at 103-105°C (SM: 2540 D.)	Not Detected	-	≤40
Settleable Solids	ml/l	Settleable Solids (SM: 2540 F.)	<0.1	-	-
Sulfide as H ₂ S	mg/l	Iodometric (SM: 4500-S ²⁻ F.)	Not Detected	-	≤1.0
Total Kjeldahl Nitrogen	mg/l	Macro Kjeldahl (SM: 4500-N _{org} B.)	0.6	-	<35
Oil & Grease	mg/l	Liquid-Liquid Partition-Gravimetric (SM: 5520 B.)	Not Detected	-	<20
Total Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	-
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	-

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED.,2023 (AWWA,APHA, WEF)

Remark : 1. Notification of the Ministry of Natural Resources and Environment, dated June 28, B.E. 2567 (2024), which was published in the Royal Government Gazette, Vol. 141, Part 233D dated August 27, B.E. 2567 (2024) . (Category B)
2. [#] ISO/IEC 17025 ACCREDITED BY DEPARTMENT OF SCIENCE SERVICE (DSS)

(MR TAWATCHAI CHONGVUTICHAJ)

LABORATORY SUPERVISOR



ห้องปฏิบัติการวิเคราะห์บริษัท โอกลา เทสติ้ง แอนด์ คอนซัลติง เซอร์วิส จำกัด

63/13 เพชรเกษม ซอย 7 แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพฯ 10600

Tel: 0 2868 1246 Fax: 0 2868 0860 www.okla-testing.com J-NAC Group



TESTING
No.0334


ANALYSIS REPORT

CUSTOMER NAME : เดอะ วัลลีย์ เขาใหญ่
ADDRESS : เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เขาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.
SAMPLING LOCATION : ตั้งแยกจากของระบบบำบัดน้ำเสีย อาคาร C
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : เหลืองใส ไม่มีตะกอน ไม่มีกลิ่น
SAMPLING DATE : APRIL 22, 2026
SAMPLING TIME : 11:00
SAMPLING BY : นายโกวิท บุฬา
REPORT NO. : RN260410768
SAMPLING SOURCE : WASTEWATER
RECEIVED DATE : APRIL 22, 2026
ANALYTICAL DATE : APRIL 22 - 30, 2026
REPORT DATE : May 4, 2026

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
pH [#]	-	Electrometric (SM: 4500-H ⁺ B.)	7.7 at 25°C	-	-
Biochemical Oxygen Demand	mg/l	Membrane Electrode (SM: 4500-O ₂ G, 5210 B.)	25.5	-	-
Total Dissolved Solids [#]	mg/l	Total Dissolved Solids Dried at 180°C (SM: 2540 C.)	443.0	-	-
Total Suspended Solids	mg/l	Total Suspended Solids Dried at 103-105°C (SM: 2540 D.)	8.0	-	-
Settleable Solids	ml/l	Settleable Solids (SM: 2540 F.)	<0.1	-	-
Sulfide as H ₂ S	mg/l	Iodometric (SM: 4500-S ²⁻ F.)	Not Detected	-	-
Total Kjeldahl Nitrogen	mg/l	Macro Kjeldahl (SM: 4500-N _{org} B)	22.0	-	-
Oil & Grease	mg/l	Liquid-Liquid Partition-Gravimetric (SM: 5520 B.)	0.6	-	-
Total Coliform Bacteria	MPN/100 ml	MPN Test	910.0	-	-
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	430.0	-	-

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED.,2023 (AWWA,APHA, WEF)

- Remark : 1. * Notification of the Ministry of Natural Resources and Environment, dated June 28, B.E. 2567 (2024), which was published in the Royal Government Gazette, Vol. 141, Part 233D dated August 27, B.E. 2567 (2024) . (Category B)
2. [#] ISO/IEC 17025 ACCREDITED BY DEPARTMENT OF SCIENCE SERVICE (DSS)



(MR. TAWATCHAI CHONGVONHAI)

LABORATORY SUPERVISOR

*** Reported analysis refers to submitted sample only. Report analysis shall not be reproduced except in full, without written approval of Laboratory. ***



ANALYSIS REPORT


CUSTOMER NAME : เดอะ วัลลีย์ เขาใหญ่
ADDRESS : เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เขาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.
SAMPLING LOCATION : บ่อพักน้ำแรกหลังจากระบบบำบัดน้ำเสีย อาคาร C
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : ไม่มีสี ไส ไม่มีตะกอน ไม่มีกลิ่น
SAMPLING DATE : APRIL 22, 2026
SAMPLING TIME : 11:00
SAMPLING BY : นายโกวิท บุฬา

REPORT NO. : RN260410769
SAMPLING SOURCE : WASTEWATER
RECEIVED DATE : APRIL 22, 2026
ANALYTICAL DATE : APRIL 22 - 30, 2026
REPORT DATE : May 4, 2026

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
pH [#]	-	Electrometric (SM: 4500-H ⁺ B.)	7.4 at 25°C	-	5.5-9.0
Biochemical Oxygen Demand	mg/l	Membrane Electrode (SM: 4500-O G, 5210 B.)	13.0	-	≤30
Total Dissolved Solids [#]	mg/l	Total Dissolved Solids Dried at 180°C (SM: 2540 C.)	275.0	-	≤1,000
Total Suspended Solids	mg/l	Total Suspended Solids Dried at 103-105°C (SM: 2540 D.)	Not Detected	-	≤40
Settleable Solids	ml/l	Settleable Solids (SM: 2540 F.)	<0.1	-	-
Sulfide as H ₂ S	mg/l	Iodometric (SM: 4500-S ²⁻ F.)	Not Detected	-	≤1.0
Total Kjeldahl Nitrogen	mg/l	Macro Kjeldahl (SM: 4500-N _{org} B)	6.0	-	<35
Oil & Grease	mg/l	Liquid-Liquid Partition-Gravimetric (SM: 5520 B.)	0.8	-	<20
Total Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	-
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	-

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED.,2023 (AWWA,APHA, WEF)

Remark : 1. * Notification of the Ministry of Natural Resources and Environment, dated June 28, B.E. 2567 (2024), which was published in the Royal Government Gazette, Vol. 141, Part 233D dated August 27, B.E. 2567 (2024) . (Category B)
2. [#] ISO/IEC 17025 ACCREDITED BY DEPARTMENT OF SCIENCE SERVICE (DSS)



LABORATORY SUPERVISOR

ANALYSIS REPORT

CUSTOMER NAME	: เดอะ วิลลีย์ เขาใหญ่	REPORT NO.	: RN260410770
ADDRESS	: เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เขาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.	SAMPLING SOURCE	: SWIMMING POOL
SAMPLING LOCATION	: สระว่ายน้ำ (ส่วนต้น)	RECEIVED DATE	: APRIL 22, 2026
SAMPLING METHOD	: GRAB	ANALYTICAL DATE	: APRIL 22 - 30, 2026
SAMPLING CONDITION	: NORMAL	REPORT DATE	: May 4, 2026
CHARACTERISTICS OF WATER	:ใส ไม่มีตะกอน ไม่มีกลิ่น		
SAMPLING DATE	: APRIL 22, 2026		
SAMPLING TIME	: 11:00		
SAMPLING BY	: นายโกวิท บุฬา		

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD
Total Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	<10
<i>Escherichia Coli</i>	per 100 ml	E.coli Procedure Using Fluorogenic Substrate (SM: 9221 F.)	Not Detected	-	Not Detected

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED.,2023 (AWWA,APHA, WEF)

- Remark :
1. * Recommendations of the Public Health Committee No. 1/2007 regarding the control of swimming pool operations or other businesses Likewise.
 2. ** mean analysis were performed by HVE Co.,Ltd .

(MR TAWATCHAI CHONGVUTICHAI)

LABORATORY SUPERVISOR



บริษัท เอชวีอี จำกัด 603 ซอยเจริญสุขนิเวศ 46 ถนนเจริญสุขนิเวศ แขวงบางมด เขตบางพลัด กรุงเทพฯ 10700
HVE CO. LTD. 603 Sol Jarunsanitwong 46 Jarunsanitwong Road Bangyaeakan Bangplad Bangkok 10700
Tel : (02) 8834956-7 , (02) 8834274 Fax : (02) 8834956 E-mail address hv_eng@hotmail.com

รายงานผลการทดสอบ
(ANALYSIS REPORT)

รายงานหมายเลข (Report No.) 7300426 วันที่ (Date) 30 เมษายน 2569
ชื่อตัวอย่าง (Sample Name)^c น้ำสระว่ายน้ำ (ส่วนต้น)
รหัสตัวอย่าง (Sample No.) No. 6904718
ลักษณะตัวอย่างทางกายภาพ^cใส, ไม่มีตะกอน
ชื่อลูกค้า (Customer name)^c บริษัท โอกลา เทสดี้ง แอนด์ คอนซัลติ้ง เซอร์วิส จำกัด (สำนักงานใหญ่)
สถานที่เก็บตัวอย่าง (Sampling site)^c Project TWL75
ที่อยู่ (Address)^c 63/13 ซอยเพชรเกษม 7 แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพฯ 10600
วันที่รับตัวอย่าง (Received Date) 22 เมษายน 2569 วันที่ตรวจวิเคราะห์ (Analyse Date) 22 เมษายน 2569 - 30 เมษายน 2569
วันที่เก็บตัวอย่าง (Collected Date)^c 22 เมษายน 2569 วิธีการเก็บตัวอย่าง (Sampling Method)^c เก็บแบบ จ้วง (Grab)

พารามิเตอร์ (Parameter)	หน่วย (Unit)	ผลการวิเคราะห์ (Result)	MDL	ค่ามาตรฐาน ^{1/} (Standard)	วิธีทดสอบ ^{4/} (Test Method)
		น้ำสระว่ายน้ำ (ส่วนต้น)			
<i>Staphylococcus aureus</i>	per 100 mL	Not Detected	-	Not Detected	In-house method based on APHA, AWWA, WEF 24 th ed. 2023, 9213 B
<i>Pseudomonas aeruginosa</i>	per 100 mL	Not Detected	-	Not Detected	APHA, AWWA, WEF 24 th ed. 2023, 9213 E

หมายเหตุ : ^{1/} ค่าแนะนำของคณะกรรมการสาธารณสุข ฉบับที่ 1/2550 เรื่อง การควบคุมการประกอบกิจการสระว่ายน้ำ หรือกิจการอื่นๆ ในพื้นที่เดียวกัน

^{4/} Standard Methods for the Examination of Water and Wastewater, APHA, AWWA, WEF, 24th ed. 2023

^c เป็นข้อมูลที่ได้จากลูกค้า

- สภาวะแวดล้อมของห้องปฏิบัติการ 25 ± 5 °C

- ห้องปฏิบัติการมีนโยบายไม่ชักตัวอย่างเอง

(นายฐานันท์ นิภารัตน์)
ผู้จัดการฝ่ายวิชาการ

(นางสาวทิพวรรณ วงศ์บุญตัน)
ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์
ทะเบียนเลขที่ ว-358-ค-0002

- รายงานผลการทดสอบนี้ให้พร้อมเฉพาะตัวอย่างตามที่ได้รับมาทดสอบเท่านั้น
- ห้ามนำรายงานผลการทดสอบนี้ไปประกาศโฆษณา
- รายงานผลการทดสอบนี้ห้ามคัดลอกถ่ายทำสำเนาเฉพาะเพียงบางส่วน โดยไม่ได้รับอนุญาตจากห้องปฏิบัติการเป็นลายลักษณ์อักษร ยกเว้นทำทั้งหมด

ANALYSIS REPORT

CUSTOMER NAME : เดอะ วิลลีย์ เขาใหญ่
 ADDRESS : เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เขาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.
 SAMPLING LOCATION : สระว่ายน้ำ (ส่วนลึก)
 SAMPLING METHOD : GRAB
 SAMPLING CONDITION : NORMAL
 CHARACTERISTICS OF WATER : ใส ไม่มีตะกอน ไม่มีกลิ่น
 SAMPLING DATE : APRIL 22, 2026
 SAMPLING TIME : 11:00
 SAMPLING BY : นายโกวิท บุฬา

REPORT NO. : RN260410771
 SAMPLING SOURCE : SWIMMING POOL
 RECEIVED DATE : APRIL 22, 2026
 ANALYTICAL DATE : APRIL 22 - 30, 2026
 REPORT DATE : May 4, 2026

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD
Total Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	<10
<i>Escherichia Coli</i>	per 100 ml	E.coli Procedure Using Fluorogenic Substrate (SM: 9221 F.)	Not Detected	-	Not Detected

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED.,2023 (AWWA,APHA, WEF)

Remark :

- * Recommendations of the Public Health Committee No. 1/2007 regarding the control of swimming pool operations or other businesses Likewise.
- ** mean analysis were performed by HVE Co.,Ltd .

(MR TAWATCHAI CHONGVUTICHA)

LABORATORY SUPERVISOR

*** Reported analysis refers to submitted sample only. Report analysis shall not be reproduced except in full, without written approval of Laboratory. ***



บริษัท เอชวีอี จำกัด 603 ซอยเจริญสุขนิทวงศ์ 46 ถนนเจริญสุขนิทวงศ์ แขวงบางมด เขตบางพลัด กรุงเทพฯ 10700
HVE CO. LTD. 603 Soi Jarunsanitwong 46 Jarunsanitwong Road Bangyeeakan Bangplad Bangkok 10700
Tel : (02) 8834958-7 , (02) 8834274 Fax : (02) 8834958 E-mail address hv_eng@hotmail.com

รายงานผลการทดสอบ
(ANALYSIS REPORT)

รายงานหมายเลข (Report No.) 7310426 วันที่ (Date) 30 เมษายน 2569
ชื่อตัวอย่าง (Sample Name)^c น้ำระเหยน้ำ (ส่วนลึก)
รหัสตัวอย่าง (Sample No.) No. 6904719
ลักษณะตัวอย่างทางกายภาพ^c สี, ไม่มีตะกอน
ชื่อลูกค้า (Customer name)^c บริษัท โอกลา เทสต์ แอนด์ คอนซัลติ้ง เซอร์วิส จำกัด (สำนักงานใหญ่)
สถานที่เก็บตัวอย่าง (Sampling site)^c Project TWL75
ที่อยู่ (Address)^c 63/13 ซอยเพชรเกษม 7 แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพฯ 10600
วันที่รับตัวอย่าง (Received Date) 22 เมษายน 2569 วันที่ตรวจวิเคราะห์ (Analyse Date) 22 เมษายน 2569 - 30 เมษายน 2569
วันที่เก็บตัวอย่าง (Collected Date)^c 22 เมษายน 2569 วิธีการเก็บตัวอย่าง (Sampling Method)^c เก็บแบบ จ้วง (Grab)

พารามิเตอร์ (Parameter)	หน่วย (Unit)	ผลการวิเคราะห์ (Result)	MDL	ค่ามาตรฐาน ^{1/} (Standard)	วิธีทดสอบ ^{4/} (Test Method)
		น้ำระเหยน้ำ (ส่วนลึก)			
<i>Staphylococcus aureus</i>	per 100 mL	Not Detected	-	Not Detected	In-house method based on APHA, AWWA, WEF 24 th ed. 2023, 9213 B
<i>Pseudomonas aeruginosa</i>	per 100 mL	Not Detected	-	Not Detected	APHA, AWWA, WEF 24 th ed. 2023, 9213 E

หมายเหตุ : ^{1/} สำหรับของคณะกรรมการสาธารณสุข ฉบับที่ 1/2550 เรื่อง การควบคุมการประกอบกิจการระเหยน้ำ หรือกิจการอื่นๆ ในทางองค์เขากัน

^{4/} Standard Methods for the Examination of Water and Wastewater, APHA, AWWA, WEF, 24th ed. 2023

^c เป็นข้อมูลที่มาจากการสุ่ม

- สภาวะแวดล้อมของห้องปฏิบัติการ 25 ± 5 °C

- ห้องปฏิบัติการมีนโยบายไม่ใช้ตัวอย่างเอง

(ลายเซ็น) _____
ผู้จัดการฝ่ายวิชาการ

ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์
ทะเบียนเลขที่ ว-358-ค-0002

- รายงานผลการทดสอบนี้ใช้รับรองเฉพาะตัวอย่างตามที่ได้รับมาทดสอบเท่านั้น
- ห้ามนำรายงานผลการทดสอบนี้ไปประกาศโฆษณา
- รายงานผลการทดสอบนี้ห้ามคัดลอกถ่ายทำสำเนาเฉพาะเพียงบางส่วน โดยไม่ได้รับอนุญาตจากห้องปฏิบัติการเป็นลายลักษณ์อักษร ยกเว้นทำทั้งฉบับ




ANALYSIS REPORT

CUSTOMER NAME : เดอะ วิลลีย์ เขาใหญ่
ADDRESS : เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เขาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.
SAMPLING LOCATION : ถังแยกกากของระบบบำบัดน้ำเสีย อาคาร A
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : เหลือง ชุ่นเล็กน้อย มีตะกอน มีกลิ่นเหม็นรุนแรง
SAMPLING DATE : MAY 21, 2026
SAMPLING TIME : 11:30
SAMPLING BY : นายโกวิท นุหา
SAMPLE NO. : 05144
REPORT NO. : RN260590139
SAMPLING SOURCE : WASTEWATER
RECEIVED DATE : MAY 21, 2026
ANALYTICAL DATE : MAY 21 - 28, 2026
REPORT DATE : MAY 29, 2026

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
pH [#]	-	Electrometric (SM: 4500-H ⁺ B.)	8.1 at 25°C	-	-
Biochemical Oxygen Demand	mg/l	Membrane Electrode (SM: 4500-O G, 5210 B.)	37.3	-	-
Total Dissolved Solids [#]	mg/l	Total Dissolved Solids Dried at 180°C (SM: 2540 C.)	399.0	-	-
Total Suspended Solids [#]	mg/l	Total Suspended Solids Dried at 103-105°C (SM: 2540 D.)	37.0	-	-
Settleable Solids	ml/l	Settleable Solids (SM: 2540 F.)	<0.1	-	-
Sulfide as H ₂ S	mg/l	Iodometric (SM: 4500-S ²⁻ F.)	Not Detected	-	-
Total Kjeldahl Nitrogen	mg/l	Macro Kjeldahl (SM: 4500-N _{org} B)	19.0	-	-
Oil & Grease	mg/l	Liquid-Liquid Partition-Gravimetric (SM: 5520 B.)	1.8	-	-
Total Coliform Bacteria	MPN/100 ml	MPN Test	1.5 × 10 ⁵	-	-
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	9.0 × 10 ⁴	-	-

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED., 2023 (AWWA, APHA, WEF)

- Remark : 1. * Notification of the Ministry of Natural Resources and Environment, dated June 28, B.E. 2567 (2024), which was published in the Royal Government Gazette, Vol. 141, Part 233D dated August 27, B.E. 2567 (2024) . (Category B)
2. [#]ISO/IEC 17025 ACCREDITED BY DEPARTMENT OF SCIENCE SERVICE (DSS)

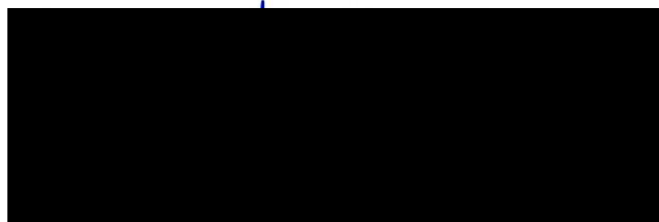

LABORATORY SUPERVISOR



ANALYSIS REPORT


CUSTOMER NAME : เดอะ วิลลีย์ เขาใหญ่
ADDRESS : เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เขาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.
SAMPLING LOCATION : บ่อกักน้ำแรกหลังออกจากระบบบำบัดน้ำเสีย อาคาร A
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : เหลืองใส ไม่มีตะกอน ไม่มีกลิ่น
SAMPLING DATE : MAY 21, 2026
SAMPLING TIME : 11:30
SAMPLING BY : นายโกวิท นุฬา

SAMPLE NO. : 05145
REPORT NO. : RN260590140
SAMPLING SOURCE : WASTEWATER
RECEIVED DATE : MAY 21, 2026
ANALYTICAL DATE : MAY 21 - 28, 2026
REPORT DATE : MAY 29, 2026

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
pH [#]	-	Electrometric (SM: 4500-H ⁺ B.)	8.0 at 25°C	-	5.5-9.0
Biochemical Oxygen Demand	mg/l	Membrane Electrode (SM: 4500-O ₂ G, 5210 B.)	24.9	-	≤30
Total Dissolved Solids [#]	mg/l	Total Dissolved Solids Dried at 180°C (SM: 2540 C.)	308.0	-	≤1,000
Total Suspended Solids [#]	mg/l	Total Suspended Solids Dried at 103-105°C (SM: 2540 D.)	10.0	-	≤40
Settleable Solids	ml/l	Settleable Solids (SM: 2540 F.)	<0.1	-	-
Sulfide as H ₂ S	mg/l	Iodometric (SM: 4500-S ²⁻ F.)	Not Detected	-	≤1.0
Total Kjeldahl Nitrogen	mg/l	Macro Kjeldahl (SM: 4500-N _{org} B)	15.0	-	<35
Oil & Grease	mg/l	Liquid-Liquid Partition-Gravimetric (SM: 5520 B.)	1.0	-	<20
Total Coliform Bacteria	MPN/100 ml	MPN Test	1.2 x 10 ⁵	-	-
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	7.5 x 10 ⁴	-	-

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED.,2023 (AWWA,APHA, WEF)

Remark : 1. Notification of the Ministry of Natural Resources and Environment, dated June 28, B.E. 2567 (2024), which was published in the Royal Government Gazette, Vol. 141, Part 233D dated August 27, B.E. 2567 (2024) . (Category B)
2. [#]ISO/IEC 17025 ACCREDITED BY DEPARTMENT OF SCIENCE SERVICE (DSS)



LABORATORY SUPERVISOR



ANALYSIS REPORT

CUSTOMER NAME : เดอะ วิลลีย์ เขาใหญ่
ADDRESS : เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เขาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.
SAMPLING LOCATION : ถังแยกกากของระบบบำบัดน้ำเสีย อาคาร B
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : เหลืองใส ไม่มีตะกอน ไม่มีกลิ่น
SAMPLING DATE : MAY 21, 2026
SAMPLING TIME : 11:30
SAMPLING BY : นายโกวิท บุฬา
SAMPLE NO. : 05146
REPORT NO. : RN260590141
SAMPLING SOURCE : WASTEWATER
RECEIVED DATE : MAY 21, 2026
ANALYTICAL DATE : MAY 21 - 28, 2026
REPORT DATE : MAY 29, 2026

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
pH [#]	-	Electrometric (SM: 4500-H ⁺ B.)	8.5 at 25°C	-	-
Biochemical Oxygen Demand	mg/l	Membrane Electrode (SM: 4500-O ₂ G, 5210 B.)	13.9	-	-
Total Dissolved Solids [#]	mg/l	Total Dissolved Solids Dried at 180°C (SM: 2540 C.)	458.0	-	-
Total Suspended Solids	mg/l	Total Suspended Solids Dried at 103-105°C (SM: 2540 D.)	4.0	-	-
Settleable Solids	ml/l	Settleable Solids (SM: 2540 F.)	<0.1	-	-
Sulfide as H ₂ S	mg/l	Iodometric (SM: 4500-S ²⁻ F.)	Not Detected	-	-
Total Kjeldahl Nitrogen	mg/l	Macro Kjeldahl (SM: 4500-N _{org} B)	6.7	-	-
Oil & Grease	mg/l	Liquid-Liquid Partition-Gravimetric (SM: 5520 B.)	Not Detected	-	-
Total Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	-
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	-

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED.,2023 (AWWA,APHA, WEF)

Remark : 1. * Notification of the Ministry of Natural Resources and Environment, dated June 28, B.E. 2567 (2024), which was published in the Royal Government Gazette, Vol. 141, Part 233D dated August 27, B.E. 2567 (2024) . (Category B)

2. [#]ISO/IEC 17025 ACCREDITED BY DEPARTMENT OF SCIENCE SERVICE (DSS)

(MR TAWATCHAI CHONGVUTICHA)

LABORATORY SUPERVISOR



ANALYSIS REPORT

CUSTOMER NAME : เดอะ วิลลีย์ เขาใหญ่
ADDRESS : เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เขาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.
SAMPLING LOCATION : บ่อกักน้ำแรกหลังออกจากระบบบำบัดน้ำเสีย อาคาร B
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : เหลืองใส ไม่มีตะกอน ไม่มีกลิ่น
SAMPLING DATE : MAY 21, 2026
SAMPLING TIME : 11:30
SAMPLING BY : นายโกวิท บุฬา
SAMPLE NO. : 05147
REPORT NO. : RN260590142
SAMPLING SOURCE : WASTEWATER
RECEIVED DATE : MAY 21, 2026
ANALYTICAL DATE : MAY 21 - 28, 2026
REPORT DATE : MAY 29, 2026

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
pH [#]	-	Electrometric (SM: 4500-H ⁺ B.)	8.0 at 25°C	-	5.5-9.0
Biochemical Oxygen Demand	mg/l	Membrane Electrode (SM: 4500-O G, 5210 B.)	8.9	-	≤30
Total Dissolved Solids [#]	mg/l	Total Dissolved Solids Dried at 180°C (SM: 2540 C.)	253.0	-	≤1,000
Total Suspended Solids	mg/l	Total Suspended Solids Dried at 103-105°C (SM: 2540 D.)	6.0	-	≤40
Settleable Solids	ml/l	Settleable Solids (SM: 2540 F.)	<0.1	-	-
Sulfide as H ₂ S	mg/l	Iodometric (SM: 4500-S ²⁻ F.)	Not Detected	-	≤1.0
Total Kjeldahl Nitrogen	mg/l	Macro Kjeldahl (SM: 4500-N _{org} B)	3.6	-	<35
Oil & Grease	mg/l	Liquid-Liquid Partition-Gravimetric (SM: 5520 B.)	Not Detected	-	<20
Total Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	-
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	-

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED., 2023 (AWWA, APHA, WEF)

- Remark : 1. * Notification of the Ministry of Natural Resources and Environment, dated June 28, B.E. 2567 (2024), which was published in the Royal Government Gazette, Vol. 141, Part 233D dated August 27, B.E. 2567 (2024) . (Category B)
2. [#] ISO/IEC 17025 ACCREDITED BY DEPARTMENT OF SCIENCE SERVICE (DSS)

(MR TAWATCHAI CHONGVUTICHA)

LABORATORY SUPERVISOR




ANALYSIS REPORT

CUSTOMER NAME : เดอะ วิลลีย์ เขาใหญ่
ADDRESS : เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เขาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.
SAMPLING LOCATION : ถังแยกกากของระบบบำบัดน้ำเสีย อาคาร C
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : เหลืองใส ไม่มีตะกอน ไม่มีกลิ่น
SAMPLING DATE : MAY 21, 2026
SAMPLING TIME : 11:30
SAMPLING BY : นายโกวิท บุหา
SAMPLE NO. : 05148
REPORT NO. : RN260590143
SAMPLING SOURCE : WASTEWATER
RECEIVED DATE : MAY 21, 2026
ANALYTICAL DATE : MAY 21 - 28, 2026
REPORT DATE : MAY 29, 2026

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
pH [#]	-	Electrometric (SM: 4500-H ⁺ B.)	7.8 at 25°C	-	-
Biochemical Oxygen Demand	mg/l	Membrane Electrode (SM: 4500-O G, 5210 B.)	19.6	-	-
Total Dissolved Solids [#]	mg/l	Total Dissolved Solids Dried at 180°C (SM: 2540 C.)	370.0	-	-
Total Suspended Solids	mg/l	Total Suspended Solids Dried at 103-105°C (SM: 2540 D.)	9.0	-	-
Settleable Solids	ml/l	Settleable Solids (SM: 2540 F.)	<0.1	-	-
Sulfide as H ₂ S	mg/l	Iodometric (SM: 4500-S ²⁻ F.)	Not Detected	-	-
Total Kjeldahl Nitrogen	mg/l	Macro Kjeldahl (SM: 4500-N _{org} B)	9.0	-	-
Oil & Grease	mg/l	Liquid-Liquid Partition-Gravimetric (SM: 5520 B.)	0.4	-	-
Total Coliform Bacteria	MPN/100 ml	MPN Test	910.0	-	-
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	150.0	-	-

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED., 2023 (AWWA, APHA, WEF)

- Remark : 1. * Notification of the Ministry of Natural Resources and Environment, dated June 28, B.E. 2567 (2024), which was published in the Royal Government Gazette, Vol. 141, Part 233D dated August 27, B.E. 2567 (2024) . (Category B)
2. # ISO/IEC 17025 ACCREDITED BY DEPARTMENT OF SCIENCE SERVICE (DSS)



(MR TAWATCHAI CHONGVUTICHAJ)

LABORATORY SUPERVISOR




ANALYSIS REPORT

CUSTOMER NAME : เดอะ วิลลีย์ เขาใหญ่
ADDRESS : เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เขาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.
SAMPLING LOCATION : บ่อพักน้ำแรกหลังออกจากระบบบำบัดน้ำเสีย อาคาร C
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : ไม่มีสี ไม่มีตะกอน ไม่มีกลิ่น
SAMPLING DATE : MAY 21, 2026
SAMPLING TIME : 11:30
SAMPLING BY : นายโกวิท บุฬา
SAMPLE NO. : 05149
REPORT NO. : RN260590144
SAMPLING SOURCE : WASTEWATER
RECEIVED DATE : MAY 21, 2026
ANALYTICAL DATE : MAY 21 - 28, 2026
REPORT DATE : MAY 29, 2026

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
pH [#]	-	Electrometric (SM: 4500-H ⁺ B.)	7.8 at 25°C	-	5.5-9.0
Biochemical Oxygen Demand	mg/l	Membrane Electrode (SM: 4500-O ₂ G, 5210 B.)	0.6	-	≤30
Total Dissolved Solids [#]	mg/l	Total Dissolved Solids Dried at 180°C (SM: 2540 C.)	373.0	-	≤1,000
Total Suspended Solids	mg/l	Total Suspended Solids Dried at 103-105°C (SM: 2540 D.)	3.0	-	≤40
Settleable Solids	ml/l	Settleable Solids (SM: 2540 F.)	<0.1	-	-
Sulfide as H ₂ S	mg/l	Iodometric (SM: 4500-S ²⁻ F.)	Not Detected	-	≤1.0
Total Kjeldahl Nitrogen	mg/l	Macro Kjeldahl (SM: 4500-N _{org} B)	Not Detected	-	<35
Oil & Grease	mg/l	Liquid-Liquid Partition-Gravimetric (SM: 5520 B.)	Not Detected	-	<20
Total Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	-
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	-

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED., 2023 (AWWA, APHA, WEF)

- Remark : 1. * Notification of the Ministry of Natural Resources and Environment, dated June 28, B.E. 2567 (2024), which was published in the Royal Government Gazette, Vol. 141, Part 233D dated August 27, B.E. 2567 (2024) . (Category B)
2. [#] ISO/IEC 17025 ACCREDITED BY DEPARTMENT OF SCIENCE SERVICE (DSS)

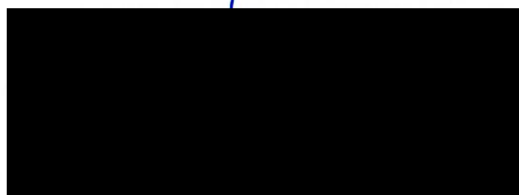

LABORATORY SUPERVISOR



ANALYSIS REPORT

CUSTOMER NAME : เดอะ วิลลีย์ เขาใหญ่
ADDRESS : เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เขาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.
SAMPLING LOCATION : สระว่ายน้ำ (ส่วนต้น)
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER :ใส ไม่มีตะกอน ไม่มีกลิ่น
SAMPLING DATE : MAY 21, 2026
SAMPLING TIME : 11:30
SAMPLING BY : นายโกวิท บุฬา
SAMPLE NO. : 05150
REPORT NO. : RN260590145
SAMPLING SOURCE : SWIMMING POOL
RECEIVED DATE : MAY 21, 2026
ANALYTICAL DATE : MAY 21 - 28, 2026
REPORT DATE : MAY 29, 2026

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD
Total Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	<10
<i>Escherichia Coli</i>	per 100 ml	E.coli Procedure Using Fluorogenic Substrate (SM: 9221 F.)	Not Detected	-	Not Detected

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED.,2023 (AWWA,APHA, WEF)

- Remark :
1. Recommendations of the Public Health Committee No. 1/2007 regarding the control of swimming pool operations or other businesses Likewise.
 2. ** mean analysis were performed by HVE Co.,Ltd .



(MR TAWATCHAI CHONGVUTICHA)

LABORATORY SUPERVISOR



บริษัท เอชวีอี จำกัด 603 ซอยจรัญสนิทวงศ์ 46 ถนนจรัญสนิทวงศ์ แขวงบางปี้น เขตบางพลัด กรุงเทพฯ 10700
HVE CO. LTD. 603 Soi Jarunsanitwong 46 Jarunsanitwong Road Bangyeekan Bangplad Bangkok 10700
Tel : (02) 8834956-7 , (02) 8834274 Fax : (02) 8834956 E-mail address hv_eng@hotmail.com

รายงานผลการทดสอบ
(ANALYSIS REPORT)

รายงานหมายเลข (Report No.) 9130526 วันที่ (Date) 30 พฤษภาคม 2569
ชื่อตัวอย่าง (Sample Name)^c น้ำระวายน้ำ (ส่วนต้น)
รหัสตัวอย่าง (Sample No.) No. 6905954
ลักษณะตัวอย่างทางกายภาพ^c ไม่มีสี ไม่มีตะกอน
ชื่อลูกค้า (Customer name)^c บริษัท โอกลา เทสดัง แอนด์ คอนซัลตัง เซอร์วิส จำกัด (สำนักงานใหญ่)
สถานที่เก็บตัวอย่าง (Sampling site)^c Project TWL75
ที่อยู่ (Address)^c 63/13 ซอยเพชรเกษม 7 แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพฯ 10600
วันที่รับตัวอย่าง (Received Date) 21 พฤษภาคม 2569 วันที่ตรวจวิเคราะห์ (Analyse Date) 21 พฤษภาคม 2569 - 30 พฤษภาคม 2569
วันที่เก็บตัวอย่าง (Collected Date)^c 21 พฤษภาคม 2569 วิธีการเก็บตัวอย่าง (Sampling Method)^c เก็บแบบ จ้วง (Grab)

พารามิเตอร์ (Parameter)	หน่วย (Unit)	ผลการวิเคราะห์ (Result)	MDL	ค่ามาตรฐาน ^{1/} (Standard)	วิธีทดสอบ ^{4/} (Test Method)
		น้ำระวายน้ำ (ส่วนต้น)			
<i>Staphylococcus aureus</i>	per 100 mL	Not Detected	-	Not Detected	In-house method based on APHA, AWWA, WEF 24 th ed. 2023, 9213 B
<i>Pseudomonas aeruginosa</i>	per 100 mL	Not Detected	-	Not Detected	APHA, AWWA, WEF 24 th ed. 2023, 9213 E

หมายเหตุ : ^{1/} ค่าแนะนำของคณะกรรมการสาธารณสุข ฉบับที่ 1/2550 เรื่อง การควบคุมการประกอบกิจการระวายน้ำ หรือกิจการอื่นๆ ในทางอนามัย

^{4/} Standard Methods for the Examination of Water and Wastewater, APHA, AWWA, WEF, 24th ed. 2023

^c เป็นข้อมูลที่มาจากรหัส

- สภาวะแวดล้อมของห้องปฏิบัติการ $25 \pm 5^{\circ}\text{C}$

- ห้องปฏิบัติการมีนโยบายไม่ใช้ตัวอย่างเอง

(นายฐานันท์ นิภารัตน์)
ผู้จัดการฝ่ายวิชาการ

(นางสาวพพรพรเย็น วงศ์บุญตัน)
ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์
ทะเบียนเลขที่ ว-358-ค-0002

- รายงานผลการทดสอบนี้ใช้รับรองเฉพาะตัวอย่างตามที่ได้รับมาทดสอบเท่านั้น
- ห้ามนำรายงานผลการทดสอบนี้ไปประกาศโฆษณา
- รายงานผลการทดสอบนี้ห้ามคัดลอกถ่ายทำสำเนาเฉพาะเพียงบางส่วน โดยไม่ได้รับอนุญาตจากห้องปฏิบัติการเป็นลายลักษณ์อักษร ยกเว้นทำทั้งหมด


ANALYSIS REPORT

CUSTOMER NAME	: เดอะ วิลลีย์ เขาใหญ่	SAMPLE NO.	: 05151
ADDRESS	: เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เขาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.	REPORT NO.	: RN260590146
SAMPLING LOCATION	: สระว่ายน้ำ (ส่วนเล็ก)	SAMPLING SOURCE	: SWIMMING POOL
SAMPLING METHOD	: GRAB	RECEIVED DATE	: MAY 21, 2026
SAMPLING CONDITION	: NORMAL	ANALYTICAL DATE	: MAY 21 - 28, 2026
CHARACTERISTICS OF WATER	: ใส ไม่มีตะกอน ไม่มีกลิ่น	REPORT DATE	: MAY 29, 2026
SAMPLING DATE	: MAY 21, 2026		
SAMPLING TIME	: 11:30		
SAMPLING BY	: นายโกวิท บุนหา		

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD
Total Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	<10
<i>Escherichia Coli</i>	per 100 ml	E.coli Procedure Using Fluorogenic Substrate (SM: 9221 F.)	Not Detected	-	Not Detected

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED., 2023 (AWWA, APHA, WEF)

- Remark :
- * Recommendations of the Public Health Committee No. 1/2007 regarding the control of swimming pool operations or other businesses Likewise.
 - ** mean analysis were performed by HVE Co.,Ltd .



(MR. PAWATCHAI CHONGVONHACHAI)

LABORATORY SUPERVISOR



บริษัท เอชวีอี จำกัด 603 ซอยเจริญสุขนิทวงศ์ 46 ถนนเจริญสุขนิทวงศ์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพฯ 10700
HVE CO. LTD. 603 Sol Jarunsanitwong 46 Jarunsanitwong Road Bangyeekan Bangplad Bangkok 10700
Tel : (02) 8834956-7 , (02) 8834274 Fax : (02) 8834956 E-mail address hv_eng@hotmail.com

รายงานผลการทดสอบ
(ANALYSIS REPORT)

รายงานหมายเลข (Report No.) 9140526 วันที่ (Date) 30 พฤษภาคม 2569
ชื่อตัวอย่าง (Sample Name)^c น้ำสระว่ายน้ำ (ส่วนลึก)
รหัสตัวอย่าง (Sample No.) No. 6905955
ลักษณะตัวอย่างทางกายภาพ^c ไม่ฟุ้ง ไม่มีตะกอน
ชื่อลูกค้า (Customer name)^c บริษัท โอกลา เทสติ้ง แอนด์ คอนซัลติ้ง เซอร์วิส จำกัด (สำนักงานใหญ่)
สถานที่เก็บตัวอย่าง (Sampling site)^c Project TWL75
ที่อยู่ (Address)^c 63/13 ซอยเพชรเกษม 7 แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพฯ 10600
วันที่รับตัวอย่าง (Received Date) 21 พฤษภาคม 2569 วันที่ตรวจวิเคราะห์ (Analyse Date) 21 พฤษภาคม 2569 - 30 พฤษภาคม 2569
วันที่เก็บตัวอย่าง (Collected Date)^c 21 พฤษภาคม 2569 วิธีการเก็บตัวอย่าง (Sampling Method)^c เก็บแบบ จ้วง (Grab)

พารามิเตอร์ (Parameter)	หน่วย (Unit)	ผลการวิเคราะห์ (Result)	MDL	ค่ามาตรฐาน ^{1/} (Standard)	วิธีทดสอบ ^{4/} (Test Method)
		น้ำสระว่ายน้ำ (ส่วนลึก)			
<i>Staphylococcus aureus</i>	per 100 mL	Not Detected	-	Not Detected	In-house method based on APHA, AWWA, WEF 24 th ed. 2023, 9213 B
<i>Pseudomonas aeruginosa</i>	per 100 mL	Not Detected	-	Not Detected	APHA, AWWA, WEF 24 th ed. 2023, 9213 E

หมายเหตุ : ^{1/} สำเนาของคณะกรรมการมาตรฐาน เลขที่ 1/2550 เรื่อง การควบคุมการประกอบกิจการสระว่ายน้ำ หรือกิจการอื่นๆ ในทางองเดียวกัน

^{4/} Standard Methods for the Examination of Water and Wastewater, APHA, AWWA, WEF, 24th ed. 2023

^c เป็นข้อมูลที่มาจากลูกค้า

- สภาวะแวดล้อมของห้องปฏิบัติการ 25 ± 5 °C

- ห้องปฏิบัติการมีนโยบายไม่ใช้ตัวอย่างเอง

(นายฐาณันท์ นามวงศ์)
ผู้จัดการฝ่ายวิชาการ

ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์
ทะเบียนเลขที่ ว-358-ค-0002

- รายงานผลการทดสอบให้ใช้รับรองเฉพาะตัวอย่างตามที่ได้รับมาทดสอบเท่านั้น
- ห้ามนำรายงานผลการทดสอบนี้ไปประกาศโฆษณา
- รายงานผลการทดสอบนี้ห้ามคัดลอกถ่ายทำสำเนาเฉพาะเพียงบางส่วน โดยไม่ได้รับอนุญาตจากห้องปฏิบัติการเป็นลายลักษณ์อักษร ยกเว้นทำทั้งฉบับ



ANALYSIS REPORT


CUSTOMER NAME : เดอะ วัลลีย์ เขาใหญ่
ADDRESS : เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เขาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.
SAMPLING LOCATION : ถังแยกกากของระบบบำบัดน้ำเสีย อาคาร A
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : เหลือง ขุ่นเล็กน้อย มีตะกอน มีกลิ่นเหม็นรุนแรง
SAMPLING DATE : JUNE 11, 2026
SAMPLING TIME : 10:30
SAMPLING BY : นายโกวิท บุฬา
SAMPLE NO. : 06128
REPORT NO. : RN260690127
SAMPLING SOURCE : WASTEWATER
RECEIVED DATE : JUNE 12, 2026
ANALYTICAL DATE : JUNE 12 - 18, 2026
REPORT DATE : JUNE 19, 2026

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
pH [#]	-	Electrometric (SM: 4500-H ⁺ B.)	8.1 at 25°C	-	-
Biochemical Oxygen Demand	mg/l	Membrane Electrode (SM: 4500-O G, 5210 B.)	35.0	-	-
Total Dissolved Solids [#]	mg/l	Total Dissolved Solids Dried at 180°C (SM: 2540 C.)	618.0	-	-
Total Suspended Solids [#]	mg/l	Total Suspended Solids Dried at 103-105°C (SM: 2540 D.)	24.0	-	-
Settleable Solids	ml/l	Settleable Solids (SM: 2540 F.)	<0.1	-	-
Sulfide as H ₂ S	mg/l	Iodometric (SM: 4500-S ²⁻ F.)	Not Detected	-	-
Total Kjeldahl Nitrogen	mg/l	Macro Kjeldahl (SM: 4500-N _{org} B)	15.0	-	-
Oil & Grease	mg/l	Liquid-Liquid Partition-Gravimetric (SM: 5520 B.)	2.4	-	-
Total Coliform Bacteria	MPN/100 ml	MPN Test	2.4 x 10 ⁵	-	-
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	1.6 x 10 ⁵	-	-

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED., 2023 (AWWA, APHA, WEF)

Remark : 1. Notification of the Ministry of Natural Resources and Environment, dated June 28, B.E. 2567 (2024), which was published in the Royal Government Gazette, Vol. 141, Part 233D dated August 27, B.E. 2567 (2024) . (Category B)

2. [#]ISO/IEC 17025 ACCREDITED BY DEPARTMENT OF SCIENCE SERVICE (DSS)

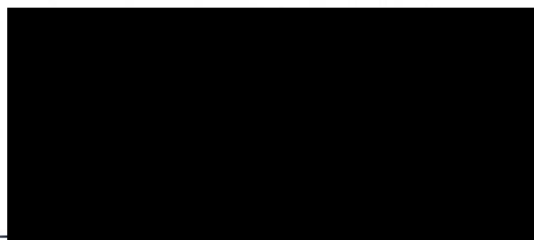

(MR TAWATCHAI CHONGVUTICHAJ)

LABORATORY SUPERVISOR



ห้องปฏิบัติการวิเคราะห์บริษัท โอกลา เทสติ้ง แอนด์ คอนซัลติง เซอร์วิส จำกัด

63/13 เพชรเกษม ซอย 7 แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพฯ 10600

Tel: 0 2868 1246 Fax: 0 2868 0860 www.okla-testing.com J-NAC Group



TESTING
No.0334

ANALYSIS REPORT

CUSTOMER NAME : เดอะ วัลลีย์ เขาใหญ่
ADDRESS : เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เขาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.
SAMPLING LOCATION : บ่อกักน้ำแรกหลังออกจากระบบบำบัดน้ำเสีย อาคาร A
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : เหลือง ขุ่นเล็กน้อย มีตะกอน มีกลิ่นเหม็นเล็กน้อย
SAMPLING DATE : JUNE 11, 2026
SAMPLING TIME : 10:30
SAMPLING BY : นายโกวิท บุญหา
SAMPLE NO. : 06129
REPORT NO. : RN260690128
SAMPLING SOURCE : WASTEWATER
RECEIVED DATE : JUNE 12, 2026
ANALYTICAL DATE : JUNE 12 - 18, 2026
REPORT DATE : JUNE 19, 2026

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
pH [#]	-	Electrometric (SM: 4500-H ⁺ B.)	8.3 at 25°C	-	5.5-9.0
Biochemical Oxygen Demand	mg/l	Membrane Electrode (SM: 4500-O G, 5210 B.)	11.0	-	≤30
Total Dissolved Solids [#]	mg/l	Total Dissolved Solids Dried at 180°C (SM: 2540 C.)	568.0	-	≤1,000
Total Suspended Solids [#]	mg/l	Total Suspended Solids Dried at 103-105°C (SM: 2540 D.)	36.0	-	≤40
Settleable Solids	ml/l	Settleable Solids (SM: 2540 F.)	<0.1	-	-
Sulfide as H ₂ S	mg/l	Iodometric (SM: 4500-S ²⁻ F.)	Not Detected	-	≤1.0
Total Kjeldahl Nitrogen	mg/l	Macro Kjeldahl (SM: 4500-N _{org} B)	4.8	-	<35
Oil & Grease	mg/l	Liquid-Liquid Partition-Gravimetric (SM: 5520 B.)	2.8	-	<20
Total Coliform Bacteria	MPN/100 ml	MPN Test	2.1 × 10 ⁵	-	-
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	1.2 × 10 ⁵	-	-

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED.,2023 (AWWA,APHA, WEF)

- Remark : 1. * Notification of the Ministry of Natural Resources and Environment, dated June 28, B.E. 2567 (2024), which was published in the Royal Government Gazette, Vol. 141, Part 233D dated August 27, B.E. 2567 (2024) . (Category B)
2. [#] ISO/IEC 17025 ACCREDITED BY DEPARTMENT OF SCIENCE SERVICE (DSS)



LABORATORY SUPERVISOR

*** Reported analysis refers to submitted sample only. Report analysis shall not be reproduced except in full, without written approval of Laboratory. ***



ANALYSIS REPORT

CUSTOMER NAME : เดอะ วิลลีย์ เขาใหญ่
ADDRESS : เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เขาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.
SAMPLING LOCATION : ถังแยกกากของระบบบำบัดน้ำเสีย อาคาร B
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : เหลืองใส มีตะกอนเล็กน้อย ไม่มีกลิ่น
SAMPLING DATE : JUNE 11, 2026
SAMPLING TIME : 10:30
SAMPLING BY : นายโกวิท บุญหา
SAMPLE NO. : 06130
REPORT NO. : RN260690129
SAMPLING SOURCE : WASTEWATER
RECEIVED DATE : JUNE 12, 2026
ANALYTICAL DATE : JUNE 12 - 18, 2026
REPORT DATE : JUNE 19, 2026

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
pH [#]	-	Electrometric (SM: 4500-H ⁺ B.)	8.2 at 25°C	-	-
Biochemical Oxygen Demand	mg/l	Membrane Electrode (SM: 4500-O G, 5210 B.)	4.9	-	-
Total Dissolved Solids [#]	mg/l	Total Dissolved Solids Dried at 180°C (SM: 2540 C.)	343.0	-	-
Total Suspended Solids	mg/l	Total Suspended Solids Dried at 103-105°C (SM: 2540 D.)	6.0	-	-
Settleable Solids	ml/l	Settleable Solids (SM: 2540 F.)	<0.1	-	-
Sulfide as H ₂ S	mg/l	Iodometric (SM: 4500-S ²⁻ F.)	Not Detected	-	-
Total Kjeldahl Nitrogen	mg/l	Macro Kjeldahl (SM: 4500-N _{org} B.)	2.2	-	-
Oil & Grease	mg/l	Liquid-Liquid Partition-Gravimetric (SM: 5520 B.)	Not Detected	-	-
Total Coliform Bacteria	MPN/100 ml	MPN Test	3.6 x 10 ³	-	-
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	910.0	-	-

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED., 2023 (AWWA, APHA, WEF)

- Remark : 1. * Notification of the Ministry of Natural Resources and Environment, dated June 28, B.E. 2567 (2024), which was published in the Royal Government Gazette, Vol. 141, Part 233D dated August 27, B.E. 2567 (2024) . (Category B)
2. [#] ISO/IEC 17025 ACCREDITED BY DEPARTMENT OF SCIENCE SERVICE (DSS)

(MR TAWATCHAI CHONGVUTICHA)

LABORATORY SUPERVISOR



ANALYSIS REPORT


CUSTOMER NAME : เดอะ วิลลีย์ เขาใหญ่
ADDRESS : เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เขาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.
SAMPLING LOCATION : บ่อพักน้ำแรกหลังออกจากระบบบำบัดน้ำเสีย อาคาร B
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : เหลืองใส มีตะกอนเล็กน้อย ไม่มีกลิ่น
SAMPLING DATE : JUNE 11, 2026
SAMPLING TIME : 10:30
SAMPLING BY : นายโกวิท บุญหา
SAMPLE NO. : 06131
REPORT NO. : RN260690130
SAMPLING SOURCE : WASTEWATER
RECEIVED DATE : JUNE 12, 2026
ANALYTICAL DATE : JUNE 12 - 18, 2026
REPORT DATE : JUNE 19, 2026

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
pH [#]	-	Electrometric (SM: 4500-H ⁺ B.)	8.6 at 25°C	-	5.5-9.0
Biochemical Oxygen Demand	mg/l	Membrane Electrode (SM: 4500-O ₂ G, 5210 B.)	2.1	-	≤30
Total Dissolved Solids [#]	mg/l	Total Dissolved Solids Dried at 180°C (SM: 2540 C.)	548.0	-	≤1,000
Total Suspended Solids	mg/l	Total Suspended Solids Dried at 103-105°C (SM: 2540 D.)	4.0	-	≤40
Settleable Solids	ml/l	Settleable Solids (SM: 2540 F.)	<0.1	-	-
Sulfide as H ₂ S	mg/l	Iodometric (SM: 4500-S ²⁻ F.)	Not Detected	-	≤1.0
Total Kjeldahl Nitrogen	mg/l	Macro Kjeldahl (SM: 4500-N _{org} B)	0.6	-	<35
Oil & Grease	mg/l	Liquid-Liquid Partition-Gravimetric (SM: 5520 B.)	Not Detected	-	<20
Total Coliform Bacteria	MPN/100 ml	MPN Test	2.7 x 10 ³	-	-
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	910.0	-	-

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED., 2023 (AWWA, APHA, WEF)

Remark : 1. Notification of the Ministry of Natural Resources and Environment, dated June 28, B.E. 2567 (2024), which was published in the Royal Government Gazette, Vol. 141, Part 233D dated August 27, B.E. 2567 (2024) . (Category B)

2. [#]ISO/IEC 17025 ACCREDITED BY DEPARTMENT OF SCIENCE SERVICE (DSS)



LABORATORY SUPERVISOR



ห้องปฏิบัติการวิเคราะห์บริษัท โอกลา เทสติ้ง แอนด์ คอนซัลติง เซอร์วิส จำกัด

63/13 เพชรเกษม ซอย 7 แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพฯ 10600

Tel: 0 2868 1246 Fax: 0 2868 0860 www.okla-testing.com J-NAC Group



TESTING
No.0334

ANALYSIS REPORT

CUSTOMER NAME : เดอะ วิลลีย์ เขาใหญ่
ADDRESS : เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เขาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.
SAMPLING LOCATION : ถังแยกกากของระบบบำบัดน้ำเสีย อาคาร C
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : เหลืองใส ไม่มีตะกอน ไม่มีกลิ่น
SAMPLING DATE : JUNE 11, 2026
SAMPLING TIME : 10:30
SAMPLING BY : นายโกวิท บุญหา
SAMPLE NO. : 06132
REPORT NO. : RN260690131
SAMPLING SOURCE : WASTEWATER
RECEIVED DATE : JUNE 12, 2026
ANALYTICAL DATE : JUNE 12 - 18, 2026
REPORT DATE : JUNE 19, 2026

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
pH [#]	-	Electrometric (SM: 4500-H ⁺ B.)	7.9 at 25°C	-	-
Biochemical Oxygen Demand	mg/l	Membrane Electrode (SM: 4500-O G, 5210 B.)	3.4	-	-
Total Dissolved Solids [#]	mg/l	Total Dissolved Solids Dried at 180°C (SM: 2540 C.)	577.0	-	-
Total Suspended Solids [#]	mg/l	Total Suspended Solids Dried at 103-105°C (SM: 2540 D.)	10.0	-	-
Settleable Solids	ml/l	Settleable Solids (SM: 2540 F.)	<0.1	-	-
Sulfide as H ₂ S	mg/l	Iodometric (SM: 4500-S ²⁻ F.)	Not Detected	-	-
Total Kjeldahl Nitrogen	mg/l	Macro Kjeldahl (SM: 4500-N _{org} B)	1.7	-	-
Oil & Grease	mg/l	Liquid-Liquid Partition-Gravimetric (SM: 5520 B.)	Not Detected	-	-
Total Coliform Bacteria	MPN/100 ml	MPN Test	2.7 x 10 ³	-	-
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	430.0	-	-

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED.,2023 (AWWA,APHA, WEF)

Remark : 1. * Notification of the Ministry of Natural Resources and Environment, dated June 28, B.E. 2567 (2024), which was published in the Royal Government Gazette, Vol. 141, Part 233D dated August 27, B.E. 2567 (2024) . (Category B)

2. [#] ISO/IEC 17025 ACCREDITED BY DEPARTMENT OF SCIENCE SERVICE (DSS)

LABORATORY SUPERVISOR

*** Reported analysis refers to submitted sample only. Report analysis shall not be reproduced except in full, without written approval of Laboratory. ***



ห้องปฏิบัติการวิเคราะห์บริษัท โอกลา เทสติ้ง แอนด์ คอนซัลติง เซอร์วิส จำกัด

63/13 เพชรเกษม ซอย 7 แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพฯ 10600

Tel: 0 2868 1246 Fax: 0 2868 0860 www.okla-testing.com J-NAC Group



TESTING
No.0334

ANALYSIS REPORT

CUSTOMER NAME : เดอะ วิลลีย์ เขาใหญ่
ADDRESS : เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เขาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.
SAMPLING LOCATION : บ่อพักน้ำแรกหลังออกจากระบบบำบัดน้ำเสีย อาคาร C
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : เหลืองใส ไม่มีตะกอน ไม่มีกลิ่น
SAMPLING DATE : JUNE 11, 2026
SAMPLING TIME : 10:30
SAMPLING BY : นายโกวิท บุญหา

SAMPLE NO. : 06133
REPORT NO. : RN260690132
SAMPLING SOURCE : WASTEWATER
RECEIVED DATE : JUNE 12, 2026
ANALYTICAL DATE : JUNE 12 - 18, 2026
REPORT DATE : JUNE 19, 2026

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
pH [#]	-	Electrometric (SM: 4500-H ⁺ B.)	7.5 at 25°C	-	5.5-9.0
Biochemical Oxygen Demand	mg/l	Membrane Electrode (SM: 4500-O ₂ G, 5210 B.)	4.6	-	≤30
Total Dissolved Solids [#]	mg/l	Total Dissolved Solids Dried at 180°C (SM: 2540 C.)	492.0	-	≤1,000
Total Suspended Solids	mg/l	Total Suspended Solids Dried at 103-105°C (SM: 2540 D.)	Not Detected	-	≤40
Settleable Solids	ml/l	Settleable Solids (SM: 2540 F.)	<0.1	-	-
Sulfide as H ₂ S	mg/l	Iodometric (SM: 4500-S ²⁻ F.)	Not Detected	-	≤1.0
Total Kjeldahl Nitrogen	mg/l	Macro Kjeldahl (SM: 4500-N _{org} B)	2.0	-	<35
Oil & Grease	mg/l	Liquid-Liquid Partition-Gravimetric (SM: 5520 B.)	Not Detected	-	<20
Total Coliform Bacteria	MPN/100 ml	MPN Test	3.6 x 10 ³	-	-
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	910.0	-	-

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED.,2023 (AWWA,APHA, WEF)

Remark : 1. Notification of the Ministry of Natural Resources and Environment, dated June 28, B.E. 2567 (2024), which was published in the Royal Government Gazette, Vol. 141, Part 233D dated August 27, B.E. 2567 (2024) . (Category B)

2. [#]ISO/IEC 17025 ACCREDITED BY DEPARTMENT OF SCIENCE SERVICE (DSS)

(MR TAWATCHAI CHONGVUTICHA)

LABORATORY SUPERVISOR

*** Reported analysis refers to submitted sample only. Report analysis shall not be reproduced except in full, without written approval of Laboratory. ***

ANALYSIS REPORT

CUSTOMER NAME : เดอะ วิลลีย์ เขาใหญ่
 ADDRESS : เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เขาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.
 SAMPLING LOCATION : สระว่ายน้ำ (ส่วนต้น)
 SAMPLING METHOD : GRAB
 SAMPLING CONDITION : NORMAL
 CHARACTERISTICS OF WATER :ใส ไม่มีตะกอน ไม่มีกลิ่น
 SAMPLING DATE : JUNE 11, 2026
 SAMPLING TIME : 10:30
 SAMPLING BY : นายโกวิท บุฬา

SAMPLE NO. : 06134
 REPORT NO. : RN260690133
 SAMPLING SOURCE : SWIMMING POOL
 RECEIVED DATE : JUNE 12, 2026
 ANALYTICAL DATE : JUNE 12 - 18, 2026
 REPORT DATE : JUNE 19, 2026

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
Total Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	<10
<i>Escherichia Coli</i>	per 100 ml	E.coli Procedure Using Fluorogenic Substrate (SM: 9221 F.)	Not Detected	-	Not Detected

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED.,2023 (AWWA,APHA, WEF)

Remark : 1. *Recommendations of the Public Health Committee No. 1/2007 regarding the control of swimming pool operations or other businesses Likewise.

(MR TAWATCHAI CHONGVUTICHA)

LABORATORY SUPERVISOR



บริษัท เอชวีอี จำกัด 603 ซอยจรัญสนิทวงศ์ 46 ถนนจรัญสนิทวงศ์ แขวงบางมด เขตบางพลัด กรุงเทพฯ 10700
HVE CO. LTD. 603 Soi Jaruansanitwong 46 Jaruansanitwong Road Bangyeekan Bangplad Bangkok 10700
Tel : (02) 8834956-7 , (02) 8834274 Fax : (02) 8834956 E-mail address hv_eng@hotmail.com

รายงานผลการทดสอบ
(ANALYSIS REPORT)

รายงานหมายเลข (Report No.) 3650626 วันที่ (Date) 21 มิถุนายน 2569
ชื่อตัวอย่าง (Sample Name)^c น้ำสระว่ายน้ำ (ส่วนต้น)
รหัสตัวอย่าง (Sample No.) No. 6906347
ลักษณะตัวอย่างทางกายภาพ^c ใส่, ไม่มีตะกอน
ชื่อลูกค้า (Customer name)^c บริษัท โอกลา เทสติ้ง แอนด์ คอนซัลติ้ง เซอร์วิส จำกัด (สำนักงานใหญ่)
สถานที่เก็บตัวอย่าง (Sampling site)^c Project TWL75
ที่อยู่ (Address)^c 63/13 ซอยเพชรเกษม 7 แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพฯ 10600
วันที่รับตัวอย่าง (Received Date) 12 มิถุนายน 2569 วันที่ตรวจวิเคราะห์ (Analysis Date) 12 มิถุนายน 2569 - 21 มิถุนายน 2569
วันที่เก็บตัวอย่าง (Collected Date)^c 11 มิถุนายน 2569 วิธีการเก็บตัวอย่าง (Sampling Method)^c เก็บแบบ จ้วง (Grab)

พารามิเตอร์ (Parameter)	หน่วย (Unit)	ผลการวิเคราะห์ (Result)	MDL	ค่ามาตรฐาน ^{1/} (Standard)	วิธีทดสอบ ^{4/} (Test Method)
		น้ำสระว่ายน้ำ (ส่วนต้น)			
<i>Staphylococcus aureus</i>	per 100 mL	Not Detected	-	Not Detected	In-house method based on APHA, AWWA, WEF 24 th ed. 2023, 9213 B
<i>Pseudomonas aeruginosa</i>	per 100 mL	Not Detected	-	Not Detected	APHA, AWWA, WEF 24 th ed. 2023, 9213 E

หมายเหตุ : ^{1/} ส่วนหนึ่งของคณะกรรมการสาธารณสุข ฉบับที่ 1/2550 เรื่อง การควบคุมการประกอบกิจการสระว่ายน้ำ หรือกิจการอื่นๆ ในทางลงเดียวกัน

^{4/} Standard Methods for the Examination of Water and Wastewater, APHA, AWWA, WEF, 24th ed. 2023

^c เป็นข้อมูลที่มาจากการสุ่ม

- สภาวะแวดล้อมของห้องปฏิบัติการ 25 ± 5 °C

- ห้องปฏิบัติการมีนโยบายไม่ใช้ตัวอย่างเอง

(นายฐานันท์ นิการัตน์)
ผู้จัดการฝ่ายวิชาการ

(นางสาวทิพวรรณ วงศ์บุญตัน)
ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์

- รายงานผลการทดสอบนี้ให้รับรองเฉพาะตัวอย่างตามที่ได้รับมาทดสอบเท่านั้น
- ห้ามนำรายงานผลการทดสอบนี้ไปประกาศโฆษณา
- รายงานผลการทดสอบนี้ห้ามคัดลอกถ่ายทำสำเนาเฉพาะเพียงบางส่วน โดยไม่ได้รับอนุญาตจากห้องปฏิบัติการเป็นลายลักษณ์อักษร ยกเว้นทำทั้งฉบับ

ANALYSIS REPORT

CUSTOMER NAME : เดอะ วิลลีย์ เขาใหญ่
 ADDRESS : เลขที่ 395 ตำบลพญาเย็น อำเภอปากช่อง, พญาเย็น, เขาใหญ่ จังหวัดนครราชสีมา, ประเทศไทย, 30320.
 SAMPLING LOCATION : สระว่ายน้ำ (ส่วนลึก)
 SAMPLING METHOD : GRAB
 SAMPLING CONDITION : NORMAL
 CHARACTERISTICS OF WATER :ใส ไม่มีตะกอน ไม่มีกลิ่น
 SAMPLING DATE : JUNE 11, 2026
 SAMPLING TIME : 10:30
 SAMPLING BY : นายโกวิท บุฬา

SAMPLE NO. : 06135
 REPORT NO. : RN260690134
 SAMPLING SOURCE : SWIMMING POOL
 RECEIVED DATE : JUNE 12, 2026
 ANALYTICAL DATE : JUNE 12 - 18, 2026
 REPORT DATE : JUNE 19, 2026

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
Total Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	<10
<i>Escherichia Coli</i>	per 100 ml	E.coli Procedure Using Fluorogenic Substrate (SM: 9221 F.)	Not Detected	-	Not Detected

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 24th ED., 2023 (AWWA, APHA, WEF)

Remark : 1. Recommendations of the Public Health Committee No. 1/2007 regarding the control of swimming pool operations or other businesses Likewise.

(MR TAWATCHAI CHONGVUTICHA)

LABORATORY SUPERVISOR



บริษัท เอชวีอี จำกัด 603 ซอยจรัญสนิทวงศ์ 46 ถนนจรัญสนิทวงศ์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพฯ 10700
HVE CO. LTD. 603 Soi Jarunsnitwong 46 Jarunsnitwong Road Bangyekan Bangplad Bangkok 10700
Tel : (02) 8834956-7 , (02) 8834274 Fax : (02) 8834956 E-mail address hv_eng@hotmail.com

รายงานผลการทดสอบ
(ANALYSIS REPORT)

รายงานหมายเลข (Report No.) 3660626 วันที่ (Date) 21 มิถุนายน 2569
ชื่อตัวอย่าง (Sample Name)^c น้ำระเหยน้ำ (ส่วนลึก)
รหัสตัวอย่าง (Sample No.) No. 6906348
ลักษณะตัวอย่างทางกายภาพ^cใส, ไม่มีตะกอน
ชื่อลูกค้า (Customer name)^cบริษัท โอกลา เทสติ้ง แอนด์ คอนซัลติ้ง เซอร์วิส จำกัด (สำนักงานใหญ่)
สถานที่เก็บตัวอย่าง (Sampling site)^cProject TWL75
ที่อยู่ (Address)^c63/13 ซอยเพชรเกษม 7 แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพฯ 10600
วันที่รับตัวอย่าง (Received Date) 12 มิถุนายน 2569 วันที่ตรวจวิเคราะห์ (Analysis Date) 12 มิถุนายน 2569 - 21 มิถุนายน 2569
วันที่เก็บตัวอย่าง (Collected Date)^c 11 มิถุนายน 2569 วิธีการเก็บตัวอย่าง (Sampling Method)^cเก็บแบบ จ้วง (Grab)

พารามิเตอร์ (Parameter)	หน่วย (Unit)	ผลการวิเคราะห์ (Result)	MDL	ค่ามาตรฐาน ^{1/} (Standard)	วิธีทดสอบ ^{4/} (Test Method)
		น้ำระเหยน้ำ (ส่วนลึก)			
<i>Staphylococcus aureus</i>	per 100 mL	Not Detected	-	Not Detected	In-house method based on APHA, AWWA, WEF 24 th ed. 2023, 9213 B
<i>Pseudomonas aeruginosa</i>	per 100 mL	Not Detected	-	Not Detected	APHA, AWWA, WEF 24 th ed. 2023, 9213 E

หมายเหตุ : ^{1/} สำหรับของคณกรรมการสาธารณสุข ฉบับที่ 1/2550 เรื่อง การควบคุมการประกอบกิจการระบายน้ำ หรือกิจการอื่นๆ ในทางองเดียวกัน

^{4/} Standard Methods for the Examination of Water and Wastewater, APHA, AWWA, WEF, 24th ed. 2023

^c เป็นข้อมูลที่ได้จากลูกค้า

- สภาพแวดล้อมของห้องปฏิบัติการ 25 ± 5 °C

- ห้องปฏิบัติการมีนโยบายไม่ซื้กตัวอย่างเอง

(นายฐานันท์ นิลารัตน์)
ผู้จัดการฝ่ายวิชาการ

(นางสาวเทพวรรณ วงศ์บุญเดิม)
ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์

- รายงานผลการทดสอบนี้ให้รับรองเฉพาะตัวอย่างตามที่ได้รับมาทดสอบเท่านั้น
- ห้ามนำรายงานผลการทดสอบนี้ไปประกาศโฆษณา
- รายงานผลการทดสอบนี้ห้ามคัดลอกถ่ายทำสำเนาเฉพาะเพียงบางส่วน โดยไม่ได้รับอนุญาตจากห้องปฏิบัติการเป็นลายลักษณ์อักษร ยกเว้นทั้งฉบับ

เอกสารแนบ 5

หนังสือรับรองห้องปฏิบัติการวิเคราะห์เอกชน



๑๑ กันยายน ๒๕๖๗

เรื่อง ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

เรียน กรรมการผู้จัดการ บริษัท โอกลา เทสต์ติ้ง แอนด์ คอนซัลติ้ง เซอร์วิส จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๑๕ กรกฎาคม ๒๕๖๗

สิ่งที่ส่งมาด้วย เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท โอกลา เทสต์ติ้ง แอนด์ คอนซัลติ้ง เซอร์วิส จำกัด จำนวน ๑ แผ่น

ตามคำขอที่อ้างถึง บริษัท โอกลา เทสต์ติ้ง แอนด์ คอนซัลติ้ง เซอร์วิส จำกัด ขอต่ออายุหนังสือ
รับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๒๑๙ สถานที่ตั้งเลขที่ ๖๓/๑๓ ซอยเพชรเกษม ๗
แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพมหานคร ต่อกรมโรงงานอุตสาหกรรม ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้บริษัท โอกลา เทสต์ติ้ง แอนด์ คอนซัลติ้ง เซอร์วิส จำกัด
ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน โดยมีองค์ประกอบดังนี้

ก. ผู้ควบคุมห้องปฏิบัติการวิเคราะห์เอกชน

- | | |
|---------------------------|----------------------------|
| ๑) นายธวัชชัย จงวุฒิชัย | ทะเบียนเลขที่ ว-๒๑๙-ค-๐๐๐๑ |
| ๒) นางสาวปนัดดา พันธกะจับ | ทะเบียนเลขที่ ว-๒๑๙-ค-๐๐๐๒ |
| ๓) นางสาวจามจุรี คำปุย | ทะเบียนเลขที่ ว-๒๑๙-ค-๐๐๐๓ |

ข. เจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน


- | | |
|-------------------------------|----------------------------|
| ๑) นางสาวนิจินาท มะติยาภักดิ์ | ทะเบียนเลขที่ ว-๒๑๙-จ-๐๐๐๑ |
| ๒) นางสาวภาณุชนารถ เชื้อวชาญ | ทะเบียนเลขที่ ว-๒๑๙-จ-๐๐๐๒ |
| ๓) นางสาวธิดารัตน์ กลัดตลาด | ทะเบียนเลขที่ ว-๒๑๙-จ-๐๐๐๓ |
| ๔) นางสาวเบญจพร อินแก้ว | ทะเบียนเลขที่ ว-๒๑๙-จ-๐๐๐๔ |
| ๕) นางสาววันวิสา หวังแวกลาง | ทะเบียนเลขที่ ว-๒๑๙-จ-๐๐๐๕ |
| ๖) นางสาวรัตตชา ศรีปราสาท | ทะเบียนเลขที่ ว-๒๑๙-จ-๐๐๐๖ |
| ๗) นายปริญญญา กล้าน้อย | ทะเบียนเลขที่ ว-๒๑๙-จ-๐๐๐๗ |
| ๘) นายโกวิท บุพา | ทะเบียนเลขที่ ว-๒๑๙-จ-๐๐๐๘ |
| ๙) นายพีรพล ถวิลหวัง | ทะเบียนเลขที่ ว-๒๑๙-จ-๐๐๐๙ |

ค. ขอบข่ายชนิดสารมลพิษที่ได้รับขึ้นทะเบียนให้วิเคราะห์ในน้ำ/น้ำเสีย และอากาศเสียตามสิ่งที่ส่งมาด้วย

หนังสือฉบับนี้จะหมดอายุในวันที่ ๑๕ สิงหาคม ๒๕๗๑ หากประสงค์จะต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ให้ยื่นคำขอต่ออายุพร้อมเอกสารประกอบคำขอต่อกรมโรงงานอุตสาหกรรมภายใน ๖๐ วัน ก่อนวันสิ้นอายุของหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ



(นายพรยศ กลั่นกรอง)

รองอธิบดี ปฏิบัติราชการแทน
อธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน

กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ

โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕

โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๔๔

ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th



เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท โอกลา เทสติ้ง แอนด์ คอนซัลติ้ง เซอร์วิส จำกัด เลขทะเบียน ว-๒๑๙
ที่ ออก ๐๓๑๐(๑)/ ๙๒๔๖ ลงวันที่ ๑๑ กันยายน ๒๕๖๗

ขอขยายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรมจำนวน ๑๔ รายการ

น้ำ/น้ำเสีย จำนวน 9 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Biochemical Oxygen Demand	1) 5-Day BOD Test, Azide Modification Method ^[2] 2) 5-Day BOD Test, Membrane Electrode Method ^[2]
2	Free Chlorine	Iodometric Method ^[2]
3	Oil & Grease	Liquid-Liquid, Partition Gravimetric Method ^[2]
4	pH	Electrometric Method ^[2]
5	Sulfide	Iodometric Method ^[2]
6	Temperature	Laboratory and Field Methods ^[2]
7	Total Dissolved Solids	Dried at 180 °C ^[2]
8	Total Kjeldahl Nitrogen	Macro-Kjeldahl Method ^[2]
9	Total Suspended Solids	Dried from 103 to 105 °C ^[2]

อากาศเสีย (ปล่องระบาย) จำนวน 5 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Carbon Monoxide	Instrument Analyzer Method ^[3]
2	Opacity	Ringelmann's Method ^[1]
3	Oxides of Nitrogen	Instrument Analyzer Method ^[3]
4	Sulfur Dioxide	Instrument Analyzer Method ^[3]
5	Total Suspended Particulate	Isokinetic Sampling, Gravimetric Method ^[3]

เอกสารอ้างอิง

- กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม เรื่อง กำหนดค่าปริมาณเขม่าควันที่เจือปนในอากาศที่ระบายออกจากปล่องของหม้อน้ำของโรงงาน พ.ศ. 2549. ราชกิจจานุเบกษา. 4 ธันวาคม 2549. เล่มที่ 123 ตอนพิเศษ 125 ง.
- APHA, AWWA, WEF. *Standard Methods for the Examination of Water and Wastewater*. 24th ed. Washington, DC: APHA, 2023.
- United States Environmental Protection Agency. *Standard of Performance for New Stationary Source*. 40 CFR 60. Appendix A, 2019.



ที่ อว 0303/167

ใบรับรองความสามารถห้องปฏิบัติการทดสอบ

ใบรับรองฉบับนี้ให้ไว้เพื่อแสดงว่า

ห้องปฏิบัติการวิเคราะห์ บริษัท โอกลา เทสติ้ง แอนด์ คอนซัลติง เซอร์วิส จำกัด
เลขที่ 63/13 ซอยเพชรเกษม 7 แขวงวัดท่าพระ
เขตบางกอกใหญ่ กรุงเทพมหานคร 10600

ได้ผ่านการประเมินความสามารถห้องปฏิบัติการทดสอบตามมาตรฐาน ISO/IEC 17025 : 2017
และข้อกำหนด กฎระเบียบ และเงื่อนไขการรับรองความสามารถห้องปฏิบัติการทดสอบ
ของสำนักบริหารและรับรองห้องปฏิบัติการ กรมวิทยาศาสตร์บริการ

LABORATORY ACCREDITATION
หมายเลขการรับรองระบบงานที่ ทดสอบ - 0334
BLA-DSS

รายละเอียดการรับรองดังขอบข่ายการรับรองแนบท้าย

ออกให้ ณ วันที่ : 10 มกราคม 2568

หมดอายุ วันที่ : 9 มกราคม 2572

ลงชื่อ :

(นางจันทร์รัตน์ วรสรรพวิทย์)

ผู้อำนวยการสำนักบริหารและรับรองห้องปฏิบัติการ

สำนักบริหารและรับรองห้องปฏิบัติการ กรมวิทยาศาสตร์บริการ
กระทรวงการอุดมศึกษา วิทยาศาสตร์ วิจัยและนวัตกรรม

ขอข่ายการรับรองความสามารถห้องปฏิบัติการทดสอบ

ชื่อห้องปฏิบัติการ : ห้องปฏิบัติการวิเคราะห์ บริษัท โอกลา เทสติ้ง แอนด์ คอนซัลติง เซอร์วิส จำกัด

สถานที่ตั้ง : เลขที่ 63/13 ซอยเพชรเกษม 7 แขวงวัดท่าพระ

เขตบางกอกใหญ่ กรุงเทพมหานคร 10600

หมายเลขการรับรองระบบงานที่ : ทดสอบ - 0334

สถานะของห้องปฏิบัติการ : ☒ ถาวร ☐ นอกสถานที่ ☐ชั่วคราว ☐ เคลื่อนที่

ลำดับ ที่	วัสดุ / ผลิตภัณฑ์ที่ทดสอบ	รายการที่ทดสอบ / ช่วงของการทดสอบ	วิธีทดสอบ / เทคนิคที่ใช้
2	น้ำเสีย	- ความเป็นกรด-ด่าง 4.0 ถึง 10.0 - สารแขวนลอยทั้งหมด ที่อุณหภูมิ 103 °C ถึง 105 °C 10 mg/L ถึง 2 000 mg/L - สารที่ละลายได้ทั้งหมด ที่อุณหภูมิ 180 °C 100 mg/L ถึง 5 000 mg/L	Standard Methods for the Examination of Water and Wastewater, APHA, AWWA & WEF, 24th ed., 2023, part 4500-H⁺ B Standard Methods for the Examination of Water and Wastewater, APHA, AWWA & WEF, 24th ed., 2023, part 2540 D Standard Methods for the Examination of Water and Wastewater, APHA, AWWA & WEF, 24th ed., 2023, part 2540 C

ออกให้ ณ วันที่ : 10 มกราคม 2568

ลงชื่อ :

(นางจันทร์รัตน์ วรสรรพวิทย)

ผู้อำนวยการสำนักบริหารและรับรองห้องปฏิบัติการ

ออกครั้งแรก ณ วันที่ 10 มกราคม 2568

ฉบับที่ 1

สำนักบริหารและรับรองห้องปฏิบัติการ กรมวิทยาศาสตร์บริการ กระทรวงการอุดมศึกษา วิทยาศาสตร์ วิจัยและนวัตกรรม

ขอข่ายการรับรองความสามารถห้องปฏิบัติการทดสอบ

ชื่อห้องปฏิบัติการ : ห้องปฏิบัติการวิเคราะห์ บริษัท โอกลา เทสติ้ง แอนด์ คอนซัลติ้ง เซอร์วิส จำกัด

สถานที่ตั้ง : เลขที่ 63/13 ซอยเพชรเกษม 7 แขวงวัดท่าพระ

เขตบางกอกใหญ่ กรุงเทพมหานคร 10600

หมายเลขการรับรองระบบงานที่ : ทดสอบ - 0334

สถานะของห้องปฏิบัติการ : ☒ ถาวร ☐ นอกสถานที่ ☐ชั่วคราว ☐เคลื่อนที่

ลำดับ ที่	วัสดุ / ผลิตภัณฑ์ที่ทดสอบ	รายการที่ทดสอบ / ช่วงของการทดสอบ	วิธีทดสอบ / เทคนิคที่ใช้
1	น้ำ	- ความเป็นกรด-ด่าง 6.0 ถึง 9.0 - สารแขวนลอยทั้งหมด ที่อุณหภูมิ 103 °C ถึง 105 °C 10 mg/L ถึง 2 000 mg/L - สารที่ละลายได้ทั้งหมด ที่อุณหภูมิ 180 °C 100 mg/L ถึง 5 000 mg/L	Standard Methods for the Examination of Water and Wastewater, APHA, AWWA & WEF, 24th ed., 2023, part 4500-H⁺ B Standard Methods for the Examination of Water and Wastewater, APHA, AWWA & WEF, 24th ed., 2023, part 2540 D Standard Methods for the Examination of Water and Wastewater, APHA, AWWA & WEF, 24th ed., 2023, part 2540 C

ออกครั้งแรก ณ วันที่ 10 มกราคม 2568

ฉบับที่ 1

สำนักบริหารและรับรองห้องปฏิบัติการ กรมวิทยาศาสตร์บริการ กระทรวงการอุดมศึกษา วิทยาศาสตร์ วิจัยและนวัตกรรม



ที่ อก ๐๓๑๐(๑)/ ๑ ๒ ๓ ๗ ๒

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๕๐๐

๒ ๘ สิงหาคม ๒๕๖๖

เรื่อง ขันทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

เรียน กรรมการผู้จัดการ บริษัท เอชวีอี จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๑๘ พฤษภาคม ๒๕๖๖

สิ่งที่ส่งมาด้วย เอกสารแนบท้ายหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท เอชวีอี จำกัด จำนวน ๒ แผ่น

ตามหนังสือที่อ้างถึง บริษัท เอชวีอี จำกัด ขอขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน พร้อม
รายชื่อผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์และรายการสารมลพิษ
ที่จะทำการวิเคราะห์ ต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้บริษัท เอชวีอี จำกัด ขันทะเบียนห้องปฏิบัติการ
วิเคราะห์เอกชน มีเลขทะเบียน ว-๓๕๘ สถานที่ตั้งเลขที่ ๖๐๓ ซอยจรัญสนิทวงศ์ ๔๖ แขวงบางยี่ขัน
เขตบางพลัด กรุงเทพมหานคร โดยมีองค์ประกอบดังนี้

ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์

- | | |
|-----------------------------|----------------------------|
| ๑) นายเอกลักษณ์ สีสาบิหาร | ทะเบียนเลขที่ ว-๓๕๘-ค-๐๐๐๑ |
| ๒) นางสาวทิพวรรณ วงศ์บุญตัน | ทะเบียนเลขที่ ว-๓๕๘-ค-๐๐๐๒ |
| ๓) นายพล ม่วงใหญ่ | ทะเบียนเลขที่ ว-๓๕๘-ค-๐๐๐๓ |

ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์

- | | |
|------------------------------|----------------------------|
| ๑) นางสาวสุปรียา หล้าอิน | ทะเบียนเลขที่ ว-๓๕๘-จ-๐๐๐๑ |
| ๒) นางสาวจิราภรณ์ ผงผานอก | ทะเบียนเลขที่ ว-๓๕๘-จ-๐๐๐๒ |
| ๓) นายธรรมรัตน์ จิรยวัฒน์สุข | ทะเบียนเลขที่ ว-๓๕๘-จ-๐๐๐๓ |
| ๔) นางสาวธนภรณ์ กำทา | ทะเบียนเลขที่ ว-๓๕๘-จ-๐๐๐๔ |
| ๕) นางสาวณัฐรดา คงบัน | ทะเบียนเลขที่ ว-๓๕๘-จ-๐๐๐๕ |
| ๖) นายฐานันท์ นิภารัตน์ | ทะเบียนเลขที่ ว-๓๕๘-จ-๐๐๐๖ |
| ๗) นายมนโรด สุดจันทร์ | ทะเบียนเลขที่ ว-๓๕๘-จ-๐๐๐๗ |

ค. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนให้วิเคราะห์ในน้ำเสียและอากาศเสีย ตามสิ่งที่

ส่งมาด้วย

หนังสือฉบับ...

หนังสือฉบับนี้มีอายุครั้งละ ๓ ปี นับจากวันที่กรมโรงงานอุตสาหกรรมออกหนังสือหากประสงค์จะต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ให้ยื่นคำขอต่ออายุพร้อมเอกสารประกอบคำขอต่อกรมโรงงานอุตสาหกรรม ภายใน ๓๐ วัน ก่อนวันสิ้นอายุของหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชนทั้งนี้สามารถยื่นคำขอผ่านระบบอิเล็กทรอนิกส์ได้ที่หน้าเว็บไซต์กรมโรงงานอุตสาหกรรม

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ



(นายประสม คำรงพงษ์)

ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน

กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ

โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕

โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๔๙

ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th



เอกสารแนบท้ายหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

บริษัท เอชวีอี จำกัด

เลขทะเบียน ว-๓๕๘

ที่ ออก ๐๓๑๐(๑)/ ๑ ๒ ๓ ๗ ๒

ลงวันที่ ๒๘ สิงหาคม ๒๕๖๖

ขอขยายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๓๑ รายการ

น้ำเสีย จำนวน 30 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Aldicarb	High-Performance Liquid Chromatographic Method ^[1]
2	Aldicarb sulfone	High-Performance Liquid Chromatographic Method ^[1]
3	Aldicarb sulfoxide	High-Performance Liquid Chromatographic Method ^[1]
4	Aldrin	Liquid-Liquid Extraction, Gas Chromatographic Method ^[1]
5	α-BHC	Liquid-Liquid Extraction, Gas Chromatographic Method ^[1]
6	Biochemical Oxygen Demand	5-Day BOD Test, Azide Modification Method ^[1]
7	Carbaryl	High-Performance Liquid Chromatographic Method ^[1]
8	Carbofuran	High-Performance Liquid Chromatographic Method ^[1]
9	Chemical Oxygen Demand	Closed Reflux, Titrimetric Method ^[1]
10	4,4'-DDD	Liquid-Liquid Extraction, Gas Chromatographic Method ^[1]
11	4,4'-DDE	Liquid-Liquid Extraction, Gas Chromatographic Method ^[1]
12	Dieldrin	Liquid-Liquid Extraction, Gas Chromatographic Method ^[1]
13	Endosulfan I	Liquid-Liquid Extraction, Gas Chromatographic Method ^[1]
14	Endosulfan II	Liquid-Liquid Extraction, Gas Chromatographic Method ^[1]
15	Endrin	Liquid-Liquid Extraction, Gas Chromatographic Method ^[1]
16	Heptachlor	Liquid-Liquid Extraction, Gas Chromatographic Method ^[1]
17	Heptachlo Epoxide	Liquid-Liquid Extraction, Gas Chromatographic Method ^[1]
18	3-Hydroxycarbofuran	High-Performance Liquid Chromatographic Method ^[1]
19	Methiocarb	High-Performance Liquid Chromatographic Method ^[1]
20	Methomyl	High-Performance Liquid Chromatographic Method ^[1]
21	1-Naphthol	High-Performance Liquid Chromatographic Method ^[1]
22	Oil & Grease	Liquid-Liquid, Partition-Gravimetric Method ^[1]
23	Oxamyl	High-Performance Liquid Chromatographic Method ^[1]
24	pH	Electrometric Method ^[1]
25	Propoxur	High-Performance Liquid Chromatographic Method ^[1]
26	Sulfide	Iodometric Method ^[1]
27	Temperature	Laboratory and Field Methods ^[1]
28	Total Dissolved Solids	Dried at 180 °C ^[1]
29	Total Kjeldahl Nitrogen	Macro Kjeldahl Method ^[1]
30	Total Suspended Solids	Dried at 103-105 °C ^[1]

อากาศเสีย (ปล่อยระบาย) จำนวน 1 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Opacity	Ringelmann's Method ^[2]

เอกสารอ้างอิง

1. APHA, AWWA, WEF. **Standard Methods for the Examination of Water and Wastewater**. 23rd ed. Washington, DC: APHA, 2017.

2. กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม เรื่อง กำหนดค่าปริมาณเขม่าควันที่เจือปนในอากาศที่ระบายออกจากปล่องของหม้อน้ำของโรงงาน พ.ศ. 2549. ราชกิจจานุเบกษา. 4 ธันวาคม 2549. เล่มที่ 123 ตอนพิเศษ 125ง.

เอกสารแนบ 6

เอกสารสอบเทียบเครื่องมือที่ใช้ในการวิเคราะห์



JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd.
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Temperature measurement laboratory
Calibration services department.



CERTIFICATE OF CALIBRATION

Certificate No. : CDT-033-69

Page 1 of 2 Pages

MEASUREMENT ITEM : Digital thermometer with sensor
MANUFACTURER : Digicon
MODEL/TYPE : DP-72
SERIAL NUMBER : 425066647
ID NUMBER : -
CONDITION AS-RECEIVED : Used item
CUSTOMER : OKLA Testing and Consulting Service Co., Ltd.
67/35-36 Floor 3, Soi Petchakasem 7/1, Petchakasem Rd,
Watthapra, Bangkokyai, Bangkok 10600

RECEIVED DATE : 19 Jan 2026
MEASUREMENT DATE : 28-29 Jan 2026
ISSUE DATE : 30 Jan 2026

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:

The temperature calibration was done by In-House calibration method as WI-CL-001 according to comparison method with standard digital temperature indicator and standard temperature probe. The temperature scale use was based on ITS-90.

Traceability:

The measurement results are traceable to the international system of units (SI) through National Institute of Metrology Thailand (NIMT) Certificate number: TT-1013-25, Certificate number: ER-0061-25.

Reference Used During Calibration:

1. Standard Temperature Probe
Model: STS-100 A500, Serial No.: 667682-09,
Due date: 9 Apr 2026
2. Digital Temperature Indicator
Model: DTI-1000-A MK II, Serial No.: 671407-00591 Due date: 22 Apr 2026

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor $k=2$, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Calibrated by:

- ☐ Mr. Sorawit Thachalad
☒ Miss Jittraporn Lertsomphol
☐ Miss Ruangrumpai Phoommit



Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager



JIRANATEE ASSOCIATES CO.,LTD.

Continuation of Certificate of Calibration Number CDT-033-69

Page 2 of 2 Pages

Result of Calibration: ☒ Without Adjustment ☐ With Adjustment

Calibration Range: 4 °C to 180 °C

Function:

Table 1: This equipment was connected with Thermocouple Type K Model: TP-01 S/N: 1280000607.
Dimension: Diameter 1.50 mm. Length 1000 mm.

<u>Immersion Depth</u> (mm)	<u>Standard Reading</u> (°C)	<u>UUC Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
70	4.085	4.0	-0.1	0.26
70	20.058	19.9	-0.1	0.26
70	79.924	79.9	0.0	0.38
70	103.983	104.6	0.6	0.54
70	149.951	150.7	0.7	0.54
70	179.931	180.3	0.3	0.74

UUC*: Unit Under Calibration

End of Certificate of Calibration



Certificate No. : C26020021

Page : 1 of 2

CERTIFICATE OF CALIBRATION

Equipment	: pH/ORP and EC/TDS/Salinity/Resistivity		
Meter Model	: HI5521-02	Serial No.	: 04160019101
Probe Model	: HI7662-W	Serial No.	: 0615024N
Resolution	: 0.1 °C	Temperature Range	: (-20 to 120)°C
Manufacturer	: Hanna Instruments	Made in	: Romania
Condition As-Received	: Used Product	Reference	: RE260170
Ambient Temperature	: (25 ± 2)°C	Relative Humidity	: (50 ± 15)%RH
Customer name	Okla Testing & Consulting Service Co., Ltd. 67/35-36, 3RD Floor, Phetkasem 7/1 Road, Wat Tha Pra, Bangkok Yai, Bangkok 10600 Thailand		
Received date	: 30 January 2026		
Calibrate date	: 4 February 2026		
Issue date	: 6 February 2026		
Calibrated Location	: Hanna Instruments (Thailand) Ltd.		
Calibration Method	: This calibrator was conducted by using in-house: calibration procedure CP-05 by using reference standard instruments.		

Calibrated by : Mr. Pichit Petthong**Approved by :**

(Mr. Anan Suwanchaisakul)

Authorized Signatory

Condition of this calibration result :

1. Reference standard instrument : This certificate is traceable to the international system of units (SI Units)

Instrument	Model	Serial No.	Certificate No.	Traceable
Digital Thermo-Hygrometer	HT-771SD	AI.07155	26H106	Technology Promotion Association (Thailand-Japan)
Temperature Block Calibrator	CTC-155A	723705-01938	T26-0057	Unithai Group Co.,Ltd.

Calibration Result :

Function : Temperature Measurement

This equipment was connected with Temperature Sensor.

Nominal Value (°C)	Standard Setting (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (± °C)
20	20.00	20.0	0.00	0.18
25	25.00	25.0	0.00	0.18
30	30.00	30.0	0.00	0.18

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95%

**** End of certificate ****



Certificate of Calibration

Certificate No. : MT26-1559

Page : 1 of 2

Customer : OKLA Testing & Consulting Service Co.,Ltd.

Address : 67/35-36 3 Rd Floor, Soi Petchkasem 7/1, Thapra, Bangkok Yai, Bangkok 10600

Description : Refrigerator

Manufacturer : Sanden

Model : SPB0500

Serial No. : SPB0500-231007454

Identification No. : N/A

Calibration Place : Laboratory

Order No. : 0336/26

Received date : Jan 29, 2026

Calibration date : Jan 29, 2026

Environment Condition :

Temperature : (25+/-10) °C

Humidity : (50+/-30) %RH

Calibration Method : Calibration were conducted using In-house calibration procedure *CP-MT-006* According to comparison with LXI Data Acquisition Switch Unit with sensor. The calibration methods based on Euramet Calibration Guide No.20 - guidelines on the Calibration of Temperature and/or Humidity Controlled Enclosures.

Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
LXI Data Acquisition Switch Unit with Sensor	34972A	MY57003222	MT25-5590	Jul 23, 2026

The effect that the result relate only to the items calibrated. It was found accurate as shown on date and place of calibration only.

Traceability : This measurement are traceable to the International System of Unit (SI), through National Institute of Metrology Thailand (NIMT)

The reported expanded uncertainty of measurement was based on standard uncertainty multiplied by coverage factor $k = 2$, providing a level of confidence of not less than 95%



Calibrated by : Mr.Kriengkrai Jomthaisong

Approved by : (Mr.Panuwat Phuklan)


Issue date : Jan 30, 2026

This calibration certificate shall not be reproduced other than in full except with the prior written approval of Inctech Metrological Center Co.,Ltd

Certificate No. : MT26-1559
Page : 2 of 2
Function : Temperature measurement
Result : Without adjustment
Calibration point : 4 °C
Resolution : 1 °C

Calibration point (°C)	Temperature of UUC* at each position (°C)									Uncertainty of measurement (+/- °C)
	Ch.1	Ch.2	Ch.3	Ch.4	Ch.5	Ch.6	Ch.7	Ch.8	Ch.9	
4	4.756	5.042	4.964	4.852	4.949	4.889	4.954	4.858	4.816	0.66

Setting temperature (°C)	Indicating Temperature (°C)	Measured stability (+/- °C)	Measured uniformity (°C)	Overall variation (°C)
4.0	4.8 to 4.9	0.21	0.36	0.54

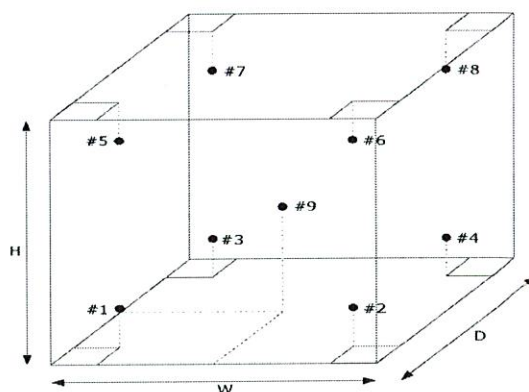

- #1 Lower Left Front
- #2 Lower Right Front
- #3 Lower Left Rear
- #4 Lower Right Rear
- #5 Upper Left Front
- #6 Upper Right Front
- #7 Upper Left Rear
- #8 Upper Right Rear
- #9 Geometric Center

Front view
UUC* = Unit under calibration

Uniformity = Maximum and Minimum difference of measured temperature at any probes and the measured temperature at the reference and same time.

Overall Variation = Difference of temperature value between the maximum and minimum any time.

Stability = One half of the maximum difference of measured temperatures at any one probe.

Certificate No. : C26020019

Page : 1 of 2

CERTIFICATE OF CALIBRATION

Equipment	: pH/ORP and EC/TDS/Salinity/Resistivity Meter		
Meter Model	: HI5521-02	Serial No.	: 04160019101
Probe Model	: HI1131B	Serial No.	: 11271CON
Resolution (pH)	: 0.01 pH	Resolution (mV)	: 0.1 mV
Manufacturer	: Hanna Instruments	Made in	: Romania
Condition As-Received	: Used Product	Reference	: RE260169
Ambient Temperature	: (25 ± 2)°C	Relative Humidity	: (50 ± 15)%RH
Customer name	Okla Testing & Consulting Service Co., Ltd. 67/35-36, 3RD Floor, Phetkasem 7/1 Road, Wat Tha Pra, Bangkok Yai, Bangkok 10600 Thailand		
Received date	: 30 January 2026		
Calibrate date	: 4 February 2026		
Issue date	: 6 February 2026		
Calibrated Location	: Hanna Instruments (Thailand) Ltd.		
Calibration Method	: This calibrator was conducted by using in-house: calibration procedure CP-01, CP-02 by using standard voltage calibrator and certified reference material (CRM).		

Calibrated by : Mr. Pichit Petthong

Approved by :

(Mr. Anan Suwanchaisakul)

Authorized Signatory

Condition of this calibration result :

1. Reference standard instrument : This certificate is traceable to the international system of units (SI Units)

Instrument	Model	Serial No.	Certificate No.	Traceable
Thermometer with sensor	HI98509	39643D	25T1021	Technology Promotion Association (Thailand-Japan)
Digital Thermo-Hygrometer	HT-771SD	AI.07155	26H106	
Documenting Process Calibrator	Fluke 753	43160061	25E2838	

2. Reference Standard Materials: This certificate is traceable to the international system of units (SI Units)

Buffer Solution	Manufacture	Certified Value	Lot Number	Exp. date
pH 4.0	CPA chem Ltd.	4.007 ± 0.006@25°C	1086537	26 April 2026
pH 7.0	CPA chem Ltd.	6.988 ± 0.007@25°C	1138616	28 August 2026
pH 10.0	CPA chem Ltd.	10.011 ± 0.008@25°C	1086538	26 April 2026

Calibration Result :

1. Electrical Potential (without electrode) - DC Voltage measurement

Performing standard curve by Simulator at: (-177.5, 0.0, 177.5) mV

Unit Under Calibration	Nominal Value	Standard Voltage Input	Average Reading		Uncertainty (± mV)
	(pH)	(mV)	(mV)	(pH)	
Meter S/N: 04160019101	4.01	177.50	177.5	4.01	0.097
	7.01	0.00	0.0	7.01	0.058
	10.01	-177.50	-177.5	10.01	0.097

2. Performance of electrode system (with electrode)

Performing standard curve by using buffer nominal : pH (4,7,10)

Unit Under Calibration	Standard pH Buffer Solution	Average Reading		Error (pH)	Uncertainty (± pH)
		(pH)	(mV)		
Electrode S/N: 11271CON	4.007	4.00	165.5	-0.007	0.011
	6.988	6.98	-2.8	-0.008	0.010
	10.011	10.01	-166.1	-0.001	0.014

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95%

** End of certificate **

Certificate No. : C26020020

Page : 1 of 2

CERTIFICATE OF CALIBRATION

Equipment	: pH/ORP and EC/TDS/Salinity/Resistivity Meter		
Meter Model	: HI5521-02	Serial No.	: 04160019101
Probe Model	: HI76312	Serial No.	: 0614117M
Resolution (EC)	: 0.01 μ S/cm	Resolution (EC)	: 0.001 mS/cm
Manufacturer	: Hanna Instruments	Made in	: Romania
Condition As-Received	: Used Product	Reference	: RE260169
Ambient Temperature	: (25 $\pm$ 2)°C	Relative Humidity	: (50 $\pm$ 15)%RH
Customer name	Okla Testing & Consulting Service Co., Ltd. 67/35-36, 3RD Floor, Phetkasem 7/1 Road, Wat Tha Pra, Bangkok Yai, Bangkok 10600 Thailand		
Received date	: 30 January 2026		
Calibrate date	: 16 February 2026		
Issue date	: 17 February 2026		
Calibrated Location	: Hanna Instruments (Thailand) Ltd.		
Calibration Method	: This calibrator was conducted by using in-house: calibration procedure CP-03 by using certified reference material (CRM).		

Calibrated by : Mr. Pichit Petthong

Approved by :

(Mr. Anan Suwanchaisakul)

Authorized Signatory

Condition of this calibration result :

1. Reference standard instrument : This certificate is traceable to the international system of units (SI Units)

Instrument	Model	Serial No.	Certificate No.	Traceable
Thermometer with sensor	HI98509	39643D	25T1021	Technology Promotion Association (Thailand-Japan)
Digital Thermo-Hygrometer	HT-771SD	AI.07155	26H106	

2. Reference Standard Materials: This certificate is traceable to the international system of units (SI Units)

Buffer Solution	Manufacture	Certified Value	Lot Number	Exp. date
84 $\mu\text{S/cm}$	CPA chem Ltd.	$84.003 \pm 0.534@25^{\circ}\text{C}$	1086539	26 April 2026
1.413 mS/cm	CPA chem Ltd.	$1.413 \pm 0.0082@25^{\circ}\text{C}$	1086540	26 April 2026

Calibration Result :

Inspection the accuracy of the EC Meter by using the following certified reference material values.

Calibration result after adjustment at : 84 $\mu\text{S/cm}$, 1.413 mS/cm

Standard EC		Unit Under Calibration Reading		Error	Uncertainty ($\pm$)
Buffer Solution		Before Adjustment	After Adjustment		
84.003	$\mu\text{S/cm}$	68.15 $\mu\text{S/cm}$	85.68 $\mu\text{S/cm}$	1.677 $\mu\text{S/cm}$	0.71 $\mu\text{S/cm}$
1.413	mS/cm	1.241 mS/cm	1.426 mS/cm	0.013 mS/cm	0.011 mS/cm

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95%

**** End of certificate ****



Certificate of Calibration

Certificate No. : MT26-1556

Page : 1 of 2

Customer : OKLA Testing & Consulting Service Co.,Ltd.

Address : 67/35-36 3 Rd Floor, Soi Petchkasem 7/1, Thapra, Bangkok Yai, Bangkok 10600

Description : Incubator

Manufacturer : ศรีอมร

Model : SM61M

Serial No. : 18021147

Identification No. : N/A

Calibration Place : Laboratory

Order No. : 0336/26

Received date : Jan 29, 2026

Calibration date : Jan 29, 2026

Environment Condition :

Temperature : (25+/-10) °C

Humidity : (50+/-30) %RH

Calibration Method : Calibration were conducted using In-house calibration procedure *CP-MT-006* According to comparison with LXI Data Acquisition Switch Unit with sensor. The calibration methods based on Euramet Calibration Guide No.20 - guidelines on the Calibration of Temperature and/or Humidity Controlled Enclosures.

Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
LXI Data Acquisition Switch Unit with Sensor	34972A	MY57003222	MT25-5590	Jul 23, 2026

The effect that the result relate only to the items calibrated. It was found accurate as shown on date and place of calibration only.

Traceability : This measurement are traceable to the International System of Unit (SI), through National Institute of Metrology Thailand (NIMT)

The reported expanded uncertainty of measurement was based on standard uncertainty multiplied by coverage factor $k = 2$, providing a level of confidence of not less than 95%



Calibrated by : Mr.Kriengkrai Jomthaisong

Approved by : 

(Mr.Panuwat Phuklan)

Issue date : Jan 30, 2026

This calibration certificate shall not be reproduced other than in full except with the prior written approval of Inctech Metrological Center Co.,Ltd



Certificate No. : MT26-1556

Page : 2 of 2

Function : Temperature measurement


Result : Without adjustment

Calibration point : 20 °C

Resolution : 0.1 °C

Calibration point (°C)	Temperature of UUC* at each position (°C)									Uncertainty of measurement (+/- °C)
	Ch.1	Ch.2	Ch.3	Ch.4	Ch.5	Ch.6	Ch.7	Ch.8	Ch.9	
20	20.295	20.568	20.013	19.730	19.837	19.932	19.780	19.498	19.791	0.45

Setting temperature (°C)	Indicating Temperature (°C)	Measured stability (+/- °C)	Measured uniformity (°C)	Overall variation (°C)
20.0	20.0	0.32	0.90	1.7

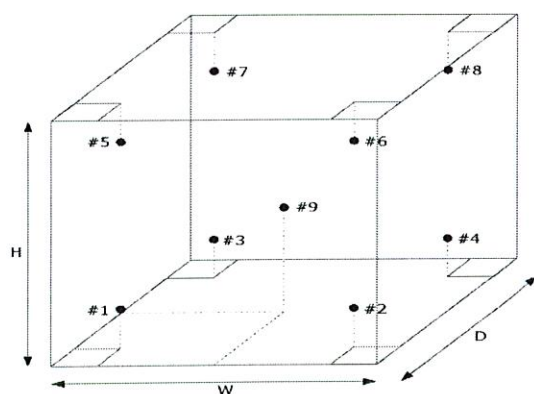

- #1 Lower Left Front
- #2 Lower Right Front
- #3 Lower Left Rear
- #4 Lower Right Rear
- #5 Upper Left Front
- #6 Upper Right Front
- #7 Upper Left Rear
- #8 Upper Right Rear
- #9 Geometric Center

Front view

UUC* = Unit under calibration

Uniformity = Maximum and Minimum difference of measured temperature at any probes and the measured temperature at the reference and same time.

Overall Variation = Difference of temperature value between the maximum and minimum any time.

Stability = One half of the maximum difference of measured temperatures at any one probe.



Certificate of Calibration

Certificate No. : MT26-1558

Page : 1 of 2

Customer : OKLA Testing & Consulting Service Co.,Ltd.

Address : 67/35-36 3 Rd Floor, Soi Petchkasem 7/1, Thapra, Bangkok Yai, Bangkok 10600

Description : Hot Air Oven

Manufacturer : Labtech

Model : LDO-060E

Serial No. : DLCCCL0513C

Identification No. : N/A

Calibration Place : Laboratory

Order No. : 0336/26

Received date : Jan 29, 2026

Calibration date : Jan 29, 2026

Environment Condition :

Temperature : (25+/-10) °C

Humidity : (50+/-30) %RH

Calibration Method : Calibration were conducted using In-house calibration procedure *CP-MT-006* According to comparison with LXI Data Acquisition Switch Unit with sensor. The calibration methods based on Euramet Calibration Guide No.20 - guidelines on the Calibration of Temperature and/or Humidity Controlled Enclosures.

Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
LXI Data Acquisition Switch Unit with Sensor	34972A	MY57003222	MT25-5590	Jul 23, 2026

The effect that the result relate only to the items calibrated. It was found accurate as shown on date and place of calibration only.

Traceability : This measurement are traceable to the International System of Unit (SI), through National Institute of Metrology Thailand (NIMT)

The reported expanded uncertainty of measurement was based on standard uncertainty multiplied by coverage factor $k = 2$, providing a level of confidence of not less than 95%



Calibrated by : Mr.Kriengkrai Jomthaisong

Approved by : 
(Mr.Panuwat Phuklan)

Issue date : Jan 30, 2026

This calibration certificate shall not be reproduced other than in full except with the prior written approval of Inctech Metrological Center Co.,Ltd



Certificate No. : MT26-1558

Page : 2 of 2

Function : Temperature measurement


Result : Without adjustment

Calibration point : 140, 160 °C

Resolution : 1 °C

Calibration point (°C)	Temperature of UUC* at each position (°C)									Uncertainty of measurement (+/- °C)
	Ch.1	Ch.2	Ch.3	Ch.4	Ch.5	Ch.6	Ch.7	Ch.8	Ch.9	
140	141.785	141.603	141.640	141.457	141.689	142.147	141.509	141.574	141.364	3.2
160	161.388	161.667	161.517	161.509	161.431	161.453	161.694	161.753	161.512	2.7

Setting temperature (°C)	Indicating Temperature (°C)	Measured stability (+/- °C)	Measured uniformity (°C)	Overall variation (°C)
140	140	2.7	2.2	5.4
160	160	2.2	2.2	4.9

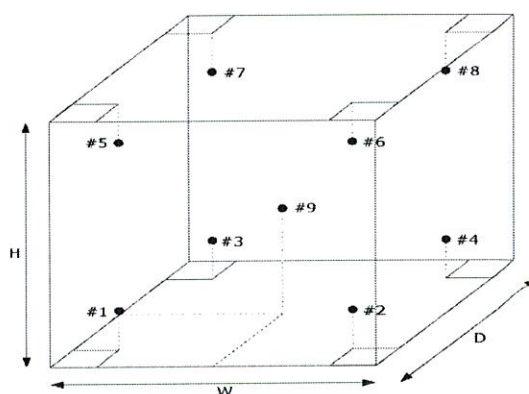

- #1 Lower Left Front
- #2 Lower Right Front
- #3 Lower Left Rear
- #4 Lower Right Rear
- #5 Upper Left Front
- #6 Upper Right Front
- #7 Upper Left Rear
- #8 Upper Right Rear
- #9 Geometric Center

Front view

UUC* = Unit under calibration

Uniformity = Maximum and Minimum difference of measured temperature at any probes and the measured temperature at the reference and same time.

Overall Variation = Difference of temperature value between the maximum and minimum any time.

Stability = One half of the maximum difference of measured temperatures at any one probe.



Certificate of Calibration

Certificate No. : MT26-1557

Page : 1 of 2

Customer : OKLA Testing & Consulting Service Co.,Ltd.

Address : 67/35-36 3 Rd Floor, Soi Petchkasem 7/1, Thapra, Bangkok Yai, Bangkok 10600

Description : Hot Air Oven

Manufacturer : KWF

Model : SOV70B

Serial No. : KWF2021021902

Identification No. : N/A

Calibration Place : Laboratory

Order No. : 0336/26

Received date : Jan 29, 2026

Calibration date : Jan 29, 2026

Environment Condition :

Temperature : (25+/-10) °C

Humidity : (50+/-30) %RH

Calibration Method : Calibration were conducted using In-house calibration procedure *CP-MT-006* According to comparison with LXI Data Acquisition Switch Unit with sensor. The calibration methods based on Euramet Calibration Guide No.20 - guidelines on the Calibration of Temperature and/or Humidity Controlled Enclosures.

Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
LXI Data Acquisition Switch Unit with Sensor	34972A	MY57003222	MT25-5590	Jul 23, 2026

The effect that the result relate only to the items calibrated. It was found accurate as shown on date and place of calibration only.

Traceability : This measurement are traceable to the International System of Unit (SI), through National Institute of Metrology Thailand (NIMT)

The reported expanded uncertainty of measurement was based on standard uncertainty multiplied by coverage factor $k = 2$, providing a level of confidence of not less than 95%



Calibrated by : Mr.Kriengkrai Jomthaisong

Approved by : 

(Mr.Panuwat Phuklan)


Issue date : Jan 30, 2026

This calibration certificate shall not be reproduced other than in full except with the prior written approval of Inctech Metrological Center Co.,Ltd

Certificate No. : MT26-1557
Page : 2 of 2
Function : Temperature measurement
Result : Without adjustment
Calibration point : 80, 104, 180 °C
Resolution : 0.1 °C

Calibration point (°C)	Temperature of UUC* at each position (°C)									Uncertainty of measurement (+/- °C)
	Ch.1	Ch.2	Ch.3	Ch.4	Ch.5	Ch.6	Ch.7	Ch.8	Ch.9	
80	80.277	80.877	79.915	80.312	80.617	80.154	79.991	80.587	80.074	0.51
104	104.268	104.528	104.228	104.120	104.485	104.519	104.304	104.664	104.154	0.71
180	180.400	180.880	180.314	180.356	180.450	180.243	180.266	180.540	180.400	1.3

Setting temperature (°C)	Indicating Temperature (°C)	Measured stability (+/- °C)	Measured uniformity (°C)	Overall variation (°C)
80.0	79.9 to 80.1	0.35	1.1	1.5
104.0	104.0 to 104.2	0.56	0.81	1.5
180.0	180.0 to 180.2	1.1	1.2	2.1

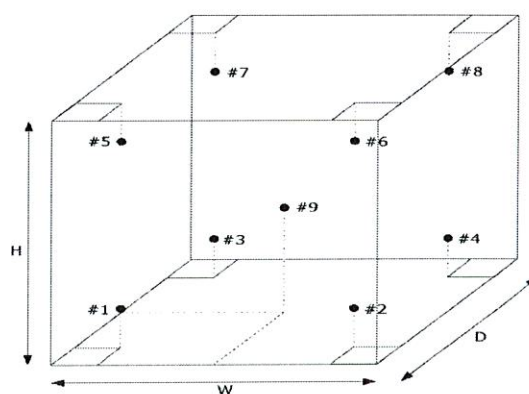

- #1 Lower Left Front
- #2 Lower Right Front
- #3 Lower Left Rear
- #4 Lower Right Rear
- #5 Upper Left Front
- #6 Upper Right Front
- #7 Upper Left Rear
- #8 Upper Right Rear
- #9 Geometric Center

Front view
UUC* = Unit under calibration

Uniformity = Maximum and Minimum difference of measured temperature at any probes and the measured temperature at the reference and same time.

Overall Variation = Difference of temperature value between the maximum and minimum any time.

Stability = One half of the maximum difference of measured temperatures at any one probe.



Certificate of Calibration

Certificate No. : MM26-1194

Page : 1 of 3

Customer : Okla Testing & Consulting Service Co.,Ltd.

Address : 67/35-36 3 rd Floor, Soi Petchkasem 7/1, Thapra, Bangkok Yai, Bangkok 10600

Description : Electronic Balance

Manufacturer : Sartorius

Model : BSA224S-CW

Serial No. : 35790699

Identification No. : N/A

Calibration Place : Balance Room

Order No. : 0336/26

Received date : Jan 29, 2026

Calibration date : Jan 29, 2026

Environment Condition :

Temperature : (25+/-10) °C

Humidity : (50+/-30) %RH

Atm. Pressure : (1010+/-10) hPa

Calibration Method : Calibration were conducted using In-house calibration procedure CP-MM-001
According to comparison with Standard Weight Set E1.

The calibration methods based on UKAS - LAB 14 : 2022

Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
Standard Weight Set	NC-001-0.2K-E1-ASS	0022	PL-512	Oct 10, 2026

The effect that the result relate only to the items calibrated. If was found accurate as shown on date and place of calibration only.

Traceability : This measurement are traceable to the International System of Unit (SI), through
National Institute of Metrology Thailand (NIMT)

The reported expanded uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k = 2, providing a level of confidence of not less than 95%



Calibrated by : Mr.Porntep Homchuay

Approved by : 
(Miss.Valailuck Janyanitas)

Issue date : Feb 02, 2026

This calibration certificate shall not be reproduced other than in full except with the prior written approval of Intech Metrological Center Co.,Ltd


Certificate No. : MM26-1194

Page : 2 of 3

Calibration Result : Without Adjustment


Function : Repeatability

Maximum Capacity : 200 g


Resolution : 0.0001 g

Nominal Weight Value	Instrument Deviation of Reading
(g)	(g)
200	0.0000

Calibration Result : Without Adjustment

Function : Effect of Off Center Loading


Front
(X)



Front
()

A Mass of 100 Was Placed to various Position on the pan.

The Weight Machine Reading Obtained is Given in The Tabel

Load	Measuring Positions					Maximum Different
	A	B	C	D	E	
(g)	(g)	(g)	(g)	(g)	(g)	(g)
100	99.9996	99.9995	99.9996	99.9996	99.9997	99.9996
						0.0002

Calibration Result : Without Adjustment

Function : Effect of Tare

Nominal Tare Weight	Standard Weight	UUC* Reading	UUC* Deviation
(g)	(g)	(g)	(g)
	Tare	0.0000	0.0000
	At 20 %	20	19.9998
	At 40 %	40	39.9998
	At 60 %	60	59.9997
	At 80 %	80	79.9997
	At 100 %	100	99.9996
100			
			0.0002
			0.0002
			0.0003
			0.0003
			0.0004

UUC* = Unit Under Calibration

**Inctech Metrological Center Co.Ltd.**

39/1 Soi 82, Sukhapiban 5 Rd., O ngoen,

Saimai, Bangkok 10220, Thailand

Tel. (662) 909-8820 (Auto 10 lines) www.imcinstrument.com

Calibration Cert. # 3884.01
ISO/IEC 17025

Certificate No. : MM26-1194

Page : 3 of 3

Calibration Result : Before Adjustment

Function : Departure of indication from nominal value

Standard Weight Value (g)	UUC* Reading (g)	UUC* Correction (g)	Uncertainty of Measurement (+/- g)
0.00000	0.0000	0.00000	0.000058
0.01000	0.0099	0.00010	0.000058
0.05000	0.0499	0.00007	0.000058
0.10000	0.1001	-0.00014	0.000058
0.20000	0.2001	-0.00014	0.000059
0.50000	0.5000	-0.00003	0.000059
1.00000	1.0000	-0.00003	0.000059
10.00001	10.0000	-0.00003	0.000064
49.99999	49.9998	0.00022	0.000090
99.99998	99.9996	0.00041	0.00014
149.99997	149.9991	0.00083	0.00027
199.99996	199.9991	0.00083	0.00027

UUC* = Unit Under Calibration

Calibration Result : After Adjustment

Standard Weight Value (g)	UUC* Reading (g)	UUC* Correction (g)	Uncertainty of Measurement (+/- g)
0.00000	0.0000	0.00000	0.000058
0.01000	0.0100	-0.00003	0.000058
0.05000	0.0500	0.00000	0.000058
0.10000	0.1000	0.00000	0.000058
0.20000	0.2000	-0.00003	0.000059
0.50000	0.5000	0.00000	0.000059
1.00000	1.0000	-0.00003	0.000059
10.00001	10.0000	-0.00001	0.000064
49.99999	50.0000	-0.00002	0.000090
99.99998	100.0000	0.00002	0.00014
149.99997	150.0000	0.00000	0.00027
199.99996	200.0000	0.00004	0.00027

UUC* = Unit Under Calibration



Inctech Metrological Center Co.Ltd.

39/1 Soi 82, Sukhapiban 5 Rd., O ngoen,

Saimai, Bangkok 10220, Thailand

Tel. (662) 909-8820 (Auto 10 lines) www.imcinstrument.com



Calibration Cert. # 3884.01
ISO/IEC 17025

Certificate of Calibration

Certificate No. : MM26-1195

Page : 1 of 3

Customer : Okla Testing & Consulting Service Co.,Ltd.

Address : 67/35-36 3 rd Floor, Soi Petchkasem 7/1, Thapra, Bangkok Yai, Bangkok 10600

Description : Electronic Balance

Manufacturer : Mettler Toledo

Model : PL6001-S

Serial No. : 1230510473

Identification No. : N/A

Calibration Place : Balance Room

Order No. : 0336/26

Received date : Jan 29, 2026

Calibration date : Jan 29, 2026

Environment Condition :

Temperature : (25+/-10) °C

Humidity : (50+/-30) %RH

Atm. Pressure : (1010+/-10) hPa

Calibration Method : Calibration were conducted using In-house calibration procedure CP-MM-001

According to comparison with Standard Weight Set.

The calibration methods based on UKAS - LAB 14 : 2022

Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
Standard Weight Set	50 mg - 2 kg	N/A	MM25-1949	May 22, 2026

The effect that the result relate only to the items calibrated. If was found accurate as shown on date and place of calibration only.

Traceability : This measurement are traceable to the International System of Unit (SI), through National Institute of Metrology Thailand (NIMT)

The reported expanded uncertainty of measurement was based on standard uncertainty multiplied by coverage factor $k = 2$, providing a level of confidence of not less than 95%



Calibrated by : Mr.Porntep Homchuay

Approved by : (Miss.Valailuck Janyanitas)

Issue date : Feb 02, 2026

This calibration certificate shall not be reproduced other than in full except with the prior written approval of Inctech Metrological Center Co.,Ltd



Certificate No. : MM26-1195

Page : 2 of 3

Calibration Result : Without Adjustment

Function : Repeatability



Maximum Capacity : 6000 g

Resolution : 0.1 g

Nominal Weight Value	Instrument Deviation of Reading
(g)	(g)
6000	0.0

Calibration Result : Without Adjustment

Function : Effect of Off Center Loading

Front
(X)Front
()

A Mass of 2000 Was Placed to various Position on the pan.

The Weight Machine Reading Obtained is Given in The Tabel

Load	Measuring Positions					Maximum Different
	A	B	C	D	E	
(g)	(g)	(g)	(g)	(g)	(g)	(g)
2000	2000.0	2000.0	2000.0	2000.0	2000.0	2000.0
						0.0

Calibration Result : Without Adjustment

Function : Effect of Tare

Nominal Tare Weight	Standard Weight	UUC* Reading	UUC* Deviation
(g)	(g)	(g)	(g)
	Tare	0.0	0.0
3000	At 20 % 600	600.0	0.0
	At 40 % 1200	1200.0	0.0
	At 60 % 1800	1800.0	0.0
	At 80 % 2400	2400.0	0.0
	At 100 % 3000	3000.0	0.0

UUC* = Unit Under Calibration



Certificate No. : MM26-1195

Page : 3 of 3

Calibration Resu : Without Adjustment

Function : Departure of indication from nominal value

Standard Weight Value (g)	UUC* Reading (g)	UUC* Correction (g)	Uncertainty of Measurement (+/- g)
0	0.0	0.0	0.058
600	600.0	0.0	0.058
1200	1200.0	0.0	0.058
1800	1800.0	0.0	0.058
2400	2400.0	0.0	0.058
3000	3000.0	0.0	0.058
3600	3600.0	0.0	0.058
4200	4200.0	0.0	0.058
4800	4800.0	0.0	0.058
5400	5400.0	0.0	0.058
6000	6000.0	0.0	0.058

UUC* = Unit Under Calibration



Inctech Metrological Center Co.Ltd.

39/1 Soi 82, Sukhapiban 5 Rd., O ngoen,

Saimai, Bangkok 10220, Thailand

Tel. (662) 909-8820 (Auto 10 lines) www.imcinstrument.com



Calibration Cert. # 3884.01
ISO/IEC 17025

Certificate of Calibration

Certificate No. : MM26-1196

Page : 1 of 3

Customer : Okla Testing & Consulting Service Co.,Ltd.
Address : 67/35-36 3 rd Floor, Soi Petchkasem 7/1, Thapra, Bangkok Yai, Bangkok 10600

Description : Electronic Balance
Manufacturer : Mettler Toledo
Model : PL3001-S
Serial No. : 1230040028
Identification No. : N/A
Calibration Place : Balance Room

Order No. : 0336/26
Received date : Jan 29, 2026
Calibration date : Jan 29, 2026
Environment Condition :
Temperature : (25+/-10) °C
Humidity : (50+/-30) %RH
Atm. Pressure : (1010+/-10) hPa

Calibration Method : Calibration were conducted using In-house calibration procedure CP-MM-001
According to comparison with Standard Weight Set.
The calibration methods based on UKAS - LAB 14 : 2022

Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
Standard Weight Set	50 mg - 2 kg	N/A	MM25-1949	May 22, 2026

The effect that the result relate only to the items calibrated. If was found accurate as shown on date and place of calibration only.

Traceability : This measurement are traceable to the International System of Unit (SI), through
National Institute of Metrology Thailand (NIMT)

The reported expanded uncertainty of measurement was based on standard uncertainty multiplied by coverage factor $k = 2$, providing a level of confidence of not less than 95%



Calibrated by : Mr.Porntep Homchuay

Approved by : 
(Miss.Valailuck Janyanitas)

Issue date : Feb 02, 2026

This calibration certificate shall not be reproduced other than in full except with the prior written approval of Inctech Metrological Center Co.,Ltd


Certificate No. : MM26-1196

Page : 2 of 3

Calibration Result : Without Adjustment


Function : Repeatability

Maximum Capacity : 3100 g


Resolution : 0.1 g

Nominal Weight Value	Instrument Deviation of Reading
(g)	(g)
3000	0.0

Calibration Result : Without Adjustment

Function : Effect of Off Center Loading


Front
(X)



Front
()

A Mass of 1000 Was Placed to various Position on the pan.

The Weight Machine Reading Obtained is Given in The Tabel

Load	Measuring Positions					Maximum Different
	A	B	C	D	E	
(g)	(g)	(g)	(g)	(g)	(g)	(g)
1000	999.9	999.9	999.9	999.9	999.9	0.0

Calibration Result : Without Adjustment

Function : Effect of Tare

Nominal Tare Weight	Standard Weight	UUC* Reading	UUC* Deviation
(g)	(g)	(g)	(g)
	Tare	0.0	0.0
1500	At 20 % 300	299.9	0.1
	At 40 % 600	599.9	0.1
	At 60 % 900	899.9	0.1
	At 80 % 1200	1199.9	0.1
	At 100 % 1500	1499.9	0.1

UUC* = Unit Under Calibration



Certificate No. : MM26-1196

Page : 3 of 3

Calibration Resu : Without Adjustment

Function : Departure of indication from nominal value

Standard Weight Value (g)	UUC* Reading (g)	UUC* Correction (g)	Uncertainty of Measurement (+/- g)
0	0.0	0.0	0.058
300	299.9	0.1	0.058
600	599.9	0.1	0.058
900	899.9	0.1	0.058
1200	1199.9	0.1	0.058
1500	1499.9	0.1	0.058
1800	1799.9	0.1	0.058
2100	2099.8	0.2	0.058
2400	2399.8	0.2	0.058
2700	2699.8	0.2	0.058
3000	2999.7	0.3	0.058

UUC* = Unit Under Calibration

Certificate No. : C26020022

Page : 1 of 2

CERTIFICATE OF CALIBRATION

Equipment	: Dissolved Oxygen and BOD Meter		
Meter Model	: HI5421-02	Serial No.	: 04240005101
Probe Model	: HI76483	Serial No.	: KC1N66J5P
Manufacturer	: Hanna Instruments	Made in	: Romania
Condition As-Received	: Used Product	Resolution	: 0.01 ppm (mg/L)
Ambient Temperature	: (25 ± 2)°C	Relative Humidity	: (50 ± 15)% RH
Reference	: RE260168		
Customer name	: Okla Testing & Consulting Service Co., Ltd.		
	67/35-36, 3RD Floor, Phetkasem 7/1 Road, Wat Tha Pra,		
	Bangkok Yai, Bangkok 10600 Thailand		
Received date	: 30 January 2026		
Calibrate date	: 6 February 2026		
Issue date	: 9 February 2026		
Calibrated Location	: Hanna Instruments (Thailand) Ltd.		
Calibration Procedure	: This calibrator was conducted by using in-house: calibration procedure		
	CP-11 by using certified reference material (CRM).		

Calibrated by : Mr. Pichit Petthong

Approved by :

(Mr. Anan Suwanchaisakul)

Authorized Signatory

Condition of this result of calibration :

1. Reference standard instrument : This certificate is traceable to the international system of units (SI Units)

Instrument	Model	Serial No.	Certificate No.	Traceable
Thermometer with sensor	HI98509	39643D	25T1021	Technology Promotion Association (Thailand-Japan)
Digital Thermo-Hygrometer	HT-771SD	AI.07155	26H106	

2. Reference standard materials: This certificate is traceable to the international system of units (SI Units)

Buffer Solution	Manufacture	Certified Value	Lot Number	Exp. date
Zero Oxygen Solution	Hanna Inc.	0.0 ± 0.1@25°C	S0121/25	August 2030

Calibration Result:

Dissolved Oxygen Measurement

Unit Under Calibration	Standard Buffer Solution	UUC Reading	Error	Uncertainty of Measurement (±)
DO Electrode	0.0 mg/L	0.00 mg/L	0.00 mg/L	N/A mg/L
S/N: KC1N66J5P	8.3 mg/L	8.30 mg/L	0.00 mg/L	0.33 mg/L

Remark : at 8.3 mg/L = Air Saturated.

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95%

**** End of certificate ****

Certificate of Calibration

Certificate No. : 69-300065-1

Page : 1 of 2

Submitted by : Okla Testing & Consulting Service Co.,Ltd.
67/35-36, 3rd Floor, Petchkasem 7/1, Petchkasem Rd.,
Wathapra, Bangkok Yai, Bangkok 10600 Thailand

Equipment : Burette
Manufacturer : ISOLAB Class : A
Capacity : 25 ml Graduation : 0.05 ml
ID No. : EM-MBR10002/17

Environment : Ambient Temperature : (20 ± 3) °C
Relative Humidity : (50 ± 10) %
Air Pressure : 1010.5 mbar.

Date of Received : 22 January 2026

Date of Calibration : 29 January 2026

Date of Issue : 29 January 2026

Calibrated by : Areerat Sombun

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-22

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241005	68-200260-4	02 Jun 2026	National Institute of Metrology (Thailand) (NIMT)

Approved by :

(Wipa Tovadee)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 69-300065-1

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Delivery Time : 49.07 sec.


Nominal Volume (ml)	Measuring Volume (ml)
5	4.9984
15	14.9932
25	24.9964

Uncertainty of measurement with in $\pm$ 0.0066 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Page : 1 of 2

Certificate No. : 69-300065-2

Submitted by : Okla Testing & Consulting Service Co.,Ltd.
67/35-36, 3rd Floor, Petchkasem 7/1, Petchkasem Rd.,
Watthapra, Bangkok Yai, Bangkok 10600 Thailand

Equipment : Burette
Manufacturer : Witeg Class : A
Capacity : 100 ml Graduation : 0.2 ml
ID No. : EM-MBR10001/18

Environment : Ambient Temperature : (20 ± 3) °C
Relative Humidity : (50 ± 10) %
Air Pressure : 1015.6 mbar.

Date of Received : 22 January 2026

Date of Calibration : 29 January 2026

Date of Issue : 29 January 2026

Calibrated by : Areerat Sombun

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-22

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241005	68-200260-4	02 Jun 2026	National Institute of Metrology (Thailand) (NIMT)

Approved by :

(Wipa Tovadee)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 69-300065-2

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Delivery Time : 43.77 sec.


Nominal Volume (ml)	Measuring Volume (ml)
20	19.9961
60	59.9874
100	99.9963

Uncertainty of measurement with in $\pm$ 0.019 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 69-300065-3

Page : 1 of 2

Submitted by : Okla Testing & Consulting Service Co.,Ltd.
67/35-36, 3rd Floor, Petchkasem 7/1, Petchkasem Rd.,
Watthapra, Bangkok Yai, Bangkok 10600 Thailand

Equipment : Measuring Pipette
Manufacturer : GLASSCO Class : A
Capacity : 1 ml Graduation : 0.01 ml
ID No. : EM-MER01001/19

Environment : Ambient Temperature : (20 ± 3) °C
Relative Humidity : (50 ± 10) %
Air Pressure : 1010.5 mbar.

Date of Received : 22 January 2026

Date of Calibration : 29 January 2026

Date of Issue : 29 January 2026

Calibrated by : Areerat Sombun

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-22

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241005	68-200260-4	02 Jun 2026	National Institute of Metrology (Thailand) (NIMT)

Approved by :

(Wipa Tovadee)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 69-300065-3

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Delivery Time : 7.31 sec.

Nominal Volume (ml)	Measuring Volume (ml)
0.1	0.1014
0.5	0.4995
1	0.9908

Uncertainty of measurement with in $\pm$ 0.0026 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 69-300065-4

Page : 1 of 2

Submitted by : Okla Testing & Consulting Service Co.,Ltd.
67/35-36, 3rd Floor, Petchkasem 7/1, Petchkasem Rd.,
Wathapra, Bangkok Yai, Bangkok 10600 Thailand

Equipment : Measuring Pipette
Manufacturer : GLASSCO Class : A
Capacity : 5 ml Graduation : 0.05 ml
ID No. : EM-MER01001/18

Environment : Ambient Temperature : (20 ± 3) °C
Relative Humidity : (50 ± 10) %
Air Pressure : 1010.5 mbar.

Date of Received : 22 January 2026

Date of Calibration : 29 January 2026

Date of Issue : 29 January 2026

Calibrated by : Areerat Sombun

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-22

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241005	68-200260-4	02 Jun 2026	National Institute of Metrology (Thailand) (NIMT)

Approved by :

(Wipa Tovadee)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 69-300065-4

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Delivery Time : 9.39 sec.


Nominal Volume (ml)	Measuring Volume (ml)
0.5	0.5001
2.5	2.4840
5	4.9842

Uncertainty of measurement with in $\pm$ 0.0027 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Page : 1 of 2

Certificate No. : 69-300065-5

Submitted by : Okla Testing & Consulting Service Co.,Ltd.
67/35-36, 3rd Floor, Petchkasem 7/1, Petchkasem Rd.,
Wattapra, Bangkok Yai, Bangkok 10600 Thailand

Equipment : Measuring Pipette
Manufacturer : GLASSCO Class : A
Capacity : 10 ml Graduation : 0.1 ml
ID No. : EM-MER01001/17

Environment : Ambient Temperature : (20 ± 3) °C
Relative Humidity : (50 ± 10) %
Air Pressure : 1010.5 mbar.

Date of Received : 22 January 2026

Date of Calibration : 29 January 2026

Date of Issue : 29 January 2026

Calibrated by : Areerat Sombun

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-22

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241005	68-200260-4	02 Jun 2026	National Institute of Metrology (Thailand) (NIMT)

Approved by :

(Wipa Tovadee)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 69-300065-5

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Delivery Time : 10.81 sec.


Nominal Volume (ml)	Measuring Volume (ml)
1	1.0008
5	4.9757
10	9.9777

Uncertainty of measurement with in $\pm$ 0.0039 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 69-300065-6

Page : 1 of 2

Submitted by : Okla Testing & Consulting Service Co.,Ltd.
67/35-36, 3rd Floor, Petchkasem 7/1, Petchkasem Rd.,
Wattapra, Bangkok Yai, Bangkok 10600 Thailand

Equipment : Volumetric Pipette
Manufacturer : GLASSCO Class : A
Capacity : 5 ml
ID No. : EM-Mbro1051/17

Environment : Ambient Temperature : (20 ± 3) °C
Relative Humidity : (50 ± 10) %
Air Pressure : 1010.7 mbar.

Date of Received : 22 January 2026

Date of Calibration : 29 January 2026

Date of Issue : 29 January 2026

Calibrated by : Areerat Sombun

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-22

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241005	68-200260-4	02 Jun 2026	National Institute of Metrology (Thailand) (NIMT)

Approved by :

(Wipa Tovadee)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 69-300065-6

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Delivery Time : 12.56 sec.

Nominal Volume (ml)	Measuring Volume (ml)
5	4.9820

Uncertainty of measurement with in $\pm$ 0.0026 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Page : 1 of 2

Certificate No. : 69-300065-7

Submitted by : Okla Testing & Consulting Service Co.,Ltd.
67/35-36, 3rd Floor, Petchkasem 7/1, Petchkasem Rd.,
Watthapra, Bangkok Yai, Bangkok 10600 Thailand

Equipment : Volumetric Pipette
Manufacturer : GLASSCO Class : A
Capacity : 10 ml
ID No. : EM-Mbro1001/17

Environment : Ambient Temperature : (20 ± 3) °C
Relative Humidity : (50 ± 10) %
Air Pressure : 1010.7 mbar.

Date of Received : 22 January 2026

Date of Calibration : 29 January 2026

Date of Issue : 29 January 2026

Calibrated by : Areerat Sombun

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-22

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241005	68-200260-4	02 Jun 2026	National Institute of Metrology (Thailand) (NIMT)

Approved by :

(Wipa Tovadee)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Page : 2 of 2

Certificate No. : 69-300065-7

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Delivery Time : 12.56 sec.


Nominal Volume (ml)	Measuring Volume (ml)
10	10.0044

Uncertainty of measurement with in $\pm$ 0.0038 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- oOo -



Certificate of Calibration

Certificate No. : 69-300065-8

Page : 1 of 2

Submitted by : Okla Testing & Consulting Service Co.,Ltd.
67/35-36, 3rd Floor, Petchkasem 7/1, Petchkasem Rd.,
Wattapra, Bangkok Yai, Bangkok 10600 Thailand

Equipment : Volumetric Pipette
Manufacturer : GLASSCO Class : A
Capacity : 20 ml
ID No. : EM-VPP20201/17

Environment : Ambient Temperature : (20 ± 3) °C
Relative Humidity : (50 ± 10) %
Air Pressure : 1010.7 mbar.

Date of Received : 22 January 2026

Date of Calibration : 29 January 2026

Date of Issue : 29 January 2026

Calibrated by : Areerat Sombun

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-22

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241005	68-200260-4	02 Jun 2026	National Institute of Metrology (Thailand) (NIMT)

Approved by :

(Wipa Tovadee)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 69-300065-8

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Delivery Time : 15.10 sec.

Nominal Volume (ml)	Measuring Volume (ml)
20	19.9816

Uncertainty of measurement with in $\pm$ 0.0064 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 69-300065-9

Page : 1 of 2

Submitted by : Okla Testing & Consulting Service Co.,Ltd.
67/35-36, 3rd Floor, Petchkasem 7/1, Petchkasem Rd.,
Watthapra, Bangkok Yai, Bangkok 10600 Thailand

Equipment : Volumetric Pipette
Manufacturer : BOROSIL Class : A
Capacity : 25 ml
ID No. : EM-VPP02501/17

Environment : Ambient Temperature : (20 ± 3) °C
Relative Humidity : (50 ± 10) %
Air Pressure : 1010.7 mbar.

Date of Received : 22 January 2026

Date of Calibration : 29 January 2026

Date of Issue : 29 January 2026

Calibrated by : Areerat Sombun

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-22

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241005	68-200260-4	02 Jun 2026	National Institute of Metrology (Thailand) (NIMT)

Approved by :

(Wipa Tovadee)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 69-300065-9

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Delivery Time : 37.49 sec.


Nominal Volume (ml)	Measuring Volume (ml)
25	24.9902

Uncertainty of measurement with in $\pm$ 0.0066 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 69-300065-13

Page : 1 of 2

Submitted by : Okla Testing & Consulting Service Co.,Ltd.
67/35-36, 3rd Floor, Petchkasem 7/1, Petchkasem Rd.,
Watthapra, Bangkok Yai, Bangkok 10600 Thailand

Equipment : Cylinder
Manufacturer : FAVORIT Class : A
Capacity : 50 ml Graduation : 1 ml
ID No. : CY50/01

Environment : Ambient Temperature : (20 ± 3) °C
Relative Humidity : (50 ± 10) %
Air Pressure : 1011.1 mbar.

Date of Received : 22 January 2026

Date of Calibration : 29 January 2026

Date of Issue : 29 January 2026

Calibrated by : Areerat Sombun

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-22

Reference Standard Instrument : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241002	68-200620-1	02 Jun 2026	National Institute of Metrology (Thailand) (NIMT)

Approved by :

(Wipa Tovadee)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 69-300065-13

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good


Nominal Volume (ml)	Measuring Volume (ml)
50	50.38

Uncertainty of measurement with in $\pm$ 0.054 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 69-300065-14

Page : 1 of 2

Submitted by : Okla Testing & Consulting Service Co.,Ltd.
67/35-36, 3rd Floor, Petchkasem 7/1, Petchkasem Rd.,
Wattapra, Bangkok Yai, Bangkok 10600 Thailand

Equipment : Cylinder
Manufacturer : DURAN Class : A
Capacity : 100 ml Graduation : 1 ml
ID No. : CY100/01

Environment : Ambient Temperature : (20 ± 3) °C
Relative Humidity : (50 ± 10) %
Air Pressure : 1011.1 mbar.

Date of Received : 22 January 2026

Date of Calibration : 29 January 2026

Date of Issue : 29 January 2026

Calibrated by : Areerat Sombun

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-22

Reference Standard Instrument : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241002	68-200620-1	02 Jun 2026	National Institute of Metrology (Thailand) (NIMT)

Approved by :

(Wipa Tovadee)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 69-300065-14

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good


Nominal Volume (ml)	Measuring Volume (ml)
50	50.26
100	100.08

Uncertainty of measurement with in $\pm$ 0.063 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 69-300065-15

Page : 1 of 2

Submitted by : Okla Testing & Consulting Service Co.,Ltd.
67/35-36, 3rd Floor, Petchkasem 7/1, Petchkasem Rd.,
Wathapra, Bangkok Yai, Bangkok 10600 Thailand

Equipment : Cylinder
Manufacturer : BOROSIL Class : A
Capacity : 500 ml Graduation : 5 ml
ID No. : 0334-58

Environment : Ambient Temperature : (20 ± 3) °C
Relative Humidity : (50 ± 10) %
Air Pressure : 1011.1 mbar.

Date of Received : 22 January 2026

Date of Calibration : 29 January 2026

Date of Issue : 29 January 2026

Calibrated by : Areerat Sombun

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-22

Reference Standard Instrument : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241002	68-200620-1	02 Jun 2026	National Institute of Metrology (Thailand) (NIMT)

Approved by

(Wipa Tovadee)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 69-300065-15

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good


Nominal Volume (ml)	Measuring Volume (ml)
500	499.05

Uncertainty of measurement with in $\pm$ 0.12 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 69-300065-10

Page : 1 of 2

Submitted by : Okla Testing & Consulting Service Co.,Ltd.
67/35-36, 3rd Floor, Petchkasem 7/1, Petchkasem Rd.,
Wattapra, Bangkok Yai, Bangkok 10600 Thailand

Equipment : Volumetric Flask
Manufacturer : SCI Class : A
Capacity : 100 ml
ID No. : EM-VPP02501/17

Environment : Ambient Temperature : (20 ± 3) °C
Relative Humidity : (50 ± 10) %
Air Pressure : 1011.1 mbar.

Date of Received : 22 January 2026

Date of Calibration : 29 January 2026

Date of Issue : 29 January 2026

Calibrated by : Areerat Sombun


Calibration Method : In-house method CAL-M3001 based on ASTM E 542-22

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241005	68-200260-4	02 Jun 2026	National Institute of Metrology (Thailand) (NIMT)

Approved by :



(Wipa Tovadee)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 69-300065-10

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good


Nominal Volume (ml)	Measuring Volume (ml)
100	99.991

Uncertainty of measurement with in $\pm$ 0.018 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 69-300065-11

Page : 1 of 2

Submitted by : Okla Testing & Consulting Service Co.,Ltd.
67/35-36, 3rd Floor, Petchkasem 7/1, Petchkasem Rd.,
Wattthapra, Bangkok Yai, Bangkok 10600 Thailand

Equipment : Volumetric Flask
Manufacturer : Borosil Class : A
Capacity : 500 ml
ID No. : EM-VPP02501/18

Environment : Ambient Temperature : (20 ± 3) °C
Relative Humidity : (50 ± 10) %
Air Pressure : 1010.9 mbar.

Date of Received : 22 January 2026

Date of Calibration : 29 January 2026

Date of Issue : 29 January 2026

Calibrated by : Arcerat Sombun

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-22

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241002	68-200620-1	02 Jun 2026	National Institute of Metrology (Thailand) (NIMT)

Approved by :

(Wipa Tovadee)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 69-300065-11

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good


Nominal Volume (ml)	Measuring Volume (ml)
500	499.99

Uncertainty of measurement with in $\pm$ 0.075 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- oOo -



Certificate of Calibration

Certificate No. : 69-300065-12

Page : 1 of 2

Submitted by : Okla Testing & Consulting Service Co.,Ltd.
67/35-36, 3rd Floor, Petchkasem 7/1, Petchkasem Rd.,
Watthapra, Bangkok Yai, Bangkok 10600 Thailand

Equipment : Volumetric Flask
Manufacturer : Borosil Class : A
Capacity : 1000 ml
ID No. : EM-VPP02501/20

Environment : Ambient Temperature : (20 ± 3) °C
Relative Humidity : (50 ± 10) %
Air Pressure : 1011.0 mbar.

Date of Received : 22 January 2026

Date of Calibration : 29 January 2026

Date of Issue : 29 January 2026

Calibrated by : Areerat Sombun

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-22

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241002	68-200620-1	02 Jun 2026	National Institute of Metrology (Thailand) (NIMT)

Approved by :

(Wipa Tovadee)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 69-300065-12

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good


Nominal Volume (ml)	Measuring Volume (ml)
1000	1000.00

Uncertainty of measurement with in $\pm$ 0.14 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- oOo -



Certificate of Calibration

Certificate No. : 69-200144-1

Page : 1 of 2

Submitted by : HVE Co.,Ltd.

603 Soi Jarunsanitwong 46, Jarunsanitwong Road, Bangyeekun, Bangplad, Bangkok 10700

Equipment : Electronic Balance

Manufacturer : SHIMADZU **Model :** ATX224R

Serial No. : D326005191

Capacity : 220 g **Resolution :** 0.0001 g

Environment : On site calibration was carried out at the Laboratory, HVE Co.,Ltd.

Ambient Temperature : (28.9 to 29.6) °C

Relative Humidity : (52.7 to 54.9) %

Air Pressure : 1007.0 mbar

Date of Received : 20 April 2026

Date of Calibration : 20 April 2026

Date of Issue : 21 April 2026

Calibrated by : Akaradath Thippichai

Calibration Method : In-house method CAL-M2001 based on UKAS Publication ref : LAB 14

Edition 7 - November 2022

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

ID No.	Cert. No.	Due Date	Traceability
E261-E2624	C02251973	07 Nov 2026	National Institute of Metrology (Thailand), (NIMT)

Approved by :

(Satja Sangkhum)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 69-200144-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Departure of indication from nominal value

Nominal Value (g)	Correction (g)	Uncertainty $\pm$ (g)
0.01	0.0000	0.00012
0.1	0.0000	0.00012
0.5	0.0000	0.00013
1	-0.0001	0.00013
10	-0.0001	0.00013
20	-0.0002	0.00014
50	-0.0002	0.00015
100	-0.0002	0.00020
150	-0.0003	0.00038
200	-0.0002	0.00038


This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.06$, providing a level of confidence of approximately 95%

Eccentric error

Load test : 50 g

A	B	C	D	E	
-0.0001	0.0000	0.0002	0.0001	0.0000	g



Repeatability

Load test : 200 g

Sidev. : 0.00005 g

- oOo -



Certificate of Calibration

Certificate No. : 69-400207-5

Page : 1 of 2

Submitted by : HVE Co., Ltd.

603 Soi Jarunsanitwong 46, Jarunsanitwong Road, Bangyeekun, Bangplad, Bangkok 10701

Equipment : Temperature controlled enclosure (Oven)

Manufacturer : Memmert

Model : UNB 500

Range : N/A °C

Resolution : 0.5 °C

Serial No. : C507.1007

ID No. : 012

Environment : On site calibration was carried out at the Laboratory, HVE Co., Ltd.

Ambient Temperature : (27.9 to 31.3) °C

Relative Humidity : (42 to 68) %

Line Voltage : (229.0 to 230.0) V

Date of Received : 20 April 2026

Date of Calibration : 20 April 2026

Date of Issue : 23 April 2026

Calibrated by : Aphisorn Worawasukullaya

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Digital Thermometer with Thermocouple probe

ID No.

Cert. No.

Due Date

Traceability

400046 & 400023 69-400119-1

26 Sep 2026

National Institute of Metrology Thailand (NIMT)

Approved by :



(Permon Chanpu)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 69-400207-5


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

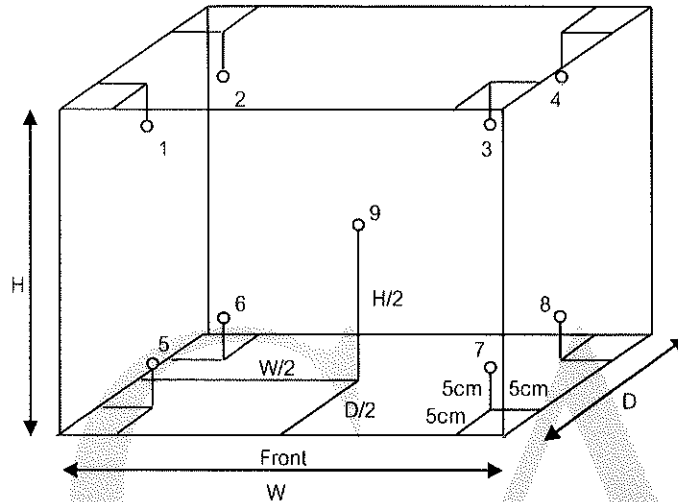

Inside of Chamber

W = 0.56 m

D = 0.40 m

H = 0.48 m

Capacity = 0.11 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
104.0	105.5	105.5	105.1	104.9	105.7	105.1	99.0	98.0	98.0	99.1	103.9	1.6
180.0	182.5	182.5	180.8	180.3	180.8	180.8	173.9	174.2	175.4	174.3	179.2	1.6

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
104.0	105.5	105.5	6.1	0.2	8.1
180.0	182.5	182.5	5.5	0.4	7.4

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 69-420034-3

Page : 1 of 2

Submitted by : HVE Co., Ltd.

603 Soi Jarunsanitwong 46 Jarunsanitwong Road, Bangyeekun, Bangplad, Bangkok 10700

Equipment : pH Meter with electrode

pH meter

Manufacturer : Hanna

Model : HI 3220

Range : N/A pH

Resolution : 0.01 pH

Serial No. : A0024904

ID No. : 083

Electrode

Model : HI 1131

Serial No. : 07702N

ID No. : 083

Environment : On site calibration was carried out at the Laboratory, HVE Co., Ltd.

Ambient Temperature : (23.5 to 26.5)°C

Relative Humidity : (35 to 45) %

Date of Received : 21 April 2026

Date of Calibration : 21 April 2026

Date of Issue : 22 April 2026

Calibrated by : Permpon Chanpu

Calibration Method : In-house method CAL-M4201 direct measurement by using standard voltage calibrator and using certified reference material (CRM)

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Multiproduct Calibrator

ID No.	Cert. No.	Due Date	Traceability
400005	SG-E-00231/68	20 Aug 2027	National Institute of Metrology Thailand (NIMT)

2. Standard Buffer Solution

pH	Cert. No.	Lot No.	Exp. Date	Traceability
4.007	61314276	1081108	28 Feb 2027	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
6.965	61318175	1081110	28 Feb 2026	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
10.010	61325043	1081109	28 Feb 2026	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025

Approved by :

(Permpon Chanpu)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 69-420034-3

Page : 2 of 2

Result of Calibration :

UUC Condition As-Received : Good

Function : Electrical measurement

pH meter

Performing standard curve by Multiproduct Calibrator at pH (4,7,10)

Adjustment Curve at nominal pH	Applied Voltage (mV)	Nominal Value (pH)	UUC Reading		Correction (mV)	Uncertainty (± mV)
			(pH)	(mV)		
4, 7, 10	177.4800	4	4.00	177.3	0.2	0.12
	0.0000	7	7.00	0.0	0.0	0.086
	-177.4800	10	10.00	-177.3	-0.2	0.12

Function : pH meter with electrode

Performing a three - buffer standard curve using buffer nominal pH (4,7,10)

Adjustment Curve at nominal pH	Standard Buffer (pH)	UUC Reading (pH)	Correction (pH)	Uncertainty (± pH)
4, 7, 10	4.008	4.01	0.00	0.0097
	6.963	7.00	-0.04	0.010
	10.011	10.01	0.00	0.014

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurment was based on a standard uncertainty multiplied by a coverage factor $k = 2$,
providing a level of confidence of approximately 95%

- o()o -



www.calibratech.co.th

Certificate of Calibration

Certificate No. : 69-400207-9

Page : 1 of 2

Submitted by : HVE Co., Ltd.

603 Soi Jarunsanitwong 46, Jarunsanitwong Road, Bangyeekun, Bangplad, Bangkok 10700

Equipment : Temperature controlled enclosure (Incubator)

Manufacturer : Lovibond

Model : TC 445 S

Range : N/A °C

Resolution : 0.1 °C

Serial No. : 0515/001080

ID No. : 112

Environment : On site calibration was carried out at the Laboratory, HVE Co., Ltd.

Ambient Temperature : (31.4 to 32.9) °C

Relative Humidity : (39 to 44) %

Line Voltage : (229.0 to 230.0) V

Date of Received : 21 April 2026

Date of Calibration : 21 April 2026

Date of Issue : 23 April 2026

Calibrated by : Aphisorn Worawasukullaya

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with RTD Probe

ID No.

Cert. No.

Due Date

Traceability

400046 & 400047

69-400018-2

24 Jul 2026

National Institute of Metrology Thailand (NIMT)

Approved by :

(Permpon Chanpu)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 69-400207-9


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

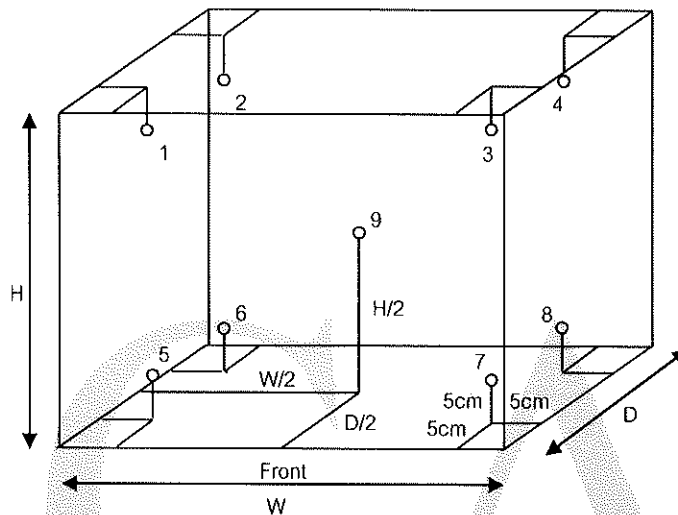

Inside of Chamber

W = 0.65 m

D = 0.60 m

H = 1.50 m

Capacity = 0.59 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
20.0	20.7	20.7	20.21	20.00	20.02	19.95	19.97	20.18	20.02	20.18	19.88	0.38

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
20.0	20.7	20.7	0.42	0.14	0.58

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 69-400207-8

Page : 1 of 2

Submitted by : HVE Co., Ltd.

603 Soi Jarunsanitwong 46, Jarunsanitwong Road, Bangyeekun, Bangplad, Bangkok 10700

Equipment : Temperature controlled enclosure (Incubator)

Manufacturer : Lovibond

Model : ET636-6

Range : N/A °C

Resolution : 0.1 °C

Serial No. : 6686 0707

ID No. : 011

Environment : On site calibration was carried out at the Laboratory, HVE Co., Ltd.

Ambient Temperature : (31.4 to 32.9) °C

Relative Humidity : (39 to 44) %

Line Voltage : (229.0 to 230.0) V

Date of Received : 21 April 2026

Date of Calibration : 21 April 2026

Date of Issue : 23 April 2026

Calibrated by : Aphisorn Worawasukullaya

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Digital Thermometer with RTD Probe

ID No.

Cert. No.

Due Date

Traceability

400046 & 400047

69-400018-2

24 Jul 2026

National Institute of Metrology Thailand (NIMT)

Approved by :



(Permpon Chanpu)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 69-400207-8


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

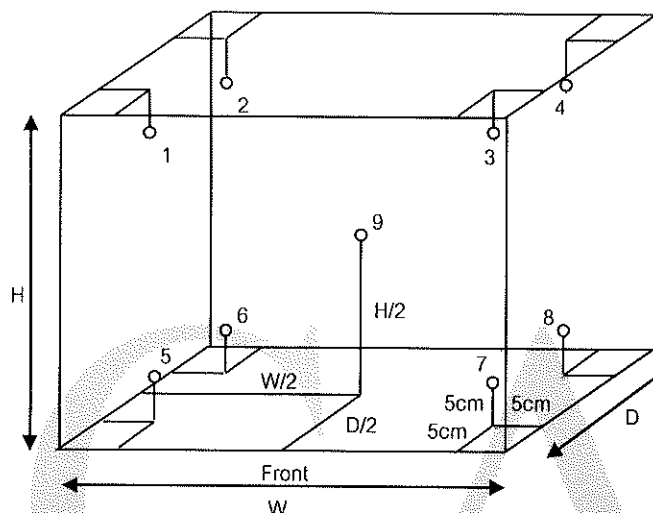

Inside of Chamber

W = 0.53 m

D = 0.43 m

H = 1.40 m

Capacity = 0.32 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
20.0	21.5	21.5	20.37	20.29	20.37	20.35	20.15	20.16	19.99	19.83	20.03	0.63

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
20.0	21.5	21.5	0.40	0.32	0.99

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 69-400213-1

Page : 1 of 2

Submitted by : HVE Co., Ltd.
603 Soi Jarunsanitwong 46 Jarunsanitwong Road,
Bangyeekun, Bangplad, Bangkok 10700

Equipment : Temperature Indicator with Thermistor Probe
Temperature Indicator

Manufacturer :	Hanna	Model :	HI 2211
Range :	N/A °C	Resolution :	0.1 °C
Serial No. :	08270179101	ID No. :	147
Thermistor probe			
Model :	HI7662	Sheath Material :	Stainless
Diameter :	3 mm.	Length :	110 mm.
Serial No. :	10161BEN	ID No. :	147

Environment : On site calibration was carried out at the Laboratory, HVE Co., Ltd.

Ambient Temperature : (23.5 to 26.5) °C

Relative Humidity : (35 to 45) %

Line Voltage : (229.0 to 230.0) VAC

Date of Received : 21 April 2026

Date of Calibration : 21 April 2026

Date of Issue : 22 April 2026

Calibrated by : Permpon Chanpu

Calibration Method : This instrument was calibrated by In-house method comparison technique CAL-M4003 by compared with PRT in the liquid bath at the constant controlled temperature.

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Platinum Resistance Thermometer (PRT)

ID No.	Cert. No.	Due Date	Traceability
400016	TT-1019-25	13 May 2027	National Institute of Metrology Thailand (NIMT)

2. Standard Digital Thermometer

ID No.	Cert. No.	Due Date	Traceability
400033	26E645	24 Feb 2028	National Institute of Metrology Thailand (NIMT)

Approved by :

(Permpon Chanpu)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 69-400213-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

Immersion Depth	Standard Reading	UUC Reading	Correction	Uncertainty
(mm.)	(°C)	(°C)	(°C)	(±°C)
110	25.002	25.0	0.0	0.19

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$,
providing a level of confidence of approximately 95%

- o()o -



Certificate of Calibration

Certificate No. : 69-400213-2

Page : 1 of 2

Submitted by : HVE Co., Ltd.
603 Soi Jarunsanitwong 46 Jarunsanitwong Road,
Bangyeekun, Bangplad, Bangkok 10700

Equipment : Temperature Indicator with Thermistor Probe
Temperature Indicator

Manufacturer :	Hanna	Model :	HI 2211
Range :	N/A °C	Resolution :	0.1 °C
Serial No. :	N/A	ID No. :	041
Thermistor probe			
Model :	N/A	Sheath Material :	Stainless
Diameter :	3 mm.	Length :	110 mm.
Serial No. :	N/A	ID No. :	041

Environment : On site calibration was carried out at the Laboratory, HVE Co., Ltd.

Ambient Temperature : (23.5 to 26.5) °C

Relative Humidity : (35 to 45) %

Line Voltage : (229.0 to 230.0) VAC

Date of Received : 21 April 2026

Date of Calibration : 21 April 2026

Date of Issue : 22 April 2026

Calibrated by : Permpon Chanpu

Calibration Method : This instrument was calibrated by In-house method comparison technique CAL-M4003 by compared with PRT in the liquid bath at the constant controlled temperature.

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Platinum Resistance Thermometer (PRT)

ID No.	Cert. No.	Due Date	Traceability
400016	TT-1019-25	13 May 2027	National Institute of Metrology Thailand (NIMT)

2. Standard Digital Thermometer

ID No.	Cert. No.	Due Date	Traceability
400033	26E645	24 Feb 2028	National Institute of Metrology Thailand (NIMT)

Approved by :

(Permpon Chanpu)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 69-400213-2

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

Immersion Depth (mm.)	Standard Reading (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (±°C)
110	25.003	24.8	0.2	0.19

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$,
providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 69-420034-1

Page : 1 of 2

Submitted by : HVE Co., Ltd.

603 Soi Jarunsanitwong 46 Jarunsanitwong Road, Bangyeekun, Bangplad, Bangkok 10700

Equipment : pH Meter with electrode

pH meter

Manufacturer : Hanna

Model : HI2211

Range : N/A pH

Resolution : 0.01 pH

Serial No. : 08270179101

ID No. : 147

Electrode

Model : HI 1131

Serial No. : 084809EN

ID No. : 147

Environment : On site calibration was carried out at the Laboratory, HVE Co., Ltd.

Ambient Temperature : (23.5 to 26.5)^o C

Relative Humidity : (35 to 45) %

Date of Received : 21 April 2026

Date of Calibration : 21 April 2026

Date of Issue : 22 April 2026

Calibrated by : Permpon Chanpu

Calibration Method : In-house method CAL-M4201 direct measurement by using standard voltage calibrator and using certified reference material (CRM)

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Multiproduct Calibrator

ID No.	Cert. No.	Due Date	Traceability
400005	SG-E-00231/68	20 Aug 2027	National Institute of Metrology Thailand (NIMT)

2. Certified Reference Material (CRM)

pH	Cert. No.	Lot No.	Exp. Date	Traceability
4.008	61340084	1209524	02 Apr 2028	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
6.963	61345799	1209526	02 Apr 2027	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
10.011	61340312	1209525	02 Apr 2027	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025

Approved by :

(Permpon Chanpu)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 69-420034-1

Page : 2 of 2

Result of Calibration :

UUC Condition As-Received : Good

Function : Electrical measurement

pH meter

Performing standard curve by Multiproduct Calibrator at pH (4,7) and (7,10)

Adjustment Curve at nominal pH	Applied Voltage (mV)	Nominal Value (pH)	UUC Reading		Correction (mV)	Uncertainty (± mV)
			(pH)	(mV)		
4, 7	177.4800	4	4.00	177.4	0.1	0.12
	0.0000	7	7.00	0.0	0.0	0.090
7,10	0.0000	7	7.00	0.0	0.0	0.090
	-177.4800	10	10.00	-177.4	-0.1	0.12

Function : pH meter with electrode

Performing a three - buffer standard curve using buffer nominal pH (4,7) and (7,10)

Adjustment Curve at nominal pH	Standard Buffer (pH)	UUC Reading (pH)	Correction (pH)	Uncertainty (± pH)
4, 7	4.008	4.01	0.00	0.0091
	6.963	7.01	-0.05	0.010
7, 10	6.963	7.01	-0.05	0.010
	10.011	10.01	0.00	0.014

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurment was based on a standard uncertainty multiplied by a coverage factor $k = 2$,
providing a level of confidence of approximately 95%

- 000 -



Certificate of Calibration

Certificate No. : 69-420034-2

Page : 1 of 2

Submitted by : HVE Co., Ltd.

603 Soi Jarunsanitwong 46 Jarunsanitwong Road, Bangyeekun, Bangplad, Bangkok 10700

Equipment : pH Meter with electrode

pH meter

Manufacturer : Hanna

Model : HI 2211

Range : N/A

pH

Resolution : 0.01 pH

Serial No. : N/A

ID No. : 041

Electrode

Model : HI 1131

Serial No. : 1025265N

ID No. : 041

Environment : On site calibration was carried out at the Laboratory, HVE Co., Ltd.

Ambient Temperature : (23.5 to 26.5)^o C

Relative Humidity : (35 to 45) %

Date of Received : 21 April 2026

Date of Calibration : 21 April 2026

Date of Issue : 22 April 2026

Calibrated by : Permpon Chanpu

Calibration Method : In-house method CAL-M4201 direct measurement by using standard voltage calibrator and using certified reference material (CRM)

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Multiproduct Calibrator

ID No.	Cert. No.	Due Date	Traceability
400005	SG-E-00231/68	20 Aug 2027	National Institute of Metrology Thailand (NIMT)

2. Certified Reference Material (CRM)

pH	Cert. No.	Lot No.	Exp. Date	Traceability
4.008	61340084	1209524	02 Apr 2028	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
6.963	61345799	1209526	02 Apr 2027	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
10.011	61340312	1209525	02 Apr 2027	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025

Approved by :

(Permpon Chanpu)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 69-420034-2

Page : 2 of 2

Result of Calibration :

UUC Condition As-Received : Good

Function : Electrical measurement

pH meter

Performing standard curve by Multiproduct Calibrator at pH (4,7) and (7,10)

Adjustment Curve at nominal pH	Applied Voltage (mV)	Nominal Value (pH)	UUC Reading		Correction (mV)	Uncertainty (± mV)
			(pH)	(mV)		
4, 7	177.4800	4	4.00	177.3	0.2	0.12
	0.0000	7	7.00	0.0	0.0	0.090
7,10	0.0000	7	7.00	0.0	0.0	0.090
	-177.4800	10	10.00	-177.4	-0.1	0.12

Function : pH meter with electrode

Performing a three - buffer standard curve using buffer nominal pH (4,7) and (7,10)

Adjustment Curve at nominal pH	Standard Buffer (pH)	UUC Reading (pH)	Correction (pH)	Uncertainty (± pH)
4, 7	4.008	4.01	0.00	0.0091
	6.963	7.01	-0.05	0.010
7, 10	6.963	7.01	-0.05	0.010
	10.011	10.01	0.00	0.014

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurment was based on a standard uncertainty multiplied by a coverage factor $k = 2$,
providing a level of confidence of approximately 95%

- o0o -



Certificate No. : C26040029

Page : 1 of 2

CERTIFICATE OF CALIBRATION

Equipment : COD Test Tube Heater

Meter Model : HI839800-02 **Serial No.** : H0175591

Tube Heater Capacity : 22 Vial Capacity **Resolution** : 0.1 °C

Temperature Range : (-10 to 160)°C **Temperature of Reaction** : 150°C

Manufacturer : Hanna Instruments **Made in** : Romania

Condition As-Received : Used Product **Reference** : RE260620

Customer name : HVE Co., Ltd.
603 Soi Charansanitwong 46, Charansanitwong Road,
Bangyikhan, Bang Phlat, Bangkok 10700

Received date : 1 April 2026

Calibrate date : 1 April 2026

Issue date : 3 April 2026

Ambient Temperature : (25 ± 2)°C

Relative Humidity : (50 ± 15)% RH

Calibrated Location : Hanna Instruments (Thailand) Ltd.

Calibrated by : Mr. Pichit Petthong**Approved by :**

(Mr. Anan Suwanchaisakul)

Authorized Signatory

3/3 10/4/26

This certificate was certified only for the instrument we calibrated. This result of calibration was found accurate on date and place of calibration only.

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Hanna Instrument (Thailand) Ltd.

Condition of this calibration result :

Reference standard instrument : This Certification is traceable to the SI Unit maintained through:

Instrument	Model	Serial No.	Certificate No.	Traceable
Digital Thermo-Hygrometer	HT-771SD	AI.07155	26H106	Technology Promotion Association (Thailand-Japan).
Data Acquisition Switch Unit	34970A	MY44065265	WK2507-171-1	WK Electric Co., Ltd.

Calibration Result :

Measurement Temperature Source Accuracy for COD Reactor.

Capacity	Nominal Value	Average Value	Error	Uncertainty ($\pm$)
22 Vials	150.0 °C	149.8 °C	-0.2 °C	0.54 °C

Unit : °C

(1A)	(2A)	(3A)	(4A)	(5A)
149.3	149.5	149.2	149.7	149.7
(1B)	(2B)	(3B)	(4B)	(5B)
149.4	150.2	150.1	150.2	150.0
(1C)	(2C)	(3C)	(4C)	(5C)
149.5	150.3	150.4	150.2	149.5
(1D)	(2D)	(3D)	(4D)	(5D)
149.7	N/A	N/A	N/A	149.8
(1E)	(2E)	(3E)	(4E)	(5E)
149.3	149.9	149.9	149.5	149.5

Figure: Shows the location of the temperature source.

Remark : N/A = not available. (Vial at 2D, 3D and 4D not ready to calibration)

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95%

** End of certificate **