



องค์การบริหารส่วนจังหวัดภูเก็ต

รายงานผลการปฏิบัติตามมาตรการป้องกันและแก้ไขผลกระทบสิ่งแวดล้อม
และมาตรการติดตามตรวจสอบผลกระทบสิ่งแวดล้อม

โครงการทำเทียบเรือท่องเที่ยวอ่าวฉลอง จังหวัดภูเก็ต

ฉบับประจำเดือนมกราคมถึงมิถุนายน พ.ศ. 2569

ภาคผนวก จ

ใบรับรองการสอบเทียบเครื่องมือ



right solutions.
right partner.

รายการเครื่องมือที่ใช้ในการวิเคราะห์ / ทดสอบ

Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Songkhla Lab	BOD	Incubator	SGK_CL0028	10-Jan-25	10-Jul-26	18
Songkhla Lab	BOD	DO/BOD Analyser	SGK_CL0101	24-Feb-26	24-Feb-27	12
Songkhla Lab	pH at 25 °C	pH meter	SGK_CL0030	31-Mar-26	1-Oct-27	18
Songkhla Lab	Oil & Grease	Electronic Top-Loading Balance	SGK_CL0045	15-Dec-25	15-Dec-26	12
Songkhla Lab	Oil & Grease	Oven	SGK_CL0024	31-Mar-26	1-Oct-27	18
Songkhla Lab	Oil & Grease	Water Bath	SGK_CL0035	16-Dec-25	16-Dec-26	12
Songkhla Lab	Total Suspended Solids	Electronic Top-Loading Balance	SGK_CL0045	15-Dec-25	15-Dec-26	12
Songkhla Lab	Total Suspended Solids	Oven	SGK_CL0024	31-Mar-26	1-Oct-27	18
Songkhla Lab	<i>Escherichia coli</i>	Autoclave	SGK_ML0002	15-Dec-25	15-Jun-27	18
Songkhla Lab	<i>Escherichia coli</i>	Incubator	SGK_ML0013	3-Jul-25	3-Jan-27	18
Songkhla Lab	<i>Escherichia coli</i>	pH meter	SGK_ML0045	17-Nov-25	17-Nov-26	12
Songkhla Lab	<i>Escherichia coli</i>	Water Bath	SGK_ML0021	16-Dec-25	16-Jun-27	18
Sea Water	Temperature	Digital Thermometer With Sensor	PHK_FS0001	10-Feb-25	10-Feb-26	12
Sea Water	pH at 25 °C	pH meter	SGK_CL0030	19-Oct-24	19-Apr-26	18
Sea Water	Salinity	Conductivity meter	SGK_CL0032	2-May-25	2-May-26	12
Sea Water	Total Suspended Solids	Electronic Top-Loading Balance	SGK_CL0045	15-Dec-25	15-Dec-26	12
Sea Water	Total Suspended Solids	Oven	SGK_CL0024	19-Oct-24	19-Apr-26	18
Sea Water	Turbidity	Turbidity Meter	SGK_FS0046	30-May-25	30-May-26	12
Sea Water	BOD	Incubator	SGK_CL0028	10-Jan-25	10-Jul-26	18
Sea Water	BOD	DO Meter With Sensor	SGK_CL0101	24-Feb-25	24-Feb-26	12
Sea Water	Dissolved Oxygen (on site)	DO Meter	PHK_FS0004	22-Sep-25	22-Sep-26	12
Sea Water	Oil & Grease	Electronic Top-Loading Balance	SGK_CL0045	15-Dec-25	15-Dec-26	12
Sea Water	Oil & Grease	Oven	SGK_CL0024	19-Oct-24	19-Apr-26	18
Sea Water	Oil & Grease	Water Bath	SGK_CL0035	16-Dec-25	16-Dec-26	12
Sea Water	Total Coliform	Autoclave	SGK_ML0001	15-Dec-25	15-Jun-27	18
Sea Water	Total Coliform	Incubator	SGK_ML0013	3-Jul-25	3-Jan-27	18
Sea Water	Total Coliform	pH Meter	SGK_ML0045	17-Nov-25	17-Nov-26	12
Sea Water	Total Coliform	Water Bath	SGK_ML0021	16-Dec-25	16-Jun-27	18

CALIBRATION CERTIFICATE

Issued Date : 13-Jan-2025

Certificate No. : 25TH0226

CSR No. : A101/05028

Page. : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Customer Laboratory

Instrument Name : Incubator

Manufacturer : Memmert

Model : ICP750

Serial No. : F816.0063

ID No. : SGK_CL0028

Resolution : 0.1 °C

Received Date : 10-Jan-2025

Calibrated Date : 10-Jan-2025

Ambient Temperature : (30 ± 10) °C

Relative Humidity : (50 ± 30) %

REVIEW BY	Ananta B.
APPROVED BY	Kanida H.
NEXT CAL. DATE	10/7/26

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.012 based on GLA - 20

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- TISTR : Thailand Institute of Scientific and Technological Research

Calibrated by : Ibrorhim Saleemin

Approved by :

Imron Rattanaylum / Technical Manager



The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data Acquisition/Switch Unit	34970A	MY58009813	PSL-T0707-1/67	22-May-2025


2. The results reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction

4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration : (✓) Without Adjustment () After Adjustment

1. Sensor Installation Diagram

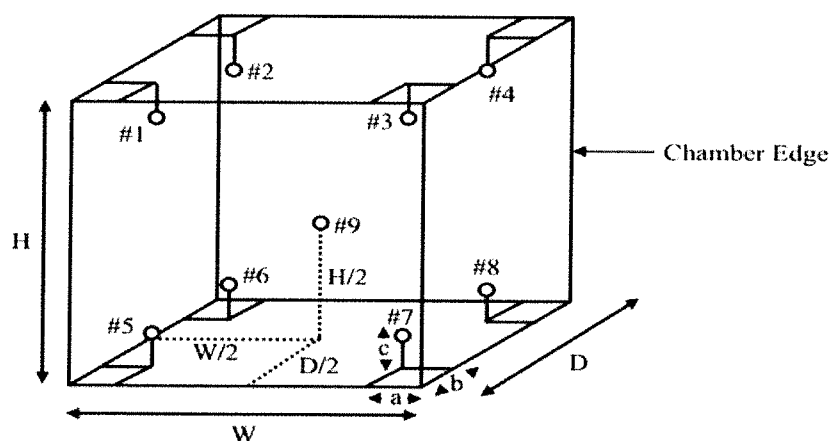

Sensor Installation Details

a = 5.0 cm
b = 5.0 cm
c = 5.0 cm

Dimension of the chamber

W = 104.0 cm
H = 120.0 cm
D = 60.0 cm



Certificate No. : 25TH0226

CSR No. : A101/05028

Page. : 3 of 3

Result of Calibration :

2. Temperature Measurement Accuracy Test

The measurement results of the Incubator and associates are reported in the manner as shown below

Cal point (°C)	Measured Standard Temperature At Spread Locations (°C)									Uncertainty (± °C)
	#1	#2	#3	#4	#5	#6	#7	#8	Ref. 9	
20	20.03	20.23	20.37	20.34	20.32	20.03	20.19	20.31	20.06	0.38

3. Performance Result

The performance of the Incubator are reported as shown below

Cal point (°C)	UUC Setting (°C)	UUC Reading (°C)	Temperature Stability (± °C)	Temperature Uniformity (°C)	Overall Variation (°C)
20	20.0	20.0	0.10	0.31	0.40

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

... End ...



Southern Calibration Service Co., Ltd.

669/35 Karnjanavanit Rd., Banpru, Hatyai, Songkla 90250 Thailand
Tel : 08 1599 0417 Fax : 0 7480 5133 Email : s.calibration@gmail.com www.scal-lab.com

CALIBRATION CERTIFICATE

Issued Date : 27-Feb-2026

Certificate No. : 26CH0116

CSR No. : A240/11995

Page. : 1 of 2

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : SCaL Laborator

Instrument Name : DO meter

Manufacturer : YSI

Model : 4010-1W

Serial No. : 24200618

ID No. : SGK_CL0101

Receipt Date : 20-Feb-2026

Calibration Date : 24-Feb-2026

Ambient Temperature : $(25 \pm 3) ^\circ\text{C}$

Relative Humidity : $(55 \pm 15) \%$

REVIEW BY	Chamkhan M.
APPROVED BY	Kanitta M.
NEXT CAL. DATE	24/2/27

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.062 based on direct measurement by using certified reference Material (CRM)

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- HANNA : Hanna Instruments.

Calibrated by : Alisara Ma

Approved by :



Sakeereen Heemhad / Laboratory Manager



The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Zero Oxygen Solution	HI7040L	C02374	S0032/21	12-Apr-2026

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction

4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration : (✓) Without Adjustment () After Adjustment

Sample Test Measurement

Serial Probe No. : 24F102419

Standard Buffer Solutions	UUC Reading	Correction	Uncertainty (±)
8.26 mg/L	8.26 mg/L	0.00 mg/L	0.16 mg/L

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

... End ...

CALIBRATION CERTIFICATE

Issued Date : 27-Feb-2026

Certificate No. : 26TH0817

CSR No. : A240/11995

Page. : 1 of 2

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : SCaL Laboratory

Instrument Name : DO Meter with probe

Manufacturer : YSI

Model : 4010-1W

Serial No. : 24200618

ID No. : SGK_CL0101

Resolution : 0.1 °C

Received Date : 20-Feb-2026

Calibrated Date : 24-Feb-2026

Ambient Temperature : (25 ± 3) °C

Relative Humidity : (55 ± 15) %

REVIEW BY	Chandran M.
APPROVED BY	Kamittha H.
NEXT CAL. DATE	24/2/27

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.011 by comparison technique with standard thermometer

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- Q Reborn : Quality Reborn Co.,Ltd.

Calibrated by : Ibrorhim Saleemin

Approved by :

Sakeereen Heemhad / Laboratory Manager

SCAL.FO.018/a010723



The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Digital Thermometer With Sensor (PRT)	1529	B4C223	QR25-2862	25-Sep-2026

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction

4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration : (☒) Without Adjustment (☐) After Adjustment

Sensor Type : RTD **Channel :** OUT **Serial Probe No. :** 24F102419

Length : 6.8 cm. **Diameter :** 0.2 cm. **Immersion :** 6.8 cm.

Cal Point (°C)	Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
20	20.007	20.2	-0.193	0.077

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

...End...

CALIBRATION CERTIFICATE

Issued Date : 3-Apr-2026

Certificate No. : 26CH0181

CSR No. : A247/12304

Page. : 1 of 2

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Customer Laboratory

Instrument Name : pH meter

Manufacturer : Mettler Toledo

Model : S220

Serial No. : B62531849

ID No. : SGK_CL0030

Electrode No. : 30014096

Received Date : 31-Mar-2026

Calibrated Date : 31-Mar-2026

Ambient Temperature : (25 ± 3) °C

Relative Humidity : (55 ± 15) %

REVIEW BY	Onanoknan M.
APPROVED BY	Kanitha H.
NEXT CAL. DATE	1/10/27

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.062 based on direct measurement with certified reference material (CRM)

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- CPAchem : CPAchem Ltd

- WK : WK Electric Co., Ltd.

Calibrated by : Alisara Ma

Approved by :

Alisara Ma / Supervisor Manager

SCAL.FO.018/a010723



The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Standard Solution	4.000	61333215	1176852	24-Dec-2026
Standard Solution	6.999	C03337	S11M004	24-Dec-2026
Standard Solution	10.01	61325050	1176853	24-Dec-2026
Temperature/Electrical Calibrator	MC2-MF	23642	WK2502-402-32	5-Feb-2027

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction

4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration :

1. Electrical Measurement

Applied Voltage (mV)	pH meter Reading		Correction (mV)	Uncertainty (± mV)	Coverage factor <i>k</i>
	(mV)	(pH)			
177.48	177.5	4.00	-0.02	0.17	2.00
0.00	0.1	7.00	-0.10	0.13	2.00
-177.48	-177.4	10.00	-0.08	0.17	2.00

2. Before Sample Test Measurement

Standard Buffer Solutions (pH)	pH meter Reading		Correction (pH)	Uncertainty (± pH)	Coverage factor <i>k</i>
	(pH)	(mV)			
4.008	4.01	159.8	-0.002	0.0092	2.00
6.999	7.07	-14.0	-0.071	0.020	2.00
10.011	10.11	-187.4	-0.099	0.042	2.00

3. After Sample Test Measurement (Performing buffer standard curve by using buffer nominal pH4, 7, 10)

Standard Buffer Solutions (pH)	pH meter Reading		Correction (pH)	Uncertainty (± pH)	Coverage factor <i>k</i>
	(pH)	(mV)			
4.008	4.00	169.8	0.008	0.0092	2.00
6.999	7.00	-4.2	-0.001	0.019	2.00
10.011	10.01	-177.6	0.001	0.042	2.00

4. Temperature Measurement

Cal Point (°C)	Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
25	25.024	25.1	-0.076	0.06

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95%

... End ...

CALIBRATION CERTIFICATE

Issued Date : 18-Dec-2025

Certificate No. : 25MA2641

CSR No. : A230/11462

Page. : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Chemical Laboratory

Instrument Name : Electronic Balance

Manufacturer : Sartorius

Model : MSE224S-100-DU

Serial No. : 34705158

ID No. : SGK_CL0045


Resolution : 0.0001 g

Received Date : 15-Dec-2025

Calibrated Date : 15-Dec-2025

Ambient Temperature : (30 ±10) °C

Relative Humidity : (50 ±20) %

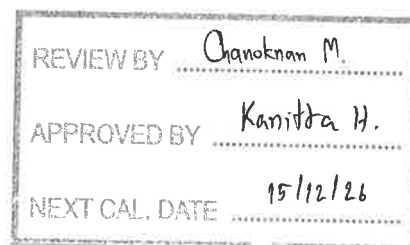

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.001 based on UKAS LAB 14 : 2022

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- SCaL : Sounthern Calibration Service Co., Ltd.,

Calibrated by : Hadbordee Dettawee

Approved by :

Imron Rattanyium / Technical Manager

SCAL.FO.018/a010723



The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Standard Weight Set	2mg to 1kg	11119514/01	25SWS001	2-Jul-2026

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction

4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration : ☒ Without Adjustment ☐ After Adjustment

1. Repeatability


Nominal Value (g)	Standard Deviation (g)
20	0.00000
200	0.00000

2. Off-center loading


A mass approximately 100g was placed on a pan and moved to various position .

The balance reading obtained are given in the table.


Position					Maximum Error from Center (g)
1	2	3	4	5	
100.0000	100.0001	100.0000	100.0001	100.0000	0.0001



Front



Front



Front

3. Effect of tare

Nominal Value (g)	Standard Value (g)	Balance Reading (g)	UUC Error (g)
20	19.9999	20.0000	0.0001
40	39.9999	40.0000	0.0001
60	60.0001	60.0000	-0.0001
80	80.0000	80.0001	0.0001
100	100.0000	100.0000	0.0000

Result of Calibration :. cont.

4. Departure from nominal value

Nominal Value (g)	Standard Value (g)	UUC Reading (g)	Correction (g)	Uncertainty ($\pm$ g)	Coverage Factor (k)
0	0.0000	0.0000	0.0000	0.00008	2.0
0.01	0.0100	0.0100	0.0000	0.00008	2.0
0.1	0.1000	0.1000	0.0000	0.00008	2.0
0.5	0.5000	0.5000	0.0000	0.00008	2.0
1	1.0000	1.0000	0.0000	0.00008	2.0
2	2.0000	2.0000	0.0000	0.00008	2.0
5	5.0000	5.0000	0.0000	0.00009	2.0
10	10.0000	10.0000	0.0000	0.00009	2.0
20	19.9999	20.0000	-0.0001	0.00009	2.0
40	39.9999	40.0000	-0.0001	0.00012	2.0
60	60.0001	60.0000	0.0001	0.00013	2.0
80	80.0000	80.0000	0.0000	0.00017	2.0
100	100.0000	100.0000	0.0000	0.00016	2.0
120	119.9999	120.0000	-0.0001	0.00024	2.0
140	139.9999	140.0001	-0.0002	0.00024	2.0
160	160.0001	160.0001	0.0000	0.00026	2.0
180	180.0000	180.0001	-0.0001	0.00030	2.0
200	199.9998	200.0000	-0.0002	0.00029	2.0

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95%

...End...

CALIBRATION CERTIFICATE

Issued Date : 3-Apr-2026

Certificate No. : 26TH1563

CSR No. : A247/12304

Page. : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Customer Laboratory

Instrument Name : Hot Air Oven

Manufacturer : Memmert

Model : UF110

Serial No. : B416.3387

ID No. : SGK_CL0024

Resolution : 0.1 °C

Received Date : 31-Mar-2026

Calibrated Date : 31-Mar-2026

Ambient Temperature : (30 ± 10) °C

Relative Humidity : (50 ± 30) %

REVIEW BY	Chanoknan M.
APPROVED BY	Kemitha H.
NEXT CAL. DATE	1/10/29

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.012 based on GLA - 20

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- Q Reborn : Quality Reborn Co.,Ltd.

Calibrated by : Ibrorhim Saleemin

Approved by :

Alisara Ma / Supervisor Manager

SCAL.FO.018/a010723



The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data Acquisition Switch Unit with Sensor	DAQ970A	MY58036254	QR25-2036	1-Jul-2026

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration


and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction

4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration : ☒ Without Adjustment ☐ After Adjustment

1. Sensor Installation Diagram

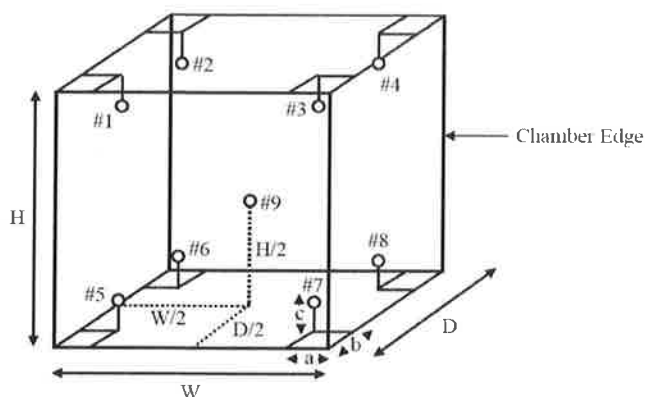

Sensor Installation Details

a = 5.0 cm
b = 5.0 cm
c = 5.0 cm

Dimension of the chamber

W = 40.0 cm
H = 40.0 cm
D = 33.0 cm

Result of Calibration :
2. Temperature Measurement Accuracy Test

The measurement results of the Hot Air Oven and associates are reported in the manner as shown below

Cal point (°C)	Measured Standard Temperature At Spread Locations (°C)									Uncertainty (±°C)
	#1	#2	#3	#4	#5	#6	#7	#8	Ref. 9	
40	40.52	40.44	40.53	40.53	40.53	40.46	40.59	40.54	40.44	0.38
70	70.81	70.87	71.26	70.87	70.18	70.96	70.24	70.47	70.09	0.44
103	103.36	103.37	103.49	103.42	102.74	103.02	103.47	102.92	102.96	0.39
104	104.06	104.09	104.50	104.14	103.50	104.15	104.47	103.84	103.84	0.42
105	105.20	105.22	105.54	105.41	105.36	105.22	105.31	105.01	105.09	0.38
180	180.78	180.86	180.98	180.98	179.46	179.33	179.32	179.41	179.42	0.55

3. Temperature Performance Result

The performance of the Hot Air Oven are reported as shown below

UUC Setting (°C)	UUC Reading (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
40.0	40.0	0.10	0.33	0.33
70.0	70.0	0.05	1.17	1.17
103.0	103.0	0.10	0.72	0.94
104.0	104.0	0.15	0.95	1.27
105.0	105.0	0.10	0.63	0.77
180.0	180.0	0.25	1.73	1.85

UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

... End ...

CALIBRATION CERTIFICATE

Issued Date : 19-Dec-2025

Certificate No. : 25TH5535

CSR No. : A230/11460

Page. : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Kamchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Chemical Laboratory

Instrument Name : Liquid Bath

Manufacturer : Memmert

Model : WNE29

Serial No. : L616.0538

ID No. : SGK_CL0035


Resolution : 0.1 °C

Received Date : 16-Dec-2025

Calibrated Date : 16-Dec-2025

Ambient Temperature : (30 ± 10) °C

Relative Humidity : (50 ± 30) %

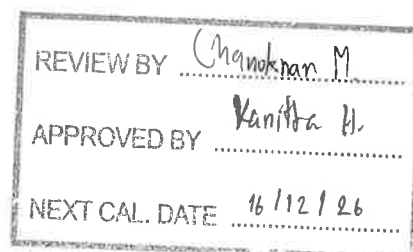

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.014 based on ASTM E 715 : 1980 (reapproved 2001)

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- Q Reborn : Quality Reborn Co.,Ltd.

Calibrated by : Ibrorhim Saleemin

Approved by :

[Signature]
Imron Rattanaylum / Technical Manager

SCAL.FO.018/a010723



The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Result of Calibration :

2. Temperature Measurement Accuracy Test

The measurement results of the Liquid Bath and associates are reported in the manner as shown below

Cal point (°C)	Measured Standard Temperature At Spread Locations (°C)					Uncertainty (± °C)
	#1	#2	#3	#4	Ref.5	
63	62.92	62.94	63.06	63.05	63.02	0.14

3. Performance Result

The performance of the Liquid Bath are reported as shown below

Cal point (°C)	UUC Setting (°C)	UUC Reading (°C)	Temperature Stability (± °C)	Temperature Uniformity (°C)	Overall Variation (°C)
63	63.5	63.5	0.05	0.17	0.20

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

... End ...

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data Acquisiton/Switch Unit	DAQ970A	MY58036254	QR25-2036	1-Jul-2026

2. The resultes reported in this certificate refer to the condition of the instrument on the date of calibration

and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction


4. Condition of Item : normal condition , no indication for any damage or mulfunction

Result of Calibration .:

(☒) Without Adjustment

(☐) After Adjustment

1. Sensor Installation Diagram

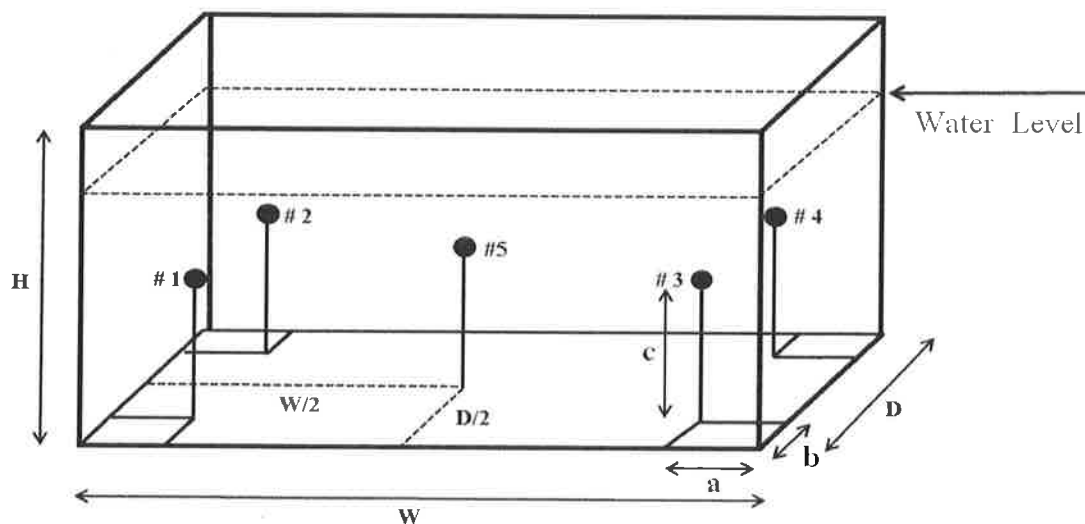

Sensor Installation Details

a = 5 cm
b = 5 cm
c = 5 cm

Dimension of the chamber

W = 45 cm
H = 30 cm
D = 35 cm

CALIBRATION CERTIFICATE

Issued Date : 18-Dec-2025

Certificate No. : 25TH5453

CSR No. : A230/11461

Page. : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Microbiological Laboratory

Instrument Name : Autoclave

Manufacturer : TOMY

Model : SX-700

Serial No. : 52134080

ID No. : SGK_ML0002

Resolution : 1 °C

Received Date : 15-Dec-2025

Calibrated Date : 15-Dec-2025

Ambient Temperature : (30 ± 10) °C

Relative Humidity : (50 ± 30) %

REVIEW BY	Nichapol R.
APPROVED BY	Kanitta H.
NEXT CAL DATE	15/6/27

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.013 based on BS 2646 : 1993 (part 5)

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- SCaL : Sounthern Calibration Service Co., Ltd.,

Calibrated by : Ibrorhim Saleemin

Approved by :

Imron Rattanaylum / Technical Manager

SCAL.FO.018/a010723



The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data logger With Sensor	GL240	C90432223	25SDAT005	16-Apr-2026


2. The results reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction

4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration : (✓) Without Adjustment () After Adjustment

1. Sensor Installation Diagram

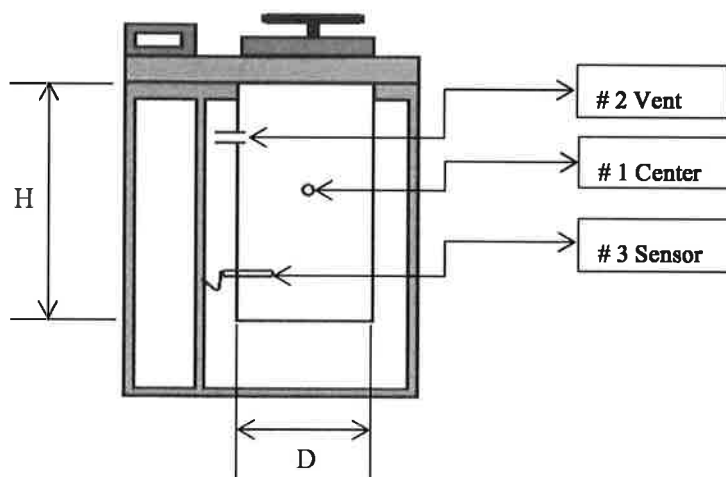

Chamber Diameter (D) : 30 cm

Chamber Height (H) : 70 cm

Result of Calibration .:

2. Temperature Measurement Accuracy Test

The measurement results of the Autoclave and associates are reported in the manner as shown below

Cal point (°C)	Measured Standard Temperature At Spread Locations (°C)			Pressure Reading	Uncertainty (± °C)
	Center #1	Vent #2	Sensor #3		
115	115.8	115.7	115.9	0.07 MPa	0.76
118	118.9	118.9	118.7	0.09 MPa	0.76
121	121.8	121.7	121.9	0.11 MPa	0.76

3. Performance Result

The performance of the Autoclave are reported as shown below

Cal point (°C)	UUC Setting (°C)	UUC Reading (°C)	Temperature Stability (± °C)	Temperature Uniformity (°C)	Overall Variation (°C)
115	115	115	0.40	0.69	0.71
118	118	118	0.50	0.82	1.00
121	121	121	0.30	0.50	0.89

- Operating Time = 900.02 sec

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

... End ...

CALIBRATION CERTIFICATE

Issued Date : 6-Jul-2025

Certificate No. : 25TH3013

CSR No. : A202/10083

Page. : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Customer Laboratory
Instrument Name : Incubator
Manufacturer : Memmert
Model : ICP750
Serial No. : F816.0061
ID No. : SGK_ML0013
Resolution : 0.1 °C
Received Date : 3-Jul-2025
Calibrated Date : 3-Jul-2025
Ambient Temperature : (30 ± 10) °C
Relative Humidity : (50 ± 30) %

REVIEW BY Nichapol R.
APPROVED BY Kanitta H.
NEXT CAL. DATE 3/09/27

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.012 based on GLA - 20

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- TISTR : Thailand Institute of Scientific and Technological Research

Calibrated by : Ibrorhim Saleemin

Approved by :

Imron Rattanaylum / Technical Manager

SCAL.FO.018/a010723



The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration


1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data Acquisition/Switch Unit	34970A	MY58009813	PSL-T0707-2/67	22-Nov-2025

- The results reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.
- This certificate is not certified any commercial transaction
- Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration .: ☒ Without Adjustment ☐ After Adjustment

1. Sensor Installation Diagram

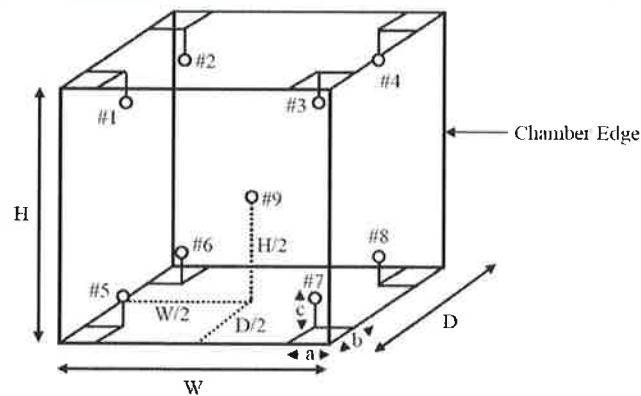

Sensor Installation Details

a = 5.0 cm
 b = 5.0 cm
 c = 5.0 cm

Dimension of the chamber

W = 104.0 cm
 H = 120.0 cm
 D = 60.0 cm

Result of Calibration :

2. Temperature Measurement Accuracy Test

The measurement results of the Incubator and associates are reported in the manner as shown below

Cal point (°C)	Measured Standard Temperature At Spread Locations (°C)									Uncertainty (±°C)
	#1	#2	#3	#4	#5	#6	#7	#8	Ref. 9	
35	34.97	35.05	35.09	35.04	35.02	34.91	34.99	35.01	34.98	0.38

3. Temperature Performance Result

The performance of the Incubator are reported as shown below

UUC Setting (°C)	UUC Reading (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
35.0	35.0	0.10	0.24	0.31

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$,
 providing a level of confidence of approximately 95%

... End ...

CALIBRATION CERTIFICATE

Issued Date : 20-Nov-2025

Certificate No. : 25CH0552

CSR No. : A222/11083

Page. : 1 of 2

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Customer Laboratory
Instrument Name : pH meter
Manufacturer : Mettler Toledo
Model : Seven Direct SD20
Serial No. : C431515609
ID No. : SGK_ML0045
Electrode No. : 4253467
Received Date : 17-Nov-2025
Calibrated Date : 17-Nov-2025
Ambient Temperature : $(25 \pm 3) ^\circ\text{C}$
Relative Humidity : $(55 \pm 15) \%$

REVIEW BY Wichapol R.
APPROVED BY Karnittha H.
NEXT CAL. DATE 17/11/26

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.008 based on direct measurement by using certified reference Material (CRM)

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- CPAchem : CPAchem Ltd
- WK : WK Electric Co., Ltd.

Calibrated by : Alisara Ma

Approved by :

Imron Rattanaaylum / Technical Manager

SCAL.FO.018/a010723



The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Standard Solution	4.000	61333215	1116005	15-Jun-2026
Standard Solution	7.000	61328150	1112965	8-Jun-2026
Standard Solution	10.01	61325050	1112967	8-Jun-2026
Temperature/Electrical Calibrator	MC2-TE	14987	WK2506-402-27	4-Jun-2027

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction

4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration :

1. Electrical Measurement

Applied Voltage (mV)	pH meter Reading		Correction (mV)	Uncertainty (± mV)
	(mV)	(pH)		
177.48	177.5	4.00	-0.02	0.17
0.00	0.0	7.00	0.00	0.13
-177.48	-177.6	10.00	0.12	0.17

2. Before Sample Test Measurement

Standard Buffer Solutions (pH)	pH meter Reading		Correction (pH)	Uncertainty (± pH)
	(pH)	(mV)		
4.008	3.93	181.9	0.078	0.0092
6.988	6.87	7.9	0.118	0.019
10.011	9.71	-160.5	0.301	0.042

3. After Sample Test Measurement

Standard Buffer Solutions (pH)	pH meter Reading		Correction (pH)	Uncertainty (± pH)
	(pH)	(mV)		
4.008	4.01	183.1	-0.002	0.0092
6.988	7.00	8.0	-0.012	0.019
10.011	10.03	-161.8	-0.019	0.042

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

... End ...

CALIBRATION CERTIFICATE

Issued Date : 19-Dec-2025

Certificate No. : 25TH5450

CSR No. : A230/11461

Page. : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Microbiological Laboratory

Instrument Name : Liquid Bath

Manufacturer : Memmert

Model : WPE45

Serial No. : L716.0558

ID No. : SGK_ML0021

Resolution : 0.1 °C

Received Date : 16-Dec-2025

Calibrated Date : 16-Dec-2025

Ambient Temperature : (30 ± 10) °C

Relative Humidity : (50 ± 30) %



Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.014 based on ASTM E 715 : 1980
(reapproved 2001)

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement
according to the International System of Unit (SI) through :

- Q Reborn : Quality Reborn Co.,Ltd.

Calibrated by : Ibrorhim Saleemin

Approved by :

Imron Rattanaylum / Technical Manager

SCAL.FO.018/a010723



The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data Acquisiton/Switch Unit	DAQ970A	MY58036254	QR25-2036	1-Jul-2026

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration

and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction


4. Condition of Item : normal condition , no indication for any damage or mulfunction

Result of Calibration :

(☒) Without Adjustment

(☐) After Adjustment

1. Sensor Installation Diagram

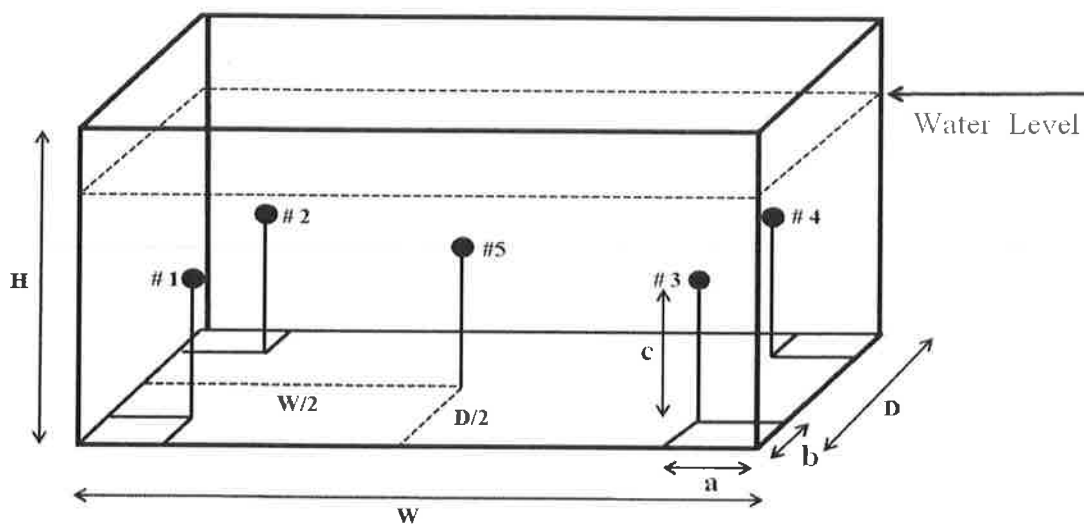

Sensor Installation Details

a = 5 cm
b = 5 cm
c = 5 cm

Dimension of the chamber

W = 45 cm
H = 30 cm
D = 35 cm

Result of Calibration :

2. Temperature Measurement Accuracy Test

The measurement results of the Liquid Bath and associates are reported in the manner as shown below

Cal point (°C)	Measured Standard Temperature At Spread Locations (°C)					Uncertainty (± °C)
	#1	#2	#3	#4	Ref.5	
44.5	44.48	44.45	44.49	44.47	44.48	0.14

3. Performance Result

The performance of the Liquid Bath are reported as shown below

Cal point (°C)	UUC Setting (°C)	UUC Reading (°C)	Temperature Stability (± °C)	Temperature Uniformity (°C)	Overall Variation (°C)
44.5	44.5	44.5	0.10	0.25	0.36

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

... End ...



Certificate of Calibration

Certificate No. : 25T204

Page : 1 of 2

Equipment : Digital Thermometer With Sensor

Manufacturer: Testo

Model : 106

Serial No.: 51164834/812

ID No.: PHK_FS0001

Condition As-Received: Used Item

Received Date: 07 February 2025

Calibration Date: 10 February 2025
to 13 February 2025

Reference: 2502-0246DSC

Ambient Temperature: (25 ± 3) °C

Relative Humidity: (50 ± 20) %

This certificate may not be reproduced other than in full,
except with the prior written approval of the head of
Corporate Services 3: Equipment Calibration and Testing Services.

Submitted by: ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand

Procedure used: Calibration were conducted using in-house calibration procedure CP-T01 according to comparison with
Industrial Platinum Resistance Thermometer (IPRT) into liquid bath temperature controller.
The temperature scale used was based on ITS-90.

Condition of this result of calibration

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Black Stack Thermometer	1560	8C454	24I598	06 Jun 2025
2) PRT Scanner Module	2562	A01303	24I598	06 Jun 2025
3) Industrial Platinum Resistance Thermometer	5627	739434	24I598	06 Jun 2025

2.The certificate is valid only to the item calibrated on date and place of calibration.

3.This Certification is traceable to the International System of Unit maintained through:
-Technology Promotion Association (Thailand-Japan), NSC-ONSC Accredited No. Calibration 0008

REVIEW BY Chayathorn P.

APPROVED BY Narakorn P.

NEXT CAL DATE 10/02/26

Calibrated by : Theerapong Ameen
Issue Date : 14 February 2025

Approved Signatory :

☐ Phalinee Prabpaipal

☐ Chatchawan Khunpiluek

☒ Wanlop Larpkern



Cert. No.: 25T204

Page.: 2 of 2

Result of Calibration:-

Without Adjustment

Function:

Temperature measurement

Dimension of probe : Diameter 3 mm., Length 55 mm. Sheath material : Stainless Steel

Immersion	Standard	UUC*		Uncertainty
<u>Depth</u>	<u>Temperature</u>	<u>Reading</u>	<u>Error</u>	<u>of Measurement</u>
(mm.)	(°C)	(°C)	(°C)	(±°C)
50	25.0033	24.9	-0.1033	0.12
50	45.0096	44.9	-0.1096	0.12

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

-o0o-





Southern Calibration Service Co., Ltd.

669/35 Karnjanavanit Rd., Banpru, Hatyai, Songkla 90250 Thailand
Tel : 08 1599 0417 Fax : 0 7480 5133 Email : s.calibration@gmail.com www.scal-lab.com



CALIBRATION CERTIFICATE

Issued Date : 22-Oct-2024

Certificate No. : 24CH0526

CSR No. : A163/08133

Page. : 1 of 2

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Chemical Laboratory
Instrument Name : pH meter
Manufacturer : Mettler Toledo
Model : S220
Serial No. : B625631849
ID No. : SGK_CL0030
Electrode No. : 2281592
Received Date : 19-Oct-2024
Calibrated Date : 19-Oct-2024
Ambient Temperature : $(25 \pm 3) ^\circ\text{C}$
Relative Humidity : $(55 \pm 15) \%$

REVIEW BY Ananta B.
APPROVED BY Kanitta H.
NEXT CAL. DATE 19/4/26

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.008 based on direct measurement by using certified reference Material (CRM)

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- CPAchem : CPAchem Ltd
- WK : WK Electric Co., Ltd.
- SCaL : Sounthern Calibration Service Co., Ltd.,

Calibrated by : Alisara Ma

Approved by :

Imron Rattanaylum / Technical Manager



The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Standard Solution	4.000	61310674	1042701	26-Oct-2025
Standard Solution	7.000	61314184	1042700	26-Oct-2025
Standard Solution	10.01	61313804	1042702	26-Oct-2025
Temperature/Electrical Calibrator	MC2-TE	14987	WK2106-299-223	31-May-2025
Digital Thermometer With Sensor	DP-77	1.360896	24SDTH005	7-Aug-2025

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration

and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction

4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration :

1. Electrical Measurement

Applied Voltage (mV)	pH meter Reading		Correction (mV)	Uncertainty (± mV)
	(mV)	(pH)		
177.48	177.5	4.00	-0.02	0.17
0.00	0.0	7.00	0.00	0.13
-177.48	-177.5	10.00	0.02	0.17

2. Before Sample Test Measurement

Standard Buffer Solutions (pH)	pH meter Reading		Correction (pH)	Uncertainty (± pH)
	(pH)	(mV)		
4.007	3.99	178.1	0.017	0.0092
6.976	7.02	1.7	-0.044	0.019
10.009	9.96	-169.6	0.049	0.038

3. After Sample Test Measurement

Standard Buffer Solutions (pH)	pH meter Reading		Correction (pH)	Uncertainty (± pH)
	(pH)	(mV)		
4.007	3.99	177.7	0.017	0.0092
6.976	7.01	3.7	-0.034	0.019
10.009	10.00	-169.0	0.009	0.038

4. Temperature Measurement

Cal Point (°C)	Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
25	25.021	25.0	0.02	0.060

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

... End ...



Certificate of Calibration

Cert.No.: 25CH504

Page.: 1 of 2

Equipment :	Conductivity Meter
Manufacturer :	Mettler Toledo
Model :	SevenCompact S230
Serial No. :	B608134488
ID No. :	SGK_CL0032
Condition As-Received:	Used Item
Received Date :	25 April 2025
Calibration Date :	02 May 2025
Reference :	2504-0711DSC-1
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. Songkhla Branch. 114/1 Moo 8 Karnchanawanich Rd., T.Ban Phru, A.Hat Yai, Songkhla 90250 Thailand
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure:	In -house method : - CP-CH6 by direct measurement with reference material (RM)
Calibrated by :	Warakorn Lerngagtrakul  Approved Signatory
Approved by :	
(✓) Chakrit Waewwanjua	
() Ponpan Paipim	
() Saithip Meangmai	
Issue Date :	05 May 2025

REVIEW BY *Chanoknan M.*

APPROVED BY *Kanitta H*

NEXT CAL DATE..... 02/05/26

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Calibration and Testing Equipment Services.



Cert.No.: 25CH504

Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instrument :-

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due date</u>
1) Thermometer	1963878	130RC095	24I995	09 Sep 2025

- This Certification is traceable to SI Throught Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials :-

- Conductivity calibration solution, Thermo Scientific (Traceable to NIST)

<u>Conductivity Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
84 $\mu\text{S/cm}$	Thermo Scientific	424/02	18 Oct 2025
1413 $\mu\text{S/cm}$	Thermo Scientific	174/03	26 Apr 2027
12.88 mS/cm	Thermo Scientific	422/01	21 Oct 2025

- Control Conductivity calibration solution temperature by Water bath (25 ± 0.1) $^{\circ}\text{C}$

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration results

Function : Conductivity Measurement

(*) Without Adjustment

Conductivity Electrode Serial No.: 5820120321

Standard Conductivity Solution	UUC* Reading	Uncertainty of Measurement ($\pm$)	Coverage factor k
84 $\mu\text{S/cm}$	84.3 $\mu\text{S/cm}$	4.3 $\mu\text{S/cm}$	2.00
1413 $\mu\text{S/cm}$	1426 $\mu\text{S/cm}$	15 $\mu\text{S/cm}$	2.00
12.88 mS/cm	12.88 mS/cm	0.14 mS/cm	2.00

Remark : - UUC* = Unit Under Calibration

- Cell constant = 0.574487 cm^{-1}

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-



Certificate of Calibration

Cert.No.: 25CH505

Page.: 1 of 2

Equipment : Conductivity Meter
Manufacturer : Mettler Toledo
Model : SevenCompact S230
Serial No. : B608134488
ID No. : SGK_CL0032
Condition As-Received: Used Item
Received Date : 25 April 2025
Calibration Date : 02 May 2025
Reference : 2504-0711DSC-2
Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd. Songkhla Branch.
114/1 Moo 8 Karnchanawanich Rd., T.Ban Phru,
A.Hat Yai, Songkhla 90250 Thailand
Ambient Temperature : $(25 \pm 2.5) ^\circ\text{C}$
Relative Humidity : $(50 \pm 15) \%$
Calibration Procedure: In -house method :
- CP-CH6 by direct measurement
with reference material (RM)
Calibrated by : Warakorn Lernagtrakul

Approved by : _____
Approved Signatory
(☒) Chakrit Waewwanjua
(☐) Ponpan Paipim
(☐) Saithip Meangmai
Issue Date : 05 May 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Calibration and Testing Equipment Services.



Cert.No.: 25CH505

Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instrument :-

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due date</u>
1) Thermometer	9549224	130RC003	25I440	16 Apr 2026

- This Certification is traceable to SI Through Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials :-

- Conductivity calibration solution, Thermo Scientific (Traceable to NIST)

<u>Conductivity Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
84 $\mu\text{S/cm}$	Thermo Scientific	424/02	18 Oct 2025

- Control Conductivity calibration solution temperature by Water bath (25 ± 0.1) $^{\circ}\text{C}$

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration results

Function : Conductivity Measurement

(*) After Adjustment at 84 $\mu\text{S/cm}$

Conductivity Electrode Serial No.: 5816340156

Standard Conductivity Solution	Before Adjustment UUC* Reading	After Adjustment UUC* Reading	Uncertainty of Measurement ($\pm$)	Coverage factor k
84 $\mu\text{S/cm}$	81.1 $\mu\text{S/cm}$	84.1 $\mu\text{S/cm}$	4.3 $\mu\text{S/cm}$	2.00

Remark : - UUC* = Unit Under Calibration

- Cell constant = 0.103477 cm^{-1}

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-



CALIBRATION CERTIFICATE

Issued Date : 22-Oct-2024

Certificate No. : 24TH4295

CSR No. : A163/08133

Page. : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Chemical Laboratory
Instrument Name : Hot Air Oven
Manufacturer : Memmert
Model : UF110
Serial No. : B416.3387
ID No. : SGK_CL0024
Resolution : 0.1 °C
Received Date : 19-Oct-2024
Calibrated Date : 19-Oct-2024
Ambient Temperature : (30 ± 10) °C
Relative Humidity : (50 ± 30) %

REVIEW BY	Ananta B.....
APPROVED BY	Karnita H.....
NEXT CAL. DATE	19/04/2026

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.012 based on GLA - 20

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- TISTR : Thailand Institute of Scientific and Technological Research

Calibrated by : Ibrrorhim Saleemin

Approved by :

Imron Rattanaylum / Technical Manager



The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data Acquisition/Switch Unit	34970A	MY58009813	PSL-T0707-1/67	22-May-2025


2. The results reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction

4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration .: (✓) Without Adjustment () After Adjustment

1. Sensor Installation Diagram

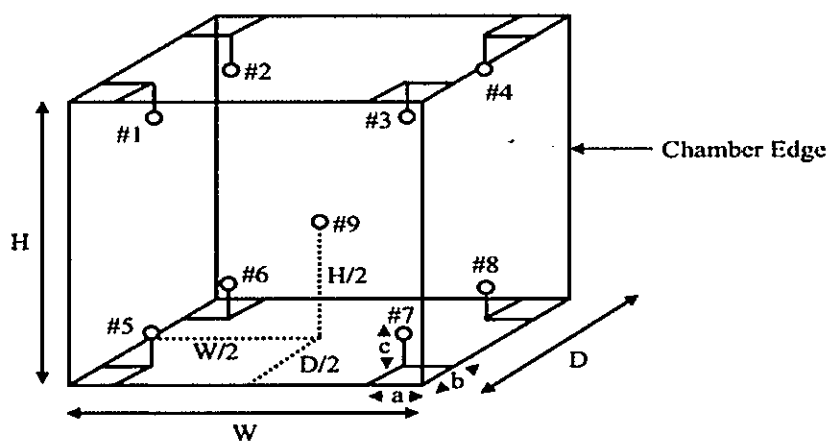

Sensor Installation Details

a = 5.0 cm
 b = 5.0 cm
 c = 5.0 cm

Dimension of the chamber

W = 55.0 cm
 H = 48.0 cm
 D = 40.0 cm

Result of Calibration :

2. Temperature Measurement Accuracy Test

The measurement results of the Hot Air Oven and associates are reported in the manner as shown below

Cal point (°C)	Measured Standard Temperature At Spread Locations (°C)									Uncertainty (±°C)
	#1	#2	#3	#4	#5	#6	#7	#8	Ref. 9	
40	40.36	40.40	40.51	40.43	40.05	40.24	40.09	40.14	39.75	0.38
70	70.27	70.30	70.45	70.24	70.24	70.43	70.29	70.30	69.95	0.36
103	102.94	102.90	103.55	102.96	103.22	103.14	103.10	103.01	102.88	0.36
104	104.15	103.99	104.27	104.06	104.09	104.23	104.26	104.15	103.90	0.36
105	105.04	104.90	105.05	104.87	104.91	104.80	104.82	104.98	104.70	0.36
180	179.19	178.93	179.82	179.10	179.27	179.68	179.12	179.73	179.12	0.41

3. Performance Result

The performance of the Hot Air Oven are reported as shown below

Cal point (°C)	UUC Setting (°C)	UUC Reading (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
40	40.0	40.0	0.20	0.84	0.84
70	70.0	70.0	0.10	0.59	0.59
103	103.0	103.0	0.20	0.73	0.74
104	104.0	104.0	0.20	0.47	0.56
105	105.0	105.0	0.20	0.44	0.46
180	180.0	180.0	0.50	0.86	1.11

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

... End ...



REVIEW BY	<u>Somsak J.</u>
APPROVED BY	<u>Kanitta H.</u>
NEXT CAL. DATE	<u>30 May 26</u>

Internal Calibration

Equipment :	<u>Turbidity Meter</u>	Manufacture :	<u>HACH</u>
ID No. :	<u>SGK_FS0046</u>	Model :	<u>2100Q/QIS</u>
Calibrate Date :	<u>May 30, 2025</u>	Serial No. :	<u>19030C074494</u>

Calibration Point	1st (NTU)	2nd (NTU)	3rd (NTU)	AVG (NTU)	Specifications	Evaluate
Standard 20 NTU	20.1	20.0	20.0	20.0	19 to 21 NTU	Pass
Standard 100 NTU	100.0	101.0	101.0	100.7	95 to 105 NTU	Pass
Standard 800 NTU	799.0	799.0	800.0	799.3	760 to 840 NTU	Pass

Calibrated by Somsak J.
(Scientist 2)

Approved by : Kanitta H.
(Section Head)



Be Right™

An ISO 9001 Certified Company

Loveland, CO 80539

(970) 669-3050

Certificate of Analysis

This is a Component of 2659405-TH / LOT A4243

PRODUCT: STABLCAL® FORMAZIN STANDARD 100 NTU

PRODUCT NUMBER: 2684901

LOT NUMBER: A4242

MANUFACTURE DATE: 08/28/2024

DATE OF ANALYSIS: 09/03/2024

TEST	SPECIFICATIONS	RESULTS
Turbidity	95 to 105 NTU	103.0 NTU

The expiration date is Nov 2025

Formazin and StablCal® solutions provided by Hach are not NIST traceable because the NIST does not carry turbidity standards. However, the use of Formazin and StablCal® as used in Hach method 8195 are accepted by the EPA as a primary standard to be used in the calibration of turbidity instruments.

Certified by: *Scott Als*

Analytical Services Chemist



An ISO 9001 Certified Company

Loveland, CO 80539

(970) 669-3050

Certificate of Analysis

This is a Component of 2659405-TH / LOT A4243

PRODUCT: STABLCAL® FORMAZIN STANDARD 800 NTU

PRODUCT NUMBER: 2660501

LOT NUMBER: A4233

MANUFACTURE DATE: 08/26/2024

DATE OF ANALYSIS: 08/30/2024

TEST	SPECIFICATIONS	RESULTS
Turbidity	760 to 840 NTU	814.3 NTU

The expiration date is Nov 2025

Formazin and StablCal® solutions provided by Hach are not NIST traceable because the NIST does not carry turbidity standards. However, the use of Formazin and StablCal® as used in Hach method 8195 are accepted by the EPA as a primary standard to be used in the calibration of turbidity instruments.

Certified by: *Scott Als*

Analytical Services Chemist



An ISO 9001 Certified Company

Loveland, CO 80539
(970) 669-3050

Certificate of Analysis

This is a Component of 2659405-TH / LOT A4243

PRODUCT: STABLCAL® FORMAZIN STANDARD 20 NTU

PRODUCT NUMBER: 2684801

LOT NUMBER: A4240

MANUFACTURE DATE: 08/28/2024

DATE OF ANALYSIS: 09/03/2024

TEST	SPECIFICATIONS	RESULTS
Turbidity	19 to 21 NTU	20.4 NTU

The expiration date is Nov 2025

Formazin and StablCal® solutions provided by Hach are not NIST traceable because the NIST does not carry turbidity standards. However, the use of Formazin and StablCal® as used in Hach method 8195 are accepted by the EPA as a primary standard to be used in the calibration of turbidity instruments.

Certified by: *Scott Als*

Analytical Services Chemist



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert. No.: 25LM26

Page.: 1 of 2

Equipment : DO Meter with Sensor

Manufacturer : YSI

Model : 4010-1W

Serial No. : 24200618

ID No. : -

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd. Songkhla Branch.
114/1 Moo 8 Karnchanawanich Rd.,
T.Ban Phru, A.Hat Yai,
Songkhla 90250 Thailand

Location : TPA Calibration Laboratory

Received Order : 21 February 2025

Calibrated Date : 24 February 2025

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

AC Line Voltage : (220 ± 22) V

Calibrated by : Warakorn Lerngagtrakul

Approved by :

Kunchit

Approved Signatory

() Chakrit Waewwanjua

() Suwit Imjai

(✓) Kunchit Promprat

Issue Date : 25 February 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : DO Meter with Sensor
Condition As-Received : Used Item
Reference : 2502-0715WC-2

Cert. No.: 25LM26

Page.: 2 of 2

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1) Digital Thermometer	2188080	2411022	TPA	17 Sep 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N.: 24F102419

<u>Calibration Point</u> (°C)	<u>Immersion Depth</u> (mm)	<u>Standard Temperature</u> (°C)	<u>UUC* Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (± °C)	<u>Coverage Factor</u> <i>k</i>
20.0	60	20.003	20.0	-0.003	0.16	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES

534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000 FAX. 0-2719-9484

Certificate of Testing

Cert.No.: 25TW32

Page.: 1 of 2

Equipment :	DO Meter
Manufacturer :	YSI
Model :	4010-1W
Serial No. :	24200618
ID No. :	-
Received Date :	21 February 2025
Test Date :	24 February 2025
Reference :	2502-0715WC-1
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. Songkhla Branch. 114/1 Moo 8 Karnchanawanich Rd., T.Ban Phru, A.Hat Yai, Songkhla 90250 Thailand
Laboratory Condition :	Temperature (25 ± 5) °C Humidity (50 ± 20) %
Test Procedure :	In - house method : CP-CH9 by Comparison Technique with Azide Modification Method
Tested by :	Walalak Sirithean
Approved by :	 Approved Signatory
() Chakrit Waewwanjua () Ponpan Paipim (✓) Saithip Meangmai	
Issue Date :	25 February 2025

REVIEW BY	Ananta B.....
APPROVED BY	Kanytha H.....
NEXT CAL. DATE	24/2/26.....



Cert.No.: 25TW32

Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

<u>Instruments</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1. Burette	-	130BU10	23CG1172	22 Mar 2025
2. Balance	14233821	110RC001	24MM131	04 July 2025

2. Standard Material :-

<u>Material</u>	<u>Manufacturer</u>	<u>Lot.No.</u>	<u>Assay</u>
Sodium Thiosulfate 5-Hydrate AR	KEMAUS	2203162447	99.6%

Result : Dissolved Oxygen Meter Adjustment With Air 100 %

Dissolved Oxygen Probe No.: 24F102419

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.22	8.28	0.0089

This report was certified only for the instrument we tested. It is allowable to use for study
Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced
other in full, without written approval of the laboratory

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)

CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES

534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000 FAX. 0-2719-9484

Certificate of Testing

Cert.No.: 25TW191

Page.: 1 of 2

Equipment : DO Meter
Manufacturer : Mettler Toledo
Model : Seven2GO
Serial No. : B905192342
ID No. : PHK_FS0004
Received Date : 19 September 2025
Test Date : 22 September 2025
Reference : 2509-0712DSC-1
Submitted by :

ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand

Laboratory Condition : Temperature (25 ± 5) °C
Humidity (50 ± 20) %
Test Procedure : In - house method : CP-CH9
by Comparison Technique with Azide Modification Method

Tested by : Walalak Sirithean

Approved by :

Saithip

Approved Signatory

- () Chakrit Waewwanjua
() Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 24 September 2025

REVIEW BY	<i>Chayathron P.</i>
APPROVED BY	<i>Narakorn P.</i>
NEXT CAL DATE	22/09/26



Cert.No.: 25TW191

Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

This measurement result is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

<u>Instruments</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1. Burette	130BU10	25CG1126	18 Mar 2027
2. Balance	110RC001	25MM316	02 July 2026

2. Standard Material :-

<u>Material</u>	<u>Manufacturer</u>	<u>Lot.No.</u>	<u>Assay</u>
Sodium Thiosulfate 5-Hydrate AR	KEMAUS	2203162447	99.6%

Result : **Dissolved Oxygen Meter Adjustment With Air 100 %**

Dissolved Oxygen Probe No.: 629461

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.20	8.27	0.0045

This report was certified only for the instrument we tested. It is allowable to use for study
Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced
other in full, without written approval of the laboratory

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert. No.: 25LM149

Page.: 1 of 2

Equipment : DO Meter with Sensor

Manufacturer : Mettler Toledo

Model : Seven2GO

Serial No. : B905192342

ID No. : PHK_FS0004

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand

Location : TPA On Site Calibration Laboratory

Received Order : 19 September 2025

Calibrated Date : 28 September 2025

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

AC Line Voltage : (220 ± 22) V

Calibrated by : Khit Ruttanaprapachai

Approved by :

Approved Signatory

- () Chakrit Waewwanjua
(✓) Suwit Imjai
() Kunchit Promprat

Issue Date : 30 September 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : DO Meter with Sensor
Condition As-Received : Used Item
Reference : 2509-0712DSC-2

Cert. No.: 25LM149

Page.: 2 of 2

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1) Digital Thermometer	2188080	25I953	TPA	05 Sep 2026

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This measurement result is traceable to the International System of Unit maintained through :

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N.: 629461

<u>Calibration Point</u> (°C)	<u>Immersion Depth</u> (mm)	<u>Standard Temperature</u> (°C)	<u>UUC* Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (± °C)	<u>Coverage Factor</u> <i>k</i>
20.0	80	20.004	20.2	0.196	0.16	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

CALIBRATION CERTIFICATE

Issued Date : 18-Dec-2025

Certificate No. : 25TH5452

CSR No. : A230/11461

Page. : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Microbiological Laboratory

Instrument Name : Autoclave

Manufacturer : TOMY

Model : SX-700

Serial No. : 52134079

ID No. : SGK_ML0001


Resolution : 1 °C

Received Date : 15-Dec-2025

Calibrated Date : 15-Dec-2025

Ambient Temperature : (30 ± 10) °C

Relative Humidity : (50 ± 30) %

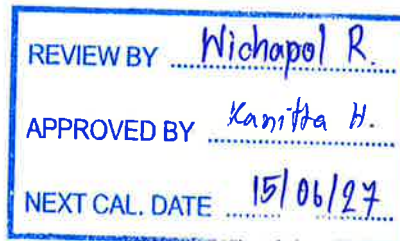**Calibration Method Used :**

This instrument was calibrated using the Calibration In - house method : SCAL.WI.013 based on BS 2646 : 1993 (part 5)

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- SCaL : Sounthern Calibration Service Co., Ltd.,

Calibrated by : Ibrorhim Saleemin

Approved by :

Imron Rattanaylum / Technical Manager

SCAL.FO.018/a010723



The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data logger With Sensor	GL240	C90432223	25SDAT005	16-Apr-2026

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction


4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration :

(☒) Without Adjustment

(☐) After Adjustment

1. Sensor Installation Diagram

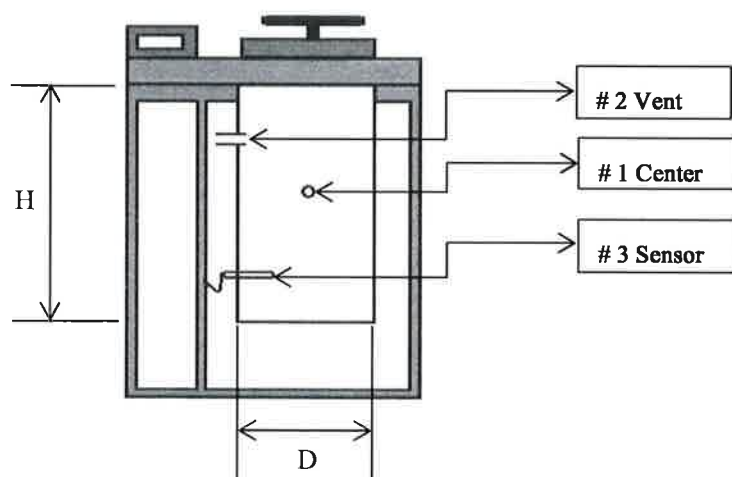

Chamber Diameter (D) : 30 cm

Chamber Height (H) : 70 cm

Result of Calibration :

2. Temperature Measurement Accuracy Test

The measurement results of the Autoclave and associates are reported in the manner as shown below

Cal point (°C)	Measured Standard Temperature At Spread Locations (°C)			Pressure Reading	Uncertainty (± °C)
	Center #1	Vent #2	Sensor #3		
121	121.9	121.8	121.9	0.11 MPa	0.76

3. Performance Result

The performance of the Autoclave are reported as shown below

Cal point (°C)	UUC Setting (°C)	UUC Reading (°C)	Temperature Stability (± °C)	Temperature Uniformity (°C)	Overall Variation (°C)
121	121	121	0.50	0.69	0.83

- Operating Time = 1800.06 sec

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$,
providing a level of confidence of approximately 95%

... End ...