

ภาคผนวกที่ 4

สรุปเอกสารสอบเทียบอุปกรณ์เครื่องมือ

Certificate No.: CP20260086EA

Operation No.: CP2026020048

Certificate of Calibration

Equipment: Sound Level Meter

Manufacturer: ACO

Model/Type: 6236 (Meter), 7052NR (Microphone), - (Preamplifier)

Serial No.: 222187 (Meter), 84151 (Microphone), - (Preamplifier)

ID No.: NS-03-017

Customer: C.E.M. Technology (Thailand) Co.,Ltd.

Address: 31/8 Moo 13 T.Rai Khung, A.Sam Phran,
Nakorn Phatom 73210

Received Date: 9 February 2026

Calibrated Date: 10 - 11 March 2026

Issued Date: 18 March 2026

Calibrated by: Ms. Juntaporn Kunhakom

Approved by: _____

(Mr. Sittichai Swaksuriyawong)

Group Manager

This report was prepared electronically using applicable electronic signature. Printing or copy of file are considered as a copy of the document.

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor (k) providing a level of confidence of approximately 95%. This certificate may not be reproduced other than in full except with the prior written approval of the Electrical and Electronics Institute, Foundation for Industrial Development.

Certificate No.: CP20260086EA

Calibration Report

Equipment: Sound Level Meter
Manufacturer: ACO
Model/Type: 6236 (Meter), 7052NR (Microphone), - (Preamplifier)
Serial No.: 222187 (Meter), 84151 (Microphone), - (Preamplifier)
ID No.: NS-03-017
Ambient Temperature: (23 ± 2) °C
Relative Humidity: (50 ± 15) %
Pressure: (101.3 ± 1.5) kPa

Method of Calibration :-
IEC61672-3:2013.

Condition of this result of calibration

1. Reference standards instrument :-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Standard microphone	4180	2661000	AA-1011-25	24 June 2026
2) Arbitrary Function Generator	AFG2021	C010063	CK20250037EA	25 June 2026
3) Programmable Attenuator	PA5	2913	EF-0026-25	9 June 2026
4) 6.5 Digit precision multimeter	8846A	9609027	CB20250141EA	20 August 2026
5) Pressure humidity and Temperature Transmitter	PTU301	F0640002	CL1-P250028 CD20250221EA	23 March 2026 8 August 2026
6) Pressure humidity and Temperature Transmitter	PTU301	F0640003	CL1-P250034 CD20250096EA	10 April 2026 29 March 2026
7) Performance Audio Analyzer	U8903B	MY56510003	CB20260043EA CK20250065EA	10 March 2027 23 September 2026

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certification is traceable to the international system of unit maintained at :-

Reference standards instrument for Acoustic function

- National Institute of Metrology (Thailand).; ILAC Policy, Item 2 (1) No.ILAC-P10:07/2020.

Reference standards instrument for Electrical function

- National Institute of Metrology (Thailand)

- Electrical and Electronics Institute; NSC Accredited Calibration No.0119

- IRPC Metrology Center, IRPC Public Co., Ltd.; NSC Accredited Calibration No.0204.

Result of Calibration:-

Function : 1. Indication at the calibration check frequency

Reference Acoustic Signal (dB)	Measured value (dB)	Deviation (dB)	Acceptance limits (dB)
-	-	-	-

Certificate No.: CP20260086EA

Calibration Report

Function : 2. Self-generated Noise

2.1 Microphone Installed

Measured value (dB)
20.7

2.2 Microphone replaced by the electrical input signal device

Frequency Weighting	Measured value (dB)
A-weighting	18.6
C-weighting	26.8
Z-weighting	33.9

Function : 3. Acoustical signal tests of frequency weightings (Without Windscreen)

Meter free-field acoustic response at a level of 84 dB.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
125	-0.4	-0.6	-0.5	±1.5
1000	0.0	0.0	0.0	±1.0
8000	0.2	0.3	0.5	±5.0

Function : 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
63	0.0	-0.2	0.0	±2.0
125	0.0	-0.2	0.0	±1.5
250	0.0	-0.1	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	-0.1	0.0	0.0	±2.0
4000	-0.4	-0.3	-0.1	±3.0
8000	-0.4	-0.4	-0.1	±5.0

Certificate No.: CP20260086EA

Calibration Report

Function : 5. Frequency and time weighting at 1 kHz

5.1 Frequency weighting at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
C-weighting	94.0	0.0	±0.2
A-weighting	94.0	0.0	±0.2
Z-weighting	93.9	-0.1	±0.2

5.2 Time weighting at 1 kHz

Time Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	94.0	0.0	±0.1
Slow	94.0	0.0	±0.1
LAeq	94.0	0.0	±0.1

Function : 6. Long-Term Stability

Long-term stability over 30 minutes, with steady 1 kHz signal at reference level.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
30	94.0	94.0	0.0	±0.3

Function : 7. Level Linearity on the reference level range

7.1 Level Linearity on the reference level range, Upper

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±1.1
99.0	99.0	0.0	±1.1
104.0	104.0	0.0	±1.1
109.0	109.0	0.0	±1.1
114.0	114.0	0.0	±1.1
119.0	119.0	0.0	±1.1
120.0	120.1	0.1	±1.1
121.0	121.1	0.1	±1.1

Certificate No.: CP20260086EA

Calibration Report

7.2 Level Linearity on the reference level range, Lower

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±1.1
89.0	89.0	0.0	±1.1
84.0	84.0	0.0	±1.1
79.0	79.0	0.0	±1.1
74.0	74.0	0.0	±1.1
69.0	69.0	0.0	±1.1
64.0	64.0	0.0	±1.1
59.0	59.0	0.0	±1.1
54.0	54.0	0.0	±1.1
49.0	49.0	0.0	±1.1
44.0	44.0	0.0	±1.1
39.0	38.8	-0.2	±1.1
34.0	33.8	-0.2	±1.1
33.0	32.9	-0.1	±1.1
32.0	31.9	-0.1	±1.1
31.0	31.0	0.0	±1.1
30.0	30.2	0.2	±1.1

Function : 8. Level Linearity including level range control

8.1. Level Linearity Including the Level Range (Reference Signal)

Range	Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
20-100	94.0	93.9	-0.1	±1.1
20-110	94.0	94.0	0.0	±1.1
30-120	94.0	94.0	0.0	±1.1
40-130	94.0	94.0	0.0	±1.1

8.2. Level Linearity Including the Level range (5dB Above Under-range)

Range	Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
20-80	25.0	25.2	0.2	±1.1
20-90	25.0	25.3	0.3	±1.1
20-100	25.0	25.6	0.6	±1.1
20-110	25.0	25.7	0.7	±1.1
30-120	35.0	35.0	0.0	±1.1
40-130	45.0	45.2	0.2	±1.1

Certificate No.: CP20260086EA

Calibration Report

Function : 9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	200	116.0	0.0	±1.0
	2	98.9	-0.1	+1.0 ; -2.5
	0.25	89.8	-0.2	+1.5 ; -5.0
Slow	200	109.5	-0.1	±1.0
	2	90.0	0.0	+1.0 ; -5.0
LAE	200	109.9	-0.1	±1.0
	2	89.9	-0.1	+1.0 ; -2.5
	0.25	80.8	-0.2	+1.5 ; -5.0

Function : 10. Peak C sound level

Number of cycles in test signal	Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Complete cycle	125.4	125.7	0.3	±3.0
Positive half cycle	124.4	124.2	-0.2	±2.0
Negative half cycle	124.4	124.2	-0.2	±2.0

Function : 11. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limits (dB)
Positive one-half cycle	Negative one-half cycle		
-	-	-	-

Function : 12. High-Level Stability

High-level stability over 5 minutes, with steady 1 kHz signal, 1 dB below upper boundary.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
5	129.0	129.0	0.0	±0.3

Certificate No.: CP20260086EA

Calibration Report

Uncertainty of measurement

Function	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1) Indication at the calibration check frequency	0.30	Not applicable
2) Self-generated Noise	0.10	Not applicable
3) Acoustical signal tests of frequency weightings - Free-field sound pressure response level	0.30	0.60 (10Hz to 4kHz) 0.70 (>4kHz to 10kHz)
4) Electrical signal tests of frequency weightings	0.20	0.20
5) Frequency and time weighting at 1 kHz	0.20	0.20
6) Long-Term Stability	0.10	0.10
7) Level Linearity on the reference level range	0.30	0.30
8) Level Linearity including level range control	0.30	0.30
9) Tone burst response	0.20	0.30
10) Peak C sound level	0.20	0.35
11) Overload indication	0.24	0.25
12) High-Level Stability	0.10	0.10

Remarks:

1. Indication at the calibration check frequency can not measured because customer does not provide a sound calibrator.
2. Overload indication can not measured because sound level meter can not set to Reference value of the standard calibration.
3. The acceptance limit is for the deviated value.
4. Acceptance limits was IEC61672-3:2013 Class 2.
5. The coverage factor $k = 2.00$

- - End of Report - -

Certificate No.: CP20250263EA

Operation No.: CP2025090257

Certificate of Calibration

Equipment: Sound Level Meter

Manufacturer: BSWA TECH

Model/Type: BSWA 309 (Meter), MP309 (Microphone), MA231T (Preamplifier)

Serial No.: 590101 (Meter), 395615 (Microphone), 590614 (Preamplifier)

ID No.: NS-04-002

Customer: C.E.M. Technology (Thailand) Co.,Ltd.

Address: 31/8 Moo 13, T.Rai Khing, A.Sam Phran,
Nakhon Pathom 73210

Received Date: 10 September 2025

Calibrated Date: 23 - 25 September 2025

Issued Date: 26 September 2025

Calibrated by: Ms. Juntaporn Kunhakom

Approved by: _____

(Mr. Sittichai Swaksuriyawong)

Group Manager

This report was prepared electronically using applicable electronic signature. Printing or copy of file are considered as a copy of the document.

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor (k) providing a level of confidence of approximately 95%. This certificate may not be reproduced other than in full except with the prior written approval of the Electrical and Electronics Institute, Foundation for Industrial Development.

Certificate No.: CP20250263EA

Calibration Report

Equipment: Sound Level Meter
 Manufacturer: BSWA TECH
 Model/Type: BSWA 309 (Meter), MP309 (Microphone), MA231T (Preamplifier)
 Serial No.: 590101 (Meter), 395615 (Microphone), 590614 (Preamplifier)
 ID No.: NS-04-002
 Ambient Temperature: (23 ± 2) °C
 Relative Humidity: (50 ± 15) %
 Pressure: (101.3 ± 1.5) kPa
 Method of Calibration :-
 IEC 61672-3:2013.

Condition of this result of calibration

1. Reference standards instrument :-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Standard microphone	4180	2661000	AA-1011-25	24 June 2026
2) Arbitrary Function Generator	AFG2021	C010063	CK20250037EA	25 June 2026
3) Programmable Attenuator	PA5	2755	EF-0035-24	28 October 2025
4) 6.5 Digit precision multimeter	8846A	9610014	CB20240215EA	26 November 2025
5) Pressure humidity and Temperature Transmitter	PTU301	F0640003	CL1-P250034 CD20250096EA	10 April 2026 29 March 2026
6) Performance Audio Analyzer	U8903B	MY56510003	CB20250030EA CK20250065EA	13 February 2026 23 September 2026

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certification is traceable to the international system of unit maintained at :-

Reference standards instrument for Acoustic function

- National Institute of Metrology (Thailand); ILAC Policy, Item 2 (1) No.ILAC-P10:07/2020.

Reference standards instrument for Electrical function

- National Institute of Metrology (Thailand)

- Electrical and Electronics Institute; NSC Accredited Calibration No.0119

- IRPC Metrology Center, IRPC Public Co., Ltd.; NSC Accredited Calibration No.0204.

Result of Calibration:-

Function : 1. Indication at the calibration check frequency

Reference Acoustic Signal (dB)	Measured value (dB)	Deviation (dB)	Acceptance limits (dB)
-	-	-	-

Certificate No.: CP20250263EA

Calibration Report

Function : 2. Self-generated Noise

2.1 Microphone Installed

Measured value (dB)
18.6

2.2 Microphone replaced by the electrical input signal device

Frequency Weighting	Measured value (dB)
A-weighting	12.0
C-weighting	15.0
Z-weighting	22.8

Function : 3. Acoustical signal tests of frequency weightings (Without Windscreen)

Meter free-field acoustic response at a level of 84 dB.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
125	0.4	0.3	0.3	±1.5
1000	-0.1	-0.1	-0.1	±1.0
8000	-1.0	-1.1	-0.6	±5.0

Function : 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
63	0.0	-0.1	0.0	±2.0
125	0.0	-0.1	0.0	±1.5
250	0.0	-0.1	0.0	±1.5
500	0.0	-0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.1	±2.0
4000	-0.1	-0.1	-0.1	±3.0
8000	-0.6	-0.5	0.0	±5.0

Function : 5. Frequency and time weighting at 1 kHz

5.1 Frequency weighting at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
C-weighting	94.0	0.0	±0.2
A-weighting	94.0	0.0	±0.2
Z-weighting	94.0	0.0	±0.2

Certificate No.: CP20250263EA

Calibration Report

5.2 Time weighting at 1 kHz

Time Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	94.0	0.0	±0.1
Slow	94.0	0.0	±0.1
LAeq	94.0	0.0	±0.1

Function : 6. Long-Term Stability

Long-term stability over 30 minutes, with steady 1 kHz signal at reference level.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
30	94.0	94.0	0.0	±0.3

Function : 7. Level Linearity on the reference level range

7.1 Level Linearity on the reference level range, Upper

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±1.1
99.0	99.0	0.0	±1.1
104.0	104.0	0.0	±1.1
109.0	109.0	0.0	±1.1
114.0	114.0	0.0	±1.1
119.0	119.0	0.0	±1.1
124.0	124.0	0.0	±1.1
129.0	129.0	0.0	±1.1
134.0	134.0	0.0	±1.1

7.2 Level Linearity on the reference level range, Lower

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±1.1
89.0	89.0	0.0	±1.1
84.0	84.0	0.0	±1.1
79.0	79.0	0.0	±1.1
74.0	74.0	0.0	±1.1
69.0	69.0	0.0	±1.1
64.0	64.0	0.0	±1.1
59.0	59.0	0.0	±1.1
54.0	54.0	0.0	±1.1
49.0	49.0	0.0	±1.1
44.0	44.0	0.0	±1.1
39.0	39.0	0.0	±1.1
34.0	34.0	0.0	±1.1

Certificate No.: CP20250263EA

Calibration Report

7.2 Level Linearity on the reference level range, Lower (Cont.)

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
29.0	29.1	0.1	±1.1
28.0	28.1	0.1	±1.1
27.0	27.1	0.1	±1.1
26.0	26.2	0.2	±1.1
25.0	25.2	0.2	±1.1
24.0	24.3	0.3	±1.1
23.0	23.4	0.4	±1.1
22.0	22.5	0.5	±1.1
21.0	21.6	0.6	±1.1
20.0	20.8	0.8	±1.1
19.0	20.0	1.0	±1.1

Function : 8. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	200	131.0	0.0	±1.0
	2	114.0	0.0	+1.0 ; -2.5
	0.25	104.9	-0.1	+1.5 ; -5.0
Slow	200	124.6	0.0	±1.0
	2	105.0	0.0	+1.0 ; -5.0
	200	125.0	0.0	±1.0
SEL	2	105.0	0.0	+1.0 ; -2.5
	0.25	95.9	-0.1	+1.5 ; -5.0

Function : 9. Peak C sound level

Number of cycles in test signal	Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Complete cycle	130.4	130.0	-0.4	±3.0
Positive half cycle	129.4	129.2	-0.2	±2.0
Negative half cycle	129.4	129.2	-0.2	±2.0

Function : 10. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limits (dB)
Positive one-half cycle	Negative one-half cycle		
137.5	137.4	-0.1	±1.5

Certificate No.: CP20250263EA

Calibration Report

Function : 11. High-Level Stability

High-level stability over 5 minutes, with steady 1 kHz signal, 1 dB below upper boundary.


Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
5	134.0	134.0	0.0	±0.3

Uncertainty of measurement

Function	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1) Indication at the calibration check frequency	0.30	Not applicable
2) Self-generated Noise	0.10	Not applicable
3) Acoustical signal tests of frequency weightings - Free-field sound pressure response level	0.30	0.60 (10Hz to 4kHz) 0.70 (>4kHz to 10kHz)
4) Electrical signal tests of frequency weightings	0.20	0.20
5) Frequency and time weighting at 1 kHz	0.20	0.20
6) Long-Term Stability	0.10	0.10
7) Level Linearity on the reference level range	0.30	0.30
8) Tone burst response	0.20	0.30
9) Peak C sound level	0.20	0.35
10) Overload indication	0.24	0.25
11) High-Level Stability	0.10	0.10

- Remarks:
1. Indication at the calibration check frequency can not measured because customer does not provide a sound calibrator.
 2. The acceptance limit is for the deviated value.
 3. Acceptance limits was IEC61672-3:2013 Class 2.
 4. The coverage factor $k = 2.00$

- - End of Report - -

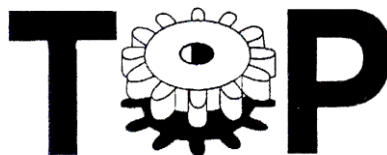

Trade & Engineering
TSP High Volume Sampler
TE-5000 TSP Sampler Verification

Site Information

Location: -	Site ID: -	Date: 10 Oct 25
Sampler: TE-5000 TSP	Serial No: 3271	Tech: Tong.P

Site Conditions

Barometric Pressure (in Hg): 28.30	Corrected Pressure (mm Hg): 718.8
Temperature (deg F): 75.7	Temperature (deg K): 297.4
Average Press. (in Hg): 27.50	Corrected Average (mm Hg): 698.5
Average Temp (Deg F): 75.1	Average Temp: (Deg K): 297.1

Calibration Orifice

Make: Tisch	Qstd Slope: 1.57894
Model: TE-5028A	Qstd Intercept: -0.01520
Serial#: 1179	Calibration Due Date 22 October 2025

Calibration Information

Plate or Test #	H2O (in)	Qstd (m3/min)	I (chart)	IC (corrected)	Linear Regression
1	8.35	1.791	60.5	58.89	Slope: 36.3288
2	6.60	1.594	55.7	54.22	Intercept: -5.0713
3	5.30	1.429	48.5	47.21	Corr. Coeff: 0.9949
4	4.60	1.332	44.3	43.12	
5	4.25	1.112	35.8	34.85	

of Observations: 5

Calculations


$Qstd = 1/m[\text{Sqrt}(H2O(Pa/Pstd)(Tstd/Ta)) - b]$
 $IC = I[\text{Sqrt}(Pa/Pstd)(Tstd/Ta)]$

Qstd = standard flow rate
IC = corrected chart response
I = actual chart response
m = calibrator Qstd slope
b = calibrator Qstd intercept
Ta = actual temperature during calibration (deg K)
Pa = actual pressure during calibration (mm Hg)
Tstd = 298 deg K
Pstd = 760 mm Hg
For subsequent calculation of sampler flow:
 $1/m((I)[\text{Sqrt}(298/Tav)(Pav/760)] - b)$

m = sampler slope
b = sampler intercept
I = chart response
Tav = daily average temperature
Pav = daily average pressure

Enter Average I (chart):	49.0
Average Flow Calculation m3/min	1.433574848
Average Flow Calculation in cfm	50.62058014
Sample Time (Hrs):	24.0
Total flow in 24 hours m3/min	2064.347782
Total flow in 24 hours cfm	72893.6354

NOTE: Ensure calibration orifice has been certified within 12 months of use

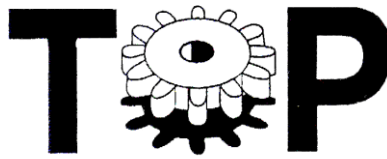

Trade & Engineering
TSP High Volume Sampler
TE-5000 TSP Sampler Verification

Site Information

Location: -	Site ID: -	Date: 7 Oct 25
Sampler: TE-5000 TSP	Serial No: 3275	Tech: Tong.P

Site Conditions

Barometric Pressure (in Hg): 28.25	Corrected Pressure (mm Hg): 717.6
Temperature (deg F): 75.3	Temperature (deg K): 297.2
Average Press. (in Hg): 27.36	Corrected Average (mm Hg): 694.9
Average Temp (Deg F): 75.2	Average Temp (Deg K): 297.2

Calibration Orifice

Make: Tisch	Qstd Slope: 1.57894
Model: TE-5028A	Qstd Intercept: -0.01520
Serial#: 1179	Calibration Due Date 22 October 2025

Calibration Information

Plate or Test #	H2O (in)	Qstd (m3/min)	I (chart)	IC (corrected)	Linear Regression
1	8.40	1.796	61.8	60.13	Slope: 36.2678
2	6.50	1.581	57.7	56.14	Intercept: -3.7246
3	5.45	1.448	50.3	48.94	Corr. Coeff: 0.9849
4	4.70	1.346	44.7	43.49	
5	4.15	1.112	37.8	36.78	
					# of Observations: 5

Calculations

$Qstd = 1/m[\text{Sqrt}(H2O(Pa/Pstd)(Tstd/Ta)) - b]$
 $IC = I[\text{Sqrt}(Pa/Pstd)(Tstd/Ta)]$

Qstd = standard flow rate
IC = corrected chart response
I = actual chart response
m = calibrator Qstd slope
b = calibrator Qstd intercept
Ta = actual temperature during calibration (deg K)
Pa = actual pressure during calibration (mm Hg)
Tstd = 298 deg K
Pstd = 760 mm Hg
For subsequent calculation of sampler flow:
 $1/m((I)[\text{Sqrt}(298/Tav)(Pav/760)] - b)$

m = sampler slope
b = sampler intercept
I = chart response
Tav = daily average temperature
Pav = daily average pressure

Enter Average I (chart):	50.5
Average Flow Calculation m3/min	1.435033909
Average Flow Calculation in cfm	50.67210063
Sample Time (Hrs):	24.0
Total flow in 24 hours m3/min	2066.448828
Total flow in 24 hours cfm	72967.82491

NOTE: Ensure calibration orifice has been certified within 12 months of use

Certificate of Analyzer Performance Testing

Calibrated Date : 18-Aug-25

Certificate No. : 0825-003

Page : 1/1

Analyzer Instruments

Analyzer Type : SO2 Analyzer
Model : 43C

Manufacturer : Thermo Environmental
Serial No. : 43C-70852-367

Environmental

Temperature : 26.4 °C
Humidity : 45.2 %RH

Calibration System

Calibrator Units

Gas Calibration : Thermo Environmental
Model : 146C
Serial No. : 514811458

Zero Air Generator : API
Model : 701
Serial No. : 179


Standard Gas

NO Conc. : 2 ppm
SO2 Conc. : 2 ppm
CO Conc. : 50 ppm

Cylinder No. : 307199
Expire Date : 10-Oct-25

Calibration Check

Gas	Zero			Span		
	Reading Value (ppm)	Expected Value (ppm)	Drift (%)	Reading Value (ppm)	Expected Value (ppm)	Drift (%)
Before						
SO2	0.083	0.000	0.08	1.99	2.000	-0.50
After						
SO2	0.000	0.000	0.00	2.00	2.000	0.00

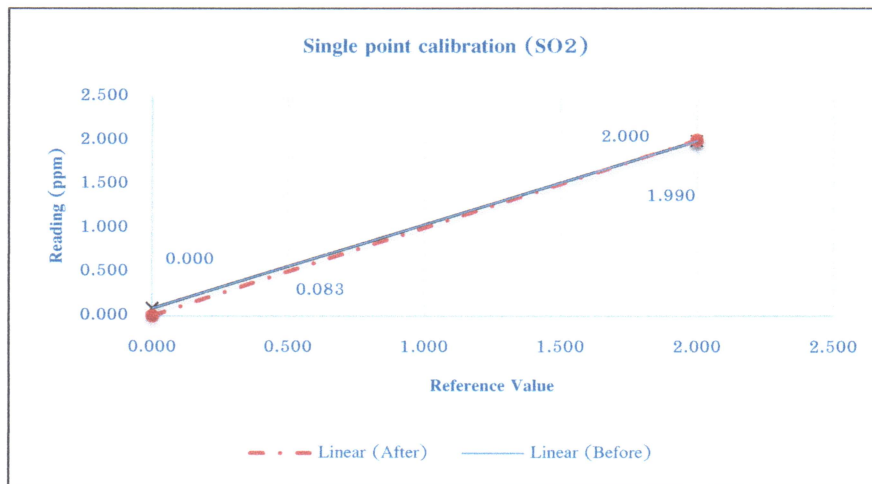

Calibrated by :

Tong Puima
(Mr. Tong Puima)

Certificate of Analyzer Performance Testing

Calibrated Date : 18-Aug-25

Certificate No. : 0825-002

Page : 1 / 1

Analyzer Instruments

Analyzer Type : SO2 Analyzer

Manufacturer : Thermo Environmental

Model : 43C

Serial No. : 43C-70853-367

Environmental

Temperature : 21.0 °C

Humidity : 42.7 %RH

Calibration System

Calibrator Units

Gas Calibration : Thermo Environmental

Zero Air Generator : API

Model : 146C

Model : 701

Serial No. : 514811458

Serial No. : 179

Standard Gas

NO Conc. : 2 ppm

Cylinder No. : 307199


SO2 Conc. : 2 ppm

Expire Date : 10-Oct-25

CO Conc. : 50 ppm

Calibration Check

Gas	Zero			Span		
	Reading Value (ppm)	Expected Value (ppm)	Drift (%)	Reading Value (ppm)	Expected Value (ppm)	Drift (%)
Before						
SO2	0.062	0.000	0.06	1.98	2.000	-1.00
After						
SO2	0.000	0.000	0.00	2.00	2.000	0.00

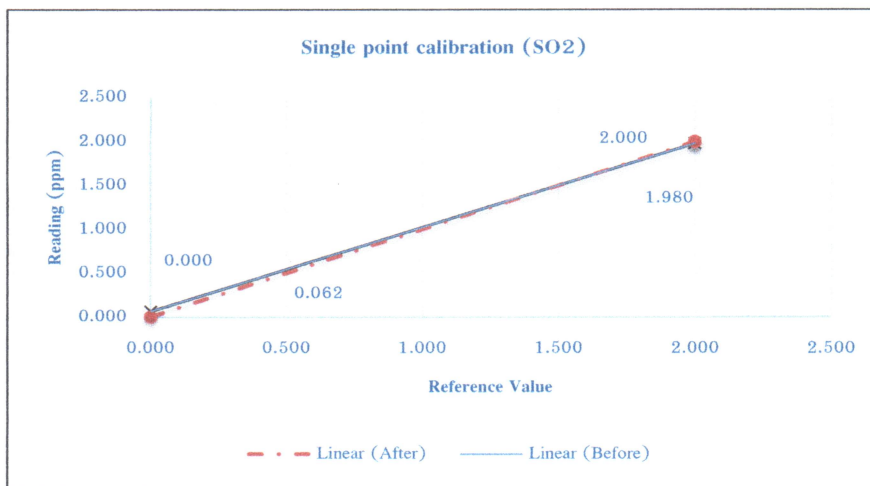

Calibrated by :

Tong Puima
(Mr. Tong Puima)