เอกสารแนบ 18

เอกสารอนุญาตห้องปฏิบัติการ

MM-C39

เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท ตรวจวัดสิ่งแวดล้อม จำกัด เลขทะเบียน ว-๓๐๑
ที่ อก ๐๓๑๐(๑)/ ๒๖๔ ๓ ลงวันที่ ๓๑ มกราคม ๒๕๖๖

ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๔ รายการ

น้ำเสีย จำนวน 4 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Biochemical Oxygen Demand	5-Day BOD Test, Membrane Electrode Method
2	pH	Electrometric Method
3	Total Dissolved Solids	Dried at 180 °C
4	Total Suspended Solids	Dried at 103-105 °C

เอกสารอ้างอิง

APHA, AWWA, WEF. **Standard Methods for the Examination of Water and Wastewater.** 23rd ed. Washington, DC: APHA, 2017.

น.18/1

ที่ อก ๐๓๑๐(๑)/ ๒๖๔ ๓

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๓๑ มกราคม ๒๕๖๖

เรื่อง ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

เรียน กรรมการผู้จัดการ บริษัท ตรวจวัดสิ่งแวดล้อม จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน ลงวันที่ ๘ ธันวาคม ๒๕๖๕

สิ่งที่ส่งมาด้วย เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน บริษัท ตรวจวัดสิ่งแวดล้อม จำกัด จำนวน ๑ แผ่น

ตามหนังสือที่อ้างถึง บริษัท ตรวจวัดสิ่งแวดล้อม จำกัด ขอต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๓๐๑ สถานที่ตั้งเลขที่ ๕/๔๕ หมู่บ้าน บ้านกลางกรุง บิซทาวน์ ซอยศรีนครินทร์ ๔๖/๑ (ปราโมทย์) แขวงหนองบอน เขตประเวศ กรุงเทพมหานคร ต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้บริษัท ตรวจวัดสิ่งแวดล้อม จำกัด ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน โดยมีองค์ประกอบดังนี้

ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์
ทะเบียนเลขที่ ว-๓๐๑-๑

ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์
ทะเบียนเลขที่ ว-๓๐๑-๒
ทะเบียนเลขที่ ว-๓๐๑-๓
ทะเบียนเลขที่ ว-๓๐๑-๔
ทะเบียนเลขที่ ว-๓๐๑-๕

ค. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนให้วิเคราะห์ในน้ำเสีย ตามสิ่งที่ส่งมาด้วย

หนังสือฉบับนี้จะหมดอายุในวันที่ ๓ มกราคม ๒๕๖๙ หากประสงค์จะต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ให้ยื่นคำขอต่ออายุพร้อมเอกสารประกอบคำขอต่อกรมโรงงานอุตสาหกรรม ภายใน ๓๐ วัน ก่อนวันสิ้นอายุของหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ทั้งนี้ สามารถยื่นคำขอผ่านระบบอิเล็กทรอนิกส์ได้ที่หน้าเว็บไซต์กรมโรงงานอุตสาหกรรม ตาม QR Code ท้ายหนังสือฉบับนี้

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน
กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ
โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕
โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๙๙
ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th

ยื่นคำขอผ่านระบบอิเล็กทรอนิกส์

Green Industry
"อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา อุตสาหกรรมสีเขียว"

MM-C39

ที่ อก ๐๓๑๐(๑)/ ๖๐๙๒

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๒๒ กรกฎาคม ๒๕๖๘

เรื่อง เปลี่ยนแปลงบุคลากรของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท ตรวจวัดสิ่งแวดล้อม จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน ลงวันที่ ๑๕ กรกฎาคม ๒๕๖๘

ตามคำขอที่อ้างถึง บริษัท ตรวจวัดสิ่งแวดล้อม จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๓๐๑ สถานที่ตั้งเลขที่ ๕/๔๕ หมู่บ้าน บ้านกลางกรุง บิซทาวน์ ซอยศรีนครินทร์ ๔๖/๑(ปราโมทย์) แขวงหนองบอน เขตประเวศ กรุงเทพมหานคร ขอเปลี่ยนแปลงบุคลากร ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว มีความเห็นดังนี้

๑. ให้ยกเลิกเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๒ ราย
ทะเบียนเลขที่ ว-๓๐๑
ทะเบียนเลขที่ ว-๓๐๑

๒. ให้เพิ่มผู้ควบคุมห้องปฏิบัติการวิเคราะห์เอกชน จำนวน ๒ ราย
ทะเบียนเลขที่ ว-๓๐๑
ทะเบียนเลขที่ ว-๓๐๑

๓. ให้เพิ่มเจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน จำนวน ๑ ราย
ทะเบียนเลขที่ ว-๓๐๑

อนึ่ง หนังสือฉบับนี้จะสิ้นอายุพร้อมหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ในวันที่ ๓ มกราคม ๒๕๖๙

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน
กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ
โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕
โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๙๙
ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th

น.18/2

ที่ อก ๐๓๑๐(๑)/๑๐๔๘๖

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๑๗ ตุลาคม ๒๕๖๗

เรื่อง ยกเลิกบุคลากรของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท ตรวจวัดสิ่งแวดล้อม จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน ลงวันที่ ๑ ตุลาคม ๒๕๖๗

ตามคำขอที่อ้างถึง บริษัท ตรวจวัดสิ่งแวดล้อม จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๓๐๑ สถานที่ตั้งเลขที่ ๕/๔๕ หมู่บ้าน บ้านกลางกรุง บิซทาวน์ ซอยศรีนครินทร์ ๔๖/๑(ปราโมทย์) แขวงหนองบอน เขตประเวศ กรุงเทพมหานคร ขอยกเลิกบุคลากร ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้ยกเลิกเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๑ ราย ได้แก่ น

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

รองอธิบดี ปฏิบัติราชการแทน
อธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน
กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ
โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕
โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๙๙
ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th

เลขที่ 43/2569

หนังสือรับรองการขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

กรมโรงงานอุตสาหกรรม ออกหนังสือฉบับนี้เพื่อ ต่ออายุ ให้
บริษัท ตรวจวัดสิ่งแวดล้อม จำกัด
ห้องปฏิบัติการวิเคราะห์เอกชนเลขทะเบียน ว-301

สถานที่ตั้งห้องปฏิบัติการ
เลขที่ 5/45 หมู่บ้านบ้านกลางกรุง บิซทาวน์ ซอยศรีนครินทร์ 46/1 (ปราโมทย์)
แขวงหนองบอน เขตประเวศ กรุงเทพมหานคร

โดยมีรายละเอียดผู้ควบคุมห้องปฏิบัติการวิเคราะห์เอกชน เจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน และขอบข่ายชนิดสารมลพิษ ดังเอกสารแนบ

ออกให้ ณ วันที่ 10 กุมภาพันธ์ 2569
หมดอายุวันที่ 3 มกราคม 2573

ทดสอบระบบ

ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กรมโรงงานอุตสาหกรรม
DEPARTMENT OF INDUSTRIAL WORKS

หนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชนฉบับนี้อาจถูกเพิกถอนได้ตามเงื่อนไขของข้อ 22 หมวด 6 แห่งประกาศกรมโรงงานอุตสาหกรรม เรื่อง ห้องปฏิบัติการวิเคราะห์เอกชน พ.ศ. 2566

50a20e9d

ที่ อก ๐๓๑๐(๑)/ ๖๗ ๓ ๓

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๑๕ สิงหาคม ๒๕๖๘

เรื่อง ยกเลิกบุคลากรของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท ตรวจวัดสิ่งแวดล้อม จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน ลงวันที่ ๑ สิงหาคม ๒๕๖๘

ตามคำขอที่อ้างถึง บริษัท ตรวจวัดสิ่งแวดล้อม จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๓๐๑ สถานที่ตั้งเลขที่ ๕/๔๕ หมู่บ้าน บ้านกลางกรุง บิซทาวน์ ซอยศรีนครินทร์ ๔๖/๑(ปราโมทย์) แขวงหนองบอน เขตประเวศ กรุงเทพมหานคร ขอยกเลิกบุคลากร ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้ยกเลิกผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๑ ราย ได้แก่ ๑

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน
กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ
โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕
โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๙๙
ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th

Green Industry
"อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา อุตสาหกรรมสีเขียว"

MM-C39

บุคลากรประจำห้องปฏิบัติการ

เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์เอกชน

ชื่อห้องปฏิบัติการ บริษัท ตรวจวัดสิ่งแวดล้อม จำกัด

เลขทะเบียน ว-301

สถานที่ตั้งห้องปฏิบัติการ เลขที่ 5/45 หมู่บ้านบ้านกลางกรุง บิชทาวน์ ซอยศรีนครินทร์ 46/1 (ปราโมทย์) แขวงหนองบอน เขตประเวศ กรุงเทพมหานคร

วันที่ออกหนังสือรับขึ้นทะเบียนห้องปฏิบัติการ 10 กุมภาพันธ์ 2569

วันที่หมดอายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการ 3 มกราคม 2573

รายชื่อเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์เอกชน ณ วันที่ออกใบรับรอง

ชื่อ-สกุล	ทะเบียนเลขที่
1	ว-301-
2	ว-301-
3	ว-301-

น.18/4

ใช้ประกอบหนังสือรับรองการขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน เลขที่ 43/2569

กรมโรงงานอุตสาหกรรม รับรองข้อมูล ณ วันที่ 10 กุมภาพันธ์ 2569

50a20e9d

บุคลากรประจำห้องปฏิบัติการ

ผู้ควบคุมห้องปฏิบัติการวิเคราะห์เอกชน

ชื่อห้องปฏิบัติการ บริษัท ตรวจวัดสิ่งแวดล้อม จำกัด

เลขทะเบียน ว-301

สถานที่ตั้งห้องปฏิบัติการ เลขที่ 5/45 หมู่บ้านบ้านกลางกรุง บิชทาวน์ ซอยศรีนครินทร์ 46/1 (ปราโมทย์) แขวงหนองบอน เขตประเวศ กรุงเทพมหานคร

วันที่ออกหนังสือรับขึ้นทะเบียนห้องปฏิบัติการ 10 กุมภาพันธ์ 2569

วันที่หมดอายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการ 3 มกราคม 2573

รายชื่อผู้ควบคุมห้องปฏิบัติการวิเคราะห์เอกชน ณ วันที่ออกใบรับรอง

ชื่อ-สกุล	ทะเบียนเลขที่
1	ว-30
2	ว-30

ใช้ประกอบหนังสือรับรองการขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน เลขที่ 43/2569

กรมโรงงานอุตสาหกรรม รับรองข้อมูล ณ วันที่ 10 กุมภาพันธ์ 2569

50a20e9d

ขอบข่ายและชนิดสารมลพิษที่ได้รับการขึ้นทะเบียน

ชื่อห้องปฏิบัติการ บริษัท ตรวจวัดสิ่งแวดล้อม จำกัด

เลขทะเบียน ว-301

สถานที่ตั้งห้องปฏิบัติการ เลขที่ 5/45 หมู่บ้านบ้านกลางกรุง บิซทาวน์ ซอยศรีนครินทร์ 46/1 (ปราโมทย์) แขวงหนองบอน เขตประเวศ กรุงเทพมหานคร

วันที่ออกหนังสือรับขึ้นทะเบียนห้องปฏิบัติการ 10 กุมภาพันธ์ 2569

วันที่หมดอายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการ 3 มกราคม 2573

ขอบข่าย	สารมลพิษ	วิธีวิเคราะห์
น้ำ/น้ำเสีย 5 รายการ	1. Biochemical Oxygen Demand 2. Oil and Grease 3. pH 4. Total Dissolved Solids 5. Total Suspended Solids	5-Day BOD Test, Membrane-Electrode Method Liquid-Liquid, Partition-Gravimetric Method Electrometric Method Dried at 180 °C Dried at 103-105 °C

<u>เอกสารอ้างอิง</u>

1. APHA, AWWA, WEF. Standard Methods for the Examination of Water and Wastewater. 23rd ed. Washington, DC: APHA, 2017.

หนังสือบันทึกการเปลี่ยนแปลง

ชื่อห้องปฏิบัติการ บริษัท ตรวจวัดสิ่งแวดล้อม จำกัด

เลขทะเบียน ว-301

สถานที่ตั้งห้องปฏิบัติการ เลขที่ 5/45 หมู่บ้านบ้านกลางกรุง บิซทาวน์ ซอยศรีนครินทร์ 46/1 (ปราโมทย์) แขวงหนองบอน เขตประเวศ กรุงเทพมหานคร

วันที่ออกหนังสือรับขึ้นทะเบียนห้องปฏิบัติการ 10 กุมภาพันธ์ 2569

วันที่หมดอายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการ 3 มกราคม 2573

ลำดับที่	สาระสำคัญของการเปลี่ยนแปลง	ผู้บันทึก
1	ขอต่ออายุทะเบียน	

List Certificate of Instrument for Environmental Quality Analysis.

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*	Remark
เครื่องมือสำหรับวิเคราะห์คุณภาพน้ำและดิน									
1	UV-VIS Spectrophotometer	Color (ADMI), Fluoride Chemical Oxygen Demand	Agilent Technologies	Cary60 G6860A / MY15410009	DQE Services Co.,Ltd.	SP25 019	26 May 25	25 May 26	-
2	UV-VIS Spectrophotometer	Sulfate, Phosphorus Nitrogen–Ammonia Nitrogen–Nitrate	Hitachi	U-5100 / 23A4-008	DQE Services Co.,Ltd.	SP25-024	17 Jun 25	16 Jun 26	-
3	COD Reactor (Heating Block)	Chemical Oxygen Demand (COD)	Hanna	HI839800-02 / H018500I	Hanna Instruments (Thailand) Ltd.	HIT-2510-0375	7 Mar 25	6 Mar 26	-
4	Cyanuric Acid Portable Photometer	Cyanuric acid	Hanna	HI97722C / 905060058111	Hanna Instruments (Thailand) Ltd.	HIT-2513-0437	24 Mar 25	23 Mar 26	-
5	Atomic Absorption Spectrophotometer (AAS)	Arsenic, Cadmium ,Chromium Copper, Iron, Manganese Zinc, Potaasium	Agilent Technologies	System ID:G8432A AA240FS / MY13160001	Thailand Institute of Scientific and Technological Research (TISTR)	MTC.ACL.No.372/68	3 Feb 25	2 Feb 26	-
6	Atomic Absorption Spectrophotometer (AAS)	Calcium, Lead, Mercury	Perkin Elmer	PinAAcle 900F / PFBS20031902	Perkin Elmer Co.,Ltd.	PinAAcle 900F Preventive Maintenance Report	29 Apr 25	28 Apr 26	-
7	Inductively Coupled Plasma (ICP)		Agilent Technologies	System ID:G8015A G8015AA / MY18030001	Agilent Technologies (Thailand) Co.,Ltd.	Preventive Maintenance Checklist	3 Nov 25	2 Nov 26	-
8	Cold Vapor Atomic Absorption Spectrophotometer (CVAAS)	Mercury(ดิน)	MILESTONE	DMA-80 / 24114043	Sithiporn Associates Co.,Ltd.	Service Protocol Report	31 Jan 25	30 Jan 26	-
9	Digestor Unit	Total Kjeldahl Nitrogen	FOSS TECATOR	DT2520 / 9190506	National Food Institute, Ministry of Industry, Thailand	2501440-001-01	27 Jan 25	26 Jan 26	-
10	Distillation Unit (Kjeldahl Method)		FOSS TECATOR	KT9 / 91905393	FOSS South East Asia	13851	25 Feb 25	24 Feb 26	-

เอกสารไม่ควบคุม

บริษัท ตรวจวัดสิ่งแวดล้อม จำกัด

List Certificate of Instrument for Environmental Quality Analysis.

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*	Remark
เครื่องมือสำหรับวิเคราะห์คุณภาพน้ำและดิน									
11	Incubator	Total Bacteria Total Coliform Bacteria	Memmert	IPP 260 / V615.0187	National Food Institute, Ministry of Industry, Thailand	2502229-001-01	19 Mar 25	18 Mar 26	-
12	Incubator	Fecal Coliform Bacteria Escherichia coli	Memmert	IPP 260 / V618.0033	National Food Institute, Ministry of Industry, Thailand	2502229-003-01	19 Mar 25	18 Mar 26	-
13	Water Bath	Pseudomonas Aeruginosa Staphylococcus Aureus	Memmert	WNE 14 / L416.0606	National Food Institute, Ministry of Industry, Thailand	2501624-001-01	10 Feb 25	9 Feb 26	-
14	Water Bath		Memmert	WNE 14 / L416.0612	National Food Institute, Ministry of Industry, Thailand	2501624-002-01	10 Feb 25	9 Feb 26	-
15	Auto Clave		ALP	CL-40L / 808763	National Food Institute, Ministry of Industry, Thailand	2502229-007-01	19 Mar 25	18 Mar 26	-
16	Auto Clave		ALP	CL-40L / 810010	National Food Institute, Ministry of Industry, Thailand	2503287-001-01	5 Jun 25	4 Jun 26	-
17	Analytical Balance		OHAUS	PX623 / C236754745	National Food Institute, Ministry of Industry, Thailand	2502227-001-01	19 Mar 25	18 Mar 26	-

Due Date of Calibration* : Based on the annual calibration plan. At least 1 time per year.

เอกสารไม่ควบคุม

MM-C39

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

NSC-TISI-TIS 17025 CALIBRATION 0404

REPORT OF CALIBRATION

Certificate No. : SP25-019

Environment Condition : Ambient Temperature 25 ± 5 °C

Relative humidity 55 ± 20 %RH

Calibration method : In-house method CP-01 Based on ASTM E275-08

Certified Reference Materials :

Material	Serial No.	Certificate No.	Due date
Absobance Standard set	25760	115663	25 October 2025
Absobance Standard set	25757	115638	25 October 2025
Wavelength Standard set	25806	115657	25 October 2025
Wavelength Standard set	25758	115665	25 October 2025

Traceability : This certification is traceable to the International System of Unit maintained at National - Institute of Standards and Technology (NIST) through Starna Scientific Limited

Spectral Band Width of UUC : 1.5 nm.

Scan Speed of UUC : 60 nm/min

Scan Interval of UUC : 0.15 nm.

Resolution of UUC : Photometric 0.0001 Abs.

Wavelength 0.1 nm.

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

NSC-TISI-TIS 17025 CALIBRATION 0404

CERTIFICATE OF CALIBRATION

Certificate No. : SP25-019

Customer : United Analyst and Engineering Consultant Co.,Ltd. (Head Office)

Address : 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Location of calibration : Instrument room (207)

Equipment : UV-Vis Spectrophotometer

Manufacturer : Agilent Technologies

Model : Cary 60

Serial No. : MY15410009

ID No. : UAE.WAT.020/2558

Received Date : 26 May 2025

Calibration Date : 26 May 2025

Issue Date : 29 May 2025

Condition Instrument : Good

Calibrated by : **Approved by :**

Technical Manager Quality Manager

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the DQE Services Co., Ltd.

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

NSC-TISI-TIS 17025 CALIBRATION 0404

REPORT OF CALIBRATION

Certificate No. : SP25-019

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor *k*
235	0.0000	0.0000	0.0000	0.0050	2.00
	0.7469	0.7488	-0.0019	0.0063	2.00
257	0.0000	0.0000	0.0000	0.0050	2.00
	0.8674	0.8663	0.0011	0.0067	2.00
313	0.0000	0.0000	0.0000	0.0050	2.00
	0.2919	0.2902	0.0017	0.0052	2.00
350	0.0000	0.0000	0.0000	0.0050	2.00
	0.6430	0.6428	0.0002	0.0063	2.00

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

NSC-TISI-TIS 17025 CALIBRATION 0404

REPORT OF CALIBRATION

Certificate No. : SP25-019

Calibration Results : Without adjustment

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor *k*
420	0.0000	0.0000	0.0000	0.0028	2.00
	0.5780	0.5739	0.0041	0.0031	2.00
	1.0484	1.0430	0.0054	0.0029	2.00
	2.1876	2.1876	0.0000	0.0084	2.00
440	0.0000	0.0000	0.0000	0.0028	2.00
	0.5595	0.5581	0.0014	0.0034	2.00
	1.0239	1.0219	0.0020	0.0035	2.00
	2.1230	2.1207	0.0023	0.0085	2.00
465	0.0000	0.0000	0.0000	0.0028	2.00
	0.5230	0.5190	0.0040	0.0029	2.00
	0.9633	0.9609	0.0024	0.0029	2.00
	1.9753	1.9719	0.0034	0.0079	2.00
546.1	0.0000	0.0000	0.0000	0.0028	2.00
	0.5181	0.5161	0.0020	0.0031	2.00
	1.0002	0.9979	0.0023	0.0033	2.00
	1.9973	2.0021	-0.0048	0.0102	2.00
590	0.0000	0.0000	0.0000	0.0028	2.00
	0.5517	0.5503	0.0014	0.0030	2.00
	1.0803	1.0808	-0.0005	0.0031	2.00
	2.0373	2.0324	0.0049	0.0105	2.00
635	0.0000	0.0000	0.0000	0.0028	2.00
	0.5591	0.5583	0.0008	0.0031	2.00
	1.0518	1.0513	0.0005	0.0030	2.00
	1.9274	1.9281	-0.0007	0.0102	2.00

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

MM-C39

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

NSC-TISI-TIS 17025 CALIBRATION 0404

CERTIFICATE OF CALIBRATION

Certificate No. : SP25-024 Page 1 of 5

Customer : United Analyst and Engineering Consultant Co.,Ltd. (Head Office)

Address : 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Location of calibration : Instrument room (207)

Equipment : UV-Vis Spectrophotometer

Manufacturer : HITACHI

Model : U-5100

Serial No. : 23A4-008

ID No. : UAE.WAS.010/2567

Received Date : 17 June 2025

Calibration Date : 17 June 2025

Issue Date : 20 June 2025

Condition Instrument : Good

Calibrated by : — **Approved by :** —

Technical Manager Quality Manager

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the DQE Services Co., Ltd.

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

NSC-TISI-TIS 17025 CALIBRATION 0404

REPORT OF CALIBRATION

Certificate No. : SP25-019 Page 5 of 5

Wavelength Accuracy :

CRMs Values (nm.)	UUC Reading (nm.)	Correction (nm.)	Uncertainty (nm.)	Coverage factor *k*
241.72	242.0	-0.28	0.18	2.00
279.45	279.5	-0.05	0.18	2.00
287.81	287.6	0.21	0.18	2.00
334.06	333.8	0.26	0.18	2.00
360.93	360.5	0.43	0.18	2.00
418.59	417.9	0.69	0.18	2.00
445.94	445.4	0.54	0.18	2.00
453.66	453.2	0.46	0.18	2.00
460.02	459.6	0.42	0.18	2.00
536.59	536.5	0.09	0.18	2.00
637.98	638.5	-0.52	0.18	2.00
431.38	430.7	0.68	0.18	2.00
472.50	472.3	0.20	0.18	2.00
513.47	513.5	-0.03	0.18	2.00
528.88	528.9	-0.02	0.18	2.00
573.17	573.8	-0.63	0.18	2.00
585.35	585.2	0.15	0.20	2.00
684.40	685.1	-0.70	0.18	2.00
740.72	741.1	-0.38	0.20	2.00
748.55	748.9	-0.35	0.18	2.00
807.03	807.1	-0.07	0.18	2.00
879.28	879.1	0.18	0.18	2.00

Remark : - UUC = Unit Under Calinration

- N/A = Not Avaiable
- The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor *k* , which for a normal distribution corresponds to a coverage probability of approximately 95%

- End of Certificate -

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

น.18/9

MM-C39

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

NSC-TISI-TIS 17025 CALIBRATION 0404

REPORT OF CALIBRATION

Certificate No. : SP25-024 Page 3 of 5

Calibration Results : Without adjustment

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor *k*
420	0.0000	0.000	0.0000	0.0028	2.00
	0.5780	0.574	0.0040	0.0031	2.00
	1.0484	1.044	0.0044	0.0029	2.00
	2.1876	2.185	0.0026	0.0075	2.00
440	0.0000	0.000	0.0000	0.0028	2.00
	0.5595	0.558	0.0015	0.0035	2.00
	1.0239	1.021	0.0029	0.0035	2.00
	2.1230	2.122	0.0010	0.0079	2.00
465	0.0000	0.000	0.0000	0.0028	2.00
	0.5230	0.519	0.0040	0.0030	2.00
	0.9633	0.961	0.0023	0.0029	2.00
	1.9753	1.975	0.0003	0.0071	2.00
546.1	0.0000	0.000	0.0000	0.0028	2.00
	0.5181	0.515	0.0031	0.0031	2.00
	1.0002	0.996	0.0042	0.0033	2.00
	1.9973	1.994	0.0033	0.0084	2.00
590	0.0000	0.000	0.0000	0.0028	2.00
	0.5517	0.549	0.0027	0.0030	2.00
	1.0803	1.078	0.0023	0.0030	2.00
	2.0373	2.031	0.0063	0.0082	2.00
635	0.0000	0.000	0.0000	0.0028	2.00
	0.5591	0.557	0.0021	0.0031	2.00
	1.0518	1.049	0.0028	0.0030	2.00
	1.9274	1.924	0.0034	0.0081	2.00

น.18/10

ไอกสารไ อสา กธ

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

NSC-TISI-TIS 17025 CALIBRATION 0404

REPORT OF CALIBRATION

Certificate No. : SP25-024 Page 2 of 5

Environment Condition : Ambient Temperature 25 ± 5 °C

Relative humidity 55 ± 20 %RH

Calibration method : In-house method CP-01 Based on ASTM E275-08

Certified Reference Materials :

Material	Serial No.	Certificate No.	Due date
Absobance Standard set	25760	115663	25 October 2025
Absobance Standard set	25757	115638	25 October 2025
Wavelength Standard set	25806	115657	25 October 2025
Wavelength Standard set	25758	115665	25 October 2025

Traceability : This certification is traceable to the International System of Unit maintained at National - Institute of Standards and Technology (NIST) through Starna Scientific Limited

Spectral Band Width of UUC : 5.0 nm.

Scan Speed of UUC : 40

Scan Interval of UUC : 0.1 nm.

Resolution of UUC : Photometric 0.001 Abs.

Wavelength 0.1 nm.

เอกสารไ อสา กธ

FM-708-02 R01 1/11/2021

MM-C39

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

NSC-TISI-TIS 17025 CALIBRATION 0404

REPORT OF CALIBRATION

Certificate No. : SP25-024

Wavelength Accuracy :

CRMs Values (nm.)	UUC Reading (nm.)	Correction (nm.)	Uncertainty (nm.)	Coverage factor *k*
241.00	240.4	0.60	0.18	2.00
279.30	278.8	0.50	0.18	2.00
288.90	288.3	0.60	0.18	2.00
334.50	333.9	0.60	0.18	2.00
361.40	360.8	0.60	0.18	2.00
418.40	417.9	0.50	0.18	2.00
447.20	446.6	0.60	0.18	2.00
459.30	459.1	0.20	0.18	2.00
537.00	536.4	0.60	0.18	2.00
638.00	637.5	0.50	0.18	2.00
441.29	440.7	0.59	0.18	2.00
479.88	479.4	0.48	0.18	2.00
513.75	513.3	0.45	0.18	2.00
528.59	528.2	0.39	0.18	2.00
575.10	574.5	0.60	0.18	2.00
585.56	585.4	0.16	0.20	2.00
684.70	684.1	0.60	0.18	2.00
740.51	740.2	0.31	0.20	2.00
747.61	747.0	0.61	0.18	2.00
807.04	806.4	0.64	0.18	2.00
879.68	879.1	0.58	0.18	2.00

Remark : - UUC = Unit Under Calinration

- N/A = Not Avaiable
- The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor *k*, which for a normal distribution corresponds to a coverage probability of approximately 95%

- End of Certificate -

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

NSC-TISI-TIS 17025 CALIBRATION 0404

REPORT OF CALIBRATION

Certificate No. : SP25-024

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor *k*
235	0.0000	0.000	0.0000	0.0050	2.00
	0.7469	0.747	-0.0001	0.0057	2.00
257	0.0000	0.000	0.0000	0.0050	2.00
	0.8674	0.864	0.0034	0.0059	2.00
313	0.0000	0.000	0.0000	0.0050	2.00
	0.2919	0.293	-0.0011	0.0051	2.00
350	0.0000	0.000	0.0000	0.0050	2.00
	0.6430	0.639	0.0040	0.0055	2.00

เอกสารไม่ควบคุม

น.18/11

MM-C39

HANNA instruments

Certificate No. : HIT-2510-0375

Condition of this calibration result:

Reference Standard Instruments : This certification is traceable to the international unit of unit maintained through:

Instruments	Model	Serial No.	Certificate No.	Traceable
Data Acquisition Switch Unit	34970A	MY44065265	WK2407-141-1	WK Electric Co., Ltd.
Digital Thermo-Hygrometer	HT-771SD	AI.07155	25H171	Technology Promotion Association (Thailand-Japan).

Calibration Result:

Measurement Temperature Source Accuracy for COD Reactor.

Capacity (Vial)	Nominal Value (°C)	Average Value (°C)	Uncertainty of Measurement (±°C)
25 Vial	150.0	150.4	0.47

Unit : °C

(1A) 150.407	(2A) 150.377	(3A) 150.269	(4A) 150.402	(5A) 150.422
(1B) 150.426	(2B) 150.394	(3B) 150.644	(4B) 150.690	(5B) 150.542
(1C) 150.477	(2C) 150.303	(3C) 150.627	(4C) 150.257	(5C) 150.176
(1D) 150.462	(2D) 150.456	(3D) 150.199	(4D) 150.406	(5D) 150.102
(1E) 150.185	(2E) 150.513	(3E) 150.235	(4E) 150.460	(5E) 150.442

Figure: Shows the location of the temperature source.

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

** End of certificate **

เอกสารไม่ควบคุม

11/8/12

HANNA instruments

Hanna Instruments (Thailand) Ltd.
410/67-68 Soi Ratchadapisek 24, Ratchadapisek Rd., Samsen-nok,
Huaykwang, Bangkok 10310 Tel: 0-2541-4199 Fax: 0-2541-4198

ilac-MRA ANAB ANSI National Accreditation Board ACCREDITED ISO/IEC 17025 CALIBRATION LABORATORY AC-3061

Certificate No. : HIT-2510-0375

CERTIFICATE OF CALIBRATION

Equipment :	COD Test Tube Heater		
Meter Model :	HI839800-02	**Serial No. :**	H018500I
Tube Heater :	25 Vial Capacity	**Resolution :**	0.1°C
Temperature Range :	(-10 to 160)°C	**Temperature of Reaction :**	150°C
Manufacturer :	Hanna Instruments	**Made in :**	Romania
Condition As-Received :	Used Product	**Reference :**	RE250401
Ambient Temperature :	(25 ± 2)°C	**Relative Humidity :**	(50 ± 15)% RH
Customer name :	United Analyst and Engineering Consultant Co., Ltd. 3 Soi Udomsuk 41, Sukhumvit Rd., Bangchak, Phrakhanong, Bangkok 10260		
Received date :	5 March 2025		
Calibrate date :	7 March 2025		
Issue date :	7 March 2025		
Calibrated Location :	Hanna Instruments (Thailand) Ltd.		
Calibration Procedure :	This calibrator was conducted by using in-house: calibration procedure CP-04 by using certified reference standard instruments.		

Calibrated by :

Approved by :

Authorized Signatory

HANNA Instruments (Thailand) Limited

This certificate was certified only for the instrument we calibrated.

This result of calibration was found accurate on date and place of calibration only.

** This certificate may not be reproduced other than in full, except with the prior written ** approval of the head of Hanna Instrument (Thailand)

เอกสารไม่ควบคุม

Condition of this result of analysis

Cal Check Standard Cuvettes Specifications :

Product code: HI97722-11 **Lot number:** SC0391/24

Standard cuvette	Standard Value (mg/L)	Lot Standard Deviation (mg/L)	Lot number	Best used before
A, ZERO	0	0.001	8366	April 2026
B, HI97722	20	0.207	7872	April 2026

Specifications for validation procedure:

Standard cuvette	Standard Value (mg/L)	Lot Standard Deviation (mg/L)	Lot number	Best used before
B, HI97722	20 ± 1	19 to 21	7872	April 2026

Method of Standardization

This quality is standardized using which is calibrated by adaptation of Turbidimetric Method as the following details below :

Result of analysis :

Cyanuric Acid Standard (mg/L)	Reading (mg/L)	Error (mg/L)
0	0	0
20 ± 1	20	0

** End of certificate **

เอกสารไม่ควบคุม

Hanna Instruments (Thailand) Ltd.
410/67-68 Soi Ratchadapisek 24, Ratchadapisek Rd., Samsen-nok,
Huaykwang, Bangkok 10310 Tel: 0-2541-4199 Fax: 0-2541-4198

CERTIFICATE OF ANALYSIS

Equipment :	Cyanuric Acid Portable Photometer		
Meter Model :	HI97722C	**Serial No. :**	905060058111
Manufacturer :	Hanna Instruments		
Made in :	Romania		
Condition As-Received :	Used Product		
Reference :	RE250509		
Customer name :	United Analyst and Engineering Consultant Co., Ltd. 3 Soi Udomsuk 41, Sukhumvit Rd., Bangchak, Phrakhanong, Bangkok 10260		
Received date :	20 March 2025		
Calibrate date :	24 March 2025		
Issue date :	24 March 2025		
Ambient Temperature :	(25 ± 2)°C		
Relative Humidity :	(50 ± 15)% RH		
Calibrated Location :	Hanna Instruments (Thailand) Ltd.		

Calibrated by : **Approved by :**

Authorized Signatory

HANNA Instruments (Thailand) Limited

This certificate was certified only for the instrument we calibrated.

This result of calibration was found accurate on date and place of calibration only.

** This certificate may not be reproduced other than in full, except with the prior written **
approval of the head of Hanna Instrument (Thailand)

เอกสารไม่ควบคุม

MM-C39

Request No. 25-68 / 0320 1 / 5 MTC. ACL. No. 372 / 68

CALIBRATION DATA

1. Noise Level

Element	Cd	Cr	Cu	Fe	Pb	Mn	Ni	Zn
Absorbance	0.0006	0.0001	-0.0009	0.0003	0.0009	0.0010	0.0007	0.0008
	-0.0001	-0.0012	-0.0007	0.0005	0.0000	0.0002	0.0009	0.0002
	-0.0007	-0.0010	-0.0002	0.0008	0.0003	0.0014	0.0009	0.0002
	-0.0002	-0.0002	-0.0005	0.0009	0.0003	0.0002	0.0008	0.0011
	0.0000	-0.0005	-0.0008	0.0008	0.0007	0.0001	-0.0004	0.0013
	0.0001	-0.0002	-0.0007	0.0006	-0.0002	-0.0001	0.0002	0.0005
	-0.0002	0.0000	-0.0004	0.0009	-0.0002	-0.0008	0.0001	0.0008
	0.0006	-0.0007	-0.0001	0.0004	-0.0001	-0.0003	0.0009	0.0003
	0.0008	-0.0008	-0.0008	0.0014	0.0007	-0.0005	0.0009	0.0005
	-0.0005	-0.0008	-0.0009	0.0013	0.0006	-0.0002	0.0002	0.0014
	-0.0002	-0.0013	0.0010	0.0011	0.0004	-0.0005	0.0001	0.0006
	-0.0005	-0.0018	0.0012	0.0014	0.0004	-0.0006	0.0005	0.0014
	-0.0009	-0.0012	0.0006	0.0014	0.0003	-0.0003	0.0004	0.0010
	0.0003	-0.0017	0.0002	0.0016	0.0003	0.0000	-0.0005	0.0002
	0.0003	-0.0015	0.0003	0.0002	0.0006	0.0003	0.0007	0.0009
	0.0004	-0.0005	0.0001	0.0014	0.0007	0.0009	0.0007	0.0007
	-0.0001	0.0018	0.0010	0.0016	0.0001	-0.0002	0.0012	-0.0002
	0.0003	-0.0017	0.0012	0.0011	0.0003	0.0005	0.0011	-0.0002
	0.0010	-0.0018	-0.0007	0.0009	0.0010	0.0009	0.0001	0.0004
	0.0004	0.0007	-0.0008	0.0004	0.0011	0.0003	0.0002	0.0000
Average Absorbance	0.000	-0.001	0.000	0.001	0.000	0.000	0.000	0.001

Continue 2 / 5

INDUSTRIAL METROLOGY AND TESTING SERVICE CENTRE

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 3219 9440

เอกสารไม่ควบคุม

Request No. 25-68 / 0320 MTC. ACL.No. 372 / 68

CALIBRATION CERTIFICATE

NOMENCLATURE : 1. Atomic Absorption Spectrophotometer "Agilent Technologies"
Model AA240FS, Serial No. MY13160001
2. Working standard solution "CPA chem"
Solution of 29 components, Lot No. 1012852

SUBMITTED BY : United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

CALIBRATION PROCEDURE : 1. Performance Verification of Atomic Absorption Spectrophotometer (WI-500-02-30)
2. Estimation Uncertainty of Measurement in Analytical Chemistry (QP-513)

CALIBRATION RANGE: 0.02, 0.10, 0.30, 0.50, 0.70 mg/l at 228.8 nm.Cd, 0.10, 0.20, 0.30, 0.50, 0.70 mg/l at 357.9 nm.Cr, 0.05, 0.10, 0.30, 0.50, 0.70 mg/l at 324.7 nm.Cu, 0.10, 0.30, 0.50, 0.70, 1.00 mg/l at 248.3 nm.Fe, 0.20, 0.50, 0.70, 1.00, 1.50 mg/l at 217.0 nm.Pb, 0.05, 0.10, 0.30, 0.50, 0.70 mg/l at 279.5 nm.Mn, 0.10, 0.30, 0.50, 0.70, 1.00 mg/l at 232.0 nm.Ni, 0.05, 0.10, 0.30, 0.50, 0.70 mg/l at 213.9 nm.Zn

CALIBRATION DATE : 3 February 2025

REFERENCE MATERIAL : Traceable to NIST "Agilent Technologies", "CARLO ERBA", "PanReac AppliChem"
Cadmium Lot No. 0001152457, Chromium Lot No. 0106315418, Copper Batch No. 0001268514, Iron Batch No. T126087A, Lead Lot No. 0123204734, Manganese Batch No. 0106301952, Nickel Batch No. 0104978044, Zinc Batch No. 0100792297

AMBIENT CONDITIONS : Temperature 25 ± 5 °C Relative humidity 50 ± 20 %

The Atomic Absorption Spectrophotometer has been calibrated against Reference Material traceable to National Institute of Standards and Technology (NIST) by The Analytical Chemistry Laboratory. The results are attached herewith.

Calibrated by .....

Approved by.....

Director of Analytical Chemistry Laboratory

Ref. 2015268013000459001

Issued Date : 7 March 2025

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217

เอกสารไม่ควบคุม

2. Precision

Element	Conc. (mg/l)	Absorbance										Ave. Abs.	SD	%RSD
Cd	0.02	0.0076	0.0066	0.0071	0.0065	0.0075	0.0066	0.0077	0.0065	0.0065	0.0065	0.007	0.0005	7.39
	0.30	0.0923	0.0921	0.0920	0.0917	0.0919	0.0904	0.0929	0.0910	0.0915	0.0927	0.092	0.0008	0.82
	0.70	0.2083	0.2082	0.2100	0.2114	0.2102	0.2091	0.2096	0.2093	0.2088	0.2082	0.209	0.0010	0.49
Cr	0.10	0.0095	0.0104	0.0097	0.0095	0.0093	0.0091	0.0096	0.0095	0.0082	0.0080	0.009	0.0007	7.63
	0.30	0.0234	0.0243	0.0237	0.0242	0.0214	0.0226	0.0232	0.0233	0.0237	0.0237	0.023	0.0008	3.61
	0.70	0.0474	0.0490	0.0497	0.0516	0.0487	0.0476	0.0474	0.0484	0.0473	0.0474	0.048	0.0014	2.85
Cu	0.05	0.0073	0.0072	0.0060	0.0068	0.0067	0.0065	0.0070	0.0066	0.0068	0.0070	0.007	0.0004	5.53
	0.30	0.0380	0.0385	0.0377	0.0382	0.0394	0.0375	0.0381	0.0392	0.0389	0.0385	0.038	0.0006	1.62
	0.70	0.0888	0.0895	0.0890	0.0902	0.0897	0.0893	0.0899	0.0890	0.0902	0.0898	0.090	0.0005	0.56
Fe	0.10	0.0102	0.0103	0.0100	0.0092	0.0109	0.0094	0.0101	0.0098	0.0092	0.0101	0.010	0.0005	5.39
	0.50	0.0421	0.0421	0.0424	0.0421	0.0425	0.0412	0.0419	0.0425	0.0419	0.0429	0.042	0.0005	1.09
	1.00	0.0791	0.0782	0.0780	0.0780	0.0776	0.0792	0.0780	0.0782	0.0786	0.0794	0.078	0.0006	0.78
Pb	0.20	0.0092	0.0087	0.0081	0.0092	0.0090	0.0087	0.0091	0.0082	0.0091	0.0088	0.009	0.0004	4.49
	0.70	0.0275	0.0290	0.0288	0.0283	0.0272	0.0286	0.0280	0.0285	0.0288	0.0286	0.028	0.0006	2.09
	1.50	0.0592	0.0580	0.0591	0.0596	0.0577	0.0589	0.0591	0.0584	0.0575	0.0595	0.059	0.0008	1.28
Mn	0.05	0.0126	0.0130	0.0123	0.0113	0.0115	0.0126	0.0122	0.0123	0.0114	0.0117	0.012	0.0006	4.81
	0.30	0.0588	0.0582	0.0584	0.0593	0.0582	0.0584	0.0596	0.0602	0.0581	0.0577	0.059	0.0008	1.33
	0.70	0.1320	0.1318	0.1313	0.1306	0.1324	0.1314	0.1320	0.1308	0.1303	0.1305	0.131	0.0007	0.56
Ni	0.10	0.0107	0.0110	0.0102	0.0098	0.0101	0.0106	0.0096	0.0108	0.0100	0.0102	0.010	0.0005	4.44
	0.50	0.0452	0.0454	0.0441	0.0449	0.0452	0.0450	0.0453	0.0452	0.0454	0.0455	0.045	0.0004	0.89
	1.00	0.0848	0.0875	0.0856	0.0853	0.0866	0.0866	0.0866	0.0865	0.0857	0.0859	0.086	0.0008	0.92
Zn	0.05	0.0367	0.0370	0.0372	0.0362	0.0369	0.0367	0.0363	0.0367	0.0365	0.0360	0.037	0.0004	1.02
	0.30	0.2022	0.2009	0.2022	0.2017	0.2022	0.2009	0.2001	0.2016	0.2022	0.2023	0.202	0.0008	0.38
	0.70	0.4118	0.4123	0.4107	0.4132	0.4142	0.4157	0.4086	0.4098	0.4101	0.4079	0.411	0.0025	0.60

Continue 3 / 5

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 3219 9440

เอกสารไม่ควบคุม

Request No. 25-68 / 0320 3 / 5 MTC. ACL. No. 372 / 68

3. Trueness

3.1 Reading on wavelength- Cadmium(Cd) at 228.8 nm.

Element	Standard Value of RM (mg/l)	Reading (mg/l)	Error of Measurement (mg/l)	Error of Measurement (%)	Uncertainty (mg/l)
Cd	0.020	0.020	0.000	1.23	± 0.005
	0.300	0.300	0.000	0.11	± 0.005
	0.700	0.688	-0.012	1.67	± 0.008

3.2 Reading on wavelength- Chromium (Cr) at 357.9 nm.

Element	Standard Value of RM (mg/l)	Reading (mg/l)	Error of Measurement (mg/l)	Error of Measurement (%)	Uncertainty (mg/l)
Cr	0.1000	0.109	0.009	9.39	± 0.009
	0.3000	0.306	0.006	1.98	± 0.012
	0.7000	0.657	-0.043	6.20	± 0.023

3.3 Reading on wavelength- Copper (Cu) at 324.7 nm.

Element	Standard Value of RM (mg/l)	Reading (mg/l)	Error of Measurement (mg/l)	Error of Measurement (%)	Uncertainty (mg/l)
Cu	0.050	0.050	0.000	0.68	± 0.003
	0.300	0.292	-0.008	2.70	± 0.009
	0.700	0.684	-0.016	2.31	± 0.020

Continue 4 / 5

INDUSTRIAL METROLOGY AND TESTING SERVICE CENTRE

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 3219 9440

เอกสารไม่ควบคุม

MM-C39

3.4 Reading on wavelength- Iron (Fe) at 248.3 nm.

Element	Standard Value of RM (mg/l)	Reading (mg/l)	Error of Measurement (mg/l)	Error of Measurement (%)	Uncertainty (mg/l)
Fe	0.100	0.107	0.007	7.06	± 0.014
	0.500	0.522	0.022	4.49	± 0.016
	1.000	0.990	-0.010	1.02	± 0.029

3.5 Reading on wavelength- Lead (Pb) at 217.0 nm.

Element	Standard Value of RM (mg/l)	Reading (mg/l)	Error of Measurement (mg/l)	Error of Measurement (%)	Uncertainty (mg/l)
Pb	0.200	0.200	0.000	0.15	± 0.014
	0.700	0.701	0.001	0.10	± 0.030
	1.500	1.480	-0.020	1.32	± 0.061

3.6 Reading on wavelength- Manganese (Mn) at 279.5 nm.

Element	Standard Value of RM (mg/l)	Reading (mg/l)	Error of Measurement (mg/l)	Error of Measurement (%)	Uncertainty (mg/l)
Mn	0.050	0.051	0.001	2.41	± 0.005
	0.300	0.291	-0.009	2.92	± 0.007
	0.700	0.665	-0.035	4.95	± 0.014

Continue 5 / 5

INDUSTRIAL METROLOGY AND TESTING SERVICE CENTRE

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

3.7 Reading on wavelength- Nickel (Ni) at 232.0 nm.

Element	Standard Value of RM (mg/l)	Reading (mg/l)	Error of Measurement (mg/l)	Error of Measurement (%)	Uncertainty (mg/l)
Ni	0.100	0.098	-0.002	1.60	± 0.013
	0.500	0.490	-0.010	2.00	± 0.018
	1.000	0.951	-0.049	4.90	± 0.032

3.8 Reading on wavelength- Zinc (Zn) at 213.9 nm.

Element	Standard Value of RM (mg/l)	Reading (mg/l)	Error of Measurement (mg/l)	Error of Measurement (%)	Uncertainty (mg/l)
Zn	0.050	0.048	-0.002	3.37	± 0.013
	0.300	0.325	0.025	8.32	± 0.013
	0.700	0.677	-0.023	3.33	± 0.019

Remark : The reported uncertainty is an expanded uncertainty calculated using a coverage factor of 2 (k = 2) which gives a level of confidence of approximately 95%

Calibrated by ..... Atipat. .....

(Mr. Atipat Ratana)

Approved by .....

Director of Analytical Chemistry Laboratory

Issued Date : 7 March 2025

INDUSTRIAL METROLOGY AND TESTING SERVICE CENTRE

End of Certificate

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

PinAAcle 900F Preventive Maintenance (PM)

Company Name:	United Analyst and Engineering Consultant Co., LTD.		
Address (Instrument Location):	41 Sukumvhit Rd., Phra Khanong, Bangkok 10260		
Serial Number:	PFBS20031902	**PM Number:**	1 of 2
Customer Name (if applicable):	K. Yainda	**Telephone Number:**	095-5580049
Customer Support Engineer Name:	K. Chayanan	**Service Order Number:**	WO-03126047
Date PM Performed: (DD-MMM-YYYY)	29-Apr-2025	**Next PM Due Date:** (DD-MMM-YYYY)	29-Oct-2025
Standard Labor Hours to Complete PM :		**5 hours**	

Part Number	Release	Publication Date	
09370145 Rev.9	A	January 2018	PerkinElmer

Scope
The purpose of this PM is to ensure the continued functionality of the PinAAcle 900F by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer.
The customer should save their method before the PM begins.

General Instructions:
The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM.
Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files.
The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer.
Update the PM sticker and instrument logbook as required.

Copyright Information
This document contains proprietary information that is protected by copyright. All rights are reserved.
No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of PerkinElmer, Inc.
Copyright © 2013 PerkinElmer, Inc.

Trademarks
Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners.
Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no Warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.
PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

เอกสารไม่ควบคุม

PerkinElmer
For the Better

PinAAcle 900F Preventive Maintenance Report

Company Name: UAE Consultant Co., LTD.

Instrument Location: 41 Sukumvhit Rd.,

Phra Khanong, Bangkok 10260

Instrument Serial No.: PFBS20031902

Date: 29-Apr-2025

เอกสารไม่ควบคุม

Additional Tools Required for PM			
Part Number (if applicable)	**Description**	**Quantity**	**Serial #**
N1013000	0.2A Neutral density filter	1	101N0089015
N1013002	1.0A Neutral density filter	1	101N0089015
03030997	System 2 EDL Driver	1	03030997
N3050605	As System 2 EDL	1	16148
N3050121	Cu Lumina HCL	1	060419-030180
N3050109	Ba Lumina HCL	1	061219-020041
N3050139	K Lumina HCL	1	030819-010130
N3050152	Ni Lumina HCL	1	052719-020020

เอกสารไม่ควบคุม

Component List

Component / Specific Model	Serial #	Configuration Notes
PinAACle900F	PFBS20031902	Syngistix V4.0.1.1935
FIAS100	100S24040501	

Parts Lists

Parts Included with the PM		
Part Number (if applicable)	**Description**	**Quantity**
B0501696	Fan Filters	2
N3160156	O-Ring Kits for Sampling Introduction (Stainless Steels Nebulizer)	N/A
N3160157	O-Ring Kits for Sampling Introduction (Plastic Nebulizer)	1
N9301714	Replacement Acetylene Filter Cartridge	1
TH001022	Replacement Air Filter Cartridge	1

Additional Reagents and Standards Required for PM				
Part Number (if applicable)	**Description**	**Quality**	**Batch/Lot #**	**Expired Date (MM/YY)**
N9300183	1000 mg/L Copper Standard	AR	27-39CUY1	Nov 2025

Additional Reagents and Standards Required for PM (Customer Support Solution)				
Part Number (if applicable)	**Description**	**Quantity**	**Batch/Lot #**	**Expiration Date (MM/YY)**
N/A	DI Water	250 ml.	AR	AR
N/A	0.5% HNO_3	250 ml.	AR	AR

เอกสารไม่ควบคุม

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. **General:**
   - ☑ Review the instrument performance with the customer and document any recent problems.
   - ☑ Inspect the customer log book and make any appropriate PM entries.
   - ☑ Perform general inspection of system for cleanliness.

2. **PC Instrument Software:**
   - ☑ Instrument Software user files/databases archived, packed, and/or deleted as needed.

3. **Mechanical:**
   - ☑ Inspect and clean all fans and filters. Replace filters if necessary
   - ☑ Inspect all gas lines for leaks and/or wear. Replace if needed.
   - ☑ Clean exterior of the instrument.
   - ☑ Inspect the burner head, burner chamber, and nebulizer. Clean if needed as stated in the Hardware Guide.
   - ☑ Check burner head dimensions with the feeler gauge as stated in the Hardware Guide in the Maintenance chapter section on cleaning the burner head and checking sloth width. Replace if out of specification
   - ☑ Check the condition of the end cap, burner head, and nebulizer O-rings. Replace if necessary.
   - ☑ Check the drain system for signs of wear. Replace worn or damaged parts.
   - ☑ Visually check for proper flame conditions when igniting the Air-C2H2 and N20-C2H2 flames (if applicable).

4. **Electrical:**
   - ☑ Inspect PC boards. Clean if necessary.
   - ☑ Carefully check all internal and external cable connections.
   - ☑ Check instrument firmware revisions upgrade to current levels (if necessary)
   - ☑ Run Diagnostics Test within the Advanced function of the Spectrometer page. Check the results in the service log folder in the Spectrometer BM Log Viewer.

5. **Optics:**
   - ☑ Inspect and clean the sample compartment windows, if needed.
   - ☑ Inspect optics. Clean or replace if necessary,

6. **Gasses:**
   - ☑ Verify that the Gasses supplied to the instrument are within the pressure and purity specifications found in the PinAAcle 900 Series Pre-installation Checklist SDB.
   - ☑ Verify that the acetylene filter and air filter element is dry. Replace if necessary.

เอกสารไม่ควบคุม

7. **Flame Interlock Check:**

Description: Check to ensure that all safety interlocks are closed.

Parameter	Specification	Test Results	Pass/Fail
Flame Sensor	Air/C_2H_2 Flame correctly shuts down	Active	Passed
Drain Sensor	Air/C_2H_2 Flame correctly shuts down	Active	Passed
Nebulizer Sensor	Air/C_2H_2 Flame correctly shuts down	Active	Passed
C_2H_2 Pressure Sensor	Air/C_2H_2 Flame correctly shuts down	Active	Passed
Air Pressure Sensor	Air/C_2H_2 Flame correctly shuts down	Active	Passed
Burner Head Sensor	Choosing Nitrous Oxide as the oxidant should trigger an interlock shuts down	Active	Passed

8. **After PM Performance tests:**

8.1 Detector Linearity with Barium

Description: Ensures that the detector is linear in the Visible Range.

Parameter	Specification	Certificate Value at 553.6 nm (Abs.)	Test Results	Pass/Fail
1.0 A ND Filter	± 5% from Cert.	0.9668	0.9878	Passed
0.2 A ND Filter	± 5% from Cert.	0.1953	0.1876	Passed

8.2 Baseline Noise at 1.0 Absorbance with Barium

Description: Ensures that a high absorbance will not produce excessive noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.010	0.0005	Passed

8.3 AA Baseline Noise with Copper

Description: Check baseline noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.001	0.0001	Passed

เอกสารไม่ควบคุม

8.4 D_2 Background Compensation with Copper

Description: Verifies the instruments ability to compensate for Background absorption.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.010	0.009	Passed

8.5 AA-BG Baseline Noise with Copper

Description: Ensures that background correction does not produce excessive noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.005	0.0001	Passed

8.6 AA-BG Baseline Noise with Arsenic

Description: Ensures that background correction does not produce excessive noise at a low wavelength.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.005	0.0004	Passed

8.7 Flame Sensitivity

Description: Instrument Sensitivity checked against Copper standard.

Standard Copper Sensitivity	Specification	Results (Abs.)	Pass/Fail
5 mg/L Sensitivity SS Neb (if applicable)	> 0.250 Abs.	N/A	Not Applicable
2 mg/L Sensitivity HS Neb (if applicable)	> 0.250 Abs.	N/A	Passed

10. Review:

- ☑ Review with the customer PM work performed.
- ☑ Review with the customer routine maintenance procedures.
- ☑ Discuss recommended customer supplied materials to have on hand.
- ☑ Attach PM sticker.

เอกสารไม่ควบคุม

Additional Comments

Additional Comments Regarding the PM

Review

The preventive maintenance checks and if applicable performance tests for PinAAcle 900F have been completed. *This PinAAcle 900F Passes ☑ Fails ☐ the preventive maintenance.*	
Review of Preventive Maintenance:	
Authorized PerkinElmer Representative:	Date: 29 Apr 2025 (DD-MMM-YYYY)
Authorized Customer Representative:	Date: 29 Apr 2025 (DD-MMM-YYYY)

เอกสารไม่ควบคุม

Customer Acknowledgment of receipt of the above repair / replacement.

Special Terms and Conditions: This is not an invoice.

Taxes will be applied to your invoice if applicable.

เอกสารไม่ควบคุม

PerkinElmer
For the Better

PerkinElmer Scientific (Thailand) Co., Ltd.
290 Soi Soonvijai 4
Khwang Bangkapi, Khet Huay Kwang
Bangkok 10310
Thailand
Tel: 66 2719 6420 ; Fax: +66 2 319 7900
http://www.perkinelmer.com

Service Report

Work Order Number	Activity Code	Billing Type	Requested Start Date	Model	Serial Number
WO-03126047	Planned Maintenance	Contract	10/01/2568 11:08 น.	AAN3200051	PFBS20031902

Service Representative Name	Contract Number	Expiry Date	Equipment ID	System ID
Kanan, Chayanan	SC-0035664109	31/10/2025	N/A	N/A

UDI Number
N/A

Equipment Location	Bill To Name
บริษัท ยูไนเต็ด แอนนาลิสต์ แอนด์ แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 51 10260 TH	บริษัท ยูไนเต็ด แอนนาลิสต์ แอนด์ แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 51 10260 TH

Customer Contact	Phone Number	Fax Number	Email	Purchase Order
K. ณาฉันคา แซ่มเล็ก(ใบหม่อน)	095-5580049	N/A	nichakorn.praemai1998@gmail.com	HPO-250100002

Work Description
- PM 2/2 (AAเครื่องเก่า) - Cleaning Cell, Chamber, Filter - Wavelength Calibrate ; Pass - Wavelength Scan As,Cu,Ba,K,Ni ; Pass -Align cell with Hg. : OK

Start Date	End Date	Work Description
29/04/2025	09/05/2025	

Tools Used					
Quantity	Calibrated Tool	Description	Serial Number	Last Calibration Date	Next Calibration Date
*** No Calibrated Tools Used ***					

Material Used				
Part Number	Part Description	Note	Lot/Serial Number	Quantity
*** No Parts Used ***				

Labour Details			
Part Number	Part Description	Start Date	Quantity
SV000013	Preventative maintenance	29/04/2025	4

Work Complete	Customer Signature	Technician Signature
Yes ☑ No ☐		
PM/OQ/PV Left with Customer		
Yes ☐ No ☑		

Terms & Conditions

เอกสารไม่ควบคุม

MM-C39

Component List

Component / Specific Model	Serial #	Firmware Version	Configuration Notes
FIAS100	100S24040501	2.20	Syngistix V4.0.1.1935

Parts Lists

Parts Included with the PM				
Part Number (if applicable)	**Description**	**Quantity**	**Batch/Lot #**	**Expiration Date (MM/YY)**
B050 2706	Fan Filter	1	N/A	N/A

Additional Tools Required for PM				
Part Number (if applicable)	**Description**	**Quantity**	**Serial #**	**Calibration Due Date (MM/YY)**
N/A	Digital Volt Meter	1	N/A	N/A
Additional Reagents and Standards Required for PM				
Part Number (if applicable)	**Description**	**Quantity**	**Batch/Lot #**	**Expiration Date (MM/YY)**
N/A	N/A	N/A	N/A	N/A

ไอกสารไ อสา กธ

Atomic Absorption/FIAS 100/400 Preventive Maintenance (PM)			
Company Name:	United Analyst and Engineering Consultant Co., LTD.		
Address (Instrument Location):	41 Sukumvhit Rd., Phra Khanong, Bangkok 10260		
Room Number:	Lab		
Asset Number (if applicable):	2 of 2W	**Customer System ID:**	K. Yanida
Service Engineer Name:	K. Chayanan	**Service Order Number:**	WO-03051971
Date PM Performed: (DD-MMM-YYYY)	29-Apr-2025	**Next PM Due Date:** (DD-MMM-YYYY)	29-Oct-2025

Part Number	Release	Publication Date	
09370005	C	January 2013	PerkinElmer®

Scope
The purpose of this PM is to ensure the continued functionality of the Atomic Absorption/FIAS 100/400 by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer.
The customer should save their method before the PM begins.

General Instructions:
Always check with the customer before making any changes that may affect the customer's analysis or calibration.
The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer.
Update the PM sticker and instrument logbook as required.

Copyright Information
This document contains proprietary information that is protected by copyright. All rights are reserved.
No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of PerkinElmer, Inc. **Copyright © 2013 PerkinElmer, Inc.**

Trademarks
Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners.
Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.
PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

เอกสารไ อสา กธ

น.18/22

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. **General:**
   - ☑ Review the instrument performance with the customer and document any recent problems.

     _____

   - ☑ Is the Working Environment Acceptable? If not, document.

     _____

   - ☐ Visual Damage (if yes, describe)

     _____

   - ☑ Check incoming AC line voltage for proper levels and grounding.
   - ☑ Verify Voltage switch on back of instrument is correct
   - ☑ Perform general inspection of system for cleanliness. Clean if needed.
   - ☑ Gas supply cylinders secured, lines leak checked and argon or nitrogen supply pressure verified (45 – 58 psi).
   - ☑ Inspect the customer log book and make any appropriate PM entries.
   - ☑ Fan checked and filter cleaned
   - ☑ Heating mantle or Universal Cell Holder checked

2. **Instrument components**
   - ☑ Non-return valve checked/repaired/replaced if needed (B019 8111). Clean the valve if there is any liquid in it. Replace the rubber sleeve (B013 5123) if it is worn. Check the flow meter for any signs of fluid in it. Clean the flow meter if needed.
   - ☑ Verify condition of pump pressure adjustment levers (B050 7794 - look for cracks or problems with the springs), pump rollers (B300 0251 check for wear), and thumb screws (B050 7796).
   - ☑ Check the Multiport valve for proper switching, flow, and insure there are no leaks. Clean valve parts and replace o-rings if needed (large o-ring: B050 1250, small o-ring: B004 5095). Use a squirt bottle & fishing line to try to dislodge clogs.
   - ☑ Firmware Version checked. Latest is 2.20.

3. **Mixing/Separation Assembly & Pump Tubing:**
   - ☑ Mixing separator assembly checked
   - ☑ Filter/membrane checked (B050 8306)
   - ☑ Condition of the pump tubing (replace if necessary), correct pump tubing for the solutions being run. Make sure the correct magazines are being used. B050 7791 for 0.13 – 1.80 mm tubing; B050 7792 for 1.60 – 3.18 mm tubing.

เอกสารไม่ควบคุม

4. **Cell, Cell Windows, Transfer Line:**
   - ☑ Cell checked
   - ☑ Cell windows checked
   - ☑ Transfer line checked for moisture (if moisture is a problem, the Nafion dryer might be needed)

5. **Operational Tests:**
   - ☑ Run DI water through the carrier/reductant/sample system. Verify smooth flow of liquid throughout without leaks. Replace tubing & fittings if needed.

6. **Review:**
   - ☑ Review with the customer PM work performed.
   - ☑ Review with the customer routine maintenance procedures.
   - ☑ Discuss recommended customer-supplied materials to have on hand.
   - ☑ Attach PM sticker.
   - ☑ Update Logbook.

เอกสารไม่ควบคุม

MM-C39

Additional Comments

Additional Comments Regarding the PM

Review

The preventive maintenance checks and if applicable performance tests for FIAS 100/400 have been completed. ***This FIAS 100/400 Passes*** ☑ ***Fails*** ☐ ***the preventive maintenance.***	
Review of Preventive Maintenance:	
Authorized PerkinElmer Representative:	Date: 29 Apr 2025 (DD-MMM-YYYY)
Authorized Customer Representative:	Date: 29 Apr 2025 (DD-MMM-YYYY)

เอกสารไม่ควบคุม

Document History

Revision	Description of Change	Page(s)	Date
A	First release		May 2008
B	Addition of Batch/Lot Number, Expiration Date, and Report Fields.	2,7	February 2009
C	Update to new format	All	January 2013

เอกสารไม่ควบคุม

น.18/24

MM-C39

Customer Acknowledgment of receipt of the above repair / replacement.

Special Terms and Conditions: This is not an invoice.

Taxes will be applied to your invoice if applicable.

เอกสารไม่ควบคุม

น.18/25

PerkinElmer
For the Better

PerkinElmer Scientific (Thailand) Co., Ltd.
290 Soi Soonvijai 4
Khwang Bangkapi, Khet Huay Kwang
Bangkok 10310
Thailand
Tel: 66 2719 6420 ; Fax: +66 2 319 7900
http://www.perkinelmer.com

Service Report

Work Order Number	Activity Code	Billing Type	Requested Start Date	Model	Serial Number
WO-03051971	Planned Maintenance	Contract	10/03/2568 23:08 น.	B0508570	100S24040501

Service Representative Name	Contract Number	Expiry Date	Equipment ID	System ID
Kanan, Chayanan	SC-0035659090	24/05/2025	N/A	N/A

UDI Number
N/A

Equipment Location	Bill To Name
บริษัท ยูไนเต็ด แอนนาลิสต์ แอนด์ แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 51 10260 TH	บริษัท ยูไนเต็ด แอนนาลิสต์ แอนด์ แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 51 10260 TH

Customer Contact	Phone Number	Fax Number	Email	Purchase Order
K. Nichakorn แพรไหม	095-5580049	N/A	penpitcha.rt42@gmail.com	HPO-240400211

Work Description

- PM 2/2 Warranty
- Cleaning Port Vale, Manifold, Tuning
- Run Hg test ; Pass

Start Date	End Date	Work Description
29/04/2025	29/04/2025	
29/04/2025	29/04/2025	

Tools Used

Quantity	Calibrated Tool	Description	Serial Number	Last Calibration Date	Next Calibration Date
*** No Calibrated Tools Used ***					

Material Used

Part Number	Part Description	Note	Lot/Serial Number	Quantity
*** No Parts Used ***				

Labour Details

Part Number	Part Description	Start Date	Quantity
SV000013	Preventative maintenance	29/04/2025	3
SV000002	Service Travel	29/04/2025	1

Work Complete	Customer Signature	Technician Signature
Yes ☑ No ☐		
PM/OQ/IPV Left with Customer		
Yes ☐ No ☑		

Terms & Conditions

เอกสารไม่ควบคุม

MM-C39

Agilent CrossLab
From Insight to Outcome

Agilent CrossLab Start Up Services

Agilent 5100 5110 ICP-OES Preventive Maintenance

Agilent Preventive Maintenance provides factory recommended service for your analytical instruments to assure reliable operation and the accuracy of your results

Delivered by highly trained and certified service engineers using genuine Agilent parts and supplies, Agilent Preventive Maintenance provides what you need to reduce unplanned downtime and keep your systems operating at their peak performance.

This checklist is used as a guide for completing the preventive maintenance tasks. A signed copy of this checklist is provided for your records.

Revision: A.02, Issued: 21 January 2022
Document Number: G8014-90075
© Agilent Technologies, Inc. 2022

Agilent

น.18/26

เอกสารควบคุม ว่

Terms & Conditions
Customer Acknowledgment of receipt of the above repair / replacement.
Special Terms and Conditions: This is not an invoice.
Taxes will be applied to your invoice if applicable.

เอกสารไม่ควบคุม

MM-C39

Important Customer Web Links

- To access **Agilent University**, visit http://www.agilent.com/crosslab/university/ to learn about training options, which include online, classroom and onsite delivery. A training specialist can work directly with you to help determine your best options.
- To access the **Agilent Resource Center** web page, visit https://www.agilent.com/en-us/agilentresources. The following information topics are available:
  - Sample Prep and Containment
  - Chemical Standards
  - Analysis
  - Service and Support
  - Application Workflows
- The **Agilent Community** is an excellent place to get answers, collaborate with others about applications and Agilent products, and find in-depth documents and videos relevant to Agilent technologies. Visit https://community.agilent.com/welcome
- Videos about specific preparation requirements for your instrument can be found by searching the **Agilent YouTube** channel at https://www.youtube.com/user/agilent
- **Need to place a service call?** Flexible Repair Options | Agilent

© Agilent Technologies, Inc. 2022

เอกสารคุมไม่ ่ว

Agilent 5100, 5110 Preventive Maintenance Checklist

Agilent CrossLab
From Insight to Outcome

Introduction

Customer Information

- Customers should provide all necessary operating supplies upon request of the engineer.
- A customer representative should be available to the engineer while performing the preventive maintenance procedures. Customers are responsible for regular maintenance and are encouraged to observe the service representative.
- Any parts not included in the Parts Lists section of this document are not part of the recommended Preventive Maintenance service nor are they included in the price of this service.
- If a system requires the use of extra or special procedures and/or parts for the maintenance service, then these must be ordered separately and charged as a repair, which may incur additional costs.
- For customers using HF applications, the instrument should be returned to its standard sample introduction system.

Revision: A.02, Issued: 21 January 2022
Document Number: G8014-90075
© Agilent Technologies, Inc. 2022

เอกสารคุมไม่ ่ว

น.18/27

MM-C39

Instrument Maintenance

System Information

☐ Check this box if an instrument configuration report is attached instead of completing the table.

Instrument System Name and ID	5110 VDV ICP-OES
Instrument System Site and Location	UAE Consultant

	List System Component Product Numbers	**List the Serial Numbers of each Component**
1.	G 8015 A	MY 18030001
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

ICP-OES Configuration Table	**Circle the type or write in the type if other**
Nebulizer Type	(SeaSpray) OneNeb | Conikal | Other
Spray Chamber	Cyclonic Single Pass (Cyclonic Double Pass) Other
Torch	Radial (Dual View) Other
Torch Type	One Piece (Semi Demountable) Fully Demountable | Other
Injector Diameter	2.4mm (1.8mm) 1.4mm | 0.8mm | Other
Injector Material	(Quartz) Ceramic | Other

© Agilent Technologies, Inc. 2022

เอกสารควบคุม ว่

Service Engineer's Responsibilities

- Contact the customer and ensure that all necessary supplies are available before the preventive maintenance visit.
- Only select those pages that relate to the system or module being serviced.
- Complete empty fields with the relevant information.
- Complete the relevant checkboxes in the checklist using either a "**X**" or tick mark "✓".
- Check **"Service not applicable"** check boxes to indicate services/tasks not delivered, as appropriate.
- Complete the Preventive Maintenance services in the most logical order relevant to the individual system service in the order of the tasks listed.
- Complete the **Service Review** section together with the customer.
- Complete the fields for page numbers at the foot of each selected page
- Add relevant page numbers to selected pages and complete the total number of pages field in the Service Completion section
- **Ask the customer to sign the Service Verification section including the customer's and your signature.**

© Agilent Technologies, Inc. 2022

เอกสารควบคุม ว่

น.18/28

Preventive Maintenance Procedures

Record Pre-PM instrument performance

- [x] Run Instrument Performance test.
- [x] Record results in Instrument Performance Test Results Table – Pre-PM.

Clean and inspect ICP-OES system

- [x] Look for any obvious external damage or problems.
- [x] Inspect water cooling hoses, gas lines and power cord for excessive wear or damage.
- [x] Perform a general internal inspection of the system for excessive dust accumulation, clean if necessary.
- [x] Inspect sample introduction components and record any required maintenance in the Service Engineer Comments and notify the customer as the required actions required.
- [x] Record the instrument operating conditions in the ICP-OES Status Results Table.
- [x] Replace the polychromator purge filter.
- [x] Replace the radial pre-optics window
- [x] Replace the axial pre-optics window for SVDV and VDV instruments.
- [x] Check exhaust flow for the correct positive extraction at the exhaust duct to insure they meet minimum specifications.
- [x] Replace air inlet dust filter.
- [ ] Replace high capacity air inlet dust filter element if installed. N/A
- [x] Remove and clean instrument water inlet filter.

Agilent Water Recirculator

- [ ] **Service not applicable**
- [x] Drain cooling fluid and remove any particles from the chiller reservoir
- [x] Remove, clean and reinstall water inlet metal mesh filter if present.
- [x] Re fill with Agilent Cool Clear cooling fluid.
- [x] Clean the cooling system Air filter and the condenser.

© Agilent Technologies, Inc. 2022

เอกสารควบคุม ว่

Preparation

- [x] Discuss any specific issues with the customer before starting.
- [x] Review the instrument logbook for recorded problems and comments.
- [x] Save instrument control settings before starting the procedure.
- [x] Perform a general inspection of the system for cleanliness.
- [x] Check for proper installation of parts, assemblies, sensors etc.
- [x] Check system for required installation of components and implementation of Service Notes
- [x] Check for required firmware/software updates and verify with customers if they would like them installed.
- [ ] For HF application systems, if standard sample introduction system was not installed, ask the customer to install it. N/A
- [x] Ask the customer to remove any samples from the ICP-OES sample introduction area, auto sampler or around the ICP-OES.

© Agilent Technologies, Inc. 2022

เอกสารควบคุม ว่

ICP-OES adjustment

- ☑ Check position of Zn peak, adjust if required.
- ☑ Check Argon Ratio, adjust to specified value if required.
- ☑ Perform Detector Calibration.
- ☑ Perform Instrument Calibration.

Record Post-PM instrument performance

- ☑ Run Instrument Performance test.
- ☑ Record results in Instrument Performance Test Results Table - Post PM.
- ☑ For systems using ICP Expert version 7.3 and above, run the following Instrument tests
  - ☑ Subsystem Communications Test
  - ☑ Air Flow
  - ☑ Water Flow
  - ☑ Gas Flows
  - ☑ RF Generator
  - ☑ Camera Test
  - ☑ Optics Test
  - ☑ Nebulizer Test
- ☑ Record the result in the Instrument Test Results Table

© Agilent Technologies, Inc. 2022

เอกสารควบคุม ไม่ ว่

SPS 3 Auto Sampler

- ☑ **Service not applicable**
- ☐ Power cycle the autosampler and verify successful initialization.
- ☐ Inspect X and Z axis belts for wear. Replace is necessary.
- ☐ Clean X and Z axis slide shafts.
- ☐ Using customer's racks and the Agilent software move the sample probe to the 4 outermost corners and rinse port, ensure that the probe is approximately centered in the vial.

SPS 4 Auto sampler

- ☑ **Service not applicable**
- ☐ Clean the spill tray, rack location mat, end frames and chassis with a damp soft cloth and diluted mild detergent.
- ☐ Clean the auto sampler cover panels, if cover kit is installed, with domestic window cleaner.
- ☐ Check the X-axis and Z-axis drive belts for cracks, splits, damaged teeth, excessive fraying, color changes or degradation from fumes.
- ☐ Check the X-axis, Theta-axis and Z-axis FFC cables for cracks, incorrect positioning, damaged edges or damaged connectors.
- ☐ Pump Tubing Replacement. Replace peristaltic pump tubing. Replace all tubing that goes from the rinse station to the pump and from the pump to the waste/rinse bottles
- ☐ Test using customer's tray and move the sample probe to the sample vial 1, wash vial and rinse port and ensure that the probe is centered in the vial. If not use calibration wizard and calibrate the position.

AVS 4, 6, 7 Advanced Valve System

- ☑ **Service not applicable**
- ☐ Replace valve rotor seal
- ☐ Check fittings for signs of leaks
- ☐ Check tubing including autosampler tubing for kinks or excessive wear
- ☐ Check high flow pump for signs of leaks

© Agilent Technologies, Inc. 2022

เอกสารควบคุม ไม่ ว่

Test Results

Instrument Performance Test Results Table

Note: These measurements do not form part of any specification and are for reference only.

	Pre PM Sensitivity Check		Post PM Sensitivity Check	
	Radial	Axial *	Radial	Axial*
Zn 213.857 nm SRBR	1783.8	2579.2	2230.8	3562.9
Mn 257.610 nm SRBR	94870.5	196149	108830	178844
Al 396.152 nm SBR	5.2	8.0	7.0	7.4
K 766.491 nm SBR	3.0	14.6	3.4	8.7

* Axial result is not applicable for G8016AA, G8012AA Radial View instruments.

Instrument Test Results Table

Note: The Instrument Test results are for systems using ICP Expert version 7.3 and above only.

Instrument Test	Result
Subsystem Communications Test	Pass
Air Flow	Pass
Water Flow	Pass
Gas Flows	Pass
RF Generator	Pass
Camera Test	Pass
Optics Test	Pass
Nebulizer test	Pass

© Agilent Technologies, Inc. 2022

เอกสารควบคุม ว่

Restore Instrument

- ☐ For HF applications, ask the customer to reinstall their sample introduction system. N/A
- ☑ Leave system in an idle state: on and purging.
- ☑ Guidance: If the PM service is performed prior to a qualification service, then use the qualification procedure as a guide for final instrument set up and checkout.

Service Review

- ☑ Attach available reports/printouts of all tests to this documentation.
- ☑ Record the Preventive Maintenance service activity in the customer's records/logbook.
- ☑ Record the PM event in the Smart Alerts logbook, if applicable.
- ☑ Update/reset instrument maintenance counters as appropriate.
- ☑ Affix the PM sticker to the system or instrument logbook based on the customer's request.
- ☑ Complete the Service Engineer Comments section if there are additional comments.
- ☑ Review this service, parts replaced, and test results obtained with the customer.
- ☑ If the instrument firmware was updated, record the details of the change in the Service Engineer's Comments box. Systems in a compliant environment may need additional documentation.
- ☑ **Complete the Signature Page with both Service Engineer and Customer signatures.**

© Agilent Technologies, Inc. 2022

เอกสารควบคุม ว่

Consumed PM Parts

Part Description	Part Number	Product or Model# where used	Quantity consumed
Axial Pre-Optic Window	G8010-68014	G8010A, G8011A, G8014A/G8015A	1
Radial Pre-Optic Window	G8010-68015	All	1
Agilent Cool Clear Coolant Fluid	5799-0037	Agilent Water Recirculator	–
Purge Gas Filter	G8010-60136	All	1
Air inlet filter	G8000-68002	All	1
High Capacity Air Filter	G8010-60189	Optional	–
Rotor seal for 6-7 port valve for AVS6/7	G8494-60002	G8494A/G8495	–
Rotor seal for 4 port valve for AVS4	G8493-60002	G8493A	–
Rinse solution to rinse station 2.5mm id x 1m	G8410-80123	SPS 4	–
Barb connector 2.5mm-1.5mm ID	G8410-80124	SPS 4	–
PVC waste tubing,8mm od x 5mm id, 2m	G8410-80122	SPS 4	–
Additional Parts may be required from engineer's stock:			
X axis drive belt	5410047500	SPS 3	–
Z axis drive belt	5410047400	SPS 3	–
Peristaltic pump tubing, PVC SolvaFlex, 3 bridged,	3710049000	SPS 4	–

Consumed Parts Reference
(Purchased by customer, not included as part of PM)

☑ Section Not Applicable.

Part Description	Part Number	Product or Model# where used	Quantity consumed

© Agilent Technologies, Inc. 2022

เอกสารควบคุม ไม่ ว่

ICP-OES Status Results Table

Note: These measurements do not form part of any specification and are for reference only.

Measurement	Standby Mode		Plasma On	
Mains Voltage	231.288	VAC	226.380	VAC
Mains Current	0.083	A	0.100	A
Instrument Temperature	21.1	°C	21.6	°C
RF Air Flow (sensor speed)	44.0	Hz	41.1	Hz
Plasma Exhaust Temperature	No measurement		47.1	°C
Water Flow Oscillator	No measurement		1.14	L/min
Water Flow Detector	0.92	L/min	0.90	L/min
Water Inlet Temperature	19.5	°C	18.5	°C
Polychromator Temperature	35.4	°C	35.4	°C
CCD Temperature	-40.1	°C	-39.9	°C
Thermal Stabilizer	35.0	°C	35.0	°C
Argon Supply Pressure	634.43	kPa	583.77	kPa
Purge Gas Supply Pressure*1	631.28	kPa	604.02	kPa
Option Gas Supply Pressure*1	–	kPa	–	kPa
Nebulizer Flow	No measurement		0.70	L/min
Nebulizer Back Pressure	No measurement		273.61	kPa
Plasma Gas Flow	No measurement		1196	L/min
Auxiliary Gas Flow	No measurement		1.00	L/min
RF Power	No measurement		1200.4	W
RF Supply Current	No measurement		8.228	A
RF Supply Voltage	No measurement		194.529	V

*1 If option installed

© Agilent Technologies, Inc. 2022

เอกสารควบคุม ไม่ ว่

Report Summary

Instrument Model	Agilent 5100/5110 VDV ICP-OES
Instrument ID	G8011A/G8015A
Instrument Serial Number	MY18030001
Software Version	7.3.1.9507
Firmware Version	3442
Tested By	Burin 5nd test final
Test Completed On	11/19/2025 2:14:28 PM

Result Summary

Subsystem Communications Test	Pass
Air Flow Test	Skipped
Water Flow Test	Skipped
Gas Flows Test	Skipped
RF Generator Test	Skipped
Camera Test	Skipped
Optics Test	Skipped
Advanced Valve System Test	Skipped
Resolution Test	Pass
Sensitivity Test	Pass
Precision Test	Pass

Subsystem Communications Test **Pass**

Signature Page

Service Engineer Comments (optional)

If there are any specific points you wish to note as part of performing the installation or other items of interest for the customer, please write in this box.

Service Verification

Service Request Number:
6008006610

Service Engineer Name:
Worawit T.

Service Engineer Signature:
Worawit T.

Total number of pages in this document:
14

Date Service Completed:
3 Nov 2025

Customer Name:
Aphorn O.

Customer Signature:
Aphorn O.

Revision: A.02, Issued: 21 January 2022
Document Number: G8014-90075
© Agilent Technologies, Inc. 2022

Agilent

เอกสารคุมไ่ ว่

MM-C39

Sensitivity Test — **Pass**

Radial

Element Wavelength	Specification	Method	Ratio	Standard	Blank
As (188.980 nm)	≥ 46.0	SRBR	96.4	735.7	50.5
Se (196.026 nm)	≥ 41.0	SRBR	79.6	779.2	77.7
Zn (213.857 nm)	≥ 1421.0	SRBR	2270.3	24005.6	110.8
Pb (220.353 nm)	≥ 46.0	SRBR	129.5	1701.5	144.5
Mn (257.610 nm)	≥ 3518.0	SRBR	9810.6	233072.5	561.7
Al (396.152 nm)	≥ 3.4	SBR	6.5	36392.0	4836.0
Ba (493.408 nm)	≥ 34.0	SBR	93.1	1586633.9	16860.6
K (766.491 nm)	≥ 1.8	SBR	1.9	54511.9	19124.8

Axial

Element Wavelength	Specification	Method	Ratio	Standard	Blank
As (188.980 nm)	≥ 208.0	SRBR	245.0	3080.3	143.7
Se (196.026 nm)	≥ 159.0	SRBR	211.9	3471.4	233.5
Zn (206.200 nm)	≥ 234.0	SRBR	771.1	8797.9	126.5
Zn (213.857 nm)	≥ 1743.0	SRBR	6307.2	120003.6	359.8
Cd (214.439 nm)	≥ 4227.0	SRBR	6012.4	96451.0	256.0
Pb (220.353 nm)	≥ 320.0	SRBR	571.2	12760.9	463.5
Mn (257.610 nm)	≥ 10625.0	SRBR	39386.8	1701779.7	1862.7
Cr (267.716 nm)	≥ 1048.0	SRBR	5192.7	206938.5	1564.3
Cu (324.754 nm)	≥ 19.0	SBR	49.4	261983.3	5202.7
Al (396.152 nm)	≥ 6.0	SBR	20.3	318135.9	14932.2
Ba (493.408 nm)	≥ 60.0	SBR	255.9	13403057.9	52173.2
K (766.491 nm)	≥ 24.0	SBR	38.7	1918325.2	48283.1

Resolution Test — **Pass**

Element Wavelength	Specification	Width
N (174.213 nm)	≤ 9.40	6.66
As (188.980 nm)	≤ 8.20	6.00
C (193.027 nm)	≤ 11.50	7.94
Mo (202.032 nm)	≤ 8.20	6.15
Cr (206.158 nm)	≤ 13.40	8.80
Zn (213.857 nm)	≤ 8.70	6.60
Pb (220.353 nm)	≤ 9.50	7.07
Co (228.615 nm)	≤ 17.20	10.73
Ba (230.424 nm)	≤ 9.40	6.85
Mn (257.610 nm)	≤ 13.30	9.20
Mn (260.568 nm)	≤ 20.30	13.82
Cr (267.716 nm)	≤ 11.00	7.99
Cu (324.754 nm)	≤ 25.00	17.85
Cu (327.395 nm)	≤ 14.20	11.44
Sr (338.071 nm)	≤ 33.50	24.20
Ba (455.403 nm)	≤ 44.00	33.83
Sr (460.733 nm)	≤ 36.00	18.28
Ba (493.408 nm)	≤ 36.00	24.97
Ba (614.171 nm)	≤ 42.00	29.36
Ar (675.283 nm)	≤ 74.00	57.75
K (766.491 nm)	≤ 80.00	73.92

MM-C39

SITHIPORN associates

DMA-80 DIRECT MERCURY ANALYZER System



SITHIPORN ASSOCIATES CO.,LTD.
451-451/1 Sirinthorn Road, Bangbumru,Bangplud, Bangkok 10700 Thailand
Tel. (662) 433-8331, 434-9191 fax: (662) 433-1679,434-9510

เอกสารควบคุม

น.18/35

Precision Test **Pass**

Radial

Element Wavelength	Specification	Measured Value % RSD
As (188.980 nm)	≤ 2.60	1.32
Se (196.026 nm)	≤ 2.60	0.81
Zn (213.857 nm)	≤ 1.50	0.25
Pb (220.353 nm)	≤ 2.60	0.78
Mn (257.610 nm)	≤ 1.50	0.28
Al (396.152 nm)	≤ 1.50	0.31
Ba (493.408 nm)	≤ 1.50	0.28
K (766.491 nm)	≤ 1.50	0.19

Axial

Element Wavelength	Specification	Measured Value % RSD
As (188.980 nm)	≤ 1.50	0.61
Se (196.026 nm)	≤ 1.50	0.72
Zn (206.200 nm)	≤ 1.50	0.37
Zn (213.857 nm)	≤ 1.50	0.32
Cd (214.439 nm)	≤ 1.50	0.31
Pb (220.353 nm)	≤ 1.50	0.37
Mn (257.610 nm)	≤ 1.50	0.69
Cr (267.716 nm)	≤ 1.50	0.35
Cu (324.754 nm)	≤ 1.50	0.49
Al (396.152 nm)	≤ 1.50	0.49
Ba (493.408 nm)	≤ 1.50	0.73
K (766.491 nm)	≤ 1.50	0.31

DMA-80 Direct Mercury Analyzer

SERVICE PROTOCOL REPORT

To be filled in before service visit (1st page)

Customer information:

Company:	บ.ยูไนเต็ด แอนนาลิสต์ฯ จก. (สนง.ใหญ่)
Department:	LAB
Person in charge:	φ JWo A› ;Q Ui PkA Y Q s \ k _ d i w U
Address:	B dY doK41X M ΘPa Θ c8ZXo^>ksNN U10260i P ; Z
Tel.:	+66 (86) 3191292
E-mail:	bhuchonk@uaeconsultant.co.th

Technical data:

Unit Serial Number:	**24114043**	
Terminal type or USB-640 Gateway:	Termianl-660	SN 24107843
Software, type and revision:	Easy Control	Rev. 03-F-SP1(2023-09-20)
Air Compressor (if present)	95100	SN 12236761
Gas system pump (if present)	-	SN -
Installation and last maintenance dates:	Inst. on: 31/01/2025	Maint. on:

NOTE: after achievement of the following protocol a filled and signed copy of this report has to be sent to Milestone srl at: service@milestonesrl.com

For the best result of the test below we recommended to use the Milestone DMA-80 Service Kit (PN DMA-SKIT).

เอกสารควบคุม ไ่ ว่

1. VISUAL INSPECTION

	Good	Damaged	Corroded/Dirty
External chassis	√		
Inside	√		
Electric parts	√		
Screws	√		

2. ELECTRICAL SAFETY TEST


Using a suitable testing device check the below reported parameters and take note of the results.

Parameter	Result	OK	Not OK
Voltage : 230 VAC (±10%)	Actual value : 223 VAC	√	
Ground : ≤ 2	Actual value: 0.8 VAC	√	

3. PRESSURE CHECK

	Oxygen (purity O_2>99,95%)		Milestone air compressor
Gas carrier		Purity: -	√

The pressure at the supply source manometer should be approx. 4.0bar
The flow rate depends by type of cuvette installed on the DMA-80 unit.


	Correct value	Actual value	Final value	Correct value	Actual value	Final value	Correct value	Actual value	Final value
Inlet pressure	3.1 bar	-	-	3.1 bar	-	-	3.1 bar	3.1 bar	Pass
Flow rate	10-12 l/h	-	-	8-10 l/h	-	-	6-8 l/h	8 l/h	Pass

Check all possible leakage points and their conditions:


	Good	Damaged	Corroded
Tubing	√		
Silicon joints	√		
O-rings	√		
Cuvette sealing O-rings	√		
Gas connections	√		
Valves	√		
Sample boat carrier	√		
Catalyst flange	√		

เอกสารควบคุม ไ่ ว่

				
Amalgamator stand by temperature	If controlled by Infrared sensor	170°C ± 10°C	170°C	Pass
	If IR sensor is not present	145°C ± 25°C	-	-
Amalgamator heating temperature	850°C ± 10°C		850°C	Pass
Cuvette	125°C ± 5°C		125°C	Pass

7. SPECTROMETER

The spectrometer can be equipped with a single beam system (ducon lamp) or with a dual beam system (tricon lamp)

	Old cuvette type						Actual cuvette type					
												
	Gain			Offset			Gain			Offset		
	Correct value	Actual value	Final value	Correct value	Actual value	Final value	Correct value	Actual value	Final value	Correct value	Actual value	Final value
Dualcell system	3,6VDC	-	-	0,015VDC ± 0,005VDC	-	-	3,93VDC	3.9V	Pass	0,015VDC ± 0,005VDC	0.015V	Pass
Tricell system*	-	-	-	-	-	-	3,96VDC	-	-	0,015VDC ± 0,005VDC	-	-

(*)The recommended Hg lamp operating signal should be around 3,96VDC (for detector 2) and 3,93VDC (for detector 1).

เอกสารควบคุม ว่

4. AUTOSAMPLER SYSTEM

	OK	Not OK	Re-Adjusted
Calibration of autosampler motor	√		
Cylinders alignment	√		

	Fast	Slow	Normal
Speed of pneumatic cylinders			√

Using the maintenance grease, periodically lightly lubricate all exposed steel rods of the horizontal and vertical cylinders.

5. COMPONENTS CHECK

Conditions of the different parts used/installed on DMA unit:

	OK	Not OK	Replaced	Cleaned
Catalyst tube			√	
Amalgamator	√			
Quartz boats	√			
Nickel boats	-			
Autosampler plate	√			
Gas kit accessories	-			

6. TEMPERATURES


	Correct value		Actual value	Final value (Pass)
Drying/ Decomposition furnace	If controlled by Infrared sensor	850°C ± 10°C	-	-
	If controlled by thermocouple	650°C ± 10°C	650	Pass
Catalyst furnace	Type 1 	515°C ± 5°C	-	-
	Type 2,3	565°C ±10°C	565°C	Pass

เอกสารควบคุม ว่

10. TESTING PROCEDURE

It consists to run some measurements for the evaluation of the analytical performance of the unit, like: absorbance, peaks shape, temperatures, lamp signal and verify the proper working of whole system.

1) Run minimum 2 blanks on the same sample boat (quartz if possible) in manner to clean it
2) Run blanks until absorbance value (Height) decrease under 0.0030 in cell 1
3) Set a fresh and stabilized 100µg/L Hg standard according to the prescriptions reported on the DMA80 User Manual. The quality of the used standard is fundamental for the success of the entire procedure
4) Weight approximately 100µg of the fresh 100µg/L – Standard (10ng) and start the analysis as a single measurement mode
5) Repeat five times the test
6) Run again two blanks measurements

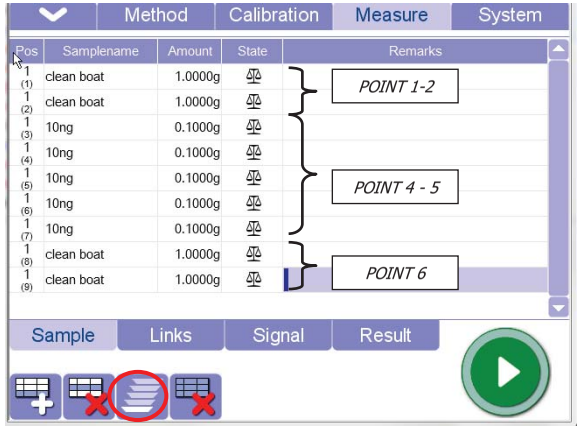

Now, it is possible to evaluate:

- Peaks

เอกสารควบคุม ไม่ ว่

	OK	Not OK
Conditions of the spectrometer system	√	
Alignment between lamp, cuvette and detector	√	
Cuvette cleaning (glass windows, sealing O-rings…)	√	
Lamp intensity	√	
Operation of the mechanical shutter (if present)	√	


8. MILESTONE AIR COMPRESSOR

Maintenance	OK	Date last service
Drain (compressor)	√	
Replacing air filters (air purification module)	√	
Check sealing connections	√	

9. PARTS TO BE REPLACED

PN	DESCRIPTION	Replaced	Not Replaced
DMA8133	Catalyst tube: 6 months if the unit runs daily, 1 year if the unit is used rarely. *In case of analyse of sample with high organic concentration the lifetime of the catalyst can be less than 6 months.*		√
DMA8134	Amalgamator: 6 months if the unit runs daily 1 year if the unit is used rarely		√
DMA8195A	Hg lamp tri-cell (model 2011): 5 years		√
DMA8137	Hg lamp dual-cell: 5 years	-	-
70200	Hg trap 1 year		√
DMA8058/B	Amalgamator coil 6 months/1 year or as soon as the heating is not more homogeneous		√
DMA8142	Nickel sample boats (set of 40pcs) 2 years if strongly used, replace after 1 year	-	-
DMA8347	Quartz sample boats (set of 10pcs) 2/3 years		√
DMA8335	Metal sample boat carrier 2 years		√
SL0108	PU-tube diam. 6/4 mm for internal O_2/air supply 2 years		√
SO0376D	Heating coil for drying/decomposition 2 years		√

เอกสารควบคุม ไม่ ว่

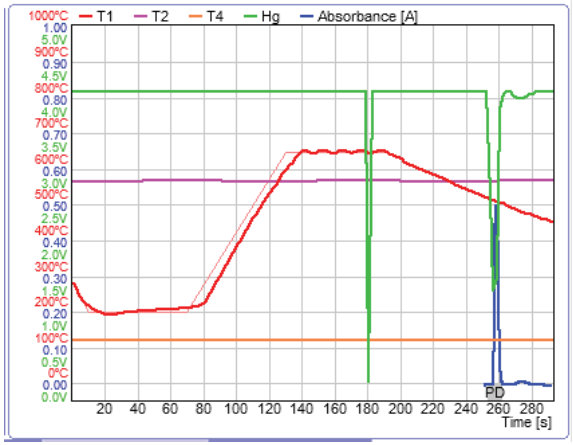


- The Hg lamp signal must be between 3.8 and 4.5V and stable. A few minutes after the start of the analysis the lamp does switch off because of the zero detection but then it instantly returns to the original condition. In case of Tricell configuration two green colour graphics are reported. After the zero shuttering the time necessary to return to full signal is longer on Tricell compare to Ducon lamp.
- During the run the catalyst oven temperature must be stable around to 565°C or 515°C.
- The drying and ashing furnace must be follow the set temperature method.
- During the run the Amalgamator furnace temperature must be stable at the stand by temperature (170°C or 145°C). Then at the release step it must raise up to 850/900°C.
- The Cuvette temperature must be stable at approximately 125°C.
- The Hg absorbance peaks must be correctly detected and reported.

11. FINAL REPORT

All screws inserted and tightened	√
All tubing sealing connections checked, cleaned or replaced and tightened	√
All heating elements are working	√
Sensors installed, checked and tightened	√
Safety devices (thermo switch) fully checked	√
All cooling fans are functioning	√
Testing procedure successfully passed	√
Necessary tools available at customer's site	√
Last revision of User Manual available at customer's site	√
Advised customer about care and maintenance instructions	√

เอกสารควบคุม ๆ ว

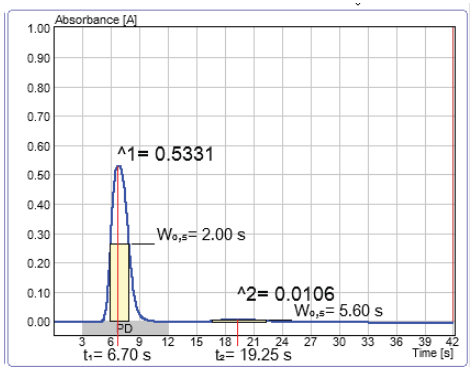

- The shape of the peak must be regular.
- The distance between Peak Cell 1 and Peak Cell 2 must be between 11 to 15 seconds.

- Results

Pos	Samplename	Amount	State	Height	Hg [ng]	[µg/kg]	Cal-Factor	Σ
- (7)	Stability10ng		M			100.290 0.92%	1.0000	
1 (8)	Stability10ng	0.1000g	✔	0.4931	9.9095	99.0951	1.0000	Σ
2 (9)	Stability10ng	0.1000g	✔	0.4965	9.9934	99.9335	1.0000	Σ
3 (10)	Stability10ng	0.1000g	✔	0.4991	10.059	100.597	1.0000	Σ
4 (11)	Stability10ng	0.1000g	✔	0.4976	10.022	100.221	1.0000	Σ
5 (12)	Stability10ng	0.1000g	✔	0.5031	10.160	101.602	1.0000	Σ

- The obtained absorbance (height) must be > 0.42 in cell 1 for each 100ppb analysis (0.22 with cuvette installed until December 2005, DMA s/n 05120292.)
- The relative standard deviation (rsd) is < 3 %.
- After two blanks (after 10ng measurements), the absorbance is < 0.0030 in cell 1(*).

(*) This condition is valid only in case the unit has: catalyst and amalgamator new, conditioned and never use before, sample boat carrier new and/or perfectly cleaned, catalyst flange new and/or perfectly cleaned, cuvette new and/or perfectly cleaned, tubes, silicon joints and o-rings replaced. Otherwise other blanks (more than 2) might be necessary.

- Temperatures & signal profiles

เอกสารควบคุม ๆ ว

สุขสาหกรรมพัฒนามูลนิธิเพื่อสถาบันอาหาร
ศูนย์บริการห้องปฏิบัติการสุขสาหกรรมอาหาร
national food institute ministry of industry
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

Verification Certificate

Certificate No.: 2501440-001-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakhanong, Bangkok 10260

Equipment: Digestion Unit (Heating Block)
Manufacturer: FOSS
Model: Tecator Digestor 2520
Serial No.: 91905060
ID No.: UAE.WAS.030/2566
Order No.: 2501440
Operation No.: 2501440-001
Date of Receipt: 27 January 2025
Date of Calibration: 27 January 2025

Calibrated by Scientist

Approved by Manager, Division of Calibration Laboratory
Responsible for the Technical Management Team

Date of Issue: 29 January 2025

The uncertainties are for a confidence probability of approximately 95 %.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่เรือ เขตบางพลัด กรุงเทพมหานคร 10700
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel. +66(0) 2422 8688 Fax +66(0) 2422 8545
nfi.or.th

เอกสารควบคุม ว่

Remarks:

Working hours of Service Engineer	

Service Engineer Name	Signature	Date
ชนม์เฉลิม วิลัยศรี	A EK Qs@\k X ^ k \ h Y _ Z	31-01-2025

Laboratory Manager / Operator acceptance signature:	

เอกสารควบคุม ว่

สถาบันอุตสาหกรรมพัฒนามูลนิธิเพื่อสถาบันอาหาร
ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
national food institute ministry of industry
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

Verification Report

Certificate No.: 2501440-001-01

Equipment: Digestion Unit (Heating Block)

Model: Tecator Digestor 2520 Serial No.: 91905060

Resolution: 1 °C ID No : UAE.WAS.030/2566

Manufacturer: FOSS

Date of Calibration: 27 January 2025

Calibration point: 380 °C

Calibration result:

Table1 : Reporting of Temperature

Block No.	UUC* Setting (°C)	UUC* Reading (°C)	Stability (±°C)	Standard Thermometer (°C)	Uncertainty (±°C)
1	380	380	0.22	377.84	2.0
2	380	380	0.19	378.68	2.0
3	380	380	0.13	378.70	2.0
4	380	380	0.12	379.82	2.0
5	380	380	0.20	381.01	2.0
6	380	380	0.16	380.48	2.0
7	380	380	0.16	378.22	2.0
8	380	380	0.19	377.99	2.0
9	380	380	0.09	378.48	2.0
10	380	380	0.15	378.17	2.0
11	380	380	0.18	377.64	2.0
12	380	380	0.11	379.27	2.0
13	380	380	0.13	378.14	2.0
14	380	380	0.25	379.11	2.0
15	380	380	0.15	379.83	2.0
16	380	380	0.18	378.05	2.0
17	380	380	0.31	378.44	2.0
18	380	380	0.18	378.29	2.0
19	380	380	0.17	378.41	2.0
20	380	380	0.13	379.24	2.0

Note:

- UUC* = Unit Under Calibration
- Immersion depth of standard thermometer in tube level high of sand is equal heater plate of UUC.
- Stability = One-half of the greatest maximum difference of measured temperatures at one sensors, for at least half an hour after reaching steady state.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor $k = 2$, providing a level of confidence of approximately 95 %.

2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพมหานคร 10700
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel +66(0) 2422 8688 Fax +66(0) 2422 8545
nfi.or.th

เอกสารควบคุม ที่

สถาบันอุตสาหกรรมพัฒนามูลนิธิเพื่อสถาบันอาหาร
ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
national food institute ministry of industry
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

Verification Report

Certificate No.: 2501440-001-01

Equipment: Digestion Unit (Heating Block)

Model: Tecator Digestor 2520 Serial No.: 91905060

Resolution: 1 °C ID No : UAE.WAS.030/2566

Manufacturer: FOSS

Date of Calibration: 27 January 2025

Location: Dry Laboratory (312), UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.

Environment Condition:
Ambient Temperature (29 ± 1) °C
Relative Humidity (58 ± 2) %
Line Voltage (224 ± 1) Volt

Condition of this results of Calibration:

1. This instrument was calibrated by insert standard thermocuples type R into its Digestion blocks and Calibration according to NFI Method W-TE-026 based on BS 4309 : 1968
   - The temperature scale used was based on ITS - 90 .
   - All data show below were final values and the initial data may be obtained upon request.
2. Reference Standard Instrument :

Instrument	Model	Serial No.	Certificate No.	Due Date	Through
Digital Thermometer with Thermocouple	34970A	MY44045576/MY41194453	TC24/0063	5-Jun-2025	N.M. Technical Center Laboratory
	Type R	S/CH1, R/CH2, R/CH3			

3. This certificate is traceable to International System of Units (SI Units).
4. This certificate was certified only for the instrument we calibrated.
5. This result of calibration was found accurate as shown on date and place of calibration only.
6. Condition of Calibrated item : Good
   UUC* Description
   Time of Record 1 Hour 6 Minute At 380 °C
7. Result of Calibration : [X] Without adjustment [ ] After adjustment

2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพมหานคร 10700
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel +66(0) 2422 8688 Fax +66(0) 2422 8545
nfi.or.th
เอกสารควบคุม ที่

MM-C39

FOSS

FOSS South East Asia
3388 Sirinrat Building, 25th – 26th Floor, Unit No. 3388/90,
Rama IV Road, Klongton , Klongtoey, Bangkok, Thailand 10110

Customer Service Report

Report No.:	13851

Date:	25 February 2025	Customer:	UAE
Job No.:	11732	Address:	BANGKOK
Instrument:	KTG Distillator	Serial:	91905393

	Travel To Customer (Hrs)		Labour (Hrs)		Travel From Customer (Hrs)	
Start	07:00	2hrs	09:00-17:00		17:00	2hrs
Finish	09:00		13:00-16:00		21:00	

Job Type

Application		Special		Standard			
Distributor	x	Courtesy Visit	x	Installation	x	Training	x
Digital Service	x	PMA Onboarding	x	Quote	x	In House	x
Internal	x	Warranty	x	Repair	x	PM	X
Investigate	x	Sales Support	x	Remote	x	Health Check Visit	x

PMA Type						
	Smartcare	x	Smartcare Pro	x	Fosscare	X
	Smartcare Advance	x	Fosscare Pro	x	N/A	x

Details of Work / Test

PM KTG 12MO

- test before PM
- cleaning KTG, Steamgth
- flushing Alkali pump
- Replace PM kit 12 MO
- test operation
  - dilution 80 = 85 mL cal to 80 mL
  - distillation 5 min 150-170 mL
  - Alkali 50 = 50 mL
  - *Recivur not use it
- all pass

Instrument Ready for Use	OK	X	Not OK*	

Part No:	Batch	Description	Qty
60100196	09.12.2024	PM kit kjeltec 9 Distillator	1

I confirm this report is accurate and complete

Signed FOSS		Signed Customer	
Name		Name	
Email:		Customer Contact.:	

*Remark:

Please scan QR code

เอกสารควบคุม ๆ

9.18/42


nfi national food institute ministry of industry
สถาบันอาหาร กระทรวงอุตสาหกรรม
ศูนย์บริการห้องปฏิบัติการสถาบันอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

Verification Report

Certificate No.:	2501440-001-01
Equipment:	Digestion Unit (Heating Block)
	Model: Tecator Digestor ; Serial No.: 91905060
	Resolution: 1 °C ID No.: UAE.WAS.030/2566
	Manufacturer: FOSS
Date of Calibration:	27 January 2025

Calibration point:	380 °C
Calibration result:	Continued

Figure 1. Location of Reference Standard and Block Diagram of Digestion Unit

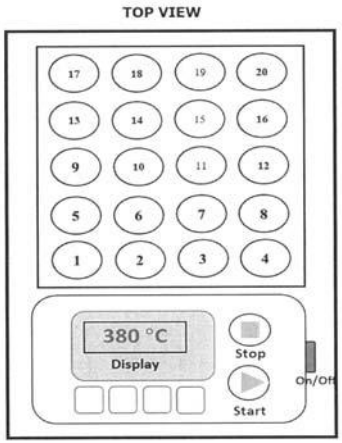

Sensor Installation Location

--------- End ---------

2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพมหานคร 10700
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel +66(0) 2422 8688 Fax +66(0) 2422 8545
nfi.or.th

เอกสารควบคุม ๆ

nfi national food institute ministry of industry
อุตสาหกรรมพัฒนามูลนิธิเพื่อสถาบันอาหาร
ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

ilac-MRA

NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Report

Certificate No.: 2502229-001-01

Equipment: CHAMBER (Incubator)
Model: IPP 260 Serial No.: V615.0187
Resolution: 0.1 °C ID No.: UAE.MIC.003/2559
Manufacturer: MEMMERT

Date of Calibration: 19 March 2025

Location: LABORATORY, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.

Environment Condition:
Ambient Temperature (16.2 ± 1) °C
Relative Humidity (32 ± 4) %
Line Voltage (223 ± 3) Volt

Condition of this results of Calibration:

1. This instrument was calibrated by insert 9 standard thermometer into its chamber and calibration according to W-TE-014 Based on TLAS G-20-1/02-08 (E): Guidelines for Calibration and Checks of Temperature Controlled Enclosures.
   - The temperature scale used was based on ITS - 90.
   - All data show below were final values and the initial data may be obtained upon request.
2. Reference Standard Instrument :

Instrument	Model	Serial No./ID No.	Certificate No.	Due Date	Through
Digital Thermometer with sensor	34972A	MY49016851	TE 670477-01	4 May 2025	NATIONAL FOOD INSTITUTE
	RTD	CH#101-109/ RTD#101-109			

3. This certificate is traceable to International System of Units (SI Units).
4. This certificate was certified only for the instrument we calibrated.
5. This result of calibration was found accurate as shown on date and place of calibration only.
6. Condition of Calibrated item : Good
   UUC Description :
   Time of Record 1 Hour 9 Minute At 35.0 °C
   Fresh air Damper [-] Open Position [-]
   [X] Close Fan [-]
   [-] Not Available
7. Result of Calibration : [X] Without adjustment [ ] After adjustment

25 March 2025

2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพมหานคร 10700
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel +66(0) 2422 8688 Fax +66(0) 2422 8545
nfi.or.th

เอกสารควบคุม

nfi national food institute ministry of industry
อุตสาหกรรมพัฒนามูลนิธิเพื่อสถาบันอาหาร
ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

ilac-MRA
NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Certificate

Certificate No.: 2502229-001-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakhanong, Bangkok 10260

Equipment: CHAMBER (Incubator)

Manufacturer: MEMMERT

Model: IPP 260

Serial No.: V615.0187

ID No.: UAE.MIC.003/2559

Order No.: 2502229

Operation No.: 2502229-001

Date of Receipt: 19 March 2025

Date of Calibration: 19 March 2025

Calibrated by Scientist

Approved by Manager, Division of Calibration Laboratory
Responsible for the Technical Management Team

Date of Issue: 25 March 2025

The uncertainties are for a confidence probability of approximately 95 %.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพมหานคร 10700
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel +66(0) 2422 8688 Fax +66(0) 2422 8545
nfi.or.th

เอกสารควบคุม

MM-C39

สถาบันอุตสาหกรรมพัฒนาอาหาร
ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Certificate

Certificate No.: 2502229-003-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakhanong, Bangkok 10260

Equipment: CHAMBER (Incubator)
Manufacturer: MEMMERT
Model: IPP260
Serial No.: V618.0033
ID No.: UAE.MIC.021/2561
Order No.: 2502229
Operation No.: 2502229-003
Date of Receipt: 19 March 2025
Date of Calibration: 19 March 2025

Calibrated by Scientist

Approved by Manager, Division of Calibration Laboratory
Responsible for the Technical Management Team

Date of Issue: 25 March 2025

The uncertainties are for a confidence probability of approximately 95 %.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65

2008 ซอยอุดมสุข 41 ถนนสุขุมวิท แขวงบางจักรี เขตบางพลัด กรุงเทพมหานคร 10700
2008 Soi 41, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel. +66(0) 2422 8688 Fax. +66(0) 2422 8545
nfi.or.th

เอกสารควบคุม ว.

ม.18/44

สถาบันอุตสาหกรรมพัฒนาอาหาร
ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Report

Certificate No.: 2502229-001-01
Equipment: CHAMBER (Incubator)
Model: IPP 260 Serial No.: V615.0187
Resolution: 0.1 °C ID No.: UAE.MIC.003/2559
Manufacturer: MEMMERT
Date of Calibration: 19 March 2025

Calibration point: 35.0 °C
Calibration result:

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
MIN	15.5	28	220.0
MAX	17.1	35	225.0




Table1 : Reporting of Temperature

Calibration point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.9 is REF)									Uncertainty ± (°C)
	# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9	
35.0	34.94	34.95	34.91	34.93	35.15	35.01	34.98	35.05	35.12	0.29

Table 2 : Reporting of Characterization Result

UUC* Setting (°C)	UUC* Reading (°C)			Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
	MIN	MAX	Average			
35.0	35.0	35.0	35.0	0.10	0.21	0.35

Note The quoted uncertainty include " Stability " and " Loading effect (20% of Temp Uniformity) "
UUC* = Unit Under Calibration
Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.
Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
Overall Variation = The difference of the maximum and minimum measured temperatures througout observation time.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2, providing a level of confidence of approximately 95 %.

--------- End ---------

25 March 2025

F-CS-012 Revision: 01 Date: 20-04-65

2008 ซอยอุดมสุข 41 ถนนสุขุมวิท แขวงบางจักรี เขตบางพลัด กรุงเทพมหานคร 10700
2008 Soi 41, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel. +66(0) 2422 8688 Fax. +66(0) 2422 8545
nfi.or.th

เอกสารควบคุม ว.

MM-C39

สถาบันอุตสาหกรรมพัฒนาอุตสาหกรรมอาหาร
ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Report

Certificate No.: 2502229-003-01

Equipment: CHAMBER (Incubator)

Model: IPP260 Serial No.: V618.0033

Resolution: 0.1 °C ID No.: UAE.MIC.021/2561

Manufacturer: MEMMERT

Date of Calibration: 19 March 2025

Calibration point: 22.0 and 25.0 °C

Calibration result:

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
MIN	22.7	58	220.0
MAX	23.3	60	225.0




Table1 : Reporting of Temperature

Calibration point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.9 is REF)									Uncertainty ± (°C)
	# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9	
22.0	22.18	22.18	22.16	22.19	21.94	21.95	21.96	21.98	22.08	0.27
25.0	25.51	25.32	25.29	25.34	25.05	25.02	25.04	25.09	25.15	0.27

Table 2 : Reporting of Characterization Result

UUC* Setting (°C)	UUC* Reading (°C)			Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
	MIN	MAX	Average			
22.0	22.0	22.0	22.0	0.026	0.14	0.29
25.0	25.0	25.0	25.0	0.035	0.36	0.55

Note The quoted uncertainty include " Stability " and " Loading effect (20% of Temp Uniformity) "

UUC* = Unit Under Calibration

Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.

Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.

Overall Variation = The difference of the maximum and minimum measured temperatures througout observation time.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2, providing a level of confidence of approximately 95 %.

--------- End ---------

25 March 2025

2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพมหานคร 10700
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel. +66(0) 2422 8688 Fax. +66(0) 2422 8545
nfi.or.th

เอกสารควบคุม ว.

น.18/45

สถาบันอุตสาหกรรมพัฒนาอุตสาหกรรมอาหาร
ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Report

Certificate No.: 2502229-003-01

Equipment: CHAMBER (Incubator)

Model: IPP260 Serial No.: V618.0033

Resolution: 0.1 °C ID No.: UAE.MIC.021/2561

Manufacturer: MEMMERT

Date of Calibration: 19 March 2025

Location: 302, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.

Environment Condition:

Ambient Temperature (23.0 ± 1) °C

Relative Humidity (59 ± 1) %

Line Voltage (223 ± 3) Volt

Condition of this results of Calibration:

1. This instrument was calibrated by insert 9 standard thermometer into its chamber and calibration according to W-TE-014 Based on TLAS G-20-1/02-08 (E): Guidelines for Calibration and Checks of Temperature Controlled Enclosures.
   - The temperature scale used was based on ITS - 90.
   - All data show below were final values and the initial data may be obtained upon request.
2. Reference Standard Instrument :

Instrument	Model	Serial No./ID No.	Certificate No.	Due Date	Through
Digital Thermometer with sensor	34972A	MY57003188	TE 670486-01	8 June 2025	NATIONAL FOOD INSTITUTE
	RTD	CH#301-309/ RTD#301-309			

3. This certificate is traceable to International System of Units (SI Units).
4. This certificate was certified only for the instrument we calibrated.
5. This result of calibration was found accurate as shown on date and place of calibration only.
6. Condition of Calibrated item : Good

   UUC Description :

   Time of Record 1 Hour 9 Minute At 22.0 and 25.0 °C

   Fresh air Damper [-] Open Position [-]

   [X] Close Fan [-]

   [-] Not Available
7. Result of Calibration : [X] Without adjustment [ ] After adjustment

25 March 2025

F-CS-012 Revision: 01 Date: 20-04-65

2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพมหานคร 10700
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel. +66(0) 2422 8688 Fax. +66(0) 2422 8545
nfi.or.th

เอกสารควบคุม ว.

สถาบันอาหาร
ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center
NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Report

Certificate No.: 2501624-001-01

Equipment: Water Bath

Model: WNE14 Serial No.: L416.0606

Resolution: 0.1 °C ID No.: UAE.MIC.002/2560


Manufacturer: MEMMERT

Date of Calibration: 10 February 2025

Calibration point: 44.5 °C

Calibration result:

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
Min	25.7	52	223.0
Max	26.3	65	225.0



Sensor Installation Location

Table1 : Reporting of Temperature

Calibration Point	Measured Temperature (°C) @ Sensor No. (Sensor No.5 is REF)					Uncertainty
(°C)	# 1	# 2	# 3	# 4	# 5	± (°C)
44.5	44.55	44.46	44.48	44.47	44.48	0.18

Table 2 : Reporting of Characterization Result

UUC* Setting	UUC* Reading (°C)			Stability	Uniformity	Overall Variation
(°C)	MIN	MAX	Average	± (°C)	(°C)	(°C)
44.5	44.5	44.5	44.5	0.082	0.070	0.29

Note The quoted uncertainty include " Stability " and " Loading effect (20% of Temp Uniformity)"

UUC* = Unit Under Calibration

Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.

Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.

Overall Variation = The difference of the maximum and minimum measured temperatures througout observation time.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2, providing a level of confidence of approximately 95 %.

--------- End ---------

19 Feb. 2025

2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพมหานคร 10700
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel: +66(0) 2422 8688 Fax: +66(0) 2422 8545
nfi.or.th

เอกสารไม่ควบคุม

สถาบันอาหาร
ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center
NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Certificate

Certificate No.: 2501624-001-01

Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.

Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakhanong, Bangkok 10260

Equipment: Water Bath

Manufacturer: MEMMERT

Model: WNE14

Serial No.: L416.0606

ID No.: UAE.MIC.002/2560

Order No.: 2501624

Operation No.: 2501624-001

Date of Receipt: 10 February 2025

Date of Calibration: 10 February 2025

Calibrated by
Scientist
WB

Approved by
Manager, Division of Calibration Laboratory
Responsible for the Technical Management Team

Date of Issue: 19 February 2025

The uncertainties are for a confidence probability of approximately 95 %.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพมหานคร 10700
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel: +66(0) 2422 8688 Fax: +66(0) 2422 8545
nfi.or.th

เอกสารไม่ควบคุม

MM-C39

สถาบันอาหาร
กระทรวงอุตสาหกรรม
national food institute
ministry of industry
สถาบันพัฒนาอุตสาหกรรมเพื่อสถาบันอาหาร
ศูนย์บริการห้องปฏิบัติการสถาบันอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

ilac-MRA

NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Certificate

Certificate No.: 2501624-002-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakhanong, Bangkok 10260

Equipment: Water Bath
Manufacturer: MEMMERT
Model: WNE14
Serial No.: L416.0612
ID No.: UAE.MIC.003/2560
Order No.: 2501624
Operation No.: 2501624-002
Date of Receipt: 10 February 2025
Date of Calibration: 10 February 2025

Calibrated by
Scientist
WB
Date of Issue: 19 February 2025

Approved by
Manager, Division of Calibration Laboratory
Responsible for the Technical Management Team

The uncertainties are for a confidence probability of approximately 95 %.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพมหานคร 10700
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel: +66(0) 2422 8688 Fax: +66(0) 2422 8545
nfi.or.th

เอกสารควบคุม

9.18/47

สถาบันอาหาร
กระทรวงอุตสาหกรรม
national food institute
ministry of industry
สถาบันพัฒนาอุตสาหกรรมเพื่อสถาบันอาหาร
ศูนย์บริการห้องปฏิบัติการสถาบันอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

ilac-MRA

NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Report

Certificate No.: 2501624-001-01
Equipment: Water Bath
Model: WNE14 Serial No.: L416.0606
Resolution: 0.1 °C ID No.: UAE.MIC.002/2560
Manufacturer: MEMMERT
Date of Calibration: 10 February 2025

Location: 302 Microbiology Laboratory, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Environment Condition:
Ambient Temperature (26 ± 1) °C
Relative Humidity (59 ± 7) %
Line Voltage (224 ± 1) Volt

Condition of this results of Calibration:

1. This instrument was calibrated by insert 5 standard thermometer into its liquid bath and calibration according to W-TE-011 based on ASTM E715-80 (2022): Standard Specification for Gravity-Convection and Forced-Circulation Water Baths.
   - The temperature scale used is ITS - 90.
   - All data show below were final values and the initial data may be obtained upon request.
2. Reference Standard Instrument :

Instrument	Model	Serial No./ID No.	Certificate No.	Due Date	Through
Digital Thermometer with sensor	34972A	MY59002902	TE 670478-01	4-May-25	NATIONAL FOOD INSTITUTE
	RTD	RTD#301-305 / CH#301-305			

3. This certificate is traceable to International System of Units (SI Units).
4. This certificate was certified only for the instrument we calibrated.
5. This result of calibration was found accurate as shown on date and place of calibration only.
6. Condition of Calibrated item : Good
   UUC Description:
   Time of Record 1 Hour 9 Minute At 44.5 °C
7. Result of Calibration :
   [X] Without adjustment
   [ ] After adjustment

19 Feb. 2025

2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพมหานคร 10700
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel: +66(0) 2422 8688 Fax: +66(0) 2422 8545
nfi.or.th

เอกสารไม่ควบคุม

MM-C39

nfi national food institute ministry of industry
อุตสาหกรรมพัฒนาบูลบีธีเพื่อสถาบันอาหาร
ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

ilac-MRA

NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Report

Certificate No.: 2501624-002-01

Equipment: Water Bath

Model: WNE14 Serial No.: L416.0612

Resolution: 0.1 °C ID No.: UAE.MIC.003/2560

Manufacturer: MEMMERT

Date of Calibration: 10 February 2025

Location: 302 Microbiology Laboratory, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.

Environment Condition:

Ambient Temperature (24 ± 1) °C

Relative Humidity (59 ± 7) %

Line Voltage (224 ± 1) Volt

Condition of this results of Calibration:

1. This instrument was calibrated by insert 5 standard thermometer into its liquid bath and calibration according to W-TE-011 based on ASTM E715-80 (2022): Standard Specification for Gravity-Convection and Forced-Circulation Water Baths.
   - The temperature scale used is ITS - 90.
   - All data show below were final values and the initial data may be obtained upon request.
2. Reference Standard Instrument :

Instrument	Model	Serial No./ID No.	Certificate No.	Due Date	Through
Digital Thermometer with sensor	34972A	MY59002902	TE 670478-01	4-May-25	NATIONAL FOOD INSTITUTE
	RTD	RTD#306-310 / CH#306-310			

3. This certificate is traceable to International System of Units (SI Units).
4. This certificate was certified only for the instrument we calibrated.
5. This result of calibration was found accurate as shown on date and place of calibration only.
6. Condition of Calibrated item : Good

   UUC Description:

   Time of Record 1 Hour 9 Minute At 44.5 °C
7. Result of Calibration :
   - [X] Without adjustment
   - [ ] After adjustment

19 Feb. 2025

2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพมหานคร 10
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel: +66(0) 2422 8688 Fax: +66(0) 2422 8545
nfi.or.th

เอกสารควบคุม

nfi national food institute ministry of industry
อุตสาหกรรมพัฒนาบูลบีธีเพื่อสถาบันอาหาร
ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

ilac-MRA

NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Report

Certificate No.: 2501624-002-01

Equipment: Water Bath

Model: WNE14 Serial No.: L416.0612

Resolution: 0.1 °C ID No.: UAE.MIC.003/2560


Manufacturer: MEMMERT

Date of Calibration: 10 February 2025

Calibration point: 44.5 °C

Calibration result:

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
Min	23.0	52	223.0
Max	25.0	65	225.0



Sensor Installation Location

Table1 : Reporting of Temperature

Calibration Point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.5 is REF)					Uncertainty ± (°C)
	# 1	# 2	# 3	# 4	# 5	
44.5	44.45	44.52	44.47	44.48	44.45	0.20

Table 2 : Reporting of Characterization Result

UUC* Setting (°C)	UUC* Reading (°C)			Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
	MIN	MAX	Average			
44.5	44.4	44.5	44.5	0.081	0.077	0.23

Note The quoted uncertainty include " Stability " and " Loading effect (20% of Temp Uniformity)"

UUC* = Unit Under Calibration

Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.

Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.

Overall Variation = The difference of the maximum and minimum measured temperatures througout observation time.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2. providing a level of confidence of approximately 95 %.

--------- End ---------

19 Feb. 2025

F-CS-012 Revision: 01 Date: 20-04-65

2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพมหานคร 10
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel: +66(0) 2422 8688 Fax: +66(0) 2422 8545
nfi.or.th

เอกสารควบคุม

MM-C39

สถาบันอาหาร
national food institute
ministry of industry
สถาบันพัฒนาอุตสาหกรรมเพื่อสถาบันอาหาร
ศูนย์บริการห้องปฏิบัติการสถาบันอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

ilac-MRA

NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Report

Certificate No.: 2502229-007-01

Equipment: Autoclave

Model: CL-40L Serial No.: 808763

Resolution: 0.1 °C ID No.: UAE.MIC.026/2563

Manufacturer: ALP

Date of Calibration: 19 March 2025

Location: LABORATORY, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.

Environment Condition: Ambient Temperature (23 ± 1) °C

Relative Humidity (60 ± 5) %

Line Voltage (225 ± 1) Volt

Condition of this results of Calibration:

1. This instrument was calibrated by insert 3 standard Data loggers with RTD into its autoclave and calibration according to W-TE-018 based on BS 2646-1:2021, Autoclaves for sterilization in laboratories Part 1: Design, construction, safety and performance - Specification.
   - The temperature scale used was based on ITS - 90.
   - All data show below were final values and the initial data may be obtained upon request.
2. Reference Standard Instrument :

Instrument	Model	Serial No.	Certificate No.	Due Date	Through
Digital Thermometer with RTD (Data Logger)	HiTemp140-PT	S35646	TE 670370-01	23-Mar-25	NATIONAL FOOD INSTITUTE
	HiTemp140-PT	S33753	TE 670371-01	23-Mar-25	NATIONAL FOOD INSTITUTE
	HiTemp140-PT	S29973	TE 670372-01	23-Mar-25	NATIONAL FOOD INSTITUTE

3. This certificate is traceable to International System of Units (SI Units).
4. This certificate was certified only for the instrument we calibrated.
5. This result of calibration was found accurate as shown on date and place of calibration only.
6. This standard does not apply to sterilizers or disinfectors used for medical, dental, pharmaceutical.
7. Condition of Calibrated item : Good

   UUC Description : Setting program function sterilization : STERILIZE/NORMAL

   Time of sterilization 15 Minute At 115.0 aand 121.0 °C
8. Result of Calibration : [X] Without adjustment [ ] After adjustment

2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพมหานคร 10700
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel: +66(0) 2422 8688 Fax: +66(0) 2422 8545
nfi.or.th

เอกสารไม่ควบคุม

สถาบันอาหาร
national food institute
ministry of industry
สถาบันพัฒนาอุตสาหกรรมเพื่อสถาบันอาหาร
ศูนย์บริการห้องปฏิบัติการสถาบันอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

ilac-MRA
NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Certificate

Certificate No.: 2502229-007-01

Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.

Address: 3 Soi Udomsuk 41, Sukhumvit Road, Bangchack, Prakhanong, Bangkok 10260

Equipment: Autoclave

Manufacturer: ALP

Model: CL-40L

Serial No.: 808763

ID No.: UAE.MIC.026/2563

Order No.: 2502229

Operation No.: 2502229-007

Date of Receipt: 19 March 2025

Date of Calibration: 19 March 2025

Calibrated by Scientist

Approved by Manager, Division of Calibration Laboratory Responsible for the Technical Management Team

Date of Issue: 25 March 2025

The uncertainties are for a confidence probability of approximately 95 %.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพมหานคร 10700
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel: +66(0) 2422 8688 Fax: +66(0) 2422 8545
nfi.or.th

เอกสารไม่ควบคุม

nfi national food institute ministry of industry
อุตสาหกรรมพัฒนามูลนิธิเพื่อสถาบันอาหาร
ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

ilac-MRA

NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Certificate

Certificate No.: 2503287-001-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakhanong, Bangkok 10260

Equipment: Autoclave
Manufacturer: ALP
Model: CL-40L
Serial No.: 810010
ID No.: UAE.MIC.032/2565
Order No.: 2503287
Operation No.: 2503287-001
Date of Receipt: 5 June 2025
Date of Calibration: 5 June 2025

Calibrated b [illegible]
Scientist

Approved by
Vice President, Department of Laboratory Services
Responsible for the Technical Management Team

Date of Issue: 11 June 2025

The uncertainties are for a confidence probability of approximately 95 %.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพมหานคร 10700
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel +66(0) 2422 8688 Fax +66(0) 2422 8545
nfi.or.th

เอกสารไม่ควบคุม

nfi national food institute ministry of industry
อุตสาหกรรมพัฒนามูลนิธิเพื่อสถาบันอาหาร
ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

ilac-MRA


NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Report

Certificate No.: 2502229-007-01
Equipment: Autoclave
Model: CL-40L Serial No.: 808763
Resolution: 0.1 °C ID No.: UAE.MIC.026/2563
Manufacturer: ALP
Date of Calibration: 19 March 2025

Calibration point: 115.0 aand 121.0 °C
Calibration result:

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
Min	22.0	55	224
Max	24.0	65	226



Standard at Position
Std#1 = Attached to the load temperature probe, within 20 mm.
Std#2 = In the upper half of the chamber
Std#3 = In the chamber drain, within 100 mm.

Table1 : Reporting of Temperature

Calibration Point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.2 is REF)			Uncertainty ± (°C)
	Std.# 1	Std.# 2 (Ref)	Std.# 3	
115.0	115.32	115.46	115.22	0.64
121.0	121.31	121.53	121.31	0.64

Table 2 : Reporting of Characterization Result

UUC* Setting (°C)	UUC* Reading				Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
	Min (°C)	Max (°C)	Average (°C)	MPa			
115.0	115.0	115.1	115.0	0.08	0.11	0.12	0.26
121.0	121.0	121.1	121.0	0.12	0.13	0.15	0.29

Note

The quoted uncertainty include " Stability " and " Loading effect (20% of Uniformity)"
UUC* = Unit Under Calibration
Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.
Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
Overall Variation = The difference of the maximum and minimum measured temperatures througout observation time.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2, providing a level of confidence of approximately 95 %.

--------- End ---------

25 March 2025

2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพมหานคร 10700
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel +66(0) 2422 8688 Fax +66(0) 2422 8545
nfi.or.th

เอกสารไม่ควบคุม

สถาบันอุตสาหกรรมพัฒนามูลนิธิเพื่อสถาบันอาหาร
ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
national food institute ministry of industry
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

ilac-MRA

THAILAND NSC-TISI-TIS 17025 CALIBRATION 0061

Calibration Report

Certificate No.: 2503287-001-01

Equipment: Autoclave

Model: CL-40L Serial No.: 810010

Resolution: 1 °C ID No.: UAE.MIC.032/2565

Manufacturer: ALP

Date of Calibration: 5 June 2025

Calibration point: 115 and 121 °C

Calibration result:

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
Min	25.8	50	225
Max	26.8	59	235

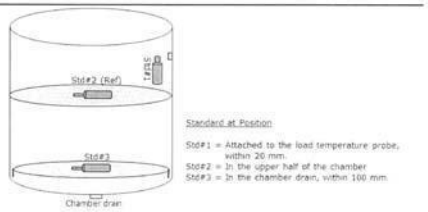


Table1 : Reporting of Temperature

Calibration Point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.2 is REF)			Uncertainty ± (°C)
	Std.# 1	Std.# 2 (Ref)	Std.# 3	
115	115.46	115.43	115.42	0.70
121	121.59	121.54	121.51	0.70

Table 2 : Reporting of Characterization Result

UUC* Setting (°C)	UUC* Reading				Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
	Min (°C)	Max (°C)	Average (°C)	MPa			
115	115	115	115	0.08	0.24	0.17	0.50
121	121	121	121	0.12	0.24	0.19	0.52

Note

The quoted uncertainty include " Stability " and " Loading effect (20% of Uniformity)"

UUC* = Unit Under Calibration

Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.

Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.

Overall Variation = The difference of the maximum and minimum measured temperatures througout observation time.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2, providing a level of confidence of approximately 95 %.

--------- End ---------

11 June 2025

2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพมหานคร 10700
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel. +66(0) 2422 8688 Fax. +66(0) 2422 8545
nfi.or.th

เอกสารไม่ควบคุม

สถาบันอุตสาหกรรมพัฒนามูลนิธิเพื่อสถาบันอาหาร
ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
national food institute ministry of industry
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

ilac-MRA

THAILAND NSC-TISI-TIS 17025 CALIBRATION 0061

Calibration Report

Certificate No.: 2503287-001-01

Equipment: Autoclave

Model: CL-40L Serial No.: 810010

Resolution: 1 °C ID No.: UAE.MIC.032/2565

Manufacturer: ALP

Date of Calibration: 5 June 2025

Location: Room 301 Media Preparation, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.

Environment Condition: Ambient Temperature (26 ± 1) °C

Relative Humidity (55 ± 5) %

Line Voltage (230 ± 5) Volt

Condition of this results of Calibration:

1. This instrument was calibrated by insert 3 standard Data loggers with RTD into its autoclave and calibration according to W-TE-018 based on BS 2646-1:2021, Autoclaves for sterilization in laboratories Part 1: Design, construction, safety and performance - Specification.
   - The temperature scale used was based on ITS - 90.
   - All data show below were final values and the initial data may be obtained upon request.
2. Reference Standard Instrument :

Instrument	Model	Serial No.	Certificate No.	Due Date	Through
Digital Thermometer with RTD (Data Logger)	HiTemp140-PT	T20627	NC-25-03-18-181	11-Mar-26	MADGETECH, INC.
	OM-CP-HITEMP-140	R56916	2502081-002-01	11-Mar-26	NATIONAL FOOD INSTITUTE
	PRTemp140	R38546	2501835-001-01	22-Feb-26	NATIONAL FOOD INSTITUTE

3. This certificate is traceable to International System of Units (SI Units).
4. This certificate was certified only for the instrument we calibrated.
5. This result of calibration was found accurate as shown on date and place of calibration only.
6. This standard does not apply to sterilizers or disinfectors used for medical, dental, pharmaceutical.
7. Condition of Calibrated item : Good

   UUC Description : Setting program function sterilization : STERILIZE/NORMAL

   Time of sterilization 20 Minute At 115 and 121 °C
8. Result of Calibration : [X] Without adjustment [ ] After adjustment

11 June 2025

F-CS-012 Revision: 01 Date: 20-04-65

2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพมหานคร 10700
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel. +66(0) 2422 8688 Fax. +66(0) 2422 8545
nfi.or.th

เอกสารไม่ควบคุม

nfi national food institute ministry of industry
อุตสาหกรรมพัฒนามูลนิธิเพื่อสถาบันอาหาร
ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

ilac-MRA

THAILAND NSC-TISI-TIS 17025 CALIBRATION 0061

Calibration Report

Certificate No.: 2502227-001-01

Equipment: Electronic Balance
Manufacturer: OHAUS
Model: PX623
Resolution: 0.001
Serial No.: C236754745
ID No.: UAE.MIC.055/2565
Capacity: 620

Date of Calibration: 19 March 2025

Calibration Results: (Continued)

Calibration Range: 0-600 g

Calibration Adjustment: Internal Calibration

3. Departure from Nominal Value:

Nominal Value (g)	Standard Value (g)	Average Reading (g)	Correction (g)	Uncertainty (± g)	Coverage Factor k
Unload	0.0000	0.000	0.000	0.00086	2.00
1	1.0000	1.000	0.000	0.00086	2.00
5	5.0000	4.999	0.001	0.00086	2.00
10	10.0000	10.000	0.000	0.00086	2.00
20	20.0000	20.000	0.000	0.00086	2.00
50	50.0000	50.000	0.000	0.00087	2.00
100	100.0001	100.000	0.000	0.00087	2.00
200	200.0001	200.001	-0.001	0.00090	2.00
300	300.0002	300.001	-0.001	0.00094	2.00
400	400.0003	399.999	0.001	0.0011	2.00
500	500.0003	499.999	0.001	0.0011	2.00
600	600.0004	600.000	0.000	0.0012	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

---------- End ----------

2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพมหานคร 10700
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10
Tel: +66(0) 2422 8688 Fax: +66(0) 2422 8545
nfi.or.th

เอกสารคุมไม่ ?

nfi national food institute ministry of industry
อุตสาหกรรมพัฒนามูลนิธิเพื่อสถาบันอาหาร
ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

ilac-MRA

THAILAND NSC-TISI-TIS 17025 CALIBRATION 0061

Calibration Certificate

Certificate No.: 2502227-001-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakhanong, Bangkok 10260

Equipment: Electronic Balance

Manufacturer: OHAUS

Model: PX623

Serial No.: C236754745

ID No.: UAE.MIC.055/2565

Order No.: 2502227

Operation No.: 2502227-001

Date of Receipt: 19 March 2025

Date of Calibration: 19 March 2025

Calibrated by Scientist

Approved by Manager, Division of Calibration Laboratory
Responsible for the Technical Management Team

Date of Issue: 25 March 2025

The uncertainties are for a confidence probability of approximately 95%

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพมหานคร 10700
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10
Tel: +66(0) 2422 8688 Fax: +66(0) 2422 8545
nfi.or.th
เอกสารคุมไม่ ?

MM-C39

JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Flow measurement laboratory
Calibration services department.

NSC – TISI – TIS 17025
CALIBRATION 0367

CERTIFICATE OF CALIBRATION

Certificate No. : **COF-049-68**

MEASUREMENT ITEM	: Top Load Orifice
MANUFACTURER	: Thermo Scientific
MODEL/TYPE	: G25A
SERIAL NUMBER	: 3375
ID NUMBER	: -
CONDITION AS-RECEIVED	: Used item
CUSTOMER	: Environmental Measurements Co., Ltd. 5/45 Baan Klang Krung Biz Town, Soi Srinagarindra 46/1 (Pramote), Nong Bon Sub-District Prawet District, Bangkok 10250
RECEIVED DATE	: 12 Nov 2025
MEASUREMENT DATE	: 17 Nov 2025
ISSUE DATE	: 17 Nov 2025

Calibration procedure:
The Orifice gas flow device was calibrated against Standard Rotary Displacement Meter (Roots Meter) Model G65/IMC/W2-dp. The WI-CL-004 was used as a calibration guideline.

Traceability:
This certificate provides a traceability of the measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MW-0016-25.

Uncertainty of Measurement:
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

ENVIRONMENTAL CONDITIONS:
Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa

CALIBRATION CONDITION:

Preconditioning	: 24 hours at ambient conditions.
Measurement Condition	: The average values during measurement are 24.1 °C and 47.8 %RH.

NOTED: *The certificate is valid only to the item calibrated on date and place of calibration.*

TABULATION OF RESULTS:
The table on next page give the measured values.

Calibrated by:

JIRANATEE ASSOCIATES CO.,LTD.

Approved signatory: .....
Calibration Department Manager

9.4.18/53

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

Jiranatee Associates Co., Ltd.

nfi national food institute ministry of industry
อุตสาหกรรมพัฒนามูลนิธิเพื่อสถาบันอาหาร
ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Report

Certificate No.: **2502227-001-01**

Equipment: Electronic Balance
Manufacturer: OHAUS
Model: PX623
Resolution: 0.001
Serial No.: C236754745
ID No.: UAE.MIC.055/2565
Capacity: 620

Date of Calibration: 19 March 2025

Environment Condition: Ambient Temperature: 22.8 ± 0.3 °C Relative Humidity: 51 ± 0.95 %
Place of Calibration: 301, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Condition of Equipment: Good Condition
Condition of This Results of Calibration:

1. Calibration Method: NFI Method W-MA-001 In-House Method based on UKAS Lab 14 : 2019
2. Reference Standards:

Reference Standard	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Standard Weight Class E2	1mg to 200g	B505567572	TCS	M2404100S	19 April 2025
Standard Weight Class E2	500g	B505567696	TCS	M2404101S	19 April 2025
Instrument	**Model**	**Serial No.**	**Calibrated By**	**Certificate No.**	**Due Date**
Thermo-Hygro Meter	608-H1	NFI.BTH 017/23	Quality Reborn	QR25-0542	10 February 2026

3. This certification is traceable to SI UNIT
4. This certificate was certified only for the instrument we calibrated.
5. This result of calibration was found accurate as shown on date and place of calibration only.


Calibration Results:

1. Repeatability of Reading:

Nominal Value (g)	Standard Deviation of Reading (g)
300	0.00042
600	0.00048

2. Off-Center Error:

A mass of 200 g was placed and moved to various position on pan.
The balance reading obtained is given in the table.



1 (g)	2 (g)	3 (g)	4 (g)	5 (g)	6 (g)	(Maximum Difference) (g)
200.002	200.003	200.001	200.001	200.002	200.002	0.001

2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่เรือ เขตบางพลัด กรุงเทพมหานคร 10700
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10
Tel +66(0) 2422 8688 Fax +66(0) 2422 8545

เอกสารคุมใ่ ว่
nfi.or.th

MM-C39

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
ilac-MRA
NSC-TISI-TIS 17025 CALIBRATION 0059 CLC

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE	:	VIBRATION METER
MANUFACTURER	:	VIBROCK
MODEL / TYPE	:	V9000
SERIAL NO.	:	2350
CLID. NO.	:	252101272
JOB CONTROL NO.	:	251118136392
CALIBRATION SERVICE	:	☑ IN-LABORATORY ☐ ON-SITE

CUSTOMER : ENVIRONMENTAL MEASUREMENTS CO., LTD.
5/45 BAAN KLANG KRUNG BIZ TOWN, SOI SRINAGARINDRA 46/1 (PRAMOTE),
NONG BON SUB-DISTRICT, PRAWET DISTRICT, BANGKOK 10250

DATE OF RECEIVED : 18 November 2025 DATE OF ISSUED : 21 November 2025

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Calibration Engineer

Approved By :

Authorized Signatory

21 November 2025

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q25136392

F3-011-05/12-23

@clccalibration

9.18/54

JIRANATEE ASSOCIATES CO.,LTD.

MEASUREMENT RESULTS:

The Orifice gas flow device was calibrated by direct comparison method with the Standard Rotary Displacement Meter (Roots Meter). The Humid air was used as a medium in the system. The standard conditions are 25°C (298.15 K) and 760 mmHg for standard temperature and standard pressure respectively.

Table 1: The results of Q Standard calibration data

Plate	Flow rate m³/min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Δp_meter mmHg	Δp_Orifice inH₂O	Y	Standard Flow [Q_s] m³/min
1	0.702	760.447	24.07	23.24	56.905	1.727	1.317	0.654
2	1.004	760.448	24.17	23.44	62.166	3.499	1.874	0.927
3	1.119	760.542	24.15	23.53	43.069	4.593	2.147	1.062
4	1.170	760.587	24.13	23.62	30.735	5.222	2.289	1.129
5	1.416	760.597	24.23	23.81	30.531	7.678	2.776	1.365

Slope (m): 2.04949
Intercept (b): -0.02534
Correlation coefficient (r): 0.99991
Uncertainty (k=2): 0.015 m³/min

Table 2: The results of Q actual calibration data

Plate	Flow rate m³/min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Δp_meter mmHg	Δp_Orifice inH₂O	Y	Standard Flow [Q_o] m³/min
1	0.702	760.447	24.07	23.24	56.905	1.727	0.822	0.651
2	1.004	760.448	24.17	23.44	62.166	3.499	1.170	0.924
3	1.119	760.542	24.15	23.53	43.069	4.593	1.340	1.058
4	1.170	760.587	24.13	23.62	30.735	5.222	1.429	1.125
5	1.416	760.597	24.23	23.81	30.531	7.678	1.733	1.361

Slope (m): 1.28368
Intercept (b): -0.01581
Correlation coefficient (r): 0.99991
Uncertainty (k = 2): 0.015 m³/min

End of Certificate of Calibration

JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co., Ltd.

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
NSC-TISI-TIS 17025 CALIBRATION 0059 CLC

CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment ( ) adjustment

CALIBRATION DATA

VELOCITY RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
(mm/s)	(frequency)		(mm/s)	(mm/s)	(mm/s)	± (% of rdg.)
10	160 Hz	peak	10.00	9.89	+0.11	1.1
20	160 Hz		20.00	19.49	+0.51	1.0
40	160 Hz		40.00	39.32	+0.68	1.0
60	160 Hz		60.00	58.74	+1.26	1.0
80	160 Hz		80.00	78.11	+1.89	1.0
100	160 Hz		100.00	97.62	+2.38	1.0

Note. The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 02 Page 62 of 138

This report is valid for the above stated instrument/s only.

End of Certificate

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
NSC-TISI-TIS 17025 CALIBRATION 0059 CLC

REPORT OF CALIBRATION

FOR

NOMENCLATURE	:	**VIBRATION METER**
MANUFACTURER	:	**VIBROCK**
MODEL / TYPE	:	**V9000**
SERIAL NO.	:	**2350**
DATE OF CALIBRATION	:	**19 November 2025**

ENVIRONMENT CONDITIONS :

Temperature : (23 ± 2) °C **Relative Humidity :** (55 ± 15) %RH

PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-127** based on **ISO 16063-21** as calibration guideline.

The calibration was performed by using Digital Multimeter, Programmable Timer/Counter, Accelerometer and Measuring Amplifier which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. Programmable Timer/Counter, Philips Model PM6680B S/N. SM607101.
2. Digital Multimeter, Keysight Technologies Model 3458A S/N. MY59352733.
3. Accelerometer with Measuring Amplifier, Bruel & Kjaer Model 8305, 2525 S/N. 397018, 2434988.

TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through Aeronautical Radio of Thailand Ltd. Certificate No. 07-0054/25 , Due Date 11 June 2026.
2. The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand) Certificate No. EE-0090-25, Due Date 31 July 2026.
3. The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand) Certificate No. AV-0056-24, Due Date 14 December 2025.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2$ which for a normal distribution corresponds to a coverage probability of approximately 95 %. It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

MM-C39

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com

CLC Accredited ISO/IEC 17025

ilac-MRA

NSC-TISI-TIS 17025 CALIBRATION 0059 CLC

REPORT OF CALIBRATION

FOR

NOMENCLATURE	:	VIBRATION METER
MANUFACTURER	:	VIBROCK
MODEL / TYPE	:	V9000
SERIAL NO.	:	2351
DATE OF CALIBRATION	:	10 November 2025

ENVIRONMENT CONDITIONS :

Temperature : (23 ± 2) °C **Relative Humidity :** (55 ± 15) %RH

PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-127** based on **ISO 16063-21** as calibration guideline.

The calibration was performed by using Digital Multimeter, Programmable Timer/Counter, Accelerometer and Measuring Amplifier which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. Digital Multimeter, Hewlett Packard Model 34401A S/N. 3146A75935.
2. Programmable Timer/Counter, Philips Model PM6680B S/N. SM607101.
3. Accelerometer with Measuring Amplifier, Bruel & Kjaer Model 8305, 2626 S/N. 705491, 1741406.

TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand) Certificate No. EE-0143-24, Due Date 06 December 2025.
2. The measurements are traceable to International System of Units (SI), through Aeronautical Radio of Thailand Ltd. Certificate No. 07-0054/25 , Due Date 11 June 2026.
3. The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand) Certificate No. AV-0051-24, Due Date 13 December 2025.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2$ which for a normal distribution corresponds to a coverage probability of approximately 95 %. It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q25131718

F3-011-05/12-23

@clccalibration

14.18/56

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com

CLC Accredited ISO/IEC 17025

ilac-MRA

NSC-TISI-TIS 17025 CALIBRATION 0059 CLC

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE	:	VIBRATION METER
MANUFACTURER	:	VIBROCK
MODEL / TYPE	:	V9000
SERIAL NO.	:	2351
CLID. NO.	:	252101273
JOB CONTROL NO.	:	251107131718
CALIBRATION SERVICE	:	☑ IN-LABORATORY ☐ ON-SITE

CUSTOMER : ENVIRONMENTAL MEASUREMENTS CO., LTD.
5/45 BAAN KLANG KRUNG BIZ TOWN, SOI SRINAGARINDRA 46/1 (PRAMOTE),
NONG BON SUB-DISTRICT, PRAWET DISTRICT, BANGKOK 10250

DATE OF RECEIVED : 07 November 2025 **DATE OF ISSUED :** 12 November 2025

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Calibration Engineer

Approved By :

Authorized Signatory

12 November 2025

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q25131718

F3-011-05/12-23

@clccalibration

MW-C39

SCARLET TECH

Certificate of Calibration

WL-21 Wireless Anemometer

Scarlet Tech Ltd. hrerby certifies that the WL-21 wireless anemometer listed below was thoroughly calibrated, test and inspected following the standard calibration procedure (st-wl-21) and is within manufacture's specification at the time when the calibration is done.

Client: Envir Service Co., Ltd.
Serial: 2504DR0058 Sensor 2504DT0058
Calibration Date: 2025/10/8
Calibration Expiry Date: 2026/10/7

The Result of Calibration

Velocity				
Measured Value (m/s)	Actual Value (m/s)	Deviation	Tolerance	Result
1.0	1.0	0.0	0.9-1.1	Pass
1.8	2.0	0.2	1.8-2.2	Pass
4.7	5.0	0.3	4.7-5.3	Pass
6.9	7.0	0.1	6.0-8.0	Pass
9.8	10.0	0.2	9.5-10.5	Pass
19.8	20.0	0.2	19.0-21.0	Pass

Wind Direction				
Measured Value (m/s)	Actual Value (m/s)	Deviation	Tolerance	Result
46°	45°	1	42-48	Pass
136°	135°	1	132-138	Pass
225°	225°	0	222-228	Pass
314°	315°	1	312-318	Pass
359°	0°	1	357-3	Pass

Inspection Room Temp	Actual Value	Deviation	Tolerance	Result
22.2°C	22.5	0.3	21.5-23.5	Pass

Atmospheric Pressure Inspection	Actual Value	Deviation	Tolerance	Result
1007	1005	2	1001-1019	Pass

Environment Conditions:

Air temperature: 22 °C
Relative humidity: 55 %
Static pressure: 102.2 kPa

Performed by: _____

Certified by Head of Engineering Department

SCARLET TECH CO., LTD. SCARLET TECH 斯卡雷特科技有限公司

This certificate may not be published or reproduced, except in full, unless Obtaining permission in writing from Scarlet Tech Ltd. 4F-3, No. 347, 2nd Sec., Heping E. Rd., Daan Dist. Taipei City 106, Taiwan

4.18/57

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com

CLC Accredited ISO/IEC 17025

ilac-MRA

NSC-TISI-TIS 17025 CALIBRATION 0059 CLC

CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment ( ) adjustment

CALIBRATION DATA

VELOCITY RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
(mm/s)	(frequency)		(mm/s)	(mm/s)	(mm/s)	±(% of rdg.)
10	160 Hz	peak	10.00	9.85	+0.15	1.1
20	160 Hz		20.00	19.51	+0.49	1.0
40	160 Hz		40.00	39.34	+0.66	1.0
60	160 Hz		60.00	58.98	+1.02	1.0
80	160 Hz		80.00	78.62	+1.38	1.0
100	160 Hz		100.00	97.51	+2.49	1.0

Note. The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 02 Page 60 of 138

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q25131718

F3-011-05/12-23

@clccalibration

MM-C39

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com

CLC Accredited ISO/IEC 17025

ilac-MRA

ANAB ANSI National Accreditation Board ACCREDITED CALIBRATION AND DIMENSIONAL MEASUREMENT ACDM-2814

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE	:	PRIMARY FLOW CALIBRATOR
MANUFACTURER	:	MESALABS
MODEL / TYPE	:	DEFENDER 510-M
SERIAL NO.	:	172525
CLID. NO.	:	212401789
JOB CONTROL NO.	:	251107131507
CALIBRATION SERVICE	:	☑ IN-LABORATORY ☐ ON-SITE

CUSTOMER : ENVIRONMENTAL MEASUREMENTS CO., LTD.
5/45 BAAN KLANG KRUNG BIZ TOWN, SOI SRINAGARINDRA 46/1 (PRAMOTE),
NONG BON SUB-DISTRICT, PRAWET DISTRICT, BANGKOK 10250

DATE OF RECEIVED : 07 November 2025 DATE OF ISSUED : 11 November 2025

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Calibration Engineer

Approved By :

Authorized Signatory

11 November 2025

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q25131507

F3-011-05/12-23

@clccalibration

น.18/58

SCARLET TECH

Certificate of Calibration

WL-21 Wireless Anemometer

Scarlet Tech Ltd. hrerby certifies that the WL-21 wireless anemometer listed below was thoroughly calibrated, test and inspected following the standard calibration procedure (st-wl-21) and is within manufacture's specification at the time when the calibration is done.

Client: Envir Service Co., Ltd.
Serial: 2504DR0060 Sensor 2504DT0060
Calibration Date: 2025/10/8
Calibration Expiry Date: 2026/10/7

The Result of Calibration

Velocity				
Measured Value (m/s)	Actual Value (m/s)	Deviation	Tolerance	Result
1.0	1.0	0.0	0.9-1.1	Pass
2.1	2.0	0.1	1.8-2.2	Pass
4.8	5.0	0.2	4.7-5.3	Pass
6.9	7.0	0.1	6.0-8.0	Pass
9.9	10.0	0.1	9.5-10.5	Pass
19.8	20.0	0.2	19.0-21.0	Pass

Wind Direction				
Measured Value (m/s)	Actual Value (m/s)	Deviation	Tolerance	Result
46°	45°	1	42-48	Pass
136°	135°	1	132-138	Pass
225°	225°	0	222-228	Pass
314°	315°	1	312-318	Pass
359°	0°	1	357-3	Pass

Inspection Room Temp	Actual Value	Deviation	Tolerance	Result
22.2°C	22.5	0.3	21.5-23.5	Pass

Atmospheric Pressure Inspection	Actual Value	Deviation	Tolerance	Result
1007	1005	2	1001-1019	Pass

Environment Conditions:
Air temperature: 22 °C
Relative humidity: 55 %
Static pressure: 102.2 kPa

Performed by. _____
Certified by Head of Engineering Department

SCARLET TECH CO., LTD.

This certificate may not be published or reproduced, except in full, unless Obtaining permission in writing from Scarlet Tech Ltd. 4F-3, No. 347, 2nd Sec., Heping E. Rd., Daan Dist. Taipai City 106, Taiwan

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
ilac-MRA
ANAB ANSI National Accreditation Board ACCREDITED ISO/IEC 17025 CALIBRATION AND DIMENSIONAL MEASUREMENT ACDM-2814

CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment ( ) adjustment

The table in the following gives the calibration results and associated measurement uncertainties of the measuring primary flow calibrator.

CALIBRATION DATA

STD Applied (L / min)	DUC Reading (L / min)	Correction (L / min)	Uncertainty ± (L/min)
0.5000	0.50521	-0.00521	0.57735
1.0000	1.0160	-0.0160	0.5774
2.0000	2.0431	-0.0431	0.5774
5.0000	5.1149	-0.1149	0.5781

Technical Note. Media of Gas : Air

Setting Temperature 23 ° C ; Pressure 101.3 kPa

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 016 Page 52 of 73

This report is valid for the above stated instrument/s only.

End of Certificate

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
ilac-MRA
ANAB ANSI National Accreditation Board ACCREDITED ISO/IEC 17025 CALIBRATION AND DIMENSIONAL MEASUREMENT ACDM-2814

REPORT OF CALIBRATION

FOR

NOMENCLATURE	:	**PRIMARY FLOW CALIBRATOR**
MANUFACTURER	:	**MESALABS**
MODEL / TYPE	:	**DEFENDER 510-M**
SERIAL NO.	:	**172525**
DATE OF CALIBRATION	:	**10 November 2025**

ENVIRONMENT CONDITIONS :

Temperature : (23 ± 2) °C **Relative Humidity :** (55 ± 10) % RH

PROCEDURE USED :

This instrument was calibrated under procedure No. **CLC-CPPF-03.** The calibration was performed by comparison with Gas Flow Meter which refers to the standard condition of 101.325 kPa and 0 °C.

REFERENCE STANDARD USED :

Gas Flow Meter, Alicat Scientific Model M-5SLPM-D-DB15 S/N. 261330.

TRACEABILITY :

The measurements are traceable to International System of Units (SI), through Chell Intrument Ltd.

Certificate No. N039747, Due Date 02 April 2026.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2$ which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

MM-C39

Request No. : 22-69 / 0084 MTC No. : PSL-P 0023 / 69

Serial No. : A.067438

Results :

UUC Range (lux)	Standard (lux)	*UUC Reading (lux)	Uncertainty of Measurement ± (lux)
2000	100	104	2.1
	500	505	11
	1000	997	21
	1500	1491	31
	2000	1982	41
20000 (×10)	2000	199	41
	3000	298	61
	4000	395	81
	5000	493	101

Note : *UUC = Unit Under Calibration.

...end of certificate...

Calibrated by :

Approved by :

Director

Photometry and Temperature Standards Laboratory

Ref. : 2012268111404571001

Issued date : 21 November 2025

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

Request No. : 22-69 / 0084 MTC No. : PSL-P 0023 / 69

CERTIFICATE OF CALIBRATION

Nomenclature : Digital Lux Meter Serial No. : A.067438

Maker : EXTECH Instruments Model : 407026

Customer : **ENVIRONMENTAL MEASUREMENTS CO., LTD.**

Address : 5/45 Baan Klang Krung Biz Town, Soi Srinagarindra 46/1 (Promote)
Nong Bon Sub-District, Prawet District, Bangkok 10250

Date of receipt : 14 November 2025

Date of calibration : 19 November 2025

Place of calibration : Photometry and Temperature Standards Laboratory, MTC. (Bangpoo)

Basis of calibration : calibration at 0 ~ 5000 lux.

Condition of calibration : - Ambient temperature : (25 ± 2) °C
- Relative humidity : (60 ± 20) %

Reference Standard : Working Standard Luminous Intensity Lamp, Serial No.: FEL003, can be traceable to international system of units (SI), through calibration certificate MTC No. PSL-P 0113/68, date of calibration 8 May 2025.

Traceability : This certificate is traceable to SI units through the National Institute of Metrology (Thailand) calibration certificate No. TP-1002-25, TP-11003-25 and TP-1004-25

Support Equipment : 1. Photometric bench , 3.0 meter long
2. DC power supply, Serial No.: MY41001705
3. Digital Multimeter , Model : 3458A , S/N : MY59351760

Calibration Procedure : The measurement was done in accordance with WI.CP.10.
The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95 %.

R.P.

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036
Fax. (66) 0 2577 9009

Office/Laboratory
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,
Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
(66) 08 3219 9440
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office
196 Phahonyothin Road, Ladyao, Chatuchak,
Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
(66) 08 1889 6827

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Road, Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
NSC-TISI-TIS 17025 CALIBRATION 0059 CLC

REPORT OF CALIBRATION

FOR

NOMENCLATURE	:	BALANCE
MANUFACTURER	:	METTLER TOLEDO
MODEL / TYPE	:	MS204TS/00
SERIAL NO.	:	B935191252[LA-002]
LOCATION SITE	:	LABORATORY - BALANCE ROOM
DATE OF CALIBRATION	:	04 February 2026

ENVIRONMENT CONDITIONS :

Temperature : 22 °C to 23 °C **Relative Humidity : 52 % to 54 %**

PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-46** based on **EURAMET cg-18 Version 4.0 (11/2015).**

The calibration was performed by Comparison with Standard Weight which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

Standard Weight, W&J Class E2 S/N. 1228.

TRACEABILITY :

The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd.

Certificate No.Q25059626 , Due Date 28 May 2027.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95%. It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Road, Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
NSC-TISI-TIS 17025 CALIBRATION 0059 CLC

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE	:	BALANCE
MANUFACTURER	:	METTLER TOLEDO
MODEL / TYPE	:	MS204TS/00
SERIAL NO.	:	B935191252[LA-002]
CLID. NO.	:	362200356
JOB CONTROL NO.	:	260130013128
CALIBRATION SERVICE	:	☐ IN-LABORATORY ☑ ON-SITE

CUSTOMER : ENVIRONMENTAL MEASUREMENTS CO., LTD.
5/45 BAAN KLANG KRUNG BIZ TOWN, SOI SRINAGARINDRA 46/1 (PRAMOTE),
NONG BON SUB-DISTRICT, PRAWET DISTRICT, BANGKOK 10250

DATE OF RECEIVED : 30 January 2026 DATE OF ISSUED : 11 February 2026

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Calibration Engineer

Approved By :

Authorized Signatory

11 February 2026

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Road, Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
NSC-TISI-TIS 17025 CALIBRATION 0059 CLC

REPORT OF CALIBRATION

FOR

NOMENCLATURE	:	BALANCE
MANUFACTURER	:	SHIMADZU
MODEL / TYPE	:	AP225WD
SERIAL NO.	:	D376300692[LA-001]
LOCATION SITE	:	LABORATORY-BALANCE ROOM
DATE OF CALIBRATION	:	04 February 2026

ENVIRONMENT CONDITIONS :

Temperature : 22 °C to 23 °C **Relative Humidity : 52 % to 54 %**

PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-46** based on **EURAMET cg-18 Version 4.0 (11/2015).**

The calibration was performed by Comparison with Weight Set which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

Standard weight, W&J Class E2 S/N. 1228

TRACEABILITY :

The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd.

Certificate No. Q25059626, Due Date 28 May 2026.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95%. It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

@clccalibration

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Road, Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
NSC-TISI-TIS 17025 CALIBRATION 0059 CLC

CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment ( ) adjustment

CALIBRATION DATA


1. Error of indications

Nominal Test Value (g)	Conventional mass (g)	Display Value (g)	Error of Balance (g)	Uncertainty ± (mg)	Coverage factor *k*
Unload	0.0000	0.0000	0.0000	0.07	2,00
0.1000	0.1000	0.1000	0.0000	0.15	2,00
0.5000	0.5000	0.5000	0.0000	0.15	2,00
1.0000	1.0000	1.0000	0.0000	0.15	2,00
2.0000	2.0000	2.0001	+0.0001	0.15	2,00
5.0000	5.0000	5.0000	0.0000	0.15	2,00
10.0000	10.0000	10.0001	+0.0001	0.15	2,00

2. Repeatability of indications

Nominal Test Value (g)	Standard Deviation of Reading (g)
10.0000	0.00005

3. Effect of eccentric application of a load on the indication

☐ 

☑ 

Nominal Test Value (g)	Display Value (g)					Maximum Difference of Center Value (g)
	Position 1	Position 2	Position 3	Position 4	Position 5	
100.0000	99.9999	100.0001	99.9999	99.9998	100.0001	0.0002

Note. The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 02 Page 116 of 138

This report is valid for the above stated instrument/s only.

End of Certificate

@clccalibration

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Road, Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
NSC-TISI-TIS 17025 CALIBRATION 0059 CLC

CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment ( ) adjustment

CALIBRATION DATA


1. Error of indications


Nominal Test Value (g)	Conventional mass (g)	Display Value (g)	Error of Balance (g)	Uncertainty ± (mg)	Coverage factor *k*
Unload	0.0000	0.0000	0.0000	0.07	2,00
1.0000	1.0000	1.0000	0.0000	0.15	2,00
10.0000	10.0000	10.0000	0.0000	0.15	2,00
20.0000	20.0000	20.0000	0.0000	0.16	2,00
40.0000	40.0000	39.9999	-0.0001	0.18	2,00
60.0000	60.0000	59.9999	-0.0001	0.18	2,00
80.0000	80.0000	79.9999	-0.0001	0.21	2,00
100.0000	100.0000	100.0000	0.0000	0.17	2,00
120.0000	120.0000	120.0000	0.0000	0.22	2,00
140.0000	140.0000	139.9999	-0.0001	0.24	2,00
160.0000	160.0000	159.9998	-0.0002	0.24	2,00
180.0000	179.9999	179.9998	-0.0001	0.27	2,00
200.0000	200.0000	199.9997	-0.0003	0.24	2,00

2. Repeatability of indications

Nominal Test Value (g)	Standard Deviation of Reading (g)
200.0000	0.000063

3. Effect of eccentric application of a load on the indication

☐ 

☑ 

Nominal Test Value (g)	Display Value (g)					Maximum Difference of Center Value (g)
	Position 1	Position 2	Position 3	Position 4	Position 5	
100.0000	100.0000	99.9999	100.0000	99.9999	99.9998	0.0002

Note. The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 02 Page 116 of 138

This report is valid for the above stated instrument/s only.

End of Certificate

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Road, Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
NSC-TISI-TIS 17025 CALIBRATION 0059 CLC

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : BALANCE
MANUFACTURER : SHIMADZU
MODEL / TYPE : AP225WD
SERIAL NO. : D376300692[LA-001]
CLID. NO. : 362100172
JOB CONTROL NO. : 260130013127
CALIBRATION SERVICE : ☐ IN-LABORATORY ☑ ON-SITE

CUSTOMER : ENVIRONMENTAL MEASUREMENTS CO., LTD.
5/45 BAAN KLANG KRUNG BIZ TOWN, SOI SRINAGARINDRA 46/1 (PRAMOTE),
NONG BON SUB-DISTRICT, PRAWET DISTRICT, BANGKOK 10250

DATE OF RECEIVED : 30 January 2026 **DATE OF ISSUED : 07 February 2026**

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Calibration Engineer

Approved By :

Authorized Signatory
07 February 2026

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Road, Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com

REPORT OF CALIBRATION

FOR

NOMENCLATURE	:	DO METER
MANUFACTURER	:	YSI
MODEL / TYPE	:	5000-230V/5010
SERIAL NO.	:	16D101626/19D100367[DOM-01]
DATE OF CALIBRATION	:	28 January 2026

ENVIRONMENT CONDITIONS :

Temperature : (25 ± 2.5) °C Relative Humidity : (50 ± 15) %RH

PROCEDURE USED :

This instrument was calibrated under procedure No. **CLC-CPCH-06.** The calibration was performed by direct measurement with Certified Reference Material (CRM).

REFERENCE STANDARD USED :

Dissolved Oxygen, Sigma-Aldrich Product ID QC3077-500ML.

TRACEABILITY :

The measurements are traceable to International System of Units (SI) , through Sigma-Aldrich USA.
Lot LRAD8571, Due Date April 2026.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2$ which for a normal distribution corresponds to a coverage probability of approximately 95 %.
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Road, Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE	:	DO METER
MANUFACTURER	:	YSI
MODEL / TYPE	:	5000-230V/5010
SERIAL NO.	:	16D101626/19D100367[DOM-01]
CLID. NO.	:	272100329
JOB CONTROL NO.	:	260127011808
CALIBRATION SERVICE	:	☑ IN-LABORATORY ☐ ON-SITE

CUSTOMER : ENVIRONMENTAL MEASUREMENTS CO., LTD.
5/45 BAAN KLANG KRUNG BIZ TOWN, SOI SRINAGARINDRA 46/1 (PRAMOTE),
NONG BON SUB-DISTRICT, PRAWET DISTRICT, BANGKOK 10250

DATE OF RECEIVED : 27 January 2026 DATE OF ISSUED : 29 January 2026

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Calibration Engineer

Approved By :

Authorized Signatory
29 January 2026

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Road, Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
ilac-MRA ANAB ACCREDITED CALIBRATION, DIMENSIONAL MEASUREMENT, AND TESTING

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE	:	HOT AIR OVEN
MANUFACTURER	:	MEMMERT
MODEL / TYPE	:	UF110
SERIAL NO.	:	B422.0026[LA-0012]
CLID. NO.	:	332202464
JOB CONTROL NO.	:	260130013129
CALIBRATION SERVICE	:	☐ IN-LABORATORY ☑ ON-SITE

CUSTOMER : ENVIRONMENTAL MEASUREMENTS CO., LTD.
5/45 BAAN KLANG KRUNG BIZ TOWN, SOI SRINAGARINDRA 46/1 (PRAMOTE),
NONG BON SUB-DISTRICT, PRAWET DISTRICT, BANGKOK 10250

DATE OF RECEIVED : 30 January 2026 DATE OF ISSUED : 09 February 2026

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Calibration Engineer

Approved By :

Authorized Signatory

09 February 2026

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Road, Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
ilac-MRA ANAB ACCREDITED CALIBRATION, DIMENSIONAL MEASUREMENT, AND TESTING

CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment ( ) adjustment

The table in the following gives the calibration results and associated measurement uncertainties of Do Meter.

CALIBRATION DATA

DO METER RESULT @ 20 °C

Nominal Value (mg/L)	DUC Reading (mg/L)	Correction (mg/L)	Uncertainty (mg/L)
8.18	8.22	-0.04	± 0.38

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 018 Page 5 of 73

This report is valid for the above stated instrument/s only.

End of Certificate

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Road, Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com

CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment ( ) adjustment

The table in the following gives the calibration results and associated measurement uncertainties of the measuring hot air oven.

CALIBRATION DATA

1. HOT AIR OVEN PERFORMANCE

DUC		Measured Uniformity	Measured Stability	Measured Overall
Setting (°C)	Indicating (°C)	(°C)	(°C)	Variation (°C)
104.0	104.0	0.29	0.16	0.55
180.0	180.0	1.08	0.38	2.16

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Road, Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com

REPORT OF CALIBRATION

FOR

NOMENCLATURE	:	**HOT AIR OVEN**
MANUFACTURER	:	**MEMMERT**
MODEL / TYPE	:	**UF110**
SERIAL NO.	:	**B422.0026[LA-0012]**
LOCATION SITE	:	**LABORATORY - HOT ZONE**
DATE OF CALIBRATION	:	**04 February 2026**

ENVIRONMENT CONDITIONS :

Temperature : 24 °C to 25 °C **Relative Humidity : 48% to 52 %**

PROCEDURE USED :

This instrument was calibrated under procedure No. **CLC-CPTH-07** based on **TLAS G-20** as calibration guidelines.

The calibration was performed by using Hydra Series II which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

Hydra Series II, Fluke Model 2635A S/N. 1700013.

TRACEABILITY :

The measurements are traceable to International System of Units (SI) , through Calibration Laboratory Co., Ltd.

Certificate No. Q25059630, Due Date 02 June 2026.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Road, Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
NSC-TISI-TIS 17025 CALIBRATION 0059 CLC

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE	:	INCUBATOR
MANUFACTURER	:	ACCUPLUS
MODEL / TYPE	:	SMART i250
SERIAL NO.	:	2059-0718-0010[LA-002]
CLID. NO.	:	332100155
JOB CONTROL NO.	:	260130013130
CALIBRATION SERVICE	:	☐ IN-LABORATORY ☑ ON-SITE

CUSTOMER : ENVIRONMENTAL MEASUREMENTS CO., LTD.
5/45 BAAN KLANG KRUNG BIZ TOWN, SOI SRINAGARINDRA 46/1 (PRAMOTE),
NONG BON SUB-DISTRICT, PRAWET DISTRICT, BANGKOK 10250

DATE OF RECEIVED : 30 January 2026 DATE OF ISSUED : 09 February 2026

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Calibration Engineer

Approved By :

Authorized Signatory

09 February 2026

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Road, Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025


CALIBRATION DATA

2. TEMPERATURE DISTRIBUTION

DUC		Measured Temperature (°C)@Probe No.9 is Ref.									Uncertainty ±(°C)	Coverage factor *k*
Setting (°C)	Indicating (°C)	1	2	3	4	5	6	7	8	9		
104.0	104.0	103.65	103.93	103.70	104.00	103.69	103.94	103.69	103.94	103.91	0.21	2,00
180.0	180.0	178.96	178.84	179.84	180.32	178.74	180.02	179.09	180.34	179.69	0.51	2,00

Technical Note : W = 56 cm, D = 40 cm, H = 48 cm.

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 018 Page 63 of 73



This report is valid for the above stated instrument/s only.

End of Certificate

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Road, Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
NSC-TISI-TIS 17025 CALIBRATION 0059 CLC

CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment ( ) adjustment

The table in the following gives the calibration results and associated measurement uncertainties of the measuring incubator.

CALIBRATION DATA

1. INCUBATOR PERFORMANCE

DUC		Measured Uniformity	Measured Stability	Measured Overall
Setting (°C)	Indicating (°C)	(°C)	(°C)	Variation (°C)
20.0	20.0	0.59	0.36	0.81

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Road, Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
NSC-TISI-TIS 17025 CALIBRATION 0059 CLC

REPORT OF CALIBRATION

FOR

NOMENCLATURE	:	**INCUBATOR**
MANUFACTURER	:	**ACCUPLUS**
MODEL / TYPE	:	**SMART i250**
SERIAL NO.	:	**2059-0718-0010[LA-002]**
LOCATION SITE	:	**LABORATORY**
DATE OF CALIBRATION	:	**04 February 2026**

ENVIRONMENT CONDITIONS :

Temperature : 24 °C to 25 °C **Relative Humidity : 48 % to 52 %**

PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-165** based on **TLAS G-20-1/02-08** as calibration guidelines.

The calibration was performed by using Hydra Series II which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

Hydra Series II, Fluke Model 2635A S/N. 8209003.

TRACEABILITY :

The measurements are traceable to International System of Units (SI) , through Calibration Laboratory Co., Ltd.

Certificate No. Q25044222, Due Date 21 April 2026.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

CALIBRATION LABORATORY CO., LTD.
2/10-11,14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com

CLC Accredited ISO/IEC 17025

NSC-TISI-TIS 17025 CALIBRATION 0059 CLC

MM-C39

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE	:	pH METER
MANUFACTURER	:	APERA
MODEL / TYPE	:	PH700/201T-F
SERIAL NO.	:	PH700X1019061009/N/A [LA-008/PH-02]
CLID. NO.	:	272401000
JOB CONTROL NO.	:	260127011809
CALIBRATION SERVICE	:	☑ IN-LABORATORY ☐ ON-SITE

CUSTOMER : ENVIRONMENTAL MEASUREMENTS CO., LTD.
5/45 BAAN KLANG KRUNG BIZ TOWN, SOI SRINAGARINDRA 46/1 (PRAMOTE),
NONG BON SUB-DISTRICT, PRAWET DISTRICT, BANGKOK 10250

DATE OF RECEIVED : 27 January 2026 DATE OF ISSUED : 29 January 2026

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Calibration Engineer

Approved By :

Authorized Signatory

29 January 2026

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

@clccalibration

ม.18/69

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Road, Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com

CLC Accredited ISO/IEC 17025

NSC-TISI-TIS 17025 CALIBRATION 0059 CLC


CALIBRATION DATA

2. TEMPERATURE DISTRIBUTION

DUC		Measured Temperature (°C)@Probe No.9 is Ref.									Uncertainty ±(°C)	Coverage factor *k*
Setting (°C)	Indicating (°C)	1	2	3	4	5	6	7	8	9		
20.0	20.0	20.63	20.71	20.61	20.43	20.53	20.50	20.53	20.56	20.38	0.60	2,00

Technical Note : W = 50 cm, D = 48 cm, H = 110 cm.

Note. The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 02 Page 129 of 138



This report is valid for the above stated instrument/s only.

End of Certificate

@clccalibration

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
NSC-TISI-TIS 17025 CALIBRATION 0059 CLC

TRACEABILITY :

1. The measurements are traceable to International System of Units (SI) , through National Institute of Metrology (Thailand).
Lot Number. 191025 , 241025. Due Date 24 December 2026.
2. The measurements are traceable to International System of Units (SI) , through Control Company.
Certificate No. 4288-15743843 , Due Date 27 February 2027.
3. The measurements are traceable to International System of Units (SI) , through Calibration Laboratory Co., Ltd.
Certificate No. Q25097314, Due Date 29 August 2026.
4. The measurements are traceable to International System of Units (SI) , through Thailand Institute of Scientific and Technological Research (TISTR). Certificate No. PSL-T 0177/68, Due Date 10 February 2026.
5. The measurements are traceable to International System of Units (SI) , through National Institute of Metrology (Thailand).
Certificate No. TT-1008-25, Due Date 04 March 2026.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
NSC-TISI-TIS 17025 CALIBRATION 0059 CLC

REPORT OF CALIBRATION

FOR

NOMENCLATURE	:	**pH METER**
MANUFACTURER	:	**APERA**
MODEL / TYPE	:	**PH700/201T-F**
SERIAL NO.	:	**PH700X1019061009/N/A [LA-008/PH-02]**
DATE OF CALIBRATION	:	**28 January 2026**

ENVIRONMENT CONDITIONS :

Temperature : (25 ± 2.5) °C **Relative Humidity :** (50 ± 15) % RH

PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-128, WI-305-238.** The calibration was performed by direct measurement with Certified Reference Material (CRM) and comparison with Temperature Bath, Precision Thermometer and IPRT which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. pH Standard Solution, NIMT TRM CODE TRM-S-2003, TRM CODE TRM-S-2007.
2. pH Standard Solution, Control Company Catalog Number 06664263,11784256, Lot Number CC818772.
3. Temperature Bath, Jingmi Model RTS-35S S/N. 16339.
4. Precision Thermometer, ASL Model F200-A-8 S/N. 014433/03.
5. IPRT, ASL Model T100-250-1D S/N. PO106346-1-13.

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Road, Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
NSC-TISI-TIS 17025 CALIBRATION 0059 CLC

REPORT OF CALIBRATION

FOR

NOMENCLATURE	:	WATER BATH
MANUFACTURER	:	MEMMERT
MODEL / TYPE	:	WNB14
SERIAL NO.	:	L418.0758[LA-004]
LOCATION SITE	:	LABORATORY - HOT ZONE
DATE OF CALIBRATION	:	04 February 2026

ENVIRONMENT CONDITIONS :

Temperature : 24 °C to 25 °C **Relative Humidity : 48% to 52%**

PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-135** based on **ASTM E 715-80:2016** as calibration guidelines.

The calibration was performed by using Hydra Data Logger which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

Hydra Data Logger, Fluke Model 2620 S/N. 5592550.

TRACEABILITY :

The measurements are traceable to International System of Units (SI) , through Calibration Laboratory Co., Ltd.

Certificate No. Q25111569, Due Date 24 March 2026.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2$ which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
NSC-TISI-TIS 17025 CALIBRATION 0059 CLC

CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment ( ) adjustment

The table in the following gives the calibration results and associated measurement uncertainties of pH meter.

CALIBRATION DATA

1. pH METER RESULT @ 25 °C

Standard pH Buffer Solution (pH)	pH Meter Reading (pH)	pH Meter Reading (mV)	Correction (pH)	Uncertainty of Measurement (± pH)	*k* Factor
4.012	4.00	123	+0.012	0.014	2,15
6.997	7.00	-53	-0.003	0.015	2,06
9.994	10.00	-220	-0.006	0.100	2,00

Note. The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 02 Page 91 of 138

***2. TEMPERATURE RESULT**

Immersion depth (mm)	Actual Temperature (°C)	DUC Reading (°C)	Correction (°C)	Uncertainty ± (°C)
100	25.00	25.0	0.00	0.08

Technical Note. Type of sensor : pH Probe

Probe ∅ 12 mm

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor of $k = 2$.

Note. * means Calibrations marked " Not TISI Accredited " in this Certificate have been included for completeness.

This report is valid for the above stated instrument/s only.

End of Certificate

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Road, Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
NSC-TISI-TIS 17025
CALIBRATION 0059
CLC

CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment ( ) adjustment

The table in the following gives the calibration results and associated measurement uncertainties of the measuring water bath.

CALIBRATION DATA

1. WATER BATH PERFORMANCE

Test Point (°C)	DUC Reading (°C)	Uniformity (°C)	Stability (°C)
95.0	95.0	0.39	0.20

@clccalibration

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Road, Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
NSC-TISI-TIS 17025
CALIBRATION 0059
CLC

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE	:	WATER BATH
MANUFACTURER	:	MEMMERT
MODEL / TYPE	:	WNB14
SERIAL NO.	:	L418.0758[LA-004]
CLID. NO.	:	332100157
JOB CONTROL NO.	:	260130013132
CALIBRATION SERVICE	:	☐ IN-LABORATORY ☑ ON-SITE

CUSTOMER : ENVIRONMENTAL MEASUREMENTS CO., LTD.
5/45 BAAN KLANG KRUNG BIZ TOWN, SOI SRINAGARINDRA 46/1 (PRAMOTE),
NONG BON SUB-DISTRICT, PRAWET DISTRICT, BANGKOK 10250

DATE OF RECEIVED : 30 January 2026 DATE OF ISSUED : 09 February 2026

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Calibration Engineer

Approved By :

Authorized Signatory
09 February 2026

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

@clccalibration

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Road, Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
NSC-TISI-TIS 17025 CALIBRATION 0059 CLC

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE	:	WATER BATH
MANUFACTURER	:	M-LAB
MODEL / TYPE	:	WBN 15
SERIAL NO.	:	0335[LA-007]
CLID. NO.	:	332300657
JOB CONTROL NO.	:	260130013133
CALIBRATION SERVICE	:	☐ IN-LABORATORY ☑ ON-SITE

CUSTOMER : ENVIRONMENTAL MEASUREMENTS CO., LTD.
5/45 BAAN KLANG KRUNG BIZ TOWN, SOI SRINAGARINDRA 46/1 (PRAMOTE),
NONG BON SUB-DISTRICT, PRAWET DISTRICT, BANGKOK 10250

DATE OF RECEIVED : 30 January 2026 DATE OF ISSUED : 09 February 2026

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Calibration Engineer

Approved By :

Authorized Signatory
09 February 2026

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Road, Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
NSC-TISI-TIS 17025 CALIBRATION 0059 CLC


CALIBRATION DATA

2. TEMPERATURE DISTRIBUTION

Test Point (°C)	DUC Reading (°C)	STD Reading (°C)					Uncertainty ±(°C)
		Probe No. 1	Probe No. 2	Probe No. 3	Probe No. 4	Probe No. 5	
95.0	95.0	96.25	96.15	96.08	95.99	96.03	0.52

Technical Note : W = 35 cm, D = 29 cm, H = 14 cm.

Note. The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 02 Page 128 of 138



This report is valid for the above stated instrument/s only.

End of Certificate

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Road, Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
NSC-TISI-TIS 17025 CALIBRATION 0059 CLC

CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment ( ) adjustment

The table in the following gives the calibration results and associated measurement uncertainties of the measuring water bath.

CALIBRATION DATA

1. WATER BATH PERFORMANCE

Test Point (°C)	DUC Reading (°C)	Uniformity (°C)	Stability (°C)
85.0	85.0	0.21	0.14

@clccalibration

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Road, Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
NSC-TISI-TIS 17025 CALIBRATION 0059 CLC

REPORT OF CALIBRATION

FOR

NOMENCLATURE	:	**WATER BATH**
MANUFACTURER	:	**M-LAB**
MODEL / TYPE	:	**WBN 15**
SERIAL NO.	:	**0335[LA-007]**
LOCATION SITE	:	**LABORATORY - HOT ZONE**
DATE OF CALIBRATION	:	**04 February 2026**

ENVIRONMENT CONDITIONS :

Temperature : 24 °C to 25 °C **Relative Humidity : 48% to 52%**

PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-135** based on **ASTM E 715-80:2016** as calibration guidelines.

The calibration was performed by using Hydra Data Logger which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

Hydra Data Logger, Fluke Model 2620 S/N. 5592550.

TRACEABILITY :

The measurements are traceable to International System of Units (SI) , through Calibration Laboratory Co., Ltd.

Certificate No. Q25111569, Due Date 24 March 2026.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2$ which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

@clccalibration

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Road, Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com
CLC Accredited ISO/IEC 17025
NSC-TISI-TIS 17025
CALIBRATION 0059
CLC


CALIBRATION DATA

2. TEMPERATURE DISTRIBUTION

Test Point (°C)	DUC Reading (°C)	STD Reading (°C)					Uncertainty ±(°C)
		Probe No. 1	Probe No. 2	Probe No. 3	Probe No. 4	Probe No. 5	
85.0	85.0	84.91	84.92	84.92	84.92	84.84	0.32

Technical Note : W = 35 cm, D = 30 cm, H = 15 cm.

Note. The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 02 Page 128 of 138



This report is valid for the above stated instrument/s only.

End of Certificate

MM-C39

ที่ อก ๐๓๑๐(๑)/ ๖๙๗๓

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๒๕ สิงหาคม ๒๕๖๘

เรื่อง ยกเลิกบุคลากรของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท ยูไนเต็ด แอนนาลิสต์ แอนด์ เอ็นจิเนียริ่ง คอนซัลแตนท์ จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน ลงวันที่ ๗ สิงหาคม ๒๕๖๘

ตามคำขอที่อ้างถึง บริษัท ยูไนเต็ด แอนนาลิสต์ แอนด์ เอ็นจิเนียริ่ง คอนซัลแตนท์ จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๑๔๕ สถานที่ตั้งเลขที่ ๓ ซอยอุดมสุข ๔๑ ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร ขอยกเลิกบุคลากร ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้ยกเลิกเจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน จำนวน ๕ ราย ได้แก่

ทะเบียนเลขที่ ว-๑๔
ทะเบียนเลขที่ ว-๑๔
ทะเบียนเลขที่ ว-๑๔
ทะเบียนเลขที่ ว-๑๔
ทะเบียนเลขที่ ว-๑๔

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

นักวิทยาศาสตร์เชี่ยวชาญ รักษาราชการแทน
ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน
กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ
โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕
โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๙๙
ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th

UAE UNITED ANALYST AND ENGINEERING CONSULTANT COMPANY LIMITED

สำเนาถูกต้อง

ที่ อก ๐๓๑๐(๑)/ ๘๓๐๒

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๐๘ ตุลาคม ๒๕๖๘

เรื่อง ยกเลิกบุคลากรของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท ยูไนเต็ด แอนนาลิสต์ แอนด์ เอ็นจิเนียริ่ง คอนซัลแตนท์ จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน ลงวันที่ ๒๕ กันยายน ๒๕๖๘

ตามคำขอที่อ้างถึง บริษัท ยูไนเต็ด แอนนาลิสต์ แอนด์ เอ็นจิเนียริ่ง คอนซัลแตนท์ จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๑๔๕ สถานที่ตั้งเลขที่ ๓ ซอยอุดมสุข ๔๑ ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร ขอยกเลิกบุคลากร ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้ยกเลิกเจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน จำนวน ๓ ราย ได้แก่

ทะเบียนเลขที่ ว-๑๔๕
ทะเบียนเลขที่ ว-๑๔๕
ทะเบียนเลขที่ ว-๑๔๕

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน
กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ
โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕
โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๙๙
ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th

UAE UNITED ANALYST AND ENGINEERING CONSULTANT COMPANY LIMITED

สำเนาถูกต้อง

MM-C39

เอกสารแนบท้ายหนังสือเปลี่ยนแปลงบุคลากรและสารมลพิษที่วิเคราะห์
บริษัท ยูไนเต็ด แอนนาลิสต์ แอนด์ เอ็นจิเนียริ่ง คอนซัลแตนท์ จำกัด เลขทะเบียน ว-๑๔๕
ที่ อก ๐๓๑๐(๑)/ ๕๖๙๑ ลงวันที่ ๐๗ กรกฎาคม ๒๕๖๘

ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๑๑ รายการ

น้ำใต้ดิน จำนวน 4 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Aluminum	Digestion, Inductively Coupled Plasma Method[1]
2	Copper	1) Digestion, Flame Atomic Absorption Spectrometric Method[1] 2) Digestion, Inductively Coupled Plasma Method[1]
3	Iron	1) Digestion, Flame Atomic Absorption Spectrometric Method[1] 2) Digestion, Inductively Coupled Plasma Method[1]
4	Molybdenum	Digestion, Inductively Coupled Plasma Method[1]

อากาศเสีย (ปล่องระบาย) จำนวน 1 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Oxides of Nitrogen	Absorption Sampling, Ion Chromatographic Method[2]

ดิน จำนวน 6 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Aluminum	Digestion, Inductively Coupled Plasma Method[3,5]
2	Copper	1) Digestion, Flame Atomic Absorption Spectrometric Method[3,6] 2) Digestion, Inductively Coupled Plasma Method[3,5]
3	Iron	1) Digestion, Flame Atomic Absorption Spectrometric Method[3,6] 2) Digestion, Inductively Coupled Plasma Method[3,5]
4	Molybdenum	Digestion, Inductively Coupled Plasma Method[3,6]
5	pH	Electrometric Method[8]
6	TPH (C_5-C_8)	Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method[4,7]

UAE สำเนาถูกต้อง
UNITED ANALYST AND ENGINEERING CONSULTANT COMPANY LIMITED

เอกสารอ้างอิง

1. APHA, AWWA, WEF. **Standard Methods for the Examination of Water and Wastewater.** 24th ed. Washington, DC: APHA, 2023.

2. United States Environmental Protection Agency. **Standards of Performance for New Stationary Sources.** 40 CFR 60. Appendix A, 2023.

3. United States...

ที่ อก ๐๓๑๐(๑)/ ๕๖๙๑

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๐๗ กรกฎาคม ๒๕๖๘

เรื่อง เปลี่ยนแปลงบุคลากรและสารมลพิษที่วิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท ยูไนเต็ด แอนนาลิสต์ แอนด์ เอ็นจิเนียริ่ง คอนซัลแตนท์ จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน ลงวันที่ ๙ พฤษภาคม ๒๕๖๘

สิ่งที่ส่งมาด้วย เอกสารแนบท้ายหนังสือเปลี่ยนแปลงบุคลากรและสารมลพิษที่วิเคราะห์ บริษัท ยูไนเต็ด แอนนาลิสต์ แอนด์ เอ็นจิเนียริ่ง คอนซัลแตนท์ จำกัด จำนวน ๒ แผ่น

ตามหนังสือที่อ้างถึง บริษัท ยูไนเต็ด แอนนาลิสต์ แอนด์ เอ็นจิเนียริ่ง คอนซัลแตนท์ จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๑๔๕ สถานที่ตั้งเลขที่ ๓ ซอยอุดมสุข ๔๑ ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร ขอเปลี่ยนแปลงบุคลากรและสารมลพิษที่วิเคราะห์ ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว มีความเห็นดังนี้

๑. ให้ยกเลิกเจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน จำนวน ๓ ราย
ทะเบียนเลขที่
ทะเบียนเลขที่
ทะเบียนเลขที่

๒. ให้เพิ่มผู้ควบคุมห้องปฏิบัติการวิเคราะห์เอกชน จำนวน ๑ ราย
ทะเบียนเลขที่

๓. ให้เพิ่มขอบข่ายสารมลพิษที่วิเคราะห์ในน้ำใต้ดิน อากาศเสีย และดิน ตามสิ่งที่ส่งมาด้วย

อนึ่ง หนังสือฉบับนี้จะหมดอายุพร้อมหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ในวันที่ ๒ กุมภาพันธ์ ๒๕๗๒

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน
กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ
โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕
โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๙๙
ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th

UAE สำเนาถูกต้อง
UNITED ANALYST AND ENGINEERING CONSULTANT COMPANY LIMITED

Green Industry
"อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา อุตสาหกรรมสีเขียว"

MM-C39



ที่ อก ๐๓๑๐(๑)/ ๑๔๙๑

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๒๔ กุมภาพันธ์ ๒๕๖๘

เรื่อง ยกเลิกบุคลากรของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท ยูไนเต็ด แอนนาลิสต์ แอนด์ เอ็นจิเนียริ่ง คอนซัลแตนท์ จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และขนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน ลงวันที่ ๑๘ กุมภาพันธ์ ๒๕๖๘

ตามคำขอที่อ้างถึง บริษัท ยูไนเต็ด แอนนาลิสต์ แอนด์ เอ็นจิเนียริ่ง คอนซัลแตนท์ จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๑๔๕ สถานที่ตั้งเลขที่ ๓ ซอยอุดมสุข ๔๑ ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร ขอยกเลิกบุคลากร ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้ยกเลิกเจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน จำนวน ๓ ราย ได้แก่

ทะเบียนเลขที่ ว
ทะเบียนเลขที่ ว
ทะเบียนเลขที่ ว

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

รองอธิบดี ปฏิบัติราชการแทน
อธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน
กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ
โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕
โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๙๙
ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th

UAE UNITED ANALYST AND ENGINEERING CONSULTANT COMPANY LIMITED สำเนาถูกต้อง

3. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Acid Digestion of Sediments, Sludges, and Soils. SW-846 Method 3050B,** 1996.

4. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Volatile Organic Compounds in Various Sample Matrices Using Equilibrium Headspace Analysis. SW-846 Method 5021A,** 2014.

5. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Inductively Coupled Plasma-Optical Emission Spectrometry. SW-846 Method 6010D,** 2018.

6. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Flame Atomic Absorption Spectrophotometry. SW-846 Method 7000B,** 2007.

7. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Volatile Organic Compounds by Gas Chromatography/ Mass Spectrometry. SW-846 Method 8260D,** 2018.

8. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Soil and Waste pH. SW-846 Method 9045D,** 2004

UAE UNITED ANALYST AND ENGINEERING CONSULTANT COMPANY LIMITED สำเนาถูกต้อง

น.18/78

MM-C39

น.18/79

ที่ อก ๐๓๑๐(๑)/ ๑๐๘๙ กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๐๗ กุมภาพันธ์ ๒๕๖๘

เรื่อง ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

เรียน กรรมการผู้จัดการ บริษัท ยูไนเต็ด แอนนาลิสต์ แอนด์ เอ็นจิเนียริ่ง คอนซัลแตนท์ จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน ลงวันที่ ๓ ธันวาคม ๒๕๖๗

สิ่งที่ส่งมาด้วย ๑. รายชื่อผู้ควบคุมห้องปฏิบัติการวิเคราะห์เอกชน จำนวน ๔๐ ราย
๒. รายชื่อเจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน จำนวน ๑๔๑ ราย
๓. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม

ตามคำขอที่อ้างถึง บริษัท ยูไนเต็ด แอนนาลิสต์ แอนด์ เอ็นจิเนียริ่ง คอนซัลแตนท์ จำกัด ขอต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๑๔๕ สถานที่ตั้งเลขที่ ๓ ซอยอุดมสุข ๔๑ ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร ต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้บริษัท ยูไนเต็ด แอนนาลิสต์ แอนด์ เอ็นจิเนียริ่ง คอนซัลแตนท์ จำกัด ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน โดยมีองค์ประกอบดังนี้

ก. ผู้ควบคุมห้องปฏิบัติการวิเคราะห์เอกชน จำนวน ๔๐ ราย ตามสิ่งที่ส่งมาด้วย ๑
ข. เจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน จำนวน ๑๔๑ ราย ตามสิ่งที่ส่งมาด้วย ๒
ค. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนให้วิเคราะห์ในน้ำ/น้ำเสีย น้ำใต้ดิน อากาศเสีย สิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว และดิน ตามสิ่งที่ส่งมาด้วย ๓

หนังสือฉบับนี้จะหมดอายุในวันที่ ๒ กุมภาพันธ์ ๒๕๗๒ หากประสงค์จะต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ให้ยื่นคำขอต่ออายุพร้อมเอกสารประกอบคำขอต่อกรมโรงงานอุตสาหกรรมภายใน ๖๐ วัน ก่อนวันสิ้นอายุของหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

รองอธิบดี ปฏิบัติราชการแทน
อธิบดีกรมโรงงานอุตสาหกรรม

UNITED ANALYST AND ENGINEERING CONSULTANT COMPANY LIMITED

สำเนาถูกต้อง

กองวิจัยและเตือนภัยมลพิษโรงงาน
กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ
โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕
โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๙
ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th

Green Industry
"อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา อุตสาหกรรมสีเขียว"

สิ่งที่ส่งมาด้วย ๑

เอกสารแนบท้ายหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท ยูไนเต็ด แอนนาลิสต์ แอนด์ เอ็นจิเนียริ่ง คอนซัลแตนท์ จำกัด เลขทะเบียน ว-๑๔๕
ที่ อก ๐๓๑๐(๑)/ ๑๐๘๙ ลงวันที่ ๐๗ กุมภาพันธ์ ๒๕๖๘

ก. ผู้ควบคุมห้องปฏิบัติการวิเคราะห์เอกชน จำนวน ๔๐ ราย

ทะเบียนเลขที่ ว-
ทะเบียนเลขที่ ว-
ทะเบียนเลขที่ ว-

เอกสารแนบท้ายหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท ยูไนเต็ด แอนนาลิสต์ แอนด์ เอ็นจิเนียริ่ง คอนซัลแตนท์ จำกัด เลขทะเบียน ว-๑๔๕
ที่ อก ๐๓๑๐(๑)/ ๑๐๘๙ ลงวันที่ ๐๗ กุมภาพันธ์ ๒๕๖๘

ข. เจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน จำนวน ๑๔๑ ราย

ทะเบี
ทะเบี
ทะเบี

ทะเบียนเลขที่
ทะเบียนเลขที่
ทะเบียนเลขที่

เอกสารแนบท้ายหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท ยูไนเต็ด แอนนาลิสต์ แอนด์ เอ็นจิเนียริ่ง คอนซัลแตนท์ จำกัด เลขทะเบียน ว-๑๔๕
ที่ อก ๐๓๑๐(๑)/ ๑๐๘๙ ลงวันที่ ๐๗ กุมภาพันธ์ ๒๕๖๘

ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๓๕๗ รายการ

น้ำ/น้ำเสีย จำนวน 46 รายการ

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
1	Aldrin	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
2	Arsenic	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method[4] 2) Digestion, Inductively Coupled Plasma Method[4]
3	Barium	Digestion, Inductively Coupled Plasma Method[4]
4	α-BHC	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
5	β-BHC	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
6	δ-BHC	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
7	γ-BHC	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
8	Biochemical Oxygen Demand	1) 5-Day BOD Test, Azide Modification Method[4] 2) 5-Day BOD Test, Membrane Electrode Method[4]
9	Cadmium	1) Digestion, Direct Air-Acetylene Flame Method[4] 2) Digestion, Inductively Coupled Plasma Method[4]
10	Chemical Oxygen Demand	1) Closed Reflux, Titrimetric Method[4] 2) Closed Reflux, Colorimetric Method[4] 3) Open Reflux, Titrimetric Method[4]
11	Chlordane	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
12	Chromium	1) Digestion, Direct Air-Acetylene Flame Method[4] 2) Digestion, Inductively Coupled Plasma Method[4]
13	Color	ADMI Weighted-Ordinate Spectrophotometric Method[4]
14	Copper	1) Digestion, Direct Air-Acetylene Flame Method[4] 2) Digestion, Inductively Coupled Plasma Method[4]
15	Cyanide	1) Distillation, Colorimetric Method[4] 2) Total Cyanide after Distillation, by Flow Injection Analysis Method[4]
16	o,p'-DDT	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
17	4,4'-DDD	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
18	4,4'-DDE	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
19	4,4'-DDT	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
20	Dieldrin	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
21	Endosulfan I	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
22	Endosulfan II	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
23	Endosulfan sulfate	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
24	Endrin	Liquid-Liquid Extraction, Gas Chromatographic Method[4]

25 Endrin aldehyde...

ทะเบียนเลขที่ ว
ทะเบียนเลขที่ ว
ทะเบียนเลขที่ ว

น้ำใต้ดิน จำนวน 126 รายการ

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
1	Acenaphthene	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
2	Acetone	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
3	Aldrin	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
4	Anthracene	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
5	Antimony	Digestion, Inductively Coupled Plasma Method[4]
6	Arsenic	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method[4] 2) Digestion, Inductively Coupled Plasma Method[4]
7	Atrazine	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
8	Barium	Digestion, Inductively Coupled Plasma Method[4]
9	Benz(a)anthracene	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
10	Benzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
11	Benzo(b)fluoranthene	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
12	Benzo(k)fluoranthene	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
13	Benzoic acid	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]

UAE สำเนาถูกต้อง UNITED ANALYST AND ENGINEERING CONSULTANT COMPANY LIMITED

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
25	Endrin aldehyde	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
26	Formaldehyde	Distillation, Colorimetric Method[2]
27	Free Chlorine	1) Iodometric Method[4] 2) DPD Ferrous Titrimetric Method[4]
28	Heptachlor	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
29	Heptachlor Epoxide	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
30	Hexavalent Chromium	Colorimetric Method[4]
31	Lead	1) Digestion, Direct Air-Acetylene Flame Method[4] 2) Digestion, Inductively Coupled Plasma Method[4]
32	Manganese	1) Digestion, Direct Air-Acetylene Flame Method[4] 2) Digestion, Inductively Coupled Plasma Method[4]
33	Mercury	Digestion, Cold-Vapor Atomic Absorption Spectrometric Method[4]
34	Methoxychlor	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
35	Nickel	1) Digestion, Direct Air-Acetylene Flame Method[4] 2) Digestion, Inductively Coupled Plasma Method[4]
36	Oil & Grease	1) Liquid-Liquid, Partition-Gravimetric Method[4] 2) Soxhlet Extraction Method[4]
37	pH	Electrometric Method[4]
38	Phenols	1) Distillation, Chloroform Extraction Method[4] 2) Distillation, Direct Photometric Method[4]
39	Selenium	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method[4] 2) Digestion, Inductively Coupled Plasma Method[4]
40	Sulfide	1) Iodometric Method[4] 2) Methylene Blue Method[4]
41	Temperature	Laboratory and Field Methods[4]
42	Total Dissolved Solids	Dried at 180 °C[4]
43	Total Kjeldahl Nitrogen	Semi-Micro-Kjeldahl Method[4]
44	Total Suspended Solids	Dried from 103 to 105 °C[4]
45	Trivalent Chromium	1) Digestion, Direct Air-Acetylene Flame Method; Colorimetric Method; Calculation[4] 2) Digestion, Inductively Coupled Plasma Method; Colorimetric Method; Calculation[4]
46	Zinc	1) Digestion, Direct Air-Acetylene Flame Method[4] 2) Digestion, Inductively Coupled Plasma Method[4]

UAE สำเนาถูกต้อง UNITED ANALYST AND ENGINEERING CONSULTANT COMPANY LIMITED

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
14	Benzo(a)pyrene	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
15	Benzo(g,h,i)perylene	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
16	Beryllium	Digestion, Inductively Coupled Plasma Method[4]
17	Bis(2-chloroethyl)ether	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
18	Bis(2-ethylhexyl)phthalate	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
19	Bromodichloromethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
20	Bromoform	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
21	Butanol	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
22	Butyl benzyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
23	Cadmium	1) Digestion, Direct Air-Acetylene Flame Method[4] 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method[4] 3) Digestion, Inductively Coupled Plasma Method[4]
24	Carbazole	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
25	Carbon disulfide	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
26	Carbon tetrachloride	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
27	Chlordane	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
28	p-Chloroaniline	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]

LABS ACCREDITED ANALYST AND ENGINEERING CONSULTANT COMPANY LIMITED สำเนาถูกต้อง

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
29	Chlorobenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
30	Chlorodibromomethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
31	Chloroform	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
32	2-Chlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
33	Chromium	1) Digestion, Direct Air-Acetylene Flame Method[4] 2) Digestion, Inductively Coupled Plasma Method[4]
34	Chromium (III)	1) Digestion, Direct Air-Acetylene Flame Method; Colorimetric Method; Calculation[4] 2) Digestion, Inductively Coupled Plasma Method; Colorimetric Method; Calculation[4]
35	Chromium (VI)	Colorimetric Method[4]
36	Chrysene	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
37	Cyanide	Distillation, Colorimetric Method[4]
38	2,4-D	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
39	DDD	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
40	DDE	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
41	DDT	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
42	Dibenz(a,h)anthracene	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]

LABS ACCREDITED ANALYST AND ENGINEERING CONSULTANT COMPANY LIMITED สำเนาถูกต้อง

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
43	Di-n-butyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
44	1,2-Dichlorobenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
45	1,3-Dichlorobenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
46	1,4-Dichlorobenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
47	3,3′-Dichlorobenzidine	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
48	1,1-Dichloroethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
49	1,2-Dichloroethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
50	1,1-Dichloroethylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
51	cis-1,2-Dichloroethylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
52	trans-1,2-Dichloroethylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
53	2,4-Dichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
54	1,2-Dichloropropane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
55	1,3-Dichloropropane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
56	1,3-Dichloropropene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
57	Dieldrin	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
58	Diethyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
59	2,4-Dimethylphenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
60	2,4-Dinitrophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
61	2,4-Dinitrotoluene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
62	2,6-Dinitrotoluene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
63	Di-n-Octyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
64	Endosulfan	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
65	Endrin	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
66	Ethylbenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
67	Fluoranthene	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
68	Fluorene	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
69	Heptachlor	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
70	Heptachlor epoxide	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
71	Hexachlorobenzene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
72	Hexachloro-1,3-butadiene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
73	n-Hexane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]

MM-C39
น.18/85

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
74	α-HCH	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
75	β-HCH	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
76	γ-HCH	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
77	Hexachlorocyclopentadiene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
78	Hexachloroethane	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
79	Indeno(1,2,3-cd)pyrene	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
80	Isophorone	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
81	Lead	1) Digestion, Direct Air-Acetylene Flame Method[4] 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method[4] 3) Digestion, Inductively Coupled Plasma Method[4]
82	Manganese	1) Digestion, Direct Air-Acetylene Flame Method[4] 2) Digestion, Inductively Coupled Plasma Method[4]
83	Mercury	Digestion, Cold-Vapor Atomic Absorption Spectrometric Method[4]
84	Methanol	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
85	Methoxychlor	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
86	Methyl bromide	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
87	Methylene chloride	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
88	2-Methylphenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
89	2-Methylnaphthalene	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
90	Methyl tert-butyl ether	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
91	Naphthalene	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
92	Nickel	1) Digestion, Direct Air-Acetylene Flame Method[4] 2) Digestion, Inductively Coupled Plasma Method[4]
93	Nitrobenzene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
94	N-Nitrosodiphenylamine	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
95	N-Nitrosodi-n-propylamine	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
96	Polychlorinated Biphenyls - PCB 1016 - PCB 1221 - PCB 1232 - PCB-1242 - PCB-1248 - PCB-1254 - PCB-1260	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
97	Pentachlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
98	pH	Electrometric Method[4]
99	Phenanthrene	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]

KAE ANALYST AND ENGINEERING CONSULTANT COMPANY LIMITED สำเนาถูกต้อง

MM-C39

น.18/86

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
116	2,4,5-Trichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
117	2,4,6-Trichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
118	1,3,5-Trimethylbenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
119	Vanadium	Digestion, Inductively Coupled Plasma Method[4]
120	Vinyl acetate	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
121	Vinyl chloride	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
122	m-Xylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
123	o-Xylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
124	p-Xylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
125	Xylene (Total)	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
126	Zinc	1) Digestion, Direct Air-Acetylene Flame Method[4] 2) Digestion, Inductively Coupled Plasma Method[4]

<u>อากาศเสีย (ปล่องระบาย) จำนวน 25 รายการ</u>

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
1	Antimony	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5]
2	Arsenic	1) Isokinetic Sampling, Digestion, Hydride Generation/ Atomic Absorption Spectrometric Method[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5]
3	Cadmium	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5]
4	Carbon Monoxide	Instrumental Analyzer Method[5]
5	Chlorine	Isokinetic Sampling, Ion Chromatographic Method[5]
6	Chromium	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method[5]

Chromium (ต่อ)...

DAE สำเนาถูกต้อง
DAE CONSULTANT COMPANY LIMITED

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
100	Phenol	1) Distillation, Chloroform Extraction Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
101	Pyrene	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
102	Selenium	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method[4] 2) Digestion, Inductively Coupled Plasma Method[4]
103	Silver	Digestion, Inductively Coupled Plasma Method[4]
104	Styrene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
105	1,1,2,2-Tetrachloroethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
106	Tetrachloroethylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
107	Toluene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
108	Toxaphene	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
109	TPH (C_5 - C_8)	1) Purge and Trap, Gas Chromatographic Method[12,22] 2) Purge and Trap, Gas Chromatographic/Mass spectrometric Method[12,27]
110	TPH ($C_{>8}$ – C_{16})	Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[9,22]
111	TPH ($C_{>16}$ – C_{35})	Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[9,22]
112	1,2,4-Trichlorobenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
113	1,1,1-Trichloroethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
114	1,1,2-Trichloroethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
115	Trichloroethylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]

116 2,4,5-Trichlorophenol...

DAE สำเนาถูกต้อง
DAE CONSULTANT COMPANY LIMITED

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
6	Chromium (ต่อ)	2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5]
7	Cobalt	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5]
8	Copper	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5]
9	Cresol	Absorption Sampling, Gas Chromatographic Method[5]
10	Dioxins/Furans	Isokinetic Sampling[5]
11	Hydrogen Chloride	Isokinetic Sampling, Ion Chromatographic Method[5]
12	Hydrogen Fluoride	Isokinetic Sampling, Ion Chromatographic Method[5]
13	Hydrogen Sulfide	Absorption Sampling, Iodometric Method[5]
14	Lead	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5]
15	Manganese	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5]
16	Mercury	Isokinetic Sampling, Digestion, Cold-Vapor Atomic Absorption Spectrometric Method[5]
17	Nickel	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5]
18	Opacity	Ringelmann's Method[1]
19	Oxides of Nitrogen	1) Absorption Sampling, Phenoldisulfonic acid Method[5] 2) Instrumental Analyzer Method[5]
20	Selenium	1) Isokinetic Sampling, Digestion, Hydride Generation/ Atomic Absorption Spectrometric Method[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5]
21	Sulfur Dioxide	1) Absorption Sampling, Barium-Thorin Titrimetric Method[5] 2) Instrumental Analyzer Method[5]
22	Sulfuric Acid	Isokinetic Sampling, Barium-Thorin Titrimetric Method[5]

23 Total Suspended Particulate...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
23	Total Suspended Particulate	Isokinetic Sampling, Gravimetric Method[5]
24	Vanadium	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5]
25	Xylene	1) Bag Sampling, Gas Chromatographic Method[5] 2) Adsorption Sampling, Gas Chromatographic Method[5]

<u>สิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว จำนวน 35 รายการ</u>

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
1	Aldrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[3,9,23] 2) Ultrasonic Extraction, Gas Chromatographic Method[10,23]
2	Antimony	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[3,6,14] 2) Digestion, Inductively Coupled Plasma Method[7,14]
3	Arsenic	1) Waste Extraction, Digestion, Hydride Generation/ Atomic Absorption Spectrometric Method[3,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method[3,6,14] 3) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method[7,16] 4) Digestion, Inductively Coupled Plasma Method[7,14]
4	Barium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[3,6,14] 2) Digestion, Inductively Coupled Plasma Method[7,14]
5	Beryllium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[3,6,14] 2) Digestion, Inductively Coupled Plasma Method[7,14]
6	Cadmium	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method[3,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method[3,6,14] 3) Digestion, Flame Atomic Absorption Spectrometric Method[7,15] 4) Digestion, Inductively Coupled Plasma Method[7,14]
7	Chlordane	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[3,9,23] 2) Ultrasonic Extraction, Gas Chromatographic Method[10,23]

8 Chromium...

UAE UNITED ANALYST AND ENGINEERING CONSULTANT COMPANY LIMITED สำเนาถูกต้อง

MM-C39

น.18/88

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
8	Chromium	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method[3,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method[3,6,14] 3) Digestion, Flame Atomic Absorption Spectrometric Method[7,15] 4) Digestion, Inductively Coupled Plasma Method[7,14]
9	Chromium (III)	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method; Waste Extraction, Colorimetric Method; Calculation[3,6,15,17] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method; Waste Extraction, Colorimetric Method; Calculation[3,6,14,17] 3) Digestion, Flame Atomic Absorption Spectrometric Method; Alkaline Digestion, Colorimetric Method; Calculation[7,8,15,17] 4) Digestion, Inductively Coupled Plasma Method; Alkaline Digestion, Colorimetric Method; Calculation[7,8,14,17]
10	Chromium (VI)	1) Waste Extraction, Colorimetric Method[3,17] 2) Alkaline Digestion, Colorimetric Method[8,17]
11	Cobalt	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[3,6,14] 2) Digestion, Inductively Coupled Plasma Method[7,14]
12	Copper	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method[3,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method[3,6,14] 3) Digestion, Flame Atomic Absorption Spectrometric Method[7,15] 4) Digestion, Inductively Coupled Plasma Method[7,14]
13	2,4-D	1) Waste Extraction, Gas Chromatographic Method[3,26] 2) Ultrasonic Extraction, Gas Chromatographic Method[26]
14	DDD	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[3,9,23] 2) Ultrasonic Extraction, Gas Chromatographic Method[10,23]

15 DDE...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
15	DDE	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[3,9,23] 2) Ultrasonic Extraction, Gas Chromatographic Method[10,23]
16	DDT	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[3,9,23] 2) Ultrasonic Extraction, Gas Chromatographic Method[10,23]
17	Dieldrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[3,9,23] 2) Ultrasonic Extraction, Gas Chromatographic Method[10,23]
18	Endrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[3,9,23] 2) Ultrasonic Extraction, Gas Chromatographic Method[10,23]
19	Heptachlor	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[3,9,23] 2) Ultrasonic Extraction, Gas Chromatographic Method[10,23]
20	Lead	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method[3,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method[3,6,14] 3) Digestion, Flame Atomic Absorption Spectrometric Method[7,15] 4) Digestion, Inductively Coupled Plasma Method[7,14]
21	Lindane	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[3,9,23] 2) Ultrasonic Extraction, Gas Chromatographic Method[10,23]
22	Mercury	1) Waste Extraction, Digestion, Cold-Vapor Atomic Absorption Spectrometric Method[3,19] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method[3,6,14] 3) Digestion, Cold-Vapor Atomic Absorption Spectrometric Method[19] 4) Digestion, Inductively Coupled Plasma Method[7,14]

Mercury (ต่อ)...

ENVIRONMENTAL ANALYST AND ENGINEERING CONSULTANT COMPANY LIMITED
สำเนาถูกต้อง

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
22	Mercury (ต่อ)	5) Thermal Decomposition Amalgamation and Atomic Absorption Spectrometric Method[20]
23	Methoxychlor	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[3,9,23] 2) Ultrasonic Extraction, Gas Chromatographic Method[10,23]
24	Molybdenum	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[3,6,14] 2) Digestion, Inductively Coupled Plasma Method[7,14]
25	Nickel	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method[3,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method[3,6,14] 3) Digestion, Flame Atomic Absorption Spectrometric Method[7,15] 4) Digestion, Inductively Coupled Plasma Method[7,14]
26	Polychlorinated Biphenyls - Aroclor 1016 - Aroclor 1221 - Aroclor 1232 - Aroclor 1242 - Aroclor 1248 - Aroclor 1254 - Aroclor 1260 - 2-Chlorobiphenyl - 2,3-Dichlorobiphenyl - 2,2',5-Trichlorobiphenyl - 2,4',5-Trichlorobiphenyl - 2,2',3,5'-Tetrachlorobiphenyl - 2,2',5,5'-Tetrachlorobiphenyl - 2,3',4,4'-Tetrachlorobiphenyl - 2,2',3,4,5'-Pentachlorobiphenyl - 2,2',4,5,5'-Pentachlorobiphenyl - 2,3,3',4',6-Pentachlorobiphenyl	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[3,9,24] 2) Ultrasonic Extraction, Gas Chromatographic Method[10,24]

UAE UNITED ANALYST AND ENGINEERING CONSULTANT COMPANY LIMITED สำเนาถูกต้อง

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
	Polychlorinated Biphenyls(ต่อ) - 2,2',3,4,4',5'-Hexachlorobiphenyl - 2,2',3,4,5,5'-Hexachlorobiphenyl - 2,2',3,5,5',6-Hexachlorobiphenyl - 2,2',4,4',5,5'-Hexachlorobiphenyl - 2,2',3,3',4,4',5-Heptachlorobiphenyl - 2,2',3,4,4',5,5'-Heptachlorobiphenyl - 2,2',3,4,4',5',6-Heptachlorobiphenyl - 2,2',3,4',5,5',6-Heptachlorobiphenyl - 2,2',3,3',4,4',5,5',6-Nonachlorobiphenyl	
27	Pentachlorophenol	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[3,9,28] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
28	pH	Electrometric Method[31,32]
29	Selenium	1) Waste Extraction, Digestion, Hydride Generation/Atomic Absorption Spectrometric Method[3,6,21] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method[3,6,14] 3) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method[7,21] 4) Digestion, Inductively Coupled Plasma Method[7,14]
30	Silver	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[3,6,14] 2) Digestion, Inductively Coupled Plasma Method[7,14]
31	Thallium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[3,6,14] 2) Digestion, Inductively Coupled Plasma Method[7,14]

UAE UNITED ANALYST AND ENGINEERING CONSULTANT COMPANY LIMITED สำเนาถูกต้อง

MM-C39
น.18/90

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
32	Toxaphene	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[3,9,23] 2) Ultrasonic Extraction, Gas Chromatographic Method[10,23]
33	Trichloroethylene	1) Waste Extraction, Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[3,12,27] 2) Waste Extraction, Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method[3,11,27] 3) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,27] 4) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method[11,27]
34	Vanadium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[3,6,14] 2) Digestion, Inductively Coupled Plasma Method[7,14]
35	Zinc	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method[3,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method[3,6,14] 3) Digestion, Flame Atomic Absorption Spectrometric Method[7,15] 4) Digestion, Inductively Coupled Plasma Method[7,14]

ดิน จำนวน 125 รายการ

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
1	Acenaphthene	1) Ultrasonic Extraction, Gas Chromatographic Method[10,25] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
2	Acetone	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,27]
3	Aldrin	1) Ultrasonic Extraction, Gas Chromatographic Method[10,23] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
4	Anthracene	1) Ultrasonic Extraction, Gas Chromatographic Method[10,25]

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
4	Anthracene (ต่อ)	2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
5	Antimony	Digestion, Inductively Coupled Plasma Method[7,14]
6	Arsenic	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method[7,16] 2) Digestion, Inductively Coupled Plasma Method[7,14]
7	Atrazine	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
8	Barium	Digestion, Inductively Coupled Plasma Method[7,14]
9	Benz(a)anthracene	1) Ultrasonic Extraction, Gas Chromatographic Method[10,25] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
10	Benzene	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,27] 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method [11,27]
11	Benzo(b)fluoranthene	1) Ultrasonic Extraction, Gas Chromatographic Method[10,25] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
12	Benzo(k)fluoranthene	1) Ultrasonic Extraction, Gas Chromatographic Method[10,25] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
13	Benzoic acid	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
14	Benzo(a)pyrene	1) Ultrasonic Extraction, Gas Chromatographic Method[10,25] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
15	Benzo(g,h,i)perylene	1) Ultrasonic Extraction, Gas Chromatographic Method[10,25] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
16	Beryllium	Digestion, Inductively Coupled Plasma Method[7,14]

UAE UNITED ANALYST AND ENGINEERING CONSULTANT COMPANY LIMITED สำเนาถูกต้อง

MM-C39

น.18/91

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
17	Bis(2-chloroethyl)ether	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
18	Bis(2-ethylhexyl)phthalate	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
19	Bromodichloromethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,27]
20	Bromoform	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,27]
21	Butanol	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,27]
22	Butyl benzyl phthalate	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
23	Cadmium	1) Digestion, Flame Atomic Absorption Spectrometric Method[7,15] 2) Digestion, Inductively Coupled Plasma Method[7,14]
24	Carbazole	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
25	Carbon disulfide	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,27]
26	Carbon tetrachloride	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,27] 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method[11,27]
27	Chlordane	1) Ultrasonic Extraction, Gas Chromatographic Method[10,23] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
28	p-Chloroaniline	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
29	Chlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,27]
30	Chlorodibromomethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,27]
31	Chloroform	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,27]
32	2-Chlorophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
33	Chromium	1) Digestion, Flame Atomic Absorption Spectrometric Method[7,15] 2) Digestion, Inductively Coupled Plasma Method[7,14]
34	Chromium (III)	1) Digestion, Flame Atomic Absorption Spectrometric Method; Alkaline Digestion, Colorimetric Method; Calculation[7,8,15,17] 2) Digestion, Inductively Coupled Plasma Method; Alkaline Digestion, Colorimetric Method; Calculation[7,8,14,17]
35	Chromium (VI)	Alkaline Digestion, Colorimetric Method[8,17]
36	Chrysene	1) Ultrasonic Extraction, Gas Chromatographic Method[10,25] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
37	Cyanide	Extraction, Distillation, Colorimetric Method[29,30]
38	2,4-D	Ultrasonic Extraction, Gas Chromatographic Method[26]
39	DDD	1) Ultrasonic Extraction, Gas Chromatographic Method[10,23] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
40	DDE	1) Ultrasonic Extraction, Gas Chromatographic Method[10,23] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
41	DDT	1) Ultrasonic Extraction, Gas Chromatographic Method[10,23] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
42	Dibenz(a,h)anthracene	1) Ultrasonic Extraction, Gas Chromatographic Method[10,25] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
43	Di-n-butyl phthalate	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
44	1,2-Dichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,27]

MM-C39
น.18/92

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
45	1,3-Dichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,27]
46	1,4-Dichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,27]
47	3,3'-Dichlorobenzidine	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
48	1,1-Dichloroethane	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,27] 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method [11,27]
49	1,2-Dichloroethane	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,27] 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method [11,27]
50	1,1-Dichloroethylene	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,27] 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method [11,27]
51	cis-1,2-Dichloroethylene	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,27] 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method [11,27]
52	trans-1,2-Dichloroethylene	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,27] 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method [11,27]
53	2,4-Dichlorophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
54	1,2-Dichloropropane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,27]
55	1,3-Dichloropropane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,27]
56	1,3-Dichloropropene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,27]
57	Dieldrin	1) Ultrasonic Extraction, Gas Chromatographic Method[10,23] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]

58 Diethyl phthalate...

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
58	Diethyl phthalate	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
59	2,4-Dimethylphenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
60	2,4-Dinitrophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
61	2,4-Dinitrotoluene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
62	2,6-Dinitrotoluene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
63	Di-n-Octyl phthalate	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
64	Endosulfan	1) Ultrasonic Extraction, Gas Chromatographic Method[10,23] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
65	Endrin	1) Ultrasonic Extraction, Gas Chromatographic Method[10,23] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
66	Ethylbenzene	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,27] 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method [11,27]
67	Fluoranthene	1) Ultrasonic Extraction, Gas Chromatographic Method[10,25] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
68	Fluorene	1) Ultrasonic Extraction, Gas Chromatographic Method[10,25] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
69	Heptachlor	1) Ultrasonic Extraction, Gas Chromatographic Method[10,23] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
70	Heptachlor epoxide	1) Ultrasonic Extraction, Gas Chromatographic Method[10,23]

Heptachlor epoxide (ต่อ)...

UNITED ANALYST AND ENGINEERING CONSULTANT COMPANY LIMITED สำเนาถูกต้อง

MM-C39

น.18/93

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
70	Heptachlor epoxide (ต่อ)	2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
71	Hexachlorobenzene	1) Ultrasonic Extraction, Gas Chromatographic Method[10,23] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
72	Hexachloro-1,3-butadiene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,27]
73	n-Hexane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,27]
74	α-HCH	1) Ultrasonic Extraction, Gas Chromatographic Method[10,23] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
75	β-HCH	1) Ultrasonic Extraction, Gas Chromatographic Method[10,23] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
76	γ-HCH	1) Ultrasonic Extraction, Gas Chromatographic Method[10,23] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
77	Hexachlorocyclopentadiene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
78	Hexachloroethane	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
79	Indeno(1,2,3-cd)pyrene	1) Ultrasonic Extraction, Gas Chromatographic Method[10,25] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
80	Isophorone	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
81	Lead	1) Digestion, Flame Atomic Absorption Spectrometric Method[7,15] 2) Digestion, Inductively Coupled Plasma Method[7,14]
82	Manganese	1) Digestion, Flame Atomic Absorption Spectrometric Method[7,15] 2) Digestion, Inductively Coupled Plasma Method[7,14]

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
83	Mercury	1) Digestion, Cold-Vapor Atomic Absorption Spectrometric Method[19] 2) Thermal Decomposition Amalgamation and Atomic Absorption Spectrometric Method[20]
84	Methanol	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,27]
85	Methoxychlor	1) Ultrasonic Extraction, Gas Chromatographic Method[10,23] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
86	Methyl bromide	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,27]
87	Methylene chloride	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,27] 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method [11,27]
88	2-Methylphenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
89	2-Methylnaphthalene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
90	Methyl tert-butyl ether	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,27]
91	Naphthalene	1) Ultrasonic Extraction, Gas Chromatographic Method[10,25] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
92	Nickel	1) Digestion, Flame Atomic Absorption Spectrometric Method[7,15] 2) Digestion, Inductively Coupled Plasma Method[7,14]
93	Nitrobenzene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
94	N-Nitrosodiphenylamine	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
95	N-Nitrosodi-n-propylamine	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
96	Polychlorinated Biphenyls - Aroclor 1016	1) Ultrasonic Extraction, Gas Chromatographic Method[10,24]

MM-C39
น.18/94

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
96	Polychlorinated Biphenyls(ต่อ) - Aroclor 1221 - Aroclor 1232 - Aroclor 1242 - Aroclor 1248 - Aroclor 1254	2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
	- Aroclor 1260	Ultrasonic Extraction, Gas Chromatographic Method[10,24]
	Polychlorinated Biphenyls - 2-Chlorobiphenyl - 2,3-Dichlorobiphenyl - 2,2',5-Trichlorobiphenyl - 2,4',5-Trichlorobiphenyl - 2,2',3,5'-Tetrachlorobiphenyl - 2,2',5,5'-Tetrachlorobiphenyl - 2,3',4,4'-Tetrachlorobiphenyl - 2,2',3,4,5'-Pentachlorobiphenyl - 2,2',4,5,5'-Pentachlorobiphenyl - 2,3,3',4',6-Pentachlorobiphenyl - 2,2',3,4,4',5'-Hexachlorobiphenyl - 2,2',3,4,5,5'-Hexachlorobiphenyl - 2,2',3,5,5',6-Hexachlorobiphenyl - 2,2',4,4',5,5'-Hexachlorobiphenyl - 2,2',3,3',4,4',5-Heptachlorobiphenyl - 2,2',3,4,4',5,5'-Heptachlorobiphenyl - 2,2',3,4,4',5',6-Heptachlorobiphenyl - 2,2',3,4',5,5',6-Heptachlorobiphenyl - 2,2',3,3',4,4',5,5',6-Nonachlorobiphenyl	

UAE UNITED ANALYST AND ENGINEERING CONSULTANT COMPANY LIMITED สำเนาถูกต้อง

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
97	Pentachlorophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
98	Phenanthrene	1) Ultrasonic Extraction, Gas Chromatographic Method[10,25] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
99	Phenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
100	Pyrene	1) Ultrasonic Extraction, Gas Chromatographic Method[10,25] 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
101	Selenium	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method[7,21] 2) Digestion, Inductively Coupled Plasma Method[7,14]
102	Silver	Digestion, Inductively Coupled Plasma Method[7,14]
103	Styrene	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,27] 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method[11,27]
104	1,1,2,2-Tetrachloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,27]
105	Tetrachloroethylene	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,27] 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method[11,27]
106	Toluene	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,27] 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method[11,27]
107	Toxaphene	Ultrasonic Extraction, Gas Chromatographic Method[10,23]
108	TPH (C_5-C_8)	1) Purge and Trap, Gas Chromatographic Meth[illegible] 2) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,22]
109	TPH ($C_{>8}$-C_{16})	Ultrasonic Extraction, Gas Chromatographic Method[10,22]
110	TPH ($C_{>16}$-C_{35})	Ultrasonic Extraction, Gas Chromatographic Method[10,22]

UAE UNITED ANALYST AND ENGINEERING CONSULTANT COMPANY LIMITED สำเนาถูกต้อง

MM-C39
น.18/95

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
111	1,2,4-Trichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,27]
112	1,1,1-Trichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,27]
113	1,1,2-Trichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,27]
114	Trichloroethylene	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,27] 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method[11,27]
115	2,4,5-Trichlorophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
116	2,4,6-Trichlorophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[10,28]
117	1,3,5-Trimethylbenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,27]
118	Vanadium	Digestion, Inductively Coupled Plasma Method[7,14]
119	Vinyl acetate	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,27]
120	Vinyl chloride	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,27]
121	m-Xylene	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,27] 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method[11,27]
122	o-Xylene	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,27] 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method[11,27]
123	p-Xylene	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,27] 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method[11,27]
124	Xylene (Total)	1) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,27] 2) Equilibrium Headspace, Gas Chromatographic/Mass Spectrometric Method[11,27]

ลำดับ	สารมลพิษ	วิธีวิเคราะห์
125	Zinc	1) Digestion, Flame Atomic Absorption Spectrometric Method[7,15] 2) Digestion, Inductively Coupled Plasma Method[7,14]

เอกสารอ้างอิง

1. กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2549. เรื่อง กำหนดค่าปริมาณเขม่าควันที่เจือปนในอากาศที่ระบายออกจากปล่องของหม้อน้ำโรงสีข้าวที่ใช้แกลบเป็นเชื้อเพลิง. **ราชกิจจานุเบกษา.** 4 ธันวาคม 2549. เล่มที่ 123 ตอนพิเศษ 125ง.

2. สมาคมวิศวกรรมสิ่งแวดล้อมแห่งประเทศไทย. **คู่มือวิเคราะห์น้ำเสีย.** พิมพ์ครั้งที่ 4. กรุงเทพฯ: เรือนแก้วการพิมพ์, 2547.

3. กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2566. เรื่อง การจัดการสิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว.**ราชกิจจานุเบกษา.** 31 พฤษภาคม 2566. เล่มที่ 140 ตอนพิเศษ 126 ง.

4. APHA, AWWA, WEF. **Standard Methods for the Examination of Water and Wastewater.** 24th ed. Washington, DC: APHA, 2023.

5. United States Environmental Protection Agency. **Standards of Performance for New Stationary Sources.** 40 CFR 60. Appendix A, 2020.

6. United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods. SW-846,** 2014.

7. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Acid Digestion of Sediments, Sludges, and Soils. SW-846 Method 3050B,** 1996.

8. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Alkaline Digestion for Hexavalent Chromium. SW-846 Method 3060A,** 1996.

9. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste 3. Physical/Chemical Methods. **Separatory Funnel Liquid-Liquid Extraction. SW-846 Method 3510C,** 1996.

10. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Ultrasonic Extraction. SW-846 Method 3550C,** 2007.

11. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Volatile Organic Compounds in Various Sample Matrices Using Equilibrium Headspace Analysis. SW-846 Method 5021A,** 2014.

12. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Purge and Trap for Aqueous Samples. SW-846 Method 5030C,** 2003.

13. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Closed System Purge and Trap and Extraction for Volatile Organics in Soil and Waste Sample. SW-846 Method 5035A,** 2000.

สำเนาถูกต้อง
UNITED ANALYST AND ENGINEERING CONSULTANT COMPANY LIMITED

MM-C39
น.18/96

27. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Volatile Organic Compounds by Gas Chromatography/ Mass Spectrometry. SW-846 Method 8260D**, 2018.

28. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Semivolatile Organic Compounds by Gas Chromatography/Mass Spectrometry. SW-846 Method 8270E**, 2018.

29. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Cyanide Extraction Procedure for Solids and Oils. SW-846 Method 9013A**, 2014.

30. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Cyanide in Waters and Extracts using Titrimetric and Manual Spectrophotometric Procedures. SW-846 Method 9014**, 2014.

31. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **pH Electrometric Measurement. SW-846 Method 9040C**, 2004.

32. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Soil and Waste pH. SW-846 Method 9045D**, 2004.

UAE UNITED ANALYST AND ENGINEERING CONSULTANT COMPANY LIMITED สำเนาถูกต้อง

14. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Inductively Coupled Plasma-Optical Emission Spectrometry. SW-846 Method 6010D**, 2014.

15. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Flame Atomic Absorption Spectrophotometry. SW-846 Method 7000B**, 2007.

16. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Arsenic (Atomic Absorption, Gaseous Hydride). SW-846 Method 7061A**, 1992.

17. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Chromium, Hexavalent (Colorimetric). SW-846 Method 7196A**, 1992.

18. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Mercury in Liquid Waste (Manual Cold Vapor Technique). SW-846 Method 7470A**, 1994.

19. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Mercury in Solid or Semisolid Waste (Manual Cold-Vapor Technique). SW-846 Method 7471B**, 1998.

20. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Mercury in Solids and Solutions by Thermal Decomposition, Amalgamation, and Atomic Absorption Spectrophotometry. SW-846 Method 7473**, 2007.

21. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Selenium (Atomic Absorption, Borohydride Reduction). SW-846 Method 7742**, 1994.

22. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Nonhalogenated Organics Using GC/FID. SW-846 Method 8015D**, 2003.

23. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Organochlorine Pesticides by Gas Chromatography. SW-846 Method 8081B**, 2007.

24. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Polychlorinated Biphenyls (PCBs) by Gas Chromatography. SW-846 Method 8082A**, 2007.

25. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Organochlorine Pesticides by Gas Chromatography. SW-846 Method 8081B**, 2007.

26. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Chlorinated Herbicides by GC Using Methylation or Pentafluorobenzylation Derivertization. SW-846 Method 8151A**, 1996.

UAE UNITED ANALYST AND ENGINEERING CONSULTANT COMPANY LIMITED สำเนาถูกต้อง

MM-C39

น.18/97