ภาคผนวก ค

ใบรับรองผลการตรวจวัดคุณภาพสิ่งแวดล้อม

โครงการโรงงานผลิตสารโพลีออล (ส่วนขยาย ครั้งที่ 2)

ภาคผนวก ค-1

ผลการตรวจวัดสารอินทรีย์ระเหยในบรรยากาศ

Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong
Thailand 21130
P/O :
Project Name : Environmental Quality Monitoring
Project Location : AIE_Rigid Polyol Plant

Lot ID: 25114101
Date Received : Jan 06, 2026
Date Reported : Jan 13, 2026
Report Number : 3476747-1C15

Sample Number	25114101-1
Sampled Date	Jan 05, 2026
Sample Description	Air Quality
Location	ชุมชนประชุมมิตรบำรุง (GPS 47P 0726469, 1407406)
Date Analysis Commenced	Jan 07, 2026
Condition of Sample	Drawn into one 6-L Canister, one amber plastic bottle and one sorbent tube, refrigerated
Barometric Pressure	759 mmHg
Atmospheric Temperature	30.5 °C

Analyte	Sampled Date/time	Unit	LOD	LOQ (LOR)	Result	Guideline Limit	Method	Guideline	Testing Location
Air Testing									
Propylene Oxide	05/01/26 - 06/01/26	ug/m3	1.2	14	Not Detected	No Standard	Based on NIOSH, 1612	-	Bangkok

Guideline :
NEB : Notification of National Environment Board, B.E. 2560 (2017)
PCD : Notification of the Pollution Control Department, which was published in the Royal Government Gazette Vol. 126 Special Part 13 D dated January 27, B.E. 2552 (2009)
Note : Prachum Mit Bamrung Community station has moderate traffic. Normal activity, Clare sky, Nearby school, templel and comunity

Sampled By : Satcha Phetsawaeng

Remark :
- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any form without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

Approved by
Chontichak.
Chonticha Subongkoch
Scientist (3)

Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong
Thailand 21130
P/O :
Project Name : Environmental Quality Monitoring
Project Location : AIE_Rigid Polyol Plant

Lot ID: 25114101
Date Received : Jan 06, 2026
Date Reported : Jan 13, 2026
Report Number : 3476747-1C15

Sample Number	25114101-2
Sampled Date	Jan 05, 2026
Sample Description	Air Quality
Location	ชุมชนมาบชลูด (GPS 47P 0730823, 1407374)
Date Analysis Commenced	Jan 07, 2026
Condition of Sample	Drawn into one 6-L Canister, one amber plastic bottle and one sorbent tube, refrigerated
Barometric Pressure	759 mmHg
Atmospheric Temperature	30.5 °C

Analyte	Sampled Date/time	Unit	LOD	LOQ (LOR)	Result	Guideline Limit	Method	Guideline	Testing Location
Air Testing									
Propylene Oxide	05/01/26 - 06/01/26	ug/m3	1.2	14	Not Detected	No Standard	Based on NIOSH, 1612	-	Bangkok

Guideline :
NEB : Notification of National Environment Board, B.E. 2560 (2017)
PCD : Notification of the Pollution Control Department, which was published in the Royal Government Gazette Vol. 126 Special Part 13 D dated January 27, B.E. 2552 (2009)
Note : Map Cha Lood Community station has moderate traffic. Normal activity, Clare sky, Nearby temple, school and comunity

Sampled By : Satcha Phetsawaeng

Remark :
- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any form without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

Approved by
Chontichak.
Chonticha Subongkoch
Scientist (3)

ADDRESS 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand | PHONE +66 0 2760 3000 | FAX +66 0 2760 3197
Life Sciences www.alsglobal.com
RIGHT SOLUTIONS RIGHT PARTNER
8525-209/ EMAIL

Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong
Thailand 21130
P/O :
Project Name : Environmental Quality Monitoring
Project Location : AIE_Rigid Polyol Plant

Lot ID: 25114101
Date Received : Jan 06, 2026
Date Reported : Jan 13, 2026
Report Number : 3476747-1C15

Sample Number	25114101-3
Sampled Date	Jan 05, 2026
Sample Description	Air Quality
Location	ชุมชนพยูน (GPS 47P 0724371, 1402551)
Date Analysis Commenced	Jan 07, 2026
Condition of Sample	Drawn into one 6-L Canister, one amber plastic bottle and one sorbent tube, refrigerated
Barometric Pressure	759 mmHg
Atmospheric Temperature	30.5 °C

Analyte	Sampled Date/time	Unit	LOD	LOQ (LOR)	Result	Guideline Limit	Method	Guideline	Testing Location
Air Testing									
Propylene Oxide	05/01/26 - 06/01/26	ug/m3	1.2	14	Not Detected	No Standard	Based on NIOSH, 1612	-	Bangkok

Guideline :
NEB : Notification of National Environment Board, B.E. 2560 (2017)
PCD : Notification of the Pollution Control Department, which was published in the Royal Government Gazette Vol. 126 Special Part 13 D dated January 27, B.E. 2552 (2009)
Note : Pa Yoon Community station has moderate traffic. Normal activity, Clare sky, Nearby temple, school and comunity

Sampled By : Satcha Phetsawaeng

Remark :
- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any form without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

Approved by
Chontichak.
Chonticha Subongkoch
Scientist (3)

Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong
Thailand 21130
P/O :
Project Name : Environmental Quality Monitoring
Project Location : AIE_Rigid Polyol Plant

Lot ID: 265877
Date Received : Feb 03, 2026
Date Reported : Feb 11, 2026
Report Number : 3491517-1C15

Sample Number	265877-1
Sampled Date	Feb 02, 2026
Sample Description	Air Quality
Location	ชุมชนประชุมมิตรบำรุง (GPS 47P 0726469, 1407406)
Date Analysis Commenced	Feb 04, 2026
Condition of Sample	Drawn into one 6-L Canister, one amber plastic bottle and one sorbent tube, refrigerated
Barometric Pressure	756 mmHg
Atmospheric Temperature	31.7 °C

Analyte	Sampled Date/time	Unit	LOD	LOQ (LOR)	Result	Guideline Limit	Method	Guideline	Testing Location
Air Testing									
Propylene Oxide	02/02/26 - 03/02/26	ug/m3	1.2	14.0	Not Detected	No Standard	Based on NIOSH, 1612	-	Bangkok

Guideline :
NEB : Notification of National Environment Board, B.E. 2560 (2017)
PCD : Notification of the Pollution Control Department, which was published in the Royal Government Gazette Vol. 126 Special Part 13 D dated January 27, B.E. 2552 (2009)
Note : Prachum Mit Bamrung Community station has moderate traffic. Normal activity, Clare sky, Nearby school, templel and comunity

Sampled By : Ronnachai Moungma

Remark :
- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any form without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

Approved by
Tanyatorn Mongkonjirawut
Supervisor

Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong
Thailand 21130
P/O :
Project Name : Environmental Quality Monitoring
Project Location : AIE_Rigid Polyol Plant

Lot ID: 265877
Date Received : Feb 03, 2026
Date Reported : Feb 11, 2026
Report Number : 3491517-1C15

Sample Number	265877-2
Sampled Date	Feb 02, 2026
Sample Description	Air Quality
Location	ชุมชนมาบชลุด (GPS 47P 0730823, 1407374)
Date Analysis Commenced	Feb 04, 2026
Condition of Sample	Drawn into one 6-L Canister, one amber plastic bottle and one sorbent tube, refrigerated
Barometric Pressure	756 mmHg
Atmospheric Temperature	31.7 °C

Analyte	Sampled Date/time	Unit	LOD	LOQ (LOR)	Result	Guideline Limit	Method	Guideline	Testing Location
Air Testing									
Propylene Oxide	02/02/26 - 03/02/26	ug/m3	1.2	14.0	Not Detected	No Standard	Based on NIOSH, 1612	-	Bangkok

Guideline :
NEB : Notification of National Environment Board, B.E. 2560 (2017)
PCD : Notification of the Pollution Control Department, which was published in the Royal Government Gazette Vol. 126 Special Part 13 D dated January 27, B.E. 2552 (2009)
Note : Map Cha Lood Community station has moderate traffic. Normal activity, Clare sky, Nearby temple, school and comunity

Sampled By : Ronnachai Moungma

Remark :
- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any form without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

Approved by
Tanyatorn Mongkonjirawut
Supervisor

Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong
Thailand 21130
P/O :
Project Name : Environmental Quality Monitoring
Project Location : AIE_Rigid Polyol Plant

Lot ID: 265877
Date Received : Feb 03, 2026
Date Reported : Feb 11, 2026
Report Number : 3491517-1C15

Sample Number	265877-3
Sampled Date	Feb 02, 2026
Sample Description	Air Quality
Location	ชุมชนพยูน (GPS 47P 0724371, 1402551)
Date Analysis Commenced	Feb 04, 2026
Condition of Sample	Drawn into one 6-L Canister, one amber plastic bottle and one sorbent tube, refrigerated
Barometric Pressure	756 mmHg
Atmospheric Temperature	31.7 °C

Analyte	Sampled Date/time	Unit	LOD	LOQ (LOR)	Result	Guideline Limit	Method	Guideline	Testing Location
Air Testing									
Propylene Oxide	02/02/26 - 03/02/26	ug/m3	1.2	14.0	Not Detected	No Standard	Based on NIOSH, 1612	-	Bangkok

Guideline :
NEB : Notification of National Environment Board, B.E. 2560 (2017)
PCD : Notification of the Pollution Control Department, which was published in the Royal Government Gazette Vol. 126 Special Part 13 D dated January 27, B.E. 2552 (2009)
Note : Pa Yoon Community station has moderate traffic. Normal activity, Clare sky, Nearby temple, school and comunity

Sampled By : Ronnachai Moungma

Remark :
- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any form without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

Approved by
Tanyatorn Mongkonjirawut
Supervisor

ADDRESS 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand | PHONE +66 0 2760 3000 | FAX +66 0 2760 3197
Life Sciences www.alsglobal.com
RIGHT SOLUTIONS RIGHT PARTNER
8525-209/ EMAIL

Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong
Thailand 21130
P/O :
Project Name : Environmental Quality Monitoring
Project Location : AIE_Rigid Polyol Plant

Lot ID: 2612659
Date Received : Mar 05, 2026
Date Reported : Mar 17, 2026
Report Number : 3504435-1C15

Sample Number	2612659-1
Sampled Date	Mar 04, 2026
Sample Description	Air Quality
Location	ชุมชนประชุมมิตรบำรุง (GPS N 12.707927, E 101.084329)
Date Analysis Commenced	Mar 06, 2026
Condition of Sample	Drawn into one 6-L Canister, one amber plastic bottle and one sorbent tube, refrigerated
Barometric Pressure	757 mmHg
Atmospheric Temperature	33.4 °C

Analyte	Sampled Date/time	Unit	LOD	LOQ (LOR)	Result	Guideline Limit	Method	Guideline	Testing Location
Air Testing									
Propylene Oxide	04/03/26 - 05/03/26	ug/m3	1.2	14	Not Detected	No Standard	Based on NIOSH, 1612	-	Bangkok

Guideline :
NEB : Notification of National Environment Board, B.E. 2560 (2017)
PCD : Notification of the Pollution Control Department, which was published in the Royal Government Gazette Vol. 126 Special Part 13 D dated January 27, B.E. 2552 (2009)
Note : Prachum Mit Bamrung Community station has moderate traffic. Normal activity, Clare sky, Nearby school, templel and comunity

Sampled By : Saknarin Jaraskay

Remark :
- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

Approved by
Tanyatorn Mongkonjirawut
Supervisor

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any form without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong
Thailand 21130
P/O :
Project Name : Environmental Quality Monitoring
Project Location : AIE_Rigid Polyol Plant

Lot ID: 2612659
Date Received : Mar 05, 2026
Date Reported : Mar 17, 2026
Report Number : 3504435-1C15

Sample Number	2612659-2
Sampled Date	Mar 04, 2026
Sample Description	Air Quality
Location	ชุมชนมาบชลูด (GPS N 12.722340, E 101.125769)
Date Analysis Commenced	Mar 06, 2026
Condition of Sample	Drawn into one 6-L Canister, one amber plastic bottle and one sorbent tube, refrigerated
Barometric Pressure	757 mmHg
Atmospheric Temperature	34.6 °C

Analyte	Sampled Date/time	Unit	LOD	LOQ (LOR)	Result	Guideline Limit	Method	Guideline	Testing Location
Air Testing									
Propylene Oxide	04/03/26 - 05/03/26	ug/m3	1.2	14	Not Detected	No Standard	Based on NIOSH, 1612	-	Bangkok

Guideline :
NEB : Notification of National Environment Board, B.E. 2560 (2017)
PCD : Notification of the Pollution Control Department, which was published in the Royal Government Gazette Vol. 126 Special Part 13 D dated January 27, B.E. 2552 (2009)
Note : Map Cha Lood Community station has moderate traffic. Normal activity, Clare sky, Nearby temple, school and comunity

Sampled By : Saknarin Jaraskay

Remark :
- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

Approved by
Tanyatorn Mongkonjirawut
Supervisor

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any form without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

ADDRESS 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand | PHONE +66 0 2760 3000 | FAX +66 0 2760 3197
Life Sciences www.alsglobal.com
RIGHT SOLUTIONS RIGHT PARTNER
8525-209/ EMAIL

Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong
Thailand 21130
P/O :
Project Name : Environmental Quality Monitoring
Project Location : AIE_Rigid Polyol Plant

Lot ID: 2612659
Date Received : Mar 05, 2026
Date Reported : Mar 17, 2026
Report Number : 3504435-1C15

Sample Number	2612659-3
Sampled Date	Mar 04, 2026
Sample Description	Air Quality
Location	ชุนชนพยูน (GPS N 12.679224, E 101.066117)
Date Analysis Commenced	Mar 06, 2026
Condition of Sample	Drawn into one 6-L Canister, one amber plastic bottle and one sorbent tube, refrigerated
Barometric Pressure	757 mmHg
Atmospheric Temperature	32.6 °C

Analyte	Sampled Date/time	Unit	LOD	LOQ (LOR)	Result	Guideline Limit	Method	Guideline	Testing Location
Air Testing									
Propylene Oxide	04/03/26 - 05/03/26	ug/m3	1.2	14	Not Detected	No Standard	Based on NIOSH, 1612	-	Bangkok

Guideline :
NEB : Notification of National Environment Board, B.E. 2560 (2017)
PCD : Notification of the Pollution Control Department, which was published in the Royal Government Gazette Vol. 126 Special Part 13 D dated January 27, B.E. 2552 (2009)
Note : Pa Yoon Community station has moderate traffic. Normal activity, Clare sky, Nearby temple, school and comunity

Sampled By : Saknarin Jaraskay

Remark :
- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

Approved by
Tanyatorn Mongkonjirawut
Supervisor

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any form without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong
Thailand 21130
P/O :
Project Name : Environmental Quality Monitoring
Project Location : AIE_Rigid Polyol Plant

Lot ID: 2625534
Date Received : Apr 02, 2026
Date Reported : Apr 16, 2026
Report Number : 3534195-1C15

Sample Number	2625534-1
Sampled Date	Apr 01, 2026
Sample Description	Air Quality
Location	ชุมชนประชุมมิตรบำรุง (GPS N 12.707927, E 101.084329)
Date Analysis Commenced	Apr 03, 2026
Condition of Sample	Drawn into one 6-L Canister, one amber plastic bottle and two sorbent tubes, refrigerated
Barometric Pressure	757 mmHg
Atmospheric Temperature	30.2 °C

Analyte	Sampled Date/time	Unit	LOD	LOQ (LOR)	Result	Guideline Limit	Method	Guideline	Testing Location
Air Testing									
Propylene Oxide	01/04/26 - 02/04/26	ug/m3	1.2	14	Not Detected	No Standard	Based on NIOSH, 1612	-	Bangkok

Guideline :
NEB : Notification of National Environment Board, B.E. 2560 (2017)
PCD : Notification of the Pollution Control Department, which was published in the Royal Government Gazette Vol. 126 Special Part 13 D dated January 27, B.E. 2552 (2009)
Note : Prachum Mit Bamrung Community station has moderate traffic. Normal activity, Cloudy, Nearby school, templel and comunity

Sampled By : Nantawat Sarin

Remark :
- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

Approved by
Tanyatorn Mongkonjirawut
Supervisor

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any form without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

ADDRESS 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand | PHONE +66 0 2760 3000 | FAX +66 0 2760 3197
Life Sciences www.alsglobal.com
RIGHT SOLUTIONS RIGHT PARTNER
8525-209/ EMAIL

Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong
Thailand 21130
P/O :
Project Name : Environmental Quality Monitoring
Project Location : AIE_Rigid Polyol Plant

Lot ID: 2625534
Date Received : Apr 02, 2026
Date Reported : Apr 16, 2026
Report Number : 3534195-1C15

Sample Number	2625534-2
Sampled Date	Apr 01, 2026
Sample Description	Air Quality
Location	ชุมชนมาบชลูด (GPS N 12.722340, E 101.125769)
Date Analysis Commenced	Apr 03, 2026
Condition of Sample	Drawn into one 6-L Canister, one amber plastic bottle and two sorbent tubes, refrigerated
Barometric Pressure	757 mmHg
Atmospheric Temperature	30.2 °C

Analyte	Sampled Date/time	Unit	LOD	LOQ (LOR)	Result	Guideline Limit	Method	Guideline	Testing Location
Air Testing									
Propylene Oxide	01/04/26 - 02/04/26	ug/m3	1.2	14	Not Detected	No Standard	Based on NIOSH, 1612	-	Bangkok

Guideline :
NEB : Notification of National Environment Board, B.E. 2560 (2017)
PCD : Notification of the Pollution Control Department, which was published in the Royal Government Gazette Vol. 126 Special Part 13 D dated January 27, B.E. 2552 (2009)
Note : Map Cha Lood Community station has moderate traffic. Normal activity, Cloudy, Nearby temple, school and comunity

Sampled By : Nantawat Sarin

Remark :
- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any form without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

Approved by
Tanyatorn Mongkonjirawut
Supervisor

Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong
Thailand 21130
P/O :
Project Name : Environmental Quality Monitoring
Project Location : AIE_Rigid Polyol Plant

Lot ID: 2625534
Date Received : Apr 02, 2026
Date Reported : Apr 16, 2026
Report Number : 3534195-1C15

Sample Number	2625534-3
Sampled Date	Apr 01, 2026
Sample Description	Air Quality
Location	ชุนชนพยูน (GPS N 12.679224, E 101.066117)
Date Analysis Commenced	Apr 03, 2026
Condition of Sample	Drawn into one 6-L Canister, one amber plastic bottle and one sorbent tube, refrigerated
Barometric Pressure	757 mmHg
Atmospheric Temperature	30.2 °C

Analyte	Sampled Date/time	Unit	LOD	LOQ (LOR)	Result	Guideline Limit	Method	Guideline	Testing Location
Air Testing									
Propylene Oxide	01/04/26 - 02/04/26	ug/m3	1.2	14	Not Detected	No Standard	Based on NIOSH, 1612	-	Bangkok

Guideline :
NEB : Notification of National Environment Board, B.E. 2560 (2017)
PCD : Notification of the Pollution Control Department, which was published in the Royal Government Gazette Vol. 126 Special Part 13 D dated January 27, B.E. 2552 (2009)
Note : Pa Yoon Community station has moderate traffic. Normal activity, Cloudy,Nearby temple, school and comunity

Sampled By : Nantawat Sarin

Remark :
- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any form without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

Approved by
Tanyatorn Mongkonjirawut
Supervisor

ADDRESS 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand | PHONE +66 0 2760 3000 | FAX +66 0 2760 3197
Life Sciences www.alsglobal.com
RIGHT SOLUTIONS RIGHT PARTNER
8525-209/ EMAIL

Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130
P/O :
Project Name : Environmental Quality Monitoring
Project Location : AIE_Rigid Polyol Plant

Lot ID: 2635222
Date Received : May 05, 2026
Date Reported : May 16, 2026
Report Number : 3558182-1C15

Sample Number	2635222-1
Sampled Date	May 04, 2026
Sample Description	Air Quality
Location	ชุมชนประชุมมิตรบำรุง (GPS N 12.707927, E 101.084329)
Date Analysis Commenced	May 06, 2026
Condition of Sample	Drawn into one 6-L Canister, one amber plastic bottle and one sorbent tube, refrigerated
Barometric Pressure	755 mmHg
Atmospheric Temperature	32.0 °C

Analyte	Sampled Date/time	Unit	LOD	LOQ (LOR)	Result	Guideline Limit	Method	Guideline	Testing Location
Air Testing									
Propylene Oxide	04/05/26 - 05/05/26	ug/m3	1.2	14	Not Detected	No Standard	Based on NIOSH, 1612	-	Bangkok

Guideline :
NEB : Notification of National Environment Board, B.E. 2560 (2017)
PCD : Notification of the Pollution Control Department, which was published in the Royal Government Gazette Vol. 126 Special Part 13 D dated January 27, B.E. 2552 (2009)
Note : Prachum Mit Bamrung Community station has moderate traffic. Normal activity, Heavy rain, Nearby school, templel and comunity.

Sampled By : Adisak Tarisoon

Remark :
- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

Approved by Chontichak.
Chonticha Subongkoch
Scientist (3)

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any form without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130
P/O :
Project Name : Environmental Quality Monitoring
Project Location : AIE_Rigid Polyol Plant

Lot ID: 2635222
Date Received : May 05, 2026
Date Reported : May 16, 2026
Report Number : 3558182-1C15

Sample Number	2635222-2
Sampled Date	May 04, 2026
Sample Description	Air Quality
Location	ชุมชนมาบชลูด (GPS N 12.722340, E 101.125769)
Date Analysis Commenced	May 06, 2026
Condition of Sample	Drawn into one 6-L Canister, one amber plastic bottle and one sorbent tube, refrigerated
Barometric Pressure	755 mmHg
Atmospheric Temperature	32.8 °C

Analyte	Sampled Date/time	Unit	LOD	LOQ (LOR)	Result	Guideline Limit	Method	Guideline	Testing Location
Air Testing									
Propylene Oxide	04/05/26 - 05/05/26	ug/m3	1.2	14	Not Detected	No Standard	Based on NIOSH, 1612	-	Bangkok

Guideline :
NEB : Notification of National Environment Board, B.E. 2560 (2017)
PCD : Notification of the Pollution Control Department, which was published in the Royal Government Gazette Vol. 126 Special Part 13 D dated January 27, B.E. 2552 (2009)
Note : Map Cha Lood Community station has moderate traffic. Normal activity, Heavy rain, Nearby temple, school and comunity.

Sampled By : Adisak Tarisoon

Remark :
- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

Approved by Chontichak.
Chonticha Subongkoch
Scientist (3)

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any form without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

ADDRESS 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand | PHONE +66 0 2760 3000 | FAX +66 0 2760 3197
Life Sciences www.alsglobal.com
RIGHT SOLUTIONS RIGHT PARTNER
8525-209/ EMAIL

Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong
Thailand 21130
P/O :
Project Name : Environmental Quality Monitoring
Project Location : AIE_Rigid Polyol Plant

Lot ID: 2635222
Date Received : May 05, 2026
Date Reported : May 16, 2026
Report Number : 3558182-1C15

Sample Number	2635222-3
Sampled Date	May 04, 2026
Sample Description	Air Quality
Location	ชุนชนพยูน (GPS N 12.679224, E 101.066117)
Date Analysis Commenced	May 06, 2026
Condition of Sample	Drawn into one 6-L Canister, one amber plastic bottle and one sorbent tube, refrigerated
Barometric Pressure	755 mmHg
Atmospheric Temperature	30.9 °C

Analyte	Sampled Date/time	Unit	LOD	LOQ (LOR)	Result	Guideline Limit	Method	Guideline	Testing Location
Air Testing									
Propylene Oxide	04/05/26 - 05/05/26	ug/m3	1.2	14	Not Detected	No Standard	Based on NIOSH, 1612	-	Bangkok

Guideline :
NEB : Notification of National Environment Board, B.E. 2560 (2017)
PCD : Notification of the Pollution Control Department, which was published in the Royal Government Gazette Vol. 126 Special Part 13 D dated January 27, B.E. 2552 (2009)
Note : Pa Yoon Community station has moderate traffic. Normal activity, Heavy rain, Nearby temple, school and comunity.

Sampled By : Adisak Tarisoon

Remark :
- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any form without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

Approved by Chontichak.
Chonticha Subongkoch
Scientist (3)

Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong
Thailand 21130
P/O :
Project Name : Environmental Quality Monitoring
Project Location : AIE_Rigid Polyol Plant

Lot ID: 2645061
Date Received : Jun 04, 2026
Date Reported : Jun 16, 2026
Report Number : 3578978-1C15

Sample Number	2645061-1
Sampled Date	Jun 02, 2026
Sample Description	Air Quality
Location	ชุมชนประชุมมิตรบำรุง (GPS N 12.707927, E 101.084329)
Date Analysis Commenced	Jun 04, 2026
Condition of Sample	Drawn into one 6-L Canister, one amber plastic bottle and one sorbent tube, refrigerated
Barometric Pressure	754 mmHg
Atmospheric Temperature	30.2 °C

Analyte	Sampled Date/time	Unit	LOD	LOQ (LOR)	Result	Guideline Limit	Method	Guideline	Testing Location
Air Testing									
Propylene Oxide	02/06/26 - 03/06/26	ug/m3	1.2	14	Not Detected	No Standard	Based on NIOSH, 1612	-	Bangkok

Guideline :
NEB 2017 : Notification of National Environmental Board, B.E. 2560 (2017)
PCD : Notification of the Pollution Control Department, which was published in the Royal Government Gazette Vol. 126 Special Part 13 D dated January 27, B.E. 2552 (2009)
Note : Prachum Mit Bamrung Community station has moderate traffic. Normal activity, Light rain, Nearby school, templel and comunity

Sampled By : Satcha Phetsawaeng

Remark :
- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any form without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

Approved by Orawan R.
Orawan Rakyong
Scientist (3)

Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong
Thailand 21130
P/O :
Project Name : Environmental Quality Monitoring
Project Location : AIE_Rigid Polyol Plant

Lot ID: 2645061
Date Received : Jun 04, 2026
Date Reported : Jun 16, 2026
Report Number : 3578978-1C15

Sample Number	2645061-2
Sampled Date	Jun 02, 2026
Sample Description	Air Quality
Location	ชุมชนมาบชลุด (GPS N 12.722340, E 101.125769)
Date Analysis Commenced	Jun 04, 2026
Condition of Sample	Drawn into one 6-L Canister, one amber plastic bottle and one sorbent tube, refrigerated
Barometric Pressure	754 mmHg
Atmospheric Temperature	30.2 °C

Analyte	Sampled Date/time	Unit	LOD	LOQ (LOR)	Result	Guideline Limit	Method	Guideline	Testing Location
Air Testing									
Propylene Oxide	02/06/26 - 03/06/26	ug/m3	1.2	14	Not Detected	No Standard	Based on NIOSH, 1612	-	Bangkok

Guideline :
NEB 2017 : Notification of National Environmental Board, B.E. 2560 (2017)
PCD : Notification of the Pollution Control Department, which was published in the Royal Government Gazette Vol. 126 Special Part 13 D dated January 27, B.E. 2552 (2009)
Note : Map Cha Lood Community station has moderate traffic. Normal activity, Light rain, Nearby temple, school and comunity

Sampled By : Satcha Phetsawaeng

Remark :
- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any form without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

Approved by
Orawan R.
Orawan Rakyong
Scientist (3)

Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong
Thailand 21130
P/O :
Project Name : Environmental Quality Monitoring
Project Location : AIE_Rigid Polyol Plant

Lot ID: 2645061
Date Received : Jun 04, 2026
Date Reported : Jun 16, 2026
Report Number : 3578978-1C15

Sample Number	2645061-3
Sampled Date	Jun 02, 2026
Sample Description	Air Quality
Location	ชุนชนพยูน (GPS N 12.679224, E 101.066117)
Date Analysis Commenced	Jun 04, 2026
Condition of Sample	Drawn into one 6-L Canister, one amber plastic bottle and one sorbent tube, refrigerated
Barometric Pressure	754 mmHg
Atmospheric Temperature	30.2 °C

Analyte	Sampled Date/time	Unit	LOD	LOQ (LOR)	Result	Guideline Limit	Method	Guideline	Testing Location
Air Testing									
Propylene Oxide	02/06/26 - 03/06/26	ug/m3	1.2	14	Not Detected	No Standard	Based on NIOSH, 1612	-	Bangkok

Guideline :
NEB 2017 : Notification of National Environmental Board, B.E. 2560 (2017)
PCD : Notification of the Pollution Control Department, which was published in the Royal Government Gazette Vol. 126 Special Part 13 D dated January 27, B.E. 2552 (2009)
Note : Pa Yoon Community station has moderate traffic. Normal activity, Light rain, Nearby temple, school and comunity

Sampled By : Satcha Phetsawaeng

Remark :
- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any form without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

Approved by
Orawan R.
Orawan Rakyong
Scientist (3)

ADDRESS 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand | PHONE +66 0 2760 3000 | FAX +66 0 2760 3197
Life Sciences www.alsglobal.com
RIGHT SOLUTIONS RIGHT PARTNER
8525-209/ EMAIL

ภาคผนวก ค-2

ผลการตรวจวัดคุณภาพอากาศในสถานประกอบการ

Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong
Thailand 21130
P/O : 4518158708
Project Name : Environmental Quality Monitoring
Project Location : AIE_DMC-Polyol Plant

Lot ID: 265919
Date Received : Feb 12, 2026
Date Reported : Feb 18, 2026
Report Number : 3491598-1

Sample Number	265919-1
Sampled Date	Feb 11, 2026
Sample Description	Air Quality
Location	หน่วยทำปฏิกิริยา
Date Analysis Commenced	Feb 13, 2026
Condition of Sample	Drawn into one sorbent tube, refrigerated
Barometric Pressure	759 mmHg
Atmospheric Temperature	29.7 °C

Analyte	Sampled Date/time	Unit	LOD	LOQ (LOR)	Result	Guideline Limit	Method	Guideline	Testing Location
Air Testing									
Propylene Oxide	09:40 AM - 11:40 AM	ppm	-	0.10	<0.10	100	NIOSH (1994), 1612	MOL	Bangkok

Guideline :
MOL : Announcement of the Department of Labour Protection and Welfare on Threshold Limit Values of Hazardous Chemical Substances Dated August 3, B.E. 2560 (2017)
Sampled By : Apichart Wilars

Remark :
- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

Approved by
Orawan Rakyong
Scientist (3)

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong
Thailand 21130
P/O : 4518158708
Project Name : Environmental Quality Monitoring
Project Location : AIE_DMC-Polyol Plant

Lot ID: 265919
Date Received : Feb 12, 2026
Date Reported : Feb 18, 2026
Report Number : 3491598-1

Sample Number	265919-2
Sampled Date	Feb 11, 2026
Sample Description	Air Quality
Location	หน่วยทำปฏิกิริยา
Personal Sampling	คุณไพรัช พักน้อย
Date Analysis Commenced	Feb 13, 2026
Condition of Sample	Drawn into one sorbent tube, refrigerated
Barometric Pressure	759 mmHg
Atmospheric Temperature	29.7 °C

Analyte	Sampled Date/time	Unit	LOD	LOQ (LOR)	Result	Guideline Limit	Method	Guideline	Testing Location
Air Testing									
Propylene Oxide	09:30 AM - 11:30 AM	ppm	-	0.10	<0.10	100	NIOSH (1994), 1612	MOL	Bangkok

Guideline :
MOL : Announcement of the Department of Labour Protection and Welfare on Threshold Limit Values of Hazardous Chemical Substances Dated August 3, B.E. 2560 (2017)
Sampled By : Apichart Wilars

Remark :
- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

Approved by
Orawan Rakyong
Scientist (3)

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand | PHONE +66 0 2760 3000 | FAX +66 0 2760 3197
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company
Life Sciences www.alsglobal.com
RIGHT SOLUTIONS RIGHT PARTNER
8525-81/ EMAIL

Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong
Thailand 21130
P/O : 4518158712
Project Name : Environmental Quality Monitoring
Project Location : AIE_Rigid Polyol Plant

Lot ID: 265926
Date Received : Feb 12, 2026
Date Reported : Feb 18, 2026
Report Number : 3491604-1

Sample Number	265926-1
Sampled Date	Feb 11, 2026
Sample Description	Air Quality
Location	หน่วยทำปฏิกิริยาของสายการผลิตที่ 2
Date Analysis Commenced	Feb 13, 2026
Condition of Sample	Drawn into one sorbent tube, refrigerated
Barometric Pressure	759 mmHg
Atmospheric Temperature	29.7 °C

Analyte	Sampled Date/time	Unit	LOD	LOQ (LOR)	Result	Guideline Limit	Method	Guideline	Testing Location
Air Testing									
Propylene Oxide	09:50 AM - 11:50 AM	ppm	-	0.10	<0.10	100	NIOSH (1994), 1612	MOL	Bangkok

Guideline :
MOL : Announcement of the Department of Labour Protection and Welfare on Threshold Limit Values of Hazardous Chemical Substances Dated August 3, B.E. 2560 (2017)
Sampled By : Apichart Wilars

Remark :
- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

Approved by
Orawan Rakyong
Scientist (3)

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong
Thailand 21130
P/O : 4518158712
Project Name : Environmental Quality Monitoring
Project Location : AIE_Rigid Polyol Plant

Lot ID: 265926
Date Received : Feb 12, 2026
Date Reported : Feb 18, 2026
Report Number : 3491604-1

Sample Number	265926-2
Sampled Date	Feb 11, 2026
Sample Description	Air Quality
Location	พนักงานที่ปฏิบัติหน้าที่ในกระบวนการผลิต
Personal Sampling	คุณราเชนทร์ ศรีพรม
Date Analysis Commenced	Feb 13, 2026
Condition of Sample	Drawn into one sorbent tube, refrigerated
Barometric Pressure	759 mmHg
Atmospheric Temperature	29.7 °C

Analyte	Sampled Date/time	Unit	LOD	LOQ (LOR)	Result	Guideline Limit	Method	Guideline	Testing Location
Air Testing									
Propylene Oxide	09:30 AM - 11:30 AM	ppm	-	0.10	<0.10	100	NIOSH (1994), 1612	MOL	Bangkok

Guideline :
MOL : Announcement of the Department of Labour Protection and Welfare on Threshold Limit Values of Hazardous Chemical Substances Dated August 3, B.E. 2560 (2017)
Sampled By : Apichart Wilars

Remark :
- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

Approved by
Orawan Rakyong
Scientist (3)

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand | PHONE +66 0 2760 3000 | FAX +66 0 2760 3197
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company
Life Sciences www.alsglobal.com
RIGHT SOLUTIONS RIGHT PARTNER
8525-205/ EMAIL

Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong
Thailand 21130
P/O : 4518158708
Project Name : Environmental Quality Monitoring
Project Location : AIE_DMC-Polyol Plant

Lot ID: 2635236
Date Received : May 11, 2026
Date Reported : May 19, 2026
Report Number : 3558206-1

Sample Number	2635236-1
Sampled Date	May 08, 2026
Sample Description	Air Quality
Location	หน่วยทำปฏิกิริยา
Date Analysis Commenced	May 14, 2026
Condition of Sample	Drawn into one sorbent tube, refrigerated
Barometric Pressure	755 mmHg
Atmospheric Temperature	31.2 °C

Analyte	Sampled Date/time	Unit	LOD	LOQ (LOR)	Result	Guideline Limit	Method	Guideline	Testing Location
Air Testing									
Propylene Oxide	09:30 AM - 11:30 AM	ppm	-	0.10	<0.10	100	NIOSH (1994), 1612	MOL	Bangkok

Guideline :
MOL : Announcement of the Department of Labour Protection and Welfare on Threshold Limit Values of Hazardous Chemical Substances Dated August 3, B.E. 2560 (2017)
Sampled By : Arnon Phoprathong

Remark :
- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

Approved by Orawan R.
Orawan Rakyong
Scientist (3)

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong
Thailand 21130
P/O : 4518158708
Project Name : Environmental Quality Monitoring
Project Location : AIE_DMC-Polyol Plant

Lot ID: 2635236
Date Received : May 11, 2026
Date Reported : May 19, 2026
Report Number : 3558206-1

Sample Number	2635236-2
Sampled Date	May 08, 2026
Sample Description	Air Quality
Location	หน่วยทำปฏิกิริยา
Personal Sampling	คุณภาณุพงศ์ อารีมิตร์
Date Analysis Commenced	May 14, 2026
Condition of Sample	Drawn into one sorbent tube, refrigerated
Barometric Pressure	755 mmHg
Atmospheric Temperature	31.2 °C

Analyte	Sampled Date/time	Unit	LOD	LOQ (LOR)	Result	Guideline Limit	Method	Guideline	Testing Location
Air Testing									
Propylene Oxide	09:30 AM - 11:30 AM	ppm	-	0.10	<0.10	100	NIOSH (1994), 1612	MOL	Bangkok

Guideline :
MOL : Announcement of the Department of Labour Protection and Welfare on Threshold Limit Values of Hazardous Chemical Substances Dated August 3, B.E. 2560 (2017)
Sampled By : Arnon Phoprathong

Remark :
- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

Approved by Orawan R.
Orawan Rakyong
Scientist (3)

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand | PHONE +66 0 2760 3000 | FAX +66 0 2760 3197
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company
Life Sciences www.alsglobal.com
RIGHT SOLUTIONS RIGHT PARTNER
8525-81/ EMAIL

Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong
Thailand 21130
P/O : 4518158712
Project Name : Environmental Quality Monitoring
Project Location : AIE_Rigid Polyol Plant

Lot ID: 2635242
Date Received : May 11, 2026
Date Reported : May 19, 2026
Report Number : 3558219-1

Sample Number	2635242-1
Sampled Date	May 08, 2026
Sample Description	Air Quality
Location	หน่วยทำปฏิกิริยาของสายการผลิตที่ 2
Date Analysis Commenced	May 14, 2026
Condition of Sample	Drawn into one sorbent tube, refrigerated
Barometric Pressure	755 mmHg
Atmospheric Temperature	31.2 °C

Analyte	Sampled Date/time	Unit	LOD	LOQ (LOR)	Result	Guideline Limit	Method	Guideline	Testing Location
Air Testing									
Propylene Oxide	10:30 AM - 12:30 PM	ppm	-	0.10	<0.10	100	NIOSH (1994), 1612	MOL	Bangkok

Guideline :
MOL : Announcement of the Department of Labour Protection and Welfare on Threshold Limit Values of Hazardous Chemical Substances Dated August 3, B.E. 2560 (2017)
Sampled By : Arnon Phoprathong

Remark :
- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

Approved by
Orawan Rakyong
Scientist (3)

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong
Thailand 21130
P/O : 4518158712
Project Name : Environmental Quality Monitoring
Project Location : AIE_Rigid Polyol Plant

Lot ID: 2635242
Date Received : May 11, 2026
Date Reported : May 19, 2026
Report Number : 3558219-1

Sample Number	2635242-2
Sampled Date	May 08, 2026
Sample Description	Air Quality
Location	พนักงานที่ปฏิบัติหน้าที่ในกระบวนการผลิต
Personal Sampling	คุณดนัย เจริญเกษร
Date Analysis Commenced	May 14, 2026
Condition of Sample	Drawn into one sorbent tube, refrigerated
Barometric Pressure	755 mmHg
Atmospheric Temperature	31.2 °C

Analyte	Sampled Date/time	Unit	LOD	LOQ (LOR)	Result	Guideline Limit	Method	Guideline	Testing Location
Air Testing									
Propylene Oxide	09:30 AM - 11:30 AM	ppm	-	0.10	<0.10	100	NIOSH (1994), 1612	MOL	Bangkok

Guideline :
MOL : Announcement of the Department of Labour Protection and Welfare on Threshold Limit Values of Hazardous Chemical Substances Dated August 3, B.E. 2560 (2017)
Sampled By : Arnon Phoprathong

Remark :
- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)

Approved by
Orawan Rakyong
Scientist (3)

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand | PHONE +66 0 2760 3000 | FAX +66 0 2760 3197
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company
Life Sciences www.alsglobal.com
RIGHT SOLUTIONS RIGHT PARTNER
8525-205/ EMAIL

ภาคผนวก ค-3

ผลการตรวจวิเคราะห์คุณภาพน้ำเสียจากกระบวนการผลิต

Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130
P/O :
Project Name : Water Testing
Project Location : AIE_DMC Polyol Plant

Lot ID: 25113828
Date Received :Jan 07, 2026
Date Reported :Jan 14, 2026
Report Number :3476334-1

Sample Number	25113828-1
Sampled Date	Jan 07, 2026 11:13 AM
Sample Description	Wastewater
Location	WW from Process
Date Analysis Commenced	Jan 07, 2026
Condition of Sample	Contained in two amber glass bottles and three plastic bottles, sample containers comply to pretreatment - preservation standards (APHA, USEPA)

Analyte	Unit	LOD	LOQ (LOR)	Result	Method	Testing Location
Water Testing						
BOD (5 days at 20 Degree C)	mg/L	-	2.0	1546	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5210 B, part 4500 - O G	Rayong
COD	mg/L	1.5	25	25075	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5220 D	Rayong
Oil & Grease	mg/L	-	3	134	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5520 B	Rayong
pH at 25 degree C		-	-	6.3	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 4500 - H (B)	Rayong
Total Dissolved Solids Dried at 180 degree C	mg/L	-	5	8	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 2540 C	Rayong

Sampling By : Wanlop Hunchainaow ทะเบียนเลขที่ ว-323-จ-0038

Remark :
- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)
- Analyte(s) marked * is/are not included in scope of Accreditation ISO/IEC 17025.
- Sampling is not included in scope of accreditation ISO/IEC 17025

Technical Management
Photchana Seeda
Scientist (4)
ทะเบียนเลขที่ ว-323-จ-0028

Approved by
Dej Changchon
Senior Manager
ทะเบียนเลขที่ ว-323-ค-0001

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences www.alsglobal.com
RIGHT SOLUTIONS RIGHT PARTNER

Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130
P/O : 4701610098
Project Name : Water Testing
Project Location : AIE_DMC Polyol Plant

Lot ID: 2645057
Date Received :Jun 04, 2026
Date Reported :Jun 11, 2026
Report Number :3578960-1

Sample Number	2645057-1
Sampled Date	Jun 04, 2026 10:50 AM
Sample Description	Wastewater
Location	WW from Process
Date Analysis Commenced	Jun 04, 2026
Condition of Sample	Contained in two amber glass bottles and three plastic bottles, sample containers comply to pretreatment - preservation standards (APHA, USEPA)

Analyte	Unit	LOD	LOQ (LOR)	Result	Method	Testing Location
Water Testing						
BOD (5 days at 20 Degree C)	mg/L	-	2.0	642	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5210 B, part 4500 - O G	Rayong
COD	mg/L	1.5	25	29101	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5220 D	Rayong
Oil & Grease	mg/L	-	3	96	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5520 B	Rayong
pH at 25 degree C		-	-	6.2	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 4500 - H (B)	Rayong
Total Dissolved Solids Dried at 180 degree C	mg/L	-	5	22	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 2540 C	Rayong

Sampling By : Nattawut Athomprommarat ทะเบียนเลขที่ ว-323-จ-0006

Remark :
- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)
- Analyte(s) marked * is/are not included in scope of Accreditation ISO/IEC 17025.
- Sampling is not included in scope of accreditation ISO/IEC 17025

Technical Management
Photchana Seeda
Scientist (4)
ทะเบียนเลขที่ ว-323-จ-0028

Approved by
Dej Changchon
Senior Manager
ทะเบียนเลขที่ ว-323-ค-0001

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences www.alsglobal.com
RIGHT SOLUTIONS RIGHT PARTNER

Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130
P/O : 4701610098
Project Name : Water Testing
Project Location : AIE_DMC Polyol Plant

Lot ID: 265552
Date Received :Feb 05, 2026
Date Reported :Feb 12, 2026
Report Number :3490950-1

Sample Number	265552-1
Sampled Date	Feb 05, 2026 11:20 AM
Sample Description	Wastewater
Location	WW from Process
Date Analysis Commenced	Feb 05, 2026
Condition of Sample	Contained in two amber glass bottles and three plastic bottles, sample containers comply to pretreatment - preservation standards (APHA, USEPA)

Analyte	Unit	LOD	LOQ (LOR)	Result	Method	Testing Location
Water Testing						
BOD (5 days at 20 Degree C)	mg/L	-	2.0	1185	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5210 B, part 4500 - O G	Rayong
COD	mg/L	1.5	25	18161	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5220 D	Rayong
Oil & Grease	mg/L	-	3	103	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5520 B	Rayong
pH at 25 degree C		-	-	5.8	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 4500 - H (B)	Rayong
Total Dissolved Solids Dried at 180 degree C	mg/L	-	5	17	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 2540 C	Rayong

Sampling By : Wanlop Hunchainaow ทะเบียนเลขที่ ว-323-จ-0038

Remark :
- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)
- Analyte(s) marked * is/are not included in scope of Accreditation ISO/IEC 17025.
- Sampling is not included in scope of accreditation ISO/IEC 17025

Technical Management
Photchana Seeda
Scientist (4)
ทะเบียนเลขที่ ว-323-จ-0028

Approved by
Dej Changchon
Senior Manager
ทะเบียนเลขที่ ว-323-ค-0001

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences www.alsglobal.com
RIGHT SOLUTIONS RIGHT PARTNER

Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130
P/O : 4701610098
Project Name : Water Testing
Project Location : AIE_DMC Polyol Plant

Lot ID: 2616236
Date Received :Mar 04, 2026
Date Reported :Mar 11, 2026
Report Number :3512444-1

Sample Number	2616236-1
Sampled Date	Mar 04, 2026 11:20 AM
Sample Description	Wastewater
Location	WW from Process
Date Analysis Commenced	Mar 04, 2026
Condition of Sample	Contained in one amber glass bottle and three plastic bottles, sample containers comply to pretreatment - preservation standards (APHA, USEPA)

Analyte	Unit	LOD	LOQ (LOR)	Result	Method	Testing Location
Water Testing						
BOD (5 days at 20 Degree C)	mg/L	-	2.0	1037	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5210 B, part 4500 - O G	Rayong
COD	mg/L	1.5	25	14548	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5220 D	Rayong
Oil & Grease	mg/L	-	3	197	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5520 B	Rayong
pH at 25 degree C		-	-	5.5	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 4500 - H (B)	Rayong
Total Dissolved Solids Dried at 180 degree C	mg/L	-	5	33	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 2540 C	Rayong

Sampling By : Wanlop Hunchainaow ทะเบียนเลขที่ ว-323-จ-0038

Remark :
- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)
- Analyte(s) marked * is/are not included in scope of Accreditation ISO/IEC 17025.
- Sampling is not included in scope of accreditation ISO/IEC 17025

Technical Management
Photchana Seeda
Scientist (4)
ทะเบียนเลขที่ ว-323-จ-0028

Approved by
Dej Changchon
Senior Manager
ทะเบียนเลขที่ ว-323-ค-0001

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences www.alsglobal.com
RIGHT SOLUTIONS RIGHT PARTNER

Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130
P/O : 4701610098
Project Name : Water Testing
Project Location : AIE_DMC Polyol Plant

Lot ID: 2625141
Date Received :Apr 01, 2026
Date Reported :Apr 08, 2026
Report Number :3533190-1

Sample Number	2625141-1
Sampled Date	Apr 01, 2026 10:45 AM
Sample Description	Wastewater
Location	WW from Process
Date Analysis Commenced	Apr 01, 2026
Condition of Sample	Contained in two amber glass bottles and three plastic bottles, sample containers comply to pretreatment - preservation standards (APHA, USEPA)

Analyte	Unit	LOD	LOQ (LOR)	Result	Method	Testing Location
Water Testing						
BOD (5 days at 20 Degree C)	mg/L	-	2.0	930	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5210 B, part 4500 - O G	Rayong
COD	mg/L	1.5	25	19303	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5220 D	Rayong
Oil & Grease	mg/L	-	3	104	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5520 B	Rayong
pH at 25 degree C		-	-	6.4	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 4500 - H (B)	Rayong
Total Dissolved Solids Dried at 180 degree C	mg/L	-	5	11	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 2540 C	Rayong

Sampling By : Surawit Narapong ทะเบียนเลขที่ ว-323-จ-0011

Remark :
- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)
- Analyte(s) marked * is/are not included in scope of Accreditation ISO/IEC 17025.
- Sampling is not included in scope of accreditation ISO/IEC 17025

Technical Management
PhotchanaS
Photchana Seeda
Scientist (4)
ทะเบียนเลขที่ ว-323-จ-0028

Approved by
D.Chuwon.
Dej Changchon
Senior Manager
ทะเบียนเลขที่ ว-323-ค-0001

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130
P/O : 4701610098
Project Name : Water Testing
Project Location : AIE_DMC Polyol Plant

Lot ID: 2634799
Date Received :May 06, 2026
Date Reported :May 13, 2026
Report Number :3557506-1

Sample Number	2634799-1
Sampled Date	May 06, 2026 11:05 AM
Sample Description	Wastewater
Location	WW from Process
Date Analysis Commenced	May 06, 2026
Condition of Sample	Contained in two amber glass bottles and three plastic bottles, sample containers comply to pretreatment - preservation standards (APHA, USEPA)

Analyte	Unit	LOD	LOQ (LOR)	Result	Method	Testing Location
Water Testing						
BOD (5 days at 20 Degree C)	mg/L	-	2.0	1280	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5210 B, part 4500 - O G	Rayong
COD	mg/L	1.5	25	18142	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5220 D	Rayong
Oil & Grease *	mg/L	-	3	211	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 5520 B	Rayong
pH at 25 degree C		-	-	6.0	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 4500 - H (B)	Rayong
Total Dissolved Solids Dried at 180 degree C	mg/L	-	5	9	Standard Methods for the Examination of Water and Wastewater. APHA, AWWA & WEF, 24th ed., 2023, part 2540 C	Rayong

Sampling By : Amonwich Wongsachai ทะเบียนเลขที่ ว-323-จ-0040

Remark :
- LOD : Limit of Detection
- "<" : Lower than LOQ (Limit of Quantitation) / LOR (Limit of Reporting)
- Analyte(s) marked * is/are not included in scope of Accreditation ISO/IEC 17025.
- Sampling is not included in scope of accreditation ISO/IEC 17025

Technical Management
Jitsupa P.
Jitsupa Pratuangsuk
Scientist (2)
ทะเบียนเลขที่ ว-323-จ-0004

Approved by
D.Chuwon.
Dej Changchon
Senior Manager
ทะเบียนเลขที่ ว-323-ค-0001

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

ภาคผนวก ค-4

ผลการตรวจวัดระดับเสียงโดยทั่วไป

Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130
P/O :
Project Name : Environmental Quality Monitoring
Project Location : AIE_DMC Polyol Plant

Lot ID: 2612676
Date Received : Feb 25, 2026
Date Reported : Mar 07, 2026
Report Number: 3519122-1C18

Sample Number 2612676-1
Parameter Noise (Leq 24 hrs.)
Location บริเวณริมรั้วทางด้านทิศตะวันตกของพื้นที่ HPPO (GPS 47P 0726777, 1405417)
Measurement Date Feb 16 - Feb 17, 2026
Measurement by Sitpawit Suwannarat
Sound Level meter Serial No. 623393

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
11:00 AM - 12:00 PM	59.6	80.4	56.7
12:00 PM - 01:00 PM	59.0	79.8	56.8
01:00 PM - 02:00 PM	59.9	87.5	56.8
02:00 PM - 03:00 PM	59.4	77.6	56.8
03:00 PM - 04:00 PM	58.7	75.3	56.8
04:00 PM - 05:00 PM	59.7	83.1	56.9
05:00 PM - 06:00 PM	60.3	79.8	57.6
06:00 PM - 07:00 PM	61.1	82.7	57.6
07:00 PM - 08:00 PM	60.8	77.6	58.2
08:00 PM - 09:00 PM	60.0	86.0	57.5
09:00 PM - 10:00 PM	59.4	77.0	57.8
10:00 PM - 11:00 PM	59.0	73.6	58.1
11:00 PM - 12:00 AM	59.1	76.7	58.3
12:00 AM - 01:00 AM	58.7	69.3	58.2
01:00 AM - 02:00 AM	58.4	71.2	57.9
02:00 AM - 03:00 AM	58.3	68.2	57.8
03:00 AM - 04:00 AM	58.6	63.5	58.1
04:00 AM - 05:00 AM	58.7	69.4	58.1
05:00 AM - 06:00 AM	58.4	69.0	57.8
06:00 AM - 07:00 AM	58.8	73.9	57.9
07:00 AM - 08:00 AM	62.0	79.9	59.3
08:00 AM - 09:00 AM	63.1	83.9	58.9
09:00 AM - 10:00 AM	60.3	74.3	58.2
10:00 AM - 11:00 AM	59.3	77.2	57.6
Leq Average 24 hrs. (dB(A))	59.8		
Lmax (dB(A))		87.5	
L90 (dB(A))			57.8
Ldn (dB(A))	65.4		
Standard (dB(A))	70	115	

Reference Method : ISO 1996-1 : 2016
Standard : 1. ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ ฉบับที่ 15 (พ.ศ. 2540) เรื่องกำหนดมาตรฐานระดับเสียงโดยทั่วไป
2. ประกาศกระทรวงอุตสาหกรรม เรื่องกำหนดค่าระดับเสียงการรบกวน และระดับเสียงที่เกิดจากการประกอบกิจการโรงงาน พ.ศ. 2548

Technical Management Chontichak
Chonticha Subongkoch
Scientist (3)

Approved by Supot S.
Supot Salamteh
Section Head

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any from without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130
P/O :
Project Name : Environmental Quality Monitoring
Project Location : AIE_DMC Polyol Plant

Lot ID: 2612676
Date Received : Feb 25, 2026
Date Reported : Mar 07, 2026
Report Number: 3519123-1C18

Sample Number 2612676-2
Parameter Noise (Leq 24 hrs.)
Location บริเวณริมรั้วทางด้านทิศตะวันตกของพื้นที่ HPPO (GPS 47P 0726777, 1405417)
Measurement Date Feb 17 - Feb 18, 2026
Measurement by Sitpawit Suwannarat
Sound Level meter Serial No. 623393

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
11:00 AM - 12:00 PM	60.3	86.4	57.1
12:00 PM - 01:00 PM	60.7	92.0	56.8
01:00 PM - 02:00 PM	59.1	76.1	56.8
02:00 PM - 03:00 PM	58.5	74.9	56.7
03:00 PM - 04:00 PM	58.1	73.9	56.6
04:00 PM - 05:00 PM	59.1	82.5	56.8
05:00 PM - 06:00 PM	59.4	74.7	57.1
06:00 PM - 07:00 PM	60.5	80.2	57.7
07:00 PM - 08:00 PM	62.1	86.5	58.4
08:00 PM - 09:00 PM	60.5	88.2	57.9
09:00 PM - 10:00 PM	59.1	74.8	57.8
10:00 PM - 11:00 PM	59.1	77.4	57.9
11:00 PM - 12:00 AM	58.8	70.5	58.1
12:00 AM - 01:00 AM	58.9	70.8	58.1
01:00 AM - 02:00 AM	59.2	77.7	58.2
02:00 AM - 03:00 AM	59.3	77.3	58.5
03:00 AM - 04:00 AM	59.0	67.7	58.4
04:00 AM - 05:00 AM	59.1	66.9	58.6
05:00 AM - 06:00 AM	59.0	68.9	58.4
06:00 AM - 07:00 AM	59.1	78.4	58.1
07:00 AM - 08:00 AM	62.0	83.9	59.2
08:00 AM - 09:00 AM	63.6	83.9	59.6
09:00 AM - 10:00 AM	60.9	78.6	58.9
10:00 AM - 11:00 AM	60.2	83.4	58.3
Leq Average 24 hrs. (dB(A))	60.0		
Lmax (dB(A))		92.0	
L90 (dB(A))			58.1
Ldn (dB(A))	65.7		
Standard (dB(A))	70	115	

Reference Method : ISO 1996-1 : 2016
Standard : 1. ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ ฉบับที่ 15 (พ.ศ. 2540) เรื่องกำหนดมาตรฐานระดับเสียงโดยทั่วไป
2. ประกาศกระทรวงอุตสาหกรรม เรื่องกำหนดค่าระดับเสียงการรบกวน และระดับเสียงที่เกิดจากการประกอบกิจการโรงงาน พ.ศ. 2548

Technical Management Chontichak
Chonticha Subongkoch
Scientist (3)

Approved by Supot S.
Supot Salamteh
Section Head

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any from without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
Life Sciences www.alsglobal.com
RIGHT SOLUTIONS RIGHT PARTNER
8525-209/ EMAIL

Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130
P/O :
Project Name : Environmental Quality Monitoring
Project Location : AIE_DMC Polyol Plant

Lot ID: 2612676
Date Received : Feb 25, 2026
Date Reported : Mar 07, 2026
Report Number: 3519124-1C18

Sample Number	2612676-3
Parameter	Noise (Leq 24 hrs.)
Location	บริเวณริมรั้วทางด้านทิศตะวันตกของพื้นที่ HPPO (GPS 47P 0726777, 1405417)
Measurement Date	Feb 18 - Feb 19, 2026
Measurement by	Sitpawit Suwannarat
Sound Level meter	Serial No. 623393

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
11:00 AM - 12:00 PM	59.3	75.9	57.8
12:00 PM - 01:00 PM	59.6	75.2	57.3
01:00 PM - 02:00 PM	59.4	71.6	57.3
02:00 PM - 03:00 PM	59.0	76.6	57.1
03:00 PM - 04:00 PM	58.7	74.2	57.0
04:00 PM - 05:00 PM	58.6	72.6	57.0
05:00 PM - 06:00 PM	60.1	80.4	57.1
06:00 PM - 07:00 PM	60.9	84.4	57.4
07:00 PM - 08:00 PM	60.3	79.1	57.1
08:00 PM - 09:00 PM	59.7	85.9	57.0
09:00 PM - 10:00 PM	59.1	80.8	57.6
10:00 PM - 11:00 PM	58.8	76.0	57.8
11:00 PM - 12:00 AM	59.0	80.4	58.0
12:00 AM - 01:00 AM	59.4	77.7	58.5
01:00 AM - 02:00 AM	58.6	74.0	58.0
02:00 AM - 03:00 AM	58.6	74.9	58.0
03:00 AM - 04:00 AM	58.1	68.8	57.6
04:00 AM - 05:00 AM	58.2	68.2	57.8
05:00 AM - 06:00 AM	58.6	70.8	58.1
06:00 AM - 07:00 AM	59.1	71.5	58.3
07:00 AM - 08:00 AM	61.9	75.7	59.7
08:00 AM - 09:00 AM	63.5	87.0	59.3
09:00 AM - 10:00 AM	61.0	84.0	57.9
10:00 AM - 11:00 AM	59.2	72.1	57.7
Leq Average 24 hrs. (dB(A))	59.7		
Lmax (dB(A))		87.0	
L90 (dB(A))			57.7
Ldn (dB(A))	65.4		
Standard (dB(A))	70	115	

Reference Method : ISO 1996-1 : 2016
Standard : 1. ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ ฉบับที่ 15 (พ.ศ. 2540) เรื่องกำหนดมาตรฐานระดับเสียงโดยทั่วไป
2. ประกาศกระทรวงอุตสาหกรรม เรื่องกำหนดค่าระดับเสียงการรบกวน และระดับเสียงที่เกิดจากการประกอบกิจการโรงงาน พ.ศ. 2548

Technical Management Chontichak
Chonticha Subongkoch
Scientist (3)

Approved by Supot S.
Supot Salamteh
Section Head

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any from without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130
P/O :
Project Name : Environmental Quality Monitoring
Project Location : AIE_DMC Polyol Plant

Lot ID: 2612676
Date Received : Feb 25, 2026
Date Reported : Mar 07, 2026
Report Number: 3519125-1C18

Sample Number	2612676-4
Parameter	Noise (Leq 24 hrs.)
Location	บริเวณริมรั้วทางด้านทิศตะวันตกของพื้นที่ HPPO (GPS 47P 0726777, 1405417)
Measurement Date	Feb 19 - Feb 20, 2026
Measurement by	Sitpawit Suwannarat
Sound Level meter	Serial No. 623393

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
11:00 AM - 12:00 PM	59.7	73.3	58.2
12:00 PM - 01:00 PM	60.4	78.5	57.7
01:00 PM - 02:00 PM	60.2	75.1	57.9
02:00 PM - 03:00 PM	58.7	71.0	57.2
03:00 PM - 04:00 PM	58.9	77.8	57.1
04:00 PM - 05:00 PM	58.3	74.0	56.7
05:00 PM - 06:00 PM	59.3	76.1	56.7
06:00 PM - 07:00 PM	61.1	85.6	56.7
07:00 PM - 08:00 PM	59.8	78.5	57.2
08:00 PM - 09:00 PM	60.5	88.7	57.1
09:00 PM - 10:00 PM	59.4	79.5	58.1
10:00 PM - 11:00 PM	59.5	76.0	58.7
11:00 PM - 12:00 AM	59.1	75.0	58.3
12:00 AM - 01:00 AM	58.9	67.7	58.3
01:00 AM - 02:00 AM	58.8	68.6	58.3
02:00 AM - 03:00 AM	59.2	69.6	58.8
03:00 AM - 04:00 AM	58.8	74.1	58.2
04:00 AM - 05:00 AM	59.1	74.3	58.6
05:00 AM - 06:00 AM	59.3	74.5	58.7
06:00 AM - 07:00 AM	60.1	81.1	59.1
07:00 AM - 08:00 AM	63.1	83.5	60.0
08:00 AM - 09:00 AM	62.9	82.4	59.0
09:00 AM - 10:00 AM	60.5	79.2	58.3
10:00 AM - 11:00 AM	59.8	72.7	58.5
Leq Average 24 hrs. (dB(A))	60.0		
Lmax (dB(A))		88.7	
L90 (dB(A))			58.2
Ldn (dB(A))	65.8		
Standard (dB(A))	70	115	

Reference Method : ISO 1996-1 : 2016
Standard : 1. ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ ฉบับที่ 15 (พ.ศ. 2540) เรื่องกำหนดมาตรฐานระดับเสียงโดยทั่วไป
2. ประกาศกระทรวงอุตสาหกรรม เรื่องกำหนดค่าระดับเสียงการรบกวน และระดับเสียงที่เกิดจากการประกอบกิจการโรงงาน พ.ศ. 2548

Technical Management Chontichak
Chonticha Subongkoch
Scientist (3)

Approved by Supot S.
Supot Salamteh
Section Head

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any from without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
Life Sciences www.alsglobal.com
RIGHT SOLUTIONS RIGHT PARTNER
8525-209/ EMAIL

Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130
P/O :
Project Name : Environmental Quality Monitoring
Project Location : AIE_DMC Polyol Plant

Lot ID: 2612676
Date Received : Feb 25, 2026
Date Reported : Mar 07, 2026
Report Number: 3519126-1C18

Sample Number	2612676-5
Parameter	Noise (Leq 24 hrs.)
Location	บริเวณริมรั้วทางด้านทิศตะวันตกของพื้นที่ HPPO (GPS 47P 0726777, 1405417)
Measurement Date	Feb 20 - Feb 21, 2026
Measurement by	Sitpawit Suwannarat
Sound Level meter	Serial No. 623393

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
11:00 AM - 12:00 PM	60.0	78.0	58.1
12:00 PM - 01:00 PM	60.2	78.1	58.0
01:00 PM - 02:00 PM	59.9	74.6	57.8
02:00 PM - 03:00 PM	59.9	79.5	57.9
03:00 PM - 04:00 PM	59.7	73.8	57.9
04:00 PM - 05:00 PM	61.5	79.0	56.7
05:00 PM - 06:00 PM	62.4	77.6	58.2
06:00 PM - 07:00 PM	62.5	80.6	57.7
07:00 PM - 08:00 PM	59.5	70.3	57.8
08:00 PM - 09:00 PM	59.0	73.7	57.7
09:00 PM - 10:00 PM	59.9	68.9	58.9
10:00 PM - 11:00 PM	59.7	76.9	58.7
11:00 PM - 12:00 AM	60.5	80.0	57.4
12:00 AM - 01:00 AM	58.5	69.7	57.8
01:00 AM - 02:00 AM	59.7	73.2	59.0
02:00 AM - 03:00 AM	60.1	67.3	59.6
03:00 AM - 04:00 AM	60.1	71.8	59.5
04:00 AM - 05:00 AM	60.1	68.1	59.6
05:00 AM - 06:00 AM	65.0	79.6	63.5
06:00 AM - 07:00 AM	64.8	76.1	61.4
07:00 AM - 08:00 AM	61.6	78.7	58.3
08:00 AM - 09:00 AM	61.0	78.4	57.4
09:00 AM - 10:00 AM	59.4	76.5	56.6
10:00 AM - 11:00 AM	60.2	76.3	56.5
Leq Average 24 hrs. (dB(A))	61.0		
Lmax (dB(A))		80.6	
L90 (dB(A))			57.9
Ldn (dB(A))	67.9		
Standard (dB(A))	70	115	

Reference Method : ISO 1996-1 : 2016
Standard : 1. ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ ฉบับที่ 15 (พ.ศ. 2540) เรื่องกำหนดมาตรฐานระดับเสียงโดยทั่วไป
2. ประกาศกระทรวงอุตสาหกรรม เรื่องกำหนดค่าระดับเสียงการรบกวน และระดับเสียงที่เกิดจากการประกอบกิจการโรงงาน พ.ศ. 2548

Technical Management Chontichak
Chonticha Subongkoch
Scientist (3)

Approved by Supot S.
Supot Salamteh
Section Head

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any from without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130
P/O :
Project Name : Environmental Quality Monitoring
Project Location : AIE_DMC Polyol Plant

Lot ID: 2612676
Date Received : Feb 25, 2026
Date Reported : Mar 07, 2026
Report Number: 3519127-1C18

Sample Number	2612676-6
Parameter	Noise (Leq 24 hrs.)
Location	บริเวณริมรั้วทางด้านทิศตะวันตกของพื้นที่ HPPO (GPS 47P 0726777, 1405417)
Measurement Date	Feb 21 - Feb 22, 2026
Measurement by	Sitpawit Suwannarat
Sound Level meter	Serial No. 623393

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
11:00 AM - 12:00 PM	58.7	73.5	55.5
12:00 PM - 01:00 PM	59.7	76.8	56.0
01:00 PM - 02:00 PM	59.5	78.5	56.1
02:00 PM - 03:00 PM	60.9	79.7	56.1
03:00 PM - 04:00 PM	59.1	78.5	55.1
04:00 PM - 05:00 PM	60.5	81.8	55.9
05:00 PM - 06:00 PM	62.8	78.7	58.7
06:00 PM - 07:00 PM	59.8	81.0	55.0
07:00 PM - 08:00 PM	56.5	68.1	54.9
08:00 PM - 09:00 PM	55.9	71.7	54.5
09:00 PM - 10:00 PM	56.7	72.5	54.7
10:00 PM - 11:00 PM	59.9	81.5	54.5
11:00 PM - 12:00 AM	60.4	79.7	55.2
12:00 AM - 01:00 AM	56.2	77.4	54.6
01:00 AM - 02:00 AM	55.0	61.4	54.3
02:00 AM - 03:00 AM	55.6	75.5	54.5
03:00 AM - 04:00 AM	56.2	76.0	54.5
04:00 AM - 05:00 AM	63.7	79.7	59.3
05:00 AM - 06:00 AM	64.4	80.0	61.1
06:00 AM - 07:00 AM	60.2	76.3	56.4
07:00 AM - 08:00 AM	60.1	79.8	55.6
08:00 AM - 09:00 AM	59.6	83.0	55.3
09:00 AM - 10:00 AM	57.8	71.9	55.2
10:00 AM - 11:00 AM	57.5	76.3	54.8
Leq Average 24 hrs. (dB(A))	59.8		
Lmax (dB(A))		83.0	
L90 (dB(A))			55.2
Ldn (dB(A))	66.6		
Standard (dB(A))	70	115	

Reference Method : ISO 1996-1 : 2016
Standard : 1. ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ ฉบับที่ 15 (พ.ศ. 2540) เรื่องกำหนดมาตรฐานระดับเสียงโดยทั่วไป
2. ประกาศกระทรวงอุตสาหกรรม เรื่องกำหนดค่าระดับเสียงการรบกวน และระดับเสียงที่เกิดจากการประกอบกิจการโรงงาน พ.ศ. 2548

Technical Management Chontichak
Chonticha Subongkoch
Scientist (3)

Approved by Supot S.
Supot Salamteh
Section Head

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any from without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
Life Sciences www.alsglobal.com
RIGHT SOLUTIONS RIGHT PARTNER
8525-209/ EMAIL

Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130
P/O :
Project Name : Environmental Quality Monitoring
Project Location : AIE_DMC Polyol Plant

Lot ID: 2612676
Date Received : Feb 25, 2026
Date Reported : Mar 07, 2026
Report Number: 3519128-1C18

Sample Number	2612676-7
Parameter	Noise (Leq 24 hrs.)
Location	บริเวณริมรั้วทางด้านทิศตะวันตกของพื้นที่ HPPO (GPS 47P 0726777, 1405417)
Measurement Date	Feb 22 - Feb 23, 2026
Measurement by	Sitpawit Suwannarat
Sound Level meter	Serial No. 623393

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
11:00 AM - 12:00 PM	57.5	72.1	54.4
12:00 PM - 01:00 PM	57.6	70.3	54.6
01:00 PM - 02:00 PM	57.2	68.6	54.5
02:00 PM - 03:00 PM	56.4	68.6	54.3
03:00 PM - 04:00 PM	58.0	72.8	54.8
04:00 PM - 05:00 PM	62.4	82.0	56.4
05:00 PM - 06:00 PM	63.7	84.4	58.5
06:00 PM - 07:00 PM	58.8	74.0	56.1
07:00 PM - 08:00 PM	56.4	67.2	55.2
08:00 PM - 09:00 PM	56.4	72.0	54.6
09:00 PM - 10:00 PM	56.0	67.7	54.7
10:00 PM - 11:00 PM	58.2	77.5	55.6
11:00 PM - 12:00 AM	57.4	80.4	55.0
12:00 AM - 01:00 AM	56.6	70.6	55.5
01:00 AM - 02:00 AM	59.2	83.0	55.8
02:00 AM - 03:00 AM	58.2	71.9	56.2
03:00 AM - 04:00 AM	60.5	76.4	56.6
04:00 AM - 05:00 AM	64.9	82.1	59.7
05:00 AM - 06:00 AM	62.7	78.4	58.2
06:00 AM - 07:00 AM	59.2	74.0	56.0
07:00 AM - 08:00 AM	58.3	69.1	55.6
08:00 AM - 09:00 AM	60.0	80.5	55.5
09:00 AM - 10:00 AM	58.0	73.4	54.9
10:00 AM - 11:00 AM	58.3	74.8	55.2
Leq Average 24 hrs. (dB(A))	59.6		
Lmax (dB(A))		84.4	
L90 (dB(A))			55.5
Ldn (dB(A))	66.7		
Standard (dB(A))	70	115	

Reference Method : ISO 1996-1 : 2016
Standard : 1. ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ ฉบับที่ 15 (พ.ศ. 2540) เรื่องกำหนดมาตรฐานระดับเสียงโดยทั่วไป
2. ประกาศกระทรวงอุตสาหกรรม เรื่องกำหนดค่าระดับเสียงการรบกวน และระดับเสียงที่เกิดจากการประกอบกิจการโรงงาน พ.ศ. 2548

Technical Management Chontichak
Chonticha Subongkoch
Scientist (3)

Approved by Supot S.
Supot Salamteh
Section Head

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any from without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130
P/O :
Project Name : Environmental Quality Monitoring
Project Location : AIE_DMC Polyol Plant

Lot ID: 2612681
Date Received : Feb 25, 2026
Date Reported : Mar 07, 2026
Report Number: 3519219-1C18

Sample Number	2612681-1
Parameter	Noise (Leq 24 hrs.)
Location	บริเวณริมรั้วทางด้านทิศใต้ของพื้นที่ HPPO (ข้างป้อม รปภ. บล๊อค 45)(GPS 47P 0727136, 1404550)
Measurement Date	Feb 16 - Feb 17, 2026
Measurement by	Sitpawit Suwannarat
Sound Level meter	Serial No. 623392

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
11:00 AM - 12:00 PM	55.2	79.2	45.5
12:00 PM - 01:00 PM	48.3	66.1	45.3
01:00 PM - 02:00 PM	53.5	75.7	45.3
02:00 PM - 03:00 PM	55.9	84.8	45.2
03:00 PM - 04:00 PM	50.9	68.1	45.5
04:00 PM - 05:00 PM	50.3	67.7	45.8
05:00 PM - 06:00 PM	51.6	69.3	47.1
06:00 PM - 07:00 PM	50.8	66.5	47.2
07:00 PM - 08:00 PM	51.4	73.6	46.8
08:00 PM - 09:00 PM	47.8	65.7	45.3
09:00 PM - 10:00 PM	47.1	65.8	45.4
10:00 PM - 11:00 PM	47.6	61.6	45.7
11:00 PM - 12:00 AM	46.6	58.6	45.3
12:00 AM - 01:00 AM	47.8	68.9	45.2
01:00 AM - 02:00 AM	49.7	70.5	45.3
02:00 AM - 03:00 AM	46.3	55.4	45.2
03:00 AM - 04:00 AM	46.4	58.7	45.1
04:00 AM - 05:00 AM	50.8	71.1	45.4
05:00 AM - 06:00 AM	47.6	59.1	46.1
06:00 AM - 07:00 AM	55.2	70.8	52.4
07:00 AM - 08:00 AM	54.8	71.1	49.9
08:00 AM - 09:00 AM	56.8	85.7	47.8
09:00 AM - 10:00 AM	55.2	78.0	45.8
10:00 AM - 11:00 AM	49.4	70.3	44.3
Leq Average 24 hrs. (dB(A))	52.0		
Lmax (dB(A))		85.7	
L90 (dB(A))			45.4
Ldn (dB(A))	56.8		
Standard (dB(A))	70	115	

Reference Method : ISO 1996-1 : 2016
Standard : 1. ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ ฉบับที่ 15 (พ.ศ. 2540) เรื่องกำหนดมาตรฐานระดับเสียงโดยทั่วไป
2. ประกาศกระทรวงอุตสาหกรรม เรื่องกำหนดค่าระดับเสียงการรบกวน และระดับเสียงที่เกิดจากการประกอบกิจการโรงงาน พ.ศ. 2548

Technical Management Chontichak
Chonticha Subongkoch
Scientist (3)

Approved by Supot S.
Supot Salamteh
Section Head

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any from without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130
P/O :
Project Name : Environmental Quality Monitoring
Project Location : AIE_DMC Polyol Plant

Lot ID: 2612681
Date Received : Feb 25, 2026
Date Reported : Mar 07, 2026
Report Number: 3519220-1C18

Sample Number	2612681-2
Parameter	Noise (Leq 24 hrs.)
Location	บริเวณริมรั้วทางด้านทิศใต้ของพื้นที่ HPPO (ข้างป้อม รปภ. บล๊อค 45)(GPS 47P 0727136, 1404550)
Measurement Date	Feb 17 - Feb 18, 2026
Measurement by	Sitpawit Suwannarat
Sound Level meter	Serial No. 623392

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
11:00 AM - 12:00 PM	48.1	73.2	44.4
12:00 PM - 01:00 PM	48.4	71.9	44.1
01:00 PM - 02:00 PM	47.6	65.7	44.1
02:00 PM - 03:00 PM	55.3	79.9	44.0
03:00 PM - 04:00 PM	55.3	78.3	45.1
04:00 PM - 05:00 PM	51.3	76.2	45.9
05:00 PM - 06:00 PM	51.6	68.3	47.5
06:00 PM - 07:00 PM	51.7	68.9	47.5
07:00 PM - 08:00 PM	52.4	73.6	46.4
08:00 PM - 09:00 PM	48.8	67.5	45.3
09:00 PM - 10:00 PM	47.3	68.7	44.9
10:00 PM - 11:00 PM	47.2	68.2	45.3
11:00 PM - 12:00 AM	46.6	61.7	45.1
12:00 AM - 01:00 AM	46.0	56.7	45.0
01:00 AM - 02:00 AM	50.5	71.8	45.6
02:00 AM - 03:00 AM	47.5	63.7	45.8
03:00 AM - 04:00 AM	47.4	56.3	46.1
04:00 AM - 05:00 AM	47.0	59.5	45.6
05:00 AM - 06:00 AM	53.8	76.5	45.6
06:00 AM - 07:00 AM	54.4	68.5	52.2
07:00 AM - 08:00 AM	54.9	71.1	51.0
08:00 AM - 09:00 AM	53.6	68.8	49.0
09:00 AM - 10:00 AM	53.7	76.9	49.0
10:00 AM - 11:00 AM	53.5	72.2	47.0
Leq Average 24 hrs. (dB(A))	51.7		
Lmax (dB(A))		79.9	
L90 (dB(A))			45.6
Ldn (dB(A))	57.0		
Standard (dB(A))	70	115	

Reference Method : ISO 1996-1 : 2016
Standard : 1. ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ ฉบับที่ 15 (พ.ศ. 2540) เรื่องกำหนดมาตรฐานระดับเสียงโดยทั่วไป
2. ประกาศกระทรวงอุตสาหกรรม เรื่องกำหนดค่าระดับเสียงการรบกวน และระดับเสียงที่เกิดจากการประกอบกิจการโรงงาน พ.ศ. 2548

Technical Management Chontichak
Chonticha Subongkoch
Scientist (3)

Approved by Supot S.
Supot Salamteh
Section Head

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any from without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130
P/O :
Project Name : Environmental Quality Monitoring
Project Location : AIE_DMC Polyol Plant

Lot ID: 2612681
Date Received : Feb 25, 2026
Date Reported : Mar 07, 2026
Report Number: 3519221-1C18

Sample Number	2612681-3
Parameter	Noise (Leq 24 hrs.)
Location	บริเวณริมรั้วทางด้านทิศใต้ของพื้นที่ HPPO (ข้างป้อม รปภ. บล๊อค 45)(GPS 47P 0727136, 1404550)
Measurement Date	Feb 18 - Feb 19, 2026
Measurement by	Sitpawit Suwannarat
Sound Level meter	Serial No. 623392

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
11:00 AM - 12:00 PM	49.7	70.0	44.9
12:00 PM - 01:00 PM	50.6	69.1	44.2
01:00 PM - 02:00 PM	49.8	69.5	44.7
02:00 PM - 03:00 PM	53.1	76.9	43.7
03:00 PM - 04:00 PM	51.1	71.0	44.0
04:00 PM - 05:00 PM	50.3	69.9	45.2
05:00 PM - 06:00 PM	52.1	70.4	47.7
06:00 PM - 07:00 PM	52.5	70.2	48.3
07:00 PM - 08:00 PM	51.0	67.3	47.6
08:00 PM - 09:00 PM	48.9	65.6	47.2
09:00 PM - 10:00 PM	48.3	61.9	47.4
10:00 PM - 11:00 PM	49.0	59.7	47.8
11:00 PM - 12:00 AM	50.9	69.8	48.1
12:00 AM - 01:00 AM	50.0	59.1	49.2
01:00 AM - 02:00 AM	49.4	57.7	48.5
02:00 AM - 03:00 AM	48.4	62.8	47.7
03:00 AM - 04:00 AM	47.8	55.1	47.2
04:00 AM - 05:00 AM	54.1	77.3	48.5
05:00 AM - 06:00 AM	52.7	81.0	49.1
06:00 AM - 07:00 AM	57.9	85.2	51.3
07:00 AM - 08:00 AM	56.6	73.2	51.2
08:00 AM - 09:00 AM	51.7	66.5	47.5
09:00 AM - 10:00 AM	49.3	67.7	46.7
10:00 AM - 11:00 AM	48.7	61.8	46.5
Leq Average 24 hrs. (dB(A))	51.9		
Lmax (dB(A))		85.2	
L90 (dB(A))			47.5
Ldn (dB(A))	58.7		
Standard (dB(A))	70	115	

Reference Method : ISO 1996-1 : 2016
Standard : 1. ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ ฉบับที่ 15 (พ.ศ. 2540) เรื่องกำหนดมาตรฐานระดับเสียงโดยทั่วไป
2. ประกาศกระทรวงอุตสาหกรรม เรื่องกำหนดค่าระดับเสียงการรบกวน และระดับเสียงที่เกิดจากการประกอบกิจการโรงงาน พ.ศ. 2548

Technical Management Chontichak
Chonticha Subongkoch
Scientist (3)

Approved by Supot S.
Supot Salamteh
Section Head

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any from without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
Life Sciences www.alsglobal.com
RIGHT SOLUTIONS RIGHT PARTNER
8525-209/ EMAIL

Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130
P/O :
Project Name : Environmental Quality Monitoring
Project Location : AIE_DMC Polyol Plant

Lot ID: 2612681
Date Received : Feb 25, 2026
Date Reported : Mar 07, 2026
Report Number: 3519222-1C18

Sample Number	2612681-4
Parameter	Noise (Leq 24 hrs.)
Location	บริเวณริมรั้วทางด้านทิศใต้ของพื้นที่ HPPO (ข้างป้อม รปภ. บล๊อค 45)(GPS 47P 0727136, 1404550)
Measurement Date	Feb 19 - Feb 20, 2026
Measurement by	Sitpawit Suwannarat
Sound Level meter	Serial No. 623392

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
11:00 AM - 12:00 PM	48.3	64.7	44.8
12:00 PM - 01:00 PM	51.2	76.0	45.0
01:00 PM - 02:00 PM	51.9	74.5	44.6
02:00 PM - 03:00 PM	54.4	78.3	44.5
03:00 PM - 04:00 PM	50.3	70.0	44.8
04:00 PM - 05:00 PM	51.1	73.2	45.7
05:00 PM - 06:00 PM	54.4	70.5	49.4
06:00 PM - 07:00 PM	53.7	68.7	49.6
07:00 PM - 08:00 PM	51.1	69.0	48.2
08:00 PM - 09:00 PM	50.4	65.5	48.5
09:00 PM - 10:00 PM	49.4	62.3	48.4
10:00 PM - 11:00 PM	49.3	62.3	48.5
11:00 PM - 12:00 AM	48.3	67.4	46.9
12:00 AM - 01:00 AM	50.8	68.9	48.1
01:00 AM - 02:00 AM	51.4	69.6	49.3
02:00 AM - 03:00 AM	50.3	58.0	49.7
03:00 AM - 04:00 AM	50.0	57.0	49.5
04:00 AM - 05:00 AM	52.0	68.7	50.2
05:00 AM - 06:00 AM	53.5	73.5	50.1
06:00 AM - 07:00 AM	56.2	70.9	54.3
07:00 AM - 08:00 AM	55.2	70.4	52.1
08:00 AM - 09:00 AM	53.4	70.1	49.3
09:00 AM - 10:00 AM	51.9	73.3	47.9
10:00 AM - 11:00 AM	54.9	76.5	46.8
Leq Average 24 hrs. (dB(A))	52.4		
Lmax (dB(A))		78.3	
L90 (dB(A))			48.4
Ldn (dB(A))	58.5		
Standard (dB(A))	70	115	

Reference Method : ISO 1996-1 : 2016
Standard : 1. ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ ฉบับที่ 15 (พ.ศ. 2540) เรื่องกำหนดมาตรฐานระดับเสียงโดยทั่วไป
2. ประกาศกระทรวงอุตสาหกรรม เรื่องกำหนดค่าระดับเสียงการรบกวน และระดับเสียงที่เกิดจากการประกอบกิจการโรงงาน พ.ศ. 2548

Technical Management Chontichak
Chonticha Subongkoch
Scientist (3)

Approved by Supot S.
Supot Salamteh
Section Head

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any from without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130
P/O :
Project Name : Environmental Quality Monitoring
Project Location : AIE_DMC Polyol Plant

Lot ID: 2612681
Date Received : Feb 25, 2026
Date Reported : Mar 07, 2026
Report Number: 3519223-1C18

Sample Number	2612681-5
Parameter	Noise (Leq 24 hrs.)
Location	บริเวณริมรั้วทางด้านทิศใต้ของพื้นที่ HPPO (ข้างป้อม รปภ. บล๊อค 45)(GPS 47P 0727136, 1404550)
Measurement Date	Feb 20 - Feb 21, 2026
Measurement by	Sitpawit Suwannarat
Sound Level meter	Serial No. 623392

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
11:00 AM - 12:00 PM	48.8	67.5	45.9
12:00 PM - 01:00 PM	49.7	68.4	45.3
01:00 PM - 02:00 PM	48.3	63.8	45.0
02:00 PM - 03:00 PM	56.8	80.9	45.9
03:00 PM - 04:00 PM	48.3	69.8	45.5
04:00 PM - 05:00 PM	53.5	74.0	46.0
05:00 PM - 06:00 PM	51.6	69.0	46.4
06:00 PM - 07:00 PM	53.4	70.6	48.4
07:00 PM - 08:00 PM	51.2	69.0	47.6
08:00 PM - 09:00 PM	49.5	60.3	47.9
09:00 PM - 10:00 PM	49.0	63.7	47.7
10:00 PM - 11:00 PM	50.4	66.9	49.0
11:00 PM - 12:00 AM	49.2	55.0	48.6
12:00 AM - 01:00 AM	50.5	70.0	47.3
01:00 AM - 02:00 AM	48.6	59.7	48.0
02:00 AM - 03:00 AM	49.8	63.2	49.1
03:00 AM - 04:00 AM	50.1	57.3	49.6
04:00 AM - 05:00 AM	50.1	61.8	49.5
05:00 AM - 06:00 AM	53.9	74.1	49.7
06:00 AM - 07:00 AM	55.0	69.6	53.6
07:00 AM - 08:00 AM	54.7	66.1	51.2
08:00 AM - 09:00 AM	51.4	68.7	48.2
09:00 AM - 10:00 AM	50.9	68.4	47.3
10:00 AM - 11:00 AM	49.8	66.5	46.6
Leq Average 24 hrs. (dB(A))	51.7		
Lmax (dB(A))		80.9	
L90 (dB(A))			47.7
Ldn (dB(A))	57.9		
Standard (dB(A))	70	115	

Reference Method : ISO 1996-1 : 2016
Standard : 1. ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ ฉบับที่ 15 (พ.ศ. 2540) เรื่องกำหนดมาตรฐานระดับเสียงโดยทั่วไป
2. ประกาศกระทรวงอุตสาหกรรม เรื่องกำหนดค่าระดับเสียงการรบกวน และระดับเสียงที่เกิดจากการประกอบกิจการโรงงาน พ.ศ. 2548

Technical Management Chontichak
Chonticha Subongkoch
Scientist (3)

Approved by Supot S.
Supot Salamteh
Section Head

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any from without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130
P/O :
Project Name : Environmental Quality Monitoring
Project Location : AIE_DMC Polyol Plant

Lot ID: 2612681
Date Received : Feb 25, 2026
Date Reported : Mar 07, 2026
Report Number: 3519224-1C18

Sample Number	2612681-6
Parameter	Noise (Leq 24 hrs.)
Location	บริเวณริมรั้วทางด้านทิศใต้ของพื้นที่ HPPO (ข้างป้อม รปภ. บล๊อค 45)(GPS 47P 0727136, 1404550)
Measurement Date	Feb 21 - Feb 22, 2026
Measurement by	Sitpawit Suwannarat
Sound Level meter	Serial No. 623392

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
11:00 AM - 12:00 PM	49.8	66.3	46.4
12:00 PM - 01:00 PM	48.7	63.5	45.5
01:00 PM - 02:00 PM	49.7	66.8	46.0
02:00 PM - 03:00 PM	49.5	68.5	46.1
03:00 PM - 04:00 PM	50.9	69.7	46.1
04:00 PM - 05:00 PM	49.1	68.5	45.1
05:00 PM - 06:00 PM	52.8	74.7	45.8
06:00 PM - 07:00 PM	54.4	72.3	48.7
07:00 PM - 08:00 PM	55.6	79.8	45.2
08:00 PM - 09:00 PM	47.4	65.0	45.0
09:00 PM - 10:00 PM	46.0	61.7	44.5
10:00 PM - 11:00 PM	46.3	59.9	44.7
11:00 PM - 12:00 AM	50.1	71.5	44.5
12:00 AM - 01:00 AM	47.3	67.9	44.6
01:00 AM - 02:00 AM	50.0	69.7	45.2
02:00 AM - 03:00 AM	45.1	52.1	44.3
03:00 AM - 04:00 AM	45.6	65.5	44.4
04:00 AM - 05:00 AM	55.7	80.9	44.5
05:00 AM - 06:00 AM	49.7	69.7	44.6
06:00 AM - 07:00 AM	56.3	70.0	52.2
07:00 AM - 08:00 AM	52.3	67.9	48.0
08:00 AM - 09:00 AM	50.4	69.8	46.1
09:00 AM - 10:00 AM	48.2	69.1	45.3
10:00 AM - 11:00 AM	49.8	73.0	45.1
Leq Average 24 hrs. (dB(A))	51.2		
Lmax (dB(A))		80.9	
L90 (dB(A))			45.2
Ldn (dB(A))	57.8		
Standard (dB(A))	70	115	

Reference Method : ISO 1996-1 : 2016
Standard : 1. ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ ฉบับที่ 15 (พ.ศ. 2540) เรื่องกำหนดมาตรฐานระดับเสียงโดยทั่วไป
2. ประกาศกระทรวงอุตสาหกรรม เรื่องกำหนดค่าระดับเสียงการรบกวน และระดับเสียงที่เกิดจากการประกอบกิจการโรงงาน พ.ศ. 2548

Technical Management Chontichak
Chonticha Subongkoch
Scientist (3)

Approved by Supot S
Supot Salamteh
Section Head

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any from without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

Analysis / Test Report

TESTING
No.0042

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130
P/O :
Project Name : Environmental Quality Monitoring
Project Location : AIE_DMC Polyol Plant

Lot ID: 2612681
Date Received : Feb 25, 2026
Date Reported : Mar 07, 2026
Report Number: 3519225-1C18

Sample Number	2612681-7
Parameter	Noise (Leq 24 hrs.)
Location	บริเวณริมรั้วทางด้านทิศใต้ของพื้นที่ HPPO (ข้างป้อม รปภ. บล๊อค 45)(GPS 47P 0727136, 1404550)
Measurement Date	Feb 22 - Feb 23, 2026
Measurement by	Sitpawit Suwannarat
Sound Level meter	Serial No. 623392

Time	Leq (dB(A))	Lmax (dB(A))	L90 (dB(A))
11:00 AM - 12:00 PM	47.9	66.3	45.3
12:00 PM - 01:00 PM	46.7	56.8	44.3
01:00 PM - 02:00 PM	47.3	62.1	44.1
02:00 PM - 03:00 PM	53.7	76.7	45.0
03:00 PM - 04:00 PM	46.3	58.4	44.1
04:00 PM - 05:00 PM	47.0	58.6	44.6
05:00 PM - 06:00 PM	51.4	72.0	45.2
06:00 PM - 07:00 PM	53.7	74.4	48.7
07:00 PM - 08:00 PM	53.0	73.2	46.4
08:00 PM - 09:00 PM	47.8	62.5	46.0
09:00 PM - 10:00 PM	45.9	57.3	44.8
10:00 PM - 11:00 PM	46.4	62.0	44.5
11:00 PM - 12:00 AM	51.0	77.2	44.7
12:00 AM - 01:00 AM	48.6	70.4	45.6
01:00 AM - 02:00 AM	46.8	69.5	45.1
02:00 AM - 03:00 AM	46.9	60.6	45.9
03:00 AM - 04:00 AM	49.4	73.0	45.5
04:00 AM - 05:00 AM	53.4	76.4	46.5
05:00 AM - 06:00 AM	52.5	69.1	46.6
06:00 AM - 07:00 AM	58.3	75.9	53.6
07:00 AM - 08:00 AM	57.8	79.7	52.0
08:00 AM - 09:00 AM	51.1	68.4	46.9
09:00 AM - 10:00 AM	48.7	59.9	45.8
10:00 AM - 11:00 AM	48.3	58.3	45.6
Leq Average 24 hrs. (dB(A))	51.7		
Lmax (dB(A))		79.7	
L90 (dB(A))			45.5
Ldn (dB(A))	58.5		
Standard (dB(A))	70	115	

Reference Method : ISO 1996-1 : 2016
Standard : 1. ประกาศคณะกรรมการสิ่งแวดล้อมแห่งชาติ ฉบับที่ 15 (พ.ศ. 2540) เรื่องกำหนดมาตรฐานระดับเสียงโดยทั่วไป
2. ประกาศกระทรวงอุตสาหกรรม เรื่องกำหนดค่าระดับเสียงการรบกวน และระดับเสียงที่เกิดจากการประกอบกิจการโรงงาน พ.ศ. 2548

Technical Management Chontichak
Chonticha Subongkoch
Scientist (3)

Approved by Supot S
Supot Salamteh
Section Head

The above results are valid only for the analyzed/tested sample(s) as indicated in this report. No part of this report or certificate may be reproduced in any from without written consent from the Laboratory. ALS Laboratory Group (Thailand) strongly recommends that this report is not reproduced except in full.

ADDRESS 616/10 Moo 5 T. Maenam Khu A. Pluakdaeng Rayong 21140 Thailand | PHONE +66 0 3304 8555 | FAX +66 0 3304 8556
Life Sciences www.alsglobal.com
RIGHT SOLUTIONS RIGHT PARTNER
8525-209/ EMAIL

ภาคผนวก ค-5

ผลตรวจวัดระดับเสียงแยกความถี่ (Octave Band)

Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130
P/O : 4518158708
Project Name : Environmental Quality Monitoring
Project Location : AIE_DMC-Polyol Plant

Lot ID: 265460
Date Received : Feb 12, 2026
Date Reported : Feb 17, 2026
Report Number : 3509835-1

Sample Number 265460-1
Parameter Octave Band
Location หน่วยทำปฏิกิริยา
Measurement Date Feb 11, 2026
Measurement By Apichart Wilars

Time	Result (dB(A))											
	Leq	16 Hz	31.5 Hz	63 Hz	125 Hz	250 Hz	500 Hz	1 kHz	2 kHz	4 kHz	8 kHz	16 kHz
09:00 AM - 10:00 AM	78.6	19.3	34.9	46.9	58.6	62.7	68.4	70.5	70.3	75.0	69.8	56.2
10:00 AM - 11:00 AM	77.5	19.9	34.8	46.6	58.1	61.8	66.1	68.4	67.9	74.5	69.3	55.4
11:00 AM - 12:00 PM	77.5	19.9	35.8	46.8	58.8	61.8	66.7	68.5	67.9	74.3	69.1	55.8
12:00 PM - 01:00 PM	77.9	20.9	35.8	46.8	57.9	61.8	67.0	69.1	68.4	75.0	69.0	55.8
01:00 PM - 02:00 PM	78.0	19.9	35.9	46.7	57.7	62.0	66.8	69.1	68.4	75.3	69.0	55.8
02:00 PM - 03:00 PM	78.9	19.7	35.4	46.9	58.1	69.3	67.2	69.7	69.0	75.7	69.2	55.9
03:00 PM - 04:00 PM	79.3	19.6	36.3	47.2	58.7	64.3	68.5	71.9	71.3	75.7	69.5	56.3
04:00 PM - 05:00 PM	79.4	19.6	36.6	47.5	58.2	64.3	68.8	72.1	71.4	75.6	69.6	56.4
Average	78.4	19.9	35.7	46.9	58.3	64.4	67.5	70.1	69.6	75.2	69.3	56.0

Reference Method : ANSI Standard S1.6-1984

Technical Management Orawan Rakyong
Scientist (3)

Approved by Supot Salamteh
Section Head

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130
P/O : 4518158708
Project Name : Environmental Quality Monitoring
Project Location : AIE_DMC-Polyol Plant

Lot ID: 265460
Date Received : Feb 12, 2026
Date Reported : Feb 17, 2026
Report Number : 3509836-1

Sample Number 265460-2
Parameter Octave Band
Location หอหล่อเย็น
Measurement Date Feb 11, 2026
Measurement By Apichart Wilars

Time	Result (dB(A))											
	Leq	16 Hz	31.5 Hz	63 Hz	125 Hz	250 Hz	500 Hz	1 kHz	2 kHz	4 kHz	8 kHz	16 kHz
09:00 AM - 10:00 AM	78.0	23.8	39.6	52.2	65.3	66.4	69.7	71.7	71.1	70.6	67.7	55.8
10:00 AM - 11:00 AM	77.5	24.9	39.2	51.9	64.9	66.1	69.2	71.1	70.4	70.4	67.5	55.5
11:00 AM - 12:00 PM	78.1	25.4	40.0	52.2	65.4	67.0	70.6	71.6	70.9	70.5	67.9	56.3
12:00 PM - 01:00 PM	78.7	27.4	40.6	52.2	65.7	67.8	71.5	72.3	71.5	70.9	68.0	56.4
01:00 PM - 02:00 PM	78.6	26.8	40.2	52.0	65.4	67.6	71.1	72.1	71.4	71.1	68.3	56.9
02:00 PM - 03:00 PM	78.1	27.1	40.4	52.0	65.5	66.9	70.1	71.4	71.1	70.9	68.2	56.8
03:00 PM - 04:00 PM	78.0	28.6	41.9	52.3	65.2	66.6	70.1	71.5	71.0	70.6	68.0	56.6
04:00 PM - 05:00 PM	77.8	27.1	41.7	52.4	65.1	66.7	69.7	71.4	70.7	70.3	67.7	56.4
Average	78.1	26.6	40.5	52.2	65.3	66.9	70.3	71.7	71.0	70.7	67.9	56.4

Reference Method : ANSI Standard S1.6-1984

Technical Management Orawan Rakyong
Scientist (3)

Approved by Supot Salamteh
Section Head

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand | PHONE +66 0 2760 3000 | FAX +66 0 2760 3197
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company
Life Sciences www.alsglobal.com
RIGHT SOLUTIONS RIGHT PARTNER
8525-81/ EMAIL
S:\Reports_Air Noise_Octave band.rpt (1:34PM)

Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130
P/O : 4518158712
Project Name : Environmental Quality Monitoring
Project Location : AIE_Rigid Polyol Plant

Lot ID: 265929
Date Received : Feb 12, 2026
Date Reported : Feb 17, 2026
Report Number : 3509846-1

Sample Number 265929-1
Parameter Octave Band
Location หน่วยทำปฏิกิริยาของสายการผลิตที่ 2
Measurement Date Feb 11, 2026
Measurement By Apichart Wilars

Time	Result (dB(A))											
	Leq	16 Hz	31.5 Hz	63 Hz	125 Hz	250 Hz	500 Hz	1 kHz	2 kHz	4 kHz	8 kHz	16 kHz
09:19 AM - 10:19 AM	80.3	16.2	32.2	45.9	55.9	64.8	69.5	70.7	74.2	77.4	64.5	43.6
10:19 AM - 11:19 AM	80.2	16.5	31.5	45.8	55.9	65.1	69.3	70.7	74.0	77.3	64.5	43.7
11:19 AM - 12:19 PM	81.6	17.7	31.4	48.8	57.6	66.7	70.3	72.5	74.9	78.6	67.4	45.2
12:19 PM - 01:19 PM	81.4	17.5	31.5	47.8	57.6	66.3	70.6	72.2	74.6	78.5	67.3	45.0
01:19 PM - 02:19 PM	81.0	16.5	31.5	44.9	55.1	63.2	68.7	70.5	74.1	78.6	68.5	45.6
02:19 PM - 03:19 PM	79.7	17.1	31.2	45.6	54.7	62.3	68.3	69.9	73.8	76.7	64.8	44.3
03:19 PM - 04:19 PM	79.6	16.8	31.6	45.6	54.8	62.6	68.6	69.7	73.5	76.8	64.5	44.1
04:19 PM - 05:19 PM	80.1	32.5	45.5	54.7	60.2	64.9	69.1	70.2	73.8	77.2	64.7	45.0
Average	80.5	24.2	37.6	48.8	56.9	64.8	69.4	70.9	74.1	77.7	66.1	44.6

Reference Method : ANSI Standard S1.6-1984

Technical Management Orawan R.
Orawan Rakyong
Scientist (3)

Approved by Supt S.
Supot Salamteh
Section Head

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130
P/O : 4518158712
Project Name : Environmental Quality Monitoring
Project Location : AIE_Rigid Polyol Plant

Lot ID: 265929
Date Received : Feb 12, 2026
Date Reported : Feb 17, 2026
Report Number : 3509847-1

Sample Number 265929-2
Parameter Octave Band
Location หอหล่อเย็นของสายการผลิตที่ 2
Measurement Date Feb 11, 2026
Measurement By Apichart Wilars

Time	Result (dB(A))											
	Leq	16 Hz	31.5 Hz	63 Hz	125 Hz	250 Hz	500 Hz	1 kHz	2 kHz	4 kHz	8 kHz	16 kHz
09:39 AM - 10:39 AM	77.6	24.6	41.6	51.4	63.6	66.6	68.4	70.6	71.0	71.8	65.9	49.9
10:39 AM - 11:39 AM	77.2	24.6	40.9	51.5	63.4	66.2	67.9	70.1	70.5	71.5	65.8	49.6
11:39 AM - 12:39 PM	77.3	25.1	41.3	51.7	63.7	66.6	68.4	70.3	70.6	71.3	65.5	50.0
12:39 PM - 01:39 PM	77.4	25.9	41.0	51.6	63.5	66.7	68.7	70.5	70.7	71.3	65.4	49.9
01:39 PM - 02:39 PM	77.4	25.8	41.4	51.4	63.5	66.6	68.7	70.5	70.9	71.5	65.4	49.9
02:39 PM - 03:39 PM	77.3	26.3	41.9	51.4	63.5	67.1	68.3	70.2	70.6	71.4	65.4	49.9
03:39 PM - 04:39 PM	77.4	25.7	42.2	51.5	63.4	66.6	68.6	70.6	70.9	71.5	65.3	50.2
04:39 PM - 05:39 PM	77.7	26.2	42.8	52.0	64.0	67.3	69.0	70.9	71.2	71.6	65.1	50.4
Average	77.4	25.6	41.7	51.6	63.6	66.7	68.5	70.5	70.8	71.5	65.5	50.0

Reference Method : ANSI Standard S1.6-1984

Technical Management Orawan R.
Orawan Rakyong
Scientist (3)

Approved by Supt S.
Supot Salamteh
Section Head

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand | PHONE +66 0 2760 3000 | FAX +66 0 2760 3197
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company
Life Sciences www.alsglobal.com
RIGHT SOLUTIONS RIGHT PARTNER
8525-205/ EMAIL
S:\Reports_Air Noise_Octave band.rpt (1:40PM)

Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130
P/O : 4518158708
Project Name : Environmental Quality Monitoring
Project Location : AIE_DMC-Polyol Plant

Lot ID: 2635235
Date Received : May 11, 2026
Date Reported : May 19, 2026
Report Number : 3573993-1

Sample Number 2635235-1
Parameter Octave Band
Location หน่วยทำปฏิกิริยา
Measurement Date May 08, 2026
Measurement By Arnon Phoprathong

Time	Result (dB(A))											
	Leq	16 Hz	31.5 Hz	63 Hz	125 Hz	250 Hz	500 Hz	1 kHz	2 kHz	4 kHz	8 kHz	16 kHz
10:01 AM - 11:01 AM	75.3	20.4	35.9	47.7	59.5	64.2	67.5	68.5	67.6	69.2	65.5	54.1
11:01 AM - 12:01 PM	75.5	20.6	36.0	47.7	59.2	64.5	67.4	68.7	67.8	69.5	65.5	54.0
12:01 PM - 01:01 PM	75.5	20.9	36.4	47.9	59.4	64.6	67.4	68.8	67.8	69.3	65.2	53.9
01:01 PM - 02:01 PM	75.3	20.6	35.9	48.2	58.8	64.1	67.4	68.4	67.5	69.4	65.2	53.7
02:01 PM - 03:01 PM	75.6	21.8	36.1	48.3	59.8	64.1	67.4	69.0	67.9	69.7	65.6	54.1
03:01 PM - 04:01 PM	75.8	21.3	36.7	48.8	60.0	64.7	67.9	69.5	68.0	69.6	65.6	53.9
04:01 PM - 05:01 PM	75.5	21.0	36.6	48.3	59.4	64.9	67.4	69.1	67.8	69.2	65.3	53.8
05:01 PM - 06:01 PM	75.4	20.8	36.6	48.2	59.5	64.6	66.9	69.1	67.7	69.2	65.3	53.8
Average	75.5	20.9	36.3	48.2	59.5	64.5	67.4	68.9	67.8	69.4	65.4	53.9

Reference Method : ANSI Standard S1.6-1984

Technical Management Orawan Rakyong
Scientist (3)

Approved by Supot Salamteh
Section Head

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand | PHONE +66 0 2760 3000 | FAX +66 0 2760 3197
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences www.alsglobal.com
RIGHT SOLUTIONS RIGHT PARTNER

Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130
P/O : 4518158708
Project Name : Environmental Quality Monitoring
Project Location : AIE_DMC-Polyol Plant

Lot ID: 2635235
Date Received : May 11, 2026
Date Reported : May 19, 2026
Report Number : 3573994-1

Sample Number 2635235-2
Parameter Octave Band
Location หอหล่อเย็น
Measurement Date May 08, 2026
Measurement By Arnon Phoprathong

Time	Result (dB(A))											
	Leq	16 Hz	31.5 Hz	63 Hz	125 Hz	250 Hz	500 Hz	1 kHz	2 kHz	4 kHz	8 kHz	16 kHz
10:04 AM - 11:04 AM	78.1	25.0	39.9	51.9	63.1	65.1	69.7	72.3	71.1	71.4	67.4	55.7
11:04 AM - 12:04 PM	79.2	24.9	37.4	50.8	61.7	64.5	69.2	72.9	72.5	73.1	70.5	61.5
12:04 PM - 01:04 PM	78.7	24.9	41.1	53.1	65.8	68.0	71.7	72.8	71.1	70.9	66.6	54.6
01:04 PM - 02:04 PM	78.2	24.1	40.0	52.2	64.4	66.6	70.7	72.3	70.9	70.9	66.7	54.6
02:04 PM - 03:04 PM	78.6	26.3	40.2	52.0	63.4	65.9	70.7	72.9	71.9	71.6	67.1	54.9
03:04 PM - 04:04 PM	79.1	25.9	39.5	53.1	64.0	67.2	72.2	73.3	71.8	71.8	67.5	55.3
04:04 PM - 05:04 PM	79.3	25.9	39.5	52.7	64.0	67.9	72.8	73.5	71.8	71.7	67.4	55.3
05:04 PM - 06:04 PM	78.3	25.7	39.7	52.8	63.9	66.1	70.3	72.3	71.3	71.4	67.3	55.3
Average	78.7	25.4	39.8	52.4	63.9	66.6	71.1	72.8	71.6	71.7	67.7	56.6

Reference Method : ANSI Standard S1.6-1984

Technical Management Orawan Rakyong
Scientist (3)

Approved by Supot Salamteh
Section Head

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand | PHONE +66 0 2760 3000 | FAX +66 0 2760 3197
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company

Life Sciences www.alsglobal.com
RIGHT SOLUTIONS RIGHT PARTNER

8525-81/ EMAIL S:\Reports_Air Noise_Octave band.rpt (12:47PM)

Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130
P/O : 4518158712
Project Name : Environmental Quality Monitoring
Project Location : AIE_Rigid Polyol Plant

Lot ID: 2635243
Date Received : May 11, 2026
Date Reported : May 19, 2026
Report Number : 3573995-1

Sample Number 2635243-1
Parameter Octave Band
Location หน่วยทำปฏิกิริยาของสายการผลิตที่ 2
Measurement Date May 08, 2026
Measurement By Arnon Phoprathong

Time	Result (dB(A))											
	Leq	16 Hz	31.5 Hz	63 Hz	125 Hz	250 Hz	500 Hz	1 kHz	2 kHz	4 kHz	8 kHz	16 kHz
10:24 AM - 11:24 AM	80.1	32.5	45.5	54.7	60.2	64.9	69.1	70.2	73.8	77.2	64.7	45.0
11:24 AM - 12:24 PM	79.6	16.8	31.6	45.6	54.8	62.6	68.6	69.7	73.5	76.8	64.5	44.1
12:24 PM - 01:24 PM	79.7	17.1	31.2	45.6	54.7	62.3	68.3	69.9	73.8	76.7	64.8	44.3
01:24 PM - 02:24 PM	80.2	16.5	31.5	45.8	55.9	65.1	69.3	70.7	74.0	77.3	64.5	43.7
02:24 PM - 03:24 PM	80.3	16.2	32.2	45.9	55.9	64.8	69.5	70.7	74.2	77.4	64.5	43.6
03:24 PM - 04:24 PM	79.2	24.9	37.4	50.8	61.7	64.5	69.2	72.9	72.5	73.1	70.5	61.5
04:24 PM - 05:24 PM	78.8	24.6	38.0	51.2	62.5	64.4	69.0	72.5	71.8	72.7	70.4	61.5
05:24 PM - 06:24 PM	78.9	25.1	38.2	51.6	61.5	64.9	69.2	72.7	71.8	72.7	70.4	61.7
Average	79.6	25.6	38.7	50.2	59.5	64.3	69.0	71.3	73.3	75.9	67.7	57.4

Reference Method : ANSI Standard S1.6-1984

Technical Management Orawan R.
Orawan Rakyong
Scientist (3)

Approved by Supt S
Supot Salamteh
Section Head

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

Analysis / Test Report

Client : Dow Chemical Thailand Ltd.
10 Moo 2, Asia Industrial Estate, Tambol Banchang, Amphur Banchang, Rayong Thailand 21130
P/O : 4518158712
Project Name : Environmental Quality Monitoring
Project Location : AIE_Rigid Polyol Plant

Lot ID: 2635243
Date Received : May 11, 2026
Date Reported : May 19, 2026
Report Number : 3573996-1

Sample Number 2635243-2
Parameter Octave Band
Location หอหล่อเย็นของสายการผลิตที่ 2
Measurement Date May 08, 2026
Measurement By Arnon Phoprathong

Time	Result (dB(A))											
	Leq	16 Hz	31.5 Hz	63 Hz	125 Hz	250 Hz	500 Hz	1 kHz	2 kHz	4 kHz	8 kHz	16 kHz
10:00 AM - 11:00 AM	76.2	27.2	41.0	51.0	64.1	65.9	67.4	69.6	68.8	69.4	66.3	54.8
11:00 AM - 12:00 PM	76.5	28.4	41.1	51.2	64.4	66.6	68.1	69.8	68.9	69.5	66.3	54.8
12:00 PM - 01:00 PM	76.5	30.0	41.6	51.5	64.8	66.8	68.0	69.7	68.9	69.5	66.3	54.5
01:00 PM - 02:00 PM	76.1	28.0	40.9	51.5	63.8	66.3	67.6	69.4	68.6	69.1	65.9	54.3
02:00 PM - 03:00 PM	76.8	28.6	41.7	51.3	63.7	66.1	67.9	70.3	70.0	70.0	66.3	54.7
03:00 PM - 04:00 PM	76.6	27.9	41.9	51.2	63.7	66.5	68.3	70.0	69.0	69.8	66.7	55.1
04:00 PM - 05:00 PM	76.6	27.5	41.9	50.9	63.6	66.7	68.3	70.0	68.9	69.6	66.5	54.9
05:00 PM - 06:00 PM	76.8	28.6	41.7	51.3	63.7	66.1	67.9	70.3	70.0	70.0	66.3	54.7
Average	76.5	28.4	41.5	51.2	64.0	66.4	67.9	69.9	69.2	69.6	66.3	54.7

Reference Method : ANSI Standard S1.6-1984

Technical Management Orawan R.
Orawan Rakyong
Scientist (3)

Approved by Supt S
Supot Salamteh
Section Head

Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. The report shall not be reproduced except in full without the written approval of the laboratory.

ADDRESS 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand | PHONE +66 0 2760 3000 | FAX +66 0 2760 3197
ALS LABORATORY GROUP (THAILAND) CO., LTD. An ALS Limited Company
Life Sciences www.alsglobal.com
RIGHT SOLUTIONS RIGHT PARTNER
8525-205/ EMAIL
S:\Reports_Air Noise_Octave band.rpt (12:55PM)

ภาคผนวก ง

เอกสารการสอบเทียบเครื่องมือตรวจวิเคราะห์

right solutions.
right partner.

รายการเครื่องมือที่ใช้ในการวิเคราะห์ / ทดสอบ

Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Ambient	Propylene Oxide	DRYCAL FLOWMETER	BKK_FS0614	10-Sep-25	9-Sep-26	12
Ambient	Propylene Oxide	DRYCAL FLOWMETER	BKK_FS0619	10-Sep-25	9-Sep-26	12
Ambient	Propylene Oxide	Air Sampling Pump	RYG_FS0505	3-Apr-26	3-Jul-26	3
Ambient	Propylene Oxide	Air Sampling Pump	RYG_FS0683	3-Apr-26	3-Jul-26	3
Ambient	Propylene Oxide	Air Sampling Pump	RYG_FS0735	2-Apr-26	2-Jul-26	3
Ambient	Propylene Oxide	GC-FID	BKK_EN0126	22-Oct-25	21-Oct-26	12
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	RYG_FS0648	16-Jan-25	15-Jul-26	18
Workplace	Propylene Oxide (Personal),	DRYCAL FLOWMETER	BKK_FS0614	10-Sep-25	9-Sep-26	12
Workplace	Propylene Oxide (Area)	DRYCAL FLOWMETER	BKK_FS0619	10-Sep-25	9-Sep-26	12
Workplace		Air Sampling Pump	RYG_FS0672	2-Jan-26	2-Apr-26	3
Workplace		Air Sampling Pump	RYG_FS0126	6-Jan-26	6-Apr-26	3
Workplace		Air Sampling Pump	RYG_FS0513	7-Jan-26	7-Apr-26	3
Workplace		Air Sampling Pump	RYG_FS0511	7-Jan-26	7-Apr-26	3
Workplace		Air Sampling Pump	RYG_FS0127	7-Apr-26	7-Jul-26	3
Workplace		Air Sampling Pump	RYG_FS0158	7-Apr-26	7-Jul-26	3
Workplace		Air Sampling Pump	RYG_FS0367	7-Apr-26	7-Jul-26	3
Workplace		Air Sampling Pump	RYG_FS0517	7-Apr-26	7-Jul-26	3
Workplace	Propylene Oxide (Personal)	GC-FID	BKK_EN0126	22-Oct-25	21-Oct-26	12
Workplace	Propylene Oxide (Area)	GC-FID	BKK_EN0126	22-Oct-25	21-Oct-26	12
Noise	Leq 24 hrs	Sound Calibrator	RYG_FS0496	19-Mar-25	19-Mar-26	12
Noise	Leq 24 hrs	Sound Level Meter	RYG_FS0618	28-Jan-26	27-Jan-27	12
Noise	Leq 24 hrs	Sound Level Meter	RYG_FS0617	21-Jan-26	20-Jan-27	12
Noise	Octave Band	Sound Calibrator	RYG_FS0215	8-Oct-25	7-Oct-26	12
Noise	Octave Band	Sound Level Meter	RYG_FS0384	29-Oct-25	28-Oct-26	12
Noise	Octave Band	Sound Level Meter	RYG_FS0388	19-Mar-25	19-Mar-26	12
Noise	Octave Band	Sound Level Meter	RYG_FS0381	29-Oct-25	29-Oct-26	12
Noise	Octave Band	Sound Level Meter	RYG_FS0386	29-Oct-25	28-Oct-26	12
Noise	Octave Band	Sound Calibrator	RYG_FS0213	9-Jan-26	8-Jan-27	12
Noise	Octave Band	Sound Level Meter	RYG_FS0439	5-Nov-25	4-Nov-26	12
Noise	Octave Band	Sound Level Meter	RYG_FS0627	21-Jan-26	20-Jan-27	12
Noise	Octave Band	Sound Level Meter	RYG_FS0438	29-Oct-25	28-Oct-26	12
Noise	Octave Band	Sound Level Meter	RYG_FS0622	21-Jan-26	20-Jan-27	12
Rayong Lab	BOD	DO meter with Sensor	RYG_EN0032	20-Jan-25	20-Jul-26	18
Rayong Lab	BOD	Incubator	RYG_EN0154	18-Mar-26	18-Sep-27	18
Rayong Lab	BOD	Burette	RYG_EN0216	18-Sep-25	18-Sep-26	12
Rayong Lab	COD	Spectrophotometer	RYG_EN0037	18-Mar-25	18-Sep-26	18
Rayong Lab	pH at 25 °C	pH meter	RYG_EN0183	18-Jul-25	18-Jan-27	18
Rayong Lab	Oil & Grease	Electronic Balance	RYG_EN0003	3-Feb-26	3-Feb-27	12
Rayong Lab	Oil & Grease	Liquid Bath (Water)	RYG_EN0220	27-Nov-25	27-Nov-26	12
Rayong Lab	Total Dissolved Solids 180°C	Electronic Balance	RYG_EN0163	3-Feb-26	3-Feb-27	12
Rayong Lab	Total Dissolved Solids 180°C	Chamber (Oven)	RYG_EN0012	10-Sep-25	10-Mar-27	18

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate of Calibration

Customer

Certificate No : 25-AFM-208

Name : ALS Laboratory Group Thailand Co., Ltd.

Request No : Req-2025-1986

Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang, Bangkok 10250

Unit Under Calibration Details

Measurement Item : Air Flow Meter

Manufacturer : Mesa Labs

Sensor Model : -

Model : 200-510M

Sensor Serial Number : -

Serial Number : 151114

Instrument Status : Used

ID : BKK_FS0614

Location of Calibration : LAB 4 AIR VELOCITY METER

Calibration Environment and Details

Temperature : 23 °C ± 3 °C

Humidity : 55 %RH ± 20 %RH

Barometric Pressure : 1013 hPa ± 10 hPa

Received Date : 3 September 2025

Calibration Date : 10 September 2025

Calibration Procedure : In-house method CP-AFM-01 by Comparison technique with Standard Primary Flow Calibrator

REVIEW BY .....

APPROVED BY .....

NEXT CAL DATE..... 09/09/26

Reference Standard	Model	Serial Number	Traceble	Due Calibration
Air Flow Meter	Gilibrator 3 Low flow	18501010006	Sensidyne	5 May 2026
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	6 May 2026
Temperature meter	GT 11	08000057	Qreborn	15 October 2025
Pressure meter	CPG2400	41000KDU/651882	TPA	21 October 2025

Traceability :

This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01 and MIT NSC-TISI-TIS Accreditation No. 0052

Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k = 2, providing a level of confidence approximately 95 %.

Calibration By :

Mr. Noppadon Luangart

Service Calibration Engineer

Approved By :

Mr. Pacit Mathavorn

Calibration Engineer Supervisor

Issue Date : 10 September 2025

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate No : 25-AFM-208

Request No : Req-2025-1986

Result of Calibration : Without Adjustment

STD Reading			UUC Readinng			Error	Uncertainty		
Temperature (°C)	Pressure (kPa)	Flow (cc/min)	Temperature (°C)	Pressure (kPa)	Flow (cc/min)	(cc/min)	(cc/min)	(°C)	(kPa)
25.5	100.98	100	-	-	100.02	0.0	3.6	1.0	0.50
25.7	100.97	503	-	-	500.81	-2.2	9.5	1.0	0.50
25.8	100.89	1003	-	-	1000.4	-3	19	1.0	0.50
26.1	100.88	2000	-	-	2001.9	2	38	1.0	0.50
26.5	100.85	3014	-	-	3002.2	-12	57	1.0	0.50
26.7	100.81	4027	-	-	4000.9	-26	76	1.0	0.50
27.0	100.74	5048	-	-	5001.8	-46	95	1.0	0.50

Note STD : Standard UUC : Unit Under Calibration

- UUC Reference Condition : At atmospheric pressure and room temperature condition, Air
- Flow Rate was corrected for non-standard operating condition by using equation :

$$Qmeas = \mathrm{Qref}\, x \frac{\mathrm{Pref}}{\mathrm{Pmeas}} x \frac{\mathrm{Tmeas}}{\mathrm{Tref}}$$

where Q = Flow Rate P = Absolute Pressure T = Absolute Temperature

meas = Measurement Condition ref = Standard Condition

* Indicates non accredited

End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

FM-708-AFM-01 Rev.06 Issue date 21/2/25

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate of Calibration

Customer

Name : ALS Laboratory Group Thailand Co., Ltd.

Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang, Bangkok 10250

Certificate No : 25-AFM-207

Request No : Req-2025-1987

Unit Under Calibration Details

Measurement Item : Air Flow Meter

Manufacturer : Mesa Labs

Model : 200-510L

Serial Number : 130026

ID : BKK_FS0619

Location of Calibration : LAB 4 AIR VELOCITY METER

Sensor Model : -

Sensor Serial Number : -

Instrument Status : Used

REVIEW BY .....

APPROVED BY .....

NEXT CAL DATE..... 09/09/26

Calibration Environment and Details

Temperature : 23 °C ± 3 °C

Humidity : 55 %RH ± 20 %RH

Barometric Pressure : 1013 hPa ± 10 hPa

Received Date : 3 September 2025

Calibration Date : 10 September 2025

Calibration Procedure : In-house method CP-AFM-01 by Comparison technique with Standard Primary Flow Calibrator

Reference Standard	Model	Serial Number	Traceble	Due Calibration
Air Flow Meter	Gilibrator 3 Low flow	18501010006	Sensidyne	5 May 2026
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	6 May 2026
Temperature meter	GT 11	08000057	Qreborn	15 October 2025
Pressure meter	CPG2400	41000KDU/651882	TPA	21 October 2025

Traceability :

This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01 and MIT NSC-TISI-TIS Accreditation No. 0052

Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k = 2, providing a level of confidence approximately 95 %.

Calibration By :

Mr. Noppadon Luangart

Service Calibration Engineer

Approved By :

Mr. Pacit Mathavorn

Calibration Engineer Supervisor

Issue Date : 10 September 2025

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate No : 25-AFM-207

Request No : Req-2025-1987

Result of Calibration : Without Adjustment

STD Reading			UUC Readinng			Error	Uncertainty		
Temperature (°C)	Pressure (kPa)	Flow (cc/min)	Temperature (°C)	Pressure (kPa)	Flow (cc/min)	(cc/min)	(cc/min)	(°C)	(kPa)
25.5	100.98	20	-	-	20.042	0.0	1.6	1.0	0.50
25.5	100.90	50	-	-	49.921	-0.1	4.0	1.0	0.50
25.5	100.91	100	-	-	100.09	0.1	3.6	1.0	0.50
25.4	100.86	150	-	-	150.34	0.3	5.4	1.0	0.50
25.6	100.93	199	-	-	200.17	1.2	7.2	1.0	0.50
25.6	100.95	301	-	-	300.05	-1	11	1.0	0.50
25.7	100.96	402	-	-	401.03	-1	14	1.0	0.50
25.7	100.95	503	-	-	500.26	-3	10	1.0	0.50

Note STD : Standard UUC : Unit Under Calibration

- UUC Reference Condition : At atmospheric pressure and room temperature condition, Air
- Flow Rate was corrected for non-standard operating condition by using equation :

$$Qmeas = \mathrm{Qref}\, x\, \frac{\mathrm{Pref}}{\mathrm{Pmeas}}\, x\, \frac{\mathrm{Tmeas}}{\mathrm{Tref}}$$

where Q = Flow Rate P = Absolute Pressure T = Absolute Temperature

meas = Measurement Condition ref = Standard Condition

* Indicates non accredited

End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

FM-708-AFM-01 Rev.06 Issue date 21/2/25

ALS Laboratory Group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Phatthanakan, Suan Luang, Bangkok 10250
T +66 2 760 3000 F +66 2 760 3197

Certificate of Calibration

Certificate No. C-030426-RYG_FS0505

Air Sampling Pump Detail

Equipment name	: Personal Air Sampling Pump	Equiment ID	: RYG_FS0505
Brand	: Gilian	Serial No.	: 20201110096
Model/Type	: GilAir Plus	Calibration Date	: 03-Apr-26
		Next calibration date	: 03-Jul-26

Reference Standard Low Flow Meter

Equipment name	: Air Flow Meter	Equiment ID	: BKK_FS0619
Brand	: MesaLabs	Serial No.	: 130026
Model/Type	: Defender 510-L	Calibration Date	: 10-Sep-25
		Due Date	: 09-Sep-26

Reference Standard High Flow Meter

Equipment name	: Air Flow Meter	Equiment ID	: BKK_FS0614
Brand	: MesaLabs	Serial No.	: 151114
Model/Type	: Defender 510-M	Calibration Date	: 10-Sep-25
		Due Date	: 09-Sep-26

Calibration Data

Air Sampling Pump setting (cc/min)	Reference Std. Flow Reading (cc/min)			Avg. (cc/min)	%Error acceptance	Acceptable range (cc/min)	Evaluation (Pass/ Fail)
	1	2	3				
Low Flow							
20	20.2	20.1	20.1	20.1	5%	19 - 21	Passed
50	50.0	50.1	49.3	49.8	5%	48 - 53	Passed
100	101.8	101.6	101.4	101.6	5%	95 - 105	Passed
200	200.7	200.7	201.9	201.1	5%	190 - 210	Passed
High Flow							
500	497.9	496.8	490.7	495.1	3%	485 - 515	Passed
1000	1002.7	999.2	1000.2	1000.7	3%	970 - 1030	Passed
2000	2006.5	2009.3	2009.3	2008.4	3%	1940 - 2060	Passed
2500	2505.1	2499.6	2499.0	2501.2	3%	2425 - 2575	Passed

---------- END OF REPORT ----------

Calibrated By: นันทวัฒน์

(Mr. Nantawat Sarin)

RYG Field Services Scientist (1)

Approved By: Supot S.

(Mr. Supot Salamteh)

Field Services Section Head

Issue date : 04-Apr-26

ALS Laboratory Group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Phatthanakan, Suan Luang, Bangkok 10250
T +66 2 760 3000 F +66 2 760 3197

Certificate of Calibration

Certificate No. C-030426-RYG_FS0683

Air Sampling Pump Detail

Equipment name	: Personal Air Sampling Pump	Equiment ID	: RYG_FS0683
Brand	: Gilian	Serial No.	: 20221110023
Model/Type	: GilAir Plus	Calibration Date	: 03-Apr-26
		Next calibration date	: 03-Jul-26

Reference Standard Low Flow Meter

Equipment name	: Air Flow Meter	Equiment ID	: BKK_FS0619
Brand	: MesaLabs	Serial No.	: 130026
Model/Type	: Defender 510-L	Calibration Date	: 10-Sep-25
		Due Date	: 09-Sep-26

Reference Standard High Flow Meter

Equipment name	: Air Flow Meter	Equiment ID	: BKK_FS0614
Brand	: MesaLabs	Serial No.	: 151114
Model/Type	: Defender 510-M	Calibration Date	: 10-Sep-25
		Due Date	: 09-Sep-26

Calibration Data

Air Sampling Pump setting (cc/min)	Reference Std. Flow Reading (cc/min)			Avg. (cc/min)	%Error acceptance	Acceptable range (cc/min)	Evaluation (Pass/ Fail)
	1	2	3				
Low Flow							
20	20.2	20.3	20.3	20.3	5%	19 - 21	Passed
50	49.7	49.8	50.0	49.8	5%	48 - 53	Passed
100	99.8	102.7	102.8	101.8	5%	95 - 105	Passed
200	202.2	201.8	201.1	201.7	5%	190 - 210	Passed
High Flow							
500	512.5	510.5	510.2	511.1	3%	485 - 515	Passed
1000	998.8	995.3	988.3	994.1	3%	970 - 1030	Passed
2000	2015.0	2014.5	2010.6	2013.4	3%	1940 - 2060	Passed
2500	2516.3	2513.6	2500.0	2510.0	3%	2425 - 2575	Passed
4000	4019.5	4033.7	4016.5	4023.2	3%	3880 - 4120	Passed

---------- END OF REPORT ----------

Calibrated By: ณัชชพล

(Mr. Natchapon Thamklang)

RYG Field Services Scientist (1)

Approved By: Supot S.

(Mr. Supot Salamteh)

Field Services Section Head

Issue date : 04-Apr-26

ALS Laboratory Group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Phatthanakan, Suan Luang, Bangkok 10250
T +66 2 760 3000 F +66 2 760 3197

Certificate of Calibration

Certificate No. C-020426-RYG_FS0735

Air Sampling Pump Detail

Equipment name	: Personal Air Sampling Pump	Equiment ID	: RYG_FS0735
Brand	: Gilian	Serial No.	: 20241110173
Model/Type	: GilAir Plus	Calibration Date	: 02-Apr-26
		Next calibration date	: 02-Jul-26

Reference Standard Low Flow Meter

Equipment name	: Air Flow Meter	Equiment ID	: BKK_FS0619
Brand	: MesaLabs	Serial No.	: 130026
Model/Type	: Defender 510-L	Calibration Date	: 10-Sep-25
		Due Date	: 09-Sep-26

Reference Standard High Flow Meter

Equipment name	: Air Flow Meter	Equiment ID	: BKK_FS0614
Brand	: MesaLabs	Serial No.	: 151114
Model/Type	: Defender 510-M	Calibration Date	: 10-Sep-25
		Due Date	: 09-Sep-26

Calibration Data

Air Sampling Pump setting (cc/min)	Reference Std. Flow Reading (cc/min)			Avg. (cc/min)	%Error acceptance	Acceptable range (cc/min)			Evaluation (Pass/ Fail)
	1	2	3						
Low Flow									
20	20.3	20.8	20.5	20.5	5%	19	-	21	Passed
50	50.2	50.3	49.5	50.0	5%	48	-	53	Passed
100	101.3	101.6	101.1	101.3	5%	95	-	105	Passed
200	202.1	203.7	203.4	203.1	5%	190	-	210	Passed
High Flow									
500	505.4	505.3	508.6	506.4	3%	485	-	515	Passed
1000	996.5	1002.1	999.6	999.4	3%	970	-	1030	Passed
2000	2003.4	2002.6	2002.0	2002.7	3%	1940	-	2060	Passed
2500	2497.7	2504.7	2501.9	2501.4	3%	2425	-	2575	Passed

---------- END OF REPORT ----------

Calibrated By: นันทวัฒน์

(Mr. Nantawat Sarin)
RYG Field Services Scientist (1)

Approved By: Supot S

(Mr. Supot Salamteh)
Field Services Section Head

Issue date : 03-Apr-26

© 2025 by Agilent Technologies

Agilent CrossLab Compliance Services

REVIEW BY: linda K.
APPROVED BY: Sm
NEXT CAL DATE: 21/10/26

Certificate of System Qualification

GC-OQ

System ID:	BKK_EN0126_GC6
Organization Name:	ALS Laboratory Group (Thailand) Co., Ltd.
Organization Location:	104 Soi 40 Phattanakan Rd., Khwang Suan Luang, Khet Suan Luang, BANGKOK 10250
Date:	October 22, 2025 2:51:58 PM
EQP Name:	AgilentRecommended
EQP Revision:	GC.02.53
Overall Qualification Status:	Pass

CDS Logon Verification - GC

Logon: Suriya Thongkaew

Overall CDS Logon Verification - GC Test Status

Pass

System Inspection and Basic Safety and Operation

Name: 7890

Setpoint Status: **Pass**

Overall System Inspection and Basic Safety and Operation Test Status

Pass

Inlet Pressure Decay

Name: 7890
Front SSL

Setpoint Status: **Pass**

Pressure: 25.0 psi

Pressure Change: 0.3 psi /5 minutes

Agilent Recommended: >= -2.0 and <= 0.5

Overall Inlet Pressure Decay Test Status

Pass

Inlet Pressure Accuracy

Name: 7890

Front SSL

Setpoint Status: **Pass**

	Setpoint		Actual	
Inlet Pressure:	25.0	psi	25.2	psi

Accuracy: 0.2 psi

Agilent Recommended: <= 1.2

Overall Inlet Pressure Accuracy Test Status

Pass

Inlet Pressure Decay

Name: 7890

Back SSL

Setpoint Status: **Pass**

Pressure: 25.0 psi

Pressure Change: 0.4 psi /5 minutes

Agilent Recommended: >= -2.0 and <= 0.5

Overall Inlet Pressure Decay Test Status

Pass

Inlet Pressure Accuracy

Name: 7890

Back SSL

Setpoint Status: **Pass**

	Setpoint		Actual	
Inlet Pressure:	25.0	psi	25.2	psi

Accuracy: 0.2 psi

Agilent Recommended: <= 1.2

Overall Inlet Pressure Accuracy Test Status

Pass

22111dijeuifhuie1

Detector Flow Accuracy

Name: 7890

Front FID

Setpoint Status: **Pass**

Flow Type: Fuel

Setpoint: 30.0 mL/min Measured Flow: 30.8 mL/min

Accuracy: 0.8 mL/min

Agilent Recommended: <= 10.0 % setpoint (3.0 ml/min)

Limit is percentage of setpoint or 0.5 ml/minute, whichever is largest.

Setpoint Status: **Pass**

Flow Type: Oxidizer

Setpoint: 400.0 mL/min Measured Flow: 396.0 mL/min

Accuracy: 4.0 mL/min

Agilent Recommended: <= 10.0 % setpoint (40.0 ml/min)

Limit is percentage of setpoint or 0.5 ml/minute, whichever is largest.

Setpoint Status: **Pass**

Flow Type: Makeup

Setpoint: 25.0 mL/min Measured Flow: 24.7 mL/min

Accuracy: 0.3 mL/min

Agilent Recommended: <= 10.0 % setpoint (2.5 ml/min)

Limit is percentage of setpoint or 0.5 ml/minute, whichever is largest.

Overall Detector Flow Accuracy Test Status

Pass

Detector Flow Accuracy

Name: 7890

Back FID

Setpoint Status: **Pass**

Flow Type: Fuel

Setpoint: 30.0 mL/min Measured Flow: 29.5 mL/min

Accuracy: 0.5 mL/min

Agilent Recommended: <= 10.0 % setpoint (3.0 ml/min)

Limit is percentage of setpoint or 0.5 ml/minute, whichever is largest.

Setpoint Status: **Pass**

Flow Type: Oxidizer

Setpoint: 400.0 mL/min Measured Flow: 397.0 mL/min

Accuracy: 3.0 mL/min

Agilent Recommended: <= 10.0 % setpoint (40.0 ml/min)

Limit is percentage of setpoint or 0.5 ml/minute, whichever is largest.

Setpoint Status: **Pass**

Flow Type: Makeup

Setpoint: 25.0 mL/min Measured Flow: 24.8 mL/min

Accuracy: 0.2 mL/min

Agilent Recommended: <= 10.0 % setpoint (2.5 ml/min)

Limit is percentage of setpoint or 0.5 ml/minute, whichever is largest.

Overall Detector Flow Accuracy Test Status

Pass

GC Oven Temperature Accuracy

Name: 7890

Setpoint Status: **Pass**

Zone: Oven

Setpoint/Actual

Temperature: 230.0 229.1 °C

Accuracy: -0.9 °C

Agilent Recommended: >= -1.0 % setpoint in K (-5.0 °C)

<= 1.0 % setpoint in K (5.0 °C)

Setpoint Status: **Pass**

Zone: Oven

Setpoint/Actual

Temperature: 100.0 99.9 °C

Accuracy: -0.1 °C

Agilent Recommended: >= -1.0 % setpoint in K (-3.7 °C)

<= 1.0 % setpoint in K (3.7 °C)

22111dijeuifhuie1

Overall GC Oven Temperature Accuracy Test Status

Pass

GC Oven Temperature Stability

Name: 7890

Setpoint Status: **Pass**

Setpoint/Average

Temperature: 100.0 99.95 °C

Stability: 0.1 °C

Agilent Recommended: <= 0.5

Overall GC Oven Temperature Stability Test Status

Pass

Scouting Run

Tested Combination1 Front SSL / Front FID

Injection Tower

Name: 7693A

Setpoint Status: Completed

Injection Volume on Column: 1.0 uL

Overall Scouting Run Status

Completed

Noise and Drift

Tested Combination1 Front SSL / Front FID

Name: 7890

Setpoint Status: Pass

Base Signal: 14.3 pA

		ASTM Noise pA		Drift pA/h
		0.05		0.03
Agilent Recommended:	<=	0.10	<=	2.50
Status:		Pass		Pass

Overall Noise and Drift Test Status

Pass

Injection Precision

Tested Combination1 Front SSL / Front FID

Name: 7693A

Setpoint Status: Pass

Injection Volume on Column: 1.0 uL

Area RSD:		0.33	%	Retention Time RSD:	0.10 %
Agilent Recommended:	<=	3.00		<=	1.00

Overall Injection Precision Test Status

Pass

Signal to Noise

Tested Combination1 Front SSL / Front FID
Injection Tower

Name: 7890

Setpoint Status: Pass

Signal to Noise: 1393680

Agilent Recommended: >= 300000

Overall Signal to Noise Test Status

Pass

Scouting Run

Tested Combination2 Back SSL / Back FID
Injection Tower

Name: 7693A

Setpoint Status: Completed

Injection Volume on Column: 1.0 uL

Overall Scouting Run Status

Completed

Noise and Drift

Tested Combination2 Back SSL / Back FID

Name: 7890

Setpoint Status: Pass

Base Signal: 13.3 pA

		ASTM Noise pA		Drift pA/h
		0.05		0.01
Agilent Recommended:	<=	0.10	<=	2.50
Status:		Pass		Pass

Overall Noise and Drift Test Status

Pass

Injection Precision

Tested Combination2	Back	SSL	/ Back	FID
Name:	7693A			

Setpoint Status: **Pass**

Injection Volume on Column: 1.0 uL

Area RSD:	0.43 %		Retention Time RSD:	0.09 %	
Agilent Recommended:	<=	3.00		<=	1.00

Overall Injection Precision Test Status

Pass

Signal to Noise

Tested Combination2	Back	SSL	/ Back	FID
	Injection Tower			
Name:	7890			

Setpoint Status: **Pass**

Signal to Noise:		1251862
Agilent Recommended:	>=	300000

Overall Signal to Noise Test Status

Pass

Instrument Details

Purpose

This section describes the as found system configuration.

Details

System

System ID	BKK_EN0126_GC6
Manufacturer	Agilent Technologies
Name	7890
Flow Data Input	Manual Data
Temperature Data Input	Manual Data or Other Data Logging

Tested Combination1

Injection Technique	Injection Tower
Sampler Identifier	Sampler 1
Inlet	Front
Detector	Front
LTM Included?	No

Tested Combination2

Injection Technique	Injection Tower
Sampler Identifier	Sampler 2
Inlet	Back
Detector	Back
LTM Included?	No

Sampler 1

Manufacturer	Agilent Technologies
Type	Injection Tower
Name	7693A
Model Number	G4513A
Serial Number	CN10340103
Firmware Revision	A.11.06
Usage	Sample Injection
Location	Front
Syringe Volume (µL)	10

Sampler 2

Manufacturer	Agilent Technologies
Type	Injection Tower
Name	7693A
Model Number	G4513A
Serial Number	CN16280128
Firmware Revision	A.11.06
Usage	Sample Injection
Location	Back
Syringe Volume (µL)	10

Sampler 3

Manufacturer	Agilent Technologies
Type	Tray
Name	7693A
Model Number	G4514A
Serial Number	CN18250032
Firmware Revision	A.12.04
Vial Heater	Not installed

Mainframe 1

Manufacturer	Agilent Technologies
Name	7890
Model Number	G3440A
Serial Number	CN11461066
Firmware Revision	A.01.16
Component ID/Asset No.	BKK_EN0126_GC-6
Oven Type	Standard

© 2025 by Agilent Technologies Agilent CrossLab Compliance Services

Inlet 1

Manufacturer	Agilent Technologies
Name	7890
Type	SSL
Location	Front
Carrier Gas	Helium
Control Type	Electronic Pressure Control (EPC)
Purged Inlet	Yes

Inlet 2

Manufacturer	Agilent Technologies
Name	7890
Type	SSL
Location	Back
Carrier Gas	Helium
Control Type	Electronic Pressure Control (EPC)
Purged Inlet	Yes

Detector 1

Manufacturer	Agilent Technologies
Name	7890
Type	FID
Adapter	Capillary
Control Type	Electronic Pressure Control (EPC)
Location	Front
Makeup Gas	Nitrogen

Detector 2

Manufacturer	Agilent Technologies
Name	7890
Type	FID
Adapter	Capillary
Control Type	Electronic Pressure Control (EPC)
Location	Back
Makeup Gas	Nitrogen

Electronic Signature

Purpose

This signature page was created and published because the ACE sign-off action was executed, which is valid for the entire document, including attachments. The ACE sign-off is an electronic signature that requires two distinct identification components: unique username and personal password. The Agilent representative who has delivered this service understands the meaning and legal status of an electronic signature. As a trained official operator, the Agilent representative has a unique password and logon to access ACE and electronically sign this document. (Other e-signatures can be applied to this document using a Document Content Management or other suitable method defined in your data access and control procedures.)

Details

Full Name of Signer:	Suriya Thongkaew
Logged On User Name:	suriya.thongkaew@non.agilent.com
Signature Creation Date:	October 22, 2025
Reason for Signature:	Executed protocol and published this original version of document

ACE Self Qualification Status

The installed version of ACE used to deliver this service passed qualification; the results conform with expected values. The self qualification summary report is available in the session folder location SDS\ClearStore\AceSelfQualification.

Regulatory Disclaimer

This document provides a protocol to verify and record instrument configuration and evidence of proper operation. It has been prepared from our interpretation of applicable regulations as well as industry best practices. The document is designed to provide an important component of a complete compliance package. Validation depends upon many factors and use of this protocol alone does not assure compliance. Agilent Technologies makes no promises or representations as to its sufficiency for any specific regulatory program.

Warranty

Agilent Technologies makes no warranty of any kind to this material, including but not limited to, the implied warranties or merchantability and fitness for a particular purpose. Agilent Technologies shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance, or use of this material.

© 2025 by Agilent Technologies Agilent CrossLab Compliance Services

User Name: suriya.thongkaew
Report Generated by Hostname: DESKTOP-2H6MTKJ

System Id: BKK_EN0126_GC6
Print Date: October 22, 2025 2:52:00 PM

OQ2025 GC ALS GC-6 CN11461066 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 21, 2025 1:44:51 PM	Audit	SessionCreated	Session	Host Name: DESKTOP-2H6MTKJ, Drive Serial Number: 76C1E981
October 21, 2025 1:44:51 PM	start	Configuration	Session	None
October 21, 2025 1:44:51 PM	Audit	Entitlement	Licensing	Session identifier generated: XYP0-PNEJ-0W00-0RZ5-HR80
October 21, 2025 1:48:11 PM	Audit	Entitlement	Licensing	Succesfully unlocked session identified by XYP0-PNEJ-0W00-0RZ5-HR80 with unlock code 76BX-519E-XKYX-1JR1-JR60
October 21, 2025 1:57:15 PM	Audit	EqpLoaded	Session	EQP details for primary technique [Gc] - File path: [ProtocolPacks/Gc/Configurations/02.53/Gc.02.53.eqp], EQP File Name: [Gc.02.53.eqp], EQP Name: [AgilentRecommended],Protocol Revision :[Gc.02.53]
October 21, 2025 1:57:39 PM	End	Configuration	Session	None
October 21, 2025 1:57:46 PM	start	Qualification	Session	OQ
October 21, 2025 1:57:46 PM	start	Execution	CDS Logon Verification - GC - 7890: - Qualitative test	None
October 21, 2025 2:18:54 PM	End	Execution	CDS Logon Verification - GC - 7890: - Qualitative test	Run Count : 1

Page 1 / 12

Date: October 22, 2025 2:51:58 PM
System ID: BKK_EN0126_GC6

User Name: suriya.thongkaew
Report Generated by Hostname: DESKTOP-2H6MTKJ
System Id: BKK_EN0126_GC6
Print Date: October 22, 2025 2:52:00 PM

OQ2025 GC ALS GC-6 CN11461066 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 21, 2025 2:19:27 PM	start	Execution	System Inspection and Basic Safety and Operation - 7890: - Qualitative Test - No setpoints associated	None
October 21, 2025 2:19:47 PM	End	Execution	System Inspection and Basic Safety and Operation - 7890: - Qualitative Test - No setpoints associated	Run Count : 1
October 21, 2025 2:19:50 PM	start	Execution	Inlet Pressure Decay - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: >= -2.0 psi and <= 0.5 psi	None
October 21, 2025 2:25:44 PM	End	Execution	Inlet Pressure Decay - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: >= -2.0 psi and <= 0.5 psi	Run Count : 1
October 21, 2025 2:25:52 PM	start	Execution	Inlet Pressure Accuracy - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	None
October 21, 2025 2:28:43 PM	End	Execution	Inlet Pressure Accuracy - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	Run Count : 1
October 21, 2025 2:28:45 PM	start	Execution	Inlet Pressure Decay - Back SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: >= -2.0 psi and <= 0.5 psi	None
October 21, 2025 2:33:42 PM	End	Execution	Inlet Pressure Decay - Back SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: >= -2.0 psi and <= 0.5 psi	Run Count : 1
October 21, 2025 2:33:50 PM	start	Execution	Inlet Pressure Accuracy - Back SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	None

User Name: suriya.thongkaew
Report Generated by Hostname: DESKTOP-2H6MTKJ
System Id: BKK_EN0126_GC6
Print Date: October 22, 2025 2:52:00 PM

OQ2025 GC ALS GC-6 CN11461066 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 21, 2025 2:34:27 PM	End	Execution	Inlet Pressure Accuracy - Back SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	Run Count : 1
October 21, 2025 2:34:32 PM	start	Execution	Detector Flow Accuracy - Front FID: - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	None
October 21, 2025 2:50:39 PM	Audit	Data	Detector Flow Accuracy - Front FID: - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry
October 21, 2025 2:50:41 PM	start	Execution	Detector Flow Accuracy - Front FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	None
October 21, 2025 2:50:45 PM	start	Execution	Detector Flow Accuracy - Front FID: - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	None
October 21, 2025 2:50:53 PM	End	Execution	Detector Flow Accuracy - Front FID: - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	Run Count : 1
October 21, 2025 2:50:56 PM	start	Execution	Detector Flow Accuracy - Front FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	None
October 21, 2025 2:54:08 PM	Audit	Data	Detector Flow Accuracy - Front FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry
October 21, 2025 2:54:15 PM	Audit	Data	DataManager	DataManager was in a data verification state but the user chose to start over
October 21, 2025 2:54:31 PM	Audit	Data	Detector Flow Accuracy - Front FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry
October 21, 2025 2:54:34 PM	End	Execution	Detector Flow Accuracy - Front FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	Run Count : 1

User Name: suriya.thongkaew System Id: BKK_EN0126_GC6
Report Generated by Hostname: DESKTOP-2H6MTKJ Print Date: October 22, 2025 2:52:00 PM

OQ2025 GC ALS GC-6 CN11461066 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 21, 2025 2:54:48 PM	start	Execution	Detector Flow Accuracy - Front FID: - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	None
October 21, 2025 2:57:00 PM	Audit	Data	Detector Flow Accuracy - Front FID: - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry
October 21, 2025 2:57:03 PM	End	Execution	Detector Flow Accuracy - Front FID: - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	Run Count : 1
October 21, 2025 2:57:38 PM	start	Execution	Detector Flow Accuracy - Back FID: - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	None
October 21, 2025 3:00:15 PM	Audit	Data	Detector Flow Accuracy - Back FID: - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry
October 21, 2025 3:00:17 PM	End	Execution	Detector Flow Accuracy - Back FID: - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	Run Count : 1
October 21, 2025 3:00:20 PM	start	Execution	Detector Flow Accuracy - Back FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	None
October 21, 2025 3:03:03 PM	Audit	Data	Detector Flow Accuracy - Back FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry
October 21, 2025 3:03:06 PM	End	Execution	Detector Flow Accuracy - Back FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	Run Count : 1
October 21, 2025 3:03:08 PM	start	Execution	Detector Flow Accuracy - Back FID: - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	None
October 21, 2025 3:07:25 PM	Audit	Data	Detector Flow Accuracy - Back FID: - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry

User Name: suriya.thongkaew System Id: BKK_EN0126_GC6
Report Generated by Hostname: DESKTOP-2H6MTKJ Print Date: October 22, 2025 2:52:00 PM

OQ2025 GC ALS GC-6 CN11461066 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 21, 2025 3:07:28 PM	End	Execution	Detector Flow Accuracy - Back FID: - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	Run Count : 1
October 21, 2025 3:07:53 PM	start	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
October 21, 2025 3:21:20 PM	Audit	Data	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry
October 21, 2025 3:21:22 PM	End	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1
October 21, 2025 3:21:36 PM	start	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
October 21, 2025 3:30:43 PM	Audit	Data	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry
October 21, 2025 3:30:45 PM	End	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1
October 21, 2025 3:30:48 PM	start	Execution	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	None
October 21, 2025 3:50:20 PM	Audit	Data	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Manual Data Entry

User Name: suriya.thongkaew System Id: BKK_EN0126_GC6
Report Generated by Hostname: DESKTOP-2H6MTKJ Print Date: October 22, 2025 2:52:00 PM

OQ2025 GC ALS GC-6 CN11461066 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 21, 2025 3:50:24 PM	End	Execution	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Run Count : 1
October 21, 2025 3:50:31 PM	start	Execution	GC Scouting Run - Injection Tower, Front SSL, Front FID: - Part of System Preparation - No limits associated	None
October 21, 2025 3:55:30 PM	Audit	AceClosed	Session	None
October 22, 2025 10:10:41 AM	Audit	AceRestarted	Session	Host Name: DESKTOP-2H6MTKJ, Drive Serial Number: 76C1E981
October 22, 2025 10:10:42 AM	Audit	SessionReloaded	Session	None
October 22, 2025 10:10:44 AM	start	Qualification	Session	OQ
October 22, 2025 10:10:45 AM	start	Execution	GC Scouting Run - Injection Tower, Front SSL, Front FID: - Part of System Preparation - No limits associated	None
October 22, 2025 2:15:45 PM	Audit	Data	DataManager	DataManager was in a data verification state but the user chose to start over
October 22, 2025 2:16:36 PM	Audit	Data	GC Scouting Run - Injection Tower, Front SSL, Front FID: - Part of System Preparation - No limits associated	Data files Path : D:\ALS GC-6\OQ2025\SCOUTING_01.D\FID1A.ch

Type text here

User Name: suriya.thongkaew System Id: BKK_EN0126_GC6
Report Generated by Hostname: DESKTOP-2H6MTKJ Print Date: October 22, 2025 2:52:00 PM

OQ2025 GC ALS GC-6 CN11461066 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 22, 2025 2:17:00 PM	Audit	Reporting	Reintegration	Reintegration Count: 1 -- [Integration Type: Injection;Baseline Correction Mode: Advanced;Initial Slope Sensitivity: 10;Initial Peak Width: 0.01;Initial Area Reject: 0;Initial Height Reject: 100;Integration: Off at 0;Integration: On at 0.1;Integration: Off at 0.5]
October 22, 2025 2:17:42 PM	End	Execution	GC Scouting Run - Injection Tower, Front SSL, Front FID: - Part of System Preparation - No limits associated	Run Count : 1
October 22, 2025 2:17:53 PM	start	Execution	Noise and Drift - Front FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	None
October 22, 2025 2:19:13 PM	Audit	Data	Noise and Drift - Front FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	Data files Path : D:\ALS GC-6\OQ2025\OQ2025 2025-10-22 11-05-22\SIGNSDRF_F_01.D\FID1A.ch
October 22, 2025 2:19:28 PM	End	Execution	Noise and Drift - Front FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	Run Count : 1
October 22, 2025 2:19:30 PM	start	Execution	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	None

User Name: suriya.thongkaew System Id: BKK_EN0126_GC6
Report Generated by Hostname: DESKTOP-2H6MTKJ Print Date: October 22, 2025 2:52:00 PM

OQ2025 GC ALS GC-6 CN11461066 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 22, 2025 2:19:56 PM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : D:\ALS GC-6\OQ2025\OQ2025 2025-10-22 11-05-22\INJPREC_F_02.D\ FID1A.ch
October 22, 2025 2:19:56 PM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : D:\ALS GC-6\OQ2025\OQ2025 2025-10-22 11-05-22\INJPREC_F_03.D\ FID1A.ch
October 22, 2025 2:19:56 PM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : D:\ALS GC-6\OQ2025\OQ2025 2025-10-22 11-05-22\INJPREC_F_04.D\ FID1A.ch
October 22, 2025 2:19:56 PM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : D:\ALS GC-6\OQ2025\OQ2025 2025-10-22 11-05-22\INJPREC_F_05.D\ FID1A.ch
October 22, 2025 2:19:56 PM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : D:\ALS GC-6\OQ2025\OQ2025 2025-10-22 11-05-22\INJPREC_F_06.D\ FID1A.ch
October 22, 2025 2:19:56 PM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : D:\ALS GC-6\OQ2025\OQ2025 2025-10-22 11-05-22\INJPREC_F_07.D\ FID1A.ch

Date: October 22, 2025 2:51:58 PM
System ID: BKK_EN0126_GC6

© 2025 by Agilent Technologies Agilent CrossLab Compliance Services

User Name: suriya.thongkaew System Id: BKK_EN0126_GC6
Report Generated by Hostname: DESKTOP-2H6MTKJ Print Date: October 22, 2025 2:52:00 PM

OQ2025 GC ALS GC-6 CN11461066 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 22, 2025 2:20:04 PM	Audit	Reporting	Reintegration	Reintegration Count: 1 – [Integration Type: Injection;Baseline Correction Mode: Advanced;Initial Slope Sensitivity: 10;Initial Peak Width: 0.01;Initial Area Reject: 0;Initial Height Reject: 100;Integration: Off at 0;Integration: On at 0.1;Integration: Off at 0.5]
October 22, 2025 2:20:24 PM	End	Execution	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Run Count : 1
October 22, 2025 2:20:34 PM	start	Execution	Signal to Noise - Injection Tower, Front SSL, Front FID: - Detector FID - L: >= 300000	None
October 22, 2025 2:20:58 PM	Audit	Data	Signal to Noise - Injection Tower, Front SSL, Front FID: - Detector FID - L: >= 300000	Data files Path : D:\ALS GC-6\OQ2025\OQ2025 2025-10-22 11-05-22\SIGTONS_F_01.D\ FID1A.ch
October 22, 2025 2:21:06 PM	Audit	Reporting	Reintegration	Reintegration Count: 1 – [Integration Type: Injection;Baseline Correction Mode: Advanced;Initial Slope Sensitivity: 10;Initial Peak Width: 0.01;Initial Area Reject: 0;Initial Height Reject: 100;Integration: Off at 0;Integration: On at 0.1;Integration: Off at 0.5]
October 22, 2025 2:21:19 PM	End	Execution	Signal to Noise - Injection Tower, Front SSL, Front FID: - Detector FID - L: >= 300000	Run Count : 1

Date: October 22, 2025 2:51:58 PM
System ID: BKK_EN0126_GC6

User Name: suriya.thongkaew System Id: BKK_EN0126_GC6
Report Generated by Hostname: DESKTOP-2H6MTKJ Print Date: October 22, 2025 2:52:00 PM

OQ2025 GC ALS GC-6 CN11461066 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 22, 2025 2:21:25 PM	start	Execution	GC Scouting Run - Injection Tower, Back SSL, Back FID: - Part of System Preparation - No limits associated	None
October 22, 2025 2:25:23 PM	Audit	Data	GC Scouting Run - Injection Tower, Back SSL, Back FID: - Part of System Preparation - No limits associated	Data files Path : D:\ALS GC-6\OQ2025_B\SCOUTING_B_01.D\FID2B.ch
October 22, 2025 2:26:18 PM	End	Execution	GC Scouting Run - Injection Tower, Back SSL, Back FID: - Part of System Preparation - No limits associated	Run Count : 1
October 22, 2025 2:26:21 PM	start	Execution	Noise and Drift - Back FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	None
October 22, 2025 2:27:00 PM	Audit	Data	Noise and Drift - Back FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	Data files Path : D:\ALS GC-6\OQ2025_B\OQ2025 2025-10-22 11-05-22\SIGNSDRF_B_01.D\FID2B.ch
October 22, 2025 2:27:42 PM	End	Execution	Noise and Drift - Back FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	Run Count : 1
October 22, 2025 2:27:46 PM	start	Execution	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	None
October 22, 2025 2:28:07 PM	Audit	Data	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : D:\ALS GC-6\OQ2025_B\OQ2025 2025-10-22 11-05-22\INJPREC_B_02.D\FID2B.ch

© 2025 by Agilent Technologies Agilent CrossLab Compliance Services

User Name: suriya.thongkaew System Id: BKK_EN0126_GC6
Report Generated by Hostname: DESKTOP-2H6MTKJ Print Date: October 22, 2025 2:52:00 PM

OQ2025 GC ALS GC-6 CN11461066 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 22, 2025 2:28:07 PM	Audit	Data	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : D:\ALS GC-6\OQ2025_B\OQ2025 2025-10-22 11-05-22\INJPREC_B_03.D\FID2B.ch
October 22, 2025 2:28:07 PM	Audit	Data	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : D:\ALS GC-6\OQ2025_B\OQ2025 2025-10-22 11-05-22\INJPREC_B_04.D\FID2B.ch
October 22, 2025 2:28:07 PM	Audit	Data	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : D:\ALS GC-6\OQ2025_B\OQ2025 2025-10-22 11-05-22\INJPREC_B_05.D\FID2B.ch
October 22, 2025 2:28:07 PM	Audit	Data	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : D:\ALS GC-6\OQ2025_B\OQ2025 2025-10-22 11-05-22\INJPREC_B_06.D\FID2B.ch
October 22, 2025 2:28:07 PM	Audit	Data	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : D:\ALS GC-6\OQ2025_B\OQ2025 2025-10-22 11-05-22\INJPREC_B_07.D\FID2B.ch
October 22, 2025 2:28:21 PM	End	Execution	Injection Precision - Injection Tower, Back SSL, Back FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Run Count : 1
October 22, 2025 2:28:28 PM	start	Execution	Signal to Noise - Injection Tower, Back SSL, Back FID: - Detector FID - L: >= 300000	None

User Name: suriya.thongkaew
Report Generated by Hostname: DESKTOP-2H6MTKJ

System Id: BKK_EN0126_GC6
Print Date: October 22, 2025 2:52:00 PM

OQ2025 GC ALS GC-6 CN11461066 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
October 22, 2025 2:28:47 PM	Audit	Data	Signal to Noise - Injection Tower, Back SSL, Back FID: - Detector FID - L: >= 300000	Data files Path : D:\ALS GC-6\OQ2025_B\OQ2025 2025-10-22 11-05-22\SIGTONS_B_01.D\ FID2B.ch
October 22, 2025 2:29:53 PM	End	Execution	Signal to Noise - Injection Tower, Back SSL, Back FID: - Detector FID - L: >= 300000	Run Count : 1
October 22, 2025 2:30:01 PM	End	Qualification	Session	OQ
October 22, 2025 2:30:01 PM	start	Reporting	Session	None
October 22, 2025 2:50:41 PM	Audit	Reporting	Session	Report Generated : Certificate
October 22, 2025 2:51:22 PM	Audit	Reporting	Session	Report Generated : Report

Page 12 / 12

Date: October 22, 2025 2:51:58 PM
System ID: BKK_EN0126_GC6

JNAC
JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Air speed measurement laboratory
Calibration services department.

NSC – TISI – TIS 17025
CALIBRATION 0367

Certificate Number
CWS-005-68

CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

MEASUREMENT ITEM : Cup anemometer
MANUFACTURER : Novalynx
MODEL/TYPE : Sensor: WS-02F
Data logger: 110-WS-25DL-D
SERIAL NUMBER : Sensor: WSD-A5978
Data logger: A5978
ID NUMBER : RYG_FS0648
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250 Thailand.

RECEIVED DATE : 10 Jan 2025
MEASUREMENT DATE : 16 Jan 2025
ISSUE DATE : 20 Jan 2025

ENVIRONMENTAL CONDITIONS:
Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010± 10	hPa

PLACE OF CALIBRATION : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITIONS

: Wind tunnel cross-section area[1]	900	cm^2
Wind direction frontal area[2]	100	cm^2
Diameter of mounting pipe[3]	-	mm
Blockage ratio of test object[4]	0.111	[-]

Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are (24.3) °C, (61.9) %RH and (1011.9) hPa.

TABULATION OF RESULTS:
The table on next page give the measured values.

Calibration procedure:
The Cup anemometer was calibrated against Standard air velocity transducer model: 8455-12 and pitot tube with precision differential pressure meter model: DPM2500 in an close test-section of Eiffel-type wind tunnel with 900 cm^2 cross test section area. The WI-CL-007 based on IEC 61400-12-1, Wind energy generation systems – Part 12-1: Power performance measurements of electricity producing wind turbines, March 2017 was used as a calibration guideline.

Traceability:
This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MW-0007-24 and MW-0065-24

Uncertainty of Measurement:
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Calibrated by:
☑ Mr. Sorawit Thachalad
☐ Miss Jittraporn Lertsomphol

JNAC JIRANATEE ASSOCIATES CO.,LTD.

Approved signatory: .....
Mr. Parinya Booncharoen
Calibration Department Manager

REVIEW BY .....
APPROVED BY .....
NEXT CAL DATE 15/ 07/ 26

Remark:
[1] Nozzle cross-section area of the wind tunnel
[2] Projected cross-section area of the tested object include mounting pipe
[3] Diameter of mounting pipe
[4] Ratio [2] to [1]

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

Jiranatee Associates Co.,Ltd.

Certificate Number
CWS-005-68

MEASUREMENT RESULTS [5]

The Cup anemometer, Unit Under Calibration (UUC) was exercise at 10 m/s for 5 minutes prior to calibration being performed. The standard air velocity 0.5 m/s to 5 m/s was calculated by a standard air velocity transducer which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section and the standard air velocity 5 m/s to 30 m/s was calculated by a pitot tube with precision differential pressure meter which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section, UUC was mounted on a round vertical tube of the lower plate at center of test section. The calibration was carried out under both rising and falling air velocity in the range of 1 m/s to 16 m/s at calibration interval of 1 m/s. The results of calibration and associated measurement uncertainties are reported in the table below.

V_{std} [6] (m/s)	Temp. wind tunnel (°C)	Temp. room (°C)	V_{UUC} [7] (m/s)	Error (m/s)	*U (k=2)* (m/s)
0.998	24.10	24.25	0.9	-0.1	0.31
2.242	24.14	24.25	2.0	-0.2	0.31
3.112	24.14	24.25	3.0	-0.1	0.31
4.235	24.12	24.25	4.0	-0.2	0.31
4.94	24.12	24.25	5.0	0.1	0.31
5.98	24.30	24.25	6.0	0.0	0.31
7.03	24.10	24.25	7.2	0.1	0.31
7.97	24.22	24.25	8.2	0.2	0.31
9.03	24.10	24.25	9.3	0.2	0.31
9.95	24.10	24.25	10.2	0.2	0.31
11.02	24.16	24.25	11.2	0.2	0.31
11.99	24.26	24.25	12.3	0.3	0.31
13.04	24.32	24.25	13.4	0.4	0.31
13.98	24.12	24.25	14.4	0.4	0.31
15.01	24.26	24.25	15.4	0.4	0.31
15.97	24.10	24.25	16.4	0.4	0.31


Remark:

[5] Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

[6] Velocity of standard

[7] Velocity of Unit Under Calibration

PHOTO OF CALIBRATION SET-UP



Calibration set-up of the Cup anemometer calibration in the wind tunnel of Jiranatee Associates Co., Ltd. The Cup anemometer shown may differ from the calibrated one. Remark: The proportion of the set- up is not true to scale due to imaging geometry.

End of Certificate of Calibration

JNAC JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Wind direction measurement laboratory
Calibration services department.

ilac-MRA NSC THAILAND
NSC – TISI – TIS 17025
CALIBRATION 0367

Certificate Number
CWD-005-68

CERTIFICATE OF CALIBRATION

MEASUREMENT ITEM : Wind Direction Sensor
MANUFACTURER : Novalynx
MODEL/TYPE : Sensor: WS-02F
Data logger: 110-WS-25DL-D
SERIAL NUMBER : Sensor: WSD-A5978
Data logger: A5978
ID NUMBER : RYG_FS0648
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250 Thailand.

RECEIVED DATE : 10 Jan 2025
MEASUREMENT DATE : 16 Jan 2025
ISSUE DATE : 20 Jan 2025

ENVIRONMENTAL CONDITIONS:
Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa

PLACE OF CALIBRATION : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITION

: Wind tunnel cross-section area[1]	900	cm^2
Wind direction frontal area[2]	129	cm^2
Diameter of mounting pipe[3]	-	mm
Blockage ratio of test object[4]	0.143	[-]

Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are (24.4)°C, (62.9) %RH and (1013.5) hPa.

TABULATION OF RESULTS:
The table on next page give the measured values.

Calibration procedure:
The wind direction sensor was calibrated against Standard Rotary Encoder model: AX4009TS-DM04-P3-S-U0 in an close test-section of Eiffel-type wind tunnel with 900 cm^2 cross test section area. The WI-CL-008 based on IEC 61400-12-1, Wind energy generation systems – Part 12-1: Power performance measurements of electricity producing wind turbines, March 2017 was used as a calibration guideline.

Traceability:
This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: DA-0027-24.

Uncertainty of Measurement:
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Calibrated by:
☑ Mr. Sorawit Thachalad
☐ Miss Jittraporn Lertsomphol

JNAC JIRANATEE ASSOCIATES CO.,LTD.

Approved signatory: .....
Mr. Parinya Booncharoen
Calibration Department Manager

Remark:
[1] Nozzle cross-section area of the wind tunnel
[2] Projected cross-section area of the tested object include mounting pipe
[3] Diameter of mounting pipe
[4] Ratio [2] to [1]

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

Jiranatee Associates Co., Ltd.

Certificate Number
CWD-005-68

MEASUREMENT RESULTS [5]

The wind direction sensor was calibrated against standard rotary encoder by comparison method. During calibration, the measurement was carried out at 45° intervals in clockwise and counterclockwise directions after offset adjustment has been made. The flow speed of wind tunnel (usually 5 m/s) is kept constant while the sensor is rotated around its vertical axis. The results of calibration and associated measurement uncertainties are reported in the table below.

Air speed	D'_{std}	D'_{uuc}	Error	*U (k=2)*
m/s	Degree (°)	Degree (°)	Degree (°)	Degree (°)
5.01	45.000	42	-3	0.80
	90.000	88	-2	0.80
	135.000	135	0	0.80
	180.000	182	2	0.80
	225.000	228	3	0.80
	270.000	273	3	0.80
	315.000	318	3	0.80
	360.000	359	-1	0.80

Remark:

[5] Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

[6] Direction of standard

[7] Direction of Unit Under Calibration

End of Certificate of Calibration

Jiranatee Associates Co., Ltd.

JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Temperature measurement laboratory
Calibration services department.

NSC – TISI – TIS 17025
CALIBRATION 0367

CERTIFICATE OF CALIBRATION

Certificate No. : CDT-029-68

MEASUREMENT ITEM : Data Logger with Temperature sensor
MANUFACTURER : Novalynx
MODEL/TYPE : 110-WS-25DL-D
SERIAL NUMBER : A5978
ID NUMBER : RYG_FS0648
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Suan Luang, Khet Suan Luang,
Bangkok 10250 Thailand.

RECEIVED DATE : 10 Jan 2025
MEASUREMENT DATE : 16 Jan 2025
ISSUE DATE : 20 Jan 2025

ENVIRONMENTAL CONDITIONS:
Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH

NOTED: *The certificate is valid only to the item calibrated on date and place of calibration.*

TABULATION OF RESULTS:
The table on next page give the measured values.

Calibration procedure:
The temperature calibration was done by In-House calibration method as WI-CL-001 according to comparison method with standard digital temperature indicator and standard temperature probe. The temperature scale use was based on ITS-90.

Traceability:
The measurement results are traceable to the international system of units (SI) through National Institute of Metrology Thailand (NIMT) Certificate number: TT-0047-24, Certificate number: ER-0113-24

Reference Used During Calibration:
1. Standard Temperature Probe
Model: STS-100 A500, Serial No.: 667682-09, Due date: 26 Mar 2025
2. Digital Temperature Indicator
Model: DTI-1000-A MK II, Serial No.: 671407-00591 Due date: 21 Oct 2025

Uncertainty of Measurement:
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Calibrated by:
☐ Mr. Sorawit Thachalad
☑ Miss Jittraporn Lertsomphol
☐ Miss Ruangrumpai Phoommit

Approved signatory: .....
Mr. Parinya Booncharoen
Calibration Department Manager

Jiranatee Associates Co., Ltd.

THIS CERTIFICATE MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

JIRANATEE ASSOCIATES CO.,LTD.

Continuation of Certificate of Calibration Number CDT-029-68

Result of Calibration: ☑ Without Adjustment ☐ With Adjustment

Calibration Range: 20 ˚C to 40 ˚C

Function:

Table 1: This equipment was connected with temperature sensor Model: HMP60 S/N: V1920213. Dimension: Diameter 12 mm. Length 80 mm.

Immersion Depth (mm)	Standard Reading (˚C)	UUC Reading (˚C)	Error (˚C)	Uncertainty (˚C)
80	20.077	19.6	-0.5	0.099
80	25.066	24.6	-0.5	0.099
80	30.054	29.6	-0.5	0.099
80	35.035	34.5	-0.5	0.099
80	40.018	39.5	-0.5	0.099

UUC*: Unit Under Calibration

End of Certificate of Calibration

JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd.

JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

NSC – TISI – TIS 17025
CALIBRATION 0367

Relative humidity and Air Temperature measurement laboratory
Calibration services department.

CERTIFICATE OF CALIBRATION

Certificate No. : CRT-003-68

MEASUREMENT ITEM : Relative humidity with data logger
MANUFACTURER : Novalynx
MODEL/TYPE : Data Logger: 110-WS-25DL-D
Sensor: HMP60
SERIAL NUMBER : Data Logger: A5978
Sensor: V1920213
ID NUMBER : RYG_FS0648
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250 Thailand.

RECEIVED DATE : 10 Jan 2025
MEASUREMENT DATE : 16 Jan 2025
ISSUE DATE : 20 Jan 2025

ENVIRONMENTAL CONDITIONS:
Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	˚C
Relative Humidity	: 55.0 ± 15.0	%RH

NOTED: *The certificate is valid only to the item calibrated on date and place of calibration.*

TABULATION OF RESULTS:
The table on next page give the measured values.

Calibration procedure:
The Relative humidity and Air Temperature calibration was done by In-House calibration method as WI-CL-009 and WI-CL-010 according to comparison method with Standard Chilled Mirror hygrometer with Temperature sensor and standard Humidity generator chamber.

Traceability:
The measurements are traceable to the international system of units (SI) through National Institute of Metrology Thailand (NIMT). Certificate number: TH-0146-24 and Jiranatee Associates Co., Ltd. Certificate number: CDT-026-68.

Uncertainty of Measurement:
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Calibrated by:
☐ Mr. Sorawit Thachalad
☑ Miss Jittraporn Lertsomphol
☐ Miss Ruangrumpai Phoommit

JIRANATEE ASSOCIATES CO.,LTD.

Approved signatory: .....
Mr. Parinya Booncharoen
Calibration Department Manager

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

JIRANATEE ASSOCIATES CO.,LTD.

Continuation of Certificate of Calibration Number: CRT-003-68

Measurement Results:

The results of calibration and associated measurement uncertainties are reported in the table below.

Result of Calibration: ☑ Without Adjustment ☐ With Adjustment

Table 1: The results of calibration of relative humidity at 30 °C are reported in table below.
Calibration Range: 20%RH to 80%RH

Air Temperature (°C)	Standard Reading (%RH)	UUC Reading (%RH)	Error (%RH)	Uncertainty ±(%RH)
29.71	19.86	18.5	-1.4	0.78
29.75	51.21	49.0	-2.2	1.3
29.75	82.84	80.0	-2.9	2.1

UUC*: Unit Under Calibration

End of Certificate of Calibration

Jiranatee Associates Co.,Ltd.

JIRANATEE ASSOCIATES CO.,LTD.
Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600(Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Pressure measurement laboratory
Calibration services department.

NSC - TISI - TIS 17025
CALIBRATION 0367

CERTIFICATE OF CALIBRATION

Certificate No. : CPR-003-68

MEASUREMENT ITEM : Digital barometer
MANUFACTURER : Novalynx
MODEL/TYPE : Sensor: 110-WS-25BP
Data logger: 110-WS-25DL-D
SERIAL NUMBER : Sensor: BP-A5978
Data logger: A5978
ID NUMBER : RYG_FS0648
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd,
Khwaeng Suan Luang, Khet Suan Luang,
Bangkok 10250 Thailand.

RECEIVED DATE : 10 Jan 2025
MEASUREMENT DATE : 16 Jan 2025
ISSUE DATE : 20 Jan 2025

Calibration procedure:
The Digital barometer was calibrated against Digital pressure calibrator. The WI-CL-003 was used as a calibration guideline.

Traceability:
The measurement results are traceable to the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MP-0009-24

Reference Used During Calibration:
1. Absolute Pressure Transducer
Model: CPG2500, Serial No.: 4100126P

Uncertainty of Measurement:
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

CONDITION OF THIS RESULT OF CALIBRATION:

1. Calibration effort for calibration sequence C
2. The UUC* was installed in vertical orientation above reference standard instrument and center of UUC* was used as the reference level.
3. Calibration conditions:
4. Condition : ☑ Normal ☐ Abnormal
   Pressure transmitting medium : Air
   ρ_{FI} (20°C, 1 bar) : 1.19 kg/m^3
   H_{amb} : (55.3±2.3) %
   t_{amb} : (23.1±0.3) °C
   p_{amb} : (1013.2±0.7) mbar
5. The certificate is valid only to the item calibrated on date and place of calibration

Calibrated by:
☑ Mr. Sorawit Thachalad
☐ Miss Jittraporn Lertsomphol

JIRANATEE ASSOCIATES CO.,LTD.

Approved signatory: .....
Mr. Parinya Booncharoen
Calibration Department Manager

THIS CERTIFICATE REPORT MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

JIRANATEE ASSOCIATES CO.,LTD.
Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Pressure measurement laboratory
Calibration services department.

NSC - TISI - TIS 17025
CALIBRATION 0367

CERTIFICATE OF CALIBRATION

Certificate No. : CPR-003-68

MEASUREMENT RESULTS : ☐ Without adjustment ☑ With adjustment

CALIBRATION IN THE RANGE OF : 950 mbar to 1050 mbar

The results of calibration and associated measurement uncertainties are reported in the table below.

STD (mbar)	UUC* (mbar)	Error (mbar)	Uncertainty (k=2) (mbar)
950.13	951.7	1.6	0.38
970.13	971.1	1.0	0.37
990.09	990.6	0.5	0.37
1010.05	1010.0	0.0	0.37
1029.99	1029.5	-0.5	0.38
1050.07	1049.0	-1.1	0.37

Note: UUC* Unit Under Calibration
: To convert the result in report unit to Pa should be multiply by 100

End of certificate

JNAC JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co., Ltd.

ALS Laboratory Group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Phatthanakan, Suan Luang, Bangkok 10250
T +66 2 760 3000 F +66 2 760 3197

Certificate of Calibration

Certificate No. C-020126-RYG_FS0672

Air Sampling Pump Detail

Equipment name	: Personal Air Sampling Pump	Equiment ID	: RYG_FS0672
Brand	: Gilian	Serial No.	: 20230810008
Model/Type	: GilAir Plus	Calibration Date	: 02-Jan-26
		Next calibration date	: 02-Apr-26

Reference Standard Low Flow Meter

Equipment name	: Air Flow Meter	Equiment ID	: BKK_FS0619
Brand	: MesaLabs	Serial No.	: 130026
Model/Type	: Defender 510-L	Calibration Date	: 10-Sep-25
		Due Date	: 9-Sep-26

Reference Standard High Flow Meter

Equipment name	: Air Flow Meter	Equiment ID	: BKK_FS0614
Brand	: MesaLabs	Serial No.	: 151114
Model/Type	: Defender 510-M	Calibration Date	: 10-Sep-25
		Due Date	: 09-Sep-26

Calibration Data

Air Sampling Pump setting (cc/min)	Reference Std. Flow Reading (cc/min)			Avg. (cc/min)	%Error acceptance	Acceptable range (cc/min)	Evaluation (Pass/ Fail)
	1	2	3				
Low Flow							
20	20.3	20.4	20.5	20.4	5%	19 - 21	Passed
50	50.6	51.2	51.7	51.2	5%	48 - 53	Passed
100	101.8	100.6	101.0	101.1	5%	95 - 105	Passed
200	201.6	199.9	198.9	200.1	5%	190 - 210	Passed
High Flow							
500	505.9	503.5	504.7	504.7	3%	485 - 515	Passed
1000	999.6	1000.2	997.4	999.1	3%	970 - 1030	Passed
2000	2003.0	2000.8	2005.9	2003.2	3%	1940 - 2060	Passed
2500	2514.5	2518.6	2514.7	2515.9	3%	2425 - 2575	Passed

---------- END OF REPORT ----------

Calibrated By: ณัชพล
(Mr. Natchapon Thamklang)
RYG Field Services Scientist (1)

Approved By: Supot S
(Mr. Supot Salamteh)
Field Services Section Head

Issue date : 03-Jan-26

ALS Laboratory Group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Phatthanakan, Suan Luang, Bangkok 10250
T +66 2 760 3000 F +66 2 760 3197

Certificate of Calibration

Certificate No. C-060126-RYG_FS0126

Air Sampling Pump Detail

Equipment name	: Personal Air Sampling Pump	Equiment ID	: RYG_FS0126
Brand	: Gilian	Serial No.	: 20150410002
Model/Type	: GilAir Plus	Calibration Date	: 06-Jan-26
		Next calibration date	: 06-Apr-26

Reference Standard Low Flow Meter

Equipment name	: Air Flow Meter	Equiment ID	: BKK_FS0619
Brand	: MesaLabs	Serial No.	: 130026
Model/Type	: Defender 510-L	Calibration Date	: 10-Sep-25
		Due Date	: 09-Sep-26

Reference Standard High Flow Meter

Equipment name	: Air Flow Meter	Equiment ID	: BKK_FS0614
Brand	: MesaLabs	Serial No.	: 151114
Model/Type	: Defender 510-M	Calibration Date	: 10-Sep-25
		Due Date	: 09-Sep-26

Calibration Data

Air Sampling Pump setting (cc/min)	Reference Std. Flow Reading (cc/min)			Avg. (cc/min)	%Error acceptance	Acceptable range (cc/min)	Evaluation (Pass/ Fail)
	1	2	3				
Low Flow							
20	19.9	20.2	20.4	20.2	5%	19 - 21	Passed
50	50.8	51.0	52.1	51.3	5%	48 - 53	Passed
100	99.4	99.1	99.8	99.4	5%	95 - 105	Passed
200	201.2	204.4	200.5	202.0	5%	190 - 210	Passed
High Flow							
500	501.2	501.5	500.0	500.9	3%	485 - 515	Passed
1000	1005.9	1004.5	1002.8	1004.4	3%	970 - 1030	Passed
2000	2001.4	2001.1	2004.3	2002.3	3%	1940 - 2060	Passed
2500	2501.5	2500.0	2499.2	2500.2	3%	2425 - 2575	Passed
4000	4002.9	3997.5	4002.3	4000.9	3%	3880 - 4120	Passed

---------- END OF REPORT ----------

Calibrated By: .....
(Mr. Natchapon Thamklang)
RYG Field Services Scientist (1)

Approved By: .....
(Mr. Supot Salamteh)
Field Services Section Head

Issue date : 07-Jan-26

ALS Laboratory Group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Phatthanakan, Suan Luang, Bangkok 10250
T +66 2 760 3000 F +66 2 760 3197

Certificate of Calibration

Certificate No. C-070126-RYG_FS0513

Air Sampling Pump Detail

Equipment name	: Personal Air Sampling Pump	Equiment ID	: RYG_FS0513
Brand	: Gilian	Serial No.	: 20201110093
Model/Type	: GilAir Plus	Calibration Date	: 07-Jan-26
		Next calibration date	: 07-Apr-26

Reference Standard Low Flow Meter

Equipment name	: Air Flow Meter	Equiment ID	: BKK_FS0619
Brand	: MesaLabs	Serial No.	: 130026
Model/Type	: Defender 510-L	Calibration Date	: 10-Sep-25
		Due Date	: 9-Sep-26

Reference Standard High Flow Meter

Equipment name	: Air Flow Meter	Equiment ID	: BKK_FS0614
Brand	: MesaLabs	Serial No.	: 151114
Model/Type	: Defender 510-M	Calibration Date	: 10-Sep-25
		Due Date	: 09-Sep-26

Calibration Data

Air Sampling Pump setting (cc/min)	Reference Std. Flow Reading (cc/min)			Avg. (cc/min)	%Error acceptance	Acceptable range (cc/min)	Evaluation (Pass/ Fail)
	1	2	3				
Low Flow							
20	20.3	20.4	20.7	20.5	5%	19 - 21	Passed
50	50.4	49.2	50.4	50.0	5%	48 - 53	Passed
100	100.1	100.0	99.4	99.8	5%	95 - 105	Passed
200	200.9	200.2	199.8	200.3	5%	190 - 210	Passed
High Flow							
500	499.4	500.5	502.9	500.9	3%	485 - 515	Passed
1000	999.7	998.0	996.4	998.0	3%	970 - 1030	Passed
2000	1999.1	2001.2	1998.8	1999.7	3%	1940 - 2060	Passed
2500	2509.9	2504.7	2504.0	2506.2	3%	2425 - 2575	Passed

---------- END OF REPORT ----------

Calibrated By: .....
(Mr. Watcharin Pongsamsuan)
RYG Field Services Scientist (1)

Approved By: .....
(Mr. Supot Salamteh)
Field Services Section Head

Issue date : 08-Jan-26

ALS Laboratory Group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Phatthanakan, Suan Luang, Bangkok 10250
T +66 2 760 3000 F +66 2 760 3197

Certificate of Calibration

Certificate No. C-070126-RYG_FS0511

Air Sampling Pump Detail

Equipment name	: Personal Air Sampling Pump	Equiment ID	: RYG_FS0511
Brand	: Gilian	Serial No.	: 20201110095
Model/Type	: GilAir Plus	Calibration Date	: 07-Jan-26
		Next calibration date	: 07-Apr-26

Reference Standard Low Flow Meter

Equipment name	: Air Flow Meter	Equiment ID	: BKK_FS0619
Brand	: MesaLabs	Serial No.	: 130026
Model/Type	: Defender 510-L	Calibration Date	: 10-Sep-25
		Due Date	: 9-Sep-26

Reference Standard High Flow Meter

Equipment name	: Air Flow Meter	Equiment ID	: BKK_FS0614
Brand	: MesaLabs	Serial No.	: 151114
Model/Type	: Defender 510-M	Calibration Date	: 10-Sep-25
		Due Date	: 09-Sep-26

Calibration Data

Air Sampling Pump setting (cc/min)	Reference Std. Flow Reading (cc/min)			Avg. (cc/min)	%Error acceptance	Acceptable range (cc/min)			Evaluation (Pass/ Fail)
	1	2	3						
Low Flow									
20	20.8	20.7	20.9	20.8	5%	19	-	21	Passed
50	50.3	51.2	51.0	50.8	5%	48	-	53	Passed
100	100.7	100.2	99.6	100.2	5%	95	-	105	Passed
200	201.3	201.4	199.6	200.8	5%	190	-	210	Passed
High Flow									
500	503.6	502.4	502.6	502.9	3%	485	-	515	Passed
1000	998.3	1001.8	1002.6	1000.9	3%	970	-	1030	Passed
2000	2004.2	2002.3	1999.5	2002.0	3%	1940	-	2060	Passed
2500	2501.7	2504.3	2503.7	2503.2	3%	2425	-	2575	Passed

---------- END OF REPORT ----------

Calibrated By: _____
(Mr. Watcharin Pongsamsuan)
RYG Field Services Scientist (1)

Approved By: _____
(Mr. Supot Salamteh)
Field Services Section Head

Issue date : 08-Jan-26

ALS Laboratory Group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Phatthanakan, Suan Luang, Bangkok 10250
T +66 2 760 3000 F +66 2 760 3197

Certificate of Calibration

Certificate No. C-070426-RYG_FS0127

Air Sampling Pump Detail

Equipment name	: Personal Air Sampling Pump	Equiment ID	: RYG_FS0127
Brand	: Gilian	Serial No.	: 20150410003
Model/Type	: GilAir Plus	Calibration Date	: 07-Apr-26
		Next calibration date	: 07-Jul-26

Reference Standard Low Flow Meter

Equipment name	: Air Flow Meter	Equiment ID	: BKK_FS0619
Brand	: MesaLabs	Serial No.	: 130026
Model/Type	: Defender 510-L	Calibration Date	: 10-Sep-25
		Due Date	: 09-Sep-26

Reference Standard High Flow Meter

Equipment name	: Air Flow Meter	Equiment ID	: BKK_FS0614
Brand	: MesaLabs	Serial No.	: 151114
Model/Type	: Defender 510-M	Calibration Date	: 10-Sep-25
		Due Date	: 09-Sep-26

Calibration Data

Air Sampling Pump setting (cc/min)	Reference Std. Flow Reading (cc/min)			Avg. (cc/min)	%Error acceptance	Acceptable range (cc/min)			Evaluation (Pass/ Fail)
	1	2	3						
Low Flow									
20	19.9	19.7	19.7	19.8	5%	19	-	21	Passed
50	50.9	51.6	51.8	51.4	5%	48	-	53	Passed
100	99.2	99.1	99.1	99.1	5%	95	-	105	Passed
200	200.2	199.9	198.0	199.4	5%	190	-	210	Passed
High Flow									
500	504.2	502.9	503.1	503.4	3%	485	-	515	Passed
1000	1001.3	1008.6	1009.1	1006.3	3%	970	-	1030	Passed
2000	2005.9	2002.1	2004.7	2004.2	3%	1940	-	2060	Passed
2500	2504.4	2508.5	2504.0	2505.6	3%	2425	-	2575	Passed

---------- END OF REPORT ----------

Calibrated By: _____
(Mr. Nantawat Sarin)
RYG Field Services Scientist (1)

Approved By: _____
(Mr. Supot Salamteh)
Field Services Section Head

Issue date : 08-Apr-26

ALS Laboratory Group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Phatthanakan, Suan Luang, Bangkok 10250
T +66 2 760 3000 F +66 2 760 3197

Certificate of Calibration

Certificate No. C-070426-RYG_FS0158

Air Sampling Pump Detail

Equipment name	: Personal Air Sampling Pump	Equiment ID	: RYG_FS0158
Brand	: Gilian	Serial No.	: 20150910030
Model/Type	: GilAir Plus	Calibration Date	: 07-Apr-26
		Next calibration date	: 07-Jul-26

Reference Standard Low Flow Meter

Equipment name	: Air Flow Meter	Equiment ID	: BKK_FS0619
Brand	: MesaLabs	Serial No.	: 130026
Model/Type	: Defender 510-L	Calibration Date	: 10-Sep-25
		Due Date	: 09-Sep-26

Reference Standard High Flow Meter

Equipment name	: Air Flow Meter	Equiment ID	: BKK_FS0614
Brand	: MesaLabs	Serial No.	: 151114
Model/Type	: Defender 510-M	Calibration Date	: 10-Sep-25
		Due Date	: 09-Sep-26

Calibration Data

Air Sampling Pump setting (cc/min)	Reference Std. Flow Reading (cc/min)			Avg. (cc/min)	%Error acceptance	Acceptable range (cc/min)	Evaluation (Pass/ Fail)
	1	2	3				
Low Flow							
20	20.7	20.3	20.7	20.6	5%	19 - 21	Passed
50	51.0	51.0	51.3	51.1	5%	48 - 53	Passed
100	100.8	100.6	99.8	100.4	5%	95 - 105	Passed
200	200.6	200.8	200.9	200.8	5%	190 - 210	Passed
High Flow							
500	501.1	501.5	501.3	501.3	3%	485 - 515	Passed
1000	1002.9	1005.7	1004.3	1004.3	3%	970 - 1030	Passed
2000	2003.8	2006.9	2003.6	2004.8	3%	1940 - 2060	Passed
2500	2501.6	2498.5	2505.1	2501.7	3%	2425 - 2575	Passed

---------- END OF REPORT ----------

Calibrated By: ณัชชพล

(Mr. Natchapon Thamklang)
RYG Field Services Scientist (1)

Approved By: Supot S

(Mr. Supot Salamteh)
Field Services Section Head

Issue date : 08-Apr-26

ALS Laboratory Group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Phatthanakan, Suan Luang, Bangkok 10250
T +66 2 760 3000 F +66 2 760 3197

Certificate of Calibration

Certificate No. C-070426-RYG_FS0367

Air Sampling Pump Detail

Equipment name	: Personal Air Sampling Pump	Equiment ID	: RYG_FS0367
Brand	: Gilian	Serial No.	: 20180610060
Model/Type	: GilAir Plus	Calibration Date	: 07-Apr-26
		Next calibration date	: 07-Jul-26

Reference Standard Low Flow Meter

Equipment name	: Air Flow Meter	Equiment ID	: BKK_FS0619
Brand	: MesaLabs	Serial No.	: 130026
Model/Type	: Defender 510-L	Calibration Date	: 10-Sep-25
		Due Date	: 09-Sep-26

Reference Standard High Flow Meter

Equipment name	: Air Flow Meter	Equiment ID	: BKK_FS0614
Brand	: MesaLabs	Serial No.	: 151114
Model/Type	: Defender 510-M	Calibration Date	: 10-Sep-25
		Due Date	: 09-Sep-26

Calibration Data

Air Sampling Pump setting (cc/min)	Reference Std. Flow Reading (cc/min)			Avg. (cc/min)	%Error acceptance	Acceptable range (cc/min)	Evaluation (Pass/ Fail)
	1	2	3				
Low Flow							
20	20.8	19.9	20.8	20.5	5%	19 - 21	Passed
50	51.9	50.2	48.6	50.2	5%	48 - 53	Passed
100	100.5	100.4	100.4	100.4	5%	95 - 105	Passed
200	202.6	201.2	200.0	201.3	5%	190 - 210	Passed
High Flow							
500	495.5	493.6	497.0	495.4	3%	485 - 515	Passed
1000	1008.0	997.4	1005.5	1003.6	3%	970 - 1030	Passed
2000	1995.3	1991.3	1997.3	1994.6	3%	1940 - 2060	Passed
2500	2492.3	2498.0	2493.5	2494.6	3%	2425 - 2575	Passed

---------- END OF REPORT ----------

Calibrated By: นันทวัฒน์

(Mr. Nantawat Sarin)
RYG Field Services Scientist (1)

Approved By: Supot S

(Mr. Supot Salamteh)
Field Services Section Head

Issue date : 08-Apr-26

ALS Laboratory Group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Phatthanakan, Suan Luang, Bangkok 10250
T +66 2 760 3000 F +66 2 760 3197

Certificate of Calibration

Certificate No. C-070426-RYG_FS0517

Air Sampling Pump Detail

Equipment name	: Personal Air Sampling Pump	Equiment ID	: RYG_FS0517
Brand	: Gilian	Serial No.	: 20201110090
Model/Type	: GilAir Plus	Calibration Date	: 07-Apr-26
		Next calibration date	: 07-Jul-26

Reference Standard Low Flow Meter

Equipment name	: Air Flow Meter	Equiment ID	: BKK_FS0619
Brand	: MesaLabs	Serial No.	: 130026
Model/Type	: Defender 510-L	Calibration Date	: 10-Sep-25
		Due Date	: 09-Sep-26

Reference Standard High Flow Meter

Equipment name	: Air Flow Meter	Equiment ID	: BKK_FS0614
Brand	: MesaLabs	Serial No.	: 151114
Model/Type	: Defender 510-M	Calibration Date	: 10-Sep-25
		Due Date	: 09-Sep-26

Calibration Data

Air Sampling Pump setting (cc/min)	Reference Std. Flow Reading (cc/min)			Avg. (cc/min)	%Error acceptance	Acceptable range (cc/min)			Evaluation (Pass/ Fail)
	1	2	3						
Low Flow									
20	20.6	20.9	20.3	20.6	5%	19	-	21	Passed
50	52.1	51.6	51.3	51.7	5%	48	-	53	Passed
100	102.1	102.1	102.0	102.1	5%	95	-	105	Passed
200	205.4	206.3	202.9	204.9	5%	190	-	210	Passed
High Flow									
500	506.9	506.4	506.5	506.6	3%	485	-	515	Passed
1000	1012.1	1009.0	1011.5	1010.9	3%	970	-	1030	Passed
2000	2010.2	2015.8	2013.5	2013.2	3%	1940	-	2060	Passed
2500	2502.2	2505.2	2502.8	2503.4	3%	2425	-	2575	Passed

---------- END OF REPORT ----------

Calibrated By: (Mr. Natchapon Thamklang)
RYG Field Services Scientist (1)

Approved By: (Mr. Supot Salamteh)
Field Services Section Head

Issue date : 08-Apr-26

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

ACCREDITED
CALIBRATION LABORATORY
AC-2961

Certificate of Calibration

Customer

Name : ALS Laboratory Group Thailand Co., Ltd.
Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang, Bangkok 10250

Certificate No : 25-ACT-042
Request No : Req-2025-0604

Unit Under Calibration Details

Measurement item : Acoustic Calibrator
Manufacturer : RION
Model : NC-75
Serial Number : 35002736
ID : RYG_FS0496

Class : 1
Range : 94 dB / 1000 Hz
Instrument Status : Used

REVIEW BY ..... Narakorn P.
APPROVED BY .....
NEXT CAL DATE..... 19/03/26

Calibration Environment and Details

Temperature : (23 ±2 °C)
Humidity : (50 ± 20 %RH)
Barometric Pressure : (1013 ±10.0 hPa)
Received Date : 6 March 2025
Calibration Date : 19 March 2025
Location of Calibration : LAB 1 Acoustic
Calibration Procedure : In-house method CP-ACT-02 based on IEC 60942:2017 Electroacoustics - Sound calibrators

Reference Standard	Model	Serial Number	Traceable	Due Calibration
Sound Calibrator	SV 35A	58079	EEI	12 June 2025
THD Multimeter	2015	1047765	NIMT	4 February 2026

Traceability : This certificate providoes traceability of measurement to recognized national standard, and to the realization of the international System of Units (SI).

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k =2, providing a level of confidence approximately 95 %.

Calibrated By : Mr. Noppadon Luangart
Service Calibration Engineer

Approved By : Mr. Pacit Mathavorn
Calibration Engineer Supervisor

Issue Date : 19 March 2025

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

Certificate No : 25-ACT-042

Request No : Req-2025-0604

Sound pressure level **Calibration Results :** Without Adjustment

Calibration Range (dB)	Without Adjustment (dB)		Adjustment (dB)		Uncertainty (± dB)	Acceptance limit Class 1 (± dB)	Result
	Measured	Deviated value	Measured	Deviated value			
94 dB / 1000 Hz	94.06	0.06	-	-	0.13	0.25	Pass

Frequency of Sound pressure level

Calibration Range (Hz)	Without Adjustment		Adjustment		Uncertainty (± %)	Acceptance limit Class 1 (± %)	Result
	Measured (Hz)	Deviated	Measured (Hz)	Deviated			
94 dB / 1000 Hz	1000.00	0.00	-	-	0.01	0.70	Pass

Total Harmonic Distortion plus Noise of Sound pressure level (THD+N %)

Calibration Range (Hz)	Without Adjustment	Adjustment	Uncertainty (± %)	Acceptance limit Class 1 (± %)	Result
	Measured (%)	Measured (%)			
94 dB / 1000 Hz	0.98	-	0.40	2.5	Pass

Note :

Function	Maximum-permitted Uncertainty of measurement
Sound pressure level	0.15 dB
Frequency	0.20%
Total distortion+noise	0.50%

- Acceptance limit was IEC60942:2017 Class 1
- The calibration results exclude the calibrator pressure correction
- The calibration results exclude the microphone volume correction

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate No : 25-ACT-042

Request No : Req-2025-0604

Decision Rule for Statements of Conformity


The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09/2019; Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass[1] = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail[1] = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

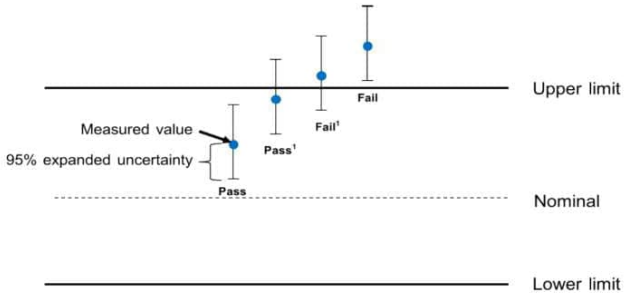

End of Calibration

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

FM-708-ACT-02 Rev.03 Issue date 5/6/24

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

Cert. No. : ACL26111
Pages : 1 of 8

Calibration Certificate

Equipment :	SOUND LEVEL METER
Manufacturer :	RION
Model :	NL-42A / Microphone UC-52 / Preamplifier NH-24
Serial No.:	00623393 / 198640 / 26421
ID No.:	RYG_FS0618

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location :	-	
Ambient Temperature :	(23.0 ± 3)	°C
Pressure :	(101.3 ± 3)	kPa
Relative Humidity :	(50.0 ± 20)	%

Received Date : 12 JANUARY 2026
Calibration Date : 28-30 JANUARY 2026
Date of Issue : 02 FEBRUARY 2026

REVIEW BY .....
APPROVED BY .....
NEXT CAL DATE..... 27/ 01/ 2027

Calibrated by : Nathakorn Pisutpaisan

Approved by :

(Nitinun Srihawan)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL26111
Job No. : VC69AC0058
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0011-25	11-FEB-26
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EEL.BP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EEL.BP 23/0268	22-APR-26
Digital Multimeter	34461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KAI	34560495	AA-3002-25	19-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :
   - 3.1 National Institute of Metrology (Thailand).
   - 3.2 Thailand Institute of Scientific and Technological Research (TISTR).
   - 3.3 Electrical And Electronics Institute (EEI).

Cert. No. : ACL26111
Job No. : VC69AC0058
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

SITHIPORN associates
SITHIPORN ASSOCIATES
CALIBRATION LABORATORY

Cert. No. : ACL26111
Job No. : VC69AC0058
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
17.1

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	12.9
C - weight	17.9
Flat	24.3

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.5	0.5	0.6	± 1.5
1000	0.2	0.2	0.2	± 1.0
8000	1.1	1.2	1.2	±5.0

Cert. No. : ACL26111
Job No. : VC69AC0058
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.1	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	-0.1	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

SITHIPORN associates
SITHIPORN ASSOCIATES
CALIBRATION LABORATORY

Cert. No. : ACL26111
Job No. : VC69AC0058
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	78.9	-0.1	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	63.9	-0.1	± 1.1
59.0	58.9	-0.1	± 1.1
54.0	53.9	-0.1	± 1.1
49.0	48.9	-0.1	± 1.1
44.0	43.9	-0.1	± 1.1
39.0	38.9	-0.1	± 1.1
34.0	33.9	-0.1	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	26.9	-0.1	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.9	-0.1	± 1.1

Cert. No. : ACL26111
Job No. : VC69AC0058
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	28.9	-0.1	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.0 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

SITHIPORN associates
SITHIPORN ASSOCIATES
CALIBRATION LABORATORY

Cert. No. : ACL26111
Job No. : VC69AC0058
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.6	0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a lavel of confidence of approximately 95 %

End of Calibration Certificate

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : ACL26083
Pages : 1 of 8

Calibration Certificate

Equipment :	SOUND LEVEL METER
Manufacturer :	RION
Model :	NL-42A / Microphone UC-52 / Preamplifier NH-24
Serial No.:	00623392 / 198639/ 26420
ID No.:	RYG_FS0617

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location :	-	
Ambient Temperature :	(23.0 ± 3)	°C
Pressure :	(101.3 ± 3)	kPa
Relative Humidity :	(50.0 ± 20)	%

REVIEW BY .....
APPROVED BY .....
NEXT CAL DATE 20/ 01/ 2027

Received Date :	05 JANUARY 2026
Calibration Date :	21 - 23 JANUARY 2026
Date of Issue :	26 JANUARY 2026

Calibrated by : Nathakorn Pisutpaisan

Approved by :

(Nitinun Srihawan)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL26083
Job No. : VC69AC0053
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0011-25	11-FEB-26
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EEL.BP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EEL.BP 23/0268	22-APR-26
Digital Multimeter	34461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KAI	34560495	AA-3002-25	19-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :
   - 3.1 National Institute of Metrology (Thailand).
   - 3.2 Thailand Institute of Scientific and Technological Research (TISTR).
   - 3.3 Electrical And Electronics Institute (EEI).

Cert. No. : ACL26083
Job No. : VC69AC0053
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

SITHIPORN associates
SITHIPORN ASSOCIATES
CALIBRATION LABORATORY

Cert. No. : ACL26083
Job No. : VC69AC0053
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
15.8

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	12.6
C - weight	19.0
Flat	24.8

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.1	0.2	0.2	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	1.1	1.2	1.2	±5.0

Cert. No. : ACL26083
Job No. : VC69AC0053
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.2	0.0	-0.1	±2.0
125	-0.1	0.1	-0.1	±1.5
250	-0.1	0.0	-0.1	±1.5
500	0.0	0.1	-0.1	±1.5
1000	-0.1	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.1	0.0	±3.0
8000	0.0	0.1	0.0	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.1	0.1	± 0.3

SITHIPORN associates
SITHIPORN ASSOCIATES
CALIBRATION LABORATORY

Cert. No. : ACL26083
Job No. : VC69AC0053
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.1	0.1	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.1	0.1	± 1.1
114.0	114.1	0.1	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.1	0.1	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	29.0	0.0	± 1.1
28.0	28.0	0.0	± 1.1
27.0	26.9	-0.1	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.9	-0.1	± 1.1

Cert. No. : ACL26083
Job No. : VC69AC0053
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	28.9	-0.1	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	116.9	-0.1	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	107.9	-0.1	1.0 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.8	-0.2	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

SITHIPORN associates
SITHIPORN ASSOCIATES
CALIBRATION LABORATORY

Cert. No. : ACL26083
Job No. : VC69AC0053
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.4	0.0	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.5	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a lavel of confidence of approximately 95 %

End of Calibration Certificate

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : ACC25058
Pages : 1 of 3

Calibration Certificate

Equipment :	SOUND CALIBRATOR
Manufacturer :	RION
Model :	NC-74
Serial No.:	34178123
ID No.:	RYG_FS0215

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location :	-	
Ambient Temperature :	(23.0 ± 3)	°C
Pressure :	(101.3 ± 3)	kPa
Relative Humidity :	(50.0 ± 20)	%

Received Date :	22 SEPTEMBER 2025
Calibration Date :	08 OCTOBER 2025
Date of Issue :	10 OCTOBER 2025

REVIEW BY .....
APPROVED BY .....
NEXT CAL DATE 07/ 10/ 2026

Calibrated by : Nathakorn Pisutpaisan

Approved by :

(Nitinun Srihawan)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACC25058
Job No. : VC68AC0188
Pages : 2 of 3

Calibration Procedure : CP-AC-03

Calibration Method :

This equipment was calibrated by follow on IEC-60942-2003 Standard.
The sound pressure level, frequency and total distortion of the sound calibrator was measured using the reference microphone.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EEL.BP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EEL.BP 23/0268	22-APR-26
Digital Multimeter	33461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KAI	34560495	AA-3002-25	19-FEB-26
Audio Analyzer	AVR-3360A	V744B6069	EF-0013-25	13-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :
   - 3.1 National Institute of Metrology (Thailand).
   - 3.2 Thailand Institute of Scientific and Technological Research (TISTR).
   - 3.3 Electrical And Electronics Institute (EEI).

Cert. No. : ACC25058
Job No. : VC68AC0188
Pages : 3 of 3

Result of calibration :

1. Sound pressure level

Specified sound pressure level (dB)	Measured value (dB)	Deviated value (dB)	Uncertainty (dB)	Acceptance limit (dB)
94	94.11	0.11	0.14	0.40

2. Frequency

Specified Frequency (Hz)	Measured value (Hz)	Deviated value (%)	Uncertainty (%)	Acceptance limit (%)
1000	1001.5	0.1	0.1	1.0

3. Total distortion

Measured value (%)	Uncertainty (%)	Acceptance limit (%)
1.83	0.10	3.0

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a lavel of confidence of approximately 95 %

End of Calibration Certificate

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

SITHIPORN associates

ilac-MRA

NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : ACL25411
Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.: 00873109 / 171842 / 73485
ID No.: RYG_FS0384

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 ±3) °C
Pressure : (101.3 ±3) kPa
Relative Humidity : (50.0 ±20) %

Received Date : 20 OCTOBER 2025
Calibration Date : 29 - 30 OCTOBER 2025
Date of Issue : 31 OCTOBER 2025

REVIEW BY .....
APPROVED BY .....
NEXT CAL DATE... 28/ 10/ 2026

Calibrated by : Nathakorn Pisutpaisan

Approved by :

(Nitinun Srihawan)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL25411
Job No. : VC69AC0014
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0011-25	11-FEB-26
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EEL.BP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EEL.BP 23/0268	22-APR-26
Digital Multimeter	34461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KAI	34560495	AA-3002-25	19-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

3.3 Electrical And Electronics Institute (EEI).

SITHIPORN associates

SITHIPORN ASSOCIATES
CALIBRATION LABORATORY

Cert. No. : ACL25411
Job No. : VC69AC0014
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

Cert. No. : ACL25411
Job No. : VC69AC0014
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
16.2

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	12.0
C - weight	18.4
Flat	23.8

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.3	0.3	0.3	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	-0.5	-0.5	-0.5	±5.0

SITHIPORN associates
SITHIPORN ASSOCIATES
CALIBRATION LABORATORY

Cert. No. : ACL25411
Job No. : VC69AC0014
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.1	-0.1	±2.0
125	-0.1	0.0	-0.1	±1.5
250	0.0	0.0	-0.1	±1.5
500	0.0	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

Cert. No. : ACL25411
Job No. : VC69AC0014
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	131.9	-0.1	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	29.0	0.0	± 1.1
28.0	28.0	0.0	± 1.1
27.0	27.0	0.0	± 1.1
26.0	26.0	0.0	± 1.1
25.0	25.0	0.0	± 1.1

SITHIPORN associates
SITHIPORN ASSOCIATES
CALIBRATION LABORATORY

Cert. No. : ACL25411
Job No. : VC69AC0014
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	28.9	-0.1	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.0 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

Cert. No. : ACL25411
Job No. : VC69AC0014
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.4	0.0	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.6	89.5	-0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor k = 2
or any value following calculation,providing a lavel of confidence of approximately 95 %

End of Calibration Certificate

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate of Calibration

Customer

Name : ALS Laboratory Group Thailand Co., Ltd.
Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang, Bangkok 10250

Certificate No : 25-SLM-113
Request No : Req-2025-0603

Unit Under Calibration Details

Measurement item : Sound Level Meter
Manufacturer : RION
Model : NL-42
Serial Number : 01173609
ID : RYG_FS0388
Resolution : 0.1 dB

Microphone Class : 2
Microphone Model : UC-52
Microphone S/N : 172170
Preamplifier Model : NH-24
Preamplifier S/N : 74021
Instrument Status : Used

Calibration Environment and Details

Temperature : 23 °C ± 2 °C
Humidity : 50 %RH ± 20 %RH
Barometric Pressure : 1013 hPa ± 10 hPa
Received Date : 6 March 2025
Calibrated Date : 19 March 2025
Calibration Procedure : In-house method CP-SLM-01 based on IEC 61672-3 : 2013 Electroacoustics - Sound level meters - Part 3: Periodic tests
Location of Calibration : Lab Acoustic

REVIEW BY ..... Narakorn P.
APPROVED BY .....
NEXT CAL DATE..... 19/03/26

Reference Standard

Instrument	Brand	Model	SN.	Due calibration	Tracebility
Standard Microphone	Brüel & Kjær	4192	2294985	25 June 2025	NIMT
Audio Generator	Svantek	Svan401	131	15 October 2025	WK Electric

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k = 2, providing a level of confidence approximately 95 %.

Calibrated By : .....
Mr. Noppadon Luangart
Service Calibration Engineer

Approved By : .....
Mr. Pacit Mathavorn
Calibration Engineer Supervisor

Issue Date : 19 March 2025

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate No : 25-SLM-113

Request No : Req-2025-0603

1. Indication at the calibration check frequency

UUC Setting	Nominal	Before Adjust		After Adjust		UNCERTAINTY	Acceptance	Result
FAST / A / 30-130	Level	UUC	ERR	UUC	ERR		Limit	
Calibrator Setting	(dB)	(dB)	(dB)	(dB)	(dB)	(± dB)	(± dB)	
1000 Hz 94 dB	94.06	94.0	-0.06	94.1	+0.04	0.20	0.30	Pass

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand RION, Model NC-75, SN.35002736

2. Self-generated noise, Microphone installed

UUC Setting	Measured	UNCERTAINTY
FAST / 30-130		
UUC Weighting	(dB)	(± dB)
A	15.8	0.10

3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting	Measured	UNCERTAINTY
FAST / 30-130		
UUC Weighting	(dB)	(± dB)
A	12.4	0.10
C	16.7	0.10
Z	20.7	0.10

4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting	Deviation from various Frequency Weighting Respone curve			UNCERTAINTY	Acceptance Limit	Result
FAST / 30-130	A	C	Z			
STD Setting	(dB)	(dB)	(dB)	(± dB)	(± dB)	
125 Hz	0.2	0.4	0.4	0.60	1.5	Pass
1000 Hz	0.0	0.0	0.0	0.60	1.0	Pass
4000 Hz	-0.1	-0.1	-0.1	0.60	3.0	Pass
8000 Hz	-1.4	-1.4	-1.3	0.70	5.0	Pass1

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate No : 25-SLM-113

Request No : Req-2025-0603

5. Electrical signal test of frequency weightings, Weighting network respone with relative to 1 kHz

UUC Setting	Deviation from various Frequency Weighting Respone curve			UNCERTAINTY	Acceptance Limit	Result
FAST / 30-130						
STD Setting	A (dB)	C (dB)	Z (dB)	(± dB)	(± dB)	
63 Hz	-0.2	-0.1	0.0	0.20	2.0	Pass
125 Hz	-0.1	0.0	0.0		1.5	Pass
250 Hz	-0.1	0.0	0.0		1.5	Pass
500 Hz	0.0	0.0	0.0		1.5	Pass
1000 Hz	0.0	0.0	0.0		1.0	Pass
2000 Hz	0.0	0.1	0.0		2.0	Pass
4000 Hz	0.0	0.0	0.0		3.0	Pass
8000 Hz	0.1	0.1	0.0		5.0	Pass
16000 Hz	-1.3	-1.4	0.0		+5, -INF.	Pass

6. Frequency and time weightings at 1kHz

UUC Setting	STD	Measured		UNCERTAINTY	Acceptance Limit	Result
FAST / 30-130	REF	UUC	ERR			
UUC Weighting	(dB)	(dB)	(dB)	(± dB)	(± dB)	
A	114.00	114.0	0.0	0.20	0.20	Pass
C	114.00	114.0	0.0		0.20	Pass
Z	114.00	114.0	0.0		0.20	Pass

UUC Setting	STD	Measured		UNCERTAINTY	Acceptance Limit	Result
30-130 / A	REF	UUC	ERR			
UUC Time Respone	(dB)	(dB)	(dB)	(± dB)	(± dB)	
Fast	114.00	114.0	0.0	0.20	0.10	Pass1
Slow	114.00	114.0	0.0		0.10	Pass1
Leq	114.00	114.0	0.0		0.10	Pass1

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd

FM-708-SLM-01 Rev.04 Issue date 5/6/24

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate No : 25-SLM-113

Request No : Req-2025-0603

7. Long Term Stability

UUC Setting	Measured	UNCERTAINTY	Acceptance	Result
FAST / A / 30-130	UUC		Limit	
STD Setting	(dB)	(± dB)	(± dB)	
Initial	114.0			
Final	114.0			
Deviated	0.0	0.10	0.30	Pass

8. Level linearity on the reference level range

UUC Setting	Anticipated	Deviation		UNCERTAINTY	Acceptance	Result
FAST / A / 30-130	REF	UUC	ERR		Limit	
STD dB	(dB)	(dB)	(dB)	(± dB)	(± dB)	
138.00	138	137.9	-0.1	0.30	1.1	Pass
134.00	134	134.0	0.0		1.1	Pass
129.00	129	128.9	-0.1		1.1	Pass
124.00	124	124.0	0.0		1.1	Pass
119.00	119	119.0	0.0		1.1	Pass
114.00	114	114.0	0.0		1.1	Pass
109.00	109	109.0	0.0		1.1	Pass
104.00	104	104.0	0.0		1.1	Pass
99.00	99	99.0	0.0		1.1	Pass
94.00	94	94.0	0.0		1.1	Pass
89.00	89	89.0	0.0		1.1	Pass
84.00	84	84.0	0.0		1.1	Pass
79.00	79	79.0	0.0		1.1	Pass
74.00	74	74.0	0.0		1.1	Pass
69.00	69	69.0	0.0		1.1	Pass
64.00	64	64.0	0.0		1.1	Pass
59.00	59	59.0	0.0		1.1	Pass
54.00	54	54.0	0.0		1.1	Pass
49.00	49	49.0	0.0		1.1	Pass
44.00	44	44.0	0.0		1.1	Pass
39.00	39	39.0	0.0		1.1	Pass
34.00	34	34.0	0.0		1.1	Pass
29.00	29	29.0	0.0		1.1	Pass
24.00	24	24.1	0.1		1.1	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate No : 25-SLM-113

Request No : Req-2025-0603

9. Level linearity including the level range control

UUC Setting	STD	Measured		UNCERTAINTY	Acceptance	Result
FAST / A	REF	UUC	ERR		Limit	
UUC Range	(dB)	(dB)	(dB)	(± dB)	(± dB)	
30-130	29.50	29.6	0.1	0.30	1.1	Pass
	114	114.0	0.0		1.1	Pass

10. Tone burst response

UUC Setting	STD	Anticipated	Measured		UNCERTAINTY	Acceptance	Result
A / 30-130	Toneburst	Ref	UUC	ERR		Limit	
UUC Time Respone	(ms)	(dB)	(dB)	(dB)	(± dB)	(± dB)	
Fast	200	126.0	126.0	0.0	0.20	1.0	Pass
	2	109.0	109.0	0.0		+1.0, -2.5	Pass
	0.25	100.0	99.9	-0.1		+1.5, -5.0	Pass
Slow	200	119.6	119.6	0.0		1.0	Pass
	2	100.0	100.0	0.0		+1.0, -5.0	Pass
SEL	200	120.0	120.0	0.0		1.0	Pass
	2	100.0	100.0	0.0		+1.0, -2.5	Pass
	0.25	91.0	90.9	-0.1		+1.5, -5.0	Pass

11. Peak C Sound level

UUC Setting	Anticipated	Measured		UNCERTAINTY	Acceptance	Result
FAST / C / 55-141	REF	UUC	ERR		Limit	
STD Setting	(dB)	(dB)	(dB)	(± dB)	(± dB)	
Complete cycle	136.4	136.4	0.00	0.20	3.0	Pass
Positive half cycle	135.4	135.2	-0.20		2.0	Pass
Negative half cycle	135.4	135.2	-0.20		2.0	Pass

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd

FM-708-SLM-01 Rev.04 Issue date 5/6/24

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate No : 25-SLM-113

Request No : Req-2025-0603

12. Overload indication

UUC Setting	Measured	UNCERTAINTY	Acceptance Limit	Result
FAST / A / 30-130	UUC			
STD Setting	(dB)	(± dB)	(± dB)	
Positive one-half cycle	139.5			
Negative one-half cycle	139.4			
Deviated	0.1	0.20	1.5	Pass

13. High Level Stability

UUC Setting	Measured	UNCERTAINTY	Acceptance Limit	Result
FAST / A / 30-130	UUC			
STD Setting	(dB)	(± dB)	(± dB)	
Initial	129.0			
Final	129.0			
Deviated	0.0	0.10	0.30	Pass

Note :

Function	Maximum-permitted Uncertainty of measurement
1. Indication at the calibration check frequency	Not applicable
2. Self-generated noise, Microphone installed	Not applicable
3. Self-generated noise, Microphone replaced by the electrical input signal device	Not applicable
4. Acoustic signal test of frequency weightings at 10 Hz to 4 kHz	0.60 dB
4. Acoustic signal test of frequency weightings at >4 kHz to 10 kHz	0.70 dB
5. Electrical signal test of frequency weightings, Weighting network respone with relative to 1 kHz	0.20 dB
6. Frequency and time weightings at 1kHz	0.20 dB
7. Long Term Stability	0.10 dB
8. Level linearity on the reference level range	0.30 dB
9. Level linearity including the level range control	0.30 dB
10. Tone burst response	0.30 dB
11. Peak C Sound level	0.35 dB
12. Overload indication	0.25 dB
13. High Level Stability	0.10 dB

- Acceptance limit and Maximum-permitted Uncertainty was IEC 61672-1:2013

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate No : 25-SLM-113

Request No : Req-2025-0603

Decision Rule for Statements of Conformity


The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09/2019; Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass[1] = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail[1] = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

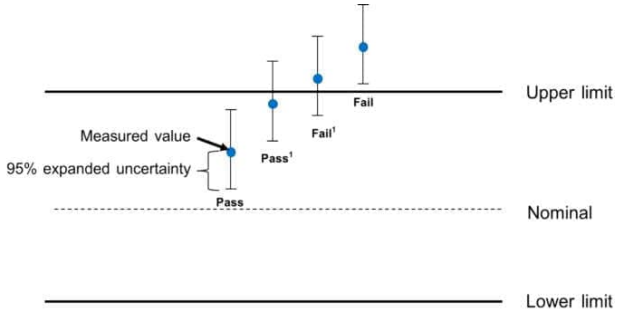

End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd

FM-708-SLM-01 Rev.04 Issue date 5/6/24

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : ACL25410
Pages : 1 of 8

Calibration Certificate

Equipment :	SOUND LEVEL METER
Manufacturer :	RION
Model :	NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.:	00873057 / 143840 / 73333
ID No.:	RYG_FS0381
Condition As Found :	GOOD
Customer :	ALS LABORATORY GROUP (THAILAND) CO., LTD. 104 PHATTHANAKAN 40, PHATTHANAKAN ROAD, KHWAENG PHATTHANAKAN, KHET SUAN LUANG, BANGKOK, 10250 THAILAND.
Location :	-
Ambient Temperature :	(23.0 ± 3) °C
Pressure :	(101.3 ± 3) kPa
Relative Humidity :	(50.0 ± 20) %
Received Date :	20 OCTOBER 2025
Calibration Date :	29 - 30 OCTOBER 2025
Date of Issue :	31 OCTOBER 2025

REVIEW BY .....
APPROVED BY .....
NEXT CAL DATE..... 29/ 10/ 2026

Calibrated by : Nathakorn Pisutpaisan

Approved by :

(Nitinun Srihawan)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL25410
Job No. : VC69AC0014
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0011-25	11-FEB-26
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EEL.BP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EEL.BP 23/0268	22-APR-26
Digital Multimeter	34461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KAI	34560495	AA-3002-25	19-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :
   - 3.1 National Institute of Metrology (Thailand).
   - 3.2 Thailand Institute of Scientific and Technological Research (TISTR).
   - 3.3 Electrical And Electronics Institute (EEI).

Cert. No. : ACL25410
Job No. : VC69AC0014
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

SITHIPORN associates
SITHIPORN ASSOCIATES
CALIBRATION LABORATORY

Cert. No. : ACL25410
Job No. : VC69AC0014
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
15.9

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	11.3
C - weight	17.2
Flat	22.9

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.3	0.3	0.3	± 1.5
1000	0.1	0.1	0.1	± 1.0
8000	-1.0	-0.9	-0.8	±5.0

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.1	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.1	0.1	± 0.3

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	28.0	0.0	± 1.1
27.0	27.0	0.0	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.9	-0.1	± 1.1

Cert. No. : ACL25410
Job No. : VC69AC0014
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	29.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	108.0	0.0	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.0 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

SITHIPORN associates
SITHIPORN ASSOCIATES
CALIBRATION LABORATORY

Cert. No. : ACL25410
Job No. : VC69AC0014
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	132.9	-0.1	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.6	0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	136.9	137.0	-0.1	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a lavel of confidence of approximately 95 %

End of Calibration Certificate

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : ACL25412
Pages : 1 of 8

Calibration Certificate

Equipment :	SOUND LEVEL METER
Manufacturer :	RION
Model :	NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.:	01073423 / 169513 / 73684
ID No.:	RYG_FS0386

REVIEW BY .....
APPROVED BY.....
NEXT CAL DATE..28/ 10/ 2026.....

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location :	-	
Ambient Temperature :	(23.0 ± 3)	°C
Pressure :	(101.3 ± 3)	kPa
Relative Humidity :	(50.0 ± 20)	%

Received Date :	20 OCTOBER 2025
Calibration Date :	29 - 30 OCTOBER 2025
Date of Issue :	31 OCTOBER 2025

Calibrated by : Nathakorn Pisutpaisan

Approved by :

(Nitinun Srihawan)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL25412
Job No. : VC69AC0014
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0011-25	11-FEB-26
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EEL.BP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EEL.BP 23/0268	22-APR-26
Digital Multimeter	34461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KAI	34560495	AA-3002-25	19-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :
   - 3.1 National Institute of Metrology (Thailand).
   - 3.2 Thailand Institute of Scientific and Technological Research (TISTR).
   - 3.3 Electrical And Electronics Institute (EEI).

Cert. No. : ACL25412
Job No. : VC69AC0014
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

SITHIPORN ASSOCIATES
CALIBRATION LABORATORY

Cert. No. : ACL25412
Job No. : VC69AC0014
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
16.1

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	13.4
C - weight	19.3
Flat	25.1

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.2	0.2	0.2	± 1.5
1000	0.1	0.1	0.1	± 1.0
8000	1.5	1.6	1.6	±5.0

Cert. No. : ACL25412
Job No. : VC69AC0014
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.1	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	-0.1	±1.5
500	0.0	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

SITHIPORN associates
SITHIPORN ASSOCIATES
CALIBRATION LABORATORY

Cert. No. : ACL25412
Job No. : VC69AC0014
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	29.0	0.0	± 1.1
28.0	28.0	0.0	± 1.1
27.0	27.0	0.0	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	25.0	0.0	± 1.1

Cert. No. : ACL25412
Job No. : VC69AC0014
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	28.9	-0.1	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.0 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

SITHIPORN associates

SITHIPORN ASSOCIATES
CALIBRATION LABORATORY

Cert. No. : ACL25412
Job No. : VC69AC0014
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.4	0.0	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.5	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a lavel of confidence of approximately 95 %

End of Calibration Certificate

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate of Calibration

Customer

Name : ALS Laboratory Group Thailand Co., Ltd.

Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang, Bangkok 10250

Certificate No : 26-ACT-007

Request No : Req-2026-0043

Unit Under Calibration Details

Measurement item : Acoustic Calibrator

Manufacturer : RION

Model : NC-74

Serial Number : 34178121

ID : RYG_FS0213

Class : 1

Range : 94 dB / 1000 Hz

Instrument Status : Used

Calibration Environment and Details

Temperature : (23 ±2 °C)

Humidity : (50 ± 20 %RH)

Barometric Pressure : (1013 ±10.0 hPa)

Received Date : 7 January 2026

Calibration Date : 9 January 2026

Location of Calibration : LAB 1 Acoustic

Calibration Procedure : In-house method CP-ACT-02 based on IEC 60942:2017 Electroacoustics - Sound calibrators

REVIEW BY .....

APPROVED BY .....

NEXT CAL DATE..... 08/ 01/ 2027 .....

Reference Standard	Model	Serial Number	Traceable	Due Calibration
Sound Calibrator	SV 35A	58079	EEI	20 June 2026
THD Multimeter	2015	1047765	NIMT	4 February 2026

Traceability : This certificate providoes traceability of measurement to recognized national standard, and to the realization of the international System of Units (SI).

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k =2, providing a level of confidence approximately 95 %.

Calibrated By : Mr. Noppadon Luangart
Service Calibration Engineer

Approved By : Mr. Pacit Mathavorn
Calibration Engineer Supervisor

Issue Date : 9 January 2026

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate No : 26-ACT-007

Request No : Req-2026-0043

Sound pressure level **Calibration Results :** Without Adjustment

Calibration Range	Without Adjustment (dB)		Adjustment (dB)		Uncertainty
(dB)	Measured	Deviated value	Measured	Deviated value	(± dB)
94 dB / 1000 Hz	94.08	0.08	-	-	0.12

Frequency of Sound pressure level

Calibration Range	Without Adjustment		Adjustment		Uncertainty
(Hz)	Measured (Hz)	Deviated value (%)	Measured (Hz)	Deviated value (%)	(± %)
94 dB / 1000 Hz	1000.00	0.000	-	-	0.010

Total Harmonic Distortion plus Noise of Sound pressure level (THD+N %)

Calibration Range	Without Adjustment	Adjustment	Uncertainty
(Hz)	Measured (%)	Measured (%)	(± %)
94 dB / 1000 Hz	1.84	-	0.17

Note :

- The calibration results exclude the calibrator pressure correction
- The calibration results exclude the microphone volume correction

End of Calibration

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

FM-708-ACT-02 Rev.04 Issue date 17/2/25

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : ACL25414
Pages : 1 of 8

Calibration Certificate

Equipment :	SOUND LEVEL METER
Manufacturer :	RION
Model :	NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.:	00597169 / 158770 / 34370
ID No.:	RYG_FS0439
Condition As Found :	GOOD
Customer :	ALS LABORATORY GROUP (THAILAND) CO., LTD. 104 PHATTHANAKAN 40, PHATTHANAKAN ROAD, KHWAENG PHATTHANAKAN, KHET SUAN LUANG, BANGKOK, 10250 THAILAND.
Location :	-
Ambient Temperature :	(23.0 ±3) °C
Pressure :	(101.3 ±3) kPa
Relative Humidity :	(50.0 ±20) %
Received Date :	20 OCTOBER 2025
Calibration Date :	05 NOVEMBER 2025
Date of Issue :	06 NOVEMBER 2025

REVIEW BY .....
APPROVED BY .....
NEXT CAL DATE 04/ 11/ 2026

Calibrated by : Nathakorn Pisutpaisan

Approved by : NITINUN. S.

(Nitinun Srihawan)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL25414
Job No. : VC69AC0014
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0011-25	11-FEB-26
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EEL.BP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EEL.BP 23/0268	22-APR-26
Digital Multimeter	34461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KAI	34560495	AA-3002-25	19-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :
   - 3.1 National Institute of Metrology (Thailand).
   - 3.2 Thailand Institute of Scientific and Technological Research (TISTR).
   - 3.3 Electrical And Electronics Institute (EEI).

NITINUN. S.

Cert. No. : ACL25414
Job No. : VC69AC0014
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

SITHIPORN associates
SITHIPORN ASSOCIATES
CALIBRATION LABORATORY

Cert. No. : ACL25414
Job No. : VC69AC0014
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
15.2

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	8.7
C - weight	15.8
Flat	21.5

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.9	0.9	0.9	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	-3.2	-3.1	-3.1	±5.0

Cert. No. : ACL25414
Job No. : VC69AC0014
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.1	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

SITHIPORN associates
SITHIPORN ASSOCIATES
CALIBRATION LABORATORY

Cert. No. : ACL25414
Job No. : VC69AC0014
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	53.9	-0.1	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	26.9	-0.1	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.9	-0.1	± 1.1

CYSTRONICS.

Cert. No. : ACL25414
Job No. : VC69AC0014
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	28.9	-0.1	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.0 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

SITHIPORN ASSOCIATES
CALIBRATION LABORATORY

Cert. No. : ACL25414
Job No. : VC69AC0014
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.7	89.6	-0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a lavel of confidence of approximately 95 %

End of Calibration Certificate

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : ACL26085
Pages : 1 of 8

Calibration Certificate

Equipment :	SOUND LEVEL METER
Manufacturer :	RION
Model :	NL-52A / Microphone UC-59 / Preamplifier NH-25
Serial No.:	01120936 / 21737 / 22325
ID No.:	RYG_FS0627

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location :	-	
Ambient Temperature :	(23.0 ±3)	°C
Pressure :	(101.3 ±3)	kPa
Relative Humidity :	(50.0 ±20)	%

REVIEW BY .....
APPROVED BY .....
NEXT CAL DATE 20/ 01/ 2027

Received Date :	05 JANUARY 2026
Calibration Date :	21 - 23 JANUARY 2026
Date of Issue :	26 JANUARY 2026

Calibrated by : Nathakorn Pisutpaisan

Approved by :

(Nitinun Srihawan)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL26085
Job No. : VC69AC0053
Pages : 2 of 8

Calibration Procedure : CP-AC-02

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0011-25	11-FEB-26
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EEL.BP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EEL.BP 23/0268	22-APR-26
Digital Multimeter	34461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KAI	34560495	AA-3002-25	19-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :
   - 3.1 National Institute of Metrology (Thailand).
   - 3.2 Thailand Institute of Scientific and Technological Research (TISTR).
   - 3.3 Electrical And Electronics Institute (EEI).

Cert. No. : ACL26085
Job No. : VC69AC0053
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

SITHIPORN associates

SITHIPORN ASSOCIATES
CALIBRATION LABORATORY

Cert. No. : ACL26085
Job No. : VC69AC0053
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	94.0	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
14.3

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	8.7
C - weight	14.1
Flat	19.7

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.2	0.2	0.2	± 1.0
1000	0.2	0.1	0.1	± 0.7
8000	0.3	0.4	0.4	+ 1.5, - 2.5

Cert. No. : ACL26085
Job No. : VC69AC0053
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	0.0	-0.1	±1.0
125	0.0	0.0	0.0	±1.0
250	0.0	0.0	-0.1	±1.0
500	0.0	0.0	-0.1	±1.0
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±1.0
4000	0.0	0.0	0.0	±1.0
8000	0.0	0.1	0.1	+ 1.5, - 2.5
16000	0.0	-1.2	-1.2	+ 2.5, -16.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.1

SITHIPORN associates
SITHIPORN ASSOCIATES
CALIBRATION LABORATORY

Cert. No. : ACL26085
Job No. : VC69AC0053
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	±0.8
136.0	136.0	0.0	±0.8
135.0	135.0	0.0	±0.8
134.0	134.0	0.0	±0.8
133.0	133.0	0.0	±0.8
132.0	132.0	0.0	±0.8
131.0	131.0	0.0	±0.8
129.0	129.0	0.0	±0.8
124.0	124.0	0.0	±0.8
119.0	119.0	0.0	±0.8
114.0	114.0	0.0	±0.8
109.0	109.0	0.0	±0.8
104.0	104.0	0.0	±0.8
99.0	99.0	0.0	±0.8
94.0	94.0	0.0	±0.8
89.0	89.0	0.0	±0.8
84.0	83.9	-0.1	±0.8
79.0	78.9	-0.1	±0.8
74.0	73.9	-0.1	±0.8
69.0	68.9	-0.1	±0.8
64.0	63.9	-0.1	±0.8
59.0	58.9	-0.1	±0.8
54.0	53.9	-0.1	±0.8
49.0	48.9	-0.1	±0.8
44.0	43.9	-0.1	±0.8
39.0	38.9	-0.1	±0.8
34.0	33.9	-0.1	±0.8
30.0	29.9	-0.1	±0.8
29.0	28.9	-0.1	±0.8
28.0	28.0	0.0	±0.8
27.0	26.9	-0.1	±0.8
26.0	25.9	-0.1	±0.8
25.0	24.9	-0.1	±0.8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.1	0.1	±0.8

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	29.1	0.1	±0.8

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.0 ; -3.0
	2	8	117.0	117.0	0.0	1.0 ; -1.5
	200	800	134.0	134.0	0.0	±0.5
Slow	2	8	108.0	108.0	0.0	1.0 ; -3.0
	200	800	127.6	127.6	0.0	±0.5
SEL	0.25	1	99.0	98.9	-0.1	1.0 ; -3.0
	2	8	108.0	108.0	0.0	1.0 ; -1.5
	200	800	128.0	128.0	0.0	±0.5

SITHIPORN associates

SITHIPORN ASSOCIATES
CALIBRATION LABORATORY

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±2.0
One	133.4	133.4	0.0	±2.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±1.0
Positive half cycle	135.4	135.2	-0.2	±1.0
Negative half cycle	135.4	135.2	-0.2	±1.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.5	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.1

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a lavel of confidence of approximately 95 %

End of Calibration Certificate

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : ACL25413
Pages : 1 of 8

Calibration Certificate

Equipment :	SOUND LEVEL METER
Manufacturer :	RION
Model :	NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.:	00597168 / 180411 / 88181
ID No.:	RYG_FS0438
Condition As Found :	GOOD
Customer :	ALS LABORATORY GROUP (THAILAND) CO., LTD. 104 PHATTHANAKAN 40, PHATTHANAKAN ROAD, KHWAENG PHATTHANAKAN, KHET SUAN LUANG, BANGKOK, 10250 THAILAND.
Location :	-
Ambient Temperature :	(23.0 ± 3) °C
Pressure :	(101.3 ± 3) kPa
Relative Humidity :	(50.0 ± 20) %
Received Date :	20 OCTOBER 2025
Calibration Date :	29 - 30 OCTOBER 2025
Date of Issue :	31 OCTOBER 2025

REVIEW BY .....
APPROVED BY .....
NEXT CAL DATE... 28/ 10/ 2026 .....

Calibrated by : Nathakorn Pisutpaisan

Approved by :

(Nitinun Srihawan)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL25413
Job No. : VC69AC0014
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0011-25	11-FEB-26
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EEL.BP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EEL.BP 23/0268	22-APR-26
Digital Multimeter	34461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KAI	34560495	AA-3002-25	19-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :
   - 3.1 National Institute of Metrology (Thailand).
   - 3.2 Thailand Institute of Scientific and Technological Research (TISTR).
   - 3.3 Electrical And Electronics Institute (EEI).

Cert. No. : ACL25413
Job No. : VC69AC0014
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

SITHIPORN associates
SITHIPORN ASSOCIATES
CALIBRATION LABORATORY

Cert. No. : ACL25413
Job No. : VC69AC0014
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
14.8

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	11.6
C - weight	18.0
Flat	23.5

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.1	0.1	0.1	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	1.3	1.4	1.4	±5.0

Cert. No. : ACL25413
Job No. : VC69AC0014
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	-0.1	-0.1	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

SITHIPORN associates
SITHIPORN ASSOCIATES
CALIBRATION LABORATORY

Cert. No. : ACL25413
Job No. : VC69AC0014
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.1	0.1	± 1.1
84.0	84.1	0.1	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.1	0.1	± 1.1
69.0	69.1	0.1	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.1	0.1	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.1	0.1	± 1.1
30.0	30.1	0.1	± 1.1
29.0	29.1	0.1	± 1.1
28.0	28.1	0.1	± 1.1
27.0	27.1	0.1	± 1.1
26.0	26.2	0.2	± 1.1
25.0	25.1	0.1	± 1.1

Cert. No. : ACL25413
Job No. : VC69AC0014
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	28.9	-0.1	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.0 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

SITHIPORN associates
SITHIPORN ASSOCIATES
CALIBRATION LABORATORY

Cert. No. : ACL25413
Job No. : VC69AC0014
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.5	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a lavel of confidence of approximately 95 %

End of Calibration Certificate

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : ACL26084
Pages : 1 of 8

Calibration Certificate

Equipment :	SOUND LEVEL METER
Manufacturer :	RION
Model :	NL-52A / Microphone UC-59 / Preamplifier NH-25
Serial No.:	00920831 / 22191 / 22220
ID No.:	RYG_FS0622

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location :	-	
Ambient Temperature :	(23.0 ±3)	°C
Pressure :	(101.3 ±3)	kPa
Relative Humidity :	(50.0 ±20)	%

Received Date : 05 JANUARY 2026
Calibration Date : 21 - 23 JANUARY 2026
Date of Issue : 26 JANUARY 2026

REVIEW BY .....
APPROVED BY .....
NEXT CAL DATE 20/ 01 /2027

Calibrated by : Nathakorn Pisutpaisan

Approved by :

(Nitinun Srihawan)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL26084
Job No. : VC69AC0053
Pages : 2 of 8

Calibration Procedure : CP-AC-02

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0011-25	11-FEB-26
Waveform Generator	33511B	MY52302742	EF-0012-25	11-FEB-26
Digital Multimeter	33461A	MY53220104	EEL.BP 24/0268	22-APR-26
Digital Multimeter	33461A	MY53220076	EEL.BP 23/0268	22-APR-26
Digital Multimeter	34461A	MY60024273	CA2025120EA	18-MAR-26
Programmable Attenuator	MAT-1070	62100114	EF-0006-25	11-FEB-26
Condenser Microphone	4180	2977900	AA-1002-25	19-FEB-26
Measuring Amplifier	NA-42KAI	34560495	AA-3002-25	19-FEB-26

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :
   - 3.1 National Institute of Metrology (Thailand).
   - 3.2 Thailand Institute of Scientific and Technological Research (TISTR).
   - 3.3 Electrical And Electronics Institute (EEI).

Cert. No. : ACL26084
Job No. : VC69AC0053
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

SITHIPORN associates
SITHIPORN ASSOCIATES
CALIBRATION LABORATORY

Cert. No. : ACL26084
Job No. : VC69AC0053
Page : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.94)	94.0	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
13.8

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting (dB)
A - weight	8.7
C - weight	14.0
Flat	19.7

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.3	0.3	0.3	± 1.0
1000	0.2	0.2	0.2	± 0.7
8000	0.7	0.8	0.8	+ 1.5, - 2.5

Cert. No. : ACL26084
Job No. : VC69AC0053
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	-0.1	0.0	±1.0
125	0.0	0.0	0.0	±1.0
250	0.0	0.0	0.0	±1.0
500	0.0	0.0	0.0	±1.0
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±1.0
4000	0.0	0.0	0.0	±1.0
8000	0.0	0.1	0.1	+ 1.5, - 2.5
16000	0.0	-1.2	-1.2	+ 2.5, -16.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.1

SITHIPORN associates
SITHIPORN ASSOCIATES
CALIBRATION LABORATORY

Cert. No. : ACL26084
Job No. : VC69AC0053
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	±0.8
136.0	136.0	0.0	±0.8
135.0	135.0	0.0	±0.8
134.0	134.0	0.0	±0.8
133.0	133.0	0.0	±0.8
132.0	132.0	0.0	±0.8
131.0	131.0	0.0	±0.8
129.0	129.0	0.0	±0.8
124.0	124.0	0.0	±0.8
119.0	119.0	0.0	±0.8
114.0	114.0	0.0	±0.8
109.0	109.0	0.0	±0.8
104.0	104.0	0.0	±0.8
99.0	99.0	0.0	±0.8
94.0	94.0	0.0	±0.8
89.0	89.0	0.0	±0.8
84.0	84.0	0.0	±0.8
79.0	79.0	0.0	±0.8
74.0	74.0	0.0	±0.8
69.0	69.0	0.0	±0.8
64.0	64.0	0.0	±0.8
59.0	59.0	0.0	±0.8
54.0	53.9	-0.1	±0.8
49.0	49.0	0.0	±0.8
44.0	43.9	-0.1	±0.8
39.0	38.9	-0.1	±0.8
34.0	33.9	-0.1	±0.8
30.0	29.9	-0.1	±0.8
29.0	28.9	-0.1	±0.8
28.0	27.9	-0.1	±0.8
27.0	26.9	-0.1	±0.8
26.0	25.9	-0.1	±0.8
25.0	24.9	-0.1	±0.8

Cert. No. : ACL26084
Job No. : VC69AC0053
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±0.8

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	29.0	28.9	-0.1	±0.8

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.0 ; -3.0
	2	8	117.0	117.0	0.0	1.0 ; -1.5
	200	800	134.0	134.0	0.0	±0.5
Slow	2	8	108.0	108.0	0.0	1.0 ; -3.0
	200	800	127.6	127.6	0.0	±0.5
SEL	0.25	1	99.0	98.9	-0.1	1.0 ; -3.0
	2	8	108.0	108.0	0.0	1.0 ; -1.5
	200	800	128.0	128.0	0.0	±0.5

SITHIPORN associates
SITHIPORN ASSOCIATES
CALIBRATION LABORATORY

Cert. No. : ACL26084
Job No. : VC69AC0053
Pages : 8 of 8

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±2.0
One	133.4	133.3	-0.1	±2.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±1.0
Positive half cycle	135.4	135.2	-0.2	±1.0
Negative half cycle	135.4	135.2	-0.2	±1.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.5	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.1

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation,providing a lavel of confidence of approximately 95 %

End of Calibration Certificate

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

ilac-MRA

NSC-TISI-TIS17025
CALIBRATION 0008

Certificate of Calibration

Cert. No.: 25LM10
Page.: 1 of 2

Equipment :	DO Meter with Sensor
Manufacturer :	YSI
Model :	5000-115V
Serial No. :	15E102796
ID No. :	RYG_EN0032

REVIEW BY Photchana S.
APPROVED BY D. Thumsa.
NEXT CAL DATE 20/07/26

Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch) 616/10 Moo 5 T. Maenam Khu, A. Pluakdaeng, Rayong 21140 Thailand
Location :	TPA On Site Calibration Laboratory
Received Order :	17 January 2025
Calibrated Date :	20 January 2025
Ambient Temperature :	(26 ± 10) °C
Relative Humidity :	(50 ± 30) %
AC Line Voltage :	(220 ± 22) V
Calibrated by :	Warakorn Lerngagtrakul
Approved by :	Approved Signatory

( ) Chakrit Waewwanjua
(✓) Suwit Imjai
( ) Kunchit Promprat

Issue Date : 23 January 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Digital Thermometer	2188080	24I1022	TPA	17 Sep 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N.: 15E100464

Calibration Point (°C)	Immersion Depth (mm)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty (± °C)	Coverage Factor *k*
20.00	60	20.002	19.81	-0.192	0.15	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor ***k***, providing a level of confidence of approximately 95 %.

-o0o-

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000 FAX. 0-2719-9484

Certificate of Testing

Equipment :	DO Meter
Manufacturer :	YSI
Model :	5000-115V
Serial No. :	15E102796
ID No. :	RYG_EN0032
Received Date :	17 January 2025
Test Date :	20 January 2025
Reference :	2501-0600DSC-1
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch) 616/10 Moo 5, T.Maenam Khu, A.Pluakdaeng, Rayong 21140, Thailand
Laboratory Condition :	Temperature (25 ± 5) °C Humidity (50 ± 20) %
Test Procedure :	In - house method : CP-CH9 by Comparison Technique with Azide Modification Method
Tested by :	Walalak Sirithean
Approved by :	Saithip Approved Signatory

( ) Pornthippa Tameyakul
( ) Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 21 January 2025

Condition of this result of calibration

1. Reference Standard Instruments :
   This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

Instruments	Serial No.	ID No.	Certificate No.	Due Date
1. Burette	-	130BU10	23CG1172	22 Mar 2025
2. Balance	14233821	110RC001	24MM131	04 July 2025

2. Standard Material :-

Material	Manufacturer	Lot.No.	Assay
Sodium Thiosulfate 5-Hydrate AR	KEMAUS	2203162447	99.6%

Result : **Dissolved Oxygen Meter Adjustment With Air 100 %**
Dissolved Oxygen Probe No.: 15E100464

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.20	8.20	0.0084

This report was certified only for the instrument we tested.It is allowable to use for study Intend to use for advertising and referral purpose is prohibited.This report may not be reproduced other in full, without written approval of the laboratory

-o0o-

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Certificate of Calibration

Equipment :	Low Temp. Incubator
Manufacturer :	Memmert
Model :	IPP750
Serial No. :	V818.0084
ID No. :	RYG_EN0154
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. Rayong Branch 616/10 Moo 5, T.Maenam Khu, A.Pluakdaeng, Rayong 21140, Thailand
Location :	BOD Room
Received Order :	01 November 2024
Calibration Date :	01 November 2024
Ambient Temperature :	(26 ± 10) °C
Relative Humidity :	(50 ± 30) %
AC Line Voltage :	(220 ± 22) V

REVIEW BY ..... Thanitak.

APPROVED BY..... D.Khunou

NEXT CAL DATE..... 01/05/26

Calibrated by : Krisda Malee

Approved by : Kunchit.
Approved Signatory

( ) Ponpan Paipim
( ) Suwit Imjai
(✓) Kunchit Promprat

Issue Date : 07 November 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-


Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY44073381	24LM73	TPA	18 May 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Environment during calibration		
	Beginning	**Finished**
Temp. (°C)	24	25
REL.Humid. (%)	55	53
AC Supply (Volt)	220	221

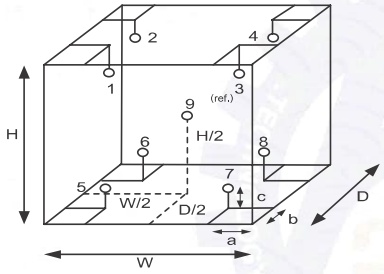

Position :	Ref. Std. ID No.:
1	1RTD-2/1
2	1RTD-2/2
3	22-01RTD-03
4	1RTD-2/4
5	1RTD-2/5
6	1RTD-2/6
7	23-01RTD-07
8	1RTD-2/8
9 (ref.)	23-01RTD-09

Probe Installation Details :

a =	10	cm
b =	10	cm
c =	10	cm

Dimension of Chamber :

D =	0.60	m
W =	1.0	m
H =	1.2	m
Capacity =	0.72	m^3

Equipment : Low Temp. Incubator
Condition As-Received : Used Item
Reference : 2411-0002OC-1
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Cert. No.: 24TM1663
Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor *k*
20.0	20.0	20.0	0.026	0.26	0.53	2

Calibration Point	Measured Temperature (°C) Position									Uncertainty
(°C)	1	2	3	4	5	6	7	8	9 (ref.)	(±°C)
20.0	20.071	19.915	20.273	20.179	19.977	19.782	20.056	20.026	20.033	0.30

Average* : The average of 30 values in each position.
Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.
Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.
Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.
UUC* : Unit Under Calibration
Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor ***k***, providing a level of confidence of approximately 95 %.

-o0o-

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

ilac-MRA
NSC-TISI-TIS17025
CALIBRATION 0008

Certificate of Calibration

Cert. No.: 26TM461
Page : 1 of 3

REVIEW BY Thanitak.
APPROVED BY D.Kunnon.
NEXT CAL DATE 18/09/27

Equipment : Low Temp. Incubator
Manufacturer : Memmert
Model : IPP750
Serial No. : V818.0084
ID No. : RYG_EN0154
Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd. Rayong Branch
616/10 Moo 5, T.Maenamkoo, A.Pluakdaeng,
Rayong 21140, Thailand
Location : BOD Room

Received Order : 18 March 2026
Calibration Date : 18 March 2026
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %
AC Line Voltage : (220 ± 22) V

Calibrated by : Preecha Hlahib

Approved by : Kunchit
Approved Signatory

( ) Chakrit Waewwanjua
( ) Suwit Imjai
(✓) Kunchit Promprat

Issue Date : 31 March 2026

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Equipment : Low Temp. Incubator **Cert. No.:** 26TM461
Condition As-Received : New Item **Page :** 2 of 3
Reference : 2603-0502OC-2

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-


Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY49023932	25LM121	TPA,	27 Jul 2026

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This measurement result is traceable to the International System of Unit maintained through :

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Not Available

Environment during calibration		
	Beginning	Finished
Temp. (°C)	23	21
REL.Humid. (%)	37	33
AC Supply (Volt)	220	221

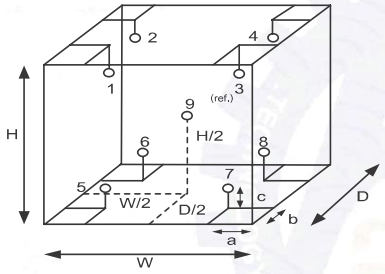

Position :	Ref. Std. ID No.:
1	19-16RTD-01
2	19-16RTD-02
3	19-16RTD-03
4	23-16RTD-04
5	19-16RTD-05
6	19-14RTD-06
7	21-16RTD-07
8	19-16RTD-08
9 (ref.)	19-16RTD-09

Probe Installation Details :

a =	10	cm
b =	10	cm
c =	10	cm

Dimension of Chamber :

D =	0.60	m
W =	1.0	m
H =	1.2	m
Capacity =	0.72	m^3

Equipment : Low Temp. Incubator **Cert. No.:** 26TM461
Condition As-Received : New Item **Page :** 3 of 3
Reference : 2603-0502OC-2
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Not Available

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor *k*
20.0	20.0	20.0	0.019	0.19	0.34	2

Calibration Point (°C)	Measured Temperature (°C) Position									Uncertainty (±°C)
	1	2	3	4	5	6	7	8	9 (ref.)	
20.0	20.185	20.132	20.303	20.160	20.001	20.054	19.983	20.060	20.163	0.30

Average* : The average of 30 values in each position.
Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.
Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.
Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.
UUC* : Unit Under Calibration
Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor ***k***, providing a level of confidence of approximately 95 %.

-o0o-

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Certificate of Calibration

Equipment :	Burette
Capacity :	50 mL
Serial No. :	-
ID. No. :	RYG_EN0216
Manufacturer :	Witeg
Made in :	Germany

REVIEW BY ..... Thanitak.

APPROVED BY..... D.Sumon.

NEXT CAL DATE..... 18/09/26

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
Rayong Branch
616/10 Moo 5 T.MaenamKoo, A.Pluakdaeng
Rayong 21140, Thailand

Ambient Temperature :	(20 ± 2.5) °C
Relative Humidity :	(50 ± 10) %
Barometric Pressure :	753 mmHg
Calibration Procedure :	ASTM E 542 - 01
Calibrated by :	Srisuda Khamtha

Approved by :

Approved Signatory

( ) Ponpan Paipim
(✓) Chakrit Waewwanjua

Issue Date : 19 September 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Condition of this result of calibration

1. Reference Standard Instruments :

Instruments	Model	Serial No.	ID. No.	Certificate No.	Traceability	Due date
1) Balance	XP205	B134206712	140RC007	25MM296	TPA	16 July 2026
2) Humidity/Baro/Temp	MHB-382SD	AM.42259	140EC016	25H1616	TPA	14 Aug 2026
3) Digital Thermometer	HH376	230806555	140EC013	25I1740	TPA	17 Jan 2026

   This measurement result is traceable to SI Unit
2. The certificate is valid only to the item calibrated on date and place of calibration.
3. True value is converted to true volume at the standard temperature of 20 °C

Calibration result :

Nominal capacity (mL)	Reading (mL)	Uncertainty (± mL)	*k* Factor
10	10.0264	0.0082	2.00
25	25.0141	0.0087	2.00
50	49.9952	0.010	2.00

Remark mL = cm^3

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k* , providing a level of confidence of approximately 95 %.

-o0o-

Certificate of Calibration

NSC-TISI-TIS 17025
Calibration 0087

Equipment:	SPECTROPHOTOMETER	Certificate No.:	C06250108
Model:	DR6000	Issued Date:	18 March 2025
Serial No. (or ID.):	1627845 (RYG_EN0037)	Job No.:	WO-00064379
Manufacturer:	HACH	Page:	1 of 3
Condition:	In Condition		

Customer: ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
616/10 Moo 5 T.Maenam Khu,
A.Pluakdaeng, Rayong 21140, Thailand.

REVIEW BY Photchanas.
APPROVED BY
NEXT CAL. DATE 18/09/26

Environment Condition: Temperature 24.4 °C ± 0.3 °C
Humidity 60.8 %RH ± 3.5 %RH

Calibration Place: ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
(Wet Chemistry Lab)
616/10 Moo 5 T.Maenam Khu, A.Pluakdaeng, Rayong 21140, Thailand.

Calibration By: Mr.Preecha Phooarsai

Calibration Date: 18 March 2025

The Method used: In house method, CAL-WI-24, base on ASTM E 275-08 and ASTM E 387-04

Traceability: This certificate is traceable to the CRM maintained by National Institute of Standards and Technology (NIST) through Starna Scientific Limited.

The standard for Wavelength Certificate No. 111583 and 111584
The standard for Photometric Certificate No. 9114984 and 111588
The standard for Stray light Certificate No. 111586 and 111585
The standard for Spectral resolution Certificate No. 111587

(Mr. Preecha Phooarsai)
Person in charge

(Miss Kaewkan Suradech)
Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Calibration Results:

Without Adjustment

Wavelength Accuracy (nm), The spectral bandwidth of Std at 2 nm and UUC at 2 nm

Standard Wavelength	Unit Under Calibration	Correction	Uncertainty
418.61	418.5	0.11	0.13
536.66	536.7	-0.04	0.13
637.98	638.3	-0.32	0.13
748.48	748.8	-0.32	0.13
807.03	807.5	-0.47	0.13

Photometric Accuracy (Absorbance)

Wavelength	Standard absorbance	Unit Under Calibration	Correction	Uncertainty
420 nm	0.0000	0.000	0.0000	0.0045
	0.2930	0.291	0.0020	0.0045
	0.5168	0.518	-0.0012	0.0045
	1.0298	1.031	-0.0012	0.0045
440 nm	0.0000	0.000	0.0000	0.0045
	0.2867	0.285	0.0017	0.0045
	0.5073	0.508	-0.0007	0.0045
	1.0083	1.009	-0.0007	0.0045
465 nm	0.0000	0.000	0.0000	0.0045
	0.2516	0.250	0.0016	0.0045
	0.4595	0.461	-0.0015	0.0045
	0.9334	0.935	-0.0016	0.0045
546.1 nm	0.0000	0.000	0.0000	0.0045
	0.2461	0.246	0.0001	0.0045
	0.4652	0.466	-0.0008	0.0045
	0.9468	0.948	-0.0012	0.0045
590 nm	0.0000	0.000	0.0000	0.0045
	0.2594	0.259	0.0004	0.0045
	0.5040	0.505	-0.0010	0.0045
	1.0032	1.004	-0.0008	0.0045
635 nm	0.0000	0.000	0.0000	0.0045
	0.2579	0.258	-0.0001	0.0045
	0.4971	0.497	0.0001	0.0045
	0.9720	0.973	-0.0010	0.0045

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth – in Asia and Beyond.
CAL-FM-C06-16: 11 Mar 2024

Calibration Results:

Without Adjustment

Photometric Accuracy (Absorbance)

Wavelength	Standard absorbance	Unit Under Calibration	Correction	Uncertainty
235 nm	0.0000	0.000	0.0000	0.0080
	0.7355	0.738	-0.0025	0.0080
257 nm	0.0000	0.000	0.0000	0.0080
	0.8574	0.857	0.0004	0.0080
313 nm	0.0000	0.000	0.0000	0.0080
	0.2864	0.290	-0.0036	0.0080
350 nm	0.0000	0.000	0.0000	0.0080
	0.6374	0.637	0.0004	0.0080

Stray light *

Standard: cut-off	UUC: Wavelength (nm)	UUC: Transmission (%T)	Absorbance (A)
260.62 +/- 0.11 nm	260.6	1.7	1.770
391.44 +/- 0.11 nm	391.4	1.4	1.854

Spectral Resolution *

Nominal Concentration 0.02 % v/v	Peak	Trough	Ratio	SBW
Standard Wavelength (nm)	268.66	266.69	1.38	2.00
UUC: Wavelength (nm)	268.2	266.2		
Std Absorbance (A)	0.4566	0.2780		
UUC: Absorbance (A)	0.413	0.299		

* Calibration Marked " Not TISI Accredited " in this Certificate have been included for completeness.

The End of Certificate

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

ใบตรวจสอบสภาพเครื่องวัดสิ่งแวดล้อม

เลขที่ใบงาน: WO-00064379

ชนิดเครื่องมือ: SPECTROPHOTOMETER รุ่น: DR6000 หมายเลขเครื่อง: 1627845

ตรวจสอบ (รับ) 18 Mar 2025 ปกติ	ตรวจสอบ (รับ) 18 Mar 2025 ไม่ปกติ	รายการตรวจเช็ค	ตรวจสอบ (ส่ง) 18 Mar 2025 ปกติ	ตรวจสอบ (ส่ง) 18 Mar 2025 ไม่ปกติ	หมายเหตุ
		General			
☑	☐	1. ความสมบูรณ์เครื่อง	☑	☐	
☑	☐	2. ความสะอาด (ช่องใส่ตัวอย่าง, ภายใน-นอกเครื่อง)	☑	☐	
☑	☐	3. สวิทช์ ปิด – เปิด เครื่อง (On-Off Swicth)	☑	☐	
☑	☐	4. ปุ่มกด (Keypad)	☑	☐	
☑	☐	5. หน้าจอ (Display, Screen Contrast)	☑	☐	
		Spectrophotometer			
☐	☐	6. แรงดันไฟฟ้า (Battery Backup) >= 2.5 VDC	☐	☐	
☐	☐	7. ตัวหมุนเลือกความยาวคลื่น (Wavelength Control)	☐	☐	
☑	☐	8. ความยาวคลื่น (Wavelength Check)	☑	☐	*
☑	☐	9. แหล่งกำเนิดแสง (UV < 3,000 hour)	☑	☐	13.5 Hours
☑	☐	10. แหล่งกำเนิดแสง (Visible < 5,000 hour)	☑	☐	893.0 Hours
☑	☐	11. ช่องวัดหลายตัวอย่าง (Carousel Module)	☑	☐	
		pH Meter and Conductivity Meter			
☐	☐	12. อิเล็คโทรด (Electrode and Connection Cable)	☐	☐	
☐	☐	13. ระดับสารละลายใน Electrode (Level KCl)	☐	☐	
☐	☐	14. ฝาปิดกันปลาย Electrode (Dust Protection Hood)	☐	☐	
☐	☐	15. ขาจับอิเล็คโทรด (Stand)	☐	☐	
		Turbidimeter			
☐	☐	16. ค่าความขุ่นที่ต่ำสุด (No Sample)	☐	☐	
☐	☐	17. ระดับการส่องสว่างของแสง (>= 2.5 ไม่เกิน 3.0)	☐	☐	
		Automatic titrator			
☐	☐	18. สภาพ Piston Burettes	☐	☐	
☐	☐	19. Function Rinsing and Dosing	☐	☐	
☐	☐	20. ระบบท่อสายยางและอุปกรณ์ประกอบ	☐	☐	

เพิ่มเติม/ข้อแนะนำ : * 656.1nm = 656.1nm

* 486.0nm = 485.7nm

Mr.Preecha Phooarsai

Service Engineer

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Certificate of Calibration

Cert.No.: 25CH847
Page.: 1 of 3

Equipment :	pH Meter
Manufacturer :	Mettler Toledo
Model :	SevenCompact S220
Serial No. :	C104059460
ID No. :	RYG_EN0183
Condition As-Received:	Used Item
Received Date :	17 July 2025
Calibration Date :	18 July 2025
Reference :	2507-0561DSC-3
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. Rayong Branch 616/10 Moo 5, T.Maenam Khu, A.Pluakdaeng, Rayong 21140, Thailand
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure :	In - house method : - CP-CH5 by direct measurement with DC voltage standard and direct measurement with certified reference material (CRM) - CP-CH8 by comparison with temperature standard

REVIEW BY ..... PhotchanaS.

APPROVED BY.....

NEXT CAL DATE.....18/01/27.....

Calibrated by : Walalak Sirithean

Approved by : Saithip

Approved Signatory

( ) Chakrit Waewwanjua
( ) Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 21 July 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Condition of this calibration result

1. Reference Standard Instrument

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1) Document Process Calibrator	54030049	130RC116	24E2759	25 Aug 2025
2) Ref. Standard Thermometer	3240076	60RC033	25I394	01 Apr 2026

- This measurement result is traceable to SI throught Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.007	CPA chem	1066665	18 Jan 2027
pH 6.965	CPA chem	1066667	18 Jan 2026
pH 10.010	CPA chem	1114385	08 June 2026

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4,7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement	Coverage factor
	pH	mV	mV	pH	(±mV)	*k*
pH Meter	4.000	177.48	177.3	4.000	0.058	2.00
S/N.: C104059460	7.000	0.00	-0.2	7.000	0.058	2.00
	10.000	-177.48	-177.6	10.000	0.058	2.00

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (±)	Coverage factor *k*
pH Electrode	4.007	4.008	184.6	0.0044	2.00
S/N.: 5240606	6.965	6.966	10.2	0.0084	2.00
	10.010	10.009	-164.9	0.0065	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : InLabExpert Pro-ISM
- Serial No. : 5240606

Dimension of probe

- Length : 120 mm.
- Diameter : 12 mm.
- Immersion Depth : 100 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (± °C)	Coverage factor *k*
25.0	25.001	25.0	-0.001	0.13	2.00

Remark - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Certificate of Calibration

Certificate No. : 25E2372
Page : 1 of 2

Equipment : pH Meter
Manufacturer: Mettler Toledo
Model : SevenCompact S220
Serial No.: C104059460
ID No.: RYG_EN0183
Condition As-Received: Used Item
Received Date: 17 July 2025
Calibration Date: 22 July 2025

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

Reference: 2507-0561DSC
Ambient Temperature: (23 ± 2) °C
Relative Humidity: (50 ± 10) %

Submitted by: ALS Laboratory Group (Thailand) Co.,Ltd. Rayong Branch
616/10 Moo 5, T.Maenam Khu, A.Pluakdaeng,
Rayong 21140, Thailand

Procedure used: Calibration were conducted using calibration procedure No. CP-E17 according to EURAMET cg-15.

Condition of this result of calibration

1.Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Multi-Product Calibrator	5500A	6315011	25E1627	19 May 2026

2.This result of calibration was made on requested at the point specified by customer.

3.The certificate is valid only to the item calibrated on date and place of calibration.

4.This measurement result is traceable to the International System of Unit maintained through:-

-Technology Promotion Association (Thailand-Japan), NSC-ONSC Accredited No. Calibration 0008

Calibrated by : Napachanok Prasomsoosiri
Issue Date : 23 July 2025

Approved Signatory : _____

[ ] Phalinee Prabpaipal
[ ] Nuntawat Khamchai
[✓] Pongsagorn Boonyaporn

Result of calibration :- (*) Without adjustment ( ) After adjustment

Function: DC voltage measurement **Range:** 2000 mV

Standard Value	UUC* Reading	Error	Uncertainty
(mV)	(mV)	(mV)	(± µV)
-200.0000	-200.0	0.0	68
-150.0000	-150.0	0.0	65
-100.0000	-100.0	0.0	63
-50.0000	-50.0	0.0	61
0.0000	0.0	0.0	58
50.0000	49.9	-0.1	61
100.0000	99.9	-0.1	63
150.0000	149.9	-0.1	65
200.0000	199.9	-0.1	68

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k* = 2, providing a level of confidence of approximately 95 %

UUC* = Unit Under Calibration.

-o0o-

SARTORIUS

Accredited by

NSC-TISI-TIS 17025
Calibration 0426

NSC-TISI-TIS 17025
CALIBRATION 0426

Calibration certificate

Calibration Certificate No. 25BKL0003

Object	Electronic non-automatic weighing instrument
Manufacturer	Sartorius
Type	MSU224S-100-DU
Serial | QM Ident. no.	31709552 | RYG_EN0003
Customer	ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
	616/10 Moo 5 T.Maenam Khu, A.Pluak Daeng, Rayong 21140, Thailand.
Order no.	2230
Number of pages	4
Date of calibration	20 Feb 2025

This calibration certificate documents the traceability to national standards.

Uncertainties of measurements are taken into account when only statements of compliance are made.

This certificate was prepared by Sartorius Corporation in accordance to the current ISO/IEC 17025:2017 standard and Sartorius Work Instruction (Method) SOP WI 08.

This certificate relate and apply this equipment only.

REVIEW BY ..... Thanitak.

APPROVED BY..... D. Thanon.

NEXT CAL DATE..... 20/02/26

This calibration certificate may not be reproduced other than in full except with the permission of NSC-TISI-TIS-17025 and the issuing laboratory. Calibration certificates without signature are not valid.

The user is obliged to have the object recalibrated at appropriate intervals.

Date	Approval of the Calibration Certificate	Person in charge
06 Mar 2025	Mr. Chonchai Inthana	Kachen Lalee

Calibration object

Single range instrument

Model	MSU224S-100-DU
Serial Number	31709552
QM Ident. no | Inventory no.	RYG_EN0003 | ---

Maximum capacity (Max. load)	220.0000 g
Measured range	220.0000 g
Scale interval	0.0001 g

Place of calibration

Address	According to page 1
Department | Cost center	Laboratory Department. | —
Building | Floor	— | 1st Floor.
Room	Balance Room.
Maximum temperature variation at place of calibration	5 K

Calibration procedure

EURAMET cg-18, V4.0 - Guidelines on the Calibration of Non-Automatic Weighing Instruments

Test equipment

Test equipment type	Test equipment ID	Valid until
Thermometer	MHB-382SD s/nB011342 Traceable to SI unit through DKSH	21 Aug 2025
Test weight set OIML R111 E2	Certificate No.M2308197S ,E2(Traceable to SI unit through TCS)	23 Aug 2025

Adjustment Status

The measuring device was internally adjusted before the calibration.

Environmental and measuring conditions

Date of calibration	20 Feb 2025
Temperature at place of calibration | Temp. diff. $T_{weights}$ - T_{place}	24.7 °C | 0.3 K
Measuring conditions	The installation site is suitable. The device was levelled. Balance was loaded up to Max before test.
Comments	Humidity 62.3 %RH.

Measurement results | Measurement uncertainties

Repeatability

Test load (nominal): 10 g | 200 g

	10 g	200 g
1	10.0000 g	200.0000 g
2	10.0000 g	200.0001 g
3	9.9999 g	200.0000 g
4	10.0000 g	200.0000 g
5	10.0000 g	200.0001 g
6	9.9999 g	200.0000 g
7	10.0000 g	200.0000 g
8	10.0000 g	200.0000 g
9	10.0000 g	200.0000 g
10	10.0000 g	200.0001 g
	s = 0.00004 g	s = 0.00005 g

Eccentricity

Test load (nominal):	**100 g**
Center	100.0000 g
Front left	100.0000 g
Back left	100.0001 g
Back right	99.9999 g
Front right	99.9999 g
Maximum deviation from centric loading indication $\lvert\Delta I_{ecc}\rvert_{max}$ = 0.0001 g	

Error of indication

Testload L	Indication I	Error E	Expansion factor k	Uncertainty $U(E)$	Uncertainty relative $U_{rel}(E)$
0.0100 g	0.0100 g	0.0000 g	2.00	0.00012 g	1.2 %
0.1000 g	0.1000 g	0.0000 g	2.00	0.00013 g	0.13 %
0.5000 g	0.5000 g	0.0000 g	2.00	0.00013 g	0.026 %
1.0000 g	1.0000 g	0.0000 g	2.00	0.00013 g	0.013 %
5.0000 g	5.0000 g	0.0000 g	2.00	0.00013 g	0.0026 %
10.0000 g	10.0000 g	0.0000 g	2.00	0.00013 g	0.0013 %
20.0000 g	20.0000 g	0.0000 g	2.00	0.00014 g	0.00068 %
50.0000 g	50.0000 g	0.0000 g	2.00	0.00015 g	0.00029 %
100.0000 g	100.0001 g	0.0001 g	2.00	0.00018 g	0.00018 %
200.0000 g	200.0000 g	0.0000 g	2.00	0.00028 g	0.00014 %
220.0000 g	220.0000 g	0.0000 g	2.00	0.00032 g	0.00015 %
Maximum error of indication		$\lvert E\rvert_{max}$ = 0.0001 g			

$U_{rel}(E)$ is the quotient of $U(E)$ and test load L. The uncertainty of measurement $U(E)$ is valid only if error E is considered. You will find reference notes on the uncertainty of measurement in use under: Appendix to the calibration certificate | Interpretation of measurement results.
Reference note: The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the documented Expansion factor, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

End of calibration certificate


Uncertainty of measurement in use

Device adjusted before measurement	Yes
Temperature deviation considered	1.5 K (isoCAL active)
Temperature coefficient considered	$1 \cdot 10^{-6}$/K
Uncertainty of the weighing result $U_{gl}(W)$	**$U_{gl}(W) = 0.00013\ g + 3.42 \cdot 10^{-6} \cdot R$**

Reference note: The current uncertainty of measurement is calculated by entering of the reading *R* into this formula. In relation to this, there is no need for a correction of the indication error. The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied with an Expansion factor of 2, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

Indication in % from max load	Net indication R	Uncertainty $U_{gl}(W)$	Uncertainty relative $U_{gl}(W)_{rel}$
1 %	2.2000 g	0.00014 g	0.0063 %
25 %	55.0000 g	0.00032 g	0.00058 %
50 %	110.0000 g	0.00051 g	0.00046 %
75 %	165.0000 g	0.00069 g	0.00042 %
100 %	220.0000 g	0.00088 g	0.00040 %

Graphic realization of the relative uncertainty of measurement | process accuracy

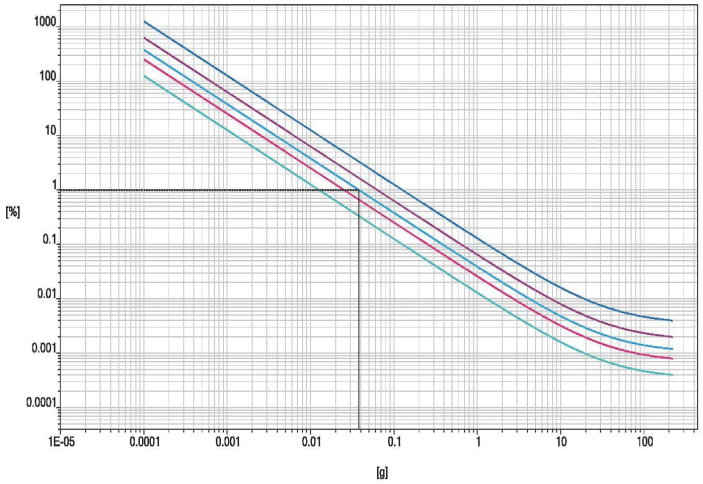

Safety factor
10
5
3
2
1

Displayed example

Process accuracy	1.00 %
Safety factor	3
Minimum sample weight	0.0380 g

SARTORIUS

Accredited by

NSC-TISI-TIS 17025
Calibration 0426

NSC-TISI-TIS 17025
CALIBRATION 0426

Calibration certificate

Calibration Certificate No. 26BCI0066

Object	Electronic non-automatic weighing instrument
Manufacturer	Sartorius
Type	MSU224S-100-DU
Serial | QM Ident. no.	31709552 | RYG_EN0003
Customer	ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
	616/10 Moo 5 T.Maenamkoo, A.Pluak Daeng, Rayong 21140, Thailand.
Order no.	278579
Number of pages	4
Date of calibration	03 Feb 2026

This calibration certificate documents the traceability to national standards.

Uncertainties of measurements are taken into account when only statements of compliance are made.

This certificate was prepared by Sartorius Corporation in accordance to the current ISO/IEC 17025:2017 standard and Sartorius Work Instruction (Method) SOP WI 08.

This certificate relate and apply this equipment only.

REVIEW BY ThanitaK.

APPROVED BY D Khumon.

NEXT CAL DATE 03/02/27

This calibration certificate may not be reproduced other than in full except with the permission of NSC-TISI-TIS-17025 and the issuing laboratory. Calibration certificates without signature are not valid.

The user is obliged to have the object recalibrated at appropriate intervals.

Date of issue	Approval of the Calibration Certificate	Person in charge
03 Feb 2026	Mr. Chonchai Inthana	Chonchai Inthana

Calibration object

Single range instrument

Model	MSU224S-100-DU
Serial Number	31709552
QM Ident. no | Inventory no.	RYG_EN0003 | ---

Maximum capacity (Max. load)	220.0000 g
Measured up to	220.0000 g
Scale interval	0.0001 g

Place of calibration

Address	According to page 1
Department | Cost center	Laboratory Department. | —
Building | Floor	— | 1st Floor.
Room	Balance Room.
Maximum temperature variation at place of calibration	5 K

Calibration procedure

EURAMET Calibration Guide No. 18, Version 4.0 (11/2015) - Guidelines on the Calibration of Non-Automatic Weighing Instruments

Test equipment

Test equipment type	Test equipment ID	Valid until
Thermometer	Testo 174H H/T250743 (Traceable to Si unit through ENTECH)	18 Nov 2026
Test weight set OIML R111 E2	Certificate No.M2508149S ,E2(Traceable to SI unit through TCS)	19 Aug 2027

Adjustment Status

The measuring device was internally adjusted before the calibration.

Environmental and measuring conditions

Date of calibration	03 Feb 2026
Temperature at place of calibration | Temp. diff. $T_{weights}$ - T_{place}	24.5 °C | 0.5 K
Measuring conditions	The installation site is suitable. The device is level. Balance was loaded up to Max before test.
Comments	Humidity 52.0 %RH.

Measurement results | Measurement uncertainties

Repeatability

Test load (nominal): 10 g | 200 g

	10 g	200 g
1	10.0000 g	200.0000 g
2	10.0000 g	200.0001 g
3	10.0000 g	200.0001 g
4	10.0001 g	200.0001 g
5	10.0000 g	200.0001 g
6	10.0000 g	200.0000 g
7	10.0000 g	200.0000 g
8	10.0000 g	200.0000 g
9	10.0000 g	200.0000 g
10	10.0000 g	200.0000 g
	s = 0.00003 g	s = 0.00005 g

Eccentricity

Test load (nominal):	**100 g**
Center	100.0000 g
Front left	100.0000 g
Back left	99.9999 g
Back right	100.0000 g
Front right	100.0000 g
Maximum deviation from centric loading indication $\lvert\Delta I_{ecc}\rvert_{max}$ = 0.0001 g	

Error of indication

Testload L	Indication I	Error E	Expansion factor k	Uncertainty $U(E)$	Uncertainty relative $U_{rel}(E)$
0.0100 g	0.0100 g	0.0000 g	2.00	0.00010 g	1.0 %
0.1000 g	0.1000 g	0.0000 g	2.00	0.00013 g	0.13 %
0.5000 g	0.5000 g	0.0000 g	2.00	0.00013 g	0.027 %
1.0000 g	1.0000 g	0.0000 g	2.00	0.00013 g	0.013 %
5.0000 g	5.0000 g	0.0000 g	2.00	0.00014 g	0.0027 %
10.0000 g	10.0000 g	0.0000 g	2.00	0.00014 g	0.0014 %
20.0000 g	20.0000 g	0.0000 g	2.00	0.00014 g	0.00071 %
50.0000 g	50.0001 g	0.0001 g	2.00	0.00015 g	0.00030 %
100.0000 g	100.0000 g	0.0000 g	2.00	0.00018 g	0.00018 %
200.0000 g	200.0000 g	0.0000 g	2.00	0.00028 g	0.00014 %
220.0000 g	220.0000 g	0.0000 g	2.00	0.00032 g	0.00015 %
Maximum error of indication		$\lvert E\rvert_{max}$ = 0.0001 g			

$U_{rel}(E)$ is the quotient of $U(E)$ and test load L. The uncertainty of measurement $U(E)$ is valid only if error E is considered. You will find reference notes on the uncertainty of measurement in use under: Appendix to the calibration certificate | Interpretation of measurement results.
Reference note: The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the documented Expansion factor, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

End of calibration certificate


Uncertainty of measurement in use

Device adjusted before measurement	Yes
Temperature deviation considered	1.5 K (isoCAL active)
Temperature coefficient considered	$1 \cdot 10^{-6}$/K
Uncertainty of the weighing result $U_{gl}(W)$	**$U_{gl}(W) = 0.00013\ g + 3.65 \cdot 10^{-6} \cdot R$**

Reference note: The current uncertainty of measurement is calculated by entering of the reading *R* into this formula. In relation to this, there is no need for a correction of the indication error. The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied with an Expansion factor of 2, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

Indication in % from max load	Net indication R	Uncertainty $U_{gl}(W)$	Uncertainty relative $U_{gl}(W)_{rel}$
1 %	2.2000 g	0.00014 g	0.0063 %
25 %	55.0000 g	0.00033 g	0.00060 %
50 %	110.0000 g	0.00053 g	0.00048 %
75 %	165.0000 g	0.00073 g	0.00044 %
100 %	220.0000 g	0.00093 g	0.00042 %

Graphic realization of the relative uncertainty of measurement | process accuracy

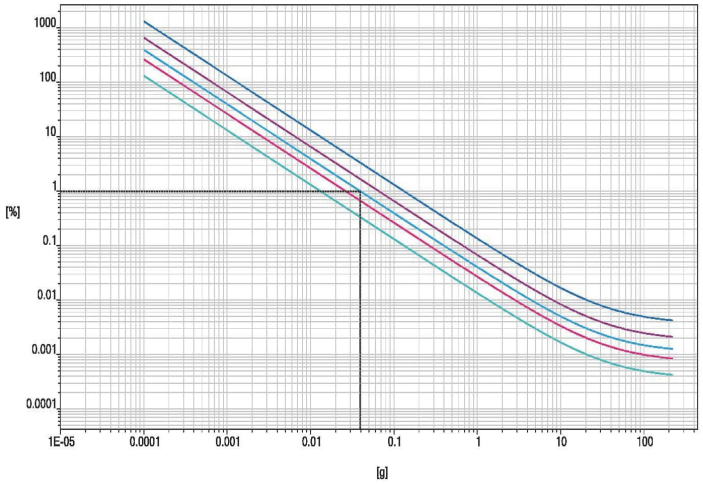

Safety factor
10
5
3
2
1

Displayed example

Process accuracy	1.00 %
Safety factor	3
Minimum sample weight	0.0395 g

SCG

Metrology Center
SCI ECO Services Company Limited
51 Moo 8, Tubkwang, Kaeng Khoi, Saraburi, Thailand 18260
Bangkok Tel : +668 9205 6851 , +669 81924 0059
Saraburi Tel : +669 8247 2360
Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

NSC-TISI-TIS 17025
CALIBRATION 0244

Certificate No. T252169

Page 1 of 3

Certificate of Calibration

Equipment : **Liquid Bath (Water)**

Manufacturer : **Memmert**

Model : **WNE29**

Serial No. : **L623.0105**

Customer Code : **RYG_EN0220**

ID No. : **T5650A5**

Customer : **ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)**
616/10 Moo 5 T.Maenamkoo,
A.Pluakdaeng, Rayong 21140

Customer Location : **Wet Chemistry Lab**

Date of Receipt : **19 November 2025**

Calibrated By : **Sujjar Naknakred (Site Calibration Manager)**

Approved By : _____ / **Boonchai Suriyawong (Site Calibration Manager)**

Date of Issue : 01 DEC 2025

REVIEW BY Thanitall.
APPROVED BY D. Suri
NEXT CAL. DATE 27/11/26

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Certificate No. T252169

Calibration Report

Equipment : **Liquid Bath (Water)**
Date of Calibration : **27 November 2025**
Environment : **Temperature : 25.5-25.7 °C**
Line Voltage : 221.8-225.5 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert five resistance thermometer detectors into its water bath , the other one thermocouple type T use for ambient temperature measurement . The calibration was done in according to WI-T36 (based on ASTM E715-80 (Reapproved 2022)).
   All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .
2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
RTD	100 OHM	M18 (CH1-CH5)	T251758	17 October 2026
DATA LOGGER	34970A	T261	T251758	17 October 2026


3. This certificate is traceable to :
   National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)
4. Condition of calibrated item : good
   Equipment Description :
   Time Constant 1 Hour 3 Minute At 63 °C
5. Adjustment :
   (X) without adjustment ( ) after adjustment

Approved By.

SCG
Metrology Center
SCI ECO Services Company Limited
51 Moo 8, Tubkwang, Kaeng Khoi, Saraburi, Thailand 18260
NSC-TISI-TIS 17025
CALIBRATION 0244

Certificate No. T252169

Calibration Report

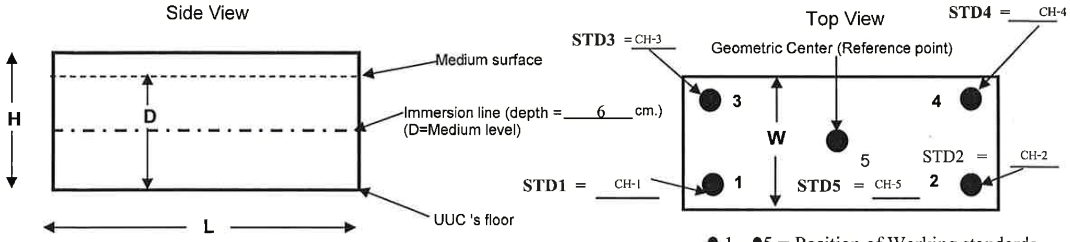

● 1~ ●5 = Position of Working standards

- D = Medium level : 12 cm. Working space dimension : 59 × 35 × 14 (WxLxH)
- UUC 's medium : Water
- Working standards are located at 2.5 cm. away from each coner and walls.

Measurement Results:

	Average Standard Reading at each position (°C)				
Calibration Point	**CH-1**	**CH-2**	**CH-3**	**CH-4**	**CH-5**
63	62.93	63.13	62.94	63.10	63.09
85	85.15	85.33	85.21	85.43	85.20

Liquid Bath (Water)			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (±°C)	Uniformity (±°C)	Uncertainty (±°C)	Coverage Factor *k*
	Min , Max	Average					
63.0	62.9 , 63.1	63.0	63.04	0.08	0.17	0.27	2.06
85.0	84.8 , 85.2	85.0	85.26	0.13	0.24	0.43	2.23

*** The quoted uncertainty exclude "uniformity"**
The calibration result apply only the above calibrated item.
The result of test was found accurate as shown on date and place of test only.
The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

End of Certificate.

Approved By.

SARTORIUS

Accredited by

NSC-TISI-TIS 17025
Calibration 0426

NSC-TISI-TIS 17025
CALIBRATION 0426

Calibration certificate

Calibration Certificate No. 25BKL0002

Object	Electronic non-automatic weighing instrument
Manufacturer	Sartorius
Type	MCE224S-2S00-U
Serial | QM Ident. no.	38101399 | RYG_EN0163
Customer	ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch) 616/10 Moo 5 T.Maenam Khu, A.Pluak Daeng, Rayong 21140, Thailand.
Order no.	2230
Number of pages	4
Date of calibration	20 Feb 2025

This calibration certificate documents the traceability to national standards.

Uncertainties of measurements are taken into account when only statements of compliance are made.

This certificate was prepared by Sartorius Corporation in accordance to the current ISO/IEC 17025:2017 standard and Sartorius Work Instruction (Method) SOP WI 08.

This certificate relate and apply this equipment only.

REVIEW BY Thanitak.

APPROVED BY D.Chumou.

NEXT CAL DATE 20/02/26

This calibration certificate may not be reproduced other than in full except with the permission of NSC-TISI-TIS-17025 and the issuing laboratory. Calibration certificates without signature are not valid.

The user is obliged to have the object recalibrated at appropriate intervals.

Date	Approval of the Calibration Certificate	Person in charge
06 Mar 2025	Mr. Chonchai Inthana	Kachen Lalee

Calibration object

Single range instrument

Model	MCE224S-2S00-U
Serial Number	38101399
QM Ident. no | Inventory no.	RYG_EN0163 | ---

Maximum capacity (Max. load)	220.0000 g
Measured range	220.0000 g
Scale interval	0.0001 g

Place of calibration

Address	According to page 1
Department | Cost center	Laboratory Department. | —
Building | Floor	— | 1st Floor.
Room	Balance Room.
Maximum temperature variation at place of calibration	5 K

Calibration procedure

EURAMET cg-18, V4.0 - Guidelines on the Calibration of Non-Automatic Weighing Instruments

Test equipment

Test equipment type	Test equipment ID	Valid until
Thermometer	MHB-382SD s/nB011342 Traceable to SI unit through DKSH	21 Aug 2025
Test weight set OIML R111 E2	Certificate No.M2308197S ,E2(Traceable to SI unit through TCS)	23 Aug 2025

Adjustment Status

The measuring device was internally adjusted before the calibration.

Environmental and measuring conditions

Date of calibration	20 Feb 2025
Temperature at place of calibration | Temp. diff. $T_{weights}$ - T_{place}	24.4 °C | 0.6 K
Measuring conditions	The installation site is suitable. The device was levelled. Balance was loaded up to Max before test.
Comments	Humidity 58.0 %RH.

Measurement results | Measurement uncertainties

Repeatability

Test load (nominal): 10 g | 200 g

	10 g	200 g
1	10.0000 g	200.0000 g
2	10.0000 g	200.0000 g
3	10.0000 g	200.0001 g
4	9.9999 g	200.0000 g
5	9.9999 g	200.0000 g
6	10.0000 g	200.0001 g
7	10.0000 g	200.0000 g
8	10.0000 g	200.0000 g
9	9.9999 g	200.0001 g
10	10.0000 g	200.0000 g
	s = 0.00005 g	s = 0.00005 g

Eccentricity

Test load (nominal):	**100 g**
Center	100.0000 g
Front left	100.0000 g
Back left	100.0000 g
Back right	100.0000 g
Front right	99.9999 g

Maximum deviation from centric loading indication

$|\Delta I_{ecc}|_{max}$ = 0.0001 g

Error of indication

Testload L	Indication I	Error E	Expansion factor k	Uncertainty $U(E)$	Uncertainty relative $U_{rel}(E)$
0.0100 g	0.0100 g	0.0000 g	2.00	0.00013 g	1.3 %
0.1000 g	0.1000 g	0.0000 g	2.00	0.00013 g	0.13 %
0.5000 g	0.5000 g	0.0000 g	2.00	0.00013 g	0.026 %
1.0000 g	1.0000 g	0.0000 g	2.00	0.00013 g	0.013 %
5.0000 g	5.0000 g	0.0000 g	2.00	0.00013 g	0.0026 %
10.0000 g	9.9999 g	-0.0001 g	2.00	0.00013 g	0.0013 %
20.0000 g	20.0000 g	0.0000 g	2.00	0.00014 g	0.00068 %
50.0000 g	50.0001 g	0.0001 g	2.00	0.00015 g	0.00029 %
100.0000 g	100.0000 g	0.0000 g	2.00	0.00018 g	0.00018 %
200.0000 g	200.0000 g	0.0000 g	2.00	0.00028 g	0.00014 %
220.0000 g	220.0000 g	0.0000 g	2.00	0.00032 g	0.00015 %
Maximum error of indication		$\|E\|_{max}$ = 0.0001 g			

$U_{rel}(E)$ is the quotient of $U(E)$ and test load L. The uncertainty of measurement $U(E)$ is valid only if error E is considered. You will find reference notes on the uncertainty of measurement in use under: Appendix to the calibration certificate | Interpretation of measurement results.
Reference note: The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the documented Expansion factor, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

End of calibration certificate


Uncertainty of measurement in use

Device adjusted before measurement	Yes
Temperature deviation considered	1.5 K (isoCAL active)
Temperature coefficient considered	1 · 10^{-6}/K
Uncertainty of the weighing result $U_{gl}(W)$	**$U_{gl}(W)$ = 0.00013 g + 1.16 · 10^{-5} · R**

Reference note: The current uncertainty of measurement is calculated by entering of the reading R into this formula. In relation to this, there is no need for a correction of the indication error. The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied with an Expansion factor of 2, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

Indication in % from max load	Net indication R	Uncertainty $U_{gl}(W)$	Uncertainty relative $U_{gl}(W)_{rel}$
1 %	2.2000 g	0.00016 g	0.0071 %
25 %	55.0000 g	0.00077 g	0.0014 %
50 %	110.0000 g	0.0014 g	0.0013 %
75 %	165.0000 g	0.0020 g	0.0012 %
100 %	220.0000 g	0.0027 g	0.0012 %

Graphic realization of the relative uncertainty of measurement | process accuracy

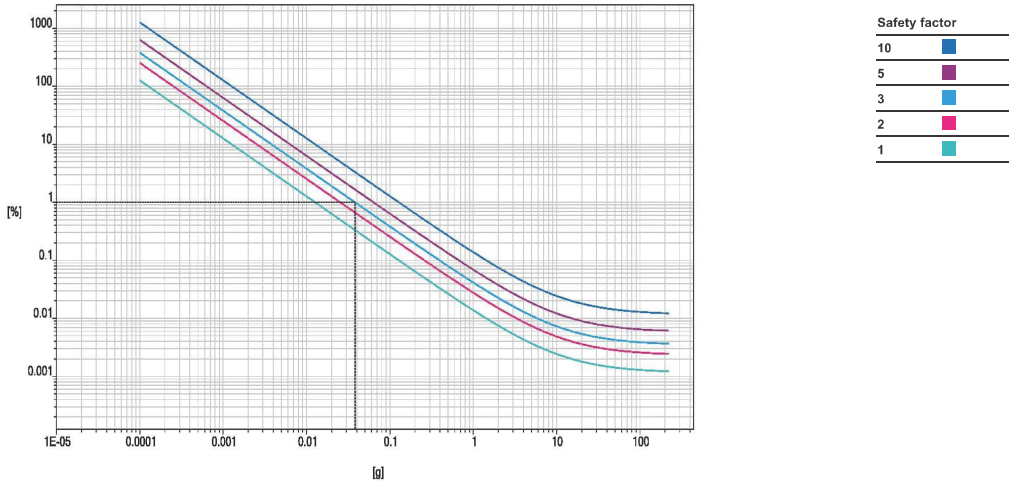

Displayed example

Process accuracy	1.00 %
Safety factor	3
Minimum sample weight	0.0381 g

SARTORIUS

Accredited by

NSC-TISI-TIS 17025
Calibration 0426

NSC-TISI-TIS 17025
CALIBRATION 0426

Calibration certificate

Calibration Certificate No. 26BCI0064

Object	Electronic non-automatic weighing instrument
Manufacturer	Sartorius
Type	MCE224S-2S00-U
Serial | QM Ident. no.	38101399 | RYG_EN0163
Customer	ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch) 616/10 Moo 5 T.Maenamkoo, A.Pluak Daeng, Rayong 21140, Thailand.
Order no.	278579
Number of pages	4
Date of calibration	03 Feb 2026

This calibration certificate documents the traceability to national standards.

Uncertainties of measurements are taken into account when only statements of compliance are made.

This certificate was prepared by Sartorius Corporation in accordance to the current ISO/IEC 17025:2017 standard and Sartorius Work Instruction (Method) SOP WI 08.

This certificate relate and apply this equipment only.

REVIEW BY ..... Thanitak.

APPROVED BY..... D.Thanon.

NEXT CAL DATE..... 03/02/27

This calibration certificate may not be reproduced other than in full except with the permission of NSC-TISI-TIS-17025 and the issuing laboratory. Calibration certificates without signature are not valid.

The user is obliged to have the object recalibrated at appropriate intervals.

Date of issue	Approval of the Calibration Certificate	Person in charge
03 Feb 2026	Mr. Chonchai Inthana	Chonchai Inthana

Calibration object

Single range instrument

Model	MCE224S-2S00-U
Serial Number	38101399
QM Ident. no | Inventory no.	RYG_EN0163 | ---

Maximum capacity (Max. load)	220.0000 g
Measured up to	220.0000 g
Scale interval	0.0001 g

Place of calibration

Address	According to page 1
Department | Cost center	Laboratory Department. | ---
Building | Floor	--- | 1st Floor.
Room	Balance Room.
Maximum temperature variation at place of calibration	5 K

Calibration procedure

EURAMET Calibration Guide No. 18, Version 4.0 (11/2015) - Guidelines on the Calibration of Non-Automatic Weighing Instruments

Test equipment

Test equipment type	Test equipment ID	Valid until
Thermometer	Testo 174H H/T250743 (Traceable to Si unit through ENTECH)	18 Nov 2026
Test weight set OIML R111 E2	Certificate No.M2508149S ,E2(Traceable to SI unit through TCS)	19 Aug 2027

Adjustment Status

The measuring device was internally adjusted before the calibration.

Environmental and measuring conditions

Date of calibration	03 Feb 2026
Temperature at place of calibration | Temp. diff. $T_{weights}$ - T_{place}	25 °C | 0.5 K
Measuring conditions	The installation site is suitable. The device is level. Balance was loaded up to Max before test.
Comments	Humidity 49.0 %RH.

Measurement results | Measurement uncertainties

Repeatability

Test load (nominal): 10 g | 200 g		
	10 g	**200 g**
1	10.0000 g	200.0000 g
2	10.0000 g	199.9999 g
3	10.0000 g	200.0000 g
4	10.0000 g	200.0001 g
5	9.9999 g	199.9999 g
6	10.0000 g	200.0000 g
7	10.0000 g	199.9999 g
8	10.0000 g	200.0000 g
9	9.9999 g	200.0001 g
10	10.0000 g	200.0000 g
	s = 0.00004 g	s = 0.00007 g

Eccentricity

Test load (nominal):	**100 g**
Center	100.0001 g
Front left	100.0002 g
Back left	100.0002 g
Back right	100.0000 g
Front right	100.0000 g
Maximum deviation from centric loading indication $\lvert\Delta I_{ecc}\rvert_{max}$ = 0.0001 g	

Error of indication

Testload L	**Indication** I	**Error** E	**Expansion factor** k	**Uncertainty** $U(E)$	**Uncertainty relative** $U_{rel}(E)$
0.0100 g	0.0100 g	0.0000 g	2.00	0.00012 g	1.2 %
0.1000 g	0.1000 g	0.0000 g	2.00	0.00017 g	0.17 %
0.5000 g	0.5000 g	0.0000 g	2.00	0.00017 g	0.034 %
1.0000 g	1.0000 g	0.0000 g	2.00	0.00017 g	0.017 %
5.0000 g	5.0000 g	0.0000 g	2.00	0.00017 g	0.0034 %
10.0000 g	10.0000 g	0.0000 g	2.00	0.00017 g	0.0017 %
20.0000 g	20.0000 g	0.0000 g	2.00	0.00018 g	0.00088 %
50.0000 g	50.0000 g	0.0000 g	2.00	0.00018 g	0.00037 %
100.0000 g	100.0001 g	0.0001 g	2.00	0.00021 g	0.00021 %
200.0000 g	200.0000 g	0.0000 g	2.00	0.00030 g	0.00015 %
220.0000 g	220.0001 g	0.0001 g	2.00	0.00034 g	0.00015 %
Maximum error of indication		$\lvert E\rvert_{max}$ = 0.0001 g			

$U_{rel}(E)$ is the quotient of $U(E)$ and test load L. The uncertainty of measurement $U(E)$ is valid only if error E is considered. You will find reference notes on the uncertainty of measurement in use under: Appendix to the calibration certificate | Interpretation of measurement results.
Reference note: The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the documented Expansion factor, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

End of calibration certificate


Uncertainty of measurement in use

Device adjusted before measurement	Yes
Temperature deviation considered	1.5 K (isoCAL active)
Temperature coefficient considered	1 · 10^{-6}/K
Uncertainty of the weighing result $U_{gI}(W)$	**$U_{gI}(W)$ = 0.00017 g + 4.25 · 10^{-6} · R**

Reference note: The current uncertainty of measurement is calculated by entering of the reading R into this formula. In relation to this, there is no need for a correction of the indication error. The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied with an Expansion factor of 2, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

Indication in % from max load	**Net indication** R	**Uncertainty** $U_{gI}(W)$	**Uncertainty relative** $U_{gI}(W)_{rel}$
1 %	2.2000 g	0.00018 g	0.0082 %
25 %	55.0000 g	0.00040 g	0.00073 %
50 %	110.0000 g	0.00064 g	0.00058 %
75 %	165.0000 g	0.00087 g	0.00053 %
100 %	220.0000 g	0.0011 g	0.00050 %

Graphic realization of the relative uncertainty of measurement | process accuracy

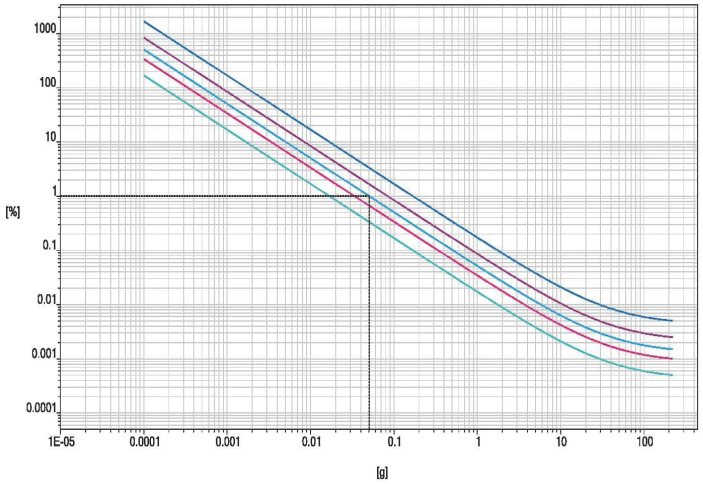

Displayed example

Process accuracy	1.00 %
Safety factor	3
Minimum sample weight	0.0507 g

SCG

Metrology Center
SCI ECO Services Company Limited
51 Moo 8, Tubkwang, Kaeng Khoi, Saraburi, Thailand 18260
Bangkok Tel : +668 9205 6851 , +669 81924 0059
Saraburi Tel : +669 8247 2360
Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

NSC-TISI-TIS 17025
CALIBRATION 0244

Certificate of Calibration

Equipment	:	**Chamber (Oven)**
Manufacturer	:	**MEMMERT**
Model	:	**UF 110**
Serial No.	:	**B416.2420**
Customer Code	:	**RYG_EN0012**
ID No.	:	**T6444A5**
Customer	:	**ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)**
		616/10 Moo 5 T.Maenamkoo,
		A.Pluakdaeng, Rayong 21140
Customer Location	:	**ENVIRONMENT LABORATORY**
Date of Receipt	:	**3 September 2025**
Calibrated By	:	**Sujjar Naknakred (Site Calibration Manager)**
Approved By	:	**Boonchai Suriyawong (Site Calibration Manager)**
Date of Issue	:	17 SEP 2025

REVIEW BY Thanitol
APPROVED BY
NEXT CAL. DATE 10/09/27

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

SCG

Metrology Center
SCI ECO Services Company Limited
51 Moo 8, Tubkwang, Kaeng Khoi, Saraburi, Thailand 18260

NSC-TISI-TIS 17025
CALIBRATION 0244

Calibration Report

Equipment	:	**Chamber (Oven)**
Date of Calibration	:	**10 September 2025**
Environment	:	**Temperature : 35.7-36.6 °C**
		Line Voltage : 226.8-233.7 V
		Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert nine resistance thermometer detectors into its chamber , the other one resistance thermometer detector use for ambient temperature measurement . The calibration was done in according to WI-T20 (based on ASTM E145-94 (Reapproved 2019) and AS2853-1986).
   All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .
2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
RTD	100 ohm	30-(CH1-10)	T242203	9 November 2025
DATA LOGGER	34970A	T47	T242203	9 November 2025

3. This certificate is traceable to :
   National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.
4. Condition of calibrated item : good
   Equipment Description :
   Time Constant 3 Hour 29 Minute At 104 °C
   Fresh Air Damper [X] Open [X] Min [ ] Medium [ ] Max
   [ ] Close
   [ ] Not Available
5. Adjustment :
   ( ) without adjustment (X) after adjustment

Approved By Boonchai

SCG


Metrology Center

SCI ECO Services Company Limited

51 Moo 8, Tubkwang, Kaeng Khoi, Saraburi, Thailand 18260

NSC-TISI-TIS 17025
CALIBRATION 0244

Calibration Report

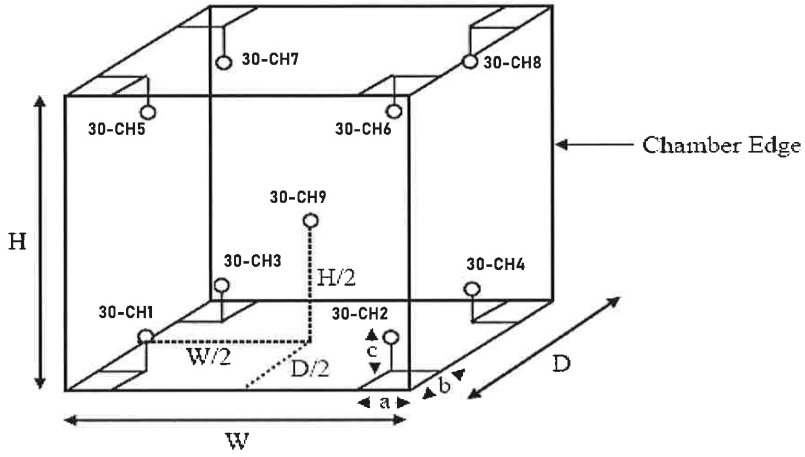

Remark : Internal Dimensions of Chamber : W (Width) = 56 cm. , H (Height) = 48 cm. and D (Depth) = 40 cm.
Size of Installed Standard sensor number 30-CH1 to number 30-CH8 : a = 5 cm. ,b = 5 cm. and c = 5 cm.
Size of Installed Standard sensor number 30-CH9 : W/2 = 56 cm./2 , H/2 = 48 cm./2 and D/2 = 40cm./2

Measurement Results

	Average Standard Reading at each position (°C)								
Calibration Point	30-CH1	30-CH2	30-CH3	30-CH4	30-CH5	30-CH6	30-CH7	30-CH8	30-CH9
104	104.02	103.70	104.01	104.16	104.11	104.08	104.01	104.33	103.61
180	180.67	178.78	180.38	179.85	179.16	180.27	180.98	181.04	179.49

Chamber (Oven)			Temperature Distribution				
Setting °C	Reading (°C)		Average (°C)	Stability (± °C)	Uniformity (°C)	Uncertainty (± °C)	Coverage Factor *k*
	Min , Max	Average					
104.0	103.9 , 104.1	104.0	104.00	0.08	0.61	0.42	2.00
180.0	179.9 , 180.1	180.0	180.07	0.21	1.51	0.52	2.00

* The quoted uncertainty exclude "uniformity"

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k which for a t-distribution, providing a level of confidence of approximately 95 % .

End of Certificate.

Approved By.

ภาคผนวก จ

สำเนาหนังสืออนุญาตขึ้นทะเบียน

ห้องปฏิบัติการวิเคราะห์เอกชน

ที่ อก ๐๓๒๐/ ๗๙๓๘

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๐๘ สิงหาคม ๒๕๖๗

เรื่อง ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน ลงวันที่ ๒๗ พฤษภาคม ๒๕๖๗

สิ่งที่ส่งมาด้วย เอกสารแนบท้ายหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด จำนวน ๓ แผ่น

ตามคำขอที่อ้างถึง บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ขอต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๓๒๓ สถานที่ตั้งเลขที่ ๖๑๖/๑๐ หมู่ที่ ๕ ตำบลแม่น้ำคู้ อำเภอปลวกแดง จังหวัดระยอง ต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน โดยมีองค์ประกอบดังนี้

ก. ผู้ควบคุมห้องปฏิบัติการวิเคราะห์เอกชน

๑) นายเดช ช้างขน	ทะเบียนเลขที่ ว-๓๒๓-ค-๐๐๐๑
๒) นางวิลาวัณย์ บริรักษ์	ทะเบียนเลขที่ ว-๓๒๓-ค-๐๐๐๒
๓) นายสุพจน์ สลามเต๊ะ	ทะเบียนเลขที่ ว-๓๒๓-ค-๐๐๐๓

ข. เจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน

๑) นายณัฐพงษ์ เพ็งชาวนา	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๐๑
๒) นางสาวกัลยทรรศน์ รักดี	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๐๒
๓) นางสาวจุฑารัตน์ ลีทองหลาง	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๐๓
๔) นางสาวจิตสุภา ประเทืองสุข	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๐๔
๕) นายสรรเสริญ คุ่ยยกสุย	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๐๕
๖) นายณัฐวุฒิ อถมพรมราช	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๐๖
๗) นายจิตกร สีวะสา	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๐๗
๘) นายสิทปวิชญ์ สุวรรณรัตน์	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๐๘
๙) นายสิทธิพันธ์ เสนาชิว	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๐๙
๑๐) นายอนุเวศน์ เตมา	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๑๐
๑๑) นายสุรวิทย์ นราพงษ์	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๑๑
๑๒) นายณัฐพล เจียงวรีวงศ์	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๑๓
๑๓) นายชานนท์ บุญชื่น	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๑๔
๑๔) นายณัฐกานต์ วงศ์อินทร์อยู่	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๑๕
๑๕) นายอานนท์ โพธิ์พระทอง	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๑๖

๑๖) นายณัชพล...

๑๖) นายณัชพล ถ้ำกลาง	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๑๗
๑๗) นายศุภณัฐ พิสัยพันธ์	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๑๘
๑๘) นายวสันต์ คินันติ	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๑๙
๑๙) นายวรัญญู ฉิมพาลี	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๒๐
๒๐) นายศุภณัฐ สกุลกิตติมศักดิ์	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๒๑
๒๑) นายเอกชัย ถันทอง	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๒๒
๒๒) นายพงษ์เทพ สิทธิเลาะ	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๒๓
๒๓) นายทินกร กุมภาษี	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๒๔
๒๔) นางสาวนันทิยา เบญจขันธ์	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๒๕
๒๕) นายสิทธิชัย ยันพิมาย	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๒๖
๒๖) นางสาวปภาณิน หลอดทอง	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๒๗
๒๗) นางสาวพจนา สีดา	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๒๘
๒๘) นางสาวธนิตา กุลศิริวงศ์	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๒๙
๒๙) นายพิทยา ทองแตง	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๓๐
๓๐) นางสาวชลธิชา สุบงกช	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๓๑
๓๑) ว่าที่ร้อยตรี รณชัย ม่วงมา	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๓๒
๓๒) นายวราวุฒิ พับพา	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๓๓
๓๓) นายศักดิ์นรินทร์ จรัสกาย	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๓๔
๓๔) นายสุรศักดิ์ สาชิน	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๓๕
๓๕) นายสถาพร ถาแก้ว	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๓๖
๓๖) นายสุทธิ์ดำรง โชคปิตินันท์	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๓๗
๓๗) นายวัลลภ ห้นไชยเนาว์	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๓๘
๓๘) นางสาววนาลี เหรียญตระกูล	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๓๙
๓๙) นายธนะสิทธิ์ วงศ์ษาไชย	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๔๐
๔๐) นายชัยนุสรณ์ เลิศนันทกุลชัย	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๔๑
๔๑) นายสัจจา เพ็ชรแสวง	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๔๒
๔๒) นายกัณฑภณ มณีสัมพันธ์	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๔๓
๔๓) นายธารินทร์ อ๊อกจินดา	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๔๔
๔๔) นายศุภชัย วงศ์สุริย์ฉาย	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๔๕
๔๕) นายไสว ต้นโพธิ์	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๔๖
๔๖) นางสาวกิตติยา สัญญาอริยาภรณ์	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๔๗
๔๖) นางสาวธิดารัตน์ ศิริมังคะโร	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๔๘
๔๗) นายพิพัฒน์ นิภัทร์เศรษฐ์	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๔๙
๔๘) นายศิริวิทย์ เรืองสม	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๕๐
๔๙) นายปาราเมศ สัตยาคุณ	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๕๑
๕๐) นายนฤนาท ธรรมสะโร	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๕๒
๕๑) นางสาวศุภรัตน์ โสจันทร์	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๕๓

๕๒) นายพชรกร...

๕๒) นายพชรกร เจิ้งเจริญ ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๕๔
๕๓) นายทิวากร เชื้อมาก ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๕๕
๕๔) นายอนุรักษ์ ทองขจรศักดา ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๕๖
๕๕) นายอภิชาติ วิลาศ ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๕๗
๕๖) นายจรัสระวี ศรีรักษา ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๕๘
๕๘) นายประสานมิตร เขื่อนเพชร ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๕๙
๕๙) นายภานุวัฒน์ วังบง ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๖๐
๖๐) นายสันติ ชัยชนะ ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๖๑
๖๑) นายทินกร กุลชาติ ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๖๒

ค. ขอบข่ายชนิดสารมลพิษที่ได้รับขึ้นทะเบียนให้วิเคราะห์ในน้ำเสีย น้ำใต้ดิน อากาศเสีย ตามสิ่งที่ส่งมาด้วย

หนังสือฉบับนี้จะหมดอายุในวันที่ ๒๘ มิถุนายน ๒๕๗๑ หากประสงค์จะต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ให้ยื่นคำขอต่ออายุพร้อมเอกสารประกอบคำขอต่อกรมโรงงานอุตสาหกรรมภายใน ๖๐ วัน ก่อนวันสิ้นอายุของหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายพรยศ กลั่นกรอง)
รองอธิบดี ปฏิบัติราชการแทน
อธิบดีกรมโรงงานอุตสาหกรรม

ศูนย์วิจัยและเตือนภัยมลพิษโรงงานภาคตะวันออก
โทร. ๐ ๓๓๑๓ ๖๐๕๙ ต่อ ๕๐๐๑-๒
ไปรษณีย์อิเล็กทรอนิกส์ eirw@diw.mail.go.th

เอกสารแนบท้ายหนังสือเปลี่ยนแปลงสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด เลขทะเบียน ว-๓๒๓
ที่ อก ๐๓๒๐/ ๗ ๙ ๓ ๘ ลงวันที่ ๐ ๘ สิงหาคม ๒๕๖๗

ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๒๔ รายการ

น้ำเสีย จำนวน 14 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Biochemical Oxygen Demand	1) 5-Day BOD Test, Membrane Electrode Method[2]
		2) 5-Day BOD Test, Azide Modification Method[2]
2	Chemical Oxygen Demand	1) Open Reflux, Titrimetric Method[2]
		2) Closed Reflux, Colorimetric Method[2]
		3) Closed Reflux, Titrimetric Method[2]
3	Color	ADMI Weighted-Ordinate Spectrophotometric Method[2]
4	Cyanide	Distillation, Colorimetric Method[2]
5	Formaldehyde	Distillation, Colorimetric Method[1]
6	Free Chlorine	DPD Ferrous Titrimetric Method[2]
7	Oil and Grease	Liquid-Liquid, Partition-Gravimetric Method[2]
8	pH	Electrometric Method[2]
9	Phenols	1) Distillation, Chloroform Extraction Method[2]
		2) Distillation, Direct Photometric Method[2]
10	Sulfide	ZnS Precipitation, Iodometric Method[2]
11	Temperature	Field Method[2]
12	Total Dissolved Solids	Dried at 180 ^{o}C [2]
13	Total Kjeldahl Nitrogen	Semi-Macro Kjeldahl Method[2]
14	Total Suspended Solids	Dried at 103-105 ^{o}C[2]

น้ำใต้ดิน จำนวน 3 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Cyanide	Distillation, Colorimetric Method[2]
2	pH	Electrometric Method[2]
3	Phenols	Distillation, Direct Photometric Method[2]

อากาศเสีย...

อากาศเสีย (ปล่องระบาย) จำนวน 7 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Carbon Monoxide	1) Sampling Bag, Non-Dispersive Infrared Method[5] 2) Instrumental Analyzer Method[9]
2	Hydrogen Sulfide	Absorption Sampling, Iodometric Method[5]
3	Opacity	Ringelmann's Method[3,4]
4	Oxide of Nitrogen	1) Absorption Sampling, Phenoldisulfonic Acid Method[8] 2) Instrumental Analyzer Method[10]
5	Sulfur Dioxide	1) Absorption Sampling, Barium-Thorin Titrimetric Acid Method[5] 2) Instrumental Analyzer Method[11]
6	Sulfuric Acid	Isokinetic Sampling, Barium – Titrimetric Method[6]
7	Total Suspended Particulate	Isokinetic Sampling, Gravimetric Method[7]

เอกสารอ้างอิง

1. ธงชัย พรรณสวัสดิ์ และวิบูลย์ลักษณ์ วิสุทธิศักดิ์, บรรณาธิการ. (2547) คู่มือวิเคราะห์น้ำเสีย. พิมพ์ครั้งที่ 4. กรุงเทพฯ: สมาคมวิศวกรรมสิ่งแวดล้อมแห่งประเทศไทย.

2. APHA, AWWA, WEF. **Standard Methods for the Examination of Water and Wastewater**. 24th ed. Washington, DC : APHA, 2023

3. กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2549. เรื่อง กำหนดค่าปริมาณเขม่าควันที่เจือปนในอากาศที่ระบายออกจากปล่องของหม้อน้ำโรงสีข้าวที่ใช้แกลบเป็นเชื้อเพลิง. **ราชกิจจานุเบกษา**. 4 ธันวาคม 2549. เล่มที่ 123 ตอนพิเศษ 125ง

4. กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2549. เรื่อง กำหนดค่าปริมาณเขม่าควันที่เจือปนในอากาศที่ระบายออกจากปล่องของหม้อน้ำของโรงงาน. **ราชกิจจานุเบกษา**. 4 ธันวาคม 2549. เล่มที่ 123 ตอนพิเศษ 125ง

5. United States Environmental Protection Agency. **Standards of Performance for New Stationary Sources**. 40 CFR 60. Appendix A, 2017.

6. United States Environmental Protection Agency. **Standards of Performance for New Stationary Sources**. 40 CFR 60. Appendix A, 2019.

7.United States...

7. United States Environmental Protection Agency. **Standards of Performance for New Stationary Sources.** 40 CFR 60. Appendix A, 2020.

8. United States Environmental Protection Agency. **Standards of Performance for New Stationary Sources**. 40 CFR 60. Appendix A, 2023.

9. United States Environmental Protection Agency. **Determination of Carbon Monoxide Emission from Stationary Sources; Instrumental Analyzer Procedure.** 40 CFR 60. Appendix A Method 10, 2017.

10. United States Environmental Protection Agency. **Determination of Oxide of Nitrogen Emission from Stationary Sources; Instrumental Analyzer Procedure.** 40 CFR 60. Appendix A Method 7E, 2023.

11. United States Environmental Protection Agency. **Determination of Sulfur dioxide Emission from Stationary Sources; Instrumental Analyzer Procedure.** 40 CFR 60. Appendix A Method 6C, 2017.

ที่ อก ๐๓๒๐/ ๑๐๐๙๙

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๐๔ ตุลาคม ๒๕๖๗

เรื่อง แก้ไขรายชื่อเจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง หนังสือ บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด เลขที่ Env 2024/005
ลงวันที่ ๓๐ สิงหาคม ๒๕๖๗

ตามหนังสือที่อ้างถึง บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๓๒๓ สถานที่ตั้งเลขที่ ๖๑๖/๑๐ หมู่ที่ ๕ ตำบลแม่น้ำคู้ อำเภอปลวกแดง จังหวัดระยอง ขอแก้ไขชื่อเจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน เนื่องจากมีความคลาดเคลื่อน ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรม ได้รับทราบและดำเนินการแก้ไขรายชื่อเจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน จำนวน ๕ ราย ตามที่แจ้งเรียบร้อยแล้ว เป็นดังนี้

ลำดับที่ ๒๗ นางพจนา สีดา
ลำดับที่ ๒๘ นางสาวธนิตา กุลสุริวงศ์
ลำดับที่ ๓๐ นางชลธิชา สุบงกช
ลำดับที่ ๓๖ นายสุทธิ์ดำรงค์ โชคปิตินันท์
ลำดับที่ ๔๒ นายกันตภณ มณีสัมพันธ์

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายพรยศ กลิ่นกรอง)
รองอธิบดี ปฏิบัติราชการแทน
อธิบดีกรมโรงงานอุตสาหกรรม

ศูนย์วิจัยและเตือนภัยมลพิษโรงงานภาคตะวันออก
โทร. ๐ ๓๓๑๓ ๖๐๕๙ ต่อ ๕๐๐๑-๒
ไปรษณีย์อิเล็กทรอนิกส์ eirw@diw.mail.go.th

Green Industry "อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา อุตสาหกรรมสีเขียว"

ที่ อก ๐๓๑๐(๓)/ ๔๒๔๖

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๒๐ พฤษภาคม ๒๕๖๘

เรื่อง ยกเลิกบุคลากรของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๑๐ เมษายน ๒๕๖๘

ตามคำขอที่อ้างถึง บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๓๒๓ สถานที่ตั้งเลขที่ ๖๑๖/๑๐ หมู่ที่ ๕ ตำบลแม่น้ำคู้ อำเภอปลวกแดง จังหวัดระยอง ขอยกเลิกบุคลากร ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้ยกเลิกเจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน จำนวน ๑ ราย ได้แก่ นายปาราเมศ สัตยาคุณ ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๕๑

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายประสม ดำรงพงษ์)
ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

ศูนย์วิจัยและเตือนภัยมลพิษโรงงานภาคตะวันออก
โทร. ๐ ๓๓๑๓ ๖๐๕๙ ต่อ ๕๐๐๑-๒
ไปรษณีย์อิเล็กทรอนิกส์ eirw@diw.mail.go.th

Green Industry "อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา อุตสาหกรรมสีเขียว"

ที่ อก ๐๓๑๐(๓)/ ๔๔๐๙

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๒๗ พฤษภาคม ๒๕๖๘

เรื่อง เปลี่ยนแปลงชื่อ-สกุลบุคลากรของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน ลงวันที่ ๑๕ พฤษภาคม ๒๕๖๘

ตามคำขอที่อ้างถึง บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๓๒๓ สถานที่ตั้งเลขที่ ๖๑๖/๑๐ หมู่ที่ ๕ ตำบลแม่น้ำคู้ อำเภอปลวกแดง จังหวัดระยอง ขอเปลี่ยนแปลงชื่อ-สกุลบุคลากร ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้เปลี่ยนแปลงชื่อ-สกุลบุคลากร จำนวน ๑ ราย จากนายธนะสิทธิ์ วงศ์ษาไชย เป็น นายอมลวิชญ์ วงศ์ษาไชย

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายประสม ดำรงพงษ์)
ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

ศูนย์วิจัยและเตือนภัยมลพิษโรงงานภาคตะวันออก
โทร. ๐ ๓๓๑๓ ๖๐๕๙ ต่อ ๕๐๐๑-๒
ไปรษณีย์อิเล็กทรอนิกส์ eirw@diw.mail.go.th

ที่ อก ๐๓๑๐(๓)/ ๙๗๖๔

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๐๒ ธันวาคม ๒๕๖๘

เรื่อง เปลี่ยนแปลงสารมลพิษที่วิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน ลงวันที่ ๓๑ ตุลาคม ๒๕๖๘

สิ่งที่ส่งมาด้วย เอกสารแนบท้ายหนังสือเปลี่ยนแปลงสารมลพิษที่วิเคราะห์
บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด จำนวน ๒ แผ่น

ตามคำขอที่อ้างถึง บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๓๒๓ สถานที่ตั้งเลขที่ ๖๑๖/๑๐ หมู่ที่ ๕ ตำบลแม่น้ำคู้ อำเภอปลวกแดง จังหวัดระยอง ขอเปลี่ยนแปลงสารมลพิษที่วิเคราะห์ ต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด เพิ่มขอบข่ายชนิดสารมลพิษที่วิเคราะห์ในน้ำเสีย และน้ำใต้ดิน ตามสิ่งที่ส่งมาด้วย

อนึ่ง หนังสือฉบับนี้จะสิ้นอายุพร้อมหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ในวันที่ ๒๘ มิถุนายน ๒๕๗๑

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นางสาวปัทมวรรณ คุณประเสริฐ)
ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน
ศูนย์วิจัยและเตือนภัยมลพิษโรงงานภาคตะวันออก
โทร. ๐ ๓๓๑๓ ๖๐๕๙ ต่อ ๕๐๐๑-๒
ไปรษณีย์อิเล็กทรอนิกส์ eirw@diw.mail.go.th

เอกสารแนบท้ายหนังสือเปลี่ยนแปลงสารมลพิษที่วิเคราะห์
บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด เลขทะเบียน ว-๓๒๓
ที่ อก ๐๓๑๐(๓)/ ๙๗๖๔ ลงวันที่ ๐๒ ธันวาคม ๒๕๖๘

ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๒๓ รายการ

น้ำเสีย จำนวน 13 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Arsenic	Digestion, Inductively Coupled Plasma Method
2	Barium	Digestion, Inductively Coupled Plasma Method
3	Cadmium	Digestion, Inductively Coupled Plasma Method
4	Chromium	Digestion, Inductively Coupled Plasma Method
5	Copper	Digestion, Inductively Coupled Plasma Method
6	Hexavalent Chromium	Colorimetric Method
7	Lead	Digestion, Inductively Coupled Plasma Method
8	Manganese	Digestion, Inductively Coupled Plasma Method
9	Mercury	Digestion, Cold-Vapor Atomic Absorption Spectrometric Method
10	Nickel	Digestion, Inductively Coupled Plasma Method
11	Selenium	Digestion, Inductively Coupled Plasma Method
12	Trivalent Chromium	Calculation
13	Zinc	Digestion, Inductively Coupled Plasma Method

น้ำใต้ดิน จำนวน 20 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Aluminum	Digestion, Inductively Coupled Plasma Method
2	Antimony	Digestion, Inductively Coupled Plasma Method
3	Arsenic	Digestion, Inductively Coupled Plasma Method
4	Barium	Digestion, Inductively Coupled Plasma Method
5	Beryllium	Digestion, Inductively Coupled Plasma Method
6	Cadmium	Digestion, Inductively Coupled Plasma Method
7	Chromium	Digestion, Inductively Coupled Plasma Method
8	Chromium (III)	Calculation
9	Chromium (VI)	Colorimetric Method
10	Copper	Digestion, Inductively Coupled Plasma Method

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
11	Iron	Digestion, Inductively Coupled Plasma Method
12	Lead	Digestion, Inductively Coupled Plasma Method
13	Manganese	Digestion, Inductively Coupled Plasma Method
14	Mercury	Digestion Cold-Vapor Atomic Absorption Spectrometric Method
15	Molybdenum	Digestion, Inductively Coupled Plasma Method
16	Nickel	Digestion, Inductively Coupled Plasma Method
17	Selenium	Digestion, Inductively Coupled Plasma Method
18	Silver	Digestion, Inductively Coupled Plasma Method
19	Vanadium	Digestion, Inductively Coupled Plasma Method
20	Zinc	Digestion, Inductively Coupled Plasma Method

เอกสารอ้างอิง

APHA, AWWA, WEF. **Standard Methods for the Examination of Water and Wastewater**. 24th ed. Washington, DC: APHA, 2023.

ที่ อก ๐๓๑๐(๓)/ ๑ ๗ ๗ ๘

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๐๖ มีนาคม ๒๕๖๙

เรื่อง เปลี่ยนแปลงบุคลากรของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน ลงวันที่ ๖ กุมภาพันธ์ ๒๕๖๙

ตามคำขอที่อ้างถึง บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๓๒๓ สถานที่ตั้งเลขที่ ๖๑๖/๑๐ หมู่ที่ ๕ ตำบลแม่น้ำคู้ อำเภอปลวกแดง จังหวัดระยอง ขอเปลี่ยนแปลงบุคลากร ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้เพิ่มเจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน จำนวน ๗ ราย ได้แก่

๑) นายอนวัช คงปลิก	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๖๓
๒) นายธนาธิป อิติวุตตา	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๖๔
๓) นายเฉลิมชัย บุญชุบ	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๖๕
๔) นางสาววิจิตรา งามเสงี่ยม	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๖๖
๕) นางสาวลลิตา คำสมัย	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๖๗
๖) นางสาวปทิตตา ชูตินันท์	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๖๘
๗) นายปฏิญญา ปานทองทา	ทะเบียนเลขที่ ว-๓๒๓-จ-๐๐๖๙

อนึ่ง หนังสือฉบับนี้จะสิ้นอายุพร้อมหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ในวันที่ ๒๘ มิถุนายน ๒๕๗๑

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายศิระ จันทร์เฉิด)
นักวิทยาศาสตร์เชี่ยวชาญ รักษาราชการแทน
ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน
ศูนย์วิจัยและเตือนภัยมลพิษโรงงานภาคตะวันออก
โทร. ๐ ๓๓๑๓ ๖๐๕๙ ต่อ ๕๐๐๑-๒
ไปรษณีย์อิเล็กทรอนิกส์ eirw@diw.mail.go.th

Green Industry กระทรวงอุตสาหกรรม "อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา อุตสาหกรรมสีเขียว"

ที่ อก ๐๓๑๐(๑)/ ๑ ๖ ๑ ๖ ๘

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๒๐ พฤศจิกายน ๒๕๖๖

เรื่อง ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน ลงวันที่ ๔ สิงหาคม ๒๕๖๖

สิ่งที่ส่งมาด้วย ๑. รายชื่อผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๑ แผ่น
๒. รายชื่อเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๕ แผ่น
๓. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๓๑ แผ่น

ตามหนังสือที่อ้างถึง บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ขอต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๒๐๔ สถานที่ตั้งเลขที่ ๑๐๔ ซอยพัฒนาการ ๔๐ ถนนพัฒนาการ แขวงพัฒนาการ เขตสวนหลวง กรุงเทพมหานคร ต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน โดยมีองค์ประกอบดังนี้

ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๖ ราย ตามสิ่งที่ส่งมาด้วย ๑
ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ ๑๘๑ ราย ตามสิ่งที่ส่งมาด้วย ๒
ค. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนให้วิเคราะห์ในน้ำเสีย น้ำใต้ดิน อากาศเสีย สิ่งปฏิกูล หรือวัสดุที่ไม่ใช้แล้ว และดิน ตามสิ่งที่ส่งมาด้วย ๓

หนังสือฉบับนี้จะหมดอายุในวันที่ ๒ กันยายน ๒๕๖๙ หากประสงค์จะต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ให้ยื่นคำขอต่ออายุพร้อมเอกสารประกอบคำขอต่อกรมโรงงานอุตสาหกรรม ภายใน ๓๐ วัน ก่อนวันสิ้นอายุของหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ทั้งนี้ สามารถยื่นคำขอผ่านระบบอิเล็กทรอนิกส์ได้ที่หน้าเว็บไซต์กรมโรงงานอุตสาหกรรม

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายศิระ จันทร์เฉิด)
นักวิทยาศาสตร์เชี่ยวชาญ รักษาราชการแทน
ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน
กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ
โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕
โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๙๙
ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th

Green Industry กระทรวงอุตสาหกรรม "อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา อุตสาหกรรมสีเขียว"

เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด เลขทะเบียน ว-๒๐๔
ที่ อก ๐๓๑๐(๑)/ ๑๖๑๖๘ ลงวันที่ ๒๐ พฤศจิกายน ๒๕๖๖

ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๖ ราย

๑) นางสาวยุพาพร จันทร์เปล่ง	ทะเบียนเลขที่ ว-๒๐๔-ค-๐๐๐๑
๒) นางสาวชัชนัย โกมารกุล ณ นคร	ทะเบียนเลขที่ ว-๒๐๔-ค-๐๐๐๒
๓) นายศรายุทธ จิตรานนท์	ทะเบียนเลขที่ ว-๒๐๔-ค-๐๐๐๓
๔) นางสาวกนกกร เอนก	ทะเบียนเลขที่ ว-๒๐๔-ค-๐๐๐๔
๕) นายสุริยา สอนแก้ว	ทะเบียนเลขที่ ว-๒๐๔-ค-๐๐๐๕
๖) นายวิชาญ ชุณหรัต	ทะเบียนเลขที่ ว-๒๐๔-ค-๐๐๐๖

เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด เลขทะเบียน ว-๒๐๔
ที่ อก ๐๓๑๐(๑)/ ๑๖๑๖๘ ลงวันที่ ๒๐ พฤศจิกายน ๒๕๖๖

ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๑๘๑ ราย

๑) นายกาจบัณฑิต กิตติศุภวณิชย์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๐๑
๒) นายภัทรพล สว่างใจธรรม์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๐๒
๓) นายนราธิป เทือกชัยคำ	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๐๓
๔) นายศิริโชค พงษ์ประสม	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๐๔
๕) นายณัฐวุฒิ ด้วงแพง	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๐๕
๖) นางสาวจินดา โชจุลธรรม	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๐๖
๗) นางสาวสาวิตรี น้อยเสงี่ยม	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๐๗
๘) นางสาวชณัฐกาญจน์ อิ่มชม	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๐๘
๙) นางสาวนรินทร์ สายเส็ง	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๐๙
๑๐) นางสาวนันทวดี สมบูรณ์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๑๐
๑๑) นางสาวศรัณยา เฉลิมธำรงค์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๑๑
๑๒) นางสาวธัญญธร มงคลจิรวุฒิ	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๑๒
๑๓) นางสาวศิริลักษณ์ บุนนาค	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๑๓
๑๔) นายนพพงศ์ จันทรุพันธุ์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๑๔
๑๕) นายนรเศรษฐ์ โกมาลย์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๑๕
๑๖) นายธันวา จริยา	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๑๖
๑๗) นางสาวเกศรินทร์ แก้วมั่น	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๑๗
๑๘) นางสาวสุวิมล ชัยเรืองวุฒิ	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๑๘
๑๙) นางสาวสุชาดา ธรรมถาวร	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๑๙
๒๐) นางสาวเปมิกา ชัยเดชธนกุล	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๒๐
๒๑) นางสาวศศิธร หมูสวัสดิ์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๒๑
๒๒) นางสาวเสาวลักษณ์ ภู่นภาอำพร	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๒๒
๒๓) นายอภิสิทธิ์ สิงหา	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๒๓
๒๔) นายศักดิ์สิทธิ์ ไพศาลพิสุทธิ์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๒๔
๒๕) ว่าที่ร้อยตรีหญิง พรรณิภา ขำเจริญ	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๒๕
๒๖) นางจิลดา คำภูแก้ว	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๒๖
๒๗) นางสาวอรวรรณ รักยง	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๒๗
๒๘) นางสาวนพรัตน์ แย้มกรานต์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๒๘
๒๙) นายจุลเดช วารินทร์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๒๙
๓๐) นางสาวดายุรัตน์ ร้องคำ	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๓๐
๓๑) นายพรมมี ศรีปัตเนตร	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๓๑
๓๒) นายอุทิศ อุ่นสิม	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๓๒
๓๓) ว่าที่ร้อยตรี เฉลิมเกียรติ อมรศรีเสริม	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๓๓
๓๔) นางสาววริยา สร้างนา	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๓๔
๓๕) นายอนุพงศ์ รัตนศรีประเสริฐ	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๓๕

๓๖) นางสาวจุฑารัตน์...

๓๖) นางสาวจุฑารัตน์ โอนสันเทียะ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๓๖
๓๗) นางสาวจารุวรรณ พิมพ์อภิกฤติยา ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๓๗
๓๘) นางสาวปรางค์ทิพย์ กิจไพศาลศักดิ์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๓๘
๓๙) นางสาวเตือนใจ ทางกลาง ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๓๙
๔๐) นางสาวจิราพร ศิริเวช ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๔๐
๔๑) นายวรากร ผูกรักษ์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๔๑
๔๒) นายทนง วิริยะสหกิจ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๔๒
๔๓) นายธนิต เจนจบ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๔๓
๔๔) นายคณิศร ขำเพชร ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๔๔
๔๕) นายภูวิช พรหมสะอาด ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๔๕
๔๖) นายธนเดช โภคาพิพัฒน์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๔๖
๔๗) นายชวฤทธิ์ วงษ์จันทร์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๔๗
๔๘) นายอาทิตย์ ศรีเสน ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๔๘
๔๙) นายเจษดินทร์ คงศักดิไทย ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๔๙
๕๐) นายจรัส บุญยิ่ง ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๕๐
๕๑) นายธนาณัติ เอนก ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๕๑
๕๒) นายอภิวัฒน์ ทุมหนู ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๕๒
๕๓) นางสาวสุภาขวัญ มาก ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๕๓
๕๔) นางสาวทัตพร ชวาลสมบูรณ์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๕๔
๕๕) นางสาวธิติมา บุญเพ็ง ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๕๕
๕๖) นางสาวภานุมาศ นามวัฒน์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๕๖
๕๗) นางสาวอุไรรัตน์ ทึงสร้างแป้น ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๕๗
๕๘) นายธีรวัฒน์ ปวงสุข ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๕๘
๕๙) นายอิทธิพล ยะโส ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๕๙
๖๐) นายประพจน์ วรรณชูชัย ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๐
๖๑) นายชยธร พวงทิพย์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๑
๖๒) นางสาวกนกวรรณ จันทบาล ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๒
๖๓) นายสิทธิโชค ธงเงิน ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๓
๖๔) นางศิลาวรรณ ใจบุญ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๔
๖๕) นางสาวพรรณธิดา พุ่มคง ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๕
๖๖) นายนวภัทร ศรีวิริยะ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๖
๖๗) นายสุวิชา ทองอ่อน ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๗
๖๘) นายวิญญู บุญตะนัย ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๘
๖๙) นายสมบูรณ์ บุตรจันทร์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๙
๗๐) นายวิรัตน์ ไชยนะรา ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๗๐
๗๑) นายนฤเบศน์ เพิ่มพูน ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๗๑
๗๒) นายจิรณัฐ ขาวละออ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๗๒
๗๓) นายอัสรี นามบุรี ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๗๓
๗๔) นายอัศวเรศ จ่อสาว ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๗๔

๗๕) นายประเสริฐ...

๗๕) นายประเสริฐ สุระขันธ์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๗๕
๗๖) นายนุกูล จันทร์เนียม ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๗๖
๗๗) นายพีรพงษ์ ทองคูณปรีดา ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๗๗
๗๘) นายนฤพล ทองนุช ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๗๘
๗๙) นายอนุวัฒน์ ม่วงแพร ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๗๙
๘๐) นายเจตศราวุฒิ ปัตตะมะ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๘๐
๘๑) นายกฤษณะ สายวรรณ์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๘๑
๘๒) นายพิชัย บุญยงค์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๘๒
๘๓) นายภานุพงศ์ โอมวงศ์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๘๓
๘๔) นายสามารถ คุ้มปลี ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๘๔
๘๕) นายสัญชัย โกศรีนาม ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๘๕
๘๖) นายณัฐวุฒิ ศรีประเสริฐ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๘๖
๘๗) นายชวัลธัช นาคพนม ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๘๗
๘๘) นายพงศธร ชัยทิพย์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๘๘
๘๙) นายสิทธิโชค ทาสีดา ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๘๙
๙๐) นายธนากร อินสุตา ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๙๐
๙๑) นางสาววรณิชชา ชาติวันชัย ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๙๑
๙๒) นางสาวพิมพ์ตะวัน มินากูล ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๙๒
๙๓) นางสาวเพชรัตน์ สิงห์สมบุญ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๙๓
๙๔) นางสาวชญานิน พรหมจันทร์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๙๔
๙๕) นายกีรติ ทวีราช ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๙๕
๙๖) นายจักริน หมั่นวิชา ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๙๖
๙๗) นายฉัตรชัย สุขเปีย ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๙๗
๙๘) นายณรนนท์ ต๊ะทองคำ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๙๘
๙๙) นายคุลยพล สนนอก ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๙๙
๑๐๐) นายทักษ์ดนัย อุบลศรี ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๐
๑๐๑) นายธนศวร นามะกุณณา ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๑
๑๐๒) นายธิติพงศ์ บัวแดง ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๒
๑๐๓) นายนนทชัย อุปถัมภ์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๓
๑๐๔) นายนัฐพล คุณสุทธิ์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๔
๑๐๕) นายนันทวัฒน์ สาริน ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๕
๑๐๖) นายปิยะนัฐ พลมะศรี ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๖
๑๐๗) นายพงศ์สิริ โสมเขียว ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๗
๑๐๘) นายพีรพัฒน์ กำคำ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๘
๑๐๙) นายภาณุพงศ์ มานิตย์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๙
๑๑๐) นายมงคล ผลาทิพย์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๑๐
๑๑๑) นายสิรินนท์ ทองอั้น ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๑๑
๑๑๒) นายอเนชา ทันสมัย ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๑๒
๑๑๓) นายอดิศักดิ์ ผมไผ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๑๓

๑๑๔) นายอนันตชัย...

๑๑๔) นายอนันตชัย วีสม ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๑๔
๑๑๕) นายวรวุธ ดีนัก ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๑๕
๑๑๖) นายแสงตะวัน นะตะสัต ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๑๖
๑๑๗) นายยุทธิพงศ์ รัตนะ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๑๗
๑๑๘) นายขยัณวุฒิ ไชยฮะนิจ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๑๘
๑๑๙) นายวิศรุต ศรีธรรมมา ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๑๙
๑๒๐) นายนนทกร เผือกผ่อง ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๒๐
๑๒๑) นายกำชัย สุทธะ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๒๑
๑๒๒) นางสาวณัฐภรณ์ บุญตะนัย ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๒๒
๑๒๓) นางสาวพัชรินทร์ แสนสร้อย ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๒๓
๑๒๔) นายไพรวัลย์ เปรี่ยมพิมาย ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๒๔
๑๒๕) นางสาวศุภมาศ ทองมาก ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๒๕
๑๒๖) นางสาวลลิตา จิตรสว่าง ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๒๖
๑๒๗) นางสาวชไมพร เสิกภู่เขียว ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๒๗
๑๒๘) นางสาวกฤติมาพร คำมีแก่น ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๒๘
๑๒๙) นางสาวสกุลรัตน์ ภาคภูมิ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๒๙
๑๓๐) นางสาวไพรินทร์ ศรีรูปี ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๐
๑๓๑) นางสาวทิพเนตร ผุยปัญญา ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๑
๑๓๒) นางสาวสาธิตา ปานทอง ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๒
๑๓๓) นางสาวอริสา ทองนวล ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๓
๑๓๔) นางสาวอรยา ค้าคล่อง ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๔
๑๓๕) นางสาวชุดาภรณ์ สุนทรสนาน ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๕
๑๓๖) นางสาวอัญชลี คำจันทร์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๖
๑๓๗) นายบุญฤทธิ์ เอี่ยมเทศ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๗
๑๓๘) นางสาวศุภรดา ปั้นมยุรา ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๘
๑๓๙) นางสาวพาฤดี คุณนาน ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๙
๑๔๐) นางสาวจิราเจต ฟองดา ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๔๐
๑๔๑) นางสาวอารยา มีชัย ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๔๑
๑๔๒) นางสาววิชชุตา นาคผจญ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๔๒
๑๔๓) นางสาวนันทิยา จันทะลุน ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๔๓
๑๔๔) นายกิตติพงศ์ แซ่ลี้ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๔๔
๑๔๕) นายอนุวัติ ภูถวิล ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๔๕
๑๔๖) นายธีรพล แสงทอง ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๔๖
๑๔๗) นายศักดิ์พิพัฒน์ บุญมั่น ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๔๗
๑๔๘) นายฐิติวัลค์ เอมอุไร ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๔๘
๑๔๙) นายชัยณรงค์ ศรีบุรินทร์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๔๙
๑๕๐) นางสาวอัจฉราวรรณ สวนสนอง ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๕๐
๑๕๑) นางสาวณัฐฐาพร สิงหา ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๕๑
๑๕๒) นายภีมเรศ แหยมโต ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๕๒

๑๕๓) นางสาวอุบล...

๑๕๓) นางสาวอุบล เศิกศิริ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๕๓
๑๕๔) นางสาวมโนรัตน์ ทองบุตร ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๕๔
๑๕๕) นายภาคภูมิ แทนไทย ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๕๕
๑๕๖) นางสาวสุภาณัฐ เมล์พ่วง ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๕๖
๑๕๗) นางสาวพรทิวา สาตาชนม์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๕๗
๑๕๘) นายเอกวิทย์ วันทะนา ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๕๘
๑๕๙) นายไตรมณฑล ทิพย์วรรณ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๕๙
๑๖๐) นายจิรเมธ ประเสริฐสิริพงศ์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๐
๑๖๑) นายจิรายุส เกษมสุข ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๑
๑๖๒) นายจีรศักดิ์ ศรีวิชัย ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๒
๑๖๓) นายณัฐกฤษณ์ สะพานแก้ว ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๓
๑๖๔) นายบูรณศักดิ์ ปะทิ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๔
๑๖๕) นายปัณณวิชญ์ เสมอทรัพย์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๕
๑๖๖) นายพิษณุพงษ์ ไชยา ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๖
๑๖๗) นายภัทรพงษ์ มณฑาทอง ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๗
๑๖๘) นายวสันต์ ตรีนกุล ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๘
๑๖๙) นายภาณุเดช เพชรอุด ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๙
๑๗๐) นายอนุกูล วิละแสง ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๗๐
๑๗๑) นายภัทรพงษ์ มีสุข ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๗๑
๑๗๒) นางสาวนุชรวี ลีละทีป ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๗๒
๑๗๓) นางสาวสุภาวดี โกศรีนาม ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๗๓
๑๗๔) นางสาวอรณิช เทียนดำ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๗๔
๑๗๕) นางสาวพรเพ็ญ ชอบสอน ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๗๕
๑๗๖) นางสาววันวิสา ขอนพิกุล ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๗๖
๑๗๗) นางสาวอรวรรณ เถาว์ทอง ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๗๗
๑๗๘) นางสาวอัยย์ลิณ เมอร์วิณณ์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๗๘
๑๗๙) นางสาววรวิสรา คุ่ยครอง ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๗๙
๑๘๐) นายวุฒิกร ศิริวรรณ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๘๐
๑๘๑) นางสาวจารุวรรณ กระจ่างพันธุ์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๘๑

เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด เลขทะเบียน ว-๒๐๔
ที่ อก ๐๓๑๐(๑)/ ๑๖๑๖๘ ลงวันที่ ๒๐ พฤศจิกายน ๒๕๖๖

ค. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๓๗๔ รายการ

น้ำเสีย จำนวน 60 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Aldicarb	High-Performance Liquid Chromatographic Method[4]
2	Aldicarb Sulfone	High-Performance Liquid Chromatographic Method[4]
3	Aldicarb Sulfoxide	High-Performance Liquid Chromatographic Method[4]
4	Aldrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
5	Arsenic	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
6	Barium	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
7	α-BHC	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
8	β-BHC	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
9	δ-BHC	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
10	γ-BHC	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
11	Biochemical Oxygen Demand	1) 5-Day BOD Test, Azide Modification Method[4] 2) 5-Day BOD Test, Membrane Electrode Method[4]
12	Carbaryl	High-Performance Liquid Chromatographic Method[4]
13	Carbofuran	High-Performance Liquid Chromatographic Method[4]
14	Cadmium	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
15	Chemical Oxygen Demand	1) Closed Reflux, Colorimetric Method[4] 2) Closed Reflux, Tritimetric Method[4]
16	Chlordane	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
17	Chromium	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
18	Color	ADMI Weighted-Ordinate Spectrophotometric Method[4]

19 Copper...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
19	Copper	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
20	Cyanide	Distillation, Colorimetric Method[4]
21	2,4´-DDD	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
22	4,4´-DDD	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
23	2,4´-DDE	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
24	4,4´-DDE	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
25	2,4´-DDT	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
26	4,4´-DDT	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
27	Dieldrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
28	Endosulfan Sulfate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
29	Endosulfan I	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
30	Endosulfan II	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
31	Endrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
32	Endrin Aldehyde	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
33	Formaldehyde	Distillation, Colorimetric Method[3]
34	Free Chlorine	1) DPD Ferrous Titrimetric Method[4] 2) DPD Colorimetric Method[4]
35	Heptachlor	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
36	Heptachlor Epoxide	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
37	Hexavalent Chromium	Colorimetric Method[4]
38	3-Hydroxycarbofuran	High-Performance Liquid Chromatographic Method[4]
39	Lead	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]

40 Manganese...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
40	Manganese	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
41	Mercury	1) Digestion, Cold-Vapor Atomic Absorption Spectrometric Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass spectrometric Method[4]
42	Methiocarb	High-Performance Liquid Chromatographic Method[4]
43	Methoxychlor	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
44	Methomyl	High-Performance Liquid Chromatographic Method[4]
45	Nickel	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
46	Oil & Grease	1) Liquid-Liquid, Partition-Gravimetric Method[4] 2) Soxhlet Extraction Method[4]
47	Oxamyl	High-Performance Liquid Chromatographic Method[4]
48	Propoxur	High-Performance Liquid Chromatographic Method[4]
49	pH	Electrometric Method[4]
50	Phenols	1) Distillation, Chloroform Extraction Method[4] 2) Distillation, Direct Photometric Method[4]
51	Selenium	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
52	Sulfide	Iodometric Method[4]
53	Temperature	Laboratory and Field Methods[4]
54	Total Dissolved Solids	Dried at 180 ^{o}C[4]
55	Total Kjeldahl Nitrogen	Semi-Micro Kjeldahl Method[4]
56	Total Phosphorous	Digestion, Colorimetric Method[4]
57	Total Suspended Solids	Dried from 103-105 ^{o}C[4]
58	Toxaphene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
59	Trivalent Chromium	1) Digestion, Inductively Coupled Plasma Method; Colorimetric Method; Calculation[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method; Colorimetric Method; Calculation[4]
60	Zinc	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[4]

น้ำใต้ดิน...

น้ำใต้ดิน จำนวน 126 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Acenaphthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
2	Acetone	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
3	Aldrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
4	Anthracene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
5	Antimony	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
6	Arsenic	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
7	Atrazine	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
8	Barium	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
9	Benz(a)anthracene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
10	Benzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
11	Benzo(b)fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
12	Benzo(k)fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
13	Benzoic Acid	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
14	Benzo(a)pyrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
15	Benzo[g,h,i]perylene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
16	Beryllium	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
17	Bis(2-chloroethyl)ether	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]

18 Bis(2-ethylhexyl)phthalate...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
18	Bis(2-ethylhexyl)phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
19	Bromodichloromethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
20	Bromoform	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
21	Butanol	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
22	Butyl benzyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
23	Cadmium	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
24	Carbazole	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
25	Carbon disulfide	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
26	Carbon tetrachloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
27	Chlordane	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
28	p-Chloroaniline	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
29	Chlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
30	Chlorodibromomethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
31	Chloroform	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
32	2-Chlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
33	Chromium	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
34	Chromium (III)	1) Digestion, Inductively Coupled Plasma Method; Colorimetric Method; Calculation[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method; Colorimetric Method; Calculation[4]
35	Chromium (VI)	Colorimetric Method[4]

36 Chrysene...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
36	Chrysene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
37	Cyanide	Distillation, Colorimetric Method[4]
38	2,4-D	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
39	DDD	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
40	DDE	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
41	DDT	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
42	Dibenz(a,h)anthracene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
43	Di-n-Butyl Phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
44	1,2-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
45	1,3-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
46	1,4-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
47	3,3-Dichlorobenzidine	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
48	1,1-Dichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
49	1,2-Dichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
50	1,1-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
51	cis-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
52	trans-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
53	2,4-Dichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
54	1,2-Dichloropropane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
55	1,3-Dichloropropane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]

56 1,3-Dichloropropene...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
56	1,3-Dichloropropene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
57	Dieldrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
58	Diethyl Phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
59	2,4-Dimethylphenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
60	2,4-Dinitrophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
61	2,4-Dinitrotoluene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
62	2,6-Dinitrotoluene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
63	Di-n-octyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
64	Endosulfan	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
65	Endrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
66	Ethylbenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
67	Fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
68	Fluorene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
69	Heptachlor	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
70	Heptachlor epoxide	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
71	Hexachlorobenzene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
72	Hexachloro-1,3-butadiene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
73	n-Hexane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
74	α-HCH	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
75	β-HCH	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]

76 γ-HCH...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
76	γ-HCH	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
77	Hexachlorocyclopentadiene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
78	Hexachloroethane	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
79	Indeno(1,2,3-cd)pyrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
80	Isophorone	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
81	Lead	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
82	Manganese	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
83	Mercury	1) Digestion, Cold Vapor Atomic Absorption Spectrometric Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
84	Methanol	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
85	Methoxychlor	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
86	Methyl bromide	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
87	Methylene chloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
88	2-Methylphenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
89	2-Methylnapthalene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
90	Methyl tert-butyl Ether	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
91	Naphthalene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
92	Nickel	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
93	Nitrobenzene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]

94 N-Nitrosodiphenylamine...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
94	N-Nitrosodiphenylamine	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
95	N-Nitrosodi-n-Propylamine	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
96	Polychlorinated Biphenyls - PCB 1016 - PCB 1221 - PCB 1232 - PCB 1242 - PCB 1248 - PCB 1254 - PCB 1260	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
97	Pentachlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
98	pH	Electrometric Method[4]
99	Phenanthrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
100	Phenol	1) Distillation, Chloroform Extraction Method[4] 2) Distillation, Direct Photometric Method[4] 3) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
101	Pyrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
102	Selenium	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
103	Silver	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
104	Styrene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
105	1,1,2,2-Tetrachloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
106	Tetrachloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
107	Toluene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
108	Toxaphene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
109	TPH (C_5-C_8)	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,25]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
110	TPH ($C_{>8}$-C_{16})	Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[9,22]
111	TPH ($C_{>16}$-C_{35})	Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[9,22]
112	1,2,4-Trichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
113	1,1,1-Trichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
114	1,1,2-Trichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
115	Trichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
116	2,4,5-Trichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
117	2,4,6-Trichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
118	1,3,5-Trimethylbenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
119	Vanadium	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
120	Vinyl acetate	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
121	Vinyl chloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
122	m-Xylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
123	o-Xylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
124	p-Xylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
125	Xylene (Total)	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
126	Zinc	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]

อากาศเสีย (ปล่องระบาย) จำนวน 28 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Antimony	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[5]
2	Arsenic	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[5]
3	Beryllium	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[5]
4	Cadmium	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[5]
5	Carbon Monoxide	1) Instrumental Analyzer Method[5] 2) Sampling Bag Non-Dispersive Infrared Method[5]
6	Chlorine	1) Absorption Sampling, Ion Chromatographic Method[5] 2) Isokinetic Sampling, Ion Chromatographic Method [5]
7	Chromium	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[5]
8	Cobalt	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[5]
9	Copper	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[5]
10	Cresol	Adsorption Sampling, Gas Chromatographic Method[5]
11	Dioxins	Isokinetic Sampling[5]
12	Hydrogen Chloride	1) Absorption Sampling, Ion Chromatographic Method[5] 2) Isokinetic Sampling, Ion Chromatographic Method[5]
13	Hydrogen Fluoride	1) Absorption Sampling, Ion Chromatographic Method[5] 2) Isokinetic Sampling, Ion Chromatographic Method[5]
14	Hydrogen Sulfide	Absorption Sampling, Iodometric Method[5]

15 Lead...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
15	Lead	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[5]
16	Manganese	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[5]
17	Mercury	1) Isokinetic Sampling, Digestion, Cold-Vapor Atomic Absorption Spectrometric Method[5] 2) Isokinetic Sampling, Digestion, Cold-Vapor Atomic Fluorescence Spectrometric Method[5]
18	Nickel	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[5]
19	Opacity	Ringelmann's Method[2]
20	Oxides of Nitrogen	1) Absorption Sampling, Phenoldisulfonic Acid Method[5] 2) Absorption Sampling, Alkaline Permanganate/ Colorimetric Method[5] 3) Instrumental Analyzer Method[5]
21	Selenium	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[5]
22	Sulfur Dioxide	1) Absorption Sampling, Barium-Thorin Titrimetric Method[5] 2) Instrumental Analyzer Method[5]
23	Sulfuric Acid	Isokinetic Sampling, Barium-Thorin Titrimetric Method[5]
24	Tellurium	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[5]
25	Tin	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[5]
26	Total Suspended Particulate	1) Isokinetic Sampling, Gravimetric Method[5] 2) Paired Train, Isokinetic Sampling, Gravimetric Method[5]

27 Vanadium...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
27	Vanadium	1) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[5]
28	Xylene	Adsorption Sampling, Gas Chromatographic Method[5]

<u>สิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว จำนวน 35 รายการ</u>

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Aldrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,26] 2) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
2	Antimony	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,17] 3) Digestion, Inductively Coupled Plasma Method[7,16] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
3	Arsenic	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,17] 3) Digestion, Inductively Coupled Plasma Method[7,16] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
4	Barium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,17] 3) Digestion, Inductively Coupled Plasma Method[7,16] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]

5 Beryllium...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
5	Beryllium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,17] 3) Digestion, Inductively Coupled Plasma Method[7,16] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
6	Cadmium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,17] 3) Digestion, Inductively Coupled Plasma Method[7,16] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
7	Chlordane	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,26] 2) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
8	Chromium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,17] 3) Digestion, Inductively Coupled Plasma Method[7,16] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
9	Chromium (III)	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method; Waste Extraction, Colorimetric Method; Calculation Method[1,6,16,19] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method; Waste Extraction, Colorimetric Method; Calculation Method[1,6,17,19] 3) Digestion, Inductively Coupled Plasma Method; Alkaline Digestion, Colorimetric Method; Calculation Method[7,8,16,19] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method; Alkaline Digestion, Colorimetric Method; Calculation Method[7,8, 17,19]

10 Chromium (VI)...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
10	Chromium (VI)	1) Waste Extraction, Colorimetric Method[1,6,19] 2) Alkaline Digestion, Colorimetric Method[8,19]
11	Cobalt	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,17] 3) Digestion, Inductively Coupled Plasma Method[7,16] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
12	Copper	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,17] 3) Digestion, Inductively Coupled Plasma Method[7,16] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
13	2,4-D	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,26] 2) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
14	DDD	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,26] 2) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
15	DDE	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,26] 2) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
16	DDT	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,26]

2) Soxhlet...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
		2) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
17	Dieldrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,26] 2) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
18	Endrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,26] 2) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
19	Heptachlor	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,26] 2) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
20	Lead	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,17] 3) Digestion, Inductively Coupled Plasma Method[7,16] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
21	Lindane	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,26] 2) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]

22 Mercury...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
22	Mercury	1) Waste Extraction, Digestion, Cold-Vapor Atomic Absorption Spectrometric Method[1,6,20] 2) Waste Extraction, Digestion, Cold-Vapor Atomic Fluorescence Spectrometric Method[1,6,30] 3) Digestion, Cold-Vapor Atomic Absorption Spectrometric Method[20] 4) Digestion, Cold-Vapor Atomic Fluorescence Spectrometric Method[30] 5) Thermal Decomposition Amalgamation and Atomic Absorption Spectrometric Method[21]
23	Methoxychlor	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,26] 2) Soxhlet Extraction, Gas Chromatographic / Mass Spectrometric Method[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic /Mass Spectrometric Method[11,26]
24	Mirex	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,26] 2) Soxhlet Extraction, Gas Chromatographic / Mass Spectrometric Method[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic /Mass Spectrometric Method[11,26]
25	Molybdenum	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,17] 3) Digestion, Inductively Coupled Plasma Method[7,16] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
26	Nickel	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,17] 3) Digestion, Inductively Coupled Plasma Method[7,16] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
27	Polychlorinated biphenyls (PCBs) - Aroclor 1016 - Aroclor 1221 - Aroclor 1232 - Aroclor 1242 - Aroclor 1248 - Aroclor 1254 - Aroclor 1260	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,26] 2) Soxhlet Extraction, Gas Chromatographic Method[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic Method[11,26]

- 2-Chlorobiphenyl...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
	- 2-Chlorobiphenyl - 2,3-Dichlorobiphenyl - 2,2',5-Trichlorobiphenyl - 2,4',5-Trichlorobiphenyl - 2,2',3,5'-Tetrachlorobiphenyl - 2,2',5,5'-Tetrachlorobiphenyl - 2,3',4,4'-Tetrachlorobiphenyl - 2,2',3,4,5'-Pentachlorobiphenyl - 2,2',4,5,5'-Pentachlorobiphenyl - 2,3,3',4',6-Pentachlorobiphenyl - 2,2',3,4,4',5'-Hexachlorobiphenyl - 2,2',3,4,5,5'-Hexachlorobiphenyl - 2,2',3,5,5',6-Hexachlorobiphenyl - 2,2',4,4',5,5'-Hexachlorobiphenyl - 2,2',3,3',4,4',5-Heptachlorobiphenyl - 2,2',3,4,4',5,5'-Heptachlorobiphenyl - 2,2',3,4,4',5',6-Heptachlorobiphenyl - 2,2',3,4',5,5',6-Heptachlorobiphenyl - 2,2',3,3',4,4',5,5',6-Nonachlorobiphenyl	
28	Pentachlorophenol	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,26] 2) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
29	pH	Electrometric Method[23,24]
30	Selenium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,17] 3) Digestion, Inductively Coupled Plasma Method[7,16] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]

31 Silver...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
31	Silver	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,17] 3) Digestion, Inductively Coupled Plasma Method[7,16] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
32	Thallium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,17] 3) Digestion, Inductively Coupled Plasma Method[7,16] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
33	Toxaphene	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,26] 2) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 3) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
34	Vanadium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,17] 3) Digestion, Inductively Coupled Plasma Method[7,16] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
35	Zinc	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,17] 3) Digestion, Inductively Coupled Plasma Method[7,16] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]

ดิน จำนวน 125 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Acenaphthene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
2	Acetone	1)Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25] 2) Equilibrium Headspace, Gas Chromatographic/ Mass Spectrometric Method[13]
3	Aldrin	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
4	Anthracene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
5	Antimony	1) Digestion, Inductively Coupled Plasma Method[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
6	Arsenic	1) Digestion, Inductively Coupled Plasma Method[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
7	Atrazine	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
8	Barium	1) Digestion, Inductively Coupled Plasma Method[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
9	Benz(a)anthracene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
10	Benzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
11	Benzo(b)fluoranthene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
12	Benzo(k)fluoranthene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
13	Benzoic acid	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
14	Benzo(a)pyrene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
15	Benzo(g,h,i)perylene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
16	Beryllium	1) Digestion, Inductively Coupled Plasma Method[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
17	Bis(2-chloroethyl)ether	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
18	Bis(2-ethylhexyl)phthalate	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
19	Bromodichloromethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
20	Bromoform	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
21	Butanol	Equilibrium Headspace, Gas Chromatographic/ Mass Spectrometric Method[13,25]
22	Butyl Benzyl Phthalate	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]

23 Cadmium...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
23	Cadmium	1) Digestion, Inductively Coupled Plasma Method[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
24	Carbazole	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
25	Carbon Disulfide	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
26	Carbon tetrachloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
27	Chlordane	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
28	p-Chloroaniline	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
29	Chlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
30	Chlorodibromomethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
31	Chloroform	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
32	2-Chlorophenol	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
33	Chromium	1) Digestion, Inductively Coupled Plasma Method[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
34	Chromium (III)	1) Digestion, Inductively Coupled Plasma Method; Alkaline Digestion, Colorimetric Method; Calculation Method[7,8,16,19] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method; Alkaline Digestion, Colorimetric Method; Calculation Method[7,8,17,19]
35	Chromium (VI)	Alkaline Digestion, Colorimetric Method[8,19]

36 Chrysene...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
36	Chrysene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
37	Cyanide	Extraction, Distillation, Colorimetric Method[27,28,29]
38	2,4-D	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
39	DDD	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
40	DDE	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
41	DDT	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
42	Dibenz(a,h)anthracene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
43	Di-n-Butyl Phthalate	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
44	1,2-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
45	1,3-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
46	1,4-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
47	3,3-Dichlorobenzidine	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
48	1,1-Dichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
49	1,2-Dichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
50	1,1-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
51	cis-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
52	trans-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
53	2,4-Dichlorophenol	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
54	1,2-Dichloropropane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
55	1,3-Dichloropropane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
56	1,3-Dichloropropene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
57	Dieldrin	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
58	Diethyl Phthalate	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
59	2,4-Dimethylphenol	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
60	2,4-Dinitrophenol	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
61	2,4-Dinitrotoluene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
62	2,6-Dinitrotoluene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
63	Di-n-Octyl Phthalate	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
64	Endosulfan	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
65	Endrin	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
66	Ethylbenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
67	Fluoranthene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
68	Fluorene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
69	Heptachlor	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
70	Heptachlor epoxide	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
71	Hexachlorobenzene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
72	Hexachloro-1,3-butadiene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
73	n-Hexane	1) Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25] 2) Equilibrium Headspace, Gas Chromatographic/ Mass Spectrometric Method[13]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
74	α-HCH	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
75	β-HCH	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
76	γ-HCH	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
77	Hexachlorocyclopentadiene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
78	Hexachloroethane	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
79	Indeno(1,2,3-cd)pyrene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
80	Isophorone	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
81	Lead	1) Digestion, Inductively Coupled Plasma Method[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
82	Manganese	1) Digestion, Inductively Coupled Plasma Method[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
83	Mercury	1) Digestion, Cold-Vapor Atomic Absorption Spectrometric Method[20] 2) Thermal Decomposition, Amalgamation, and Atomic Absorption Spectrophotometry[21] 3) Digestion, Cold-Vapor Atomic Fluorescence Spectrometric Method[30]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
84	Methanol	1) Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25] 2) Equilibrium Headspace, Gas Chromatographic/ Mass Spectrometric Method[13,25]
85	Methoxychlor	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
86	Methyl Bromide	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
87	Methylene Chloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
88	2-methylphenol	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
89	2-Methylnaphthalene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
90	Methyl tert-Butyl Ether	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
91	Naphthalene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
92	Nickel	1) Digestion, Inductively Coupled Plasma Method[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
93	Nitrobenzene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
94	N-Nitrosodiphenylamine	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
95	N-Nitrosodi-n-propylamine	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
96	Polychlorinated biphenyls (PCBs) - Aroclor 1016 - Aroclor 1221 - Aroclor 1232 - Aroclor 1242 - Aroclor 1248 - Aroclor 1254 - Aroclor 1260 - 2-Chlorobiphenyl - 2,2',3,5'-Tetrachlorobiphenyl - 2,2',5,5'-Tetrachlorobiphenyl - 2,3',4,4'-Tetrachlorobiphenyl - 2,2',3,4,5'-Pentachlorobiphenyl - 2,2',4,5,5'-Pentachlorobiphenyl - 2,3,3',4',6-Pentachlorobiphenyl - 2,2',3,4,4',5'-Hexachlorobiphenyl - 2,2',3,4,5,5'-Hexachlorobiphenyl - 2,2',3,5,5',6-Hexachlorobiphenyl - 2,2',4,4',5,5'-Hexachlorobiphenyl - 2,2',3,3',4,4',5-Heptachlorobiphenyl - 2,2',3,4,4',5,5'-Heptachlorobiphenyl - 2,2',3,4,4',5',6-Heptachlorobiphenyl - 2,2',3,4',5,5',6-Heptachlorobiphenyl - 2,2',3,3',4,4',5,5',6-Nonachlorobiphenyl	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
97	Pentachlorophenol	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
98	Phenanthrene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
99	Phenol	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
100	Pyrene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
101	Selenium	1) Digestion, Inductively Coupled Plasma Method[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
102	Silver	1) Digestion, Inductively Coupled Plasma Method[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
103	Styrene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
104	1,1,2,2-Tetrachloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
105	Tetrachloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
106	Toluene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
107	Toxaphene	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
108	TPH (C_5–C_8)	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
109	TPH ($C_{>8}$– C_{16})	1) Automate Extraction, Gas Chromatographic Method[11,22] 2) Solvent Extraction, Gas Chromatographic Method[12,22] 3) Ultrasonic Extraction, Gas Chromatographic Method[22,31]
110	TPH ($C_{>16}$ – C_{35})	1) Automate Extraction, Gas Chromatographic Method[11,22] 2) Solvent Extraction, Gas Chromatographic Method[12,22] 3) Ultrasonic Extraction, Gas Chromatographic Method[22,31]
111	1,2,4-Trichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
112	1,1,1-Trichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
113	1,1,2-Trichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
114	Trichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]

115 2,4,5-Trichlorophenol...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
115	2,4,5-Trichlorophenol	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
116	2,4,6-Trichlorophenol	1) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,26] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,26]
117	1,3,5-Trimethylbenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
118	Vanadium	1) Digestion, Inductively Coupled Plasma Method[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]
119	Vinyl Acetate	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
120	Vinyl Chloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
121	m-Xylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
122	o-Xylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
123	p-Xylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
124	Xylene (Total)	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[15,25]
125	Zinc	1) Digestion, Inductively Coupled Plasma Method[7,16] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,17]

เอกสารอ้างอิง

1. กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2566. เรื่อง การจัดการสิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว. **ราชกิจจานุเบกษา.** 31 พฤษภาคม 2566. เล่มที่ 140 ตอนพิเศษ 126 ง.

2. กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2549. เรื่อง กำหนดค่าปริมาณเขม่าควันที่เจือปนในอากาศที่ระบายออกจากปล่องของหม้อน้ำโรงสีข้าวที่ใช้แกลบเป็นเชื้อเพลิง. **ราชกิจจานุเบกษา.** 4 ธันวาคม 2549. เล่มที่ 123 ตอนพิเศษ 125ง.

3. สมาคมวิศวกรรมสิ่งแวดล้อมแห่งประเทศไทย. **คู่มือวิเคราะห์น้ำเสีย.** พิมพ์ครั้งที่ 4. กรุงเทพฯ: เรือนแก้วการพิมพ์, 2547.

4. APHA, AWWA, WEF. **Standard Methods for the Examination of Water and Wastewater.** 24th ed. Washington, DC: APHA, 2023.

5. United States...

5. United States Environmental Protection Agency. **Standards of Performance for New Stationary Sources.** 40 CFR 60. Appendix A, 2023.

6. United States Environmental Protection Agency. **Test Methods for Evaluating Solid Waste Physical/Chemical Methods. SW-846,** 2014.

7. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Acid Digestion of Sludges and Sediments and Soils. SW-846 Method 3050B,** 1996.

8. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Alkaline Digestion for Hexavalent Chromium. SW-846 Method 3060A,** 1996.

9. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Separatory Funnel Liquid-Liquid Extraction. SW-846 Method 3510C,** 1996.

10. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Soxhlet Extraction. SW-846 Method 3540C,** 1996.

11. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Automated Soxhlet Extraction. SW-846 Method 3541,** 1994.

12. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Microscale Solvent Extraction (MSE). SW-846 Method 3570,** 2002.

13. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Volatile Organic Compounds (VOCs) in Various Sample Matrices Using Equilibrium Headspace Analysis. SW-846 Method 5021A,** 2014.

14. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Purge-and-Trap for Aqueous Samples. SW-846 Method 5030B,** 1996.

15. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Closed-System Purge-and-Trap and Extraction for Volatile Organics in Soil and Waste Samples. SW-846 Method 5035,** 1996.

16. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Inductively Coupled Plasma-Atomic Emission Spectrometry. SW-846 Method 6010B,** 1996.

17. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Inductively Coupled Plasma-Mass Spectrometry. SW-846 Method 6020A,** 2007.

18. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Antimony and Arsenic (Atomic Absorption, Borohydride Reduction). SW-846 Method 7062,** 1994. เพิ่มใหม่

19. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Chromium, Hexavalent (Colorimetric). SW-846 Method 7196A,** 1992.

20. United States...

20. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Mercury in Solid or Semisolid Waste (Manual Cold-Vapor Technique). SW-846 Method 7471B,** 2007.

21. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Mercury in Solids and Solutions by Thermal Decomposition, Amalgamation, and Atomic Absorption Spectrophotometry. SW-846 Method 7473,** 2007.

22. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Nonhalogenated Organics by Gas Chromatography. SW-846 Method 8015C,** 2007.

23. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **pH Electrometric Measurement. SW-846 Method 9040C,** 2004.

24. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Soil and Waste pH. SW-846 Method 9045D,** 2004.

25. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Volatile Organic Compounds by Gas Chromatography/ Mass Spectrometry (GC/MS). SW-846 Method 8260D,** 2018.

26. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Semivolatile Organic Compounds by Gas Chromatography/ Mass Spectrometry (GC/MS). SW-846 Method 8270E,** 2018.

27. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Total and Amenable Cyanide: Distillation SW-846 Method 9010B,** 1996.

28. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Cyanide Extraction Procedure for Solids and Oil. SW-846 Method 9013A,** 1996.

29. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Cyanide in Waters and Extracts Using Titrimetric and Manual Spectrophotometric Procedures. SW-846 Method 9014,** 2014.

30. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Mercury in Sediment and Tissue Samples by Atomic Fluorescence Spectrometry. SW-846 Method 7474,** 2007.

31. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Ultrasonic Extraction. SW-846 Method 3550C,** 2007.



ที่ อก ๐๓๑๐(๑)/ ๔๑๒๑

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๒๕ เมษายน ๒๕๖๗

เรื่อง เปลี่ยนแปลงบุคลากรของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน ลงวันที่ ๒๙ มีนาคม ๒๕๖๗

ตามคำขอที่อ้างถึง บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๒๐๔ สถานที่ตั้งเลขที่ ๑๐๔ ซอยพัฒนาการ ๔๐ ถนนพัฒนาการ แขวงพัฒนาการ เขตสวนหลวง กรุงเทพมหานคร ขอเปลี่ยนแปลงบุคลากร ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว มีความเห็นดังนี้

๑. ให้ยกเลิกเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๓ ราย

๑) นางสาวพรรณธิดา พุ่มคง	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๕
๒) นายกำชัย สุทธะ	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๒๑
๓) นางสาวศุภรดา ปั้นมยุรา	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๘

๒. ให้เพิ่มเจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน จำนวน ๑๒ ราย

๑) นางสาวฐานิดา กลิ่นเขียว	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๘๒
๒) นางสาวกัญญ์ภัสสร สายคำ	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๘๓
๓) นางสาวณัฐนันท์ กันทะวงค์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๘๔
๔) นายอำนาจ วงษาเคน	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๘๕
๕) นายกฤษณพล ปัญญาวงค์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๘๖
๖) นายณชากร หรรษา	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๘๗
๗) นายวัชรินทร์ ผ่องสามสวน	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๘๘
๘) นายณัฐพงศ์ โสภา	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๘๙
๙) นายศักรินทร์ ปานเพ็ง	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๙๐
๑๐) นายณัฐพล ชุ่มชื่น	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๙๑
๑๑) นายธนา สุพาพันธุ์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๙๒
๑๒) นายนราธร แก้วพงษ์ษา	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๙๓

อนึ่ง หนังสือฉบับนี้...

อนึ่ง หนังสือฉบับนี้จะหมดอายุพร้อมหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ในวันที่ ๒ กันยายน ๒๕๖๙

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายพรยศ กลั่นกรอง)
รองอธิบดี ปฏิบัติราชการแทน
อธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน
กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ
โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕
โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๙๙
ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th

ที่ อก ๐๓๑๐(๑)/๑๒๓๖๘ ๑

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๑๘ ธันวาคม ๒๕๖๗

เรื่อง ยกเลิกบุคลากรของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน ลงวันที่ ๒ ธันวาคม ๒๕๖๗

ตามคำขอที่อ้างถึง บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๒๐๔ สถานที่ตั้งเลขที่ ๑๐๔ ซอยพัฒนาการ ๔๐ ถนนพัฒนาการ แขวงพัฒนาการ เขตสวนหลวง กรุงเทพมหานคร ขอยกเลิกบุคลากร ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้ยกเลิกเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๘ ราย ได้แก่

๑) นายประพจน์ วรรณชูชัย	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๖๐
๒) นายจิรณัฐ ขาวละออ	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๗๒
๓) นายพีรพัฒน์ กำคำ	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๘
๔) นางสาวอรยา ค้าคล่อง	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๔
๕) นายกิตติพงศ์ แซ่ลี้	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๔๔
๖) นายจิรเมธ ประเสริฐสิริพงศ์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๐
๗) นายภัทรพงษ์ มณฑาทอง	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๖๗
๘) นางสาวจารุวรรณ กระจ่างพันธุ์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๘๑

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายธีรทัศน์ อิศรางกูร ณ อยุธยา)
รองอธิบดี ปฏิบัติราชการแทน
อธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน
กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ
โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕
โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๙๙
ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th

ที่ อก ๐๓๑๐(๑)/ ๓๑๔๐

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๑๐ เมษายน ๒๕๖๘

เรื่อง ยกเลิกบุคลากรของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน ลงวันที่ ๒ เมษายน ๒๕๖๘

ตามคำขอที่อ้างถึง บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๒๐๔ สถานที่ตั้งเลขที่ ๑๐๔ ซอยพัฒนาการ ๔๐ ถนนพัฒนาการ แขวงพัฒนาการ เขตสวนหลวง กรุงเทพมหานคร ขอยกเลิกบุคลากร ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้ยกเลิกเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๒ ราย ได้แก่

๑) นายธิติพงศ์ บัวแดง	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๒
๒) นายมงคล ผลาทิพย์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๐๑๐

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายธีรทัศน์ อิศรางกูร ณ อยุธยา)
รองอธิบดี ปฏิบัติราชการแทน
อธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน
กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ
โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕
โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๙๙
ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th

Green Industry
"อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา อุตสาหกรรมสีเขียว"

ที่ อก ๐๓๑๐(๑)/ ๕๖๗๓

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๐๕ มิถุนายน ๒๕๖๘

เรื่อง เปลี่ยนแปลงบุคลากรของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน ลงวันที่ ๓ พฤษภาคม ๒๕๖๘

ตามคำขอที่อ้างถึง บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๒๐๔ สถานที่ตั้งเลขที่ ๑๐๔ ซอยพัฒนาการ ๔๐ ถนนพัฒนาการ แขวงพัฒนาการ เขตสวนหลวง กรุงเทพมหานคร ขอเปลี่ยนแปลงบุคลากร ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้เพิ่มเจ้าหน้าที่ห้องปฏิบัติการวิเคราะห์เอกชน จำนวน ๑๑ ราย ได้แก่

๑) นายคุณากร มันชื่น	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๙๔
๒) นายชัยมงคล แสนมาตร	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๙๕
๓) นายเอกรินทร์ บุดสักที	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๙๖
๔) นายพัชชานนท์ อินปริก	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๙๗
๕) นายศตวรรษ แก้วกันหา	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๙๘
๖) นายวิกรม มีศิริ	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๙๙
๗) นายภคนันท์ คำจันทราช	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๒๐๐
๘) นายศิรวิทย์ มีไพฑูรย์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๒๐๑
๙) นายธีรพงษ์ ศรีคำแหง	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๒๐๒
๑๐) นายอภิสิทธิ์ ศรีคงแก้ว	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๒๐๓
๑๑) ว่าที่ร้อยตรี ภาณุพงศ์ แสนศรี	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๒๐๔

อนึ่ง หนังสือฉบับนี้จะสิ้นอายุพร้อมหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ในวันที่ ๒ กันยายน ๒๕๖๙

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายศิริระ จับหร่ำเพ็ง)
นักวิทยาศาสตร์เชี่ยวชาญ รักษาราชการแทน
ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน
กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ
โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕
โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๙๙
ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th

ที่ อก ๐๓๑๐(๑)/ ๖๙๐๘

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๒๑ สิงหาคม ๒๕๖๘

เรื่อง เปลี่ยนแปลงสารมลพิษที่วิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน ลงวันที่ ๒๗ มิถุนายน ๒๕๖๘

สิ่งที่ส่งมาด้วย เอกสารแนบท้ายหนังสือเปลี่ยนแปลงสารมลพิษที่วิเคราะห์ บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด จำนวน ๖ แผ่น

ตามคำขอที่อ้างถึง บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๒๐๔ สถานที่ตั้งเลขที่ ๑๐๔ ซอยพัฒนาการ ๔๐ ถนนพัฒนาการ แขวงพัฒนาการ เขตสวนหลวง กรุงเทพมหานคร ขอเปลี่ยนแปลงสารมลพิษที่วิเคราะห์ ต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด เพิ่มขอบข่ายชนิดสารมลพิษที่วิเคราะห์ในน้ำใต้ดิน สิ่งปฏิกูลและวัสดุที่ไม่ใช้แล้ว และดิน ตามสิ่งที่ส่งมาด้วย

อนึ่ง หนังสือฉบับนี้จะสิ้นอายุพร้อมหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ในวันที่ ๒ กันยายน ๒๕๖๙

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นางสาวปัทมวรรณ คุณประเสริฐ)
ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน
กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ
โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕
โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๙๙
ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th

เอกสารแนบท้ายหนังสือเปลี่ยนแปลงสารมลพิษที่วิเคราะห์
บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด เลขทะเบียน ว-๒๐๔
ที่ อก ๐๓๑๐(๑)/ ๖๙๐๘ ลงวันที่ ๒๑ สิงหาคม ๒๕๖๘

ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๔๐ รายการ

น้ำใต้ดิน จำนวน ๔ รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Aluminum	Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[2]
2	Copper	Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[2]
3	Iron	Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[2]
4	Molybdenum	Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[2]

สิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว จำนวน 17 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Antimony	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,3,7] 3) Digestion, Inductively Coupled Plasma Method[4,6] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
2	Arsenic	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,3,7] 3) Digestion, Inductively Coupled Plasma Method[4,6] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
3	Barium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,3,7] 3) Digestion, Inductively Coupled Plasma Method[4,6] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]

Beryllium

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
4	Beryllium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,3,7] 3) Digestion, Inductively Coupled Plasma Method[4,6] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
5	Cadmium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,3,7] 3) Digestion, Inductively Coupled Plasma Method[4,6] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
6	Chromium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,3,7] 3) Digestion, Inductively Coupled Plasma Method[4,6] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
7	Chromium (III)	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method; Waste Extraction, Colorimetric Method; Calculation Method[1,3,6,8] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method; Waste Extraction, Colorimetric Method; Calculation Method[1,3,7,8] 3) Digestion, Inductively Coupled Plasma Method; Alkaline Digestion, Colorimetric Method; Calculation Method[4,5,6,8] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method; Alkaline Digestion, Colorimetric Method; Calculation Method[4,5,7,8]
8	Cobalt	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,3,7]

3) Digestion...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
		3) Digestion, Inductively Coupled Plasma Method[4,6] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
9	Copper	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,3,7] 3) Digestion, Inductively Coupled Plasma Method[4,6] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
10	Lead	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,3,7] 3) Digestion, Inductively Coupled Plasma Method[4,6] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
11	Molybdenum	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,3,7] 3) Digestion, Inductively Coupled Plasma Method[4,6] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
12	Nickel	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,3,7] 3) Digestion, Inductively Coupled Plasma Method[4,6] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
13	Selenium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,3,7] 3) Digestion, Inductively Coupled Plasma Method[4,6] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
14	Silver	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,3,7] 3) Digestion, Inductively Coupled Plasma Method[4,6] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
15	Thallium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,3,7] 3) Digestion, Inductively Coupled Plasma Method[4,6] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
16	Vanadium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,3,7] 3) Digestion, Inductively Coupled Plasma Method[4,6] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
17	Zinc	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,3,6] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,3,7] 3) Digestion, Inductively Coupled Plasma Method[4,6] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]

ดิน จำนวน 19 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Aluminum	1) Digestion, Inductively Coupled Plasma Method[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
2	Antimony	1) Digestion, Inductively Coupled Plasma Method[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
3	Arsenic	1) Digestion, Inductively Coupled Plasma Method[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
4	Barium	1) Digestion, Inductively Coupled Plasma Method[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
5	Beryllium	1) Digestion, Inductively Coupled Plasma Method[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
6	Cadmium	1) Digestion, Inductively Coupled Plasma Method[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
7	Chromium	1) Digestion, Inductively Coupled Plasma Method[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
8	Chromium (III)	1) Digestion, Inductively Coupled Plasma Method; Alkaline Digestion, Colorimetric Method; Calculation Method[4,5,6,8] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method; Alkaline Digestion, Colorimetric Method; Calculation Method[4,5,7,8]
9	Copper	1) Digestion, Inductively Coupled Plasma Method[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
10	Iron	1) Digestion, Inductively Coupled Plasma Method[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
11	Lead	1) Digestion, Inductively Coupled Plasma Method[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
12	Manganese	1) Digestion, Inductively Coupled Plasma Method[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
13	Molybdenum	1) Digestion, Inductively Coupled Plasma Method[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
14	Nickel	1) Digestion, Inductively Coupled Plasma Method[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
15	pH	Electrometric Method[9]
16	Selenium	1) Digestion, Inductively Coupled Plasma Method[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
17	Silver	1) Digestion, Inductively Coupled Plasma Method[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
18	Vanadium	1) Digestion, Inductively Coupled Plasma Method[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]
19	Zinc	1) Digestion, Inductively Coupled Plasma Method[4,6] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4,7]

เอกสารอ้างอิง

1. กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2566. เรื่อง การจัดการสิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว. **ราชกิจจานุเบกษา.** 31 พฤษภาคม 2566. เล่มที่ 140 ตอนพิเศษ 126 ง.

2. APHA, AWWA, WEF. **Standard Methods for the Examination of Water and Wastewater.** 24th ed. Washington, DC: APHA, 2023.

3. United States Environmental Protection Agency. **Test Methods for Evaluating Solid Waste Physical/Chemical Methods. SW-846**.

4. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Acid Digestion of Sediments, Sludges, and Soils. SW-846 Method 3050B,** 1996.

5. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Alkaline Digestion for Hexavalent Chromium. SW-846 Method 3060A,** 1996.

6. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Inductively Coupled Plasma-Optical Emission Spectrometry. SW-846 Method 6010D,** 2018.

7. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Inductively Coupled Plasma-Mass Spectrometry. SW-846 Method 6020B,** 2014.

8. United States Environmental Protection Agency. Test Methods for Evaluating Solid Waste Physical/Chemical Methods. **Chromium, Hexavalent (Colorimetric). SW-846 Method 7196A,** 1992.

9. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Soil and Waste pH. SW-846 Method 9045D,** 2004.



ที่ อก ๐๓๑๐(๑)/๘๐ ๑๑

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๒๖ กันยายน ๒๕๖๘

เรื่อง เปลี่ยนแปลงบุคลากร ชื่อตัวและชื่อสกุลของบุคลากร

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน ลงวันที่ ๒๑ สิงหาคม ๒๕๖๘

ตามคำขอที่อ้างถึง บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัดห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๒๐๔ สถานที่ตั้งเลขที่ ๑๐๔ ซอยพัฒนาการ ๔๐ ถนนพัฒนาการ แขวงพัฒนาการ เขตสวนหลวง กรุงเทพมหานคร ขอเปลี่ยนแปลงบุคลากร ชื่อตัวและชื่อสกุลของบุคลากร ต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว มีความเห็นดังนี้

๑. ให้ยกเลิกเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๒ ราย

๑) นางสาวพาฤดี คุณนาน ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๓๙

๒) นางสาวอรณิช เทียนดำ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๑๗๔

๒. ให้เปลี่ยนชื่อตัวและชื่อสกุลของเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จากเดิม นายอาทิตย์ ศรีเสน เป็น นายรัฐธีร์ ทวีกิจวรพจน์ ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๔๘

อนึ่ง หนังสือฉบับนี้จะสิ้นอายุพร้อมหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ในวันที่ ๒ กันยายน ๒๕๖๙

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นางสาวปัทมวรรณ คุณประเสริฐ)
ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน
กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ
โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕
โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๙๙
ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th

right solutions.
right partner.

bangkok@alsglobal.com

ALS Line Official
ID: @alsthailand

ALS Facebook
Search: ALS Thailand