



QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584



CERTIFICATE No : 24E4141
REFERENCE No : 73037-3

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : pH METER
MANUFACTURER : MILWAUKEE
MODEL : MW102
SERIAL No : 11006210200
ID No : TLC-L132
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : TOPS-LAB CONSULTANTS CO., LTD.
189 MOO.3 BANGRAKPHATTHANA
BANGBUATHONG NONTHABURI 11110

CALIBRATED BY

:

[Redacted Signature]

CALIBRATION DATE

:

07-May-24

APPROVED BY

:

[Redacted Signature]

ISSUED DATE

:

09-May-24

RECEIVED DATE

:

07-May-24

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.



QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 24E4141

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : pH METER
MANUFACTURER : MILWAUKEE
ID No : TLC-L132
RECEIVED DATE : 07-May-24
AMBIENT TEMPERATURE : 26° C ± 1° C
MODEL : MW102
SERIAL NUMBER : 11006210200
CALIBRATION DATE : 07-May-24
RELATIVE HUMIDITY : 49 %RH ± 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT METHOD BASED ON WI-TQ-062. THE DISPLAY UNIT WAS TESTED BY GENERATING STANDARD VOLTAGE TO THE UNIT AND READ THE VALUE COMPARED WITH CALCULATED VALUE. THE DISPLAY AND ELECTRODE WAS CALIBRATED BY USING STANDARD pH BUFFER SOLUTION.
2. REFERENCE STANDARD INSTRUMENTS :-

<u>INSTRUMENT</u>	<u>MODEL</u>	<u>SERIAL No/</u> <u>LOT No</u>	<u>CERTIFICATE No</u>	<u>DUE DATE</u>
1) pH STANDARD SOLUTION	00651-06	CC767907	4880-13836406	29-Dec-24
2) pH STANDARD SOLUTION	00651-08	CC765602	4881-13757019	18-Nov-24
3) pH STANDARD SOLUTION	00651-10	CC767180	4882-13813369	14-Dec-24
4) PROCESS CALIBRATOR	CA150	91S6079	24E1251	09-Apr-25
5) BATH	260014	1247 48074	23T9014	13-Sep-24
6) THERMOMETER WITH PROBE	421504	55000379	23T9623	13-Sep-24

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO SI UNIT MAINTAINED AT :-
 - NATIONAL INSTITUTE OF STANDARD AND TECHNOLOGY, USA.
 - NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION : WITHOUT ADJUSTMENT

1. DISPLAY UNIT WITH pH ELECTRODE S/N: SE220

STANDARD pH BUFFER SOLUTION (pH)	UUC READING (pH)	CORRECTION (pH)	VALUE BEFORE ADJUSTMENT	UNCERTAINTY OF MEASUREMENT (± pH)	COVERAGE FACTOR k
4.006	4.01	-0.004	---	0.013	2.0
6.999	7.00	-0.001	---	0.013	2.0
10.007	10.01	-0.003	---	0.014	2.0

UUC : UNIT UNDER CALIBRATION

THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com



CERTIFICATE No : 24T4147
REFERENCE No : 73038-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : INCUBATOR
MANUFACTURER : AQUALYTIC
MODEL : ET618-4
SERIAL No : 0109/13922
ID No : TLC-L005
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : TOPS-LAB CONSULTANTS CO., LTD.
189 MOO.3 BANGRAKPHATTHANA
BANGBUATHONG NONTABURI 11110

CALIBRATED BY :

CALIBRATION DATE :

07-May-24

APPROVED BY :

ISSUED DATE :

09-May-24

RECEIVED DATE :

07-May-24

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.

F-G010 REV : 03



CERTIFICATE No : 24T4147

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : INCUBATOR
MANUFACTURER : AQUALYTIC
MODEL : ET618-4
ID No : TLC-L005
RECEIVED DATE : 07-May-24
AMBIENT TEMPERATURE : 26 °C ± 1 °C

S/N : 0109/13922
CALIBRATION DATE : 07-May-24
RELATIVE HUMIDITY : 53 %RH ± 10 %RH

CONDITION OF THIS RESULTS OF CALIBRATION


1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO TLAS G-20 BY COMPARISON WITH CALIBRATED RTD Pt100 UNDER NO LOAD CONDITION. THE TEMPERATURE PROBES WERE PLACED ON NINE POINTS AND LOCATED ONE THERMOMETER PROBE IN EACH OF THE EIGHT CORNERS OF THE CHAMBER AND WAS AWAY FROM THE EACH WALL OF 5 cm TO 10 cm. AND PLACED THE NINTH THERMOMETER PROBE WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE CHAMBER. THE UNIFORMITY WAS MEASURED BETWEEN REFERENCE PROBE AND OTHER PROBES AT THE SAME TIME.

2. REFERENCE STANDARD INSTRUMENTS :-

<u>INSTRUMENT</u>	<u>MODEL</u>	<u>SERIAL No</u>	<u>CERTIFICATE No</u>	<u>DUE DATE</u>
1) DATA LOGGER WITH RTD	HYDRA 2635A	7301307	23T6636	10-Jul-24

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

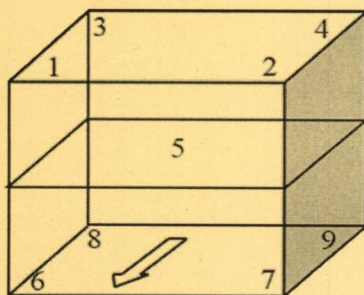

GENERAL INFORMATION

Overall Ambient Temperature around the Chamber (°C) variation : 0
Overall Line Voltage (V) variation : 6
Instrument Condition : Normal
Chamber Size (W*L*H): 55*46*70 cm

CHAMBER PERFORMANCE

Controller Temperature (°C)	Indicating Temperature (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
20.0	20.0	0.26	0.12	0.52

TEMPERATURE MEASUREMENT ACCURACY TEST

Controller Temp (°C)	Indicating Temp (°C)	Measured Temperature (°C) at Spread Locations									Uncertainty (± °C)
		#1	#2	#3	#4	Ref. 5	#6	#7	#8	#9	
20.0	20.0	19.77	19.73	19.72	19.73	19.72	19.73	19.72	19.76	19.78	0.35

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2: LOCATION 5 WAS REFERENCE LOCATION.

NOTE 3 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k =2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



CERTIFICATE No : 24T4143

REFERENCE No : 73037-5

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : HOT AIR OVEN

MANUFACTURER : BINDER

MODEL : FED 53

SERIAL No : 07-29050

ID No : TLC-L004

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : TOPS-LAB CONSULTANTS CO., LTD.
189 MOO.3 BANGRAKPHATTHANA
BANGBUATHONG NONTABURI 11110

CALIBRATED BY :

CALIBRATION DATE :

07-May-24

APPROVED BY :

ISSUED DATE :

09-May-24

RECEIVED DATE :

07-May-24



CERTIFICATE No : 24T4143

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : HOT AIR OVEN
MANUFACTURER : BINDER
MODEL : FED 53
ID No : TLC-L004 S/N : 07-29050
RECEIVED DATE : 07-May-24 CALIBRATION DATE : 07-May-24
AMBIENT TEMPERATURE : 33 °C ± 1 °C RELATIVE HUMIDITY : 56 %RH ± 10 %RH

CONDITION OF THIS RESULTS OF CALIBRATION


1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO TLAS G-20 BY COMPARISON WITH CALIBRATED THERMOCOUPLE TYPE K UNDER NO LOAD CONDITION. THE THERMOCOUPLES WERE PLACED ON NINE POINTS AND LOCATED ONE THERMOCOUPLE IN EACH OF THE EIGHT CORNERS OF THE CHAMBER AND WAS AWAY FROM THE EACH WALL OF 5 cm TO 10 cm. AND PLACED THE NINTH THERMOCOUPLE WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE CHAMBER. THE UNIFORMITY WAS MEASURED BETWEEN REFERENCE PROBE AND OTHER PROBES AT THE SAME TIME.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH TC TYPE K	HYDRA 2635A	7408027	23T6638	10-Jul-24

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

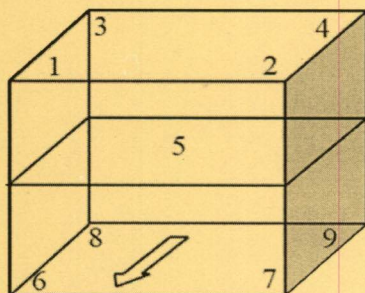

FRONT

GENERAL INFORMATION

Overall Ambient Temperature around the Chamber (°C) variation : 0
Overall Line Voltage (V) variation : 7
Instrument Condition : Normal
Chamber Size (W*L*H): 40*33*40 cm; Vent =1/3

CHAMBER PERFORMANCE

Controller Temperature (°C)	Indicating Temperature (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
104	104	0.26	0.83	1.44
180	180	0.44	1.75	2.20

TEMPERATURE MEASUREMENT ACCURACY TEST

Controller Temp (°C)	Indicating Temp (°C)	Measured Temperature (°C) at Spread Locations									Uncertainty (±°C)
		#1	#2	#3	#4	Ref. 5	#6	#7	#8	#9	
104	104	104.16	103.74	104.06	103.72	104.29	104.64	104.80	103.95	104.21	0.71
180	180	180.78	179.69	179.95	180.48	179.78	181.07	181.25	179.50	180.42	1.1

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2: LOCATION 5 WAS REFERENCE LOCATION.

NOTE 3 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k =2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com



CERTIFICATE No : 24M4140
REFERENCE No : 73037-2

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : ELECTRONIC BALANCE
MANUFACTURER : METTLER TOLEDO
MODEL : AE240-S
SERIAL No : K59437
ID No : TLC-L001
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : TOPS-LAB CONSULTANTS CO., LTD.
189 MOO.3 BANGRAKPHATTHANA
BANGBUATHONG NONTHABURI 11110

CALIBRATED BY :



CALIBRATION DATE :

07-May-24

APPROVED BY :



ISSUED DATE :

09-May-24

RECEIVED DATE :

07-May-24

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.



CERTIFICATE No : 24M4140

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : ELECTRONIC BALANCE MODEL : AE240-S
MANUFACTURER : METTLER TOLEDO S/N : K59437
ID No : TLC-L001 RECEIVED DATE : 07-May-24
AIR PRESSURE : 1014mbar \pm 1mbar CALIBRATION DATE : 07-May-24
AMBIENT TEMPERATURE : 25°C \pm 1°C RELATIVE HUMIDITY : 49 %RH \pm 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 120 g WAS 0.000045 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (\pm g)
0.0	0.0000	0.0000	0.000095
0.1	0.1003	-0.0003	0.000095
0.2	0.2004	-0.0004	0.00010
0.5	0.5005	-0.0005	0.00010
1.0	1.0006	-0.0006	0.00010
2.0	2.0006	-0.0006	0.00010
5.0	5.0008	-0.0008	0.00010
10.0	10.0009	-0.0009	0.00010
20.0	20.0012	-0.0012	0.00011
50.0	50.0015	-0.0015	0.00012
100.0	100.0018	-0.0018	0.00019
120.0	120.0020	-0.0020	0.00019

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	100.0015
2	100.0015
3	100.0015
4	100.0018
5	100.0017
OFF-CENTER LOADING	0.0003

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



CERTIFICATE No : 24T4143

REFERENCE No : 73037-5

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : HOT AIR OVEN

MANUFACTURER : BINDER

MODEL : FED 53

SERIAL No : 07-29050

ID No : TLC-L004

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : TOPS-LAB CONSULTANTS CO., LTD.
189 MOO.3 BANGRAKPHATTHANA
BANGBUATHONG NONTABURI 11110

CALIBRATED BY

:

CALIBRATION DATE

:

07-May-24

APPROVED BY

:

ISSUED DATE

:

09-May-24

RECEIVED DATE

:

07-May-24



CERTIFICATE No : 24T4143

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : HOT AIR OVEN
MANUFACTURER : BINDER
MODEL : FED 53
ID No : TLC-L004 S/N : 07-29050
RECEIVED DATE : 07-May-24 CALIBRATION DATE : 07-May-24
AMBIENT TEMPERATURE : 33 °C ± 1 °C RELATIVE HUMIDITY : 56 %RH ± 10 %RH

CONDITION OF THIS RESULTS OF CALIBRATION


1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO TLAS G-20 BY COMPARISON WITH CALIBRATED THERMOCOUPLE TYPE K UNDER NO LOAD CONDITION. THE THERMOCOUPLES WERE PLACED ON NINE POINTS AND LOCATED ONE THERMOCOUPLE IN EACH OF THE EIGHT CORNERS OF THE CHAMBER AND WAS AWAY FROM THE EACH WALL OF 5 cm TO 10 cm. AND PLACED THE NINTH THERMOCOUPLE WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE CHAMBER. THE UNIFORMITY WAS MEASURED BETWEEN REFERENCE PROBE AND OTHER PROBES AT THE SAME TIME.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH TC TYPE K	HYDRA 2635A	7408027	23T6638	10-Jul-24

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

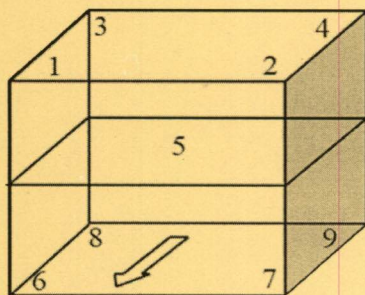

FRONT

GENERAL INFORMATION

Overall Ambient Temperature around the Chamber (°C) variation : 0
Overall Line Voltage (V) variation : 7
Instrument Condition : Normal
Chamber Size (W*L*H): 40*33*40 cm; Vent =1/3

CHAMBER PERFORMANCE

Controller Temperature (°C)	Indicating Temperature (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
104	104	0.26	0.83	1.44
180	180	0.44	1.75	2.20

TEMPERATURE MEASUREMENT ACCURACY TEST

Controller Temp (°C)	Indicating Temp (°C)	Measured Temperature (°C) at Spread Locations									Uncertainty (±°C)
		#1	#2	#3	#4	Ref. 5	#6	#7	#8	#9	
104	104	104.16	103.74	104.06	103.72	104.29	104.64	104.80	103.95	104.21	0.71
180	180	180.78	179.69	179.95	180.48	179.78	181.07	181.25	179.50	180.42	1.1

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2 : LOCATION 5 WAS REFERENCE LOCATION.

NOTE 3 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k =2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com



NSC-TISI-TIS17025
CALIBRATION 0049

CERTIFICATE No : 24T4152

REFERENCE No : 73038-6

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : FREEZER

MANUFACTURER : SANDEN INTERCOOL

MODEL : YPR-068S

SERIAL No : YPR068201S-1011-00028

ID No : TLC-L008

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : TOPS-LAB CONSULTANTS CO., LTD.
189 MOO.3 BANGRAKPHATTHANA
BANGBUATHONG NONTABURI 11110


CALIBRATED BY :



CALIBRATION DATE :

07-May-24

APPROVED BY :

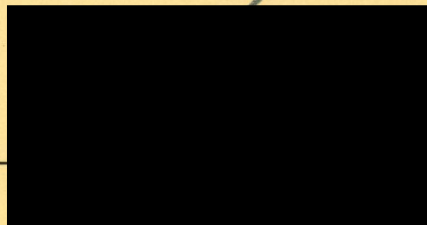

ISSUED DATE :

09-May-24

RECEIVED DATE :

07-May-24

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.



CERTIFICATE No : 24T4152

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : FREEZER
MANUFACTURER : SANDEN INTERCOOL
ID No : TLC-L008
RECEIVED DATE : 07-May-24
AMBIENT TEMPERATURE : 31 °C ± 1 °C

MODEL : YPR-068S
SERIAL NUMBER : YPR068201S-1011-00028
CALIBRATION DATE : 07-May-24
RELATIVE HUMIDITY : 53 %RH ± 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO TLAS G-20 BY COMPARISON WITH CALIBRATED THERMOCOUPLE TYPE K UNDER NO LOAD CONDITION. THE THERMOCOUPLES WERE PLACED ON 13 POINTS AND LOCATED AS THE PICTURE BELOW AND WAS AWAY FROM THE EACH WALL OF 5 cm TO 10 cm. AND PLACED THE SEVENTH THERMOCOUPLE WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE CHAMBER. THE UNIFORMITY WAS MEASURED BETWEEN REFERENCE PROBE AND OTHER PROBES AT THE SAME TIME.

2. REFERENCE STANDARD INSTRUMENTS :-


INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH TC TYPE K	HYDRA 2635A	7903007	23T6640	14-Jul-24

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

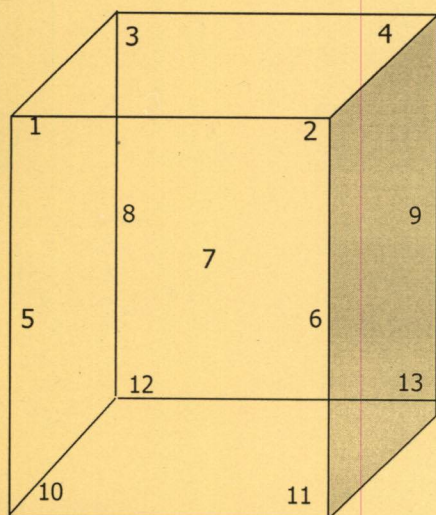

FRONT

GENERAL INFORMATION

Overall Ambient Temperature around the Chamber (°C) variation : 1
Overall Line Voltage (V) variation : 6
Instrument Condition : Normal
Chamber Size (W*L*H): 58*61*138 cm

CHAMBER PERFORMANCE

Controller Temperature (°C)	Indicating Temperature (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
3	3	1.88	1.14	4.39

TEMPERATURE MEASUREMENT ACCURACY TEST

Controller temperature (°C)		3
Indicating Temperature		3
Measured Temperature (°C) at Spread Locations	1	4.13
	2	3.77
	3	3.54
	4	3.76
	5	3.48
	6	3.27
	7 Ref.	3.46
	8	3.00
	9	3.22
	10	3.32
	11	3.88
	12	3.56
	13	3.50
Uncertainty of Measurement(± °C)		2.4

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2 : LOCATION 7 WAS REFERENCE LOCATION.

NOTE 3 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA. THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY COVERAGE FACTOR k=2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert.No.: 25CH351

Page.: 1 of 3

Equipment : pH Meter
Manufacturer : Mettler Toledo
Model : SevenCompact S220
Serial No. : B635935610
ID No. : TLC-L067
Condition As-Received: Used Item
Received Date : 18 March 2025
Calibration Date : 19 March 2025
Reference : 2503-0577DN-1
Submitted by : Tops-Lab Consultants Co.,Ltd.
189 Moo. 3, Bangrakphatthana,
Bangbuathong, Nonthaburi 11110
Ambient Temperature : (25 ± 2.5) °C
Relative Humidity : (50 ± 15) %
Calibration Procedure : In - house method :
- CP-CH5 by direct measurement with DC voltage
standard and direct measurement with
certified reference material (CRM)
- CP-CH8 by comparison with temperature standard

Calibrated by :

Approved by :

Approved Signatory

(✓) Chakrit Waewwanjua
() Ponpan Paipim
() Saithip Meangmai

Issue Date :

20 March 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Cert.No.: 25CH351

Page.: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Document Process Calibrator	54030049	130RC116	24E2759	25 Aug 2025
2) Ref. Standard Thermometer	4982054	110RC044	24I757	14 July 2025

- This Certification is traceable to SI Through Technology Promotion Association (Thailand - Japan)

- 2. Certified Reference Materials** :The measurement results are traceable to SI through Hach Lenge GmbH Ltd.,
Deutsche Akkreditierungsstelle, Accredited No.D-RM-15184-01-00
:The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.007	CPA chem	1066665	18 Jan 2027
pH 6.999	Hach Lenge GmbH	C03220	29 Oct 2026
pH 10.010	CPA chem	1066669	18 Jan 2026

- 3. This certificate is valid only to the item calibrated on date and place of calibration.**

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4,7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (±mV)	Coverage factor <i>k</i>
	pH	mV	mV	pH		
pH Meter S/N.: B635935610	4.000	177.48	177.4	4.000	0.058	2.00
	7.000	0.00	0.0	7.000	0.058	2.00
	10.000	-177.48	-177.4	10.000	0.058	2.00



Cert.No.: 25CH351

Page.: 3 of 3

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (\pm)	Coverage factor k
pH Electrode S/N.: 6455014	4.007	4.008	178.0	0.0044	2.00
	6.999	6.999	2.5	0.0084	2.00
	10.010	10.010	-169.2	0.0065	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : InLabExpert Pro-ISM
- Serial No. : 6455014

Dimension of probe

- Length : 120 mm.
- Diameter : 12 mm.
- Immersion Depth : 100 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (\pm °C)	Coverage factor k
23.0	22.998	23.0	0.002	0.13	2.00
25.0	25.000	25.0	0.000	0.13	2.00
27.0	26.999	27.0	0.001	0.13	2.00

Remark - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-

Certificate of Calibration

Certificate No. : 68-400225-2 **Page : 1 of 2**

Submitted by : Tops-Lab Consultants Co.,Ltd.
189 Moo 3 Bangrakphatthana, Bangbuathong, Nonthaburi 11110

Equipment : Temperature controlled enclosure (Incubator)
 Manufacturer : Aqualytic Model : ET 618-4
 Range : N/A °C Resolution : 0.1 °C
 Serial No. : 0109/13922 ID No. : TLC-L005

Environment : On site calibration was carried out at the Laboratory, Tops-Lab Consultants Co.,Ltd.
 Ambient Temperature : (24.0 to 24.5) °C
 Relative Humidity : (40 to 45) %
 Line Voltage : (220.0 to 228.0) V

Date of Received : 21 April 2025

Date of Calibration : 21 April 2025

Date of Issue : 23 April 2025

Calibrated by : Permpon Chanpu


Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
 Standard Digital Thermometer with RTD Probe

ID No.	Cert. No.	Due Date	Traceability
400029 & 400048	68-400063-1	01 Aug 2025	National Institute of Metrology Thailand (NIMT)

Approved by :



Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 68-400225-2


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

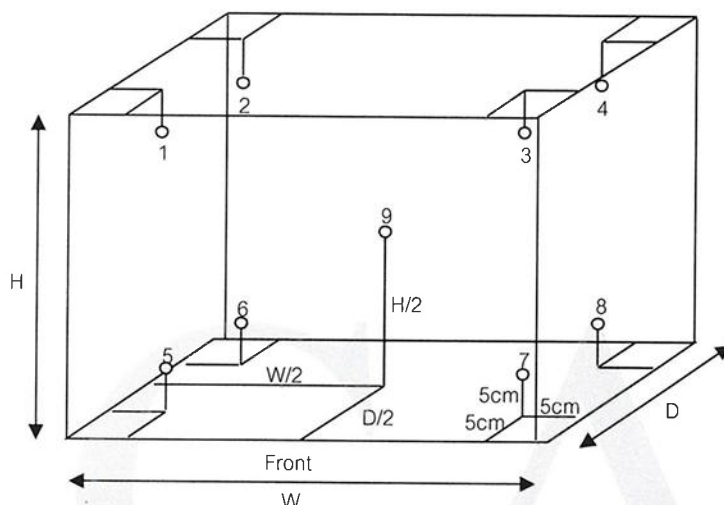

Inside of Chamber

W = 0.55 m

D = 0.48 m

H = 0.72 m

Capacity = 0.19 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
20.0	20.0	20.0	20.02	19.83	19.79	19.82	19.77	19.72	19.85	19.84	19.80	0.58

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
20.0	20.0	20.0	0.32	0.27	0.67

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 68-400225-6

Page : 1 of 2

Submitted by : Tops-Lab Consultants Co., Ltd.
189 Moo 3 Bangrakphatthana, Bangbuathong, Nonthaburi 11110

Equipment : Water Bath
Manufacturer : Memmert Model : WNE 14
Range : N/A °C Resolution : 0.1 °C
Serial No. : L413.1292 ID No. : TLC-L030

Environment : On site calibration was carried out at the Laboratory, Tops-Lab Consultants Co., Ltd.
Ambient Temperature : (32.0 to 34.0) °C
Relative Humidity : (45 to 50) %
Line Voltage : (220.0 to 228.0) V

Date of Received : 21 April 2025

Date of Calibration : 21 April 2025

Date of Issue : 23 April 2025


Calibrated by : Permpon Chanpu

Calibration Method : This instrument was calibrated by In-house method CAL-M4006 based on ASTM E715-80
The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with RTD probe

ID No.	Cert. No.	Due Date	Traceability
400029 & 400031	67-400582-1	24 Apr 2025	National Institute of Metrology Thailand (NIMT)

Approved by :



Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration


Certificate No. : 68-400225-6

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

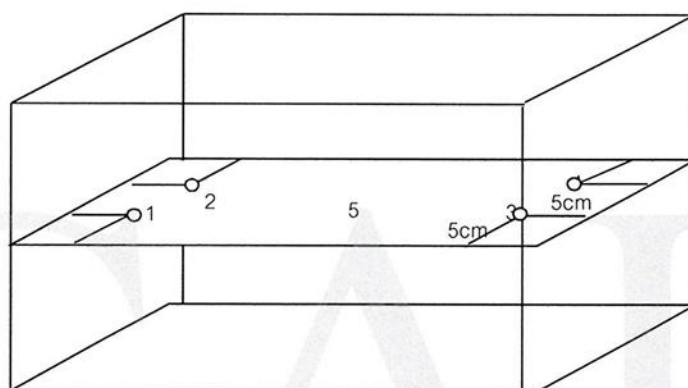

Front

Test Point (° C)	Setting Temperature (° C)	Indicating Temperature (° C)	Measured Temperature (° C) @ Sensor					Uncertainty (± ° C)	Measured Uniformity (° C)	Measured Stability (° C)
			No.							
			1	2	3	4	5			
85.0	85.0	85.0	84.47	84.38	84.43	84.58	84.50	0.24	0.30	0.13
95.0	95.0	95.0	94.45	94.45	94.19	94.09	94.45	0.24	0.49	0.12

Remark The uncertainty is not combine uniformity of the water bath

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 68-400225-1

Page : 1 of 2

Submitted by : Tops-Lab Consultants Co.,Ltd.
189 Moo 3 Bangrakphatthana, Bangbuathong, Nonthaburi 11110

Equipment : Temperature controlled enclosure (Oven)
Manufacturer : Binder Model : FED 53
Range : N/A °C Resolution : 1 °C
Serial No. : 07-29050 ID No. : TLC-L004

Environment : On site calibration was carried out at the Laboratory, Tops-Lab Consultants Co.,Ltd.
Ambient Temperature : (32.0 to 34.0) °C
Relative Humidity : (45 to 50) %
Line Voltage : (220.0 to 228.0) V

Date of Received : 21 April 2025

Date of Calibration : 21 April 2025

Date of Issue : 23 April 2025

Calibrated by : Perinpon Chanpu

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with Thermocouple probe

ID No.	Cert. No.	Due Date	Traceability
400029 & 400032	67-400584-1	29 Apr 2025	National Institute of Metrology Thailand (NIMT)

Approved by :

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 68-400225-1


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

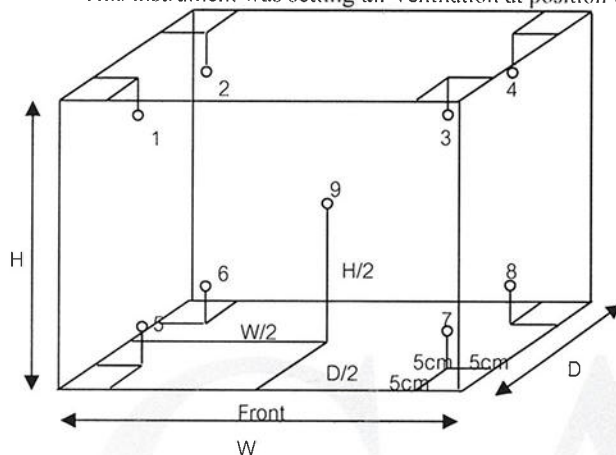

Inside of Chamber

W = 0.40 m

D = 0.33 m

H = 0.40 m

Capacity = 0.05 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
104	104	104	105.5	104.4	103.8	104.0	105.7	104.4	104.3	104.8	104.1	0.97
180	180	180	181.9	179.5	179.3	179.3	182.8	180.7	181.0	181.3	179.7	1.3

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
104	104	104	1.7	0.1	2.2
180	180	180	3.5	0.3	3.9

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2 , providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 68-200133-1

Page : 1 of 2

Submitted by : Tops-Lab Consultants Co.,Ltd.
189 Moo 3 Bangrakphatthana, Bangbuathong, Nonthaburi 11110

Equipment : Electronic Balance
Manufacturer : Mettler Toledo Model : MS205DU
Serial No. : B420605448 ID No. : TLC-L038
Capacity : 220 g Resolution : 82g/0.00001g, 220g/0.0001g

Environment : On site calibration was carried out at the Laboratory, Tops-Lab Consultants Co.,Ltd.
Ambient Temperature : (27.9 to 28.3) °C
Relative Humidity : (48.5 to 52.6) %
Air Pressure : (1009.0 to 1010.0) mbar

Date of Received : 21 April 2025

Date of Calibration : 21 April 2025

Date of Issue : 22 April 2025

Calibrated by : Satja Sangkhum


Calibration Method : In-house method CAL-M2001 based on UKAS Publication ref : LAB 14
Edition 7 - November 2022

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

ID No.	Cert. No.	Due Date	Traceability
E261-E2624	C02242009	07 Nov 2025	National Institute of Metrology (Thailand), (NIMT)

Approved by :

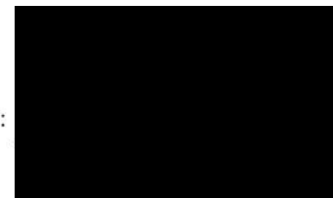

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 68-200133-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Departure of indication from nominal value

Nominal Value (g)	Correction (g)	Uncertainty \pm (g)
0.1	0.00000	0.000014
0.2	0.00000	0.000017
0.5	0.00001	0.000022
1	0.00000	0.000026
2	0.00001	0.000034
5	-0.00001	0.000043
10	0.00000	0.000053
20	-0.00001	0.000071
50	0.00002	0.00011
100	0.0000	0.00020
200	-0.0001	0.00038


This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$, providing a level of confidence of approximately 95%

Eccentric error

Load test : 100 g

A B C D E
0.0002 0.0001 -0.0002 -0.0001 0.0000 g



Repeatability

Load test : 200 g

Stdev. : 0.00005 g

- o0o -

