ภาคผนวก ง

เอกสารสอบเทียบเครื่องมือ

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Ambient									
1	Orifice Transfer Standard Calibrator	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM_{10})	Tisch Environmental,Inc.	TE-5025A 3383	Jiranatee Associates Co., Ltd.	COF-040-68	30 Sep 25	29 Sep 26	-
2	U-Tube Manometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM_{10})	Dwyer	1221-36-W/M -	Technology Promotion Association (Thailand-Japan)	25P3508	9 Sep 25	8 Sep 26	-
3	Aneroid Barometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM_{10})	Barigo, Germany	-	Technology Promotion Association (Thailand-Japan)	26P1519	22 Apr 26	21 Apr 27	-
4	Dial Thermo-Hygrometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM_{10})	Barigo, Germany	-	Technology Promotion Association (Thailand-Japan)	26H710	17 Apr 26	16 Apr 27	-
1	High Volume Air Sampler	Total Suspended Particulate (TSP)	Andersen Instruments, Inc.	GL 2000 H-1 0104-109	Jiranatee Associates Co., Ltd.	Ref. No.3383	30 Sep 25	29 Sep 26	-
2	High Volume Air Sampler	Total Suspended Particulate (TSP)	Andersen Instruments, Inc.	GL 2000 H-1 0104-110	Jiranatee Associates Co., Ltd.	Ref. No.3383	30 Sep 25	29 Sep 26	-
1	High Volume Air Sample	Particulate Matter < 10 µm (PM_{10})	Andersen Instruments, Inc.	IP10 4390	Jiranatee Associates Co., Ltd.	Ref. No.3383	30 Sep 25	29 Sep 26	-
2	High Volume Air Sample	Particulate Matter < 10 µm (PM_{10})	Andersen Instruments, Inc.	IP10 4393	Jiranatee Associates Co., Ltd.	Ref. No.3383	30 Sep 25	29 Sep 26	-
1	Wind Speed/Wind Direction	WS/WD	Scarlet Tech Ltd.	LSI 17037708	Thai Meteorological Department	395/25	22 Aug 25	21 Aug 26	-
2	Wind Speed/Wind Direction	WS/WD	Scarlet Tech Ltd.	LSI 17037713	Thai Meteorological Department	394/25	22 Aug 25	21 Aug 26	-
1	Vibration Meter	Vibration Level Acceleration Level	Instantel Inc.	Micromate UM11229	Calibration Laboratory Co.Ltd	Q25084761	19 Jul 25	18 Jul 26	-
2	Vibration Meter	Vibration Level Acceleration Level	Instantel Inc.	Micromate UM11230	Calibration Laboratory Co.Ltd	Q25149760	23 Dec 25	22 Dec 26	-
3	Vibration Meter	Vibration Level Acceleration Level	Instantel Inc.	Micromate UM11355	Calibration Laboratory Co.Ltd	Q25088636	1 Aug 25	31 Jul 26	-
4	Vibration Meter	Vibration Level Acceleration Level	Instantel Inc.	Micromate UM11356	Calibration Laboratory Co.Ltd	Q25084762	19 Jul 25	18 Jul 26	-
5	Vibration Meter	Vibration Level Acceleration Level	Instantel Inc.	Micromate UM12393	Calibration Laboratory Co.Ltd	Q25084758	19 Jul 25	18 Jul 26	-
6	Vibration Meter	Vibration Level Acceleration Level	Instantel Inc.	Micromate UM12395	Calibration Laboratory Co.Ltd	Q25084756	19 Jul 25	18 Jul 26	-
7	Vibration Meter	Vibration Level Acceleration Level	Instantel Inc.	Micromate UM12866	Calibration Laboratory Co.Ltd	Q25084755	19 Jul 25	18 Jul 26	-
8	Vibration Meter	Vibration Level Acceleration Level	Instantel Inc.	Micromate UM12867	Calibration Laboratory Co.Ltd	Q25088635	1 Aug 25	31 Jul 26	-
9	Vibration Meter	Vibration Level Acceleration Level	Instantel Inc.	Micromate UM12890	Calibration Laboratory Co.Ltd	Q25084760	19 Jul 25	18 Jul 26	-

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Ambient									
10	Vibration Meter	Vibration Level Acceleration Level	Instantel Inc.	Micromate UM13205	Calibration Laboratory Co.Ltd	Q25088632	1 Aug 25	31 Jul 26	-
11	Vibration Meter	Vibration Level Acceleration Level	Instantel Inc.	Micromate UM14106	Calibration Laboratory Co.Ltd	Q25149758	22 Dec 25	21 Dec 26	-
12	Vibration Meter	Vibration Level Acceleration Level	Instantel Inc.	Micromate UM11057	Calibration Laboratory Co.Ltd	Q25084763	19 Jul 25	18 Jul 26	-
1	Sound Level Calibrator (Acoustic Calibrator)	Calibrate Sound Level Meter	Larson Davis	CAL150 6855	Innovative Instrument Co.,Ltd.	25-ACT-137	9 Sep 25	8 Sep 26	-
2	Sound Level Meter	$L_{Aeq\ 24\ hours}$, L_{Amax}, L_{A90}, L_{Adn}	Larson Davis	LxT2 0005286	Innovative Instrument Co.,Ltd.	25-SLM-272	11 Aug 25	10 Aug 27	-
3	Sound Level Meter	$L_{Aeq\ 24\ hours}$, L_{Amax}, L_{A90}, L_{Adn}	Larson Davis	LxT2 0005287	Innovative Instrument Co.,Ltd.	25-SLM-241	29 Jul 25	28 Jul 27	-
4	Sound Level Meter	$L_{Aeq\ 24\ hours}$, L_{Amax}, L_{A90}, L_{Adn}	Larson Davis	LxT2 0005288	Innovative Instrument Co.,Ltd.	25-SLM-242	29 Jul 25	28 Jul 27	-
5	Sound Level Meter	$L_{Aeq\ 24\ hours}$, L_{Amax}, L_{A90}, L_{Adn}	Larson Davis	LxT2 0005298	Electrical And Electronics Institute Foundation For Industrial Development	CP20240341EA	23 Sep 24	22 Sep 26	-
6	Sound Level Meter	$L_{Aeq\ 24\ hours}$, L_{Amax}, L_{A90}, L_{Adn}	Larson Davis	LxT2 0005341	Innovative Instrument Co.,Ltd.	25-SLM-339	9 Oct 25	8 Oct 27	-
7	Sound Level Meter	$L_{Aeq\ 24\ hours}$, L_{Amax}, L_{A90}, L_{Adn}	Larson Davis	LxT2 0005343	Innovative Instrument Co.,Ltd.	25-SLM-340	10 Oct 25	9 Oct 27	-
8	Sound Level Meter	$L_{Aeq\ 24\ hours}$, L_{Amax}, L_{A90}, L_{Adn}	Larson Davis	LxT2 0005349	Innovative Instrument Co.,Ltd.	25-SLM-337	9 Oct 25	8 Oct 27	-
9	Sound Level Meter	$L_{Aeq\ 24\ hours}$, L_{Amax}, L_{A90}, L_{Adn}	Larson Davis	LxT2 0005395	Electrical And Electronics Institute Foundation For Industrial Development	CP20250041EA	3 Feb 25	2 Feb 27	-

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Stack									
1	Pre-Test Console	Total Suspended Particulate Particular Matter (PM_{10})	Apex Instruments, USA.	XC-572-V 0707048	Envi Equipment Service Co., Ltd.	E25-060064	23 Jun 25	22 Jun 26	-
2	Flue gas Analyzer	Sulphur Dioxide Oxide of Nitrogen as Nitrogen Dioxide	Testo	Testo 350 61658806/0419	Entech Industrial Sulution Co., Ltd.	G 250001	7 Jul 25	6 Jul 26	-

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Ambient									
1	Sound Level Calibrator (Acoustic Calibrator)	Calibrate Sound Level Meter	Larson Davis	CAL150 6855	Innovative Instrument Co.,Ltd.	25-ACT-137	9 Sep 25	8 Sep 26	-
2	Sound Level Meter	$L_{Aeq\ 24\ hours}$, L_{Amax}, L_{A90}, L_{Adn}	Larson Davis	LxT2 0005299	Innovative Instrument Co.,Ltd.	25-SLM-273	11 Aug 25	10 Aug 27	-
3	Sound Level Meter	$L_{Aeq\ 24\ hours}$, L_{Amax}, L_{A90}, L_{Adn}	Larson Davis	LxT2 0005328	Electrical And Electronics Institute Foundation For Industrial Development	CP20250040EA	3 Feb 25	2 Feb 27	-
4	Sound Level Meter	$L_{Aeq\ 24\ hours}$, L_{Amax}, L_{A90}, L_{Adn}	Larson Davis	LxT2 0006699	Innovative Instrument Co.,Ltd.	26-SLM-184	12 May 26	11 May 28	-

List of Instruments Certification for Water Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Water									
1	pH Meter	pH	Ecosence	pH100A 24H005160JEN	Technology Promotion Association (Thailand-Japan)	25CH1182	15 Oct 25	14 Oct 26	-
2	DO Meter	DO	Horiba	LAQUA-DO210 HE9M0013	Technology Promotion Association (Thailand-Japan)	25TW236	20 Nov 25	20 Nov 26	-
3	Conductivity Meter	Conductivity	YSI	Pro30 18K100976	Technology Promotion Association (Thailand-Japan)	25CH1183	15 Oct 25	14 Oct 26	-

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Ambient									
1	Sound Level Calibrator (Acoustic Calibrator)	Calibrate Sound Level Meter	Larson Davis	CAL150 6307	Innovative Instrument Co.,Ltd.	25-ACT-136	9 Sep 25	8 Sep 26	-
2	Sound Level Meter	$L_{Aeq\ 24\ hours}$, L_{Amax}, L_{A90}, L_{Adn}	Larson Davis	LxT2 0005286	Innovative Instrument Co.,Ltd.	25-SLM-272	11 Aug 25	10 Aug 27	-
3	Sound Level Meter	$L_{Aeq\ 24\ hours}$, L_{Amax}, L_{A90}, L_{Adn}	Larson Davis	LxT2 0005287	Innovative Instrument Co.,Ltd.	25-SLM-241	29 Jul 25	28 Jul 27	-
4	Sound Level Meter	$L_{Aeq\ 24\ hours}$, L_{Amax}, L_{A90}, L_{Adn}	Larson Davis	LxT2 0005288	Innovative Instrument Co.,Ltd.	25-SLM-242	29 Jul 25	28 Jul 27	-
5	Sound Level Meter	$L_{Aeq\ 24\ hours}$, L_{Amax}, L_{A90}, L_{Adn}	Larson Davis	LxT2 0005299	Innovative Instrument Co.,Ltd.	25-SLM-273	11 Aug 25	10 Aug 27	-

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Ambient									
1	Orifice Transfer Standard Calibrator	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM_{10})	Thermo Scientific	G25A 158M	Jiranatee Associates Co., Ltd.	COF-025-68	21 Jul 25	20 Jul 26	-
2	U-Tube Manometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM_{10})	Dwyer	1221-36-W/M -	Technology Promotion Association (Thailand-Japan)	25P3506	9 Sep 25	8 Sep 26	-
3	Air Flow Meter	Particular Matter ($PM_{2.5}$)	Mesa Labs	DeltaCal DC1 163268	Innovative Instrument Co.,Ltd.	CGF-022-68	15 Oct 25	14 Oct 26	-
4	Aneroid Barometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM_{10}) Particular Matter ($PM_{2.5}$)	Barigo, Germany	-	Technology Promotion Association (Thailand-Japan)	25P1379	17 Apr 25	16 Apr 26	-
5	Dial Thermo-Hygrometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM_{10}) Particular Matter ($PM_{2.5}$)	Barigo, Germany	-	Technology Promotion Association (Thailand-Japan)	25H808	10 Apr 25	9 Apr 26	-
6	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i CM08130002	UAE Consultant Co.,Ltd.	17022026	17 Feb 26	16 Feb 27	-
7	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i CM19050148	UAE Consultant Co.,Ltd.	20022026	20 Feb 26	19 Feb 27	-
8	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i CM19050149	UAE Consultant Co.,Ltd.	24022026	24 Feb 26	23 Feb 27	-
9	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i CM19050150	UAE Consultant Co.,Ltd.	24022026	24 Feb 26	23 Feb 27	-
10	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i CM22177051	UAE Consultant Co.,Ltd.	12122025	12 Dec 25	11 Dec 26	-
11	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i CM22387035	UAE Consultant Co.,Ltd.	17022026	17 Feb 26	16 Feb 27	-
12	Standard Gases (Mixture)	Nitrogen Dioxide	Airgas	EB0162121 2016PSIG	Airgas an Air Liquide company	E05NI91E15A0014	6 Jul 23	6 Jul 31	-

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Ambient									
13	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i CM22387061	UAE Consultant Co.,Ltd.	12022026	12 Feb 26	11 Feb 27	-
14	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i CM22387063	UAE Consultant Co.,Ltd.	23022026	23 Feb 26	22 Feb 27	-
15	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i CM22387065	UAE Consultant Co.,Ltd.	12022026	12 Feb 26	11 Feb 27	-
16	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i CM22387067	UAE Consultant Co.,Ltd.	03032026	3 Mar 26	2 Mar 27	-
17	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i 1200906875	UAE Consultant Co.,Ltd.	23022026	23 Feb 26	22 Feb 27	-
18	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i 1201778111	UAE Consultant Co.,Ltd.	12022026	12 Feb 26	11 Feb 27	-
19	Standard Gases (Mixture)	Sulphur Dioxide	Airgas	EB0162121 2016PSIG	Airgas an Air Liquide company	E05NI91E15A0014	6 Jul 23	6 Jul 31	-
20	Wind Speed/Wind Direction	WS/WD	Scarlet Tech Ltd.	034B / 500 Y11374 / X20002	Thai Meteorological Department	198/26	25 Mar 26	24 Mar 27	-
21	Wind Speed/Wind Direction	WS/WD	LSI Lastem	E-LOG 305 / DNA 821 20020305 / 20040161	Thai Meteorological Department	226/26	17 Apr 26	16 Apr 27	-
22	Wind Speed/Wind Direction	WS/WD	LSI Lastem	E-LOG 305 / DNA 821 20040002 / 20040162	Thai Meteorological Department	232/26	22 Apr 26	21 Apr 27	-
23	Wind Speed/Wind Direction	WS/WD	LSI Lastem	E-LOG 305 / DNA 821 20040004 / 20040163	Thai Meteorological Department	263/26	7 May 26	6 May 27	-
24	Wind Speed/Wind Direction	WS/WD	LSI Lastem	E-LOG 305 / DNA 821 20040005 / 20040164	Thai Meteorological Department	264/26	7 May 26	6 May 27	-
25	Wind Speed/Wind Direction	WS/WD	LSI Lastem	E-LOG 305 / DNA 821 20040006 / 20040165	Thai Meteorological Department	265/26	7 May 26	6 May 27	-

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Ambient									
26	Vibration Meter	Vibration Level Acceleration Level	Instantel Inc.	Micromate UM11229	Calibration Laboratory Co.Ltd	Q25084761	19 Jul 25	18 Jul 26	-
27	Vibration Meter	Vibration Level Acceleration Level	Instantel Inc.	Micromate UM11230	Calibration Laboratory Co.Ltd	Q25149760	23 Dec 25	22 Dec 26	-
28	Vibration Meter	Vibration Level Acceleration Level	Instantel Inc.	Micromate UM11355	Calibration Laboratory Co.Ltd	Q25088636	1 Aug 25	31 Jul 26	-
29	Vibration Meter	Vibration Level Acceleration Level	Instantel Inc.	Micromate UM11356	Calibration Laboratory Co.Ltd	Q25084762	19 Jul 25	18 Jul 26	-
30	Vibration Meter	Vibration Level Acceleration Level	Instantel Inc.	Micromate UM12393	Calibration Laboratory Co.Ltd	Q25084758	19 Jul 25	18 Jul 26	-
31	Vibration Meter	Vibration Level Acceleration Level	Instantel Inc.	Micromate UM12394	Calibration Laboratory Co.Ltd	Q25070066	18 Jun 25	17 Jun 26	-
32	Vibration Meter	Vibration Level Acceleration Level	Instantel Inc.	Micromate UM12395	Calibration Laboratory Co.Ltd	Q25084756	19 Jul 25	18 Jul 26	-
33	Vibration Meter	Vibration Level Acceleration Level	Instantel Inc.	Micromate UM12866	Calibration Laboratory Co.Ltd	Q25084755	19 Jul 25	18 Jul 26	-
34	Vibration Meter	Vibration Level Acceleration Level	Instantel Inc.	Micromate UM12867	Calibration Laboratory Co.Ltd	Q25088635	1 Aug 25	31 Jul 26	-
35	Vibration Meter	Vibration Level Acceleration Level	Instantel Inc.	Micromate UM12888	Calibration Laboratory Co.Ltd	Q25070063	18 Jun 25	17 Jun 26	-
36	Vibration Meter	Vibration Level Acceleration Level	Instantel Inc.	Micromate UM12890	Calibration Laboratory Co.Ltd	Q25084760	19 Jul 25	18 Jul 26	-
37	Vibration Meter	Vibration Level Acceleration Level	Instantel Inc.	Micromate UM12891	Calibration Laboratory Co.Ltd	Q25070068	18 Jun 25	17 Jun 26	-
38	Vibration Meter	Vibration Level Acceleration Level	Instantel Inc.	Micromate UM13204	Calibration Laboratory Co.Ltd	Q25070070	18 Jun 25	17 Jun 26	-

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Ambient									
39	Sound Level Calibrator (Acoustic Calibrator)	Calibrate Sound Level Meter	Larson Davis	CAL150 6855	Innovative Instrument Co.,Ltd.	25-ACT-137	9 Sep 25	8 Sep 27	-
40	Sound Level Meter	$L_{Aeq\ 24\ hours}$, L_{Amax}, L_{A90}, L_{Adn}	Larson Davis	LxT2 0005349	Innovative Instrument Co.,Ltd.	25-SLM-337	9 Oct 25	8 Oct 27	-
41	Sound Level Meter	$L_{Aeq\ 24\ hours}$, L_{Amax}, L_{A90}, L_{Adn}	Larson Davis	LxT2 0006617	Innovative Instrument Co.,Ltd.	25-SLM-338	9 Oct 25	8 Oct 27	-
42	Sound Level Meter	$L_{Aeq\ 24\ hours}$, L_{Amax}, L_{A90}, L_{Adn}	Larson Davis	LxT2 0005286	Innovative Instrument Co.,Ltd.	25-SLM-272	11 Aug 25	10 Aug 27	-
43	Sound Level Meter	$L_{Aeq\ 24\ hours}$, L_{Amax}, L_{A90}, L_{Adn}	Larson Davis	LxT2 0005287	Innovative Instrument Co.,Ltd.	25-SLM-241	29 Jul 25	28 Jul 27	-
44	Sound Level Meter	$L_{Aeq\ 24\ hours}$, L_{Amax}, L_{A90}, L_{Adn}	Larson Davis	LxT2 0005288	Innovative Instrument Co.,Ltd.	25-SLM-242	29 Jul 25	28 Jul 27	-
45	Sound Level Meter	$L_{Aeq\ 24\ hours}$, L_{Amax}, L_{A90}, L_{Adn}	Larson Davis	LxT2 0005299	Innovative Instrument Co.,Ltd.	25-SLM-273	11 Aug 25	10 Aug 27	-
46	Sound Level Meter	$L_{Aeq\ 24\ hours}$, L_{Amax}, L_{A90}, L_{Adn}	Larson Davis	LxT2 0005328	Electrical And Electronics Institute Foundation For Industrial Development	CP20250040EA	3 Feb 25	2 Feb 27	-
47	Sound Level Meter	$L_{Aeq\ 24\ hours}$, L_{Amax}, L_{A90}, L_{Adn}	Larson Davis	LxT2 0005341	Innovative Instrument Co.,Ltd.	25-SLM-339	9 Oct 25	8 Oct 27	-

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Stack									
1	Pre-Test Console	Total Suspended Particulate Xylene Chlorine Hydrogen Chloride Hydrogen Fluoride Hydrogen Sulfide Sulphuric Acid Particulate Matter < 10 µm (PM_{10}) Cresol Antimony Argon Beryllium Cadmium Chromium Copper Lead Magnesium Mercury Nickel Vanadium TOC Cobalt	Apex Instruments, USA.	XC-572-V 0807048	Envi Equipment Service Co., Ltd.	E25-070066	8 Jul 25	7 Jul 26	-
2	Flue gas Analyzer	Sulphur Dioxide Oxide of Nitrogen as Nitrogen Dioxide Carbon Monoxide	Testo	Testo 350 61658783/0419	Entech Industrial Sulution Co., Ltd.	G 250285	30 Oct 25	29 Oct 26	-

List of Opacity Training Certification for Opacity Mesurement

No.	Name	Training Couse	Train	Date	Remark
1	Mr.Theerawat Martphosri	Opacity	Pollution Control Department	30-31 March 2017	-
2	Mr.Akawut Sanoejai	Opacity	Pollution Control Department	28-29 March 2019	-
3	Mr.Apiwich Toungtee	Opacity	Pollution Control Department	12-13 March 2015	-
4	Mr.Kannikorn Raso	Opacity	Pollution Control Department	30-31 March 2017	-
5	Mr.Pongthep Laokajorn	Opacity	Pollution Control Department	12-13 March 2015	-
6	Mr.Suksan Pansing	Opacity	Pollution Control Department	29-31 August 2007	-
7	Mr.Ronnapob Putragulpattana	Opacity	Pollution Control Department	22-23 March 2018	-

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
53/4 PATTANAKARN ROAD SOI 15, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9494

Certificate of Calibration

Certificate No. : 25P3505
Page : 1 of 2

Equipment : U-Tube Manometer
Manufacturer: Dwyer
Model : 1221-36-W/M
Serial No.: -
ID No.: UAE.EFM.020/2560
Condition As-Received: Used Item
Received Date: 03 September 2025
Calibration Date: 09 September 2025

Reference: 2509-0144/WSC
Ambient Temperature: (23 ± 2) °C
Relative Humidity: (50 ± 15) %
Atmospheric Pressure: 1010 mbar

Submitted by: United Analyst and Engineering Consultant Co.,Ltd.
81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to calibration procedure CP-P04, using " DKD-R 6-1 ; Calibration of Pressure Gauges " as a guidelines.

Condition of this result of calibration

1.Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Pressure Calibrator	PC106P	1189	MP-0218-24	24 Sep 2025

2.This result of calibration was made on requested at the point specified by customer.
3.Scale and conversion factor is 1 kPa = 4.0146293 inH₂O
4.This instrument was used clean air as pressure media.
5.This instrument was calibrated by applied pressure to high-port (+) side and low-port (-) side open to atmospheric pressure.
6.This instrument was installed in vertical orientation and top of the pressure port was used as the reference level.
7.The certificate is valid only to the item calibrated on date and place of calibration.
8.This measurement result is traceable to the International System of Unit maintained through:-
-National Institute of Metrology (Thailand), NSC-ONSC Accredited No. Calibration 0144

Calibrated by : Suksan Khankaew
Issue Date : 10 September 2025

Approved Signatory : Attapol P
[ ] Phatinee Prabpaipal
[ ] Sura Suwannasri
[√] Attapol Panurach

เอกสารไม่ควบคุม

THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 25 March, 2026

Certification No. 198/26

Page : 1 of 2

Object : Weather Station

Manufacturer : Met One Instruments

Type : Data Logger 580 Wind Sensor 034B

Serial No. : Data Logger X20002 Wind Sensor Y11374

Customer : United Analyst and Engineering Consultant Co.,Ltd.
81 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Prakanong, Bangkok 10260.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1009.2 hPa

NATIONAL STANDARD WIND TUNNEL :
: Micromanometer Theodor Friedrichs FC014 Serial No. 9310119
: HOOK GAGE NO 1425 Pitot Tube Theodor Friedrichs Type 0800.0000 serial 9023
N.I.S.T. Test Reference Number 731/241460 : Standard Velocity at 20 - 30 m/sec
: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)
Serial Number 110730029 (sensor 120629586)
JAPAN QUALITY ASSURANCE ORGANIZATION : Standard Velocity at 0 - 20 m/sec

Calibrated by : Watcharapol Subwat
Mr. Watcharapol Subwat
Mechanical Engineer

Signed :
Mr. Pisood Promsut
(Authorised Signatory)
for the Chief
Sub-Standard Instrument

เอกสารไม่ควบคุม

Cert.No.: 25P3505
Page: 2 of 2

Result of calibration:- Without adjustment
Function:- Pressure Measurement
Increasing Pressure

Range : 0 inH₂O to 36 inH₂O
Scale Interval : 0.1 inH₂O (The Second Estimate)

Applied Pressure	UUC Indication High-port side	UUC Indication Low-port side	ΔP	Error
0.00	0.00	0.00	0.00	0.00
2.00	0.95	-1.05	2.00	0.00
4.00	1.95	-2.05	4.00	0.00
6.00	2.95	-3.05	6.00	0.00
8.00	3.95	-4.05	8.00	0.00
10.00	4.95	-5.05	10.00	0.00
12.00	5.95	-6.05	12.00	0.00
14.00	7.00	-7.05	14.05	0.05
16.00	8.00	-8.05	16.05	0.05
18.00	9.00	-9.10	18.10	0.10
20.00	10.00	-10.10	20.10	0.10
22.00	11.05	-11.10	22.15	0.15
24.00	12.05	-12.10	24.15	0.15
26.00	13.05	-13.10	26.15	0.15
28.00	14.05	-14.10	28.15	0.15
30.00	15.05	-15.05	30.10	0.10
32.00	16.10	-16.05	32.15	0.15
34.00	17.10	-17.05	34.15	0.15
35.70	18.00	-17.90	35.90	0.20

The uncertainty of measurement was ± 0.11 inH₂O
* ΔP = High-port side - Low-port side
* UUC = Unit Under Calibration
The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95 %.

-000-

เอกสารไม่ควบคุม

THAI METEOROLOGICAL DEPARTMENT
4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration

Certification No. 198/26

25 March, 2026

Page : 2 of 2

Standard	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
Ultrasonic Anemometer	Pressure	Vacumm	Velocity	Velocity	Correction
m/sec	inches H2O	inches H2O	m/sec	m/sec	m/sec
1.00	-	-	-	0.9	0.0
3.02	-	-	-	3.0	0.02
5.00	-	-	-	5.0	0.0
7.00	-	-	-	7.0	0.0
9.02	-	-	-	9.0	0.02
11.01	-	-	-	11.0	0.01
13.01	-	-	-	12.9	0.11
15.01	-	-	-	15.0	0.01
17.02	-	-	-	17.0	0.02
20.02	-	-	-	20.1	-0.08

Vane Angel Bench Stand Model 18112
Young Meteorological Instruments

WIND DIRECTION	TESTED WIND DIRECTION
0	0
90	91
180	179
270	270

Calibrated by : Watcharapol
Mr. Watcharapol Subwat
Mechanical Engineer

Calibration & Test Section
Meteorological Instruments Bureau

เอกสารไม่ควบคุม

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484

Certificate of Calibration

Certificate No. : 26H710
Page : 1 of 2

Equipment :	Dial Thermo-Hygrometer
Manufacturer:	Barigo
Model :	-
Serial No.:	-
ID No.:	UAE.ANV.004/2548
Condition As-Received:	Used Item
Received Date:	10 April 2026
Calibration Date:	17 April 2026 to 22 April 2026
Reference:	2604-0315WSC
Ambient Temperature:	(25 ± 3) °C
Relative Humidity:	(50 ± 20) %

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

Submitted by: United Analyst and Engineering Consultant Co.,Ltd.
81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Procedure used: Calibration were conducted using in-house calibration procedure CP-H02 according to comparison with standard chilled mirror sensor for humidity measurement function and comparison with standard temperature probe for temperature measurement function into humidity / temperature chamber.

Condition of this result of calibration

1.Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Chilled-Mirror Hygrometer	Dew Master	41292	23277	06 May 2026
2) Handheld Thermometer With Sensor	1523	5717096	25I1200	21 Nov 2026

2.The certificate is valid only to the item calibrated on date and place of calibration.

3.This measurement result is traceable to the International System of Unit maintained through:-

-Thunder Scientific Corporation, NVLAB Accreditation No. Calibration 200582-0

-Technology Promotion Association (Thailand-Japan), NSC-ONSC Accredited No. Calibration 0008

Calibrated by : Kraipop Onrat
Issue Date : 23 April 2026

Approved Signatory : Viporn
[ ] Chakrit Waewwanjua
[ ] Pornthippa Tameyakul
[✓] Viporn Tantiyawutti

เอกสารไม่ควบคุม

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484

Certificate of Calibration

Certificate No. : 26P1519
Page : 1 of 2

Equipment :	Anéroid Barometer
Manufacturer:	Barigo
Model :	-
Serial No.:	-
ID No.:	UAE.ANV.123/2550
Condition As-Received:	Used Item
Received Date:	10 April 2026
Calibration Date:	22 April 2026
Reference:	2604-0316WSC
Ambient Temperature:	(23 ± 2) °C
Relative Humidity:	(50 ± 15) %

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

Submitted by: United Analyst and Engineering Consultant Co.,Ltd.
81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to calibration procedure CP-P10, using " DKD-R 6-1 ; Calibration of Pressure Gauges " as a guidelines.

Condition of this result of calibration

1.Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Pressure Indicator	DPI142	1422505046	MP-0150-25	20 May 2026

2.This result of calibration was made on requested at the point specified by customer.

3.The certificate is valid only to the item calibrated on date and place of calibration.

4.This measurement result is traceable to the International System of Unit maintained through:-

-National Institute of Metrology Thailand (NIMT)

Calibrated by : Somchai Chaichan
Issue Date : 24 April 2026

Approved Signatory : S Sm
[ ] Phalinee Prabpalpal
[✓] Sura Suwannasri
[ ] Attapol Panurach

เอกสารไม่ควบคุม

Result of Calibration:- Without Adjustment
Function: Humidity Measurement.

Reference Temperature (°C)	Standard Humidity (%R.H.)	UUC* Reading (%R.H.)	UUC* Correction (%R.H.)	Uncertainty of Measurement (±%R.H.)
25.0	40.1	40	0.1	1.6
25.0	60.0	60	0.0	1.7
25.0	80.0	78	2.0	1.9

Result of Calibration:- Without Adjustment
Function: Temperature Measurement.

Standard Temperature (°C)	UUC* Reading (°C)	UUC* Correction (°C)	Uncertainty of Measurement (±°C)
20.012	20.5	-0.488	0.65
25.028	25.0	0.028	0.65
30.005	30.0	0.005	0.65
35.019	35.0	0.019	0.65
40.040	39.5	0.540	0.65

UUC* : Unit Under Calibration
The reported uncertainty of measurement was base on standard uncertainty multiplied by coverage factor k = 2.00, providing confidence level approximately 95%.

-o0o-

เอกสารไม่ควบคุม

Technical information and UUC* settings during calibration:

Result of calibration	: Without adjustment	**Range**	: 960 hPa to 1030 hPa
Pressure type	: Absolute Pressure	**Scale Interval:**	1 hPa (The Fifth Estimate)
Installation	: Vertical Orientation	**Pressure medium**	: Clean air
Atmospheric pressure	: (1008 ± 10) mbar	**Reference level**	: at the center of the dial

Increasing Pressure

Applied Pressure (hPa)	954.50	966.01	977.33	988.29	999.08	1010.17	1021.66	1032.68
UUC* Indication (hPa)	960.0	970.0	980.0	990.0	1000.0	1010.0	1020.0	1030.0
Error (hPa)	5.50	3.99	2.67	1.71	0.92	-0.17	-1.66	-2.68

Decreasing Pressure

Applied Pressure (hPa)	1032.67	1021.79	1010.29	999.07	988.40	977.64	965.87	954.39
UUC* Indication (hPa)	1030.0	1020.0	1010.0	1000.0	990.0	980.0	970.0	960.0
Error (hPa)	-2.67	-1.79	-0.29	0.93	1.60	2.36	4.13	5.61

The uncertainty of measurement was ± 0.25 hPa

* UUC = Unit Under Calibration
The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม

JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd.
63/34-35, 6770-86
Petchkasem 7,7/1, Rd. Bratthayang, Bangkruai,
Bangkok 10530(Thailand)
Tel: +66(0)8
Mobile: +66(0)2
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Flow measurement laboratory
Calibration services department.

ilac-MRA THAILAND NSC – TISI – TIS 17025 CALIBRATION 0367

CERTIFICATE OF CALIBRATION

Certificate No. : COF-040-68

MEASUREMENT ITEM	: Top Load Orifice
MANUFACTURER	: TSCH
MODEL/TYPE	: TF-5025A
SERIAL NUMBER	: 3383
ID NUMBER	: UAE.EFM.063/2580
CONDITION AS-RECEIVED	: Used item
CUSTOMER	: United Analyst and Engineering Consultant Co., Ltd. 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakhanong, Bangkok 10260
RECEIVED DATE	: 29 Aug 2025
MEASUREMENT DATE	: 29 Sep 2025
ISSUE DATE	: 30 Sep 2025

Calibration procedure:
The Orifice gas flow device was calibrated against Standard Rotary Displacement Meter (Roots Meter) Model G65/IMC/AD-sp. The MB CL-004 was used as a calibration guideline.

Traceability:
This certificate provides a traceability of the measurement to recognized the national standards, and to realization of the International system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MM.0016.25.

Uncertainty of Measurement:
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

ENVIRONMENTAL CONDITIONS:
Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 2.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa

CALIBRATION CONDITION:

Preconditioning	: 24 hours at ambient conditions.
Measurement Condition	: The average values during measurement are 23.2 °C and 55.9 %RH.

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:
The table on next page give the measured values.

Calibrated by:
☐ Mr. Sorawit Thuchalad
☑ Miss Ittraporn Letsomphol

Approved signatory: .....
Mr. Parinya Booncharoen
Calibration Department Manager

เอกสารไม่ควบคุม

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR RE... IN WRITING FROM THE LABORATORY

Jiranatee Associates Co.,Ltd.

JIRANATEE ASSOCIATES CO.,LTD.

Continuation of Certificate of Calibration Number COF-040-68

MEASUREMENT RESULTS:

The Orifice gas flow device was calibrated by direct comparison method with the Standard Rotary Displacement Meter (Roots Meter). The humid air was used as a medium in the system. The standard conditions are 25°C (298.15 K) and 760 mmHg for standard temperature and standard pressure respectively.

Table 1: The results of Q standard calibration data

Plate	Flow rate m^3/min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Δp_meter mmHg	Δp_Orifice inH2O	F	Standard Flow [Q_s] m^3/min
1	0.704	753.311	22.97	22.08	56.514	1.512	1.228	0.602
2	1.001	753.266	22.99	22.37	62.412	3.014	1.734	0.918
3	1.116	753.254	23.06	22.48	41.501	3.969	1.990	1.054
4	1.164	753.258	23.09	22.55	29.909	4.404	2.101	1.117
5	1.410	753.191	23.04	22.66	28.108	6.537	2.554	1.356

Slope (m): 1.87959
Intercept (b): 0.00567
Correlation coefficient (r): 0.99982
Uncertainty (k=2): 0.015 m^3/min

Table 2: The results of Q actual calibration data

Plate	Flow rate m^3/min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Δp_meter mmHg	Δp_Orifice inH2O	F	Standard Flow [Q_a] m^3/min
1	0.704	753.311	22.97	22.08	56.514	1.512	0.771	0.655
2	1.001	753.266	22.99	22.37	62.412	3.014	1.088	0.920
3	1.116	753.254	23.06	22.48	41.501	3.969	1.249	1.056
4	1.164	753.258	23.09	22.55	29.909	4.404	1.319	1.120
5	1.410	753.191	23.04	22.66	28.108	6.537	1.603	1.359

Slope (m): 1.17726
Intercept (b): 0.00356
Correlation coefficient (r): 0.99982
Uncertainty (k = 2): 0.015 m^3/min

End of Certificate of Calibration

เอกสารไม่ควบคุม

THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 22 August, 2025 Certification No. 394/25

Object : เครื่องมือตรวจวัดอุตุนิยมวิทยา

Manufacturer : LSI

Type : Data Logger E-LOG 305 Wind speed DNA202 Wind direction DNA212
Thermoigrometers DMA672.1 Barometer DQA 240.1

Mfg Code : Data Logger 17037713 Wind speed BQ1705627 Wind direction19050292
Thermoigrometers 24070483 Barometer R1605257

Customer : United Analyst and Engineering Consultant Co.,Ltd.
81 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Prakanong, Bangkok 10260.

Calibration Condition : Temperature 25.1 ° C Barometric Pressure 1010.5 hPa

NATIONAL STANDARD WIND TUNNEL : Vane Angel Bench Stand Model 18112
: Micromanometer Theodor Friedrichs FC014 Serial No. 9310119 : HOOK GAGE NO 1425
N.I.S.T. Test Reference Number 731/241460 : Standard Velocity at 20 - 30 m/sec
: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)
Serial Number 110730029 (sensor 120529586)
JAPAN QUALITY ASSURANCE ORGANIZATION : Standard Velocity at 0 - 20 m/sec
STANDARD THERMOMETER : Theodor Friedrich : Dry No.8390/94 Wet No. 8389/94
: Thermoschneider No.9188 : testo, testo 645 Serial No. 02848057
STANDARD BAROMETER : Digital Barometer Vaisala Type PTB220 No. V1260015

Calibrated by : Watcharapol Signed : Pigood Promsut
Mr. Watcharapol Subwat
Mechanical Engineer

(Authorised Signatory)
for the Chief
Sub-Standard Instrument

เอกสารไม่ควบคุม

THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration

Certification No. 394/25

22 August, 2025

Standard	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
Ultrasonic Anemometer	Pressure	Vacumm	Velocity	Velocity	Correction
m/sec	inches H20	inches H20	m/sec	m/sec	m/sec
1.00	-	-	-	1.0	0.00
3.02	-	-	-	3.0	0.02
5.00	-	-	-	5.0	0.00
7.04	-	-	-	7.0	0.04
9.02	-	-	-	9.0	0.02
11.02	-	-	-	10.9	0.12
13.01	-	-	-	13.0	0.01
15.01	-	-	-	14.9	0.11
17.02	-	-	-	17.0	0.02
20.02	-	-	-	19.9	0.12

Vane Angel Bench Stand Model 18112
Young Meteorological Instruments

WIND DIRETION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	270

Calibrated by : Watcharapol
Mr. Watcharapol Subwat
Mechanical Engineer

Calibration & Test Section
Meteorological Instruments Bureau

เอกสารไม่ควบคุม

THAI METEOROLOGICAL DEPARTMENT
4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration

Certification No. 394/25

22 August, 2025 Page : 3 of 7

Standard Barometer Pressure	Tested Barometer Pressure	Correction
1009.20	1008.98	0.22
1009.04	1008.85	0.19
1008.82	1008.72	0.10
1008.65	1008.58	0.07
1008.46	1008.45	0.01
1008.15	1008.05	0.10
1007.64	1007.52	0.12
1007.43	1007.25	0.18
1007.27	1007.12	0.15
1007.04	1006.98	0.06
1006.43	1006.32	0.11
1006.21	1006.18	0.03
1008.62	1008.45	0.17
1008.41	1008.32	0.09
1008.09	1008.05	0.04
1007.58	1007.52	0.06
1007.32	1007.25	0.07
1007.12	1006.98	0.14
1006.84	1006.72	0.12
1006.28	1006.18	0.10

Average

Calibrated by :
Mr. Watcharapol Subwat
Mechanical Engineer

Calibration & Test Section
Meteorological Instruments Bureau

เอกสารไม่ควบคุม

THAI METEOROLOGICAL DEPARTMENT
4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration

Certification No. 394/25

22 August, 2025 Page : 5 of 7

Standard Temp. °C	Temperature Sensor Reading	
	Reading °C	Correction °C
45.14	45.21	-0.07
30.25	30.31	-0.06
15.24	15.32	-0.08

Calibrated by :
Mr. Watcharapol Subwat
Mechanical Engineer

Calibration & Test Section
Meteorological Instruments Bureau

เอกสารไม่ควบคุม

THAI METEOROLOGICAL DEPARTMENT
4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration

Certification No. 394/25

22 August, 2025 Page : 4 of 7

Standard Barometer Pressure	Tested Barometer Pressure	Correction
756.96	756.8	0.16
756.84	756.7	0.14
756.68	756.6	0.08
756.55	756.5	0.05
756.41	756.4	0.01
756.17	756.1	0.07
755.79	755.7	0.09
755.63	755.5	0.13
755.51	755.4	0.11
755.34	755.3	0.04
754.88	754.8	0.08
754.72	754.7	0.02
756.53	756.4	0.13
756.37	756.3	0.07
756.13	756.1	0.03
755.75	755.7	0.05
755.55	755.5	0.05
755.40	755.3	0.10
755.19	755.1	0.09
754.77	754.7	0.07

Average

Calibrated by :
Mr. Watcharapol Subwat
Mechanical Engineer

Calibration & Test Section
Meteorological Instruments Bureau

เอกสารไม่ควบคุม

THAI METEOROLOGICAL DEPARTMENT
4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration

Certification No. 394/25

22 August, 2025 Page : 6 of 7

Standard Humidity % R.H.	Relative Humidity Sensor Reading	
	Reading % R.H.	Correction % R.H.
95.53	97.6	-2.07
65.24	66.5	-1.26
44.12	44.9	-0.78

Calibrated by :
Mr. Watcharapol Subwat
Mechanical Engineer

Calibration & Test Section
Meteorological Instruments Bureau

เอกสารไม่ควบคุม

Date of Issue 22 August, 2025 Certification No. 394/25

Page: 7 of 7

ใบรับรอง

หนังสือฉบับนี้ขอรับรองว่า เครื่องวัดฝน ยี่ห้อ LSI LASTEM แบบ TIPPING BUCKET Code. DQA230.1 Serial No.19050180 ทำการสอบเทียบกับแก้ววัดฝนแบบแก้วคาง GAUGE DIAMETER 8.0 INCHES, NEGRETTI & ZAMBRA LONDON No. 71082 และสามารถนำไปใช้ได้ มีค่าถูกต้องตามรายละเอียดของเครื่องมือ (0.2 mm/TIP)

ลงชื่อ.....

(นายวัชรพล ทรัพย์วัฒน์)

วิศวกรชำนาญการ

เอกสารไม่ควบคุม

THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration

Certification No. 395/25

22 August, 2025 Page : 2 of 7

Standard	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
Ultrasonic Anemometer	Pressure	Vacumen	Velocity	Velocity	Correction
m/sec	inches H2O	inches H2O	m/sec	m/sec	m/sec
1.00	-	-	-	1.0	0.00
3.02	-	-	-	2.9	0.12
5.00	-	-	-	5.0	0.00
7.04	-	-	-	6.9	0.14
9.02	-	-	-	9.0	0.02
11.02	-	-	-	10.9	0.12
13.01	-	-	-	13.0	0.01
15.01	-	-	-	14.9	0.11
17.02	-	-	-	17.0	0.02
20.02	-	-	-	19.9	0.12

Vane Angel Bench Stand Model 18112 Young Meteorological Instruments	
WIND DIRETION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	270

Calibrated by : Watcharapol

Mr. Watcharapol Subwat

Mechanical Engineer

Calibration & Test Section

Meteorological Instruments Bureau

เอกสารไม่ควบคุม

THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 22 August, 2025 Certification No. 395/25

Page : 1 of 7

Object : เครื่องมือตรวจวัดอุตุนิยมวิทยา

Manufacturer : LSI

Type : Data Logger E-LOG 305 Wind speed DNA202 Wind direction DNA212
Thermolgrometers DMA672.1 Barometer DQA 240.1

Mfg Code : Data Logger 17037708 Wind speed BQ1705625 Wind direction19020250
Thermolgrometers 24070579 Barometer R1605260

Customer : United Analyst and Engineering Consultant Co.,Ltd.
81 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Prakanong, Bangkok 10260.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1009.9 hPa

NATIONAL STANDARD WIND TUNNEL : Vane Angel Bench Stand Model 18112
: Micromanometer Theodor Friedrichs FC014 Serial No. 9310119 : HOOK GAGE NO 1425
N.I.S.T. Test Reference Number: 731/241460 : Standard Velocity at 20 - 30 m/sec
: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)
Serial Number 110730029 (sensor 120629586)
JAPAN QUALITY ASSURANCE ORGANIZATION : Standard Velocity at 0 - 20 m/sec
STANDARD THERMOMETER : Theodor Friedrich : Dry No.8390/94 Wet No. 8389/94
: Thermoschneider No.9188 : testo, testo 645 Serial No. 02848057
STANDARD BAROMETER : Digital Barometer Vaisala Type PTB220 No. V1220015

Calibrated by : Watcharapol
Mr. Watcharapol Subwat
Mechanical Engineer

Signed : Pisood
Mr. Pisood Promsut
(Authorised Signatory)
for the Chief
Sub-Standard Instrument

เอกสารไม่ควบคุม

THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration

Certification No. 395/25

22 August, 2025 Page : 3 of 7

Standard Barometer	Tested Barometer	Correction
Pressure	Pressure	
1009.20	1009.12	0.08
1009.04	1008.98	0.06
1008.82	1008.85	-0.03
1008.65	1008.72	-0.07
1008.46	1008.45	0.01
1008.15	1008.18	-0.03
1007.64	1007.52	0.12
1007.43	1007.38	0.05
1007.27	1007.25	0.02
1007.04	1006.98	0.06
1006.43	1006.45	-0.02
1006.21	1006.32	-0.11
1008.62	1008.58	0.04
1008.41	1008.32	0.09
1008.09	1008.05	0.04
1007.58	1007.52	0.06
1007.32	1007.25	0.07
1007.12	1006.98	0.14
1006.84	1006.85	-0.01
1006.28	1006.32	-0.04

Average

Calibrated by : Watcharapol

Mr. Watcharapol Subwat

Mechanical Engineer

Calibration & Test Section

Meteorological Instruments Bureau

เอกสารไม่ควบคุม

THAI METEOROLOGICAL DEPARTMENT
4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration

Certification No. 395/25

22 August, 2025 Page : 4 of 7

Standard Barometer Pressure	Tested Barometer Pressure	Correction
756.96	756.9	0.06
756.84	756.8	0.04
756.68	756.7	-0.02
756.55	756.6	-0.05
756.41	756.4	0.01
756.17	756.2	-0.03
755.79	755.7	0.09
755.63	755.6	0.03
755.51	755.5	0.01
755.34	755.3	0.04
754.88	754.9	-0.02
754.72	754.8	-0.08
756.53	756.5	0.03
756.37	756.3	0.07
756.13	756.1	0.03
755.75	755.7	0.05
755.55	755.5	0.05
755.40	755.3	0.10
755.19	755.2	-0.01
754.77	754.8	-0.03
	Average	0.03

Calibrated by :
Mr. Watcharapol Subwat
Mechanical Engineer

Calibration & Test Section
Meteorological Instruments Bureau

เอกสารไม่ควบคุม

THAI METEOROLOGICAL DEPARTMENT
4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration

Certification No. 395/25

22 August, 2025 Page : 6 of 7

Standard Humidity % R.H.	Relative Humidity Sensor Reading	
	Reading % R.H.	Correction % R.H.
95.53	97.1	-1.57
65.24	66.1	-0.86
44.12	44.5	-0.38

Calibrated by :
Mr. Watcharapol Subwat
Mechanical Engineer

Calibration & Test Section
Meteorological Instruments Bureau

เอกสารไม่ควบคุม

THAI METEOROLOGICAL DEPARTMENT
4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration

Certification No. 395/25

22 August, 2025 Page : 5 of 7

Standard Temp. °C	Temperature Sensor Reading	
	Reading °C	Correction °C
45.14	45.24	-0.10
30.25	30.34	-0.09
15.24	15.29	-0.05

Calibrated by :
Mr. Watcharapol Subwat
Mechanical Engineer

Calibration & Test Section
Meteorological Instruments Bureau

เอกสารไม่ควบคุม

Date of Issue 22 August, 2025 Certification No. 395/25

Page: 7 of 7

ใบรับรอง

หนังสือฉบับนี้ขอรับรองว่า เครื่องวัดฝน ยี่ห้อ LSI LASTEM แบบ TIPPING BUCKET Code. DQA230,1#C Serial No.PC1705209 ทำการสอบเทียบกับแก้ววัดฝนแบบแก้วควง GAUGE DIAMETER 8.0 INCHES, NEGRETTI & ZAMBRA LONDON No. 71082 และสามารถนำไปใช้ได้ มีค่าถูกต้องตามรายละเอียดของเครื่องมือ (0.2 mm/TIP)

ลงชื่อ.....

(นายวัชรพล ทรัพย์วัฒน์)

วิศวกรชำนาญการ

เอกสารไม่ควบคุม

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE	:	VIBRATION METER
MANUFACTURER	:	INSTANTEL
MODEL / TYPE	:	721A2501/721A2901
SERIAL NO.	:	UM12890/UM12890 [UAE.EFM.026/2561]
CLID. NO.	:	251900038
JOB CONTROL NO.	:	250719084760
CALIBRATION SERVICE	:	☑ IN-LABORATORY ☐ ON-SITE

CUSTOMER : UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,
BANGCHAK, PHRAKHANONG, BANGKOK 10260

DATE OF RECEIVED : 19 July 2025 DATE OF ISSUED : 24 July 2025

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Suwit Phuanbusabong
Calibration Engineer

Approved By : Mongkol Yotsoontorn
Authorized Signatory
24 July 2025

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q25084760
F3-011-05/12-23

เอกสารไม่ควบคุม

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com

CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment ( ) adjustment

CALIBRATION DATA

1. ACCELERATION RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
(g)	(frequency)		(g)	(g)	(g)	±(% of rdg.)
0.3	50 Hz	peak	0.300	0.298	+0.002	1.9
0.4	50 Hz		0.400	0.397	+0.003	1.3
0.5	50 Hz		0.500	0.495	+0.005	1.3
0.6	50 Hz		0.600	0.592	+0.008	2.5
0.7	50 Hz		0.700	0.689	+0.011	2.5
0.3	100 Hz	peak	0.300	0.299	+0.001	1.9
0.4	100 Hz		0.400	0.397	+0.003	1.3
0.5	100 Hz		0.500	0.495	+0.005	1.3
0.6	100 Hz		0.600	0.593	+0.007	2.5
0.7	100 Hz		0.700	0.691	+0.009	2.5

2. VELOCITY RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
(mm/s)	(frequency)		(mm/s)	(mm/s)	(mm/s)	±(% of rdg.)
3	50 Hz	peak	3.000	3.023	-0.023	1.8
4	50 Hz		4.000	4.043	-0.043	1.8
5	50 Hz		5.000	5.052	-0.052	1.8
6	50 Hz		6.000	6.063	-0.063	1.8
7	50 Hz		7.000	7.072	-0.072	1.8
3	100 Hz	peak	3.000	3.008	-0.008	2.7
4	100 Hz		4.000	4.012	-0.012	1.3
5	100 Hz		5.000	5.019	-0.019	1.3
6	100 Hz		6.000	6.023	-0.023	1.0
7	100 Hz		7.000	7.031	-0.031	1.0

Certificate No. Q25084760
F3-011-05/12-23

เอกสารไม่ควบคุม

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com

REPORT OF CALIBRATION

FOR

NOMENCLATURE	:	VIBRATION METER
MANUFACTURER	:	INSTANTEL
MODEL / TYPE	:	721A2501/721A2901
SERIAL NO.	:	UM12890/UM12890 [UAE.EFM.026/2561]
DATE OF CALIBRATION	:	19 July 2025

ENVIRONMENT CONDITIONS :

Temperature : (23 ± 2) °C Relative Humidity : (55 ± 15) %RH

PROCEDURE USED :

This instrument was calibrated under procedure No. **CLC-CPEE-08** based on **ISO 16063-21** as calibration guideline.
The calibration was performed by using Digital Multimeter, Programmable Timer/Counter and Accelerometer with Measuring Amplifier which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. Digital Multimeter, Wavetek Model 1281 S/N. 29320.
2. Programmable Timer/Counter, Philips Model PM6680B S/N. SM607101.
3. Accelerometer with Measuring Amplifier, Bruel & Kjaer Model 8305, 2625 S/N. 397018, 2434988.

TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through Aeronautical Radio of Thailand Ltd. Certificate No. 05-0316/23 , Due Date 21 July 2025.
2. The measurements are traceable to International System of Units (SI), through Aeronautical Radio of Thailand Ltd. Certificate No. 07-0054/25 , Due Date 11 June 2026.
3. The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand) Certificate No. AV-0056-24, Due Date 14 December 2025.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k = 2,00 which for a normal distribution corresponds to a coverage probability of approximately 95 %.
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q25084760
F3-011-05/12-23

เอกสารไม่ควบคุม

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com

CALIBRATION DATA

3. DISPLACEMENT RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
(mm)	(frequency)		(mm)	(mm)	(mm)	±(% of rdg.)
0.03	50 Hz	peak	0.030	0.030	0.000	2.1
0.04	50 Hz		0.040	0.040	0.000	1.7
0.05	50 Hz		0.050	0.050	0.000	1.4
0.06	50 Hz		0.060	0.061	-0.001	1.3
0.07	50 Hz		0.070	0.071	-0.001	1.1
0.03	100 Hz	peak	0.030	0.030	0.000	2.1
0.04	100 Hz		0.040	0.040	0.000	1.7
0.05	100 Hz		0.050	0.050	0.000	1.4
0.06	100 Hz		0.060	0.061	-0.001	1.3
0.07	100 Hz		0.070	0.071	-0.001	1.1

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 015 Page 1,2 of 68

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q25084760
F3-011-05/12-23

เอกสารไม่ควบคุม

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Road, Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE	:	VIBRATION METER
MANUFACTURER	:	INSTANTEL
MODEL / TYPE	:	721A2501/721A3301
SERIAL NO.	:	UM11230/UM11230[UAE.EFM.029/2559]
CLID. NO.	:	251701315
JOB CONTROL NO.	:	251222149760
CALIBRATION SERVICE	:	☑ IN-LABORATORY ☐ ON-SITE

CUSTOMER : UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,
BANGCHAK, PHRAKHANONG, BANGKOK 10260

DATE OF RECEIVED : 22 December 2025 DATE OF ISSUED : 25 December 2025

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Suwit Phuanbusabong
Calibration Engineer

Approved By : Mongkol Yotsoontorn
Authorized Signatory
25 December 2025

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q25149760
F3-011-05/12-23

เอกสารไม่ควบคุม

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Road, Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com

CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment ( ) adjustment

CALIBRATION DATA

1. ACCELERATION RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
(g)	(frequency)		(g)	(g)	(g)	± (% of rdg.)
0.3	50 Hz		0.300	0.304	-0.004	1.9
0.4	50 Hz		0.400	0.406	-0.006	1.6
0.5	50 Hz	peak	0.500	0.507	-0.007	1.6
0.6	50 Hz		0.600	0.608	-0.008	2.5
0.7	50 Hz		0.700	0.710	-0.010	2.5
0.3	100 Hz		0.300	0.302	-0.002	1.9
0.4	100 Hz		0.400	0.404	-0.004	1.6
0.5	100 Hz	peak	0.500	0.506	-0.006	1.6
0.6	100 Hz		0.600	0.608	-0.008	2.5
0.7	100 Hz		0.700	0.709	-0.009	2.5

2. VELOCITY RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
(mm/s)	(frequency)		(mm/s)	(mm/s)	(mm/s)	± (% of rdg.)
3	50 Hz		3.000	3.029	-0.029	1.8
4	50 Hz		4.000	4.038	-0.038	1.8
5	50 Hz	peak	5.000	5.067	-0.067	1.8
6	50 Hz		6.000	6.076	-0.076	1.8
7	50 Hz		7.000	7.089	-0.089	1.8
3	100 Hz		3.000	3.029	-0.029	1.6
4	100 Hz		4.000	4.039	-0.039	1.6
5	100 Hz	peak	5.000	5.045	-0.045	1.6
6	100 Hz		6.000	6.059	-0.059	1.5
7	100 Hz		7.000	7.068	-0.068	1.5

Certificate No. Q25149760
F3-011-05/12-23

เอกสารไม่ควบคุม

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Road, Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com

REPORT OF CALIBRATION

FOR

NOMENCLATURE	:	VIBRATION METER
MANUFACTURER	:	INSTANTEL
MODEL / TYPE	:	721A2501/721A3301
SERIAL NO.	:	UM11230/UM11230[UAE.EFM.029/2559]
DATE OF CALIBRATION	:	23 December 2025

ENVIRONMENT CONDITIONS :
Temperature : (23 ± 2) °C Relative Humidity : (55 ± 15) %RH

PROCEDURE USED :
This instrument was calibrated under procedure No. **CLC-CPEE-08** based on **ISO 16063-21** as calibration guideline.
The calibration was performed by using Digital Multimeter, Programmable Timer/Counter and Vibration Calibrator with Measuring Amplifier which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :
1. Digital Multimeter, Keysight Technologies Model 3458A S/N. MY59352733.
2. Programmable Timer/Counter, Philips Model PM6680B S/N. SM607101.
3. Vibration Calibrator, The Modal Shop Model 9110D S/N. 11424.

TRACEABILITY :
1. The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand) Certificate No. EE-0090-25, Due Date 31 July 2026.
2. The measurements are traceable to International System of Units (SI), through Aeronautical Radio of Thailand Ltd. Certificate No. 07-0054/25 , Due Date 11 June 2026.
3. The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand) Certificate No. AV-0030-24, Due Date 22 July 2026.

UNCERTAINTY :
The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2$ which for a normal distribution corresponds to a coverage probability of approximately 95 %
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q25149760
F3-011-05/12-23

เอกสารไม่ควบคุม

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Road, Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax. 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com

CALIBRATION DATA

3. DISPLACEMENT RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
(mm)	(frequency)		(mm)	(mm)	(mm)	± (% of rdg.)
0.03	50 Hz		0.030	0.030	0.000	2.5
0.04	50 Hz		0.040	0.040	0.000	2.1
0.05	50 Hz	peak	0.050	0.050	0.000	1.9
0.06	50 Hz		0.060	0.061	-0.001	1.8
0.07	50 Hz		0.070	0.071	-0.001	1.8
0.03	100 Hz		0.030	0.030	0.000	2.5
0.04	100 Hz		0.040	0.040	0.000	2.1
0.05	100 Hz	peak	0.050	0.050	0.000	1.9
0.06	100 Hz		0.060	0.061	-0.001	1.8
0.07	100 Hz		0.070	0.071	-0.001	1.8

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 017 Page 1,2 of 73

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q25149760
F3-011-05/12-23

เอกสารไม่ควบคุม

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE	:	VIBRATION METER
MANUFACTURER	:	INSTANTEL
MODEL / TYPE	:	721A2601/721A3301
SERIAL NO.	:	UM11355/UM11355 [UAE.EFM.002/2560]
CLID. NO.	:	252000637
JOB CONTROL NO.	:	250730088636
CALIBRATION SERVICE	:	☑ IN-LABORATORY ☐ ON-SITE

CUSTOMER : UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,
BANGCHAK, PHRAKHANONG, BANGKOK 10260

DATE OF RECEIVED : 30 July 2025 DATE OF ISSUED : 05 August 2025

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Suwit Phuanbusabong
Calibration Engineer

Approved By : Mongkol Yotsoontorn
Authorized Signatory
05 August 2025

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

เอกสารไม่ควบคุม
@clccalibration

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com

CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment ( ) adjustment

CALIBRATION DATA

1. ACCELERATION RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
(g)	(frequency)		(g)	(g)	(g)	± (% of rdg.)
0.3	50 Hz	peak	0.300	0.297	+0.003	1.9
0.4	50 Hz		0.400	0.396	+0.004	1.6
0.5	50 Hz		0.500	0.494	+0.006	1.6
0.6	50 Hz		0.600	0.593	+0.007	2.5
0.7	50 Hz		0.700	0.693	+0.007	2.5
0.3	100 Hz	peak	0.300	0.300	0.000	1.9
0.4	100 Hz		0.400	0.399	+0.001	1.6
0.5	100 Hz		0.500	0.498	+0.002	1.6
0.6	100 Hz		0.600	0.597	+0.003	2.5
0.7	100 Hz		0.700	0.696	+0.004	2.5

2. VELOCITY RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
(mm/s)	(frequency)		(mm/s)	(mm/s)	(mm/s)	± (% of rdg.)
3	50 Hz	peak	3.000	3.008	-0.008	1.8
4	50 Hz		4.000	4.018	-0.018	1.8
5	50 Hz		5.000	5.026	-0.026	1.8
6	50 Hz		6.000	6.032	-0.032	1.8
7	50 Hz		7.000	7.039	-0.039	1.8
3	100 Hz	peak	3.000	3.008	-0.008	1.6
4	100 Hz		4.000	4.014	-0.014	1.6
5	100 Hz		5.000	5.021	-0.021	1.6
6	100 Hz		6.000	6.028	-0.028	1.5
7	100 Hz		7.000	7.034	-0.034	1.5

เอกสารไม่ควบคุม
@clccalibration

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com

REPORT OF CALIBRATION

FOR

NOMENCLATURE	:	VIBRATION METER
MANUFACTURER	:	INSTANTEL
MODEL / TYPE	:	721A2601/721A3301
SERIAL NO.	:	UM11355/UM11355 [UAE.EFM.002/2560]
DATE OF CALIBRATION	:	01 August 2025

ENVIRONMENT CONDITIONS :

Temperature : (23 ± 2) °C Relative Humidity : (55 ± 15) %RH

PROCEDURE USED :

This instrument was calibrated under procedure No. **CLC-CPEE-08** based on **ISO 16063-21** as calibration guideline.
The calibration was performed by using Advanced Multimeter, Programmable Timer/Counter and Accelerometer with Measuring Amplifier which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. Advanced Multimeter, Transmile Model 8104 S/N. N2164D24.
2. Programmable Timer/Counter, Philips Model PM6680B S/N. SM607101.
3. Accelerometer with Measuring Amplifier, Bruel & Kjaer Model 8305, 2625 S/N. 397018, 2434988.

TRACEABILITY :

1. The measurements are traceable to International System of Units (SI) , through Transmille Ltd.
Certificate No. 54742, Due Date 02 July 2026.
2. The measurements are traceable to International System of Units (SI), through Aeronautical Radio of Thailand Ltd.
Certificate No. 07-0054/25 , Due Date 11 June 2026.
3. The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand)
Certificate No. AV-0056-24, Due Date 14 December 2025.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2,00$ which for a normal distribution corresponds to a coverage probability of approximately 95 %.
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

เอกสารไม่ควบคุม
@clccalibration

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com

CALIBRATION DATA

3. DISPLACEMENT RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
(mm)	(frequency)		(mm)	(mm)	(mm)	± (% of rdg.)
0.03	50 Hz	peak	0.030	0.030	0.000	2.5
0.04	50 Hz		0.040	0.040	0.000	2.1
0.05	50 Hz		0.050	0.050	0.000	1.9
0.06	50 Hz		0.060	0.060	0.000	1.8
0.07	50 Hz		0.070	0.069	+0.001	1.8
0.03	100 Hz	peak	0.030	0.030	0.000	2.5
0.04	100 Hz		0.040	0.040	0.000	2.1
0.05	100 Hz		0.050	0.050	0.000	1.9
0.06	100 Hz		0.060	0.060	0.000	1.8
0.07	100 Hz		0.070	0.069	+0.001	1.8

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 015 Page 1,2 of 68

This report is valid for the above stated instrument/s only.

End of Certificate

เอกสารไม่ควบคุม
@clccalibration

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE	:	VIBRATION METER
MANUFACTURER	:	INSTANTEL
MODEL / TYPE	:	721A2601/721A3301
SERIAL NO.	:	UM11057/UM11057 [UAE.EFM.024/2562]
CLID. NO.	:	252000248
JOB CONTROL NO.	:	250719084763
CALIBRATION SERVICE	:	☑ IN-LABORATORY ☐ ON-SITE

CUSTOMER : UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,
BANGCHAK, PHRAKHANONG, BANGKOK 10260

DATE OF RECEIVED : 19 July 2025 DATE OF ISSUED : 24 July 2025

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Suwit Phuanbusabong
Calibration Engineer

Approved By : Mongkol Yotsoontorn
Authorized Signatory
24 July 2025

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q25084763
F3-011-05/12-23

เอกสารไม่ควบคุม

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com

CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : (X) without adjustment ( ) adjustment

CALIBRATION DATA

1. ACCELERATION RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
(g)	(frequency)		(g)	(g)	(g)	± (% of rdg.)
0.3	50 Hz	peak	0.300	0.305	-0.005	1.9
0.4	50 Hz		0.400	0.407	-0.007	1.3
0.5	50 Hz		0.500	0.509	-0.009	1.3
0.6	50 Hz		0.600	0.610	-0.010	2.5
0.7	50 Hz		0.700	0.712	-0.012	2.5
0.3	100 Hz	peak	0.300	0.305	-0.005	1.9
0.4	100 Hz		0.400	0.406	-0.006	1.3
0.5	100 Hz		0.500	0.508	-0.008	1.3
0.6	100 Hz		0.600	0.610	-0.010	2.5
0.7	100 Hz		0.700	0.713	-0.013	2.5

2. VELOCITY RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
(mm/s)	(frequency)		(mm/s)	(mm/s)	(mm/s)	± (% of rdg.)
3	50 Hz	peak	3.000	3.031	-0.031	1.8
4	50 Hz		4.000	4.039	-0.039	1.8
5	50 Hz		5.000	5.046	-0.046	1.8
6	50 Hz		6.000	6.055	-0.055	1.8
7	50 Hz		7.000	7.063	-0.063	1.8
3	100 Hz	peak	3.000	3.031	-0.031	2.7
4	100 Hz		4.000	4.045	-0.045	1.3
5	100 Hz		5.000	5.053	-0.053	1.3
6	100 Hz		6.000	6.067	-0.067	1.0
7	100 Hz		7.000	7.071	-0.071	1.0

Certificate No. Q25084763
F3-011-05/12-23

เอกสารไม่ควบคุม

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com

REPORT OF CALIBRATION

FOR

NOMENCLATURE	:	VIBRATION METER
MANUFACTURER	:	INSTANTEL
MODEL / TYPE	:	721A2601/721A3301
SERIAL NO.	:	UM11057/UM11057 [UAE.EFM.024/2562]
DATE OF CALIBRATION	:	19 July 2025

ENVIRONMENT CONDITIONS :
Temperature : (23 ± 2) °C Relative Humidity : (55 ± 15) %RH

PROCEDURE USED :
This instrument was calibrated under procedure No. CLC-CPEE-08 based on ISO 16063-21 as calibration guideline.
The calibration was performed by using Digital Multimeter, Programmable Timer/Counter and Accelerometer with Measuring Amplifier which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :
1. Digital Multimeter, Wavetek Model 1281 S/N. 29320.
2. Programmable Timer/Counter, Philips Model PM6680B S/N. SM607101.
3. Accelerometer with Measuring Amplifier, Bruel & Kjaer Model 8305, 2625 S/N. 397018, 2434988.

TRACEABILITY :
1. The measurements are traceable to International System of Units (SI), through Aeronautical Radio of Thailand Ltd.
Certificate No. 05-0316/23 , Due Date 21 July 2025.
2. The measurements are traceable to International System of Units (SI), through Aeronautical Radio of Thailand Ltd.
Certificate No. 07-0054/25 , Due Date 11 June 2026.
3. The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand)
Certificate No. AV-0056-24, Due Date 14 December 2025.

UNCERTAINTY :
The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k = 2,00 which for a normal distribution corresponds to a coverage probability of approximately 95 %.
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q25084763
F3-011-05/12-23

เอกสารไม่ควบคุม

CALIBRATION LABORATORY CO., LTD.
2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com

CALIBRATION DATA

3. DISPLACEMENT RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
(mm)	(frequency)		(mm)	(mm)	(mm)	± (% of rdg.)
0.03	50 Hz	peak	0.030	0.030	0.000	2.1
0.04	50 Hz		0.040	0.040	0.000	1.7
0.05	50 Hz		0.050	0.050	0.000	1.4
0.06	50 Hz		0.060	0.060	0.000	1.3
0.07	50 Hz		0.070	0.071	-0.001	1.1
0.03	100 Hz	peak	0.030	0.030	0.000	2.1
0.04	100 Hz		0.040	0.040	0.000	1.7
0.05	100 Hz		0.050	0.050	0.000	1.4
0.06	100 Hz		0.060	0.060	0.000	1.3
0.07	100 Hz		0.070	0.071	-0.001	1.1

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 015 Page 1,2 of 68

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q25084763
F3-011-05/12-23

เอกสารไม่ควบคุม

ELECTRICAL AND ELECTRONICS INSTITUTE
FOUNDATION FOR INDUSTRIAL DEVELOPMENT
975 Moo 4, Bangpoo Industrial Estate, Soi 8, Sukhumvit Road km 37,
Phraek Sa, Mueang Samut Prakan, Samut Prakan 10280
Tel: +66 2709 4860 Fax: +66 2324 0917

NSC-TISI-TIS 17025
CALIBRATION 0119

Certificate No.: CP20250041EA
Operation No.: CP2024090313

Certificate of Calibration

Equipment:	Sound Level Meter
Manufacturer:	Larson Davis (Meter), PCB (Microphone), PCB (Preamplifier)
Model/Type:	LxT2 (Meter), 375A04 (Microphone), PRMLxT2C (Preamplifier)
Serial No.:	0005395 (Meter), 351846 (Microphone), 073797 (Preamplifier)
ID No.:	UAE.EFM.032/2564
Customer:	United Analyst and Engineering Consultant Co.,Ltd.
Address:	81 Soi Udomsuk 41, Sukhumvit Road, Bangchak Phrakhanong, Bangkok 10260
Received Date:	24 January 2025
Calibrated Date:	3 - 4 February 2025
Issued Date:	5 February 2025
Calibrated by:	Ms. Juntapom Kunhakorn

Approved by: _____
(Mr. Sittichai Swaksuriyawong)
Group Manager

This report was prepared electronically using applicable electronic signature. Printing or copy of file are considered as a copy of the document.
The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor (k) providing a level of confidence of approximately 95%. This certificate may not be reproduced other than in full except with the prior written approval of the Electrical and Electronics Institute, Foundation for Industrial Development.

เอกสารไม่ควบคุม

Certificate No.: CP20250041EA

Calibration Report

Equipment: Sound Level Meter
Manufacturer: Larson Davis (Meter), PCB (Microphone), PCB (Preamplifier)
Model/Type: LxT2 (Meter), 375A04 (Microphone), PRMLxT2C (Preamplifier)
Serial No.: 0005395 (Meter), 351846 (Microphone), 073797 (Preamplifier)
ID No.: UAE.EFM.032/2564
Ambient Temperature: (23 ± 2) °C
Relative Humidity: (50 ± 15) %
Pressure: (101.3 ± 1.5) kPa
Method of Calibration :-
IEC 61672-3:2013.

Condition of this result of calibration
1. Reference standards instrument :-

	Instrument	Model	Serial No.	Cert. No.	Due Date
1)	Standard microphone	4180	2661000	AA-1007-24	6 June 2025
2)	Arbitrary Function Generator	AFG2021	C010063	CK20240048EA	23 June 2025
3)	Programmable Attenuator	PA5	2913	EF-0021-24	3 June 2025
4)	6.5 Digit precision multimeter	8846A	9609027	CB20240128EA	31 July 2025
5)	Pressure humidity and Temperature Transmitter	PTU301	F0640002	CL1-P240022 CD20240180EA	20 March 2025 7 August 2025
6)	Performance Audio Analyzer	UB903B	MY56510003	CB20240035EB CK20240069EA	13 February 2025 19 September 2025

2. This result of calibration was found accurate as shown on date and place of calibration only.
3. This certification is traceable to the international system of unit maintained at :-
Reference standards instrument for Acoustic function
- National Institute of Metrology (Thailand)
- Electrical and Electronics Institute; NSC Accredited Calibration No.0119
Reference standards instrument for Electrical function
- National Institute of Metrology (Thailand)
- Electrical and Electronics Institute; NSC Accredited Calibration No.0119

Result of Calibration:-
Function : 1. Indication at the calibration check frequency

Reference Acoustic Signal (dB)	Measured value (dB)	Deviation (dB)	Acceptance limits (dB)
-	-	-	-

เอกสารไม่ควบคุม

Certificate No.: CP20250041EA

Calibration Report

Function : 2. Self-generated Noise
2.1 Microphone Installed

Measured value (dB)
31.1

2.2 Microphone replaced by the electrical input signal device

Frequency Weighting	Measured value (dB)
A-weighting	28.1
C-weighting	27.9
Z-weighting	34.1

Function : 3. Acoustical signal tests of frequency weightings (Without Windscreen)
Meter free-field acoustic response at a level of 84 dB.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
125	0.1	0.0	0.1	±1.5
1000	-0.1	-0.1	-0.1	±1.0
8000	-0.7	-0.8	-0.4	±5.0

Function : 4. Electrical signal tests of frequency weightings
Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
63	-0.1	0.0	0.0	±2.0
125	-0.1	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	-0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	-0.1	0.0	0.1	±5.0

Function : 5. Frequency and time weighting at 1 kHz
5.1 Frequency weighting at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
C-weighting	94.0	0.0	±0.2
A-weighting	94.0	0.0	±0.2
Z-weighting	94.0	0.0	±0.2

เอกสารไม่ควบคุม

Certificate No.: CP20250041EA

Calibration Report

5.2 Time weighting at 1 kHz

Time Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	94.0	0.0	±0.1
Slow	94.0	0.0	±0.1
LAeq	94.0	0.0	±0.1

Function : 6. Long-Term Stability
Long-term stability over 30 minutes, with steady 1 kHz signal at reference level.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
30	94.0	94.0	0.0	±0.3

Function : 7. Level Linearity on the reference level range
7.1 Level Linearity on the reference level range, Upper

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±1.1
99.0	99.0	0.0	±1.1
104.0	104.1	0.1	±1.1
109.0	109.1	0.1	±1.1
114.0	114.1	0.1	±1.1
119.0	119.1	0.1	±1.1
124.0	124.1	0.1	±1.1
129.0	129.1	0.1	±1.1
134.0	134.1	0.1	±1.1
139.0	139.1	0.1	±1.1

เอกสารไม่ควบคุม

Certificate No.: CP20250041EA

Calibration Report

7.2 Level Linearity on the reference level range, Lower

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±1.1
89.0	89.0	0.0	±1.1
84.0	84.0	0.0	±1.1
79.0	79.0	0.0	±1.1
74.0	74.0	0.0	±1.1
69.0	69.0	0.0	±1.1
64.0	64.0	0.0	±1.1
59.0	59.0	0.0	±1.1
54.0	54.0	0.0	±1.1
49.0	49.0	0.0	±1.1
44.0	44.1	0.1	±1.1
39.0	39.4	0.4	±1.1

Function : 8. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	200	136.0	0.0	±1.0
	2	118.9	-0.1	+1.0 ; -2.5
	0.25	109.5	-0.5	+1.5 ; -5.0
Slow	200	129.5	-0.1	±1.0
	2	109.9	-0.1	+1.0 ; -5.0
LAE	200	130.0	0.0	±1.0
	2	110.0	0.0	+1.0 ; -2.5
	0.25	100.9	-0.1	+1.5 ; -5.0

Function : 9. Peak C sound level

Number of cycles in test signal	Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Complete cycle	135.4	134.7	-0.7	±3.0
Positive half cycle	134.4	134.0	-0.4	±2.0
Negative half cycle	134.4	134.0	-0.4	±2.0

Function : 10. Overload indication

Measured value (dB)		Deviated value	Acceptance limits
Positive one-half cycle	Negative one-half cycle	(dB)	(dB)
142.1	142.1	0.0	±1.5

เอกสารไม่ควบคุม

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7-139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL : 0669-2116-5869-1 FAX: 0669-2116-7140

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

Certificate No : 25-SLM-241
Request No : Req-2025-1240

Unit Under Calibration Details

Measurement item : Sound Level Meter
Manufacturer : LARSON DAVIS
Model : LxT2
Serial Number : 0005287
ID : UAE.EFM.103/2562
Resolution : 0.1 dB

Microphone Class : 2
Microphone Model : 377A04
Microphone S/N : 350427
Preamplifier Model : PRMLXT2B
Preamplifier S/N : 056074
Instrument Status : Used

Calibration Environment and Details

Temperature : 23 °C ± 2 °C
Humidity : 50 %RH ± 20 %RH
Barometric Pressure : 1013 hPa ± 10 hPa
Received Date : 16 July 2025
Calibrated Date : 29 July 2025
Calibration Procedure : In-house method CP-SLM-01 based on IEC 61672-3 : 2013 Electroacoustics - Sound level meters - Part 3: Periodic tests
Location of Calibration : Lab Acoustic

Reference Standard

Instrument	Brand	Model	SN.	Due calibration	Traceability
Multifunction Acoustic Calibrator	Bruel&Kjaer	4226	3412381	8 May 2026	NIMT
Audio Generator	Svantek	Svan401	131	15 October 2025	WK Electric

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k = 2$, providing a level of confidence approximately 95 %.

Calibrated By : Mr. Noppadon Luangart, Service Calibration Engineer
Approved By : Mr. Pacit Mathuvorn, Calibration Engineer Supervisor
Issue Date : 29 July 2025

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

ELECTRICAL AND ELECTRONICS INSTITUTE
FOUNDATION FOR INDUSTRIAL DEVELOPMENT

Certificate No.: CP20250041EA

Calibration Report

Function : 11. High-Level Stability

High-level stability over 5 minutes, with steady 1 kHz signal, 1 dB below upper boundary.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
5	139.0	139.0	0.0	±0.3

Uncertainty of measurement

Function	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1) Indication at the calibration check frequency	0.30	Not applicable
2) Self-generated Noise	0.10	Not applicable
3) Acoustical signal tests of frequency weightings - Free-field sound pressure response level	0.30	0.60 (10Hz to 4kHz) 0.70 (>4kHz to 10kHz)
4) Electrical signal tests of frequency weightings	0.20	0.20
5) Frequency and time weighting at 1 kHz	0.20	0.20
6) Long-Term Stability	0.10	0.10
7) Level Linearity on the reference level range	0.30	0.30
8) Tone burst response	0.20	0.30
9) Peak C sound level	0.20	0.35
10) Overload indication	0.24	0.25
11) High-Level Stability	0.10	0.10

Remarks: 1. The acceptance limit is for the deviated value.
2. Acceptance limits was IEC61672-3:2013 Class 2.
3. The coverage factor $k = 2.00$

- - End of Report - -

เอกสารไม่ควบคุม

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7-139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL : 0669-2116-5869-1 FAX: 0669-2116-7140

Certificate No : 25-SLM-241
Request No : Req-2025-1240

1. Indication at the calibration check frequency

UUC Setting	Nominal	Before Adjust		After Adjust		UNCERTAINTY
FAST / A / 37-139	Level	UUC	ERR	UUC	ERR	
Calibrator Setting	(dB)	(dB)	(dB)	(dB)	(dB)	(± dB)
1000 Hz 114 dB	114.68	115.2	0.52	114.7	0.02	0.20

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand 3M, Model AC-300, SN. AC-300001087

2. Self-generated noise, Microphone installed

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139		
UUC Weighting	(dB)	(± dB)
A	27.4	0.10

3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139		
UUC Weighting	(dB)	(± dB)
A	27.2	0.10
C	27.9	0.10
Z	34.6	0.10

4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting	Deviation from various Frequency Weighting Respone curve			UNCERTAINTY
FAST / 37-139	A	C	Z	
STD Setting	(dB)	(dB)	(dB)	(± dB)
125 Hz	0.4	0.3	0.3	0.60
1000 Hz	0.0	0.0	0.0	0.60
4000 Hz	0.1	0.1	0.1	0.60
8000 Hz	-0.3	-0.3	-0.2	0.70

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL.: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate No : 25-SLM-241
Request No : Req-2025-1240

5. Electrical signal test of frequency weightings, Weighting network respone with relative to 1 kHz

UUC Setting	Deviation from various Frequency			UNCERTAINTY
FAST / 37-139	Weighting Respone curve			
STD Setting	A (dB)	C (dB)	Z (dB)	(± dB)
63 Hz	0.2	0.2	0.2	0.20
125 Hz	0.1	0.2	0.2	
250 Hz	0.0	0.1	0.1	
500 Hz	0.0	0.1	0.0	
1000 Hz	0.0	0.0	0.0	
2000 Hz	0.0	0.0	0.0	
4000 Hz	-0.1	-0.1	-0.1	
8000 Hz	-0.2	-0.2	-0.1	
16000 Hz	-0.2	-0.2	-0.3	

6. Frequency and time weightings at 1kHz

UUC Setting	STD	Measured		UNCERTAINTY
FAST / 37-139	REF	UUC	ERR	
UUC Weighting	(dB)	(dB)	(dB)	(± dB)
A	114.00	114.0	0.0	0.20
C	114.00	114.0	0.0	
Z	114.00	114.0	0.0	

UUC Setting	STD	Measured		UNCERTAINTY
37-139 / A	REF	UUC	ERR	
UUC Time Respone	(dB)	(dB)	(dB)	(± dB)
Fast	114.00	114.0	0.0	0.20
Slow	114.00	114.0	0.0	
Leq	114.00	114.0	0.0	

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL.: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate No : 25-SLM-241
Request No : Req-2025-1240

9. Level linearity including the level range control

UUC Setting	STD	Measured		UNCERTAINTY
FAST / A	REF	UUC	ERR	
UUC Range	(dB)	(dB)	(dB)	(± dB)
37-139	42.00	42.1	0.1	0.30
	114	114.0	0.0	

10. Tone burst response

UUC Setting	STD	Anticipated	Measured		UNCERTAINTY
A / 37-139	Toneburst	Ref	UUC	ERR	
UUC Time Respone	(ms)	(dB)	(dB)	(dB)	(± dB)
Fast	200	135.0	134.9	-0.1	0.20
	2	118.0	117.9	-0.1	
	0.25	109.0	108.7	-0.3	
Slow	200	128.6	128.4	-0.2	
	2	109.0	108.8	-0.2	
SEL	200	129.0	129.0	0.0	
	2	109.0	109.1	+0.1	
	0.25	100.0	99.9	-0.1	

11. Peak C Sound level

UUC Setting	Anticipated	Measured		UNCERTAINTY
FAST / C / 95-142	REF	UUC	ERR	
STD Setting	(dB)	(dB)	(dB)	(± dB)
Complete cycle	137.4	136.8	-0.60	0.20
Positive half cycle	136.4	136.2	-0.20	
Negative half cycle	136.4	136.2	-0.20	

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL.: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate No : 25-SLM-243
Request No : Req-2025-1240

7. Long Term Stability

UUC Setting	Measured	UNCERTAINTY
FAST / A / 37-139	UUC	
STD Setting	(dB)	(± dB)
Initial	114.0	[redacted]
Final	114.0	
Deviated	0.0	0.10

8. Level linearity on the reference level range

UUC Setting	Anticipated	Deviation		UNCERTAINTY
FAST / A / 37-139	REF	UUC	ERR	
STD dB	(dB)	(dB)	(dB)	(± dB)
139.00	139	139.0	0.0	0.30
134.00	134	134.0	0.0	
129.00	129	129.0	0.0	
124.00	124	124.0	0.0	
119.00	119	119.0	0.0	
114.00	114	114.0	0.0	
109.00	109	109.0	0.0	
104.00	104	104.0	0.0	
99.00	99	99.0	0.0	
94.00	94	93.9	-0.1	
89.00	89	88.9	-0.1	
84.00	84	83.9	-0.1	
79.00	79	78.9	-0.1	
74.00	74	73.9	-0.1	
69.00	69	68.9	-0.1	
64.00	64	63.9	-0.1	
59.00	59	58.9	-0.1	
54.00	54	54.0	0.0	
49.00	49	49.0	0.0	
44.00	44	44.0	0.0	
39.00	39	39.2	0.2	
38.00	38	38.3	0.3	
37.00	37	37.4	0.4	
36.00	36	36.5	0.5	

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL.: (66)0-2116-5860-1 FAX: (66)0-2116-7140

Certificate No : 25-SLM-241
Request No : Req-2025-1240

12. Overload indication

UUC Setting	Measured	UNCERTAINTY
FAST / A / 37-139	UUC	
STD Setting	(dB)	(± dB)
Positive one-half cycle	140.8	[redacted]
Negative one-half cycle	140.6	
Deviated	0.2	0.20

13. High Level Stability

UUC Setting	Measured	UNCERTAINTY
FAST / A / 37-139	UUC	
STD Setting	(dB)	(± dB)
Initial	138.0	[redacted]
Final	138.0	
Deviated	0.0	0.10

End of Certificate

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (6610-2116-5860-1 FAX: (6610-2116-7140

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD. **Certificate No :** 25-SLM-242

Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260 **Request No :** Req-2025-1241

Unit Under Calibration Details

Measurement item	: Sound Level Meter	Microphone Class	: 2
Manufacturer	: LARSON DAVIS	Microphone Model	: 375B02
Model	: LxT2	Microphone S/N	: 011731
Serial Number	: 0005288	Preamplifier Model	: PRMLxT2B
ID	: UAE.EFM.104/2562	Preamplifier S/N	: 056075
Resolution	: 0.1 dB	Instrument Status	: Used

Calibration Environment and Details

Temperature : 23 °C ± 2 °C

Humidity : 50 %RH ± 20 %RH

Barometric Pressure : 1013 hPa ± 10 hPa

Received Date : 16 July 2025

Calibrated Date : 29 July 2025

Calibration Procedure : In-house method CP-SLM-01 based on IEC 61672-3 : 2013 Electroacoustics - Sound level meters - Part 3: Periodic tests

Location of Calibration : Lab Acoustic

Reference Standard

Instrument	Brand	Model	SN	Due calibration	Traceability
Multifunction Acoustic Calibrator	Bruel&Kjaer	4226	3412381	8 May 2026	NIMT
Audio Generator	Svantek	Svan401	131	15 October 2025	WK Electric

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k = 2$, providing a level of confidence approximately 95 %.

Calibrated By : Mr. Noppadon Luangart, Service Calibration Engineer

Approved By : Mr. Pacit Mathavorn, Calibration Engineer Supervisor

Issue Date : 29 July 2025

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (6610-2116-5860-1 FAX: (6610-2116-7140

Certificate No : 25-SLM-242

Request No : Req-2025-1241

5. Electrical signal test of frequency weightings, Weighting network respone with relative to 1 kHz

UUC Setting	Deviation from various Frequency Weighting Respone curve			UNCERTAINTY
FAST / 37-139				
STD Setting	A (dB)	C (dB)	Z (dB)	(± dB)
63 Hz	-0.1	0.0	0.0	0.20
125 Hz	-0.1	0.1	0.0	
250 Hz	-0.1	0.0	0.0	
500 Hz	0.0	0.1	0.0	
1000 Hz	0.0	0.0	0.0	
2000 Hz	0.1	0.1	0.0	
4000 Hz	0.0	0.1	0.1	
8000 Hz	0.0	0.0	0.1	
16000 Hz	0.0	0.0	-0.1	

6. Frequency and time weightings at 1kHz

UUC Setting	STD	Measured		UNCERTAINTY
FAST / 37-139	REF	UUC	ERR	
UUC Weighting	(dB)	(dB)	(dB)	(± dB)
A	114.00	114.0	0.0	0.20
C	114.00	114.0	0.0	
Z	114.00	114.0	0.0	

UUC Setting	STD	Measured		UNCERTAINTY
37-139 / A	REF	UUC	ERR	
UUC Time Respone	(dB)	(dB)	(dB)	(± dB)
Fast	114.00	114.0	0.0	0.20
Slow	114.00	114.0	0.0	
Leq	114.00	114.0	0.0	

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

FM-708-SLM-01 Rev.04 Issue date 17/2/25

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (6610-2116-5860-1 FAX: (6610-2116-7140

Certificate No : 25-SLM-242

Request No : Req-2025-1241

1. Indication at the calibration check frequency

UUC Setting	Nominal	Before Adjust		After Adjust		UNCERTAINTY
FAST / A / 37-139	Level	UUC	ERR	UUC	ERR	
Calibrator Setting	(dB)	(dB)	(dB)	(dB)	(dB)	(± dB)
1000 Hz 114 dB	114.68	115.2	0.52	114.7	0.02	0.20

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand 3M, Model AC-300, SN. AC-300001087

2. Self-generated noise, Microphone installed

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139		
UUC Weighting	(dB)	(± dB)
A	30.8	0.10

3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139		
UUC Weighting	(dB)	(± dB)
A	30.6	0.10
C	30.2	0.10
Z	34.3	0.10

4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting	Deviation from various Frequency Weighting Respone curve			UNCERTAINTY
FAST / 37-139	A	C	Z	
STD Setting	(dB)	(dB)	(dB)	(± dB)
125 Hz	0.1	0.1	0.1	0.60
1000 Hz	0.0	0.0	0.0	0.60
4000 Hz	1.6	1.6	1.6	0.60
8000 Hz	2.2	2.2	2.3	0.70

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

FM-708-SLM-01 Rev.04 Issue date 17/2/25

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (6610-2116-5860-1 FAX: (6610-2116-7140

Certificate No : 25-SLM-242

Request No : Req-2025-1241

7. Long Term Stability

UUC Setting	Measured	UNCERTAINTY
FAST / A / 37-139	UUC	
STD Setting	(dB)	(± dB)
Initial	114.0	
Final	114.0	
Deviated	0.0	0.10

8. Level linearity on the reference level range

UUC Setting	Anticipated	Deviation		UNCERTAINTY
FAST / A / 37-139	REF	UUC	ERR	
STD dB	(dB)	(dB)	(dB)	(± dB)
139.00	139	139.0	0.0	0.30
134.00	134	134.0	0.0	
129.00	129	129.0	0.0	
124.00	124	124.0	0.0	
119.00	119	119.0	0.0	
114.00	114	114.0	0.0	
109.00	109	109.0	0.0	
104.00	104	104.0	0.0	
99.00	99	99.0	0.0	
94.00	94	94.0	0.0	
89.00	89	89.0	0.0	
84.00	84	84.0	0.0	
79.00	79	79.0	0.0	
74.00	74	74.0	0.0	
69.00	69	69.0	0.0	
64.00	64	64.0	0.0	
59.00	59	59.0	0.0	
54.00	54	54.1	0.1	
49.00	49	49.1	0.1	
44.00	44	44.2	0.2	
40.00	40	40.5	0.5	

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

FM-708-SLM-01 Rev.04 Issue date 17/2/25

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL.: 06610-2116-5860-1 FAX: 06610-2116-7140

Certificate No : 25-SLM-242
Request No : Req-2025-1241

9. Level linearity including the level range control

UUC Setting	STD	Measured		UNCERTAINTY
FAST / A	REF	UUC	ERR	
UUC Range	(dB)	(dB)	(dB)	(± dB)
37-139	45.20	45.4	0.2	0.30
	114	114.0	0.0	

10. Tone burst response

UUC Setting	STD	Anticipated	Measured		UNCERTAINTY
A / 37-139	Toneburst	Ref	UUC	ERR	
UUC Time Respone	(ms)	(dB)	(dB)	(dB)	(± dB)
Fast	200	135.0	134.9	-0.1	0.20
	2	118.0	117.8	-0.2	
	0.25	109.0	108.7	-0.3	
Slow	200	128.6	128.4	-0.2	
	2	109.0	108.8	-0.2	
SEL	200	129.0	129.0	0.0	
	2	109.0	108.9	-0.1	
	0.25	100.0	99.8	-0.2	

11. Peak C Sound level

UUC Setting	Anticipated	Measured		UNCERTAINTY
FAST / C / 95-142	REF	UUC	ERR	
STD Setting	(dB)	(dB)	(dB)	(± dB)
Complete cycle	137.4	136.7	-0.70	0.20
Positive half cycle	136.4	136.1	-0.30	
Negative half cycle	136.4	136.1	-0.30	

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL.: 06610-2116-5860-1 FAX: 06610-2116-7140

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

Certificate No : 25-SLM-247
Request No : Req-2025-1640

Unit Under Calibration Details

Measurement item : Sound Level Meter
Manufacturer : LARSON DAVIS
Model : LxT2
Serial Number : 0005398
ID : UAE.EFM.035/2564
Resolution : 0.1 dB

Microphone Class : 2
Microphone Model : 375A04
Microphone S/N : 328675
Preamplifier Model : PRMLxT2C
Preamplifier S/N : 073793
Instrument Status : Used

Calibration Environment and Details

Temperature : 23 °C ± 2 °C
Humidity : 50 %RH ± 20 %RH
Barometric Pressure : 1013 hPa ± 10 hPa
Received Date : 16 July 2025
Calibrated Date : 30 July 2025
Calibration Procedure : In-house method CP-SLM-01 based on IEC 61672-1 : 2013 Electroacoustics - Sound level meters - Part 1: Periodic tests
Location of Calibration : Lab Acoustic

Reference Standard

Instrument	Brand	Model	SN.	Due calibration	Traceability
Multifunction Acoustic Calibrator	Bruel&Kjaer	4226	3412381	8 May 2026	NIMT
Audio Generator	Svantek	Svan401	131	15 October 2025	WK Electric

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k = 2, providing a level of confidence approximately 95 %.

Calibrated By : Mr. Noppadon Tungart
Service Calibration Engineer

Approved By : Mr. Pacit Maithavorn
Calibration Engineer Supervisor

Issue Date : 30 July 2025

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL.: 06610-2116-5860-1 FAX: 06610-2116-7140

Certificate No : 25-SLM-242
Request No : Req-2025-1241

12. Overload indication

UUC Setting	Measured	UNCERTAINTY
FAST / A / 37-139	UUC	
STD Setting	(dB)	(± dB)
Positive one-half cycle	142.5	
Negative one-half cycle	142.4	
Deviated	0.1	0.20

13. High Level Stability

UUC Setting	Measured	UNCERTAINTY
FAST / A / 37-139	UUC	
STD Setting	(dB)	(± dB)
Initial	138.0	
Final	138.0	
Deviated	0.0	0.10

End of Certificate

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL.: 06610-2116-5860-1 FAX: 06610-2116-7140

Certificate No : 25-SLM-247
Request No : Req-2025-1640

1. Indication at the calibration check frequency

UUC Setting	Nominal	Before Adjust		After Adjust		UNCERTAINTY
FAST / A / 37-139	Level	UUC	ERR	UUC	ERR	
Calibrator Setting	(dB)	(dB)	(dB)	(dB)	(dB)	(± dB)
1000 Hz 114 dB	114.68	115.2	0.52	114.7	0.02	0.20

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand 3M, Model AC-300, SN. AC-300001087

2. Self-generated noise, Microphone installed

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139		
UUC Weighting	(dB)	(± dB)
A	28.1	0.10

3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139		
UUC Weighting	(dB)	(± dB)
A	28.0	0.10
C	27.5	0.10
Z	31.7	0.10

4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting	Deviation from various Frequency Weighting Respone curve			UNCERTAINTY
FAST / 37-139	A	C	Z	
STD Setting	(dB)	(dB)	(dB)	(± dB)
125 Hz	0.1	0.2	0.1	0.60
1000 Hz	0.0	0.0	0.0	0.60
4000 Hz	0.6	0.8	0.7	0.60
8000 Hz	0.7	0.8	0.8	0.70

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 0660-2116-5860-1 FAX: 0660-2116-7140

Certificate No : 25-SLM-247
Request No : Req-2025-1640

5. Electrical signal test of frequency weightings, Weighting network respone with relative to 1 kHz

UUC Setting	Deviation from various Frequency Weighting Respone curve			UNCERTAINTY
FAST / 37-139				
STD Setting	A (dB)	C (dB)	Z (dB)	(± dB)
63 Hz	-0.2	-0.1	-0.1	0.20
125 Hz	-0.2	0.0	-0.1	
250 Hz	-0.1	-0.1	-0.1	
500 Hz	-0.1	0.0	-0.1	
1000 Hz	0.0	0.0	0.0	
2000 Hz	0.0	0.0	0.0	
4000 Hz	0.0	0.0	0.0	
8000 Hz	-0.1	-0.1	0.0	
16000 Hz	-0.1	-0.1	-0.1	

6. Frequency and time weightings at 1kHz

UUC Setting	STD	Measured		UNCERTAINTY
FAST / 37-139	REF	UUC	ERR	
UUC Weighting	(dB)	(dB)	(dB)	(± dB)
A	114.00	114.0	0.0	0.20
C	114.00	114.0	0.0	
Z	114.00	114.0	0.0	

UUC Setting	STD	Measured		UNCERTAINTY
37-139 / A	REF	UUC	ERR	
UUC Time Respone	(dB)	(dB)	(dB)	(± dB)
Fast	114.00	114.0	0.0	0.20
Slow	114.00	114.0	0.0	
Leq	114.00	114.0	0.0	

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 0660-2116-5860-1 FAX: 0660-2116-7140

Certificate No : 25-SLM-247
Request No : Req-2025-1640

9. Level linearity including the level range control

UUC Setting	STD	Measured		UNCERTAINTY
FAST / A	REF	UUC	ERR	
UUC Range	(dB)	(dB)	(dB)	(± dB)
37-139	43.10	43.2	0.1	0.30
	114	114.0	0.0	

10. Tone burst response

UUC Setting	STD	Anticipated	Measured		UNCERTAINTY
A / 37-139	Toneburst	Ref	UUC	ERR	
UUC Time Respone	(ms)	(dB)	(dB)	(dB)	(± dB)
Fast	200	135.0	135.0	0.0	0.20
	2	118.0	117.8	-0.2	
	0.25	109.0	108.6	-0.4	
Slow	200	128.6	128.5	-0.1	
	2	109.0	108.9	-0.1	
SEL	200	129.0	129.0	0.0	
	2	109.0	109.0	0.0	
	0.25	100.0	99.9	-0.1	

11. Peak C Sound level

UUC Setting	Anticipated	Measured		UNCERTAINTY
FAST / C / 95-142	REF	UUC	ERR	
STD Setting	(dB)	(dB)	(dB)	(± dB)
Complete cycle	137.0	136.7	-0.70	0.20
Positive half cycle	136.4	136.1	-0.30	
Negative half cycle	136.4	136.1	-0.30	

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd

FM-708-SLM-01 Rev.06 Issue date 17/2/25

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 0660-2116-5860-1 FAX: 0660-2116-7140

Certificate No : 25-SLM-247
Request No : Req-2025-1640

7. Long Term Stability

UUC Setting	Measured	UNCERTAINTY
FAST / A / 37-139	UUC	
STD Setting	(dB)	(± dB)
Initial	114.0	[redacted]
Final	114.0	
Deviated	0.0	0.10

8. Level linearity on the reference level range

UUC Setting	Anticipated	Deviation		UNCERTAINTY
FAST / A / 37-139	REF	UUC	ERR	
STD dB	(dB)	(dB)	(dB)	(± dB)
139.00	139	139.0	0.0	0.30
134.00	134	134.0	0.0	
129.00	129	129.0	0.0	
124.00	124	124.0	0.0	
119.00	119	119.0	0.0	
114.00	114	114.0	0.0	
109.00	109	109.0	0.0	
104.00	104	104.0	0.0	
99.00	99	99.0	0.0	
94.00	94	93.9	-0.1	
89.00	89	88.9	-0.1	
84.00	84	83.9	-0.1	
79.00	79	78.9	-0.1	
74.00	74	73.9	-0.1	
69.00	69	68.9	-0.1	
64.00	64	63.9	-0.1	
59.00	59	58.9	-0.1	
54.00	54	54.0	0.0	
49.00	49	49.0	0.0	
44.00	44	44.0	0.0	
39.00	39	39.1	0.3	
38.00	38	38.4	0.4	

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd

FM-708-SLM-01 Rev.06 Issue date 17/2/25

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 0660-2116-5860-1 FAX: 0660-2116-7140

Certificate No : 25-SLM-247
Request No : Req-2025-1640

12. Overload indication

UUC Setting	Measured	UNCERTAINTY
FAST / A / 37-139	UUC	
STD Setting	(dB)	(± dB)
Positive one-half cycle	141.9	[redacted]
Negative one-half cycle	141.9	
Deviated	0.0	0.20

13. High Level Stability

UUC Setting	Measured	UNCERTAINTY
FAST / A / 37-139	UUC	
STD Setting	(dB)	(± dB)
Initial	138.0	[redacted]
Final	138.0	
Deviated	0.0	0.10

End of Certificate

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd

FM-708-SLM-01 Rev.06 Issue date 17/2/25

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL.: (0)60-2116-5860-1 FAX: (0)60-2116-7140

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address : 81 Soi Udomsuk 41, Sukhonvit Road, Bangchak, Prakanong, Bangkok 10260

Certificate No : 25-SLM-272
Request No : Req-2025-1706

Unit Under Calibration Details

Measurement item	: Sound Level Meter	Microphone Class	: 2
Manufacturer	: LARSON DAVIS	Microphone Model	: 377B02
Model	: LxT2	Microphone S/N	: 011740
Serial Number	: 0005286	Preamplifier Model	: PRMLxT2B
ID	: UAE.IEFM.102/2562	Preamplifier S/N	: 056087
Resolution	: 0.1 dB	Instrument Status	: Used

Calibration Environment and Details

Temperature : 23 °C ± 2 °C
Humidity : 50 %RH ± 20 %RH
Barometric Pressure : 1013 hPa ± 10 hPa
Received Date : 22 July 2025
Calibrated Date : 11 August 2025
Calibration Procedure : In-house method CP-SLM-01 based on IEC 61672-3 : 2013 Electroacoustics - Sound level meters - Part 3: Periodic tests
Location of Calibration : Lab Acoustic

Reference Standard

Instrument	Brand	Model	SN	Due calibration	Traceability
Multifunction Acoustic Calibrator	Bruel&Kjaer	4226	3412381	8 May 2026	NIMT
Audio Generator	Svantek	Svan401	131	15 October 2025	WK Electric

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k = 2$, providing a level of confidence approximately 95 %.

Calibrated By : Mr. Noppadon Luangan
Service Calibration Engineer

Approved By : Mr. Pacit Mathavorn
Calibration Engineer Supervisor

Issue Date : 11 August 2025

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL.: (0)60-2116-5860-1 FAX: (0)60-2116-7140

Certificate No : 25-SLM-272
Request No : Req-2025-1706

5. Electrical signal test of frequency weightings, Weighting network respone with relative to 1 kHz

UUC Setting	Deviation from various Frequency Weighting Respone curve			UNCERTAINTY
FAST / 37-139				
STD Setting	A (dB)	C (dB)	Z (dB)	(± dB)
63 Hz	-0.2	0.0	0.0	0.20
125 Hz	-0.1	0.0	0.0	
250 Hz	-0.1	0.0	0.0	
500 Hz	-0.1	0.0	0.0	
1000 Hz	0.0	0.0	0.0	
2000 Hz	0.0	0.0	0.0	
4000 Hz	0.0	0.0	0.0	
8000 Hz	0.0	0.0	0.0	
16000 Hz	-0.1	-0.1	-0.1	

6. Frequency and time weightings at 1kHz

UUC Setting	STD	Measured		UNCERTAINTY
FAST / 37-139	REF	UUC	ERR	
UUC Weighting	(dB)	(dB)	(dB)	(± dB)
A	114.00	114.0	0.0	0.20
C	114.00	114.0	0.0	
Z	114.00	114.0	0.0	

UUC Setting	STD	Measured		UNCERTAINTY
37-139 / A	REF	UUC	ERR	
UUC Time Respone	(dB)	(dB)	(dB)	(± dB)
Fast	114.00	114.0	0.0	0.20
Slow	114.00	114.0	0.0	
Leq	114.00	114.0	0.0	

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL.: (0)60-2116-5860-1 FAX: (0)60-2116-7140

Certificate No : 25-SLM-272
Request No : Req-2025-1706

1. Indication at the calibration check frequency

UUC Setting	Nominal	Before Adjust		After Adjust		UNCERTAINTY
FAST / A / 37-139	Level	UUC	ERR	UUC	ERR	
Calibrator Setting	(dB)	(dB)	(dB)	(dB)	(dB)	(± dB)
1000 Hz 114 dB	114.13	114.9	0.77	114.1	-0.03	0.20

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 36, SN. 107224

2. Self-generated noise, Microphone installed

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139		
UUC Weighting	(dB)	(± dB)
A	31.5	0.10

3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139		
UUC Weighting	(dB)	(± dB)
A	31.2	0.10
C	30.7	0.10
Z	35.1	0.10

4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting	Deviation from various Frequency Weighting Respone curve			UNCERTAINTY
FAST / 37-139	A	C	Z	(± dB)
STD Setting	(dB)	(dB)	(dB)	
125 Hz	0.2	0.2	0.2	0.60
1000 Hz	0.0	0.0	0.0	0.60
4000 Hz	1.6	1.7	1.7	0.60
8000 Hz	2.3	2.3	2.3	0.70

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL.: (0)60-2116-5860-1 FAX: (0)60-2116-7140

Certificate No : 25-SLM-272
Request No : Req-2025-1706

7. Long Term Stability

UUC Setting	Measured	UNCERTAINTY
FAST / A / 37-139	UUC	
STD Setting	(dB)	(± dB)
Initial	114.0	
Final	114.0	
Deviated	0.0	0.10

8. Level linearity on the reference level range

UUC Setting	Anticipated	Deviation		UNCERTAINTY
FAST / A / 37-139	REF	UUC	ERR	
STD dB	(dB)	(dB)	(dB)	(± dB)
139.00	139	139.0	0.0	0.30
134.00	134	134.0	0.0	
129.00	129	129.0	0.0	
124.00	124	124.0	0.0	
119.00	119	119.0	0.0	
114.00	114	114.0	0.0	
109.00	109	109.0	0.0	
104.00	104	104.0	0.0	
99.00	99	99.0	0.0	
94.00	94	94.0	0.0	
89.00	89	89.0	0.0	
84.00	84	84.0	0.0	
79.00	79	79.0	0.0	
74.00	74	74.0	0.0	
69.00	69	69.0	0.0	
64.00	64	64.0	0.0	
59.00	59	59.0	0.0	
54.00	54	54.0	0.0	
49.00	49	49.1	0.1	
44.00	44	44.2	0.2	
43.00	43	43.3	0.3	
42.00	42	42.4	0.4	
41.00	41	41.5	0.5	

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7-139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 06610-2116-5860-1 FAX: 06610-2116-7140

Certificate No : 25-SLM-272

Request No : Req-2025-1706

9. Level linearity including the level range control

UUC Setting	STD	Measured		UNCERTAINTY
FAST / A	REF	UUC	ERR	
UUC Range	(dB)	(dB)	(dB)	(± dB)
37-139	46.60	46.7	0.1	0.30
	114	114.0	0.0	

10. Tone burst response

UUC Setting	STD	Anticipated	Measured		UNCERTAINTY
A / 37-139	Toneburst	Ref	UUC	ERR	
UUC Time Respone	(ms)	(dB)	(dB)	(dB)	(± dB)
Fast	200	135.0	134.9	-0.1	0.20
	2	118.0	117.8	-0.2	
	0.25	109.0	108.5	-0.5	
Slow	200	128.6	128.4	-0.2	
	2	109.0	108.8	-0.2	
SEL	200	129.0	129.0	0.0	
	2	109.0	108.9	-0.1	
	0.25	100.0	99.8	-0.2	

11. Peak C Sound level

UUC Setting	Anticipated	Measured		UNCERTAINTY
FAST / C / 95-142	REF	UUC	ERR	
STD Setting	(dB)	(dB)	(dB)	(± dB)
Complete cycle	137.4	136.8	-0.60	0.20
Positive half cycle	136.4	136.2	-0.20	
Negative half cycle	136.4	136.2	-0.20	

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd

FM-708-SLM-01 Rev.06 Issue date 17/2/25

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7-139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 06610-2116-5860-1 FAX: 06610-2116-7140

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.

Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

Certificate No : 25-SLM-337

Request No : Req-2025-2017

Unit Under Calibration Details

Measurement Item	: Sound Level Meter	Microphone Class	: 2
Manufacturer	: LARSON DAVIS	Microphone Model	: 375A04
Model	: LxT2	Microphone S/N	: 368645
Serial Number	: 0005349	Preamplifier Model	: PRMLxT2B
ID	: UAE.EFM.046/2563	Preamplifier S/N	: 056141
Resolution	: 0.1 dB	Instrument Status	: Used

Calibration Environment and Details

Temperature : 23 °C ± 2 °C

Humidity : 50 %RH ± 20 %RH

Barometric Pressure : 1013 hPa ± 10 hPa

Received Date : 5 September 2025

Calibrated Date : 9 October 2025

Calibration Procedure : In-house method CP-SLM-01 based on IEC 61672-3 : 2013 Electroacoustics - Sound level meters - Part 3: Periodic tests

Location of Calibration : Lab Acoustic

Reference Standard

Instrument	Brand	Model	SN	Due calibration	Traceability
Standard Microphone	Bruel&Kjaer	4226	3412381	7 May 2026	NIMT
Audio Generator	Svantek	Sven401	131	27 September 2026	WK Electric

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k = 2, providing a level of confidence approximately 95 %.

Calibrated By : Mr. Noppadon Luangart

Service Calibration Engineer

Approved By : Mr. Pacit Mathavorn

Calibration Engineer Supervisor

Issue Date : 9 October 2025

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd

FM-708-SLM-01 Rev.06 Issue date 17/2/25

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7-139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 06610-2116-5860-1 FAX: 06610-2116-7140

Certificate No : 25-SLM-272

Request No : Req-2025-1706

12. Overload indication

UUC Setting	Measured	UNCERTAINTY
FAST / A / 37-139	UUC	
STD Setting	(dB)	(± dB)
Positive one-half cycle	145.5	
Negative one-half cycle	145.6	
Deviated	-0.1	0.20

13. High Level Stability

UUC Setting	Measured	UNCERTAINTY
FAST / A / 37-139	UUC	
STD Setting	(dB)	(± dB)
Initial	138.0	
Final	138.0	
Deviated	0.0	0.10

End of Certificate

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd

FM-708-SLM-01 Rev.06 Issue date 17/2/25

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7-139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 06610-2116-5860-1 FAX: 06610-2116-7140

Certificate No : 25-SLM-337

Request No : Req-2025-2017

1. Indication at the calibration check frequency

UUC Setting	Nominal	Before Adjust		After Adjust		UNCERTAINTY
FAST / A / 37-139	Level	UUC	ERR	UUC	ERR	
Calibrator Setting	(dB)	(dB)	(dB)	(dB)	(dB)	(± dB)
1000 Hz 114 dB	113.75	113.7	-0.05	113.7	-0.05	0.20

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, SN: 58079

2. Self-generated noise, Microphone installed

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139		
UUC Weighting	(dB)	(± dB)
A	24.3	0.10

3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139		
UUC Weighting	(dB)	(± dB)
A	23.7	0.10
C	22.9	0.10
Z	27.4	0.10

4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting	Deviation from various Frequency Weighting Respone curve			UNCERTAINTY
FAST / 37-139	A	C	Z	
STD Setting	(dB)	(dB)	(dB)	(± dB)
125 Hz	0.1	0.2	0.2	0.60
1000 Hz	0.0	0.0	0.0	0.60
4000 Hz	0.3	0.4	0.4	0.60
8000 Hz	-0.1	0.0	0.1	0.70

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd

FM-708-SLM-01 Rev.06 Issue date 17/2/25

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL : 06610-2116-5860-1 FAX: 06610-2116-7140

Certificate No : 25-SLM-337
Request No : Req-2025-2017

5. Electrical signal test of frequency weightings, Weighting network respone with relative to 1 kHz

UUC Setting	Deviation from various Frequency			UNCERTAINTY
FAST / 37-139	Weighting Respone curve			
STD Setting	A (dB)	C (dB)	Z (dB)	(± dB)
63 Hz	-0.1	0.0	0.0	0.20
125 Hz	-0.1	0.0	0.0	
250 Hz	-0.1	0.0	0.0	
500 Hz	0.0	0.1	0.0	
1000 Hz	0.0	0.0	0.0	
2000 Hz	0.0	0.1	0.0	
4000 Hz	0.0	0.0	0.0	
8000 Hz	0.0	0.0	0.1	
16000 Hz	0.0	-0.1	-0.1	

6. Frequency and time weightings at 1kHz

UUC Setting	STD	Measured		UNCERTAINTY
FAST / 37-139	REF	UUC	ERR	
UUC Weighting	(dB)	(dB)	(dB)	(± dB)
A	114.00	114.0	0.0	0.20
C	114.00	114.0	0.0	
Z	114.00	114.0	0.0	

UUC Setting	STD	Measured		UNCERTAINTY
37-139 / A	REF	UUC	ERR	
UUC Time Respone	(dB)	(dB)	(dB)	(± dB)
Fast	114.00	114.0	0.0	0.20
Slow	114.00	114.0	0.0	
Leq	114.00	114.0	0.0	

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL : 06610-2116-5860-1 FAX: 06610-2116-7140

Certificate No : 25-SLM-337
Request No : Req-2025-2017

9. Level linearity including the level range control

UUC Setting	STD	Measured		UNCERTAINTY
FAST / A	REF	UUC	ERR	
UUC Range	(dB)	(dB)	(dB)	(± dB)
37-139	39.30	39.4	0.1	0.30
	114	114.0	0.0	

10. Tone burst response

UUC Setting	STD	Anticipated	Measured		UNCERTAINTY
A / 37-139	Toneburst	Ref	UUC	ERR	
UUC Time Respone	(ms)	(dB)	(dB)	(dB)	(± dB)
Fast	200	135.0	134.9	-0.1	0.20
	2	118.0	117.8	-0.2	
	0.25	109.0	108.8	-0.2	
Slow	200	128.6	128.5	-0.1	
	2	109.0	108.9	-0.1	
SEL	200	129.0	129.0	0.0	
	2	109.0	109.0	0.0	
	0.25	100.0	99.9	-0.1	

11. Peak C Sound level

UUC Setting	Anticipated	Measured		UNCERTAINTY
FAST / C / 95-142	REF	UUC	ERR	
STD Setting	(dB)	(dB)	(dB)	(± dB)
Complete cycle	137.4	136.7	-0.70	0.20
Positive half cycle	136.4	136.2	-0.20	
Negative half cycle	136.4	136.2	-0.20	

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

FM-708-SLM-01 Rev.06 Issue date 17/2/25

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL : 06610-2116-5860-1 FAX: 06610-2116-7140

Certificate No : 25-SLM-337
Request No : Req-2025-2017

7. Long Term Stability

UUC Setting	Measured	UNCERTAINTY
FAST / A / 37-139	UUC	
STD Setting	(dB)	(± dB)
Initial	114.0	[redacted]
Final	114.0	
Deviated	0.0	0.10

8. Level linearity on the reference level range

UUC Setting	Anticipated	Deviation		UNCERTAINTY
FAST / A / 37-139	REF	UUC	ERR	
STD dB	(dB)	(dB)	(dB)	(± dB)
136.00	136	135.9	-0.1	0.30
135.00	135	134.9	-0.1	
134.00	134	133.9	-0.1	
129.00	129	129.0	0.0	
124.00	124	124.0	0.0	
119.00	119	119.0	0.0	
114.00	114	114.0	0.0	
109.00	109	109.0	0.0	
104.00	104	104.0	0.0	
99.00	99	99.0	0.0	
94.00	94	93.9	-0.1	
89.00	89	88.9	-0.1	
84.00	84	83.9	-0.1	
79.00	79	78.9	-0.1	
74.00	74	73.9	-0.1	
69.00	69	68.9	-0.1	
64.00	64	63.9	-0.1	
59.00	59	58.9	-0.1	
54.00	54	53.9	-0.1	
49.00	49	48.9	-0.1	
44.00	44	43.9	-0.1	
39.00	39	39.1	0.1	
34.00	34	34.3	0.3	

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

FM-708-SLM-01 Rev.06 Issue date 17/2/25

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL : 06610-2116-5860-1 FAX: 06610-2116-7140

Certificate No : 25-SLM-337
Request No : Req-2025-2017

12. Overload indication

UUC Setting	Measured	UNCERTAINTY
FAST / A / 37-139	UUC	
STD Setting	(dB)	(± dB)
Positive one-half cycle	141.8	[redacted]
Negative one-half cycle	141.8	
Deviated	0.0	0.20

13. High Level Stability

UUC Setting	Measured	UNCERTAINTY
FAST / A / 37-139	UUC	
STD Setting	(dB)	(± dB)
Initial	138.0	[redacted]
Final	138.0	
Deviated	0.0	0.10

End of Certificate

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

FM-708-SLM-01 Rev.06 Issue date 17/2/25

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7-139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL : 06610-2116-5860-1 FAX: 06610-2116-7140

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

Certificate No : 25-SLM-339
Request No : Req-2025-2019

Unit Under Calibration Details

Measurement item : Sound Level Meter
Manufacturer : LARSON DAVIS
Model : LxT2
Serial Number : 0005341
ID : UAE.EFM.038/2563
Resolution : 0.1 dB

Microphone Class : 2
Microphone Model : 377B02
Microphone S/N : 11793
Preamplifier Model : PRMLxT2B
Preamplifier S/N : 056133
Instrument Status : Used

Calibration Environment and Details

Temperature : 23 °C ± 2 °C
Humidity : 50 %RH ± 20 %RH
Barometric Pressure : 1013 hPa ± 10 hPa
Received Date : 5 September 2025
Calibrated Date : 9 October 2025
Calibration Procedure : In-house method CP-SLM-01 based on IEC 61672-3 : 2013 Electroacoustics - Sound level meters - Part 3: Periodic tests
Location of Calibration : Lab Acoustic

Reference Standard

Instrument	Brand	Model	SN.	Due calibration	Traceability
Standard Microphone	Brael&Kjaer	4226	3412381	7 May 2026	NIMT
Audio Generator	Svantek	Svan401	131	27 September 2026	WK Electric

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k = 2, providing a level of confidence approximately 95 %.

Calibrated By :
Mr. Noppadon Luangart
Service Calibration Engineer

Approved By :
Mr. Pacit Mathavom
Calibration Engineer Supervisor

Issue Date : 9 October 2025

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7-139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL : 06610-2116-5860-1 FAX: 06610-2116-7140

Certificate No : 25-SLM-339
Request No : Req-2025-2019

5. Electrical signal test of frequency weightings, Weighting network respone with relative to 1 kHz

UUC Setting	Deviation from various Frequency Weighting Respone curve			UNCERTAINTY
FAST / 37-139				
STD Setting	A (dB)	C (dB)	Z (dB)	(± dB)
63 Hz	-0.2	-0.1	-0.1	0.20
125 Hz	-0.1	0.0	-0.1	
250 Hz	-0.1	-0.1	-0.1	
500 Hz	-0.1	0.0	-0.1	
1000 Hz	0.0	0.0	-0.1	
2000 Hz	0.0	0.0	0.0	
4000 Hz	0.0	0.0	0.0	
8000 Hz	-0.1	-0.1	0.0	
16000 Hz	-0.1	-0.1	-0.1	

6. Frequency and time weightings at 1kHz

UUC Setting	STD	Measured		UNCERTAINTY
FAST / 37-139	REF	UUC	ERR	
UUC Weighting	(dB)	(dB)	(dB)	(± dB)
A	114.00	114.0	0.0	0.20
C	114.00	114.0	0.0	
Z	114.00	114.0	0.0	

UUC Setting	STD	Measured		UNCERTAINTY
37-139 / A	REF	UUC	ERR	
UUC Time Respone	(dB)	(dB)	(dB)	(± dB)
Fast	114.00	114.0	0.0	0.20
Slow	114.00	114.0	0.0	
Leq	114.00	114.0	0.0	

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7-139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL : 06610-2116-5860-1 FAX: 06610-2116-7140

Certificate No : 25-SLM-339
Request No : Req-2025-2019

1. Indication at the calibration check frequency

UUC Setting	Nominal	Before Adjust		After Adjust		UNCERTAINTY
FAST / A / 37-139	Level	UUC	ERR	UUC	ERR	
Calibrator Setting	(dB)	(dB)	(dB)	(dB)	(dB)	(± dB)
1000 Hz 114 dB	113.75	113.9	0.15	113.7	-0.05	0.20

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, SN. 58079

2. Self-generated noise, Microphone installed

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139		
UUC Weighting	(dB)	(± dB)
A	29.3	0.10

3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139		
UUC Weighting	(dB)	(± dB)
A	28.9	0.10
C	28.6	0.10
Z	32.8	0.10

4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting	Deviation from various Frequency Weighting Respone curve			UNCERTAINTY
FAST / 37-139	A	C	Z	(± dB)
STD Setting	(dB)	(dB)	(dB)	
125 Hz	0.2	0.2	0.2	0.60
1000 Hz	0.0	0.0	0.0	0.60
4000 Hz	1.1	1.2	1.1	0.60
8000 Hz	0.4	0.4	0.4	0.70

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7-139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL : 06610-2116-5860-1 FAX: 06610-2116-7140

Certificate No : 25-SLM-339
Request No : Req-2025-2019

7. Long Term Stability

UUC Setting	Measured	UNCERTAINTY
FAST / A / 37-139	UUC	
STD Setting	(dB)	(± dB)
Initial	114.0	
Final	114.0	
Deviated	0.0	0.10

8. Level linearity on the reference level range

UUC Setting	Anticipated	Deviation		UNCERTAINTY
FAST / A / 37-139	REF	UUC	ERR	
STD dB	(dB)	(dB)	(dB)	(± dB)
139.00	139	139.0	0.0	0.30
134.00	134	134.0	0.0	
129.00	129	129.0	0.0	
124.00	124	124.0	0.0	
119.00	119	119.0	0.0	
114.00	114	114.0	0.0	
109.00	109	109.0	0.0	
104.00	104	104.0	0.0	
99.00	99	99.0	0.0	
94.00	94	94.0	0.0	
89.00	89	89.0	0.0	
84.00	84	84.0	0.0	
79.00	79	79.0	0.0	
74.00	74	74.0	0.0	
69.00	69	69.0	0.0	
64.00	64	64.0	0.0	
59.00	59	59.0	0.0	
54.00	54	54.0	0.0	
49.00	49	49.1	0.1	
44.00	44	44.2	0.2	
39.00	39	39.5	0.5	
38.00	38	38.7	0.7	

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7 139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 06610-2116-5869-1 FAX: 06610-2116-7140

Certificate No : 25-SLM-339
Request No : Req-2025-2019

9. Level linearity including the level range control

UUC Setting	STD	Measured		UNCERTAINTY
FAST / A	REF	UUC	ERR	
UUC Range	(dB)	(dB)	(dB)	(± dB)
37-139	43.70	43.9	0.2	0.30
	114	114.0	0.0	

10. Tone burst response

UUC Setting	STD	Anticipated	Measured		UNCERTAINTY
A / 37-139	Toneburst	Ref	UUC	ERR	
UUC Time Respone	(ms)	(dB)	(dB)	(dB)	(± dB)
Fast	200	135.0	134.9	-0.1	0.20
	2	118.0	117.6	-0.4	
	0.25	109.0	108.6	-0.4	
Slow	200	128.6	128.4	-0.2	
	2	109.0	108.8	-0.2	
SEL	200	129.0	129.0	0.0	
	2	109.0	109.0	0.0	
	0.25	100.0	99.9	-0.1	

11. Peak C Sound level

UUC Setting	Anticipated	Measured		UNCERTAINTY
FAST / C / 95-142	REF	UUC	ERR	
STD Setting	(dB)	(dB)	(dB)	(± dB)
Complete cycle	137.4	136.8	-0.60	0.20
Positive half cycle	136.4	136.2	-0.20	
Negative half cycle	136.4	136.2	-0.20	

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7 139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 06610-2116-5869-1 FAX: 06610-2116-7140

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

Certificate No : 25-SLM-340
Request No : Req-2025-2024

Unit Under Calibration Details

Measurement item : Sound Level Meter
Manufacturer : LARSON DAVIS
Model : LxT2
Serial Number : 0005343
ID : UAE.IFM.049/2563
Resolution : 0.1 dB

Microphone Class : 2
Microphone Model : 375A04
Microphone S/N : 368644
Preamplifier Model : PRMLxT2B
Preamplifier S/N : 056135
Instrument Status : Used

Calibration Environment and Details

Temperature : 23 °C ± 2 °C
Humidity : 50 %RH ± 20 %RH
Barometric Pressure : 1013 hPa ± 10 hPa
Received Date : 5 September 2025
Calibrated Date : 10 October 2025
Calibration Procedure : In-house method CP-SLM-01 based on IEC 61672-3 : 2013 Electroacoustics - Sound level meters - Part 3: Periodic tests
Location of Calibration : Lab Acoustic

Reference Standard

Instrument	Brand	Model	SN	Due calibration	Traceability
Standard Microphone	Brüel&Kjaer	4226	3412381	7 May 2026	NIMT
Audio Generator	Svantek	Svan401	131	27 September 2026	WK Electric

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k = 2$, providing a level of confidence approximately 95 %.

Calibrated By :
Mr. Noppadon Luangart
Service Calibration Engineer

Approved By :
Mr. Pacit Mathavorn
Calibration Engineer Supervisor

Issue Date : 10 October 2025

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7 139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 06610-2116-5869-1 FAX: 06610-2116-7140

Certificate No : 25-SLM-339
Request No : Req-2025-2019

12. Overload indication

UUC Setting	Measured	UNCERTAINTY
FAST / A / 37-139	UUC	
STD Setting	(dB)	(± dB)
Positive one-half cycle	142.7	[redacted]
Negative one-half cycle	142.7	
Deviated	0.0	0.20

13. High Level Stability

UUC Setting	Measured	UNCERTAINTY
FAST / A / 37-139	UUC	
STD Setting	(dB)	(± dB)
Initial	138.0	[redacted]
Final	138.0	
Deviated	0.0	0.10

End of Certificate

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7 139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 06610-2116-5869-1 FAX: 06610-2116-7140

Certificate No : 25-SLM-340
Request No : Req-2025-2024

1. Indication at the calibration check frequency

UUC Setting	Nominal	Before Adjust		After Adjust		UNCERTAINTY
FAST / A / 37-139	Level	UUC	ERR	UUC	ERR	
Calibrator Setting	(dB)	(dB)	(dB)	(dB)	(dB)	(± dB)
1000 Hz 114 dB	113.75	113.6	-0.15	113.7	-0.05	0.20

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, SN. 58079

2. Self-generated noise, Microphone installed

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139		
UUC Weighting	(dB)	(± dB)
A	24.7	0.10

3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139		
UUC Weighting	(dB)	(± dB)
A	23.9	0.10
C	23.3	0.10
Z	27.6	0.10

4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting	Deviation from various Frequency Weighting Respone curve			UNCERTAINTY
FAST / 37-139	A	C	Z	
STD Setting	(dB)	(dB)	(dB)	(± dB)
125 Hz	0.1	0.2	0.2	0.60
1000 Hz	0.0	0.0	0.0	0.60
4000 Hz	0.6	0.7	0.7	0.60
8000 Hz	1.0	1.1	1.1	0.70

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7 139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL : 06610-2116-5860-1 FAX: 06610-2116-7140

Certificate No : 25-SLM-340
Request No : Req-2025-2024

5. Electrical signal test of frequency weightings, Weighting network respone with relative to 1 kHz

UUC Setting	Deviation from various Frequency Weighting Respone curve			UNCERTAINTY
FAST / 37-139				
STD Setting	A (dB)	C (dB)	Z (dB)	(± dB)
63 Hz	-0.1	0.0	0.0	0.20
125 Hz	-0.1	0.0	0.0	
250 Hz	-0.1	0.0	0.0	
500 Hz	0.0	0.0	0.0	
1000 Hz	0.0	0.0	0.0	
2000 Hz	0.0	0.1	0.0	
4000 Hz	0.0	0.0	0.0	
8000 Hz	0.0	0.0	0.0	
16000 Hz	0.0	-0.1	-0.1	

6. Frequency and time weightings at 1kHz

UUC Setting	STD	Measured		UNCERTAINTY
FAST / 37-139	REF	UUC	ERR	
UUC Weighting	(dB)	(dB)	(dB)	(± dB)
A	114.00	114.0	0.0	0.20
C	114.00	114.0	0.0	
Z	114.00	114.0	0.0	

UUC Setting	STD	Measured		UNCERTAINTY
37-139 / A	REF	UUC	ERR	
UUC Time Respone	(dB)	(dB)	(dB)	(± dB)
Fast	114.00	114.0	0.0	0.20
Slow	114.00	114.0	0.0	
Leq	114.00	114.0	0.0	

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7 139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL : 06610-2116-5860-1 FAX: 06610-2116-7140

Certificate No : 25-SLM-340
Request No : Req-2025-2024

9. Level linearity including the level range control

UUC Setting	STD	Measured		UNCERTAINTY
FAST / A	REF	UUC	ERR	
UUC Range	(dB)	(dB)	(dB)	(± dB)
37-139	39.60	39.7	0.1	0.30
	114	114.0	0.0	

10. Tone burst response

UUC Setting	STD	Anticipated	Measured		UNCERTAINTY
A / 37-139	Toneburst	Ref	UUC	ERR	
UUC Time Respone	(ms)	(dB)	(dB)	(dB)	(± dB)
Fast	200	135.0	135.0	0.0	0.20
	2	118.0	117.8	-0.2	
	0.25	109.0	108.8	-0.2	
Slow	200	128.6	128.5	-0.1	
	2	109.0	108.9	-0.1	
SEL	200	129.0	129.1	+0.1	
	2	109.0	109.0	0.0	
	0.25	100.0	99.9	-0.1	

11. Peak C Sound level

UUC Setting	Anticipated	Measured		UNCERTAINTY
FAST / C / 95-142	REF	UUC	ERR	
STD Setting	(dB)	(dB)	(dB)	(± dB)
Complete cycle	137.4	136.7	-0.70	0.20
Positive half cycle	136.4	136.1	-0.30	
Negative half cycle	136.4	136.1	-0.30	

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7 139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL : 06610-2116-5860-1 FAX: 06610-2116-7140

Certificate No : 25-SLM-340
Request No : Req-2025-2024

7. Long Term Stability

UUC Setting	Measured	UNCERTAINTY
FAST / A / 37-139	UUC	
STD Setting	(dB)	(± dB)
Initial	114.0	[redacted]
Final	114.0	
Deviated	0.0	0.10

8. Level linearity on the reference level range

UUC Setting	Anticipated	Deviation		UNCERTAINTY
FAST / A / 37-139	REF	UUC	ERR	
STD dB	(dB)	(dB)	(dB)	(± dB)
136.00	136	136.0	0.0	0.30
135.00	135	135.0	0.0	
134.00	134	134.0	0.0	
129.00	129	129.0	0.0	
124.00	124	124.0	0.0	
119.00	119	119.0	0.0	
114.00	114	114.0	0.0	
109.00	109	109.0	0.0	
104.00	104	104.0	0.0	
99.00	99	99.0	0.0	
94.00	94	94.0	0.0	
89.00	89	89.0	0.0	
84.00	84	84.0	0.0	
79.00	79	79.0	0.0	
74.00	74	74.0	0.0	
69.00	69	69.0	0.0	
64.00	64	64.0	0.0	
59.00	59	59.0	0.0	
54.00	54	54.0	0.0	
49.00	49	49.0	0.0	
44.00	44	44.0	0.0	
39.00	39	39.2	0.2	
34.00	34	34.4	0.4	

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7 139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL : 06610-2116-5860-1 FAX: 06610-2116-7140

Certificate No : 25-SLM-340
Request No : Req-2025-2024

12. Overload indication

UUC Setting	Measured	UNCERTAINTY
FAST / A / 37-139	UUC	
STD Setting	(dB)	(± dB)
Positive one-half cycle	141.2	[redacted]
Negative one-half cycle	141.2	
Deviated	0.0	0.20

13. High Level Stability

UUC Setting	Measured	UNCERTAINTY
FAST / A / 37-139	UUC	
STD Setting	(dB)	(± dB)
Initial	138.0	[redacted]
Final	138.0	
Deviated	0.0	0.10

End of Certificate

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7 139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 06602116-5860-1 FAX: 06602116-7140

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.

Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

Certificate No : 25-ACT-137
Request No : Req-2025-1828

Unit Under Calibration Details

Measurement item : Acoustic Calibrator
Manufacturer : LARSON DAVIS
Model : CAL150
Serial Number : 6855
ID : UAE.EFM.046/2566

Class : 2
Range : 94 , 114 dB 1000 Hz
Instrument Status : Used

Calibration Environment and Details

Temperature : (23 ±2 °C)
Humidity : (50 ± 20 %RH)
Barometric Pressure : (1013 ±10.0 hPa)
Received Date : 7 August 2025
Calibration Date : 9 September 2025
Location of Calibration : LAB 1 Acoustic
Calibration Procedure : In-house method CP-ACT-02 based on IEC 60942:2017 Electroacoustics - Sound calibrators

Reference Standard	Model	Serial Number	Traceable	Due Calibration
Sound Calibrator	SV 35A	58079	EEI	20 June 2026
THD Multimeter	2015	1047765	NIMT	4 February 2026

Traceability : This certificate providoes traceability of measurement to recognized national standard, and to the realization of the international System of Units (SI).

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k =2, providing a level of confidence approximately 95 %.

Calibrated By : Mr. Noppadon Luangart
Service Calibration Engineer

Approved By : Mr. Pacit Mathavorn
Calibration Engineer Supervisor

Issue Date : 9 September 2025

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.
เอกสารไม่ควบคุม

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7 139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 06602116-5860-1 FAX: 06602116-7140

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

Certificate No : 26-SLM-216
Request No : Req-2026-1168

Unit Under Calibration Details

Measurement item : Sound Level Meter
Manufacturer : LARSON DAVIS
Model : LxT2
Serial Number : 0005399
ID : UAE.EFM.036/2564
Resolution : 0.1 dB

Microphone Class : 2
Microphone Model : 375A04
Microphone S/N : 373079
Preamplifier Model : PRMLxT2B
Preamplifier S/N : 071560
Instrument Status : Used

Calibration Environment and Details

Temperature : 23 °C ± 2 °C
Humidity : 50 %RH ± 20 %RH
Barometric Pressure : 1013 hPa ± 10 hPa
Received Date : 7 May 2026
Calibrated Date : 2 June 2026
Calibration Procedure : In-house method CP-SLM-01 based on IEC 61672-3 : 2013 Electroacoustics - Sound level meters - Part 3: Periodic tests
Location of Calibration : Lab Acoustic

Reference Standard

Instrument	Brand	Model	SN.	Due calibration	Traceability
Standard Microphone	Bruel&Kjaer	4226	3412381	15 May 2027	NIMT
Audio Generator	Svantek	Svan401	131	27 September 2026	WK Electric

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k = 2, providing a level of confidence approximately 95 %.

Calibrated By : Mr. Noppadon Luangart
Service Calibration Engineer

Approved By : Mr. Jedsada Thongyoi
Lab Manager

Issue Date : 2 June 2026

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.
เอกสารไม่ควบคุม

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7 139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 06602116-5860-1 FAX: 06602116-7140

Certificate No : 25-ACT-137
Request No : Req-2025-1828

Sound pressure level — **Calibration Results :** Without Adjustment

Calibration Range (dB)	Without Adjustment (dB)		Adjustment (dB)		Uncertainty (± dB)
	Measured	Deviated value	Measured	Deviated value	
94 dB / 1000 Hz	93.81	-0.19	-	-	0.11
114 dB / 1000 Hz	113.94	-0.06	-	-	0.11

Frequency of Sound pressure level

Calibration Range (Hz)	Without Adjustment		Adjustment		Uncertainty (± %)
	Measured (Hz)	Deviated value	Measured (Hz)	Deviated value	
94 dB / 1000 Hz	1000.00	0.00	-	-	0.01
114 dB /1000 Hz	1000.00	0.00	-	-	0.01

Total Harmonic Distortion plus Noise of Sound pressure level (THD+N %)

Calibration Range (Hz)	Without Adjustment	Adjustment	Uncertainty (± %)
	Measured (%)	Measured (%)	
94 dB / 1000 Hz	1.18	-	0.17
114 dB / 1000 Hz	0.63	-	0.17

Note :

- The calibration results exclude the calibrator pressure correction
- The calibration results exclude the microphone volume correction

End of Calibration

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.
เอกสารไม่ควบคุม

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7 139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 06602116-5860-1 FAX: 06602116-7140

Certificate No : 26-SLM-216
Request No : Req-2026-1168

1. Indication at the calibration check frequency

UUC Setting	Nominal	Before Adjust		After Adjust		UNCERTAINTY
FAST / A / 37-139	Level	UUC	ERR	UUC	ERR	
Calibrator Setting	(dB)	(dB)	(dB)	(dB)	(dB)	(± dB)
1000 Hz 114 dB	113.75	113.6	-0.15	113.7	-0.05	0.20

Note : Absolute sensitivity was established by the use of Multifunction Acoustic Calibrator Brand SVANTEK, Model SV 35A, SN. 58079

2. Self-generated noise, Microphone installed

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139		
UUC Weighting	(dB)	(± dB)
A	23.7	0.10

3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139		
UUC Weighting	(dB)	(± dB)
A	23.0	0.10
C	22.2	0.10
Z	26.6	0.10

4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting	Deviation from various Frequency Weighting Respone curve			UNCERTAINTY
FAST / 37-139	A	C	Z	
STD Setting	(dB)	(dB)	(dB)	(± dB)
125 Hz	0.2	0.2	0.2	0.60
1000 Hz	0.0	0.0	0.0	0.60
4000 Hz	-0.1	-0.1	-0.1	0.60
8000 Hz	-0.8	-0.7	-0.7	0.70

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.
เอกสารไม่ควบคุม

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7 139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 06(0)-2116-5860-1 FAX: 06(0)-2116-7140

Certificate No : 26-SLM-216
Request No : Req-2026-1168

5. Electrical signal test of frequency weightings, Weighting network respone with relative to 1 kHz

UUC Setting	Deviation from various Frequency Weighting Respone curve			UNCERTAINTY
FAST / 37-139				
STD Setting	A (dB)	C (dB)	Z (dB)	(± dB)
63 Hz	-0.1	0.0	0.0	0.20
125 Hz	-0.1	0.1	0.0	
250 Hz	0.0	0.0	0.0	
500 Hz	0.0	0.1	0.0	
1000 Hz	0.0	0.0	0.0	
2000 Hz	0.1	0.1	0.0	
4000 Hz	0.0	0.1	0.1	
8000 Hz	0.0	0.0	0.1	
16000 Hz	0.0	0.0	-0.1	

6. Frequency and time weightings at 1kHz

UUC Setting	STD	Measured		UNCERTAINTY
FAST / 37-139	REF	UUC	ERR	
UUC Weighting	(dB)	(dB)	(dB)	(± dB)
A	114.00	114.0	0.0	0.20
C	114.00	114.0	0.0	
Z	114.00	114.0	0.0	

UUC Setting	STD	Measured		UNCERTAINTY
37-139 / A	REF	UUC	ERR	
UUC Time Respone	(dB)	(dB)	(dB)	(± dB)
Fast	114.00	114.0	0.0	0.20
Slow	114.00	114.0	0.0	
Leq	114.00	114.0	0.0	

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the laboratory. This report is only
FM-708-SLM-01 Rev.0 Issue date 17/2/25
เอกสารไม่ควบคุม

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7 139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 06(0)-2116-5860-1 FAX: 06(0)-2116-7140

Certificate No : 26-SLM-216
Request No : Req-2026-1168

9. Level linearity including the level range control

UUC Setting	STD	Measured		UNCERTAINTY
FAST / A	REF	UUC	ERR	
UUC Range	(dB)	(dB)	(dB)	(± dB)
37-139	38.60	38.8	0.2	0.30
	114	114.0	0.0	

10. Tone burst response

UUC Setting	STD	Anticipated	Measured		UNCERTAINTY
A / 37-139	Toneburst	Ref	UUC	ERR	
UUC Time Respone	(ms)	(dB)	(dB)	(dB)	(± dB)
Fast	200	135.0	135.0	0.0	0.20
	2	118.0	117.6	-0.4	
	0.25	109.0	108.8	-0.2	
Slow	200	128.6	128.5	-0.1	
	2	109.0	108.9	-0.1	
SEL	200	129.0	129.0	0.0	
	2	109.0	109.0	0.0	
	0.25	100.0	99.9	-0.1	

11. Peak C Sound level

UUC Setting	Anticipated	Measured		UNCERTAINTY
FAST / C / 95-142	REF	UUC	ERR	
STD Setting	(dB)	(dB)	(dB)	(± dB)
Complete cycle	137.4	136.5	-0.90	0.20
Positive half cycle	136.4	136.1	-0.30	
Negative half cycle	136.4	136.1	-0.30	

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the laboratory. This report is only
FM-708-SLM-01 Rev.0 Issue date 17/2/25
เอกสารไม่ควบคุม

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7 139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 06(0)-2116-5860-1 FAX: 06(0)-2116-7140

Certificate No : 26-SLM-216
Request No : Req-2026-1168

7. Long Term Stability

UUC Setting	Measured	UNCERTAINTY
FAST / A / 37-139	UUC	
STD Setting	(dB)	(± dB)
Initial	114.0	[redacted]
Final	114.0	
Deviated	0.0	0.10

8. Level linearity on the reference level range

UUC Setting	Anticipated	Deviation		UNCERTAINTY
FAST / A / 37-139	REF	UUC	ERR	
STD dB	(dB)	(dB)	(dB)	(± dB)
139.00	139	139.0	0.0	0.30
134.00	134	134.0	0.0	
129.00	129	129.0	0.0	
124.00	124	124.0	0.0	
119.00	119	119.0	0.0	
114.00	114	114.0	0.0	
109.00	109	109.0	0.0	
104.00	104	104.0	0.0	
99.00	99	99.0	0.0	
94.00	94	94.0	0.0	
89.00	89	89.0	0.0	
84.00	84	84.0	0.0	
79.00	79	79.0	0.0	
74.00	74	74.0	0.0	
69.00	69	69.0	0.0	
64.00	64	64.0	0.0	
59.00	59	59.0	0.0	
54.00	54	54.0	0.0	
49.00	49	49.0	0.0	
44.00	44	44.0	0.0	
39.00	39	39.1	0.1	
34.00	34	34.3	0.3	
33.00	33	33.4	0.4	

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the laboratory. This report is only
FM-708-SLM-01 Rev.0 Issue date 17/2/25
เอกสารไม่ควบคุม

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7 139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 06(0)-2116-5860-1 FAX: 06(0)-2116-7140

Certificate No : 26-SLM-216
Request No : Req-2026-1168

12. Overload indication

UUC Setting	Measured	UNCERTAINTY
FAST / A / 37-139	UUC	
STD Setting	(dB)	(± dB)
Positive one-half cycle	140.2	[redacted]
Negative one-half cycle	140.0	
Deviated	0.2	0.20

13. High Level Stability

UUC Setting	Measured	UNCERTAINTY
FAST / A / 37-139	UUC	
STD Setting	(dB)	(± dB)
Initial	138.0	[redacted]
Final	138.0	
Deviated	0.0	0.10

End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the laboratory. This report is only
FM-708-SLM-01 Rev.0 Issue date 17/2/25
เอกสารไม่ควบคุม

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

Certificate of Calibration

Cert.No.: 25CH1182
Page.: 1 of 3

Equipment : pH Meter
Manufacturer : EcoSense
Model : pH100A
Serial No. : 24H005160JEN
ID No. : UAE.EFM.042/2567(EFM.pH.05/67)
Condition As-Received: Used Item
Received Date : 14 October 2025
Calibration Date : 15 October 2025
Reference : 2510-0389WSC-2
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260
Ambient Temperature : (25 ± 2.5) °C
Relative Humidity : (50 ± 15) %
Calibration Procedure : In - house method :
- CP-CH5 by direct measurement with DC voltage standard and direct measurement with certified reference material (CRM)
- CP-CH8 by comparison with temperature standard

Calibrated by : Walalak Sirithean

Approved by : Approved Signatory

(✓) Chakrit Waewwanjua
( ) Ponpan Paipim
( ) Saithip Meangmai

Issue Date : 17 October 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7)(7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (±)	Coverage factor k
pH Electrode	4.007	4.01	161	0.0091	2.07
S/N.: 240904SIA805377	6.999	7.00	-12	0.0095	2.00
	6.999	7.00	-14	0.0092	2.00
	10.010	10.02	-186	0.0095	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;
- Model : -
- Serial No. : 240904SIA805377

Dimension of probe
- Length : 110 mm.
- Diameter : 12 mm.
- Immersion Depth : 100 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (± °C)	Coverage factor k
15.0	15.001	15.0	-0.001	0.13	2.00
30.0	30.002	29.9	-0.102	0.13	2.00
45.0	45.002	44.8	-0.202	0.13	2.00

Remark - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม

Condition of this calibration result

1. Reference Standard Instrument

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1) Document Process Calibrator	54030049	130RC116	25E2743	25 Aug 2026
2) Ref. Standard Thermometer	4982054	110RC044	25I708	03 July 2026

- This measurement result is traceable to SI throught Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials ;The measurement results are traceable to SI through Hach Lenge GmbH Ltd., Deutsche Akkreditierungsstelle, Accredited No.D-RM-15184-01-00
;The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.007	CPA chem	1114384	12 June 2027
pH 6.999	Hach Lenge GmbH	C03273	13 May 2027
pH 10.010	CPA chem	1135355	16 Aug 2026

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4,7)(7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement	Coverage factor
	pH	mV	mV	pH	(±mV)	k
pH Meter	4.00	177.48	177	4.01	0.58	2.00
S/N.: 24H005160JEN	7.00	0.00	0	7.00	0.58	2.00
	7.00	0.00	0	7.00	0.58	2.00
	10.00	-177.48	-177	10.01	0.58	2.00

เอกสารไม่ควบคุม

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000 FAX. 0-2719-9484

Certificate of Testing

Cert.No.: 25TW108
Page.: 1 of 2

Equipment : DO Meter
Manufacturer : Horiba
Model : LAQUA-DO210
Serial No. : HE2L0036
ID No. : UAE.EFM.018/2566(EFM.DO.03/66)
Received Date : 20 May 2025
Test Date : 21 May 2025
Reference : 2505-0605WSC-7
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260
Laboratory Condition : Temperature (25 ± 5) °C
Humidity (50 ± 20) %
Test Procedure : In - house method : CP-CH9
by Comparison Technique with Azide Modification Method

Tested by : Walalak Sirithean

Approved by : Approved Signatory

( ) Chakrit Waewwanjua
( ) Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 23 May 2025

เอกสารไม่ควบคุม

Condition of this result of calibration

1. Reference Standard Instruments :
   This measurement result is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

Instruments	Serial No.	ID No.	Certificate No.	Due Date
1. Burette	-	130BU10	25CG1126	18 Mar 2027
2. Balance	14233821	110RC001	24MM131	04 July 2025

2. Standard Material :-

Material	Manufacturer	Lot.No.	Assay
Sodium Thiosulfate 5-Hydrate AR	KEMAUS	2203162447	99.6%

Result : **Dissolved Oxygen Meter Adjustment With Air 100 %**
Dissolved Oxygen Probe No.: 9K0L0009

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.22	8.22	0.0071

This report was certified only for the instrument we tested.It is allowable to use for study Intend to use for advertising and referral purpose is prohibited.This report may not be reproduced other in full, without written approval of the laboratory

-o0o-

เอกสารไม่ควบคุม

Equipment : DO Meter with Sensor
Condition As-Received : Used Item
Reference : 2505-0605WSC-8

Procedure Used :-
Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.
The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Digital Thermometer	2188080	24I1022	TPA	17 Sep 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)
Result of Calibration :- (*) Without Adjustment
Function : Temperature measurement.
This instrument was connected with thermistor sensor , S/N.: 9K0L0009

Calibration Point (°C)	Immersion Depth (mm)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty (± °C)	Coverage Factor *k*
15.0	100	15.004	15.2	0.196	0.16	2.00
30.0	100	30.005	30.1	0.095	0.16	2.00
45.0	100	45.006	45.0	-0.006	0.16	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor ***k***, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

ilac-MRA
NSC-TISI-TIS17025 CALIBRATION 0008

Certificate of Calibration

Equipment : DO Meter with Sensor
Manufacturer : Horiba
Model : LAQUA-DO210
Serial No. : HE2L0036
ID No. : UAE.EFM.018/2566(EFM.DO.03/66)
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260
Location : TPA On Site Calibration Laboratory

Received Order : 20 May 2025
Calibrated Date : 22 May 2025
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %
AC Line Voltage : (220 ± 22) V

Calibrated by : Preecha Hlahib
Approved by : Kunchit
Approved Signatory

( ) Chakrit Waewwanjua
( ) Suwit Imjai
(✓) Kunchit Promprat

Issue Date : 28 May 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

ilac-MRA
NSC-TISI-TIS17025 CALIBRATION 0008

Certificate of Calibration

Equipment : Conductivity Meter
Manufacturer : YSI Environmental
Model : Pro 30
Serial No. : 18K100976
ID No. : UAE.EFM.071/2562(ENV.SCT.01/62)
Condition As-Received: Used Item
Received Date : 14 October 2025
Calibration Date : 15 October 2025
Reference : 2510-0392WSC-1
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260
Ambient Temperature : (25 ± 2.5) °C
Relative Humidity : (50 ± 15) %
Calibration Procedure: In -house method :
- CP-CH6 by direct measurement with certified reference material (CRM)
- CP-CH8 by comparison with temperature standard

Calibrated by : Walalak Sirithean
Approved by :
Approved Signatory

(✓) Chakrit Waewwanjua
( ) Ponpan Paipim
( ) Saithip Meangmai

Issue Date : 17 October 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

Condition of this result of calibration

1. Reference Standard Instrument :-

Instrument	Serial No.	ID No.	Certificate No.	Due date
1) Thermometer	9549224	130RC003	25I440	16 Apr 2026
2) Ref. Std.Thermometer	4982054	110RC044	25I708	03 July 2026

- This measurement result is traceable to SI throught Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials :-

- Conductivity calibration solution, CPA chem Ltd., The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Conductivity Solution	Manufacturer	Lot No.	Exp. date
1413.5 µS/cm	CPA Chem	1135361	16 Aug 2026
12.881 mS/cm	CPA Chem	1081099	11 Mar 2026

- Control Conductivity calibration solution temperature by Water bath (25 ± 0.1) °C

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration results

Function : Conductivity Measurement

(*) After Adjustment at 1413.5 µS/cm

Conductivity Electrode Serial No.: 18L100008

Standard Conductivity Solution	Before Adjustment UUC* Reading	After Adjustment UUC* Reading	Uncertainty of Measurement (±)	Coverage factor *k*
1413.5 µS/cm	1415 µS/cm	1414 µS/cm	9.2 µS/cm	2.00
12.881 mS/cm	12.91 mS/cm	12.88 mS/cm	0.086 mS/cm	2.00

Remark : **- UUC* = Unit Under Calibration**

เอกสารไม่ควบคุม

United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel. 0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

MULTI-POINT GAS TEST REPORT


Test Date : Feb 17,2026

Equipment :	Gas Analyzer (NO_2)	**Model :**	42i
Manufacturer :	Thermo Scientific	**Serial Number :**	CM22387035

Standard Gas Concentration			**Dilutor Detail**	
Sulphur Dioxide (SO_2)	42.89 PPM		Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	46.77 PPM		Model :	146i
Methane (CH_4)	- PPM		Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB0159156			
Expiration Date :	Nov 6,2026			

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.8	0.80	0.79	0.79
Level 3	40.00%	200.0	200.5	0.50	0.25	0.25
Level 4	60.00%	300.0	300.7	0.70	0.23	0.23
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range :Acceptable Limit ± 5%		500.0 ppb		Average Difference (%)		0.26

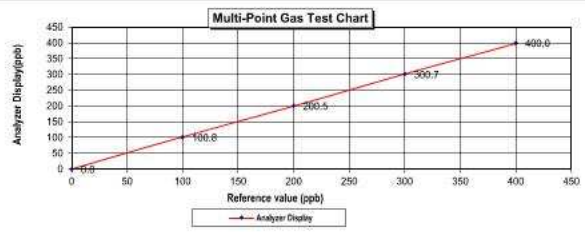

Calculate by ....17.../...02...../...2569.

Approve by ....17.../...Feb.../...2026.

เอกสารไม่ควบคุม

Calibration Results

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : PRO30 COND-T
- Serial No. : 18L100008

Dimension of probe;

- Length : 93.6 mm
- Diameter : 2.7 mm
- Immersion Depth : 90 mm

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of Measurement (± °C)	Coverage factor *k*
15.0	15.002	14.9	-0.102	0.13	2.00
30.0	30.002	29.9	-0.102	0.13	2.00
45.0	45.001	44.9	-0.102	0.13	2.00

Remark : - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม

United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel. 0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

MULTI-POINT GAS TEST REPORT


Test Date : Feb 17,2026

Equipment :	Gas Analyzer (NO_2)	**Model :**	42i
Manufacturer :	Thermo Scientific	**Serial Number :**	CM08130002

Standard Gas Concentration			**Dilutor Detail**	
Sulphur Dioxide (SO_2)	42.89 PPM		Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	46.77 PPM		Model :	146i
Methane (CH_4)	- PPM		Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB0159156			
Expiration Date :	Nov 6,2026			

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.9	0.90	0.89	0.89
Level 3	40.00%	200.0	200.7	0.70	0.35	0.35
Level 4	60.00%	300.0	300.8	0.80	0.27	0.27
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range :Acceptable Limit ± 5%		500.0 ppb		Average Difference (%)		0.30

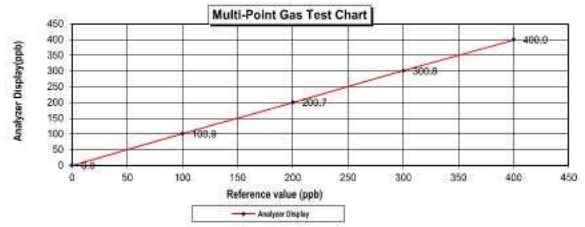

Calculate by ....17.../...02...../...2569.

Approve by ....17.../...Feb.../...2026.

เอกสารไม่ควบคุม

United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel. 0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

MULTI-POINT GAS TEST REPORT

Test Date : Feb 20,2026


Equipment :	Gas Analyzer (NO_2)	**Model :**	42i
Manufacturer :	Thermo Scientific	**Serial Number :**	CM19050148

Standard Gas Concentration			**Dilutor Detail**	
Sulphur Dioxide (SO_2)	42.89 PPM		Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	46.77 PPM		Model :	146i
Methane (CH_4)	- PPM		Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB0159156			
Expiration Date :	Nov 6,2026			

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.6	0.60	0.60	0.60
Level 3	40.00%	200.0	200.7	0.70	0.35	0.35
Level 4	60.00%	300.0	300.9	0.90	0.30	0.30
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range 500.0 ppb				Average Difference (%)		0.25

:Acceptable Limit ± 5%

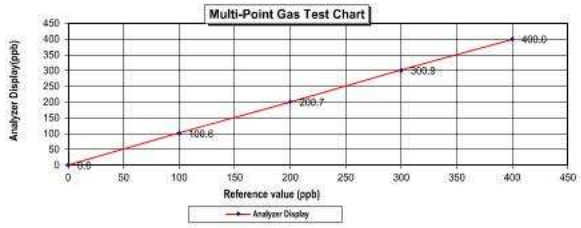

Calculate by ..... **Approve by** .....

20 / 02 / 2569 20 / Feb / 2026

เอกสารไม่ควบคุม

United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel. 0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

MULTI-POINT GAS TEST REPORT

Test Date : Feb 24,2026


Equipment :	Gas Analyzer (NO_2)	**Model :**	42i
Manufacturer :	Thermo Scientific	**Serial Number :**	CM19050150

Standard Gas Concentration			**Dilutor Detail**	
Sulphur Dioxide (SO_2)	42.89 PPM		Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	46.77 PPM		Model :	146i
Methane (CH_4)	- PPM		Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB0159156			
Expiration Date :	Nov 06,2026			

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.6	0.60	0.60	0.60
Level 3	40.00%	200.0	200.3	0.30	0.15	0.15
Level 4	60.00%	300.0	300.5	0.50	0.17	0.17
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range 500.0 ppb				Average Difference (%)		0.18

:Acceptable Limit ± 5%

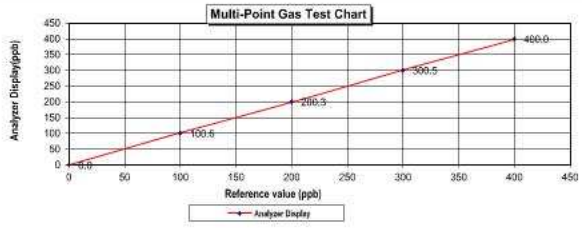

Calculate by ..... **Approve by** .....

24 / 02 / 2569 24 / Feb / 2026

เอกสารไม่ควบคุม

United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel. 0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

MULTI-POINT GAS TEST REPORT

Test Date : Feb 24,2026


Equipment :	Gas Analyzer (NO_2)	**Model :**	42i
Manufacturer :	Thermo Scientific	**Serial Number :**	CM19050149

Standard Gas Concentration			**Dilutor Detail**	
Sulphur Dioxide (SO_2)	42.89 PPM		Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	46.77 PPM		Model :	146i
Methane (CH_4)	- PPM		Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB0159156			
Expiration Date :	Nov 06,2026			

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.8	0.80	0.79	0.79
Level 3	40.00%	200.0	201.9	1.90	0.94	0.94
Level 4	60.00%	300.0	300.4	0.40	0.13	0.13
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range 500.0 ppb				Average Difference (%)		0.37

:Acceptable Limit ± 5%

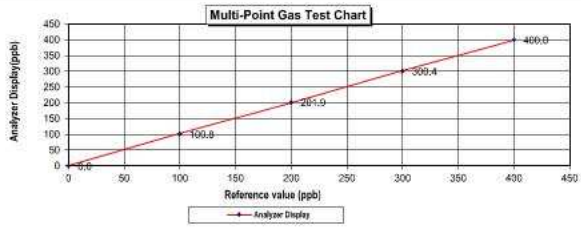

Calculate by ..... **Approve by** .....

24 / 02 / 2569 24 / Feb / 2026

เอกสารไม่ควบคุม

Airgas
an Air Liquide company

Airgas Specialty Gases
Airgas USA LLC
630 United Drive
Durham, NC 27713
Airgas.com

CERTIFICATE OF ANALYSIS

Grade of Product: EPA PROTOCOL STANDARD

Customer:	AIR LIQUIDE (THAILAND) LTD		
Part Number:	E04NI99E15A01D3	Reference Number:	122-402880224-1
Cylinder Number:	EB0159156	Cylinder Volume:	144.0 CF
Laboratory:	124 - Durham (SAP) - NC	Cylinder Pressure:	2015 PSIG
PGVP Number:	B22023	Valve Outlet:	660
Gas Code:	CO,NO,NOX,SO2,BALN	Certification Date:	Nov 06, 2023

Expiration Date: Nov 06, 2026

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA-600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results relate only to the items tested. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS

Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	45.00 PPM	46.78 PPM	G1	+/- 1.3% NIST Traceable	10/30/2023, 11/06/2023
NITRIC OXIDE	45.00 PPM	46.77 PPM	G1	+/- 1.3% NIST Traceable	10/30/2023, 11/06/2023
SULFUR DIOXIDE	45.00 PPM	42.89 PPM	G1	+/- 1.0% NIST Traceable	10/30/2023, 11/06/2023
CARBON MONOXIDE	1000 PPM	965.9 PPM	G1	+/- 0.7% NIST Traceable	10/30/2023
NITROGEN	Balance				

CALIBRATION STANDARDS

Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
NTRM	21060703	CC707954	48.41 PPM NITRIC OXIDE/NITROGEN	+/- 1.2%	Sep 21, 2025
PRM	PRM	D913660	15.01 PPM NITROGEN DIOXIDE/AIR	+/- 1.5%	Feb 16, 2023
GMIS	124206889	CC322689	4.573 PPM NITROGEN DIOXIDE/NITROGEN	+/- 1.6%	Feb 17, 2026
NTRM	16061005	CC473180	49.02 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.8%	Mar 22, 2028
NTRM	14060154	CC436951	990.9 PPM CARBON MONOXIDE/NITROGEN	+/- 0.6%	Nov 15, 2025

The SRM, NTRM, PRM, or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet iS50 AUP2010249 CO	FTIR	Oct 11, 2023
Nicolet iS50 AUP2010249 NO	FTIR	Oct 11, 2023
Nicolet iS50 AUP2010249 NO2	FTIR	Oct 11, 2023
Nicolet iS50 AUP2010249 SO2	FTIR	Oct 11, 2023

Triad Data Available Upon Request

NOTES:GROSS WEIGHT: 28.4 kg
NET WEIGHT: 4.7 kg

Signature on file
Approved for Release

United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel. 0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

MULTI-POINT GAS TEST REPORT

Test Date : Feb 23,2026


Equipment :	Gas Analyzer (SO_2)	**Model :**	43i
Manufacturer :	Thermo SCIENTIFIC	**Serial Number :**	1200906875

Standard Gas Concentration			**Dilutor Detail**	
Sulphur Dioxide (SO_2)	42.89	PPM	Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH_4)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB01159156			
Expiration Date :	Nov 06,2026			

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.9	0.90	0.89	0.89
Level 3	40.00%	200.0	200.7	0.70	0.35	0.35
Level 4	60.00%	300.0	300.7	0.70	0.23	0.23
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range		500.0 ppb		Average Difference (%)		0.29

:Acceptable Limit ± 5%

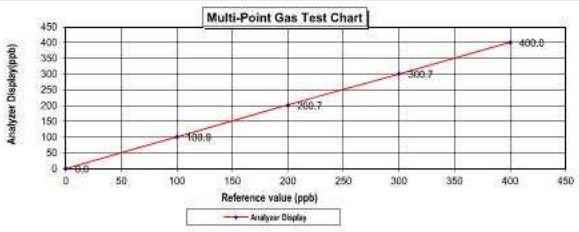

Calculate by ..... 23 / 02 / 2569

Approve by ..... 23 / Feb / 2026

เอกสารไม่ควบคุม

JIRANATEE ASSOCIATES CO.,LTD.
Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Wuttisara, Bangkokyai,
Bangkok 10600(Thailand)
Tel: +6693680812
Mobile: +66865999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Flow measurement laboratory
Calibration services department.

ilac-MRA THAILAND NSC – TISI – TIS 17025 CALIBRATION 0367

CERTIFICATE OF CALIBRATION

Certificate No. : COF-046-68

MEASUREMENT ITEM	: Top Load Orifice
MANUFACTURER	: TISCH
MODEL/TYPE	: TE-5025A
SERIAL NUMBER	: 3541
ID NUMBER	: UAE.EFM.177/2561
CONDITION AS-RECEIVED	: Used item
CUSTOMER	: United Analyst and Engineering Consultant Co., Ltd. 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
RECEIVED DATE	: 20 Oct 2025
MEASUREMENT DATE	: 30 Oct 2025
ISSUE DATE	: 30 Oct 2025

ENVIRONMENTAL CONDITIONS:
Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa

CALIBRATION CONDITION:
Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are 22.9 °C and 51.5 %RH.

NOTED: *The certificate is valid only to the item calibrated on date and place of calibration.*

TABULATION OF RESULTS:
The table on next page give the measured values.

Calibration procedure:
The Orifice gas flow device was calibrated against Standard Rotary Displacement Meter (Roots Meter) Model GSS/MC/W3-dp. The WI-CL-004 was used as a calibration guideline.

Traceability:
This certificate provides a traceability of the measurement to recognized the national standards, and to realization of the International system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MW-0016-25.

Uncertainty of Measurement:
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Calibrated by:
☐ Mr. Sorawit Thachalad
☑ Miss Jittraporn Lertsomphol

JNAC JIRANATEE ASSOCIATES CO.,LTD.

Approved signatory: .....
Mr. Parinya Booncharoen
Calibration Department Manager

เอกสารไม่ควบคุม

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel. 0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

MULTI-POINT GAS TEST REPORT

Test Date : May 6,2025


Equipment :	Gas Analyzer (SO_2)	**Model :**	43i
Manufacturer :	Thermo SCIENTIFIC	**Serial Number :**	CM22387067

Standard Gas Concentration			**Dilutor Detail**	
Sulphur Dioxide (SO_2)	42.89	PPM	Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH_4)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB0159156			
Expiration Date :	Nov 06,2026			

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.7	0.70	0.70	0.70
Level 3	40.00%	200.0	200.6	0.60	0.30	0.30
Level 4	60.00%	300.0	300.7	0.70	0.23	0.23
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range		500.0 ppb		Average Difference (%)		0.25

:Acceptable Limit ± 5%

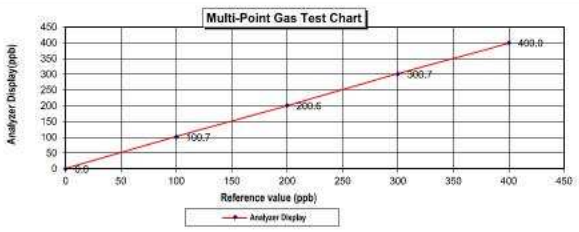

Calculate by ..... 6 / 05 / 2025

Approve by ..... 6 / May / 2025

เอกสารไม่ควบคุม

JNAC JIRANATEE ASSOCIATES CO.,LTD.

Continuation of Certificate of Calibration Number COF-046-68

MEASUREMENT RESULTS:

The Orifice gas flow device was calibrated by direct comparison method with the Standard Rotary Displacement Meter (Roots Meter). The Humid air was used as a medium in the system. The standard conditions are 25°C (298.15 K) and 760 mmHg for standard temperature and standard pressure respectively.

Table 1: The results of Q Standard calibration data

Plate	Flow rate m^3/min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Δp_meter mmHg	Δp_Orifice inH_2O	Y	Standard Flow [Q_s] m^3/min
1	0.707	756.239	22.82	21.98	57.881	1.726	1.315	0.656
2	1.001	756.198	22.79	22.22	61.550	3.424	1.853	0.923
3	1.116	756.152	23.30	22.72	41.184	4.509	2.124	1.057
4	1.169	756.110	23.30	22.77	30.459	5.085	2.256	1.125
5	1.414	756.090	23.37	22.86	29.934	7.544	2.747	1.361

Slope (m): 2.02829
Intercept (b): -0.01895
Correlation coefficient (r): 0.99976
Uncertainty (Δ=2): 0.015 m^3/min

Table 2: The results of Q actual calibration data

Plate	Flow rate m^3/min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Δp_meter mmHg	Δp_Orifice inH_2O	Y	Standard Flow [Q_a] m^3/min
1	0.707	756.239	22.82	21.98	57.881	1.726	0.822	0.654
2	1.001	756.198	22.79	22.22	61.550	3.424	1.158	0.921
3	1.116	756.152	23.30	22.72	41.184	4.509	1.328	1.057
4	1.169	756.110	23.30	22.77	30.459	5.085	1.412	1.124
5	1.414	756.090	23.37	22.86	29.934	7.544	1.720	1.360

Slope (m): 1.27036
Intercept (b): -0.01181
Correlation coefficient (r): 0.99976
Uncertainty (Δ = 2): 0.015 m^3/min

End of Certificate of Calibration

JNAC JIRANATEE ASSOCIATES CO.,LTD.

เอกสารไม่ควบคุม

Jiranatee Associates Co., Ltd.

JIRANATEE ASSOCIATES CO.,LTD.
Jiranatee Associates Co.,Ltd.
63/14-15, 67/35-36
Petchkasem 7, 7/1, Rd Wattharra, Bangkokyai,
Bangkok 10600(Thailand)
Tel. +6602608012
Mobile. +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Flow measurement laboratory
Calibration services department

NSC – TISI – TIS 17025
CALIBRATION 0367

CERTIFICATE OF CALIBRATION

Certificate No. : COF-040-68

MEASUREMENT ITEM	: Top Load Orifice
MANUFACTURER	: TISCH
MODEL/TYPE	: TE-5025A
SERIAL NUMBER	: 3383
ID NUMBER	: UAE.EFM.063/2560
CONDITION AS-RECEIVED	: Used item
CUSTOMER	: United Analyst and Engineering Consultant Co., Ltd. 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
RECEIVED DATE	: 29 Aug 2025
MEASUREMENT DATE	: 29 Sep 2025
ISSUE DATE	: 30 Sep 2025

ENVIRONMENTAL CONDITIONS:
Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa

CALIBRATION CONDITION:
Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are 23.2 °C and 55.9 %RH.

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:
The table on next page give the measured values.

Calibration procedure:
The Orifice gas flow device was calibrated against Standard Rotary Displacement Meter (Roots Meter) Model G65/MC/W2-dp. The WI-CL-004 was used as a calibration guideline.

Traceability:
This certificate provides a traceability of the measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MM-0016-25.

Uncertainty of Measurement:
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Calibrated by:
☐ Mr. Sorawit Thachaled
☒ Miss Ittraporn Letsomphol

Approved signatory: .....
Mr. Parinya Boonchanten
Calibration Department Manager

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION IN PART HAS BEEN GRANTED IN WRITING FROM THE LABORATORY

เอกสารไม่ควบคุม

United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel. 0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

MULTI-POINT GAS TEST REPORT


Test Date : Feb 20,2026

Equipment :	Gas Analyzer (NO_2)	**Model :**	42i
Manufacturer :	Thermo Scientific	**Serial Number :**	CM19050148

Standard Gas Concentration			**Dilutor Detail**	
Sulphur Dioxide (SO_2)	42.89 PPM		Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	46.77 PPM		Model :	146i
Methane (CH_4)	- PPM		Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB0159156			
Expiration Date :	Nov 6,2026			

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.6	0.60	0.60	0.60
Level 3	40.00%	200.0	200.7	0.70	0.35	0.35
Level 4	60.00%	300.0	300.9	0.90	0.30	0.30
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range		500.0 ppb		Average Difference (%)		0.25
:Acceptable Limit ± 5%						

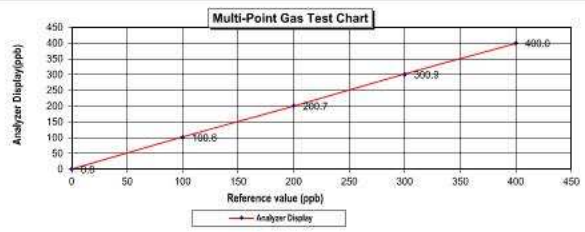

Calculate by
20 / 02 / 2569

Approve by
20 / Feb / 2026

เอกสารไม่ควบคุม

MEASUREMENT RESULTS:

The Orifice gas flow device was calibrated by direct comparison method with the Standard Rotary Displacement Meter (Roots Meter). The Humid air was used as a medium in the system. The standard conditions are 25°C (298.15 K) and 760 mmHg for standard temperature and standard pressure respectively.

Table 1: The results of Q Standard calibration data

Plate	Flow rate m^3/min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Δp_meter mmHg	Δp_Orifice inH$_2$O	Y	Standard Flow [Q_{std}] m^3/min
1	0.704	753.311	22.97	22.08	56.514	1.512	1.229	0.692
2	1.001	753.266	22.99	22.37	62.412	3.014	1.734	0.918
3	1.116	753.254	23.08	22.48	41.501	3.969	1.990	1.054
4	1.164	753.258	23.09	22.55	29.909	4.424	2.101	1.117
5	1.410	753.191	23.04	22.66	28.108	6.537	2.554	1.356

Slope (m): 1.87959
Intercept (b): 0.00567
Correlation coefficient (r): 0.99982
Uncertainty (k=2): 0.015 m^3/min

Table 2: The results of Q actual calibration data

Plate	Flow rate m^3/min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Δp_meter mmHg	Δp_Orifice inH$_2$O	Y	Standard Flow [Q_{std}] m^3/min
1	0.704	753.311	22.97	22.08	56.514	1.512	0.771	0.653
2	1.001	753.266	22.99	22.37	62.412	3.014	1.088	0.920
3	1.116	753.254	23.08	22.48	41.501	3.969	1.249	1.056
4	1.164	753.258	23.09	22.55	29.909	4.424	1.319	1.120
5	1.410	753.191	23.04	22.66	28.108	6.537	1.601	1.359

Slope (m): 1.17728
Intercept (b): 0.00356
Correlation coefficient (r): 0.99982
Uncertainty (k = 2): 0.015 m^3/min

End of Certificate of Calibration

เอกสารไม่ควบคุม

United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel. 0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

MULTI-POINT GAS TEST REPORT


Test Date : May 7,2025

Equipment :	Gas Analyzer (NO_2)	**Model :**	42i
Manufacturer :	Thermo Scientific	**Serial Number :**	1182920009

Standard Gas Concentration			**Dilutor Detail**	
Sulphur Dioxide (SO_2)	42.89 PPM		Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	46.77 PPM		Model :	146i
Methane (CH_4)	- PPM		Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB0159156			
Expiration Date :	Nov 6,2026			

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.6	0.60	0.60	0.60
Level 3	40.00%	200.0	200.7	0.70	0.35	0.35
Level 4	60.00%	300.0	300.7	0.70	0.23	0.23
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range		500.0 ppb		Average Difference (%)		0.24
:Acceptable Limit ± 5%						

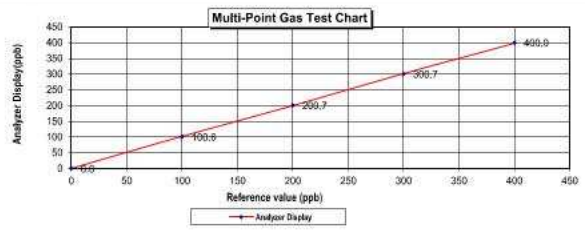

Calculate by
7 / 05 / 2025

Approve by
7 / May / 2025

เอกสารไม่ควบคุม

Airgas
an Air Liquide company

Airgas Specialty Gases
Airgas USA LLC
6141 Easton Road
Plumsteadville, PA 18949
Airgas.com

CERTIFICATE OF ANALYSIS

Grade of Product: EPA PROTOCOL STANDARD

Customer:	AIR LIQUIDE (THAILAND) LTD--		
Part Number:	E05NI91E15A0014	Reference Number:	160-402772205-1
Cylinder Number:	EB0162121	Cylinder Volume:	144.0 CF
Laboratory:	124 - Plumsteadville - PA	Cylinder Pressure:	2016 PSIG
PGVP Number:	A12023	Valve Outlet:	660
Gas Code:	CO,CO2,NO,NOX,SO2,BALN	Certification Date:	Jul 06, 2023

Expiration Date: Jul 06, 2031

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results relate only to the items tested. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS

Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	100.0 PPM	100.4 PPM	G1	+/- 0.9% NIST Traceable	06/27/2023, 07/06/2023
NITRIC OXIDE	100.0 PPM	100.2 PPM	G1	+/- 0.9% NIST Traceable	06/27/2023, 07/06/2023
SULFUR DIOXIDE	100.0 PPM	100.0 PPM	G1	+/- 1.4% NIST Traceable	06/27/2023, 07/06/2023
CARBON MONOXIDE	200.0 PPM	199.2 PPM	G1	+/- 0.3% NIST Traceable	06/26/2023
CARBON DIOXIDE	8.000 %	7.982 %	G1	+/- 1.2% NIST Traceable	06/27/2023
NITROGEN	Balance				

CALIBRATION STANDARDS

Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
GMIS	104202308	CC754364	98.36 PPM NITRIC OXIDE/NITROGEN	+/- 0.4%	Jan 04, 2031
PRM	C2219101	APE1514048	100.19 PPM NITRIC OXIDE/NITROGEN	+/- 0.3%	Feb 28, 2025
GMIS	2023042525	CC754381	98.52 PPM NITRIC OXIDE/NITROGEN	+/-0.4%	Apr 25, 2031
PRM	12409	D913660	15.01 PPM NITROGEN DIOXIDE/AIR	+/- 1.5%	Feb 17, 2023
GMIS	153400202002	EB0130037	9.693 PPM NITROGEN DIOXIDE/NITROGEN	+/- 1.5%	Sep 29, 2025
NTRM	160102-22	KAL003820	97.68 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.8%	Nov 01, 2027
CO	230601	CC745902	249.47 PPM CARBON MONOXIDE/NITROGEN	+/- 0.3%	Dec 09, 2028
NTRM	130606-02	CC411730	13.359 % CARBON DIOXIDE/NITROGEN	+/- 0.6%	May 14, 2025

The SRM, NTRM, PRM, or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet IS50 FTIR AUP2010245 CO2	FTIR	Jun 15, 2023
SIEMENS ULTRAMAT6E N1-C8-180	NDIR	Jun 14, 2023
Nicolet IS50 FTIR AUP2010245 NO	FTIR	Jun 29, 2023
Nicolet IS50 FTIR AUP2010245 NO2	FTIR	Jun 15, 2023
Nicolet IS50 FTIR AUP2010245 SO2	FTIR	Jun 08, 2023

Approved for Release

เอกสารไม่ควบคุม

Airgas
an Air Liquide company

Airgas Specialty Gases
Airgas USA LLC
6141 Easton Road
Plumsteadville, PA 18949
Airgas.com

CERTIFICATE OF ANALYSIS

Grade of Product: EPA PROTOCOL STANDARD

Customer: AIR LIQUIDE (THAILAND) LTD--
Part Number: E05NI91E15A0014
Cylinder Number: EB0162121
Laboratory: 124 - Plumsteadville - PA
PGVP Number: A12023
Gas Code: CO,CO2,NO,NOX,SO2,BALN
Reference Number: 160-402772205-1
Cylinder Volume: 144.0 CF
Cylinder Pressure: 2016 PSIG
Valve Outlet: 660
Certification Date: Jul 06, 2023

Expiration Date: Jul 06, 2031

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results relate only to the items tested. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS

Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	100.0 PPM	100.4 PPM	G1	+/- 0.9% NIST Traceable	06/27/2023, 07/06/2023
NITRIC OXIDE	100.0 PPM	100.2 PPM	G1	+/- 0.9% NIST Traceable	06/27/2023, 07/06/2023
SULFUR DIOXIDE	100.0 PPM	100.0 PPM	G1	+/- 1.4% NIST Traceable	06/27/2023, 07/06/2023
CARBON MONOXIDE	200.0 PPM	199.2 PPM	G1	+/- 0.3% NIST Traceable	06/26/2023
CARBON DIOXIDE	8.000 %	7.982 %	G1	+/- 1.2% NIST Traceable	06/27/2023
NITROGEN	Balance				

CALIBRATION STANDARDS

Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
GMIS	104202308	CC754364	98.36 PPM NITRIC OXIDE/NITROGEN	+/- 0.4%	Jan 04, 2031
PRM	C2219101	APE1514048	100.19 PPM NITRIC OXIDE/NITROGEN	+/- 0.3%	Feb 28, 2025
GMIS	2023042525	CC754381	98.52 PPM NITRIC OXIDE/NITROGEN	+/-0.4%	Apr 25, 2031
PRM	12409	D913660	15.01 PPM NITROGEN DIOXIDE/AIR	+/- 1.5%	Feb 17, 2023
GMIS	153400202002	EB0130037	9.693 PPM NITROGEN DIOXIDE/NITROGEN	+/- 1.5%	Sep 29, 2025
NTRM	160102-22	KAL003820	97.68 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.8%	Nov 01, 2027
CO	230601	CC745902	249.47 PPM CARBON MONOXIDE/NITROGEN	+/- 0.3%	Dec 09, 2028
NTRM	130606-02	CC411730	13.359 % CARBON DIOXIDE/NITROGEN	+/- 0.6%	May 14, 2025

The SRM, NTRM, PRM, or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet IS50 FTIR AUP2010245 CO2	FTIR	Jun 15, 2023
SIEMENS ULTRAMAT6E N1-C8-180	NDIR	Jun 14, 2023
Nicolet IS50 FTIR AUP2010245 NO	FTIR	Jun 29, 2023
Nicolet IS50 FTIR AUP2010245 NO2	FTIR	Jun 15, 2023
Nicolet IS50 FTIR AUP2010245 SO2	FTIR	Jun 08, 2023

Approved for Release

Page 1 of 1

เอกสารไม่ควบคุม

UAE
UNITED ANALYST AND ENGINEERING CONSULTANT COMPANY LIMITED

United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel. 0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

MULTI-POINT GAS TEST REPORT


Test Date : May 7,2025

Equipment :	Gas Analyzer (NO_2)	**Model :**	42i
Manufacturer :	Thermo Scientific	**Serial Number :**	1182920009

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO_2)	42.89 PPM		Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	46.77 PPM		Model :	146i
Methane (CH_4)	- PPM		Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB0159156			
Expiration Date :	Nov 6,2026			

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.6	0.60	0.60	0.60
Level 3	40.00%	200.0	200.7	0.70	0.35	0.35
Level 4	60.00%	300.0	300.7	0.70	0.23	0.23
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range :Acceptable Limit ± 5%		500.0 ppb		Average Difference (%)		0.24

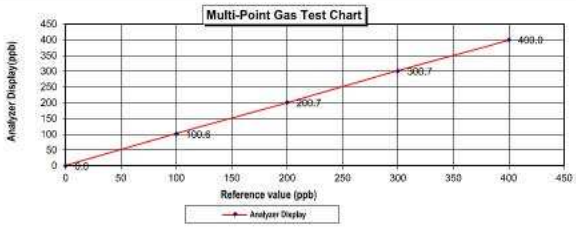

Calculate by
7 / 05 / 2025

Approve by
7 / May / 2025

เอกสารไม่ควบคุม

UAE
UNITED ANALYST AND ENGINEERING CONSULTANT COMPANY LIMITED

United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel. 0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

MULTI-POINT GAS TEST REPORT


Test Date : July 17,2025

Equipment :	Gas Analyzer (CO)	**Model :**	48i
Manufacturer :	Thermo Scientific	**Serial Number :**	1201497733

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO_2)	42.89 PPM		Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	46.77 PPM		Model :	146i
Methane (CH_4)	- PPM		Serial Number :	1180540071
Carbon Monoxide (CO)	965.9 PPM			
Cylinder No. :	EB0159156			
Expiration Date :	Nov 06,2026			

Multi-point gas test data

Reference Value (ppm)			Analyzer Display (ppm)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.0	0.0	0.0	0.0
Level 2	20.00%	10.0	10.7	0.7	6.5	6.5
Level 3	40.00%	20.0	20.8	0.8	3.8	3.8
Level 4	60.00%	30.0	30.9	0.9	2.9	2.9
Level 5	80.00%	40.0	40.0	0.0	0.0	0.0
Remark : Measuring Range :Acceptable Limit ± 5%		50.0 ppm		Average Difference (%)		2.66

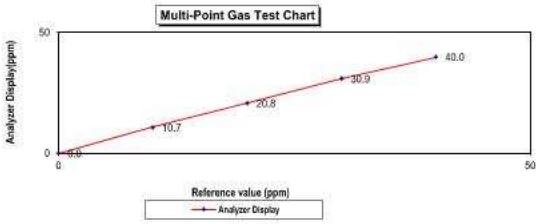

Calculate by
17 / 07 / 2568

Approve by
17 / July / 2025

เอกสารไม่ควบคุม

United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel. 0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

MULTI-POINT GAS TEST REPORT

Test Date : July 29,2025


Equipment :	Gas Analyzer (CO)	**Model :**	48i
Manufacturer :	Thermo SCIENTIFIC	**Serial Number :**	1201778118

Standard Gas Concentration			**Dilutor Detail**	
Sulphur Dioxide (SO_2)	42.89	PPM	Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH_4)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9	PPM		
Cylinder No. :	EB01159156			
Expiration Date :	Nov 06,2026			

Multi-point gas test data

Reference Value (ppm)			Analyzer Display (ppm)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.0	0.0	0.0	0.0
Level 2	20.00%	10.0	10.8	0.8	7.4	7.4
Level 3	40.00%	20.0	20.5	0.5	2.4	2.4
Level 4	60.00%	30.0	30.9	0.9	2.9	2.9
Level 5	80.00%	40.0	40.0	0.0	0.0	0.0
Remark : Measuring Range		50.0 ppm		Average Difference (%)		2.55

:Acceptable Limit ± 5%

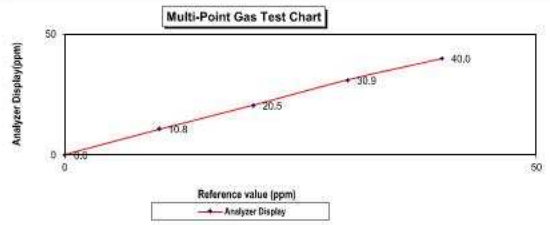

Calculate by ..... 29 / 07 / 2568

Approve by ..... 29 / July / 2025

เอกสารไม่ควบคุม

THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 7 May, 2026 Certification No. 263/26

Object : Wind speed and wind direction

Manufacturer : LSI Lastem ID No. : UAE.EFM.121/2563

Type : Data Logger E-LOG 305 wind speed and wind direction DNA 821

Serial No. : Data Logger 20040004 wind speed and wind direction 20040163

Customer : United Analyst and Engineering Consultant Co.,Ltd.
81 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Prakanong, Bangkok 10260.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1008.2 hPa

NATIONAL STANDARD WIND TUNNEL :
: Micromanometer Theodor Friedrichs FC014 Serial No. 9310119
: HOOK GAGE NO 1425 Pitot Tube Theodor Friedrichs Type 0800.0000 serial 9023
N.I.S.T. Test Reference Number 731/241460 : Standard Velocity at 20 - 30 m/sec
: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)
Serial Number 110730029 (sensor 120629586)
JAPAN QUALITY ASSURANCE ORGANIZATION : Standard Velocity at 0 - 20 m/sec

Calibrated by : Signed :
Mr. Watcharapol Subwat
Mechanical Engineer
Mr. Pisood Promsut
Authorised Signatory
for the Chief
Sub-Standard Instruments

เอกสารไม่ควบคุม

Airgas
an Air Liquide company

Airgas Specialty Gases
Airgas USA LLC
6141 Easton Road
Plumsteadville, PA 18949
Airgas.com

CERTIFICATE OF ANALYSIS

Grade of Product: EPA PROTOCOL STANDARD

Customer:	AIR LIQUIDE (THAILAND) LTD--		
Part Number:	E05NI91E15A0014	Reference Number:	160-402772205-1
Cylinder Number:	EB0162121	Cylinder Volume:	144.0 CF
Laboratory:	124 - Plumsteadville - PA	Cylinder Pressure:	2016 PSIG
PGVP Number:	A12023	Valve Outlet:	660
Gas Code:	CO,CO2,NO,NOX,SO2,BALN	Certification Date:	Jul 06, 2023
	Expiration Date: Jul 06, 2031		

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted. The results relate only to the items tested. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS

Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	100.0 PPM	100.4 PPM	G1	+/- 0.9% NIST Traceable	06/27/2023, 07/06/2023
NITRIC OXIDE	100.0 PPM	100.2 PPM	G1	+/- 0.9% NIST Traceable	06/27/2023, 07/06/2023
SULFUR DIOXIDE	100.0 PPM	100.0 PPM	G1	+/- 1.4% NIST Traceable	06/27/2023, 07/06/2023
CARBON MONOXIDE	200.0 PPM	199.2 PPM	G1	+/- 0.3% NIST Traceable	06/26/2023
CARBON DIOXIDE	8.000 %	7.982 %	G1	+/- 1.2% NIST Traceable	06/27/2023
NITROGEN	Balance				

CALIBRATION STANDARDS

Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
GMIS	104202308	CC754364	98.36 PPM NITRIC OXIDE/NITROGEN	+/- 0.4%	Jan 04, 2031
PRM	C2219101	APE1514048	100.19 PPM NITRIC OXIDE/NITROGEN	+/- 0.3%	Feb 28, 2025
GMIS	2023042525	CC754381	98.52 PPM NITRIC OXIDE/NITROGEN	+/-0.4%	Apr 25, 2031
PRM	12409	D913660	15.01 PPM NITROGEN DIOXIDE/AIR	+/- 1.5%	Feb 17, 2023
GMIS	153400202002	EB0130037	9.693 PPM NITROGEN DIOXIDE/NITROGEN	+/- 1.5%	Sep 29, 2025
NTRM	160102-22	KAL003820	97.68 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.8%	Nov 01, 2027
CO	230801	CC745902	249.47 PPM CARBON MONOXIDE/NITROGEN	+/- 0.3%	Dec 09, 2028
NTRM	130606-02	CC411730	13.359 % CARBON DIOXIDE/NITROGEN	+/- 0.6%	May 14, 2025

The SRM, NTRM, PRM, or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet IS50 FTIR AUP2010245 CO2	FTIR	Jun 15, 2023
SIEMENS ULTRAMAT6E N1-C8-180	NDIR	Jun 14, 2023
Nicolet IS50 FTIR AUP2010245 NO	FTIR	Jun 29, 2023
Nicolet IS50 FTIR AUP2010245 NO2	FTIR	Jun 15, 2023
Nicolet IS50 FTIR AUP2010245 SO2	FTIR	Jun 08, 2023

Approved for Release

เอกสารไม่ควบคุม

THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration

Certification No. 263/26

7 May, 2026

Standard	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
Ultrasonic Anemometer	Pressure	Vacumm	Velocity	Velocity	Correction
m/sec	inches H20	inches H20	m/sec	m/sec	m/sec
1.00	-	-	-	1.0	0.00
3.02	-	-	-	3.0	0.02
5.00	-	-	-	5.0	0.00
7.04	-	-	-	7.0	0.04
9.02	-	-	-	9.0	0.02
11.01	-	-	-	11.0	0.01
13.01	-	-	-	13.0	0.01
15.01	-	-	-	15.1	-0.09
17.02	-	-	-	17.0	0.02
20.02	-	-	-	20.1	-0.08

Vane Angel Bench Stand Model 18112
Young Meteorological Instruments

WIND DIRECTION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	270

Calibrated by :
Mr. Watcharapol Subwat
Mechanical Engineer
Calibration & Test Section
Meteorological Instruments Bureau

เอกสารไม่ควบคุม

THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 7 May, 2026 Certification No. 267/26

Object : Wind speed and wind direction

Manufacturer : LSI Lastem ID No. : UAE.EFM.137/2563

Type : Data Logger E-LOG 305 wind speed and wind direction DNA 821

Serial No. : Data Logger 20080021 wind speed and wind direction 20040197

Customer : United Analyst and Engineering Consultant Co.,Ltd.
81 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Prakanong, Bangkok 10260.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1006.9 hPa

NATIONAL STANDARD WIND TUNNEL :
: Micromanometer Theodor Friedrichs FC014 Serial No. 9310119
: HOOK GAGE NO 1425 Pitot Tube Theodor Friedrichs Type 0800.0000 serial 9023
N.I.S.T. Test Reference Number 731/241460 : Standard Velocity at 20 - 30 m/sec
: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)
Serial Number 110730029 (sensor 120629586)
JAPAN QUALITY ASSURANCE ORGANIZATION : Standard Velocity at 0 - 20 m/sec

Calibrated by : Watcharapol Subwat
Mr. Watcharapol Subwat
Mechanical Engineer

Signed : Pisood Promsut
Mr. Pisood Promsut

(Authorised Signatory)
for the Chief
Sub-Standard Instrument

เอกสารไม่ควบคุม

THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 11 May, 2026 Certification No. 274/26

Object : Wind speed and wind direction

Manufacturer : LSI Lastem ID No. : UAE.EFM.138/2563

Type : Data Logger E-LOG 305 wind speed and wind direction DNA 821

Serial No. : Data Logger 20080022 wind speed and wind direction 20050136

Customer : United Analyst and Engineering Consultant Co.,Ltd.
81 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Prakanong, Bangkok 10260.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1008.1 hPa

NATIONAL STANDARD WIND TUNNEL :
: Micromanometer Theodor Friedrichs FC014 Serial No. 9310119
: HOOK GAGE NO 1425 Pitot Tube Theodor Friedrichs Type 0800.0000 serial 9023
N.I.S.T. Test Reference Number 731/241460 : Standard Velocity at 20 - 30 m/sec
: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)
Serial Number 110730029 (sensor 120629586)
JAPAN QUALITY ASSURANCE ORGANIZATION : Standard Velocity at 0 - 20 m/sec

Calibrated by : Watcharapol Subwat
Mr. Watcharapol Subwat
Mechanical Engineer

Signed : Pisood Promsut
Mr. Pisood Promsut

(Authorised Signatory)
for the Chief
Sub-Standard Instrument

เอกสารไม่ควบคุม

THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration

Certification No. 267/26

7 May, 2026

Standard	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
Ultrasonic Anemometer	Pressure	Vacumm	Velocity	Velocity	Correction
m/sec	inches H2O	inches H2O	m/sec	m/sec	m/sec
1.00	-	-	-	1.0	0.00
3.02	-	-	-	3.0	0.02
5.00	-	-	-	5.0	0.00
7.04	-	-	-	7.0	0.04
9.02	-	-	-	9.0	0.02
11.01	-	-	-	11.0	0.01
13.01	-	-	-	13.0	0.01
15.01	-	-	-	15.0	0.01
17.02	-	-	-	17.0	0.02
20.02	-	-	-	20.0	0.02

Vane Angel Bench Stand Model 18112 Young Meteorological Instruments	
WIND DIRECTION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	270

Calibrated by : Watcharapol Subwat
Mr. Watcharapol Subwat
Mechanical Engineer

Calibration & Test Section
Meteorological Instruments Bureau

เอกสารไม่ควบคุม

THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration

Certification No. 274/26

11 May, 2026

Standard	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
Ultrasonic Anemometer	Pressure	Vacumm	Velocity	Velocity	Correction
m/sec	inches H2O	inches H2O	m/sec	m/sec	m/sec
1.00	-	-	-	1.0	0.00
3.02	-	-	-	3.0	0.02
5.00	-	-	-	5.0	0.00
7.04	-	-	-	7.0	0.04
9.02	-	-	-	9.0	0.02
11.01	-	-	-	11.0	0.01
13.01	-	-	-	13.0	0.01
15.01	-	-	-	15.0	0.01
17.02	-	-	-	17.0	0.02
20.02	-	-	-	20.0	0.02

Vane Angel Bench Stand Model 18112 Young Meteorological Instruments	
WIND DIRECTION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	270

Calibrated by : Watcharapol Subwat
Mr. Watcharapol Subwat
Mechanical Engineer

Calibration & Test Section
Meteorological Instruments Bureau

เอกสารไม่ควบคุม

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7 139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL : 0660-2116-5860-1 FAX: 0660-2116-7140

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD

Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

Certificate No : 24-ACT-091

Request No : Req-2024-1380

Unit Under Calibration Details

Measurement item : Acoustic Calibrator
Manufacturer : SVANTEK
Model : SV 36
Serial Number : 107224
ID : UAE.EFM.171/2564

Class : 1
Range : 94 , 114 dB / 1000 Hz
Instrument Status : Used

Calibration Environment and Details

Temperature : 23 +2 °C)
Humidity : 50 ± 20 %RH)
Barometric Pressure : 1013 +10.0 hPa)
Received Date : 24 June 2024
Calibration Date : 26 June 2024
Location of Calibration : LAB 1 Acoustic
Calibration Procedure : In-house method CP-ACT-02 based on IEC 60942:2017 Electroacoustics - Sound calibrators

Reference Standard	Model	Serial Number	Traceable	Due Calibration
Sound Calibrator	SV 35A	58079	EEI	12 June 2025
THD Multimeter	2015	1047765	NIMT	16 January 2025

Traceability : This certificate providoes traceability of measurement to recognized national standard, and to the realization of the international System of Units (SI).

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k =2, providing a level of confidence approximately 95 %.

Calibrated By :
Mr. Noppadon Luangart
Service Calibration Engineer

Approved By :
Mr. Pacit Mathavorn
Calibration Engineer Supervisor

Issue Date : 26 June 2024

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the laboratory.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7 139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL : 0660-2116-5860-1 FAX: 0660-2116-7140

Certificate No : 24-ACT-091

Request No : Req-2024-1380

Decision Rule for Statements of Conformity


The standard decision rule employed for the statements of conformity to each calibration result will be applied using JLAC-G8:09/2019 Guidelines on the Reporting of Compliance with Specification as following Fig. and statements:

Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass[1] = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail[2] = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

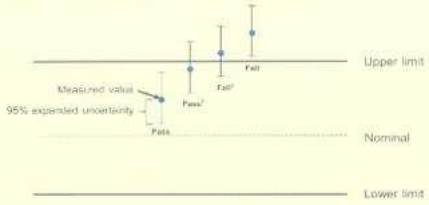

End of Calibration

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the laboratory.

FM-708-ACT-02 Rev.03 Issue date 5/6/24

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7 139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL : 0660-2116-5860-1 FAX: 0660-2116-7140

Certificate No : 24-ACT-091

Request No : Req-2024-1380

Sound pressure level — **Calibration Results :** Without Adjustment

Calibration Range (dB)	Without Adjustment (dB)		Adjustment (dB)		Uncertainty (± dB)	Acceptance limit Class 1 (± dB)	Result
	Measured	Deviated value	Measured	Deviated value			
94 dB / 1000 Hz	94.02	0.02	-	-	0.14	0.25	Pass
114 dB / 1000 Hz	114.05	0.05	-	-	0.13	0.25	Pass

Frequency of Sound pressure level

Calibration Range (Hz)	Without Adjustment		Adjustment		Uncertainty (± %)	Acceptance limit Class 1 (± %)	Result
	Measured (Hz)	Deviated	Measured (Hz)	Deviated			
94 dB / 1000 Hz	1000.00	0.00	-	-	0.01	0.70	Pass
114 dB / 1000 Hz	1000.00	0.00	-	-	0.01	0.70	Pass

Total Harmonic Distortion plus Noise of Sound pressure level (THD+N %)

Calibration Range (Hz)	Without Adjustment Measured (%)	Adjustment Measured (%)	Uncertainty (± %)	Acceptance limit Class 1 (± %)	Result
94 dB / 1000 Hz	0.24	-	0.40	2.5	Pass
114 dB / 1000 Hz	0.44	-	0.40	2.5	Pass

Note :

Function	Maximum-permitted Uncertainty of measurement
Sound pressure level	0.15 dB
Frequency	0.20%
Total distortion+noise	0.50%

- Acceptance limit was IEC60942:2017 Class 1
- The calibration results exclude the calibrator pressure correction
- The calibration results exclude the microphone volume correction

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the laboratory.

FM-708-ACT-02 Rev.03 Issue date 5/6/24

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7 139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL : 0660-2116-5860-1 FAX: 0660-2116-7140

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

Certificate No : 26-SLM-159
Request No : Req-2026-0832

Unit Under Calibration Details

Measurement item : Sound Level Meter
Manufacturer : LARSON DAVIS
Model : LxT1
Serial Number : 0007309
ID : UAE.EFM.041/2566
Resolution : 0.1 dB

Microphone Class : 1
Microphone Model : 377B02
Microphone S/N : 345239
Preamplifier Model : PRMLxT1
Preamplifier S/N : 077644
Instrument Status : Used

Calibration Environment and Details

Temperature : 23 °C ± 2 °C
Humidity : 50 %RH ± 20 %RH
Barometric Pressure : 1013 hPa ± 10 hPa
Received Date : 25 March 2026
Calibrated Date : 22 April 2026
Calibration Procedure : In-house method CP-SLM-01 based on IEC 61672-3 : 2013 Electroacoustics - Sound level meters - Part 3: Periodic tests
Location of Calibration : Lab Acoustic

Reference Standard

Instrument	Brand	Model	SN.	Due calibration	Traceability
Standard Microphone	Bruel&Kjaer	4226	3412381	7 May 2026	NIMT
Audio Generator	Svantek	Svan401	131	27 September 2026	WK Electric

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k = 2, providing a level of confidence approximately 95 %.

Calibrated By :
Mr. Noppadon Luangart
Service Calibration Engineer

Approved By :
Mr. Pacit Mathavorn
Calibration Engineer Supervisor

Issue Date : 22 April 2026

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the laboratory.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7 139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 06606-2116-5860-1 FAX: 06606-2116-7140

Certificate No : 26-SLM-159
Request No : Req-2026-0832

1. Indication at the calibration check frequency

UUC Setting	Nominal	Before Adjust		After Adjust		UNCERTAINTY
FAST / A / 37-139	Level	UUC	ERR	UUC	ERR	
Calibrator Setting	(dB)	(dB)	(dB)	(dB)	(dB)	(± dB)
1000 Hz 114 dB	113.75	114.5	0.75	113.7	-0.05	0.20

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, SN. 58079

2. Self-generated noise, Microphone installed

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139		
UUC Weighting	(dB)	(± dB)
A	30.8	0.10

3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139		
UUC Weighting	(dB)	(± dB)
A	28.6	0.10
C	28.8	0.10
Z	33.2	0.10

4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting	Deviation from various Frequency Weighting Respone curve			UNCERTAINTY
FAST / 37-139	A	C	Z	
STD Setting	(dB)	(dB)	(dB)	(± dB)
125 Hz	0.0	0.1	0.0	0.60
1000 Hz	0.0	0.0	0.0	0.60
4000 Hz	0.6	0.6	0.6	0.60
8000 Hz	0.7	0.7	0.7	0.70

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the laboratory. This certificate shall not be used to claim product certification, approval, or endorsement by NVLAP, NIST, or any agency of the U.S. Government.
FM-708-SLM-01 Rev.4 Issue date 17/2/25
เอกสารไม่ควบคุม

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7 139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 06606-2116-5860-1 FAX: 06606-2116-7140

Certificate No : 26-SLM-159
Request No : Req-2026-0832

7. Long Term Stability

UUC Setting	Measured	UNCERTAINTY
FAST / A / 37-139	UUC	
STD Setting	(dB)	(± dB)
Initial	114.0	
Final	114.0	
Deviated	0.0	0.10

8. Level linearity on the reference level range

UUC Setting	Anticipated	Deviation		UNCERTAINTY
FAST / A / 37-139	REF	UUC	ERR	
STD dB	(dB)	(dB)	(dB)	(± dB)
139.00	139	139.0	0.0	
134.00	134	134.0	0.0	
129.00	129	129.0	0.0	
124.00	124	124.0	0.0	
119.00	119	119.0	0.0	
114.00	114	114.0	0.0	
109.00	109	109.0	0.0	
104.00	104	104.0	0.0	
99.00	99	98.9	-0.1	
94.00	94	93.9	-0.1	
89.00	89	88.9	-0.1	
84.00	84	83.9	-0.1	0.30
79.00	79	78.9	-0.1	
74.00	74	73.9	-0.1	
69.00	69	68.9	-0.1	
64.00	64	63.9	-0.1	
59.00	59	58.9	-0.1	
54.00	54	53.9	-0.1	
49.00	49	49.0	0.0	
44.00	44	44.1	0.1	
39.00	39	39.4	0.4	
38.00	38	38.5	0.5	
37.00	37	37.6	0.6	

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the laboratory. This certificate shall not be used to claim product certification, approval, or endorsement by NVLAP, NIST, or any agency of the U.S. Government.
FM-708-SLM-01 Rev.4 Issue date 17/2/25
เอกสารไม่ควบคุม

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7 139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 06606-2116-5860-1 FAX: 06606-2116-7140

Certificate No : 26-SLM-159
Request No : Req-2026-0832

5. Electrical signal test of frequency weightings, Weighting network respone with relative to 1 kHz

UUC Setting	Deviation from various Frequency Weighting Respone curve			UNCERTAINTY
FAST / 37-139				
STD Setting	A (dB)	C (dB)	Z (dB)	(± dB)
63 Hz	-0.2	-0.1	-0.1	
125 Hz	-0.1	0.0	-0.1	
250 Hz	-0.1	0.0	0.0	
500 Hz	-0.1	0.0	-0.1	
1000 Hz	0.0	0.0	-0.1	0.20
2000 Hz	0.0	0.0	0.0	
4000 Hz	0.0	0.0	0.0	
8000 Hz	-0.1	-0.1	0.0	
16000 Hz	-0.1	-0.1	-0.2	

6. Frequency and time weightings at 1kHz

UUC Setting	STD	Measured		UNCERTAINTY
FAST / 37-139	REF	UUC	ERR	
UUC Weighting	(dB)	(dB)	(dB)	(± dB)
A	114.00	114.0	0.0	
C	114.00	114.0	0.0	0.20
Z	114.00	114.0	0.0	

UUC Setting	STD	Measured		UNCERTAINTY
37-139 / A	REF	UUC	ERR	
UUC Time Respone	(dB)	(dB)	(dB)	(± dB)
Fast	114.00	114.0	0.0	
Slow	114.00	114.0	0.0	0.20
Leq	114.00	114.0	0.0	

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the laboratory. This certificate shall not be used to claim product certification, approval, or endorsement by NVLAP, NIST, or any agency of the U.S. Government.
FM-708-SLM-01 Rev.4 Issue date 17/2/25
เอกสารไม่ควบคุม

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7 139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 06606-2116-5860-1 FAX: 06606-2116-7140

Certificate No : 26-SLM-159
Request No : Req-2026-0832

9. Level linearity including the level range control

UUC Setting	STD	Measured		UNCERTAINTY
FAST / A	REF	UUC	ERR	
UUC Range	(dB)	(dB)	(dB)	(± dB)
37-139	42.80	43.0	0.2	0.30
	114	114.0	0.0	

10. Tone burst response

UUC Setting	STD	Anticipated	Measured		UNCERTAINTY
A / 37-139	Toneburst	Ref	UUC	ERR	
UUC Time Respone	(ms)	(dB)	(dB)	(dB)	(± dB)
Fast	200	135.0	135.0	0.0	
	2	118.0	117.7	-0.3	
	0.25	109.0	108.6	-0.4	
Slow	200	128.6	128.5	-0.1	0.20
	2	109.0	108.9	-0.1	
SEL	200	129.0	129.0	0.0	
	2	109.0	109.0	0.0	
	0.25	100.0	99.9	-0.1	

11. Peak C Sound level

UUC Setting	Anticipated	Measured		UNCERTAINTY
FAST / C / 95-142	REF	UUC	ERR	
STD Setting	(dB)	(dB)	(dB)	(± dB)
Complete cycle	137.4	136.8	-0.60	
Positive half cycle	136.4	136.2	-0.20	0.20
Negative half cycle	136.4	136.2	-0.20	

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the laboratory. This certificate shall not be used to claim product certification, approval, or endorsement by NVLAP, NIST, or any agency of the U.S. Government.
FM-708-SLM-01 Rev.4 Issue date 17/2/25
เอกสารไม่ควบคุม

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7 139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL : 06606-2116-5860-1 FAX: 06606-2116-7140

Certificate No : 26-SLM-159
Request No : Req-2026-0832

12. Overload indication

UUC Setting	Measured	UNCERTAINTY
FAST / A / 37-139	UUC	
STD Setting	(dB)	(± dB)
Positive one-half cycle	143.2	
Negative one-half cycle	143.3	
Deviated	-0.1	0.20

13. High Level Stability

UUC Setting	Measured	UNCERTAINTY
FAST / A / 37-139	UUC	
STD Setting	(dB)	(± dB)
Initial	138.0	
Final	138.0	
Deviated	0.0	0.10

End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.
FM-TR-SLM-01 Rev 4 Issue date 17/2/25
เอกสารไม่ควบคุม

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7 139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL : 06606-2116-5860-1 FAX: 06606-2116-7140

Certificate No : 26-SLM-158
Request No : Req-2026-0831

1. Indication at the calibration check frequency

UUC Setting	Nominal	Before Adjust		After Adjust		UNCERTAINTY
FAST / A / 37-139	Level	UUC	ERR	UUC	ERR	
Calibrator Setting	(dB)	(dB)	(dB)	(dB)	(dB)	(± dB)
1000 Hz 114 dB	113.75	113.9	0.15	113.7	-0.05	0.20

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, SN. 58079

2. Self-generated noise, Microphone installed

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139		
UUC Weighting	(dB)	(± dB)
A	28.7	0.10

3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139		
UUC Weighting	(dB)	(± dB)
A	28.3	0.10
C	28.0	0.10
Z	32.4	0.10

4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting	Deviation from various Frequency Weighting Respone curve			UNCERTAINTY
FAST / 37-139	A	C	Z	
STD Setting	(dB)	(dB)	(dB)	(± dB)
125 Hz	0.1	0.2	0.1	0.60
1000 Hz	0.0	0.0	0.0	0.60
4000 Hz	0.2	0.3	0.3	0.60
8000 Hz	0.3	0.4	0.4	0.70

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.
FM-TR-SLM-01 Rev 4 Issue date 17/2/25
เอกสารไม่ควบคุม

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7 139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL : 06606-2116-5860-1 FAX: 06606-2116-7140

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

Certificate No : 26-SLM-158
Request No : Req-2026-0831

Unit Under Calibration Details

Measurement item : Sound Level Meter
Manufacturer : LARSON DAVIS
Model : LxT1
Serial Number : 0007308
ID : UAE.EFM.040/2566
Resolution : 0.1 dB

Microphone Class : 1
Microphone Model : 377B02
Microphone S/N : 345238
Preamplifier Model : PRMLxT1
Preamplifier S/N : 077643
Instrument Status : Used

Calibration Environment and Details

Temperature : 23 °C ± 2 °C
Humidity : 50 %RH ± 20 %RH
Barometric Pressure : 1013 hPa ± 10 hPa
Received Date : 25 March 2026
Calibrated Date : 22 April 2026
Calibration Procedure : In-house method CP-SLM-01 based on IEC 61672-3 : 2013 Electroacoustics - Sound level meters - Part 3: Periodic tests
Location of Calibration : Lab Acoustic

Reference Standard

Instrument	Brand	Model	SN.	Due calibration	Traceability
Standard Microphone	Brueel&Kjaer	4226	3412381	7 May 2026	NIMT
Audio Generator	Svantek	Svan401	131	27 September 2026	WK Electric

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k = 2, providing a level of confidence approximately 95 %.

Calibrated By :
Mr. Noppadon Luangarl
Service Calibration Engineer

Approved By :
Mr. Pacit Mathavorn
Calibration Engineer Supervisor

Issue Date : 22 April 2026

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.
FM-TR-SLM-01 Rev 4 Issue date 17/2/25
เอกสารไม่ควบคุม

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7 139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL : 06606-2116-5860-1 FAX: 06606-2116-7140

Certificate No : 26-SLM-158
Request No : Req-2026-0831

5. Electrical signal test of frequency weightings, Weighting network respone with relative to 1 kHz

UUC Setting	Deviation from various Frequency Weighting Respone curve			UNCERTAINTY
FAST / 37-139				
STD Setting	A (dB)	C (dB)	Z (dB)	(± dB)
63 Hz	-0.2	-0.3	0.0	0.20
125 Hz	-0.1	0.0	0.0	
250 Hz	-0.1	0.0	0.0	
500 Hz	-0.1	0.0	0.0	
1000 Hz	0.0	0.0	0.0	
2000 Hz	0.0	0.0	0.0	
4000 Hz	0.0	0.0	0.0	
8000 Hz	-0.1	-0.3	0.0	
16000 Hz	-0.1	-0.1	-0.1	

6. Frequency and time weightings at 1kHz

UUC Setting	STD	Measured		UNCERTAINTY
FAST / 37-139	REF	UUC	ERR	
UUC Weighting	(dB)	(dB)	(dB)	(± dB)
A	114.00	114.0	0.0	0.20
C	114.00	114.0	0.0	
Z	114.00	114.0	0.0	

UUC Setting	STD	Measured		UNCERTAINTY
37-139 / A	REF	UUC	ERR	
UUC Time Respone	(dB)	(dB)	(dB)	(± dB)
Fast	114.00	114.0	0.0	0.20
Slow	114.00	114.0	0.0	
Leq	114.00	114.0	0.0	

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.
FM-TR-SLM-01 Rev 4 Issue date 17/2/25
เอกสารไม่ควบคุม

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7 139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 06680-2116-5860-1 FAX: 06680-2116-7140

Certificate No : 26-SLM-158
Request No : Req-2026-0831

7. Long Term Stability

UUC Setting	Measured	UNCERTAINTY
FAST / A / 37-139	UUC	
STD Setting	(dB)	(± dB)
Initial	114.0	
Final	114.0	
Deviated	0.0	0.10

8. Level linearity on the reference level range

UUC Setting	Anticipated	Deviation		UNCERTAINTY
FAST / A / 37-139	REF	UUC	ERR	
STD dB	(dB)	(dB)	(dB)	(± dB)
139.00	139	139.0	0.0	
134.00	134	134.0	0.0	
129.00	129	129.0	0.0	
124.00	124	124.0	0.0	
119.00	119	119.0	0.0	
114.00	114	114.0	0.0	
109.00	109	109.0	0.0	
104.00	104	104.0	0.0	
99.00	99	98.9	-0.1	
94.00	94	94.0	0.0	
89.00	89	89.0	0.0	
84.00	84	84.0	0.0	0.30
79.00	79	79.0	0.0	
74.00	74	74.0	0.0	
69.00	69	69.0	0.0	
64.00	64	64.0	0.0	
59.00	59	59.0	0.0	
54.00	54	54.0	0.0	
49.00	49	49.0	0.0	
44.00	44	44.1	0.1	
39.00	39	39.4	0.4	
38.00	38	38.5	0.5	
37.00	37	37.6	0.6	

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.
FM-708-SLM-01 Rev.4 Issue date 17/2/25
เอกสารไม่ควบคุม

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7 139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 06680-2116-5860-1 FAX: 06680-2116-7140

Certificate No : 26-SLM-158
Request No : Req-2026-0831

9. Level linearity including the level range control

UUC Setting	STD	Measured		UNCERTAINTY
FAST / A	REF	UUC	ERR	
UUC Range	(dB)	(dB)	(dB)	(± dB)
37-139	42.40	42.5	0.1	0.30
	114	114.0	0.0	

10. Tone burst response

UUC Setting	STD	Anticipated	Measured		UNCERTAINTY
A / 37-139	Toneburst	Ref	UUC	ERR	
UUC Time Respone	(ms)	(dB)	(dB)	(dB)	(± dB)
Fast	200	135.0	135.0	0.0	0.20
	2	118.0	117.7	-0.3	
	0.25	109.0	108.7	-0.3	
Slow	200	128.6	128.5	-0.1	
	2	109.0	108.9	-0.1	
SEL	200	129.0	129.1	+0.1	
	2	109.0	109.0	0.0	
	0.25	100.0	99.9	-0.1	

11. Peak C Sound level

UUC Setting	Anticipated	Measured		UNCERTAINTY
FAST / C / 95-142	REF	UUC	ERR	
STD Setting	(dB)	(dB)	(dB)	(± dB)
Complete cycle	137.4	136.7	-0.70	0.20
Positive half cycle	136.4	136.1	-0.30	
Negative half cycle	136.4	136.1	-0.30	

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.
FM-708-SLM-01 Rev.4 Issue date 17/2/25
เอกสารไม่ควบคุม

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7 139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 06680-2116-5860-1 FAX: 06680-2116-7140

Certificate No : 26-SLM-158
Request No : Req-2026-0831

12. Overload indication

UUC Setting	Measured	UNCERTAINTY
FAST / A / 37-139	UUC	
STD Setting	(dB)	(± dB)
Positive one-half cycle	142.6	
Negative one-half cycle	142.7	
Deviated	-0.1	0.20

13. High Level Stability

UUC Setting	Measured	UNCERTAINTY
FAST / A / 37-139	UUC	
STD Setting	(dB)	(± dB)
Initial	138.0	
Final	138.0	
Deviated	0.0	0.10

End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.
FM-708-SLM-01 Rev.4 Issue date 17/2/25
เอกสารไม่ควบคุม

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7 139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 06680-2116-5860-1 FAX: 06680-2116-7140

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

Certificate No : 26-AFM-105
Request No : Req-2026-1035

Unit Under Calibration Details

Measurement Item : Air Flow Meter
Manufacturer : TSI
Model : 4146
Serial Number : 41461214007
ID : UAE.EMA2.093/2555
Location of Calibration : LAB 4 AIR VELOCITY METER

Sensor Model : -
Sensor Serial Number : -
Instrument Status : Used

Calibration Environment and Details

Temperature : 23 °C ± 3 °C
Humidity : 55 %RH ± 20 %RH
Barometric Pressure : 1013 hPa ± 10 hPa
Received Date : 20 April 2026
Calibration Date : 3 June 2026
Calibration Procedure : In-house method CP-AFM-01 by Comparison technique with Standard Primary Flow Calibrator

Reference Standard	Model	Serial Number	Traceble	Due Calibration
Air Flow Meter	Gilibrator 3 Low flow	18501010006	Sensidyne	7 May 2027
Air Flow Meter	Gilibrator 3 Standard flow	19031011002	Sensidyne	7 May 2027
Temperature meter	GT 11	12000077	Qreborn	10 October 2026
Pressure meter	CPG2400	41900KDU651882	TPA	17 October 2026

Traceability :
This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01 and MIT NSC-TISI-TIS Accreditation No. 0052

Note :
The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k = 2$, providing a level of confidence approximately 95 %.

Calibration By : Mr. Noppadon Luangsart
Service Calibration Engineer

Approved By : Mr. Jedsada Thongyoi
Lab Manager

Issue Date : 3 June 2026

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.
FM-708-AFM-01 Rev.06 issue date 23/2/25
เอกสารไม่ควบคุม

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (6610-2116-5860-1 FAX: (6610-2116-7140

Certificate No : 26-AFM-105

Request No : Req-2026-1035

Result of Calibration : Without Adjustment

STD Reading			UUC Reading			Error	Uncertainty		
Temperature (°C)	Pressure (kPa)	Flow (l/min)	Temperature (°C)	Pressure (kPa)	Flow (l/min)	(l/min)	(l/min)	(°C)	(kPa)
24.4	100.52	0.020	-	-	0.020	0.000	0.0016	1.0	0.50
24.4	100.48	0.050	-	-	0.050	0.000	0.0040	1.0	0.50
24.4	100.50	0.099	-	-	0.101	0.002	0.0036	1.0	0.50
24.2	100.49	0.197	-	-	0.202	0.005	0.0072	1.0	0.50
24.2	100.49	0.498	-	-	0.503	0.005	0.0095	1.0	0.50
24.2	100.49	0.995	-	-	1.009	0.014	0.019	1.0	0.50
24.3	100.47	1.682	-	-	1.708	0.026	0.032	1.0	0.50
24.4	100.46	1.975	-	-	2.004	0.029	0.038	1.0	0.50
24.5	100.37	2.951	-	-	3.004	0.053	0.057	1.0	0.50
24.7	100.28	3.939	-	-	4.006	0.067	0.076	1.0	0.50
24.9	100.15	4.929	-	-	5.011	0.082	0.095	1.0	0.50

Note STD : Standard UUC : Unit Under Calibration

- UUC Reference Condition : 21.1 °C, 101.3 kPa, Air
- Flow Rate was corrected for non-standard operating condition by using equation :

$$Qmeas = Qref \times \frac{Pref}{Pmeas} \times \frac{Tmeas}{Tref}$$

where Q = Flow Rate P = Absolute Pressure T = Absolute Temperature
meas = Measurement Condition ref = Standard Condition

* Indicates non accredited

End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Cert. No.: 25H1370

Page.: 2 of 2

Result of Calibration:- Without Adjustment

Function: Humidity Measurement.

Reference Temperature (°C)	Standard Humidity (%R.H.)	UUC* Reading (%R.H.)	Correction (%R.H.)	Uncertainty of Measurement (±%R.H.)
25.0	40.1	40	0.1	1.3
25.0	50.1	48	2.1	1.6
25.0	60.0	57	3.0	1.6
25.0	70.2	68	2.2	1.6

Result of Calibration:- Without Adjustment

Function: Temperature Measurement.

Standard Temperature (°C)	UUC* Reading (°C)	Correction (°C)	Uncertainty of Measurement (±°C)
19.953	20.1	-0.147	0.42
25.001	25.1	-0.099	0.42
30.043	30.1	-0.057	0.42
40.023	40.0	0.023	0.42

UUC* : Unit Under Calibration

The reported uncertainty of measurement was base on standard uncertainty multiplied by coverage factor k = 2.00, providing confidence level approximately 95%.

-o0o-

เอกสารไม่ควบคุม

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484

NSC-TISI-TIS17025 CALIBRATION 0008

Certificate of Calibration

Certificate No. : 25H1370
Page : 1 of 2

Equipment : Digital Thermo-Hygrometer
Manufacturer: Digicon
Model : TH-02A
Serial No.: 435031146
ID No.: UAE.EFM.004/2567
Condition As-Received: Used Item
Received Date: 04 July 2025
Calibration Date: 08 July 2025 to 15 July 2025
Reference: 2507-0215WSC
Ambient Temperature: (25 ± 3) °C
Relative Humidity: (50 ± 20) %

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

Submitted by: United Analyst and Engineering Consultant Co.,Ltd.
81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Procedure used: Calibration were conducted using in-house calibration procedure CP-H03 according to comparison with standard chilled mirror sensor for humidity measurement function and comparison with standard temperature probe for temperature measurement function into humidity / temperature chamber.

Condition of this result of calibration

1.Reference standards instruments

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Dew Point Hygrometer	Optidew 401	164756	TH-0005-25	05 Feb 2026
2) Handheld Thermometer With Sensor	1523	5717096	24I1241	18 Nov 2025

2.The certificate is valid only to the item calibrated on date and place of calibration.

3.This measurement result is traceable to the International System of Unit maintained through:-
-National Institute of Metrology (Thailand), NSC-ONSC Accredited No. Calibration 0144
-Technology Promotion Association (Thailand-Japan), NSC-ONSC Accredited No. Calibration 0008

Calibrated by : Somchai Dumwor
Issue Date : 21 July 2025

Approved Signatory :
[ ] Chakrit Waewwanjua
[ ] Pornthippa Tameyakul
[✓] Viporn Tantiyawutti

เอกสารไม่ควบคุม

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: (6610-2116-5860-1 FAX: (6610-2116-7140

NSC-TISI-TIS17025 CALIBRATION0298

Certificate of Calibration

Customer
Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

Certificate No : 25-TPM-345
Request No : Req-2025-1688
Page : 1/2

Unit Under Calibration Details

Calibration Parameter	: Temperature		
Instrument Name	: Thermal Environment Monitor	Range Calibration	: 20°C to 60°C
Manufacturer	: Quest Technologies	Type of Sensor	: RTD
Model	: QT-34	Sensor Diameter (mm)	: 4.5
Serial Number	: TEB060015	Calibration Position (mm)	: 67.5
Resolution	: 0.1 °C	Instrument Status	: Used
ID Number	: UAE.EMA2.057/2552		

Calibration Environment and Details

Temperature : 23 °C ± 3 °C
Humidity : 55 %RH ± 15 %RH
Received Date : 21 July 2025
Calibrated Date : 24 July 2025
Calibration Procedure : In-house method CP-TPM-01 by Comparison with Standard Thermometer.

Reference Standard : Digital Thermometer with Sensor, Manufacturer: GINGO/GINGO, Model: GT11/ RTD100, SN: 12000077, ID: AR-TPM Which was calibrated on 15 October 2024, Calibration Certificate No. : QR24-2836

Traceability : This Certificate is traceable to SI Unit through Quality Reborn Co., Ltd., NSC-ONSC Accreditation No.: Calibration 0292

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor *k* =2, providing a level of confidence approximately 95 %.

Approved By :
Mr. Noppadon Luangart
Technical Manager

Issue Date : 24 July 2025

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7 139 MOO 13, SOI SUN TINAKORN 11 TAMBON BANG KAEO
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 16609-2106-5960 FAX: 16609-2106-7140

innovative instrument

NSC-T101-TIS17025
CALIBRATION0298

Calibration Note

UUC Adjustment : Not Adjust

Certificate No : 25-TPM-345
Request No : Req-2025-1688
Page : 2/2

Result of Calibration :

UUC Sensor	Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (±°C)
WET	20.003	20.1	- 0.1	0.14
	25.003	25.1	- 0.1	0.14
	30.003	30.1	- 0.1	0.14
	35.004	35.1	- 0.1	0.14
	40.002	40.1	- 0.1	0.14
	45.002	45.0	0.0	0.14
	50.003	50.0	0.0	0.14
	60.002	60.0	0.0	0.14
DRY	20.003	20.0	0.0	0.14
	25.004	25.0	0.0	0.14
	30.003	30.0	0.0	0.14
	35.002	35.0	0.0	0.14
	40.003	39.9	+ 0.1	0.14
	45.002	44.9	+ 0.1	0.14
	50.003	49.9	+ 0.1	0.14
	60.003	59.9	+ 0.1	0.14
GLOBE	20.003	20.0	0.0	0.14
	25.002	25.0	0.0	0.14
	30.002	30.0	0.0	0.14
	35.003	35.0	0.0	0.14
	40.003	40.0	0.0	0.14
	45.005	44.9	+ 0.1	0.14
	50.003	49.9	+ 0.1	0.14
	60.004	59.9	+ 0.1	0.14

End of Certificate

Calibrated By :

Mr. Sittichok Jirapakdeesakul

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the

FM-706-TPM-01 Rev.01 Issue date 13/02/20

เอกสารไม่ควบคุม

United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel. 0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

MULTI-POINT GAS TEST REPORT

Test Date : Feb 23,2026


Equipment :	Gas Analyzer (SO_2)	**Model :**	43i
Manufacturer :	Thermo SCIENTIFIC	**Serial Number :**	CM22387063

Standard Gas Concentration			**Dilutor Detail**	
Sulphur Dioxide (SO_2)	42.89 PPM		Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	46.77 PPM		Model :	146i
Methane (CH_4)	- PPM		Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB0159156			
Expiration Date :	Nov 06,2026			

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.7	0.70	0.70	0.70
Level 3	40.00%	200.0	200.9	0.90	0.45	0.45
Level 4	60.00%	300.0	300.9	0.90	0.30	0.30
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range 500.0 ppb				Average Difference (%)		0.29

:Acceptable Limit ± 5%

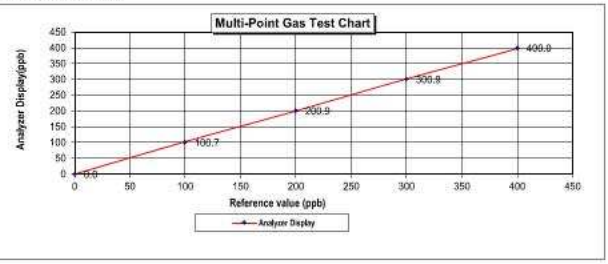

Calculate by 23 / 02 / 2569

Approve by 23 / Feb / 2026

เอกสารไม่ควบคุม

United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel. 0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

MULTI-POINT GAS TEST REPORT

Test Date : Feb 12,2026


Equipment :	Gas Analyzer (SO_2)	**Model :**	43i
Manufacturer :	Thermo SCIENTIFIC	**Serial Number :**	CM22387061

Standard Gas Concentration			**Dilutor Detail**	
Sulphur Dioxide (SO_2)	42.89 PPM		Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	46.77 PPM		Model :	146i
Methane (CH_4)	- PPM		Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB01159156			
Expiration Date :	Nov 06,2026			

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.5	0.50	0.50	0.50
Level 3	40.00%	200.0	200.9	0.90	0.45	0.45
Level 4	60.00%	300.0	300.6	0.60	0.20	0.20
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range 500.0 ppb				Average Difference (%)		0.23

:Acceptable Limit ± 5%

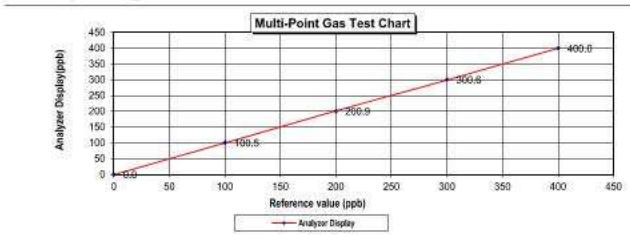

Calculate by 12 / 02 / 2069

Approve by 12 / Feb / 2026

เอกสารไม่ควบคุม

United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel. 0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

MULTI-POINT GAS TEST REPORT

Test Date : Feb 12,2026


Equipment :	Gas Analyzer (SO_2)	**Model :**	43i
Manufacturer :	Thermo SCIENTIFIC	**Serial Number :**	CM22387065

Standard Gas Concentration			**Dilutor Detail**	
Sulphur Dioxide (SO_2)	42.89 PPM		Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	46.77 PPM		Model :	146i
Methane (CH_4)	- PPM		Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB01159156			
Expiration Date :	Nov 06,2026			

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.4	0.40	0.40	0.40
Level 3	40.00%	200.0	200.8	0.80	0.40	0.40
Level 4	60.00%	300.0	300.7	0.70	0.23	0.23
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range 500.0 ppb				Average Difference (%)		0.21

:Acceptable Limit ± 5%

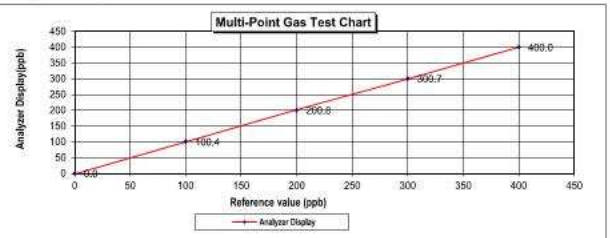

Calculate by 12 / 02 / 2569

Approve by 12 / Feb / 2026

เอกสารไม่ควบคุม

United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel. 0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

MULTI-POINT GAS TEST REPORT


Test Date : Mar 3,2026

Equipment :	Gas Analyzer (SO_2)	**Model :**	43i
Manufacturer :	Thermo SCIENTIFIC	**Serial Number :**	CM22387067

Standard Gas Concentration			**Dilutor Detail**	
Sulphur Dioxide (SO_2)	42.89	PPM	Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	46.77	PPM	Model :	146i
Methane (CH_4)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	965.9			
Cylinder No. :	EB0159156			
Expiration Date :	Nov 06,2026			

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.7	0.70	0.70	0.70
Level 3	40.00%	200.0	200.5	0.50	0.25	0.25
Level 4	60.00%	300.0	300.8	0.80	0.27	0.27
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range 500.0 ppb :Acceptable Limit ± 5%				Average Difference (%)		0.24

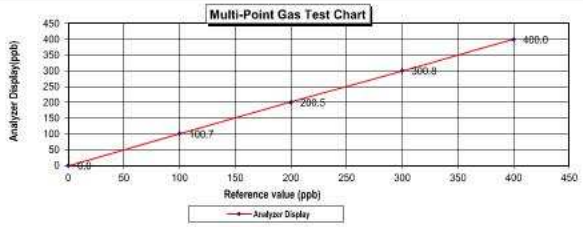

Calculate by ..... 3 / 03 / 2569

Approve by ..... 3 / Mar / 2026

เอกสารไม่ควบคุม

THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration

Certification No. 236/26

22 April, 2026

Standard	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
Ultrasonic Anemometer	Pressure	Vacumm	Velocity	Velocity	Correction
m/sec	inches H2O	inches H2O	m/sec	m/sec	m/sec
1.00	-	-	-	1.0	0.00
3.02	-	-	-	3.0	0.02
5.00	-	-	-	5.0	0.00
7.04	-	-	-	7.0	0.04
9.02	-	-	-	9.0	0.02
11.01	-	-	-	11.0	0.01
13.01	-	-	-	13.0	0.01
15.01	-	-	-	15.0	0.01
17.02	-	-	-	17.0	0.02
20.02	-	-	-	20.0	0.02

Vane Angel Bench Stand Model 18112 Young Meteorological Instruments	
WIND DIRECTION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	270

Calibrated by : Watcharapol

Mr. Watcharapol Subwat
Mechanical Engineer

Calibration & Test Section
Meteorological Instruments Bureau

เอกสารไม่ควบคุม

THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 22 April, 2026 Certification No. 236/26

Object : Wind speed and wind direction

Manufacturer : LSI Lastem ID No. : UAE.EFM.133/2563

Type : Data Logger E-LOG 305 wind speed and wind direction DNA 821

Serial No. : Data Logger 20040062 wind speed and wind direction 20040185

Customer : United Analyst and Engineering Consultant Co.,Ltd.
81 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Prakanong, Bangkok 10260.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1011.3 hPa

NATIONAL STANDARD WIND TUNNEL :
: Micromanometer Theodor Friedrichs FC014 Serial No. 9310119
: HOOK GAGE NO 1425 Pitot Tube Theodor Friedrichs Type 0800.0000 serial 9023
N.I.S.T. Test Reference Number 731/241460 : Standard Velocity at 20 - 30 m/sec
: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)
Serial Number 110730029 (sensor 120629586)
JAPAN QUALITY ASSURANCE ORGANIZATION : Standard Velocity at 0 - 20 m/sec

Calibrated by : Watcharapol Signed :

Mr. Watcharapol Subwat Mr. Pisood Promsut
Mechanical Engineer

(Authorised Signatory)
for the Chief
Sub-Standard Instrument

เอกสาร ไม่ควบคุม

THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 11 May, 2026 Certification No. 271/26

Object : Wind speed and wind direction

Manufacturer : LSI Lastem ID No. : UAE.EFM.132/2563

Type : Data Logger E-LOG 305 wind speed and wind direction DNA 821

Serial No. : Data Logger 20040061 wind speed and wind direction 20040184

Customer : United Analyst and Engineering Consultant Co.,Ltd.
81 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Prakanong, Bangkok 10260.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1008.9 hPa

NATIONAL STANDARD WIND TUNNEL :
: Micromanometer Theodor Friedrichs FC014 Serial No. 9310119
: HOOK GAGE NO 1425 Pitot Tube Theodor Friedrichs Type 0800.0000 serial 9023
N.I.S.T. Test Reference Number 731/241460 : Standard Velocity at 20 - 30 m/sec
: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)
Serial Number 110730029 (sensor 120629586)
JAPAN QUALITY ASSURANCE ORGANIZATION : Standard Velocity at 0 - 20 m/sec

Calibrated by : Watcharapol Signed :

Mr. Watcharapol Subwat Mr. Pisood Promsut
Mechanical Engineer

(Authorised Signatory)
for the Chief
Sub-Standard Instrument

เอกสาร ไม่ควบคุม

THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration

Certification No. 271/26

11 May, 2026

Standard	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
Ultrasonic Anemometer	Pressure	Vacumm	Velocity	Velocity	Correction
m/sec	inches H2O	inches H2O	m/sec	m/sec	m/sec
1.00	-	-	-	1.0	0.00
3.02	-	-	-	2.9	0.12
5.00	-	-	-	5.0	0.00
7.04	-	-	-	6.9	0.14
9.02	-	-	-	9.0	0.02
11.01	-	-	-	11.0	0.01
13.01	-	-	-	13.0	0.01
15.01	-	-	-	15.0	0.01
17.02	-	-	-	17.0	0.02
20.02	-	-	-	20.0	0.02

Vane Angel Bench Stand Model 18112 Young Meteorological Instruments	
WIND DIRECTION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	270

Calibrated by :

Mr. Watcharapol Subwat

Mechanical Engineer

Calibration & Test Section

Meteorological Instruments Bureau

เอกสารไม่ควบคุม

United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel.0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

Certificate of Calibration

Certificate No.: 250422-1-BL002-25
Code No.: BL002-25

Customer Name:	United Analyst and Engineering Consultant Co., Ltd.
Address:	3 Soi Udom suk 41, Sukhumvit Rd., Bang Chak, Phar Khanong, Bangkok 10260
Equipment:	Electronic Balance
Manufacturer:	Mettler Toledo
Model:	AB204-S/FACT
Serial No.:	1129361010
Asset No. :	UAE.WAS.002/2552
Building : N/A	Floor : 1 Room : 107
Received Date:	April 22, 2025
Date of Calibation :	April 23, 2025
Calibration Conditions:	Temperature 22.8 °C to 23.4 °C
	Humidity 54.8 % to 68.9 %
	Pressure 756.6 mmHg to 758.2 mmHg
Calibrated by:	Sakkarin Srirahang
Approved by:	Suwit Chotnok Signature:
Issued Date:	April 25, 2025

Note : 1) The Uncertainties are for a confidence probability of approximately 95%
2) This Certificate is valid only to the item calibrated on date and place of calibration.
3) This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the United Analyst and Engineering Consultant Co.,Ltd. (UAE)

เอกสารไม่ควบคุม

United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel.0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

Certificate No.: 250422-1-BL002-25
Code No.: BL002-25

Equipment:	Electronic Balance	Manufacturer:	Mettler Toledo
Model:	AB204-S/FACT	Readability:	0.0001 g
Serial No.:	1129361010	ID No.:	UAE.WAS.002/2552
Max. Capacity:	220 g		
Calibration Date:	April 23, 2025		

Calibraton Result: (Continued)
Calibraton Range: 0 - 200 g
Calibraton Adjustment: Internal Calibration

3. Error of Indication from nominal or conventional mass value:

Nominal Value (g)	Reference Value (g)	Indication (g)	Correction (g)	Uncertainty (± mg)	Coverage Factor k
Unload	0.0000000	0.0000	0.0000	0.10	2.05
0.01	0.0100025	0.0099	0.0001	0.10	2.05
0.05	0.0500056	0.0500	0.0000	0.10	2.05
0.1	0.1000012	0.0999	0.0001	0.10	2.05
0.5	0.5000133	0.5000	0.0000	0.10	2.05
1	1.0000105	1.0000	0.0000	0.10	2.05
10	10.000010	10.0000	0.0000	0.11	2.04
40	40.000076	40.0000	0.0000	0.14	2.00
50	50.000056	50.0000	0.0001	0.13	2.00
80	80.000107	80.0000	0.0001	0.18	2.00
100	100.000109	99.9999	0.0002	0.17	2.00
120	120.00015	119.9999	0.0003	0.21	2.00
150	150.000165	149.9998	0.0003	0.24	2.00
160	160.000175	159.9997	0.0005	0.26	2.00
200	200.000129	199.9998	0.0004	0.30	2.00

4. Effect of Tare test:

Tare Load (g)	Test Load (g)	Indication (g)	Correction (g)
100	20.000041	19.9999	0.0001
	40.000076	39.9998	0.0002
	60.000066	59.9997	0.0003
	80.000107	79.9999	0.0002
	100.000168	100.0004	-0.0003

Remark:
The report uncertainty of measurment was based on standard uncertainty multiplied by coverage factor k, providing a level of confidence approximately 95%

o---o-End-o---o

เอกสารไม่ควบคุม

United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel.0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

Certificate No.: 250422-1-BL002-25
Code No.: BL002-25

Equipment:	Electronic Balance	Manufacturer:	Mettler Toledo
Model:	AB204-S/FACT	Readability:	0.0001 g
Serial No.:	1129361010	ID No.:	UAE.WAS.002/2552
Max. Capacity:	220 g		
Calibration Date:	April 23, 2025		
Condition As-Received:	In Condition		

Condition of Equipment:
Condition of This Result of Calibration:
1. Calibration Method: This instrument was calibrated by method UAE.CP.CAL.006 In-House Method based on UKAS Lab 14 : 2022
2. Reference Standrads:


Reference Standard:	Model	Serial No.	Calibrated By	Certificate No.	Traceability	Due Date
Standard Weight Class E2 (OIML)	1 mg to 1 kg	B749109122	AMARC	25-009359	Mettler-Toledo	21-Jan-27
Standard Weight Class F1 (OIML)	1 mg to 200 g	11119512	AMARC	24-013840	Mettler-Toledo	04-Feb-26
Instrument	**Model**	**Serial No.**	**Calibrated By**	**Certificate No.**	**Traceability**	**Due Date**
Thermo-Hygro-Baro Meter	MHB-382SD	AK.46457	SUCCESS	SG-H-00997/67	Success Gateway	21-Nov-25
Thermo-Hygro-Baro Meter	MHB-382SD	AK.46457	TPA	25PT95	TPA	25-Feb-26

3. This certification is traceable to SI Unit
4. This certification was certified only for the indtrument we calibrated
5. This result of calibration wae found accurate as show on date and place of calibration only.
6. Through the reference standard laboratory of AMARC 25-009359 Calibration 0152

Calibraton Result:
1. Repeatability of Reading:

Nominal Value (g)	Standard Deviation of Reading (g)
200*	0.000045

2. Eccentric or off-center loading
A mass of 100 g was placed and moved to various position on pan
The Balance reading obtained is given in the table.

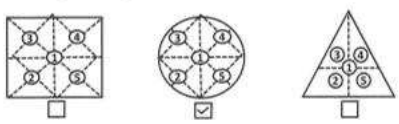

1 (g)	2 (g)	3 (g)	4 (g)	5 (g)	Maximum Difference (g)
100.0000	99.9996	99.9997	100.0003	100.0005	0.0005

เอกสารไม่ควบคุม

United Analyst and Engineering Consultant Co., Ltd. (UAE)
Certified Laboratory (ISO/IEC 17025)

List of Instrument Certificates for Environmental Quality Analysis

No.	Instruments/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*
1	Atomic Absorption Spectrometer	CADMIUM CHROMIUM TRIVALENT COPPER IRON LEAD MANGANESE NICKEL ZINC	Agilent Technologies	AA240FS / MY13160003	Agilent Technologies (Thailand) Co.,Ltd.	Preventive Maintenance Checklist	26/1/2026	25/1/2027
2	Atomic Absorption Spectrometer	ARSENIC SELENIUM	Perkin Elmer	PinAAcle 900F / P8520031902	Perkin Elmer Co.,Ltd.	Preventive Maintenance Report	27/10/2025	26/10/2026
3	Analytical Balance	FAT OIL AND GREASE	Mettler Toledo	AB204-S/FACT / 1129361010	United Analyst and Engineering Consultant Co., Ltd.	250422-1 BL002-25	23/4/2025	22/4/2026
4	Analytical Balance	TOTAL DISSOLVED SOLIDS TOTAL SOLIDS	Mettler Toledo	XSR205DU / C21048B394	National Food Institute,Ministry of Industry, Thailand	2602226-002-01	20/3/2025	19/3/2026
5	Analytical Balance	TOTAL SUSPENDED SOLIDS	Mettler Toledo	XSR205DU / C09071872	National Food Institute,Ministry of Industry, Thailand	2602226-001-01	20/3/2025	19/3/2026
6	Continuous Flow Analyzer(CFA)	CYANIDE AS HCN	Skalar Analytical B.V., the Netherlands	San++SK00-02 / 182688	EKSH (Thailand) Ltd.	WO-00070079	23/5/2025	22/5/2026
7	DO Meter	BIOCHEMICAL OXYGEN DEMAND	YSI	5100 / 11B 101863	Technology Promotion Association (Thailand-Japan)	26TM50	2/3/2026	1/3/2027

สถาบันอาหาร
ศูนย์บริการวิชาการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

NSC-TIS-ITA 17025
CALIBRATION 0081

Calibration Certificate

Certificate No.: 2502226-002-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road, Bangchack, Prakhanong, Bangkok 10260

Equipment:	Electronic Balance
Manufacturer:	METTLER TOLEDO
Model:	XSR205DU
Serial No.:	C210685394
ID No.:	UAE.WAO.010/2565
Order No.:	2502226
Operation No.:	2502226-002
Date of Receipt:	19 March 2025
Date of Calibration:	20 March 2025

Calibrated by Mr.Yothin Charoensuk, Scientist
Approved by (Mr.Pheraphat Tuanjit), Manager, Division of Calibration Laboratory
Date of Issue: 25 March 2025 — Responsible for the Technical Management Team

The uncertainties are for a confidence probability of approximately 95%

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-003 Revision: 01 Date: 20-04-65

123/456 ซอยอุดมสุข 41 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
โทร +66(0) 2428 8888 โทรสาร +66(0) 2428 8444

ผลการสอบเทียบนี้ออกให้ในนามของ สถาบันอาหาร เท่านั้น

สถาบันอาหาร
ศูนย์บริการวิชาการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

NSC-TIS-ITA 17025
CALIBRATION 0081

Calibration Report

Certificate No.: 2502226-002-01
Equipment: Electronic Balance — **Manufacturer:** METTLER TOLEDO; **Model:** XSR205DU; **Resolution:** 0.00001 g / 0.0001 g; **Serial No.:** C210685394; **ID No.:** UAE.WAO.010/2565; **Capacity:** 82 g / 220 g

Date of Calibration: 20 March 2025
Environment Condition: Ambient Temperature: 21.2 ± 0.6 °C Relative Humidity: 48 ± 3.5 %
Place of Calibration: 208 Balance Room, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Condition of Equipment: Good Condition
Condition of This Results of Calibration:
1. Calibration Method: NFI Method W-MA-001 In-House Method based on UKAS Lab 14 : 2019
2. Reference Standards:

Reference Standard	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Standard Weight Class E2	1mg to 200g	8595567572	TCS	M24041805	19 April 2025
Instrument	**Model**	**Serial No.**	**Calibrated By**	**Certificate No.**	**Due Date**
Thermo-Hygro Meter	608-H1	NFI.8TH 017/23	Quality Reborn	QR25-0542	10 February 2026


3. This certification is traceable to SI UNIT
4. This certificate was certified only for the instrument we calibrated.
5. This result of calibration was found accurate as shown on date and place of calibration only.

Calibration Results:

1. Repeatability of Reading:

Nominal Value (g)	Standard Deviation of Reading (g)
40	0.0000042
80	0.0000042
100	0.000000
200	0.000000

2. Off-Center Error:
A mass of 100 g was placed and moved to various position on pan.
The balance reading obtained in given in the table.



1 (g)	2 (g)	3 (g)	4 (g)	5 (g)	6 (g)	(Maximum Difference) (g)
100.0001	100.0001	100.0001	100.0001	100.0001	100.0001	0.0000

F-CS-012 Revision: 01 Date: 20-04-65

123/456 ซอยอุดมสุข 41 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
โทร +66(0) 2428 8888 โทรสาร +66(0) 2428 8444

ผลการสอบเทียบนี้ออกให้ในนามของ สถาบันอาหาร เท่านั้น

List of Instrument Certificates for Environmental Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*
8	Gas Chromatography	a-BHC ALDRIN b-BHC d-BHC DIELDRIN ENDOSULFAN I ENDOSULFAN II ENDOSULFAN SULFATE ENDRIN ENDRIN ALDEHYDE g-BHC HEPTACHLOR HEPTACHLOR EPOXIDE METHOXYCHLOR pp-DDD pp-DDE pp-DDT	Agilent Technologies	8890 / US2229A024	Agilent Technologies (Thailand) Co.,Ltd.	Preventive Maintenance Checklist	16/6/2025	15/6/2026
9	Mercury Analyzer	TOTAL MERCURY	NIC, Japan	RA-4500 / 11780278	Coax Group Corporation Ltd.	Preventive Maintenance Report	2/7/2025	1/7/2026
10	Hot Air Oven	TOTAL DISSOLVED SOLIDS TOTAL SOLIDS TOTAL SUSPENDED SOLIDS	Memmert	UF55 / B212.0411	Technology Promotion Association (Thailand-Japan)	25TM579	19/3/2025	18/3/2026
11	Cooled Incubator	TOTAL COLIFORM BACTERIA	Binder	KB400 / WTB20200000015535	National Food Institute, Ministry of Industry, Thailand	2502229-006-01	19/3/2025	18/3/2026
12	Incubator	FECAL COLIFORM BACTERIA	Memmert	IPP260 / V615.0187	National Food Institute, Ministry of Industry, Thailand	2502229-001-01	19/3/2025	18/3/2026
13	Inductively Coupled Plasma- Optical Emission Spectrometer(ICP-OES)	BARIUM TITANIUM	Agilent Technologies, USA	5110 VDV(G8015AA) / MY18030001	Agilent Technologies (Thailand) Co.,Ltd.	Preventive Maintenance Checklist	3/11/2025	2/11/2026

List of Instrument Certificates for Environmental Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*
14	pH Meter	pH	Horiba	LAQUA-PH210 / HA9MG047	technology promotion association (thailand-japan	26CH231	26/2/2026	26/2/2027
15	UV-VIS Spectrophotometer	CHROMIUM HEXAVALENT	Agilent	Cary 60 G6860A / MY1541009	DQE Services Co.,Ltd.	SP25-019	26/5/2025	25/5/2026
16	UV-VIS Spectrophotometer	HYDROGEN SULPHIDE NITRATE NITROGEN PHOSPHATE SULPHATE	Hitachi	U-2900 / 21E22-009	DQE Services Co.,Ltd.	SP25-021	26/5/2025	25/5/2026
17	UV/VIS Spectrophotometer	CHEMICAL OXYGEN DEMAND FORMALDEHYDE PHENOLS	Hitachi High-Tech Science Corporation Tokyo Japan	U-5100 / 23A4-008	DQE Services Co.,Ltd.	SP25-024	17/6/2025	16/6/2026
18	Turbidity Meter (Portable)	TURBIDITY (NTU)	Oakton Instruments(China)	T100IR / 1120501017	Technology Promotion Association (Thailand-Japan)	25CH1053	9/9/2025	7/9/2026
19	Water Bath	FECAL COLIFORM BACTERIA	Memmert	WNE 14 / L416.0612	Technology Promotion Association (Thailand-Japan)	26TM194	2/2/2026	1/2/2027

Due Date of Calibration* : Based on the annual calibration plan. At least 1 time per year.

Calibration Report

Certificate No.: 2502226-002-01

Equipment: Electronic Balance **Manufacturer:** METTLER TOLEDO

Model: XSR205DU **Resolution:** 0.00001 g / 0.0001 g

Serial No.: C210685394 **ID No.:** UAE.WAO.010/2565

Capacity: 82 g / 220 g

Date of Calibration: 20 March 2025 **Page 3 of 4**

Calibration Results: **(Continued)**

Calibration Range: 0-80 g

Calibration Adjustment: Internal Calibration

3. Departure from Nominal Value: (Range: 0 - 82 g ; Resolution: 0.00001 g)

Nominal Value (g)	Standard Value (g)	Average Reading (g)	Correction (g)	Uncertainty (± g)	Coverage Factor k
Unload	0.000000	0.00000	0.00000	0.0000087	2.00
0.001	0.001003	0.00100	0.00000	0.0000090	2.00
0.005	0.005002	0.00501	-0.00001	0.0000092	2.00
0.01	0.010003	0.01002	-0.00002	0.0000089	2.00
0.05	0.049996	0.05001	-0.00001	0.0000096	2.00
0.1	0.100011	0.10002	-0.00001	0.000011	2.00
0.5	0.500016	0.50004	-0.00002	0.000014	2.00
1	1.000003	1.00005	-0.00005	0.000016	2.00
2	2.000023	2.00006	-0.00004	0.000017	2.00
5	5.000015	5.00006	-0.00005	0.000020	2.00
10	10.000009	10.00005	-0.00004	0.000026	2.00
20	20.000033	20.00007	-0.00004	0.000037	2.00
30	30.000039	30.00009	-0.00005	0.000050	2.00
50	50.000028	50.00008	-0.00005	0.000068	2.00
80	80.000067	80.00013	-0.00005	0.00011	2.00

for N. niyomdat

เอกสารไม่ควบคุม
2008 ซอยอินทามระ 36 ถนนอินทามระ แขวงอินทามระ เขตบางซื่อ กรุงเทพมหานคร 10800
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel. +66(0) 2422 8688 Fax +66(0) 2422 8505
nfi.or.th

Agilent CrossLab Start Up Services

Agilent 5100 5110 ICP-OES Preventive Maintenance

Agilent Preventive Maintenance provides factory recommended service for your analytical instruments to assure reliable operation and the accuracy of your results

Delivered by highly trained and certified service engineers using genuine Agilent parts and supplies, Agilent Preventive Maintenance provides what you need to reduce unplanned downtime and keep your systems operating at their peak performance.

This checklist is used as a guide for completing the preventive maintenance tasks. A signed copy of this checklist is provided for your records

Revision: A.02, Issued: 21 January 2022
Document Number: G8014-90075
© Agilent Technologies, Inc. 2022

Agilent

เอกสารไม่ควบคุม

สถาบันอาหาร
กระทรวงอุตสาหกรรม
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

Calibration Report

Certificate No.: 2502226-002-01

Equipment: Electronic Balance **Manufacturer:** METTLER TOLEDO

Model: XSR205DU **Resolution:** 0.00001 g / 0.0001 g

Serial No.: C210685394 **ID No.:** UAE.WAO.010/2565

Capacity: 82 g / 220 g

Date of Calibration: 20 March 2025 **Page 4 of 4**

Calibration Results: **(Continued)**

Calibration Range: >80-200 g

Calibration Adjustment: Internal Calibration

3. Departure from Nominal Value: (Range: >80 - 200 g ; Resolution: 0.0001 g)

Nominal Value (g)	Standard Value (g)	Average Reading (g)	Correction (g)	Uncertainty (± g)	Coverage Factor k
90	90.00010	90.0002	-0.0001	0.00015	2.00
100	100.00006	100.0001	-0.0000	0.00016	2.00
110	110.00007	110.0002	-0.0001	0.00017	2.00
120	120.00009	120.0002	-0.0001	0.00018	2.00
130	130.00010	130.0002	-0.0001	0.00019	2.00
140	140.00013	140.0002	-0.0001	0.00019	2.00
150	150.00009	150.0002	-0.0001	0.00021	2.00
160	160.00010	160.0002	-0.0001	0.00022	2.00
170	170.00012	170.0002	-0.0001	0.00023	2.00
200	200.00013	200.0002	-0.0001	0.00028	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

---------- End ----------

for N. niyomdat

F-CS-012 Revision: 01 Date: 20.04.65
เอกสารไม่ควบคุม
2008 ซอยอินทามระ 36 ถนนอินทามระ แขวงอินทามระ เขตบางซื่อ กรุงเทพมหานคร 10800
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel. +66(0) 2422 8688 Fax +66(0) 2422 8505
nfi.or.th

Introduction

Customer Information

- Customers should provide all necessary operating supplies upon request of the engineer.
- A customer representative should be available to the engineer while performing the preventive maintenance procedures. Customers are responsible for regular maintenance and are encouraged to observe the service representative.
- Any parts not included in the Parts Lists section of this document are not part of the recommended Preventive Maintenance service nor are they included in the price of this service.
- If a system requires the use of extra or special procedures and/or parts for the maintenance service, then these must be ordered separately and charged as a repair, which may incur additional costs.
- For customers using HF applications, the instrument should be returned to its standard sample introduction system.

Revision: A.02, Issued: 21 January 2022
Document Number: G8014-90075
© Agilent Technologies, Inc. 2022

Agilent

เอกสารไม่ควบคุม

Important Customer Web Links

- To access **Agilent University**, visit http://www.agilent.com/crosslab/university/ to learn about training options, which include online, classroom and onsite delivery. A training specialist can work directly with you to help determine your best options.
- To access the **Agilent Resource Center** web page, visit https://www.agilent.com/en-us/agilentresources. The following information topics are available:
  - Sample Prep and Containment
  - Chemical Standards
  - Analysis
  - Service and Support
  - Application Workflows
- The **Agilent Community** is an excellent place to get answers, collaborate with others about applications and Agilent products, and find in-depth documents and videos relevant to Agilent technologies. Visit https://community.agilent.com/welcome
- Videos about specific preparation requirements for your instrument can be found by searching the **Agilent YouTube** channel at https://www.youtube.com/user/agilent
- **Need to place a service call?** Flexible Repair Options | Agilent

เอกสารไม่ควบคุม

Instrument Maintenance

System Information

☐ Check this box if an instrument configuration report is attached instead of completing the table.

Instrument System Name and ID	5110 VDV ICP-OES
Instrument System Site and Location	UAE Consultant

List System Component Product Numbers	List the Serial Numbers of each Component
1. G 8019 A	MY 19030001
2.	
3.	
4.	
5.	
6.	
7.	
8.	
9.	

ICP-OES Configuration Table	Circle the type or write in the type if other
Nebulizer Type	SeaSpray | OneNeb | Conikal | Other
Spray Chamber	Cyclonic Single Pass | Cyclonic Double Pass | Other
Torch	Radial | Dual View | Other
Torch Type	One Piece | Semi Demountable | Fully Demountable | Other
Injector Diameter	2.4mm | 3mm | 1.4mm | 0.8mm | Other
Injector Material	Quartz | Ceramic | Other

เอกสารไม่ควบคุม

Service Engineer's Responsibilities

- Contact the customer and ensure that all necessary supplies are available before the preventive maintenance visit.
- Only select those pages that relate to the system or module being serviced.
- Complete empty fields with the relevant information.
- Complete the relevant checkboxes in the checklist using either a "**X**" or tick mark "✓".
- Check **"Service not applicable"** check boxes to indicate services/tasks not delivered, as appropriate.
- Complete the Preventive Maintenance services in the most logical order relevant to the individual system service in the order of the tasks listed.
- Complete the **Service Review** section together with the customer.
- Complete the fields for page numbers at the foot of each selected page
- Add relevant page numbers to selected pages and complete the total number of pages field in the Service Completion section
- **Ask the customer to sign the Service Verification section including the customer's and your signature.**

เอกสารไม่ควบคุม

Preparation

- ☑ Discuss any specific issues with the customer before starting.
- ☑ Review the instrument logbook for recorded problems and comments.
- ☑ Save instrument control settings before starting the procedure.
- ☑ Perform a general inspection of the system for cleanliness.
- ☑ Check for proper installation of parts, assemblies, sensors etc.
- ☑ Check system for required installation of components and implementation of Service Notes
- ☑ Check for required firmware/software updates and verify with customers if they would like them installed.
- ☐ For HF application systems, if standard sample introduction system was not installed, ask the customer to install it. N/A
- ☑ Ask the customer to remove any samples from the ICP-OES sample introduction area, auto sampler or around the ICP-OES.

เอกสารไม่ควบคุม

Preventive Maintenance Procedures

Record Pre-PM instrument performance

- [x] Run Instrument Performance test.
- [x] Record results in Instrument Performance Test Results Table – Pre-PM.

Clean and inspect ICP-OES system

- [x] Look for any obvious external damage or problems.
- [x] Inspect water cooling hoses, gas lines and power cord for excessive wear or damage.
- [x] Perform a general internal inspection of the system for excessive dust accumulation, clean if necessary.
- [x] Inspect sample introduction components and record any required maintenance in the Service Engineer Comments and notify the customer as the required actions required.
- [x] Record the instrument operating conditions in the ICP-OES Status Results Table.
- [x] Replace the polychromator purge filter.
- [x] Replace the radial pre-optics window.
- [x] Replace the axial pre optics window for SVDV and VDV instruments.
- [x] Check exhaust flow for the correct positive extraction at the exhaust duct to insure they meet minimum specifications.
- [x] Replace air inlet dust filter.
- [ ] Replace high capacity air inlet dust filter element, if installed. N/A
- [x] Remove and clean instrument water inlet filter.

Agilent Water Recirculator

- [ ] **Service not applicable**
- [x] Drain cooling fluid and remove any particles from the chiller reservoir.
- [x] Remove, clean and reinstall water inlet metal mesh filter if present.
- [x] Re fill with Agilent Cool Clear cooling fluid.
- [x] Clean the cooling system Air filter and the condenser.

เอกสารไม่ควบคุม

ICP-OES adjustment

- [x] Check position of Zn peak, adjust if required.
- [x] Check Argon Ratio, adjust to specified value if required.
- [x] Perform Detector Calibration.
- [x] Perform Instrument Calibration.

Record Post-PM instrument performance

- [x] Run Instrument Performance test.
- [x] Record results in Instrument Performance Test Results Table - Post PM.
- [x] For systems using ICP Expert version 7.3 and above, run the following Instrument tests
  - [x] Subsystem Communications Test
  - [x] Air Flow
  - [x] Water Flow
  - [x] Gas Flows
  - [x] RF Generator
  - [x] Camera Test
  - [x] Optics Test
  - [x] Nebulizer Test
- [x] Record the result in the Instrument Test Results Table

เอกสารไม่ควบคุม

SPS 3 Auto Sampler

- [x] **Service not applicable**
- [ ] Power cycle the autosampler and verify successful initialization.
- [ ] Inspect X and Z axis belts for wear. Replace is necessary.
- [ ] Clean X and Z axis slide shafts.
- [ ] Using customer's racks and the Agilent software move the sample probe to the 4 outermost corners and rinse port, ensure that the probe is approximately centered in the vial.

SPS 4 Auto sampler

- [x] **Service not applicable**
- [ ] Clean the spill tray, rack location mat, end frames and chassis with a damp soft cloth and diluted mild detergent.
- [ ] Clean the auto sampler cover panels, if cover kit is installed, with domestic window cleaner.
- [ ] Check the X-axis and Z-axis drive belts for cracks, splits, damaged teeth, excessive fraying, color changes or degradation from fumes.
- [ ] Check the X-axis, Theta-axis and Z-axis FFC cables for cracks, incorrect positioning, damaged edges or damaged connectors.
- [ ] Pump Tubing Replacement. Replace peristaltic pump tubing. Replace all tubing that goes from the rinse station to the pump and from the pump to the waste/rinse bottles
- [ ] Test using customer's tray and move the sample probe to the sample vial 1, wash vial and rinse port and ensure that the probe is centered in the vial. If not use calibration wizard and calibrate the position.

AVS 4, 6, 7 Advanced Valve System

- [x] **Service not applicable**
- [ ] Replace valve rotor seal
- [ ] Check fittings for signs of leaks
- [ ] Check tubing including autosampler tubing for kinks or excessive wear
- [ ] Check high flow pump for signs of leaks

เอกสารไม่ควบคุม

Restore Instrument

- [ ] For HF applications, ask the customer to re install their sample introduction system. N/A
- [x] Leave system in an idle state: on and purging.
- [x] Guidance: If the PM service is performed prior to a qualification service, then use the qualification procedure as a guide for final instrument set up and checkout.

Service Review

- [x] Attach available reports/printouts of all tests to this documentation.
- [x] Record the Preventive Maintenance service activity in the customer's records/logbook.
- [x] Record the PM event in the Smart Alerts logbook, if applicable.
- [x] Update/reset instrument maintenance counters as appropriate.
- [x] Affix the PM sticker to the system or instrument logbook based on the customer's request.
- [x] Complete the Service Engineer Comments section if there are additional comments.
- [x] Review this service, parts replaced, and test results obtained with the customer.
- [x] If the instrument firmware was updated, record the details of the change in the Service Engineer's Comments box. Systems in a compliant environment may need additional documentation.
- [x] **Complete the Signature Page with both Service Engineer and Customer signatures.**

เอกสารไม่ควบคุม

Test Results

Instrument Performance Test Results Table

Note: These measurements do not form part of any specification and are for reference only.

	Pre PM Sensitivity Check		Post PM Sensitivity Check	
	Radial	Axial *	Radial	Axial*
Zn 213.857 nm SRBR	1782.8	2879.2	2230.8	3662.9
Mn 257.610 nm SRBR	95670.5	196149	10683.0	176884
Al 396.152 nm SBR	5.2	8.0	7.0	7.4
K 766.491 nm SBR	3.0	14.6	3.4	8.7

* Axial result is not applicable for G8016AA, G8012AA Radial View instruments.

Instrument Test Results Table

Note: The Instrument Test results are for systems using ICP Expert version 7.3 and above only.

Instrument Test	Result
Subsystem Communications Test	Pass
Air Flow	Pass
Water Flow	Pass
Gas Flows	Pass
RF Generator	Pass
Camera Test	Pass
Optics Test	Pass
Nebulizer test	Pass

เอกสารไม่ควบคุม

Consumed PM Parts

Part Description	Part Number	Product or Model# where used	Quantity consumed
Axial Pre-Optic Window	G8010-60014	G8010A, G8011A, G8014A/G8015A	1
Radial Pre-Optic Window	G8010-60015	All	1
Agilent Cool Clear Coolant Fluid	5799-0037	Agilent Water Recirculator	–
Purge Gas Filter	G8010-60136	All	1
Air Inlet filter	G8000-68002	All	1
High Capacity Air Filter	G8010-60189	Optional	–
Rotor seal for 6-7 port valve for AVS6/7	G8494-60002	G8494A/G8495	–
Rotor seal for 4 port valve for AVS4	G8493-60002	G8493A	–
Rinse solution to rinse station 2.5mm id x 1m	G8410-80123	SPS 4	–
Barb connector 2.5mm-1.5mm ID	G8410-80124	SPS 4	–
PVC waste tubing,8mm od x 5mm id, 2m	G8410-80122	SPS 4	–
Additional Parts may be required from engineer's stock:			
X axis drive belt	5410047500	SPS 3	–
Z axis drive belt	5410047400	SPS 3	–
Peristaltic pump tubing, PVC SolvaFlex, 3 bridged	3710049000	SPS 4	–

Consumed Parts Reference
(Purchased by customer, not included as part of PM)

☑ Section Not Applicable

Part Description	Part Number	Product or Model# where used	Quantity consumed

เอกสารไม่ควบคุม

ICP-OES Status Results Table

Note: These measurements do not form part of any specification and are for reference only.

Measurement	Standby Mode		Plasma On	
Mains Voltage	231.288	VAC	228.350	VAC
Mains Current	0.083	A	0.100	A
Instrument Temperature	21.1	°C	21.6	°C
RF Air Flow (sensor speed)	44.0	Hz	41.1	Hz
Plasma Exhaust Temperature	No measurement		47.1	°C
Water Flow Oscillator	No measurement		1.14	L/min
Water Flow Detector	0.92	L/min	0.90	L/min
Water Inlet Temperature	19.5	°C	18.5	°C
Polychromator Temperature	35.4	°C	36.4	°C
CCD Temperature	-40.1	°C	-39.9	°C
Thermal Stabilizer	35.0	°C	35.0	°C
Argon Supply Pressure	634.43	kPa	583.77	kPa
Purge Gas Supply Pressure*1	631.28	kPa	604.02	kPa
Option Gas Supply Pressure*1	–	kPa	–	kPa
Nebulizer Flow	No measurement		0.70	L/min
Nebulizer Back Pressure	No measurement		273.61	kPa
Plasma Gas Flow	No measurement		1195	L/min
Auxiliary Gas Flow	No measurement		1.00	L/min
RF Power	No measurement		1200.4	W
RF Supply Current	No measurement		8.228	A
RF Supply Voltage	No measurement		194.529	V

*1 If option installed

เอกสารไม่ควบคุม

Signature Page

Service Engineer Comments (optional)

If there are any specific points you wish to note as part of performing the installation or other items of interest for the customer, please write in this box.

Service Verification

Service Request Number:
6008006610

Service Engineer Name:
Worawit T.

Service Engineer Signature:
Worawit T.

Total number of pages in this document
14

Date Service Completed:
3 Nov 2025

Customer Name
Apharn O.

Customer Signature:
Apharn O.

เอกสารไม่ควบคุม

United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel.0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

Certificate of Calibration

Certificate No.: 260311-2-BL003-26
Code No.: BL003-26
Page: 1 of 3

Customer Name: United Analyst and Engineering Consultant Co., Ltd.
Address: 3 Soi Udom suk 41, Sukhumvit Rd., Bang Chak, Phar Khanong, Bangkok 10260

Equipment: Electronic Balance
Manufacturer: Mettler Toledo
Model: XP6
Serial No.: 8322373893
Asset No. : UAE.AIR.019/2556
Building : UAE number 3 Floor : 2 Room : 206

Received Date: March 11, 2026
Date of Calibation : March 13, 2026
Calibration Conditions: Temperature 18.1 °C to 19.9 °C
Humidity 56.5 % to 60.1 %
Pressure 756.6 mmHg to 756.4 mmHg

Calibrated by: Thanachat Chatpahol
Approved by: Suwit Chotnok Signature:
Issued Date: March 17, 2026

Note : 1) The Uncertainties are for a confidence probability of approximately 95%
2) This Certificate is valid only to the item calibrated on date and place of calibration.
3) This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the United Analyst and Engineering Consultant Co.,Ltd. (UAE)

เอกสารไม่ควบคุม

United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel.0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

Equipment: Electronic Balance Manufacturer: Mettler Toledo
Model: XP6 Readability: 0.000001g, 1ug
Serial No.: 8322373893 ID No.: UAE.AIR.019/2556
Max. Capacity: 6.1 g
Calibration Date: March 13, 2026

Calibration Result: (Continued)
Calibration Range: 0 to 6 (g)
Calibration Adjustment: Internal Calibration

3. Error of indication from nominal or conventional mass value:

Nominal Value (g)	Reference Value (g)	Indication (g)	Correction (g)	Uncertainty (± mg)	Coverage Factor k
Unload	0.0000000	0.000000	0.000000	0.0030	2.65
0.001	0.0010020	0.001001	0.000001	0.0035	2.13
0.010	0.0100005	0.010000	0.000000	0.0035	2.13
0.050	0.0500003	0.049999	0.000002	0.0040	2.06
0.100	0.1000383	0.100038	0.000001	0.0047	2.03
0.15	0.1500986	0.150096	0.000002	0.0074	2.00
0.17	0.1700114	0.170010	0.000001	0.0096	2.00
0.20	0.2000908	0.200097	-0.000006	0.0059	2.00
1.50	1.5000240	1.500020	0.000007	0.015	2.00
3.00	3.0000244	3.000015	0.000009	0.018	2.00
4.50	4.5000342	4.500021	0.000014	0.026	2.00
6.00	6.0000265	6.000001	0.000025	0.022	2.00

4. Effect of Tare test:

Tare Load (g)	Test Load (g)	Indication (g)	Correction (g)
3	0.600020	0.600018	0.000002
	1.200013	1.200020	-0.000007
	1.800033	1.800038	-0.000005
	2.400014	2.400013	0.000001
	3.000024	3.000016	0.000008

Remark:
The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k, providing a level of confidence of approximately 95%

o---o-End-o---o

เอกสารไม่ควบคุม

United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel.0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

Equipment: Electronic Balance Manufacturer: Mettler Toledo
Model: XP6 Readability: 0.000001g, 1ug
Serial No.: 8322373893 ID No.: UAE.AIR.019/2556
Max. Capacity: 6.1 g
Calibration Date: March 13, 2026
Condition As-Received: In Condition
Condition of Equipment:
Condition of This Result of Calibration:
1. Calibration Method: This instrument was calibrated by method UAE CP-CAL-006 In-house Method based on OIML R 76-1 : 2006
2. Reference Standards:

Reference Standard:	Model	Serial No.	Calibrated By	Certificate No.	Traceability	Due Date
Standard Weight Class E2 (OIML)	1 mg to 1 kg	CS10551605	METTLER TOLEDO GmbH	CS10641605	METTLER TOLEDO GmbH	3-Mar-27
Standard Weight Class E2 (OIML)	1 mg to 1 kg	8749109222	AMARC	25-009359	AMARC	21-Jan-27


Instrument	Model	Serial No.	Calibrated By	Certificate No.	Traceability	Due Date
Thermo-Hygro-Baro Meter	MHB-382SD	AX44457	SUCCESS	SG-H-00992/68	Success Gateway	26-Nov-26
Thermo-Hygro-Baro Meter	MHB-382SD	AX44457	TPA	25P0464	TPA	16-Dec-26

3. This certification is traceable to SI Unit
4. This certification was certified only for the instrument we calibrated
5. This result of calibration was found accurate as shown on date and place of calibration only.
6. Through the reference standard laboratory at Mettler-Toledo GmbH CS10641605 , SAS Accreditation number SCS 0030
7. Through the reference standard laboratory of AMARC 25-009359 , TISI Accreditation number 0157

Calibration Result:
1. Repeatability of Reading:

Nominal Value (g)	Standard Deviation of Reading (g)
6	0.000002

2. Eccentric or off-center loading
A mass of 2 g was placed and moved to various position on pan
The Balance reading obtained is given in the table.



1 (g)	2 (g)	3 (g)	4 (g)	5 (g)	Maximum Difference (g)
2.0000	2.0000	2.0000	2.0000	2.0000	0.0000

เอกสารไม่ควบคุม

nfi สถาบันอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

Calibration Certificate

Certificate No.: 2502226-001-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakhanong, Bangkok 10260

Equipment: Electronic Balance
Manufacturer: METTLER TOLEDO
Model: XSR205DU
Serial No.: C009071872
ID No.: UAE.WAO.012/2563
Order No.: 2502226
Operation No.: 2502226-001
Date of Receipt: 19 March 2025
Date of Calibration: 20 March 2025

Calibrated by Mr.Yothin Charoensuk
Scientist

Approved by for N. Tuanjit
(Mr.Pheraphat Tuanjit)
Manager, Division of Calibration Laboratory
Responsible for the Technical Management Team

Date of Issue: 25 March 2025

The uncertainties are for a confidence probability of approximately 95%

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

2008 ถนนอุดมสุข 41 แขวงอุดมสุข เขตบางนา กรุงเทพมหานคร 10260
2008 Soi 41, Udom Suk Road, Bang Na Khwang Udomsuk, Bang Phar District, Bangkok 10260, Thailand
Tel. +66(0) 2432-8588 Fax +66(0) 2432-8545
nfi.or.th

เอกสารไม่ควบคุม

สถาบันอาหาร
กรมส่งเสริมอุตสาหกรรม
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

Calibration Report

Certificate No.: 2502226-001-01

Equipment: Electronic Balance
Manufacturer: METTLER TOLEDO
Model: XSR205DU
Resolution: 0.00001 g / 0.0001 g
Serial No.: C309071872
ID No.: UAE.WAO.012/2563
Capacity: 82 g / 220 g

Date of Calibration: 20 March 2025

Environment Condition: Ambient Temperature: 21.2 ± 0.6 °C Relative Humidity: 48 ± 3.5 %
Place of Calibration: 208 Balance Room, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Condition of Equipment: Good Condition
Condition of This Results of Calibration:

1. Calibration Method: NFI Method W-MA-001 In-House Method based on LAAS Lab 14 : 2019
2. Reference Standards:

Reference Standard	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Standard Weight Class F2	1mg to 200g	8N556795/2	TCS	K24041005	16 April 2025
Instrument	**Model**	**Serial No.**	**Calibrated By**	**Certificate No.**	**Due Date**
Thermo Hygro Meter	608-H1	M-LBTH 017/23	Quality Kasorn	QR25-0542	10 February 2026

3. This certification is traceable to SI UNIT
4. This certificate was certified only for the instrument we calibrate.
5. This result of calibration was found accurate as shown on date and place of calibration only.

Calibration Results:

1. Repeatability of Reading:

Nominal Value (g)	Standard Deviation of Reading (g)
40	0.0000052
80	0.0000042
100	0.0000000
200	0.0000000

2. Off-Center Error:

A mass of 100 g was placed and moved to various position on pan.
The balance reading obtained is given in the table.

☑ ☐ ☐

1 (g)	2 (g)	3 (g)	4 (g)	5 (g)	6 (g)	(Maximum Difference) (g)
100.0001	100.0001	100.0001	100.0001	100.0001	100.0003	0.0003

for N. miyarbait

2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพมหานคร 10700
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel. +66(0) 2422 8688 Fax +66(0) 2422 8545
nfi.or.th
เอกสารไม่ควบคุม

สถาบันอาหาร
กรมส่งเสริมอุตสาหกรรม
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

Calibration Report

Certificate No.: 2502226-001-01

Equipment: Electronic Balance
Manufacturer: METTLER TOLEDO
Model: XSR205DU
Resolution: 0.00001 g / 0.0001 g
Serial No.: C309071872
ID No.: UAE.WAO.012/2563
Capacity: 82 g / 220 g

Date of Calibration: 20 March 2025

Calibration Results: (Continued)
Calibration Range: >80-200 g
Calibration Adjustment: Internal Calibration

3. Departure from Nominal Value: (Range: >80 - 200 g ; Resolution: 0.0001 g)

Nominal Value (g)	Standard Value (g)	Average Reading (g)	Correction (g)	Uncertainty (± g)	Coverage Factor #
90	90.00010	90.0002	0.0001	0.00015	2.00
100	100.00000	100.0001	0.0000	0.00016	2.00
110	110.00007	110.0001	0.0000	0.00017	2.00
120	120.00009	120.0002	0.0001	0.00018	2.00
130	130.00010	130.0002	0.0001	0.00019	2.00
140	140.00013	140.0002	0.0001	0.00019	2.00
150	150.00009	150.0002	0.0001	0.00021	2.00
160	160.00010	160.0002	0.0001	0.00022	2.00
170	170.00012	170.0002	0.0001	0.00023	2.00
200	200.00013	200.0002	0.0001	0.00028	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor # , providing a level of confidence of approximately 95 %.

---------- End ----------

for N. miyarbait
F-CS-012 Revision: 01 Date: 20-06-65
2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพมหานคร 10700
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel. +66(0) 2422 8688 Fax +66(0) 2422 8545
nfi.or.th
เอกสารไม่ควบคุม

สถาบันอาหาร
กรมส่งเสริมอุตสาหกรรม
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

Calibration Report

Certificate No.: 2502226-001-01

Equipment: Electronic Balance
Manufacturer: METTLER TOLEDO
Model: XSR205DU
Resolution: 0.00001 g / 0.0001 g
Serial No.: C309071872
ID No.: UAE.WAO.012/2563
Capacity: 82 g / 220 g

Date of Calibration: 20 March 2025

Calibration Results: (Continued)
Calibration Range: 0-80 g
Calibration Adjustment: Internal Calibration

3. Departure from Nominal Value: (Range: 0 - 82 g ; Resolution: 0.00001 g)

Nominal Value (g)	Standard Value (g)	Average Reading (g)	Correction (g)	Uncertainty (± g)	Coverage Factor #
Unload	0.000000	0.00000	0.00000	0.0000089	2.00
0.001	0.001003	0.00100	0.00000	0.0000092	2.00
0.005	0.005002	0.00500	0.00000	0.0000094	2.00
0.01	0.013003	0.01300	0.00000	0.0000091	2.00
0.05	0.049996	0.05000	0.00000	0.0000098	2.00
0.1	0.100011	0.10000	0.00001	0.000011	2.00
0.5	0.500016	0.50000	0.00002	0.000014	2.00
1	1.000003	1.00001	-0.00001	0.000016	2.00
2	2.000023	2.00005	-0.00003	0.000017	2.00
5	5.000015	5.00005	-0.00003	0.000021	2.00
10	10.000009	10.00005	-0.00004	0.000026	2.00
20	20.000030	20.00012	-0.00009	0.000037	2.00
30	30.000039	30.00012	-0.00008	0.000050	2.00
50	50.000028	50.00014	-0.00011	0.000068	2.00
80	80.000067	80.00020	-0.00013	0.00011	2.00

for N. miyarbait
F-CS-012 Revision: 01 Date: 20-06-65
2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพมหานคร 10700
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel. +66(0) 2422 8688 Fax +66(0) 2422 8545
nfi.or.th
เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

CERTIFICATE OF CALIBRATION

Certificate No. : SP25-019

Customer : United Analyst and Engineering Consultant Co.,Ltd. (Head Office)

Address : 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Location of calibration : Instrument room (207)

Equipment : UV-Vis Spectrophotometer

Manufacturer : Agilent Technologies

Model : Cary 60

Serial No. : MY15410009

ID No. : UAE.WAT.020/2558

Received Date : 26 May 2025

Calibration Date : 26 May 2025

Issue Date : 29 May 2025

Condition Instrument : Good

Calibrated by : (Mr.Tanawut Rittidach) Technical Manager

Approved by : (Ms.Chonticha Sangngern) Quality Manager

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the DQE Services Co., Ltd.

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP25-019

Environment Condition : Ambient Temperature 25 ± 5 °C

Relative humidity 55 ± 20 %RH

Calibration method : In-house method CP-01 Based on ASTM E275-08

Certified Reference Materials :

Material	Serial No.	Certificate No.	Due date
Absobance Standard set	25760	115663	25 October 2025
Absobance Standard set	25757	115638	25 October 2025
Wavelength Standard set	25806	115657	25 October 2025
Wavelength Standard set	25758	115665	25 October 2025

Traceability : This certification is traceable to the International System of Unit maintained at National - Institute of Standards and Technology (NIST) through Starna Scientific Limited

Spectral Band Width of UUC : 1.5 nm.

Scan Speed of UUC : 60 nm/min

Scan Interval of UUC : 0.15 nm.

Resolution of UUC : Photometric 0.0001 Abs.

Wavelength 0.1 nm.

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP25-019

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
235	0.0000	0.0000	0.0000	0.0050	2.00
	0.7469	0.7488	-0.0019	0.0063	2.00
257	0.0000	0.0000	0.0000	0.0050	2.00
	0.8674	0.8663	0.0011	0.0067	2.00
313	0.0000	0.0000	0.0000	0.0050	2.00
	0.2919	0.2902	0.0017	0.0052	2.00
350	0.0000	0.0000	0.0000	0.0050	2.00
	0.6430	0.6428	0.0002	0.0063	2.00

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP25-019

Calibration Results : Without adjustment

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
420	0.0000	0.0000	0.0000	0.0028	2.00
	0.5780	0.5739	0.0041	0.0031	2.00
	1.0484	1.0430	0.0054	0.0029	2.00
	2.1876	2.1876	0.0000	0.0084	2.00
440	0.0000	0.0000	0.0000	0.0028	2.00
	0.5595	0.5581	0.0014	0.0034	2.00
	1.0239	1.0219	0.0020	0.0035	2.00
	2.1230	2.1207	0.0023	0.0085	2.00
465	0.0000	0.0000	0.0000	0.0028	2.00
	0.5230	0.5190	0.0040	0.0029	2.00
	0.9633	0.9609	0.0024	0.0029	2.00
	1.9753	1.9719	0.0034	0.0079	2.00
546.1	0.0000	0.0000	0.0000	0.0028	2.00
	0.5181	0.5161	0.0020	0.0031	2.00
	1.0002	0.9979	0.0023	0.0033	2.00
	1.9973	2.0021	-0.0048	0.0102	2.00
590	0.0000	0.0000	0.0000	0.0028	2.00
	0.5517	0.5503	0.0014	0.0030	2.00
	1.0803	1.0808	-0.0005	0.0031	2.00
	2.0373	2.0324	0.0049	0.0105	2.00
635	0.0000	0.0000	0.0000	0.0028	2.00
	0.5591	0.5583	0.0008	0.0031	2.00
	1.0518	1.0513	0.0005	0.0030	2.00
	1.9274	1.9281	-0.0007	0.0102	2.00

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP25-019

Wavelength Accuracy :

CRMs Values (nm.)	UUC Reading (nm.)	Correction (nm.)	Uncertainty (nm.)	Coverage factor k
241.72	242.0	-0.28	0.18	2.00
279.45	279.5	-0.05	0.18	2.00
287.81	287.6	0.21	0.18	2.00
334.06	333.8	0.26	0.18	2.00
360.93	360.5	0.43	0.18	2.00
418.59	417.9	0.69	0.18	2.00
445.94	445.4	0.54	0.18	2.00
453.66	453.2	0.46	0.18	2.00
460.02	459.6	0.42	0.18	2.00
536.59	536.5	0.09	0.18	2.00
637.98	638.5	-0.52	0.18	2.00
431.38	430.7	0.68	0.18	2.00
472.50	472.3	0.20	0.18	2.00
513.47	513.5	-0.03	0.18	2.00
528.88	528.9	-0.02	0.18	2.00
573.17	573.8	-0.63	0.18	2.00
585.35	585.2	0.15	0.20	2.00
684.40	685.1	-0.70	0.18	2.00
740.72	741.1	-0.38	0.20	2.00
748.55	748.9	-0.35	0.18	2.00
807.03	807.1	-0.07	0.18	2.00
879.28	879.1	0.18	0.18	2.00

Remark : - UUC = Unit Under Calibration

- N/A = Not Avaiable
- The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%

- End of Certificate -

เอกสารไม่ควบคุม

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

Certificate of Calibration

Cert. No.: 25TM578
Page : 1 of 3

Equipment : BOD Incubator
Manufacturer : ARCO
Model : UR-1320
Serial No. : -
ID No. : UAE.WAO.006/2553
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260
Location : Lab Floor 2

Received Order : 19 March 2025
Calibration Date : 19 March 2025
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %
AC Line Voltage : (220 ± 22) V

Calibrated by : Man Pattanapongpaiboon

Approved by :
Approved Signatory

( ) Chakrit Waewwanjua
( ) Suwit Imjai
(✓) Kunchit Promprat

Issue Date : 27 March 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor k
20.0	20.0	19.9	0.49	0.69	1.1	2

Calibration Point (°C)	Measured Temperature (°C) Position									Uncertainty
	1	2	3	4	5	6	7	8	9 (ref.)	(±°C)
20.0	20.025	19.753	20.063	19.839	20.103	20.086	20.152	20.211	19.804	0.69

Average* : The average of 30 values in each position.
Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.
Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.
Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.
UUC* : Unit Under Calibration
Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor ***k***, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม

Procedure Used :-
Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).
The temperature scale used was based on ITS-90.


Condition of this result of calibration
1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY44073381	24LM73	TPA	18 May 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.
Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Environment during calibration	Beginning	Finished
Temp. (°C)	28	28
REL.Humid. (%)	56	55
AC Supply (Volt)	224	224



Position :	Ref. Std. ID No.:
1	1RTD-2/1
2	1RTD-2/2
3	22-01RTD-03
4	1RTD-2/4
5	1RTD-2/5
6	1RTD-2/6
7	23-01RTD-07
8	1RTD-2/8
9 (ref.)	23-01RTD-09

Probe Installation Details :
a = 10 cm
b = 10 cm
c = 10 cm

Dimension of Chamber :
D = 0.62 m
W = 1.2 m
H = 1.2 m
Capacity = 0.89 m³

เอกสารไม่ควบคุม

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000 FAX 0-2719-9484

Certificate of Testing

Cert.No.: 25TW29
Page.: 1 of 2

Equipment : DO Meter
Manufacturer : YSI
Model : 5100
Serial No. : 11B 101863
ID No. : UAE.WAO.004/2554
Received Date : 14 February 2025
Test Date : 17 February 2025
Reference : 2502-0473DSC-1
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260

Laboratory Condition : Temperature (25 ± 5) °C
Humidity (50 ± 20) %
Test Procedure : In - house method : CP-CH9
by Comparison Technique with Azide Modification Method

Tested by : Walalak Sirithean

Approved by :
Approved Signatory

( ) Chakrit Waewwanjua
( ) Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 18 February 2025

เอกสารไม่ควบคุม

Condition of this result of calibration

1. Reference Standard Instruments :
This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

Instruments	Serial No.	ID No.	Certificate No.	Due Date
1. Burette	-	130BU10	23CG1172	22 Mar 2025
2. Balance	14233821	110RC001	24MM131	04 July 2025

2. Standard Material :-

Material	Manufacturer	Lot.No.	Assay
Sodium Thiosulfate 5-Hydrate AR	KEMAUS	2203162447	99.6%

Result : **Dissolved Oxygen Meter Adjustment With Air 100 %**
Dissolved Oxygen Probe No.: 24F100202

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.22	8.22	0.0055

This report was certified only for the instrument we tested.It is allowable to use for study Intend to use for advertising and referral purpose is prohibited.This report may not be reproduced other in full, without written approval of the laboratory

-o0o-

เอกสารไม่ควบคุม

United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel.0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com


Certificate of Calibration

Certificate No.: 250422-1-BL002-25
Code No.: BL002-25

Customer Name:	United Analyst and Engineering Consultant Co., Ltd.			
Address:	3 Soi Udom suk 41, Sukhumvit Rd., Bang Chak, Phar Khanong, Bangkok 10260			
Equipment:	Electronic Balance			
Manufacturer:	Mettler Toledo			
Model:	AB204-S/FACT			
Serial No.:	1129361010			
Asset No. :	UAE.WAS.002/2552			
Building :	N/A	Floor : 1		Room : 107
Received Date:	April 22, 2025			
Date of Calibation :	April 23, 2025			
Calibration Conditions:	Temperature	22.8 °C	to	23.5 °C
	Humidity	56.8 %	to	68.9 %
	Pressure	756.6 mm Hg	to	758.2 mm Hg
Calibrated by:	Sakkarin Srirahang			
Approved by:	Suwit Chotnok	Signature:		
Issued Date:	April 25, 2025			

Note : 1) The Uncertainties are for a confidence probability of approximately 95%
2) This Certificate is valid only to the item calibrated on date and place of calibration.
3) This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the United Analyst and Engineering Consultant Co.,Ltd. (UAE)

เอกสารไม่ควบคุม

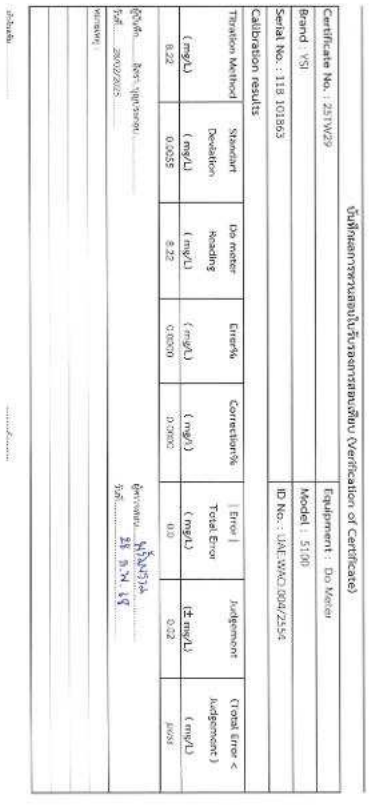

บันทึกผลการสอบเทียบ (Verification of Certificate)

Certificate No. : 25TW29
Brand : YSI
Serial No. : 118 101863
Calibration results
ID No. : UAE.WAS.002/2552
Equipment : Do Meter
Model : 5100

Titration Method (mg/L)	Standard Deviation (mg/L)	Do meter Reading (mg/L)	Error% (mg/L)	Correction% (mg/L)	[Error] Total Error (mg/L)	Judgement (± mg/L)	(Total Error < Judgement) (mg/L)
8.22	0.0055	8.22	0.0000	0.0000	0.0	0.22	pass

ผู้ปฏิบัติ ..... ตรวจสอบ .....
วันที่ 28/02/2025
Manager

เอกสารไม่ควบคุม

United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel.0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

Certificate No.: 250422-1-BL002-25
Code No.: BL002-25

Equipment:	Electronic Balance	Manufacturer:	Mettler Toledo
Model:	AB204-S/FACT	Readability:	0.0001 g
Serial No.:	1129361010	ID No.:	UAE.WAS.002/2552
Max. Capacity:	220 g		
Calibration Date:	April 23, 2025		
Condition As-Received:	In Condition		

Condition of Equipment:

Condition of This Result of Calibration:

1. Calibration Method: This instrument was calibrated by method UAE.CP/CAL.006 In-House Method based on UKAS Lab 14 : 2022
2. Reference Standrads:

Reference Standard:	Model	Serial No.	Calibrated By	Certificate No.	Traceability	Due Date
Standard Weight Class E2 (OIML)	1 mg to 1 kg	8M6109122	AMARC	25-009359	Mettler-Toledo	21-Jan-27
Standard Weight Class F1 (OIML)	1 mg to 200 g	11119512	AMARC	24-013843	Mettler-Toledo	04-Feb-26
Instrument	**Model**	**Serial No.**	**Calibrated By**	**Certificate No.**	**Traceability**	**Due Date**
Thermo-Hygro-Baro Meter	MHB-382SD	AK46457	SUCCESS	SS-41009267	Success Gateway	21-Nov-25
Thermo-Hygro-Baro Meter	MHB-382SD	AK46457	TPA	25P795	TPA	25-Feb-26


3. This certification is traceable to SI Unit.
4. This certification was certified only for the instrument we calibrated.
5. This result of calibration was found accurate as show on date and place of calibration only.
6. Through the reference standard laboratory of AMARC 25-009359 Calibration 0152

Calibraton Result:

1. Repeatability of Reading:

Nominal Value (g)	Standard Deviation of Reading (g)
200*	0.000045

2. Eccentric or off-center loading
A mass of 100 g was placed and moved to various position on pan
The Balance reading obtained is given in the table.

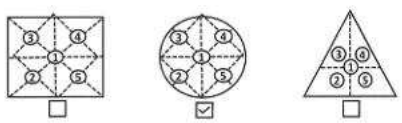

1 (g)	2 (g)	3 (g)	4 (g)	5 (g)	Maximum Difference (g)
100.0000	99.9996	99.9997	100.0005	100.0005	0.0005

เอกสารไม่ควบคุม

United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel.0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

Certificate No.: 250422-1-BL002-25
Code No.: BL002-25

Equipment:	Electronic Balance	Manufacturer:	Mettler Toledo
Model:	AB204-S/FACT	Readability:	0.0001 g
Serial No.:	1129361010	ID No.:	UAE.WAS.002/2552
Max. Capacity:	220 g		
Calibration Date:	April 23, 2025		

Calibraton Result: (Continued)
Calibraton Range: 0 - 200 g
Calibraton Adjustment: Internal Calibration

3. Error of indication from nominal or conventional mass value:

Nominal Value (g)	Reference Value (g)	Indication (g)	Correction (g)	Uncertainty (± mg)	Coverage Factor k
Unload	0.0000000	0.0000	0.0000	0.10	2.05
0.01	0.0100025	0.0099	0.0001	0.10	2.05
0.05	0.0500056	0.0500	0.0000	0.10	2.05
0.1	0.1000012	0.0999	0.0001	0.10	2.05
0.5	0.5000133	0.5000	0.0000	0.10	2.05
1	1.0000105	1.0000	0.0000	0.10	2.05
10	10.000010	10.0000	0.0000	0.11	2.04
40	40.000076	40.0000	0.0000	0.14	2.00
50	50.000056	50.0000	0.0001	0.15	2.00
80	80.000107	80.0000	0.0001	0.18	2.00
100	100.000109	99.9999	0.0002	0.17	2.00
120	120.00015	119.9999	0.0003	0.21	2.00
150	150.000165	149.9998	0.0003	0.24	2.00
160	160.000175	159.9997	0.0005	0.26	2.00
200	200.000129	199.9998	0.0004	0.30	2.00

4. Effect of Tare test:

Tare Load (g)	Test Load (g)	Indication (g)	Correction (g)
100	20.000041	19.9999	0.0001
	40.000076	39.9998	0.0002
	60.000066	59.9997	0.0003
	80.000107	79.9999	0.0002
	100.000168	100.0004	-0.0003

Remark:
The report uncertainty of measurement was based on standard uncertainty multiplies by coverage factor k, providing [illegible]

o—o-End-o—o

เอกสารไม่ควบคุม

Qualification Report

PM_Checklist : CM_OQ and PQ
Inuvion: Anion (ID#1248)

For
UAE Consultant Co.,Ltd.
(1st Warranty)

เอกสารไม่ควบคุม

ARCHEMICA

Certificate of Calibration

Inuvion : (Anion System ID#1248)

This certificate is to verify that instrument below are calibrated
by Archemica International Co.,Ltd.

Inuvion S/N : 250451070
AS-DV S/N : 25027024

for

UAE Consultant Co.,Ltd.

ARCHEMICA
บริษัท อาร์เคมีก้า อินเตอร์เนชั่นแนล จำกัด
ARCHEMICA INTERNATIONAL CO.,LTD.

Operator Signature : _____ Date : Mar 19, 2026

(Mr.Itsaraphap Bumrungjeam)
Applications Chemist

เอกสารไม่ควบคุม

PM

Preventive Maintenance
Check List

เอกสารไม่ควบคุม

Dionex Ion Chromatography
Preventive Maintenance Report

Customer Organization	Name/ Department
UAE Consultant Co.,Ltd.	K.Suwan
Engineer	**Date**
Mr.Itsaraphap Bumrungjeam	19/Mar/26

Instrument Detail

Instrument Model	Application
Inuvion (ID#1248)	Anion
Instrument components	**Serial Number**
Inuvion	250451070
AS-DV	25027024

Consumable Detail

Columns	Guard Columns	Suppressors	Concentrators	Etc.
AS22	AG22	ASRS300		

Remark:

Perform By Archemica

ARCHEMICA

Archemica
19/3/26
Date

Customer
19/3/26
Date

เอกสารไม่ควบคุม

AS-DV Autosampler Preventive Maintenance Checklist

Model	Serial number	Firmware Version
☒ AS-DV	25027024	1.6.0

No.	Description	Result			
	Power and Connection	**Checked**	**Cleaned**	**Replaced**	**N/A**
1.	AS-DV power on	☒	-	-	☐
2.	AS-DV connection	☒	-	-	☐
	Sampling Unit	**Checked**	**Cleaned**	**Replaced**	**N/A**
3.	Sampling needle	☐	☒	☐	☐
4.	Sampling tubing (Transfer line)	☐	☒	☐	☐
5.	Reconnect sampling needle & tubing	☒	-	-	☐
	Others	**Checked**	**Cleaned**	**Replaced**	**N/A**
6.	Check carousel movement	☒	-	-	☐
7.	Check needle movement	☒	-	-	☐
8.	Lubricate needle drive	☒	☐ Lubricated	-	☐
9.	AS-DV cover	☒	☐	☐	☐
	Optional Injection Valve	**Checked**	**Cleaned**	**Replaced**	**N/A**
10.	High pressure valve Port	☐	☐	☐	☒
11.	- Rotor seal	☐	☐	☐	☒
12.	- Stator face	☐	☐	☐	☒
13.	- Reconnected liquid line to the valve	☐	☐	☐	☒

Others (comments)

เอกสารไม่ควบคุม

General ICS Maintenance Checklist

No.	Description	Result			
	Power and Connection	**Checked**	**Cleaned**	**Replaced**	**N/A**
1	Instrument power on	☒	-	-	☐
2	Instrument connection	☒	-	-	☐
	Injection Valve (Optional)	**Checked**	**Cleaned**	**Replaced**	**N/A**
3	Rebuilt injection valve 6 port	☐	☒	☐	☐
4	- Rotor seal	☐	☒	☐	☐
5	- Stator face	☐	☒	☐	☐
	Optional Auxiliary Valve (Optional)	**Checked**	**Cleaned**	**Replaced**	**N/A**
6	Rebuilt auxiliary valve port	☐	☐	☐	☒
7	- Rotor seal	☐	☐	☐	☒
8	- Stator face	☐	☐	☐	☒
	Check Valves	**Checked**	**Cleaned**	**Replaced**	**N/A**
9	Inlet check valve assembly	☐	☒	☐	☐
10	Outlet check valve assembly	☐	☒	☐	☐
11	Verified correct flow orientation:	☒	-	-	☐
	Piston and Piston Seal	**Checked**	**Cleaned**	**Replaced**	**N/A**
12	Piston rinse seal in *primary* pump head	☐	☒	☐	☐
13	Piston seal in *primary* pump head	☐	☒	☐	☐
14	Piston in *primary* pump head	☐	☒	☐	☐
15	Piston rinse seal in *secondary* pump head	☐	☒	☐	☐
16	Piston seal in *secondary* pump head	☐	☒	☐	☐
17	Piston in *secondary* pump head	☐	☒	☐	☐
	Waste Valve and Priming Valve	**Checked**	**Cleaned**	**Replaced**	**N/A**
18	Waste valve	☒	☐	☐	☐
19	Priming valve	☒	☐	☐	☐
	Conductivity Cell (Optional)	**Checked**	**Cleaned**	**Replaced**	**N/A**
20	Check conductivity cell	☒	☐	☐	☐
21	Check electrochemical cell	☐	☐	☐	☒
22	- Working electrode	☐	☐	☐	☒
23	- Reference electrode	☐	☐	☐	☒
24	- Gasket	☐	☐	☐	☒
25	- Cell body	☐	☐	☐	☒
	Others	**Checked**	**Cleaned**	**Replaced**	**N/A**
26	Sample Loop Size 25 uL	☐	☒	☐	☐
27	End-line filter	☒	-	☐	☐
28	Leak sensor	☒	☐	☐	☐
29	Lubricate pump mechanic	☒	☐ Lubricated	-	☐
30	Reconnected liquid lines to the valve	☒	-	-	☐
31	Reconnected liquid lines to pump heads	☒	-	-	☐
32	Primed pump	☒	-	-	☐
33	Checked pump for leaks	☒	-	-	☐
34	Checked gas for leaks	☒	-	-	☐

เอกสารไม่ควบคุม

CM OQ

Chromeleon
Operation Qualification

เอกสารไม่ควบคุม

ThermoFisher SCIENTIFIC

Chromeleon Operational Qualification

General Information

	Computer Name	Version Number:
Instrument Controller:	DESKTOP-SQDHP9U	7.3.2 Build 14225
Client:	DESKTOP-SQDHP9U	7.3.2.14225
Operator:	Mr.Itsaraphap Bumrungjeam	

Overall Test Result: ***Passed***

Comparison Format:

All Parameters:	Significant Digits:	10

ARCHEMICA
บริษัท อาร์คีมิคา อินเตอร์เนชั่นแนล จำกัด
ARCHEMICA INTERNATIONAL CO.,LTD.

19/3/26
Reviewer's Signature / Date

19/3/26
Operator's Signature / Date

เอกสารไม่ควบคุม

ThermoFisher SCIENTIFIC

Chromeleon Operational Qualification, Part 1

Verification of Selected Results

Detection Algorithm:	Cobra
Calibration Type:	Lin, WithOffset
Evaluation Type:	Area
Standard Method:	External
Calibration Mode:	Total

Report Variable	*Peak Name*	*Status*
Offset (c0)	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Slope (c1)	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Correlation Coefft.	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Variance	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Std. Deviation	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Rel. Std. Dev.	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Variance Coeff.	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok

เอกสารไม่ควบคุม

ThermoFisher SCIENTIFIC

Chromeleon Operational Qualification, Part 1

Verification of Selected Results

Report Variable	*Peak Name*	*Status*
Calibration Point X	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Calibration Point Y	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Amount [ng]	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Resolution (EP)	Acetanilide	ok
	Acetophenone	ok
Resolution (USP)	Acetanilide	ok
	Acetophenone	ok
Peak Asymmetry (EP/USP)	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Peak Asymmetry (AIA)	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok

เอกสารไม่ควบคุม

ThermoFisher SCIENTIFIC

Chromeleon Operational Qualification, Part 1

Verification of Selected Results

Report Variable	*Peak Name*	*Status*
Theoretical Plates (EP)	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Theoretical Plates (USP)	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Theoretical Plates (JP)	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok

Test Result: ***Passed***

เอกสารไม่ควบคุม

ThermoFisher SCIENTIFIC

Chromeleon Operational Qualification, Part 2

Most Frequently Used Parameters: Comparison with Expected Results

Detection Algorithm: Cobra
Calibration Type: Lin, WithOffset
Evaluation Type: Area
Standard Method: External
Calibration Mode: Total

Variable Category	Report Variable	Peak Name	Status
Injection	No.		ok
	Name		ok
	Type		ok
	Position		ok
	Status		ok
	Volume		ok
	Dilution Factor		ok
	Weight		ok
	IntStd		ok
	InstrumentMethod		ok
	ProcessingMethod		ok
Chromatogram	Channel		ok
	No. of Peaks		ok
	Chromatogram Start Time		ok
	Signal Min.		ok
	Signal Max.		ok
	Unit		ok
	Noise		ok
Peak Results	No.	Acetanilide	ok
	No.	Acetophenone	ok
	No.	Propiophenone	ok
	Peak Name	Acetanilide	ok
	Peak Name	Acetophenone	ok
	Peak Name	Propiophenone	ok
	Ret.Time	Acetanilide	ok
	Ret.Time	Acetophenone	ok
	Ret.Time	Propiophenone	ok

เอกสารไม่ควบคุม

ThermoFisher SCIENTIFIC

Chromeleon Operational Qualification, Part 2

Most Frequently Used Parameters: Comparison with Expected Results

Variable Category	Report Variable	Peak Name	Status
Peak Results	Abs.Ret.Dev.	Acetanilide	ok
	Ret.Dev.(abs)	Acetophenone	ok
	Ret.Dev.(abs)	Propiophenone	ok
	Rel.Ret.Dev.	Acetanilide	ok
	Ret.Dev.(rel)	Acetophenone	ok
	Ret.Dev.(rel)	Propiophenone	ok
	Area	Acetanilide	ok
	Area	Acetophenone	ok
	Area	Propiophenone	ok
	Rel.Area	Acetanilide	ok
	Rel.Area (Total)	Acetophenone	ok
	Rel.Area (Total)	Propiophenone	ok
	Height	Acetanilide	ok
	Height	Acetophenone	ok
	Height	Propiophenone	ok
	Rel.Height (Total)	Acetanilide	ok
	Rel.Height (Total)	Acetophenone	ok
	Rel.Height (Total)	Propiophenone	ok
	Amount	Acetanilide	ok
	Amount	Acetophenone	ok
	Amount	Propiophenone	ok
	Concentration	Acetanilide	ok
	Concentration	Acetophenone	ok
	Concentration	Propiophenone	ok
	Rel.Amount	Acetanilide	ok
	Rel.Amount	Acetophenone	ok
	Rel.Amount	Propiophenone	ok
	Peak Width (0%)	Acetanilide	ok
	Peak Width (0%)	Acetophenone	ok
	Peak Width (0%)	Propiophenone	ok
	Peak Width (5%)	Acetanilide	ok
	Peak Width (5%)	Acetophenone	ok
	Peak Width (5%)	Propiophenone	ok
	Peak Width (10%)	Acetanilide	ok
	Peak Width (10%)	Acetophenone	ok
	Peak Width (10%)	Propiophenone	ok

เอกสารไม่ควบคุม

ThermoFisher SCIENTIFIC

Chromeleon Operational Qualification, Part 2

Most Frequently Used Parameters: Comparison with Expected Results

Variable Category	Report Variable	Peak Name	Status
Peak Results	Peak Width (50%)	Acetanilide	ok
	Peak Width (50%)	Acetophenone	ok
	Peak Width (50%)	Propiophenone	ok
	Left Width (0%)	Acetanilide	ok
	Left Width (0%)	Acetophenone	ok
	Left Width (0%)	Propiophenone	ok
	Right Width (0%)	Acetanilide	ok
	Right Width (0%)	Acetophenone	ok
	Right Width (0%)	Propiophenone	ok
	Peak Start	Acetanilide	ok
	Peak Start	Acetophenone	ok
	Peak Start	Propiophenone	ok
	Peak Stop	Acetanilide	ok
	Peak Stop	Acetophenone	ok
	Peak Stop	Propiophenone	ok
	Peak Start Value	Acetanilide	ok
	Peak Start Value	Acetophenone	ok
	Peak Start Value	Propiophenone	ok
	Peak Stop Value	Acetanilide	ok
	Peak Stop Value	Acetophenone	ok
	Peak Stop Value	Propiophenone	ok
	BL-Value Peak Start	Acetanilide	ok
	BL-Value Peak Start	Acetophenone	ok
	BL-Value Peak Start	Propiophenone	ok
	BL-Value Peak Stop	Acetanilide	ok
	BL-Value Peak Stop	Acetophenone	ok
	BL-Value Peak Stop	Propiophenone	ok
	Type	Acetanilide	ok
	Type	Acetophenone	ok
	Type	Propiophenone	ok
	Resolution (EP)	Acetanilide	ok
	Resolution(EP)	Acetophenone	ok
	Resolution(USP)	Acetanilide	ok
	Resolution(USP)	Acetophenone	ok
	Asymmetry(EP)	Acetanilide	ok
	Asymmetry(EP)	Acetophenone	ok
	Asymmetry(EP)	Propiophenone	ok

เอกสารไม่ควบคุม

ThermoFisher SCIENTIFIC

Chromeleon Operational Qualification, Part 2

Most Frequently Used Parameters: Comparison with Expected Results

Variable Category	Report Variable	Peak Name	Status
Peak Results	Asymmetry(AIA)	Acetanilide	ok
	Asymmetry(AIA)	Acetophenone	ok
	Asymmetry(AIA)	Propiophenone	ok
	Theor. Plates(EP)	Acetanilide	ok
	Theor. Plates(EP)	Acetophenone	ok
	Theor. Plates(EP)	Propiophenone	ok
	Theor. Plates(USP)	Acetanilide	ok
	Theor. Plates(USP)	Acetophenone	ok
	Theor. Plates(USP)	Propiophenone	ok
	Theor.Plates (JP)	Acetanilide	ok
	Theor. Plates(JP)	Acetophenone	ok
	Theor. Plates(JP)	Propiophenone	ok
Peak Calibration	Cal.Mode	Acetanilide	ok
	Cal.Mode	Acetophenone	ok
	Cal.Mode	Propiophenone	ok
	Cal.Type	Acetanilide	ok
	Cal.Type	Acetophenone	ok
	Cal.Type	Propiophenone	ok
	Weights	Acetanilide	ok
	Weights	Acetophenone	ok
	Weights	Propiophenone	ok
	Calibr. Coefficient C0	Acetanilide	ok
	Calibr. Coefficient C0	Acetophenone	ok
	Calibr. Coefficient C0	Propiophenone	ok
	Calibr. Coefficient C1	Acetanilide	ok
	Calibr. Coefficient C1	Acetophenone	ok
	Calibr. Coefficient C1	Propiophenone	ok
	RF-Value	Acetanilide	ok
	RF-Value	Acetophenone	ok
	RF-Value	Propiophenone	ok
	No. of Points	Acetanilide	ok
	No. of Points	Acetophenone	ok

เอกสารไม่ควบคุม

ThermoFisher SCIENTIFIC

Chromeleon Operational Qualification, Part 2

Most Frequently Used Parameters: Comparison with Expected Results

Variable Category	Report Variable	Peak Name	Status
Peak Calibration	No. of Points	Propiophenone	ok
	No. of Points(disabled)	Acetanilide	ok
	No. of Points(disabled)	Acetophenone	ok
	No. of Points(disabled)	Propiophenone	ok
	Variance	Acetanilide	ok
	Variance	Acetophenone	ok
	Variance	Propiophenone	ok
	Var.Coeff	Acetanilide	ok
	Var.Coeff	Acetophenone	ok
	Var.Coeff	Propiophenone	ok
	Std.Dev.	Acetanilide	ok
	Std.Dev.	Acetophenone	ok
	Std.Dev.	Propiophenone	ok
	Rel.Std.Dev.	Acetanilide	ok
	Rel.Std.Dev.	Acetophenone	ok
	Rel.Std.Dev.	Propiophenone	ok
	Corr.Coeff.	Acetanilide	ok
	Corr.Coeff.	Acetophenone	ok
	Corr.Coeff.	Propiophenone	ok
	R-Square	Acetanilide	ok
	R-Square	Acetophenone	ok
	R-Square	Propiophenone	ok
	Adj. R-Square	Acetanilide	ok
	Adj. R-Square	Acetophenone	ok
	Adj. R-Square	Propiophenone	ok
	X	Acetanilide	ok
	X	Acetophenone	ok
	X	Propiophenone	ok
	Y	Acetanilide	ok
	Y	Acetophenone	ok
	Y	Propiophenone	ok
	W	Acetanilide	ok
	W	Acetophenone	ok
	W	Propiophenone	ok
	F(X)	Acetanilide	ok
	F(X)	Acetophenone	ok
	F(X)	Propiophenone	ok

เอกสารไม่ควบคุม

ThermoFisher SCIENTIFIC

Chromeleon Operational Qualification, Part 2

Most Frequently Used Parameters: Comparison with Expected Results

Variable Category	Report Variable	Peak Name	Status
Peak Calibration	Residual for Cal.Point X	Acetanilide	ok
	Residual for Cal.Point X	Acetophenone	ok
	Residual for Cal.Point X	Propiophenone	ok
	Calibration Point Status	Acetanilide	ok
	Calibration Point Status	Acetophenone	ok
	Calibration Point Status	Propiophenone	ok
	Amount	Acetanilide	ok
	Amount	Acetophenone	ok
	Amount	Propiophenone	ok
Component	Cal.Type	Acetanilide	ok
	Peak Type	Acetanilide	ok
	Left Limit	Acetophenone	ok
	Right Limit	Acetanilide	ok
	Group	Acetanilide	ok
	Factor	Acetophenone	ok
	Amount	Acetanilide	ok
	Conc.Unit	Acetophenone	ok

เอกสารไม่ควบคุม

ThermoFisher SCIENTIFIC

Chromeleon Operational Qualification, Part 2

Most Frequently Used Parameters: Comparison with Expected Results

Variable Category	Report Variable	Peak Name	Status
Peak Purity	PPI	Acetanilide	ok
	PPI	Acetophenone	ok
	PPI	Propiophenone	ok
	RSD PPI	Acetanilide	ok
	RSD PPI	Acetophenone	ok
	RSD PPI	Propiophenone	ok
	Match	Acetanilide	ok
	Match	Acetophenone	ok
	Match	Propiophenone	ok
	RSD Match	Acetanilide	ok
	RSD Match	Acetophenone	ok
	RSD Match	Propiophenone	ok
	Rel.Max at	Acetanilide	ok
	Rel.Max at	Acetophenone	ok
	Rel.Max at	Propiophenone	ok

Test Result: ***Passed***

เอกสารไม่ควบคุม

ThermoFisher SCIENTIFIC

Chromeleon Operational Qualification, Part 3

System Suitability Test: Comparison with Expected Results

Variable Category	Report Variable	Status
System Suitability Test Case	Number	ok
	Name	ok
	Inj.Condition	ok
	Eval. Formula	ok
	Operator	ok
	Statistics	ok
	Rounding	ok
	MinimumNumberOfInjections	ok
	MaximumNumberOfInjections	ok
	Channel	ok
	Peak	ok
	Ref. Value Formula 1	ok
	Ref. Value Formula 2	ok
	N.A.	ok
System Suitability Test Case Result	Inj. Eval. Result	ok
	Eval. Result	ok
	Peak Result	ok
	Injection Condition Result	ok
	Ref. Value 1	ok
	Ref. Value 2	ok
	Result	ok
	Message	ok
	Average	ok
	Count	ok
	Maximum	ok
	Minimum	ok
	Range	ok
	Rel. Range	ok
	Rel. Std. Dev.	ok
	Std. Dev.	ok
	Sum	ok

Test Result: ***Passed***

เอกสารไม่ควบคุม

PQ

Performance Qualification

เอกสารไม่ควบคุม

Service Details

ThermoFisher SCIENTIFIC

System Repeatability OQ Autosampler AS-DV 1 Test 1	PASSED
Carryover OQ Autosampler AS-DV 1 Test 1	PASSED
Flow Rate Repeatability OQ Pump Inuvion Core 1 Test 1	PASSED
Noise Drift OQ Detector (Inuvion CD) Conductivity Detector 1 Test 1	PASSED
Detector Linearity OQ Detector (Inuvion CD) Conductivity Detector 1 Test 1	PASSED
Oven Temperature Accuracy OQ Column Compartment Inuvion Core 1 Test 1	PASSED
Service Review and Completion	PASSED

เอกสารไม่ควบคุม

Service Summary

ThermoFisher SCIENTIFIC

These IQOQ Results should be reviewed by the Customer. If the IQOQ is accepted, both the Customer and the Service Representative should sign the IQOQ Results, below.

IQOQ Results

Based upon the actual results obtained, this IQOQ **PASSED** the acceptance criteria described in the Installation Qualification and Operational Qualification procedure.

Service Representative

A Field Service Representative signature below confirms the completion of all aspects of the Installation Qualification and Operational Qualification and have concluded that the system has been successfully verified to be operating as required.

Customer

A Customer signature below confirms the completion of all aspects of the Installation Qualification and Operational Qualification have been completed and that the system has been successfully verified to be operating as required.

ARCHEMICA
บริษัท อาร์เคมีก้า อินเตอร์เนชั่นแนล จำกัด
ARCHEMICA INTERNATIONAL CO.,LTD.

Thermo Representative			
Signature:		Date:	19/3/26
Customer			
Signature:		Date:	19/3/26

เอกสารไม่ควบคุม

Test Equipment and Standards

ThermoFisher SCIENTIFIC

Test Equipment

Equipment	Manufacturer	Model	Serial Number	Cal Ver Date	Good Until
Multimeter	FLUKE	289	59270015	19 Dec 2025	19 Dec 2026
Thermocouple	FLUKE	K Type	59270015	22 Dec 2025	22 Dec 2026

Test Standards and Solvents

Description	Manufacturer	Conc. / Grade	Part Number	Lot Number	Expiration Date
Nitrate	Thermo Scientific	5 ppm	060254	250414	Apr 2026
Nitrate	Thermo Scientific	10 ppm	060254	250414	Apr 2026
Nitrate	Thermo Scientific	25 ppm	060254	250414	Apr 2026
Nitrate	Thermo Scientific	50 ppm	060254	250414	Apr 2026
Nitrate	Thermo Scientific	100 ppm	060254	250414	Apr 2026
Nitrate	Thermo Scientific	1000 ppm	060254	250414	Apr 2026

เอกสารไม่ควบคุม

Autosampler AS-DV 1

ThermoFisher SCIENTIFIC

Autosampler Information

Autosampler Model	AS-DV
Serial Number	25027024
Firmware Version	
Instrument Assigned	Instrument 1
Tray Type	10.0 mL Vials
Syringe Volume	N/A
Loop Volume	25 µL
Connection	USB
Powered On Successfully?	Yes

เอกสารไม่ควบคุม

Carryover OQ Autosampler AS-DV 1 Test 1

ThermoFisher SCIENTIFIC

System Information

Model	AS-DV	Acquisition Date	19/3/26
Serial Number	25027024	Sequence	OQ_IC_IVN_ASDV_CD
System Name	Inuvion_Anion		
Test Configuration	Default		

Data Entry Mode

Data Entry Mode	Import

Peak Results

	Sample Name	Injection Volume (uL)	Retention Time (min)	Area (µS*min)
Blank	Reference Blank	25	0.5033	0.006
High	High Standard	25	0.5017	58.096
Carryover	Carryover	25	0.4983	0.009

Carryover Area Results

Test	Measured	OQ Limit	Result
Carryover Area Result	0.01 %	≤ 0.10 %	PASSED

เอกสารไม่ควบคุม

System Repeatability OQ Autosampler AS-DV 1 Test 1

ThermoFisher SCIENTIFIC

System Information

Model	AS-DV	Acquisition Date	19/3/26
Serial Number	25027024	Sequence	OQ_IC_IVN_ASDV_CD
System Name	Inuvion_Anion		
Test Configuration	Default		

Data Entry Mode

Data Entry Mode	Import

Peak Results

Sample Name	Injection Volume (uL)	Retention Time (min)	Area (µS*min)
Repeatability 01	25	0.5017	3.048
Repeatability 02	25	0.5017	3.066
Repeatability 03	25	0.5017	3.063
Repeatability 04	25	0.5	3.08
Repeatability 05	25	0.5	3.08
Repeatability 06	25	0.5017	3.084

Repeatability Results

Test	Measured	OQ Limit	Result
Retention Time Result	0.2 % RSD	≤ 5.0 % RSD	PASSED
Area Result	0.4 % RSD	≤ 1.0 % RSD	PASSED

เอกสารไม่ควบคุม

Pump Inuvion Core 1

ThermoFisher SCIENTIFIC

Pump Information

Pump Model	Inuvion Core
Serial Number	250451070
Firmware Version	
Pump Position	Single Unit
Seal Type	N/A
Pressure Units	psi
Connection	USB
Powered On Successfully?	Yes

เอกสารไม่ควบคุม

Flow Rate Repeatability OQ Pump Inuvion Core 1 Test 1

ThermoFisher SCIENTIFIC

System Information

Model	Inuvion Core	Acquisition Date	19/3/26
Serial Number	250451070	Sequence	OQ_IC_IVN_ASDV_CD
System Name	Inuvion_Anion	Pump Position	Single Unit
Test Configuration	Default		

Data Entry Mode

Data Entry Mode	Import

Peak Results

Sample Name	Injection Volume (uL)	Retention Time (min)
Repeatability 01	25	0.5017
Repeatability 02	25	0.5017
Repeatability 03	25	0.5017
Repeatability 04	25	0.5
Repeatability 05	25	0.5
Repeatability 06	25	0.5017


Repeatability Results

Test	Measured	OQ Limit	Result
Retention Time Result	0.2 % RSD	≤ 5.0 % RSD	PASSED

เอกสารไม่ควบคุม

Noise Drift OQ Detector (Inuvion CD) Conductivity Detector 1 Test 1

ThermoFisher SCIENTIFIC

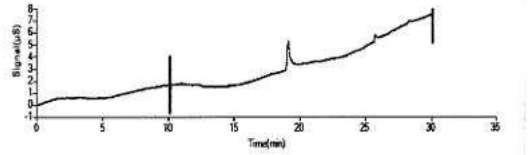

System Information

Model	Inuvion CD	Acquisition Date	19/3/26
Serial Number	250452051	Sequence	OQ_IC_IVN_ASDV_CD
System Name	Inuvion_Anion		
Test Configuration	Default		

Data Entry Mode

Data Entry Mode	Import

Noise Drift Results

Test	Measured	OQ Limit	Result	Conversion Factor
Noise Result	0.3 nS	≤ 2.0 nS	PASSED	1000
Drift Result	18.7 nS/hr	≤ 20.0 nS/hr	PASSED	1000

เอกสารไม่ควบคุม

Detector (Inuvion CD) Conductivity Detector 1

ThermoFisher SCIENTIFIC


Detector Information

Detector Model	Inuvion CD
Serial Number	250452051
Powered On Successfully?	Yes

เอกสารไม่ควบคุม

Detector Linearity OQ Detector (Inuvion CD) Conductivity Detector 1 Test 1

ThermoFisher SCIENTIFIC

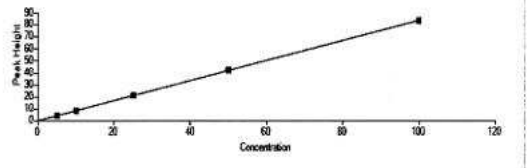

System Information

Model	Inuvion CD	Acquisition Date	19/3/26
Serial Number	250452051	Sequence	OQ_IC_IVN_ASDV_CD
System Name	Inuvion_Anion		
Test Configuration	Default		

Data Entry Mode

Data Entry Mode	Import

Peak Results

Sample Name	Concentration (ppm)	Peak Height (uS)	Calculated
IC Detector Linearity 01	5	4.522	4.782503
IC Detector Linearity 02	10	8.769	9.884257
IC Detector Linearity 03	25	21.525	25.207537
IC Detector Linearity 04	50	42.422	50.310279
IC Detector Linearity 05	100	83.633	99.815428

Linearity Results

Test	Measured	OQ Limit	Result
R^2	1.000	≥ 0.999	PASSED

เอกสารไม่ควบคุม

Column Compartment Inuvion Core 1

ThermoFisher SCIENTIFIC

Compartment Information

Compartment Model	Inuvion Core
Serial Number	250451070
Firmware Version	
Active Preheater?	N/A
Post Column Cooler?	N/A
Powered On Successfully?	Yes

เอกสารไม่ควบคุม

ThermoFisher SCIENTIFIC

Certificate of Analysis

Dionex Nitrate OQ/PQ IC Standards Kit
(Set of 6)

Product Number 060254
Certificate of Analysis

Lot Number 250414

Expiration of Certification
April 2026

The Dionex Nitrate Standard was developed to aid the analysis of anions by Ion Chromatography (IC). The single-ion standard was prepared by the dissolution of high-purity salt in ≥18.2 megohm deionized water, which was tested by IC for ionic contaminants. The bottle label states the nominal concentration value of the ionic component for informational purposes only. The actual ion concentration value was determined by Ion Chromatography. The IC system was standardized using the National Institute of Standards & Technology (NIST), Standard Reference Material, SRM 3185 (Nitrate Standard Solution). Actual concentration values determined for the single-ion is listed below.

Dionex Nitrate Standard

Vial #	Concentration (mg/L)	
1	5.10	± 0.03
2	10.15	± 0.04
3	25.49	± 0.05
4	50.03	± 0.06
5	99.7	± 0.3
6	993	± 18

ARCHEMICA
บริษัท อาร์เคมิก้า อินเทอร์เนชั่นแนล จำกัด
ARCHEMICA INTERNATIONAL CO.,LTD.
19/3/26

The concentration value is based a proven reliable method of analysis. The estimated uncertainties are two standard deviations of the concentration value. The concentration value is warranted to be stable for one year from the date of manufacture.

The preparation and analyses of the Dionex Nitrate Standard was performed with extreme care by Thermo Scientific Corporation Consumables Manufacturing Department in Sunnyvale California.

Document No. 078690-01 20-Dec-2011

Learn more at thermofisher.com/documents

Research Use Only. Not for Clinical, Patient or Diagnostic Use. © 2024 Thermo Fisher Scientific Inc. All rights reserved. All trademarks are the property of Thermo Fisher Scientific and its subsidiaries unless otherwise specified. This information is presented as an example of the capabilities of Thermo Fisher Scientific products. It is not intended to encourage use of these products in any manner that might infringe the intellectual property rights of others. Specifications, terms and pricing are subject to change. Not all products are available in all countries. Please consult your local sales representative for details. COA 80-031318-B

thermoscientific

เอกสารไม่ควบคุม

SYSTRONICS INSLAB COMPANY LIMITED
18/11-12, Sukhumvit Rd., Nernphra, Muang Rayong, Rayong 21150, Thailand
Tel.+66(38) 694 145-8, Email : calibration@systronics.co.th

ilac-MRA

CERTIFICATE OF CALIBRATION

Certificate No. TL250437
Page. 2 of 2

Result of Calibration :

(Without Adjustment)

Sensor of UUC* : Thermocouple Wire Type : K Serial No.: - ID/Tag No.: 59270015
Dimension : Length : 930 mm Diameter : 1.5 mm

Immersion Depth	Standard Reading	UUC* Reading	Correction Value	Uncertainty of Measurement (±)	Coverage Factor
mm	°C	°C	°C	°C	k =
150	-0.0039	0.6	-0.6	0.50	2.00
150	50.0050	50.3	-0.3	0.50	2.00
150	99.9944	100.3	-0.3	0.50	2.00

UUC* : Unit Under Calibration

END OF CERTIFICATE

ARCHEMICA
บริษัท อาร์เคมิก้า อินเทอร์เนชั่นแนล จำกัด
ARCHEMICA INTERNATIONAL CO.,LTD.
19/3/26

เอกสารไม่ควบคุม

ThermoFisher SCIENTIFIC

Certificate of Completion

This certifies that

Itsaraphap Bumrungjeam

Has successfully completed

eLearn: RPG IC-Specific Qualification Service Training

Issued electronically and approved by:

Thermo Fisher University LMS
Certification Management and Compliance Group
tmc.training@thermofisher.com

ARCHEMICA
บริษัท อาร์เคมิก้า อินเทอร์เนชั่นแนล จำกัด
ARCHEMICA INTERNATIONAL CO.,LTD.
19/3/26

Valid for 3 years from:

Nov/25/2025

Disclaimer: This certificate is only valid during employment with the Thermo Fisher Scientific including its subsidiaries and certified contractors.

The world leader in serving science

เอกสารไม่ควบคุม

FOSS

FOSS South East Asia
3388 Sirinrat Building, 25th – 26th Floor, Unit No. 3388/90,
Rama IV Road, Klongton , Klongtoey, Bangkok, Thailand 10110

Customer Service Report

Report No.:	13854		
Date:	24 February 2025	Customer:	UAE
Job No.:	11735	Address:	BANGKOK
Instrument:	KT810	Serial:	91889052

	Travel To Customer (Hrs)		Labour (Hrs)		Travel From Customer (Hrs)	
Start	07:00	2hrs	09:00-12:00 / 13:00-14:00	5hrs	15:00	
Finish	09:00				17:00	

Job Type							
Application		Special		Standard			
Distributor		Courtesy Visit		Installation		Training	
Digital Service		PMA Onboarding		Quote		In House	
Internal		Warranty		Repair		PM	X
Investigate		Sales Support		Remote		Health Check Visit	

PMA Type						
	Smartcare		Smartcare Pro		Fosscare	X
	Smartcare Advance		Fosscare Pro		N/A	

Details of Work / Test

A-PM KT800 12Mo

- test before PM
- Cleaning KT800, 36 Mo replace
- flushing Alkali pump
- test operation
  - Dilution 80 - 80 mL
  - Distillation 6 min 150 - 170 mL
  - Alkali 50 - 80 mL
  - all pass

Instrument Ready for Use	OK	X	Not OK*	

Part No:	Batch	Description	Qty
60031810	08.01.2024	FOSS PM Kit KT800 1200 36Mo	1

I confirm this report is accurate and complete

Signed FOSS		Signed Customer	Supharkorn P.
Name		Name	
Email:		Customer Contact.:	

*Remark:

Please scan QR code

เอกสารไม่ควบคุม

2008 ซอยสุขุมวิท 36 แขวงพระโขนงใต้ เขตวัฒนา กรุงเทพมหานคร 10110
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel. +66(0) 2424 6666 Fax. +66(0) 2424 6565

nfi สถาบันอาหาร กระทรวงอุตสาหกรรม
กรมส่งเสริมอุตสาหกรรม
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

ilac-MRA

NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Report

Certificate No.: 2502229-006-01

Equipment: CHAMBER (Incubator)
Model: KB 400 Serial No.: 20200000015535
Resolution: 0.1 °C ID No.: UAE.MIC.018/2564
Manufacturer: BINDER

Date of Calibration: 19 March 2025

Location: LABORATORY, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.

Environment Condition:
Ambient Temperature (18 ± 1) °C
Relative Humidity (50 ± 5) %
Line Voltage (223 ± 3) Volt

Condition of this results of Calibration:

1. This instrument was calibrated by insert 13 standard thermometer into its chamber and calibration according to W-TE-014 Based on TLAS G-20-1/02-08 (E): Guidelines for Calibration and Checks of Temperature Controlled Enclosures.
   - The temperature scale used was based on ITS - 90.
   - All data show below were final values and the initial data may be obtained upon request.
2. Reference Standard Instrument :

Instrument	Model	Serial No./ID No.	Certificate No.	Due Date	Through
Digital Thermometer with sensor	34972A	MY49016851	TE 670477-01	4 May 2025	NATIONAL FOOD INSTITUTE
	RTD	C=420; 303 / RTD=200; 303			

3. This certificate is traceable to International System of Units (SI Units).
4. This certificate was certified only for the instrument we calibrated.
5. This result of calibration was found accurate as shown on date and place of calibration only.
6. Condition of Calibrated item : Good
   UUC Description :
   Time of Record 1 Hour 9 Minute At 35.0 °C
   Fresh air Damper [ ] Open Position [ ]
   [X] Close Fan [ ]
   [ ] Not Available
7. Result of Calibration : [X] Without adjustment [ ] After adjustment

P. Jaenghanlit
25 March 2025

F-CS-012 Revision: 01 Date: 20-04-65

เอกสารไม่ควบคุม

2008 ซอยสุขุมวิท 36 แขวงพระโขนงใต้ เขตวัฒนา กรุงเทพมหานคร 10110
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel. +66(0) 2424 6666 Fax. +66(0) 2424 6565

nfi สถาบันอาหาร กระทรวงอุตสาหกรรม
กรมส่งเสริมอุตสาหกรรม
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

ilac-MRA

NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Certificate

Certificate No.: 2502229-006-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakhanong, Bangkok 10260

Equipment: CHAMBER (Incubator)
Manufacturer: BINDER
Model: KB 400
Serial No.: 20200000015535
ID No.: UAE.MIC.018/2564
Order No.: 2502229
Operation No.: 2502229-006
Date of Receipt: 19 March 2025
Date of Calibration: 19 March 2025

Calibrated by Mr.Jerawut Prapawuttipong
Scientist

Approved by (Mr.Pheraphat Tuanjit) (for)
Manager, Division of Calibration Laboratory
Responsible for the Technical Management Team

Date of Issue: 25 March 2025

The uncertainties are for a confidence probability of approximately 95 %.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65

เอกสารไม่ควบคุม

2008 ซอยสุขุมวิท 36 แขวงพระโขนงใต้ เขตวัฒนา กรุงเทพมหานคร 10110
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel. +66(0) 2424 6666 Fax. +66(0) 2424 6565

nfi สถาบันอาหาร กระทรวงอุตสาหกรรม
กรมส่งเสริมอุตสาหกรรม
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

ilac-MRA

NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Report

Certificate No.: 2502229-006-01

Equipment: CHAMBER (Incubator)
Model: KB 400 Serial No.: 20200000015535
Resolution: 0.1 °C ID No.: UAE.MIC.018/2564
Manufacturer: BINDER

Date of Calibration: 19 March 2025

Calibration point: 35.0 °C

Calibration result:

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
MIN	17.1	45	220.0
MAX	18.1	55	225.0




Table1 : Reporting of Temperature

Calibration point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.13 is REF)													Uncertainty ± (°C)
	# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9	# 10	# 11	# 12	# 13	
35.0	34.98	35.17	34.99	34.92	35.16	35.01	35.00	35.12	35.00	34.96	35.02	35.17	35.04	0.27

Table 2 : Reporting of Characterization Result

UUC* Setting (°C)	UUC* Reading (°C)			Temperature Stability ± (°C)	Temperature Uniformity (°C)	Overall Variation (°C)
	MIN	MAX	Average			
35.0	35.0	35.0	35.0	0.029	0.15	0.30

Note The quoted uncertainty include " Stability " and " Loading effect (20% of Temp Uniformity) "
UUC* = Unit Under Calibration
Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.
Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
Overall Variation = The difference of the maximum and minimum measured temperatures throughout observation time.
The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2, providing a level of confidence of approximately 95 %.

--------- End ---------

P. Jaenghanlit
25 March 2025

F-CS-012 Revision: 01 Date: 20-04-65

เอกสารไม่ควบคุม

2008 ซอยสุขุมวิท 36 แขวงพระโขนงใต้ เขตวัฒนา กรุงเทพมหานคร 10110
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel. +66(0) 2424 6666 Fax. +66(0) 2424 6565

United Analyst and Engineering Consultant Co., Ltd.

Automatic Mercury Analyzer

Model : RA-4500

Preventive Maintenance Report

SERIAL No. RA-4500	:	11780278
Soft version	:	Ver 2.0.5
ROM version	:	Ver 2.0.2
DATE	:	02 JULY 2025
DUE DATE	:	02 JULY 2026

INSPECTED BY : Natthaphong P.
(Natthaphong P.)

APPROVED BY :
(Kitichai S.)

Kinetic Solutions Company Limited.
2, Soi Lat Krabang 1, Lat Krabang Subdistrict,
Lat Krabang District, Bangkok 10520
Tel. (+66) 062-789-5221

เอกสารไม่ควบคุม

Inspection details

Remark	
1. Cleaning Mercury Analyzer RA-4500	
- Body case, Cell Detector, Table of Sample	
2. Replace consumable one year set for RA-4500	
3. Checking Mercury Analyzer RA-4500	
- Mercury Lamp	- Outlet Activated Carbon Filter
- Membrane Filter	- Flow Sensor
- Main Pump Tube	- Valves
- Motor Pump	- Heater
- Motor Reagent pump	- Cooling Fan
- Motor of Arm	- Stirrer motor
- Motor of Table	- Color sersor
- Motor of Lift	- Instrument Performance
4. Adjust Optical system	
5. Inspection Calibration curve and Repeatability of Mercury Analyzer RA-4500	
หมายเหตุ Heater Box เริ่มเสื่อมสภาพ แนะนำให้เปลี่ยนในรอบ PM ถัดไป	

เอกสารไม่ควบคุม

Inspection

ITEMS		SPECIFICATIONS	RESULT	JUDGE
1. Quantity	-	Accessories are completed.	GOOD	OK
2. Appearance	2.1 Overall Appearance	No visible damage.	GOOD	OK
	2.2 Parts / Cables	Correctly placed and connected.	GOOD	
3. Indication	Nameplate / Label	Plate and Label are indicated.	GOOD	OK
4. Self check				
4.1 GLP Counter	Mercury Lamp	5000 hours	110 hr	OK
	Membrane Filter	2000 hours or 1 year after replace	< 1 hr	OK
	Main Pump Tube	750 hours or 1 year after replace	< 1 hr	OK
	Absorbed Hg	1500 mg	< 1 hr	OK
	P1 Tube	2000 hours or 1 year after replace	< 1 hr	OK
	P2 Tube	2000 hours or 1 year after replace	< 1 hr	OK
	P3 Tube	2000 hours or 1 year after replace	< 1 hr	OK
	P4 Tube	2000 hours or 1 year after replace	< 1 hr	OK
	P5 Tube	2000 hours or 1 year after replace	< 1 hr	OK
	P6 Tube	2000 hours or 1 year after replace	< 1 hr	OK
	P7 Tube	2000 hours or 1 year after replace	< 1 hr	OK
	Heater	2000 hours	42 hr	OK
4.2 Check/Test	Flow rate Adjustment	Flow rate 0.14 - 0.20 L/min	0.18 L/min	OK
	Signals Detector	V.SIG is 3.5 - 4.5 V.	4.03 V.	OK
		V.REF is 3.5 - 4.5 V.	4.03 V.	OK
	Cooling Fan	Check the operation of cooling fan	PASS	OK
	Color Sensor	signals (R,G,B) at least one nonzero	PASS	OK
	Radiation Thermometer	a positive valve form thermometer	PASS	OK
	Heater	heater temp rises 4 °C within 5 min.	PASS	OK
5. Heater	Temperature	At 95°C ± 2°C with 30 min.	94.7°C	OK
6. Calibration Curve	no pretreatment	0-10ng : Max.Dev. 5.0%	0.90%	OK
7. Repeatability	100 µg/L (n=5)	Average: 100 ± 5 µg/L	101.4 µg/L	OK
		C.V. ≤ 5.0%	0.71%	OK
8. Blank	no pretreatment	Less than 0.5 (AREA)	0.103 AREA	OK

Apparatus

NAME	Date Certified	Expiration
Mercury ICP Standard (1000 µg/mL) AccuStandard, Inc. Lot 223035027	March 10, 2023	March 10, 2028


เอกสารไม่ควบคุม

Title : Preventive Maintanance
Date : 02/07/2025
Name : Kinetic Solutions
Memo : Calibration curve 0-10ng

Method


Method1 (Pretreatment:without)
(1+1)H2SO4 : 0.9mL
10w/v% SnCl2 : 0.5mL
Measurement Time(sec) : 120sec

Calib



STD

No.	STD [ug/L]	SVOL [mL]	CVOL [mL]	DVOL [mL]	STD [ng]	AREA [ON]	MEAS [ng]	Dev [%]	Note
1	0.000	5.000	5.000	5.000	0.000	0.1107	0.0000	-	
2	100.000	0.025	5.000	5.000	2.500	3.2690	2.4250	3.0	
3	100.000	0.050	5.000	5.000	5.000	6.5434	4.9392	1.2	
4	100.000	0.075	5.000	5.000	7.500	9.8649	7.4895	0.1	
5	100.000	0.100	5.000	5.000	10.000	13.2088	10.0570	0.6	

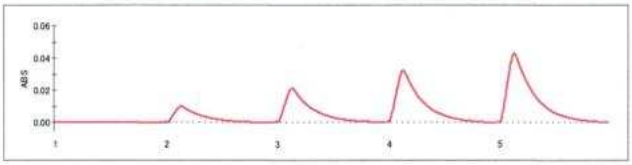

SMP


No.	NAME	SVOL [mL]	CVOL [mL]	DVOL [mL]	AREA [ON]	MEAS [ng]	CONC [ug/L]	Note
1	STD 100 ppb	0.050	5.000	5.000	6.7338	5.0854	101.708	
2	STD 100 ppb	0.050	5.000	5.000	6.7129	5.0693	101.386	
3	STD 100 ppb	0.050	5.000	5.000	6.6370	5.0110	100.220	
4	STD 100 ppb	0.050	5.000	5.000	6.7489	5.0970	101.940	
5	STD 100 ppb	0.050	5.000	5.000	6.7514	5.0989	101.978	
6	Blank	5.000	5.000	5.000	0.1035	-0.0055	0.000	

Statistics

No.	NAME	TRY	AV [ug/L]	SD [ug/L]	Cv [%]
1	STD 100 ppb	5	101.4464	0.724979	0.71

เอกสารไม่ควบคุม

NIC NIPPON INSTRUMENTS CORPORATION

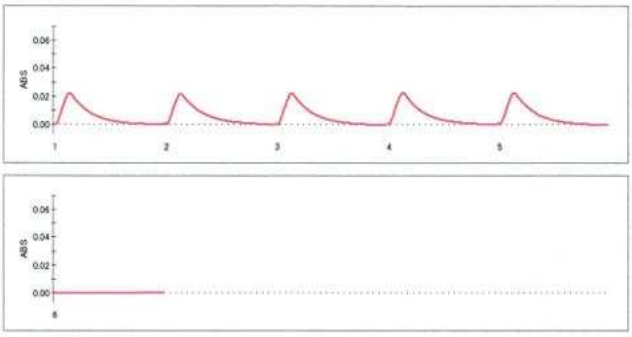

Self Check

```
Heat check:PASS!! ( 25.7degC[05:00] ->  29.7degC[02:29])
Sensor check:PASS!! ( 253~  15= 238)
Leak check:PASS!! (0.18L/min)
Sig/Ref check:PASS!! (Sig:4.03V, Ref:4.03V)
Drift check:PASS!! ( 0.0000037 - -0.0000026 =  0.0000063)
```


1. **Quality Standards:**
   ISO 17034:2016 – General Requirements for the Competence of Reference Material Producers
   ISO/IEC 17025:2017 – General Requirements for the Competence of Testing And Calibration Laboratories
   ISO 9001:2015 – Quality Management System – Requirements Eagle Registrations
2. **Intended Use:** The product covered by this certificate is designed for calibration or for use in quality control procedures for the specified chemical compounds listed on the reverse side. This product can be used for quantification and/or identification. This product can also be used as a reference material to validate analytical procedures, subject to the conditions under Section 7.
3. **Manufacturing:** All balances are calibrated daily using an in-house procedure with weights that are compared annually to master weights and traceable to NIST. The balances are also calibrated annually by an ISO/IEC 17025 accredited calibration laboratory. Please refer to the NIST test number listed on the front of this certificate. Class A glassware is used in the manufacture and quality control of all standards. Good Laboratory Practices have been used throughout the preparation of this Standard.
4. **Homogeneity:** This product is sufficiently homogeneous and any sample size would be within the uncertainty budget.
5. **Stability:** The manufacturer guarantees the stability of this solution through the expiration date stated on the label, when handled and stored according to the conditions stated on the label
6. **Uncertainty:** The uncertainty values as stated on the face of this certificate have been determined using the EURACHEM/CITAC Guide. We report a combined expanded uncertainty equal to the positive square root of the total variance of the uncertainty of the components using the following formula: $u_c = \sqrt{(u(V))^2 + (u(m))^2 + (u(V))^2 + (u(RO))^2}$ This formula represents uncertainty components from the mass, volume, short-term stability, long-term stability and homogeneity factors associated with the production of this product. The expanded uncertainty, assumes a normal distribution and a coverage factor of $k=2$ is chosen using approximately a 95% confidence level.
7. **Legal Notice and Limit of Liability:** This product is for routine laboratory analysis and research purposes only. The company's liability will be limited to replacement of product or refund of purchase price. Notice of claims must be made within thirty (30) days from date of delivery.

เอกสารไม่ควบคุม

NIPPON INSTRUMENTS CORPORATION

เอกสารไม่ควบคุม

125 Market Street
New Haven, CT 06513
USA

Tel (203)786-5290
Fax (203)786-5287
www.AccuStandard.com

AccuStandard® Inc.

CERTIFICATE OF ANALYSIS

AccuTrace™ Reference Standard

Catalog No: ICP-34N-1
Description: Mercury ICP Standard
Element: Mercury (Hg)
SRM: 3133
Lot: 223035027
Matrix: 10% Nitric acid
Hazards: *Refer to SDS for complete safety information*

Date Certified: Mar 10, 2023
Expiration: Mar 10, 2028
Density: 1.052 g/mL
Sample Size: 100 mL
Components: 1
Storage Condition: Ambient (>5 °C)

Signal Word: Danger

Certified Reference Material

ANAB AR-1463 ISO/IEC 17025

Certified Concentration: 1000 µg/mL

Trace Elements in µg/mL

Ag nd<0.02	Ce nd<0.2	Gd nd<0.02	Lu nd<0.02	Pb nd<0.2	Sc nd<0.02	Ti nd<0.02
Al nd<0.02	Co nd<0.02	Ge nd<0.2	Mg nd<0.02	Pd nd<0.2	Se nd<0.2	Tl nd<0.2
As nd<0.2	Cr nd<0.02	Hf nd<0.02	Mn nd<0.02	Pr nd<0.2	Si N/A	Tm nd<0.02
Au nd<0.02	Cs N/A	Hg *	Mo nd<0.02	Pt nd<0.2	Sm nd<0.2	U nd<0.2
B nd<0.2	Cu nd<0.02	Ho nd<0.02	Na nd<0.02	Rb N/A	Sn nd<0.02	V nd<0.02
Ba nd<0.02	Dy nd<0.02	In nd<0.2	Nb nd<0.2	Re nd<0.2	Sr nd<0.02	W nd<0.2
Be nd<0.02	Er nd<0.02	Ir nd<0.2	Nd nd<0.02	Rh nd<0.2	Ta nd<0.2	Y nd<0.02
Bi nd<0.2	Eu nd<0.02	K nd<0.2	Ni nd<0.02	Ru nd<0.02	Tb nd<0.02	Yb nd<0.02
Ca nd<0.02	Fe nd<0.02	La nd<0.02	Os N/A	S N/A	Te nd<0.2	Zn nd<0.02
Cd nd<0.02	Ga nd<0.02	Li nd<0.02	P N/A	Sb nd<0.2	Th nd<0.02	Zr nd<0.02

This Certified Reference Material was verified in accordance with ISO/IEC 17025 (AT-1339) and ISO 17034 (AR-1463).
This solution was assayed gravimetrically, using a balance calibrated against weight sets, ID #88270, traceable to NIST.
A product with a suffix (-1A, -2B, etc. or -01, -02, etc.) on its lot number has had its expiration date extended and is identical to the same lot number without the suffix.
This product contains mercury and MUST be disposed of in accordance with all federal, state and local regulations.
The gravimetric uncertainty for this product is ±0.24%. The CRM uncertainty is ±2.4%.
In order to verify the concentration(s), the final solution was checked by plasma emission spectroscopy (ICP) against material traceable to the above listed NIST SRM(s).
We use the highest purity raw materials available to minimize impurity levels in the final solution. Typically 99.999%+ pure starting materials are used as well as high purity acids and ASTM Type I 18 megohm deionized water.
All trace level elemental impurities were determined via plasma emission spectroscopy on the concentrate.
All weights are traceable through NIST. Test No. 684/291344-18 & 684/292805-19
All glassware used in preparation is Class A.
All bottles are acid leached and triple rinsed with deionized water prior to use.
Shake bottle prior to use and do not pipette directly out of the bottle. Use only cleaned Class A volumetric glassware. Keep bottle tightly capped.

Certified By: Megan O'Leary, Inorganic QC Manager

For use in routine laboratory analysis.

AccuStandard is accredited to ISO 17034, ISO/IEC 17025 and certified to ISO 9001:2015

เอกสารไม่ควบคุม

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

Certificate of Calibration

Cert.No.: 25CH1053
Page.: 1 of 2

Equipment :	Turbidity Meter
Manufacturer :	Oakton
Model :	T100IR
Serial No. :	1120501017
ID. No. :	UAE.WAT.056/2563
Condition As-Received:	Used Item
Received Date :	05 September 2025
Calibration Date :	08 September 2025
Reference :	2509-0212DSC-1
Submitted by :	United Analyst and Engineering Consultant Co.,Ltd. 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Ambient Temperature :	(23 ± 3.0) °C
Relative Humidity :	(50 ± 20) %
Calibration Procedure :	In - house method : CP-CH11 Direct measurement by using Formazin standard solution
Calibrated by :	Walalak Sirithean
Approved by :	Approved Signatory

( ) Chakrit Waewwanjua
( ) Ponpan Palpim
(✓) Saithip Meangmai

Issue Date : 9 September 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Calibration and Testing Equipment Services.

เอกสารไม่ควบคุม

Condition of this calibration result

1. Reference Standard Instruments :

Instruments	ID No.	Certificate No.	Due date
1) Data Logger	130EC012	24H2043	23 Sep 2025
2) Liquid-in Glass Thermometer	130RC003	25I440	16 Apr 2026

- This measurement result is traceable to SI through Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials : Turbidity Standard solution (Formzin)
- The measurement results are traceable to SI through CPA chem Ltd.,

Turbidity Solution	Manufacturer	Lot No.	Exp. date
20.0 NTU	CPA Chem	1088008	18 Mar 2026
100.0 NTU	CPA Chem	1088007	18 Mar 2026
400 NTU	CPA Chem	1088018	18 Mar 2026
800 NTU	CPA Chem	1088017	18 Mar 2026

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration result

Performing five - Formazin suspension standard curve by using 0, 20, 100, 400, 800 NTU
Tubidity Meter serial number : 1120501017

Standard Formazine suspension (NTU)	UUC* Reading (NTU)	Uncertainty of Measurement (± NTU)	Coverage Factor k
0	0.00	0.026	2.00
20.0	20.2	0.20	2.00
100.0	100	1.2	2.00
400	403	2.4	2.00
800	799	4.3	2.00

Remark - UUC* = Unit Under Calibration
- NTU = Nephelometric Turbidity Units

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม

United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel.0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

Equipment: Electronic Balance
Manufacturer: Mettler Toledo
Model: AB204-S/FACT
Readability: 0.0001 g
Serial No.: 1129361010
ID No.: UAE.WAS.002/2552
Max. Capacity: 220 g
Calibration Date: April 23, 2025
Condition As-Received: In Condition

Condition of Equipment:

Condition of This Result of Calibration:

1. Calibration Method: This instrument was calibrated by method UAE.CP/CAL.006 In-House Method based on UKAS Lab 14 : 2022
2. Reference Standrads:

Reference Standard:	Model	Serial No.	Calibrated By	Certificate No.	Traceability	Due Date
Standard Weight Class E2 (OIML)	1 mg to 1 kg	B786109122	AMARC	25-009359	Mettler-Toledo	21 Jan 27
Standard Weight Class F1 (OIML)	1 mg to 200 g	11119512	AMARC	24-013863	Mettler-Toledo	04-Feb-26
Instrument	**Model**	**Serial No.**	**Calibrated By**	**Certificate No.**	**Traceability**	**Due Date**
Thermo-Hygro-Baro Meter	MHB-382SD	AK46957	SUCCESS	SB-E100972/67	Success Gateway	21 Nov 25
Thermo-Hygro-Baro Meter	MHB-382SD	AK46957	TPA	25P705	TPA	25-Feb-26


3. This certification is traceable to SI Unit
4. This certification was certified only for the instrument we calibrated
5. This result of calibration was found accurate as show on date and place of calibration only.
6. Through the reference standard laboratory of AMARC 25-009359 Calibration 0152

Calibraton Result:

1. Repeatability of Reading:

Nominal Value (g)	Standard Deviation of Reading (g)
200*	0.000045

2. Eccentric or off-center loading
A mass of 100 g was placed and moved to various position on pan
The Balance reading obtained is given in the table.



1 (g)	2 (g)	3 (g)	4 (g)	5 (g)	Maximum Difference (g)
100.0000	99.9996	99.9997	100.0003	100.0005	0.0005

เอกสารไม่ควบคุม

United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel.0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

Certificate of Calibration

Customer Name: United Analyst and Engineering Consultant Co., Ltd.
Address: 3 Soi Udom suk 41, Sukhumvit Rd., Bang Chak, Phar Khanong, Bangkok 10260

Equipment: Electronic Balance
Manufacturer: Mettler Toledo
Model: AB204-S/FACT
Serial No.: 1129361010
Asset No. : UAE.WAS.002/2552
Building : N/A Floor : 1 Room : 107

Received Date: April 22, 2025
Date of Calibation : April 23, 2025
Calibration Conditions: Temperature 22.8 °C to 23.4 °C
Humidity 56.8 % to 68.9 %
Pressure 756.6 mmHg to 758.2 mmHg

Calibrated by: Sakkarin Srirahang

Approved by: Suwit Chotnok Signature:

Issued Date: April 25, 2025

Note : 1) The Uncertainties are for a confidence probability of approximately 95%
2) This Certificate is valid only to the item calibrated on date and place of calibration.
3) This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the United Analyst and Engineering Consultant Co.,Ltd. (UAE)

เอกสารไม่ควบคุม

United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel.0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

Equipment: Electronic Balance
Manufacturer: Mettler Toledo
Model: AB204-S/FACT
Readability: 0.0001 g
Serial No.: 1129361010
ID No.: UAE.WAS.002/2552
Max. Capacity: 220 g
Calibration Date: April 23, 2025

Calibraton Result: (Continued)
Calibraton Range: 0 - 200 g
Calibraton Adjustment: Internal Calibration

3. Error of indication from nominal or conventional mass value:

Nominal Value (g)	Reference Value (g)	Indication (g)	Correction (g)	Uncertainty (± mg)	Coverage Factor k
Unload	0.0000000	0.0000	0.0000	0.10	2.05
0.01	0.0100025	0.0099	0.0001	0.10	2.05
0.05	0.0500056	0.0500	0.0000	0.10	2.05
0.1	0.1000012	0.0999	0.0001	0.10	2.05
0.5	0.5000133	0.5000	0.0000	0.10	2.05
1	1.0000105	1.0000	0.0000	0.10	2.05
10	10.000010	10.0000	0.0000	0.11	2.04
40	40.000076	40.0000	0.0000	0.14	2.00
50	50.000056	50.0000	0.0001	0.13	2.00
80	80.000107	80.0000	0.0001	0.18	2.00
100	100.000109	99.9999	0.0002	0.17	2.00
120	120.00015	119.9999	0.0003	0.21	2.00
150	150.000165	149.9998	0.0003	0.24	2.00
160	160.000175	159.9997	0.0005	0.26	2.00
200	200.000129	199.9998	0.0004	0.30	2.00

4. Effect of Tare test:

Tare Load (g)	Test Load (g)	Indication (g)	Correction (g)
100	20.000041	19.9999	0.0001
	40.000076	39.9998	0.0002
	60.000066	59.9997	0.0003
	80.000107	79.9999	0.0002
	100.000168	100.0004	-0.0003

Remark:
The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k, providing a level of confidence of approximately 95%.

o—o-End-o—o

เอกสารไม่ควบคุม

สถาบันอาหาร
ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

ilac-MRA

NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Certificate

Certificate No.: 2502229-001-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakhanong, Bangkok 10260

Equipment: CHAMBER (Incubator)
Manufacturer: MEMMERT
Model: IPP 260
Serial No.: V615.0187
ID No.: UAE.MIC.003/2559
Order No.: 2502229
Operation No.: 2502229-001
Date of Receipt: 19 March 2025
Date of Calibration: 19 March 2025

Calibrated by Mr.Jerawut Prapawuttipong
Scientist

Approved by (Mr.Pheraphat Tuanjit) (for)
Manager, Division of Calibration Laboratory
Responsible for the Technical Management Team

Date of Issue: 25 March 2025

The uncertainties are for a confidence probability of approximately 95 %.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

เอกสารไม่ควบคุม

2008 ซอยอุดมสุข 36 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel. +66(0) 2422 8688 Fax +66(0) 2422 8545

สถาบันอาหาร
ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

ilac-MRA

NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Report

Certificate No.: 2502229-001-01
Equipment: CHAMBER (Incubator)
Model: IPP 260 Serial No.: V615.0187
Resolution: 0.1 °C ID No.: UAE.MIC.003/2559
Manufacturer: MEMMERT
Date of Calibration: 19 March 2025

Calibration point: 35.0 °C
Calibration result:

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
MIN	15.5	28	220.0
MAX	17.1	35	225.0



Table1 : Reporting of Temperature

Calibration point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.9 is REF)									Uncertainty ± (°C)
	# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9	
35.0	34.94	34.95	34.91	34.93	35.15	35.01	34.98	35.05	35.12	0.29

Table 2 : Reporting of Characterization Result

UUC* Setting (°C)	UUC* Reading (°C)			Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
	MIN	MAX	Average			
35.0	35.0	35.0	35.0	0.10	0.21	0.35

Note: The quoted uncertainty include " Stability " and " Loading effect (20% of Temp Uniformity) "
UUC* = Unit Under Calibration
Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.
Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
Overall Variation = The difference of the maximum and minimum measured temperatures througout observation time.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2, providing a level of confidence of approximately 95 %.

--------- End ---------

25 March 2025

เอกสารไม่ควบคุม

2008 ซอยอุดมสุข 36 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel. +66(0) 2422 8688 Fax +66(0) 2422 8545

สถาบันอาหาร
ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

ilac-MRA

NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Report

Certificate No.: 2502229-001-01
Equipment: CHAMBER (Incubator)
Model: IPP 260 Serial No.: V615.0187
Resolution: 0.1 °C ID No.: UAE.MIC.003/2559
Manufacturer: MEMMERT
Date of Calibration: 19 March 2025

Location: LABORATORY, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Environment Condition:
Ambient Temperature (16.2 ± 1) °C
Relative Humidity (32 ± 4) %
Line Voltage (223 ± 3) Volt

Condition of this results of Calibration:

1. This instrument was calibrated by insert 9 standard thermometer into its chamber and calibration according to W-TE-014 Based on TLAS G-20-1/02-08 (E): Guidelines for Calibration and Checks of Temperature Controlled Enclosures.
   - The temperature scale used was based on ITS - 90.
   - All data show below were final values and the initial data may be obtained upon request.
2. Reference Standard Instrument :

Instrument	Model	Serial No./ID No.	Certificate No.	Due Date	Through
Digital Thermometer with sensor	34972A	MY49016851	TE 670477-01	4 May 2025	NATIONAL FOOD INSTITUTE
	RTD	C-2101-109/ RTD2101-109			

3. This certificate is traceable to International System of Units (SI Units).
4. This certificate was certified only for the instrument we calibrated.
5. This result of calibration was found accurate as shown on date and place of calibration only.
6. Condition of Calibrated item : Good
   UUC Description :
   Time of Record 1 Hour 9 Minute At 35.0 °C
   Fresh air Damper [-] Open Position [-]
   [X] Close Fan [-]
   [-] Not Available
7. Result of Calibration : [X] Without adjustment [ ] After adjustment

25 March 2025

เอกสารไม่ควบคุม

2008 ซอยอุดมสุข 36 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel. +66(0) 2422 8688 Fax +66(0) 2422 8545

สถาบันอาหาร
ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

ilac-MRA

NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Certificate

Certificate No.: 2502229-006-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakhanong, Bangkok 10260

Equipment: CHAMBER (Incubator)
Manufacturer: BINDER
Model: KB 400
Serial No.: 20200000015535
ID No.: UAE.MIC.018/2564
Order No.: 2502229
Operation No.: 2502229-006
Date of Receipt: 19 March 2025
Date of Calibration: 19 March 2025

Calibrated by Mr.Jerawut Prapawuttipong
Scientist

Approved by (Mr.Pheraphat Tuanjit) (for)
Manager, Division of Calibration Laboratory
Responsible for the Technical Management Team

Date of Issue: 25 March 2025

The uncertainties are for a confidence probability of approximately 95 %.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

เอกสารไม่ควบคุม

2008 ซอยอุดมสุข 36 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel. +66(0) 2422 8688 Fax +66(0) 2422 8545

สถาบันอาหาร
กระทรวงอุตสาหกรรม
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

NSC-TISI-TIS 17025 CALIBRATION 0061

Calibration Report

Certificate No.: 2502229-006-01

Equipment: CHAMBER (Incubator)

Model: KB 400 Serial No.: 20200000015535

Resolution: 0.1 °C ID No.: UAE.MIC.018/2564

Manufacturer: BINDER

Date of Calibration: 19 March 2025 Page 2 of 3

Location: LABORATORY, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.

Environment Condition:
Ambient Temperature (18 ± 1) °C
Relative Humidity (50 ± 5) %
Line Voltage (223 ± 3) Volt

Condition of this results of Calibration:

1. This instrument was calibrated by insert 13 standard thermometer into its chamber and calibration according to W-TE-014 Based on TLAS G-20-1/02-08 (E): Guidelines for Calibration and Checks of Temperature Controlled Enclosures.
   - The temperature scale used was based on ITS - 90.
   - All data show below were final values and the initial data may be obtained upon request.
2. Reference Standard Instrument :

Instrument	Model	Serial No./ID No.	Certificate No.	Due Date	Through
Digital Thermometer with sensor	34972A	MY49015851	TE 6/0477-01	4 May 2025	NATIONAL FOOD INSTITUTE
	RTD	CH220-303 / RTD#220-303			

3. This certificate is traceable to International System of Units (SI Units).
4. This certificate was certified only for the instrument we calibrated.
5. This result of calibration was found accurate as shown on date and place of calibration only.
6. Condition of Calibrated item : Good

UUC Description :
Time of Record 1 Hour 9 Minute At 35.0 °C
Fresh air Damper - Open Position -
X Close Fan
- Not Available

7. Result of Calibration : [X] Without adjustment [ ] After adjustment

P. Jeenghobkit
25 March 2025

F-CS-012 Revision: 01 Date: 20-04-65

เอกสารไม่ควบคุม

2008 ซอยอารีมสัมพันธ์ 36 ถนนอารีมสัมพันธ์ แขวงบางกะปิ เขตห้วยขวาง กรุงเทพมหานคร 10310
2008 Soi 36, Arun Amarn Road, Bang Kapi Khan Subdistrict, Bang Phat District, Bangkok 10700, Thailand
Tel. +66(0) 2028 8688, Fax +66(0) 2028 8505

DQE Services Co.,Ltd.
DQE Services
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

NSC-TISI-TIS 17025 CALIBRATION 0494

CERTIFICATE OF CALIBRATION

Certificate No. : SP25-024 Page 1 of 5

Customer : United Analyst and Engineering Consultant Co.,Ltd. (Head Office)

Address : 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Location of calibration : Instrument room (207)

Equipment : UV-Vis Spectrophotometer

Manufacturer : HITACHI

Model : U-5100

Serial No. : 23A4-008

ID No. : UAE.WAS.010/2567

Received Date : 17 June 2025

Calibration Date : 17 June 2025

Issue Date : 20 June 2025

Condition Instrument : Good

Calibrated by : ธนุส
(Mr.Tanawut Rittidach)
Technical Manager

Approved by : ชลธิชา
(Ms.Chonticha Sangngern)
Quality Manager

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the DQE Services Co., Ltd.

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

สถาบันอาหาร
กระทรวงอุตสาหกรรม
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

NSC-TISI-TIS 17025 CALIBRATION 0061

Calibration Report

Certificate No.: 2502229-006-01

Equipment: CHAMBER (Incubator)

Model: KB 400 Serial No.: 20200000015535

Resolution: 0.1 °C ID No.: UAE.MIC.018/2564

Manufacturer: BINDER

Date of Calibration: 19 March 2025 Page 3 of 3

Calibration point: 35.0 °C

Calibration result:

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
MIN	17.1	45	220.0
MAX	18.1	55	226.0




Table1 : Reporting of Temperature

Calibration point	Measured Temperature (°C) @ Sensor No. (Sensor No.13 is REF)													Uncertainty
(°C)	# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9	# 10	# 11	# 12	# 13	± (°C)
35.0	34.98	35.17	34.99	34.92	35.18	35.01	35.00	35.12	35.00	34.96	35.02	35.17	35.04	0.27

Table 2 : Reporting of Characterization Result

UUC* Setting	UUC* Reading (°C)			Temperature Stability	Temperature Uniformity	Overall Variation
(°C)	MIN	MAX	Average	± (°C)	(°C)	(°C)
35.0	35.0	35.0	35.0	0.029	0.15	0.30

Note The quoted uncertainty include " Stability " and " Loading effect (20% of Temp Uniformity) "
UUC* = Unit Under Calibration
Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.
Uniformity = The maximum difference of measurec temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
Overall Variation = The difference of the maximum and minimum measured temperatures througout observation time.
The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2, providing a level of confidence of approximately 95 %.

---------- End ----------

P. Jeenghobkit
25 March 2025

F-CS-012 Revision: 01 Date: 20-04-65

เอกสารไม่ควบคุม

2008 ซอยอารีมสัมพันธ์ 36 ถนนอารีมสัมพันธ์ แขวงบางกะปิ เขตห้วยขวาง กรุงเทพมหานคร 10310
2008 Soi 36, Arun Amarn Road, Bang Kapi Khan Subdistrict, Bang Phat District, Bangkok 10700, Thailand
Tel. +66(0) 2028 8688, Fax +66(0) 2028 8505

DQE Services Co.,Ltd.
DQE Services
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

NSC-TISI-TIS 17025 CALIBRATION 0494

REPORT OF CALIBRATION

Certificate No. : SP25-024 Page 2 of 5

Environment Condition : Ambient Temperature 25 ± 5 °C

Relative humidity 55 ± 20 %RH

Calibration method : In-house method CP-01 Based on ASTM E275-08

Certified Reference Materials :

Material	Serial No.	Certificate No.	Due date
Absobance Standard set	25760	115663	25 October 2025
Absobance Standard set	25757	115638	25 October 2025
Wavelength Standard set	25806	115657	25 October 2025
Wavelength Standard set	25758	115665	25 October 2025

Traceability : This certification is traceable to the International System of Unit maintained at National - Institute of Standards and Technology (NIST) through Starna Scientific Limited

Spectral Band Width of UUC : 5.0 nm.

Scan Speed of UUC : 40

Scan Interval of UUC : 0.1 nm.

Resolution of UUC : Photometric 0.001 Abs.

Wavelength 0.1 nm.

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP25-024

Calibration Results : Without adjustment

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
420	0.0000	0.000	0.0000	0.0028	2.00
	0.5780	0.574	0.0040	0.0031	2.00
	1.0484	1.044	0.0044	0.0029	2.00
	2.1876	2.185	0.0026	0.0075	2.00
440	0.0000	0.000	0.0000	0.0028	2.00
	0.5595	0.558	0.0015	0.0035	2.00
	1.0239	1.021	0.0029	0.0035	2.00
	2.1230	2.122	0.0010	0.0079	2.00
465	0.0000	0.000	0.0000	0.0028	2.00
	0.5230	0.519	0.0040	0.0030	2.00
	0.9633	0.961	0.0023	0.0029	2.00
	1.9753	1.975	0.0003	0.0071	2.00
546.1	0.0000	0.000	0.0000	0.0028	2.00
	0.5181	0.515	0.0031	0.0031	2.00
	1.0002	0.996	0.0042	0.0033	2.00
	1.9973	1.994	0.0033	0.0084	2.00
590	0.0000	0.000	0.0000	0.0028	2.00
	0.5517	0.549	0.0027	0.0030	2.00
	1.0803	1.078	0.0023	0.0030	2.00
	2.0373	2.031	0.0063	0.0082	2.00
635	0.0000	0.000	0.0000	0.0028	2.00
	0.5591	0.557	0.0021	0.0031	2.00
	1.0518	1.049	0.0028	0.0030	2.00
	1.9274	1.924	0.0034	0.0081	2.00

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP25-024

Wavelength Accuracy :

CRMs Values (nm.)	UUC Reading (nm.)	Correction (nm.)	Uncertainty (nm.)	Coverage factor k
241.00	240.4	0.60	0.18	2.00
279.30	278.8	0.50	0.18	2.00
288.90	288.3	0.60	0.18	2.00
334.50	333.9	0.60	0.18	2.00
361.40	360.8	0.60	0.18	2.00
418.40	417.9	0.50	0.18	2.00
447.20	446.6	0.60	0.18	2.00
459.30	459.1	0.20	0.18	2.00
537.00	536.4	0.60	0.18	2.00
638.00	637.5	0.50	0.18	2.00
441.29	440.7	0.59	0.18	2.00
479.88	479.4	0.48	0.18	2.00
513.75	513.3	0.45	0.18	2.00
528.59	528.2	0.39	0.18	2.00
575.10	574.5	0.60	0.18	2.00
585.56	585.4	0.16	0.20	2.00
684.70	684.1	0.60	0.18	2.00
740.51	740.2	0.31	0.20	2.00
747.61	747.0	0.61	0.18	2.00
807.04	806.4	0.64	0.18	2.00
879.68	879.1	0.58	0.18	2.00

Remark : - UUC = Unit Under Calibration
- N/A = Not Avaiable
- The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%

- End of Certificate -

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP25-024

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
235	0.0000	0.000	0.0000	0.0050	2.00
	0.7469	0.747	-0.0001	0.0057	2.00
257	0.0000	0.000	0.0000	0.0050	2.00
	0.8674	0.864	0.0034	0.0059	2.00
313	0.0000	0.000	0.0000	0.0050	2.00
	0.2919	0.293	-0.0011	0.0051	2.00
350	0.0000	0.000	0.0000	0.0050	2.00
	0.6430	0.639	0.0040	0.0055	2.00

เอกสารไม่ควบคุม

Technology

DKSH

Service Report

TO	FOR
Company: United Analyst and Engineering Consultant Co., Ltd. _ Bangkok-HQ Address: 700/2 หมู่ที่ 1 Phrakhanong District, Bangkok, 10260	Work Order Number: WO-00074079 Contact: Kamphong Boonpuang Email: kamphong.b@uaeconsultant.co.th Tel: +66 2763 2828 (7021), +66 8 6347 7390

WORK ORDER INFORMATION			
Top-Level		Order Type	Preventive Maintenance
Installed Product ID	IB-00105024	Billing Type	Chargeable
Product	SKALAR 2SAN59000 SAN++ Classic CFA 230V 2SAN59000	PO No.	HPO-250400209
Serial No.	182688	Warranty No.	
		Contract No.	

PRODUCTS SERVICED		
Installed Product Id	Serial Number	Product
IB-00105024	182688	SKALAR 2SAN59000 SAN++ Classic CFA 230V 2SAN59000

PROBLEM DESCRIPTION
PM 1 ครั้งปี **ใบเสนอราคาเลขที่ Q-120095

Line Number	Engineer	Start Date And Time	End Date And Time	Billable Labor Hour	Billable Travel Hour	Travel KM
WL-00342192	Yongyuth Chanphong	05/23/2025 9:30 AM	05/23/2025 6:00 PM	8.5		
Total				8.5	0	0

! Reach us at DKSH Service-Hotline : +66 2 639 7000
2533 Sukhumvit Road, Bangchak, 10260, Phrakhanong, Bangkok, Thailand
Phone +66 2 639 7000 Fax +66 2 333 1026

Delivering Growth - in Asia and beyond

เอกสารไม่ควบคุม

Line Number	Work Description
WL-00342192	- ทำ PM เสร็จแล้ว, เครื่องพร้อมใช้งาน

PARTS CONSUMED		
Part No	Part Description	Quantity

EXPENSES			
Part No	Expense Type	Description	Line Quantity

RECOMMENDED PARTS
อะไหล่สำรองที่ควรสั่งซื้อทั้งหมด 7 รายการ คือ Pump tube 3 รายการ (SA3028, SA3032 และ SA3034), หลอดไฟ Halogen 6V/10W (90020012) 1 รายการ จำนวน 2 หลอด, Tubing polyethylene 3 รายการ (SA3142, SA5141 และ SA5142)

REMARKS

Travel Time Disclaimer:
Please note that the travel time in this report only includes time taken to reach the installed equipment location. It does not include our engineer's return travel time.

Customer Signature:

K Kanphong

Customer Signature

Technician: Yongyuth Chanphong
Job Title: Service Manager
Email: yongyuth.yc@dksh.com

Date: 06/06/2025

เอกสารไม่ควบคุม

Check with Standard

Item	Characteristic	Before	After	Remark
14	Base Line Test	☐ Pass ☐ Fail ☑ N/A	☑ Pass ☐ Fail ☐ N/A	
15	Detector Signal Test	☐ Pass ☐ Fail ☑ N/A	☑ Pass ☐ Fail ☐ N/A	

Summary of checked

☑ The instrument can work normally and efficiently. (เครื่องมือวิเคราะห์ทำงานได้ปกติและมีประสิทธิภาพ)
☐ The instrument can work but it's requiring to maintenance. (เครื่องมือวิเคราะห์ทำงานได้แต่ต้องบำรุงรักษา)
☐ The instrument could not work it's requiring to repair. (เครื่องมือวิเคราะห์ไม่สามารถทำงานได้และต้องการซ่อมบำรุง)

Remark :

* Pump tube, Tubing polyethylene และ Air tube เริ่มเสื่อมสภาพ ให้เปลี่ยนอะไหล่ทั้งหมดเพื่อความมั่นใจในการใช้งาน

หมายเหตุ แนะนำอะไหล่ที่ควรสั่งเพิ่มเติม 7 รายการ ดังนี้
1. อะไหล่ สารเคมีตรวจ Ammonia จำนวน 3 รายการ (SA3032, SA5141 และ 90020012)
2. อะไหล่ สารเคมีตรวจ Phenol และ Cyanide จำนวน 6 รายการ (SA3028, SA3034, SA3142, SA5142 และ 90020012)

Standard Equipment Used

Equipment	Equipment I.D.	
Digital multi meter	S/N 57600592	Due date : 19-Jun-2025
Thermo hygrometer	S/N 39520444/904	Due date : 27-Dec-2025

Test By : (Mr. Yongyuth Chanphong)
Position : Supervisor, Technical Service

Approved by : (Mr. Eknapong Wankliang)
Position : Manager, Technical Services

เอกสารไม่ควบคุม

Job No. WO-00074079

Test Report

Customers	United Analyst and Engineering Consultant Co., Ltd.		
Equipment	Continuous Flow Analyzer	Manufacturer	SKALAR
Controller Mdel	SAS000	Auto Sample Model	SA1052
Controller Serial No.	182688	Auto Sample Serial No.	181729
Date of test	23-May-2025	Period	12 Month
Environment temperature	24.3 °C	Humidity	54.4 %RH

Results

Instrument Checked

Item	Characteristic	Before	After	Remark
1	Visual inspect	☑ Pass ☐ Fail	☑ Pass ☐ Fail	
2	Power supply (210 - 240 VAC)	220 VAC	220 VAC	
3	Computer	☑ Pass ☐ Fail	☑ Pass ☐ Fail	
4	Program	☑ Pass ☐ Fail	☑ Pass ☐ Fail	
5	Auto sampler	☑ Pass ☐ Fail	☑ Pass ☐ Fail	
6	Module holder			
	- Motor pump	☑ Pass ☐ Fail	☑ Pass ☐ Fail	
	- Pump tube	☐ Pass ☑ Fail	☑ Pass ☐ Fail	*
	- Air-injection	☑ Pass ☐ Fail	☑ Pass ☐ Fail	*
	- Chemistry manifolds, Switching valve, Coil, Membrane	☑ Pass ☐ Fail	☑ Pass ☐ Fail	
7	Detector			
	- Filter	☑ Pass ☐ Fail	☑ Pass ☐ Fail	
	- Flow cell	☑ Pass ☐ Fail	☑ Pass ☐ Fail	
	- Lamp	☑ Pass ☐ Fail	☑ Pass ☐ Fail	
8	Interface	☑ Pass ☐ Fail	☑ Pass ☐ Fail	
9	Rinsing valves	☐ Pass ☐ Fail ☑ N/A	☐ Pass ☐ Fail ☑ N/A	
10	Temperature / Reactor	☑ Pass ☐ Fail ☐ N/A	☑ Pass ☐ Fail ☐ N/A	
11	Flame photometer	☐ Pass ☐ Fail ☑ N/A	☐ Pass ☐ Fail ☑ N/A	
12	UPS / Stabilizer	☑ Pass ☐ Fail ☐ N/A	☑ Pass ☐ Fail ☐ N/A	

Warning and Error Checked

Item	Event	Before	After
13	Error list	☑ None ☐ Appear : _____	☑ None ☐ Appear : _____


เอกสารไม่ควบคุม


Base Line Test : Reagent_Baseline_CN_Phenol_NH3




เอกสารไม่ควบคุม


Detector Signal Test : Phenol

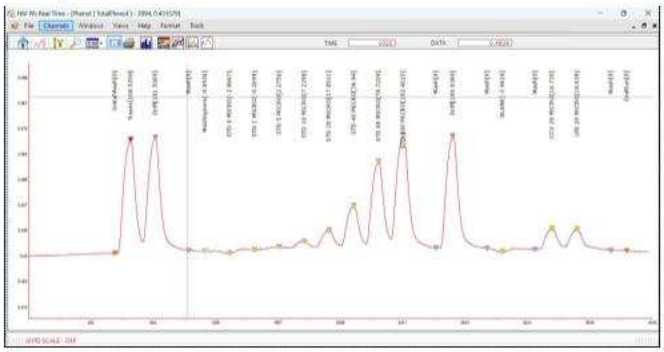

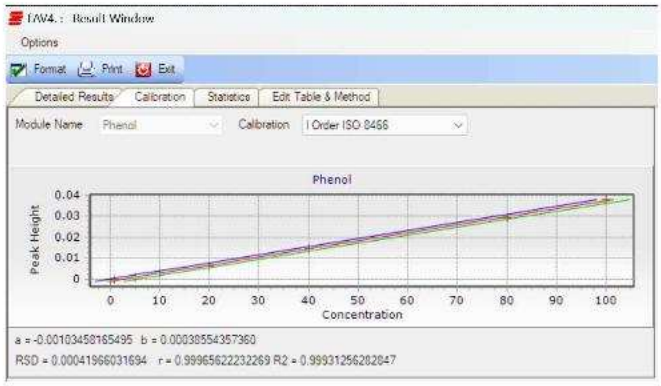



Detector Signal Test : CN

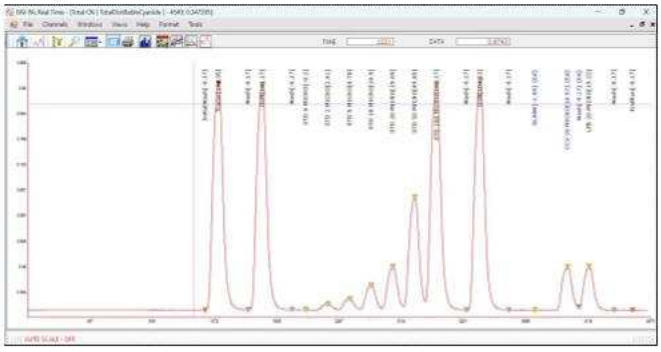

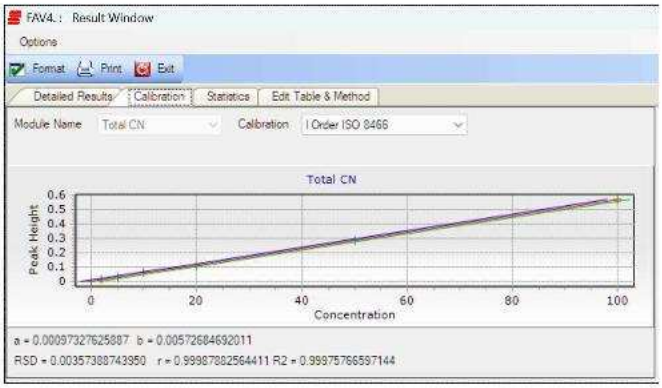

Detector Signal Test : NH3

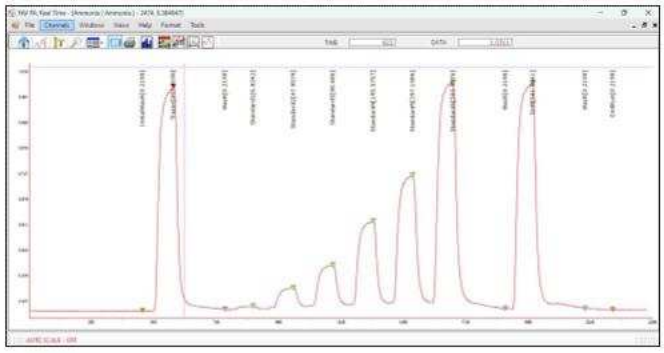

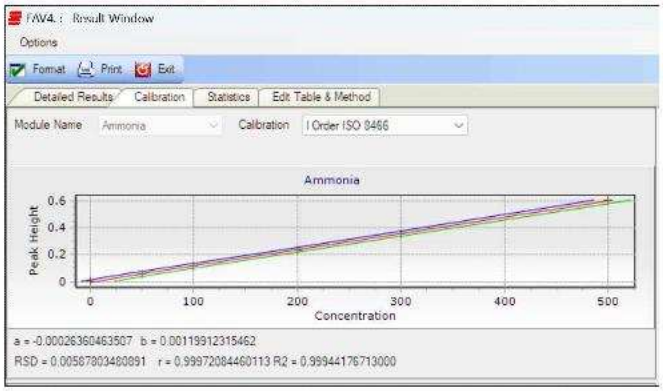

HANNA instruments

Hanna Instruments (Thailand) Ltd.

410/67-68 Soi Ratchadapisek 24, Ratchadapisek Rd., Samsen-nok, Huaykwang, Bangkok 10310 Tel: 0-2541-4199 Fax: 0-2541-4198

ilac-MRA ANAB ACCREDITED CALIBRATION LABORATORY AC-3061

Certificate No. : HIT-2510-0375

Page : 1 of 2

CERTIFICATE OF CALIBRATION

Equipment :	COD Test Tube Heater		
Meter Model :	HI839800-02	**Serial No. :**	H0185001
Tube Heater :	25 Vial Capacity	**Resolution :**	0.1°C
Temperature Range :	(-10 to 160)°C	**Temperature of Reaction :**	150°C
Manufacturer :	Hanna Instruments	**Made in :**	Romania
Condition As-Received :	Used Product	**Reference :**	RE250401
Ambient Temperature :	(25 ± 2)°C	**Relative Humidity :**	(50 ± 15)% RH
Customer name :	United Analyst and Engineering Consultant Co., Ltd.		
	3 Soi Udomsuk 41, Sukhumvit Rd., Bangchak,		
	Phrakhanong, Bangkok 10260		
Received date :	5 March 2025		
Calibrate date :	7 March 2025		
Issue date :	7 March 2025		
Calibrated Location :	Hanna Instruments (Thailand) Ltd.		
Calibration Procedure :	This calibrator was conducted by using in-house: calibration procedure CP-04 by using certified reference standard instruments.		

Calibrated by : ☑ Mr. Pichit Petthong
☐ Mr. Channarong Soinak

Approved by : Mr. Anan Suwanchaisakul
Authorized Signatory

HANNA Instruments (Thailand) Limited

This certificate was certified only for the instrument we calibrated.

This result of calibration was found accurate on date and place of calibration only.

** This certificate may not be reproduced other than in full, except with the prior written ** approval of the head of Hanna Instrument (Thailand)

เอกสารไม่ควบคุม

HANNA instruments

Certificate No. : HIT-2510-0375

Condition of this calibration result:

Reference Standard Instruments : This certification is traceable to the international unit of unit maintained through:

Instruments	Model	Serial No.	Certificate No.	Traceable
Data Acquisition Switch Unit	34970A	MY44065265	WK2407-141-1	WK Electric Co., Ltd.
Digital Thermo-Hygrometer	HT-771SD	AL07155	25H171	Technology Promotion Association (Thailand-Japan).

Calibration Result:

Measurement Temperature Source Accuracy for COD Reactor.

Capacity (Vial)	Nominal Value (°C)	Average Value (°C)	Uncertainty of Measurement (±°C)
25 Vial	150.0	150.4	0.47

Unit : °C

(1A) 150.407	(2A) 150.377	(3A) 150.269	(4A) 150.402	(5A) 150.422
(1B) 150.426	(2B) 150.394	(3B) 150.644	(4B) 150.690	(5B) 150.542
(1C) 150.477	(2C) 150.303	(3C) 150.627	(4C) 150.257	(5C) 150.176
(1D) 150.462	(2D) 150.456	(3D) 150.199	(4D) 150.406	(5D) 150.102
(1E) 150.185	(2E) 150.513	(3E) 150.235	(4E) 150.460	(5E) 150.442

Figure: Shows the location of the temperature source.

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

** End of certificate **

เอกสารไม่ควบคุม

Agilent CrossLab
From Insight to Outcome

Introduction

Customer Information

- Customers should provide all necessary operating supplies upon request of the engineer.
- A customer representative should be available to the engineer while performing the preventive maintenance procedures. Customers are responsible for regular maintenance and are encouraged to observe the service representative.
- Any parts not included in the Parts Lists section of this document are not part of the recommended Preventive Maintenance service nor are they included in the price of this service.
- If a system requires the use of extra or special procedures and/or parts for the maintenance service, then these must be ordered separately and charged as a repair, which may incur additional costs.
- For customers using HF applications, the instrument should be returned to its standard sample introduction system.

© Agilent Technologies, Inc. 2022

Agilent

เอกสารไม่ควบคุม

Agilent CrossLab
From Insight to Outcome

Agilent CrossLab Start Up Services

Agilent 5100 5110 ICP-OES Preventive Maintenance

Agilent Preventive Maintenance provides factory recommended service for your analytical instruments to assure reliable operation and the accuracy of your results

Delivered by highly trained and certified service engineers using genuine Agilent parts and supplies, Agilent Preventive Maintenance provides what you need to reduce unplanned downtime and keep your systems operating at their peak performance.

This checklist is used as a guide for completing the preventive maintenance tasks. A signed copy of this checklist is provided for your records

© Agilent Technologies, Inc. 2022

Agilent

เอกสารไม่ควบคุม

Agilent CrossLab
From Insight to Outcome

Important Customer Web Links

- To access **Agilent University**, visit http://www.agilent.com/crosslab/university/ to learn about training options, which include online, classroom and onsite delivery. A training specialist can work directly with you to help determine your best options.
- To access the **Agilent Resource Center** web page, visit https://www.agilent.com/en-us/agilentresources. The following information topics are available:
  - Sample Prep and Containment
  - Chemical Standards
  - Analysis
  - Service and Support
  - Application Workflows
- The **Agilent Community** is an excellent place to get answers, collaborate with others about applications and Agilent products, and find in-depth documents and videos relevant to Agilent technologies. Visit https://community.agilent.com/welcome
- Videos about specific preparation requirements for your instrument can be found by searching the **Agilent YouTube** channel at https://www.youtube.com/user/agilent
- **Need to place a service call?** Flexible Repair Options | Agilent

© Agilent Technologies, Inc. 2022

Agilent

เอกสารไม่ควบคุม

Service Engineer's Responsibilities

- Contact the customer and ensure that all necessary supplies are available before the preventive maintenance visit.
- Only select those pages that relate to the system or module being serviced.
- Complete empty fields with the relevant information.
- Complete the relevant checkboxes in the checklist using either a "X" or tick mark "✓".
- Check **"Service not applicable"** check boxes to indicate services/tasks not delivered, as appropriate.
- Complete the Preventive Maintenance services in the most logical order relevant to the individual system service in the order of the tasks listed.
- Complete the **Service Review** section together with the customer.
- Complete the fields for page numbers at the foot of each selected page
- Add relevant page numbers to selected pages and complete the total number of pages field in the Service Completion section
- **Ask the customer to sign the Service Verification section including the customer's and your signature.**

© Agilent Technologies, Inc. 2022

เอกสารไม่ควบคุม

Preparation

- ☑ Discuss any specific issues with the customer before starting.
- ☑ Review the instrument logbook for recorded problems and comments.
- ☑ Save instrument control settings before starting the procedure.
- ☑ Perform a general inspection of the system for cleanliness.
- ☑ Check for proper installation of parts, assemblies, sensors etc.
- ☑ Check system for required installation of components and implementation of Service Notes
- ☑ Check for required firmware/software updates and verify with customers if they would like them installed.
- ☐ For HF application systems, if standard sample introduction system was not installed, ask the customer to install it. N/A
- ☑ Ask the customer to remove any samples from the ICP-OES sample introduction area, auto sampler or around the ICP-OES.

© Agilent Technologies, Inc. 2022

เอกสารไม่ควบคุม

Instrument Maintenance

System Information

☐ Check this box if an instrument configuration report is attached instead of completing the table.

Instrument System Name and ID	5110 VDV ICP-OES
Instrument System Site and Location	UAE Consultant

List System Component Product Numbers	List the Serial Numbers of each Component
1. G 8015 A	MY 19030001
2.	
3.	
4.	
5.	
6.	
7.	
8.	
9.	

ICP-OES Configuration Table	Circle the type or write in the type if other
Nebulizer Type	(SeaSpray) OneNeb Conical | Other
Spray Chamber	Cyclonic Single Pass (Cyclonic Double Pass) Other
Torch	Radial (Dual View) Other
Torch Type	One Piece (Semi Demountable) Fully Demountable | Other
Injector Diameter	2.4mm (1.8mm) 1.4mm | 0.8mm | Other
Injector Material	(Quartz) Ceramic | Other

© Agilent Technologies, Inc. 2022

เอกสารไม่ควบคุม

Preventive Maintenance Procedures

Record Pre-PM instrument performance

- ☑ Run Instrument Performance test.
- ☑ Record results in Instrument Performance Test Results Table – Pre-PM.

Clean and inspect ICP-OES system

- ☑ Look for any obvious external damage or problems.
- ☑ Inspect water cooling hoses, gas lines and power cord for excessive wear or damage.
- ☑ Perform a general internal inspection of the system for excessive dust accumulation, clean if necessary.
- ☑ Inspect sample introduction components and record any required maintenance in the Service Engineer Comments and notify the customer of the required actions required.
- ☑ Record the instrument operating conditions in the ICP-OES Status Results Table.
- ☑ Replace the polychromator purge filter.
- ☑ Replace the radial pre-optics window.
- ☑ Replace the axial pre optics window for SVDV and VDV instruments.
- ☑ Check exhaust flow for the correct positive extraction at the exhaust duct to insure they meet minimum specifications.
- ☑ Replace air inlet dust filter.
- ☐ Replace high capacity air inlet dust filter element if installed. N/A
- ☑ Remove and clean instrument water inlet filter.

Agilent Water Recirculator

- ☐ **Service not applicable**
- ☑ Drain cooling fluid and remove any particles from the chiller reservoir.
- ☑ Remove, clean and reinstall water inlet metal mesh filter if present.
- ☑ Re fill with Agilent Cool Clear cooling fluid.
- ☑ Clean the cooling system Air filter and the condenser.

© Agilent Technologies, Inc. 2022

เอกสารไม่ควบคุม

SPS 3 Auto Sampler

- [x] **Service not applicable**
- [ ] Power cycle the autosampler and verify successful initialization.
- [ ] Inspect X and Z axis belts for wear. Replace is necessary.
- [ ] Clean X and Z axis slide shafts.
- [ ] Using customer's racks and the Agilent software move the sample probe to the 4 outermost corners and rinse port, ensure that the probe is approximately centered in the vial.

SPS 4 Auto sampler

- [x] **Service not applicable**
- [ ] Clean the spill tray, rack location mat, end frames and chassis with a damp soft cloth and diluted mild detergent.
- [ ] Clean the auto sampler cover panels, if cover kit is installed, with domestic window cleaner.
- [ ] Check the X-axis and Z-axis drive belts for cracks, splits, damaged teeth, excessive fraying, color changes or degradation from fumes.
- [ ] Check the X-axis, Theta-axis and Z-axis FFC cables for cracks, incorrect positioning, damaged edges or damaged connectors.
- [ ] Pump Tubing Replacement. Replace peristaltic pump tubing. Replace all tubing that goes from the rinse station to the pump and from the pump to the waste/rinse bottles
- [ ] Test using customer's tray and move the sample probe to the sample vial 1, wash vial and rinse port and ensure that the probe is centered in the vial. If not use calibration wizard and calibrate the position.

AVS 4, 6, 7 Advanced Valve System

- [x] **Service not applicable**
- [ ] Replace valve rotor seal
- [ ] Check fittings for signs of leaks
- [ ] Check tubing including autosampler tubing for kinks or excessive wear
- [ ] Check high flow pump for signs of leaks

เอกสารไม่ควบคุม

Restore Instrument

- [ ] For HF applications, ask the customer to re install their sample introduction system. N/A
- [x] Leave system in an idle state: on and purging.
- [x] Guidance: If the PM service is performed prior to a qualification service, then use the qualification procedure as a guide for final instrument set up and checkout.

Service Review

- [x] Attach available reports/printouts of all tests to this documentation.
- [x] Record the Preventive Maintenance service activity in the customer's records/logbook.
- [x] Record the PM event in the Smart Alerts logbook, if applicable.
- [x] Update/reset instrument maintenance counters as appropriate.
- [x] Affix the PM sticker to the system or instrument logbook based on the customer's request.
- [x] Complete the Service Engineer Comments section if there are additional comments.
- [x] Review this service, parts replaced, and test results obtained with the customer.
- [x] If the instrument firmware was updated, record the details of the change in the Service Engineer's Comments box. Systems in a compliant environment may need additional documentation.
- [x] **Complete the Signature Page with both Service Engineer and Customer signatures.**

เอกสารไม่ควบคุม

ICP-OES adjustment

- [x] Check position of Zn peak, adjust if required.
- [x] Check Argon Ratio, adjust to specified value if required.
- [x] Perform Detector Calibration.
- [x] Perform Instrument Calibration.

Record Post-PM instrument performance

- [x] Run Instrument Performance test.
- [x] Record results in Instrument Performance Test Results Table - Post PM.
- [x] For systems using ICP Expert version 7.3 and above, run the following Instrument tests

  - [x] Subsystem Communications Test
  - [x] Air Flow
  - [x] Water Flow
  - [x] Gas Flows
  - [x] RF Generator
  - [x] Camera Test
  - [x] Optics Test
  - [x] Nebulizer Test

- [x] Record the result in the Instrument Test Results Table

เอกสารไม่ควบคุม

Test Results

Instrument Performance Test Results Table

Note: These measurements do not form part of any specification and are for reference only.

	Pre PM Sensitivity Check		Post PM Sensitivity Check	
	Radial	Axial *	Radial	Axial*
Zn 213.857 nm SRBR	17982.8	2879.2	22308	3662.9
Mn 257.610 nm SRBR	95670.5	196149	106832.0	179844
Al 396.152 nm SBR	5.2	8.0	7.0	7.4
K 766.491 nm SBR	3.0	14.6	3.4	8.7

* Axial result is not applicable for G8016AA, G8012AA Radial View instruments.

Instrument Test Results Table

Note: The Instrument Test results are for systems using ICP Expert version 7.3 and above only.

Instrument Test	Result
Subsystem Communications Test	Pass
Air Flow	Pass
Water Flow	Pass
Gas Flows	Pass
RF Generator	Pass
Camera Test	Pass
Optics Test	Pass
Nebulizer test	Pass

เอกสารไม่ควบคุม

ICP-OES Status Results Table

Note: These measurements do not form part of any specification and are for reference only.

Measurement	Standby Mode		Plasma On	
Mains Voltage	231.288	VAC	228.330	VAC
Mains Current	0.083	A	0.100	A
Instrument Temperature	21.1	°C	21.6	°C
RF Air Flow (sensor speed)	44.0	Hz	41.1	Hz
Plasma Exhaust Temperature	No measurement		47.1	°C
Water Flow Oscillator	No measurement		1.14	L/min
Water Flow Detector	0.92	L/min	0.90	L/min
Water Inlet Temperature	19.5	°C	18.5	°C
Polychromator Temperature	35.4	°C	35.4	°C
CCD Temperature	-40.1	°C	-39.9	°C
Thermal Stabilizer	35.0	°C	35.0	°C
Argon Supply Pressure	634.43	kPa	583.77	kPa
Purge Gas Supply Pressure*1	631.28	kPa	604.02	kPa
Option Gas Supply Pressure*1	–	kPa	–	kPa
Nebulizer Flow	No measurement		0.70	L/min
Nebulizer Back Pressure	No measurement		273.61	kPa
Plasma Gas Flow	No measurement		1196	L/min
Auxiliary Gas Flow	No measurement		1.00	L/min
RF Power	No measurement		1200.4	W
RF Supply Current	No measurement		8.228	A
RF Supply Voltage	No measurement		194.529	V

*1 If option installed

Agilent

เอกสารไม่ควบคุม

Signature Page

Service Engineer Comments (optional)

If there are any specific points you wish to note as part of performing the installation or other items of interest for the customer, please write in this box.

Service Verification

Service Request Number:
6008006630

Service Engineer Name:
Worawit T.

Service Engineer Signature:
Worawit T.

Total number of pages in this document
14

Date Service Completed:
3 Nov 2025

Customer Name
Aphorn O.

Customer Signature
Aphorn O.

Agilent

เอกสารไม่ควบคุม

Consumed PM Parts

Part Description	Part Number	Product or Model# where used	Quantity consumed
Axial Pre-Optic Window	G8010-68014	G8010A, G8011A, G8014A/G8015A	1
Radial Pre-Optic Window	G8010-68015	All	1
Agilent Cool Clear Coolant Fluid	5793-0037	Agilent Water Recirculator	–
Purge Gas Filter	G8010-60136	All	1
Air Inlet filter	G8000-68002	All	1
High Capacity Air Filter	G8010-60139	Optional	–
Rotor seal for 6-7 port valve for AVS6/7	G8494-60002	G8494A/G8495	–
Rotor seal for 4 port valve for AVS4	G8493-60002	G8493A	–
Rinse solution to rinse station 2.5mm id x 1m	G8410-80123	SPS 4	–
Barb connector 2.5mm-1.5mm ID	G8410-80124	SPS 4	–
PVC waste tubing,8mm od x 5mm id, 2m	G8410-80122	SPS 4	–
Additional Parts may be required from engineer's stock:			
X axis drive belt	5410047500	SPS 3	–
Z axis drive belt	5410047400	SPS 3	–
Peristaltic pump tubing, PVC SolveFlex, 3 bridged,	3710049000	SPS 4	–

Consumed Parts Reference
(Purchased by customer, not included as part of PM)

☑ Section Not Applicable

Part Description	Part Number	Product or Model# where used	Quantity consumed

Agilent

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

DQE Services

CERTIFICATE OF CALIBRATION

Certificate No. : SP25-019 Page 1 of 5

Customer : United Analyst and Engineering Consultant Co.,Ltd. (Head Office)

Address : 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Location of calibration : Instrument room (207)

Equipment : UV-Vis Spectrophotometer

Manufacturer : Agilent Technologies

Model : Cary 60

Serial No. : MY15410009

ID No. : UAE.WAT.020/2558

Received Date : 26 May 2025

Calibration Date : 26 May 2025

Issue Date : 29 May 2025

Condition Instrument : Good

Calibrated by : (Mr.Tanawut Rittidach)
Technical Manager

Approved by : (Ms.Chonticha Sangngern)
Quality Manager

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the DQE Services Co., Ltd.

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP25-019

Environment Condition : Ambient Temperature 25 ± 5 °C

Relative humidity 55 ± 20 %RH

Calibration method : In-house method CP-01 Based on ASTM E275-08

Certified Reference Materials :

Material	Serial No.	Certificate No.	Due date
Absobance Standard set	25760	115663	25 October 2025
Absobance Standard set	25757	115638	25 October 2025
Wavelength Standard set	25806	115657	25 October 2025
Wavelength Standard set	25758	115665	25 October 2025

Traceability : This certification is traceable to the International System of Unit maintained at National - Institute of Standards and Technology (NIST) through Starna Scientific Limited

Spectral Band Width of UUC : 1.5 nm.

Scan Speed of UUC : 60 nm/min

Scan Interval of UUC : 0.15 nm.

Resolution of UUC : Photometric 0.0001 Abs.

Wavelength 0.1 nm.

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP25-019

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
235	0.0000	0.0000	0.0000	0.0050	2.00
	0.7469	0.7488	-0.0019	0.0063	2.00
257	0.0000	0.0000	0.0000	0.0050	2.00
	0.8674	0.8663	0.0011	0.0067	2.00
313	0.0000	0.0000	0.0000	0.0050	2.00
	0.2919	0.2902	0.0017	0.0052	2.00
350	0.0000	0.0000	0.0000	0.0050	2.00
	0.6430	0.6428	0.0002	0.0063	2.00

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP25-019

Calibration Results : Without adjustment

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
420	0.0000	0.0000	0.0000	0.0028	2.00
	0.5780	0.5739	0.0041	0.0031	2.00
	1.0484	1.0430	0.0054	0.0029	2.00
	2.1876	2.1876	0.0000	0.0084	2.00
440	0.0000	0.0000	0.0000	0.0028	2.00
	0.5595	0.5581	0.0014	0.0034	2.00
	1.0239	1.0219	0.0020	0.0035	2.00
	2.1230	2.1207	0.0023	0.0085	2.00
465	0.0000	0.0000	0.0000	0.0028	2.00
	0.5230	0.5190	0.0040	0.0029	2.00
	0.9633	0.9609	0.0024	0.0029	2.00
	1.9753	1.9719	0.0034	0.0079	2.00
546.1	0.0000	0.0000	0.0000	0.0028	2.00
	0.5181	0.5161	0.0020	0.0031	2.00
	1.0002	0.9979	0.0023	0.0033	2.00
	1.9973	2.0021	-0.0048	0.0102	2.00
590	0.0000	0.0000	0.0000	0.0028	2.00
	0.5517	0.5503	0.0014	0.0030	2.00
	1.0803	1.0808	-0.0005	0.0031	2.00
	2.0373	2.0324	0.0049	0.0105	2.00
635	0.0000	0.0000	0.0000	0.0028	2.00
	0.5591	0.5583	0.0008	0.0031	2.00
	1.0518	1.0513	0.0005	0.0030	2.00
	1.9274	1.9281	-0.0007	0.0102	2.00

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP25-019

Wavelength Accuracy :

CRMs Values (nm.)	UUC Reading (nm.)	Correction (nm.)	Uncertainty (nm.)	Coverage factor k
241.72	242.0	-0.28	0.18	2.00
279.45	279.5	-0.05	0.18	2.00
287.81	287.6	0.21	0.18	2.00
334.06	333.8	0.26	0.18	2.00
360.93	360.5	0.43	0.18	2.00
418.59	417.9	0.69	0.18	2.00
445.94	445.4	0.54	0.18	2.00
453.66	453.2	0.46	0.18	2.00
460.02	459.6	0.42	0.18	2.00
536.59	536.5	0.09	0.18	2.00
637.98	638.5	-0.52	0.18	2.00
431.38	430.7	0.68	0.18	2.00
472.50	472.3	0.20	0.18	2.00
513.47	513.5	-0.03	0.18	2.00
528.88	528.9	-0.02	0.18	2.00
573.17	573.8	-0.63	0.18	2.00
585.35	585.2	0.15	0.20	2.00
684.40	685.1	-0.70	0.18	2.00
740.72	741.1	-0.38	0.20	2.00
748.55	748.9	-0.35	0.18	2.00
807.03	807.1	-0.07	0.18	2.00
879.28	879.1	0.18	0.18	2.00

Remark : - UUC = Unit Under Calibration

- N/A = Not Avaiable
- The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%

- End of Certificate -

เอกสารไม่ควบคุม

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

Certificate of Calibration

Cert. No.: 25TM579
Page : 1 of 3

Equipment : Hot Air Oven
Manufacturer : Memmert
Model : UF 55
Serial No. : B212.0411
ID No. : UAE.WAO.005/2556
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260
Location : Lab Floor 2

Received Order : 19 March 2025
Calibration Date : 19 March 2025
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %
AC Line Voltage : (220 ± 22) V

Calibrated by : Man Pattanapongpaiboon

Approved by : Approved Signatory

( ) Chakrit Waewwanjua
( ) Suwit Imjai
(✓) Kunchit Promprat

Issue Date : 27 March 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2503-0437OC-3
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Cert. No.: 25TM579
Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor k
104.0	104.0	104.0	0.040	0.43	0.78	2
120.0	120.0	120.0	0.64	1.3	1.6	2
180.0	180.0	180.0	0.49	1.5	1.8	2

Calibration Point (°C)	Measured Temperature (°C) Position									Uncertainty
	1	2	3	4	5	6	7	8	9 (ref.)	(±°C)
104.0	104.335	104.135	104.363	104.317	103.649	103.738	104.179	104.229	104.025	0.42
120.0	119.575	119.366	119.807	119.905	118.994	119.194	119.888	119.994	120.064	1.1
180.0	180.286	179.510	180.401	180.551	179.281	179.463	180.196	180.451	180.374	1.2

Average* : The average of 30 values in each position.
Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.
Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.
Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.
UUC* : Unit Under Calibration
Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor ***k***, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม

Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2503-0437OC-3

Cert. No.: 25TM579
Page : 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD) and Thermocouple Type T.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-


Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY44073361	24LM73	TPA	18 May 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Environment during calibration	Beginning	Finished
Temp. (°C)	27	28
REL.Humid. (%)	49	55
AC Supply (Volt)	221	224



Position :	Ref. Std. ID No.: @ Calibration Point (120,180) °C	(104) °C
1	23-01TC-01	1RTD-2/1
2	23-01TC-02	1RTD-2/2
3	23-01TC-03	22-01RTD-03
4	23-01TC-04	1RTD-2/4
5	23-01TC-05	1RTD-2/5
6	23-01TC-06	1RTD-2/6
7	23-01TC-07	23-01RTD-07
8	23-01TC-08	1RTD-2/8
9 (ref.)	23-01TC-09	23-01RTD-09

Probe Installation Details :
a = 5.0 cm
b = 5.0 cm
c = 5.0 cm

Dimension of Chamber :
D = 0.50 m
W = 0.80 m
H = 0.75 m
Capacity = 0.30 m³

เอกสารไม่ควบคุม

Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

Calibration Certificate

Certificate No.: 2502229-001-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakhanong, Bangkok 10260

Page 1 of 3

Equipment: CHAMBER (Incubator)
Manufacturer: MEMMERT
Model: IPP 260
Serial No.: V615.0187
ID No.: UAE.MIC.003/2559
Order No.: 2502229
Operation No.: 2502229-001
Date of Receipt: 19 March 2025
Date of Calibration: 19 March 2025

Calibrated by Mr.Jerawut Prapawuttipong
Scientist

Approved by (Mr.Pheraphat Tuanjit) (for)
Manager, Division of Calibration Laboratory
Responsible for the Technical Management Team

Date of Issue: 25 March 2025

The uncertainties are for a confidence probability of approximately 95 %.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65

2008 ถนนสุขุมวิท 39 แขวงสุขุมวิท เขตวัฒนา กรุงเทพมหานคร 10110
2008 Soi 39, Asok Montri Road, Khlong Tan Nuea Subdistrict, Watthana District, Bangkok 10110, Thailand
โทร +66(0) 2392 6580 โทรสาร +66(0) 2392 6845

เอกสารไม่ควบคุม

สถาบันอุตสาหกรรมแห่งชาติ
กรมส่งเสริมอุตสาหกรรม
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

ilac-MRA

NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Report

Certificate No.: 2502229-001-01

Equipment: CHAMBER (Incubator)

Model: IPP 260 Serial No.: V615.0187

Resolution: 0.1 °C ID No.: UAE.MIC.003/2559

Manufacturer: MEMMERT

Date of Calibration: 19 March 2025

Location: LABORATORY, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.

Environment Condition:

Ambient Temperature (16.2 ± 1) °C

Relative Humidity (32 ± 4) %

Line Voltage (223 ± 3) Volt

Condition of this results of Calibration:

1. This instrument was calibrated by insert 9 standard thermometer into its chamber and calibration according to WI-TE-014 Based on TLAS G-20-1/02-08 (E): Guidelines for Calibration and Checks of Temperature Controlled Enclosures.
   - The temperature scale used was based on ITS - 90.
   - All data show below were final values and the initial data may be obtained upon request.
2. Reference Standard Instrument :

Instrument	Model	Serial No./ID No.	Certificate No.	Due Date	Through
Digital Thermometer with sensor	34972A	MY49016851	TE 670477-01	4 May 2025	NATIONAL FOOD INSTITUTE
	RTD	CH2101-109/ RTD0101-109			

3. This certificate is traceable to International System of Units (SI Units).
4. This certificate was certified only for the instrument we calibrated.
5. This result of calibration was found accurate as shown on date and place of calibration only.
6. Condition of Calibrated Item : Good

   UUC Description :

   Time of Record 1 Hour 9 Minute At 35.0 °C

   Fresh air Damper [-] Open Position [-]

   [X] Close Fan [-]

   [-] Not Available
7. Result of Calibration : [X] Without adjustment [ ] After adjustment

25 March 2025

2008 ซอยศูนย์วิจัย 36 ถนนศูนย์วิจัย แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2008 Soi 36, Arun Amarin Road, Bang Y Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel. +66(0) 2422 8688 Fax +66(0) 2422 8545
nfi.or.th

เอกสารไม่ควบคุม

PerkinElmer
For the Better

PinAAcle 900F
Preventive Maintenance Report

Company Name: UAE Consultant Co., LTD.

Instrument Location: 41 Sukumvhit Rd.,

Phra Khanong, Bangkok 10260

Instrument Serial No.: PFBS20031902

Date: 27 Oct 2025

เอกสารไม่ควบคุม

สถาบันอุตสาหกรรมแห่งชาติ
กรมส่งเสริมอุตสาหกรรม
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

ilac-MRA

NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Report

Certificate No.: 2502229-001-01

Equipment: CHAMBER (Incubator)

Model: IPP 260 Serial No.: V615.0187

Resolution: 0.1 °C ID No.: UAE.MIC.003/2559

Manufacturer: MEMMERT

Date of Calibration: 19 March 2025

Calibration point: 35.0 °C

Calibration result:

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
MIN	15.5	28	220.0
MAX	17.1	35	225.0



Table1 : Reporting of Temperature

Calibration point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.9 is REF)									Uncertainty ± (°C)
	# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9	
35.0	34.94	34.95	34.91	34.93	35.15	35.01	34.98	35.05	35.12	0.29

Table 2 : Reporting of Characterization Result

UUC* Setting (°C)	UUC* Reading (°C)			Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
	MIN	MAX	Average			
35.0	35.0	35.0	35.0	0.10	0.21	0.35

Note: The quoted uncertainty include " Stability " and " Loading effect (20% of Temp Uniformity) "

UUC* = Unit Under Calibration

Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.

Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.

Overall Variation = The difference of the maximum and minimum measured temperatures througout observation time.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2, providing a level of confidence of approximately 95 %.

--------- End ---------

25 March 2025

F-CS-012 Revision: 01 Date: 20-04-65

2008 ซอยศูนย์วิจัย 36 ถนนศูนย์วิจัย แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2008 Soi 36, Arun Amarin Road, Bang Y Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel. +66(0) 2422 8688 Fax +66(0) 2422 8545
nfi.or.th

เอกสารไม่ควบคุม

PinAAcle 900F Preventive Maintenance (PM)

Company Name:	United Analyst and Engineering Consultant Co., LTD.		
Address (Instrument Location):	41 Sukumvhit Rd., Phra Khanong, Bangkok 10260		
Serial Number:	PFBS20031902	**PM Number:**	1 of 2
Customer Name (if applicable):	K. Yainda	**Telephone Number:**	095-5580049
Customer Support Engineer Name:	K. Chayanan	**Service Order Number:**	WO-06332081
Date PM Performed: (DD-MMM-YYYY)	27 Oct 2025	**Next PM Due Date:** (DD-MMM-YYYY)	27 Apr 2026
Standard Labor Hours to Complete PM :		**5 hours**	

Part Number	Release	Publication Date	
09370145 Rev.9	A	January 2018	PerkinElmer

Scope
The purpose of this PM is to ensure the continued functionality of the PinAAcle 900F by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer.
The customer should save their method before the PM begins.

General Instructions:
The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM.
Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files.
The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer.
Update the PM sticker and instrument logbook as required.

Copyright Information
This document contains proprietary information that is protected by copyright. All rights are reserved.
No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of PerkinElmer, Inc.
Copyright © 2013 PerkinElmer, Inc.

Trademarks
Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners.
Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no Warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.
PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

เอกสารไม่ควบคุม

Component List

Component / Specific Model	Serial #	Configuration Notes
PinAACle900F	PFBS20031902	Syngistix V.4.0.1.1935
FIAS100	100S24040501	

Parts Lists

Parts Included with the PM		
Part Number (if applicable)	**Description**	**Quantity**
B0501696	Fan Filters	1
N3160156	O-Ring Kits for Sampling Introduction (Stainless Steels Nebulizer)	N/A
N3160157	O-Ring Kits for Sampling Introduction (Plastic Nebulizer)	1
N9301714	Replacement Acetylene Filter Cartridge	1
TH001022	Replacement Air Filter Cartridge	1

Additional Reagents and Standards Required for PM				
Part Number (if applicable)	**Description**	**Quality**	**Batch/Lot #**	**Expired Date (MM/YY)**
N9300183	1000 mg/L Copper Standard	AR	28-83CUY1	Nov 2026

Additional Reagents and Standards Required for PM (Customer Support Solution)				
Part Number (if applicable)	**Description**	**Quantity**	**Batch/Lot #**	**Expiration Date (MM/YY)**
N/A	DI Water	250 mL	AR	AR
N/A	0.5% HNO_3	250 mL	AR	AR

เอกสารไม่ควบคุม

Additional Tools Required for PM			
Part Number (if applicable)	**Description**	**Quantity**	**Serial #**
N1013000	0.2A Neutral density filter	1	101N0089015
N1013002	1.0A Neutral density filter	1	101N0089015
03030997	System 2 EDL Driver	1	03030997
N3050605	As System 2 EDL	1	16148
N3050121	Cu Lumina HCL	1	060419-030180
N3050109	Be Lumina HCL	1	061219-020041
N3050139	K Lumina HCL	1	030819-010130
N3050152	Ni Lumina HCL	1	052719-020020

เอกสารไม่ควบคุม

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. **General:**
   - ☑ Review the instrument performance with the customer and document any recent problems.
   - ☑ Inspect the customer log book and make any appropriate PM entries.
   - ☑ Perform general inspection of system for cleanliness.
2. **PC Instrument Software:**
   - ☑ Instrument Software user files/databases archived, packed, and/or deleted as needed.
3. **Mechanical:**
   - ☑ Inspect and clean all fans and filters. Replace filters if necessary
   - ☑ Inspect all gas lines for leaks and/or wear. Replace if needed.
   - ☑ Clean exterior of the instrument.
   - ☑ Inspect the burner head, burner chamber, and nebulizer. Clean if needed as stated in the Hardware Guide.
   - ☑ Check burner head dimensions with the feeler gauge as stated in the Hardware Guide in the Maintenance chapter section on cleaning the burner head and checking sloth width. Replace if out of specification
   - ☑ Check the condition of the end cap, burner head, and nebulizer O-rings. Replace if necessary.
   - ☑ Check the drain system for signs of wear. Replace worn or damaged parts.
   - ☑ Visually check for proper flame conditions when igniting the Air-C2H2 and N20-C2H2 flames (if applicable).
4. **Electrical:**
   - ☑ Inspect PC boards. Clean if necessary.
   - ☑ Carefully check all internal and external cable connections.
   - ☑ Check instrument firmware revisions upgrade to current levels (if necessary)
   - ☑ Run Diagnostics Test within the Advanced function of the Spectrometer page. Check the results in the service log folder in the Spectrometer BM Log Viewer.
5. **Optics:**
   - ☑ Inspect and clean the sample compartment windows, if needed.
   - ☑ Inspect optics. Clean or replace if necessary.
6. **Gasses:**
   - ☑ Verify that the Gasses supplied to the instrument are within the pressure and purity specifications found in the PinAAcle 900 Series Pre-installation Checklist SDB.
   - ☑ Verify that the acetylene filter and air filter element is dry. Replace if necessary.

เอกสารไม่ควบคุม

7. **Flame Interlock Check:**

Description: Check to ensure that all safety interlocks are closed.

Parameter	Specification	Test Results	Pass/Fail
Flame Sensor	Air/C_2H_2 Flame correctly shuts down	Active	Passed
Drain Sensor	Air/C_2H_2 Flame correctly shuts down	Active	Passed
Nebulizer Sensor	Air/C_2H_2 Flame correctly shuts down	Active	Passed
C_2H_2 Pressure Sensor	Air/C_2H_2 Flame correctly shuts down	Active	Passed
Air Pressure Sensor	Air/C_2H_2 Flame correctly shuts down	Active	Passed
Burner Head Sensor	Choosing Nitrous Oxide as the oxidant should trigger an interlock shuts down	Active	Passed

8. **After PM Performance tests:**

8.1 Detector Linearity with Barium

Description: Ensures that the detector is linear in the Visible Range.

Parameter	Specification	Certificate Value at 553.6 nm (Abs.)	Test Results	Pass/Fail
1.0 A ND Filter	± 5% from Cert.	0.9995	0.9887	Passed
0.2 A ND Filter	± 5% from Cert.	0.1936	0.1896	Passed

8.2 Baseline Noise at 1.0 Absorbance with Barium

Description: Ensures that a high absorbance will not produce excessive noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.010	0.001	Passed

8.3 AA Baseline Noise with Copper

Description: Check baseline noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.001	0.0001	Passed

เอกสารไม่ควบคุม

8.4 D_2 Background Compensation with Copper

Description: Verifies the instruments ability to compensate for Background absorption.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.010	0.0001	Passed

8.5 AA-BG Baseline Noise with Copper

Description: Ensures that background correction does not produce excessive noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.005	0.0001	Passed

8.6 AA-BG Baseline Noise with Arsenic

Description: Ensures that background correction does not produce excessive noise at a low wavelength.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.005	0.0004	Passed

8.7 Flame Sensitivity

Description: Instrument Sensitivity checked against Copper standard.

Standard Copper Sensitivity	Specification	Results (Abs.)	Pass/Fail
5 mg/L Sensitivity SS Neb (if applicable)	> 0.250 Abs.	N/A	Not Applicable
2 mg/L Sensitivity HS Neb (if applicable)	> 0.250 Abs.	N/A	Not Applicable

10. **Review:**
    - ☑ Review with the customer PM work performed.
    - ☑ Review with the customer routine maintenance procedures.
    - ☑ Discuss recommended customer supplied materials to have on hand.
    - ☑ Attach PM sticker.

เอกสารไม่ควบคุม

Additional Comments

Additional Comments Regarding the PM

Review

The preventive maintenance checks and if applicable performance tests for PinAAcle 900F have been completed.	
This PinAAcle 900F Passes ☑ Fails ☐ the preventive maintenance.	
Review of Preventive Maintenance:	
Authorized PerkinElmer Representative: Chayanan k.	Date: 27 Oct 2025 (DD-MMM-YYYY)
Authorized Customer Representative:	Date: 27 Oct 2025 (DD-MMM-YYYY)

เอกสารไม่ควบคุม

Atomic Absorption/FIAS 100/400 Preventive Maintenance (PM)

Company Name:	United Analyst and Engineering Consultant Co., LTD.		
Address (Instrument Location):	41 Sukumvhit Rd., Phra Khanong, Bangkok 10260		
Room Number:	Lab		
Asset Number (if applicable):	1 of 2	**Customer System ID:**	K. Yanida
Service Engineer Name:	K. Chayanan	**Service Order Number:**	WO-06332087
Date PM Performed: (DD-MMM-YYYY)	27-Oct-2025	**Next PM Due Date:** (DD-MMM-YYYY)	27-Apr-2026

Part Number	Release	Publication Date	
09370005	C	January 2013	PerkinElmer®

Scope
The purpose of this PM is to ensure the continued functionality of the Atomic Absorption/FIAS 100/400 by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer.
The customer should save their method before the PM begins.

General Instructions:
Always check with the customer before making any changes that may affect the customer's analysis or calibration.
The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer.
Update the PM sticker and instrument logbook as required.

Copyright Information
This document contains proprietary information that is protected by copyright. All rights are reserved.
No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of PerkinElmer, Inc. **Copyright © 2013 PerkinElmer, Inc.**

Trademarks
Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners.
Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.
PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

เอกสารไม่ควบคุม

Component List

Component / Specific Model	Serial #	Firmware Version	Configuration Notes
FIAS100	100S24040501	2.20	Syngistix V4.0.1.1935

Parts Lists

Parts Included with the PM				
Part Number (If applicable)	**Description**	**Quantity**	**Batch/Lot #**	**Expiration Date** (MM/YY)
B050 2706	Fan Filter	1	N/A	N/A

Additional Tools Required for PM				
Part Number (If applicable)	**Description**	**Quantity**	**Serial #**	**Calibration Due Date** (MM/YY)
N/A	Digital Volt Meter	1	N/A	N/A
Additional Reagents and Standards Required for PM				
Part Number (If applicable)	**Description**	**Quantity**	**Batch/Lot #**	**Expiration Date** (MM/YY)
N/A	N/A	N/A	N/A	N/A

เอกสารไม่ควบคุม

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. **General:**
   - ☑ Review the instrument performance with the customer and document any recent problems.

     _____

   - ☑ Is the Working Environment Acceptable? If not, document.

     _____

   - ☐ Visual Damage (if yes, describe)

     _____

   - ☑ Check incoming AC line voltage for proper levels and grounding.
   - ☑ Verify Voltage switch on back of instrument is correct
   - ☑ Perform general inspection of system for cleanliness. Clean if needed.
   - ☑ Gas supply cylinders secured, lines leak checked and argon or nitrogen supply pressure verified (45 – 58 psi).
   - ☑ Inspect the customer log book and make any appropriate PM entries.
   - ☑ Fan checked and filter cleaned
   - ☑ Heating mantle or Universal Cell Holder checked

2. **Instrument components**
   - ☑ Non-return valve checked/repaired/replaced if needed (B019 8111). Clean the valve if there is any liquid in it. Replace the rubber sleeve (B013 5123) if it is worn. Check the flow meter for any signs of fluid in it. Clean the flow meter if needed.
   - ☑ Verify condition of pump pressure adjustment levers (B050 7794 - look for cracks or problems with the springs), pump rollers (B300 0251 check for wear), and thumb screws (B050 7796).
   - ☑ Check the Multiport valve for proper switching, flow, and insure there are no leaks. Clean valve parts and replace o-rings if needed (large o-ring: B050 1250, small o-ring: B004 5095). Use a squirt bottle & fishing line to try to dislodge clogs.
   - ☑ Firmware Version checked. Latest is 2.20.

3. **Mixing/Separation Assembly & Pump Tubing:**
   - ☑ Mixing separator assembly checked
   - ☑ Filter/membrane checked (B050 8306)
   - ☑ Condition of the pump tubing (replace if necessary), correct pump tubing for the solutions being run. Make sure the correct magazines are being used. B050 7791 for 0.13 – 1.80 mm tubing; B050 7792 for 1.60 – 3.18 mm tubing.

เอกสารไม่ควบคุม

4. **Cell, Cell Windows, Transfer Line:**
   - ☑ Cell checked
   - ☑ Cell windows checked
   - ☑ Transfer line checked for moisture (if moisture is a problem, the Nafion dryer might be needed)

5. **Operational Tests:**
   - ☑ Run DI water through the carrier/reductant/sample system. Verify smooth flow of liquid throughout without leaks. Replace tubing & fittings if needed.

6. **Review:**
   - ☑ Review with the customer PM work performed.
   - ☑ Review with the customer routine maintenance procedures.
   - ☑ Discuss recommended customer-supplied materials to have on hand.
   - ☑ Attach PM sticker.
   - ☑ Update Logbook.

เอกสารไม่ควบคุม

Additional Comments

Additional Comments Regarding the PM

Review

The preventive maintenance checks and if applicable performance tests for FIAS 100/400 have been completed.

This FIAS 100/400 Passes ☑ ***Fails*** ☐ ***the preventive maintenance.***

Review of Preventive Maintenance:	
Authorized PerkinElmer Representative: Chayanam K.	Date: 27 Oct 2025 (DD-MMM-YYYY)
Authorized Customer Representative: [illegible]	Date: 27 Oct 2025 (DD-MMM-YYYY)

เอกสารไม่ควบคุม

Document History

Revision	Description of Change	Page(s)	Date
A	First release		May 2008
B	Addition of Batch/Lot Number, Expiration Date, and Report Fields.	2,7	February 2009
C	Update to new format	All	January 2013

เอกสารไม่ควบคุม

Perkin

PerkinElmer TruQ

PerkinElmer Number: N9300163
Element and Matrix: 1000 µg/mL Copper in 2% HNO3
Starting Material: Copper Metal
Starting Material Lot No: 10221A
Density: 1.011 g/mL @ 20°C

Lot No: 28-83CUY1
Certification Date: MAY - - 2025
Expiration Date: NOV 30 2026

Trace Metallic Impurities in the Actual Solution via ICP / ICP-MS Analysis:

Element	µg/mL	Element	µg/mL	Element	µg/mL	Element	µg/mL	Element	µg/mL
Ag	0.005	Dy	<0.001	Li	<0.001	Pt	<0.001	Tb	<0.001
Al	<0.002	Er	<0.001	Lu	<0.001	Rb	<0.001	Te	<0.001
As	<0.001	Eu	<0.001	Mg	<0.001	Re	<0.001	Th	<0.001
Au	<0.001	Fe	0.02	Mn	<0.001	Rh	0.002	Ti	<0.001
B	<0.001	Ga	<0.001	Mo	<0.001	Ru	<0.001	Tl	<0.001
Ba	<0.001	Gd	<0.001	Na	0.004	Sb	<0.001	Tm	<0.001
Be	<0.001	Ge	<0.001	Nb	<0.001	Sc	<0.001	U	<0.001
Bi	<0.001	Hf	<0.001	Nd	<0.001	Se	<0.002	V	<0.001
Ca	<0.01	Hg	<0.001	Ni	<0.001	Si	<0.1	W	<0.001
Cd	<0.001	Ho	<0.001	P	<0.2	Sm	<0.001	Y	<0.001
Ce	<0.001	In	<0.001	Pb	0.005	Sn	0.003	Yb	<0.001
Co	<0.001	Ir	<0.001	Pd	<0.001	Sr	<0.001	Zn	0.02
Cr	<0.001	K	<0.1	Pr	<0.001	Ta	<0.001	Zr	<0.001
Cs	<0.001	La	<0.001						

Traceability Documentation for Solution Standard:

Certified Value: 999 µg/mL ±5 µg/mL (refer to side 2)
Certified Value is Traceable to: NIST SRM #3114
*** Classical Wet Assay:** 997 µg/mL
Method: EDTA titration using PAN as indicator. EDTA standardized against Pb(NO$_3$)$_2$ NIST SRM #928.

***Instrument Analysis using ICP Spectrometer:** 1001 µg/mL
via NIST SRM #3114

We guarantee that our PerkinElmer TruQ Atomic Spectroscopy Standards are stable and accurate to ±0.5% of certified concentration until the expiration date, provided the standards are kept tightly capped and stored under normal laboratory conditions. This value is the sum of cumulative errors associated with the analytical determinations, pipetting, and diluting to final volume. For these solutions we use high purity acids, ASTM Type I water (18 megohm double deionized), and leached, triple-rinsed bottles. All glassware used is class A.

Certifying Officer: Y. Parikh
Yogesh Parikh, Senior Spectroscopist

เอกสารไม่ควบคุม

Terms & Conditions

Customer Acknowledgment of receipt of the above repair / replacement.

Special Terms and Conditions: This is not an invoice.

Taxes will be applied to your invoice if applicable.

เอกสารไม่ควบคุม

PerkinElmer
For the Better

PerkinElmer Scientific (Thailand) Co., Ltd.
290 Soi Soonvijai 4
Krwang Bangkapi, Khet Huay Kwang
Bangkok 10310
Thailand
Tel: 66 2719 6420 ; Fax: +66 2 319 7900
http://www.perkinelmer.com

Service Report

Work Order Number	Activity Code	Billing Type	Requested Start Date	Model	Serial Number
WO-0833286	Planned Maintenance	Contract	28/04/2568 10:27 a.	AAnalyst 300	PFBS2003902
Service Representative Name	**Contract Number**		**Expiry Date**	**Equipment ID**	**System ID**
Kanan, Chayanan	SC-0035664169		31/10/2025	N/A	N/A
UDI Number					
N/A					
Equipment Location			**Bill To Name**		
บริษัท ปูโรเด็ด แอนะลิติค แอนด์ เซอรวิเซอร์ จำกัด (มหาชน) กรุงเทพมหานคร 51 10260 TH			บริษัท ปูโรเด็ด แอนะลิติค แอนด์ เซอรวิเซอร์ จำกัด (มหาชน) กรุงเทพมหานคร 51 10260 TH		
Customer Contact	**Phone Number**	**Fax Number**	**Email**		**Purchase Order**
ผู้ติดต่อ แผนกวิทยาศาสตร์	085-5580049	N/A	yaninchanlek@gmail.com		HPO-250100002

Work Description

- PM 1/2 (Monthly)
- Cleaning Cell, Chamber, Filter
- Wavelength Calibrate ; Pass
- Wavelength Scan As,Cu,Be,K,Ni ; Pass
- Align cell with Hg. ; OK

Start Date	End Date	Work Description
27/10/2025	27/10/2025	
27/10/2025	27/10/2025	

Tools Used

Quantity	Calibrated Tool	Description	Serial Number	Last Calibration Date	Next Calibration Date
*** No Calibrated Tools Used ***					

Material Used

Part Number	Part Description	Note	Lot/Serial Number	Quantity
N9301714	Balston G2-HZ Filter Cartridge			1

Labour Details

Part Number	Part Description	Start Date	Quantity
SV000013	Preventative maintenance	27/10/2025	4
SV000002	Service Travel	27/10/2025	2

Work Complete	Customer Signature	Technician Signature
Yes ☑ No ☐	ผู้ลงนาม	Chayanan k.
PM/OQ/PV Left with Customer: Yes ☐ No ☑	2/11/2568 ผู้ติดต่อ แผนกวิทยาศาสตร์	2/11/2568 Kanan, Chayanan

เอกสารไม่ควบคุม

PerkinElmer
For the Better

PerkinElmer Scientific (Thailand) Co., Ltd.
290 Soi Soonvijai 4
Krwang Bangkapi, Khet Huay Kwang
Bangkok 10310
Thailand
Tel: 66 2719 6420 Fax: +66 2 319 7900
http://www.perkinelmer.com

Service Report

100S24040501

Work Order Number	Activity Code	Billing Type	Requested Start Date	Model	Serial Number
WO-0833286	Planned Maintenance	Contract	28/04/2568 10:29 a.	FIAS100	100S24040201
Service Representative Name	**Contract Number**		**Expiry Date**	**Equipment ID**	**System ID**
Kanan, Chayanan	SC-0035664136		31/10/2025	N/A	N/A
UDI Number					
N/A					
Equipment Location			**Bill To Name**		
บริษัท ปูโรเด็ด แอนะลิติค แอนด์ เซอรวิเซอร์ จำกัด (มหาชน) กรุงเทพมหานคร 51 10260 TH			บริษัท ปูโรเด็ด แอนะลิติค แอนด์ เซอรวิเซอร์ จำกัด (มหาชน) กรุงเทพมหานคร 51 10260 TH		
Customer Contact	**Phone Number**	**Fax Number**	**Email**		**Purchase Order**
ผู้ติดต่อ แผนกวิทยาศาสตร์	085-5580049	N/A	yaninchanlek@gmail.com		HPO-250100002

Work Description

- PM 1of 2 (SN_100S24040501)
- Cleaning Port Vale, Manifold, Tuning
- Run Hg test ; Pass

Start Date	End Date	Work Description
27/10/2025	27/10/2025	
27/10/2025	27/10/2025	

Tools Used

Quantity	Calibrated Tool	Description	Serial Number	Last Calibration Date	Next Calibration Date
*** No Calibrated Tools Used ***					

Material Used

Part Number	Part Description	Note	Lot/Serial Number	Quantity
B0134040	Sample Loop, 500UL			1
B0501350	O-Ring *5.77 x 1.78			1
B0500748	O-RING 16 X 1.75 VITON			2

Labour Details

Part Number	Part Description	Start Date	Quantity
SV000013	Preventative maintenance	27/10/2025	3
SV000002	Service Travel	27/10/2025	2

Work Complete	Customer Signature	Technician Signature
Yes ☑ No ☐	ผู้ลงนาม	Chayanan k.
PM/OQ/PV Left with Customer: Yes ☐ No ☑	2/11/2568 ผู้ติดต่อ แผนกวิทยาศาสตร์	2/11/2568 Kanan, Chayanan

เอกสารไม่ควบคุม

Terms & Conditions
Customer Acknowledgment of receipt of the above repair / replacement.
Special Terms and Conditions: This is not an invoice.
Taxes will be applied to your invoice if applicable.

3/11/2568 WO-06332087

เอกสารไม่ควบคุม

Condition of this calibration result

1. Reference Standard Instrument

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1) Document Process Calibrator	54030049	130RC116	25E2743	25 Aug 2026
2) Ref. Standard Thermometer	4982054	110RC044	25I708	03 July 2026

- This measurement result is traceable to SI throught Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials :The measurement results are traceable to SI through Hach Lenge GmbH Ltd., Deutsche Akkreditierungsstelle, Accredited No.D-RM-15184-01-00
:The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.007	CPA chem	1114384	12 June 2027
pH 6.999	Hach Lenge GmbH	C03273	13 May 2027
pH 10.010	CPA chem	1114385	08 June 2026

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4,7)(7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement	Coverage factor
	pH	mV	mV	pH	(±mV)	k
pH Meter	4.00	177.48	177.4	4.01	0.058	2.00
S/N.: HA0A0005	7.00	0.00	0.1	7.00	0.058	2.00
	7.00	0.00	0.1	7.00	0.058	2.00
	10.00	-177.48	-177.2	10.01	0.058	2.00

เอกสารไม่ควบคุม

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

NSC-TISI-TIS17025 CALIBRATION 0008

Certificate of Calibration

Equipment :	pH Meter
Manufacturer :	Horiba
Model :	LAQUA-PH210
Serial No. :	HA0A0005
ID No. :	UAE.EFM.004/2563(EFM.pH.04/63)
Condition As-Received:	Used Item
Received Date :	09 December 2025
Calibration Date :	11 December 2025
Reference :	2512-0243WSC-2
Submitted by :	United Analyst and Engineering Consultant Co.,Ltd. 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure :	In - house method : - CP-CH5 by direct measurement with DC voltage standard and direct measurement with certified reference material (CRM) - CP-CH8 by comparison with temperature standard
Calibrated by :	Warakorn Lerngagtrakul
Approved by :	Approved Signatory

(✓) Chakrit Waewwanjua
( ) Ponpan Paipim
( ) Saithip Meangmai

Issue Date : 12 December 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7)(7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (±)	Coverage factor k
pH Electrode	4.007	4.01	175.4	0.0085	2.05
S/N.: -	6.999	7.00	-0.3	0.0095	2.00
	6.999	7.01	-0.5	0.0096	2.00
	10.010	10.01	-170.6	0.0092	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : -
- Serial No. : -

Dimension of probe

- Length : 112 mm.
- Diameter : 16 mm.
- Immersion Depth : 100 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (± °C)	Coverage factor k
15.0	15.002	15.0	-0.002	0.13	2.00
30.0	30.002	30.0	-0.002	0.13	2.00
45.0	45.003	45.0	-0.003	0.13	2.00

Remark - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม

United Analyst and Engineering Consultant Co., Ltd.

Automatic Mercury Analyzer

Model : RA-4500

Preventive Maintenance Report

SERIAL No. RA-4500	:	11780278
Soft version	:	Ver 2.0.5
ROM version	:	Ver 2.0.2
DATE	:	02 JULY 2025
DUE DATE	:	02 JULY 2026

INSPECTED BY : Natthaphong P.
(Natthaphong P.)

APPROVED BY :
(Kitichai S.)

Kinetic Solutions Company Limited.
2, Soi Lat Krabang 1, Lat Krabang Subdistrict,
Lat Krabang District, Bangkok 10520
Tel. (+66) 062-789-5221

เอกสารไม่ควบคุม

Inspection details

Remark	
1. Cleaning Mercury Analyzer RA-4500	
- Body case, Cell Detector, Table of Sample	
2. Replace consumable one year set for RA-4500	
3. Checking Mercury Analyzer RA-4500	
- Mercury Lamp	- Outlet Activated Carbon Filter
- Membrane Filter	- Flow Sensor
- Main Pump Tube	- Valves
- Motor Pump	- Heater
- Motor Reagent pump	- Cooling Fan
- Motor of Arm	- Stirrer motor
- Motor of Table	- Color sersor
- Motor of Lift	- Instrument Performance
4. Adjust Optical system	
5. Inspection Calibration curve and Repeatability of Mercury Analyzer RA-4500	
หมายเหตุ Heater Box เริ่มเสื่อมสภาพ แนะนำให้เปลี่ยนในรอบ PM ถัดไป	

เอกสารไม่ควบคุม

Inspection

ITEMS		SPECIFICATIONS	RESULT	JUDGE
1. Quantity	-	Accessories are completed.	GOOD	OK
2. Appearance	2.1 Overall Appearance	No visible damage.	GOOD	OK
	2.2 Parts / Cables	Correctly placed and connected.	GOOD	
3. Indication	Nameplate / Label	Plate and Label are indicated.	GOOD	OK
4. Self check				
4.1 GLP Counter	Mercury Lamp	5000 hours	110 hr	OK
	Membrane Filter	2000 hours or 1 year after replace	< 1 hr	OK
	Main Pump Tube	750 hours or 1 year after replace	< 1 hr	OK
	Absorbed Hg	1500 mg	< 1 hr	OK
	P1 Tube	2000 hours or 1 year after replace	< 1 hr	OK
	P2 Tube	2000 hours or 1 year after replace	< 1 hr	OK
	P3 Tube	2000 hours or 1 year after replace	< 1 hr	OK
	P4 Tube	2000 hours or 1 year after replace	< 1 hr	OK
	P5 Tube	2000 hours or 1 year after replace	< 1 hr	OK
	P6 Tube	2000 hours or 1 year after replace	< 1 hr	OK
	P7 Tube	2000 hours or 1 year after replace	< 1 hr	OK
	Heater	2000 hours	42 hr	OK
4.2 Check/Test	Flow rate Adjustment	Flow rate 0.14 - 0.20 L/min	0.18 L/min	OK
	Signals Detector	V.SIG is 3.5 - 4.5 V.	4.03 V.	OK
		V.REF is 3.5 - 4.5 V.	4.03 V.	OK
	Cooling Fan	Check the operation of cooling fan	PASS	OK
	Color Sensor	signals (R,G,B) at least one nonzero	PASS	OK
	Radiation Thermometer	a positive valve form thermometer	PASS	OK
	Heater	heater temp rises 4 °C within 5 min.	PASS	OK
5. Heater	Temperature	At 95°C ± 2°C with 30 min.	94.7°C	OK
6. Calibration Curve	no pretreatment	0-10ng : Max.Dev. 5.0%	0.90%	OK
7. Repeatability	100 µg/L (n=5)	Average: 100 ± 5 µg/L	101.4 µg/L	OK
		C.V. ≤ 5.0%	0.71%	OK
8. Blank	no pretreatment	Less than 0.5 (AREA)	0.103 AREA	OK

Apparatus

NAME	Date Certified	Expiration
Mercury ICP Standard (1000 µg/mL) AccuStandard, Inc. Lot 223035027	March 10, 2023	March 10, 2028


เอกสารไม่ควบคุม

Title : Preventive Maintanance
Date : 02/07/2025
Name : Kinetic Solutions
Memo : Calibration curve 0-10ng

Method


Method1 (Pretreatment:without)
(1+1)H2SO4 : 0.9mL
10w/v% SnCl2 : 0.5mL
Measurement Time(sec) : 120sec

Calib



STD

No.	STD [ug/L]	SVOL [mL]	CVOL [mL]	DVOL [mL]	STD [ng]	AREA [ON]	MEAS [ng]	Dev [%]	Note
1	0.000	5.000	5.000	5.000	0.000	0.1107	0.0000	-	
2	100.000	0.025	5.000	5.000	2.500	3.2690	2.4250	3.0	
3	100.000	0.050	5.000	5.000	5.000	6.5434	4.9392	1.2	
4	100.000	0.075	5.000	5.000	7.500	9.8649	7.4895	0.1	
5	100.000	0.100	5.000	5.000	10.000	13.2088	10.0570	0.6	

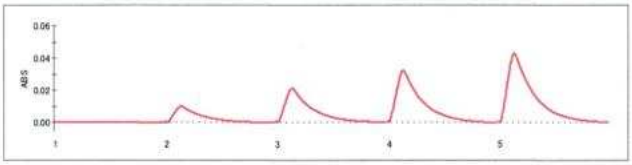

SMP


No.	NAME	SVOL [mL]	CVOL [mL]	DVOL [mL]	AREA [ON]	MEAS [ng]	CONC [ug/L]	Note
1	STD 100 ppb	0.050	5.000	5.000	6.7338	5.0854	101.708	
2	STD 100 ppb	0.050	5.000	5.000	6.7129	5.0693	101.386	
3	STD 100 ppb	0.050	5.000	5.000	6.6370	5.0110	100.220	
4	STD 100 ppb	0.050	5.000	5.000	6.7489	5.0970	101.940	
5	STD 100 ppb	0.050	5.000	5.000	6.7514	5.0989	101.978	
6	Blank	5.000	5.000	5.000	0.1035	-0.0055	0.000	

Statistics

No.	NAME	TRY	AV [ug/L]	SD [ug/L]	Cv [%]
1	STD 100 ppb	5	101.4464	0.724979	0.71

เอกสารไม่ควบคุม

NIC NIPPON INSTRUMENTS CORPORATION

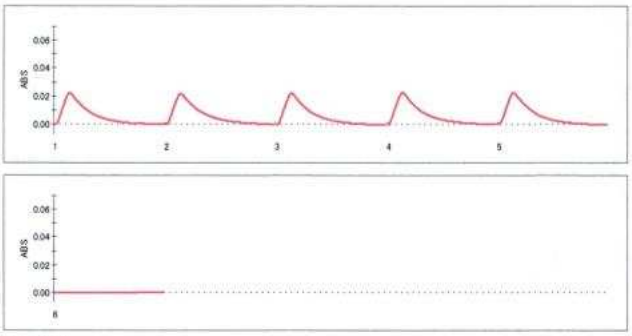

Self Check

```
Heat check:PASS!! ( 25.7degC[05:00] ->  29.7degC[02:29])
Sensor check:PASS!! ( 253-  15= 238)
Leak check:PASS!! (0.18L/min)
Sig/Ref check:PASS!! (Sig:4.03V, Ref:4.03V)
Drift check:PASS!! ( 0.0000037 - -0.0000026 =  0.0000063)
```

1. **Quality Standards:**
   ISO 17034:2016 – General Requirements for the Competence of Reference Material Producers
   ISO/IEC 17025:2017 – General Requirements for the Competence of Testing And Calibration Laboratories
   ISO 9001:2015 – Quality Management System – Requirements
   Eagle Registrations
2. **Intended Use:** The product covered by this certificate is designed for calibration or for use in quality control procedures for the specified chemical compounds listed on the reverse side. This product can be used for quantification and/or identification. This product can also be used as a reference material to validate analytical procedures, subject to the conditions under Section 7.
3. **Manufacturing:** All balances are calibrated daily using an in-house procedure with weights that are compared annually to master weights and traceable to NIST. The balances are also calibrated annually by an ISO/IEC 17025 accredited calibration laboratory. Please refer to the NIST test number listed on the front of this certificate. Class A glassware is used in the manufacture and quality control of all standards. Good Laboratory Practices have been used throughout the preparation of this Standard.
4. **Homogeneity:** This product is sufficiently homogeneous and any sample size would be within the uncertainty budget.
5. **Stability:** The manufacturer guarantees the stability of this solution through the expiration date stated on the label, when handled and stored according to the conditions stated on the label
6. **Uncertainty:** The uncertainty values as stated on the face of this certificate have been determined using the EURACHEM/CITAC Guide. We report a combined expanded uncertainty equal to the positive square root of the total variance of the uncertainty of the components using the following formula: $u_c = \sqrt{(u(V))^2 + (u(m))^2 + (u(V))^2 + (u(RO))^2}$ This formula represents uncertainty components from the mass, volume, short-term stability, long-term stability and homogeneity factors associated with the production of this product. The expanded uncertainty, assumes a normal distribution and a coverage factor of $k=2$ is chosen using approximately a 95% confidence level.
7. **Legal Notice and Limit of Liability:** This product is for routine laboratory analysis and research purposes only. The company's liability will be limited to replacement of product or refund of purchase price. Notice of claims must be made within thirty (30) days from date of delivery.

เอกสารไม่ควบคุม
NIPPON INSTRUMENTS CORPORATION
เอกสารไม่ควบคุม

125 Market Street
New Haven, CT 06513
USA

Tel (203)786-5290
Fax (203)786-5287
www.AccuStandard.com

AccuStandard® Inc.

CERTIFICATE OF ANALYSIS

AccuTrace™ Reference Standard

Catalog No: ICP-34N-1
Description: Mercury ICP Standard
Element: Mercury (Hg)
SRM: 3133
Lot: 223035027
Matrix: 10% Nitric acid
Hazards: *Refer to SDS for complete safety information*

Date Certified: Mar 10, 2023
Expiration: Mar 10, 2028
Density: 1.052 g/mL
Sample Size: 100 mL
Components: 1
Storage Condition: Ambient (>5 °C)

Certified Reference Material

Signal Word: Danger

ANAB AR-1463 ISO/IEC 17025 ISO 17034 ISO Guide 34 ILAC-MRA

Certified Concentration: 1000 µg/mL

Trace Elements in µg/mL

Ag	nd<0.02	Ce	nd<0.2	Gd	nd<0.02	Lu	nd<0.02	Pb	nd<0.2	Sc	nd<0.02	Ti	nd<0.02
Al	nd<0.02	Co	nd<0.02	Ge	nd<0.2	Mg	nd<0.02	Pd	nd<0.2	Se	nd<0.2	Tl	nd<0.2
As	nd<0.2	Cr	nd<0.02	Hf	nd<0.02	Mn	nd<0.02	Pr	nd<0.2	Si	N/A	Tm	nd<0.02
Au	nd<0.02	Cs	N/A	Hg	*	Mo	nd<0.02	Pt	nd<0.2	Sm	nd<0.2	U	nd<0.2
B	nd<0.2	Cu	nd<0.02	Ho	nd<0.02	Na	nd<0.02	Rb	N/A	Sn	nd<0.02	V	nd<0.02
Ba	nd<0.02	Dy	nd<0.02	In	nd<0.2	Nb	nd<0.2	Re	nd<0.2	Sr	nd<0.02	W	nd<0.2
Be	nd<0.02	Er	nd<0.02	Ir	nd<0.2	Nd	nd<0.02	Rh	nd<0.2	Ta	nd<0.2	Y	nd<0.02
Bi	nd<0.2	Eu	nd<0.02	K	nd<0.2	Ni	nd<0.02	Ru	nd<0.02	Tb	nd<0.02	Yb	nd<0.02
Ca	nd<0.02	Fe	nd<0.02	La	nd<0.02	Os	N/A	S	N/A	Te	nd<0.2	Zn	nd<0.02
Cd	nd<0.02	Ga	nd<0.02	Li	nd<0.02	P	N/A	Sb	nd<0.2	Th	nd<0.02	Zr	nd<0.02

This Certified Reference Material was verified in accordance with ISO/IEC 17025 (AT-1339) and ISO 17034 (AR-1463).
This solution was assayed gravimetrically, using a balance calibrated against weight sets, ID #88270, traceable to NIST
A product with a suffix (-1A, -2B, etc. or -01, -02, etc.) on its lot number has had its expiration date extended and is identical to the same lot number without the suffix.
This product contains mercury and MUST be disposed of in accordance with all federal, state and local regulations.
The gravimetric uncertainty for this product is ±0.24%. The CRM uncertainty is ±2.4%
In order to verify the concentration(s), the final solution was checked by plasma emission spectroscopy (ICP) against material traceable to the above listed NIST SRM(s).
We use the highest purity raw materials available to minimize impurity levels in the final solution. Typically 99.999%+ pure starting materials are used as well as high purity acids and ASTM Type I 18 megohm deionized water
All trace level elemental impurities were determined via plasma emission spectroscopy on the concentrate.
All weights are traceable through NIST. Test No. 684/291344-18 & 684/292805-19
All glassware used in preparation is Class A.
All bottles are acid leached and triple rinsed with deionized water prior to use.
Shake bottle prior to use and do not pipette directly out of the bottle. Use only cleaned Class A volumetric glassware. Keep bottle tightly capped.

Certified By: Margaret O'Leary, Inorganic QC Manager

For use in routine laboratory analysis.

AccuStandard is accredited to ISO 17034, ISO/IEC 17025 and certified to ISO 9001:2015

เอกสารไม่ควบคุม

Technology

DKSH

Service Report

TO	FOR
Company: United Analyst and Engineering Consultant Co., Ltd. _ Bangkok-HQ Address: 700/2 หมู่ที่ 1 Phrakhanong District, Bangkok, 10260	Work Order Number: WO-00074079 Contact: Kamphong Boonpuang Email: kamphong.b@uaeconsultant.co.th Tel: +66 2763 2828 (7021), +66 8 6347 7390

WORK ORDER INFORMATION			
Top-Level		Order Type	Preventive Maintenance
Installed Product ID	IB-00105024	Billing Type	Chargeable
Product	SKALAR 2SAN59000 SAN++ Classic CFA 230V 2SAN59000	PO No.	HPO-250400209
Serial No.	182688	Warranty No.	
		Contract No.	

PRODUCTS SERVICED		
Installed Product Id	Serial Number	Product
IB-00105024	182688	SKALAR 2SAN59000 SAN++ Classic CFA 230V 2SAN59000

PROBLEM DESCRIPTION
PM 1 ครั้งปี **ใบเสนอราคาเลขที่ Q-120095

Line Number	Engineer	Start Date And Time	End Date And Time	Billable Labor Hour	Billable Travel Hour	Travel KM
WL-00342192	Yongyuth Chanphong	05/23/2025 9:30 AM	05/23/2025 6:00 PM	8.5		
Total				8.5	0	0

! Reach us at DKSH Service-Hotline : +66 2 639 7000
2533 Sukhumvit Road, Bangchak, 10260, Phrakhanong, Bangkok, Thailand
Phone +66 2 639 7000 Fax +66 2 333 1026

Delivering Growth - in Asia and beyond

เอกสารไม่ควบคุม

Line Number	Work Description
WL-00342192	- ทำ PM เสร็จแล้ว, เครื่องพร้อมใช้งาน

PARTS CONSUMED		
Part No	Part Description	Quantity

EXPENSES			
Part No	Expense Type	Description	Line Quantity

RECOMMENDED PARTS
อะไหล่สำรองที่ควรสั่งซื้อทั้งหมด 7 รายการ คือ Pump tube 3 รายการ (SA3028, SA3032 และ SA3034), หลอดไฟ Halogen 6V/10W (90020012) 1 รายการ จำนวน 2 หลอด, Tubing polyethylene 3 รายการ (SA3142, SA5141 และ SA5142)

REMARKS

Travel Time Disclaimer:
Please note that the travel time in this report only includes time taken to reach the installed equipment location. It does not include our engineer's return travel time.

Customer Signature:

K Kanphong

Customer Signature

Technician: Yongyuth Chanphong
Job Title: Service Manager
Email: yongyuth.yc@dksh.com

Date: 06/06/2025

เอกสารไม่ควบคุม

Check with Standard

Item	Characteristic	Before	After	Remark
14	Base Line Test	☐ Pass ☐ Fail ☑ N/A	☑ Pass ☐ Fail ☐ N/A	
15	Detector Signal Test	☐ Pass ☐ Fail ☑ N/A	☑ Pass ☐ Fail ☐ N/A	

Summary of checked

☑ The instrument can work normally and efficiently. (เครื่องมือวิเคราะห์ทำงานได้ปกติและมีประสิทธิภาพ)
☐ The instrument can work but it's requiring to maintenance. (เครื่องมือวิเคราะห์ทำงานได้แต่ต้องบำรุงรักษา)
☐ The instrument could not work it's requiring to repair. (เครื่องมือวิเคราะห์ไม่สามารถทำงานได้และต้องการซ่อมบำรุง)

Remark :

* Pump tube, Tubing polyethylene และ Air tube เริ่มเสื่อมสภาพ ให้เปลี่ยนอะไหล่ทั้งหมดเพื่อความมั่นใจในการใช้งาน

หมายเหตุ แนะนำอะไหล่ที่ควรสั่งเพิ่มเติม 7 รายการ ดังนี้
1. อะไหล่ สารเคมีตรวจ Ammonia จำนวน 3 รายการ (SA3032, SA5141 และ 90020012)
2. อะไหล่ สารเคมีตรวจ Phenol และ Cyanide จำนวน 6 รายการ (SA3028, SA3034, SA3142, SA5142 และ 90020012)

Standard Equipment Used

Equipment	Equipment I.D.	
Digital multi meter	S/N 57600592	Due date : 19-Jun-2025
Thermo hygrometer	S/N 39520444/904	Due date : 27-Dec-2025

Test By : (Mr. Yongyuth Chanphong)
Position : Supervisor, Technical Service

Approved by : (Mr. Eknapong Wankliang)
Position : Manager, Technical Services

เอกสารไม่ควบคุม

Job No. WO-00074079

Test Report

Customers	United Analyst and Engineering Consultant Co., Ltd.		
Equipment	Continuous Flow Analyzer	Manufacturer	SKALAR
Controller Mdel	SAS000	Auto Sample Model	SA1052
Controller Serial No.	182688	Auto Sample Serial No.	181729
Date of test	23-May-2025	Period	12 Month
Environment temperature	24.3 °C	Humidity	54.4 %RH

Results

Instrument Checked

Item	Characteristic	Before	After	Remark
1	Visual inspect	☑ Pass ☐ Fail	☑ Pass ☐ Fail	
2	Power supply (210 - 240 VAC)	220 VAC	220 VAC	
3	Computer	☑ Pass ☐ Fail	☑ Pass ☐ Fail	
4	Program	☑ Pass ☐ Fail	☑ Pass ☐ Fail	
5	Auto sampler	☑ Pass ☐ Fail	☑ Pass ☐ Fail	
6	Module holder			
	- Motor pump	☑ Pass ☐ Fail	☑ Pass ☐ Fail	
	- Pump tube	☐ Pass ☑ Fail	☑ Pass ☐ Fail	*
	- Air-injection	☑ Pass ☐ Fail	☑ Pass ☐ Fail	*
	- Chemistry manifolds, Switching valve, Coil, Membrane	☑ Pass ☐ Fail	☑ Pass ☐ Fail	
7	Detector			
	- Filter	☑ Pass ☐ Fail	☑ Pass ☐ Fail	
	- Flow cell	☑ Pass ☐ Fail	☑ Pass ☐ Fail	
	- Lamp	☑ Pass ☐ Fail	☑ Pass ☐ Fail	
8	Interface	☑ Pass ☐ Fail	☑ Pass ☐ Fail	
9	Rinsing valves	☐ Pass ☐ Fail ☑ N/A	☐ Pass ☐ Fail ☑ N/A	
10	Temperature / Reactor	☑ Pass ☐ Fail ☐ N/A	☑ Pass ☐ Fail ☐ N/A	
11	Flame photometer	☐ Pass ☐ Fail ☑ N/A	☐ Pass ☐ Fail ☑ N/A	
12	UPS / Stabilizer	☑ Pass ☐ Fail ☐ N/A	☑ Pass ☐ Fail ☐ N/A	

Warning and Error Checked

Item	Event	Before	After
13	Error list	☑ None ☐ Appear : _____	☑ None ☐ Appear : _____


เอกสารไม่ควบคุม


Base Line Test : Reagent_Baseline_CN_Phenol_NH3




เอกสารไม่ควบคุม


Detector Signal Test : Phenol

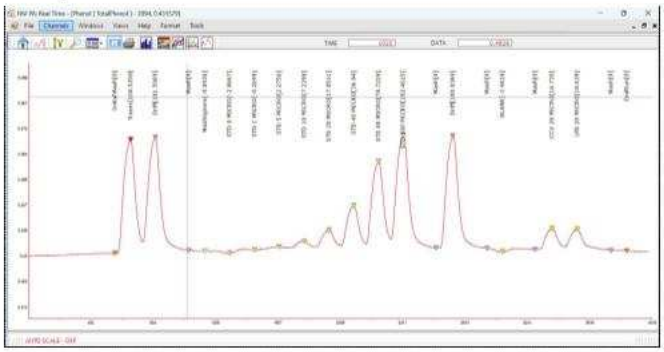

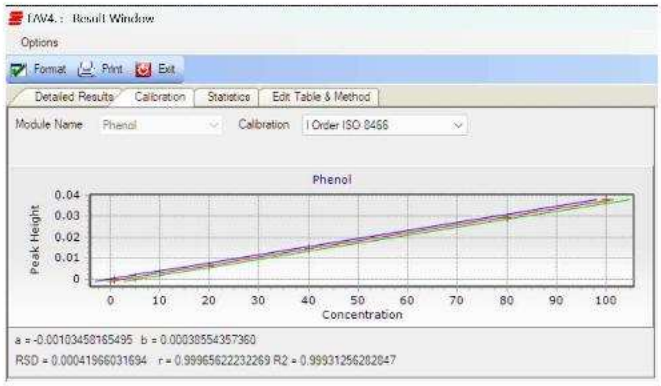



Detector Signal Test : CN

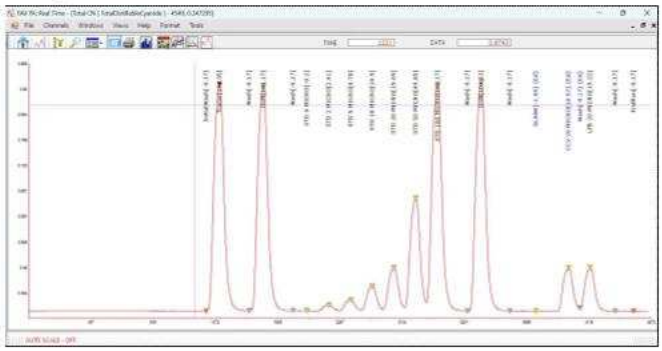

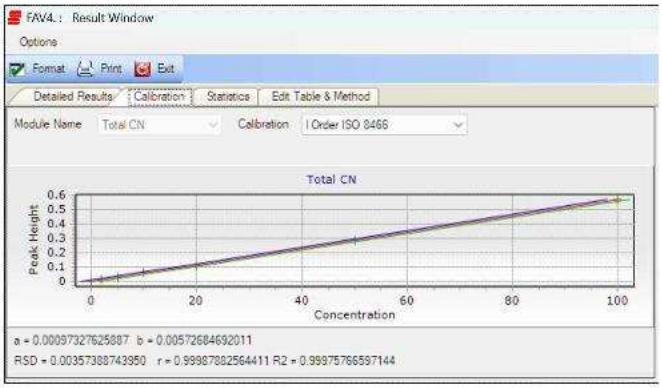

Detector Signal Test : NH3

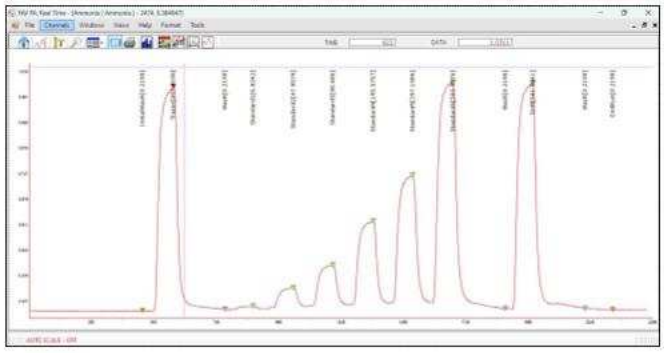

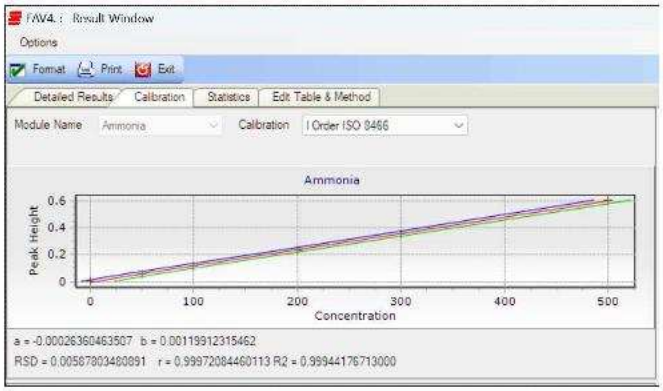

UAE TOX 009/2566

Agilent CrossLab
From Insight to Outcome

Agilent CrossLab Start Up Services

Agilent 8890 Gas Chromatograph
Preventive Maintenance Checklist

Agilent Preventive Maintenance provides factory recommended service for your analytical instruments to assure reliable operation and the accuracy of your results.

Delivered by highly trained and certified service engineers using genuine Agilent parts and supplies, Agilent Preventive Maintenance provides everything you need to reduce unplanned downtime and keep your systems operating at their peak. This checklist will be completed at the end of the service and provided to you as a record of the preventive maintenance activities.

Agilent

Introduction

Customer Information

- Customers should provide all necessary operating supplies upon request of the engineer.
- A customer representative should be available to the engineer while performing the preventive maintenance procedures.
- Any parts, not included in the Parts Lists section of this document, are not part of the recommended Preventive Maintenance service, nor are they included in the price of this service.
- If a system requires the use of extra or special procedures and/or parts for the maintenance additional costs.

Important Customer Web Links

- For more information about *Agilent Technologies services*, please visit our website using the following URL: http://www.agilent.com/en-us/productu/crosslab-instrument-services/service-repair
- The **Agilent Community** is an excellent place to get answers, collaborate with others about applications and Agilent products, and find in-depth documents and videos relevant to Agilent technologies. Visit https://community.agilent.com/welcome.
- To access **Agilent University**, visit http://www.agilent.com/crosslab/university/ to learn about training options, which include online, classroom and onsite delivery. A training specialist can work directly with you to help determine your best options.
- A useful **Agilent Resource Center** web page is available, which includes short videos on maintenance, quick lists of consumables for new instruments, and other valuable information. Check out the Resource Page here: https://www.agilent.com/en-us/agilentresources.
- **Need technical support, FAQs, supplies?** – visit our **Support Home page** http://www.agilent.com/search/support.
- Videos about specific preparation requirements for your instrument can be found by searching the *Agilent YouTube* channel at https://www.youtube.com/user/agilent.

เอกสารไม่ควบคุม

System Information

☑ Check this box if an instrument configuration report is attached instead of completing the table below.

Instrument System Name and ID	UAE-TOX-009/2566 / US2229A024
Instrument System Site and Location	UAE / Room 404

List System Component Product Numbers	List the Serial Numbers of each Component
1. B8490A	US2229A024
2. G4519A	CN22285350
3. G4514A	CN2228 7018
4.	
5.	
6.	
7.	
8.	
9.	
10.	

Preparation

- ☑ Discuss any specific issues with the customer before starting.
- ☑ Review the instrument logbook for recorded problems and comments.
- ☑ Save instrument control settings before starting the procedure.
- ☑ Perform a general inspection of the system for cleanliness.
- ☑ Check for proper installation of parts, assemblies, sensors etc.
- ☑ Check system for required installation of components, settings as defined by current Service Notes.
- ☑ Check for required firmware updates and verify with customers if they would like them installed.
- ☑ Before starting the following procedures, record the Detector Signal Output(s) in the results table. If the GC is turned OFF or in a service mode, comparing the detector outputs before and after the service is not possible.

เอกสารไม่ควบคุม

Service Engineer's Responsibilities

- Contact the customer and ensure that all necessary supplies are available before the preventive maintenance visit.
- Only select those pages that relate to the system or module being serviced.
- Complete empty fields with the relevant information.
- Complete the relevant checkboxes in the checklist using either a "X" or tick mark "✓".
- Check **"Section not applicable"** check boxes to indicate services/tasks not delivered, as appropriate.
- Complete the Preventive Maintenance service in the order of the tasks listed.
- Complete the Service Review section together with the customer.
- Complete the fields for page numbers at the foot of each selected page
- Complete the total number of pages field in the Service Completion section
- ***Ask the customer to sign the Service Completion section including the customer's and your signature.***

Additional Instruction Notes

- Check for any active service notes for this unit. If there are any applicable "Safety" or "Modification Recommended" Service notes, plan to implement the changes on this unit before doing any qualification service.
- Do not implement firmware updates, unless you get approval from the customer and are sure that they are compatible with the instrument control software.

เอกสารไม่ควบคุม

Preventive Maintenance Procedure

Clean and inspect GC

- ☑ Unplug power cord from the power source.
- ☑ Open GC covers and vacuum/remove any dust/debris. Pay particular attention to cooling fans.
- ☑ Inspect internal connectors for proper contact and placement.
- ☑ Reconnect Power to the GC. Power the GC on and verify the power on self-test passed.
- ☑ Verify oven motor spins freely and turns on with the oven door closed; off when the door is opened.
- ☑ Verify operation of all other fans - the inlet and EPC cooling fans.
- ☑ Verify oven intake/outlet flap assembly is operating smoothly while heating and cooling the oven

Inlet and detector consumable replacement

- ☑ Replace the split vent trap cartridge (filter) using the Maintenance procedure from either the Browser User interfaces on units with these inlets: Split/Splitless Capillary (SSL), Multi-Mode Inlet (MMI), Programmed Temperature Vaporizer (PTV), Volatiles Interface (VI).
- ☑ If the inlet system is used in Split Mode with viscous samples, inspect and clean the split vent tube on the inlet and flush or replace the tubing between the inlet and the split vent trap.
- ☑ For the inlets installed, perform inlet maintenance using the Maintenance procedure from the Browser user interfaces. Record the results. (Leak and restriction Test)
- ☑ If the GC includes a Flame Ionization Detector (FID), replace the jet. If the ignitor shows any buildup of sample or corrosion, replace the ignitor. Examine the FID collector and castle assemblies for contamination – clean as necessary.

Zero Sensors and Leak test

- ☑ Zero all pressure sensors using the Browser interface.
- ☑ Perform inlet pressure decay test(s) from the diagnostics screen on the Browser User interface. Record if test passed or failed in the results table.

Note: If the PM is done in preparation for an Operational Qualification, then the pressure decay test defined within that protocol can be used for the PM

เอกสารไม่ควบคุม

ALS Maintenance

- ☐ **Section NOT applicable**
- ☑ Check all cabling and configuration settings between GC, tray, and injectors.
- ☑ Vacuum or remove any dust, especially around fans.
- ☑ Check operation of all fans.
- ☑ Check syringe for smooth plunger operation.
- ☑ Check for smooth operation of the needle support – clean if necessary

Restore Instrument

- ☑ Restore the normal operating conditions or customer method using the Browser interface or Data System.
- ☑ Purge the system with carrier flow for 15 minutes
- ☑ Bake out the system, then restore the normal operating conditions
- ☑ After equilibration, check and record the post PM detector signal output values. Results should be similar or lower than the detector outputs recorded prior to PM
- ☑ Perform a chemical checkout. If this is a routine PM, inject the customer's sample using the ALS if applicable. This will act as a final checkout of both the ALS and the GC.

Note: If the PM Service is performed prior to a qualification service, then use the qualification procedure as a guide for final instrument set up and checkout.

เอกสารไม่ควบคุม

PM Parts List Table

Note: The following kits are recommended for capillary and purged packed inlets. If this is a general PM and the customer has a preferred set of consumables, you may use the customer's consumables.

Part description	Part number	Product or model# where used	Quantity consumed
SSL Capillary Inlet PM kit, Splitless	5188-6497	8890 GC	N/A
SSL Capillary Inlet PM kit, Split	5188-6496	8890 GC	1
SSL Capillary Ultra Inert Inlet Gold Seal with Washer	5190-6144	8890 GC	N/A
SSL Capillary Ultra Inert Inlet Splitless Liner - Single taper with Glass Wool	5190-2293	8890 GC	N/A
SSL Capillary Ultra Inert Inlet Low Pressure Drop Split Liner - with Glass Wool	5190-2295	8890 GC	N/A
PP Inlet PM kit	5188-6498	8890 GC	N/A
Split vent trap PM kit, single cartridge (for MMI, PTV & VI)	5188-6495	8890 GC	N/A
MMI Cleaning Kit	G3510-60820	8890 GC	N/A
PTV Septumless Head Rebuild Kit	5182-9747	8890 GC	N/A
PTV Septumless Head Teflon Guide	5182-9748	8890 GC	N/A
Ignitor (glow plug) assembly with O ring	19231-60680	8890 GC	1
FID Collector Rebuild/Cleaning Kit	G1531-67000	8890 GC	N/A
FID Collector Replacement Kit	G1531-67001	8890 GC	N/A
Standard .011-inch FID Jet	5200-0176	8890 GC	1
Universal .018-inch FID Jet	5200-0177	8890 GC	N/A

เอกสารไม่ควบคุม

Signature Page

Service Review

- ☐ Attach available reports/printouts of all tests to this documentation.
- ☑ Record the Preventive Maintenance service activity in the customer's records/logbook.
- ☑ Update/reset instrument maintenance counters as appropriate.
- ☑ Affix the PM sticker to the system or instrument logbook based on the customer's request.
- ☑ Complete the Service Engineer Comments section if there are additional comments.
- ☑ Review with the customer this service, parts replaced, and test results obtained.
- ☑ If the instrument firmware was updated, record the details of the change in the Service Engineer's Comments box or if necessary, in the customer's IQ records.
- ☐ Supply the customer with a copy of the Smart Alerts flyer.
- ☐ Describe Smart Alerts to the customer.
- ☐ Install Smart Alerts if requested.

PM Test Results Table

Test description	Before PM Service	After PM Service
Front detector output	N/A	249.1 Hz
Back detector output	N/A	19.9 pA
AUX 1 detector output	N/A	N/A
AUX 2 detector output	N/A	N/A
Test description	**Expected test result**	**Actual test result**
Leak and Restriction Test after front inlet maintenance	Pass	Pass
Leak and Restriction Test after back inlet maintenance	Pass	Pass
Leak and Restriction Test after front inlet Split Vent Trap replacement	Pass	Pass
Leak and Restriction Test after back inlet Split Vent Trap replacement	Pass	Pass
Front inlet pressure decay test	Pass	Pass
Back inlet pressure decay test	Pass	Pass

เอกสารไม่ควบคุม

Service Engineer Comments

If there are any specific points you wish to note as part of performing the service or other items of interest for the customer, please write include them in this box.

Service Completion

Service request number 6077959060 Date service completed 16 June 2025

Agilent signature [signature] Customer signature [signature] 16/June/2025

Total number of pages in this document 9 pages

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

CERTIFICATE OF CALIBRATION

Certificate No. : SP25-019 Page 1 of 5

Customer : United Analyst and Engineering Consultant Co.,Ltd. (Head Office)

Address : 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Location of calibration : Instrument room (207)

Equipment : UV-Vis Spectrophotometer

Manufacturer : Agilent Technologies

Model : Cary 60

Serial No. : MY15410009

ID No. : UAE.WAT.020/2558

Received Date : 26 May 2025

Calibration Date : 26 May 2025

Issue Date : 29 May 2025

Condition Instrument : Good

Calibrated by : (Mr.Tanawut Rittidach) Technical Manager

Approved by : (Ms.Chonticha Sangngern) Quality Manager

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the DQE Services Co., Ltd.

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP25-019 Page 2 of 5

Environment Condition : Ambient Temperature 25 ± 5 °C

Relative humidity 55 ± 20 %RH

Calibration method : In-house method CP-01 Based on ASTM E275-08

Certified Reference Materials :

Material	Serial No.	Certificate No.	Due date
Absobance Standard set	25760	115663	25 October 2025
Absobance Standard set	25757	115638	25 October 2025
Wavelength Standard set	25806	115657	25 October 2025
Wavelength Standard set	25758	115665	25 October 2025

Traceability : This certification is traceable to the International System of Unit maintained at National Institute of Standards and Technology (NIST) through Starna Scientific Limited

Spectral Band Width of UUC : 1.5 nm.

Scan Speed of UUC : 60 nm/min

Scan Interval of UUC : 0.15 nm.

Resolution of UUC : Photometric 0.0001 Abs.

Wavelength 0.1 nm.

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP25-019 Page 3 of 5

Calibration Results : Without adjustment

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
420	0.0000	0.0000	0.0000	0.0028	2.00
	0.5780	0.5739	0.0041	0.0031	2.00
	1.0484	1.0430	0.0054	0.0029	2.00
	2.1876	2.1876	0.0000	0.0084	2.00
440	0.0000	0.0000	0.0000	0.0028	2.00
	0.5595	0.5581	0.0014	0.0034	2.00
	1.0239	1.0219	0.0020	0.0035	2.00
	2.1230	2.1207	0.0023	0.0085	2.00
465	0.0000	0.0000	0.0000	0.0028	2.00
	0.5230	0.5190	0.0040	0.0029	2.00
	0.9633	0.9609	0.0024	0.0029	2.00
	1.9753	1.9719	0.0034	0.0079	2.00
546.1	0.0000	0.0000	0.0000	0.0028	2.00
	0.5181	0.5161	0.0020	0.0031	2.00
	1.0002	0.9979	0.0023	0.0033	2.00
	1.9973	2.0021	-0.0048	0.0102	2.00
590	0.0000	0.0000	0.0000	0.0028	2.00
	0.5517	0.5503	0.0014	0.0030	2.00
	1.0803	1.0808	-0.0005	0.0031	2.00
	2.0373	2.0324	0.0049	0.0105	2.00
635	0.0000	0.0000	0.0000	0.0028	2.00
	0.5591	0.5583	0.0008	0.0031	2.00
	1.0518	1.0513	0.0005	0.0030	2.00
	1.9274	1.9281	-0.0007	0.0102	2.00

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP25-019 Page 4 of 5

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
235	0.0000	0.0000	0.0000	0.0050	2.00
	0.7469	0.7488	-0.0019	0.0063	2.00
257	0.0000	0.0000	0.0000	0.0050	2.00
	0.8674	0.8663	0.0011	0.0067	2.00
313	0.0000	0.0000	0.0000	0.0050	2.00
	0.2919	0.2902	0.0017	0.0052	2.00
350	0.0000	0.0000	0.0000	0.0050	2.00
	0.6430	0.6428	0.0002	0.0063	2.00

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP25-019

Wavelength Accuracy :

CRMs Values (nm.)	UUC Reading (nm.)	Correction (nm.)	Uncertainty (nm.)	Coverage factor k
241.72	242.0	-0.28	0.18	2.00
279.45	279.5	-0.05	0.18	2.00
287.81	287.6	0.21	0.18	2.00
334.06	333.8	0.26	0.18	2.00
360.93	360.5	0.43	0.18	2.00
418.59	417.9	0.69	0.18	2.00
445.94	445.4	0.54	0.18	2.00
453.66	453.2	0.46	0.18	2.00
460.02	459.6	0.42	0.18	2.00
536.59	536.5	0.09	0.18	2.00
637.98	638.5	-0.52	0.18	2.00
431.38	430.7	0.68	0.18	2.00
472.50	472.3	0.20	0.18	2.00
513.47	513.5	-0.03	0.18	2.00
528.88	528.9	-0.02	0.18	2.00
573.17	573.8	-0.63	0.18	2.00
585.35	585.2	0.15	0.20	2.00
684.40	685.1	-0.70	0.18	2.00
740.72	741.1	-0.38	0.20	2.00
748.55	748.9	-0.35	0.18	2.00
807.03	807.1	-0.07	0.18	2.00
879.28	879.1	0.18	0.18	2.00

Remark : - UUC = Unit Under Calibration
- N/A = Not Avaiable
- The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%

- End of Certificate -

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP25-021

Environment Condition : Ambient Temperature 25 ± 5 °C

Relative humidity 55 ± 20 %RH

Calibration method : In-house method CP-01 Based on ASTM E275-08

Certified Reference Materials :

Material	Serial No.	Certificate No.	Due date
Absobance Standard set	25760	115663	25 October 2025
Absobance Standard set	25757	115638	25 October 2025
Wavelength Standard set	25806	115657	25 October 2025
Wavelength Standard set	25758	115665	25 October 2025

Traceability : This certification is traceable to the International System of Unit maintained at National - Institute of Standards and Technology (NIST) through Starna Scientific Limited

Spectral Band Width of UUC : 1.5 nm.

Scan Speed of UUC : 200 nm/min

Scan Interval of UUC : 0.1 nm.

Resolution of UUC : Photometric 0.001 Abs.

Wavelength 0.1 nm.

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

CERTIFICATE OF CALIBRATION

Certificate No. : SP25-021

Customer : United Analyst and Engineering Consultant Co.,Ltd. (Head Office)

Address : 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Location of calibration : Instrument room (207)

Equipment : UV-Vis Spectrophotometer

Manufacturer : HITACHI

Model : U-2900

Serial No. : 21E22-009

ID No. : UAE.WAT.051/2564

Received Date : 26 May 2025

Calibration Date : 26 May 2025

Issue Date : 29 May 2025

Condition Instrument : Good

Calibrated by : (Mr.Tanawut Rittidach) Technical Manager

Approved by : (Ms.Chonticha Sangngern) Quality Manager

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the DQE Services Co., Ltd.

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP25-021

Calibration Results : Without adjustment

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
420	0.0000	0.000	0.0000	0.0028	2.00
	0.5780	0.574	0.0040	0.0031	2.00
	1.0484	1.043	0.0054	0.0029	2.00
	2.1876	2.185	0.0026	0.0075	2.00
440	0.0000	0.000	0.0000	0.0028	2.00
	0.5595	0.558	0.0015	0.0034	2.00
	1.0239	1.022	0.0019	0.0035	2.00
	2.1230	2.121	0.0020	0.0079	2.00
465	0.0000	0.000	0.0000	0.0028	2.00
	0.5230	0.519	0.0040	0.0030	2.00
	0.9633	0.960	0.0033	0.0029	2.00
	1.9753	1.973	0.0023	0.0070	2.00
546.1	0.0000	0.000	0.0000	0.0028	2.00
	0.5181	0.516	0.0021	0.0031	2.00
	1.0002	0.998	0.0022	0.0033	2.00
	1.9973	1.995	0.0023	0.0084	2.00
590	0.0000	0.000	0.0000	0.0028	2.00
	0.5517	0.550	0.0017	0.0030	2.00
	1.0803	1.080	0.0003	0.0030	2.00
	2.0373	2.036	0.0013	0.0079	2.00
635	0.0000	0.000	0.0000	0.0028	2.00
	0.5591	0.558	0.0011	0.0031	2.00
	1.0518	1.051	0.0008	0.0030	2.00
	1.9274	1.926	0.0014	0.0080	2.00

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP25-021 Page 4 of 5

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
235	0.0000	0.000	0.0000	0.0050	2.00
	0.7469	0.748	-0.0011	0.0057	2.00
257	0.0000	0.000	0.0000	0.0050	2.00
	0.8674	0.866	0.0014	0.0059	2.00
313	0.0000	0.000	0.0000	0.0050	2.00
	0.2919	0.291	0.0009	0.0051	2.00
350	0.0000	0.000	0.0000	0.0050	2.00
	0.6430	0.640	0.0030	0.0055	2.00

เอกสารไม่ควบคุม

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

Certificate of Calibration

Cert.No.: 25CH1053
Page.: 1 of 2

Equipment :	Turbidity Meter
Manufacturer :	Oakton
Model :	T100IR
Serial No. :	1120501017
ID. No. :	UAE.WAT.056/2563
Condition As-Received:	Used Item
Received Date :	05 September 2025
Calibration Date :	08 September 2025
Reference :	2509-0212DSC-1
Submitted by :	United Analyst and Engineering Consultant Co.,Ltd. 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Ambient Temperature :	(23 ± 3.0) °C
Relative Humidity :	(50 ± 20) %
Calibration Procedure :	In - house method : CP-CH11 Direct measurement by using Formazin standard solution
Calibrated by :	Walalak Sinthean
Approved by :	Approved Signatory

( ) Chakrit Waewwanjua
( ) Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 9 September 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Calibration and Testing Equipment Services.

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP25-021 Page 5 of 5

Wavelength Accuracy :

CRMs Values (nm.)	UUC Reading (nm.)	Correction (nm.)	Uncertainty (nm.)	Coverage factor k
241.72	241.0	0.72	0.18	2.00
279.45	278.8	0.65	0.18	2.00
287.81	287.2	0.61	0.18	2.00
334.06	333.6	0.46	0.18	2.00
360.93	360.6	0.33	0.18	2.00
418.59	418.2	0.39	0.18	2.00
445.94	445.6	0.34	0.18	2.00
460.02	459.8	0.22	0.18	2.00
536.59	536.6	-0.01	0.18	2.00
637.98	638.0	-0.02	0.18	2.00
431.38	431.2	0.18	0.18	2.00
472.50	472.4	0.10	0.18	2.00
513.47	513.4	0.07	0.18	2.00
528.88	528.8	0.08	0.18	2.00
573.17	573.2	-0.03	0.18	2.00
585.35	585.0	0.35	0.20	2.00
684.40	684.4	0.00	0.18	2.00
740.72	741.0	-0.28	0.20	2.00
748.55	748.8	-0.25	0.18	2.00
807.03	807.2	-0.17	0.18	2.00
879.28	879.6	-0.32	0.18	2.00

Remark : - UUC = Unit Under Calibration
- N/A = Not Available
- The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor *k*, which for a normal distribution corresponds to a coverage probability of approximately 95%

- End of Certificate -

เอกสารไม่ควบคุม

Cert.No. : 25CH1053
Page. : 2 of 2

Condition of this calibration result

1. Reference Standard Instruments :

Instruments	ID No.	Certificate No.	Due date
1) Data Logger	130EC012	24H2043	23 Sep 2025
2) Liquid-in Glass Thermometer	130RC003	25I440	16 Apr 2026

- This measurement result is traceable to SI through Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials : Turbidity Standard solution (Formzin)
- The measurement results are traceable to SI through CPA chem Ltd..

Turbidity Solution	Manufacturer	Lot No.	Exp. date
20.0 NTU	CPA Chem	1088008	18 Mar 2026
100.0 NTU	CPA Chem	1088007	18 Mar 2026
400 NTU	CPA Chem	1088018	18 Mar 2026
800 NTU	CPA Chem	1088017	18 Mar 2026

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration result

Performing five - Formazin suspension standard curve by using 0, 20, 100, 400, 800 NTU
Tubidity Meter serial number : 1120501017

Standard Formazine suspension (NTU)	UUC* Reading (NTU)	Uncertainty of Measurement (± NTU)	Coverage Factor k
0	0.00	0.026	2.00
20.0	20.2	0.20	2.00
100.0	100	1.2	2.00
400	403	2.4	2.00
800	799	4.3	2.00

Remark - UUC* = Unit Under Calibration
- NTU = Nephelometric Turbidity Units

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม

สถาบันอาหาร
กลุ่มบริหารองค์ความรู้และนวัตกรรม
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

Calibration Certificate

Certificate No.: 2503287-001-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakhanong, Bangkok 10260

Equipment: Autoclave
Manufacturer: ALP
Model: CL-40L
Serial No.: 810010
ID No.: UAE.MIC.032/2565
Order No.: 2503287
Operation No.: 2503287-001
Date of Receipt: 5 June 2025
Date of Calibration: 5 June 2025

Calibrated by Mr.Pheraphat Tuanjit
Scientist

Approved by (Miss Preeyaporn Jaengkarnkit)
Vice President, Department of Laboratory Services
Responsible for the Technical Management Team

Date of Issue: 11 June 2025

The uncertainties are for a confidence probability of approximately 95 %.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

เอกสารไม่ควบคุม

2008 ซอยอุดมสุข 36 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel +66(0) 2422 8688 Fax +66(0) 2422 8545
nfi.or.th

สถาบันอาหาร
กลุ่มบริหารองค์ความรู้และนวัตกรรม
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

Calibration Report

Certificate No.: 2503287-001-01
Equipment: Autoclave
Model: CL-40L Serial No.: 810010
Resolution: 1 °C ID No.: UAE.MIC.032/2565
Manufacturer: ALP
Date of Calibration: 5 June 2025

Calibration point: 115 and 121 °C
Calibration result:

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
Min	25.8	52	225
Max	26.8	59	235

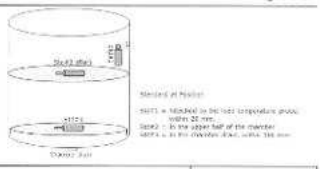


Table1 : Reporting of Temperature

Calibration Point	Measured Temperature (°C) @ Sensor No. (Sensor No.2 is REF)			Uncertainty
(°C)	Std.# 1	Std.# 2 (Ref)	Std.# 3	± (°C)
115	115.46	115.43	115.42	0.70
121	121.59	121.54	121.51	0.70

Table 2 : Reporting of Characterization Result

UUC* Setting	UUC* Reading				Stability	Uniformity	Overall Variation
(°C)	Min (°C)	Max (°C)	Average (°C)	MPa	± (°C)	(°C)	(°C)
115	115	115	115	0.08	0.24	0.17	0.50
121	121	121	121	0.12	0.24	0.19	0.52

Note
The quoted uncertainty include " Stability " and " Loading effect (20% of Uniformity)"
UUC* = Unit Under Calibration
Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.
Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
Overall Variation = The difference of the maximum and minimum measured temperatures througout observation time.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2, providing a level of confidence of approximately 95 %.

--------- End ---------

11 June 2025

เอกสารไม่ควบคุม

2008 ซอยอุดมสุข 36 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel +66(0) 2422 8688 Fax +66(0) 2422 8545
nfi.or.th

สถาบันอาหาร
กลุ่มบริหารองค์ความรู้และนวัตกรรม
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

Calibration Report

Certificate No.: 2503287-001-01
Equipment: Autoclave
Model: CL-40L Serial No.: 810010
Resolution: 1 °C ID No.: UAE.MIC.032/2565
Manufacturer: ALP
Date of Calibration: 5 June 2025

Location: Room 301 Media Preparation, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Environment Condition: Ambient Temperature (26 ± 1) °C
Relative Humidity (55 ± 5) %
Line Voltage (230 ± 5) Volt

Condition of this results of Calibration:

1. This instrument was calibrated by insert 3 standard Data loggers with RTD into its autoclave and calibration according to W-TE-018 based on BS 2646-1:2021, Autoclaves for sterilization in laboratories Part 1: Design, construction, safety and performance - Specification.
- The temperature scale used was based on ITS - 90.
- All data show below were final values and the initial data may be obtained upon request.

2. Reference Standard Instrument :

Instrument	Model	Serial No.	Certificate No.	Due Date	Through
Digital Thermometer with RTD (Data Logger)	HiTemp140-PT	T20827	NC 25-03-18-181	11-Mar-26	MADGETECH, INC.
	OM-CP-HITEMP-140	R58915	2502081-002-01	11-Mar-26	NATIONAL FOOD INSTITUTE
	PRTemp140	R38545	2501835-001-01	22-Feb-26	NATIONAL FOOD INSTITUTE

3. This certificate is traceable to International System of Units (SI Units).
4. This certificate was certified only for the instrument we calibrated.
5. This result of calibration was found accurate as shown on date and place of calibration only.
6. This standard does not apply to sterilizers or disinfectors used for medical, dental, pharmaceutical.
7. Condition of Calibrated item : Good
UUC Description : Setting program function sterilization : STERILIZE/NORMAL
Time of sterilization 20 Minute At 115 and 121 °C
8. Result of Calibration : [X] Without adjustment [ ] After adjustment

11 June 2025

เอกสารไม่ควบคุม

2008 ซอยอุดมสุข 36 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel +66(0) 2422 8688 Fax +66(0) 2422 8545
nfi.or.th

Agilent

Agilent AA Series Spectrometers

Preventative Maintenance Checklist

[redacted]

Foreword

Agilent Preventive Maintenance provides factory recommended service for your analytical systems to assure reliable operation and the accuracy of your results.

Delivered by highly trained and certified service engineers using genuine Agilent parts and supplies, Agilent Preventive Maintenance provides everything you need to reduce unplanned downtime and keep your systems operating at their peak. This checklist will be completed at the end of the service and provided to you as a record of the installation.

NOTE While non-current production AA instrument and or accessory models are not covered specifically in this document it can be used as a basic reference.

For more information about Agilent Technologies services please visit our web site using the following URL http://www.agilent.com/en-us/services

เอกสารไม่ควบคุม

Contents

Customer information 3
Service Engineer's Responsibilities 3
Other important Customer Web links 3
System information 4
Preparation, Safe operation and initial performance checks 4
Preventative maintenance procedures 5
- Flame systems 5
- Furnace systems 6
- Accessories 8
- Restore System 9
- Guidance 9

Signature Page 9
- Service Review 9
- Test Results 10
- AA consumable and parts list 10
- Service Engineer Comments (optional) 11

Service Completion 12

Agilent
เอกสารไม่ควบคุม

System information

☐ Check this box if an instrument configuration report is attached instead of completing this table.

Instrument system name and ID	240 FS AAS
Instrument system site and location	United Analyst and Engineering Consultant
List system component product numbers	List the serial numbers of each component
1 G 9432 A	1 MY 13160001
2	2
3	3
4	4
5	5
6	6
7	7
8	8
9	9
10	10

Preparation, Safe operation and Initial performance checks

☐ Agilent AA safe operation flow chart inspections (to determine if the PM can be performed).

NOTE If by following the flow chart the instrument is deemed to be unsafe for continued use you MUST NOT continue PM work. Inform the customer immediately of the Agilent recommendation that use of the instrument be discontinued.

☑ Discuss any specific questions or issues with the customer prior to starting.
☐ For HF application systems, if standard sample introduction system was not installed, ask the customer to install it. N/A
☑ Review the instrument logbook for recorded problems and comments.
☑ Save instrument control settings before starting the procedure.
☑ Perform a general inspection of the system for cleanliness.
☑ Check for proper installation of parts, assemblies, sensors etc.
☑ Check system for required installation of components, settings as defined by current Service Notes.

Agilent
เอกสารไม่ควบคุม

Customer information

- Customers should provide all necessary operating supplies upon request of the engineer.
- A customer representative should be available to the engineer while performing the preventive maintenance procedures.
- Any parts, not included in the Parts Lists section of this document, are not part of the recommended Preventive Maintenance service, nor are they included in the price of this service.
- If a system requires the use of extra or special procedures and/or parts for the maintenance service, then these must be ordered separately and charged as a repair, which may incur additional costs.

Service Engineer's Responsibilities

- Contact the customer and ensure that all necessary supplies are available before the preventive maintenance visit.
- Confirm the ability of the instrument to deliver continued safe operation as established via the Agilent AA safe operation flow chart. **(Refer directly to the AA 55/240/280 Preventive Maintenance Scope of Work to make this decision.)**
- Only select those pages that relate to the system or module being serviced.
- Complete empty fields with the relevant information.
- Complete the relevant checkboxes in the checklist using either a "X" or tick mark "√".
- Check "Section not applicable" check boxes to indicate services/tasks not delivered, as appropriate.
- Complete the Preventive Maintenance service in the order of the tasks listed.
- Complete the Service Review section together with the customer.
- Complete the fields for page numbers at the foot of each selected page.
- Complete the total number of pages field in the Service Completion section.
- Ask the customer to sign the Service Completion section including the customer's and your signature.

This information is subject to change without notice.

Other important Customer Web links

- How to get information on your product: Literature Library – http://www.agilent.com/chem/library
- Need to know more? www.agilent.com/chem/education
- Need technical support, FAQs? www.agilent.com/chem/techsupp
- Need supplies? www.agilent.com/chem/supplies

Agilent
เอกสารไม่ควบคุม

☑ Check for required firmware updates and verify with customers if they would like them installed.
☑ Use SVD to perform a Full Wavelength Scan for Cu HCL - "As found test_1"
☑ Perform a Basic Cu ABS test - "As found test_2"
☑ Print the Details page or screen captures of the test results and attach to the end of this checklist.

Preventative maintenance procedures

Flame systems

☐ Section NOT applicable.

Electronic components

☑ Review and confirm instrument configuration data in SVD.
☑ Confirm power supply voltages using the SVD Power Supply diagnostic.
☑ For Dual Beam instruments - Confirm RBC frequency using the SVD RBC frequency diagnostic.

Mechanical components

☑ Check the burner adjuster controls for complete and free movement. If the burner adjustor needs lubrication, use Molykote 321 or mineral-based molybdenum disulphide grease.
☑ Run SVD tests to exercise all motor drives over the full range of their travel.
- ☑ Monochromator drive
- ☑ Slit drive
- ☑ Lamp selector
- ☐ Automatic Burner Adjuster

Optics components

☑ Check that external optical surfaces are clean – Clean or replace as required.
☑ Use SVD and perform Mono Wavelength Correction.
☑ Use SVD and perform Slit Calibration.
☑ Use SVD and perform Grating Squareness Diagnostic.
☑ Use SVD and perform Zero Order Offset/Mono Correction.
☑ Use SVD and perform Wavelength Repeatability.
☑ Physically inspect selected HC lamps (customer to supply per their choice) and measure the % Gain for each lamp. Advise customer if lamps are showing emission degradation due to age.
☑ Check that the signal energy of the D2 and HC lamps track properly. Advise customer if their D2 lamp is showing emission degradation due to age.

Agilent
เอกสารไม่ควบคุม

Sample introduction and Atomization

- ☑ Inspect the burner interlock plate to ensure that the interlock pin is secure and correct for the burner type.
- ☑ Clean the burner slot with a clean white card.
- ☑ Check the uniformity of the slot width.
- ☑ Clean the burner if required.
- ☑ Change the burner o-ring and lubricate with PFPE grease.
- ☑ Clean the nebulizer, spray chamber and liquid trap.
- ☑ Change all o-rings and seals in the nebulizer, nebulizer block and spray chamber and lubricate.
- ☑ Check that the pressure relief bung releases readily.
- ☑ Change o-rings on the fuel and oxidant delivery barbs and lubricate.
- ☑ Leave the liquid trap EMPTY and verify the flame will not ignite in this state.
- ☑ Refill liquid trap and check that overfill drains freely into the drain/waste tube.
- ☑ Check the drain/waste tube for good drainage. It should not have tight bends, kinks or loops and the lower end must be above the liquid level in the waste vessel.
- ☑ Check and clean the igniter electrode.

Gas handling components and safety interlocks

- ☑ Pressure test for leaks
- ☑ Leak test gasbox internal components using gasbox leak tester G8434-67013
- ☑ Check safety interlock status and operation using the SVD interlock monitoring diagnostic.

Analytical performance for Flame systems

- ☑ Ignite a flame.
- ☑ Check that you can adjust the nebulizer uptake rate from 4 to 6.5 mL per minute.
- ☑ Optimize the instrument ready to perform Cu sensitivity test.
- ☑ Create a manual method to perform a Basic Cu ABS test - "Final Performance Testing."
- ☑ Run a PM completed sensitivity test for a 5 ppm copper sample and record the results in the AA PM Performance test results and measurements table.

Furnace systems

- ☑ Section NOT applicable.

Electronic components

- ☐ Review and confirm instrument configuration data in SVD.
- ☐ Confirm power supply voltages using the SVD Power Supply diagnostic.

Mechanical components

- ☐ Run SVD tests to exercise all motor drives over the full range of their travel.
  - ☐ Monochromator drive
  - ☐ Slit drive

Agilent
เอกสารไม่ควบคุม

Agilent AA Series Spectrometers Preventative Maintenance Checklist

Accessories

- ☐ Section NOT applicable.

Sample introduction pump system (SIPS) accessory

- ☑ Section NOT Applicable.
- ☐ Re-torque screws securing the hubs, presser arms and pump rotors.
- ☐ Adjust each roller so that it rotates freely.
- ☐ Wipe clean the pump rotor rollers and pump bands with a dry clean cloth.
- ☐ Ensure that the presser arms and the surfaces near the pump are free from dirt and spills.
- ☐ Remove the pump module rear cover and check for the incursion of liquids and any signs of corrosion.
- ☐ Re-torque the nuts that fasten the motor mounting plates to the chassis.
- ☐ Check clips securing the diluents holder and replace if necessary.
- ☐ Disconnect, clean T-piece, and reassemble the tubing using the following steps.
- ☐ Remove the T-piece by disconnecting the pump tubes, the pump bands and all other tubing.
- ☐ Place the T-piece in an ultrasonic bath containing strong detergent 1-5% Decon 30 or similar, for approximately 5-10 minutes.
- ☐ Wash the T-piece under a tap with a strong flow of water.
- ☐ Rinse with distilled water through all of the inlets in the reverse direction to normal sample flow.
- ☐ Reassemble.

Sample preparation system (SPS 4) accessory

- ☑ Section NOT Applicable.

The Agilent SPS 4 autosampler is designed to need minimal maintenance.

The following maintenance requirements are suggested to maintain the performance of the autosampler.

- ☐ Cleaning the spill tray, rack location mat, end frames and chassis accessories with a damp soft cloth and diluted mild detergent.
- ☐ Cleaning the autosampler cover panels with domestic window cleaner.
- ☐ Checking the X- axis and Z- axis drive belts for cracks, splits, damaged teeth, excessive fraying, color changes or degradation from fumes.
- ☐ Check the X- axis, Theta- axis and Z- axis FFC cables for cracks, incorrect positioning, damaged edge or damaged connectors.

NOTE The autosampler requires no extra lubrication throughout its lifetime.

For further details refer to the SPS 4 service manual G8410-90050.

Revision: 12.0, Issued: November 2025
Document Number: D0140117
© Agilent Technologies, Inc. 2025

Agilent
เอกสารไม่ควบคุม

Agilent AA Series Spectrometers Preventative Maintenance Checklist

- ☐ Lamp selector

Optics components

- ☐ Check that external optical surfaces are clean – Clean or replace as required.
- ☐ Use SVD and perform Mono Wavelength Correction.
- ☐ Use SVD and perform Slit Calibration.
- ☐ Use SVD and perform Grating Squareness Diagnostic.
- ☐ Use SVD and perform Zero Order Offset/Mono Correction.
- ☐ Use SVD and perform Wavelength Repeatability.
- ☐ Physically inspect selected HC lamps (customer to supply per their choice) and measure the % Gain for each lamp. Advise customer if lamps are showing emission degradation due to age.

Gas handling, water system, and workhead component checks

- ☐ Inspect the GTA workhead gas hoses and connections for leaks.
- ☐ Pressure test for gas leaks
- ☐ If the cooler system is accessible (stand-alone) check for correct operation and coolant/water level – this includes any temperature and pressure settings plus filter cleaning (air flow and water).
- ☐ Inspect the GTA workhead water hoses and connections for leaks.
- ☐ Check all graphite components and replace if necessary.
  - ☐ Tube
  - ☐ Electrodes
  - ☐ Shroud
- ☐ Check and clean the end windows on the workhead.
- ☐ Check safety interlock operation.

Analytical performance for Furnace systems

- ☐ Optimize the instrument ready to perform Cu sensitivity test.
- ☐ Run the sensitivity test for a 25 ppb copper sample and record the results in the results table.

PSD autosampler accessory for Furnace systems

- ☑ Section NOT applicable.
- ☐ Check condition of the PSD capillary – replace if necessary
- ☐ Check condition and operation of PSD syringe – ensure it does not have air locks and bubbles.
- ☐ Change PSD rinse bottle o-ring.
- ☐ Check and clean the rinse vessel.
- ☐ Check the drain tube for good drainage. It should not have tight bends, kinks or loops and the lower end must be above the liquid level in the waste vessel.
- ☐ Ensure that the waste vessel is suitable for use with the furnace system.

Revision: 12.0, Issued: November 2025
Document Number: D0140117
© Agilent Technologies, Inc. 2025

Agilent
เอกสารไม่ควบคุม

Agilent AA Series Spectrometers Preventative Maintenance Checklist

Vapor generation accessory VGA (hydride generator)

- ☐ Section NOT Applicable.
- ☐ Inspect VGA gas supply hose.
- ☐ Inspect/replace VGA pump tubing.
- ☐ Check low gas pressure interlock setting– adjust if required.
- ☐ Check precision orifice gas flow setting – adjust if required.
- ☐ Check gas regulator pressure to 46 psi (325 kPa) – adjust if required.
- ☐ Clean the exterior surfaces of the accessory with soft lint free cloth. This cloth can be dampened with warm water or a mild detergent. Do not use organic solvents or abrasive cleaning agents.

UltrAA Lamp Accessory (external)

- ☑ Section NOT Applicable.
- ☐ Check the condition of the power cable.
- ☐ Clean the exterior surfaces of the accessory with soft lint free cloth. This cloth can be dampened with warm water or a mild detergent. Do not use organic solvents or abrasive cleaning agents.

Restore System

- ☐ If you have altered the customer's instrumentation during the course of PM, restore to the original status to allow the customer to conduct their normal activities (e.g., reload the customer's method.)

Guidance

If the PM service is performed prior to a qualification service, then use the qualification procedure as a guide for final instrument set up and checkout.

Signature Page

Service Review

- ☐ Attach available reports/printouts of all tests to this documentation.
- ☐ Record the Preventive Maintenance service activity in the customer's records/logbook.
- ☐ Update/reset instrument maintenance counters as appropriate.
- ☐ Affix the PM sticker to the system or instrument logbook based on the customer's request.
- ☐ Complete the Service Engineer Comments section if there are additional comments.
- ☐ Review this service, parts replaced, and test results obtained with the customer.
- ☐ If the instrument firmware was updated, record the details of the change in the Service Engineer's Comments box or if necessary, in the customer's IQ records.

Revision: 12.0, Issued: November 2025
Document Number: D0140117
© Agilent Technologies, Inc. 2025

Agilent
เอกสารไม่ควบคุม

Test Results

Test description	Expected test result:	Actual test result
Flame optics PMT Gain test		
For copper at 324.8 nm, 4 mA, 0.5 nm slit width	< 55 %	46 %
Flame performance test with 5 ppm copper sample		
Air /acetylene, mixing paddle removed	Abs value > 0.3	0.6331
Air /acetylene, mixing paddle installed 10 replicates	%RSD < 1.0	0.71
Deuterium furnace optics PMT Gain test		
For copper at 324.8 nm, 4 mA, 0.5 nm slit width	< 55 %	-
Deuterium furnace performance test with 25 ppb copper sample (324.8 nm)		
Precision %RSD	≤ 4.0%	-
Abs value	≥ 0.15	-
Zeeman furnace analytical performance: 25 ppb copper sample (324.8 nm)		
Precision %RSD	≤ 4.0%	-
Abs value	≥ 0.15	-
MSR% (327.4 nm)	≥70 %	-

AA consumable and parts list

Part Description	Part Number	Product/Model # where used	PM supplied or Consumable	Instrument-Type
Test Solution – Cu 5ppm solution	6510030100	55 240 280	PM supplied	Common
Test Solution - Blank solution	5190-7007	55 240 280	PM supplied	Common
Copper, 1000 ug/ml, 100ml	5190-8279	55 240 280	*	Common
Kit, Mk 7 O-rings, aqueous, complete set	9910093400	55 240 280	PM supplied	Flame
Organic Kit	9910093500	55 240 280	PM supplied	Flame
Wire Nebulizer Cleaning	9910024700	55 240 280	consumable	Flame
Tubing-Capillary Std Nebs	9910024800	55 240 280	consumable	Flame
Capillary Tube Hivac Neb (3) (organics only)	9910044000	55 240 280	consumable	Flame
Glass impact beads (5/pk)	9910025700	55 240 280	consumable	Flame

Agilent

เอกสารไม่ควบคุม

Service Completion

Service Request Number: 6009809466
Service Engineer Name: Kanyakorn S
Service Engineer Signature: Kanyakorn S.
Date of Service Completion: 26 Jan 2026
Customer Name: Jamida Hanjo
Customer Signature:

Agilent

เอกสารไม่ควบคุม

Teflon impact beads (5/pk): (organics only)	9910053900	55 240 280	consumable	Flame
Burner cleaning strip (100/pk)	9910053900	55 240 280	consumable	Flame
Window UV silica – round (right side)	2010082600	55 240 280	PM supplied	Common
Window UV silica – rectangular (left side)	2010082500	55 240 280	PM supplied	Common
Pad adhesive window (round)	4910012700	55 240 280	PM supplied	Common
Pad adhesive window (rectangular)	4910012800	55 240 280	PM supplied	Common
Electrode kit (1 pr) (D2)	6310003400	GTA120	PM supplied	Furnace
Shroud (D2)	6310003100	GTA120	PM supplied	Furnace
Zeeman electrode kit (1 pr)	5310003500	GTA120	PM supplied	Furnace
Zeeman shroud	6310003600	GTA120	PM supplied	Furnace
O-ring PSD rinse bottle	6910025900	PSD120	PM supplied	Furnace

* For engineers who only service AA instruments: 5190-8279 can be used as a cheaper alternative for 5610030100.

Items classified as PM supplied in the above table are included in the standard PM.

Those classified as consumable should be provided by the customer or charged to the customer if supplied by the Agilent service engineer.

Service Engineer Comments (optional)

If there are any specific points you wish to note as part of performing the installation or other items of interest for the customer, please write them in this box.

Agilent

เอกสารไม่ควบคุม

SVD Results Report

VARIAN

Report ID:3 *Diagnostic Start Time:1/26/2026 8:39:56 AM* *Diagnostic End Time:1/26/2026 9:05:49 AM*

Customer: UAE *Service Engineer:* Kanyakorn S.

Address: *Contact Details:* 0263763631

Instrument Configuration

Configuration:

Serial Number:	MY13160001	**Turret Type:**	Automatic
Instrument Model:	Varian AA140/240/280	**Number Of Lamps:**	4
Flame Instrument:	True	**Mono Type:**	Automatic
Furnace Instrument:	True	**Gasbox Type:**	'Y' Gas Box
Zeeman Present:	False	**Auto Burner Adjuster:**	False
Internal Zeeman:	False	**Mains Frequency:**	50
Internal UltrAA:	False	**Firmware Version:**	2.11
Optics Type:	Double Beam	**Photomultiplier Type:**	Normal(900nm)
D2 BG Correction Fitted:	True	**PWB Version:**	45
Boot Block Version:	1.09		

EEPROM Data:

Instrument Run Hours:	79270.902	**D2 Run Hours:**	58906.000
Zero Wavelength Offset:	30.095	**D2 Serial Number:**	not set !
Mono Correction:	0.765	**D2 Install Date:**	1/1/1970
Flame Hours:	35125.582	**D2 Original Intensity:**	1.000
		D2 Last Intensity:	475.000

Frequency:

Averaging Period: 30.0
Datapoint Count: 20

Upper Limit: 51.00		**Highest Measured Frequency:** 50.00
	Average Frequency: 50.00	
Lower Limit: 49.00		**Lowest Measured Frequency:** 50.00

Result: Passed

เอกสารไม่ควบคุม

Power Supply:

Averaging Period: 30.0
Datapoint Count: 20

	Lower Limit (V)	Actual (V)	Upper Limit (V)	Result:
12.00 V Rail	10.80	12.20	13.20	Passed
-12.00 V Rail	-13.20	-11.90	-10.80	Passed
5.00 V Rail	4.50	5.02	5.50	Passed
310.00 V Rail	279.00	320.00	341.00	Passed

เอกสารไม่ควบคุม

Wavelength Repeatability:

Lamp Used: Copper
Lamp Current(mA): 4
Peak Used(nm): 324.750
Slit Width(nm): 0.2
Connected to Socket: 3
Slit Height: Normal

Lamp Alignment: Performed

Lower Limit(nm) 324.768 324.888 Upper Limit(nm)

(Approach from Zero Order)	(Approach from end)
Sample 1: 324.828	Sample 2: 324.823
Sample 3: 324.823	Sample 4: 324.823
Sample 5: 324.823	Sample 6: 324.819
Sample 7: 324.823	Sample 8: 324.819
Sample 9: 324.819	Sample 10: 324.819

Mean: 324.823 Standard Deviation: 0.003


Result: Passed

เอกสารไม่ควบคุม

Optics

Beam Balance:

Lamp Type: Copper
Peak Selected: 324.80
Lamp Socket Used: 3
Lamp Alignment: Performed

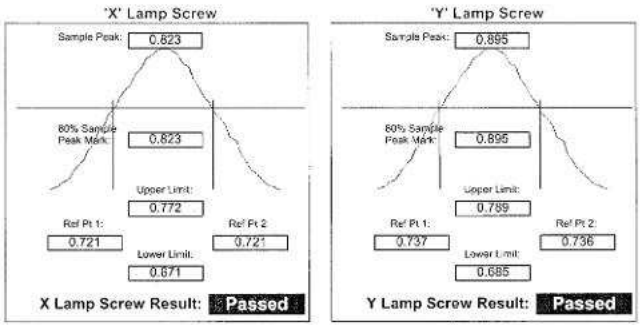

X Lamp Screw Result: Passed
Y Lamp Screw Result: Passed

Grating Squareness:

Lamp Element(s): Copper
Lamp Turret Position: 3
Lamp Current(mA): 4.00
Slit Width(nm): 0.5
1st Order Wavelength(nm): 324.80
Lamp Alignment: Performed

	Lower Limit (nm)	Actual (nm)	Upper Limit (nm)	Result:
Zero Order	-0.10	0.00	0.10	Passed
First Order	324.45	324.74	325.15	Passed
Second Order	649.23	649.50	649.97	Passed

เอกสารไม่ควบคุม

Mechanical

Wavelength Drive: Passed

Slit Drive: Passed

Turret Drive: Passed

Auto Burner Adjuster Drive: Untested

Miscellaneous

Signal Processing Linearity:

Calculate Mode: New Calc Mode

	Lower Limit	Actual	Upper Limit	Result:
S0	114	261	297	Passed
S1	156	165	191	Passed
S2	271	296	332	Passed
S3	474	508	579	Passed
S4	825	919	1008	Passed
S5	1435	1529	1754	Passed
S6	2498	2771	3053	Passed
S7	4347	4755	5313	Passed

Interlocks:

Burner Fitted: Working
N2O Burner Fitted: Untested
Flame Shield Closed: Working
Gas Control Fitted: Untested
Pressure Release Bung Fitted: Working
Liquid Trap Fitted: Working
Flame Detect: Working
GCU Active: Working
Oxidant Pressure: Working
Oxidant Changeover: Untested
Ignition: Working

เอกสารไม่ควบคุม

Auto Lamp Recognition:

Lamp 1: 87 - Silver/Cadmium/Lead/Zinc(Ultr/AA) (Ag/C
Lamp 2: 68 - Zinc (Zn)
Lamp 3: 14 - Copper (Cu)
Lamp 4: Uncoded Lamp/Not Connected
Lamp 5: Not Supported
Lamp 6: Not Supported
Lamp 7: Not Supported
Lamp 8: Not Supported

Result: Passed

GTA Temperature Monitoring:

Not Performed

Notes:

Signatures:

Jawida Hayi	26 Jan 26	Kanyakorn S.	26 Jan 2026
UAE	Date	Kanyakorn S.	Date

Sequential by time report 1/26/2026 10:15 AM SpectrAA
Page 1 of 1

Analyst
Date Started 1/26/2026 9:07 AM GMT: 1/26/2026 2:07 AM
Worksheet Precision Test
Comment
Methods Cu
Computer name DESKTOP-RSUIFRS
Serial Number: MY13160001

Method: Cu (Flame)

Sample ID	Exp Abs	%RSD	Mean Abs		
5 ppm Cu	0.618	0.7	0.6180		
	Readings				
	0.6145	0.6187	0.6081	0.6158	0.6253	0.6196
	0.6197	0.6195	0.6188	0.6189	1/26/2026	

Report Generated At: 1/26/2026 9:05:42 AM 6 SVD Results Report

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

Sequential by time report 1/26/2026 9:54 AM SpectrAA
Page 1 of 1

Analyst
Date Started 1/26/2026 9:07 AM GMT: 1/26/2026 2:27 AM
Worksheet Sensitivity Test
Comment
Methods Cu
Computer name DESKTOP-RSUIFRS
Serial Number: MY13160001

Method: Cu (Flame)

Sample ID	Exp Abs	%RSD	Mean Abs	
5 ppm Cu	0.633	1.4	0.6331	
	Readings			
	0.6413	0.6340	0.6241	1/26/2026

เอกสารไม่ควบคุม

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

ilac-MRA
NSC-TISI-TIS17025 CALIBRATION 0005

Certificate of Calibration

Cert.No.: 26CH144
Page.: 1 of 3

Equipment :	Conductivity Meter
Manufacturer :	Horiba
Model :	LAQUA-EC210
Serial No. :	HC9L0013
ID No. :	UAE.EFM.011/2563(EFM.SCT.05/63)
Condition As-Received:	Used Item
Received Date :	02 February 2026
Calibration Date :	03 February 2026
Reference :	2602-0038WSC-3
Submitted by :	United Analyst and Engineering Consultant Co.,Ltd. 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure:	In -house method : - CP-CH6 by direct measurement with certified reference material (CRM) - CP-CH8 by comparison with temperature standard
Calibrated by :	Walalak Sirithean
Approved by :	Approved Signatory

( ) Chakrit Waewwanjua
( ) Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 04 February 2026

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Condition of this result of calibration

1. Reference Standard Instrument :-

Instrument	Serial No.	ID No.	Certificate No.	Due date
1) Thermometer	9549224	130RC003	25I440	16 Apr 2026
2) Ref. Std.Thermometer	4982054	110RC044	25I708	03 July 2026

- This measurement result is traceable to SI throught Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials :-
   - Conductivity calibration solution, CPA chem Ltd., The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Conductivity Solution	Manufacturer	Lot No.	Exp. date
1413.5 µS/cm	CPA Chem	1150497	30 Oct 2026
12.881 mS/cm	CPA Chem	1081099	11 Mar 2026

   - Control Conductivity calibration solution temperature by Water bath (25 ± 0.1) °C

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration results

Function : Conductivity Measurement

(*) After Adjustment at 1413.5 µS/cm

Conductivity Electrode Serial No.: 9B9F0286

Standard Conductivity Solution	Before Adjustment UUC* Reading	After Adjustment UUC* Reading	Uncertainty of Measurement (±)	Coverage factor *k*
1413.5 µS/cm	1431 µS/cm	1413 µS/cm	9.2 µS/cm	2.00
12.881 mS/cm	12.92 mS/cm	12.76 mS/cm	0.086 mS/cm	2.00

Remark : **- UUC* = Unit Under Calibration**

สุสลาหกรรมพัฒนาอุตสาหกรรมอาหาร
ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center
ilac-MRA
NSC-TISI-TIS 17025 CALIBRATION 0061

Calibration Certificate

Certificate No.: 2503287-002-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road, Bangchack, Prakhanong, Bangkok 10260

Equipment: CHAMBER (Incubator)
Manufacturer: BINDER
Model: KB 400
Serial No.: 20220000000391
ID No.: UAE.MIC.029/2565
Order No.: 2503287
Operation No.: 2503287-002
Date of Receipt: 5 June 2025
Date of Calibration: 5 June 2025

Calibrated by Mr.Pheraphat Tuanjit, Scientist
Approved by (Miss Preeyaporn Jaengkarnkit), Vice President, Department of Laboratory Services, Responsible for the Technical Management Team
Date of Issue: 11 June 2025

The uncertainties are for a confidence probability of approximately 95 %.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

เอกสารไม่ควบคุม
2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพมหานคร
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel. +66(0) 2422 8688 Fax. +66(0) 2422 8545
nfi.or.th

Calibration Results

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe:
- Model : 9383
- Serial No. : 9B9F0286

Dimension of probe:
- Length : 110 mm
- Diameter : 16 mm
- Immersion Depth : 100 mm

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of Measurement (± °C)	Coverage factor *k*
15.0	15.002	15.0	-0.002	0.13	2.00
30.0	30.001	30.0	-0.001	0.13	2.00
45.0	45.001	45.0	-0.001	0.13	2.00

Remark : - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

สุสลาหกรรมพัฒนาอุตสาหกรรมอาหาร
ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center
ilac-MRA
NSC-TISI-TIS 17025 CALIBRATION 0061

Calibration Report

Certificate No.: 2503287-002-01
Equipment: CHAMBER (Incubator)
Model: KB 400 Serial No.: 20220000000391
Resolution: 0.1 °C ID No.: UAE.MIC.029/2565
Manufacturer: BINDER
Date of Calibration: 5 June 2025

Location: Room 302 Microbiology Laboratory, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Environment Condition:
Ambient Temperature (18 ± 1) °C
Relative Humidity (53 ± 6) %
Line Voltage (230 ± 5) Volt

Condition of this results of Calibration:

1. This instrument was calibrated by insert 13 standard thermometer into its chamber and calibration according to W-TE-014 Based on TLAS G-20-1/02-08 (E): Guidelines for Calibration and Checks of Temperature Controlled Enclosures.
   - The temperature scale used was based on ITS - 90.
   - All data show below were final values and the initial data may be obtained upon request.
2. Reference Standard Instrument :

Instrument	Model	Serial No./ID No.	Certificate No.	Due Date	Through
Digital Thermometer with sensor	34972A	MY59003377	2501168-001-01	13 January 2026	NATIONAL FOOD INSTITUTE
	RTD	CH#101-203 / RTD#101-203			

3. This certificate is traceable to International System of Units (SI Units).
4. This certificate was certified only for the instrument we calibrated.
5. This result of calibration was found accurate as shown on date and place of calibration only.
6. Condition of Calibrated item : Good
   UUC Description :
   Time of Record 1 Hour 9 Minute At 35.0 °C
   Fresh air Damper [-] Open Position [-]
   [X] Close Fan [100%]
   [-] Not Available
7. Result of Calibration : [X] Without adjustment [ ] After adjustment

11 June 2025

เอกสารไม่ควบคุม
2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพมหานคร
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel. +66(0) 2422 8688 Fax. +66(0) 2422 8545
nfi.or.th

nfi สถาบันอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

ilac-MRA
NSC-TISI-TIB 17025 CALIBRATION 0061

Calibration Report

Certificate No.: 2503287-002-01

Equipment: CHAMBER (Incubator)

Model: KB 400 Serial No.: 20220000000391

Resolution: 0.1 °C ID No.: UAE.MIC.029/2565

Manufacturer: BINDER

Date of Calibration: 5 June 2025

Calibration point: 35.0 °C

Calibration result:

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
MIN	17.4	48	225.0
MAX	18.5	59	235.0




Table1 : Reporting of Temperature

Calibration point	Measured Temperature (°C) @ Sensor No. (Sensor No.13 is REF)												Uncertainty
(°C)	# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9	# 10	# 11	# 12	# 13	± (°C)
35.0	35.08	35.11	35.01	35.13	35.17	35.09	34.98	34.89	35.15	35.05	35.06	34.89	35.06	0.27

Table 2 : Reporting of Characterization Result

UUC* Setting	UUC* Reading (°C)			Temperature Stability	Temperature Uniformity	Overall Variation
(°C)	MIN	MAX	Average	± (°C)	(°C)	(°C)
35.0	35.0	35.1	35.0	0.038	0.17	0.34

Note: The quoted uncertainty include " Stability " and " Loading effect (20% of Temp Uniformity) "

UUC* = Unit Under Calibration

Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.

Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.

Overall Variation = The difference of the maximum and minimum measured temperatures throughout observation time.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2, providing a level of confidence of approximately 95 %.

--------- End ---------

17 June 2025

F-CS-012 Revision: 01 Date: 20-04-65

เอกสารไม่ควบคุม

อุตสาหกรรมอาหาร 2008 ซอย 86 ถนนอรุณอมรินทร์ แขวงบางยี่เรือ เขตธนบุรี กรุงเทพมหานคร 10600
2008 Soi 86, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel +66(0) 2422 8608 Fax +66(0) 2422 8545
nfi.or.th

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP25-024

Environment Condition : Ambient Temperature 25 ± 5 °C

Relative humidity 55 ± 20 %RH

Calibration method : In-house method CP-01 Based on ASTM E275-08

Certified Reference Materials :

Material	Serial No.	Certificate No.	Due date
Absobance Standard set	25760	115663	25 October 2025
Absobance Standard set	25757	115638	25 October 2025
Wavelength Standard set	25806	115657	25 October 2025
Wavelength Standard set	25758	115665	25 October 2025

Traceability : This certification is traceable to the International System of Unit maintained at National - Institute of Standards and Technology (NIST) through Starna Scientific Limited

Spectral Band Width of UUC : 5.0 nm.

Scan Speed of UUC : 40

Scan Interval of UUC : 0.1 nm.

Resolution of UUC : Photometric 0.001 Abs.

Wavelength 0.1 nm.

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

CERTIFICATE OF CALIBRATION

Certificate No. : SP25-024

Customer : United Analyst and Engineering Consultant Co.,Ltd. (Head Office)

Address : 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Location of calibration : Instrument room (207)

Equipment : UV-Vis Spectrophotometer

Manufacturer : HITACHI

Model : U-5100

Serial No. : 23A4-008

ID No. : UAE.WAS.010/2567

Received Date : 17 June 2025

Calibration Date : 17 June 2025

Issue Date : 20 June 2025

Condition Instrument : Good

Calibrated by : (Mr.Tanawut Rittidach) Technical Manager

Approved by : (Ms.Chonticha Sangngern) Quality Manager

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the DQE Services Co., Ltd.

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP25-024

Calibration Results : Without adjustment

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
420	0.0000	0.000	0.0000	0.0028	2.00
	0.5780	0.574	0.0040	0.0031	2.00
	1.0484	1.044	0.0044	0.0029	2.00
	2.1876	2.185	0.0026	0.0075	2.00
440	0.0000	0.000	0.0000	0.0028	2.00
	0.5595	0.558	0.0015	0.0035	2.00
	1.0239	1.021	0.0029	0.0035	2.00
	2.1230	2.122	0.0010	0.0079	2.00
465	0.0000	0.000	0.0000	0.0028	2.00
	0.5230	0.519	0.0040	0.0030	2.00
	0.9633	0.961	0.0023	0.0029	2.00
	1.9753	1.975	0.0003	0.0071	2.00
546.1	0.0000	0.000	0.0000	0.0028	2.00
	0.5181	0.515	0.0031	0.0031	2.00
	1.0002	0.996	0.0042	0.0033	2.00
	1.9973	1.994	0.0033	0.0084	2.00
590	0.0000	0.000	0.0000	0.0028	2.00
	0.5517	0.549	0.0027	0.0030	2.00
	1.0803	1.078	0.0023	0.0030	2.00
	2.0373	2.031	0.0063	0.0082	2.00
635	0.0000	0.000	0.0000	0.0028	2.00
	0.5591	0.557	0.0021	0.0031	2.00
	1.0518	1.049	0.0028	0.0030	2.00
	1.9274	1.924	0.0034	0.0081	2.00

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP25-024

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor *k*
235	0.0000	0.000	0.0000	0.0050	2.00
	0.7469	0.747	-0.0001	0.0057	2.00
257	0.0000	0.000	0.0000	0.0050	2.00
	0.8674	0.864	0.0034	0.0059	2.00
313	0.0000	0.000	0.0000	0.0050	2.00
	0.2919	0.293	-0.0011	0.0051	2.00
350	0.0000	0.000	0.0000	0.0050	2.00
	0.6430	0.639	0.0040	0.0055	2.00

เอกสารไม่ควบคุม

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

ilac-MRA
NSC-TISI-TIS17025 CALIBRATION 0008

Certificate of Calibration

Cert.No.: 25CH606

Equipment :	pH Meter
Manufacturer :	Horiba
Model :	LAQUA-PH210
Serial No. :	HA0A0006
ID No. :	UAE.EFM.006/2563(EFM.pH.06/03)
Condition As-Received:	Used Item
Received Date :	26 May 2025
Calibration Date :	27 May 2025
Reference :	2505-0796WSC-1
Submitted by :	United Analyst and Engineering Consultant Co.,Ltd. 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure :	In - house method : - CP-CH5 by direct measurement with DC voltage standard and direct measurement with certified reference material (CRM) - CP-CH8 by comparison with temperature standard
Calibrated by :	Warakorn Lerngagtrakul
Approved by :	Saithip Approved Signatory

( ) Chakrit Waewwanjua
( ) Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 28 May 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP25-024

Wavelength Accuracy :

CRMs Values (nm.)	UUC Reading (nm.)	Correction (nm.)	Uncertainty (nm.)	Coverage factor *k*
241.00	240.4	0.60	0.18	2.00
279.30	278.8	0.50	0.18	2.00
288.90	288.3	0.60	0.18	2.00
334.50	333.9	0.60	0.18	2.00
361.40	360.8	0.60	0.18	2.00
418.40	417.9	0.50	0.18	2.00
447.20	446.6	0.60	0.18	2.00
459.30	459.1	0.20	0.18	2.00
537.00	536.4	0.60	0.18	2.00
638.00	637.5	0.50	0.18	2.00
441.29	440.7	0.59	0.18	2.00
479.88	479.4	0.48	0.18	2.00
513.75	513.3	0.45	0.18	2.00
528.59	528.2	0.39	0.18	2.00
575.10	574.5	0.60	0.18	2.00
585.56	585.4	0.16	0.20	2.00
684.70	684.1	0.60	0.18	2.00
740.51	740.2	0.31	0.20	2.00
747.61	747.0	0.61	0.18	2.00
807.04	806.4	0.64	0.18	2.00
879.68	879.1	0.58	0.18	2.00

Remark : - UUC = Unit Under Calibration
- N/A = Not Available
- The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor *k*, which for a normal distribution corresponds to a coverage probability of approximately 95%

- End of Certificate -

เอกสารไม่ควบคุม

Condition of this calibration result

1. Reference Standard Instrument

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1) Document Process Calibrator	54030049	130RC116	24E2759	25 Aug 2025
2) Ref. Standard Thermometer	4982054	110RC044	24I757	14 July 2025

- This measurement result is traceable to SI throught Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials :The measurement results are traceable to SI through Hach Lenge GmbH Ltd., Deutsche Akkreditierungsstelle, Accredited No.D-RM-15184-01-00
: The measurement results are traceable to SI through CPA chem Ltd., Deutsche Akkreditierungsstelle, Accredited No.D-RM-15184-01-00

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.007	CPA chem	1066665	18 Jan 2027
pH 7.000	Hach Lenge GmbH	C03232	02 Dec 2026
pH 10.010	CPA chem	1066669	18 Jan 2026

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4,7)(7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement	Coverage factor
	pH	mV	mV	pH	(±mV)	*k*
pH Meter	4.00	177.48	177.5	4.01	0.058	2.00
S/N.: HA0A0006	7.00	0.00	0.0	7.00	0.058	2.00
	7.00	0.00	0.0	7.00	0.058	2.00
	10.00	-177.48	-177.4	10.01	0.058	2.00

เอกสารไม่ควบคุม

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7)(7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (±)	Coverage factor *k*
pH Electrode S/N.: Q92M0159	4.007	4.01	181.7	0.0071	2.00
	7.000	7.00	6.4	0.0085	2.00
	7.000	7.00	6.5	0.0092	2.00
	10.010	10.00	-168.7	0.0095	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : 9652-10D
- Serial No. : Q92M0159

Dimension of probe

- Length : 103 mm.
- Diameter : 16 mm.
- Immersion Depth : 80 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (± °C)	Coverage factor *k*
15.0	15.002	15.0	-0.002	0.13	2.00
30.0	30.003	30.0	-0.003	0.13	2.00
45.0	45.003	45.0	-0.003	0.13	2.00

Remark - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม

Condition of this result of calibration

1. Reference Standard Instruments :
   This measurement result is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

Instruments	ID No.	Certificate No.	Due Date
1. Burette	130BU10	25CG1126	18 Mar 2027
2. Balance	110RC001	25MM316	02 July 2026

2. Standard Material :-

Material	Manufacturer	Lot.No.	Assay
Sodium Thiosulfate 5-Hydrate AR	KEMAUS	2203162447	99.6%

Result : **Dissolved Oxygen Meter Adjustment With Air 100 %**
Dissolved Oxygen Probe No.: 22M102385

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.22	8.31	0.0055

This report was certified only for the instrument we tested.It is allowable to use for study Intend to use for advertising and referral purpose is prohibited.This report may not be reproduced other in full, without written approval of the laboratory

-o0o-

เอกสารไม่ควบคุม

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000 FAX. 0-2719-9484

Certificate of Testing

Equipment :	DO Meter
Manufacturer :	YSI
Model :	4010-2W
Serial No. :	20260326
ID No. :	UAE.WAO.060/2563
Received Date :	17 October 2025
Test Date :	22 October 2025
Reference :	2510-0505DSC-1
Submitted by :	United Analyst and Engineering Consultant Co.,Ltd. 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Laboratory Condition :	Temperature (25 ± 5) °C Humidity (50 ± 20) %
Test Procedure :	In - house method : CP-CH9 by Comparison Technique with Azide Modification Method
Tested by :	Walalak Sirithean
Approved by :	Approved Signatory

( ) Chakrit Waewwanjua
( ) Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 23 October 2025

เอกสารไม่ควบคุม

Agilent CrossLab
From Insight to Outcome

Agilent CrossLab Start Up Services

Agilent 5100 5110 ICP-OES Preventive Maintenance

Agilent Preventive Maintenance provides factory recommended service for your analytical instruments to assure reliable operation and the accuracy of your results

Delivered by highly trained and certified service engineers using genuine Agilent parts and supplies, Agilent Preventive Maintenance provides what you need to reduce unplanned downtime and keep your systems operating at their peak performance.

This checklist is used as a guide for completing the preventive maintenance tasks. A signed copy of this checklist is provided for your records

Revision: A.02, Issued: 21 January 2022
Document Number: G8014-90275
© Agilent Technologies, Inc. 2022

Agilent

เอกสารไม่ควบคุม

Introduction

Customer Information

- Customers should provide all necessary operating supplies upon request of the engineer.
- A customer representative should be available to the engineer while performing the preventive maintenance procedures. Customers are responsible for regular maintenance and are encouraged to observe the service representative.
- Any parts not included in the Parts Lists section of this document are not part of the recommended Preventive Maintenance service nor are they included in the price of this service.
- If a system requires the use of extra or special procedures and/or parts for the maintenance service, then these must be ordered separately and charged as a repair, which may incur additional costs.
- For customers using HF applications, the instrument should be returned to its standard sample introduction system.

เอกสารไม่ควบคุม

Service Engineer's Responsibilities

- Contact the customer and ensure that all necessary supplies are available before the preventive maintenance visit.
- Only select those pages that relate to the system or module being serviced.
- Complete empty fields with the relevant information.
- Complete the relevant checkboxes in the checklist using either a "**X**" or tick mark "✓".
- Check **"Service not applicable"** check boxes to indicate services/tasks not delivered, as appropriate.
- Complete the Preventive Maintenance services in the most logical order relevant to the individual system service in the order of the tasks listed.
- Complete the **Service Review** section together with the customer.
- Complete the fields for page numbers at the foot of each selected page
- Add relevant page numbers to selected pages and complete the total number of pages field in the Service Completion section
- **Ask the customer to sign the Service Verification section including the customer's and your signature.**

เอกสารไม่ควบคุม

Important Customer Web Links

- To access **Agilent University**, visit http://www.agilent.com/crosslab/university/ to learn about training options, which include online, classroom and onsite delivery. A training specialist can work directly with you to help determine your best options.
- To access the **Agilent Resource Center** web page, visit https://www.agilent.com/en-us/agilentresources. The following information topics are available:
  - Sample Prep and Containment
  - Chemical Standards
  - Analysis
  - Service and Support
  - Application Workflows
- The **Agilent Community** is an excellent place to get answers, collaborate with others about applications and Agilent products, and find in-depth documents and videos relevant to Agilent technologies. Visit https://community.agilent.com/welcome
- Videos about specific preparation requirements for your instrument can be found by searching the **Agilent YouTube** channel at https://www.youtube.com/user/agilent
- **Need to place a service call?** Flexible Repair Options | Agilent

เอกสารไม่ควบคุม

Instrument Maintenance

System Information

☐ Check this box if an instrument configuration report is attached instead of completing the table.

Instrument System Name and ID	5110 VDV ICP-OES
Instrument System Site and Location	UAE Consultant

	List System Component Product Numbers	List the Serial Numbers of each Component
1.	G 8015 A	MY 18030001
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

ICP-OES Configuration Table	Circle the type or write in the type if other
Nebulizer Type	SeaSpray | OneNeb | Conikal | Other
Spray Chamber	Cyclonic Single Pass | Cyclonic Double Pass | Other
Torch	Radial | Dual View | Other
Torch Type	One Piece | Semi Demountable | Fully Demountable | Other
Injector Diameter	2.4mm | 1.8mm | 1.4mm | 0.8mm | Other
Injector Material	Quartz | Ceramic | Other

เอกสารไม่ควบคุม

Preparation

- [x] Discuss any specific issues with the customer before starting.
- [x] Review the instrument logbook for recorded problems and comments.
- [x] Save instrument control settings before starting the procedure.
- [x] Perform a general inspection of the system for cleanliness.
- [x] Check for proper installation of parts, assemblies, sensors etc.
- [x] Check system for required installation of components and implementation of Service Notes.
- [x] Check for required firmware/software updates and verify with customers if they would like them installed.
- [ ] For HF application systems, if standard sample introduction system was not installed, ask the customer to install it. N/A
- [x] Ask the customer to remove any samples from the ICP-OES sample introduction area, auto sampler or around the ICP-OES.

เอกสารไม่ควบคุม

SPS 3 Auto Sampler

- [x] **Service not applicable**
- [ ] Power cycle the autosampler and verify successful initialization.
- [ ] Inspect X and Z axis belts for wear. Replace is necessary.
- [ ] Clean X and Z axis slide shafts.
- [ ] Using customer's racks and the Agilent software move the sample probe to the 4 outermost corners and rinse port, ensure that the probe is approximately centered in the vial.

SPS 4 Auto sampler

- [x] **Service not applicable**
- [ ] Clean the spill tray, rack location mat, end frames and chassis with a damp soft cloth and diluted mild detergent.
- [ ] Clean the auto sampler cover panels, if cover kit is installed, with domestic window cleaner.
- [ ] Check the X-axis and Z-axis drive belts for cracks, splits, damaged teeth, excessive fraying, color changes or degradation from fumes.
- [ ] Check the X-axis, Theta-axis and Z-axis FFC cables for cracks, incorrect positioning, damaged edges or damaged connectors.
- [ ] Pump Tubing Replacement. Replace peristaltic pump tubing. Replace all tubing that goes from the rinse station to the pump and from the pump to the waste/rinse bottles
- [ ] Test using customer's tray and move the sample probe to the sample vial 1, wash vial and rinse port and ensure that the probe is centered in the vial. If not use calibration wizard and calibrate the position.

AVS 4, 6, 7 Advanced Valve System

- [x] **Service not applicable**
- [ ] Replace valve rotor seal
- [ ] Check fittings for signs of leaks
- [ ] Check tubing including autosampler tubing for kinks or excessive wear
- [ ] Check high flow pump for signs of leaks

เอกสารไม่ควบคุม

Preventive Maintenance Procedures

Record Pre-PM instrument performance

- [x] Run Instrument Performance test.
- [x] Record results in Instrument Performance Test Results Table – Pre-PM.

Clean and inspect ICP-OES system

- [x] Look for any obvious external damage or problems.
- [x] Inspect water cooling hoses, gas lines and power cord for excessive wear or damage.
- [x] Perform a general internal inspection of the system for excessive dust accumulation, clean if necessary.
- [x] Inspect sample introduction components and record any required maintenance in the Service Engineer Comments and notify the customer as the required actions required.
- [x] Record the instrument operating conditions in the ICP-OES Status Results Table.
- [x] Replace the polychromator purge filter.
- [x] Replace the radial pre-optics window.
- [x] Replace the axial pre optics window for SVDV and VDV instruments.
- [x] Check exhaust flow for the correct positive extraction at the exhaust duct to insure they meet minimum specifications.
- [x] Replace air inlet dust filter.
- [ ] Replace high capacity air inlet dust filter element if installed. N/A
- [x] Remove and clean instrument water inlet filter.

Agilent Water Recirculator

- [ ] **Service not applicable**
- [x] Drain cooling fluid and remove any particles from the chiller reservoir.
- [x] Remove, clean and reinstall water inlet metal mesh filter if present.
- [x] Re fill with Agilent Cool Clear cooling fluid.
- [x] Clean the cooling system Air filter and the condenser.

เอกสารไม่ควบคุม

ICP-OES adjustment

- [x] Check position of Zn peak, adjust if required.
- [x] Check Argon Ratio, adjust to specified value if required.
- [x] Perform Detector Calibration.
- [x] Perform Instrument Calibration.

Record Post-PM instrument performance

- [x] Run Instrument Performance test.
- [x] Record results in Instrument Performance Test Results Table - Post PM.
- [x] For systems using ICP Expert version 7.3 and above, run the following instrument tests
  - [x] Subsystem Communications Test
  - [x] Air Flow
  - [x] Water Flow
  - [x] Gas Flows
  - [x] RF Generator
  - [x] Camera Test
  - [x] Optics Test
  - [x] Nebulizer Test
- [x] Record the result in the Instrument Test Results Table

เอกสารไม่ควบคุม

Restore Instrument

- ☐ For HF applications, ask the customer to re install their sample introduction system. N/A
- ☑ Leave system in an idle state: on and purging.
- ☑ Guidance: If the PM service is performed prior to a qualification service, then use the qualification procedure as a guide for final instrument set up and checkout.

Service Review

- ☑ Attach available reports/printouts of all tests to this documentation.
- ☑ Record the Preventive Maintenance service activity in the customer's records/logbook.
- ☑ Record the PM event in the Smart Alerts logbook, if applicable.
- ☑ Update/reset instrument maintenance counters as appropriate.
- ☑ Affix the PM sticker to the system or instrument logbook based on the customer's request.
- ☑ Complete the Service Engineer Comments section if there are additional comments.
- ☑ Review this service, parts replaced, and test results obtained with the customer.
- ☑ If the instrument firmware was updated, record the details of the change in the Service Engineer's Comments box. Systems in a compliant environment may need additional documentation.
- ☑ **Complete the Signature Page with both Service Engineer and Customer signatures.**

เอกสารไม่ควบคุม

ICP-OES Status Results Table

Note: These measurements do not form part of any specification and are for reference only.

Measurement	Standby Mode		Plasma On	
Mains Voltage	231.288	VAC	228.330	VAC
Mains Current	0.083	A	0.106	A
Instrument Temperature	21.1	°C	21.6	°C
RF Air Flow (sensor speed)	44.0	Hz	41.1	Hz
Plasma Exhaust Temperature	No measurement		47.1	°C
Water Flow Oscillator	No measurement		1.14	L/min
Water Flow Detector	0.92	L/min	0.90	L/min
Water Inlet Temperature	19.5	°C	19.5	°C
Polychromator Temperature	35.4	°C	35.4	°C
CCD Temperature	-40.1	°C	-39.9	°C
Thermal Stabilizer	35.0	°C	35.0	°C
Argon Supply Pressure	634.43	kPa	583.77	kPa
Purge Gas Supply Pressure*1	631.28	kPa	604.02	kPa
Option Gas Supply Pressure*1	-	kPa	-	kPa
Nebulizer Flow	No measurement		0.70	L/min
Nebulizer Back Pressure	No measurement		233.61	kPa
Plasma Gas Flow	No measurement		1196	L/min
Auxiliary Gas Flow	No measurement		1.00	L/min
RF Power	No measurement		1200.4	W
RF Supply Current	No measurement		8.228	A
RF Supply Voltage	No measurement		194.529	V

*1 If option installed

เอกสารไม่ควบคุม

Test Results

Instrument Performance Test Results Table

Note: These measurements do not form part of any specification and are for reference only.

	Pre PM Sensitivity Check		Post PM Sensitivity Check	
	Radial	Axial *	Radial	Axial*
Zn 213.857 nm SRBR	1783.8	2879.2	2230.8	3662.9
Mn 257.610 nm SRBR	95670.5	196149	106830	178844
Al 396.152 nm SBR	5.2	8.0	7.0	7.4
K 766.491 nm SBR	3.0	14.6	3.4	8.7

* Axial result is not applicable for G8016AA, G8012AA Radial View instruments.

Instrument Test Results Table

Note: The Instrument Test results are for systems using ICP Expert version 7.3 and above only.

Instrument Test	Result
Subsystem Communications Test	Pass
Air Flow	Pass
Water Flow	Pass
Gas Flows	Pass
RF Generator	Pass
Camera Test	Pass
Optics Test	Pass
Nebulizer test	Pass

เอกสารไม่ควบคุม

Consumed PM Parts

Part Description	Part Number	Product or Model# where used	Quantity consumed
Axial Pre-Optic Window	G8010-80014	G8010A, G8011A, G8014A/G8015A	1
Radial Pre-Optic Window	G8010-80015	All	1
Agilent Cool Clear Coolant Fluid	5799-0037	Agilent Water Recirculator	-
Purge Gas Filter	G8010-60136	All	1
Air Inlet filter	G8000-68002	All	1
High Capacity Air Filter	G8010-60189	Optional	-
Rotor seal for 6-7 port valve for AVS6/7	G8494-68002	G8494A/G8495	-
Rotor seal for 4 port valve for AVS4	G8493-68002	G8493A	-
Rinse solution to rinse station 2.5mm id x 1m	G8410-80123	SPS 4	-
Barb connector 2.5mm-1.5mm ID	G8410-80124	SPS 4	-
PVC waste tubing,8mm od x 5mm id, 2m	G8410-80122	SPS 4	-
Additional Parts may be required from engineer's stock:			
X axis drive belt	5410047500	SPS 3	-
Z axis drive belt	5410047400	SPS 3	-
Peristaltic pump tubing, PVC SolvaFlex, 3 bridged	3710049000	SPS 4	-

Consumed Parts Reference
(Purchased by customer, not included as part of PM)

☑ Section Not Applicable

Part Description	Part Number	Product or Model# where used	Quantity consumed

เอกสารไม่ควบคุม

Agilent CrossLab
From Insight to Outcome

Signature Page

Service Engineer Comments (optional)

If there are any specific points you wish to note as part of performing the installation or other items of interest for the customer, please write in this box.

Service Verification

Service Request Number:
6008 006610

Service Engineer Name:
Worawit T.

Service Engineer Signature:
Worawit T.

Total number of pages in this document:
14

Date Service Completed:
3 Nov 2025

Customer Name:
Aphorn O.

Customer Signature:
Aphorn O.

© Agilent Technologies, Inc. 2022

Agilent

เอกสารไม่ควบคุม

Condition of this result of calibration

1. Reference Standard Instrument :-

Instrument	Serial No.	ID No.	Certificate No.	Due date
1) Thermometer	9549224	130RC003	25I440	16 Apr 2026
2) Ref. Std.Thermometer	4982054	110RC044	25I708	03 July 2026

- This measurement result is traceable to SI throught Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials :-
   - Conductivity calibration solution, CPA chem Ltd., The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Conductivity Solution	Manufacturer	Lot No.	Exp. date
1413.3 µS/cm	CPA Chem	1187337	18 Jan 2027
12.882 mS/cm	CPA Chem	1135362	16 Aug 2026

   - Control Conductivity calibration solution temperature by Water bath (25 ± 0.1) °C

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration results

Function : Conductivity Measurement

(*) After Adjustment at 1413.3 µS/cm

Conductivity Electrode Serial No.: 9B9F0277

Standard Conductivity Solution	Before Adjustment UUC* Reading	After Adjustment UUC* Reading	Uncertainty of Measurement (±)	Coverage factor *k*
1413.3 µS/cm	1462 µS/cm	1413 µS/cm	9.2 µS/cm	2.00
12.882 mS/cm	13.25 mS/cm	12.81 mS/cm	0.086 mS/cm	2.00

Remark : - UUC* = Unit Under Calibration

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

ilac-MRA
NSC-TISI-TIS17025
CALIBRATION 0008

Certificate of Calibration

Equipment :	Conductivity Meter
Manufacturer :	Horiba
Model :	LAQUA-EC210
Serial No. :	HC9L0015
ID No. :	UAE.EFM.010/2563(EFM.SCT.04/63)
Condition As-Received:	Used Item
Received Date :	24 February 2026
Calibration Date :	26 February 2026
Reference :	2602-0799WSC-2
Submitted by :	United Analyst and Engineering Consultant Co.,Ltd. 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure:	In -house method : - CP-CH6 by direct measurement with certified reference material (CRM) - CP-CH8 by comparison with temperature standard
Calibrated by :	Walalak Sirithean
Approved by :	Approved Signatory

( ) Chakrit Waewwanjua
( ) Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 27 February 2026

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Calibration Results

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : 9383
- Serial No. : 9B9F0277

Dimension of probe;

- Length : 110 mm
- Diameter : 16 mm
- Immersion Depth : 90 mm

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of Measurement (± °C)	Coverage factor *k*
15.0	15.002	15.0	-0.002	0.13	2.00
30.0	30.001	30.0	-0.001	0.13	2.00
45.0	45.001	45.0	-0.001	0.13	2.00

Remark : - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

สถาบันอาหาร
กลุ่มบริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

NSC-TISI-TIS 17025 CALIBRATION 0061

Calibration Certificate

Certificate No.: 2503682-004-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road, Bangchack, Prakhanong, Bangkok 10260

Equipment: CHAMBER (Incubator)
Manufacturer: BINDER
Model: KB 400
Serial No.: 20220000022479
ID No.: UAE.MIC.028/2566
Order No.: 2503682
Operation No.: 2503682-004
Date of Receipt: 1 July 2025
Date of Calibration: 1 July 2025

Calibrated by Mr.Pheraphat Tuanjit, Scientist
Approved by (Miss Preeyaporn Jaengkarnkit), Vice President, Department of Laboratory Services, Responsible for the Technical Management Team
Date of Issue: 3 July 2025

The uncertainties are for a confidence probability of approximately 95 %.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

2008 อาคารสินสุขวัฒน์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่เรือ เขตธนบุรี กรุงเทพมหานคร 10600
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel. +66(0) 2422 6688 Fax +66(0) 2422 8543
nfi.or.th

เอกสารไม่ควบคุม

สถาบันอาหาร
กลุ่มบริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

NSC-TISI-TIS 17025 CALIBRATION 0061

Calibration Report

Certificate No.: 2503682-004-01
Equipment: CHAMBER (Incubator)
Model: KB 400 Serial No.: 20220000022479
Resolution: 0.1 °C ID No.: UAE.MIC.028/2566
Manufacturer: BINDER
Date of Calibration: 1 July 2025

Calibration point: 35.0 °C
Calibration result:

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
MIN	20.1	45	225.0
MAX	22.0	65	235.0

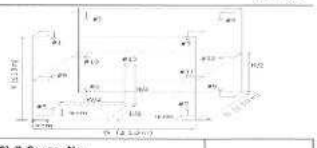


Table1 : Reporting of Temperature

Calibration point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.13 is REF)												Uncertainty ± (°C)
	# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9	# 10	# 11	# 12	# 13	
35.0	35.19	35.03	34.83	35.21	34.96	34.94	34.84	34.84	35.05	34.94	35.15	34.79	34.92	0.27

Table 2 : Reporting of Characterization Result

UUC* Setting (°C)	UUC* Reading (°C)			Temperature Stability ± (°C)	Temperature Uniformity (°C)	Overall Variation (°C)
	MIN	MAX	Average			
34.8	34.8	34.8	34.8	0.040	0.29	0.50

Note: The quoted uncertainty include " Stability " and " Loading effect (20% of Temp Uniformity) "
UUC* = Unit Under Calibration
Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.
Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
Overall Variation = The difference of the maximum and minimum measured temperatures througout observation time.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2, providing a level of confidence of approximately 95 %.

--------- End ---------

3 July 2025

2008 อาคารสินสุขวัฒน์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่เรือ เขตธนบุรี กรุงเทพมหานคร 10600
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel. +66(0) 2422 6688 Fax +66(0) 2422 8543
nfi.or.th

เอกสารไม่ควบคุม

สถาบันอาหาร
กลุ่มบริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

NSC-TISI-TIS 17025 CALIBRATION 0061

Calibration Report

Certificate No.: 2503682-004-01
Equipment: CHAMBER (Incubator)
Model: KB 400 Serial No.: 20220000022479
Resolution: 0.1 °C ID No.: UAE.MIC.028/2566
Manufacturer: BINDER
Date of Calibration: 1 July 2025

Location: Microbiology Laboratory, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Environment Condition:
Ambient Temperature (21 ± 1) °C
Relative Humidity (55 ± 10) %
Line Voltage (230 ± 5) Volt

Condition of this results of Calibration:

1. This instrument was calibrated by insert 13 standard thermometer into its chamber and calibration according to W-TE-014 Based on TLAS G-20-1/02-08 (E): Guidelines for Calibration and Checks of Temperature Controlled Enclosures.
   - The temperature scale used was based on ITS - 90.
   - All data show below were final values and the initial data may be obtained upon request.
2. Reference Standard Instrument :

Instrument	Model	Serial No./ID No.	Certificate No.	Due Date	Through
Digital Thermometer with sensor	34972A	MY59003377	2501168-001-01	13 January 2026	NATIONAL FOOD INSTITUTE
	RTD	CH#101-203 / STD#101-203			

3. This certificate is traceable to International System of Units (SI Units).
4. This certificate was certified only for the instrument we calibrated.
5. This result of calibration was found accurate as shown on date and place of calibration only.
6. Condition of Calibrated item : Good
   UUC Description :
   Time of Record 1 Hour 9 Minute At 35.0 °C
   Fresh air Damper [-] Open Position [-]
   [X] Close Fan [100%]
   [-] Not Available
7. Result of Calibration : [X] Without adjustment [ ] After adjustment

3 July 2025

2008 อาคารสินสุขวัฒน์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่เรือ เขตธนบุรี กรุงเทพมหานคร 10600
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel. +66(0) 2422 6688 Fax +66(0) 2422 8543
nfi.or.th

เอกสารไม่ควบคุม

PerkinElmer
For the Better

PinAAcle 900F
Preventive Maintenance Report

Company Name: UAE Consultant Co., LTD.
Instrument Location: 41 Sukumvhit Rd.,
Phra Khanong, Bangkok 10260
Instrument Serial No.: PFBS20031902
Date: 27 Oct 2025

เอกสารไม่ควบคุม

PinAAcle 900F Preventive Maintenance (PM)

Company Name:	United Analyst and Engineering Consultant Co., LTD.		
Address (Instrument Location):	41 Sukumvhit Rd., Phra Khanong, Bangkok 10260		
Serial Number:	PFBS20031902	**PM Number:**	1 of 2
Customer Name (if applicable):	K. Yainda	**Telephone Number:**	095-5580049
Customer Support Engineer Name:	K. Chayanan	**Service Order Number:**	WO-06332081
Date PM Performed: (DD-MMM-YYYY)	27 Oct 2025	**Next PM Due Date:** (DD-MMM-YYYY)	27 Apr 2026
Standard Labor Hours to Complete PM :		**5 hours**	

Part Number	Release	Publication Date	
09370145 Rev.9	A	January 2018	PerkinElmer®

Scope
The purpose of this PM is to ensure the continued functionality of the PinAAcle 900F by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer.
The customer should save their method before the PM begins.

General Instructions
The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM.
Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files.
The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer.
Update the PM sticker and instrument logbook as required.

Copyright Information
This document contains proprietary information that is protected by copyright. All rights are reserved.
No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of PerkinElmer, Inc.
Copyright © 2013 PerkinElmer, Inc.

Trademarks
Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners.
Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no Warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.
PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

เอกสารไม่ควบคุม

Component List

Component / Specific Model	Serial #	Configuration Notes
PinAACle900F	PFBS20031902	Syngistix V.4.0.1.1935
FIAS100	100524040501	

Parts Lists

Parts Included with the PM		
Part Number (if applicable)	**Description**	**Quantity**
B0501696	Fan Filters	1
N3160156	O-Ring Kits for Sampling Introduction (Stainless Steels Nebulizer)	N/A
N3160157	O-Ring Kits for Sampling Introduction (Plastic Nebulizer)	1
N9301714	Replacement Acetylene Filter Cartridge	1
TH001022	Replacement Air Filter Cartridge	1

Additional Reagents and Standards Required for PM				
Part Number (if applicable)	**Description**	**Quality**	**Batch/Lot #**	**Expired Date** (MM/YY)
N9300183	1000 mg/L Copper Standard	AR	28-83CUY1	Nov 2026

Additional Reagents and Standards Required for PM (Customer Support Solution)				
Part Number (if applicable)	**Description**	**Quantity**	**Batch/Lot #**	**Expiration Date** (MM/YY)
N/A	DI Water	250 mL	AR	AR
N/A	0.5% HNO_3	250 mL	AR	AR

เอกสารไม่ควบคุม

Additional Tools Required for PM			
Part Number (if applicable)	**Description**	**Quantity**	**Serial #**
N1013000	0.2A Neutral density filter	1	101N0089015
N1013002	1.0A Neutral density filter	1	101N0089015
03030997	System 2 EDL Driver	1	03030997
N3050605	As System 2 EDL	1	16148
N3050121	Cu Lumina HCL	1	060419-030180
N3050109	Be Lumina HCL	1	061219-020041
N3050139	K Lumina HCL	1	030819-010130
N3050152	Ni Lumina HCL	1	052719-020020

เอกสารไม่ควบคุม

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. **General:**
   - ☑ Review the instrument performance with the customer and document any recent problems.
   - ☑ Inspect the customer log book and make any appropriate PM entries.
   - ☑ Perform general inspection of system for cleanliness.
2. **PC Instrument Software:**
   - ☑ Instrument Software user files/databases archived, packed, and/or deleted as needed.
3. **Mechanical:**
   - ☑ Inspect and clean all fans and filters. Replace filters if necessary
   - ☑ Inspect all gas lines for leaks and/or wear. Replace if needed.
   - ☑ Clean exterior of the instrument.
   - ☑ Inspect the burner head, burner chamber, and nebulizer. Clean if needed as stated in the Hardware Guide.
   - ☑ Check burner head dimensions with the feeler gauge as stated in the Hardware Guide in the Maintenance chapter section on cleaning the burner head and checking sloth width. Replace if out of specification
   - ☑ Check the condition of the end cap, burner head, and nebulizer O-rings. Replace if necessary.
   - ☑ Check the drain system for signs of wear. Replace worn or damaged parts.
   - ☑ Visually check for proper flame conditions when igniting the Air-C2H2 and N20-C2H2 flames (if applicable).
4. **Electrical:**
   - ☑ Inspect PC boards. Clean if necessary.
   - ☑ Carefully check all internal and external cable connections.
   - ☑ Check instrument firmware revisions upgrade to current levels (if necessary)
   - ☑ Run Diagnostics Test within the Advanced function of the Spectrometer page. Check the results in the service log folder in the Spectrometer BM Log Viewer.
5. **Optics:**
   - ☑ Inspect and clean the sample compartment windows, if needed.
   - ☑ Inspect optics. Clean or replace if necessary.
6. **Gasses:**
   - ☑ Verify that the Gasses supplied to the instrument are within the pressure and purity specifications found in the PinAAcle 900 Series Pre-Installation Checklist SDB.
   - ☑ Verify that the acetylene filter and air filter element is dry. Replace if necessary.

เอกสารไม่ควบคุม

7. Flame Interlock Check:

Description: Check to ensure that all safety interlocks are closed.

Parameter	Specification	Test Results	Pass/Fail
Flame Sensor	Air/C_2H_2 Flame correctly shuts down	Active	Passed
Drain Sensor	Air/C_2H_2 Flame correctly shuts down	Active	Passed
Nebulizer Sensor	Air/C_2H_2 Flame correctly shuts down	Active	Passed
C_2H_2 Pressure Sensor	Air/C_2H_2 Flame correctly shuts down	Active	Passed
Air Pressure Sensor	Air/C_2H_2 Flame correctly shuts down	Active	Passed
Burner Head Sensor	Choosing Nitrous Oxide as the oxidant should trigger an interlock shuts down	Active	Passed

8. After PM Performance tests:

8.1 Detector Linearity with Barium

Description: Ensures that the detector is linear in the Visible Range.

Parameter	Specification	Certificate Value at 553.6 nm (Abs.)	Test Results	Pass/Fail
1.0 A ND Filter	± 5% from Cert.	0.9995	0.9887	Passed
0.2 A ND Filter	± 5% from Cert.	0.1936	0.1896	Passed

8.2 Baseline Noise at 1.0 Absorbance with Barium

Description: Ensures that a high absorbance will not produce excessive noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.010	0.001	Passed

8.3 AA Baseline Noise with Copper

Description: Check baseline noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.001	0.0001	Passed

เอกสารไม่ควบคุม

8.4 D_2 Background Compensation with Copper

Description: Verifies the instruments ability to compensate for Background absorption.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.010	0.0001	Passed

8.5 AA-BG Baseline Noise with Copper

Description: Ensures that background correction does not produce excessive noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.005	0.0001	Passed

8.6 AA-BG Baseline Noise with Arsenic

Description: Ensures that background correction does not produce excessive noise at a low wavelength.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.005	0.0004	Passed

8.7 Flame Sensitivity

Description: Instrument Sensitivity checked against Copper standard.

Standard Copper Sensitivity	Specification	Results (Abs.)	Pass/Fail
5 mg/L Sensitivity SS Neb (if applicable)	> 0.250 Abs.	N/A	Not Applicable
2 mg/L Sensitivity HS Neb (if applicable)	> 0.250 Abs.	N/A	Not Applicable

10. Review:

- ☑ Review with the customer PM work performed.
- ☑ Review with the customer routine maintenance procedures.
- ☑ Discuss recommended customer supplied materials to have on hand.
- ☑ Attach PM sticker.

เอกสารไม่ควบคุม

Additional Comments

Additional Comments Regarding the PM

Review

The preventive maintenance checks and if applicable performance tests for PinAAcle 900F have been completed.

This PinAAcle 900F Passes ☑ Fails ☐ the preventive maintenance.

Review of Preventive Maintenance:

Authorized PerkinElmer Representative: Chayanan K.	Date: 27 Oct 2025 (DD-MMM-YYYY)
Authorized Customer Representative: [signature]	Date: 27 Oct 2025 (DD-MMM-YYYY)

เอกสารไม่ควบคุม

Atomic Absorption/FIAS 100/400 Preventive Maintenance (PM)

Company Name:	United Analyst and Engineering Consultant Co., LTD.		
Address (Instrument Location):	41 Sukumvhit Rd., Phra Khanong, Bangkok 10260		
Room Number:	Lab		
Asset Number (if applicable):	1 of 2	**Customer System ID:**	K. Yanida
Service Engineer Name:	K. Chayanan	**Service Order Number:**	WO-06332087
Date PM Performed: (DD-MMM-YYYY)	27-Oct-2025	**Next PM Due Date:** (DD-MMM-YYYY)	27-Apr-2026

Part Number	Release	Publication Date	
09370005	C	January 2013	PerkinElmer®

Scope
The purpose of this PM is to ensure the continued functionality of the Atomic Absorption/FIAS 100/400 by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer.
The customer should save their method before the PM begins.

General Instructions:
Always check with the customer before making any changes that may affect the customer's analysis or calibration.
The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer.
Update the PM sticker and instrument logbook as required.

Copyright Information
This document contains proprietary information that is protected by copyright. All rights are reserved.
No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of PerkinElmer, Inc. **Copyright © 2013 PerkinElmer, Inc.**

Trademarks
Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners.
Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.
PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

เอกสารไม่ควบคุม

Component List

Component / Specific Model	Serial #	Firmware Version	Configuration Notes
FIAS100	100S24040501	2.20	Syngistix V4.0.1.1935

Parts Lists

Parts Included with the PM				
Part Number (if applicable)	Description	Quantity	Batch/Lot #	Expiration Date (MM/YY)
B050 2706	Fan Filter	1	N/A	N/A

Additional Tools Required for PM				
Part Number (if applicable)	Description	Quantity	Serial #	Calibration Due Date (MM/YY)
N/A	Digital Volt Meter	1	N/A	N/A
Additional Reagents and Standards Required for PM				
Part Number (if applicable)	Description	Quantity	Batch/Lot #	Expiration Date (MM/YY)
N/A	N/A	N/A	N/A	N/A

เอกสารไม่ควบคุม

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. **General:**
   - ☑ Review the instrument performance with the customer and document any recent problems.

     _____

   - ☑ Is the Working Environment Acceptable? If not, document.

     _____

   - ☐ Visual Damage (if yes, describe)

     _____

   - ☑ Check incoming AC line voltage for proper levels and grounding.
   - ☑ Verify Voltage switch on back of instrument is correct
   - ☑ Perform general inspection of system for cleanliness. Clean if needed.
   - ☑ Gas supply cylinders secured, lines leak checked and argon or nitrogen supply pressure verified (45 – 58 psi).
   - ☑ Inspect the customer log book and make any appropriate PM entries.
   - ☑ Fan checked and filter cleaned
   - ☑ Heating mantle or Universal Cell Holder checked

2. **Instrument components**
   - ☑ Non-return valve checked/repaired/replaced if needed (B019 8111). Clean the valve if there is any liquid in it. Replace the rubber sleeve (B013 5123) if it is worn. Check the flow meter for any signs of fluid in it. Clean the flow meter if needed.
   - ☑ Verify condition of pump pressure adjustment levers (B050 7794 - look for cracks or problems with the springs), pump rollers (B300 0251 check for wear), and thumb screws (B050 7796).
   - ☑ Check the Multiport valve for proper switching, flow, and insure there are no leaks. Clean valve parts and replace o-rings if needed (large o-ring: B050 1250, small o-ring: B004 5095). Use a squirt bottle & fishing line to try to dislodge clogs.
   - ☑ Firmware Version checked. Latest is 2.20.

3. **Mixing/Separation Assembly & Pump Tubing:**
   - ☑ Mixing separator assembly checked
   - ☑ Filter/membrane checked (B050 8306)
   - ☑ Condition of the pump tubing (replace if necessary), correct pump tubing for the solutions being run. Make sure the correct magazines are being used. B050 7791 for 0.13 – 1.80 mm tubing; B050 7792 for 1.60 – 3.18 mm tubing.

เอกสารไม่ควบคุม

4. **Cell, Cell Windows, Transfer Line:**
   - ☑ Cell checked
   - ☑ Cell windows checked
   - ☑ Transfer line checked for moisture (if moisture is a problem, the Nafion dryer might be needed)

5. **Operational Tests:**
   - ☑ Run DI water through the carrier/reductant/sample system. Verify smooth flow of liquid throughout without leaks. Replace tubing & fittings if needed.

6. **Review:**
   - ☑ Review with the customer PM work performed.
   - ☑ Review with the customer routine maintenance procedures.
   - ☑ Discuss recommended customer-supplied materials to have on hand.
   - ☑ Attach PM sticker.
   - ☑ Update Logbook.

เอกสารไม่ควบคุม

Additional Comments

Additional Comments Regarding the PM

Review

The preventive maintenance checks and if applicable performance tests for FIAS 100/400 have been completed.

This FIAS 100/400 Passes ☑ ***Fails*** ☐ ***the preventive maintenance.***

Review of Preventive Maintenance:	
Authorized PerkinElmer Representative: Chayanan K.	Date: 27 Oct 2025 (DD-MMM-YYYY)
Authorized Customer Representative: [illegible]	Date: 27 Oct 2025 (DD-MMM-YYYY)

เอกสารไม่ควบคุม

Document History

Revision	Description of Change	Page(s)	Date
A	First release		May 2008
B	Addition of Batch/Lot Number, Expiration Date, and Report Fields.	2,7	February 2009
C	Update to new format	All	January 2013

เอกสารไม่ควบคุม

PerkinElmer
For the Better

PerkinElmer Scientific (Thailand) Co., Ltd.
250 Soi Soonvija 4
Khwang Sangyapi, Khet Huay Kwang
Bangkok 10310
Thailand
Tel: 66 2719 6420 ; Fax: +66 2 319 7900
http://www.perkinelmer.com

Service Report

Work Order Number	Activity Code	Billing Type	Requested Start Date	Model	Serial Number
WO-0633286	Planned Maintenance	Contract	28/04/2568 10:27 น.	AAnalyst 400	FFBS2003190Z
Service Representative Name	**Contract Number**		**Expiry Date**	**Equipment ID**	**System ID**
Kanan, Chayanan	SC-003906189		31/10/2025	N/A	N/A
UDI Number					
N/A					
Equipment Location			**Bill To Name**		
บริษัท ปูโรเด็ค แอนะลิติคัล เอเชีย [illegible] กรุงเทพมหานคร 51 10260 TH			บริษัท ปูโรเด็ค แอนะลิติคัล เอเชีย [illegible] กรุงเทพมหานคร 51 10260 TH		
Customer Contact	**Phone Number**	**Fax Number**	**Email**		**Purchase Order**
[illegible]	085-5580649	N/A	yaninlachamlek@gmail.com		PO-2561000002

Work Description

- PM 1/2 (Annual)
- Cleaning Cell, Chamber, Filter
- Wavelength Calibrate ; Pass
- Wavelength Scan As,Cu,Be,K,Na ; Pass
-Align cell with Hg. ; OK

Start Date	End Date	Work Description
27/10/2025	27/10/2025	
27/10/2025	27/10/2025	

Tools Used

Quantity	Calibrated Tool	Description	Serial Number	Last Calibration Date	Next Calibration Date
*** No Calibrated Tools Used ***					

Material Used

Part Number	Part Description	Note	Lot/Serial Number	Quantity
N9301714	Balston G2+2 Filter Cartridge			1

Labour Details

Part Number	Part Description	Start Date	Quantity
SV000013	Preventative maintenance	27/10/2025	4
SV000002	Service Travel	27/10/2025	2

Work Complete	Customer Signature	Technician Signature
Yes ☑ No ☐	[illegible]	Chayanan k.
PM/OQ/PV Left with Customer: Yes ☐ No ☑	2/11/2568 [illegible]	2/11/2568 Kanan, Chayanan

เอกสารไม่ควบคุม

Perkin

PerkinElmer TruQ

PerkinElmer Number: N9300163
Element and Matrix: 1000 µg/mL Copper in 2% HNO3
Starting Material: Copper Metal
Starting Material Lot No: 10221A
Density: 1.011 g/mL @ 20°C

Lot No: 28-83CUY1
Certification Date: MAY - - 2025
Expiration Date: NOV 30 2026

Trace Metallic Impurities in the Actual Solution via ICP / ICP-MS Analysis:

Element	µg/mL	Element	µg/mL	Element	µg/mL	Element	µg/mL	Element	µg/mL
Ag	0.005	Dy	<0.001	Li	<0.001	Pt	<0.001	Tb	<0.001
Al	<0.002	Er	<0.001	Lu	<0.001	Rb	<0.001	Te	<0.001
As	<0.001	Eu	<0.001	Mg	<0.001	Re	<0.001	Th	<0.001
Au	<0.001	Fe	0.02	Mn	<0.001	Rh	0.002	Ti	<0.001
B	<0.001	Ga	<0.001	Mo	<0.001	Ru	<0.001	Tl	<0.001
Ba	<0.001	Gd	<0.001	Na	0.004	Sb	<0.001	Tm	<0.001
Be	<0.001	Ge	<0.001	Nb	<0.001	Sc	<0.001	U	<0.001
Bi	<0.001	Hf	<0.001	Nd	<0.001	Se	<0.002	V	<0.001
Ca	<0.01	Hg	<0.001	Ni	<0.001	Si	<0.1	W	<0.001
Cd	<0.001	Ho	<0.001	P	<0.2	Sm	<0.001	Y	<0.001
Ce	<0.001	In	<0.001	Pb	0.005	Sn	0.003	Yb	<0.001
Co	<0.001	Ir	<0.001	Pd	<0.001	Sr	<0.001	Zn	0.02
Cr	<0.001	K	<0.1	Pr	<0.001	Ta	<0.001	Zr	<0.001
Cs	<0.001	La	<0.001						

Traceability Documentation for Solution Standard:

Certified Value: 999 µg/mL ±5 µg/mL (refer to side 2)
Certified Value is Traceable to: NIST SRM #3114
*** Classical Wet Assay:** 997 µg/mL
Method: EDTA titration using PAN as indicator. EDTA standardized against $Pb(NO_3)_2$ NIST SRM #928.

***Instrument Analysis using ICP Spectrometer:** 1001 µg/mL
via NIST SRM #3114

We guarantee that our PerkinElmer TruQ Atomic Spectroscopy Standards are stable and accurate to ±0.5% of certified concentration until the expiration date, provided the standards are kept tightly capped and stored under normal laboratory conditions. This value is the sum of cumulative errors associated with the analytical determinations, pipetting, and diluting to final volume. For these solutions we use high purity acids, ASTM Type 1 water (18 megohm double deionized), and leached, triple-rinsed bottles. All glassware used is class A.

Certifying Officer: Y. Parikh
Yogesh Parikh, Senior Spectroscopist

เอกสารไม่ควบคุม

Terms & Conditions

Customer Acknowledgment of receipt of the above repair / replacement.

Special Terms and Conditions: This is not an invoice.

Taxes will be applied to your invoice if applicable.

เอกสารไม่ควบคุม

PerkinElmer
For the Better

PerkinElmer Scientific (Thailand) Co., Ltd.
298 Soi Soonvijai 4
Khwang Bangkapi, Khet Huay Kwang
Bangkok 10310
Thailand
Tel: 66 2719 6420 Fax: +66 2 319 7900
http://www.perkinelmer.com

Service Report

100S24040501

Work Order Number	Activity Code	Billing Type	Requested Start Date	Model	Serial Number
WO-06332957	Planned Maintenance	Contract	28/04/2568 10:29:%.	FBAS100	100820040201
Service Representative Name	**Contract Number**	**Expiry Date**	**Equipment ID**	**System ID**
Kanan, Chayanan	SO-00356641-05	31/10/2025	N/A	N/A
UDI Number				
N/A				

Equipment Location	Bill To Name
บริษัท ยูไนเต็ด อนาลิสต์ แอนด์ เอนจิเนียริ่ง คอนซัลแตนท์ จำกัด เลขที่ 41 ซอยอุดมสุข 41 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 51 10260 TH	บริษัท ยูไนเต็ด อนาลิสต์ แอนด์ เอนจิเนียริ่ง คอนซัลแตนท์ จำกัด เลขที่ 41 ซอยอุดมสุข 41 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 51 10260 TH

Customer Contact	Phone Number	Fax Number	Email	Purchase Order
ยุวเทียนา พรมนิล(ใบพลู)	095-6560949	N/A	yaridacmenlek@gmail.com	HPO-2b0100602

Work Description

- PM 1of 2 (S/N_100820040501)
- Cleaning Port Vale, Manifold, Tuning
- Run Hg test ; Pass

Start Date	End Date	Work Description
27/10/2025	27/10/2025	
27/10/2025	27/10/2025	

Tools Used

Quantity	Calibrated Tool	Description	Serial Number	Last Calibration Date	Next Calibration Date
*** No Calibrated Tools Used ***					

Material Used

Part Number	Part Description	Note	Lot/Serial Number	Quantity
B0194040	Sample Loop, 500UL			1
B0501250	O-Ring 18.77 x 1.78			1
B0500748	O-RING 16 X 1.78 VITON			2

Labor Details

Part Number	Part Description	Start Date	Quantity
SV000013	Preventative maintenance	27/10/2025	3
SV000002	Service Travel	27/10/2025	2

Work Complete	Customer Signature	Technician Signature
Yes ☑ No ☐	ยุวเทียนา	Chayanan K.
PM/OQ/PV Left with Customer		
Yes ☐ No ☑	3/11/2568 ยุวเทียนา พรมนิล(ใบพลู)	3/11/2568 Kanan, Chayanan

เอกสารไม่ควบคุม

Terms & Conditions

Customer Acknowledgment of receipt of the above repair / replacement.

Special Terms and Conditions: This is not an invoice.

Taxes will be applied to your invoice if applicable.

เอกสารไม่ควบคุม

UAE United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel.0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

Certificate of Calibration

Certificate No.: 260311-2-BL002-26
Code No.: BL002-26

Customer Name: United Analyst and Engineering Consultant Co., Ltd.
Address: 3 Soi Udom suk 41, Sukhumvit Rd., Bang Chak, Phar Khanong, Bangkok 10260

Equipment: Electronic Balance
Manufacturer: Mettler Toledo
Model: XSR205DU
Serial No.: C009071872
Asset No. : UAE.WAO.012/2563
Building : UAE number 3 Floor : 2 Room : 208

Received Date: March 11, 2026
Date of Calibation : March 12, 2026
Calibration Conditions: Temperature 23.8 °C to 24.1 °C
Humidity 53.0 % to 59.0 %
Pressure 755.5 mmHg to 755.6 mmHg

Calibrated by: Thanachat Chaipanol
Approved by: Suwit Chotnok Signature:
Issued Date: March 16, 2026

Note : 1) The Uncertainties are for a confidence probability of approximately 95%
2) This Certificate is valid only to the item calibrated on date and place of calibration.
3) This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the United Analyst and Engineering Consultant Co.,Ltd. (UAE)

เอกสารไม่ควบคุม

UAE United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel.0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

Equipment: Electronic Balance
Model: XSR205DU
Serial No.: C009071872
Max. Capacity: 81 g / 220 g
Calibration Date: March 12, 2026
Condition As Received: In Condition

Manufacturer: Mettler Toledo
Readability: 0 to 81 (g) 0.01 mg > 80 to 200 (g) 0.1 mg
ID No.: UAE.WAO.312/2565

Condition of Equipment:
Condition of This Result of Calibration:
1. Calibration Method: This instrument was calibrated by method UAE CP CAL 005 (Internal Method based on OIML Publ 14 : 2022)
2. Reference Standards

Reference Standard:	Model	Serial No.	Calibrated By	Certificate No.	Traceability	Due Date
Standard Weight Class F2 (OIML)	1 mg to 1 kg	[illegible]	METTLER TOLEDO GmbH	CS10641635	Mettler-Toledo GmbH	3 Mar 27
Standard Weight Class F2 (OIML)	1 mg to 1 kg	B749109122	AMARC	25-009359	Mettler-Toledo	21 Jan 27


Instrument	Model	Serial No.	Calibrated By	Certificate No.	Traceability	Due Date
Thermo Hygro Baro Meter	MHB-382SJ	AK46157	SUCCESS	SCI H 01992/68	Success Gateway	26 Nov 26
Thermo Hygro Baro Meter	MHB-382SJ	AK46157	UAE	25#4464	UAE	18 Dec 26

3. This certification is traceable to SI Unit.
4. This certification was certified only for the instrument we calibrated.
5. The result of calibration was found accurate as shown on date and place of calibration only.
6. Through the reference standard laboratory of Mettler Toledo GmbH (CS10641635, SAS accreditation number SCS 0032
7. Through the reference standard laboratory of AMARC (25-009359), TIS accreditation number 0152

Calibration Result:
1. Repeatability of Reading:

Nominal Value (g)	Standard Deviation of Reading (g)
80	0.000008
200*	0.000345

2. Eccentric or off-center loading
A mass of 100 g was placed and moved to various position on pan
The Balance reading obtained is given in the table.

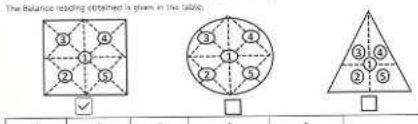

1 (g)	2 (g)	3 (g)	4 (g)	5 (g)	Maximum Difference (g)
100.0000	100.0000	100.0000	100.0000	100.0000	0.0000

เอกสารไม่ควบคุม

United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel.0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

Certificate No.: 260311-2-BL002-26
Code No.: BL002-26
Page: 3 of 4

Equipment:	Electronic Balance	Manufacturer:	Mettler Toledo
Model:	XSR205DU	Readability:	0 to 81 (g): 0.01 mg > 80 to 200 (g) : 01 mg
Serial No.:	C009071872	ID No.:	UAE WAO.012/2563
Max. Capacity:	81 g / 220 g		
Calibration Date:	March 12, 2026		

Calibraton Result: (Continued)
Calibraton Range: 0 to 80 (g)
Calibraton Adjustment: Internal Calibration

3. Error of indication from nominal or conventional mass value: (Range: 0 to 81 (g) ; Resolution: 0.00001 g)

Nominal Value (g)	Reference Value (g)	Indication (g)	Correction (g)	Uncertainty (± mg)	Coverage Factor k
Unload	0.0000000	0.0000	0.0000	0.015	2.25
0.001	0.0010020	0.0010	0.00002	0.015	2.23
0.005	0.0050025	0.0050	-0.00002	0.015	2.23
0.01	0.0100005	0.0100	-0.00002	0.015	2.25
0.05	0.0500003	0.0500	-0.00001	0.015	2.21
0.10	0.1000083	0.1000	-0.00001	0.015	2.20
0.50	0.5000121	0.5000	-0.00002	0.016	2.15
1	1.0000119	1.0000	0.00000	0.016	2.12
2	2.0000125	2.0000	-0.00001	0.017	2.09
5	5.0000146	5.0000	-0.00002	0.020	2.05
10	10.0000330	10.0001	-0.00002	0.023	2.00
20	20.000028	20.0001	-0.00005	0.033	2.00
30	30.000061	30.0001	-0.00004	0.051	2.00
40	40.000054	40.0001	-0.00004	0.063	2.00
50	50.000057	50.0001	-0.00005	0.064	2.00
60	60.000070	60.0001	-0.00004	0.081	2.00
80	80.000098	80.0001	-0.00001	0.11	2.00

เอกสารไม่ควบคุม

UAE TOX 009/2566

Agilent CrossLab
From Insight to Outcome

Agilent CrossLab Start Up Services
Agilent 8890 Gas Chromatograph
Preventive Maintenance Checklist

Agilent Preventive Maintenance provides factory recommended service for your analytical instruments to assure reliable operation and the accuracy of your results.

Delivered by highly trained and certified service engineers using genuine Agilent parts and supplies, Agilent Preventive Maintenance provides everything you need to reduce unplanned downtime and keep your systems operating at their peak. This checklist will be completed at the end of the service and provided to you as a record of the preventive maintenance activities.

Agilent

เอกสารไม่ควบคุม

United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel.0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

Certificate No.: 260311-2-BL002-26
Code No.: BL002-26
Page: 4 of 4

Equipment:	Electronic Balance	Manufacturer:	Mettler Toledo
Model:	XSR205DU	Readability:	0 to 81 (g): 0.01 mg > 80 to 200 (g) : 01 mg
Serial No.:	C009071872	ID No.:	UAE WAO.012/2563
Max. Capacity:	81 g / 220 g		
Calibration Date:	March 12, 2026		

Calibraton Result: (Continued)
Calibraton Range: > 80 to 200 (g)
Calibraton Adjustment: Internal Calibration

3. Error of indication from nominal or conventional mass value: (Range: > 80 to 200 (g) ; Resolution: 0.0001 g)

Nominal Value (g)	Reference Value (g)	Indication (g)	Correction (g)	Uncertainty (± mg)	Coverage Factor k
Unload	0.0000000	0.0000	0.0000	0.02	2.25
90	90.0000910	90.0000	0.0000	0.16	2.00
100	100.0000420	100.0000	0.0000	0.16	2.00
110	110.0000750	110.0000	0.0000	0.17	2.00
120	120.0000680	120.0000	0.0001	0.18	2.00
130	130.0001010	130.0000	0.0000	0.20	2.00
140	140.0000960	140.0000	0.0001	0.21	2.00
150	150.0000790	150.0000	0.0001	0.21	2.00
160	160.0001120	160.0000	0.0001	0.23	2.00
170	170.0001050	170.0000	-0.0002	0.24	2.00
200	200.0001460	200.0000	-0.0002	0.26	2.00

4. Effect of Tare test:

Tare Load (g)	Test Load (g)	Indication (g)	Correction (g)
100	20.000028	20.0000	0.0000
	40.000054	40.0002	-0.0001
	60.000070	60.0002	-0.0001
	80.000098	80.0002	-0.0001
	100.000042	100.0000	-0.0002

Remark:
The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k, providing a level of confidence of approximately 95%

o---o-End-o---o

เอกสารไม่ควบคุม

Agilent CrossLab

Agilent 8890 GC Preventive Maintenance Checklist

Introduction

Customer Information

- Customers should provide all necessary operating supplies upon request of the engineer.
- A customer representative should be available to the engineer while performing the preventive maintenance procedures.
- Any parts, not included in the Parts Lists section of this document, are not part of the recommended Preventive Maintenance service, nor are they included in the price of this service.
- If a system requires the use of extra or special procedures and/or parts for the maintenance additional costs.

Important Customer Web Links

- For more information about *Agilent Technologies services*, please visit our website using the following URL: http://www.agilent.com/en-us/products/crosslab-instrument-services/service-repair
- The **Agilent Community** is an excellent place to get answers, collaborate with others about applications and Agilent products, and find in-depth documents and videos relevant to Agilent technologies. Visit https://community.agilent.com/welcome.
- To access **Agilent University**, visit http://www.agilent.com/crosslab/university/ to learn about training options, which include online, classroom and onsite delivery. A training specialist can work directly with you to help determine your best options.
- A useful **Agilent Resource Center** web page is available, which includes short videos on maintenance, quick lists of consumables for new instruments, and other valuable information. Check out the Resource Page here: https://www.agilent.com/en-us/agilentresources.
- **Need technical support, FAQs, supplies?** – visit our **Support Home page** http://www.agilent.com/search/support.
- Videos about specific preparation requirements for your instrument can be found by searching the *Agilent YouTube* channel at https://www.youtube.com/user/agilent.

Revision: 2.01, Issued: September 14, 2021
Agile Document Number: D0013610
DE number: 44166.7597222222
© Agilent Technologies, Inc. 2021

Agilent

เอกสารไม่ควบคุม

Service Engineer's Responsibilities

- Contact the customer and ensure that all necessary supplies are available before the preventive maintenance visit.
- Only select those pages that relate to the system or module being serviced.
- Complete empty fields with the relevant information.
- Complete the relevant checkboxes in the checklist using either a "X" or tick mark "✓".
- Check **"Section not applicable"** check boxes to indicate services/tasks not delivered, as appropriate.
- Complete the Preventive Maintenance service in the order of the tasks listed.
- Complete the Service Review section together with the customer.
- Complete the fields for page numbers at the foot of each selected page
- Complete the total number of pages field in the Service Completion section
- ***Ask the customer to sign the Service Completion section including the customer's and your signature.***

Additional Instruction Notes

- Check for any active service notes for this unit. If there are any applicable "Safety" or "Modification Recommended" Service notes, plan to implement the changes on this unit before doing any qualification service.
- Do not implement firmware updates, unless you get approval from the customer and are sure that they are compatible with the instrument control software.

เอกสารไม่ควบคุม

Preventive Maintenance Procedure

Clean and inspect GC

- ☑ Unplug power cord from the power source.
- ☑ Open GC covers and vacuum/remove any dust/debris. Pay particular attention to cooling fans.
- ☑ Inspect internal connectors for proper contact and placement.
- ☑ Reconnect Power to the GC. Power the GC on and verify the power on self-test passed.
- ☑ Verify oven motor spins freely and turns on with the oven door closed; off when the door is opened.
- ☑ Verify operation of all other fans - the inlet and EPC cooling fans.
- ☑ Verify oven intake/outlet flap assembly is operating smoothly while heating and cooling the oven

Inlet and detector consumable replacement

- ☑ Replace the split vent trap cartridge filter using the Maintenance procedure from either the Browser User interfaces on units with these inlets: Split/Splitless Capillary (SSL), Multi-Mode Inlet (MMI), Programmed Temperature Vaporizer (PTV), Volatiles Interface (VI).
- ☑ If the inlet system is used in Split Mode with viscous samples, inspect and clean the split vent tube on the inlet and flush or replace the tubing between the inlet and the split vent trap.
- ☑ For the inlets installed, perform inlet maintenance using the Maintenance procedure from the Browser user interfaces. Record the results. (Leak and Restriction Test)
- ☑ If the GC includes a Flame Ionization Detector (FID), replace the jet. If the ignitor shows any buildup of sample or corrosion, replace the ignitor. Examine the FID collector and castle assemblies for contamination – clean as necessary.

Zero Sensors and Leak test

- ☑ Zero all pressure sensors using the Browser interface.
- ☑ Perform inlet pressure decay test(s) from the diagnostics screen on the Browser User interface. Record if test passed or failed in the results table.

Note: If the PM is done in preparation for an Operational Qualification, then the pressure decay test defined within that protocol can be used for the PM

เอกสารไม่ควบคุม

System Information

☑ Check this box if an instrument configuration report is attached instead of completing the table below.

Instrument System Name and ID	UAE-TOX.009/2566 / US2229A024
Instrument System Site and Location	UAE / Room 404

List System Component Product Numbers	List the Serial Numbers of each Component
1. G4460A	US2229A024
2. G4519A	CN22285350
3. G4514A	CN2228 7018
4.	
5.	
6.	
7.	
8.	
9.	
10.	

Preparation

- ☑ Discuss any specific issues with the customer before starting.
- ☑ Review the instrument logbook for recorded problems and comments.
- ☑ Save instrument control settings before starting the procedure.
- ☑ Perform a general inspection of the system for cleanliness.
- ☑ Check for proper installation of parts, assemblies, sensors etc.
- ☑ Check system for required installation of components, settings as defined by current Service Notes.
- ☑ Check for required firmware updates and verify with customers if they would like them installed.
- ☑ Before starting the following procedures, record the Detector Signal Output(s) in the results table. If the GC is turned OFF or in a service mode, comparing the detector outputs before and after the service is not possible.

เอกสารไม่ควบคุม

ALS Maintenance

- ☐ **Section NOT applicable**
- ☑ Check all cabling and configuration settings between GC, tray, and injectors.
- ☑ Vacuum or remove any dust, especially around fans.
- ☑ Check operation of all fans.
- ☑ Check syringe for smooth plunger operation.
- ☑ Check for smooth operation of the needle support – clean if necessary

Restore Instrument

- ☑ Restore the normal operating conditions or customer method using the Browser interface or Data System.
- ☑ Purge the system with carrier flow for 15 minutes
- ☑ Bake out the system, then restore the normal operating conditions
- ☑ After equilibration, check and record the post PM detector signal output values. Results should be similar or lower than the detector outputs recorded prior to PM
- ☑ Perform a chemical checkout. If this is a routine PM, inject the customer's sample using the ALS if applicable. This will act as a final checkout of both the ALS and the GC.

Note: If the PM Service is performed prior to a qualification service, then use the qualification procedure as a guide for final instrument set up and checkout.

เอกสารไม่ควบคุม

Signature Page

Service Review

- ☐ Attach available reports/printouts of all tests to this documentation.
- ☑ Record the Preventive Maintenance service activity in the customer's records/logbook.
- ☑ Update/reset instrument maintenance counters as appropriate.
- ☑ Affix the PM sticker to the system or instrument logbook based on the customer's request.
- ☑ Complete the Service Engineer Comments section if there are additional comments.
- ☑ Review with the customer this service, parts replaced, and test results obtained.
- ☑ If the instrument firmware was updated, record the details of the change in the Service Engineer's Comments box or if necessary, in the customer's IQ records.
- ☐ Supply the customer with a copy of the Smart Alerts flyer.
- ☐ Describe Smart Alerts to the customer.
- ☐ Install Smart Alerts if requested.

PM Test Results Table

Test description	Before PM Service	After PM Service
Front detector output	N/A	249.1 Hz
Back detector output	N/A	19.9 pA
AUX 1 detector output	N/A	N/A
AUX 2 detector output	N/A	N/A
Test description	**Expected test result**	**Actual test result**
Leak and Restriction Test after front inlet maintenance	Pass	Pass
Leak and Restriction Test after back inlet maintenance	Pass	Pass
Leak and Restriction Test after front inlet Split Vent Trap replacement	Pass	Pass
Leak and Restriction Test after back inlet Split Vent Trap replacement	Pass	Pass
Front inlet pressure decay test	Pass	Pass
Back inlet pressure decay test	Pass	Pass

เอกสารไม่ควบคุม

Service Engineer Comments

If there are any specific points you wish to note as part of performing the service or other items of interest for the customer, please write include them in this box.

Service Completion

Service request number 6077579060

Date service completed 16 Jun. 2025

Agilent signature

Customer signature 16/June/2025

Total number of pages in this document 9 pages

เอกสารไม่ควบคุม

PM Parts List Table

Note: The following kits are recommended for capillary and purged packed inlets. If this is a general PM and the customer has a preferred set of consumables, you may use the customer's consumables.

Part description	Part number	Product or model# where used	Quantity consumed
SSL Capillary Inlet PM kit, Splitless	5188-6497	8890 GC	N/A
SSL Capillary Inlet PM kit, Split	5188-6496	8890 GC	1
SSL Capillary Ultra Inert Inlet Gold Seal with Washer	5190-6144	8890 GC	N/A
SSL Capillary Ultra Inert Inlet Splitless Liner - Single taper with Glass Wool	5190-2293	8890 GC	N/A
SSL Capillary Ultra Inert Inlet Low Pressure Drop Split Liner - with Glass Wool	5190-2295	8890 GC	N/A
PP Inlet PM kit	5188-6498	8890 GC	N/A
Split vent trap PM kit, single cartridge (for MMI, PTV & VI)	5188-6495	8890 GC	N/A
MMI Cleaning Kit	G3510-60820	8890 GC	N/A
PTV Septumless Head Rebuild Kit	5182-9747	8890 GC	N/A
PTV Septumless Head Teflon Guide	5182-9748	8890 GC	N/A
Ignitor (glow plug) assembly with O-ring	19231-60680	8890 GC	1
FID Collector Rebuild/Cleaning Kit	G1531-67000	8890 GC	N/A
FID Collector Replacement Kit	G1531-67001	8890 GC	N/A
Standard .011-inch FID Jet	5200-0176	8890 GC	1
Universal .018-inch FID Jet	5200-0177	8890 GC	N/A

เอกสารไม่ควบคุม

DQE Services

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

CERTIFICATE OF CALIBRATION

Certificate No. : SP25-021 Page 1 of 5

Customer : United Analyst and Engineering Consultant Co.,Ltd. (Head Office)

Address : 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Location of calibration : Instrument room (207)

Equipment : UV-Vis Spectrophotometer

Manufacturer : HITACHI

Model : U-2900

Serial No. : 21E22-009

ID No. : UAE.WAT.051/2564

Received Date : 26 May 2025

Calibration Date : 26 May 2025

Issue Date : 29 May 2025

Condition Instrument : Good

Calibrated by : (Mr.Tanawut Rittidach) Technical Manager

Approved by : (Ms.Chonticha Sangngern) Quality Manager

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the DQE Services Co., Ltd.

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP25-021

Environment Condition : Ambient Temperature 25 ± 5 °C

Relative humidity 55 ± 20 %RH

Calibration method : In-house method CP-01 Based on ASTM E275-08

Certified Reference Materials :

Material	Serial No.	Certificate No.	Due date
Absobance Standard set	25760	115663	25 October 2025
Absobance Standard set	25757	115638	25 October 2025
Wavelength Standard set	25806	115657	25 October 2025
Wavelength Standard set	25758	115665	25 October 2025

Traceability : This certification is traceable to the International System of Unit maintained at National - Institute of Standards and Technology (NIST) through Starna Scientific Limited

Spectral Band Width of UUC : 1.5 nm.

Scan Speed of UUC : 200 nm/min

Scan Interval of UUC : 0.1 nm.

Resolution of UUC : Photometric 0.001 Abs.

Wavelength 0.1 nm.

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP25-021

Calibration Results : Without adjustment

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
420	0.0000	0.000	0.0000	0.0028	2.00
	0.5780	0.574	0.0040	0.0031	2.00
	1.0484	1.043	0.0054	0.0029	2.00
	2.1876	2.185	0.0026	0.0075	2.00
440	0.0000	0.000	0.0000	0.0028	2.00
	0.5595	0.558	0.0015	0.0034	2.00
	1.0239	1.022	0.0019	0.0035	2.00
	2.1230	2.121	0.0020	0.0079	2.00
465	0.0000	0.000	0.0000	0.0028	2.00
	0.5230	0.519	0.0040	0.0030	2.00
	0.9633	0.960	0.0033	0.0029	2.00
	1.9753	1.973	0.0023	0.0070	2.00
546.1	0.0000	0.000	0.0000	0.0028	2.00
	0.5181	0.516	0.0021	0.0031	2.00
	1.0002	0.998	0.0022	0.0033	2.00
	1.9973	1.995	0.0023	0.0084	2.00
590	0.0000	0.000	0.0000	0.0028	2.00
	0.5517	0.550	0.0017	0.0030	2.00
	1.0803	1.080	0.0003	0.0030	2.00
	2.0373	2.036	0.0013	0.0079	2.00
635	0.0000	0.000	0.0000	0.0028	2.00
	0.5591	0.558	0.0011	0.0031	2.00
	1.0518	1.051	0.0008	0.0030	2.00
	1.9274	1.926	0.0014	[illegible]	[illegible]

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP25-021

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
235	0.0000	0.000	0.0000	0.0050	2.00
	0.7469	0.748	-0.0011	0.0057	2.00
257	0.0000	0.000	0.0000	0.0050	2.00
	0.8674	0.866	0.0014	0.0059	2.00
313	0.0000	0.000	0.0000	0.0050	2.00
	0.2919	0.291	0.0009	0.0051	2.00
350	0.0000	0.000	0.0000	0.0050	2.00
	0.6430	0.640	0.0030	0.0055	2.00

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP25-021

Wavelength Accuracy :

CRMs Values (nm.)	UUC Reading (nm.)	Correction (nm.)	Uncertainty (nm.)	Coverage factor k
241.72	241.0	0.72	0.18	2.00
279.45	278.8	0.65	0.18	2.00
287.81	287.2	0.61	0.18	2.00
334.06	333.6	0.46	0.18	2.00
360.93	360.6	0.33	0.18	2.00
418.59	418.2	0.39	0.18	2.00
445.94	445.6	0.34	0.18	2.00
460.02	459.8	0.22	0.18	2.00
536.59	536.6	-0.01	0.18	2.00
637.98	638.0	-0.02	0.18	2.00
431.38	431.2	0.18	0.18	2.00
472.50	472.4	0.10	0.18	2.00
513.47	513.4	0.07	0.18	2.00
528.88	528.8	0.08	0.18	2.00
573.17	573.2	-0.03	0.18	2.00
585.35	585.0	0.35	0.20	2.00
684.40	684.4	0.00	0.18	2.00
740.72	741.0	-0.28	0.20	2.00
748.55	748.8	-0.25	0.18	2.00
807.03	807.2	-0.17	0.18	2.00
879.28	879.6	-0.32	0.18	2.00

Remark : - UUC = Unit Under Calibration

- N/A = Not Available
- The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%

- End of Certificate -

เอกสารไม่ควบคุม

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

Certificate of Calibration

Cert.No.: 25CH1053
Page.: 1 of 2

Equipment :	Turbidity Meter
Manufacturer :	Oakton
Model :	T100IR
Serial No. :	1120501017
ID. No. :	UAE.WAT.056/2563
Condition As-Received:	Used Item
Received Date :	05 September 2025
Calibration Date :	08 September 2025
Reference :	2509-0212DSC-1
Submitted by :	United Analyst and Engineering Consultant Co.,Ltd. 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Ambient Temperature :	(23 ± 3.0) °C
Relative Humidity :	(50 ± 20) %
Calibration Procedure :	In - house method : CP-CH11 Direct measurement by using Formazin standard solution
Calibrated by :	Walalak Sirithean
Approved by :	Approved Signatory

( ) Chakrit Waewwanjua
( ) Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 9 September 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Calibration and Testing Equipment Services.

เอกสารไม่ควบคุม

สถาบันวิจัยและพัฒนาอุตสาหกรรมอาหาร
กรมส่งเสริมอุตสาหกรรม
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

Calibration Certificate

Certificate No.: 2602300-001-01
Page : 1 of 2

Equipment:	CHAMBER (Hot Air Oven)		
Manufacturer:	MEMMERT	**Customer Name:**	UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Model:	UF55	**Address:**	3 Soi Udomsuk 41, Sukhumvit Road
Serial No.:	B212.0411		Bangchak, Phrakhanong, Bangkok 10260
ID No.:	UAE.WAO.035/2555		
Order No.:	2602300		
Operation No.:	2602300-001		
Date of Receipt:	11 March 2026		
Date of Calibration:	11 March 2026		

Metrological traceability:

1. Calibration Method:
   - The instrument was calibrated by inserting 9 standard thermometers into its chamber, in accordance with W TE-014, based on TLAS G-20-1/02-08 (E): Guidelines for Calibration and Checks of Temperature Controlled Enclosures.
   - The temperature scale used in this laboratory is the International Temperature Scale of 1990 (ITS-90).
   - All data shown below are final values, and the initial data may be obtained upon request.
2. Reference Standard Instrument

Instrument	Model/Type	Serial No./ID No.	Certificate No.	Due Date	Through
Digital Thermometer with sensor	34972A RTD	MY56003932 CH401-266-RTD401-266	2502797.002.01	3 May 2026	NATIONAL FOOD INSTITUTE

3. This certificate is traceable to the International System of Units (SI).
4. This certificate is valid only for the instrument that was calibrated.
5. The result of this calibration was found to be accurate only on the date and at the place of calibration shown.

Calibrated by	Mr.Manas Somsak Specialist	**Approved by**	(Mr.Pheraphat Tuanjit) Manager, Division of Calibration Laboratory Responsible for the Technical Management Team
Date of Issue:	18 March 2026		

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

2008 ซอยอุดมสุข 36 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel +66(0) 2422 8688 Fax +66(0) 2422 8545
nfi.or.th

เอกสารไม่ควบคุม

Cert.No. : 25CH1053
Page. : 2 of 2

Condition of this calibration result

1. Reference Standard Instruments :

Instruments	ID No.	Certificate No.	Due date
1) Data Logger	130EC012	24H2043	23 Sep 2025
2) Liquid-in Glass Thermometer	130RC003	25I440	16 Apr 2026

- This measurement result is traceable to SI through Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials : Turbidity Standard solution (Formzin)
   - The measurement results are traceable to SI through CPA chem Ltd.,

Turbidity Solution	Manufacturer	Lot No.	Exp. date
20.0 NTU	CPA Chem	1088008	18 Mar 2026
100.0 NTU	CPA Chem	1088007	18 Mar 2026
400 NTU	CPA Chem	1088018	18 Mar 2026
800 NTU	CPA Chem	1088017	18 Mar 2026

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration result

Performing five - Formazin suspension standard curve by using 0, 20, 100, 400, 800 NTU
Tubidity Meter serial number : 1120501017

Standard Formazine suspension (NTU)	UUC* Reading (NTU)	Uncertainty of Measurement (± NTU)	Coverage Factor *k*
0	0.00	0.026	2.00
20.0	20.2	0.20	2.00
100.0	100	1.2	2.00
400	403	2.4	2.00
800	799	4.3	2.00

Remark - UUC* = Unit Under Calibration
- NTU = Nephelometric Turbidity Units

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k* , providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม

สถาบันวิจัยและพัฒนาอุตสาหกรรมอาหาร
กรมส่งเสริมอุตสาหกรรม
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

Calibration Certificate

Certificate No.: 2602300-001-01
Page : 2 of 2

Calibration Condition:

Equipment:	CHAMBER (Hot Air Oven)	**Place of Calibration:**	Laboratory
UUC* Resolution:	0.1 °C		UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Condition of the item:	Normal & Good	**Environment Conditions:**	Ambient Temperature (23.8 ± 1.0) °C
	Without adjustment / As Found		Relative Humidity (47.8 ± 4) %
	- Time of record 1 hour 9 minute / point		Line Voltage (222 ± 3) V

Calibration Results:

Table1 : Reporting of Temperature

Calibration Point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.9 is REF) Std.#1	Std.#2	Std.#3	Std.#4	Std.#5	Std.#6	Std.#7	Std.#8	Std.#9	Measurement Uncertainty (±°C)
104.0	104.22	103.87	103.90	104.17	103.96	103.98	104.22	104.17	104.00	0.53
120.0	120.21	119.78	119.86	120.15	119.83	119.85	120.24	120.20	119.96	0.73
180.0	180.27	179.37	179.73	180.31	179.61	179.13	180.35	180.25	179.84	0.99

Table 2 : Reporting of Characterization Results


UUC* Setting (°C)	UUC* Reading (°C) Max	Min	Average	Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
104.0	104.0	104.0	104.0	0.05	0.44	0.75
120.0	120.0	120.0	120.0	0.05	0.43	0.79
180.0	180.0	180.0	180.0	0.07	0.93	1.56

Note
- UUC* : Unit Under Calibration
- The quoted uncertainty includes contributions from Stability and Loading Effect (2)% of Temperature Uniformity)
- Stability = One half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.
- Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature of the reference location which are observed at the same time.
- Overall Variation = The difference of The maximum and minimum measured temperatures throughout observation time.

For more information, details of the sensor installation should be reported.

Fresh air Damper: Open / Posters; X Close / 100% Fan speed; - Not Available

Dimension of inside chamber and sensor installation location (cm)			
W x H x D	49	x 48	x 33
a x b x c	10	x 10	x 10



The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k = 2, providing a level of confidence of approximately 95 %.

-------- End of Report --------

2008 ซอยอุดมสุข 36 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel +66(0) 2422 8688 Fax +66(0) 2422 8545
nfi.or.th

เอกสารไม่ควบคุม

Agilent

Agilent AA Series Spectrometers

Preventative Maintenance Checklist

[redacted]

Foreword

Agilent Preventive Maintenance provides factory recommended service for your analytical systems to assure reliable operation and the accuracy of your results.

Delivered by highly trained and certified service engineers using genuine Agilent parts and supplies, Agilent Preventive Maintenance provides everything you need to reduce unplanned downtime and keep your systems operating at their peak. This checklist will be completed at the end of the service and provided to you as a record of the installation.

NOTE While non-current production AA instrument and or accessory models are not covered specifically in this document it can be used as a basic reference.

For more information about Agilent Technologies services please visit our web site using the following URL http://www.agilent.com/en-us/services

เอกสารไม่ควบคุม

Customer information

- Customers should provide all necessary operating supplies upon request of the engineer.
- A customer representative should be available to the engineer while performing the preventive maintenance procedures.
- Any parts, not included in the Parts Lists section of this document, are not part of the recommended Preventive Maintenance service, nor are they included in the price of this service.
- If a system requires the use of extra or special procedures and/or parts for the maintenance service, then these must be ordered separately and charged as a repair, which may incur additional costs.

Service Engineer's Responsibilities

- Contact the customer and ensure that all necessary supplies are available before the preventive maintenance visit.
- Confirm the ability of the instrument to deliver continued safe operation as established via the Agilent AA safe operation flow chart. **(Refer directly to the AA 55/240/280 Preventive Maintenance Scope of Work to make this decision.)**
- Only select those pages that relate to the system or module being serviced.
- Complete empty fields with the relevant information.
- Complete the relevant checkboxes in the checklist using either a "X" or tick mark "√".
- Check "Section not applicable" check boxes to indicate services/tasks not delivered, as appropriate.
- Complete the Preventive Maintenance service in the order of the tasks listed.
- Complete the Service Review section together with the customer.
- Complete the fields for page numbers at the foot of each selected page.
- Complete the total number of pages field in the Service Completion section.
- Ask the customer to sign the Service Completion section including the customer's and your signature.

This information is subject to change without notice.

Other important Customer Web links

- How to get information on your product: Literature Library – http://www.agilent.com/chem/library
- Need to know more? www.agilent.com/chem/education
- Need technical support, FAQs? www.agilent.com/chem/techsupp
- Need supplies? www.agilent.com/chem/supplies

Revision: 12.0, Issued: November 2025
Document Number: D0140137
© Agilent Technologies, Inc. 2025

Agilent

เอกสารไม่ควบคุม

Contents

Customer information	3
Service Engineer's Responsibilities	3
Other important Customer Web links	3
System information	4
Preparation, Safe operation and initial performance checks	4
Preventative maintenance procedures	5
Flame systems	5
Furnace systems	6
Accessories	8
Restore System	9
Guidance	9
Signature Page	9
Service Review	9
Test Results	10
AA consumable and parts list	10
Service Engineer Comments (optional)	11
Service Completion	12

Revision: 12.0, Issued: November 2025
Document Number: D0140137
© Agilent Technologies, Inc. 2025

Agilent

เอกสารไม่ควบคุม

System information

☐ Check this box if an instrument configuration report is attached instead of completing this table.

Instrument system name and ID	240FS AAS
Instrument system site and location	United Analyst and Engineering Consultant
List system component product numbers	List the serial numbers of each component
1 G9432A	1 MY13160001
2	2
3	3
4	4
5	5
6	6
7	7
8	8
9	9
10	10

Preparation, Safe operation and Initial performance checks

☐ Agilent AA safe operation flow chart inspections (to determine if the PM can be performed).

NOTE If by following the flow chart the instrument is deemed to be unsafe for continued use you MUST NOT continue PM work. Inform the customer immediately of the Agilent recommendation that use of the instrument be discontinued.

☑ Discuss any specific questions or issues with the customer prior to starting.
☐ For HF application systems, if standard sample introduction system was not installed, ask the customer to install it. N/A
☑ Review the instrument logbook for recorded problems and comments.
☑ Save instrument control settings before starting the procedure.
☑ Perform a general inspection of the system for cleanliness.
☑ Check for proper installation of parts, assemblies, sensors etc.
☑ Check system for required installation of components, settings as defined by current Service Notes.

Revision: 12.0, Issued: November 2025
Document Number: D0140137
© Agilent Technologies, Inc. 2025

Agilent

เอกสารไม่ควบคุม

- [x] Check for required firmware updates and verify with customers if they would like them installed
- [x] Use SVD to perform a Full Wavelength Scan for Cu HCL - "As found test_1"
- [x] Perform a Basic Cu ABS test - "As found test_2"
- [x] Print the Details page or screen captures of the test results and attach to the end of this checklist.

Preventative maintenance procedures

Flame systems

- [ ] Section NOT applicable.

Electronic components

- [x] Review and confirm instrument configuration data in SVD
- [x] Confirm power supply voltages using the SVD Power Supply diagnostic.
- [x] For Dual Beam instruments - Confirm RBC frequency using the SVD RBC frequency diagnostic.

Mechanical components

- [x] Check the burner adjuster controls for complete and free movement. If the burner adjuster needs lubrication, use Molykote 321 or mineral-based molybdenum disulphide grease.
- [x] Run SVD tests to exercise all motor drives over the full range of their travel:
  - [x] Monochromator drive
  - [x] Slit drive
  - [x] Lamp selector
  - [ ] Automatic Burner Adjuster

Optics components

- [x] Check that external optical surfaces are clean – Clean or replace as required.
- [x] Use SVD and perform Mono Wavelength Correction.
- [x] Use SVD and perform Slit Calibration.
- [x] Use SVD and perform Grating Squareness Diagnostic.
- [x] Use SVD and perform Zero Order Offset/Mono Correction.
- [x] Use SVD and perform Wavelength Repeatability.
- [x] Physically inspect selected HC lamps (customer to supply per their choice) and measure the % Gain for each lamp. Advise customer if lamps are showing emission degradation due to age.
- [x] Check that the signal energy of the D2 and HC lamps track properly. Advise customer if their D2 lamp is showing emission degradation due to age.

Agilent
เอกสารไม่ควบคุม

- [ ] Lamp selector

Optics components

- [ ] Check that external optical surfaces are clean – Clean or replace as required.
- [ ] Use SVD and perform Mono Wavelength Correction.
- [ ] Use SVD and perform Slit Calibration.
- [ ] Use SVD and perform Grating Squareness Diagnostic.
- [ ] Use SVD and perform Zero Order Offset/Mono Correction.
- [ ] Use SVD and perform Wavelength Repeatability.
- [ ] Physically inspect selected HC lamps (customer to supply per their choice) and measure the % Gain for each lamp. Advise customer if lamps are showing emission degradation due to age.

Gas handling, water system, and workhead component checks

- [ ] Inspect the GTA workhead gas hoses and connections for leaks.
- [ ] Pressure test for gas leaks
- [ ] If the cooler system is accessible (stand-alone) check for correct operation and coolant/water level – this includes any temperature and pressure settings plus filter cleaning (air flow and water).
- [ ] Inspect the GTA workhead water hoses and connections for leaks.
- [ ] Check all graphite components and replace if necessary.
  - [ ] Tube
  - [ ] Electrodes
  - [ ] Shroud
- [ ] Check and clean the end windows on the workhead.
- [ ] Check safety interlock operation.

Analytical performance for Furnace systems

- [ ] Optimize the instrument ready to perform Cu sensitivity test.
- [ ] Run the sensitivity test for a 25 ppb copper sample and record the results in the results table.

PSD autosampler accessory for Furnace systems

- [x] Section NOT applicable.
- [ ] Check condition of the PSD capillary – replace if necessary
- [ ] Check condition and operation of PSD syringe – ensure it does not have air locks and bubbles.
- [ ] Change PSD rinse bottle o-ring.
- [ ] Check and clean the rinse vessel.
- [ ] Check the drain tube for good drainage. It should not have tight bends, kinks or loops and the lower end must be above the liquid level in the waste vessel.
- [ ] Ensure that the waste vessel is suitable for use with the furnace system.

Agilent
เอกสารไม่ควบคุม

Sample introduction and Atomization

- [x] Inspect the burner interlock plate to ensure that the interlock pin is secure and correct for the burner type.
- [x] Clean the burner slot with a clean white card.
- [x] Check the uniformity of the slot width.
- [x] Clean the burner if required.
- [x] Change the burner o-ring and lubricate with PFPE grease.
- [x] Clean the nebulizer, spray chamber and liquid trap.
- [x] Change all o-rings and seals in the nebulizer, nebulizer block and spray chamber and lubricate.
- [x] Check that the pressure relief bung releases readily.
- [x] Change o-rings on the fuel and oxidant delivery barbs and lubricate.
- [x] Leave the liquid trap EMPTY and verify the flame will not ignite in this state.
- [x] Refill liquid trap and check that overfill drains freely into the drain/waste tube.
- [x] Check the drain/waste tube for good drainage. It should not have tight bends, kinks or loops and the lower end must be above the liquid level in the waste vessel.
- [x] Check and clean the igniter electrode.

Gas handling components and safety interlocks

- [x] Pressure test for leaks
- [x] Leak test gasbox internal components using gasbox leak tester G8434-67013
- [x] Check safety interlock status and operation using the SVD interlock monitoring diagnostic.

Analytical performance for Flame systems

- [x] Ignite a flame.
- [x] Check that you can adjust the nebulizer uptake rate from 4 to 6.5 mL per minute.
- [x] Optimize the instrument ready to perform Cu sensitivity test.
- [x] Create a manual method to perform a Basic Cu ABS test - "Final Performance Testing."
- [x] Run a PM completed sensitivity test for a 5 ppm copper sample and record the results in the AA PM Performance test results and measurements table.

Furnace systems

- [x] Section NOT applicable.

Electronic components

- [ ] Review and confirm instrument configuration data in SVD
- [ ] Confirm power supply voltages using the SVD Power Supply diagnostic.

Mechanical components

- [ ] Run SVD tests to exercise all motor drives over the full range of their travel:
  - [ ] Monochromator drive
  - [ ] Slit drive

Agilent
เอกสารไม่ควบคุม

Accessories

- [ ] Section NOT applicable.

Sample introduction pump system (SIPS) accessory

- [x] Section NOT Applicable.
- [ ] Re-torque screws securing the hubs, presser arms and pump rotors.
- [ ] Adjust each roller so that it rotates freely.
- [ ] Wipe clean the pump rotor rollers and pump bands with a dry clean cloth.
- [ ] Ensure that the presser arms and the surfaces near the pump are free from dirt and spills.
- [ ] Remove the pump module rear cover and check for the incursion of liquids and any signs of corrosion.
- [ ] Re-torque the nuts that fasten the motor mounting plates to the chassis.
- [ ] Check clips securing the diluents holder and replace if necessary.
- [ ] Disconnect, clean T-piece, and reassemble the tubing using the following steps.
- [ ] Remove the T-piece by disconnecting the pump tubes, the pump bands and all other tubing.
- [ ] Place the T-piece in an ultrasonic bath containing strong detergent 1-5% Decon 30 or similar, for approximately 5-10 minutes.
- [ ] Wash the T-piece under a tap with a strong flow of water.
- [ ] Rinse with distilled water through all of the inlets in the reverse direction to normal sample flow.
- [ ] Reassemble.

Sample preparation system (SPS 4) accessory

- [x] Section NOT Applicable.

The Agilent SPS 4 autosampler is designed to need minimal maintenance.

The following maintenance requirements are suggested to maintain the performance of the autosampler.

- [ ] Cleaning the spill tray, rack location mat, end frames and chassis accessories with a damp soft cloth and diluted mild detergent.
- [ ] Cleaning the autosampler cover panels with domestic window cleaner.
- [ ] Checking the X- axis and Z- axis drive belts for cracks, splits, damaged teeth, excessive fraying, color changes or degradation from fumes.
- [ ] Check the X- axis, Theta- axis and Z- axis FFC cables for cracks, incorrect positioning, damaged edge or damaged connectors.

NOTE The autosampler requires no extra lubrication throughout its lifetime.

For further details refer to the SPS 4 service manual G8410-90050.

Agilent
เอกสารไม่ควบคุม

Vapor generation accessory VGA (hydride generator)

- ☐ Section NOT Applicable.
- ☐ Inspect VGA gas supply hose.
- ☐ Inspect/replace VGA pump tubing.
- ☐ Check low gas pressure interlock setting– adjust if required.
- ☐ Check precision orifice gas flow setting – adjust if required.
- ☐ Check gas regulator pressure to 46 psi (325 kPa) – adjust if required.
- ☐ Clean the exterior surfaces of the accessory with soft lint free cloth. This cloth can be dampened with warm water or a mild detergent. Do not use organic solvents or abrasive cleaning agents.

UltrAA Lamp Accessory (external)

- ☑ Section NOT Applicable.
- ☐ Check the condition of the power cable.
- ☐ Clean the exterior surfaces of the accessory with soft lint free cloth. This cloth can be dampened with warm water or a mild detergent. Do not use organic solvents or abrasive cleaning agents.

Restore System

- ☐ If you have altered the customer's instrumentation during the course of PM, restore to the original status to allow the customer to conduct their normal activities (e.g., reload the customer's method.)

Guidance

If the PM service is performed prior to a qualification service, then use the qualification procedure as a guide for final instrument set up and checkout.

Signature Page

Service Review

- ☐ Attach available reports/printouts of all tests to this documentation.
- ☐ Record the Preventive Maintenance service activity in the customer's records/logbook.
- ☐ Update/reset instrument maintenance counters as appropriate.
- ☐ Affix the PM sticker to the system or instrument logbook based on the customer's request.
- ☐ Complete the Service Engineer Comments section if there are additional comments.
- ☐ Review this service, parts replaced, and test results obtained with the customer.
- ☐ If the instrument firmware was updated, record the details of the change in the Service Engineer's Comments box or if necessary, in the customer's IQ records.

Agilent
เอกสารไม่ควบคุม

Teflon impact beads (5/pk): (organics only)	9910053900	55 240 280	consumable	Flame
Burner cleaning strip (100/pk)	9910053900	55 240 280	consumable	Flame
Window UV silica – round (right side)	2010082600	55 240 280	PM supplied	Common
Window UV silica – rectangular (left side)	2010082500	55 240 280	PM supplied	Common
Pad adhesive window (round)	4910012700	55 240 280	PM supplied	Common
Pad adhesive window (rectangular)	4910012800	55 240 280	PM supplied	Common
Electrode kit (1 pr) (D2)	6310003400	GTA120	PM supplied	Furnace
Shroud (D2)	6310003100	GTA120	PM supplied	Furnace
Zeeman electrode kit (1 pr)	5310003500	GTA120	PM supplied	Furnace
Zeeman shroud	6310003600	GTA120	PM supplied	Furnace
O-ring PSD rinse bottle	6910025900	PSD120	PM supplied	Furnace

* For engineers who only service AA instruments 5190-6279 can be used as a cheaper alternative for 5610030100.

Items classified as PM supplied in the above table are included in the standard PM.

Those classified as consumable should be provided by the customer or charged to the customer if supplied by the Agilent service engineer.

Service Engineer Comments (optional)

If there are any specific points you wish to note as part of performing the installation or other items of interest for the customer, please write them in this box.

Agilent
เอกสารไม่ควบคุม

Test Results

Test description	Expected test result	Actual test result
Flame optics PMT Gain test		
For copper at 324.8 nm, 4 mA, 0.5 nm slit width	< 55 %	46 %
Flame performance test with 5 ppm copper sample		
Air /acetylene, mixing paddle removed	Abs value > 0.5	0.6391
Air /acetylene, mixing paddle installed 10 replicates	%RSD < 1.0	0.7 %
Deuterium furnace optics PMT Gain test		
For copper at 324.8 nm, 4 mA, 0.5 nm slit width	< 55 %	-
Deuterium furnace performance test with 25 ppb copper sample (324.8 nm)		
Precision %RSD	≤ 4.0%	-
Abs value	≥ 0.15	-
Zeeman furnace analytical performance: 25 ppb copper sample (324.8 nm)		
Precision %RSD	≤ 4.0%	-
Abs value	≥ 0.15	-
MSR% (327.4 nm)	≥70 %	-

AA consumable and parts list

Part Description	Part Number	Product/Model # where used	PM supplied or Consumable	Instrument-Type
Test Solution – Cu 6ppm solution	6510030100	55 240 280	PM supplied	Common
Test Solution - Blank solution	5190-7001	55 240 280	PM supplied	Common
Copper, 1000 ug/ml, 100ml	5190-6279	55 240 280	*	Common
Kit, Mk 7 O-rings, aqueous, complete set	9910093400	55 240 280	PM supplied	Flame
Organic Kit	9910093500	55 240 280	PM supplied	Flame
Wire Nebulizer Cleaning	9910024700	55 240 280	consumable	Flame
Tubing-Capillary Std Nebs	9910024800	55 240 280	consumable	Flame
Capillary Tube Hivac Neb (3) (organics only)	9910044000	55 240 280	consumable	Flame
Glass impact beads (5/pk)	9910025700	55 240 280	consumable	Flame

Agilent
เอกสารไม่ควบคุม

Service Completion

Service Request Number: 6009858466
Service Engineer Name: Kanyakorn S
Service Engineer Signature: Kanyakorn S.

Date of Service Completion: 26 Jan 2026
Customer Name: Manida Hongo
Customer Signature:

Agilent
เอกสารไม่ควบคุม

SVD Results Report

VARIAN

Report ID:3 *Diagnostic Start Time:1/26/2026 8:39:56 AM* *Diagnostic End Time:1/26/2026 9:05:49 AM*

Customer: UAE *Service Engineer:* Kacyakorn S.

Address: *Contact Details:* 0263763#1

Instrument Configuration

Configuration:

Serial Number: MY13180001
Instrument Model: Varian AA140/240/280
Flame Instrument: True
Furnace Instrument: True
Zeeman Present: False
Internal Zeeman: False
Internal UltrAA: False
Optics Type: Double Beam
D2 BG Correction Fitted: True
Boot Block Version: 1.09

Turret Type: Automatic
Number Of Lamps: 4
Mono Type: Automatic
Gasbox Type: 'Y' Gas Box
Auto Burner Adjuster: False
Mains Frequency: 50
Firmware Version: 2.11
Photomultiplier Type: Normal(900nm)
PWB Version: 45

EEPROM Data:

Instrument Run Hours: 79270.602
Zero Wavelength Offset: 30.095
Mono Correction: 0.765
Flame Hours: 35125.582

D2 Run Hours: 58906.000
D2 Serial Number: not set !
D2 Install Date: 1/1/1970
D2 Original Intensity: 1.000
D2 Last Intensity: 475.000

Frequency:

Averaging Period: 30.0
Datapoint Count: 20

Upper Limit: 51.00
Average Frequency: 50.00
Lower Limit: 49.00
Highest Measured Frequency: 50.00
Lowest Measured Frequency: 50.00

Result: Passed

เอกสารไม่ควบคุม

Power Supply:

Averaging Period: 30.0
Datapoint Count: 20

	Lower Limit (V)	Actual (V)	Upper Limit (V)	Result:
12.00 V Rail	10.80	12.20	13.20	Passed
-12.00 V Rail	-13.20	-11.90	-10.80	Passed
5.00 V Rail	4.50	5.02	5.50	Passed
310.00 V Rail	279.00	320.00	341.00	Passed


เอกสารไม่ควบคุม

Optics

Beam Balance:


Lamp Type: Copper
Lamp Socket Used: 3
Peak Selected: 324.80
Lamp Alignment: Performed

'X' Lamp Screw

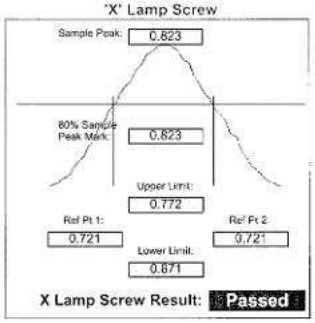

X Lamp Screw Result: Passed

'Y' Lamp Screw

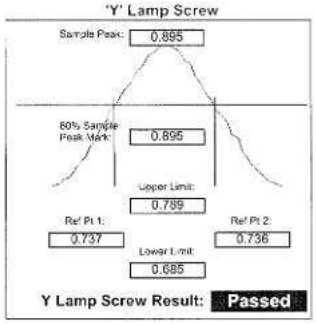

Y Lamp Screw Result: Passed

Grating Squareness:

Lamp Element(s): Copper
Lamp Turret Position: 3
Lamp Current(mA): 4.00
Slit Width(nm): 0.5
1st Order Wavelength(nm): 324.80
Lamp Alignment: Performed

	Lower Limit (nm)	Actual (nm)	Upper Limit (nm)	Result:
Zero Order	-0.10	0.00	0.10	Passed
First Order	324.45	324.74	325.15	Passed
Second Order	649.23	649.50	649.97	Passed

เอกสารไม่ควบคุม

Wavelength Repeatability:

Lamp Used: Copper
Peak Used(nm): 324.750
Connected to Socket: 3
Lamp Current(mA): 4
Slit Width(nm): 0.2
Slit Height: Normal

Lamp Alignment: Performed

Lower Limit(nm) 324.768 324.888 **Upper Limit(nm)**

(Approach from Zero Order)	*(Approach from end)*
Sample 1: 324.828	Sample 2: 324.823
Sample 3: 324.823	Sample 4: 324.823
Sample 5: 324.823	Sample 6: 324.819
Sample 7: 324.823	Sample 8: 324.819
Sample 9: 324.819	Sample 10: 324.819

Mean: 324.823 **Standard Deviation:** 0.003

Result: Passed

เอกสารไม่ควบคุม

Mechanical

Wavelength Drive: Passed

Slit Drive: Passed

Turret Drive: Passed

Auto Burner Adjuster Drive: Untested

Miscellaneous

Signal Processing Linearity:

Calculate Mode: New Calc Mode

	Lower Limit	Actual	Upper Limit	Result:
S0	114	261	297	Passed
S1	156	165	191	Passed
S2	271	296	332	Passed
S3	474	508	579	Passed
S4	825	919	1008	Passed
S5	1435	1529	1754	Passed
S6	2498	2771	3053	Passed
S7	4347	4755	5313	Passed

Interlocks:

Burner Fitted:	Working	Flame Detect:	Working
N2O Burner Fitted:	Untested	GCU Active:	Working
Flame Shield Closed:	Working	Oxidant Pressure:	Working
Gas Control Fitted:	Untested	Oxidant Changeover:	Untested
Pressure Release Bung Fitted:	Working	Ignition:	Working
Liquid Trap Fitted:	Working		

เอกสารไม่ควบคุม

Sequential by time report 1/26/2026 9:54 AM SpectrAA
Page 1 of 1

Analyst
Date Started 1/26/2026 9:07 AM GMT: 1/26/2026 2:07 AM
Worksheet Sensitivity Test
Comment
Methods Cu
Computer name DESKTOP-R9UFRS
Serial Number: MY13160001

Method: Cu (Flame)

Sample ID	Exp Abs	%RSD	Mean Abs	
5 ppm Cu	0.633	1.4	0.6331	
	Readings			
	0.6413	0.6340	0.6241	1/26/2026

เอกสารไม่ควบคุม

Auto Lamp Recognition:

Lamp 1: 87 - Silver/Cadmium/Lead/Zinc(UltrAA) (Ag/C	Lamp 5: Not Supported
Lamp 2: 68 - Zinc (Zn)	Lamp 6: Not Supported
Lamp 3: 14 - Copper (Cu)	Lamp 7: Not Supported
Lamp 4: Uncoded Lamp/Not Connected	Lamp 8: Not Supported

Result: Passed

GTA Temperature Monitoring: Not Performed

Notes:

Signatures:

Jawad Hayat	26 Jan 26	Kanyakorn S.	26 Jan 2026
UAE	Date	Kanyakorn S.	Date

เอกสารไม่ควบคุม

Sequential by time report 1/26/2026 10:15 AM SpectrAA
Page 1 of 1

Analyst
Date Started 1/26/2026 9:07 AM GMT: 1/26/2026 2:07 AM
Worksheet Precision Test
Comment
Methods Cu
Computer name DESKTOP-R9UFRS
Serial Number: MY13160001

Method: Cu (Flame)

Sample ID	Exp Abs	%RSD	Mean Abs			
5 ppm Cu	0.618	0.7	0.6189			
	Readings					
	0.6145	0.6187	0.6081	0.6158	0.6253	0.6196
	0.6197	0.6195	0.6188	0.6189	1/26/2026	

เอกสารไม่ควบคุม

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000 FAX. 0-2719-9484

Certificate of Testing

Cert.No.: 26TW50
Page.: 1 of 2

Equipment :	DO Meter
Manufacturer :	YSI
Model :	5100
Serial No. :	11B 101863
ID No. :	UAE.WAO.004/2554
Received Date :	27 February 2026
Test Date :	02 March 2026
Reference :	2602-0915DSC-1
Submitted by :	United Analyst and Engineering Consultant Co.,Ltd. 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Laboratory Condition :	Temperature (25 ± 5) °C Humidity (50 ± 20) %
Test Procedure :	In - house method : CP-CH9 by Comparison Technique with Azide Modification Method
Tested by :	Walalak Sirithean
Approved by :	Saithip Approved Signatory

( ) Chakrit Waewwanjua
( ) Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 03 March 2026

เอกสารไม่ควบคุม

United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel.0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

Certificate of Calibration

Certificate No.: 260311-2-BL001-26
Code No.: BL001-26
Page: 1 of 4

Customer Name:	United Analyst and Engineering Consultant Co., Ltd.			
Address:	3 Soi Udom suk 41, Sukhumvit Rd., Bang Chak, Phar Khanong, Bangkok 10260			
Equipment:	Electronic Balance			
Manufacturer:	Mettler Toledo			
Model:	XSR205DU			
Serial No.:	C210685394			
Asset No. :	UAE.WAO.010/2565			
Building :	UAE number 3	Floor : 2		Room : 208
Received Date:	March 11, 2026			
Date of Calibation :	March 12, 2026			
Calibration Conditions:	Temperature	23.0 °C	to	23.6 °C
	Humidity	51.5 %	to	54.4 %
	Pressure	755.7 mmHg	to	757.9 mmHg
Calibrated by:	Thanachat Chatpahol			
Approved by:	Suwit Chotnok	Signature:		
Issued Date:	March 16, 2026			

Note : 1) The Uncertainties are for a confidence probability of approximately 95%
2) This Certificate is valid only for the item calibrated on date and place of calibration.
3) This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the United Analyst and Engineering Consultant Co.,Ltd. (UAE).

เอกสารไม่ควบคุม

Cert.No.: 26TW50
Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :
This measurement result is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

Instruments	ID No.	Certificate No.	Due Date
1. Burette	130BU10	25CG1126	18 Mar 2027
2. Balance	110RC001	25MM316	02 July 2026

2. Standard Material :-

Material	Manufacturer	Lot.No.	Assay
Sodium Thiosulfate 5-Hydrate AR	KEMAUS	2203182447	99.6%

Result : **Dissolved Oxygen Meter Adjustment With Air 100 %**
Dissolved Oxygen Probe No.: 24F100202

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.20	8.20	0.0084

This report was certified only for the instrument we tested.It is allowable to use for study Intend to use for advertising and referral purpose is prohibited.This report may not be reproduced other in full, without written approval of the laboratory

-o0o-

เอกสารไม่ควบคุม

United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel.0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

Certificate No.: 260311-2-BL001-26
Code No.: BL001-26
Page: 2 of 4

Equipment: Electronic Balance
Manufacturer: Mettler Toledo
Model: XSR205DU
Readability: 0.01 mg , > 80 to 220.0 g : 0.1 mg
Serial No.: C210685394
ID No.: UAE.WAO.010/2565
Max. Capacity: 81 g / 220 g
Calibration Date: March 12, 2026
Condition As-Received: In Condition
Condition of Equipment:

Condition of This Result of Calibration:
1. Calibration Method: This instrument was calibrated by method UAE.CP-CAL-009 as In-house Method based on JJAPS Jan 01 2002
2. Reference Standards:

Reference Standard:	Model	Serial No.	Calibrated By	Certificate No.	Traceability	Due Date
Standard Weight Class E2 (OIML)	1 mg to 1 kg	C510641605	METTLER TOLEDO GmbH	C510641605	METTLER TOLEDO GmbH	3-Mar-27
Standard Weight Class E2 (OIML)	1 mg to 1 kg	B749109122	AMARC	23-009359	AMARC	23-Jan-27


Instrument	Model	Serial No.	Calibrated By	Certificate No.	Traceability	Due Date
Thermo-Hygro-Syro Meter	MHB-382SD	A4464437	SUCCESS	SSH-B0997/68	Success Gateway	26 Nov 26
Thermo-Hygro-Baro Meter	MHB-382SD	A4464437	TPA	25/9444	TPA	18 Dec 26

3. This certification is traceable to SI Unit.
4. This certification was certified only for the instrument we calibrated.
5. This result of calibration was found accurate as show on date and place of calibration only.
6. Through the reference standard laboratory of Mettler-Toledo GmbH C510641605, SAS accreditation number: SCS 0032
7. Through the reference standard laboratory of AMARC 23-009359, TISI accreditation number: 0432

Calibration Result:
1. Repeatability of Reading:

Nominal Value (g)	Standard Deviation of Reading (g)
60	0.000019
200*	0.000055

2. Eccentric or off-center loading
A mass of 100 g was placed and moved to various position on pan
The Balance reading obtained is given in the table.

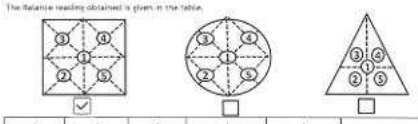

1 (g)	2 (g)	3 (g)	4 (g)	5 (g)	Maximum Difference (g)
100.0002	100.0002	100.0003	100.0004	100.0003	0.0001

เอกสารไม่ควบคุม

United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel.0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

Equipment:	Electronic Balance	Manufacturer:	Mettler Toledo
Model:	XSR205DU	Readability:	0 to 81 (g): 0.01 mg , > 80 to 200 (g) : 0.1 mg
Serial No.:	C210685394	ID No.:	UAE.WAO.010/2565
Max. Capacity:	81 g / 220 g		
Calibration Date:	March 12, 2026		

Calibraton Result: (Continued)
Calibraton Range: 0 to 80 (g)
Calibraton Adjustment: Internal Calibration

3. Error of Indication from nominal or conventional mass value: (Range: 0 to 81 (g) , Resolution: 0.00001 g)

Nominal Value (g)	Reference Value (g)	Indication (g)	Correction (g)	Uncertainty (± mg)	Coverage Factor k
Unload	0.0000000	0.00000	0.00000	0.032	2.65
0.001	0.0010020	0.00101	0.00000	0.032	2.65
0.005	0.0050025	0.00501	-0.00001	0.032	2.65
0.01	0.0100005	0.01001	-0.00001	0.032	2.65
0.05	0.0500003	0.05001	-0.00001	0.032	2.65
0.10	0.1000083	0.10000	0.00001	0.033	2.65
0.50	0.5000121	0.50001	0.00000	0.033	2.65
1	1.0000119	1.00005	-0.00002	0.032	2.52
2	2.0000125	2.00003	-0.00002	0.033	2.52
5	5.0000146	5.00003	-0.00002	0.033	2.32
10	10.0000330	10.00006	-0.00003	0.034	2.21
20	20.000028	20.00006	-0.00003	0.041	2.07
30	30.000061	30.00017	-0.00011	0.055	2.00
40	40.000054	40.00021	-0.00016	0.066	2.00
50	50.000037	50.00023	-0.00019	0.068	2.00
60	60.000070	60.00029	-0.00022	0.084	2.00
80	80.000098	80.00039	-0.00030	0.12	2.00

e.Cal

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
DQE Services
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

CERTIFICATE OF CALIBRATION

Certificate No. : SP25-024

Customer : United Analyst and Engineering Consultant Co.,Ltd. (Head Office)

Address : 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Location of calibration : Instrument room (207)

Equipment : UV-Vis Spectrophotometer

Manufacturer : HITACHI

Model : U-5100

Serial No. : 23A4-008

ID No. : UAE.WAS.010/2567

Received Date : 17 June 2025

Calibration Date : 17 June 2025

Issue Date : 20 June 2025

Condition Instrument : Good

Calibrated by : ธนุส
(Mr.Tanawut Rittidach)
Technical Manager

Approved by : ชลธิชา
(Ms.Chonticha Sangngern)
Quality Manager

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the DQE Services Co., Ltd.

เอกสารไม่ควบคุม

United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel.0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

Equipment:	Electronic Balance	Manufacturer:	Mettler Toledo
Model:	XSR205DU	Readability:	0 to 81 (g): 0.01 mg , > 80 to 200 (g) : 0.1 mg
Serial No.:	C210685394	ID No.:	UAE.WAO.010/2565
Max. Capacity:	81 g / 220 g		
Calibration Date:	March 12, 2026		

Calibraton Result: (Continued)
Calibraton Range: > 81 to 200 (g)
Calibraton Adjustment: Internal Calibration

3. Error of Indication from nominal or conventional mass value: (Range: > 81 - 220 (g) , Resolution: 0.0001 g)

Nominal Value (g)	Reference Value (g)	Indication (g)	Correction (g)	Uncertainty (± mg)	Coverage Factor k
Unload	0.0000000	0.0000	0.0000	0.032	2.65
90	90.0000910	90.0004	-0.0003	0.16	2.00
100	100.0000420	100.0003	-0.0003	0.16	2.00
110	110.0000750	110.0004	-0.0003	0.18	2.00
120	120.0000680	120.0004	-0.0003	0.19	2.00
130	130.0001010	130.0005	-0.0004	0.20	2.00
140	140.0000960	140.0004	-0.0003	0.21	2.00
150	150.0000790	150.0005	-0.0004	0.22	2.00
160	160.0001120	160.0006	-0.0005	0.23	2.00
170	170.0001050	170.0003	-0.0002	0.24	2.00
200	200.0001460	200.0001	0.0000	0.26	2.00

4. Effect of Tare test:

Tare Load (g)	Test Load (g)	Indication (g)	Correction (g)
100	20.000028	20.0001	0.0000
	40.000054	40.0001	0.0000
	60.000070	60.0000	0.0001
	80.000098	80.0000	0.0001
	100.000109	100.0000	0.0001

Remark: -
The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k, providing a level of confidence of approximately 95%

o---o-End-o---o

e.Cal

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
DQE Services
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP25-024

Environment Condition : Ambient Temperature 25 ± 5 °C

Relative humidity 55 ± 20 %RH

Calibration method : In-house method CP-01 Based on ASTM E275-08

Certified Reference Materials :

Material	Serial No.	Certificate No.	Due date
Absobance Standard set	25760	115663	25 October 2025
Absobance Standard set	25757	115638	25 October 2025
Wavelength Standard set	25806	115657	25 October 2025
Wavelength Standard set	25758	115665	25 October 2025

Traceability : This certification is traceable to the International System of Unit maintained at National - Institute of Standards and Technology (NIST) through Starna Scientific Limited

Spectral Band Width of UUC : 5.0 nm.

Scan Speed of UUC : 40

Scan Interval of UUC : 0.1 nm.

Resolution of UUC : Photometric 0.001 Abs.

Wavelength 0.1 nm.

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP25-024

Calibration Results : Without adjustment

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
420	0.0000	0.000	0.0000	0.0028	2.00
	0.5780	0.574	0.0040	0.0031	2.00
	1.0484	1.044	0.0044	0.0029	2.00
	2.1876	2.185	0.0026	0.0075	2.00
440	0.0000	0.000	0.0000	0.0028	2.00
	0.5595	0.558	0.0015	0.0035	2.00
	1.0239	1.021	0.0029	0.0035	2.00
	2.1230	2.122	0.0010	0.0079	2.00
465	0.0000	0.000	0.0000	0.0028	2.00
	0.5230	0.519	0.0040	0.0030	2.00
	0.9633	0.961	0.0023	0.0029	2.00
	1.9753	1.975	0.0003	0.0071	2.00
546.1	0.0000	0.000	0.0000	0.0028	2.00
	0.5181	0.515	0.0031	0.0031	2.00
	1.0002	0.996	0.0042	0.0033	2.00
	1.9973	1.994	0.0033	0.0084	2.00
590	0.0000	0.000	0.0000	0.0028	2.00
	0.5517	0.549	0.0027	0.0030	2.00
	1.0803	1.078	0.0023	0.0030	2.00
	2.0373	2.031	0.0063	0.0082	2.00
635	0.0000	0.000	0.0000	0.0028	2.00
	0.5591	0.557	0.0021	0.0031	2.00
	1.0518	1.049	0.0028	0.0030	2.00
	1.9274	1.924	0.0034	0.0081	2.00

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP25-024

Wavelength Accuracy :

CRMs Values (nm.)	UUC Reading (nm.)	Correction (nm.)	Uncertainty (nm.)	Coverage factor k
241.00	240.4	0.60	0.18	2.00
279.30	278.8	0.50	0.18	2.00
288.90	288.3	0.60	0.18	2.00
334.50	333.9	0.60	0.18	2.00
361.40	360.8	0.60	0.18	2.00
418.40	417.9	0.50	0.18	2.00
447.20	446.6	0.60	0.18	2.00
459.30	459.1	0.20	0.18	2.00
537.00	536.4	0.60	0.18	2.00
638.00	637.5	0.50	0.18	2.00
441.29	440.7	0.59	0.18	2.00
479.88	479.4	0.48	0.18	2.00
513.75	513.3	0.45	0.18	2.00
528.59	528.2	0.39	0.18	2.00
575.10	574.5	0.60	0.18	2.00
585.56	585.4	0.16	0.20	2.00
684.70	684.1	0.60	0.18	2.00
740.51	740.2	0.31	0.20	2.00
747.61	747.0	0.61	0.18	2.00
807.04	806.4	0.64	0.18	2.00
879.68	879.1	0.58	0.18	2.00

Remark : - UUC = Unit Under Calibration
- N/A = Not Available
- The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor *k*, which for a normal distribution corresponds to a coverage probability of approximately 95%

- End of Certificate -

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP25-024

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
235	0.0000	0.000	0.0000	0.0050	2.00
	0.7469	0.747	-0.0001	0.0057	2.00
257	0.0000	0.000	0.0000	0.0050	2.00
	0.8674	0.864	0.0034	0.0059	2.00
313	0.0000	0.000	0.0000	0.0050	2.00
	0.2919	0.293	-0.0011	0.0051	2.00
350	0.0000	0.000	0.0000	0.0050	2.00
	0.6430	0.639	0.0040	0.0055	2.00

เอกสารไม่ควบคุม

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

Certificate of Calibration

Cert. No.: 26TM194
Page : 1 of 3

Equipment :	Water Bath
Manufacturer :	Memmert
Model :	WNE 14
Serial No. :	L416.0612
ID No. :	MIC.003/2560
Submitted by :	United Analyst and Engineering Consultant Co.,Ltd. 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Location :	Microbiology Laboratory (302)
Received Order :	02 February 2026
Calibration Date :	02 February 2026
Ambient Temperature :	(26 ± 10) °C
Relative Humidity :	(50 ± 30) %
AC Line Voltage :	(220 ± 22) V
Calibrated by :	Krisda Malee
Approved by :	Kunchit Approved Signatory

( ) Chakrit Waewwanjua
( ) Suwit Imjai
(✓) Kunchit Promprat

Issue Date : 17 February 2026

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2602-0004OC-2
Cert. No.: 26TM194
Page : 2 of 3

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT04 Based on ASTM E715 according to direct measurement method with Data Acquisition which connected with Industrial Platinum Resistance Thermometer (IPRT).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-


Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY57013711	25LM117	TPA	17 Jul 2026

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This measurement result is traceable to the International System of Unit maintained through :

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Heat transfer medium used : Water

	Environmental		AC Voltage Supply
	(°C)	(%R.H.)	(Volt)
Beginning of Calibration	25	52	221
Finished of Calibration	24	51	220



Front

Position :	Ref. Std. ID No.:
1	4803988-001
2	4803988-002
3	4803988-003
4	4803988-004
5(ref.)	4803988-005

เอกสารไม่ควบคุม

Agilent CrossLab
From Insight to Outcome

Agilent CrossLab Start Up Services

Agilent 5100 5110 ICP-OES Preventive Maintenance

Agilent Preventive Maintenance provides factory recommended service for your analytical instruments to assure reliable operation and the accuracy of your results

Delivered by highly trained and certified service engineers using genuine Agilent parts and supplies, Agilent Preventive Maintenance provides what you need to reduce unplanned downtime and keep your systems operating at their peak performance.

This checklist is used as a guide for completing the preventive maintenance tasks. A signed copy of this checklist is provided for your records

Revision: A.02, Issued: 21 January 2022
Document Number: G8014-90075
© Agilent Technologies, Inc. 2022

Agilent

เอกสารไม่ควบคุม

Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2602-0004OC-2
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Cert. No.: 26TM194
Page : 3 of 3

Calibration point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Average* Standard Reading (°C) Position 1	2	3	4	5 (ref.)	Uncertainty (± °C)
44.5	44.6	44.6	44.518	44.463	44.472	44.508	44.521	0.15

Calibration point (°C)	Uniformity (°C)	Stability (± °C)	Coverage Factor *k*
44.5	0.11	0.044	2

Average* : The average of 30 values in each position.
Uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.
Stability : One-half of the greatest maximum difference of measured temperature at any one probe.
UUC* : Unit Under Calibration
Note : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม

Agilent CrossLab
From Insight to Outcome

Introduction

Customer Information

- Customers should provide all necessary operating supplies upon request of the engineer.
- A customer representative should be available to the engineer while performing the preventive maintenance procedures. Customers are responsible for regular maintenance and are encouraged to observe the service representative.
- Any parts not included in the Parts Lists section of this document are not part of the recommended Preventive Maintenance service nor are they included in the price of this service.
- If a system requires the use of extra or special procedures and/or parts for the maintenance service, then these must be ordered separately and charged as a repair, which may incur additional costs.
- For customers using HF applications, the instrument should be returned to its standard sample introduction system.

Revision: A.02, Issued: 21 January 2022
Document Number: G8014-90075
© Agilent Technologies, Inc. 2022

Agilent

เอกสารไม่ควบคุม

Important Customer Web Links

- To access **Agilent University**, visit http://www.agilent.com/crosslab/university/ to learn about training options, which include online, classroom and onsite delivery. A training specialist can work directly with you to help determine your best options.
- To access the **Agilent Resource Center** web page, visit https://www.agilent.com/en-us/agilentresources. The following information topics are available:
  - Sample Prep and Containment
  - Chemical Standards
  - Analysis
  - Service and Support
  - Application Workflows
- The **Agilent Community** is an excellent place to get answers, collaborate with others about applications and Agilent products, and find in-depth documents and videos relevant to Agilent technologies. Visit https://community.agilent.com/welcome
- Videos about specific preparation requirements for your instrument can be found by searching the **Agilent YouTube** channel at https://www.youtube.com/user/agilent
- **Need to place a service call?** Flexible Repair Options | Agilent

เอกสารไม่ควบคุม

Instrument Maintenance

System Information

☐ Check this box if an instrument configuration report is attached instead of completing the table.

Instrument System Name and ID	5110 VDV ICP-OES
Instrument System Site and Location	UAE Consultant

List System Component Product Numbers	List the Serial Numbers of each Component
1. G 8019 A	MY 19030001
2.	
3.	
4.	
5.	
6.	
7.	
8.	
9.	

ICP-OES Configuration Table	Circle the type or write in the type if other
Nebulizer Type	SeaSpray | OneNeb | Conikal | Other
Spray Chamber	Cyclonic Single Pass | Cyclonic Double Pass | Other
Torch	Radial | Dual View | Other
Torch Type	One Piece | Semi Demountable | Fully Demountable | Other
Injector Diameter	2.4mm | 3mm | 1.4mm | 0.8mm | Other
Injector Material	Quartz | Ceramic | Other

เอกสารไม่ควบคุม

Service Engineer's Responsibilities

- Contact the customer and ensure that all necessary supplies are available before the preventive maintenance visit.
- Only select those pages that relate to the system or module being serviced.
- Complete empty fields with the relevant information.
- Complete the relevant checkboxes in the checklist using either a "**X**" or tick mark "✓".
- Check **"Service not applicable"** check boxes to indicate services/tasks not delivered, as appropriate.
- Complete the Preventive Maintenance services in the most logical order relevant to the individual system service in the order of the tasks listed.
- Complete the **Service Review** section together with the customer.
- Complete the fields for page numbers at the foot of each selected page
- Add relevant page numbers to selected pages and complete the total number of pages field in the Service Completion section
- **Ask the customer to sign the Service Verification section including the customer's and your signature.**

เอกสารไม่ควบคุม

Preparation

- ☑ Discuss any specific issues with the customer before starting.
- ☑ Review the instrument logbook for recorded problems and comments.
- ☑ Save instrument control settings before starting the procedure.
- ☑ Perform a general inspection of the system for cleanliness.
- ☑ Check for proper installation of parts, assemblies, sensors etc.
- ☑ Check system for required installation of components and implementation of Service Notes
- ☑ Check for required firmware/software updates and verify with customers if they would like them installed.
- ☐ For HF application systems, if standard sample introduction system was not installed, ask the customer to install it. N/A
- ☑ Ask the customer to remove any samples from the ICP-OES sample introduction area, auto sampler or around the ICP-OES.

เอกสารไม่ควบคุม

Preventive Maintenance Procedures

Record Pre-PM instrument performance

- [x] Run Instrument Performance test.
- [x] Record results in Instrument Performance Test Results Table – Pre-PM.

Clean and inspect ICP-OES system

- [x] Look for any obvious external damage or problems.
- [x] Inspect water cooling hoses, gas lines and power cord for excessive wear or damage.
- [x] Perform a general internal inspection of the system for excessive dust accumulation, clean if necessary.
- [x] Inspect sample introduction components and record any required maintenance in the Service Engineer Comments and notify the customer as the required actions required.
- [x] Record the instrument operating conditions in the ICP-OES Status Results Table.
- [x] Replace the polychromator purge filter.
- [x] Replace the radial pre-optics window.
- [x] Replace the axial pre optics window for SVDV and VDV instruments.
- [x] Check exhaust flow for the correct positive extraction at the exhaust duct to insure they meet minimum specifications.
- [x] Replace air inlet dust filter.
- [ ] Replace high capacity air inlet dust filter element, if installed. N/A
- [x] Remove and clean instrument water inlet filter.

Agilent Water Recirculator

- [ ] **Service not applicable**
- [x] Drain cooling fluid and remove any particles from the chiller reservoir.
- [x] Remove, clean and reinstall water inlet metal mesh filter if present.
- [x] Re fill with Agilent Cool Clear cooling fluid.
- [x] Clean the cooling system Air filter and the condenser.

เอกสารไม่ควบคุม

ICP-OES adjustment

- [x] Check position of Zn peak, adjust if required.
- [x] Check Argon Ratio, adjust to specified value if required.
- [x] Perform Detector Calibration.
- [x] Perform Instrument Calibration.

Record Post-PM instrument performance

- [x] Run Instrument Performance test.
- [x] Record results in Instrument Performance Test Results Table - Post PM.
- [x] For systems using ICP Expert version 7.3 and above, run the following Instrument tests
  - [x] Subsystem Communications Test
  - [x] Air Flow
  - [x] Water Flow
  - [x] Gas Flows
  - [x] RF Generator
  - [x] Camera Test
  - [x] Optics Test
  - [x] Nebulizer Test
- [x] Record the result in the Instrument Test Results Table

เอกสารไม่ควบคุม

SPS 3 Auto Sampler

- [x] **Service not applicable**
- [ ] Power cycle the autosampler and verify successful initialization.
- [ ] Inspect X and Z axis belts for wear. Replace is necessary.
- [ ] Clean X and Z axis slide shafts.
- [ ] Using customer's racks and the Agilent software move the sample probe to the 4 outermost corners and rinse port, ensure that the probe is approximately centered in the vial.

SPS 4 Auto sampler

- [x] **Service not applicable**
- [ ] Clean the spill tray, rack location mat, end frames and chassis with a damp soft cloth and diluted mild detergent.
- [ ] Clean the auto sampler cover panels, if cover kit is installed, with domestic window cleaner.
- [ ] Check the X-axis and Z-axis drive belts for cracks, splits, damaged teeth, excessive fraying, color changes or degradation from fumes.
- [ ] Check the X-axis, Theta-axis and Z-axis FFC cables for cracks, incorrect positioning, damaged edges or damaged connectors.
- [ ] Pump Tubing Replacement. Replace peristaltic pump tubing. Replace all tubing that goes from the rinse station to the pump and from the pump to the waste/rinse bottles
- [ ] Test using customer's tray and move the sample probe to the sample vial 1, wash vial and rinse port and ensure that the probe is centered in the vial. If not use calibration wizard and calibrate the position.

AVS 4, 6, 7 Advanced Valve System

- [x] **Service not applicable**
- [ ] Replace valve rotor seal
- [ ] Check fittings for signs of leaks
- [ ] Check tubing including autosampler tubing for kinks or excessive wear
- [ ] Check high flow pump for signs of leaks

เอกสารไม่ควบคุม

Restore Instrument

- [ ] For HF applications, ask the customer to re install their sample introduction system. N/A
- [x] Leave system in an idle state: on and purging.
- [x] Guidance: If the PM service is performed prior to a qualification service, then use the qualification procedure as a guide for final instrument set up and checkout.

Service Review

- [x] Attach available reports/printouts of all tests to this documentation.
- [x] Record the Preventive Maintenance service activity in the customer's records/logbook.
- [x] Record the PM event in the Smart Alerts logbook, if applicable.
- [x] Update/reset instrument maintenance counters as appropriate.
- [x] Affix the PM sticker to the system or instrument logbook based on the customer's request.
- [x] Complete the Service Engineer Comments section if there are additional comments.
- [x] Review this service, parts replaced, and test results obtained with the customer.
- [x] If the instrument firmware was updated, record the details of the change in the Service Engineer's Comments box. Systems in a compliant environment may need additional documentation.
- [x] **Complete the Signature Page with both Service Engineer and Customer signatures.**

เอกสารไม่ควบคุม

Test Results

Instrument Performance Test Results Table

Note: These measurements do not form part of any specification and are for reference only.

	Pre PM Sensitivity Check		Post PM Sensitivity Check	
	Radial	Axial *	Radial	Axial*
Zn 213.857 nm SRBR	1782.8	2879.2	2230.8	3662.9
Mn 257.610 nm SRBR	95670.5	196149	10683.0	176884
Al 396.152 nm SBR	5.2	8.0	7.0	7.4
K 766.491 nm SBR	3.0	14.6	3.4	8.7

* Axial result is not applicable for G8016AA, G8012AA Radial View instruments.

Instrument Test Results Table

Note: The Instrument Test results are for systems using ICP Expert version 7.3 and above only.

Instrument Test	Result
Subsystem Communications Test	Pass
Air Flow	Pass
Water Flow	Pass
Gas Flows	Pass
RF Generator	Pass
Camera Test	Pass
Optics Test	Pass
Nebulizer test	Pass

เอกสารไม่ควบคุม

Consumed PM Parts

Part Description	Part Number	Product or Model# where used	Quantity consumed
Axial Pre-Optic Window	G8010-60014	G8010A, G8011A, G8014A/G8015A	1
Radial Pre-Optic Window	G8010-60015	All	1
Agilent Cool Clear Coolant Fluid	5799-0037	Agilent Water Recirculator	–
Purge Gas Filter	G8010-60136	All	1
Air Inlet filter	G8000-68002	All	1
High Capacity Air Filter	G8010-60189	Optional	–
Rotor seal for 6-7 port valve for AVS6/7	G8494-60002	G8494A/G8495	–
Rotor seal for 4 port valve for AVS4	G8493-60002	G8493A	–
Rinse solution to rinse station 2.5mm id x 1m	G8410-80123	SPS 4	–
Barb connector 2.5mm-1.5mm ID	G8410-80124	SPS 4	–
PVC waste tubing,8mm od x 5mm id, 2m	G8410-80122	SPS 4	–
Additional Parts may be required from engineer's stock:			
X axis drive belt	5410047500	SPS 3	–
Z axis drive belt	5410047400	SPS 3	–
Peristaltic pump tubing, PVC SolvaFlex, 3 bridged	3710049000	SPS 4	–

Consumed Parts Reference
(Purchased by customer, not included as part of PM)

☑ Section Not Applicable

Part Description	Part Number	Product or Model# where used	Quantity consumed

เอกสารไม่ควบคุม

ICP-OES Status Results Table

Note: These measurements do not form part of any specification and are for reference only.

Measurement	Standby Mode		Plasma On	
Mains Voltage	231.288	VAC	228.350	VAC
Mains Current	0.083	A	0.100	A
Instrument Temperature	21.1	°C	21.6	°C
RF Air Flow (sensor speed)	44.0	Hz	41.1	Hz
Plasma Exhaust Temperature	No measurement		47.1	°C
Water Flow Oscillator	No measurement		1.14	L/min
Water Flow Detector	0.92	L/min	0.90	L/min
Water Inlet Temperature	19.5	°C	18.5	°C
Polychromator Temperature	35.4	°C	36.4	°C
CCD Temperature	-40.1	°C	-39.9	°C
Thermal Stabilizer	35.0	°C	35.0	°C
Argon Supply Pressure	634.43	kPa	583.77	kPa
Purge Gas Supply Pressure*1	631.28	kPa	604.02	kPa
Option Gas Supply Pressure*1	–	kPa	–	kPa
Nebulizer Flow	No measurement		0.70	L/min
Nebulizer Back Pressure	No measurement		273.61	kPa
Plasma Gas Flow	No measurement		1195	L/min
Auxiliary Gas Flow	No measurement		1.00	L/min
RF Power	No measurement		1200.4	W
RF Supply Current	No measurement		8.228	A
RF Supply Voltage	No measurement		194.529	V

*1 If option installed

เอกสารไม่ควบคุม

Signature Page

Service Engineer Comments (optional)

If there are any specific points you wish to note as part of performing the installation or other items of interest for the customer, please write in this box.

Service Verification

Service Request Number:
6008006610

Service Engineer Name:
Worawit T.

Service Engineer Signature:
Worawit T.

Total number of pages in this document
14

Date Service Completed:
3 Nov 2025

Customer Name
Apharn O.

Customer Signature:
Apharn O.

เอกสารไม่ควบคุม

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000 FAX. 0-2719-9484

Certificate of Testing

Cert.No.: 25TW236
Page.: 1 of 2

Equipment :	DO Meter
Manufacturer :	Horiba
Model :	LAQUA-DO210
Serial No. :	HE9M0013
ID No. :	UAE.EFM.016/2563 (EFM.DO.05/63)
Received Date :	18 November 2025
Test Date :	20 November 2025
Reference :	2511-0529WSC-1
Submitted by :	United Analyst and Engineering Consultant Co.,Ltd. 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Laboratory Condition :	Temperature (25 ± 5) °C Humidity (50 ± 20) %
Test Procedure :	In - house method : CP-CH9 by Comparison Technique with Azide Modification Method
Tested by :	Walalak Sirithean
Approved by :	Saithip Approved Signatory

( ) Chakrit Waewwanjua
( ) Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 21 November 2025

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

Certificate of Calibration

Cert. No.: 25LM172
Page.: 1 of 2

Equipment :	DO Meter with Sensor
Manufacturer :	Horiba
Model :	LAQUA-DO210
Serial No. :	HE9M0013
ID No. :	UAE.EFM.016/2563(EFM.DO.05/63)
Submitted by :	United Analyst and Engineering Consultant Co.,Ltd. 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Location :	TPA On Site Calibration Laboratory
Received Order :	18 November 2025
Calibrated Date :	21 November 2025
Ambient Temperature :	(26 ± 10) °C
Relative Humidity :	(50 ± 30) %
AC Line Voltage :	(220 ± 22) V
Calibrated by :	Warakorn Lerngagtrakul
Approved by :	Kunchit Approved Signatory

( ) Chakrit Waewwanjua
( ) Suwit Imjai
(✓) Kunchit Promprat

Issue Date : 24 November 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Condition of this result of calibration

1. Reference Standard Instruments :
   This measurement result is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

Instruments	ID No.	Certificate No.	Due Date
1. Burette	130BU10	25CG1126	18 Mar 2027
2. Balance	110RC001	25MM316	02 July 2026

2. Standard Material :-

Material	Manufacturer	Lot.No.	Assay
Sodium Thiosulfate 5-Hydrate AR	KEMAUS	2203162447	99.6%

Result : **Dissolved Oxygen Meter Adjustment With Air 100 %**
Dissolved Oxygen Probe No.: 9K9M0021

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.22	8.20	0.0055

This report was certified only for the instrument we tested.It is allowable to use for study Intend to use for advertising and referral purpose is prohibited.This report may not be reproduced other in full, without written approval of the laboratory

-o0o-

Equipment : DO Meter with Sensor
Condition As-Received : Used Item
Reference : 2511-0529WSC-2

Procedure Used :-
Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.
The temperature scale used was based on ITS-90.

Condition of this result of calibration
1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Digital Thermometer	A7B843	25I17	TPA	06 Jan 2026

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This measurement result is traceable to the International System of Unit maintained through :
   Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment
Function : Temperature measurement.
This instrument was connected with temperature sensor, S/N.: 9K9M0021

Calibration Point (°C)	Immersion Depth (mm)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty (± °C)	Coverage Factor *k*
15.0	80	14.998	15.0	0.002	0.16	2.00
30.0	80	30.003	29.9	-0.103	0.16	2.00
45.0	80	45.000	44.8	-0.200	0.16	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor ***k***, providing a level of confidence of approximately 95 %.

-o0o-

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

Certificate of Calibration

Equipment : pH Meter
Manufacturer : Horiba
Model : LAQUA-PH210
Serial No. : HA9M0047
ID No. : UAE.EFM.005/2563 (EFM.pH.05/63)
Condition As-Received: Used Item
Received Date : 24 February 2026
Calibration Date : 26 February 2026
Reference : 2602-0796WSC-2
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260
Ambient Temperature : (25 ± 2.5) °C
Relative Humidity : (50 ± 15) %
Calibration Procedure : In - house method :
- CP-CH5 by direct measurement with DC voltage standard and direct measurement with certified reference material (CRM)
- CP-CH8 by comparison with temperature standard

Calibrated by : Walalak Sirithean

Approved by : _____
Approved Signatory

( ) Chakrit Waewwanjua
( ) Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 27 February 2026

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7)(7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (±)	Coverage factor k
pH Electrode	4.008	4.01	161.1	0.0079	2.00
S/N.: -	7.000	7.00	-10.4	0.0096	2.00
	7.000	7.00	-9.9	0.0095	2.00
	10.010	10.02	-177.9	0.0095	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;
- Model : -
- Serial No. : -

Dimension of probe
- Length : 103 mm.
- Diameter : 16 mm.
- Immersion Depth : 90 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (± °C)	Coverage factor k
15.0	15.001	15.0	-0.001	0.13	2.00
30.0	30.001	30.0	-0.001	0.13	2.00
45.0	45.001	44.9	-0.101	0.13	2.00

Remark - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Condition of this calibration result

1. Reference Standard Instrument

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1) Document Process Calibrator	54030049	130RC116	25E2743	25 Aug 2026
2) Ref. Standard Thermometer	4982054	110RC044	25I708	03 July 2026

- This measurement result is traceable to SI throught Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials :The measurement results are traceable to SI through Hach Lenge GmbH Ltd., Deutsche Akkreditierungsstelle, Accredited No.D-RM-15184-01-00
:The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.008	CPA chem	1187328	18 Jan 2028
pH 7.000	Hach Lenge GmbH	C03319	17 Oct 2027
pH 10.010	CPA chem	1187332	18 Jan 2027

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4,7)(7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement	Coverage factor
	pH	mV	mV	pH	(±mV)	k
pH Meter	4.00	177.48	177.3	4.01	0.058	2.00
S/N.: HA9M0047	7.00	0.00	0.0	7.02	0.058	2.00
	7.00	0.00	0.0	7.02	0.058	2.00
	10.00	-177.48	-177.2	10.01	0.058	2.00

PerkinElmer®
For the Better

PinAAcle 900F
Preventive Maintenance Report

Company Name: UAE Consultant Co., LTD.

Instrument Location: 41 Sukumvhit Rd.,

Phra Khanong, Bangkok 10260

Instrument Serial No.: PFBS20031902

Date: 27 Oct 2025

เอกสารไม่ควบคุม

PinAAcle 900F Preventive Maintenance (PM)

Company Name:	United Analyst and Engineering Consultant Co., LTD.		
Address (Instrument Location):	41 Sukumvhit Rd., Phra Khanong, Bangkok 10260		
Serial Number:	PFBS20031902	**PM Number:**	1 of 2
Customer Name (if applicable):	K. Yainda	**Telephone Number:**	095-5580049
Customer Support Engineer Name:	K. Chayanan	**Service Order Number:**	WO-06332081
Date PM Performed: (DD-MMM-YYYY)	27 Oct 2025	**Next PM Due Date:** (DD-MMM-YYYY)	27 Apr 2026
Standard Labor Hours to Complete PM :		**5 hours**	

Part Number	Release	Publication Date	
09370145 Rev.9	A	January 2018	PerkinElmer®

Scope
The purpose of this PM is to ensure the continued functionality of the PinAAcle 900F by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer.
The customer should save their method before the PM begins.

General Instructions
The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM.
Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files.
The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer.
Update the PM sticker and instrument logbook as required.

Copyright Information
This document contains proprietary information that is protected by copyright. All rights are reserved.
No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of PerkinElmer, Inc.
Copyright © 2013 PerkinElmer, Inc.

Trademarks
Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners.
Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no Warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.
PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

เอกสารไม่ควบคุม

Component List

Component / Specific Model	Serial #	Configuration Notes
PinAACle900F	PFBS20031902	Syngistix V.4.0.1.1935
FIAS100	100524040501	

Parts Lists

Parts Included with the PM		
Part Number (if applicable)	**Description**	**Quantity**
B0501696	Fan Filters	1
N3160156	O-Ring Kits for Sampling Introduction (Stainless Steels Nebulizer)	N/A
N3160157	O-Ring Kits for Sampling Introduction (Plastic Nebulizer)	1
N9301714	Replacement Acetylene Filter Cartridge	1
TH001022	Replacement Air Filter Cartridge	1

Additional Reagents and Standards Required for PM				
Part Number (if applicable)	**Description**	**Quality**	**Batch/Lot #**	**Expired Date** (MM/YY)
N9300183	1000 mg/L Copper Standard	AR	28-83CUY1	Nov 2026

Additional Reagents and Standards Required for PM (Customer Support Solution)				
Part Number (if applicable)	**Description**	**Quantity**	**Batch/Lot #**	**Expiration Date** (MM/YY)
N/A	DI Water	250 mL	AR	AR
N/A	0.5% HNO_3	250 mL	AR	AR

เอกสารไม่ควบคุม

Additional Tools Required for PM			
Part Number (if applicable)	**Description**	**Quantity**	**Serial #**
N1013000	0.2A Neutral density filter	1	101N0089015
N1013002	1.0A Neutral density filter	1	101N0089015
03030997	System 2 EDL Driver	1	03030997
N3050605	As System 2 EDL	1	16148
N3050121	Cu Lumina HCL	1	060419-030180
N3050109	Be Lumina HCL	1	061219-020041
N3050139	K Lumina HCL	1	030819-010130
N3050152	Ni Lumina HCL	1	052719-020020

เอกสารไม่ควบคุม

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. **General:**
   - ☑ Review the instrument performance with the customer and document any recent problems.
   - ☑ Inspect the customer log book and make any appropriate PM entries.
   - ☑ Perform general inspection of system for cleanliness.
2. **PC Instrument Software:**
   - ☑ Instrument Software user files/databases archived, packed, and/or deleted as needed.
3. **Mechanical:**
   - ☑ Inspect and clean all fans and filters. Replace filters if necessary
   - ☑ Inspect all gas lines for leaks and/or wear. Replace if needed.
   - ☑ Clean exterior of the instrument.
   - ☑ Inspect the burner head, burner chamber, and nebulizer. Clean if needed as stated in the Hardware Guide.
   - ☑ Check burner head dimensions with the feeler gauge as stated in the Hardware Guide in the Maintenance chapter section on cleaning the burner head and checking sloth width. Replace if out of specification
   - ☑ Check the condition of the end cap, burner head, and nebulizer O-rings. Replace if necessary.
   - ☑ Check the drain system for signs of wear. Replace worn or damaged parts.
   - ☑ Visually check for proper flame conditions when igniting the Air-C2H2 and N20-C2H2 flames (if applicable).
4. **Electrical:**
   - ☑ Inspect PC boards. Clean if necessary.
   - ☑ Carefully check all internal and external cable connections.
   - ☑ Check instrument firmware revisions upgrade to current levels (if necessary)
   - ☑ Run Diagnostics Test within the Advanced function of the Spectrometer page. Check the results in the service log folder in the Spectrometer BM Log Viewer.
5. **Optics:**
   - ☑ Inspect and clean the sample compartment windows, if needed.
   - ☑ Inspect optics. Clean or replace if necessary.
6. **Gasses:**
   - ☑ Verify that the Gasses supplied to the instrument are within the pressure and purity specifications found in the PinAAcle 900 Series Pre-Installation Checklist SDB.
   - ☑ Verify that the acetylene filter and air filter element is dry. Replace if necessary.

เอกสารไม่ควบคุม

7. Flame Interlock Check:

Description: Check to ensure that all safety interlocks are closed.

Parameter	Specification	Test Results	Pass/Fail
Flame Sensor	Air/C_2H_2 Flame correctly shuts down	Active	Passed
Drain Sensor	Air/C_2H_2 Flame correctly shuts down	Active	Passed
Nebulizer Sensor	Air/C_2H_2 Flame correctly shuts down	Active	Passed
C_2H_2 Pressure Sensor	Air/C_2H_2 Flame correctly shuts down	Active	Passed
Air Pressure Sensor	Air/C_2H_2 Flame correctly shuts down	Active	Passed
Burner Head Sensor	Choosing Nitrous Oxide as the oxidant should trigger an interlock shuts down	Active	Passed

8. After PM Performance tests:

8.1 Detector Linearity with Barium

Description: Ensures that the detector is linear in the Visible Range.

Parameter	Specification	Certificate Value at 553.6 nm (Abs.)	Test Results	Pass/Fail
1.0 A ND Filter	± 5% from Cert.	0.9995	0.9887	Passed
0.2 A ND Filter	± 5% from Cert.	0.1936	0.1896	Passed

8.2 Baseline Noise at 1.0 Absorbance with Barium

Description: Ensures that a high absorbance will not produce excessive noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.010	0.001	Passed

8.3 AA Baseline Noise with Copper

Description: Check baseline noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.001	0.0001	Passed

เอกสารไม่ควบคุม

8.4 D_2 Background Compensation with Copper

Description: Verifies the instruments ability to compensate for Background absorption.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.010	0.0001	Passed

8.5 AA-BG Baseline Noise with Copper

Description: Ensures that background correction does not produce excessive noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.005	0.0001	Passed

8.6 AA-BG Baseline Noise with Arsenic

Description: Ensures that background correction does not produce excessive noise at a low wavelength.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.005	0.0004	Passed

8.7 Flame Sensitivity

Description: Instrument Sensitivity checked against Copper standard.

Standard Copper Sensitivity	Specification	Results (Abs.)	Pass/Fail
5 mg/L Sensitivity SS Neb (if applicable)	> 0.250 Abs.	N/A	Not Applicable
2 mg/L Sensitivity HS Neb (if applicable)	> 0.250 Abs.	N/A	Not Applicable

10. Review:

- ☑ Review with the customer PM work performed.
- ☑ Review with the customer routine maintenance procedures.
- ☑ Discuss recommended customer supplied materials to have on hand.
- ☑ Attach PM sticker.

เอกสารไม่ควบคุม

Additional Comments

Additional Comments Regarding the PM

Review

The preventive maintenance checks and if applicable performance tests for PinAAcle 900F have been completed.

This PinAAcle 900F Passes ☑ Fails ☐ the preventive maintenance.

Review of Preventive Maintenance:

Authorized PerkinElmer Representative: Chayanan K.	Date: 27 Oct 2025 (DD-MMM-YYYY)
Authorized Customer Representative: [signature]	Date: 27 Oct 2025 (DD-MMM-YYYY)

เอกสารไม่ควบคุม

Atomic Absorption/FIAS 100/400 Preventive Maintenance (PM)

Company Name:	United Analyst and Engineering Consultant Co., LTD.		
Address (Instrument Location):	41 Sukumvhit Rd., Phra Khanong, Bangkok 10260		
Room Number:	Lab		
Asset Number (if applicable):	1 of 2	**Customer System ID:**	K. Yanida
Service Engineer Name:	K. Chayanan	**Service Order Number:**	WO-06332087
Date PM Performed: (DD-MMM-YYYY)	27-Oct-2025	**Next PM Due Date:** (DD-MMM-YYYY)	27-Apr-2026

Part Number	Release	Publication Date	
09370005	C	January 2013	PerkinElmer®

Scope
The purpose of this PM is to ensure the continued functionality of the Atomic Absorption/FIAS 100/400 by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer.
The customer should save their method before the PM begins.

General Instructions:
Always check with the customer before making any changes that may affect the customer's analysis or calibration.
The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer.
Update the PM sticker and instrument logbook as required.

Copyright Information
This document contains proprietary information that is protected by copyright. All rights are reserved.
No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of PerkinElmer, Inc. **Copyright © 2013 PerkinElmer, Inc.**

Trademarks
Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners.
Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.
PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

เอกสารไม่ควบคุม

Component List

Component / Specific Model	Serial #	Firmware Version	Configuration Notes
FIAS100	100S24040501	2.20	Syngistix V4.0.1.1935

Parts Lists

Parts Included with the PM				
Part Number (if applicable)	Description	Quantity	Batch/Lot #	Expiration Date (MM/YY)
B050 2706	Fan Filter	1	N/A	N/A

Additional Tools Required for PM				
Part Number (if applicable)	Description	Quantity	Serial #	Calibration Due Date (MM/YY)
N/A	Digital Volt Meter	1	N/A	N/A
Additional Reagents and Standards Required for PM				
Part Number (if applicable)	Description	Quantity	Batch/Lot #	Expiration Date (MM/YY)
N/A	N/A	N/A	N/A	N/A

เอกสารไม่ควบคุม

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. **General:**
   - ☑ Review the instrument performance with the customer and document any recent problems.

     _____

   - ☑ Is the Working Environment Acceptable? If not, document.

     _____

   - ☐ Visual Damage (if yes, describe)

     _____

   - ☑ Check incoming AC line voltage for proper levels and grounding.
   - ☑ Verify Voltage switch on back of instrument is correct
   - ☑ Perform general inspection of system for cleanliness. Clean if needed.
   - ☑ Gas supply cylinders secured, lines leak checked and argon or nitrogen supply pressure verified (45 – 58 psi).
   - ☑ Inspect the customer log book and make any appropriate PM entries.
   - ☑ Fan checked and filter cleaned
   - ☑ Heating mantle or Universal Cell Holder checked

2. **Instrument components**
   - ☑ Non-return valve checked/repaired/replaced if needed (B019 8111). Clean the valve if there is any liquid in it. Replace the rubber sleeve (B013 5123) if it is worn. Check the flow meter for any signs of fluid in it. Clean the flow meter if needed.
   - ☑ Verify condition of pump pressure adjustment levers (B050 7794 - look for cracks or problems with the springs), pump rollers (B300 0251 check for wear), and thumb screws (B050 7796).
   - ☑ Check the Multiport valve for proper switching, flow, and insure there are no leaks. Clean valve parts and replace o-rings if needed (large o-ring: B050 1250, small o-ring: B004 5095). Use a squirt bottle & fishing line to try to dislodge clogs.
   - ☑ Firmware Version checked. Latest is 2.20.

3. **Mixing/Separation Assembly & Pump Tubing:**
   - ☑ Mixing separator assembly checked
   - ☑ Filter/membrane checked (B050 8306)
   - ☑ Condition of the pump tubing (replace if necessary), correct pump tubing for the solutions being run. Make sure the correct magazines are being used. B050 7791 for 0.13 – 1.80 mm tubing; B050 7792 for 1.60 – 3.18 mm tubing.

เอกสารไม่ควบคุม

4. **Cell, Cell Windows, Transfer Line:**
   - ☑ Cell checked
   - ☑ Cell windows checked
   - ☑ Transfer line checked for moisture (if moisture is a problem, the Nafion dryer might be needed)

5. **Operational Tests:**
   - ☑ Run DI water through the carrier/reductant/sample system. Verify smooth flow of liquid throughout without leaks. Replace tubing & fittings if needed.

6. **Review:**
   - ☑ Review with the customer PM work performed.
   - ☑ Review with the customer routine maintenance procedures.
   - ☑ Discuss recommended customer-supplied materials to have on hand.
   - ☑ Attach PM sticker.
   - ☑ Update Logbook.

เอกสารไม่ควบคุม

Additional Comments

Additional Comments Regarding the PM

Review

The preventive maintenance checks and if applicable performance tests for FIAS 100/400 have been completed.

This FIAS 100/400 Passes ☑ ***Fails*** ☐ ***the preventive maintenance.***

Review of Preventive Maintenance:	
Authorized PerkinElmer Representative: Chayanan K.	Date: 27 Oct 2025 (DD-MMM-YYYY)
Authorized Customer Representative: [illegible]	Date: 27 Oct 2025 (DD-MMM-YYYY)

เอกสารไม่ควบคุม

Document History

Revision	Description of Change	Page(s)	Date
A	First release		May 2008
B	Addition of Batch/Lot Number, Expiration Date, and Report Fields.	2,7	February 2009
C	Update to new format	All	January 2013

เอกสารไม่ควบคุม

PerkinElmer
For the Better

PerkinElmer Scientific (Thailand) Co., Ltd.
250 Soi Soonvija 4
Khwang Sangyapi, Khet Huay Kwang
Bangkok 10310
Thailand
Tel: 66 2719 6420 ; Fax: +66 2 319 7900
http://www.perkinelmer.com

Service Report

Work Order Number	Activity Code	Billing Type	Requested Start Date	Model	Serial Number
WO-0633286	Planned Maintenance	Contract	28/04/2568 10:27 น.	AAnalyst 400	FFBS2003190Z
Service Representative Name	**Contract Number**		**Expiry Date**	**Equipment ID**	**System ID**
Kanan, Chayanan	SC-003906189		31/10/2025	N/A	N/A
UDI Number					
N/A					
Equipment Location			**Bill To Name**		
บริษัท ปูโรเด็ค แอนะลิติค (ประเทศไทย) จำกัด (มหาชน) เขตพระโขนง กรุงเทพมหานคร 51 10260 TH			บริษัท ปูโรเด็ค แอนะลิติค (ประเทศไทย) จำกัด (มหาชน) เขตพระโขนง กรุงเทพมหานคร 51 10260 TH		
Customer Contact	**Phone Number**	**Fax Number**	**Email**		**Purchase Order**
คุณวันเพ็ญ เหมมิตร์(วันเพ็ญ)	085-5580649	N/A	yanindachamlek@gmail.com		PO-256100002

Work Description

- PM 1/2 (AAnalyst)
- Cleaning Cell, Chamber, Filter
- Wavelength Calibrate ; Pass
- Wavelength Scan As,Cu,Be,K,Ni ; Pass
-Align cell with Hg. ; OK

Start Date	End Date	Work Description
27/10/2025	27/10/2025	
27/10/2025	27/10/2025	

Tools Used

Quantity	Calibrated Tool	Description	Serial Number	Last Calibration Date	Next Calibration Date
*** No Calibrated Tools Used ***					

Material Used

Part Number	Part Description	Note	Lot/Serial Number	Quantity
N9301714	Balston G2+2 Filter Cartridge			1

Labour Details

Part Number	Part Description	Start Date	Quantity
SV000013	Preventative maintenance	27/10/2025	4
SV000002	Service Travel	27/10/2025	2

Work Complete	Customer Signature	Technician Signature
Yes ☑ No ☐	คุณวันเพ็ญ	Chayanan k.
PM/OQ/PV Left with Customer: Yes ☐ No ☑	2/11/2568 คุณวันเพ็ญ เหมมิตร์(วันเพ็ญ)	2/11/2568 Kanan, Chayanan

เอกสารไม่ควบคุม

Perkin

PerkinElmer TruQ

PerkinElmer Number: N9300163
Element and Matrix: 1000 µg/mL Copper in 2% HNO3
Starting Material: Copper Metal
Starting Material Lot No: 10221A
Density: 1.011 g/mL @ 20°C

Lot No: 28-83CUY1
Certification Date: MAY - - 2025
Expiration Date: NOV 30 2026

Trace Metallic Impurities in the Actual Solution via ICP / ICP-MS Analysis:

Element	µg/mL	Element	µg/mL	Element	µg/mL	Element	µg/mL	Element	µg/mL
Ag	0.005	Dy	<0.001	Li	<0.001	Pt	<0.001	Tb	<0.001
Al	<0.002	Er	<0.001	Lu	<0.001	Rb	<0.001	Te	<0.001
As	<0.001	Eu	<0.001	Mg	<0.001	Re	<0.001	Th	<0.001
Au	<0.001	Fe	0.02	Mn	<0.001	Rh	0.002	Ti	<0.001
B	<0.001	Ga	<0.001	Mo	<0.001	Ru	<0.001	Tl	<0.001
Ba	<0.001	Gd	<0.001	Na	0.004	Sb	<0.001	Tm	<0.001
Be	<0.001	Ge	<0.001	Nb	<0.001	Sc	<0.001	U	<0.001
Bi	<0.001	Hf	<0.001	Nd	<0.001	Se	<0.002	V	<0.001
Ca	<0.01	Hg	<0.001	Ni	<0.001	Si	<0.1	W	<0.001
Cd	<0.001	Ho	<0.001	P	<0.2	Sm	<0.001	Y	<0.001
Ce	<0.001	In	<0.001	Pb	0.005	Sn	0.003	Yb	<0.001
Co	<0.001	Ir	<0.001	Pd	<0.001	Sr	<0.001	Zn	0.02
Cr	<0.001	K	<0.1	Pr	<0.001	Ta	<0.001	Zr	<0.001
Cs	<0.001	La	<0.001						

Traceability Documentation for Solution Standard:

Certified Value: 999 µg/mL ±5 µg/mL (refer to side 2)
Certified Value is Traceable to: NIST SRM #3114
*** Classical Wet Assay:** 997 µg/mL
Method: EDTA titration using PAN as indicator. EDTA standardized against $Pb(NO_3)_2$ NIST SRM #928.

***Instrument Analysis using ICP Spectrometer:** 1001 µg/mL
via NIST SRM #3114

We guarantee that our PerkinElmer TruQ Atomic Spectroscopy Standards are stable and accurate to ±0.5% of certified concentration until the expiration date, provided the standards are kept tightly capped and stored under normal laboratory conditions. This value is the sum of cumulative errors associated with the analytical determinations, pipetting, and diluting to final volume. For these solutions we use high purity acids, ASTM Type 1 water (18 megohm double deionized), and leached, triple-rinsed bottles. All glassware used is class A.

Certifying Officer: Y. Parikh
Yogesh Parikh, Senior Spectroscopist

เอกสารไม่ควบคุม

Terms & Conditions

Customer Acknowledgment of receipt of the above repair / replacement.

Special Terms and Conditions: This is not an invoice.

Taxes will be applied to your invoice if applicable.

เอกสารไม่ควบคุม

PerkinElmer
For the Better

PerkinElmer Scientific (Thailand) Co., Ltd.
290 Soi Soonvijai 4
Khwang Bangkapi, Khet Huay Kwang
Bangkok 10310
Thailand
Tel: 66 2719 6420 ; Fax: +66 2 319 7900
http://www.perkinelmer.com

Service Report

100S24040501

Work Order Number	Activity Code	Billing Type	Requested Start Date	Model	Serial Number
WO-06332087	Planned Maintenance	Contract	28/04/2568 10:29 น.	FIA8100	100S20040005

Service Representative Name	Contract Number	Expiry Date	Equipment ID	System ID
Kanan, Chayanan	SC-0035864109	31/10/2025	N/A	N/A

UDI Number
N/A

Equipment Location	Bill To Name
บริษัท ยูไนเต็ด แอนะแลิสต์ แอนด์ เซอร์วิเจอรส เซอเซอร์วิสซ กรุงเทพมหานคร 51 10260 TH	บริษัท ยูไนเต็ด แอนะแลิสต์ แอนด์ เซอร์วิเจอรส เซอเซอร์วิสซ กรุงเทพมหานคร 51 10260 TH

Customer Contact	Phone Number	Fax Number	Email	Purchase Order
ญาณินัดดา เหลมสิทธิ์(ไบหลวง)	095-5580049	N/A	yanindachamlek@gmail.com	HPO-250100002

Work Description

- PM 1of 2 (S/N_100S24040501)
- Cleaning Port Vale, Manifold, Tuning
- Run Hg test ; Pass

Start Date	End Date	Work Description
27/10/2025	27/10/2025	
27/10/2025	27/10/2025	

Tools Used

Quantity	Calibrated Tool	Description	Serial Number	Last Calibration Date	Next Calibration Date
*** No Calibrated Tools Used ***					

Material Used

Part Number	Part Description	Note	Lot/Serial Number	Quantity
80194049	Sample Loop, 500UL			1
80501250	O-Ring 18.77 x 1.78			1
80500748	O-RING 16 X 1,78 VITON			2

Labour Details

Part Number	Part Description	Start Date	Quantity
SV000013	Preventative maintenance	27/10/2025	3
SV000002	Service Travel	27/10/2025	2

Work Complete	Customer Signature	Technician Signature
Yes ☑ No ☐	ญาณินัดดา	Chayanan K.
PM/OQ/PV Left with Customer		
Yes ☐ No ☑	3/11/2568 ญาณินัดดา เหลมสิทธิ์(ไบหลวง)	3/11/2568 Kanan, Chayanan

เอกสารไม่ควบคุม

Terms & Conditions

Customer Acknowledgment of receipt of the above repair / replacement.

Special Terms and Conditions: This is not an invoice.

Taxes will be applied to your invoice if applicable.

เอกสารไม่ควบคุม

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

ilac-MRA

NSC-TISI-TIS17025
CALIBRATION 0008

Certificate of Calibration

Equipment :	pH Meter
Manufacturer :	Horiba
Model :	LAQUA-PH210
Serial No. :	HA0A0005
ID No. :	UAE.EFM.004/2563(EFM.pH.04/63)
Condition As-Received:	Used Item
Received Date :	09 December 2025
Calibration Date :	11 December 2025
Reference :	2512-0243WSC-2
Submitted by :	United Analyst and Engineering Consultant Co.,Ltd. 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure :	In - house method : - CP-CH5 by direct measurement with DC voltage standard and direct measurement with certified reference material (CRM) - CP-CH8 by comparison with temperature standard
Calibrated by :	Warakorn Lerngagtrakul
Approved by :	Approved Signatory
	(✓) Chakrit Waewwanjua ( ) Ponpan Paipim ( ) Saithip Meangmai
Issue Date :	12 December 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

Condition of this calibration result

1. Reference Standard Instrument

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1) Document Process Calibrator	54030049	130RC116	25E2743	25 Aug 2026
2) Ref. Standard Thermometer	4962054	110RC044	25I708	03 July 2026

- This measurement result is traceable to SI throught Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials :The measurement results are traceable to SI through Hach Lenge GmbH Ltd., Deutsche Akkreditierungsstelle, Accredited No.D-RM-15184-01-00
:The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.007	CPA chem	1114384	12 June 2027
pH 6.999	Hach Lenge GmbH	C03273	13 May 2027
pH 10.010	CPA chem	1114385	08 June 2026

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4,7)(7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement	Coverage factor
	pH	mV	mV	pH	(±mV)	k
pH Meter	4.00	177.48	177.4	4.01	0.058	2.00
S/N.: HA0A0005	7.00	0.00	0.1	7.00	0.058	2.00
	7.00	0.00	0.1	7.00	0.058	2.00
	10.00	-177.48	-177.2	10.01	0.058	2.00

เอกสารไม่ควบคุม

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7)(7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (±)	Coverage factor k
pH Electrode	4.007	4.01	175.4	0.0085	2.05
S/N.: -	6.999	7.00	-0.3	0.0095	2.00
	6.999	7.01	-0.5	0.0096	2.00
	10.010	10.01	-170.6	0.0092	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : -
- Serial No. : -

Dimension of probe

- Length : 112 mm.
- Diameter : 16 mm.
- Immersion Depth : 100 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (±°C)	Coverage factor k
15.0	15.002	15.0	-0.002	0.13	2.00
30.0	30.002	30.0	-0.002	0.13	2.00
45.0	45.003	45.0	-0.003	0.13	2.00

Remark - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP25-021

Environment Condition : Ambient Temperature 25 ± 5 °C

Relative humidity 55 ± 20 %RH

Calibration method : In-house method CP-01 Based on ASTM E275-08

Certified Reference Materials :

Material	Serial No.	Certificate No.	Due date
Absobance Standard set	25760	115663	25 October 2025
Absobance Standard set	25757	115638	25 October 2025
Wavelength Standard set	25806	115657	25 October 2025
Wavelength Standard set	25758	115665	25 October 2025

Traceability : This certification is traceable to the International System of Unit maintained at National - Institute of Standards and Technology (NIST) through Starna Scientific Limited

Spectral Band Width of UUC : 1.5 nm.

Scan Speed of UUC : 200 nm/min

Scan Interval of UUC : 0.1 nm.

Resolution of UUC : Photometric 0.001 Abs.

Wavelength 0.1 nm.

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

CERTIFICATE OF CALIBRATION

Certificate No. : SP25-021

Customer : United Analyst and Engineering Consultant Co.,Ltd. (Head Office)

Address : 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Location of calibration : Instrument room (207)

Equipment : UV-Vis Spectrophotometer

Manufacturer : HITACHI

Model : U-2900

Serial No. : 21E22-009

ID No. : UAE.WAT.051/2564

Received Date : 26 May 2025

Calibration Date : 26 May 2025

Issue Date : 29 May 2025

Condition Instrument : Good

Calibrated by : (Mr.Tanawut Rittidach) Technical Manager

Approved by : (Ms.Chonticha Sangngern) Quality Manager

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the DQE Services Co., Ltd.

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP25-021

Calibration Results : Without adjustment

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
420	0.0000	0.000	0.0000	0.0028	2.00
	0.5780	0.574	0.0040	0.0031	2.00
	1.0484	1.043	0.0054	0.0029	2.00
	2.1876	2.185	0.0026	0.0075	2.00
440	0.0000	0.000	0.0000	0.0028	2.00
	0.5595	0.558	0.0015	0.0034	2.00
	1.0239	1.022	0.0019	0.0035	2.00
	2.1230	2.121	0.0020	0.0079	2.00
465	0.0000	0.000	0.0000	0.0028	2.00
	0.5230	0.519	0.0040	0.0030	2.00
	0.9633	0.960	0.0033	0.0029	2.00
	1.9753	1.973	0.0023	0.0070	2.00
546.1	0.0000	0.000	0.0000	0.0028	2.00
	0.5181	0.516	0.0021	0.0031	2.00
	1.0002	0.998	0.0022	0.0033	2.00
	1.9973	1.995	0.0023	0.0084	2.00
590	0.0000	0.000	0.0000	0.0028	2.00
	0.5517	0.550	0.0017	0.0030	2.00
	1.0803	1.080	0.0003	0.0030	2.00
	2.0373	2.036	0.0013	0.0079	2.00
635	0.0000	0.000	0.0000	0.0028	2.00
	0.5591	0.558	0.0011	0.0031	2.00
	1.0518	1.051	0.0008	0.0030	2.00
	1.9274	1.926	0.0014	0.0080	2.00

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP25-021 Page 4 of 5

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
235	0.0000	0.000	0.0000	0.0050	2.00
	0.7469	0.748	-0.0011	0.0057	2.00
257	0.0000	0.000	0.0000	0.0050	2.00
	0.8674	0.866	0.0014	0.0059	2.00
313	0.0000	0.000	0.0000	0.0050	2.00
	0.2919	0.291	0.0009	0.0051	2.00
350	0.0000	0.000	0.0000	0.0050	2.00
	0.6430	0.640	0.0030	0.0055	2.00

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP25-021 Page 5 of 5

Wavelength Accuracy :

CRMs Values (nm.)	UUC Reading (nm.)	Correction (nm.)	Uncertainty (nm.)	Coverage factor k
241.72	241.0	0.72	0.18	2.00
279.45	278.8	0.65	0.18	2.00
287.81	287.2	0.61	0.18	2.00
334.06	333.6	0.46	0.18	2.00
360.93	360.6	0.33	0.18	2.00
418.59	418.2	0.39	0.18	2.00
445.94	445.6	0.34	0.18	2.00
460.02	459.8	0.22	0.18	2.00
536.59	536.6	-0.01	0.18	2.00
637.98	638.0	-0.02	0.18	2.00
431.38	431.2	0.18	0.18	2.00
472.50	472.4	0.10	0.18	2.00
513.47	513.4	0.07	0.18	2.00
528.88	528.8	0.08	0.18	2.00
573.17	573.2	-0.03	0.18	2.00
585.35	585.0	0.35	0.20	2.00
684.40	684.4	0.00	0.18	2.00
740.72	741.0	-0.28	0.20	2.00
748.55	748.8	-0.25	0.18	2.00
807.03	807.2	-0.17	0.18	2.00
879.28	879.6	-0.32	0.18	2.00

Remark : - UUC = Unit Under Calibration
- N/A = Not Avaiable
- The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%

- End of Certificate -

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000 FAX. 0-2719-9484

Certificate of Testing

Cert.No.: 26TW14
Page.: 1 of 2

Equipment :	DO Meter
Manufacturer :	Horiba
Model :	LAQUA-DO210
Serial No. :	HE9M0003
ID No. :	UAE.EFM.015/2563 (EFM.DO.04/63)
Received Date :	15 January 2026
Test Date :	16 January 2026
Reference :	2601-0460WSC-3
Submitted by :	United Analyst and Engineering Consultant Co.,Ltd. 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Laboratory Condition :	Temperature (25 ± 5) °C Humidity (50 ± 20) %
Test Procedure :	In - house method : CP-CH9 by Comparison Technique with Azide Modification Method
Tested by :	Walalak Sirithean
Approved by :	Saithip Approved Signatory

( ) Chakrit Waewwanjua
( ) Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 19 January 2026

Cert.No.: 26TW14
Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :
This measurement result is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

Instruments	ID No.	Certificate No.	Due Date
1. Burette	130BU10	25CG1126	18 Mar 2027
2. Balance	110RC001	25MM316	02 July 2026

2. Standard Material :-

Material	Manufacturer	Lot.No.	Assay
Sodium Thiosulfate 5-Hydrate AR	KEMAUS	2203162447	99.6%

Result : **Dissolved Oxygen Meter Adjustment With Air 100 %**
Dissolved Oxygen Probe No.: 9K2B0020

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.20	8.20	0.0045

This report was certified only for the instrument we tested.It is allowable to use for study Intend to use for advertising and referral purpose is prohibited.This report may not be reproduced other in full, without written approval of the laboratory

-o0o-

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

Certificate of Calibration

Cert. No.: 26LM10
Page.: 1 of 2

Equipment : DO Meter with Sensor

Manufacturer : Horiba

Model : LAQUA-DO210

Serial No. : HE9M0003

ID No. : UAE.EFM.015/2563 (EFM.DO.04/63)

Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong, Bangkok 10260

Location : TPA On Site Calibration Laboratory

Received Order : 15 January 2026
Calibrated Date : 19 January 2026
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %
AC Line Voltage : (220 ± 22) V

Calibrated by : Warakorn Lerngagtrakul

Approved by : Kunchit
Approved Signatory

( ) Chakrit Waewwanjua
( ) Suwit Imjai
(✓) Kunchit Promprat

Issue Date : 22 January 2026

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Equipment : DO Meter with Sensor
Condition As-Received : Used Item
Reference : 2601-0460WSC-4

Cert. No.: 26LM10
Page.: 2 of 2

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Digital Thermometer	2188080	25I953	TPA	05 Sep 2026

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This measurement result is traceable to the International System of Unit maintained through :

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N.: 9K2B0020

Calibration Point (°C)	Immersion Depth (mm)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty (± °C)	Coverage Factor *k*
15.0	80	15.003	15.0	-0.003	0.16	2.00
30.0	80	30.005	29.9	-0.105	0.16	2.00
45.0	80	45.001	44.9	-0.101	0.16	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor ***k***, providing a level of confidence of approximately 95 %.

-o0o-

Agilent

Agilent AA Series Spectrometers

Preventative Maintenance Checklist

[redacted]

Foreword

Agilent Preventive Maintenance provides factory recommended service for your analytical systems to assure reliable operation and the accuracy of your results.

Delivered by highly trained and certified service engineers using genuine Agilent parts and supplies, Agilent Preventive Maintenance provides everything you need to reduce unplanned downtime and keep your systems operating at their peak. This checklist will be completed at the end of the service and provided to you as a record of the installation.

NOTE While non-current production AA instrument and or accessory models are not covered specifically in this document it can be used as a basic reference.

For more information about Agilent Technologies services please visit our web site using the following URL http://www.agilent.com/en-us/services

เอกสารไม่ควบคุม

Contents

Customer information	3
Service Engineer's Responsibilities	3
Other important Customer Web links	3
System information	4
Preparation, Safe operation and Initial performance checks	4
Preventative maintenance procedures	5
Flame systems	5
Furnace systems	6
Accessories	8
Restore System	9
Guidance	9
Signature Page	9
Service Review	9
Test Results	10
AA consumable and parts list	10
Service Engineer Comments (optional)	11
Service Completion	12

Revision: 12.0, Issued: November 2025
Document Number: D01401 17
© Agilent Technologies, Inc. 2025

Agilent
เอกสารไม่ควบคุม

Customer information

- Customers should provide all necessary operating supplies upon request of the engineer.
- A customer representative should be available to the engineer while performing the preventive maintenance procedures.
- Any parts, not included in the Parts Lists section of this document, are not part of the recommended Preventive Maintenance service, nor are they included in the price of this service.
- If a system requires the use of extra or special procedures and/or parts for the maintenance service, then these must be ordered separately and charged as a repair, which may incur additional costs.

Service Engineer's Responsibilities

- Contact the customer and ensure that all necessary supplies are available before the preventive maintenance visit.
- Confirm the ability of the instrument to deliver continued safe operation as established via the Agilent AA safe operation flow chart. **(Refer directly to the AA 55/240/280 Preventive Maintenance Scope of Work to make this decision.)**
- Only select those pages that relate to the system or module being serviced.
- Complete empty fields with the relevant information.
- Complete the relevant checkboxes in the checklist using either a "X" or tick mark "√".
- Check "Section not applicable" check boxes to indicate services/tasks not delivered, as appropriate.
- Complete the Preventive Maintenance service in the order of the tasks listed.
- Complete the Service Review section together with the customer.
- Complete the fields for page numbers at the foot of each selected page.
- Complete the total number of pages field in the Service Completion section.
- Ask the customer to sign the Service Completion section including the customer's and your signature.

This information is subject to change without notice.

Other important Customer Web links

- How to get information on your product: Literature Library – http://www.agilent.com/chem/library
- Need to know more? www.agilent.com/chem/education
- Need technical support, FAQs? www.agilent.com/chem/techsupp
- Need supplies? www.agilent.com/chem/supplies

Revision: 12.0, Issued: November 2025
Document Number: D0140117
© Agilent Technologies, Inc. 2025

Agilent

เอกสารไม่ควบคุม

- ☑ Check for required firmware updates and verify with customers if they would like them installed.
- ☑ Use SVD to perform a Full Wavelength Scan for Cu HCL - "As found test_1"
- ☑ Perform a Basic Cu ABS test - "As found test_2"
- ☑ Print the Details page or screen captures of the test results and attach to the end of this checklist.

Preventative maintenance procedures

Flame systems

- ☐ Section NOT applicable.

Electronic components

- ☑ Review and confirm instrument configuration data in SVD.
- ☑ Confirm power supply voltages using the **SVD Power Supply diagnostic**.
- ☑ For Dual Beam instruments - Confirm RBC frequency using the **SVD RBC frequency diagnostic**.

Mechanical components

- ☑ Check the burner adjuster controls for complete and free movement. If the burner adjuster needs lubrication, use Molykote 321 or mineral-based molybdenum disulphide grease.
- ☑ Run SVD tests to exercise all motor drives over the full range of their travel.
  - ☑ Monochromator drive
  - ☑ Slit drive
  - ☑ Lamp selector
  - ☐ Automatic Burner Adjuster

Optics components

- ☑ Check that external optical surfaces are clean – Clean or replace as required.
- ☑ Use SVD and perform **Mono Wavelength Correction**.
- ☑ Use SVD and perform **Slit Calibration**.
- ☑ Use SVD and perform **Grating Squareness Diagnostic**.
- ☑ Use SVD and perform **Zero Order Offset/Mono Correction**.
- ☑ Use SVD and perform **Wavelength Repeatability**.
- ☑ Physically inspect selected HC lamps (customer to supply per their choice) and measure the % Gain for each lamp. Advise customer if lamps are showing emission degradation due to age.
- ☑ Check that the signal energy of the D2 and HC lamps track properly. Advise customer if their D2 lamp is showing emission degradation due to age.

Revision: 12.0, Issued: November 2025
Document Number: D0140117
© Agilent Technologies, Inc. 2025

Agilent

เอกสารไม่ควบคุม

System information

☐ Check this box if an instrument configuration report is attached instead of completing this table.

Instrument system name and ID	240 FS AAS
Instrument system site and location	United Analyst and Engineering Consultant
List system component product numbers	**List the serial numbers of each component**
1 G8432A	1 MY13160001
2	2
3	3
4	4
5	5
6	6
7	7
8	8
9	9
10	10

Preparation, Safe operation and Initial performance checks

☐ Agilent AA safe operation flow chart inspections (to determine if the PM can be performed).

NOTE If by following the flow chart the instrument is deemed to be unsafe for continued use you MUST NOT continue PM work. Inform the customer immediately of the Agilent recommendation that use of the instrument be discontinued.

- ☑ Discuss any specific questions or issues with the customer prior to starting.
- ☐ For HF application systems, if standard sample introduction system was not installed, ask the customer to install it. N/A
- ☑ Review the instrument logbook for recorded problems and comments.
- ☑ Save instrument control settings before starting the procedure.
- ☑ Perform a general inspection of the system for cleanliness.
- ☑ Check for proper installation of parts, assemblies, sensors etc.
- ☑ Check system for required installation of components, settings as defined by current Service Notes.

Revision: 12.0, Issued: November 2025
Document Number: D0140117
© Agilent Technologies, Inc. 2025

Agilent

เอกสารไม่ควบคุม

Sample introduction and Atomization

- ☑ Inspect the burner interlock plate to ensure that the interlock pin is secure and correct for the burner type.
- ☑ Clean the burner slot with a clean white card.
- ☑ Check the uniformity of the slot width.
- ☑ Clean the burner if required.
- ☑ Change the burner o-ring and lubricate with PFPE grease.
- ☑ Clean the nebulizer, spray chamber and liquid trap.
- ☑ Change all o-rings and seals in the nebulizer, nebulizer block and spray chamber and lubricate.
- ☑ Check that the pressure relief bung releases readily.
- ☑ Change o-rings on the fuel and oxidant delivery barbs and lubricate.
- ☑ Leave the liquid trap EMPTY and verify the flame will not ignite in this state.
- ☑ Refill liquid trap and check that overfill drains freely into the drain/waste tube.
- ☑ Check the drain/waste tube for good drainage. It should not have tight bends, kinks or loops and the lower end must be above the liquid level in the waste vessel.
- ☑ Check and clean the igniter electrode.

Gas handling components and safety interlocks

- ☑ Pressure test for leaks.
- ☑ Leak test gasbox internal components using gasbox leak tester G8434-67013.
- ☑ Check safety interlock status and operation using the **SVD interlock monitoring diagnostic**.

Analytical performance for Flame systems

- ☑ Ignite a flame.
- ☑ Check that you can adjust the nebulizer uptake rate from 4 to 6.5 mL per minute.
- ☑ Optimize the instrument ready to perform Cu sensitivity test.
- ☑ Create a manual method to perform a Basic Cu ABS test - "Final Performance Testing."
- ☑ Run a PM completed sensitivity test for a 5 ppm copper sample and record the results in the AA PM Performance test results and measurements table.

Furnace systems

- ☑ Section NOT applicable.

Electronic components

- ☐ Review and confirm instrument configuration data in SVD.
- ☐ Confirm power supply voltages using the **SVD Power Supply diagnostic**.

Mechanical components

- ☐ Run SVD tests to exercise all motor drives over the full range of their travel.
  - ☐ Monochromator drive
  - ☐ Slit drive

Revision: 12.0, Issued: November 2025
Document Number: D0140117
© Agilent Technologies, Inc. 2025

Agilent

เอกสารไม่ควบคุม

- ☐ Lamp selector

Optics components

- ☐ Check that external optical surfaces are clean – Clean or replace as required.
- ☐ Use SVD and perform **Mono Wavelength Correction**.
- ☐ Use SVD and perform **Slit Calibration**.
- ☐ Use SVD and perform **Grating Squareness Diagnostic**.
- ☐ Use SVD and perform **Zero Order Offset/Mono Correction**.
- ☐ Use SVD and perform **Wavelength Repeatability**.
- ☐ Physically inspect selected HC lamps (customer to supply per their choice) and measure the % Gain for each lamp. Advise customer if lamps are showing emission degradation due to age.

Gas handling, water system, and workhead component checks

- ☐ Inspect the GTA workhead gas hoses and connections for leaks.
- ☐ Pressure test for gas leaks
- ☐ If the cooler system is accessible (stand-alone) check for correct operation and coolant/water level – this includes any temperature and pressure settings plus filter cleaning (air flow and water).
- ☐ Inspect the GTA workhead water hoses and connections for leaks.
- ☐ Check all graphite components and replace if necessary.
  - ☐ Tube
  - ☐ Electrodes
  - ☐ Shroud
- ☐ Check and clean the end windows on the workhead.
- ☐ Check safety interlock operation.

Analytical performance for Furnace systems

- ☐ Optimize the instrument ready to perform Cu sensitivity test.
- ☐ Run the sensitivity test for a 25 ppb copper sample and record the results in the results table.

PSD autosampler accessory for Furnace systems

- ☑ Section NOT applicable.
- ☐ Check condition of the PSD capillary – replace if necessary
- ☐ Check condition and operation of PSD syringe – ensure it does not have air locks and bubbles.
- ☐ Change PSD rinse bottle o-ring.
- ☐ Check and clean the rinse vessel.
- ☐ Check the drain tube for good drainage. It should not have tight bends, kinks or loops and the lower end must be above the liquid level in the waste vessel.
- ☐ Ensure that the waste vessel is suitable for use with the furnace system.

Agilent
เอกสารไม่ควบคุม

Vapor generation accessory VGA (hydride generator)

- ☐ Section NOT Applicable.
- ☐ Inspect VGA gas supply hose.
- ☐ Inspect/replace VGA pump tubing.
- ☐ Check low gas pressure interlock setting– adjust if required.
- ☐ Check precision orifice gas flow setting – adjust if required.
- ☐ Check gas regulator pressure to 46 psi (325 kPa) – adjust if required.
- ☐ Clean the exterior surfaces of the accessory with soft lint free cloth. This cloth can be dampened with warm water or a mild detergent. Do not use organic solvents or abrasive cleaning agents.

UltrAA Lamp Accessory (external)

- ☑ Section NOT Applicable.
- ☐ Check the condition of the power cable.
- ☐ Clean the exterior surfaces of the accessory with soft lint free cloth. This cloth can be dampened with warm water or a mild detergent. Do not use organic solvents or abrasive cleaning agents.

Restore System

- ☐ If you have altered the customer's instrumentation during the course of PM, restore to the original status to allow the customer to conduct their normal activities (e.g., reload the customer's method.)

Guidance

If the PM service is performed prior to a qualification service, then use the qualification procedure as a guide for final instrument set up and checkout.

Signature Page

Service Review

- ☐ Attach available reports/printouts of all tests to this documentation.
- ☐ Record the Preventive Maintenance service activity in the customer's records/logbook.
- ☐ Update/reset instrument maintenance counters as appropriate.
- ☐ Affix the PM sticker to the system or instrument logbook based on the customer's request.
- ☐ Complete the Service Engineer Comments section if there are additional comments.
- ☐ Review this service, parts replaced, and test results obtained with the customer.
- ☐ If the instrument firmware was updated, record the details of the change in the Service Engineer's Comments box or if necessary, in the customer's IQ records.

Agilent
เอกสารไม่ควบคุม

Accessories

- ☐ Section NOT applicable.

Sample introduction pump system (SIPS) accessory

- ☑ Section NOT Applicable.
- ☐ Re-torque screws securing the hubs, presser arms and pump rotors.
- ☐ Adjust each roller so that it rotates freely.
- ☐ Wipe clean the pump rotor rollers and pump bands with a dry clean cloth.
- ☐ Ensure that the presser arms and the surfaces near the pump are free from dirt and spills.
- ☐ Remove the pump module rear cover and check for the incursion of liquids and any signs of corrosion.
- ☐ Re-torque the nuts that fasten the motor mounting plates to the chassis.
- ☐ Check clips securing the diluents holder and replace if necessary.
- ☐ Disconnect, clean T-piece, and reassemble the tubing using the following steps.
- ☐ Remove the T-piece by disconnecting the pump tubes, the pump bands and all other tubing.
- ☐ Place the T-piece in an ultrasonic bath containing strong detergent 1-5% Decon 30 or similar, for approximately 5-10 minutes.
- ☐ Wash the T-piece under a tap with a strong flow of water.
- ☐ Rinse with distilled water through all of the inlets in the reverse direction to normal sample flow.
- ☐ Reassemble.

Sample preparation system (SPS 4) accessory

- ☑ Section NOT Applicable.

The Agilent SPS 4 autosampler is designed to need minimal maintenance.

The following maintenance requirements are suggested to maintain the performance of the autosampler.

- ☐ Cleaning the spill tray, rack location mat, end frames and chassis accessories with a damp soft cloth and diluted mild detergent.
- ☐ Cleaning the autosampler cover panels with domestic window cleaner.
- ☐ Checking the X- axis and Z- axis drive belts for cracks, splits, damaged teeth, excessive fraying, color changes or degradation from fumes.
- ☐ Check the X- axis, Theta- axis and Z- axis FFC cables for cracks, incorrect positioning, damaged edge or damaged connectors.

NOTE The autosampler requires no extra lubrication throughout its lifetime.

For further details refer to the SPS 4 service manual G8410-90050.

Agilent
เอกสารไม่ควบคุม

Test Results

Test description	Expected test result	Actual test result
Flame optics PMT Gain test		
For copper at 324.8 nm, 4 mA, 0.5 nm slit width	< 55 %	46 %
Flame performance test with 5 ppm copper sample		
Air /acetylene, mixing paddle removed	Abs value > 0.6	0.6381
Air /acetylene, mixing paddle installed 10 replicates	%RSD < 1.0	0.7 %
Deuterium furnace optics PMT Gain test		
For copper at 324.8 nm, 4 mA, 0.5 nm slit width	< 55 %	-
Deuterium furnace performance test with 25 ppb copper sample (324.8 nm)		
Precision %RSD	≤ 4.0%	-
Abs value	≥ 0.15	-
Zeeman furnace analytical performance: 25 ppb copper sample (324.8 nm)		
Precision %RSD	≤ 4.0%	-
Abs value	≥ 0.15	-
MSR% (327.4 nm)	≥70 %	-

AA consumable and parts list

Part Description	Part Number	Product/Model # where used	PM supplied or Consumable	Instrument-Type
Test Solution – Cu 6ppm solution	6610030103	55 240 280	PM supplied	Common
Test Solution - Blank solution	5190-7901	55 240 280	PM supplied	Common
Copper, 1000 ug/ml, 100ml	5190-6279	55 240 280	*	Common
Kit, Mk 7 O-rings, aqueous, complete set	9910093400	55 240 280	PM supplied	Flame
Organic Kit	9910093500	55 240 280	PM supplied	Flame
Wire Nebulizer Cleaning	9910024700	55 240 280	consumable	Flame
Tubing-Capillary Std Nebs	9910024800	55 240 280	consumable	Flame
Capillary Tube Hivac Neb (3) (organics only)	9910044000	55 240 280	consumable	Flame
Glass impact beads (5/pk)	9910025700	55 240 280	consumable	Flame

Agilent
เอกสารไม่ควบคุม

Teflon impact beads (5/pk): (organics only)	9910053900	55 240 280	consumable	Flame
Burner cleaning strip (100/pk)	9910053900	55 240 280	consumable	Flame
Window UV silica – round (right side)	2010082600	55 240 280	PM supplied	Common
Window UV silica – rectangular (left side)	2010082500	55 240 280	PM supplied	Common
Pad adhesive window (round)	4910012700	55 240 280	PM supplied	Common
Pad adhesive window (rectangular)	4910012800	55 240 280	PM supplied	Common
Electrode kit (1 pr) (D2)	6310003400	GTA120	PM supplied	Furnace
Shroud (D2)	6310003100	GTA120	PM supplied	Furnace
Zeeman electrode kit (1 pr)	5310003500	GTA120	PM supplied	Furnace
Zeeman shroud	6310003600	GTA120	PM supplied	Furnace
O-ring PSD rinse bottle	6910025900	PSD120	PM supplied	Furnace

* For engineers who only service AA instruments 5100-8275 can be used as a cheaper alternative for 5610030100

Items classified as PM supplied in the above table are included in the standard PM.

Those classified as consumable should be provided by the customer or charged to the customer if supplied by the Agilent service engineer.

Service Engineer Comments (optional)

If there are any specific points you wish to note as part of performing the installation or other items of interest for the customer, please write them in this box.

Agilent
เอกสารไม่ควบคุม

SVD Results Report

VARIAN

Report ID:3 *Diagnostic Start Time:1/26/2026 8:39:56 AM* *Diagnostic End Time:1/26/2026 9:05:49 AM*

Customer: UAE *Service Engineer:* Kanyakorn S.

Address: *Contact Details:* 0263763631

Instrument Configuration

Configuration:

Serial Number: MY13180001
Instrument Model: Varian AA140/240/280
Flame Instrument: True
Furnace Instrument: True
Zeeman Present: False
Internal Zeeman: False
Internal UltrAA: False
Optics Type: Double Beam
D2 BG Correction Fitted: True
Boot Block Version: 1.09

Turret Type: Automatic
Number Of Lamps: 4
Mono Type: Automatic
Gasbox Type: 'Y' Gas Box
Auto Burner Adjuster: False
Mains Frequency: 50
Firmware Version: 2.11
Photomultiplier Type: Normal(900nm)
PWB Version: 45

EEPROM Data:

Instrument Run Hours: 79270.802
Zero Wavelength Offset: 30.095
Mono Correction: 0.766
Flame Hours: 35125.582

D2 Run Hours: 58906.000
D2 Serial Number: not set !
D2 Install Date: 1/1/1970
D2 Original Intensity: 1.000
D2 Last Intensity: 475.000

Frequency:

Averaging Period: 30.0
Datapoint Count: 20

Upper Limit: 51.00
Lower Limit: 49.00
Average Frequency: 50.00
Highest Measured Frequency: 50.00
Lowest Measured Frequency: 50.00

Result: Passed

เอกสารไม่ควบคุม

Service Completion

Service Request Number: 6009098466
Service Engineer Name: Kanyakorn S.
Service Engineer Signature: Kanyakorn S.

Date of Service Completion: 26 Jan 2026
Customer Name: Hamda Hamad
Customer Signature:

Agilent
เอกสารไม่ควบคุม

Power Supply:

Averaging Period: 30.0
Datapoint Count: 20


	Lower Limit (V)	Actual (V)	Upper Limit (V)	Result:
12.00 V Rail	10.80	12.20	13.20	Passed
-12.00 V Rail	-13.20	-11.90	-10.80	Passed
5.00 V Rail	4.50	5.02	5.50	Passed
310.00 V Rail	279.00	320.00	341.00	Passed

เอกสารไม่ควบคุม


Optics

Beam Balance:

Lamp Type: Copper
Lamp Socket Used: 3
Peak Selected: 324.80
Lamp Alignment: Performed

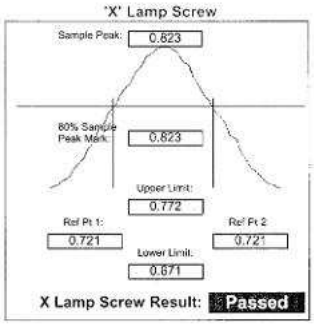

X Lamp Screw Result: Passed

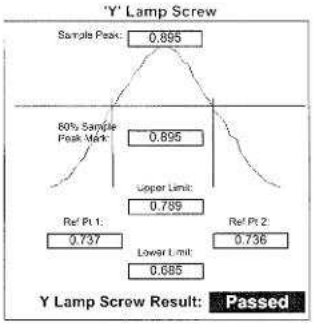

Y Lamp Screw Result: Passed

Grating Squareness:

Lamp Element(s): Copper
Lamp Turret Position: 3
Lamp Current(mA): 4.00
Slit Width(nm): 0.5
1st Order Wavelength(nm): 324.80
Lamp Alignment: Performed

	Lower Limit (nm)	Actual (nm)	Upper Limit (nm)	Result:
Zero Order	-0.10	0.00	0.10	Passed
First Order	324.45	324.74	325.15	Passed
Second Order	649.23	649.50	649.97	Passed

เอกสารไม่ควบคุม

Mechanical

Wavelength Drive: Passed

Slit Drive: Passed

Turret Drive: Passed

Auto Burner Adjuster Drive: Untested

Miscellaneous

Signal Processing Linearity:

Calculate Mode: New Calc Mode

	Lower Limit	Actual	Upper Limit	Result:
S0	114	261	297	Passed
S1	156	165	191	Passed
S2	271	296	332	Passed
S3	474	508	579	Passed
S4	825	919	1008	Passed
S5	1435	1529	1754	Passed
S6	2498	2771	3053	Passed
S7	4347	4755	5313	Passed

Interlocks:

Burner Fitted: Working
N2O Burner Fitted: Untested
Flame Shield Closed: Working
Gas Control Fitted: Untested
Pressure Release Bung Fitted: Working
Liquid Trap Fitted: Working
Flame Detect: Working
GCU Active: Working
Oxidant Pressure: Working
Oxidant Changeover: Untested
Ignition: Working

เอกสารไม่ควบคุม

Wavelength Repeatability:

Lamp Used: Copper
Lamp Current(mA): 4
Peak Used(nm): 324.750
Slit Width(nm): 0.2
Connected to Socket: 3
Slit Height: Normal
Lamp Alignment: Performed

Lower Limit(nm) 324.768 — 324.888 **Upper Limit(nm)**

(Approach from Zero Order)		(Approach from end)	
Sample 1:	324.828	Sample 2:	324.823
Sample 3:	324.823	Sample 4:	324.823
Sample 5:	324.823	Sample 6:	324.819
Sample 7:	324.823	Sample 8:	324.819
Sample 9:	324.819	Sample 10:	324.819

Mean: 324.823 **Standard Deviation:** 0.003

Result: Passed

เอกสารไม่ควบคุม

Auto Lamp Recognition:

Lamp 1: 87 - Silver/Cadmium/Lead/Zinc(UltrAA) (Ag/C
Lamp 2: 68 - Zinc (Zn)
Lamp 3: 14 - Copper (Cu)
Lamp 4: Uncoded Lamp/Not Connected
Lamp 5: Not Supported
Lamp 6: Not Supported
Lamp 7: Not Supported
Lamp 8: Not Supported

Result: Passed

GTA Temperature Monitoring:

Not Performed

Notes:

Signatures:

Jamil de Hayi	26 Jan 26	Kanyakorn S.	26 Jan 2026
UAE	Date	Kanyakorn S.	Date

เอกสารไม่ควบคุม

Sequential by time report 1/26/2026 9:54 AM SpectrAA
Page 1 of 1

Analyst
Date Started 1/26/2026 9:07 AM GMT: 1/26/2026 2:07 AM
Worksheet Sensitivity Test
Comment
Methods Cu
Computer name DESKTOP-RSUFRS
Serial Number: MY13160001

Method: Cu (Flame)

Sample ID	Exp Abs	%RSD	Mean Abs		
5 ppm Cu	0.633	1.4	0.6331		
	Readings				
	0.6413	0.6340	0.6241	1/26/2026	

เอกสารไม่ควบคุม

Sequential by time report 1/26/2026 10:15 AM SpectrAA
Page 1 of 1

Analyst
Date Started 1/26/2026 9:07 AM GMT: 1/26/2026 2:07 AM
Worksheet Precision Test
Comment
Methods Cu
Computer name DESKTOP-RSUFRS
Serial Number: MY13160001

Method: Cu (Flame)

Sample ID	Exp Abs	%RSD	Mean Abs			
5 ppm Cu	0.618	0.7	0.6180			
	Readings					
	0.6145	0.6187	0.6081	0.6168	0.6253	0.6196
	0.6197	0.6195	0.6188	0.6189	1/26/2026	

เอกสารไม่ควบคุม

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX.0-2719-9484

Certificate of Calibration

Cert.No.: 26CH143
Page.: 1 of 3

Equipment :	Conductivity Meter
Manufacturer :	Horiba
Model :	LAQUA-EC210
Serial No. :	HC9L0011
ID No. :	UAE.EFM.009/2563(EFM.SCT.03/63)
Condition As-Received:	Used Item
Received Date :	02 February 2026
Calibration Date :	03 February 2026
Reference :	2602-0038WSC-2
Submitted by :	United Analyst and Engineering Consultant Co.,Ltd. 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure:	In -house method : - CP-CH6 by direct measurement with certified reference material (CRM) - CP-CH8 by comparison with temperature standard
Calibrated by :	Walalak Sirithean
Approved by :	Approved Signatory

( ) Chakrit Waewwanjua
( ) Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 04 February 2026

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Cert.No.: 26CH143
Page.: 2 of 3

Condition of this result of calibration

1. Reference Standard Instrument :-

Instrument	Serial No.	ID No.	Certificate No.	Due date
1) Thermometer	9549224	130RC003	25I440	16 Apr 2026
2) Ref. Std.Thermometer	4982054	110RC044	25I708	03 July 2026

- This measurement result is traceable to SI throught Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials :-
- Conductivity calibration solution, CPA chem Ltd., The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Conductivity Solution	Manufacturer	Lot No.	Exp. date
1413.5 µS/cm	CPA Chem	1150497	30 Oct 2026
12.881 mS/cm	CPA Chem	1081099	11 Mar 2026

- Control Conductivity calibration solution temperature by Water bath (25 ± 0.1) °C

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration results

Function : Conductivity Measurement
(*) After Adjustment at 1413.5 µS/cm
Conductivity Electrode Serial No.: 9B9F0045

Standard Conductivity Solution	Before Adjustment UUC* Reading	After Adjustment UUC* Reading	Uncertainty of Measurement (±)	Coverage factor *k*
1413.5 µS/cm	1569 µS/cm	1413 µS/cm	9.2 µS/cm	2.00
12.881 mS/cm	14.07 mS/cm	12.82 mS/cm	0.086 mS/cm	2.00

Remark : **- UUC* = Unit Under Calibration**

Calibration Results

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : 9383
- Serial No. : 9B9F0045

Dimension of probe;

- Length : 110 mm
- Diameter : 16 mm
- Immersion Depth : 100 mm

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of Measurement (± °C)	Coverage factor *k*
15.0	15.002	15.0	-0.002	0.13	2.00
30.0	30.001	30.0	-0.001	0.13	2.00
45.0	45.001	45.0	-0.001	0.13	2.00

Remark : - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Condition of this result of calibration

1. Reference Standard Instrument :-

Instrument	Serial No.	ID No.	Certificate No.	Due date
1) Thermometer	9549224	130RC003	25I440	16 Apr 2026
2) Ref. Std.Thermometer	4982054	110RC044	25I708	03 July 2026

- This measurement result is traceable to SI throught Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials :-
   - Conductivity calibration solution, CPA chem Ltd., The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Conductivity Solution	Manufacturer	Lot No.	Exp. date
1413.5 µS/cm	CPA Chem	1150497	30 Oct 2026
12.881 mS/cm	CPA Chem	1081099	11 Mar 2026

   - Control Conductivity calibration solution temperature by Water bath (25 ± 0.1) °C

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration results

Function : Conductivity Measurement

(*) After Adjustment at 1413.5 µS/cm

Conductivity Electrode Serial No.: 9B9F0286

Standard Conductivity Solution	Before Adjustment UUC* Reading	After Adjustment UUC* Reading	Uncertainty of Measurement (±)	Coverage factor *k*
1413.5 µS/cm	1431 µS/cm	1413 µS/cm	9.2 µS/cm	2.00
12.881 mS/cm	12.92 mS/cm	12.76 mS/cm	0.086 mS/cm	2.00

Remark : - UUC* = Unit Under Calibration

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

Certificate of Calibration

Equipment :	Conductivity Meter
Manufacturer :	Horiba
Model :	LAQUA-EC210
Serial No. :	HC9L0013
ID No. :	UAE.EFM.011/2563(EFM.SCT.05/63)
Condition As-Received:	Used Item
Received Date :	02 February 2026
Calibration Date :	03 February 2026
Reference :	2602-0038WSC-3
Submitted by :	United Analyst and Engineering Consultant Co.,Ltd. 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure:	In -house method : - CP-CH6 by direct measurement with certified reference material (CRM) - CP-CH8 by comparison with temperature standard
Calibrated by :	Walalak Sirithean
Approved by :	Approved Signatory

( ) Chakrit Waewwanjua
( ) Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 04 February 2026

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Calibration Results

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : 9383
- Serial No. : 9B9F0286

Dimension of probe;

- Length : 110 mm
- Diameter : 16 mm
- Immersion Depth : 100 mm

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of Measurement (± °C)	Coverage factor *k*
15.0	15.002	15.0	-0.002	0.13	2.00
30.0	30.001	30.0	-0.001	0.13	2.00
45.0	45.001	45.0	-0.001	0.13	2.00

Remark : - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

Certificate of Calibration

Cert.No.: 26CH145
Page.: 1 of 3

Equipment : Conductivity Meter
Manufacturer : Horiba
Model : LAQUA-EC210
Serial No. : HC1L0016
ID No. : UAE.EFM.014/2565(EFM.SCT.01/65)
Condition As-Received: Used Item
Received Date : 02 February 2026
Calibration Date : 03 February 2026
Reference : 2602-0038WSC-4
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260

Ambient Temperature : (25 ± 2.5) °C
Relative Humidity : (50 ± 15) %
Calibration Procedure: In -house method :
- CP-CH6 by direct measurement with certified reference material (CRM)
- CP-CH8 by comparison with temperature standard

Calibrated by : Walalak Sirithean

Approved by :
Approved Signatory

( ) Chakrit Waewwanjua
( ) Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 04 February 2026

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Calibration Results
Function : Temperature Measurement
(*) Without adjustment
This equipment was connected with Temperature Probe;
- Model : 9383
- Serial No. : 9B1J0042

Dimension of probe;
- Length : 110 mm
- Diameter : 16 mm
- Immersion Depth : 100 mm

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of Measurement (± °C)	Coverage factor k
15.0	15.002	15.0	-0.002	0.13	2.00
30.0	30.001	30.0	-0.001	0.13	2.00
45.0	45.001	45.0	-0.001	0.13	2.00

Remark : - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Condition of this result of calibration
1. Reference Standard Instrument :-

Instrument	Serial No.	ID No.	Certificate No.	Due date
1) Thermometer	9549224	130RC003	25I440	16 Apr 2026
2) Ref. Std.Thermometer	4982054	110RC044	25I708	03 July 2026

- This measurement result is traceable to SI throught Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials :-
- Conductivity calibration solution, CPA chem Ltd., The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Conductivity Solution	Manufacturer	Lot No.	Exp. date
1413.5 µS/cm	CPA Chem	1150497	30 Oct 2026
12.881 mS/cm	CPA Chem	1081099	11 Mar 2026

- Control Conductivity calibration solution temperature by Water bath (25 ± 0.1) °C

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration results
Function : Conductivity Measurement
(*) After Adjustment at 1413.5 µS/cm
Conductivity Electrode Serial No.: 9B1J0042

Standard Conductivity Solution	Before Adjustment UUC* Reading	After Adjustment UUC* Reading	Uncertainty of Measurement (±)	Coverage factor k
1413.5 µS/cm	1330 µS/cm	1413 µS/cm	9.2 µS/cm	2.00
12.881 mS/cm	12.17 mS/cm	12.91 mS/cm	0.086 mS/cm	2.00

Remark : **- UUC* = Unit Under Calibration**

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000 FAX. 0-2719-9484

Certificate of Testing

Cert.No.: 25TW213
Page.: 1 of 2

Equipment : DO Meter
Manufacturer : YSI
Model : 4010-2W
Serial No. : 20260326
ID No. : UAE.WAO.060/2563
Received Date : 17 October 2025
Test Date : 22 October 2025
Reference : 2510-0505DSC-1
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260

Laboratory Condition : Temperature (25 ± 5) °C
Humidity (50 ± 20) %
Test Procedure : In - house method : CP-CH9
by Comparison Technique with Azide Modification Method

Tested by : Walalak Sirithean

Approved by : Saithip
Approved Signatory

( ) Chakrit Waewwanjua
( ) Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 23 October 2025

เอกสารไม่ควบคุม

Cert.No.: 25TW213
Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :
   This measurement result is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

Instruments	ID No.	Certificate No.	Due Date
1. Burette	130BU10	25CG1126	18 Mar 2027
2. Balance	110RC001	25MM316	02 July 2026

2. Standard Material :-

Material	Manufacturer	Lot.No.	Assay
Sodium Thiosulfate 5-Hydrate AR	KEMAUS	2203162447	99.6%

Result : **Dissolved Oxygen Meter Adjustment With Air 100 %**
Dissolved Oxygen Probe No.: 22M102385

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.22	8.31	0.0055

This report was certified only for the instrument we tested.It is allowable to use for study Intend to use for advertising and referral purpose is prohibited.This report may not be reproduced other in full, without written approval of the laboratory

-o0o-

เอกสารไม่ควบคุม

FOSS

Customer Service Report

FOSS South East Asia
3388 Sirinrat Building, 25th – 26th Floor, Unit No. 3388/90,
Rama IV Road, Klongton , Klongtoey, Bangkok, Thailand 10110

Report No.:	15257
Date:	Feb 12, 2026
Customer:	UAE
Job No.:	14590
Address:	Bangkok
Instrument:	DT2520
Serial:	91905060

	Travel To Customer (Hrs)		Labour (Hrs)		Travel From Customer (Hrs)	
Start	-		13.30	1.5	-	
Finish	-	-	15.00		-	-

Job Type						
Application		Special		Standard		
Distributor		Courtesy Visit		Installation		In House
Digital Service		PMA Approval Check		Quote		PM X
Internal		Warranty -		Repair		HC Visit
Training		Sales Support		Investigate		Others

PMA Type					
	Smartcare		Smartcare Pro		Fosscare X
	Smartcare Advance		Fosscare Pro		N/A

Details of Work / Test

- PM -
- Visual Check
  + No leak -ok
  + No Damage -ok
- Change PM kit x 1 Set -ok
- Function Check
  + Quick mode
    + Set Temp Timer -ok
    + Run -ok
  - Heating -ok
  - Lift + Up down -ok
- Clean x20 holes with Cloth head

Instrument Ready for Use	OK	X	Not OK*	

Part No:	Batch	Description	Q'ty
60079730	29.09.2025	FOD PM kit, Digester 20 pcs, 12 mths	1

I confirm this report is accurate and complete

Signed FOSS		Signed Customer	
Name:	Anuwat Patchan / Jakkaew	Name	
Tel:		Tel:	
Email:		Email:	

*Remark:

เอกสารไม่ควบคุม

Please scan QR code

FOSS

Customer Service Report

FOSS South East Asia
3388 Sirinrat Building, 25th – 26th Floor, Unit No. 3388/90,
Rama IV Road, Klongton , Klongtoey, Bangkok, Thailand 10110

Report No.:	15256
Date:	Feb 12, 2026
Customer:	UAE
Job No.:	14589
Address:	Bangkok
Instrument:	KT9 Distillator
Serial:	91905393

	Travel To Customer (Hrs)		Labour (Hrs)		Travel From Customer (Hrs)	
Start	08.00	1.5	09.30	4	-	-
Finish	09.30		13.30		-	-

Job Type						
Application		Special		Standard		
Distributor		Courtesy Visit		Installation		In House
Digital Service		PMA Approval Check		Quote		PM X
Internal		Warranty -		Repair		HC Visit
Training		Sales Support		Investigate		Others

PMA Type					
	Smartcare		Smartcare Pro		Fosscare X
	Smartcare Advance		Fosscare Pro		N/A

Details of Work / Test

- PM -
- Visual Check
  + No leak -ok
  + No damage -ok
- change PM kit x1 Set -ok
- Function Check
  + Digestion -ok
  + Alkali -ok
  + Receiver -Not Use
  + Steam Distill -ok

Instrument Ready for Use	OK	X	Not OK*	

Part No:	Batch	Description	Q'ty
60100196	11.05.2025	PM kit kjeltec 8 Distillator	1

I confirm this report is accurate and complete

Signed FOSS		Signed Customer	
Name:	Anuwat Patchan / Jakkaew	Name	
Tel:		Tel:	061 950 9894
Email:		Email:	Pitiya.Sakuwong@gmail.com

*Remark:

เอกสารไม่ควบคุม

Please scan QR code

UAE.FM.6.4.028-L00/9-SEP-2020

แบบบันทึกผลการทวนสอบเตาย่อย (Heating Block/Digestion Unit)

รายละเอียดเครื่องมือที่ทวนสอบ — หมายเลขประจำเครื่องบริษัท: UAE.WAS.011/1590
เครื่องมือ: Digestion Units — ยี่ห้อ: Foss Tecator
หมายเลขเครื่อง: 91990869 — รุ่น: 1570 auto
หมายเลขใบสอบเทียบ: 2409257-001-01 — วันที่สอบเทียบ: 03/11/2025

รายละเอียดเครื่องมือที่ใช้ทวนสอบ (Reference Standard) — สภาวะที่ทวนสอบ
เครื่องมือ: Digital Thermometer, Thermocouple Type K — ยี่ห้อ: - — สภาวะที่ทวนสอบ
หมายเลขเครื่อง: 1.5390105 — รุ่น: DM-52 — อุณหภูมิ: -
หมายเลขประจำเครื่องบริษัท: UAE.WAS.249/2565 — ความชื้นสัมพัทธ์: -
หมายเลขเครื่อง(Probe): UAE.WAS.005/2565
หมายเลขใบสอบเทียบ: 2500496-001-01 — วันที่สอบเทียบ: 03/11/2565 — ทวนสอบโดย: ปิติยา

ผลการทวนสอบเตาย่อย Calibration Point 380 °C

เตาย่อยหลุมที่ Calibration Point 380 °C Setting Point 380 °C	อุณหภูมิที่อ่านได้จากเตาย่อย (°C) Digestor Unit UAE.WAS.049/2560 ครั้งที่ 1	ครั้งที่ 2	ค่าเฉลี่ย	ค่าผลต่างแก้แล้ว	อุณหภูมิที่อ่านได้จาก Reference Standard (°C) UAE.WAS.004/2565 ; Thermometer UAE.WAS.005/2565 ; Thermocouple ครั้งที่ 1	ครั้งที่ 2	ค่าเฉลี่ย	ค่าผลต่างแก้แล้ว Correction 0.0
A1	380	380	380	-	379.6	379.3	379.5	379.5
A2	381	381	381	-	380.7	380.3	380.5	380.5
A3	381	380	381	-	380.6	380.4	380.4	380.4
A4	381	381	381	-	381.4	381.2	381.3	381.3
B1	381	382	381	-	381.1	380.9	381.1	381.1
B2	380	381	381	-	380.6	380.8	380.7	380.7
B3	380	381	381	-	382.8	383.1	383.0	383.0
B4	381	381	381	-	381.2	381.1	381.0	381.0
C1	380	380	380	-	380.7	380.4	380.4	380.4
C2	380	381	381	-	379.7	379.3	379.5	379.5
C3	380	380	380	-	380.5	380.9	380.7	380.7
C4	381	381	381	-	381.1	381.3	381.2	381.2
				-				


สมายเหตุ : เก็บในแฟ้ม 2569-05

เอกสารไม่ควบคุม

\\ae.netapp\Netapp_LAB\Lab-EK\INSTRUMENT (11-2)\คอมบันทึกผลการทวนสอบ, ตัวอย่างการบันทึกการทวนสอบ, Digestor TKN (2025_2555)

ผลการทวนสอบ (ต่อ)

เลาย่อยหลุมที่ / Calibration Point 330 °C / Setting Point 330 °C	อุณหภูมิที่อ่านได้จากเลาย่อย (°C) Digestor Unit: UAE.WAS.011/5568				อุณหภูมิที่อ่านได้จาก Reference Standard (°C) UAE.WAS.005/2555 : Thermometer UAE.WAS.005/2555 : Thermocouple			
	ครั้งที่ 1	ครั้งที่ 2	ค่าเฉลี่ย	ผิดค่าแก้แล้ว	ครั้งที่ 1	ครั้งที่ 2	ค่าเฉลี่ย	ผิดค่าแก้แล้ว Correction 0.0
D1	390	391	391	-	390.8	391.3	391.6	391.6
D2	390	391	391	-	390.5	391.7	391.9	391.5
D3	391	391	391	-	391.9	391.5	391.7	391.7
D4	391	390	391	-	390.6	390.9	390.4	390.4
				-				
E1	391	391	391		391.0	390.8	390.9	391.1
E2	391	391	391	-	390.7	391.1	390.9	390.9
E3	390	391	391	-	390.1	391.9	391.0	391.0
E4	389	390	390	-	390.1	389.5	389.9	389.9
				-				
ค่าเฉลี่ย	-		-	-	-	-	-	-
ค่าส่วนเบี่ยงเบนมาตรฐาน	-		-	-	-	-	-	-
ค่าความผิดพลาด	พิจารณาค่าความผิดพลาดแต่ละจุดให้อยู่ในช่วงเกณฑ์การยอมรับ							
เกณฑ์การยอมรับ	380 ±5 °C							
ผลการทวนสอบ								



ผู้บันทึก ปิติพร
วันที่ 13 ก.พ. 68

ผู้ตรวจสอบ
วันที่ 25 ก.พ. 68

หมายเหตุ : เก็บในแฟ้ม WQ - 04

เอกสารไม่ควบคุม

Condition of this result of calibration

1. Reference Standard Instruments :
   This measurement result is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

Instruments	ID No.	Certificate No.	Due Date
1. Burette	130BU10	25CG1126	18 Mar 2027
2. Balance	110RC001	25MM316	02 July 2026

2. Standard Material :-

Material	Manufacturer	Lot.No.	Assay
Sodium Thiosulfate 5-Hydrate AR	KEMAUS	2203182447	99.6%

Result : **Dissolved Oxygen Meter Adjustment With Air 100 %**
Dissolved Oxygen Probe No.: 24F100202

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.20	8.20	0.0084

This report was certified only for the instrument we tested.It is allowable to use for study Intend to use for advertising and referral purpose is prohibited.This report may not be reproduced other in full, without written approval of the laboratory

-o0o-

เอกสารไม่ควบคุม

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000 FAX. 0-2719-9484

Certificate of Testing

Equipment :	DO Meter
Manufacturer :	YSI
Model :	5100
Serial No. :	11B 101863
ID No. :	UAE.WAO.004/2554
Received Date :	27 February 2026
Test Date :	02 March 2026
Reference :	2602-0915DSC-1
Submitted by :	United Analyst and Engineering Consultant Co.,Ltd. 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Laboratory Condition :	Temperature (25 ± 5) °C Humidity (50 ± 20) %
Test Procedure :	In - house method : CP-CH9 by Comparison Technique with Azide Modification Method
Tested by :	Walalak Sirithean
Approved by :	Sailhip Approved Signatory

( ) Chakrit Waewwanjua
( ) Ponpan Paipim
(✓) Sailhip Meangmal

Issue Date : 03 March 2026

เอกสารไม่ควบคุม

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

ilac-MRA
NSC-TISI-TIS17025 CALIBRATION 0006

Certificate of Calibration

Equipment :	Water Bath
Manufacturer :	Memmert
Model :	WNE 14
Serial No. :	L416.0612
ID No. :	MIC.003/2560
Submitted by :	United Analyst and Engineering Consultant Co.,Ltd. 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Location :	Microbiology Laboratory (302)
Received Order :	02 February 2026
Calibration Date :	02 February 2026
Ambient Temperature :	(26 ± 10) °C
Relative Humidity :	(50 ± 30) %
AC Line Voltage :	(220 ± 22) V
Calibrated by :	Krisda Malee
Approved by :	Kunchit Approved Signatory

( ) Chakrit Waewwanjua
( ) Suwit Imjai
(✓) Kunchit Promprat

Issue Date : 17 February 2026

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX.0-2719-9484

Certificate of Calibration

Cert.No.: 26CH231
Page.: 1 of 3

Equipment :	pH Meter
Manufacturer :	Horiba
Model :	LAQUA-PH210
Serial No. :	HA9M0047
ID No. :	UAE.EFM.005/2563 (EFM.pH.05/63)
Condition As-Received:	Used Item
Received Date :	24 February 2026
Calibration Date :	26 February 2026
Reference :	2602-0796WSC-2
Submitted by :	United Analyst and Engineering Consultant Co.,Ltd. 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure :	In - house method : - CP-CH5 by direct measurement with DC voltage standard and direct measurement with certified reference material (CRM) - CP-CH8 by comparison with temperature standard
Calibrated by :	Walalak Sirithean
Approved by :	Approved Signatory

( ) Chakrit Waewwanjua
( ) Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 27 February 2026

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT04 Based on ASTM E715 according to direct measurement method with Data Acquisition which connected with Industrial Platinum Resistance Thermometer (IPRT).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-


Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY57013711	25LM117	TPA	17 Jul 2026

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This measurement result is traceable to the International System of Unit maintained through :

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Heat transfer medium used : Water

	Environmental		AC Voltage Supply
	(°C)	(%R.H.)	(Volt)
Beginning of Calibration	25	52	221
Finished of Calibration	24	51	220



Front

Position :	Ref. Std. ID No.:
1	4803988-001
2	4803988-002
3	4803988-003
4	4803988-004
5(ref.)	4803988-005

เอกสารไม่ควบคุม

Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source

Calibration point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Average* Standard Reading (°C) Position 1	2	3	4	5 (ref.)	Uncertainty (± °C)
44.5	44.6	44.6	44.518	44.463	44.472	44.508	44.521	0.15

Calibration point (°C)	Uniformity (°C)	Stability (± °C)	Coverage Factor *k*
44.5	0.11	0.044	2

Average* : The average of 30 values in each position.
Uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.
Stability : One-half of the greatest maximum difference of measured temperature at any one probe.
UUC* : Unit Under Calibration
Note : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม

Condition of this calibration result

1. Reference Standard Instrument

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1) Document Process Calibrator	54030049	130RC116	25E2743	25 Aug 2026
2) Ref. Standard Thermometer	4982054	110RC044	25I708	03 July 2026

- This measurement result is traceable to SI throught Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials :The measurement results are traceable to SI through Hach Lenge GmbH Ltd., Deutsche Akkreditierungsstelle, Accredited No.D-RM-15184-01-00
:The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.008	CPA chem	1187328	18 Jan 2028
pH 7.000	Hach Lenge GmbH	C03319	17 Oct 2027
pH 10.010	CPA chem	1187332	18 Jan 2027

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4,7)(7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement	Coverage factor
	pH	mV	mV	pH	(±mV)	*k*
pH Meter	4.00	177.48	177.3	4.01	0.058	2.00
S/N.: HA9M0047	7.00	0.00	0.0	7.02	0.058	2.00
	7.00	0.00	0.0	7.02	0.058	2.00
	10.00	-177.48	-177.2	10.01	0.058	2.00

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7)(7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (±)	Coverage factor *k*
pH Electrode	4.008	4.01	161.1	0.0079	2.00
S/N.: -	7.000	7.00	-10.4	0.0096	2.00
	7.000	7.00	-9.9	0.0095	2.00
	10.010	10.02	-177.9	0.0095	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : -
- Serial No. : -

Dimension of probe

- Length : 103 mm.
- Diameter : 16 mm.
- Immersion Depth : 90 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (± °C)	Coverage factor *k*
15.0	15.001	15.0	-0.001	0.13	2.00
30.0	30.001	30.0	-0.001	0.13	2.00
45.0	45.001	44.9	-0.101	0.13	2.00

Remark - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Condition of this result of calibration

1. Reference Standard Instrument :-

Instrument	Serial No.	ID No.	Certificate No.	Due date
1) Thermometer	9549224	130RC003	25I440	16 Apr 2026
2) Ref. Std.Thermometer	4982054	110RC044	25I708	03 July 2026

- This measurement result is traceable to SI throught Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials :-
   - Conductivity calibration solution, CPA chem Ltd., The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Conductivity Solution	Manufacturer	Lot No.	Exp. date
1413.3 µS/cm	CPA Chem	1187337	18 Jan 2027
12.882 mS/cm	CPA Chem	1135362	16 Aug 2026

   - Control Conductivity calibration solution temperature by Water bath (25 ± 0.1) °C

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration results

Function : Conductivity Measurement

(*) After Adjustment at 1413.3 µS/cm

Conductivity Electrode Serial No.: 9B9F0277

Standard Conductivity Solution	Before Adjustment UUC* Reading	After Adjustment UUC* Reading	Uncertainty of Measurement (±)	Coverage factor *k*
1413.3 µS/cm	1462 µS/cm	1413 µS/cm	9.2 µS/cm	2.00
12.882 mS/cm	13.25 mS/cm	12.81 mS/cm	0.086 mS/cm	2.00

Remark : - UUC* = Unit Under Calibration

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

Certificate of Calibration

Equipment :	Conductivity Meter
Manufacturer :	Horiba
Model :	LAQUA-EC210
Serial No. :	HC9L0015
ID No. :	UAE.EFM.010/2563(EFM.SCT.04/63)
Condition As-Received:	Used Item
Received Date :	24 February 2026
Calibration Date :	26 February 2026
Reference :	2602-0799WSC-2
Submitted by :	United Analyst and Engineering Consultant Co.,Ltd. 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure:	In -house method : - CP-CH6 by direct measurement with certified reference material (CRM) - CP-CH8 by comparison with temperature standard
Calibrated by :	Walalak Sirithean
Approved by :	Approved Signatory

( ) Chakrit Waewwanjua
( ) Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 27 February 2026

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Calibration Results

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : 9383
- Serial No. : 9B9F0277

Dimension of probe;

- Length : 110 mm
- Diameter : 16 mm
- Immersion Depth : 90 mm

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of Measurement (± °C)	Coverage factor *k*
15.0	15.002	15.0	-0.002	0.13	2.00
30.0	30.001	30.0	-0.001	0.13	2.00
45.0	45.001	45.0	-0.001	0.13	2.00

Remark : - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

Certificate of Calibration

Equipment : Conductivity Meter
Manufacturer : Horiba
Model : LAQUA-EC210
Serial No. : HC1L0026
ID No. : UAE.EFM.015/2565(EFM.SCT.02/65)
Condition As-Received: Used Item
Received Date : 24 February 2026
Calibration Date : 26 February 2026
Reference : 2602-0799WSC-3
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260

Ambient Temperature : (25 ± 2.5) °C
Relative Humidity : (50 ± 15) %
Calibration Procedure: In -house method :
- CP-CH6 by direct measurement with certified reference material (CRM)
- CP-CH8 by comparison with temperature standard

Calibrated by : Walalak Sirithean

Approved by :
Approved Signatory

( ) Chakrit Waewwanjua
( ) Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 27 February 2026

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Condition of this result of calibration

1. Reference Standard Instrument :-

Instrument	Serial No.	ID No.	Certificate No.	Due date
1) Thermometer	9549224	130RC003	25I440	16 Apr 2026
2) Ref. Std.Thermometer	4982054	110RC044	25I708	03 July 2026

- This measurement result is traceable to SI throught Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials :-
- Conductivity calibration solution, CPA chem Ltd., The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Conductivity Solution	Manufacturer	Lot No.	Exp. date
1413.3 µS/cm	CPA Chem	1187337	18 Jan 2027
12.882 mS/cm	CPA Chem	1135362	16 Aug 2026

- Control Conductivity calibration solution temperature by Water bath (25 ± 0.1) °C

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration results
Function : Conductivity Measurement
(*) After Adjustment at 1413.3 µS/cm
Conductivity Electrode Serial No.: 9B1J0077

Standard Conductivity Solution	Before Adjustment UUC* Reading	After Adjustment UUC* Reading	Uncertainty of Measurement (±)	Coverage factor *k*
1413.3 µS/cm	1400 µS/cm	1413 µS/cm	9.3 µS/cm	2.00
12.882 mS/cm	12.78 mS/cm	12.81 mS/cm	0.086 mS/cm	2.00

Remark : **- UUC* = Unit Under Calibration**

Calibration Results
Function : Temperature Measurement
(*) Without adjustment
This equipment was connected with Temperature Probe;
- Model : 9383
- Serial No. : 9B1J0077

Dimension of probe;
- Length : 110 mm
- Diameter : 16 mm
- Immersion Depth : 90 mm

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of Measurement (± °C)	Coverage factor *k*
15.0	15.002	15.0	-0.002	0.13	2.00
30.0	30.001	30.1	0.099	0.13	2.00
45.0	45.001	45.1	0.099	0.13	2.00

Remark : **- UUC* = Unit Under Calibration**

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000 FAX. 0-2719-9484

Certificate of Testing

Equipment : DO Meter
Manufacturer : Horiba
Model : LAQUA-DO210
Serial No. : HE2L0016
ID No. : UAE.EFM.016/2566(EFM.DO.01/66)
Received Date : 24 February 2026
Test Date : 26 February 2026
Reference : 2602-0801WSC-1
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260

Laboratory Condition : Temperature (25 ± 5) °C
Humidity (50 ± 20) %
Test Procedure : In - house method : CP-CH9
by Comparison Technique with Azide Modification Method

Tested by : Walalak Sirithean

Approved by :
Approved Signatory

( ) Chakrit Waewwanjua
( ) Ponpan Paipim
(✓) Saithip Meangmai

Issue Date : 27 February 2026

Condition of this result of calibration

1. Reference Standard Instruments :
This measurement result is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

Instruments	ID No.	Certificate No.	Due Date
1. Burette	130BU10	25CG1126	18 Mar 2027
2. Balance	110RC001	25MM316	02 July 2026

2. Standard Material :-

Material	Manufacturer	Lot.No.	Assay
Sodium Thiosulfate 5-Hydrate AR	KEMAUS	2203162447	99.6%

Result : **Dissolved Oxygen Meter Adjustment With Air 100 %**
Dissolved Oxygen Probe No.: 9K2J0004

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.22	8.22	0.0084

This report was certified only for the instrument we tested.It is allowable to use for study Intend to use for advertising and referral purpose is prohibited.This report may not be reproduced other in full, without written approval of the laboratory

-o0o-

Equipment : DO Meter with Sensor
Condition As-Received : Used Item
Reference : 2602-0801WSC-2
Procedure Used :-
Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.
The temperature scale used was based on ITS-90.

Condition of this result of calibration
1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Digital Thermometer	2188080	25I953	TPA	05 Sep 2026

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This measurement result is traceable to the International System of Unit maintained through :
Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment
Function : Temperature measurement.
This instrument was connected with temperature sensor, S/N.: 9K2J0004

Calibration Point (°C)	Immersion Depth (mm)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty (± °C)	Coverage Factor *k*
15.0	80	15.002	15.0	-0.002	0.16	2.00
30.0	80	30.005	29.9	-0.105	0.16	2.00
45.0	80	45.002	44.9	-0.102	0.16	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor ***k***, providing a level of confidence of approximately 95 %.

-o0o-

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

ilac-MRA
NSC-TISI-TIS17025 CALIBRATION 0308

Certificate of Calibration

Equipment : DO Meter with Sensor
Manufacturer : Horiba
Model : LAQUA-DO210
Serial No. : HE2L0016
ID No. : UAE.EFM.016/2566(EFM.DO.01/66)
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong, Bangkok 10260
Location : TPA On Site Calibration Laboratory
Received Order : 24 February 2026
Calibrated Date : 26 February 2026
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %
AC Line Voltage : (220 ± 22) V
Calibrated by : Warakorn Lerngagtrakul
Approved by : Kunchit
Approved Signatory
( ) Chakrit Waewwanjua
( ) Suwit Imjai
(✓) Kunchit Promprat
Issue Date : 05 March 2026

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel.0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

ilac-MRA
NSC-TISI-TIS 17025 CALIBRATION 0418

Certificate of Calibration

Certificate No.: 260311-2-BL002-26
Code No.: BL002-26

Customer Name: United Analyst and Engineering Consultant Co., Ltd.
Address: 3 Soi Udom suk 41, Sukhumvit Rd., Bang Chak, Phar Khanong, Bangkok 10260

Equipment: Electronic Balance
Manufacturer: Mettler Toledo
Model: XSR205DU
Serial No.: C009071872
Asset No. : UAE.WAO.012/2563
Building : UAE number 3 Floor : 2 Room : 208

Received Date: March 11, 2026
Date of Calibation : March 12, 2026
Calibration Conditions: Temperature 23.8 °C to 24.1 °C
Humidity 50.0 % to 59.0 %
Pressure 755.5 mmHg to 755.6 mmHg

Calibrated by: Thanachat Chatpahol
Approved by: Suwit Chotnok Signature:

Issued Date: March 16, 2026

Note : 1) The Uncertainties are for a confidence probability of approximately 95%
2) This Certificate is valid only to the item calibrated on date and place of calibration.
3) This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the United Analyst and Engineering Consultant Co.,Ltd. (UAE)

เอกสารไม่ควบคุม

United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel.0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

Equipment: Electronic Balance
Model: XSR205DU
Serial No.: C009071872
Max. Capacity: 81 g / 220 g
Calibration Date: March 12, 2026
Condition As Received: In Condition

Manufacturer: Mettler Toledo
Readability: 0 to 81 (g): 0.01 mg > 80 to 200 (g) : 01 mg
ID No.: UAE.WAO.312/2565

Condition of Equipment:

Condition of This Result of Calibration:
1. Calibration Method: This instrument was calibrated by method UAE.OP.CAL.005 In-House Method based on OIML Lec 76 - 2022
2. Reference Standards:

Reference Standard:	Model	Serial No.	Calibrated By	Certificate No.	Traceability	Due Date
Standard Weight Class F2 (OIML)	1 mg to 1 kg	C510641605	METTLER TOLEDO GmbH	C510641605	Mettler-Toledo GmbH	3 Mar 27
Standard Weight Class F2 (OIML)	1 mg to 1 kg	8749109172	AMARC	25-009359	Mettler-Toledo	21 Jan 27


Instrument	Model	Serial No.	Calibrated By	Certificate No.	Traceability	Due Date
Thermo-Hygro-Baro Meter	MHB-382SD	AK.06/57	SUCCESS	SS H 03992/68	Success Gateway	26-Nov-26
Thermo-Hygro-Baro Meter	MHB-382SD	AK.46/67	UAA	25/44494	UAA	18-Dec-26

3. This certification is traceable to SI Unit
4. This certification was certified only for the instrument we calibrated.
5. The result of calibration was found accurate as shown on date and place of calibration only.
6. Through the reference standard laboratory of Mettler Toledo (Thai) : CS10641605, SAS accreditation number SES 0082
7. Through the reference standard laboratory of AMARC 25-009359, TIS accreditation number 0158

Calibration Result:
1. Repeatability of Reading:

Nominal Value (g)	Standard Deviation of Reading (g)
80	0.000008
200*	0.000045

2. Eccentric or off-center loading
A mass of 100 g was placed and moved to various position on pan
The Balance reading obtained is given in the table.

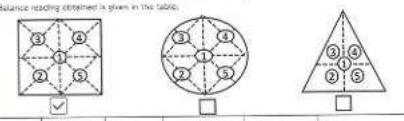

1 (g)	2 (g)	3 (g)	4 (g)	5 (g)	Maximum Difference (g)
100.0000	100.0000	100.0000	100.0000	100.0000	0.0000

c.oj

เอกสารไม่ควบคุม

United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel.0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

Equipment: Electronic Balance
Model: XSR205DU
Serial No.: C009071872
Max. Capacity: 81 g / 220 g
Calibration Date: March 12, 2026

Manufacturer: Mettler Toledo
Readability: 0 to 81 (g): 0.01 mg > 80 to 200 (g) : 01 mg
ID No.: UAE.WAO.312/2565

Calibration Result: (Continued)
Calibration Range: > 80 to 200 (g)
Calibration Adjustment: Internal Calibration

3. Error of Indication from nominal or conventional mass value: (Range: > 80 to 200 (g) ; Resolution: 0.0001 g)

Nominal Value (g)	Reference Value (g)	Indication (g)	Correction (g)	Uncertainty (± mg)	Coverage Factor k
Unload	0.0000000	0.0000	0.0000	0.02	2.25
90	90.0000910	90.0000	0.0000	0.16	2.00
100	100.0000420	100.0000	0.0000	0.16	2.00
110	110.0000750	110.0000	0.0000	0.17	2.00
120	120.0000680	120.0000	0.0001	0.18	2.00
130	130.0001010	130.0000	0.0000	0.20	2.00
140	140.0000960	140.0000	0.0001	0.21	2.00
150	150.0000790	150.0000	0.0001	0.21	2.00
160	160.0001120	160.0000	0.0001	0.23	2.00
170	170.0001050	170.0000	-0.0002	0.24	2.00
200	200.0001460	200.0000	-0.0002	0.26	2.00

4. Effect of Tare test:

Tare Load (g)	Test Load (g)	Indication (g)	Correction (g)
100	20.000028	20.0000	0.0000
	40.000054	40.0002	-0.0001
	60.000070	60.0002	-0.0001
	80.000098	80.0002	-0.0001
	100.000042	100.0000	-0.0002

Remark:
The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k, providing a level of confidence of approximately 95%

a---a-End-a---o

c.oj

เอกสารไม่ควบคุม

United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel.0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

Equipment: Electronic Balance
Model: XSR205DU
Serial No.: C009071872
Max. Capacity: 81 g / 220 g
Calibration Date: March 12, 2026

Manufacturer: Mettler Toledo
Readability: 0 to 81 (g): 0.01 mg > 80 to 200 (g) : 01 mg
ID No.: UAE.WAO.312/2565

Calibration Result: (Continued)
Calibration Range: 0 to 80 (g)
Calibration Adjustment: Internal Calibration

3. Error of Indication from nominal or conventional mass value: (Range: 0 to 81 (g) ; Resolution: 0.00001 g)

Nominal Value (g)	Reference Value (g)	Indication (g)	Correction (g)	Uncertainty (± mg)	Coverage Factor k
Unload	0.0000000	0.0000	0.0000	0.015	2.25
0.001	0.0010020	0.0010	0.00000	0.015	2.23
0.005	0.0050025	0.0050	-0.00002	0.015	2.23
0.01	0.0100005	0.0100	0.00002	0.015	2.23
0.05	0.0500003	0.0500	-0.00001	0.015	2.21
0.10	0.1000083	0.1000	-0.00001	0.015	2.20
0.50	0.5000121	0.5000	-0.00002	0.016	2.15
1	1.0000119	1.0000	0.00000	0.016	2.12
2	2.0000125	2.0000	-0.00001	0.017	2.09
5	5.0000146	5.0000	-0.00002	0.020	2.05
10	10.0000330	10.0001	-0.00002	0.023	2.00
20	20.000028	20.0001	-0.00005	0.033	2.00
30	30.000061	30.0001	-0.00004	0.051	2.00
40	40.000050	40.0001	-0.00004	0.063	2.00
50	50.000057	50.0001	-0.00005	0.064	2.00
60	60.000070	60.0001	-0.00004	0.081	2.00
80	80.000098	80.0001	-0.00001	0.11	2.00

c.oj

เอกสารไม่ควบคุม

สถาบันอาหาร
ศูนย์บริการห้องปฏิบัติการสอบเทียบ
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

Calibration Certificate

Certificate No.: 2602300-001-01
Page : 1 of 2

Equipment: CHAMBER (Hot Air Oven)
Manufacturer: MEMMERT
Model: UF55
Serial No.: B212.0411
ID No.: UAE.WAO.035/2558
Order No.: 2602300
Operation No.: 2602300-001
Date of Receipt: 11 March 2026
Date of Calibration: 11 March 2026

Customer Name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD
Address: 3 Soi Udomsuk 41, Sukhumvit Road
Bangchak, Phrakhanong, Bangkok 10260

Metrological traceability:

1. Calibration Method:
- This instrument was calibrated by inserting 9 standard thermometers into its chamber, in accordance with W TE-014, based on TLAS G-20-1/02-08 (E): Guidelines for Calibration and Checks of Temperature Controlled Enclosures.
- The temperature scale used in this laboratory is the International Temperature Scale of 1990 (ITS-90).
- All data shown below are final values, and the initial data may be obtained upon request.

2. Reference Standard Instrument

Instrument	Model/Type	Serial No./ID No.	Certificate No.	Due Date	Through
Digital Thermometer with sensor	34972A RTD	MY56002902 CH#01-206, CH#02-206	2502795-002-01	3 May 2026	NATIONAL FOOD INSTITUTE

3. This certificate is traceable to the International System of Units (SI).
4. This certificate is valid only for the instrument that was calibrated.
5. The result of this calibration was found to be accurate only on the date and at the place of calibration shown.

Calibrated by: Mr.Manas Somsak
Specialist

Approved by: (Mr.Pheraphat Tuanjit)
Manager, Division of Calibration Laboratory
Responsible for the Technical Management Team

Date of Issue: 18 March 2026

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

2008 ซอยอุดมสุข 35 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2008 Soi 35, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel. +66(0) 2422 8888 Fax +66(0) 2422 8545
nfi.or.th

เอกสารไม่ควบคุม

สถาบันพัฒนาอุตสาหกรรมอาหาร
ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

ilac-MRA
NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Certificate

Certificate No.: 2602300-001-01

Calibration Condition:

Equipment:	CHAMBER (Hot Air Oven)	Place of Calibration:	Laboratory
UUC* Resolution:	0.1 °C		UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Condition of the Item:	Normal & Good	Environment Conditions:	Ambient Temperature (29.6 ± 1.0)°C
	Without adjustment / As Found		Relative Humidity (47.8 ± 4)%
	- Time of record 1 hour 0 minute / point		Line Voltage (222 ± 3)V

Calibration Results:

Table1 : Reporting of Temperature

Calibration Point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.9 is REF)									Measurement Uncertainty (±°C)
	Std.#1	Std.#2	Std.#3	Std.#4	Std.#5	Std.#6	Std.#7	Std.#8	Std.#9	
104.0	104.22	103.87	103.99	104.17	103.66	103.58	104.22	104.17	104.09	0.53
120.0	120.21	119.78	119.86	120.13	119.63	119.58	120.24	120.20	119.96	0.73
160.0	160.27	159.77	159.73	160.31	159.61	159.63	160.35	160.25	159.84	0.99

Table 2 : Reporting of Characterization Results

UUC* Setting (°C)	UUC* Reading (°C)			Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
	Max	Min	Average			
104.0	104.0	104.0	104.0	0.05	0.44	0.75
120.0	120.0	120.0	120.0	0.05	0.43	0.79
160.0	160.0	160.0	160.0	0.07	0.93	1.56


Note
- UUC* : Unit Under Calibration
- The quoted uncertainty includes contributions from Stability and Loading Effect (20% of Temperature Uniformity).
- Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.
- Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
- Overall Variation = The difference of The maximum and minimum measured temperatures throughout observation time.

For more information, details of the sensor installation should be reported.

Fresh air Damper: [ ] Open [ ] Position; [X] Close [100% Fan speed]; [ ] Not Available

Dimension of inside chamber and sensor installation location (mm):

W x H x D	40	x 40	x 30
a x b x c	10	x 10	x 10



The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k = 2, providing a level of confidence of approximately 95 %.

---------- End of Report ----------

2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพมหานคร 10700
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel. +66(0) 2422 8688 Fax +66(0) 2422 8545
nfi.or.th

เอกสารไม่ควบคุม

สถาบันพัฒนาอุตสาหกรรมอาหาร
ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

ilac-MRA
NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Certificate

Certificate No.: 2602303-001-01

Calibration Condition:

Equipment:	CHAMBER (Incubator)	Place of Calibration:	Microbiology Laboratory
UUC* Resolution:	0.1 °C		UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Condition of the Item:	Normal & Good	Environment Conditions:	Ambient Temperature (17.2 ± 1)°C
	Without adjustment / As Found		Relative Humidity (51.5 ± 4)%
	- Time of record 1 hour 0 minute / point		Line Voltage (229 ± 2)V

Calibration Results:

Table1 : Reporting of Temperature

Calibration Point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.9 is REF)									Measurement Uncertainty (±°C)
	Std.#1	Std.#2	Std.#3	Std.#4	Std.#5	Std.#6	Std.#7	Std.#8	Std.#9	
35.0	35.01	34.94	35.00	35.15	35.26	34.99	34.78	34.83	35.02	0.28

Table 2 : Reporting of Characterization Results

UUC* Setting (°C)	UUC* Reading (°C)			Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
	Max	Min	Average			
35.0	35.0	35.0	35.0	0.026	0.24	0.53


Note
- UUC* : Unit Under Calibration
- The quoted uncertainty includes contributions from Stability and Loading Effect (20% of Temperature Uniformity).
- Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.
- Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
- Overall Variation = The difference of The maximum and minimum measured temperatures throughout observation time.

For more information, details of the sensor installation should be reported.

Fresh air Damper: [ ] Open [ ] Position; [X] Close [100% Fan speed]; [ ] Not Available

Dimension of inside chamber and sensor installation location (mm):

W x H x D	64	x 48	x 50
a x b x c	10	x 10	x 10



The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k = 2, providing a level of confidence of approximately 95 %.

---------- End of Report ----------

2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพมหานคร 10700
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel. +66(0) 2422 8688 Fax +66(0) 2422 8545
nfi.or.th

เอกสารไม่ควบคุม

สถาบันพัฒนาอุตสาหกรรมอาหาร
ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

ilac-MRA
NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Certificate

Certificate No.: 2602303-001-01

Equipment:	CHAMBER (Incubator)		
Manufacturer:	MEMMERT	Customer Name:	UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Model:	IPP260	Address:	3 Soi Udomsuk 41, Sukhumvit Road,
Serial No.:	V615.0187		Bangkok, Prakanong, Bangkok 10260
ID No.:	UAE.MIC.003/2559		
Order No.:	2602303		
Operation No.:	2602303-001		
Date of Receipt:	11 March 2026		
Date of Calibration:	11 March 2026		

Metrological traceability:

1. Calibration Method:
   - This instrument was calibrated by inserting 9 standard thermometers into its chamber, in accordance with W-TE-014 based on TLAS G 20-1/02-08 (E): Guidelines for Calibration and Checks of Temperature Controlled Enclosures.
   - The temperature scale used in this laboratory is the International Temperature Scale of 1990 (ITS-90).
   - All data shown below are final values, and the initial data may be obtained upon request.
2. Reference Standard Instrument:

Instrument	Model/Type	Serial No./ID No.	Certificate No.	Due Date	Through
Digital Thermometer with sensor	DAQ972A RTD	MY59008864 CH#01-09/ RTD#01-09	2502544-001-01	28 March 2026	NATIONAL FOOD INSTITUTE

3. This certificate is traceable to the International System of Units (SI).
4. This certificate is valid only for the instrument that was calibrated.
5. The result of this calibration was found to be accurate only on the date and at the place of calibration shown.

Calibrated by: Mr.Nuttapol Niyomchat, Specialist

Approved by: (Mr.Pheraphat Tuanjit)
Manager, Division of Calibration Laboratory
Responsible for the Technical Management Team

Date of Issue: 19 March 2026

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพมหานคร 10700
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel. +66(0) 2422 8688 Fax +66(0) 2422 8545
nfi.or.th

เอกสารไม่ควบคุม

สถาบันพัฒนาอุตสาหกรรมอาหาร
ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

ilac-MRA
NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Certificate

Certificate No.: 2602303-006-01

Equipment:	CHAMBER (Incubator)		
Manufacturer:	BINDER	Customer Name:	UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Model:	KB 400	Address:	3 Soi Udomsuk 41, Sukhumvit Road,
Serial No.:	20200000015535		Bangkok, Prakanong, Bangkok 10260
ID No.:	UAE.MIC.016/2564		
Order No.:	2602303		
Operation No.:	2602303-006		
Date of Receipt:	11 March 2026		
Date of Calibration:	11 March 2026		

Metrological traceability:

1. Calibration Method:
   - This instrument was calibrated by inserting 8 standard thermometers into its chamber, in accordance with W-TE-014 based on TLAS G 20-1/02-08 (E): Guidelines for Calibration and Checks of Temperature Controlled Enclosures.
   - The temperature scale used in this laboratory is the International Temperature Scale of 1990 (ITS-90).
   - All data shown below are final values, and the initial data may be obtained upon request.
2. Reference Standard Instrument:

Instrument	Model/Type	Serial No./ID No.	Certificate No.	Due Date	Through
Digital Thermometer with sensor	DAQ972A RTD	MY59008864 CH#01-09/ RTD#01-09	2502544-001-01	28 March 2026	NATIONAL FOOD INSTITUTE

3. This certificate is traceable to the International System of Units (SI).
4. This certificate is valid only for the instrument that was calibrated.
5. The result of this calibration was found to be accurate only on the date and at the place of calibration shown.

Calibrated by: Mr.Nuttapol Niyomchat, Specialist

Approved by: (Mr.Pheraphat Tuanjit)
Manager, Division of Calibration Laboratory
Responsible for the Technical Management Team

Date of Issue: 19 March 2026

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพมหานคร 10700
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel. +66(0) 2422 8688 Fax +66(0) 2422 8545
nfi.or.th

เอกสารไม่ควบคุม

nfi สถาบันอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

Calibration Certificate

Certificate No.: 2602303-006-01
Page : 2 of 2

Calibration Condition:

Equipment:	CHAMBER (Incubator)	Place of Calibration:	Microbiology Laboratory
UUC* Resolution	0.1 °C		UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD
Condition of the Item:	Normal & Good	Environment Conditions:	Ambient Temperature (17.2 ± 1) °C
	Without adjustment / As Found		Relative Humidity (51.5 ± 4) %
	Time of record : 1 hour 0 minute / point		Line Voltage (229 ± 2) V

Calibration Results:

Table1 : Reporting of Temperature

Calibration Point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.9 is REF)									Measurement Uncertainty (±°C)
	Std.#1	Std.#2	Std.#3	Std.#4	Std.#5	Std.#6	Std.#7	Std.#8	Std.#9	
35.0	34.78	34.86	34.91	34.93	35.22	35.21	35.22	35.12	34.83	0.08

Table 2 : Reporting of Characterization Results

UUC* Setting (°C)	UUC* Reading (°C)			Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
	Max	Min	Average			
35.0	35.0	35.0	35.0	0.034	0.39	0.52

Note
- UUC* : Unit Under Calibration
-The quoted uncertainty includes contributions from "Stability" and "Loading Effect (20% of Temperature Uniformity)".
- Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.
- Uniformity = The maximum difference of measured temperatures of any sensors and the measured temperature at the reference location which are observed at the same time.
- Overall Variation = The difference of The maximum and minimum measured temperatures throughout observation time.

For more information, details of the sensor installation should be reported.

Fresh air Damper: - Open, - Position
S - Close, 100% Fan speed
- Not Available

Dimension of mold chamber (inc. sensor installation location) (cm)

W x H x D	65	x	125	x	48
a x b x c	10	x	10	x	10



The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k = 2, providing a level of confidence of approximately 95 %.

End of Report

F-CS-009 Revision: 02 Date: 01-10-68

อุตสาหกรรมอาหาร 36 ถนนอรุณอมรินทร์ แขวงบางยี่เรือ เขตธนบุรี กรุงเทพมหานคร 10600
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok, 10700, Thailand
Tel. +66(0) 2422 8888 Fax +66(0) 2422 8845

เอกสารไม่ควบคุม

UAE United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel.0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

Certificate No.: 260311-2-BL001-26
Code No.: BL001-26
Page: 2 of 4

Equipment:	Electronic Balance	Manufacturer:	Mettler Toledo
Model:	XSR205DU	Readability:	0 to 81 (g): 0.01 mg , > 80 to 220 (g): 0.1 mg
Serial No.:	C210685394	ID No.:	UAE.WAO.010/2565
Max. Capacity:	81 g / 220 g		
Calibration Date:	March 12, 2026		
Condition As-Received:	In Condition		

Condition of Equipment:

Condition of This Result of Calibration:

1. Calibration Method: This instrument was calibrated by method UAE.QT-CAL-005 in-House Method based on OIML Lab 11 : 2002
2. Reference Standards:

Reference Standard:	Model	Serial No.	Calibrated By	Certificate No.	Traceability	Due Date
Standard Weight Class E2 (OIML)	1 mg to 1 kg	C3.0641.005	METTLER TOLEDO GmbH	C3.0641.005	METTLER TOLEDO GmbH	3-Mar-27
Standard Weight Class E2 (OIML)	1 mg to 1 kg	B749.05122	AMARC	23-009359	AMARC	23-Jan-27

Instrument	Model	Serial No.	Calibrated By	Certificate No.	Traceability	Due Date
Thermo-Hygro-Baro Meter	WMB-38250	A4.44A32	SUCCESS	SS-H.009992/68	Success Gateway	26 Nov 26
Thermo-Hygro-Baro Meter	WMB-38250	A4.44A57	TPA	2594644	TPA	18 Dec 26

3. This certification is traceable to SI Unit.
4. This certification was certified only for the instruments we calibrated.
5. This result of calibration was found accurate as shown on date and place of calibration only.
6. through the reference standard laboratory of Mettler-Toledo GmbH CS.0641.005, SAS accreditation number: SCS 0032
7. Through the reference standard laboratory of AMARC 23-009359, TISI accreditation number 0032


Calibration Result:

1. Repeatability of Reading:

Nominal Value (g)	Standard Deviation of Reading (g)
80	0.000019
200*	0.000055

2. Eccentric or off-center loading

A mass of 100 g was placed and moved to various position on pan.
The Balance reading obtained is given in the table.

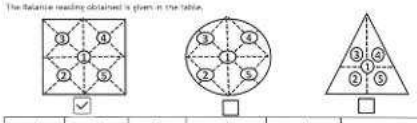

1 (g)	2 (g)	3 (g)	4 (g)	5 (g)	Maximum Difference (g)
100.0002	100.0002	100.0003	100.0004	100.0003	0.0001

เอกสารไม่ควบคุม

UAE United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel.0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

Certificate of Calibration

Certificate No.: 260311-2-BL001-26
Code No.: BL001-26
Page: 1 of 4

Customer Name:	United Analyst and Engineering Consultant Co., Ltd.			
Address:	3 Soi Udom suk 41, Sukhumvit Rd., Bang Chak, Phar Khanong, Bangkok 10260			
Equipment:	Electronic Balance			
Manufacturer:	Mettler Toledo			
Model:	XSR205DU			
Serial No.:	C210685394			
Asset No. :	UAE.WAO.010/2565			
Building :	UAE number 3	Floor : 2	Room : 208	
Received Date:	March 11, 2026			
Date of Calibation :	March 12, 2026			
Calibration Conditions:	Temperature	23.0 °C	to	23.6 °C
	Humidity	51.5 %	to	54.4 %
	Pressure	755.7 mmHg	to	757.9 mmHg
Calibrated by:	Thanachat Chatpahol			
Approved by:	Suwit Chotnok	Signature:		
Issued Date:	March 16, 2026			

Note : 1) The Uncertainties are for a confidence probability of approximately 95%
2) This Certificate is valid only to the item calibrated on date and place of calibration.
3) This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the United Analyst and Engineering Consultant Co.,Ltd. (UAE).

เอกสารไม่ควบคุม

UAE United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel.0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

Certificate No.: 260311-2-BL001-26
Code No.: BL001-26
Page: 3 of 4

Equipment:	Electronic Balance	Manufacturer:	Mettler Toledo
Model:	XSR205DU	Readability:	0 to 81 (g): 0.01 mg , > 80 to 200 (g) : 0.1 mg
Serial No.:	C210685394	ID No.:	UAE.WAO.010/2565
Max. Capacity:	81 g / 220 g		
Calibration Date:	March 12, 2026		

Calibration Result: (Continued)
Calibration Range: 0 to 80 (g)
Calibration Adjustment: Internal Calibration

3. Error of indication from nominal or conventional mass value: (Range: 0 to 81 (g) ; Resolution: 0.00001 g)

Nominal Value (g)	Reference Value (g)	Indication (g)	Correction (g)	Uncertainty (± mg)	Coverage Factor k
Unload	0.0000000	0.00000	0.00000	0.032	2.65
0.001	0.0010020	0.00161	0.00000	0.032	2.65
0.005	0.0050025	0.00501	-0.00001	0.032	2.65
0.01	0.0100005	0.01001	-0.00001	0.032	2.65
0.05	0.0500003	0.05001	-0.00001	0.032	2.65
0.10	0.1000083	0.10000	0.00001	0.033	2.65
0.50	0.5000121	0.50001	0.00000	0.033	2.65
1	1.0000119	1.00003	-0.00002	0.032	2.52
2	2.0000125	2.00003	-0.00002	0.033	2.52
5	5.0000146	5.00003	-0.00002	0.033	2.32
10	10.0000330	10.00006	-0.00003	0.034	2.21
20	20.000028	20.00006	-0.00003	0.041	2.07
30	30.000061	30.00017	-0.00011	0.055	2.00
40	40.000054	40.00021	-0.00016	0.066	2.00
50	50.000037	50.00023	-0.00019	0.068	2.00
60	60.000070	60.00029	-0.00022	0.084	2.00
80	80.000098	80.00039	-0.00030	0.12	2.00

เอกสารไม่ควบคุม

United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel.0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

Equipment: Electronic Balance
Manufacturer: Mettler Toledo
Model: XSR285DU
Readability: ≤ 81 (g): 0.01 mg , > 81 to 200 (g): 0.1 mg
Serial No.: C210685394
ID No.: UAE.WAS.010/2565
Max. Capacity: 81 g / 220 g
Calibration Date: March 12, 2026

Calibration Result: (Continued)
Calibration Range: > 81 to 200 (g)
Calibration Adjustment: Internal Calibration

3. Error of Indication from nominal or conventional mass value: (Range: > 81 - 220 (g) , Resolution: 0.0001 g)

Nominal Value (g)	Reference Value (g)	Indication (g)	Correction (g)	Uncertainty (± mg)	Coverage Factor k
Unload	0.0000000	0.0000	0.0000	0.032	2.65
90	90.0000910	90.0004	-0.0003	0.16	2.00
100	100.0000420	100.0003	-0.0003	0.16	2.00
110	110.0000750	110.0004	-0.0003	0.18	2.00
120	120.0000680	120.0004	-0.0003	0.19	2.00
130	130.0001010	130.0005	-0.0004	0.20	2.00
140	140.0000960	140.0004	-0.0003	0.21	2.00
150	150.0000790	150.0005	-0.0004	0.22	2.00
160	160.0001120	160.0004	-0.0003	0.23	2.00
170	170.0001050	170.0003	-0.0002	0.24	2.00
200	200.0001460	200.0001	0.0000	0.26	2.00

4. Effect of Tare test:

Tare Load (g)	Test Load (g)	Indication (g)	Correction (g)
100	20.000028	20.0001	0.0000
	40.000054	40.0001	0.0000
	60.000070	60.0000	0.0001
	80.000098	80.0000	0.0001
	100.000109	100.0000	0.0001

Remark: -
The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k, providing a level of confidence of approximately 95%

o---o-End-o---o

เอกสารไม่ควบคุม

United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel.0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

Equipment: Electronic Balance
Manufacturer: Mettler Toledo
Model: AB204-S/FACT
Readability: 0.0001 g
Serial No.: 1129361010
ID No.: UAE.WAS.002/2552
Max. Capacity: 220 g
Calibration Date: April 3, 2026
Condition As-Received: In Condition

Condition of Equipment:
Condition of This Result of Calibration:
1. Calibration Method: This instrument was calibrated by internal UAE.PCAL-006 (Release Method based on UKAS Lab 34 : 2022)
2. Reference Standards:

Reference Standard:	Model	Serial No.	Calibrated By	Certificate No.	Traceability	Due Date
Standard Weight Class E2 (OIML)	1 mg to 1 kg	C310681605	METTLER TOLEDO (China)	C310681605	Mettler Toledo	5-Mar-27


Instrument	Model	Serial No.	Calibrated By	Certificate No.	Traceability	Due Date
Thermo-Hygro Baro Meter	MHB-382SD	AK466547	SATTRIS	SCH-00002/68	Success Gateway	26-Nov-26
Thermo-Hygro Baro Meter	MHB-382SD	AK466547	TPA	25P0468	TPA	18-Dec-26

3. This certification is traceable to SI Unit
4. This certification was certified only for the instrument we calibrated
5. This result of calibration was found accurate as show on date and place of calibration only.
6. Through the reference standard laboratory of Mettler-Toledo (Thai) Co.,Ltd.,ISO accreditation number SCL 0032

Calibration Result:
1. Repeatability of Reading:

Nominal Value (g)	Standard Deviation of Reading (g)
200*	0.00010

2. Eccentric or off-center loading
A mass of 100 g was placed and moved to various position on pan
The Balance reading obtained is given in the table.

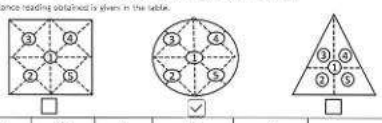

1 (g)	2 (g)	3 (g)	4 (g)	5 (g)	Maximum Difference (g)
100.0025	100.0022	100.0022	100.0029	100.0030	0.0008

เอกสารไม่ควบคุม

United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel.0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

Certificate of Calibration

Certificate No.: 260318-1-BL007-26
Code No.: BL007-26
Page: 1 of 3

Customer Name: United Analyst and Engineering Consultant Co., Ltd.
Address: 3 Soi Udom suk 41, Sukhumvit Rd., Bang Chak, Phar Khanong, Bangkok 10260

Equipment: Electronic Balance
Manufacturer: Mettler Toledo
Model: AB204-S/FACT
Serial No.: 1129361010
Asset No. : UAE.WAS.002/2552
Building : UAE No.3 Floor : 1 Room : 107

Received Date: April 2, 2026
Date of Calibation : April 3, 2026
Calibration Conditions: Temperature start 21.9 °C end 22.1 °C
Humidity start 60.6 % end 60.1 %
Pressure start 756.6 mmHg end 755.1 mmHg

Calibrated by: Thanachat Chatpahol

Approved by: Suwit Chotnok Signature:

Issued Date: April 7, 2026

Note : 1) The Uncertainties are for a confidence probability of approximately 95%
2) This Certificate is valid only to the item calibrated on date and place of calibration.
3) This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the United Analyst and Engineering Consultant Co.,Ltd. (UAE)

เอกสารไม่ควบคุม

United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Tel.0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

Equipment: Electronic Balance
Manufacturer: Mettler Toledo
Model: AB204-S/FACT
Readability: 0.0001 g
Serial No.: 1129361010
ID No.: UAE.WAS.002/2552
Max. Capacity: 220 g
Calibration Date: April 3, 2026

Calibration Result: (Continued)
Calibration Range: 0 - 200 g
Calibration Adjustment: Internal Calibration

3. Error of Indication from nominal or conventional mass value:

Nominal Value (g)	Reference Value (g)	Indication (g)	Correction (g)	Uncertainty (± mg)	Coverage Factor k
Unload	0.0000000	0.0000	0.0000	0.17	2.37
0.01	0.0100085	0.0099	0.0001	0.17	2.32
0.05	0.0500085	0.0499	0.0001	0.17	2.32
0.1	0.1000085	0.0999	0.0001	0.17	2.32
0.5	0.5000121	0.5000	0.0000	0.17	2.32
1.0	1.0000119	1.0000	0.0000	0.17	2.32
10.0	10.000033	10.0003	-0.0003	0.17	2.32
40.0	40.000054	40.0010	-0.0010	0.18	2.23
50.0	50.000037	50.0013	-0.0012	0.18	2.23
80.0	80.000098	80.0020	-0.0019	0.19	2.11
100.0	100.000042	100.0025	-0.0024	0.20	2.10
120.0	120.000068	120.0028	-0.0027	0.22	2.06
150.0	150.000079	150.0035	-0.0035	0.24	2.04
160.0	160.000112	160.0036	-0.0035	0.25	2.03
200.0	200.000146	200.0049	-0.0047	0.28	2.00

4. Effect of Tare test:

Tare Load (g)	Test Load (g)	Indication (g)	Correction (g)
100	20.000028	20.0004	-0.0005
	40.000054	40.0009	-0.0008
	60.000070	60.0013	-0.0012
	80.000098	80.0017	-0.0016
	100.000042	100.0021	-0.0021

Remark: -
The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k, providing a level of confidence of approximately 95%

o---o-End-o---o

เอกสารไม่ควบคุม

HANNA instruments

Hanna Instruments (Thailand) Ltd.

410/67-68 Soi Ratchadapisek 24, Ratchadapisek Rd., Samsen-nok, Huaykwang, Bangkok 10310 Tel: 0-2541-4199 Fax: 0-2541-4198

AC-3061

Certificate No. : C26030163

Page : 1 of 2

CERTIFICATE OF CALIBRATION

Equipment	: COD Test Tube Heater		
Meter Model	: HI839800-02	Serial No.	: 06480019101
Tube Heater Capacity	: 25 Vial Capacity	Resolution	: 0.1 °C
Temperature Range	: (-10 to 160)°C	Temperature of Reaction	: 150°C
Manufacturer	: Hanna Instruments	Made in	: Romania
Condition As-Received	: Used Product	Reference	: RE260497
Ambient Temperature	: (25 ± 2)°C	Relative Humidity	: (50 ± 15)% RH
Customer name	: United Analyst and Engineering Consultant Co., Ltd. 3 Soi Udomsuk 41, Sukhumvit Rd., Bangchak Phrakhanong, Bangkok 10260		
Received date	: 12 March 2026		
Calibrate date	: 17 March 2026		
Issue date	: 18 March 2026		
Calibrated Location	: Hanna Instruments (Thailand) Ltd.		
Calibration Procedure	: This calibrator was conducted by using in-house: calibration procedure CP-04 by using certified reference standard instruments.		

Calibrated by : Mr. Pichit Petthong

Approved by : (Mr. Anan Suwanchaisakul) Authorized Signatory

HANNA instruments (Thailand) Limited

This certificate was certified only for the instrument we calibrated. This result of calibration was found accurate on date and place of calibration only.

This certificate may not be reproduced other than in full, except with the prior written approval of [illegible] Ltd.

เอกสารไม่ควบคุม

Form ER 5/1/2026

DQE Services Co.,Ltd.

DQE Services 32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230

Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

CERTIFICATE OF CALIBRATION

Certificate No. : SP26-014 Page 1 of 5

Customer : United Analyst and Engineering Consultant Co.,Ltd. (Head Office)

Address : 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Location of calibration : Instrument room (207)

Equipment : UV-Vis Spectrophotometer

Manufacturer : HITACHI

Model : U-5100

Serial No. : 23A4-008

ID No. : UAE.WAS.010/2567

Received Date : 18 May 2026

Calibration Date : 18 May 2026

Issue Date : 21 May 2026

Condition Instrument : Good

Calibrated by : (Mr.Pacit Mathavorn) Calibration Engineer

Approved by : (Ms.Chonticha Sangngern) Quality Manager

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the DQE Services Co., Ltd.

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

HANNA instruments

Certificate No. : C26030163

Page : 2 of 2

Condition of this calibration result :

Reference standard instrument : This Certification is traceable to the SI Unit maintained through:

Instrument	Model	Serial No.	Certificate No.	Traceable
Digital Thermo-Hygrometer	HT-771SD	AI.07155	26H106	Technology Promotion Association (Thailand-Japan).
Data Acquisition Switch Unit	34970A	MY44065265	WK2507-171-1	WK Electric Co., Ltd.

Calibration Result :

Measurement Temperature Source Accuracy for COD Reactor.

Capacity	Nominal Value	Average Value	Error	Uncertainty (±)
25 Vials	150.0 °C	150.1 °C	0.1 °C	0.53 °C

Unit : °C

(1A)	(2A)	(3A)	(4A)	(5A)
149.7	149.7	150.1	150.4	150.4
(1B)	(2B)	(3B)	(4B)	(5B)
150.4	150.3	150.2	150.2	150.1
(1C)	(2C)	(3C)	(4C)	(5C)
149.9	150.2	150.0	150.2	149.9
(1D)	(2D)	(3D)	(4D)	(5D)
150.2	150.2	150.0	150.0	150.0
(1E)	(2E)	(3E)	(4E)	(5E)
150.1	149.8	150.2	150.2	149.8

Figure: Shows the location of the temperature source.

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k=2, providing a level of confidence of approximately 95%

** End of certificate **

เอกสารไม่ควบคุม

Form ER 5/1/2026

DQE Services Co.,Ltd.

DQE Services 32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230

Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP26-014 Page 2 of 5

Environment Condition : Ambient Temperature 25 ± 5 °C

Relative humidity 55 ± 20 %RH

Calibration method : In-house method CP-01 Based on ASTM E275-08

Certified Reference Materials :

Material	Serial No.	Certificate No.	Due date
Absobance Standard set	25760	136858	5 November 2027
Absobance Standard set	25757	136848	5 November 2027
Wavelength Standard set	25806	136824	5 November 2027
Wavelength Standard set	25758	136827	5 November 2027

Traceability : This certification is traceable to the International System of Unit maintained at National - Institute of Standards and Technology (NIST) through Starna Scientific Limited

Spectral Band Width of UUC : 5.0 nm.

Scan Speed of UUC : 40

Scan Interval of UUC : 0.1 nm.

Resolution of UUC : Photometric 0.001 Abs.

Wavelength 0.1 nm.

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP26-014

Calibration Results : Without adjustment

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
420	0.0000	0.000	0.0000	0.0028	2.00
	0.5772	0.574	0.0032	0.0031	2.00
	1.0478	1.043	0.0048	0.0029	2.00
	2.1879	2.182	0.0059	0.0082	2.00
440	0.0000	0.000	0.0000	0.0028	2.00
	0.5581	0.556	0.0021	0.0034	2.00
	1.0224	1.020	0.0024	0.0035	2.00
	2.1227	2.121	0.0017	0.0079	2.00
465	0.0000	0.000	0.0000	0.0028	2.00
	0.5225	0.518	0.0045	0.0029	2.00
	0.9628	0.961	0.0018	0.0028	2.00
	1.9744	1.974	0.0004	0.0070	2.00
546.1	0.0000	0.000	0.0000	0.0028	2.00
	0.5174	0.514	0.0034	0.0031	2.00
	0.9990	0.996	0.0030	0.0033	2.00
	1.9953	1.995	0.0003	0.0087	2.00
590	0.0000	0.000	0.0000	0.0028	2.00
	0.5508	0.549	0.0018	0.0030	2.00
	1.0801	1.078	0.0021	0.0029	2.00
	2.0356	2.028	0.0076	0.0079	2.00
635	0.0000	0.000	0.0000	0.0028	2.00
	0.5579	0.558	-0.0001	0.0031	2.00
	1.0512	1.050	0.0012	0.0029	2.00
	1.9257	1.923	0.0027	0.0083	2.00

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP26-014

Wavelength Accuracy :

CRMs Values (nm.)	UUC Reading (nm.)	Correction (nm.)	Uncertainty (nm.)	Coverage factor k
241.00	240.3	0.70	0.18	2.00
279.30	278.9	0.40	0.18	2.00
288.90	288.2	0.70	0.18	2.00
334.50	333.8	0.70	0.18	2.00
361.40	360.7	0.70	0.18	2.00
418.40	417.9	0.50	0.18	2.00
447.20	446.6	0.60	0.18	2.00
459.30	459.4	-0.10	0.18	2.00
537.00	536.5	0.50	0.18	2.00
638.00	637.3	0.70	0.18	2.00
441.29	440.6	0.69	0.18	2.00
479.88	479.2	0.68	0.18	2.00
513.75	513.0	0.75	0.18	2.00
528.59	528.1	0.49	0.18	2.00
575.10	574.5	0.60	0.18	2.00
585.56	585.0	0.56	0.20	2.00
684.70	684.2	0.50	0.18	2.00
740.51	739.9	0.61	0.20	2.00
747.61	747.0	0.61	0.18	2.00
807.04	806.5	0.54	0.18	2.00
879.68	879.0	0.68	0.18	2.00

Remark : - UUC = Unit Under Calibration
- N/A = Not Available
- The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor *k*, which for a normal distribution corresponds to a coverage probability of approximately 95%
- * Indicates non TISI accredited

- End of Certificate -

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP26-014

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
235	0.0000	0.000	0.0000	0.0050	2.00
	0.7455	0.744	0.0015	0.0056	2.00
257	0.0000	0.000	0.0000	0.0050	2.00
	0.8656	0.863	0.0026	0.0059	2.00
313	0.0000	0.000	0.0000	0.0050	2.00
	0.2910	0.290	0.0010	0.0051	2.00
350	0.0000	0.000	0.0000	0.0050	2.00
	0.6414	0.640	0.0014	0.0055	2.00

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

CERTIFICATE OF CALIBRATION

Certificate No. : SP26-013

Customer : United Analyst and Engineering Consultant Co.,Ltd. (Head Office)

Address : 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Location of calibration : Instrument room (207)

Equipment : UV-Vis Spectrophotometer

Manufacturer : Agilent Technologies

Model : Cary 60

Serial No. : MY15410009

ID No. : UAE.WAT.020/2558

Received Date : 18 May 2026

Calibration Date : 18 May 2026

Issue Date : 21 May 2026

Condition Instrument : Good

Calibrated by : (Mr.Pacit Mathavorn)
Calibration Engineer

Approved by : (Ms.Chontiba Sangngern)
Quality Manager

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the DQE Services Co., Ltd.

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP26-013

Environment Condition : Ambient Temperature 25 ± 5 °C

Relative humidity 55 ± 20 %RH

Calibration method : In-house method CP-01 Based on ASTM E275-08

Certified Reference Materials :

Material	Serial No.	Certificate No.	Due date
Absobance Standard set	25760	136858	5 November 2027
Absobance Standard set	25757	136848	5 November 2027
Wavelength Standard set	25806	136824	5 November 2027
Wavelength Standard set	25758	136827	5 November 2027

Traceability : This certification is traceable to the International System of Unit maintained at National - Institute of Standards and Technology (NIST) through Starna Scientific Limited

Spectral Band Width of UUC : 1.5 nm.

Scan Speed of UUC : 60 nm/min

Scan Interval of UUC : 0.15 nm.

Resolution of UUC : Photometric 0.000 Abs.

Wavelength 0.1 nm.

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP26-013

Calibration Results : Without adjustment

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
420	0.0000	0.0001	-0.0001	0.0028	2.00
	0.5772	0.5731	0.0041	0.0031	2.00
	1.0478	1.0427	0.0051	0.0029	2.00
	2.1879	2.1782	0.0097	0.0075	2.00
440	0.0000	0.0000	0.0000	0.0028	2.00
	0.5581	0.5574	0.0007	0.0034	2.00
	1.0224	1.0210	0.0014	0.0035	2.00
	2.1227	2.1159	0.0068	0.0083	2.00
465	0.0000	0.0000	0.0000	0.0028	2.00
	0.5225	0.5184	0.0041	0.0029	2.00
	0.9628	0.9603	0.0025	0.0028	2.00
	1.9744	1.9698	0.0046	0.0073	2.00
546.1	0.0000	0.0000	0.0000	0.0028	2.00
	0.5174	0.5150	0.0024	0.0031	2.00
	0.9990	0.9964	0.0026	0.0033	2.00
	1.9953	1.9884	0.0069	0.0085	2.00
590	0.0000	0.0000	0.0000	0.0028	2.00
	0.5508	0.5491	0.0017	0.0030	2.00
	1.0801	1.0781	0.0020	0.0029	2.00
	2.0356	2.0274	0.0082	0.0078	2.00
635	0.0000	0.0000	0.0000	0.0028	2.00
	0.5579	0.5570	0.0009	0.0031	2.00
	1.0512	1.0491	0.0021	0.0029	2.00
	1.9257	1.9201	0.0056	0.0079	2.00

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP26-013

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
235	0.0000	0.0000	0.0000	0.0050	2.00
	0.7455	0.7457	-0.0002	0.0056	2.00
257	0.0000	0.0000	0.0000	0.0050	2.00
	0.8656	0.8669	-0.0013	0.0059	2.00
313	0.0000	0.0000	0.0000	0.0050	2.00
	0.2910	0.2907	0.0003	0.0051	2.00
350	0.0000	0.0000	0.0000	0.0050	2.00
	0.6414	0.6414	0.0000	0.0055	2.00

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP26-013

Wavelength Accuracy :

CRMs Values (nm.)	UUC Reading (nm.)	Correction (nm.)	Uncertainty (nm.)	Coverage factor k
241.70	241.6	0.10	0.18	2.00
279.44	279.2	0.24	0.18	2.00
287.71	287.6	0.11	0.18	2.00
334.02	333.5	0.52	0.18	2.00
360.89	360.2	0.69	0.18	2.00
418.53	417.8	0.73	0.18	2.00
445.82	445.2	0.62	0.18	2.00
453.67	453.0	0.67	0.18	2.00
459.99	459.6	0.39	0.18	2.00
536.52	536.4	0.12	0.18	2.00
638.00	638.2	-0.20	0.18	2.00
431.22	430.5	0.72	0.18	2.00
472.66	472.2	0.46	0.18	2.00
513.39	513.3	0.09	0.18	2.00
528.90	528.7	0.20	0.18	2.00
572.99	573.6	-0.61	0.18	2.00
585.19	585.7	-0.51	0.20	2.00
684.50	684.5	0.00	0.18	2.00
741.02	741.2	-0.18	0.20	2.00
748.56	749.0	-0.44	0.18	2.00
807.02	806.8	0.22	0.18	2.00
879.41	879.4	0.01	0.18	2.00

Remark : - UUC = Unit Under Calibration

- N/A = Not Avaiable
- The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor *k*, which for a normal distribution corresponds to a coverage probability of approximately 95%
- * Indicates non TISI accredited

- End of Certificate -

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

CERTIFICATE OF CALIBRATION

Certificate No. : SP26-012

Customer : United Analyst and Engineering Consultant Co.,Ltd. (Head Office)

Address : 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Location of calibration : Instrument room (207)

Equipment : UV-Vis Spectrophotometer

Manufacturer : HITACHI

Model : U-2900

Serial No. : 21E22-009

ID No. : UAE.WAT.051/2564

Received Date : 18 May 2026

Calibration Date : 18 May 2026

Issue Date : 21 May 2026

Condition Instrument : Good

Calibrated by : (Mr.Pacit Mathavorn)
Calibration Engineer

Approved by : (Ms.Chonticha Sangngern)
Quality Manager

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the DQE Services Co., Ltd.

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP26-012

Environment Condition : Ambient Temperature 25 ± 5 °C

Relative humidity 55 ± 20 %RH

Calibration method : In-house method CP-01 Based on ASTM E275-08

Certified Reference Materials :

Material	Serial No.	Certificate No.	Due date
Absobance Standard set	25760	136858	5 November 2027
Absobance Standard set	25757	136848	5 November 2027
Wavelength Standard set	25806	136824	5 November 2027
Wavelength Standard set	25758	136827	5 November 2027

Traceability : This certification is traceable to the International System of Unit maintained at National - Institute of Standards and Technology (NIST) through Starna Scientific Limited

Spectral Band Width of UUC : 1.5 nm.

Scan Speed of UUC : 200 nm/min

Scan Interval of UUC : 0.1 nm.

Resolution of UUC : Photometric 0.001 Abs.

Wavelength 0.1 nm.

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP26-012

Calibration Results : Without adjustment

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
420	0.0000	0.000	0.0000	0.0028	2.00
	0.5772	0.575	0.0022	0.0031	2.00
	1.0478	1.043	0.0048	0.0029	2.00
	2.1879	2.197	-0.0091	0.0075	2.00
440	0.0000	0.000	0.0000	0.0028	2.00
	0.5581	0.558	0.0001	0.0034	2.00
	1.0224	1.022	0.0004	0.0035	2.00
	2.1227	2.131	-0.0083	0.0079	2.00
465	0.0000	0.000	0.0000	0.0028	2.00
	0.5225	0.518	0.0045	0.0029	2.00
	0.9628	0.961	0.0018	0.0028	2.00
	1.9744	1.981	-0.0066	0.0070	2.00
546.1	0.0000	0.000	0.0000	0.0028	2.00
	0.5174	0.515	0.0024	0.0031	2.00
	0.9990	0.997	0.0020	0.0033	2.00
	1.9953	1.995	0.0003	0.0084	2.00
590	0.0000	0.000	0.0000	0.0028	2.00
	0.5508	0.549	0.0018	0.0030	2.00
	1.0801	1.079	0.0011	0.0029	2.00
	2.0356	2.036	-0.0004	0.0079	2.00
635	0.0000	0.000	0.0000	0.0028	2.00
	0.5579	0.558	-0.0001	0.0031	2.00
	1.0512	1.050	0.0012	0.0029	2.00
	1.9257	1.928	-0.0023	0.0079	2.00

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP26-012

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
235	0.0000	0.000	0.0000	0.0050	2.00
	0.7455	0.742	0.0035	0.0056	2.00
257	0.0000	0.000	0.0000	0.0050	2.00
	0.8656	0.860	0.0056	0.0059	2.00
313	0.0000	0.000	0.0000	0.0050	2.00
	0.2910	0.288	0.0030	0.0051	2.00
350	0.0000	0.000	0.0000	0.0050	2.00
	0.6414	0.635	0.0064	0.0055	2.00

เอกสารไม่ควบคุม

DQE Services Co.,Ltd.
32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Ladprao, Bangkok 10230
Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com

REPORT OF CALIBRATION

Certificate No. : SP26-012

Wavelength Accuracy :

CRMs Values (nm.)	UUC Reading (nm.)	Correction (nm.)	Uncertainty (nm.)	Coverage factor k
241.72	241.3	0.42	0.18	2.00
279.45	279.0	0.45	0.18	2.00
287.81	287.4	0.41	0.18	2.00
334.06	333.8	0.26	0.18	2.00
360.93	360.5	0.43	0.18	2.00
418.59	418.0	0.59	0.18	2.00
445.94	445.5	0.44	0.18	2.00
453.66	453.5	0.16	0.18	2.00
460.02	459.5	0.52	0.18	2.00
536.59	536.5	0.09	0.18	2.00
637.98	638.0	-0.02	0.18	2.00
431.38	431.0	0.38	0.18	2.00
472.50	472.5	0.00	0.18	2.00
513.47	513.3	0.17	0.18	2.00
528.88	528.5	0.38	0.18	2.00
573.17	573.0	0.17	0.18	2.00
585.35	585.0	0.35	0.20	2.00
684.40	684.0	0.40	0.18	2.00
740.72	740.5	0.22	0.20	2.00
748.55	748.5	0.05	0.18	2.00
807.03	807.0	0.03	0.18	2.00
879.28	879.3	-0.02	0.18	2.00

Remark : - UUC = Unit Under Calibration
- N/A = Not Available
- The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k, which for a normal distribution corresponds to a coverage probability of approximately 95%
- * Indicates non TISI accredited

- End of Certificate -

เอกสารไม่ควบคุม

Technology

DKSH

LABOR DETAILS					
Technician	Serial Number	Start Date And Time	End Date And Time	Billable Labor Hour	Billable Travel Hour
Yongyuth Chanphong		05/13/2026 10:00 AM	05/13/2026 5:30 PM		

PARTS USED		
Part No	Part Description	Parts Qty

WORK DETAILS			
Technician	Start Date And Time	Serial Number	Work Description
Yongyuth Chanphong	05/13/2026 10:00 AM		- ทำ PM เรียบร้อย, เครื่องพร้อมใช้งาน - นำ Pump tube 3036 จาก เครื่องใหม่ มาสำรอง จำนวน 6 เส้น - Coil with heat-exchanger 10 turns ชำรุด, แก้ไขแล้ว สามารถใช้งานได้ปกติ

Customer Signature:

K Natacha

Customer Signature

Technician: Yongyuth Chanphong
Job Title: Service Manager
Email: yongyuth.yc@dksh.com

Date: 05/29/2026

เอกสารไม่ควบคุม

Technology

DKSH

Service Report

Customer Details
Location Address:
700/2 หมู่ที่ 1
จังหวัดชลบุรี, 20000

Sold to Organization:
United Analyst and Engineering Consultant Co., Ltd. _
Bangkok-HQ

Contact: Isara Bunprakob
Email: isara.b@uaeconsultant.co.th
Tel: +66 2763 2828 Ext 7018

WORK ORDER DETAILS			
Work Order Number	WO-00120844	PO Number	Q-214543
Order Type	Preventive Maintenance	Billing Type	Chargeable

PRODUCTS SERVICED				
Installed Product Id	Serial Number	Product	Warranty No.	Contract No.
IB-00105024	182688	SKALAR 2SAN59000 SAN++ Classic CFA 230V 2SAN59000		SER_ANALYTICAL1_PM_Re SC_Silver_Skalar_SA5000_182688_25/26

PROBLEM DESCRIPTION
สอบเทียบเครื่องมือ Continuous Flow Analyzer (CFA) Munufacturer: Skalar Analytical Model: San++5000-02 Serial: 182688 ID : UAE.WAS.043/2561

WORK PERFORMED
13 May 2026 - ทำ PM เรียบร้อย, เครื่องพร้อมใช้งาน ** อะไหล่ที่ควรสำรอง ** 1. Method Ammonia - Pump tube (3026, 3027) - PVC 6.00mm, ID (5155) 2. Method Phenol and Cyanide - Pump tube (3025, 3031, 3035, 3036 = 2 pcs) - Coil with heat-exchanger (5304) - Lubricant (5418)

เอกสารไม่ควบคุม

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484

NSC-TISI-TIS17025 CALIBRATION 0008

Certificate of Calibration

Cert. No.: 26TM196
Page : 1 of 3

Equipment :	BOD Incubator
Manufacturer :	Arco
Model :	UC4-1320
Serial No. :	13URC4S013201
ID No. :	UAE.WAO.015/2561
Submitted by :	United Analyst and Engineering Consultant Co.,Ltd. 3 Soi Udomsuk 41, Sukhumvit Road Bangchak, Phrakhanong Bangkok 10260
Location :	Lab. Floor 2
Received Order :	02 February 2026
Calibration Date :	03 February 2026
Ambient Temperature :	(26 ± 10) °C
Relative Humidity :	(50 ± 30) %
AC Line Voltage :	(220 ± 22) V
Calibrated by :	Krisda Malee
Approved by :	Kunchit Approved Signatory

( ) Chakrit Waewwanjua
( ) Suwit Imjai
(✓) Kunchit Promprat

Issue Date : 17 February 2026

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

Equipment : BOD Incubator
Condition As-Received : Used Item
Reference : 2602-0003OC-1

Cert. No.: 26TM196

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-


Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY57013711	25LM117	TPA	17 Jul 2026

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This measurement result is traceable to the International System of Unit maintained through :

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Not Available

Environment during calibration		
	Beginning	Finished
Temp. (°C)	26	25
REL.Humid. (%)	48	49
AC Supply (Volt)	221	220



Position :	Ref. Std. ID No.:
1	22-18RTD-2/1
2	18RTD-2/2
3	18RTD-2/3
4	18RTD-2/4
5	18RTD-2/5
6	25-18RTD-2/6
7	25-18RTD-2/7
8	21-18RTD-2/10
9 (ref.)	18RTD-2/9

Probe Installation Details :

a =	10	cm
b =	10	cm
c =	10	cm

Dimension of Chamber :

D =	0.62	m
W =	1.2	m
H =	1.2	m
Capacity =	0.89	m³

เอกสารไม่ควบคุม

Equipment : BOD Incubator
Condition As-Received : Used Item
Reference : 2602-0003OC-1
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Not Available

Cert. No.: 26TM196

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor k
20.0	20.0	19.9	0.65	0.40	1.4	2

Calibration Point (°C)	Measured Temperature (°C) Position									Uncertainty (± °C)
	1	2	3	4	5	6	7	8	9 (ref.)	
20.0	20.079	19.917	20.065	19.973	19.943	19.959	19.852	19.860	20.006	0.84

Average* : The average of 30 values in each position.
Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.
Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.
Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.
UUC* : Unit Under Calibration
Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม