

ภาคผนวก ฉ

ใบรับรองการสอบเทียบเครื่องมือ



right solutions.
right partner.

รายการเครื่องมือที่ใช้ในการวิเคราะห์ / ทดสอบ

Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Water Lab	pH at 25 °C	pH meter	BKK_EN0342	9-Oct-25	9-Oct-26	12
Water Lab	Oil & Grease	Electronic Top-Loading Balance	BKK_EN0003	17-Jul-25	17-Jul-26	12
Water Lab	Oil & Grease	Water Bath	BKK_EN0439	9-Oct-25	9-Oct-26	12
Water Lab	Total Suspended Solids	Electronic Top-Loading Balance	BKK_EN0003	17-Jul-25	17-Jul-26	12
Water Lab	Total Suspended Solids	Oven	BKK_EN0425	6-Oct-25	6-Oct-26	12
Water Lab	Total Dissolved Solids 180°C	Electronic Top-Loading Balance	BKK_EN0003	17-Jul-25	17-Jul-26	12
Water Lab	Total Dissolved Solids 180°C	Oven	BKK_EN0425	6-Oct-25	6-Oct-26	12
Water Lab	BOD	DO Meter	BKK_EN0017	20-May-25	20-Nov-26	18
Water Lab	BOD	Incubator	BKK_EN0272	24-Dec-25	24-Dec-26	12
Water Lab	BOD	Burette	BKK_EN0422	3-Sep-25	3-Sep-26	12
Water Lab	COD	Hot Block	BKK_EN0370	23-Dec-25	23-Dec-26	12
Water Lab	COD	Spectrophotometer	BKK_EN0356	8-Oct-25	8-Oct-26	12
Water Lab	Lead	ICP-MS	BKK_EL0043	3-Oct-25	2-Oct-26	12
Water Lab	Lead	Hot Block	BKK_EL0054	4-Mar-25	4-Sep-26	18
Water Lab	Lead	Chamber (Cooling Room)	BKK_EN0167	4-Jun-25	4-Dec-26	18



Certificate of Calibration

Cert.No.: 25CH1162

Page.: 1 of 3

Equipment : pH Meter
Manufacturer : Hach
Model : HQ411d
Serial No. : 200100031163
ID No. : BKK_EN0342
Condition As-Received: Used Item
Received Date : 08 October 2025
Calibration Date : 09 October 2025
Reference : 2510-0271DSC-1
Submitted by :

ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand

Ambient Temperature : (25 ± 2.5) °C
Relative Humidity : (50 ± 15) %
Calibration Procedure : In - house method :
- CP-CH5 by direct measurement with
certified reference material (CRM)
- CP-CH8 by comparison with temperature standard

Calibrated by : Walalak Sirithean

Approved by :

Approved Signatory

- () Chakrit Waewwanjua
() Ponpan Paipim
(✓) Saithip Meangmai

Issue Date :

10 October 2025

REVIEW BY

APPROVED BY

NEXT CAL DATE.....09/10/26

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Cert.No.: 25CH1162

Page.: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Ref. Standard Thermometer	4982054	110RC044	25I708	03 July 2026
- This measurement result is traceable to SI through Technology Promotion Association (Thailand - Japan)				

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.007	CPA chem	1114384	12 June 2027
pH 6.965	CPA chem	1066667	18 Jan 2026
pH 10.010	CPA chem	1135355	16 Aug 2026

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7,10)

<u>Unit Under Calibration</u>	<u>Standard pH Buffer Solution</u>	<u>Actual pH Reading</u>	<u>Actual mV Reading (mV)</u>	<u>Uncertainty of pH Measurement (±)</u>	<u>Coverage factor <i>k</i></u>
pH Electrode S/N.: 252063043080	4.007	3.996	176.6	0.0046	2.00
	6.965	6.974	1.1	0.0084	2.00
	10.010	9.996	-176.9	0.0070	2.00

Remark - Can not connect the BNC because the plug does not match with the socket.



Cert.No.: 25CH1162

Page.: 3 of 3

Calibration Results

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : PHC281
- Serial No. : 252063043080

Dimension of probe

- Length : 103 mm.
- Diameter : 12 mm.
- Immersion Depth : 90 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (± °C)	Coverage factor <i>k</i>
25.0	25.001	25.0	-0.001	0.13	2.00

Remark - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Accredited by

NSC-TISI-TIS 17025

Calibration 0426



NSC-TISI-TIS 17025

CALIBRATION 0426


Calibration certificate

Calibration Certificate No. 25BCI0265

Object	Electronic non-automatic weighing instrument	This calibration certificate documents the traceability to national standards.
Manufacturer	Sartorius	Uncertainties of measurements are taken into account when only statements of compliance are made.
Type	MSE224S-100-DU	This certificate was prepared by Sartorius Corporation in accordance to the current ISO/IEC 17025:2017 standard and Sartorius Work Instruction (Method) SOP WI 08.
Serial QM Ident. no.	27405555 BKK_EN0003	This certificate relate and apply this equipment only.
Customer	ALS Laboratory Group (Thailand)Co., Ltd. 104 Phatthanakarn 40,Phattanakarn Rd.,Khwaeng Phatthanakarn ,Khet Suan Luang,Bangkok 10250	REVIEW BY  APPROVED BY  NEXT CAL DATE.....17/07/26
Order no.	265054	
Number of pages	4	
Date of calibration	17 Jul 2025	

This calibration certificate may not be reproduced other than in full except with the permission of NSC-TISI-TIS-17025 and the issuing laboratory. Calibration certificates without signature are not valid.

The user is obliged to have the object recalibrated at appropriate intervals.

Date of issue	17 Jul 2025	Approval of the Calibration Certificate 	Person in charge 
		Mr. Chonchai Inthana	Chonchai Inthana

Calibration object

Single range instrument

Model	MSE224S-100-DU
Serial Number	27405555
QM Ident. no Inventory no.	BKK_EN0003 ---

Maximum capacity (Max. load)	220.0000 g
Measured up to	220.0000 g
Scale interval	0.0001 g

Place of calibration

Address	According to page 1
Department Cost center	ENVI Department ---
Building Floor	--- 1st Floor.
Room	Laboratory Room.
Maximum temperature variation at place of calibration	5 K

Calibration procedure

EURAMET Calibration Guide No. 18, Version 4.0 (11/2015) - Guidelines on the Calibration of Non-Automatic Weighing Instruments

Test equipment

Test equipment type	Test equipment ID	Valid until
Thermometer	Testo 174(Traceable to Si unit through ENTECH)	11 Nov 2025
Test weight set OIML R111 E2	Certificate No.M2308197S ,E2(Traceable to SI unit through TCS)	23 Aug 2025

Adjustment Status

The measuring device was internally adjusted before the calibration.

Environmental and measuring conditions

Date of calibration	17 Jul 2025
Temperature at place of calibration Temp. diff. $T_{\text{weights}} - T_{\text{place}}$	22.5 °C 0.7 K
Measuring conditions	The installation site is suitable. The device is level. Balance was loaded up to Max before test.
Comments	Humidity 58.0 %RH.

Measurement results | Measurement uncertainties

Repeatability

Test load (nominal): 10 g 200 g		
	10 g	200 g
1	10.0000 g	200.0000 g
2	10.0000 g	199.9999 g
3	10.0000 g	200.0000 g
4	10.0000 g	200.0000 g
5	10.0001 g	199.9999 g
6	10.0000 g	200.0000 g
7	10.0000 g	200.0000 g
8	10.0001 g	200.0000 g
9	10.0000 g	200.0000 g
10	10.0000 g	199.9999 g
	$s = 0.00004 \text{ g}$	$s = 0.00005 \text{ g}$

Eccentricity

Test load (nominal): 100 g	
Center	100.0000 g
Front left	100.0001 g
Back left	100.0000 g
Back right	100.0001 g
Front right	100.0001 g
Maximum deviation from centric loading indication $ \Delta l_{\text{ecc}} _{\text{max}} = 0.0001 \text{ g}$	

Error of indication

Testload	Indication	Error	Expansion factor	Uncertainty	Uncertainty relative
L	I	E	k	$U(E)$	$U_{\text{rel}}(E)$
0.0100 g	0.0100 g	0.0000 g	2.00	0.00012 g	1.2 %
0.1000 g	0.1000 g	0.0000 g	2.00	0.00013 g	0.13 %
1.0000 g	1.0000 g	0.0000 g	2.00	0.00013 g	0.013 %
2.0000 g	2.0000 g	0.0000 g	2.00	0.00013 g	0.0065 %
5.0000 g	5.0000 g	0.0000 g	2.00	0.00013 g	0.0026 %
10.0000 g	10.0000 g	0.0000 g	2.00	0.00013 g	0.0013 %
20.0000 g	20.0000 g	0.0000 g	2.00	0.00014 g	0.00068 %
50.0000 g	50.0000 g	0.0000 g	2.00	0.00015 g	0.00029 %
100.0000 g	100.0000 g	0.0000 g	2.00	0.00018 g	0.00018 %
200.0000 g	200.0000 g	0.0000 g	2.00	0.00028 g	0.00014 %
220.0000 g	220.0001 g	0.0001 g	2.00	0.00032 g	0.00015 %

Maximum error of indication $|E|_{\text{max}} = 0.0001 \text{ g}$

$U_{\text{rel}}(E)$ is the quotient of $U(E)$ and test load L . The uncertainty of measurement $U(E)$ is valid only if error E is considered. You will find reference notes on the uncertainty of measurement in use under: Appendix to the calibration certificate | Interpretation of measurement results.
Reference note: The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the documented Expansion factor, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

End of calibration certificate

Uncertainty of measurement in use

Device adjusted before measurement	Yes
Temperature deviation considered	1.5 K (isoCAL active)
Temperature coefficient considered	$1 \cdot 10^{-6}/\text{K}$


Uncertainty of the weighing result $U_{gl}(W)$

$U_{gl}(W) = 0.00013 \text{ g} + 4.19 \cdot 10^{-6} \cdot R$

Reference note: The current uncertainty of measurement is calculated by entering of the reading R into this formula. In relation to this, there is no need for a correction of the indication error. The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied with an Expansion factor of 2, determined in accordance with the European Calibration Guideline EURAMET cg-18, V4.0. There is a 95 % probability that the value of the measurand will be in the assigned value range.

Indication in % from max load	Net indication R	Uncertainty $U_{gl}(W)$	Uncertainty relative $U_{gl}(W)_{rel}$
1 %	2.2000 g	0.00014 g	0.0063 %
25 %	55.0000 g	0.00036 g	0.00066 %
50 %	110.0000 g	0.00059 g	0.00054 %
75 %	165.0000 g	0.00082 g	0.00050 %
100 %	220.0000 g	0.0011 g	0.00048 %

Graphic realization of the relative uncertainty of measurement | process accuracy

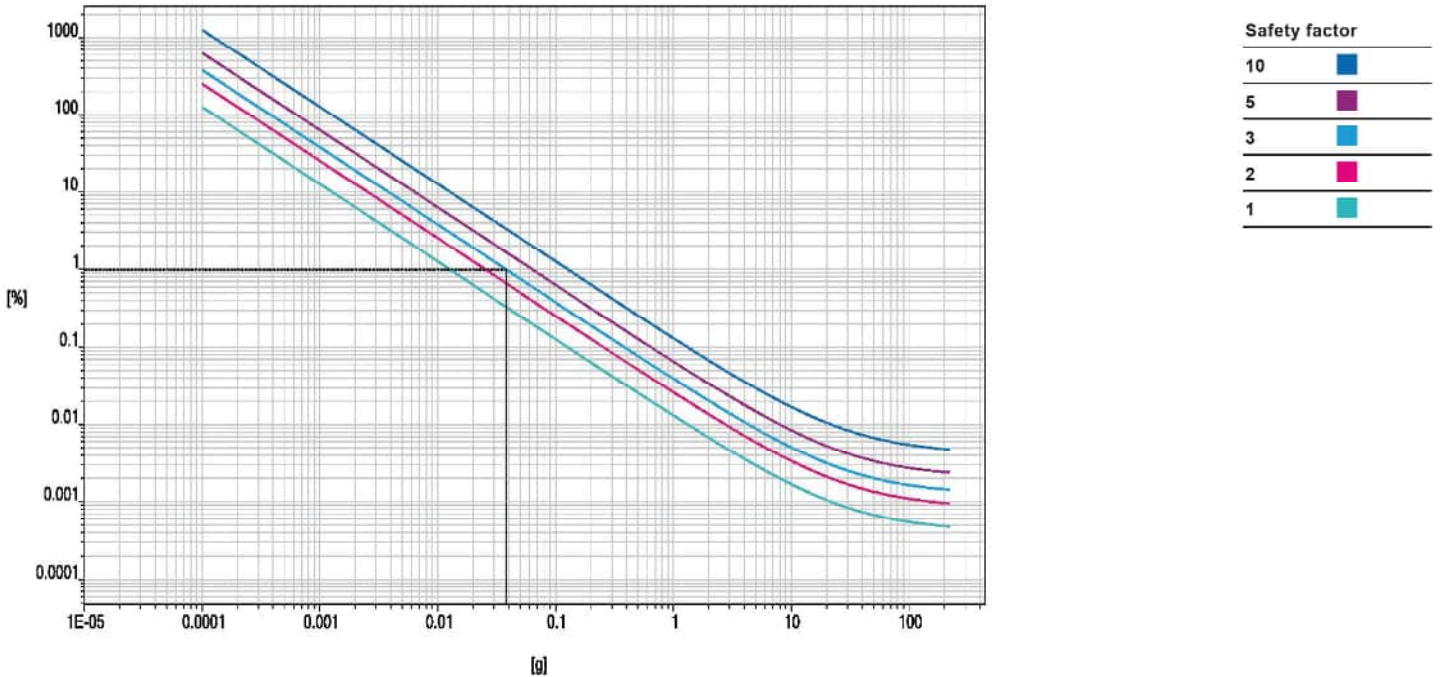

Displayed example

Process accuracy	1.00 %
Safety factor	3
Minimum sample weight	0.0380 g



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert. No.: 25TM528

Page : 1 of 3

Equipment : Water Bath
Manufacturer : Memmert
Model : WNE 29
Serial No. : L622.0282
ID No. : BKK_EN0439

REVIEW BY

APPROVED BY

NEXT CAL DATE 09/10/26

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand

Location : Organic Preparation Lab

Received Order : 08 October 2025

Calibration Date : 09 October 2025

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

AC Line Voltage : (220 ± 22) V

Calibrated by : Kunchit Promprat

Approved by :

Approved Signatory

() Chakrit Waewwanjua

() Ponpan Paipim

(✓) Suwit Imjai

Issue Date : 28 October 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2510-0042OC-13

Cert. No.: 25TM528
Page : 2 of 3

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT04 Based on ASTM E715 according to direct measurement method with Data Acquisition which connected with Industrial Platinum Resistance Thermometer (IPRT).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1) Data Acquisition	MY58041391	25LM20	TPA	08 Feb 2026

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This measurement result is traceable to the International System of Unit maintained through :


Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Heat transfer medium used : Water

	<u>Environmental</u>		<u>AC Voltage Supply</u>
	(°C)	(%R.H.)	(Volt)
Beginning of Calibration	24	63	224
Finished of Calibration	24	58	224

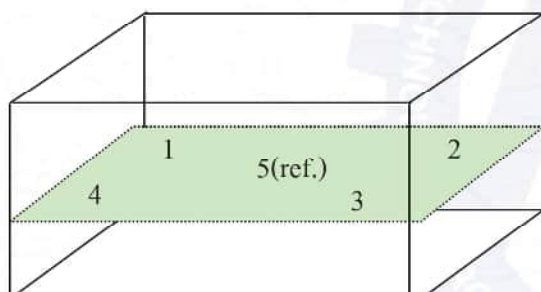

Front

<u>Position :</u>	<u>Ref. Std. ID No.:</u>
1	70RC143
2	70RC144
3	70RC145
4	70RC146
5(ref.)	70RC147



Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2510-0042OC-13
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source

Cert. No.: 25TM528
Page : 3 of 3

Calibration point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Average* Standard Reading (°C)					Uncertainty (± °C)
			Position					
			1	2	3	4	5 (ref.)	
85.0	85.0	85.0	84.863	84.748	84.869	84.990	84.966	0.21

Calibration point (°C)	Uniformity (°C)	Stability (± °C)	Coverage Factor <i>k</i>
85.0	0.33	0.12	2

Average* : The average of 30 values in each position.

Uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Stability : One-half of the greatest maximum difference of measured temperature at any one probe.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES

534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000 FAX. 0-2719-9484

Certificate of Testing

Cert.No.: 25TW101

Page.: 1 of 2

Equipment :

DO Meter

Manufacturer :

YSI

Model :

5000-230V

Serial No. :

09J101147

ID No. :

BKK_EN0017

Received Date :

19 May 2025

Test Date :

20 May 2025

Reference :

2505-0593DSC-1

Submitted by :

ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand

Laboratory Condition :

Temperature (25 ± 5) °C

Humidity (50 ± 20) %

Test Procedure :

In - house method : CP-CH9

by Comparison Technique with Azide Modification Method

Tested by :

Walalak Sirithean

Approved by :

Approved Signatory

() Chakrit Waewwanjua

() Ponpan Paipim

(✓) Saithip Meangmai

Issue Date :

20 May 2025

REVIEW BY

APPROVED BY

NEXT CAL DATE..... 20/11/26



Cert.No.: 25TW101

Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

This measurement result is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

<u>Instruments</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1. Burette	-	130BU10	25CG1126	18 Mar 2027
2. Balance	14233821	110RC001	24MM131	04 July 2025

2. Standard Material :-

<u>Material</u>	<u>Manufacturer</u>	<u>Lot.No.</u>	<u>Assay</u>
Sodium Thiosulfate 5-Hydrate AR	KEMAUS	2203162447	99.6%

Result : **Dissolved Oxygen Meter Adjustment With Air 100 %**

Dissolved Oxygen Probe No.: 16K100498

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.20	8.21	0.0090

This report was certified only for the instrument we tested. It is allowable to use for study
Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced
other in full, without written approval of the laboratory

-o0o-



Certificate of Calibration

Cert. No.: 25LM83

Page.: 1 of 2

Equipment : DO Meter with Sensor

Manufacturer : YSI

Model : 5000-230V

Serial No. : 09J101147

ID No. : BKK_EN0017

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand

Location : TPA On Site Calibration Laboratory

Received Order : 19 May 2025

Calibrated Date : 20 May 2025

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

AC Line Voltage : (220 ± 22) V

Calibrated by : Warakorn Lerngagtrakul

Approved by :

Approved Signatory

() Chakrit Waewwanjua

() Suwit Imjai

(✓) Kunchit Promprat

Issue Date :

26 May 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : DO Meter with Sensor
Condition As-Received : Used Item
Reference : 2505-0593DSC-2

Cert. No.: 25LM83

Page.: 2 of 2

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Digital Thermometer	2188080	2411022	TPA	17 Sep 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N.: 16K100498

Calibration Point (°C)	Immersion Depth (mm)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty (± °C)	Coverage Factor <i>k</i>
20.00	60	20.003	19.92	-0.083	0.15	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Certificate No. T252279

Page 1 of 4

Certificate of Calibration

Equipment : Chamber (Incubator)

Manufacturer : MEMMERT

Model : ICP 750

Serial No. : F818.0033

Customer Code : BKK_EN0272

ID No. : T8041A4

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd.,

Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250

Customer Location : Wet Chemistry Lab 2


Date of Receipt : 17 December 2025

Calibrated By : Atiphong Rongrat (Technician)

Approved By :  Boonchai Suriyawong (Site Calibration Manager)

Date of Issue : 12 JAN 2026

Date of Issue : _____

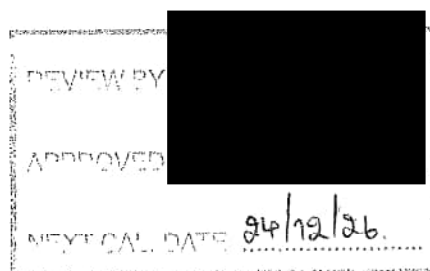

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Certificate No. T252279

Page 2 of 4

Calibration Report

Equipment : Chamber (Incubator)
 Date of Calibration : 24 December 2025
 Environment : Temperature : 23.4-24.9 °C
 Line Voltage : 221.4-224.7 V
 Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert 12 resistance thermometer detectors into its chamber , the other one resistance thermometer detector use for ambient temperature measurement . The calibration was done in according to WI-T20 (based on ASTM E145-94 (Reapproved 2001) and AS2853-1986).

All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
RTD	100 ohm	31-(CH1-10)	T250835	24 May 2026
RTD	100 ohm	32-(CH1-10)	T250835	24 May 2026
DATA LOGGER	34970A	T193	T250835	24 May 2026

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

Equipment Description :

Time Constant 2 Hour - Minute At 20 °C
 Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
☐ Close
☒ Not Available

5. Adjustment :

(X) without adjustment


() after adjustment

Approved By. 

Certificate No. T252279

Page 3 of 4

Calibration Report

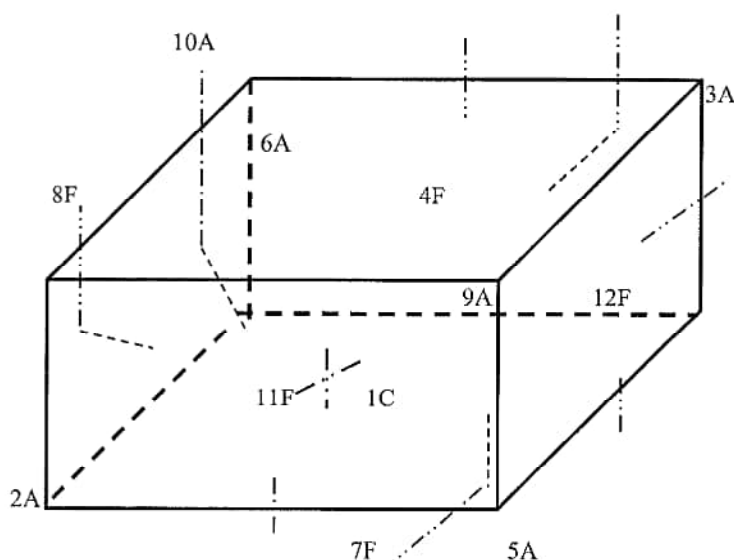

C = Centre , F = Centre of Face , A = Corner , E = Centre of Edge

1C	=	31-CH1
2A	=	31-CH2
3A	=	31-CH3
4F	=	31-CH4
5A	=	31-CH5
6A	=	31-CH6
7F	=	31-CH7
8F	=	31-CH8
9A	=	31-CH9
10A	=	31-CH10
11F	=	32-CH1
12F	=	32-CH2

Approved By. _____



Certificate No. T252279

Page 4 of 4

Calibration Report

Measurement Results :

Calibration Point	Average Standard Reading at each position (°C)											
	31-CH1	31-CH2	31-CH3	31-CH4	31-CH5	31-CH6	31-CH7	31-CH8	31-CH9	31-CH10	32-CH1	32-CH2
20	20.11	20.22	20.03	20.39	20.12	19.80	19.89	20.19	20.26	19.97	19.85	20.06

Chamber (Incubator)			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (±°C)	Uniformity (°C)	Uncertainty (±°C)	Coverage Factor k
	Min , Max	Average					
20.0	19.9 , 20.1	20.0	20.07	0.10	0.59	0.39	2.03

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor **k** which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By. [REDACTED]



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert.No.: 25CG3385

Page.: 1 of 2

Equipment :	Burette
Capacity :	50 mL
Serial No. :	-
ID. No. :	BKK_EN0422
Manufacturer :	Witeg
Made in :	Germany
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand
Ambient Temperature :	(20 ± 2.5) °C
Relative Humidity :	(50 ± 10) %
Barometric Pressure :	753 mmHg
Calibration Procedure :	ASTM E 542 - 01
Calibrated by :	Srisuda Khamtha 1
Approved by :	 Approved Signatory
() Ponpan Paipim	
(✓) Chakrit Waewwanjua	

Issue Date : 3 September 2025

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : Burette
Received Date : 1 September 2025
Condition As-Received : Used Item
Calibration Date : 3 September 2025
Reference : 2509-0049DSC-1

Cert.No.: 25CG3385

Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

<u>Instruments</u>	<u>Model</u>	<u>Serial No.</u>	<u>ID. No.</u>	<u>Certificate No.</u>	<u>Traceability</u>	<u>Due date</u>
1) Balance	MS204TS	C226356983	140RC010	24MM603	TPA	10 Oct 2025
2) Data Logger	HL-20D	20683159	140EC012	24H2129	TPA	15 Oct 2025
3) Digital Thermometer	HH376	230806555	140EC013	25I1740	TPA	17 Jan 2026

This measurement result is traceable to SI Unit

2. The certificate is valid only to the item calibrated on date and place of calibration.

3. True value is converted to true volume at the standard temperature of 20 °C

Calibration result :

Nominal capacity (mL)	Reading (mL)	Uncertainty (± mL)	k Factor
10	9.9941	0.0082	2.00
25	24.9804	0.0087	2.00
50	49.9819	0.010	2.00

Remark mL = cm³

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-



Metrology Center
SCI ECO Services Company Limited

51 Moo 8, Tubkwang, Kaeng Khoi, Saraburi, Thailand 18260

Bangkok Tel : +668 9205 6851 , +669 81924 0059

Saraburi Tel : +669 8247 2360

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No. T252276

Certificate of Calibration

Page 1 of 4

Equipment : Hot Block

Manufacturer : Environmental Express

Model : B3000-240


Serial No. : 2021CODW148

Customer Code : BKK_EN0370

ID No. : T2940A5

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,
Khet Suan Luang, Bangkok 10250

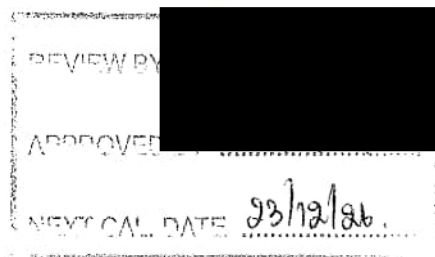

Customer Location : Wet Chemistry Lab2

Date of Receipt : 17 December 2025

Calibrated By : Sujjar Naknakred (Site Calibration Manager)

Approved By : [Redacted] Boonchai Suriyawong (Site Calibration Manager)

Date of Issue : 06 JAN 2026

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.



Metrology Center

SCI ECO Services Company Limited

51 Moo 8, Tubkwang, Kaeng Khoi, Saraburi, Thailand 18260

Certificate No. T252276

Page 2 of 4

Calibration Report

Equipment : Hot Block
Date of Calibration : 23 December 2025
Environment : Temperature : 24°C - 24.4°C
Line Voltage : 221.3 V - 225.6 V
Relative Humidity 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert 29 standard thermocouples type T into its chamber , the other one standard thermocouples type T use for ambient temperature measurement . The calibration was done in according to WI-T20.

All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN221-TN230	T251759	17 October 2026
TC	TYPE T	TN231-TN240	T251759	17 October 2026
DATA LOGGER	34970A	T261	T251759	17 October 2026

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

Equipment Description :

Time Constant 1 Hour 37 Minute At 150 °C
Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
☐ Close
☒ Not Available


5. Adjustment :

() without adjustment

(X) after adjustment

Approved By. _____

Calibration Report

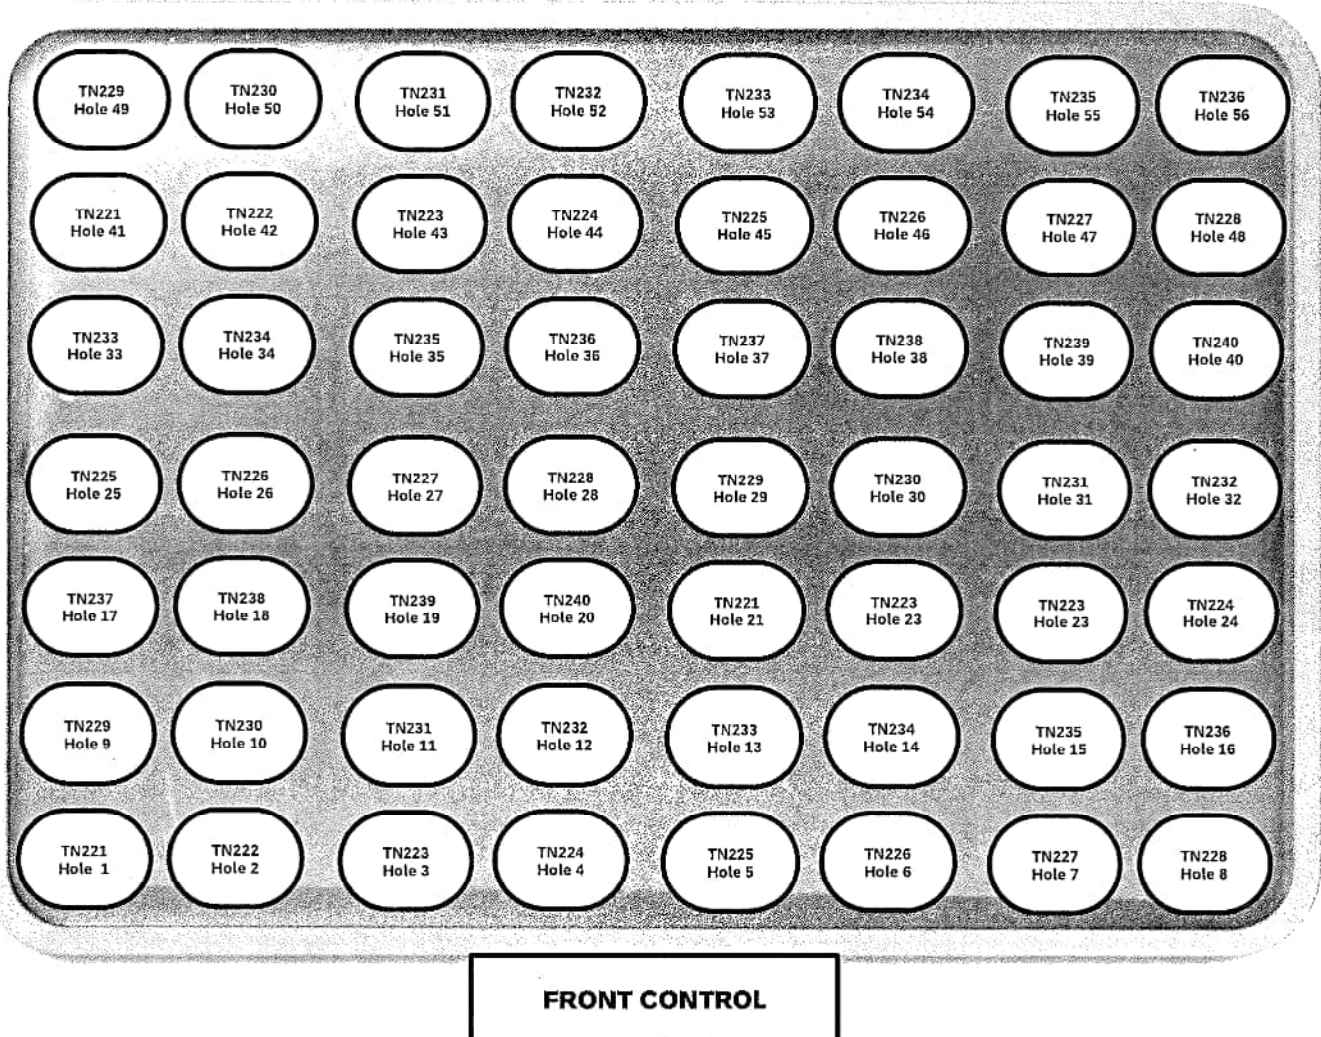

Approved By. 

Calibration Report

Measurement Results

		Average Standard Reading at each position (°C)									
CAL POINT		TN221 Hole 1	TN222 Hole 2	TN223 Hole 3	TN224 Hole 4	TN225 Hole 5	TN226 Hole 6	TN227 Hole 7	TN228 Hole 8	TN229 Hole 9	TN230 Hole 10
150	Max °C	149.91	150.71	150.47	150.02	149.97	150.84	150.22	150.75	150.45	149.98
	Min °C	149.18	150.18	149.80	149.36	149.59	150.31	149.77	150.44	149.46	149.53
	Average °C	149.55	150.44	150.13	149.69	149.78	150.58	149.99	150.59	149.95	149.76
CAL POINT		TN231 Hole 11	TN232 Hole 12	TN233 Hole 13	TN234 Hole 14	TN235 Hole 15	TN236 Hole 16	TN237 Hole 17	TN238 Hole 18	TN239 Hole 19	TN240 Hole 20
150	Max °C	150.12	150.09	149.94	150.13	150.67	150.36	150.65	150.21	150.30	150.12
	Min °C	149.57	149.50	149.55	149.59	150.36	150.06	149.73	149.84	149.52	149.59
	Average °C	149.85	149.79	149.75	149.86	150.51	150.21	150.19	150.02	149.91	149.86
CAL POINT		TN221 Hole 21	TN222 Hole 22	TN223 Hole 23	TN224 Hole 24	TN225 Hole 25	TN226 Hole 26	TN227 Hole 27	TN228 Hole 28	TN229 Hole 29	TN230 Hole 30
150	Max °C	150.10	149.78	150.36	150.52	150.24	149.78	149.81	149.61	150.36	150.05
	Min °C	149.57	149.39	149.42	149.94	150.00	149.53	149.14	149.38	150.04	149.69
	Average °C	149.83	149.59	149.89	150.23	150.12	149.65	149.48	149.49	150.20	149.87
CAL POINT		TN231 Hole 31	TN232 Hole 32	TN233 Hole 33	TN234 Hole 34	TN235 Hole 35	TN236 Hole 36	TN237 Hole 37	TN238 Hole 38	TN239 Hole 39	TN240 Hole 40
150	Max °C	150.07	149.46	149.52	149.91	150.05	150.20	149.69	149.70	150.04	149.73
	Min °C	149.49	149.30	149.39	149.70	149.66	149.68	149.35	149.33	149.75	149.46
	Average °C	149.78	149.38	149.46	149.80	149.85	149.94	149.52	149.52	149.90	149.60
CAL POINT		TN221 Hole 41	TN222 Hole 42	TN223 Hole 43	TN224 Hole 44	TN225 Hole 45	TN226 Hole 46	TN227 Hole 47	TN228 Hole 48	TN229 Hole 49	TN230 Hole 50
150	Max °C	149.51	150.32	150.30	149.69	149.91	149.93	150.14	149.58	149.91	150.29
	Min °C	149.18	149.81	149.56	149.44	149.38	149.60	149.61	149.27	149.36	149.48
	Average °C	149.35	150.07	149.93	149.57	149.65	149.77	149.87	149.42	149.64	149.88
CAL POINT		TN231 Hole 51	TN232 Hole 52	TN233 Hole 53	TN234 Hole 54	TN235 Hole 55	TN236 Hole 56				
150	Max °C	150.25	150.40	150.59	150.13	150.57	150.43				
	Min °C	149.31	149.89	150.13	149.68	149.75	149.87				
	Average °C	149.78	150.14	150.36	149.90	150.16	150.15				

Hot Block			Temperature Distribution	
Setting (°C)	Reading (°C)		Stability (± °C)	Uncertainty (± °C)
	Min , Max	Average		
150	149.9 , 150.1	150.0	0.50	1.01

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

End of Certificate.

Approved By. _____



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert.No.: 25CHO537

Page.: 1 of 3

Equipment :	Spectrophotometer
Manufacturer :	HACH
Model :	DR3900
Serial No. :	2021559
ID No. :	BKK_EN0356
Condition As-Received:	Used Item
Received Date :	08 October 2025
Calibration Date :	08 October 2025
Reference :	2510-0042OC-11
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand
Calibration Place :	Wet Chemistry Lab 2
Ambient Temperature :	(21.9 to 21.9) °C (On-Site)
Relative Humidity :	(62 to 65) % (On-Site)
Calibration Procedure :	In - house method : CP-OCH4 based on ASTM E 275-08
Calibrated by :	Uthen Kankawi
Approved by :	Approved Signatory
() Chakrit Waewwanjua	
() Ponpan Paipim	
(✓) Saithip Meangmai	
Issue Date :	9 October 2025

REVIEW BY

APPROVED

NEXT CAL DATE.....08/10/26

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Cert. No. : 25CHO537

Page : 2 of 3

Condition of calibration result

1. Reference Standard Material :

<u>Material</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due date</u>
1. Absorbance Standard set	44487	122584	31 May 2026
2. Wavelength Standard set	36730	118120	15 Jan 2026
3. Wavelength Standard set	36730	118121	15 Jan 2026

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certificate is traceable to the International System of Unit maintained through :

- Starna Scientific Ltd.

4. Spectral BandWidth : 5 nm
Scan Speed : - nm/min

Calibration Results : without adjustment

Wavelength Accuracy

Certified Values of Reference Material (nm)	UUC Reading (nm)	Uncertainty of Measurement ($\pm$ nm)	Coverage Factor <i>k</i>
418.40	418	0.59	2.00
479.88	480	0.59	2.00
513.75	513	0.59	2.00
537.00	536	0.59	2.00
638.00	638	0.59	2.00
747.61	748	0.59	2.00
807.04	807	0.59	2.00



Cert. No. : 25CHO537

Page : 3 of 3

Calibration Results : without adjustment

Photometric Accuracy

Wavelength (nm)	Certified Values of Reference Material (Abs)	UUC Reading (Abs)	Uncertainty of Measurement ($\pm$ Abs)	Coverage Factor <i>k</i>
420.0	Zero	0.000	0.0028	2.00
	0.5750	0.573	0.0028	2.00
	0.7156	0.713	0.0028	2.00
	1.0176	1.014	0.0028	2.00
440.0	Zero	0.000	0.0028	2.00
	0.5598	0.557	0.0028	2.00
	0.7037	0.700	0.0028	2.00
	1.0013	0.997	0.0028	2.00
465.0	Zero	0.000	0.0028	2.00
	0.5222	0.522	0.0028	2.00
	0.6646	0.664	0.0028	2.00
	0.9444	0.945	0.0028	2.00
546.1	Zero	0.000	0.0028	2.00
	0.5234	0.523	0.0028	2.00
	0.7007	0.700	0.0028	2.00
	0.9992	0.999	0.0028	2.00
590.0	Zero	0.000	0.0028	2.00
	0.5573	0.556	0.0028	2.00
	0.7760	0.773	0.0028	2.00
	1.1104	1.108	0.0028	2.00
635.0	Zero	0.000	0.0028	2.00
	0.5648	0.565	0.0028	2.00
	0.7654	0.765	0.0028	2.00
	1.0961	1.096	0.0028	2.00

Remark

- Each individual filter is measured against the empty filter holder (blank) used to zero the spectrophotometer
- UUC = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k* , providing a level of confidence of approximately 95 %.


Agilent Technologies

Agilent Technologies (Thailand) Limited
U CHU LIANG BLDG. 22/F UNIT A,D
968 RAMA 4 ROAD, SILOM, BANGRAK
Bangkok 10500 Thailand

Tel. +662 637 6363
Fax: +662 632 4334
Email: ccc-smt@agilent.com
Website: www.agilent.com/chem

Customer Contact:

ALS Laboratory Group (Thailand) Co
Ltd Head Office

104 Phatthanakan 40 Phatthanakan Rd
Khwaeng Phatthanakan Khet Suan

TAX ID : 0105540004859

Chanattagarn.lmchom@alsglobal.com
27603068

Invoice To:

ALS Laboratory Group (Thailand) Co
Ltd Head Office

104 Phatthanakan 40 Phatthanakan Rd
Khwaeng Phatthanakan Khet Suan

SERVICE REPORT

Customer Purchase Order Number:	Customer Number: 70371013
Service Request:	Service Request Date:
Service Order: 6007607368	Service Confirmation: 6906615981

Delivery Site:

ALS Laboratory Group (Thailand) Co
Ltd Head Office

104 Phatthanakan 40 Phatthanakan Rd
Khwaeng Phatthanakan Khet Suan

Location:

Room
Bldg
Lab
Dept

Direct Inquiries to:

Contact Name: Customer Contact Center
Contact E-mail: ccc-smt@agilent.com
Contact Telephone: +662 637 6363
Contact Fax: +662 632 4334

REVIEW BY ..	
APPROVED BY ..	
TEXT CAL. DATE	02/10/2026

products | applications | software | services

Learn more about Agilent's Special Offers, Products, Services and our
full range of laboratory productivity solutions optimized for your
applications and workflows. Visit us at www.agilent.com/chem

Agilent Technologies (Thailand) Limited. Head Office
U Chu Liang Bldg. 22/F Unit A,D
968 Rama 4 Road, Silom, Bangrak,
Bangkok 10500 Thailand
Tax ID : 0105542068218

Citibank N.A. Bangkok Branch
399 Interchange 21 Building, Sukhumvit Road, Klongtoey Nau
Sub-district, Wattana District, Bangkok 10110 Thailand
Acc. No: 012-4452-007,
THB:Krung Thai Bank PCL
Siam Square Br.,416/1-2 Rama I Rd.,Pathumwan, BKK 10330
Thailand

ORIGINAL

Service Instrument:

Model Number	Model Description	Serial Number	System Handle	Parent Asset
SYS-IM-7900	ICPMS 7900 System			
G8410A	SPS 4 Autosampler	AU15430722	ICP MS 7900	SYS-IM-7900
G8411A	ISIS 3 for Agilent 7850/7900/8900	JP15510227	ICP MS 7900	SYS-IM-7900
G3292A	PSC 6106T Chiller	2U15A1948	ICP MS 7900	SYS-IM-7900
G8403A	Agilent 7900 ICP-MS	JP15471169	ICP MS 7900	SYS-IM-7900

Service Items:

Item	Service/Part #	Description	Qty	Entitlement	Service Start	Service End
1000	EOQ	Enterprise Operational Qualification	1.00	Agreement Entitlement - 100 % covered	03.10.2025	03.10.2025
1010	5185-5850	ICP-MS Checkout Solutions	1.00	Agreement Entitlement - 100 % covered		

Additional Information:

Service Information:**Problem Description:**

*WU-EQQ-IM-7900-5001413366

Service Provided:

Perform OQ hardware control. Test logon , tune , BG and stability.
Test OQ control of instrument ICPMS=BKK_EL0043
After done the instrument test all pass.

Service Overview Code:

Reason Code: Scheduled Service
Diagnosis Code: Scheduled Service
Resolution Code: Scheduled Service

Reported Hours:

5.0

Travel Hours:

1.5

Customer Field Service**Representative Name:**


Panthep Kurasathain

Customer Field Service**Representative Signature:****Date:**

03 Oct 2025

Customer Name:

Anchalee Khamjan

Customer Signature:**Date:**

03 Oct 2025

Additional Comments:



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th

E-Mail : calibrate@scg.co.th

Certificate No. T250355

Page 1 of 6

Certificate of Calibration

Equipment : HEATING BLOCK

Manufacturer : Environmental Express

Model : SC 196

Serial No. : 6974CECW3285

Customer Code : BKK_EL0054

ID No. : T5306A3

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250

Customer Location : Acid Digestion Lab

Date of Receipt : 26 February 2025

Calibrated By : Atiphong Rongrat (Technician)

Approved By :  / Boonchai Suriyawong (Site Calibration Manager)

Date of Issue : 17 MAR 2025



The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th

E-Mail : calibrate@scg.co.th

Certificate No. T250355

Page 2 of 6

Calibration Report

Equipment : HEATING BLOCK
Date of Calibration : 4 March 2025
Environment : Temperature : 24.4-24.9 °C
Line Voltage : 221.6-226.3 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert nine standard thermocouples type T into its chamber , the other one standard thermocouples type T use for ambient temperature measurement . The calibration was done in according to WI-T20.

All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN221-TN230	T240712	19 April 2025
TC	TYPE T	TN231-TN240	T240712	19 April 2025
TC	TYPE T	TN241-TN250	T240401	16 March 2025
TC	TYPE T	TN251-TN260	T240401	16 March 2025
DATA LOGGER	34970A	T193	T240401	16 March 2025

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

Equipment Description :

Time Constant 2 Hour 40 Minute At 95 °C

Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max

☐ Close

☒ Not Available

5. Adjustment :

() without adjustment


(X) after adjustment

Approved By. _____

Certificate No. T250355

Page 3 of 6

Calibration Report

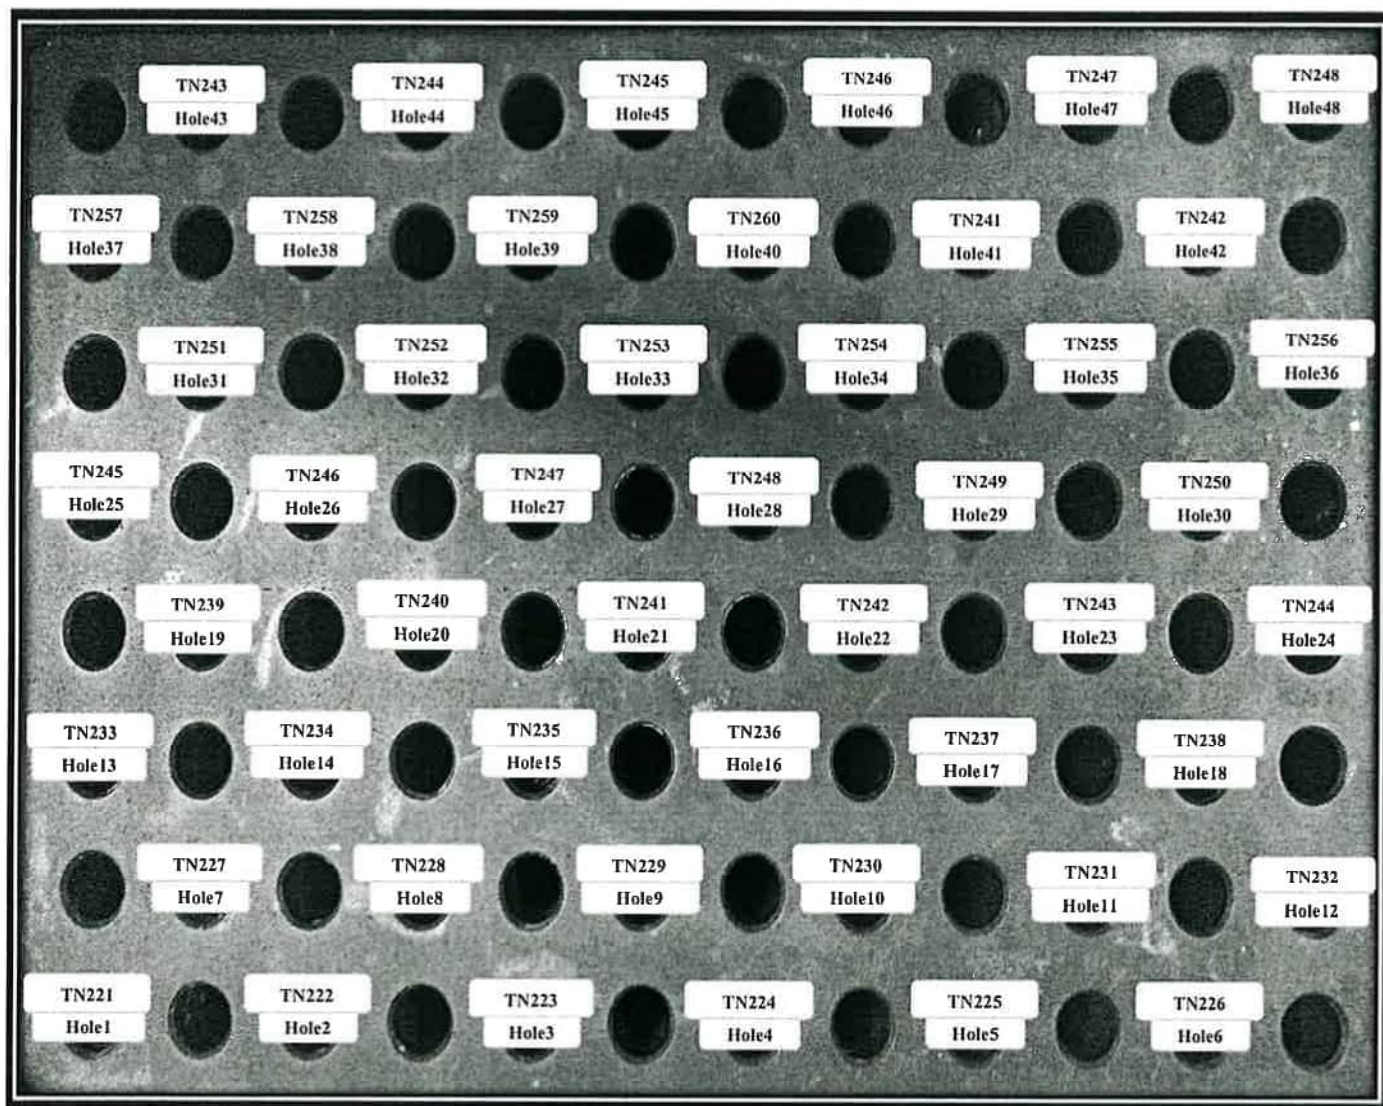

FRONT CONTROL

Approved By. _____

Calibration Report

Measurement Results

Calibration Point		Average Standard Reading at each position (°C)					
R1 Hole1-Hole6		TN221	TN222	TN223	TN224	TN225	TN226
CAL POINT	Max	94.85	95.37	95.03	95.25	95.52	94.75
95	Min	94.17	94.66	94.38	94.63	94.87	94.12
	Average	94.51	95.02	94.70	94.94	95.20	94.43
R2 Hole7-Hole12		TN227	TN228	TN229	TN230	TN231	TN232
	Max	94.71	94.56	94.79	95.32	95.44	95.06
	Min	94.05	93.88	94.10	94.65	94.90	94.65
	Average	94.38	94.22	94.44	94.99	95.17	94.85
R3 Hole13-Hole18		TN233	TN234	TN235	TN236	TN237	TN238
	Max	95.26	95.43	95.40	95.71	95.41	95.06
	Min	94.54	94.64	94.71	95.10	94.86	94.42
	Average	94.90	95.03	95.06	95.41	95.13	94.74
R4 Hole19-Hole24		TN239	TN240	TN241	TN242	TN243	TN244
	Max	95.13	95.06	95.68	96.16	95.35	95.80
	Min	94.39	94.43	94.86	95.51	94.88	95.12
	Average	94.76	94.75	95.27	95.83	95.12	95.46
R5 Hole25-Hole30		TN245	TN246	TN247	TN248	TN249	TN250
	Max	94.95	95.81	95.39	95.82	95.66	95.66
	Min	94.47	95.03	94.67	94.99	94.84	94.87
	Average	94.71	95.42	95.03	95.41	95.25	95.27
R6 Hole31-Hole36		TN251	TN252	TN253	TN254	TN255	TN256
	Max	96.07	95.34	96.28	95.39	94.95	95.12
	Min	95.28	94.55	95.51	94.62	94.13	94.35
	Average	95.67	94.95	95.90	95.00	94.54	94.73
R7 Hole37-Hole42		TN257	TN258	TN259	TN260	TN241	TN242
	Max	95.15	95.63	96.11	95.09	95.34	95.51
	Min	94.38	94.88	95.32	94.28	94.54	94.72
	Average	94.76	95.25	95.71	94.69	94.94	95.11
R8 Hole43-Hole48		TN243	TN244	TN245	TN246	TN247	TN248
	Max	95.84	95.87	95.44	95.72	95.65	95.75
	Min	95.06	95.10	94.60	94.95	94.87	94.98
	Average	95.45	95.48	95.02	95.34	95.26	95.36

Approved By.



Calibration Report

Measurement Results

Calibration Point		Average Standard Reading at each position (°C)					
R1 Hole1-Hole6		TN221	TN222	TN223	TN224	TN225	TN226
CAL POINT	Max	104.48	104.40	104.60	105.27	105.24	105.19
105	Min	104.15	104.02	104.25	104.94	104.91	104.93
	Average	104.32	104.21	104.42	105.10	105.08	105.06
R2 Hole7-Hole12		TN227	TN228	TN229	TN230	TN231	TN232
	Max	105.20	105.45	105.58	105.96	105.81	106.03
	Min	104.92	105.14	105.29	105.64	105.53	105.79
	Average	105.06	105.29	105.43	105.80	105.67	105.91
R3 Hole13-Hole18		TN233	TN234	TN235	TN236	TN237	TN238
	Max	106.09	106.14	105.83	106.25	105.97	105.88
	Min	105.80	105.89	105.57	106.00	105.69	105.65
	Average	105.94	106.01	105.70	106.13	105.83	105.77
R4 Hole19-Hole24		TN239	TN240	TN241	TN242	TN243	TN244
	Max	105.87	105.75	105.30	105.07	105.22	105.66
	Min	105.62	105.52	105.13	104.90	105.05	105.49
	Average	105.74	105.63	105.21	104.98	105.14	105.57
R5 Hole25-Hole30		TN245	TN246	TN247	TN248	TN249	TN250
	Max	105.62	105.54	105.52	105.75	105.97	105.69
	Min	105.45	105.35	105.31	105.57	105.81	105.49
	Average	105.53	105.44	105.41	105.66	105.89	105.59
R6 Hole31-Hole36		TN251	TN252	TN253	TN254	TN255	TN256
	Max	106.19	106.34	106.47	105.96	105.76	105.35
	Min	106.02	106.16	106.31	105.77	105.58	105.18
	Average	106.10	106.25	106.39	105.87	105.67	105.27
R7 Hole37-Hole42		TN257	TN258	TN259	TN260	TN241	TN242
	Max	106.21	105.59	105.45	105.36	106.08	106.09
	Min	106.04	105.42	105.28	105.20	105.90	105.92
	Average	106.12	105.51	105.37	105.28	105.99	106.00
R8 Hole43-Hole48		TN243	TN244	TN245	TN246	TN247	TN248
	Max	106.54	106.33	105.78	105.38	105.42	105.69
	Min	106.38	106.16	105.60	105.20	105.25	105.52
	Average	106.46	106.25	105.69	105.29	105.33	105.61

Approved By.

Calibration Report

Measurement Results:

HEATING BLOCK			Temperature Distribution	
Setting (°C)	Reading (°C)		Stability ($\pm$ °C)	Uncertainty ($\pm$ °C)
	Min , Max	Average		
102.0	-	102.0	0.43	0.83
107.0	-	107.0	0.20	0.70

* The quoted uncertainty exclude " uniformity "

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By. _____





Metrology Center
SCI ECO Services Company Limited

51 Moo 8, Tubkwang, Kaeng Khoi, Saraburi, Thailand 18260

Bangkok Tel : +668 9205 6851 , +669 81924 0059

Saraburi Tel : +669 8247 2360

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th



Certificate No. T250873

Page 1 of 4

Certificate of Calibration

Equipment : Chamber (Cooling Room)

Manufacturer : KOLDTECH

Model : KM 320

Serial No. : TBN-1012061/05

Customer Code : BKK_EN0167

ID No. : T2463A3

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,

Khet Suan Luang, Bangkok 10250

Customer Location : Laboratory Room

Date of Receipt : 28 May 2025

Calibrated By : Atiphong Rongrat (Technician)

Approved By : [Redacted] / Boonchai Suriyawong (Site Calibration Manager)

Date of Issue : 19 JUN 2025

REVIEW BY

APPROVED BY

NEXT CAL DATE..... 04/12/26

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Certificate No. T250873

Page 2 of 4

Calibration Report

Equipment : Chamber (Cooling Room)
Date of Calibration : 4 June 2025
Environment : Temperature : 23.4-24.9 °C
Line Voltage : 221.4-230.2 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert 16 standard thermocouples type T into its chamber , the other one standard thermocouples type T use for ambient temperature measurement . The calibration was done in according to WI-T20 (based on ASTM E145-94 (Reapproved 2001) and AS2853-1986).
All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN91-TN100	T242036	3 December 2025
TC	TYPE T	TN101-TN110	T242036	3 December 2025
DATA LOGGER	34970A	T121	T242036	3 December 2025

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

Equipment Description :

Time Constant 2 Hour 20 Minute At 3 °C
Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
☐ Close
☒ Not Available

5. Adjustment :

(X) without adjustment


() after adjustment

Approved By. 

Certificate No. T250873

Page 3 of 4

Calibration Report

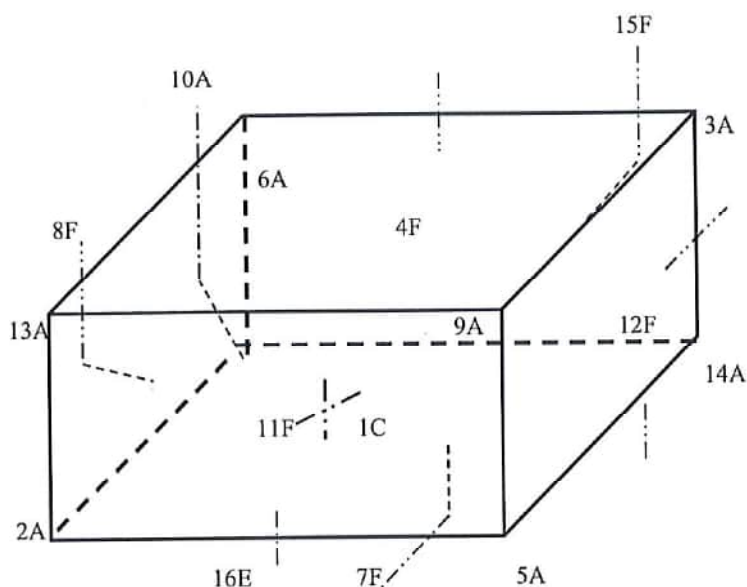

C = Centre , F = Centre of Face , A = Corner , E = Centre of Edge

1C = TN91	12F = TN102
2A = TN92	13A = TN103
3A = TN93	14A = TN104
4F = TN94	15F = TN105
5A = TN95	16E = TN106
6A = TN96	
7F = TN97	
8F = TN98	
9A = TN99	
10A = TN100	
11F = TN101	

Approved By. _____



Certificate No. T250873

Page 4 of 4

Calibration Report

Measurement Results

Calibration Point	Average Standard Reading at each position (°C)											
	TN91	TN92	TN93	TN94	TN95	TN96	TN97	TN98	TN99	TN100	TN101	TN102
3.0	2.95	2.92	3.09	2.92	3.16	3.50	3.40	3.03	3.14	2.98	3.44	3.13
	TN103	TN104	TN105	TN106								
	3.19	3.06	3.46	2.92								

Chamber (Cooling Room)			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (± °C)	Uniformity (°C)	Uncertainty (± °C)	Coverage Factor <i>k</i>
	Min , Max	Average					
3.0	2.8 , 3.9	3.4	3.14	1.20	1.30	1.90	2.04

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By. _____

